




US 20170245874A1

(19) **United States**(12) **Patent Application Publication**
Bailey et al.(10) **Pub. No.: US 2017/0245874 A1**(43) **Pub. Date: Aug. 31, 2017**(54) **BROADLY FOCUSED ULTRASONIC
PROPULSION PROBES, SYSTEMS, AND
METHODS****Publication Classification**(51) **Int. Cl.***A61B 17/22* (2006.01)*A61B 8/08* (2006.01)(52) **U.S. Cl.**CPC *A61B 17/22004* (2013.01); *A61B 8/085*
(2013.01); *A61B 2017/22005* (2013.01)(71) Applicants: **University of Washington**, Seattle, WA
(US); **Sonomotion, Inc.**, Emerald Hills,
CA (US)(72) Inventors: **Michael R. Bailey**, Seattle, WA (US);
Bryan Cunitz, Seattle, WA (US);
Barbrina Dunmire, Seattle, WA (US);
Adam Maxwell, Seattle, WA (US);
Oren Levy, Seattle, WA (US)(73) Assignees: **University of Washington**, Seattle, WA
(US); **Sonomotion, Inc.**, Emerald Hills,
CA (US)(21) Appl. No.: **15/519,821**(22) PCT Filed: **Oct. 19, 2015**(86) PCT No.: **PCT/US15/56261**

§ 371 (c)(1),

(2) Date: **Apr. 17, 2017****Related U.S. Application Data**(60) Provisional application No. 62/065,432, filed on Oct.
17, 2014, provisional application No. 62/160,458,
filed on May 12, 2015.(57) **ABSTRACT**

Disclosed herein are ultrasonic probes and systems incorporating the probes. The probes are configured to produce an ultrasonic therapy exposure that, when applied to a kidney stone, will exert an acoustic radiation force sufficient to produce ultrasonic propulsion. Unlike previous probes configured to produce ultrasonic propulsion, however, the disclosed probes are engineered to produce a relatively large (both wide and long) therapy region effective to produce ultrasonic propulsion. This large therapy region allows the probe to move a plurality of kidney stones (or fragments from lithotripsy) in parallel, thereby providing the user the ability to clear several stones from an area simultaneously. This "broadly focused" probe is, in certain embodiments, combined in a single handheld unit with a typical ultrasound imaging probe to produce real-time imaging. Methods of using the probes and systems to move kidney stones are also provided.

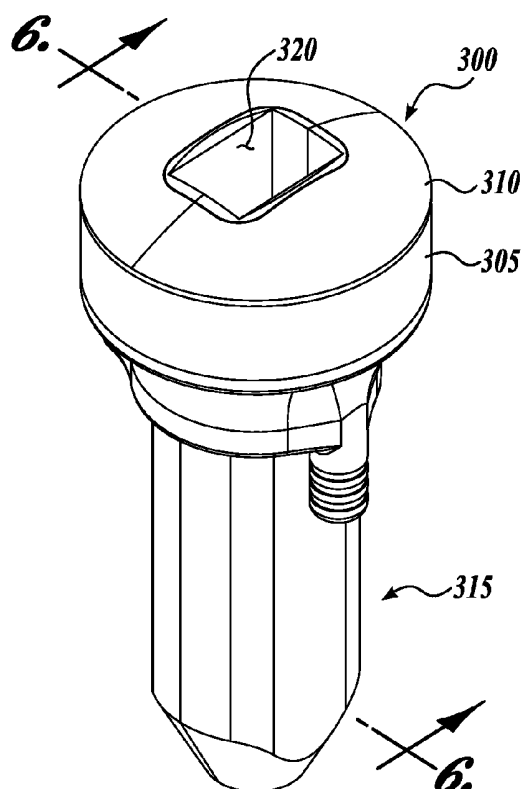

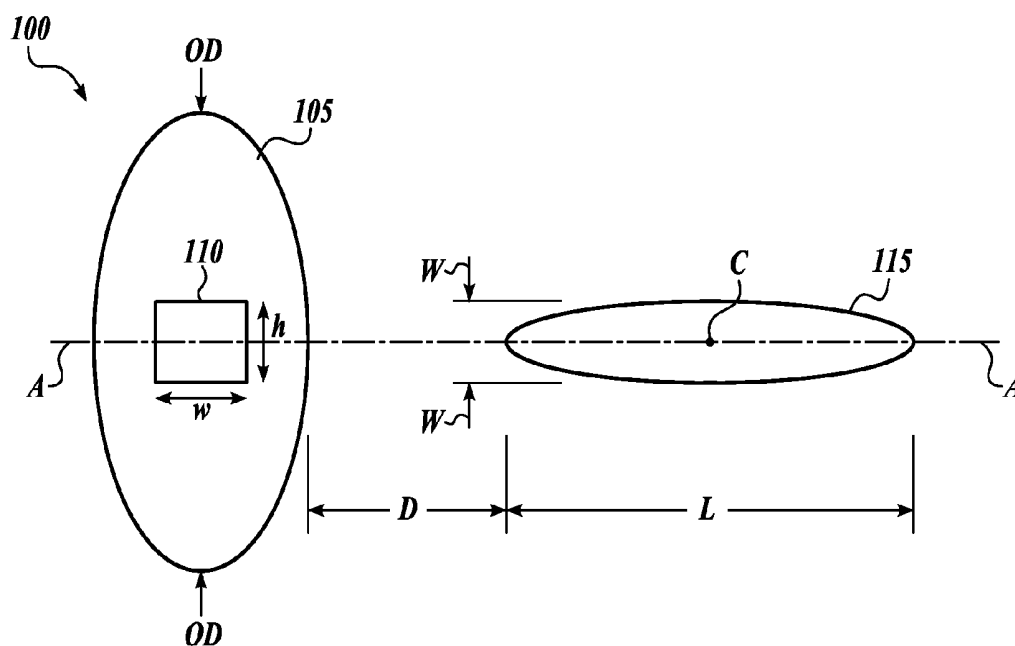


Fig. 1A.

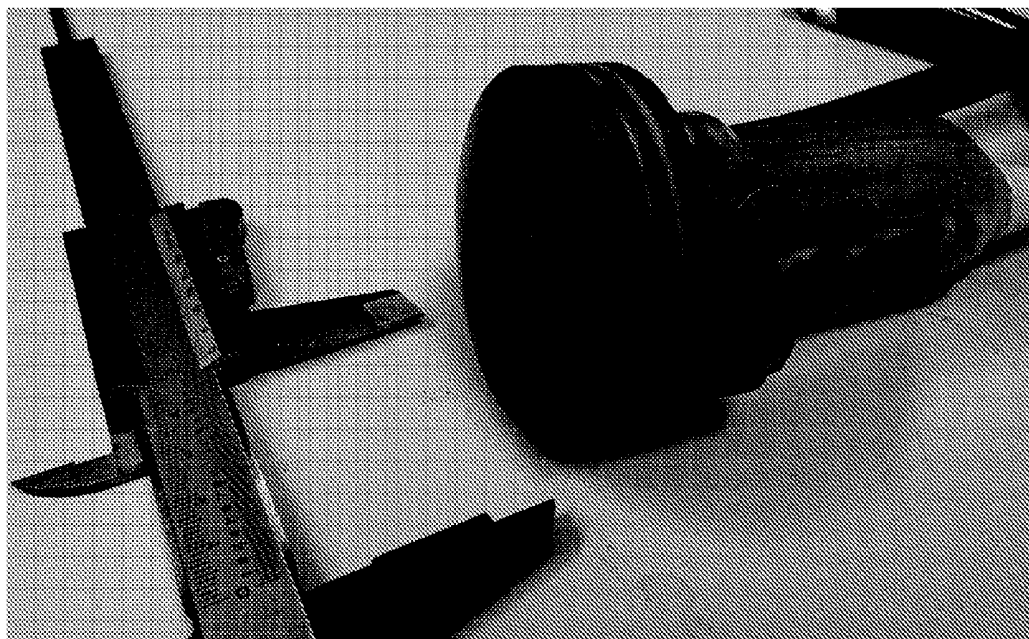


Fig. 1B.

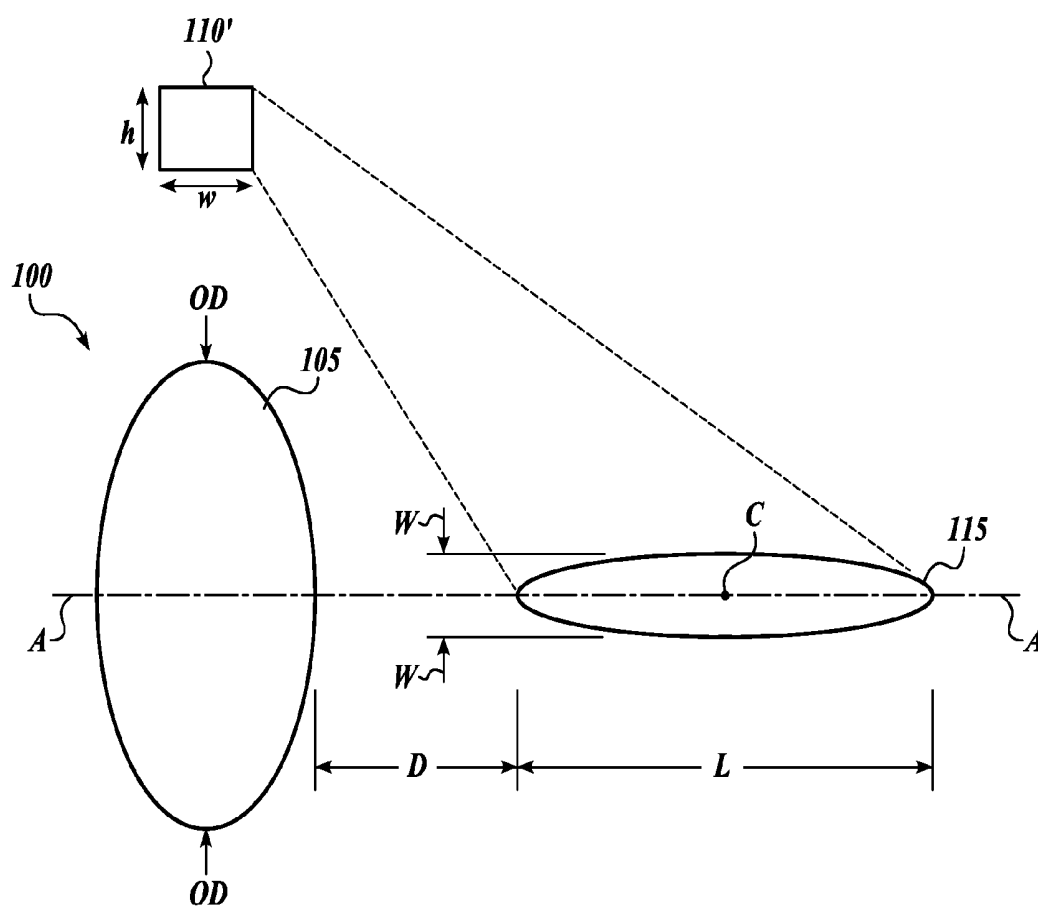


Fig. 1C.

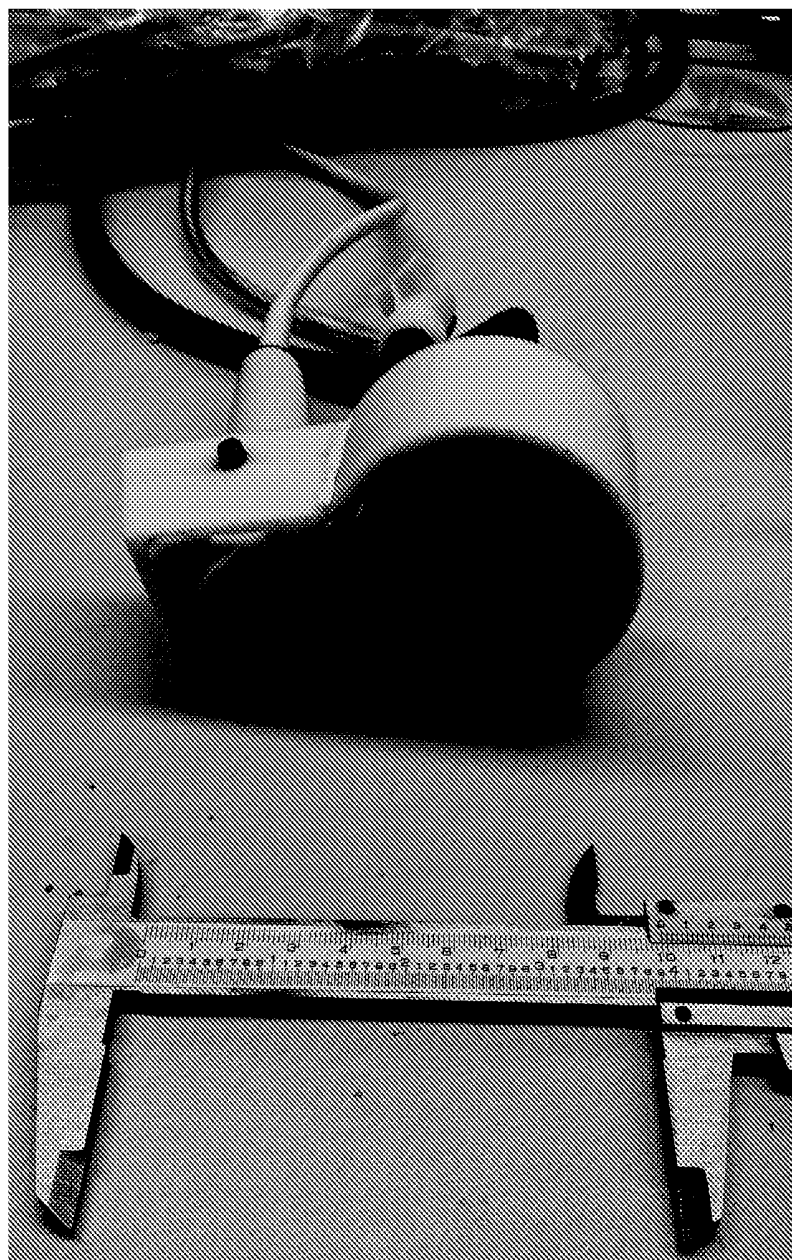


Fig. 1D.

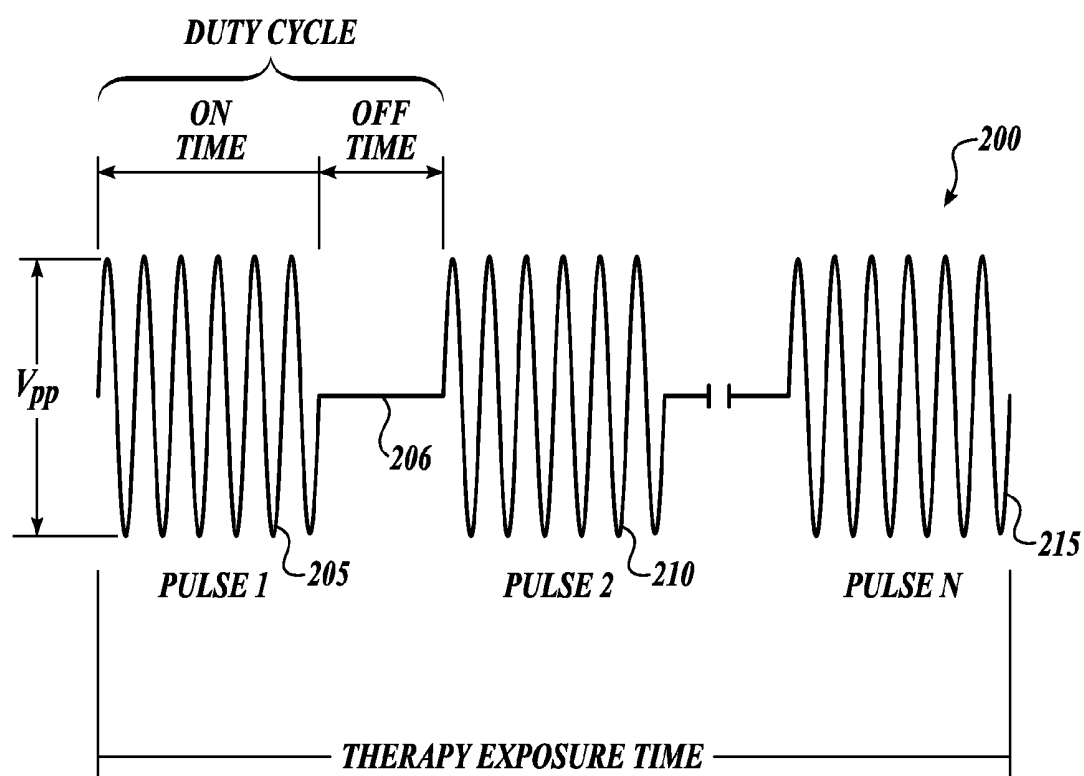


Fig. 2.

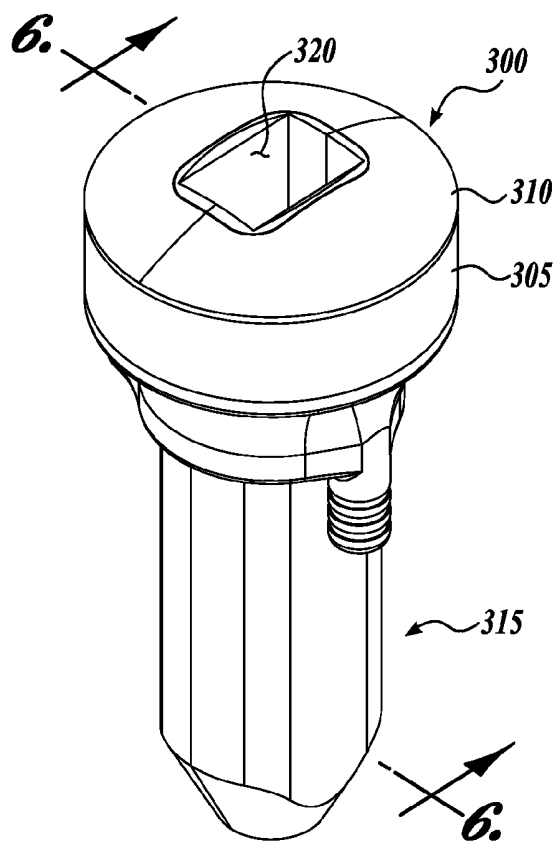


Fig. 3.

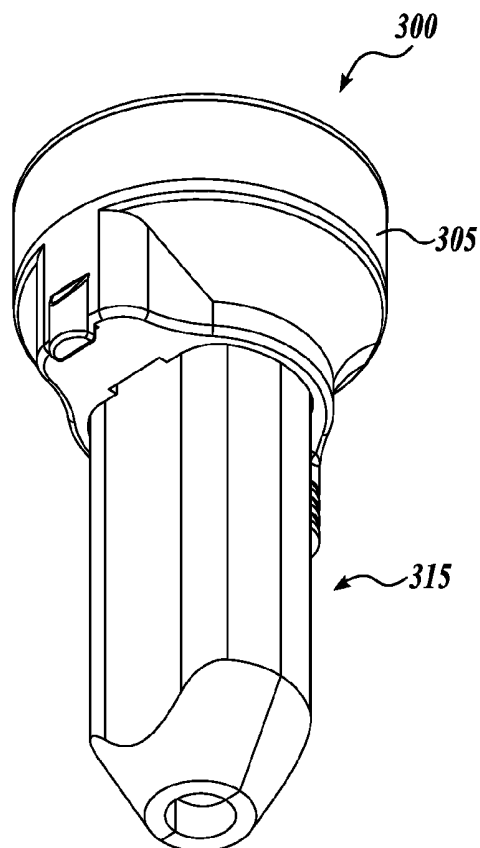
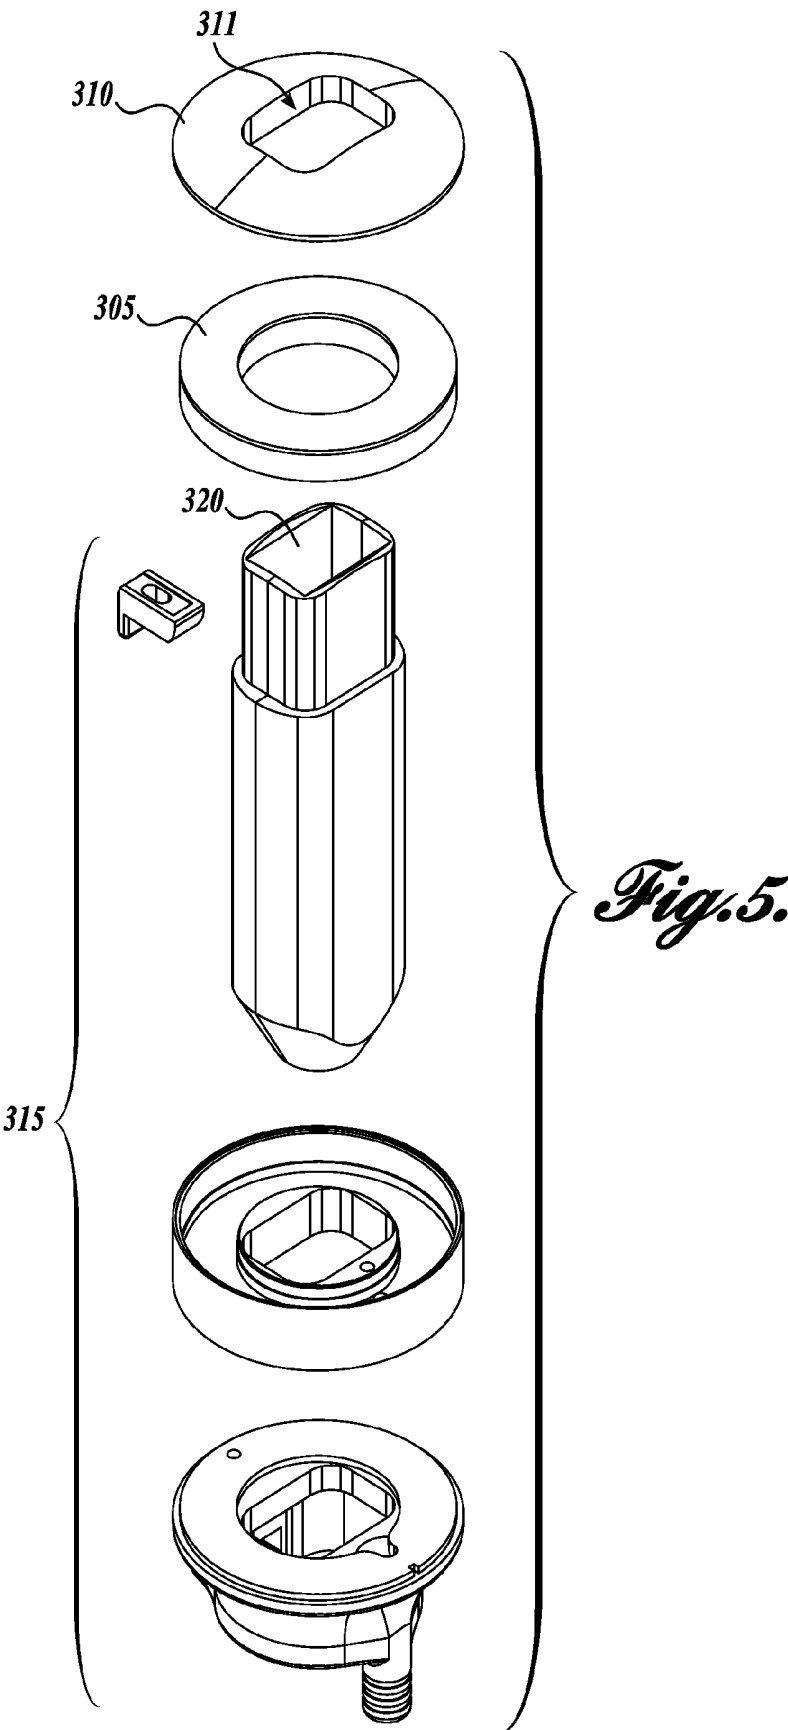


Fig. 4.



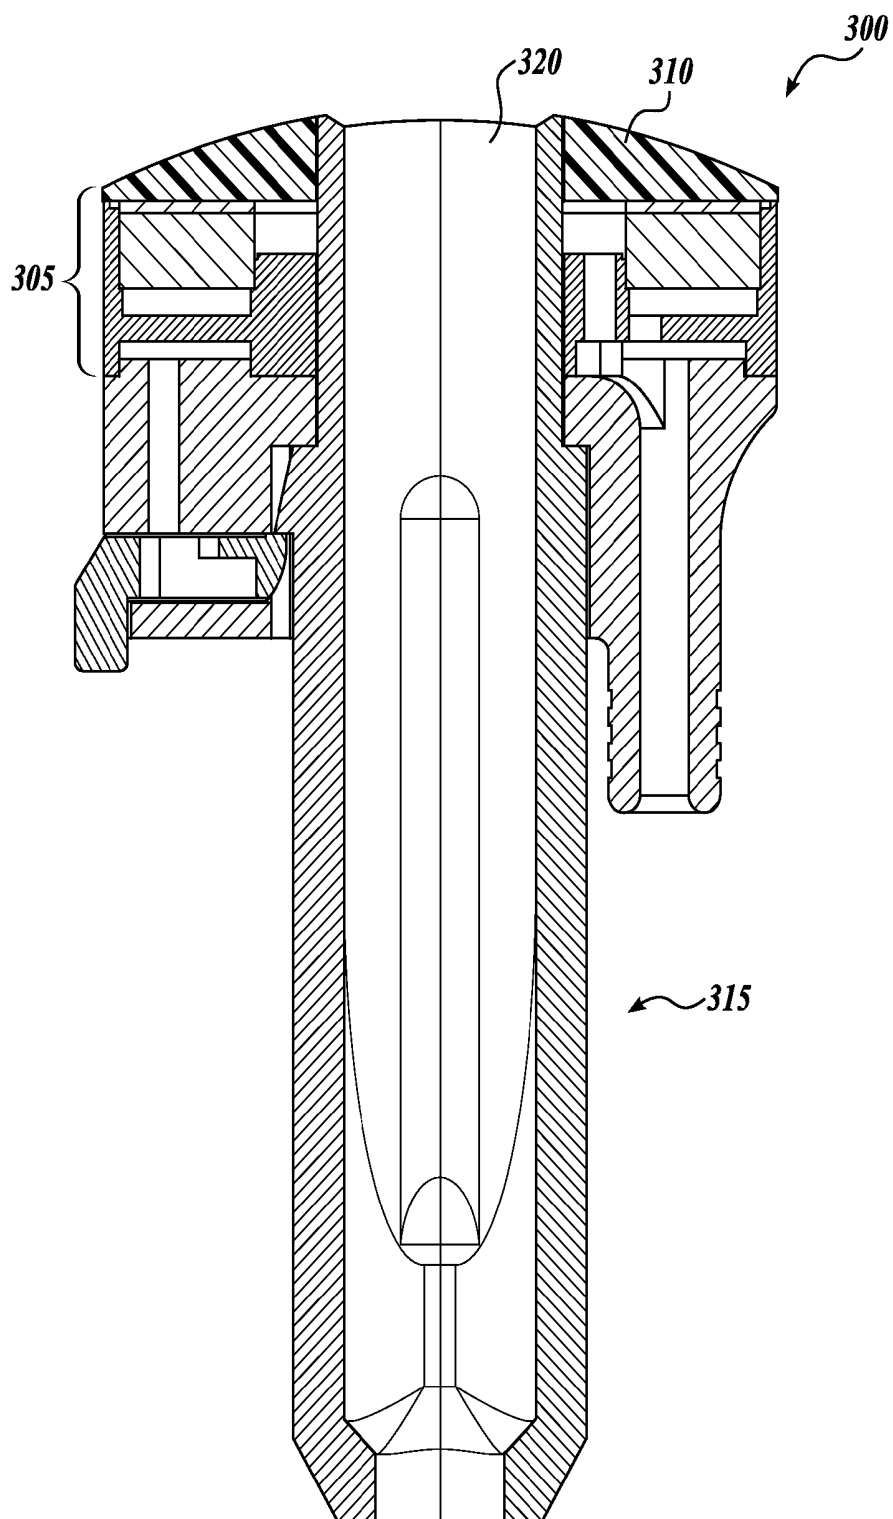


Fig. 6.

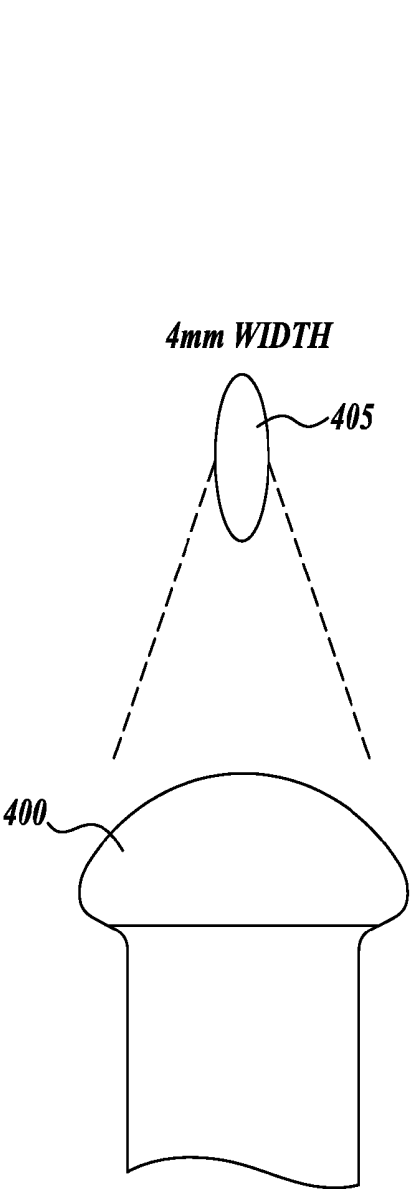


Fig. 7A.
(PRIOR ART)

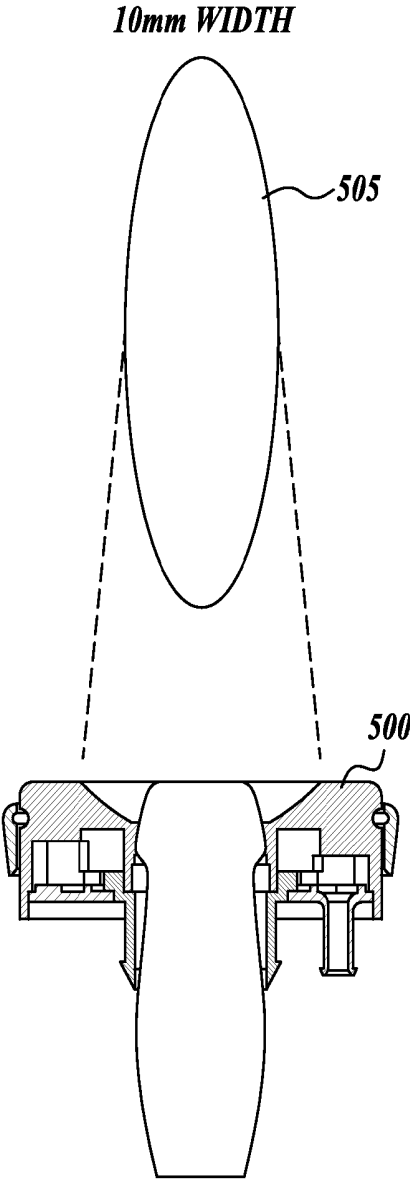


Fig. 7B.

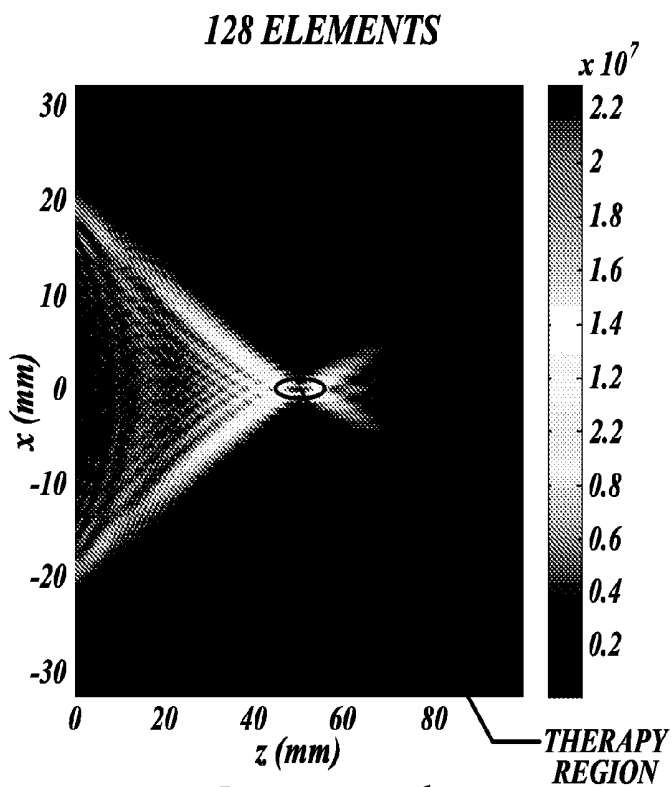


Fig. 8A.

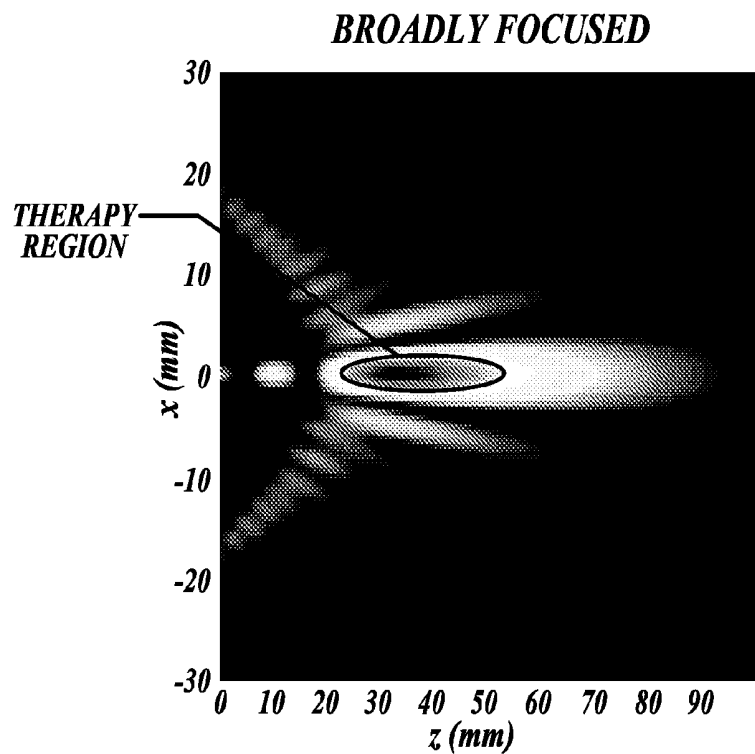


Fig. 8B.

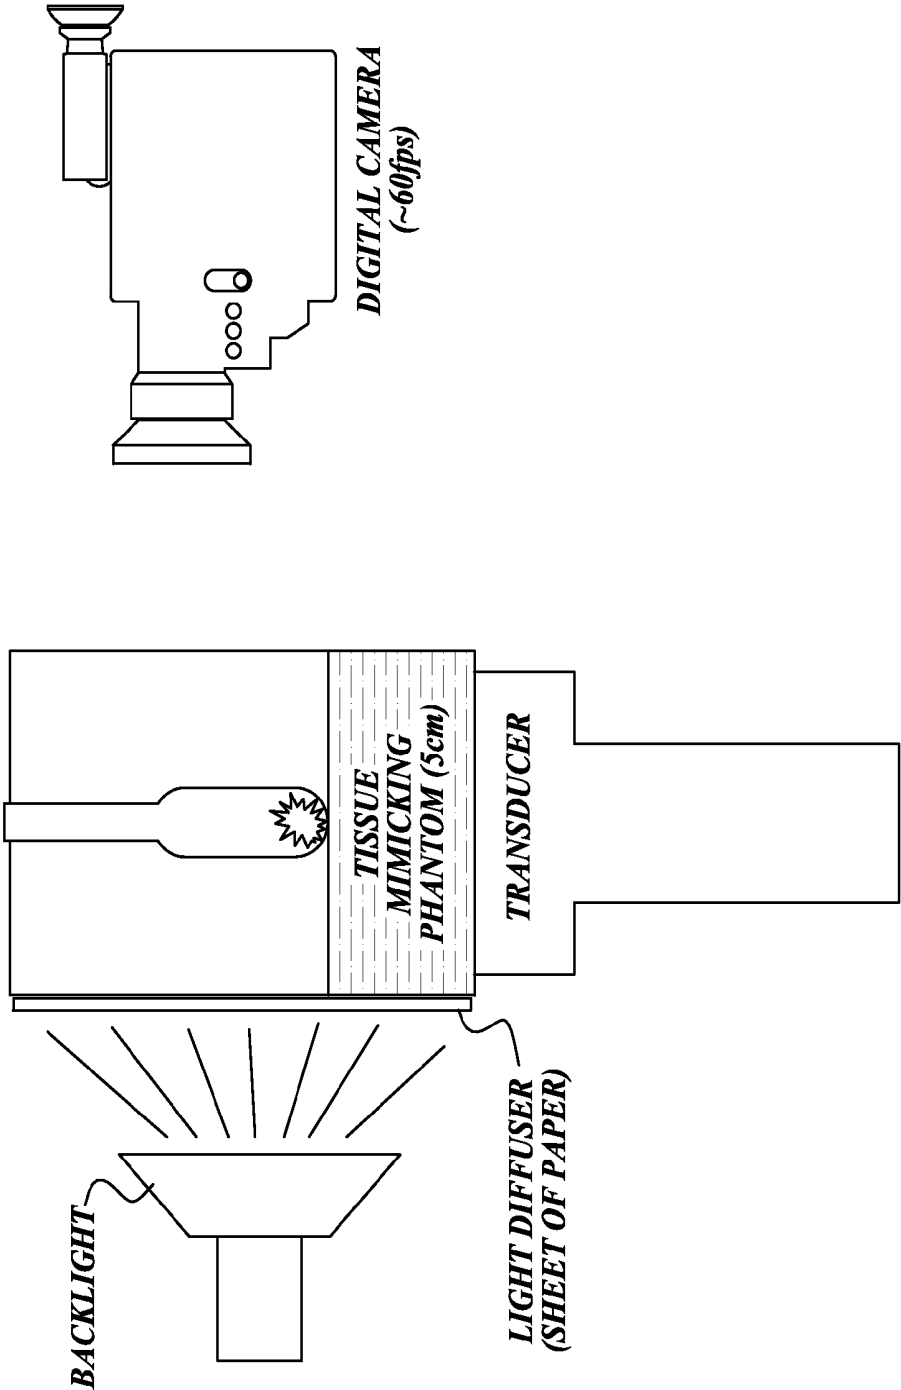


Fig. 9.

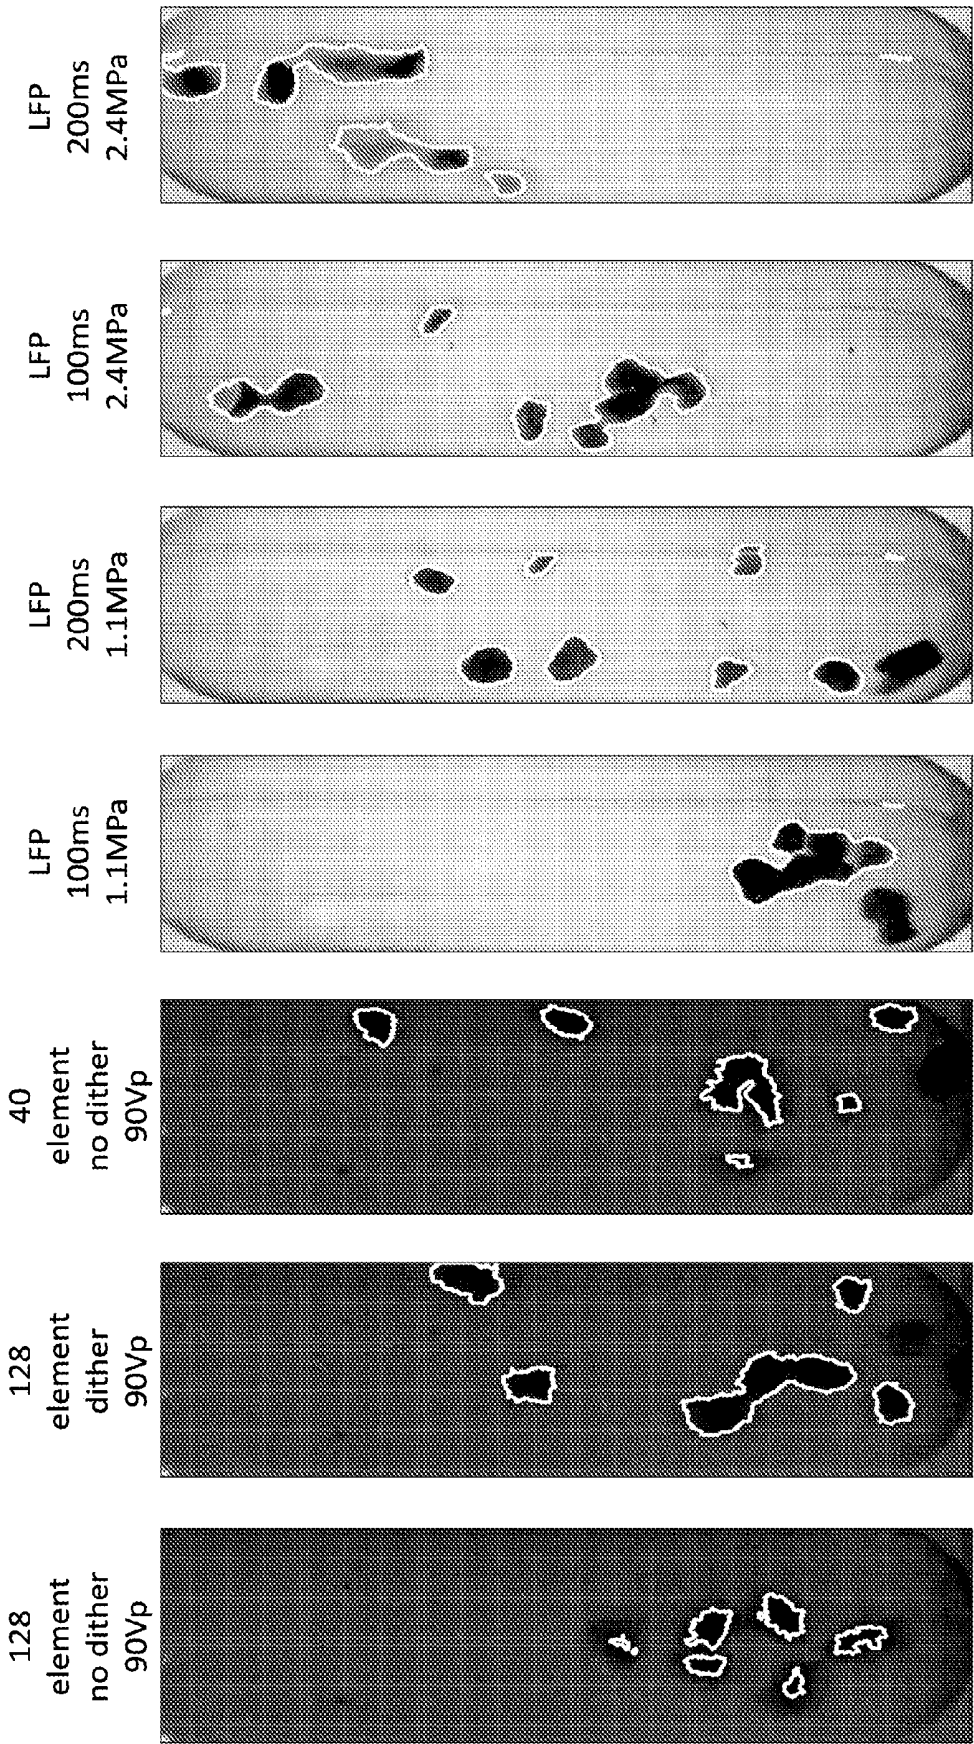


Fig. 10.

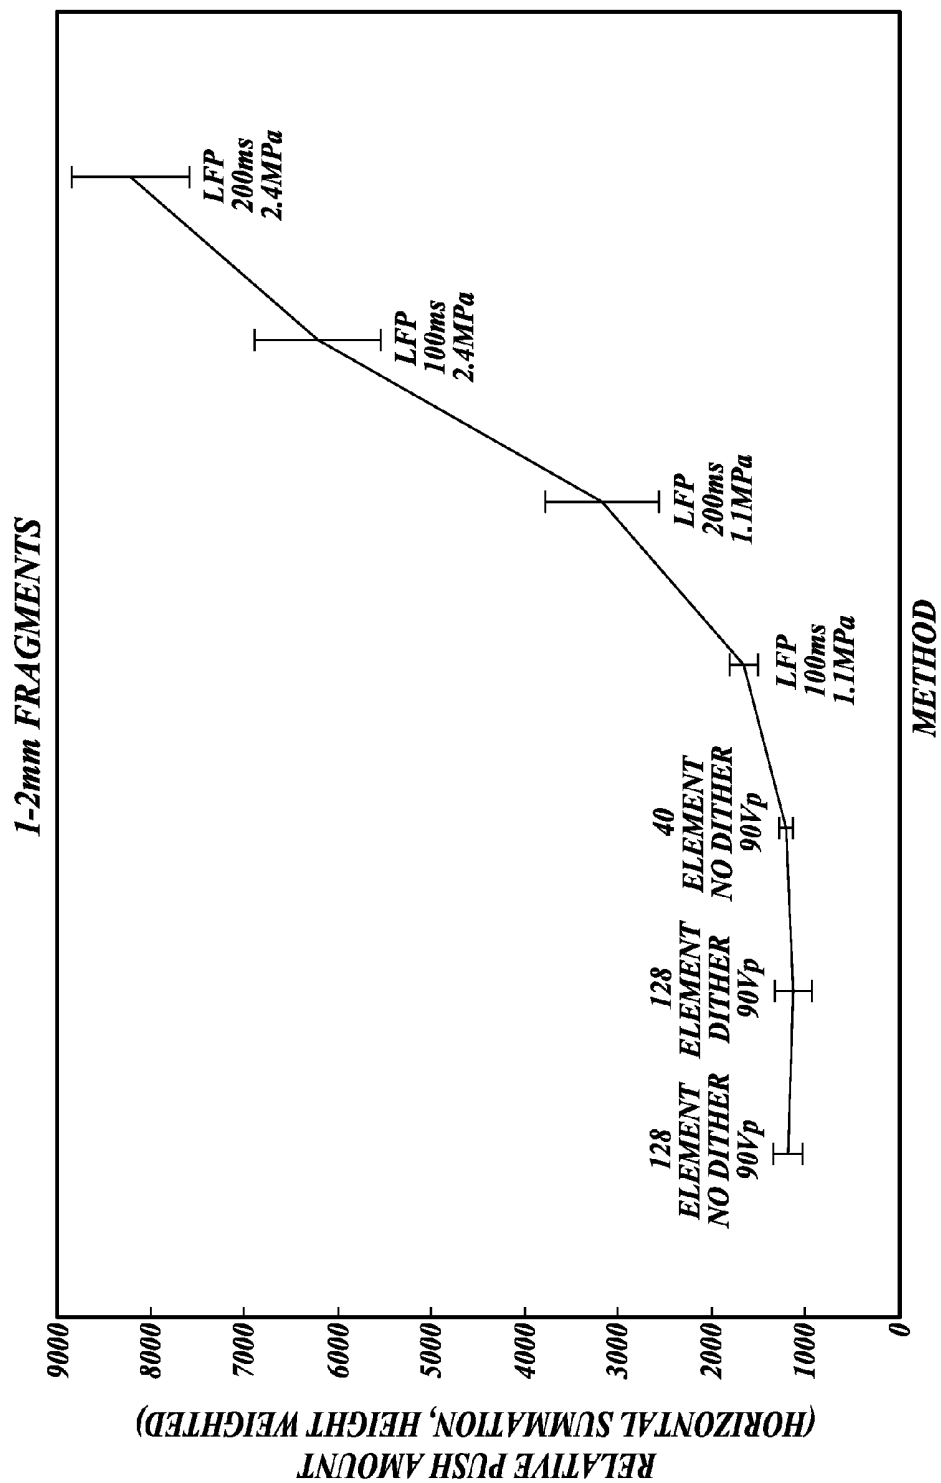


Fig. 11.

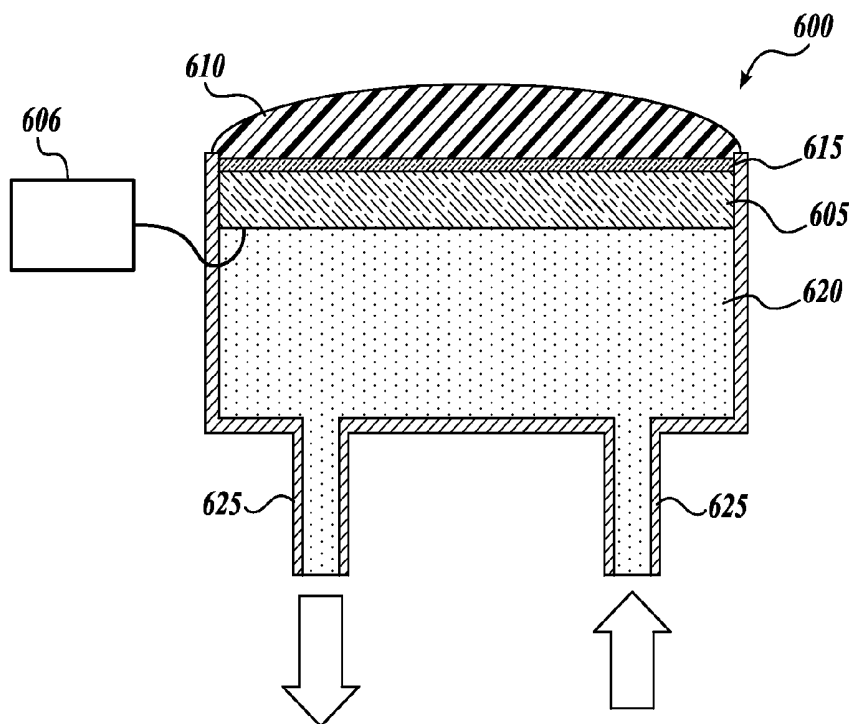


Fig. 12A.

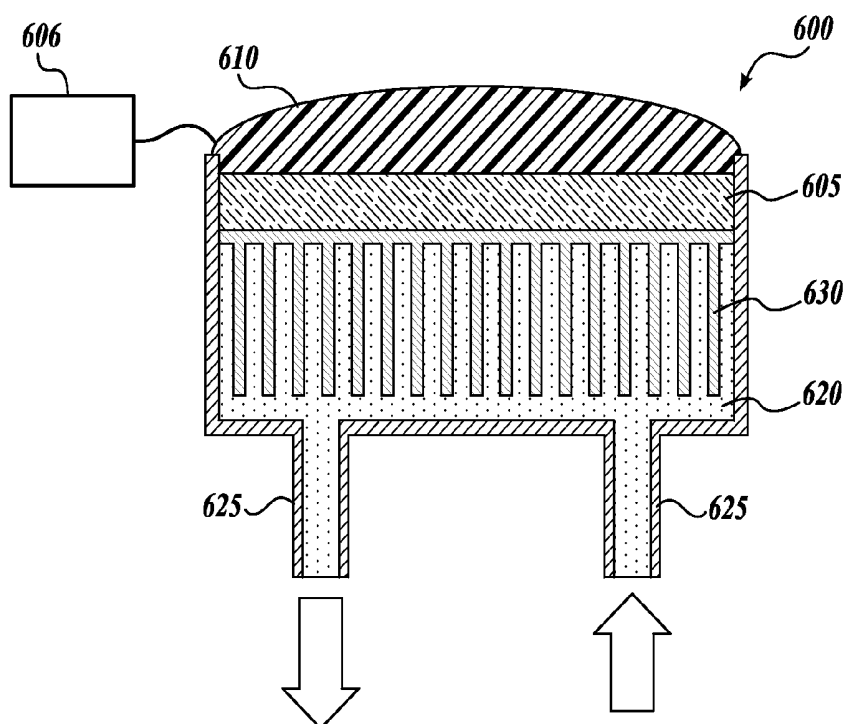


Fig. 12B.

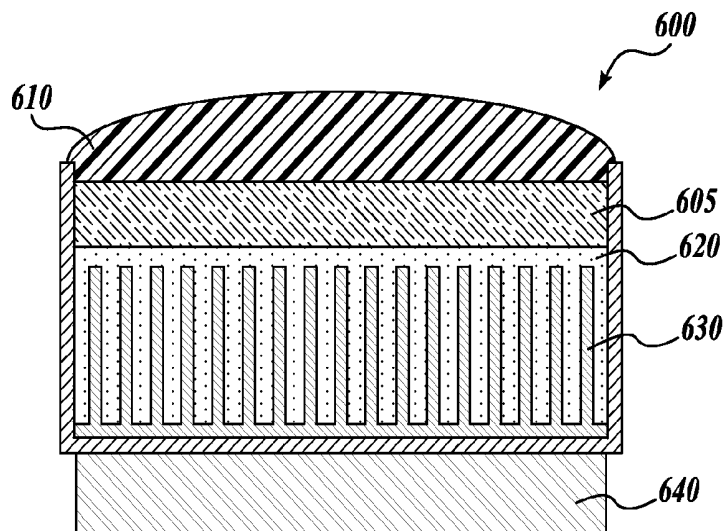


Fig. 12C.

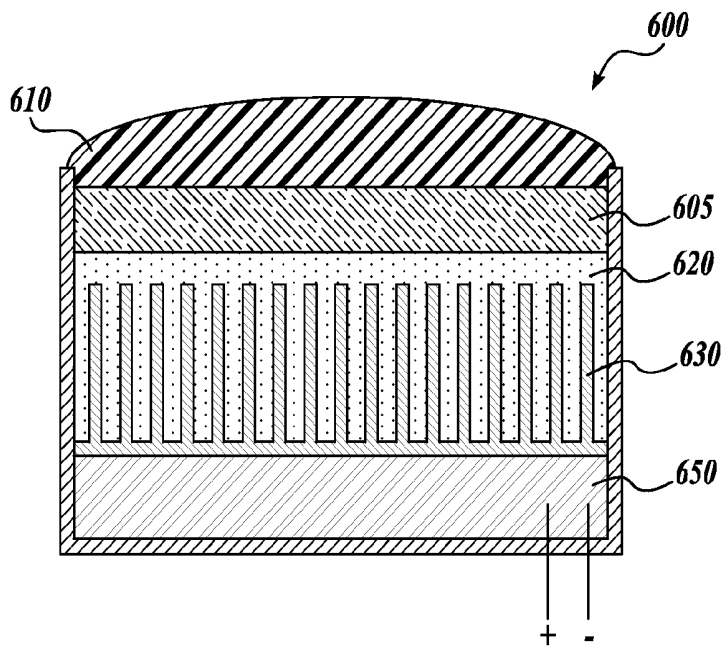


Fig. 12D.

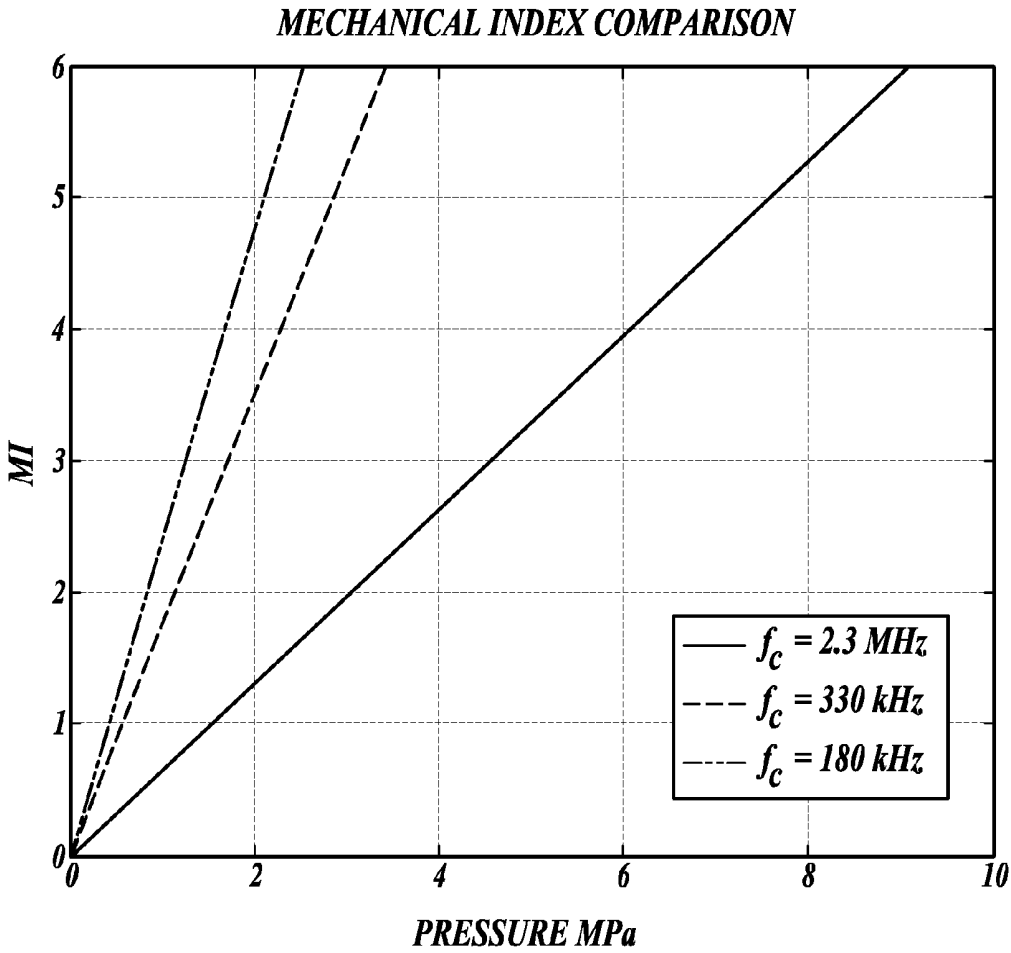


Fig.13.

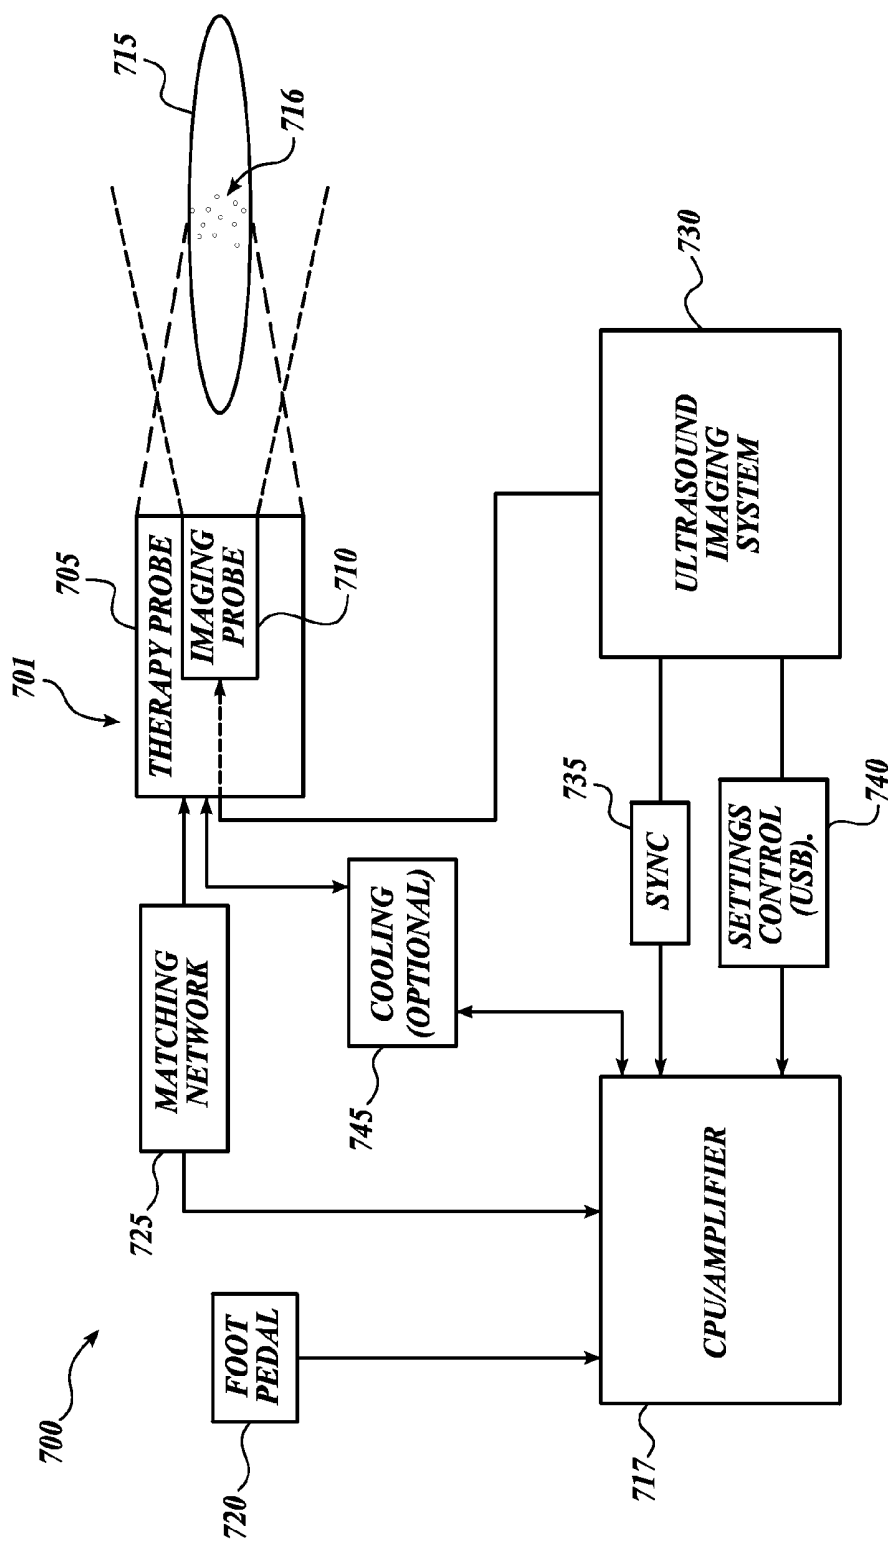


Fig. 14.

BROADLY FOCUSED ULTRASONIC PROPULSION PROBES, SYSTEMS, AND METHODS

CROSS-REFERENCES TO RELATED APPLICATIONS

[0001] This application claims the benefit of U.S. Patent Application No. 62/065,432, filed Oct. 17, 2014, and U.S. Patent Application No. 62/160,458, filed May 12, 2015, the disclosure of each of which are hereby incorporated by reference in its entirety.

STATEMENT OF GOVERNMENT LICENSE RIGHTS

[0002] This invention was made with Government support under R01 DK092197 and P01 DK043881, awarded by the National Institutes of Health National Institute of Diabetes and Digestive and Kidney Diseases; and SMST03402, awarded by the National Space Biomedical Research Institute. The Government has certain rights in the invention.

BACKGROUND

[0003] The disclosed embodiments address the need to safely facilitate the expulsion of kidney stones from an afflicted patient. The National Institute of Diabetes and Digestive and Kidney Diseases (NIDDK) Urinary Stone Disease Research Opportunities and Challenges (USDROC) Workshop website characterizes the problem as follows: "Urinary Stone Disease (USD) is an important health care problem affecting both adults and children, causing pain and suffering for the patient and a financial burden to the Nation. One in 11 Americans now has USD, and the prevalence is increasing. According to the NIDDK-funded study, Urological Diseases in America, the direct medical cost of USD in the United States is \$10 billion annually, making it the most expensive urologic condition." Residual fragments are widely considered to be the overwhelming clinical and research priority in USD, because current treatment options, such as shock wave lithotripsy (SWL) or ureteroscopic lithotripsy (URS), leave behind small residual stone fragments. Studies have shown that while most residual stone fragments will pass, others may grow and in approximately 20% to 40% of patients, lead to symptomatic events such as pain, emergency room visits, or additional procedures. Yet until now no tool or methods exist by which a large number of residual stone fragments can be manipulated (in parallel) within a patient. The primary viable option is presently the serial use of focused ultrasound to manipulate one stone at a time. However, for a large number of small stones this serial method is unfeasible. Accordingly, new tools and method for manipulating a plurality of kidney stones within a patient are desirable.

SUMMARY

[0004] This summary is provided to introduce a selection of concepts in a simplified form that are further described below in the Detailed Description. This summary is not intended to identify key features of the claimed subject matter, nor is it intended to be used as an aid in determining the scope of the claimed subject matter.

[0005] In one aspect, an ultrasonic therapy system configured to apply a non-lithotriptic acoustic radiation force to

a kidney stone is provided. In one embodiment, the ultrasonic therapy system, comprises:

[0006] (a) a therapy probe configured to generate ultrasonic exposure directed towards a therapy region; and

[0007] (b) an imaging probe configured to ultrasonically image the therapy region;

[0008] wherein the therapy probe is configured to produce a therapy exposure comprising one or more therapy pulses over a therapy exposure time, wherein the therapy exposure has the following characteristics:

[0009] (i) a frequency of 100 kHz to 1 MHz;

[0010] (ii) therapy exposure time of at least 10 ms;

[0011] (iii) a peak negative pressure in the therapy region of 0.5 MPa to 5 MPa;

[0012] (iv) the therapy region of one pulse defining a volume subjected to a full-width half-maximum pressure or greater and the therapy region having a length of 2 cm or greater in an axial direction and 2 mm or more in width; and

[0013] (v) the therapy region is sufficient to exert an acoustic radiation force on a kidney stone having a diameter of from 0.5 mm to 20 mm disposed within the therapy region, wherein the acoustic radiation force applied to the kidney stone is from 50 μ N to 0.5 N, and wherein the acoustic radiation force is not sufficient to fragment the kidney stone.

[0014] In another aspect, a method of moving one or more target objects using ultrasonic propulsion is provided. In one embodiment, the method includes applying a non-lithotriptic acoustic radiation force to a target object using an ultrasonic therapy system as shown and described herein.

[0015] In another aspect, a method of moving one or more kidney stones in a therapy region using ultrasonic propulsion is provided. In one embodiment, the method includes using a broadly focused ultrasound therapy probe to apply a force on one or more kidney stones having a diameter of from 0.5 mm to 20 mm disposed within the therapy region, wherein the acoustic radiation force applied to each of the one or more kidney stones is from 50 μ N to 0.5 N, and wherein the acoustic radiation force is not sufficient to fragment the kidney stones.

DESCRIPTION OF THE DRAWINGS

[0016] The foregoing aspects and many of the attendant advantages of this invention will become more readily appreciated as the same become better understood by reference to the following detailed description, when taken in conjunction with the accompanying drawings, wherein:

[0017] FIG. 1A illustrates the relationship between a therapy probe, an imaging probe, and a therapy region of an ultrasonic therapy system in accordance with embodiments disclosed herein;

[0018] FIG. 1B is a photograph of a prototype combination therapy probe (annular) and imaging probe (center) in accordance with embodiments disclosed herein;

[0019] FIG. 1C illustrates another embodiment of a therapy system, wherein the therapy probe and imaging probe are separately arranged but both focused on the therapy region;

[0020] FIG. 1D is a photograph of a prototype combination of a non-axial therapy probe and imaging probe of the type illustrated in FIG. 1C;

[0021] FIG. 2 illustrates an exemplary ultrasonic therapy exposure in accordance with embodiments disclosed herein;

[0022] FIGS. 3-6 illustrate an exemplary therapy probe in accordance with embodiments disclosed herein;

[0023] FIGS. 7A and 7B illustrate the therapy region sizes generated by a prior art probe (FIG. 7A) and a therapy probe in accordance with embodiments disclosed herein (FIG. 7B);

[0024] FIGS. 8A and 8B graphically illustrate simulated therapy region sizes generated by a 128 element prior art probe (FIG. 8A) and a single-element therapy probe in accordance with embodiments disclosed herein (FIG. 8B);

[0025] FIG. 9 schematically illustrates an experimental system for evaluating the efficacy of an ultrasonic probe in pushing one or more artificial kidney stones;

[0026] FIG. 10 is a series of photographs depicting experimental results comparing the ultrasonic pushing force of prior art and exemplary ultrasonic transducers;

[0027] FIG. 11 graphically illustrates data collected from 10 iterations of the experiment illustrated in FIGS. 9 and 10 to determine the relative push strength of prior art and exemplary ultrasonic transducers;

[0028] FIGS. 12A-12D schematically illustrate various embodiments of representative therapy probes having cooling systems incorporated therein in accordance with embodiments disclosed herein;

[0029] FIG. 13 graphically illustrates the correlation between mechanical index (MI), pressure, and frequency of an ultrasound system; and

[0030] FIG. 14 is a block diagram depicting the components of a representative ultrasonic therapy system in accordance with embodiments disclosed herein.

DETAILED DESCRIPTION

[0031] Disclosed herein are ultrasonic therapy probes and systems incorporating the probes. The probes are configured to produce an ultrasonic therapy exposure that, when applied to a kidney stone, will exert an acoustic radiation force sufficient to produce ultrasonic propulsion. Unlike previous probes configured to produce ultrasonic propulsion, however, the disclosed probes are engineered to produce a relatively large (both wide and long) therapy region effective to produce ultrasonic propulsion. This large therapy region allows the probe to move a plurality of kidney stones (or fragments from lithotripsy) in parallel, thereby providing the user the ability to clear several stones from an area simultaneously. This “broadly focused” probe is, in certain embodiments, combined in a single handheld unit with a typical ultrasound imaging probe. By coordinating the ultrasound signals produced by both the therapy probe and the imaging probe a user of the combined probe can image stones in real time as the broadly focused ultrasound moves stones within a patient. Methods of using the probes and systems to move kidney stones are also provided.

[0032] Advantages of the disclosed broadly focused beam include easier alignment. The wide beam yields a greater probability of targeting a stone. The relatively long therapy region accounts for the difficulty in changing focal depth during use, therefore simplifying targeting. Furthermore, the disclosed system allows for simpler cheaper systems, particularly in embodiments that utilize a single therapy transducer (“fixed focus”). Finally, the disclosed embodiments, during treatment, yield no “hot spots” of high amplitude (>-6 dB compared to focal pressure), making the devices and methods safer and more predictable when applied to patients.

[0033] In one aspect, an ultrasonic therapy system configured to apply a non-lithotriptic acoustic radiation force to a kidney stone is provided. In one embodiment, the ultrasonic therapy system, comprises:

[0034] (a) a therapy probe configured to generate ultrasonic exposure directed towards a therapy region; and

[0035] (b) an imaging probe configured to ultrasonically image the therapy region;

[0036] wherein the therapy probe is configured to produce a therapy exposure comprising one or more therapy pulses over a therapy exposure time, wherein the therapy exposure has the following characteristics:

[0037] (i) a frequency of 100 kHz to 1 MHz;

[0038] (ii) therapy exposure time of at least 10 ms;

[0039] (iii) a peak negative pressure in the therapy region of 0.5 MPa to 5 MPa;

[0040] (iv) the therapy region of one pulse defining a volume subjected to a full-width half-maximum pressure or greater and the therapy region having a length of 2 cm or greater in an axial direction and 2 mm or more in width; and

[0041] (v) the therapy region is sufficient to exert an acoustic radiation force on a kidney stone having a diameter of from 0.5 mm to 20 mm disposed within the therapy region, wherein the acoustic radiation force applied to the kidney stone is from 50 μ N to 0.5 N, and wherein the acoustic radiation force is not sufficient to fragment the kidney stone.

[0042] The ultrasonic system may be better understood by referencing the diagrammatic illustration of FIG. 1A, which illustrates a combined probe 100 including both a therapy probe 105 and an imaging probe 110. Disposed along axis A of both probes 105 and 110 is the therapy region 115.

[0043] The therapy region 115 is defined herein as the volume of space (e.g., within a patient) subjected to a full-width half-maximum (FWHM) pressure or greater. In this regard, the therapy probe 105 will produce a maximum pressure at a certain point in the therapy region 115 and the boundaries of the therapy region 115 are defined by the region wherein the pressure is FWHM in view of the maximum pressure. The therapy region 115 has a center point C, a length L, and a width W, and begins a distance D from the therapy probe 105. As used herein, the therapy region “width” is defined as the distance between the locations in the field orthogonal to the acoustic axis A where the pressure reaches -6 dB relative to the peak focal pressure.

[0044] The therapy probe 115 is annular (at least roughly circular) as depicted in FIG. 1A, having an outside dimension OD. The therapy probe 115 is circular in one embodiment. The imaging probe 110 is typically rectangular, having a height h and width w. The sizes of the combined probe 100 and, relatedly, the therapy probe 105 and imaging probe 110, are of great importance. The combined probe 100 must be compact (e.g., OD of 5 cm or less) in order to be easily handheld by an operator and to be maneuverable to position at any point along a patient’s skin. These dimensional constraints lead to the coaxial combination of the probes 105 and 110 to form the compact combined probe 100. An exemplary combined probe 100 is pictured in FIG. 1B.

[0045] In an embodiment of the system distinct from that of FIGS. 1A and 1B, FIG. 1C illustrates a system without an integrated imaging probe 110. Instead, a separately disposed imaging probe 110' is utilized. The imaging probe 110' is still coordinated with the therapy probe 105 during use and is

still focused on the therapy region 115. However, the imaging probe 110' is not coaxially disposed on axis A. This arrangement does not provide the benefits of ease of use when coaxially focusing on the therapy region 115, although this embodiment may be more easily fabricated from off-the-shelf components because a custom coaxial probe (e.g., combined probe 100) need not be fabricated.

[0046] During operation, the therapy probe 105 emits a therapy exposure comprising one or more ultrasonic therapy pulses over a therapy exposure time (refer to FIG. 2 for a visual illustration of the therapy exposure signal). If imaging is utilized, the therapy probe 105 and imaging probe 110 are coordinated such that their signals do not overlap yet images are acquired frequently enough (e.g., at least one frame per second, fps). By acquiring images of the therapy region 115 during a therapy exposure, the operator can see the movement of stones in real time and adjust aim and/or focus as needed to accomplish the treatment (e.g., move the stones towards expulsion from the kidney or other region).

[0047] The term "therapy exposure" relates herein to a series of pulses over an exposure time. The exposure time is defined in certain embodiments by a user activating the therapy probe by an on switch or other mechanism. An exemplary mechanism is on on/off switch, such as a foot-activated switch. Several therapy exposures may be utilized by a user during treatment of a patient for a cumulative therapy exposure session. Therapy exposures end when the system is continuously off for a prolonged period (e.g., 1 second or greater). An "off" period between pulses (i.e., when the duty cycle is less than 100%) does not mark the end of a therapy exposure.

[0048] The ultrasonic therapy system is non-lithotriptic and therefore the ultrasound applied by the system is not sufficient to break a kidney stone. The purpose of the system is to provide a relatively large therapy region in which the therapy probe produces sufficient acoustic radiation force to move any kidney stones within the therapy region. While the description herein discusses the unusual utility of the systems in moving a plurality of stones or fragments, it will be appreciated that the movement of a single stone, even a single large stone is also contemplated in certain embodiments. As an example, a single large stone may be moved that is blocking the ureter.

[0049] The therapy exposure is an ultrasonic signal as depicted in FIG. 2. It can be defined by a number of parameters, including frequency, therapy exposure time, the peak negative pressure in the therapy region, power, intensity, and driving voltage.

[0050] The therapy region is sufficient to exert an acoustic radiation force on a kidney stone having a diameter of from 0.5 mm to 20 mm disposed within the therapy region, wherein the acoustic radiation force applied to the kidney stone is from 50 μ N to 0.5 N, and wherein the acoustic radiation force is not sufficient to fragment the kidney stone. This characteristic of the system and therapy region indicates the nature of the force exerted by the therapy probe: non-lithotriptic and "pushing" using an acoustic radiation force. The acoustic radiation force can be measured experimentally in vitro (e.g., on the bench) using an acoustic radiation force balance or load cell, a radiation force radiometer, or any other technique known to those of skill in the art.

[0051] The combined probe 100 has a handheld form factor for ease of clinical use. An exemplary combined probe

100 is pictured in FIG. 1B and FIGS. 3-6 are line drawings depicting the housing and therapy probe. Referring now to FIGS. 3-6, the housing 300 includes a therapy probe transducer 305 a lens 310, an elongate handle 315, and a housing 320 configured to hold an imaging probe, which fits through the lens 310 and therapy transducer 305 via an aperture 311 in each. FIG. 6 is a cross-sectional view of the housing 300.

[0052] In the exemplary embodiments the therapy probe transducer 305 is a custom PZT transducer and the imaging probe is a commercial imaging probe. However, it will be appreciated that in other embodiments both probes are custom made or both are commercially available.

[0053] FIGS. 7A and 7B compare the relative therapy region sizes of a commercial therapy probe (FIG. 7A) compared to the broadly focused therapy probe disclosed herein (FIG. 7B). The size of the therapy region can be an order of magnitude larger, which allows for a broader push on a plurality of stones or fragments.

[0054] It should be noted that while the disclosed embodiments are described in the context of moving kidney stones (or fragments thereof) using broadly focused ultrasound, the concepts disclosed herein can also be used to move other embedded objects, including, but not limited to, stones, fragments, blood clots, bullets, mucous, cystic fibrosis mucous, flowing blood, impacted stool in constipation, rectal, urethral and bladder foreign bodies, ureteral stones, bladder stones, airway foreign bodies, nasal congestion, sinus obstruction, impacted cerumen (ear wax), tissue flaps (like a torn retina), or floating objects in the eye and dust located in any of the gall bladder, the salivary tract, biliary tract or any other anatomical location, of a human or other mammal. An additional use for the disclosed embodiments is to become a part of the maintenance program of implanted foreign bodies to prevent encrustation or occlusion over time. For example, ureteral stents become encrusted from urine solutes precipitating over time on the surface of the stent. The stent could receive intermittent pushing every 3 weeks to "disrupt" or slow the encrustation process. A similar embodiment could be envisioned for cardiac stents."

[0055] As used herein, the term "about" indicates that the subject value can be modified by plus or minus 5% and still fall within the disclosed embodiment. Additionally, stated values are in situ. Relatedly, the term "derated" used herein means measured in the water tank and extrapolated to values in situ. Equations for producing derated ultrasonic values are known to those of skill in the art. For example, the equation X (derated pressure in MPa) = $0.03 \text{ db/cm/MHz} \times \text{depth of tissue penetration (cm)} \times \text{MHz center frequency of pulse} \times \text{initial amplitude of the focal pressure measured in water (MPa)} \times N_p / 8.7 \text{ db (Np=neper)}$.

[0056] Specific aspects of the ultrasonic therapy system and methods will now be described in further detail.

[0057] Therapy Probe Characteristics

[0058] The therapy probe is an ultrasonic transducer. Ultrasonic transducers are generally known in the art and are formed from piezoelectric materials, such as lead zirconate titanate (PZT).

[0059] In one embodiment, the pulses have a duration of 1 ms to 350 ms. In a further embodiment, the pulses have a duration of 10 ms to 200 ms. In yet a further embodiment, the pulses have a duration of 50 ms to 200 ms. An exemplary embodiment utilizes 25 ms pulse durations.

[0060] 350 ms is an upper pulse duration limit due to the desire to coordinate the therapy probe with the imaging

probe. The imaging probe should not be receiving signals to make an image when the therapy probe is transmitting, and so a therapy pulse must be turned “off” in order to make time for an imaging pulse. This relationship may be better understood with reference to FIG. 2, which illustrates a therapy exposure 200 comprising a number of pulses 205, 210, 215. Each pulse 205 et al. has an on time which is followed by an off time 206 in which the imaging probe can operate to produce at least two frames per second. This frame rate, while low, still allows an operator to track kidney stones exposed to the therapy exposure sufficiently.

[0061] In an alternative embodiment, imaging is not used during therapy exposure. However, imaging the therapy region provides significant benefits to use.

[0062] The total time over which the therapy probe operates is referred to as the “therapy exposure time.” The duty cycle is defined as the percentage of on time compared to total on time and off time before a new pulse begins.

[0063] Due to the low frequency and power of the therapy probe, a 100% duty cycle is possible, although imaging in such a situation must be accomplished in a manner that does not interfere with the therapy probe. Accordingly, in one embodiment the therapy exposure is a single continuous pulse.

[0064] Average power is another characteristic useful for defining the therapy probe and the therapy exposure. Average power is defined as the total power emitted over the active area of the probe averaged over the duration of the therapy exposure. In one embodiment, the therapy probe is configured to produce an average power of 5 W to 200 W for 1 second to 10 min. In one embodiment, the therapy probe is configured to produce an average power of 10 W to 200 W for 1 second to 10 min. In one embodiment, the therapy probe is configured to produce an average power of 15 W to 60 W for 1 second to 10 min.

[0065] In one embodiment, the therapy region is defined by a single therapy pulse. The definitions described herein of beam width are for exposure to one focus. This is in contrast to a system that uses a sequence of pulses focused on different points to broaden the total exposed width. The width used herein is the width of a beam at a snapshot in time. It is not the width constructed by a succession of pulses.

[0066] In one embodiment, the therapy region has a length of 2 cm to 15 cm. In one embodiment, the therapy region has a length of 4 cm to 10 cm. In one embodiment, the therapy region has a length of 3 cm or greater. In one embodiment, the therapy region has a length of 5 cm or greater. In one embodiment, the therapy region has a length of 15 cm or less.

[0067] In one embodiment, the therapy region has a width of 2 mm to 20 mm. In one embodiment, the therapy region has a width of 1 mm to 10 mm. In one embodiment, the therapy region has a width of 5 mm to 8 mm. In one embodiment, the therapy region has a width of greater than 3 mm. In one embodiment, the therapy region has a width of greater than 5 mm. In one embodiment, the therapy region has a width of less than 10 mm. In one embodiment, the therapy region has a width of less than 20 mm.

[0068] In one embodiment, the therapy region has a width of at least 1 mm and a length of at least 2 cm; In one embodiment, the therapy region has a width of at least 2 mm

and a length of at least 1 cm. In one embodiment, the therapy region has a width of at least 1 mm and a length of at least 1 cm.

[0069] In one embodiment, the frequency is 200 kHz to 500 kHz. In one embodiment, the frequency is 300 kHz to 450 kHz.

[0070] In one embodiment, the peak negative pressure in the therapy region is 1.0 MPa to 4.0 MPa. In one embodiment, the peak negative pressure in the therapy region is 1.5 MPa to 3.5 MPa.

[0071] In one embodiment, the therapy region begins at least 1 cm from the therapy probe. In one embodiment, the therapy region begins at least 3 cm from the therapy probe. In one embodiment, the therapy region begins at least 5 cm from the therapy probe.

[0072] In one embodiment, the therapy exposure is at least 1 second long. In one embodiment, the therapy exposure is at least 10 seconds long. In one embodiment, the therapy exposure is at least 30 seconds long. In one embodiment, the therapy exposure is at least 60 seconds long. In one embodiment, the therapy exposure is at least 5 minutes long. In one embodiment, the therapy exposure is at least 10 minutes long.

[0073] In one embodiment, the therapy exposure comprises a therapy burst that comprises a plurality of pulses separated by off periods. This configuration is illustrated in FIG. 2.

[0074] In one embodiment, the therapy burst has a duty cycle of greater than 30%. In one embodiment, the therapy burst has a duty cycle of greater than 50%. In one embodiment, the therapy burst has a duty cycle of greater than 75%.

[0075] The disclosed system operates within defined ranges of mechanical index. Mechanical index is defined herein as peak negative pressure (MPa)/square root of frequency (in MHz). FIG. 13 graphically illustrates the correlation between mechanical index (MI), pressure, and frequency of an ultrasound system. In one embodiment, the mechanical index is 10 or below, which is the upper limit before stone fragmentation is likely occur. In one embodiment, the mechanical index is 4 or below, which is an FDA limit related to imaging. In one embodiment, the mechanical index is 1.9 or below, which is a lower FDA limit.

[0076] Probe Shapes

[0077] In one embodiment, the therapy probe has a largest aperture dimension (e.g., FIG. 1A OD) that is 5 cm or less. In one embodiment, the therapy probe has a largest aperture dimension (e.g., FIG. 1A OD) that is 2 cm or greater. In other embodiments, the OD is greater than 5 cm. Accordingly, in one embodiment the OD is less than 10 cm. In yet another embodiment the OD is less than 7 cm.

[0078] In one embodiment, the therapy probe has a single ultrasonic therapy element, thereby providing a fixed focus to define the therapy region.

[0079] In one embodiment, the therapy probe is annular with a center cavity configured that is acoustically transparent in order to allow the imaging probe to image through the center cavity.

[0080] In one embodiment, the therapy probe and the imaging probe are configured to mate together coaxially. Coaxial probes are illustrated in FIG. 1A, disposed along axis A. As used herein, the term “mate” refers to an arrangement where the therapy probe and imaging probe are disposed within the same combined probe, as illustrated in FIGS. 1A and 1B. Similarly, FIGS. 3-6 illustrate a FIG. 1C

illustrates non-coaxial probes, although in such a configuration the therapy probe **105** and imaging probe **110'** are still synchronized to provide a therapy exposure and image the therapy region **115**.

[0081] The imaging probe can be any imaging probe known to those of skill in the art that is sufficient to image the therapy region and synchronize with the therapy probe. Referring to FIG. 1A and 1C, the imaging probe **110** or **110'** has a height *h* and a width *w*. In one embodiment the height is from 1 cm to 2 cm. In one embodiment, the width is from 1 cm to 3 cm.

[0082] Imaging Synchronization

[0083] In one embodiment, the imaging probe and therapy probe are synchronized, such that imaging probe produces an imaging signal during an off period of the therapy exposure between pulses.

[0084] In one embodiment, the ultrasonic therapy system further comprises a switch configured to transition the ultrasonic therapy system from an imaging mode, wherein only the imaging probe is activated without the therapy probe, to a therapy mode, wherein the imaging probe and the therapy probe are both activated and synchronized to alternately produce an image of the therapy region and apply the therapy exposure to the therapy region.

[0085] In one embodiment, the ultrasonic therapy system is further configured to adjust a distance from the therapy probe to the start of the therapy region in response to changing a depth-of-focus of the imaging probe or vice versa.

[0086] Lenses

[0087] In one embodiment, the ultrasonic therapy system further includes a lens related to the therapy probe. A lens is essentially any material used to couple ultrasound to tissue. The lens is flat on the distal surface in one embodiment. In another embodiment the lens is convex on the distal surface. In another embodiment the lens is concave on the distal surface, thereby having a small cavity that can be filled with a gel or disposable pad.

[0088] In one embodiment, the lens is formed from a material selected from the group consisting of plastic, oil, ceramic, alcohol, water based fluid, gel, metal (e.g., aluminum), graphite, and combinations thereof. Representative plastics include siloxanes and urethanes. Particularly beneficial are polymers that can be polymerized at room temperature.

[0089] In one embodiment, the lens provides acoustic matching between the therapy probe and a therapy target.

[0090] In another embodiment, a matching layer is included in between the transducer and the lens. See, for example, part **615** in FIG. 12A. The matching layer does not provide focusing but instead functions to transition impedance between the transducer and lens. Impedance mismatch will produce acoustic energy noise. Representative matching layer materials include composites, such as epoxies loaded with tungsten, aluminum or graphite.

[0091] Amplifier

[0092] In one embodiment, the ultrasonic therapy system further includes an amplifier configured to drive the therapy probe. The amplifier can be off-the-shelf or custom designed to produce the necessary power. An example of an amplifier incorporated into a representative system in FIG. 14. In one embodiment, the amplifier is configured to operate at a voltage (peak-to-peak) of 100 V to 3,000 V. In one embodiment, the amplifier is configured to operate at a (time

average) power of 10 W to 1000 W. In one embodiment, the amplifier is configured to operate at a (time average) power of 20 W to 1000 W. In one embodiment, the amplifier is configured to operate at a (time average) power of 20 W to 500 W.

[0093] Cooling

[0094] In one embodiment, the ultrasonic therapy system further includes a cooling mechanism configured to remove heat from the therapy probe. FIGS. 12A-12D illustrate representative embodiments of probes **600** with incorporated cooling systems. Generally, the probe **600** includes a transducer **605**, a lens **610**, and a matching layer **615** between the transducer **605** and lens **610** to provide acoustic matching. An inlet and outlet **625** provides liquid or gas access to a cooling cavity **620**.

[0095] An optional thermocouple **606** or other temperature measurement component is applied to the transducer **605** (FIG. 12A) or the lens **610** (FIG. 12B), or both (not pictured). The thermocouple **606** can be attached to a display in order to provide the operator with a visual indication of the temperature of the transducer **605**, in case overheating is a danger, or the lens **610** if burning the patient's skin is a danger. The thermocouple can also be interfaced with a CPU or other system component in order to automate the indication of dangerous conditions or provide a feedback signal related to driving the transducer **605** (e.g., if the transducer **605** temperature rises dangerously the system will shut off the transducer **605**, activate cooling, and/or warn the operator).

[0096] The cooling cavity **620** is filled with a gas (e.g., air) in one embodiment. In another embodiment, the cooling cavity is filled with a liquid (e.g., water). The gas or liquid can be circulated through the inlet and outlet **625** to provide improved cooling.

[0097] Referring to FIG. 12B, a heat sink **630** is interfaced with the transducer **605** to remove heat therefrom. A plurality of fins of the heat sink **630** extend into the cooling cavity **620** to dissipate heat further.

[0098] Referring to FIG. 12C the heat sink **630** is instead disposed on the opposite wall of the cooling cavity **620** from the transducer **605**. A second heat sink **640** (or second portion of the first heat sink **630**) is disposed on the outside of the cooling cavity **620** in order to dissipate heat transferred from the transducer **605**, to the cooling cavity **620**, through the first heat sink **630** and then second heat sink **640**.

[0099] FIG. 12D is yet a further embodiment, which integrates a thermo-electric cooler **650** (TEC or Peltier element) to manage heat transferred from the transducer **605**.

[0100] In one embodiment, the cooling mechanism is selected from the group consisting of air cooling, liquid cooling, a heat sink, a heat pipe, a thermo-electric cooler, and combinations thereof.

[0101] In one embodiment, the cooling mechanism is configured to remove heat from a portion of the therapy probe selected from the group consisting of a lens and an ultrasonic therapy element.

[0102] Central Processing Unit (CPU)

[0103] In one embodiment, the ultrasonic therapy system further includes a central processing unit (CPU) and a user interface, wherein the therapy probe, the imaging probe, and the user interface are each operatively connected through the CPU, and wherein the CPU is configured to control ultra-

sonic exposure from the therapy probe according to the user interface. The CPU can be any CPU known to those of skill in the art, such as a personal computer. The CPU may be used to coordinate the activities of the various system components (e.g., probes, amplifier, imaging), as described in more detail below with reference to FIG. 14.

[0104] In one embodiment, the imaging probe is configured to produce an ultrasound image of the therapy region on the user interface and wherein the imaging probe is synchronized with the therapy probe to obtain images of the therapy region in between pulses from the therapy probe.

[0105] In one embodiment, the CPU is configured to change the location or size of the therapy region via the therapy probe in response to input through the user interface.

[0106] Expanded System

[0107] FIG. 14 schematically illustrates an “expanded” system 700 that includes many of the components already disclosed. A combined probe 701 includes a therapy probe 705 and an imaging probe 710 imbedded therein. A therapy region 715 is illustrated as containing a plurality of targets (e.g., kidney stones). A CPU/amplifier 717 ultimately drives the therapy probe 705 and coordinates with the ultrasound imaging system 730 to coordinate the imaging probe 710 and therapy probe 705. The CPU and amplifier may be split into different components or may be combined in a single unit. The amplifier 717 can be activated by several mechanisms, with the mechanism in FIG. 14 being a foot pedal 720. During operation, a user presses a foot pedal 720 to activate the therapy exposure via the amplifier 717 and therapy probe 705. Use of the foot pedal 720 allows the user hands-free activation of the system 700. When the foot is removed from the pedal 720 the therapy exposure ceases. A number of pulses are emitted from the therapy probe 705 during the therapy exposure.

[0108] The amplifier 717 powers the therapy probe 705 via a matching network 725 that provides the appropriate power characteristics to the therapy probe 705 to generate the desired signal.

[0109] The imaging probe 710 provides imaging via an ultrasound imaging system 730 of the type known to those of skill in the art. Coordination with the amplifier 717 is made via a synchronization 735 bridge and setting and controls are coordinate 740 (e.g., by USB).

[0110] An optional cooling system 745 can be activated to cool the combined probe 701 and may receive input from a temperature sensor (e.g., a thermocouple). The cooling system 745 may interface with the CPU/amplifier 717 to shut off or reduce use of the therapy probe 705 if the temperature reaches a set limit. Or the sensor may be used to active the cooling system 745 to cool the therapy probe 705.

[0111] Probes

[0112] In another aspect, a combined probe is provided according to the embodiments shown and described. The probe includes a therapy probe and at least a cavity in which to coaxially dispose an imaging probe. In certain embodiments, the combined probe includes the imaging probe disposed within the cavity. The combined probe can be interfaced with an amplifier and imaging system as disclosed herein and can be used to perform the methods disclosed herein.

[0113] Methods

[0114] In another aspect, a method of moving one or more target objects using ultrasonic propulsion is provided. In one

embodiment, the method includes applying a non-lithotriptic acoustic radiation force to a target object using an ultrasonic therapy system as shown and described herein. While the disclosed embodiments are primarily described in the context of moving kidney stones, it will be appreciated that the systems can be applied to move any small object within the appropriate range from the therapy probe. The target need not be in a living being.

[0115] In one embodiment, the target object is at least one in vivo kidney stone. The systems can be applied to patients in need in any manner useful to one of skill in the art. The systems are designed to ease the movement and eventual removal of kidney stones or fragments from the body. Therefore, the disclosed methods utilize the disclosed systems for moving one or more kidney stones.

[0116] In one embodiment, at least one the kidney stone is within a patient in an area selected from the group consisting of a kidney, a ureteropelvic junction (UPJ), a bladder, a ureterovesicle junction (UVJ), and a ureter. These are the typical portions of a human in which one or more kidney stones may reside and whose removal the systems and methods can facilitate.

[0117] In one embodiment, the at least one kidney stone is moved a distance of at least 3 mm. This is a significant distance within a patient and indicates the broad moving effect of the systems and methods.

[0118] In yet a further embodiment, a plurality of kidney stones are simultaneously moved a distance of at least 3 mm. In this embodiment, the at least one kidney stone is a plurality of kidney stones and wherein the plurality of kidney stones are moved a distance of at least 3 mm during the therapy exposure time.

[0119] In another aspect, a method of moving one or more kidney stones in a therapy region using ultrasonic propulsion is provided. In one embodiment, the method includes using a broadly focused ultrasound therapy probe to apply a force on one or more kidney stones having a diameter of from 0.5 mm to 20 mm disposed within the therapy region, wherein the acoustic radiation force applied to each of the one or more kidney stones is from 50 μ N to 0.5 N, and wherein the acoustic radiation force is not sufficient to fragment the kidney stones. This aspect is not necessarily tied to the exact devices disclosed herein, although such devices and systems are compatible with the present method. However, the present aspect at its most basic level is directed to use of broadly focused ultrasound to apply pressure to kidneys stones. In one embodiment, an imaging probe is synchronized with the therapy probe. This method is compatible with all of the systems, device, and methods disclosed elsewhere herein.

[0120] The following example is included for the purpose of illustrating, not limiting, the described embodiments.

EXAMPLES

[0121] Therapy Probe Design

[0122] In this Example we discuss single-element low-frequency design. Specifically, prior art lithotripsy and ultrasonic propulsion systems revealed the need and capability to expel clusters of stone fragments. These systems also failed to move large stones observably and did not detach stones. With the disclosed new single-element, broadly focused we can expel more fragments in a cluster more quickly. The change is an order of magnitude and enables 10 $\times$ the number of pulses with each pulse 10 $\times$ wider and spread across the

entire stone cluster. The new design therefore also has more promise to detach and move large stones. These advances potentially cut treatment from hours to minutes and make ultrasonic propulsion clinically viable.

[0123] The shift from a prior art 128-element, 2-MHz imaging/pushing probe to a single element, low frequency (300 kHz) therapy probe enables displacing an entire cluster of stones. The imbedded imaging probe allows the user to observe fragment and cluster displacement while effectively sweeping a region stone free.

[0124] Advantages of lower frequency include:

[0125] Less focal heating=ability to send more pulses

[0126] Less attenuation through tissue or ribs

[0127] Higher intensities without nonlinear saturation

[0128] Broader beam=easier targeting and potential to move a pile of fragments

[0129] Potential to break stones off attachments as 300 kHz is used for comminution

[0130] The potential disadvantages are:

[0131] Cavitation is more likely at low frequency. Cavitation may injure tissue but also helps break stones. A cavitation monitor has been added.

[0132] Potentially less radiation force on <1 mm fragments at lower frequency but very little force is needed for such small stones.

[0133] Advantages of single-element, single focus include:

[0134] Minimize probe heating

[0135] Unique low cost therapy component

[0136] Standard unmodified ultrasound imaging hardware (don't have to "push" with the imaging probe)

[0137] Single user operation

[0138] The potential disadvantages are:

[0139] The user has to align the stone in the focus.

[0140] There are technical reasons most medical ultrasound is in the MHz range and comparatively little has been done at 300 kHz.

[0141] Several prototypes have been designed and built. All have a roughly annual therapy element at 330 kHz. In the hole in the middle is an imaging probe. This is a low frequency imaging probe for medical imaging and is not normally used for medical therapy. The thicker elements use more voltage. In addition, most applications of PZTs want one dimension much larger than the other 2 with the other two being about a wavelength. The thicker elements make it harder to do this and the risk is other modes taking energy and causing heating. One embodiment has a p7-4 imager, the other has a p4-2 imager, and the last has a linear 128 element imager centered at 4-5 MHz (p6-3 imager). These all tend to be higher frequency imagers than normally used for kidneys and they have a smaller field of view.

[0142] The overall footprint diameter is 5 cm or less. This size factor is important when considering the usability of the probe in a clinical context. First, the probe must be easily hand held and operable with one hand. Second the probe must be small enough to apply to a patient at several different points on the body, which requires a small probe that can mate with any skin surface.

[0143] We have a lens over the therapy probe that is selected for good energy transfer to the subject through proper matching of the acoustic properties and to reduce the modes. We built the lenses out of plastic, metal and graphite. The choice also affects the curvature of the face. We place the imaging probe at aperture of the curvature for best

imaging (setting it back from the aperture reduces image quality but allows a smaller hole in the therapy probe). Then we use an acoustically transparent cover and either coupling gel or fluid in the space to make a flat face on the probe for coupling. This fluid might be used optionally be used for cooling, too, and the cover can be disposable.

[0144] An exemplary combined probe is pictured in FIG. 1B, with this model referred having a convex hole and a relatively large (about 1x2 cm) imaging probe. The annular therapy probe is typically driven at 400 KHz. The annular, single element therapy transducer can be seen around the perimeter and the central feature is the imbedded imaging probe.

[0145] Another probe, the Propulse-2R is as follows: hand held, off the shelf P4-2 Philips phased array imaging probe that is removable from the central cavity of the probe; therapy probe is about 5 cm in diameter; imaging probe is coaxial; imbedded thermocouple on the therapy probe transducer; convex RTV (room temperature vulcanization) lens; and no cooling system.

[0146] Another exemplary combined probe includes a single element therapy transducer with an imaging probe on the side, as illustrated in FIG. 1C and pictured in FIG. 1D. The exemplary probe of FIG. 1D includes a concave aluminum lens, a 3D printed housing with a concave lens with water coupling, a second lens that is concave formed from RTV silicon.

[0147] Other variations utilized in experimental probes are as follows:

[0148] Cold-water cooling on the outside of the probe.

[0149] Backside cooling. Oil cooling on the back side of the therapy transducer. Forced air back cooling. Vortex back cooling

[0150] A therapy-probe-only system was fabricated, with no imager.

[0151] Certain prototypes included a metal lens, cooling system, with and without latex, and a concave lens.

[0152] A system was fabricated wherein the imager and therapy probes were connected but not concentric.

[0153] Stacked transducers.

[0154] Porous ceramic and composite transducers.

[0155] 1-16 element therapy elements on either side of an imaging probe

[0156] Redesigned imaging probes to make them flatter to have a farther focus, to lower the frequency, and to have better cooling.

[0157] Exemplary Test Results

[0158] FIGS. 8A and 8B are graphical depictions of simulation data relating to a prior art therapy probe (FIG. 8A) and an exemplary probe (FIG. 8B). The simulation data were generated using the FOCUS ultrasound simulator from Michigan State University. Comparative FIG. 8A is a 128 element transducer operating at 2.4 MHz while exemplary FIG. 8B is a single transducer element operating at 400 kHz and dimensions of inner diameter 3 cm, outer diameter 5 cm, and geometric focus of 5 cm.

[0159] Because the figures are converted from color, the full data cannot be presented properly herein. However, a black line is drawn around the boundary in each figure showing the region of highest pressure, which defines the respective therapy regions.

[0160] FIGS. 9-11 relate to experimental testing to determine the "stone pushing" efficacy of the therapy probes (sometimes referred to herein as "LFP" or low-frequency

pusher probes) according to the disclosed embodiments and compare them to prior art therapy probes. In order to accomplish this, an experimental design according to FIG. 9 was employed. Specifically, simulated kidney stones were pushed by a transducer while recording the “pushing” of the stones using a digital camera and subsequent image analysis.

[0161] In this example the stone fragments were created using BEGO simulated kidney stone material cement in 1 cm tall×6 mm diameter cylindrical molds. The hardened model stones were crushed into fragments and sieved into groups of 3-4 mm, 2-3 mm, 1-2 mm, and <1 mm, each having a sum mass of 80 mg. In addition there was a single model stone of 160 mg and a single model stone of 80 mg. Each group was placed into a pipette and filled with distilled and degassed water.

[0162] Each pipette was placed vertical in a holder with a 5 cm phantom between the transducer and stones.

[0163] The phantom (IEC 60601-2-37) simulated human tissue with attenuation approximately 0.5 dB/cm/MHz and sound speed near 1540 cm/s.

[0164] A video camera was used to record the stone motion at approximately 60 fps.

[0165] Ten acquisitions were made for each system configuration and stone grouping. The exemplary LFP probe was operated at 350 kHz. Both the Propulse-I system (clinical system with the C5-2 diagnostic probe, 128 elements activated, dithered focal volume) and 40 element configuration (C5-2 diagnostic probe with 40 elements activated with no dithering) were operated at their maximum output power. The low frequency probe was tested at 1.1 MPa and 2.4 MPa and 100 ms and 200 ms. Each video frame was processed using two different methods. One method segmented all fragments separately, measured the height of the center of the fragments, and estimated the total volume of the fragment based upon the segmented cross-sectional area. The height was multiplied by the volume and summed for all segmented fragments in the field of view. This summed value is the metric for this method. This method does well for all methods where the fragments are >1 mm, but cannot segment the small pieces effectively. The second method simply thresholds the image appropriately, and takes a summation of all the resulting pixels scaled by their height.

[0166] FIG. 10 compiles still images at the endpoint (maximum pushed distance) of a test run for each of the transducers tested. The transducers were all tested using the same simulated kidney stones and related environment. The LFP transducers, particularly at higher pressures, were more effective at moving multiple stones longer distances. Relating these results back to the simulations of FIGS. 8A and 8B, the LFP transducers (FIG. 8B) produce a much larger therapy region, with higher pushing force on the stones, than traditional therapy probes (FIG. 8A). Until now, such a broad focus was not desirable.

[0167] FIG. 11 summarizes data for 10 sample runs of the type illustrated in FIG. 10, in order to numerically characterize the efficacy of the transducers. The Y-axis relates to Relative Push Amount, which is calculated by averaging 10 push runs. It is the sum of the heights of the dark pixels (pixels related to stone) and standard deviation error bars. As was seen in FIG. 10, the LFP transducers according to the disclosed embodiments provided significantly superior pushing force on the stones. The unusual and unexpected efficacy of the inventive transducers compared to the prior art is apparent when viewing FIG. 11

[0168] While illustrative embodiments have been illustrated and described, it will be appreciated that various changes can be made therein without departing from the spirit and scope of the invention.

1. An ultrasonic therapy system configured to apply a non-lithotriptic acoustic radiation force to a kidney stone, comprising:

- (a) a therapy probe configured to generate ultrasonic exposure directed towards a therapy region; and
- (b) an imaging probe configured to ultrasonically image the therapy region;

wherein the therapy probe is configured to produce a therapy exposure comprising one or more therapy pulses over a therapy exposure time, wherein the therapy exposure has the following characteristics:

- (i) a frequency of 100 kHz to 1 MHz;
- (ii) therapy exposure time of at least 10 ms;
- (iii) a peak negative pressure in the therapy region of 0.5 MPa to 5 MPa;
- (iv) the therapy region of one pulse defining a volume subjected to a full-width half-maximum pressure or greater and the therapy region having a length of 2 cm or greater in an axial direction and 2 mm or more in width; and
- (v) the therapy region is sufficient to exert an acoustic radiation force on a kidney stone having a diameter of from 0.5 mm to 20 mm disposed within the therapy region, wherein the acoustic radiation force applied to the kidney stone is from 50 μ N to 0.5 N, and wherein the acoustic radiation force is not sufficient to fragment the kidney stone.

2. (canceled)

3. The ultrasonic therapy system of claim 1, wherein the therapy probe is configured to produce an average power of 10 W to 200 W for 1 second to 10 min.

4-10. (canceled)

11. The ultrasonic therapy system of claim 1, wherein the therapy exposure is a single continuous pulse.

12. The ultrasonic therapy system of claim 1, wherein the therapy exposure comprises a therapy burst that comprises a plurality of pulses separated by off periods.

13-14. (canceled)

15. The ultrasonic therapy system of claim 1, wherein the therapy probe has a largest aperture dimension that is 5 cm or less.

16. The ultrasonic system of claim 1, wherein the therapy probe has a single ultrasonic therapy element, thereby providing a fixed focus to define the therapy region.

17. The ultrasonic therapy system of claim 1, wherein the therapy probe is annular with a center cavity configured that is acoustically transparent in order to allow the imaging probe to image through the center cavity.

18. The ultrasonic therapy system of claim 1, wherein the therapy probe and the imaging probe are configured to mate together coaxially.

19. The ultrasonic therapy system of claim 1, wherein the imaging probe and therapy probe are synchronized, such that imaging probe produces an imaging signal during an off period of the therapy exposure between pulses.

20. The ultrasonic therapy system of claim 19, further comprising a switch configured to transition the ultrasonic therapy system from an imaging mode, wherein only the imaging probe is activated without the therapy probe, to a therapy mode, wherein the imaging probe and the therapy

probe are both activated and synchronized to alternately produce an image of the therapy region and apply the therapy exposure to the therapy region.

21. The ultrasonic therapy system of claim **19**, further configured to adjust a distance from the therapy probe to the start of the therapy region in response to changing a depth-of-focus of the imaging probe or vice versa.

22. The ultrasonic therapy system of claim **1**, further comprising a lens related to the therapy probe.

23. (canceled)

24. The ultrasonic therapy system of claim **22**, wherein the lens provides acoustic matching between the therapy probe and a therapy target.

25. The ultrasonic therapy system of claim **1**, further comprising an amplifier configured to drive the therapy probe.

26-27. (canceled)

28. The ultrasonic therapy system of claim **1**, further comprising a cooling mechanism configured to remove heat from the therapy probe.

29. (canceled)

30. The ultrasonic therapy system of claim **28**, wherein the cooling mechanism is configured to remove heat from a

portion of the therapy probe selected from the group consisting of a lens and an ultrasonic therapy element.

31. The ultrasonic therapy system of claim **1**, further comprising a central processing unit (CPU) and a user interface, wherein the therapy probe, the imaging probe, and the user interface are each operatively connected through the CPU, and wherein the CPU is configured to control ultrasonic exposure from the therapy probe according to the user interface.

32. The ultrasonic therapy system of claim **31**, wherein the imaging probe is configured to produce an ultrasound image of the therapy region on the user interface and wherein the imaging probe is synchronized with the therapy probe to obtain images of the therapy region in between pulses from the therapy probe.

33. The ultrasonic therapy system of claim **31**, wherein the CPU is configured to change the location or size of the therapy region via the therapy probe in response to input through the user interface.

34. A method, comprising applying a non-lithotriptic acoustic radiation force to a target object using an ultrasonic therapy system of claim **1**.

35-38. (canceled)

* * * * *

专利名称(译)	广泛聚焦的超声波推进探针，系统和方法		
公开(公告)号	US20170245874A1	公开(公告)日	2017-08-31
申请号	US15/519821	申请日	2015-10-19
[标]申请(专利权)人(译)	华盛顿大学		
申请(专利权)人(译)	华盛顿大学		
当前申请(专利权)人(译)	华盛顿大学		
[标]发明人	BAILEY MICHAEL R CUNITZ BRYAN DUNMIRE BARBRINA MAXWELL ADAM LEVY OREN		
发明人	BAILEY, MICHAEL R. CUNITZ, BRYAN DUNMIRE, BARBRINA MAXWELL, ADAM LEVY, OREN		
IPC分类号	A61B17/22 A61B8/08		
CPC分类号	A61B17/22004 A61B2017/22005 A61B8/085 A61B17/2258 A61B2018/00023 A61B2018/00511 A61N7/02		
优先权	62/065432 2014-10-17 US 62/160458 2015-05-12 US		
其他公开文献	US10667831		
外部链接	Espacenet USPTO		

摘要(译)

本文公开了超声探针和结合探针的系统。探针配置成产生超声治疗暴露，当应用于肾结石时，将施加足以产生超声推进的声辐射力。然而，与配置成产生超声推进的先前探针不同，所公开的探针被设计成产生有效产生超声推进的相对大（宽和长）治疗区域。该大治疗区域允许探针平行移动多个肾结石（或来自碎石的碎片），从而使用户能够同时从一个区域清除多个结石。在某些实施例中，该“广泛聚焦”探针在单个手持单元中与典型的超声成像探头组合以产生实时成像。还提供了使用探针和系统移动肾结石的方法。

