



US 20190175152A1


(19) **United States**(12) **Patent Application Publication**
SMITH et al.(10) **Pub. No.: US 2019/0175152 A1**(43) **Pub. Date: Jun. 13, 2019**(54) **CALIBRATION OF ULTRASOUND PROBES**


(60) Provisional application No. 61/169,200, filed on Apr. 14, 2009.

(71) Applicant: **MAUI IMAGING, INC.**, Sunnyvale, CA (US)**Publication Classification**(72) Inventors: **David M. SMITH**, Lodi, CA (US);
Sharon L. ADAM, San Jose, CA (US);
Donald F. SPECHT, Los Altos, CA (US);
Kenneth D. BREWER, Santa Clara, CA (US);
John P. LUNSFORD, San Carlos, CA (US);
David J. SPECHT, San Jose, CA (US)(51) **Int. Cl.**
A61B 8/00 (2006.01)
G01S 15/89 (2006.01)
G01S 7/52 (2006.01)(73) Assignee: **MAUI IMAGING, INC.**, Sunnyvale, CA (US)(52) **U.S. Cl.**
CPC **A61B 8/587** (2013.01); **A61B 8/4483** (2013.01); **A61B 8/4254** (2013.01); **A61B 8/00** (2013.01); **A61B 8/4444** (2013.01); **A61B 8/4218** (2013.01); **G01S 15/8915** (2013.01); **G01S 15/8913** (2013.01); **G01S 7/5205** (2013.01); **A61B 8/4477** (2013.01)(21) Appl. No.: **16/277,853**(57) **ABSTRACT**(22) Filed: **Feb. 15, 2019****Related U.S. Application Data**

(63) Continuation of application No. 15/044,932, filed on Feb. 16, 2016, now Pat. No. 10,206,662, which is a continuation of application No. 13/279,110, filed on Oct. 21, 2011, now Pat. No. 9,282,945, which is a continuation-in-part of application No. 12/760,327, filed on Apr. 14, 2010, now Pat. No. 8,473,239.

A method of calibrating an ultrasound probe includes mounting an ultrasound probe onto a calibration system, transmitting an ultrasound test signal from an element of the probe through a test medium of the calibration system, and receiving the test signal on a matrix of hydrophones such that an element's position relative to other elements and other arrays within the same probe can be computed. Further, the system described herein is configured to detect the acoustic performance of elements of a probe and report the results to an end user or service provider.

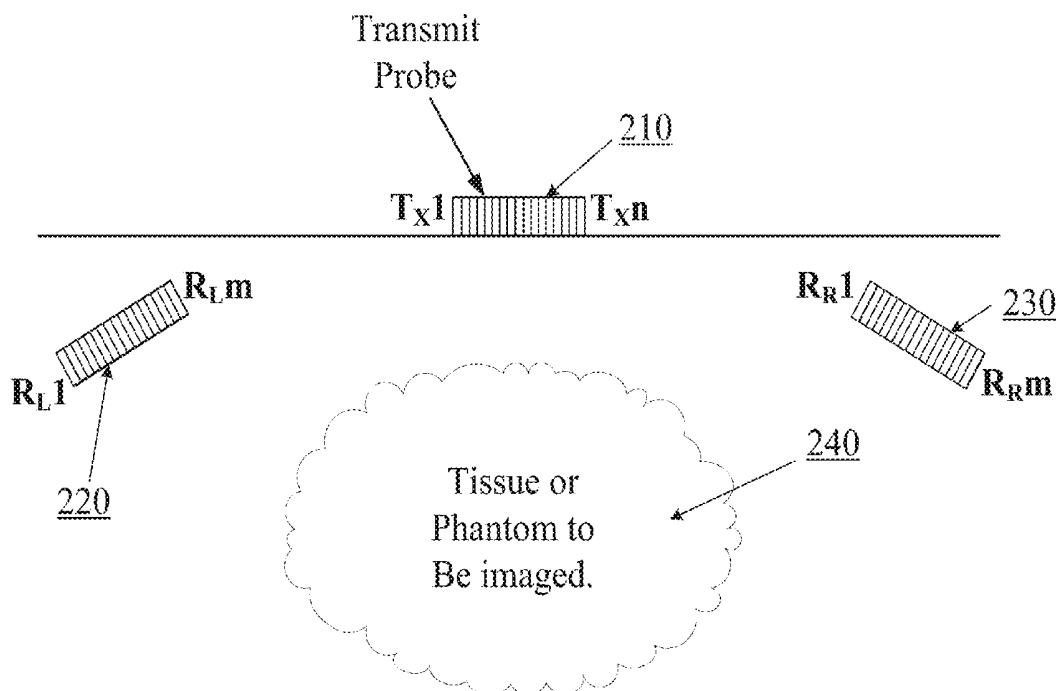

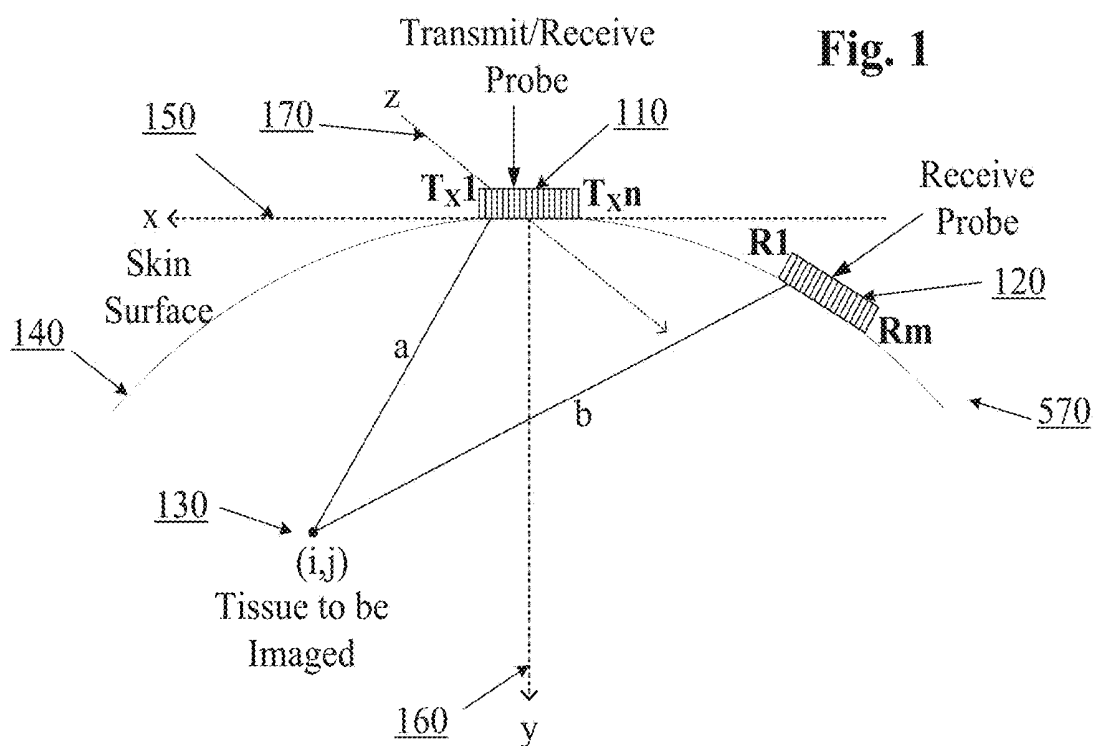

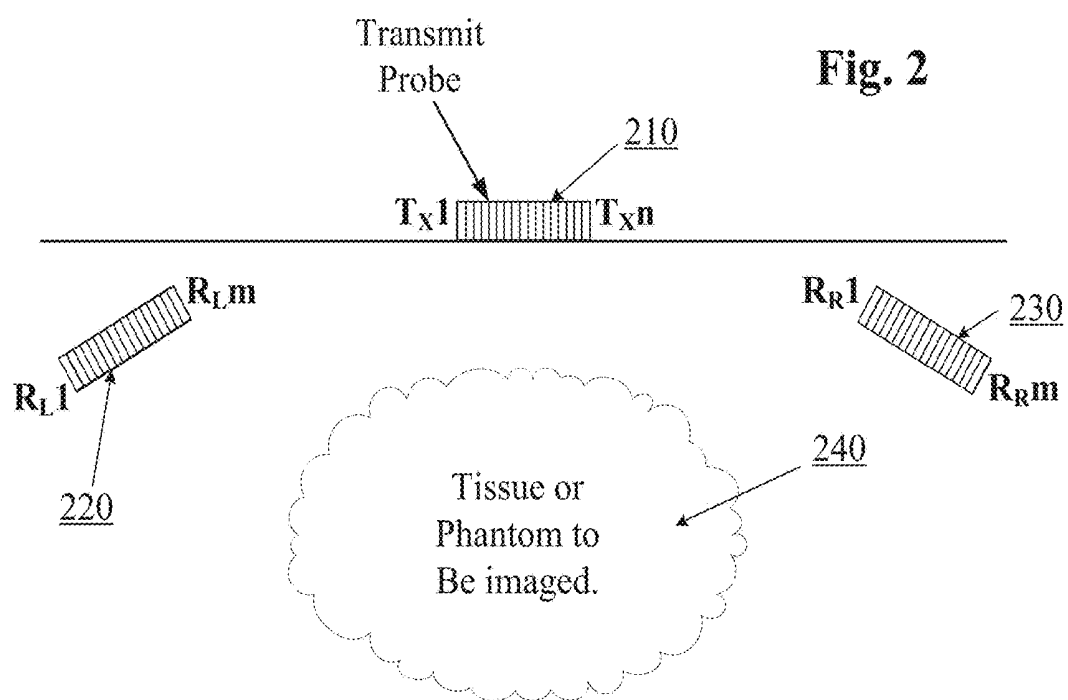
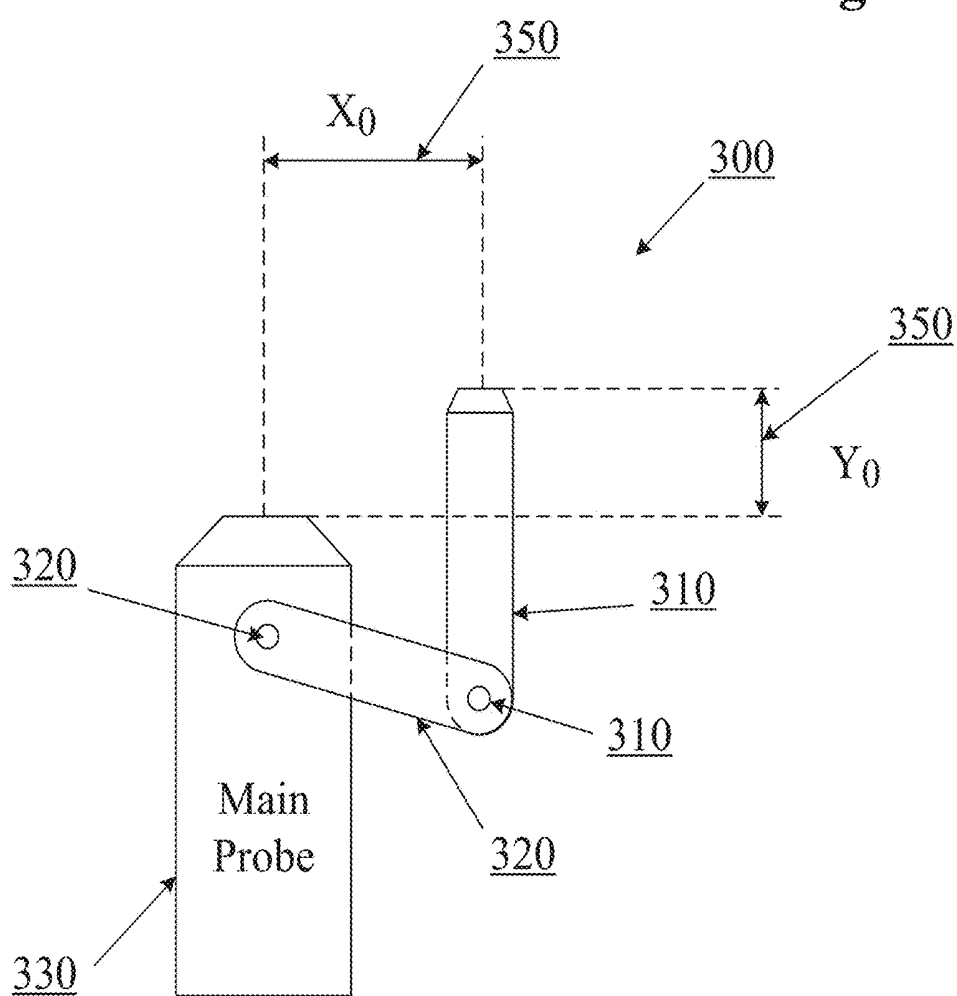
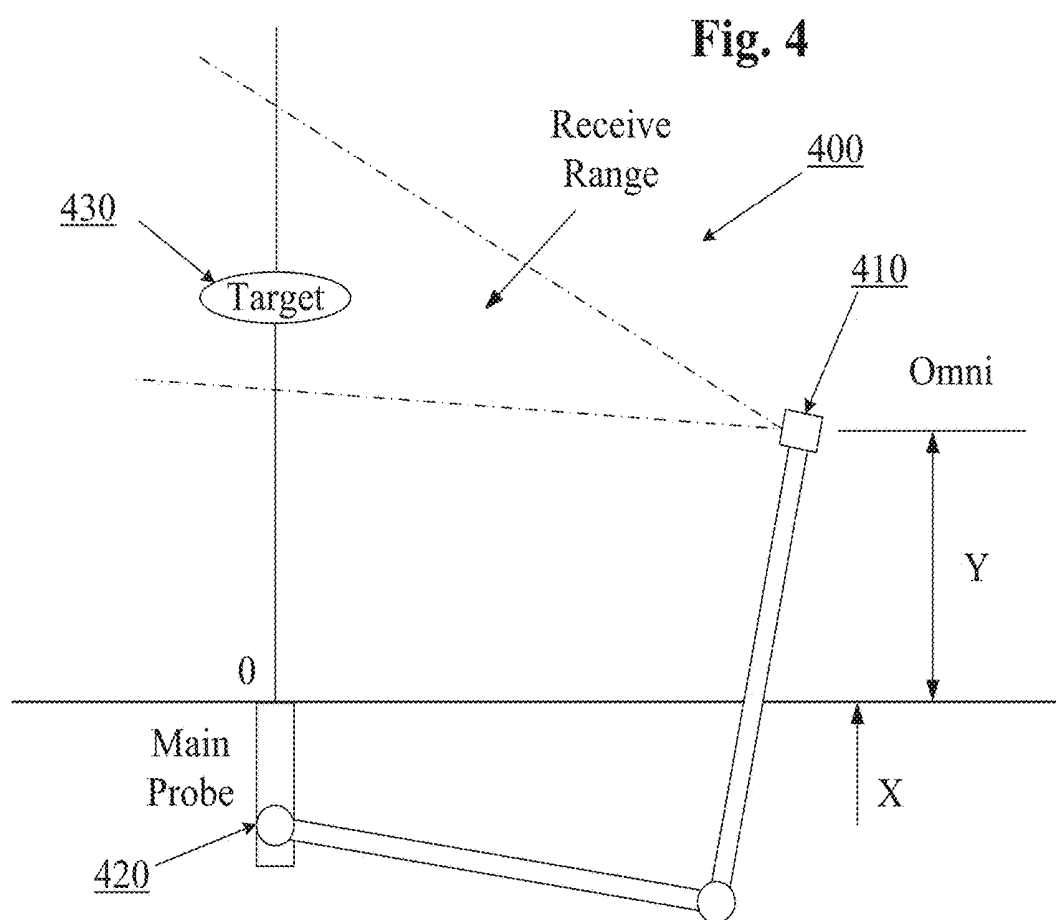
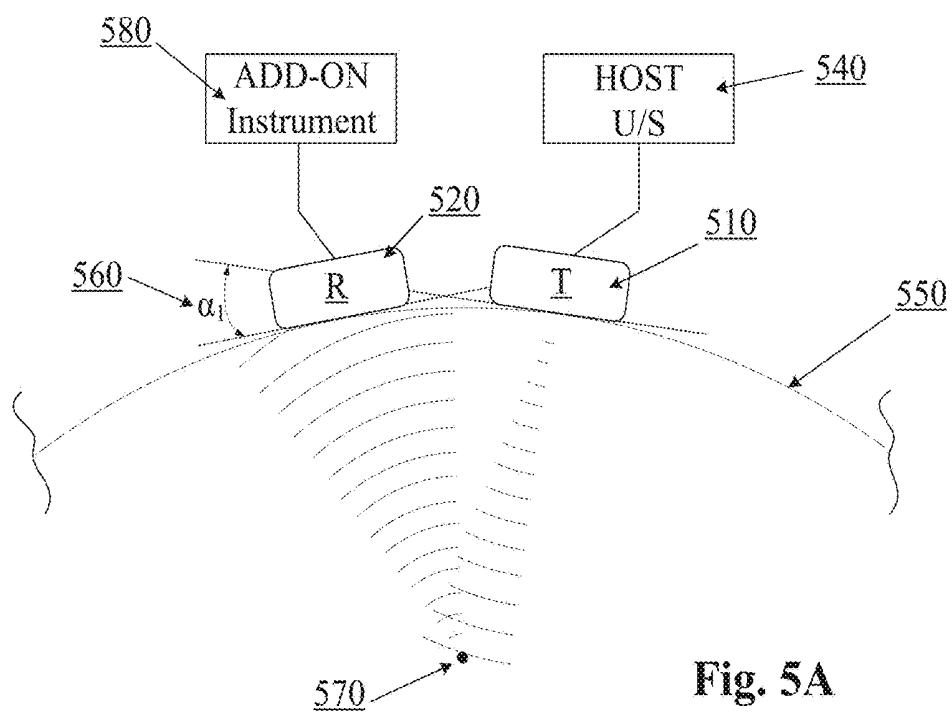
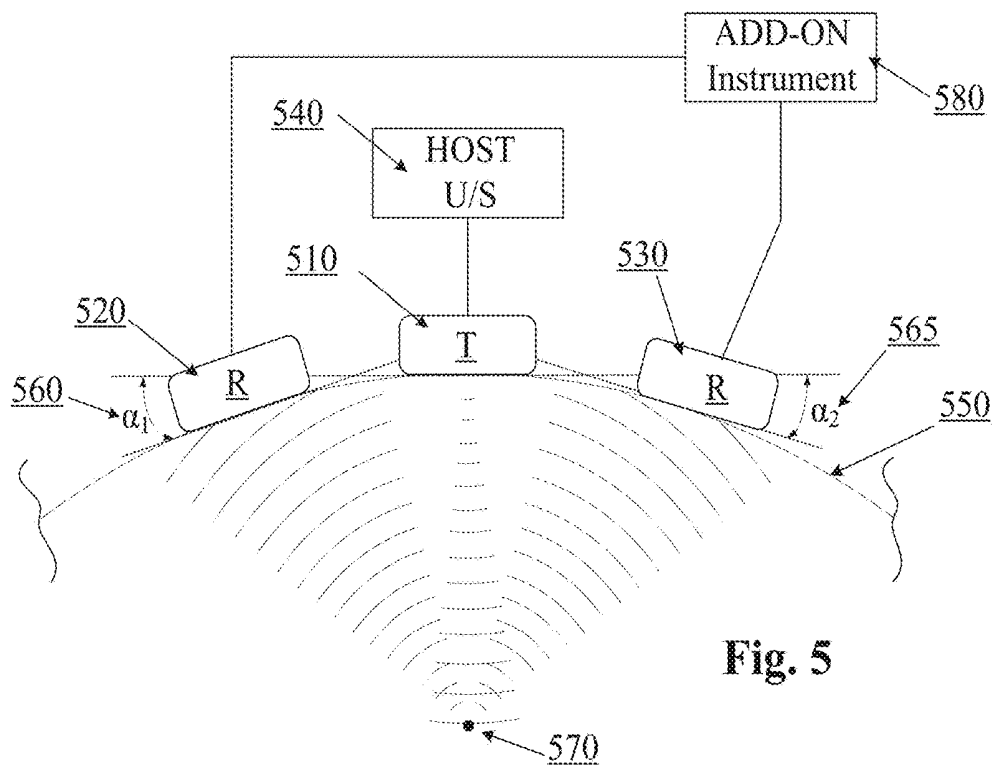


Fig. 3







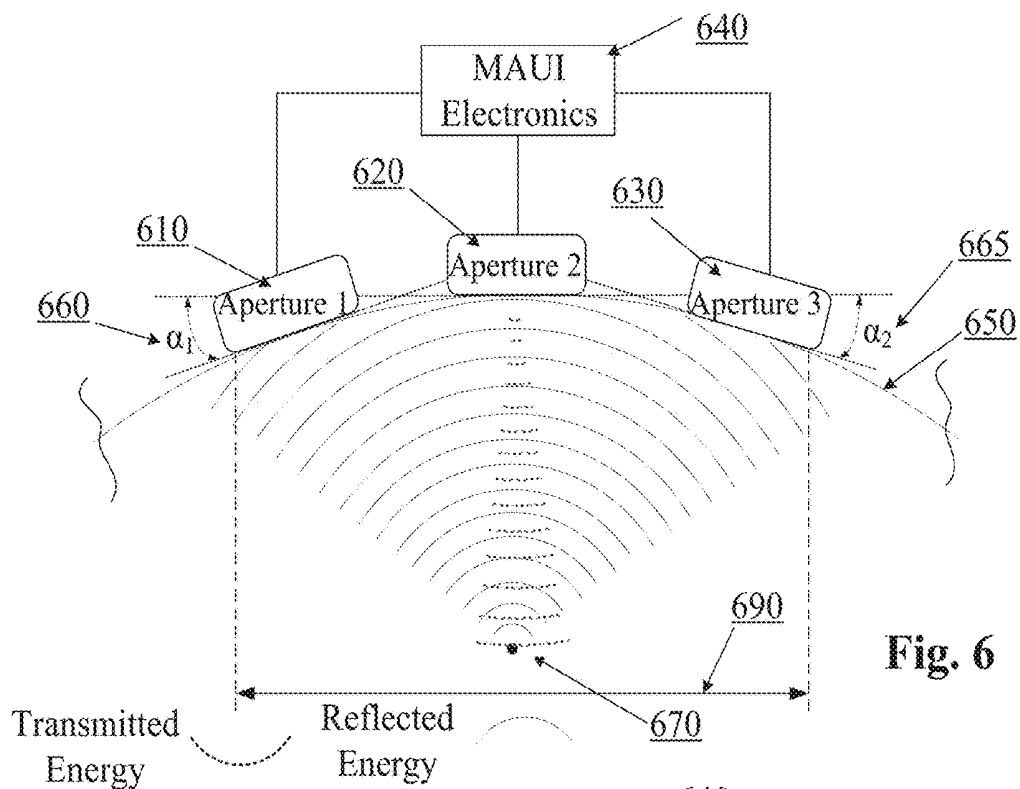


Fig. 6

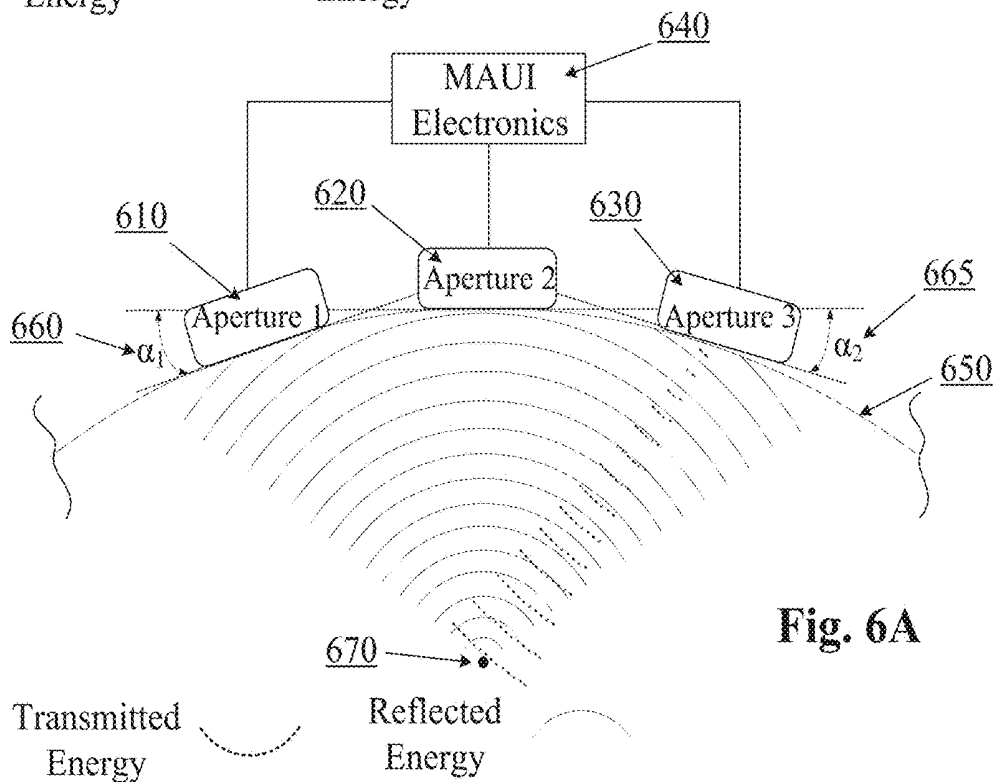


Fig. 6A

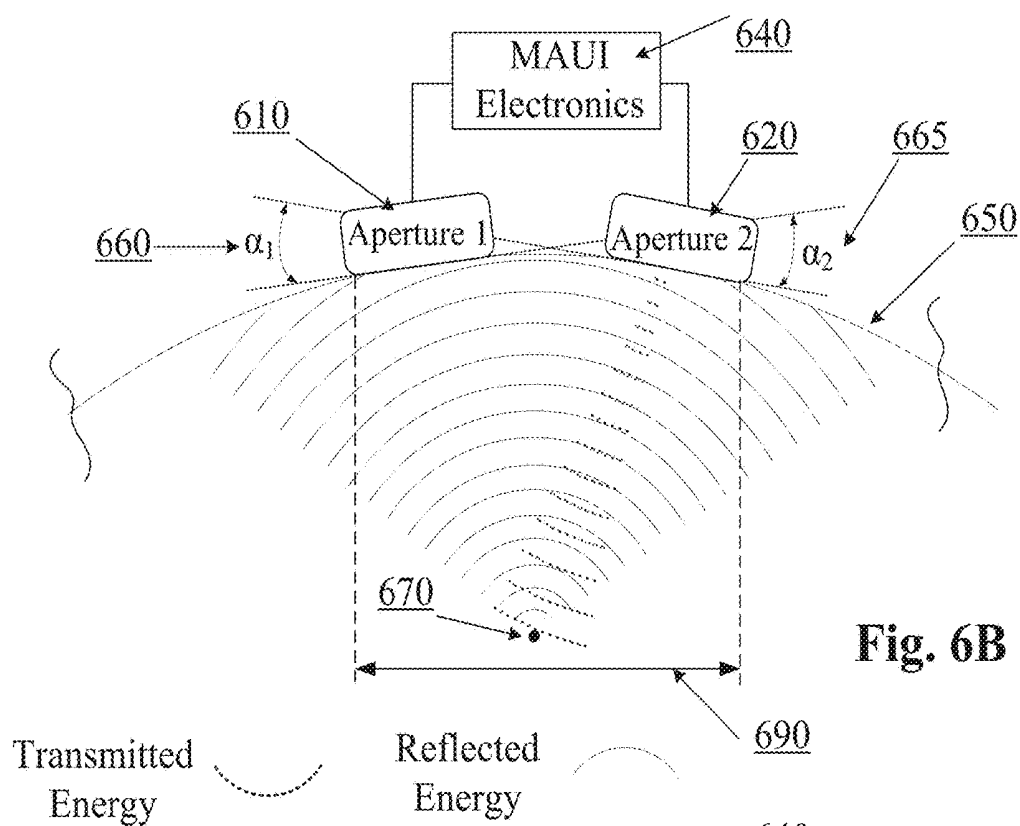


Fig. 6B

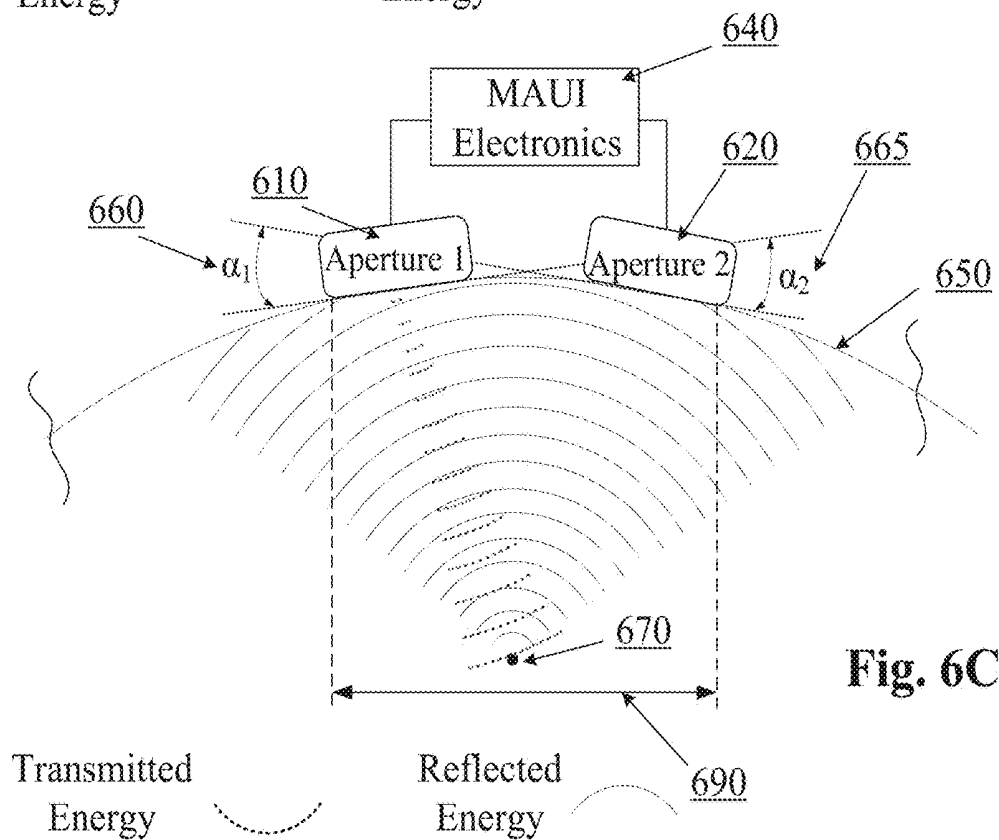


Fig. 6C

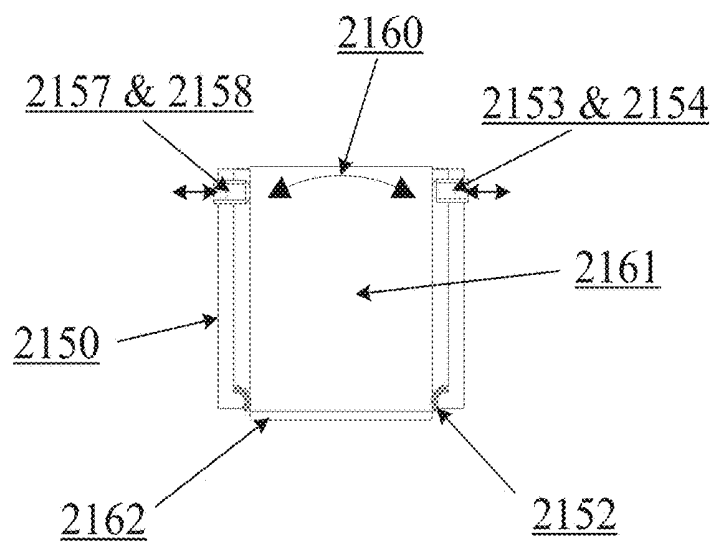
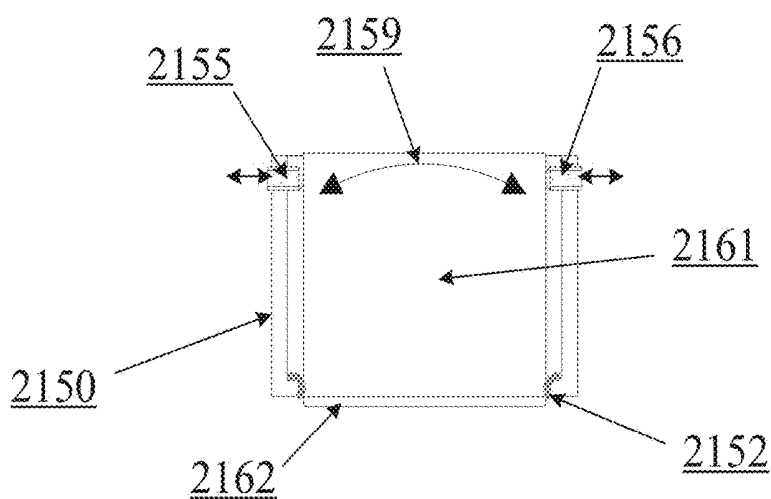
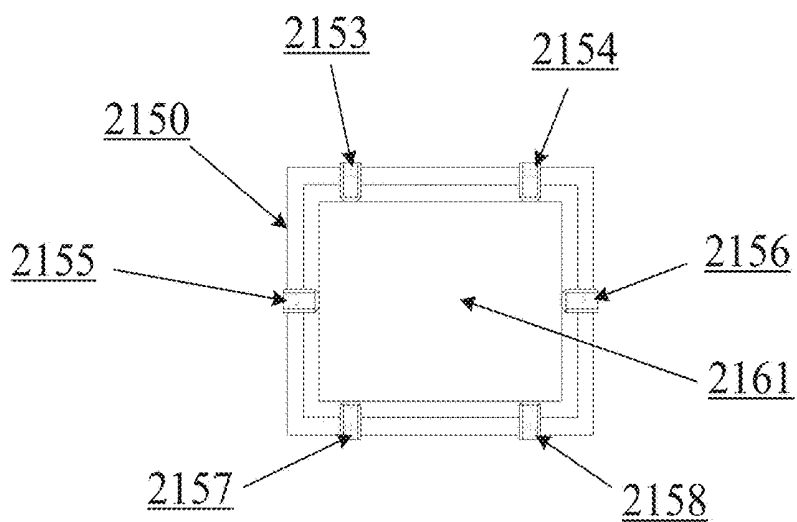


Fig. 8A

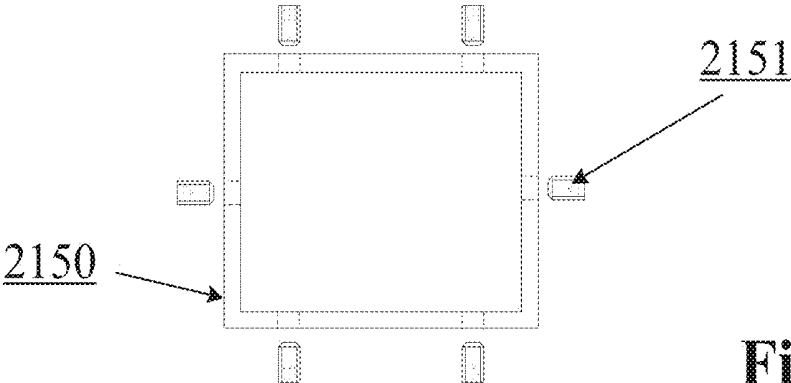


Fig. 8B

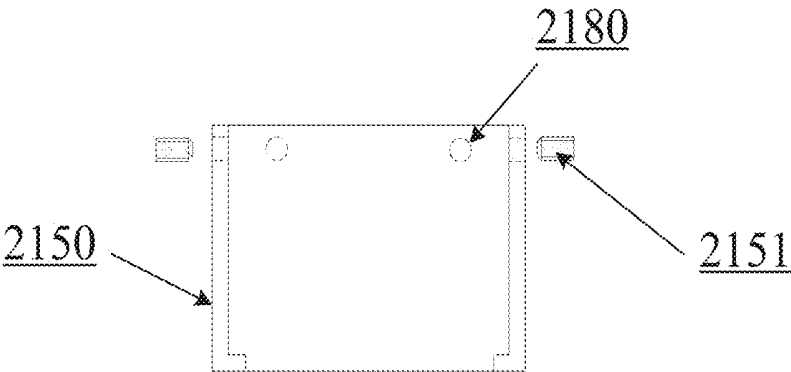


Fig. 8C

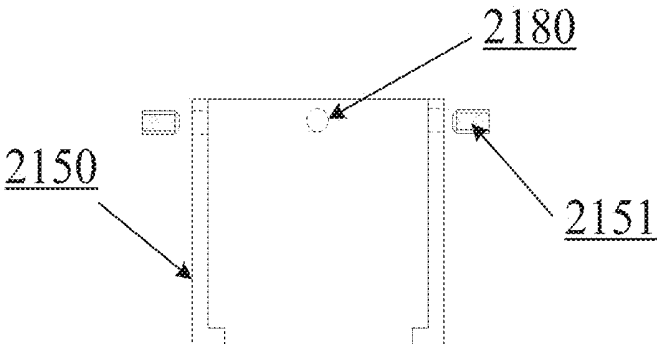


Fig. 9A

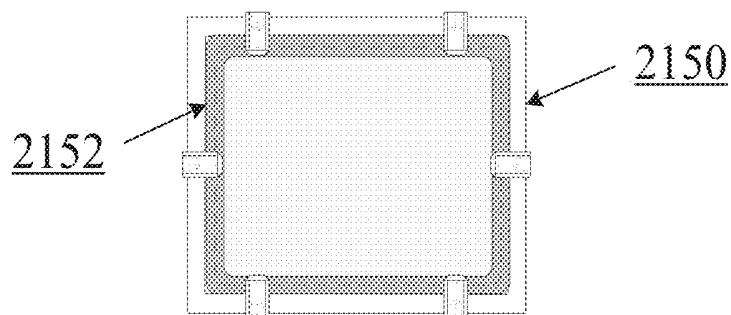


Fig. 9B

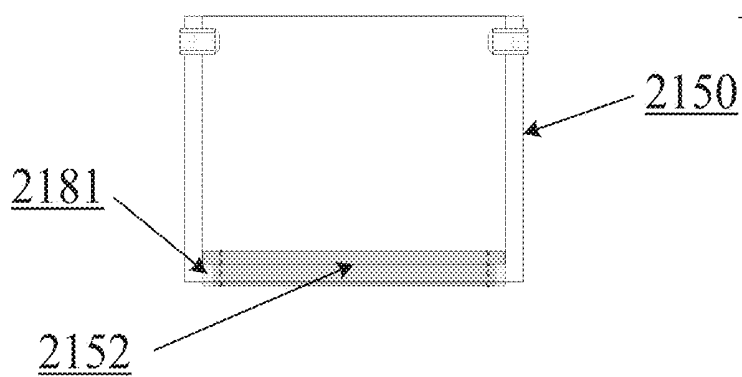


Fig. 9C

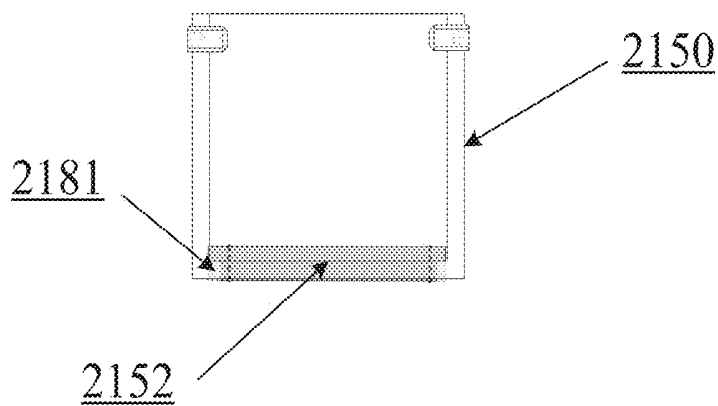
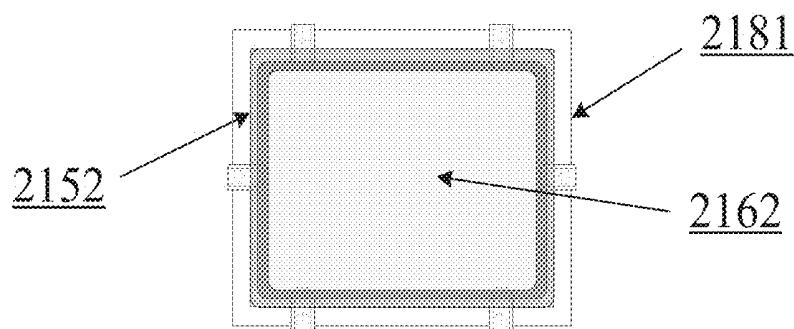
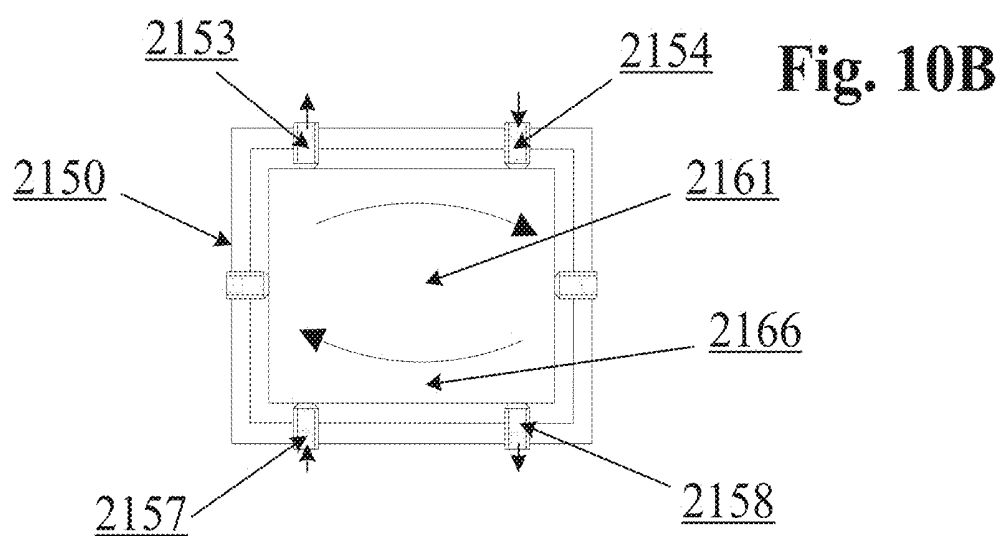
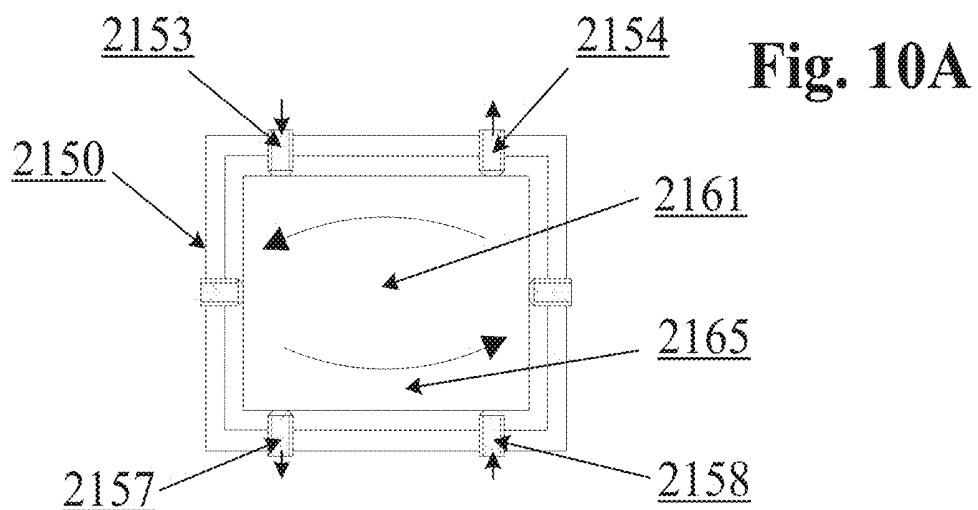


Fig. 9D





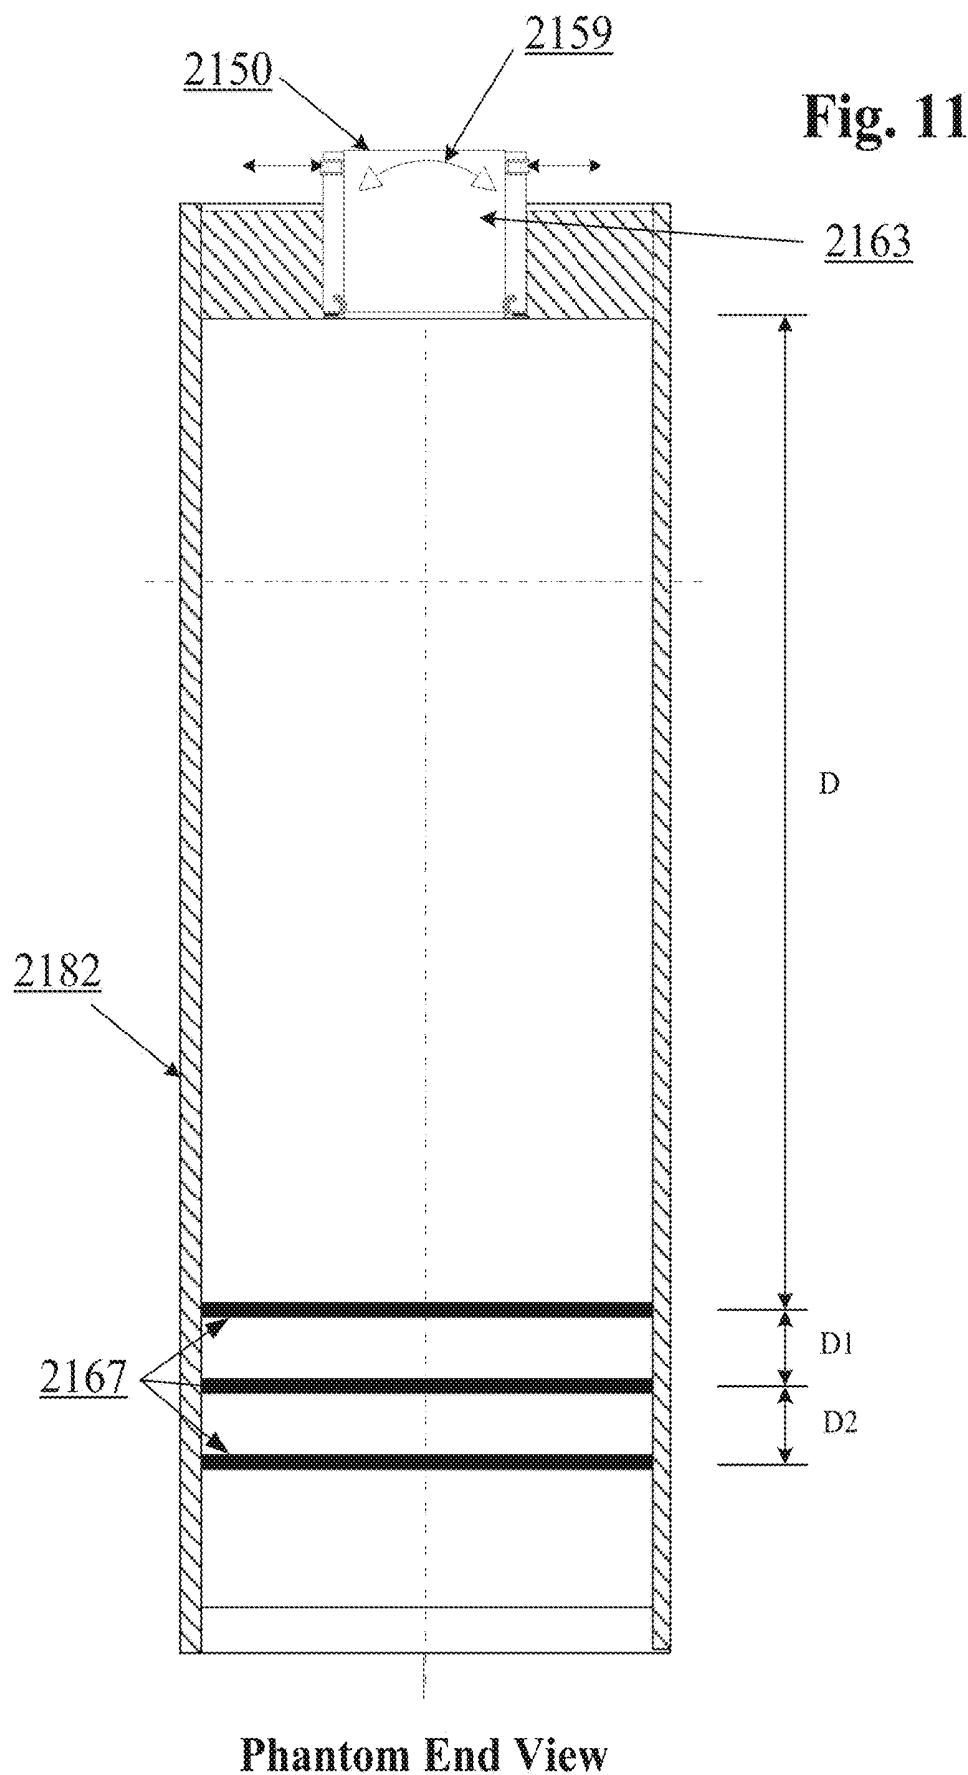


Fig. 12

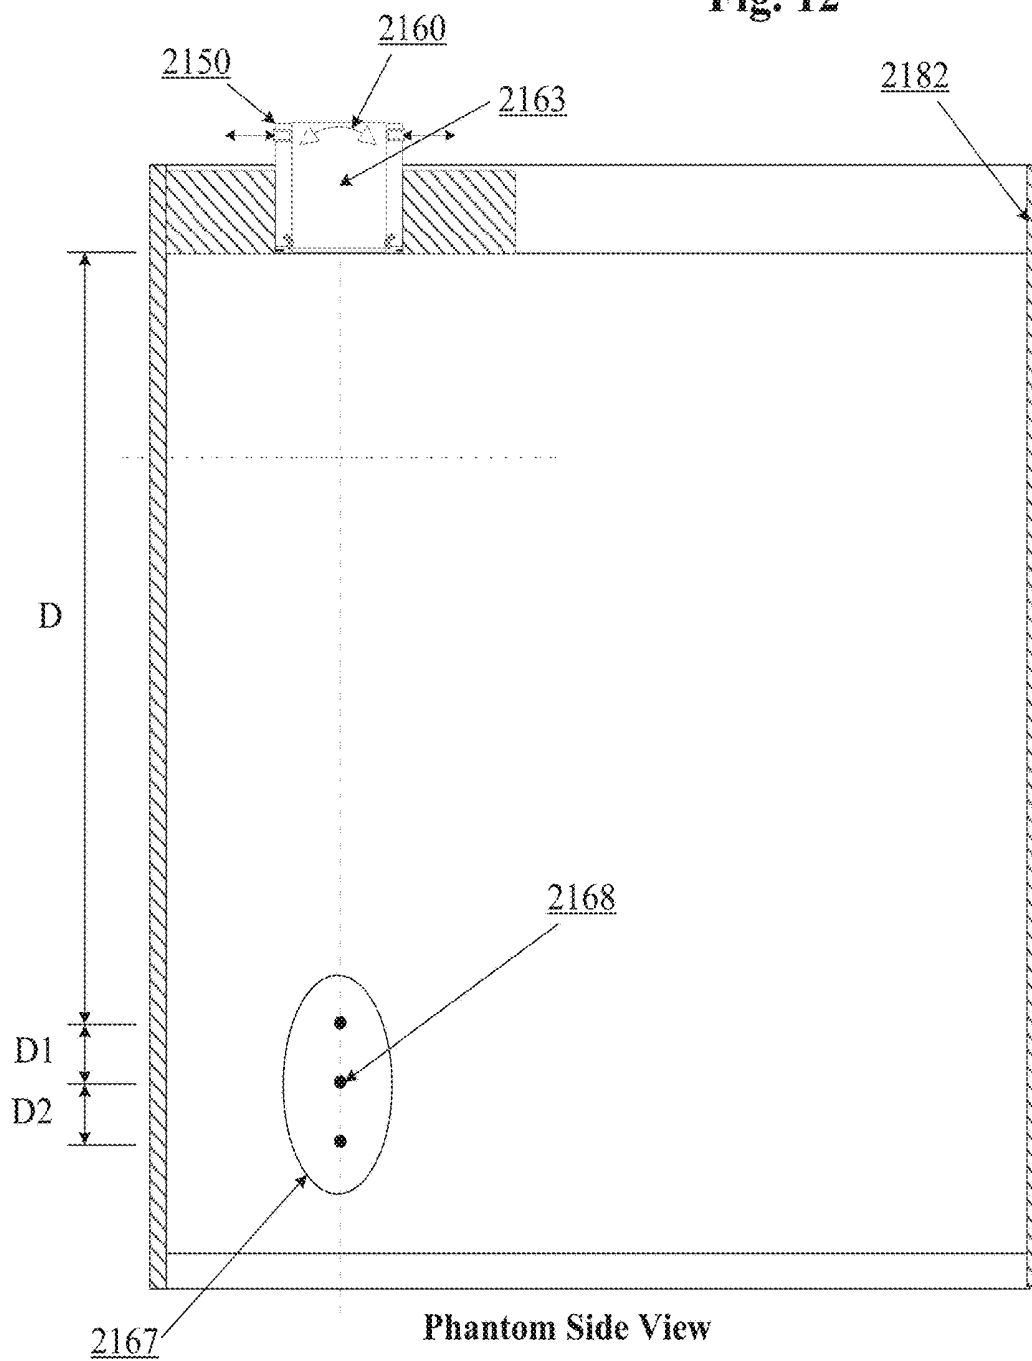


Fig. 13A

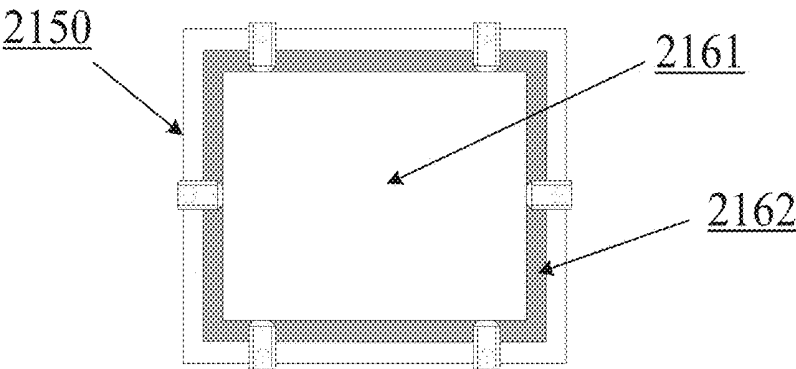


Fig. 13B

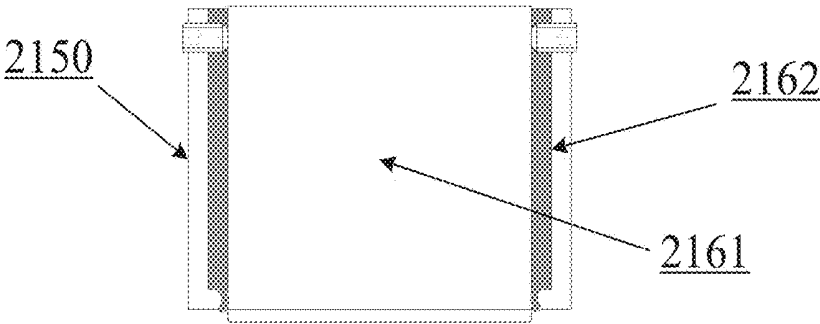


Fig. 13C

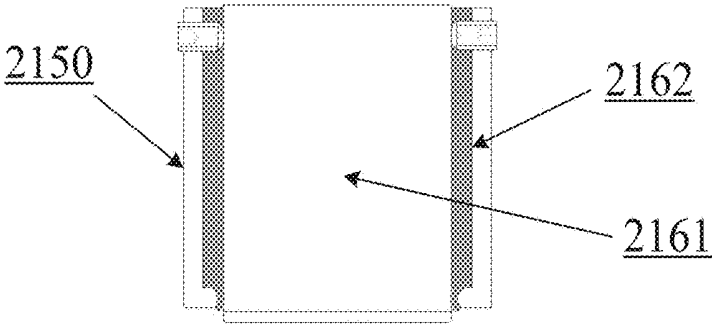


Fig. 14A

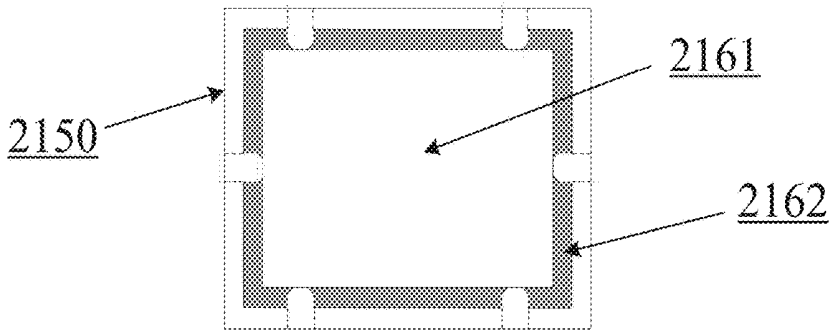


Fig. 14B

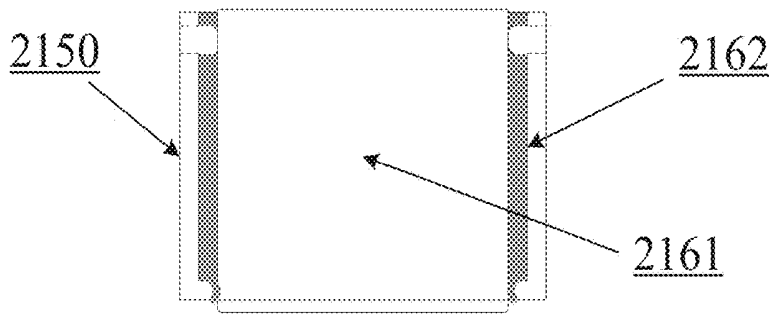
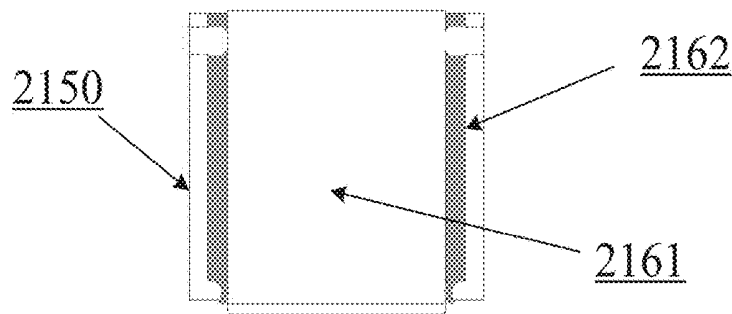


Fig. 14C



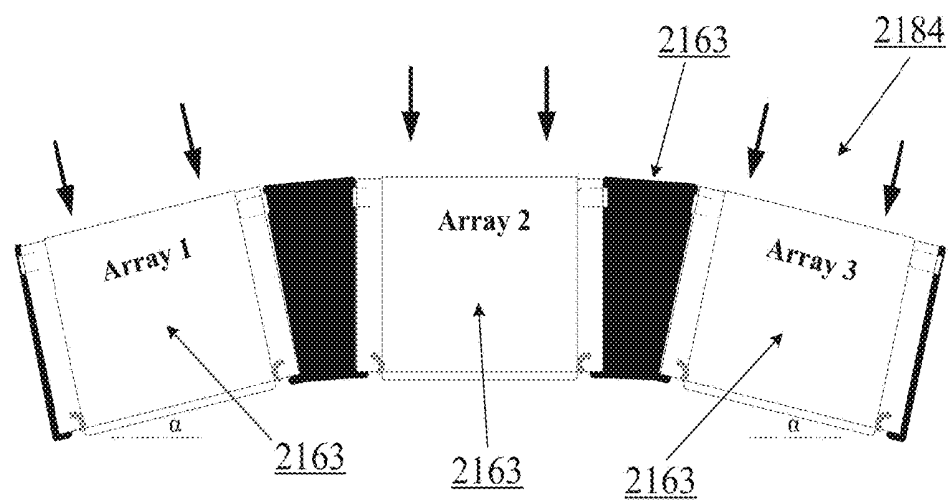
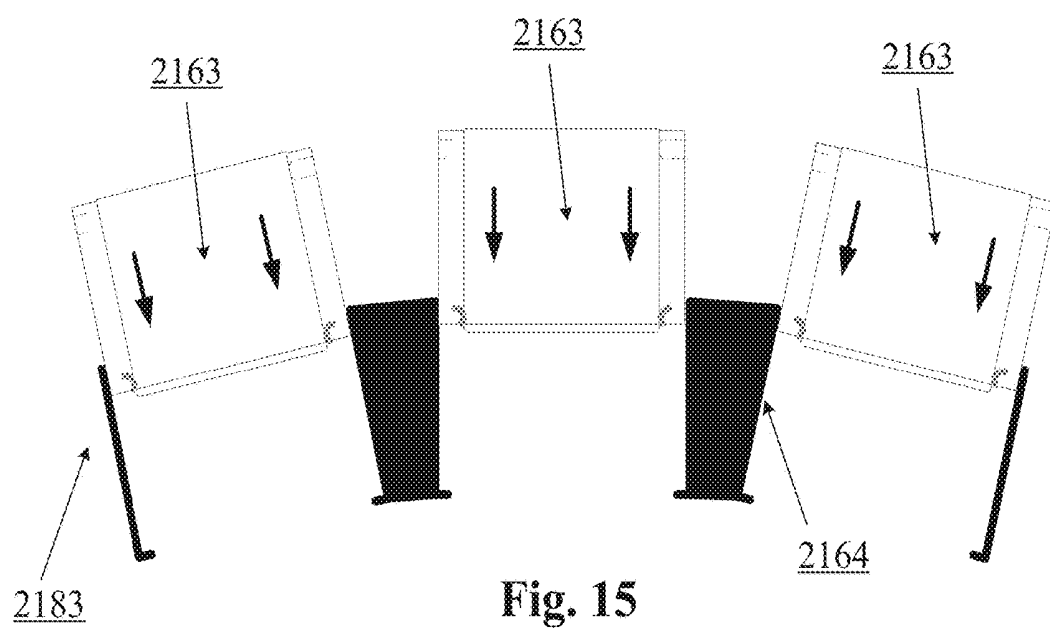
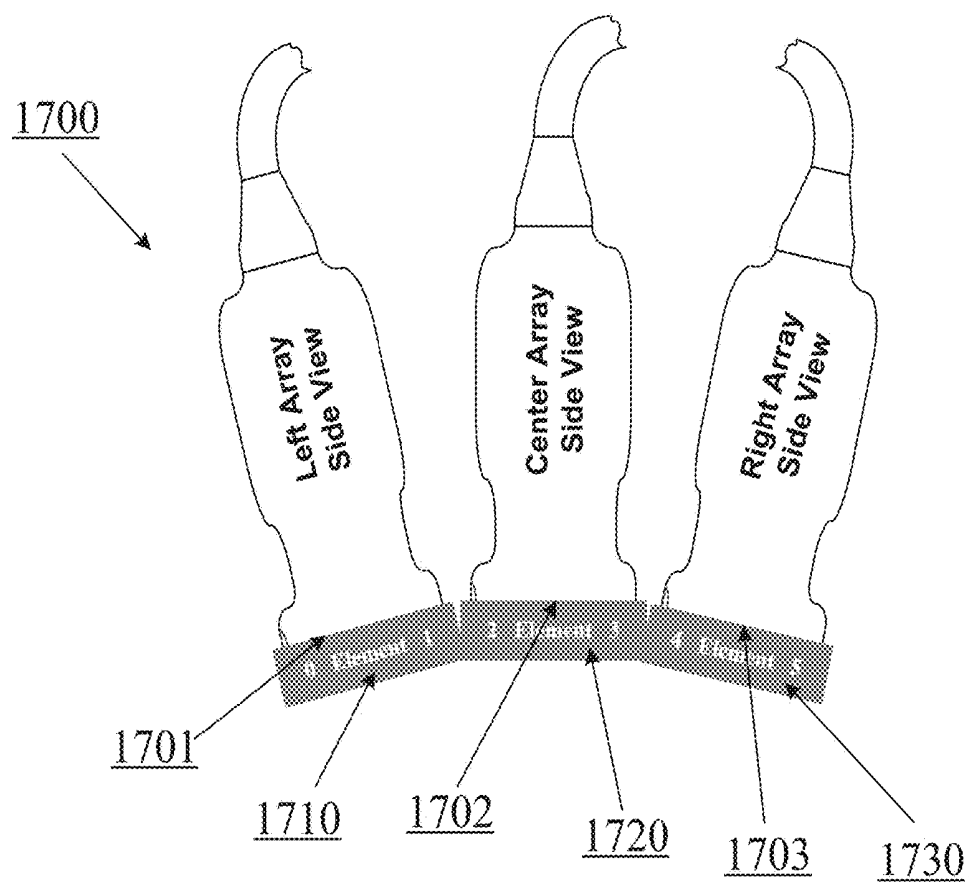


Fig. 16

Fig. 17



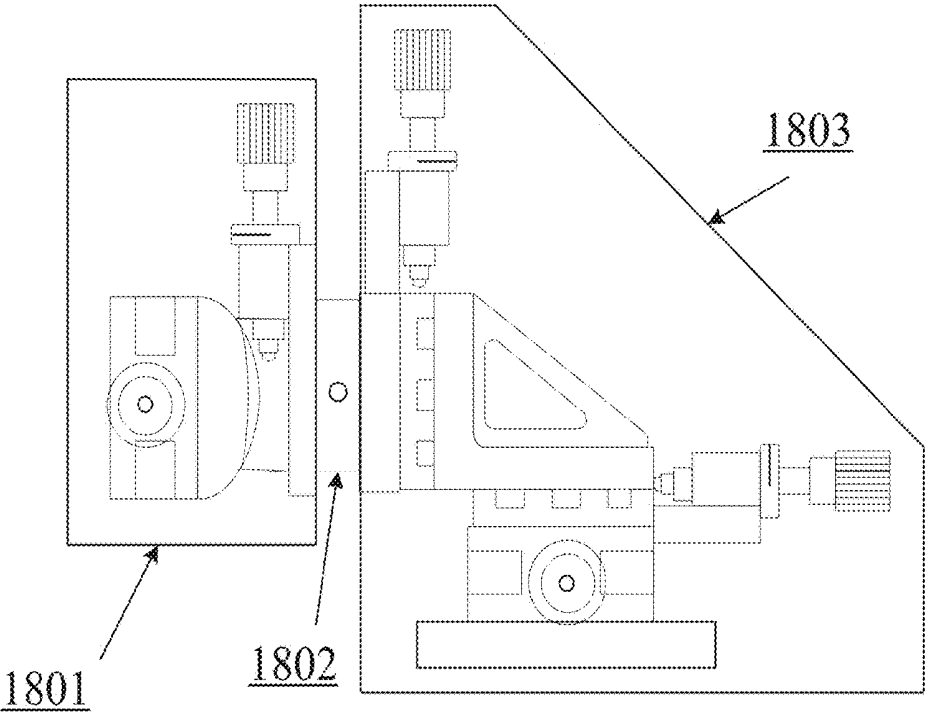


Fig. 18A

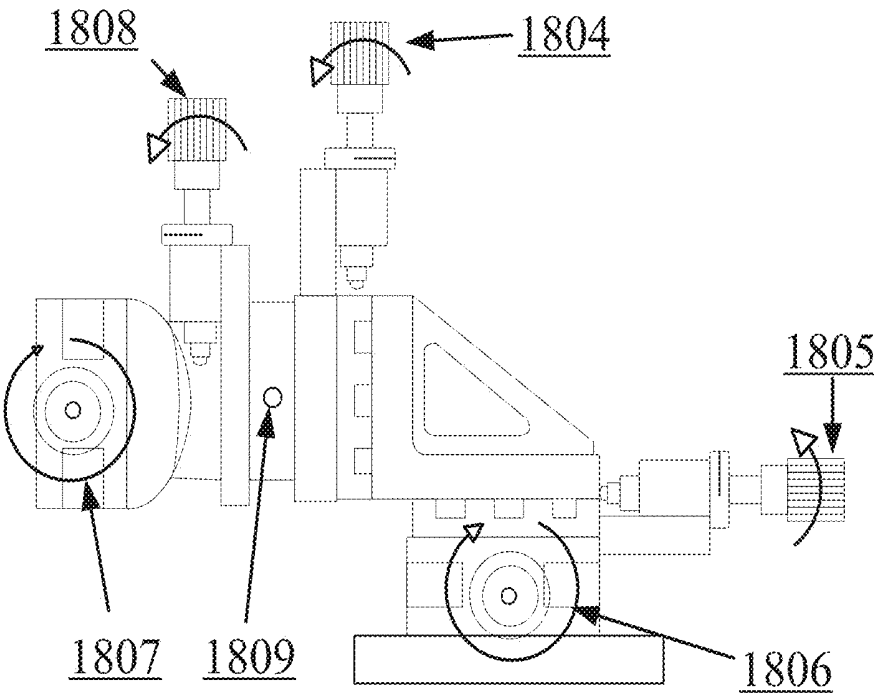


Fig. 18B

Fig. 19A



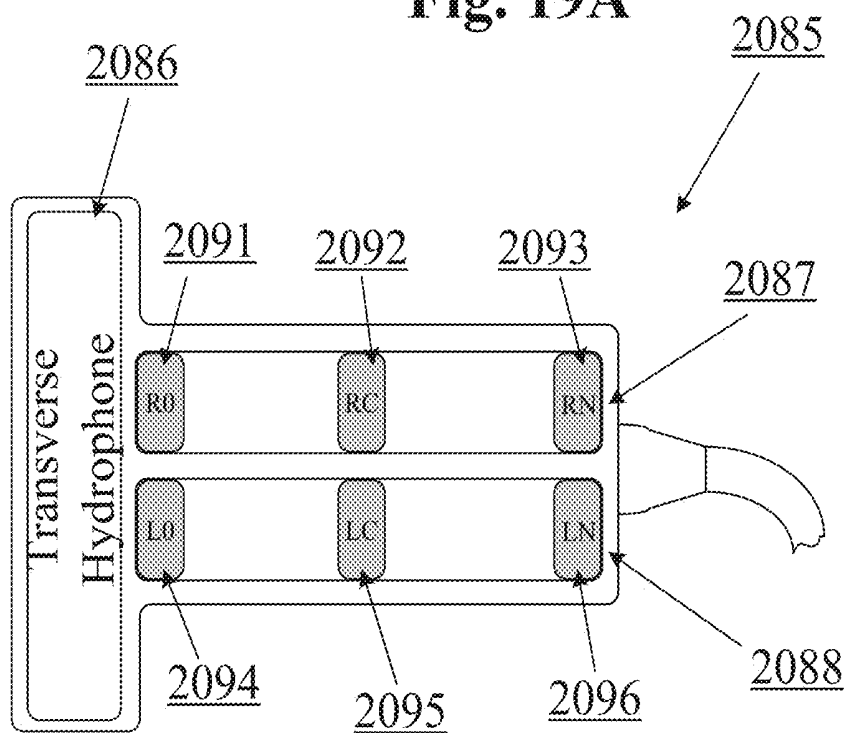


Fig. 19B

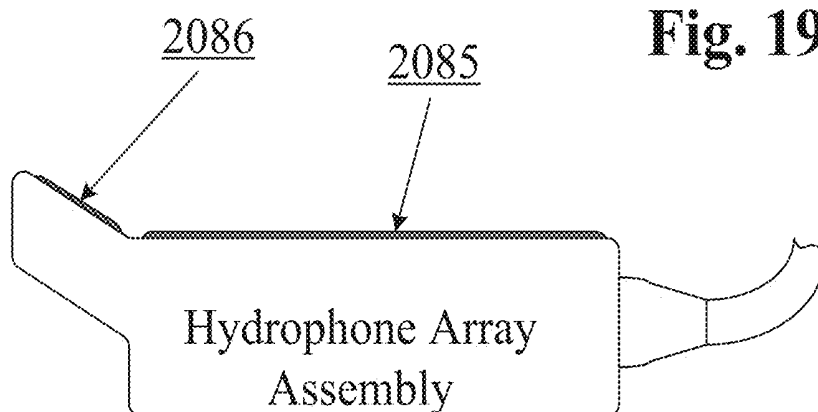

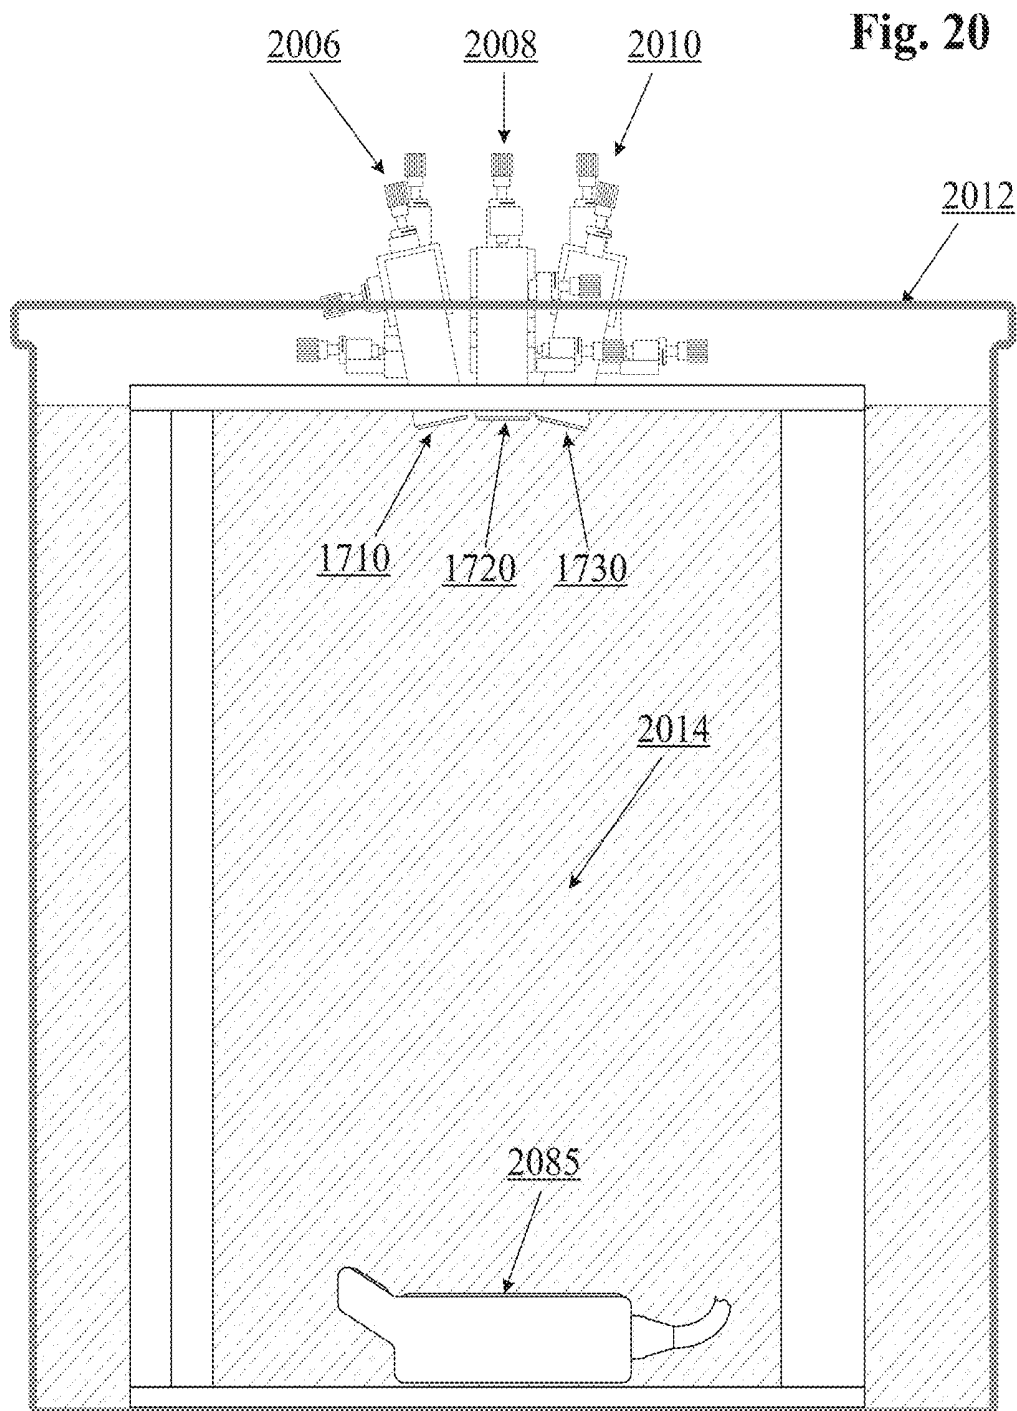

Assembled test fixture in tank.

Fig. 21A


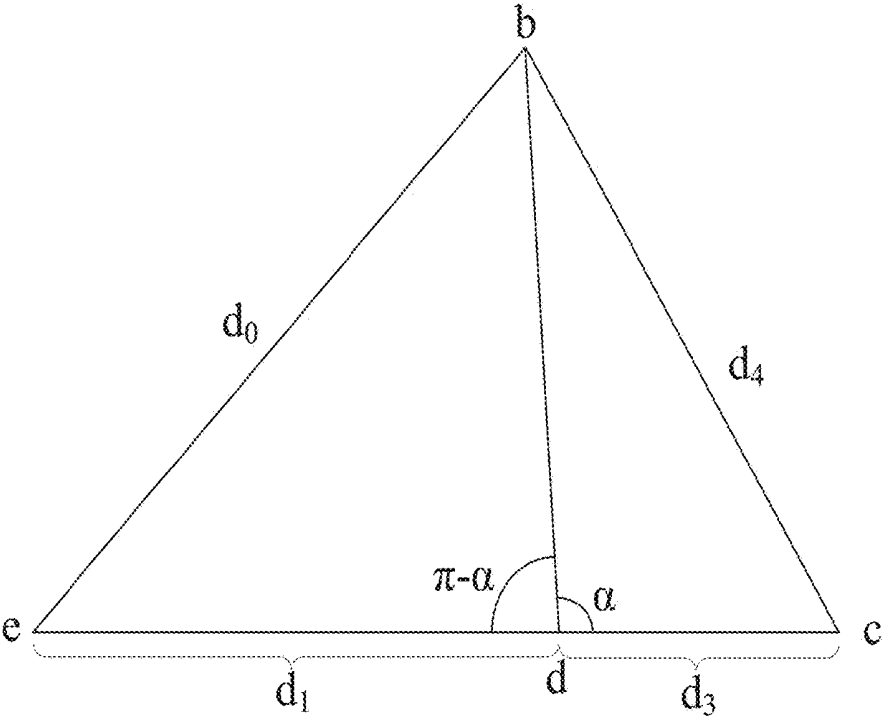


Fig. 21B

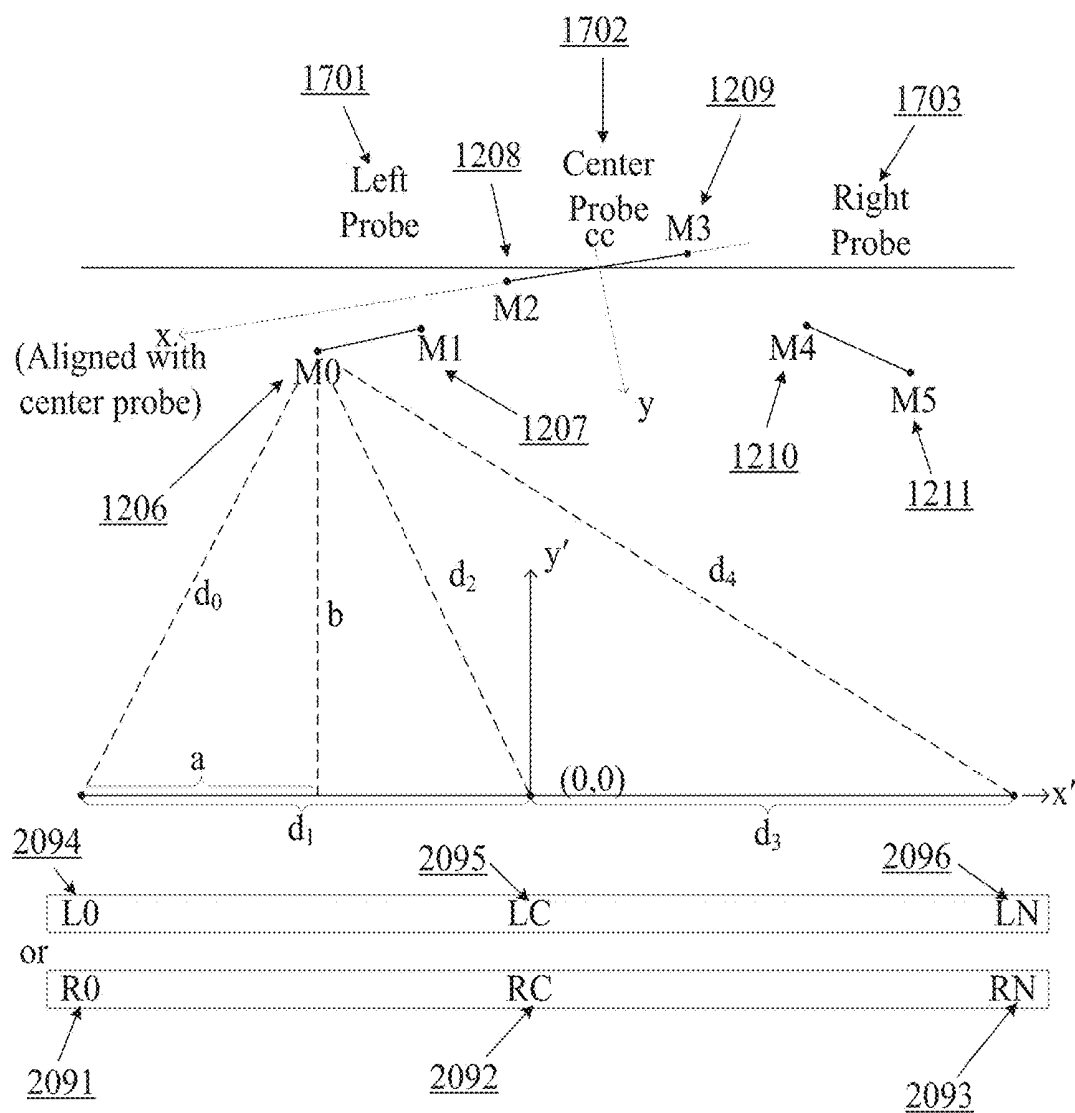

First reference is LC or RC

Final reference is center of center probe (cc)

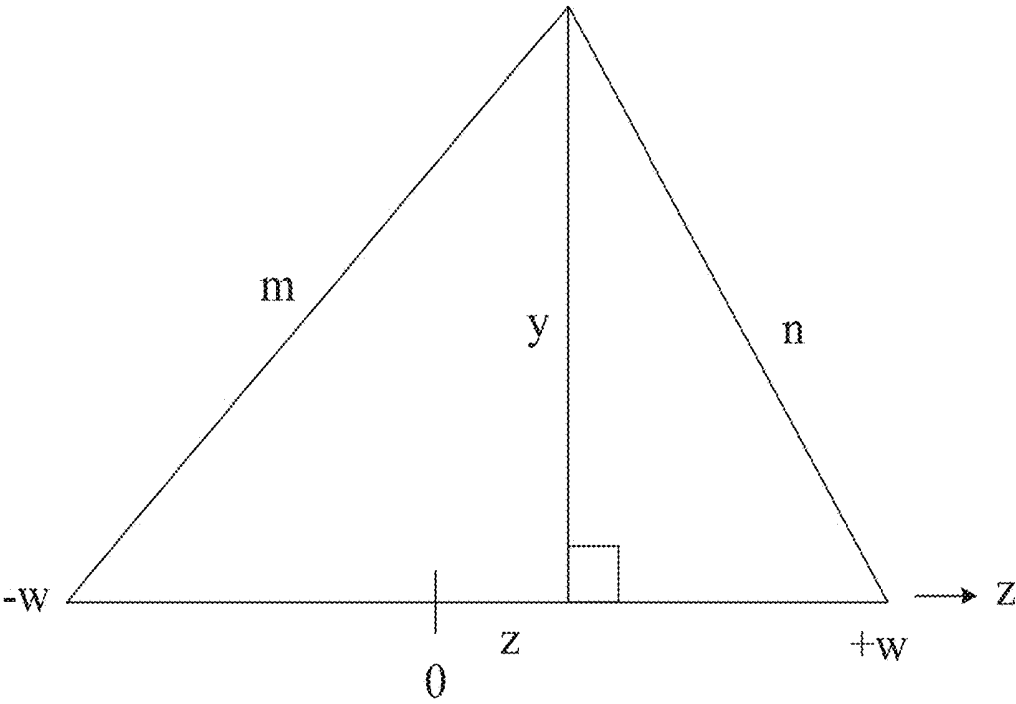


Fig. 21C

Fig. 22

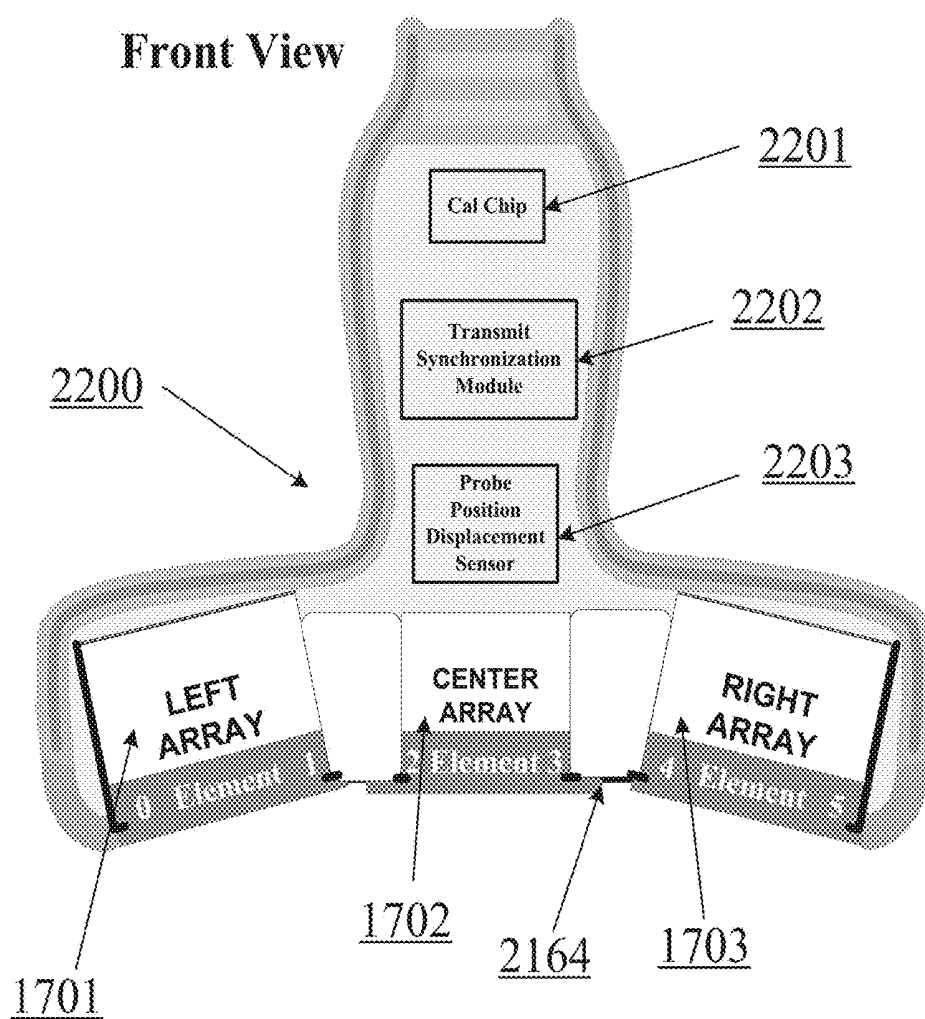


Fig. 23A

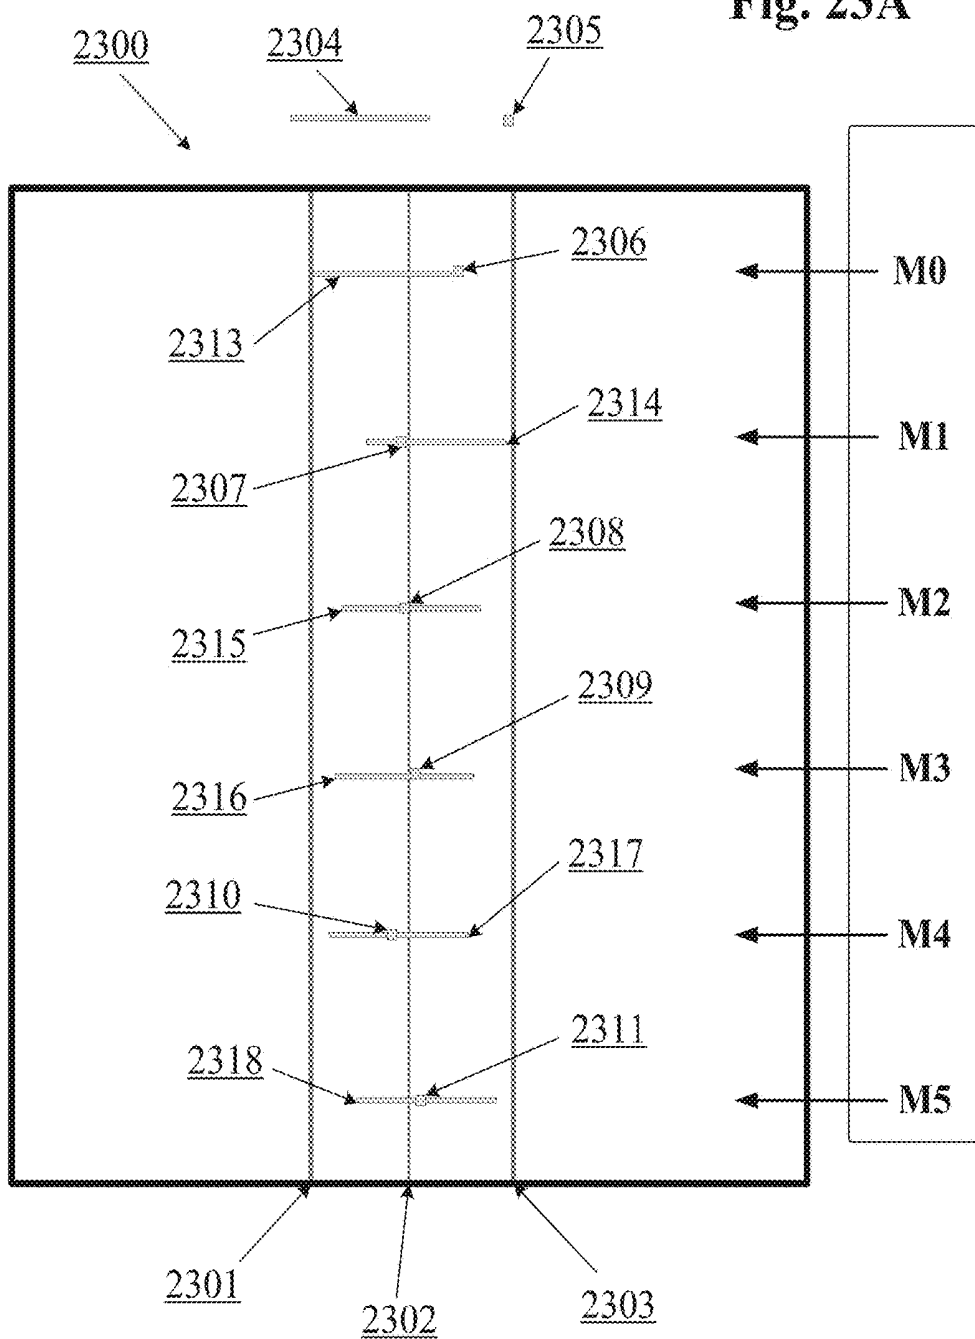


Fig. 23B

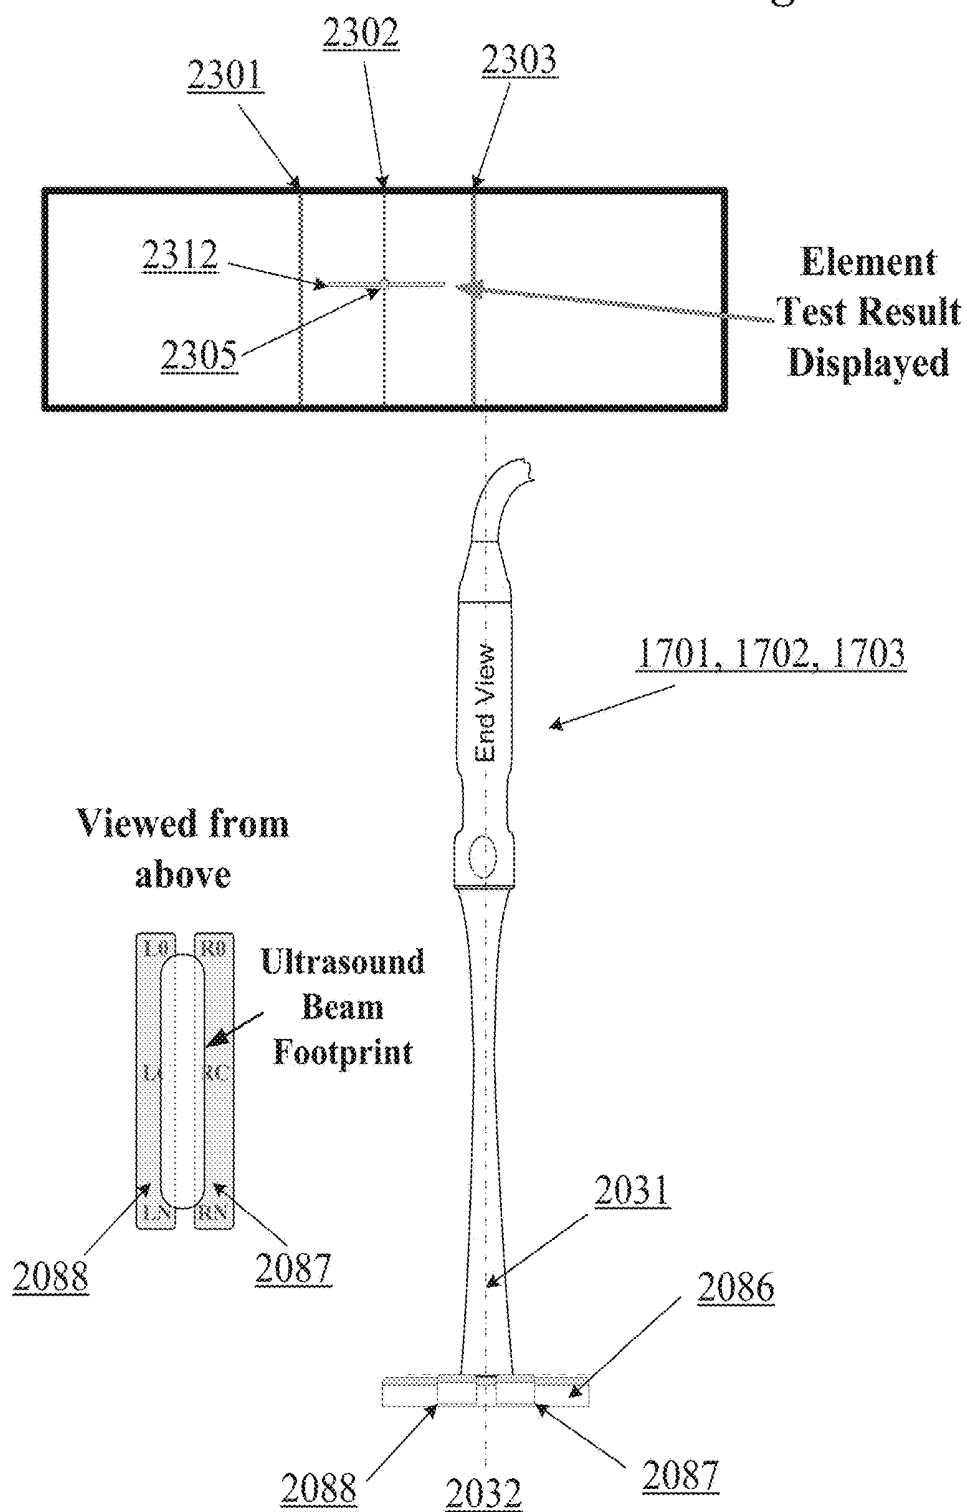


Fig. 23C

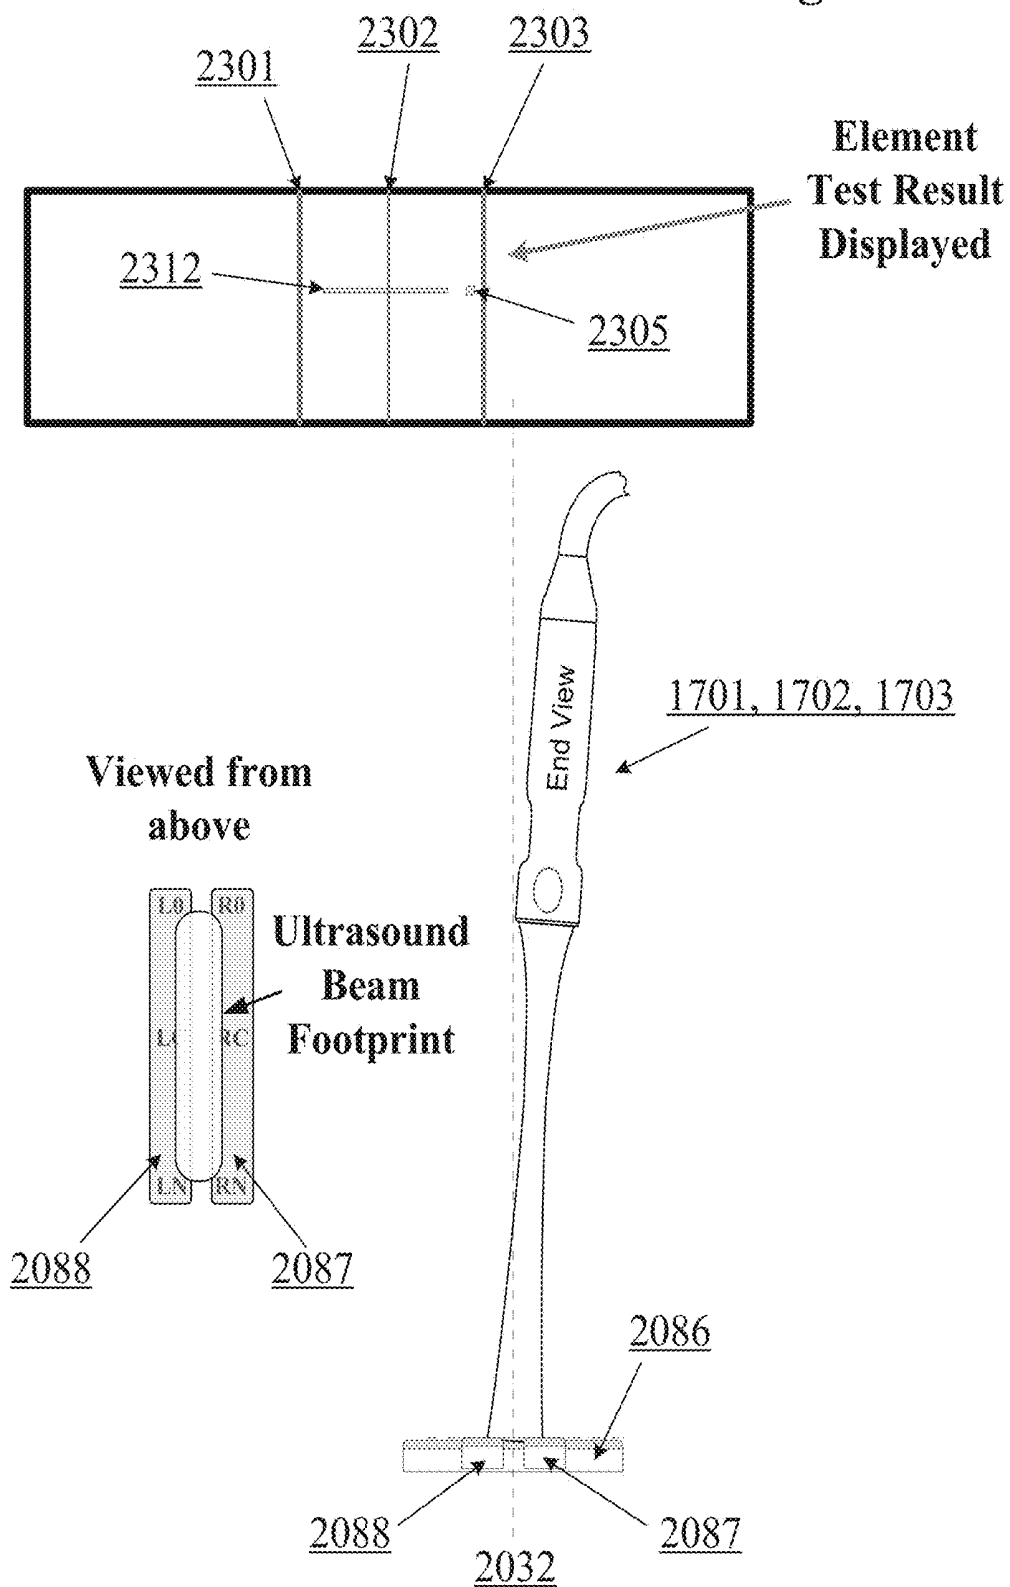


Fig. 23D

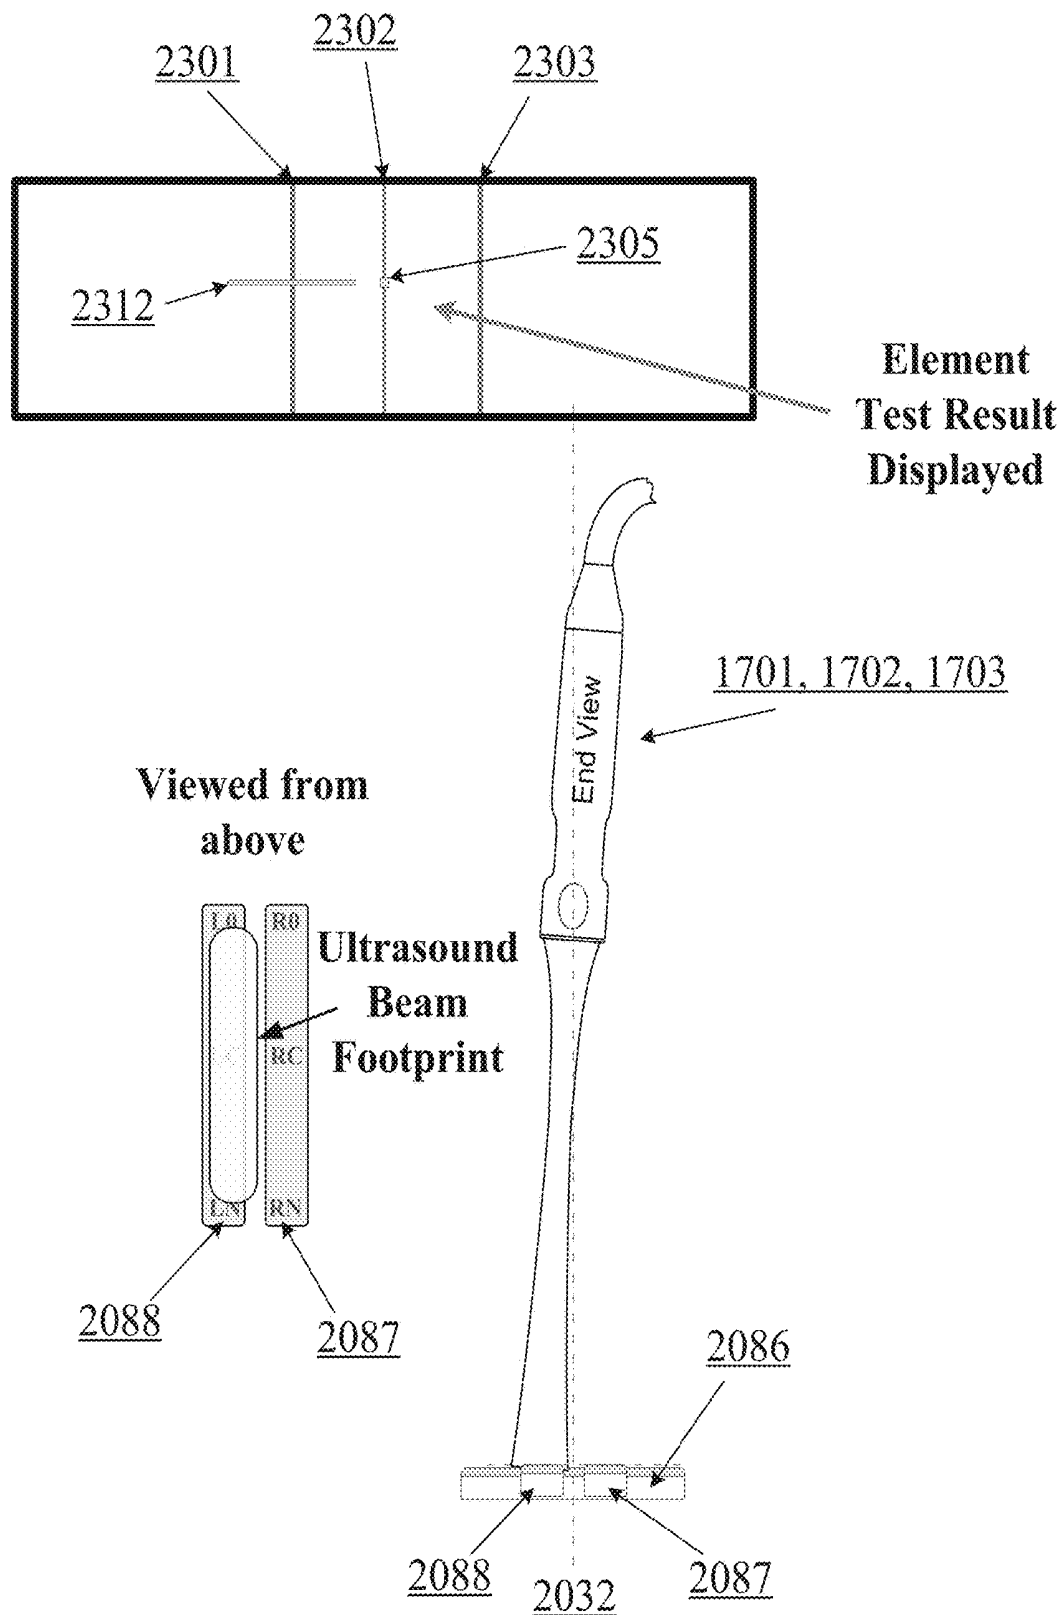


Fig. 24

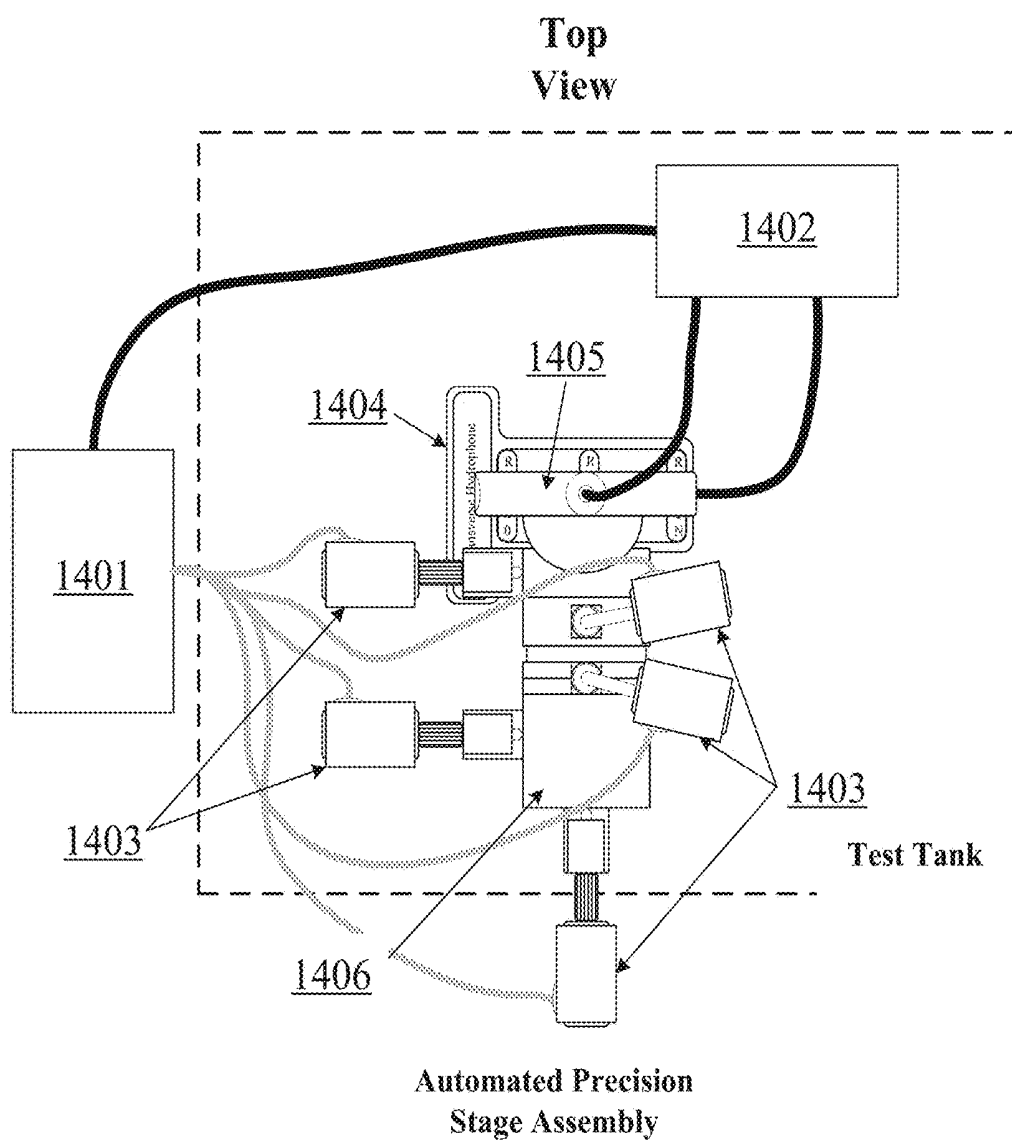
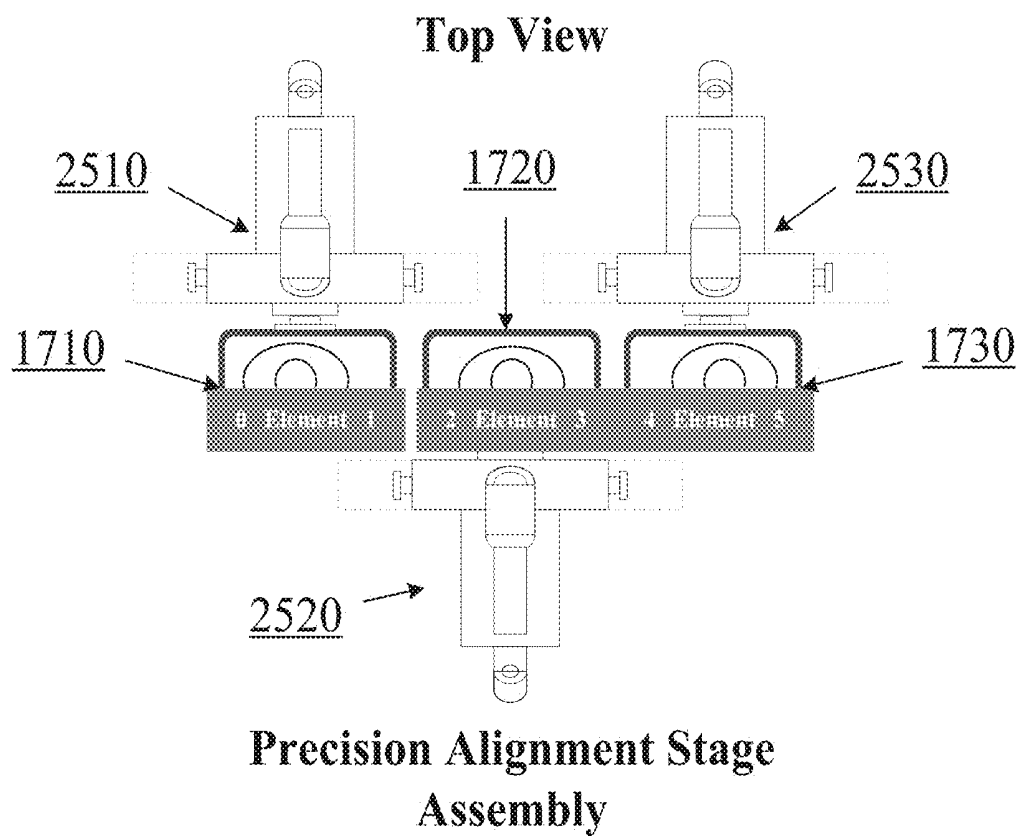


Fig. 25



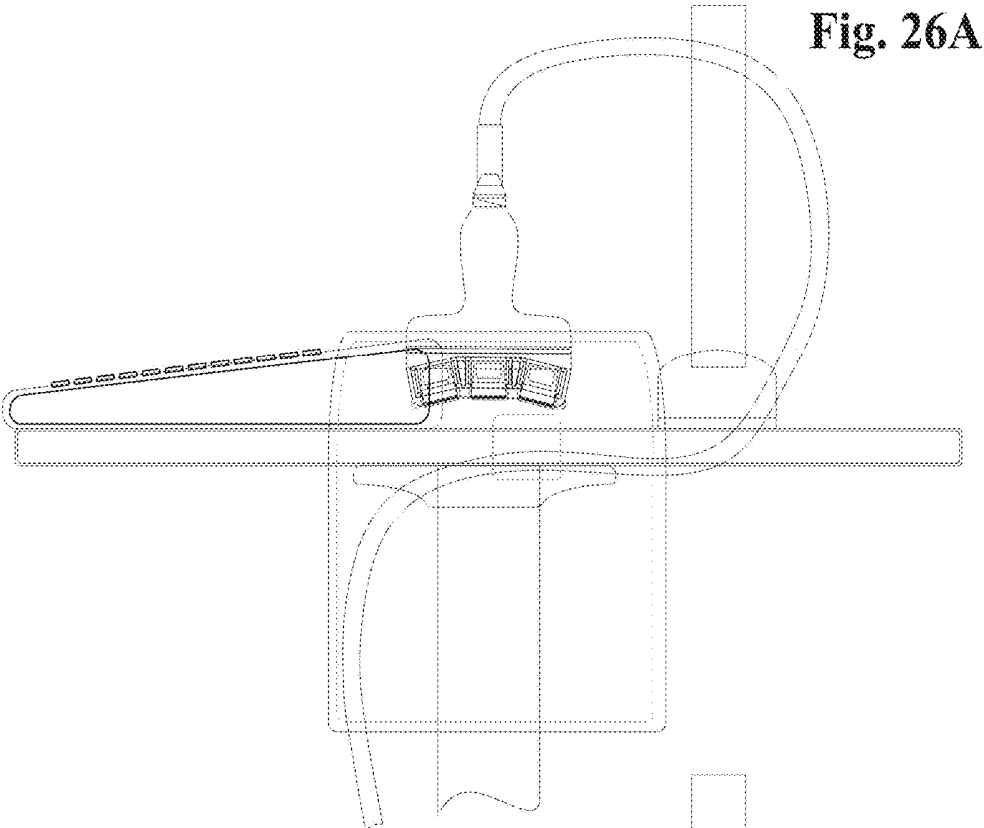


Fig. 26A

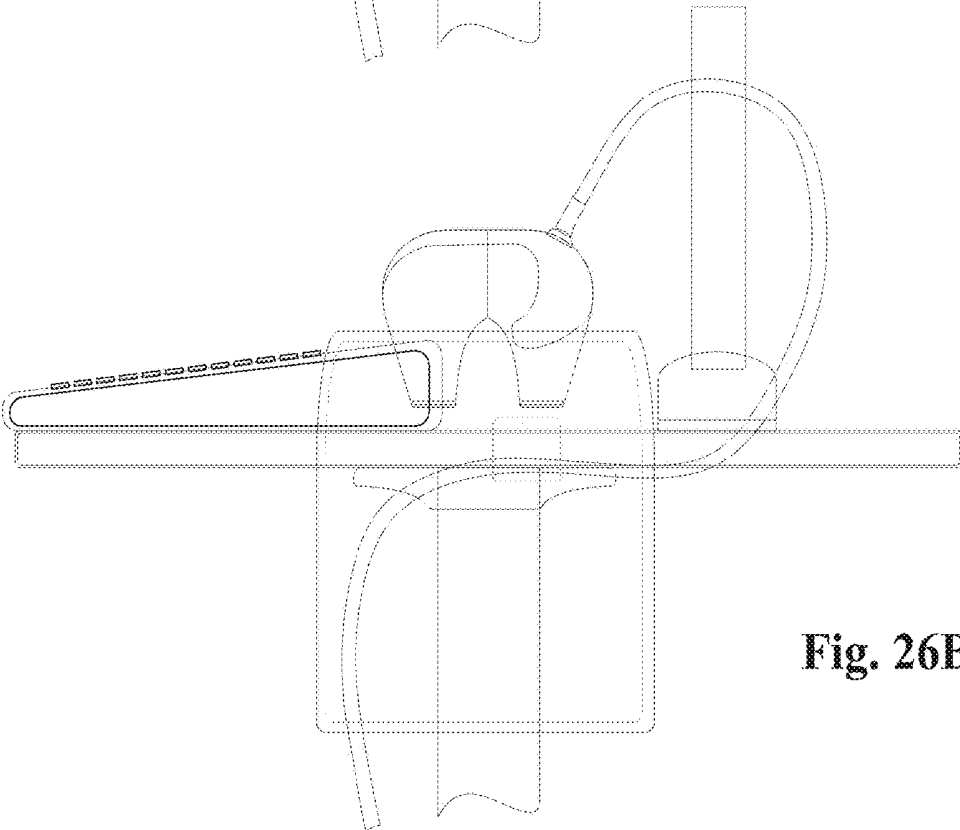


Fig. 26B

Fig. 27A

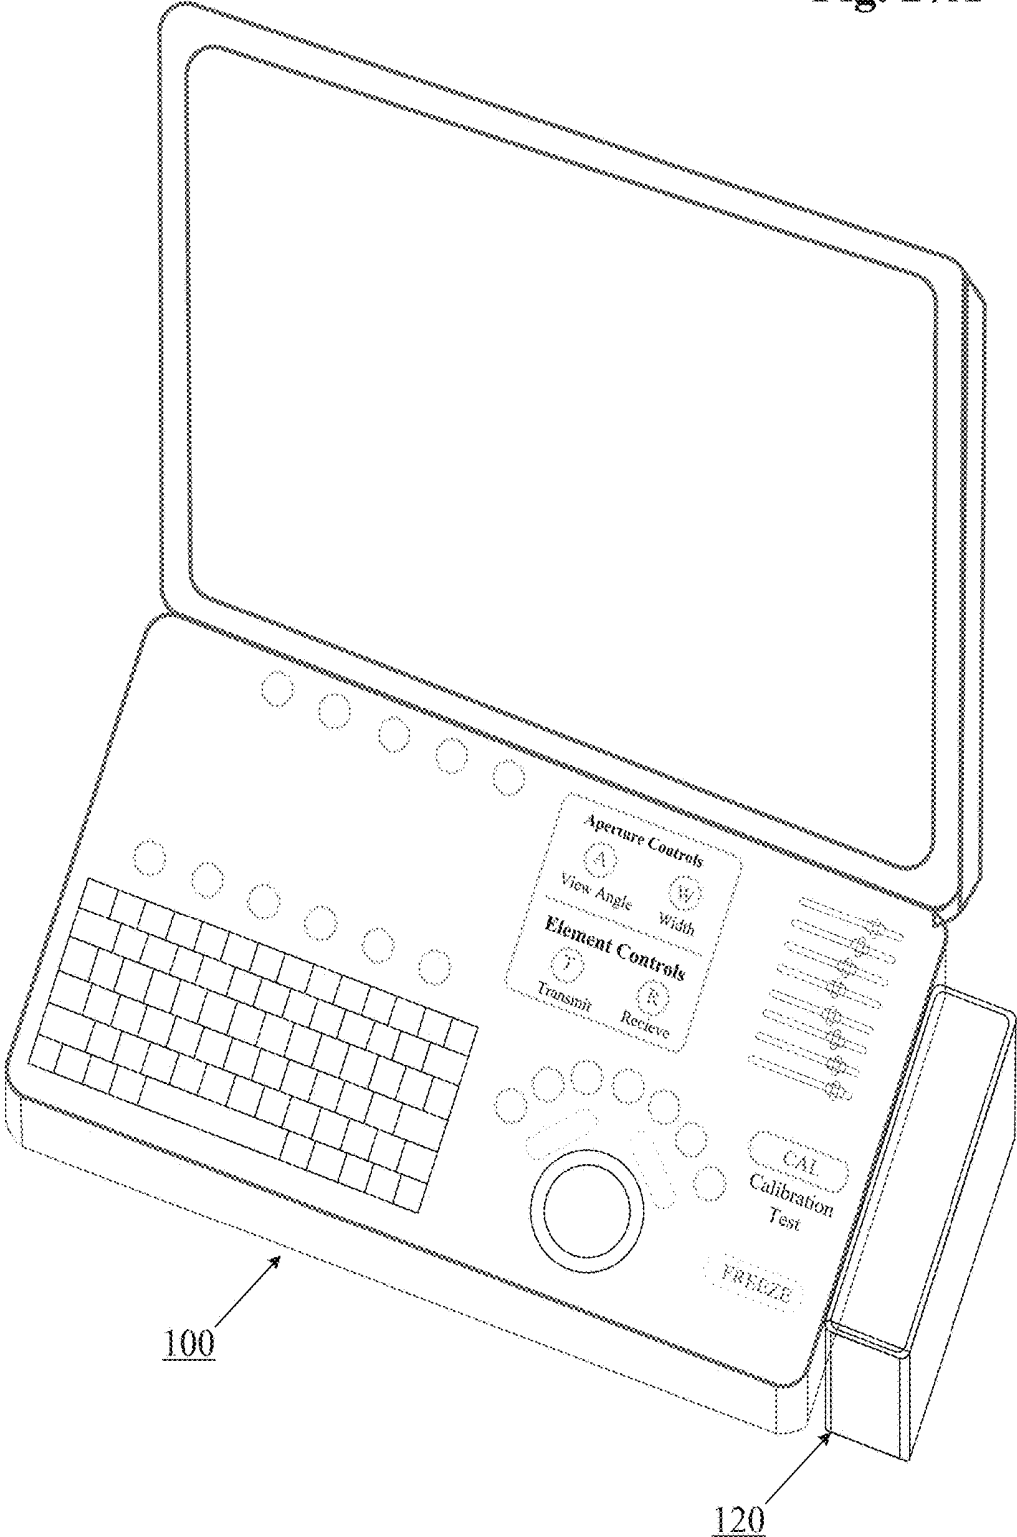
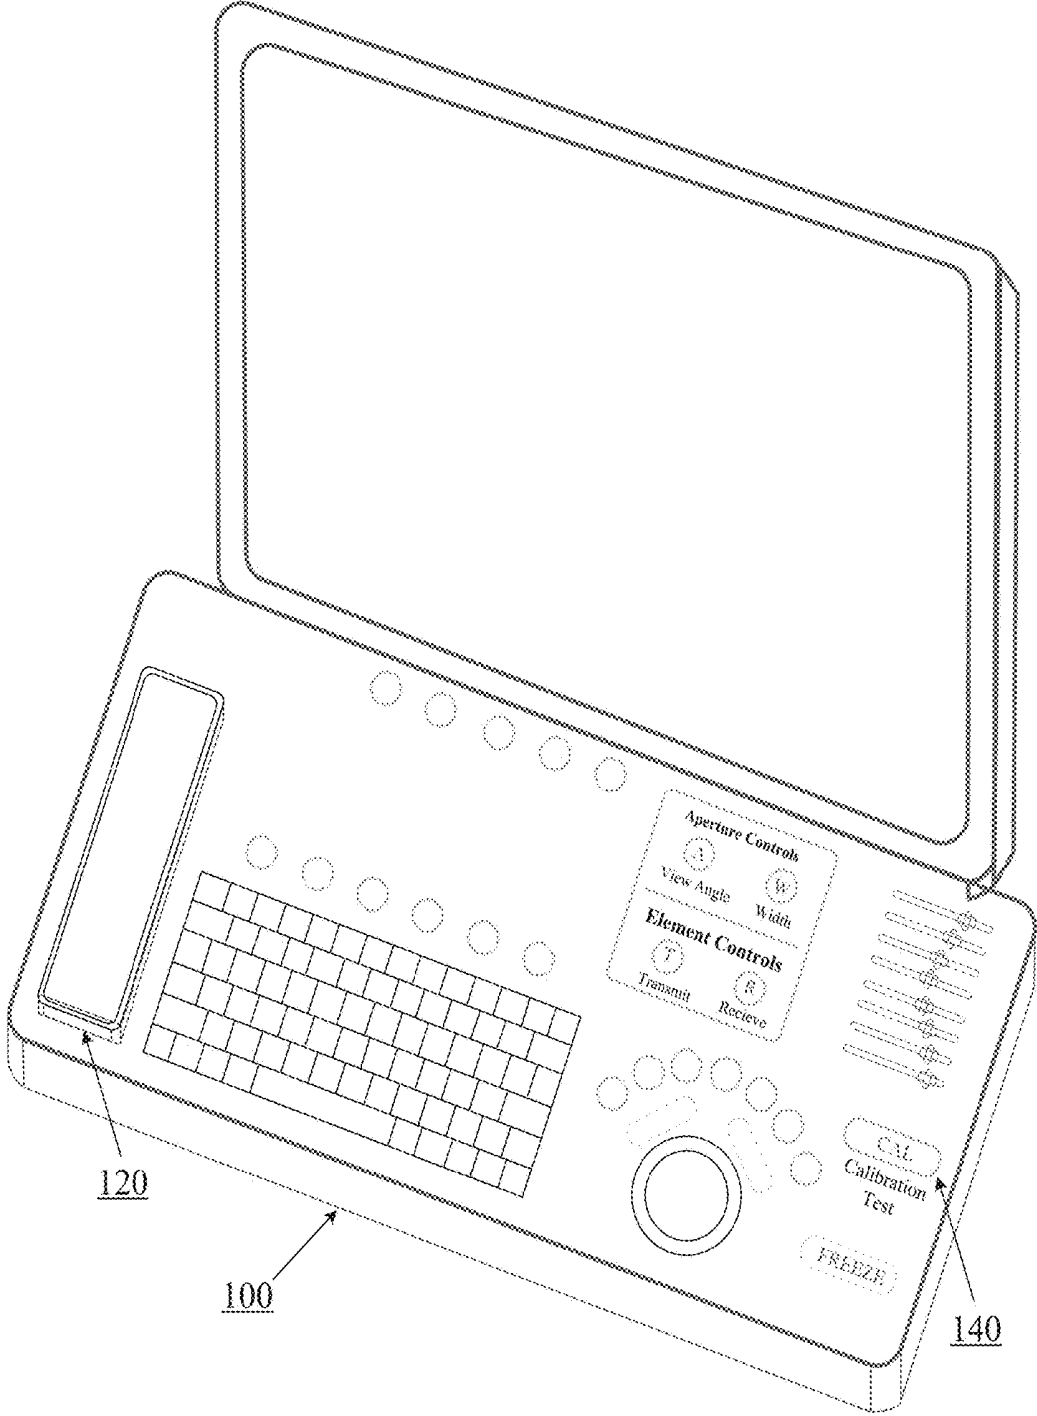
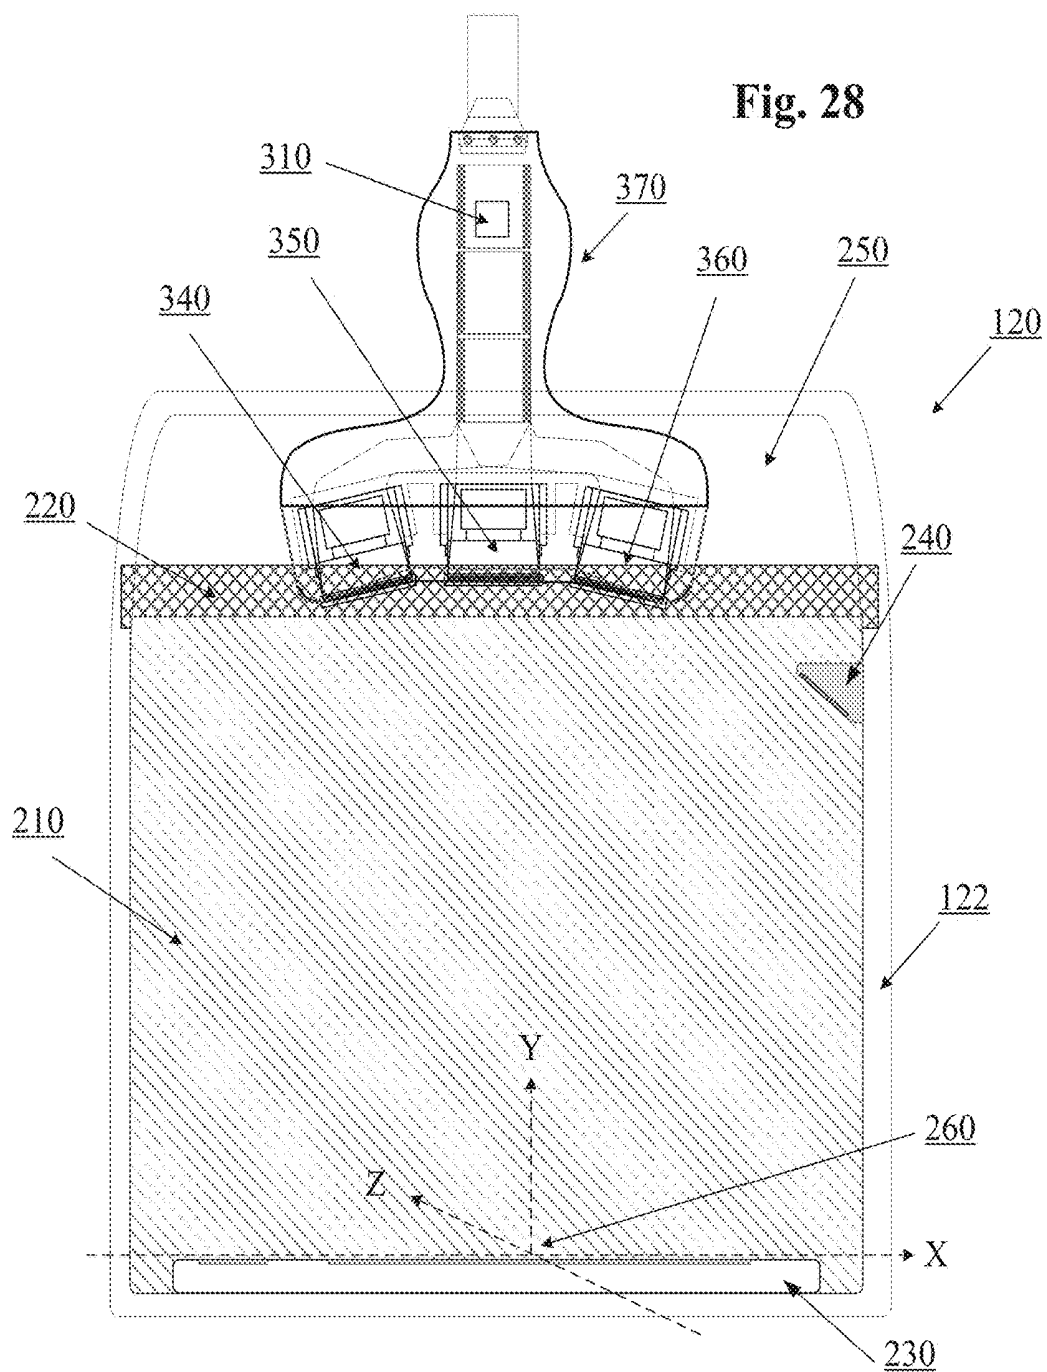


Fig. 27B





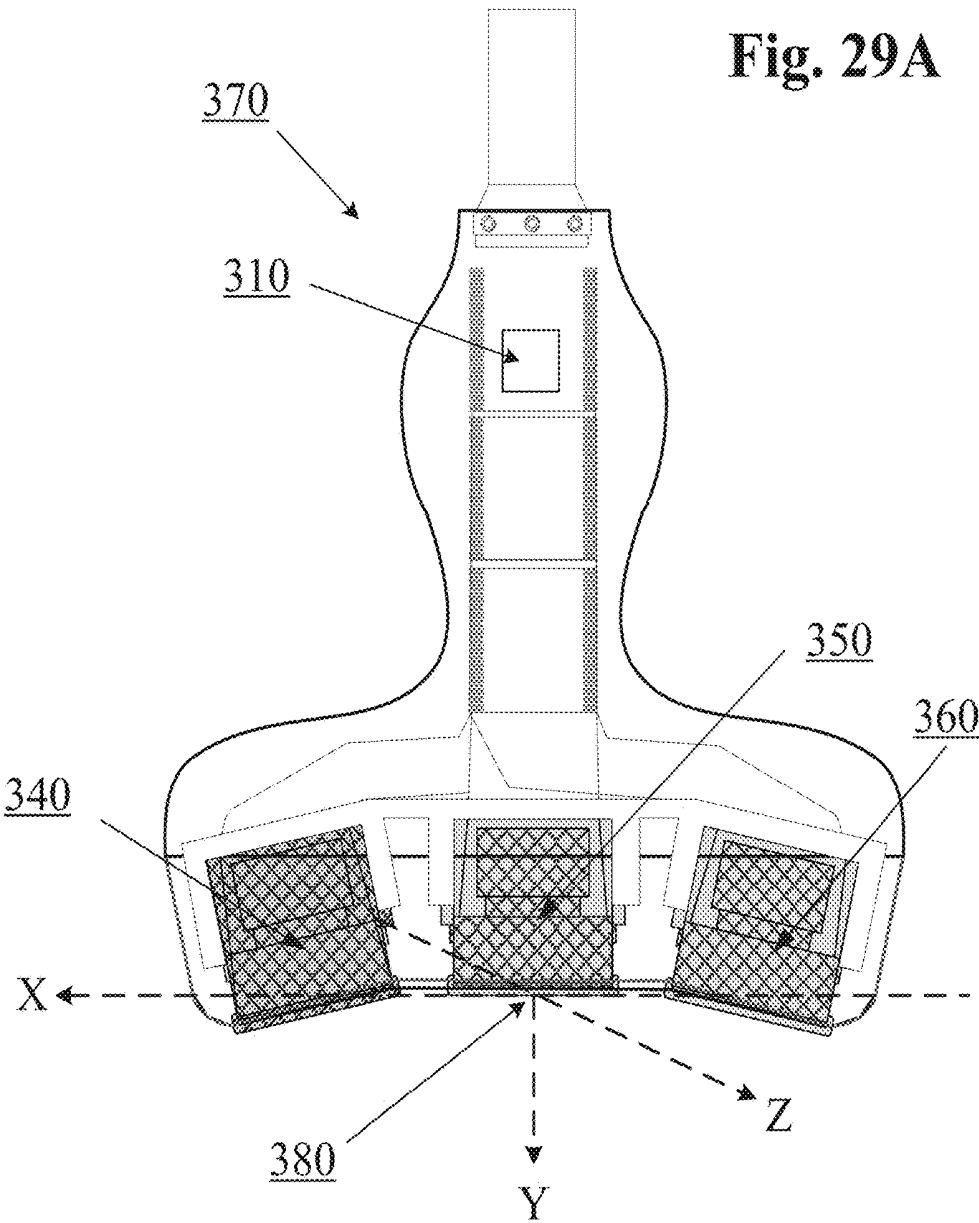
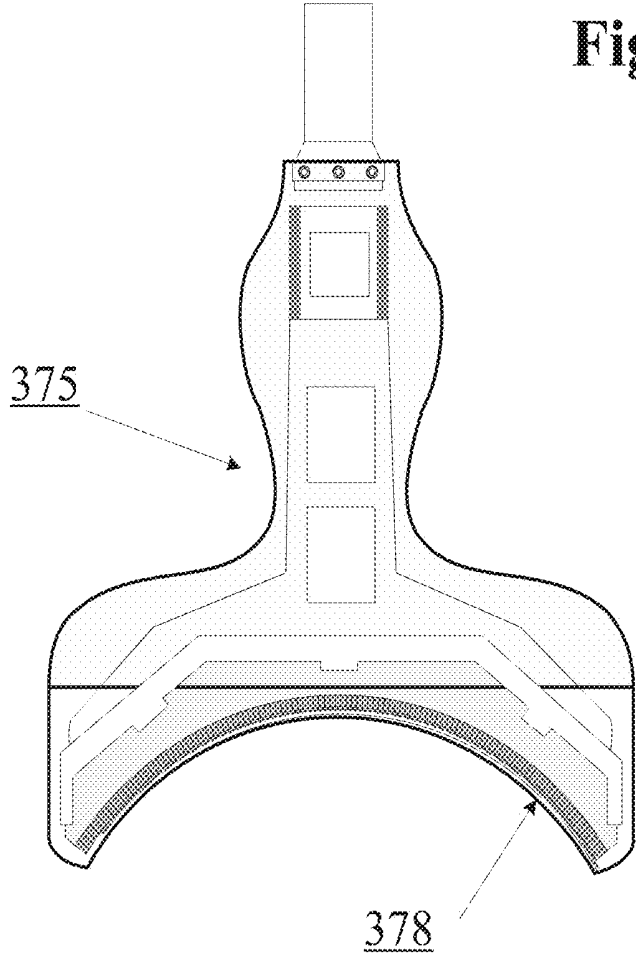
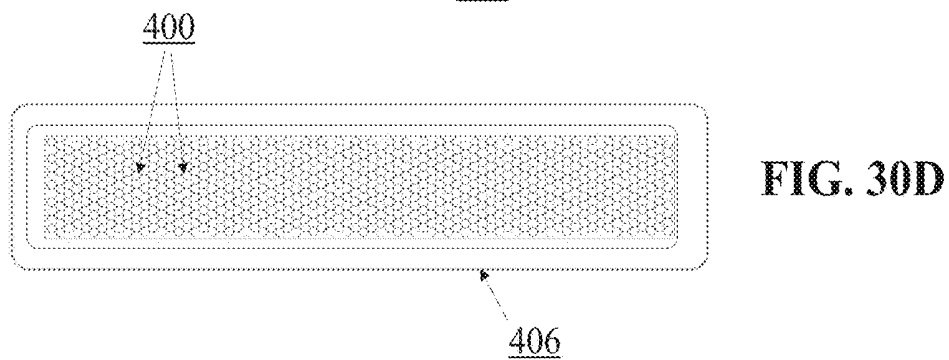
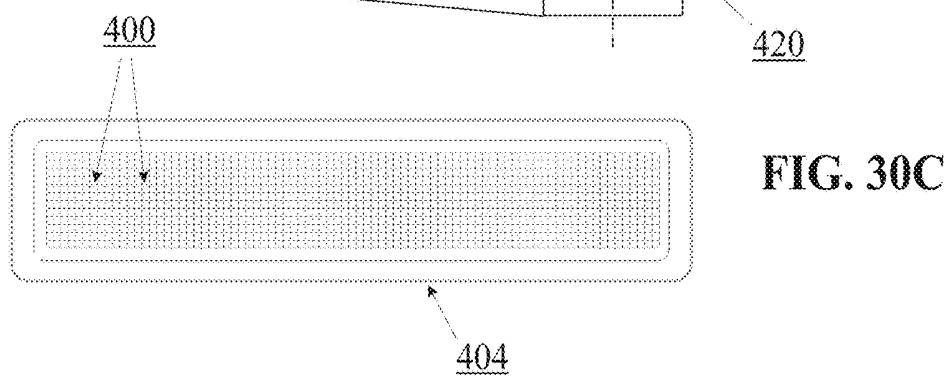
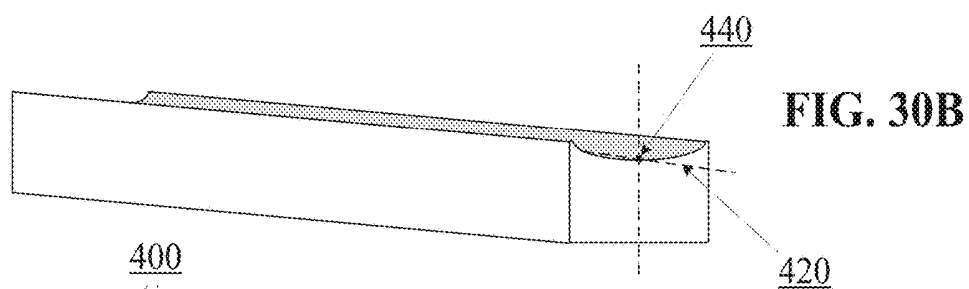
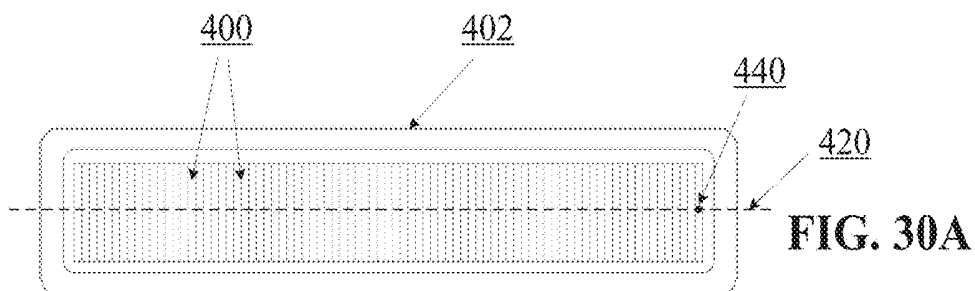
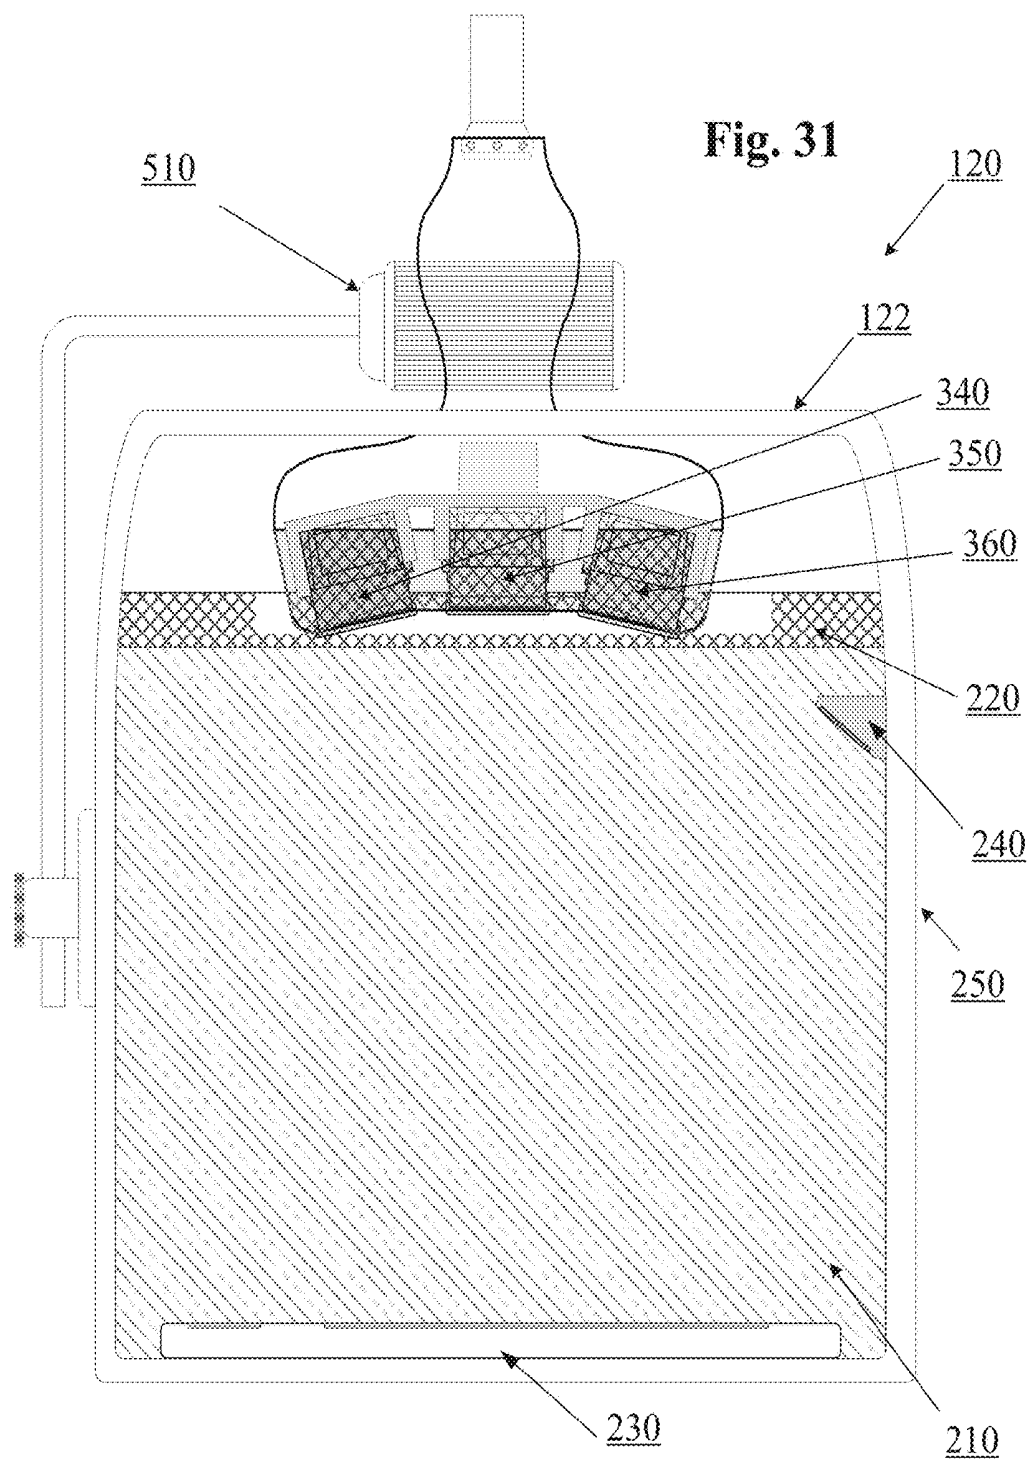


Fig. 29B







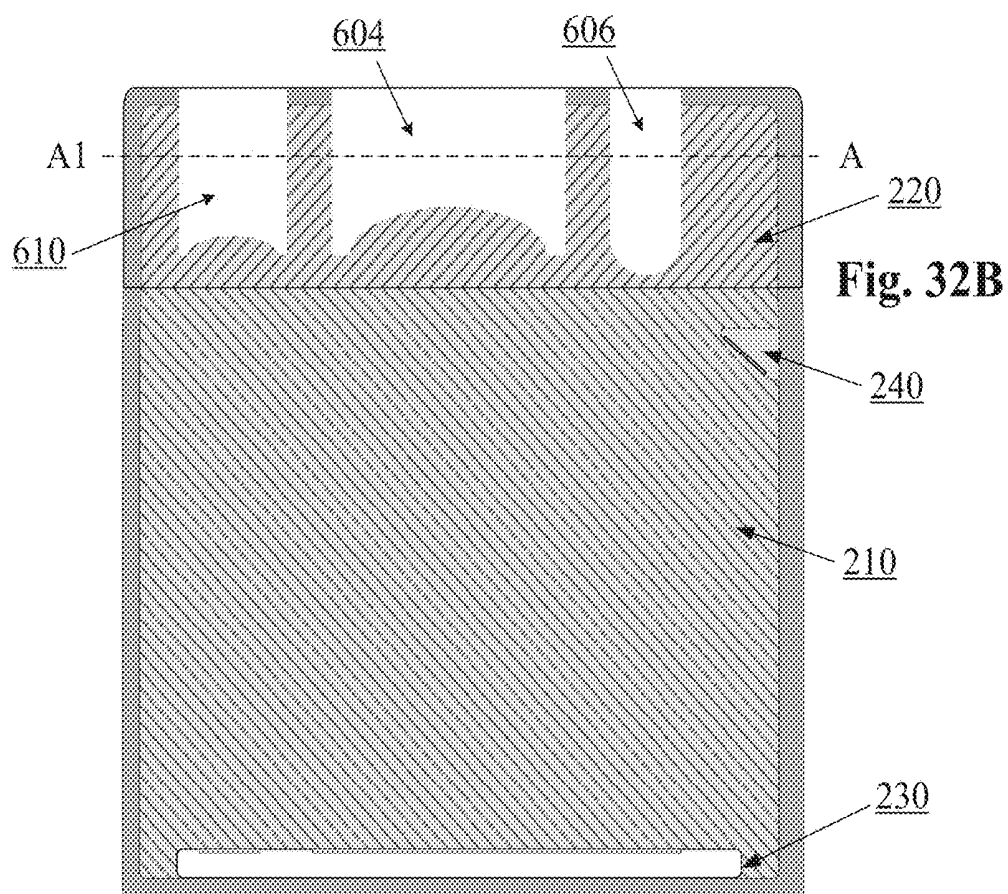
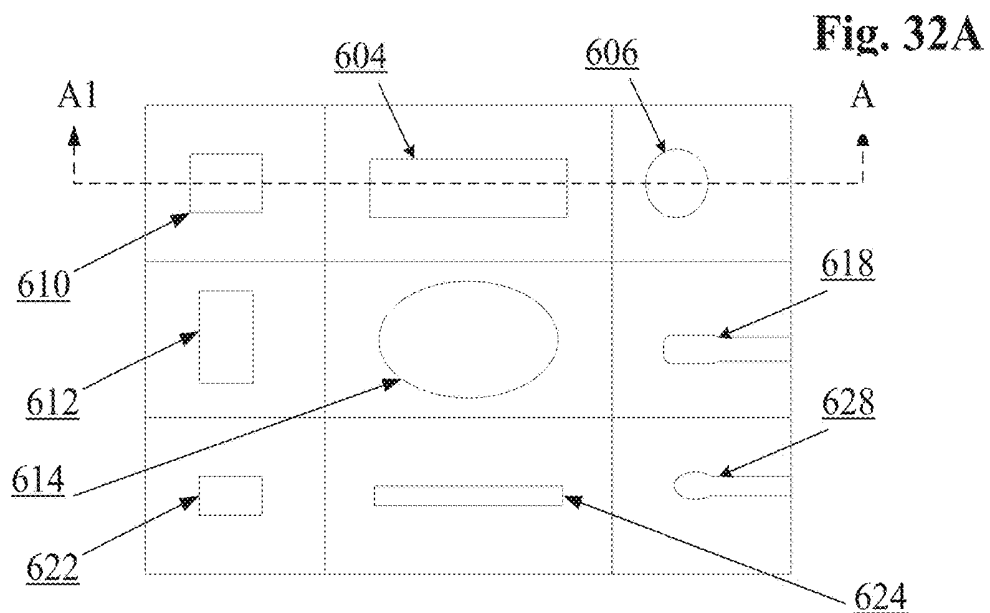


Fig. 33A

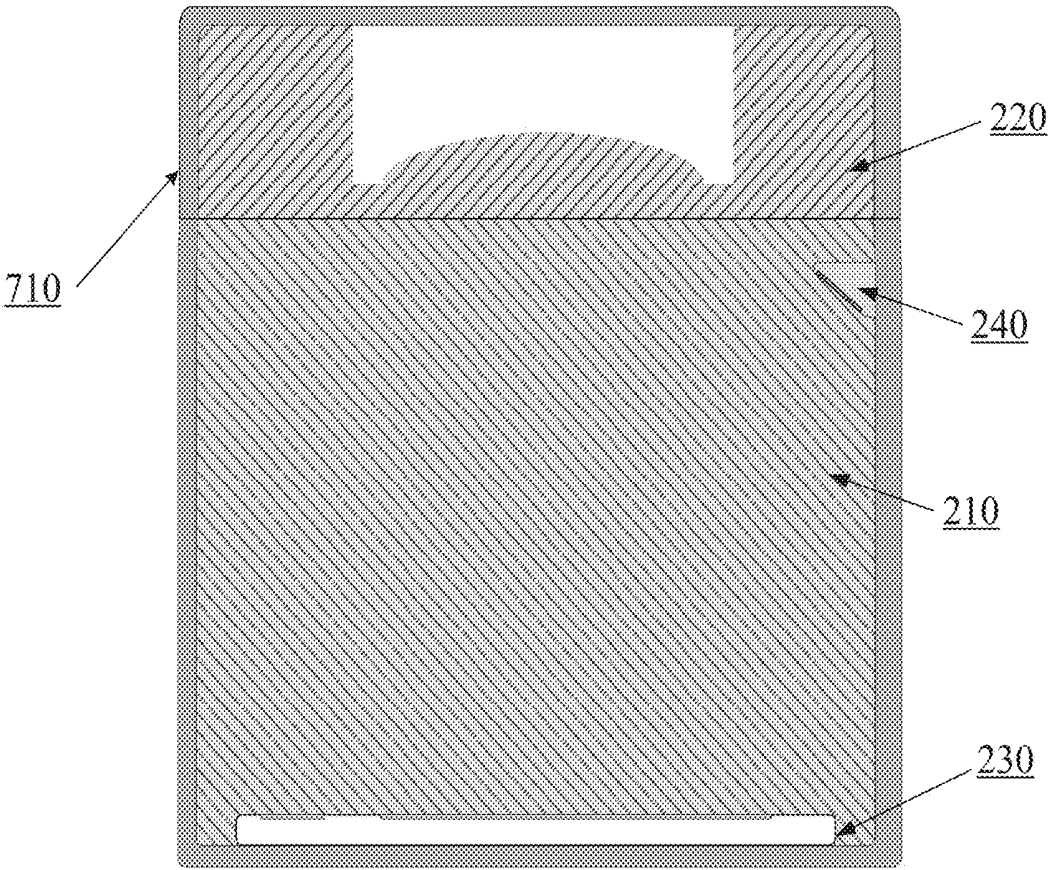


Fig. 33B

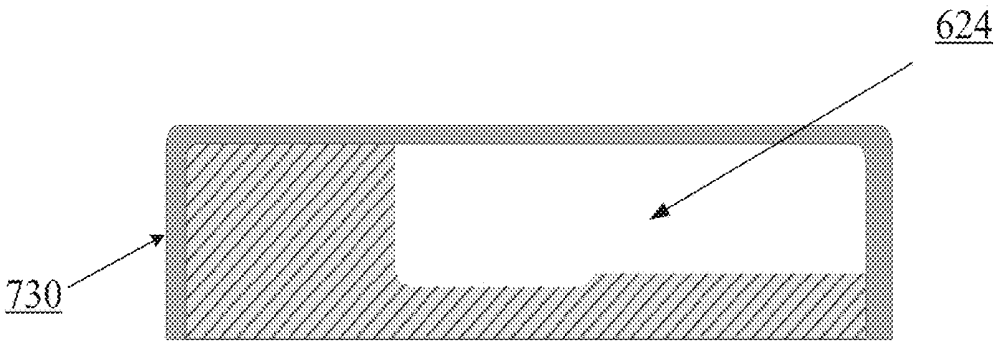
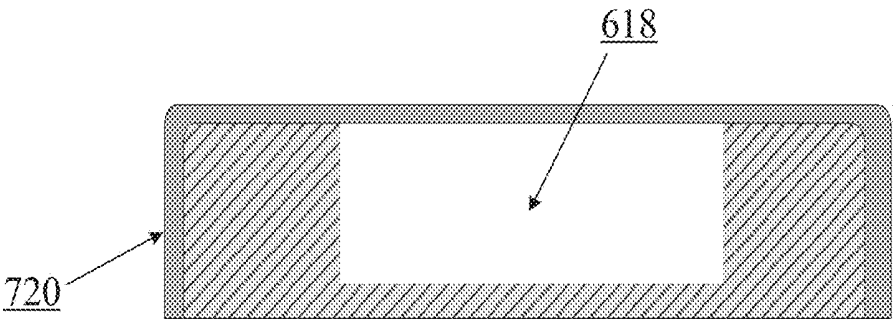
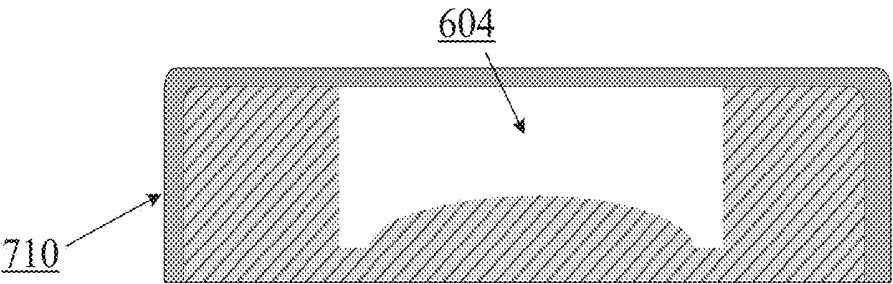


Fig. 34A


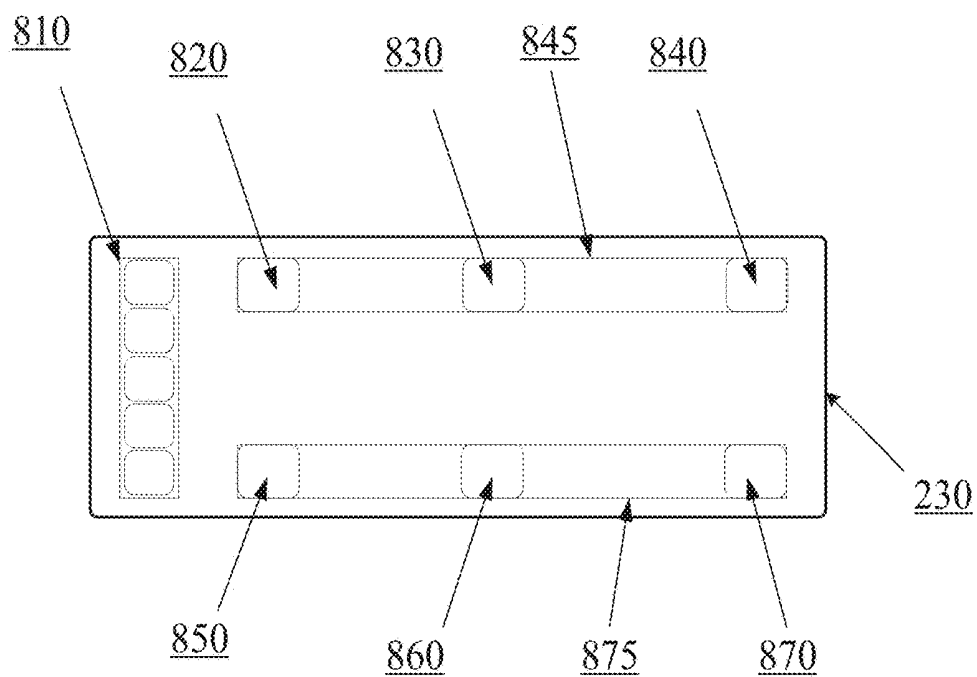


Fig. 34B

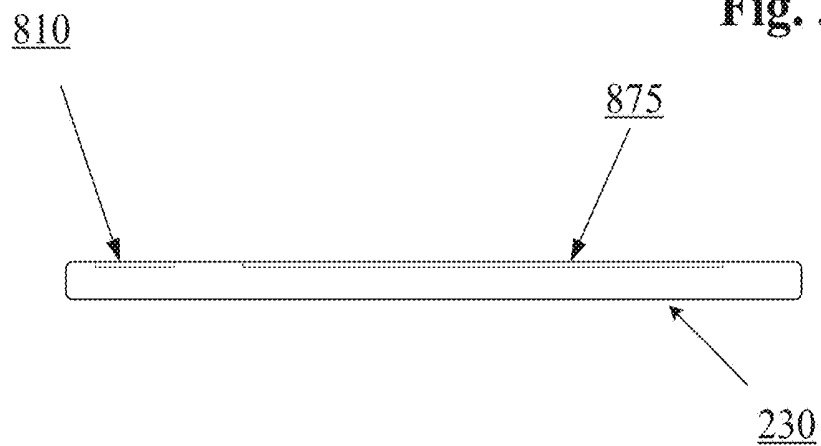

CALIBRATION OF ULTRASOUND PROBES

CROSS REFERENCE TO RELATED APPLICATIONS

[0001] This is a continuation of U.S. patent application Ser. No. 15/044,932, filed Feb. 16, 2016, now U.S. Pat. No. 10,206,662, which is a continuation of U.S. patent application Ser. No. 13/279,110, filed Oct. 21, 2011, now U.S. Pat. No. 9,282,945, which is a continuation-in-part of U.S. patent application Ser. No. 12/760,327, filed Apr. 14, 2010, now U.S. Pat. No. 8,473,239, which claims the benefit of U.S. Provisional Patent Application No. 61/169,200, filed Apr. 14, 2009, titled “Alignment and Fixturing of the Universal Multiple Aperture Medical Ultrasound Transducer”. All of the above referenced patents and applications are incorporated herein by reference in their entireties.

[0002] This application is relevant to Applicant’s co-owned patent applications including U.S. patent application Ser. No. 12/760,375, filed Apr. 14, 2010, titled “Universal Multiple Aperture Medical Ultrasound Probe”, published Oct. 14, 2010 as U.S. Patent Publication No. 2010-0262013, and U.S. Provisional Patent Application No. 61/392,896, filed Oct. 13, 2010, titled “Multiple Aperture Medical Ultrasound Transducers.” All of the above referenced patents and applications are incorporated herein by reference in their entireties.

INCORPORATION BY REFERENCE

[0003] Unless otherwise specified herein, all patents, publications and patent applications mentioned in this specification are herein incorporated by reference to the same extent as if each individual publication or patent application was specifically and individually indicated to be incorporated by reference.

FIELD

[0004] The present invention relates generally to imaging techniques, and more particularly to ultrasound imaging, and still more particularly to systems and methods for calibration and quality assurance measurement of ultrasound probes, particularly probes having multiple apertures.

BACKGROUND

[0005] In conventional ultrasonic imaging, a focused beam of ultrasound energy is transmitted into body tissues to be examined and the returned echoes are detected and plotted to form an image. While ultrasound has been used extensively for diagnostic purposes, conventional ultrasound has been greatly limited by depth of scanning, speckle noise, poor lateral resolution, obscured tissues and other such problems.

[0006] Significant improvements have been made in the field of ultrasound imaging with the creation of multiple aperture imaging, examples of which are shown and described in Applicant’s U.S. Pat. No. 8,007,439 issued Aug. 30, 2011 and titled “Method and Apparatus to Produce Ultrasonic Images Using Multiple Apertures”; U.S. Pat. No. 9,146,313 issued Sep. 29, 2015, titled “Point Source Transmission and Speed-Of-Sound Correction Using Multiple-Aperture Ultrasound Imaging”; and U.S. patent application Ser. No. 12/760,375, filed Apr. 14, 2010, titled “Universal Multiple Aperture Medical Ultrasound Probe,” all three of which are incorporated herein by reference. Multiple aper-

ture imaging methods and systems allow for ultrasound signals to be both transmitted and received from separate apertures.

[0007] One problem with multiple aperture imaging is that it can be difficult to know the exact position of the elements of a large apparatus with multiple and separate physical points of contact (“footprints”) on the patient. It is desirable for each element position to be known to within $\frac{1}{10}$ wavelength (for example, 0.03 mm at 3 MHz). In contrast, with conventional ultrasound probes, regardless of array vertical displacement or integration (e.g., 1.5D or 2D), there has never been a need to solve alignment and position issues between multiple arrays or multiple individual elements. The calibration methods and apparatuses described herein teach how to solve these problems for Universal Multiple Aperture ultrasound probes.

SUMMARY

[0008] In general, in one aspect, a method of calibrating an ultrasound probe includes mounting an ultrasound probe onto a calibration system, transmitting an ultrasound test signal from an element of the probe through a test medium of the calibration system, receiving the test signal at a first hydrophone of the calibration system at a first time; receiving the test signal at a second hydrophone of the calibration system at a second time, receiving the test signal at a third hydrophone of the calibration system at a third time, and determining an acoustic position of the element based upon differences in the first time, the second time, and the third time.

[0009] This and other embodiments may include one or more of the following features.

[0010] The elements can be part of an array having a plurality of elements, and the method can further include repeating the transmitting, receiving, and determining steps for at least one additional element in the array. The transmitting, receiving, and determining steps can be performed for every element in the array. The transmitting, receiving, and determining steps can be performed for less than all of the elements in the array, and the method can further include interpolating acoustic positions of all remaining elements. The probe can include a plurality of distinct arrays, and the transmitting, receiving, and determining steps can be performed for at least two elements in each array. The plurality of arrays can be separated by physical space. At least one array can be non-planar with respect to another array.

[0011] The first, second, and third hydrophones can be part of a first line of hydrophones and fourth, fifth, and sixth hydrophones can be part of a second line that is parallel to the first line, and the method can further include receiving the test signal on all six hydrophones and determining an x, y, and z position of the element based on differences of arrival times at each hydrophone. Further, there can be a third line of two or more hydrophones that is transverse to the first and second lines, and the method can further include computing the angle of transmission of the element based upon the position of maximum levels of energy received on any of the hydrophones.

[0012] The method can further include storing the determine position of the element in a memory chip on the probe. The method can further include overwriting position data stored in a memory chip with the determined position.

[0013] The method can further include establishing a tank coordinate system relative to the first, second, or third

hydrophone. The method can further include determining a position of every element of the probe relative to the tank coordinate system. The method can further include establishing a probe coordinate system relative to an element of the probe. The method can further include rotating or translating all of the determined positions to the probe coordinate system. The position can be determined relative to a Cartesian coordinate system.

[0014] The method can further include storing the determined position in memory and retrieving the stored position during imaging or image processing.

[0015] The method can further include transmitting an ultrasound test signal from a fourth hydrophone to the first, second, or third hydrophone to verify the operation of the first, second, or third hydrophone.

[0016] In general, in one aspect, a method of determining functionality of an ultrasound probe can include mounting an ultrasound probe onto a calibration system, transmitting an ultrasound signal between a hydrophone of the calibration system and an element of the probe, the transmitting occurring through test medium of the calibration system; and determining an acoustic performance of the element.

[0017] This and other embodiments can include one or more of the following features.

[0018] The test signal can be transmitted from the hydrophone and received by the element. The test signal can be transmitted from the element and received by the hydrophone.

[0019] The element can be part of an array having a plurality of elements, and the method can further include repeating the transmitting, receiving, and determining steps for at least one additional element in the array. The probe can include a plurality of distinct arrays, and the transmitting, receiving, and determining steps can be performed for at least one element of each array.

[0020] The test signal can be transmitted by the first, second, or third hydrophone and received by a fourth hydrophone to verify signal performance.

[0021] The determined acoustic performance can be stored and transmitted electronically to report probe performance to service providers and end users.

[0022] In general, in one aspect, a system for calibrating an ultrasound probe includes a tank substantially filled with a test medium, a dock attached to the tank, and a plurality of hydrophones. The dock is configured to hold an ultrasound probe. The plurality of hydrophones are arranged in a matrix along a wall of the tank opposite the dock.

[0023] This and other embodiments can include one or more of the following features.

[0024] The system can further include a controller configured to send an ultrasound signal from an element of the probe through the test medium to first, second, and third hydrophones of the plurality of hydrophones, and the controller can be further configured to determine an acoustic position of the element based upon differences in times that the signal is received at the first, second, and third hydrophones.

[0025] The system can further include the probe, and the probe can include at least two arrays separated by a physical space, and the dock can be configured so as to hold at least one of the arrays at a non-orthogonal angle with respect to the hydrophone matrix. The probe can include a calibration memory chip configured to store data obtained by the calibration system.

[0026] The dock can be configured to conform to the ultrasound probe shape. The dock can be configured such that, when the probe is positioned in the dock, the probe is directly adjacent to the test medium. The material of the dock can have substantially the same speed of sound as the test medium.

[0027] The matrix can include a first row of hydrophones, a second row of hydrophones parallel to the first row of hydrophones, and a third row of hydrophones transverse to the first and second rows.

[0028] The system can further include a calibrator hydrophone located on a wall of the tank separate from the wall along which the plurality of hydrophone receivers are arranged.

BRIEF DESCRIPTION OF THE FIGURES

[0029] FIG. 1 illustrates a two-aperture system.

[0030] FIG. 2 illustrates a three-aperture system.

[0031] FIG. 3 is a schematic diagram showing a possible fixture for positioning an omni-directional probe relative to the main probe.

[0032] FIG. 4 is a schematic diagram showing a non-instrumented linkage for two probes.

[0033] FIG. 5 is a block diagram of the transmit and receive functions where a three array Multiple Aperture Ultrasound Transducer and the associated MAUI electronics are used in conjunction with a host ultrasound machine. In this embodiment, the center probe is used for transmit only and mimics the normal operation of the host transmit probe.

[0034] FIG. 5A is a block diagram of the transmit and receive functions where a two array Multiple Aperture Ultrasound Transducer and the associated MAUI electronics are used as an add-on to a host ultrasound machine, primarily for cardiac applications, with an add-on instrument. In this case, one probe is used for transmit only and mimics the normal operation of the host transmit probe, while the other probe operates only as a receiver.

[0035] FIG. 6 is a block diagram of the transmit and receive functions where a Multiple Aperture Ultrasound Transducer is used in conjunction with only a Multiple Aperture Ultrasonic Imaging (MAUI) device. The stand-alone MAUI electronics control all elements on all apertures. Any element may be used as a transmitter or omni-receiver, or grouped into transmit and receive full apertures or even sub-arrays. In this figure the insonification emanates from the central aperture, aperture 2 of 3 apertures.

[0036] FIG. 6A depicts the insonification emanating from other than center aperture, in this figure Aperture 3 of 3.

[0037] FIG. 6B is an illustration of two apertures being used a Multiple Aperture Ultrasound Transducer is used in conjunction with only a Multiple Aperture Ultrasonic Imaging (MAUI) device. In this figure the insonification emanates from aperture 2 of 2.

[0038] FIG. 6C is an illustration of two apertures being used a Multiple Aperture Ultrasound Transducer is used in conjunction with only a Multiple Aperture Ultrasonic Imaging (MAUI) device. In this figure the insonification emanates from aperture 1 of 2.

[0039] FIG. 7A is a top view of the precision array carrier with six adjustment screws and an array installed.

[0040] FIG. 7B is a side view showing the longitudinal axis adjustment of an array in the precision array carrier being supported by the array-centering gasket.

[0041] FIG. 7C is an end view showing the transverse axis adjustment of the array in the precision array carrier being supported by the array-centering gasket.

[0042] FIG. 8A is a top view of the precision array carrier.

[0043] FIG. 8B is a side (longitudinal) view of the precision array carrier.

[0044] FIG. 8C is an end (lateral) view of the precision array carrier.

[0045] FIG. 9A is a top view of the precision array carrier with a centering gasket in place.

[0046] FIG. 9B is a side view (longitudinal) of the precision array carrier with a centering gasket in place.

[0047] FIG. 9C is an end view (lateral) the precision array carrier with a centering gasket in place.

[0048] FIG. 9D is a bottom view of the precision array carrier with a centering gasket in place.

[0049] FIG. 10A is a top view of the array in the precision array carrier during a counter-clockwise rotational axis adjustment.

[0050] FIG. 10B is a top view of the array in the precision array carrier during a clockwise rotational axis adjustment.

[0051] FIG. 11 shows an end view of a precision array carrier **2150** installed on a tissue equivalent phantom **2182** and ready to transmit and receive during alignment.

[0052] FIG. 12 shows a side view of the phantom **2182** with the ends of the targets **2167** visible.

[0053] FIG. 13A is a top view of a carrier assembly with arrays installed (to become a precision carrier array assembly) and aligned within a precision transducer receptacle and stabilized with an acoustic damping material.

[0054] FIG. 13B is a side view of a precision array carrier with arrays installed (to become a precision carrier array assembly) and aligned within a precision transducer receptacle and stabilized with an acoustic damping material.

[0055] FIG. 13C is an end view of a precision carrier array with arrays installed (to become a precision carrier array assembly) and aligned within a precision transducer receptacle and stabilized with an acoustic damping material.

[0056] FIG. 14A is a top view of a precision carrier array with arrays installed and aligned within a precision transducer head receptacle, the acoustic damping material has set and alignment screws have been removed.

[0057] FIG. 14B is a side view of a precision carrier array assembly with arrays installed and aligned within a precision transducer head receptacle, the acoustic damping material has set and alignment screws have been removed.

[0058] FIG. 14C is an end view of a precision carrier array with arrays installed and aligned within a precision transducer head receptacle, the acoustic damping material has set and alignment screws have been removed.

[0059] FIG. 15 shows a precision transducer receptacle or nose piece and three precision carrier array assemblies seated atop the transducer guides.

[0060] FIG. 16 shows the precision transducer receptacle or nose piece and three precision carrier array assemblies as in FIG. 22, and an ultrasound transducer array seated in each transducer guide of the nose piece.

[0061] FIG. 17 is a drawing using three independent probes and their installed arrays or transducers. This illustration represents the positional nomenclature and array element numbering conventions.

[0062] FIG. 18A shows the Precision Stage Assembly and sections that control movement in three different axes.

[0063] FIG. 18B shows the controls for the Precision Stage Assembly.

[0064] FIG. 19A depicts is an enclosure containing Right and Left Axial Hydrophones and a Transverse Hydrophone.

[0065] FIG. 19B depicts the dual Axial Hydrophones from the side and illustrates the angular orientation of the Transverse Hydrophone.

[0066] FIG. 20 is a representation of probes attached to the precision stage assemblies on top of a fluid filled tank, and well above the hydrophone assembly.

[0067] FIG. 21A is a graphic of basic geometry used to begin the conversion of distance difference into total distance.

[0068] FIG. 21B is a graphic of the detailed geometry used to begin the conversion of distance difference into total distance allowing for the precision location of array element using three hydrophones.

[0069] FIG. 21C is a graphic of geometry used to compute the z position of an element.

[0070] FIG. 22 illustrates a nose piece containing three separate arrays after it is installed into a Multiple Aperture Transducer. This figure includes the transducer specific calibration chip, the transmit synchronization module and probe position displacement sensor.

[0071] FIG. 23A is a representation of the graphical user interface or GUI developed to allow for the precise location of elements of multiple arrays under test.

[0072] FIG. 23B depicts an array of elements under test with the ultrasound beam in the center of the transverse hydrophone, centered between the left and right hydrophones with the results displayed on the graphical user interface.

[0073] FIG. 23C is a representation of an array under test where its beam is on center but with the array to the right of center with the results displayed on the graphical user interface.

[0074] FIG. 23D is a representation of an array under test that is physically on the center axis, but has its beam is to the left of center with the results displayed on the graphical user interface.

[0075] FIG. 24 is a representation of the automatic precision stage assembly and its major components.

[0076] FIG. 25 is a representation using three arrays and three precision alignment stage assemblies showing their physical placement during testing.

[0077] FIG. 26A is an illustration of an Onboard Calibration and Quality Assurance fixture mounted to the side of the MAUI standalone system. This illustration depicts a MAUI Radiology probe being evaluated.

[0078] FIG. 26B illustrates the Onboard Calibration and Quality Assurance fixture evaluating a MAUI Cardiac probe.

[0079] FIG. 27A is a perspective view illustrating an embodiment of a calibration system attached to a multiple aperture ultrasound imaging (MAUI) control panel.

[0080] FIG. 27B illustrates an embodiment of a calibration system built into a MAUI electronics control panel.

[0081] FIG. 28 represents a side section view of a calibration system.

[0082] FIG. 29A illustrates a multiple aperture probe containing three separate arrays This figure includes a transducer specific calibration chip mounted within the probe handle.

[0083] FIG. 29B illustrates an embodiment of a curvilinear multiple aperture ultrasound imaging probe.

[0084] FIG. 30A is a bottom view of a 1D or 1.5D ultrasound transducer array.

[0085] FIG. 30B is a perspective view of a single 1D or 1.5D ultrasound transducer element with a longitudinal geometric centerline shown.

[0086] FIG. 30C is a bottom view of a 2D matrix ultrasound transducer array.

[0087] FIG. 30D is a bottom view of a CMUT ultrasound transducer array.

[0088] FIG. 31 illustrates an embodiment of a calibration system with an adjustable clasp retaining one embodiment of a MAUI probe in a docking site which may contain a coupling gel.

[0089] FIG. 32A shows the top view of an embodiment of a calibration system containing a removable docking site which contains multiple docking forms for various shapes and types of probes.

[0090] FIG. 32B shows a side view illustrating an embodiment of a calibration system containing a removable docking site having three different docking forms for receiving ultrasound probes.

[0091] FIG. 33A shows a side section view of an embodiment of a calibration system with a removable docking site with a single docking form for receiving an ultrasound probe.

[0092] FIG. 33B is a section view illustrating three embodiments of docking forms for curvilinear, linear and trans-esophageal ultrasound probes.

[0093] FIG. 34A is a plan view illustration of one embodiment of a hydrophone matrix which may be located at a bottom of a calibration system.

[0094] FIG. 34B a side view of the hydrophone matrix of FIG. 34A.

DETAILED DESCRIPTION

[0095] The following disclosure provides embodiments of calibration systems and related operation methods for calibrating ultrasound imaging probes, and particularly multiple aperture ultrasound imaging (MAUI) probes. Embodiments herein also provide systems and methods for operating such a calibration system for various purposes relating to quality assurance of the probes.

[0096] In some embodiments, a calibrating system may be configured to identify the location of each and every individual element in an ultrasound probe to a high degree of accuracy and precision. In probes having multiple arrays of transducer elements, a calibration system may be configured to identify the location and/or orientation of individual arrays. In other embodiments, a calibration system may be configured to identify the location of only selected elements of one or more arrays. In some embodiments, the location of elements and/or arrays may be determined in a three dimensional space such as a given X, Y, and Z coordinate system. In other embodiments, the location of elements and/or arrays may be determined in only two dimensions, such as an X, Y coordinate system which may correspond to an imaging plane of the probe.

[0097] As used herein, references to the “exact” or “precise” position of transducer elements (and similar terms) may imply a relatively tight tolerance. For example, in some embodiments ultrasound probe calibration systems and methods may provide information describing the acoustic

position of each transducer element in an array to within a distance of a fraction of a wavelength of ultrasound being used. In some embodiments, the acoustic position of transducer elements may be determined to within $\frac{1}{10}$ of a wavelength. In other embodiments, the acoustic position of transducer elements may be determined to within a tolerance of less than $\frac{1}{10}$ of a wavelength. In some embodiments, such as for calibrating a standard (i.e., single aperture) ultrasound probe, much looser tolerances may also be used, provided that such tolerances meet the needs of a particular system.

[0098] The simplest multi-aperture system consists of two apertures, as shown in FIG. 1. One aperture could be used entirely for transmit elements 110 and the other for receive elements 120. Transmit elements can be interspersed with receive elements, or some elements could be used both for transmit and receive. In this example, the probes have two different lines of sight to the tissue to be imaged 130. That is, they maintain two separate physical apertures on the surface of the skin 140. Multiple Aperture Ultrasonic Transducers are not limited to use from the surface of the skin, they can be used anywhere in or on the body to include intracavity and intravenous probes. In transmit/receive probe 110, the positions of the individual elements T_{x1} through T_{xn} can be measure in three different axes. This illustration shows the probe perpendicular to the x axis 150, so each element would have a different position x and the same position y on the y axis 160. However, the y axis positions of elements in probe 120 would be different since it is angled down. The z axis 170 comes in or out of the page and is very significant in determine whether an element is in or out of the scan plane.

[0099] Referring to FIG. 1, suppose that a Transmit Probe containing ultrasound transmitting elements $T_1, T_2, \dots T_n$ 110 and a Receive Probe 120 containing ultrasound receive elements $R_1, R_2, \dots R_m$ are placed on the surface of a body to be examined (such as a human or animal). Both probes can be sensitive to the same plane of scan, and the mechanical position of each element of each probe is known precisely relative to a common reference such as one of the probes. In one embodiment, an ultrasound image can be produced by insonifying the entire region to be imaged (e.g., a plane through the heart, organ, tumor, or other portion of the body) with a transmitting element (e.g., transmit element T_{x1}), and then “walking” down the elements on the Transmit probe (e.g., $T_{x2}, \dots T_{xn}$) and insonifying the region to be imaged with each of the transmit elements. Individually, the images taken from each transmit element may not be sufficient to provide a high resolution image, but the combination of all the images can provide a high resolution image of the region to be imaged. Then, for a scanning point represented by coordinates (i,j), it is a simple matter to calculate the total distance “a” from a particular transmit element T_{xn} to an element of tissue 130 plus the distance “b” from the tissue 130 to a particular receive element. With this information, one could begin rendering a map of scatter positions and amplitudes by tracing the echo amplitude to all of the points for the given locus.

[0100] Another multi-aperture system is shown FIG. 2 and consists of transducer elements in three apertures. In one concept, elements in the center aperture 210 can be used for transmitting and then elements in the left 220 and right 230 apertures can be used for receiving. Another possibility is that elements in all three apertures can be used for both transmitting and receiving, although the compensation for

speed of sound variation would be more complicated under these conditions. Positioning elements or arrays around the tissue **240** to be imaged provides much more data than simply having a single probe **210** over the top of the tissue.

[0101] The Multiple Aperture Ultrasonic Imaging methods described herein are dependent on a probe apparatus that allows the position of every element to be known and reports those positions to any new apparatus the probe becomes attached. FIGS. **3** and **4** demonstrate how a single omni-probe **310** or **410** can be attached to a main transducer (phased array or otherwise) so as to collect data, or conversely, to act as a transmitter where the main probe then becomes a receiver. In both of these embodiments the omni-probe is already aligned within the scan plan. Therefore, only the x and y positions **350** need be calculated and transmitted to the processor. It is also possible to construct a probe with the omni-probe out of the scan plane for better transverse focus.

[0102] An aspect of the omni-probe apparatus includes returning echoes from a separate relatively non-directional receive transducer **310** and **410** located away from the insonifying probe transmit transducer **320** and **420**, and the non-directional receive transducer can be placed in a different acoustic window from the insonifying probe. The omni-directional probe can be designed to be sensitive to a wide field of view for this purpose.

[0103] The echoes detected at the omni-probe may be digitized and stored separately. If the echoes detected at the omni-probe (**310** in FIG. **3** and **410** in FIG. **4**) are stored separately for every pulse from the insonifying transducer, it is surprising to note that the entire two-dimensional image can be formed from the information received by the one omni. Additional copies of the image can be formed by additional omni-directional probes collecting data from the same set of insonifying pulses.

[0104] In FIG. **5**, the entire probe, when assembled together, is used as an add-on device. It is connected to both an add-on instrument or MAUI Electronics **580** and to any host ultrasound system **540**. The center array **510** can be used for transmit only. The outrigger arrays **520** and **530** can be used for receive only and are illustrated here on top of the skin line **550**. Reflected energy off of scatterer **570** can therefore only be received by the outrigger arrays **520** and **530**. The angulation of the outboard arrays **520** and **530** are illustrated as angles α_1 **560** or α_2 **565**. These angles can be varied to achieve optimum beamforming for different depths or fields of view. α_1 and α_2 are often the same for outboard arrays, however, there is no requirement to do so. The MAUI Electronics can analyze the angles and accommodate asymmetrical configurations. FIG. **5A** demonstrates the right transducer **510** being used to transmit, and the other transducer **520** is being used to receive.

[0105] FIG. **6** is much like FIG. **5**, except the Multiple Aperture Ultrasound Imaging System (MAUI Electronics) **640** used with the probe is a stand-alone system with its own on-board transmitter (i.e., no host ultrasound system is used). This system may use any element on any transducer **610**, **620**, or **630** for transmit or receive. The angulation of the outboard arrays **610** and **630** is illustrated as angle α **660**. This angle can be varied to achieve optimum beamforming for different depths or fields of view. The angle is often the same for outboard arrays; however, there is no requirement to do so. The MAUI Electronics will analyze the angle and accommodate asymmetrical configurations.

[0106] In this illustration, transmitted energy is coming from an element or small group of elements in Aperture **2 620** and reflected off of scatterer **670** to all other elements in all the apertures. Therefore, the total width **690** of the received energy is extends from the outermost element of Aperture **1 610** to the outmost element of Aperture **2 630**. FIG. **6A** shows the right array **610** transmitting, and all three arrays **610**, **620** and **630** receiving. FIG. **6B** shows elements on the left array **610** transmitting, and elements on the right array **620** receiving. Using one transducer for transmit only has advantages with regard to a lack of distortion due to variation in fat layer. In a standalone system, transmit and/or receive elements can be mixed in both or all three apertures.

[0107] FIG. **6b** is much like FIG. **5A**, except the Multiple Aperture Ultrasound Imaging System (MAUI Electronics) **640** used with the probe is a stand-alone system with its own on-board transmitter. This system may use any element on any array **610** or **620** for transmit or receive as is shown in FIG. **6C**. As shown in either FIG. **6B** or FIG. **6C**, a transmitting array provides angle off from the target that adds to the collective aperture width **690** the same way two receive only transducers would contribute.

[0108] Some embodiments described herein include a precision carrier for the proper alignment of a universal multiple aperture ultrasound transducer. Referring to FIGS. **7A-7C**, transducer array **2161** can be already “potted” in its own fixture **2161** with lens **2162** intact. Potting procedures are conventional methods to secure the transducer array to its lens and to the case. Flex circuitry, cabling, and attachment to the larger multiple aperture ultrasound transducer fixture can take place after the potting procedure is complete. A benefit of such embodiments is that they do not use the same transducers during the alignment. Different transducers with different “pots” can be utilized in any location of the alignment fixture thanks to the flexibility of the alignment carrier.

[0109] FIGS. **8A-8C** provide views of the basic structure and features of embodiments of a precision carrier **2150** for a multiple aperture ultrasound transducer array. FIG. **8A** shows a top view of a precision array carrier **2150** with six positioning screws **2151**. FIG. **8B** shows a side view of a precision array carrier **2150** having two threaded screw holes **2180** on each side. When positioning screws **2151** are inserted into threaded screw holes (e.g., screw holes **2155** and **2156** in FIG. **7B**), adjustments may be made to employ longitudinal corrections **2159** to the “seated” array. FIG. **8C** shows a side view of a precision carrier **2150** with threaded screw holes **2180** located on each end. When positioning screws are inserted into these threaded screw holes, adjustments may be made to employ lateral corrections **2160** to the “seated” array (as illustrated in FIG. **7C**).

[0110] FIGS. **9A-9D** show a precision array carrier **2150** with an array-centering gasket **2152** installed. FIG. **9A** is a top view of the precision carrier **2150**, with an array-centering gasket **2152** placed at the bottom of the carrier where the lens **2162** located in the center. FIGS. **9B-9D** show side, end, and bottom views of the carrier, respectively. The array centering gasket **2152** can be located on the carrier’s L-shaped shoulder **2181**, as illustrated in FIG. **9B**. Further, as shown in FIG. **9B**, the gasket **2152** can extend the entire length of the carrier over the L-shaped shoulder **2181**. The gasket **2152** can extend around the corners of the L-shaped shoulder **2181** to cover the ends of the carrier as it illustrated in FIG. **9C**. The gasket provides the array

translational centering and a pivot point for positioning adjustments during operation without interfering with the integrity of the lens **2162**. FIG. 9D provides a view of the lens **2162**, the bottom of the precision carrier array centering gasket **2152**, and finally the L-shaped shoulder **2181**.

[0111] Referring back to FIGS. 7A-7C, which show top, end, and side views, respectively of a precision array carrier **2150** with an array **2161** inserted therein. The array **2161** is supported end-to-end by positioning screws **2155** and **2156**. The array can be supported from each side by positioning screws **2153**, **2154**, **2157**, **2158** and from the bottom by the array centering gasket **2152**. FIG. 7B shows the array **2161** in the precision array carrier **2150** being supported by array centering gasket **2152** and ready for longitudinal adjustment. Alternately tightening and loosening positioning screws **2155** and **2156** allows the array **2161** to be adjusted through arc **2159** to correct longitudinal axis errors. FIG. 7C shows the array **2161** in the precision array carrier **2150** supported by the array centering gasket **2152** ready for transverse alignment. Alternately adjusting positioning screw pairs **2157**, **2158** and **2153**, **2154** allow the array **2161** to be corrected for transverse axis errors.

[0112] FIGS. 10A and 10B show a top views of a precision array carrier **2150** with the array **2161** inserted. Arrows depict, respectively, counter-clockwise and clockwise rotational adjusting by way of selective screw adjustments. FIG. 10A shows a tightening of position screws **2153** and **2158** while loosening position screws **2154** and **2157** shifting the array **2161** in a counter-clockwise arc **2165** to correct rotational axis errors. FIG. 10B shows a tightening position of screws **2154** and **2157** while loosening position screws **2153** and **2158** to shift the array **2161** in a clockwise arc **2166** to correct rotational axis errors.

[0113] FIG. 11 shows an end view of a precision array carrier **2150** installed on a tissue equivalent phantom or test block **2182** and ready to transmit and receive during alignment. A 'phantom' is a structure filled with tissue equivalent material that has a speed of sound characteristics similar to that of human tissue with known voids and reflectors placed at known locations within the phantom. This end view of the phantom shows one embodiment including three targets **2167** in profile view. These targets can be echogenic, very reflective, or anechoic, void of reflection. The top target can be at a pre-determined depth D from the surface of the phantom and the face of array carrier **2150**. The other targets can be spaced at distances D1 and D2 from the top target. In some embodiments, the pre-determined depth D can be 100 mm from the top target to the face of the array. The other targets can have D1 and D2 distances of 10 mm, for example. However, any range of depths for the targets **2167** can be used, depending on the desired application of the transducer arrays. The perpendicular targets **2167** serve to assist during the longitudinal adjustment of the array positioning. When correctly positioned, the three targets would be displayed as exactly perpendicular to the front of the array, and further, each target **2167** would be displayed equidistantly one to the other.

[0114] FIG. 12 shows a side view of the phantom **2182** with the ends of the targets **2167** visible. Once transmitting and receiving, a lateral adjustment could be made to the array **2163** in the carrier **2150**. The correct alignment is for achieved when all targets are visible above and below the center target **2168**.

[0115] FIGS. 13A-13C show a precision array carrier **2150** with an array **2161** inserted and aligned, in top, side, and end views, respectively. At this stage an acoustic damping material **2162** can be poured into the gap between the array and the carrier to stabilize the position of arrays **2161**. FIG. 13B is a side view of the precision array carrier **2150** showing the gap between the array **2161** and the precision array carrier **2150** filled with acoustic damping material **2162**. FIG. 13C shows the gap between the array **2161** and the precision array carrier **2150** filled with acoustic damping material **2162**.

[0116] FIGS. 14A-14C show the precision array carrier **2150** with the array **2161** inserted and aligned in top, side, and end views, respectively. The acoustic damping material **2162** has cured and the six alignment screws have been removed. FIG. 14B is a side view of the precision array carrier **2150** with the array **2161** inserted, aligned, the acoustic damping material **2162** cured and the position alignment screws removed. At this point, the precision array carrier **2150** with its captured array becomes a precision carrier array assembly **2163**.

[0117] FIG. 15 shows a multi-aperture ultrasound probe assembly **2183** constructed with precision transducer receptacles surrounded by structural supports **2164**. The structural supports **2164** can be constructed out of many hard materials (e.g., metals or plastics) and usually are built into a larger structure such as the probe **2200** in FIG. 22. In FIG. 15, the three precision carrier array assemblies **2163** are inserted into the precision transducer receptacles **2166**.

[0118] FIG. 16 shows the multi-aperture probe assembly **2183** having precision transducer receptacles **2166** with the precision array assemblies **2163** each locked into the receptacles, thus completing the construction of the multi-aperture ultrasound probe **2184** having three transducer arrays.

[0119] FIG. 22 shows a completed probe **2200** with arrays **1701**, **1702**, and **1703** fitted in array receptacles and ready for submission to the calibration cycle.

[0120] Alternative apparatus and methods for constructing and aligning multi-aperture ultrasound probes will now be discussed. Variations in the ultrasound beam displacement or rotation of both the insonifying and receiving probes about the x, y and z axes are preferably detected and corrected to achieve the best image quality. A MAUI alignment fixture for aligning a multi-aperture probe uses one or more precision angular alignment controls, precision stage assemblies that provide for the adjustment, in 6 degrees of freedom of the each array under test.

[0121] One factor in making multi-aperture imaging systems is the importance of precisely aligning the elements of the multiple arrays. It is well recognized that by increasing the effective aperture of a probe system by including more than one probe head and using the elements of all of the probes to render an image, the lateral resolution of the image can be greatly improved. In order to render an image, the relative positions of all of the elements are preferably known precisely. In some embodiments, if the probe system has position and rotation adjustments, a display is provided to position all of the elements to be in the same plane of scan and to transmit or receive in the same plane of scan.

[0122] FIG. 17 shows a probe system **1700** comprising three probes **1701**, **1702**, and **1703** working together as a multi-aperture transducer though not assembled in a single shell. This is not a standard embodiment of a multiple aperture transducer, but serves here to aid in describing

arrays alignment. A multi-aperture transducer can comprise of any number of arrays **1710**, **1720**, **1730** (two or more), or even individual elements. For practical reasons, arrays in probes can easily be manufactured with a large number of elements and element spacing within a head can be well controlled. If one can precisely position the end elements of each probe, it is possible to imply the positions of the other elements. Therefore, a fixture will be described which finds the positions of the elements. This apparatus could determine the exact location of independent elements either inside or outside of an array; however, because arrays are typically constructed in a linear format, the embodiment discussed here only identifies the end elements.

[0123] In FIG. 17 these end elements are designated as element numbers 0 through 5, where 0 and 1 are the end elements of array **1710**, 2 and 3 are the end elements of arrays **1720** and 4 and 5 are the end elements of array **1730**. Any of the intermediate elements could be located in the same way as will be described.

[0124] A precision alignment stage assembly is shown in FIG. 18A. The far left area of the assembly **1801** allows for the mechanical connection of a single probe, such as **1701** from FIG. 17. The precision alignment stage assembly has three separate mechanisms **1801**, **1802** and **1803** that control the position of the attached array in x, y and z axes. Several alignment stage assemblies can be used in concert so that multiple probe arrays can be manipulated independently. FIG. 18B allows the operator to manipulate an array in any axis by using controls **1805**, **1806**, **1807**, **1808**, and bearing **1809**. Precision screws **1804**, **1805**, **1806**, **1807**, and **1808** can be adjusted, and bearing **1809** can be rotated to affect one or more axes for the array during the alignment process.

[0125] FIG. 25 shows the arrays **1710**, **1720** and **1730** attached in line to precision alignment stages **2510**, **2520** and **2530**. With the arrays set in place, they can now transmit to common points of interest and compare their points of impact with the other arrays.

[0126] As used herein, calibration of an ultrasound probe may involve determining the acoustic position of each individual ultrasound element in a probe with a desired degree of precision relative to some known coordinate system. The basic technique for aligning and calibrating a multiple aperture probe can be seen with reference to FIGS. 19A, 19 and 20.

[0127] FIG. 20 illustrates probes **1701**, **1702** and **1703** from FIG. 17 now attached to alignment stage assemblies above a tank or test block **2012**. The tank can be filled with any liquid, fluid, gel, solid, or other medium **2014** that is desirable for manufacture and safety considerations, as long as the speed of sound for the fluid is known. The tank can include a mounting location for the alignment stage assemblies. In some embodiments, as shown in FIG. 20, multiple alignment stage assemblies holding transducer elements can be mounted on the test block. From this position, it is possible to transmit ultrasonic pulses from the elements of any of the arrays to be received by ultrasonic sensor or hydrophones **2085** at the other end of the tank **2012**.

[0128] As used herein, the term “hydrophone” is used in a generic sense and refers to any instrument capable of accurately receiving and transducing ultrasound waves into electronic signals. In some embodiments, hydrophones may also be used to transmit ultrasound signals. Thus, in some embodiments, hydrophones may comprise piezoelectric transducer arrays, or any other suitable technology. The term

“hydrophone” is generally used herein to refer to ultrasound receiving and/or transmitting instruments attached to a calibration system, as distinct from the transducer elements and arrays of ultrasound imaging probes to be calibrated.

[0129] As shown in FIGS. 19A-19B, the hydrophone **2085** can be a multi-axis ultrasonic hydrophone **2085** configured to detect the X, Y and Z positions of each element of a single array or multiple arrays under test. The multi-axis hydrophone **2085** can include a transverse hydrophone **2086**, and right and left hydrophones **2087** and **2088**. The common targets for the probes **1701**, **1702** and **1703** to shoot at are elements **2091**, **2092** and **2093** on the right hydrophone **2087**. On the left hydrophone **2088**, elements **2094**, **2095**, and **2096** are the targets.

[0130] In use, the probe can be attached to a signal generator configured to excite any of the transducer elements to transmit ultrasonic pulses. An ultrasonic signal is transmitted which exhibits good autocorrelation properties (e.g., a long frequency sweep, or ‘chirp’ waveform, a short (wideband) pulse, a spread spectrum waveform, etc) from at least one element in arrays **1710**, **1720** and **1730**. The transmitted ultrasound signal can travel through the test block and be received by the receiving hydrophone transducer elements **2091**, **2092**, **2093**, **2094**, **2095**, **2096** and the transverse hydrophone **2086**. It is important to note that detection of the ultrasonic signal or pulse as received by the hydrophone arrays cannot be detected accurately enough by cross correlation with the signal impressed on the probe element because the probe element itself distorts the signal.

[0131] Two innovative techniques are used to obtain the needed accuracy in finding the relative time delays and hence the relative distances. The first technique is to use cross correlation between the signal received at one element of the hydrophone (for example **2091**) and the signal received at another element of the same hydrophone (for example **2093**). The correlation peak will yield the time difference and thus the distance difference.

[0132] The second technique is to interpolate between samples of the received waveforms to obtain better time resolution than simply the sampling interval. Perhaps the best way to accomplish both of these tasks is to take the Fourier transform of both signals, fill in zeros for the high frequency components of a much larger transform. Call these larger transforms FFT1 and FFT2. Then find the peak of the inverse transform of (FFT1*(conjugate of FFT2)).

[0133] A third technique may be used to convert differential distances to total distance. Consider the triangle bce in FIG. 21A where the point b represents one of the elements for which we need to compute a position, and c and e are known reference points in the bottom of the water tank. The distance d_4 represents a total distance between the test element at point b and the hydrophone element at point c (**840** or **870**). Similarly, the distance d_0 represents a total distance between the test element at point b and the hydrophone element at point e (**820** or **850**). It is desired to measure the lengths d_4 and d_0 by triangulation, but just knowing the difference between d_0 and d_4 is not enough. By adding a transverse hydrophone (see **2086** in FIG. 19A) in the bottom of the tank we have two triangles from which we can compute d_0 and d_4 . Let e, d, and c be the locations of the hydrophones **2094**, **2095** and **2096** or **2091**, **2092** and **2093** of FIG. 19A.

[0134] For the following analysis, the hydrophones **2094**, **2095** and **2096** are preferably on the same line and on a

parallel line to that formed by **2091**, **2092** and **2093**. The distance between **2094** and **2095** is designated d and the distance between **2095** and **2096** is designated d_3 . d_1 and d_3 are preferably known precisely as this becomes the reference “yardstick” for the other measurements. **2095** should be roughly centered between **2094** and **2096** LN, but d_1 does not need to equal d_3 . The same is true for **R0**, **RC**, and **RN**. **[0135]** Let d_2 be the reference distance and define measured distances as:

$$d_2m = d_2 - d_2 = 0$$

$$d_0m = d_0 - d_2$$

$$d_4m = d_4 - d_2$$

[0136] From the law of cosines we have

$$d_4^2 = d_2^2 + d_3^2 - 2d_3d_2 \cos \alpha$$

$$d_0^2 = d_2^2 + d^2 - 2d_1d_2 \cos(\pi - \alpha) = d_2^2 + d^2 + 2d_1d_2 \cos \alpha$$

$$\cos \alpha = (d_4^2 - d_2^2 - d_3^2) / (-2d_3d_2) = (d_0^2 - d_2^2 - d_1^2) / (2d_1d_2)$$

$$d_4^2 - d_2^2 - d_3^2 = -(d_0^2 - d_2^2 - d_1^2) d_3 / d_1$$

$$(d_4m + d_2)^2 - d_2^2 - d_3^2 + (d_0m + d_2)^2 d_3 / d_1 - d_1^2 d_3 / d_1 - d_1 d_3 = 0$$

[0137] Combining and canceling terms this becomes

$$d_2 = (-d_4m^2 + d_3^2 - d^2 d_3 / d_1 + d_1 d_3) / (2d_4m + 2d_0md_3 / d_1)$$

[0138] Then $d_0 = d_{0m} + d_2$ and $d_4 = d_{4m} + d_2$.

[0139] Thus we have the full measurements from received differential times.

[0140] Two parallel “yardsticks” or right and left hydrophones are provided in the bottom of the tank in order to measure position along the z axis (i.e., the axis perpendicular to the scan plane), as illustrated in FIG. 23B. It will be the goal to position all of the probe elements from all three arrays **1701**, **1702** and **1703** in a line midway between the two yardsticks using the various controls illustrated in FIG. 18B.

[0141] Referring now to FIG. 21B, consider the measurement of the position of any probe element such as **M0 1206**. First, consider using the right yardstick **R0-RC-RN 2091**, **2092**, **2093**. By transmitting a chirp signal from element **M0 1206** and receiving it on hydrophones at **R0**, **RC**, and **RN 2091**, **2092** and **2093**, one can calculate the differential times for transmission along the paths d_0 , d_2 , and d_4 . Times can be converted to distances if the speed of ultrasound of the test block medium is known. If the test block medium is water, the speed of sound is approximately $\text{sos} = 1.40238742 + 5.03821344 * \text{TE} / 1000 - 5.80539349 * \text{TEA}2 / 100000 + 3.32000870 * \text{TEA}3 / 100000 - 0.00144537900 * \text{TEA}4 / 1000000000 + 2.99402365 * \text{TEA}5 / 1000000000000$ in mm per microsecond where TE is the temperature in degrees Celsius. Differential distances can be converted to total distances according to the derivation above.

[0142] Now from trigonometry, distance $a = (d_0^2 - d_4^2 + (d_1 + d_3)^2) / (2(d_1 + d_3))$

[0143] The position along the x' axis is $d_1 - a$.

[0144] Assuming that the element is midway between the two yardsticks, then the position along the y' axis is $\sqrt{(d_0^2 - a^2 - (x'/2)^2)}$.

[0145] Initially considerable error may occur as a result of this assumption, but the measurement of z will allow for adjustment of the element or the entire probe assembly until this assumption is satisfied.

[0146] Again referring to FIG. 21B, the same computations for x' and y' can be made using the left hydrophone array **2094**, **2095** and **2095**. In some embodiments, the results of the measurements made with the right hydrophone array may be averaged with results of measurements made with the left hydrophone array.

[0147] Advantageously, by having two hydrophone arrays or “yardsticks,” the z axis can be measured, i.e., the position of the elements in or out of the scan plane. Then the array alignment apparatus can display it (see FIG. 22A, **2300**), and thus allow either manual (FIG. 18B) or automatic (FIG. 24) correction and alignment. The z variable is related to the time of arrival difference of the pulse as received at **RC 2092** and **LC 2095**. The probe position should be adjusted until the time difference is close to zero. When this is done, all of the x and y measurements will be accurate and the relative positions of all of the elements will be known.

[0148] In some embodiments, the right and left hydrophone arrays may be used to measure an acoustic position of a test element along the z axis; i.e., the test element’s position in or out of the scan plane. In some embodiments, following such a measurement the calibration system may display and/or automatically correct an alignment of the probe within the docking area of the calibration system. In other embodiments, the calibration system may direct an operator to manually adjust an alignment of the probe.

[0149] The z variable may be proportional to the distance d_2 as computed from the hydrophones on track **845** minus the distance d_2 as computed from the hydrophones on track **875** in FIG. 34A. In some embodiments, the probe position may be adjusted until this difference is close to zero.

[0150] In other embodiments in which the probe element cannot be mechanically centered between the two tracks, the z position can be computed. This is particularly true for 1.5D probes and 2D probes where it is not possible to position all elements simultaneously to a central position. In these cases, the acoustic position of elements along the z axis may be stored in the calibration table along with x and y coordinates as discussed above.

[0151] The value of z can be computed through a straightforward trigonometric calculation as illustrated in FIG. 21C.

[0152] Let m = the distance d_2 as computed from the hydrophones on track **845** and let n = the distance d_2 as computed from the hydrophones on track **875**.

[0153] Let w indicate half the known distance between the two tracks.

$$n^2 = (w - z)^2 + y^2$$

$$m^2 = (w + z)^2 + y^2$$

$$\text{then } n^2 = (w - z)^2 + m^2 - (w + z)^2$$

$$\text{and } z = (m^2 - n^2) / 4w.$$

[0154] In some embodiments, the transverse hydrophone array may be used to determine an angular displacement of a probe test element. In some embodiments, such information may be used to direct automatic or manual re-positioning of the probe. In alternative embodiments, such information may be incorporated into stored calibration data.

[0155] In some embodiments, a controller, such as a computer, can scan and find the maximum signal strength on the transverse hydrophone **2086** and record the angular displacement for the probe element.

[0156] To use the multiple aperture array alignment apparatus as a daily calibrator, multiple aperture ultrasound transducers may already be fully assembled, such as the embodiment illustrated in FIG. 22. Therefore, all of these measurements will preferably be referenced to axes on the probe assembly. In the multi-aperture transducer probe assembly 2200 shown in FIG. 22, it would be reasonable to rotate and translate all measurements to a new coordinate system (x, y) centered on the center array. The appropriate coordinate system would be dependent on the ultrasound imaging system for which the probe assembly would be used. The multi-aperture probe can have a resident calibration memory or cal chip 2201 that can be programmed with calibration data received from the automated precision stage assembly, described below.

[0157] The transmit synchronization module 2202 is not related to calibration, but may be used to identify the start of pulse when the probe is used as an add-on device with a host machine transmitting. The probe displacement sensor 2203 can be an accelerometer or gyroscope that senses the three dimensional movement of the probe. During calibration, the probe should be securely attached to the array alignment apparatus so that the probe is still. The calibration system may then compare information from the position sensor of the probe with information from the position sensor of the calibration tank 122 to determine whether the probe is properly aligned.

[0158] Referring now to FIG. 23A, a proprietary graphical user interface or GUI 2300, allows the elemental array data to be visualized in real-time allowing for correction of the x, y and z variation errors. The two wide vertical lines 2001 and 2003 represent the z positions of the yardsticks R0-RC-RN (2091, 2092, and 2093 from FIG. 19A) and L0-LC-LN (2094, 2095, and 2096 from FIG. 19A). The thinner vertical line 2302 is the z=0 line and the desired position of each of the elements of a probe system. The vertical position is the x coordinate.

[0159] Each small square, such as 2305, 2306, 2307, 2308, 2309, 2310 and 2011, is the position of a probe element in the x-z plane. In this example there are six small squares indicating the positions of the end elements of three probe heads. However, the positions of more or fewer elements could be displayed in this way. The thin horizontal lines 2312, 2313, 2314, 2315, 2316, 2317 and 2018 represent the directivity and angular spread of each element as detected on the multi-axis hydrophone. A useful angular spread measure is the number of hydrophone elements on the transverse hydrophone array which record signal strength greater or equal to half of the maximum strength.

[0160] FIG. 23B depicts a probe element positioned correctly with the z position 2305 at or near z=0 and its directivity positioned over the centerline. In contrast, FIG. 23C depicts a probe element with its z position 2305 offset toward the right hydrophone. The resulting display shows the small square, 2305, to the right of centerline, 2302. Note that in this case, the element position is in error, but the element directivity remains over the centerline as indicated on the display by the horizontal line 2312 remaining centered over centerline, 2302.

[0161] Finally, FIG. 23D depicts a probe element correctly positioned with its z 2305 position at or near z=0, 2302. The directivity 2312, however, is misaligned in this case with an offset toward the left hydrophone as indicated by the horizontal line shifted to the left of centerline, 2302. In this case,

the directivity needs to be corrected by adjusting the angulation to bring the directivity back over center. This could be accomplished, for example, by using controls 1805 and 1807 in FIG. 18B. Thus with this display, element position and directivity can be monitored simultaneously and both brought into alignment.

[0162] Adjustments of the probe position and angulation with the precision alignment stage assembly or assemblies should continue until all of the small squares and all of the horizontal lines are aligned on the center vertical line as closely as practicable, ensuring in alignment in the z axis. As this is done, the x and y positions will be computed accurately and no separate iteration will be required for these.

[0163] In some manufacturing formats, arrays 2406 could be loaded into an automated precision stage assembly like the one in FIG. 24. Here, arrays while still within their nose pieces can still be manipulated. In FIG. 24, we see an automated precision stage assembly, 2406, fitted with precision stepper motors, 2403. Stepper motor controller, 2401, drives the transducer, 2405, under test in response to instructions from controller, 2402. The controller, 2401, evaluates data from the hydrophone assembly, 2404, and calculates transducer corrections. Test programs residing in the controller, 2402, provide transducer specific calibration data back to the transducer, 2405, under test incorporation in its on board calibration chip, 2201. This automatically acquired element and array position data would be MAUI probe specific and would be used to optimize probe and system performance.

[0164] Using the precision stage assemblies with the array alignment system is only part of the value of the system. FIGS. 20A and 20B illustrate array alignment systems 2610 attached to the control unit 2620 of an ultrasound machine 2600. A cut away shows hydrophone assembly 2085 is located at the bottom of the fluid filled system 2610. In FIG. 26A a MAUI general radiology probe 2630 is affixed to the system for testing. In FIG. 26B, a MAUI cardiac probe 2640 is affixed to the system for calibration. The portability of this system, therefore allows for calibration of probes in the field multiple times per day. Additionally the MAUI system would alert the operator if service or maintenance was required.

[0165] To calibrate a probe, MAUI electronic apparatus can send a test pattern to the arrays in the probe to transmit to the hydrophone assembly 2085. When the positions of the probes and their directivities are reported as a result of the sequence, the positions of all of the elements can be downloaded to a file specific to that probe. Each file may be stored in the probe calibration chip 2201. The calibration chip may report element positions in x, y and z axes to every MAUI electronic apparatus it connects to, and therefore can perform multiple aperture imaging without recalibrating before use with a different MAUI apparatus. The calibration chip memory can also be used to analyze probe performance and reliability.

[0166] In the special case in which all of the transmit and receive elements are aligned in the same plane or are manufactured so that there is no adjustment in z position, a simplified alignment fixture can be used. Instead of two parallel "yardsticks" of hydrophones, a single yardstick can be used. In this case the probe would be centered over the single yardstick using a plumb bob or a clamping device. The x and y measurements would then be made assuming

$z=0$ and $z_r=0$. This is possible since accuracy in the value of z is much less critical in beamforming than is accuracy in the values of x and y . Thus adjusting z by the relatively crude methods of sighting with a plumb bob or clamping to a machined edge of the probe can be acceptable in spite of the high accuracy demands for measurement of x and y . Obviously, the cost of this simplified fixture would be much reduced resulting in a fixture which could be used in the field rather just in the probe assembly factory.

[0167] Embodiments below provide further systems and methods for calibrating ultrasound imaging probes as well as systems and methods for testing quality assurance characteristics of ultrasound imaging probes. Although the following embodiments are shown and described with reference to multiple aperture ultrasound imaging (MAUI) probes, the skilled artisan will recognize that many features of the systems and methods described may also be applied to ultrasound probes of any configuration where it is desirable to determine the acoustic position or the health of one or more ultrasound transducer elements in an ultrasound probe.

[0168] As discussed above and with further reference to FIGS. 28, 34A, and 34B, some embodiments of a calibration process may comprise three stages: First, a single test-element of the probe may transmit an ultrasound test signal into the calibration tank 122 through the filler material 210. Second, the hydrophones 230 may receive the ultrasound test signal, and associated electronics and/or software may geometrically triangulate the origin of the test signal in order to determine an acoustic position of the test element to within a desired degree of accuracy. Third, the acoustic position of the test element may be transformed into a coordinate system with a known origin relative to the probe. Coordinates for the test element may be stored in a table of coordinates associated with the probe. These steps may then be repeated for each transducer element in each transducer array within a probe until the acoustic position of each element is determined and recorded in a table of coordinates.

[0169] Embodiments of the systems and methods herein may quantify both transmitted and received ultrasonic pulses and use the information obtained to identify the acoustic position of single transducer elements and/or full arrays of transducer elements. Further, embodiments of the systems and methods herein may also quantify the “health” of probe elements. The “health” of a probe element may refer to a number of factors including transmitting and receiving efficiency of probe elements, element sensitivity, and electronic functionality.

[0170] Probes with multiple aperture arrays may be properly aligned during production as discussed above. However, regularly recalibrating an ultrasound probe throughout the life of the probe as opposed to only during manufacturing can allow for high quality imaging over a long period of time without requiring the probe to be returned to a manufacturer or repair facility. To address these needs, a calibration system may be provided to accompany probes into the field. In some embodiments, a calibration system may be attached to or integrally formed with an ultrasound control panel. In some embodiments, a calibration system may include a tank in the shape of an open-topped box with a mounting portion in a top section of the box for holding a probe in a calibration orientation and a plurality of receivers at a bottom of the box for receiving ultrasound signals transmitted from the probe.

[0171] By providing a calibration system as an attachment to an ultrasound imaging system, the calibration system becomes easily accessible to operators. In some embodiments, the calibration system may serve as a probe storage location for holding probes not in use. In some embodiments, a plurality of imaging probes of different configurations may be stored in the calibration system. Probes may then be selectively calibrated according to a calibration process, thus making a wide range of probe designs readily available for imaging. Moreover, adjustable multiple aperture probes may be re-configured into a different shape and then recalibrated for each patient.

[0172] Referring to FIG. 27A, a calibration system 120 may work in conjunction with a control panel 100. The control panel 100 can contain and control electronic hardware and software configured to transmit, receive and process ultrasound signals using a multiple aperture ultrasound imaging (MAUI) probe. Such hardware and software is generically referred to herein as MAUI electronics. As shown in FIG. 27A, the calibration system 120 may be externally mounted to a control panel 100. In such embodiments, the system 120 may be electronically connected to the MAUI electronics by a wired system which may include any desired wiring arrangement, such as wiring harnesses or removable plugs. Alternatively, referring to FIG. 27B, a calibration system 120 may be embedded into the control panel 100. In further embodiments, a calibration system 120 may be provided as an entirely separate device, which may be electronically connected to the MAUI electronics by any suitable wired or wireless arrangement. In further embodiments, the electronics controlling a calibration system, including electronics controlling a probe during calibration may be entirely independent (physically and/or electronically) of the electronics used for controlling an ultrasound imaging process.

[0173] As shown in FIG. 28, in some embodiments the calibration system 120 may resemble a rectangular tank that may be relatively small in size without the bulky alignment features that can be required during manufacturing. In some embodiments, an opening at the top of the tank 122 may be sized to receive a probe 370. The tank 122 may have an overall height approximately the length of a pencil box (e.g., between about 10 and 24 inches in some embodiments), although larger or smaller tanks may also be used. In some embodiments, a width and/or depth (e.g., in/out of the plane of FIG. 28) of the tank 122 may be sized to minimize undesired reflections from side walls of the tank. Additionally, a material and internal surface texture of the tank 122 may also be engineered to minimize noise from undesired reflected ultrasound waves.

[0174] In some embodiments, a matrix of ultrasonic sensors or hydrophones 230 may be attached to the bottom of the tank 122. The matrix of hydrophones 230 can function similar to the multi-axis hydrophone 2085 described above. It is desirable for the calibration tank 122 to be configured such that an entire ultrasound path between the probe and all receivers is occupied by a material with a consistent and known speed of sound. Thus, similar to the tank 2012 described above, the tank 122 may be filled by a filler 210 made of a liquid, gel or solid material with a consistent and known speed of sound. The filler 210 may be any material that is desirable for manufacture and safety considerations. The speed of sound through the filler 210 should be known precisely in order to accurately calculate the distance trav-

eled by any given ultrasound pulse during a calibration process. In one embodiment, the filler **210** is made of a relatively rigid ballistics gel. The filler **210** can occupy substantially all of the tank **122**. In some embodiments, the filler occupies most of the tank **122** except for a top layer which may be reserved for a docking area **220** configured for receiving an ultrasound probe to be calibrated.

[0175] In some embodiments, the docking area **220** may be an empty void which may be filled with a liquid or gel which may conform to a shape of a probe to be calibrated such as the illustrated multiple aperture probe **370**. In other embodiments, the docking area **220** may include a molded piece of ballistics gel (or other suitable material) configured to conform to the shape of a probe to be calibrated. Preferably, the material used in the docking area **220** has substantially the same speed of sound as the filler material **210**. In other embodiments, the docking area and/or the entire filler may comprise a flexible bladder filled with a suitable liquid or gel material. In some embodiments, the probe and/or the docking area may be coated with an ultrasound coupling gel as will be clear to the skilled artisan.

[0176] For the best results, probes should be substantially immobile during all calibration and quality testing. To reduce error the calibration system **120** may be equipped with a mechanical docking device configured to hold the probe(s) in a substantially rigid and consistent position. Referring to FIG. **31**, in some embodiments, an adjustable clasp **510** may be provided to capture and hold a probe **370** by a handle section or any other suitable portion of the probe. In other embodiments, a clasp or grasping element may be integrally formed with the docking area **220**. In some embodiments, the docking area **220** and/or a clasp **510** may include electronic contacts or other elements which may interact with corresponding features on a probe to ensure consistently proper positioning of the probe for calibration.

[0177] In other embodiments, accelerometers, gyroscopes or other position sensors within the probe may be used to inform an operator of proper or improper positioning of a probe within a docking area of a calibration system. In some embodiments, corresponding position sensors (e.g., gyroscopes, accelerometers or other sensors) may be provided in or on the calibration tank. A calibration system may then compare information from the position sensor of the probe with information from the position sensor of the calibration tank **120** to determine whether the probe is properly aligned for calibration.

[0178] FIGS. **32A-33B** illustrate embodiments of docking devices **610** that may be used in a docking area of a calibration system. FIG. **32A** shows an embodiment of a docking device **610** with a plurality of probe-specific molded receivers (**602-628**). In such an embodiment, each probe that might be used with a particular system may have a specific receiver within the calibration system. For example, the top center docking site **604** may be configured to receive a curvilinear MAUI probe **375** having a continuous concave curved array **378** of ultrasound transducer elements such as that shown in FIG. **29B**.

[0179] FIG. **32B** is a cross-sectional view of the calibration tank taken through line A1-A in the plan view of FIG. **32A**. In some embodiments, each docking device molded receiver may be manufactured to best fit the specific needs of each probe; this can be especially useful for probes with a more tight curvature or uniquely designed probes.

[0180] Other embodiments, as shown for example in FIGS. **33A** and **33B** may feature interchangeable docking receivers custom made for each transducer. The docking receivers **710**, **720**, and **730** may be removably attached to a docking area **220** of the calibration system. Each receiver **710**, **720**, and **730** may be formed for a specific type of probe. In further embodiments, one or more receivers may be configured to receive any of the probes shown and described in U.S. patent application Ser. No. 13/029,907 published as US Patent Publication 2011/0201933, now U.S. Pat. No. 9,146,313, and incorporated herein by reference.

[0181] In some embodiments, the dock may be configured such that the ultrasound probe may be stored in the dock when not in use. The user or operator can then optionally calibrate the probe prior to removing the probe from the dock.

[0182] In some embodiments, one or more temperature sensors may be provided and configured to measure a temperature of the filler **210**. As discussed above, the temperature of the filler material **210** is used to calculate the acoustic position of transducer elements in a probe during calibration. Thus, in some embodiments, a plurality of temperature sensors (e.g., thermocouples, thermistors, optical thermal imaging systems, etc.) may be positioned throughout the tank to obtain enough measurements to determine an average temperature of the filler **210** at any given time. In other embodiments, a single temperature sensor may be sufficient.

[0183] In some embodiments, a hydrophone matrix **230** such as that shown in FIG. **34A** and FIG. **28B** may be used to detect the X, Y and Z positions of each element of a single array or multiple arrays in a probe under calibration. In some embodiments, the multi-axis hydrophone **230** can include a transverse hydrophone array **810**, a right hydrophone array **845** and a left hydrophone array **875**. In other embodiments, the hydrophone matrix may include only a single array of hydrophone elements. In other embodiments, a hydrophone matrix may comprise a two-dimensional array of many detector elements to enable further measurements. For example, the hydrophone matrix may comprise a 3x3 array, a 4x4 array, a 4x6 array or any other 'n'x'm' array of hydrophone elements.

[0184] In some embodiments, the hydrophone matrix **230** may act as a target when the probe is firing. In some embodiments, hydrophone elements selected to be detectors to may depend on the size, shape and orientation of the probe to be calibrated. In some embodiments, such calibration process details may be stored in the calibration chip or another data store in communication with the calibration system electronics.

[0185] Ultrasound transducer elements or arrays of elements are typically cut from a common crystal wafer (e.g., of a piezoelectric crystal) to form 1D, 1.5D and 2D arrays. Alternatively, some ultrasound elements may be printed or machined into a micromachined lattice structure to form an array called a Capacitive Micromachined Ultrasonic Transducer (CMUT) array. FIG. **24A** illustrates a 1D piezoelectric transducer array in which each rectangular segment represents a single transducer element **400**. Such an array is referred to as one-dimensional because the array has only rows of longitudinal transducer elements without columns. FIG. **24B** illustrates a 2D piezoelectric transducer array in which each square segment represents a separate transducer element **400**. Such an array is referred to as 2-dimensional

because the array of elements extends in two directions, having both rows and columns. FIG. 30C illustrates a CMUT array in which each transducer element 400 has a more complex geometric shape. Furthermore, a CMUT array has a much more complex arrangement, where elements are not necessarily arranged in rows and columns.

[0186] In the case of conventional 1D and 1.5D phased array probes, the position of the elements is often roughly determined by the size of the cuts inside the crystal wafer upon initial manufacture. Referring to FIG. 30B, in this process, the acoustic center of each element is assumed to be at the center of the shaped crystalline structure 440, usually a parabolic channel running down the mid portion 420 of the elements. This may or may not be the true acoustic center of the element due to slight variations in the structure of the PZT crystal or variability in the machining process. Nonetheless, transmit and receive beamformers typically assume that the acoustic center position of a transducer element is coincident with its geometric center. When the true acoustic center of an element is not exactly at the geometric center (e.g., along the longitudinal axis 420), then both transmit waveform energy and echoes being received are not being optimized. They are subject to the errors of being out of alignment, which detrimentally affects image quality and depth. The same problem may also exist for 1.5D, 2D and CMUT arrays. Therefore, even traditional single-aperture phased array probes may benefit from regular calibration using the systems and methods described herein.

[0187] Once an ultrasound probe is firmly mounted in the docking area of the calibration system, a calibration process may be initiated. In some embodiments, a calibration process may be initiated by a user pressing a button (e.g., 140 in FIG. 27B) on a calibrator or imaging system control panel.

[0188] In some embodiments, the calibration system may be configured to determine the acoustic position of transducer elements relative to a single array of which an individual test element is a part. For example, in the case of a multiple aperture probe such as that shown in FIG. 29A, the acoustic position of each element on the center array 350 may be determined relative to a coordinate system 380 centered on that array. Similarly, the acoustic positions of elements in the left 340 and right 360 arrays may also be determined relative to separate coordinate systems centered on those respective arrays.

[0189] A further calibration process may then be employed to detect the position of one full array relative to another, thereby providing information describing the relative positions of the three coordinate systems. In such an embodiment, test signals may be transmitted from elements at opposite ends or corners of each array to be located relative to other arrays. This may allow for the measurement of the length, acoustic center and 3-dimensional orientation of each array relative to other arrays in a probe containing multiple arrays. For example, the position and orientation of a planar transducer array may be determined by identifying the three-dimensional location of a sufficient number of array elements to define the orientation of the array's planar surface. In some embodiments, three elements may be sufficient to define the plane of an array. In other embodiments, several or all elements may be located to define the orientation of the array's plane. In some embodiments, information describing the orientation of a planar array may be stored along with other calibration data. Such embodi-

ments may be especially useful when calibrating adjustable probes which may contain two or more physically separate arrays which are free to move relative to one another.

[0190] In some embodiments, the calibration system can be configured to transmit a new test signal to the hydrophone matrix from every element of the probe such that the acoustic location of every element of the probe can be determined. In other embodiments, a test signal can be sent from only a few of the probe elements, such as two probe elements in an array, and the remaining locations can be determined through interpolation.

[0191] Many transmit pulse patterns may be used in the step of transmitting an ultrasound test signal from a test element. In some embodiments, an ultrasonic test signal may be transmitted which exhibits good autocorrelation properties. In some embodiments, such a test signal may comprise a long frequency sweep, a 'chirp' waveform, a spread spectrum waveform, a 'ping', a pseudorandom sequence, or another suitable pattern. In some embodiments, a test signal may be selected to require minimal computational complexity.

[0192] As will be clear to the skilled artisan in view of the discussion herein, the only directly measurable ultrasound parameter in the calibration system is the time delay between transmission of a test signal from a probe test element and receipt of the test signal at each hydrophone element. Based on these time delays, known speed of sound through the filler material, and known physical geometry of the calibration system, the position of a test element may be calculated.

[0193] It is important to note that in many cases, a test element may distort the timing of a transmitted signal. Thus, in some embodiments, it may be desirable to perform time delay measurements without relying on a presumed "transmit time" as determined by a time of sending an electrical signal to a transducer element. In such embodiments, the total distance traveled by an ultrasound test signal may be determined by using only the speed of sound and the difference between the time at which the test signal is received at a first hydrophone element and a time-of-receipt of the test signal at a second hydrophone element.

[0194] Multiple techniques, such as those described above with reference to FIGS. 21A, 21B & 21C, may be used to obtain the needed accuracy in finding the relative time delays and hence the relative distances, including using cross correlation between the signal received at one hydrophone element (e.g., 820) and the signal received at another element of the same hydrophone array (e.g., 840), interpolating between samples of the received waveforms to obtain better time resolution than simply the sampling interval, and converting a differential distance measured by two hydrophone elements to a total distance traveled by an ultrasound test signal.

[0195] Referring to FIG. 28, a coordinate system 260 can be established relative to the hydrophone matrix. In FIG. 28, the X-axis is aligned with left and right directions in the tank, the Y-axis is aligned with the "up and down" directions in the tank, and the Z-axis is perpendicular to the scan-plane and the plane of FIG. 28. The position of a plurality of probe elements, such as every probe element, can then be determined relative to the coordinate system 260.

[0196] In some embodiments, position measurements may be translated from the coordinate system 260 with an origin relative to the hydrophones matrix to a coordinate system

380 with an origin located on the probe itself, as shown in FIG. 29. In the coordinate system **380** shown in FIG. 29, the X-axis lies along a center line of all three arrays, the Y-axis is perpendicular to the plane of the center array, and the Z-axis is perpendicular to the X & Y axes, extending in and out of the page of FIG. 29A. In some embodiments, a process of rotating and translating coordinates may be used to translate the coordinate systems. In some embodiments, an appropriate probe-relative coordinate system may be dependent on the ultrasound imaging system for which the probe assembly is to be used.

[0197] With a conventional array, a transmit pulse from a transmitting element to a reflector is easily calculated back to a given receive element. Assuming a constant speed of sound, the positions in a conventional matrix or linear array are mechanically assumed so that transmit and receive paths can be easily computed. In multiple aperture imaging it is important to determine the position of each element relative to the position of any other element(s) in a known space such as a Cartesian X, Y, and Z coordinate system illustrated in FIG. 31 for example. In some embodiments, such a coordinate system may have one element designated as an origin and acoustic center positions of all other element(s) may be assigned coordinates relative to this initial position. From this the position of any element may then be known relative to any other.

[0198] As will be clear to the skilled artisan, the origin of a coordinate system may be centered at any element, or at any other point on or off of the probe. Additionally, the calibration system need not necessarily use a Cartesian coordinate system; any suitable coordinate system may be used, provided that such a coordinate system gives accurate information about the position of transducer elements.

[0199] The information obtained through calibration as well as the new coordinate system may then be compared to original element position information for the probe, as well as any previous calibration data. In some embodiments, this information may be tracked over time to better understand the properties of the probe elements and the probes as they are used. In some embodiments, this time-series calibration information may be stored and/or analyzed in an ultrasound imaging system, a remote server system, or any other suitable computing system.

[0200] During manufacturing, each MAUI transducer may be properly aligned and calibrated according to the type of crystal matrix used. The initial coordinate system and calibration may then be programmed into a memory chip **310**, which can be set in the handle of the probe as shown in FIG. 29A. When the probe is recalibrated at some later time, the calibration system electronics may compare the new calibration results to the initial or last-known position of the elements. Difference data or new position data may then be updated in the calibration chip **310**. Besides maintaining the calibration data, calibration chip **310** may also contain data for setting up a general layout of each probe, this information may be used to inform the calibration system of the number of elements to fire and in roughly what order or design during calibration.

[0201] In some embodiments, calibration data for a probe may be stored in a location other than the probe itself. It is generally desirable for calibration data to be associated specifically with the probe it describes, but such information may be stored in any practical physical location. For example, in some embodiments, a probe may have an ID

chip which carries substantially only an identification number which may be used to retrieve a unique calibration record stored in a remote (e.g., internet-accessible) database, in an ultrasound imaging system, or any other location. In some embodiments, communications systems may also be provided to allow for logging of calibration data into an ultrasound imaging system data log, and/or sending to a service provider and/or providing an operator with an appropriate on screen notification.

[0202] Each probe may have a unique element coordinate table which may be permanently associated with the probe, and which may be updated in subsequent calibration processes. In some embodiments, the calibration data overwrites calibration data previously stored in the memory. Overwriting advantageously ensures that updated data is constantly available, even in systems with small amounts of available memory.

[0203] In some embodiments, probes may be recalibrated and data stored as many times as desired by an operator, technician, or manufacturer.

[0204] The stored coordinate table may be used by ultrasound imaging system electronics in order improve the quality of ultrasound images generated using the calibrated probe. In one embodiment, the updated position data can be used during imaging, e.g., the stored data can be used as an input in an algorithm used to generate an image from a multiple aperture ultrasound imaging system. In another embodiment, the stored coordinate table can be used in post-image processing, i.e., the stored data can be used to decode stored image data or raw echo data.

[0205] Instruments of any kind used in the field on a daily basis will typically suffer from general wear and tear. To better understand the degradation of ultrasound transducers over time, as well as to obtain regular feedback pertaining to the general functionality of the probe, the calibration system may also be configured to perform general quality assurance functions. In some embodiments, the calibration system may test both the transmitting and receiving functions of the probe, report operational capabilities to the sonographer and send probe functionality data and repair requests to the service provider.

[0206] In some embodiments, the quality assurance test may be performed before each calibration so that the information obtained can be used to more accurately calibrate the probe. In some embodiments, after securing a probe in a docking area of the calibration system, a quality assurance test sequence may be manually or automatically initiated. For example, in some embodiments, the quality assurance test may be initiated via a button on the control panel. In some embodiments, a quality assurance test sequence may comprise three stages: The first stage will be referred to as hydrophone verification, the second stage will be referred to as an element transmit test and the third will be referred to as an element receive test.

[0207] In some embodiments, an additional self-test hydrophone **240** may be mounted to a side wall near the top of the tank **122** for use in quality assurance testing. The self-test hydrophone **240** and corresponding control electronics may be configured to check the position and function of the hydrophones of the main hydrophone matrix **230** in order to ensure proper calibration of the calibration system. In one embodiment the self-test hydrophone **240** may be located in the top of the tank **122** along the centerline of the hydrophone matrix **230**. In other embodiments, a self-test

hydrophone **240** may be positioned at any other location within the tank suitable for performing the described functions. In a process similar to the process for calibrating ultrasound probe elements, the self-test hydrophone **240** may send and receive ultrasound pulses to the main calibration hydrophones **230** and then use this information to ensure the hydrophones **230** are functioning properly and accurately.

[0208] Each hydrophone of the main hydrophone matrix **230** may also transmit a self-test signal to be received by the self-calibrator hydrophone **240**. The process may be similar to those described elsewhere herein for the calibration and quality assurance testing of ultrasound probe elements. The proper functioning and exact location of the hydrophone elements is very important for the best possible calibration of the probes.

[0209] In some embodiments, the hydrophone verification stage may ensure that information obtained from the hydrophones is accurate. As shown in FIG. **28**, some embodiments of the calibration system may be equipped with one or more self-calibrator hydrophones **240** located in a top corner of the tank. A self-calibrator hydrophone **240** may be used to verify the transmitting and receiving capabilities of the hydrophones elements of the hydrophone arrays **810**, **845**, **875** in the hydrophone matrix **230**. In some embodiments, the self-calibrator may also be used to verify the acoustic positions of the elements of the main hydrophone matrix **230**. The self-calibrator may transmit ultrasonic self-test signal pulse or pulses in a set pattern from a known location. The strength of received signals and the order in which they are received may be used to determine the acoustic position and receiving functionality of the hydrophone elements using methods similar to those described above.

[0210] In some embodiments, a quality assurance transmit test may be designed to test the transmit strength, efficiency and/or effectiveness of each transducer element of an ultrasound probe. A QA transmit test may begin by exciting a test transducer element with a precise electrical signal to cause the transducer to transmit ultrasonic pulses. The transmit test signal may have any shape and frequency as desired, preferably with good autocorrelation properties as discussed above with reference to calibration test embodiments.

[0211] The test signals may then be received by one or more hydrophone elements. The received frequency may then be transformed by the hydrophone transducer into specific amplitudes of electrical charge. From the resulting charges obtained by the hydrophones, the calibration system may determine whether a received signal has expected properties based on the electrical signal input to the test element. After testing all test elements, the calibration system may determine which test elements fall below an average transmitting capability and which fail to fire at all. This information may be obtained by comparing the amplitudes created by each test signal and then identifying which elements fall below the mean and by how much. In some embodiments, QA transmit test result data may be stored in a calibration chip within a probe or in any other suitable location. In some embodiments, an absolute value of a mean transmit strength may also be stored and analyzed over time to evaluate the long term health of a probe.

[0212] In some embodiments, a quality assurance receive test may evaluate the receiving capabilities of each probe element in a similar (but opposite) process. In some embodiments, a calibration hydrophone (**230** or **240**) may transmit

a precise ultrasonic test signal pulse or pulses of a known frequency. Each probe element may then receive the test signal and transform it into an electrical charge with a specific amplitude. The electric charges or amplitudes of the receiving probe elements may then be compared relative to each other and to any previous receive test data. Much like the transmitting test elements that are receiving poorly or not converting the ultrasonic pulses at all may fall out of tolerance. The average of the element receiving pulse amplitudes compared over time may indicate the degradation of elements. As above, test data may be logged, stored, and analyzed over time.

[0213] In some embodiments an ultrasound system operator/technician may be provided with information about quality assurance calibration and test data resulting from the above processes. In some embodiments, a service provider and/or probe manufacturer may also be informed of calibration and/or test data, e.g., when elements are underperforming or no longer transmitting or receiving. This information can be used to decide when to schedule probe repairs or when a probe should be replaced. Compensation for elements which are no longer firing, or for the adjustment of transmit amplitude and receive gain of any particular element may then be done internally to the electronics of an ultrasound imaging system (e.g., MAUI electronics in the case of a multiple aperture ultrasound imaging system).

[0214] Although many of the embodiments of ultrasound probe calibration and quality assurance testing systems and methods are shown and described with reference to multiple aperture ultrasound imaging probes, these systems and methods can also be applied to single aperture ultrasound imaging systems.

[0215] Terms such as “optimized,” “optimum,” “precise,” “exact” and similar terms used in relation to quantitative parameters are merely intended to indicate design parameters which may be controlled or varied in accordance with general engineering principles, and may involve a compromise based on the balancing of competing design factors. Use of these terms is not intended to imply or require that the parameters or components thereof are designed for the best possible or theoretical performance.

[0216] The above disclosure is sufficient to enable one of ordinary skill in the art to practice the invention, and provides the best mode of practicing the invention presently contemplated by the inventor. While there is provided herein a full and complete disclosure of the preferred embodiments of this invention, it is not desired to limit the invention to the exact construction, dimensional relationships, and operation shown and described. Various modifications, alternative constructions, changes and equivalents will readily occur to those skilled in the art and may be employed, as suitable, without departing from the true spirit and scope of the invention. Such changes might involve alternative materials, components, structural arrangements, sizes, shapes, forms, functions, operational features or the like.

What is claimed is:

1. A multiple aperture ultrasound probe comprising:
 - a probe housing;
 - a probe bracket positioned within and secured to the probe housing;
 - a first transducer array secured to a substantially planar plate-shaped first precision alignment element by a layer of a solidified polymer material interposed between a first surface of the first precision alignment

element and a first surface of the first transducer array, a second surface of the first precision alignment element being secured to the probe bracket;
a second transducer array secured to a substantially planar plate-shaped second precision alignment element by a layer of a solidified polymer material interposed between a first surface of the second precision alignment element and a first surface of the second transducer array, the second precision alignment element being secured to the probe bracket; and
a solidified polymer material disposed in a space between the probe bracket and the probe housing.

2. The probe of claim 1, wherein the first transducer array and the second transducer array are precisely aligned relative to the first precision alignment element and second precision alignment element, respectively.

3. The probe of claim 1, wherein the first surface of first transducer array is approximately parallel to a surface defined by transducer elements.

4. The probe of claim 1, wherein the first precision alignment element is secured to the probe bracket by a plurality of mechanical fasteners.

* * * * *

专利名称(译)	超声探头的校准		
公开(公告)号	US20190175152A1	公开(公告)日	2019-06-13
申请号	US16/277853	申请日	2019-02-15
[标]申请(专利权)人(译)	茂伊成像股份有限公司		
申请(专利权)人(译)	MAUI IMAGING , INC.		
当前申请(专利权)人(译)	MAUI IMAGING , INC.		
[标]发明人	SMITH DAVID M ADAM SHARON L SPECHT DONALD F BREWER KENNETH D LUNSFORD JOHN P SPECHT DAVID J		
发明人	SMITH, DAVID M. ADAM, SHARON L. SPECHT, DONALD F. BREWER, KENNETH D. LUNSFORD, JOHN P. SPECHT, DAVID J.		
IPC分类号	A61B8/00 G01S15/89 G01S7/52		
CPC分类号	A61B8/587 A61B8/4483 A61B8/4254 A61B8/00 A61B8/4477 A61B8/4218 G01S15/8915 G01S15/8913 G01S7/5205 A61B8/4444		
优先权	61/169200 2009-04-14 US		
外部链接	Espacenet USPTO		

摘要(译)

校准超声探头的方法包括将超声探头安装到校准系统上，通过校准系统的测试介质从探头的元件发射超声测试信号，以及在水听器矩阵上接收测试信号，使得可以计算元素相对于同一探针内其他元素和其他数组的位置。此外，这里描述的系统被配置为检测探测器的元件的声学性能并将结果报告给最终用户或服务提供者。

