



US006482158B2

(12) **United States Patent**
Mault

(10) **Patent No.:** **US 6,482,158 B2**
(45) **Date of Patent:** **Nov. 19, 2002**

(54) **SYSTEM AND METHOD OF ULTRASONIC MAMMOGRAPHY**

(75) Inventor: **James R. Mault**, Evergreen, CO (US)

(73) Assignee: **Healthetech, Inc.**, Golden, CO (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) Appl. No.: **09/854,950**

(22) Filed: **May 14, 2001**

(65) **Prior Publication Data**

US 2001/0044581 A1 Nov. 22, 2001

Related U.S. Application Data

(60) Provisional application No. 60/205,709, filed on May 19, 2000.

(51) **Int. Cl.**⁷ **A61B 8/00**
(52) **U.S. Cl.** **600/437; 600/443; 600/459;**
128/915

(58) **Field of Search** 600/437, 442,
600/447, 459; 128/915-916

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,630,798 A	3/1953	White et al.	128/2.07
2,826,912 A	3/1958	Kritz	73/194
2,831,348 A	4/1958	Kritz	73/861.28
2,838,399 A	6/1958	Vogel, Jr.	99/48
2,869,357 A	11/1959	Kritz	73/32
2,911,825 A	11/1959	Kritz	73/194
2,920,012 A	1/1960	Sanders et al.	167/51.5
3,213,684 A	10/1965	Seaton et al.	73/190
3,220,255 A	11/1965	Scranton et al.	73/204
3,250,270 A	5/1966	Bloom	128/2.07
3,306,283 A	2/1967	Arp	128/2.07
3,523,529 A	8/1970	Kissen	128/2.07
3,527,205 A	9/1970	Jones	128/2.08
3,681,197 A	8/1972	Smith	195/63
3,726,270 A	4/1973	Griffis et al.	128/2.08

(List continued on next page.)

FOREIGN PATENT DOCUMENTS

DE	198 10 476	9/1998
EP	0459647 A2	12/1991
EP	0 712 638	12/1995
EP	1013221 A1	6/2000
GB	2323292	9/1998
WO	WO 96/40340	12/1996
WO	99/60925	5/1999

OTHER PUBLICATIONS

Medical Progress Through Technology, vol. 9, No. 1, 1982 Berlin (D), pp. 27-32, R. Salminen et al., "Computerized Breath-By-Breath Analysis of Respiratory Variables During Exercise."

(List continued on next page.)


Primary Examiner—Francis J. Jaworski

(74) *Attorney, Agent, or Firm*—Gifford, Krass, Groh, Sprinkle, Anderson & Citkowski, P.C.

(57) **ABSTRACT**

A system for ultrasonic mammography includes an ultrasonic mammography device for constructing an ultrasonic image of a breast having a support structure with an ultrasonic transducer mounted on the support structure. The system also includes a personal digital assistant operatively connected to the ultrasonic transducer via a communication link, a patient computer system operatively connected to the personal digital assistant via a second communication link, and a healthcare provider computer system operatively connected to the patient computer system via an internet, for constructing the image of the breast. The method includes the steps of positioning the ultrasonic mammography device having an ultrasonic transducer on the patient and activating the ultrasonic transducer to generate a signal for constructing an image of the breast. The method also includes the steps of transmitting the signal from the ultrasonic transducer to the personal digital assistant, and transmitting the signal via an internet to a healthcare provider computer. The method further includes the steps of using the signal to construct an image of the patient's breast.

23 Claims, 3 Drawing Sheets

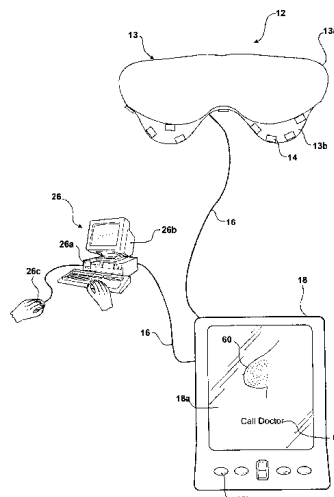

U.S. PATENT DOCUMENTS

3,797,480 A	3/1974	Williams	128/2.08	4,807,169 A	2/1989	Overbeck	364/715.01
3,799,149 A	3/1974	Rummel et al.	128/2.07	4,823,808 A	4/1989	Clegg et al.	128/773
3,814,091 A	6/1974	Henkin	128/188	4,850,371 A	7/1989	Broadhurst et al.	600/532
3,834,375 A	9/1974	Sanctuary et al.	128/2.07	4,853,854 A	8/1989	Behar et al.	364/413.01
3,895,630 A	7/1975	Bachman	128/2.07	4,855,942 A	8/1989	Bianco	364/561
3,938,551 A	2/1976	Henkin	137/613	4,855,945 A	8/1989	Sakai	364/709.2
3,962,917 A	6/1976	Terada	73/204	4,856,531 A	8/1989	Merilainen	600/532
3,967,690 A	7/1976	Northcutt	177/25	4,880,014 A	11/1989	Zarowitz et al.	128/734
3,972,038 A	7/1976	Fletcher et al.	340/189 M	4,891,756 A	1/1990	Williams, III	364/413.29
3,991,304 A	11/1976	Hillsman	235/151.33	4,894,793 A	1/1990	Ikemoto et al.	364/709.03
4,003,396 A	1/1977	Fleischmann	137/83	4,895,163 A	1/1990	Libke et al.	128/734
4,008,712 A	2/1977	Nyboer	128/2.1 Z	4,909,259 A	3/1990	Tehrani	600/531
4,051,847 A	10/1977	Henkin	128/145.6	4,911,175 A	3/1990	Shizgal	128/734
4,078,554 A	3/1978	Lemaitre et al.	128/2.08	4,911,256 A	3/1990	Attikouzel	177/25.16
4,100,401 A	7/1978	Tutt et al.	235/92 MT	4,914,959 A	4/1990	Mylvaganam et al.	73/861.28
4,101,071 A	7/1978	Brejnik et al.	235/92 MT	4,917,108 A	4/1990	Mault	600/531
4,113,039 A	9/1978	Ozaki et al.	177/25	4,924,389 A	5/1990	Gerbaulet et al.	364/413.29
4,117,834 A	10/1978	McPartland et al.	128/2 S	4,947,862 A	8/1990	Kelly	128/734
4,151,668 A	5/1979	Hugerford	40/495	4,951,197 A	8/1990	Mellinger	364/413.2
4,159,416 A	6/1979	Brejnik et al.	235/92 MT	4,954,954 A	9/1990	Madsen et al.	364/413.29
4,186,735 A	2/1980	Henneman et al.	128/201.25	4,955,946 A	9/1990	Mount et al.	600/532
4,188,946 A	2/1980	Watson et al.	128/204.22	4,965,553 A	10/1990	DelBiondo, II et al.	340/573
4,192,000 A	3/1980	Lipsey	364/415	4,966,155 A	10/1990	Jackson	128/671
4,197,857 A	4/1980	Osborn	600/531	4,986,268 A	1/1991	Tehrani	128/204
4,200,094 A	4/1980	Gedeon et al.	128/201.13	4,998,018 A	3/1991	Kurahashi et al.	250/343
4,211,239 A	7/1980	Raemer et al.	128/716	5,007,429 A	4/1991	Treatch et al.	128/677
4,212,079 A	7/1980	Segar et al.	364/900	5,012,411 A	4/1991	Policastro et al.	364/413.06
4,221,224 A	9/1980	Clark	128/718	5,019,974 A	5/1991	Beckers	364/413.02
4,221,959 A	9/1980	Sessler	377/13	5,022,406 A	6/1991	Tomlinson	128/719
4,224,952 A	9/1980	Sidorenko et al.	128/782	5,033,561 A	7/1991	Hettinger	177/25.16
4,230,108 A	10/1980	Young		5,038,773 A	8/1991	Norlien et al.	128/205.23
4,244,020 A	1/1981	Ratcliff	364/413	5,038,792 A	8/1991	Mault	128/718
4,318,447 A	3/1982	Northcutt	177/25	5,042,500 A	8/1991	Norlien et al.	600/532
4,321,674 A	3/1982	Krames et al.	364/413	5,042,501 A	8/1991	Kenny et al.	600/532
4,341,867 A	7/1982	Johansen	435/189	5,060,506 A	10/1991	Douglas	73/24.1
4,353,375 A	10/1982	Colburn et al.	128/782	5,060,655 A	10/1991	Rudolph	128/716
4,359,057 A	11/1982	Manzella	128/718	5,060,656 A	10/1991	Howard	128/718
4,366,873 A	1/1983	Levy et al.	177/25	5,063,937 A	11/1991	Ezenwa et al.	128/723
4,368,740 A	1/1983	Binder	128/718	5,068,536 A	11/1991	Rosenthal	250/341
4,380,802 A	4/1983	Segar et al.	364/900	5,069,220 A	12/1991	Casparie et al.	128/719
4,386,604 A	6/1983	Hershey	128/718	5,072,737 A	12/1991	Goulding	128/718
4,387,777 A	6/1983	Ash	177/43	5,077,476 A	12/1991	Rosenthal	250/341
4,423,792 A	1/1984	Cowan	177/25	5,081,871 A	1/1992	Glaser	73/863.23
4,425,805 A	1/1984	Ogura et al.	73/861.29	5,086,781 A	2/1992	Bookspan	128/734
4,440,177 A	4/1984	Anderson et al.	600/532	5,095,900 A	3/1992	Fertig et al.	128/207.14
4,444,201 A	4/1984	Itoh	128/716	5,095,913 A	3/1992	Yelderman et al.	128/719
4,463,764 A	8/1984	Anderson et al.	600/532	5,117,674 A	6/1992	Howard	73/31.07
4,566,461 A	1/1986	Lubell et al.	128/668	5,119,825 A	6/1992	Huhn	600/529
4,571,682 A	2/1986	Silverman et al.	364/413	5,178,155 A	1/1993	Mault	128/718
4,572,208 A	2/1986	Cutler et al.	128/718	5,179,958 A	1/1993	Mault	128/718
4,575,804 A	3/1986	Ratcliff	364/715	5,203,344 A	4/1993	Scheltinga	128/734
4,577,710 A	3/1986	Ruzumna	177/245	5,214,966 A	6/1993	Delsing	73/861.28
4,598,700 A	7/1986	Tamm	128/671	5,233,520 A	8/1993	Kretsch et al.	364/413.29
4,608,995 A	9/1986	Linnarsson et al.	128/713	5,233,996 A	8/1993	Coleman et al.	600/529
4,619,269 A	10/1986	Cutler et al.	128/719	5,263,491 A	11/1993	Thornton	128/774
4,629,015 A	12/1986	Fried et al.	177/25	5,280,429 A	1/1994	Withers	364/413.15
4,648,396 A	3/1987	Raemer	600/534	5,282,473 A	2/1994	Braig et al.	600/532
4,650,218 A	3/1987	Hawke	283/67	5,282,840 A	2/1994	Hudrlik	607/28
4,658,832 A	4/1987	Brugnoli	600/532	5,285,794 A	2/1994	Lynch	128/719
4,686,624 A	8/1987	Blum et al.	364/415	5,293,875 A	3/1994	Stone	128/719
4,709,331 A	11/1987	Barkett et al.	364/413	5,299,579 A	4/1994	Gedeon et al.	600/532
4,731,726 A	3/1988	Allen, III	364/416	5,303,712 A	4/1994	Van Duren	600/529
4,753,245 A	6/1988	Gedeon	128/718	5,307,263 A	4/1994	Brown	364/413.09
4,756,670 A	7/1988	Arai	417/43	5,309,921 A	5/1994	Kisner et al.	600/532
4,757,453 A	7/1988	Nasiff	364/415	5,326,973 A	7/1994	Eckerbom et al.	250/343
4,781,184 A	11/1988	Fife	128/205.12	5,335,667 A	8/1994	Cha et al.	128/34
4,793,362 A	12/1988	Tedner	128/734	5,355,879 A	10/1994	Brain	
4,796,182 A	1/1989	Duboff	364/413.29	5,357,972 A	10/1994	Norlien	128/725
4,796,639 A	1/1989	Snow et al.	600/532	5,363,857 A	11/1994	Howard	600/531
4,803,625 A	2/1989	Fu et al.	364/413.03				

5,372,141 A	12/1994	Gallup et al.	128/734	5,897,493 A	4/1999	Brown	600/300
5,387,164 A	2/1995	Brown, Jr.	4829/9	5,899,855 A	5/1999	Brown	600/301
5,388,043 A	2/1995	Hettinger	364/413.29	5,902,234 A	5/1999	Webb	600/300
5,398,688 A	3/1995	Laniado	128/660.02	5,908,301 A	6/1999	Lutz	434/236
5,398,695 A	3/1995	Anderson et al.	600/532	5,910,107 A	6/1999	Iliff	600/300
5,402,796 A	4/1995	Packer et al.	128/719	5,913,310 A	6/1999	Brown	128/897
5,412,560 A	5/1995	Dennison	364/413.01	5,918,603 A	7/1999	Brown	128/897
5,412,564 A	5/1995	Ecer	364/413.29	5,922,610 A	7/1999	Alving et al.	436/116
5,415,176 A	5/1995	Sato et al.	128/734	5,932,812 A	8/1999	Delsing	73/861.02
5,417,222 A	* 5/1995	Dempsey et al.	128/903	5,933,136 A	8/1999	Brown	345/327
5,419,326 A	5/1995	Harnoncourt	128/660.02	5,941,825 A	8/1999	Lang et al.	600/449
5,421,344 A	6/1995	Popp	128/734	5,951,300 A	9/1999	Brown	434/236
5,425,374 A	6/1995	Ueda et al.	600/532	5,957,585 A	9/1999	Micheels et al.	600/532
5,449,000 A	9/1995	Libke et al.	128/734	5,957,846 A	* 9/1999	Chiang et al.	600/447
5,450,193 A	9/1995	Carlsen et al.	356/301	5,974,124 A	10/1999	Schlueter, Jr. et al. ..	379/106.02
5,454,721 A	10/1995	Kuch	434/127	5,989,188 A	11/1999	Birkhoelzer et al.	600/300
5,468,961 A	11/1995	Gradon et al.	250/345	5,997,476 A	12/1999	Brown	600/300
5,474,072 A	* 12/1995	Shmulewitz	128/915	6,010,459 A	1/2000	Silkoff et al.	600/532
5,485,402 A	1/1996	Smith et al.	364/566	6,013,007 A	1/2000	Root et al.	482/8
5,503,151 A	4/1996	Harnoncourt et al. ..	128/660.02	6,014,578 A	1/2000	Minoz	600/350
5,542,420 A	8/1996	Goldman et al.	128/630	6,015,389 A	1/2000	Brown	600/533
5,570,697 A	11/1996	Walker et al.	128/719	6,024,281 A	2/2000	Shepley	235/375
5,579,782 A	12/1996	Masuo	128/734	6,024,699 A	2/2000	Surwit et al.	600/300
5,611,351 A	3/1997	Sato et al.	128/734	6,030,342 A	2/2000	Amano et al.	600/301
5,615,689 A	4/1997	Kotler	128/734	6,032,676 A	2/2000	Moore	128/898
5,632,281 A	5/1997	Rayburn	128/719	6,040,531 A	3/2000	Miller-Kovach et al.	177/25.16
5,645,071 A	7/1997	Harnoncourt et al.	128/719	6,042,383 A	3/2000	Herron	434/238
5,647,370 A	7/1997	Harnoncourt	128/725	6,044,843 A	4/2000	O'Neil et al.	128/204.23
5,673,691 A	10/1997	Abrams et al.	128/630	6,045,513 A	4/2000	Stone et al.	600/508
5,676,132 A	10/1997	Tillotson et al.	128/204.23	6,077,193 A	6/2000	Buhler et al.	482/8
5,678,562 A	10/1997	Sellers	128/710	6,083,006 A	7/2000	Coffman	434/127
5,678,571 A	10/1997	Brown	128/898	6,095,949 A	8/2000	Arai	482/4
5,691,927 A	11/1997	Gump	364/709.01	6,095,985 A	8/2000	Raymond et al.	600/513
5,704,350 A	1/1998	Williams, III	128/630	6,101,478 A	8/2000	Brown	705/2
5,705,735 A	1/1998	Acorn	73/23.3	6,122,536 A	9/2000	Sun et al.	600/341
5,720,296 A	2/1998	Cha	128/734	6,135,950 A	10/2000	Adams	600/300
5,729,479 A	3/1998	Golan	364/709.2	6,135,951 A	10/2000	Richardson et al.	600/300
5,740,801 A	* 4/1998	Branson	128/920	6,146,377 A	* 11/2000	Lee et al.	606/13
5,746,214 A	5/1998	Brown et al.	128/693	6,283,761 B1	* 9/2001	Joao	434/236
5,754,288 A	5/1998	Yamamoto et al.	356/301	OTHER PUBLICATIONS			
5,788,643 A	8/1998	Feldman	600/506	British Journal of Anaesthesia, vol. 49, 1977 London (GB)			
5,789,660 A	8/1998	Kofoed et al.	73/23.3	pp. 575-587, J.A. Bushman et al. "Closed Circuit Anaes-			
5,796,009 A	8/1998	Delsing	73/861.28	thetia."			
5,796,640 A	8/1998	Sugarman et al.	364/709.02	Determination of Nitric Oxide Levels by Fluorescence Spec-			
5,800,360 A	9/1998	Kisner et al.	600/532	troscopy, Gabor G. and Allon, N. in Biochemical, Pharma-			
5,810,722 A	9/1998	Heikkila	600/300	cological, and Clinical Aspects of Nitric Oxide, edited by			
5,816,246 A	10/1998	Mirza	128/726	B.A. Weissman et al., Plenum Press, New York, 1995, p. 57.			
5,817,031 A	10/1998	Masuo et al.	600/547	IEEE Transactions on Biomedical Engineering, vol. 35, No.			
5,819,735 A	10/1998	Mansfield et al.	128/630	9, Sep. 1988, pp. 653-659, Capek et al., "Noninvasive			
5,822,715 A	10/1998	Worthington et al.	702/19	Measurement of Cardiac Output Using Partial CO2			
5,827,179 A	10/1998	Lichter et al.	600/300	Rebreathing."			
5,831,175 A	11/1998	Fletcher-Haynes	73/861.28	Clinics in Chest Medicine (Review), vol. 10, 1989, pp.			
5,832,448 A	11/1998	Brown	705/2	255-264, Heigenhauser et al., "Measurement of Cardiac			
5,834,626 A	11/1998	DeCastro et al.	73/23.3	Output by Carbon Dioxide Rebreathing Methods."			
5,836,300 A	11/1998	Mault	600/532				
5,836,312 A	11/1998	Moore	128/897				
5,876,351 A	3/1999	Rohde	600/523				
5,890,128 A	3/1999	Diaz et al.	705/2				

* cited by examiner

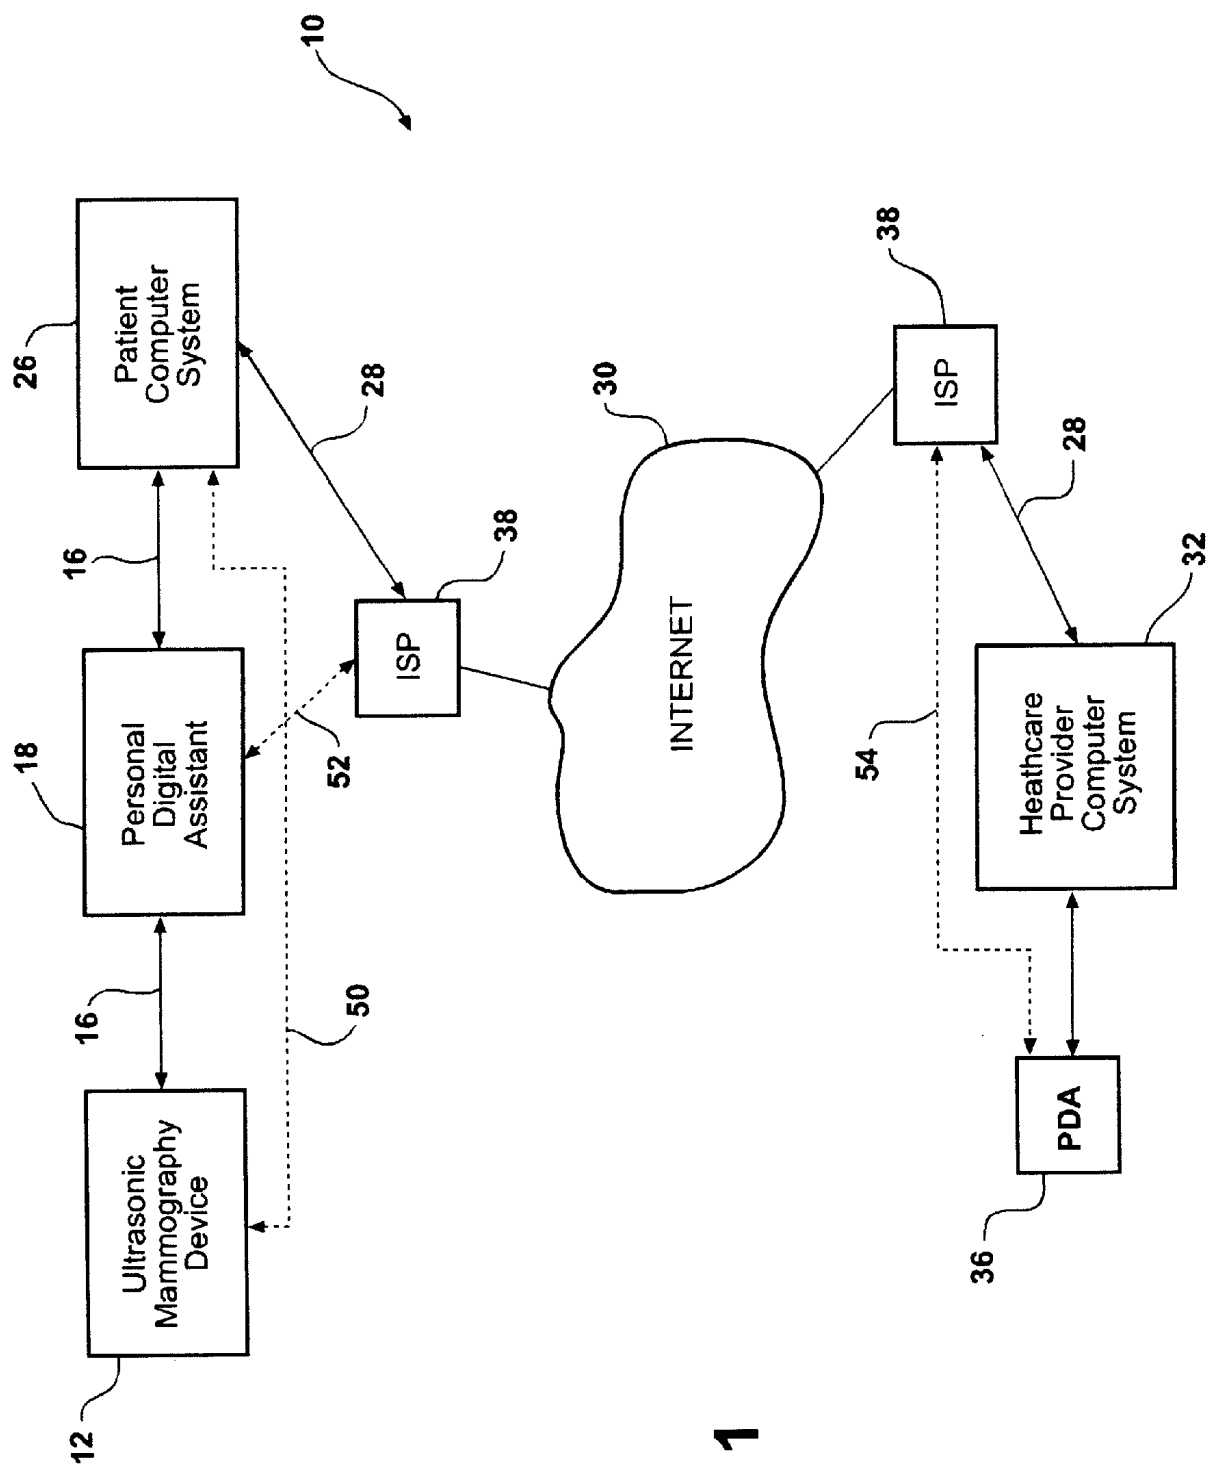
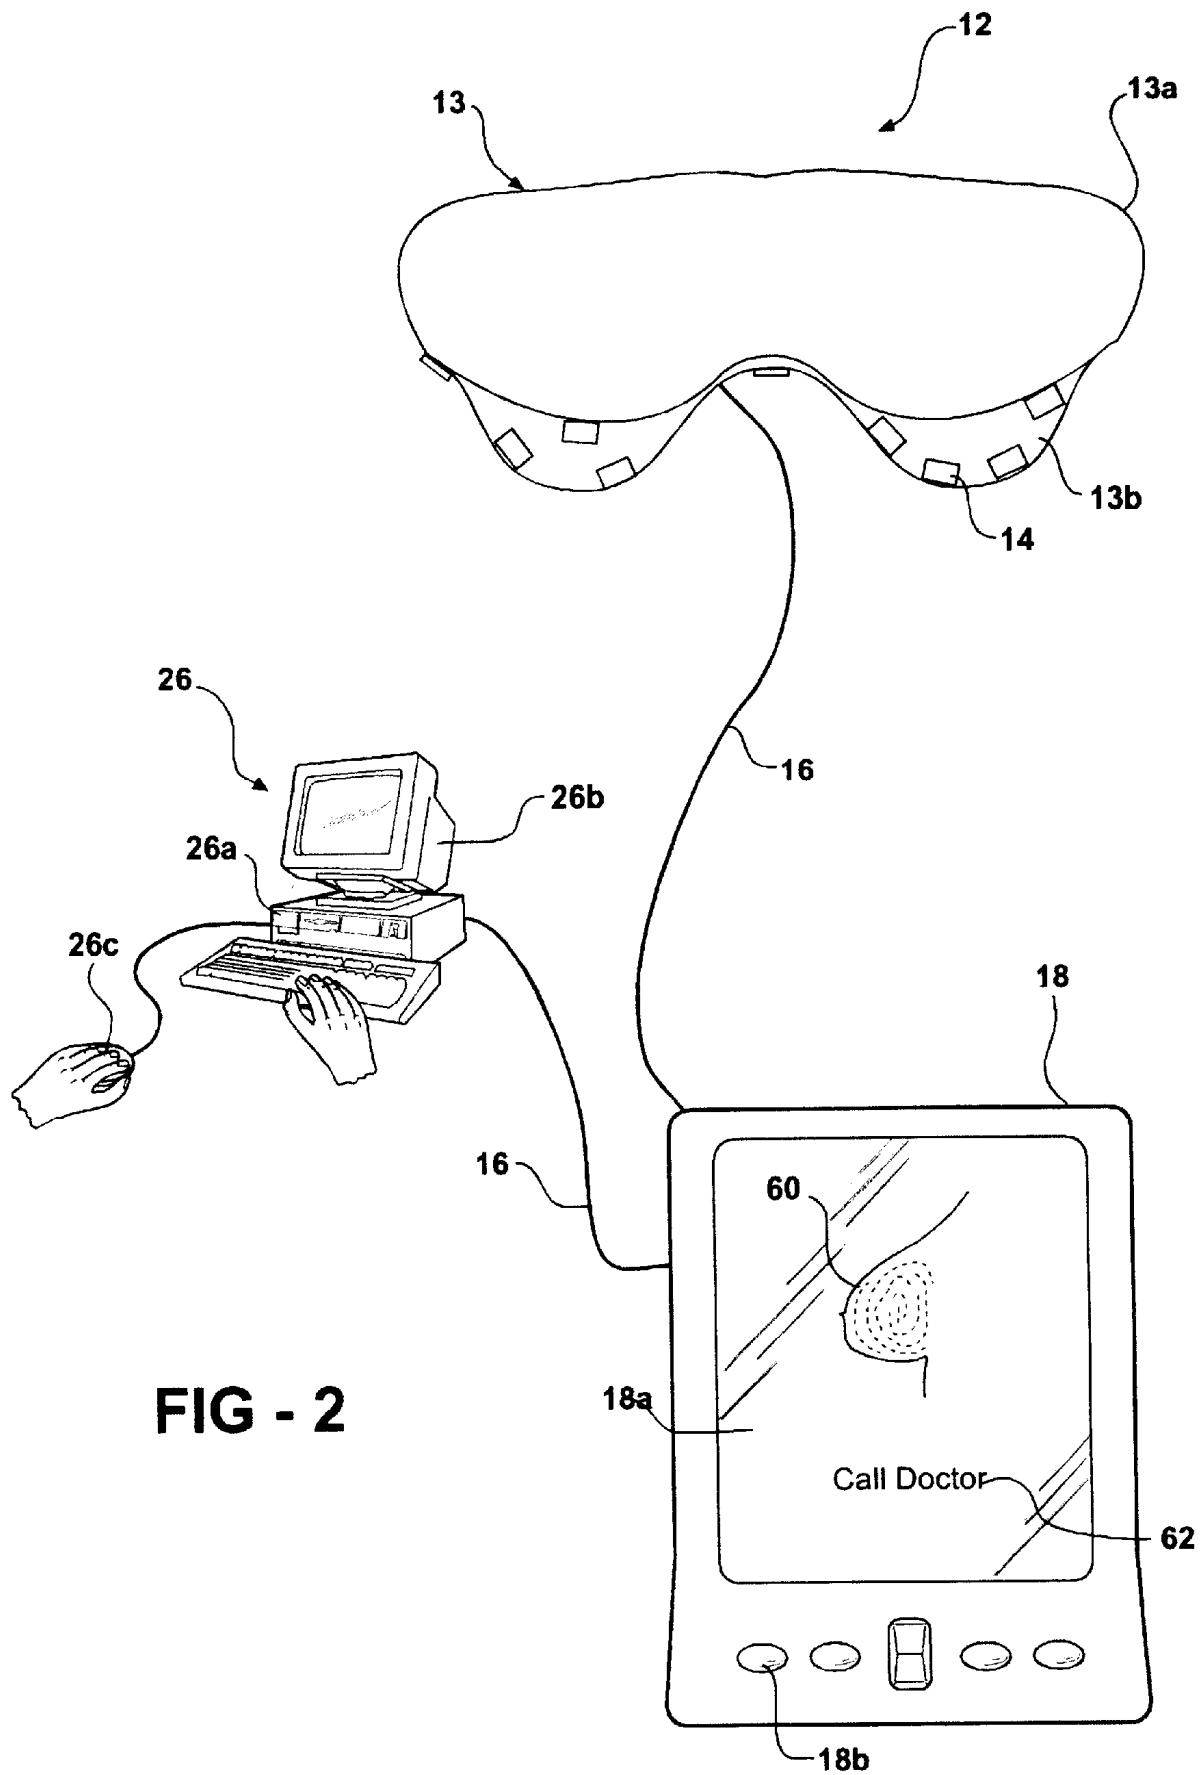
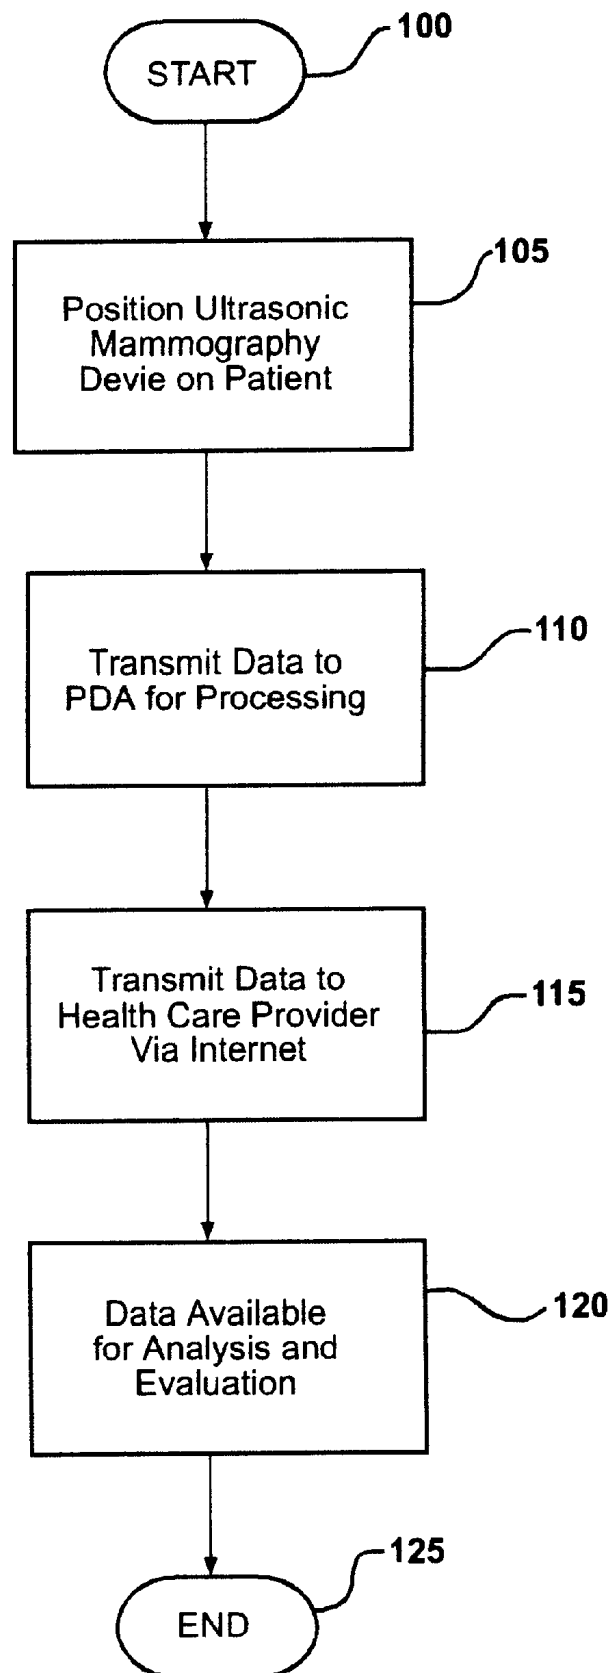


FIG - 1



**FIG - 3**

SYSTEM AND METHOD OF ULTRASONIC MAMMOGRAPHY

RELATED APPLICATION

This application claims priority of United States Provisional Patent Application 60/205,709 filed May 19, 2000, and is incorporated herein by reference.

BACKGROUND OF THE INVENTION

1. Field of the Invention

The present invention relates generally to ultrasonic medical monitoring and, more specifically, to a system and method of ultrasonic mammography for detecting a physiological condition of a patient's breast.

2. Description of the Related Art

Medical monitoring involves the measurement of a physiological condition of a patient. An example of a medical monitor is disclosed in U.S. application Ser. No. 09/669,125 (filed Sep. 25, 2000) and Ser. No. 09/821,417 (filed Mar. 29, 2001, entitled "Monitoring System"), the disclosures of which are incorporated herein by reference. Conventional breast imaging is typically accomplished using a mammography ultrasound device within a medical setting, such as a hospital or clinic. The American Medical Association has set forth guidelines recommending how frequently a woman should undergo a mammography, since early detection of a medical condition, such as breast cancer, greatly affects the success of treatment for the condition. However, access to the hospital or clinic may affect the frequency in which the patient undergoes a mammography.

While the mammography devices currently used work well, some women may procrastinate in receiving a mammography, since the current method for obtaining an ultrasonic image of a breast typically often involves some discomfort to the patient, e.g. through pressing the breast as flat as possible. Thus, there is a need in the art for a system and method of breast imaging using ultrasonic measurements, which does not cause such discomfort. Further, the measurements may be carried out at the home of the user, and the information transmitted to a medical health provider over a communications network for analysis and evaluation purposes.

SUMMARY OF THE INVENTION

One advantage of the present invention is that a system and method of ultrasonic mammography is provided for remote imaging of a breast of a patient. Another advantage of the present invention is that a system and method is provided that obtains an ultrasonic image of the patient's breast, stores the data, and transmits the data to a healthcare provider via an Internet. Still another advantage of the present invention is that a system and method is provided that includes an ultrasonic transducer disposed within a brassiere device to obtain the ultrasonic image of the patient's breast. Yet still another advantage of the present invention is that a system and method is provided that includes a personal digital assistant that stores the measured data and transmits the data via the Internet to the healthcare provider. A further advantage of the present invention is that a system and method is provided wherein the healthcare provider can evaluate the image of the breast in real-time irrespective of the physical location of the patient and the healthcare provider. Yet a further advantage of the present invention is that a system and method is provided that is cost-effective in obtaining an image of the patient's breast.

Accordingly, the present invention is a system and method for ultrasonic mammography. The system for ultrasonic mammography includes an ultrasonic mammography device for constructing an ultrasonic image of a breast having a support structure with an ultrasonic transducer mounted on the support structure. The system also includes a personal digital assistant operatively connected to the ultrasonic transducer via a communication link, a patient computer system operatively connected to the personal digital assistant via a second communication link, and a healthcare provider computer system operatively connected to the patient computer system via an internet, for constructing the image of the breast. The method includes the steps of positioning the ultrasonic mammography device having an ultrasonic transducer on the patient and activating the ultrasonic transducer to generate a signal for constructing an image of the breast. The method also includes the steps of transmitting the signal from the ultrasonic transducer to the personal digital assistant, and transmitting the signal via an internet to a healthcare provider computer. The method further includes the steps of using the signal to construct an image of the patient's breast.

Other features and advantages of the present invention will be readily appreciated, as the same becomes better understood after reading the subsequent description taken in conjunction with the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a schematic diagram of a system for ultrasonic mammography, according to the present invention.

FIG. 2 is an elevational front view of an ultrasonic mammography device for the system of FIG. 1, according to the present invention.

FIG. 3 is a flowchart of a method for ultrasonic mammography, according to the present invention, utilizing the system of FIG. 1.

DESCRIPTION OF THE PREFERRED EMBODIMENT(S)

Referring to FIG. 1 a system for ultrasonic mammography is illustrated. The system 10 includes an ultrasonic mammography device 12 having a brassiere shape. The device 12 is intended to be worn by a patient (not shown) to obtain an ultrasonic image of the patient's breast. The ultrasonic mammography device 12 includes a support structure 13 having a frame portion 13a and a cup portion 13b attached to the frame portion 13a. It should be appreciated that the frame portion 13a and cup portion 13b are integral and formed as one piece. Preferably, the size of the frame portion 13a and cup portion 13b is adjustable, to accommodate a variety of patient sizes. It should be appreciated that a uniform medium, such as water, other liquids, a gel, etc. may be used to take up volume in the cups 13b not filled by the patient's breasts.

The ultrasonic mammography device 12 also includes a predetermined number of ultrasonic transducers 14 arranged in a predetermined manner on the support structure, to construct the image of the breast. Each ultrasonic transducer 14 has a processor, a transmitter, and a receiver. The ultrasonic transducer 14 generates a signal, encapsulates the measurement data therein, and transmits the signal via a telecommunication link 16 to a personal digital assistant 18 in a manner to be described.

Ultrasonic transducers 14 of various types are suitable for this invention, e.g. devices containing piezoelectric crystals,

conducting (e.g. metal) plates, micromachined semiconductors, etc. In the preferred embodiment, the transducers **14** are capable of both transmitting and detecting or receiving ultrasound. The active elements of the ultrasonic transducer **14** may be in direct contact with the patient's breast, or an intermediate layer (not shown), such as a gel or film. The gel is a conventional ultrasound coupling gel, or other such material, that prevents the formation of air voids when the ultrasonic transducer **14** is fitted to the patient, in order to reduce ultrasonic reflection from the skin surface of the patient. It should be appreciated that the gel can be applied either to the ultrasonic transducer **14** and/or skin of the patient, prior to placement of the ultrasonic mammography device **14** on the patient.

Activation of the ultrasonic transducer **14** generates an ultrasonic signal targeted at a predetermined fixed point, such as the breastbone of the patient. The ultrasonic signal bounces from the predetermined fixed point to the ultrasonic transducer **14**, wherein the ultrasonic transducer **14** receives the ultrasonic signal. The processor portion of the ultrasonic transducer **14** calculates the distance of the ultrasonic path measured between the predetermined fixed point and the ultrasonic transducer **14**.

Preferably, the ultrasonic transducer **14** is a microscopic transducer formed on a silicon wafer using an etching technique. A plurality of microscopic transducers may be arranged in a phased array. Ultrasonic sensors arrays such as those described in U.S. Pat. Nos. 5,894,452; 5,619,476; and 5,870,351, which are incorporated by reference, can be fabricated on silicon wafers using micromachining technology. It is known that such micromachined sensors may operate as either ultrasonic transmitters or detectors. An example of this type of a silicon-based ultrasonic transducer is manufactured by Sensant.

Data from each sensor array is collected and used to enhance the real-time image constructed from measurements made by the ultrasonic transducer **14**. In another mode of operation, at least one sensor array is used as an ultrasound source while the other devices are used as imaging detectors. The roles of ultrasound source and imaging detectors are interchanged in various permutations, and a composite ultrasound image is generated by a computer. Alternatively, the ultrasonic transducer **14** includes two sensors attached at predetermined points surrounding the breast of the patient, and the path therebetween the sensors is measured.

Preferably, the predetermined number of ultrasonic transducers **14** are arranged in a predetermined manner around the front of the patient's body, and in particular the breast portion, but they may also be located around the side and back of the patient's body. For example, with four transducers **14**, one transducer **14** operates as a detector, to detect a signal, such as ultrasound radiation transmitted from the second, third and fourth transducers. Likewise, when the second transducer **14** is operating as a detector, it receives the signal representing ultrasound radiation transmitted from the first, third or fourth transducers **14**. It should be appreciated that for four transducers **14**, there are 12 potential measurements, with different permutations of detector and receiver locations.

For example, a predetermined number of ultrasonic transducers **14** represented by N, requires $N(N-1)$ such measurements. Assuming that ultrasound radiation detected by the first transducer **14** after transmission by the second transducer **14** carries the same information as that detected by the second transducer **14** after transmission by first transducer

14, the number of measurements may be reduced to $(N/2)(N-1)$ without loss of information. However, this reduction may be at the expense of greater imaging errors. Preferably, the plurality of transducers **14** are arranged around the ultrasonic mammography device **12** in sufficient number in a manner to be described, to construct an ultrasonic image of the breast computationally from the measured data.

Hence, having a plurality of ultrasonic transducers **14** arranged around the ultrasonic mammography device **12** allows a large number of independent measurements to be made for use in constructing an image of the breast. For example, the measurements can be used to construct a three-dimensional ultrasonic image of the breast. The ultrasonic image of the breast allows for the visualization of tissue composing the breast and detection of conditions of the breast, such as a tumor. It should be appreciated that a two-dimensional image may also be constructed from the data. Another approach provides for the creation a database of detected intensity measurements for various receiver-transmitter pairs. Any significant changes in the database over time may indicate a condition such as formation of a tumor.

Preferably, the ultrasonic mammography device **12** is a rigid structure, that is fitted to the patient. The ultrasonic mammography device **12** can be allowed temporary flexibility during fitting to the patient. The relative positions of each of the ultrasonic transducers **14** on the support structure is determinable by measuring signal strengths for all transmitter-receiver permutations for the ultrasonic mammography device **12** in air, or in a uniform medium of known ultrasonic properties. If the overall transmission-receiver sensitivity is known for a particular receiver-transmitter pair, the signal strength is related to transmitter-receiver separation. If all transmitter-receiver distances are measured in this way, the relative spatial locations of the ultrasonic transducers **14** on the ultrasonic mammography device **12** is determinable. Transmitter-detector sensitivity is calibrated by independent measurements, e.g. forming the cup portion of the ultrasound mammography device **12** to a known shape.

In another embodiment, the ultrasound mammography device **12** is flexible, and is fitted to the breast of the patient before ultrasound measurements are taken of the breast. In this case, the relative positions of each of the ultrasonic transducers **14** may not be known accurately before ultrasound imaging begins, and imaging with absolute spatial accuracy may not be possible. However, a condition such as a tumor may be detected by identifying any localized regions of differing ultrasound absorption, for example by comparing the receiver outputs of closely spaced ultrasonic transducers **14**. Computer modeling of the ultrasonic data provides a reasonable approximation of breast shape to create the ultrasonic images. For example, breast size or shape measurements can be determined by the patient at the time of ultrasonic imaging.

In operation, using N transducers **14**, with one transducer **14** as a receiver, signals from the other $N-1$ receivers are detected. Alternatively, for a single transducer **14** used as a receiver, the signals are detected sequentially, allowing detected intensities for all transmitter-receiver pair combinations to be measured separately. In another example, signals from a plurality of transducers **14** may be detected simultaneously. In this case, the signals from different transducers **14** may be differentiated by different emission frequencies or different time-dependent modulations. Signal processing is used to differentiate the detected signals, and make relative intensity measurements for each of them. Data

representing the ultrasound measurements is stored and processed in a manner to be described.

The system **10** includes a personal digital assistant (PDA) **18** having a memory, a processor, a display screen **18a** and an input mechanism **18b** that operatively receives the output signal generated by the ultrasonic transducer **14**, processes the signal, and transmits the signal in a manner to be described. The PDA **18** includes all portable computing devices, such as a notebook computer, a hand-held computer, a palm-held organizer, a web-enabled cellular phone, or the like that provides computing and information storage and retrieval. In this example, the PDA **18** is a hand-held device, such as the Palm or Handspring Visor. It should be appreciated that in an alternative embodiment, a personal computer **24** (to be described) is used to receive, process and transmit the signal from the ultrasonic transducer **14**, as shown at **50**.

The system **10** also includes a telecommunication link **16** for communicating between the ultrasonic transducer **14** and the PDA **18**. The telecommunication link **16** can be a wire operatively connecting the PDA and ultrasonic transducer. Alternatively, the telecommunication link is a wireless link. One example of a wireless link is a universal shortwave wireless connectivity protocol referred to as Bluetooth, as is known in the art. Another example of a wireless link is a memory module, also known as a memory stick. It should be appreciated that each ultrasonic transducer **14** transmits continuously at predetermined intervals based on a time unit contained therein, or at such a time as remotely triggered by a signal transmitted from the PDA **18**.

The system **10** includes a patient computer system **26** operatively connected to the PDA **18**, for receiving information from the PDA **18** and transmitting the information via a communication link **28** over the internet **30**, to a healthcare provider computer system **32**. The patient and healthcare provider computer systems **26**, **32** are connected to an internet infrastructure **30**, such as the Internet, via a telecommunication link **34**, such as wires (e.g. a telephone line or a cable line) or a wireless connection. It should be appreciated that the patient computer system **26** and healthcare provider computer system **32** are conventional and known in the art. The patient computer system **26** includes a processor and memory **26a**, display terminal **26b**, and input device **26c**.

In an alternative embodiment shown at **52**, the PDA **18** is a wireless PDA capable of directly accessing the internet **30** using wireless technology, as is known in the art. It should be appreciated that the healthcare provider may access the patient information on the healthcare provider computer system **32**. Alternatively, the healthcare provider can access the information via a PDA **36**, as shown at **54**.

As is known in the art, the Internet **30** includes providers, such as Internet Access Providers (IAPs), Internet Service Providers (ISPs) and Network Service Providers (NSPs) (not shown) and routers (not shown) that provide wired and wireless digital telecommunications throughout the world using a TCP/IP networking protocol. It should be appreciated that the computers **26**, **32** or PDAs **18**, **36** may access the Internet directly, or they may be operatively connected to a Local Area Network (LAN) (not shown) over which information is transmitted to other computers on the same LAN or to computers on other LANS through a localized Intranet.

The Internet **30** includes a plurality of web site servers (not shown) that interactively transfer information to a user through the user's computer. The web site server is a

computer system operatively connected to a provider in a conventional manner. The web site provides for interactive communication between the host of the web site and a visitor to the web site. The communication is facilitated by a series of screens, referred to as pages, displayed on the display screen, with the first page referred to as a home page. When the user visits a particular web site, the user is served a page displayed on the video monitor referred to as a home page. The user may interact with the page via the input device, such as by making a selection or a request.

In the preferred embodiment, the ultrasound data from the ultrasound mammography device **12** is transferred to a personal digital assistant (PDA) or portable computer in the possession of the patient. Data transfer can use a wireless, IR, optical, other electromagnetic radiation, or electrical link. It should be appreciated that images may be computed by the PDA **18**, or alternatively by the healthcare provider computer system **32**. Data, and/or images are transmitted, preferably using a computer network such as the Internet, to a computer accessible by a physician or other healthcare professional. The physician can study the data or images, and make a diagnosis. A computer expert system resident with the healthcare provider computer system **32** can also be used to determine if there is a medical condition associated with the data or images.

Referring to FIG. 3, a method for ultrasonic mammography is provided. The method begins in bubble **100** and continues to block **105**, with positioning the ultrasound mammography device **12** on the patient, so that the transducers **14** surround the breast, as previously described. The ultrasonic transducer **14** is activated, to generate an ultrasound radiation signal used in constructing a real-time three-dimensional image of the breast, as previously described. The methodology advances to block **110**.

In block **110**, the data in the form of a signal from the ultrasonic transducer **14** is transmitted to the PDA **18** for processing. The PDA **18** receives the data from the ultrasonic transducer **14** and generates a set of values and interpretive information from the data. The data is stored on the PDA **18**. For example, the PDA **18** receives the data as a set of ultrasonic path measurements sampled during a predetermined time interval and a set of predetermined timestamps, wherein each measurement has a corresponding timestamp. The PDA **18** includes software which algorithmically evaluates the measurement values to construct the image of the breast.

Preferably, the processed data is displayed on the display screen **18a** of the PDA **18** as an image as shown at **60**. Advantageously, the processed data can be compared to a predetermined criterion, such as image quality, and a message is displayed on the display screen **18a**. For example, the message may prompt the user to contact the healthcare provider, as shown at **62**. The user of the PDA **18** reviews the screens, redisplay selected screens, or inputs data into displayed fields by utilizing the operator control devices of the PDA **18**; e.g., a stylus. As one skilled in the art will recognize, the capabilities of the PDA **18** include the functionality to process and display the information as dictated by the objectives of the healthcare provider.

In an alternative embodiment, the PDA **18** transmits the data via the Internet **30** to the healthcare provider for processing. The data is processed and analyzed in the healthcare provider's computer system **32**, to construct the image of the patient's breast.

The methodology advances to block **115**, and the processed data is transmitted by the PDA **18** to the healthcare

provider via the Internet 30, as previously described. The methodology advances to block 120.

In block 120, the data is received by the healthcare provider and made available to the healthcare provider for further analysis and study. For example, the data is stored on a database on the healthcare provider's computer system 32. The information is retrieved and displayed in the form of web pages. The server stores and displays the information via web pages, either by itself or in combination with previously stored information pertinent to a particular patient profile. Further, the server utilizes various software components to process and present the information according to predetermined care objectives. It should be appreciated that the server can process data from a plurality of patients.

The healthcare provider retrieves the information via a variety of means. Typically, the server displays the information on the web pages; however, the healthcare provider may download the information from the server to a computing device of his/her choice; e.g., a PDA 36 or another personal computer (not shown).

It should be appreciated that the healthcare provider can communicate with the patient on the PDA 18. For example, the healthcare provider, after reviewing the patient's information, uploads a text message from their computer to a common interface, such as the web site. The server of the web site transmits the information via the Internet 30 to the PDA 18, which activates an alarm to notify the patient of an incoming message, and displays the same on the display unit portion of the PDA 18 as shown at 62.

The present invention has been described in an illustrative manner. It is to be understood that the terminology, which has been used, is intended to be in the nature of words of description rather than of limitation.

Many modifications and variations of the present invention are possible in light of the above teachings. Therefore, within the scope of the appended claims, the present invention may be practiced other than as specifically described.

What is claimed is:

1. An ultrasonic mammography device for constructing an image of a breast comprising:

- (a) a support structure having a brassiere shape that is worn by a patient;
- (b) at least one ultrasonic transmitter mounted on the support structure in a predetermined position; and
- (c) at least one ultrasonic detector mounted on the support structure in a predetermined position, wherein ultrasonic measurements from the ultrasonic transmitter and ultrasonic detector are used in constructing the image of the patient's breast.

2. The ultrasonic mammography device of claim 1, wherein the support structure includes a frame portion and a cup portion that are integral and formed as one piece.

3. The ultrasonic mammography device of claim 1, wherein the ultrasonic transmitter and ultrasonic detector are a silicon-based ultrasonic transducer.

4. A system for ultrasonic mammography comprising:

an ultrasonic mammography device for constructing an ultrasonic image of a breast, wherein the ultrasonic mammography device includes a support structure having an ultrasonic transducer mounted on the support structure in a predetermined position for constructing an image of the breast;

a personal digital assistant operatively connected to said ultrasonic transducer via a communication link;

a patient computer system operatively connected to said personal digital assistant via a second communication link, wherein said patient computer system includes a memory, a processor, a display device and an input device; and

a healthcare provider computer system operatively connected to said patient computer system via a communications network, wherein said healthcare provider computer system includes a memory, a processor, a display device and an input device and activation of said ultrasonic transducer generates a data signal that is transmitted to said personal digital assistant via said communication link, and transmission of said signal to said healthcare provider computer system via said second communication link, for constructing the image of the breast.

5. A system as set forth in claim 4 wherein said ultrasonic transducer is an ultrasonic transducer having a plurality of microscopic transducers arranged in an array on a silicon wafer.

6. A system as set forth in claim 4 wherein said PDA includes a memory, a processor, a display screen and an input mechanism.

7. A system as set forth in claim 4 wherein said communication link is a Bluetooth wireless communication link.

8. A system as set forth in claim 4 wherein the communications network is the Internet.

9. A system as set forth in claim 4 wherein said healthcare provider computer system is operatively connected to a plurality of patient computer systems, for evaluating a plurality of patients.

10. A system for ultrasonic mammography comprising:

an ultrasonic mammography device having a predetermined number of ultrasonic transducers, with each having a processor, a transmitter and a receiver in a predetermined position, and each arranged wherein said ultrasound mammography device is positioned over the breast of the patient;

a personal digital assistant operatively connected to said ultrasonic transducer via a communication link, wherein said personal digital assistant includes a memory, a processor, a display screen, an input mechanism, and a wireless communication mechanism for wireless communication via the internet;

a healthcare provider computer system in communication with said personal digital assistant via a communications network, wherein said healthcare provider computer system includes a memory, a processor, a display device and an input device; and

activation of said ultrasonic transducer generates transmission of a data signal to said personal digital assistant via said communication link, and wireless transmission of said signal between said personal digital assistant and said healthcare provider computer system over the communications network for analysis by the healthcare provider.

11. A system as set forth in claim 10 wherein said ultrasonic transducer is an ultrasonic transducer having a plurality of microscopic transducers arranged in an array on a silicon wafer.

12. A system as set forth in claim 10 wherein said communication link is a Bluetooth wireless communication link.

13. A system as set forth in claim 10 wherein the communications network is the Internet.

14. A system as set forth in claim 10 wherein said healthcare provider computer system is operatively con-

9

nected to a plurality of patient computer systems for simultaneously evaluating a plurality of patients.

15. A system as set forth in claim **10** wherein said ultrasonic transducer is an ultrasonic transducer having a plurality of microscopic transducers arranged in an array on a silicon wafer.

16. A method of ultrasonic mammography, said method comprising the steps of:

positioning an ultrasonic mammography device having an ultrasonic transducer on the patient to obtain an image of the patient's breast;

activating the ultrasonic transducer to generate a signal, wherein the ultrasonic transducer includes a processor, a transmitter and a receiver;

transmitting the signal from the ultrasonic transducer to a personal digital assistant, wherein the personal digital assistant includes a memory, a processor, a display screen and an input mechanism;

transmitting the signal from the personal digital assistant via a communications network to a healthcare provider computer, wherein the healthcare provider computer includes a memory, a processor, a display screen and an input device; and

using the signal to construct an image of the patient's breast.

17. A method as set forth in claim **16** wherein said ultrasonic transducer is an ultrasonic transducer having a

10

plurality of microscopic transducers arranged in an array on a silicon wafer.

18. A method as set forth in claim **16** wherein said step of transmitting the signal between the ultrasonic transducer and the personal digital assistant includes transmitting the signal via a Bluetooth wireless communication link.

19. A method as set forth in claim **16** wherein said step of transmitting the signal from the personal digital assistant includes the step of transmitting the signal via the Internet.

20. A method as set forth in claim **16** wherein said step of transmitting the signal from the personal digital assistant includes the step of transmitting the signal to a patient computer system having a memory, a processor, a display screen, and an input device.

21. A system as set forth in claim **16** including the step of receiving, by said healthcare provider computer system, a plurality of signals from a plurality of patients, for simultaneously evaluating a plurality of patients.

22. A system as set forth in claim **16** wherein said step of using the signal includes the step of using the personal digital assistant to construct an image of the patient's breast from the signal.

23. A system as set forth in claim **16** wherein said step of using the signal includes the step of using the healthcare provider computer to construct an image of the patient's breast.

* * * * *

专利名称(译)	超声乳房X线照相术的系统和方法		
公开(公告)号	US6482158	公开(公告)日	2002-11-19
申请号	US09/854950	申请日	2001-05-14
[标]申请(专利权)人(译)	詹姆士R.莫特		
申请(专利权)人(译)	MAULT JAMES R.		
[标]发明人	MAULT JAMES R		
发明人	MAULT, JAMES R.		
IPC分类号	A61B5/044 A61B5/087 A61B5/08 A61B5/053 A61B5/0402 A61B5/22 A61B5/00 A61B5/083 A61B5/11 A61B5/024 A61B5/022 A61B7/00 A61B8/08 A61B8/00		
CPC分类号	A61B5/044 A61B5/0537 A61B5/0833 A61B5/087 A61B5/222 A61B5/4872 A61B5/6817 A61B5/6826 A61B5/6838 A61B5/6896 A61B5/742 A61B8/0825 A61B5/0008 A61B5/022 A61B5/02438 A61B5/14532 A61B5/1455 A61B7/00 A61B2560/0295 A61B2560/0456 A61B2560/0462 A61B2560/0468 A61B2560/0475 Y10S128/915		
优先权	60/205709 2000-05-19 US		
其他公开文献	US20010044581A1		
外部链接	Espacenet USPTO		

摘要(译)

一种用于超声乳房X线照相术的系统，包括用于构造乳房的超声图像的超声乳房摄影装置，该乳房具有支撑结构，其中超声换能器安装在支撑结构上。该系统还包括通过通信链路可操作地连接到超声换能器的个人数字助理，通过第二通信链路可操作地连接到个人数字助理的患者计算机系统，以及通过可操作地连接到患者计算机系统的医疗保健提供者计算机系统。互联网，用于构建乳房的形象。该方法包括以下步骤：将具有超声换能器的超声乳房造影设备定位在患者身上并激活超声换能器以产生用于构建乳房图像的信号。该方法还包括将信号从超声换能器传输到个人数字助理，以及通过互联网将信号传输到医疗保健提供者计算机的步骤。该方法还包括使用该信号构建患者乳房图像的步骤。

