



US007144371B2

(12) **United States Patent**
Edwardsen et al.

(10) **Patent No.:** **US 7,144,371 B2**
(45) **Date of Patent:** ***Dec. 5, 2006**

(54) **TRANSESOPHAGEAL ULTRASOUND PROBE
HAVING A ROTATING ENDOSCOPE SHAFT**

(75) Inventors: **Stephen Dodge Edwardsen**, Sandefjord
(NO); **Dag Jordfald**, Horten (NO)

(73) Assignee: **GE Medical Systems Global
Technology Company, LLC**,
Waukesha, WI (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 181 days.

This patent is subject to a terminal dis-
claimer.

(21) Appl. No.: **10/805,819**

(22) Filed: **Mar. 22, 2004**

(65) **Prior Publication Data**

US 2004/0176691 A1 Sep. 9, 2004

Related U.S. Application Data

(63) Continuation of application No. 10/317,158, filed on
Dec. 10, 2002, now Pat. No. 6,749,572, which is a
continuation of application No. 09/681,296, filed on
Mar. 14, 2001, now abandoned.

(51) **Int. Cl.**
A61B 8/14 (2006.01)

(52) **U.S. Cl.** 600/459; 600/467

(58) **Field of Classification Search** 600/437,
600/442, 443, 447, 459-472

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

| | | | |
|----------------|--------|-----------------------|---------|
| 5,211,176 A * | 5/1993 | Ishiguro et al. | 600/463 |
| 5,215,092 A * | 6/1993 | Wray | 600/445 |
| 5,388,584 A * | 2/1995 | King | 600/462 |
| 5,413,107 A * | 5/1995 | Oakley et al. | 600/463 |
| 5,479,929 A * | 1/1996 | Cooper et al. | 600/459 |
| 5,634,466 A * | 6/1997 | Gruner | 600/459 |
| 5,738,631 A * | 4/1998 | Konstorum | 600/148 |
| 6,749,572 B1 * | 6/2004 | Edwardsen et al. | 600/459 |

* cited by examiner


Primary Examiner—Ali Imam



(74) *Attorney, Agent, or Firm*—McAndrews, Held &
Malloy, Ltd.; Peter J. Vogel; Michael A. Dellapenna

(57) **ABSTRACT**

A transesophageal ultrasound probe for imaging internal structures via an imaging element located on the distal end of a rotating endoscope shaft. The probe includes a rotating endoscope having an imaging element mounted on the distal end of the rotating endoscope shaft. The probe also includes a control handle for controlling the imaging controls and a rotation tube that extends through the rotating endoscope shaft and into the control handle. The rotating shaft rotates relative to, and independently of, the control handle. Preferably, the rotating shaft is rotated via a rotation control wheel. The rotation control wheel is fastened or bonded to the rotating tube so that manual rotation of the control wheel causes the rotation tube to rotate, and therefore, the rotating shaft to rotate. Because the rotating endoscope shaft rotates, an imaging element located on, or within, the rotating shaft also rotates.

14 Claims, 4 Drawing Sheets

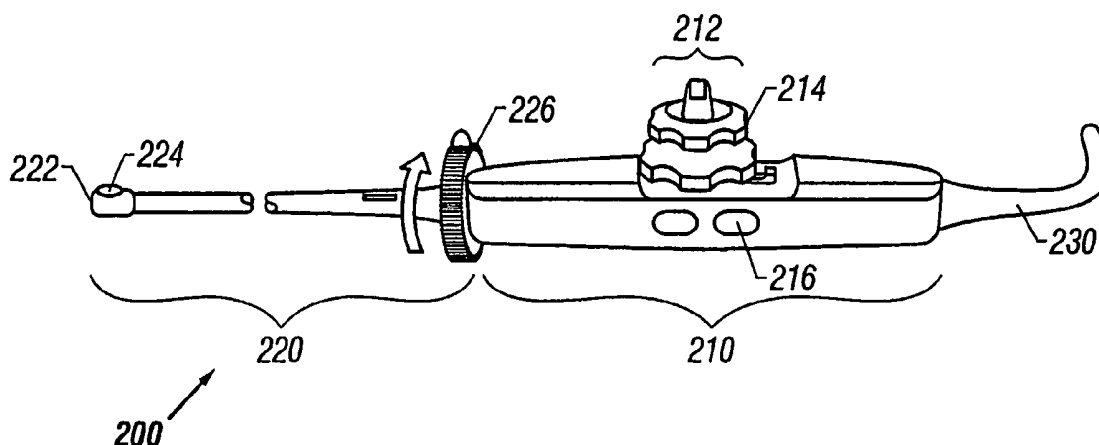

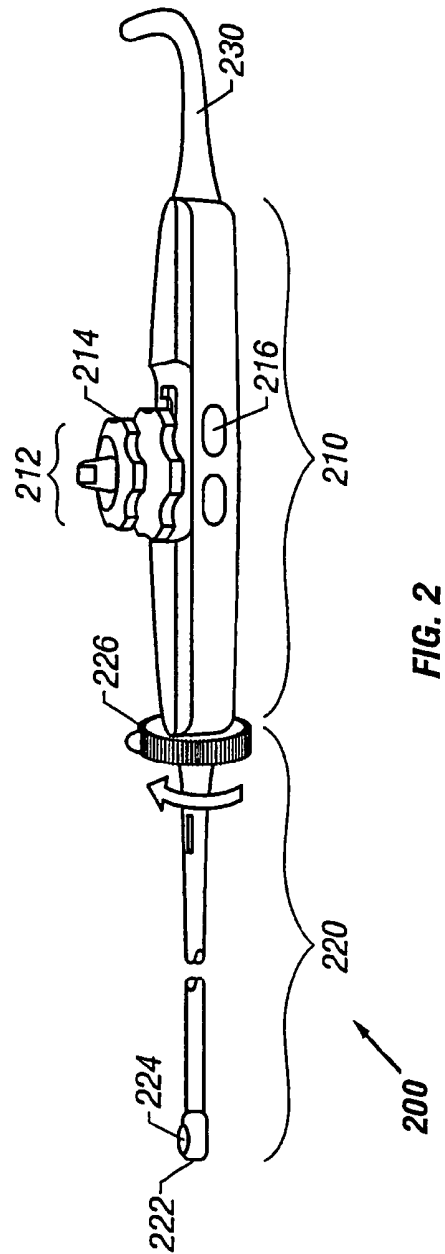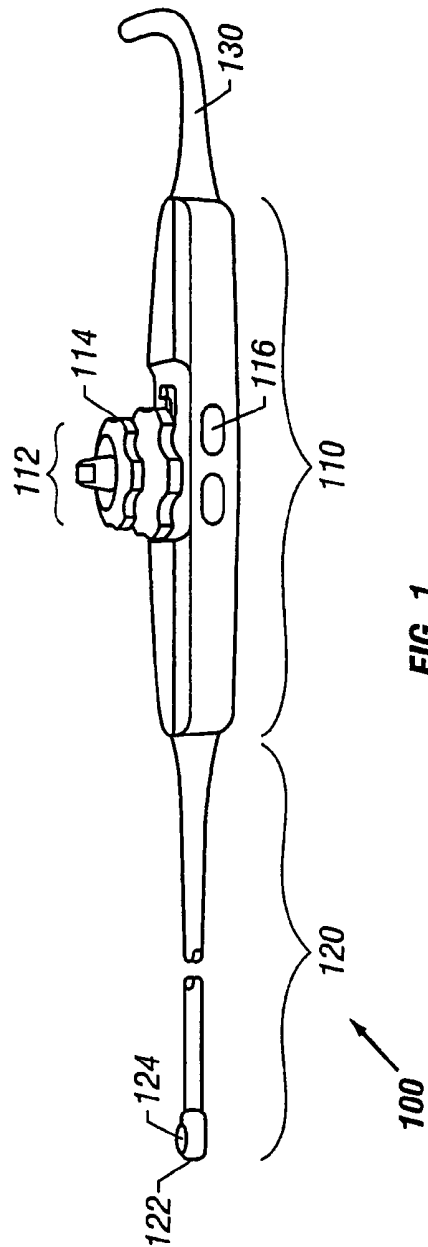

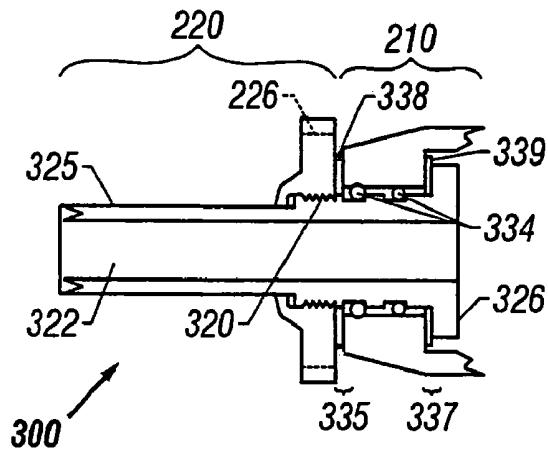


FIG. 3

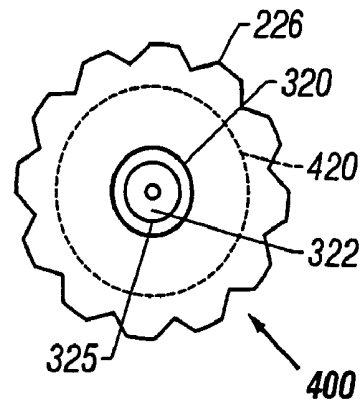


FIG. 4

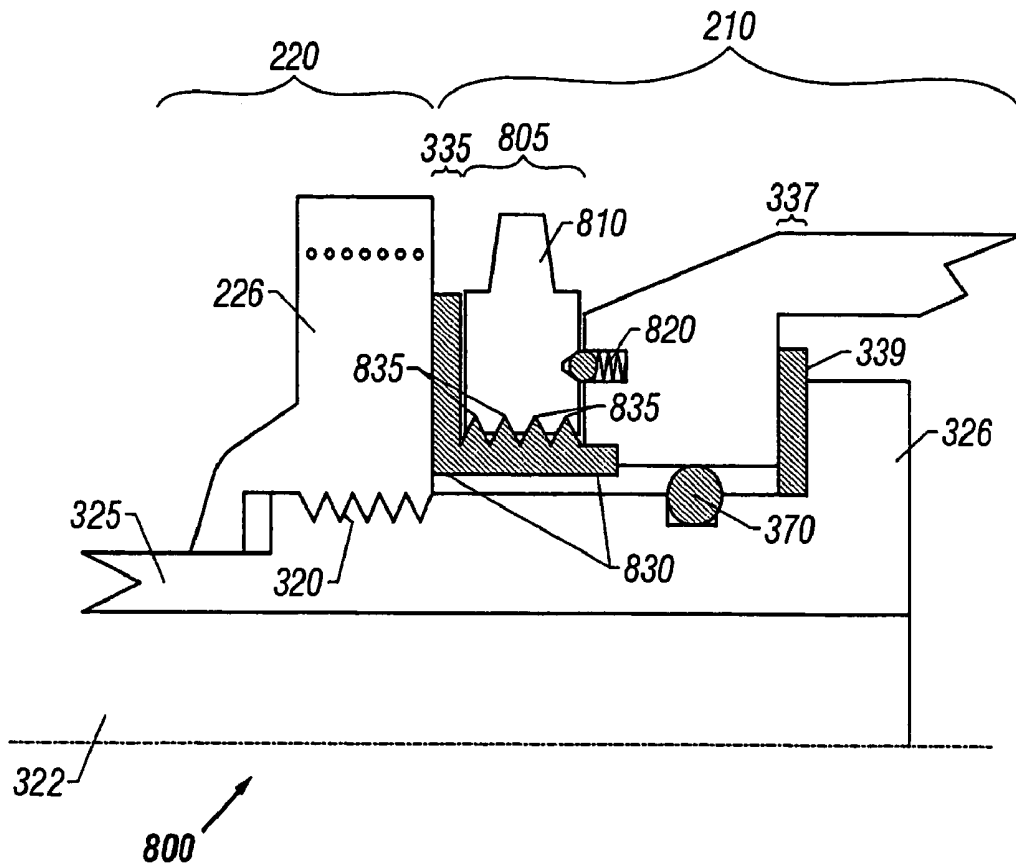


FIG. 5

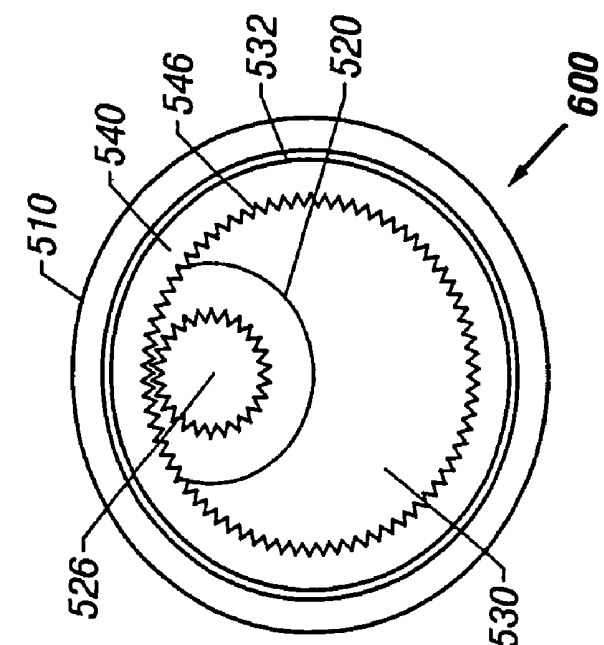


FIG. 7

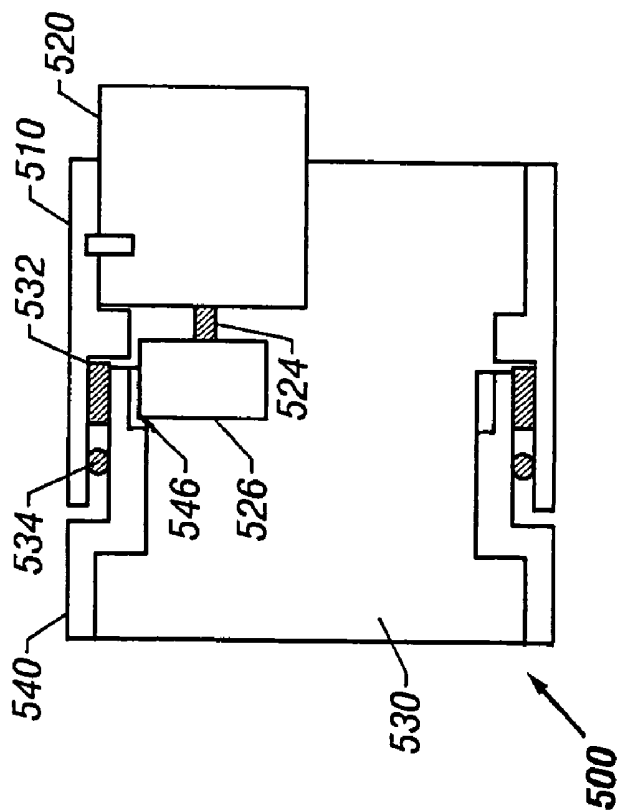


FIG. 6

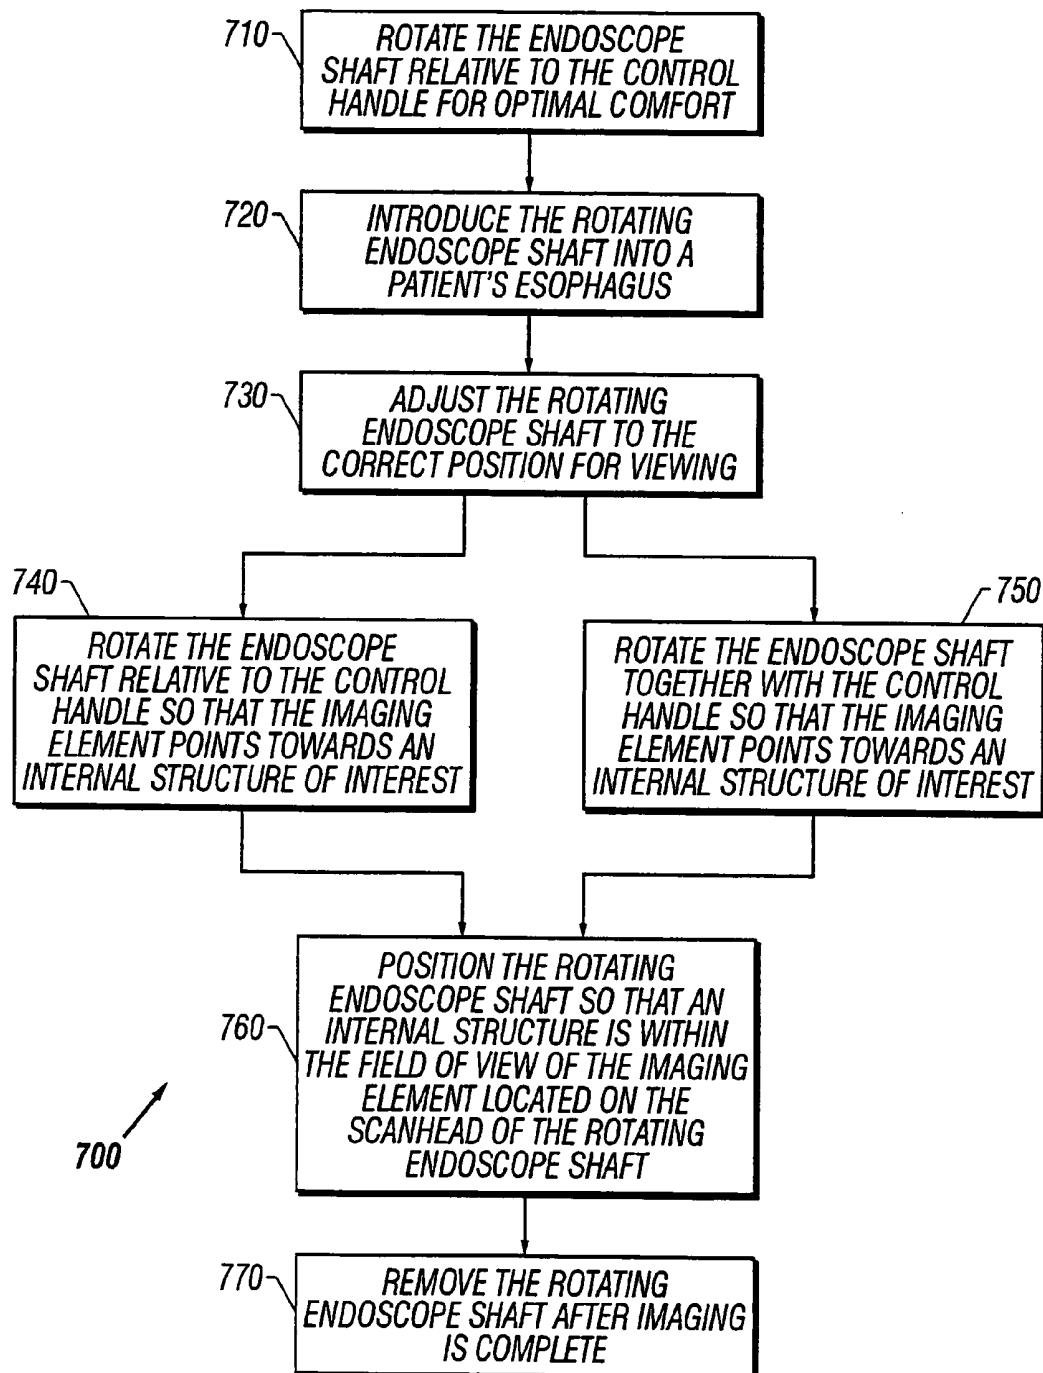


FIG. 8

TRANSESOPHAGEAL ULTRASOUND PROBE HAVING A ROTATING ENDOSCOPE SHAFT

CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a continuation of application Ser. No. 10/317,158, filed Dec. 10, 2002, now U.S. Pat. No. 6,749, 572, which is a continuation of Application No. 09/681,296, filed Mar. 14, 2001 now abandoned.

STATEMENT REGARDING FEDERALLY SPONSORED RESEARCH OR DEVELOPMENT

Not Applicable.

REFERENCE TO MATERIALS ON COMPACT DISC

Not Applicable

BACKGROUND OF THE INVENTION

A preferred embodiment of the present invention generally relates to transesophageal probes, and more particularly relates to an improved transesophageal ultrasound probe having a rotating endoscope shaft.

Various medical conditions affect internal organs and structures. Efficient diagnosis and treatment of these conditions typically require a physician to directly observe a patient's internal organs and structures. For example, diagnosis of various heart ailments often requires a cardiologist to directly observe affected areas of a patient's heart. Instead of more intrusive surgical techniques, ultrasound imaging is often utilized to directly observe images of a patient's internal organs and structures.

Transesophageal Echocardiography (TEE) is one approach to observing a patient's heart through the use of an ultrasound transducer. TEE typically includes a probe, a processing unit, and a monitor. The probe is connected to the processing unit which in turn is connected to the monitor. In operation, the processing unit sends a triggering signal to the probe. The probe then emits ultrasonic signals into the patient's heart. The probe then detects echoes of the previously emitted ultrasonic signals. Then, the probe sends the detected signals to the processing unit which converts the signals into images. The images are then displayed on the monitor. The probe typically includes a semi-flexible endoscope that includes a transducer located near the end of the endoscope.

Typically, during TEE, the endoscope is introduced into the mouth of a patient and positioned in the patient's esophagus. The endoscope is then positioned so that the transducer is in a position to facilitate heart imaging. That is, the endoscope is positioned so that the heart or other internal structure to be imaged is in the direction of view of the transducer. Typically, the transducer sends ultrasonic signals through the esophageal wall that come into contact with the heart or other internal structures. The transducer then receives the ultrasonic signals as they bounce back from various points within the internal structures of the patient. The transducer then sends the received signals back through the endoscope typically via wiring. After the signals travel through the endoscope, the signals enter the processing unit typically via wires connecting the endoscope to the processing unit.

Often, in addition to the heart, it may be desirable to image other internal structures within the body of a patient. Imaging other internal structures may require re-positioning of the probe in order to view the internal organs. Additionally, viewing the heart and/or other internal structures from various angles and perspectives may require re-positioning of the probe.

FIG. 1 illustrates a conventional transesophageal ultrasound probe **100** according to one embodiment of the prior art. The probe **100** includes a control handle **110**, a fixed endoscope shaft **120** fastened to the distal end of the control handle **110**, and a system cable **130** attached to the proximal end of the control handle **110**. The fixed endoscope shaft **120** includes a scanhead **122** located at the distal end of the fixed endoscope shaft **120**. The scanhead **122** includes an imaging element **124**, such as a transducer (not shown). The control handle **110** includes imaging controls **112** mounted on the control handle **110**. The imaging controls **112** include imaging control wheels **114** and scan plane push buttons **116** that control the orientation of the scanhead **122**. The imaging element **124** is connected to a processing unit (not shown) via wiring (not shown) that extends through the scanhead **122** and throughout the length of the body of the probe **100**. The wiring in the probe **100** is then connected via the system cable **130** to the processing unit. The processing unit is then connected via wiring to a monitor (not shown) for display of the image.

In operation, the fixed endoscope shaft **120** of the probe **100** is introduced into the esophagus of a patient. The fixed endoscope shaft **120** is then positioned via the control handle **110** so that the internal structure to be imaged is within the field of view of the imaging element **124** located on, or within, the scanhead **122**. Typically, the probe **100** is axially rotated to position the desired internal structure in the field of view of the imaging element **124**. In order to rotate the endoscope shaft **120**, the entire probe **100** must be rotated. That is, the control handle **110** must be rotated so that the imaging element **124** may image internal structures from different angles and perspectives. For example, to rotate the direction of view **124** of the imaging element of the scanhead **122** by 30°, the control handle **110** typically needs to be rotated 30° because the fixed endoscope shaft **120** is firmly fixed to the control handle **110**. Thus, the fixed endoscope shaft **120** is not allowed to rotate independently of the control handle **110**. Therefore, as the control handle **110** is rotated by 30°, the imaging controls **112** will also be rotated by 30°. Unfortunately, rotating the imaging controls **112** often may cause confusing and/or counter-intuitive operation of the probe **100**. That is, because the imaging controls **112** are fixed, it may be difficult or impossible for an operator to obtain the images he/she desires. Further, observing the resulting images from the physically rotated probe may be confusing. The confusion may lead to misdiagnosis, risks of injury and/or increased time to perform the imaging procedure.

Therefore, a need has existed for a transesophageal ultrasound probe that provides greater and easier access to images of a patient's internal structures. Further, a need has also existed for a transesophageal ultrasound probe that facilitates more intuitive imaging of internal structures from various angles and perspectives.

SUMMARY OF THE INVENTION

The present invention relates to an internal imaging probe for use in a medical imaging system. The probe includes a rotating shaft, such as a rotating endoscope shaft, having an

imaging element, such as a transducer, mounted on the distal end of the rotating shaft. The probe also includes a control handle for controlling the imaging element. Preferably, a rotating tube within the probe extends through the rotating shaft into the control handle. The rotation of the rotating tube causes the rotating shaft to rotate. The rotating shaft rotates relative to, and independently of, the control handle to which it is connected. Washers and O-rings provide low friction connections between the rotating tube located in the probe and the control handle.

Preferably, the rotating shaft is rotated via a rotation control wheel located at the distal end of the control handle. The rotation control wheel is fastened or bonded to the rotating tube so that manual rotation of the control wheel causes the rotating tube, and therefore the rotating shaft, to rotate. Because the rotating shaft rotates, an imaging element located on, or within, the rotating shaft also rotates. The rotating shaft may also be set in a locked position so that the rotating shaft may be configured, or preset, to various rotated positions.

Alternatively, the rotation of the rotating shaft may be fully automated. The automated probe may include a motor fixed to a fixed portion of the shaft, or to the control handle. The motor also includes a driving cog wheel, or gear system, that operatively engages a driven cog wheel, or gear system, attached to a rotating portion of the shaft. The rotation of the rotating shaft may then be controlled by levers, potentiometers, or other such devices located on the control handle.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 illustrates a conventional transesophageal ultrasound probe according to one embodiment of the prior art.

FIG. 2 illustrates a transesophageal ultrasound probe according to a preferred embodiment of the present invention.

FIG. 3 illustrates a transverse cross-sectional view of the transesophageal ultrasound probe of FIG. 2 according to a preferred embodiment of the present invention.

FIG. 4 illustrates an axial cross-sectional view through the rotation control wheel of the transesophageal ultrasound probe of FIG. 2 according to a preferred embodiment of the present invention.

FIG. 5 illustrates a transverse cross-sectional view of the transesophageal ultrasound probe of FIG. 2 with a braking mechanism according to an alternative embodiment of the present invention.

FIG. 6 illustrates a transverse cross-sectional view of a transesophageal ultrasound probe segment according to an alternative embodiment of the present invention.

FIG. 7 illustrates an cross-sectional axial view of the transesophageal ultrasound probe segment of FIG. 6 according to an alternative embodiment of the present invention.

FIG. 8 illustrates a flow chart of a preferred embodiment of the present invention.

DETAILED DESCRIPTION OF THE INVENTION

The foregoing summary, as well as the following detailed description of the preferred embodiments of the present invention, will be better understood when read in conjunction with the appended drawings. For the purpose of illustrating the invention, there are shown in the drawings, embodiments which are presently preferred. It should be

understood, however, that the present invention is not limited to the precise arrangements and instrumentality shown in the attached drawings.

FIG. 2 illustrates a transesophageal ultrasound probe 200 according to a preferred embodiment of the present invention. The probe 200 includes a control handle 210, a rotating endoscope shaft 220 extending from the control handle 210, and a system cable 230 connecting the control handle 210 to a processing unit (not shown). The control handle 210 includes imaging controls 212 mounted on the control handle 210. The imaging controls 212 include imaging control wheels 214 and scan plane push buttons 216 for controlling the movement of an imaging element 224 located on, or within, the distal end of the imaging probe 200. The rotating endoscope shaft 220 includes a scanhead 222. The scanhead 222 includes the imaging element 224, such as a transducer. Preferably, the imaging element is located at the distal end of the rotating endoscope shaft 220. Additionally, the rotating endoscope shaft 220 includes a rotation control wheel 226 fastened to the rotating shaft 220 and located at the distal end of the control handle 210.

FIG. 3 illustrates a transverse cross-sectional view 300 of the transesophageal ultrasound probe 200 of FIG. 2 according to a preferred embodiment of the present invention. The cross sectional view 300 includes the control handle 210, the rotating endoscope shaft 220, a rotating tube 325 having an extended proximal end 326, the rotation control wheel 226, a threaded interface 320, an inner cavity 322, a wheel stop area 335, a washer 338, O-rings 334, a tube stop area 337, and a washer 339. The rotating tube 325 extends throughout the body of the rotating shaft 220 and into the control handle 210. The inner cavity 322 is formed within the rotating tube 325. The rotating tube 325 is fastened to the rotation control wheel 226 at the threaded interface 320. The rotation control wheel 226 abuts the wheel stop area 335 via the washer 338. The washer 338 in turn abuts the control handle 210. The control handle 210 is connected to the rotation tube 325 via the O-rings 334. The control handle 210 abuts the tube stop area 337 via the washer 339. The washer 339 in turn abuts the extended proximal end 326 of the rotation tube 325. The washer 338 and O-rings 334 provide a low-friction connection between the control handle 210 and the rotation control wheel 226. Similarly, the washer 339 and O-rings 334 provide a low-friction connection between the control handle 210 and the extended proximal end 326 of the rotation tube 325. Additionally, the O-rings 334 provide a sealing connection between the control handle 210 and the rotating tube 325.

FIG. 4 illustrates an axial cross-sectional view 400 through the rotation control wheel 226 of the transesophageal ultrasound probe 200 of FIG. 2 according to a preferred embodiment of the present invention. FIG. 4 includes the rotation tube 325 defining the inner cavity 322, the threaded interface 320, a reference line 420 illustrating the circumference of the extended control handle 210 and the control wheel 226.

Referring to FIG. 3, the rotating tube 325 is fastened to the control wheel 226 via the threaded interface 320. Preferably, the rotating tube 325 is securely fastened to the rotation control wheel 226 via the threaded interface 320 with a fastening agent, such as glue or some other fastening agent, that forms a fluid-tight seal. The control wheel 226 is separated from the control handle 210 by the washer 338. For example, the washer may be a low friction plastic washer that fits over the rotating tube 325. Alternatively, the washer 338 may be a locking washer. In addition to providing a low friction interface between the rotation control

wheel 226 and the control handle 210, the washer 338 also provides a seal between the rotation control wheel 226 and the control handle 210. Additionally, the O-rings 334 form a fluid-tight seal between the control handle 210 and the rotating endoscope shaft 220.

The control handle 210 is separated from the proximal end 326 of the rotating tube 325 by the washer 339. Preferably, the diameter of the proximal end 325 of the rotating tube 325 is greater than the diameter of the internally introduced portion of the rotating tube 325. Preferably, the proximal end 325 of the rotating tube 325 abuts the tube stop area 337 when the probe 200 of FIG. 2 is fully assembled.

During assembly, the rotation control wheel 226 is rotated on the thread of the rotating tube 325 while the rotating tube 325 does not rotate, thus introducing the proximal end 326 of the rotating tube 325 into contact with the tube stop area 337 as the rotation control wheel 226 comes into contact with the wheel stop area 335. The washer 338 cushions and seals a low-friction connection between the rotation control wheel 226 and the control handle 210 as the rotation control wheel 226 and the control handle 210 come together. Similarly, the washer 339 cushions and seals a low-friction connection between the proximal end 326 of the rotating tube 325 and the control handle 210 as the proximal end 326 of the rotating tube 325 and the control handle 210 come together.

Once the rotation control wheel 226 has been rotated to its fullest extent, the rotation control wheel 226 is sealed to the rotating tube 325 at the threaded interface 320. Thus, the washer 338 forms a compressive seal between the rotation control wheel 226 and the control handle 210; and the washer 339 forms a compressive seal between the proximal end 326 of the rotating tube 325 and the control handle 210 at the tube stop area 337. Washers and O-rings may be integrated as part of the rotation control wheel 226, rotating tube 325 or the control handle 210 if necessary. For example, if the rotation control wheel 226 is composed of hard plastic, then the washer 338 may not be necessary.

In general, the probe 200 of FIG. 2 may be included in a medical imaging system. Such a medical imaging system may include the probe 200, a processing unit (not shown), and a monitor (not shown). In operation, an internal structure is imaged by the probe 200 and the resultant image is sent to the processing unit for processing and display on the monitor.

Referring again to FIG. 2, in operation, the rotating endoscope shaft 220 is introduced into the patient's esophagus via the patient's mouth in a similar fashion as that of the conventional probe 100 of FIG. 1. Once the rotating endoscope shaft 220 is introduced, the rotating endoscope shaft 220 is positioned such that an internal structure to be imaged is within the field of view of the imaging element 224. The imaging element 224, such as a transducer, located within the scanhead 222 is controlled via the imaging controls 212 located on the control handle 210. The imaging element 224 is connected to the imaging controls 212 via wiring (not shown) within the inner cavity 322 of the probe 200. During imaging, the imaging element 224 of the scanhead 222 sends and receives signals through wiring (not shown) located within the inner cavity 322 of the imaging probe 200 to a processing unit (not shown) via the system cable 230. The processing unit receives the signals via the system cable 230, which is in turn connected to wiring located within the probe 200.

During imaging, the rotating endoscope shaft 220 may be rotated relative to, and independent of, the control handle

210. That is, the control handle 210 may remain in one orientation while the rotating endoscope shaft 220 is rotated about an axis that is common to both the rotating endoscope shaft 220 and the control handle 210. In order to rotate the rotating endoscope shaft 220 about the common axis, the rotation control wheel 226 is turned. Because the rotating tube 325 is fastened to the rotation control wheel 226, rotation of the rotation control wheel 226 causes a corresponding rotation in the rotating tube 325. The rotation of the rotating tube 325 causes the rotating endoscope shaft 220 to rotate. The independent rotation of the rotating endoscope shaft 220 allows the control handle 210 to remain in the same orientation throughout the imaging process while the rotating endoscope shaft 220 rotates to allow the imaging element 224 of the scanhead 222 to image internal structures from different angles and perspectives.

Optionally, the rotating endoscope shaft 220 may be set, or locked, into position at any point throughout its rotation by a locking mechanism (not shown). The locking mechanism may be controlled via the rotation control wheel 226, or additional controls located on the control handle 210. For example, the rotating endoscope shaft 220 may be locked, or set, into a position corresponding to a position that is comfortable and intuitive to a particular physician, cardiologist, or other user of the probe 200. For example, an individual may prefer to position the imaging element 224 fixed to the rotating endoscope shaft 220 at a 30° radial rotation with respect to the imaging controls 212 positioned on the control handle 210 before, and throughout, the imaging process. Alternatively, the rotation of the rotating endoscope shaft 220 may be sufficiently stiff so that a locking mechanism is not necessary.

Also, a physical end-stop may be located on the proximal end 326 of the rotating tube 325. The end-stop may limit the rotation of the rotating tube 325 and therefore, the rotating endoscope shaft 220, to 180° or less in order to prevent twisting the various wires and cables (not shown) located in the inner cavity 322 of the probe 220. The end-stop may be a pin, block, notch, or other stopping mechanism attached to the proximal end 326 of rotating tube 325 that comes into contact with another pin, block, notch, or other stopping mechanism, attached to the interior of the control handle 210.

FIG. 5 illustrates a transverse cross-sectional view 800 of the transesophageal ultrasound probe 200 of FIG. 2 with a low friction braking mechanism 805 according to an alternative embodiment of the present invention. The cross-sectional view 800 includes the control handle 210, the rotating endoscope shaft 220, the rotating tube 325 having the extended proximal end 326, the rotation control wheel 226, the threaded interface 320, the inner cavity 322, the wheel stop area 335, a single O-ring 370, the tube stop area 337, the washer 339, and a low friction braking mechanism 805. The braking mechanism 805 includes a brake handle 810, a brake limit 820, an flanged cylinder brake 830, and a series of threads 835 between the brake handle 810 and the brake 830. The low friction washer 338 of FIG. 3 is replaced by the low friction braking mechanism 805. The brake 830 is threadably fastened onto the rotating braking handle 810 via the threads 835. The brake limit 820 is preferably a spring-ball configuration that limits, or restricts, the rotation of the brake handle 810. The brake limit 820 is positioned within the main body of the control handle 210 and extends into the rotating braking handle 810.

In operation, the brake handle 810 is engaged to brake, or lock, the rotation of the rotating tube 325. Preferably, the brake handle 810 is rotated to brake the rotating tube 325.

Because the brake **830** is threadably fastened onto the brake handle **810**, the brake **830** moves linearly towards, or away from, the rotation control wheel **226** as the brake handle **810** is rotated. As the brake handle **810** rotates in a locking direction, the brake **830** is compressed into the rotation control wheel **226**. The brake **830** brakes the rotation control wheel **226** as the brake **830** is compressed into the rotation control wheel **226**. As the rotation of the rotation control wheel **226** is braked, the rotation of the rotating tube **325** is also braked. The brake limit **820** limits the rotation of the brake handle **810**. For example, the brake limit **820** may include pre-defined locked positions that stop the rotation of the brake handle **810** as the brake handle **810** rotates into one of the locked positions. As the brake handle **810** rotates away from the locking direction, thereby disengaging the brake **830**, the brake **830** moves away from the rotation control wheel **226**. As the brake **830** is disengaged, the rotation control wheel **226** is able to rotate; thus, the rotating tube **325** is able to rotate.

Alternatively, the brake mechanism **805** may include a screw that may be positioned perpendicular to the surface of the rotating tube **325** via a threaded hole in the control handle **210**. As the screw is engaged, the screw moves toward the rotating tube **325**. The screw restricts the rotation of the rotating tube **325** as the screw is threaded through the control handle **210** towards, and into, the rotating tube **325**. The rotating tube **325** may include notches that may receive the screw. As the screw enters the notches on the rotating tube **325**, the rotation of the rotating tube is restricted.

Alternatively, the rotation of the rotating endoscope shaft **220** may be controlled in various ways. For example, the probe **200** may be fully automated. That is, the rotation of the rotating endoscope shaft **220** may be controlled through the use of motors, gears, and/or cog wheels.

FIG. 6 illustrates a transverse cross-sectional view of a transesophageal ultrasound probe segment **500** according to an alternative embodiment of the present invention. The transverse cross-sectional view includes a fixed endoscope shaft **510**, a rotating shaft **540**, bearings **532**, an inner cavity **530**, and an O-ring **534**. The fixed endoscope shaft **510** includes a motor **520** mounted to the interior of the fixed endoscope shaft **510**. The motor **510** includes an axle **524** extending toward the distal end of the probe segment **500** and a driving cog wheel **526** attached at the opposite end of the axle **524** from the motor **510**. The rotating shaft **540** includes a driven cog wheel **546** extending into the inner cavity **530**. The bearings **532** encircle the fixed endoscope shaft **510** and provide a low-friction connection between the fixed endoscope shaft **510** and the rotating shaft **540**. The inner cavity **530** is formed within the probe segment **500** and extends through the fixed endoscope shaft **510** and the rotating shaft **540**. The O-ring **534** encircles the fixed endoscope shaft **510** and provides a fluid-tight seal between the fixed endoscope shaft **510** and the rotating shaft **540**.

FIG. 7 illustrates an axial cross-sectional view **600** of the transesophageal ultrasound probe segment **500** of FIG. 6 according to an alternative embodiment of the present invention. The cross-sectional axial view **600** includes the fixed endoscope shaft **510**, the motor **520**, the driving cog wheel **526**, the inner cavity **530**, the bearing **532**, the rotating shaft **540** and the driven cog wheel **546**.

In operation, the rotating shaft **540** is engaged by controls (not shown), such as buttons, levers, or potentiometers, located on the control handle **210**. The motor **520** is electrically connected to the controls via wiring. When activated, the motor **520** rotates the axle **524**, which in turn, rotates the driving cog wheel **526**. The driving cog wheel

526 operatively engages the driven cog wheel **546**. Therefore, as the driving cog wheel **526** rotates, the driven cog wheel **546** rotates in the same direction as that of the driving cog wheel **526**. The rotation of the driven cog wheel **546** in turn causes the rotating shaft **540** to rotate in the same direction as that of the driven cog wheel **546**. The scanhead **222** located on the distal end of rotating shaft **540** therefore rotates as the rotating shaft **540** rotates.

The interface between the rotating shaft **540** and the fixed endoscope shaft **510** may be located at various points of the probe segment **500**. For example, the interface between the rotating shaft **540** and the fixed endoscope shaft **510** may be located near the control handle **210**, near the scanhead **222**, or positioned at various points between the control handle **210** and the scanhead **222**. Alternatively, the fixed endoscope shaft **510** may be part of the control handle **210** of the probe **200** of FIG. 2. Thus, the motor **520** may be attached to the interior of the control handle **210**.

FIG. 8 illustrates a flow chart **700** of a preferred embodiment of the present invention. First, at step **710**, a physician rotates the endoscope shaft **220** relative to the control handle **210** to suit the physician's preference. That is, the physician rotates the endoscope shaft **220** at step **710** for optimal comfort. Next, at step **720**, the physician introduces the rotating endoscope shaft **220** into a patient's esophagus. The physician then adjusts, or positions, the rotating endoscope shaft **220** to a suitable position for viewing at step **730**. That is, the physician adjusts, or positions, the rotating endoscope shaft **220** to a suitable position for viewing a particular internal structure.

The physician then rotates the endoscope shaft **220** so that the imaging element **224** points towards an internal structure of interest. The physician may either rotate the endoscope shaft **220** relative to the control handle **210** via the rotation control wheel **226** at step **740**, or the physician may rotate the endoscope shaft **220** together with the control handle **210**. Next, at step **760**, the physician positions the rotating endoscope shaft **220** so that an internal structure to be imaged is within the field of view of the imaging element **224** located on the scanhead **222** of the rotating endoscope shaft **220**. At step **760**, the rotating endoscope shaft **220** is positioned via imaging controls **212** or other controls on the control handle **210** so that an internal structure is within the field of view of the imaging element **224** located on the scanhead **222**. After the physician positions the rotating endoscope shaft **220** so that an internal structure is within the field of view of the imaging element **224**, the internal structure is imaged. Finally, at step **770**, the physician removes the rotating endoscope shaft **220** from the esophagus of the patient after imaging is complete.

Alternatively, the physician may rotate the rotating endoscope shaft **220** via the rotation control wheel **226** during the imaging process to view different internal structures within the body of the patient. Also, the physician may rotate the rotating endoscope shaft **220** via the rotation control wheel **226** during the imaging process to view the original internal structure from a different perspective.

Thus the present invention provides an improved transesophageal ultrasound probe that provides greater and easier access to images of internal structures within a patient because the probe includes a rotating shaft that rotates independently of the probe's control handle. The independent rotation of the rotating shaft provides greater imaging access. Further, the transesophageal ultrasound probe having a rotating endoscope shaft facilitates more intuitive images of internal structures from various angles and perspectives. Additionally, various other imaging methods, such as live

9

video, may be used with the present invention. Also, the present invention is not limited to imaging. For example, the present invention may also be utilized in surgical applications such as trans-rectal prostate treatment.

While particular elements, embodiments and applications of the present invention have been shown and described, it is understood that the invention is not limited thereto since modifications may be made by those skilled in the art, particularly in light of the foregoing teaching. It is therefore contemplated by the appended claims to cover such modifications and incorporate those features which come within the spirit and scope of the invention.

The invention claimed is:

1. An internal imaging probe including:

a rotating endoscope shaft having an imaging element;

a fixed endoscope shaft;

a driving cog wheel; and

a driven cog wheel attached to said rotating endoscope shaft;

said driving cog wheel operatively engaging said driven cog wheel to rotate said rotating endoscope shaft relative to said fixed endoscope shaft.

2. The probe of claim 1 further including a control handle, wherein said control handle includes said fixed endoscope shaft.

3. The probe of claim 2, wherein said motor is located within said fixed endoscope shaft.

4. The probe of claim 1 further including a control handle, wherein a portion of said fixed endoscope shaft protrudes from said control handle.

5. The probe of claim 4, wherein said motor is located within said fixed endoscope shaft.

6. The probe of claim 1, wherein said motor is located within said fixed endoscope shaft.

10

7. The probe of claim 1 further including an O-ring forming a seal between said rotating endoscope shaft and said fixed endoscope shaft.

8. A medical imaging system including a probe for imaging internal structures of a patient, said probe including:

a rotating endoscope shaft having an imaging element;

a fixed endoscope shaft;

a motor affixed to said fixed endoscope shaft;

a driving cog wheel attached to said motor; and

a driven cog wheel attached to said rotating endoscope shaft;

said driving cog wheel operatively engaging said driven cog wheel to rotate said rotating endoscope shaft relative to said fixed endoscope shaft.

9. The probe of claim 8 further including a control handle, wherein said control handle includes said fixed endoscope shaft.

10. The system of claim 8 further including a control handle, wherein a portion of said fixed endoscope shaft protrudes from said control handle.

11. The probe of claim 10, wherein said motor is located within said fixed endoscope shaft.

12. The probe of claim 8, wherein said motor is located within said fixed endoscope shaft.

13. The probe of claim 9, wherein said motor is located within said fixed endoscope shaft.

14. The system of claim 8 further including an O-ring forming a seal between said rotating endoscope shaft and said fixed endoscope shaft.

* * * * *

| | | | |
|----------------|---|---------|------------|
| 专利名称(译) | 经食管超声探头具有旋转内窥镜轴 | | |
| 公开(公告)号 | US7144371 | 公开(公告)日 | 2006-12-05 |
| 申请号 | US10/805819 | 申请日 | 2004-03-22 |
| [标]申请(专利权)人(译) | EDWARDSSEN STEPHEN DODGE JORDFALD DAG | | |
| 申请(专利权)人(译) | EDWARDSSEN STEPHEN DODGE JORDFALD DAG | | |
| 当前申请(专利权)人(译) | 通用电气医疗系统全球性技术公司，有限责任公司 | | |
| [标]发明人 | EDWARDSSEN STEPHEN DODGE JORDFALD DAG | | |
| 发明人 | EDWARDSSEN, STEPHEN DODGE JORDFALD, DAG | | |
| IPC分类号 | A61B8/14 A61B8/12 | | |
| CPC分类号 | A61B1/00177 A61B1/00183 A61B1/273 A61B8/12 A61B8/4461 | | |
| 审查员(译) | 伊玛目阿里 | | |
| 其他公开文献 | US20040176691A1 | | |
| 外部链接 | Espacenet USPTO | | |

摘要(译)

经食道超声探头，用于通过位于旋转内窥镜轴的远端上的成像元件对内部结构成像。探针包括旋转内窥镜，该旋转内窥镜具有安装在旋转内窥镜轴的远端上的成像元件。探针还包括用于控制成像控制的控制手柄和延伸通过旋转内窥镜轴并进入控制手柄的旋转管。旋转轴相对于控制手柄旋转并且独立于控制手柄旋转。优选地，旋转轴通过旋转控制轮旋转。旋转控制轮紧固或结合到旋转管，使得控制轮的手动旋转使旋转管旋转，因此旋转轴旋转。因为旋转内窥镜轴旋转，位于旋转轴上或旋转轴内的成像元件也旋转。

