



US009192790B2

(12) **United States Patent**
Hastings et al.

(10) **Patent No.:** **US 9,192,790 B2**
(45) **Date of Patent:** **Nov. 24, 2015**

(54) **FOCUSED ULTRASONIC RENAL
DENERVATION**

2007/003; A61B 8/4488; A61B 8/12; A61B
8/0891; A61B 18/0206; A61B 2018/00434;
A61B 2018/00404; A61B 2018/00511; A61B
2019/528

(75) Inventors: **Roger Hastings**, Maple Grove, MN
(US); **Allan C. Shuros**, St. Paul, MN
(US); **Frank Ingle**, Palo Alto, CA (US);
Mark A. Hollingsworth, Bloomington,
MN (US)

USPC 600/439, 471; 601/3; 606/27
See application file for complete search history.

(73) Assignee: **Boston Scientific Scimed, Inc.**, Maple
Grove, MN (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 207 days.

(56) **References Cited**

U.S. PATENT DOCUMENTS

164,184 A 6/1875 Kidder
1,167,014 A 1/1916 O'Brien

(Continued)

FOREIGN PATENT DOCUMENTS

DE 10038737 A1 2/2002
EP 1053720 A1 11/2000

(Continued)

OTHER PUBLICATIONS

Gentry et al., "Combined 3D Intracardiac Echo and Ultrasound Ablation", Medical Imaging 2003: Ultrasonic and Signal Processing, vol. 5035, 2003, pp. 166-173.

(Continued)

Related U.S. Application Data

(60) Provisional application No. 61/324,164, filed on Apr.
14, 2010.

(51) **Int. Cl.**
A61B 8/00 (2006.01)
A61N 7/02 (2006.01)
A61B 8/08 (2006.01)
(Continued)

(52) **U.S. Cl.**
CPC **A61N 7/022** (2013.01); **A61B 8/0891**
(2013.01); **A61B 8/12** (2013.01); **A61B 8/4488**
(2013.01); **A61B 18/0206** (2013.01); **A61B**
2018/00404 (2013.01); **A61B 2018/00434**
(2013.01); **A61B 2018/00511** (2013.01);
(Continued)

(58) **Field of Classification Search**
CPC A61N 7/022; A61N 2007/0095; A61N


Primary Examiner — Jonathan Cwern

(74) *Attorney, Agent, or Firm* — Kacvinsky Daisak Bluni
PLLC

(57) **ABSTRACT**

Acoustic energy is delivered to innervated vascular that contributes to renal sympathetic nerve activity, such as innervated tissue of the renal artery and abdominal aorta. Focused acoustic energy is delivered via an intravascular device of sufficient power to ablate innervated renal or aortal tissue. Focused acoustic energy may be delivered via an intravascular or extracorporeal device to image and locate target innervated renal or aortal tissue. Intravascular, extravascular, or transvascular focused ultrasound devices provide for high precision denervation of innervated vascular to terminate renal sympathetic nerve activity.

18 Claims, 22 Drawing Sheets

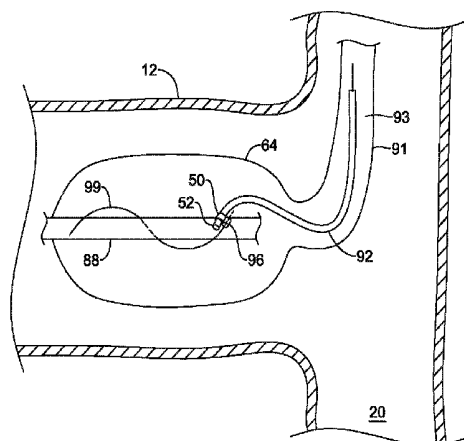

(51)	Int. Cl.			5,300,068 A	4/1994	Rosar et al.
	<i>A61B 8/12</i>	(2006.01)		5,301,683 A	4/1994	Durkan
	<i>A61B 18/02</i>	(2006.01)		5,304,115 A	4/1994	Pflueger et al.
	<i>A61B 19/00</i>	(2006.01)		5,304,121 A	4/1994	Sahatjian
	<i>A61N 7/00</i>	(2006.01)		5,304,171 A	4/1994	Gregory et al.
(52)	U.S. Cl.			5,304,173 A	4/1994	Kittrell et al.
	<i>A61B 18/00</i>	(2006.01)		5,306,250 A	4/1994	March et al.
	CPC	<i>A61B 2019/528</i> (2013.01); <i>A61N 2007/003</i>		5,312,328 A	5/1994	Nita et al.
		(2013.01); <i>A61N 2007/0095</i> (2013.01)		5,314,466 A	5/1994	Stern et al.
				5,322,064 A	6/1994	Lundquist
(56)	References Cited			5,324,255 A	6/1994	Passafaro et al.
	U.S. PATENT DOCUMENTS			5,326,341 A	7/1994	Lew et al.
				5,326,342 A	7/1994	Pflueger et al.
				5,330,518 A	7/1994	Neilson et al.
				5,333,614 A	8/1994	Feiring
				5,342,292 A	8/1994	Nita et al.
				5,344,395 A	9/1994	Whalen et al.
				5,364,392 A	11/1994	Warner et al.
				5,365,172 A	11/1994	Hrovat et al.
				5,368,557 A	11/1994	Nita et al.
				5,368,558 A	11/1994	Nita et al.
				5,380,274 A	1/1995	Nita et al.
				5,380,319 A	1/1995	Saito et al.
				5,382,228 A	1/1995	Nita et al.
				5,383,874 A	1/1995	Jackson et al.
				5,383,917 A	1/1995	Desai et al.
				5,397,301 A	3/1995	Pflueger et al.
				5,397,339 A	3/1995	Desai
				5,401,272 A	3/1995	Perkins et al.
				5,403,311 A	4/1995	Abele et al.
				5,405,318 A	4/1995	Nita et al.
				5,405,346 A	4/1995	Grundy et al.
				5,409,000 A	4/1995	Imran
				5,417,672 A	5/1995	Nita et al.
				5,419,767 A	5/1995	Eggers et al.
				5,427,118 A	6/1995	Nita et al.
				5,432,876 A	7/1995	Appeldorn et al.
				5,441,498 A	8/1995	Perkins et al.
				5,447,509 A	9/1995	Mills et al.
				5,451,207 A	9/1995	Yock et al.
				5,453,091 A	9/1995	Taylor et al.
				5,454,788 A	10/1995	Walker et al.
				5,454,809 A	10/1995	Janssen
				5,455,029 A	10/1995	Hartman et al.
				5,456,682 A	10/1995	Edwards et al.
				5,457,042 A	10/1995	Hartman et al.
				5,471,982 A	12/1995	Edwards et al.
				5,474,530 A	12/1995	Passafaro et al.
				5,478,351 A	12/1995	Meade et al.
				5,496,311 A	3/1996	Abele et al.
				5,496,312 A	3/1996	Klicek et al.
				5,498,261 A	3/1996	Strul
				5,505,201 A	4/1996	Grill et al.
				5,505,730 A	4/1996	Edwards
				5,507,744 A	4/1996	Tay et al.
				5,522,873 A	6/1996	Jackman et al.
				5,531,520 A	7/1996	Grimson et al.
				5,540,656 A	7/1996	Pflueger et al.
				5,540,679 A	7/1996	Fram et al.
				5,540,681 A	7/1996	Strul et al.
				5,542,917 A	8/1996	Nita et al.
				5,545,161 A	8/1996	Imran
				5,562,100 A	10/1996	Kittrell et al.
				5,571,122 A	11/1996	Kelly et al.
				5,571,151 A	11/1996	Gregory
				5,573,531 A	11/1996	Gregory et al.
				5,573,533 A	11/1996	Strul
				5,584,831 A	12/1996	McKay
				5,584,872 A	12/1996	Lafontaine et al.
				5,588,962 A	12/1996	Nicholas et al.
				5,599,346 A	2/1997	Edwards et al.
				5,601,526 A	2/1997	Chapelon et al.
				5,609,606 A	3/1997	O'Boyle et al.
				5,626,576 A	5/1997	Janssen
				5,630,837 A	5/1997	Crowley
				5,637,090 A	6/1997	McGee et al.
				5,643,255 A	7/1997	Organ
				5,643,297 A	7/1997	Nordgren et al.
				5,647,847 A	7/1997	Lafontaine et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

5,649,923	A	7/1997	Gregory et al.	5,871,524	A	2/1999	Knowlton et al.
5,651,780	A	7/1997	Jackson et al.	5,875,782	A	3/1999	Ferrari et al.
5,653,684	A	8/1997	Laptewicz et al.	5,876,369	A	3/1999	Houser
5,662,671	A	9/1997	Barbut et al.	5,876,374	A	3/1999	Alba et al.
5,665,062	A	9/1997	Houser	5,876,397	A	3/1999	Edelman et al.
5,665,098	A	9/1997	Kelly et al.	5,879,348	A	3/1999	Owens et al.
5,666,964	A	9/1997	Meilus	5,891,114	A	4/1999	Chien et al.
5,667,490	A	9/1997	Keith et al.	5,891,135	A	4/1999	Jackson et al.
5,672,174	A	9/1997	Gough et al.	5,891,136	A	4/1999	McGee et al.
5,676,693	A	10/1997	Lafontaine	5,891,138	A	4/1999	Tu et al.
5,678,296	A	10/1997	Fleischhacker et al.	5,895,378	A	4/1999	Nita
5,681,282	A	10/1997	Eggers et al.	5,897,552	A	4/1999	Edwards et al.
RE35,656	E	11/1997	Feinberg et al.	5,902,328	A	5/1999	Lafontaine et al.
5,688,266	A	11/1997	Edwards et al.	5,904,651	A	5/1999	Swanson et al.
5,693,015	A	12/1997	Walker et al.	5,904,667	A	5/1999	Falwell et al.
5,693,029	A	12/1997	Leonhardt et al.	5,904,697	A	5/1999	Gifford et al.
5,693,043	A	12/1997	Kittrell et al.	5,904,709	A	5/1999	Arndt et al.
5,693,082	A	12/1997	Warner et al.	5,906,614	A	5/1999	Stern et al.
5,695,504	A	12/1997	Gifford et al.	5,906,623	A	5/1999	Peterson
5,697,369	A	12/1997	Long, Jr. et al.	5,906,636	A	5/1999	Casscells et al.
5,697,909	A	12/1997	Eggers et al.	5,916,192	A	6/1999	Nita et al.
5,702,386	A	12/1997	Stern et al.	5,916,227	A	6/1999	Keith et al.
5,702,433	A	12/1997	Taylor et al.	5,916,239	A	6/1999	Geddes et al.
5,706,809	A	1/1998	Littmann et al.	5,919,219	A	7/1999	Knowlton et al.
5,713,942	A	2/1998	Stern et al.	5,924,424	A	7/1999	Stevens et al.
5,715,819	A	2/1998	Svenson et al.	5,925,038	A	7/1999	Panescu et al.
5,735,846	A	4/1998	Panescu et al.	5,934,284	A	8/1999	Plaia et al.
5,741,214	A	4/1998	Ouchi et al.	5,935,063	A	8/1999	Nguyen
5,741,248	A	4/1998	Stern et al.	5,938,670	A	8/1999	Keith et al.
5,741,249	A	4/1998	Moss et al.	5,947,977	A	9/1999	Slepian et al.
5,743,903	A	4/1998	Stern et al.	5,948,011	A	9/1999	Knowlton et al.
5,748,347	A	5/1998	Erickson	5,951,494	A	9/1999	Wang et al.
5,749,914	A	5/1998	Janssen	5,951,539	A	9/1999	Nita et al.
5,755,682	A	5/1998	Knudson et al.	5,954,717	A	9/1999	Behl et al.
5,755,715	A	5/1998	Stern et al.	5,957,882	A	9/1999	Nita et al.
5,755,753	A	5/1998	Knowlton et al.	5,957,941	A	9/1999	Ream et al.
5,769,847	A	6/1998	Panescu et al.	5,957,969	A	9/1999	Warner et al.
5,769,880	A	6/1998	Truckai et al.	5,961,513	A	10/1999	Swanson et al.
5,775,338	A	7/1998	Hastings	5,964,757	A	10/1999	Ponzi et al.
5,776,174	A	7/1998	Van Tassel	5,967,976	A	10/1999	Larsen et al.
5,779,698	A	7/1998	Clayman et al.	5,967,978	A	10/1999	Littmann et al.
5,782,760	A	7/1998	Schaer	5,967,984	A	10/1999	Chu et al.
5,785,702	A	7/1998	Murphy et al.	5,971,975	A	10/1999	Mills et al.
5,797,849	A	8/1998	Vesely et al.	5,972,026	A	10/1999	Laufer et al.
5,797,903	A	8/1998	Swanson et al.	5,980,563	A	11/1999	Tu et al.
5,800,484	A	9/1998	Gough et al.	5,989,208	A	11/1999	Nita et al.
5,800,494	A	9/1998	Campbell et al.	5,989,284	A	11/1999	Laufer
5,810,802	A	9/1998	Panescu et al.	5,993,462	A	11/1999	Pomeranz et al.
5,810,803	A	9/1998	Moss et al.	5,997,497	A	12/1999	Nita et al.
5,810,810	A	9/1998	Tay et al.	5,999,678	A	12/1999	Murphy-Chutorian et al.
5,817,092	A	10/1998	Behl	6,004,269	A	12/1999	Crowley et al.
5,817,113	A	10/1998	Gifford et al.	6,004,316	A	12/1999	Laufer et al.
5,817,144	A	10/1998	Gregory et al.	6,007,514	A	12/1999	Nita
5,823,956	A	10/1998	Roth et al.	6,010,522	A	1/2000	Barbut et al.
5,827,203	A	10/1998	Nita et al.	6,013,033	A	1/2000	Berger et al.
5,827,268	A	10/1998	Laufer	6,014,590	A	1/2000	Wayne et al.
5,829,447	A	11/1998	Stevens et al.	6,022,309	A	2/2000	Celliers et al.
5,830,213	A	11/1998	Panescu et al.	6,024,740	A	2/2000	Lesh et al.
5,830,222	A	11/1998	Makower	6,030,611	A	2/2000	Gorecki et al.
5,832,228	A	11/1998	Holden et al.	6,032,675	A	3/2000	Rubinsky et al.
5,833,593	A	11/1998	Liprie	6,033,397	A	3/2000	Laufer et al.
5,836,874	A	11/1998	Swanson et al.	6,033,398	A	3/2000	Farley et al.
5,840,076	A	11/1998	Swanson et al.	6,036,687	A	3/2000	Laufer et al.
5,843,016	A	12/1998	Lugnani et al.	6,036,689	A	3/2000	Tu et al.
5,846,238	A	12/1998	Jackson et al.	6,041,260	A	3/2000	Stern et al.
5,846,239	A	12/1998	Swanson et al.	6,050,994	A	4/2000	Sherman et al.
5,846,245	A	12/1998	McCarthy et al.	6,056,744	A	5/2000	Edwards
5,848,969	A	12/1998	Panescu et al.	6,056,746	A	5/2000	Goble et al.
5,853,411	A	12/1998	Wayne et al.	6,063,085	A	5/2000	Tay et al.
5,855,614	A	1/1999	Stevens et al.	6,066,096	A	5/2000	Smith et al.
5,860,974	A	1/1999	Abele	6,066,139	A	5/2000	Ryan et al.
5,865,801	A	2/1999	Houser	6,068,638	A	5/2000	Makower
5,868,735	A	2/1999	Lafontaine et al.	6,068,653	A	5/2000	Lafontaine
5,868,736	A	2/1999	Swanson et al.	6,071,277	A	6/2000	Farley et al.
5,871,483	A	2/1999	Jackson et al.	6,071,278	A	6/2000	Panescu et al.
				6,078,839	A	6/2000	Carson
				6,079,414	A	6/2000	Roth
				6,080,171	A	6/2000	Keith et al.
				6,081,749	A	6/2000	Ingle et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,086,581	A	7/2000	Reynolds et al.	6,293,942	B1	9/2001	Goble et al.
6,093,166	A	7/2000	Knudson et al.	6,293,943	B1	9/2001	Panescu et al.
6,096,021	A	8/2000	Helm et al.	6,296,619	B1	10/2001	Brisken et al.
6,099,526	A	8/2000	Wayne et al.	6,298,256	B1	10/2001	Meyer
6,102,908	A	8/2000	Tu et al.	6,299,379	B1	10/2001	Lewis
6,106,477	A	8/2000	Miesel et al.	6,299,623	B1	10/2001	Wulfman
6,110,187	A	8/2000	Donlon	6,309,379	B1	10/2001	Willard et al.
6,114,311	A	9/2000	Parmacek et al.	6,309,399	B1	10/2001	Barbut et al.
6,117,101	A	9/2000	Diederich et al.	6,311,090	B1	10/2001	Knowlton
6,117,128	A	9/2000	Gregory	6,317,615	B1	11/2001	KenKnight et al.
6,120,476	A	9/2000	Fung et al.	6,319,242	B1	11/2001	Patterson et al.
6,120,516	A	9/2000	Selmon et al.	6,319,251	B1	11/2001	Tu et al.
6,121,775	A	9/2000	Pearlman	6,322,559	B1	11/2001	Daulton et al.
6,123,679	A	9/2000	Lafaut et al.	6,325,797	B1	12/2001	Stewart et al.
6,123,682	A	9/2000	Knudson et al.	6,325,799	B1	12/2001	Goble
6,123,702	A	9/2000	Swanson et al.	6,328,699	B1	12/2001	Eigler et al.
6,123,703	A	9/2000	Tu et al.	6,346,074	B1	2/2002	Roth
6,123,718	A	9/2000	Tu et al.	6,346,104	B2	2/2002	Daly et al.
6,129,725	A	10/2000	Tu et al.	6,350,248	B1	2/2002	Knudson et al.
6,135,997	A	10/2000	Laufer et al.	6,350,276	B1	2/2002	Knowlton
6,142,991	A	11/2000	Schatzberger et al.	6,353,751	B1	3/2002	Swanson et al.
6,142,993	A	11/2000	Wayne et al.	6,355,029	B1	3/2002	Joye et al.
6,149,647	A	11/2000	Tu et al.	6,357,447	B1	3/2002	Swanson et al.
6,152,899	A	11/2000	Farley et al.	6,361,519	B1	3/2002	Knudson et al.
6,152,912	A	11/2000	Jansen et al.	6,364,840	B1	4/2002	Crowley
6,156,046	A	12/2000	Passafaro et al.	6,371,965	B2	4/2002	Gifford, III et al.
6,158,250	A	12/2000	Tibbals et al.	6,375,668	B1	4/2002	Gifford et al.
6,159,187	A	12/2000	Park et al.	6,377,854	B1	4/2002	Knowlton
6,159,225	A	12/2000	Makower	6,377,855	B1	4/2002	Knowlton
6,161,048	A	12/2000	Sluijter et al.	6,379,352	B1	4/2002	Reynolds et al.
6,162,184	A	12/2000	Swanson et al.	6,379,373	B1	4/2002	Sawhney et al.
6,165,163	A	12/2000	Chien et al.	6,381,497	B1	4/2002	Knowlton
6,165,172	A	12/2000	Farley et al.	6,381,498	B1	4/2002	Knowlton
6,165,187	A	12/2000	Reger et al.	6,383,151	B1	5/2002	Diederich et al.
6,168,594	B1	1/2001	Lafontaine et al.	6,387,105	B1	5/2002	Gifford, III et al.
6,171,321	B1	1/2001	Gifford, III et al.	6,387,380	B1	5/2002	Knowlton
6,179,832	B1	1/2001	Jones et al.	6,389,311	B1	5/2002	Wayne et al.
6,179,835	B1	1/2001	Panescu et al.	6,389,314	B2	5/2002	Feiring
6,179,859	B1	1/2001	Bates et al.	6,391,024	B1	5/2002	Sun et al.
6,183,468	B1	2/2001	Swanson et al.	6,394,096	B1	5/2002	Constantz
6,183,486	B1	2/2001	Snow et al.	6,394,956	B1	5/2002	Chandrasekaran et al.
6,190,379	B1	2/2001	Heuser et al.	6,398,780	B1	6/2002	Farley et al.
6,191,862	B1	2/2001	Swanson et al.	6,398,782	B1	6/2002	Pecor et al.
6,197,021	B1	3/2001	Panescu et al.	6,398,792	B1	6/2002	O'Connor
6,200,266	B1	3/2001	Shokrollahi et al.	6,401,720	B1	6/2002	Stevens et al.
6,203,537	B1	3/2001	Adrian	6,402,719	B1	6/2002	Ponzi et al.
6,203,561	B1	3/2001	Ramee et al.	6,405,090	B1	6/2002	Knowlton
6,210,406	B1	4/2001	Webster	6,409,723	B1	6/2002	Edwards
6,211,247	B1	4/2001	Goodman	6,413,255	B1	7/2002	Stern
6,217,576	B1	4/2001	Tu et al.	6,421,559	B1	7/2002	Pearlman
6,219,577	B1	4/2001	Brown, III et al.	6,423,057	B1	7/2002	He et al.
6,228,076	B1	5/2001	Winston et al.	6,425,867	B1	7/2002	Vaezy et al.
6,228,109	B1	5/2001	Tu et al.	6,425,912	B1	7/2002	Knowlton
6,231,516	B1	5/2001	Keilman et al.	6,427,118	B1	7/2002	Suzuki
6,231,587	B1	5/2001	Makower	6,428,534	B1	8/2002	Joye et al.
6,235,044	B1	5/2001	Root et al.	6,428,536	B2	8/2002	Panescu et al.
6,236,883	B1	5/2001	Ciacchio et al.	6,430,446	B1	8/2002	Knowlton
6,237,605	B1	5/2001	Vaska et al.	6,432,102	B2	8/2002	Joye et al.
6,238,389	B1	5/2001	Paddock et al.	6,436,056	B1	8/2002	Wang et al.
6,238,392	B1	5/2001	Long	6,438,424	B1	8/2002	Knowlton
6,241,666	B1	6/2001	Pomeranz et al.	6,440,125	B1	8/2002	Rentrop
6,241,753	B1	6/2001	Knowlton	6,442,413	B1	8/2002	Silver
6,245,020	B1	6/2001	Moore et al.	6,443,965	B1	9/2002	Gifford, III et al.
6,245,045	B1	6/2001	Stratienko	6,445,939	B1	9/2002	Swanson et al.
6,248,126	B1	6/2001	Lesser et al.	6,447,505	B2	9/2002	McGovern et al.
6,251,128	B1	6/2001	Knopp et al.	6,447,509	B1	9/2002	Bonnet et al.
6,258,087	B1	7/2001	Edwards et al.	6,451,034	B1	9/2002	Gifford, III et al.
6,273,886	B1	8/2001	Edwards et al.	6,451,044	B1	9/2002	Naghavi et al.
6,280,466	B1	8/2001	Kugler et al.	6,453,202	B1	9/2002	Knowlton
6,283,935	B1	9/2001	Laufer et al.	6,454,737	B1	9/2002	Nita et al.
6,283,959	B1	9/2001	Lalonde et al.	6,454,757	B1	9/2002	Nita et al.
6,284,743	B1	9/2001	Parmacek et al.	6,454,775	B1	9/2002	Demarais et al.
6,287,323	B1	9/2001	Hammerslag	6,458,098	B1	10/2002	Kanesaka
6,290,696	B1	9/2001	Lafontaine	6,461,378	B1	10/2002	Knowlton
6,292,695	B1	9/2001	Webster, Jr. et al.	6,468,276	B1	10/2002	McKay
				6,468,297	B1	10/2002	Williams et al.
				6,470,216	B1	10/2002	Knowlton
				6,470,219	B1	10/2002	Edwards et al.
				6,471,696	B1	10/2002	Berube et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,475,213	B1	11/2002	Whayne et al.	6,666,858	B2	12/2003	Lafontaine
6,475,215	B1	11/2002	Tanrisever	6,666,863	B2	12/2003	Wentzel et al.
6,475,238	B1	11/2002	Fedida et al.	6,669,655	B1	12/2003	Acker et al.
6,477,426	B1	11/2002	Fenn et al.	6,669,692	B1	12/2003	Nelson et al.
6,480,745	B2	11/2002	Nelson et al.	6,673,040	B1	1/2004	Samson et al.
6,481,704	B1	11/2002	Koster et al.	6,673,064	B1	1/2004	Rentrop
6,482,202	B1	11/2002	Goble et al.	6,673,066	B2	1/2004	Werneth
6,484,052	B1	11/2002	Visuri et al.	6,673,090	B2	1/2004	Root et al.
6,485,489	B2	11/2002	Teirstein et al.	6,673,101	B1	1/2004	Fitzgerald et al.
6,488,679	B1	12/2002	Swanson et al.	6,673,290	B1	1/2004	Whayne et al.
6,489,307	B1	12/2002	Phillips et al.	6,676,678	B2	1/2004	Gifford, III et al.
6,491,705	B2	12/2002	Gifford, III et al.	6,679,268	B2	1/2004	Stevens et al.
6,494,891	B1	12/2002	Cornish et al.	6,681,773	B2	1/2004	Murphy et al.
6,497,711	B1	12/2002	Plaia et al.	6,682,541	B1	1/2004	Gifford, III et al.
6,500,172	B1	12/2002	Panescu et al.	6,684,098	B2	1/2004	Oshio et al.
6,500,174	B1	12/2002	Maguire et al.	6,685,732	B2	2/2004	Kramer
6,508,765	B2	1/2003	Suorsa et al.	6,685,733	B1	2/2004	Dae et al.
6,508,804	B2	1/2003	Sarge et al.	6,689,086	B1	2/2004	Nita et al.
6,508,815	B1	1/2003	Strul et al.	6,689,148	B2	2/2004	Sawhney et al.
6,511,478	B1	1/2003	Burnside et al.	6,690,181	B1	2/2004	Dowdeswell et al.
6,511,496	B1	1/2003	Huter et al.	6,692,490	B1	2/2004	Edwards
6,511,500	B1	1/2003	Rahme	6,695,830	B2	2/2004	Vigil et al.
6,514,236	B1	2/2003	Stratienko	6,695,857	B2	2/2004	Gifford, III et al.
6,514,245	B1	2/2003	Williams et al.	6,699,241	B2	3/2004	Rappaport et al.
6,514,248	B1	2/2003	Eggers et al.	6,699,257	B2	3/2004	Gifford, III et al.
6,517,534	B1	2/2003	McGovern et al.	6,702,748	B1	3/2004	Nita et al.
6,517,572	B2	2/2003	Kugler et al.	6,702,811	B2	3/2004	Stewart et al.
6,522,913	B2	2/2003	Swanson et al.	6,706,010	B1	3/2004	Miki et al.
6,522,926	B1	2/2003	Kieval et al.	6,706,011	B1	3/2004	Murphy-Chutorian et al.
6,524,299	B1	2/2003	Tran et al.	6,706,037	B2	3/2004	Zvuloni et al.
6,527,765	B2	3/2003	Kelman et al.	6,709,431	B2	3/2004	Lafontaine
6,527,769	B2	3/2003	Langberg et al.	6,711,429	B1	3/2004	Gilboa et al.
6,540,761	B2	4/2003	Houser	6,712,815	B2	3/2004	Sampson et al.
6,542,781	B1	4/2003	Koblish et al.	6,714,822	B2	3/2004	King et al.
6,544,780	B1	4/2003	Wang	6,716,184	B2	4/2004	Vaezy et al.
6,546,272	B1	4/2003	MacKinnon et al.	6,720,350	B2	4/2004	Kunz et al.
6,547,788	B1	4/2003	Maguire et al.	6,723,043	B2	4/2004	Kleeman et al.
6,549,800	B1	4/2003	Atalar et al.	6,723,064	B2	4/2004	Babaev
6,552,796	B2	4/2003	Magnin et al.	6,736,811	B2	5/2004	Panescu et al.
6,554,780	B1	4/2003	Sampson et al.	6,743,184	B2	6/2004	Sampson et al.
6,558,381	B2	5/2003	Ingle et al.	6,746,401	B2	6/2004	Panescu
6,558,382	B2	5/2003	Jahns et al.	6,746,464	B1	6/2004	Makower
6,564,096	B2	5/2003	Mest	6,746,474	B2	6/2004	Saadat
6,565,582	B2	5/2003	Gifford, III et al.	6,748,953	B2	6/2004	Sherry et al.
6,569,109	B2	5/2003	Sakurai et al.	6,749,607	B2	6/2004	Edwards et al.
6,569,177	B1	5/2003	Dillard et al.	6,752,805	B2	6/2004	Maguire et al.
6,570,659	B2	5/2003	Schmitt	6,760,616	B2	7/2004	Hoey et al.
6,572,551	B1	6/2003	Smith et al.	6,763,261	B2	7/2004	Casscells, III et al.
6,572,612	B2	6/2003	Stewart et al.	6,764,501	B2	7/2004	Ganz
6,577,902	B1	6/2003	Laufer et al.	6,769,433	B2	8/2004	Zikorus et al.
6,579,308	B1	6/2003	Jansen et al.	6,770,070	B1	8/2004	Balbierz
6,579,311	B1	6/2003	Makower	6,771,996	B2	8/2004	Bowe et al.
6,582,423	B1	6/2003	Thapliyal et al.	6,773,433	B2	8/2004	Stewart et al.
6,589,238	B2	7/2003	Edwards et al.	6,786,900	B2	9/2004	Joye et al.
6,592,526	B1	7/2003	Lenker	6,786,901	B2	9/2004	Joye et al.
6,592,567	B1	7/2003	Levin et al.	6,786,904	B2	9/2004	Döscher et al.
6,595,959	B1	7/2003	Stratienko	6,788,977	B2	9/2004	Fenn et al.
6,600,956	B2	7/2003	Maschino et al.	6,790,206	B2	9/2004	Panescu
6,602,242	B1	8/2003	Fung et al.	6,790,222	B2	9/2004	Kugler et al.
6,602,246	B1	8/2003	Joye et al.	6,796,981	B2	9/2004	Wham et al.
6,605,084	B2	8/2003	Acker et al.	6,797,933	B1	9/2004	Mendis et al.
6,623,452	B2	9/2003	Chien et al.	6,797,960	B1	9/2004	Spartiotis et al.
6,623,453	B1	9/2003	Guibert et al.	6,800,075	B2	10/2004	Mische et al.
6,632,193	B1	10/2003	Davison et al.	6,802,857	B1	10/2004	Walsh et al.
6,632,196	B1	10/2003	Houser	6,807,444	B2	10/2004	Tu et al.
6,645,223	B2	11/2003	Boyle et al.	6,811,550	B2	11/2004	Holland et al.
6,648,854	B1	11/2003	Patterson et al.	6,813,520	B2	11/2004	Truckai et al.
6,648,878	B2	11/2003	Lafontaine	6,814,730	B2	11/2004	Li
6,648,879	B2	11/2003	Joye et al.	6,814,733	B2	11/2004	Schwartz et al.
6,651,672	B2	11/2003	Roth	6,823,205	B1	11/2004	Jara
6,652,513	B2	11/2003	Panescu et al.	6,824,516	B2	11/2004	Batten et al.
6,652,515	B1	11/2003	Maguire et al.	6,827,726	B2	12/2004	Parodi
6,656,136	B1	12/2003	Weng et al.	6,827,926	B2	12/2004	Robinson et al.
6,658,279	B2	12/2003	Swanson et al.	6,829,497	B2	12/2004	Mogul
6,659,981	B2	12/2003	Stewart et al.	6,830,568	B1	12/2004	Kesten et al.
				6,837,886	B2	1/2005	Collins et al.
				6,837,888	B2	1/2005	Ciarrocca et al.
				6,845,267	B2	1/2005	Harrison
				6,847,848	B2	1/2005	Sterzer

(56)

References Cited

U.S. PATENT DOCUMENTS

6,849,073	B2	2/2005	Hoey et al.	7,083,614	B2	8/2006	Fjield et al.
6,849,075	B2	2/2005	Bertolero et al.	7,084,276	B2	8/2006	Vu et al.
6,853,425	B2	2/2005	Kim et al.	7,087,026	B2	8/2006	Callister et al.
6,855,123	B2	2/2005	Nita	7,087,051	B2	8/2006	Bourne et al.
6,855,143	B2	2/2005	Davison	7,087,052	B2	8/2006	Sampson et al.
6,869,431	B2	3/2005	Maguire et al.	7,087,053	B2	8/2006	Vanney
6,872,183	B2	3/2005	Sampson et al.	7,089,065	B2	8/2006	Westlund et al.
6,884,260	B2	4/2005	Kugler et al.	7,097,641	B1	8/2006	Arless et al.
6,889,694	B2	5/2005	Hooven	7,100,614	B2	9/2006	Stevens et al.
6,893,436	B2	5/2005	Woodard et al.	7,101,368	B2	9/2006	Lafontaine
6,895,077	B2	5/2005	Karellas et al.	7,104,983	B2	9/2006	Grasso, III et al.
6,895,265	B2	5/2005	Silver	7,104,987	B2	9/2006	Biggs et al.
6,898,454	B2	5/2005	Atalar et al.	7,108,715	B2	9/2006	Lawrence-Brown et al.
6,899,711	B2	5/2005	Stewart et al.	7,112,196	B2	9/2006	Brosch et al.
6,899,718	B2	5/2005	Gifford, III et al.	7,112,198	B2	9/2006	Satake
6,905,494	B2	6/2005	Yon et al.	7,112,211	B2	9/2006	Gifford, III et al.
6,908,462	B2	6/2005	Joye et al.	7,122,019	B1	10/2006	Kesten et al.
6,909,009	B2	6/2005	Koridze	7,122,033	B2	10/2006	Wood
6,911,026	B1	6/2005	Hall et al.	7,134,438	B2	11/2006	Makower et al.
6,915,806	B2	7/2005	Pacek et al.	7,137,963	B2	11/2006	Nita et al.
6,923,805	B1	8/2005	LaFontaine et al.	7,137,980	B2	11/2006	Buyssse et al.
6,926,246	B2	8/2005	Ginggen	7,153,315	B2	12/2006	Miller
6,926,713	B2	8/2005	Rioux et al.	7,155,271	B2	12/2006	Halperin et al.
6,926,716	B2	8/2005	Baker et al.	7,157,491	B2	1/2007	Mewshaw et al.
6,929,009	B2	8/2005	Makower et al.	7,157,492	B2	1/2007	Mewshaw et al.
6,929,632	B2	8/2005	Nita et al.	7,158,832	B2	1/2007	Kieval et al.
6,929,639	B2	8/2005	Lafontaine	7,160,296	B2	1/2007	Pearson et al.
6,932,776	B2	8/2005	Carr	7,162,303	B2	1/2007	Levin et al.
6,936,047	B2	8/2005	Nasab et al.	7,165,551	B2	1/2007	Edwards et al.
6,942,620	B2	9/2005	Nita et al.	7,169,144	B2	1/2007	Hoey et al.
6,942,657	B2	9/2005	Sinofsky et al.	7,172,589	B2	2/2007	Lafontaine
6,942,677	B2	9/2005	Nita et al.	7,172,610	B2	2/2007	Heitzmann et al.
6,942,692	B2	9/2005	Landau et al.	7,181,261	B2	2/2007	Silver et al.
6,949,097	B2	9/2005	Stewart et al.	7,184,811	B2	2/2007	Phan et al.
6,949,121	B1	9/2005	Laguna	7,184,827	B1	2/2007	Edwards
6,952,615	B2	10/2005	Satake	7,189,227	B2	3/2007	Lafontaine
6,953,425	B2	10/2005	Brister	7,192,427	B2	3/2007	Chapelon et al.
6,955,174	B2	10/2005	Joye et al.	7,192,586	B2	3/2007	Bander
6,955,175	B2	10/2005	Stevens et al.	7,197,354	B2	3/2007	Sobe
6,959,711	B2	11/2005	Murphy et al.	7,198,632	B2	4/2007	Lim et al.
6,960,207	B2	11/2005	Vanney et al.	7,200,445	B1	4/2007	Dalbec et al.
6,962,584	B1	11/2005	Stone et al.	7,201,749	B2	4/2007	Govari et al.
6,964,660	B2	11/2005	Maguire et al.	7,203,537	B2	4/2007	Mower
6,966,908	B2	11/2005	Maguire et al.	7,214,234	B2	5/2007	Rapacki et al.
6,972,015	B2	12/2005	Joye et al.	7,220,233	B2	5/2007	Nita et al.
6,972,024	B1	12/2005	Kilpatrick et al.	7,220,239	B2	5/2007	Wilson et al.
6,974,456	B2	12/2005	Edwards et al.	7,220,257	B1	5/2007	Lafontaine
6,978,174	B2	12/2005	Gelfand et al.	7,220,270	B2	5/2007	Sawhney et al.
6,979,329	B2	12/2005	Burnside et al.	7,232,458	B2	6/2007	Saadat
6,979,420	B2	12/2005	Weber	7,232,459	B2	6/2007	Greenberg et al.
6,984,238	B2	1/2006	Gifford, III et al.	7,238,184	B2	7/2007	Megerman et al.
6,985,774	B2	1/2006	Kieval et al.	7,241,273	B2	7/2007	Maguire et al.
6,986,739	B2	1/2006	Warren et al.	7,241,736	B2	7/2007	Hunter et al.
6,989,009	B2	1/2006	Lafontaine	7,247,141	B2	7/2007	Makin et al.
6,989,010	B2	1/2006	Francischelli et al.	7,250,041	B2	7/2007	Chiu et al.
6,991,617	B2	1/2006	Hektner et al.	7,250,440	B2	7/2007	Mewshaw et al.
7,001,378	B2	2/2006	Yon et al.	7,252,664	B2	8/2007	Nasab et al.
7,006,858	B2	2/2006	Silver et al.	7,252,679	B2	8/2007	Fischell et al.
7,022,105	B1	4/2006	Edwards	7,264,619	B2	9/2007	Venturelli
7,022,120	B2	4/2006	Lafontaine	7,279,600	B2	10/2007	Mewshaw et al.
7,025,767	B2	4/2006	Schaefer et al.	7,280,863	B2	10/2007	Shachar
7,033,322	B2	4/2006	Silver	7,282,213	B2	10/2007	Schroeder et al.
7,033,372	B1	4/2006	Cahalan	7,285,119	B2	10/2007	Stewart et al.
7,041,098	B2	5/2006	Farley et al.	7,285,120	B2	10/2007	Im et al.
7,050,848	B2	5/2006	Hoey et al.	7,288,089	B2	10/2007	Yon et al.
7,063,670	B2	6/2006	Sampson et al.	7,288,096	B2	10/2007	Chin
7,063,679	B2	6/2006	Maguire et al.	7,291,146	B2	11/2007	Steinke et al.
7,063,719	B2	6/2006	Jansen et al.	7,293,562	B2	11/2007	Malecki et al.
7,066,895	B2	6/2006	Podany	7,294,125	B2	11/2007	Phalen et al.
7,066,900	B2	6/2006	Botto et al.	7,294,126	B2	11/2007	Sampson et al.
7,066,904	B2	6/2006	Rosenthal et al.	7,294,127	B2	11/2007	Leung et al.
7,072,720	B2	7/2006	Puskas	7,297,131	B2	11/2007	Nita
7,074,217	B2	7/2006	Strul et al.	7,297,475	B2	11/2007	Koiwai et al.
7,081,112	B2	7/2006	Joye et al.	7,300,433	B2	11/2007	Lane et al.
7,081,114	B2	7/2006	Rashidi	7,301,108	B2	11/2007	Egitto et al.
				7,310,150	B2	12/2007	Guillermo et al.
				7,313,430	B2	12/2007	Urquhart et al.
				7,314,483	B2	1/2008	Landau et al.
				7,317,077	B2	1/2008	Averback et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,323,006 B2	1/2008	Andreas et al.	7,591,996 B2	9/2009	Hwang et al.
7,326,206 B2	2/2008	Paul et al.	7,597,704 B2	10/2009	Frazier et al.
7,326,226 B2	2/2008	Root et al.	7,598,228 B2	10/2009	Hattori et al.
7,326,235 B2	2/2008	Edwards	7,599,730 B2	10/2009	Hunter et al.
7,326,237 B2	2/2008	DePalma et al.	7,603,166 B2	10/2009	Casscells, III et al.
7,329,236 B2	2/2008	Kesten et al.	7,604,608 B2	10/2009	Nita et al.
7,335,180 B2	2/2008	Nita et al.	7,604,633 B2	10/2009	Truckai et al.
7,335,192 B2	2/2008	Keren et al.	7,615,015 B2	11/2009	Coleman
7,338,467 B2	3/2008	Lutter	7,615,072 B2	11/2009	Rust et al.
7,341,570 B2	3/2008	Keren et al.	7,617,005 B2	11/2009	Demarais et al.
7,343,195 B2	3/2008	Strommer et al.	7,620,451 B2	11/2009	Demarais et al.
7,347,857 B2	3/2008	Anderson et al.	7,621,902 B2	11/2009	Nita et al.
7,348,003 B2	3/2008	Salcedo et al.	7,621,929 B2	11/2009	Nita et al.
7,352,593 B2	4/2008	Zeng et al.	7,626,015 B2	12/2009	Feinstein et al.
7,354,927 B2	4/2008	Vu	7,626,235 B2	12/2009	Kinoshita
7,359,732 B2	4/2008	Kim et al.	7,632,268 B2	12/2009	Edwards et al.
7,361,341 B2	4/2008	Salcedo et al.	7,632,845 B2	12/2009	Vu et al.
7,364,566 B2	4/2008	Elkins et al.	7,635,383 B2	12/2009	Gumm
7,367,970 B2	5/2008	Govari et al.	7,640,046 B2	12/2009	Pastore et al.
7,367,975 B2	5/2008	Malecki et al.	7,641,633 B2	1/2010	Laufer et al.
7,371,231 B2	5/2008	Rioux et al.	7,641,679 B2	1/2010	Joye et al.
7,387,126 B2	6/2008	Cox et al.	7,646,544 B2	1/2010	Batchko et al.
7,393,338 B2	7/2008	Nita	7,647,115 B2	1/2010	Levin et al.
7,396,355 B2	7/2008	Goldman et al.	7,653,438 B2	1/2010	Deem et al.
7,402,151 B2	7/2008	Rosenman et al.	7,655,006 B2	2/2010	Sauvageau et al.
7,402,312 B2	7/2008	Rosen et al.	7,662,114 B2	2/2010	Seip et al.
7,404,824 B1	7/2008	Webler et al.	7,664,548 B2	2/2010	Amurthur et al.
7,406,970 B2	8/2008	Zikorus et al.	7,670,279 B2	3/2010	Gertner
7,407,502 B2	8/2008	Strul et al.	7,670,335 B2	3/2010	Keidar
7,407,506 B2	8/2008	Makower	7,671,084 B2	3/2010	Mewshaw et al.
7,407,671 B2	8/2008	McBride et al.	7,678,104 B2	3/2010	Keidar
7,408,021 B2	8/2008	Averback et al.	7,678,106 B2	3/2010	Lee
7,410,486 B2	8/2008	Fuimaono et al.	7,678,108 B2	3/2010	Chrisitian et al.
7,413,556 B2	8/2008	Zhang et al.	7,691,080 B2	4/2010	Seward et al.
7,425,212 B1	9/2008	Danek et al.	7,699,809 B2	4/2010	Urmey
7,426,409 B2	9/2008	Casscells, III et al.	7,706,882 B2	4/2010	Francischelli et al.
7,435,248 B2	10/2008	Taimisto et al.	7,715,912 B2	5/2010	Rezai et al.
7,447,453 B2	11/2008	Kim et al.	7,717,853 B2	5/2010	Nita
7,449,018 B2	11/2008	Kramer	7,717,909 B2	5/2010	Strul et al.
7,452,538 B2	11/2008	Ni et al.	7,717,948 B2	5/2010	Demarais et al.
7,473,890 B2	1/2009	Grier et al.	7,722,539 B2 *	5/2010	Carter et al. 600/439
7,476,384 B2	1/2009	Ni et al.	7,725,157 B2	5/2010	Dumoulin et al.
7,479,157 B2	1/2009	Weber et al.	7,727,178 B2	6/2010	Wilson et al.
7,481,803 B2	1/2009	Kesten et al.	7,736,317 B2	6/2010	Stephens et al.
7,485,104 B2	2/2009	Kieval	7,736,360 B2	6/2010	Mody et al.
7,486,805 B2	2/2009	Krattiger	7,736,362 B2	6/2010	Eberl et al.
7,487,780 B2	2/2009	Hoooven	7,738,952 B2	6/2010	Yun et al.
7,493,154 B2	2/2009	Bonner et al.	7,740,629 B2	6/2010	Anderson et al.
7,494,485 B2	2/2009	Beck et al.	7,741,299 B2	6/2010	Feinstein et al.
7,494,486 B2	2/2009	Mische et al.	7,742,795 B2	6/2010	Stone et al.
7,494,488 B2	2/2009	Weber	7,744,594 B2	6/2010	Yamazaki et al.
7,494,661 B2	2/2009	Sanders	7,753,907 B2	7/2010	DiMatteo et al.
7,495,439 B2	2/2009	Wiggins	7,756,583 B2	7/2010	Demarais et al.
7,497,858 B2	3/2009	Chapelon et al.	7,758,510 B2	7/2010	Nita et al.
7,499,745 B2	3/2009	Littrup et al.	7,758,520 B2	7/2010	Griffin et al.
7,500,985 B2	3/2009	Saadat	7,759,315 B2	7/2010	Cuzzocrea et al.
7,505,812 B1	3/2009	Eggers et al.	7,766,833 B2	8/2010	Lee et al.
7,505,816 B2	3/2009	Schmeling et al.	7,766,878 B2	8/2010	Tremaglio, Jr. et al.
7,507,233 B2	3/2009	Littrup et al.	7,766,892 B2	8/2010	Keren et al.
7,507,235 B2	3/2009	Keogh et al.	7,767,844 B2	8/2010	Lee et al.
7,511,494 B2	3/2009	Wedeen	7,769,427 B2	8/2010	Shachar
7,512,445 B2	3/2009	Truckai et al.	7,771,372 B2	8/2010	Wilson
7,527,643 B2	5/2009	Case et al.	7,771,421 B2	8/2010	Stewart et al.
7,529,589 B2	5/2009	Williams et al.	7,776,967 B2	8/2010	Perry et al.
7,540,852 B2	6/2009	Nita et al.	7,777,486 B2	8/2010	Hargreaves et al.
7,540,870 B2	6/2009	Babaev	7,780,660 B2	8/2010	Bourne et al.
RE40,863 E	7/2009	Tay et al.	7,789,876 B2	9/2010	Zikorus et al.
7,556,624 B2	7/2009	Laufer et al.	7,792,568 B2	9/2010	Zhong et al.
7,558,625 B2	7/2009	Levin et al.	7,799,021 B2	9/2010	Leung et al.
7,563,247 B2	7/2009	Maguire et al.	7,803,168 B2	9/2010	Gifford et al.
7,566,319 B2	7/2009	McAuley et al.	7,806,871 B2	10/2010	Li et al.
7,569,052 B2	8/2009	Phan et al.	7,811,265 B2	10/2010	Hering et al.
7,582,111 B2	9/2009	Krolik et al.	7,811,281 B1	10/2010	Rentrop
7,584,004 B2	9/2009	Caparso et al.	7,811,313 B2	10/2010	Mon et al.
7,585,835 B2	9/2009	Hill et al.	7,816,511 B2	10/2010	Kawashima et al.
			7,818,053 B2	10/2010	Kassab
			7,819,866 B2	10/2010	Bednarek
			7,822,460 B2	10/2010	Halperin et al.
			7,828,837 B2	11/2010	Khoury

(56)

References Cited

U.S. PATENT DOCUMENTS

7,832,407 B2	11/2010	Gertner	8,152,830 B2	4/2012	Gumm
7,833,220 B2	11/2010	Mon et al.	8,162,933 B2	4/2012	Francischelli et al.
7,837,676 B2	11/2010	Sinelnikov et al.	8,175,711 B2	5/2012	Demarais et al.
7,837,720 B2	11/2010	Mon	8,187,261 B2	5/2012	Watson
7,841,978 B2	11/2010	Gertner	8,190,238 B2	5/2012	Moll et al.
7,846,157 B2	12/2010	Kozel	8,192,053 B2	6/2012	Owen et al.
7,846,160 B2	12/2010	Payne et al.	8,198,611 B2	6/2012	Lafontaine et al.
7,846,172 B2	12/2010	Makower	8,214,056 B2	7/2012	Hoffer et al.
7,849,860 B2	12/2010	Makower et al.	8,221,407 B2	7/2012	Phan et al.
7,850,685 B2	12/2010	Kunis et al.	8,226,637 B2	7/2012	Satake
7,853,333 B2	12/2010	Demarais	8,231,617 B2	7/2012	Satake
7,854,733 B2	12/2010	Govari	8,241,217 B2	8/2012	Chiang et al.
7,854,734 B2	12/2010	Biggs et al.	8,257,724 B2	9/2012	Cromack et al.
7,857,756 B2	12/2010	Warren et al.	8,257,725 B2	9/2012	Cromack et al.
7,862,565 B2	1/2011	Eder et al.	8,260,397 B2	9/2012	Ruff et al.
7,863,897 B2	1/2011	Slocum, Jr. et al.	8,263,104 B2	9/2012	Ho et al.
7,869,854 B2	1/2011	Shachar et al.	8,273,023 B2	9/2012	Razavi
7,873,417 B2	1/2011	Demarais et al.	8,277,379 B2	10/2012	Lau et al.
7,887,538 B2	2/2011	Bleich et al.	8,287,524 B2	10/2012	Siegel
7,894,905 B2	2/2011	Pless et al.	8,287,532 B2	10/2012	Carroll et al.
7,896,873 B2	3/2011	Hiller et al.	8,292,881 B2	10/2012	Brannan et al.
7,901,400 B2	3/2011	Wham et al.	8,293,703 B2	10/2012	Averback et al.
7,901,402 B2	3/2011	Jones et al.	8,295,902 B2	10/2012	Salahieh et al.
7,901,420 B2	3/2011	Dunn	8,295,912 B2	10/2012	Gertner
7,905,862 B2	3/2011	Sampson	8,308,722 B2	11/2012	Ormsby et al.
7,918,850 B2	4/2011	Govari et al.	8,317,776 B2	11/2012	Ferren et al.
7,927,370 B2	4/2011	Webler et al.	8,317,810 B2	11/2012	Stangenes et al.
7,937,143 B2	5/2011	Demarais et al.	8,329,179 B2	12/2012	Ni et al.
7,938,830 B2	5/2011	Saadat et al.	8,336,705 B2	12/2012	Okahisa
7,942,874 B2	5/2011	Eder et al.	8,343,031 B2	1/2013	Gertner
7,942,928 B2	5/2011	Webler et al.	8,343,145 B2	1/2013	Brannan
7,946,976 B2	5/2011	Gertner	8,347,891 B2	1/2013	Demarais et al.
7,950,397 B2	5/2011	Thapliyal et al.	8,353,945 B2	1/2013	Andreas et al.
7,955,293 B2	6/2011	Nita et al.	8,364,237 B2	1/2013	Stone et al.
7,956,613 B2	6/2011	Wald	8,366,615 B2	2/2013	Razavi
7,959,627 B2	6/2011	Utley et al.	8,382,697 B2	2/2013	Brenneman et al.
7,962,854 B2	6/2011	Vance et al.	8,388,680 B2	3/2013	Starksen et al.
7,967,782 B2	6/2011	Laufer et al.	8,396,548 B2	3/2013	Perry et al.
7,967,808 B2	6/2011	Fitzgerald et al.	8,398,629 B2	3/2013	Thistle
7,972,327 B2	7/2011	Eberl et al.	8,401,667 B2	3/2013	Gustus et al.
7,972,330 B2	7/2011	Alejandro et al.	8,403,881 B2	3/2013	Ferren et al.
7,983,751 B2	7/2011	Zdeblick et al.	8,406,877 B2	3/2013	Smith et al.
8,001,976 B2	8/2011	Gertner	8,409,172 B2	4/2013	Moll et al.
8,007,440 B2	8/2011	Magnin et al.	8,409,193 B2	4/2013	Young et al.
8,012,147 B2	9/2011	Lafontaine	8,409,195 B2	4/2013	Young
8,019,435 B2	9/2011	Hastings et al.	8,418,362 B2	4/2013	Zerfas et al.
8,021,362 B2	9/2011	Deem et al.	8,452,988 B2	5/2013	Wang
8,021,413 B2	9/2011	Dierking et al.	8,454,594 B2	6/2013	Demarais et al.
8,025,661 B2	9/2011	Arnold et al.	8,460,358 B2	6/2013	Andreas et al.
8,027,718 B2	9/2011	Spinner et al.	8,465,452 B2	6/2013	Kassab
8,031,927 B2	10/2011	Karl et al.	8,469,919 B2	6/2013	Ingle et al.
8,033,284 B2	10/2011	Porter et al.	8,473,067 B2	6/2013	Hastings et al.
8,048,144 B2	11/2011	Thistle et al.	8,480,663 B2	7/2013	Ingle et al.
8,052,636 B2	11/2011	Moll et al.	8,485,992 B2	7/2013	Griffin et al.
8,052,700 B2	11/2011	Dunn	8,486,060 B2	7/2013	Kotmel et al.
8,062,289 B2	11/2011	Babaev	8,486,063 B2	7/2013	Werneth et al.
8,075,580 B2	12/2011	Makower	8,488,591 B2	7/2013	Miali et al.
8,080,006 B2	12/2011	Lafontaine et al.	2001/0007070 A1	7/2001	Stewart et al.
8,088,127 B2	1/2012	Mayse et al.	2001/0020126 A1	9/2001	Swanson et al.
8,116,883 B2	2/2012	Williams et al.	2001/0039419 A1	11/2001	Francischelli et al.
8,119,183 B2	2/2012	O'Donoghue et al.	2002/0022864 A1	2/2002	Mahvi et al.
8,120,518 B2	2/2012	Jang et al.	2002/0042639 A1	4/2002	Murphy-Chutorian et al.
8,123,741 B2	2/2012	Marrouche et al.	2002/0045811 A1	4/2002	Kittrell et al.
8,128,617 B2	3/2012	Bencini et al.	2002/0045890 A1	4/2002	Celliers et al.
8,131,371 B2	3/2012	Demarais et al.	2002/0049375 A1	4/2002	Strommer et al.
8,131,372 B2	3/2012	Levin et al.	2002/0062146 A1	5/2002	Makower et al.
8,131,382 B2	3/2012	Asada	2002/0065542 A1	5/2002	Lax et al.
8,137,274 B2	3/2012	Weng et al.	2002/0072710 A1	6/2002	Stewart et al.
8,140,170 B2	3/2012	Rezai et al.	2002/0087151 A1	7/2002	Mody et al.
8,143,316 B2	3/2012	Ueno	2002/0095197 A1	7/2002	Lardo et al.
8,145,316 B2	3/2012	Deem et al.	2002/0107536 A1	8/2002	Hussein
8,145,317 B2	3/2012	Demarais et al.	2002/0147480 A1	10/2002	Mamayek
8,150,518 B2	4/2012	Levin et al.	2002/0169444 A1	11/2002	Mest et al.
8,150,519 B2	4/2012	Demarais et al.	2002/0198520 A1	12/2002	Coen et al.
8,150,520 B2	4/2012	Demarais et al.	2003/0028111 A1	2/2003	Vaezy et al.
			2003/0065317 A1	4/2003	Rudie et al.
			2003/0092995 A1	5/2003	Thompson
			2003/0139689 A1	7/2003	Shturman et al.
			2003/0195501 A1	10/2003	Sherman et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2003/0199747 A1	10/2003	Michlitsch et al.	2005/0251116 A1	11/2005	Steinke et al.
2003/0225336 A1	12/2003	Callister et al.	2005/0252553 A1	11/2005	Ginggen
2004/0010118 A1	1/2004	Zerhusen et al.	2005/0256398 A1	11/2005	Hastings et al.
2004/0019348 A1	1/2004	Stevens et al.	2005/0267556 A1	12/2005	Shuros et al.
2004/0024371 A1	2/2004	Plicchi et al.	2006/0004323 A1	1/2006	Chang et al.
2004/0043030 A1	3/2004	Griffiths et al.	2006/0018949 A1	1/2006	Ammon et al.
2004/0064090 A1	4/2004	Keren et al.	2006/0024564 A1	2/2006	Manclaw
2004/0073206 A1	4/2004	Foley et al.	2006/0025765 A1	2/2006	Landman et al.
2004/0088002 A1	5/2004	Boyle et al.	2006/0062786 A1	3/2006	Salcedo et al.
2004/0093055 A1	5/2004	Bartorelli et al.	2006/0083194 A1	4/2006	Dhrimaj et al.
2004/0106871 A1	6/2004	Hunyor et al.	2006/0089637 A1	4/2006	Werneth et al.
2004/0117032 A1	6/2004	Roth	2006/0089638 A1	4/2006	Carmel et al.
2004/0147915 A1	7/2004	Hasebe	2006/0095096 A1	5/2006	DeBenedictis et al.
2004/0162550 A1	8/2004	Govari et al.	2006/0106375 A1	5/2006	Werneth et al.
2004/0162555 A1	8/2004	Farley et al.	2006/0142790 A1	6/2006	Gertner
2004/0167506 A1	8/2004	Chen	2006/0142801 A1	6/2006	Demarais et al.
2004/0176757 A1	9/2004	Siheinikov et al.	2006/0147492 A1	7/2006	Hunter et al.
2004/0186356 A1	9/2004	O'Malley et al.	2006/0167106 A1	7/2006	Zhang et al.
2004/0187875 A1	9/2004	He et al.	2006/0167498 A1	7/2006	DiLorenzo
2004/0193211 A1	9/2004	Voegele et al.	2006/0171895 A1	8/2006	Bucay-Couto
2004/0220556 A1	11/2004	Cooper et al.	2006/0184221 A1	8/2006	Stewart et al.
2004/0243022 A1	12/2004	Carney et al.	2006/0195139 A1	8/2006	Gertner
2004/0243124 A1	12/2004	Im et al.	2006/0206150 A1	9/2006	Demarais et al.
2004/0253304 A1	12/2004	Gross et al.	2006/0212076 A1	9/2006	Demarais et al.
2004/0267132 A1 *	12/2004	Podany 600/459	2006/0212078 A1	9/2006	Demarais et al.
2004/0267250 A1	12/2004	Yon et al.	2006/0224153 A1	10/2006	Fischell et al.
2005/0010095 A1	1/2005	Stewart et al.	2006/0229659 A1	10/2006	Gifford et al.
2005/0015125 A1	1/2005	Mioduski et al.	2006/0235474 A1	10/2006	Demarais et al.
2005/0080374 A1	4/2005	Esch et al.	2006/0239921 A1	10/2006	Mangat et al.
2005/0129616 A1	6/2005	Salcedo et al.	2006/0240070 A1	10/2006	Cromack et al.
2005/0137180 A1	6/2005	Robinson et al.	2006/0241648 A1	10/2006	Bleich et al.
2005/0143817 A1	6/2005	Hunter et al.	2006/0247266 A1	11/2006	Yamada et al.
2005/0148842 A1	7/2005	Wang et al.	2006/0247760 A1	11/2006	Ganesan et al.
2005/0149069 A1	7/2005	Bertolero et al.	2006/0263393 A1	11/2006	Demopulos et al.
2005/0149080 A1	7/2005	Hunter et al.	2006/0265014 A1	11/2006	Demarais et al.
2005/0149158 A1	7/2005	Hunter et al.	2006/0265015 A1	11/2006	Demarais et al.
2005/0149173 A1	7/2005	Hunter et al.	2006/0269555 A1	11/2006	Salcedo et al.
2005/0149175 A1	7/2005	Hunter et al.	2006/0271111 A1	11/2006	Demarais et al.
2005/0154277 A1	7/2005	Tang et al.	2006/0276852 A1	12/2006	Demarais et al.
2005/0154445 A1	7/2005	Hunter et al.	2006/0287644 A1	12/2006	Inganas et al.
2005/0154453 A1	7/2005	Hunter et al.	2007/0016184 A1	1/2007	Cropper et al.
2005/0154454 A1	7/2005	Hunter et al.	2007/0016274 A1	1/2007	Boveja et al.
2005/0165389 A1	7/2005	Swain et al.	2007/0027390 A1	2/2007	Maschke et al.
2005/0165391 A1	7/2005	Maguire et al.	2007/0043077 A1	2/2007	Mewshaw et al.
2005/0165467 A1	7/2005	Hunter et al.	2007/0043409 A1	2/2007	Brian et al.
2005/0165488 A1	7/2005	Hunter et al.	2007/0049924 A1	3/2007	Rahn
2005/0175661 A1	8/2005	Hunter et al.	2007/0066957 A1	3/2007	Demarais et al.
2005/0175662 A1	8/2005	Hunter et al.	2007/0066972 A1	3/2007	Ormsby et al.
2005/0175663 A1	8/2005	Hunter et al.	2007/0073151 A1 *	3/2007	Lee 600/439
2005/0177103 A1	8/2005	Hunter et al.	2007/0093710 A1	4/2007	Maschke
2005/0177225 A1	8/2005	Hunter et al.	2007/0100405 A1	5/2007	Thompson et al.
2005/0181004 A1	8/2005	Hunter et al.	2007/0106247 A1	5/2007	Burnett et al.
2005/0181008 A1	8/2005	Hunter et al.	2007/0112327 A1	5/2007	Yun et al.
2005/0181011 A1	8/2005	Hunter et al.	2007/0118107 A1	5/2007	Francischelli et al.
2005/0181977 A1	8/2005	Hunter et al.	2007/0123851 A1	5/2007	Alejandro et al.
2005/0182479 A1	8/2005	Bonsignore et al.	2007/0129633 A1	6/2007	Lee et al.
2005/0183728 A1	8/2005	Hunter et al.	2007/0129720 A1	6/2007	Demarais et al.
2005/0186242 A1	8/2005	Hunter et al.	2007/0129760 A1	6/2007	Demarais et al.
2005/0186243 A1	8/2005	Hunter et al.	2007/0129761 A1	6/2007	Demarais et al.
2005/0186244 A1	8/2005	Hunter et al.	2007/0135875 A1	6/2007	Demarais et al.
2005/0191331 A1	9/2005	Hunter et al.	2007/0149963 A1	6/2007	Matsukuma et al.
2005/0203410 A1	9/2005	Jenkins	2007/0162109 A1	7/2007	Davila et al.
2005/0209587 A1	9/2005	Joye et al.	2007/0167821 A1 *	7/2007	Lee et al. 600/463
2005/0214205 A1	9/2005	Salcedo et al.	2007/0173805 A1	7/2007	Weinberg et al.
2005/0214207 A1	9/2005	Salcedo et al.	2007/0173899 A1	7/2007	Levin et al.
2005/0214208 A1	9/2005	Salcedo et al.	2007/0179496 A1	8/2007	Swoyer et al.
2005/0214209 A1	9/2005	Salcedo et al.	2007/0198007 A1	8/2007	Govari et al.
2005/0214210 A1	9/2005	Salcedo et al.	2007/0203480 A1	8/2007	Mody et al.
2005/0214268 A1	9/2005	Cavanagh et al.	2007/0203549 A1	8/2007	Demarais et al.
2005/0228286 A1	10/2005	Messerly et al.	2007/0207186 A1	9/2007	Scanlon et al.
2005/0228415 A1	10/2005	Gertner	2007/0208134 A1	9/2007	Hunter et al.
2005/0228460 A1	10/2005	Levin et al.	2007/0208210 A1	9/2007	Gelfand et al.
2005/0232921 A1	10/2005	Rosen et al.	2007/0208256 A1	9/2007	Marilla
2005/0234312 A1	10/2005	Suzuki et al.	2007/0208301 A1	9/2007	Evard et al.
2005/0240116 A1 *	10/2005	Saadat et al. 600/549	2007/0213735 A1	9/2007	Saadat et al.
2005/0245862 A1	11/2005	Seward	2007/0219576 A1	9/2007	Cangialosi
			2007/0225781 A1	9/2007	Saadat et al.
			2007/0232913 A1	10/2007	Lau
			2007/0233170 A1	10/2007	Gertner

(56)

References Cited

U.S. PATENT DOCUMENTS

2007/0239062 A1	10/2007	Chopra et al.	2009/0043372 A1	2/2009	Northrop et al.
2007/0248639 A1	10/2007	Demopoulos et al.	2009/0054082 A1	2/2009	Kim et al.
2007/0249703 A1	10/2007	Mewshaw et al.	2009/0062873 A1	3/2009	Wu et al.
2007/0254833 A1	11/2007	Hunter et al.	2009/0069671 A1	3/2009	Anderson
2007/0265687 A1	11/2007	Deem et al.	2009/0076409 A1	3/2009	Wu et al.
2007/0278103 A1	12/2007	Hoerr et al.	2009/0088735 A1	4/2009	Abboud et al.
2007/0282302 A1	12/2007	Wachsman et al.	2009/0105631 A1	4/2009	Kieval
2007/0292411 A1	12/2007	Salcedo et al.	2009/0112091 A1	4/2009	Chiang
2007/0293782 A1	12/2007	Marino	2009/0112202 A1	4/2009	Young
2007/0299043 A1	12/2007	Hunter et al.	2009/0118620 A1	5/2009	Tgavalekos et al.
2008/0004673 A1	1/2008	Rossing et al.	2009/0118726 A1	5/2009	Auth et al.
2008/0009927 A1	1/2008	Vilims	2009/0125099 A1	5/2009	Weber et al.
2008/0015501 A1	1/2008	Gertner	2009/0131798 A1	5/2009	Minar et al.
2008/0021408 A1	1/2008	Jacobsen et al.	2009/0143640 A1	6/2009	Saadat et al.
2008/0033049 A1	2/2008	Mewshaw	2009/0156988 A1	6/2009	Ferren et al.
2008/0039746 A1 *	2/2008	Hissong et al. 601/3	2009/0157057 A1	6/2009	Ferren et al.
2008/0039830 A1	2/2008	Munger et al.	2009/0157161 A1	6/2009	Desai et al.
2008/0051454 A1	2/2008	Wang	2009/0171333 A1	7/2009	Hon
2008/0058791 A1	3/2008	Eberl	2009/0192558 A1	7/2009	Whitehurst et al.
2008/0064957 A1	3/2008	Spence	2009/0198223 A1	8/2009	Thilwind et al.
2008/0071269 A1	3/2008	Hilario et al.	2009/0203962 A1	8/2009	Miller et al.
2008/0071306 A1	3/2008	Gertner	2009/0203993 A1	8/2009	Mangat et al.
2008/0082109 A1	4/2008	Moll et al.	2009/0204134 A1	8/2009	Kassab
2008/0086072 A1	4/2008	Bonutti et al.	2009/0204170 A1	8/2009	Hastings et al.
2008/0086185 A1	4/2008	Amurthur et al.	2009/0209885 A1	8/2009	Babaev
2008/0091193 A1	4/2008	Kauphusman et al.	2009/0209949 A1	8/2009	Ingle
2008/0097251 A1	4/2008	Babaev	2009/0209951 A1	8/2009	Marrouche
2008/0097426 A1	4/2008	Root et al.	2009/0210953 A1	8/2009	Moyer et al.
2008/0108867 A1	5/2008	Zhou	2009/0216317 A1	8/2009	Cromack et al.
2008/0119879 A1	5/2008	Brenneman et al.	2009/0221939 A1	9/2009	Demarais et al.
2008/0125772 A1	5/2008	Stone et al.	2009/0221955 A1	9/2009	Babaev
2008/0132450 A1	6/2008	Lee et al.	2009/0226429 A1	9/2009	Salcedo et al.
2008/0140002 A1	6/2008	Ramzipoor et al.	2009/0240249 A1	9/2009	Chan et al.
2008/0146918 A1	6/2008	Magnin et al.	2009/0247933 A1	10/2009	Maor et al.
2008/0147002 A1	6/2008	Gertner	2009/0247966 A1	10/2009	Gunn et al.
2008/0161662 A1	7/2008	Golijanin et al.	2009/0248012 A1	10/2009	Maor et al.
2008/0161717 A1	7/2008	Gertner	2009/0253974 A1	10/2009	Rahme
2008/0161801 A1	7/2008	Steinke et al.	2009/0264755 A1	10/2009	Chen et al.
2008/0171944 A1	7/2008	Brenneman et al.	2009/0270850 A1	10/2009	Zhou et al.
2008/0171974 A1	7/2008	Lafontaine et al.	2009/0281533 A1	11/2009	Ingle et al.
2008/0172035 A1	7/2008	Starksen et al.	2009/0287137 A1	11/2009	Crowley
2008/0172104 A1	7/2008	Kieval et al.	2009/0287202 A1	11/2009	Ingle
2008/0188912 A1	8/2008	Stone et al.	2009/0299355 A1	12/2009	Bencini
2008/0188913 A1	8/2008	Stone et al.	2009/0299356 A1	12/2009	Watson
2008/0208162 A1	8/2008	Joshi	2009/0306644 A1	12/2009	Mayse et al.
2008/0208169 A1	8/2008	Boyle et al.	2009/0318749 A1	12/2009	Stolen et al.
2008/0208182 A1	8/2008	Lafontaine	2010/0009267 A1	1/2010	Chase et al.
2008/0213331 A1	9/2008	Gelfand et al.	2010/0030061 A1	2/2010	Canfield et al.
2008/0215117 A1	9/2008	Gross	2010/0048983 A1	2/2010	Ball et al.
2008/0221448 A1	9/2008	Khuri-Yakub et al.	2010/0049099 A1	2/2010	Thapliyal et al.
2008/0234780 A1	9/2008	Smith	2010/0049186 A1	2/2010	Ingle et al.
2008/0234790 A1	9/2008	Bayer et al.	2010/0049188 A1	2/2010	Nelson et al.
2008/0243091 A1	10/2008	Humphreys et al.	2010/0049191 A1	2/2010	Habib et al.
2008/0245371 A1	10/2008	Gruber	2010/0049283 A1	2/2010	Johnson
2008/0249525 A1	10/2008	Lee et al.	2010/0057150 A1	3/2010	Demarais et al.
2008/0249547 A1	10/2008	Dunn	2010/0069837 A1	3/2010	Rassat et al.
2008/0255550 A1	10/2008	Bell	2010/0076299 A1	3/2010	Gustus et al.
2008/0255642 A1	10/2008	Zarins et al.	2010/0076425 A1	3/2010	Carroux
2008/0262489 A1	10/2008	Steinke	2010/0087782 A1	4/2010	Ghaffari et al.
2008/0275484 A1	11/2008	Gertner	2010/0106005 A1	4/2010	Karczmar et al.
2008/0281312 A1	11/2008	Werneth et al.	2010/0114244 A1	5/2010	Manda et al.
2008/0281347 A1	11/2008	Gertner	2010/0130815 A1 *	5/2010	Gross et al. 600/30
2008/0287918 A1	11/2008	Rosenman et al.	2010/0130836 A1	5/2010	Malchano et al.
2008/0294037 A1	11/2008	Richter	2010/0137860 A1	6/2010	Demarais et al.
2008/0300618 A1	12/2008	Gertner	2010/0137952 A1	6/2010	Demarais et al.
2008/0312644 A1	12/2008	Fourkas et al.	2010/0160903 A1	6/2010	Krespi
2008/0312673 A1	12/2008	Viswanathan et al.	2010/0160906 A1	6/2010	Jarrard
2008/0317818 A1	12/2008	Griffith et al.	2010/0168624 A1	7/2010	Sliwa
2009/0018486 A1	1/2009	Goren et al.	2010/0168731 A1	7/2010	Wu et al.
2009/0018609 A1	1/2009	DiLorenzo	2010/0168739 A1	7/2010	Wu et al.
2009/0024194 A1	1/2009	Arcot-Krishnamurthy et al.	2010/0168777 A1	7/2010	Stangenes et al.
2009/0024195 A1	1/2009	Rezaei et al.	2010/0174282 A1	7/2010	Demarais et al.
2009/0030312 A1	1/2009	Hadjicostis	2010/0191112 A1	7/2010	Demarais et al.
2009/0030411 A1	1/2009	Werneth et al.	2010/0191232 A1	7/2010	Boveda
2009/0036948 A1	2/2009	Levin et al.	2010/0217162 A1	8/2010	Hissong et al.
			2010/0222786 A1	9/2010	Kassab
			2010/0222851 A1	9/2010	Deem et al.
			2010/0222854 A1	9/2010	Demarais et al.
			2010/0228122 A1	9/2010	Keenan et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2010/0249604 A1 9/2010 Hastings et al.
 2010/0249773 A1 9/2010 Clark et al.
 2010/0256616 A1 10/2010 Katoh et al.
 2010/0268217 A1 10/2010 Habib
 2010/0268307 A1 10/2010 Demarais et al.
 2010/0284927 A1 11/2010 Lu et al.
 2010/0286684 A1 11/2010 Hata et al.
 2010/0298821 A1 11/2010 Garbagnati
 2010/0305036 A1 12/2010 Barnes et al.
 2010/0312141 A1 12/2010 Keast et al.
 2010/0324472 A1 12/2010 Wulfinan
 2011/0009750 A1 1/2011 Taylor et al.
 2011/0021976 A1 1/2011 Li et al.
 2011/0034832 A1 2/2011 Cioanta et al.
 2011/0040324 A1 2/2011 McCarthy et al.
 2011/0044942 A1 2/2011 Puri et al.
 2011/0060324 A1 3/2011 Wu et al.
 2011/0071400 A1 3/2011 Hastings et al.
 2011/0071401 A1 3/2011 Hastings et al.
 2011/0077498 A1 3/2011 McDaniel
 2011/0092781 A1 4/2011 Gertner
 2011/0092880 A1 4/2011 Gertner
 2011/0104061 A1 5/2011 Seward
 2011/0112400 A1 5/2011 Emery et al.
 2011/0118598 A1* 5/2011 Gertner 600/431
 2011/0118600 A1 5/2011 Gertner
 2011/0118726 A1 5/2011 De La Rama et al.
 2011/0130708 A1 6/2011 Perry et al.
 2011/0137155 A1 6/2011 Weber et al.
 2011/0144479 A1 6/2011 Hastings et al.
 2011/0146673 A1 6/2011 Keast et al.
 2011/0166499 A1 7/2011 Demarais et al.
 2011/0178570 A1 7/2011 Demarais
 2011/0200171 A1 8/2011 Beetel et al.
 2011/0202098 A1 8/2011 Demarais et al.
 2011/0207758 A1 8/2011 Sobotka et al.
 2011/0208096 A1 8/2011 Demarais et al.
 2011/0257523 A1 10/2011 Hastings et al.
 2011/0257564 A1 10/2011 Demarais et al.
 2011/0257622 A1 10/2011 Salahieh et al.
 2011/0257641 A1 10/2011 Hastings et al.
 2011/0257642 A1 10/2011 Griggs, III
 2011/0263921 A1 10/2011 Vrba et al.
 2011/0264011 A1 10/2011 Wu et al.
 2011/0264075 A1 10/2011 Leung et al.
 2011/0264086 A1 10/2011 Ingle
 2011/0264116 A1 10/2011 Kocur et al.
 2011/0270238 A1 11/2011 Rizq et al.
 2011/0306851 A1 12/2011 Wang
 2011/0307034 A1 12/2011 Hastings
 2011/0319809 A1 12/2011 Smith
 2012/0029496 A1 2/2012 Smith
 2012/0029500 A1 2/2012 Jensen
 2012/0029505 A1 2/2012 Jensen
 2012/0029509 A1 2/2012 Smith
 2012/0029510 A1 2/2012 Haverkost
 2012/0029511 A1 2/2012 Smith et al.
 2012/0029512 A1 2/2012 Willard et al.
 2012/0029513 A1 2/2012 Smith et al.
 2012/0059241 A1 3/2012 Hastings et al.
 2012/0059286 A1 3/2012 Hastings et al.
 2012/0065506 A1 3/2012 Smith
 2012/0065554 A1 3/2012 Pikus
 2012/0095461 A1 4/2012 Herscher et al.
 2012/0101413 A1 4/2012 Beetel et al.
 2012/0101490 A1 4/2012 Smith
 2012/0101538 A1 4/2012 Ballakur et al.
 2012/0109021 A1 5/2012 Hastings et al.
 2012/0116382 A1 5/2012 Ku et al.
 2012/0116383 A1 5/2012 Mauch et al.
 2012/0116392 A1 5/2012 Willard
 2012/0116438 A1 5/2012 Salahieh et al.
 2012/0116486 A1 5/2012 Naga et al.
 2012/0123243 A1 5/2012 Hastings
 2012/0123258 A1 5/2012 Willard

2012/0123261 A1 5/2012 Jensen et al.
 2012/0123303 A1 5/2012 Sogard et al.
 2012/0123406 A1 5/2012 Edmunds et al.
 2012/0130289 A1 5/2012 Demarais et al.
 2012/0130345 A1 5/2012 Levin et al.
 2012/0130359 A1 5/2012 Turovskiy
 2012/0130360 A1 5/2012 Buckley et al.
 2012/0130362 A1 5/2012 Hastings et al.
 2012/0130368 A1 5/2012 Jensen
 2012/0130458 A1 5/2012 Ryba et al.
 2012/0136344 A1 5/2012 Buckley et al.
 2012/0136349 A1 5/2012 Hastings
 2012/0136350 A1 5/2012 Goshgarian et al.
 2012/0136417 A1 5/2012 Buckley et al.
 2012/0136418 A1 5/2012 Buckley et al.
 2012/0143181 A1 6/2012 Demarais et al.
 2012/0143293 A1 6/2012 Mauch et al.
 2012/0143294 A1 6/2012 Clark et al.
 2012/0150267 A1 6/2012 Buckley et al.
 2012/0157986 A1 6/2012 Stone et al.
 2012/0157987 A1 6/2012 Steinke et al.
 2012/0157988 A1 6/2012 Stone et al.
 2012/0157989 A1 6/2012 Stone et al.
 2012/0157992 A1 6/2012 Smith et al.
 2012/0157993 A1 6/2012 Jensen et al.
 2012/0158101 A1 6/2012 Stone et al.
 2012/0158104 A1 6/2012 Huynh et al.
 2012/0172837 A1 7/2012 Demarais et al.
 2012/0172870 A1 7/2012 Jensen et al.
 2012/0184952 A1 7/2012 Jensen et al.
 2012/0197198 A1 8/2012 Demarais et al.
 2012/0197252 A1 8/2012 Deem et al.
 2012/0232409 A1 9/2012 Stahmann et al.
 2012/0265066 A1 10/2012 Crow et al.
 2012/0265198 A1 10/2012 Crow et al.
 2013/0012844 A1 1/2013 Demarais et al.
 2013/0012866 A1 1/2013 Deem et al.
 2013/0012867 A1 1/2013 Demarais et al.
 2013/0013024 A1 1/2013 Levin et al.
 2013/0023865 A1 1/2013 Steinke et al.
 2013/0035681 A1 2/2013 Subramaniam et al.
 2013/0066316 A1 3/2013 Steinke et al.
 2013/0085489 A1 4/2013 Fain et al.
 2013/0090563 A1 4/2013 Weber
 2013/0090578 A1 4/2013 Smith et al.
 2013/0090647 A1 4/2013 Smith
 2013/0090649 A1 4/2013 Smith et al.
 2013/0090650 A1 4/2013 Jensen et al.
 2013/0090651 A1 4/2013 Smith
 2013/0090652 A1 4/2013 Jensen
 2013/0096550 A1 4/2013 Hill
 2013/0096553 A1 4/2013 Hill et al.
 2013/0096554 A1 4/2013 Groff et al.
 2013/0096604 A1 4/2013 Hanson et al.
 2013/0110106 A1 5/2013 Richardson
 2013/0116687 A1 5/2013 Willard
 2013/0165764 A1 6/2013 Scheuermann et al.
 2013/0165844 A1 6/2013 Shuros et al.
 2013/0165916 A1 6/2013 Mathur et al.
 2013/0165917 A1 6/2013 Mathur et al.
 2013/0165920 A1 6/2013 Weber et al.
 2013/0165923 A1 6/2013 Mathur et al.
 2013/0165924 A1 6/2013 Mathur et al.
 2013/0165925 A1 6/2013 Mathur et al.
 2013/0165926 A1 6/2013 Mathur et al.
 2013/0165990 A1 6/2013 Mathur et al.
 2013/0172815 A1 7/2013 Perry et al.
 2013/0172872 A1 7/2013 Subramaniam et al.
 2013/0172877 A1 7/2013 Subramaniam et al.
 2013/0172878 A1 7/2013 Smith
 2013/0172879 A1 7/2013 Sutermeister
 2013/0172880 A1 7/2013 Willard
 2013/0172881 A1 7/2013 Hill et al.

FOREIGN PATENT DOCUMENTS

EP 1180004 A1 2/2002
 EP 1335677 B1 8/2003
 EP 1579889 9/2005

(56)

References Cited

FOREIGN PATENT DOCUMENTS

EP	1874211	A2	1/2008
EP	1906853	A2	4/2008
EP	1961394	A2	8/2008
EP	1620156	B1	7/2009
EP	2076193	A2	7/2009
EP	2091455	A2	8/2009
EP	2197533	A1	6/2010
EP	2204134		7/2010
EP	2208506	A1	7/2010
EP	1579889	B1	8/2010
EP	2092957	B1	1/2011
EP	2349044	A1	8/2011
EP	2027882	B1	10/2011
EP	2378956	A2	10/2011
EP	2037840	B1	12/2011
EP	2204134	B1	4/2012
EP	2320821	B1	10/2012
GB	2456301	A	7/2009
WO	9858588	A1	12/1998
WO	9900060	A1	1/1999
WO	0047118	A1	8/2000
WO	WO0047118		8/2000
WO	03026525	A1	4/2003
WO	2004100813	A2	11/2004
WO	2004110258	A2	12/2004
WO	WO2004110258		12/2004
WO	WO2006022790		3/2006
WO	WO2006041847		4/2006
WO	WO2006041881		4/2006
WO	2006105121	A2	10/2006
WO	WO2007035537		3/2007
WO	WO2007078997		7/2007
WO	WO2007086965		8/2007
WO	WO2007103879		9/2007
WO	WO2007103881		9/2007
WO	WO2007121309		10/2007
WO	WO2007146834		12/2007
WO	2008014465	A2	1/2008
WO	WO2008003058		1/2008
WO	WO2008061150		5/2008
WO	WO2008061152		5/2008
WO	WO2008070413		6/2008
WO	2009121017	A1	10/2009
WO	2010067360	A2	6/2010
WO	WO2010067360		6/2010
WO	WO2010078175		7/2010
WO	2010102310	A2	9/2010
WO	WO2010129661		11/2010
WO	2011005901	A2	1/2011
WO	2011053757	A1	5/2011
WO	2011053772	A1	5/2011
WO	WO2011053757		5/2011
WO	WO2011053772		5/2011
WO	2011091069	A1	7/2011
WO	WO2011091069		7/2011
WO	2011130534	A2	10/2011
WO	WO2011130005		10/2011
WO	WO2011139589		11/2011
WO	2012019156	A1	2/2012
WO	WO2012019156		2/2012
WO	2013049601	A2	4/2013

OTHER PUBLICATIONS

Lafon et al., "Optimizing the Shape of Ultrasound Transducers for Interstitial Thermal Ablation", Medical Physics, vol. 29, Issue 3, 2002, 8 pages.

Invitation to Pay Additional Search Fees dated Feb. 17, 2011 from PCT Application No. PCT/US2010/062458, 8 pages.

International Search Report and Written Opinion dated May 10, 2011 from PCT Application No. PCT/US2010/062457, 10 pages.

U.S. Appl. No. 12/980,952, filed Dec. 29, 2010, Rizq et al.

U.S. Appl. No. 12/980,972, filed Dec. 29, 2010, Vrba et al.

U.S. Appl. No. 61/324,163, filed Apr. 14, 2010, Hastings et al.

Toytman et al., "Tissue Dissection with Ultrafast Laser Using Extended and Multiple Foci", SPIE Proceedings, Optical Interactions with Tissues and Cells XXI, vol. 7562, 2010, 10 pages.

Blue Cross Blue Shield Medical Policy, "Surgery Section—MRI-Guided Focused Ultrasound (MRgFUS) for the Treatment of Uterine Fibroids and Other Tumors", 2004, 5 pages.

Seip et al., "Transurethral High Intensity Focused Ultrasound: Catheter Based Prototypes and Experimental Results", IEEE Ultrasonics Symposium Proceedings, 2000, 4 pages.

U.S. Appl. No. 13/225,962, filed Sep. 6, 2011, Hastings.

U.S. Appl. No. 13/227,446, filed Sep. 7, 2011, Hastings et al.

U.S. Appl. No. 13/243,114, filed Sep. 23, 2011, Jenson et al.

U.S. Appl. No. 13/243,134, filed Sep. 23, 2011, Sogard et al.

U.S. Appl. No. 13/283,203, filed Oct. 27, 2011, Hastings.

U.S. Appl. No. 13/295,182, filed Nov. 14, 2011, Hastings.

Lafon et al., "Optimizing the Shape of Ultrasound Transducers for Interstitial Thermal Ablation", Med Phys. Mar. 2002; 29(3): 290-7 (abstract only).

G. Ter Haar, "Ultrasound Focal Beam Surgery", Ultrasound in Med. & Biol., 1995, vol. 21, No. 9, pp. 1089-1100.

Zhou et al., "Non-Thermal Ablation of Rabbit Liver VX2 Tumor by Pulsed High Intensity Focused Ultrasound Contrast Agent: Pathological Characteristics", World Journal of Gastroenterology, vol. 14(43), Nov. 21, 2008, pp. 6743-6747.

Invitation to Pay Additional Fees dated Aug. 4, 2011 for PCT Application No. PCT/US2011/032524, 6 pages.

International Search Report and Written Opinion dated Oct. 26, 2011 for PCT Application No. PCT/US2011/032524, 16 pages.

Invitation to Pay Additional Fees dated Jan. 30, 2012 for PCT Application No. PCT/US2011/061157, 7 pages.

International Search Report and Written Opinion dated Dec. 23, 2011 for PCT Application No. PCT/US2011/050731, 14 pages.

Baun, "Interaction with Soft Tissue", Principles of General & Vascular Sonography, Chapter 2, pp. 23-34, Mar. 5, 2009.

Van Den Berg, "Light echoes image the human body," OLE, Oct. 2001, p. 35-37.

"IntraLuminal: Products," IntraLuminal Therapeutics, Inc., 2003, p. 1-9.

"Laser Catheter to Aid Coronary Surgery," TechTalk: MIT, Jan. 9, 1991, p. 1-4.

"Optical Coherence Tomography: Advantages of OCT," LightLab Imaging Technology.

"Optical Coherence Tomography: Image Gallery Cardiovascular Procedures," LightLab Imaging Technology.

"Optical Coherence Tomography: LightLab Imaging Starts US Cardiology Clinical Investigations," LightLab Imaging Technology, 2002.

"Optical Coherence Tomography: LightLab Sees Bright Prospects for Cardiac Application of OCT Technology," LightLab Imaging Technology, 2001, vol. 27, No. 35.

"Optical Coherence Tomography: What is OCT?," LightLab Imaging Technology.

"Optical Coherence Tomography: Why Use OCT?," LightLab Imaging Technology.

"Products—Functional Measurement," VOLCANO Functional Measurement Products US, Mar. 24, 2003, p. 1-2.

Brown et al., "Radiofrequency capacitive heaters: the effect of coupling medium resistivity on power absorption along a mouse leg," Physics in Medicine and Biology, 1993, p. 1-12, vol. 38.

Carrington, "Future of CVI: It's all about plaque: Identification of vulnerable lesions, not 'rusty pipes,' could become cornerstone of preventive cardiology," Diagnostic Imaging, 2001, p. 1-8.

Chen et al., "Percutaneous pulmonary artery denervation completely abolishes experimental pulmonary arterial hypertension in vivo," EuroIntervention, 2013, p. 1-8.

Cimino, "Preventing plaque attack," Mass High Tech, 2001, p. 1-2.

Dahm et al., "Relation of Degree of Laser Debulking of In-Stent Restenosis as a Predictor of Restenosis Rate," The American Journal of Cardiology, 2002, p. 68-70, vol. 90.

De Korte et al., "Characterization of Plaque Components With Intravascular Ultrasound Elastography in Human Femoral and Coronary Arteries In Vitro," Circulation, Aug. 8, 2000, p. 617-623.

(56)

References Cited

OTHER PUBLICATIONS

- Durney et al., "Radiofrequency Radiation Dosimetry Handbook," Oct. 1986, p. 1-2, Fourth Edition.
- Durney et al., "Radiofrequency Radiation Dosimetry Handbook: Contents," Oct. 1986, p. 1-5, Fourth Edition.
- Fournier-Desseux et al., "Assessment of 1-lead and 2-lead electrode patterns in electrical impedance endotomography," *Physiological Measurement*, 2005, p. 337-349. Vol. 26, Institute of Physics Publishing.
- Fram et al., "Feasibility of Radiofrequency Powered, Thermal Balloon Ablation of Atrioventricular Bypass Tracts Via the Coronary Sinus: In Vivo Canine Studies," *PACE*, Aug. 1995, p. 1518-1530, vol. 18.
- Fram et al., "Low Pressure Radiofrequency Balloon Angioplasty: Evaluation in Porcine Peripheral Arteries," *JACC*, 1993, p. 1512-1521, vol. 21, No. 6, American College of Cardiology.
- Fujimori et al., "Significant Prevention of In-Stent Restenosis by Evans Blue in Patients with Acute Myocardial Infarction," *American Heart Association*, 2002.
- Fujita et al., "Sarpogrelate, An Antagonist of 5-HT(2A) Receptor, Treatment Reduces Restenosis After Coronary Stenting," *American Heart Association*, 2002.
- Gabriel, "Appendix A: Experimental Data," 1999, p. 1-21.
- Gabriel, "Appendix C: Modeling the frequency dependence of the dielectric properties to a 4 dispersions spectrum," p. 1-6.
- Gregory et al., "Liquid Core Light Guide for Laser Angioplasty," *The Journal of Quantum Electronics*, Dec. 1990, p. 2289-2296, vol. 26, No. 12.
- Kaplan et al., "Healing after Arterial Dilatation with Radiofrequency Thermal and Nonthermal Balloon Angioplasty Systems," *Journal of Investigative Surgery*, 1993, p. 33-52, vol. 6.
- Kolata, "New Studies Question Value of Opening Arteries," *The New York Times*, Mar. 21, 2004, p. 1-5.
- Konings et al., "Development of an Intravascular Impedance Catheter for Detection of Fatty Lesions in Arteries," *IEEE Transactions on Medical Imaging*, Aug. 1997, p. 439-446, vol. 16, No. 4.
- Kurtz et al., "Lamellar Refractive Surgery with Scanned Intrastromal Picosecond and Femtosecond Laser Pulses in Animal Eyes," *Journal of Refractive Surgery*, Sep./Oct. 1998, p. 541-548.
- Lee et al., "Thermal Compression and Molding of Atherosclerotic Vascular Tissue With Use of Radiofrequency Energy: Implications for Radiofrequency Balloon Angioplasty," *JACC*, 1989, p. 1167-1175, vol. 13, No. 5, American College of Cardiology.
- Lima et al., "Efficacy and Safety of Oral Sirolimus to Treat and Prevent In-Stent Restenosis: A Pilot Study Results," *American Heart Association*, 2002, p. 2929.
- Lima et al., "Systemic Immunosuppression Inhibits In-Stent Coronary Intimal Proliferation in Renal Transplant Patients," *American Heart Association*, 2002, p. 2928.
- Morice et al., "A Randomized Comparison of a Sirolimus-Eluting Stent With a Standard Stent for Coronary Revascularization," *The New England Journal of Medicine*, Jun. 6, 2012, p. 1773-1780, vol. 346, No. 23.
- Muller-Leisse et al., "Effectiveness and Safety of Ultrasonic Atherosclerotic Plaque Ablation: In Vitro Investigation," *CardioVascular and Interventional Radiology*, 1993, p. 303-307, vol. 16.
- Nair et al., "Regularized Autoregressive Analysis of Intravascular Ultrasound Backscatter: Improvement in Spatial Accuracy of Tissue Maps," *IEEE Transactions on Ultrasonics*, Apr. 2004, p. 420-431, vol. 51, No. 4.
- Popma et al., "Percutaneous Coronary and Valvular Intervention," p. 1364-1405.
- Resar et al., "Endoluminal Sealing of Vascular Wall Disruptions With Radiofrequency-Heated Balloon Angioplasty," *Catheterization and Cardiovascular Diagnosis*, 1993, p. 161-167, vol. 29.
- Romer et al., "Histopathology of Human Coronary Atherosclerosis by Quantifying Its Chemical Composition With Raman Spectroscopy," *Circulation*, 1998, p. 878-885, vol. 97.
- Schauerte et al., "Catheter Ablation of Cardiac Autonomic Nerves for Prevention of Vagal Atrial Fibrillation," *Circulation*, 2000, p. 2774-2780, vol. 102.
- Scheller et al., "Intracoronary Paclitaxel Added to Contrast Media Inhibits In-Stent Restenosis of Porcine Coronary Arteries," *American Heart Association*, 2002, p. 2227.
- Scheller et al., "Potential solutions to the current problem: coated balloon," *EuroIntervention*, 2008, p. C63-C66, vol. 4 (Supplement C).
- Shaffer, "Scientific basis of laser energy," *Clinics in Sports Medicine*, 2002, p. 585-598, vol. 21.
- Shmatukha et al., "MRI temperature mapping during thermal balloon angioplasty," *Physics in Medicine and Biology*, 2006, p. N163-N171, vol. 51.
- Slager et al., "Vaporization of Atherosclerotic Plaques by Spark Erosion," *J Am Coll Cardiol*, 1985, p. 21-25.
- Stiles et al., "Simulated Characterization of Atherosclerotic Lesions in the Coronary Arteries by Measurement of Bioimpedance," *IEEE Transactions on Biomedical Engineering*, Jul. 2003, p. 916-921, vol. 50, No. 7.
- Suselbeck et al., "In vivo intravascular electric impedance spectroscopy using a new catheter with integrated microelectrodes," *Basic Res Cardiol*, 2005, p. 28-34, vol. 100.
- Suselbeck et al., "Intravascular electric impedance spectroscopy of atherosclerotic lesions using a new impedance catheter system," *Basic Res Cardiol*, 2005, p. 446-452, vol. 100.
- Tepe et al., "Local Delivery of Paclitaxel to Inhibit Restenosis during Angioplasty of the Leg," *The New England Journal of Medicine*, 2008, p. 689-699, vol. 358.
- CardioVascular Technologies Inc., "Heated Balloon Device Technology," 11 pages, 2008.
- Strategic Business Development, Inc., "Thermal and Disruptive Angioplasty: A Physician's Guide," 8 pages, 1990.
- Zhang et al., "Non-contact Radio-Frequency Ablation for Obtaining Deeper Lesions," *IEEE Transaction on Biomedical Engineering*, vol. 50, No. 2, 6 pages, Feb. 2003.
- Lazebnik et al., "Tissue Strain Analytics Virtual Touch Tissue Imaging and Qualification," *Siemens Whitepaper*, Oct. 2008, 7 pages.
- Han et al., "Third-Generation Cryosurgery for Primary and Recurrent Prostate Cancer," *BJU International*, vol. 93, pp. 14-18.
- Zhou et al., "Mechanism Research of Cryoanalgesia," *Forefront Publishing Group*, 1995.
- Florete, "Cryoblation Procedure for Back Pain," *Jacksonville Medicine*, Oct. 1998, 10 pages.
- Stevenson, "Irrigated RF Ablation: Power Titration and Fluid Management for Optimal Safety Efficacy," 2005, 4 pages.
- Giliatt et al., "The Cause of Nerve Damage in Acute Compression," *Trans Am Neurol Assoc*, 1974: 99; 71-4.
- Omura et al., "A Mild Acute Compression Induces Neurapraxia in Rat Sciatic Nerve," *The International Journal of Neuroscience*, vol. 114 (12), pp. 1561-1572.
- Baun, "Interaction with Soft Tissue," *Principles of General & Vascular Sonography*, Chapter 2, pp. 23-24, Before Mar. 2012.
- Blue Cross Blue Shield Medical Policy, "Surgery Section—MRI-Guided Focused Ultrasound (MRgFUS) for the Treatment of Uterine Fibroids and Other Tumors," 2005, 5 pages.
- Gentry et al., "Combines 3D Intracardiac Echo and Ultrasound Ablation," *Medical Imaging 2003: Ultrasonic and Signal Processing*, vol. 5035, 2003, pp. 166-173.
- Lafon et al., "Optimizing the Shape of Ultrasound Transducers for Interstitial Thermal Ablations," *MED Phys*, Mar. 2002; 29(3): 290-7 (abstract only).
- G. Ter Haar, "Ultrasound Focal Beam Surgery," *Ultrasound in Med. & Biol.*, 1995, vol. 21, No. 9, pp. 1089-1100.
- Seip et al., "Transurethral High Intensity Focused Ultrasound: Catheter Based Prototypes and Experimental Results," *IEEE Ultrasonics Symposium Proceeding*, 2000, 4 pages.
- Toytman et al., "Tissue Dissection with Ultrafast Laser Using Extended and Multiple Foci," *SPIE Proceeding, Optical Interactions with Tissues and Cells XXI*, vol. 7562, 2010, 10 pages.
- Zhou et al., "Non-Thermal Ablation of Rabbit Liver VX2 Tumor by Pulsed High Intensity Focused Ultrasound Contrast Agent: Pathological Characteristics," *World Journal of Gastroenterology*, vol. 14(43), Nov. 21, 2008, pp. 6743-6747.
- US 8,398,630, 03/2013, Demarais et al. (withdrawn)

* cited by examiner

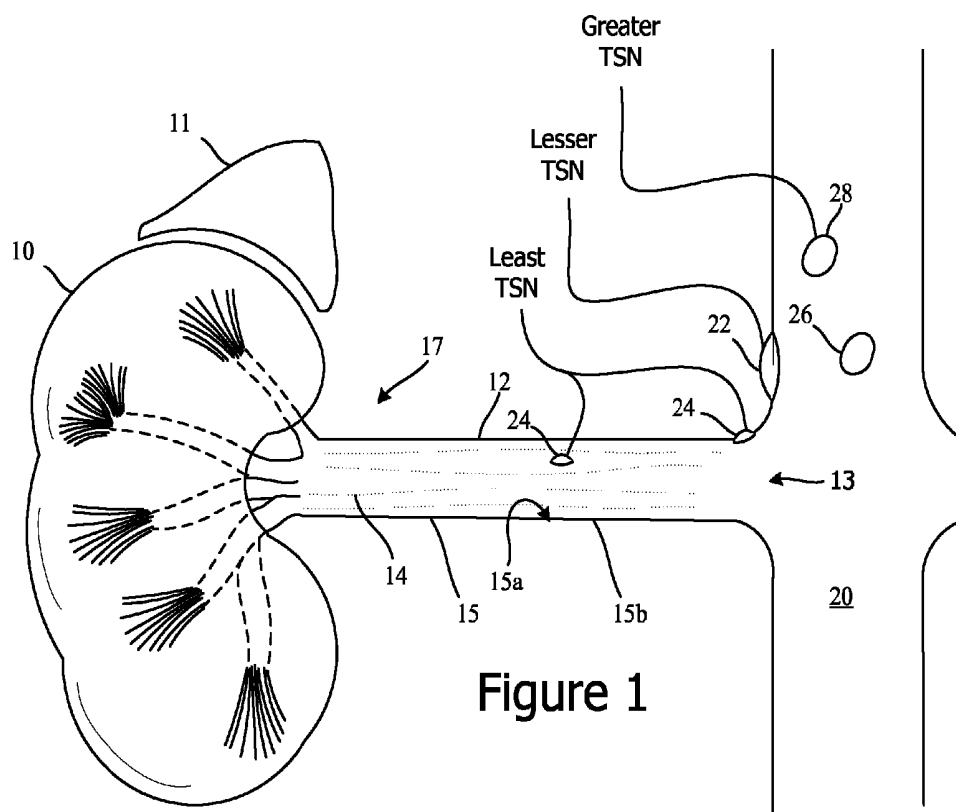


Figure 1

Figure 2A

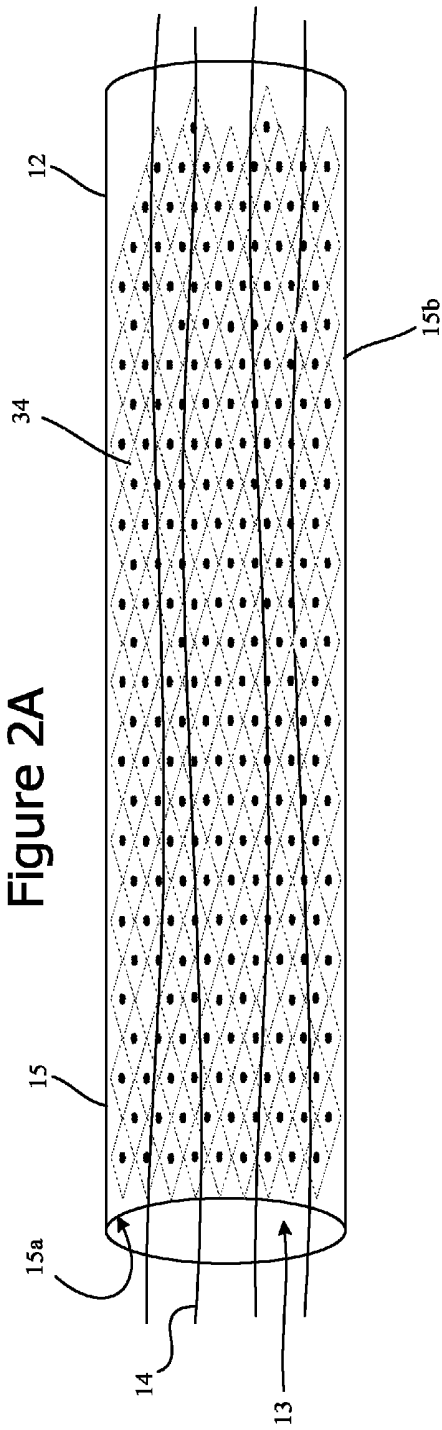
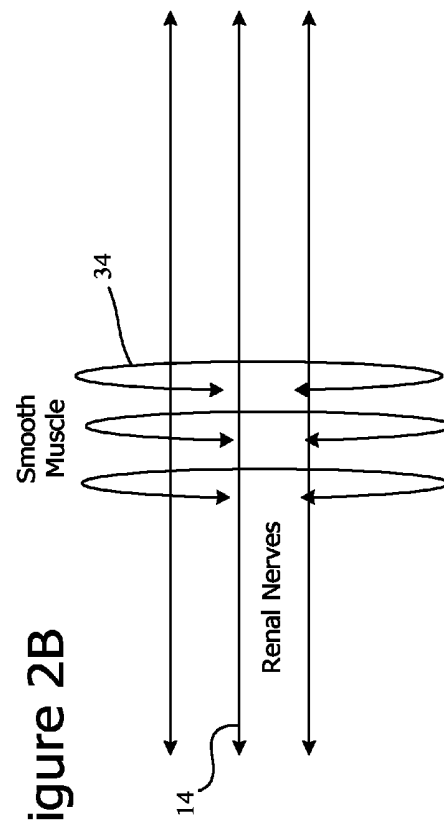


Figure 2B



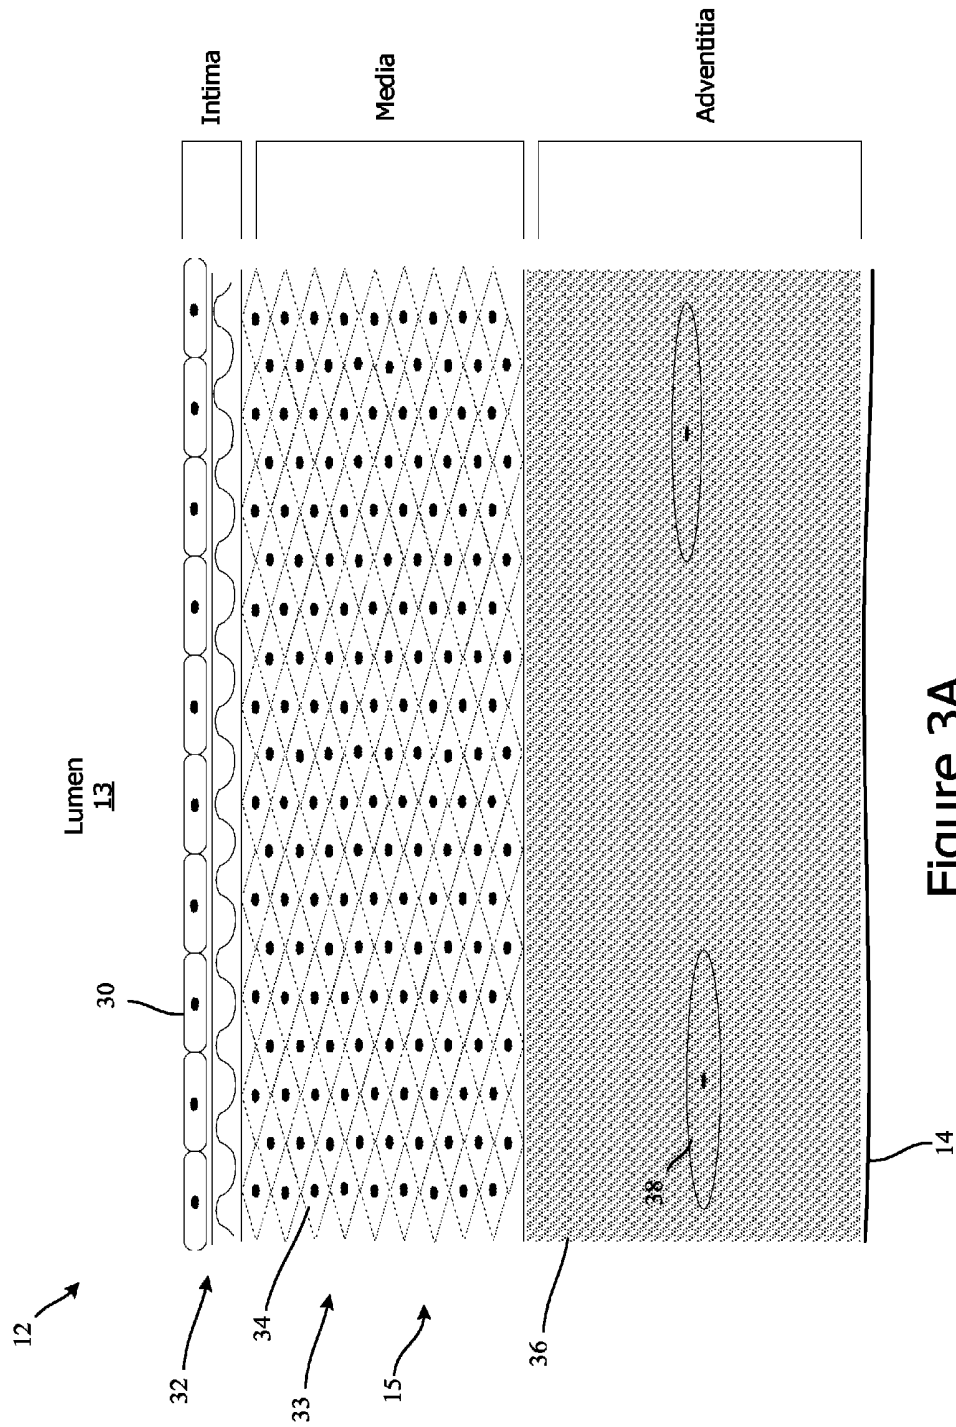


Figure 3A

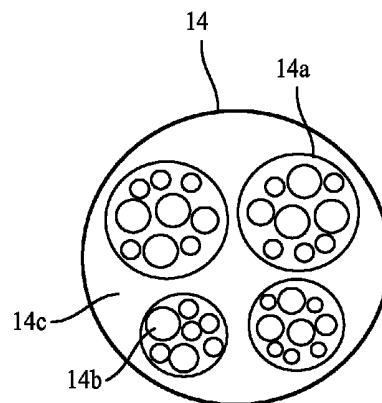
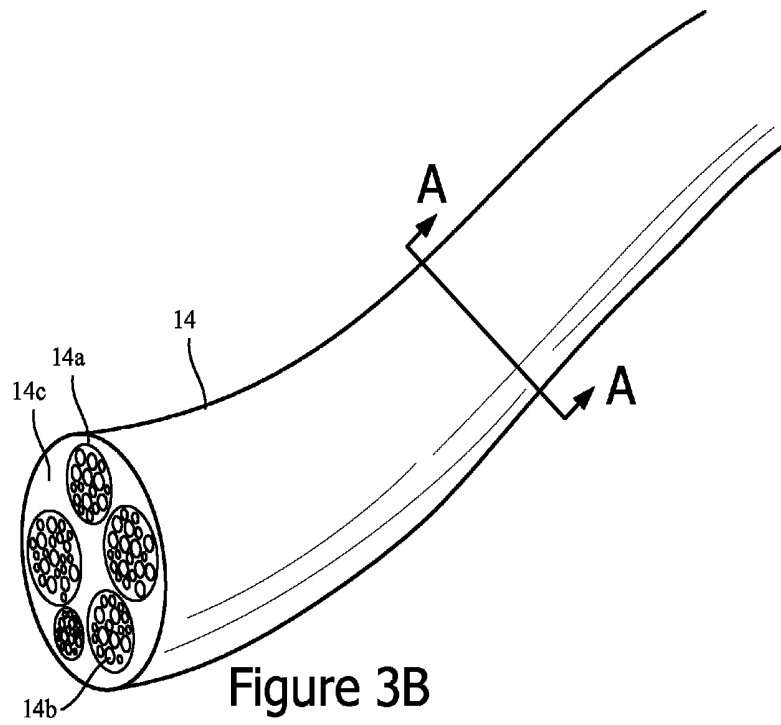


Figure 3C

Figure 4

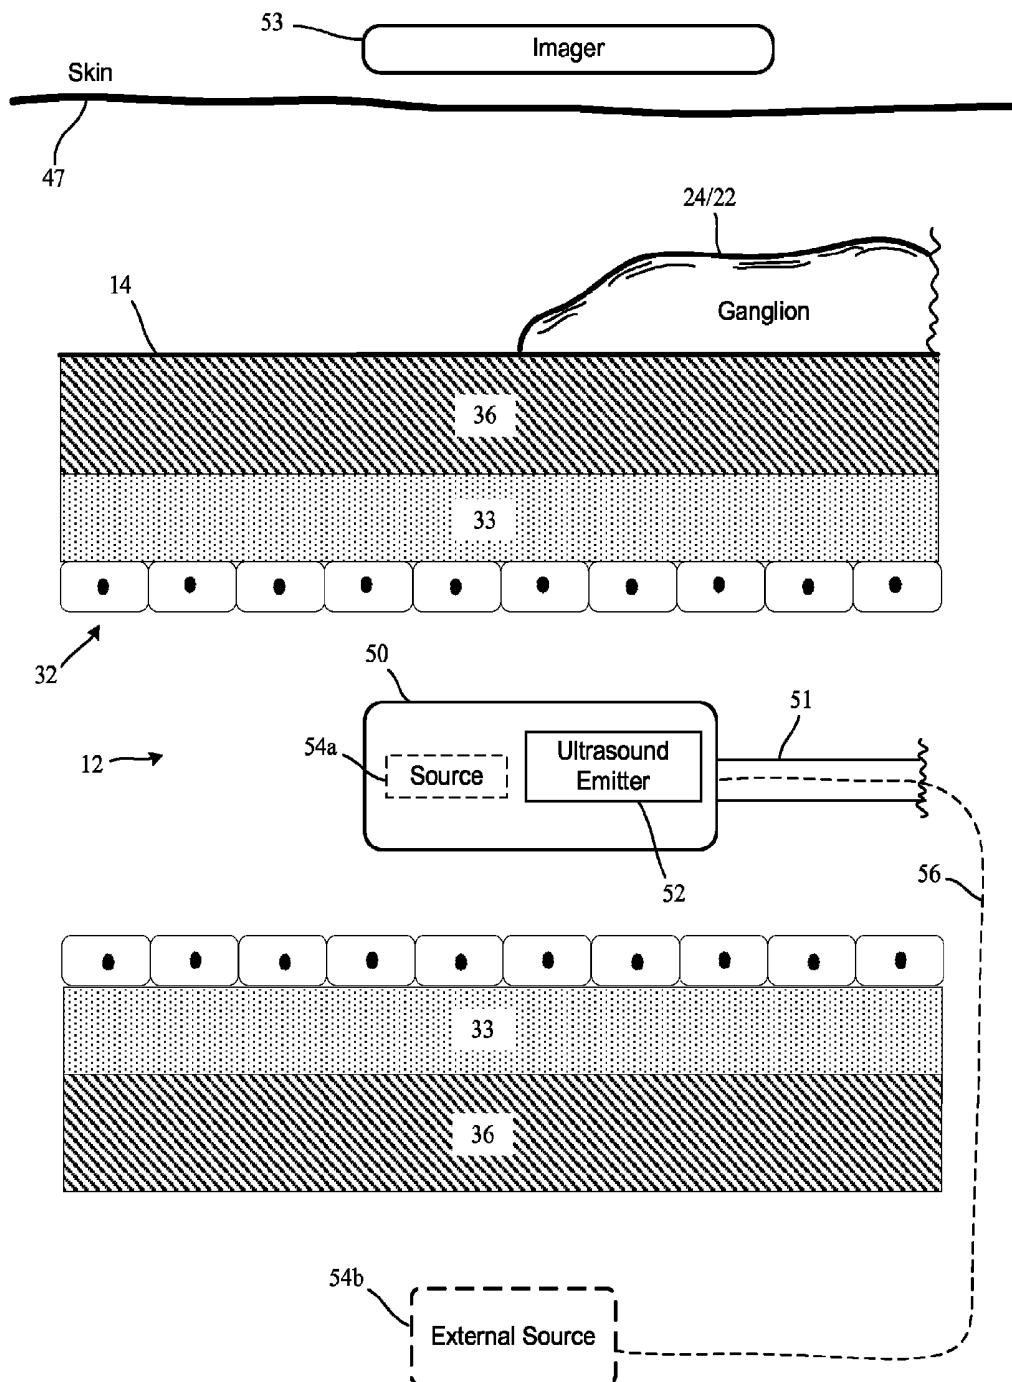


Figure 5

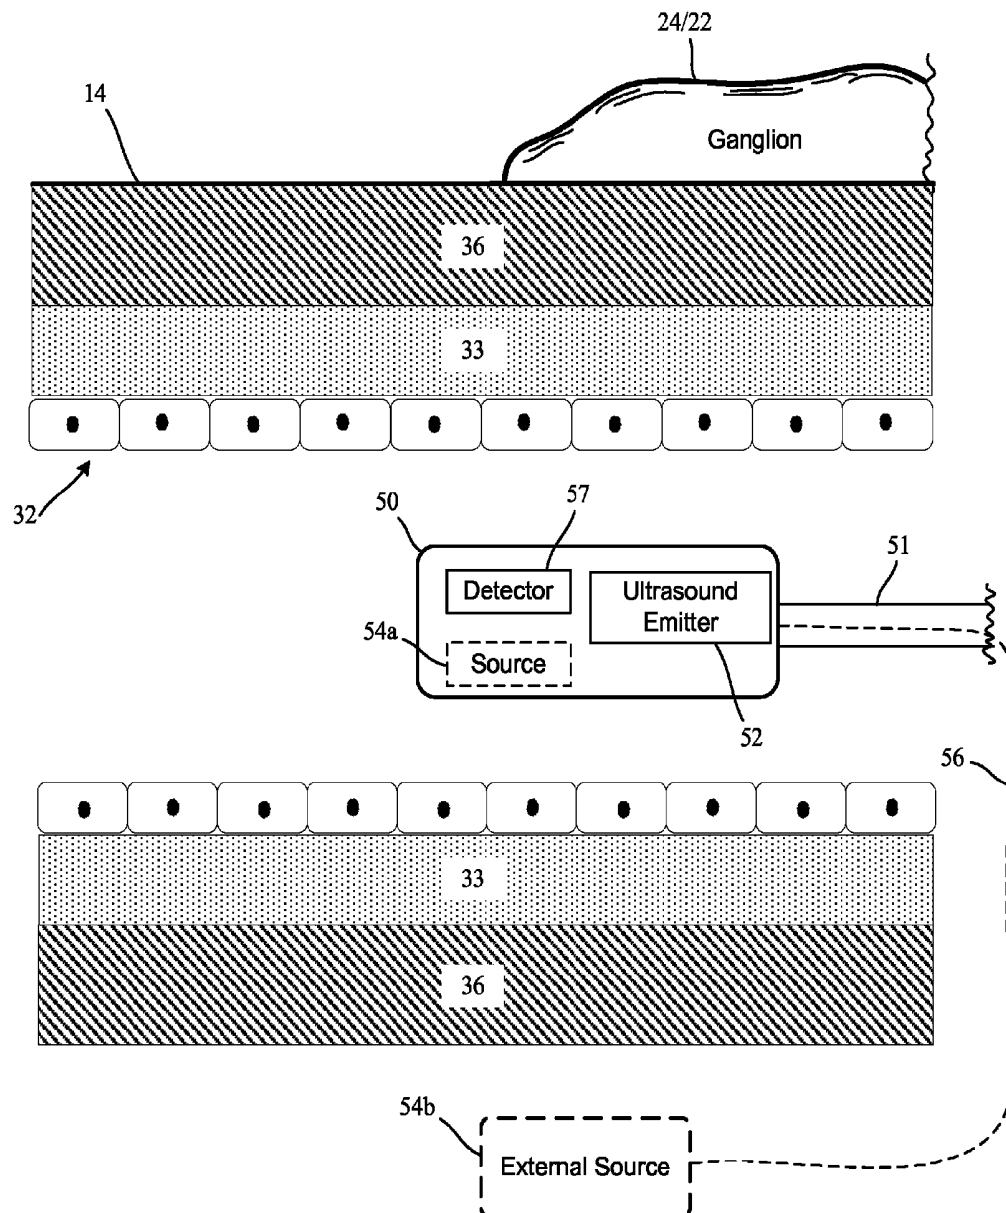
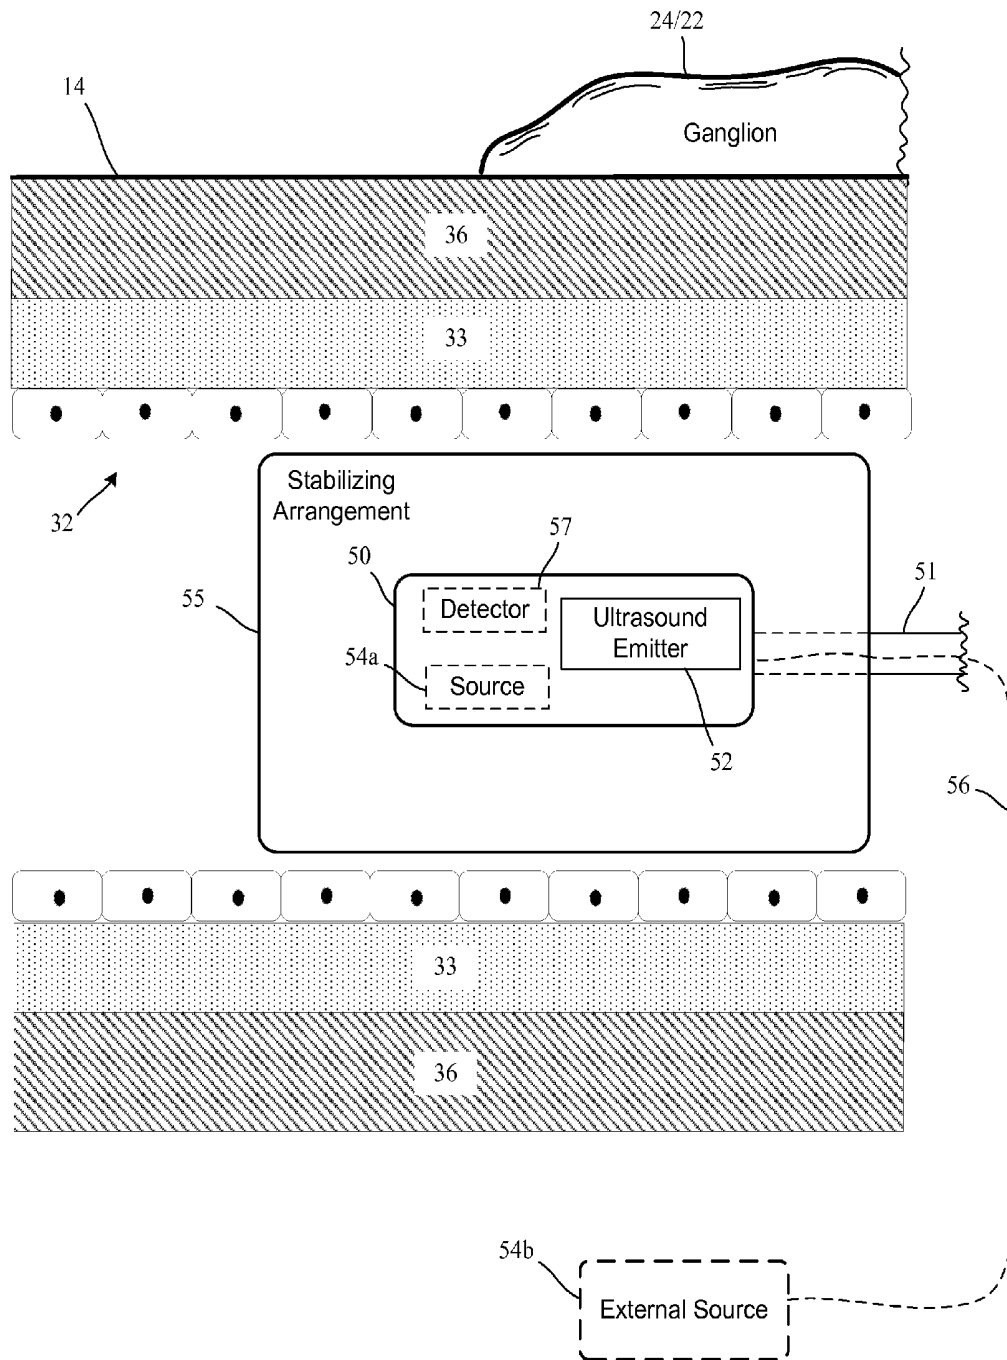


Figure 6



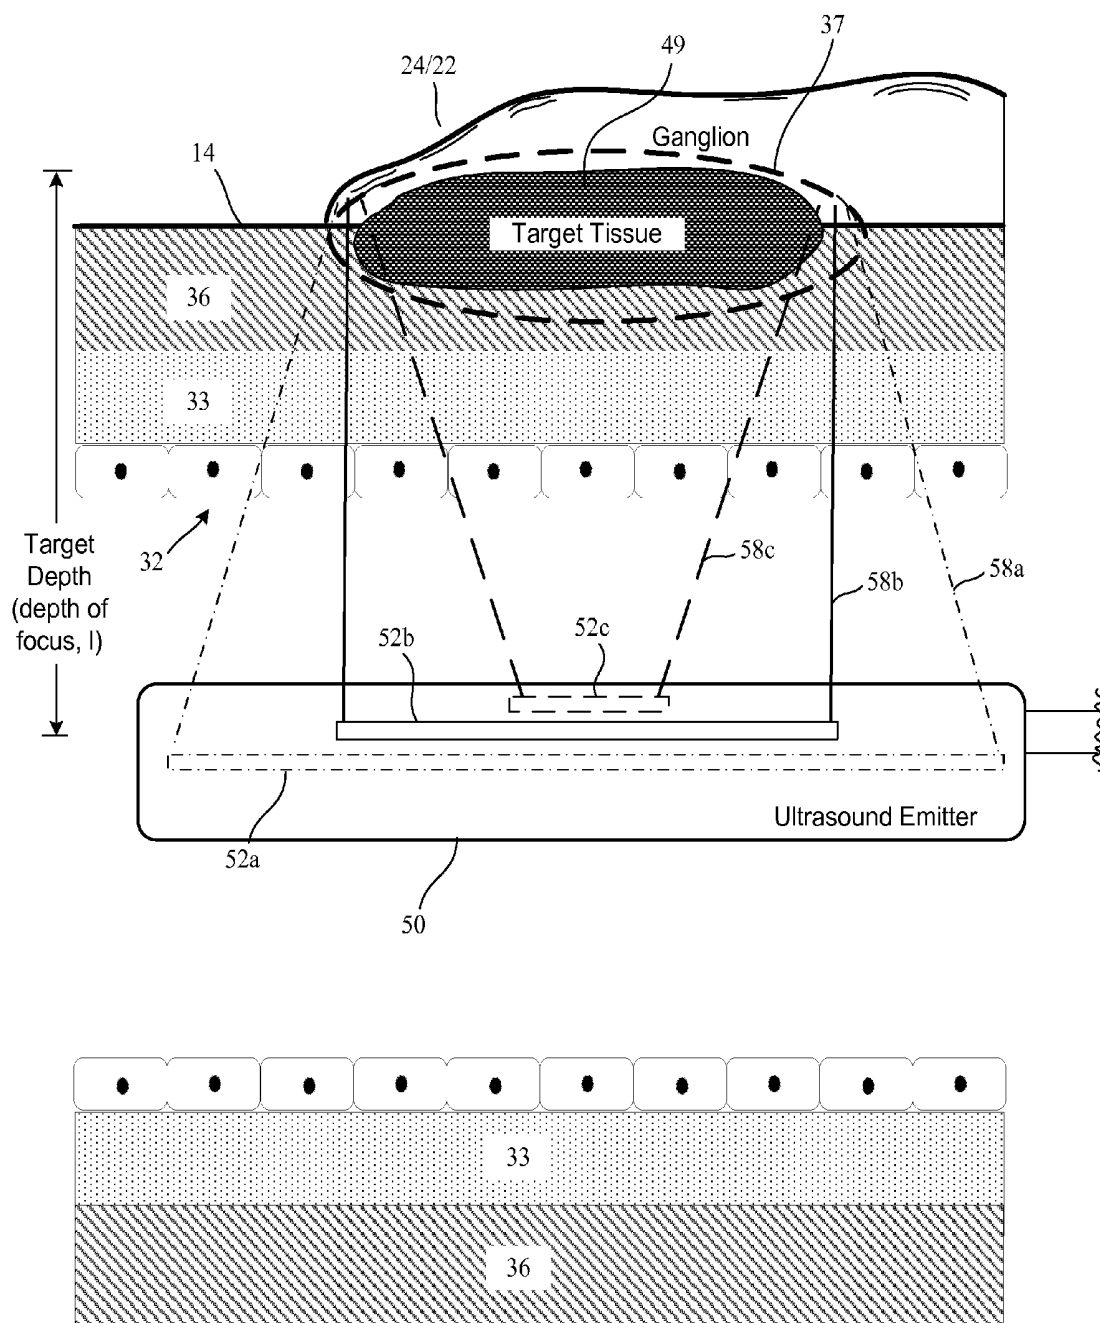
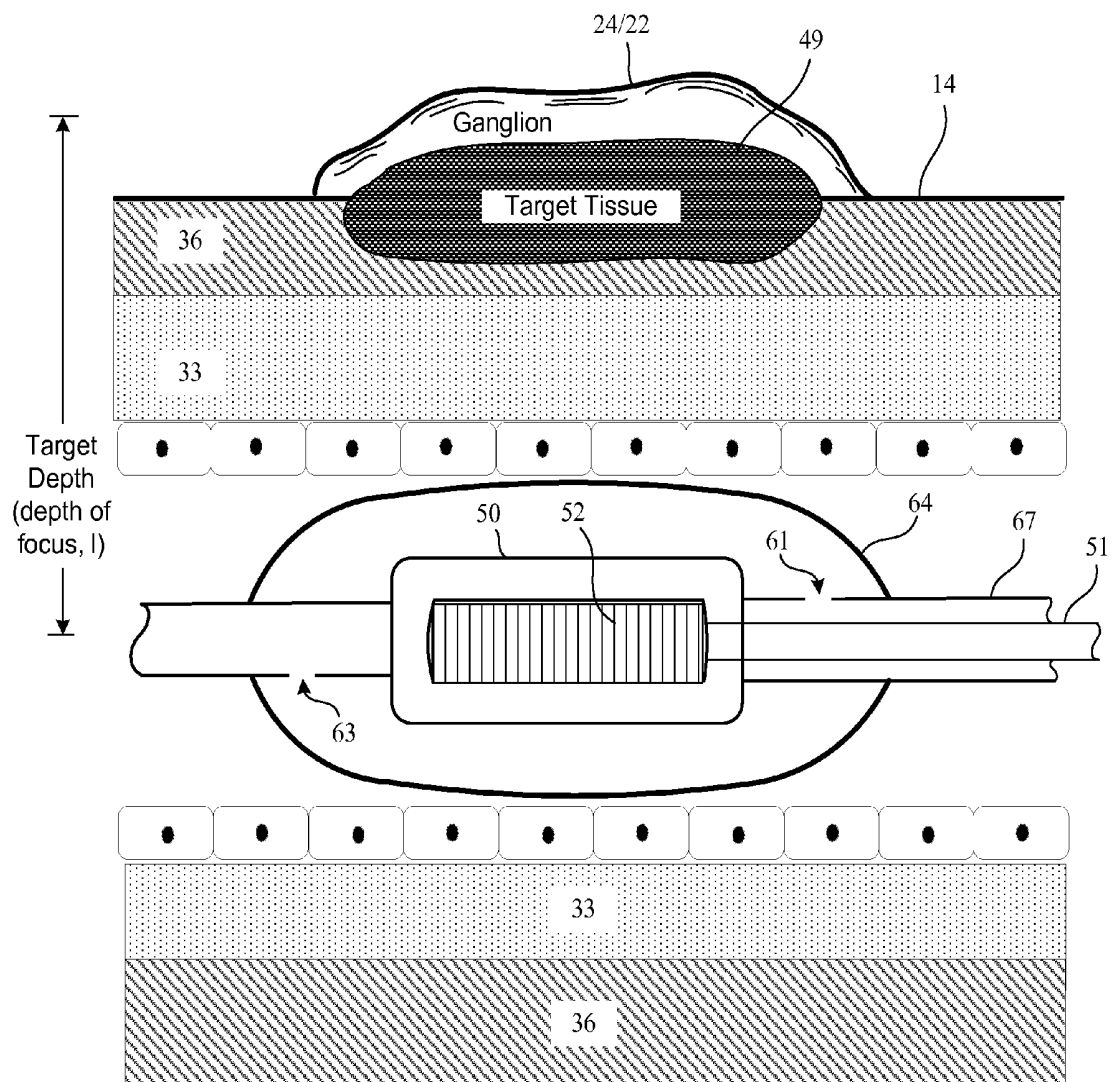


Figure 7

Figure 8



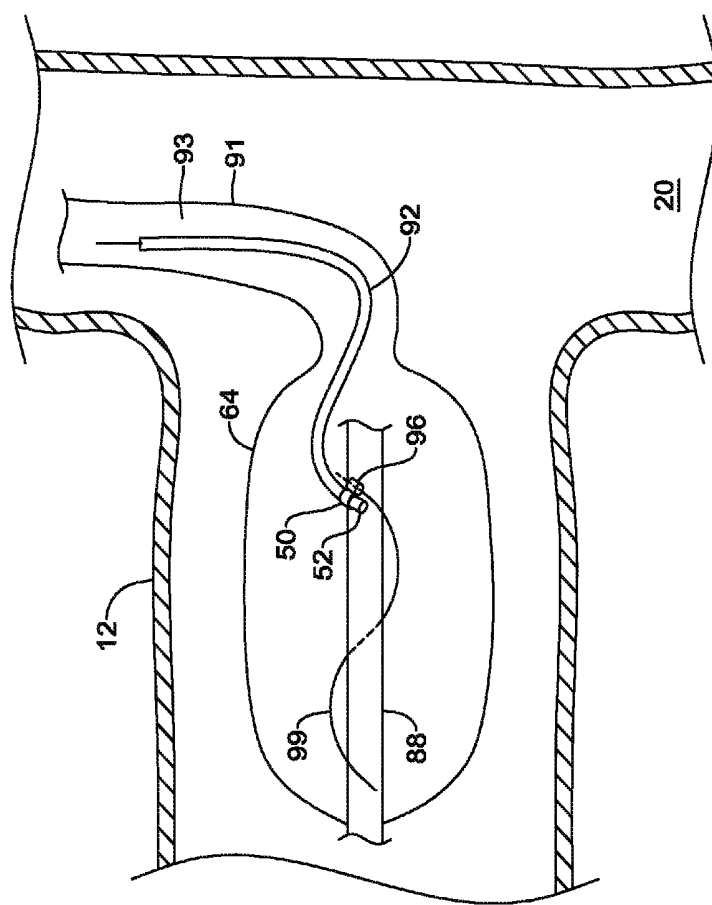


Figure 9

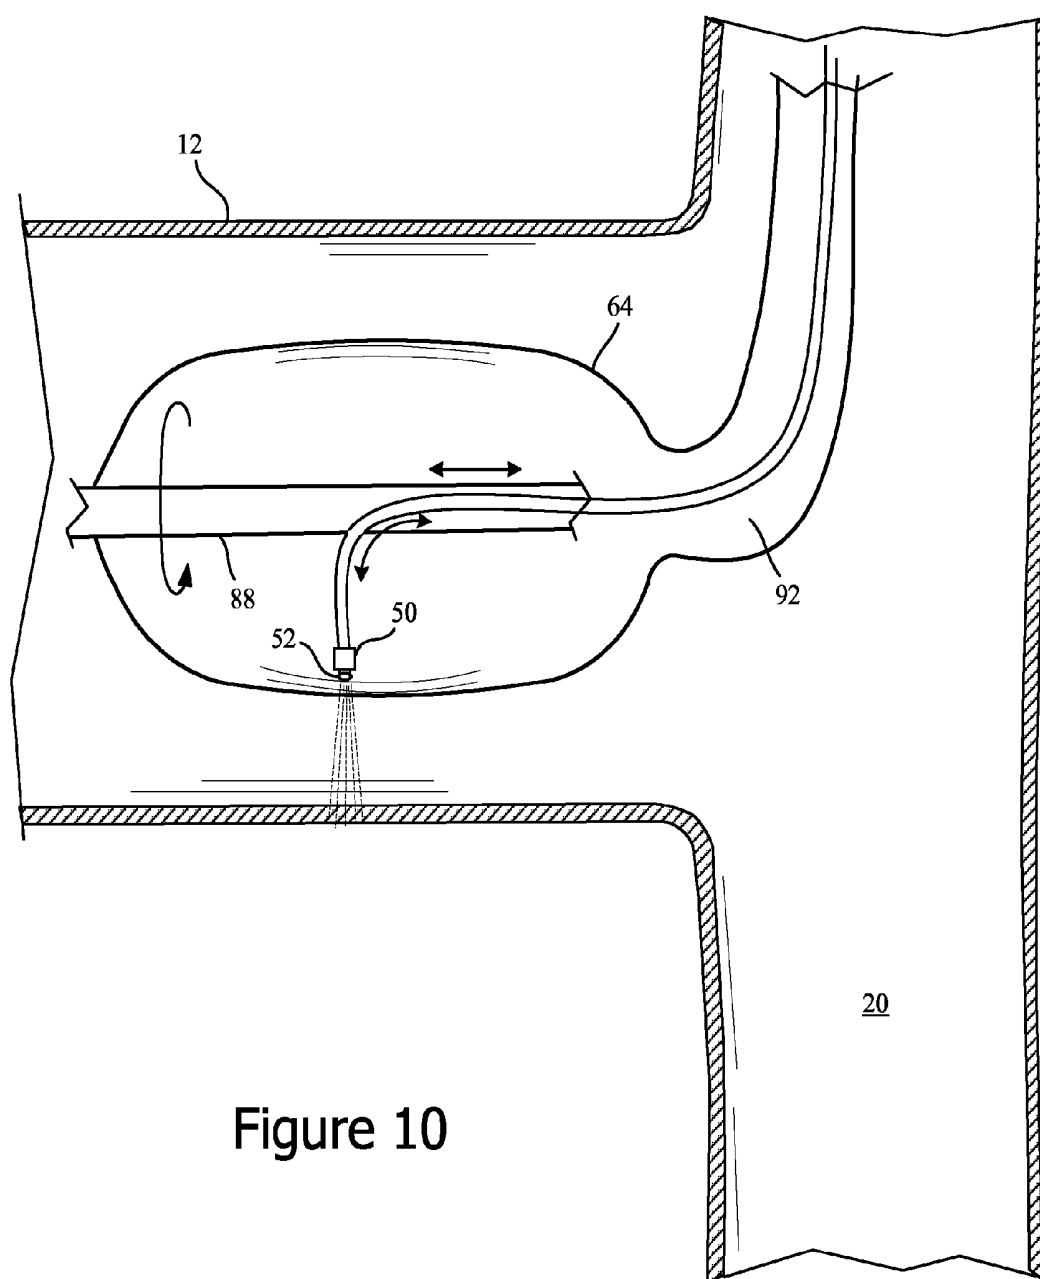


Figure 10

Figure 11

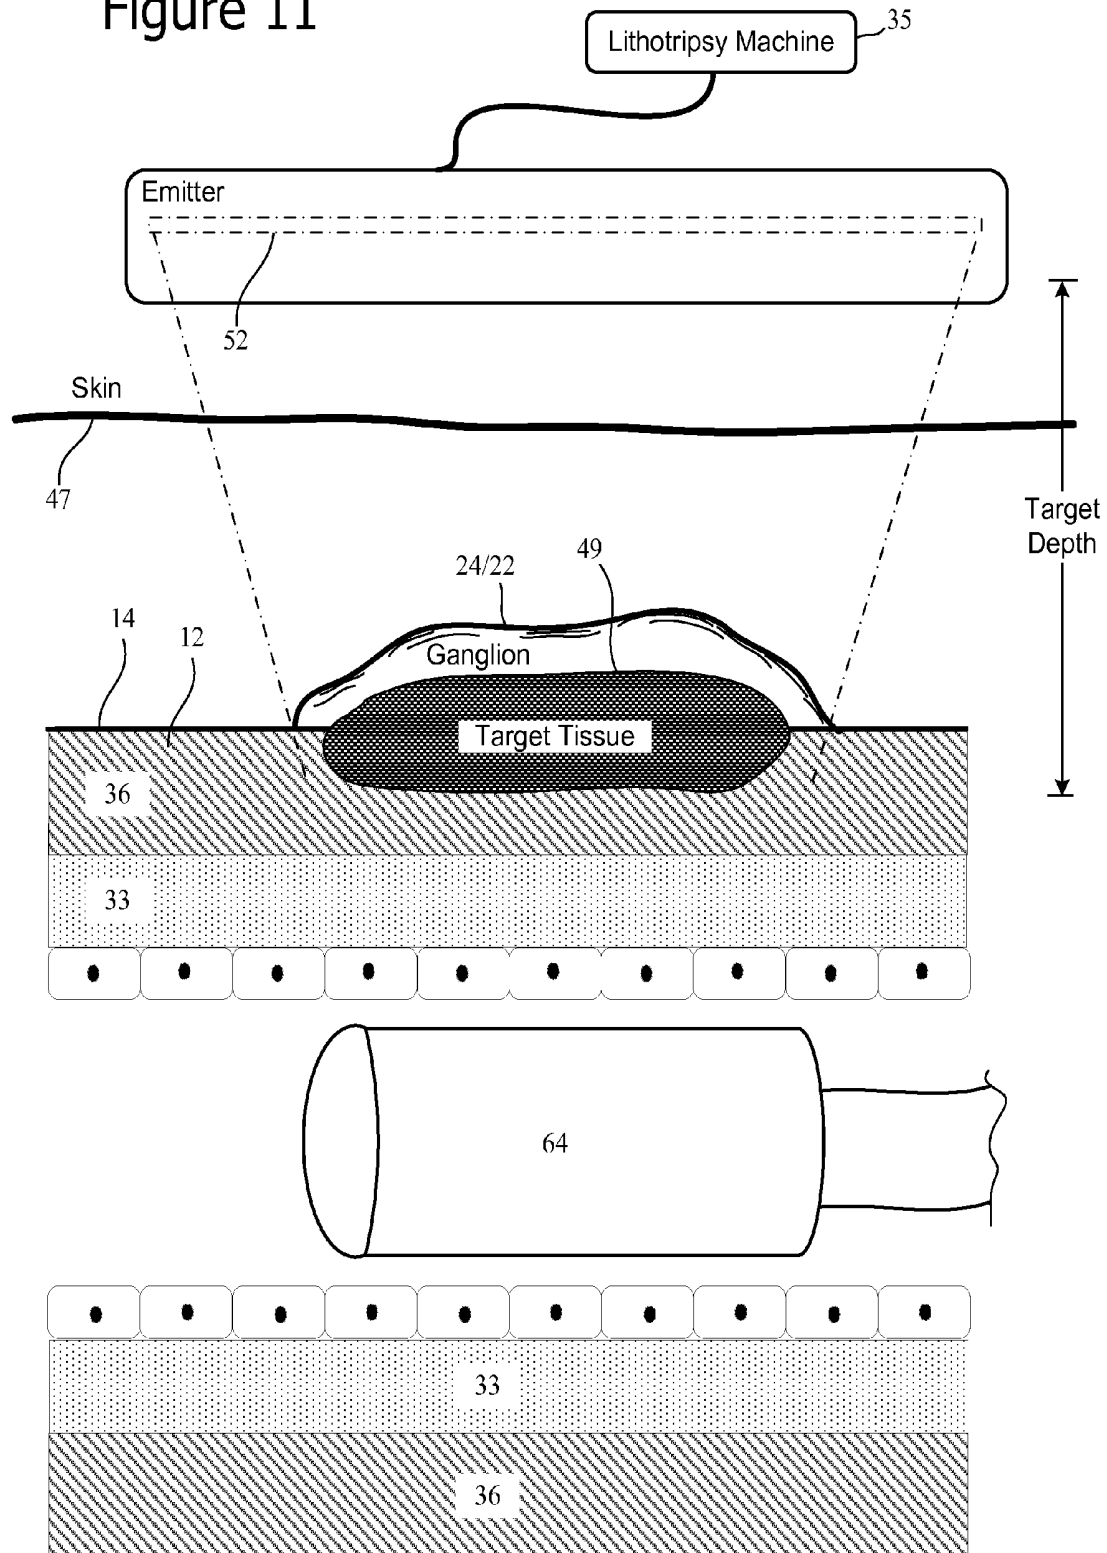


Figure 12A

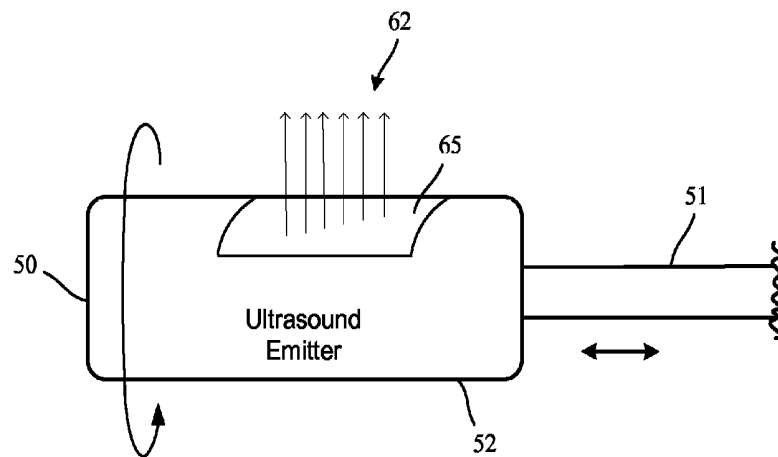
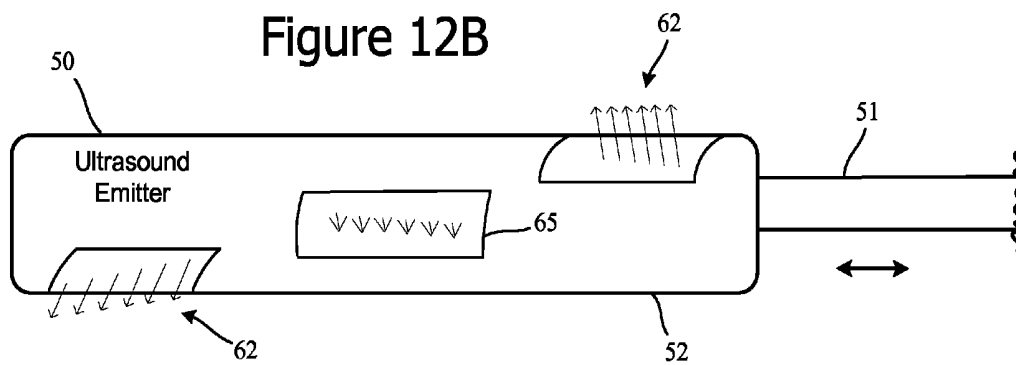


Figure 12B



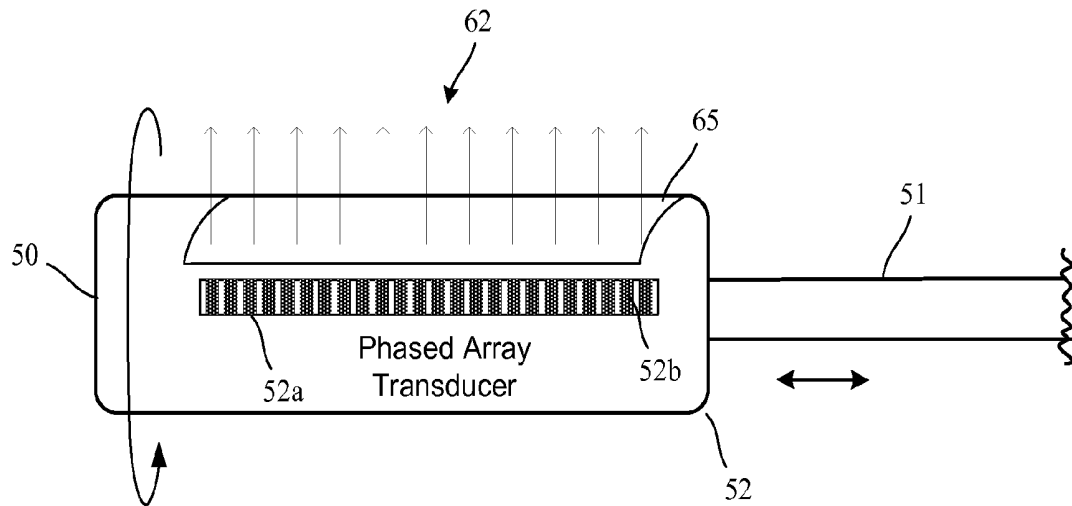


Figure 12C

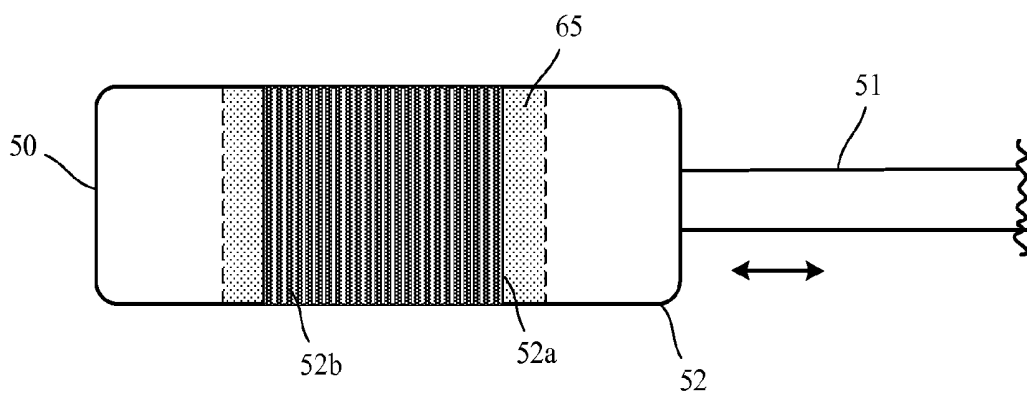


Figure 12D

Figure 13A

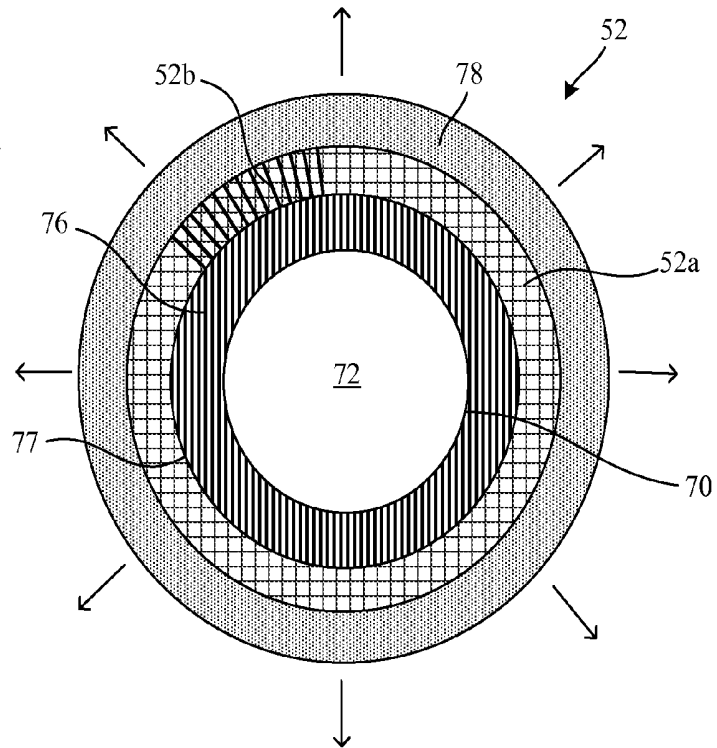
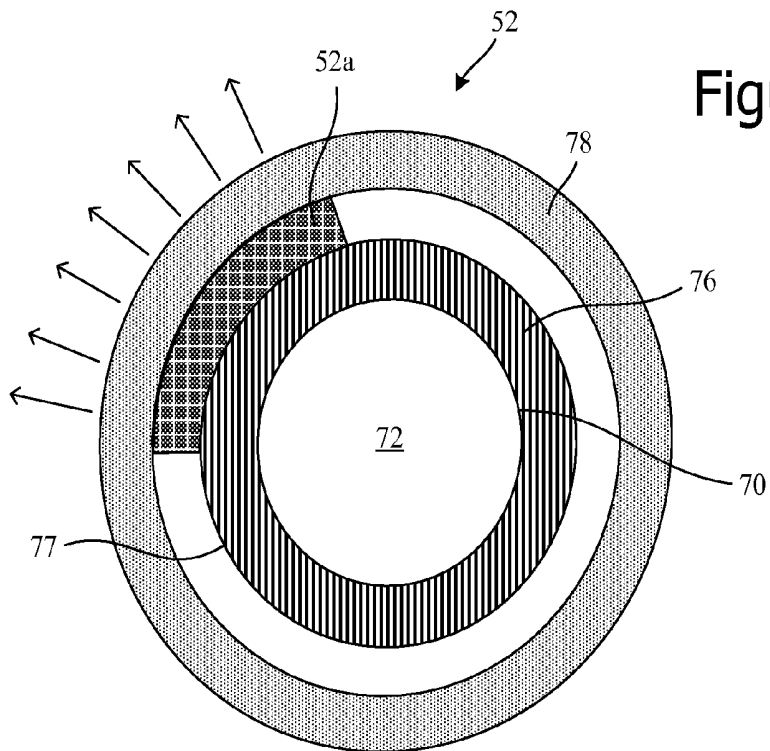
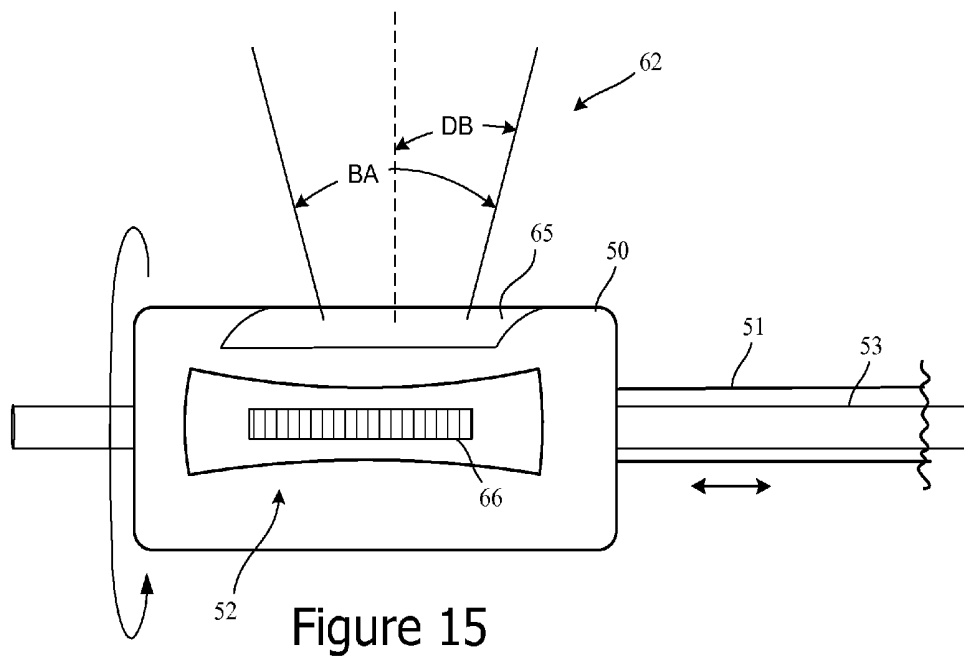
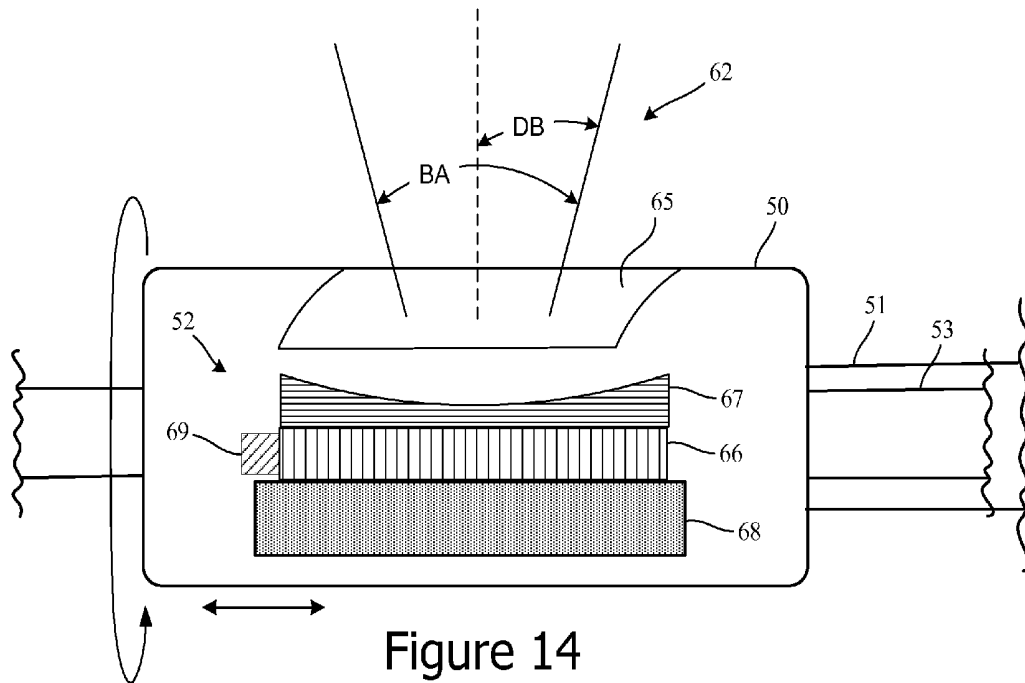


Figure 13B





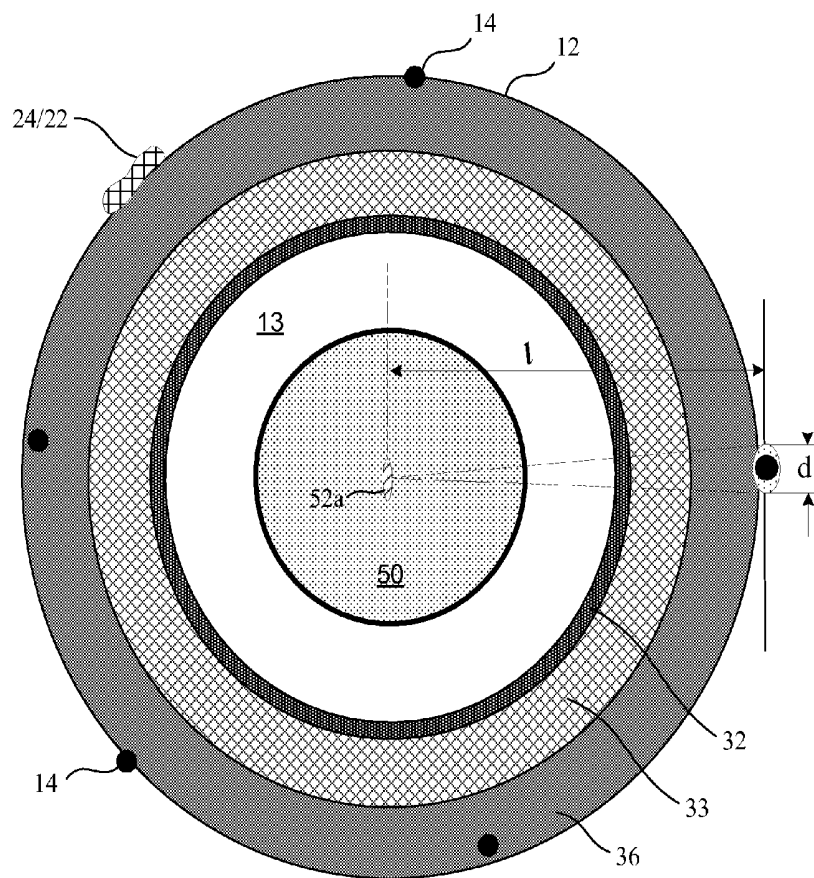


Figure 16

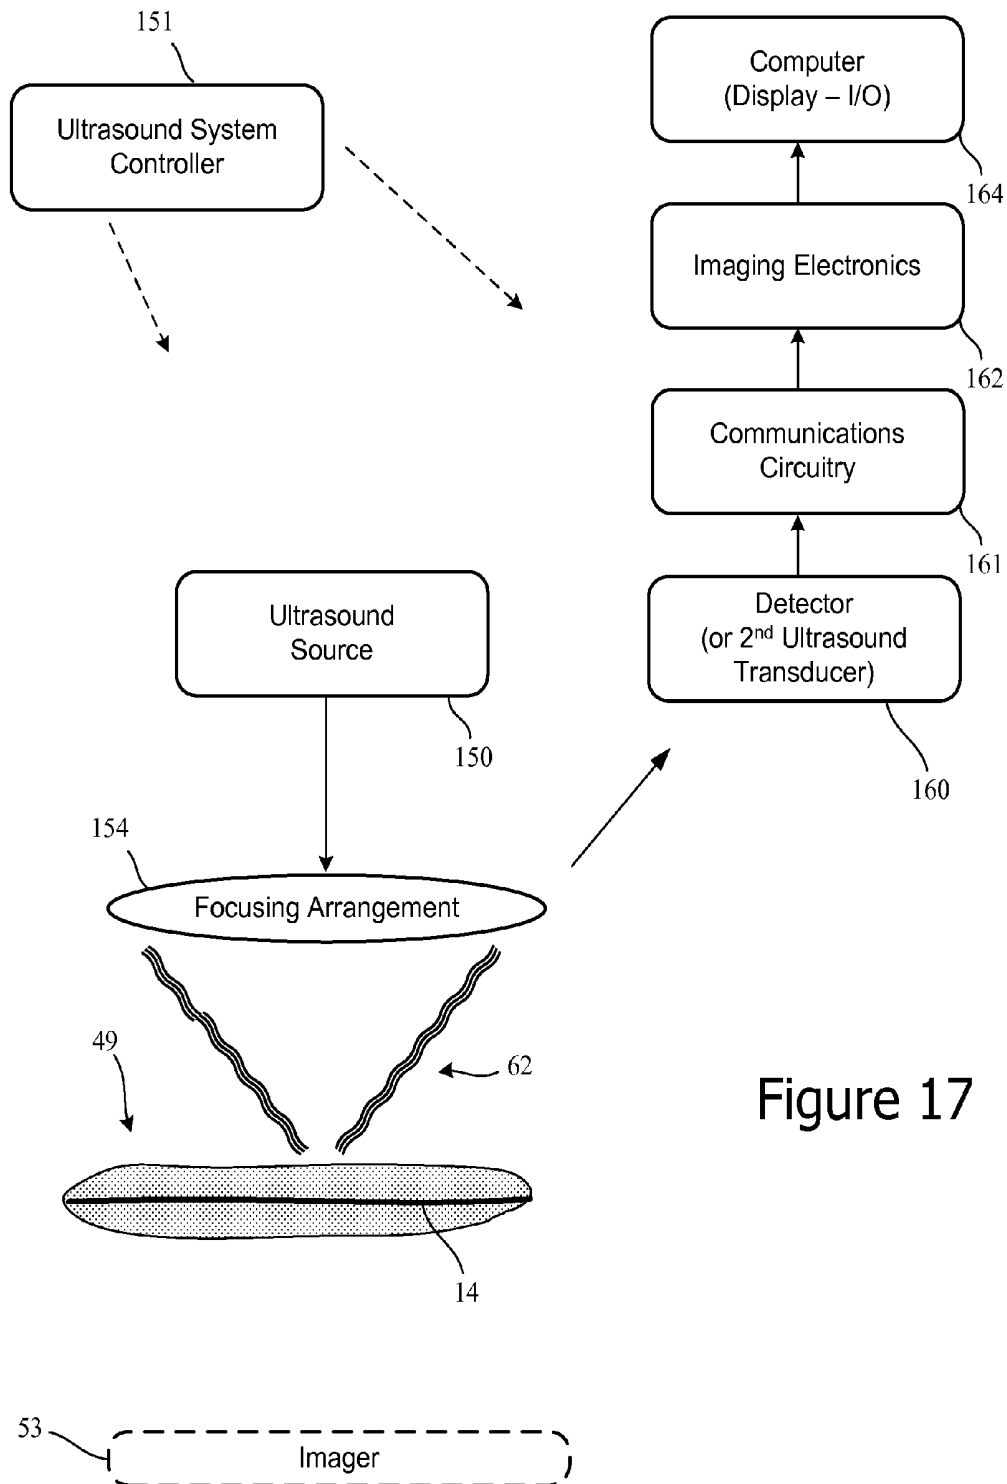


Figure 17

Figure 18A

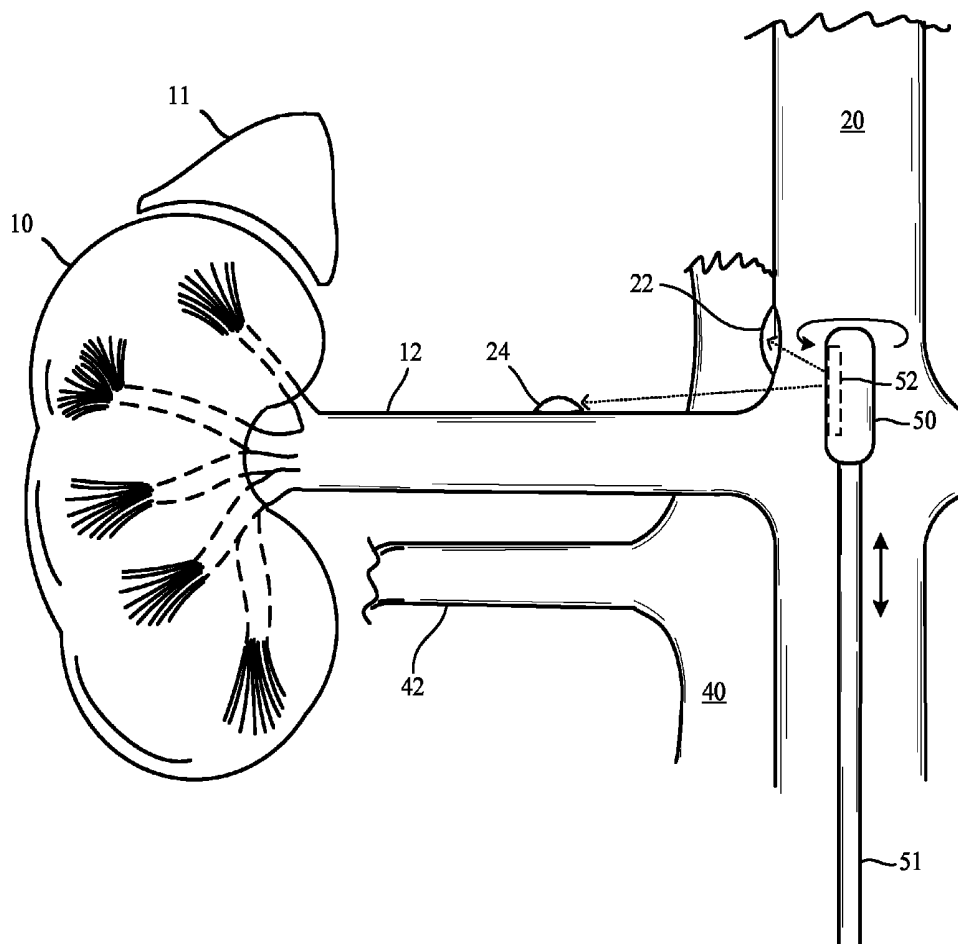


Figure 18B

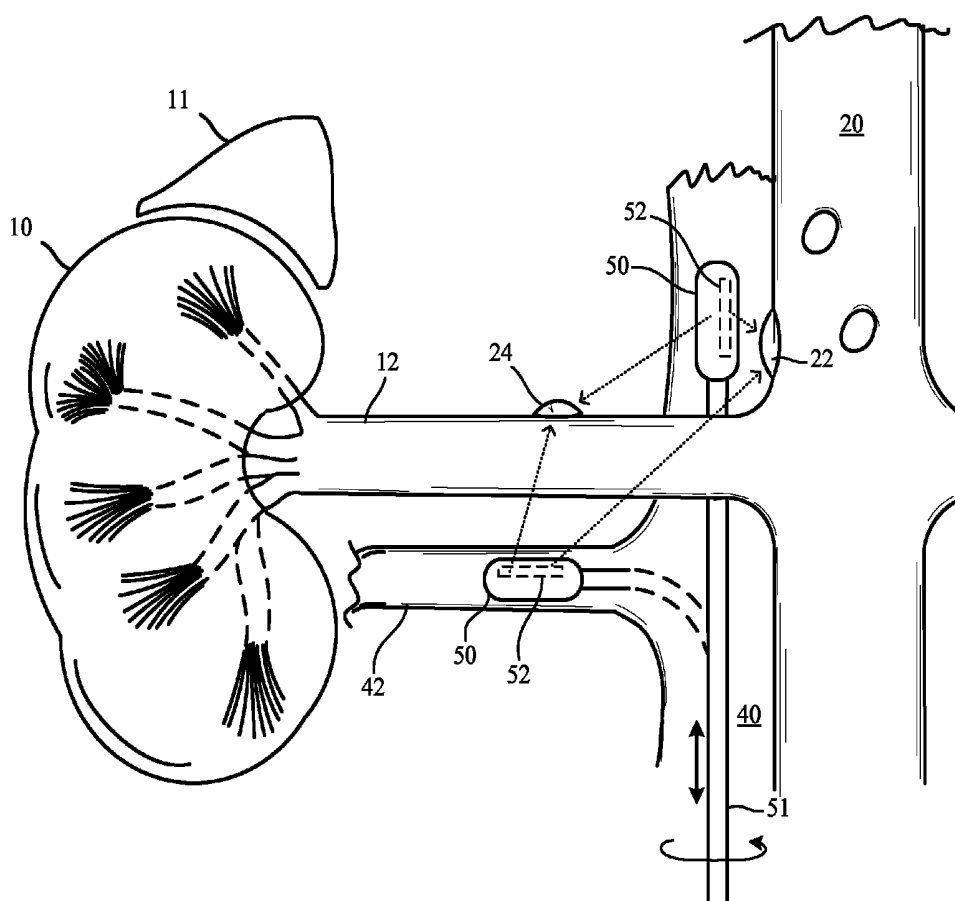
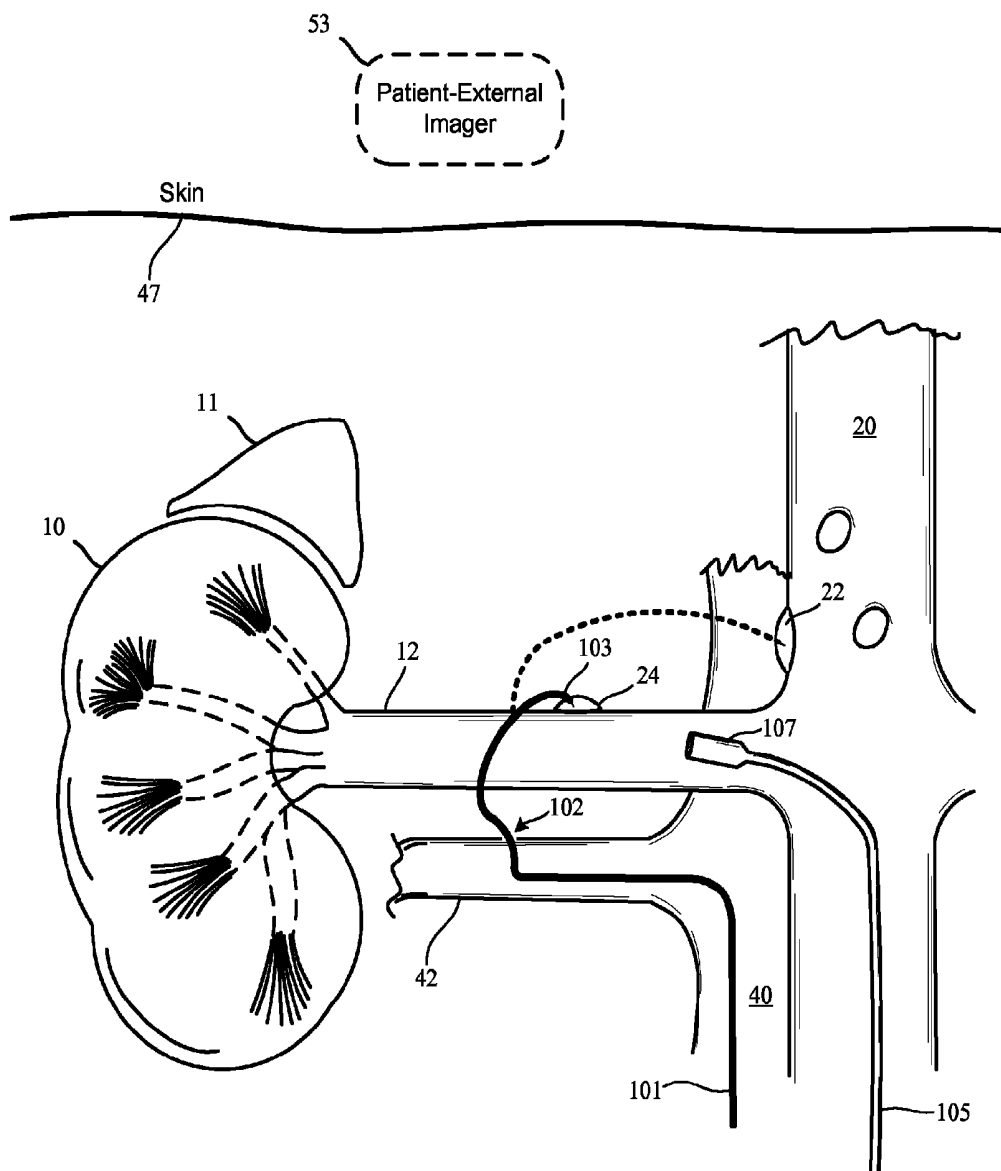


Figure 19



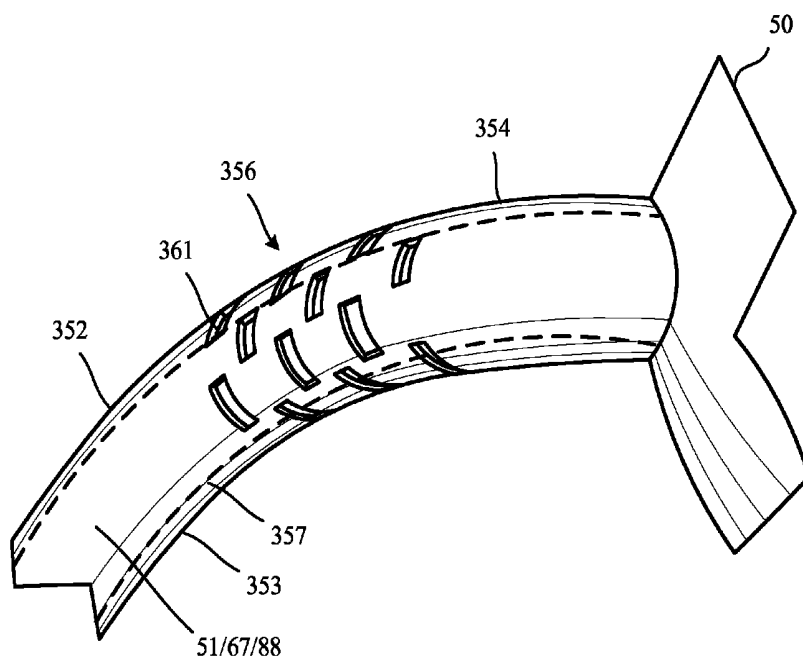


Figure 20

FOCUSED ULTRASONIC RENAL DENERVATION

RELATED APPLICATIONS

This application claims the benefit of Provisional Patent Application Ser. No. 61/324,164 filed on Apr. 14, 2010, to which priority is claimed pursuant to 35 U.S.C. §119(e) and which is hereby incorporated herein by reference in its entirety.

TECHNICAL FIELD

The present invention is related to systems and methods for denervating renal vasculature, including disruption and termination of renal sympathetic nerve activity, to improve cardiac and/or renal function.

BACKGROUND

The kidneys are instrumental in a number of body processes, including blood filtration, regulation of fluid balance, blood pressure control, electrolyte balance, and hormone production. One primary function of the kidneys is to remove toxins, mineral salts, and water from the blood to form urine. The kidneys receive about 20-25% of cardiac output through the renal arteries that branch left and right from the abdominal aorta, entering each kidney at the concave surface of the kidneys, the renal hilum.

Blood flows into the kidneys through the renal artery and the afferent arteriole, entering the filtration portion of the kidney, the renal corpuscle. The renal corpuscle is composed of the glomerulus, a thicket of capillaries, surrounded by a fluid-filled, cup-like sac called Bowman's capsule. Solutes in the blood are filtered through the very thin capillary walls of the glomerulus due to the pressure gradient that exists between the blood in the capillaries and the fluid in the Bowman's capsule. The pressure gradient is controlled by the contraction or dilation of the arterioles. After filtration occurs, the filtered blood moves through the efferent arteriole and the peritubular capillaries, converging in the interlobular veins, and finally exiting the kidney through the renal vein.

Particles and fluid filtered from the blood move from the Bowman's capsule through a number of tubules to a collecting duct. Urine is formed in the collecting duct and then exits through the ureter and bladder. The tubules are surrounded by the peritubular capillaries (containing the filtered blood). As the filtrate moves through the tubules and toward the collecting duct, nutrients, water, and electrolytes, such as sodium and chloride, are reabsorbed into the blood.

The kidneys are innervated by the renal plexus which emanates primarily from the aorticorenal ganglion. Renal ganglia are formed by the nerves of the renal plexus as the nerves follow along the course of the renal artery and into the kidney. The renal nerves are part of the autonomic nervous system which includes sympathetic and parasympathetic components. The sympathetic nervous system is known to be the system that provides the bodies "fight or flight" response, whereas the parasympathetic nervous system provides the "rest and digest" response. Stimulation of sympathetic nerve activity triggers the sympathetic response which causes the kidneys to increase production of hormones that increase vasoconstriction and fluid retention. This process is referred to as the renin-angiotensin-aldosterone-system (RAAS) response to increased renal sympathetic nerve activity.

In response to a reduction in blood volume, the kidneys secrete renin, which stimulates the production of angiotensin.

Angiotensin causes blood vessels to constrict, resulting in increased blood pressure, and also stimulates the secretion of the hormone aldosterone from the adrenal cortex. Aldosterone causes the tubules of the kidneys to increase the reabsorption of sodium and water, which increases the volume of fluid in the body and blood pressure.

Congestive heart failure (CHF) is a condition that has been linked to kidney function. CHF occurs when the heart is unable to pump blood effectively throughout the body. When blood flow drops, renal function degrades because of insufficient perfusion of the blood within the renal corpuscles. The decreased blood flow to the kidneys triggers an increase in sympathetic nervous system activity (i.e., the RAAS becomes too active) that causes the kidneys to secrete hormones that increase fluid retention and vasoconstriction. Fluid retention and vasoconstriction in turn increases the peripheral resistance of the circulatory system, placing an even greater load on the heart, which diminishes blood flow further. If the deterioration in cardiac and renal functioning continues, eventually the body becomes overwhelmed, and an episode of heart failure decompensation occurs, often leading to hospitalization of the patient.

Hypertension is a chronic medical condition in which the blood pressure is elevated. Persistent hypertension is a significant risk factor associated with a variety of adverse medical conditions, including heart attacks, heart failure, arterial aneurysms, and strokes. Persistent hypertension is a leading cause of chronic renal failure. Hyperactivity of the sympathetic nervous system serving the kidneys is associated with hypertension and its progression. Deactivation of nerves in the kidneys via renal denervation can reduce blood pressure, and may be a viable treatment option for many patients with hypertension who do not respond to conventional drugs.

SUMMARY

Devices, systems, and methods of the invention are directed to delivery of focused acoustic energy to innervated vasculature for one or both of imaging and ablating the innervated vasculature. Embodiments of the invention are directed to modifying renal sympathetic nerve activity using ultrasonic denervation therapy. Embodiments of the invention are directed to ultrasonic scanning or imaging of innervated tissues that contribute to renal sympathetic nerve activity.

In accordance with various embodiments, an apparatus includes a catheter configured for deployment within a vessel proximate innervated tissue that contributes to renal sympathetic nerve activity. An acoustic transducer is provided at a distal end of the catheter and dimensioned for deployment within the vessel proximate the innervated tissue. A focusing arrangement is positioned relative to the acoustic transducer and configured to focus acoustic energy outwardly beyond an inner wall of the vessel and into the innervated tissue at or proximate an outer wall of the vessel. A controller is configured to control the acoustic transducer for at least one of scanning tissue and ablating the innervated tissue. In some embodiments, the controller is configured to selectively control the acoustic transducer for scanning tissue and ablating innervated tissue.

In other embodiments, an apparatus includes a catheter configured for deployment within a vessel proximate innervated tissue, and an acoustic transducer is provided at a distal end of the catheter and dimensioned for deployment within the vessel. A focusing arrangement is positioned relative to the acoustic transducer and configured to focus acoustic energy outwardly beyond an inner wall of the vessel and into the innervated tissue at or proximate an outer wall of the

vessel. A cryoballoon is dimensioned for deployment within the vessel and configured to freeze the innervated tissue. The acoustic transducer and focusing arrangement cooperate to deliver acoustic energy to frozen innervated tissue at an intensity sufficient to disrupt nerve cells of the innervated tissue.

According to some embodiments of the invention, an apparatus for facilitating delivery of acoustic energy to innervated vasculature includes a catheter configured for intravascular deployment and an ultrasound unit coupled to the catheter. An acoustic phased array transducer is provided at a distal end of the catheter and coupled to the ultrasound unit. The phased array transducer comprises a multiplicity of acoustic elements. Driver electronics are coupled to the phased array transducer. A controller is coupled to the driver electronics and configured to control activation of each of the acoustic elements of the phased array transducer for one or both of scanning and ablating target tissue of the innervated vasculature. The ultrasound unit may be an external unit or an internal unit. The ultrasound unit may be integrated at least in part at the distal end of the catheter, and the acoustic transducer may be integral or coupled to the ultrasound unit.

In other embodiments, an apparatus for facilitating delivery of acoustic energy to innervated vasculature includes a catheter configured for intravascular deployment and an ultrasound unit coupled to the catheter. An acoustic transducer is provided at a distal end of the catheter and coupled to the ultrasound unit. The acoustic transducer is configured for high intensity focused ultrasound operation in at least a cavitation ablation mode that forms bubbles within target tissue of the innervated vasculature and work to mechanically disrupt nerve fibers and ganglia included within the target tissue upon implosion or explosion.

In accordance with some embodiments, an apparatus for facilitating delivery of acoustic energy to innervated vasculature includes an imaging device configured for scanning the innervated vasculature and locating target tissue of the innervated vasculature. A catheter is configured for intravascular deployment and is coupled to an ultrasound unit. An acoustic transducer is provided at a distal end of the catheter and coupled to the ultrasound unit. The acoustic transducer is configured to deliver acoustic energy to the target tissue sufficient to ablate the target tissue located by the imaging device.

In further embodiments, an apparatus for facilitating delivery of acoustic energy to innervated vasculature includes a catheter configured for intravascular deployment and comprises an ultrasound unit coupled to the catheter. The apparatus includes an acoustic transducer provided at a distal end of the catheter and coupled to the ultrasound unit. The acoustic transducer is configured to deliver acoustic energy to target tissue of the innervated vasculature sufficient to ablate the target tissue. A balloon arrangement is configured to encompass at least the acoustic transducer. The balloon arrangement comprises a balloon that inflates under a very low pressure of about 1 to 2 pounds per square inch (PSI) or less above an ambient pressure that is adjacent to and outside the balloon.

According to other embodiments, an apparatus for facilitating delivery of acoustic energy to innervated vasculature includes a cryoballoon arrangement dimensioned for intravascular deployment and configured to freeze target tissue of the innervated vasculature. A catheter is configured for intravascular deployment and comprises an acoustic transducer at a distal end of the catheter. The acoustic transducer is coupled to an ultrasound unit. The acoustic transducer is configured to deliver acoustic energy to the frozen target tissue sufficient to destroy nerve cells of the target tissue.

In accordance with other embodiments, an apparatus for facilitating delivery of acoustic energy to innervated vasculature includes a cryoballoon arrangement dimensioned for intravascular deployment and configured to provide cooling for the innervated vasculature, such as the renal artery. A catheter is configured for intravascular deployment and comprises an acoustic transducer at a distal end of the catheter. The acoustic transducer is coupled to an ultrasound unit. The acoustic transducer is configured to deliver acoustic energy to the target tissue sufficient to destroy nerve cells of the target tissue.

In other embodiments, an apparatus of the invention facilitates delivery of acoustic energy to innervated vasculature that includes a ganglion that contributes to renal sympathetic nerve activity. The apparatus includes a catheter configured for intravascular deployment and is coupled to an ultrasound unit. The apparatus includes an acoustic focusing arrangement and an acoustic transducer provided at a distal end of the catheter, the acoustic transducer positioned relative to the focusing arrangement. The acoustic transducer and focusing arrangement are configured to deliver acoustic energy to a target ganglion of the innervated vasculature sufficient to destroy nerve cells included within the target ganglion.

In accordance with other embodiments, an apparatus for facilitating delivery of acoustic energy to innervated vasculature includes an imaging device configured for scanning the innervated vasculature and locating target tissue of the innervated vasculature. The apparatus includes a lithotripsy device configured to deliver high-energy acoustic shockwaves to the target tissue sufficient to denervate the target tissue located by the imaging device. A cryotherapy arrangement may be included, which is dimensioned for intravascular deployment and configured to freeze the target tissue. Nerve tissue, if damaged, has the potential to regenerate, especially if the nerve containing sheath has not been disrupted. New nerve growth occurs typically through the existing nerve sheath. If the nerve sheaths are disrupted or cut, nerve regeneration to the end organ is more difficult. An apparatus that combines both a freezing action followed by a mechanical acoustic wave action has the advantage of disrupting the nerve sheaths and preventing nerve regeneration to the targeted organ.

In further embodiments, an apparatus for facilitating delivery of an ablation agent to innervated vasculature includes an imaging device configured for scanning the innervated vasculature and locating a target ganglion of the renal artery or the abdominal aorta that contributes to renal sympathetic nerve activity. A delivery catheter is dimensioned for intravascular deployment in a vessel proximate the renal artery or the abdominal aorta. The delivery catheter includes a tissue penetrating feature configured to penetrate a wall of the vessel to create an access hole and to penetrate the target ganglion. A steering mechanism is configured for steering the delivery catheter through the access hole and to an extravascular location adjacent the target ganglion. A dispensing arrangement is configured to facilitate dispensing of an ablation agent from the delivery catheter into the target ganglion, whereby the ablation agent kills nerve cells of the target ganglion sufficient to terminate renal sympathetic nerve activity. The dispensing arrangement may be configured to facilitate dispensing of a neurotoxin, a venom, a cryogenic agent, a radioactive material, or radioactive seeds.

The above summary of the present invention is not intended to describe each embodiment or every implementation of the present invention. Advantages and attainments, together with a more complete understanding of the invention, will become apparent and appreciated by referring to the

following detailed description and claims taken in conjunction with the accompanying drawings.

DESCRIPTION OF THE DRAWINGS

FIG. 1 is an illustration of a right kidney and renal vasculature including a renal artery branching laterally from the abdominal aorta;

FIGS. 2A and 2B illustrate sympathetic innervation of the renal artery;

FIG. 3A illustrates various tissue layers of the wall of the renal artery;

FIGS. 3B and 3C illustrate a portion of a renal nerve;

FIG. 4 illustrates an ultrasound unit deployed in a renal artery and an optional external imaging system or device in accordance with embodiments of the invention;

FIG. 5 illustrates an ultrasound unit deployed in a renal artery which incorporates one or both of imaging and ultrasonic denervation therapy delivery capabilities in accordance with embodiments of the invention;

FIG. 6 illustrates an ultrasound unit deployed in a renal artery using a stabilization arrangement in accordance with embodiments of the invention;

FIG. 7 shows different possible beam profiles of acoustic energy emitted by an ultrasound unit deployed in a renal artery in accordance with embodiments of the invention;

FIGS. 8-10 illustrate an ultrasound unit and a balloon arrangement deployed in a renal artery in accordance with embodiments of the invention;

FIG. 11 illustrates a lithotripsy machine which is preferably operated in cooperation with a cryoballoon arrangement deployed in a renal artery in accordance with embodiments of the invention;

FIGS. 12A and 12B illustrate ultrasound units having single and distributed ultrasonic elements in accordance with embodiments of the invention;

FIGS. 12C and 12D illustrate ultrasound units that include one or more acoustic phased array transducers in accordance with embodiments of the invention;

FIGS. 13A and 13B are sectional views of ultrasound units that include one or more acoustic phased array transducers in accordance with embodiments of the invention;

FIGS. 14 and 15 illustrate ultrasound units that include one or more acoustic transducers of varying configuration in accordance with embodiments of the invention;

FIG. 16 is an exaggerated sectional view of a renal artery and an acoustic energy beam emitted from a focusing arrangement of an ultrasound unit positioned within a lumen of the renal artery in accordance with embodiments of the invention;

FIG. 17 shows an ultrasound delivery apparatus which includes an ultrasonic source, focusing arrangement, detector, imaging electronics, and computer system for processing and displaying ultrasonic imaging data in accordance with embodiments of the invention;

FIGS. 18A and 18B illustrate representative deployment configurations of a focused ultrasound catheter that can be operated for one or both of transvascular scanning and denervation of innervated vasculature in accordance with embodiments of the invention;

FIG. 19 illustrates an apparatus for facilitating guided delivery of an ablation agent to ganglia that contribute to renal sympathetic nerve activity in accordance with embodiments of the invention; and

FIG. 20 shows a hinge mechanism that can be built into a catheter or other elongated member to enhance access to the renal artery and other vasculature in accordance with embodiments of the invention.

While the invention is amenable to various modifications and alternative forms, specifics thereof have been shown by way of example in the drawings and will be described in detail. It is to be understood, however, that the intention is not to limit the invention to the particular embodiments described. On the contrary, the intention is to cover all modifications, equivalents, and alternatives falling within the scope of the invention as defined by the appended claims.

DETAILED DESCRIPTION

In the following description, references are made to the accompanying drawings which illustrate various embodiments of the invention. It is to be understood that other embodiments may be utilized, and structural and functional changes may be made to these embodiments without departing from the scope of the present invention.

Embodiments of the invention are directed to systems, devices, and procedures for delivering ultrasonic denervation therapy to innervated renal vasculature. Embodiments of the invention are directed to systems, devices, and procedures for denervating renal vasculature using ultrasonic denervation therapy to disrupt target tissue so that renal sympathetic nerve activity is permanently terminated. Embodiments of the invention are directed to systems, devices, and procedures for scanning or imaging innervated renal vasculature to locate target tissue for denervation and to evaluate the efficacy of ultrasonic denervation therapy delivered to the target tissue. Other approaches may be used to evaluate the effectiveness of an ultrasonic denervation treatment, such as an electrode arrangement (e.g., electrode array) arranged at spaced-apart locations relative to innervated target tissue, which can sense nerve activity along nerve fibers (and at ganglia) of the innervated target tissue.

The disclosed embodiments are generally directed to imaging and/or denervating innervated renal vascular tissue that contributes to renal function, particularly renal sympathetic nerve activity. Target innervated vasculature of the renal artery, for example, preferably includes renal nerves, renal ganglia, aortal ganglia and other nerves and ganglia that contribute to renal sympathetic nerve activity. Although preferred embodiments of the invention provide for complete and permanent termination of renal sympathetic nerve activity, various embodiments may be implemented to provide for temporary (e.g., weeks or months) cessation of renal sympathetic nerve activity.

Representative embodiments of the invention described herein are generally directed to ultrasonic imaging and denervation apparatuses and therapies involving continuous or pulsed ultrasound at frequencies well above the human audible range of hearing, which corresponds to sound in the range of about 20 hertz to 20 kHz. The term "ultrasound" is intended to apply to all acoustic energy (e.g., longitudinal or transverse, mechanical waves) with a frequency greater than 20 kHz. Ultrasonic apparatuses according to embodiments of the invention typically operate at frequencies between about 1 MHz to about 80 MHz, with many apparatuses operating at frequencies between about 2 MHz to about 5 MHz. Intravascular and intracardiac ultrasonic imaging devices generally operate in the frequency range between about 5 MHz and 60 MHz.

According to various embodiments, ultrasonic apparatuses and procedures of the invention are directed to imaging renal

tissue and/or positioning an ultrasonic denervation device within the renal artery or vein, for example. Various embodiments include an intravascular (e.g., endovascular, intra-to-extra vascular, or transvascular) ultrasonic denervation device configured to provide both imaging of, and denervation therapy to, target tissue of innervated renal vasculature.

Other embodiments include an intravascular ultrasonic denervation device configured to provide denervation therapy to target tissue of innervated renal vasculature, with imaging provided by a separate device, which may be an endovascular, intra-to-extravascular, transvascular, extravascular, or extra-corporeal imaging device or system.

In general, suitable scanning, imaging and/or locating apparatuses provide target depth, range, and or volume data that are used by the system computer to facilitate locating of target tissue and adjustment of various device or system parameters, such as power parameters (e.g., amplitude, frequency, continuous mode, pulse mode, etc.), focus parameters (e.g., focal length, beam spread and/or divergence, phased array pulse duration and sequencing, etc.), and operating mode (e.g., scan, denervate, and concurrent scan+denervate modes), among others.

Data associated with imaging and denervation procedures may be communicated to an external system which produces imaging data and visual information useful for positioning the ultrasonic denervation device and evaluating the efficacy of an ultrasonic denervation procedure. The external system, for example, may include a computer which includes a display. Data and visual information concerning the scanning and ultrasonic denervation therapy procedures are preferably presented on the display. The computer may include an interface for communicating with other systems and devices, including a network or server.

Various embodiments of the invention are directed to apparatuses that deliver focused acoustic energy to target tissue that causes an increase in the temperature of the target tissue to a level that disrupts nerve structures of the target tissue and prevents chronic recovery of nerve fibers/ganglion in the target tissue resulting from the burn injury. Other embodiments are directed to apparatuses that deliver focused energy to target tissue that causes mechanical disruption of target tissue and prevents chronic recovery of nerve fibers/ganglion in the target tissue resulting from the mechanical disruption (e.g., cavitation microbubbles). Preferred ultrasound apparatuses include those that achieve a desired level of disruption of target tissue while leaving adjacent or intervening tissue uninjured or negligibly injured (e.g., subject to healing without permanent adverse effects).

The frequency of acoustic energy generated by ultrasonic apparatuses of the invention is preferably selected so that acoustic energy is absorbed substantially in the wall of the renal artery, preferably the outer wall region. In some embodiments, the ultrasonic apparatus is configured to emit acoustic energy of sufficient power to raise the temperature of targeted renal artery wall tissue to above 50° C. to kill the target artery tissue and nerve/ganglion within it. In other embodiments, the ultrasonic apparatus is configured to emit acoustic energy of sufficient power to raise the temperature of targeted renal artery wall tissue to above 65° C. to reform the collagen in target artery wall tissue and mechanically change the tissue property. In further embodiments, the ultrasonic apparatus is configured to emit acoustic energy of sufficient power to raise the temperature of targeted renal artery wall tissue to between 65° C. and 100° C. to render the fat from the target tissue, and totally disrupt the target tissue and prevent chronic recovery of the nerve fibers/ganglion from the burn injury.

Embodiments of the invention are directed to an intravascular device that includes a focused ultrasonic transducer, such as a High Intensity Focused Ultrasound (HIFU) device. HIFU is a highly accurate medical technology that uses high-intensity focused ultrasound to heat and destroy target tissue rapidly. A HIFU approach can focus acoustic energy to generate heat deep within target tissue at a substantial distance from the ultrasonic transducer. An important difference between HIFU and other forms of focused energy, such as RF or radiation therapy, is that the passage of ultrasound energy through intervening tissue has no apparent cumulative effect on the intervening tissue.

According to various embodiments, a HIFU transducer is incorporated or otherwise supported by a catheter dimensioned for deployment in the renal artery, renal vein, abdominal aorta, or other vessel near the kidneys. The HIFU transducer generates ultrasound beams that can be focused on target tissue located near to, or relatively distant from, the transducer. For example, embodiments of an intravascular HIFU transducer of the present invention may be used to inject acoustic energy into target tissue located about 0.5 mm to about 90 mm away from the HIFU transducer.

In short range applications, such as renal artery denervation conducted from within the renal artery, an intravascular HIFU device may be used to inject acoustic energy into target tissue of the renal artery located about 1 mm to about 4 mm away from the HIFU transducer. In long range applications, such as renal artery denervation conducted from within the renal vein or abdominal aorta, an intravascular HIFU device may be used to inject acoustic energy into target tissue of the renal artery located about 5 mm to about 80 mm away from the HIFU transducer.

Using a HIFU transducer of the present invention, one or more focal zones at or within a location, region, or volume within target tissue can be subjected to high intensity ultrasound energy, while tissue surrounding the target tissue is subjected to much lower intensity ultrasound energy. In this manner, target tissue can be heated to a sufficiently high temperature so as to cause a desired thermal effect (e.g., ablation, coagulation, denaturation, necrosis) while tissue surrounding the target area is not subject to damaging temperatures. Due to the significant energy deposition at the focal zone, the temperature within the target tissue rises to 65° to 85° C., destroying the target tissue, which includes nerves and/or ganglia, by coagulative necrosis.

Each sonication of the ultrasonic beams emitted by the HIFU transducer treats a precisely defined portion of the target tissue. HIFU denervation may be accomplished manually, automatically, or semi-automatically. For example, renal artery denervation may be accomplished by moving an intravascular HIFU transducer arrangement within the renal artery by robotic control of the catheter to which the HIFU transducer is connected. By way of further example, renal artery denervation may be accomplished by moving (translating and/or rotating) an intravascular HIFU transducer arrangement relative to a catheter to which the HIFU transducer is connected via electronic motor control.

Ultrasonic denervation therapy using acoustic energy involves the conversion of acoustic energy into heat when acoustic energy is absorbed by target tissue. Illumination of target tissue that includes nerves and ganglia with acoustic energy, for example, leads to thermal damage of the target tissue. The diffusion of heat energy into the surrounding tissue, however, can thermally damage tissue outside the target area or volume of tissue. A cooling apparatus is preferably used to minimize thermal trauma to the surrounding tissue. Various cooling apparatuses are contemplated herein for this

purpose, including cryoballoons, cryocatheters, irrigation arrangements, cooling lumens, Peltier cooling apparatuses, and blood diversion apparatuses, among others.

In embodiments that utilize focused ultrasound, such as HIFU, local cooling apparatuses may not be required or desired, because focused acoustic energy can be projected to target tissue spaced apart from the ultrasonic transducer (e.g., by 1-90 mm) without heating tissue surrounding the target tissue.

Turning now to the figures, FIG. 1 is an illustration of a right kidney 10 and renal vasculature including a renal artery 12 branching laterally from the abdominal aorta 20. In FIG. 1, only the right kidney 10 is shown for purposes of simplicity of explanation, but reference will be made herein to both right and left kidneys and associated renal vasculature and nervous system structures, all of which are contemplated within the context of embodiments of the present invention. The renal artery 12 is purposefully shown to be disproportionately larger than the right kidney 10 and abdominal aorta 20 in order to facilitate discussion of various features and embodiments of the present disclosure.

The right and left kidneys are supplied with blood from the right and left renal arteries that branch from respective right and left lateral surfaces of the abdominal aorta 20. Each of the right and left renal arteries is directed across the crus of the diaphragm, so as to form nearly a right angle with the abdominal aorta 20. The right and left renal arteries extend generally from the abdominal aorta 20 to respective renal sinuses proximate the hilum 17 of the kidneys, and branch into segmental arteries and then interlobular arteries within the kidney 10. The interlobular arteries radiate outward, penetrating the renal capsule and extending through the renal columns between the renal pyramids. Typically, the kidneys receive about 20% of total cardiac output which, for normal persons, represents about 1200 mL of blood flow through the kidneys per minute.

The primary function of the kidneys is to maintain water and electrolyte balance for the body by controlling the production and concentration of urine. In producing urine, the kidneys excrete wastes such as urea and ammonium. The kidneys also control reabsorption of glucose and amino acids, and are important in the production of hormones including vitamin D, renin and erythropoietin.

An important secondary function of the kidneys is to control metabolic homeostasis of the body. Controlling hemostatic functions include regulating electrolytes, acid-base balance, and blood pressure. For example, the kidneys are responsible for regulating blood volume and pressure by adjusting volume of water lost in the urine and releasing erythropoietin and renin, for example. The kidneys also regulate plasma ion concentrations (e.g., sodium, potassium, chloride ions, and calcium ion levels) by controlling the quantities lost in the urine and the synthesis of calcitriol. Other hemostatic functions controlled by the kidneys include stabilizing blood pH by controlling loss of hydrogen and bicarbonate ions in the urine, conserving valuable nutrients by preventing their excretion, and assisting the liver with detoxification.

Also shown in FIG. 1 is the right suprarenal gland 11, commonly referred to as the right adrenal gland. The suprarenal gland 11 is a star-shaped endocrine gland that rests on top of the kidney 10. The primary function of the suprarenal glands (left and right) is to regulate the stress response of the body through the synthesis of corticosteroids and catecholamines, including cortisol and adrenaline (epinephrine), respectively. Encompassing the kidneys 10, suprarenal glands 11, renal vessels 12, and adjacent perirenal fat is the

renal fascia, e.g., Gerota's fascia, (not shown), which is a fascial pouch derived from extraperitoneal connective tissue.

The autonomic nervous system of the body controls involuntary actions of the smooth muscles in blood vessels, the digestive system, heart, and glands. The autonomic nervous system is divided into the sympathetic nervous system and the parasympathetic nervous system. In general terms, the parasympathetic nervous system prepares the body for rest by lowering heart rate, lowering blood pressure, and stimulating digestion. The sympathetic nervous system effectuates the body's fight-or-flight response by increasing heart rate, increasing blood pressure, and increasing metabolism.

In the autonomic nervous system, fibers originating from the central nervous system and extending to the various ganglia are referred to as preganglionic fibers, while those extending from the ganglia to the effector organ are referred to as postganglionic fibers. Activation of the sympathetic nervous system is effected through the release of adrenaline (epinephrine) and to a lesser extent norepinephrine from the suprarenal glands 11. This release of adrenaline is triggered by the neurotransmitter acetylcholine released from preganglionic sympathetic nerves.

The kidneys and ureters (not shown) are innervated by the renal nerves 14. FIGS. 1 and 2A-2B illustrate sympathetic innervation of the renal vasculature, primarily innervation of the renal artery 12 and distal structures such as the kidney 10. The primary functions of sympathetic innervation of the renal vasculature include regulation of renal blood flow, stimulation of renin release, and direct stimulation of water and sodium ion reabsorption.

Most of the nerves innervating the renal vasculature are sympathetic postganglionic fibers arising from the superior mesenteric ganglion 26. The renal nerves 14 extend generally axially along the renal arteries 12, enter the kidneys 10 at the hilum 17, follow the branches of the renal arteries 12 within the kidney 10, and extend to individual nephrons. Other renal ganglia, such as the renal ganglia 24, superior mesenteric ganglion 26, the left and right aorticorenal ganglia 22, and celiac ganglia 28 also innervate the renal vasculature. The celiac ganglion 28 is joined by the greater thoracic splanchnic nerve (greater TSN). The aorticorenal ganglion 26 is joined by the lesser thoracic splanchnic nerve (lesser TSN) and innervates the greater part of the renal plexus.

Sympathetic signals to the kidney 10 are communicated via innervated renal vasculature that originates primarily at spinal segments T10-T12 and L1. Parasympathetic signals originate primarily at spinal segments S2-S4 and from the medulla oblongata of the lower brain. Sympathetic nerve traffic travels through the sympathetic trunk ganglia, where some may synapse, while others synapse at the aorticorenal ganglion 22 (via the lesser thoracic splanchnic nerve, i.e., lesser TSN) and the renal ganglion 24 (via the least thoracic splanchnic nerve, i.e., least TSN). The postsynaptic sympathetic signals then travel along nerves 14 of the renal artery 12 to the kidney 10. Presynaptic parasympathetic signals travel to sites near the kidney 10 before they synapse on or near the kidney 10.

With particular reference to FIG. 2A, the renal artery 12, as with most arteries and arterioles, is lined with smooth muscle 34 that controls the diameter of the renal artery lumen 13. Smooth muscle, in general, is an involuntary non-striated muscle found within the media layer of large and small arteries and veins, as well as various organs. The glomeruli of the kidneys, for example, contain a smooth muscle-like cell called the mesangial cell. Smooth muscle is fundamentally

different from skeletal muscle and cardiac muscle in terms of structure, function, excitation-contraction coupling, and mechanism of contraction.

Smooth muscle cells can be stimulated to contract or relax by the autonomic nervous system, but can also react on stimuli from neighboring cells and in response to hormones and blood borne electrolytes and agents (e.g., vasodilators or vasoconstrictors). Specialized smooth muscle cells within the afferent arteriole of the juxtaglomerular apparatus of kidney 10, for example, produces renin which activates the angiotension II system.

The renal nerves 14 innervate the smooth muscle 34 of the renal artery wall 15 and extend lengthwise in a generally axial or longitudinal manner along the renal artery wall 15. The smooth muscle 34 surrounds the renal artery circumferentially, and extends lengthwise in a direction generally transverse to the longitudinal orientation of the renal nerves 14, as is depicted in FIG. 2B.

The smooth muscle 34 of the renal artery 12 is under involuntary control of the autonomic nervous system. An increase in sympathetic activity, for example, tends to contract the smooth muscle 34, which reduces the diameter of the renal artery lumen 13 and decreases blood perfusion. A decrease in sympathetic activity tends to cause the smooth muscle 34 to relax, resulting in vessel dilation and an increase in the renal artery lumen diameter and blood perfusion. Dilation and contraction of the distal bed of renal arterioles fed by the renal artery is similarly controlled by distal branches of the renal autonomic nerves, and these "resistance vessels" are most important in determining the total blood flow through the renal artery. Conversely, increased parasympathetic activity tends to relax the smooth muscle 34, while decreased parasympathetic activity tends to cause smooth muscle contraction.

FIG. 3A shows a segment of a longitudinal cross-section through a renal artery, and illustrates various tissue layers of the wall 15 of the renal artery 12. The innermost layer of the renal artery 12 is the endothelium 30, which is the innermost layer of the intima 32 and is supported by an internal elastic membrane. The endothelium 30 is a single layer of cells that contacts the blood flowing through the vessel lumen 13. Endothelium cells are typically polygonal, oval, or fusiform, and have very distinct round or oval nuclei. Cells of the endothelium 30 are involved in several vascular functions, including control of blood pressure by way of vasoconstriction and vasodilation, blood clotting, and acting as a barrier layer between contents within the lumen 13 and surrounding tissue, such as the membrane of the intima 32 separating the intima 32 from the media 34, and the adventitia 36. The membrane or maceration of the intima 32 is a fine, transparent, colorless structure which is highly elastic, and commonly has a longitudinal corrugated pattern.

Adjacent the intima 32 is the media 33, which is the middle layer of the renal artery 12. The media is made up of smooth muscle 34 and elastic tissue. The media 33 can be readily identified by its color and by the transverse arrangement of its fibers. More particularly, the media 33 consists principally of bundles of smooth muscle fibers 34 arranged in a thin plate-like manner or lamellae and disposed circularly around the arterial wall 15. The outermost layer of the renal artery wall 15 is the adventitia 36, which is made up of connective tissue. The adventitia 36 includes fibroblast cells 38 that play an important role in wound healing.

A renal nerve 14 is shown proximate the adventitia 36 and extending longitudinally along the renal artery 12. The main trunk of the renal nerves 14 generally lies at or adjacent the adventitia of the renal artery 12, with certain branches cours-

ing into the media to enervate the renal artery smooth muscle. For example, renal nerves may be situated in the adventitia proximate the outer wall of the renal artery (e.g., tunica adventitia) or within the vasa vasorum, such as the vasa vasorum externae.

FIGS. 4-6 illustrate ultrasound arrangements for treating innervated renal and/or aortic tissue that contribute to renal sympathetic nerve activity in accordance with embodiments of the invention. FIGS. 4-6 show an exaggerated sectional view of a portion of a patient's renal artery 12. The tissue layers of the renal artery 12 include the intima 32, which comprises the endothelium, the media 33, which includes smooth muscle, and the adventitia 36. A renal nerve 14 and a ganglion (e.g., renal ganglion 24 or aorticorenal ganglion 22) are shown on or proximate an outer section of the adventitia 36 for illustrative purposes.

In various embodiments according to FIGS. 4-6, an ultrasound unit 50 comprises an ultrasound delivery apparatus capable of transmitting acoustic energy into innervated renal vasculature that disrupts target tissue which includes one or both of renal nerves 14 and ganglia 24/22. Acoustic energy transmitted by an emitter 52 of the ultrasound unit 50 is preferably sufficient to disrupt the target tissue so that renal sympathetic nerve activity is permanently terminated.

It is understood that in the embodiments shown in FIGS. 4-6 and in other figures, the ultrasound unit 50 may comprise components that are entirely or partially implantable, and may comprise components that are entirely or partially external of the patient. For example, the ultrasound unit 50 may comprise an implantable transducer and an external ultrasound source. By way of further example, the ultrasound unit 50 may comprise an implantable transducer and an implantable ultrasound source. An implantable ultrasound source may be powered by an implantable or external power source. In another example, the ultrasound unit 50 may be integrated at least in part at the distal end of the catheter, and the acoustic transducer may be integral or coupled to the ultrasound unit. Other configurations are contemplated herein.

In other embodiments, an ultrasound unit 50 comprises an ultrasound delivery apparatus capable of transmitting acoustic energy into innervated renal vasculature that facilitates locating of renal nerves 14 and ganglia 24/22 but insufficient to significantly disrupt renal sympathetic nerve activity (e.g., insufficient to effect appreciable or permanent cessation of renal sympathetic nerve activity). In such embodiments, the ultrasound unit 50 may be used in combination with a detector to facilitate imaging and locating of target structures within or near renal artery and aortic tissue.

In further embodiments, an ultrasound unit 50 comprises an ultrasound delivery apparatus capable of transmitting acoustic energy into innervated renal vasculature that facilitates locating of renal nerves 14 and ganglia 24/22 within target tissue and transmitting acoustic energy into the target tissue that significantly disrupts renal sympathetic nerve activity, such as by permanently terminating renal sympathetic nerve activity. In other embodiments, a separate internal or external imaging device may be used to facilitate locating of renal nerves 14 and ganglia 24/22 within target tissue, and an intravascular ultrasound unit 50 is configured to transmit acoustic energy into the target tissue sufficient to significantly or permanently disrupt renal sympathetic nerve activity.

According to the embodiments shown in FIGS. 4-6, an ultrasound unit 50 includes an ultrasonic emitter 52 disposed in a housing to which a distal end of a catheter 51 is connected. The emitter 52 is coupled to an ultrasonic source 54. The emitter 52 typically includes, or is adjacent to, an

arrangement that facilitates focusing of acoustic energy received from the ultrasonic source **54** and directs acoustic energy to target renal tissue. In some embodiments, as shown in FIG. **4**, the ultrasound unit **50** includes an ultrasonic emitter **52** and a separate imaging system **53** or device for imaging renal tissue and guiding acoustic energy emitted by the ultrasound unit **50** to the target renal tissue. The imaging system or device **53** may be used to assist in delivering and positioning the ultrasound unit **50** to and within the renal artery **12**.

The imaging system or device **53** may be external to the patient (i.e., outside the skin **47**) or at least partially implantable, such as an endovascular imaging device (e.g., IVUS or intravascular ultrasound device). Suitable intravascular, transvascular, extravascular, and extracorporeal apparatuses include various MRI, laser, and ultrasound apparatuses, for example.

In other embodiments, as shown in FIG. **5**, the ultrasound unit **50** includes an ultrasonic emitter **52** and a detector **57** or other local imaging device for imaging renal tissue and directing acoustic energy to target tissue of the renal vasculature. The ultrasonic emitter **52** and detector **57** may be used to assist in delivering and positioning the ultrasound unit **50** to and within the renal artery **12**. For example, the detector **57** may comprise an ultrasound detector that receives acoustic energy (e.g., echoes) reflected from the target tissue.

In various embodiments, a single transducer operates as the emitter **52** and the detector **57**. In other embodiments, one transducer operates as the emitter **52** and another transducer operates as the detector **57**. In further embodiments, the transducer that is configured to deliver denervation therapy is also operative as a scanning transducer. In some embodiments, separate denervation and scanning transducers are employed. It is understood that the emitter and/or receiver components shown in the figures may define single transducer elements or an array of transducer elements.

In some embodiments, for example, the ultrasound unit **50** is configured to selectively operate in a scan mode and a denervation mode, allowing the ultrasound unit **50** to locate target tissue in the scan mode and then permanently disrupt renal nerve fibers and ganglia within the target tissue in the denervation mode. Details of components and functionality that can be adapted for use in or by the ultrasound unit **50** are described in greater detail hereinbelow and disclosed in U.S. Pat. Nos. 5,344,395 and 5,601,526, which are incorporated herein by reference.

FIG. **6** shows another embodiment of an ultrasound arrangement for denervating renal vasculature that contributes to renal sympathetic nerve activity in accordance with the invention. A support or stabilizing arrangement **55** is provided to aid in maintaining the ultrasound unit **50** at a relatively constant distance from the artery wall as the ultrasound unit **50** is translated and/or rotated within the lumen of the renal artery **12**.

In various configurations, it is desirable to stabilize the position of the ultrasound unit **50** within the renal artery **12** so that the intensity of the acoustic energy emitted by the ultrasound unit **50** does not vary significantly with location, which could otherwise result in over-treated and under-treated regions. One approach to keeping the ultrasound unit **50** at a constant distance from the wall of the renal artery is to incorporate the ultrasound unit **50** into a balloon which can be expanded until it fills the arterial lumen, embodiments of which are discussed below with reference to FIGS. **8-11**. Other stabilizing arrangements **55** are contemplated, such as a stent or an expandable cage or basket arrangement.

In FIGS. **4-6**, the emitter **52** may be coupled to an external ultrasonic source **54b** via a coupling **56**. The external ultra-

sonic source **54b** is situated external to the renal artery, such as at a location outside the body. The coupling **56** is typically an electrical coupling disposed within a catheter, which enters the renal vasculature at a suitable access vessel location (e.g., superior or inferior abdominal aorta or inferior vena cava). In other embodiments, the ultrasonic source **54a** can be disposed within the housing of the ultrasound unit **50** and may draw power from a power source internal to the ultrasound unit **50** (battery, capacitor, energy harvesting device) or from a patient-external power source. The ultrasonic source **54a** may also be housed in a separate unit inside the body (e.g., a subcutaneous pocket or within the abdominal cavity, among other locations) and draw power from an internal power source or an external power source (e.g., via electromagnetic induction using an RF source external of the patient).

Locating target tissue may involve locating renal or aortic ganglia and/or artery tissue which includes renal nerves **14**, such as the adventitia proximate the outer wall of the renal artery or the vasa vasorum externae. For example, one or more locating components of the ultrasound unit **50** may be used to scan the renal artery **12** or adjacent tissue that includes renal nerves and/or renal/aortic ganglia. The ultrasound unit **50** (or other locating apparatus, internal or external) may be controlled to scan for target tissue in deep layers of the adventitia and/or the vasa vasorum, such as the vasa vasorum externae which penetrates the outer adventitia (tunica adventitia). Once located, the target tissue may be treated using the ultrasound unit **50**.

According to various embodiments that employ an external imager **53**, such as that shown in FIG. **4**, an MRI system may be used to locate target tissue (e.g., renal nerves and ganglia of the renal artery, vasa vasorum, and abdominal aorta), determine the depth, length, and/or width of the target tissue (e.g., for 1-D, 2-D, or 3-D imaging), and guide acoustic energy emitted by the ultrasound unit **50** to the target tissue. The MRI system may be used to identify renal nerves and ganglia of the renal artery, vasa vasorum, and abdominal aorta, before they are destroyed by the ultrasonic emitter **52**. In accordance with embodiments that use high intensity focused ultrasound, Magnetic Resonance-guided Focused Ultrasound (MRg-FUS) apparatuses and techniques may be used to treat innervated target tissue.

An MRI system of the invention may be used to accurately quantify the heating of target tissue produced by the ultrasonic emitter **52** during a renal denervation procedure. For example, the MRI system preferably identifies the ultrasound path and monitors heat rise in the target tissue. An MRI system of the invention preferably provides for high soft tissue contrast and imaging in any orientation, which enhances guiding of HIFU ablation energy to target innervated renal vasculature.

Heating, position, and other imaging information developed by the MRI system is preferably used to aid in controlling ultrasonic ablation of target tissue, particularly when using a HIFU implementation. This information may be used to provide automatic (e.g., robotic) or semi-automatic (e.g., partially robotic) control of a renal denervation procedure in real-time (or near real-time), via the MRI system computer and/or physician, respectively.

In various embodiments, a real-time interactive MRI (rt-MRI) system is used to provide for concurrent imaging of target innervated renal vasculature by the MRI system and ablation of the target vasculature by the ultrasound unit **50**. Embodiments of an interactive real-time MRI system include a highly parallel MRI device having upwards to 32 channels or more. For example, an MRI system of the invention may include 32-element phased arrays, which may be defined by

multiple synchronized scanner-receiver subsystems. Software of the MRI system coordinates the real-time acquisition, reconstruction, and display of 32-channel images across the multiple subsystems.

Real-time, large field-of-view (FOV) imaging can be achieved by using interleaved echo-planar and single-shot fast-spin-echo pulse sequences. In one approach, parallel image acquisition is augmented by independently offsetting the frequency of different array elements to variably shift their FOV. When augmented parallel imaging is combined with conventional parallel imaging techniques, a significant increase of image acceleration factors can be achieved. Increasing the number of coils can significantly increase the FOV in two dimensions during rapid imaging, with no or negligible degradation of imaging time or spatial resolution.

Interactive real-time MRI in combination with an ultrasound unit **50** can enhance procedural safety by identifying unexpected complications early in a denervation procedure. A real-time MRI system of the invention preferably provides high tissue contrast in any orientation, which facilitates accurate locating of target tissue of the renal artery, vasa vasorum, and abdominal aorta. For example, a multi-slice, real-time MRI system may be used to guide ultrasound unit emissions across vascular tissue boundaries with high precision.

In other embodiments, an ultrasonographic imaging system **53** is used to locate target tissue, determine the depth, length, and/or width of the target tissue (e.g., for 1-D, 2-D, or 3-D imaging), and guide acoustic energy emitted by the ultrasound unit **50** to the target tissue within the renal artery **12**, vasa vasorum, and abdominal aorta. In various embodiments that use high intensity focused ultrasound, Ultrasound-guided Focused Ultrasound (USgFUS) apparatuses and techniques may be used to treat innervated tissue of the renal artery. Suitable ultrasonographic systems include those configured with extracorporeal, intravascular, or transvascular imaging components.

In other embodiments, a combination of an ultrasonic device and a laser device is used to cooperatively provide imaging of, and denervation therapy to, innervated renal vasculature. According to some embodiments, one of the ultrasonic device and the laser device is used for imaging, while the other of the ultrasonic device and the laser device is used for renal denervation. The ultrasonic device or the laser device (or both, if desired) is capable of transmitting acoustic and/or optical energy into the renal artery wall sufficient to disrupt target tissue that includes renal nerves **14** and/or ganglia **24/22**. The acoustic and/or optical energy is preferably sufficient to disrupt the target tissue so that renal sympathetic nerve activity is permanently terminated. Combinations of ultrasonic and laser devices that can be used cooperatively to image and denervate renal vasculature include ultrasonic and laser device combinations disclosed in previously cited commonly owned U.S. Patent Publication No. 2011/0257641, filed as U.S. Provisional Patent Application Ser. No. 61/324,163 on Apr. 14, 2010 and entitled "Phototherapy for Renal Denervation."

In other embodiments, a combination of an ultrasonic device and a laser device is used to cooperatively provide imaging of, and denervation therapy to, innervated renal vasculature. According to some embodiments, one of the ultrasonic device and the laser device is used for imaging, while the other of the ultrasonic device and the laser device is used for renal denervation. The ultrasonic device or the laser device (or both, if desired) is capable of transmitting acoustic and/or optical energy into the renal artery wall sufficient to disrupt target tissue that includes renal nerves **14** and/or ganglia **24/22**. The acoustic and/or optical energy is preferably

sufficient to disrupt the target tissue so that renal sympathetic nerve activity is permanently terminated. Combinations of ultrasonic and laser devices that can be used cooperatively to image and denervate renal vasculature include ultrasonic and laser device combinations disclosed in previously cited commonly owned U.S. Patent Publication No. 2011/0257641, filed as U.S. Provisional Patent Application Ser. No. 61/324,163 on Apr. 14, 2010 and entitled "Phototherapy for Renal Denervation."

FIG. 7 illustrates an embodiment of an ultrasound arrangement for denervating renal vasculature that contributes to renal sympathetic nerve activity in accordance with the invention. According to this embodiment, an ultrasound unit **50** is shown deployed in a patient's renal artery **12** and equipped with an ultrasonic emitter **52** configured to deliver focused acoustic energy to target tissue **49** that includes renal nerves **14** and/or renal or aortic ganglia **24/22**. Various emitters **52a-52c** are shown for illustrative purposes that have different possible beam patterns **58**, including concave, convex, and linear beam patterns.

The ultrasound unit **50** may incorporate one or more of the same or disparate emitters **52a-52c** to achieve desired acoustic energy characteristics, including a desired acoustic beam pattern or geometry, beam spread, beam divergence, and/or focal length, among other characteristic. Various mechanical and electronic beam shaping or beamforming apparatuses and techniques may be used to achieve desired acoustic energy characteristics. Different acoustic energy characteristics may be required or desired depending on a number of factors, including the separation distance between the ultrasound unit **50** and the target tissue (e.g., short range vs. long range targets; intravascular vs. transvascular targets) and modes of ultrasound unit operation (e.g., scan vs. ablation modes), among others.

In various embodiments, the ultrasound unit **50** incorporates an acoustic transducer arrangement **52a** that emits acoustic energy in a generally conical-shaped beam **58a** that converges at a generally elliptical focal region **37** situated at a desired depth of focus, *l*. The ultrasonic unit **50** is positioned so that the focal region **37** is coincident with respect to target tissue that includes renal nerve fibers **14** and/or ganglion tissue **24/22**. After properly positioning the ultrasonic unit **50**, focused ultrasonic energy (e.g., HIFU) is transmitted to the focal region **37** at the desired depth, *l*, to destroy the renal nerve fibers **14** and/or ganglion tissue **24/22** within the focal region **37**. An acoustic transducer arrangement **52** of the ultrasonic unit **50** may have a fixed focal length, but preferably has a variable focal length.

To ensure protection of non-targeted renal artery and aortal tissue layers during HIFU or other form of ultrasonic renal denervation, various temperature control apparatuses may be used to enhance cooling at or proximate to the ultrasound unit **50**. In general, the maximum temperature of the inner wall of the renal artery may be kept below some target temperature, such as 50° C., by providing heat transfer sufficient to limit the temperature rise at the inner artery wall, while allowing for a temperature increase above the target temperature within the artery wall tissue sufficient to permanently disrupt the renal nerve fibers/ganglia.

FIG. 8 illustrates an embodiment of an ultrasound arrangement for denervating renal vasculature that contributes to renal sympathetic nerve activity in accordance with the invention. According to this embodiment, an ultrasound unit **50** is configured for deployment within a balloon **64**. The ultrasound unit **50** is shown disposed at a distal end of a catheter **51** and situated within the balloon **64** at a relatively central location. When expanded, the balloon **64** contacts the inner wall

of the renal artery and stabilizes the ultrasound unit **50** at a desired location and orientation within the balloon (e.g., central location oriented axially along the balloon's central axis).

The balloon **64** may be configured to allow blood flow within the renal artery to provide cooling of the artery wall during an ablation procedure. A perfusion balloon (e.g., fluted or channeled balloon) or a fluid diversion arrangement (e.g., longitudinal inlet/outlet ports or channels) may be used to allow perfusion of blood to cool the artery wall during ultrasonic ablation.

In other embodiments, the ultrasound unit **50** may be incorporated into a balloon **64** which can be expanded to the internal diameter of the renal artery, so that the balloon blocks or partially blocks the flow of blood. The balloon **64** can be filled with a liquid that provides good acoustic coupling between the ultrasound unit **50** and balloon wall, such as saline, D5W, or a suitable cryogenic liquid. The liquid used to fill the balloon **64** preferably allows acoustic energy emitted from the ultrasonic emitter **52** to efficiently propagate through the liquid medium and through the balloon before impinging on renal artery tissue. The liquid in the balloon **64** is preferably acoustically "transparent" to the frequencies of the acoustic energy emitted by the ultrasound unit **50**.

It is desirable that the liquid supplied to the balloon **64** not be toxic and should be soluble in blood to minimize possible embolic damage if the liquid should leak out of the balloon **64**. The liquid in the balloon **64** may be circulated with open or closed irrigation to keep the inner wall of the artery from being heated above 50° C. during an ultrasonic ablation procedure, while the internal tissue and nerve/ganglion of the renal artery is heated above 50° C., to disrupt the nerve function while avoiding stenosis of the renal artery wall due to the response to burn injury. The liquid may be a cooling liquid, such as a cryogenic liquid.

In the embodiment shown in FIG. 8, the balloon **64** includes an inlet manifold **61** and an outlet manifold **63** that facilitate pressurization, depressurization, and circulation of a cooling or cryogenic liquid within the balloon **64**. The balloon **64** may comprise a single or multiple balloon structure, with appropriate lumens provided in the catheter **51** or other catheter of the treatment apparatus. One or more temperature sensors (not shown) are provided at the balloon **64** to monitor temperature near or at the vessel wall.

An advantage of using a balloon **64** of the type shown in FIG. 8 is that the ultrasound unit **50** can be translated and rotated without contacting the renal artery wall. In some embodiments, the shaft **67** can incorporate a spiral rail that forces the ultrasound unit **50** (or at least the emitter **52**) to travel a helical path as it is advanced and retracted through the renal artery lumen. An illustrative example of such a configuration is shown in FIG. 9, which is described in detail hereinbelow. In other embodiments, the emitter **52** of the ultrasound unit **50** is oriented off-axis with respect to the longitudinal axis of the shaft **67**. For example, the emitter **52** may be oriented at an angle of about 45° to about 135° relative to the longitudinal axis of the shaft **67**, with about 90° representing a preferred orientation. An illustrative example of such a configuration is shown in FIG. 10, which is described in detail hereinbelow.

According to various embodiments, the balloon **64** or a balloon separate from the ultrasound unit **50** may be implemented to deliver cryogenic therapy to innervated renal vasculature in combination with ultrasonic ablation therapy. In some embodiments, a balloon arrangement separate from the ultrasonic device **50** is used so that a wider range of cryogenic fluids (liquids and gasses) can be used to achieve desired therapeutic temperatures. For embodiments that use a sepa-

rate cryoballoon arrangement, the cryogenic fluid that fills the balloon need not be an acoustic coupling fluid, since the ultrasound unit **50** is not situated within the cryoballoon. It is noted that the ultrasound unit **50** may be situated in a separate balloon (e.g., balloon **64**), and that the separate cryoballoon and balloon **64** within which the ultrasound unit **50** is situated may be supported by a common catheter or separate catheters.

Suitable cryoballoons include those that can cause renal tissue freezing and/or denervation at therapeutic temperatures ranging between approximately 0° C. and approximately -180° C. For example, embodiments of a cryoballoon may be implemented to cause renal tissue freezing and/or denervation with temperatures at the renal nerves ranging from approximately 0° C. to approximately -30° C. at the higher end, and to about -140° C. to -180° C. at the lower end. These therapeutic temperature ranges may vary based on the combined therapeutic effect of delivering cryogenic and ultrasonic denervation therapy energy to innervated target tissue of the renal artery and/or aorta. A variety of useful cryogenic fluids may be employed, including saline, a mixture of saline and ethanol, Freon or other fluorocarbons, nitrous oxide, liquid nitrogen, and liquid carbon dioxide, for example.

According to another embodiment, an ultrasound unit **50** of the type shown in FIG. 8 (with or without a balloon, such as balloon **64**) can include a lumen arrangement for transporting a thermal transfer fluid to provide local cooling (not freezing) of the intimal layer adjacent the ultrasound unit **50**. In this embodiment, the catheter shaft **61** may incorporate one or more cooling lumens that interact directly with the adjacent intimal layer to counteract the application of higher intensity energies targeted for renal nerves that are further away or deeper in the artery wall. In other embodiments, a separate cooling catheter arrangement may be employed to provide direct localized cooling to the renal artery wall.

The balloon **64** shown in FIG. 8 and in other figures is preferably a very low pressure balloon system. It is desirable to achieve minimal contact between the balloon **64** or other stabilizing arrangement and the inner wall of the renal artery in order to avoid injuring the sensitive endothelium of the artery. Very low pressure balloon systems can serve to provide minimal contact with the renal artery's inner wall and stabilization of the ultrasound unit **50**.

The balloon **64** or other stabilizing balloon can be constructed as a compliant balloon as is known in the art. For example, balloon **64** may comprise a compliant material configured to enable the balloon **64** to inflate under a very low pressure, such as about 1 to 2 pounds per square inch (PSI) or less (e.g., 0.5 PSI or less) above an ambient pressure that is adjacent to and outside the balloon **64**. The compliance of balloon **64** preferably results in little or negligible circumferential force applied to the vessel wall, while readily allowing the balloon to conform to irregularities in the shape of the tissue of the aortal/renal vasculature, which results in more efficient delivery of cooling or cryotherapy to tissues surrounding the target tissue (i.e., renal nerve fibers and renal ganglia).

All or a portion of the balloon **64** may be made of a highly compliant material that elastically expands upon pressurization. Because the balloon **64** elastically expands from a deflated state to an inflated state, the balloon **64** has an extremely low profile in the deflated state when compared to non-compliant or semi-compliant balloons. According to some embodiments, use of high compliance materials in the construction of the balloon **64**, in combination with a hinge mechanism **56** built into the catheter **51** (see, e.g., hinge **356** shown in FIG. 20), provides for enhanced efficacy and safety

when attempting to navigate a catheter **51** supporting an ultrasound unit **50** and one or more balloons through a nearly 90 degree turn from the abdominal aorta **20** into the ostium of the renal artery **12**.

Suitable materials for constructing all or a portion of the balloon **64** or other balloon include thermoplastic or thermoplastic elastomers, rubber type materials such as polyurethanes, natural rubber, or synthetic rubbers. The resulting balloon may be crosslinked or non-crosslinked. Other suitable materials for constructing all or a portion of the balloon **64** include silicone, urethane polymer, low durometer PEBAX, or an extruded thermoplastic polyisoprene rubber such as a low durometer hydrogenated polyisoprene rubber. These and other suitable materials may be used individually or in combination to construct the balloon **64**. Details of various materials suitable and configurations for constructing a balloon **64**, a stabilizing balloon or other balloon arrangement according to various embodiments are disclosed in commonly owned U.S. Pat. No. 7,198,632, U.S. application Ser. Nos. 12/980,952, and 12/980,972, which are incorporated herein by reference.

Embodiments of the invention may incorporate selected balloon, catheter, lumen, control, and other features of the devices disclosed in the following commonly owned U.S. patents and published patent applications: U.S. Patent Publication Nos. 2009/0299356, 2009/0299355, 2009/0287202, 2009/0281533, 2009/0209951, 2009/0209949, 2009/0171333, 2008/0312644, 2008/0208182, and 2008/0058791, and U.S. Pat. Nos. 5,868,735, 6,290,696, 6,648,878, 6,666,858, 6,709,431, 6,929,639, 6,989,009, 7,022,120, 7,101,368, 7,172,589, 7,189,227, 7,198,632, and 7,220,257, which are incorporated herein by reference. Embodiments of the invention may incorporate selected balloon, catheter, and other features of the devices disclosed in U.S. Pat. Nos. 6,355,029, 6,428,534, 6,432,102, 6,468,297, 6,514,245, 6,602,246, 6,648,879, 6,786,900, 6,786,901, 6,811,550, 6,908,462, 6,972,015, and 7,081,112, which are incorporated herein by reference.

In various embodiments, the balloon **64** comprises a cryoballoon (or a separate cryoballoon may be used as previously discussed) and the ultrasound unit **50** includes one or more ultrasonic emitters **52**. The balloon **64** and ultrasound unit **50** cooperate to deliver acoustic and thermal energy to target tissue **49**. In some embodiments, the ultrasound unit **50** comprises an ultrasonic emitter **52** that creates lesions in the artery wall primarily through disruptive heating of target tissue. In other embodiments, the ultrasound unit **50** comprises an ultrasonic emitter **52** that creates lesions in the artery wall primarily by production of cavitation bubbles, which work to mechanically disrupt nerve fibers and ganglia with the bubbles implode or explode.

According to various embodiments, a denervation therapy procedure using the apparatus shown in FIG. **8** involves selectively freezing and heating (and optionally thawing) target tissue **49** that includes renal nerves **14** and/or ganglia **24/22**. For example, target innervated tissue **49** is frozen using a cryoballoon **64**. Before the target tissue **49** thaws, acoustic energy is transmitted to the target tissue **49** by the ultrasound unit **50** to fracture the renal nerve fibers and nerve sheaths located in the adventitia or vasa vasorum externae, thereby permanently terminating renal sympathetic nerve traffic along the treated renal nerve structures. A detailed discussion of renal nerve structures and degrees of nerve disruption that can be achieved using embodiments of the invention is provided in previously cited U.S. application Ser. No. 12/980,952.

The cryoballoon **64** and/or catheter apparatus is preferably configured to allow blood to flow at or near the inner vessel wall after cryotherapy has been delivered to allow for local heating of the endothelium and adjacent tissue (e.g., intima and media tissue) while the adventitia remains frozen. Acoustic energy is preferably transmitted to the still-frozen adventitia layer (at least to deeper layers near the vessel's outer wall) to permanently disrupt renal nerves and ganglia included in the frozen tissue.

An advantage of using combined cryogenic and ultrasonic therapies for denervating renal artery and aortal tissue is that blood coagulation and embolization associated with RF ablation is avoided. Another advantage is that nerve regeneration over time that can occur when using cryotherapy alone is prevented, because of the fracturing of the renal nerve sheath resulting from mechanical disruption when using cavitation ultrasonic denervation therapy, or from thermal necrotic coagulation when using thermal ultrasonic denervation therapy, which permanently disrupts renal nerve sheaths.

With reference to FIG. **9**, there is shown an embodiment of an ultrasonic ablation apparatus which includes an ultrasound unit **50** incorporated into a balloon **64**. The ultrasonic ablation apparatus shown in FIG. **9** may include an imaging capability. The balloon **64** may be affixed adjacent to a distal end of a first catheter **91**. The first catheter **91** may include a central shaft **88** disposed within a lumen **93** of the first catheter **91** and within an interior volume of the balloon **64**. A spiral rail **99** may be disposed about an outer surface of the central shaft **88** adjacent to a distal end of the central shaft **88**. In some instances, the spiral rail **99** may be mounted on the central shaft **88** such that it extends around the entire circumference of the central shaft **88**. In other instances, the spiral rail **99** may extend around only a portion of the circumference of the central shaft **88**. The ultrasound unit **50** and/or emitter **52** may be disposed adjacent to a distal end of a second catheter **92**. The second catheter **92** may be disposed within the lumen **93** of the first catheter **91** and slidable relative to the first catheter **91** such that the ultrasound unit **50** may be moved along the spiral rail **99**. An advantage of using a balloon **64** of the type shown in FIG. **9** is that the translation and rotation of the ultrasound unit **50** may be accomplished by drawing or sliding the ultrasound unit **50** along a spiral rail **99** mounted on a central shaft **88** of the balloon **64**. A keyed channel arrangement **96**, for example, may be disposed at the distal end of the catheter **92** supporting the ultrasound unit **50**, which receives and captures the spiral rail **99** such that drawing or sliding the second catheter **92** may cause the ultrasound unit **50** to follow the spiral path of the spiral rail **99**.

The emitter **52** of the ultrasound unit **50** may be orientated at a desired angle relative to the longitudinal axis of the shaft **88** or relative to the rail **99**. For example, the ultrasound unit **50** may be orientated at an angle ranging between 0 and 90 degrees relative to the longitudinal axis of the shaft **88** or the rail **99**. With the ultrasound unit **50** moving axially along a spiral path defined by the rail **99** inside the balloon **64**, no scraping of the renal artery wall **12** will occur. The catheter **92** is preferably translated along the rail **99** causing the ultrasound unit **50** to rotate and create a spiral burn, which interrupts any neural transmissions passing longitudinally within the wall of the renal artery **12**. As discussed above, the balloon **64** may be filled with an acoustically transparent liquid, such as a cooling liquid.

FIG. **10** illustrates an ultrasonic ablation apparatus, which includes an ultrasound unit **50** situated at a distal end of a catheter **92**, incorporated into a balloon **64** in accordance with various embodiments of the invention. The ultrasonic ablation apparatus of FIG. **10** may include an imaging capability.

In the embodiment shown in FIG. 10, the ultrasound unit 50 at the distal end of a catheter 92 is oriented off-axis with respect to the longitudinal axis of the shaft 88. In FIG. 10, the emitter 52 of the ultrasound unit 50 is shown oriented about 90° relative to the longitudinal axis of the shaft 88. It is understood that other emitter orientations may be desirable.

For example, the ultrasound unit 50 may be oriented at an angle of about 45° to about 135° relative to the longitudinal axis of the shaft 88. Also, the emitter 52 may be biased more toward the shaft 88 than the outer surface of the balloon 64. The ultrasound unit 50 may be configured to extend from and retract into the shaft 88 under user or robotic control, which may be of particular benefit when expanding and contracting the balloon 64. The shaft 88 and the ultrasound unit 50 may be

translatable and/or rotatable within the balloon 64. FIG. 11 shows an embodiment of an extracorporeal denervation arrangement for denervating renal vasculature that contributes to renal sympathetic nerve activity in accordance with the invention. According to this embodiment, an emitter 52 of a lithotripsy machine 35 is shown positioned at or above the patient's skin 47 proximate a renal artery 12. The lithotripsy machine 35 generates high-energy shockwaves that are directed to target tissue 49 to fragment renal nerve and ganglia tissue structures (e.g., sheaths of nerve fibers located in the adventitia, vasa vasorum, or in ganglia). The lithotripsy machine 35 may be configured as an extracorporeal shock-wave lithotripsy (ESWL) machine, for example.

The lithotripsy machine 35 uses one or both of x-rays and ultrasound scanning to locate target tissue that includes innervated renal vasculature. The lithotripsy machine 35 generates an acoustic shockwave, which is transmitted into the body via the emitter 52. Embodiments of an extracorporeal lithotripsy system for denervating renal and aortal tissue may incorporate components and functionality disclosed in U.S. Pat. No. 6,123,679, which is incorporated herein by reference.

According to other embodiments, an intracorporeal lithotripsy system may be used to denervate renal and aortal vasculature that contributes to renal sympathetic nerve activity. An intracorporeal lithotripsy system typically includes an endoscope that is percutaneously advanced to a location within the body proximate a renal artery or the abdominal aorta. An acoustic shockwave is transmitted from an emitter 52 of the endoscope into the renal artery or the abdominal aorta to disrupt innervated target tissue. Embodiments of an intracorporeal lithotripsy system for denervating renal and aortal tissue may incorporate components and functionality disclosed in commonly owned U.S. Pat. No. 5,906,623, which is incorporated herein by reference.

In other embodiments, an intracorporeal laser lithotripsy or lasertripsy system may be used to denervate renal and aortal vasculature that contributes to renal sympathetic nerve activity. An intracorporeal lasertripsy system of the present invention includes a laser source and an optical fiber that extends along a longitudinal axis of a rigid or flexible endoscope. Laser light of an appropriate wavelength and power is transmitted from the optical fiber to a focal point or region that includes innervated renal tissue. Various types of lasertripsy systems and laser sources may be used, including systems that include a pulsed dye laser, an alexandrite laser, a neodymium laser, and a holmium laser, for example. Embodiments of an intracorporeal lasertripsy denervation system for denervating renal and aortal tissue may incorporate components and functionality disclosed in commonly owned U.S. Provisional Application Ser. No. 61/324,163, and in commonly owned U.S. Pat. No. 7,104,983, both of which are incorporated herein by reference.

In accordance with various embodiments employing acoustic or laser lithotripsy, and as further shown in FIG. 11, an intravascular cryocatheter or cryoballoon 64 is deployed within the renal artery to freeze target tissue 49 prior to delivering lithotripsy therapy to the target tissue 49. Freezing the target tissue 49 prior to delivering lithotripsy therapy enhances disruption of target nerve structures by the shockwaves impinging on the frozen target tissue 49. Freezing of the target tissue 49 in the context of the embodiment illustrated in FIG. 11 may be accomplished using various devices and techniques described herein.

FIGS. 12A-12D show different embodiments of an ultrasound unit 50 configured for denervating renal vasculature that contributes to renal sympathetic nerve activity in accordance with the invention. In the embodiment shown in FIG. 12A, the emitter 52 of the ultrasound unit 50 includes an aperture 65 through which an acoustic energy beam 62 passes. The aperture 65 may be a void, a lens arrangement, or acoustic coupling material that allows for efficient transmission of the acoustic energy beam 62 from the emitter 52 and out of the ultrasound unit 50. The aperture 65 and emitter 52 are situated at a desired location of the ultrasound unit 50, and can be "aimed" at target tissue by rotating and translating the catheter 51 to which the ultrasound unit 50 is attached, or the ultrasound unit 50 relative to the catheter 51 in embodiments where the ultrasound unit 50 is movable relative to the catheter 51, either manually or robotically.

According one approach, the catheter 51 can be translated and rotated along the rail 99 to cause the ultrasound unit 50 to create a spiral burn. In another approach, an ultrasound unit 50 equipped with a focused ultrasonic emitter 52 can be rotated to create a circular or cylindrical burn without incurring undue risk of stenosis of the renal artery 12.

One advantage of creating a circular or cylindrical lesion in the renal artery wall is that the longitudinal extent of the lesion is limited, which allows for repeated denervation procedures to be performed at untreated regions of the renal artery without undue risk of artery stenosis. For example, a circular or cylindrical lesion may be created near the ostium of the renal artery, leaving the majority of renal artery tissue untreated. Should additional renal denervation be required, a subsequent circular or cylindrical lesion may be created near the center or distal end of the renal artery. A mapping of renal artery lesion locations for a given patient may be stored to aid in avoiding previously treated regions of the artery when performing a subsequent ablation procedure.

FIG. 12B shows an ultrasound unit 50 comprising a multiplicity of apertures 65 and emitters 52. The apertures 65 and emitters 52 are preferably situated so that their beam patterns 62 collectively impinge on renal artery tissue in a generally spiral pattern and at target depths in the renal artery wall. The spiral lesion may either be continuous or a sequential and overlapping line of ablated spots.

The ultrasound unit 50 shown in FIG. 12B advantageously facilitates a "one-shot" denervation therapy of the renal artery or other vessel in accordance with embodiments of the present invention. The term "one-shot" treatment refers to treating the entirety of a desired portion of a vessel without having to move the treatment implement or arrangement to other vessel locations in order to complete the treatment procedure (as is the case for a step-and-repeat denervation therapy approach).

A one-shot treatment approach according to the embodiment shown in FIG. 12B advantageously facilitates delivery of denervation therapy that treats at least one location of each nerve fiber extending along a target vessel, such as the renal artery, without having to reposition the ultrasound unit 50

during denervation therapy delivery. The embodiment of an ultrasound unit **50** shown in FIG. 12B allows a physician to position the ultrasound unit **50** at a desired vessel location, and completely treat the vessel without having to move the ultrasound unit **50** to a new vessel location.

It is noted that, in some embodiments, the ultrasound unit **50** can be coupled to the catheter **51** using a coupling arrangement that allows the ultrasound unit **50** to be rotated relative to the catheter **51**. A manual or motorized apparatus may be controlled to cause rotation of the ultrasound unit **50** relative to the catheter **51**. In other embodiments, the ultrasound unit **50** may be coupled to the catheter **51** such that rotation of the catheter **51** causes rotation of the ultrasound unit **50**.

FIGS. 12C and 12D illustrate embodiments of an ultrasound unit **50** configured for denervating renal vasculature that contributes to renal sympathetic nerve activity in accordance with the invention. In the embodiments shown in FIGS. 12C and 12D, the emitter **52** of the ultrasound unit **50** includes an acoustic phased array transducer **52a** which comprises a multiplicity of acoustic elements **52b**. The phased array transducer **52a** shown in FIG. 12C extends over a radial segment of the ultrasound unit's circumference, allowing an acoustic energy beam **62** to pass through an aperture **65** (e.g., lens arrangement) and impinge on target tissue. As can be the case in other embodiments, the emitter **52** of the ultrasound unit **50** may be aimed at target tissue by rotating and translating the catheter **51**, or by moving the ultrasound unit **50** relative to the catheter **51**, either manually or robotically.

In the embodiment shown in FIG. 12D, a phased array transducer **52a** extends over all or nearly all of the ultrasound unit's circumference, allowing an acoustic energy beam **62** to pass through an annular aperture **65** (e.g., lens arrangement) and impinge on a circular or cylindrical target tissue region. After positioning the ultrasound unit **50** within the renal artery, for example, renal denervation can be conducted without having to translate or rotate the catheter **51** or ultrasound unit **50**.

A cooling arrangement may be incorporated in the embodiments of FIGS. 12A-12D to ensure that the temperature of inner arterial or aortal wall tissue (e.g., intima, media) is limited to prevent thermal injury to this tissue. In embodiments that include focused acoustic transducers or transducer arrays, however, such cooling arrangement may not be required or desired, which can result in intravascular denervation apparatuses of reduced size and complexity.

Different embodiments of phased array acoustic emitter arrangements that can be incorporated in ultrasound units **50** of the invention are shown in FIGS. 13 and 14. Phased array transducers **52a** are typically more effective than conventional planar or curved piezoelectric transducers and are well suited for high power ultrasonic ablation of innervated renal vasculature. The phased array transducers **52a** comprise a number of individual ultrasonic elements **52b**, often called "pixels," with each pixel having a respective wired connection to an electrical driver. By controlling the phases of each of the electrical drivers, an ultrasound beam can be electronically scanned in a target tissue location.

FIGS. 13A and 13B are sectional views of an ultrasonic emitter **52** comprising different configurations of phased array transducers **52a** having a generally cylindrical shape in accordance with embodiments of the invention. The ultrasonic emitter **52** shown in FIG. 13A includes a phased array transducer **52a** comprising a multiplicity of individual ultrasonic elements **52b** supported by a flexible circuit substrate **77** and arranged in a spaced-apart relationship about the circumference of the ultrasonic emitter **52** (although only a few representative elements **52b** are shown in FIG. 13A for clar-

ity). In FIG. 13B, the ultrasonic emitter **52** includes a phased array transducer **52a** comprising a multiplicity of individual ultrasonic elements **52b** supported by a flexible circuit substrate **77** and arranged in a spaced-apart relationship about a radial segment of the circumference of the ultrasonic emitter **52**.

In the embodiment shown in FIG. 13A, acoustic energy is emitted in a circular or cylindrical beam pattern, which provides for scanning and/or ablating of a circular or cylindrical target region of the renal artery or abdominal aorta. It is noted that the phased array transducer **52a** shown in FIG. 13A need not extend along the entirety of the ultrasonic emitter's circumference, since the ultrasonic beam spread at the opposing ends has a laterally extending aspect. In the embodiment shown in FIG. 13B, acoustic energy is emitted in a partial circular or cylindrical beam pattern (e.g., $<360^\circ$, such as 20° - 90°), which provides for scanning and/or ablating of a partial circular or cylindrical region of renal artery or abdominal aorta target tissue.

Adjacent an outer circumference of the phased array transducer **52a** is an acoustic lens **78**, as is shown in FIGS. 13A and 13B. An acoustic coupling material or liquid may be disposed between the phased array transducer **52a** and the acoustic lens **78**. Adjacent an inner circumference of the phased array transducer **52a** are one or more acoustic layers **76**, which are in contact with a cylindrical backing member **72** that encompasses a supportive core **72**.

The phased array transducer **52a** shown in FIGS. 13A and 13B may be formed by dividing one or more larger piezoelectric blocks into two or more individual ultrasonic elements **52b** supported by the flexible circuit substrate **77**. Individual ultrasonic elements **52b** are responsive to an appropriate electrical stimulus for generating acoustic energy in the ultrasonic frequency range. The number of individual ultrasonic elements **52b** may vary significantly depending on transducer configuration and requirements.

For example, a HIFU ultrasonic emitter **52a** that incorporates one or more ultrasonic phased array transducers **52a** may include 10 or less ultrasonic elements **52b** to as many as 1,000 elements **52b** or more (e.g., ≥ 24 , ≥ 64 , ≥ 256 , ≥ 512 , ≥ 768 , or ≥ 1024 individual elements **52b** may be incorporated in ultrasonic phased array transducers **52a** according to various embodiments).

HIFU phased array driving electronics can be adapted to control the phase and amplitude of individual ultrasonic elements **52b** using an appropriate number of control channels. For example, a HIFU ultrasonic emitter **52a** may include up to 1024 discrete ultrasonic elements **52b** each controlled by a separate channel with 2 ns phase resolution, 8-bit amplitude resolution, operate over a frequency range of 1 to 5 MHz, and deliver between 8 and 15 W of power to each channel.

The use of a large number of ultrasonic elements and control channels allows for the elimination of mechanical motion components of conventional single-element and array HIFU systems. For example, a HIFU phased array transducer **52a** that incorporates a large number of ultrasonic elements and channels can simulate movement of the array using various known subaperture focusing techniques. A HIFU phased array transducer **52a** may be electronically controlled to generate sufficiently high HIFU intensities at foci of spherical or cylindrical geometries and at a desired depth within innervated renal tissue.

It is noted that curvilinear or convex sector phased arrays may be used as an alternative to, or in concert with, a linear phased array configuration. A curvilinear phased array operates in the same manner as the linear array in that the scan lines are directed perpendicular to the transducer face. The

acoustic beams generated by curvilinear or convex sector phased arrays are typically focused, rather than steered.

The power level and frequency range may be selected to provide for both scanning (e.g., lower power) and ablating (e.g., higher power) of innervated renal tissue. Although the acoustic power and transducer efficiency will vary among ultrasound transducer implementation, it is desirable that power levels corresponding to focal peak intensities equal to or greater than about 2000 W/cm² in target tissue be achieved, which are capable of producing coagulative necrosis in the target tissue.

With reference to FIG. 14, an ultrasound unit 50 includes an ultrasonic transducer 52 that can operate in a scan mode, a thermal ablation mode, or a cavitation ablation mode. As is shown in FIG. 14, the transducer 52 includes a transducer element 66 (e.g., a piezoelectric element), a focusing lens 67, and acoustic material 68 which can be configured as an acoustic backing for the transducer 52.

The diameter and frequency of the transducer element 66 and the characteristics of the focusing lens 67 on the front of the transducer element 66 are preferably selected to maximize the intensity of acoustic power in the wall of the renal artery, which makes efficient use of the available power, reduces collateral damage, and makes the lesion relatively insensitive to small changes in the spacing from the transducer face to the artery wall. A temperature sensing element 69 may be provided and positioned to contact the transducer element 66 to monitor its temperature and prevent overheating. An acoustic backing layer 68 may be provided on the transducer element 66 to broaden the bandwidth of the transducer element 66 and to minimize the need for the ultrasound driver (not shown) to adapt the drive frequency to the ultrasound unit 50, which is typically a disposable element.

As was discussed above, the transducer element 66 may be operated in a scan mode, such as an A-scan mode or a B-scan mode as is understood in the art. Operating in the scan mode allows the system computer to diagnostically detect the range to the artery wall and potentially the thickness of the wall, and adapt the ultrasonic power and velocity of catheter translation so that a lesion of desired depth can be accomplished by the computer in the ultrasonic power drive unit.

Operating the ultrasound unit 50 in the scan mode allows the physician to see the lesion forming and estimate its depth intermittently or continuously. For example, the transducer element 66 may transmit continuously for a period during which the tissue in range will heat up. The transducer element 66 can then transmit a relatively short pulse and "listen" for the echoes as the system functions as an A-scan ultrasonic imager. The transducer element 66 can then detect the artery walls, lesion depth, and bubbles resulting from disruptive cavitation within the target tissue, and adjust the power strategy as desired. The transducer element 66 can then continue to transmit continuously for a period of time at the same or a modified transmit power.

It is noted that the ultrasound unit 50 may incorporate multiple transducers 52. In these configurations, some of the transducers 52 can operate continuously in a scan mode, while other transducers 52 can be operated continuously, intermittently, or sequentially in a cavitation ablation mode. For example, an ultrasound unit 50 may incorporate multiple transducers 52 that are arranged to produce a spiral lesion at the desired depth in the wall of the renal artery while the ultrasound unit 50 remains stationary within the lumen of the renal artery. This configuration provides for a "one-shot" denervation therapy approach in accordance with various embodiments of the invention.

With further reference to FIG. 14, the transducer 52 according to various embodiments includes a planar disk transducer element 66. As shown, the disk transducer 52 is supported within the housing of the ultrasound unit 50 which may have a cylindrical shape. The ultrasound unit 50 in this configuration can be translated longitudinally and rotated relative to a shaft 53 by appropriate manipulation of the catheter 51 to which the ultrasound unit 50 is connected. By properly translating and/or rotating the ultrasound unit 50, the location of the ablation moves, so that a spiral ablation or series of spot ablations may be made in the renal wall artery at the desired depth.

With a planar disk transducer 52, the ultrasound intensity is approximately constant near the transducer 52 and then drops faster as the range exceeds the diameter of the disk transducer element 66. A mechanism is preferably employed to stabilize the disk transducer element 66 so that its plane is parallel to the renal artery. It is also preferably to maintain the distance between the disk transducer element 66 and the artery wall approximately constant as the disk transducer 52 is translated and rotated.

The planar disk transducer 52 shown in FIG. 14 is a very practical design which can produce a relatively controllable burn width and depth as the disk transducer 52 is translated and displaced to produce a spiral burn inside the renal artery wall at the desired depth.

The beam angle of an ultrasonic disk transducer 52 will be normal to the disk transducer element 66 and centered on the axis of the disk transducer element 66. The beam angle, BA, shown in FIG. 14 can be characterized by:

$$\sin \theta = 1.2V/(DF)$$

where θ is the half angle of the diverging beam (DB) in the far field, V is the sound velocity in the material, D is the diameter of the transducer element 66, and F is the frequency of the transducer 52.

FIG. 15 shows another embodiment of an ultrasound unit 50 that includes a barrel shaped cylindrical ultrasonic transducer 52 that is configured to operate at least in a cavitation ablation mode. The barrel shaped cylindrical ultrasonic transducer 52 may also be operated in other modes, including a scan mode as discussed previously. In the configuration shown in FIG. 15, the hollow cylindrical barrel shaped transducer 52 rides over a central shaft 53 to treat the desired location on the renal artery. If not masked with acoustic reflector material, the transducer 52 will treat a complete 360° ring of tissue. If masked with an acoustic reflector material, the treatment will cover only part of the artery wall circumference.

Rotating the barrel shaped transducer 52 controls which angular section of the renal artery will be treated. Translating a masked barrel shaped transducer 52 will produce a spiral lesion if continuously on, or a spiral of spots within the renal artery wall if powered intermittently. It is desirable to use a centering mechanism to insure that the barrel shaped transducer 52 is centered in the lumen of the renal artery because the ultrasound power intensity decreases as the square of the distance from the center if the barrel transducer element 66 is longer than the inner diameter of the artery. It is also desirable to provide for cooling of the barrel transducer element 66, since its efficiency is typically not more than about 40%. Cooling can be accomplished by allowing blood to flow past the transducer 52 or by providing cooling liquid such as saline or D5W, which can be closed or open irrigated.

The beam angle, BA, of a barrel shaped cylindrical transducer 52 will be normal to the axis of the cylinder defining the transducer element 66 and will diverge with a beam, DB,

which has one angle in the plane which intersects the axis of the cylinder and a second angle in the plane perpendicular to the first plane. The angle (DB) in the first plane is similar to that calculated above. The angle in the second plane is related to the diameter of the barrel of the transducer element 66, but the effective diameter is only about half as wide because ultrasound cannot be transmitted much off the normal, which makes the beam divergence about twice as great.

For either of the ultrasonic transducers 66 shown in FIGS. 14 and 15, it is desirable to choose a transducer diameter based on the renal artery diameter, which is about 5 mm, and a separation between the transducer 66 and the artery wall. It is desirable to choose the optimum frequency to minimize the beam divergence at the artery wall location.

It is noted that the ultrasound units 50 shown in FIGS. 14 and 15 may be used with various stabilization arrangements, including balloons. In some embodiments, the transducer assembly 50 is enclosed within a balloon filled with saline, so that the balloon and shaft center the transducer 52 in the renal artery and the balloon stops blood flow so that less total power is required to heat the artery wall to ablate it. In other embodiments, the ultrasound units 50 shown in FIGS. 14 and 15 may be adapted to travel along a spiral rail supported by a shaft, such as is shown in FIG. 9, and may further travel within a filled balloon as shown and described with reference to FIG. 10.

FIG. 16 is an exaggerated sectional view of a renal artery 12 and an ultrasonic beam emitted from an ultrasonic emitter 52a of an ultrasound unit 50 positioned within a lumen 13 of the renal artery 12. In this illustrative embodiment, the ultrasonic emitter 52a is configured to focus acoustic energy at a volume of tissue of the adventitia 36 proximate the outer wall of the renal artery 12 that includes a renal nerve 14.

As previously discussed, the ultrasound unit 50 may be operated to scan the adventitia 36 and vasa vasorum for renal nerves 14 and ganglia 24/22 using relatively low power acoustic energy. The ultrasound unit 50 may also be operated to deliver relatively high power acoustic energy to create lesions that permanently disrupt the target renal nerve 14. Employment of an ultrasound unit 50 that includes a HIFU emitter 52a advantageously spares tissues of the intima 32 and media 33 from injury.

It is generally known that a typical renal artery of a human adult has a diameter of about 5 mm. Embodiments of ultrasonic emitter and lens arrangements described herein may be implemented to project acoustic energy to foci having a depth of focus ranging between about 1 mm to about 10 mm, which is sufficient to reach target tissues of the renal artery wall, including ganglia, and the vasa vasorum proximate the outer wall of the renal artery.

In various embodiments, an ultrasonic emitter 52a may be implemented to project acoustic energy to foci having a depth of focus that falls within a target range that encompasses the outer adventitial layers of the renal artery. In other embodiments, an ultrasonic emitter 52a may be implemented to project acoustic energy to foci having a depth of focus that falls within a target range that encompasses the outer adventitial layers of the renal artery and the vasa vasorum proximate the outer wall of the renal artery. It is understood that ultrasonic emitter and lens arrangements may be configured for projecting acoustic energy to foci having a depth of focus that falls within a target range that encompasses renal nerves of the renal artery's ostium and ganglia of the abdominal aorta.

According to various embodiments, a multiplicity of separate ultrasonic emitter and/or lens arrangements may be used to project acoustic energy to multiple foci having different depths of focus. Particular ones of the multiplicity of

arrangements may be selectively operated for scanning and/or ablating at different tissue depths. For example, scanning at different depths within the outer renal artery wall and adjacent vasa vasorum can be performed to locate target tissue that includes one or both of renal nerves and ganglia. After determining the target tissue location and depth, which may alternatively be accomplished using a separate internal or external imager, a selected one or more of the ultrasonic emitter and/or lens arrangements may be used to ablate the target tissue at the determined depth.

FIG. 17 illustrates an embodiment of an ultrasound system for denervating and optionally scanning innervated vasculature that contributes to renal sympathetic nerve activity in accordance with the invention. The ultrasound system shown in FIG. 17 includes a controller 151 configured to execute program instructions for controlling components and operations of the ultrasound system. The ultrasound system includes an ultrasound source 150 that generates acoustic energy having desired characteristics, such as desired frequency, intensity, beam pattern, and penetration depth characteristics. In some embodiments, the ultrasound source 150 is configured to generate a continuous wave (CW) acoustic beam. In other embodiments, the ultrasonic source 150 is configured to generate high intensity, low duty cycle pulses of acoustic energy.

The ultrasound delivery apparatus shown in FIG. 17 can be operated in a scanning or imaging mode, an ultrasonic denervation therapy mode, or both (sequentially or concurrently). In some embodiments, it may be desirable to incorporate a separate ultrasound delivery apparatus for each of a scanning or imaging mode and an ultrasonic denervation therapy mode.

According to various embodiments, acoustic energy produced by the ultrasonic source 150 is directed to a focusing arrangement 154. The focusing arrangement 154 may include one or more acoustic lenses for shaping and directing acoustic energy received from the ultrasonic source 150 to target tissue 49, such as renal artery tissue which includes a renal nerve 14. The acoustic energy exiting the focusing arrangement 154 and penetrating the target tissue 49 is preferably a focused ultrasonic beam 62 of sufficient intensity to permanently disrupt renal nerves 14 included in the target tissue 49. An imager 53 (external or internal) is preferably used to facilitate positioning of an ultrasound unit of the ultrasound delivery apparatus, and may also be used to determine or adjust various operating parameters, such as acoustic energy intensity, duty cycle, frequency, beam shape, beam direction, axial depth, and longitudinal resolution, for example.

In some embodiments, target renal artery tissue 49 can be heated using focused acoustic energy 62, and, if the artery wall tissue temperature exceeds 50° C., the tissue can be killed. However, the target tissue 49 will not be physically and permanently disrupted until the temperature of the target tissue 49 exceeds about 65° C., where the collagen reforms. With focused acoustic energy beams 62, a small focus can be achieved deep in target tissues 49, such as a focal region or volume within the adventitia tunica or vasa vasorum that includes a renal nerve or ganglion. When the temperature within the target tissue 49 reaches a sufficient level (e.g., >65° C.), the target tissue 49 is thermally coagulated (e.g., coagulative necrosis). By focusing at more than one tissue location or by scanning the focused beam, a volume of target tissue can be thermally ablated.

Other embodiments of the invention are directed to an ultrasound source 150 and a focusing arrangement 154 configured for operation in a cavitation ablation mode. Operating the ultrasound source 150 and focusing arrangement 154 in a

cavitation ablation mode, for example, is preferably accomplished by transmitting a string of high intensity, low duty cycle acoustic energy pulses into the target tissue **49**. Embodiments of the invention are also directed to an ultrasound source **150** and focusing arrangement **154** that is selectively operable in a cavitation ablation mode and a scan mode, allowing the ultrasound unit to locate target renal artery tissue in one mode and then permanently disrupt renal nerve fibers and ganglia within the target tissue in a second mode.

In accordance with other embodiments, acoustic energy produced by the ultrasonic source **150** may be used for imaging tissues of the renal and aortal vasculature. In ultrasonic imaging applications, the intensity of the acoustic energy is less than that required for ablation, and is preferably low enough to avoid thermal injury to scanned tissue.

In the embodiment shown in FIG. **17**, acoustic energy backreflected from the target tissue **49** is received at a detector **160**. The detector **160** may be incorporated in the transducer of the ultrasound source **150** or in a separate detector component. The detector **160** typically converts received acoustic energy to an electrical signal, which is transmitted to imaging electronics **162** via communications circuitry **161**. Imaging electronics **162** preferably implements one or more known techniques for imaging scanned tissue **49** at various depths and transverse lengths or regions (e.g., focal volumes) using the backreflected acoustic energy. Output from the imaging electronics **162** is received by a computer **164** which preferably includes a display. Data and visual information concerning the scanning and ultrasonic denervation procedures are preferably presented on the display. The computer **164** may include an interface (I/O) for communicating with other systems and devices.

The controller **151** of the ultrasound system may be configured to generate a 2D image by controlling the sweep of the ultrasonic beam **62**. The ultrasound source **150** may be swept mechanically, such as by rotating or swinging. In another approach, a 1D phased array ultrasound source **150** may be used to sweep the ultrasonic beam **62** electronically. The received data is processed by the computer **164** and used to construct the image. This image is a 2D representation of a slice into the renal artery or abdominal aorta. 3D images can be generated in real-time by acquiring a series of adjacent 2D images, such as by using one or more 2D phased array ultrasonic transducers that sweep the ultrasonic beam **62**.

The ultrasound system may be operated in one or more scanning modes. In an A-scan mode, for example, a single ultrasonic transducer is used to scan a line through the renal artery tissue with the echoes plotted on a display as a function of depth. In a B-scan mode, a linear array of ultrasonic transducers are used to simultaneously scan a plane through the renal artery tissue that can be viewed as a two-dimensional image on the display.

FIGS. **18A** and **18B** illustrate representative deployment configurations of a focused ultrasound catheter that can be operated for one or both of transvascular scanning and denervation of innervated vasculature in accordance with embodiments of the invention. In FIG. **18A**, an ultrasound unit **50** is shown deployed in a patient's abdominal aorta **20** proximate a renal artery **12**. In FIG. **18B**, an ultrasound unit **50** is shown deployed in a patient's inferior vena cava **40** proximate a renal artery **12**. In this position shown in FIG. **18B**, the ultrasound unit **50** can be used to denervate the aorticorenal ganglion **22** and/or the renal ganglion **24**.

When positioned within the patient's renal vein **42**, as also shown in FIG. **18B**, the ultrasound unit **50** can be used to denervate the aorticorenal ganglion and/or the renal ganglion. According to one procedure, the ultrasound unit **50** is moved

to a renal vein location for denervating renal ganglia **24** of the renal artery **12**, and moved to an inferior vena cava location for denervating ganglia of the abdominal aorta, such as the aorticorenal ganglion **22**.

The ultrasound unit **50** includes an ultrasonic emitter **52** that can be operated in a denervation mode and, optionally, a scanning mode. In this representative illustration, the ultrasonic emitter **52** is operated in a scan mode to aid in locating target tissue, such as aorticorenal ganglion **22** and renal ganglion **24**.

After locating the target tissue, the ultrasonic emitter **52** or another imaging device (external or internal) is used to determine the range to the target tissue. The ultrasonic emitter **52** is focused electronically (e.g., via a subaperture or electronic focus or steering technique) or mechanically at the target tissue based on the range information. Acoustic energy is transmitted to the target tissue sufficient to permanently denervate the target tissue, by use of thermal or cavitation ablation modes.

It is noted that an ultrasound unit **50** in accordance with various embodiments of the invention may incorporate multiple ultrasonic devices for purposes of imaging and/or ablating target tissue. Some of the ultrasonic devices, for example, can operate continuously in a scan mode, while other ultrasonic devices can be operated continuously, intermittently, or sequentially in an ablation mode.

FIG. **19** illustrates an apparatus for facilitating guided delivery of an ablation agent to ganglia that contribute to renal sympathetic nerve activity in accordance with embodiments of the invention. According to various embodiments, a delivery catheter **101** is used cooperatively with an imaging system to locate a target ganglion and deliver an ablation agent to the target ganglion. In FIG. **19**, the delivery catheter **101** is configured for intra-to-extra vascular deployment, and the imaging system may include an intravascular imaging catheter **105** or an external imager **53** of a type previously described.

According to some embodiments, an intravascular imaging catheter **105** is delivered to a location within a patient's renal artery **12**, typically accessed via the inferior abdominal aorta **20**. The intravascular imaging catheter **105** preferably includes an imaging device **107**, such as an IVUS device or other ultrasonic imaging device, or a laser imaging device, such as a laser transducer or other optical imaging device. With the imaging device **107** properly positioned in or proximate the renal artery **12**, the delivery catheter **101** is advanced into the renal vein **42**, typically accessed via the inferior vena cava **40**. The delivery catheter **101** preferably includes a steering mechanism. Suitable steering mechanisms that can be incorporated in a delivery catheter **101** of the present invention include various mechanisms incorporated into known steerable guide catheters.

The delivery catheter **101** includes a tissue penetrating feature at its distal tip, such as tissue piercing tip **103**, to aid in creating an access hole **102** in the renal vein **42**. Alternatively, an energy source, for example radiofrequency or laser, may be applied at the catheter tip to assist in puncturing the wall of the renal vein **42**. With aid from the imaging catheter **105** or external imager **53**, the delivery catheter **101** is advanced through the access hole **102** and navigated around the exterior of the renal artery **12** to a location adjacent a target ganglion, such as a renal ganglion **24**.

Using the tissue piercing tip **103**, the delivery catheter **101** is forcibly advanced so that a portion of the distal tip of the delivery catheter **101** penetrates into the renal ganglion **24**. An ablation agent is delivered to ganglion tissue via the delivery catheter **101**. The ablation agent is preferably effective in

killing nerve fibers of the renal ganglion **24**, so that all renal sympathetic nerve activity associated with the renal ganglion **24** is permanently terminated.

In some embodiments, the delivery catheter **101** includes a lumen which is fluidly coupled to a distal port and a proximal port of the delivery catheter **101**. The proximal port is coupled to an ablation agent source, and the distal port is configured to dispense an ablation agent from the distal tip of the delivery catheter **101**. In other embodiments, a cavity of the distal tip of the delivery catheter **101** contains an ablation agent, which may be a fluid, a solid, or a soluble mixture or matrix. The ablation agent may be eluted or otherwise communicated from the cavity of the distal tip of the delivery catheter **101** into the renal ganglion **24**.

The delivery catheter **101** may be configured to deliver a variety of ablation agents via an ablation dispensing arrangement (e.g., lumen and port system, distal tip cavity). The ablation agent may take the form of a pharmacological agent or mixture of agents (e.g., a neurotoxin or venom), a thermal transfer fluid (hot or cold), or radioactive material or seeds (e.g., iodine-125 or palladium-103 for low dosage rate brachytherapy, iridium-192 for high dose rate brachytherapy). A variety of cryogens may be employed as ablation agents, including cold saline or cold saline and ethanol mixture, Freon or other fluorocarbon refrigerants, nitrous oxide, liquid nitrogen, and liquid carbon dioxide, for example. Alternatively, DC, AC, or RF electrical current may be dispensed from tip **103** via a lead that passes through lumen **102** to heat tissue or alter tissue sufficiently for ablation.

After delivering the ablation agent to the renal ganglion **24**, the delivery catheter **101** can be navigated to another ganglion, such as the aorticorenal ganglion **22**, the superior mesenteric ganglion, or the celiac ganglia or plexus. The imaging catheter **107** is preferably moved to an appropriate intravascular location to aid navigation and positioning of the delivery catheter **101**, such as a location within the abdominal aorta **20** or renal vein **40**.

One or more physiologic parameters can be monitored during the procedure to determine the effect of the ablation agent on the patient's renal sympathetic nerve activity. For example, an electrode arrangement may be situated in contact with the inner or outer wall of the renal artery **12** near opposing sides of the renal ganglion **24**. The electrode arrangement may be configured to measure nerve impulses transmitted along renal nerve fibers that couple to or pass through the renal ganglion **24**. By way of further example, one or more physiological parameters that are sensitive to changes in renal sympathetic nerve activity may be monitored, and the efficacy of the ablation agent at the renal ganglion **24** may be determined based on measured changes in the physiological parameter(s). Suitable apparatuses for these purposes are disclosed in commonly owned U.S. Patent Publication No. 2008/0234780 and in U.S. Pat. No. 6,978,174, which are incorporated herein by reference.

It is noted that marker bands can be placed on one or multiple parts of the catheter **105** and/or **101** to enable visualization during the delivery, imaging, and/or denervation procedures. The marker bands may be solid or split bands of platinum or other radiopaque metal, for example.

Referring now to FIG. **20**, a catheter **51** to which an ultrasound unit **50** of the present invention is connected may incorporate a hinge mechanism **356** built into the catheter **51** proximate the ultrasound unit **50**. The hinge mechanism **356** may be built into other elongated intravascular device embodiments of the disclosure, such as shaft **67** and shaft **88** of balloons **64** shown in FIGS. **8-11**, respectively. The hinge mechanism **356** is constructed to enhance user manipulation

of the catheter **51** when navigating around a nearly 90 degree turn from the abdominal aorta into the renal artery. It is understood that one or more hinge mechanisms **356** may be built into other catheters and sheaths that may be used to facilitate access to the renal artery via the abdominal aorta. For example, a delivery sheath or guide catheter that is used to provide renal artery access for a catheter **51** of a type described herein may incorporate one or more hinge mechanisms **356**.

FIG. **20** illustrates a portion of the catheter **51** that incorporates a hinge mechanism **356** in accordance with embodiments of the invention. The hinge mechanism **356** is provided at a location of the catheter **51** between a proximal section **352** and a distal section **354** of the catheter's shaft. The hinge mechanism **356** is preferably situated near the proximal section of the ultrasound unit **50**. According to various embodiments, the hinge mechanism **356** comprises a slotted tube arrangement that is configured to provide a flexible hinge point of the catheter's shaft proximate the ultrasound unit **50**.

The catheter's shaft may be formed to include an elongate core member **357** and a tubular member **353** disposed about a portion of the core member **357**. The tubular member **353** may have a plurality of slots **361** formed therein. The slotted hinge region **356** of the catheter's shaft may be configured to have a preferential bending direction.

For example, the tubular member **352** may have a plurality of slots **361** that are formed by making a pair of cuts into the wall of tubular member **361** that originate from opposite sides of tubular member **353**, producing a lattice region of greater flexibility relative to the proximal and distal sections **352**, **354** of the catheter's shaft. The thickness of the catheter wall at the hinge region **356** can be varied so that one side of the catheter wall is thicker than the opposite side. This difference in wall thickness alone (e.g., a hinge region devoid of slots) or in combination with a difference in slot (void) density at the hinge region **356** provides for a preferential bending direction of the distal portion of the catheter **51**.

A hinge arrangement **356** constructed to provide for a preferential bending direction allows a physician to more easily and safely navigate the ultrasound unit **50** to make the near 90 degree turn into the renal artery from the abdominal aorta, for example. One or more marker bands may be incorporated at the hinge region **356** to provide visualization of this region of the catheter's shaft during deployment. Details of useful hinge arrangements that can be incorporated into embodiments of a catheter **51** of the present invention or other component that facilitates access to the renal artery/vein from the abdominal aorta are disclosed in U.S. Patent Publication Nos. 2008/0021408 and 2009/0043372, which are incorporated herein by reference. It is noted that the catheter **51** may incorporate a steering mechanism in addition to, or exclusion of, a hinge arrangement **356**. Known steering mechanisms incorporated into steerable guide catheters may be incorporated in various embodiments of a catheter **51** of the present invention.

The discussion provided herein concerning degrees of induced renal nerve damage, temperature ranges, amount of energy delivered into target tissue, and other embodiment details presented in this disclosure are provided for non-limiting illustrative purposes. Actual therapeutic parameters associated with the denervation apparatuses and methodologies may vary somewhat or significantly from those described herein, and be impacted by a number of factors, including patient-specific factors (e.g., the patient's unique renal vasculature and sympathetic nervous system characteristics), refractoriness to drugs impacting renal function, type and technology of the therapy device(s), therapy duration and

frequency, use of a single therapy device or multiplicity of therapy devices (in sequential or concurrent use), structural characteristics of the therapy device(s) employed, and other implementation and physiologic particulars, among others.

The foregoing description of the various embodiments of the invention has been presented for the purposes of illustration and description. It is not intended to be exhaustive or to limit the invention to the precise form disclosed. Many modifications and variations are possible in light of the above teaching. For example, the devices and techniques disclosed herein may be employed in vasculature of the body other than renal vasculature, such as coronary and peripheral vessels and structures. By way of further example, embodiments of an ultrasonic denervation unit may be implemented for chronic use, and structures other than a catheter, such as a stent, may be used to maintain positioning of the ultrasonic denervation unit within the renal artery or other vessel. It is intended that the scope of the invention be limited not by this detailed description, but rather by the claims appended hereto.

What is claimed is:

1. An apparatus, comprising:
 - a first catheter including a central shaft and an inflatable balloon, the first catheter configured for deployment within a vessel proximate innervated tissue that contributes to renal sympathetic nerve activity;
 - a second catheter slidable relative to the first catheter;
 - a spiral rail mounted on an outer surface of the central shaft adjacent a distal end of the central shaft within an interior volume of the inflatable balloon;
 - an acoustic transducer provided at the distal end of the second catheter and dimensioned for deployment within the vessel proximate the innervated tissue, wherein the second catheter includes a keyed channel member that is disposed around an outer surface of the spiral rail such that the acoustic transducer is translated along a helical path as the acoustic transducer is distally advanced or proximally retracted;
 - a focusing arrangement configured to focus acoustic energy outwardly beyond an inner wall of the vessel and into the innervated tissue at or proximate an outer wall of the vessel; and
 - a controller configured to control the acoustic transducer for at least one of scanning tissue and ablating the innervated tissue.
2. The apparatus of claim 1, wherein the controller is configured to control the acoustic transducer to selectively scan tissue and ablate the innervated tissue.
3. The apparatus of claim 1, wherein the acoustic transducer comprises an acoustic phased array transducer, the phased array transducer comprising:
 - a plurality of acoustic elements; and
 - driver electronics coupled to the acoustic elements;
 further wherein the controller is coupled to the driver electronics and configured to control activation of each of the acoustic elements of the phased array transducer for at least one of scanning tissue and ablating the innervated tissue.

4. The apparatus of claim 3, wherein the controller is configured to control activation of the acoustic elements of the phased array transducer for selectively scanning tissue and ablating the innervated tissue.

5. The apparatus of claim 1, wherein the acoustic transducer comprises a high-intensity focused ultrasound (HIFU) transducer.

6. The apparatus of claim 1, wherein the acoustic transducer comprises a linear phased array transducer.

7. The apparatus of claim 1, wherein the acoustic transducer comprises a curvilinear or a convex sector phased array transducer.

8. The apparatus of claim 1, wherein:

the acoustic transducer comprises an acoustic phased array transducer; and

the controller is configured to electronically adjust a focal length of the phased array transducer consistent with a distance between the phased array transducer and the innervated tissue.

9. The apparatus of claim 1, wherein the acoustic transducer and focusing arrangement cooperate to focus acoustic energy at foci at a desired depth within the innervated tissue of sufficient intensity to ablate the innervated tissue while negligibly injuring inner wall tissue of the vessel.

10. The apparatus of claim 1, wherein the acoustic transducer and focusing arrangement cooperate to focus acoustic energy at foci of spherical or cylindrical geometries at a desired depth within the innervated tissue in each of a first mode and a second mode, the first mode associated with acoustic energy of an intensity for scanning innervated tissue, and the second mode associated with acoustic energy of an intensity for ablating the innervated tissue.

11. The apparatus of claim 1, wherein the acoustic transducer is configured to generate an acoustic power level corresponding to focal peak intensities equal to or greater than about 2000 W/cm² in the innervated tissue.

12. The apparatus of claim 1, wherein the acoustic transducer is configured for high intensity focused ultrasound operation in a cavitation ablation mode that produces bubbles within the innervated tissue that work to mechanically disrupt nerve fibers and ganglia included within the innervated tissue upon bursting.

13. The apparatus of claim 1, wherein the inflatable balloon is configured to receive a liquid that provides good acoustic coupling between the acoustic transducer and a wall of the balloon.

14. The apparatus of claim 1, wherein the inflatable balloon is configured to facilitate cooling of an inner wall of the vessel by one or both of a blood perfusion arrangement or an arrangement for receiving a thermal transfer fluid.

15. The apparatus of claim 1, wherein the keyed channel member is keyed with the spiral rail.

16. The apparatus of claim 1, wherein the keyed channel member captures the spiral rail.

17. The apparatus of claim 1, wherein the keyed channel member supports the acoustic transducer.

18. The apparatus of claim 1, wherein the keyed channel member is attached to the acoustic transducer.

* * * * *

专利名称(译)	聚焦超声肾脏去神经支配		
公开(公告)号	US9192790	公开(公告)日	2015-11-24
申请号	US13/086116	申请日	2011-04-13
[标]申请(专利权)人(译)	黑斯廷斯ROGER SHUROS ALLANÇ 英格尔FRANK 霍林斯沃思MARK		
申请(专利权)人(译)	黑斯廷斯ROGER SHUROS ALLANÇ 英格尔FRANK 霍林斯沃思MARK		
当前申请(专利权)人(译)	BOSTON SCIENTIFIC SCIMED , INC.		
[标]发明人	HASTINGS ROGER SHUROS ALLAN C INGLE FRANK HOLLINGSWORTH MARK A		
发明人	HASTINGS, ROGER SHUROS, ALLAN C. INGLE, FRANK HOLLINGSWORTH, MARK A.		
IPC分类号	A61B8/00 A61B8/12 A61B8/08 A61N7/02 A61B18/02 A61B19/00 A61N7/00 A61B18/00		
CPC分类号	A61N7/022 A61B8/0891 A61B8/12 A61B8/4488 A61B18/0206 A61B2018/00404 A61B2018/00434 A61B2018/00511 A61B2019/528 A61N2007/003 A61N2007/0095 A61B2090/3784		
优先权	61/324164 2010-04-14 US		
其他公开文献	US20110257523A1		
外部链接	Espacenet USPTO		

摘要(译)

声能被传递到神经支配的血管，其促成肾交感神经活动，例如肾动脉和腹主动脉的神经支配组织。通过具有足够功率的血管内装置递送聚焦声能以消融神经支配的肾或主动脉组织。可以通过血管内或体外装置递送聚焦声能以对目标神经支配的肾或主动脉组织进行成像和定位。血管内，血管外或经血管聚焦超声装置提供神经支配血管的高精度去神经支配以终止肾交感神经活动。

