





US 20140039318A1

(19) **United States**(12) **Patent Application Publication**  
**Zhang et al.**(10) **Pub. No.: US 2014/0039318 A1**(43) **Pub. Date: Feb. 6, 2014**(54) **AUTOMATED DETECTION OF SUSPECTED  
ABNORMALITIES IN ULTRASOUND  
BREAST IMAGES**(71) Applicants: **Wei Zhang**, San Jose, CA (US);  
**Shih-Ping Wang**, Los Altos, CA (US);  
**Alexander Schneider**, Los Altos, CA  
(US); **Nico Karssemeijer**,  
Beek-Ubbergen (NL)(72) Inventors: **Wei Zhang**, San Jose, CA (US);  
**Shih-Ping Wang**, Los Altos, CA (US);  
**Alexander Schneider**, Los Altos, CA  
(US); **Nico Karssemeijer**,  
Beek-Ubbergen (NL)(73) Assignee: **QVIEW, INC.**, Los Altos, CA (US)(21) Appl. No.: **14/044,842**(22) Filed: **Oct. 2, 2013****Related U.S. Application Data**(63) Continuation-in-part of application No. 12/839,371,  
filed on Jul. 19, 2010, Continuation-in-part of applica-  
tion No. PCT/US2009/066020, filed on Nov. 27, 2009.(60) Provisional application No. 61/860,900, filed on Jul.  
31, 2013, provisional application No. 61/830,241,  
filed on Jun. 3, 2013, provisional application No.  
61/728,166, filed on Nov. 19, 2012, provisional applica-  
tion No. 61/709,136, filed on Oct. 2, 2012.**Publication Classification**(51) **Int. Cl.**  
**A61B 8/08** (2006.01)  
(52) **U.S. Cl.**  
CPC ..... **A61B 8/0825** (2013.01); **A61B 8/5238**  
(2013.01)  
USPC ..... **600/443**(57) **ABSTRACT**

A method and system for processing and displaying breast ultrasound information is described. A 2D feature weighted volumetric coronal image as a “guide” or “road map” is generated from the 3D ultrasound data volume to represent the 3D dataset with the goal of emphasizing abnormalities within the breast while excluding non-breast structures, particularly those external to the breast such as ribs and chest wall.

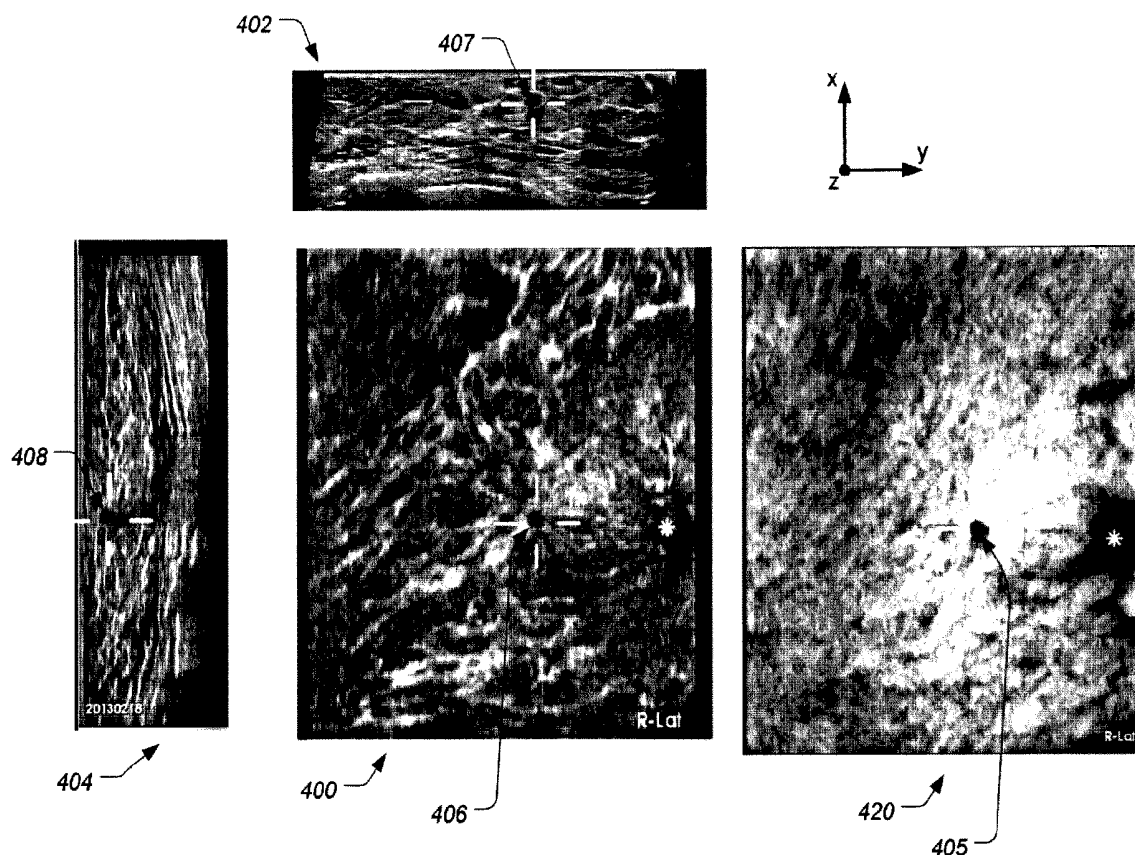

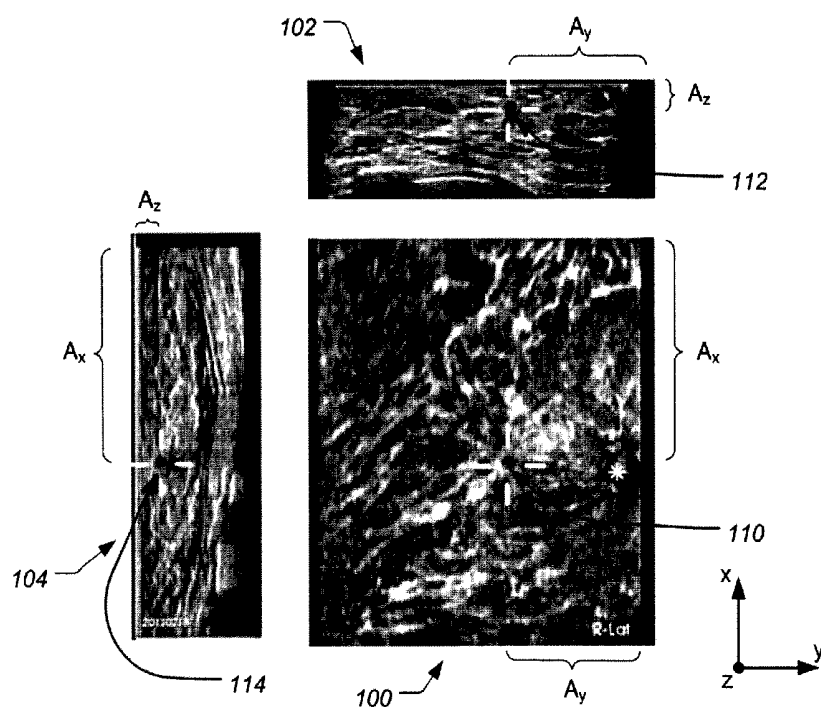

*Fig. 1*  
(Prior Art)



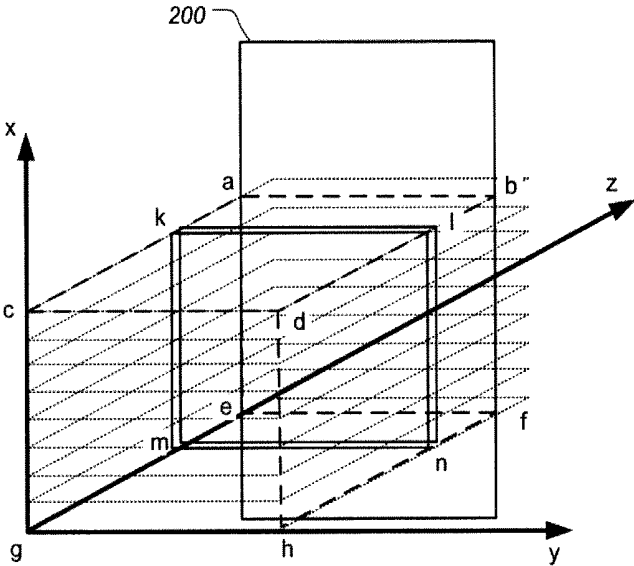


Fig. 2

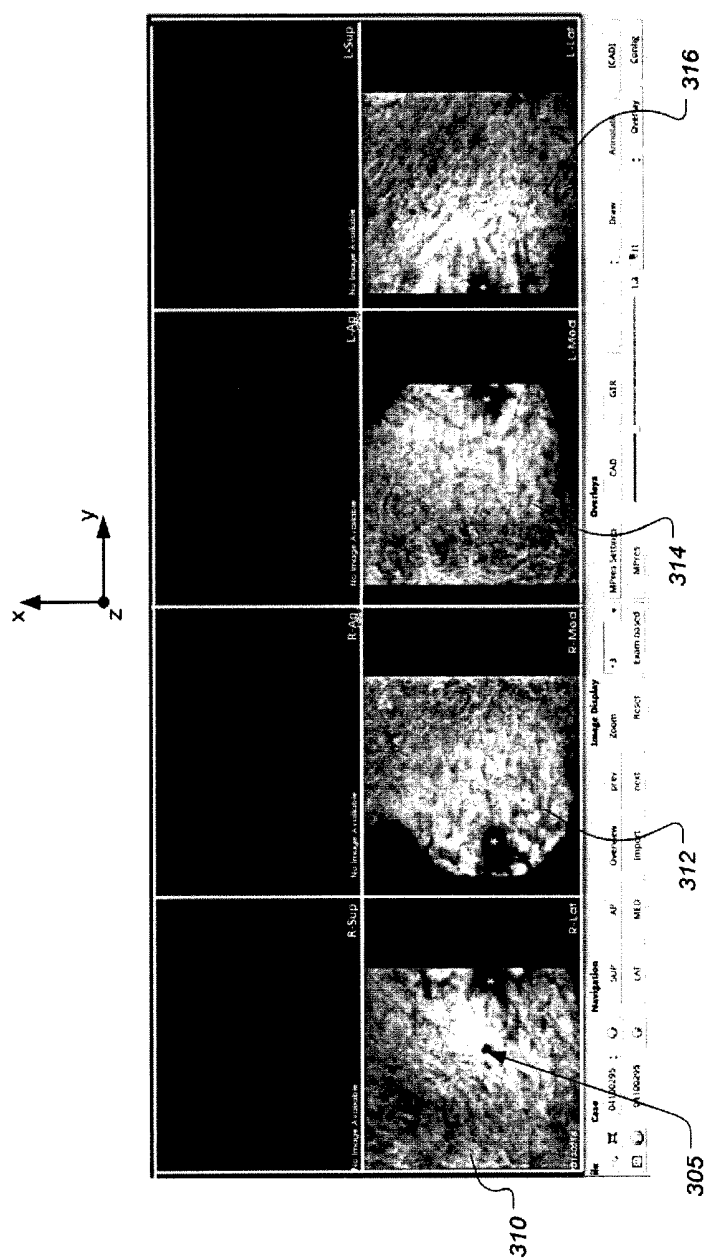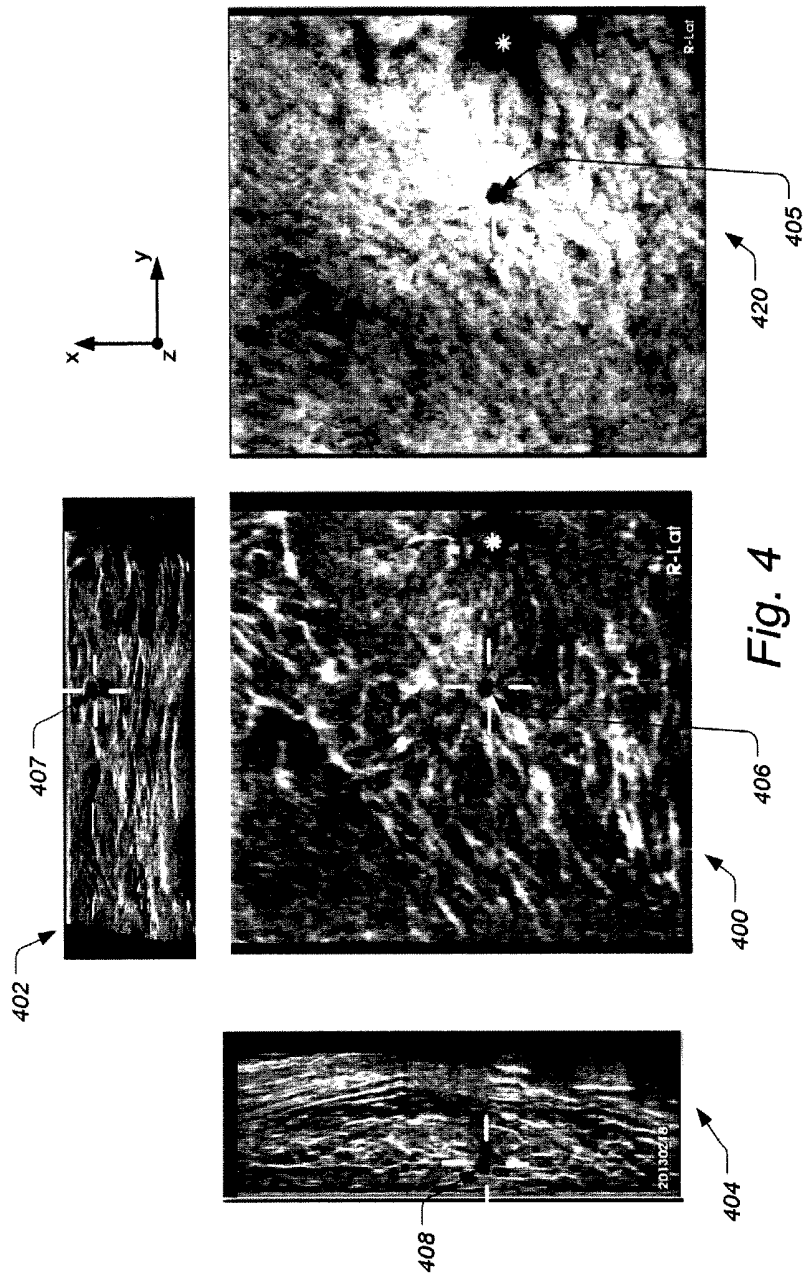

**Fig. 3**



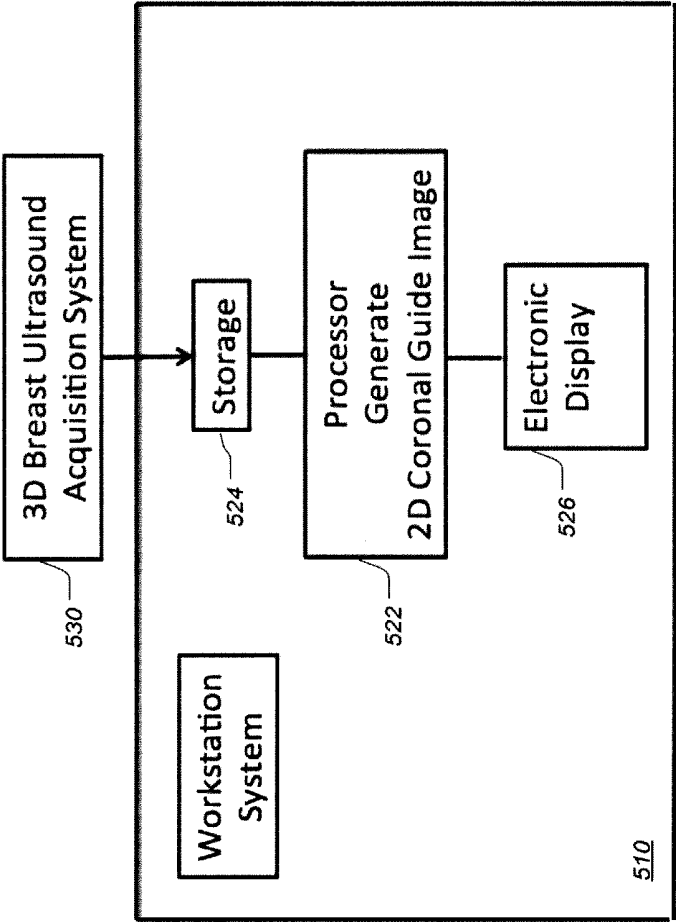
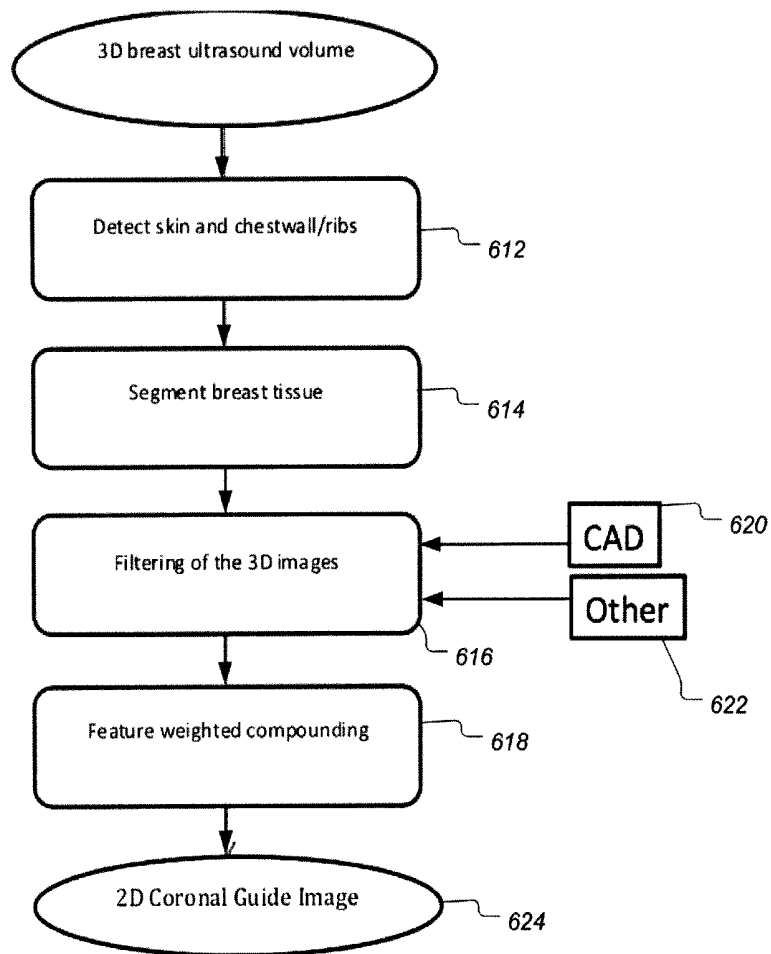


Fig. 5

*Fig. 6*

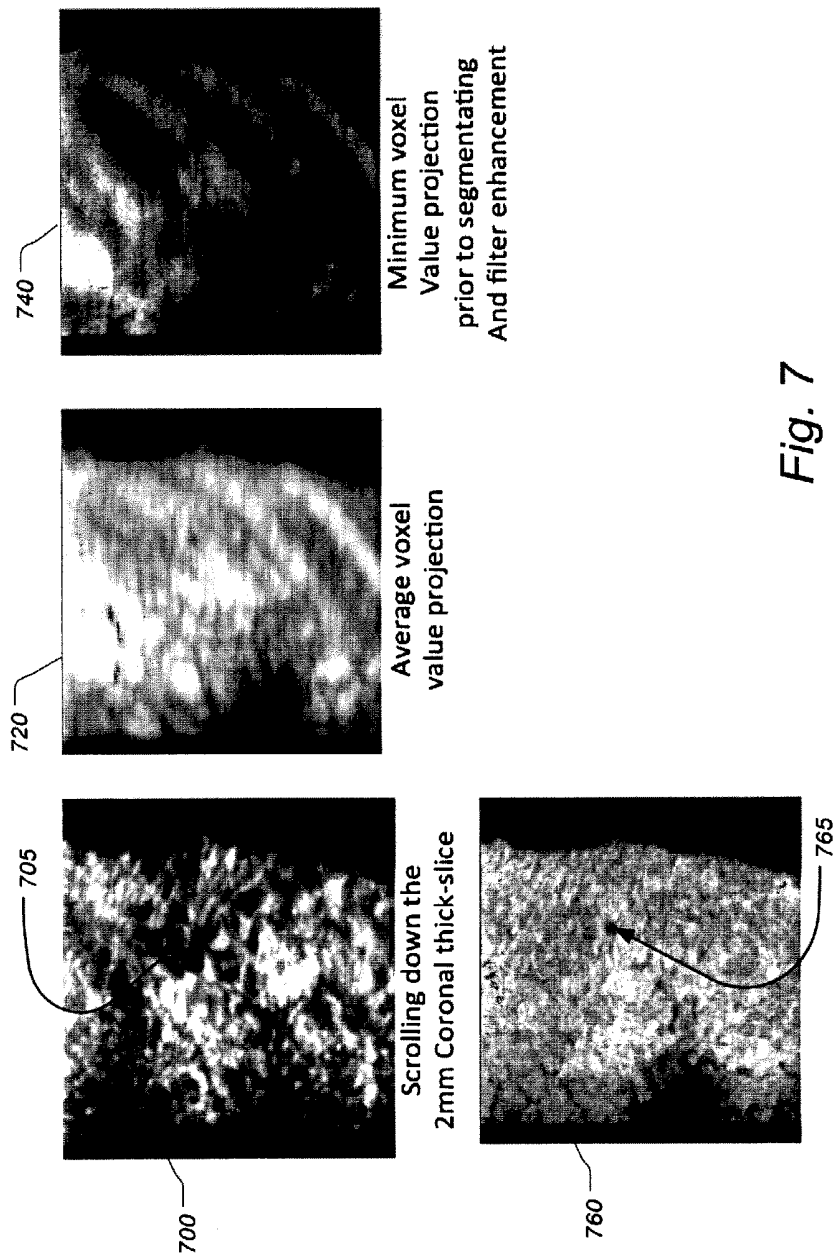
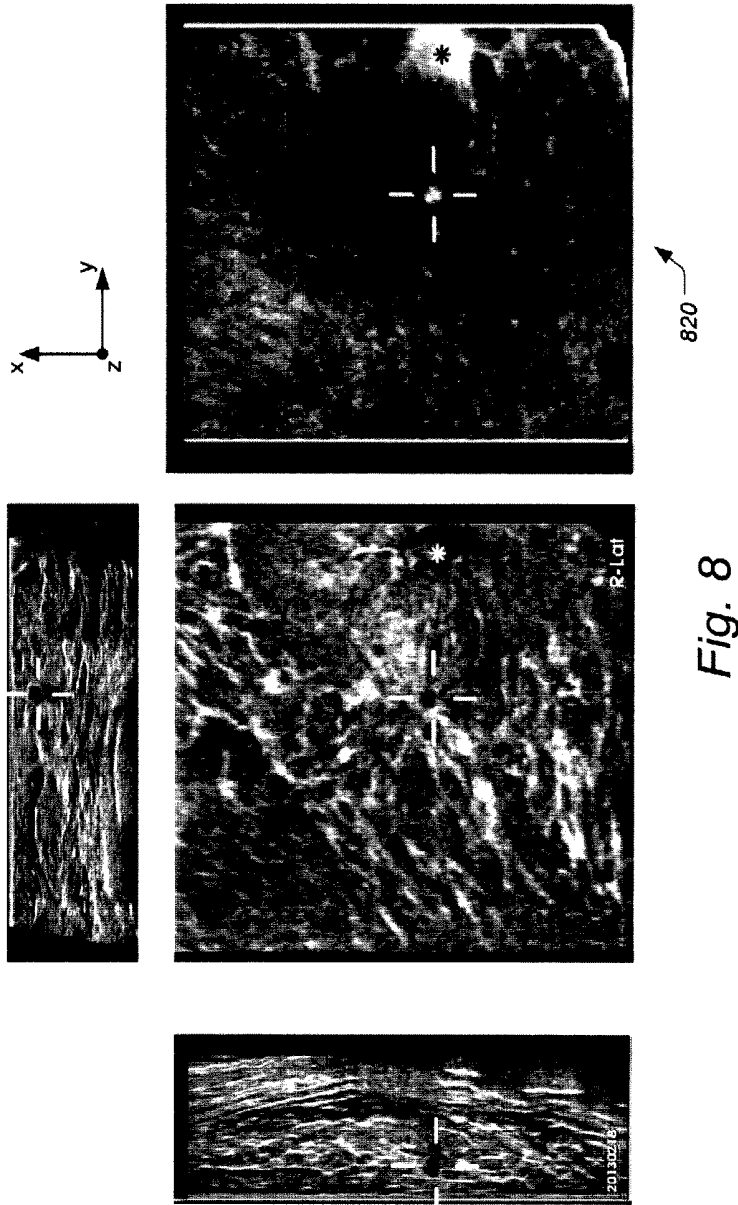


Fig. 7



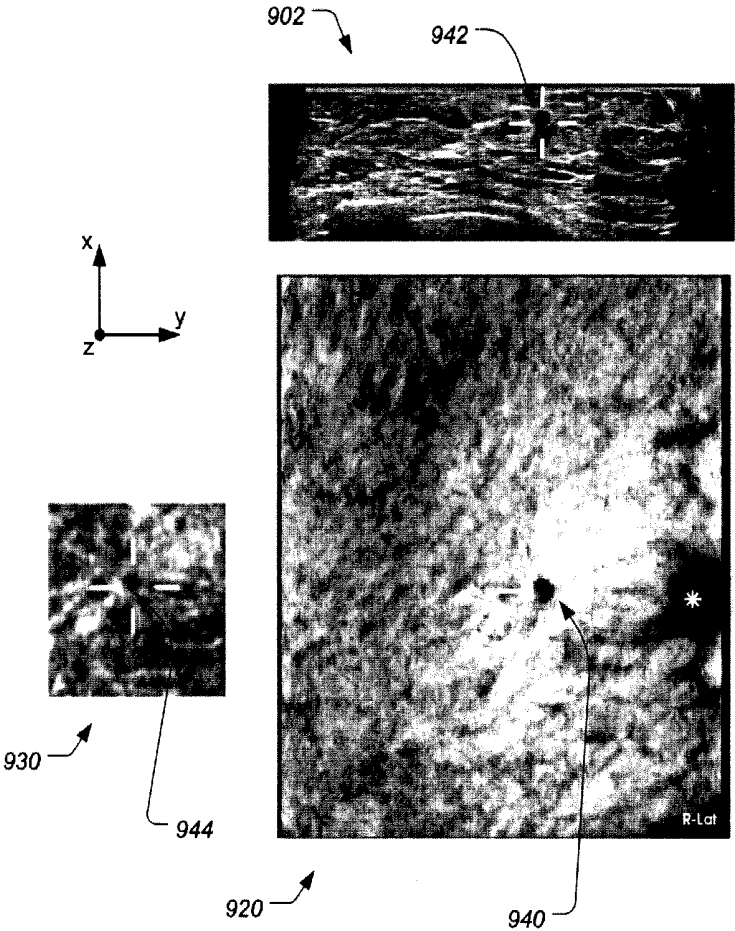


Fig. 9

## **AUTOMATED DETECTION OF SUSPECTED ABNORMALITIES IN ULTRASOUND BREAST IMAGES**

### **REFERENCE TO RELATED APPLICATIONS**

[0001] This patent application claims the benefit of and incorporates by reference each of the following applications:

[0002] U.S. Prov. Ser. No. 61/709/136 filed Oct. 2, 2012;

[0003] U.S. Prov. Ser. No. 61/728,166 filed on Nov. 19, 2012;

[0004] U.S. Prov. Ser. No. 61/830,241 filed on Jun. 3, 2013; and

[0005] U.S. Prov. Ser. No. 61/860,900 filed on Jul. 31, 2013.

[0006] This application is a continuation-in-part of and incorporated by reference each of the following applications:

[0007] U.S. Ser. No. 2012/0014578 filed on Jul. 19, 2010; and

[0008] International Patent Application No. WO 2011/065950 A1 filed on Nov. 27, 2009.

### **FIELD**

[0009] The method and system described in this patent specification relate to displaying 3D breast ultrasound images and other information in a manner believed to better assist their reading and interpretation by physicians or other users of the method and system. More specifically, the patent specification relates to a method and system of displaying a feature weighted volumetric 2D coronal image as a “guide” for users to find abnormalities in 3D breast ultrasound images more quickly and with less errors, in accordance with the method and system described herein.

### **BACKGROUND**

[0010] This invention is in the field of early detection of breast cancer. In the US, the expected statistical figures for breast cancer in 2013 are: approximately 230,000 new cases and 40,000 deaths. The mortality rate would be lowered if breast cancers could be detected in the earlier stage. Screening with X-ray mammography has been the gold standard for the early detection of breast cancer. However, in about 40% of the screening population, where the women have more than 50% of their breasts covered by dense fibro-glandular breast tissues, X-ray mammography has been found to be inadequate in depicting regions of breast covered by the dense breast tissues. Recent clinical studies show that breast ultrasound could be very effective for breasts with dense tissues, particularly automated 3D breast ultrasound. Currently, the only breast ultrasound system that received USFDA approval for breast cancer screening so far is an automated 3D breast ultrasound system using a chestward compression scanning procedure.

[0011] The subject matter claimed herein is not limited to embodiments that solve any disadvantages or that operate only in environments such as those described above. Rather, this background is only provided to illustrate one exemplary technology area where some embodiments described herein may be practiced.

### **SUMMARY**

[0012] According to some embodiments, a computer workstation system is described for ultrasound examination of a patient's breast. The system includes: a storage system for an

image dataset in the form of a plurality of two-dimensional scan images representative of a chestwardly compressed breast sonographically scanned using an automated three-dimensional breast ultrasound acquisition system; a processor configured to: (a) generate a three-dimensional volumetric dataset based on said image dataset; (b) segment and filter said three-dimensional volumetric dataset; and (c) generate a two-dimensional coronal guide image based on the segmented and filtered three-dimensional volumetric dataset, wherein said two-dimensional guide image includes visually enhanced suspected abnormalities within said segmented and filtered three-dimensional volumetric dataset if present in the breast; and an interactive user interface configured to: (a) electronically display to a user said coronal guide image; (b) receive user input indicating a user's selection of a suspected abnormality; and (c) in response to the user's selection displaying one or more of the plurality of two-dimensional scan images corresponding to the selected suspected abnormality.

[0013] According to some embodiments, a method and system for processing and displaying breast ultrasound information is provided, wherein a 2D feature weighted volumetric coronal image as a “guide” or “road map” is generated from the 3D ultrasound data volume to represent the 3D dataset with the goal of emphasizing abnormalities within the breast while excluding non-breast structures, particularly those external to the breast such as ribs and chest wall, in accordance with the method and system described herein.

[0014] In one preferred embodiment, the 2D feature weighted volumetric guide is displayed in the form of a 2D coronal guide image together with a display as in current commercial automated 3D breast ultrasound systems employing chestward compression scans, where a 2D original axial scan image, and a 2D orthogonal (constructed to be orthogonal to the axial scan) image are displayed with the composite 2D coronal thick-slice image(s). By clicking any exhibited abnormality in the 2D feature weighted volumetric coronal guide, with pre-calculated xyz coordinates, the corresponding abnormality can show up in the 2D coronal thick-slice image as well as at the corresponding locations in the 2D original axial scan image and the orthogonal sagittal image.

[0015] In another preferred embodiment, the 2D coronal guide image is displayed together with just the 2D original axial scan image for the quickest review and a snippet of one or more 2D coronal thick-slices. It is sometimes useful to show the coronal thick-slice image, because readers would like to confirm their assessment by examining the presence of spiculations of a mass nodule that only show in composite coronal thick-slices. The quick review of the 2D axial scan images is done in the manner described above.

[0016] In yet another preferred embodiment, the 2D coronal guide image is displayed in inverted polarity. That is, in regular guides, the abnormalities are dark colored on relatively light breast tissue background, and in the inverted polarity guides, the abnormalities are light colored on a relatively dark breast tissue background. A reason is that some readers prefer to read the inverted polarity guides, which resemble mammograms (also with light colored abnormalities on a dark background).

[0017] In still another preferred embodiment, the 2D coronal guide image is generated through a process of segmenting away non-breast structure and using a filter to enhance the remaining volumetric breast tissue to make the abnormalities more visible and more prominent.

**[0018]** In yet another preferred embodiment, the filter includes a computer aided detection (CAD) algorithm that can detect and ranks the lesions by likelihood. This is particularly useful for very small abnormalities or lesions that show significant likelihood of being malignant by CAD and yet the above described filter may not be enough to make these small abnormalities visible or prominent in the 2D coronal guide image.

**[0019]** In still another preferred embodiment, additional information is shown with an abnormality such as its size, volume, relative probability, likelihood of being malignant, etc.

**[0020]** In another preferred embodiment, the 2D coronal guide image is displayed on a separate monitor situated adjacent to the display monitor of a commercial automated 3D breast ultrasound system.

**[0021]** In another preferred embodiment, the 2D coronal guide image is displayed on a separate sheet of paper to be viewed with the display monitor of a commercial automated 3D breast ultrasound system.

#### BRIEF DESCRIPTION OF THE DRAWINGS

**[0022]** To further clarify the above and other advantages and features of the subject matter of this patent specification, specific examples of embodiments thereof are illustrated in the appended drawings. It should be appreciated that these drawings depict only illustrative embodiments and are therefore not to be considered limiting of the scope of this patent specification or the appended claims. The subject matter hereof will be described and explained with additional specificity and detail through the use of the accompanying drawings in which:

**[0023]** FIG. 1 illustrates aspects of a known commercial system using a 2 mm thick coronal thick-slice as a road map;

**[0024]** FIG. 2 illustrates aspects of chestward compression scan orientation in relationship to a 2D coronal thick-slice according to prior art, as well as a volume from which a 2D coronal volumetric guide is derived, according to some embodiments;

**[0025]** FIG. 3 illustrates aspects of a start up screen with four coronal guide images, according to some embodiments;

**[0026]** FIG. 4 illustrates aspects of a displayed coronal guide image, an original 2D axial slice, an orthogonal 2D slice, and a coronal thick-slice, according to some embodiments;

**[0027]** FIG. 5 is a diagram illustrating aspects of a system for generating and displaying a two-dimensional coronal guide image, according to some embodiments;

**[0028]** FIG. 6 is a flow chart illustrating aspects of generating and displaying a two-dimensional coronal guide image, according to some embodiments;

**[0029]** FIG. 7 illustrates effects of segmenting non-breast structures and filter enhancement of a minimum voxel value projection; according to some embodiments;

**[0030]** FIG. 8 illustrates aspects of a displayed inverted coronal guide image along with an original 2D axial slice, an orthogonal 2D slice, and a coronal thick-slice, according to some embodiments; and

**[0031]** FIG. 9 illustrates aspects of a displayed coronal guide image along with an original 2D axial slice with a snippet of a coronal thick slice, according to some embodiments.

#### DETAILED DESCRIPTION

**[0032]** A detailed description of examples of preferred embodiments is provided below. While several embodiments are described, it should be understood that the new subject matter described in this patent specification is not limited to any one embodiment or combination of embodiments described herein, but instead encompasses numerous alternatives, modifications, and equivalents. In addition, while numerous specific details are set forth in the following description in order to provide a thorough understanding work, some embodiments can be practiced without some or all of these details. Moreover, for the purpose of clarity, certain technical material that is known in the related art has not been described in detail in order to avoid unnecessarily obscuring the new subject matter described herein. It should be clear that individual features of one or several of the specific embodiments described herein can be used in combination with features or other described embodiments. Further, like reference numbers and designations in the various drawings indicate like elements.

**[0033]** There are two major problems facing any practical breast cancer screening modality. The first major problem of breast cancer screening is the “cost”. Since breast cancer has a very low prevalence rate such that one cancer is generally found in 200 to 300 patients screened, the per patient screening cost must be kept low, typically to the range of \$100-\$200, in order to achieve a reasonable cost per cancer detected. This cost range is generally translated into limiting reading/interpretation time to about 3 minutes per patient and an automated scanning system with a throughput of over 2,000 patients per year. For screening X-ray mammography, where only 4 new images are generated per patient, this 3-minute interpretation time requirement is relatively easily met. However, for breast ultrasound screening, where over 1,200 to 3,000 new images are generated per patient, the 3 minutes of reading/interpretation time limit becomes a real challenge.

**[0034]** The second major problem of breast cancer screening is the “oversight”, where obvious cancers are overlooked during the reading/interpretation. The delay in the cancer detection due to oversight would generally cause the cancer to progress to a more advanced stage resulting in increases in treatment cost and decrease in patient survivability. This problem is particularly serious when trying to read/interpret quickly. In a study on blind re-reading by 5 breast radiologists of 427 prior screening mammograms, which were taken a year before the cancer detection, published in Radiology in 2000 (by Warren-Burhenne et al, Vol. 215, pages 554-562), reports that as many as 115 (or 27%) of these prior mammograms were detected by all 5 radiologists and thus should be classed as oversights. In order to reduce the oversight problem, commercial computer-aided diagnosis (CAD) systems have been developed for X-ray mammography screening. Development of clinically useful CAD was no trivial matter, as the CAD must achieve sensitivities close to that of human readers. The development was undertaken by several commercial firms, some in collaboration with universities and national laboratories, over many years and consumed over \$100 million in combined developmental cost. The CAD’s impact was clearly visible. After 10 years of its commercial introduction, as reported by a study published in JACR in 2010 (by Rao et al, Vol. 7, pages 802-805) that, by year 2008, 75% of the screening mammograms were read with CAD.

**[0035]** The commercial automated 3D breast ultrasound systems all perform chestward compression scans. That is,

the ultrasound beam is generally directed chestward during the scan while the breast is generally compressed chestward. This method has many advantages over the earlier non chestward-compressed ultrasound scanning methods such as the method that clamps the breast between a vise-like scanning plates, as in the case of mammography. Namely, the advantages are: patient comfort is much better, the breast tissue is thinner during the scan, and high higher ultrasound frequency could be employed resulting in much better image quality. This is chestward compressed scan method is described more in details in U.S. Pat. No. 7,828,733, which also taught the use of a composite 2D coronal thick-slice method that could be used as a guide or road map to aid the more rapid search for abnormalities. Instead of searching through 300 scanned 2D images in a typical scan of the breast, the reader now searches through far fewer coronal 2D thick-slice images. The coronal thick-slice thickness range was 2-20 mm as stated in the claims of U.S. Pat. No. 7,828,733, but the Figures (e.g. FIGS. 17, 18, 19, 20, 23, and 25) of U.S. Pat. No. 7,828,733 all showed thickness ranges of 6-8 mm as six such thick-slices were sufficient to cover the entire chestward compressed breast. This composite coronal thick-slice road map image has been proven to be very useful and is used in all current commercial automated 3D breast ultrasound systems. However, in all current commercial systems, the most popular coronal thick-slice thickness is in the range of 0.5 mm to 2 mm, resulting in 15 to 60 2D coronal thick-slice images per scan (or 3 to 10 fold increase in the number of 2D coronal thick-slice images as taught by U.S. Pat. No. 7,828,733). The reason for such thickness selection is better image quality and less chance to miss smaller lesions or abnormalities. There will be more discussions in the following parts of this specification on composite coronal thick-slice guide and its comparison with the present invention.

**[0036]** In commercial automated 3D breast ultrasound screening systems using chestward compression scans, for each patient, two to five scans would typically be made on each breast. Each typical scan would generate 300 new images. Thus, 1,200 to 3,000 new images total would typically be generated for each patient. With the 300 to 700 fold increase in the number of new images over screening mammography, one could see that efficient methods and systems must be developed to better manage both the reading/interpretation time as well as the oversight problems before breast ultrasound screening could be broadly employed. Indeed, since the worldwide commercial introduction of automated 3D breast ultrasound using chestward compression several years ago, radiologists at hundreds of facilities around the world have been struggling to read/interpret the huge volume of breast ultrasound images. At the present time, the best readers, even using the composite 2 mm coronal thick-slice image as a road map, could barely reach the 3 minutes limit per patient, while the majority of the readers are averaging more than 5 minutes per patient. There have been no published studies on the "oversight" in automated 3D breast ultrasound yet, but one could venture to guess that the oversight rate could not have been below that found for screening mammography, which is 27%. It is not a surprise that these readers have uniformly been, in the past years, asking researchers to develop some methods and/or systems that could both speed up the reading and reduce the oversight.

**[0037]** In view of the above, an interactive user interface method and system are described for viewing large number of new images within a time limit of 3 minutes and with low oversight.

**[0038]** FIG. 1 illustrates aspects of a known commercial system using a 2 mm thick coronal thick-slice as a road map. FIG. 1 illustrates a prior art road map in the form of currently used commercial "composite coronal thick-slice" method for the reading/interpreting of the 3D breast ultrasound images.

**[0039]** FIG. 1 illustrates a prior art road map in the form of currently used commercial "composite coronal thick-slice" method for the reading/interpreting of the 3D breast ultrasound images. The current commercial automated 3D breast ultrasound systems typically use a thick-slice **100** having a thickness of 2 mm (range around 0.5 to 2 mm), although the U.S. Pat. No. 7,828,733 discussed a range of 2-20 mm when first filed in 2004. Moving to thinner and thinner thickness with commercial systems means that readers must search through more thick slices, e.g., 20 to 30 composite coronal thick-slices per scan currently, although it can be a 10x reduction of search volume vs. the raw 2D axial scan images. In the meantime, readers at hundreds of facilities may still struggle to reach the 3-minute read time limit. In contrast to that, this patent specification teaches a method and a system in which only one composite coronal guide image for each scan can be sufficient. Most of the scans actually show no abnormalities resulting in substantial decrease in the read time. With the addition of CAD, the oversight problem for ultrasound breast imaging should also be reduced. Also shown in FIG. 1 is the original axial 2D image **102** and constructed orthogonal 2D image **104**. After searching through many 2D coronal images such as **100**, the user finds abnormality **110** in image **100**. Clicking on abnormality **110** in image **100** (with a location of  $A_x, A_y, A_z$ ), automatically brings up corresponding abnormalities **112** and **114** in images **102** and **104** respectively.

**[0040]** FIG. 2 illustrates aspects of chestward compression scan orientation in relationship to a 2D coronal thick-slice according to prior art, as well as a volume from which a 2D coronal volumetric guide is derived, according to some embodiments. FIG. 2 illustrates chestward compression scan orientation in relationship to a 2D coronal thick-slice guide (k,l,m,n) and the volume (a,b,c,d,e,f,g,h) from which the 2D coronal volumetric guide is derived. Chestwall **200** is shown. The planes a,b,c,d to e,f,g,h are the original axial scanned images.

**[0041]** FIG. 3 illustrates aspects of a start up screen with four coronal guide images, according to some embodiments. FIG. 3 illustrates a typical startup screen of the workstation after a patient scan by the automated 3D ultrasound breast system, which screen shows a set of coronal guide images, one corresponds to each scan. Although in this patient there are only 2 scans per breast, current commercial systems may take up to 5 scans per breast. The most prominent abnormality is on the R-Lat coronal guide image.

**[0042]** FIG. 3 illustrates a typical startup screen of the workstation after a patient scan by an automated 3D ultrasound breast system, which shows a set of coronal guide images **310**, **312**, **314** and **316**, with one guide image corresponding to each scan. Although there could be 5 scans per breast, FIG. 3 shows just 2 scans per breast for this patient. The most prominent abnormality, **305**, is on the R-Lat coronal guide image.

**[0043]** FIG. 4 illustrates aspects of a displayed coronal guide image, an original 2D axial slice, an orthogonal 2D slice, and a coronal thick-slice, according to some embodiments. FIG. 4 illustrates a screen resulting after clicking the prominent abnormality **405** in the R-Lat coronal guide image **420**. Since the xyz coordinates have been previously com-

puted, the click on **405** immediately brings up the corresponding abnormality **406** in 2-D coronal thick-slice **400**. Also, the corresponding abnormality **407** in the axial image **402** as well as abnormality **408** in the orthogonal image **404**. X-direction is the axial direction, usually parallel to the patient's head-to-toe direction, and is also the direction of the linear ultrasound scanning. Y-direction is parallel to the patient's left-right direction. Z-direction is the chestward direction. The reader, in most cases a radiologist, can quickly review the 2D axial scan images by activating the scroll bar in the guide and scroll through the axial images. Likewise, the orthogonal images can be reviewed quickly by activating the corresponding scroll bar. A blank coronal guide image can mean the absence of any significant or prominent abnormalities in the guide image and the associated 3D breast volume.

[0044] FIG. 4 illustrates what happens after clicking the prominent abnormality in the R-Lat coronal guide image. Since the xyz coordinates have been previously computed, the click immediately brings up the corresponding abnormality in the axial image as well as in the orthogonal image. X-direction is the axial direction, usually parallel to the patient's head-to-toe direction, and is also the direction of the linear ultrasound scanning. Y-direction is parallel to the patient's left-right direction. Z-direction is the chestward direction. The reader, in most cases a radiologist, can quickly review the 2D axial scan images by activating the scroll bar in the guide and scroll through the axial images. Likewise, the orthogonal images can be reviewed quickly by activating the corresponding scroll bar. A blank coronal guide image can mean the absence of any significant or prominent abnormalities in the guide image and the associated 3D breast volume.

[0045] FIG. 5 is a diagram illustrating aspects of a system for generating and displaying a two-dimensional coronal guide image, according to some embodiments. FIG. 5 illustrates a block diagram of a workstation system for the storage of data, processing to generate display the 2D Coronal guide image for the reading/interpreting of the 3D breast ultrasound images according to a preferred embodiment.

[0046] FIG. 5 illustrates in block diagram form a workstation system **510** for the storage of data and processing to generate display the 2D Coronal guide image for the reading/interpreting of the 3D breast ultrasound images according to a preferred embodiment. Shown in workstation **510** is storage **524**, processor **522** for generating 2-D coronal guide image, and a display **526**. Also shown the 3-D breast ultrasound acquisition system **530** as the source of 3D ultrasound data.

[0047] FIG. 6 is a flow chart illustrating aspects of generating and displaying a two-dimensional coronal guide image, according to some embodiments. FIG. 6 illustrates a process flow leading to the generation of the 2D Coronal guide image.

[0048] FIG. 6 illustrates a flow process in generating the 2D coronal guide image. The flowchart illustrates an algorithm that can be used in each module, such as breast tissue segmentation or chestwall/rib detection. First, in step **612**, the skin, chest-wall and ribs are detected. In step **614**, the region containing only breast tissue is segmented. Skin region can be simply defined as the region within certain distance range from the top, say 0 to 2 mm. In the Filtering step **616**, the 3D volume image is filtered by a group of filters that are designed to suppress noise and artifacts and enhance lesions. As an example, the filters can be a gradient conversion filter and a line conversion filter. The gradient conversion filter is designed to enhance the dark rounded shapes and the line conversion filter is designed to enhance lines radiating from a

center which resemble a speculation or architectural distortion. Another example of the filter can be a computer aided detection (CAD) algorithm **620** that can detects and rank the lesions by likelihood. Other filters **622** can be derived from techniques such as minimum voxel value, Doppler data, and/or elastography data.

[0049] The weights,  $w(x, y, z)$  for compounding are generated by combining the outputs of the filters.

$$w(x, y, z) = \sum_i^N k_i f_i(x, y, z)$$

Where N is the total number of filters,  $f_i(x, y, z)$  is the output of  $i$ th filter and  $k_i$  is a constant scaling factor for  $i$ th filter. The weight is also normalized from 0 to 1 as the probability of a voxel overlap with a cancer lesion.

[0050] The atlas image  $a(x, y)$  is generated by projecting the volumetric image along the z direction (excluding skin, chestwall and rib regions) modulated by the weight. The equation below shows one example of the projection by taking the minimum value of the weighted intensity along the z axis.

$$a(x, y) = \min_{\text{across } z} (I(x, y, z)(1 - w(x, y, z)))$$

Where  $I(x, y, z)$  is the intensity or voxel value of the 3D ultrasound volumetric image.

[0051] FIG. 7 illustrates effects of segmenting non-breast structures and filter enhancement of a minimum voxel value projection; according to some embodiments. FIG. 7 illustrates effects of segmenting and filter enhancement of coronal image.

[0052] FIG. 7 illustrates the profound effect of segmentation and filter enhancement of volumetric coronal image. **700** shows a 2 mm 2D coronal thick-slice image. After searching by scrolling through approximately 30 such images in the chestward (z-direction) direction, a cancer like abnormality **705** is found. **720** shows the volumetric compounding by showing the 2D coronal image of average voxel value projection average, by taking the average voxel value along the z direction (perpendicular to the coronal image plane and chestwall) of the breast. The cancer like abnormality is not visible in this image. **740** shows a similar projection along the z-direction using the minimum voxel value. Again, the cancer like abnormality is not visible. **760** shows the minimum voxel value volumetric projection after segmenting non-breast tissues and application of filter enhancement, which process has been described above. The cancer like abnormality **765** is now very visible.

[0053] FIG. 8 illustrates aspects of a displayed inverted coronal guide image along with an original 2D axial slice, an orthogonal 2D slice, and a coronal thick-slice, according to some embodiments. FIG. 8 illustrates a 2D coronal guide image **820** in reverse polarity, which some readers may prefer.

[0054] FIG. 9 illustrates aspects of a displayed coronal guide image along with an original 2D axial slice with a snippet of a coronal thick slice, according to some embodiments. FIG. 9 illustrates an example with fewer display components, including the 2D coronal guide, just one set of 2D images from the scan for review and scroll review, and a snippet or whole of the 2D coronal thick-slice. The display of the 2D coronal thick-slice may be useful because readers may like to confirm their assessment by examining the presence of

spiculations of the mass nodule which only show in the 2D composite coronal thick-slices.

[0055] FIG. 9 illustrates an example with fewer display components, including the 2D coronal guide 920, just one 2D image 902 from the scan for review and scroll review, and a snippet 930 or whole of the 2D coronal thick-slice. The display of the 2D coronal thick-slice may be useful because readers may like to confirm their assessment by examining the presence of spiculations of the mass nodule which only show in the 2D composite coronal thick-slices. Clicking the abnormality 940 in guide image 920 automatically brings up the corresponding abnormalities 942 and 944 in images 902 and snippet 930, respectively.

[0056] Although the foregoing has been described in some detail for purposes of clarity, it will be apparent that certain changes and modifications may be made without departing from the principles thereof. It should be noted that there are many alternative ways of implementing both the processes and apparatuses described herein, including for using the described devices or certain aspects thereof for hysteroscopy but not for endometrial biopsy, or for endometrial biopsy but not for hysteroscopy, or for endoscopy and/or biopsy other than of the uterus. For example, in some applications the device shown in FIGS. 50-51 could also be used for taking fluid and/or fluid/tissue endometrial samples through the forward facing fluid parts. Accordingly, the present embodiments are to be considered as illustrative and not restrictive, and the body of work described herein is not to be limited to

the details given herein, which may be modified within the scope and equivalents of the appended claims.

What is claimed is:

1. A computer workstation system for ultrasound examination of a patient's breast, comprising:
  - a storage system for an image dataset in the form of a plurality of two-dimensional scan images representative of a chestwardly compressed breast sonographically scanned using an automated three-dimensional breast ultrasound acquisition system;
  - a processor configured to: (a) generate a three-dimensional volumetric dataset based on said image dataset; (b) segment and filter said three-dimensional volumetric dataset; and (c) generate a two-dimensional coronal guide image based on the segmented and filtered three-dimensional volumetric dataset, wherein said two-dimensional guide image includes visually enhanced suspected abnormalities within said segmented and filtered three-dimensional volumetric dataset if present in the breast; and
  - an interactive user interface configured to: (a) electronically display to a user said coronal guide image; (b) receive user input indicating a user's selection of a suspected abnormality; and (c) in response to the user's selection displaying one or more of the plurality of two-dimensional scan images corresponding to the selected suspected abnormality.

\* \* \* \* \*

|                |                                                                                                          |         |            |
|----------------|----------------------------------------------------------------------------------------------------------|---------|------------|
| 专利名称(译)        | 自动检测超声乳房图像中的疑似异常                                                                                         |         |            |
| 公开(公告)号        | <a href="#">US20140039318A1</a>                                                                          | 公开(公告)日 | 2014-02-06 |
| 申请号            | US14/044842                                                                                              | 申请日     | 2013-10-02 |
| [标]申请(专利权)人(译) | 张伟<br>王师PING<br>SCHNEIDER ALEXANDER<br>KARSSEMEIJER NICO                                                 |         |            |
| 申请(专利权)人(译)    | 张伟<br>王，施平<br>SCHNEIDER，ALEXANDER<br>KARSSEMEIJER，NICO                                                   |         |            |
| 当前申请(专利权)人(译)  | QVIEW，医疗INC                                                                                              |         |            |
| [标]发明人         | ZHANG WEI<br>WANG SHIH PING<br>SCHNEIDER ALEXANDER<br>KARSSEMEIJER NICO                                  |         |            |
| 发明人            | ZHANG, WEI<br>WANG, SHIH-PING<br>SCHNEIDER, ALEXANDER<br>KARSSEMEIJER, NICO                              |         |            |
| IPC分类号         | A61B8/08                                                                                                 |         |            |
| CPC分类号         | A61B8/5238 A61B8/0825 G06T7/0012 G06T2207/10132 G06T2207/30068                                           |         |            |
| 优先权            | 61/830241 2013-06-03 US<br>61/709136 2012-10-02 US<br>61/860900 2013-07-31 US<br>61/728166 2012-11-19 US |         |            |
| 其他公开文献         | US9826958                                                                                                |         |            |
| 外部链接           | <a href="#">Espacenet</a> <a href="#">USPTO</a>                                                          |         |            |

#### 摘要(译)

描述了一种用于处理和显示乳房超声信息的方法和系统。从3D超声数据体积生成2D特征加权体积冠状图像作为“指南”或“道路地图”以表示3D数据集，目的是强调乳房内的异常，同时排除非乳房结构，特别是外部的胸部如肋骨和胸壁。

