



US006743176B2

(12) **United States Patent**
Kato

(10) **Patent No.:** **US 6,743,176 B2**
(45) **Date of Patent:** **Jun. 1, 2004**

(54) **ULTRASONIC IMAGE DISPLAY APPARATUS
AND ULTRASONIC IMAGE DISPLAY
METHOD**

(75) Inventor: **Sei Kato**, Tokyo (JP)

(73) Assignee: **GE Medical Systems Global
Technology Company, LLC**,
Waukesha, WI (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 0 days.

(21) Appl. No.: **10/417,482**

(22) Filed: **Apr. 17, 2003**

(65) **Prior Publication Data**

US 2003/0199766 A1 Oct. 23, 2003

(30) **Foreign Application Priority Data**

Apr. 18, 2002 (JP) 2002-115973

(51) Int. Cl.⁷ **A61B 8/00**

(52) U.S. Cl. **600/440**

(58) Field of Search 600/437, 440-441,
600/443, 447; 382/132

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,773,425 A * 9/1988 Saitou 600/440

4,787,393 A * 11/1988 Fukukita et al. 600/440
5,182,728 A * 1/1993 Shen et al. 367/7
5,250,933 A 10/1993 Beaudin et al.
5,274,759 A 12/1993 Yoshioka
5,367,318 A 11/1994 Beaudin et al.
5,740,267 A * 4/1998 Echerer et al. 382/132
5,840,034 A 11/1998 Amemiya et al.
6,084,565 A * 7/2000 Kiya 345/115
6,139,497 A 10/2000 Amemiya et al.
6,217,515 B1 4/2001 Yamakawa et al.

* cited by examiner

Primary Examiner—Francis J. Jaworski

(74) *Attorney, Agent, or Firm*—Carl B. Horton, Esq.;
Armstrong Teasdale LLP

(57) **ABSTRACT**

For the purpose of improving monitor display condition operating ease and enabling easy display of an arbitrary site, an ultrasonic image based on an echo signal received by an ultrasonic probe **3** is produced by an image producing section **12**, a display area is formed on a screen by a display area forming section **17**, a displayed range of the ultrasonic image to be displayed in the display area is selected by a displayed range selecting section **14**, and scrolling of a selected range and rotation of the displayed range are achieved by a displayed range moving section **15** and a displayed range rotating section **16**, respectively, based on a position on the monitor screen specified by the pointing device **3**.

20 Claims, 13 Drawing Sheets

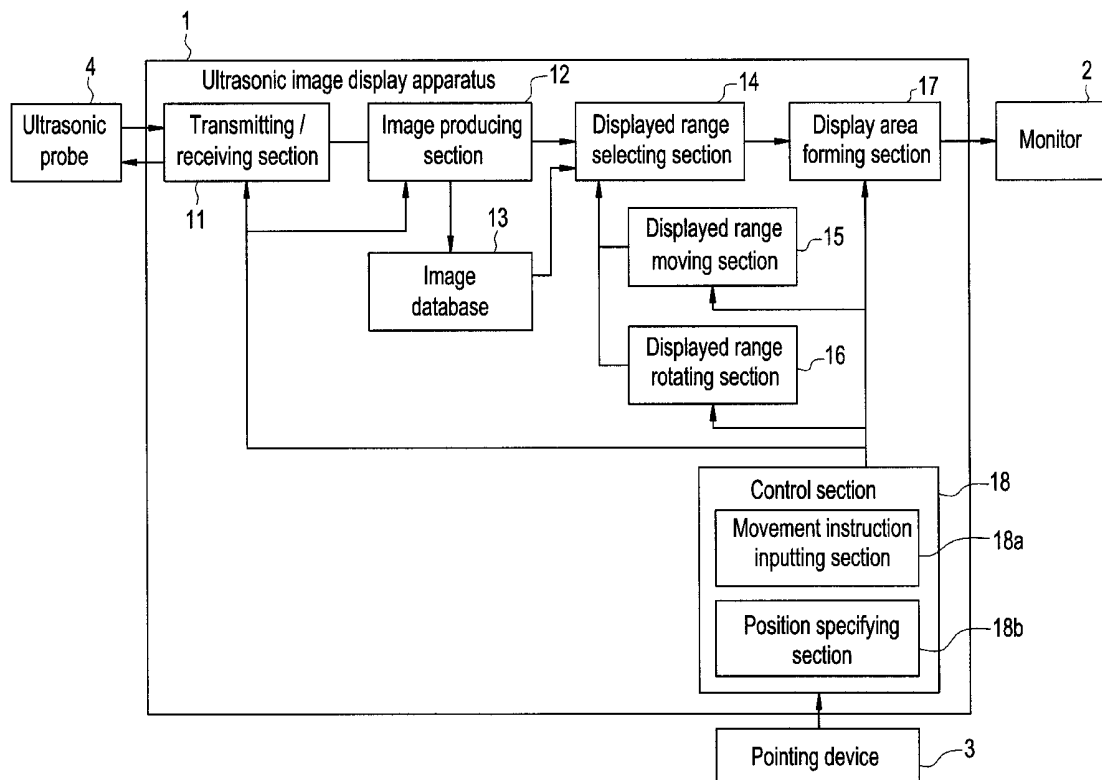


FIG. 1

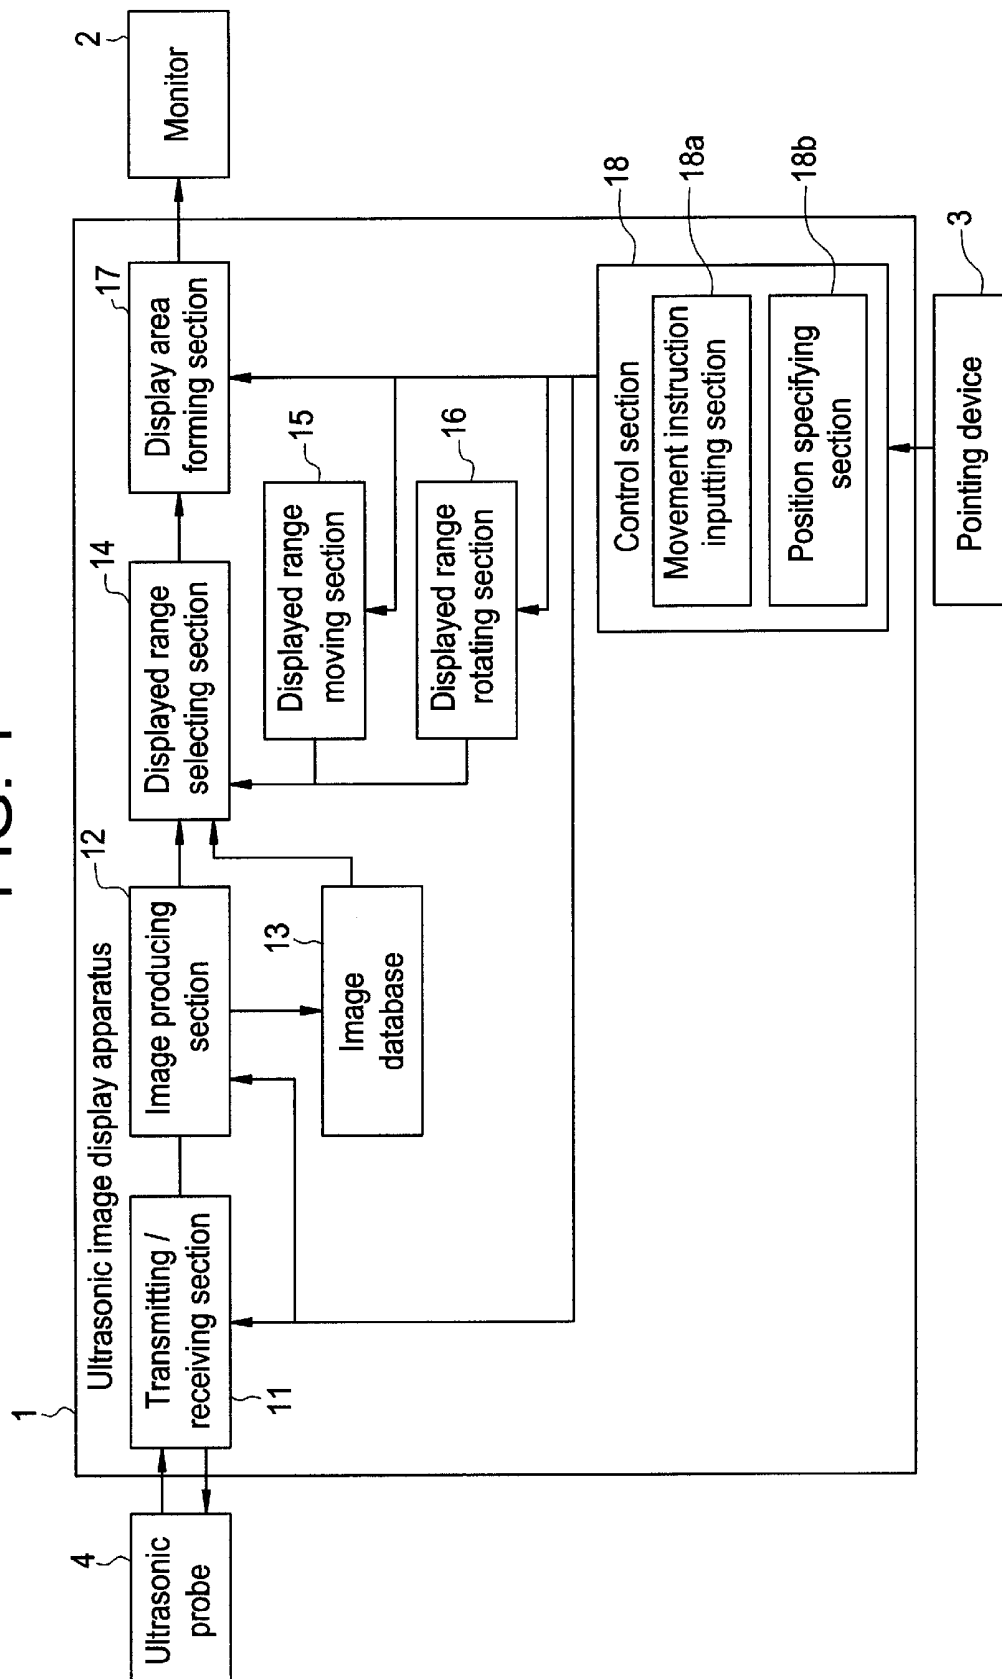


FIG. 2

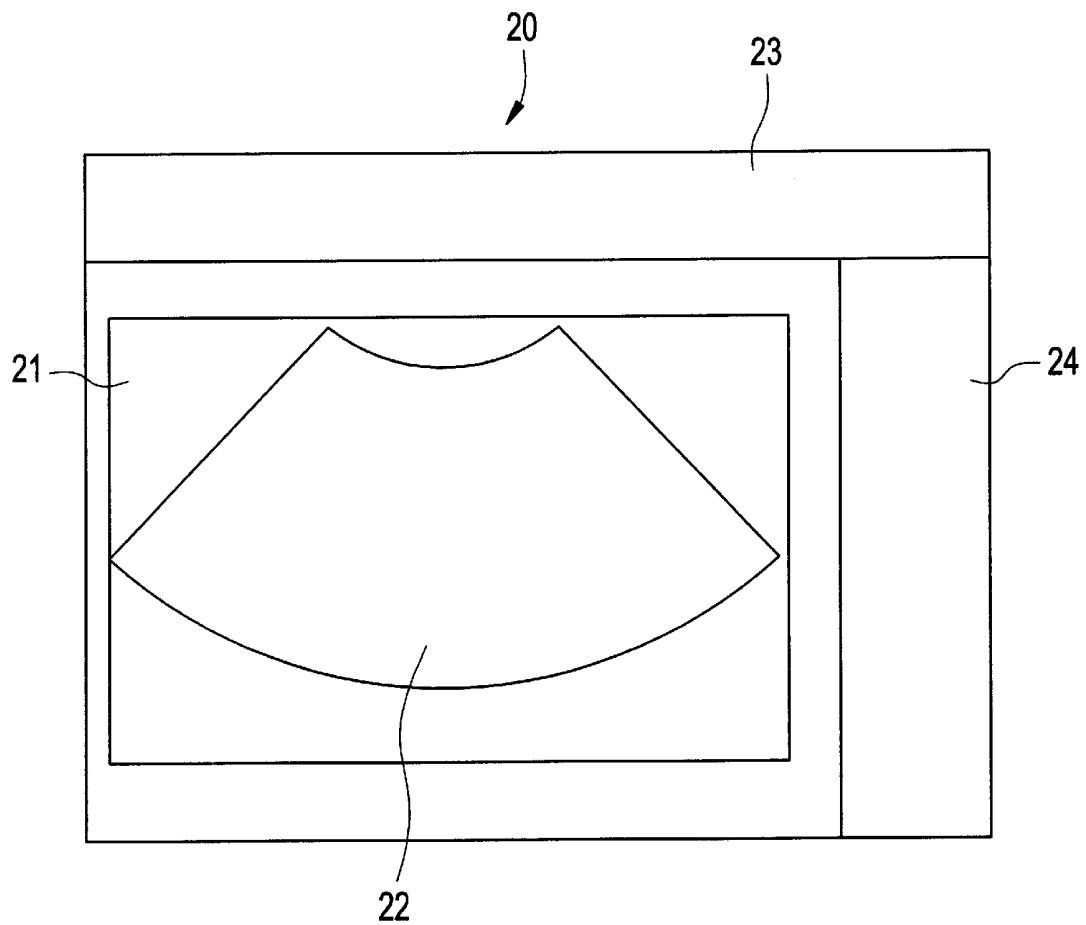


FIG. 3A

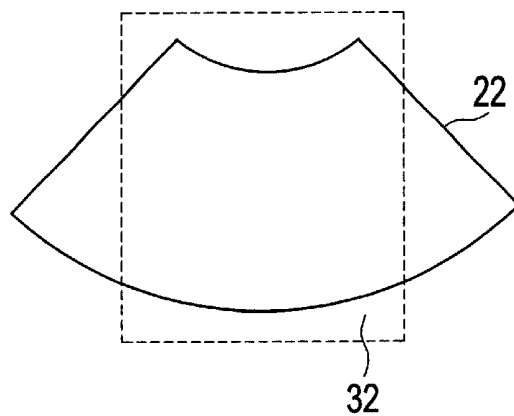


FIG. 3B

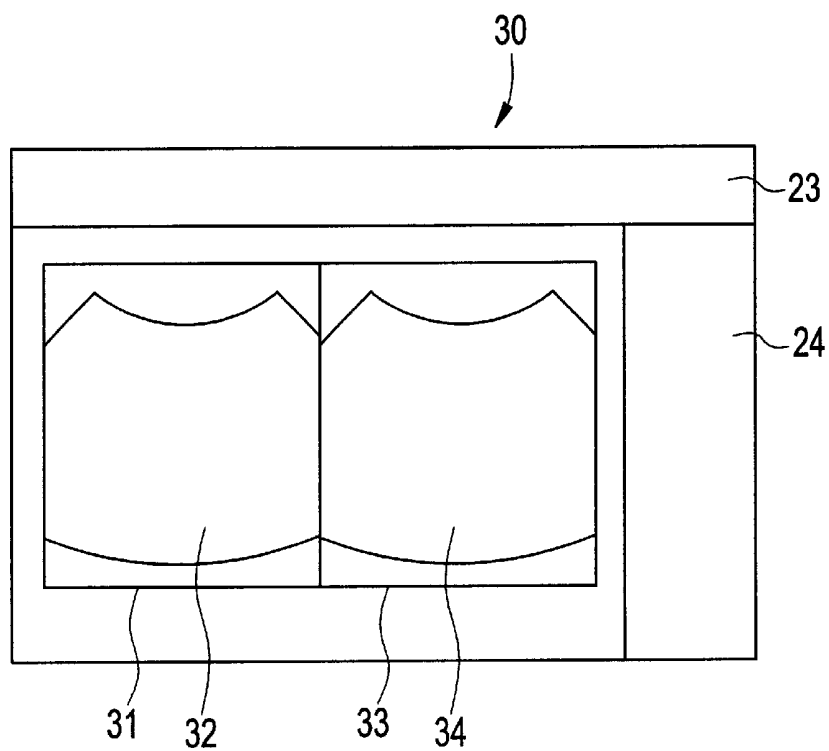


FIG. 4A

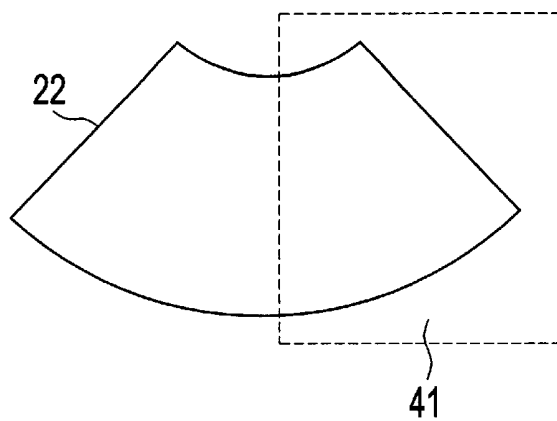


FIG. 4B

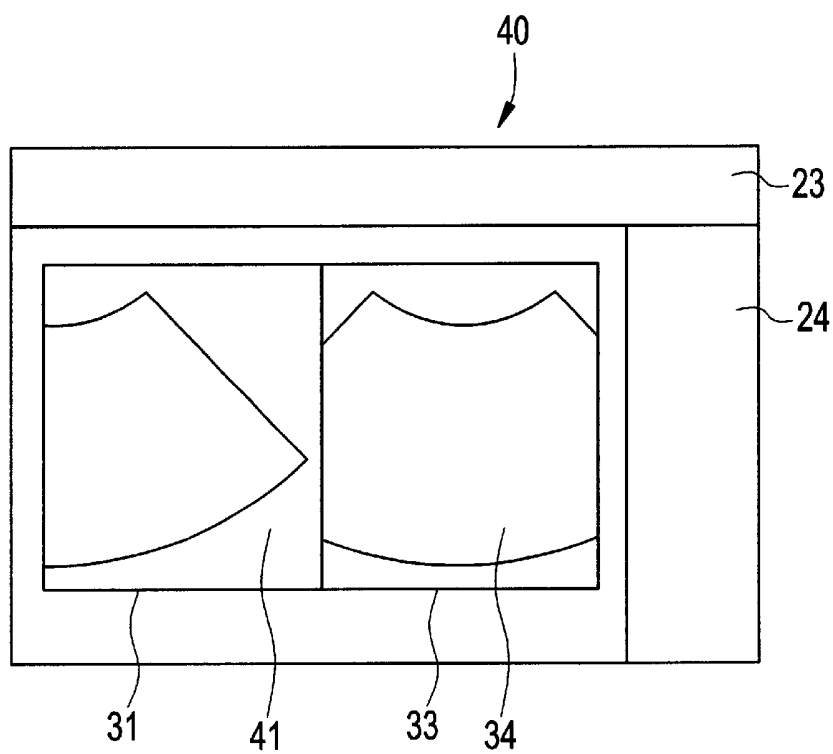


FIG. 5A

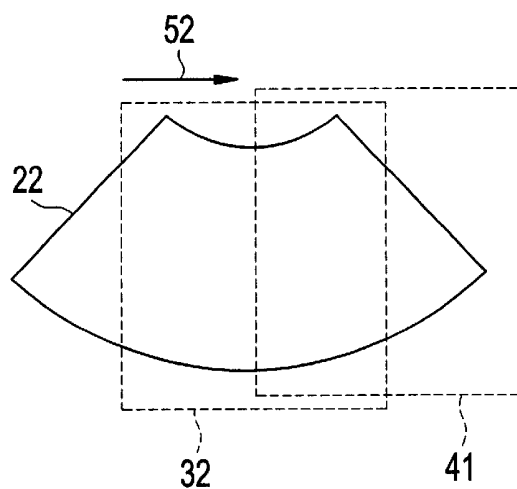


FIG. 5B

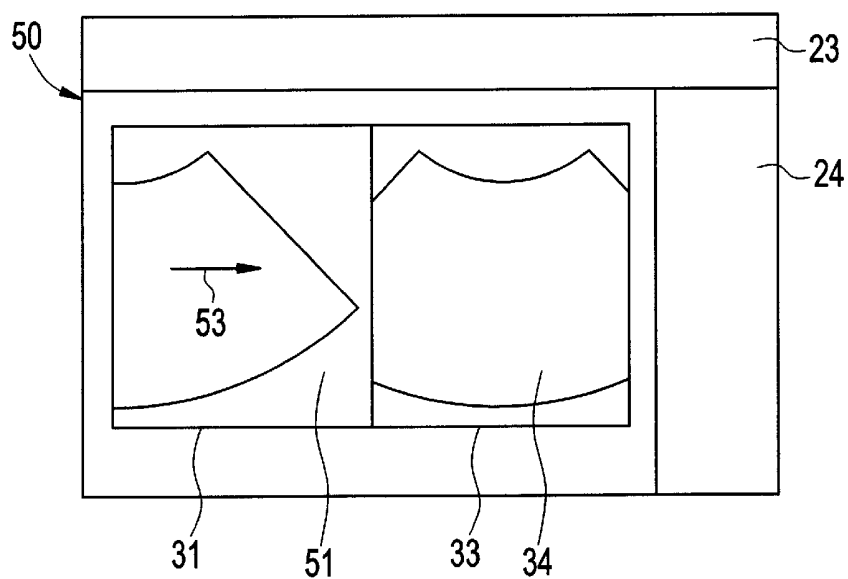


FIG. 5C

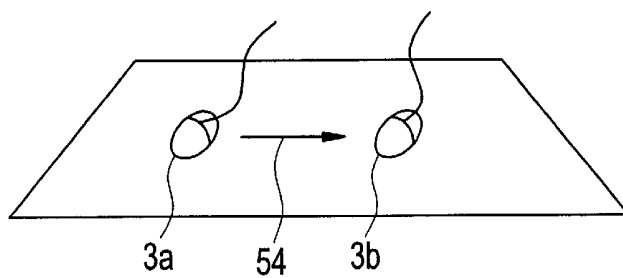


FIG. 6A

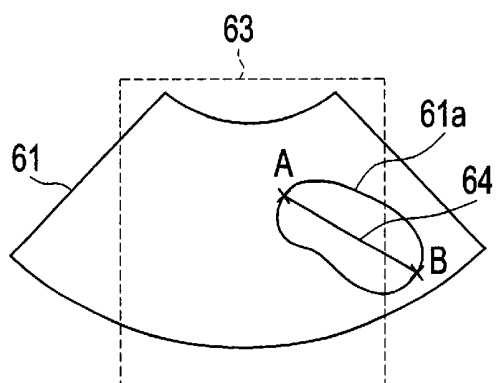


FIG. 6B

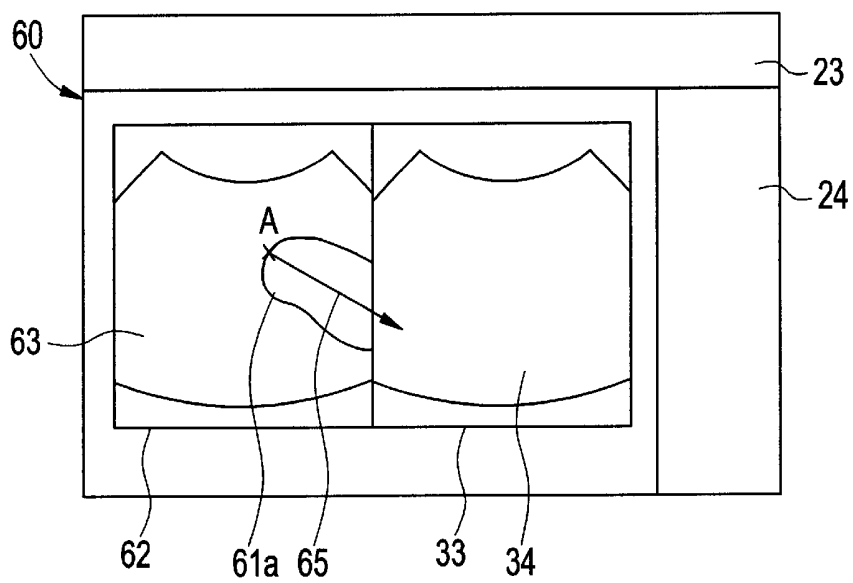


FIG. 6C

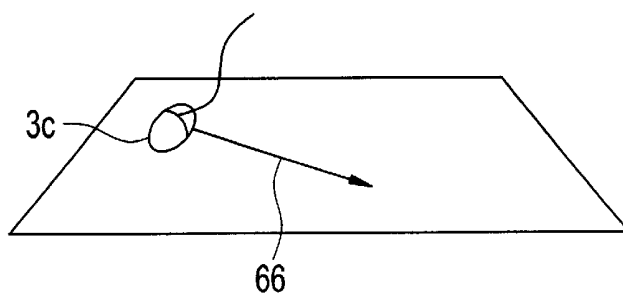


FIG. 7A

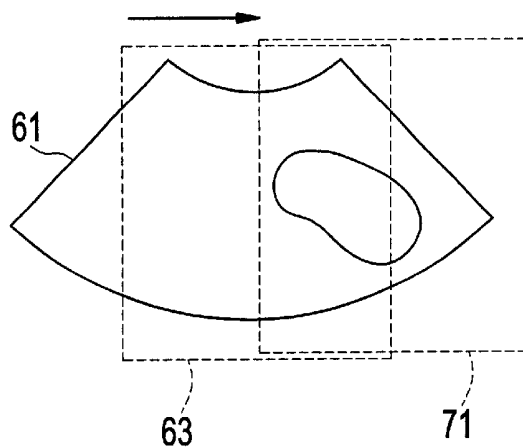


FIG. 7B

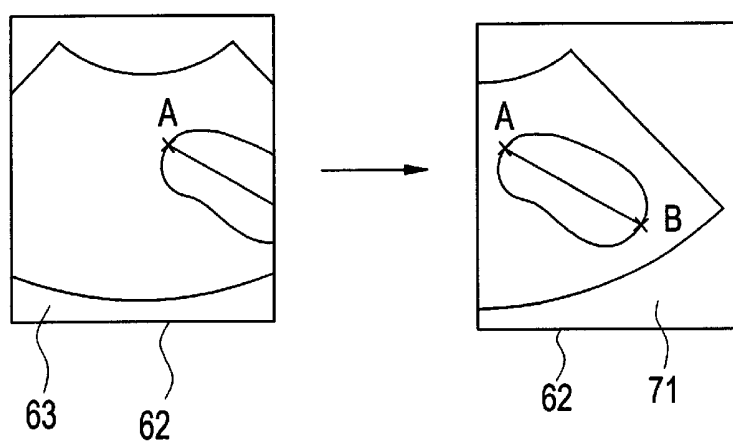


FIG. 7C

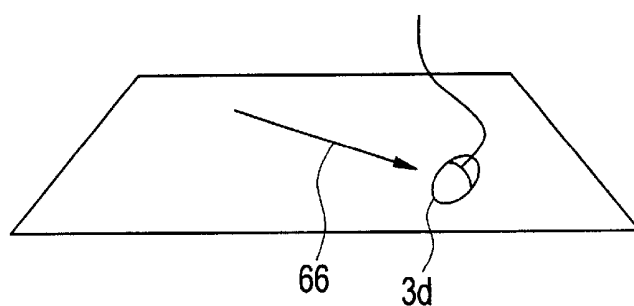


FIG. 8

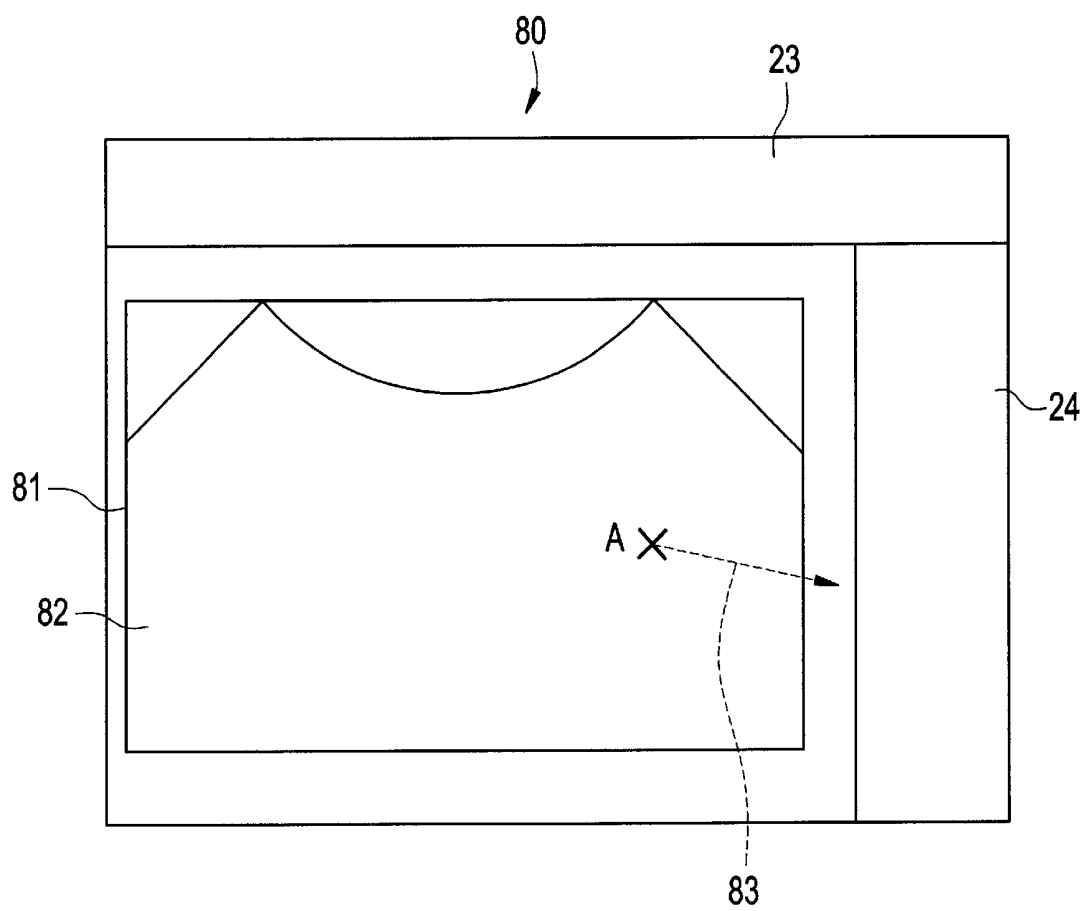


FIG. 9

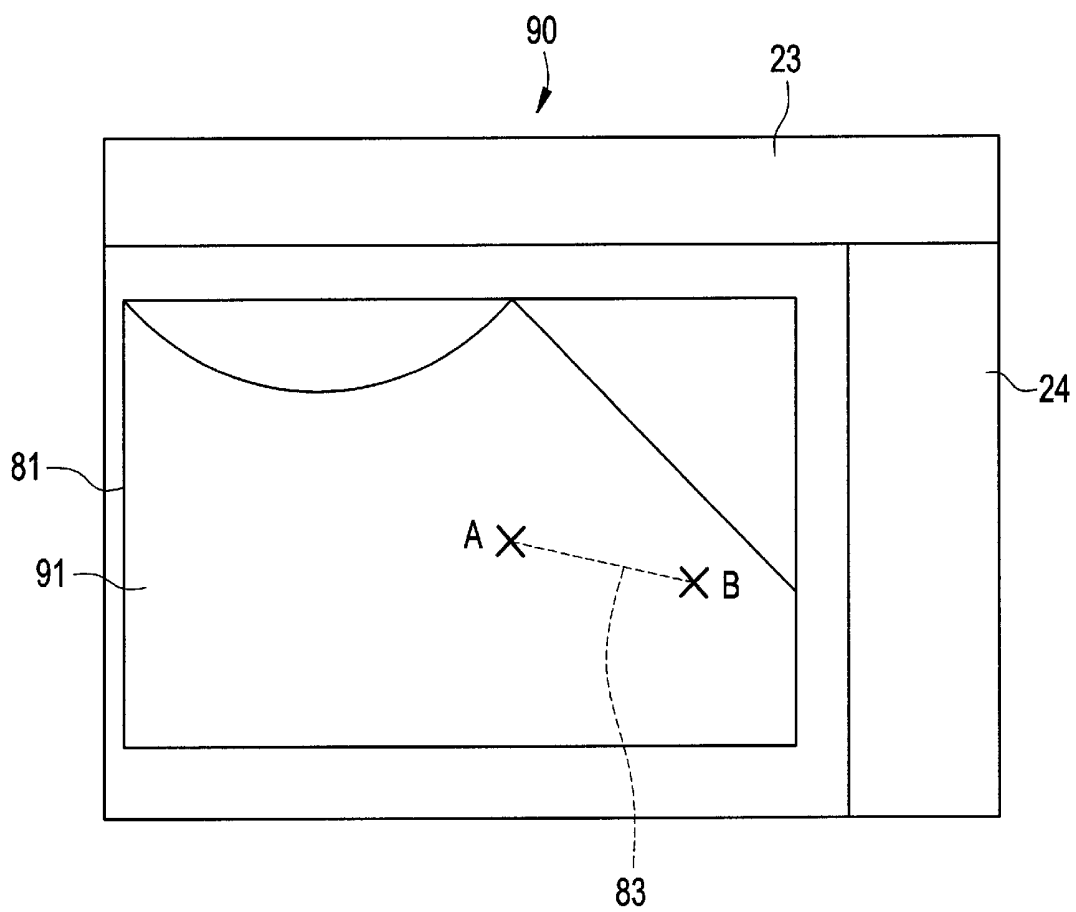


FIG. 10

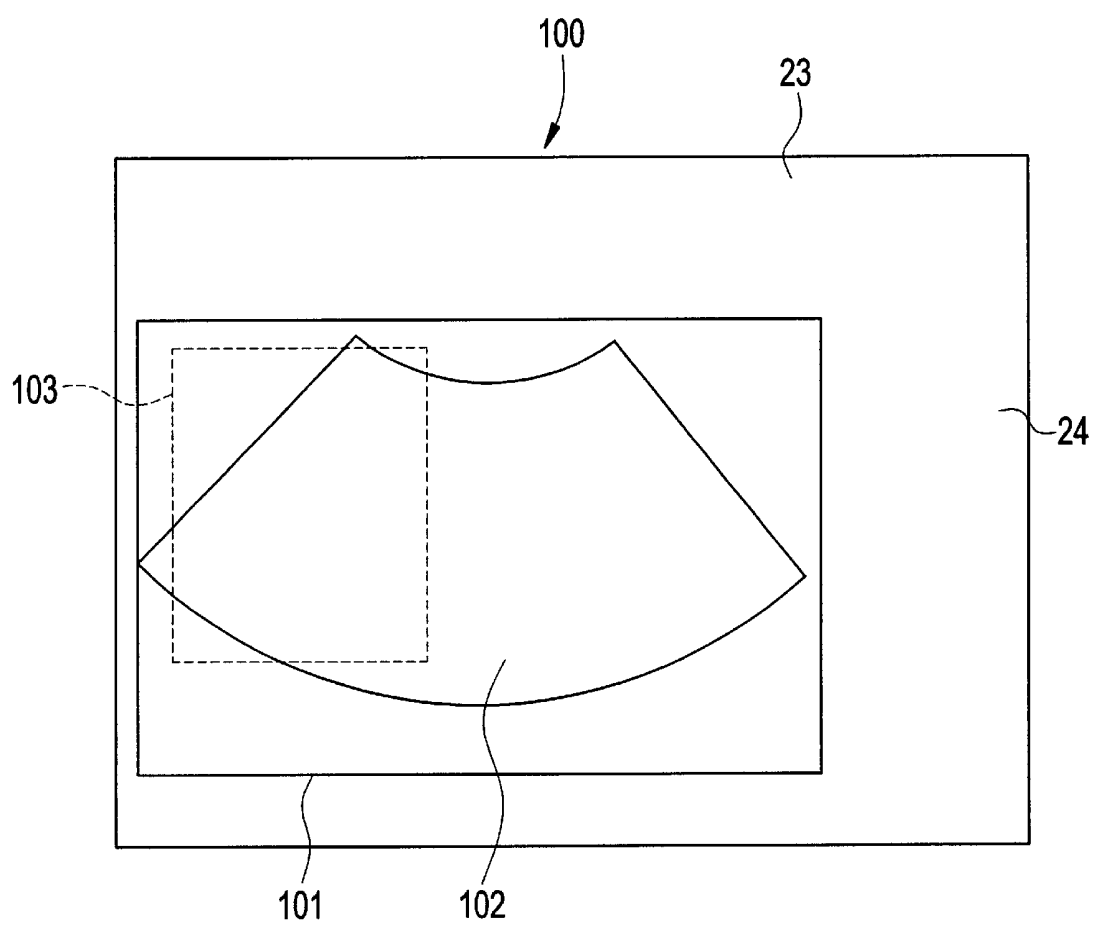


FIG. 11

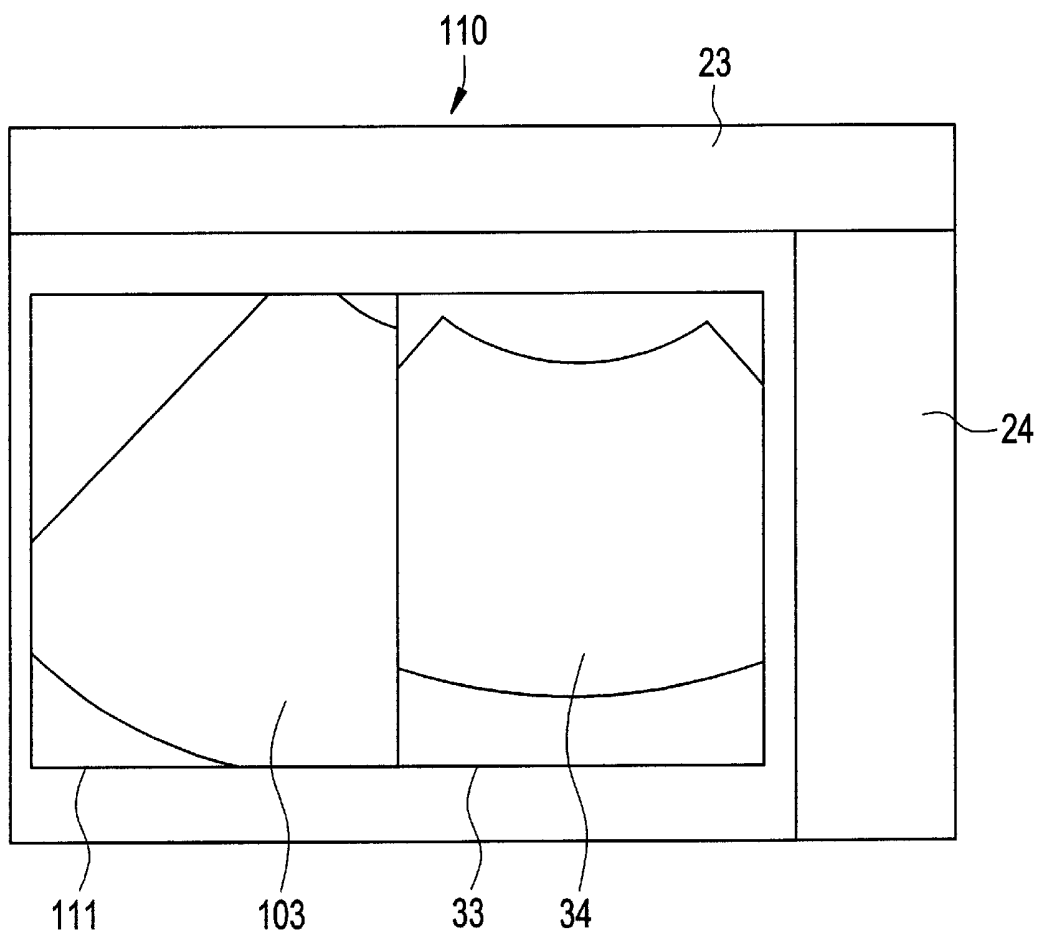


FIG. 12A

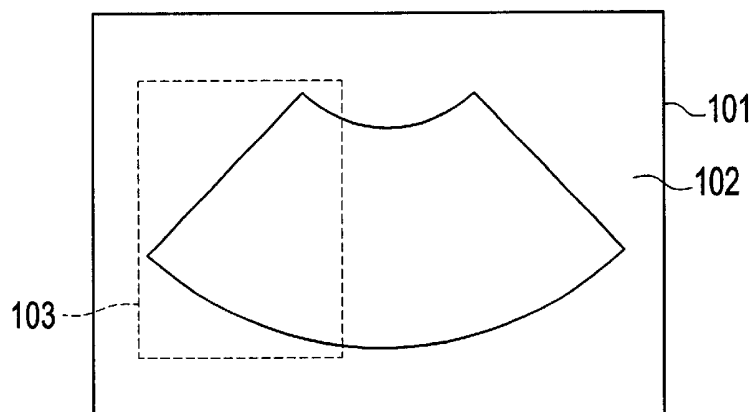


FIG. 12B

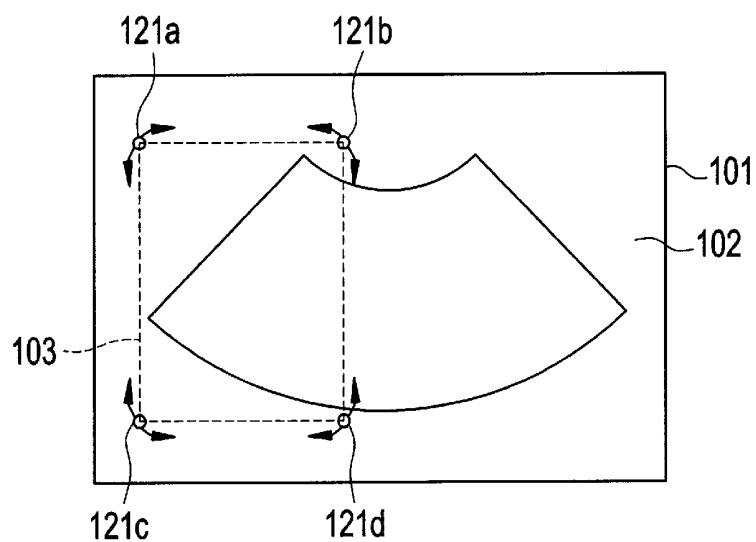


FIG. 12C


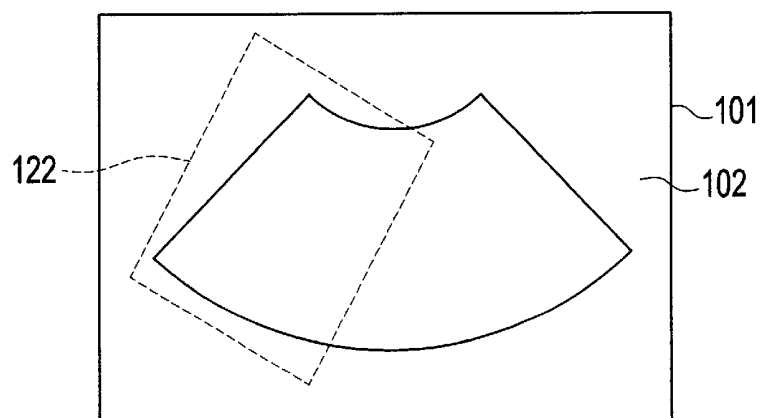


FIG. 13

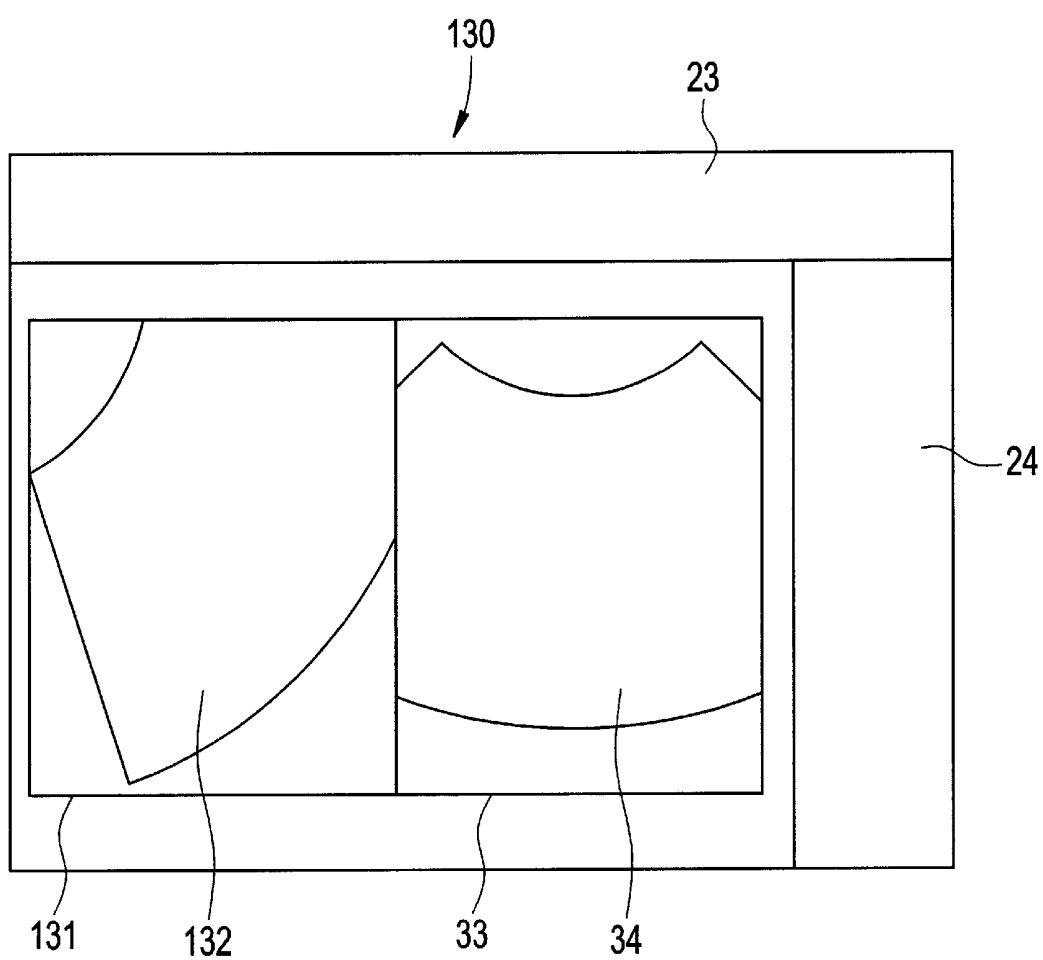

ULTRASONIC IMAGE DISPLAY APPARATUS AND ULTRASONIC IMAGE DISPLAY METHOD

This application claims the benefit of Japanese Applica- 5
tion No. 2002-115973 filed Apr. 18, 2002.

BACKGROUND OF THE INVENTION

The present invention relates to an ultrasonic image 10
display apparatus and ultrasonic image display method for
producing an ultrasonic image based on an echo signal
output by an ultrasonic probe and displaying the ultrasonic
image on a monitor, and more particularly to an ultrasonic
image apparatus and ultrasonic image display method that
improve monitor display condition operating ease and
enable easy display of an arbitrary site.

Conventionally, an ultrasonic image display apparatus for 15
imaging the interior of a subject by applying ultrasound to
a region to be examined in the subject with an abutting
ultrasonic probe, and producing an image of an echo signal
of reflected waves of the applied ultrasound is commonly
used in non-destructive examination. Since ultrasound is
harmless to a living body, the ultrasonic image display
apparatus is especially useful for medical applications and is
used for detection of foreign material in the living body,
determination of lesion degree, observation of a tumor or a
fetus, and the like.

In the conventional ultrasonic image display apparatus, in 20
general, a display method of displaying a single ultrasonic
image produced based on an echo signal and a display
method of simultaneously displaying a plurality of ultra-
sonic images are switchably used. The method of displaying
a single ultrasonic image is used for displaying the whole
ultrasonic image produced from an echo signal on a monitor, 25
and the method of simultaneously displaying a plurality of
ultrasonic images is used for comparison between the ultra-
sonic images. When the plurality of ultrasonic images are
displayed, the screen of the monitor must be allocated
among a plurality of display areas, and accordingly the
display area available for displaying each ultrasonic image
becomes smaller. To display the ultrasonic images in suffi-
cient resolution and size, part of each ultrasonic image
produced from an echo signal must be selectively displayed.
Therefore, the ultrasonic image display apparatus selectively 30
displays necessary parts of ultrasonic images for comparison
between the ultrasonic images by switching the display
between the single ultrasonic image display and multiple
ultrasonic image display.

Moreover, the ultrasonic image display apparatus usually 35
has a function of measuring distance, area, volume, and the
like in the ultrasonic image. In measuring distance in the
ultrasonic image, a pointing device capable of specifying an
arbitrary point on the monitor, such as a mouse, is employed
and two arbitrary points are specified to calculate the dis- 40
tance therebetween; or an arbitrary curve is specified using
the pointing device to calculate the length thereof. In mea-
suring an area, an arbitrary region is specified using the
pointing device to calculate the area of that region. In
measuring volume, processing for calculating the volume 45
from area and distance measurements is executed. When
distance, area or volume is to be calculated as described
above, the single display by which the whole ultrasonic
image can be displayed is more suitable than the multiple
display by which only part of the ultrasonic image is 50
displayed, because the locations to be specified must be
displayed on the monitor.

Furthermore, when an echo signal received by the ultra-
sonic probe is displayed as an ultrasonic image, the operator
must hold the ultrasonic probe against the region to be
examined and operate the ultrasonic image display apparatus
at the same time. Usually, the ultrasonic image display
apparatus must be operated by one hand because the other
hand is used for holding the ultrasonic probe. Therefore,
ease of operation in operating the ultrasonic image apparatus
is very important. For example, it is desirable that the
operation for switching between the single display and
multiple display described above can be easily done by one
hand, and that a desired portion of the ultrasonic image can
be displayed.

In the conventional ultrasonic image display apparatus 15
described above, when part of an ultrasonic image is dis-
played in the multiple display and a certain location of the
ultrasonic image not in that part is to be displayed, the
multiple display must be switched to the single display.
Therefore, when measurement of distance or area is to be
made on locations including those not displayed in the
multiple display, processing for switching from the multiple
display to the single display is required, thus imposing
limitation on the measurement in the multiple display. That
is, the conventional ultrasonic image display apparatus 25
requires the operator to conduct cumbersome operations,
leading to problems that ease of operation is reduced and the
time needed for the operations is increased.

SUMMARY OF THE INVENTION

Therefore, an object of the present invention is to provide
an ultrasonic image display apparatus and ultrasonic image
display method that improve monitor display condition
operating ease and enable easy display of an arbitrary site.

To solve the aforementioned problems and attain the
object, the present invention in accordance with a first aspect
provides an ultrasonic image display apparatus for produc-
ing an ultrasonic image based on an echo signal received by
an ultrasonic probe and displaying said ultrasonic image on
a monitor, said apparatus characterized in comprising: dis- 35
play area forming means for forming on a screen of said
monitor a display area in which at least part of said ultra-
sonic image is displayed; displayed range selecting means
for selecting a displayed range to be displayed in said
display area from said ultrasonic image; displayed range
moving means for conducting movement of said displayed
range of said ultrasonic image; and movement instruction
inputting means for inputting a direction and an amount of
the movement of said displayed range to said displayed
range moving means.

According to the invention of the first aspect, the ultra-
sonic image display apparatus produces an ultrasonic image
based on an echo signal received by an ultrasonic probe,
forms a display area for displaying the ultrasonic image on
a monitor screen, selects a displayed range to be displayed
in the display area from the ultrasonic image, and allows
scrolling of the displayed range of the ultrasonic image.

The present invention in accordance with a second aspect
is, in the invention in accordance with the first aspect,
characterized in that said ultrasonic image display apparatus
further comprises position specifying means for specifying
an arbitrary position on said monitor screen, and when the
position specified by said position specifying means is
moved from the inside to the outside of said display area,
said displayed range moving means conducts movement of
said displayed range according to the amount of said move- 65
ment.

According to the invention of the second aspect, when an arbitrary position on the monitor screen specified by the position specifying means is moved from the inside to the outside of the display area, the ultrasonic image display apparatus scrolls the displayed range according to the amount of the movement.

The present invention in accordance with a third aspect is, in the invention in accordance with the second aspect, characterized in comprising a single user interface that operates as said movement instruction inputting means or said position specifying means by switching its operation.

According to the invention of the third aspect, the scrolling of the displayed range can be conducted in a plurality of methods by switchably using a single user interface.

The present invention in accordance with a fourth aspect is, in the invention in accordance with any one of the first-third aspects, characterized in that said display area forming means is capable of switching display between single display in which a single display area is formed on said monitor screen and multiple display in which a plurality of display areas are formed on said monitor screen.

According to the invention of the fourth aspect, the ultrasonic image display apparatus is capable of switching display between single display in which a single display area is displayed on the monitor screen and multiple display in which a plurality of display areas are displayed, and allows scrolling of the displayed range of an ultrasonic image in the single or multiple display.

The present invention in accordance with a fifth aspect is, in the invention in accordance with any one of the first-fourth aspects, characterized in that said ultrasonic image display apparatus further comprises image storing means for storing an ultrasonic image converted from said echo signal as still image data, and said displayed range selecting means selects an ultrasonic image to be displayed and its displayed range from among said ultrasonic image converted from said echo signal and ultrasonic images stored in said image storing means.

According to the invention of the fifth aspect, the ultrasonic image display apparatus can arbitrarily select an ultrasonic image to be displayed in a display area from among a scan image produced from an echo signal and ultrasonic images stored in the image storing means, and allows scrolling of the displayed range.

The present invention in accordance with a sixth aspect is, in the invention in accordance with any one of the first-fifth aspects, characterized in that when said display area forming means forms a plurality of display areas, said displayed range selecting means selects ultrasonic images to be displayed and their displayed ranges respectively for said plurality of display areas.

According to the sixth aspect, when a plurality of display areas are displayed on the monitor screen, the ultrasonic image display apparatus can arbitrarily select ultrasonic images to be displayed in respective display areas from among a scan image produced from an echo signal and ultrasonic images stored in the image storing means, and allows scrolling of the displayed ranges.

The present invention in accordance with a seventh aspect is, in the invention in accordance with any one of the fourth-sixth aspects, characterized in that when said display area forming means switches display from the single display to the multiple display, said displayed range selecting means selects part of the ultrasonic image displayed in the single display as said displayed range, and displays said displayed range in at least one of said plurality of display areas.

According to the invention of the seventh aspect, when display is switched from the single display to the multiple display, the ultrasonic image display apparatus selects part of the ultrasonic image displayed in the single display as the displayed range, and displays it in at least one of the plurality of display areas.

The present invention in accordance with an eighth aspect is, in the invention in accordance with any one of the first-seventh aspects, characterized in further comprising displayed range rotating means for rotating said displayed range of said ultrasonic image.

According to the invention of the eighth aspect, the ultrasonic image display apparatus can rotate the displayed range of an ultrasonic image displayed in a display area to display the range at a desired angle.

The present invention in accordance with a ninth aspect provides an ultrasonic image display method for producing an ultrasonic image based on an echo signal received by an ultrasonic probe and displaying said ultrasonic image on a monitor, said method characterized in comprising: a display area forming step of forming on a screen of said monitor a display area in which at least part of said ultrasonic image is displayed; a displayed range selecting step of selecting a displayed range to be displayed in said display area from said ultrasonic image; a displayed range moving step of conducting movement of said displayed range of said ultrasonic image; and a movement instructing step of inputting a direction and an amount of the movement of said displayed range to said displayed range moving means.

According to the invention of the ninth aspect, the ultrasonic image display method produces an ultrasonic image based on an echo signal received by an ultrasonic probe, forms a display area for displaying the ultrasonic image on a monitor screen, selects a displayed range to be displayed in the display area from the ultrasonic image, and allows scrolling of the displayed range of the ultrasonic image.

The present invention in accordance with a tenth aspect is, in the invention in accordance with the ninth aspect, characterized in that said ultrasonic image display method further comprises a position specifying step of specifying an arbitrary position on said monitor screen, and when the position specified by said position specifying step is moved from the inside to the outside of said display area, said displayed range moving step conducts movement of said displayed range according to the amount of said movement.

According to the invention of the tenth aspect, when an arbitrary position on the monitor screen specified by the position specifying means is moved from the inside to the outside of the display area, the ultrasonic image display method scrolls the displayed range according to the amount of the movement.

The present invention in accordance with an eleventh aspect is, in the invention in accordance with the ninth or tenth aspect, characterized in that said movement instructing step and said position specifying step are executed by a single user interface.

According to the invention of the eleventh aspect, the scrolling of the displayed range can be conducted in a plurality of methods by switchably using a single user interface.

The present invention in accordance with a twelfth aspect is, in the invention in accordance with the ninth-eleventh aspect, characterized in that said display area forming step is capable of switching display between single display in which a single display area is formed on said monitor screen and multiple display in which a plurality of display areas are formed on said monitor screen.

According to the invention of the twelfth aspect, the ultrasonic image display method is capable of switching display between single display in which a single display area is displayed on the monitor screen and multiple display in which a plurality of display areas are displayed, and allows scrolling of the displayed range of an ultrasonic image in the single or multiple display.

The present invention in accordance with a thirteenth aspect is, in the invention in accordance with any one of the ninth–twelfth aspects, characterized in that said ultrasonic image display method further comprises an image storing step of storing an ultrasonic image produced based on said echo signal as still image data, and said displayed range selecting step selects an ultrasonic image to be displayed and its displayed range from among said ultrasonic image converted from said echo signal and ultrasonic images stored by said image storing step.

According to the invention of the thirteenth aspect, the ultrasonic image display method can arbitrarily select an ultrasonic image to be displayed in a display area from among a scan image produced from an echo signal and ultrasonic images stored in the image storing means, and allows scrolling of the displayed range.

The present invention in accordance with a fourteenth aspect is, in the invention in accordance with any one of the ninth–thirteenth aspects, characterized in that when said display area forming step forms a plurality of display areas, said displayed range selecting step selects ultrasonic images to be displayed and their displayed ranges respectively for said plurality of display areas.

According to the fourteenth aspect, when a plurality of display areas are displayed on the monitor screen, the ultrasonic image display method can arbitrarily select ultrasonic images to be displayed in respective display areas from among a scan image produced from an echo signal and ultrasonic images stored in the image storing means, and allows scrolling of the displayed ranges.

The present invention in accordance with a fifteenth aspect is, in the invention in accordance with the twelfth–fourteenth aspect, characterized in that when said display area forming step switches display from the single display to the multiple display, said displayed range selecting step selects part of the ultrasonic image displayed in the single display as said displayed range, and displays said displayed range in at least one of said plurality of display areas.

According to the invention of the fifteenth aspect, when display is switched from the single display to the multiple display, the ultrasonic image display method selects part of the ultrasonic image displayed in the single display as the displayed range, and displays it in at least one of the plurality of display areas.

The present invention in accordance with a sixteenth aspect is, in the invention in accordance with any one of the ninth–fifteenth aspects, characterized in further comprising a displayed range rotating step of rotating said displayed range of said ultrasonic image.

According to the invention of the sixteenth aspect, the ultrasonic image display method can rotate the displayed range of an ultrasonic image displayed in a display area to display the range at a desired angle.

Therefore, in the ultrasonic image display apparatus and ultrasonic image display method in accordance with the present invention for displaying an ultrasonic image produced based on an echo signal output by an ultrasonic probe in one or more display areas formed on the monitor screen, a displayed range of the ultrasonic image displayed in the

display area can be scrolled in the display area; and therefore, an effect that there are provided an ultrasonic image display apparatus and ultrasonic image display method that improve monitor display condition operating ease and enable easy display of an arbitrary site is obtained.

Further objects and advantages of the present invention will be apparent from the following description of the preferred embodiments of the invention as illustrated in the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is an explanatory diagram for explaining the overall configuration of an ultrasonic image display apparatus in accordance with the present embodiment.

FIG. 2 is an explanatory diagram for explaining a monitor screen when a display area forming section forms a single display area.

FIG. 3 is an explanatory diagram for explaining a monitor screen when the display area forming section forms two display areas.

FIG. 4 is an explanatory diagram for explaining a monitor screen in which two display areas are formed and an edge portion of an ultrasonic image is displayed.

FIG. 5 is an explanatory diagram for explaining an operation for modifying a display area using a movement instruction inputting section.

FIG. 6 is an explanatory diagram for explaining an operation for modifying a display area using a position specifying section.

FIG. 7 is an explanatory diagram for explaining an example of modification of a displayed range.

FIG. 8 is an explanatory diagram for explaining a scroll operation by a pointing device in single display.

FIG. 9 is an explanatory diagram for explaining a monitor screen in single display after switching a displayed range by an operation of a pointing device.

FIG. 10 is an explanatory diagram for explaining a monitor screen in the single display condition before switching to multiple display.

FIG. 11 is an explanatory diagram for explaining a monitor screen after switching from single display to multiple display.

FIG. 12 is an explanatory diagram for explaining an operation for rotating a displayed range of an ultrasonic image.

FIG. 13 is an explanatory diagram for explaining a condition of an ultrasonic image displayed after rotation.

DETAILED DESCRIPTION OF THE INVENTION

An ultrasonic image display apparatus in accordance with an embodiment of the present invention will now be described in detail with reference to the accompanying drawings.

In this embodiment, an ultrasonic image display apparatus that allows use of a whole ultrasonic image in a limited display area by scrolling and rotating a portion of the ultrasonic image that is displayed on a monitor will be described.

FIG. 1 is an explanatory diagram for explaining the overall configuration of the ultrasonic image display apparatus in accordance with the present embodiment. In FIG. 1, the ultrasonic image display apparatus 1 is connected with a

monitor **2**, a pointing device **3**, and an ultrasonic probe **4**. The monitor **2** employed may be of any type, such as a CRT monitor or a liquid crystal monitor. The pointing device **3** is implemented by means for specifying arbitrary points on a screen of the monitor **2**, such as a mouse, trackball, cursor key or the like.

The ultrasonic image display apparatus **1** comprises therein a transmitting/receiving section **11** connected to the ultrasonic probe **4**, an image producing section **12** for producing an ultrasonic image from an echo signal received by the ultrasonic probe **4**, an image database **13** for storing images produced by the image producing section **12**, a display area forming section **17** for forming on the monitor **2** screen a display area in which the ultrasonic image is displayed, a displayed range selecting section **14** for determining a range of the ultrasonic image that is to be displayed in the display area, a displayed range moving section **15** for scrolling the displayed range of the ultrasonic image, a displayed range rotating section **16** for rotating the displayed range of the ultrasonic image, and a control section **18** connected with the pointing device **3** and an input interface which is not shown.

The control section **18** comprises therein a movement instruction inputting section **18a** and a position specifying section **18b**. The movement instruction inputting section **18a** outputs to the displayed range moving section **15** a direction and an amount of movement supplied by the pointing device **3** as a direction and amount of movement of the displayed range of the ultrasonic image. The position specifying section **18b** translates positional information supplied by the pointing device **3** into a position on the monitor **2** screen, and also translates movement of the pointing device **3** into movement on the screen. The control section **18** handles a plurality of types of processing in response to inputs from the pointing device **3** by switchably using the movement instruction inputting section **18a** and position specifying section **18b**.

The control section **18** also supplies a driving signal to the ultrasonic probe **4** via the transmitting/receiving section **11** to transmit ultrasound. The ultrasonic probe **4** receives an echo signal of reflected waves of the transmitted ultrasound and outputs the echo signal to the image producing section **12** via the transmitting/receiving section **11**.

When an ultrasonic image is to be displayed using the ultrasonic image display apparatus **1**, the ultrasonic probe **4** is first abutted against a region to be examined in a subject to transmit ultrasound, and the ultrasonic probe **4** receives an echo signal of reflected waves of the transmitted ultrasound. The image producing section **12** produces a scan image representing the echo signal received by the ultrasonic probe **4** as an image in real time. Thus, if a change in the echo signal received by the ultrasonic probe **4** arises, the ultrasonic image produced by the image producing section **12** varies according to the change. The control section **18** transmits a control command for directing the image producing section **12** to store the ultrasonic image when save of the ultrasonic image is commanded using the pointing device **3** or a console panel (not shown). When the control command to store the ultrasonic image is received from the control section **18**, the image producing section **12** stores the ultrasonic image that is a scan image at that time in the image database **13**.

The display area forming section **17** forms at least one display area in which the ultrasonic image is displayed on the monitor **2** screen. The displayed areas are defined by specifying the number of display areas, their sizes, and their

locations. The displayed range selecting section **14** identifies an ultrasonic image to be displayed in a display area formed by the display area forming section **17**, and its displayed range to be displayed in the display area. When a plurality of display areas are formed, the displayed range selecting section **14** selects ultrasonic images to be displayed and their displayed ranges for the respective display areas. Moreover, the displayed range selecting section **14** can arbitrarily select an ultrasonic image to be displayed in the display area from among the scan image produced by the image producing section **14** and the ultrasonic images stored in the image database **13**.

The monitor **2** displays the ultrasonic image and its displayed range selected by the displayed range selecting section **14** in the display area formed by the display area forming section **17**. By thus forming the display area by the display area forming section **17** and determining an ultrasonic image to be displayed in the display area and its displayed range by the displayed range selecting section **14**, an arbitrary ultrasonic image can be selected and displayed to have a desired size, and ultrasonic image single display and multiple display can be switched.

Furthermore, the control section **18** modifies the displayed range using the movement instruction inputting section **18a** or position specifying section **18b** in response to an input from the pointing device **3**. Specifically, when scrolling of the displayed range of the ultrasonic image is specified, a control command to move the displayed range is output to the displayed range moving section **15**. When rotation of the displayed range of the ultrasonic image is specified, a control command to rotate the displayed range is output to the displayed range rotating section **16**.

The displayed range moving section **15** scrolls the displayed range selected at that time by the displayed range selecting section **14** in response to the control command received from the control section **18**. The displayed range rotating section **16** rotates the displayed range selected at that time by the displayed range selecting section **14** in an arbitrary direction in response to the control command received from the control section **13**.

Next, description will be specifically made on a screen displayed on the monitor **2** by the ultrasonic image display apparatus **1** and modification of the display screen using the pointing device **3** with reference to FIGS. 2–13. FIG. 2 is an explanatory diagram for explaining a monitor screen when the display area forming section **17** forms a single display area. FIG. 3 is an explanatory diagram for explaining a monitor screen when the display area forming section **17** forms two display areas. In FIG. 2, the monitor screen **20** comprises a display area **21**, an information display area **23**, and an operation area **24**; and an ultrasonic image **22** is displayed in the display area **21**. In FIG. 3(b), the monitor screen **30** comprises display areas **31** and **33**, the information display area **23**, and the operation area **24**; and a displayed range **32** that is part of the ultrasonic image **22** is displayed in the display area **31**, and a displayed range **34** of another ultrasonic image is displayed in the display area **33**.

The information display area **23** is for displaying information relating to the ultrasonic image and measurement status, and the operation area **24** is for displaying virtual buttons for operations by the pointing device. The information display area **23** and operation area **24** may be in any location and have any size as necessary.

Since the monitor screen **20** forms the single display, a display area **21** of sufficient size can be secured and the whole ultrasonic image **22** can be displayed. On the other

hand, since two display areas must be secured in the monitor screen **30**, the display areas **31** and **33** are smaller than the display area **21**. Accordingly, an ultrasonic image cannot be displayed as a whole in the display area **31** or **33**, and a partial region is selectively displayed. As shown in FIG. **3(a)**, in the display area **31**, part of the ultrasonic image **22** is selected as the displayed range **32** for display. In FIG. **3(b)**, both in the display areas **32** and **34**, portions near the centers of the whole ultrasonic images are selected, and edge portions are not displayed. FIG. **4** is an explanatory diagram for explaining a monitor screen in which two display areas are formed and an edge portion of an ultrasonic image is displayed. In FIG. **4**, the monitor screen **40** comprises the display areas **31** and **33**, information display area **23** and operation area **24**; and a displayed range **41** that is part of the ultrasonic image **22** near an edge portion is displayed in the display area **31**, and the displayed range **34** is displayed in the display area **33**.

When such a plurality of display areas are formed, an ultrasonic image cannot be displayed as a whole in a display area, and therefore, a need to modify the displayed range of the ultrasonic image in the display area arises. The ultrasonic image display apparatus **1** modifies the displayed range using the movement instruction inputting section **18a** or position specifying section **18b** in response to an input from the pointing device **3**.

FIG. **5** is an explanatory diagram for explaining an operation for modifying the display area using the movement instruction inputting section **18a**. When the pointing device **3** is operated and moved, the movement instruction inputting section **18a** outputs the direction and amount of the movement to the displayed range moving section **15** as a direction and amount of movement of the displayed range of the ultrasonic image **22**. Thus, when the pointing device **3** is moved from a position **3a** to a position **3b** (FIG. **5(c)**), the displayed range of the ultrasonic image **22** is moved from the displayed range **32** to the displayed range **41** (FIG. **5(a)**) corresponding to the amount of pointing device movement **54**. The amount of displayed range movement **52** in this case is determined by the amount of the pointing device movement **54**. During the operation of the pointing device **3**, a monitor screen **50** sequentially changes and displays a displayed range **51** corresponding to the operation of the pointing device **3**, as shown in FIG. **5(b)**. That is, the displayed range **51** in the display area **31** scrolls in the direction of movement **53**. It should be noted that the operation of the pointing device used for the movement of the displayed range and the operation of the pointing device used for specifying a position on the screen must be discriminated. For example, if a mouse is employed as the pointing device, a movement operation of the mouse with a predetermined button on the mouse pressed, i.e., an operation generally referred to as dragging, causes the movement of the displayed range; and a movement operation of the mouse without pressing any button causes the position specification on the screen, whereby the movement of the displayed range and the position specification on the screen can be discriminated.

Since the direction and amount of movement of the display area can be directly input by an operation of the pointing device **3** by the aforementioned operation for modifying the display area using the movement instruction inputting section **18a**, the display area can be modified by a simple operation and a desired range of the ultrasonic image **22** can be displayed. While the description has been made on a case in which the displayed range is modified in the display area **31** that is one of two display areas **31** and **33**, the

displayed range can be modified in the other display range **33** by a similar operation. Which of the plurality of display areas is affected by an operation of the pointing device **3** is determined by a selective action ascribed to the pointing device **3**; for example, if a mouse is used as the pointing device **3**, the plurality of display areas may be switched from one to another by clicking a predetermined button.

Next, an operation for modifying the display area using the position specifying section **18b** will be described. FIG. **6** is an explanatory diagram for explaining an operation for modifying the display area using the position specifying section **18b**. The description hereinbelow will be made on a case in which a subject image **61a** is present inside an ultrasonic image **61** and the length of the subject image **61a** is to be measured. FIG. **6(a)** shows the ultrasonic image **61**, which is the whole ultrasonic image; and FIG. **6(b)** shows a monitor screen **60**. The ultrasonic image **61** contains the subject image **61a** from the center to a portion near an edge of the ultrasonic image **61**. The monitor screen **60** comprises display areas **62** and **33**, the information display area **23**, and the operation area **24**; and a displayed range **63** is displayed in the display area **62**, and the displayed range **34** is displayed in the display area **33**. The displayed range **63** represents a portion near the center of the ultrasonic image **61**, and the subject image **61a** is partially displayed.

When the length of the subject image **61a**, i.e., a distance **64** between two points A and B shown in FIG. **6(a)**, is to be measured, the pointing device **3** is first operated in the condition of FIG. **6(b)**, and the measurement start point A is specified and selected by the position specifying section **18b**. Then, the pointing device **3** is moved from a position **3c** corresponding to the measurement start point A to move the specified position in the display area **62**, as shown in FIG. **6(c)**. The amount of the specified position movement **65** on the monitor screen corresponds to the amount of the pointing device movement **66**.

If the specified position is moved outside the display area **62** by the operation of the pointing device **3**, the position specifying section **18b** outputs a command to modify the displayed range to the displayed range moving section **15**. The modification of the displayed range is achieved by scrolling the displayed range so that the destination of the movement of the specified position falls within the display area **62**. FIG. **7** is an explanatory diagram for explaining an example of the modification of the displayed range. As shown in FIG. **7(c)**, when the pointing device **3** has been moved to a position **3d** corresponding to the measurement end point B by the amount of pointing device movement **66**, the displayed range of the ultrasonic image **61** moves from the displayed range **63** to a displayed range **71** as shown in FIG. **7(a)**. Thus, the displayed range displayed in the display area **62** is scrolled from the displayed range **63** to the displayed range **71** as shown in FIG. **7(b)**, and the measurement end point B is displayed in the display area **62**.

When the specified position is thus moved from the inside to the outside of the display area by the operation of the pointing device **3**, the displayed range of the ultrasonic image is scrolled so that the destination of the movement falls within the display area, whereby a desired range of the ultrasonic image can be displayed without switching display from multiple display to single display. Moreover, the movement of the displayed range using the position specifying section **18b** can achieve specification of the distance to be measured and scrolling of the displayed range at the same time; and therefore, the need to switch the display mode in order to display the whole site to be measured is eliminated, and measurement may be started even if only part of the site to be measured is displayed.

Such scrolling of the displayed range may be used not only in the multiple display but in the single display. FIG. 8 is an explanatory diagram for explaining a scroll operation by the pointing device in the single display; and FIG. 9 is an explanatory diagram for explaining a monitor screen in the single display after switching the displayed range by an operation of the pointing device. In FIG. 8, a monitor screen 80 comprises a display area 81, the information display area 23, and the operation area 24; and a displayed range 82 of the ultrasonic image with its central portion enlarged is displayed in the display area 81. In the monitor screen 80, for example, when a specified position specified by the pointing device 3 is moved from a specified position A within the display area 81 to a position outside thereof, as indicated by the amount of specified position movement 83, the position specifying section 18b outputs a command to the displayed range moving section 15 to move the displayed range so that the destination of the movement of the specified position falls within the display area 81. The displayed range moving section 15 scrolls and moves the displayed range selected by the displayed range selecting section 14 in response to the command. After scrolling the displayed range, the monitor 2 displays a monitor screen 90 shown in FIG. 9.

The monitor screen 90 comprises the display area 81, information display area 23, and operation area 24; and a displayed range 91 near the edge of the ultrasonic image is displayed in the display area 81. The displayed range 91 represents an image after scrolling the displayed range 82 of the ultrasonic image. The specified position A is identical to that in the displayed range 82 of the ultrasonic image; and a specified position 3 that is the destination of the movement is further displayed. Thus, even if the ultrasonic image is enlarged and displayed in a single display area and part of the ultrasonic image is not displayed, when the specified position is moved from the inside to the outside of the display area by the pointing device 3, the selected range of the ultrasonic image is scrolled so that the destination falls within the display area, whereby a desired range of the ultrasonic image can be displayed. While the description has been made on scrolling of the displayed range by the position specifying section 18b, the displayed range may be moved by using the movement instruction inputting section 18a.

Next, switching from the single display to the multiple display will be described. FIG. 10 is an explanatory diagram for explaining a monitor screen in the single display condition before switching to the multiple display; and FIG. 11 is an explanatory diagram for explaining a monitor screen after switching from the single display to the multiple display. In FIG. 10, a monitor screen 100 comprises a display area 101, the information display area 23, and the operation area 24; and an ultrasonic image 102 is displayed in the display area 101. Here, the ultrasonic image 102 is displayed as a whole. When a desired range of the ultrasonic image 102 is selected as a specified range 103 by the pointing device 3, the display area forming section 14 switches the display from the single display to the multiple display, and the displayed range selecting section 14 displays the specified range 103 in one of the plurality of display areas. At that time, the display area selecting section 14 displays the selected range of the ultrasonic image enlarged as necessary. So that, when the specified range 103 is selected in the single display, it can be specified which is to be executed between enlarged single display in which the specified range 103 is enlarged and displayed in a single display screen and multiple display in which the specified range 103 is displayed in one of the

plurality of display areas, it is possible, for example, to display a menu on the screen when the specified range 103 is selected to thereby allow selection of the desired display mode from the menu.

Thus, after switching from the single display to the multiple display, the monitor 2 displays a monitor screen 110 shown in FIG. 11. The monitor screen 110 comprises display areas 111 and 33, the information display area 23, and the operation area 24; and the specified range 103 that is a portion near the edge of the ultrasonic image 102 is displayed enlarged in the display area 111. The ultrasonic image displayed in the display area 111 may be a scan image produced by the image producing section 12, or an ultrasonic image may be arbitrarily selected from the image database 15 and displayed. Thus, when the display is switched from the single display to the multiple display, a desired range is selected from the ultrasonic image displayed in the single display and the range is displayed in one of the plurality of the display areas, whereby a desired display condition can be directly achieved from the single display.

Next, rotation of the displayed range will be described. If the plurality of display areas are displayed at the same time, a plurality of ultrasonic images can be compared; but, to achieve the comparison more easily, it is desirable that the ultrasonic images be displayed at an arbitrary inclination. For example, when ultrasonic images of the right and left kidneys are to be compared, an ultrasonic image of one kidney is stored beforehand, and an ultrasonic image obtained by scanning the other kidney is compared with the stored ultrasonic image. However, since the ultrasonic probe 3 receives an echo signal based on the positional relationship with a subject to be examined and the ultrasonic image is produced based on the echo signal, the two ultrasonic images are not always acquired in the same direction. Accordingly, the location at which the ultrasonic probe is abutted is appropriately adjusted to acquire an image similar to the previously acquired ultrasonic image. The work for such a cumbersome operation can be reduced by an arbitrarily rotatable ultrasonic image.

FIG. 12 is an explanatory diagram for explaining an operation for rotating an ultrasonic image. In FIG. 12(a), a display area 101 displays an ultrasonic image 102. When a specified range 103 is selected in the ultrasonic image 102, rotation markers 121a, 121b, 121c and 121d indicating that the specified range is rotatable in the ultrasonic image 102 are displayed, as shown in FIG. 12(b). The user then selects one of the rotation markers 121a, 121b, 121c and 121d by operating the pointing device 3, and specifies an amount of rotation by moving the pointing device 3. The control section 18 transmits the amount of rotation specified by the operation of the pointing device 3 to the displayed range rotating section 16. The displayed range rotating section 16 rotates the specified range based on the received amount of rotation, and then displays a specified range 122 on the monitor 2 as shown in FIG. 12(c). A specific operation for this is as follows, for example: a mouse is employed as the pointing device 3, the position is adjusted to the rotation marker 121a, and a predetermined button on the mouse is pressed to select the rotation marker 121a. Then, the mouse is moved with the button pressed (the mouse is dragged) to rotate the specified range 103 as the rotation marker 121a follows the movement of the mouse.

After the user has specified a desired amount of rotation, the display area forming section 17 switches the screen display from the single display to the multiple display, and displays the specified range after the rotation in one of the plurality of display areas. FIG. 13 is an explanatory diagram

13

for explaining the ultrasonic image displayed after the rotation. In FIG. 13, a monitor screen 130 comprises display areas 131 and 33, the information display area 23, and the operation area 24; and a displayed range 132 is displayed in the display area 131 and the ultrasonic image 34 is displayed in the display area 33. The displayed range 132 is identical to the specified range 122 determined in FIG. 12(c), and represents an image obtained by rotating the ultrasonic image to a desired angle. Thus, by rotating the display area using the pointing device, a desired displayed range can be easily displayed at a desired angle.

The rotation of the displayed range can be done arbitrarily on an ultrasonic image(s) being displayed in the single display or multiple display. Moreover, the rotation operation can be added to the switching from the single display to the multiple display. By adding the rotation operation to the switching from the single display to the multiple display, an ultrasonic image of a desired displayed range at a desired angle can be displayed by a single operation.

As described above, in the ultrasonic image display apparatus in accordance with the present embodiment, an ultrasonic image based on an echo signal received by the ultrasonic probe 3 is produced by the image producing section 12, a display area is formed on the screen by the display area forming section 17, a displayed range of the ultrasonic image to be displayed in the display area is selected by the displayed range selecting section 14, and scrolling of a selected range and rotation of the displayed range are achieved by the displayed range moving section 15 and displayed range rotating section 16, respectively, based on a position on the monitor screen specified by the pointing device 3; and therefore, a portion displayed on the monitor can be scrolled and rotated to allow use of the whole ultrasonic image in a limited display area, thus improving monitor display condition operating ease.

Although the preceding description of the embodiment has been made on a case in which two display areas are formed as an example of the multiple display and movement and rotation of the displayed range are performed on one of the two display areas, the number of display areas in the multiple display is not limited to two but any number may be used, and the movement and rotation operations on the displayed range may be performed on any one of the number of the display areas.

Moreover, while the description has been made on a case in which the mouse is employed as the pointing device 3 in the embodiment, any input device capable of inputting a position on the monitor screen, such as a trackball or cursor key, may be used.

What is claimed is:

1. An ultrasonic image display apparatus for producing an ultrasonic image based on an echo signal received by an ultrasonic probe and displaying said ultrasonic image on a monitor, said apparatus comprising:

- display area forming means for forming on a screen of said monitor a display area;
- displayed range selecting means for selecting a first displayed range to be displayed in said display area from said ultrasonic image;
- displayed range moving means for conducting movement of said first displayed range of said ultrasonic image;
- movement instruction inputting means for inputting a direction and an amount of movement of said first displayed range to said displayed range moving means; and
- a position specifying means configured to be moved from a first position within said display area to a second

14

position outside said display area, wherein when said position specifying means is moved from the first position within said display area to the second position outside said display area, a second displayed range from said ultrasonic image is displayed in said display area, and said second displayed range includes image data not included within the first displayed range.

2. The ultrasonic image display apparatus of claim 1, wherein said position specifying means specifies an arbitrary position on said monitor screen, and when the position specified by said position specifying means is moved from within said display area to the outside of said display area, said displayed range moving means conducts movement of said first displayed range according to the amount of said movement.

3. The ultrasonic image display apparatus of claim 1, further comprising a single user interface that operates as said movement instruction inputting means or said position specifying means by switching its operation.

4. The ultrasonic image display apparatus of claim 1, wherein said display area forming means is capable of switching display between single display in which a single display area is formed on said monitor screen and multiple display in which a plurality of display areas are formed on said monitor screen.

5. The ultrasonic image display apparatus of claim 1, wherein said ultrasonic image display apparatus further comprises image storing means for storing an ultrasonic image converted from said echo signal as still image data, and said displayed range selecting means selects an ultrasonic image to be displayed and its displayed range from among said ultrasonic image converted from said echo signal and ultrasonic images stored in said image storing means.

6. The ultrasonic image display apparatus of claim 1, wherein when said display area forming means forms a plurality of display areas, said displayed range selecting means selects ultrasonic images to be displayed and their displayed ranges respectively for said plurality of display areas.

7. The ultrasonic image display apparatus of claim 4, wherein when said display area forming means switches display from the single display to the multiple display, said displayed range selecting means selects part of the ultrasonic image displayed in the single display as said first displayed range, and displays said first displayed range in at least one of said plurality of display areas.

8. The ultrasonic image display apparatus of claim 1, further comprising displayed range rotating means for rotating said first displayed range of said ultrasonic image.

9. An ultrasonic image display method for producing an ultrasonic image based on an echo signal received by an ultrasonic probe and displaying said ultrasonic image on a monitor, said method comprising the steps of:

- forming on a screen of said monitor a display area in which at least part of said ultrasonic image is displayed;
- selecting a first displayed range to be displayed in said display area from said ultrasonic image;
- conducting movement of said first displayed range of said ultrasonic image;
- inputting a direction and an amount of the movement of said first displayed range to a displayed range moving means;
- moving from a first position within said display area to a second position outside said display area; and
- displaying, from said ultrasonic image, a second displayed range within said display area when said mov-

15

ing from a first position within said display area to a second position outside said display area occurs, wherein said second displayed range includes image data not included within said first displayed range.

10. The ultrasonic image display method of claim 9, 5 wherein said ultrasonic image display method further comprises a position specifying step of specifying an arbitrary position on said monitor screen, and when the position specified by said position specifying step is moved from within said display area to the outside of said display area, 10 said conducting movement step conducts movement of said first displayed range according to the amount of said movement.

11. The ultrasonic image display method of claim 9, 15 wherein said conducting movement step and said inputting a direction step are executed by a single user interface.

12. The ultrasonic image display method of claim 9, 20 wherein said forming on a screen step is capable of switching display between single display in which a single display area is formed on said monitor screen and multiple display in which a plurality of display areas are formed on said monitor screen.

13. The ultrasonic image display method of claim 12, 25 wherein when said forming on a screen step switches display from the single display to the multiple display, said selecting a first displayed range step selects part of the ultrasonic image displayed in the single display as said first displayed range, and displays said first displayed range in at least one of said plurality of display areas.

14. The ultrasonic image display method of claim 9, 30 wherein said ultrasonic image display method further comprises an image storing step of storing an ultrasonic image converted from said echo signal as still image data, and said selecting a first displayed range step selects an ultrasonic image to be displayed and said first displayed range from 35 among said ultrasonic image converted from said echo a ultrasonic images stored by said image storing step.

15. The ultrasonic image display method of claim 9, 40 wherein when said forming on a screen step forms a plurality of display areas, said selecting a first displayed range step selects ultrasonic images to be displayed and their displayed ranges respectively for said plurality of display areas.

16. The ultrasonic image display method of claim 9, further comprising a displayed range rotating step of rotating said first displayed range of said ultrasonic image.

16

17. An ultrasonic image display apparatus for producing an ultrasonic image based on an echo signal received by an ultrasonic probe and displaying the ultrasonic image on a monitor, said apparatus comprising:

a display area forming section configured to form on a screen of said monitor a display area;

a displayed range selecting section configured to enable a selection of a first displayed range to be displayed in said display area from the ultrasonic image;

a displayed range moving section configured to enable a movement of the first displayed range of the ultrasonic image;

a movement instruction inputting section configured to enable inputting a direction and an amount of movement of the first displayed range; and

a position specifying section configured to be moved from a first position within said display area to a second position outside said display area, wherein when said position specifying section is moved from the first position within said display area to the second position outside said display area, a second displayed range from said ultrasonic image is displayed in said display area, and said second displayed range includes image data not included within the first displayed range.

18. The ultrasonic image display apparatus of claim 17, wherein said position specifying section is further configured to enable specifying an arbitrary position on said monitor screen, and when the position specified by said position specifying section is moved from within said display area to the outside of said display area, said displayed range moving means conducts movement of the first displayed range according to the amount of the movement.

19. The ultrasonic image display apparatus of claim 17, wherein said display area forming section is further configured to enable switching between a single display in which a single display area is formed on said monitor screen and a multiple display in which a plurality of display areas are formed on said monitor screen.

20. The ultrasonic image display apparatus of claim 17, further comprising a displayed range rotating section for rotating the first displayed range of the ultrasonic image.

* * * * *

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : 6,743,176 B2
DATED : June 1, 2004
INVENTOR(S) : Sei Kato

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

Column 15,

Line 36, after "echo" delete "a" and insert -- signal and --.

Signed and Sealed this

Second Day of May, 2006

A handwritten signature in black ink on a light gray dotted background. The signature is written in a cursive style and reads "Jon W. Dudas".

JON W. DUDAS

Director of the United States Patent and Trademark Office

专利名称(译)	超声波图像显示装置和超声波图像显示方法		
公开(公告)号	US6743176	公开(公告)日	2004-06-01
申请号	US10/417482	申请日	2003-04-17
[标]申请(专利权)人(译)	加藤SEI		
申请(专利权)人(译)	加藤SEI		
当前申请(专利权)人(译)	通用电气医疗系统全球性技术公司，有限责任公司		
[标]发明人	KATO SEI		
发明人	KATO, SEI		
IPC分类号	A61B8/00 G01S7/52 G01S15/89 G09G5/00 G09G5/14 G09G5/34 H04N7/18		
CPC分类号	A61B8/00 A61B8/462		
优先权	2002115973 2002-04-18 JP		
其他公开文献	US20030199766A1		
外部链接	Espacenet USPTO		

摘要(译)

为了改善监视器显示状态操作的容易性并且能够容易地显示任意位置，由图像产生部分12产生基于由超声探头3接收的回波信号的超声图像，在屏幕上形成显示区域通过显示区域形成部分17，由显示区域选择部分14选择要在显示区域中显示的超声图像的显示范围，并且通过显示范围实现所选范围的滚动和显示范围的旋转。移动部分15和显示范围旋转部分16分别基于由指示设备3指定的监视器屏幕上的位置。

