



US 20180272159A1

(19) **United States**(12) **Patent Application Publication**
Slayton et al.(10) **Pub. No.: US 2018/0272159 A1**(43) **Pub. Date: Sep. 27, 2018**(54) **ULTRASOUND PROBE FOR FAT AND
CELLULITE REDUCTION****Publication Classification**(71) Applicant: **Guided Therapy Systems, LLC**, Mesa,
AZ (US)(72) Inventors: **Michael H. Slayton**, Tempe, AZ (US);
Peter G. Barthe, Phoenix, AZ (US);
Inder Raj S. Makin, Mesa, AZ (US)(21) Appl. No.: **15/996,295**(22) Filed: **Jun. 1, 2018****Related U.S. Application Data**

(63) Continuation of application No. 15/821,281, filed on Nov. 22, 2017, now Pat. No. 10,010,725, which is a continuation of application No. 15/650,246, filed on Jul. 14, 2017, now Pat. No. 9,827,450, which is a continuation of application No. 15/374,918, filed on Dec. 9, 2016, now Pat. No. 9,707,412, which is a continuation of application No. 15/041,829, filed on Feb. 11, 2016, now Pat. No. 9,522,290, which is a continuation of application No. 14/550,720, filed on Nov. 21, 2014, now Pat. No. 9,283,410, which is a continuation of application No. 14/164,598, filed on Jan. 27, 2014, now Pat. No. 8,915,854, which is a continuation of application No. 13/789,562, filed on Mar. 7, 2013, now Pat. No. 8,636,665, which is a continuation of application No. 13/356,405, filed on Jan. 23, 2012, now Pat. No. 8,672,848, which is a continuation of application No. 11/163,154, filed on Oct. 6, 2005, now Pat. No. 8,133,180.

(60) Provisional application No. 60/616,753, filed on Oct. 6, 2004.

(51) **Int. Cl.**

A61N 7/02 (2006.01)
G01S 15/89 (2006.01)
A61B 8/08 (2006.01)
A61B 8/14 (2006.01)
A61B 8/00 (2006.01)
A61N 7/00 (2006.01)
A61B 90/00 (2016.01)


(52) **U.S. Cl.**


CPC *A61N 7/02* (2013.01); *H05K 999/99*
(2013.01); *G01S 15/8936* (2013.01); *G01S*
15/8906 (2013.01); *A61B 8/483* (2013.01);
A61B 8/14 (2013.01); *A61N 2007/0008*
(2013.01); *A61N 7/00* (2013.01); *A61B 8/461*
(2013.01); *A61B 8/4483* (2013.01); *A61B*
2090/378 (2016.02); *A61B 8/4455* (2013.01);
A61B 8/429 (2013.01)

(57)

ABSTRACT

A method and system for providing ultrasound treatment to a tissue that contains a lower part of dermis and proximal protrusions of fat lobuli into the dermis. An embodiment delivers ultrasound energy to the region creating a thermal injury and coagulating the proximal protrusions of fat lobuli, thereby eliminating the fat protrusions into the dermis. An embodiment can also include ultrasound imaging configurations using the same or a separate probe before, after or during the treatment. In addition various therapeutic levels of ultrasound can be used to increase the speed at which fat metabolizes. Additionally the mechanical action of ultrasound physically breaks fat cell clusters and stretches the fibrous bonds. Mechanical action will also enhance lymphatic drainage, stimulating the evacuation of fat decay products.

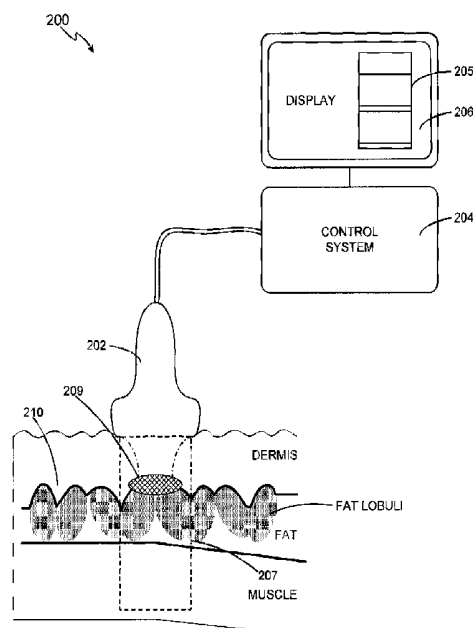

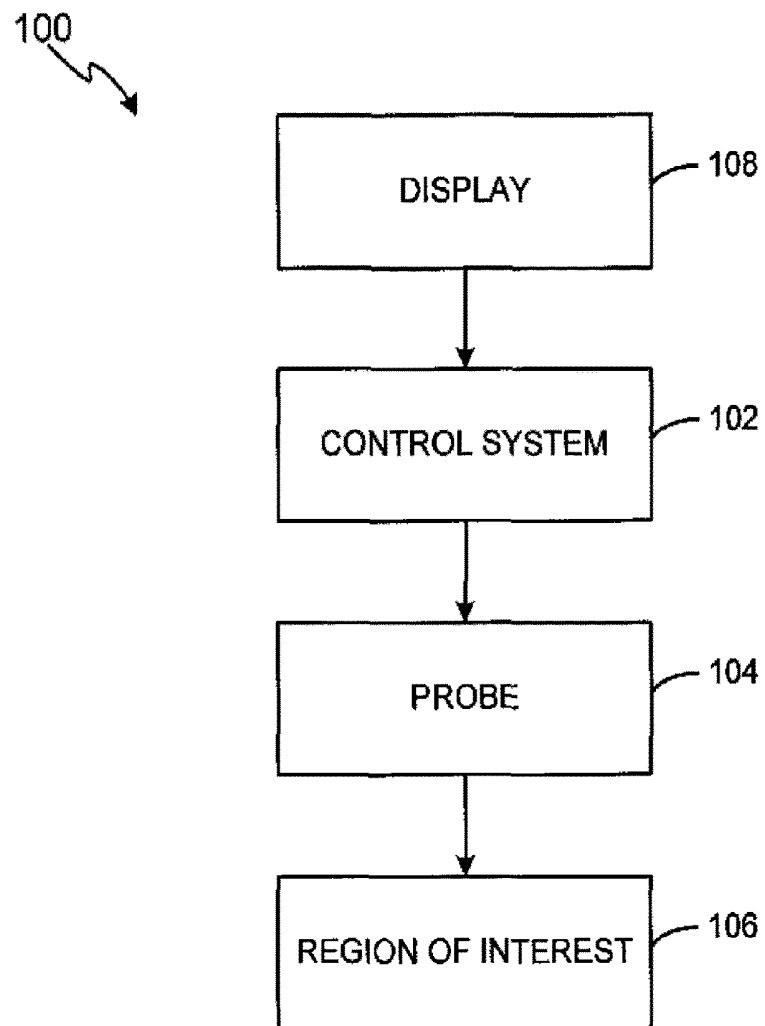**FIG. 1**

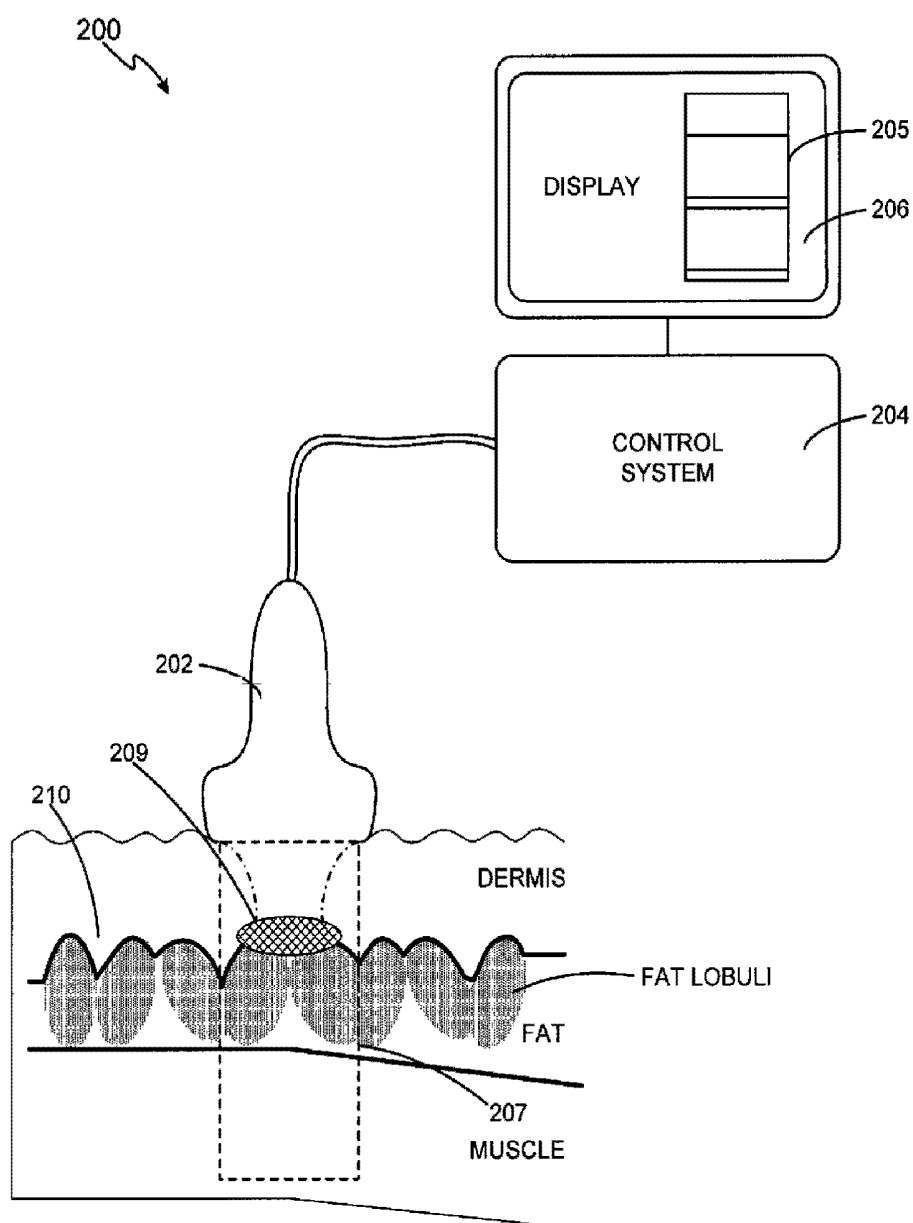


FIG. 2

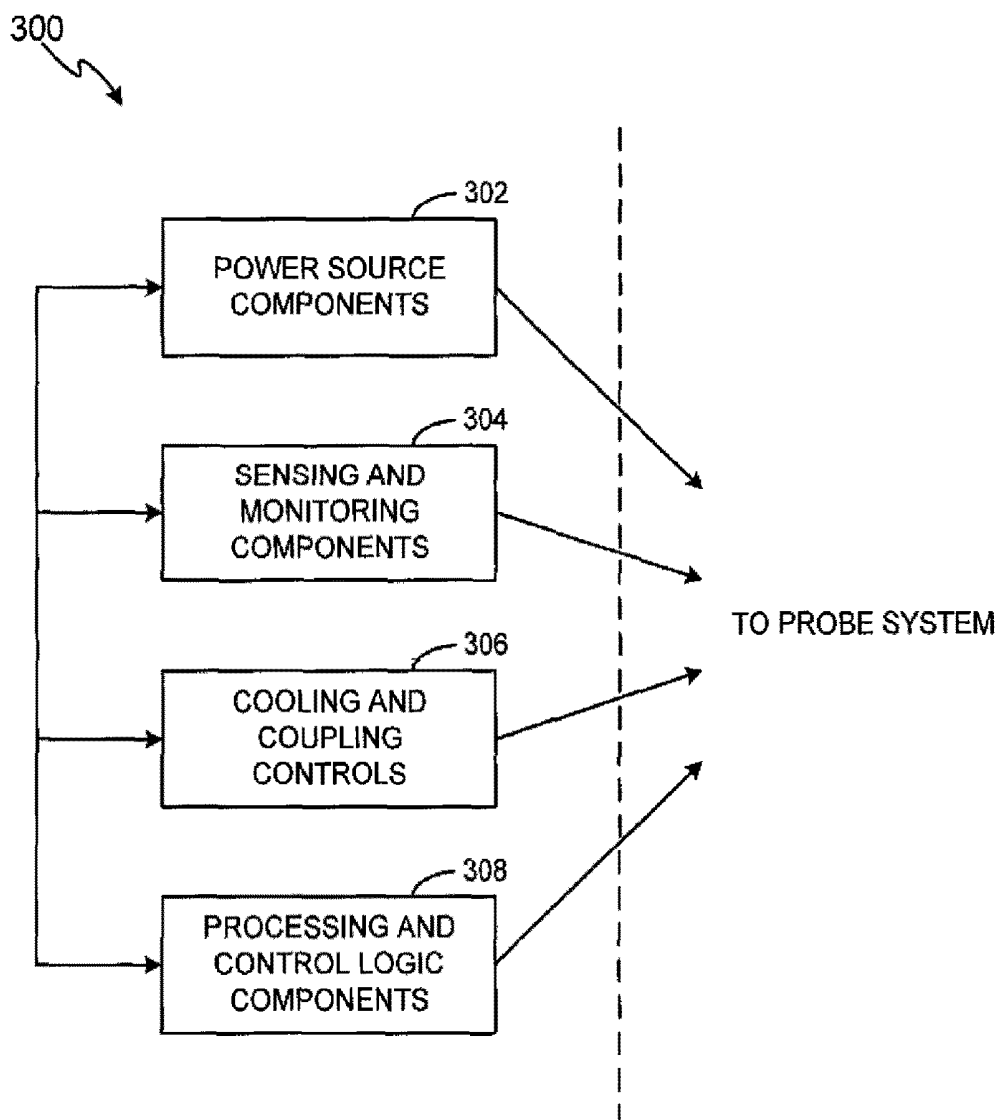


FIG. 3A

300 ↘

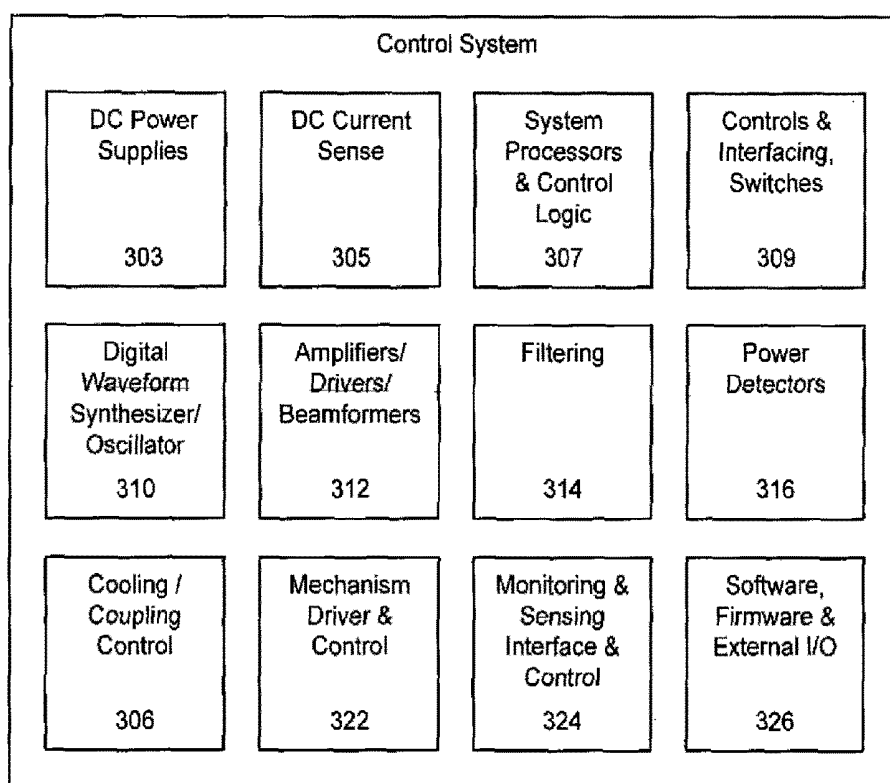


FIG. 3B

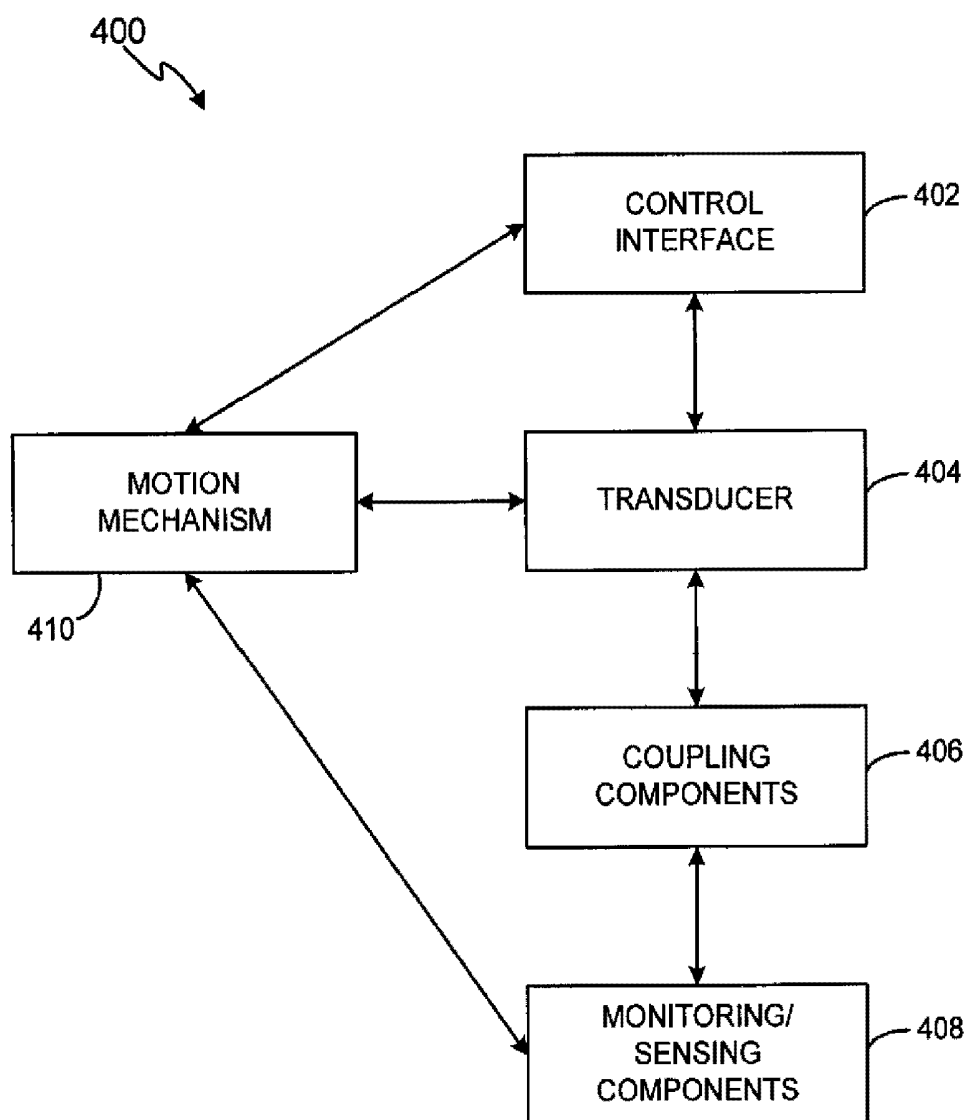


FIG. 4A

400

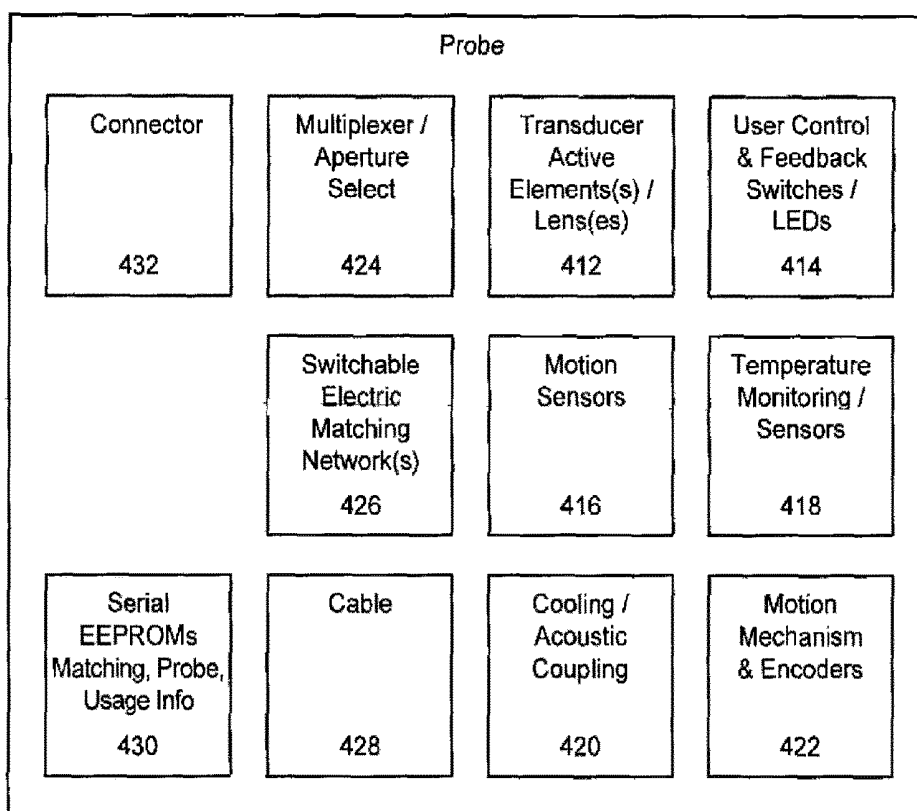



FIG. 4B

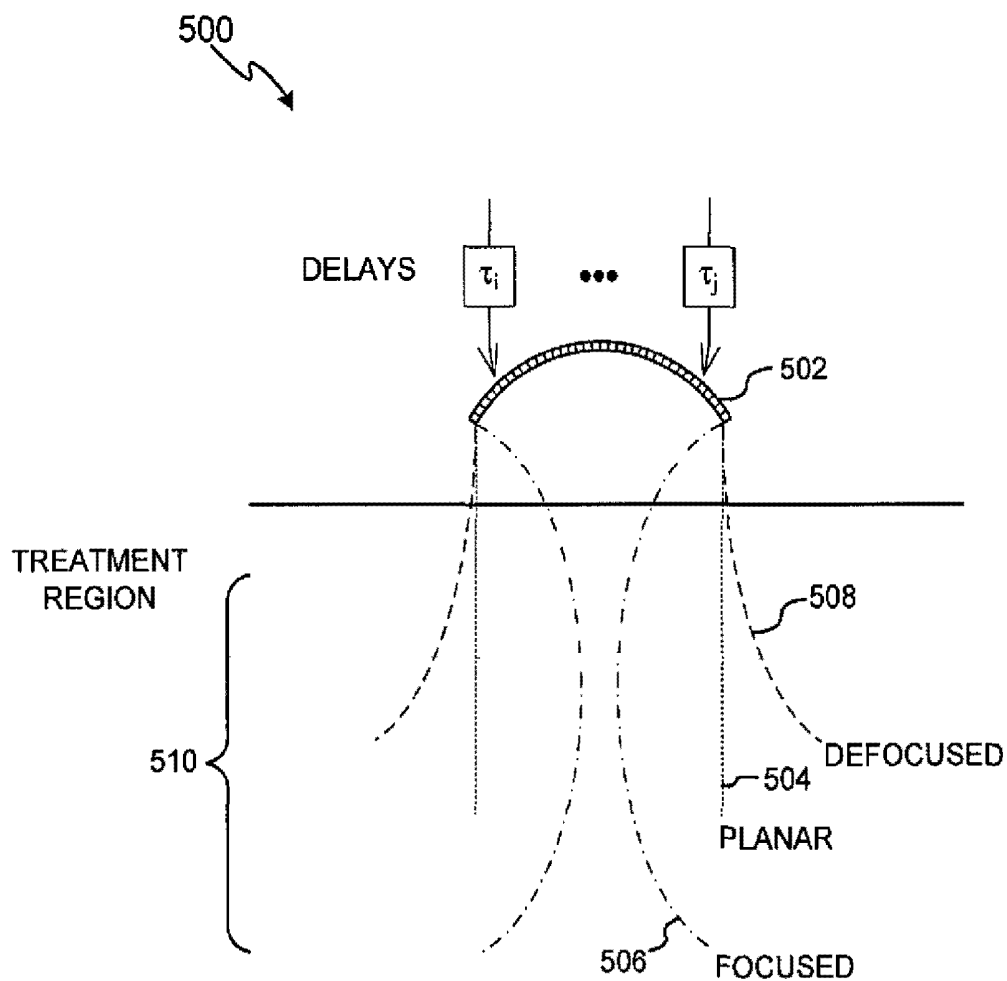


FIG. 5

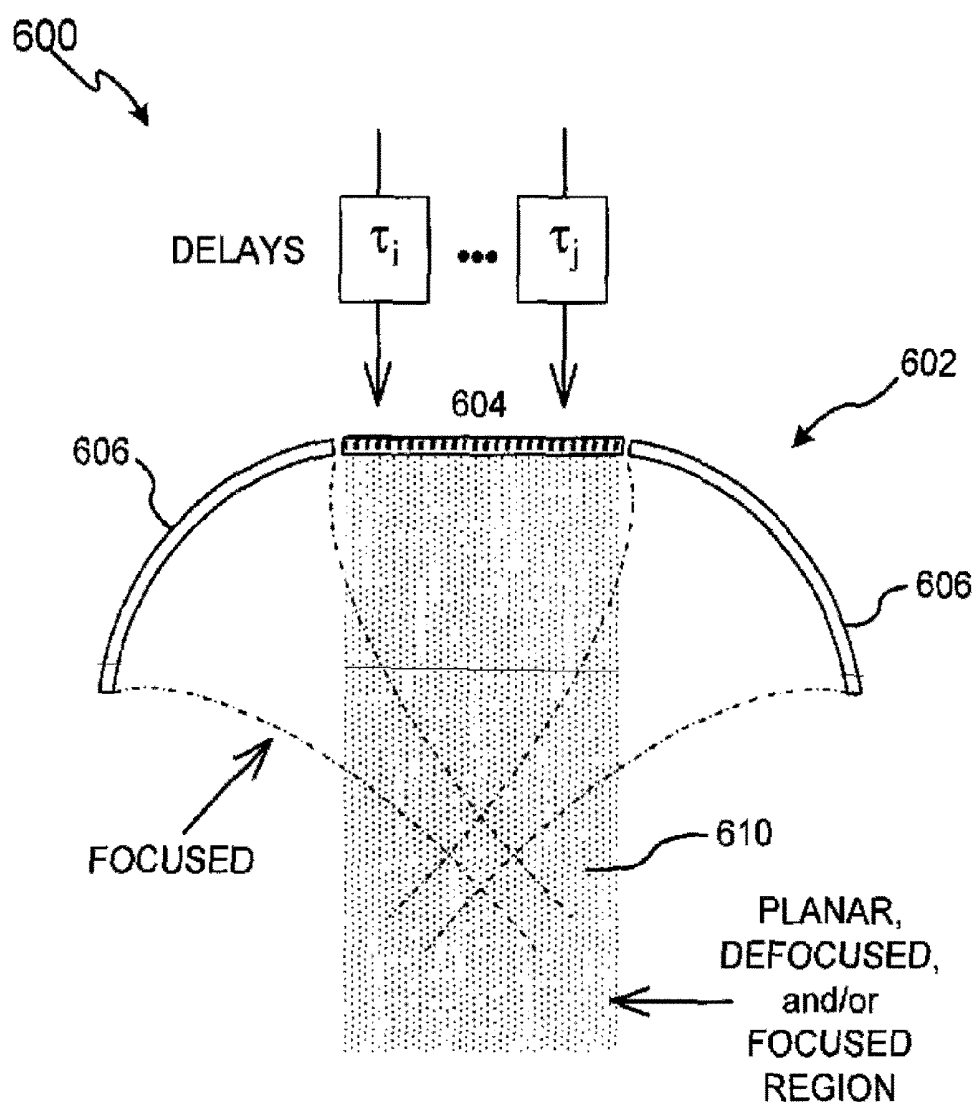


FIG. 6A

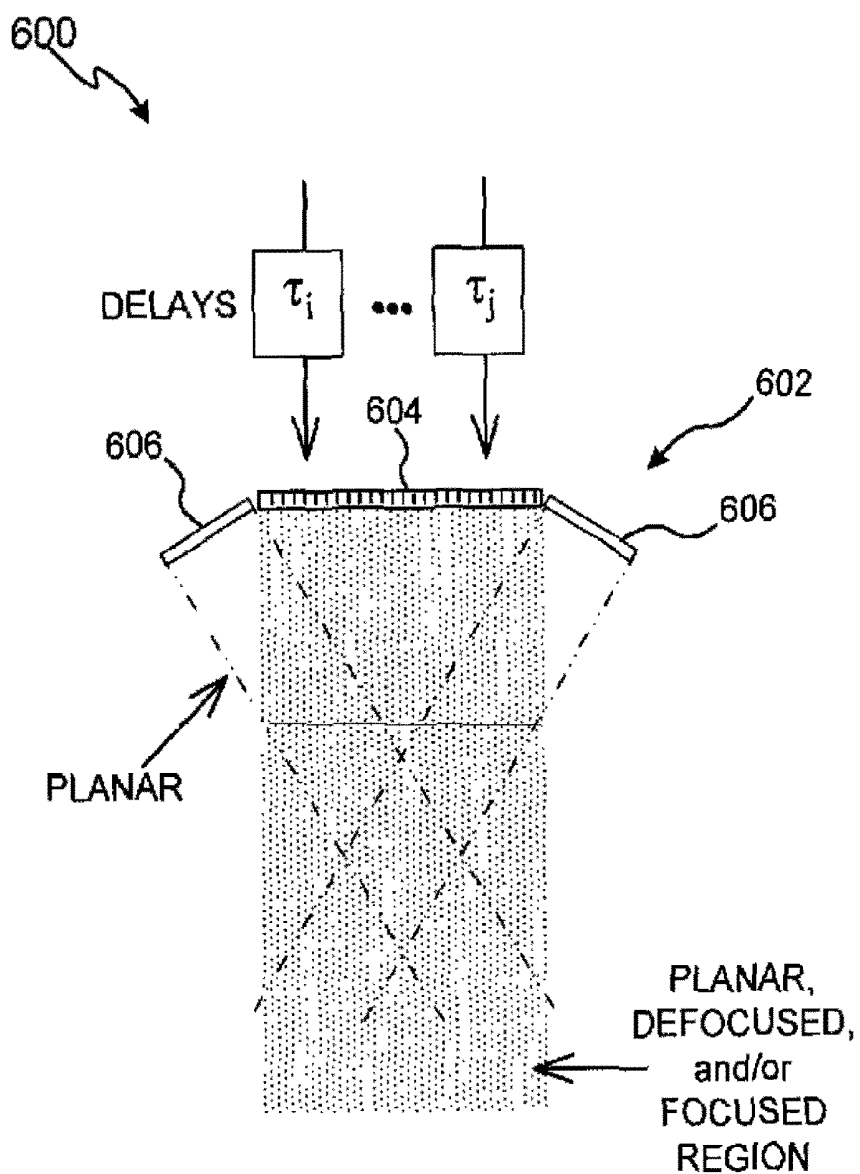


FIG. 6B

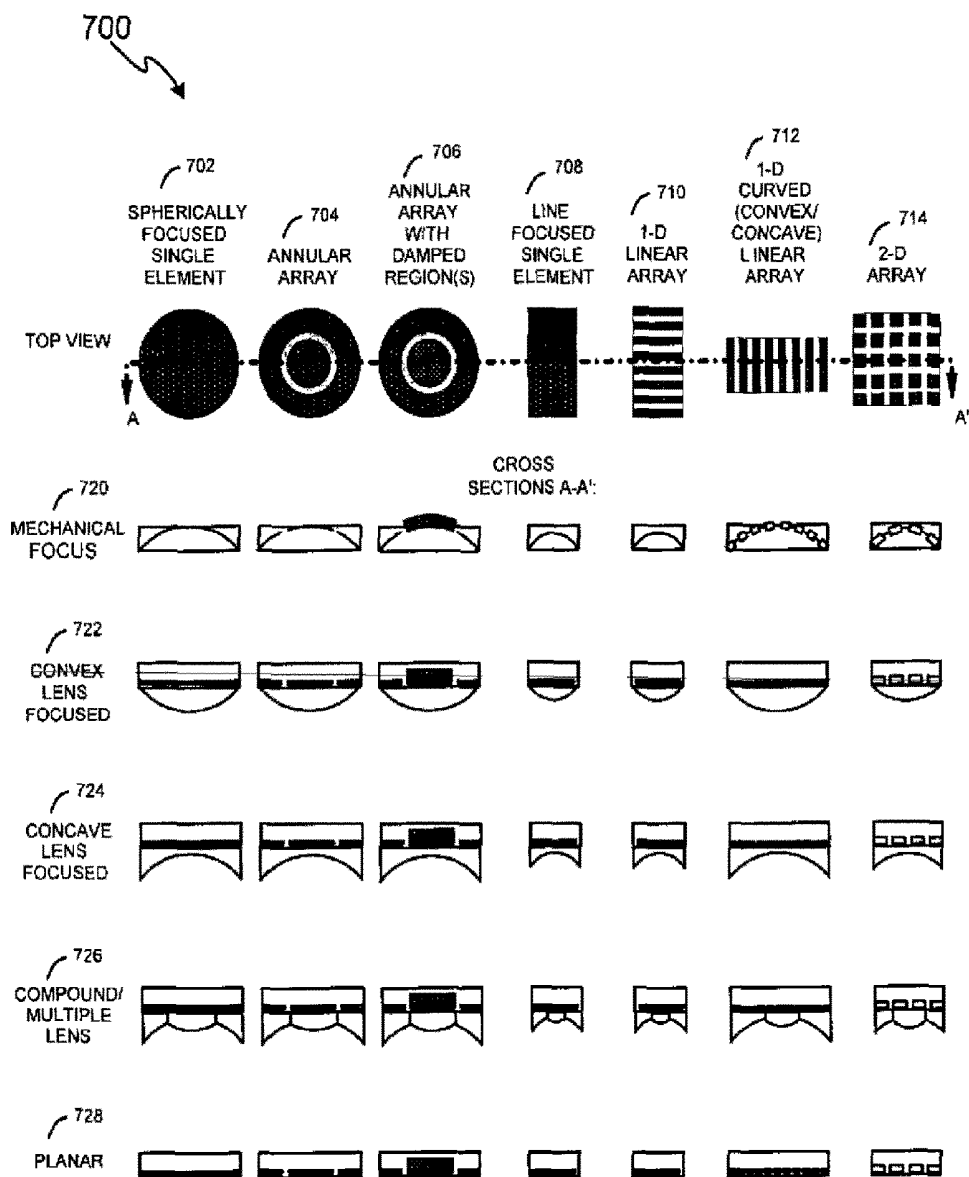


FIG. 7

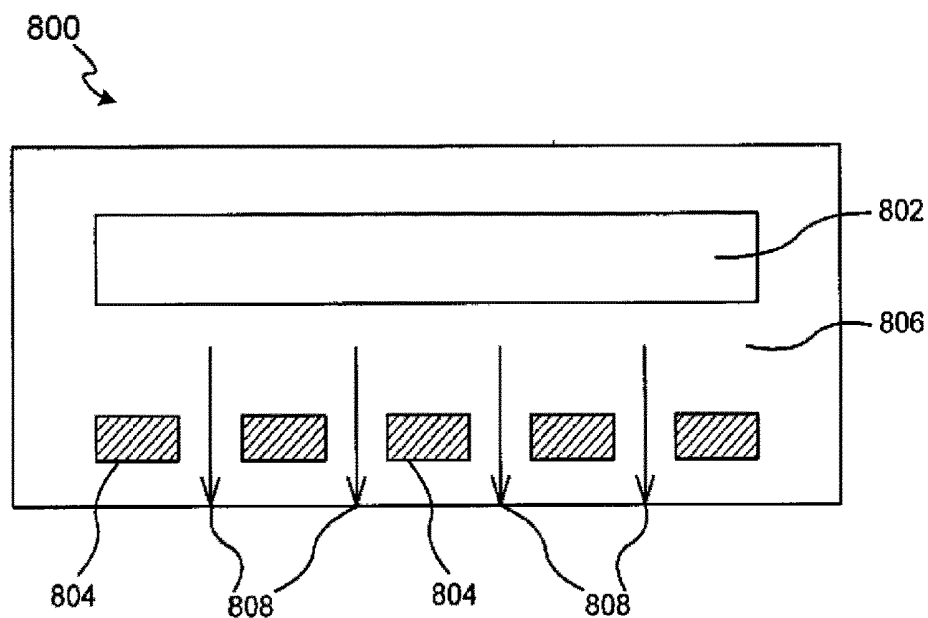


FIG. 8A

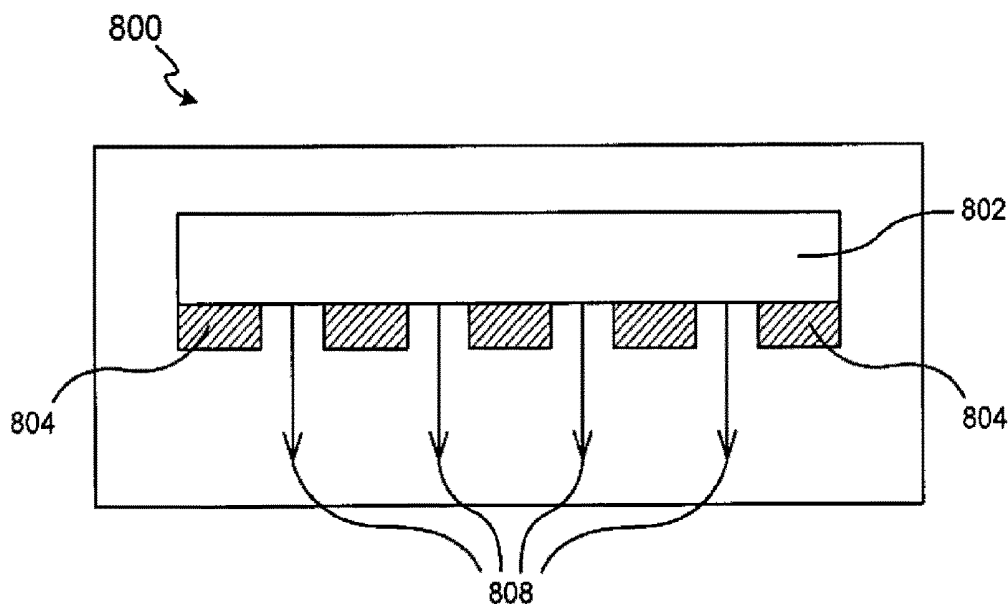


FIG. 8B

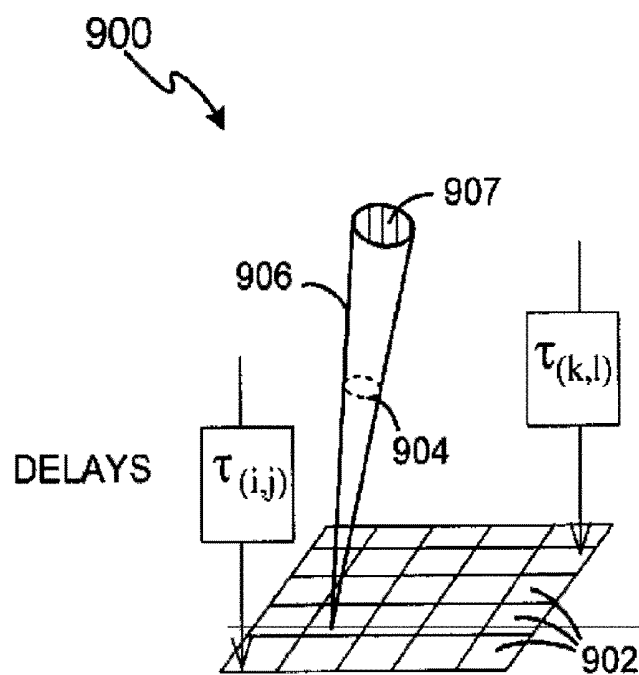


FIG. 9

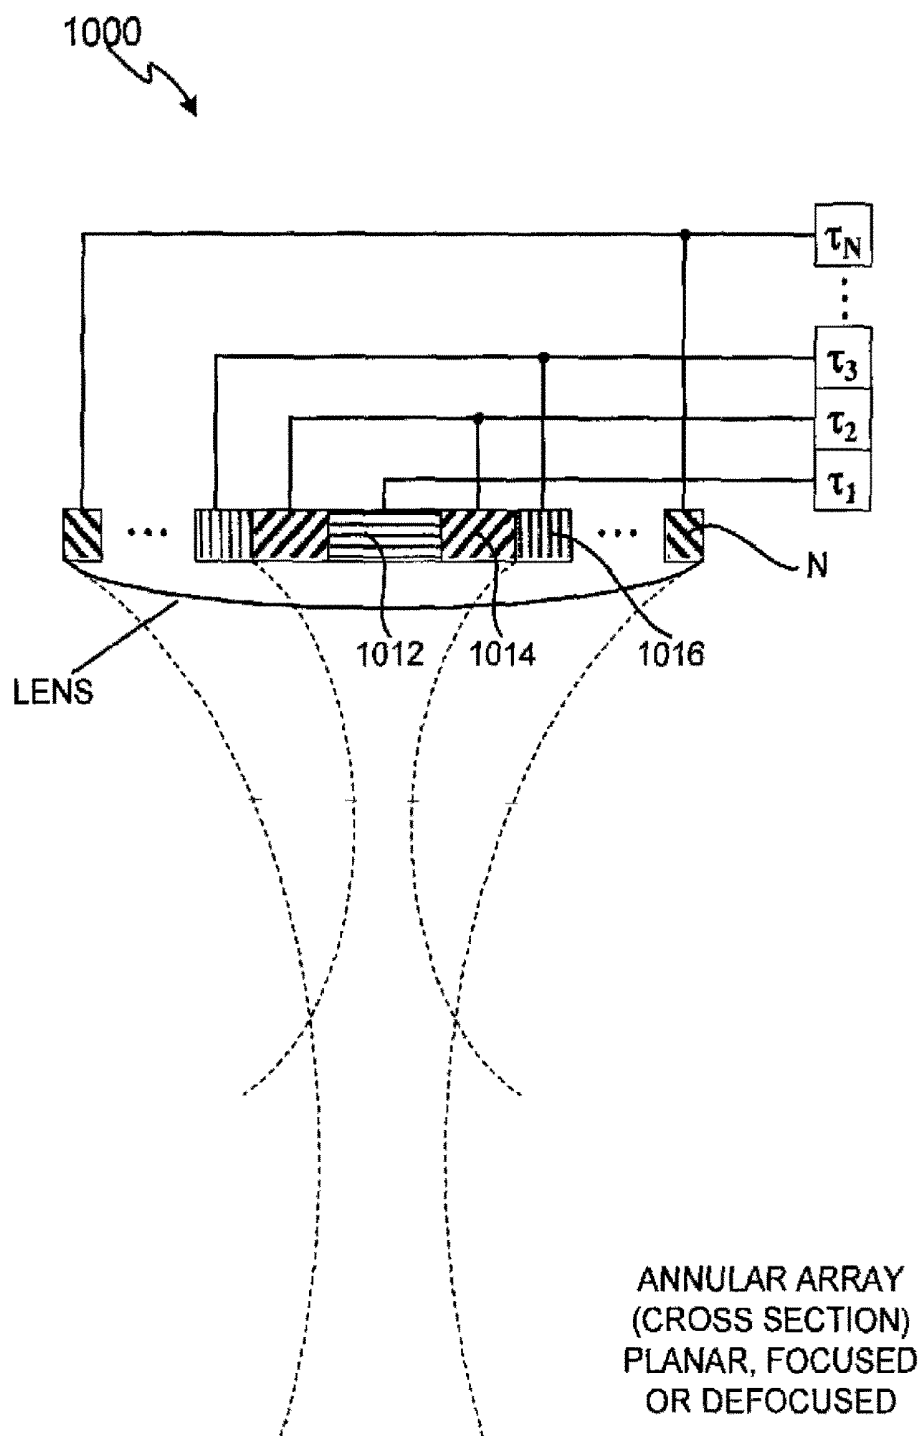


FIG. 10A

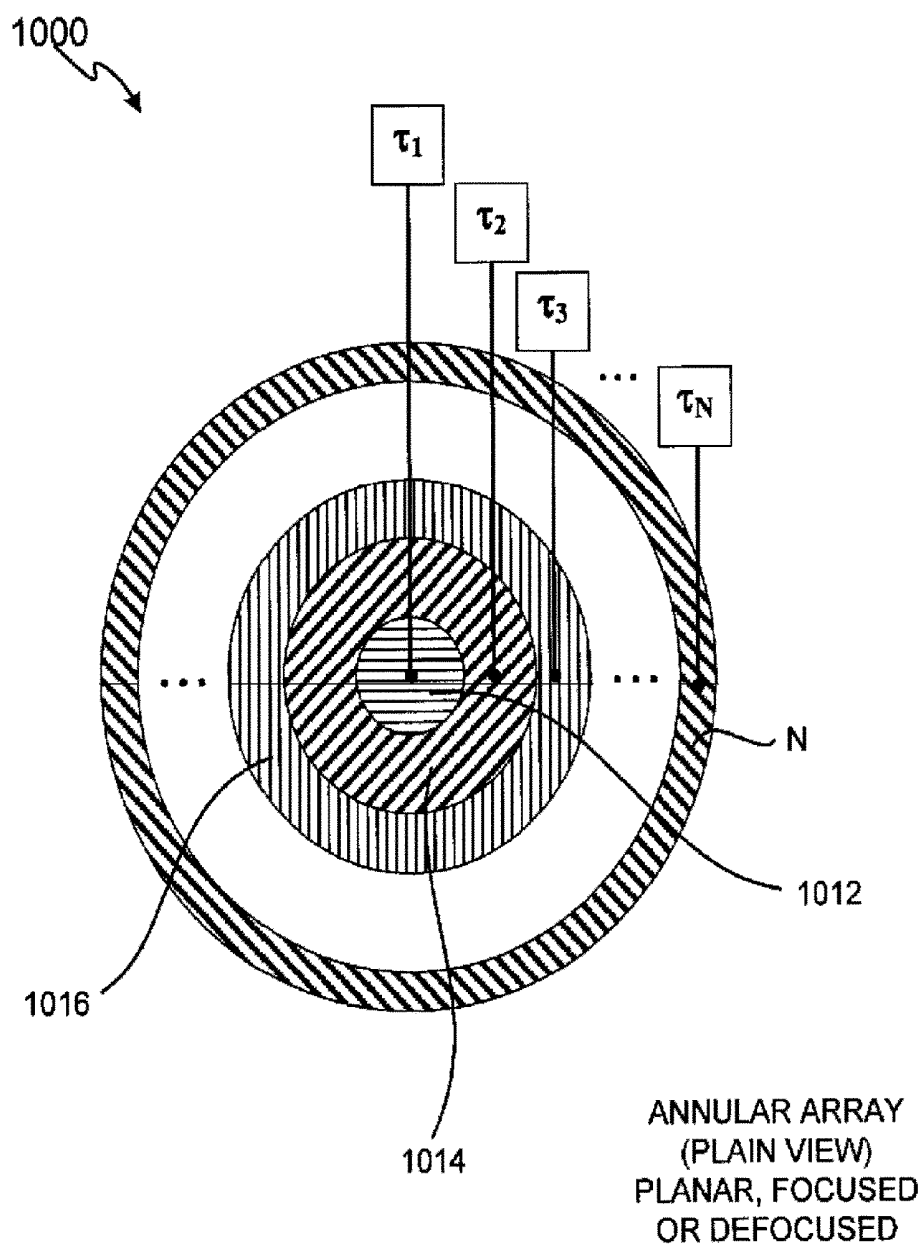


FIG. 10B

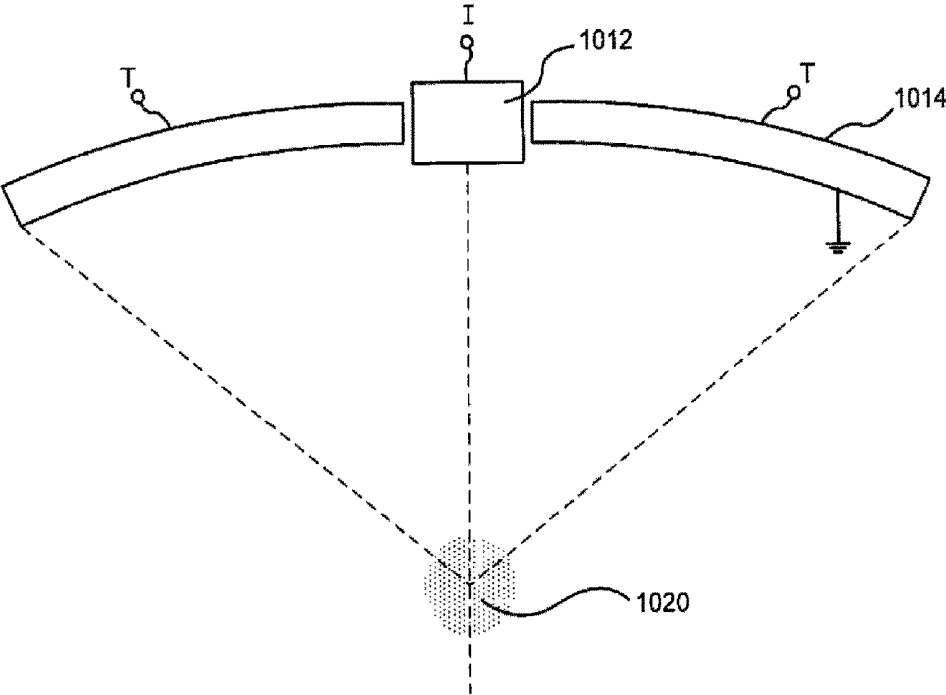


FIG. 10C

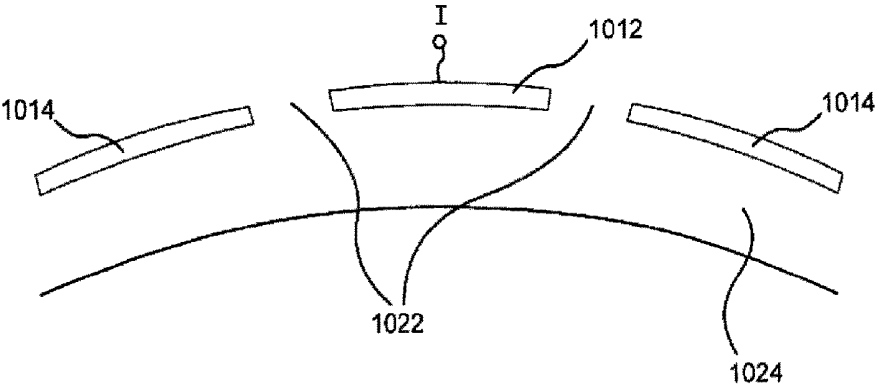


FIG. 10D

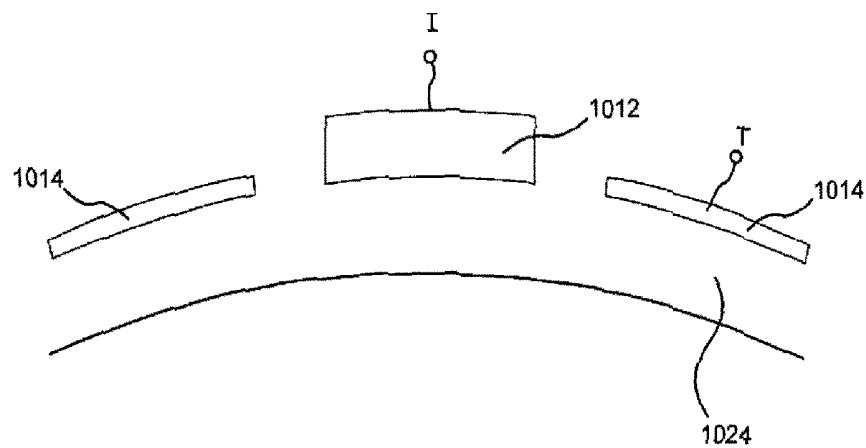


FIG. 10E

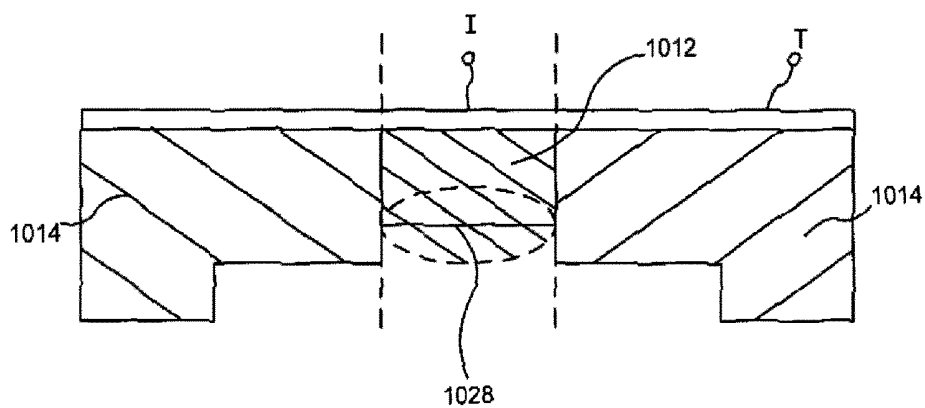


FIG. 10F

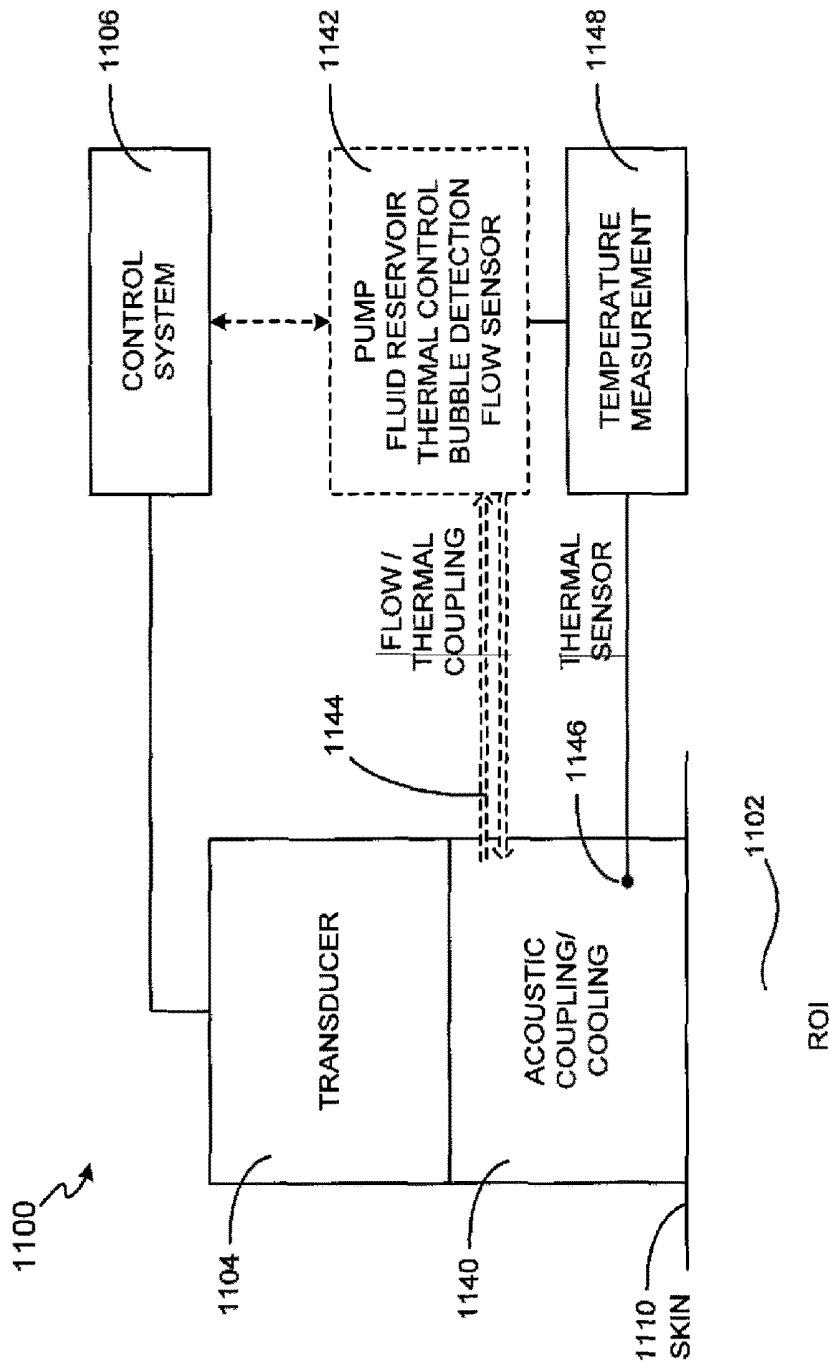


FIG. 11

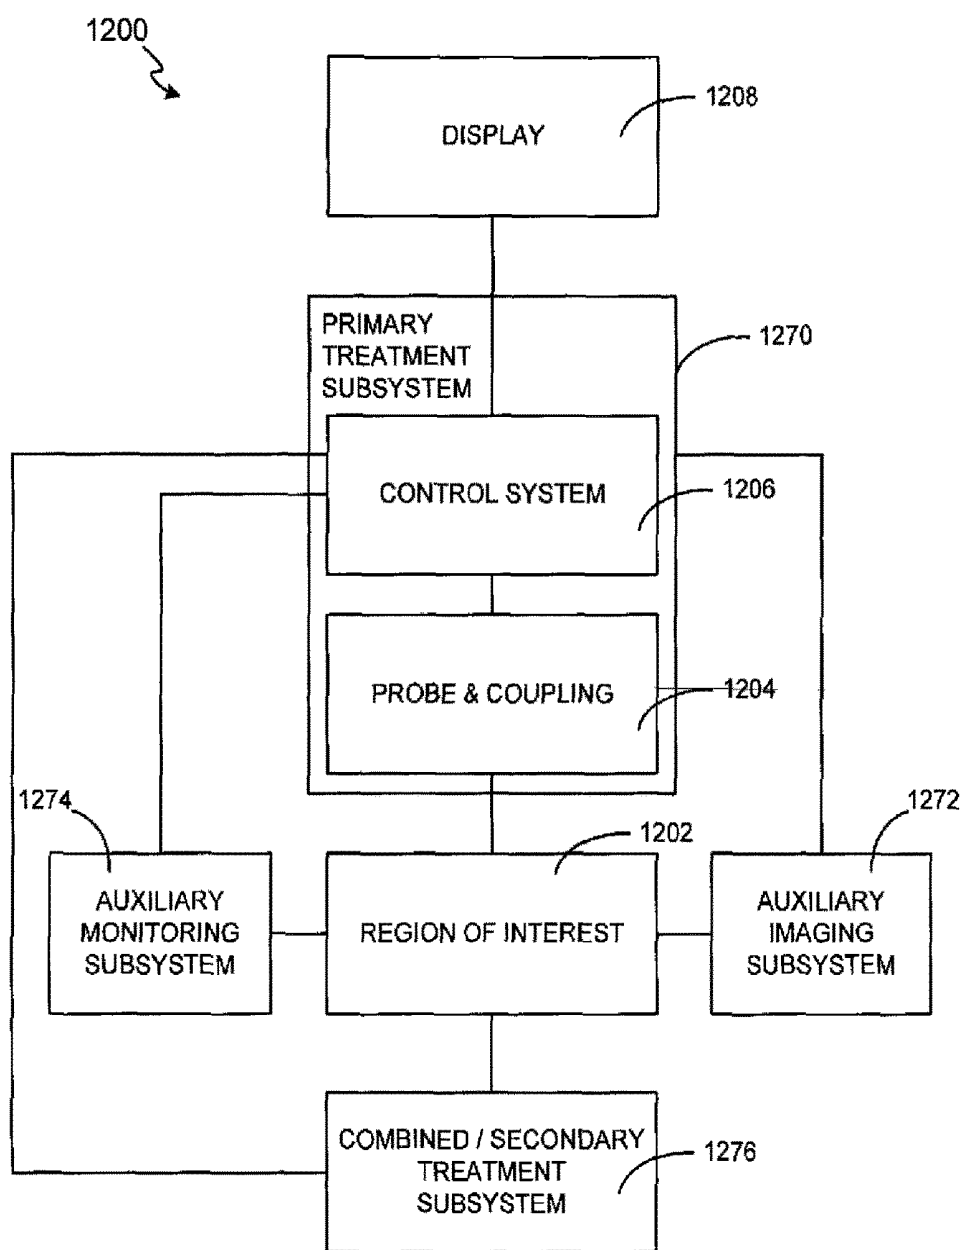


FIG. 12

ULTRASOUND PROBE FOR FAT AND CELLULITE REDUCTION

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application is a continuation of U.S. patent application Ser. No. 15/821,281 filed Nov. 22, 2017, which is a continuation of U.S. patent application Ser. No. 15/650,246 filed Jul. 14, 2017, now U.S. Pat. No. 9,827,450, which is a continuation of U.S. patent application Ser. No. 15/374,918 filed Dec. 9, 2016, now U.S. Pat. No. 9,707,412, which is a continuation of U.S. application Ser. No. 15/041,829 filed Feb. 11, 2016, now U.S. Pat. No. 9,522,290, which is a continuation of U.S. application Ser. No. 14/550,720 filed Nov. 21, 2014, now U.S. Pat. No. 9,283,410, which is a continuation of U.S. application Ser. No. 14/164,598 filed Jan. 27, 2014, now U.S. Pat. No. 8,915,854, which is a continuation of U.S. application Ser. No. 13/789,562 filed Mar. 7, 2013, now U.S. Pat. No. 8,636,665, which is a continuation of U.S. application Ser. No. 13/356,405 filed Jan. 23, 2012, now U.S. Pat. No. 8,672,848, which is a continuation of U.S. application Ser. No. 11/163,154 filed on Oct. 6, 2005, now U.S. Pat. No. 8,133,180, which claims the benefit of priority to U.S. Provisional No. 60/616,753, filed on Oct. 6, 2004, each of which are hereby incorporated by reference in their entirety herein. Any and all priority claims identified in the Application Data Sheet, or any correction thereto, are hereby incorporated by reference under 37 CFR 1.57.

BACKGROUND

Field of the Invention

[0002] The present invention relates to ultrasound therapy systems, and in particular to a method and system for treating cellulite.

Description of the Related Art

[0003] Cellulite is a common skin disorder that appears as an irregularity of skin contour, often characterized by a dimple appearance of the skin. This condition affects 80% of women worldwide and tends to gather superficially around the thighs, hips, and buttocks.

[0004] Cellulite develops in the body when fat is deposited immediately below the dermis and contained in fat chambers (lobuli) that can become swollen. As the fat cells grow in size, lobuli tend to protrude into a dermis layer, surrounding tissue becomes compressed and hardened, making blood circulation more difficult in trapping fluids. Reduced elasticity of the adipose tissue produces an undesirable tension between the layers. The resulting protrusions and depressions of connective tissue anchor points create the appearance of cellulite.

[0005] This condition responds with varying results to invasive procedures, such as liposuction. The non-invasive technologies such as massagers, and low frequency ultrasound diathermy, show marginal results. Preliminary results shown by combination of infrared light and RF energy have some promise of improving skin contours, but significant progress is needed.

SUMMARY

[0006] In accordance with various aspects of the present invention, a method and system for non-invasive treatment of cellulite with ultrasound are provided. An exemplary treatment method and system comprises a therapeutic ultrasound system for providing ultrasound treatment to a deep tissue region that contains a lower part of dermis and proximal protrusions of fat lobuli into the dermis. Such an exemplary treatment system delivers conformal ultrasound therapeutic energy to the region creating a thermal injury and coagulating the proximal protrusions of fat lobuli, thereby eliminating the fat protrusions into the dermis the dermis resulting in improved appearance of the overlying superficial layers of the skin. In accordance with exemplary embodiments, an exemplary treatment system may include ultrasound imaging mechanisms using the same or a separate probe before, after or during the treatment. Other imaging configurations can be utilized to image, monitor, and provide feedback of ultrasound therapy, such as MRI, X-Ray, PET, infrared or others.

BRIEF DESCRIPTION OF THE DRAWINGS

[0007] The subject matter of the invention is particularly pointed out in the concluding portion of the specification. The invention, however, both as to organization and method of operation, may best be understood by reference to the following description taken in conjunction with the accompanying drawing figures, in which like parts may be referred to by like numerals:

[0008] FIG. 1 illustrates a block diagram of an exemplary ultrasound treatment system for treating cellulite in accordance with an exemplary embodiment of the present invention;

[0009] FIG. 2 illustrates a cross sectional diagram of an exemplary probe system in accordance with exemplary embodiments of the present invention;

[0010] FIGS. 3A and 3B illustrate block diagrams of an exemplary control system in accordance with exemplary embodiments of the present invention;

[0011] FIGS. 4A and 4B illustrate block diagrams of an exemplary probe system in accordance with exemplary embodiments of the present invention;

[0012] FIG. 5 illustrates a cross-sectional diagram of an exemplary transducer in accordance with an exemplary embodiment of the present invention;

[0013] FIGS. 6A and 6B illustrate cross-sectional diagrams of an exemplary transducer in accordance with exemplary embodiments of the present invention;

[0014] FIG. 7 illustrates exemplary transducer configurations for ultrasound treatment in accordance with various exemplary embodiments of the present invention;

[0015] FIGS. 8A and 8B illustrate cross-sectional diagrams of an exemplary transducer in accordance with another exemplary embodiment of the present invention;

[0016] FIG. 9 illustrates an exemplary transducer configured as a two-dimensional array for ultrasound treatment in accordance with an exemplary embodiment of the present invention;

[0017] FIGS. 10A-10F illustrate cross-sectional diagrams of exemplary transducers in accordance with other exemplary embodiments of the present invention;

[0018] FIG. 11 illustrates a schematic diagram of an acoustic coupling and cooling system in accordance with an exemplary embodiment of the present invention; and

[0019] FIG. 12 illustrates a block diagram of a treatment system comprising an ultrasound treatment subsystem combined with additional subsystems and methods of treatment monitoring and/or treatment imaging as well as a secondary treatment subsystem in accordance with an exemplary embodiment of the present invention.

DETAILED DESCRIPTION

[0020] The present invention may be described herein in terms of various functional components and processing steps. It should be appreciated that such components and steps may be realized by any number of hardware components configured to perform the specified functions. For example, the present invention may employ various medical treatment devices, visual imaging and display devices, input terminals and the like, which may carry out a variety of functions under the control of one or more control systems or other control devices. In addition, the present invention may be practiced in any number of medical contexts and that the exemplary embodiments relating to a non-invasive cellulite treatment system as described herein are merely indicative of exemplary applications for the invention. For example, the principles, features and methods discussed may be applied to any medical application. Further, various aspects of the present invention may be suitably applied to other applications.

[0021] In accordance with various aspects of the present invention, a non-invasive method and system for treating cellulite are provided. For example, in accordance with an exemplary embodiment, with reference to FIG. 1, an exemplary treatment system 100 configured to treat a region of interest 106 comprises a control system 102, an imaging/therapy probe with acoustic coupling 104, and a display system 108.

[0022] Control system 102 and display system 108 can comprise various configurations for controlling probe 104 and overall system 100 functionality, such as, for example, a microprocessor with software and a plurality of input/output devices, system and devices for controlling electronic and/or mechanical scanning and/or multiplexing of transducers, a system for power delivery, systems for monitoring, systems for sensing the spatial position of the probe and/or transducers, and/or systems for handling user input and recording treatment results, among others. Imaging/therapy probe 104 can comprise various probe and/or transducer configurations. For example, probe 104 can be configured for a combined dual-mode imaging/therapy transducer, coupled or co-housed imaging/therapy transducers, or simply a separate therapy probe and an imaging probe.

[0023] In accordance with an exemplary embodiment, treatment system 100 is configured for treating a deep tissue region that contains a lower part of dermis and proximal protrusions of fat lobuli into the dermis, by first, imaging of region of interest 106 for localization of the treatment area and surrounding structures, second, delivery of ultrasound energy at a depth, distribution, timing, and energy level to achieve the desired therapeutic effect, and third to monitor the treatment area before, during, and after therapy to plan and assess the results and/or provide feedback. As to the delivery of energy, control system 102 and transducer system 102 can be suitably configured to deliver conformal

ultrasound therapeutic energy to ROI 106 creating a thermal injury and coagulating the proximal protrusions of fat lobuli, thereby eliminating the fat protrusions into the dermis. As used herein, the term “dermis” refers to any part of the dermis and/or the epidermis.

[0024] In addition, by treatment of ROI 106, transducer system 102 may be configured to deliver one or more energy fields to promote one or more effects, for example, ablation of existing tissue, the breaking up of fat cell clusters, stretching of the fibrous bonds, enhancement of lymphatic drainage, stimulation of the evacuation of fat decay products, and/or enhanced cell permeability in order to treat cellulite.

[0025] An exemplary ultrasound therapy system of FIG. 1 is further illustrated in an exemplary embodiment in FIG. 2. A therapy transducer system 200 includes a transducer probe 202 connected to a control system 204, and display 206, in combination may provide therapy, imaging, and/or temperature or other tissue parameters monitoring to region of interest 210. Exemplary transducer system 200 is configured for first, imaging and display of region of interest 210 for localization of the treatment area and surrounding structures, second, delivery of focused, unfocused, or defocused ultrasound energy at a depth, distribution, timing, and energy level to achieve the desired therapeutic effect of thermal ablation to treat cellulite, and third to monitor the treatment area and surrounding structures before, during, and after therapy to plan and assess the results and/or provide feedback to control system 204 and/or an operator.

[0026] Exemplary transducer probe 202 can be configured to be suitably controlled and/or operated in various manners. For example, transducer probe 202 may be configured for use within an ultrasound treatment system, an ultrasound imaging system and/or an ultrasound imaging, therapy, and/or treatment monitoring system, including motion control subsystems.

[0027] Control system 204 can be configured with one or more subsystems, processors, input devices, displays and/or the like. Display 206 may be configured to image and/or monitor ROI 210 and/or any particular sub-region within ROI 210. Display 206 can be configured for two-dimensional, three-dimensional, real-time, analog, digital and/or any other type of imaging. Exemplary embodiments of both control system 204 and display 206 are described in greater detail herein.

[0028] Region of interest 210, can be comprised of superficial layer (epidermis/dermis) subcutaneous fat, lobuli, and muscle. Exemplary transducer system 200, is configured to provide cross-sectional two-dimensional imaging of the region 207, displayed as an image 205, with a controlled thermal lesion 209, confined approximately to proximal portion of fat lobuli and lower portion of dermis.

[0029] Transducer system 200 can be configured with the ability to controllably produce conformal treatment areas in superficial human tissue within region of interest 210 through precise spatial and temporal control of acoustic energy deposition. In accordance with an exemplary embodiment, control system 204 and transducer probe 202 can be suitably configured for spatial control of the acoustic energy by controlling the manner of distribution of the acoustical energy. For example, spatial control may be realized through selection of the type of one or more transducer configurations insonifying region of interest 210, selection of the placement and location of transducer probe

202 for delivery of acoustical energy relative to region-of-interest **210**, e.g., transducer probe **202** configured for scanning over part or whole of region-of-interest **210** to deliver conformal ultrasound therapeutic energy to create a thermal injury and to coagulate the proximal protrusions of fat lobuli, thereby eliminating the fat protrusions into the dermis. Transducer probe **202** may also be configured for control of other environment parameters, e.g., the temperature at the acoustic coupling interface can be controlled. In addition to the spatial control, control system **204** and/or transducer probe **202** can also be configured for temporal control, such as through adjustment and optimization of drive amplitude levels, frequency/waveform selections, and timing sequences and other energy drive characteristics to control the treatment of tissue. The spatial and/or temporal control can also be facilitated through open-loop and closed-loop feedback arrangements, such as through the monitoring of various positional and temporal characteristics. For example, through such spatial and/or temporal control, an exemplary treatment system **200** can enable the regions of thermal injury to possess arbitrary shape and size and allow the tissue to be treated in a controlled manner.

[0030] Transducer system **200** may be used to provide a mechanical action of ultrasound to physically break fat cell clusters and stretch the fibrous bonds. This mechanical action will also enhance lymphatic drainage, stimulating the evacuation of fat decay products. That is, the ultrasound may facilitate movement of the muscles and soft tissues within ROI **210**, thereby facilitating the loosening of fat deposits and/or the break up of fibrous tissue surrounding fat deposits.

[0031] In addition, transducer system **200** can be configured to deliver various therapeutic levels of ultrasound to increase the speed at which fat metabolizes, according to the Arrhenius Law: $Y = Ae^{-B/T}$, where Y is the yield of metabolic reaction, A and B are constants, and T is the temperature in degrees Kelvin. In one exemplary embodiment, transducer system **200** is configured to provide various therapeutic levels of ultrasound to increase the speed at which fat metabolizes. That is, according to Arrhenius Law, the yield, Y of a metabolic reaction is a function of temperature, T: $Y = Ae^{-B/T}$, where A and B are constants, and T is the temperature in degrees Kelvin. Thus, ultrasound treatment from transducer system **200**, ranging from approximately 750 kHz to 20 MHz, can increase the temperature in a treatment area, thereby increasing the metabolic reaction yield for that treatment area.

[0032] As previously described, control systems **104** and **204** may be configured in various manners with various subsystems and subcomponents. With reference to FIGS. 3A and 3B, in accordance with exemplary embodiments, an exemplary control system **300** can be configured for coordination and control of the entire therapeutic treatment process in accordance with the adjustable settings made by a therapeutic treatment system user. For example, control system **300** can suitably comprise power source components **302**, sensing and monitoring components **304**, cooling and coupling controls **306**, and/or processing and control logic components **308**. Control system **300** can be configured and optimized in a variety of ways with more or less subsystems and components to implement the therapeutic system for cellulite treatment, and the embodiment in FIGS. 3A and 3B are merely for illustration purposes.

[0033] For example, for power sourcing components **302**, control system **300** can comprise one or more direct current (DC) power supplies **303** configured to provide electrical energy for entire control system **300**, including power required by a transducer electronic amplifier/driver **312**. A DC current sense device **305** can also be provided to confirm the level of power going into amplifiers/drivers **312** for safety and monitoring purposes.

[0034] Amplifiers/drivers **312** can comprise multi-channel or single channel power amplifiers and/or drivers. In accordance with an exemplary embodiment for transducer array configurations, amplifiers/drivers **312** can also be configured with a beamformer to facilitate array focusing. An exemplary beamformer can be electrically excited by an oscillator/digitally controlled waveform synthesizer **310** with related switching logic.

[0035] The power sourcing components can also include various filtering configurations **314**. For example, switchable harmonic filters and/or matching may be used at the output of amplifier/driver **312** to increase the drive efficiency and effectiveness. Power detection components **316** may also be included to confirm appropriate operation and calibration. For example, electric power and other energy detection components **316** may be used to monitor the amount of power going to an exemplary probe system.

[0036] Various sensing and monitoring components **304** may also be suitably implemented within control system **300**. For example, in accordance with an exemplary embodiment, monitoring, sensing and interface control components **324** may be configured to operate with various motion detection systems **322** implemented within transducer probe **104** to receive and process information such as acoustic or other spatial and temporal information from a region of interest. Sensing and monitoring components can also include various controls, interfacing and switches **309** and/or power detectors **316**. Such sensing and monitoring components **304** can facilitate open-loop and/or closed-loop feedback systems within treatment system **100**.

[0037] For example, In such an open-loop system, a system user can suitably monitor the imaging and/or other spatial or temporal parameters and then adjust or modify same to accomplish a particular treatment objective. Instead of, or in combination with open-loop feedback configurations, an exemplary treatment system can comprise a closed-loop feedback system, wherein images and/or spatial/temporal parameters can be suitably monitored within monitoring component to generate signals.

[0038] During operation of exemplary treatment system **100**, a lesion configuration of a selected size, shape, orientation is determined. Based on that lesion configuration, one or more spatial parameters are selected, along with suitable temporal parameters, the combination of which yields the desired conformal lesion. Operation of the transducer can then be initiated to provide the conformal lesion or lesions. Open and/or closed-loop feedback systems can also be implemented to monitor the spatial and/or temporal characteristics, and/or other tissue parameter monitoring, to further control the conformal lesions.

[0039] Cooling/coupling control systems **306** may be provided to remove waste heat from exemplary probe **104**, provide a controlled temperature at the superficial tissue interface and deeper into tissue, and/or provide acoustic coupling from transducer probe **104** to region-of-interest **106**. Such cooling/coupling control systems **306** can also be

configured to operate in both open-loop and/or closed-loop feedback arrangements with various coupling and feedback components.

[0040] Processing and control logic components 308 can comprise various system processors and digital control logic 307, such as one or more of microcontrollers, microprocessors, field-programmable gate arrays (FPGAs), computer boards, and associated components, including firmware and control software 326, which interfaces to user controls and interfacing circuits as well as input/output circuits and systems for communications, displays, interfacing, storage, documentation, and other useful functions. System software and firmware 326 controls all initialization, timing, level setting, monitoring, safety monitoring, and all other system functions required to accomplish user-defined treatment objectives. Further, various control switches 308 can also be suitably configured to control operation.

[0041] An exemplary transducer probe 104 can also be configured in various manners and comprise a number of reusable and/or disposable components and parts in various embodiments to facilitate its operation. For example, transducer probe 104 can be configured within any type of transducer probe housing or arrangement for facilitating the coupling of transducer to a tissue interface, with such housing comprising various shapes, contours and configurations depending on the particular treatment application. For example, in accordance with an exemplary embodiment, transducer probe 104 can be depressed against a tissue interface whereby blood perfusion is partially or wholly cut-off, and tissue flattened in superficial treatment region-of-interest 106. Transducer probe 104 can comprise any type of matching, such as for example, electric matching, which may be electrically switchable; multiplexer circuits and/or aperture/element selection circuits; and/or probe identification devices, to certify probe handle, electric matching, transducer usage history and calibration, such as one or more serial EEPROM (memories). Transducer probe 104 may also comprise cables and connectors; motion mechanisms; motion sensors and encoders; thermal monitoring sensors; and/or user control and status related switches, and indicators such as LEDs. For example, a motion mechanism in probe 104 may be used to controllably create multiple lesions, or sensing of probe motion itself may be used to controllably create multiple lesions and/or stop creation of lesions, e.g. for safety reasons if probe 104 is suddenly jerked or is dropped. In addition, an external motion encoder arm may be used to hold the probe during use, whereby the spatial position and attitude of probe 104 is sent to the control system to help controllably create lesions. Furthermore, other sensing functionality such as profilometers or other imaging modalities may be integrated into the probe in accordance with various exemplary embodiments.

[0042] With reference to FIGS. 4A and 4B, in accordance with an exemplary embodiment, a transducer probe 400 can comprise a control interface 402, a transducer 404, coupling components 406, and monitoring/sensing components 408, and/or motion mechanism 410. However, transducer probe 400 can be configured and optimized in a variety of ways with more or less parts and components to provide ultrasound energy for cellulite treatment, and the embodiment in FIGS. 4A and 4B are merely for illustration purposes.

[0043] In accordance with an exemplary embodiment of the present invention, transducer probe 400 is configured to deliver energy over varying temporal and/or spatial distri-

butions in order to provide energy effects and initiate responses in a region of interest. These effects can include, for example, thermal, cavitation, hydrodynamic, and resonance induced tissue effects. For example, exemplary transducer probe 400 can be operated under one or more frequency ranges to provide two or more energy effects and initiate one or more responses in the region of interest. In addition, transducer probe 400 can also be configured to deliver planar, defocused and/or focused energy to a region of interest to provide two or more energy effects and to initiate one or more reactions. These responses can include, for example, diathermy, hemostasis, revascularization, angiogenesis, growth of interconnective tissue, tissue reformation, ablation of existing tissue, protein synthesis and/or enhanced cell permeability. These and various other exemplary embodiments for such combined ultrasound treatment, effects and responses are more fully set forth in U.S. patent application Ser. No. 10/950,112, entitled "METHOD AND SYSTEM FOR COMBINED ULTRASOUND TREATMENT," Filed Sep. 24, 2004 and incorporated herein by reference.

[0044] Control interface 402 is configured for interfacing 428 with control system 300 to facilitate control of transducer probe 400. Control interface components 402 can comprise multiplexer/aperture select 424, switchable electric matching networks 426, serial EEPROMs and/or other processing components and matching and probe usage information 430 and interface connectors 432.

[0045] Coupling components 406 can comprise various devices to facilitate coupling of transducer probe 400 to a region of interest. For example, coupling components 406 can comprise cooling and acoustic coupling system 420 configured for acoustic coupling of ultrasound energy and signals. Acoustic cooling/coupling system 420 with possible connections such as manifolds may be utilized to couple sound into the region-of-interest, control temperature at the interface and deeper into tissue, provide liquid-filled lens focusing, and/or to remove transducer waste heat. Coupling system 420 may facilitate such coupling through use of various coupling mediums, including air and other gases, water and other fluids, gels, solids, and/or any combination thereof, or any other medium that allows for signals to be transmitted between transducer active elements 412 and a region of interest. In addition to providing a coupling function, in accordance with an exemplary embodiment, coupling system 420 can also be configured for providing temperature control during the treatment application. For example, coupling system 420 can be configured for controlled cooling of an interface surface or region between transducer probe 400 and a region of interest and beyond and beyond by suitably controlling the temperature of the coupling medium. The suitable temperature for such coupling medium can be achieved in various manners, and utilize various feedback systems, such as thermocouples, thermistors or any other device or system configured for temperature measurement of a coupling medium. Such controlled cooling can be configured to further facilitate spatial and/or thermal energy control of transducer probe 400.

[0046] In accordance with an exemplary embodiment, with additional reference to FIG. 11, acoustic coupling and cooling 1140 can be provided to acoustically couple energy and imaging signals from transducer 1104 to and from the region of interest 1102, to provide thermal control at the probe 1100 to region-of-interest interface 1110, and to

remove potential waste heat from the transducer probe at region 1144. Temperature monitoring can be provided at the coupling interface via a thermal sensor 1146 to provide a mechanism of temperature measurement 1148 and control via control system 1106 and a thermal control system 1142. Thermal control may consist of passive cooling such as via heat sinks or natural conduction and convection or via active cooling such as with peltier thermoelectric coolers, refrigerants, or fluid-based systems comprised of pump, fluid reservoir, bubble detection, flow sensor, flow channels/tubing 1144 and thermal control 1142.

[0047] Monitoring and sensing components 408 can comprise various motion and/or position sensors 416, temperature monitoring sensors 418, user control and feedback switches 414 and other like components for facilitating control by control system 300, e.g., to facilitate spatial and/or temporal control through open-loop and closed-loop feedback arrangements that monitor various spatial and temporal characteristics.

[0048] Motion mechanism 410 can comprise manual operation, mechanical arrangements, or some combination thereof. For example, a motion mechanism 422 can be suitably controlled by control system 300, such as through the use of accelerometers, encoders or other position/orientation devices 416 to determine and enable movement and positions of transducer probe 400. Linear, rotational or variable movement can be facilitated, e.g., those depending on the treatment application and tissue contour surface.

[0049] Transducer 404 can comprise one or more transducers configured for producing conformal lesions of thermal injury in superficial human tissue within a region of interest through precise spatial and temporal control of acoustic energy deposition. Transducer 404 can also comprise one or more transduction elements and/or lenses 412. The transduction elements can comprise a piezoelectrically active material, such as lead zirconate titanate (PZT), or any other piezoelectrically active material, such as a piezoelectric ceramic, crystal, plastic, and/or composite materials, as well as lithium niobate, lead titanate, barium titanate, and/or lead metaniobate. In addition to, or instead of, a piezoelectrically active material, transducer 404 can comprise any other materials configured for generating radiation and/or acoustical energy. Transducer 404 can also comprise one or more matching layers configured along with the transduction element such as coupled to the piezoelectrically active material. Acoustic matching layers and/or damping may be employed as necessary to achieve the desired electroacoustic response.

[0050] In accordance with an exemplary embodiment, the thickness of the transduction element of transducer 404 can be configured to be uniform. That is, a transduction element 412 can be configured to have a thickness that is substantially the same throughout. In accordance with another exemplary embodiment, the thickness of a transduction element 412 can also be configured to be variable. For example, transduction element(s) 412 of transducer 404 can be configured to have a first thickness selected to provide a center operating frequency of a lower range, for example from approximately 750 kHz to 5 MHz. Transduction element 404 can also be configured with a second thickness selected to provide a center operating frequency of a higher range, for example from approximately 5 MHz to 20 MHz or more. Transducer 404 can be configured as a single broadband transducer excited with at least two or more

frequencies to provide an adequate output for generating a desired response. Transducer 404 can also be configured as two or more individual transducers, wherein each transducer comprises one or more transduction element. The thickness of the transduction elements can be configured to provide center-operating frequencies in a desired treatment range. For example, transducer 404 can comprise a first transducer configured with a first transduction element having a thickness corresponding to a center frequency range of approximately 750 kHz to 5 MHz, and a second transducer configured with a second transduction element having a thickness corresponding to a center frequency of approximately 5 MHz to 20 MHz or more.

[0051] Transducer 404 may be composed of one or more individual transducers in any combination of focused, planar, or unfocused single-element, multi-element, or array transducers, including 1-D, 2-D, and annular arrays; linear, curvilinear, sector, or spherical arrays; spherically, cylindrically, and/or electronically focused, defocused, and/or lensed sources. For example, with reference to an exemplary embodiment depicted in FIG. 5, transducer 500 can be configured as an acoustic array to facilitate phase focusing. That is, transducer 500 can be configured as an array of electronic apertures that may be operated by a variety of phases via variable electronic time delays. By the term “operated,” the electronic apertures of transducer 500 may be manipulated, driven, used, and/or configured to produce and/or deliver an energy beam corresponding to the phase variation caused by the electronic time delay. For example, these phase variations can be used to deliver defocused beams 508, planar beams 504, and/or focused beams 506, each of which may be used in combination to achieve different physiological effects in a region of interest 510. Transducer 500 may additionally comprise any software and/or other hardware for generating, producing and/or driving a phased aperture array with one or more electronic time delays.

[0052] Transducer 500 can also be configured to provide focused treatment to one or more regions of interest using various frequencies. In order to provide focused treatment, transducer 500 can be configured with one or more variable depth devices to facilitate treatment. For example, transducer 500 may be configured with variable depth devices disclosed in U.S. patent application Ser. No. 10/944,500, entitled “System and Method for Variable Depth Ultrasound”, filed on Sep. 16, 2004, having at least one common inventor and a common Assignee as the present application, and incorporated herein by reference. In addition, transducer 500 can also be configured to treat one or more additional ROI 510 through the enabling of sub-harmonics or pulse-echo imaging, as disclosed in U.S. patent application Ser. No. 10/944,499, entitled “Method and System for Ultrasound Treatment with a Multi-directional Transducer”, filed on Sep. 16, 2004, having at least one common inventor and a common Assignee as the present application, and also incorporated herein by reference.

[0053] Moreover, any variety of mechanical lenses or variable focus lenses, e.g. liquid-filled lenses, may also be used to focus and or defocus the sound field. For example, with reference to exemplary embodiments depicted in FIGS. 6A and 6B, transducer 600 may also be configured with an electronic focusing array 604 in combination with one or more transduction elements 606 to facilitate increased flexibility in treating ROI 610. Array 602 may be configured in

a manner similar to transducer 502. That is, array 602 can be configured as an array 604 of electronic apertures that may be operated by a variety of phases via variable electronic time delays, for example, $T_1, T_2 \dots T_j$. By the term “operated,” the electronic apertures of array 604 may be manipulated, driven, used, and/or configured to produce and/or deliver energy in a manner corresponding to the phase variation caused by the electronic time delay. For example, these phase variations can be used to deliver defocused beams, planar beams, and/or focused beams, each of which may be used in combination to achieve different physiological effects in ROI 610.

[0054] Transduction elements 606 may be configured to be concave, convex, and/or planar. For example, in an exemplary embodiment depicted in FIG. 6A, transduction elements 606 are configured to be concave in order to provide focused energy for treatment of ROI 610. Additional embodiments are disclosed in U.S. patent application Ser. No. 10/944,500, entitled “Variable Depth Transducer System and Method”, and again incorporated herein by reference.

[0055] In another exemplary embodiment, depicted in FIG. 6B, transduction elements 606 can be configured to be substantially flat in order to provide substantially uniform energy to ROI 610. While FIGS. 6A and 6B depict exemplary embodiments with transduction elements 604 configured as concave and substantially flat, respectively, transduction elements 604 can be configured to be concave, convex, and/or substantially flat. In addition, transduction elements 604 can be configured to be any combination of concave, convex, and/or substantially flat structures. For example, a first transduction element can be configured to be concave, while a second transduction element can be configured to be substantially flat.

[0056] With reference to FIGS. 8A and 8B, transducer 800 can be configured as single-element arrays, wherein a single-element 802, e.g., a transduction element of various structures and materials, can be configured with a plurality of masks 804, such masks comprising ceramic, metal or any other material or structure for masking or altering energy distribution from element 802, creating an array of energy distributions 808. Masks 804 can be coupled directly to element 802 or separated by a standoff 806, such as any suitably solid or liquid material.

[0057] An exemplary transducer 404 can also be configured as an annular array to provide planar, focused and/or defocused acoustical energy. For example, with reference to FIGS. 10A and 10B, in accordance with an exemplary embodiment, an annular array 1000 can comprise a plurality of rings 1012, 1014, 1016 to N. Rings 1012, 1014, 1016 to N can be mechanically and electrically isolated into a set of individual elements, and can create planar, focused, or defocused waves. For example, such waves can be centered on-axis, such as by methods of adjusting corresponding transmit and/or receive delays, $\tau_1, \tau_2, \tau_3 \dots \tau_N$. An electronic focus can be suitably moved along various depth positions, and can enable variable strength or beam tightness, while an electronic defocus can have varying amounts of defocusing. In accordance with an exemplary embodiment, a lens and/or convex or concave shaped annular array 1000 can also be provided to aid focusing or defocusing such that any time differential delays can be reduced. Movement of annular array 1000 in one, two or three-dimensions, or along any path, such as through use of probes and/or any conventional

robotic arm mechanisms, may be implemented to scan and/or treat a volume or any corresponding space within a region of interest.

[0058] Transducer 404 can also be configured in other annular or non-array configurations for imaging/therapy functions. For example, with reference to FIGS. 10C-10F, a transducer can comprise an imaging element 1012 configured with therapy element(s) 1014. Elements 1012 and 1014 can comprise a single-transduction element, e.g., a combined imaging/transducer element, or separate elements, can be electrically isolated 1022 within the same transduction element or between separate imaging and therapy elements, and/or can comprise standoff 1024 or other matching layers, or any combination thereof. For example, with particular reference to FIG. 10F, a transducer can comprise an imaging element 1012 having a surface 1028 configured for focusing, defocusing or planar energy distribution, with therapy elements 1014 including a stepped-configuration lens configured for focusing, defocusing, or planar energy distribution.

[0059] In accordance with another aspect of the invention, transducer probe 400 may be configured to provide one, two or three-dimensional treatment applications for focusing acoustic energy to one or more regions of interest. For example, as discussed above, transducer probe 400 can be suitably diced to form a one-dimensional array, e.g., a transducer comprising a single array of sub-transduction elements.

[0060] In accordance with another exemplary embodiment, transducer probe 400 may be suitably diced in two-dimensions to form a two-dimensional array. For example, with reference to FIG. 9, an exemplary two-dimensional array 900 can be suitably diced into a plurality of two-dimensional portions 902. Two-dimensional portions 902 can be suitably configured to focus on the treatment region at a certain depth, and thus provide respective slices 904 of the treatment region. As a result, the two-dimensional array 900 can provide a two-dimensional slicing of the image plane of a treatment region, thus providing two-dimensional treatment.

[0061] In accordance with another exemplary embodiment, transducer probe 400 may be suitably configured to provide three-dimensional treatment. For example, to provide three dimensional treatment of a region of interest, with reference again to FIG. 3, a three-dimensional system can comprise transducer probe 400 configured with an adaptive algorithm, such as, for example, one utilizing three-dimensional graphic software, contained in a control system, such as control system 300. The adaptive algorithm is suitably configured to receive two-dimensional imaging, temperature and/or treatment information relating to the region of interest, process the received information, and then provide corresponding three-dimensional imaging, temperature and/or treatment information.

[0062] In accordance with an exemplary embodiment, with reference again to FIG. 9, an exemplary three-dimensional system can comprise a two-dimensional array 900 configured with an adaptive algorithm to suitably receive slices 904, 907 from different image planes of the treatment region, process the received information, and then provide volumetric information 906, e.g., three-dimensional imaging, temperature and/or treatment information. Moreover, after processing the received information with the adaptive

algorithm, the two-dimensional array **900** may suitably provide therapeutic heating to the volumetric region **906** as desired.

[0063] Alternatively, rather than utilizing an adaptive algorithm, such as three-dimensional software, to provide three-dimensional imaging and/or temperature information, an exemplary three-dimensional system can comprise a single transducer **404** configured within a probe arrangement to operate from various rotational and/or translational positions relative to a target region.

[0064] To further illustrate the various structures for transducer **404**, with reference to FIG. 7, ultrasound therapy transducer **700** can be configured for a single focus, an array of foci, a locus of foci, a line focus, and/or diffraction patterns. Transducer **700** can also comprise single elements, multiple elements, annular arrays, one-, two-, or three-dimensional arrays, broadband transducers, and/or combinations thereof, with or without lenses, acoustic components, and mechanical and/or electronic focusing. Transducers configured as spherically focused single elements **702**, annular arrays **704**, annular arrays with damped regions **706**, line focused single elements **708**, 1-D linear arrays **710**, 1-D curvilinear arrays **712** in concave or convex form, with or without elevation focusing, 2-D arrays **714**, and 3-D spatial arrangements of transducers may be used to perform therapy and/or imaging and acoustic monitoring functions. For any transducer configuration, focusing and/or defocusing may be in one plane or two planes via mechanical focus **720**, convex lens **722**, concave lens **724**, compound or multiple lenses **726**, planar form **728**, or stepped form, such as illustrated in FIG. 10F. Any transducer or combination of transducers may be utilized for treatment. For example, an annular transducer may be used with an outer portion dedicated to therapy and the inner disk dedicated to broadband imaging wherein such imaging transducer and therapy transducer have different acoustic lenses and design, such as illustrated in FIG. 10C-10F.

[0065] Various shaped treatment lesions can be produced using the various acoustic lenses and designs in FIGS. 10A-10F. For example, mushroom shaped lesions may be produced from a spherically focused source, and/or planar lesions from a flat source. That is, as the application of ablative ultrasound energy continues, this causes thermal expansion to generate a growing lesion. Concave planar sources and arrays can produce a "V-shaped" or ellipsoidal lesion. Electronic arrays, such as a linear array, can produce defocused, planar, or focused acoustic beams that may be employed to form a wide variety of additional lesion shapes at various depths. An array may be employed alone or in conjunction with one or more planar or focused transducers. Such transducers and arrays in combination produce a very wide range of acoustic fields and their associated benefits. A fixed focus and/or variable focus lens or lenses may be used to further increase treatment flexibility. A convex-shaped lens, with acoustic velocity less than that of superficial tissue, may be utilized, such as a liquid-filled lens, gel-filled or solid gel lens, rubber or composite lens, with adequate power handling capacity; or a concave-shaped, low profile, lens may be utilized and composed of any material or composite with velocity greater than that of tissue. While the structure of transducer source and configuration can facilitate a particular shaped lesion as suggested above, such structures are not limited to those particular shapes as the

other spatial parameters, as well as the temporal parameters, can facilitate additional shapes within any transducer structure and source.

[0066] Through operation of ultrasound system **100**, a method for treatment of cellulite can be realized that can facilitate effective and efficient therapy without creating chronic injury to human tissue. For example, a user may first select one or more transducer probe configurations for treating a region of interest. The user may select any probe configuration described herein. Because the treatment region ranges from approximately 0 mm to 3.5 cm, exemplary transducer probes may include, for example, an annular array, a variable depth transducer, a mechanically moveable transducer, a cylindrical-shaped transducer, a linear or flat transducer and the like. As used herein, the term user may include a person, employee, doctor, nurse, and/or technician, utilizing any hardware and/or software of other control systems.

[0067] Once one or more transducers are selected, the user may then image a region of interest in order to plan a treatment protocol. By imaging a region of interest, the user may use the same treatment transducer probe and/or one or more additional transducers to image the region of interest at a high resolution. In one embodiment, the transducer may be configured to facilitate high speed imaging over a large region of interest to enable accurate imaging over a large region of interest. In another embodiment, ultrasound imaging may include the use of Doppler flow monitoring and/or color flow monitoring. In addition other means of imaging such as photography and other visual optical methods, MRI, X-Ray, PET, infrared or others can be utilized separately or in combination for imaging and feedback of the superficial tissue and the vascular tissue in the region of interest.

[0068] In accordance with another exemplary embodiment, with reference to FIG. 12, an exemplary treatment system **200** can be configured with and/or combined with various auxiliary systems to provide additional functions. For example, an exemplary treatment system **1200** for treating a region of interest **1206** can comprise a control system **1202**, a probe **1204**, and a display **1208**. Treatment system **1200** further comprises an auxiliary imaging modality **1274** and/or auxiliary monitoring modality **1272** may be based upon at least one of photography and other visual optical methods, magnetic resonance imaging (MRI), computed tomography (CT), optical coherence tomography (OCT), electromagnetic, microwave, or radio frequency (RF) methods, positron emission tomography (PET), infrared, ultrasound, acoustic, or any other suitable method of visualization, localization, or monitoring of cellulite within region-of-interest **1206**, including imaging/monitoring enhancements. Such imaging/monitoring enhancement for ultrasound imaging via probe **1204** and control system **1202** could comprise M-mode, persistence, filtering, color, Doppler, and harmonic imaging among others; furthermore an ultrasound treatment system **1270**, as a primary source of treatment, may be combined with a secondary source of treatment **1276**, including radio frequency (RF), intense pulsed light (IPL), laser, infrared laser, microwave, or any other suitable energy source.

[0069] Because the location and thickness of the fat lobuli varies from one patient to another (due to genetics, weight, age, etc.), imaging using a transducer can facilitate treatment within a patient, however imaging is not required to treat cellulite.

[0070] By planning a treatment protocol, the user may choose one or more spatial and/or temporal characteristics to provide conformal ultrasound energy to a region of interest. For example, the user may select one or more spatial characteristics to control, including, for example, the use one or more transducers, one or more mechanical and/or electronic focusing mechanisms, one or more transduction elements, one or more placement locations of the transducer relative to the region of interest, one or more feedback systems, one or more mechanical arms, one or more orientations of the transducer, one or more temperatures of treatment, one or more coupling mechanisms and/or the like.

[0071] In addition, the user may choose one or more temporal characteristics to control in order to facilitate treatment of the region of interest. For example, the user may select and/or vary the treatment time, frequency, power, energy, amplitude and/or the like in order to facilitate temporal control. For more information on selecting and controlling ultrasound spatial and temporal characteristics, see U.S. application Ser. No. 11/163,148, entitled "Method and System for Controlled Thermal Injury," filed Oct. 6, 2005 and previously incorporated herein by reference.

[0072] After planning of a treatment protocol is complete, the treatment protocol can be implemented. That is, a transducer system can be used to deliver ultrasound energy to a treatment region to ablate select tissue in order to facilitate cellulite treatment. By delivering energy, the transducer may be driven at a select frequency, a phased array may be driven with certain temporal and/or spatial distributions, a transducer may be configured with one or more transduction elements to provide focused, defocused and/or planar energy, and/or the transducer may be configured and/or driven in any other ways hereinafter devised.

[0073] In one exemplary embodiment, energy is delivered in relatively small ablative areas in order to minimize and/or prevent scar tissue from forming. That is, each ablative area of treatment can range from approximately 100 microns to 55 mm in diameter. In another exemplary embodiment, ultrasound energy is used in a "lawnmower" type fashion to evenly ablate a treatment region to provide a substantially planar surface of lobuli. This "lawnmower"-type ablation in turn, helps to achieve a substantially smooth surface of the epidermis.

[0074] In one exemplary embodiment, energy is delivered at a treatment depth of approximately 0 mm to 3.5 cm. The energy may range from 750 kHz to about 10 MHz, with typical applications ranging from 2 MHz to 10 MHz. In order to deliver energy in this treatment range, the transducer can be driven at power levels ranging from 20 W to 200 W. Because treatment time and treatment power are interrelated, these variables may differ from one patient to another and/or from one region of interest to another.

[0075] Once the treatment protocol has been implemented, the region of tissue may have one or more reactions to the treatment. For example, in one embodiment, the tissue responds by enhancement of lymphatic drainage, evacuation of fat decay products, creation of a thermal injury and/or coagulation of proximal protrusions of fat lobuli.

[0076] Upon treatment, the steps outlined above can be repeated one or more additional times to provide for optimal treatment results. Different ablation sizes and shapes may affect the recovery time and time between treatments. For example, in general, the larger the surface area of the treatment lesion, the faster the recovery. The series of

treatments can also enable the user to tailor additional treatments in response to a patient's responses to the ultrasound treatment.

[0077] The present invention has been described above with reference to various exemplary embodiments. However, those skilled in the art will recognize that changes and modifications may be made to the exemplary embodiments without departing from the scope of the present invention. For example, the various operational steps, as well as the components for carrying out the operational steps, may be implemented in alternate ways depending upon the particular application or in consideration of any number of cost functions associated with the operation of the system, e.g., various steps may be deleted, modified, or combined with other steps. These and other changes or modifications are intended to be included within the scope of the present invention, as set forth in the following claims.

1. (canceled)
2. An ultrasound treatment probe for treatment of cellulite, the probe comprising:
 - a piezoelectric ultrasound therapy element connected to a motion mechanism,
 - wherein the piezoelectric ultrasound therapy element is configured for acoustic coupling to a skin surface,
 - wherein the piezoelectric ultrasound therapy element is configured for delivery of ultrasound energy at a temperature sufficient to coagulate fat cells in fat lobuli that protrude into a dermis layer to create an appearance of cellulite at a depth under the skin surface,
 - wherein the motion mechanism is configured to operate with an encoder configured to determine movement of the piezoelectric ultrasound therapy element within the probe,
 - wherein the motion mechanism moves the piezoelectric ultrasound therapy element to form one or more thermal foci at the depth for coagulating fat thereby reducing an appearance of cellulite.
3. The probe of claim 2,
 - wherein the encoder is configured for monitoring a position of the piezoelectric ultrasound therapy element on the motion mechanism in a housing of the ultrasound probe,
 - wherein the piezoelectric ultrasound therapy element is a single element that delivers the ultrasound energy at a frequency of between 2 MHz to 10 MHz,
 - wherein the ultrasound energy is delivered with a treatment power of between 20 W and 200 W,
 - wherein the piezoelectric ultrasound therapy element is configured to deliver the ultrasound energy at the depth below the skin surface,
 - wherein the ultrasound energy generates a thermal lesion with a dimension of between 100 microns to 55 mm in the region of interest.
4. The probe of claim 2, wherein the piezoelectric ultrasound therapy element is one of the group consisting of spherically focused and cylindrically focused.
5. The probe of claim 2, wherein the ultrasound energy increases a speed at which fat metabolizes according to Arrhenius Law: $Y = A \cdot e^{-B/T}$, where Y is a yield of metabolic reaction, A and B are constants, and T is a temperature in degrees Kelvin.
6. The probe of claim 2, wherein the piezoelectric ultrasound therapy element is configured to operate with a control system comprising a processor, wherein the piezo-

electric ultrasound therapy element is configured for communication with the control system, wherein the probe is disposable.

7. The probe of claim 2, wherein the motion mechanism is a linear motion mechanism for linear movement of the piezoelectric ultrasound therapy element to form a plurality of thermal lesions along a line at the depth in the region of interest.

8. The probe of claim 2, further comprising a piezoelectric ultrasound imaging element and an information storage EEPROM, wherein the probe is reusable.

9. The probe of claim 2, further comprising a piezoelectric ultrasound imaging element co-housed with the piezoelectric ultrasound therapy element.

10. The probe of claim 2, wherein the motion mechanism is configured for any one of the group consisting of linear, rotational, and variable movement of the piezoelectric ultrasound therapy element.

11. An ultrasound probe for treatment of cellulite, the probe comprising:

a piezoelectric ultrasound therapy element configured for acoustic coupling through the ultrasound probe to a skin surface,

wherein a plurality of fat lobuli containing fat cells protrude into a dermis layer under the skin surface, wherein the piezoelectric ultrasound therapy element is configured for delivery of energy at a temperature sufficient to coagulate at least a portion of the fat cells in the plurality of fat lobuli at a depth under the skin surface, thereby reducing an appearance of cellulite.

12. The probe of claim 11,

wherein the piezoelectric ultrasound therapy element is a single element that delivers ultrasound energy at a frequency of between 2 MHz to 10 MHz,

wherein the ultrasound energy is delivered with a treatment power of between 20 W and 200 W,

wherein the piezoelectric ultrasound therapy element is configured to deliver the ultrasound energy up to 3.5 cm below the skin surface,

wherein the ultrasound energy generates a thermal lesion with a dimension of between 100 microns to 55 mm in the region of interest.

13. The probe of claim 11,

further comprising a housing, the housing containing a piezoelectric ultrasound imaging element,

wherein the piezoelectric ultrasound imaging element is configured for imaging a region of interest under the skin surface, wherein the region of interest comprises a tissue, wherein the tissue comprises the plurality of fat lobuli,

wherein the probe is disposable,.

14. The probe of claim 11,

wherein the piezoelectric ultrasound therapy element is a single element that delivers ultrasound energy at a frequency of between 750 kHz to 10 MHz, and

wherein the ultrasound energy increases a speed at which fat metabolizes according to Arrhenius Law: $Y = A \cdot e^{-B/T}$, where Y is a yield of metabolic reaction, A and B are constants, and T is a temperature in degrees Kelvin.

15. The probe of claim 11, further comprising a storage system comprising probe identification and probe usage history,

wherein the piezoelectric ultrasound therapy element is configured for connection to a control system,

wherein the control system comprises: a processor, software, a power supply, and a communication device.

16. An ultrasound probe for treatment of cellulite, the probe comprising:

a housing, a piezoelectric ultrasound therapy element, and a motion mechanism,

wherein the piezoelectric ultrasound therapy element delivers ultrasound energy to a tissue below a skin surface at a frequency of between 2 MHz to 10 MHz, wherein the tissue comprises a plurality of fat lobuli that protrude into a dermis layer to create an appearance of cellulite,

wherein the piezoelectric ultrasound therapy element is configured for delivery of the ultrasound energy at a temperature sufficient to coagulate at least a portion of a plurality of fat lobuli at a depth under the skin surface, wherein the piezoelectric ultrasound therapy element is connected to the motion mechanism inside the housing, wherein the motion mechanism is configured to operate with an encoder,

wherein the motion mechanism moves the piezoelectric ultrasound therapy element to form a plurality of thermal lesions at the depth for reducing an appearance of cellulite.

17. The probe of claim 16,

wherein the piezoelectric ultrasound therapy element is a single element,

wherein the piezoelectric ultrasound therapy element is configured to deliver the ultrasound energy at the depth below the skin surface, wherein the depth is a single, fixed depth,

wherein the ultrasound energy generates a thermal lesion with a dimension of between 100 microns to 55 mm in a region of interest.

18. The probe of claim 16, wherein the piezoelectric ultrasound therapy element is configured to operate with a control system that comprises a spatial control and a temporal control, the spatial control and the temporal control controlling the delivery of the ultrasound energy at a temperature sufficient to cause coagulation of at least the portion of the plurality of fat lobuli at the depth under the skin surface, wherein the ultrasound energy is delivered with a treatment power of between 20 W and 200 W.

19. The probe of claim 18, further comprising a storage system comprising probe identification and probe usage history, wherein the probe is disposable.

20. The probe of claim 16, wherein the ultrasound energy increases a speed at which fat metabolizes according to Arrhenius Law: $Y = A \cdot e^{-B/T}$, where Y is a yield of metabolic reaction, A and B are constants, and T is a temperature in degrees Kelvin.

21. The probe of claim 16, wherein the piezoelectric ultrasound therapy element is configured to deliver the ultrasound energy at an energy level for causing at least one of ablating tissue, stretching fibrous bonds, or stimulating evacuation of fat decay products in the region of interest.

* * * * *

专利名称(译)	用于减少脂肪和脂肪团的超声波探头		
公开(公告)号	US20180272159A1	公开(公告)日	2018-09-27
申请号	US15/996295	申请日	2018-06-01
申请(专利权)人(译)	引导治疗系统公司		
当前申请(专利权)人(译)	引导治疗系统公司		
[标]发明人	SLAYTON MICHAEL H BARTHE PETER G MAKIN INDER RAJ S		
发明人	SLAYTON, MICHAEL H. BARTHE, PETER G. MAKIN, INDER RAJ S.		
IPC分类号	A61N7/02 G01S15/89 A61B8/08 A61B8/14 A61B8/00 A61N7/00 A61B90/00		
CPC分类号	G01S15/8936 A61B8/461 H05K999/99 A61B2090/378 A61B8/429 A61N7/00 A61B8/14 A61N2007/0008 A61N7/02 A61B8/483 A61B8/4483 A61B8/4455 G01S15/8906		
优先权	60/616753 2004-10-06 US		
其他公开文献	US10245450		
外部链接	Espacenet USPTO		

摘要(译)

一种用于向组织提供超声治疗的方法和系统，所述组织包含真皮的下部和进入真皮的脂肪小叶的近端突起。一个实施例将超声能量传递到该区域，产生热损伤并凝结脂肪小叶的近端突起，从而消除进入真皮的脂肪突起。一个实施例还可以包括在治疗之前，之后或期间使用相同或单独的探针的超声成像配置。此外，可以使用各种治疗水平的超声来增加脂肪代谢的速度。另外，超声的机械作用物理地破坏脂肪细胞团并拉伸纤维状结合。机械作用还会增强淋巴引流，刺激脂肪腐烂产物的排出。

