



US009986977B2

(12) **United States Patent**
Kim et al.

(10) **Patent No.:** **US 9,986,977 B2**
(45) **Date of Patent:** **Jun. 5, 2018**

(54) **ULTRASONIC DIAGNOSTIC APPARATUS
AND METHOD OF OPERATING THE SAME**

(56) **References Cited**

U.S. PATENT DOCUMENTS

- (71) Applicant: **SAMSUNG MEDISON CO., LTD.**,
Gangwon-Do (KR)
- (72) Inventors: **Nam-Woong Kim**, Gangwon-do (KR);
Gil-Ju Jin, Gangwon-do (KR)
- (73) Assignee: **SAMSUNG MEDISON CO., LTD.**,
Gangwon-Do (KR)

5,505,203 A * 4/1996 Deitrich A61B 8/00
600/437

5,552,645 A * 9/1996 Weng A61B 5/0002
307/112

5,776,065 A * 7/1998 Mehmanpazir A61B 8/00
600/437

6,261,249 B1 7/2001 Talish et al.
6,409,665 B1 6/2002 Scott et al.
8,403,853 B2 3/2013 Nakamura

(Continued)

- (*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 695 days.

FOREIGN PATENT DOCUMENTS

JP 2011-067544 A 4/2011
KR 2006-0075733 A 7/2006

(Continued)

(21) Appl. No.: **14/493,112**

(22) Filed: **Sep. 22, 2014**

OTHER PUBLICATIONS

(65) **Prior Publication Data**
US 2015/0265253 A1 Sep. 24, 2015

International Search Report and Written Opinion issued in counter-
part International Patent Application dated Dec. 30, 2014; 12
pages in English language.

(30) **Foreign Application Priority Data**
Mar. 18, 2014 (KR) 10-2014-0031820

Primary Examiner — Long V Le

Assistant Examiner — Angela M Hoffa

(74) *Attorney, Agent, or Firm* — McDermott Will &
Emery LLP


- (51) **Int. Cl.**
A61B 8/00 (2006.01)
- (52) **U.S. Cl.**
CPC **A61B 8/54** (2013.01); **A61B 8/4281**
(2013.01); **A61B 8/4477** (2013.01); **A61B**
8/4405 (2013.01); **A61B 8/4444** (2013.01);
A61B 8/585 (2013.01)

(58) **Field of Classification Search**
CPC A61B 8/54; A61B 8/4477; A61B 8/4281;
A61B 8/585; A61B 8/4405; A61B 8/4444
See application file for complete search history.

(57) **ABSTRACT**

Provided are an ultrasonic diagnostic apparatus and a
method of operating the same. The ultrasonic diagnostic
apparatus includes: a first ultrasonic transceiver that trans-
mits an ultrasonic signal and receives a first echo signal that
is reflected, through a deactivated probe from among a
plurality of probes; a gel detector that determines whether
gel is applied on the deactivated probe based on the received
first echo signal; and a controller that activates the deacti-
vated probe when it is determined that the gel is applied on
the deactivated probe.

15 Claims, 7 Drawing Sheets

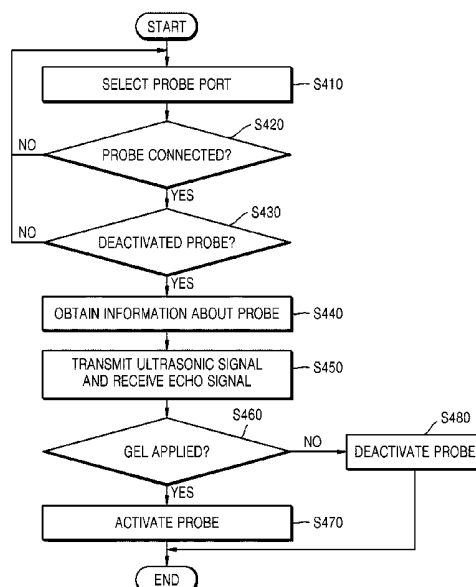

(56)

References Cited

U.S. PATENT DOCUMENTS

9,504,446	B2 *	11/2016	Jaeger	A61N 7/02
9,610,065	B2 *	4/2017	Kim	A61B 8/54
2005/0113699	A1	5/2005	Haugen et al.	
2006/0173346	A1	8/2006	Lee	
2006/0241464	A1	10/2006	Ohtake et al.	
2007/0232907	A1 *	10/2007	Pelissier	A61B 8/00
				600/437
2013/0072800	A1	3/2013	Lee	
2014/0107487	A1 *	4/2014	Kim	A61B 8/4263
				600/459
2015/0045673	A1 *	2/2015	Kim	A61B 8/4438
				600/459
2016/0106396	A1 *	4/2016	Jin	A61B 8/54
				600/437
2016/0183920	A1 *	6/2016	Woo	A61B 8/54
				600/440

FOREIGN PATENT DOCUMENTS

KR	2007-0022291	A	2/2007
KR	10-2011-0083781	A	7/2011
KR	10-2013-0030664	A	3/2013
KR	10-1263831		5/2013

* cited by examiner

FIG. 1

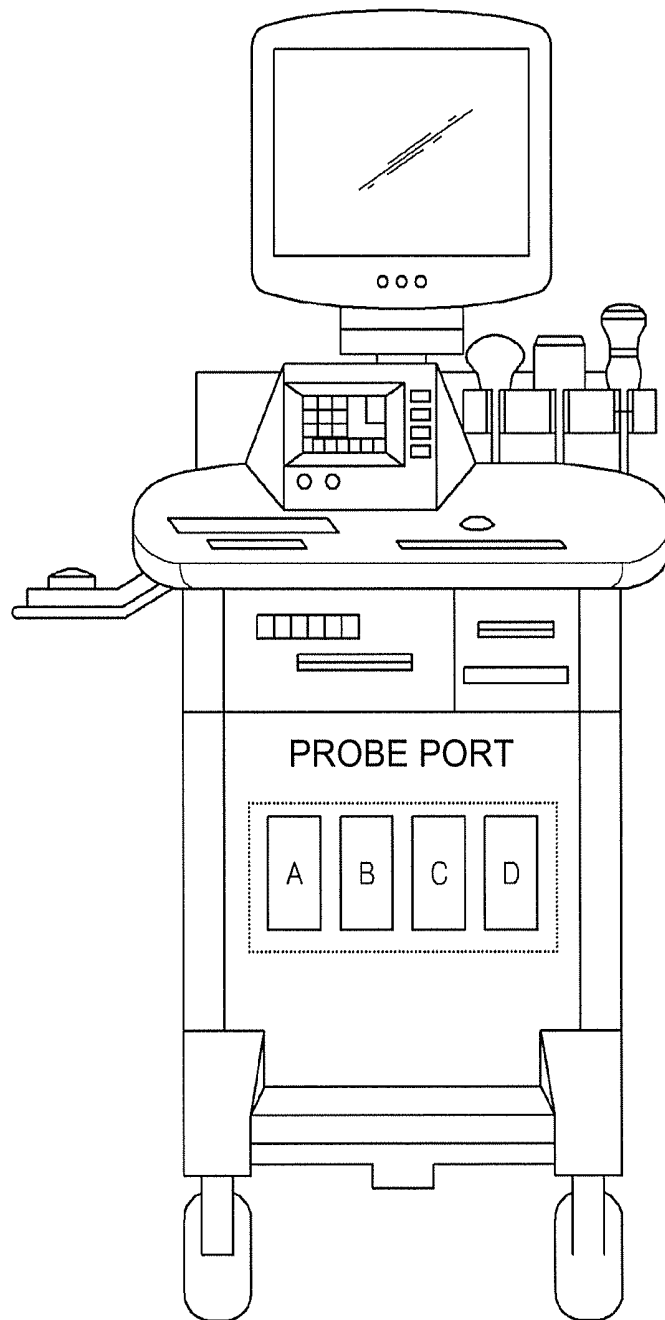
100

FIG. 2

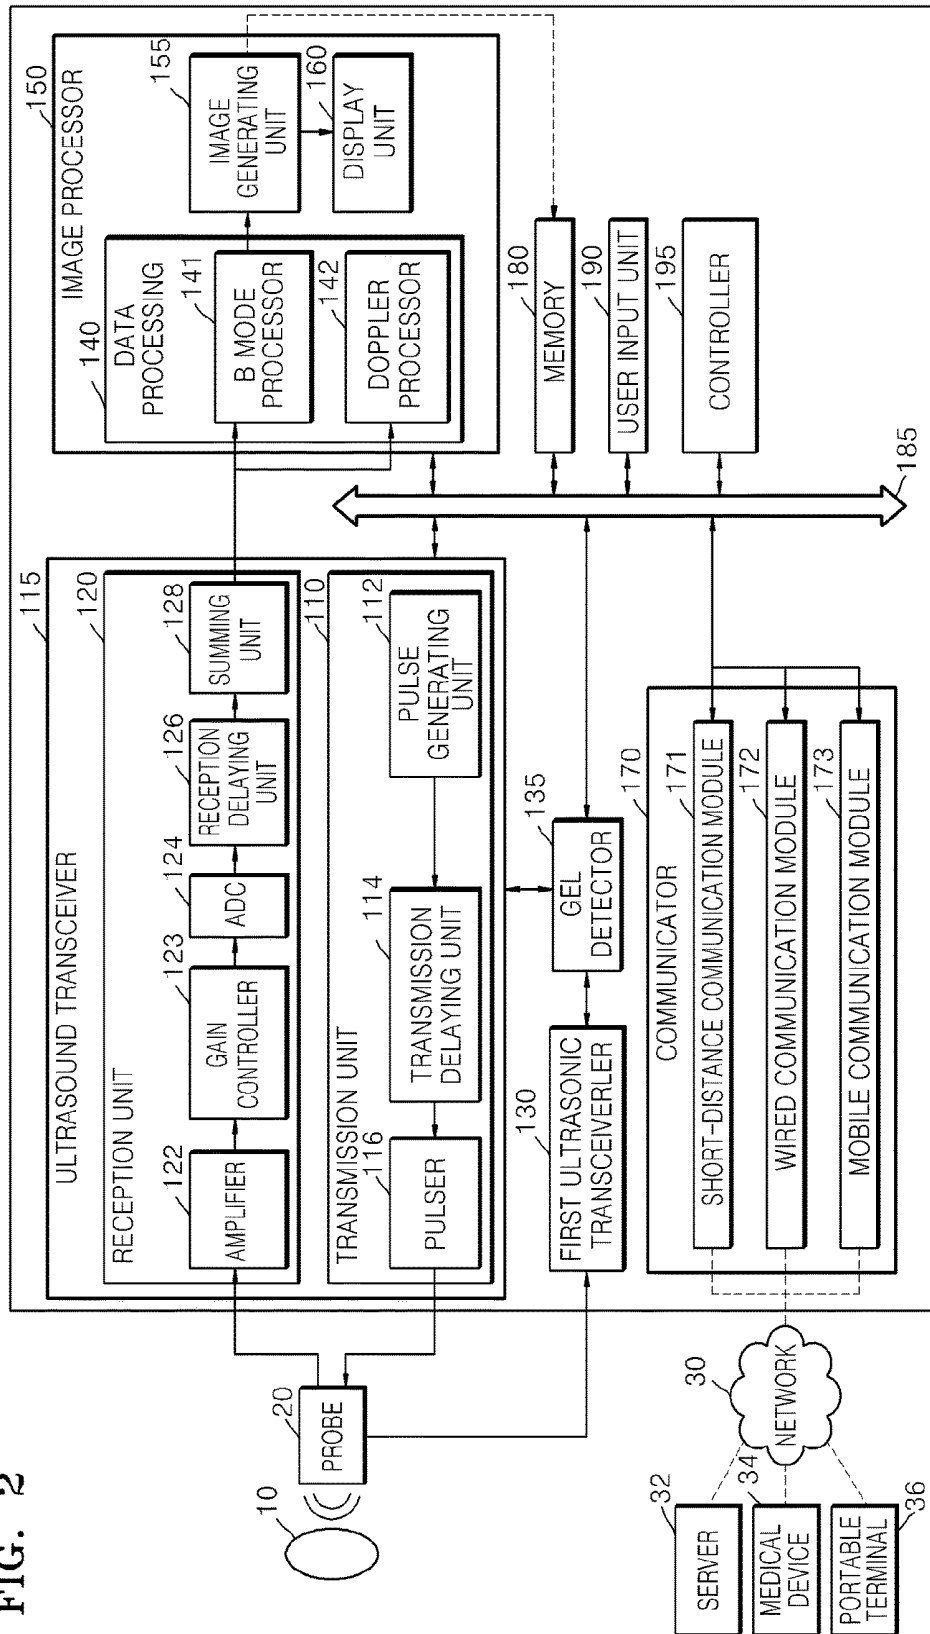


FIG. 3

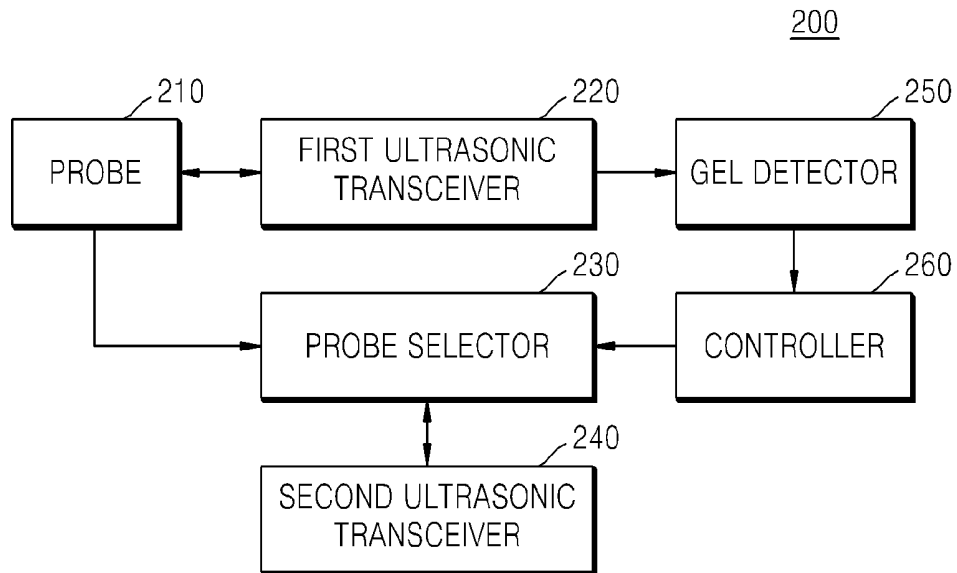


FIG. 4

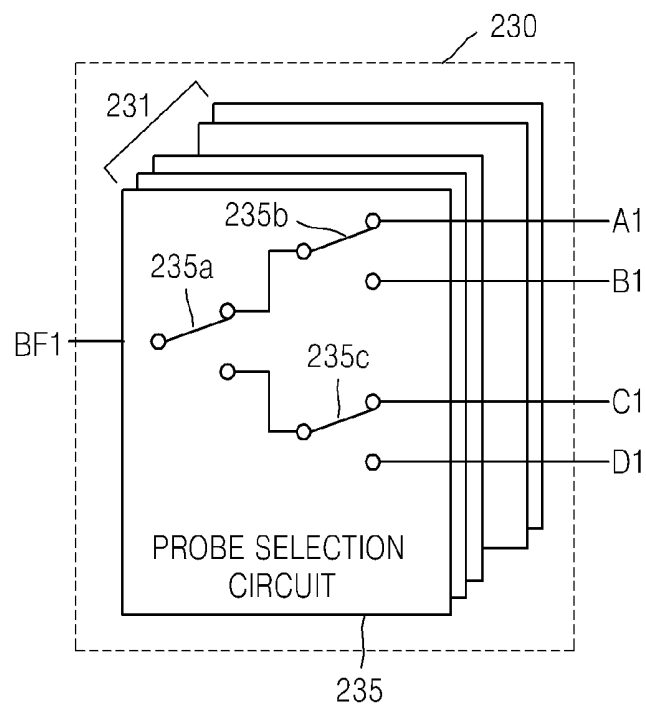


FIG. 5

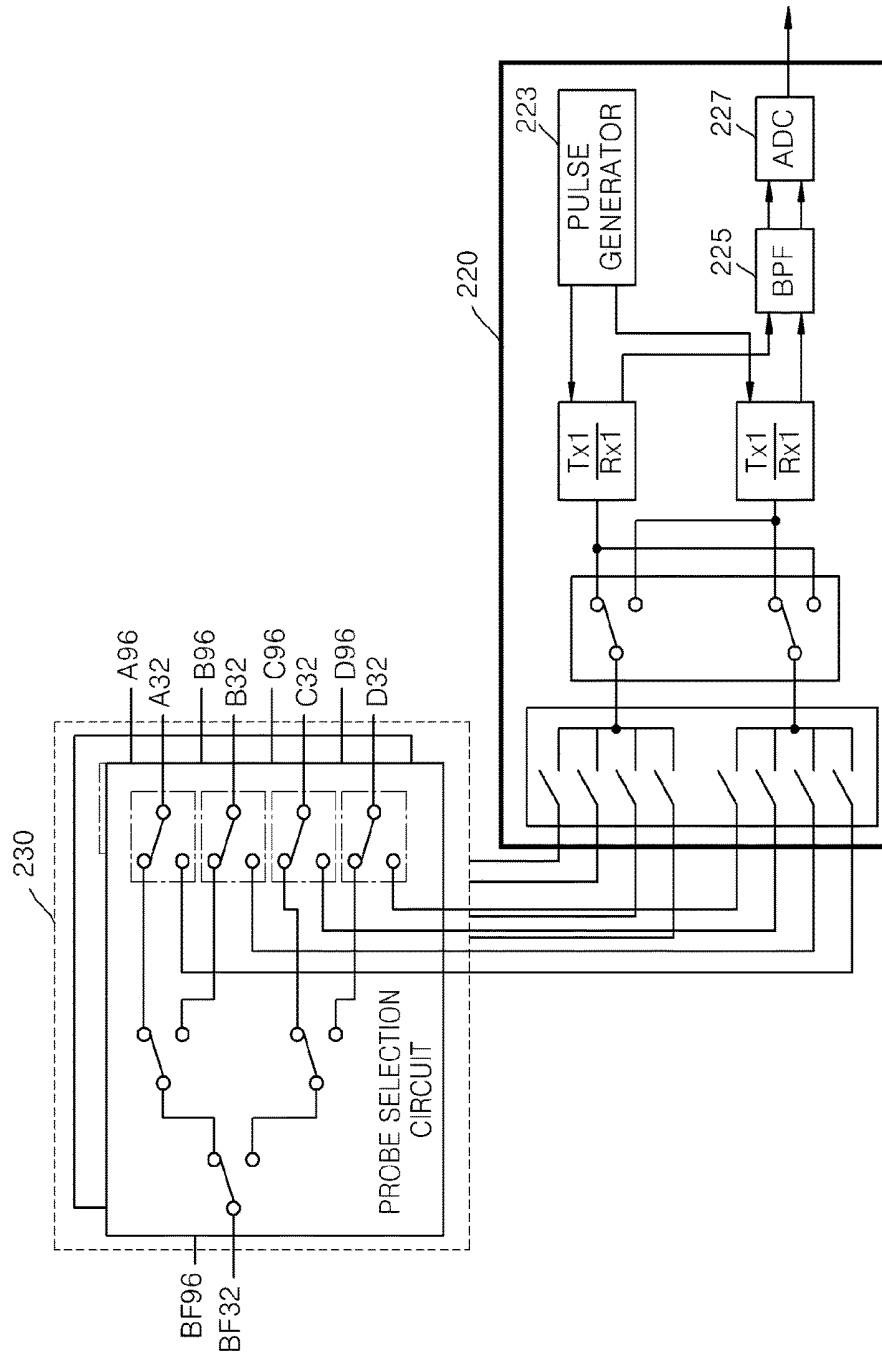


FIG. 6

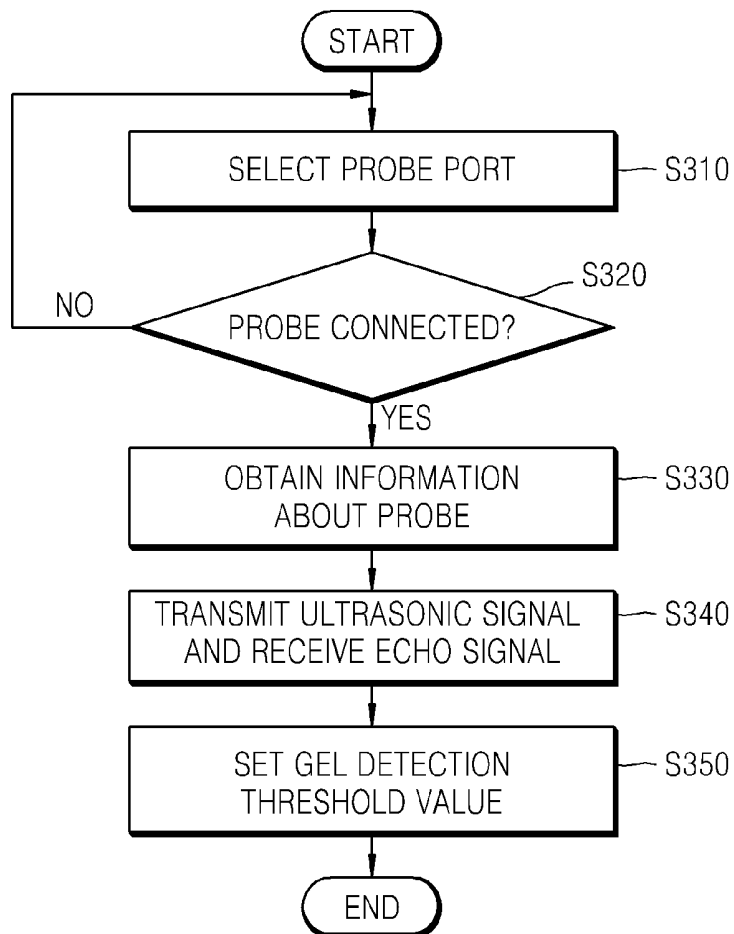


FIG. 7A

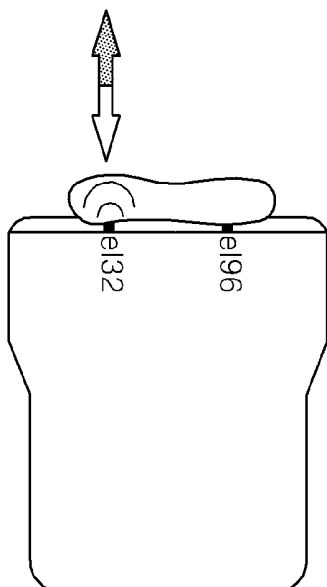


FIG. 7B

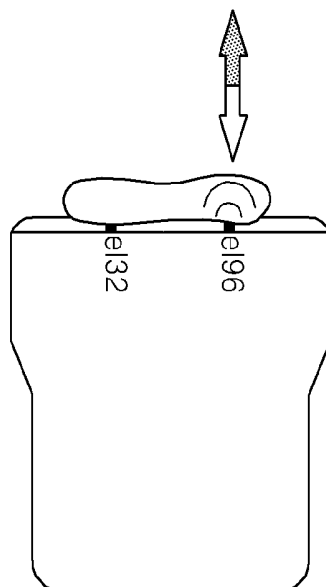


FIG. 7C

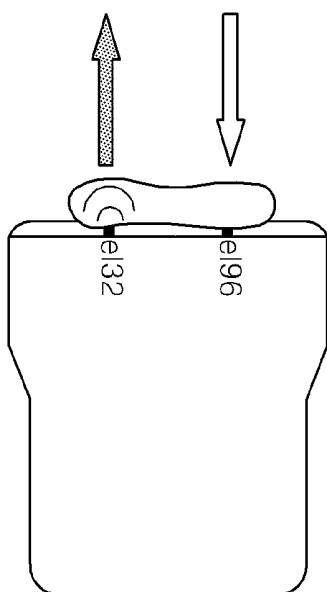


FIG. 7D


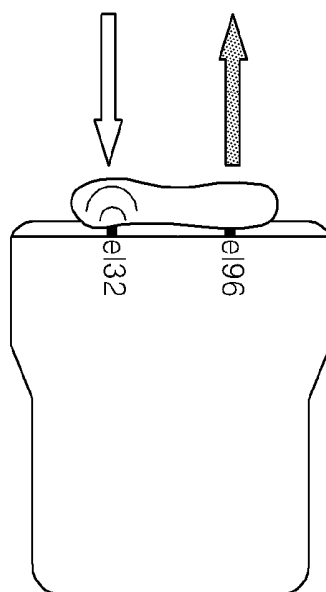


FIG. 8

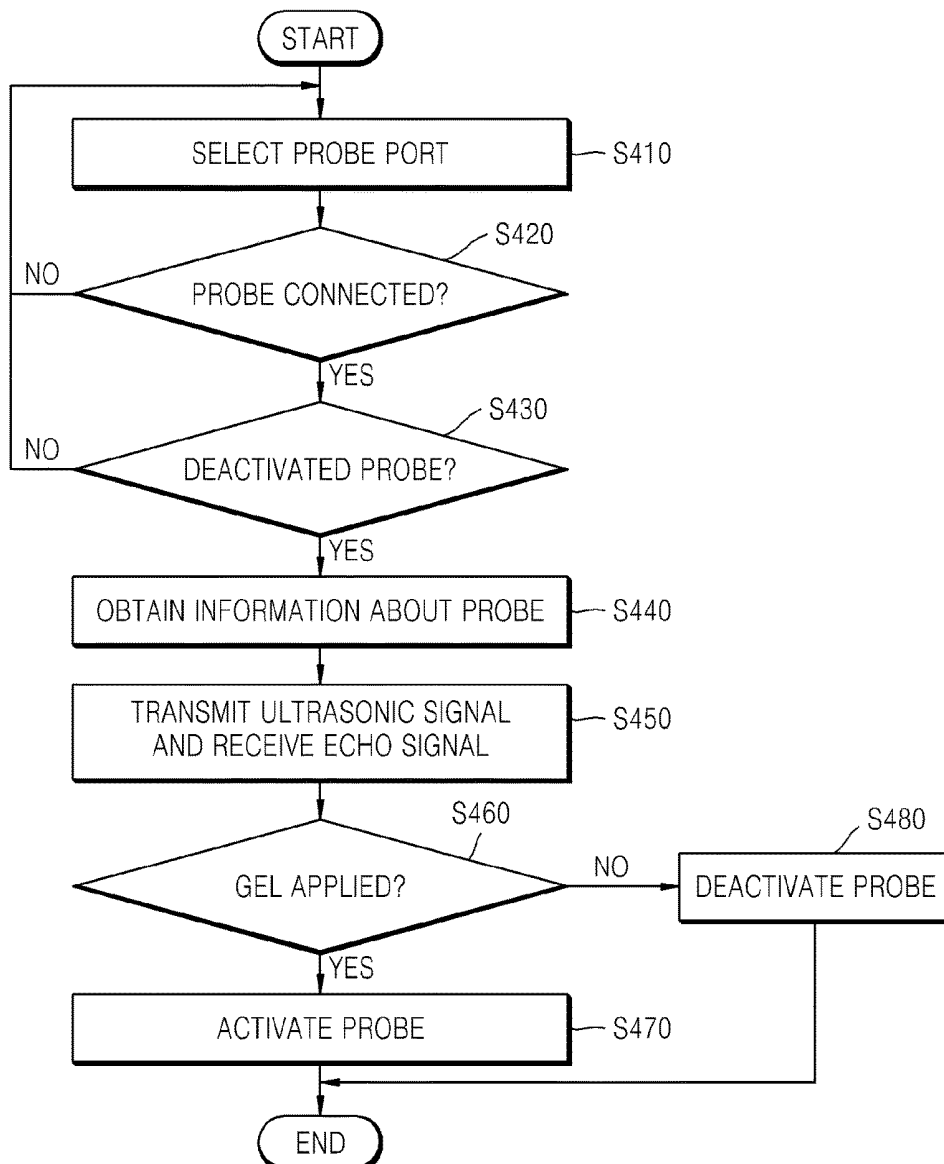

ULTRASONIC DIAGNOSTIC APPARATUS AND METHOD OF OPERATING THE SAME

RELATED APPLICATIONS

This application claims the benefit of Korean Patent Application No. 10-2014-0031820, filed on Mar. 18, 2014, in the Korean Intellectual Property Office, the disclosure of which is incorporated herein in its entirety by reference.

BACKGROUND

1. Field

One or more embodiments of the present invention relate to an ultrasonic diagnostic apparatus and a method of operating the same, and more particularly, to an ultrasonic diagnostic apparatus capable of automatically changing a probe, and a method of operating the same.

2. Description of the Related Art

An ultrasonic diagnostic apparatus irradiates an ultrasonic signal generated by a transducer of a probe to a target object, and receives information about an echo signal reflected from the target object to obtain an image of a region inside the target object. In detail, the ultrasonic diagnostic apparatus is used for medical purposes, for example, to observe the inside of the target object, to detect a foreign substance, and to measure an injury. Such an ultrasonic diagnostic apparatus is widely used together with another imaging diagnostic apparatus since the ultrasonic diagnostic apparatus has high stability compared to a diagnostic apparatus using an X-ray, is capable of displaying an image in real-time, and is safe because of no radiation exposure.

Meanwhile, the ultrasonic diagnostic apparatus may provide a brightness (B) mode that displays reflection coefficients of an ultrasonic signal reflected from a target object in a 2-dimensional (2D) image, a Doppler mode that displays an image of a moving target object, in detail, a blood flow, by using a Doppler effect, an elastic mode that displays an image showing a difference between a reaction when compression is applied to a target object and a reaction when compression is not applied.

SUMMARY

One or more embodiments of the present invention include an ultrasonic diagnostic apparatus that is capable of automatically changing a probe by determining a will of a user to change the probe, for example, an act of applying gel to the probe, and a method of operating the ultrasonic diagnostic apparatus.

Additional aspects will be set forth in part in the description which follows and, in part, will be apparent from the description, or may be learned by practice of the presented embodiments.

According to one or more embodiments of the present invention, an ultrasonic diagnostic apparatus includes: a first ultrasonic transceiver that transmits an ultrasonic signal and receives a first echo signal that is reflected, through a deactivated probe from among a plurality of probes; a gel detector that determines whether gel is applied on the deactivated probe based on the first echo signal; and a controller that activates the deactivated probe when it is determined that the gel is applied on the deactivated probe.

The controller may obtain information about the deactivated probe, and the first ultrasonic transceiver, based on the obtained information, may determine a transmission frequency of the ultrasonic signal and a reception bandwidth of

the first echo signal, transmit the ultrasonic signal according to the determined transmission frequency, and receive the first echo signal according to the determined reception bandwidth.

The deactivated probe may include at least one element, and the first ultrasonic transceiver may transmit the ultrasonic signal and receive the first echo signal through the at least one element.

The deactivated probe may include a first element and a second element, and the first ultrasonic transceiver may operate in at least one of a first mode for transmitting the ultrasonic signal and receiving the first echo signal through the first element, a second mode for transmitting the ultrasonic signal and receiving the first echo signal through the second element, a third mode for transmitting the ultrasonic signal through the first element and receiving the first echo signal through the second element, and a fourth mode for transmitting the ultrasonic signal through the second element and receiving the first echo signal through the first element.

The first ultrasonic transceiver, based on information about a probe among the plurality of probes, may transmit an ultrasonic signal to the probe on which gel is applied, and receive a second echo signal, the controller may set a gel detection threshold value based on the second echo signal, and the gel detector may determine whether the gel is applied on the deactivated probe by comparing a value of the first echo signal and the gel detection threshold value.

The gel detector may determine that the gel is applied on the deactivated probe when the value of the first echo signal is higher than the gel detection threshold value.

The ultrasonic diagnostic apparatus may further include: a beam former that performs beamforming by receiving an ultrasonic signal from an activated probe from among the plurality of probes; and a probe selector that deactivates at least one probe from among the plurality of probes by electrically disconnecting the at least one probe from the beam former, or activates the at least one probe by electrically connecting the at least one probe to the beam former.

The ultrasonic diagnostic apparatus may further include: a second ultrasonic transceiver that transmits an ultrasonic signal to an activated probe from among the plurality of probes, and receives a third echo signal that is reflected; and an image generator that generates an ultrasonic image based on the third echo signal.

According to one or more embodiments of the present invention, a method of operating an ultrasonic diagnostic apparatus, the method includes: transmitting an ultrasonic signal and receiving a first echo signal that is reflected, through a deactivated probe from among a plurality of probes; determining whether gel is applied on the deactivated probe based on the received first echo signal; and activating the deactivated probe when it is determined that the gel is applied on the probe.

The method may further include obtaining information about the deactivated probe, wherein the transmitting of the ultrasonic signal and receiving of the first echo signal may include, based on the obtained information, determining a transmission frequency of the ultrasonic signal and a reception bandwidth of the first echo signal, transmitting the ultrasonic signal according to the determined transmission frequency, and receiving the first echo signal according to the determined reception bandwidth.

The deactivated probe may include at least one element, and the transmitting of the ultrasonic signal and receiving of

the first echo signal may include transmitting the ultrasonic signal and receiving the first echo signal through the at least one element.

The deactivated probe may include a first element and a second element, and the transmitting of the ultrasonic signal and receiving of the first echo signal may include at least one of operating in a first mode for transmitting the ultrasonic signal and receiving the first echo signal through the first element, operating in a second mode for transmitting the ultrasonic signal and receiving the first echo signal through the second element, operating in a third mode for transmitting the ultrasonic signal through the first element and receiving the first echo signal through the second element, and operating in a fourth mode for transmitting the ultrasonic signal through the second element and receiving the first echo signal through the first element.

The method may further include: based on information about a probe among the plurality of probes, transmitting an ultrasonic signal to the probe on which gel is applied, and receiving a second echo signal; and based on the second echo signal, setting a gel detection threshold value, wherein the determining of whether the gel is applied on the deactivated probe may include determining whether the gel is applied on the deactivated probe by comparing a value of the first echo signal and the gel detection threshold value.

The determining of whether the gel is applied on the deactivated probe may include determining that the gel is applied on the deactivated probe when the value of the first echo signal is higher than the gel detection threshold value.

The method may further include: deactivating at least one probe from among the plurality of probes by electrically disconnecting the at least one probe from a beam former or activating the at least one probe by electrically connecting the at least one probe to the beam former; and performing beamforming by receiving an ultrasonic signal from an activated probe from among the plurality of probes.

The method may further include: transmitting an ultrasonic signal to an activated probe from among the plurality of probes, and receiving a third echo signal that is reflected; and generating an ultrasonic image based on the third echo signal.

BRIEF DESCRIPTION OF THE DRAWINGS

These and/or other aspects will become apparent and more readily appreciated from the following description of the embodiments, taken in conjunction with the accompanying drawings in which:

FIG. 1 is a diagram of an exterior of an ultrasonic diagnostic apparatus, according to an embodiment of the present invention;

FIG. 2 is a block diagram of an ultrasonic diagnostic apparatus according to an embodiment of the present invention;

FIG. 3 is a block diagram of an ultrasonic diagnostic apparatus according to another embodiment of the present invention;

FIG. 4 is a diagram for describing a probe selector of FIG. 3;

FIG. 5 is a diagram for describing a first ultrasonic transceiver of FIG. 3;

FIG. 6 is a flowchart of a method of operating an ultrasonic diagnostic apparatus, according to an embodiment of the present invention;

FIGS. 7 (a), 7 (b), 7 (c) and 7 (d) illustrate reference diagrams for describing the method of FIG. 6; and

FIG. 8 is a flowchart of a method of operating an ultrasonic diagnostic apparatus, according to another embodiment of the present invention.

DETAILED DESCRIPTION

The terms used in this specification are those general terms currently widely used in the art in consideration of functions in regard to the present invention, but the terms may vary according to the intention of those of ordinary skill in the art, precedents, or new technology in the art. Also, specified terms may be selected by the applicant, and in this case, the detailed meaning thereof will be described in the detailed description of the invention. Thus, the terms used in the specification should be understood not as simple names but based on the meaning of the terms and the overall description of the invention.

Throughout the specification, it will also be understood that when a component "includes" an element, unless there is another opposite description thereto, it should be understood that the component does not exclude another element but may further include another element. In addition, terms such as "... unit", "... module", or the like refer to units that perform at least one function or operation, and the units may be implemented as hardware or software or as a combination of hardware and software.

Throughout the specification, an "ultrasonic image" refers to an image of a target object obtained using an ultrasonic wave. Furthermore, in the present specification, a "target object" may include a person or an animal, or a part of a person or an animal. For example, the target object may include the liver, the heart, the womb, the brain, a breast, the abdomen, or a blood vessel. Furthermore, the "target object" may include a phantom. A phantom is a material having a volume that is approximately the density and effective atomic number of a living thing, and may include a sphere phantom having a property similar to a human body.

An ultrasonic image may be variously realized. For example, an ultrasonic image may be at least one of an amplitude (A) mode image, a brightness (B) mode image, a color (C) mode image, and a Doppler (D) mode image. Alternatively, according to an embodiment of the present invention, an ultrasonic image may be a 2-dimensional (2D) image or a 3D image.

Furthermore, in the present specification, "user" refers to a medical professional, such as a doctor, a nurse, a medical laboratory technologist, or an engineer who repairs a medical apparatus, but the user is not limited thereto.

Expressions such as "at least one of," when preceding a list of elements, modify the entire list of elements and do not modify the individual elements of the list.

Embodiments of the invention now will be described more fully hereinafter with reference to the accompanying drawings, in which illustrative embodiments of the invention are shown.

FIG. 1 is a diagram of an exterior of an ultrasonic diagnostic apparatus 100, according to an embodiment of the present invention.

Referring to FIG. 1, the ultrasonic diagnostic apparatus 100 may include a plurality of probe ports A through D, and a plurality of probes may be connected to a main body of the ultrasonic diagnostic apparatus 100 via the probe ports A through D.

Accordingly, a user may respectively pre-connect the plurality of probes to the plurality of probe ports according to purpose, and may select and use at least one of the pre-connected probes according to diagnostic situations.

Here, the ultrasonic diagnostic apparatus **100** may automatically select a probe by determining whether gel is applied to a probe connected to a probe port. Also, the ultrasonic diagnostic apparatus **100** may activate the selected probe, transmit an ultrasonic signal to the activated probe, receive a reflected echo signal, and obtain an ultrasonic image.

Meanwhile, the ultrasonic diagnostic apparatus **100** according to an embodiment of the present invention may be embodied not only as a cart type apparatus, but also as a portable apparatus. Examples of portable ultrasonic diagnostic apparatuses may include a picture archiving and communications system (PACS) viewer, a smart phone, a laptop computer, a personal digital assistant (PDA), and a tablet PC, but are not limited thereto.

FIG. 2 is a block diagram of the ultrasonic diagnostic apparatus **100** according to an embodiment of the present invention.

Referring to FIG. 2, the ultrasonic diagnostic apparatus **100** may include a probe **20**, a first ultrasonic transceiver **130**, a second ultrasonic transceiver **115**, a gel detector **135**, an image processor **150**, a communication unit **170**, a memory **180**, a user input unit **190**, and a controller **195**, which may be connected to each other via a bus **185**.

The probe **20** transmits an ultrasonic signal to a target object **10** based on a driving signal applied by the first and second ultrasonic transceivers **130** and **115** and receives an echo signal reflected by the target object **10**. The probe **20** includes a plurality of transducer elements and the plurality of transducer elements oscillate based on electric signals transmitted thereto and generate acoustic energy, that is, ultrasonic waves. Furthermore, the probe **20** may be connected to a main body of the ultrasonic diagnostic apparatus **100** via wires or wirelessly. According to embodiments of the present invention, the ultrasonic diagnostic apparatus **100** may include a plurality of probes **20**.

The first and second ultrasonic transceivers **130** and **115** transmit an ultrasonic signal and receive an echo signal that is reflected, through the probe **20**.

Here, the first ultrasonic transceiver **130** may transmit and receive ultrasonic waves to detect whether gel is applied on a probe. The first ultrasonic transceiver **130** may determine a transmission frequency of an ultrasonic signal to be transmitted and a reception bandwidth of an echo signal to be received based on information about a probe, and may transmit an ultrasonic signal according to the determined transmission frequency and receive an echo signal according to the determined reception bandwidth.

Operations of the first ultrasonic transceiver **130** will be described in detail later with reference to FIGS. 6 through 8.

The gel detector **135** may determine whether gel is applied on the probe **20** based on the echo signal received by the first ultrasonic transceiver **130**. For example, when a value of the received echo signal is higher than a pre-set gel detection threshold value, the gel detector **135** may determine that gel is applied on the probe **20**. However, an embodiment of the present invention is not limited thereto.

Here, a gel detection threshold value may be set based on an echo signal reflected in response to a transmitted ultrasonic signal, through a probe on which gel is applied. Also, the set gel detection threshold value may be stored in the memory **180**.

The second ultrasonic transceiver **115** may transmit and receive ultrasonic signals to obtain an ultrasonic image, and may include a transmitter **110** and a receiver **120**.

The transmitter **110** supplies a driving signal to the probe **20** and includes a pulse generator **112**, a transmission delay **114**, and a pulser **116**. The pulse generator **112**

generates pulses for forming transmission ultrasonic signals based on a predetermined pulse repetition frequency (PRF), and the transmission delay **114** applies a delay time to the pulses in order to determine transmission directionality of ultrasonic signal. Pulses to which a delay time is applied correspond to a plurality of vibrators included in the probe **20**, respectively. The pulser **116** applies a driving signal (or a driving pulse) to the probe **20** at timing intervals corresponding to each pulse to which a delay time is applied.

The receiver **120** generates ultrasonic data by processing an echo signal received by the probe **20** and may include an amplifier **122**, an analog-digital converter (ADC) **124**, a reception delay **126**, and an adder **128**. The amplifier **122** amplifies echo signals in each channel, and the ADC **124** analog-to-digital converts the amplified echo signals. The reception delay **126** processes the digitally-converted echo signals by applying delay times for determining reception directionality to the digitally-converted echo signals, and the adder **128** generates ultrasonic data by adding the echo signals processed by the reception delay **126**.

The image processor **150** generates an ultrasonic image by scan-converting ultrasonic data generated by the second ultrasonic transceiver **115**, and displays the ultrasonic image.

Meanwhile, an ultrasonic image may include not only a grayscale ultrasonic image obtained by scanning a target object in an A mode, a B mode, and a motion (M) mode, but also a Doppler image showing movement of the target object. Examples of the Doppler image include a blood flow Doppler image showing flow of blood (i.e., a color Doppler image), a tissue Doppler image showing movement of tissues, and a spectral Doppler image showing the speed at which a target object moves as a waveform.

A B mode processor **141** extracts B mode components from ultrasonic data and processes the B mode components.

An image generator **155** may generate an ultrasonic image in which signal intensities are represented as brightness based on the extracted B mode components.

Similarly, a Doppler processor **142** may extract Doppler components from ultrasonic data, and the image generator **155** may generate a Doppler image indicating movement of a target object as colors or waveforms based on the extracted Doppler components.

The image generator **155** according to an embodiment of the present invention may generate a 2D ultrasonic image or may generate an elastic image in which deformation of the target object **10** according to pressure is visualized. Furthermore, the image generator **155** may display various types of additional information on an ultrasonic image by using text and graphics. Meanwhile, the generated ultrasonic image may be stored in the memory **180**.

A display unit **160** displays the generated ultrasonic image. The display unit **160** may display not only an ultrasonic image, but also various types of information processed by the ultrasonic diagnostic apparatus **100** on a screen via a graphic user interface (GUI). Meanwhile, the ultrasonic diagnostic apparatus **100** may include two or more display units **160** according to embodiments of the present invention.

The display unit **160** may include at least one of a liquid crystal display, a thin film transistor-liquid crystal display, an organic light-emitting diode, a flexible display, a 3D display, and an electrophoretic display.

When the display unit **160** and a user input unit are combined in a layer structure to form a touch screen, the display unit **160** may also be used as an input device capable of receiving information according to a touch of a user, as well as an output device.

The touch screen may be configured to detect not only a touched area but also a pressure applied to the touched area. Also, the touch screen may be configured to detect not only a real-touch but also a proximity touch.

Herein, a 'real-touch' indicates a case where a pointer actually touches a screen, and a 'proximity-touch' indicates a case where a pointer does not actually touch a screen but approaches the screen while still maintaining a predetermined distance therefrom. Herein, a pointer is a touching tool for touching or proximity-touching a certain portion of a displayed screen. Examples of the pointer include an electronic pen or a finger.

Although not shown, the ultrasonic diagnostic apparatus **100** may include various sensors inside or near a touch screen to detect a real-touch or a proximity touch on the touch screen. An example of a sensor for detecting a touch on a touch screen includes a tactile sensor.

A tactile sensor is a sensor for detecting, with sensitivity similar to that of a person, contact of a certain target object. The tactile sensor may detect various types of information, for example, roughness of a contact surface, rigidity of the certain target object, and a temperature of a contact point.

Another example of the sensor for detecting a touch on a touch screen includes a proximity sensor. The proximity sensor is a sensor for detecting an existence of a target object approaching or near a predetermined detection surface by using force of an electromagnetic field or an infrared light, without having to detect a mechanical touch.

Examples of the proximity sensor include a transmission type photoelectric sensor, a direct reflection type photoelectric sensor, a mirror reflection type photoelectric sensor, a high frequency oscillation type proximity sensor, a capacitance type proximity sensor, a magnetic proximity sensor, and an infrared proximity sensor.

The communication unit **170** connected to a network **30** via wires or wirelessly and communicates with an external device or a server. The communication unit **170** may exchange data with a hospital server or another medical device in a hospital that is connected with a picture archiving and communications system (PACS). Furthermore, the communication unit **170** may perform data communication according to the digital imaging and communications in medicine (DICOM) standard.

The communication unit **170** may transmit and receive data related to diagnosis of a target object, e.g., an ultrasonic image, ultrasonic data, and Doppler data of the target object, via the network **30** and may also transmit and receive medical images obtained via other medical devices, e.g., a CT image, a MR image, and an X-ray image. Furthermore, the communication unit **170** may receive information related to a diagnosis history or treatment schedule of a patient from a server and utilize the information to diagnose the patient. Furthermore, the communication unit **170** may perform data communication not only with a server or a medical device in a hospital, but also with a portable terminal of a doctor or a patient.

The communication unit **170** is connected to the network **30** via wires or wirelessly and may exchange data with a server **32**, a medical device **34**, or a portable terminal **36**. The communication unit **170** may include one or more components that enable communication with external devices, e.g., a close-distance communication module **171**, a wired communication module **172**, and a mobile communication module **173**.

The close-distance communication module **171** may refer to a module for close-distance communication within a predetermined distance. Examples of close-distance com-

munication techniques according to an embodiment of the present invention may include wireless LAN, Wi-Fi, Bluetooth, Zigbee, Wi-Fi Direct (WFD), ultra wideband (UWB), infrared data association (IrDA), Bluetooth Low Energy (BLE), and near field communication (NFC), but are not limited thereto.

The wired communication module **172** refers to a module for communication using electric signals or optical signals. Examples of wired communication techniques according to an embodiment of the present invention may include a pair cable, a coaxial cable, an optical fiber cable, and an Ethernet cable.

The mobile communication module **173** transmits and receives wireless signals with at least one from among a station, an external terminal, and a server on a mobile communication network. Here, the wireless signals may include voice call signals, video call signals, or various types of data for transmission and reception of text/multimedia messages.

The memory **180** stores various types of data processed by the ultrasonic diagnostic apparatus **100**. For example, the memory **180** may store medical data related to diagnosis of a target object, such as ultrasonic data and ultrasonic image that are input or output, and may also store algorithms or programs to be executed in the ultrasonic diagnostic apparatus **100**.

According to an embodiment of the present invention, the memory **180** may pre-map and store a cross section information image corresponding to cross section information of a target object. For example, the memory **180** may store a first cross section information image corresponding to first cross section information, and a second cross section information image corresponding to second cross section information. Cross section information may include various types of data for identifying cross sections of a target object. For example, the first cross section information may include data about a shape, a length, or an area of an object included only in an ultrasonic image of a first cross section of a target object, or may include a brightness value of a certain range only shown in the first cross section image.

The memory **180** may be embodied as any of various storage media, e.g., a flash memory, a hard disk drive, an EEPROM, etc. Furthermore, the ultrasonic diagnostic apparatus **100** may utilize a web storage server or a cloud server that functions as the memory **180** online.

The user input unit **190** generates input data that is input by the user to control operations of the ultrasonic diagnostic apparatus **100**. The user input unit **190** may include hardware components, such as a keypad, a mouse, a touch pad, a track ball, and a jog switch, but alternatively, the user input unit **190** may further include various components, such as an electrocardiogram measuring module, a respiration measuring module, a voice recognition sensor, a gesture recognition sensor, a fingerprint recognition sensor, an iris recognition sensor, a depth sensor, a distance sensor, etc.

According to an embodiment of the present invention, the user input unit **190** may receive a user input for selecting any one of a first ultrasonic image and a second ultrasonic image, or may receive a user input for selecting any one of a plurality of cross sections included in a cross section information image.

In detail, a touch pad may include a touch screen that has a layer structure including the display unit **160** described above.

Here, the ultrasonic diagnostic apparatus **100** according to an embodiment of the present invention may display an ultrasonic image in a predetermined mode and a control

panel for the ultrasonic image on a touch screen. Also, the ultrasonic diagnostic apparatus **100** may detect a touch gesture of a user on the ultrasonic image through the touch screen.

The ultrasonic diagnostic apparatus **100** according to an embodiment of the present invention may physically provide, in a control panel of a general ultrasonic apparatus, buttons which are frequently used by a user, while providing remaining buttons via a touch screen in forms of a GUI.

The controller **195** may control overall operations of the ultrasonic diagnostic apparatus **100**. In other words, the controller **195** may control operations among the probe **20**, the first and second ultrasonic transceivers **130** and **115**, the image processor **150**, the communication unit **170**, the memory **180**, and the user input unit **190** of FIG. 2.

All or some of the probe **20**, the second ultrasonic transceiver **115**, the image processor **150**, the communication unit **170**, the memory **180**, the user input unit **190**, and the controller **195** may be implemented as software modules. However, an embodiment of the present invention is not limited thereto, and some of the components stated above may be implemented as hardware modules. Furthermore, at least one of the second ultrasonic transceiver **115**, the image processor **150**, and the communication unit **170** may be included in the controller **195**. However, an embodiment of the present invention is not limited thereto.

FIG. 3 is a block diagram of an ultrasonic diagnostic apparatus **200** according to another embodiment of the present invention, FIG. 4 is a diagram for describing a probe selector **230** of FIG. 3, and FIG. 5 is a diagram for describing a first ultrasonic transceiver **220** of FIG. 3.

Referring to FIG. 3, the ultrasonic diagnostic apparatus **200** may include a probe **210**, the probe selector **230**, the first ultrasonic transceiver **220**, a second ultrasonic transceiver **240**, a gel detector **250**, and a controller **260**.

The probe **210** of FIG. 3 corresponds to the probe **20** of FIG. 2, and may include a plurality of transducer elements. Each transducer element may transmit an ultrasonic signal to a target object according to a driving signal applied from the first or second ultrasonic transceiver **220** or **240**, and may receive an echo signal reflected from the target object.

The probe selector **230** may activate at least one of a plurality of the probes **210** respectively connected to probe ports. In order to obtain an ultrasonic image, an activated probe may transmit an ultrasonic signal to a target object according to a driving signal applied from the second ultrasonic transceiver **240**, and receive an echo signal reflected from the target object.

For example, the second ultrasonic transceiver **240** of FIG. 3 may include a beam former, and a probe activated by the probe selector **230** may be electrically connected to the beam former. Here, the beam former may include the transmitter **110** and the receiver **120** of FIG. 2.

Referring to FIG. 4, the probe selector **230** may include a plurality of probe selection circuits for connecting the beam former and the probe port. For example, when the probe **210** includes 128 transducer elements, the second ultrasonic transceiver **240** includes 128 beam forming circuits, and 128 channels are formed, the probe selector **230** may include 128 probe selection circuits **231**, i.e., first through 128th probe selection circuits.

Hereinafter, for convenience of description, one or more embodiments of the present invention will be described based on a first probe selection circuit **235** that is one of the 128 probe selection circuits **231**. Accordingly, descriptions about the first probe selection circuit **235** may also be applied to the second through 128th probe selection circuits.

As shown in FIG. 4, the first probe selection circuit **235** may include a mechanical or electronic switch (hereinafter, referred to as a switch), and for example, when the number of probe ports is 4, the first probe selection circuit **235** may include three switches **235a** through **235c**, but an embodiment of the present invention is not limited thereto.

For example, when a probe port A in FIG. 1 is to be connected to a beam former BF, the first probe selection circuit **235** may use the two switches **235a** and **235b** to electrically connect a probe port A1 corresponding to the first channel to a beam former BF1. Similarly to the first probe selection circuit **235**, the second through 128th probe selection circuits may electrically connect probe ports A2 through A128 corresponding to second through 128th channels to beam formers BF2 through BF128, respectively.

Accordingly, the second ultrasonic transceiver **240** may process an echo signal received through the activated probe.

In order to determine whether gel is applied on a probe connected to a probe port, the first ultrasonic transceiver **220** may apply a driving signal to the probe and receive an echo signal. For example, referring to FIG. 5, the first ultrasonic transceiver **220** may include circuits connected to a plurality of probe ports, and the first ultrasonic transceiver **220** may use a plurality of switches to electrically connect probe ports corresponding to certain elements (in FIG. 5, 32nd and 96th elements included in a plurality of probes to pulse transmitter Tx1 and Tx2 or receivers Rx1 and Rx2. Here, the certain elements may be changed according to probes or to improve functions.

Also, the first ultrasonic transceiver **220** includes a pulse generator **223**, and the pulse generator **223** may generate a pulse having a frequency in a physically transmittable band in a probe based on probe information, and transmit the generated pulse to the pulse transmitters Tx1 and Tx2.

Also, the first ultrasonic transceiver **220** may include a band pass filter (BPF) **225**, and may input a signal having a bandwidth through which the frequency in the transmittable band may pass, from among signals received by the receivers Rx1 and Rx2, to an ADC **227**.

The echo signal that is processed may be input to the gel detector **250**, and the gel detector **250** may determine whether gel is applied on a probe based on a value of the echo signal.

The gel detector **250** may compare the value of the echo signal and a pre-set gel detection threshold value, and determine that the gel is applied on the probe when the value of the echo signal is higher than the pre-set gel detection threshold value. Setting of a gel detection threshold value will be described in detail later with reference to FIGS. 6 and 7.

When it is determined that the gel is applied on the probe, the controller **260** may activate the probe. For example, the controller **260** may transmit a probe change command to the probe selector **230** to deactivate a currently activated probe and activate the probe on which the gel is applied.

Meanwhile, the ultrasonic diagnostic apparatuses **100** and **200** of FIGS. 2 and 3 are only examples, and components of the ultrasonic diagnostic apparatuses **100** and **200** may be combined or omitted, or a new component may be added based on specifications of an actual ultrasonic diagnostic apparatus. In other words, two or more components may be combined into one component or one component may be divided into two or more components if required. Also, functions performed by each component are for describing one or more embodiments of the present invention, and detailed operations or apparatuses do not limit the scope of the invention.

FIG. 6 is a flowchart of a method of operating the ultrasonic diagnostic apparatus **100** or **200**, according to an embodiment of the present invention, and FIG. 7 illustrates reference diagrams for describing the method of FIG. 6.

Referring to FIG. 6, the ultrasonic diagnostic apparatus **100** or **200** selects a probe port in operation **S310**, and may determine whether a probe is connected to the selected probe port in operation **S320**. For example, as shown in FIG. 1, when the ultrasonic diagnostic apparatus **100** includes four probe ports A through D, it may be determined whether a probe is connected to the probe ports A through D.

When it is determined that the probe is connected to the selected probe port, the ultrasonic diagnostic apparatus **100** or **200** may obtain information about the connected probe in operation **S330**.

For example, an identification (ID) of the probe connected to the probe port may be recognized and then compared to a pre-stored ID of the probe, and corresponding information about the probe may be obtained.

Also, the ultrasonic diagnostic apparatus **100** or **200** may transmit an ultrasonic signal and receive an echo signal through a probe on which gel is applied based on the obtained information, in operation **S340**.

Here, the ultrasonic diagnostic apparatus **100** or **200** may transmit an ultrasonic signal having a transmission frequency that is physically transmittable from the probe, and receive an echo signal having a reception bandwidth corresponding to the transmission frequency, based on the information. Also, the ultrasonic diagnostic apparatus **100** or **200** may transmit an ultrasonic signal and receive an echo signal through at least one element included in the probe. Here, the ultrasonic diagnostic apparatus **100** or **200** may transmit an ultrasonic signal and receive an echo signal through first and second elements included in the probe.

For example, referring to FIG. 7, when the probe has 128 elements, the first element may be a 32nd element **el32**, and the second element may be a 96th element **el96**. However, an embodiment of the present invention is not limited thereto, and any number of elements may be selected in any method.

As shown in FIG. 7 (a), the ultrasonic diagnostic apparatus **100** or **200** may transmit an ultrasonic signal through the first element (32nd element **el32**) and receive an echo signal through the first element (32nd element **el32**) in a first mode.

Alternatively, as shown in FIG. 7 (b), the ultrasonic diagnostic apparatus **100** or **200** may transmit an ultrasonic signal through the second element (96th element **el96**) and receive an echo signal through the second element (96th element **el96**) in a second mode.

Alternatively, as shown in FIG. 7 (c), the ultrasonic diagnostic apparatus **100** or **200** may transmit an ultrasonic signal through the first element (32nd element **el32**) and receive an echo signal through the second element (96th element **el96**) in a third mode.

Alternatively, as shown in FIG. 7 (d), the ultrasonic diagnostic apparatus **100** or **200** may transmit an ultrasonic signal through the second element (96th element **el96**) and receive an echo signal through the first element (32nd element **el32**) in a fourth mode.

However, operations of the first ultrasonic transceiver **220** are not limited to the first through fourth modes described above, and the first ultrasonic transceiver **220** may transmit an ultrasonic signal and receive an echo signal in any operation mode based on the number of elements for transmitting an ultrasonic signal and receiving an echo signal.

Meanwhile, the first ultrasonic transceiver **220** may set a gel detection threshold value based on the received echo signal in operation **S350**.

For example, when the first ultrasonic transceiver **220** receives echo signals by operating in the first through fourth modes described above with reference to FIG. 7, the first ultrasonic transceiver **220** may set first through fourth gel detection threshold values based on the echo signals received in the first through fourth modes. Also, the first through fourth gel detection threshold values may be stored in the memory **180**.

Meanwhile, a gel detection threshold value may be set by performing operations **S330** through **S350** on another probe connected to another probe port.

When power is supplied to the ultrasonic diagnostic apparatus **100** or **200**, operations **S310** through **S350** of FIG. 6 are performed, and then operations **S310** through **S350** of FIG. 6 may be performed whenever a connected probe is changed by monitoring whether a new probe is connected to a probe port.

FIG. 8 is a flowchart of a method of operating the ultrasonic diagnostic apparatus **100** or **200**, according to another embodiment of the present invention.

Referring to FIG. 8, the ultrasonic diagnostic apparatus **100** or **200** may select any one of a plurality of probe ports in operation **S410** and determine whether a probe is connected to the selected probe port in operation **S420**.

Here, when a probe is not connected, the ultrasonic diagnostic apparatus **100** or **200** may select another probe port to determine whether a probe is connected to the other probe port.

On the other hand, when a probe is already connected to a probe port, the ultrasonic diagnostic apparatus **100** or **200** may determine whether the connected probe is a deactivated probe in operation **S430**. For example, the ultrasonic diagnostic apparatus **100** or **200** may check a connection state between the probe port to which a probe is connected and the second ultrasonic transceiver **115** or **240** to determine whether the probe is a deactivated probe.

When the probe is an activated probe, the ultrasonic diagnostic apparatus **100** or **200** may select another probe port to perform operations **S420** and **S430**.

On the other hand, when the probe is a deactivated probe, the ultrasonic diagnostic apparatus **100** or **200** may obtain information about the deactivated probe in operation **S440**.

For example, an ID of the probe connected to the probe port may be recognized and then compared with a pre-stored ID of the probe, and corresponding information about the probe may be obtained.

Also, the ultrasonic diagnostic apparatus **100** or **200** may transmit an ultrasonic signal and receive an echo signal in operation **S450** through the deactivated probe, based on the obtained information.

Here, the ultrasonic diagnostic apparatus **100** or **200** may transmit an ultrasonic signal having a transmission frequency that is physically transmittable from the probe, and receive an echo signal having a reception bandwidth corresponding to the transmission frequency, based on the information about the probe.

Also, the ultrasonic diagnostic apparatus **100** or **200** may transmit an ultrasonic signal and receive an echo signal through at least one element included in the probe. Here, the ultrasonic diagnostic apparatus **100** or **200** may transmit an ultrasonic signal and receive an echo signal through first and second elements included in the probe, and for example, as

described above with reference to FIG. 7, may transmit an ultrasonic signal and receive an echo signal in one of the first through fourth modes.

Accordingly, the ultrasonic diagnostic apparatus **100** or **200** may receive a first echo signal in the first mode, a second echo signal in the second mode, a third echo signal in the third mode, and a fourth echo signal in the fourth mode, and may obtain values of the first through fourth echo signals.

Also, the ultrasonic diagnostic apparatus **100** or **200** may determine whether gel is applied on the deactivated probe in operation **S460** by comparing a gel detection threshold value that is pre-set according to the method described above with reference to FIG. 6, and the value of the echo signal obtained in operation **S450**.

For example, the ultrasonic diagnostic apparatus **100** or **200** may determine that the gel is applied on the probe when the value of the echo signal is higher than the gel detection threshold value. Alternatively, the ultrasonic diagnostic apparatus **100** or **200** may determine whether the gel is applied on the probe by comparing the values of the first through fourth echo signals respectively with first through fourth gel detection threshold values.

When it is determined that the gel is applied on the probe, the ultrasonic diagnostic apparatus **100** or **200** may activate the probe in operation **S470**.

For example, a probe change command may be transmitted to the probe selector **230** to deactivate a currently activated probe and activate the probe on which the gel is applied.

On the other hand, when it is determined that the gel is not applied on the probe, the ultrasonic diagnostic apparatus **100** or **200** may maintain the probe to be in a deactivated state in operation **S480**.

As described above, according to the one or more of the above embodiments of the present invention, a process of changing a probe may be removed or reduced by manipulating a control panel of an ultrasonic diagnostic apparatus, thereby increasing convenience of using the ultrasonic diagnostic apparatus and reducing an ultrasonic diagnosis time.

Also, a user may be less stressed by preventing repeated operations of changing a probe by manipulating the control panel.

The invention can also be embodied as computer readable codes on a computer readable recording medium. The computer readable recording medium is any data storage device that can store data which can be thereafter read by a computer system. Examples of the computer readable recording medium include read-only memory (ROM), random-access memory (RAM), CD-ROMs, magnetic tapes, floppy disks, optical data storage devices, etc. The computer readable recording medium can also be distributed over network coupled computer systems so that the computer readable code is stored and executed in a distributed fashion.

While this invention has been particularly shown and described with reference to embodiments thereof, it will be understood by those of ordinary skill in the art that various changes in form and details may be made therein without departing from the spirit and scope of the invention as defined by the appended claims. The embodiments should be considered in a descriptive sense only and not for purposes of limitation. Therefore, the scope of the invention is defined not by the detailed description of the invention but by the appended claims, and all differences within the scope will be construed as being included in the present invention.

What is claimed is:

1. An ultrasonic diagnostic apparatus comprising:

a first ultrasonic transceiver that transmits an ultrasonic signal by applying a first driving signal to a deactivated probe from among a plurality of probes connected to probe ports of the ultrasonic diagnostic apparatus, and receives a first echo signal that is reflected, through the deactivated probe; and

a controller that determines whether gel is applied on the deactivated probe based on the first echo signal and activates the deactivated probe when the gel is applied on the deactivated probe by electrically connecting the deactivated probe to a beam former in a second ultrasonic transceiver of the ultrasonic diagnostic apparatus, wherein the second ultrasonic transceiver transmits an ultrasonic signal to an object by applying a second driving signal to the activated probe from among the plurality of probes, and receives a second echo signal that is reflected from the object, through the activated probe, and

wherein the controller generates an ultrasonic image representing the object based on the second echo signal.

2. The ultrasonic diagnostic apparatus of claim 1, wherein the controller obtains a transmission frequency and a reception bandwidth corresponding to the deactivated probe, based on identification information of the deactivated probe, and

the first ultrasonic transceiver transmits the ultrasonic signal according to the transmission frequency, and receives the first echo signal according to the reception bandwidth.

3. The ultrasonic diagnostic apparatus of claim 1, wherein the first ultrasonic transceiver transmits the ultrasonic signal and receives the first echo signal by applying the driving signal to one or two transducer elements from among a plurality of transducer elements of the deactivated probe.

4. The ultrasonic diagnostic apparatus of claim 1, wherein the deactivated probe comprises a first transducer element and a second transducer element, and

the first ultrasonic transceiver operates in at least one of a first mode for transmitting the ultrasonic signal and receiving the first echo signal through the first transducer element, a second mode for transmitting the ultrasonic signal and receiving the first echo signal through the second transducer element, a third mode for transmitting the ultrasonic signal through the first transducer element and receiving the first echo signal through the second transducer element, and a fourth mode for transmitting the ultrasonic signal through the second transducer element and receiving the first echo signal through the first transducer element.

5. The ultrasonic diagnostic apparatus of claim 1, wherein the controller determines that the gel is applied on the deactivated probe when a value of the first echo signal is higher than a gel detection threshold value.

6. The ultrasonic diagnostic apparatus of claim 1, wherein the controller deactivates a preactivated probe from among the plurality of probes by electrically disconnecting the preactivated probe from the beam former in the second ultrasonic transceiver.

7. The ultrasonic diagnostic apparatus of claim 1, wherein the controller determines a probe from among the plurality of probes as the deactivated probe based on whether the probe is connected to the beam former in the second ultrasonic transceiver.

15

8. A method of operating an ultrasonic diagnostic apparatus, the method comprising:

causing a first ultrasonic transceiver to transmit an ultrasonic signal by applying a first driving signal to a deactivated probe from among a plurality of probes connected to probe ports of the ultrasonic diagnostic apparatus, and receive a first echo signal that is reflected, through the deactivated probe;
determining whether gel is applied on the deactivated probe based on the received first echo signal;
activating the deactivated probe when the gel is applied on the deactivated probe by electrically connecting the deactivated probe to a beam former in a second ultrasonic transceiver of the ultrasonic diagnostic apparatus;
causing the second ultrasonic transceiver to transmit an ultrasonic signal to an object by applying a second driving signal to the activated probe, and receive a second echo signal that is reflected from the object, through the activated probe; and
generating an ultrasonic image representing the object based on the second echo signal.

9. The method of claim 8, further comprising obtaining a transmission frequency and a reception bandwidth corresponding to the deactivated probe, based on identification information of the deactivated probe,

wherein the causing the first ultrasonic transceiver to transmit of the ultrasonic signal and receive the first echo signal comprises causing the first ultrasonic transceiver to transmit the ultrasonic signal according to the transmission frequency, and receive the first echo signal according to the reception bandwidth.

10. The method of claim 8, wherein the causing the first ultrasonic transceiver to transmit of the ultrasonic signal and receive the first echo signal comprises causing the first ultrasonic transceiver to transmit the ultrasonic signal and receive the first echo signal by applying the driving signal to one or two transducer element from among a plurality of transducer elements of the deactivated probe.

11. The method of claim 8, wherein the deactivated probe comprises a first transducer element and a second transducer element, and

the causing the first ultrasonic transceiver to transmit the ultrasonic signal and receive the first echo signal comprises at least one of operating in a first mode for transmitting the ultrasonic signal and receiving the first echo signal through the first transducer element, operating in a second mode for transmitting the ultrasonic signal and receiving the first echo signal through the

16

second transducer element, operating in a third mode for transmitting the ultrasonic signal through the first transducer element and receiving the first echo signal through the second transducer element, and operating in a fourth mode for transmitting the ultrasonic signal through the second transducer element and receiving the first echo signal through the first transducer element.

12. The method of claim 8, wherein the determining of whether the gel is applied on the deactivated probe comprises determining that the gel is applied on the deactivated probe when a value of the first echo signal is higher than a gel detection threshold value.

13. The method of claim 8, further comprising:
deactivating a preactivated probe from among the plurality of probes by electrically disconnecting the preactivated probe from the beam former in the second ultrasonic transceiver.

14. The method of claim 8, further comprising determining a probe from among the plurality of probes as the deactivated probe based on whether the probe is connected to the beam former in the second ultrasonic transceiver.

15. A non-transitory computer-readable recording medium having recorded thereon a program for executing a method of operating an ultrasonic diagnostic apparatus, that when executed by a processor, performs the method comprising:

causing a first ultrasonic transceiver to transmit an ultrasonic signal by applying a first driving signal to a deactivated probe from among a plurality of probes connected to probe ports of the ultrasonic diagnostic apparatus, and receive a first echo signal that is reflected, through the deactivated probe;

determining whether gel is applied on the deactivated probe based on the received first echo signal;

activating the deactivated probe when the gel is applied on the deactivated probe by electrically connecting the deactivated probe to a beam former in a second ultrasonic transceiver of the ultrasonic diagnostic apparatus;
causing the second ultrasonic transceiver to transmit an ultrasonic signal to an object by applying a second driving signal to the activated probe, and receive a second echo signal that is reflected from the object, through the activated probe; and

generating an ultrasonic image representing the object based on the second echo signal.

* * * * *

专利名称(译)	超声诊断设备及其操作方法		
公开(公告)号	US9986977	公开(公告)日	2018-06-05
申请号	US14/493112	申请日	2014-09-22
[标]申请(专利权)人(译)	三星麦迪森株式会社		
申请(专利权)人(译)	三星MEDISON CO. , LTD.		
当前申请(专利权)人(译)	三星MEDISON CO. , LTD.		
[标]发明人	KIM NAM WOONG JIN GIL JU		
发明人	KIM, NAM-WOONG JIN, GIL-JU		
IPC分类号	A61B8/00		
CPC分类号	A61B8/54 A61B8/4281 A61B8/4477 A61B8/585 A61B8/4405 A61B8/4444		
代理机构(译)	MCDERMOTT WILL & EMERY LLP		
优先权	1020140031820 2014-03-18 KR		
其他公开文献	US20150265253A1		
外部链接	Espacenet USPTO		

摘要(译)

提供了一种超声波诊断设备及其操作方法。所述超声波诊断装置包括：第一超声波收发器，其发送超声波信号并通过多个探头中的去激活探头接收反射的第一回波信号；凝胶检测器，其基于所接收的第一回波信号来确定凝胶是否被施加在去激活的探针上；以及控制器，当确定凝胶施加在去激活探针上时激活去激活探针。

