



US 20120232393A1

(19) **United States**(12) **Patent Application Publication**
LEE et al.(10) **Pub. No.: US 2012/0232393 A1**(43) **Pub. Date: Sep. 13, 2012**(54) **ULTRASOUND SYSTEM AND SIGNAL
PROCESSING UNIT CONFIGURED FOR
TIME GAIN AND LATERAL GAIN
COMPENSATION**(30) **Foreign Application Priority Data**

Dec. 7, 2006 (KR) 10-2006-123752

Publication Classification(75) Inventors: **Doo Sik LEE**, Seoul (KR); **Mi
Jeoung AHN**, Seoul (KR)(51) **Int. Cl.**
A61B 8/14 (2006.01)(52) **U.S. Cl.** **600/443**(73) Assignee: **Samsung Medison Co., Ltd.**,
Kangwon-do (KR)(57) **ABSTRACT**(21) Appl. No.: **13/475,686**(22) Filed: **May 18, 2012****Related U.S. Application Data**(63) Continuation of application No. 13/184,094, filed on
Jul. 15, 2011, which is a continuation of application
No. 11/857,860, filed on Sep. 19, 2007, now Pat. No.
8,016,759.

The present invention provides an ultrasound system, which comprises: a signal acquiring unit to transmit an ultrasound signal to an object and acquire an echo signal reflected from the object; a signal processing unit to control TGC (Time Gain Compensation) and LGC (Lateral Gain Compensation) of the echo signal; a TGC/LGC setup unit adapted to set TGC and LGC values based on TGC and LGC curves inputted by a user; and an image producing unit adapted to produce an ultrasound image of the object based on the echo signal. The signal processing unit is further adapted to control the TGC and the LGC of the echo signal based on the TGC and LGC values set by the TGC/LGC setup unit.

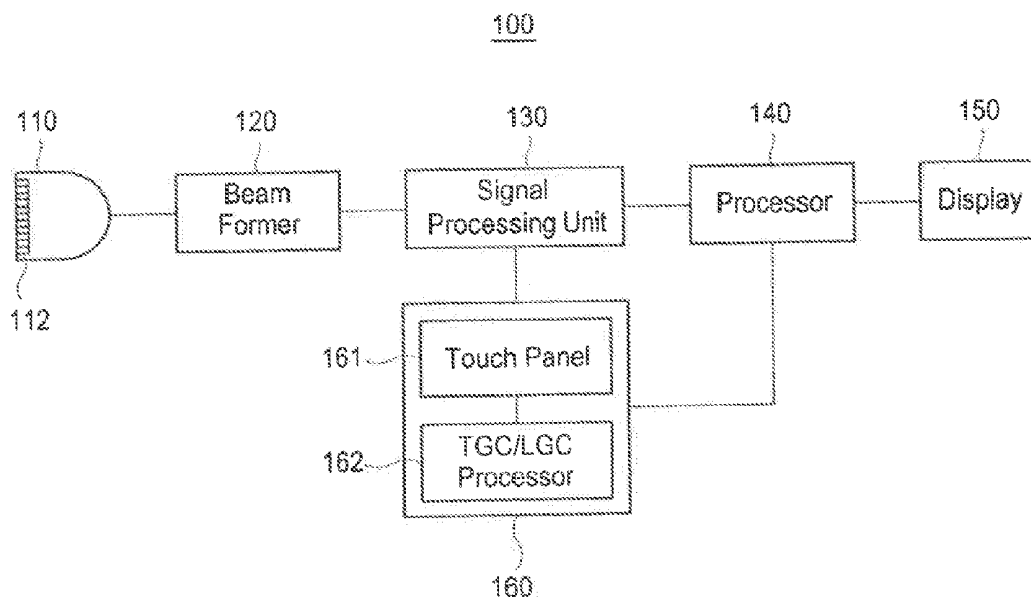


FIG. 1

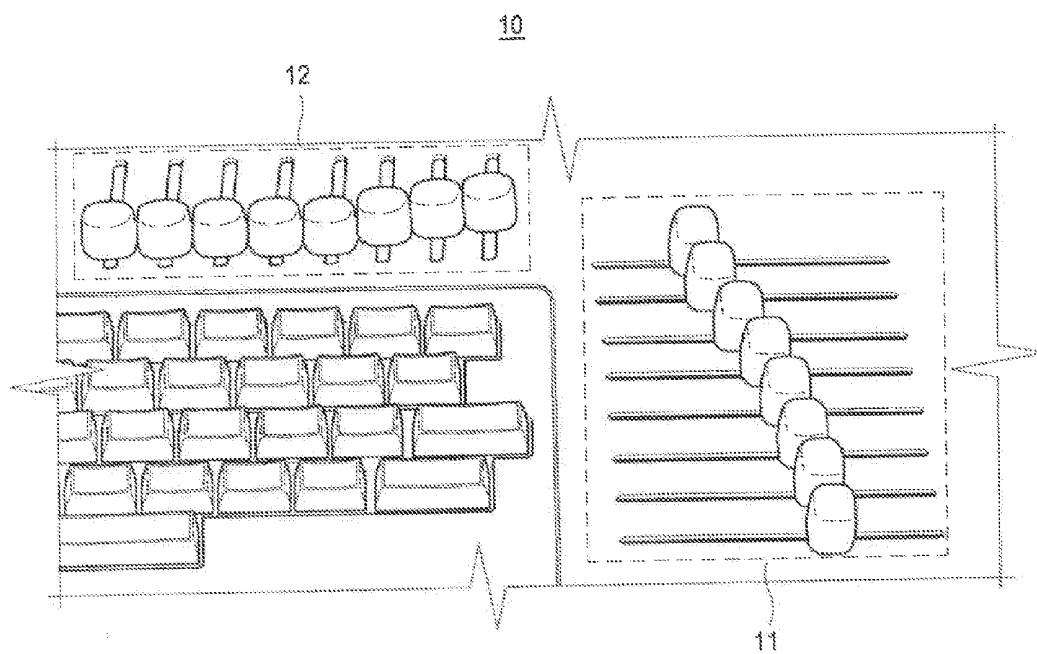


FIG. 2

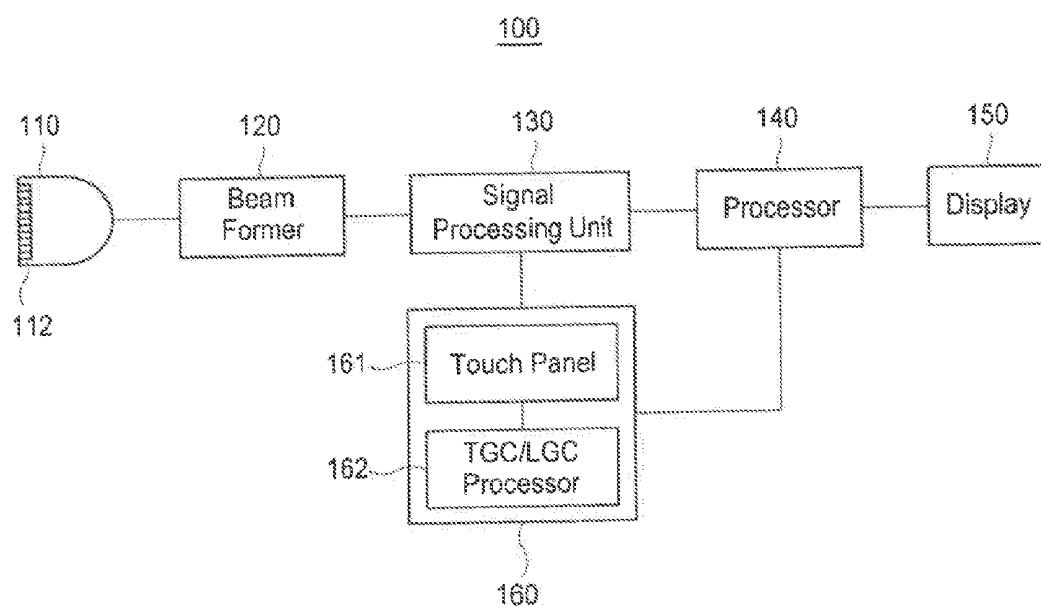


FIG. 3

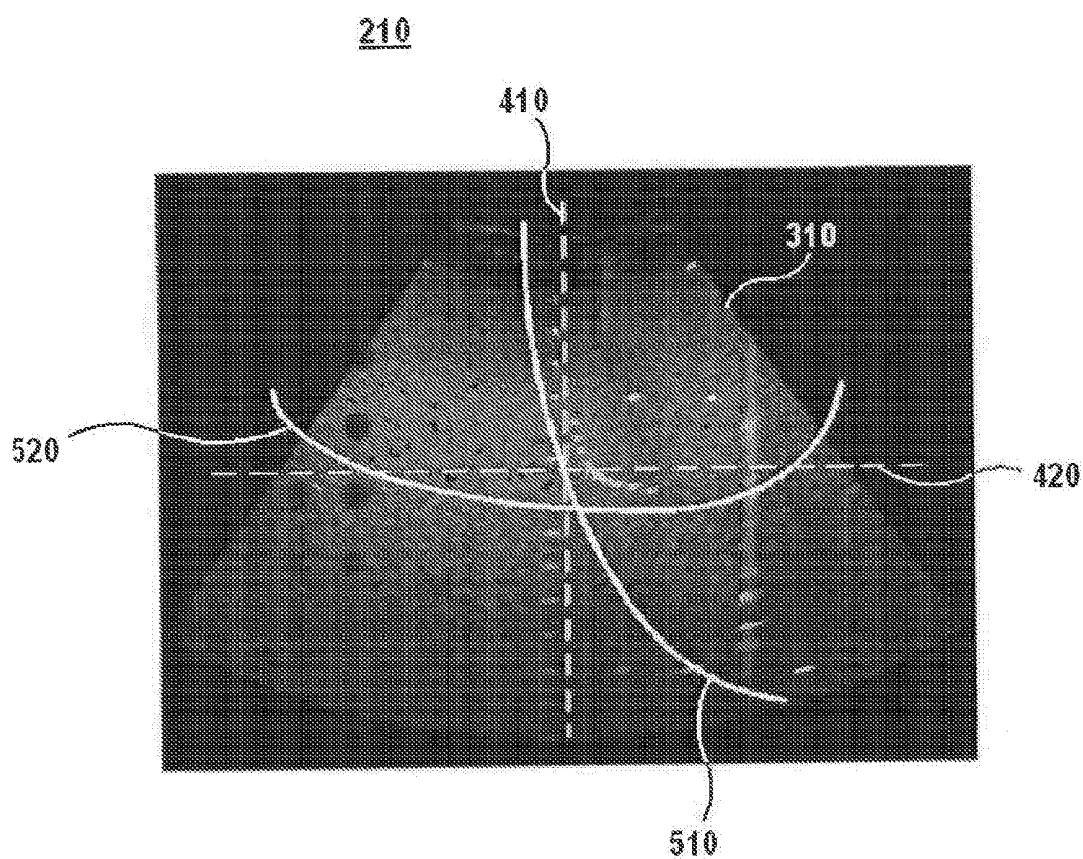


FIG. 4

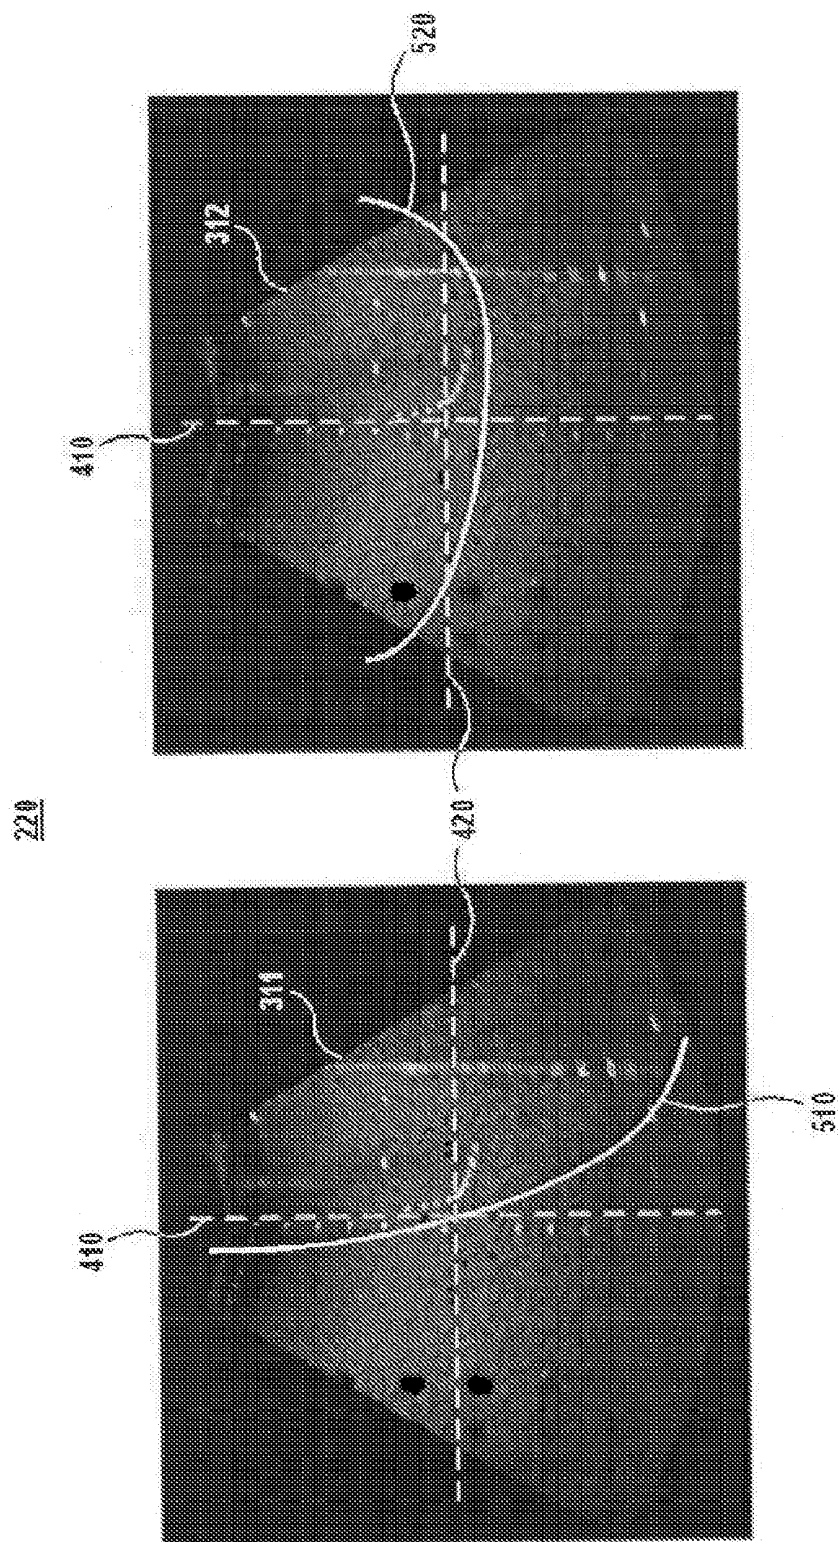


FIG. 5

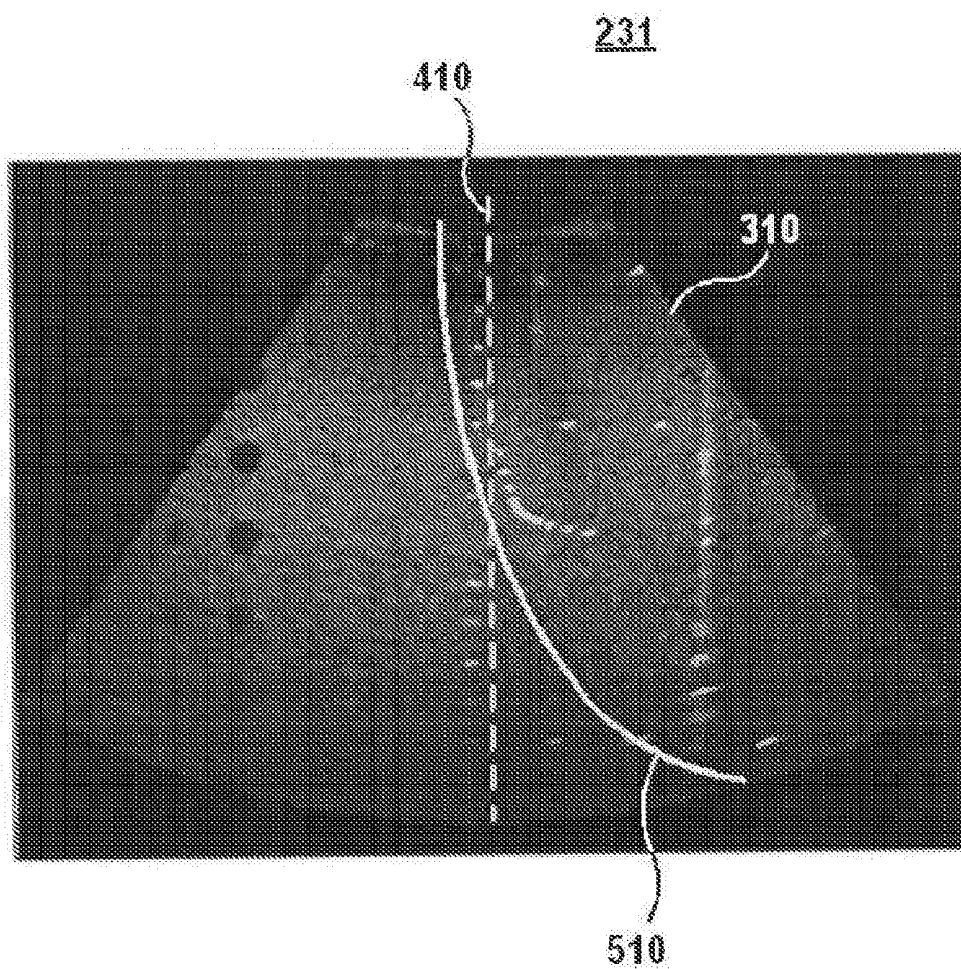


FIG. 6

232

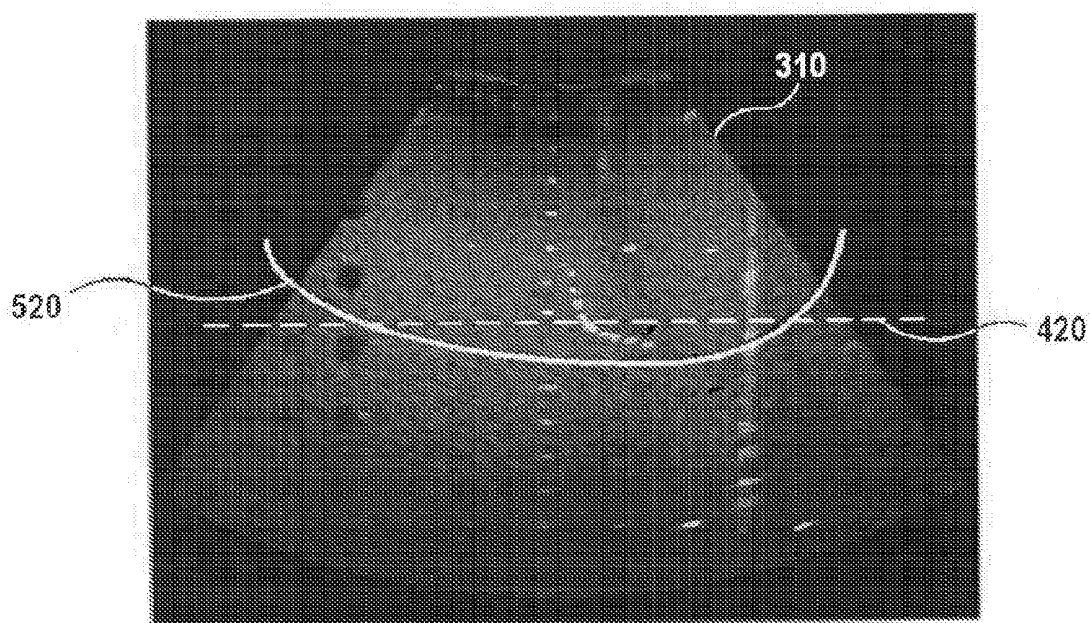


FIG. 7


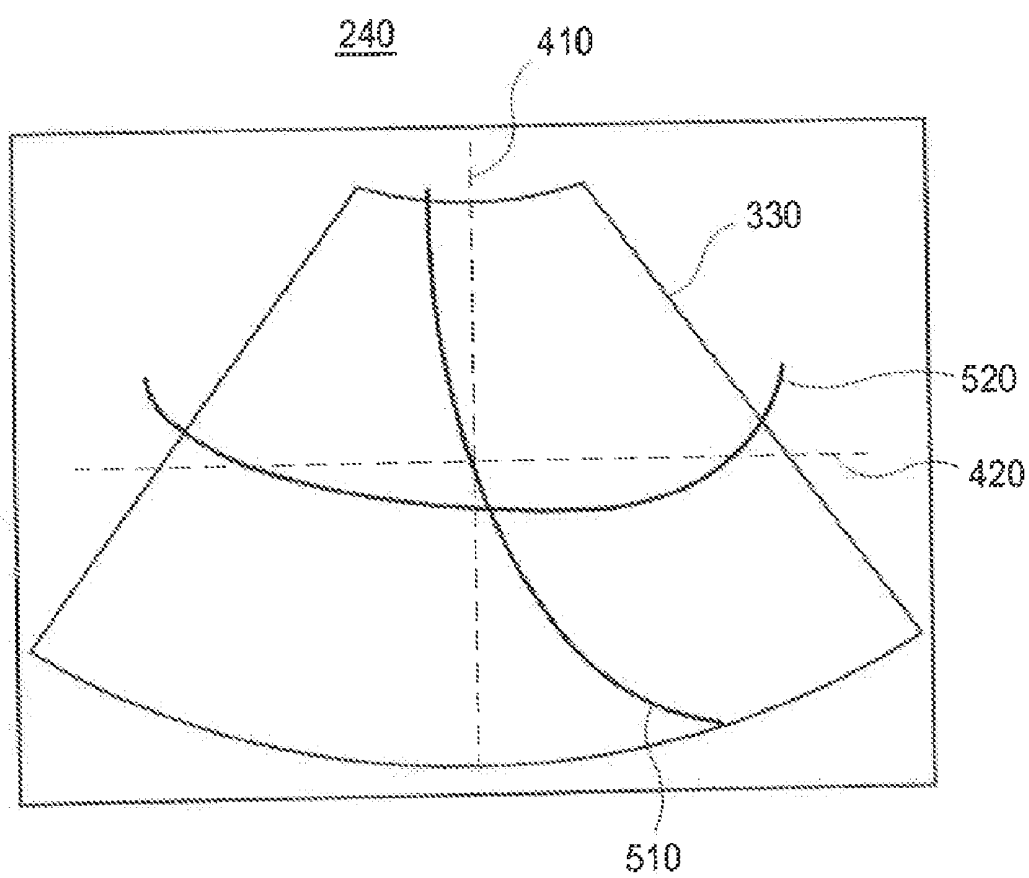


FIG. 8

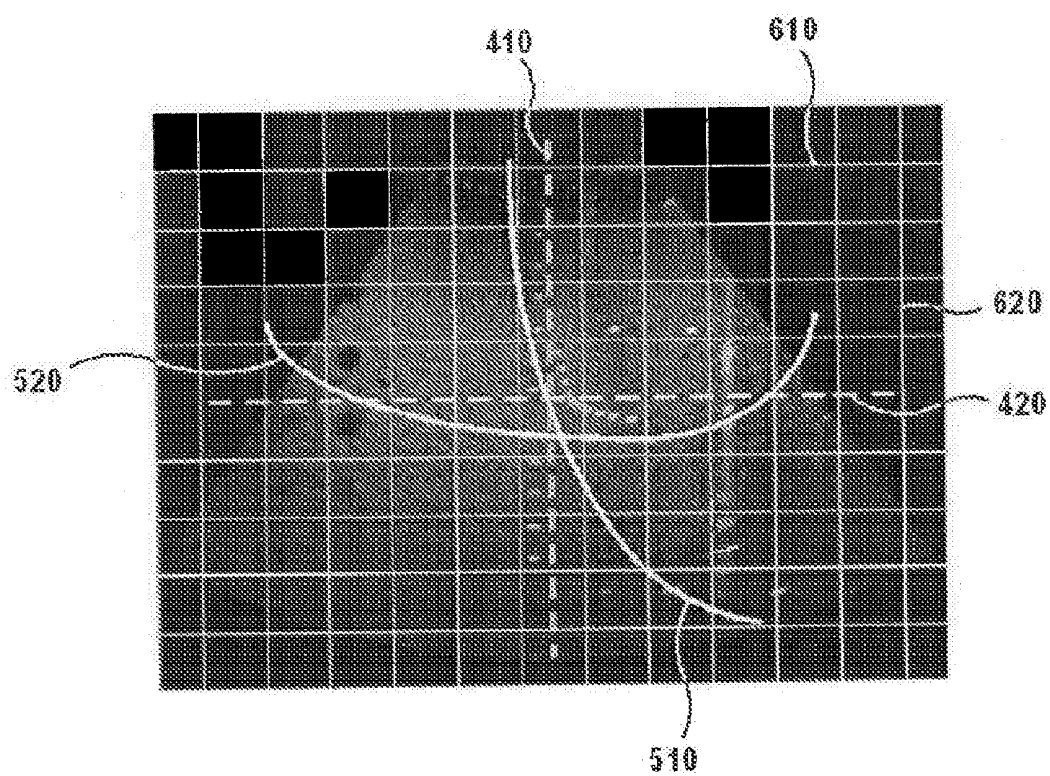

ULTRASOUND SYSTEM AND SIGNAL PROCESSING UNIT CONFIGURED FOR TIME GAIN AND LATERAL GAIN COMPENSATION

[0001] The present application claims priority from Korean Patent Application No. 10-2006-0123752 filed on Dec. 7, 2006, the entire subject matter of which is incorporated herein by reference.

BACKGROUND

[0002] 1. Field

[0003] The present invention generally relates to an ultrasound system, and more particularly to an ultrasound system adapted to precisely and easily perform TGC (Time Gain Compensation) and LGC (Lateral Gain Compensation).

[0004] 2. Background

[0005] An ultrasound system has become an important and popular diagnostic tool since it has a wide range of applications. Specifically, due to its non-invasive and non-destructive nature, the ultrasound system has been extensively used in the medical profession. Modern high-performance ultrasound systems and techniques are commonly used to produce two or three-dimensional diagnostic images of internal features of an object.

[0006] In order to transmit and receive ultrasound signals, the ultrasound system is generally provided with a probe including a wideband transducer. When the transducer is electrically stimulated, it produces ultrasound signals and transmits them into a human body. The ultrasound signals transmitted into the human body are reflected from borders between human tissues and then returned to the transducer. The returned ultrasound echo signals are converted into electric signals. Thereafter, ultrasound image data for imaging the tissues is produced by amplifying and signal-processing the echo signals.

[0007] Typically, the ultrasound system is provided with a control panel including a plurality of input units in order to perform a control function of acquiring the ultrasound image, a menu control function, a measurement and annotation function, etc. The control panel is comprised of a touch panel, an image control unit, a measurement control unit, etc. The touch panel displays menus for optimizing an ultrasound image displayed on a display unit. The menus on the touch panel can be touched and selected by a user. The image control unit controls the ultrasound image, whereas the measurement control unit measures a distance to the object, a circumference of the object, etc. As illustrated in FIG. 1, the image control unit includes a plurality of TGC control keys **11** and a plurality of LGC control keys **12**. The TGC control keys **11** are used to control a gain of each echo signal based on depth of the position from which the echo signal is reflected. Further, since the echo signal is attenuated at the outer right and left sides, the LGC control keys **12** are used to control a gain of the attenuated echo signal.

[0008] In the conventional system, the TGC control keys **11** and the LGC control keys **12** are arranged on different areas of the control panel. The problem associated with such an arrangement is that the size of the control panel must be inevitably increased. Further, a user of the system suffers a great inconvenience when operating the TGC control keys **11** and the LGC control keys **12**. Another problem of the conventional system is that since the TGC control keys **11** and

LGC control keys **12** are comprised of slide-type variable resistors, it is very difficult for an unskilled user to finely control TGC and LGC with the TGC control keys **11** and the LGC control keys **12**.

[0009] In order to resolve the above problems, the present invention is directed to providing an ultrasound system adapted to display a setup screen used to input TGC and LGC curves on a touch panel and perform TGC and LGC based on the inputted TGC and LGC curves.

[0010] The present invention provides an ultrasound system, which comprises: a signal acquiring unit adapted to transmit an ultrasound signal to an object and acquire an echo signal reflected from the object; a signal processing unit adapted to perform TGC (Time Gain Compensation) and LGC (Lateral Gain Compensation) upon the echo signal at a coarse compensation mode based on predetermined TGC and LGC values; an image producing unit adapted to produce an ultrasound image of the object based on the TGC and LGC compensated echo signal; an input unit adapted to allow a user to provide TGC and LGC curves; and a TGC/LGC setup processor adapted to set TGC and LGC values based on the TGC and LGC curves provided by the user. The signal processing unit is further adapted to perform the TGC and LGC upon the echo signal at a fine compensation mode based on the TGC and LGC values set by the TGC/LGC setup processor.

[0011] In addition, the present invention provides an ultrasound system, which comprises: a processor adapted to configure a setup screen for display; and a touch panel adapted to display the setup screen so as to allow a user to input TGC and LGC curves. The processor is further adapted to calculate the TGC and LGC values based on the inputted TGC and the LGC curves.

BRIEF DESCRIPTION OF THE DRAWINGS

[0012] Arrangements and embodiments may be described in detail with reference to the following drawings in which like reference numerals refer to like elements and wherein:

[0013] FIG. 1 is a schematic diagram illustrating conventional TGC and LGC control keys;

[0014] FIG. 2 is a block diagram showing a structure of an ultrasound system according to one embodiment of the present invention;

[0015] FIGS. 3 to 7 illustrate a setup screen according to one embodiment of the present; and

[0016] FIG. 8 illustrates an exemplary distinction between TGC and LGC curves according to one embodiment of the present invention.

DETAILED DESCRIPTION OF THE PRESENT INVENTION

[0017] A detailed description may be provided with reference to the accompanying drawings. One of ordinary skill in the art may realize that the following description is illustrative only and is not in any way limiting. Other embodiments of the present invention may readily suggest themselves to such skilled persons having the benefit of this disclosure.

[0018] Certain embodiments of the present invention will be explained below with reference to FIGS. 2 to 8.

[0019] As illustrated in FIG. 2, an ultrasound system **100** comprises: a probe **110**; a beam former **120**; a signal processing unit **130**; a processor **140**; a display unit **150**; and a TGC/LGC setup unit **160**. The probe **110** includes a plurality

of transducers **112**. Each of the transducers **112** may be configured to transmit an ultrasound signal to an object and receive the ultrasound signal reflected from the object. The beam former **120** may be configured to focus the transmitted ultrasound signals from the transducers **112** on the object and collect the reflected ultrasound signals from the object to the transducers **112** together with corresponding time delay.

[0020] The signal processing unit **130** may be configured to amplify the signals collected by the beam former **120** and control gains of the amplified echo signals. Specifically, the signal processing unit **130** may be configured to perform TGC (Time Gain Compensation) and LGC (Lateral Gain Compensation) upon the echo signals based on predetermined TGC and LGC values at a coarse compensation mode (e.g., in an initial operation stage). The signal processing unit **130** may be further configured to perform TGC and LGC upon the echo signals based on TGC and LGC values calculated in a TGC/LGC setup unit **160** using a curve inputted by a user at a fine compensation mode (e.g., during operations).

[0021] The processor **140** may be configured to receive the echo signals from the signal processing unit **130** and produce an ultrasound image signal based on the echo signals. The display unit **150** may be adapted to receive the ultrasound image signal from the processor and display an ultrasound image based on the signal.

[0022] The TGC/LGC setup unit **160** may include a touch panel **161** and a TGC/LGC setup processor **162**.

[0023] The touch panel **161** may be configured to display a setup screen and detect TGC/LGC curves inputted by the user on the touch panel **161** to produce a detecting signal. The touch panel **161** detects the user's input according to either the pressure sensing method or the electromagnetic induction method. The touch panel **161** may be a touch panel included in a control panel (not shown) of the ultrasound system **100**. Alternatively, it may be separate and apart from the ultrasound system **100**.

[0024] In one embodiment of the present invention, the touch panel **161** may be configured to display a setup screen **210** (shown in FIG. 3) including an ultrasound image **310** and first and second reference lines **410**, **420**. The ultrasound image **310** is based on the echo signal, the TGC and LGC of which are controlled based on the predetermined TGC and LGC values. The first and second reference lines **410**, **420** may be used to detect a TGC curve **510** and a LGC curve **520** inputted by the user (i.e., to determine whether a curve inputted by the user is a TGC curve **510** or a LGC curve **520**). After inputting a curve, the user can modify a portion of the curve.

[0025] In another embodiment of the present invention, the touch panel **161** may be configured to display a setup screen **220** (shown in FIG. 4) including first and second ultrasound images **311**, **312** and first and second reference lines **410**, **420**. The first and second ultrasound images **311**, **312** are based on the echo signal, the TGC and LGC of which are controlled based on the predetermined TGC and LGC values. The first and second reference lines **410**, **420** may be used to detect whether a curve inputted by the user is a TGC curve **510** or a LGC curve **520**. The first ultrasound image **311** may be identical to the second initial ultrasound image **312**.

[0026] In yet another embodiment of the present invention, the touch panel **161** may be configured to display a first setup screen **231** (shown in FIG. 5) including an ultrasound image **310** and a first reference line **410**. The ultrasound image **310** is based on the echo signal, the TGC and LGC of which are controlled based on the predetermined TGC and LGC values.

The first reference line **410** may be used to detect a TGC curve **510** inputted by the user. The touch panel may then display a second setup screen **232** (shown in FIG. 6) including the ultrasound image **310** and a second reference line **420**. The second reference lines **420** may be used to detect a LGC curve **520** inputted by the user. Alternatively, the touch panel **161** may be configured to display the second setup screen **232** before the first setup screen **231**.

[0027] In still yet another embodiment of the present invention, the touch panel **161** may be configured to display a setup screen **240** (shown in FIG. 7) including a virtual ultrasound image **330** and first and second reference lines **410**, **420**.

[0028] The TGC/LGC setup processor **162** may be configured to detect TGC and LGC curves **510**, **520** inputted by the user on the touch panel **161**. The TGC/LGC setup processor **162** may then calculate new TGC and LGC values in consideration of the detected TGC and LGC curves and transmit the values to the signal processing unit **130**.

[0029] In one embodiment of the present invention, as illustrated in FIG. 8, the TGC/LGC setup processor **162** may be configured to establish a first group of lines **610** and a second group of lines **620**. The first group of lines **610** is perpendicular to a first reference line **410** and the lines in said group are equally spaced apart from each other. The second group of lines **620** is perpendicular to a second reference line **420** and the lines in this group are equally spaced apart from each other. If it is determined that a curve inputted by the user (such as the curve **510**) intersects the first group of lines more often than the second group of lines, then the TGC/LGC setup processor **162** recognizes that the curve is a TGC curve. Alternatively, if it is determined that a curve inputted by the user (such as the curve **520**) intersects the second group of lines more often than the first group of lines, then the TGC/LGC setup processor **162** recognizes that the curve is a LGC curve. The TGC/LGC setup processor **162** then calculates the new TGC value corresponding to the TGC curve **510** based on the first reference line **410**. It also calculates the LGC value corresponding to the LGC curve **520** based on the second reference line **420**. The TGC value and the LGC value are transmitted to the signal processing unit **130**.

[0030] The present invention allows the user to accurately control the TGC and LGC by using the TGC and LGC curves inputted into the touch panel, thereby improving operational accuracy and time. Further, the present invention reduces the size of the control panel to thereby improve the spatial efficiency.

[0031] Although the present invention has been described with reference to a number of preferred embodiments thereof, it should be understood that numerous other modifications and embodiments can be devised by those skilled in the art that will fall within the spirit and scope of the principles of this disclosure. More particularly, numerous variations and modifications are possible in the component parts and/or arrangements of the subject combination arrangement within the scope of the disclosure, the drawings and the appended claims. In addition to variations and modifications in the component parts and/or arrangements, alternative uses will also be apparent to those skilled in the art.

1-13. (canceled)

14. An ultrasound system, comprising:

a signal acquiring unit configured for transmitting an ultrasound signal to an object and acquiring an echo signal reflected from the object;

a touch panel configured for receiving a compensation line inputted by a user's touch on the touch panel;
 a processing unit configured for determining a compensation value based on the received compensation line, performing a compensation on the echo signal based on the determined compensation value and generating an ultrasound image of the object based on the compensated echo signal.

15. The ultrasound system of claim **14**, wherein the touch panel is included in a control panel to control operations of the ultrasound system.

16. The ultrasound system of claim **15**, further comprising a display configured for displaying the ultrasound image of the object, the display being detached from the control panel.

17. The ultrasound system of claim **16**, wherein the display is configured to receive a compensation line inputted by a user's touch on the ultrasound image.

18. The ultrasound system of claim **15**, wherein the control panel includes a touch panel display to display an ultrasound image of the object.

19. The ultrasound system of claim **18**, wherein the touch panel display is configured to receive a compensation line inputted by a user's touch on the ultrasound image.

20. The ultrasound system of claim **15**, wherein the touch panel displays the ultrasound image of the object thereon and the compensation line inputted by the user's input on the ultrasound image.

21. The ultrasound system of claim **16**, wherein the received compensation line is not displayed on both the touch panel and the display, and the display displays the ultrasound image after the compensation.

22. The ultrasound system of claim **16**, wherein the received compensation line is displayed on the display.

23. The ultrasound system of claim **14**, wherein the received compensation line is displayed on the touch panel.

24. The ultrasound system of claim **14**, wherein the compensation line is a Time Gain Compensation (TGC) line or a Lateral Gain Compensation (LGC) line.

25. The ultrasound system of claim **24**, wherein the compensation is a TGC or a LGC depending upon whether the received compensation line is the TGC line or the LGC line.

26. The ultrasound system of claim **25**, wherein the processing unit is further configured to perform a second TGC or LGC on the echo signal at a coarse compensation mode based on a predetermined TGC or LGC value before the first compensation.

27. The ultrasound system of claim **24**, wherein the processing unit causes the touch panel to display a first reference line and a second reference line, which are perpendicular to each other, on the ultrasound image used to determine whether the compensation line is a TGC line or a LGC line.

28. The ultrasound system of claim **27**, wherein the processing unit causes the touch panel to further display a first group of lines perpendicular to the first reference line, each of which is spaced apart from adjacent lines at a first uniform distance, and a second group of lines perpendicular to the second reference line, each of which is spaced apart from adjacent lines at a second uniform distance.

29. The ultrasound system of claim **28**, wherein the processing unit determines that the received compensation line is a TGC line when the received compensation line intersects the first group of lines more than the second group of lines, and the processing unit determines that the received compen-

sation line is a LGC line when the received compensation line intersect the second group of lines more than the second group of lines more than the first group of lines.

30. The ultrasound system of claim **29**, wherein the processing unit calculates a new TGC value based on the received compensation line and the first reference line if the received compensation line is the TGC, and the processing unit calculates a new LGC value based on the received compensation line and the second reference line, if the received compensation line is the LGC line.

31. The ultrasound system of claim **30**, wherein the processing unit compensates the echo signal based on the new TGC value or the new LGC value.

32. An ultrasound system, comprising:

a signal acquiring unit configured for transmitting an ultrasound signal to an object and acquiring an echo signal reflected from the object;

a display configured for displaying an ultrasound image of the object, the display including a touch panel configured for receiving a compensation line inputted by a user's touch on the touch panel;

a processing unit configured for determining a compensation value based on the received compensation line, performing a compensation on the echo signal based on the determined compensation value and generating the ultrasound image of the object based on the compensated echo signal.

33. The ultrasound system of claim **32**, wherein the received compensation line is not displayed on the touch panel and the area where the ultrasound image is displayed on the display, and the display displays the ultrasound image after the compensation.

34. The ultrasound system of claim **32**, wherein the received compensation line is displayed on the touch panel.

35. The ultrasound system of claim **32**, wherein the received compensation line is displayed on the area where the ultrasound image is displayed.

36. The ultrasound system of claim **32**, wherein the compensation line is a Time Gain Compensation (TGC) line or a Lateral Gain Compensation (LGC) line.

37. The ultrasound system of claim **36**, wherein the compensation is a TGC or a LGC depending upon whether the received compensation line is the TGC line or the LGC line.

38. The ultrasound system of claim **37**, wherein the processing unit is further configured to perform a second TGC or LGC on the echo signal at a coarse compensation mode based on a predetermined TGC or LGC value before the first compensation.

39. The ultrasound system of claim **36**, wherein the processing unit causes the touch panel to display a first reference line and a second reference line, which are perpendicular to each other, on the ultrasound image used to determine whether the compensation line is a TGC line or a LGC line.

40. The ultrasound system of claim **39**, wherein the processing unit causes the touch panel to further display a first group of lines perpendicular to the first reference line, each of which is spaced apart from adjacent lines at a first uniform distance, and a second group of lines perpendicular to the second reference line, each of which is spaced apart from adjacent lines at a second uniform distance.

41. The ultrasound system of claim **40**, wherein the processing unit determines that the received compensation line is a TGC line when the received compensation line intersects the first group of lines more than the second group of lines,

and the processing unit determines that the received compensation line is a LGC line when the received compensation line intersect the second group of lines more than the second group of lines more than the first group of lines.

42. The ultrasound system of claim **41**, wherein the processing unit calculates a new TGC value based on the received compensation line and the first reference line if the received compensation line is the TGC, and the processing unit calculates a new LGC value based on the received compensation line and the second reference line, if the received compensation line is the LGC line.

43. The ultrasound system of claim **42**, wherein the processing unit compensates the echo signal based on the new TGC value or the new LGC value.

44. The ultrasound system of claim **32**, wherein the touch panel is separately located, on the display, from an area where the ultrasound image is displayed.

45. An ultrasound system, comprising:

a probe configured for transmitting an ultrasound signal to an object and receiving the ultrasound signal reflected from the object; and

a portable computer connected to the probe,

wherein the portable computer includes:

a signal acquiring unit configured for transmitting an ultrasound signal to an object and acquiring an echo signal reflected from the object;

a touch screen configured for receiving a user's touch input and displaying an ultrasound image of the object, the touch screen receiving a compensation line by a user's touch;

a processing unit configured for determining a compensation value based on the received compensation line, performing a compensation on the echo signal based on the determined compensation value and generating the ultrasound image of the object based on the compensated echo signal.

46. The ultrasound system of claim **45**, wherein the received compensation line is not displayed on the touch screen, and the touch screen displays the ultrasound image after the compensation.

47. The ultrasound system of claim **45**, wherein the received compensation line is displayed on the touch screen.

48. The ultrasound system of claim **45**, wherein the compensation line is a Time Gain Compensation (TGC) line or a Lateral Gain Compensation (LGC) line.

49. The ultrasound system of claim **48**, wherein the compensation is a TGC or a LGC depending upon whether the received compensation line is the TGC line or the LGC line.

50. The ultrasound system of claim **49**, wherein the processing unit is further configured to perform a second TGC or LGC on the echo signal at a coarse compensation mode based on a predetermined TGC or LGC value before the first compensation.

51. The ultrasound system of claim **48**, wherein the processing unit causes the touch screen to display a first reference line and a second reference line, which are perpendicular to each other, on the ultrasound image used to determine whether the compensation line is a TGC line or a LGC line.

52. The ultrasound system of claim **51**, wherein the processing unit causes the touch screen to further display a first group of lines perpendicular to the first reference line, each of which is spaced apart from adjacent lines at a first uniform distance, and a second group of lines perpendicular to the

second reference line, each of which is spaced apart from adjacent lines at a second uniform distance.

53. The ultrasound system of claim **52**, wherein the processing unit determines that the received compensation line is a TGC line when the received compensation line intersects the first group of lines more than the second group of lines, and the processing unit determines that the received compensation line is a LGC line when the received compensation line intersect the second group of lines more than the second group of lines more than the first group of lines.

54. The ultrasound system of claim **53**, wherein the processing unit calculates a new TGC value based on the received compensation line and the first reference line if the received compensation line is the TGC, and the processing unit calculates a new LGC value based on the received compensation line and the second reference line, if the received compensation line is the LGC line.

55. The ultrasound system of claim **54**, wherein the processing unit compensates the echo signal based on the new TGC value or the new LGC value.

56. The ultrasound system of claim **45**, wherein the portable computer is a tablet computer having a touch-type input interface.

57. The ultrasound system of claim **45**, wherein the portable computer has wireless communication capability.

58. A portable computer connected to a probe, which transmits an ultrasound signal to an object and receives the ultrasound signal reflected from the object, the portable computer comprising:

a signal acquiring unit configured for transmitting an ultrasound signal to an object and acquiring an echo signal reflected from the object;

a touch screen configured for receiving a user's touch input and displaying an ultrasound image of the object, the touch screen receiving a compensation line by a user's touch;

a processing unit configured for determining a compensation value based on the received compensation line, performing a compensation on the echo signal based on the determined compensation value and generating the ultrasound image of the object based on the compensated echo signal.

59. The portable computer of claim **58**, wherein the received compensation line is not displayed on the touch screen, and the touch screen displays the ultrasound image after the compensation.

60. The portable computer of claim **58**, wherein the received compensation line is displayed on the touch screen.

61. The portable computer of claim **58**, wherein the compensation line is a Time Gain Compensation (TGC) line or a Lateral Gain Compensation (LGC) line.

62. The portable computer of claim **61**, wherein the compensation is a TGC or a LGC depending upon whether the received compensation line is the TGC line or the LGC line.

63. The portable computer of claim **62**, wherein the processing unit is further configured to perform a second TGC or LGC on the echo signal at a coarse compensation mode based on a predetermined TGC or LGC value before the first compensation.

64. The portable computer of claim **61**, wherein the processing unit causes the touch screen to display a first reference line and a second reference line, which are perpendicular to each other, on the ultrasound image used to determine whether the compensation line is a TGC line or a LGC line.

65. The portable computer of claim **64**, wherein the processing unit causes the touch screen to further display a first group of lines perpendicular to the first reference line, each of which is spaced apart from adjacent lines at a first uniform distance, and a second group of lines perpendicular to the second reference line, each of which is spaced apart from adjacent lines at a second uniform distance.

66. The portable computer of claim **65**, wherein the processing unit determines that the received compensation line is a TGC line when the received compensation line intersects the first group of lines more than the second group of lines, and the processing unit determines that the received compensation line is a LGC line when the received compensation line intersect the second group of lines more than the second group of lines more than the first group of lines.

67. The portable computer of claim **66**, wherein the processing unit calculates a new TGC value based on the received compensation line and the first reference line if the received compensation line is the TGC, and the processing unit calculates a new LGC value based on the received compensation line and the second reference line, if the received compensation line is the LGC line.

68. The portable computer of claim **67**, wherein the processing unit compensates the echo signal based on the new TGC value or the new LGC value.

69. The portable computer of claim **58**, wherein the portable computer is a tablet computer having a touch-type input interface.

70. The portable computer of claim **58**, wherein the portable computer has wireless communication capability.

* * * * *

专利名称(译)	超声系统和信号处理单元配置用于时间增益和横向增益补偿		
公开(公告)号	US20120232393A1	公开(公告)日	2012-09-13
申请号	US13/475686	申请日	2012-05-18
[标]申请(专利权)人(译)	三星麦迪森株式会社		
申请(专利权)人(译)	三星MEDISON CO. , LTD.		
当前申请(专利权)人(译)	三星MEDISON CO. , LTD.		
[标]发明人	LEE DOO SIK AHN MI JEOUNG		
发明人	LEE, DOO SIK AHN, MI JEOUNG		
IPC分类号	A61B8/14		
CPC分类号	A61B8/00 A61B8/463 A61B8/467 G01S7/52033 G01S7/52084 A61B8/5207 A61B8/4254 A61B8/4444 A61B8/5269 A61B8/54 A61B8/461 A61B8/14 A61B6/467 A61B8/46 A61B8/462 A61B8/465 G06F3/01 G06F3/048 G06F3/0484 G06F3/04845 G06F3/04847 G06T7/0012		
优先权	1020060123752 2006-12-07 KR		
其他公开文献	US9055920		
外部链接	Espacenet USPTO		

摘要(译)

本发明提供一种超声系统，包括：信号获取单元，用于将超声信号发送到物体并获取从物体反射的回波信号；信号处理单元，用于控制回波信号的TGC（时间增益补偿）和LGC（横向增益补偿）；TGC / LGC设置单元，适于根据用户输入的TGC和LGC曲线设置TGC和LGC值；图像产生单元，适于基于回波信号产生对象的超声图像。信号处理单元还适于基于由TGC / LGC设置单元设置的TGC和LGC值来控制回波信号的TGC和LGC。

