



US008088071B2

(12) **United States Patent**
Hwang et al.

(10) **Patent No.:** **US 8,088,071 B2**
(45) **Date of Patent:** ***Jan. 3, 2012**

(54) **MODULAR APPARATUS FOR DIAGNOSTIC
ULTRASOUND**

(75) Inventors: **Juin-Jet Hwang**, Mercer Island, WA
(US); **Blake W. Little**, Bothell, WA (US)

(73) Assignee: **SonoSite, Inc.**, Bothell, WA (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 89 days.

This patent is subject to a terminal dis-
claimer.

5,205,175 A 4/1993 Garza et al.
5,295,485 A 3/1994 Shinomura et al.
5,318,027 A 6/1994 Fukui
5,323,291 A 6/1994 Boyle et al.
5,347,425 A 9/1994 Herron et al.
5,375,604 A 12/1994 Kelly et al.
5,457,784 A 10/1995 Wells et al.

(Continued)

FOREIGN PATENT DOCUMENTS

DE 2003/10224234 1/2003

(Continued)

OTHER PUBLICATIONS

Logiz Book [GE Medical Systems website], [retrieved on Apr. 3,
2003] Retrieved from General Electric Medical Systems website
using Internet<URL:http://www.gemedicalsystems.com/rad/us/prod-
ucts.logizbook/logizbook_intro3.html (total of 3 pages).

(Continued)

(21) Appl. No.: **12/467,899**

(22) Filed: **May 18, 2009**

(65) **Prior Publication Data**

US 2009/0275835 A1 Nov. 5, 2009

Related U.S. Application Data

(62) Division of application No. 10/356,335, filed on Jan.
31, 2003, now Pat. No. 7,534,211.

(60) Provisional application No. 60/369,023, filed on Mar.
29, 2002.

(51) **Int. Cl.**

A61B 8/14 (2006.01)

A61B 8/00 (2006.01)

G06F 13/00 (2006.01)

(52) **U.S. Cl.** **600/459; 600/437; 710/303**

(58) **Field of Classification Search** **600/437,**
600/459; 710/303, 304

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,688,579 A 8/1987 Inahara et al.
4,715,385 A 12/1987 Cudahy et al.
4,895,161 A 1/1990 Cudahy et al.
4,907,118 A 3/1990 Hames

Primary Examiner — Michael Rozanski


(74) *Attorney, Agent, or Firm* — Perkin Coie LLP

(57)

ABSTRACT

A modular diagnostic ultrasound apparatus is provided com-
prising a core unit, system electronics and an I/O port. The
core unit comprises a housing and a system electronics pack-
age within the housing. The system electronics has one or
more concatenated filters, including a front end transmit/
receive circuit, a processor, a back end circuit for scan con-
version, a system clock and a programmable system memory
device. There is at least one I/O port connected to the front end
and the back end of the system electronics package and
extending through the core unit housing wherein all system
data processing information is transmitted or received
through the I/O port.

21 Claims, 8 Drawing Sheets

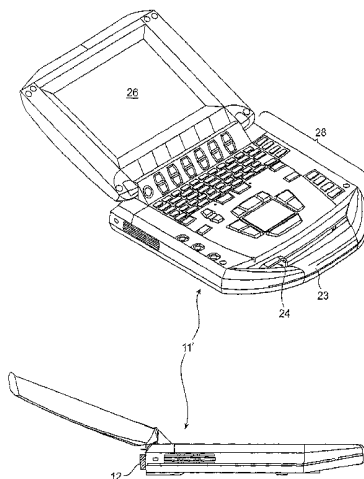

U.S. PATENT DOCUMENTS

5,460,547	A	10/1995	Belt et al.	6,569,102	B2	5/2003	Imran et al.
5,568,359	A	10/1996	Cavello et al.	6,575,908	B2	6/2003	Barnes et al.
5,590,658	A	1/1997	Chiang et al.	6,592,521	B1	7/2003	Urbano et al.
5,603,323	A	2/1997	Pflugrath et al.	6,593,528	B2	7/2003	Franklin-Lees et al.
5,604,663	A	2/1997	Shin et al.	6,595,921	B1	7/2003	Urbano et al.
5,615,678	A	4/1997	Kirkham et al.	6,618,206	B2	9/2003	Tarakci et al.
5,627,974	A	5/1997	Watts et al.	6,629,928	B1	10/2003	Dolan et al.
5,640,953	A	6/1997	Bishop et al.	6,663,567	B2	12/2003	Ji et al.
5,640,960	A	6/1997	Jones et al.	6,669,634	B2	12/2003	Amemiya et al.
5,682,902	A	11/1997	Herleikson	6,685,645	B1	2/2004	McLaughlin et al.
5,685,314	A	11/1997	Geheb et al.	6,716,167	B1	4/2004	Henderson et al.
5,687,387	A	11/1997	Endejan et al.	6,721,178	B1	4/2004	Clark et al.
5,687,717	A	11/1997	Halpern et al.	6,733,455	B2	5/2004	Mo et al.
5,699,243	A *	12/1997	Eckel et al. 700/17	6,745,146	B1	6/2004	Brown et al.
5,715,823	A	2/1998	Wood et al.	6,773,399	B2	8/2004	Xi et al.
5,722,412	A	3/1998	Pflugrath et al.	6,852,081	B2	2/2005	Sumanaweera et al.
5,752,917	A	5/1998	Fuchs	6,866,631	B2	3/2005	McLaughlin et al.
5,757,616	A	5/1998	May et al.	6,866,632	B1	3/2005	Chou et al.
5,758,649	A	6/1998	Iwashita et al.	6,896,658	B2	5/2005	Ji et al.
5,795,297	A	8/1998	Daigle	6,936,008	B2	8/2005	Tarakci et al.
5,839,442	A	11/1998	Chiang et al.	6,969,352	B2	11/2005	Chiang et al.
5,851,186	A	12/1998	Wood et al.	6,980,419	B2	12/2005	Smith et al.
5,872,557	A	2/1999	Wiemer et al.	7,009,840	B2	3/2006	Clark et al.
5,888,087	A	3/1999	Hanson et al.	7,037,264	B2	5/2006	Poland
5,891,035	A	4/1999	Wood et al.	7,037,267	B1	5/2006	Lipson et al.
5,892,299	A	4/1999	Siewert et al.	7,141,020	B2	11/2006	Poland et al.
5,897,498	A	4/1999	Canfield, II et al.	7,188,620	B2	3/2007	Amarasinghe
5,938,607	A	8/1999	Jago et al.	7,534,211	B2 *	5/2009	Hwang et al. 600/459
5,971,923	A	10/1999	Finger	7,591,786	B2 *	9/2009	Holmberg et al. 600/437
5,982,614	A	11/1999	Reid	2001/0055978	A1	12/2001	Herrod et al.
6,031,356	A	2/2000	Harada et al.	2002/0016545	A1	2/2002	Quistgaard et al.
6,063,030	A	5/2000	Vara et al.	2002/0082479	A1	6/2002	Frangesch et al.
6,117,085	A	9/2000	Picatti et al.	2002/0103435	A1	8/2002	Mault
6,132,379	A	10/2000	Patacsil et al.	2002/0143256	A1	10/2002	Wing et al.
6,135,801	A	10/2000	Helot et al.	2002/0173721	A1	11/2002	Grunwald et al.
6,142,940	A	11/2000	Lathbury et al.	2003/0004414	A1	1/2003	McLaughlin et al.
6,171,244	B1	1/2001	Finger et al.	2003/0009102	A1	1/2003	Quistgaard et al.
6,178,474	B1	1/2001	Hamano et al.	2003/0013959	A1	1/2003	Grunwald et al.
6,183,417	B1	2/2001	Geheb et al.	2003/0013965	A1	1/2003	Quistgaard et al.
6,190,326	B1	2/2001	McKinnon et al.	2003/0013966	A1	1/2003	Barnes et al.
6,203,498	B1	3/2001	Bunce et al.	2004/0004460	A1	1/2004	Fitch et al.
6,206,578	B1	3/2001	Shin et al.	2004/0150963	A1	8/2004	Holmberg et al.
6,241,673	B1	6/2001	Williams	2004/0152982	A1	8/2004	Hwang et al.
6,248,073	B1	6/2001	Gilbert et al.	2004/0158154	A1	8/2004	Hanafy et al.
6,251,073	B1	6/2001	Imran et al.	2005/0131294	A1	6/2005	Ji et al.
6,312,381	B1	11/2001	Knell et al.	2006/0013966	A1	1/2006	Koninckx et al.
6,358,204	B1	3/2002	Finger et al.	2006/0098864	A1	5/2006	Ziel
6,364,839	B1	4/2002	Little et al.	2007/0274693	A1	11/2007	Farbarik
6,379,304	B1	4/2002	Gilbert et al.				
6,407,335	B1	6/2002	Franklin-Lees et al.				
6,409,660	B1	6/2002	Sjoqvist et al.				
6,424,120	B1	7/2002	Chen				
D461,814	S	8/2002	Felix et al.				
6,436,039	B1	8/2002	Lannutti et al.				
6,436,040	B1	8/2002	Collamore et al.				
6,440,071	B1	8/2002	Slayton et al.				
6,440,072	B1	8/2002	Schuman et al.				
6,440,076	B1	8/2002	Sudol et al.				
D462,446	S	9/2002	Felix et al.				
6,447,451	B1	9/2002	Wing et al.				
6,468,212	B1	10/2002	Scott et al.				
6,468,213	B1	10/2002	Knell et al.				
6,471,651	B1	10/2002	Hwang et al.				
D467,002	S	12/2002	Felix et al.				
6,488,625	B1	12/2002	Randall et al.				
6,491,630	B1	12/2002	Saccardo et al.				
6,493,220	B1	12/2002	Clark et al.				
6,497,664	B1	12/2002	Randall et al.				
6,500,126	B1	12/2002	Brock-Fisher				
D469,539	S	1/2003	Felix et al.				
6,508,763	B1	1/2003	Urbano et al.				
D469,877	S	2/2003	Felix et al.				
6,517,491	B1	2/2003	Thiele et al.				
6,524,244	B1	2/2003	Knell et al.				
6,542,846	B1	4/2003	Miller et al.				
6,561,979	B1	5/2003	Wood et al.				
6,569,097	B1	5/2003	McMorrow et al.				
6,569,101	B2	5/2003	Quistgaard et al.				

FOREIGN PATENT DOCUMENTS

EP	1 215 510	6/2002
EP	1215510	6/2002
JP	8275926	10/1996
JP	8280635	10/1996
JP	2002-542870	12/2002
WO	WO-94/14128	6/1994
WO	WO 01/13796	3/2001
WO	WO 2004/080364	9/2004

OTHER PUBLICATIONS

International Partial Search Report issued for PCT/US2004/002423, dated Oct. 5, 2004.

Extended Search Report issued for European Application No. 09013813 dated Nov. 26, 2009, 3 pgs.

Chiang et al., "PC-Based Ultrasound Imaging System in a Probe", 2000 IEEE Ultrasonics Symposium, San Juan PR, Oct. 22-25, 2000, IEEE US vol. 2, Oct. 22, 2000, 6 pgs.

Plaintiff and Counterclaim Defendant SonoSite's Preliminary Invalidity Contentions, United States District Court, Case SACV07-222AG (FFMx), dated Sep. 11, 2007, pp. 1-4, including Exhibits B-M, pp. 1-368.

English-Translated Chinese Office Action issued for Chinese Patent Application 200480006334.4; Dated Jan. 4, 2008; 11 pages.

International Search Report Issued for PCT/US2004/002671, dated Jul. 5, 2004.

* cited by examiner

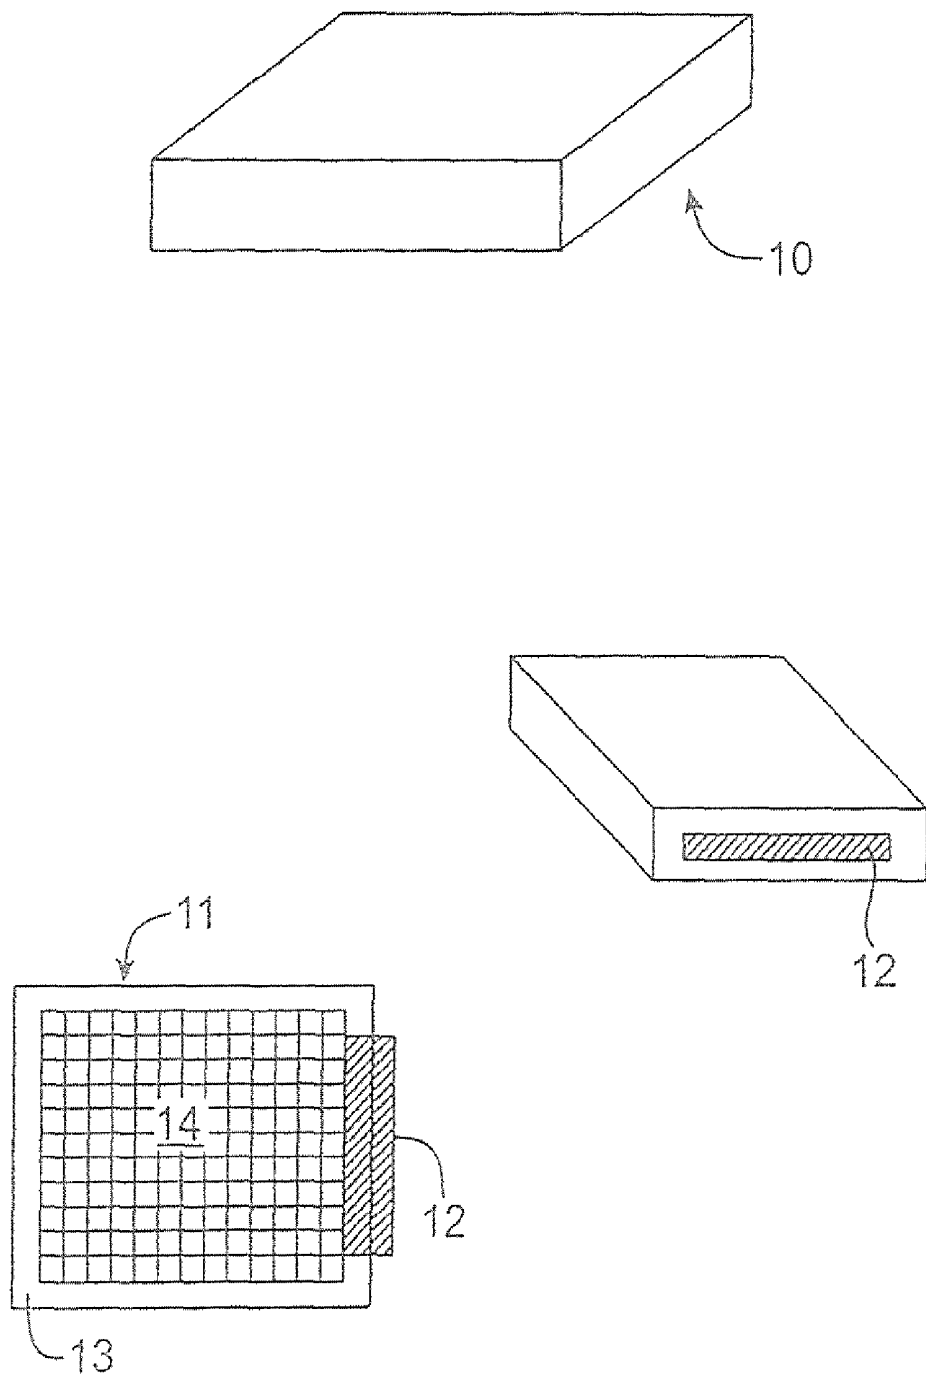


FIG. 1A

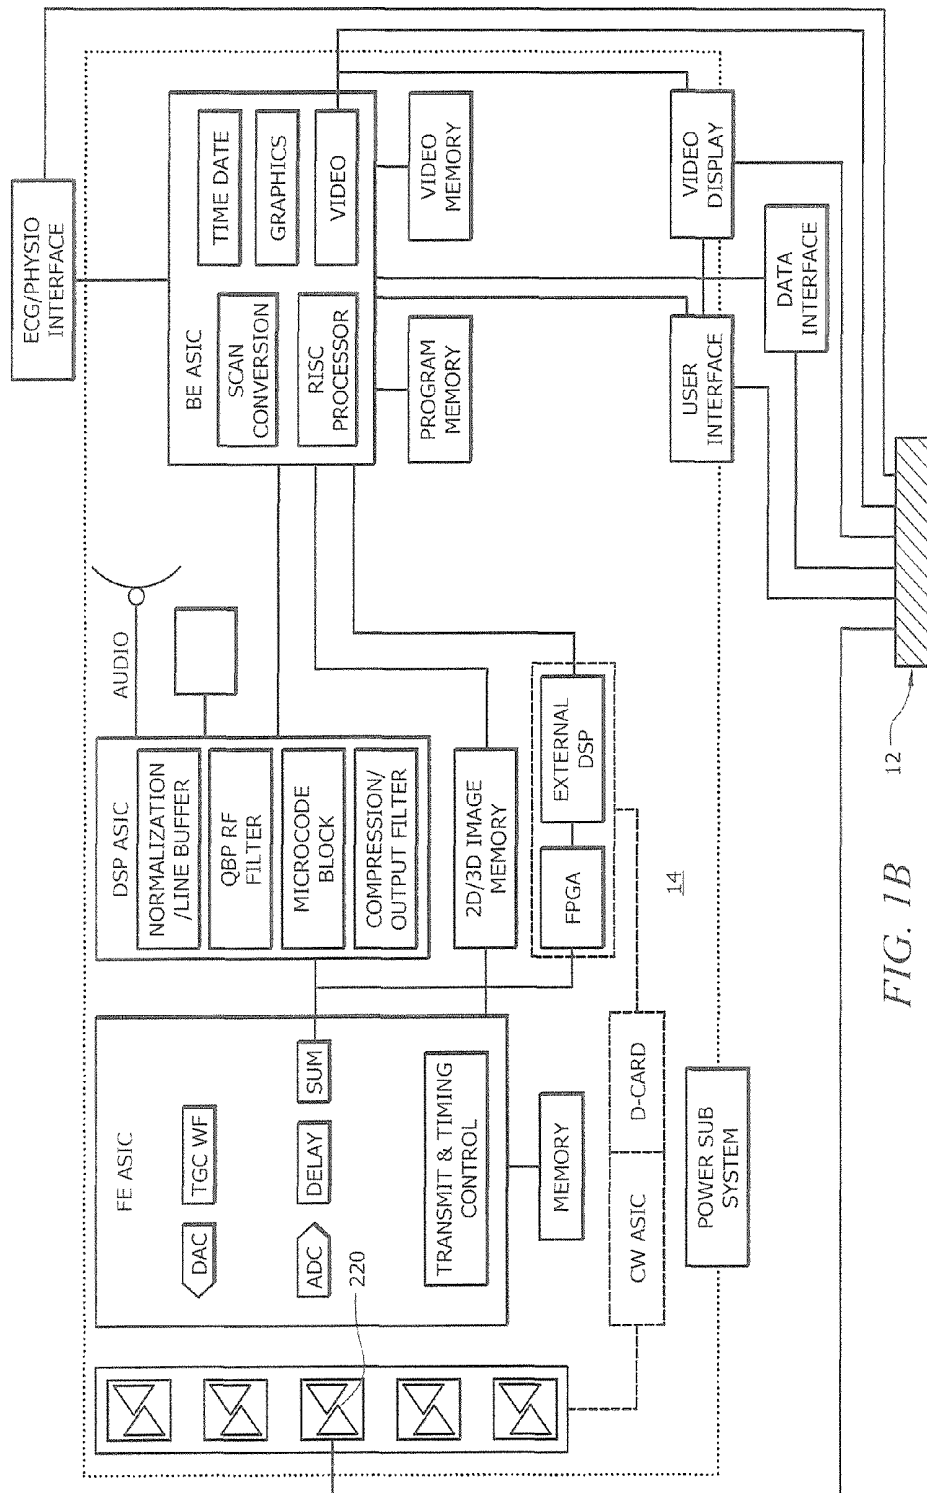


FIG. 1B

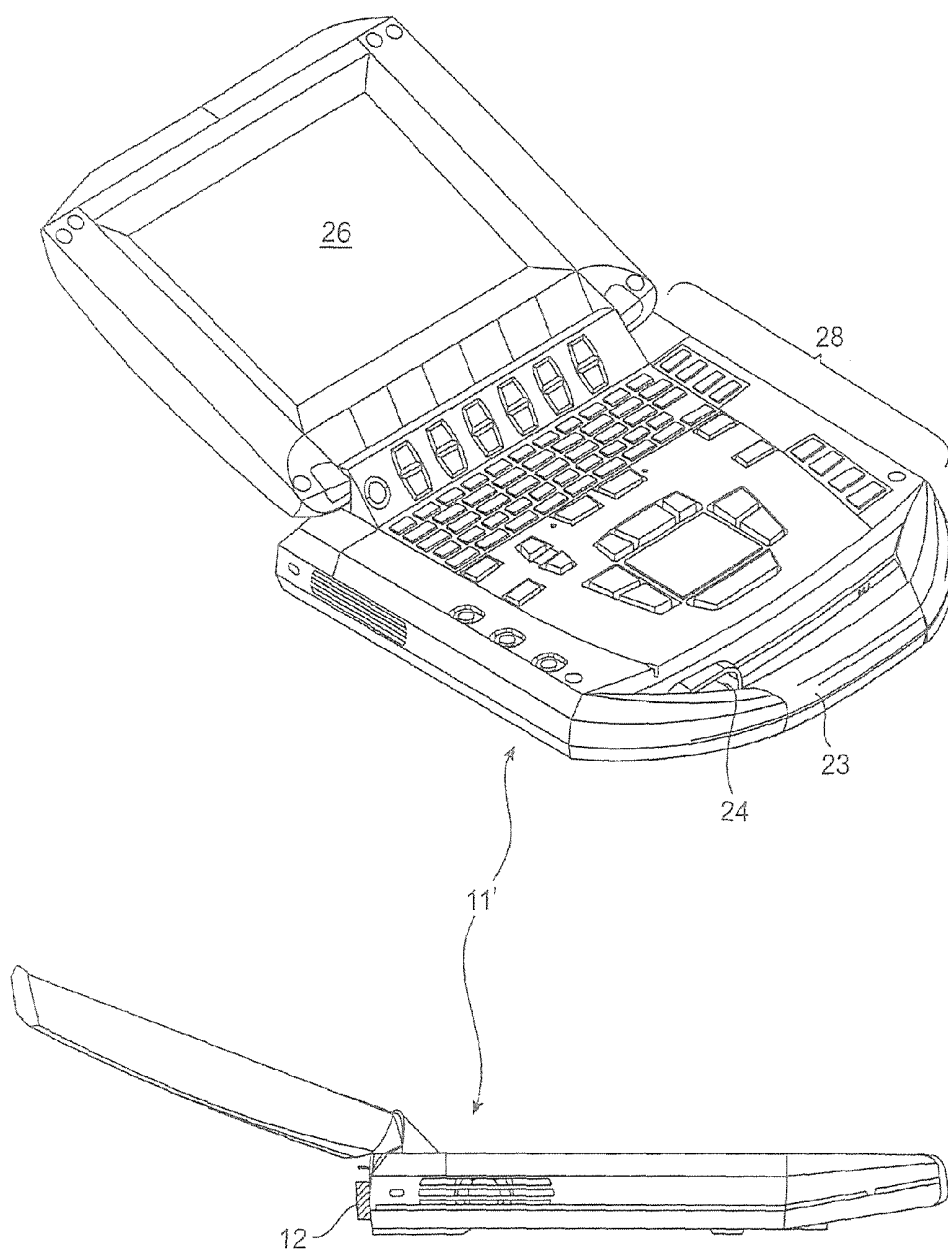


FIG. 1C

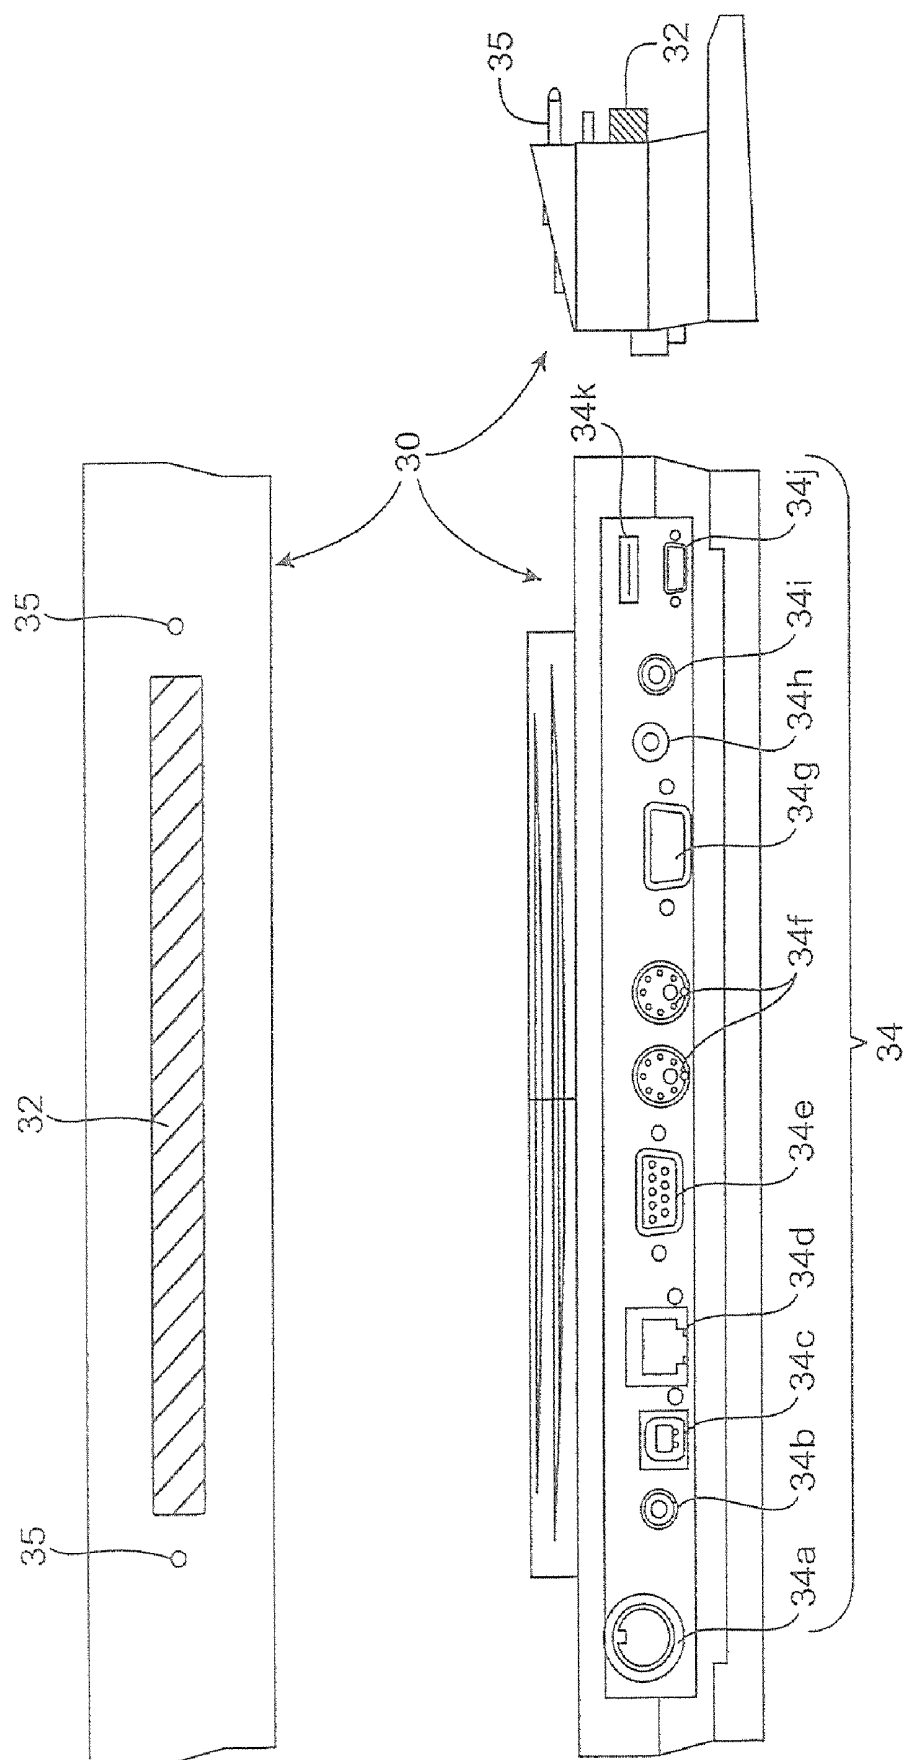


FIG. 2

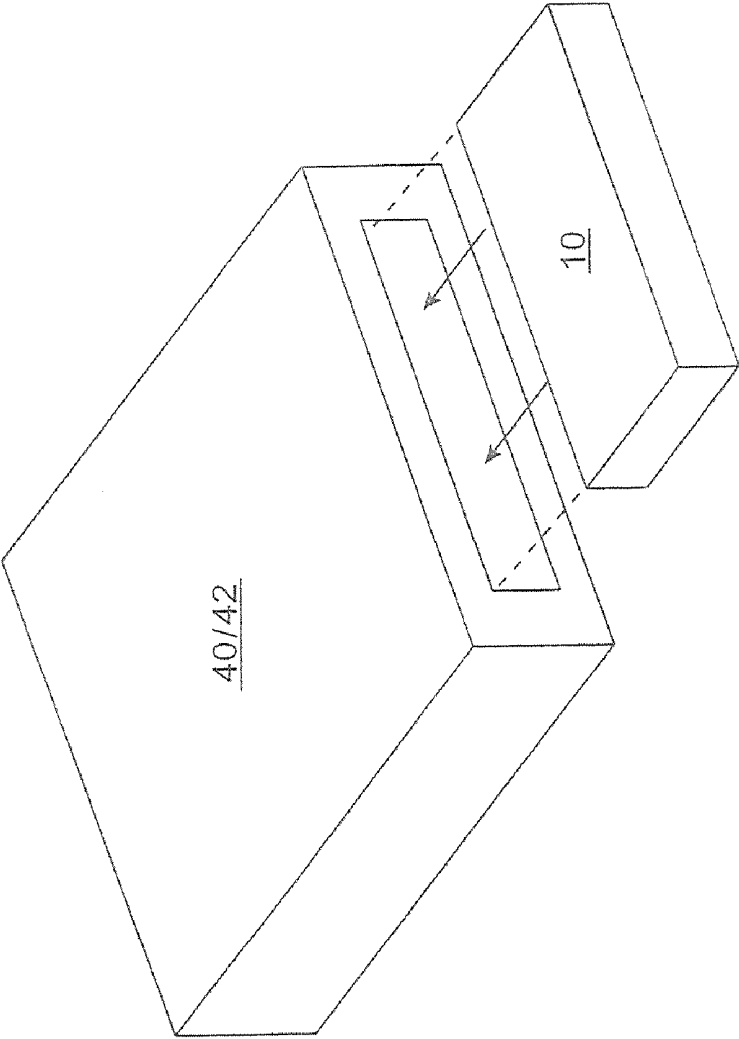


FIG. 3A

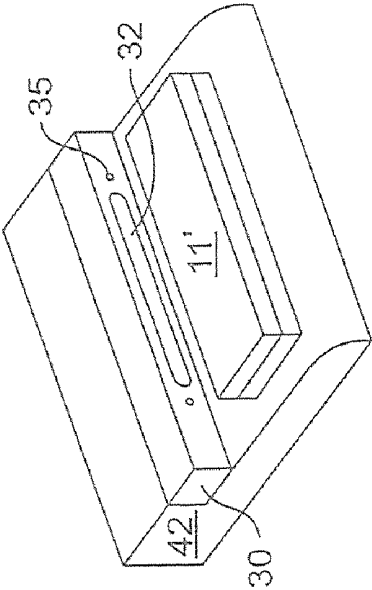


FIG. 3B

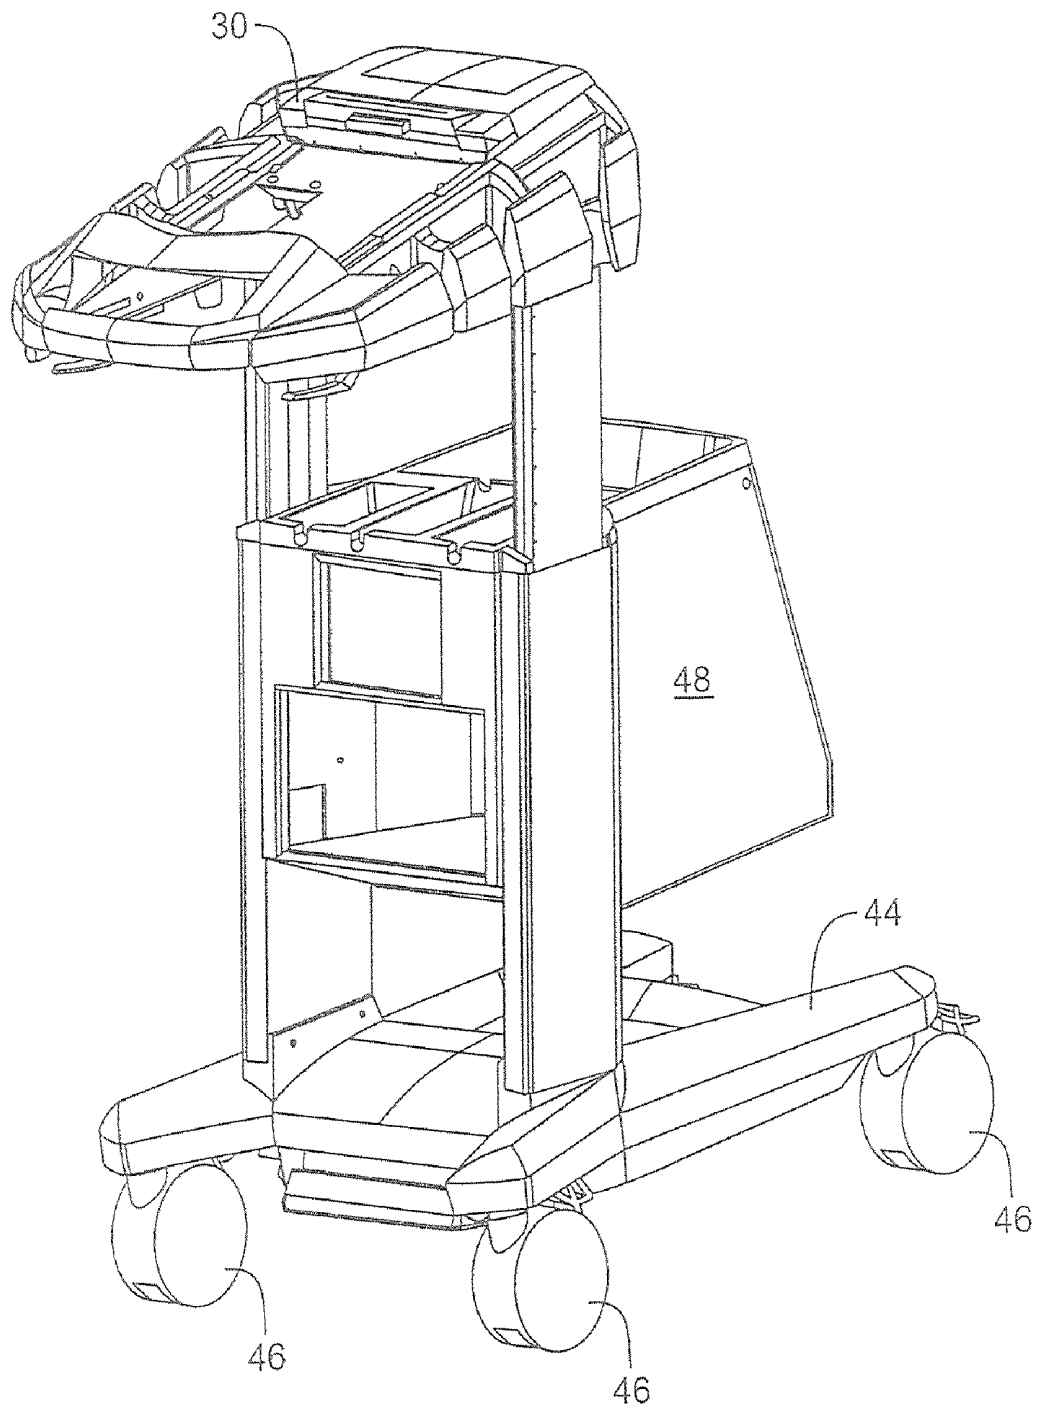


FIG. 4

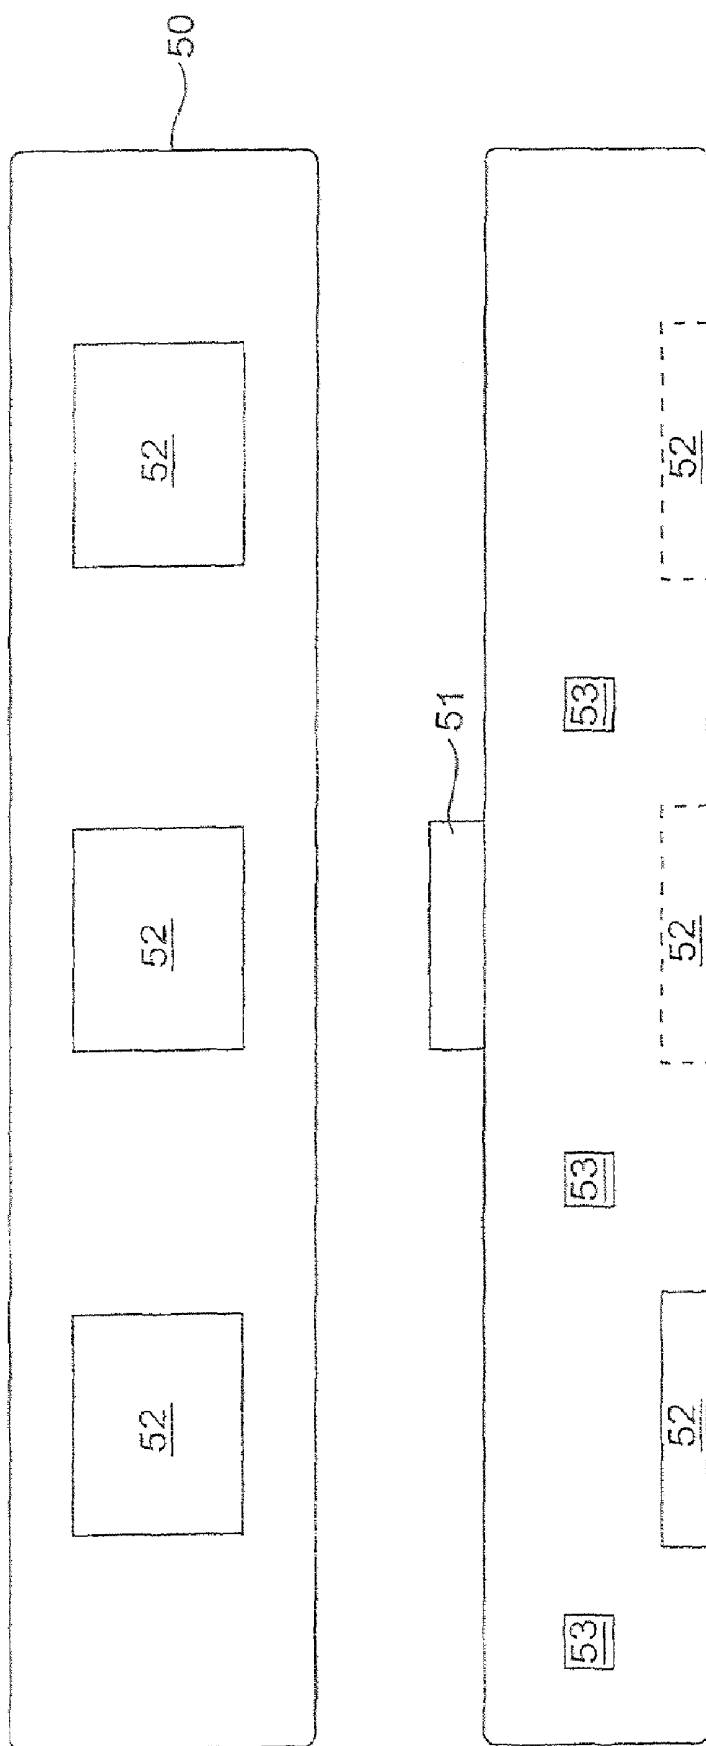


FIG. 5

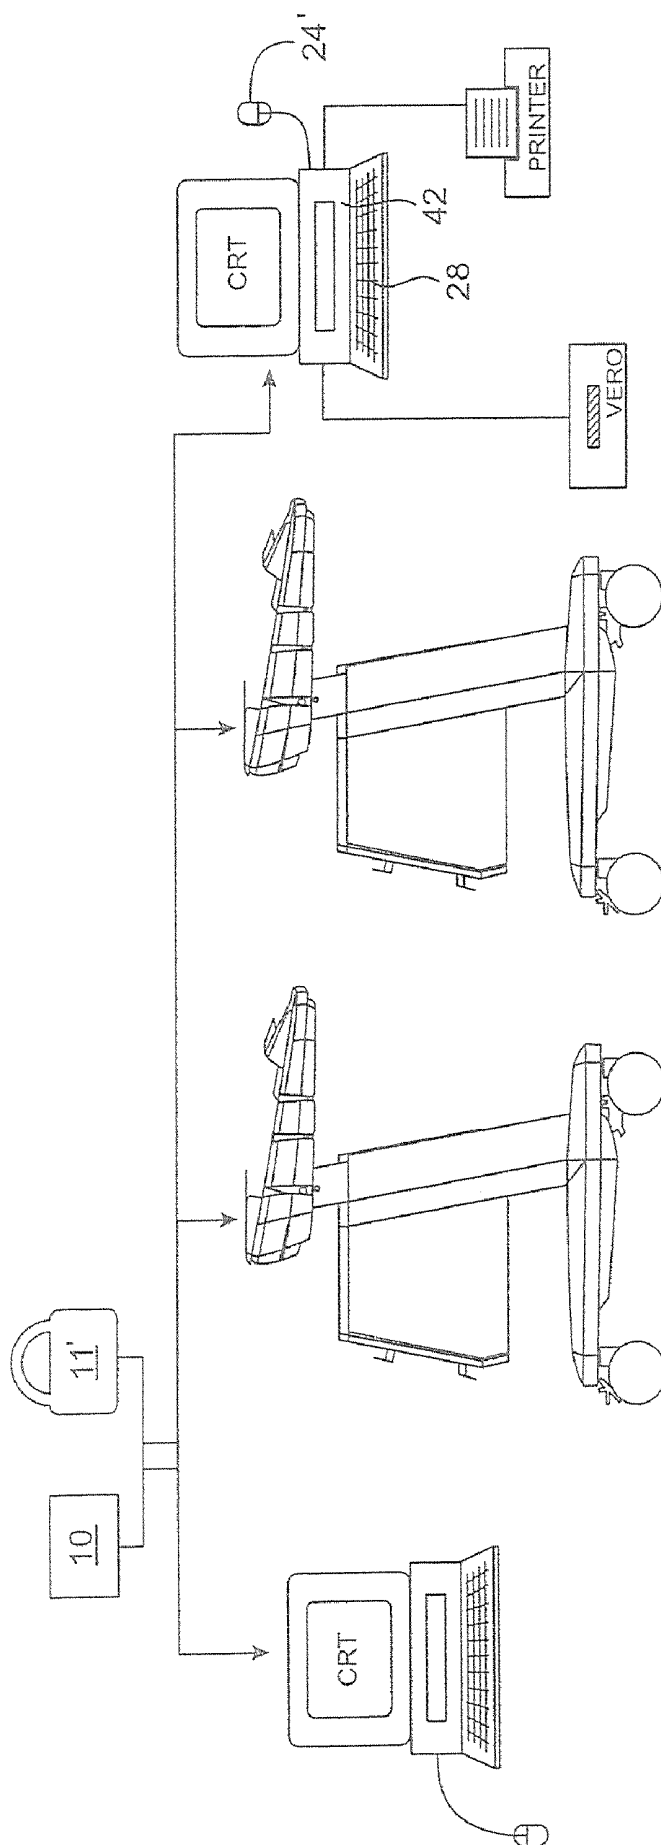


FIG. 6

MODULAR APPARATUS FOR DIAGNOSTIC ULTRASOUND

CROSS-REFERENCE TO RELATED APPLICATIONS

The present application is a divisional of commonly assigned, patent application Ser. No. 10/356,335 entitled "MODULAR APPARATUS FOR DIAGNOSTIC ULTRASOUND," filed Jan. 31, 2003, which is now U.S. Pat. No. 7,534,211 and which itself claims priority to U.S. Provisional Patent Application 60/369,023, entitled "LAPTOP ULTRASOUND DEVICE," filed Mar. 29, 2002, the disclosures of which are hereby incorporated herein by reference.

This case also includes common subject matter with U.S. patent application Ser. No. 10/356,401, filed Jan. 31, 2003, the contents of which are herein incorporated by reference.

TECHNICAL FIELD

The present invention relates to diagnostic ultrasound equipment. More particularly the present invention describes a modular system having a mobile core module for data processing, beam forming and system operations, and additional modules capable of connecting to the core module to provide additional features and connectivity to peripheral devices needed in diagnostic ultrasound procedures.

BACKGROUND OF THE INVENTION

Modern ultrasound diagnostic systems are large, complex instruments. Today's premium ultrasound systems, while mounted in carts for portability, continue to weigh several hundred pounds. In the past, ultrasound systems such as the ADR 4000 ultrasound system, produced by Advanced Technology Laboratories, Inc., were smaller desktop units about the size of a personal computer. However such instruments lacked many of the advanced features of today's premium ultrasound systems such as color Doppler imaging and three dimensional display capabilities.

The judicious use of power and signal processing on ASIC devices has enabled smaller systems to push past the feature limitations in smaller older systems that employed mechanical transducers or analog chip sets. Digital beamforming and advanced processing are now available on smaller systems such as the SonoHeart Elite, by SonoSite, Inc., and common assignee of the present invention. The success of the handheld device has spawned competitive products that are beginning to offer more advanced features. However, the use of a small handheld requires a trade off in the form of display size and battery life. Cart based units provide users with the luxury of full sized CRT monitors, as well as a host of peripheral devices at the ready. Hand held devices offer portability, but are restricted to the features built in to their chassis. Some hand held devices are offered in combination with an interface to added peripherals through a cart add on, however this increases the cost of the device and requires a user to buy specialized equipment from the manufacturer of the hand held.

Thus, there remains a need for a diagnostic ultrasound instrument which provides the advantages of light weight mobility, combined with advanced functionality traditionally restricted to larger cart based system.

There is also a need for a more economical diagnostic ultrasound system that will allow small users and institutions to purchase ultrasound units that have the capacity the user or

institution requires without having to pay the expense of additional features the user or institution will not use.

There further remains a need for a device that is portable and remains highly resistant to shock damage from being dropped or jostled during transport from place to place.

BRIEF SUMMARY OF THE INVENTION

The present invention relates to a modular diagnostic ultrasound apparatus for use in multiple environments. In a first embodiment a modular diagnostic ultrasound apparatus is disclosed comprising a core unit, a system electronics package and at least one I/O port. The core unit is a housing containing the system electronics package. The system electronics package has one or more concatenated functions and includes a front end transmit/receive circuit, a processors a back end circuit for scan conversion, a system clock and a programmable system memory device. There is also at least one I/O port connected to the front end and the back end of the system electronics package and extending through the core unit housing wherein all system data processing information is transmitted or received through the at least one I/O port.

In a second embodiment, a modular diagnostic ultrasound apparatus contained within a clamshell style enclosure weighing less than 10 pounds (4.5 kg), said enclosure further comprising: a bottom unit having a system electronics package, a battery, a plurality of user interface elements positioned substantially on a top surface of said bottom unit, at least one I/O port connector in electronic communication with said system electronics package and extending through the enclosure; a top unit hingedly connected to said bottom unit, consisting of a video display screen; and an aperture for receiving a transducer connector, said aperture being positioned substantially on the underside of the bottom unit.

In another aspect of the present invention, a mini-dock for connecting peripheral devices to a modular diagnostic ultrasound apparatus is disclosed, the mini-dock comprising: a receptacle housing; a plurality of peripheral device ports, mounted in the receptacle housing, each peripheral device port connected to one or more individual electrical connector (s) for electrical communication with a receptacle; and a receptacle for releasably mating with an I/O port of the modular diagnostic ultrasound apparatus, the receptacle capable of electronic communication with said plurality of peripheral device ports.

Another aspect of the present invention is a docking station for connecting a plurality of peripheral devices to a modular diagnostic ultrasound apparatus, the docking station comprising: a mini-dock having a housing, a plurality of peripheral device ports in electronic communication with a receptacle, the mini-dock being fixedly attached to a base; a base having a means for guiding a modular diagnostic ultrasound apparatus into alignment with the mini-dock, and a means for securing the modular diagnostic ultrasound apparatus to the mini-dock; and a power supply incorporated within the base and in electronic communication with the mini-dock such that electrical power can be fed from the power supply to the modular ultrasound apparatus through the mini-dock.

Another aspect of the modular diagnostic ultrasound apparatus is a multi-transducer connector module (multi-tap module) comprising a housing having a raised relief connector for mating with an aperture for a transducer connector on a modular diagnostic ultrasound apparatus, the multi-transducer connector having a plurality of recess connectors for fittingly engaging a plurality of transducer connectors (each using a raised relief connector adaptor), the housing having a switch for each recess connector by which an operator can

select which transducer is connected to the ultrasound device to be used at any particular moment. The switch for selecting which transducer to be used may either be an electromechanical switch, or a software implementation of a switch controlled through the user interface of the modular diagnostic ultrasound apparatus.

Still another aspect of the present invention is a mobile docking station for use with a modular diagnostic ultrasound apparatus comprising: a base having a plurality of castors wherein at least one said castor is capable of locking; a tower mounted on said base; a docking station located substantially near the top of the tower, the docking station capable of releasably receiving a modular diagnostic ultrasound apparatus; and a recesses for a plurality of peripheral devices, ergonomically positioned within said tower to allow a user convenient operation of the modular diagnostic ultrasound apparatus and a number of peripheral devices in the course of a diagnostic ultrasound scan procedure.

The modular diagnostic ultrasound apparatus also includes a system for diagnostic ultrasound examinations comprising a modular diagnostic ultrasound apparatus having an aperture for receiving a transducer connector, a sample data beam-former and signal processing electronics combined and at least one I/O port, the modular ultrasound apparatus being releasably connected to a mini-dock; a mini-dock having a plurality of peripheral device ports and a receptacle for releasably engaging said I/O port; and a mobile docking station for the modular diagnostic ultrasound apparatus, a tower, a plurality of recesses for peripheral devices and base; wherein the modular diagnostic ultrasound apparatus may operate as a portable diagnostic ultrasound device when removed from said system, or as a cart style ultrasound system when in electronic communication with said mini-dock.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1A illustrates in block diagram form the architecture of a hand held ultrasound system.

FIG. 1B shows a core unit module of the present invention.

FIG. 1C shows a clamshell embodiment of the core unit.

FIG. 2 shows a mini-dock style connector module.

FIGS. 3A and 3B show a docking station style system module.

FIG. 4 shows a mobile workstation style system module.

FIG. 5 shows a multi-tap transducer module.

FIG. 6 shows a multi station system incorporating all the modules.

DETAILED DESCRIPTION OF THE INVENTION

The focus of the present invention lies in a modular ultrasound system having a core module having the essential ultrasound processor functions, and a series of additional modules which, when combined with the core module; provide expanded capability and utility to the core module. The following description gives both the principle embodiment and alternative embodiments of the invention. Use of certain terms in the disclosure warrant clarification before an in depth discussion can occur.

The invention presented here is for an ultrasound device to be principally used for diagnostic purposes. However the term diagnostic should not be misconstrued to be read as being for non-therapeutic purposes. We use the term diagnostic to mean providing high quality imaging, as is characteristic of diagnostic imaging devices in the medical ultrasound industry. Because the present invention can provide images for use in biopsy procedures, Peripherally Inserted Central

Catheter (PICC) lines and other procedures, the use of the ultrasound device herein is not purely for diagnosis of diseases. However, we specifically disclaim any use of the present invention for a purely therapeutic purpose, such as ablative ultrasound thermal heating (as in the treatment of hypothermia) or mechanical tissue disruption, such as the generation of cavitation effects. The diagnostic ultrasound device of the present invention runs with the same power and frequency of devices used for diagnostic imaging, or therapies using diagnostic imaging—the device itself is not used as the source of therapy.

A focal point of the invention is the communication ability of the core module to the various other modules that comprise the system of the invention. Thus the core module has a single I/O port in its preferred embodiment sometimes referred to as the plug. The plug is a multi-pin electronic communication adaptor for matingly engaging a receptacle. The receptacle is a device with a corresponding pin set to match up the plug, and read data from the core module and sort it out to a variety of other devices that are in electronic communication with the receptacle. In alternative embodiments, there may be multiple I/O ports and a plug. The plug retains its function in all embodiments of the present invention, though electronic communication with additional module and components may be achieved through dedicated I/O ports. Any port in addition to the plug is a dedicate I/O port designed to receive input, or transmit output to a particular device. Likewise, in alternative embodiments of modules with a receptacle, there are no other I/O ports involved except the receptacle designed to mate with and communicate with the plug.

The core unit has a system electronics that should be understood to be the central processing core of the ultrasound device and the ultrasound engine. It can be thought of as an ultrasound motherboard. The system electronics of the core module, both in the preferred embodiment, and alternative embodiments, has the capacity to recognize and drive a group of transducer arrays such that a single core module can be connected with a plurality of transducers and perform all types of ultrasound procedures the transducers are designed for.

Turning now to FIG. 1A, a core module I/O for an ultrasound system is illustrated having system electronics 14 allowing the core module 10 to operate as a data processing and signal processing unit for a modular ultrasound system 60. The core module 10 comprises a housing 11 having the system electronics 14 mated to an I/O connector (plug) 12. A gap space 13 exists between the system electronics 14 and housing 11 and can be filled with an impact resistant padding material, or the housing can be made to abut the system electronics to eliminate or minimize the gap space. Its simplest form the core module 10 comprises just the system electronics 14 without a power supply, transducer, video interface or user interface. The core module 10 is highly mobile and very lightweight. The core module can be easily moved from place to place and mated to a modular ultrasound system 60 having the additional components desired for performing any variety of ultrasound scans.

The system electronics 14 (FIG. 1B) has one or more concatenated functions (filters) and includes a transmit/receive ASIC (beamformer) which are capable of driving one or more transducer arrays (not shown). The concatenated functions are ultrasound functions for processing signals in various ways. Two examples are a QBP filter and a digital Doppler processing function. The concatenated functions are not necessarily serially linked in that they require each other to operate. Though this is true in some cases where the processing of one type of signal is needed for the handling of another

(e.g. QBP can be used by both a B mode and a PW Doppler mode), it is not necessary that a circuit for color power angio is linked together with continuous wave Doppler, in this instance, the filters can operate independently. The transmit/receive ASIC also controls the active transmit and receive apertures of a transducer array and the gain of the received echo signals. Echo data received by the transmit/receive ASIC are provided to the adjacent front end ASIC, which digitizes and beamforms the echoes from the individual transducer elements into coherent scan line signals. The front end ASIC also controls the transmit waveform timing, aperture and focusing of the ultrasound beam through control signals provided for by the transmit/receive ASIC. A memory device is connected to the front end ASIC which stores data used by the beamformer.

The beamformed scan line signals are coupled from the front end ASIC to the adjacent digital signal processing ASIC. The digital signal processing ASIC filters the scan line signals and can provide additional features such as synthetic aperture formation, frequency compounding, Doppler processing such as power Doppler (color power angio) processing, speckle reduction, and pulse wave Doppler. Additional features such as continuous wave Doppler, can be incorporated into the system electronics if desired.

The ultrasound information is then coupled to the adjacent back end ASIC for scan conversion and the production of video outputs signals through the I/O port to the monitoring device attached to the core module. A memory device is coupled to the back end ASIC to provide storage used in three dimensional, 2D and power Doppler (3d CPA) imaging. The back end ASIC also adds alphanumeric information to the display such as the time, date, and patient identification. A graphics processor overlays the ultrasound image with information such as depth and focus markers and cursors. The graphics processor need not be incorporated into the core electronics system package, instead relying on a dedicated graphics processor card integrated into a docking module **40** of the modular system **60**, and receiving the necessary component information from the core module. The video data can be transmitted through the I/O port **12** in one of several formats including NTSC, PAL, and RGB. Frames of ultrasound images are exported to an external video memory again through the I/O port **12** coupled to the back end ASIC. The stored data can be retrieved through the system electronics using a playback mode for either live Cineloop® real time sequence or as individual stills.

The back end ASIC also includes the central processor for the core module. The central processor is preferably a RISC (reduced instruction set controller) processor. The RISC processor is coupled to the front-end and digital signal processing ASICs to control and synchronize the processing and control functions for both the core module, and the modular system the core module may be linked into at the time. A program memory is coupled to the back end ASIC to store program data which is used by the RISC processor to operate and control the core module, and the various elements of the modular system (transducer, multitap connector, video data overlay features, etc.). The RISC processor is also coupled to any user interface controls connected to the modular system, the RISC processor accepts user inputs to direct and control the operations of the core module, and the modular system as illustrated, all the inputs and outputs of the system electronics are designed to go through a single I/O port **12**.

The main system, application and control software are stored in a persistent memory device integrated directly into the system electronics. The system software, control software and application software are loaded into the system electron-

ics processors during power up. The core module may use any number of persistent memory devices integrated into the system electronics. Each ASIC includes a separate memory core having the necessary loadable data on it that is loaded into each ASIC during the power up cycle. The main system and application software includes the essential driver and communications information for the core module to communicate with and control, a select number of peripherals. In particular these peripherals include scan heads, preferred user I/O devices (such as keyboards, pointer devices and touch screen interface recognition), printers, VCRs, monitors and data storage devices. The entire volume of system and application software should be efficiently coded to preserve space and avoid the need for a large capacity storage device like a hard drive. Since the core module is principally designed for diagnostic ultrasound, large capacity storage devices such as hard drives should not be necessary. The omission of devices like a hard drive, power supply and other elements commonly incorporated into computers or typical hand held products allows the core module to be manufactured with the smallest foot print the technology will allow. The housing for the core module only needs to securely enclose the system electronics and the I/O port. To improve impact resistance, the system electronics can be encased in resin or epoxy.

Power for the core module is provided by the modular system through the I/O port, or in the alternative, through a separate I/O used as a dedicated power terminal. Although the core module preferably does not have a built in power supply, it still requires a power monitoring/regulating circuit to provide proper power to the individual components during use. An external power supply can feed energy to the core module either through the I/O port, or through a dedicated power adaptor; however the power supply "brick" must be separate from the core module.

In an alternative embodiment, as shown in FIG. 1C the core module can incorporate additional hardware elements allowing the core module to operate as a stand alone device. In a first alternative embodiment, the core module **10** includes the features of previously described hand-held ultrasound systems in the form of system electronics, video out with the addition of an on board video display device **26**, and a plurality of user inputs **28** in the form of a pointer, alphanumeric keypad, touch screen, programmable hot keys, and/or display control dials. This embodiment may also include speakers for audio output (not shown) and/or a direct transducer connection **24**. The core module **10** now requires an internal power supply **25** in the form of a battery in order to operate as a stand alone device. This embodiment also requires either a built in or removable data storage device.

For ergonomic considerations, the stand alone version of the core module may be in the form of a tablet style PC or a laptop computer, as both of these designs are commonly used today and provide users with a familiar design and interface mode. In these embodiments the core module must have sufficient video capabilities to drive the video device coupled to the core module, such as an LCD device. The display output can be as low as six bit to provide sufficient color capacity to drive the core module video display, or an external display that the core module may be attached to. The display output is preferably 8 or 16 bit, but can include 24 bit RGB output. Color supporting bandwidth is necessary for some ultrasound scans that involve color display (PW, color angio) or higher definition gray scale. Where the core module **10** may be connected to a docking station **40** having an independent video processor, the data necessary for the video display need only be transmitted to the independent video processor. It is both possible and desirable in certain instances to be able

to utilize both displays simultaneously, such as in the instances where more than one display is desired, or where it is necessary to check one display against the other as in a system diagnostic test.

In another variation on this embodiment, a form factor having the tablet or laptop configuration may include a built in handle **23**. The handle **23** may be used strictly for carrying the core module **20**, or it may serve as a sound chamber for speakers built into the handle. The handle may also serve as an I/O port for a dedicated connection, such as an external mouse, power adaptor or other user interface tool. In operation a user may use the handle as a wrist rest to reduce the incidence of repetitive motion syndrome while inputting information into the core module **10** through the user interface **28**.

No matter what user interface elements are incorporated into the core module, the principle design is still focused toward, and optimized for, using the core module with a modular system. Thus while the core module may have the features of a portable or hand-held ultrasound system, it remains primarily the core module of a larger modular system that has greater capacity for complete diagnostic ultrasound scans with a full range of peripheral devices at the ready.

As shown in FIG. **2**, the connection between the core module **10** and the modular system is through a receptacle module **30** or mini-dock. The receptacle module **30** connects peripheral devices to the core module **10**. The receptacle module **30** comprises a receptacle housing, peripheral ports **34** and a receptacle **32**. The receptacle module housing is a body designed to contain the hardware needed to provide the electronic communication between the peripheral devices and the core module **10**. A plurality of peripheral device ports **34** are mounted in said receptacle housing **30**, each peripheral device port is connected to one or more individual electrical connector(s) for electrical communication with a receptacle **32**. The receptacle **32** is designed for releasably mating with the I/O port **12** of the core module **10**. Thus the core module **10** may communicate with the desired peripheral devices through the receptacle module: and vice versa.

The electronic communication between said receptacle **32** and the plurality of peripheral device ports **34** can be either a pass through connection or an active connection. If the connection is active, the receptacle module **30** contains one or more active circuits. The interface functions essentially as an interface converter for signals. Typically the active circuits required are analog to digital (A/D) and digital to analog (D/A) converts for video out and in. It may also perform digital-to-digital conversion (D/D) for different digital video outputs. By placing the A/D and D/A converters in the receptacle housing **30**, space and weight is conserved within the core module **10**. This provides a substantial weight and real estate savings in the core module **10** whether it is used as a stand alone unit, or as a central processing core for a modular system. Video A/D and D/A converters should not be needed in the core module having built in video, since the built in display should be able to use the native signal without conversion.

The receptacle housing may also have a latching mechanism **35** for securing itself to the core module **10**. A simple latch, such as tension locking arms or hooks may be used, or an interlocking connector like rails and grooves. A manual release of the interlocking mechanism allows for an easy release of the core module and the receptacle module. This feature may be found in another module when the receptacle module **30** is connected to either a docking station **40** or a mobile docking stand **50**. The receptacle housing itself contains all the connectors needed for the core unit to interface

with a wide body of peripheral devices. Examples of such connections include specialized adaptors for power **34a**, printer **34b**, network **34c**, Ethernet **34d**, RS232 adaptor **34e**, S-video out **34f**, VGA out **34g**, composite video out **34h**, sound out **34i**, physio-adaptor **34j** (as for an ECG measuring device), and transducer adaptor **34k**. The physio port is designed for receiving input from a device that measures some physiological parameter that a user can combine with a diagnostic ultrasound scan to produce a more accurate diagnosis. Electro cardio gram (ECG) measurements are an example of such a physio-monitoring device that can be used in conjunction with the ultrasound scan. Additional controls for a full sized user interface station (keyboard, pointer, input devices) may use an additional port, or go through the Ethernet adaptor **34d** or RS232 **34e** port. The peripheral devices are "off the shelf" materials commonly used in hospitals and ultrasound scanning environments, and the receptacle housing uses peripheral ports to match these existing technologies. However the receptacle module can be constructed and configured to communicate with virtually any device so long as the system electronics **14** has the appropriate communications protocol programmed into it. The receptacle housing may further include a surge protector (not shown) to shield the core module from electrical surges while plugged into a power supply.

The receptacle housing uses a plurality of electrical pins in the receptacle **32** for communication with the I/O port **12** of the core module **10**. The layout of the pins varies with the intended communication the core module would need to interact with a modular system, or a series of stand alone peripherals. Further pin economy may be achieved by using the same pins for communicating to different devices through a well timed cycle of instructions based on the system clock, such as with an **12C** protocol. An example of the pin layout is as follows:

PINS 1-20 Power and ground
PINS 21-106 Digital video out
PINS 107-143 Communication links, (e.g. RS232, Ethernet, USB printer, **12C**, ECG and Audio in/out).
PINS 144-200 Connection status lines, additional ground lines, and spare lines.

In a fourth embodiment of the present invention, as shown in FIGS. **3A** and **3B**, a docking station **40** is designed to mate with the core module **10** through a receptacle module **30**. The docking station **40** is used for connecting a plurality of peripheral devices to the core module. The docking station **40** comprising a receptacle module **30** component as described above attached to a base unit **42**. The base unit **42** has a means for guiding the core module **10** into alignment with the receptacle module **30**. The base **42** also preferably includes a means for securing the core module and the receptacle module into place while connected. The means for guiding the core module into place and securing the core module into position can be the same feature. By way of example, the docking station may include a mechanical tray or cradle having an open position that the core module can be placed into, then the mechanical tray or cradle is moved to a closed position with the core module in place. The movement of the mechanical tray or cradle causes the core module to be moved into the proper position and locked into position at the same time. As long as the mechanical tray or cradle is in place, the core module cannot be removed or become misaligned. The mechanism could be a simple funnel type of guide rails that ensure the core module is funneled into the correct orientation for proper docking. The user in this case must apply the necessary force to ensure the core module and receptacle module or docking station properly line up. An electrome-

chanical device may also be used. A small motor could be used to perform the mechanical work of a person, and the motor could be activated as soon as it detects the core module in place, or by the push of a button from a user. The docking station incorporates a power supply within the base and in electronic communication with the receptacle module such that electrical power can be fed from the power supply to the core module through the receptacle module/mini-dock.

Alternatively the docking station may utilize a housing having a slot or aperture for slidably receiving the core module. Thus in a fashion similar to the way a VHS tape is inserted into a VCR, the core module would be placed into the docking station having a housing, and an electromechanical component would draw the core module into the housing and secure it in place. In this embodiment the housing can be either attached to the base, or incorporate the base into a single component. In this embodiment it is not possible to utilize and video display which may be incorporated into the core module, therefore it would be preferable to reinforce the internal frame of the housing to support the weight of a video display, such as a CRT, LCD or plasma display monitor.

In either format, the docking station would not be mobile, so the use of additional accessories that ordinarily would not be considered highly portable is logistically acceptable here. Such additional components include a larger, more ergonomically designed user interface, such as a full size QWERTY style keyboard, a pointing device such as a mouse, track ball or "joy stick." A large touch screen can also be used to allow the use of on screen hot keys and supplemental pointer device.

As shown in FIG. 5, a fifth module for use with the docking station is a multi-transducer interface module 50. The multi-transducer interface module 50 has a single transducer connector 51 for mating with the docking station 40, or in the alternative with the transducer connector aperture 24' (FIG. 6) of the core module, and a plurality of transducer connector apertures 52 incorporated into the multi-tap module. In this manner the docking station 40 can have at the ready a variety of ultrasound probes, such as a neonatal probe, trans-esophageal probe, or any other probe desired to be used in a diagnostic scan. When the core module 10 is mated to the docking station 40 and powered up, the core module 10 can detect which transducers are connected to the system and select the appropriate beamformer program and data processing to match the probe. The multi-tap module 50 may incorporate either a plurality of electromechanical switches 53 to allow a user to switch between probes, or the core module 10 may contain a soft switch within its system electronics package to switch between transducers at the direction of a user.

Additional utility is realized in a sixth embodiment in the form of a mobile docking station as shown in FIG. 4. The mobile docking station comprises a base 44 having a plurality of castors 46 wherein at least one said castor is capable of locking a tower 48 is mounted on the base and a docking station 40 is located substantially near the top of the tower 48, the docking station 40 is capable of releasably receiving the core module 10.

The mobile docking station 45 can incorporate a plurality of storage bins into the tower design. The bins can be used for the storage of both peripheral devices such as a printer, data storage device and VCR, as well as peripheral equipment such as coupling gels, transducers, connecting cables and the like. The tower is preferably height adjustable and may include gas cylinders actuated by a manual trigger to raise or lower the docking station. The tower is preferably a weight balanced design to avoid imbalance of the mobile docking station either while in use, or while being moved from place to place. The tower may be any design corresponding to the

weight balanced design, such as an "A" frame, "Z" frame, an inverted "T" frame, or an "I" frame. Multiple other frames are equally usable assuming the base has been weighted to compensate for the positioning of peripheral devices and accessory products that might be used in the ordinary course of the mobile docking station.

Similar in the design and intended use of the stationary docking station, the mobile docking station can incorporate the interface to the core module for a multi-transducer adaptor (multi-tap module) and an enhanced user interface utilizing full sized components for ease of use.

In another embodiment of the present invention, as shown in FIG. 6 a system is envisioned for providing enhanced diagnostic ultrasound flexibility and capacity through the use of one or more core modules 10 and a plurality of docking stations 40. The docking stations may either be desktop stationary 40 or mobile 45 in design. In this manner, a user, such as a hospital or clinic can reduce the costs of purchasing a variety of ultrasound devices, and instead purchase a multitude of cheaper docking stations 40 or mobile docking stations 45. It can be appreciated by those who perform ultrasound scans that there is an advantage for only paying for expensive equipment such as the core module once or twice, and being able to carry that around easily and using it with cheaper docking stations or mobile docking stations. Substantial savings in capital equipment may be made in using a system of this design. The alternative embodiment of the core module 10 which incorporates hand held functionality can then operate as a mobile or field device and then return to a docking station for operation with a plurality of peripheral devices, thus enabling the mobile unit to perform as the processor for an ultrasound suite. The core module 10 is designed to provide complex ultrasound capabilities such as those found in large, premium devices, as well as scaled down feature sets in the event it is plugged into a dock with less capable peripherals. The core module is fairly simple in construction, yet provides the processing for as many ultrasound features as a user may desire. The core may be easily and quickly removed from one dock and inserted into another, even if the docking station is "hot" (powered).

Where the core module is moved from one docking station to another within system 60, the system electronics package has the capability to either automatically detect, or identify through user input, the type of ultrasound probe attached to the docking station it is being used with, and draw on the appropriate concatenated filters needed. This allows maximum flexibility and minimum user effort in the system.

While the descriptions above provide a sense of the invention, the full scope of the invention is more accurately provided in the appended claims.

What is claimed is:

1. A modular diagnostic ultrasound system, said system comprising:

- a core module having at least one I/O port; and
- a receptacle module releasably mated with said core module, said receptacle module having a plurality of connector apertures for connecting to a plurality of diagnostic probes and a single transducer connector for connecting to said core module via said at least one I/O port, wherein when said core module is mated to said receptacle module, said core module detects which of said plurality of diagnostic probes are attached to said receptacle module, switches between said plurality of diagnostic probes under direction of a user, and selects beamformer programming and data processing to match a selected diagnostic probe.

11

2. The modular diagnostic ultrasound system of claim 1, said receptacle module further comprising:

- a receptacle housing;
- a plurality of peripheral ports mounted in said receptacle housing; and
- a receptacle for releasably mating with said at least one I/O port and electrically communicating with said plurality of peripheral ports.

3. The modular diagnostic ultrasound system of claim 2 wherein said electrically communicating occurs through a pass-through connection.

4. The modular diagnostic ultrasound system of claim 3 wherein said electrically communicating occurs through an active connection.

5. The modular diagnostic ultrasound system of claim 4, said receptacle module further comprising:

- at least one active circuit.

6. The modular diagnostic ultrasound system of claim 2, said receptacle module further comprising:

- a latching mechanism for securing said receptacle module to said core module.

7. The modular diagnostic ultrasound system of claim 2 wherein said receptacle module is attached to a docking station.

8. The modular diagnostic ultrasound system of claim 7 wherein said docking station is stationary.

9. The modular diagnostic ultrasound system of claim 7 wherein said docking station is mobile.

10. The modular diagnostic ultrasound system of claim 1 wherein said core module switches between said plurality of diagnostic probes using a plurality of electromechanical switches.

11. The modular diagnostic ultrasound system of claim 1 wherein said core module switches between said plurality of diagnostic probes using a soft switch within said core module.

12. A modular diagnostic ultrasound apparatus comprising:

- a core module including a system electronics package mated to at least one plug; and

- a receptacle module having a receptacle for matingly engaging said at least one plug of said core module, a plurality of connector apertures for connecting to a plurality of diagnostic probes, and a plurality of peripheral ports for connecting to a plurality of peripheral devices, wherein said receptacle reads data from said core module and sends data to at least one of said plurality of peripheral devices in electronic communication with said receptacle and wherein when said core module is mated to said receptacle module, said core module detects which of said plurality of diagnostic probes are attached to said receptacle module and selects beamformer programming and data processing to match a detected diagnostic probe.

13. The modular diagnostic ultrasound apparatus of claim 12, said system electronics package further comprising:

- a transmit/receive ASIC which receives echo data;

12

- a front end ASIC which transforms said echo data into beamformed scan line signals; and

- a back end ASIC which converts said beamformed scan line signals to video output signals.

14. The modular diagnostic ultrasound apparatus of claim 13, said system electronics package further comprising:

- a digital signal processing ASIC which filters said beamformed scan line signals.

15. The modular diagnostic ultrasound apparatus of claim 14, said back end ASIC further comprising:

- a central processor coupled to said front end ASIC and said digital signal processing ASIC to control and synchronize processing and control functions for said core module.

16. The modular diagnostic ultrasound apparatus of claim 12, said system electronics package further comprising:

- at least one programmable system memory device.

17. The modular diagnostic ultrasound apparatus of claim 12 wherein said core module is configured to switch between said plurality of diagnostic probes under direction of a user, and select beamformer programming and data processing to match a selected diagnostic probe.

18. A modular ultrasound diagnostic system, said system comprising:

- a core module including at least one I/O port; and
- a mini-dock configured to connect a plurality of diagnostic probes and peripheral devices to said core module, said mini-dock comprising a receptacle housing, a plurality of peripheral device ports for connecting to said plurality of peripheral devices, a plurality of connector apertures for connecting to said plurality of diagnostic probes, and a receptacle for matingly engaging with said at least one I/O port of said core module, said receptacle in electronic communication with said plurality of peripheral device ports, wherein said core module communicates with said plurality of peripheral devices through said mini-dock and wherein when said core module is mated to said mini-dock, said core module is configured to switch between said plurality of diagnostic probes connected to said core module under direction of a user, wherein said core module is configured to select beamformer programming and data processing to match a selected diagnostic probe.

19. The modular ultrasound diagnostic system of claim 18 wherein each of said plurality of peripheral device ports is mounted in said receptacle housing and is connected to one or more electrical connectors for electrical communication with said receptacle.

20. The modular ultrasound diagnostic system of claim 18 having one or more means for removably connecting said mini-dock to said core module.

21. The modular ultrasound diagnostic system of claim 18 wherein at least one of said plurality of peripheral device ports comprises an ultrasound transducer adaptor.

* * * * *

专利名称(译)	用于诊断超声的模块化设备		
公开(公告)号	US8088071	公开(公告)日	2012-01-03
申请号	US12/467899	申请日	2009-05-18
[标]申请(专利权)人(译)	索诺塞特公司		
申请(专利权)人(译)	SONOSITE INC.		
当前申请(专利权)人(译)	FUJIFILM SONOSITE , INC.		
[标]发明人	HWANG JUIN JET LITTLE BLAKE W		
发明人	HWANG, JUIN-JET LITTLE, BLAKE W.		
IPC分类号	A61B8/14 A61B8/00 G06F13/00 G01S7/521 G01S15/89		
CPC分类号	G01S7/52079 G01S7/52082 G01S15/899 A61B8/4411 A61B8/4427 A61B8/4433 A61B8/4405 A61B8/56		
优先权	60/369023 2002-03-29 US		
其他公开文献	US20090275835A1		
外部链接	Espacenet USPTO		

摘要(译)

提供了一种模块化诊断超声设备，包括核心单元，系统电子器件和I/O端口。核心单元包括壳体和在壳体内的系统电子封装。系统电子器件具有一个或多个级联滤波器，包括前端发射/接收电路，处理器，用于扫描转换的后端电路，系统时钟和可编程系统存储器设备。存在至少一个I/O端口，其连接到系统电子封装的前端和后端并延伸穿过核心单元壳体，其中通过I/O端口发送或接收所有系统数据处理信息。

