



US010639008B2

(12) **United States Patent**  
**Lindekugel et al.**

(10) **Patent No.:** **US 10,639,008 B2**  
(45) **Date of Patent:** **May 5, 2020**

(54) **SUPPORT AND COVER STRUCTURES FOR AN ULTRASOUND PROBE HEAD**

(75) Inventors: **Eric W. Lindekugel**, Salt Lake City, UT (US); **Jeremy B. Cox**, Salt Lake City, UT (US); **Daniel B. Blanchard**, North Salt Lake, UT (US); **Christian W. Crook**, West Jordan, UT (US); **Eddie K. Burnside**, Bountiful, UT (US); **Jeanette E. Southard**, Park City, UT (US); **Kevin W. Stinger**, Kaysville, UT (US); **Amir Orome**, Sandy, UT (US)

(73) Assignee: **C. R. Bard, Inc.**, Franklin Lakes, NJ (US)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 2383 days.

(21) Appl. No.: **13/206,396**

(22) Filed: **Aug. 9, 2011**

(65) **Prior Publication Data**

US 2011/0313293 A1 Dec. 22, 2011

**Related U.S. Application Data**

(63) Continuation-in-part of application No. 12/900,750, filed on Oct. 8, 2010.

(Continued)

(51) **Int. Cl.**  
**A61B 8/00** (2006.01)  
**A61B 17/34** (2006.01)

(Continued)

(52) **U.S. Cl.**  
CPC ..... **A61B 8/44** (2013.01); **A61B 8/42** (2013.01); **A61B 8/4209** (2013.01);  
(Continued)

(58) **Field of Classification Search**

CPC ... A61B 8/4281; A61B 8/4455; A61B 8/4472;  
A61B 10/00; A61B 17/3403; A61B 8/44;  
(Continued)

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

3,133,244 A 5/1964 Wojtulewicz  
3,297,020 A 1/1967 Mathiesen  
(Continued)

**FOREIGN PATENT DOCUMENTS**

AU 642647 11/1990  
AU 1860597 B2 6/1999  
(Continued)

**OTHER PUBLICATIONS**

Forauer, AR et al, Change in Peripherally Inserted Central Catheter Tip Location with Abduction and Adduction of the Upper Extremity, J Vasc Interv Radiol, pp. 1315-1318, vol. 11 No. 10, Nov.-Dec. 2000.

(Continued)


*Primary Examiner* — Amanda Lauritzen Moher

(74) *Attorney, Agent, or Firm* — Rutan & Tucker LLP

(57) **ABSTRACT**

A probe cap for use with an ultrasound probe including a head portion and an acoustic surface is disclosed. In one embodiment, the probe cap includes a body that defines a cavity sized for releasably receiving the head portion of the probe therein. The probe cap body further defines a hole that is proximate the acoustic surface of the head portion. A compliant spacer component is disposed in the hole. The spacer component can include a hydrogel and provides an acoustic path between the acoustic surface and a tissue surface of a patient. The spacer component includes a skin contact surface that defines a concavity and is deformable against the tissue surface. Additional embodiments disclose various probe cap and accompanying needle guide designs

(Continued)

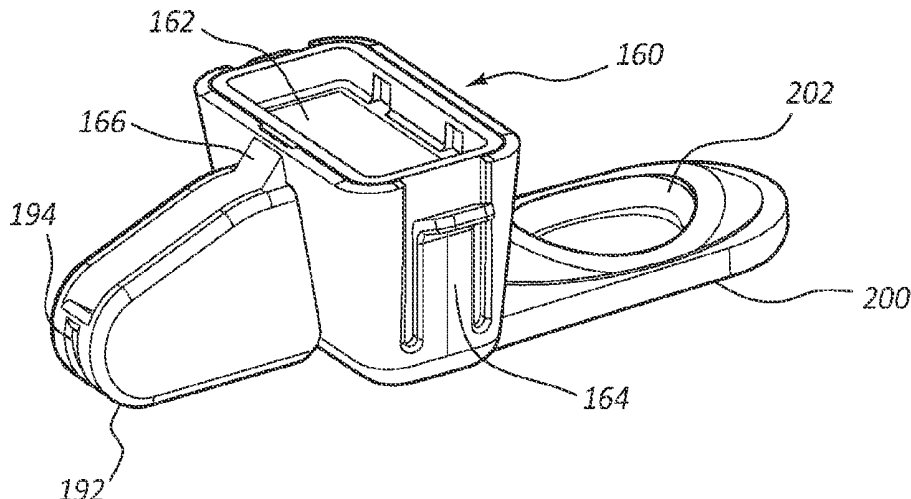

for use in assisting a clinician with ultrasound probe use and needle insertion into a patient.

### 13 Claims, 26 Drawing Sheets

### Related U.S. Application Data

- (60) Provisional application No. 61/372,044, filed on Aug. 9, 2010, provisional application No. 61/249,850, filed on Oct. 8, 2009.

(51) **Int. Cl.**

*A61B 10/00* (2006.01)  
*A61B 18/00* (2006.01)  
*A61B 18/02* (2006.01)  
*G10K 11/02* (2006.01)  
*A61K 49/22* (2006.01)

(52) **U.S. Cl.**

CPC ..... *A61B 8/4272* (2013.01); *A61B 8/4281* (2013.01); *A61B 8/4444* (2013.01); *A61B 8/4455* (2013.01); *A61B 8/46* (2013.01); *A61B 10/00* (2013.01); *A61B 17/3403* (2013.01); *A61B 8/4218* (2013.01); *A61B 8/4227* (2013.01); *A61B 8/4236* (2013.01); *A61B 8/4472* (2013.01); *A61B 8/4483* (2013.01); *A61B 2018/00964* (2013.01); *A61B 2018/0231* (2013.01); *A61B 2562/00* (2013.01); *A61B 2562/0204* (2013.01); *A61B 2562/16* (2013.01); *A61K 49/226* (2013.01); *G10K 11/02* (2013.01)

(58) **Field of Classification Search**

CPC ..... *A61B 8/46*; *A61B 8/4444*; *A61B 8/4272*; *A61B 8/4209*; *A61B 8/42*; *A61B 8/4483*; *A61B 8/4236*; *A61B 8/4227*; *A61B 8/4218*; *A61B 2562/16*; *A61B 2562/0204*; *A61B 2562/00*; *A61B 2018/0231*; *A61B 2018/00964*; *A61M 25/02*  
 USPC ..... 600/459  
 See application file for complete search history.

(56) **References Cited**

### U.S. PATENT DOCUMENTS

3,625,200 A	12/1971	Muller
3,674,014 A	7/1972	Tillander et al.
3,817,241 A	6/1974	Grausz
3,847,157 A	11/1974	Caillouette et al.
3,868,565 A	2/1975	Kuipers
3,902,501 A	9/1975	Citron et al.
3,995,623 A	12/1976	Blake et al.
4,003,369 A	1/1977	Heilman et al.
4,063,561 A	12/1977	McKenna
4,072,146 A	2/1978	Howes
4,114,601 A	9/1978	Abels
4,149,535 A	4/1979	Volder et al.
4,173,228 A	11/1979	Steenwyk et al.
4,175,566 A	11/1979	Millar
4,181,120 A	1/1980	Kunii et al.
4,224,949 A	9/1980	Scott et al.
4,244,362 A	1/1981	Anderson
4,246,792 A	1/1981	Matzuk
4,289,139 A	9/1981	Enjoji et al.
4,317,078 A	2/1982	Weed et al.
4,327,722 A	5/1982	Groshong et al.
4,362,166 A	12/1982	Furler et al.
4,365,639 A	12/1982	Goldreyer
4,380,237 A	4/1983	Newbower
4,402,324 A	9/1983	Lindgren et al.
4,407,294 A	10/1983	Vilkomerson
4,429,693 A	2/1984	Blake et al.
4,431,005 A	2/1984	McCormick
4,431,214 A	2/1984	Buffington
4,445,501 A	5/1984	Bresler
4,459,854 A	7/1984	Richardson et al.
4,469,106 A	9/1984	Harui
4,483,343 A	11/1984	Beyer et al.
4,491,137 A	1/1985	Jingu
4,565,201 A	1/1986	Lass
4,572,198 A	2/1986	Codrington
4,577,634 A	3/1986	Gessman
4,582,067 A	4/1986	Silverstein et al.
4,588,394 A	5/1986	Schulte et al.
4,593,687 A	6/1986	Gray
4,593,699 A	6/1986	Poncy et al.
4,595,012 A	6/1986	Webler et al.
4,601,706 A	7/1986	Aillon
4,608,989 A	9/1986	Drue
4,608,992 A	9/1986	Hakim et al.
4,619,247 A	10/1986	Inoue et al.
4,622,644 A	11/1986	Hansen
4,644,960 A	2/1987	Johans
4,652,820 A	3/1987	Maresca
4,665,925 A	5/1987	Millar
4,667,230 A	5/1987	Arakawa et al.
4,674,518 A	6/1987	Salo
4,676,249 A	6/1987	Arenas et al.
4,681,106 A	7/1987	Kensley et al.
4,681,117 A	7/1987	Brodman et al.
4,688,578 A	8/1987	Takano et al.
4,692,148 A	9/1987	Kantrowitz et al.
4,697,595 A	10/1987	Breyer et al.
4,700,997 A	10/1987	Strand
4,706,681 A	11/1987	Breyer et al.
4,710,708 A	12/1987	Rorden et al.
4,733,669 A	3/1988	Segal
4,737,794 A	4/1988	Jones
4,741,356 A	5/1988	Letzo et al.
4,742,356 A	5/1988	Kuipers
4,753,247 A	6/1988	Kirsner et al.
4,770,185 A	9/1988	Silverstein et al.
4,771,788 A	9/1988	Millar
4,781,685 A	11/1988	Lehmann et al.
4,784,646 A	11/1988	Feingold
4,787,070 A	11/1988	Suzuki et al.
4,787,396 A	11/1988	Pidorenko
4,793,361 A	12/1988	DuFault
4,794,930 A	1/1989	Machida et al.
4,796,632 A	1/1989	Boyd et al.
4,798,588 A	1/1989	Aillon
4,798,598 A	1/1989	Bonello et al.
4,809,681 A	3/1989	Kantrowitz et al.
4,809,713 A	3/1989	Grayzel
4,813,729 A	3/1989	Speckhart
4,821,731 A	4/1989	Martinelli et al.
4,836,214 A	6/1989	Sramek
4,840,622 A	6/1989	Hardy
4,849,692 A	7/1989	Blood
4,850,358 A	7/1989	Millar
4,852,580 A	8/1989	Wood
4,856,317 A	8/1989	Pidorenko et al.
4,856,529 A	8/1989	Segal
4,860,757 A	8/1989	Lynch et al.
4,867,169 A	9/1989	Machida et al.
4,869,263 A	9/1989	Segal et al.
4,869,718 A	9/1989	Brader
4,887,606 A	12/1989	Yock et al.
4,887,615 A	12/1989	Taylor
4,889,128 A	12/1989	Millar
4,899,756 A	2/1990	Sonek
4,901,725 A	2/1990	Nappholz et al.
4,905,698 A	3/1990	Strohl, Jr. et al.
4,911,173 A	3/1990	Terwilliger
4,911,174 A	3/1990	Pederson et al.
4,924,870 A	5/1990	Wlodarczyk et al.
4,943,770 A	7/1990	Ashley-Rollman et al.
4,945,305 A	7/1990	Blood
4,947,852 A	8/1990	Nassi et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

4,957,111 A	9/1990	Millar	5,279,129 A	1/1994	Ito
4,961,433 A	10/1990	Christian	5,279,607 A	1/1994	Schentag et al.
4,966,148 A	10/1990	Millar	5,280,786 A	1/1994	Wlodarczyk et al.
4,967,753 A	11/1990	Haase et al.	5,287,331 A	2/1994	Schindel et al.
4,977,886 A	12/1990	Takehana et al.	5,289,373 A	2/1994	Zarge et al.
4,989,608 A	2/1991	Ratner	5,292,342 A	3/1994	Nelson et al.
4,995,396 A	2/1991	Inaba et al.	5,295,485 A	3/1994	Shinomura et al.
4,998,916 A	3/1991	Hammerslag et al.	5,307,072 A	4/1994	Jones, Jr.
5,005,592 A	4/1991	Cartmell	5,311,871 A	5/1994	Yock
5,016,173 A	5/1991	Kenet et al.	5,313,949 A	5/1994	Yock
5,025,799 A	6/1991	Wilson	5,318,025 A	6/1994	Dumoulin et al.
5,029,585 A	7/1991	Lieber et al.	5,325,860 A	7/1994	Seward et al.
5,040,548 A	8/1991	Yock	5,325,873 A	7/1994	Hirschi et al.
5,042,486 A	8/1991	Pfeiler et al.	5,330,496 A	7/1994	Alferness
5,045,071 A	9/1991	McCormick et al.	5,331,966 A	7/1994	Bennett et al.
5,046,497 A	9/1991	Millar	5,333,614 A	8/1994	Feiring
5,050,607 A	9/1991	Bradley et al.	5,337,678 A	8/1994	Grout et al.
5,057,095 A	10/1991	Fabian	5,341,807 A	8/1994	Nardella
5,058,595 A	10/1991	Kern	5,343,865 A	9/1994	Gardineer et al.
5,067,489 A	11/1991	Lind	5,345,940 A	9/1994	Seward et al.
5,076,278 A	12/1991	Vilkomerson et al.	5,348,020 A	9/1994	Hutson
5,076,279 A *	12/1991	Arenson ..... A61B 1/00142 600/459	5,350,352 A	9/1994	Buchholtz et al.
5,078,140 A	1/1992	Kwoh	5,357,961 A	10/1994	Fields et al.
5,078,148 A	1/1992	Nassi et al.	5,369,624 A	11/1994	Fukukita et al.
5,078,149 A *	1/1992	Katsumata ..... A61B 8/4281 600/459	5,375,596 A	12/1994	Twiss et al.
5,078,678 A	1/1992	Katims	5,376,083 A	12/1994	Mische
5,078,714 A	1/1992	Katims	5,377,678 A	1/1995	Dumoulin et al.
5,084,022 A	1/1992	Claude	5,385,053 A	1/1995	Wlodarczyk et al.
5,092,341 A	3/1992	Kelen	5,390,675 A	2/1995	Sheehan et al.
5,099,845 A	3/1992	Besz et al.	5,391,199 A	2/1995	Ben-Haim
5,099,850 A	3/1992	Matsui et al.	5,394,876 A	3/1995	Ma
5,100,387 A	3/1992	Ng	5,394,877 A	3/1995	Orr et al.
5,105,829 A	4/1992	Fabian et al.	5,395,366 A	3/1995	D'Andrea et al.
5,109,862 A	5/1992	Kelen et al.	5,398,683 A	3/1995	Edwards et al.
5,114,401 A	5/1992	Stuart et al.	5,398,691 A	3/1995	Martin et al.
5,121,750 A	6/1992	Katims	5,405,366 A	4/1995	Fox et al.
D327,740 S	7/1992	Arioka et al.	5,411,485 A	5/1995	Tennican et al.
5,134,370 A	7/1992	Jefferts et al.	5,413,107 A	5/1995	Oakley et al.
5,144,955 A	9/1992	O'Hara	5,422,478 A	6/1995	Wlodarczyk et al.
5,158,086 A	10/1992	Brown et al.	5,425,367 A	6/1995	Shapiro et al.
5,160,342 A	11/1992	Reger et al.	5,425,370 A	6/1995	Vilkomerson
5,161,536 A	11/1992	Vilkomerson et al.	5,425,382 A	6/1995	Golden et al.
5,174,295 A	12/1992	Christian et al.	5,427,114 A	6/1995	Colliver et al.
5,184,601 A	2/1993	Putman	5,429,132 A	7/1995	Guy et al.
5,190,045 A	3/1993	Frazin	5,429,617 A	7/1995	Hammersmark et al.
5,202,985 A	4/1993	Goyal	5,431,641 A	7/1995	Grozinger et al.
5,211,165 A	5/1993	Dumoulin et al.	5,433,729 A	7/1995	Adams et al.
5,211,636 A	5/1993	Mische	5,437,276 A	8/1995	Takada et al.
5,212,988 A	5/1993	White et al.	5,437,277 A	8/1995	Dumoulin et al.
5,214,615 A	5/1993	Bauer et al.	5,438,873 A	8/1995	Wlodarczyk et al.
5,217,026 A	6/1993	Stoy et al.	5,443,066 A	8/1995	Dumoulin et al.
5,220,924 A	6/1993	Frazin	5,443,489 A	8/1995	Ben-Haim
5,235,987 A	8/1993	Wolfe	5,445,150 A	8/1995	Dumoulin et al.
5,239,464 A	8/1993	Blair et al.	5,450,846 A	9/1995	Goldreyer
5,240,004 A	8/1993	Walinsky et al.	5,453,575 A	9/1995	O'Donnell et al.
5,243,995 A	9/1993	Maier	5,456,256 A	10/1995	Schneider
5,246,007 A	9/1993	Frisbie et al.	5,456,718 A	10/1995	Szymaitis
5,247,171 A	9/1993	Wlodarczyk et al.	5,464,016 A	11/1995	Nicholas et al.
5,251,635 A	10/1993	Dumoulin et al.	5,469,851 A	11/1995	Lipschutz
5,255,680 A	10/1993	Darrow et al.	5,474,065 A	12/1995	Meathrel et al.
5,257,636 A	11/1993	White	5,476,090 A	12/1995	Kishi
5,257,979 A	11/1993	Jagpal	5,480,422 A	1/1996	Ben-Haim
5,259,386 A	11/1993	Sharkawy	5,487,729 A	1/1996	Avellanet et al.
5,261,409 A	11/1993	Dardel	5,490,522 A *	2/1996	Dardel ..... A61B 1/00142 600/461
5,265,610 A	11/1993	Darrow et al.	5,492,538 A	2/1996	Johlin, Jr.
5,265,614 A	11/1993	Hayakawa et al.	5,494,038 A	2/1996	Wang et al.
5,267,569 A	12/1993	Lienhard	5,500,012 A	3/1996	Brucker et al.
5,270,810 A	12/1993	Nishimura	5,505,205 A	4/1996	Solomon et al.
5,271,404 A	12/1993	Corl et al.	5,509,822 A	4/1996	Negus et al.
5,273,025 A	12/1993	Sakiyama et al.	5,513,637 A	5/1996	Twiss et al.
5,273,042 A	12/1993	Lynch et al.	5,515,853 A	5/1996	Smith et al.
5,274,551 A	12/1993	Corby, Jr.	5,522,878 A	6/1996	Montecalvo et al.
5,275,053 A	1/1994	Wlodarczyk et al.	5,526,812 A	6/1996	Dumoulin et al.
			5,531,664 A	7/1996	Adachi et al.
			5,540,033 A	7/1996	Fox et al.
			5,540,230 A	7/1996	Vilkomerson
			5,540,681 A	7/1996	Strul et al.
			5,542,938 A	8/1996	Avellanet et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

5,546,949 A	8/1996	Frazin et al.	5,751,785 A	5/1998	Moorman et al.
5,546,951 A	8/1996	Ben-Haim	5,752,513 A	5/1998	Acker et al.
5,558,091 A	9/1996	Acker et al.	5,758,650 A	6/1998	Miller et al.
5,568,809 A	10/1996	Ben-haim	5,762,064 A	6/1998	Polvani
5,569,183 A *	10/1996	Kieturakis ..... A61B 17/00008 604/500	5,767,669 A	6/1998	Hansen et al.
D375,450 S	11/1996	Bidwell et al.	5,767,960 A	6/1998	Orman et al.
5,570,671 A	11/1996	Hickey	5,769,786 A	6/1998	Wiegel
5,575,291 A *	11/1996	Hayakawa ..... C08J 3/075 600/459	5,769,843 A	6/1998	Abela et al.
5,583,286 A	12/1996	Matsuyama	5,769,881 A	6/1998	Schroepel et al.
5,588,442 A	12/1996	Scovil et al.	5,771,896 A	6/1998	Sliwa, Jr. et al.
5,592,939 A	1/1997	Martinelli	5,775,322 A	7/1998	Silverstein et al.
5,598,846 A	2/1997	Peszynski	5,775,332 A	7/1998	Goldman
5,599,299 A	2/1997	Weaver et al.	5,779,638 A	7/1998	Vesely et al.
5,600,330 A	2/1997	Blood	5,782,767 A	7/1998	Pretlow, III
5,610,967 A	3/1997	Moorman et al.	5,782,769 A	7/1998	Hwang et al.
5,615,678 A	4/1997	Kirkham et al.	5,785,657 A	7/1998	Breyer et al.
5,617,864 A	4/1997	Stouffer et al.	5,787,049 A	7/1998	Bates
5,617,866 A	4/1997	Marian, Jr.	5,792,055 A	8/1998	McKinnon et al.
5,622,169 A	4/1997	Golden et al.	5,795,297 A	8/1998	Daigle
5,622,170 A	4/1997	Schulz	5,795,298 A	8/1998	Vesely et al.
5,622,184 A	4/1997	Ashby et al.	5,795,632 A	8/1998	Buchalter
5,623,931 A *	4/1997	Wung ..... A61B 17/3403 600/461	5,797,849 A	8/1998	Vesely et al.
5,624,430 A	4/1997	Eton et al.	5,800,352 A	9/1998	Ferre et al.
5,626,554 A	5/1997	Ryaby et al.	5,800,410 A	9/1998	Gawreluk
5,626,870 A	5/1997	Monshipouri et al.	5,800,497 A	9/1998	Bakels et al.
5,630,419 A	5/1997	Ranalletta	5,803,089 A	9/1998	Ferre et al.
5,640,960 A	6/1997	Jones et al.	5,810,733 A	9/1998	Van Creveld et al.
5,644,612 A	7/1997	Moorman et al.	5,816,245 A	10/1998	Manseur et al.
5,645,065 A	7/1997	Shapiro et al.	5,817,022 A	10/1998	Vesely
5,651,047 A	7/1997	Moorman et al.	5,817,024 A	10/1998	Ogle et al.
5,654,864 A	8/1997	Ritter et al.	5,820,549 A	10/1998	Marian, Jr.
D383,968 S	9/1997	Bidwell et al.	5,824,031 A	10/1998	Cookston et al.
5,662,115 A	9/1997	Torp et al.	5,829,444 A	11/1998	Ferre et al.
5,665,477 A	9/1997	Meathrel et al.	5,830,145 A	11/1998	Tenhoff
5,666,473 A	9/1997	Wallace	5,831,260 A	11/1998	Hansen
5,666,958 A	9/1997	Rothenberg et al.	5,833,608 A	11/1998	Acker
5,668,888 A	9/1997	Doi et al.	5,833,622 A	11/1998	Meathrel et al.
5,669,383 A	9/1997	Johnson	5,835,561 A	11/1998	Moorman et al.
5,669,388 A	9/1997	Vilkomerson	5,836,882 A	11/1998	Frazin
5,676,159 A	10/1997	Navis	5,836,990 A	11/1998	Li
5,676,673 A	10/1997	Ferre et al.	5,840,024 A	11/1998	Taniguchi et al.
5,691,898 A	11/1997	Rosenberg et al.	5,840,025 A	11/1998	Ben-Haim
5,694,945 A	12/1997	Ben-Haim	5,840,030 A	11/1998	Ferek-Petric et al.
5,695,479 A	12/1997	Jagpal	5,840,031 A	11/1998	Crowley
5,697,377 A	12/1997	Wittkampf	5,842,986 A	12/1998	Avrin et al.
5,699,801 A	12/1997	Atalar et al.	5,843,076 A	12/1998	Webster, Jr. et al.
5,700,889 A	12/1997	Blair	5,843,153 A	12/1998	Johnston et al.
5,713,362 A	2/1998	Vilkomerson	5,844,140 A	12/1998	Seale
5,713,363 A	2/1998	Seward et al.	5,846,198 A	12/1998	Killmann
5,713,946 A	2/1998	Ben-Haim	5,855,553 A	1/1999	Tajima et al.
5,715,817 A	2/1998	Stevens-Wright et al.	5,855,558 A	1/1999	Nakao et al.
5,716,389 A	2/1998	Walinsky et al.	5,859,893 A	1/1999	Moorman et al.
5,718,241 A	2/1998	Ben-Haim et al.	5,865,748 A	2/1999	Co et al.
D391,838 S	3/1998	Bidwell et al.	5,868,673 A	2/1999	Vesely
5,722,412 A	3/1998	Pflugrath et al.	5,873,822 A	2/1999	Ferre et al.
5,727,550 A	3/1998	Montecalvo	5,876,328 A	3/1999	Fox et al.
5,727,552 A	3/1998	Ryan	5,879,297 A	3/1999	Haynor et al.
5,727,553 A	3/1998	Saad	5,893,363 A	4/1999	Little et al.
5,729,055 A	3/1998	Manning	5,897,495 A	4/1999	Aida et al.
5,729,129 A	3/1998	Acker	5,899,860 A	5/1999	Pfeiffer et al.
5,729,584 A	3/1998	Moorman et al.	5,902,238 A	5/1999	Golden et al.
5,730,129 A	3/1998	Darrow et al.	5,907,487 A	5/1999	Rosenberg et al.
5,731,996 A	3/1998	Gilbert	5,908,385 A	6/1999	Chechelski et al.
5,733,323 A	3/1998	Buck et al.	5,910,113 A	6/1999	Pruter
5,738,096 A	4/1998	Ben-Haim	5,910,120 A	6/1999	Kim et al.
5,738,099 A	4/1998	Chang	5,913,820 A	6/1999	Bladen et al.
5,740,808 A	4/1998	Panescu et al.	5,913,830 A	6/1999	Miles
5,742,394 A	4/1998	Hansen	5,919,141 A	7/1999	Money et al.
5,744,953 A	4/1998	Hansen	5,919,170 A	7/1999	Woessner
5,748,767 A	5/1998	Raab	5,928,145 A	7/1999	Ocali et al.
5,749,835 A	5/1998	Glantz	5,929,607 A	7/1999	Rosenberg et al.
5,749,938 A	5/1998	Coombs	5,931,786 A *	8/1999	Whitmore, III ..... A61B 8/12 600/459
			5,931,788 A	8/1999	Keen et al.
			5,931,818 A	8/1999	Werp et al.
			5,941,858 A	8/1999	Johnson
			5,941,889 A	8/1999	Cermak
			5,941,904 A	8/1999	Johnston et al.
			5,944,022 A	8/1999	Nardella et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

5,944,023 A	8/1999	Johnson et al.	6,172,499 B1	1/2001	Ashe
5,953,683 A	9/1999	Hansen et al.	6,173,199 B1	1/2001	Gabriel
5,957,857 A	9/1999	Hartley	6,173,715 B1	1/2001	Sinanan et al.
5,961,923 A	10/1999	Nova et al.	6,175,756 B1	1/2001	Ferre et al.
5,967,978 A	10/1999	Littmann et al.	6,176,829 B1	1/2001	Vilkomerson
5,967,980 A	10/1999	Ferre et al.	6,193,743 B1	2/2001	Brayton et al.
5,967,991 A	10/1999	Gardineer et al.	6,200,305 B1	3/2001	Berthiaume et al.
5,969,722 A	10/1999	Palm	6,203,498 B1	3/2001	Bunce et al.
5,978,705 A	11/1999	KenKnight et al.	6,203,499 B1	3/2001	Imling et al.
5,982,915 A	11/1999	Doi et al.	6,206,843 B1	3/2001	Iger et al.
5,983,126 A	11/1999	Wittkampf	6,208,884 B1	3/2001	Kumar et al.
5,984,908 A	11/1999	Davis et al.	6,211,626 B1	4/2001	Lys et al.
5,991,693 A	11/1999	Zalewski	6,211,666 B1	4/2001	Acker
5,997,473 A	12/1999	Taniguchi et al.	6,212,426 B1	4/2001	Swanson
5,997,481 A	12/1999	Adams et al.	6,216,027 B1	4/2001	Willis et al.
6,006,123 A	12/1999	Nguyen et al.	6,216,028 B1	4/2001	Haynor et al.
6,011,988 A	1/2000	Lynch et al.	6,216,029 B1	4/2001	Paltieli
6,014,473 A	1/2000	Hossack et al.	6,223,087 B1	4/2001	Williams
6,014,580 A	1/2000	Blume et al.	6,226,547 B1	5/2001	Lockhart et al.
6,015,414 A	1/2000	Werp et al.	6,230,046 B1	5/2001	Crane et al.
6,017,496 A	1/2000	Nova et al.	6,233,476 B1	5/2001	Strommer et al.
6,019,724 A	2/2000	Gronningsaeter et al.	6,233,479 B1	5/2001	Haddad et al.
6,019,725 A	2/2000	Vesely et al.	6,238,344 B1	5/2001	Gamelsky et al.
6,023,638 A	2/2000	Swanson	6,241,673 B1	6/2001	Williams
6,026,312 A	2/2000	Shemwell et al.	6,246,231 B1	6/2001	Ashe
6,031,765 A	2/2000	Lee et al.	6,246,898 B1	6/2001	Vesely et al.
6,032,070 A	2/2000	Flock et al.	6,248,072 B1	6/2001	Murkin
6,039,694 A	3/2000	Larson et al.	6,248,074 B1	6/2001	Ohno et al.
6,050,718 A	4/2000	Schena et al.	6,248,075 B1	6/2001	McGee et al.
6,052,610 A	4/2000	Koch	6,251,073 B1	6/2001	Imran et al.
6,052,618 A	4/2000	Dahlke et al.	6,253,770 B1	7/2001	Acker et al.
D424,693 S	5/2000	Pruter	6,259,941 B1	7/2001	Chia et al.
6,059,718 A	5/2000	Taniguchi et al.	6,261,231 B1	7/2001	Damphousse et al.
6,064,903 A	5/2000	Riechers et al.	6,263,230 B1	7/2001	Haynor et al.
6,064,905 A	5/2000	Webster, Jr. et al.	6,266,550 B1	7/2001	Selmon et al.
6,066,094 A	5/2000	Ben-Haim	6,266,551 B1	7/2001	Osadchy et al.
6,068,599 A	5/2000	Saito et al.	6,266,552 B1	7/2001	Slettenmark
6,073,043 A	6/2000	Schneider	6,266,563 B1	7/2001	KenKnight et al.
6,074,367 A	6/2000	Hubbell	6,271,833 B1	8/2001	Rosenberg et al.
6,075,442 A	6/2000	Welch	6,272,371 B1	8/2001	Shlomo
6,076,007 A	6/2000	England et al.	6,272,374 B1	8/2001	Flock et al.
6,080,108 A *	6/2000	Dunham	6,275,258 B1	8/2001	Chim
			6,275,724 B1	8/2001	Dickinson et al.
			6,277,077 B1	8/2001	Briskin et al.
			6,284,459 B1	9/2001	Nova et al.
			6,285,898 B1	9/2001	Ben-Haim
			6,288,704 B1	9/2001	Flack et al.
			6,292,678 B1	9/2001	Hall et al.
6,082,366 A	7/2000	Andra et al.	6,292,680 B1	9/2001	Somogyi et al.
6,083,170 A	7/2000	Ben-Haim	6,292,901 B1	9/2001	Lys et al.
6,099,524 A	8/2000	Lipson et al.	6,293,955 B1	9/2001	Houser et al.
6,100,026 A	8/2000	Nova et al.	6,296,604 B1	10/2001	Garibaldi et al.
6,102,044 A	8/2000	Naidyhorski	6,296,614 B1 *	10/2001	Pruter
6,106,472 A	8/2000	Chiang et al.			
6,107,699 A	8/2000	Swanson			
6,112,111 A	8/2000	Glantz	6,298,261 B1	10/2001	Rex
6,113,504 A	9/2000	Kuesters	6,304,768 B1	10/2001	Blume et al.
6,113,547 A	9/2000	Catallo et al.	6,306,097 B1	10/2001	Park et al.
6,115,624 A	9/2000	Lewis et al.	6,311,082 B1	10/2001	Creighton, IV et al.
6,117,085 A	9/2000	Picatti et al.	6,315,709 B1	11/2001	Garibaldi et al.
6,120,445 A	9/2000	Grunwald	6,315,727 B1	11/2001	Coleman et al.
6,126,608 A	10/2000	Kemme et al.	6,319,668 B1	11/2001	Nova et al.
6,128,174 A	10/2000	Ritter et al.	6,323,769 B1	11/2001	Dames et al.
6,129,668 A	10/2000	Haynor et al.	6,323,770 B1	11/2001	Dames et al.
6,132,378 A	10/2000	Marino	6,324,416 B1	11/2001	Seibert
6,132,379 A	10/2000	Patacsil et al.	6,325,540 B1	12/2001	Lounsberry et al.
6,135,961 A	10/2000	Pflugrath et al.	6,325,762 B1	12/2001	Tjin
6,136,274 A	10/2000	Nova et al.	6,329,139 B1	12/2001	Nova et al.
6,138,681 A	10/2000	Chen et al.	6,329,916 B1	12/2001	Dames et al.
6,139,496 A	10/2000	Chen et al.	6,330,467 B1	12/2001	Creighton, IV et al.
6,139,502 A	10/2000	Fredriksen	6,332,089 B1	12/2001	Acker et al.
6,142,946 A	11/2000	Hwang et al.	6,332,874 B1	12/2001	Eliassen et al.
6,144,300 A	11/2000	Dames et al.	6,340,588 B1	1/2002	Nova et al.
6,148,823 A	11/2000	Hastings	6,340,868 B1	1/2002	Lys et al.
6,152,933 A	11/2000	Werp et al.	6,341,231 B1	1/2002	Ferre et al.
6,157,853 A	12/2000	Blume et al.	6,346,081 B1	2/2002	Vilkomerson
6,165,144 A	12/2000	Talish et al.	6,348,911 B1	2/2002	Rosenberg et al.
6,166,496 A	12/2000	Lys et al.	6,350,160 B1	2/2002	Feuersanger et al.
6,166,806 A	12/2000	Tjin	6,352,363 B1	3/2002	Munger et al.
6,167,765 B1	1/2001	Weitzel	6,355,026 B1	3/2002	Mick

A61B 8/08  
600/459A61B 17/3403  
600/461

(56)

## References Cited

## U.S. PATENT DOCUMENTS

6,361,499 B1	3/2002	Bates et al.	6,529,761 B2	3/2003	Creighton, IV et al.
6,364,823 B1	4/2002	Garibaldi et al.	6,530,887 B1	3/2003	Gilbert et al.
6,364,839 B1	4/2002	Little et al.	6,534,982 B1	3/2003	Jakab
6,366,804 B1	4/2002	Mejia	6,535,625 B1	3/2003	Chang et al.
6,368,285 B1	4/2002	Osadchy et al.	6,537,192 B1	3/2003	Elliott et al.
6,370,411 B1	4/2002	Osadchy et al.	6,537,196 B1	3/2003	Creighton, IV et al.
6,373,240 B1	4/2002	Govari	6,538,634 B1	3/2003	Chui et al.
6,373,388 B1	4/2002	Dames et al.	6,540,685 B1	4/2003	Rhoads et al.
6,374,134 B1	4/2002	Bladen et al.	6,540,699 B1	4/2003	Smith et al.
6,374,670 B1	4/2002	Spelman et al.	6,542,766 B2	4/2003	Hall et al.
6,375,606 B1	4/2002	Garibaldi et al.	6,544,251 B1	4/2003	Crawford
6,375,639 B1	4/2002	Duplessie et al.	6,546,270 B1	4/2003	Goldin et al.
6,377,857 B1	4/2002	Brayton et al.	6,546,279 B1	4/2003	Bova et al.
6,379,302 B1	4/2002	Kessman et al.	6,546,787 B1	4/2003	Schiller et al.
6,379,303 B1	4/2002	Seitz et al.	6,549,794 B1	4/2003	Nadeau, Jr. et al.
6,379,307 B1 *	4/2002	Filly ..... A61B 8/0833	6,552,841 B1	4/2003	Lasser et al.
		600/461	6,556,858 B1	4/2003	Zeman
			6,562,019 B1	5/2003	Sell
6,381,485 B1	4/2002	Hunter et al.	6,564,087 B1	5/2003	Pitris et al.
6,383,139 B1	5/2002	Hwang et al.	6,569,101 B2	5/2003	Quistgaard et al.
6,385,472 B1	5/2002	Hall et al.	6,571,004 B1	5/2003	Florent et al.
6,385,476 B1	5/2002	Osadchy et al.	6,574,518 B1	6/2003	Lounsberry et al.
6,398,736 B1	6/2002	Seward	6,575,908 B2	6/2003	Barnes et al.
6,401,723 B1	6/2002	Garibaldi et al.	6,577,080 B2	6/2003	Lys et al.
6,406,442 B1	6/2002	McFann et al.	6,577,896 B2	6/2003	Werner et al.
6,412,978 B1	7/2002	Watanabe et al.	6,584,343 B1	6/2003	Ransbury et al.
6,412,980 B1	7/2002	Lounsberry et al.	6,593,754 B1	7/2003	Steber et al.
6,416,475 B1	7/2002	Hwang et al.	6,593,884 B1	7/2003	Gilboa et al.
6,417,839 B1	7/2002	Odell	6,596,791 B2	7/2003	Santar et al.
6,418,332 B1	7/2002	Mastrototaro et al.	6,597,943 B2	7/2003	Taha et al.
6,418,335 B2	7/2002	Avrin et al.	6,599,249 B1	7/2003	Nordgren et al.
6,423,002 B1	7/2002	Hossack	6,607,488 B1	8/2003	Jackson et al.
6,423,050 B1	7/2002	Twardowski	6,610,058 B2	8/2003	Flores
6,427,079 B1	7/2002	Schneider et al.	6,611,141 B1	8/2003	Schulz et al.
6,428,551 B1	8/2002	Hall et al.	6,615,071 B1	9/2003	Casscells, III et al.
6,430,315 B1	8/2002	Makram-Ebeid	6,615,155 B2	9/2003	Gilboa
6,432,069 B1	8/2002	Godo et al.	6,618,612 B1	9/2003	Acker et al.
6,436,050 B2	8/2002	Garrison et al.	6,626,832 B1	9/2003	Paltieli et al.
6,438,411 B1	8/2002	Guttman et al.	6,626,834 B2	9/2003	Dunne et al.
6,442,416 B1	8/2002	Schultz	6,626,902 B1	9/2003	Kucharczyk et al.
6,443,902 B1	9/2002	Sasady	6,630,879 B1	10/2003	Creighton, IV et al.
6,443,907 B1	9/2002	Mansy et al.	6,635,027 B1	10/2003	Cragg et al.
6,445,943 B1	9/2002	Ferre et al.	6,645,148 B2	11/2003	Nguyen-Dinh et al.
6,459,919 B1	10/2002	Lys et al.	6,648,875 B2	11/2003	Simpson et al.
6,463,121 B1	10/2002	Milnes	6,649,914 B1	11/2003	Moorman et al.
6,473,167 B1	10/2002	Odell	6,652,506 B2	11/2003	Bowe et al.
6,474,341 B1	11/2002	Hunter et al.	6,662,034 B2	12/2003	Segner et al.
6,475,146 B1	11/2002	Frelburger et al.	6,669,633 B2	12/2003	Brodsky et al.
6,475,152 B1	11/2002	Kelly, Jr. et al.	6,672,308 B1	1/2004	Gaspari
6,475,223 B1	11/2002	Werp et al.	6,677,752 B1	1/2004	Creighton, IV et al.
6,477,402 B1	11/2002	Lynch et al.	6,679,857 B1	1/2004	Bastia et al.
6,484,118 B1	11/2002	Govari et al.	6,684,176 B2	1/2004	Willins et al.
6,485,426 B2	11/2002	Sandhu	6,685,644 B2	2/2004	Seo
6,487,916 B1	12/2002	Gomm et al.	6,687,531 B1	2/2004	Ferre et al.
6,491,671 B1	12/2002	Larson, III et al.	6,689,119 B1	2/2004	Di Caprio et al.
6,493,573 B1	12/2002	Martinelli et al.	6,690,963 B2	2/2004	Ben-Haim et al.
6,496,715 B1	12/2002	Lee et al.	6,690,964 B2	2/2004	Bieger et al.
6,498,944 B1	12/2002	Ben-Haim et al.	6,690,968 B2	2/2004	Mejia
6,500,141 B1 *	12/2002	Irion et al. .... 604/22	6,694,167 B1	2/2004	Ferre et al.
6,505,062 B1	1/2003	Ritter et al.	6,695,786 B2	2/2004	Wang et al.
6,507,751 B2	1/2003	Blume et al.	6,701,179 B1	3/2004	Martinelli et al.
6,508,802 B1	1/2003	Rosengart et al.	6,701,918 B2	3/2004	Fariss et al.
6,512,958 B1	1/2003	Swoyer et al.	6,702,749 B2	3/2004	Paladini et al.
6,514,249 B1	2/2003	Maguire et al.	6,702,804 B1	3/2004	Ritter et al.
6,515,657 B1	2/2003	Zanelli	6,704,590 B2	3/2004	Haldeman
6,516,212 B1	2/2003	Bladen et al.	6,709,390 B1	3/2004	Marie Pop
6,516,231 B1	2/2003	Flammang	6,711,429 B1	3/2004	Gilboa et al.
6,516,807 B1	2/2003	Panescu et al.	6,711,431 B2	3/2004	Sarin et al.
6,517,491 B1	2/2003	Thiele et al.	6,719,698 B2	4/2004	Manor et al.
6,517,520 B2	2/2003	Chang et al.	6,719,699 B2	4/2004	Smith
6,522,906 B1	2/2003	Salisbury, Jr. et al.	6,719,724 B1	4/2004	Walker et al.
6,522,907 B1	2/2003	Bladen et al.	6,719,756 B1	4/2004	Muntermann
6,522,909 B1	2/2003	Garibaldi et al.	6,720,745 B2	4/2004	Lys et al.
6,524,303 B1	2/2003	Garibaldi	6,733,511 B2	5/2004	Hall et al.
6,528,954 B1	3/2003	Lys et al.	6,736,782 B2	5/2004	Pfeiffer et al.
6,528,991 B2	3/2003	Ashe	6,738,656 B1	5/2004	Ferre et al.
			6,740,103 B2	5/2004	Hall et al.
			6,743,177 B2	6/2004	Ito et al.
			6,746,402 B2	6/2004	Ustuner

(56)

## References Cited

## U.S. PATENT DOCUMENTS

6,754,596 B2	6/2004	Ashe	7,033,603 B2	4/2006	Nelson et al.
6,755,789 B2	6/2004	Stringer et al.	D520,139 S	5/2006	Chaggares
6,755,816 B2	6/2004	Ritter et al.	D520,140 S	5/2006	Chaggares
6,757,557 B1	6/2004	Bladen et al.	7,038,398 B1	5/2006	Lys et al.
6,763,261 B2	7/2004	Casscells, III et al.	7,038,657 B2	5/2006	Rosenberg et al.
6,764,449 B2	7/2004	Lee et al.	7,043,293 B1	5/2006	Baura
6,768,496 B2	7/2004	Bieger et al.	7,054,228 B1	5/2006	Hickling
6,772,001 B2	8/2004	Maschke et al.	7,066,914 B2	6/2006	Andersen
6,774,624 B2	8/2004	Anderson et al.	7,066,924 B1	6/2006	Garibaldi et al.
6,780,154 B2	8/2004	Hunt et al.	D525,363 S	7/2006	Chaggares
6,783,493 B2	8/2004	Chiang et al.	7,070,565 B2	7/2006	Vaezy et al.
6,783,536 B2	8/2004	Vilsmeier et al.	7,072,704 B2	7/2006	Bucholz
6,784,660 B2	8/2004	Ashe	7,082,325 B2	7/2006	Hashimshony et al.
6,785,571 B2	8/2004	Glossop et al.	7,090,639 B2	8/2006	Govari
6,786,219 B2	9/2004	Garibaldi et al.	7,096,148 B2	8/2006	Anderson et al.
6,788,967 B2	9/2004	Ben-Haim et al.	7,096,870 B2	8/2006	Lamprich et al.
6,794,667 B2	9/2004	Noshi	7,098,907 B2	8/2006	Houston et al.
6,799,066 B2	9/2004	Steines et al.	7,103,205 B2	9/2006	Wang et al.
6,814,704 B2	11/2004	Weilandt	7,104,980 B1	9/2006	Laherty et al.
6,815,651 B2	11/2004	Odell	7,106,043 B1	9/2006	Da Silva et al.
6,816,266 B2	11/2004	Varshneya et al.	7,106,431 B2	9/2006	Odell
6,817,364 B2	11/2004	Garibaldi	7,106,479 B2	9/2006	Roy et al.
6,832,199 B1	12/2004	Kucek et al.	7,107,105 B2	9/2006	Bjorklund et al.
6,834,201 B2	12/2004	Gillies et al.	7,132,804 B2	11/2006	Lys et al.
6,844,713 B2	1/2005	Steber et al.	7,137,976 B2	11/2006	Ritter et al.
6,845,142 B2	1/2005	Ohishi	7,141,812 B2	11/2006	Appleby et al.
6,856,823 B2	2/2005	Ashe	7,142,905 B2	11/2006	Slayton et al.
6,860,422 B2	3/2005	Hull et al.	7,148,970 B2	12/2006	de Boer
6,862,467 B2	3/2005	Moore et al.	7,153,291 B2	12/2006	Bierman
6,869,390 B2	3/2005	Elliott et al.	7,161,453 B2	1/2007	Creighton, IV
6,869,401 B2	3/2005	Gilbert et al.	7,162,291 B1	1/2007	Nachaliel
6,875,179 B2	4/2005	Ferguson et al.	7,167,738 B2	1/2007	Schweikard et al.
6,879,160 B2	4/2005	Jakab	7,169,107 B2	1/2007	Jersey-Willuhn et al.
6,884,219 B1	4/2005	Pruter	7,174,201 B2	2/2007	Govari et al.
6,889,091 B2	5/2005	Hine et al.	7,175,646 B2	2/2007	Brenneman et al.
6,895,268 B1	5/2005	Rahn et al.	7,180,252 B2	2/2007	Lys et al.
6,902,528 B1	6/2005	Garibaldi et al.	7,184,820 B2	2/2007	Jersey-Willuhn et al.
6,908,433 B1	6/2005	Pruter	7,189,198 B2	3/2007	Harburn et al.
6,911,026 B1	6/2005	Hall et al.	7,190,819 B2	3/2007	Viswanathan
6,923,782 B2	8/2005	O'Mahony et al.	7,194,295 B2	3/2007	Vilsmeier
6,926,673 B2	8/2005	Roberts et al.	7,204,798 B2	4/2007	Zdeblick et al.
6,934,575 B2	8/2005	Ferre et al.	7,206,064 B2	4/2007	Rogers et al.
6,936,010 B2	8/2005	Fang et al.	7,207,941 B2	4/2007	Sharf
6,940,379 B2	9/2005	Creighton	7,211,082 B2	5/2007	Hall et al.
6,941,166 B2	9/2005	MacAdam et al.	7,214,191 B2	5/2007	Stringer et al.
6,947,788 B2	9/2005	Gilboa et al.	7,215,326 B2	5/2007	Rosenberg
6,950,689 B1	9/2005	Willis et al.	7,221,104 B2	5/2007	Lys et al.
6,953,754 B2	10/2005	Machida et al.	7,223,256 B2	5/2007	Bierman
6,958,677 B1	10/2005	Carter	7,229,400 B2	6/2007	Elliott et al.
6,959,214 B2	10/2005	Pape et al.	7,231,243 B2	6/2007	Tearney et al.
6,962,566 B2	11/2005	Quistgaard et al.	7,236,157 B2	6/2007	Schena et al.
6,968,846 B2	11/2005	Viswanathan	7,236,816 B2	6/2007	Kumar et al.
6,969,352 B2	11/2005	Chiang et al.	7,237,313 B2	7/2007	Skujins et al.
6,975,197 B2	12/2005	Creighton, IV	7,241,267 B2	7/2007	Furia
6,976,962 B2	12/2005	Bullis	7,244,234 B2	7/2007	Ridley et al.
6,976,987 B2	12/2005	Flores	7,248,032 B1	7/2007	Hular et al.
6,980,843 B2	12/2005	Eng et al.	7,248,914 B2	7/2007	Hastings et al.
6,980,852 B2	12/2005	Jersey-Willuhn et al.	7,264,584 B2	9/2007	Ritter et al.
6,980,921 B2	12/2005	Anderson et al.	7,270,662 B2	9/2007	Visram et al.
6,986,739 B2	1/2006	Warren et al.	7,275,682 B2	10/2007	Excoffier et al.
6,999,821 B2	2/2006	Jenney et al.	7,276,044 B2	10/2007	Ferry et al.
7,001,355 B2	2/2006	Nunomura et al.	7,286,034 B2	10/2007	Creighton
7,008,418 B2	3/2006	Hall et al.	7,291,146 B2	11/2007	Steinke et al.
7,010,338 B2	3/2006	Ritter et al.	7,297,140 B2	11/2007	Orlu et al.
7,015,393 B2	3/2006	Weiner et al.	7,308,296 B2	12/2007	Lys et al.
7,017,584 B2	3/2006	Garibaldi et al.	7,310,150 B2	12/2007	Guillermo et al.
7,019,610 B2	3/2006	Creighton, IV et al.	7,321,228 B2	1/2008	Govari
7,020,512 B2	3/2006	Ritter et al.	7,322,990 B1	1/2008	Mark et al.
D518,574 S	4/2006	Chaggares	7,342,058 B2	3/2008	Peppmoller et al.
7,022,075 B2	4/2006	Grunwald et al.	D566,284 S	4/2008	Kitayama et al.
7,022,082 B2	4/2006	Sonek	7,355,716 B2	4/2008	de Boer et al.
7,026,927 B2	4/2006	Wright et al.	7,360,427 B2	4/2008	Drinkwater et al.
7,027,634 B2	4/2006	Odell	7,366,376 B2	4/2008	Shishkov et al.
7,028,387 B1	4/2006	Huynh et al.	7,366,562 B2	4/2008	Dukeshherer et al.
7,029,446 B2	4/2006	Wendelken et al.	7,366,563 B2	4/2008	Kleen et al.
			7,373,271 B1	5/2008	Schneider
			7,382,949 B2	6/2008	Bouma et al.
			7,418,169 B2	8/2008	Tearney et al.
			7,447,408 B2	11/2008	Bouma et al.

(56)		References Cited			
		U.S. PATENT DOCUMENTS			
7,452,331	B1	11/2008	Pruter	2002/0019447	A1
7,452,358	B2	11/2008	Stern et al.	2002/0022777	A1
D585,556	S	1/2009	Kosaku	2002/0032391	A1
7,479,141	B2	1/2009	Kleen et al.	2002/0038088	A1 *
7,534,223	B2	5/2009	Boutilette et al.		
7,538,859	B2	5/2009	Tearney et al.	2002/0055680	A1
7,547,282	B2	6/2009	Lo et al.	2002/0082559	A1
7,551,293	B2	6/2009	Yelin et al.	2002/0113555	A1
D599,909	S	9/2009	Rinott et al.	2002/0114518	A1
7,588,541	B2	9/2009	Floyd et al.	2002/0120193	A1
D603,050	S	10/2009	Chen	2002/0123679	A1
7,599,730	B2	10/2009	Hunter et al.	2002/0128554	A1
7,604,596	B2	10/2009	Hwang et al.	2002/0133079	A1
D603,520	S	11/2009	Ninomiya et al.	2002/0151789	A1
7,635,336	B1	12/2009	Pruter	2002/0156363	A1
7,637,163	B2	12/2009	Fetzer et al.	2002/0156376	A1
7,640,053	B2	12/2009	Verin	2002/0165448	A1
7,651,469	B2	1/2010	Osborne et al.	2002/0165534	A1
7,652,080	B2	1/2010	Peppmoller et al.	2002/0198568	A1
D609,814	S	2/2010	Banryu	2003/0002727	A1
7,665,893	B2	2/2010	Buchalter	2003/0009132	A1
7,668,583	B2	2/2010	Fegert et al.	2003/0011359	A1
7,670,294	B2	3/2010	Kisen et al.	2003/0013966	A1
7,686,766	B2	3/2010	Quistgaard et al.	2003/0018276	A1
7,691,066	B2 *	4/2010	Kosaku ..... A61B 8/0833 600/459	2003/0028113	A1
7,699,782	B2	4/2010	Angelsen et al.	2003/0036696	A1
7,727,192	B2	6/2010	Tokumoto et al.	2003/0040671	A1
7,740,586	B2	6/2010	Hwang et al.	2003/0072805	A1
7,751,865	B2	7/2010	Jascob et al.	2003/0073894	A1
7,766,839	B2	8/2010	Rogers et al.	2003/0076281	A1
7,774,051	B2	8/2010	Voth	2003/0083698	A1
7,794,407	B2	9/2010	Rothenberg	2003/0088195	A1
7,798,970	B2	9/2010	Lo et al.	2003/0100849	A1
7,819,807	B2	10/2010	Barnes et al.	2003/0114742	A1
7,819,810	B2	10/2010	Stringer et al.	2003/0114777	A1
7,837,627	B1	11/2010	Pruter	2003/0120150	A1
D629,526	S	12/2010	Ladwig et al.	2003/0120154	A1
D629,527	S	12/2010	Crunkilton	2003/0139661	A1
7,846,103	B2 *	12/2010	Cannon, Jr. .... A61B 17/3403 600/437	2003/0139664	A1
7,850,613	B2	12/2010	Stribling	2003/0149328	A1
D630,756	S	1/2011	Kitayama	2003/0149359	A1
D630,757	S	1/2011	Kitayama	2003/0152290	A1
7,909,815	B2	3/2011	Whitmore, III et al.	2003/0158482	A1
7,931,596	B2	4/2011	Rachlin et al.	2003/0160721	A1
7,976,469	B2	7/2011	Bonde et al.	2003/0163037	A1
7,998,073	B2	8/2011	Roth et al.	2003/0171681	A1 *
8,052,606	B2	11/2011	Barnes et al.		
8,073,529	B2	12/2011	Cermak et al.	2003/0171691	A1
8,118,743	B2	2/2012	Park et al.	2003/0173953	A1
8,137,281	B2	3/2012	Huang et al.	2003/0176787	A1
8,147,408	B2	4/2012	Bunce et al.	2003/0184544	A1
8,216,146	B2	7/2012	Hwang et al.	2003/0191392	A1
8,257,264	B2	9/2012	Park et al.	2003/0191460	A1
8,353,840	B1 *	1/2013	Pruter ..... A61B 8/0833 24/327	2003/0195418	A1
8,388,541	B2	3/2013	Messerly et al.	2003/0195420	A1
8,388,546	B2	3/2013	Rothenberg	2003/0199746	A1
8,430,889	B2	4/2013	Zeng et al.	2003/0208142	A1
8,437,833	B2	5/2013	Silverstein	2003/0216639	A1
8,449,531	B2	5/2013	Whitmore, III et al.	2003/0220557	A1
D684,265	S	6/2013	Cadera	2003/0220578	A1
8,478,382	B2	7/2013	Burnside et al.	2003/0229298	A1
8,496,592	B2	7/2013	Ridley et al.	2003/0233042	A1
8,496,593	B2	7/2013	Park et al.	2004/0015070	A1
8,512,256	B2	8/2013	Rothenberg	2004/0015079	A1
8,801,693	B2	8/2014	He et al.	2004/0024301	A1
D724,745	S	3/2015	Orome et al.	2004/0030319	A1
D727,495	S *	4/2015	Bown ..... A61B 8/4444 D24/130	2004/0043688	A1
10,022,147	B2 *	7/2018	Lee ..... A61B 8/4209	2004/0054278	A1
2001/0053915	A1 *	12/2001	Grossman ..... A61B 90/13 606/130	2004/0059226	A1
				2004/0082916	A1
				2004/0087877	A1
				2004/0088136	A1
				2004/0097803	A1
				2004/0097804	A1
				2004/0097805	A1
				2004/0097806	A1
				2004/0116809	A1
				2004/0127805	A1
				2004/0131998	A1
				2/2002	Renn et al.
				2/2002	Crieghton et al.
				3/2002	McFann et al.
				3/2002	Imran ..... A61B 8/08 600/443
				5/2002	Miele et al.
				6/2002	Chang et al.
				8/2002	Lys et al.
				8/2002	Wilt
				8/2002	Chiang et al.
				9/2002	Dominguez
				9/2002	Seward
				9/2002	Sandhu
				10/2002	Mansy et al.
				10/2002	Hunter et al.
				10/2002	Wang et al.
				11/2002	Ben-Haim et al.
				11/2002	Hayzelden et al.
				12/2002	Hafer et al.
				1/2003	MacMahon
				1/2003	Schwartz et al.
				1/2003	Ashe
				1/2003	Barnes et al.
				1/2003	Mansy et al.
				2/2003	Gilbert et al.
				2/2003	Willis et al.
				2/2003	Somogyi et al.
				4/2003	Miyazawa et al.
				4/2003	Chiang et al.
				4/2003	Morgan et al.
				5/2003	Whitehurst et al.
				5/2003	Vardi et al.
				5/2003	Jang
				6/2003	Lewkowicz et al.
				6/2003	Griffin et al.
				6/2003	Govari
				6/2003	Sauer et al.
				7/2003	Kimchy et al.
				7/2003	Hunt et al.
				8/2003	Elliott et al.
				8/2003	Smith
				8/2003	Odell
				8/2003	Poland et al.
				8/2003	Gilboa et al.
				8/2003	Bladen et al.
				9/2003	Weilandt ..... A61B 17/3403 600/464
				9/2003	Casscells et al.
				9/2003	Ashe
				9/2003	Gilbert et al.
				10/2003	Prudent
				10/2003	Haldeman
				10/2003	Hobbs et al.
				10/2003	Barnes et al.
				10/2003	Mendlein et al.
				10/2003	Fuimaono et al.
				11/2003	Boudewijn et al.
				11/2003	Gilboa et al.
				11/2003	Cleary et al.
				11/2003	Ho et al.
				12/2003	Iwami et al.
				12/2003	Ashe
				1/2004	Liang et al.
				1/2004	Berger et al.
				2/2004	Hockett et al.
				2/2004	Korkor et al.
				3/2004	Soerens et al.
				3/2004	Kimchy et al.
				3/2004	Peszynski et al.
				4/2004	Jenkins
				5/2004	Besz et al.
				5/2004	Ashe
				5/2004	Panescu
				5/2004	Sobe
				5/2004	Verard et al.
				5/2004	Hunter et al.
				6/2004	Chow et al.
				7/2004	MacAdam et al.
				7/2004	Marom et al.



(56)

## References Cited

## U.S. PATENT DOCUMENTS

2004/0133111 A1 *	7/2004	Szczzech et al. ....	600/461	2006/0025684 A1	2/2006	Quistgaard et al.	
2004/0133130 A1	7/2004	Ferry et al.		2006/0058633 A1	3/2006	Hoshino et al.	
2004/0135069 A1	7/2004	Odell		2006/0068074 A1	3/2006	Stefandl	
2004/0138564 A1	7/2004	Hwang et al.		2006/0084867 A1	4/2006	Tremblay et al.	
2004/0138570 A1	7/2004	Nita et al.		2006/0116571 A1	6/2006	Maschke et al.	
2004/0147837 A1	7/2004	Macaulay et al.		2006/0116578 A1	6/2006	Grunwald et al.	
2004/0150963 A1	8/2004	Holmberg et al.		2006/0149134 A1	7/2006	Soper et al.	
2004/0152972 A1	8/2004	Hunter		2006/0173329 A1	8/2006	Irioka et al.	
2004/0155609 A1	8/2004	Lys et al.		2006/0173407 A1	8/2006	Shaughnessy et al.	
2004/0158140 A1	8/2004	Fuimaono et al.		2006/0176242 A1	8/2006	Jaramaz et al.	
2004/0171924 A1	9/2004	Mire et al.		2006/0184074 A1	8/2006	Vaezy et al.	
2004/0176688 A1	9/2004	Haldeman		2006/0188487 A1	8/2006	Thomas et al.	
2004/0186461 A1	9/2004	DiMatteo		2006/0206037 A1	9/2006	Braxton	
2004/0199069 A1	10/2004	Connelly et al.		2006/0211944 A1	9/2006	Mauge et al.	
2004/0210289 A1	10/2004	Wang et al.		2006/0224188 A1	10/2006	Libbus et al.	
2004/0230271 A1	11/2004	Wang et al.		2006/0247746 A1	11/2006	Danek et al.	
2004/0231065 A1	11/2004	Daniel et al.		2006/0264756 A1 *	11/2006	Lo et al. ....	600/459
2004/0234453 A1	11/2004	Smith		2006/0276867 A1	12/2006	Viswanathan	
2004/0253365 A1	12/2004	Warren et al.		2007/0010753 A1	1/2007	MacAdam	
2004/0254470 A1	12/2004	Drinkwater et al.		2007/0016007 A1	1/2007	Govari et al.	
2004/0260174 A1	12/2004	Keene		2007/0016013 A1	1/2007	Camus	
2004/0267086 A1	12/2004	Anstadt et al.		2007/0016068 A1	1/2007	Grunwald et al.	
2005/0004450 A1	1/2005	Ben-Haim et al.		2007/0016069 A1	1/2007	Grunwald et al.	
2005/0021019 A1	1/2005	Hashimshony et al.		2007/0016070 A1	1/2007	Grunwald et al.	
2005/0033150 A1	2/2005	Takahashi et al.		2007/0016072 A1	1/2007	Grunwald et al.	
2005/0033177 A1 *	2/2005	Rogers et al. ....	600/455	2007/0049822 A1	3/2007	Bunce et al.	
2005/0035014 A1 *	2/2005	Cane .....	A61M 5/158 206/365	2007/0049846 A1	3/2007	Bown et al.	
2005/0038355 A1	2/2005	Gellman et al.		2007/0055141 A1	3/2007	Kruger et al.	
2005/0049486 A1	3/2005	Urquhart et al.		2007/0055142 A1	3/2007	Webler	
2005/0049510 A1	3/2005	Haldeman et al.		2007/0060992 A1	3/2007	Pappone	
2005/0063194 A1	3/2005	Lys et al.		2007/0062544 A1	3/2007	Rauk Bergstrom et al.	
2005/0070788 A1	3/2005	Wilson et al.		2007/0073155 A1	3/2007	Park et al.	
2005/0075561 A1	4/2005	Golden		2007/0087038 A1	4/2007	Richardson et al.	
2005/0085716 A1	4/2005	Hamm et al.		2007/0093710 A1	4/2007	Maschke	
2005/0085718 A1	4/2005	Shahidi		2007/0100285 A1	5/2007	Griffin et al.	
2005/0085720 A1	4/2005	Jascob et al.		2007/0112282 A1	5/2007	Skujins et al.	
2005/0101868 A1 *	5/2005	Ridley .....	A61B 8/0833 600/459	2007/0123769 A1	5/2007	Fuller et al.	
2005/0101869 A1	5/2005	Burba et al.		2007/0123805 A1	5/2007	Shireman et al.	
2005/0105081 A1	5/2005	Odell		2007/0129770 A1	6/2007	Younis	
2005/0105101 A1	5/2005	Duling et al.		2007/0135803 A1	6/2007	Belson	
2005/0112135 A1	5/2005	Cormier et al.		2007/0135886 A1	6/2007	Maschke	
2005/0113669 A1	5/2005	Helfer et al.		2007/0156205 A1	7/2007	Larson et al.	
2005/0113676 A1	5/2005	Weiner et al.		2007/0161904 A1	7/2007	Urbano	
2005/0113700 A1	5/2005	Yanagihara et al.		2007/0161915 A1	7/2007	Desai	
2005/0113873 A1	5/2005	Weiner et al.		2007/0167738 A1	7/2007	Timinger et al.	
2005/0113874 A1	5/2005	Connelly et al.		2007/0167801 A1	7/2007	Webler et al.	
2005/0113876 A1	5/2005	Weiner et al.		2007/0167808 A1	7/2007	Nozaki	
2005/0131291 A1 *	6/2005	Floyd et al. ....	600/424	2007/0167817 A1	7/2007	Huang et al.	
2005/0149002 A1	7/2005	Wang et al.		2007/0167997 A1	7/2007	Forsberg et al.	
2005/0151489 A1	7/2005	Lys et al.		2007/0197905 A1	8/2007	Timinger et al.	
2005/0154308 A1	7/2005	Quistgaard et al.		2007/0208255 A1	9/2007	Ridley et al.	
2005/0159644 A1	7/2005	Takano		2007/0225589 A1	9/2007	Viswanathan	
2005/0159790 A1	7/2005	Shalev		2007/0225610 A1	9/2007	Mickley et al.	
2005/0165301 A1	7/2005	Smith et al.		2007/0232882 A1	10/2007	Glossop et al.	
2005/0165313 A1	7/2005	Byron et al.		2007/0232910 A1	10/2007	Hwang et al.	
2005/0175665 A1	8/2005	Hunter et al.		2007/0238984 A1	10/2007	Maschke et al.	
2005/0175703 A1	8/2005	Hunter et al.		2007/0239018 A1	10/2007	Fetzer et al.	
2005/0178395 A1	8/2005	Hunter et al.		2007/0244413 A1	10/2007	Biggins	
2005/0178396 A1	8/2005	Hunter et al.		2007/0247454 A1	10/2007	Rahn et al.	
2005/0182295 A1	8/2005	Soper et al.		2007/0249911 A1	10/2007	Simon	
2005/0203368 A1	9/2005	Verin		2007/0265526 A1	11/2007	Govari et al.	
2005/0203396 A1	9/2005	Angelsen et al.		2007/0276241 A1 *	11/2007	Park .....	A61B 8/00 600/437
2005/0205081 A1	9/2005	Barker et al.		2007/0280974 A1	12/2007	Son et al.	
2005/0215901 A1	9/2005	Anderson et al.		2007/0282196 A1	12/2007	Birk et al.	
2005/0215945 A1	9/2005	Harris et al.		2007/0282197 A1	12/2007	Bill et al.	
2005/0222532 A1	10/2005	Bertolero et al.		2007/0299352 A1	12/2007	Harlev et al.	
2005/0228281 A1	10/2005	Nefos		2008/0008745 A1	1/2008	Stinchcomb et al.	
2005/0240102 A1 *	10/2005	Rachlin .....	A61B 8/10 600/437	2008/0009720 A1	1/2008	Schefelker et al.	
2005/0256398 A1	11/2005	Hastings et al.		2008/0009743 A1	1/2008	Hayasaka	
2005/0256541 A1	11/2005	Stypulkowski		2008/0015442 A1 *	1/2008	Watson .....	A61B 8/0841 600/459
2006/0015003 A1	1/2006	Moaddes et al.		2008/0027320 A1	1/2008	Bolorforosh et al.	
2006/0025677 A1	2/2006	Verard et al.		2008/0045908 A1	2/2008	Gould et al.	
				2008/0051626 A1	2/2008	Sato et al.	
				2008/0081958 A1	4/2008	Denison et al.	
				2008/0082136 A1	4/2008	Gaudiani	
				2008/0097232 A1	4/2008	Rothenberg	
				2008/0108949 A1	5/2008	Beasley et al.	

(56)

## References Cited

## U.S. PATENT DOCUMENTS

2008/0110261 A1 5/2008 Randall et al.  
 2008/0110263 A1 5/2008 Klessel et al.  
 2008/0110266 A1 5/2008 Randall et al.  
 2008/0112265 A1 5/2008 Urbano et al.  
 2008/0114095 A1 5/2008 Peppmoller et al.  
 2008/0114239 A1 5/2008 Randall et al.  
 2008/0114241 A1 5/2008 Randall et al.  
 2008/0114246 A1 5/2008 Randall et al.  
 2008/0114247 A1 5/2008 Urbano et al.  
 2008/0114248 A1 5/2008 Urbano et al.  
 2008/0114249 A1 5/2008 Randall et al.  
 2008/0114250 A1 5/2008 Urbano et al.  
 2008/0114251 A1 5/2008 Weymer et al.  
 2008/0114252 A1 5/2008 Randall et al.  
 2008/0114253 A1 5/2008 Randall et al.  
 2008/0114370 A1\* 5/2008 Schoenefeld ..... 606/96  
 2008/0119737 A1 5/2008 Urbano et al.  
 2008/0125772 A1 5/2008 Stone et al.  
 2008/0139944 A1 6/2008 Weymer et al.  
 2008/0146939 A1 6/2008 McMorrow et al.  
 2008/0146940 A1 6/2008 Jenkins et al.  
 2008/0152204 A1 6/2008 Huo et al.  
 2008/0154100 A1 6/2008 Thalmeier et al.  
 2008/0166453 A1 7/2008 Steele et al.  
 2008/0171934 A1 7/2008 Greenan et al.  
 2008/0183075 A1 7/2008 Govari et al.  
 2008/0188747 A1 8/2008 Randall et al.  
 2008/0188750 A1 8/2008 Randall et al.  
 2008/0188752 A1 8/2008 Randall et al.  
 2008/0200754 A1 8/2008 Buchalter  
 2008/0208060 A1\* 8/2008 Murkin ..... A61B 8/06  
 600/459  
 2008/0228082 A1 9/2008 Scheirer et al.  
 2008/0255404 A1 10/2008 Nogawa et al.  
 2008/0255475 A1 10/2008 Kondrosky et al.  
 2008/0275765 A1 11/2008 Kuchar  
 2008/0281206 A1 11/2008 Bartlett et al.  
 2008/0319311 A1 12/2008 Hamadeh  
 2009/0005675 A1 1/2009 Grunwald et al.  
 2009/0018497 A1 1/2009 Birchard et al.  
 2009/0018574 A1\* 1/2009 Martin ..... 606/213  
 2009/0024018 A1 1/2009 Boyden et al.  
 2009/0036774 A1\* 2/2009 Weng et al. .... 600/439  
 2009/0036790 A1 2/2009 Landesberg et al.  
 2009/0043205 A1 2/2009 Pelissier et al.  
 2009/0076327 A1 3/2009 Ohki  
 2009/0082661 A1 3/2009 Saladin et al.  
 2009/0084382 A1 4/2009 Jalde et al.  
 2009/0101577 A1 4/2009 Fulkerson et al.  
 2009/0118612 A1 5/2009 Grunwald et al.  
 2009/0118706 A1 5/2009 Schweikert et al.  
 2009/0124901 A1 5/2009 Fink et al.  
 2009/0136099 A1 5/2009 Boyden et al.  
 2009/0143736 A1 6/2009 Mittermeyer et al.  
 2009/0149748 A1 6/2009 Lenhardt et al.  
 2009/0156926 A1 6/2009 Messerly et al.  
 2009/0163810 A1 6/2009 Kanade et al.  
 2009/0171217 A1 7/2009 Kim et al.  
 2009/0171219 A1 7/2009 Uchibori  
 2009/0177083 A1\* 7/2009 Matsumura ..... A61B 8/08  
 600/437  
 2009/0177090 A1 7/2009 Grunwald et al.  
 2009/0177092 A1 7/2009 Riechers et al.  
 2009/0203989 A1 8/2009 Burnside et al.  
 2009/0204113 A1 8/2009 MacAdam et al.  
 2009/0209950 A1 8/2009 Starksen  
 2009/0227952 A1 9/2009 Blakstvedt et al.  
 2009/0234328 A1 9/2009 Cox et al.  
 2009/0258171 A1 10/2009 Uang  
 2009/0259124 A1 10/2009 Rothenberg  
 2009/0262982 A1 10/2009 Markowitz et al.  
 2009/0270722 A1 10/2009 Floyd et al.  
 2009/0275828 A1 11/2009 Shachar et al.  
 2009/0275833 A1 11/2009 Ikeda et al.  
 2009/0297441 A1 12/2009 Canham et al.

2010/0004543 A1 1/2010 Ahlund et al.  
 2010/0004547 A1 1/2010 Scholz et al.  
 2010/0016726 A1 1/2010 Meier  
 2010/0036227 A1 2/2010 Cox et al.  
 2010/0049062 A1 2/2010 Ziv  
 2010/0055153 A1 3/2010 Majmudar  
 2010/0055184 A1 3/2010 Zeitels et al.  
 2010/0057157 A1 3/2010 Govari et al.  
 2010/0060472 A1 3/2010 Kimura et al.  
 2010/0083719 A1 4/2010 Peppmoller et al.  
 2010/0094116 A1 4/2010 Silverstein  
 2010/0106011 A1 4/2010 Byrd et al.  
 2010/0114573 A1 5/2010 Huang et al.  
 2010/0126149 A1 5/2010 Kondou  
 2010/0143119 A1 6/2010 Kooijman et al.  
 2010/0179429 A1 7/2010 Ho et al.  
 2010/0185097 A1 7/2010 Hall  
 2010/0198048 A1 8/2010 Togawa  
 2010/0204569 A1 8/2010 Burnside et al.  
 2010/0217116 A1 8/2010 Eck et al.  
 2010/0222663 A1 9/2010 Wilder et al.  
 2010/0222664 A1 9/2010 Lemon et al.  
 2010/0234733 A1 9/2010 Wahlheim  
 2010/0249598 A1 9/2010 Smith et al.  
 2010/0258033 A1 10/2010 Yang et al.  
 2010/0273895 A1 10/2010 Stinchcomb et al.  
 2010/0298702 A1 11/2010 Rogers et al.  
 2010/0312121 A1\* 12/2010 Guan ..... A61B 8/0833  
 600/461  
 2010/0317981 A1 12/2010 Grunwald  
 2010/0318026 A1 12/2010 Grunwald  
 2010/0331712 A1 12/2010 Rothenberg  
 2011/0015527 A1 1/2011 Heasty et al.  
 2011/0015533 A1 1/2011 Cox et al.  
 2011/0040186 A1 2/2011 Matsumura  
 2011/0040187 A1 2/2011 Matsumura  
 2011/0040212 A1 2/2011 Dietz et al.  
 2011/0052694 A1 3/2011 Stinchcomb et al.  
 2011/0060215 A1 3/2011 Tupin, Jr. et al.  
 2011/0087107 A1 4/2011 Lindekugel et al.  
 2011/0087117 A1 4/2011 Tremper et al.  
 2011/0171286 A1 7/2011 Cecile et al.  
 2011/0196248 A1 8/2011 Grunwald  
 2011/0202123 A1\* 8/2011 Bonutti ..... A61F 2/958  
 623/1.11  
 2011/0278500 A1 11/2011 Bergeron  
 2011/0282188 A1 11/2011 Burnside et al.  
 2011/0295108 A1 12/2011 Cox et al.  
 2011/0313293 A1 12/2011 Lindekugel et al.  
 2012/0046562 A1 2/2012 Powers et al.  
 2012/0059270 A1 3/2012 Grunwald  
 2012/0095319 A1 4/2012 Kondrosky et al.  
 2012/0108950 A1 5/2012 He et al.  
 2012/0143029 A1 6/2012 Silverstein et al.  
 2012/0165679 A1 6/2012 Orome et al.  
 2012/0220854 A1 8/2012 Messerly et al.  
 2013/0006102 A1 1/2013 Wilkes et al.  
 2013/0060116 A1 3/2013 Messerly et al.  
 2013/0085391 A1 4/2013 Matsumura et al.  
 2013/0116571 A1 5/2013 Cox et al.  
 2013/0123597 A1 5/2013 Rothenberg  
 2013/0131704 A1 5/2013 Pechoux  
 2013/0245488 A1 9/2013 Quinn et al.  
 2013/0338503 A1 12/2013 Cohen et al.  
 2014/0180116 A1 6/2014 Lindekugel et al.  
 2015/0314104 A1\* 11/2015 Almansouri ..... A61M 25/0606  
 128/845

## FOREIGN PATENT DOCUMENTS

AU 20009592 9/2000  
 AU 20015250 6/2001  
 AU 768362 B2 12/2003  
 AU 2001229024 B2 9/2005  
 AU 2001283703 B2 5/2006  
 AU 2006202149 6/2006  
 AU 2006904933 9/2006  
 AU 2006283022 B2 2/2012  
 CA 2420676 2/2002

(56)

## References Cited

## FOREIGN PATENT DOCUMENTS

CN 1672649 A 9/2005  
 CN 101390754 A 3/2009  
 CN 102014757 A 4/2011  
 CN 102209490 A 10/2011  
 CN 102802514 A 11/2012  
 CN 102821679 A 12/2012  
 CN 103037761 A 4/2013  
 CN 103037762 A 4/2013  
 CN 103118591 A 5/2013  
 CN 103228219 A 7/2013  
 DE 4319033 C1 6/1994  
 DE 9404028 U1 8/1994  
 EP 0359697 3/1990  
 EP 0362821 4/1990  
 EP 0399536 A1 11/1990  
 EP 0815793 A2 1/1998  
 EP 0823261 A2 2/1998  
 EP 0928976 A2 7/1999  
 EP 1311226 A1 5/2003  
 EP 1504713 A1 2/2005  
 EP 2313143 A1 4/2011  
 EP 2440122 A1 4/2012  
 EP 2464407 A2 6/2012  
 EP 2482719 A1 8/2012  
 EP 2575610 A1 4/2013  
 EP 2575611 A1 4/2013  
 EP 2603145 A2 6/2013  
 EP 2605699 A2 6/2013  
 FR 2545349 11/1984  
 JP 01097440 4/1989  
 JP H02 13439 A 1/1990  
 JP 03023853 A 1/1991  
 JP 03173542 A 7/1991  
 JP 4090741 8/1992  
 JP 9-503054 3/1997  
 JP 09-094298 A 4/1997  
 JP 10043310 2/1998  
 JP 10290839 A 11/1998  
 JP 11128237 A 5/1999  
 JP 2001161683 6/2001  
 JP 2001340334 12/2001  
 JP 2003501127 A 1/2003  
 JP 2003061752 A 3/2003  
 JP 2003299654 10/2003  
 JP 2003334191 11/2003  
 JP 2002520893 2/2004  
 JP 2004505748 T 2/2004  
 JP 2004515298 A 5/2004  
 JP 2004-313271 A 11/2004  
 JP 2006508744 A 3/2006  
 JP 5010604 6/2012  
 JP 2012-529929 11/2012  
 JP 2013-518676 A 5/2013  
 JP 2013-535301 A 9/2013  
 WO 9112836 A1 9/1991  
 WO 1992003090 3/1992  
 WO 1994003159 A1 2/1994  
 WO 1994004938 3/1994  
 WO 1996005768 A1 2/1996  
 WO 1996007352 A1 3/1996  
 WO 1996041119 12/1996  
 WO 1997029683 A1 8/1997  
 WO 1997043989 A1 11/1997  
 WO 199916495 A1 4/1999  
 WO 9949407 A1 9/1999  
 WO 2000019906 4/2000  
 WO 2000040155 7/2000  
 WO 2000074775 A1 12/2000  
 WO 2001076479 A1 10/2001  
 WO 2002015973 A1 2/2002  
 WO 2002025277 A1 3/2002  
 WO 2003061752 7/2003  
 WO 2003077759 A1 9/2003  
 WO 2004049970 A2 6/2004  
 WO 2005033524 A1 4/2005

WO 2005033574 A1 4/2005  
 WO 2005117690 A1 12/2005  
 WO 2006074509 A1 7/2006  
 WO 2006074510 A1 7/2006  
 WO 2006078677 A2 7/2006  
 WO 2006103661 A2 10/2006  
 WO 2006111056 A1 10/2006  
 WO 2007002541 A2 1/2007  
 WO 2007005976 A1 1/2007  
 WO 2007014447 A1 2/2007  
 WO 2007034196 A2 3/2007  
 WO 2007067324 A1 6/2007  
 WO 2007069168 A2 6/2007  
 WO 2007109123 A2 9/2007  
 WO 2007126536 A2 11/2007  
 WO 2007144894 A1 12/2007  
 WO 2008005480 A1 1/2008  
 WO 2008024515 A2 2/2008  
 WO 2008024596 A2 2/2008  
 WO 2008028253 3/2008  
 WO 2008083111 7/2008  
 WO 2008118992 A1 10/2008  
 WO 2008126074 A2 10/2008  
 WO 2008131017 A2 10/2008  
 WO 2008136008 A2 11/2008  
 WO 2009002514 A2 12/2008  
 WO 2009009064 A1 1/2009  
 WO 2009057774 A1 5/2009  
 WO 2009070616 A2 6/2009  
 WO 2009100158 A1 8/2009  
 WO 2009123819 A2 10/2009  
 WO 2009126340 A1 10/2009  
 WO 2009129475 A1 10/2009  
 WO 2009129477 A1 10/2009  
 WO 2009134605 A2 11/2009  
 WO 2009137262 A2 11/2009  
 WO 2010002313 A1 1/2010  
 WO 2010018500 A1 2/2010  
 WO 2010022370 A1 2/2010  
 WO 2010027349 A1 3/2010  
 WO 2010027471 A2 3/2010  
 WO 2010030820 A1 3/2010  
 WO 2010132857 A1 11/2010  
 WO 2010143196 A1 12/2010  
 WO 2010144922 A1 12/2010  
 WO 2011019760 A2 2/2011  
 WO 2011041450 A1 4/2011  
 WO 2011044421 A1 4/2011  
 WO 2011051406 A1 5/2011  
 WO 2011064209 A1 6/2011  
 WO 2011084593 A2 7/2011  
 WO 2011097312 A1 8/2011  
 WO 2011128052 A2 10/2011  
 WO 2011150358 A1 12/2011  
 WO 2012021542 A2 2/2012  
 WO 2012024577 A2 2/2012  
 WO 2012058461 A1 5/2012  
 WO 2012060562 A2 5/2012  
 WO 2012083245 A1 6/2012  
 WO 2012088535 A1 6/2012  
 WO 2013006817 A1 1/2013  
 WO 2013070775 A1 5/2013  
 WO 2013188833 A2 12/2013  
 WO 2014134171 A1 9/2014

## OTHER PUBLICATIONS

Frassinelli, P et al, Utility of Chest Radiographs after Guidewire Exchanges of Central Venous Catheters, Crit Care Med, pp. 611-615, vol. 26 No. 3, Mar. 1998.  
 Frazin L et al, A Doppler Guided Retrograde Catheterization System, Cathet. Cardiovasc Diagn, pp. 41-50, May 1992.  
 French, PJ et al, Sensors for Catheter Applications, Sensors Update, vol. 13 Issue 1 pp. 107-153, Dec. 2003.  
 GB Application 0800474.9 filed Aug. 24, 2006 Office Action dated Aug. 9, 2010.  
 GB Application 0800474.9 filed Aug. 24, 2006 Office Action dated Mar. 17, 2010.

(56)

## References Cited

## OTHER PUBLICATIONS

- Gebauer, B et al, Ultrasound and Fluoroscopy-guided Implantation of Peripherally Inserted Central Venous Catheters (PICCs), ROFO, pp. 386-391, vol. 176 No. 3, Mar. 2004 (Abstract only).
- Gebhard, et al., "The accuracy of Electrocardiogram-Controlled Central Line Placement." The International Anesthesia Research Society, vol. 104, No. 1 Jan. 2007.
- Gladwin, MT et al, Cannulation of the Internal Jugular Vein: is postprocedural chest radiography always necessary?, Crit Care Med, 33 pages, Oct. 2000.
- Gonzales, et al. "Peripherally Inserted Central Catheter Placement in Swine Using Magnet Detection." Journal of Intravenous Nursing, vol. 22, No. 3, May/Jun. 1999.
- Greenall, M.J. et al, Cardiac Tamponade and Central Venous Catheters, British Medical Journal, pp. 595-597, Jun. 14, 1975.
- Guillory, "Basic Principles of Technologies for Catheter Localization." C.R. Bard internal paper, Oct. 20, 2004.
- Guth, AA, Routine Chest X-rays after Insertion of Implantable Long-Term Venous Catheters: Necessary or Not?, Am Surg, pp. 26-29, vol. 67 No. 1, Jan. 2001 (Abstract only).
- Hill, Bradley, Identifying the Caval-Atrial Junction Using Smart-Catheter Technology presentation, 22nd Annual Scientific Meeting of the AVA in Savannah, Georgia, Sep. 13, 2008.
- Hoffman, Thomas et al, Simultaneous Measurement of Pulmonary Venous Flow by Intravascular Catheter Doppler Velocimetry and Transesophageal Doppler Echocardiography: Relation to Left Atrial Pressure and Left Atrial and Left Ventricular Function, pp. 239-249, J Am Coll Cardiol, Jul. 1995.
- Hoffmann, et al. "New Procedure in Transesophageal Echocardiography: Multiplane Transesophageal Echocardiography and Transesophageal Stress Echocardiography." Herz, vol. 18, No. 5, pp. 269-277, Oct. 1993.
- Iacopino, Domenico Gerardo et al, Intraoperative Microvascular Doppler Monitoring of Blood Flow within a Spinal Dural Arteriovenous Fistula: A Precious Surgical Tool, vol. 10, 5 pages, Neurosurg. Focus, Feb. 2001.
- Kim, Ko et al, Positioning Internal Jugular Venous Catheters using the Right Third Intercostal Space in Children, Acta Anaesthesiol Scand, pp. 1284-1286, vol. 47 No. 10, Nov. 2003.
- Kjelstrup T et al, Positioning of Central Venous Catheters using ECG, Tidsskr nor Laegeforen, pp. 599-601, vol. 111 No. 5, Feb. 1999 (Abstract only).
- Kowalski, CM et al, Migration of Central Venous Catheters: Implications for Initial Catheter Tip Positioning, J Vasc Interv Radiol, pp. 443-447, vol. 8 No. 3, May-Jun. 1997.
- Leowenthal, MR et al, The Peripherally Inserted Central Catheter (PICC): A Prospective Study of its Natural History after Fossa Insertion, Anaesth Intensive Care, pp. 21-24; vol. 30 No. 1, Feb. 2002.
- Lepage Ronan et al, ECG Segmentation and P-wave Feature Extraction: Application to Patients Prone to Atrial Fibrillation, IEEE/EMBS Proceedings, 23rd Annual Conference, Istanbul, Turkey, Oct. 25-28, 2001.
- Liu, Ji-Bin et al, Catheter-Based Intraluminal Sonography, J Ultrasound Med, pp. 145-160, vol. 23, 2004.
- Lucey, B et al, Routine Chest Radiographs after Central Line Insertion: Mandatory Postprocedural Evaluation or Unnecessary Waste of Resources?, Cardiovasc Interv Radiol, pp. 381-384, vol. 22 No. 5, Sep.-Oct. 1999.
- Lynch, RE et al, A Procedure for Placing Pediatric Femoral Venous Catheter Tips near the Right Atrium, Pediatr Emerg Care, pp. 130-132, vol. 18 No. 2, Apr. 2002.
- Madan, et al. "Right Atrial Electrocardiography: A Technique for the Placement of Central Venous Catheters for Chemotherapy or Intravenous Nutrition." British Journal of Surgery, vol. B1, pp. 1604-1605, 1994.
- Madias, John E, Intracardiac (Superior Vena Cava/Right Atrial) ECGs using Saline Solution as the Conductive Medium for the Proper Positioning of the Shiley Hemodialysis Catheter: Is it Not Time to Forego the Postinsertion Chest Radiograph?, pp. 2363-2367, Chest, 2003.
- Martin, Roy W, An Ultrasoundic Catheter for Intravascular Measurement of Blood Flow: Technical Details, IEEE Transactions on Sonics and Ultrasonics, vol. SU-27, No. 6, pp. 277-286, Nov. 1980.
- McDonnell, "Intra-Atrial Electrocardiography (ECG) for Catheter Placement." Literature review prepared for Bard Access Systems, Oct. 2007.
- McGee et al., "Accurate Placement of Central Venous Catheters: A Prospective, Randomize, Multicenter Trail." Critical Care Medicine, vol. 21 No. 8, Aug. 1993.
- MedGraphics, CardioPerfect® Resting/Stress ECG System, 3 pages, 2001.
- Michenfelder, John et al, Air Embolism During Neurosurgery—An Evaluation of Right-Atrial Catheters for Diagnosis and Treatment, JAMA, pp. 1353-1358, vol. 208, No. 8, May 26, 1969.
- Michenfelder, John et al, Air Embolism During Neurosurgery . . . A New Method of Treatment, Anesthesia and Analgesia . . . Current Researches, pp. 390-395, vol. 45, No. 4, Jul.-Aug. 1966.
- Microbird™ Miniaturized DC Magnetic Sensors for Intra-body Navigation and Localization, Specifications, 2005.
- Micronix Pty Ltd "CathRite" Guiding Styled Core Manufacturing, Jun. 15, 2006.
- Murthy, Vrudhula et al, Analysis of Power Spectral Densities of Electrocardiograms, Mathematical Biosciences, pp. 41-51, vol. 12 No. 1-2, Oct. 1971.
- Nadroo, AM et al, Changes in Upper Extremity Position Cause Migration of Peripherally Inserted Central Catheters in Neonates, Pediatrics, pp. 131-136, vol. 110, Jul. 2002.
- Nakatani, K et al, Accurate Placement of Central Venous Catheters—ECG-guided method vs Patient Height Method, Masui, pp. 34-38, vol. 51 No. 1, Jan. 2002.
- Nazarian, GK et al, Changes in Tunneled Catheter Tip Position when a patient is Upright, J Vasc Interv Radiol, pp. 437-441, vol. 8 No. 3, May-Jun. 1997.
- Neurometer® CPT, Clinical Applications. Neurotron, Inc. website: [www.neurotron.com/CLINAPS.html](http://www.neurotron.com/CLINAPS.html), last accessed Oct. 23, 2006.
- Neurometer® CPT, Frequently Asked Questions. Neurotron, Inc. website: [www.neurotron.com/CPTFAQ/html](http://www.neurotron.com/CPTFAQ/html), last accessed Oct. 23, 2006.
- Neurometer® CPT, Products Page. Neurotron, Inc. website: [www.neurotron.com/products.html](http://www.neurotron.com/products.html), last accessed Oct. 23, 2006.
- Neurometer® Electrodiagnostic Neuroselective Sensory Nerve Evaluation: Charts, Tables, Documents & Downloads. Neurotron, Inc. website: [www.neurotron.com/downloads.html](http://www.neurotron.com/downloads.html), last accessed Oct. 23, 2006.
- Odd, De et al, Does Radio-opaque Contrast Improve Radiographic localisation of Percutaneous Central Venous Lines?, Arch Dis Child Fetal Neonatal Ed, pp. 41-43, vol. 89 No. 1, Jan. 2004.
- Palesty, JA et al, Routine Chest Radiographs Following Central Venous Recatheterization over a Wire are not Justified, Am J Surg, pp. 618-621, vol. 176 No. 6, Dec. 1998.
- Paliotti, Roberta P. et al, Intravascular Doppler Technique for Monitoring Renal Venous Blood Flow in Man, J Nephrol, pp. 57-62, 2003.
- Parker, K.H. et al, Cardiovascular Fluid Dynamics, Department of Bioengineering, National Heart and Lung Institute, Imperial College of Science, Technology and Medicine, Cardiovascular Haemodynamics, pp. 1-28, Sep. 26, 2005.
- Pawlik, et al., "Central Venous Catheter Placement: Comparison of the Intravascular Guidewire and the Fluid Column Electrocardiograms." European Journal of Anaesthesiology, vol. 41, pp. 594-599, 2004.
- Starr, David S et al, EKG Guided Placement of Subclavian CVP Catheters Using J-Wire, pp. 673-676, Ann. Surg, Dec. 1986.
- Stas, M et al, Peroperative Intravasal Electrographic Control of Catheter Tip Position in Access Ports Placed by Venous Cut-Down Technique, EJSO, pp. 316-320, vol. 27, 2001.
- Stereotaxis Magetic Navigation System with Navigant™ User Interface, 2005 Brochure.
- Tepa® Health Innovation PC based ECG System Introduction and Technical Specifications, EKG Master USB, 2 pages, Nov. 2003.

(56)

## References Cited

## OTHER PUBLICATIONS

- The FloWire Doppler Guide Wire located <<http://www.volcanocorp.com/products/flowire-doppler-guide-wire.php>>, 2011.
- Traxal Technologies, Tracking Technology website overview: [www.traxal.com/rd/rd\\_classroom\\_trackingtechnology.htm](http://www.traxal.com/rd/rd_classroom_trackingtechnology.htm), last accessed Dec. 1, 2006.
- UAB Health Systems, Arrhythmias, retrieved from <http://www.health.uab.edu/14564/> on Nov. 15, 2007, 12 pages.
- U.S. Appl. No. 11/466,602, filed Aug. 23, 2006 Advisory Action dated Jun. 22, 2009.
- U.S. Appl. No. 11/466,602, filed Aug. 23, 2006 Final Office Action dated Apr. 8, 2010.
- U.S. Appl. No. 11/466,602, filed Aug. 23, 2006 Final Office Action dated Jan. 30, 2009.
- U.S. Appl. No. 11/466,602, filed Aug. 23, 2006 Non-Final Office Action dated Sep. 25, 2009.
- U.S. Appl. No. 11/552,094, filed Oct. 23, 2006 Non-Final Office Action dated Apr. 27, 2009.
- U.S. Appl. No. 11/552,094, filed Oct. 23, 2006 Notice of Allowance dated May 20, 2010.
- U.S. Appl. No. 12/369,625, filed Feb. 11, 2009 Non-Final Office Action dated Jul. 20, 2011.
- U.S. Appl. No. 11/552,094, filed Oct. 23, 2006 Notice of Allowability dated Apr. 2, 2010.
- Valdivieso, J.R. Perez, et al., Evaluation of a formula for optimal positioning of a central venous catheter inserted through the right internal jugular vein, *Rev. Esp. Anestesiología. Reanim.* 2003; 50: 77-79.
- VasoNova Inc, Vascular navigation system for accurate placement of PICCs, *Start-Up Emerging Medical Ventures*, pp. 44-45, vol. 14 No. 7, Jul.-Aug. 2009.
- VIASYS Healthcare MedSystems, Navigator® Benefits, 2008.
- VIASYS Healthcare MedSystems, Navigator® Research in Cost Justification, 2008.
- Watters, et al. "Use of Electrocardiogram to Position Right Atrial Catheters During Surgery." *Annals of Surgery*, vol. 225, No. 2, pp. 165-171, 1997.
- Welch Allyn Cardioperfect® PC-Based Resting ECG, 2003.
- Wilson, R. G. et al, Right Atrial Electrocardiography in Placement of Central Venous Catheters, *The Lancet*, pp. 462-463, Feb. 27, 1988.
- Worley, Seth J. "Use of a Real-Time Three-Dimensional Magnetic Navigation System for Radiofrequency Ablation of Accessory Pathways." *PACE*, vol. 21 pp. 1636-1643, Aug. 1998.
- Yilmazlar A et al, Complications of 1303 Central Venous Cannulations, *J R Soc Med*, pp. 319-321, vol. 90 No. 6, Jun. 1997 (Abstract only).
- Yoon, SZ et al, Usefulness of the Carina as a Radiographic Landmark for Central Venous Catheter Placement in Paediatric Patients, *Br J Anaesth*, Jul. 2005.
- Yoshida, Teruhisa et al, Detection of Concealed Left Sided Accessory Atrioventricular Pathway by P Wave Signal Averaged Electrocardiogram, *J Am Coll Cardiol*, pp. 55-62, 1999.
- Zaaroor, et al. "Novel Magnetic Technology for Intraoperative Intracranial Frameless Navigation: In Vivo and in Vitro Results." *Neurosurgery*, vol. 48, No. 5, pp. 1100-1107, May 2001.
- "Ascension to Launch New 3D Guidance™ Tracker at TCT 2006." Press Release from Ascension website: [www.ascension-tech.com/news/press\\_101106.php](http://www.ascension-tech.com/news/press_101106.php), last accessed Dec. 1, 2006.
- Acuson—The Value of Vision, AcuNav Diagnostic Ultrasound Catheter, 2000.
- Advertising flyer for GAVECELT—The Italian Group for Long Term Venous Access Devices, for program on International Meeting on PICC's, Midline Catheters and Long Term Venous Access Devices in Catholic University, Rome, Italy on Dec. 3, 4, 5, 2008.
- Alexander, GD et al, The Role of Nitrous Oxide in Postoperative Nausea and Vomiting, Collection of Abstracts Presented at the International Anesthesia Research Society by various speakers, 58th Congress, Mar. 12-14, 1984, *Anesthesia and Analgesia*, pp. 175-284, vol. 63, 1984.
- Allan, P.L. et al, Role of Ultrasound in the Assessment of Chronic Venous Insufficiency, *Ultrasound Quarterly*, vol. 17, No. 1, pp. 3-10, 2001.
- Andropoulos, et al. "A Controlled Study of the Transesophageal Echocardiography to Guide Central Venous Catheter Placement in Congenital Heart Surgery Patients." *The International Anesthesia Research Society*, vol. 89, pp. 65-70, 1999.
- Anonymous author, Correct Catheter Placement with a low-impact, reliable and economical method, <[http://www.cvc-partner.com/index\\_cfm?103A955CC6844BF58ACFE3C9C1471959](http://www.cvc-partner.com/index_cfm?103A955CC6844BF58ACFE3C9C1471959)>, last accessed Dec. 22, 2011.
- Arai, J et al, Detection of Peripherally Inserted Central Catheter Occlusion by in-line Pressure Monitoring, *Paediatr Anaesth*, pp. 621-624, vol. 12 No. 7, Sep. 2002.
- Arrow International, Inc., The Arrow-Johans RAECG Adapter-Making Proper Central Venous Catheter Placement More Reliable (Model No. EG-04900), Technical Report 1987, USA.
- Aslamy, et al. "MRI of Central Venous Anatomy: Implications for Central Venous Catheter Insertion." *American College of Chest Physicians*, Jun. 8, 2009.
- AU 2006283022 filed Aug. 24, 2006 Office Action dated Dec. 22, 2010.
- AURORA® System Technical Specifications 2004.
- B. Braun Website, "The Optimal Position of the Central Venous Catheter." [http://www.cvcpartner.com/index\\_cfm18F1BDEA1310466194960A39F4E90968](http://www.cvcpartner.com/index_cfm18F1BDEA1310466194960A39F4E90968) (2009).
- Bailey, SH et al, Is Immediate Chest Radiograph Necessary after Central Venous Catheter Placement in a Surgical Intensive Care Unit?, *Am J Surg*, pp. 517-522, vol. 180 No. 6, Dec. 2000.
- Barber, JM et al, A Nurse led Peripherally Inserted Central Catheter Line Insertion Service is Effective with Radiological Support, *Clin Radiol*, pp. 352-354, vol. 57 No. 5, May 2002.
- Bard Access Systems, Sherlock Tip Location System, 5 pages, 2006.
- Bard Access Systems, Site Rite Vascular Access Ultrasound System, 4 pages, 2005.
- Benchimol, Alberto et al, Right Atrium and Superior Vena Cava Flow Velocity in Man Measured with the Doppler-Catheter Flowmeter-Telemetry System, *The Amer Journal of Medicine*, pp. 303-309, vol. 48, Mar. 1970.
- BioAdvance Lumen Vu, Greenhouse Fund Feb. 2004 Recipient, [www.bioadvance.com](http://www.bioadvance.com) <<http://www.bioadvance.com>>, 2005.
- Borgobello, Bridget, App allows users to view electrocardiograms on smartphones dated Oct. 15, 2010; printed from <http://www.gizmag.com/app-to-view-electrocardiograms-on-smartphones/16664/> on Feb. 4, 2011.
- Buehrle, Douglas, PICC Placement in Humans using Electromagnetic Detection, <[http://www.corpakmedsystems.com/supplement\\_material/supplementpages/navigator/navarticle.html](http://www.corpakmedsystems.com/supplement_material/supplementpages/navigator/navarticle.html)>, 2008.
- C.R. Bard, Inc., Bard Electrophysiology Product Catalogue, Bard Catheters, pp. 74-75 (2002), USA.
- Cadman, A et al, To Clot or Not to Clot? That is the question in Central Venous Catheters, *Clinical Radiology*, pp. 349-355, vol. 59 No. 4, Apr. 2004.
- Calvert, N et al, The Effectiveness and Cost-effectiveness of Ultrasound Locating Devices for Central Venous Access: A Systematic Review and Economic Evaluation, *Health Technology Assessment*, vol. 7, No. 12, 2003.
- Carlson, R et al, Secondary Migration of a Central Venous Catheter—A Case Report, *Minerva Anestesiologica*, pp. 927-931, vol. 69 No. 12, Dec. 2003.
- Caruso, LJ et al, A Better Landmark for Positioning a Central Venous Catheter, *J Clinical Monitoring and Computing*, pp. 331-334, vol. 17 No. 6, Aug. 2002.
- Cavatorta, et al., "Central Venous Catheter Placement in Hemodialysis: Evaluation of Electrocardiography Using a Guidewire." *The Journal of Vascular Access*, vol. 2, pp. 45-50, 2001.
- Chalkiadis, GA et al, Depth of Central Venous Catheter Insertion in Adults: An Audit and Assessment of a Technique to Improve Tip Position, *Anaesth Intensive Care*, pp. 61-66, vol. 26 No. 1, Feb. 1998.

(56)

## References Cited

## OTHER PUBLICATIONS

- Chamsi-Pasha, Hassan et al, Cardiac Complications of Total Parenteral Nutrition: The Role of Two-Dimensional Echocardiography in Diagnosis, *Annals of the Royal College of Surgeons of England*, pp. 120-123, vol. 71, 1989.
- Chaturvedi et al., "Catheter Malplacement During Central Venous Cannulation Through Arm Veins in Pediatric Patients." *Journal of Neurosurgical Anesthesiology*, vol. 15, No. 3 pp. 170-175, Jan. 2003.
- Chen, Zhongping et al, Optical Doppler Tomography: Imaging in vivo Blood Flow Dynamics Following Pharmacological Intervention and Photodynamic Therapy, 7 pages, vol. 67, *Photochemistry and Photobiology*, 1998.
- Cheng, KI et al, A Novel Approach of Intravenous Electrocardiograph Technique in Correct Position the Long-Term Central Venous Catheter, *Kaohsiung J Med Sci*, pp. 241-247, vol. 16 No. 5, May 2000 (Abstract only).
- Chu, et al., "Accurate Central Venous Port—A Catheter Placement: Intravenous Electrocardiography and Surface Landmark Techniques Compared by Using Transesophageal Echocardiography." *The International Anesthesia Research Society*, vol. 98, pp. 910-914, 2004.
- Claasz, Antonia et al, A Study of the Relationship of the Superior Vena Cava to the Bony Landmarks of the Sternum in the Supine Adult: Implications for Magnetic Guidance Systems, *Journal*, vol. 12 No. 3, *JAVA*, Jul. 24, 2007.
- Clifford, et al. "Assessment of Hepatic Motion Secondary to Respiration for Computer Assisted Interventions." *Computer Aided Surgery*, vol. 7, pp. 291-299, 2002.
- Colley, Peter S et al, ECG-Guided Placement of Sorenson CVP Catheters via Arm Veins, *Anesthesia and Analgesia*, pp. 953-956, vol. 63, 1984.
- Collier, PE et al, Cardiac Tamponade from Central Venous Catheters, *Am J Surg*, pp. 212-214, vol. 176 No. 2, Aug. 1998.
- Corsten, et al., "Central Placement Catheter Placement Using the ECG-Guided Cavafix-Certodyn SD Catheter." *Journal of Clinical Anesthesiology*, vol. 6, Nov./Dec. 1994.
- Cucchiara, Roy et al, Time Required and Success Rate of Percutaneous Right Atrial Catheterization: Description of a Technique, *Canad. Anaesth. Soc. J.*, pp. 572-573, vol. 27, No. 6, Nov. 1980.
- Cullinane, DC et al, The Futility of Chest Roentgenograms Following Routine Central Venous Line Changes, *Am J Surg*, pp. 283-285, vol. 176 No. 3, Sep. 1998.
- Curet, Myriam J. et al., University and Practice-based Physicians' Input on the Content of a Surgical Curriculum, *The American Journal of Surgery®* vol. 178 Jul. 1999, 78-84.
- David, et al., "Is ECG-Guidance a Helpful Method to Correctly Position a Central Venous Catheter During Prehospital Emergency Care?" *ACTA Anaesthesiologica Scandinavica*, vol. 49, pp. 1010-1014, 2005.
- Deltec Cath-Finder® Tracking System Operation Manual, 1994.
- Egelhof, Petra, Effects of Somatostatin on Portal Blood Flow and Portal Vein Pressure in Patients with Portal Hypertension due to Liver Cirrhosis Invasive Monitoring during TIPSS Procedures, Dissertation submitted to: Technical University of Munich, Faculty of Medicine, May 13, 2002; Date of examination: Feb. 26, 2003.
- Engelhardt, W et al, ECG-Controlled Placement of Central Venous Catheters in Patients with Atrial Fibrillation, *Anaesthesist*, pp. 476-479, vol. 38 No. 9, Sep. 1989 (Abstract only).
- Fearon, William F et al, Evaluating Intermediate Coronary Lesions in the Cardiac Catheterization Laboratory, vol. 4, No. 1, 7 pages, *Reviews in Cardiovascular Medicine*, 2003.
- Felleiter P et al, Use of Electrocardiographic Placement Control of Central Venous Catheters in Austria, *Acta Med Austriaca*, pp. 109-113, vol. 26 No. 3, 1999 (Abstract only).
- Bankier, Alexander A., Azygos Arch Cannulation by Central Venous Catheters: Radiographic Detection of Malposition and Subsequent Complications, *Journal of Thoracic Imaging* 12:64-69 (1997).
- Cardella, John F. et al., Interventinal Radiologic Placement of Peripherally Inserted Central Catheters, *Journal of Vascular and Interventional Radiology* 1993; 4:653-660.
- Chang, Thomas C. et al., Are Routine Ch Ladiographs Necessary After Image-Guided Placement of Internal Jugular Central Venous Access Devices?, *AJR Feb. 1998*;170:335-337.
- Cheung, P., et al., The Effect of a Disposable Probe Cover on Pulse Oximetry, *Anaesth Intensive Care* 2002; 30: 211-214.
- CN 200880012117.4 filed Apr. 16, 2008 First Office Action dated Dec. 23, 2011.
- EP 09808901.4 filed Aug. 21, 2009 European Search Report dated May 23, 2012.
- EP 09813632.8 filed Apr. 5, 2011 European Search Report dated Jul. 4, 2012.
- Gjendemsjo, Anders, et al., Energy and Power, The Connexions Project, Version 1.2, Feb. 20, 2004.
- Joosting, Jean-Pierre, "Dual-interface RFID-compatible EEPROM enables remote access to electronic device parameters," *EE Times*, Mar. 8, 2010.
- JP 2008-528151 filed Aug 24, 2006 Notice of Grant dated May 6, 2012.
- JP 2010-504220 filed Sep. 3, 2009 Office Action dated May 21, 2012.
- Koffler, Julia, et al., Epinephrine application via an endotracheal airway and via the Combitube in esophageal position, *Critical Care Medicine*: May 2000, vol. 28: Issue 5, pp. 1445-1449.
- Lum, Phillip, A New Formula-Based Measurement Guide for Optimal Positioning of Central Venous Catheters, *JAVA*, vol. 9, No. 2, pp. 80-85, 2004.
- Markovich, Mary B., Central Venous Catheter Tip Placement: Determination of Posterior Malposition—A Case Study, *JAVA*, vol. 11, No. 2, pp. 85-89, 2006.
- PCT/US2008/060502 filed Apr. 16, 2008 International Search Report and Written Opinion dated Oct. 16, 2008.
- PCT/US2010/045084 filed Aug. 10, 2010 International Preliminary Report on Patentability dated Feb. 23, 2012.
- PCT/US2010/045084 filed Aug. 10, 2010 Written Opinion dated Apr. 14, 2011.
- PCT/US2011/038415 filed May 27, 2011 International Search Report dated Sep. 28, 2011.
- PCT/US2011/038415 filed May 27, 2011 Written Opinion dated Sep. 28, 2011.
- PCT/US2011/047127 filed Aug. 9, 2011 International Search Report dated Feb. 29, 2012.
- PCT/US2011/047127 filed Aug. 9, 2011 Written Opinion dated Feb. 29, 2012.
- PCT/US2011/048403 filed Aug. 19, 2011 International Search Report dated Dec. 15, 2011.
- PCT/US2011/048403 filed Aug. 19, 2011 Written Opinion dated Dec. 15, 2011.
- PCT/US2011/052793 filed Sep. 22, 2011 International Search Report dated Jan. 6, 2012.
- PCT/US2011/052793 filed Sep. 22, 2011 Written Opinion dated Jan. 6, 2012.
- PCT/US2011/067268 filed Dec. 23, 2011 International Search Report and Written Opinion dated Apr. 27, 2012.
- Popp, M. B. et al., Accuracy of implanted port placement with the use of the electromagnetic CathTrack® catheter locator system, *The Journal of Vascular Access* 2005; 6: 9-12.
- Rutherford, J. S. et al., Depth of Central Venous Catheterization: An Audit of Practice in a Cardiac Surgical Unit, *Anaesth Intens Care* 1994; 22: 267-271.
- Schuster, M. et al., The carina as a landmark in central venous catheter placement, *British Journal of Anaesthesia* 85 (2): 192-4 (2000).
- Siela, Debra, Using Chest Radiography in the Intensive Care Unit, *Crit Care Nurse* Aug. 1, 2002 vol. 22 No. 4, pp. 18-27.
- U.S. Appl. No. 12/104,253, filed Apr. 16, 2008 Final Office Action dated Jul. 27, 2011.
- U.S. Appl. No. 12/104,253, filed Apr. 16, 2008 Non-Final Office Action dated Nov. 29, 2010.
- U.S. Appl. No. 12/323,273, filed Nov. 25, 2008 Non-Final Office Action dated Jun. 8, 2012.

(56)

**References Cited**

## OTHER PUBLICATIONS

- U.S. Appl. No. 12/369,625, filed Feb. 11, 2009 Final Office Action dated Feb. 23, 2012.
- U.S. Appl. No. 12/427,244, filed Apr. 21, 2009 Non-Final Office Action dated Jan. 19, 2012.
- U.S. Appl. No. 12/557,401, filed Sep. 10, 2009 Non-Final Office Action dated Apr. 24, 2012.
- U.S. Appl. No. 12/878,915, filed Sep. 9, 2010 Non-Final Office Action dated Mar. 15, 2012.
- Vesely, Thomas M. et al., Central Venous Catheter Tip Position: A Continuing Controversy, *J Vasc Interv Radiol* 2003; 14:527-534.
- Wong, Jeffrey J. et al., Azygos Tip Placement for Hemodialysis Catheters in Patients with Superior Vena Cava Occlusion, *Cardiovasc Intervent Radiol* (2006) 29:143-146.
- Zachariou, Zacharias et al., Intra-atrial ECG recording: a new and safe method for implantation of Broviac catheters in children, *Pediatr Surg Int* (1994) 9: 457-458.
- CN 200880125528.4 filed Nov. 25, 2008 First Office Action dated Jun. 5, 2012.
- EP 08855396.1 filed Jun. 15, 2010 European Search Report dated Jul. 31, 2012.
- Konings, MK, et al., Development of an intravascular impedance catheter for detection of fatty lesions in arteries, *IEEE Trans Med Imaging* Aug. 1997; 16(4):439-46.
- PCT/US2011/058138 filed Oct. 27, 2011 International Search Report dated Feb. 7, 2012.
- PCT/US2011/058138 filed Oct. 27, 2011 Written Opinion dated Feb. 7, 2012.
- PCT/US2012/045814 filed Jul. 6, 2012 International Search Report and Written Opinion dated Oct. 1, 2012.
- Pop, Gheorghe A. et al., Catheter-based impedance measurements in the right atrium for continuously monitoring hematocrit and estimating blood viscosity changes; an in vivo feasibility study in swine, *Biosensors and Bioelectronics* 19 (2004) 1685-1693.
- U.S. Appl. No. 11/466,602, filed Aug. 23, 2006 Appeal Board Decision dated Sep. 17, 2012.
- U.S. Appl. No. 12/369,625, filed Feb. 11, 2009 Notice of Allowance dated Oct. 5, 2012.
- U.S. Appl. No. 12/369,625, filed Feb. 11, 2009 Notice of Panel Decision dated Aug. 1, 2012.
- U.S. Appl. No. 12/545,762, filed Aug. 21, 2009 Non-Final Office Action dated Aug. 1, 2012.
- U.S. Appl. No. 12/715,556, filed Mar. 2, 2010 Non-Final Office Action dated Sep. 13, 2012.
- U.S. Appl. No. 12/878,915, filed Sep. 9, 2010 Final Office Action dated Sep. 26, 2012.
- U.S. Appl. No. 13/118,138, filed May 27, 2011 Non-Final Office Action dated Oct. 3, 2012.
- U.S. Appl. No. 13/213,622, filed Aug. 19, 2011 Non-Final Office Action dated Jul. 31, 2012.
- U.S. Appl. No. 13/336,919, filed Dec. 23, 2011 Non-Final Office Action dated Oct. 16, 2012.
- PCT/US2006/033079 filed Aug. 24, 2006 International Preliminary Report on Patentability dated Feb. 26, 2008.
- PCT/US2006/033079 filed Aug. 24, 2006 Search Report dated Dec. 19, 2006.
- PCT/US2006/033079 filed Aug. 24, 2006 Written Opinion dated Dec. 19, 2006.
- PCT/US2008/084751 filed Nov. 25, 2008 International Preliminary Report on Patentability dated Jun. 1, 2010.
- PCT/US2008/084751 filed Nov. 25, 2008 Search Report dated May 20, 2009.
- PCT/US2008/084751 filed Nov. 25, 2008 Written Opinion dated May 20, 2009.
- PCT/US2009/033116 filed Feb. 4, 2009 International Preliminary Report on Patentability dated Aug. 10, 2010.
- PCT/US2009/033116 filed Feb. 4, 2009 Search Report dated Mar. 13, 2009.
- PCT/US2009/033116 filed Feb. 4, 2009 Written Opinion dated Mar. 13, 2009.
- PCT/US2009/041051 filed Apr. 17, 2009 Search Report dated Jul. 28, 2009.
- PCT/US2009/041051 filed Apr. 17, 2009 Written Opinion dated Jul. 28, 2009.
- PCT/US2009/054687 filed Aug. 21, 2009 International Preliminary Report on Patentability dated Feb. 22, 2011.
- PCT/US2009/054687 filed Aug. 21, 2009 Search Report dated Oct. 6, 2009.
- PCT/US2009/054687 filed Aug. 21, 2009 Written Opinion dated Oct. 6, 2009.
- PCT/US2009/056567 filed Sep. 10, 2009 International Preliminary Report on Patentability dated Mar. 15, 2011.
- PCT/US2009/056567 filed Sep. 10, 2009 Search Report dated Nov. 6, 2009.
- PCT/US2009/056567 filed Sep. 10, 2009 Written Opinion dated Nov. 6, 2009.
- PCT/US2010/038555 filed Jun. 14, 2010 Search Report dated Oct. 5, 2010.
- PCT/US2010/038555 filed Jun. 14, 2010 Written Opinion dated Oct. 5, 2010.
- PCT/US2010/045084 filed Aug. 10, 2010 Search Report dated Apr. 14, 2011.
- PCT/US2010/050773 filed Sep. 29, 2010 Search Report dated Jan. 24, 2011.
- PCT/US2010/050773 filed Sep. 29, 2010 Written Opinion dated Jan. 24, 2011.
- PCT/US2010/051917 filed Oct. 8, 2010 Search Report dated Nov. 29, 2010.
- PCT/US2010/051917 filed Oct. 8, 2010 Written Opinion dated Nov. 29, 2010.
- PCT/US2011/023497 filed Feb. 2, 2011 Search Report dated Jun. 6, 2011.
- PCT/US2011/023497 filed Feb. 2, 2011 Written Opinion dated Jun. 6, 2011.
- Pennington, C.R., Right Atrial Thrombus: a Complication of Total Parenteral Nutrition, *British Medical Journal*, pp. 446-447, vol. 295, Aug. 15, 1987.
- Perez, Valdivieso JR et al, Evaluation of a Formula for Optimal Positioning of a Central Venous Catheter through the Right Internal Jugular Vein, *Rev Esp Anesthesiol Reanim*, pp. 77-79, vol. 50 No. 2, Feb. 2003.
- Petersen, J et al, Silicone Venous Access Devices Positioned with their Tip High in the Superior Vena Cava are More Likely to Malfunction, *Am J Surg*, pp. 38-41, vol. 178 No. 1, Jul. 1999.
- Pittiruti, et al, Intracavitary EKG Monitoring: A reliable method for controlling tip position during and after PICC Insertion presentation in Catholic University, Rome, Italy in 2008.
- Pittiruti, et al. "The EKG Method for Positioning the Tip of PICCs: Results from Two Preliminary Studies." *JAVA*, vol. 13, No. 4, pp. 179-185, 2008.
- Polos, PG. et al, Tips for Monitoring the Position of a Central Venous Catheter—How Placement can go awry—even when the anatomy is normal, *J Crit Illn*, pp. 660-674, vol. 8 No. 6, Jun. 1993 (Abstract only).
- Randolph AG et al, Ultrasound guidance for placement of central venous catheters: a meta-analysis of the literature, *Critical Care Medicine*, pp. 2053-2058, vol. 24, Dec. 1996.
- Reece, A et al, Positioning Long Lines: Contrast Versus Plain Radiography, *Arch Dis Child Fetal Neonatal Ed*, pp. 129-130, vol. 84 No. 2, Mar. 2001.
- Reynolds, N et al, Assessment of Distal Tip Position of Long Term Central Venous Feeding Catheters using Transesophageal Echocardiology, *JPEN J Parenter Enteral Nutr*, pp. 39-41, vol. 25 No. 1, Jan.-Feb. 2001.
- Ruschulte, Heiner et al, Prevention of Central Venous Catheter related infections with chlorhexidine gluconate impregnated wound dressings: A randomized controlled trial, presented as an abstract at the Annual meeting of the European Society of Anaesthesiologists (ESA) in Madrid, Spain in Jun. 2006, 12 pages, *Annals of Hematology*, Jul. 14, 2008.
- Sacolick, et al. "Electromagnetically Tracked Placement of a Peripherally Inserted Central Catheter." *SPIE Medical Imaging*, 2004 Proceedings.

(56)

## References Cited

## OTHER PUBLICATIONS

- Salem, et al. "A New Peripherally Implanted Subcutaneous Permanent Central Venous Access Device for Patients Requiring Chemotherapy." *Journal of Clinical Oncology*, vol. 11, No. 11, pp. 2181-2185, Nov. 1993.
- Savary, D et al, Intra-atrial Monitoring to Add Insertion of a Central Venous Line in Pre-Hospital Emergency Care *Journal Europeen des Urgences*, pp. 75-78, vol. 17 No. 2, 2004.
- Schafer et al. "Incorrect placement of a vena cava catheter and its prevention by intra-atrial ECG." *Anaesthesist*. Jan. 1988;37(1):49-51.
- Schummer, et al. "Central Venous Catheters—The inability of 'intra-atrial ECG' to prove adequate positioning." *British Journal of Anaesthesia*, vol. 93, No. 2, pp. 193-198, 2004.
- Schummer, W et al, ECG-guided Central Venous Catheter Positioning: Does it detect the Pericardial Reflection rather than the Right Atrium?, *Eur J Anaesthesiol*, pp. 600-605, vol. 21 No. 8, Aug. 2004 (Abstract only).
- Schummer, W et al, Intra-Atrial ECG is not a Reliable Method for Positioning Left Internal Jugular Vein Catheters, *Br J Anaesth*, pp. 481-486, vol. 91 No. 4, Oct. 2003.
- Schummer, W, Central Venous Catheter—the Inability of "Intra-Atrial ECG" to prove Adequate Positioning, *Br J Anaesth*, pp. 193-198, vol. 93 No. 2, Aug. 2004.
- Simon, et al., "Central Venous Catheter Placement in Children: Evaluation of Electrocardiography Using J-Wire." *Paediatric Anaesthesia* vol. 9, pp. 501-504, 1999.
- Smith, Brigham, et al., Intravenous electrocardiographic guidance for placement of peripherally inserted central catheters, *Journal of Electrocardiology* 43 (2010) 274-278.
- Stark, DD et al, Radiographic Assessment of Venous Catheter Position in Children: Value of the Lateral View, *Pediatric Radiology*, pp. 76-80, vol. 14 No. 2, 1984.
- Starkhammar et al. "Cath-Finder Catheter Tracking System: A New Device for Positioning of Central Venous Catheters. Early Experience from Implantation of Brachial portal Systems." *Acta Anaesthesiol Scandinavia*, vol. 34, No. 4 pp. 296-300, May 1990.
- Starkhammar, H et al, Central Venous Catheter Placement using Electromagnetic Position Sensing: A Clinical Evaluation, *Biomed. Instrum Technol*, vol. 30 No. 2, pp. 164-170; Mar.-Apr. 1996.
- U.S. Appl. No. 29/428,649, filed Aug. 1, 2012 Notice of Allowance dated Jul. 5, 2013.
- VIASYS Health Care Inc. Cortrak © Fact Sheet, 2005.
- VIASYS MedSystems, Cortrak™ Systems Brochure, 2005.
- Volcano ComboMap Features and Benefits/Technical Specifications, 2 pages, 2011.
- AU 2008329807 exam requested Aug. 13, 2012 Examination Report No. 1 dated Feb. 15, 2013.
- AU 2011289513 filed Jan. 21, 2013 Examiners Report dated Jul. 5, 2013.
- AU 2012202293 filed Apr. 19, 2012 Examination Report No. 1 dated Apr. 24, 2013.
- AU 2013204243 filed Apr. 12, 2013 Examiner's Report dated Jun. 5, 2013.
- B. Braun, Certofix Central Venous Catheter for Placement Using the Seldinger Technique with Simultaneous ECG Lead Option, Feb. 2010.
- C.R. Bard, CathTrack™ Catheter Location System at [www.bardaccess.com](http://www.bardaccess.com) <<http://www.bardaccess.com>>, last accessed Apr. 28, 2011.
- CA 2,619,909 filed Aug. 24, 2006 Examiner's Report dated Oct. 26, 2012.
- CN 200880012117.4 filed Apr. 16, 2008 Second Office Action dated Oct. 8, 2012.
- CN 200880012117.4 filed Apr. 16, 2008 Third Office Action dated Apr. 27, 2013.
- CN 200880125528.4 filed Nov. 25, 2008 Second Office Action dated Mar. 6, 2013.
- CN 200880125528.4 filed Nov. 25, 2008 Third Office Action dated Jul. 1, 2013.
- CN 200980123021.X filed Dec. 17, 2010 First Office Action dated Nov. 19, 2012.
- CN 200980144663.8 filed May 9, 2011 First Office Action dated Dec. 5, 2012.
- EP 08855396.1 filed Jun. 15, 2010 Intent to Grant dated Jul. 5, 2013.
- EP 09707467.8 supplemental European search report dated Jun. 18, 2013.
- EP 09808901.4 filed Aug. 21, 2009 Examination Report dated May 10, 2013.
- EP 09813632.8 filed Apr. 5, 2011 Office Action dated Apr. 30, 2013.
- EP 12177438.4 filed Jul. 23, 2012 European Search Report dated Dec. 4, 2012.
- EP 12177438.4 filed Jul. 23, 2012 extended European Search Report dated Mar. 25, 2013.
- Hill, Bradley et al, Abstract of article discussing VasaNova VPS as guide for placement of PICCs. 2009.
- JP 2010-504220 filed Sep. 3, 2009 Final Office Action dated Apr. 18, 2013.
- PCT/US2011/038391 filed May 27, 2011 International Preliminary Report on Patentability and Written Opinion dated Dec. 4, 2012.
- PCT/US2011/038391 filed May 27, 2011 International Search Report dated Sep. 21, 2011.
- PCT/US2011/038415 filed May 27, 2011 International Preliminary Report on Patentability dated Dec. 13, 2012.
- PCT/US2011/047127 filed Aug. 9, 2011 International Preliminary Report on Patentability dated Apr. 18, 2013.
- PCT/US2011/052793 filed Sep. 22, 2011 International Preliminary Report on Patentability dated Apr. 4, 2013.
- PCT/US2011/058138 filed Oct. 27, 2011 International Preliminary Report on Patentability dated May 10, 2013.
- PCT/US2011/067268 filed Dec. 23, 2011 International Preliminary Report on Patentability dated Jul. 4, 2013.
- PCT/US2012/063956 filed Nov. 7, 2012 International Search Report and Written Opinion dated Apr. 1, 2013.
- Rutala, Guideline for Disinfection and Sterilization in Healthcare Facilities, 2008.
- STEREOTAXIS, Expanding the Possibilities of Interventional Medicine: Remote Navigation and Automation, pp. 1-8, Apr. 2011.
- U.S. Appl. No. 11/466,602, filed Aug. 23, 2006 Non-Final Office Action dated Mar. 28, 2013.
- U.S. Appl. No. 11/466,602, filed Aug. 23, 2006 Notice of Allowance dated Dec. 3, 2012.
- U.S. Appl. No. 12/426,175, filed Apr. 17, 2009 Non-Final Office Action dated Dec. 3, 2012.
- U.S. Appl. No. 12/545,762, filed Aug. 21, 2009 Final Office Action dated Mar. 7, 2013.
- U.S. Appl. No. 12/575,456, filed Oct. 7, 2009 Non-Final Office Action dated Oct. 5, 2012.
- U.S. Appl. No. 12/854,083, filed Aug. 10, 2010 Non-Final Office Action dated Jan. 29, 2013.
- U.S. Appl. No. 12/878,915, filed Sep. 9, 2010 Notice of Allowance dated Jan. 8, 2013.
- U.S. Appl. No. 12/900,750, filed Oct. 8, 2010 Final Office Action dated Dec. 3, 2013.
- U.S. Appl. No. 12/900,750, filed Oct. 8, 2010 Non-Final Office Action dated Apr. 10, 2014.
- U.S. Appl. No. 12/900,750, filed Oct. 8, 2010 Non-Final Office Action dated Jun. 3, 2013.
- U.S. Appl. No. 13/118,138, filed May 27, 2011 Final Office Action dated Apr. 3, 2013.
- U.S. Appl. No. 13/213,622, filed Aug. 19, 2011 Final Office Action dated Feb. 19, 2013.
- U.S. Appl. No. 13/283,395, filed Oct. 27, 2011 Non-Final Office Action dated Apr. 23, 2013.
- U.S. Appl. No. 13/336,919, filed Dec. 23, 2011 Advisory Action dated May 23, 2013.
- U.S. Appl. No. 13/336,919, filed Dec. 23, 2011 Final Office Action dated Mar. 1, 2013.
- U.S. Appl. No. 13/337,987, filed Dec. 27, 2011 Non-Final Office Action dated Mar. 15, 2013.
- U.S. Appl. No. 13/671,382, filed Nov. 7, 2012 Non-Final Office Action dated Mar. 10, 2014.



(56)

**References Cited**

## OTHER PUBLICATIONS

CN 201180048882.3 filed Apr. 9, 2013 First Office Action dated Jun. 30, 2014.  
 PCT/US2013/045999 filed Jun. 14, 2013 International Search Report and Written Opinion dated Nov. 21, 2013.  
 PCT/US2014/018681 filed Feb. 26, 2014 International Search Report and Written Opinion dated May 19, 2014.  
 Silindir, M. et al., "Sterilization Methods and the Comparison of E-Beam Sterilization with Gamma Radiation Sterilization," *FABAD J. Pharm. Sci.*, 34, 43-53, 2009.  
 U.S. Appl. No. 12/900,750, filed Oct. 8, 2010 Final Office Action dated Sep. 4, 2014.  
 U.S. Appl. No. 12/900,750, filed Oct. 8, 2010 Non-Final Office Action dated Jan. 30, 2015.  
 U.S. Appl. No. 13/671,382, filed Nov. 7, 2012 Final Office Action dated Sep. 23, 2014.  
 Butler et al. "Practical Considerations for Analog Operation of Bucket-Brigade Circuits" *IEEE Journal of Solid-State Circuits*, vol. SC-8, No. 2, Apr. 1973.  
 CN 201180048882.3 filed Apr. 9, 2013 Second Office Action dated Mar. 18, 2015.  
 CN 201180048882.3 filed Apr. 9, 2013 Third Office Action dated Aug. 19, 2014.  
 Freeman et al. "Delta-Sigma Oversampled Ultrasound Beamformer with Dynamic Delays" *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency control*, vol. 46, No. 2,—Mar. 1999.  
 JP 2013-524183 filed Feb. 8, 2015 First Office Action dated Jun. 24, 2015.  
 Mo et al. "Front-End Processor Using BBD Distributed Delay-Sum Architecture for Micromachined Ultrasonic Sensor Array" *Journal of Microelectromechanical Systems*, vol. 12, No. 4, Aug. 2003.  
 Mo et al. "Integrated analog beam former based on bucket brigade device for micromachined ultrasonic sensor array" *Sensors and Actuators A* 101 (2002) 203-211—Apr. 22, 2012.  
 Mo et al. "Pipelined Delay-Sum Architecture Based on Bucket-Brigade Devices for On-Chip Ultrasound Beamforming" *IEEE Journal of Solid-State Circuits*, vol. 38, No. 10, Oct. 2003.  
 Mucci, R. A. "A Comparison of Efficient Beamforming Algorithms" *IEEE Transactions on Acoustics, Speech, and Signal Processing*, vol. ASSP-32, No. 3,—Jun. 1984.  
 Savord et al. "Fully Sampled Matrix Transducer for Real Time 3D Ultrasonic Imaging" *IEEE Ultrasonics Symposium-945*—2003.  
 Tanaka et al. "Development of BBD Adding-Delay Architecture for Ultrasonic Micro Array Sensor" *IEEJ Trans. SM*, vol. 125, No. 4 2005.  
 Thomenius "Evolution of Ultrasound Beamformers" *IEEE Ultrasonics Symposium* 1996.  
 U.S. Appl. No. 12/900,750, filed Oct. 8, 2010 Final Office Action dated Oct. 19, 2015.

U.S. Appl. No. 13/671,382, filed Nov. 7, 2012 Advisory Action dated May 27, 2015.  
 U.S. Appl. No. 13/671,382, filed Nov. 7, 2012 Final Office Action dated Mar. 12, 2015.  
 U.S. Appl. No. 13/918,707, filed Jun. 14, 2013 Non-Final Office Action dated Jul. 3, 2017.  
 U.S. Appl. No. 13/918,707, filed Jun. 14, 2013 Non-Final Office Action dated May 9, 2016.  
 U.S. Appl. No. 14/190,591, filed Feb. 26, 2014 Non-Final Office Action dated May 17, 2017.  
 U.S. Appl. No. 13/918,707, filed Jun. 14, 2013 Final Office Action dated Apr. 16, 2018.  
 U.S. Appl. No. 14/190,591, filed Feb. 26, 2014 Non-Final Office Action dated Apr. 19, 2018.  
 CN 201380031663.3 filed Dec. 15, 2014 Office Action dated Dec. 21, 2017.  
 CN 201480010486.5 filed Aug. 25, 2015 Office Action dated Jun. 13, 2018.  
 CN 201480010486.5 filed Aug. 25, 2015 Office Action dated Nov. 16, 2017.  
 U.S. Appl. No. 12/900,750, filed Oct. 8, 2010 Examiner's Answer dated Oct. 23, 2018.  
 U.S. Appl. No. 12/900,750, filed Oct. 8, 2010 Non-Final Office Action dated Jun. 27, 2019.  
 U.S. Appl. No. 13/918,707, filed Jun. 14, 2013 Examiner's Answer dated Jan. 25, 2019.  
 U.S. Appl. No. 14/190,591, filed Feb. 26, 2014 Examiner's Answer dated Sep. 11, 2018.  
 U.S. Appl. No. 14/190,591, filed Feb. 26, 2014 Final Office Action dated Oct. 30, 2017.  
 CN 201380031663.3 filed Dec. 15, 2014 Office Action dated Jan. 19, 2017.  
 CN 201380031663.3 filed Dec. 15, 2014 Office Action dated Jul. 12, 2017.  
 CN 201380031663.3 filed Dec. 15, 2014 Office Action dated Jun. 1, 2016.  
 ComboWire® Pressure/Flow Guide Wire Ref 9500 Series, Instructions for Use, Apr. 2011.  
 EP 13804474.8 filed Jan. 7, 2015 Partial European Search Report dated May 31, 2016.  
 EP 14756632.7 filed Aug. 24, 2015 Extended European Search Report dated Sep. 30, 2016.  
 MICRONIX CathRite™ Cardiac Access Device Brochure. Jun. 2004.  
 U.S. Appl. No. 12/900,750, filed Oct. 8, 2010 Final Office Action dated Aug. 4, 2017.  
 U.S. Appl. No. 12/900,750, filed Oct. 8, 2010 Non-Final Office Action dated Jan. 26, 2017.

\* cited by examiner







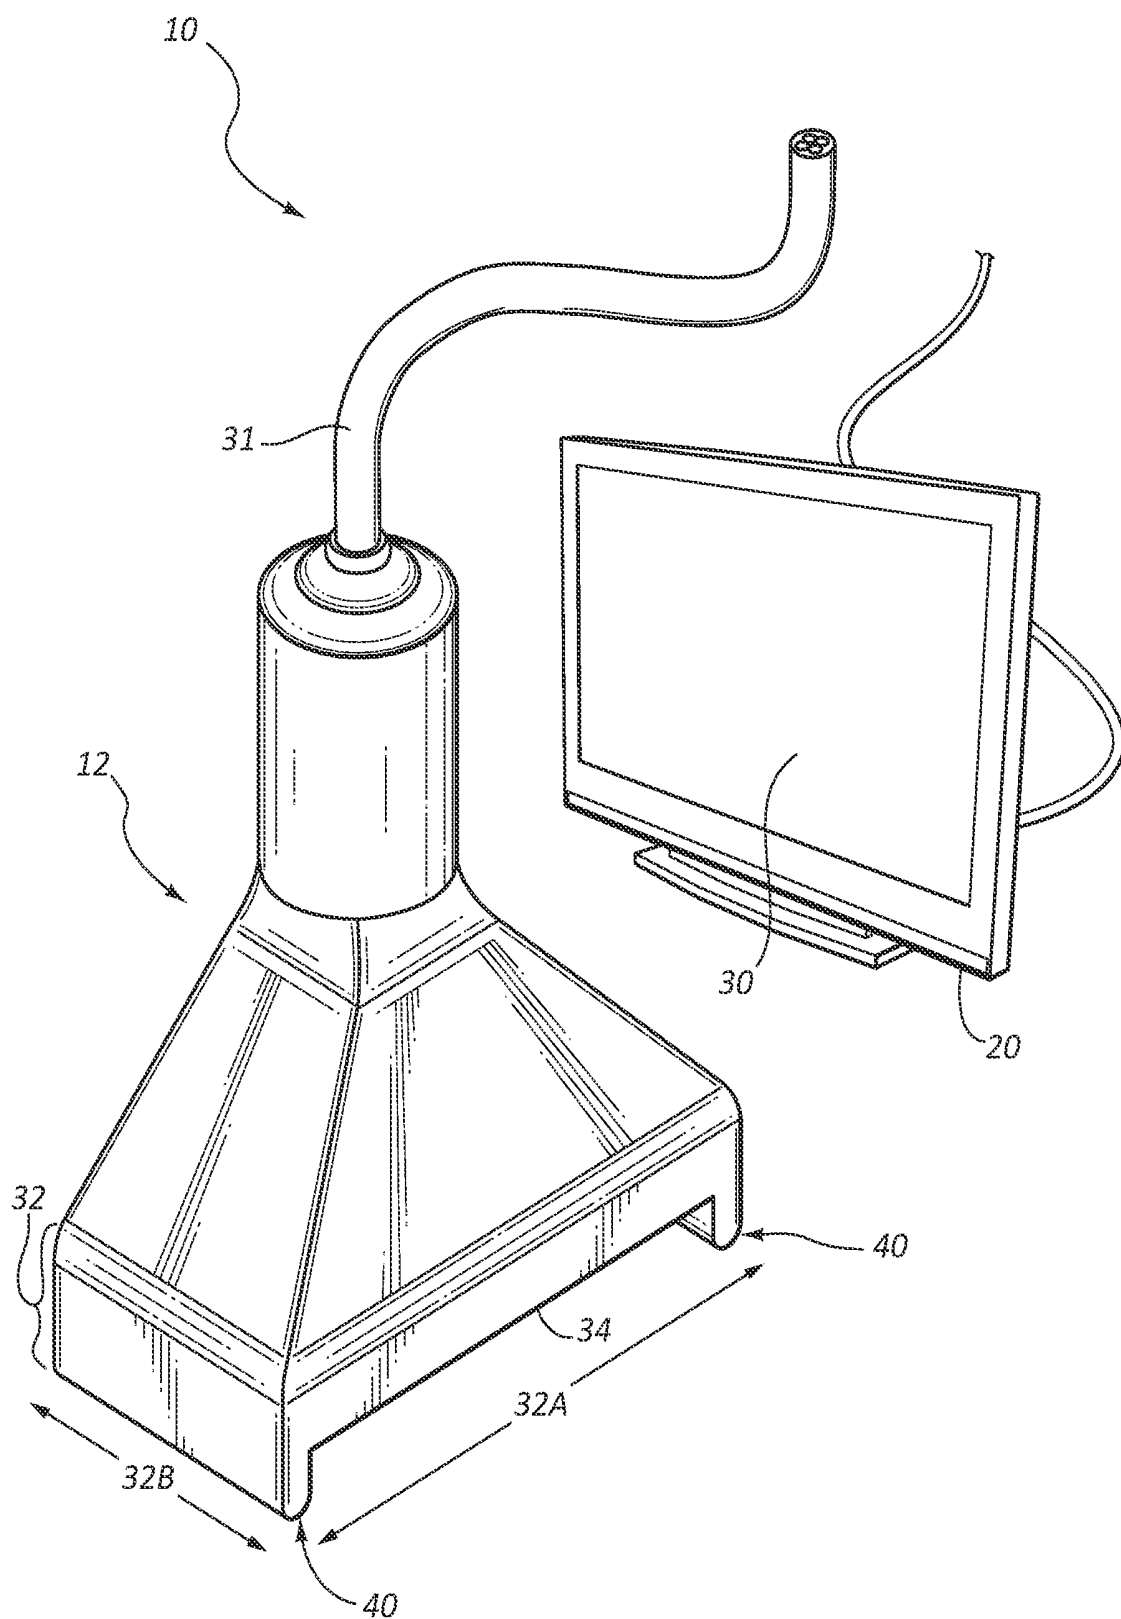



FIG. 1A

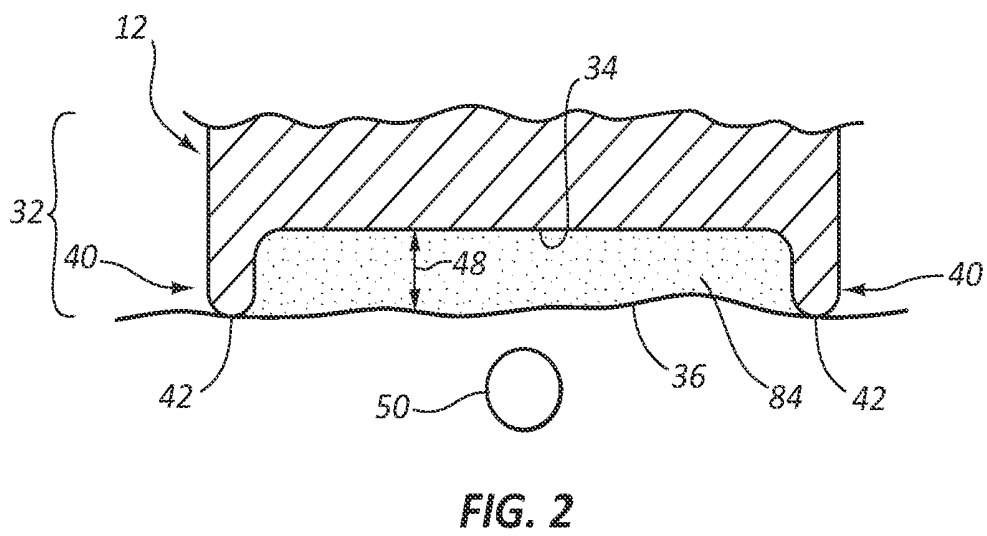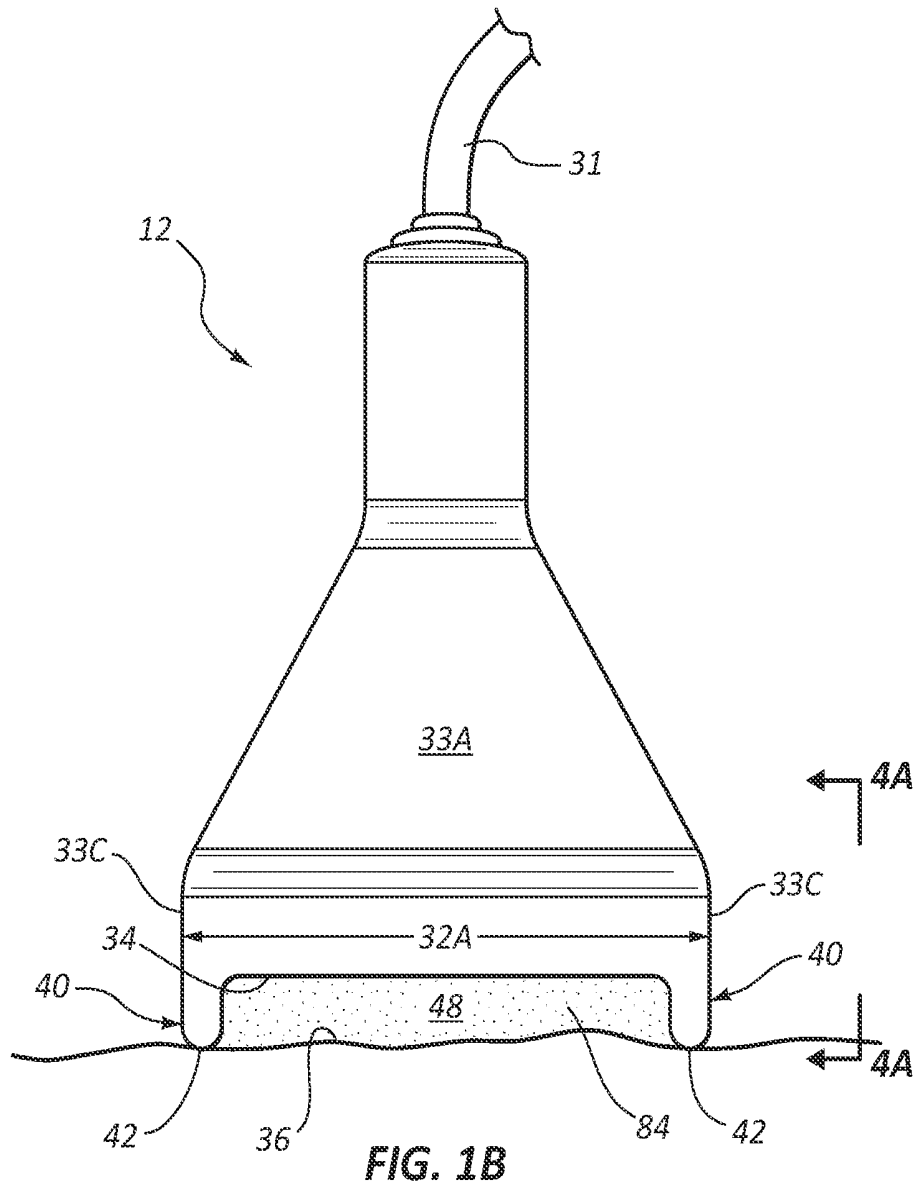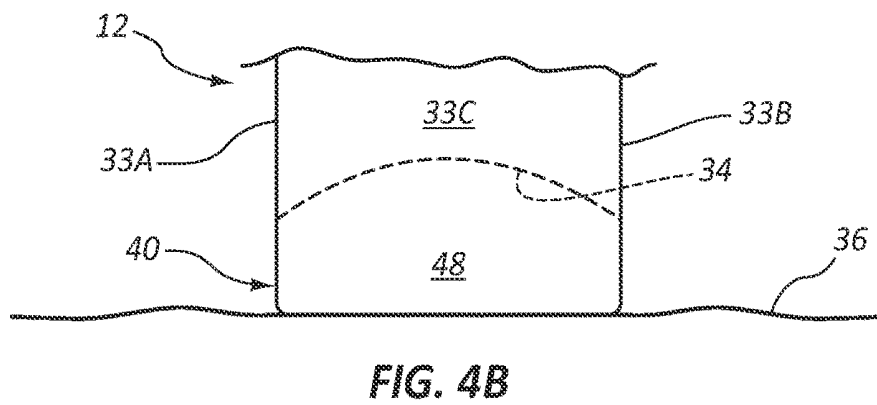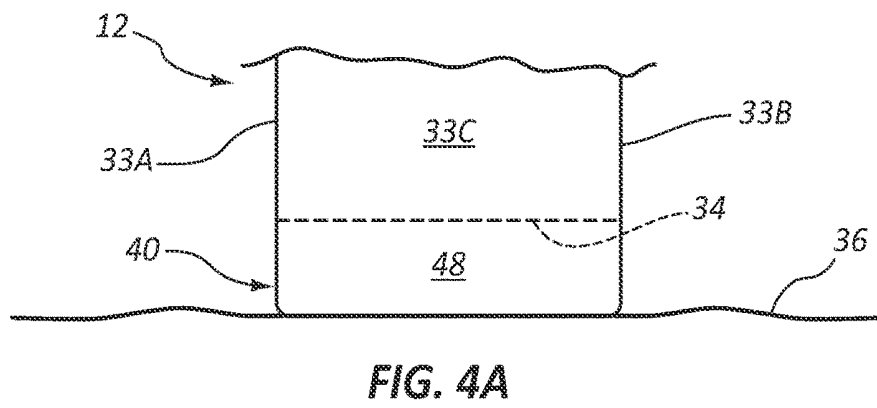

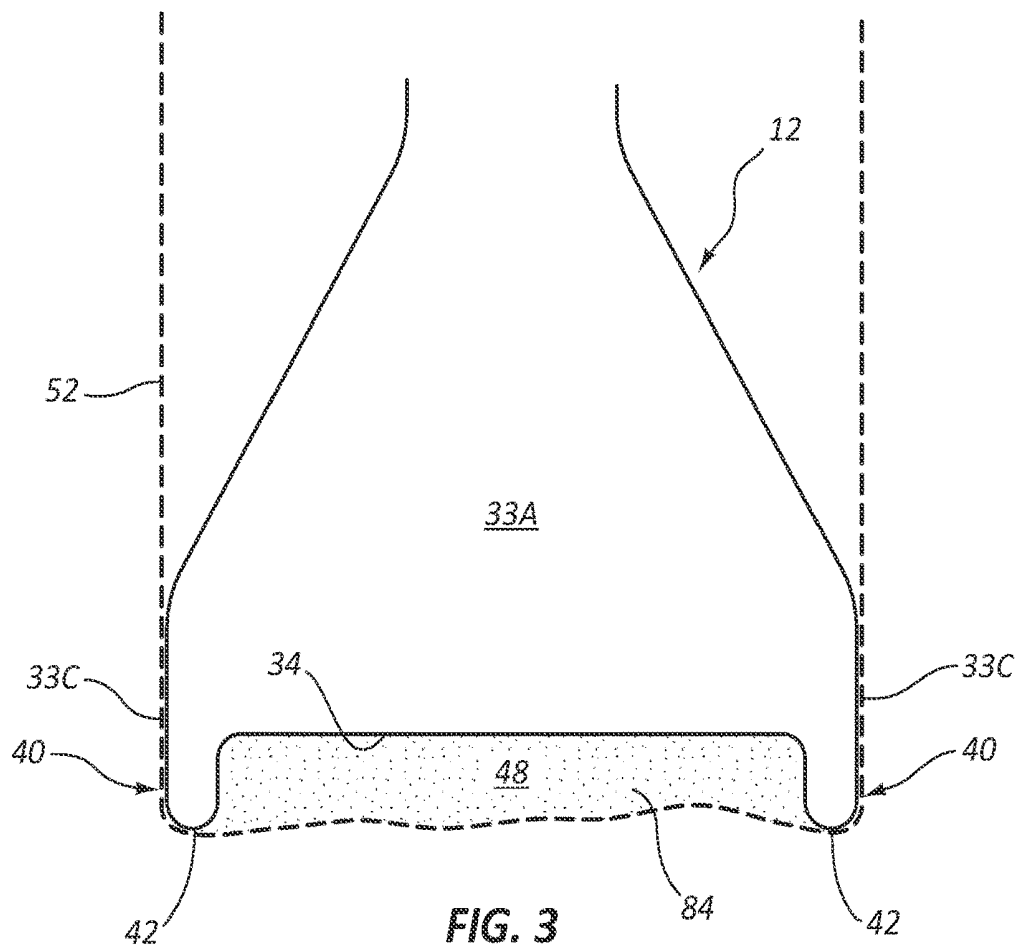


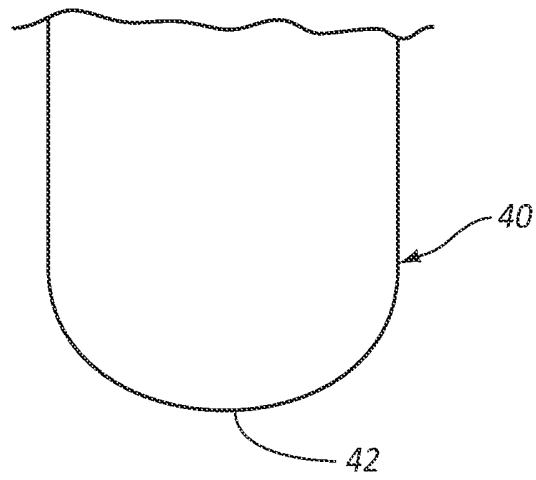

**FIG. 5**

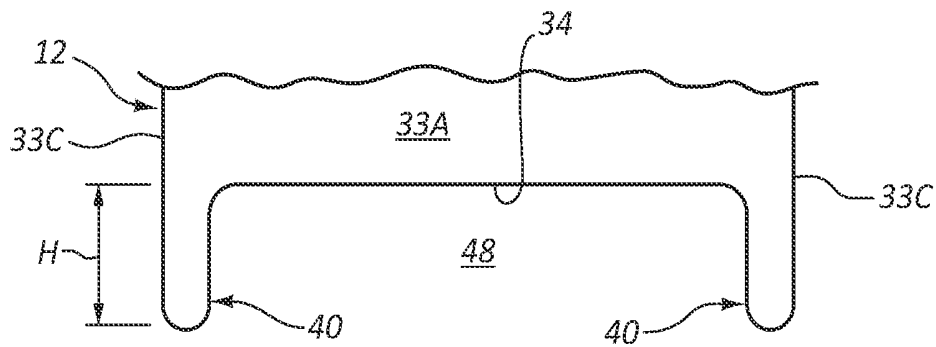

**FIG. 6**

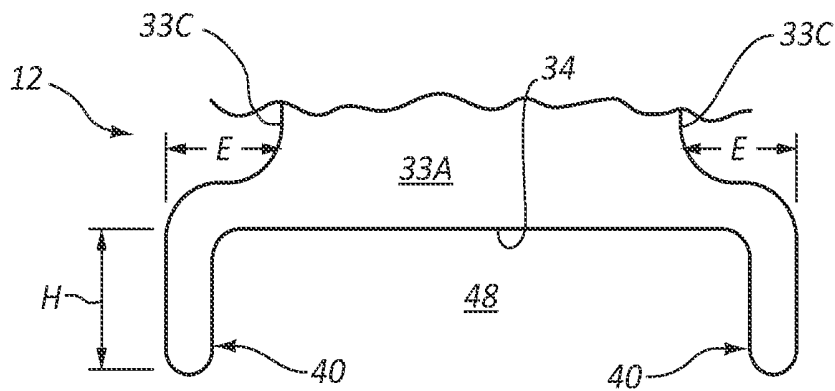

**FIG. 7**

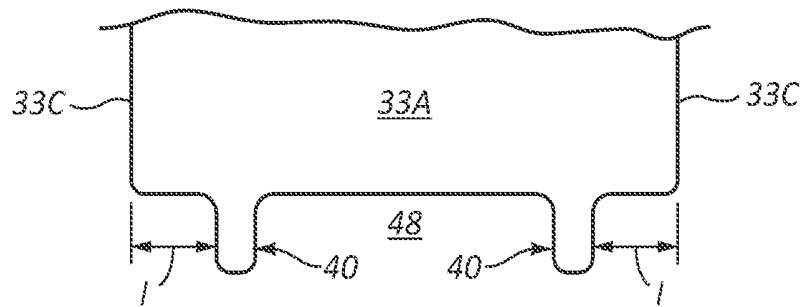


FIG. 8

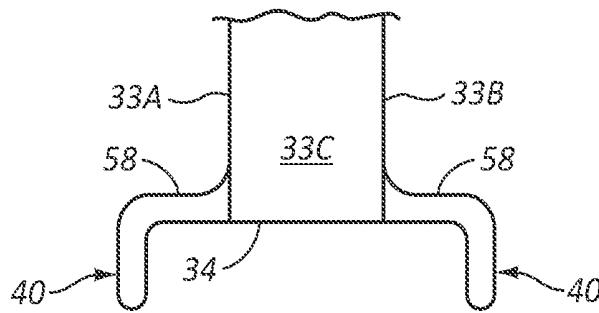


FIG. 9A

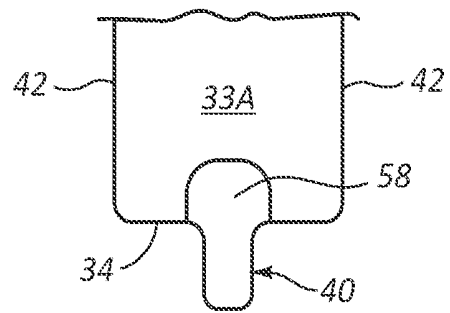


FIG. 9B



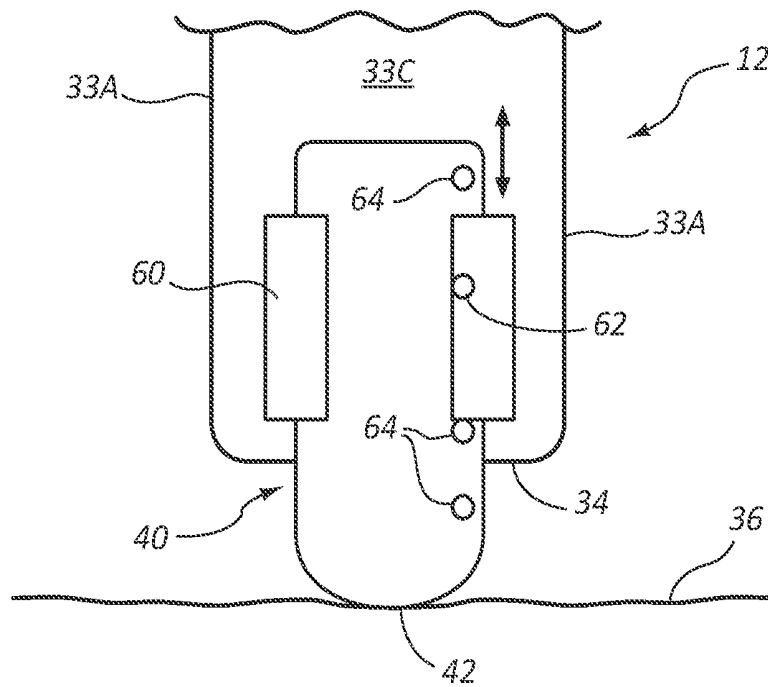



FIG. 10

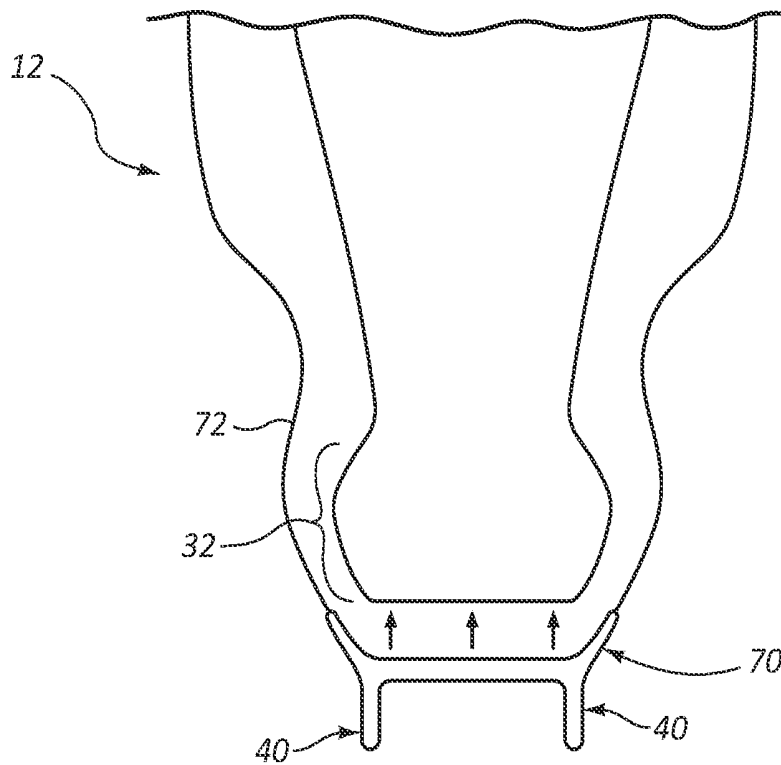


**FIG. 11**

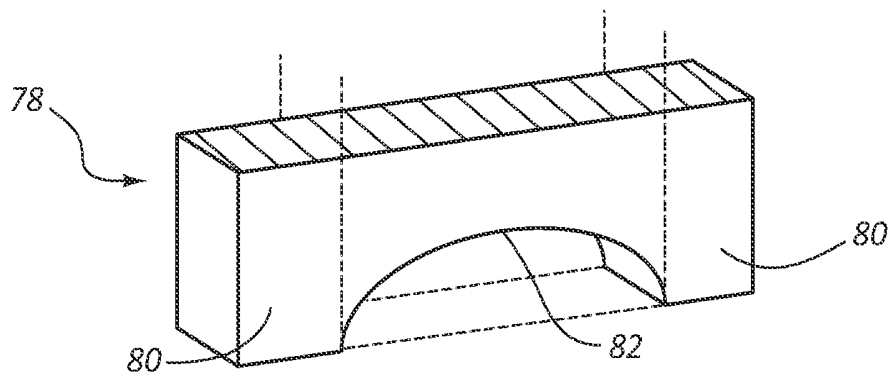


**FIG. 12**

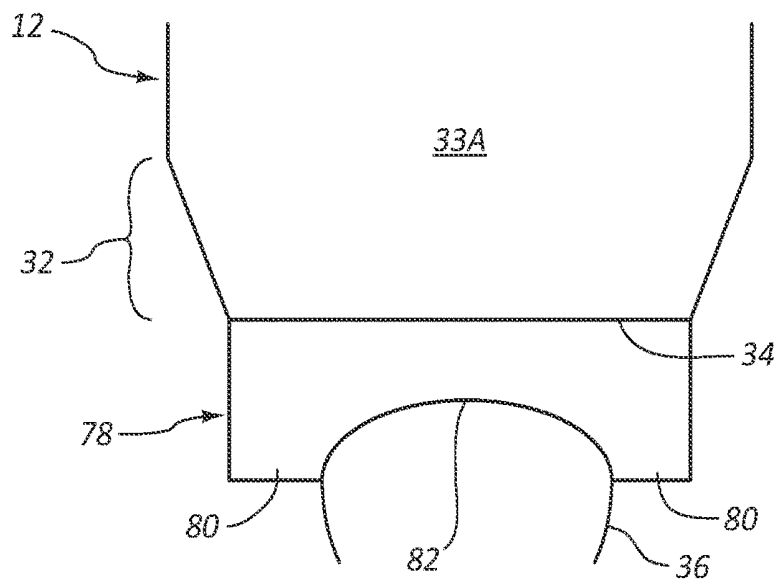

**FIG. 13A**

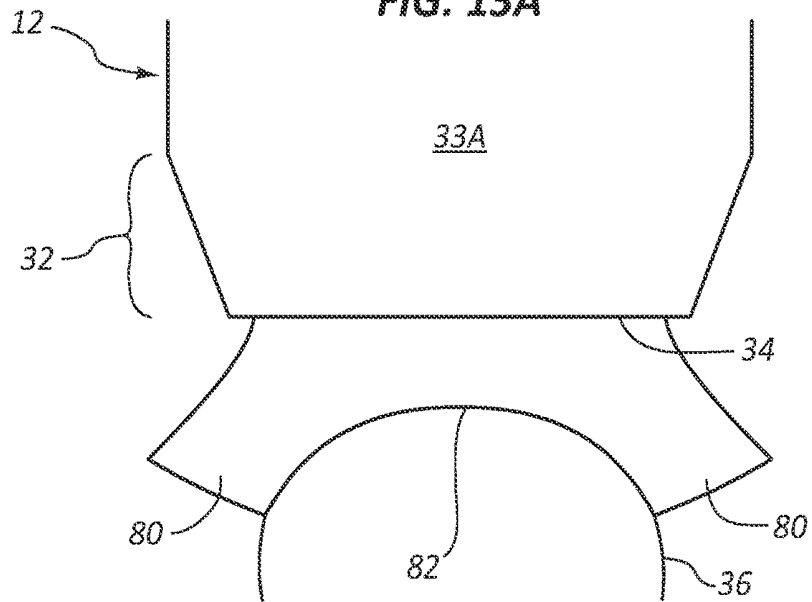


**FIG. 13B**

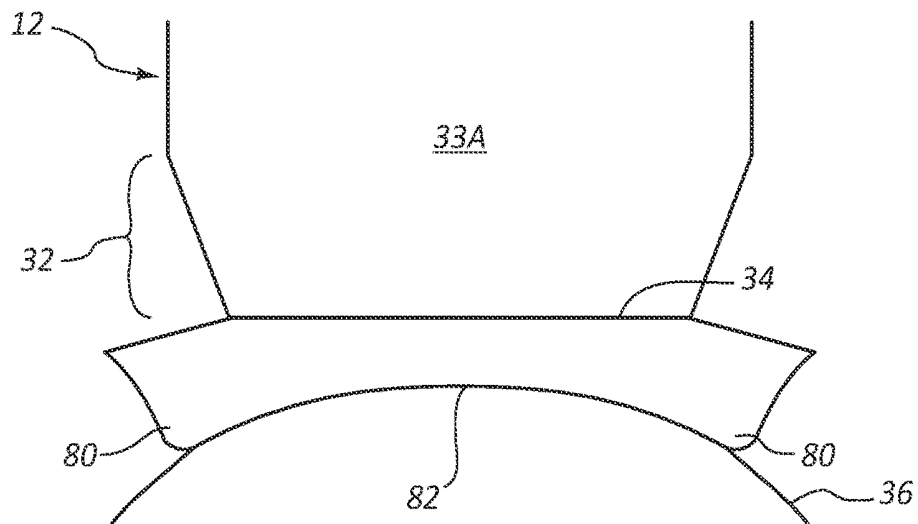


**FIG. 13C**



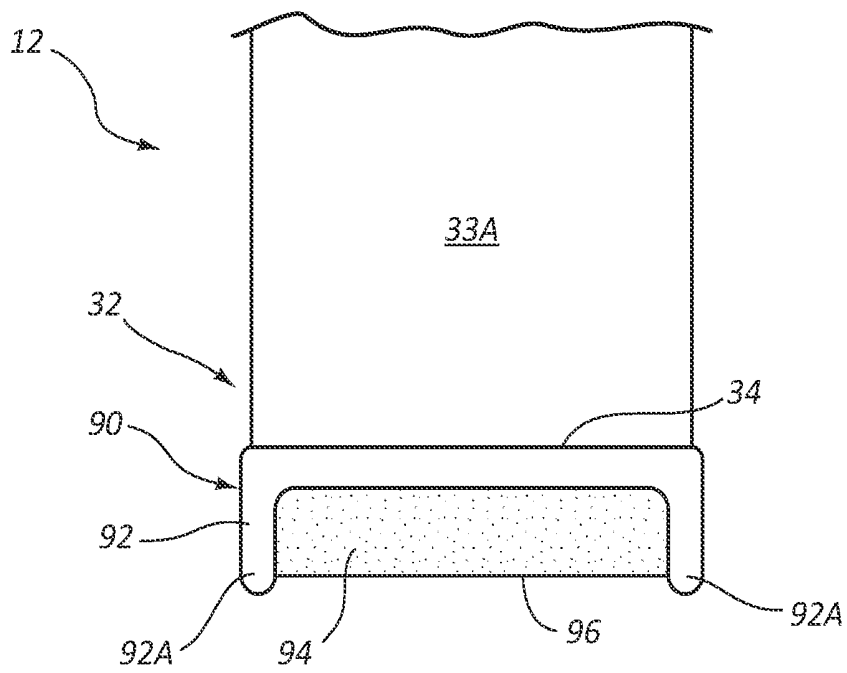

**FIG. 14**

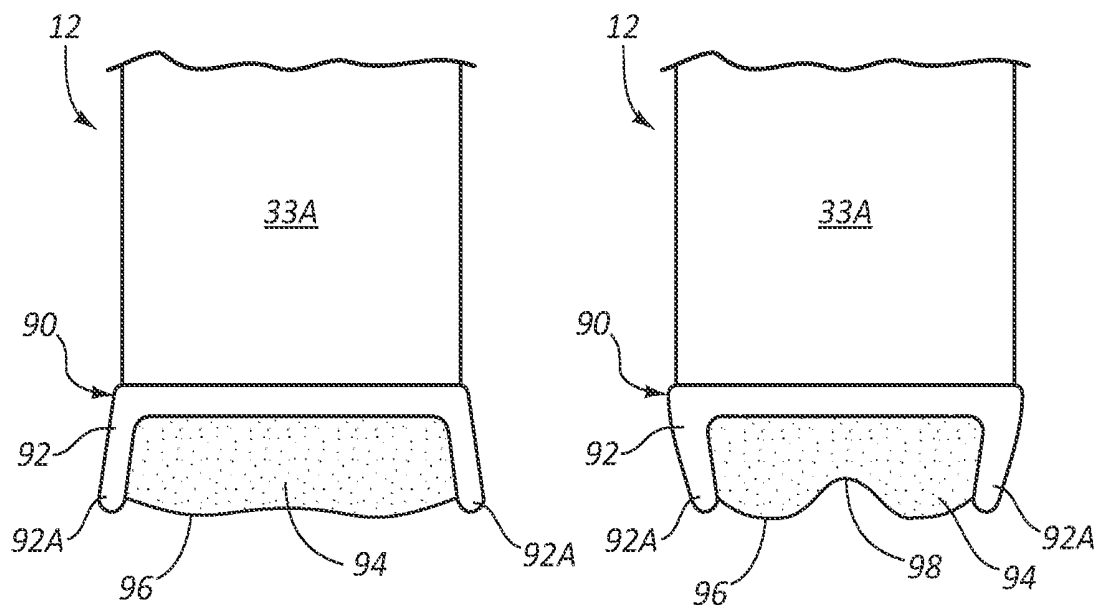

**FIG. 15A**

**FIG. 15B**

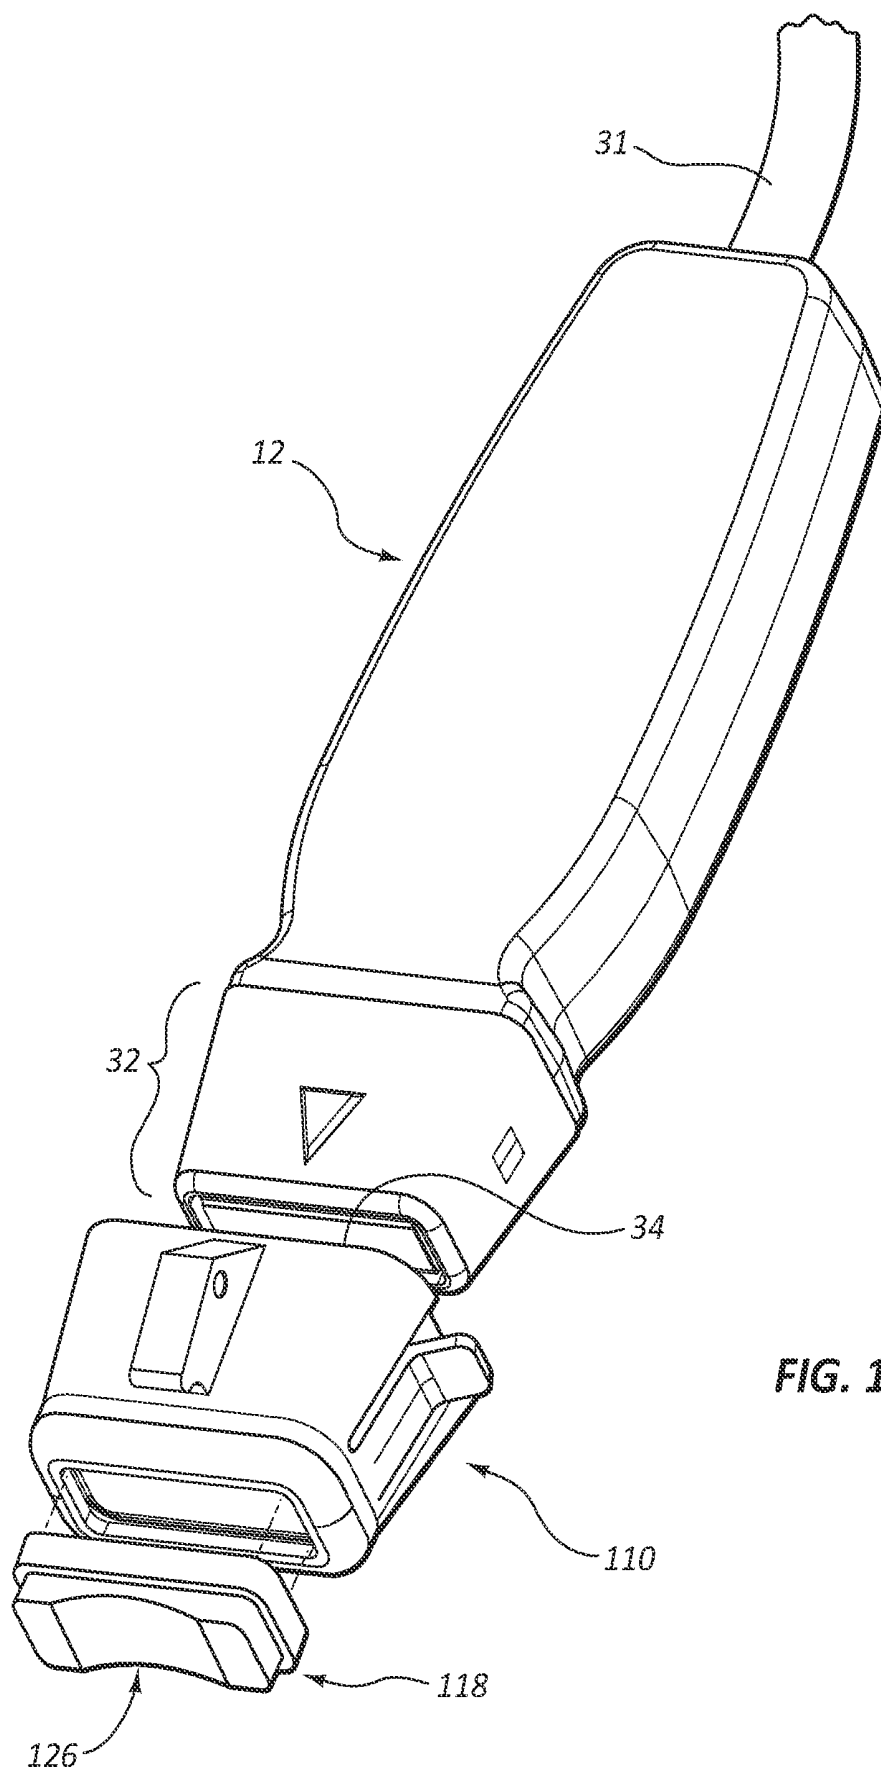


FIG. 16

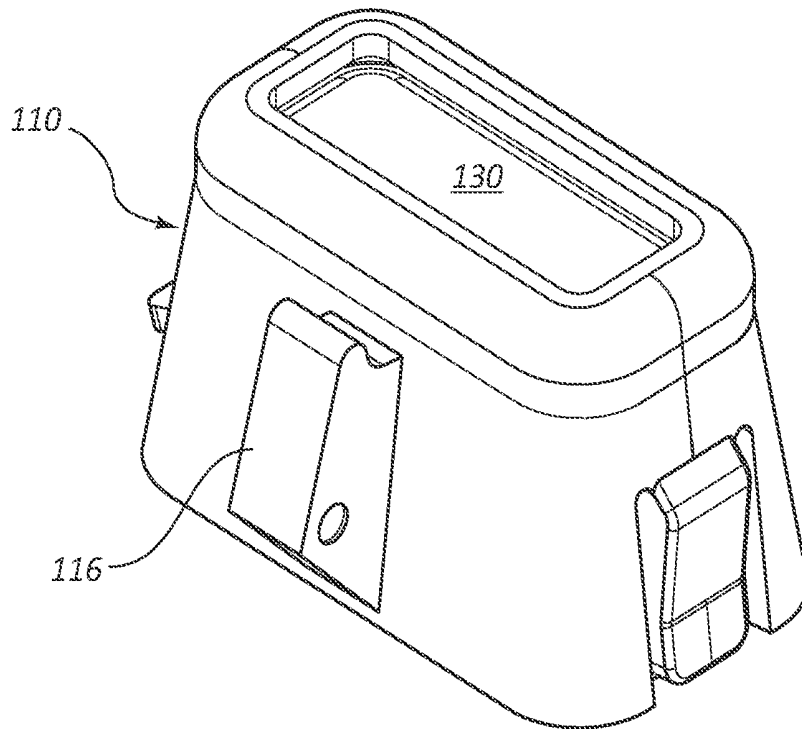


FIG. 17A



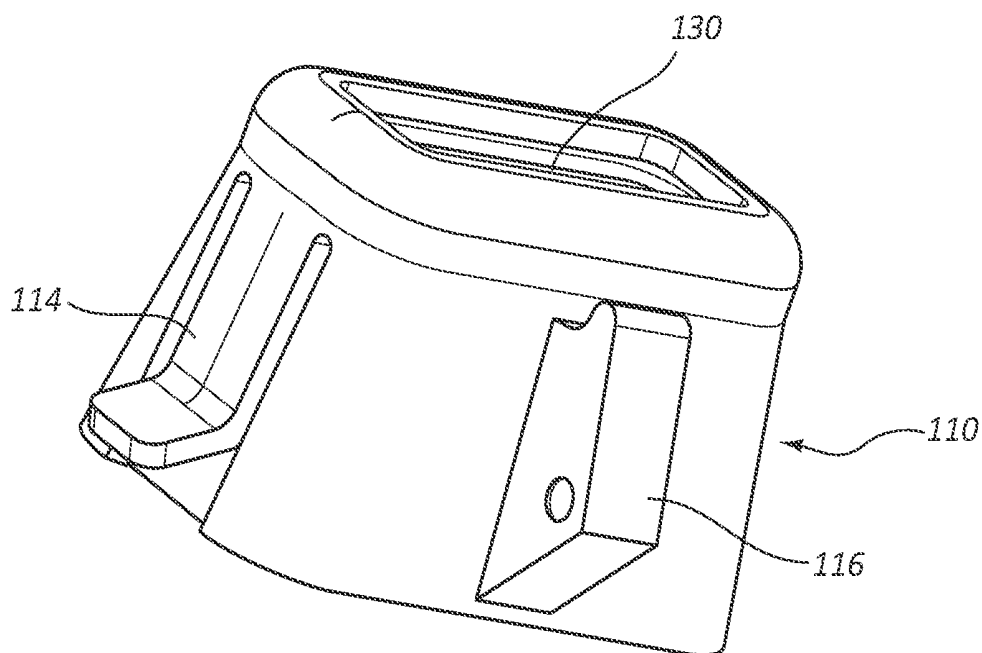


FIG. 17B

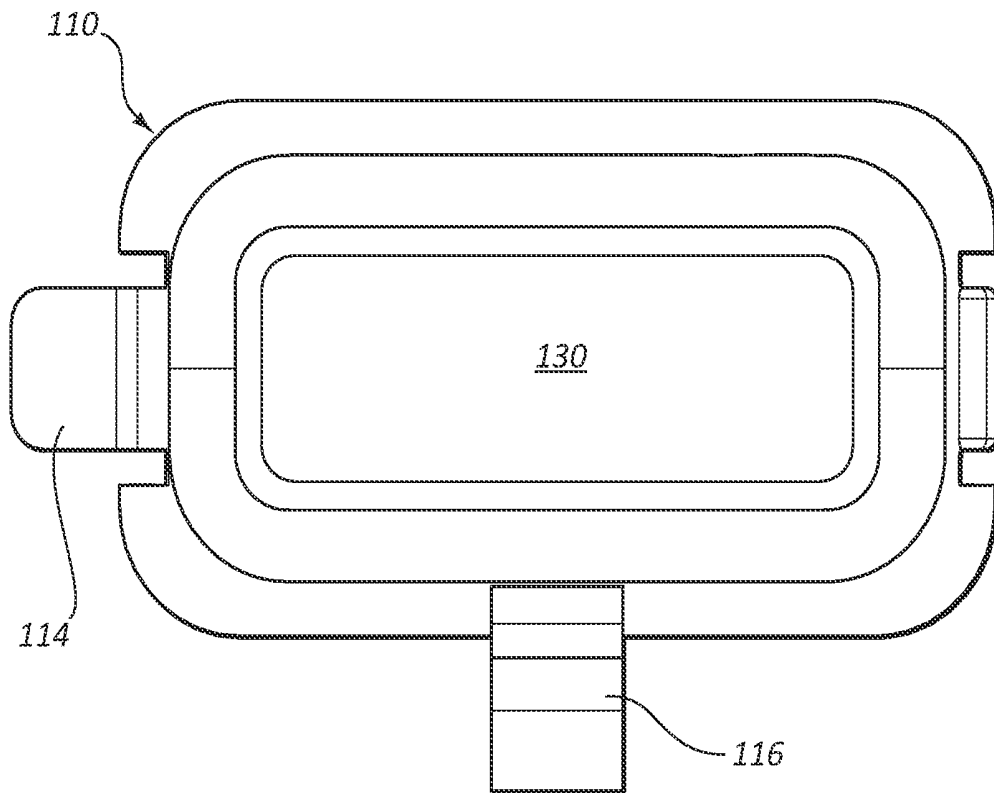

**FIG. 17C**

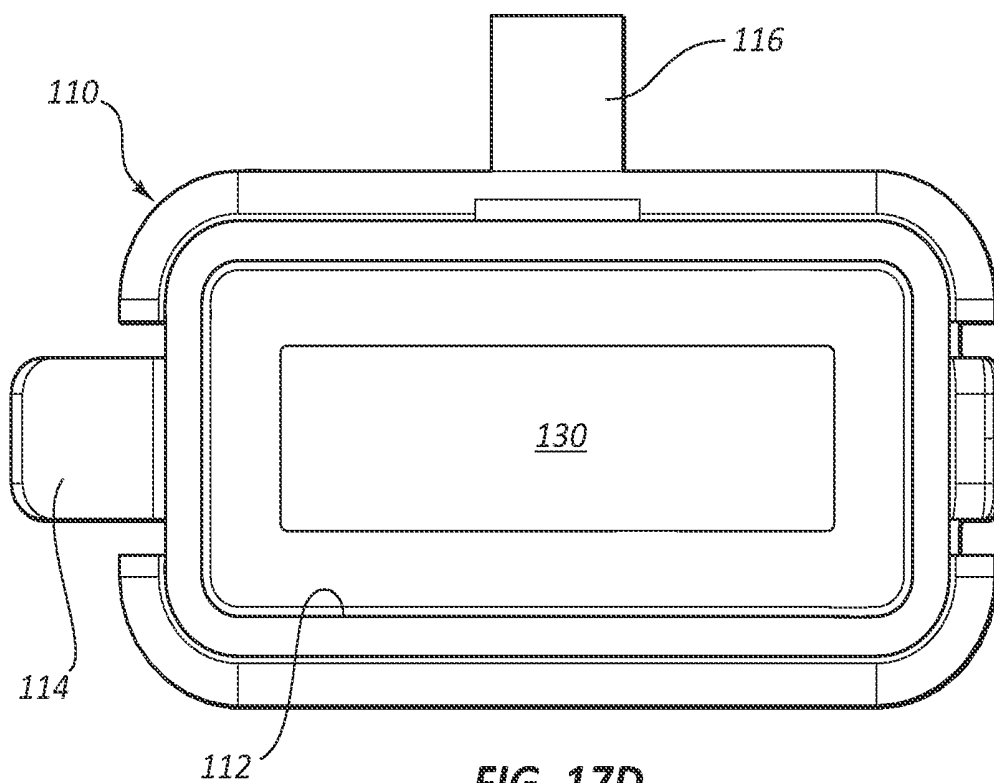

**FIG. 17D**

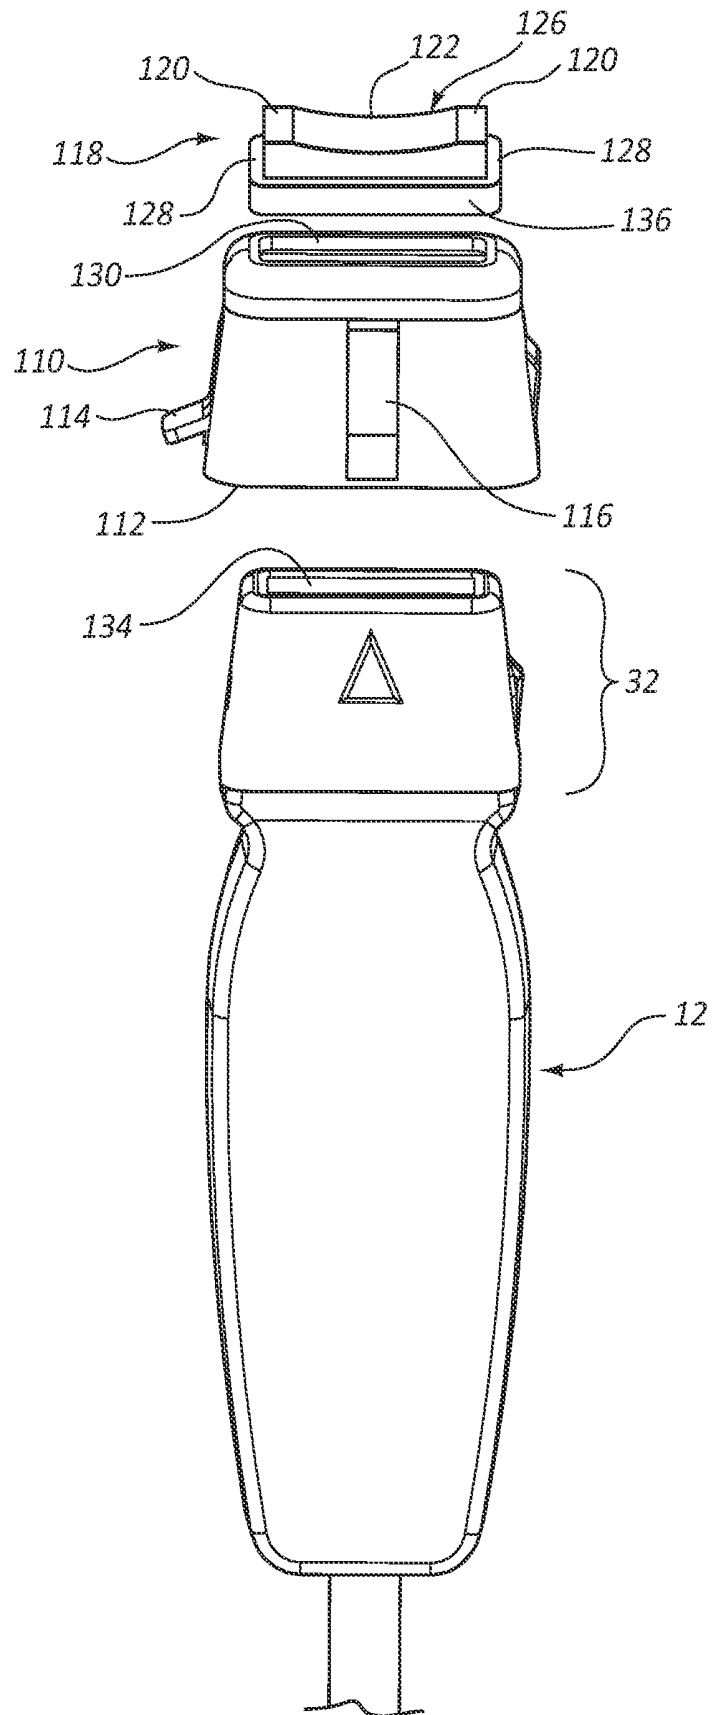


FIG. 18A

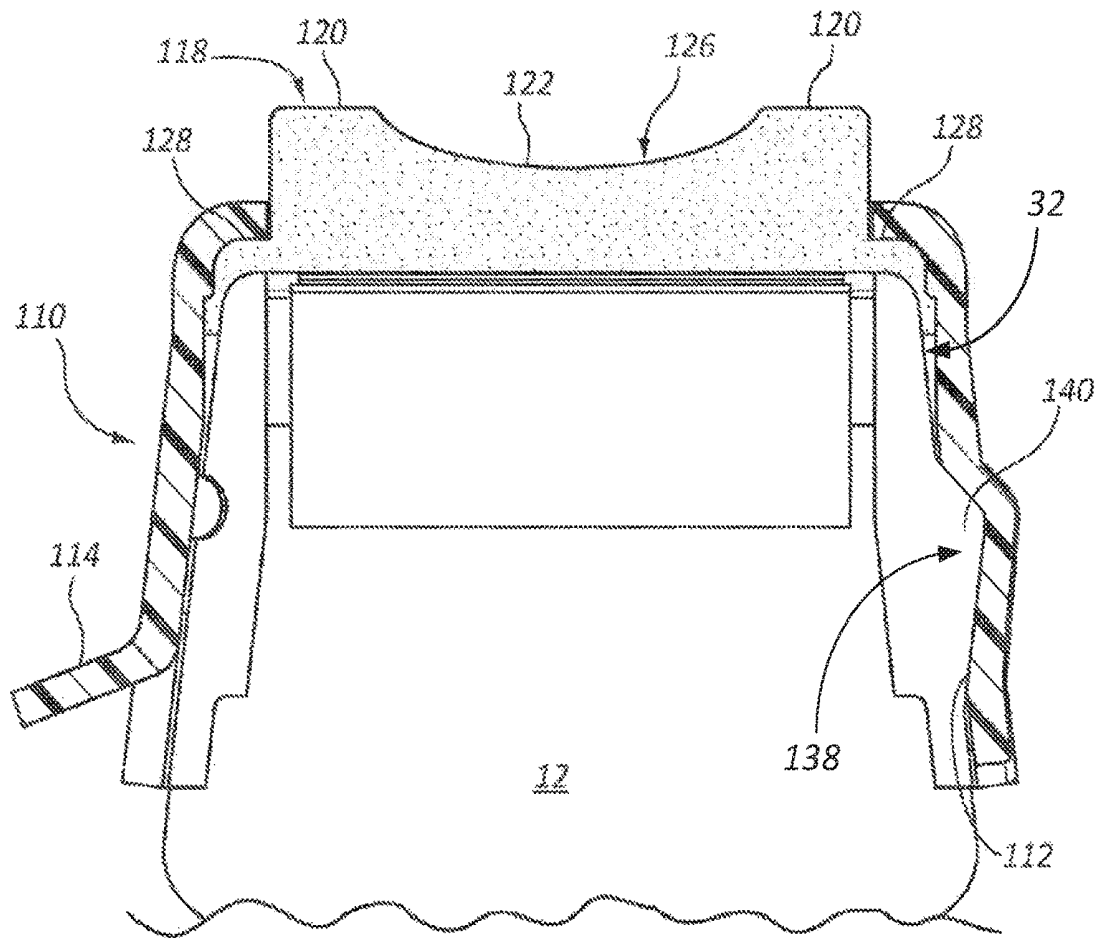


FIG. 18B

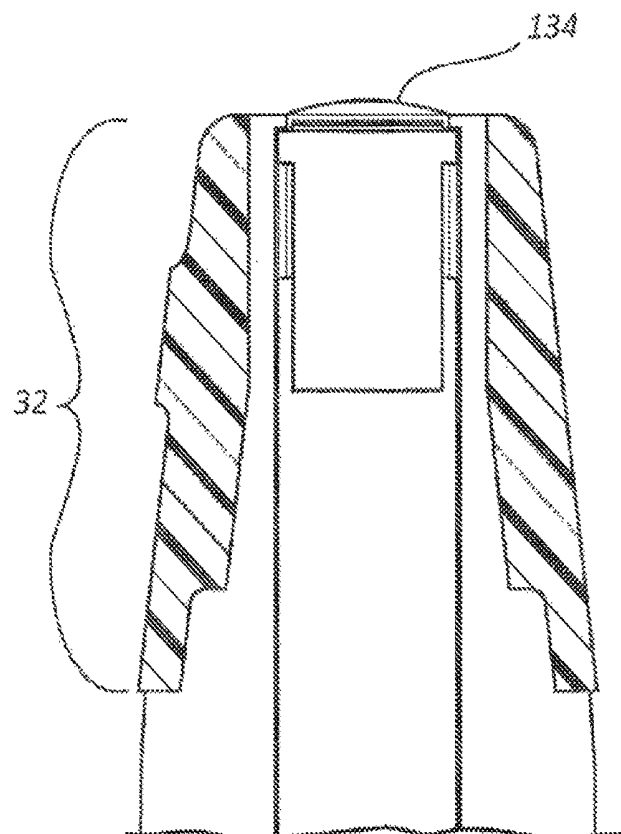


FIG. 19

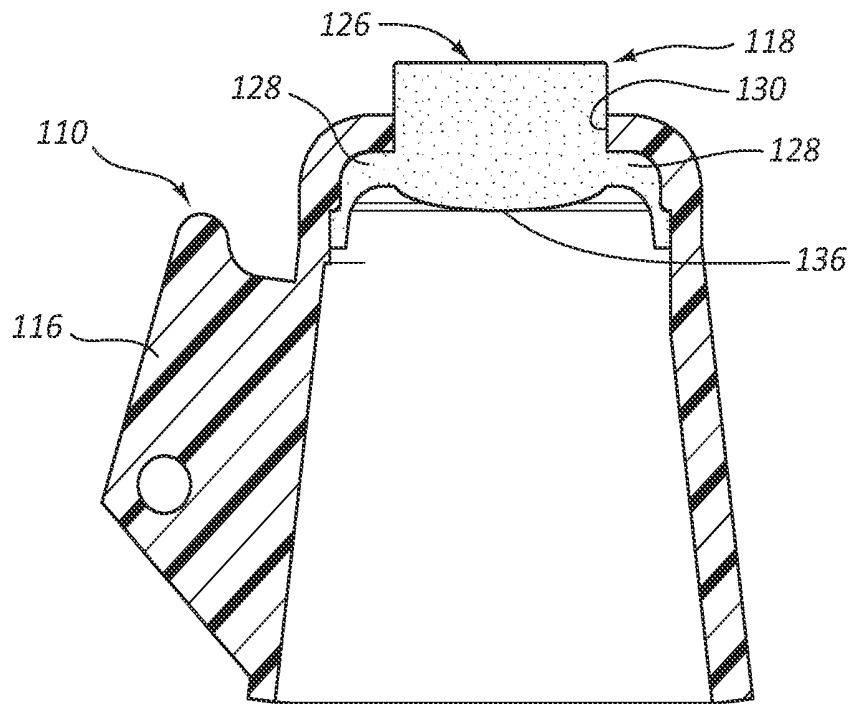


FIG. 20

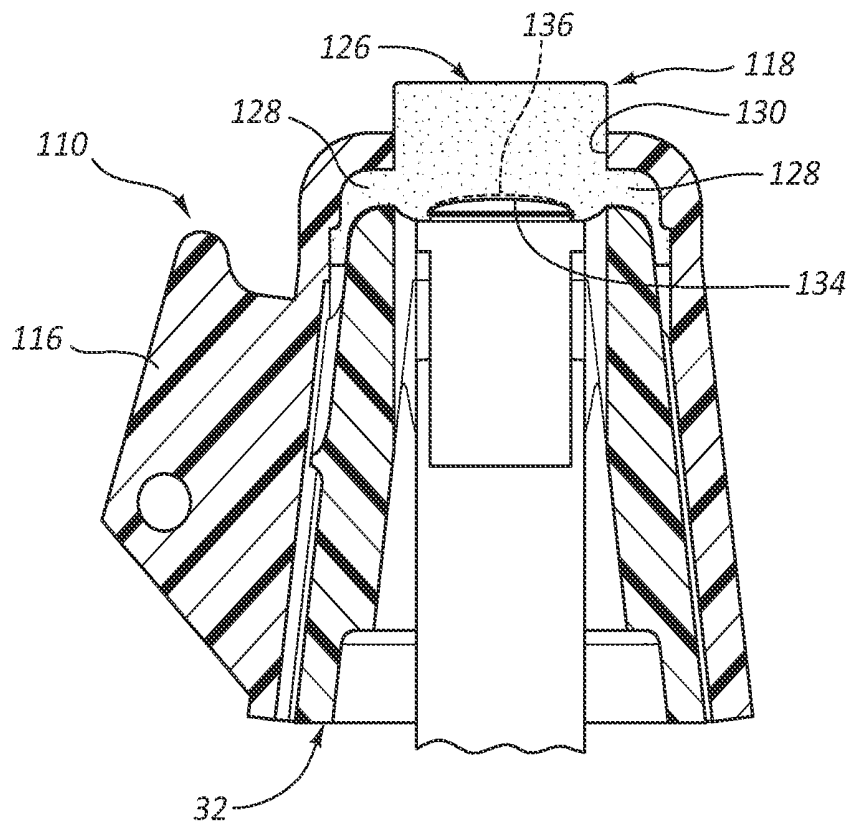


FIG. 21

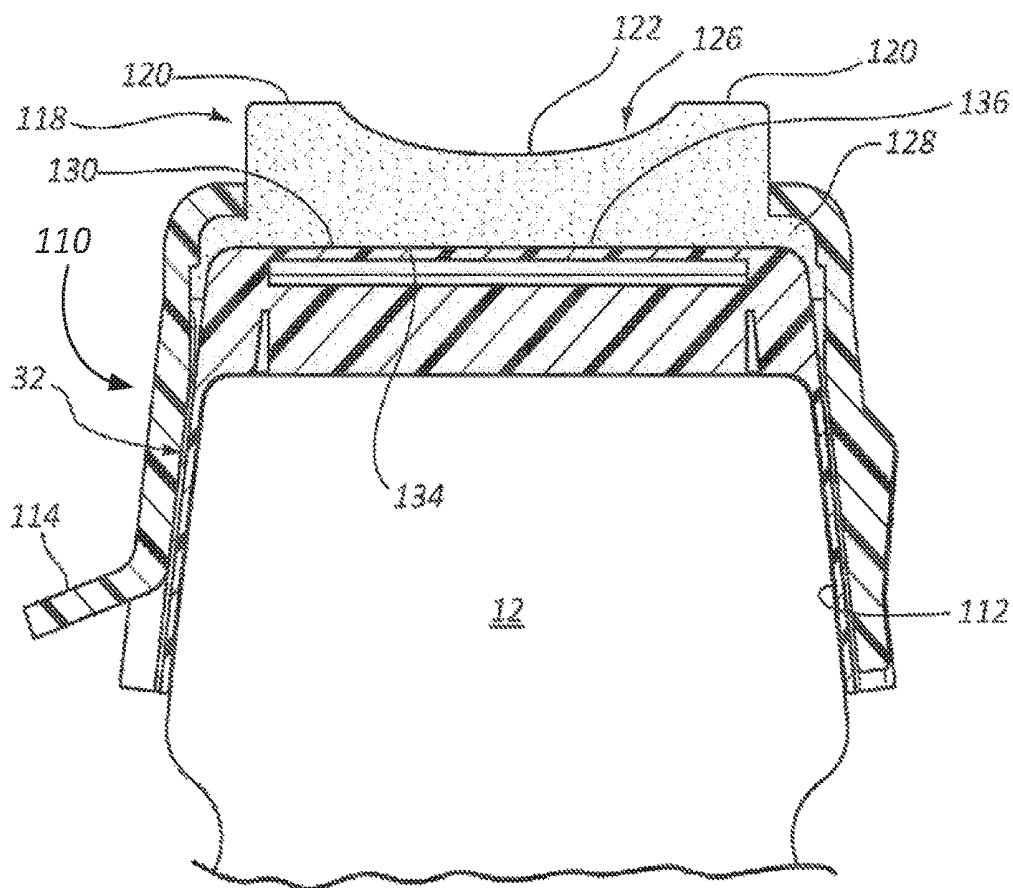


FIG. 22

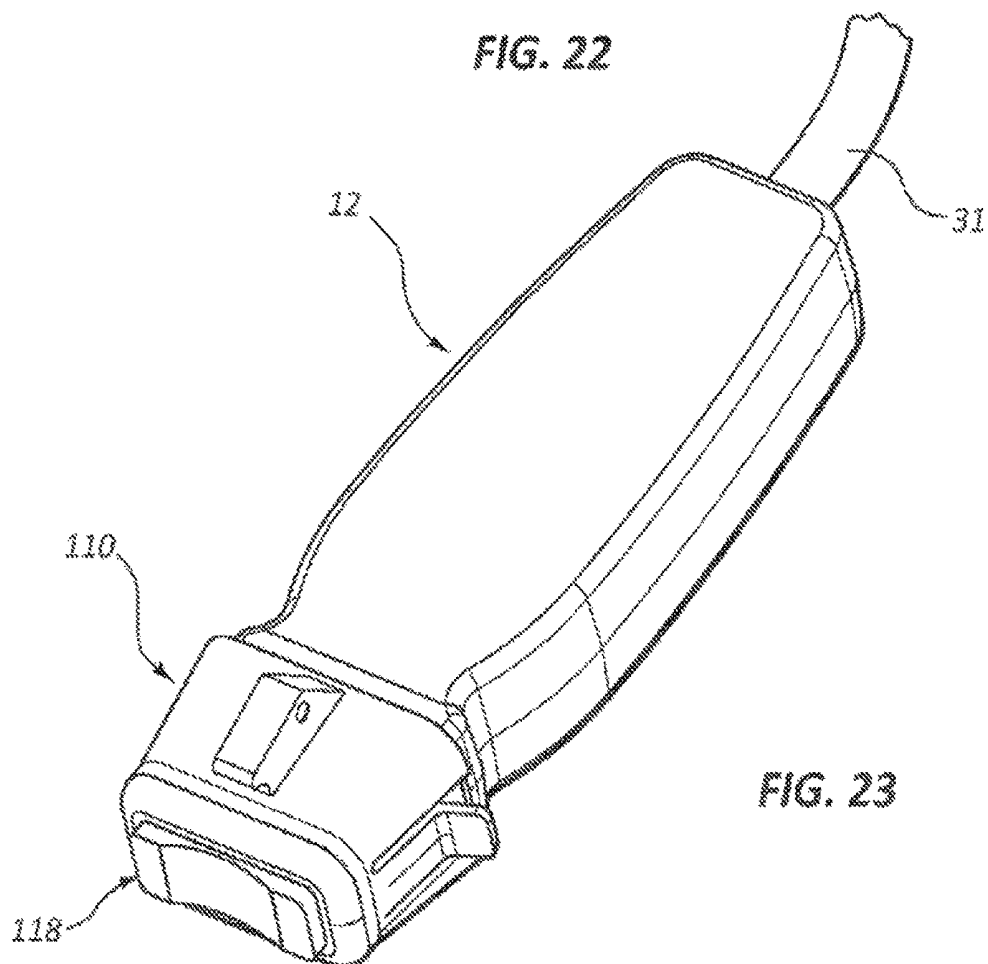


FIG. 23



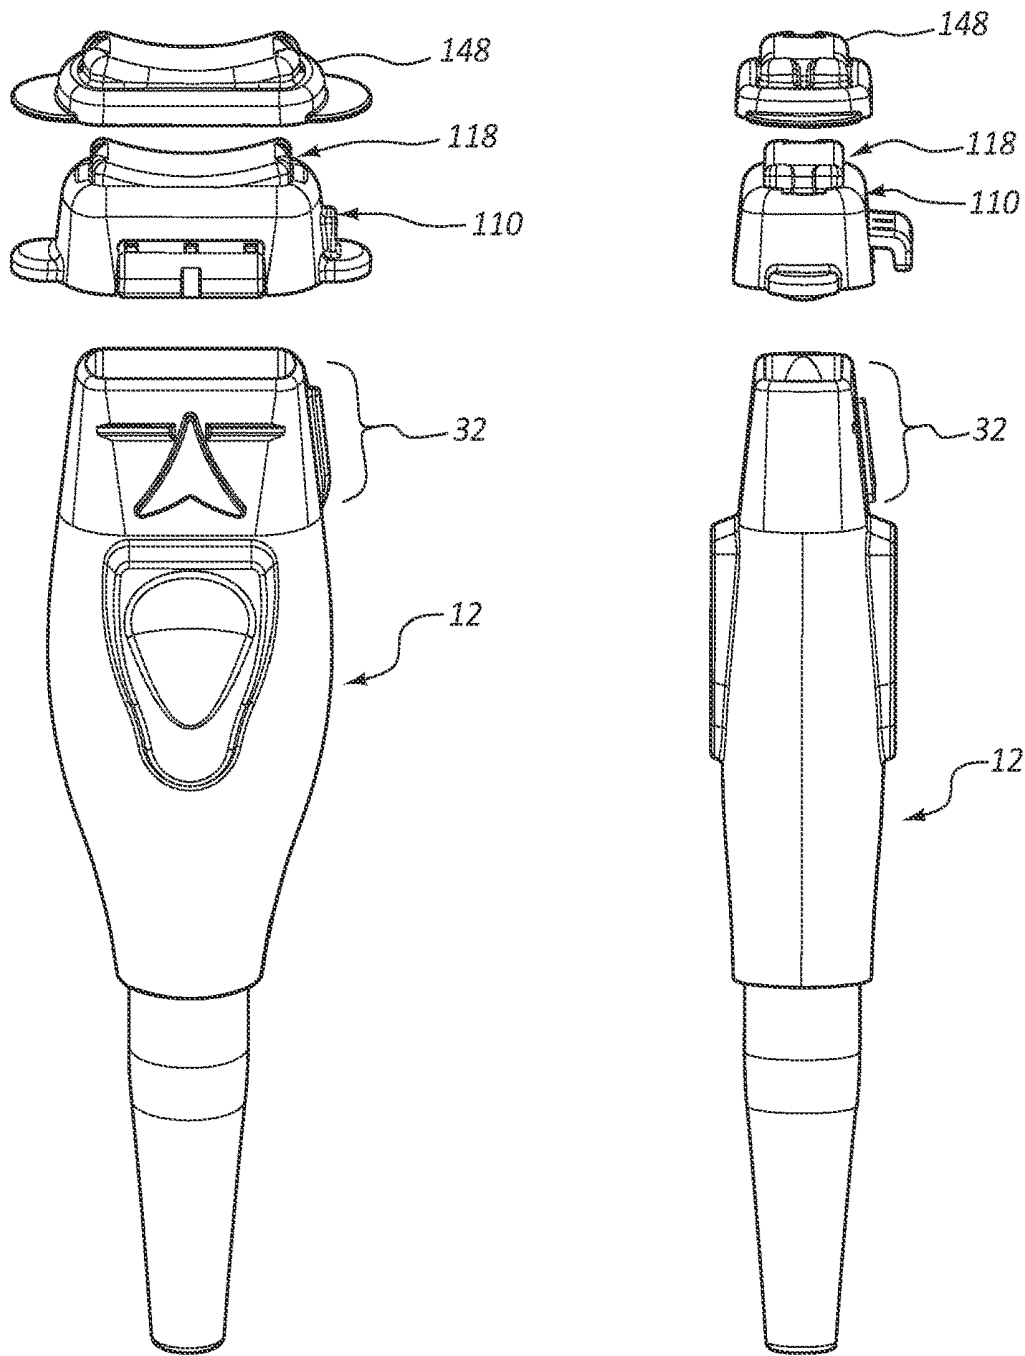


FIG. 24A

FIG. 24B

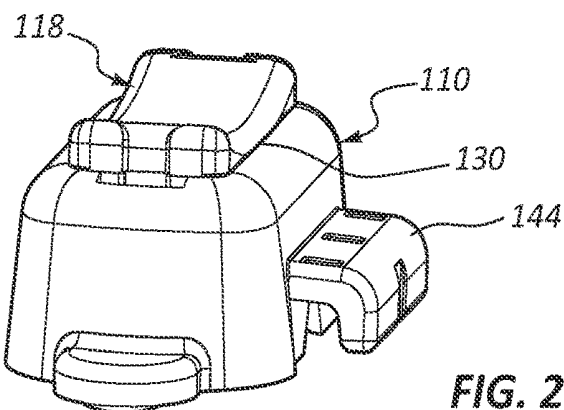
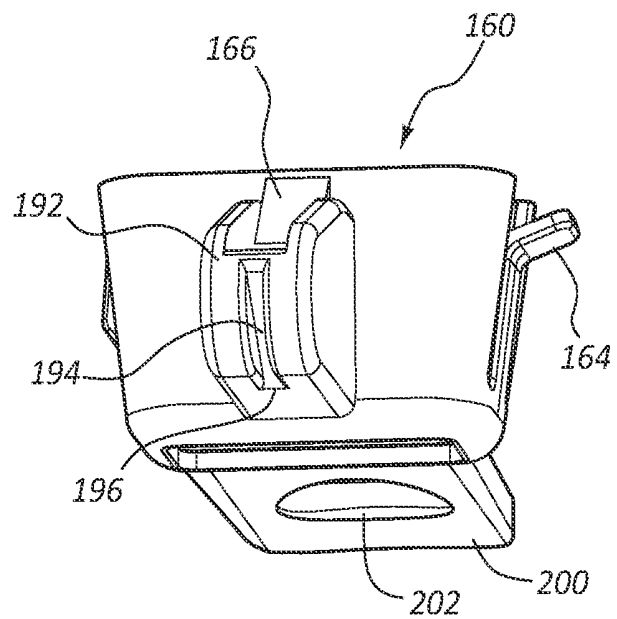
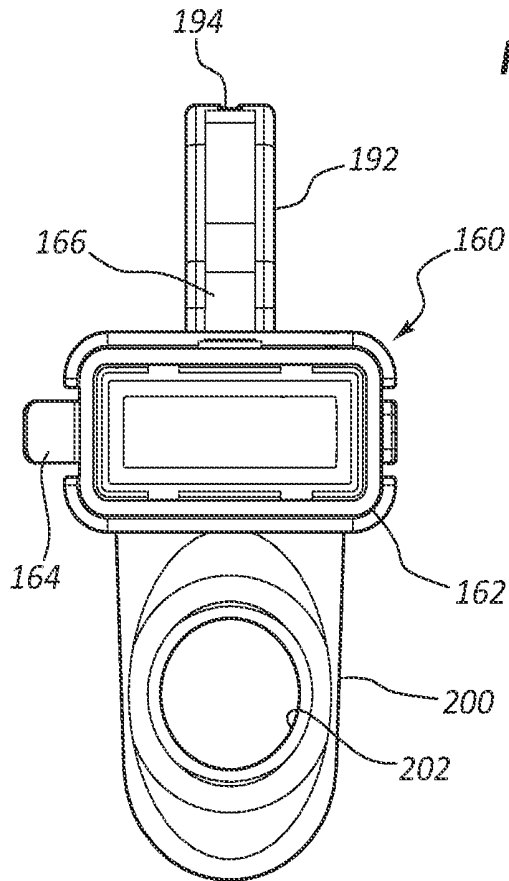
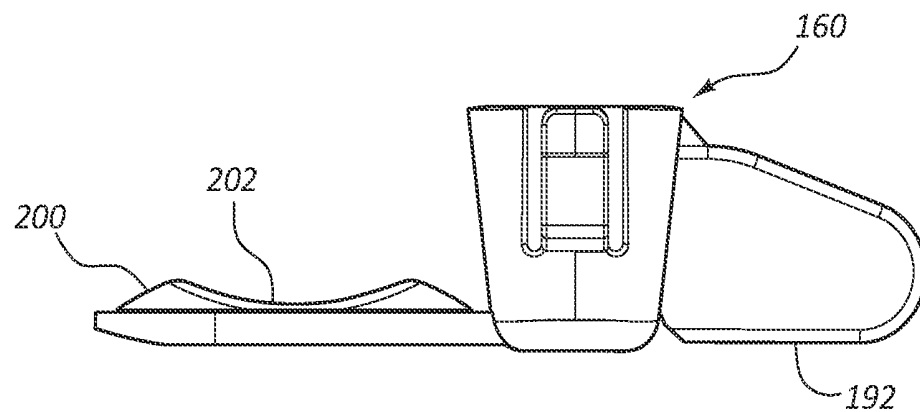
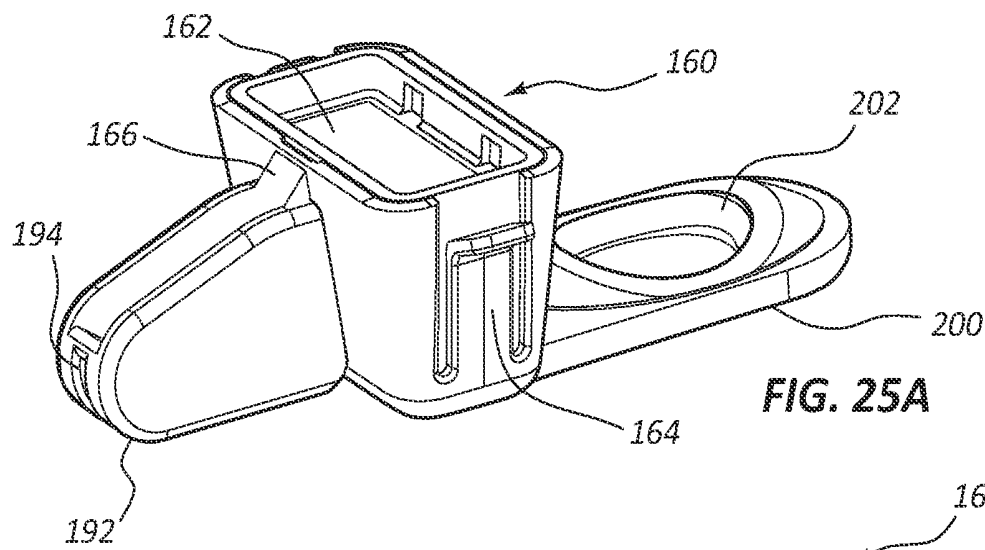


FIG. 24C



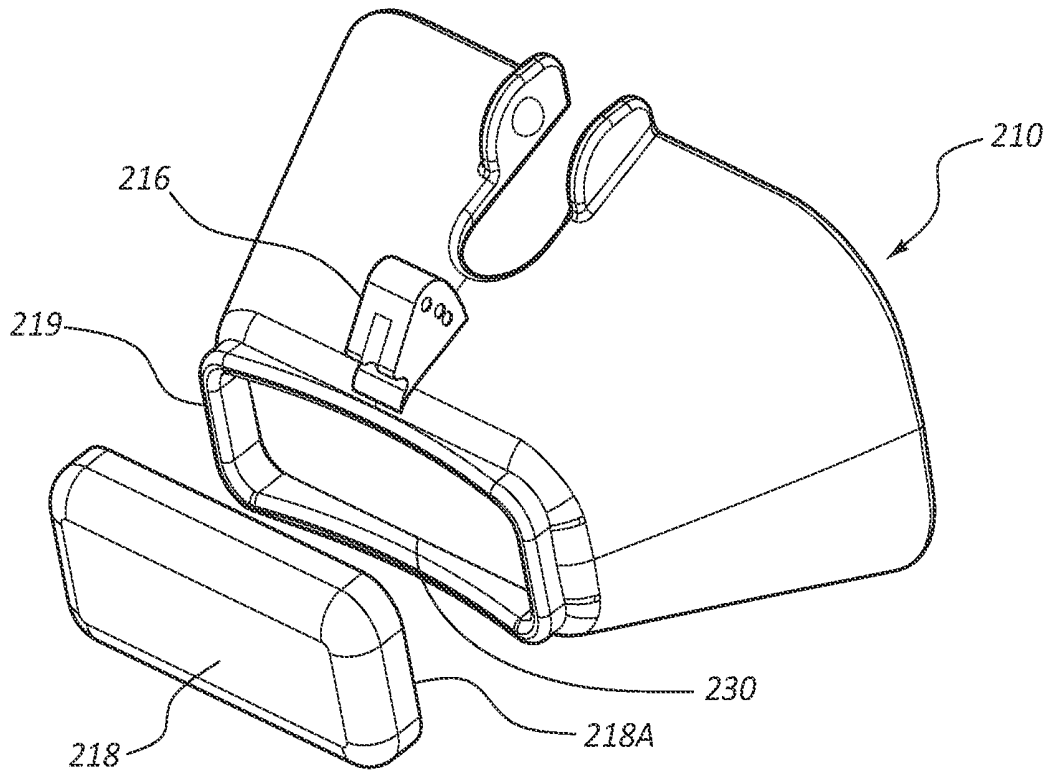


FIG. 26A

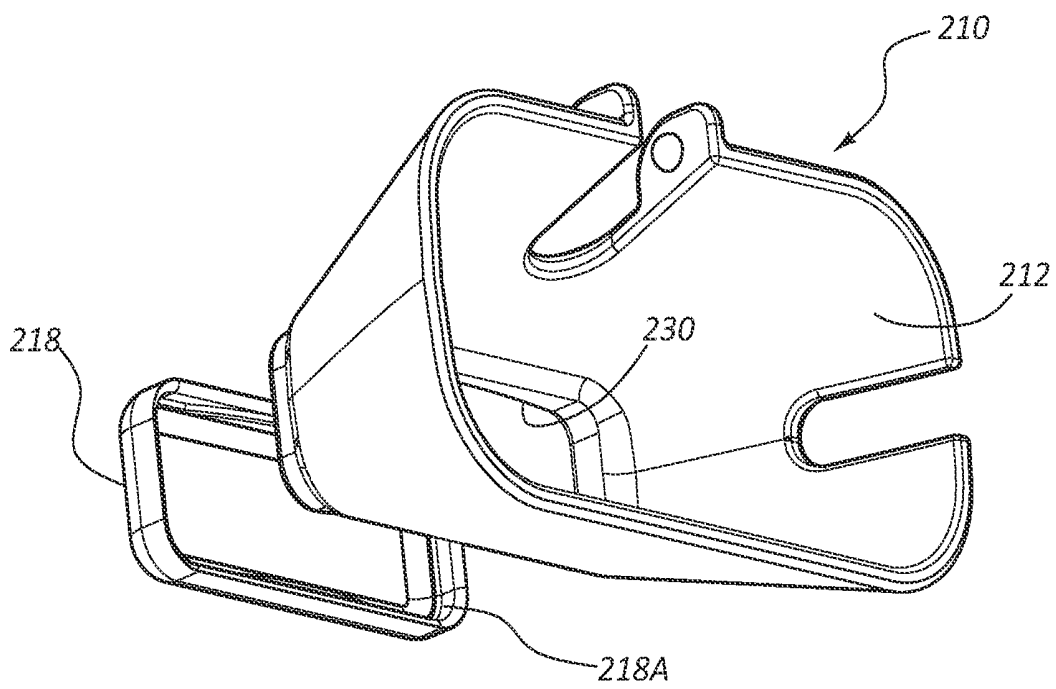


FIG. 26B

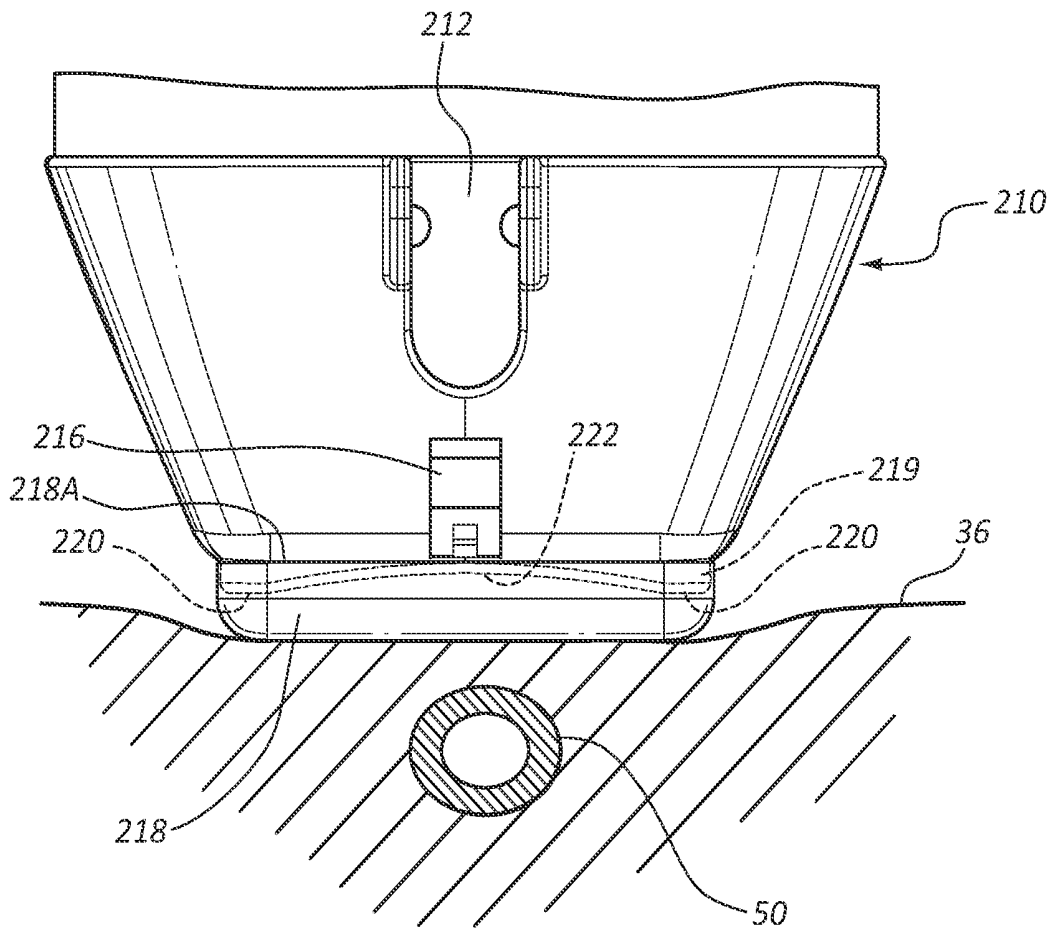


FIG. 27

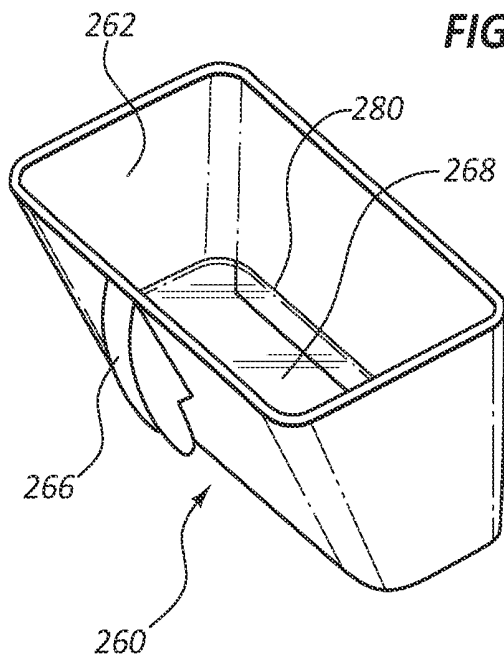


FIG. 28A

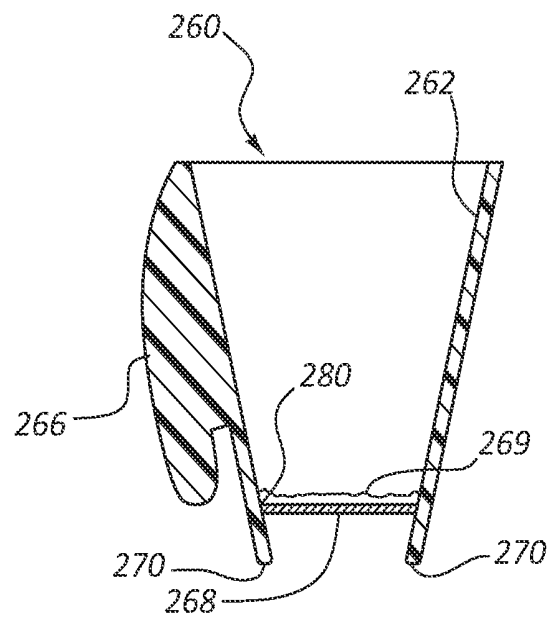


FIG. 28B

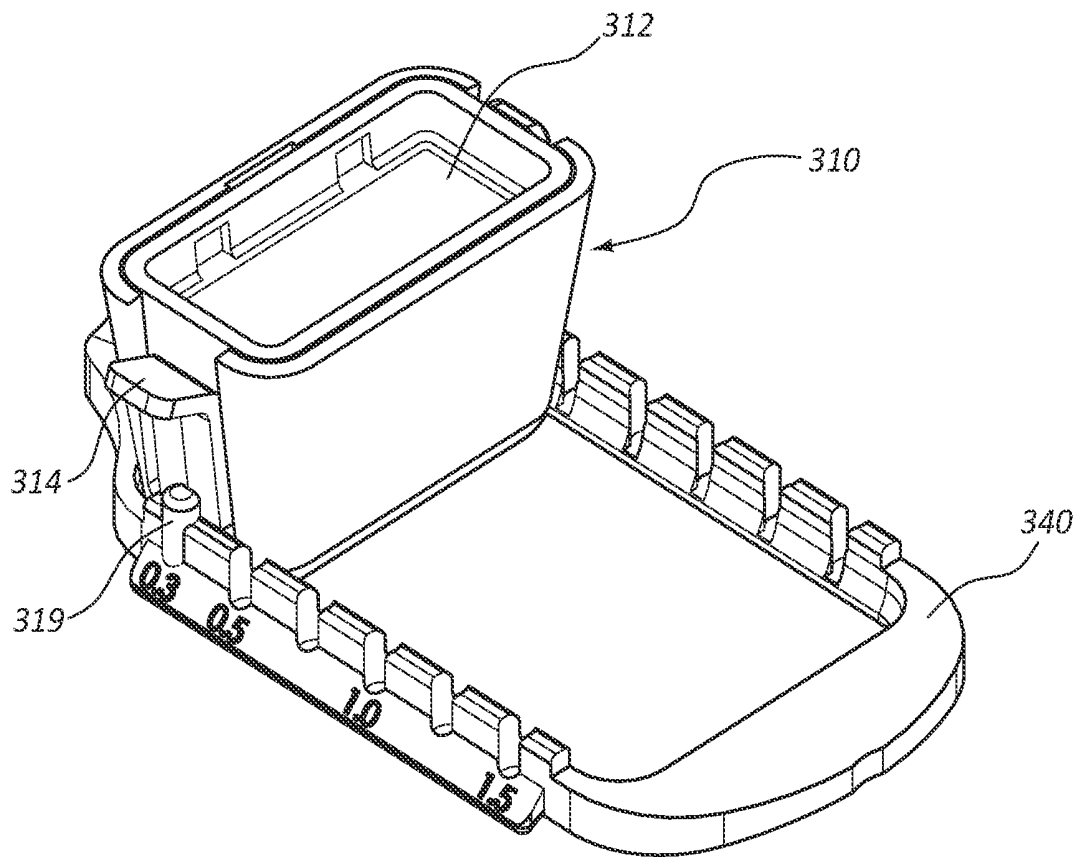


FIG. 29A

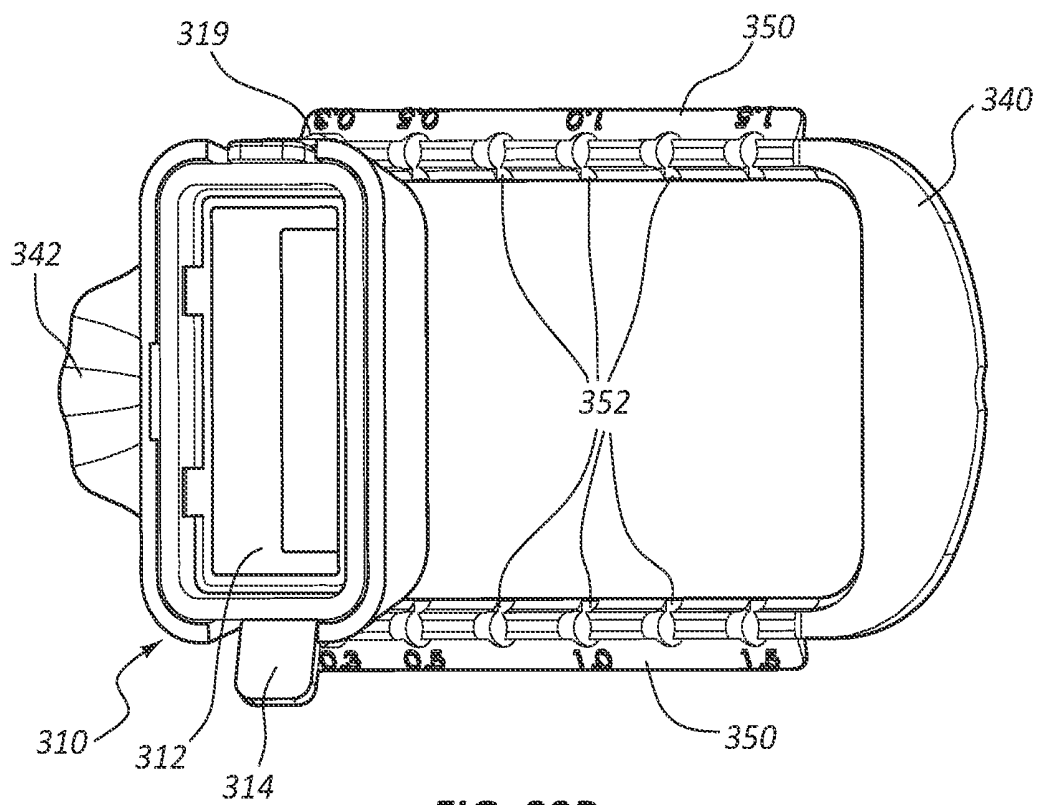


FIG. 29B

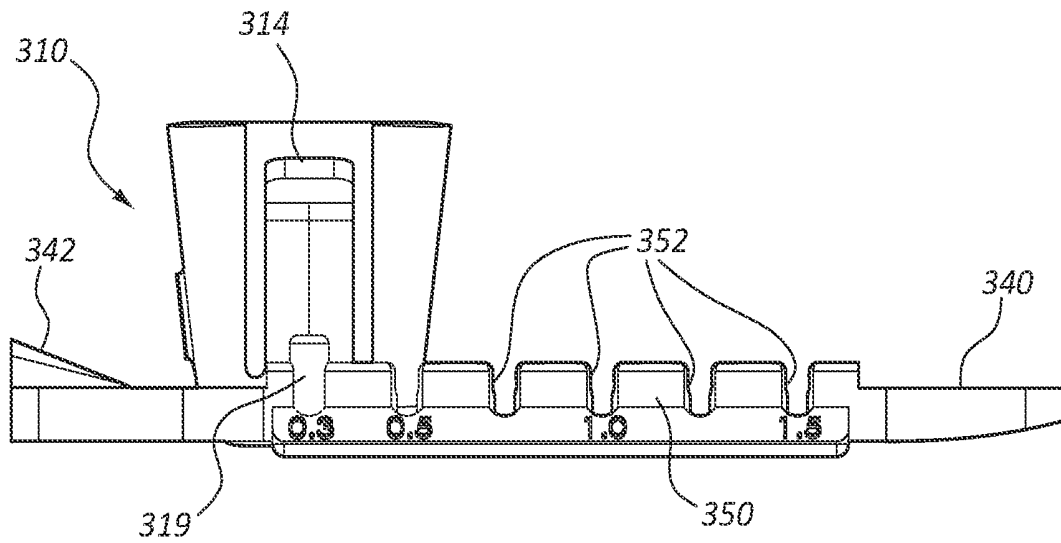


FIG. 29C



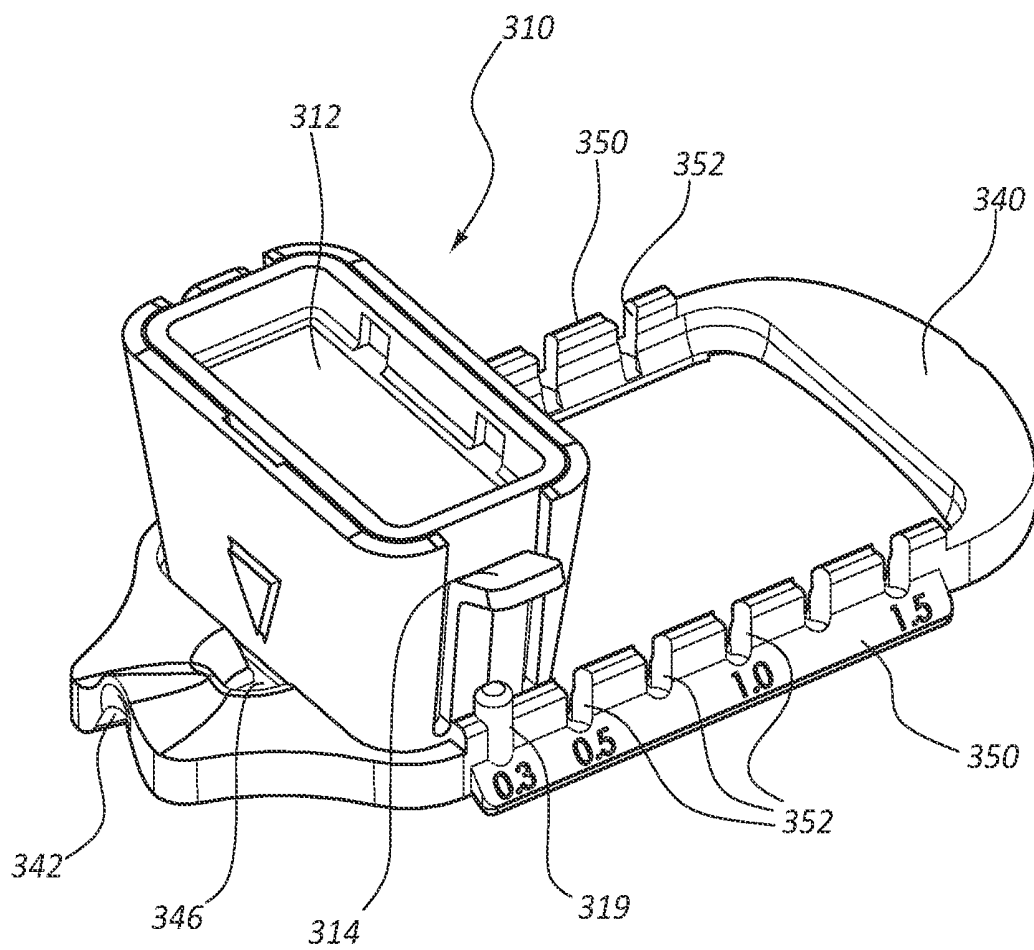


FIG. 29D

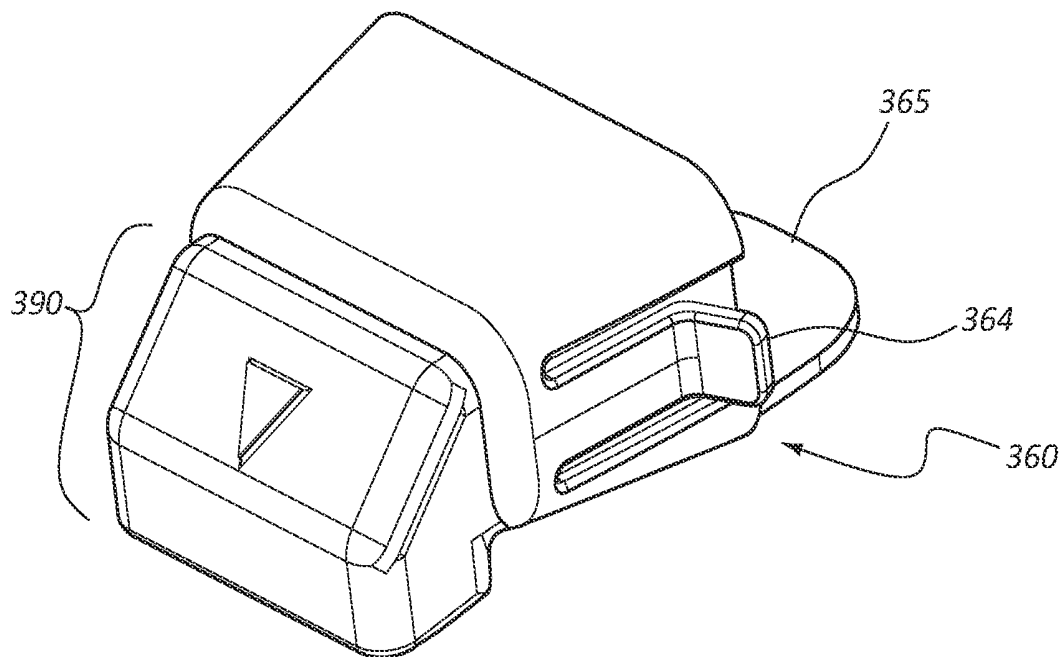

**FIG. 30A**

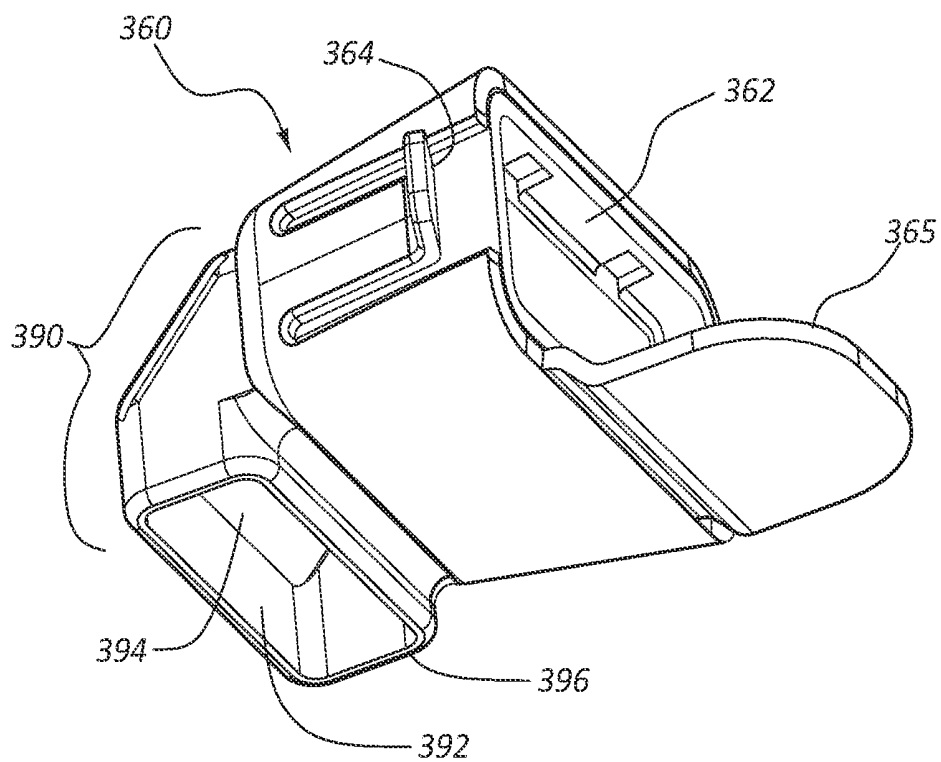

**FIG. 30B**

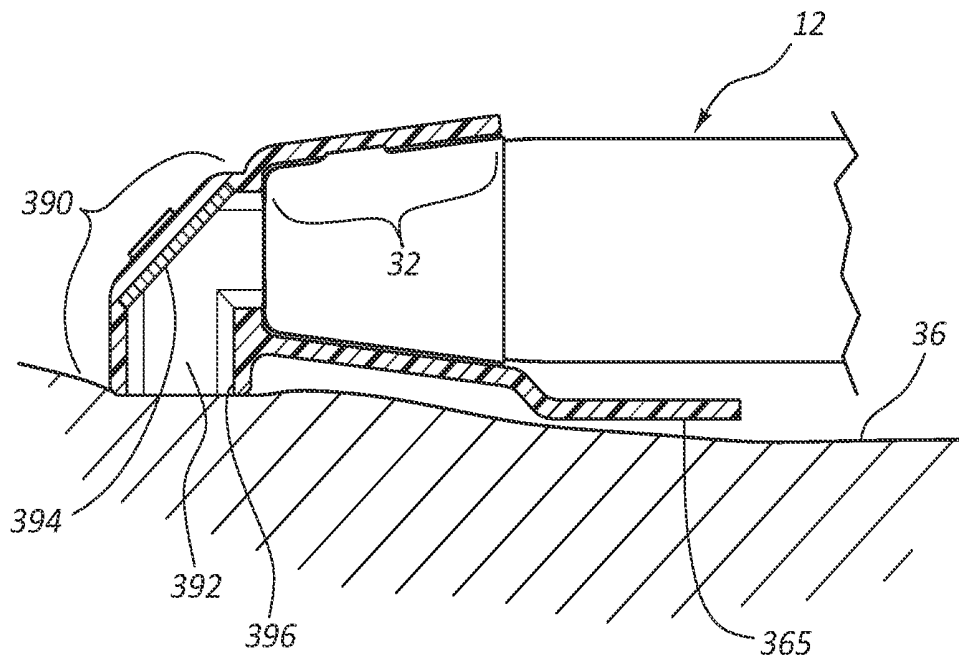


FIG. 31

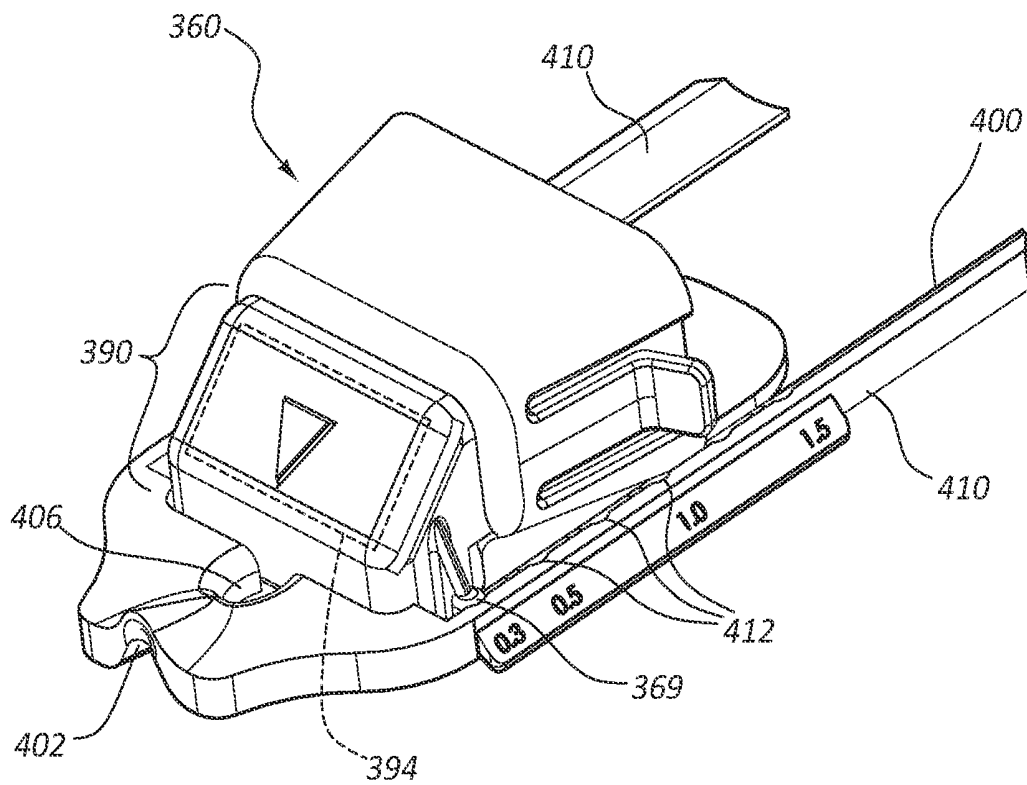


FIG. 32



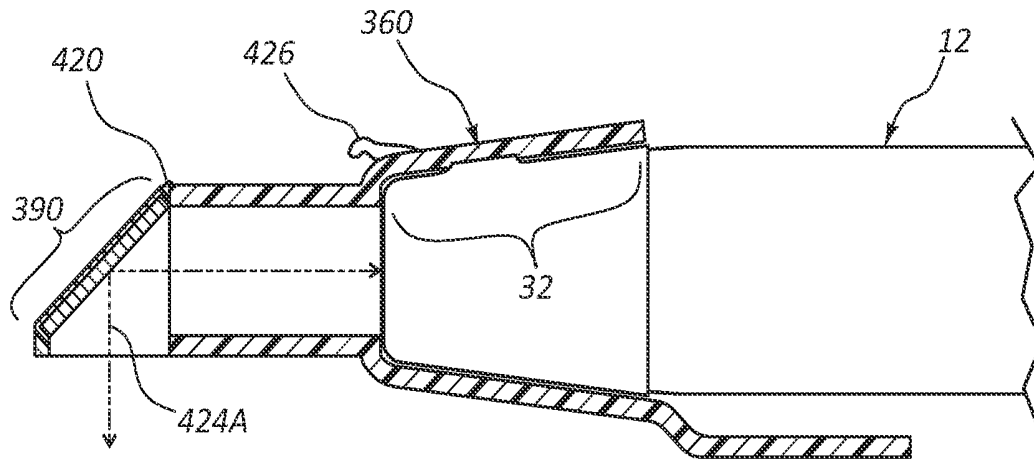


FIG. 33A



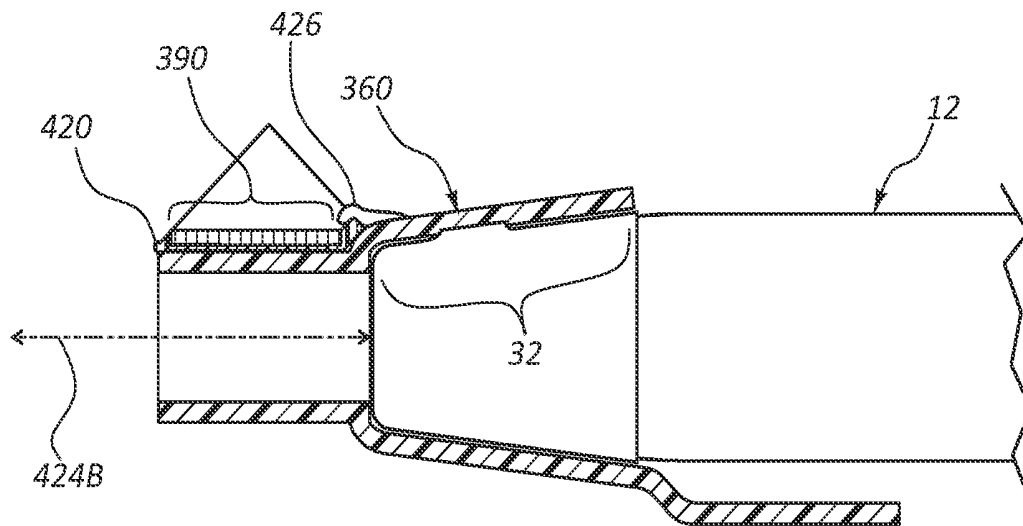



FIG. 33B

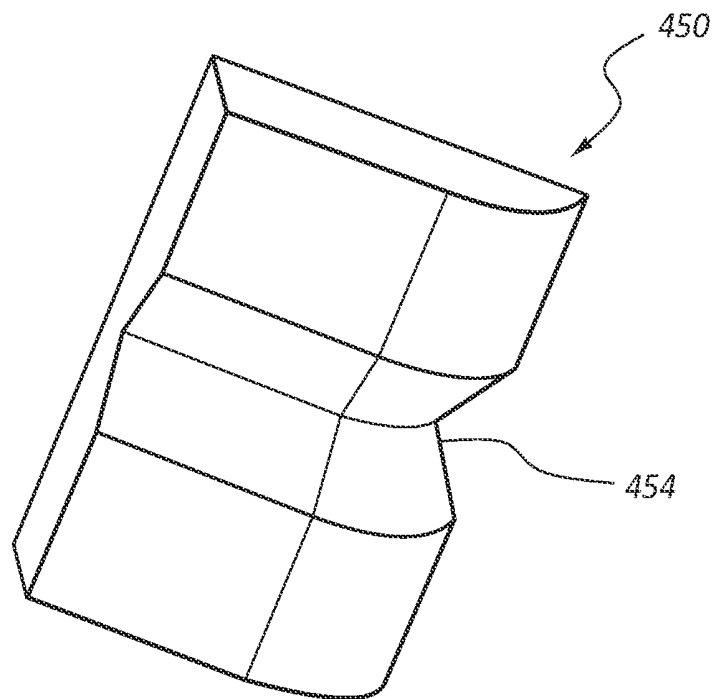

**FIG. 34**

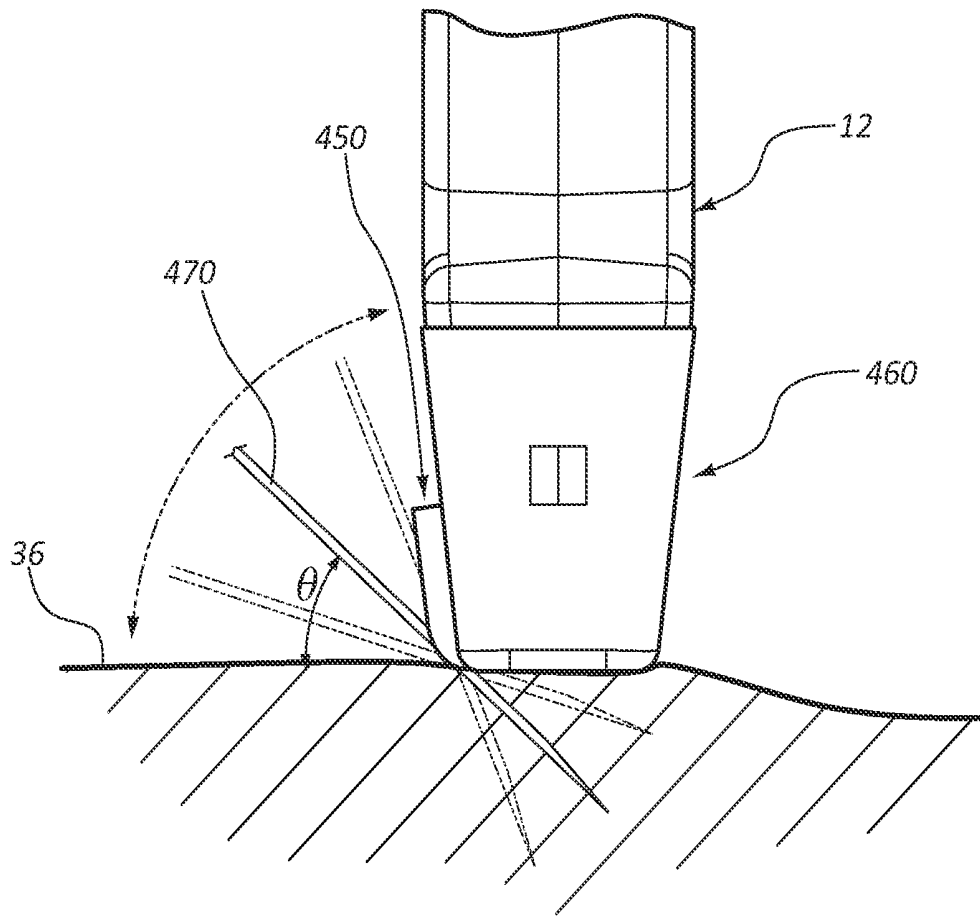

**FIG. 35A**

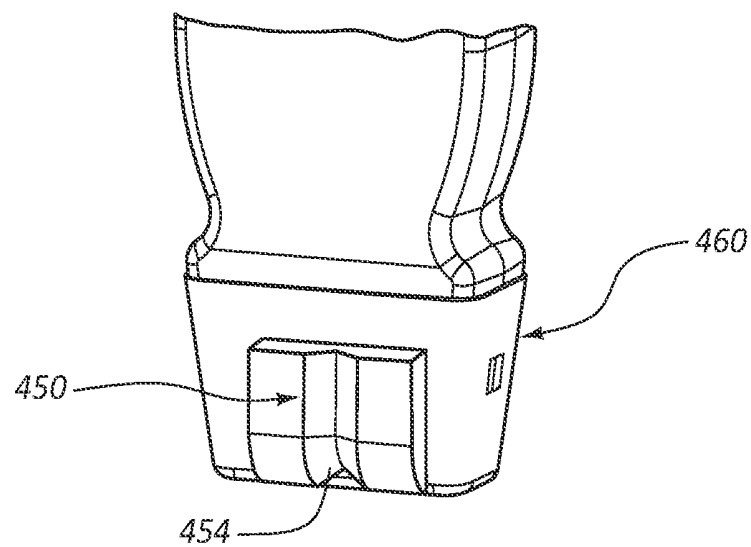

**FIG. 35B**

1

## SUPPORT AND COVER STRUCTURES FOR AN ULTRASOUND PROBE HEAD

### CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a continuation-in-part of U.S. application Ser. No. 12/900,750, filed Oct. 8, 2010, and entitled "Spacers for Use with an Ultrasound Probe," which claims the benefit of U.S. Provisional Patent Application No. 61/372,044, filed Aug. 9, 2010, and entitled "Support and Cover Structures for an Ultrasound Probe Head," and of U.S. Provisional Patent Application No. 61/249,850, filed Oct. 8, 2009, and entitled "Ultrasound Probe Spacers." Each of these applications is incorporated herein by reference in its entirety.

### BRIEF SUMMARY

Briefly summarized, embodiments of the present invention are directed to a probe cap for use with an ultrasound probe including a head portion and an acoustic surface. In one embodiment, the probe cap includes a body that defines a cavity sized for releasably receiving the head portion of the probe therein. The probe cap body further defines a hole that is proximate the acoustic surface of the head portion. A compliant spacer component is disposed in the hole. The spacer component can include a hydrogel and provides an acoustic path between the acoustic surface and a tissue surface of a patient. The spacer component further includes a skin contact surface that defines a concavity and is deformable against the skin. The skin contact surface can further define one or more spacer elements adjacent the concavity for distributing the load of the probe pressing against the skin and preventing compression of subcutaneous structures of the patient.

In another embodiment, an ultrasound imaging system for imaging a subcutaneous structure of a patient is disclosed and includes a display, an ultrasound probe including an acoustic surface from which ultrasound signals are emitted, and first and second spacer elements. The spacer elements are positioned proximate opposite ends of the acoustic surface and are configured to provide a gap between the acoustic surface and a tissue surface of the patient. So configured, the spacer elements prevent compression of the subcutaneous structure of the patient.

In addition, embodiments to be further described below disclose various probe cap and accompanying needle guide designs for use in assisting a clinician with ultrasound probe use and needle insertion into a patient.

These and other features of embodiments of the present invention will become more fully apparent from the following description and appended claims, or may be learned by the practice of embodiments of the invention as set forth hereinafter.

### BRIEF DESCRIPTION OF THE DRAWINGS

A more particular description of the present disclosure will be rendered by reference to specific embodiments thereof that are illustrated in the appended drawings. It is appreciated that these drawings depict only typical embodiments of the invention and are therefore not to be considered limiting of its scope. Example embodiments of the invention will be described and explained with additional specificity and detail through the use of the accompanying drawings in which:

2

FIGS. 1A and 1B are perspective and side views, respectively, of an ultrasound probe including spacer elements configured in accordance with one embodiment;

FIG. 2 is a simplified cross sectional view of the ultrasound probe of FIGS. 1A and 1B used to image a vessel of a patient;

FIG. 3 is a side view of the ultrasound probe of FIGS. 1A and 1B enclosed within a sheath in accordance with one embodiment;

FIGS. 4A and 4B are side views of a portion of an ultrasound probe including spacer elements and further showing examples of possible acoustic surface configurations in accordance with one embodiment;

FIG. 5 is a side view of a portion of an ultrasound probe including a spacer element in accordance with one embodiment;

FIG. 6 shows ultrasound spacer elements configured in accordance with one embodiment;

FIG. 7 shows ultrasound spacer elements configured in accordance with one embodiment;

FIG. 8 shows ultrasound spacer elements configured in accordance with one embodiment;

FIGS. 9A and 9B show spacer elements configured in accordance with one embodiment;

FIG. 10 is a side view of an ultrasound probe including spacer elements configured in accordance with one embodiment;

FIG. 11 is a side view of an ultrasound probe including a cap including spacer elements and a sheath in accordance with one embodiment;

FIG. 12 is a perspective view of a spacer component in accordance with one embodiment;

FIGS. 13A-13C show use of the spacer component of FIG. 12 in accordance with one embodiment;

FIG. 14 is a side view of a spacer component in accordance with one embodiment;

FIGS. 15A-15B show use of the spacer component of FIG. 14 in accordance with one embodiment;

FIG. 16 is an exploded perspective view of an ultrasound probe and a probe cap in accordance with one embodiment;

FIGS. 17A-17D are various views of the probe cap of FIG. 16;

FIGS. 18A and 18B are an exploded perspective view and cross sectional side view of an ultrasound probe/probe cap and a spacer component, respectively;

FIG. 19 is a cross sectional view of a head portion of the ultrasound probe of FIG. 16;

FIG. 20 is a cross sectional view of the probe cap of FIG. 16;

FIG. 21 is a cross sectional view of a head portion of the ultrasound probe of FIG. 16 received within the probe cap of FIG. 16;

FIG. 22 is another cross sectional view showing a head portion of the ultrasound probe of FIG. 16 received within the probe cap of FIG. 16;

FIG. 23 is a perspective view of a mated configuration of the ultrasound probe and probe cap of FIG. 16;

FIGS. 24A and 24B are front and side views, respectively, of an ultrasound probe and accompanying probe cap including a compliant spacer component according to one embodiment;

FIG. 24C is a perspective view of the probe cap of FIGS. 24A and 24B;

FIGS. 25A-25D are various views of a probe cap according to one embodiment;

FIGS. 26A and 26B are various exploded views of a probe cap configured according to one embodiment;

FIG. 27 is a side view of the probe cap of FIGS. 26A and 26B shown in contact with a patient's skin above a subcutaneous vessel;

FIGS. 28A and 28B are perspective and cross sectional views, respectively, of a probe cap according to one embodiment;

FIGS. 29A-29D are various views of a probe cap assembly according to one embodiment;

FIGS. 30A and 30B are various perspective views of a probe cap according to one embodiment;

FIG. 31 is a cross sectional side view of the probe cap of FIGS. 30A and 30B shown attached to an ultrasound probe;

FIG. 32 is a perspective view of a probe cap according to one embodiment;

FIGS. 33A and 33B are partial cross sectional side views of an ultrasound probe and probe cap in accordance with one embodiment;

FIG. 34 is a perspective view of a needle guide according to one embodiment; and

FIGS. 35A and 35B are side and perspective views, respectively, of the needle guide of FIG. 34 attached to a probe cap according to one embodiment.

#### DETAILED DESCRIPTION OF SELECTED EMBODIMENTS

Reference will now be made to figures wherein like structures will be provided with like reference designations. It is understood that the drawings are diagrammatic and schematic representations of exemplary embodiments of the present invention, and are neither limiting nor necessarily drawn to scale.

For clarity it is to be understood that the word "proximal" refers to a direction relatively closer to a clinician using the device to be described herein, while the word "distal" refers to a direction relatively further from the clinician. For example, the end of a catheter placed within the body of a patient is considered a distal end of the catheter, while the catheter end remaining outside the body is a proximal end of the catheter. Also, the words "including," "has," and "having," as used herein, including the claims, shall have the same meaning as the word "comprising."

Embodiments of the present invention are generally directed to various components for spacing an acoustic surface of an ultrasound probe from a tissue surface of a patient during ultrasound procedures to image subcutaneous tissues of the patient. Such ultrasound procedures are employed, for instance, in connection with the placement of a catheter within a vessel of the patient. As will be described, the components for spacing the acoustic surface in one embodiment prevent undesired compression of subcutaneous vessels, especially superficial vessels, which in turn improves the imaging of such vessels by the probe. In addition, embodiments to be described further below disclose various probe cap and accompanying needle guide designs for use in assisting a clinician with ultrasound probe use and needle insertion into a patient.

Reference is first made to FIGS. 1A and 1B, which depict an ultrasound imaging system 10 according to one embodiment, including an ultrasound probe 12 and a console 20 including a display 30 for depicting an image produced by the probe. In the present embodiment, the probe 12 is operably connected to the console 20 via a cable 31, though in one embodiment the probe can be wirelessly connected thereto.

The probe 12 includes a head 32 defined by a longitudinal length 32A and a width 32B. The body of the probe

generally defines a front face 33A, a rear face 33B, and side faces 33C. It should be appreciated that the preceding description of the probe is not meant to limit application of the principles described herein in any way. The probe head 32 includes an acoustic surface 34 extending along at least a portion of a longitudinal length 32A of the probe head from which ultrasonic impulses are emitted in order to penetrate and image subcutaneous portions of the patient. Note that the size, shape and configuration of both the probe and acoustic surface can vary from what is described herein while still residing within the principles of the present disclosure. Note also that FIG. 1A shows just one example of an ultrasound imaging system; other systems including other components can also benefit from the principles described herein.

As depicted in FIGS. 1A and 1B, in accordance with one embodiment the probe head 32 includes two spacer elements, generally depicted at 40, disposed adjacent the probe acoustic surface 34 at each end of the longitudinal length 32A. Each spacer element 40 acts as an extended surface to provide a gap 48 between the acoustic surface 34 and the skin 36 or other tissue surface of the patient, as further described below, when the probe 12 is placed on the patient's skin for use in subcutaneous imaging.

In greater detail, each spacer element 40 in the present embodiment defines a blade-like extended surface that includes a contact surface 42 for contacting the tissue/skin 36 of the patient. The contact surface 42 can be shaped in one of several configurations, as will be discussed further below.

Reference is now made to FIG. 2. When no spacers are present on an ultrasound probe, the acoustic surface thereof directly contacts the patient's skin during imaging, which can cause a downward pressure sufficient to undesirably compress a subcutaneous vessel disposed beneath the probe. Further, the proximity of the probe acoustic surface to the patient's skin can cause the focal point of the probe to reside below the vessel to be imaged, resulting in less than optimal image resolution of superficial vessels or other objects residing relatively close to the skin surface.

In contrast to the above, FIG. 2 shows the probe 12 including the spacer elements 40 disposed at each longitudinal end of the probe head 32 and adjacent the acoustic surface 34. So configured, the acoustic surface 34 is spaced apart from the patient's skin 36 during probe use, and only the contact surfaces 42 of the spacer elements 40 are in contact therewith. The gap 48 is thus defined between the acoustic surface 34 and the patient's skin 36, which can be filled with an ultrasonic gel 84 or other acoustically transparent substance to improve imaging, in one embodiment.

Because the acoustic surface 34 of the ultrasound probe head 32 is not in direct contact with the patient's skin 36 during probe use, pressure on the skin imposed by the acoustic surface is avoided, which in turn prevents a vessel 50 underneath the probe 12 from being compressed by the probe during use. Instead, any downward force provided by the probe 12 is directed through the spacer elements 40. As such, the vessel 50 below the acoustic surface 34 remains patent and can be accurately imaged. Further, the increased distance between the acoustic surface 34 and the patient's skin 36 provided by the gap 48 moves the focal spot of the probe 12 to a location relatively close below the skin surface, which enables superficial vessels and other objects residing near the skin surface to be brought more closely to the focal point of the probe and be sharply imaged.

Note that the gap 48 shown in FIGS. 1A-2 is bounded during probe use by the acoustic surface 34, the skin 36, and

the spacer elements 40. As such, the gap 48 remains open below the front and rear faces 33A, 33B of the probe 12. Note that additional spacers could be employed to further define the gap 48, if desired.

Reference is now made to FIG. 3 in describing one embodiment, wherein a sheath 52 is placed over the probe 12 to provide a sterile field about the probe. The sheath 52 can be disposed about the probe 12 such that a relatively close fit is defined between the sheath and the side faces 33C and front/rear faces 33A, 33B of the probe so that the ultrasound gel 84 can be included in and confined within the gap 48 by the sheath and the spacer elements 40. Note that sheaths or barriers of many different styles or configurations may be used.

FIGS. 4A and 4B show example surface configurations for the acoustic surface 34. In FIG. 4A, the acoustic surface 34 is flat as to be substantially parallel with the patient's skin 36 during probe use. In FIG. 4B, the acoustic surface 34 defines a concave shape with respect to the skin 36. This configuration can assist in trapping a volume of ultrasound gel within the gap 48. Of course, other acoustic surface configurations can be employed.

FIG. 5 gives one example of a possible configuration for the contact surface 42 of the spacer element 40, wherein the contact surface defines a convex shape for engagement with the patient's skin or other tissue surface. Note this is in contrast to the relatively flat contact surface 42 shown in FIGS. 4A and 4B, for instance. Other spacer contact surface shapes can be employed, including straight, rounded, angled, etc.

FIG. 6 shows that a height "H" of each spacer element 40 can be defined according to a particular need or application in order to define a particular separation between the acoustic surface 34 and the patient's skin 36 during use of the probe 12. Note that in one embodiment, the spacer elements are integrally formed with the probe housing. In another embodiment, the spacer elements are removably attached to the probe. The spacer elements can include materials similar to or different from those materials included in the probe housing.

Reference is now made to FIGS. 7 and 8, wherein FIG. 7 shows that in one embodiment the spacer elements 40 can be configured to extend longitudinally a distance "E" past the side surfaces 33C of the probe 12. In FIG. 8, each of the spacer elements 40 is inset a distance "I" from the probe side surfaces 33C.

FIGS. 9A and 9B depict yet another possible spacer element configuration according to one embodiment, wherein each spacer element 40 is included at an end of an extension arm 48 that extends from a corresponding one of the front and rear faces 33A, 33B of the probe 12. Such a configuration may be useful, for instance, in advancing the probe 12 along the patient skin 36 in a direction parallel to the longitudinal length of the acoustic surface 34. These and other spacer configurations are therefore contemplated as residing with the spirit of the present disclosure.

FIG. 10 shows a height-adjustable spacer element 40 so as to allow variation in the set-off distance of the acoustic surface 34 from the skin 36. In the illustrated embodiment, a bracket 60 that slidably receives the spacer element 40 is included on the side face 33C of the probe 12 and includes a depression or hole 62. Corresponding protuberances 64 are included on the spacer element 40 and are configured to be selectively received into the hole 62 so as to removably lock the spacer element in place at a specified height. The protuberances 64 are distributed along the length of the spacer element 40 such that one of multiple spacer heights

may be selected. A similarly adjustable spacer element is included on the opposite side face of the probe 12. Of course, other adjustable spacer element configurations can be included on the probe in addition to that explicitly described here.

FIG. 11 shows details of yet another embodiment, wherein the spacer elements 40 are included on a cap 70 that is removably attachable to the probe head 32. In the present embodiment, the cap is snapped on to the probe head 32 via an interference fit, but in other embodiments other attachment schemes can be employed, including inter-engaging surfaces on the probe and cap, for example. A sheath 72 is attached to the cap 70 so as to provide a sterile barrier for the ultrasound probe 10. In one embodiment the cap 70 and sheath 72 are disposable.

It should be appreciated that the number, size, height, shape, etc., of the spacer elements can vary from what is explicitly described herein. For instance, one, three, or more spacers can be included. Or the relative heights of the spacers can differ one from another so as to produce an angled probe-to-skin configuration. The probe can include one of many different shapes, designs, etc. These and other modifications are thus considered part of the present disclosure.

FIG. 12 depicts details of a spacer component 78 configured for attachment to the probe head 32, as shown in FIG. 13A, according to one embodiment. The spacer component 78 includes a body of compliant material, such as a hydrogel, in one embodiment, which generally maintains its intended shape when deforming forces are absent. The compliant material in one embodiment can include AQUA-FLEX® ultrasound gel from Parker Laboratories, Inc., Fairfield, N.J. The spacer component 78 further defines spacer elements 80 on each longitudinal end thereof, with a concavity 82 defined between the spacer elements. It is appreciated that other suitable materials can be employed for the compliant material of the spacer component, including acoustically transparent, sufficiently solid materials such as soft silicone, rubber, etc. In one embodiment, the compliant material is thermoformable, sterilizable, and shelf stable for at least one year.

As shown in FIGS. 13A-13C, the spacer component 78 due to its compliant nature can deform so as to conform to the shape of the surface of the patient's skin 36 during use of the probe 12. For example, the probe 12 including the spacer component 78 can be placed on a patient's arm. So positioned, the spacers 80 of the spacer component 78 can deform as needed as to match the cross sectional curvature of the arm surface and maintain contact with the skin 36 thereof. FIGS. 13B and 13C show such deformation of the spacer component 78 for relatively larger arms. Thus, the spacer component 78 provides an acoustic path between the acoustic surface and the skin surface without need of a flowable ultrasound gel. It is appreciated that the spacer component can be used in connection with imaging other portions of the patient's body and that the spacer component can define other shapes for contacting differently shaped body portions. Further, in one embodiment, an ultrasound gel can be included between the spacer component and the skin, such as in the concavity thereof.

FIG. 14 depicts a spacer component 90 according to another embodiment, including a flexible casing 92 that can operably attach to the probe head 32, as shown. The casing 92 includes arms 92A that contain a compliant insert 94, such as hydrogel in one embodiment. As shown in FIGS. 15A and 15B, the spacer component 90 is positioned on the probe head 32 so as to provide both spacing and an acoustic

path between the acoustic surface **34** and the surface of the skin **36** or other tissue surface such that flowable ultrasound gel is not needed. So configured, the insert **94** thereof defines a contact surface **96** for contacting the surface of the skin **36** during ultrasound probe use. In one embodiment, the arms **92A** of the casing **92** can be pressed inward to modify the shape of the contact surface **96**. For instance, FIG. **15A** shows that the contact surface **96** of the insert **94** defines a relatively shallow concavity **98** when the arms **92A** of the casing **92** are allowed to flex outward. When the arms **92A** are pressed inward as in FIG. **15B**, however, the insert **94** is compressed by the arms and the concavity **98** of the contact surface **96** becomes relatively more pronounced. Such a configuration of the contact surface **96** may be desirable to stabilize a position of the subcutaneous vessel while preventing its collapse. The arms **92A** can be biased to restore themselves to a given position when not being pressed by a user.

FIG. **16** shows details of a probe cap **110** for use with the probe **12** according to one embodiment. The cap **110** is configured to receive therein the head **32** of the probe **12** and to provide a spacer component **118** for providing desired spacing between the acoustic surface **34** of the probe head **32** and the skin **36**.

As shown in FIGS. **17A-17D**, the cap **110** defines a cavity **112** that is sized to receive therein the head **32** of the probe **12**. An engagement feature **114** is included with the cap **110** to releasably and mechanically attach the cap to the probe **12**, though it is appreciated that various designs can be employed to accomplish the same functionality. The cap **110** further includes a needle guide base **116** on which a detachable needle guide can be placed so as to assist a clinician in placing a needle through the skin **36** after a vessel has been located through use of the ultrasound system **10** (FIG. **1A**).

With continuing reference to FIGS. **17A-17D**, reference is made to FIGS. **18A** and **18B**, which depict various details of the spacer component **118**, which is disposed in a hole **130** defined in the cap **110**, best seen in FIGS. **17A** and **17C**. As shown, the spacer component **118** includes a skin contact surface **126** that defines two spacer elements **120** and a concavity **122** disposed therebetween. The spacer component includes **118** a compliant material, such as hydrogel in one embodiment, though it is appreciated that other suitable materials can also be employed. The spacer component **118** thus requires no use of flowable ultrasound gel to be applied to the skin **36** in order to provide an acoustic path between the acoustic surface **134** and the patient's skin. The spacer component **118** further defines a lip **128** about a perimeter thereof to assist in its retention within the hole **130** of the cap **110**, as seen in FIG. **18B**. As shown, in the present embodiment the lip **128** is shaped so as to be sandwiched between the cap **110** and probe head **32**, thus preventing its unintended removal from the cap. A recess **138** is also shown on the cap **110** to receive therein an orientation nub **140** on the probe head **32**, which nub **140** provides a landmark for orienting an ultrasound image on the display **30** (FIG. **1A**) with the orientation of the probe **12** as held by the clinician.

FIG. **19** shows that in the present embodiment the acoustic surface **134** of the probe head **32** defines a convex shape. Correspondingly, FIG. **20** shows that a probe contact surface **136** of the compliant spacer component **118** also defines a convex surface. FIG. **21** shows that when the probe head **32** is received into the cavity **112** of the cap **110**, the convexly shaped probe contact surface **136** of the spacer component **118** deformably engages the convexly shaped acoustic surface **134** of the probe head **32** so as to ensure adequate contact therebetween and to provide a suitable acoustic path

through the spacer component. Of course, other complementary shapes can be employed on the acoustic surface and probe contact surface of the spacer component.

FIG. **22** shows another view of the engagement between the probe head **32** and the cap **110**, according to the present embodiment. FIG. **23** shows the cap **110**, including the spacer component **118**, removably attached to the probe **12**. Note that in one embodiment the cap provides a sterile barrier for the probe head, and is disposable.

FIGS. **24A-24C** depict the probe cap **110** and the concavely-shaped, compliant spacer component **118** according to one embodiment, together with the ultrasound probe **12**. As shown, a suitably shaped cover **148** is also included for covering the spacer component **118** to prevent contamination thereof and to prevent the spacer component from drying out before use. When use of the probe cap is desired the cover **148**, which is fit to the probe cap **110** via a friction or other suitable fit, can be simply removed and discarded by the clinician.

As best seen in FIG. **24C**, the cap **110** includes in the present embodiment a bracket **144** to which a needle guide can be removably attached so as to enable guidance of a needle toward a desired vessel imaged by the ultrasound probe **12**. Further details regarding one non-limiting example of a needle guide that can be attached to the bracket **144** can be found, for instance, in U.S. Provisional Application No. 61/426,297, filed Dec. 22, 2010, and entitled "Selectable Angle Needle Guide," which is incorporated herein by reference in its entirety. Note that the needle guide and bracket can vary from what is shown and described herein.

The discussion below discusses yet other structures for enhancing use of an ultrasonic probe in connection with placement of catheters and other medical devices in the body of a patient. Indeed, the embodiments disclosed herein facilitate ease of use when ultrasonically imaging portions of the patient body in preparation for device placement therein. Examples of such placement scenarios include the insertion by a clinician of a needle, PICC catheter, PIV catheter, mid-line catheter, etc. into the patient body via a transcutaneous insertion site.

FIGS. **25A-25D** show details of a probe cap **160** according to one embodiment, which defines a cavity **162** for receiving therein the head **32** of the probe **12** and an engagement feature **164** for enabling removable engagement of the cap to the probe head. A fixture **166** is included on the side of the cap **160** and is configured for removably receiving thereon a needle guide **192**. In another embodiment, this and other needle guides disclosed herein can be permanently attached to the cap. Note that, though not shown here, a spacer component similar to those shown and described in connection with FIGS. **24A-24C** is disposed in the aperture **130** of the cap **160** to provide an acoustic pathway from the probe head **32** to the patient's skin.

As best seen in FIG. **25D**, the needle guide **192** defines a channel **194** into which a portion of a cannula of a needle to be inserted into the patient can be temporarily received. Note that the size of the channel can accommodate needle cannulas of various sizes/diameters, as here, or can be configured to accept needles of a predetermined size. An abutment surface **196** is included at a distal end of the channel **194** about which the needle can pivot so as to continuously define differing angles of attack with respect to the patient's skin during needle insertion procedures. As such, the needle guide **192** is capable of guiding the needle at any one of a variety of angles of attack toward the patient's skin while

maintaining alignment of the needle with the subcutaneous vessel being imaged by the probe 12.

Note that the probe cap 160 and other caps discussed herein can be configured to mate with the head portion of the ultrasound probe in a variety of ways, including friction fit, clip-pocket engagement, adhesively, hook-and-loop, etc. The cap portion of the probe cap can also vary in design from what is shown and described herein.

The cap 160 further includes a stabilization arm 200 extending from a distal portion of the cap body. The stabilization arm 200 is configured to rest against the skin of the patient when the cap-equipped probe is held vertically and placed against the patient's skin during ultrasound imaging procedures, thus stabilizing the probe in the vertical position. Moreover, the stabilization arm 200 can assist in securing the cap-equipped probe to the patient's skin via the use of a cord or elastic band, for instance, that is extended about the patient's arm and over the stabilization arm, thus maintaining the ultrasound probe in the upright position without manual contact by the clinician during use and providing more freedom to the clinician during the imaging procedure. A hole 202 is also defined in the stabilization arm 200 in one embodiment to enable the clinician to press the patient's skin therethrough in order to locate/occlude a subcutaneous vessel. The area proximate the perimeter of the hole 202 is contoured in the present embodiment to assist with finger placement by the clinician. FIGS. 26A and 26B show various details of a probe cap 210 according to another embodiment, including a cavity 212 defined by the cap body that is configured to supportably receive the head 32 of the ultrasound probe 12 therein via snap-fit or other suitable modality. A fixture 216 for receiving thereon a needle guide is also included on the cap body.

A compliant membrane 218 defining a lip 218A about its perimeter is included for attachment to the cap body. Specifically, the cap body defines a ridge 219 about an aperture 230 at the distal end of the body. The lip 218A of the membrane 218 is configured to resiliently attach to the ridge 219 so as to join the membrane to the cap body and cover the ultrasound transducer of the probe head 32 when the cap 210 is attached to the probe 12. The membrane 218 thus provides an acoustic pathway between the transducer and the patient's skin. Note that ultrasound gel on the patient's skin may, but need not, be used with the cap 210 during ultrasound imaging. Note also that the membrane 218 in one embodiment includes silicone, though other suitable, compliant materials can also be employed.

In greater detail, the ridge 219 includes a concavely shaped concavity 222, as best seen in FIGS. 26A and 27, such that it defines two standoff's, or spacers 220, on either end. The compliant nature of the membrane 218 enables it to deform to the concavity 222 of the ridge 219 when the membrane is placed against the patient's skin during ultrasound procedures. Thus, the membrane 218 can conform to the skin 36 of the patient during ultrasound imaging so as to enable imaging of subcutaneous structures, such as a superficial vessel 50 seen in FIG. 27, without providing undesired compressive forces thereon.

FIGS. 28A and 28B depict a probe cap 260 according to one embodiment, wherein the body of the cap defines a cavity 262 and a fixture 266 for receiving thereon a needle guide. An ultrasonically transparent membrane 268 is included proximate an aperture 280 at a distal end of the cap body to cover the transducer of the head of an ultrasound probe inserted therein. An ultrasonically transmissive medium, such as ultrasound gel 269, can be placed on an interior surface of the membrane 268 to ensure acoustic

coupling between the transducer and the skin of the patient. As with other cap embodiments described herein the probe cap 260 can be configured as a sterile cap to provide sterility or isolation for the ultrasound probe. Spacers 270 can also be included on either side of the membrane 268 to prevent compression by the cap 260 of superficial vessels when the cap 260 is placed against the skin. Note that ultrasound gel can also be placed between the membrane 268 and the patient's skin to improve signal transfer, if desired.

FIGS. 29A-29D depict details of a probe cap assembly 310 according to another embodiment, wherein the assembly includes a cap body defining a cavity 312 for receiving therein the head 32 of the ultrasound probe 12, as before. Also as before, an engagement feature 314 is included to secure the cap body to the probe 12.

The cap body is movable between two parallel rails 350 of a bracket 340. Each rail 350 includes a plurality of slots 352 that align with corresponding slots on the opposing rail 350. Tabs 319 included on either longitudinal end of the cap body are configured to be selectively received into corresponding opposed slots 352 of the rails 350, as shown in FIGS. 29A-29D. In the illustrated embodiment, the cap body is selectively repositionable along the bracket rails 350 via manual movement by lifting the cap body so as to remove the tabs 319 from the corresponding slots 352, repositioning the cap body as desired with respect to the bracket rail slots, then inserting the tabs into the selected slots. In other embodiments, it is appreciated that other modalities for moving the cap body relative to the bracket are possible, including sliding movement, gear-driven movement, etc.

As best seen in FIGS. 29B-29D, a needle guide 342 is included in the bracket to guide a needle into the patient's body when the probe cap assembly 310 is placed on the patient's skin. An observation hole 346 is also included on the bracket 340 so as to enable a clinician inserting the needle to observe blood flashback upon the needle accessing the subcutaneous vessel.

Note that the needle guide 342 in the present embodiment is disposed at a fixed angle with respect to the bracket 340 and that the cap body is movable along the bracket with respect to the needle guide. This arrangement thus enables subcutaneous tissue to be imaged, by the ultrasound probe disposed in the cap body, at differing discrete distances from the needle guide 342. Further, this arrangement enables a needle inserted through the needle guide 342 to access an ultrasonically imaged vessel or other target at any one of a plurality of depths below the skin without the need for adjusting the angle of attack of the needle.

In greater detail, the probe 12 while disposed in the cap body of the probe cap assembly 310 can ultrasonically image a subcutaneous vessel within the patient and determine the depth below the skin surface at which the vessel resides. One or more of the slots 352 are marked with a number, indicating the depth below the skin at which a needle inserted into the patient through the needle guide 342 will intercept the subcutaneous vessel. Thus, the bracket 340 can be adjusted until the tabs 319 thereof are disposed in the slots 352 on either rail 350 corresponding to the depth of the imaged vessel. When the needle is inserted into the patient's skin through the needle guide 342, it can be advanced until it intercepts and accesses the imaged vessel at the determined depth, as desired. As such, it is appreciated that the probe cap assembly 310 can assist with needle access of an ultrasonically imaged vessel through a fixed-angle needle guide regardless of the depth of the vessel, thus obviating the need for an adjustable angle needle guide in the present embodiment. Note that the depth measurements of the



bracket can vary from what is shown, but in one embodiment, the depths accessible via the probe cap assembly 310 vary from about 0.3 cm to about 1.5 cm.

FIGS. 30A and 30B depict a probe cap 360 according to another embodiment, wherein the cap body defines a cavity 362 for receiving therein the head 32 of the ultrasound probe 12 and an engagement feature 364 to secure the cap body to the probe 12. A stabilization arm 365 extends from the cap body so as to enable the cap 360 (and the probe 12 received therein) to be secured to the patient via a band wrapped around the stabilization arm and the arm of the patient, for instance.

As shown, the probe cap 360 further includes a deflector portion 390 for deflecting an ultrasound signal both emanating from and travelling to the transducer of the ultrasound probe 12. The deflector portion 390 is formed as part of the probe cap 360 and defines a channel 392 and an aperture 396 through which ultrasound signals can pass. The deflector portion 390 further includes a deflecting surface 394 disposed in the channel 392. In the present embodiment the deflecting surface 394 is disposed at an angle of about 45 degrees with respect to the transducer surface of the probe head 32 so as to deflect ultrasound signals emanating therefrom through an angle of about 90 degrees, though the deflecting surface can be positioned in other embodiments at other angles so as to produce different resulting angles of signal deflection with respect to the probe transducer.

FIG. 31 shows the probe cap 360 positioned against the skin 356 of a patient such that signals emanating from the transducer of the probe head 32 travel through the channel 392, are deflected by the deflecting surface 394, and are directed downward into the body of the patient. Ultrasound signals reflected by an imaged target within the body and received into the channel 392 are also similarly deflected by the deflecting surface 394 toward the probe head 32 for receipt by the transducer. The deflecting surface 394 can include any suitable material having a suitable density so as to reflect the ultrasonic signals travelling through the channel 392. In one embodiment, the deflecting surface includes a plastic material. Also, in one embodiment, the channel 392 is at least partially filled with an ultrasonically transmissive medium, such as an ultrasound gel. In another embodiment, a hydrogel-based spacer component can be disposed in the channel 392, as in previous embodiments. In yet another embodiment, the deflector portion can be integrated into the probe head itself, without the presence of a probe cap. Use of the deflecting probe cap 360 enables the probe 12 to be positioned parallel to the skin 36 of the patient, thus eliminating the need for the clinician to hold the probe upright during use.

FIG. 32 shows that the deflecting probe cap 360 in one embodiment can be included as part of an assembly similar to that shown in FIGS. 29A-29D, wherein the cap body is selectively movable between two rails 410 of a bracket 400. The rails 410 each include corresponding slots 412 for receipt of tabs 369 included on the cap body so as to position the probe cap at one of a plurality of possible distances from a needle guide 402 included on the bracket 400. As before, an observation hole 406 is included proximate the needle guide 402. As described further above in connection with FIGS. 29A-29D, the assembly shown in FIG. 32 enables vessels at a variety of subcutaneous depths to be ultrasonically imaged and accessed by a needle disposed in the fixed-angle needle guide 402 by moving the bracket 400 with respect to the probe cap 360 such that the needle intercepts the imaged vessel at the intended depth.

FIGS. 33A and 33B depict the deflecting probe cap 360 according to one embodiment, wherein the deflector portion 390 is hingedly connected to the remainder portion of the cap body via a hinge component 420, including a mechanical or living hinge for instance. So configured, the deflector portion can be selectively positioned so as to deflect ultrasound signals along a deflected signal path 424A (FIG. 33A), or rotated out of the ultrasound signal path (FIG. 33B) so as to enable the ultrasound signals to travel along an undeflected signal path 424B. A latch 426 or other suitable modality can be included to selectively secure the deflector portion 390 in place. Note that in one embodiment a deflecting probe cap can be adjustable such that deflection of the ultrasound signal can be achieved through a variety of angles.

FIG. 34 shows a needle guide 450 according to one embodiment that can be employed with one or more of the probe caps described herein, such as the probe cap 460 shown in FIG. 35B, or can be attached directly to the ultrasound probe. As shown, the needle guide 450 includes a curved, V-shaped open channel 454 that centers a needle therein yet enables the clinician to continuously adjust the angle of attack  $\theta$  for the needle at the insertion site during needle insertion, as shown in FIG. 35A. Note that the shape of the channel can vary from what is shown and described.

Embodiments of the invention may be embodied in other specific forms without departing from the spirit of the present disclosure. The described embodiments are to be considered in all respects only as illustrative, not restrictive. The scope of the embodiments is, therefore, indicated by the appended claims rather than by the foregoing description. All changes that come within the meaning and range of equivalency of the claims are to be embraced within their scope.

What is claimed is:

1. A cap for use with an ultrasound probe, comprising: a cap body defining a cavity into which a head portion of the ultrasound probe is removably received; a stabilization arm extending from a first side of the cap body for stabilizing the cap against a skin surface of a patient; and a needle guide associated with a second side of the cap body different from the first side thereof, wherein the needle guide is separate from the stabilization arm.

2. The cap as defined in claim 1, wherein the stabilization arm further defines a hole to enable a clinician to contact the skin surface of the patient proximate a needle insertion area, a perimeter area proximate the hole being contoured.

3. The cap as defined in claim 1, further including an engagement feature for securing the cap to the ultrasound probe, wherein the engagement feature is configured to couple with a corresponding engagement feature of the head portion of the ultrasound probe.

4. The cap as defined in claim 1, wherein the needle guide is removably attachable to a fixture included on the cap body.

5. The cap as defined in claim 1, wherein the needle guide includes a channel in which a portion of a needle can be movably received, the channel including an abutment surface upon which the needle can pivot within the channel so as to selectively alter an angle of attack of the needle with respect to the skin surface of the patient.

6. The cap as defined in claim 1, wherein the stabilization arm extends from the cap body enabling the cap to be secured to the patient with a band or strap wrapped around the stabilization arm and the patient so as to support the ultrasound probe against the skin surface of the patient.

## 13

7. The cap as defined in claim 1, wherein the stabilization arm has a tallest height that is less than half a height of the cap body.

8. A cap assembly for use with an ultrasound probe, comprising:

a cap body defining a cavity into which a head portion of the ultrasound probe is removably received, wherein the cap body includes a tab; and

a bracket including a stationary needle guide, the cap body received in the bracket at a plurality of designated locations along a length thereof, the cap body movable with respect to the bracket in accordance with the plurality of designated locations so as to enable a distance between the needle guide and the cap body to be selectively varied, wherein each of the plurality of designated locations are configured to couple with the tab to secure a positioning of the cap body.

9. The cap assembly as defined in claim 8, wherein the needle guide defines a fixed angle of attack for a needle disposed therein, and wherein selective variation of the

## 14

distance between the needle guide and the cap body enables interception of a subcutaneous path of the needle with a desired subcutaneous target imaged by the ultrasound probe.

10. The cap assembly as defined in claim 9, wherein the bracket includes demarcations indicating a depth of interception of the needle with the imaged subcutaneous target.

11. The cap assembly as defined in claim 8, wherein the bracket includes first and second rails between which the cap body is movably disposed, the first and second rails including a plurality of aligned slots into which the tab disposed on the cap body can be removably received to position the cap body at a predetermined distance from the needle guide.

12. The cap assembly as defined in claim 8, wherein the cap assembly is configured to direct ultrasound signals into a patient produced by the ultrasound probe when the cap assembly is placed against skin of the patient.

13. The cap assembly as defined in claim 8, wherein the bracket further includes an observation hole proximate the needle guide for observing blood flashback from a needle.

\* \* \* \* \*

专利名称(译)	超声波探头的支撑和盖结构		
公开(公告)号	<a href="#">US10639008</a>	公开(公告)日	2020-05-05
申请号	US13/206396	申请日	2011-08-09
申请(专利权)人(译)	C. R. BARD , INC.		
当前申请(专利权)人(译)	C. R. BARD , INC.		
[标]发明人	LINDEKUGEL ERIC W COX JEREMY B BLANCHARD DANIEL B CROOK CHRISTIAN W BURNSIDE EDDIE K SOUTHARD JEANETTE E STINGER KEVIN W OROME AMIR		
发明人	LINDEKUGEL, ERIC W. COX, JEREMY B. BLANCHARD, DANIEL B. CROOK, CHRISTIAN W. BURNSIDE, EDDIE K. SOUTHARD, JEANETTE E. STINGER, KEVIN W. OROME, AMIR		
IPC分类号	A61B8/00 A61B17/34 A61B10/00 A61B18/00 A61B18/02 G10K11/02 A61K49/22		
CPC分类号	A61B8/4455 A61B8/4272 A61B8/4444 A61B8/4281 A61B8/42 A61B17/3403 A61B8/46 A61B8/4209 A61B10/00 A61B8/44 A61B2018/0231 A61B2562/16 A61B2018/00964 A61B8/4227 A61B2562/0204 A61B8/4472 A61K49/226 A61B8/4218 A61B8/4483 G10K11/02 A61B8/4236 A61B2562/00		
优先权	61/372044 2010-08-09 US 61/249850 2009-10-08 US		
其他公开文献	US20110313293A1		
外部链接	<a href="#">Espacenet</a>		

# 摘要(译)

公开了一种用于包括头部和声学表面的超声探头的探头盖。 在一个实施例中，探针帽包括主体，该主体限定了空腔，该空腔的尺寸设计成可释放地将探针的头部容纳在其中。 探针帽主体还限定出靠近头部的声表面的孔。 顺应性的隔离部件被布置在孔中。 间隔物组件可包括水凝胶，并在患者的声学表面和组织表面之间提供声学路径。 间隔物部件包括限定凹面并且可抵靠组织表面变形的皮肤接触表面。 附加的实施例公开了各种探针帽和随附的针头引导器设计，用于协助临床医生使用超声探针并将针头插入患者体内。

