


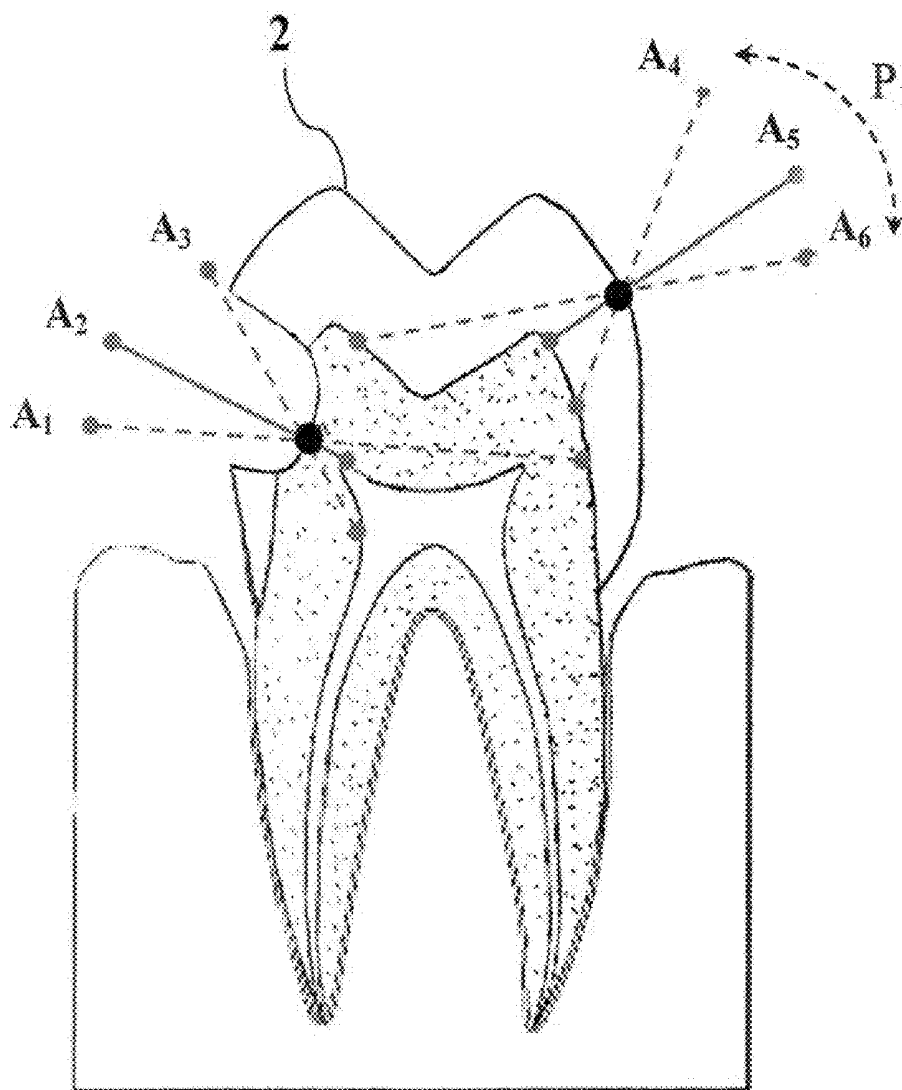

US 20100227295A1

(19) **United States**(12) **Patent Application Publication**
Maev et al.(10) **Pub. No.: US 2010/0227295 A1**(43) **Pub. Date: Sep. 9, 2010**(54) **ULTRASONIC DEVICE FOR ASSESSMENT
OF INTERNAL TOOTH STRUCTURE****Publication Classification**(76) Inventors: **Roman Gr. Maev**, Windsor (CA);
Eugene V. Malyarenko, Troy, MI
(US); **Alexander Ilyutovich**, Fort
Lee, NJ (US)(51) **Int. Cl.**
A61B 8/00 (2006.01)
A61C 19/04 (2006.01)(52) **U.S. Cl.** **433/215**Correspondence Address:
CARLSON, GASKEY & OLDS, P.C.
400 WEST MAPLE ROAD, SUITE 350
BIRMINGHAM, MI 48009 (US)(57) **ABSTRACT**

Example embodiments of this invention include a method and a device for assessing the internal structure of the tooth. In one example, the method is comprised of emitting a sequence of ultrasonic pulses from a given point on the tooth surface into the tooth at various directions of incidence (angles of incidence) with respect to the local tooth surface, recording the corresponding sequence of ultrasonic echoes from different internal dental formations, and processing the collected ultrasonic pulse-echo and pulse-direction data to present internal structure of the tooth in quantitative or graphical form.

(21) Appl. No.: **12/708,741**(22) Filed: **Feb. 19, 2010****Related U.S. Application Data**(60) Provisional application No. 61/153,759, filed on Feb.
19, 2009.

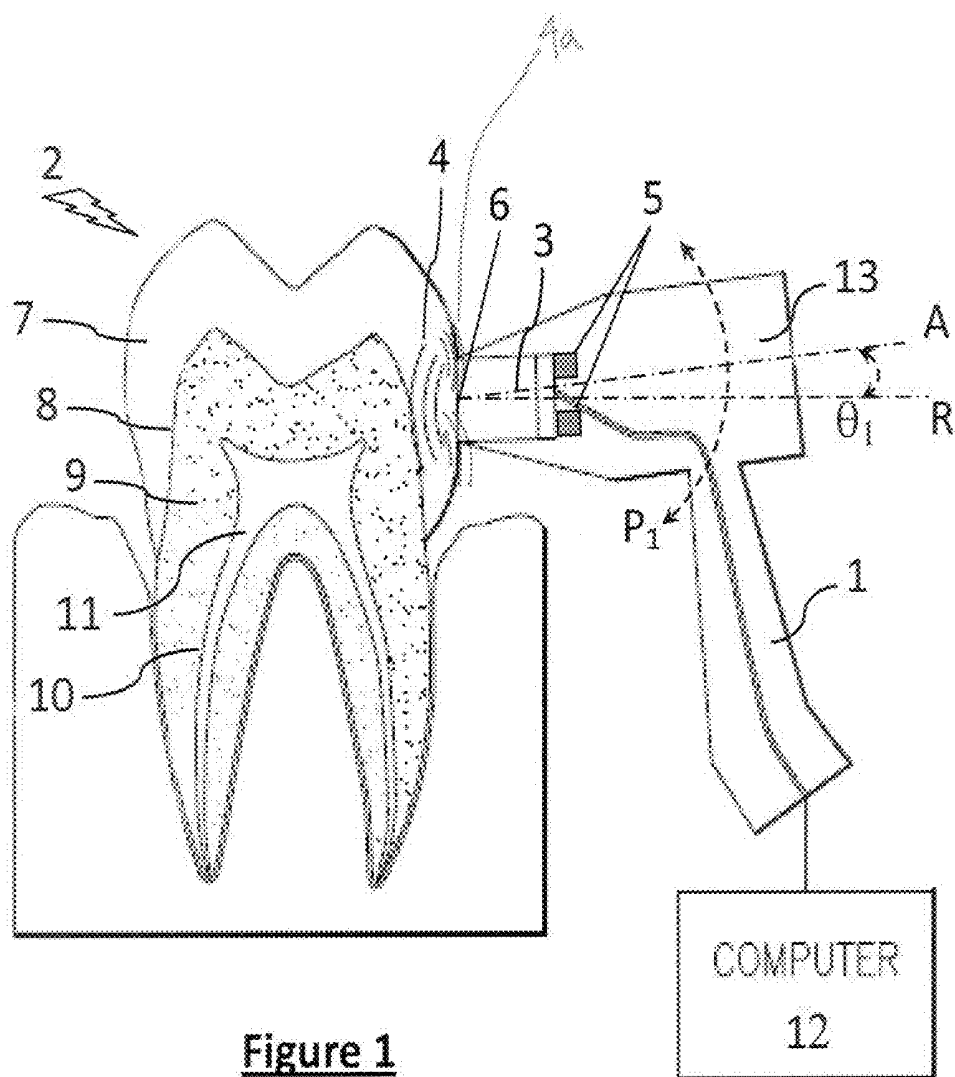


Figure 1

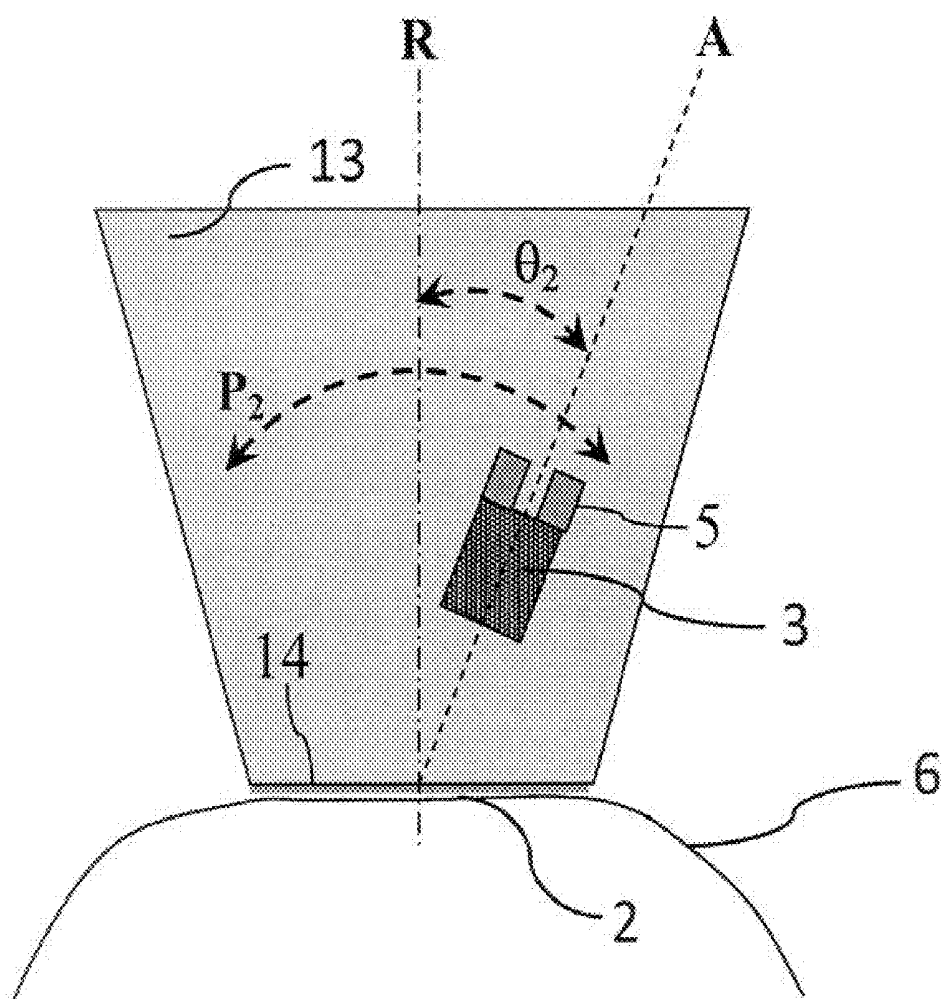


Figure 2

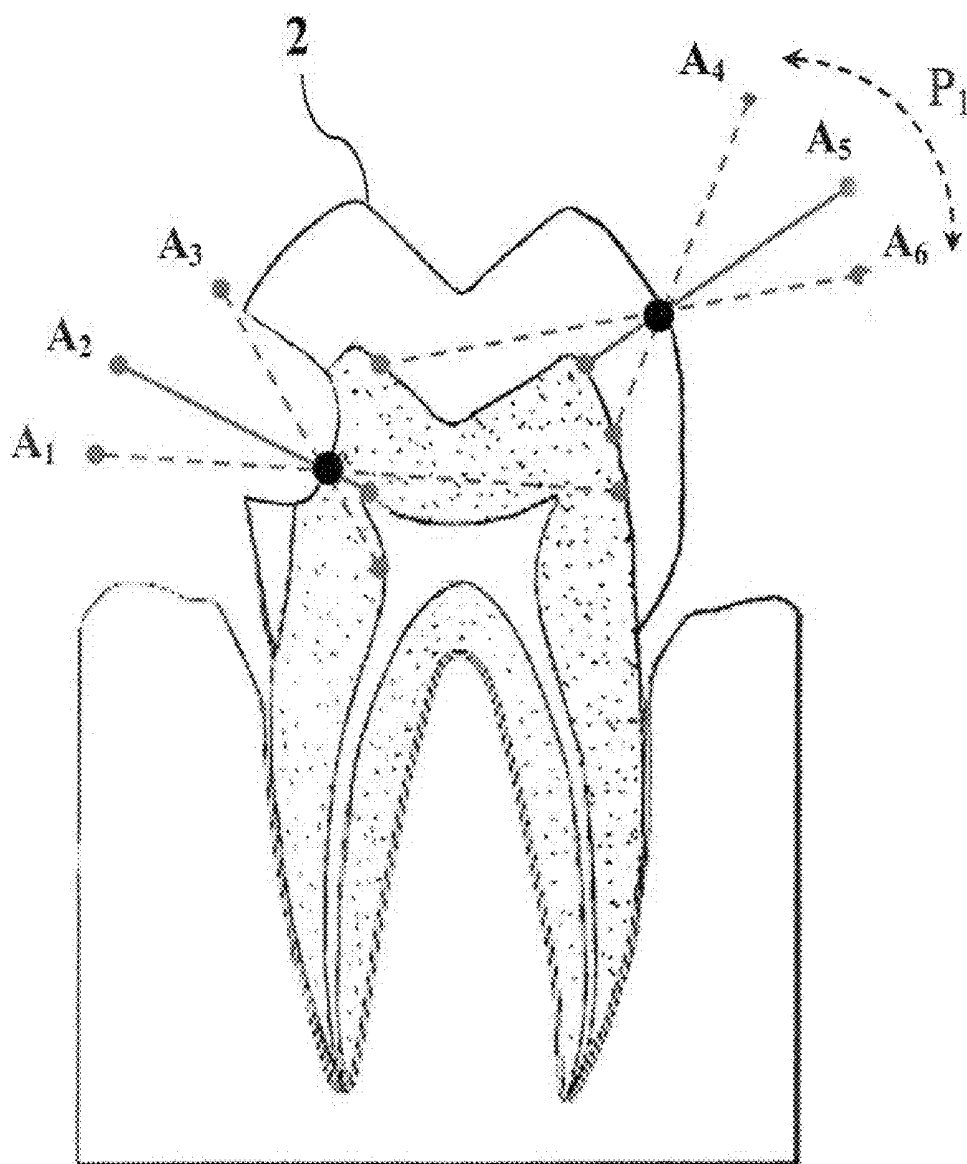


Figure 3

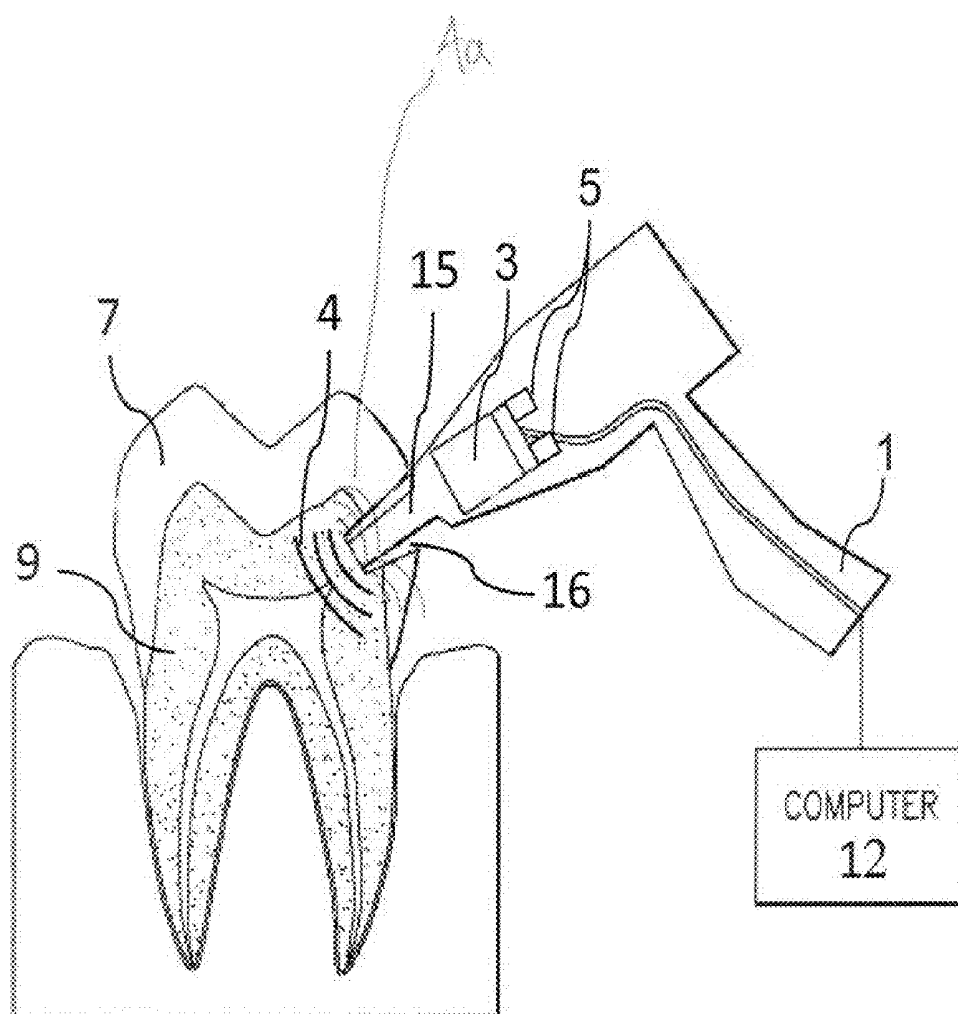


Figure 4

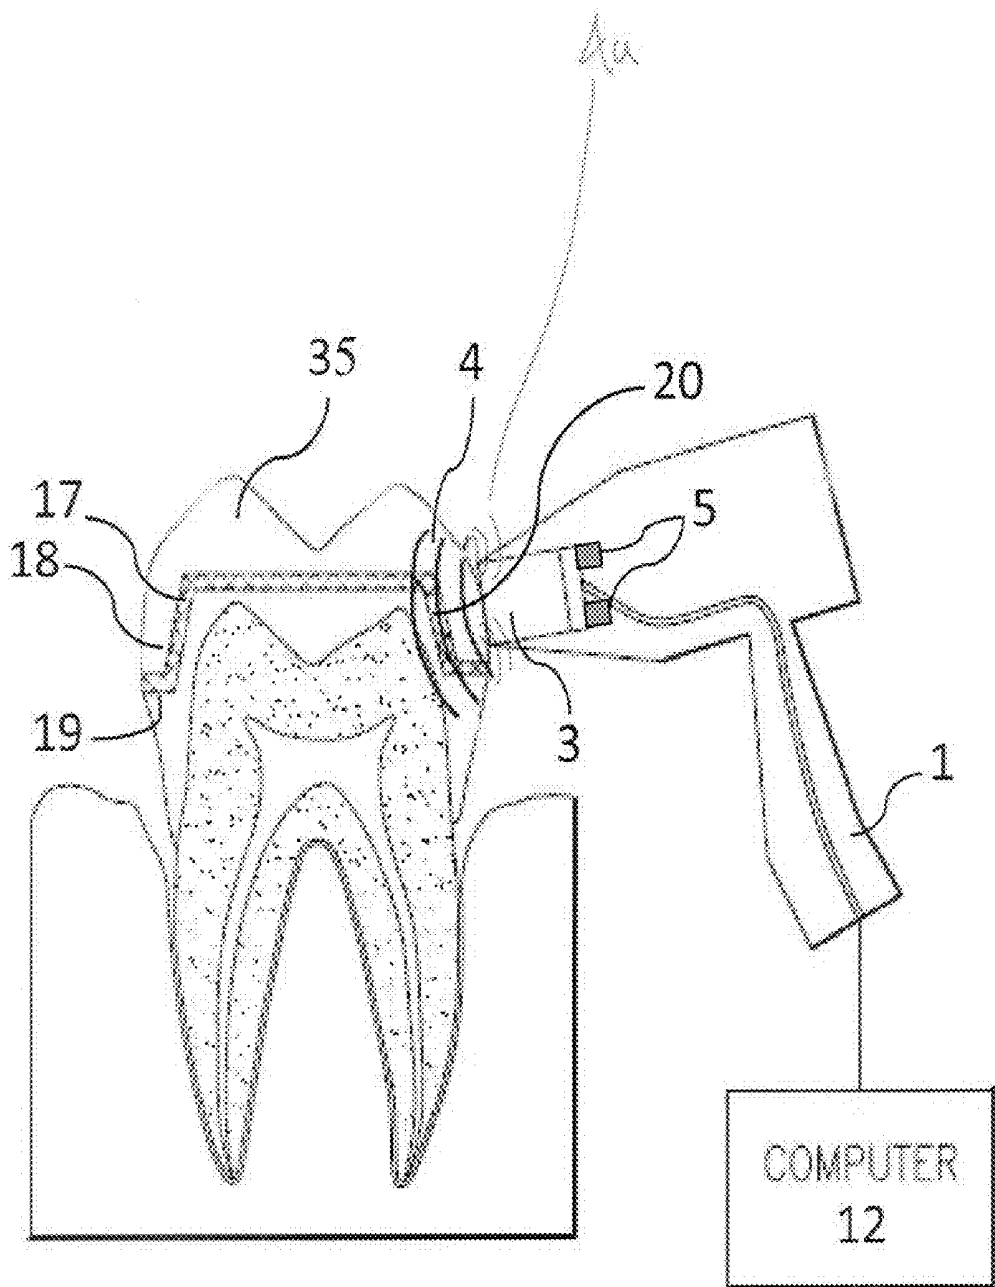


Figure 5

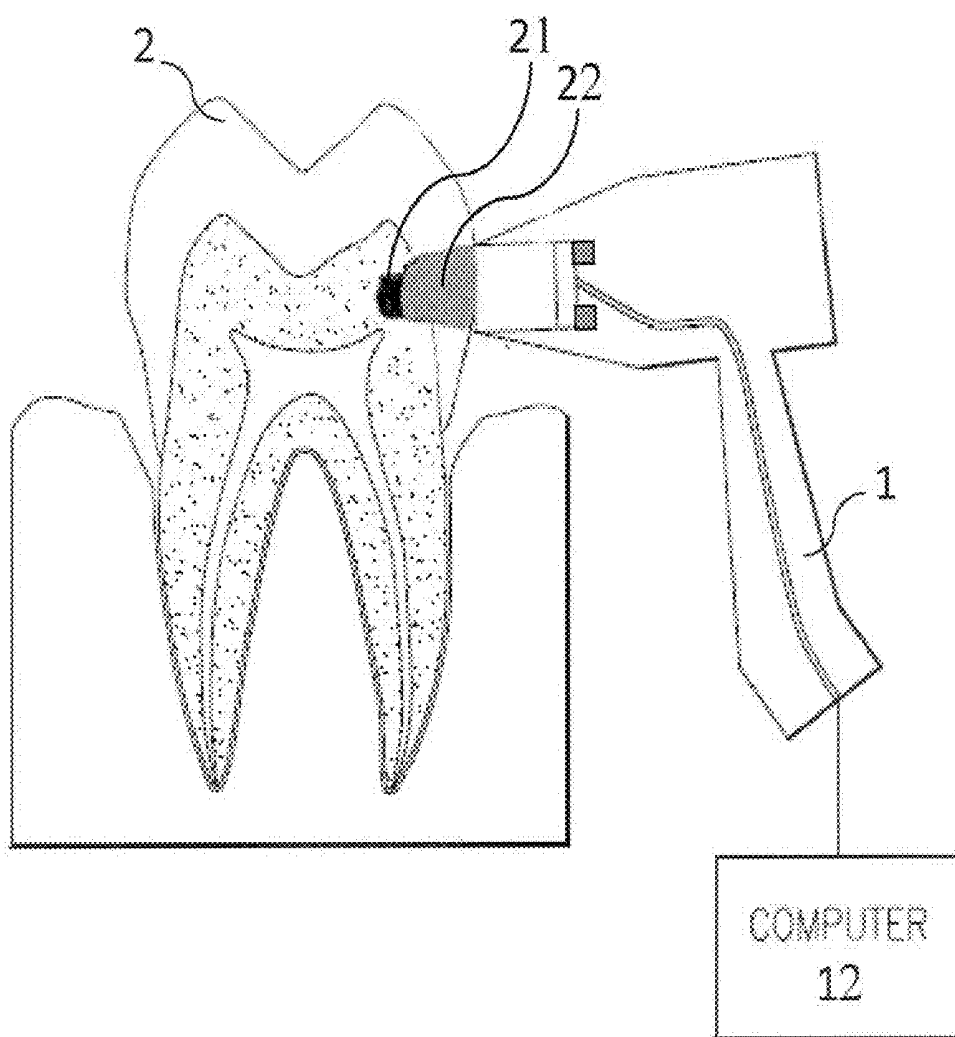
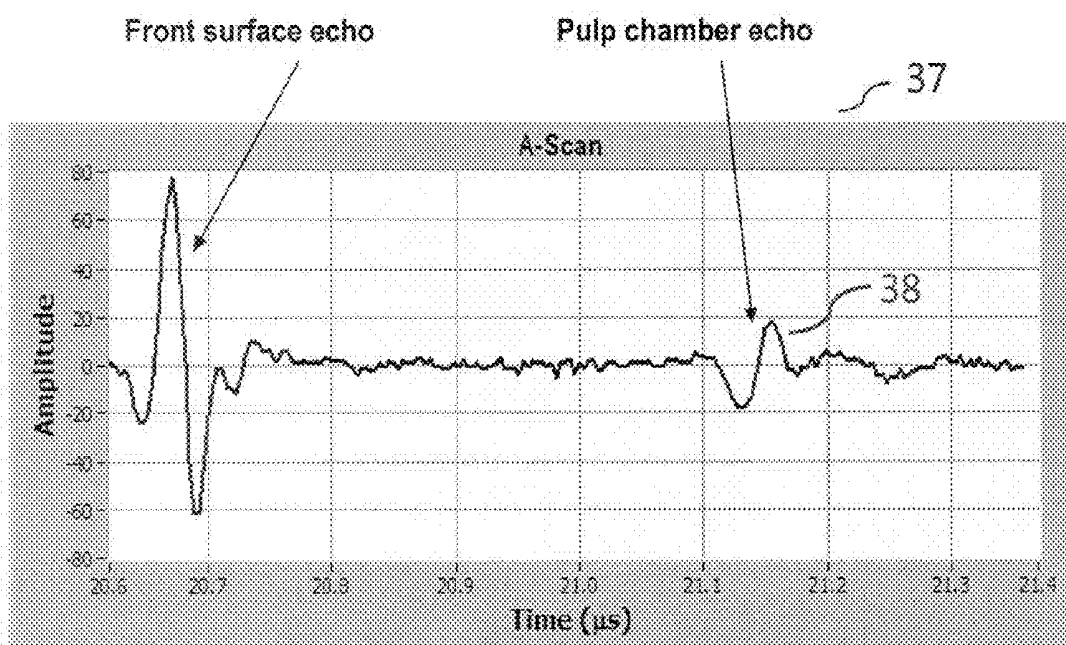


Figure 6

A-scanFigure 7

Sector-scan

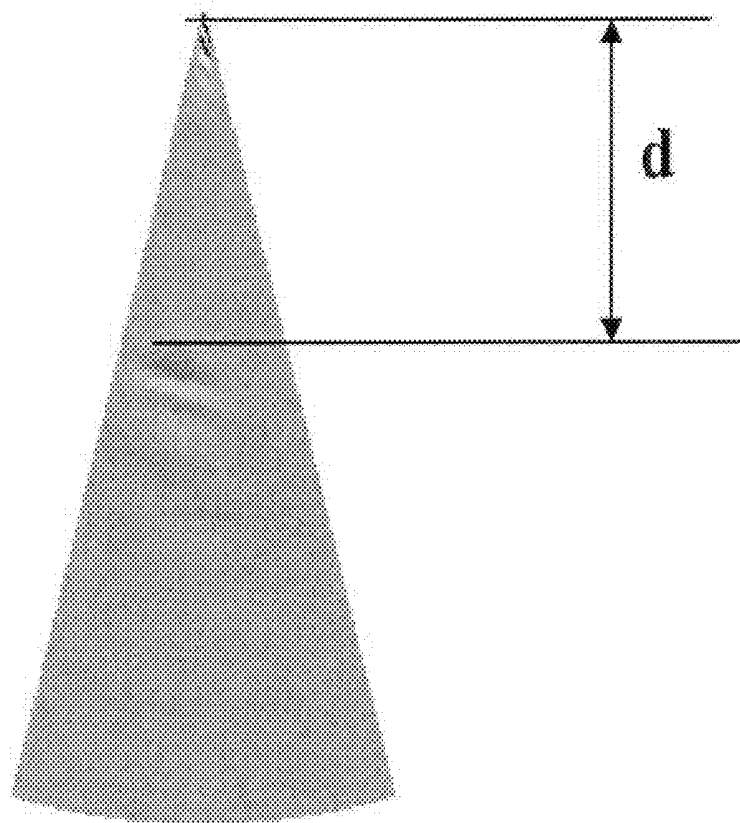


Figure 8

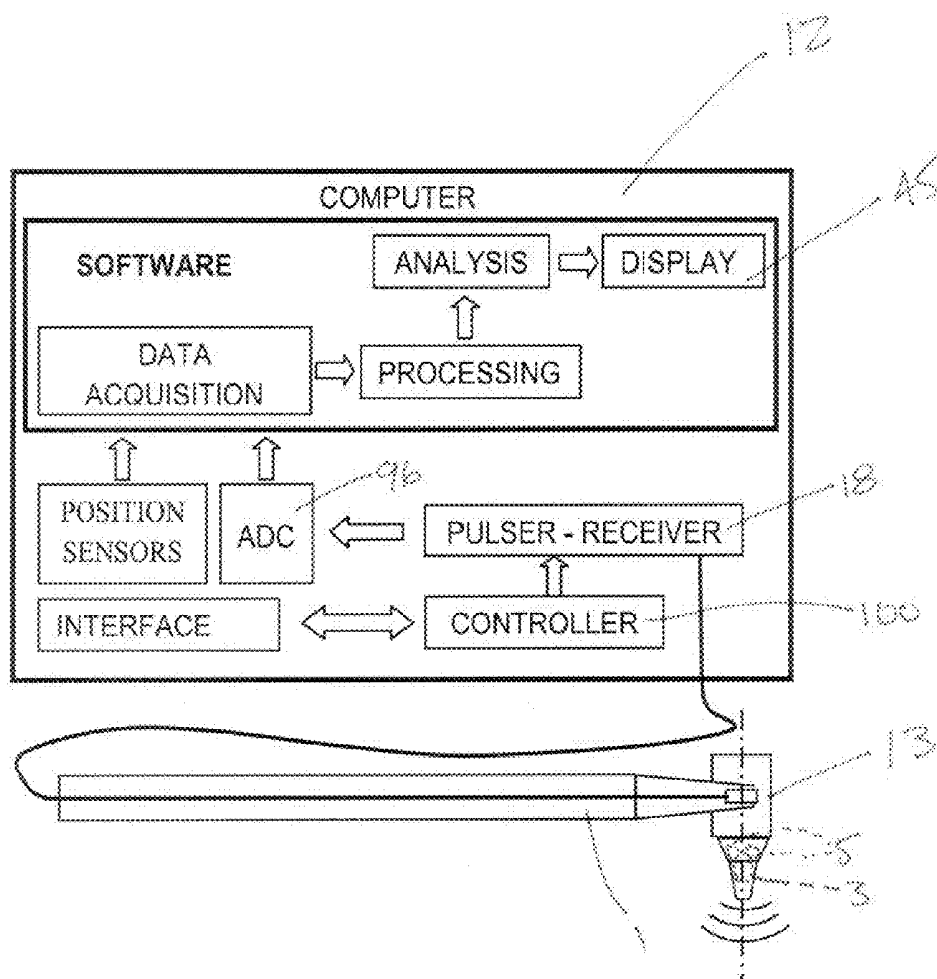


Figure 9

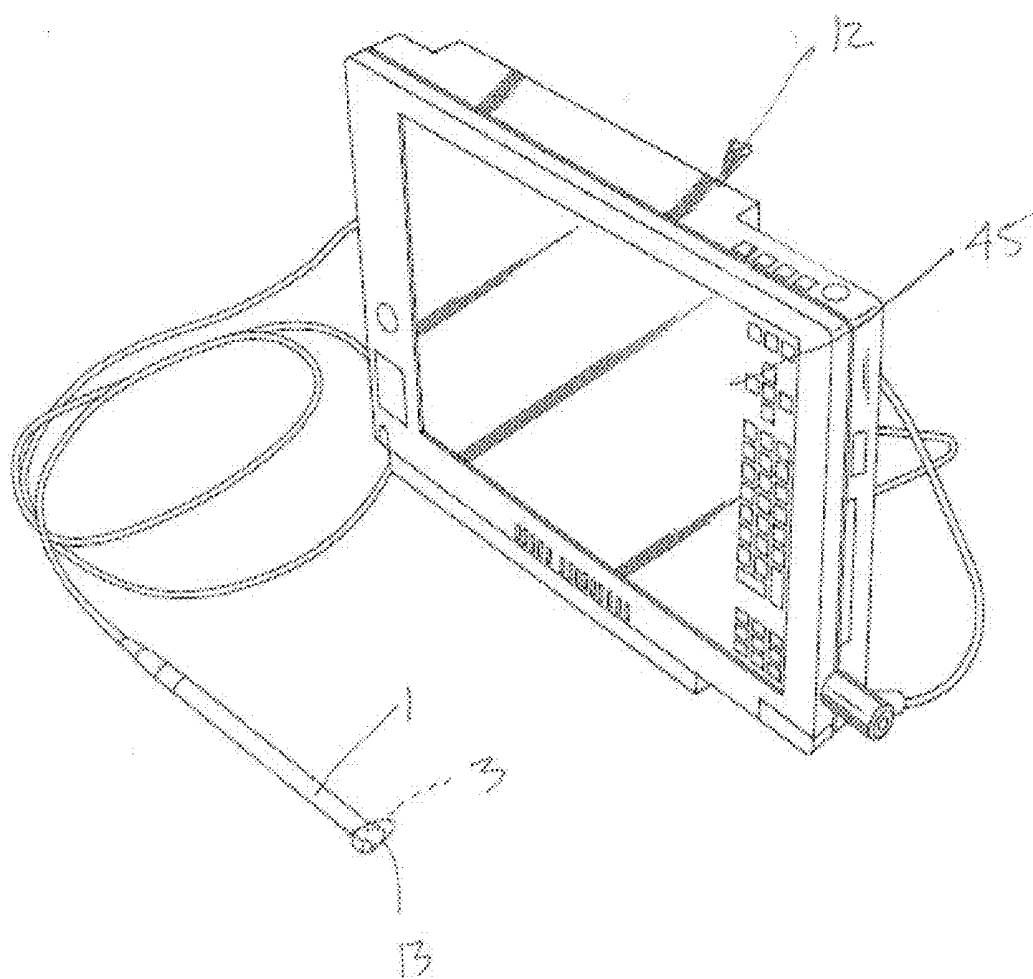


Figure 10

ULTRASONIC DEVICE FOR ASSESSMENT OF INTERNAL TOOTH STRUCTURE

REFERENCE TO RELATED APPLICATIONS

[0001] The present invention claims priority to U.S. Provisional Patent Application No. 61/153,759, filed Feb. 19, 2009.

BACKGROUND

[0002] This invention relates generally to an ultrasonic diagnostic tool, and more specifically to a portable (handheld) ultrasonic 3-D imaging device for dental applications.

[0003] A dentist diagnosing a dental condition often relies on subjective data such as patient complaints, intraoral visual examination results, and results of selective physical probing. Unfortunately, this information is non-quantitative and relies heavily on dentist skill and experience.

[0004] Information about internal dental formations (tooth microanatomy) is useful for many reasons. For example, information about internal dental formations, such as distances to the enamel/dentine and dentine/pulp interfaces from the tooth surface, helps the dentist plan treatment. Measurements taken during drilling and other tooth processing techniques without significant interruption of the treatment process facilitate controlling the distance from the drill tip to internal structures of the tooth, (e.g., pulp). Monitoring the bond between restoration material and tooth tissue can identify failed bonds, which can cause caries or cavities in the interface between restoration material and tooth tissue (e.g., dentine). Monitoring the bond between a dental crown and the tooth also facilitates detecting and locating flaws, which can decrease the strength of the restored tooth or lead to caries or cavities under the crown.

[0005] Imaging systems, such as conventional X-ray diagnostics, often fail to provide comprehensive results. More sophisticated imaging systems, such as Optical-Coherent Tomography, Cone-Beam Tomography or Terahertz Pulse Imaging, are costly and complex. Further, as is known, the enamel and dentine layers that cover the pulp are irregularly shaped. Measurements of these layers with existing imaging systems are often inaccurate, especially around corners and inside restoration areas, due to internal dental formation interfaces being at a non-zero angle relative to the tooth surface.

SUMMARY

[0006] Example embodiments of this invention include a method and a device for assessing the internal structure of the tooth. In one example, the method is comprised of emitting a sequence of ultrasonic pulses from a given point on the tooth surface into the tooth at various directions of incidence (angles of incidence) with respect to the local tooth surface, recording the corresponding sequence of ultrasonic echoes from different internal dental formations, and processing the collected ultrasonic pulse-echo and pulse-direction data to present internal structure of the tooth in quantitative or graphical form.

[0007] The example proposed device includes a signal generator for forming ultrasonic signals, one or several transducers for emission and reception of ultrasonic pulses, position sensors for determining the angular position of the transducer, means for positioning of the transducer on the tooth surface, a receiver for acquiring and amplifying ultrasonic signals, an analog-to-digital converter for transforming sig-

nals and position sensors data to digital representation, and a computer for providing control of the device, signal and data processing, and visualization.

[0008] The example computer gives a quantitative presentation of the pulse-echo data with corresponding angles of incidence in the form of an A-scan or a sector scan. The latter can be transformed into a graphical 3-D presentation of the internal tooth structure. Also, the computer can calculate such parameters as thicknesses of the internal tooth layers, including enamel, dentin, and cementum, or distances to the interfaces between said internal layers from any point of interest on the tooth surface. In addition to presentation of the internal geometries of the tooth, the device may also calculate other geometric parameters based on the echoes from surrounding areas of the tooth, such as soft tissues, bone, periodontal pockets etc.

BRIEF DESCRIPTION OF THE DRAWINGS

[0009] FIG. 1 shows a cross-sectional side view of a tooth and an example ultrasonic dental probe.

[0010] FIG. 2 shows a schematic top view of an example system for positioning a transducer of the FIG. 1 ultrasonic dental probe.

[0011] FIG. 3 shows example positions of the axis of the FIG. 1 ultrasonic dental probe relative to the tooth.

[0012] FIG. 4 shows a cross-sectional view of a tooth and an example ultrasonic dental probe having a cylindrical tip for monitoring a drilling process.

[0013] FIG. 5 shows a cross-sectional view of a crowned tooth and the FIG. 1 ultrasonic dental probe.

[0014] FIG. 6 shows a cross-sectional view of a filled tooth and the FIG. 1 ultrasonic dental probe.

[0015] FIG. 7 shows example A-scans of a sample tooth.

[0016] FIG. 8 shows an example sector scan identifying the pulp chamber.

[0017] FIG. 9 schematically shows the flow of an example dental assessment system.

[0018] FIG. 10 shows a perspective view of an example dental diagnostic device.

DETAILED DESCRIPTION OF THE PRESENTLY PREFERRED EMBODIMENT

[0019] Referring to FIGS. 1 and 2, a handheld dental probe 1 is used to examine internal formations of a tooth 2. The dental probe 1 includes an ultrasonic transducer 3, which is configured to emit an ultrasonic pulse 4 into the tooth 2 at high frequency (e.g., 20 MHz or more), and position sensors 5.

[0020] Internal structures of the tooth 2 reflect the ultrasonic pulse 4 back to the dental probe 1 as reflected signals 4a. The reflected signals 4a (or echoes) received by the transducer 3 comprise reflections from various internal structures of the tooth 2, including an interface 8 between an enamel layer 7 and a dentine layer 9, and an interface 10 between the dentine layer 9 and a pulp layer 11. The thickness of a particular layer, or the distance to the corresponding interface (e.g. dentine-pulp interface), can be determined from the time of flight of the ultrasonic echo reflected by that interface.

[0021] In this example, the position sensors 5 are used to establish a direction of incidence of each ultrasonic pulse 4 based on at least two angles of deviation of a transducer axis A from a reference axis R. In this example, θ_1 represents an angle of deviation in a vertical plane, and θ_2 represents an angle of deviation in a horizontal plane. The reference axis R

is established normal to a point of contact **6** between the tooth **2** and the probe **1** in one example.

[0022] The output data of the position sensors **5** (θ_1 and θ_2) is saved with the waveform of the reflected signals **4a** on a computer **12**. That is, the echo waveform is associated with angular coordinates θ_1 and θ_2 , which indicate the direction of incidence of the ultrasonic pulse **4** that produced the echo, and saved.

[0023] In this example the angle position sensors are angular velocity gyro-sensors based on quartz crystals. A person skilled in the art and having the benefit of this disclosure would know how to incorporate such sensors into the probe **1**. As known, such quartz-based crystals are used in electronic devices like digital and video cameras, handheld GPS navigation devices, etc.

[0024] In one example, the dental probe **1** is placed at some point of interest on the tooth surface during examination, and the dentist manually tilts the probe **1** along path P_i for example, in different directions keeping fixed the point of contact **6** between the probe and the tooth.

[0025] In another example, an electromechanical tilting of the transducer **3** is implemented to automate the angular motion of the transducer **3** along path P_2 and systematically sample within a narrow 3-D sector in the neighborhood of the reference axis **R**. In such an example, the dentist holds the tip of the probe **1** against the tooth surface at **6**, and the tilting mechanism (not shown) changes the ultrasonic incidence angle by tilting the transducer **3** with respect to the reference axis **R** in two mutually perpendicular planes. At each whole angle, an echo waveform is saved together with the two angles of the transducer **3** tilt. The stored collection of echo waveforms and angles can be ordered according to the values of the transducer tilt and readily displayed in the form of a volumetric sector scan (3-D image) or a sequence of plane sector scans (2-D images).

[0026] The electromechanical tilting may be implemented using a variety of techniques. In one example, the whole angle is sampled systematically by regular scanning along pre-defined trajectories. Another example randomly samples the whole angle. Since the required tilting range is relatively small, two piezo linear actuators may be used for both approaches.

[0027] A single spatial oscillator (spring based) is used to sample the whole angle in an uncontrolled fashion in one example. Other example actuators include mechanical actuators, piezo-bimorph actuators, magnetostrictive actuators, etc. The angular position of the probe, in one example, is derived from the actual or commanded displacement of the actuator(s). In another example, the angular position of the probe is derived from the angular position sensors either mounted directly on the probe or in contact with the probe.

[0028] In one example, acoustic contact between the ultrasonic probe and the tooth surface at **6** is maintained by providing a laminar water flow in the contact area. Certain hygienic coupling gels can be used as well. In another example, the ultrasonic coupling is provided with an elastic layer bonded to the contact surface of the ultrasonic probe.

[0029] If the automated tilting is implemented, the transducer **3** moves inside a housing **13** at the end of the handheld probe **1**. The housing **13** is filled with water or gel in one example. An ultrasonically transparent membrane **14** covers an opening in the contact face of the housing **13** to facilitate establishing the acoustic coupling between the housing **13** and the tooth **2**.

[0030] In this example, since stored ultrasonic waveforms are associated with the angular data determining the direction of the transducer **3** with respect to the reference direction **R** (e.g. normal to the tooth surface), the extracted distance to the interface **6** is also associated with a certain direction of propagation inside the tooth. Changing the angle of incidence by manually (or automatically) tilting the transducer **3** changes the direction of propagation inside the tooth **2** and thus the distances to the structural interfaces from the probe tip, calculated along the ultrasonic propagation path. This information can be relied upon to determine the nearest point of a given interface to the point **6** (at the tip of the probe). This information can be used to reconstruct spatial geometry of the internal tooth structures within the 3-D sector insonified by the ultrasonic transducer **3**. Examination of this reconstructed geometry can reveal dental interfaces and help identify their closest points to the transducer tip, such as closest point of dentin/pulp interface (which, as known, is critical for monitoring the tooth drilling processes).

[0031] The volumetric sector scan approaches described herein provides more accurate measurements of the distance between the transducer tip and the chosen interface (e.g. dentine/pulp) than a single scan approach because, as shown in FIG. 3, the received echo of the prior art single scan approaches may not correspond to the nearest interface point for certain positions of the transducer axis A_{1-6} .

[0032] Referring to FIG. 4, an ultrasonic transducer **3** equipped with a cylindrical tip **15** produces the ultrasonic pulse **4** as the probe tip **15** inserted into the bore **16** advances the bore in the enamel layer **7** and part of the dentine layer **9** of the tooth **2** by drilling and removing tooth tissues. The thickness of the residual portion of the dentine layer **9** may be calculated from the acoustic time of flight between the bottom of the drilled bore **16** and the dentine-pulp interface, for example.

[0033] Referring to FIG. 5, a crown-type dental prosthesis **35** attaches to the tooth **2** with a layer of adhesive **17** resulting in a crown-adhesive interface **18** and an adhesive-enamel interface **19**. The ultrasonic transducer **3** mounted in the handheld dental probe **1** without the tip, or inside the probe **1** (FIG. 2) with the tip attached, directs the ultrasonic pulse **4** toward the tooth **2** and the crown **35**. The crown-adhesive interface **18** and the adhesive-enamel or adhesive-dentine interface **19** both produce distinguishable echoes. Flaws or voids **20** in the adhesive can be located by interpreting amplitude increases and changes in the returning echoes of the ultrasonic pulse **4**. For example, a distortion in the return echo may identify the adhesive void **20** or a shrinkage cavity **21** between the tooth **2** and the filling **22** (FIG. 6).

[0034] FIG. 8 shows an example sector scan **39** from a tooth sample (in vitro). In this example, the distance d corresponds generally to the distance from the tooth surface to the pulp chamber. The sector scan **39** is a result of processing collected A-scans **37** (FIG. 7) and corresponding angle position data in a computer. Each such A-scan **37** corresponds to a particular value of the tilt angle and contains an echo from the tooth surface and subsequent reflections from internal structures. In this example the reflection **38** is from the pulp chamber. The distance d to the pulp chamber from the tooth surface is calculated as a product the time delay between respective echoes and the average speed of sound in the tooth material along the propagation path.

[0035] Referring to FIG. 9, the flow of an example proposed dental assessment system incorporates the handheld

dental probe **1** with embedded angular position sensors **5** connected with computer **12**. As shown, the ultrasonic transducer **3** and the angular position sensors **5** are bundled with the dental probe **1**. Housing **13** is designed to allow for achieving varying angles of incidence of the ultrasonic pulse **4** to the contact area between the probe's tip and tooth surface by automatic or manual means.

[0036] To achieve maximum penetration of the ultrasonic pulse **4** into the tooth **2** when the dental layers are deposited parallel to interfaces, the axis X of the housing **13** should remain approximately perpendicular to the surface of the tooth **2**. Surface irregularities of the tooth **2** may increase the difficulties in maintaining this position and may produce undesirable distorted echoes of the ultrasonic pulse **4** that should be properly treated. To avoid this, the operator may manually adjust orientation of the probe **1** until a better reference position is achieved.

[0037] Depending on the space constraints and handling needs, other many designs of the dental probe **1** may be used. For example, a tapered ultrasonic guide element, a cylindrical probe tip **15** (FIG. 4), a solid or elastic cone-shaped guide element, or a hollow solid or elastic cone-shaped guide filled with water or hygienic gel all may be used. To comply with bio-safety and hygienic standards, the handheld dental probe **1** typically incorporates bio-protection means, such as a sterilizable or disposable parts or a disposable sterile sleeve.

[0038] Since the proposed device is designed for operation at high ultrasonic frequencies (tens of MHz) that are strongly attenuated by most materials, the example ultrasonic probe is engineered to minimize the associated energy losses. This is achieved, in one example, by decreasing the length of propagation inside the probe and optimizing the acoustic coupling to the tooth surface. For example, a thin layer of elastic material (e.g. natural rubber, plastisol, etc.) may be adhesively bonded directly to the contact surface of the transducer tip. In another embodiment, such a layer is bonded to the contact surface of a (cylindrical or cone-shaped) delay line or a liquid-filled chamber where the transducer is electromechanically tilted. The thickness and material of said elastic

layer may vary depending on the application needs and the acoustic properties of the material at the operating frequency. [0039] The interchangeable housing **13** in the current examples facilitate maintaining the position of the probe **1** and directing the ultrasonic pulse **4** at the tooth **2**. The shape of the housing **13** may be modified to enable access to certain hard to reach areas, e.g., between the teeth **2** or at the lower edge of the crown **10**.

[0040] The dental probe **1** communicates signals from the ultrasonic transducer **3** to the pulser-receiver **18**, and signals from the angular position sensors **5** to the conditioning circuit. An analog-to-digital converter **96** transforms the ultrasonic and angular position data to the appropriate digital format and transfers them through a controller **100** to a computer **12**. The computer **12** processes and analyzes the input data and displays the results in a numerical or graphical form.

[0041] FIG. 10 shows another example of the housing **13** incorporating an ultrasonic transducer **3** and mounted to the probe **1**. The example computer **12** communicates with the pulser-receiver and angular position sensors (not shown) in the probe **1**. When directed at the tooth **2** (FIG. 1), the computer **12** displays on a display **45**, in real time and in a graphical format, the measurements of the tooth **2** based on the echoes from internal features of the tooth **2**. In addition, the display **45** shows real-time visualization of the tooth **2** and any noted defects in the tooth **2**, to facilitate real time examination of the tooth **2**. In another example, the dental probe may be separately connected to an ultrasonic generator and a graphical display.

What is claimed is:

1. A method for evaluating the structure of a tooth including the steps of:

- a) generating a signal;
- b) receiving a return signal;
- c) receiving position data about the signal, the return signal, or both; and
- d) determining the geometry of said tooth using said step b).

* * * * *

专利名称(译)	用于评估内部牙齿结构的超声波装置		
公开(公告)号	US20100227295A1	公开(公告)日	2010-09-09
申请号	US12/708741	申请日	2010-02-19
[标]申请(专利权)人(译)	MAEV ROMAN GR MALYARENKO EUGENE V ILYUTOVICH ALEXANDER		
申请(专利权)人(译)	MAEV ROMAN GR MALYARENKO EUGENE V ILYUTOVICH ALEXANDER		
当前申请(专利权)人(译)	MAEV ROMAN GR MALYARENKO EUGENE V ILYUTOVICH ALEXANDER		
[标]发明人	MAEV ROMAN GR MALYARENKO EUGENE V ILYUTOVICH ALEXANDER		
发明人	MAEV, ROMAN GR. MALYARENKO, EUGENE V. ILYUTOVICH, ALEXANDER		
IPC分类号	A61B8/00 A61C19/04		
CPC分类号	A61B8/0875 A61C19/04 A61B8/483		
优先权	61/153759 2009-02-19 US		
其他公开文献	US10603008		
外部链接	Espacenet USPTO		

摘要(译)

本发明的示例性实施例包括用于评估牙齿内部结构的方法和装置。在一个示例中，该方法包括以相对于局部牙齿表面的各种入射方向（入射角）从牙齿表面上的给定点向牙齿发射一系列超声脉冲，记录相应的超声波序列。来自不同内部牙齿形成的回波，并处理收集的超声脉冲回波和脉冲方向数据，以定量或图形形式呈现牙齿的内部结构。

