



US 20080188754A1

(19) **United States**(12) **Patent Application Publication**
Peszynski et al.(10) **Pub. No.: US 2008/0188754 A1**(43) **Pub. Date: Aug. 7, 2008**(54) **ULTRASOUND PROBE HAVING AN
OPERATIONAL INDICATOR ASSEMBLY**(75) Inventors: **Michael Peszynski**, Newburyport,
MA (US); **Heather Knowles**,
Devens (FR)


Correspondence Address:

**PHILIPS INTELLECTUAL PROPERTY &
STANDARDS****P.O. BOX 3001****BRIARCLIFF MANOR, NY 10510**(73) Assignee: **KONINKLIJKE PHILIPS
ELECTRONICS, N.V.**,
EINDHOVEN (NL)(21) Appl. No.: **11/912,514**(22) PCT Filed: **Apr. 20, 2006**(86) PCT No.: **PCT/IB2006/051224**

§ 371 (c)(1),

(2), (4) Date: **Oct. 25, 2007****Related U.S. Application Data**(60) Provisional application No. 60/674,491, filed on Apr.
25, 2005.**Publication Classification**(51) **Int. Cl.**
A61B 8/13 (2006.01)(52) **U.S. Cl.** **600/459**(57) **ABSTRACT**

An ultrasound probe (202) having an operational indicator assembly (204) for indicating operational data relating to the ultrasound probe (202), and especially data relating to the sterility of the ultrasound probe (202), is provided. The ultrasound probe (202) has a housing (203) fabricated from materials suitable for internal and non-internal medical use. At least one ultrasound transducer (209) is housed by the housing (203) and positioned to direct ultrasound energy along a propagation path to the patient. The operational indicator assembly (204) indicates operational data relating to the ultrasound probe (202) to an operator thereof, and especially data relating to the disinfection status of the ultrasound probe (202).

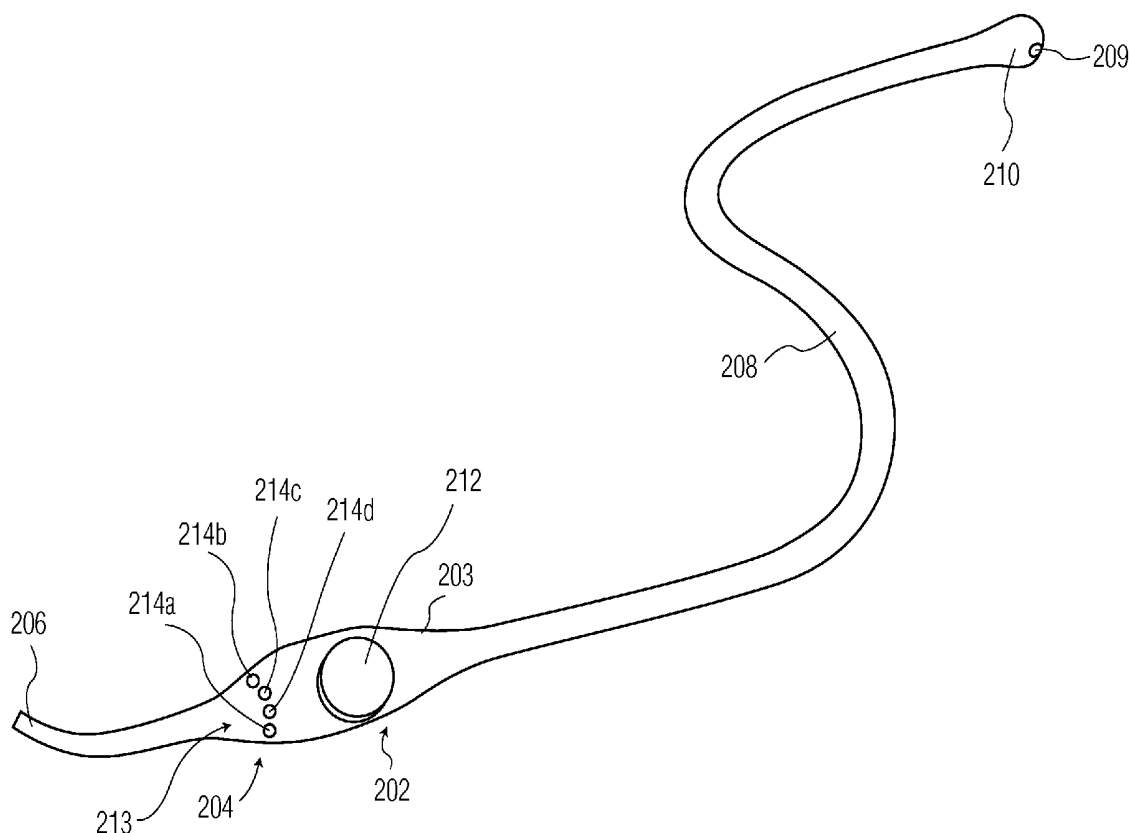

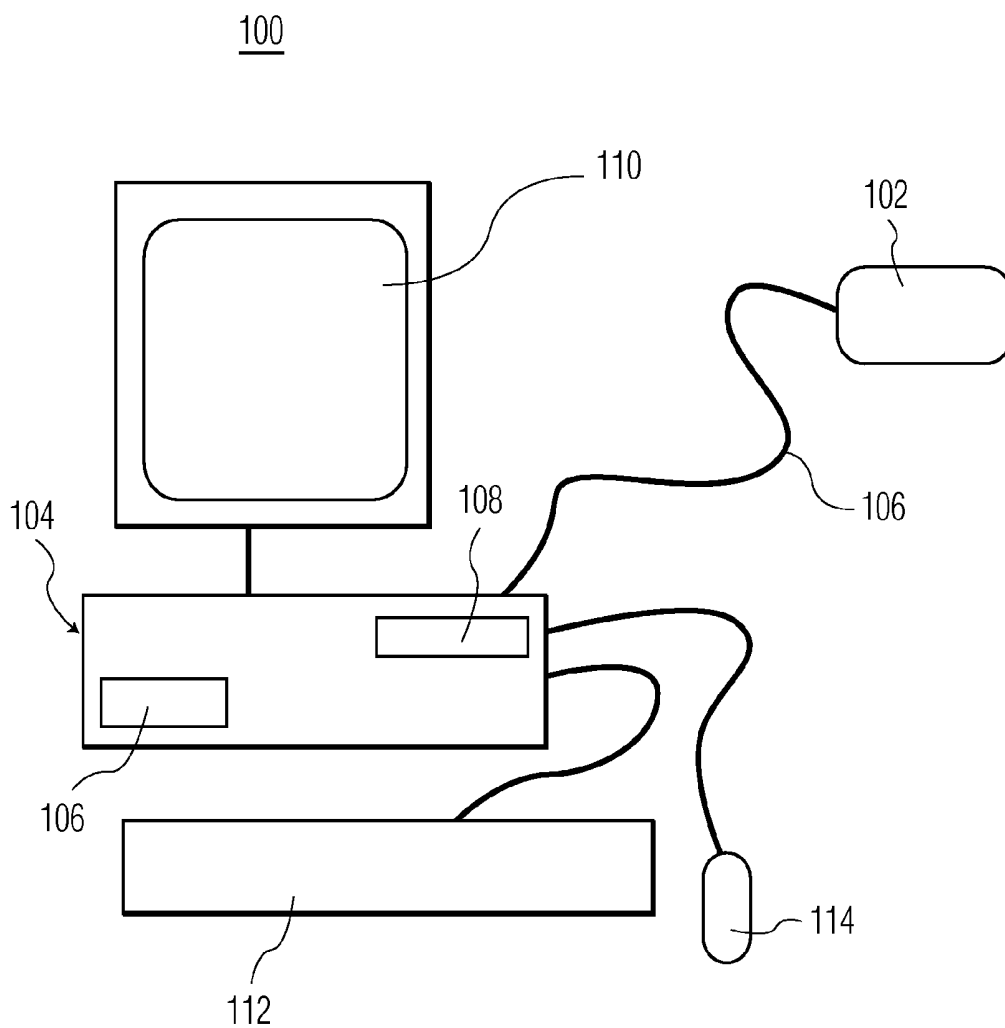


FIG. 1
PRIOR ART

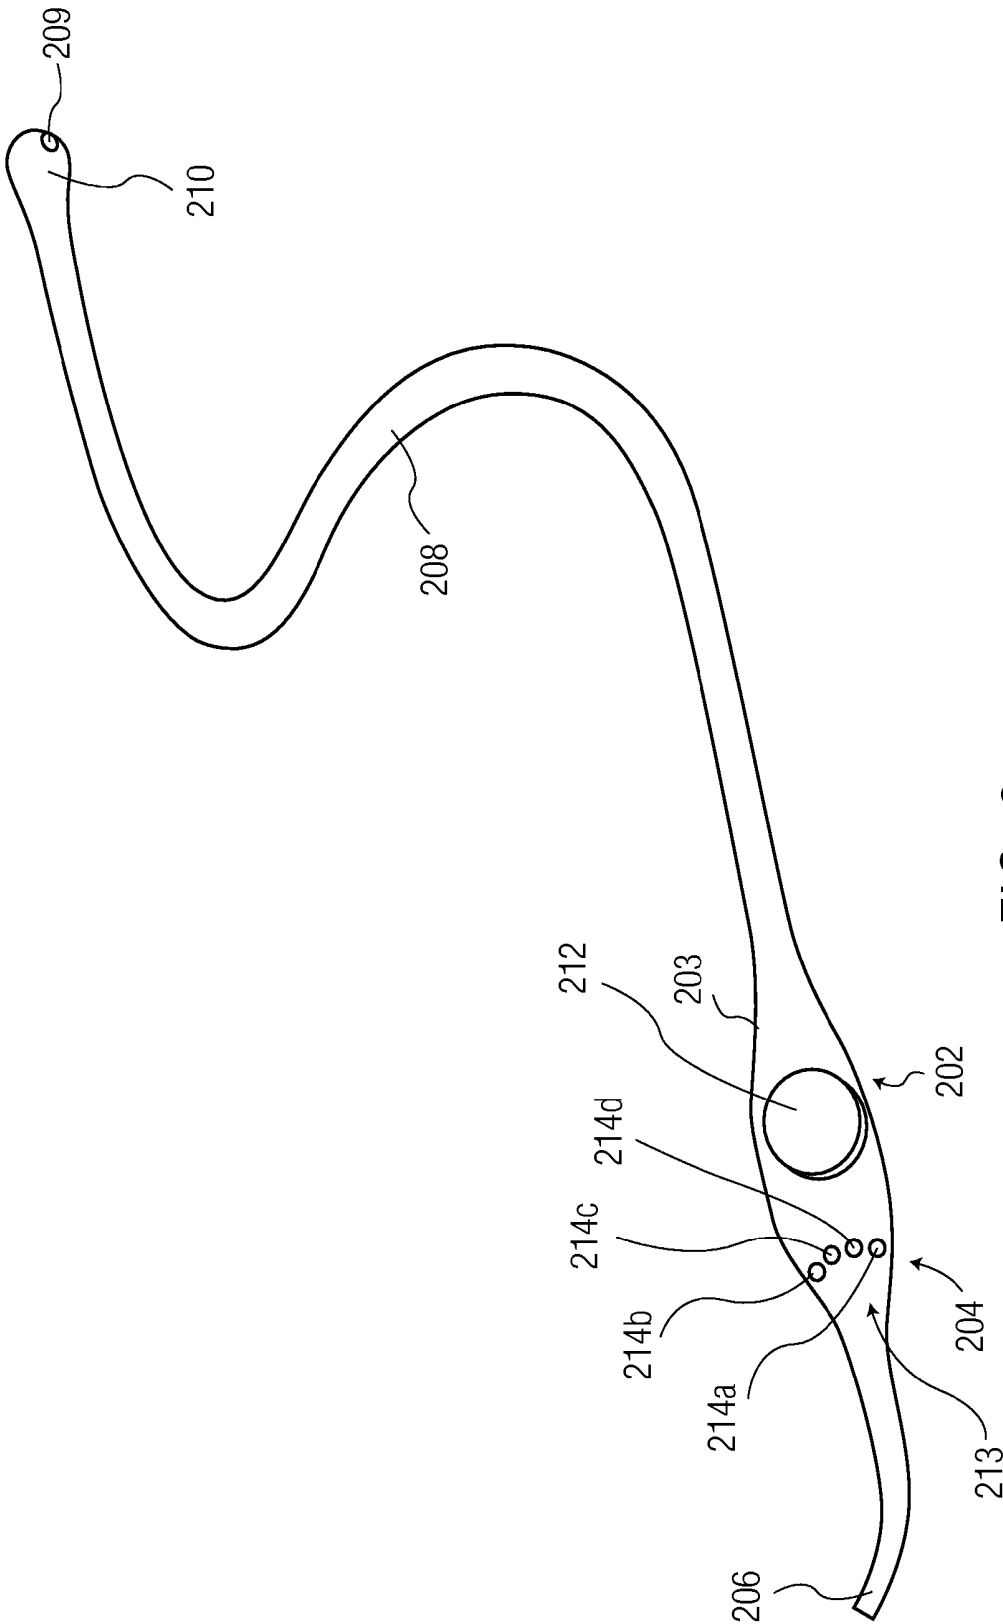


FIG. 2

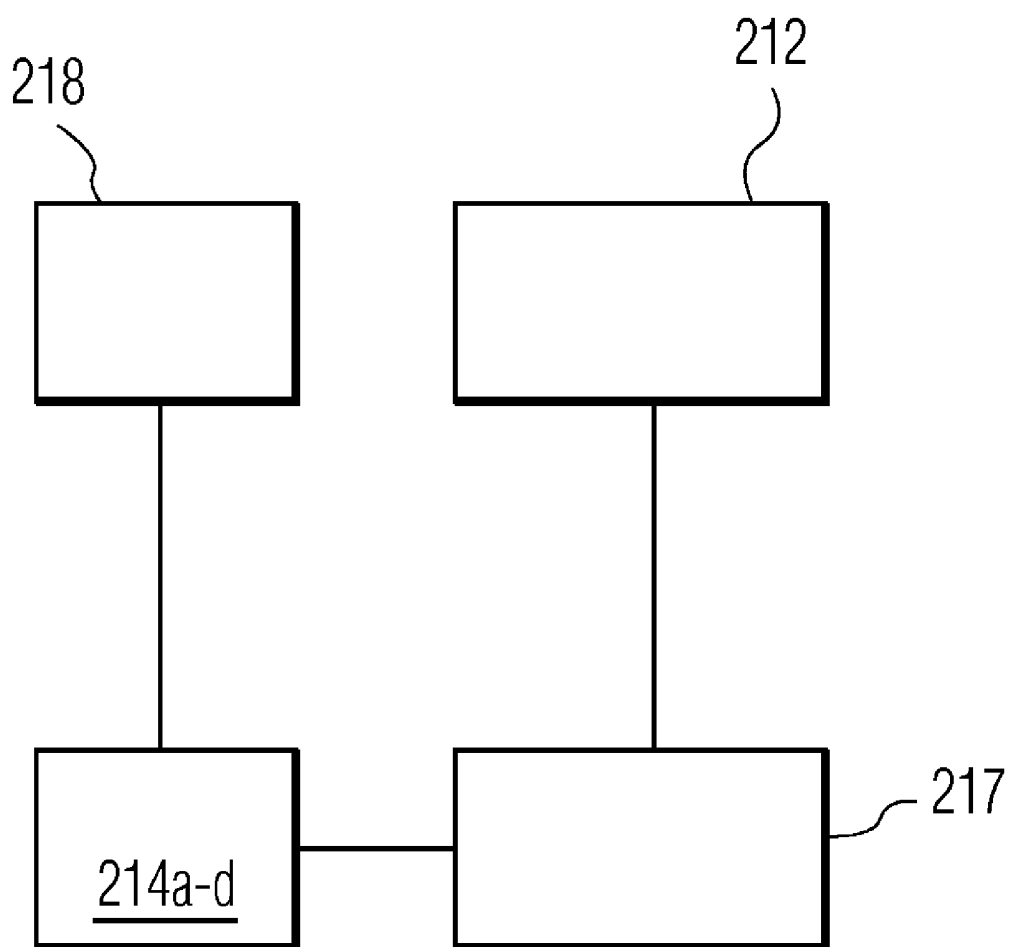


FIG. 3

ULTRASOUND PROBE HAVING AN OPERATIONAL INDICATOR ASSEMBLY

BACKGROUND OF THE DISCLOSURE

[0001] 1. Field of the Invention

[0002] The present disclosure relates generally to ultrasound probes used in medical diagnostic and treatment procedures. In particular, the present disclosure relates to an ultrasound probe having an operational indicator assembly.

[0003] 2. Description of the Related Art

[0004] Medical ultrasound imaging has become a popular means for visualizing and medically diagnosing the condition and health of interior regions of the human body. With this technique, a disinfected ultrasound probe having an array of acoustic transducers or a single transducer, in operative communication with an ultrasound system console via an interconnection cable, is provided against the patient's tissue or inserted within the patient's gastrointestinal tract where it is actuated to emit and receive focused ultrasound waves in a scanning fashion. The scanned ultrasound waves, or ultrasound beams, allow the systematic creation of image slices of the patient's internal tissues for display on a monitor of the ultrasound system console.

[0005] During ultrasonic imaging, the disinfected ultrasound probe is susceptible to becoming contaminated. Accordingly, it is an object of the present disclosure to present a system for providing operational data relating to the ultrasound probe, and especially data relating to the disinfection state of the ultrasound probe.

SUMMARY OF THE DISCLOSURE

[0006] The present disclosure provides an ultrasound probe having an operational indicator assembly for indicating operational data relating to the ultrasound probe, and especially data relating to the disinfection state of the ultrasound probe. In particular, the present disclosure provides an ultrasound probe having a housing fabricated from materials suitable for internal and non-internal medical use. At least one ultrasound transducer is housed by the housing and positioned to direct ultrasound energy along a propagation path to the patient. The operational indicator assembly indicates operational data relating to the ultrasound probe to an operator thereof, and especially data relating to the disinfection state of the ultrasound probe.

[0007] In particular, the present disclosure provides an ultrasound probe having a housing; at least one ultrasound transducer within the housing and positioned to direct ultrasound energy along a propagation path; and an operational indicator assembly provided to the housing and having means for controlling at least one indicator system for indicating at least one operational characteristic relating to the ultrasound probe. The at least one indicator system can include a plurality of LEDs or a liquid crystal display (LCD) for indicating the at least one operational characteristic relating to the ultrasound probe. One of the at least one operational characteristic indicated by the at least one indicator system relates to the disinfection status of the ultrasound probe.

[0008] Preferably, the means for controlling includes a programming button positioned on the housing for transmitting

at least one signal to at least one processor and/or EEPROM for controlling the at least one indicator system.

BRIEF DESCRIPTION OF THE DRAWINGS

[0009] These and other features, aspects, and advantages of the present disclosure will become better understood with regard to the following description, appended claims, and accompanying drawings wherein:

[0010] FIG. 1 is an illustration of a prior art ultrasound medical imaging system;

[0011] FIG. 2 illustrates an exemplary embodiment of an ultrasound probe having an operational indicator assembly and configured for internal use in accordance with the present disclosure; and

[0012] FIG. 3 illustrates a block diagram of the ultrasound probe shown by FIG. 2.

DESCRIPTION OF THE PREFERRED EMBODIMENTS

[0013] Referring to FIG. 1 a prior art medical ultrasound imaging system 100 is shown. The system 100 includes an ultrasound imaging probe 102 connected to an imaging workstation 104. The imaging workstation 104 contains one or more processors 106 and at least one storage device 108, such as a hard drive, RAM disk, etc. The storage device(s) 108 may be used for storing the controlling and imaging software for the ultrasound system 100 as well as providing temporary and long term storage of image data acquired by the ultrasound probe 102. The ultrasound imaging system 100 also provides a video display 110 and user input devices, including a keyboard 112 and a mouse 114.

[0014] The processor 106 is configured to execute controlling and imaging software. The imaging software allows the operator of the system 100 to visualize and manipulate the data received from the ultrasound probe 102.

[0015] An exemplary embodiment of the present disclosure, as shown in FIG. 2, provides an ultrasound medical imaging probe 202 having a housing 203 and an operational indicator assembly 204 for indicating operational data relating to the ultrasound probe 202 to an operator thereof, and especially data relating to the disinfection status of the ultrasound probe 202. The probe 202 further includes a cable 206 for connecting to an imaging workstation, such as imaging workstation 104 shown by FIG. 1. An articulating stalk 208 is provided for enabling the probe 202 to be inserted into a patient's gastrointestinal tract for performing imaging operations as known in the art. A distal end 210 of the articulating stalk 208 houses an ultrasound transducer array or an ultrasound transducer 209 and related imaging circuitry as known in the art for performing the imaging operations.

[0016] In one embodiment, the operational indicator assembly 204 includes a programming button 212 and an indicator system 213 having a series of LEDs 214a-d positioned in proximity to the programming button 212 for indicating operational information to an operator of the probe 202, including information relating to the disinfection status of the probe 202. In accordance to which LEDs 214a-d are lit, the operator associates the lit LEDs as forming a code which is then used to determine information regarding the probe 202. The information is determined by corresponding the code to at least one rule of a set of predetermined rules. For example, if none of the LEDs 214a-d are lit, then the probe

202 is high level disinfected (e.g., code: none lit; rule: probe is high level disinfected). If LED **214a** is lit, then the probe **202** has been sterilized.

[0017] Other operational data can also be indicated by lighting one or more of the LEDs **214a-d**, such as visual inspection has passed, electrical test status, and the probe **202** needs to be serviced. Correspondingly, the LEDs could indicate this status. For example, if LED **214b** is lit, the probe has passed visual inspection. If LED **214c** is lit, the probe has passed an electrical safety test, etc. The LEDs **214a-d** are progressively lit by the operator pressing on programming button **212** to indicate the disinfection status of the probe and other data. For example, if none of the LEDs **214a-d** are lit and the operator presses the programming button **212** one time, LED **214a** is lit; two times, LED **214b** is lit; three times, LED **214c** is lit; four times, LED **214d** is lit; five times, LEDs **214a** and **214b** are lit; six times, LEDs **214a** and **214c** are lit; seven times, LEDs **214a** and **214d** are lit; eight times, LEDs **214b** and **214c** are lit; and so on.

[0018] Other configurations are envisioned within the scope of the present disclosure for indicating operational data relating to the probe **202**, including data relating to the disinfection status of the probe **202**, using the LEDs **214a-d** of the operational indicator assembly **204**. For example, LED **214a** can be a green LED which is lit automatically or manually when the probe **202** is actuated for performing an imaging operation, and LED **214b** can be a red LED which is lit automatically or manually when the probe **202** is de-actuated following the imaging operation to indicate the probe **202** is no longer disinfected or sterile.

[0019] By pressing the programming button **212**, at least one processor and/or EEPROM **217** within the probe **202** is programmed to light the one or more LEDs **214a-d** as described above for indicating operational data relating to the probe **202**. It is also envisioned for the indicator assembly **213** to include a liquid crystal display (LCD) or other indicator means for indicating and/or displaying operational data, including data relating to the disinfection status of the probe **202**.

[0020] The LEDs **214a-d** provide a quick and efficient safety check regarding the operational and disinfection status of the probe **202**, prior to the use of the probe **202** by the operator. The LEDs **214a-d** are powered by the imaging system **100** when the probe **202** is plugged thereto and by a battery **218** housed by the probe **202** when the probe **202** is unplugged from the imaging system **100**. The battery **218** is preferably a rechargeable nickel metal hydride battery as known in the art.

[0021] In another embodiment, the disinfection status of the probe **202** can be programmed electronically by operatively interfacing the probe **202** to an automated disinfection machine (automated reprocessor), which programs the at least one processor and/or EEPROM **217** and changes the status indicator LEDs **214a-d**, based on the probe **202** passing or failing the disinfection cycle, as specified in the reprocessor software. Similarly, the probe **202** could be operatively interfaced with a leakage current tester, which programs the at least one processor and/or EEPROM **217** to allow display of the status on the probe **202** and on a display of the leakage current tester. Additionally, in either of these embodiments, the at least one processor and/or EEPROM **217** could lock out usage of the probe **202** under unsafe conditions.

[0022] The imaging workstation **104** can be used to interrogate at least one processor and/or EEPROM **217** for receiv-

ing signals relating to operational data of the probe **202**. The imaging workstation **104** can then interpret the signals and display the operational data on the video display **110** for viewing by the operator and printing by a printer.

[0023] The described embodiments of the present disclosure are intended to be illustrative rather than restrictive, and are not intended to represent every embodiment of the present disclosure. Various modifications and variations can be made without departing from the spirit or scope of the disclosure as set forth in the following claims both literally and in equivalents recognized in law.

1. An ultrasound probe (**202**) comprising:

a housing (**203**);

at least one ultrasound transducer (**209**) within the housing (**203**) and positioned to direct ultrasound energy along a propagation path; and

an operational indicator assembly (**204**) provided to the housing (**203**) and having means for controlling at least one indicator system (**213**) for indicating at least one operational characteristic relating to said ultrasound probe (**202**).

2. The ultrasound probe (**202**) according to claim 1, wherein said at least one indicator system (**213**) includes a plurality of LEDs (**214a-d**).

3. The ultrasound probe (**202**) according to claim 1, wherein said at least one indicator system (**213**) includes a liquid crystal display (LCD).

4. The ultrasound probe (**202**) according to claim 1, wherein said at least one operational characteristic indicated by the at least one indicator system (**213**) is the disinfection status of the ultrasound probe (**202**).

5. The ultrasound probe (**202**) according to claim 1, wherein the means for controlling includes a programming button (**212**) positioned on the housing (**203**) for transmitting at least one signal to at least one processor (**217**) for controlling the at least one indicator system (**213**).

6. The ultrasound probe (**202**) according to claim 1, wherein the means for controlling includes a programming button (**212**) positioned on the housing (**203**) for transmitting at least one signal to an EEPROM (**217**) for controlling the at least one indicator system (**213**).

7. The ultrasound probe (**202**) according to claim 1, wherein the means for controlling prevents operation of the probe (**202**) based on the at least one operational characteristic relating to said probe (**202**).

8. The ultrasound probe (**202**) according to claim 1, further comprising means for operatively connecting said probe (**202**) to at least one external device capable of controlling the at least one indicator system (**213**).

9. A method for indicating at least one operational characteristic of a medical instrument, the method comprising:

providing an operational indicator assembly (**204**) to the medical instrument having means for controlling at least one indicator system (**213**) for indicating the at least one operational characteristic relating to said medical instrument; and

activating the operational indicator assembly (**204**) to display a code via the at least one indicator system (**213**), wherein said code corresponds to the at least one operational characteristic in accordance with a set of predetermined rules.

10. The method according to claim 9, wherein said at least one indicator system (**213**) includes a plurality of LEDs (**214a-d**).

11. The method according to claim 9, wherein said at least one indicator system (213) includes a liquid crystal display (LCD).

12. The method according to claim 9, wherein said at least one operational characteristic indicated by the at least one indicator system (213) is the disinfection status of the medical instrument.

13. The method according to claim 9, wherein the means for controlling includes a programming button (212) for transmitting at least one signal to at least one processor (217) for controlling the at least one indicator system (213).

14. The method according to claim 9, wherein the means for controlling includes a programming button (212) for transmitting at least one signal to an EEPROM (217) for controlling the at least one indicator system (213).

15. The method according to claim 9, wherein the means for controlling prevents operation of the medical instrument based on the at least one operational characteristic relating to said medical instrument.

16. The method according to claim 9, further comprising operatively connecting said medical instrument to at least one external device capable of controlling the at least one indicator system (213).

17. A medical ultrasound imaging system comprising: an ultrasound probe (202) having at least one ultrasound transducer (209) for directing ultrasound energy along a propagation path; and

an operational indicator assembly (204) provided to a housing (203) of the ultrasound probe (202), said operational indicator assembly (204) having means for controlling at least one indicator system (213) for indicating at least one operational characteristic relating to said ultrasound probe (202).

18. The imaging system according to claim 17, wherein said at least one operational characteristic indicated by the at least one indicator system (213) is the disinfection status of the ultrasound probe (202).

19. The imaging system according to claim 17, wherein the means for controlling prevents operation of the ultrasound probe (202) based on the at least one operational characteristic relating to said ultrasound probe (202).

20. The imaging system according to claim 17, further comprising means for operatively connecting said ultrasound probe (202) to at least one external device capable of controlling the at least one indicator system (213).

* * * * *

专利名称(译)	超声探头具有操作指示器组件		
公开(公告)号	US20080188754A1	公开(公告)日	2008-08-07
申请号	US11/912514	申请日	2006-04-20
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦电子N.V.		
当前申请(专利权)人(译)	皇家飞利浦电子N.V.		
[标]发明人	PESZYNSKI MICHAEL KNOWLES HEATHER		
发明人	PESZYNSKI, MICHAEL KNOWLES, HEATHER		
IPC分类号	A61B8/13		
CPC分类号	A61B8/00 A61B8/467 A61N7/00 A61B2560/0276 A61B2019/4873 A61B8/461 A61B2090/0814 A61B2090/0815		
优先权	60/674491 2005-04-25 US		
其他公开文献	US9339253		
外部链接	Espacenet USPTO		

摘要(译)

提供了一种超声探头 (202)，其具有用于指示与超声探头 (202) 相关的操作数据的操作指示器组件 (204)，尤其是与超声探头 (202) 的无菌有关的数据。超声探头 (202) 具有由适于内部和非内部医疗用途的材料制成的壳体 (203)。至少一个超声换能器 (209) 由壳体 (203) 容纳并定位成沿着传播路径将超声能量引导至患者。操作指示器组件 (204) 向其操作者指示与超声探头 (202) 有关的操作数据，尤其是与超声探头 (202) 的消毒状态有关的数据。

