



US 20100113905A1

(19) **United States**(12) **Patent Application Publication**
Park(10) **Pub. No.: US 2010/0113905 A1**(43) **Pub. Date: May 6, 2010**(54) **ULTRASOUND IMAGE DISPLAY WITH
ADDITIONAL INFORMATION USING PPG
AND ECG SIGNALS****Publication Classification**

- (51) **Int. Cl.**
A61B 5/1455 (2006.01)
A61B 8/14 (2006.01)
(52) **U.S. Cl.** **600/324; 600/443**
(57) **ABSTRACT**

(75) **Inventor: Joong Hoon Park, Seoul (KR)**

Correspondence Address:
JONES DAY
222 EAST 41ST ST
NEW YORK, NY 10017 (US)

(73) **Assignee: Medison Co., Ltd.**(21) **Appl. No.: 12/609,926**(22) **Filed: Oct. 30, 2009**(30) **Foreign Application Priority Data**

Oct. 31, 2008 (KR) 10-2008-0107476

An embodiment for displaying an ultrasound image with additional information using a photoplethysmography (PPG) signal and an electrocardiogram (ECG) signal in an ultrasound system is disclosed. The ultrasound system includes a photoplethysmography (PPG) signal generating unit and an electrocardiogram (ECG) signal generating unit. The PPG signal generating unit and the ECG signal generating unit generate a PPG signal for the target object and an ECG signal for the target object, respectively. An additional information forming unit forms additional information by using the PPG signal and the ECG signal. A display unit displays ultrasound images of the target object together with the additional information.

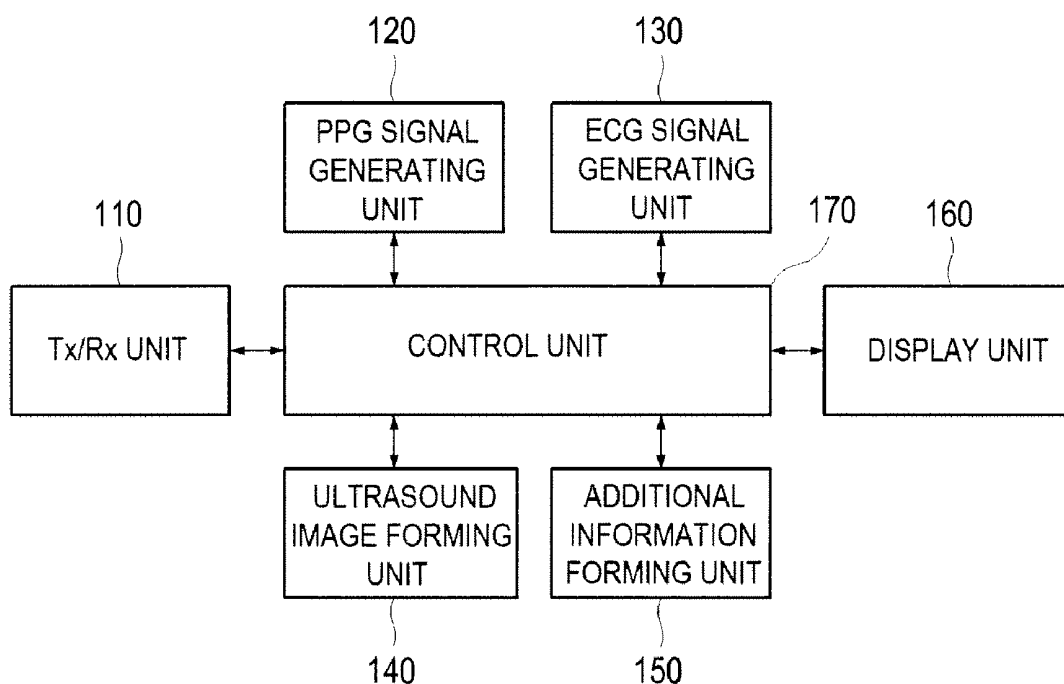
100

FIG. 1

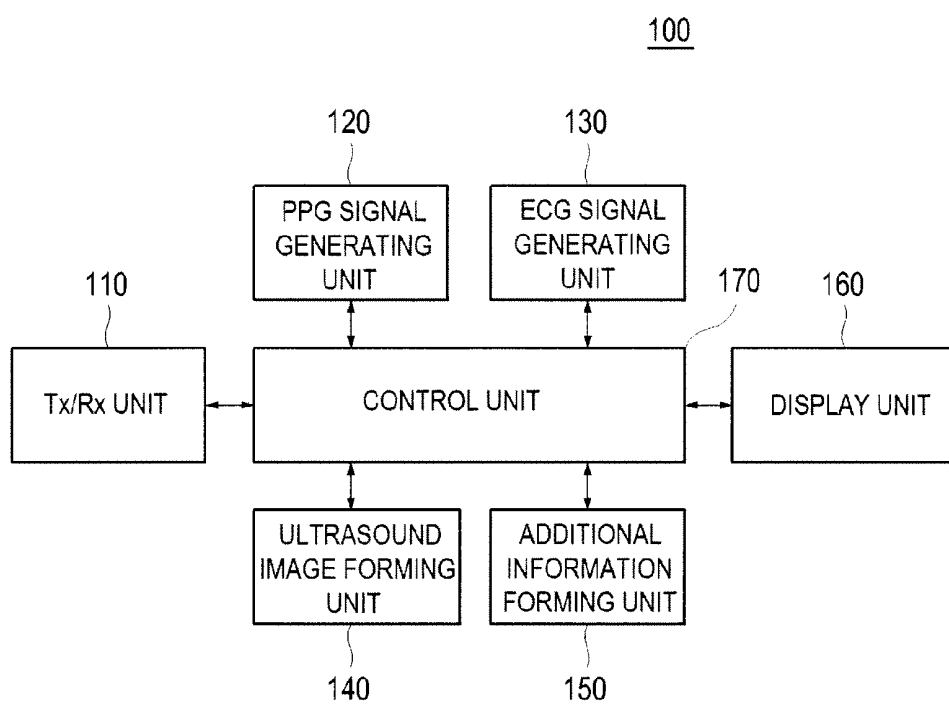


FIG. 2


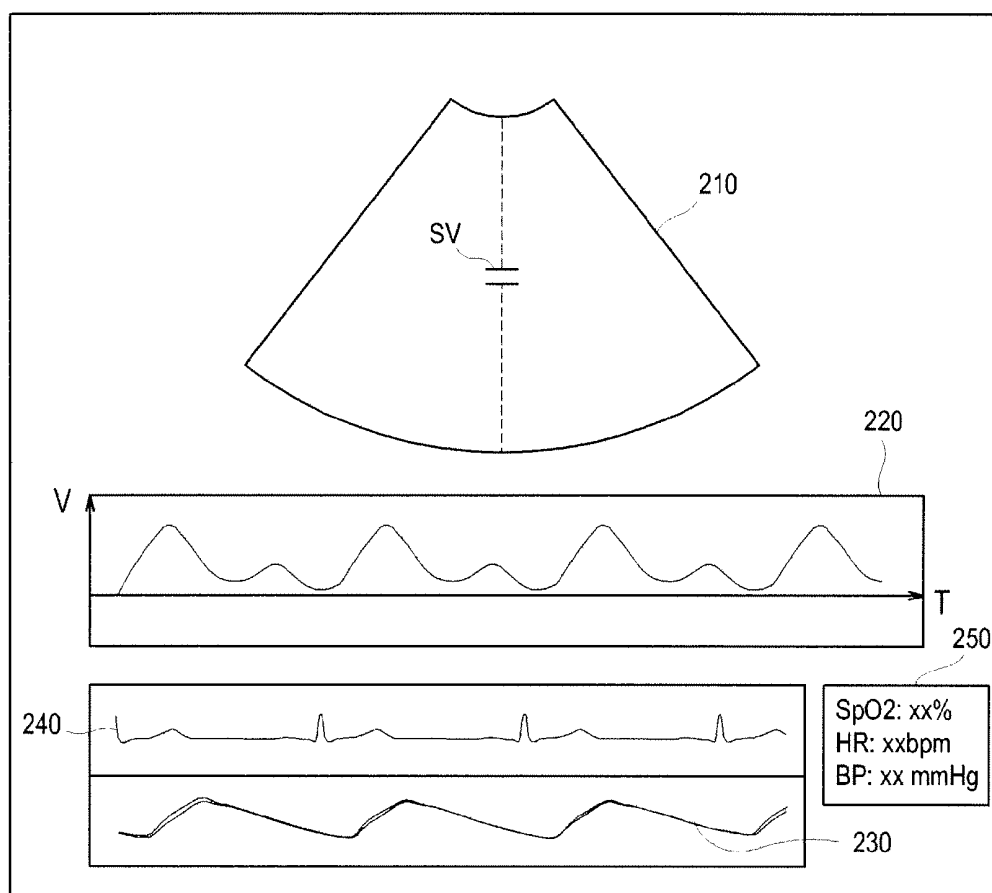


FIG. 3

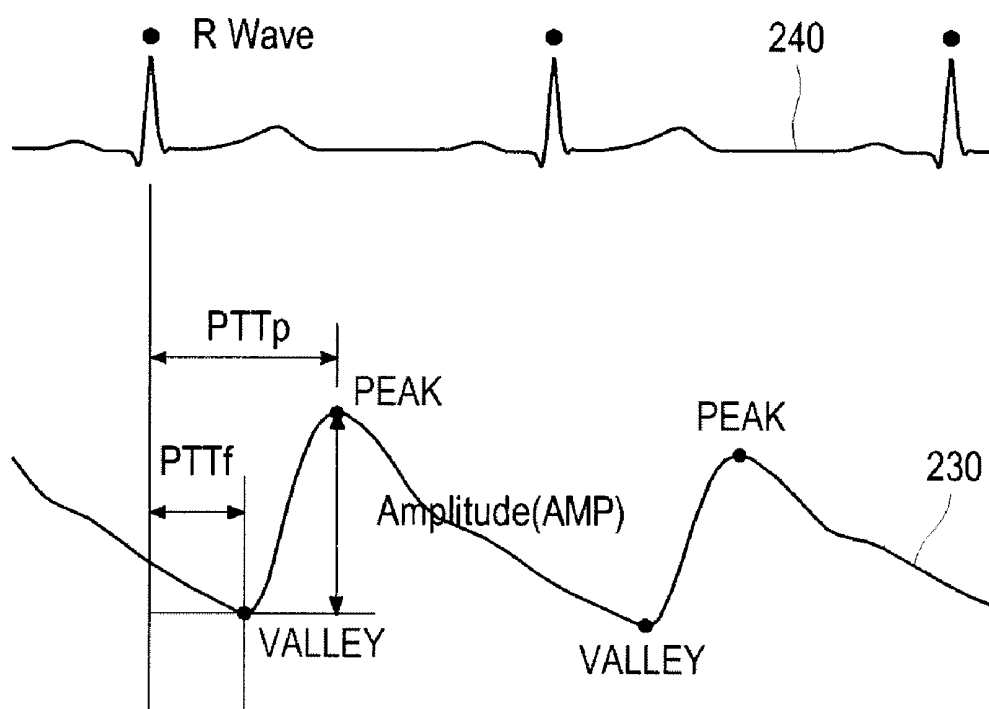

ULTRASOUND IMAGE DISPLAY WITH ADDITIONAL INFORMATION USING PPG AND ECG SIGNALS

[0001] The present application claims priority from Korean Patent Application No. 10-2008-0107476 filed on Oct. 31, 2008, the entire subject matter of which is incorporated herein by reference.

TECHNICAL FIELD

[0002] The present disclosure generally relates to ultrasound systems, and more particularly to an ultrasound image display with additional information using a photoplethysmography (PPG) signal and an electrocardiogram (ECG) signal in an ultrasound system.

BACKGROUND

[0003] Photoplethysmography (PPG) is known as an optical measurement technique that can obtain physiologic information from a target object such as blood oxygen saturation (SpO₂), heart rate, etc. PPG is often performed by using a pulse oximeter. The pulse oximeter is commonly worn on a relative narrow portion of a human body (e.g., finger, ear, etc.) and emits an infrared light and a red light thereto. The pulse oximeter may compute a ratio of red to infrared light absorption of hemoglobin and oxyhemoglobin, and measures variance of blood volume by using the computed ratio to thereby obtain the physiologic information. The physiologic information is important in examining the status of a patient.

[0004] Generally, additional information such as physiologic information and a PPG waveform is very useful for examining a patient. Unfortunately, the conventional ultrasound system does not provide such additional information. Thus, there has been a need for an ultrasound system that can provide such additional information to perform more accurate examination.

SUMMARY

[0005] An embodiment for ultrasound image display with additional information using a photoplethysmography (PPG) signal and an electrocardiogram (ECG) signal is disclosed herein. In one embodiment, by way of non-limiting example, an ultrasound system comprises: a transmission/reception (Tx/Rx) unit operable to transmit ultrasound signals to a target object and receive echo signals reflected from the target object to thereby output receive signals; an ultrasound image forming unit operable to form ultrasound images based on the receive signals; a photoplethysmography (PPG) signal generating unit operable to generate a PPG signal for the target object; an electrocardiogram (ECG) signal generating unit operable to generate an ECG signal for the target object; an additional information forming unit operable to form additional information by using the PPG signal and the ECG signal; and a display unit to display the ultrasound images and the additional information.

[0006] The Summary is provided to introduce a selection of concepts in a simplified form that are further described below in the Detailed Description. This Summary is not intended to

identify key or essential features of the claimed subject matter, nor is it intended to be used in determining the scope of the claimed subject matter.

BRIEF DESCRIPTION OF THE DRAWINGS

[0007] FIG. 1 is a block diagram showing an illustrative embodiment of an ultrasound system.

[0008] FIG. 2 is a schematic diagram showing an example of displaying ultrasound images and additional information.

[0009] FIG. 3 is a schematic diagram showing an example of computing pulse transit times by using a PPG waveform and an ECG waveform.

DETAILED DESCRIPTION

[0010] A detailed description may be provided with reference to the accompanying drawings. One of ordinary skill in the art may realize that the following description is illustrative only and is not in any way limiting. Other embodiments of the present invention may readily suggest themselves to such skilled persons having the benefit of this disclosure.

[0011] FIG. 1 is a block diagram showing an illustrative embodiment of an ultrasound system 100. As shown in FIG. 1, the ultrasound system 100 may include a transmission and reception (Tx/Rx) unit 110. The Tx/Rx unit 110 may be operable to transmit ultrasound signals to a target object and receive echo signals reflected from the target object. The Tx/Rx unit 110 may be further operable to form receive signals based on the echo signals. In one embodiment, the receive signals may include first receive signals obtained in a B-mode and second receive signals obtained in a D-mode. The second receive signals may be obtained by repeatedly transmitting the ultrasound signals to a region of interest, e.g., a sample volume SV (see FIG. 2).

[0012] In one embodiment, the Tx/Rx unit 110 may include a transmit signal generator (not shown) that may be operable to generate a plurality of Tx signals for transmission of the ultrasound signals. The Tx/Rx unit 110 may further include an ultrasound probe (not shown). The ultrasound probe may include an array transducer consisting of a plurality of elements. The array transducer may be either 1D or 2D array transducer, although it is certainly not limited thereto. The array transducer may be operable to generate ultrasound signals in response to the Tx signals. Also, the array transducer may be further operable to convert the echo signals into electrical receive signals.

[0013] The Tx/Rx unit 110 may further include a beam former (not shown) that is coupled to the ultrasound probe. The beam former may be operable to perform analog-to-digital conversion upon the electrical receive signals to thereby output digital receive signals. The beam former may be also operable to apply delays to the digital receive signals in consideration of positions of the transducer elements and focal points, and then may sum the delayed digital receive signals to thereby output a plurality of receive-focused beams.

[0014] The ultrasound system 100 may further include a photoplethysmography (PPG) signal generating unit 120. The PPG signal generating unit 120 may include at least one PPG sensor (not shown). The PPG sensor may be worn on a specific portion of the target object such as a finger, toe, ear, etc. The PPG sensor may emit an infrared light and a red light to the specific portion to thereby detect a blood flow therefrom. The PPG sensor may be operable to generate the PPG

signal based on the blood flow detection. The PPG sensor may include a pulse oximeter and the like.

[0015] The ultrasound system **100** may further include an electrocardiogram (ECG) signal generating unit **130**. The ECG signal generating unit **130** may be operable to generate an ECG signal. In generating the ECG signal, any electrocardiographic device, which is well known to a person skilled in the art, may be used. Thus, detailed descriptions thereof will be omitted herein.

[0016] The ultrasound system **100** may further include an ultrasound image forming unit **140**. The ultrasound image forming unit **140** may be operable to form an ultrasound image based on the receive signals, which are provided from the Tx/Rx unit **110**. In one embodiment, the ultrasound system **100** may be operable to form a B-mode image **210** based on the first receive signals and a Doppler-mode image **220** based on the second receive signals, as shown in FIG. 2.

[0017] The ultrasound system **100** may further include an additional information forming unit **150**. The additional information forming unit **150** may be operable to form additional information such as physiologic information based on the PPG signal and the ECG signal. In one embodiment, the physiologic information may include blood oxygen saturation, heart rate and blood pressure. Referring to FIG. 2, the additional information forming unit **150** may be operable to form a PPG waveform **230** based on the PPG signal. Also, the additional information forming unit **150** may be operable to form an ECG waveform **240** based on the ECG signal. The additional information forming unit **150** may be further operable to form the physiologic information **250** including information on the blood oxygen saturation (SpO₂), heart rate (HR) and blood pressure (BP) based on the PPG waveform **230** and the ECG form **240**. The HR information may be obtained by using the characteristic of the PPG waveform that it is synchronized with a heart beat.

[0018] Referring to FIG. 3, the additional information forming unit **150** may be operable to detect peak points and valley points on the PPG waveform **230**, as well as peak points on the ECG waveform **240**. The additional information forming unit **150** may be further operable to compute an interval between the peak point of the PPG waveform **230** and the peak point of the ECG waveform **240** (hereinafter, referred to as first pulse transit time PPT_p). The additional information forming unit **150** may be further operable to compute an interval between the valley point of the PPG waveform **230** and the peak point of the ECG waveform **240** (hereinafter, referred to as second pulse transit time PPT_v). In one embodiment, the additional information forming unit **150** may be operable to form the BP information by using the characteristic of the blood pressure that is inverse proportional to the computed first and second pulse transit times PPT_p and PPT_v. That is, if the blood pressure increases, then the distensibility of the blood wall decreases so that the first and second pulse transit times PPT_p and PPT_v may be reduced. On the other hand, if the blood pressure decreases, then the distensibility of the blood wall increases so that the first and second pulse transit times PPT_p and PPT_v may increase.

[0019] In one embodiment, the additional information forming unit **150** may include a PPG waveform forming section (not shown), an ECG waveform forming section (not shown) and a physiologic information forming section (not shown). The PPG waveform forming section may be operable to form the PPG waveform and the ECG waveform forming section may be operable to form the ECG waveform. The

physiologic information forming section may be operable to form the physiologic information based on the PPG waveform and the ECG waveform.

[0020] Referring back to FIG. 1, the ultrasound system **100** may further include a display unit **160**. The display unit **160** may be any display capable of displaying images such as an ultrasound image. The display unit **160** may be one of CRT, LCD, flat panel display and the like, although it is not limited thereto. The ultrasound images formed in the ultrasound image forming unit **140**, i.e., the B-mode image **210** and the Doppler-mode image **220**, may be displayed on a screen of the display unit **160**, as shown in FIG. 2. Also, the additional information formed in the additional information forming unit **150**, i.e., the PPG waveform **230**, ECG waveform **240** and physiologic information **250**, are displayed on the screen of the display unit **160**.

[0021] The ultrasound system **100** may further include a control unit **170** that may be operable to control the transmission and the reception of the ultrasound signals. The control unit **170** may be further operable to control the formation and display of the ultrasound images. Also, the control unit **170** may be operable to control the generation of the PPG and ECG signals and the formation of the additional information. In one embodiment, the control unit **170** may be operable to control the display unit **160** such that the additional information such as the blood oxygen saturation, heart rate and blood pressure are displayed together with the ultrasound image on the screen of the display unit **160**. Thus, the examination upon the heart using the ultrasound system may be more accurately performed.

[0022] Although embodiments have been described with reference to a number of illustrative embodiments thereof, it should be understood that numerous other modifications and embodiments can be devised by those skilled in the art that will fall within the spirit and scope of the principles of this disclosure. More particularly, numerous variations and modifications are possible in the component parts and/or arrangements of the subject combination arrangement within the scope of the disclosure, the drawings and the appended claims. In addition to variations and modifications in the component parts and/or arrangements, alternative uses will also be apparent to those skilled in the art.

What is claimed is:

1. An ultrasound system, comprising:

a transmission/reception (Tx/Rx) unit operable to transmit ultrasound signals to a target object and receive echo signals reflected from the target object to thereby output receive signals;

an ultrasound image forming unit operable to form ultrasound images based on the receive signals;

a photoplethysmography (PPG) signal generating unit operable to generate a PPG signal for the target object;

an electrocardiogram (ECG) signal generating unit operable to generate an ECG signal for the target object;

an additional information forming unit operable to form additional information by using the PPG signal and the ECG signal; and

a display unit for displaying the ultrasound images and the additional information.

2. The ultrasound system of claim 1, wherein the additional information include a PPG waveform, an ECG waveform and physiologic information.

3. The ultrasound system of claim 2, wherein the physiologic information include blood oxygen saturation, heart rate and blood pressure.

4. The ultrasound system of claim 3, wherein the additional information forming unit includes:

- a PPG waveform forming section operable to form the PPG waveform by using the PPG signal;
- an ECG waveform forming section operable to form the ECG waveform by using the ECG signal; and
- a physiologic information forming section operable to form the physiologic information by using the PPG waveform and the ECG waveform.

5. The ultrasound system of claim 4, wherein the physiologic information forming section is configured to:

detect peak points and valley points on the PPG waveform and peak points on the ECG waveform;

compute a first pulse transit time representing an interval between the peak point of the PPG waveform and the peak point of the ECG waveform and a second pulse transit time representing an interval between the valley point of the PPG waveform and the peak point of the ECG waveform; and

form information on the blood pressure by using the first and second pulse transit times.

* * * * *

专利名称(译)	使用PPG和ECG信号的附加信息的超声图像显示		
公开(公告)号	US20100113905A1	公开(公告)日	2010-05-06
申请号	US12/609926	申请日	2009-10-30
申请(专利权)人(译)	MEDISON CO. , LTD.		
当前申请(专利权)人(译)	MEDISON CO. , LTD.		
[标]发明人	PARK JOONG HOON		
发明人	PARK, JOONG HOON		
IPC分类号	A61B5/1455 A61B8/14		
CPC分类号	A61B5/0205 A61B5/02416 A61B5/14551 A61B8/08 A61B8/463 G01S7/52073 G01S15/899		
优先权	1020080107476 2008-10-31 KR		
外部链接	Espacenet USPTO		

摘要(译)

公开了一种用于在超声系统中使用光电脉搏波描记术 (PPG) 信号和心电图 (ECG) 信号显示具有附加信息的超声图像的实施例。超声系统包括光电容积描记 (PPG) 信号产生单元和心电图 (ECG) 信号产生单元。PPF信号生成单元和ECG信号生成单元分别生成目标对象的PPG信号和目标对象的ECG信号。附加信息形成单元通过使用PPG信号和ECG信号形成附加信息。显示单元显示目标对象的超声图像以及附加信息。

