

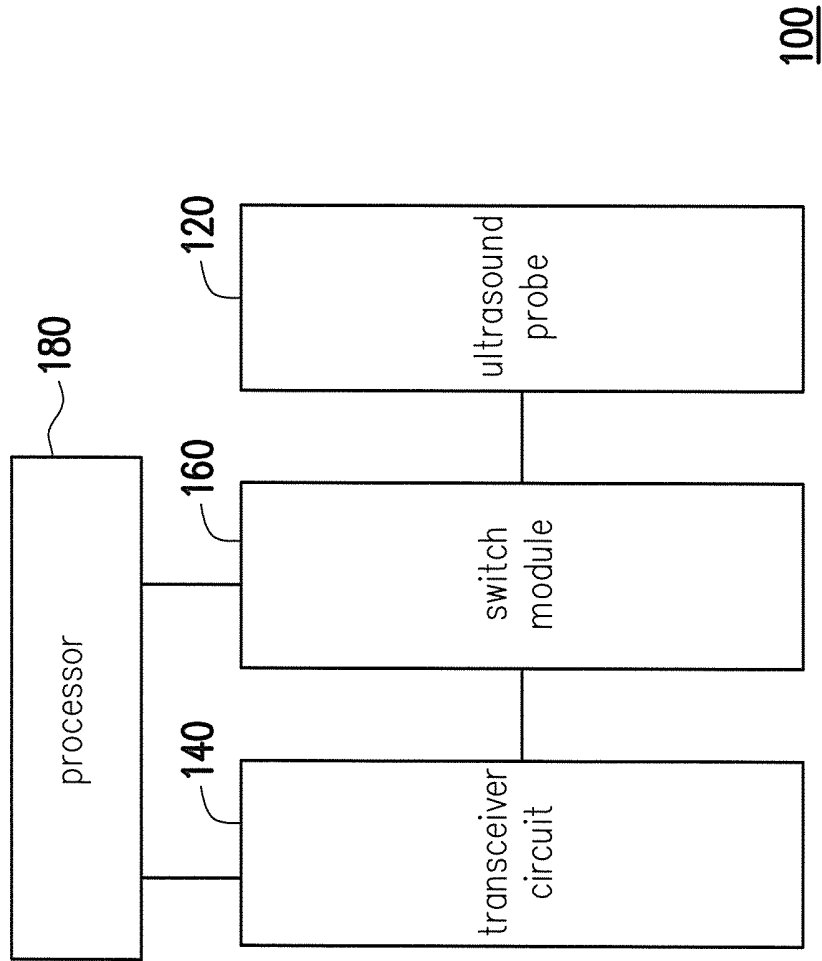


FIG. 1

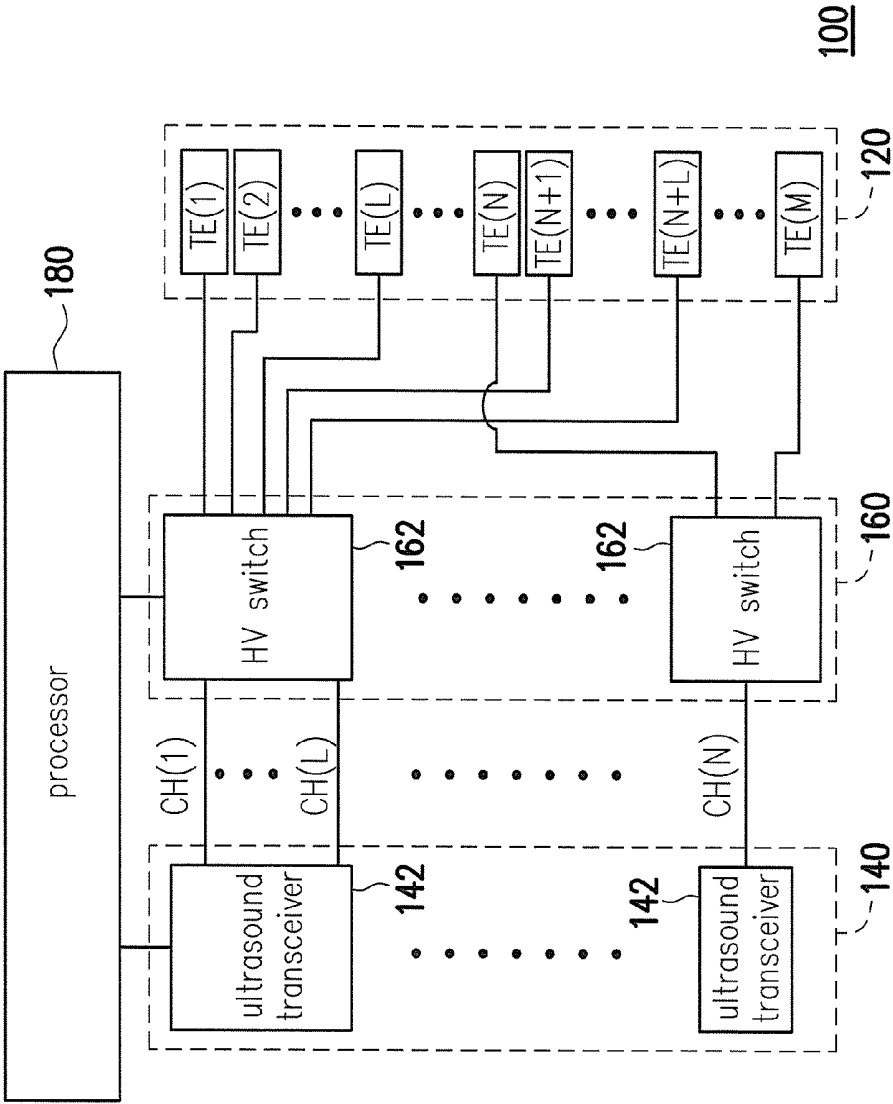


FIG. 2

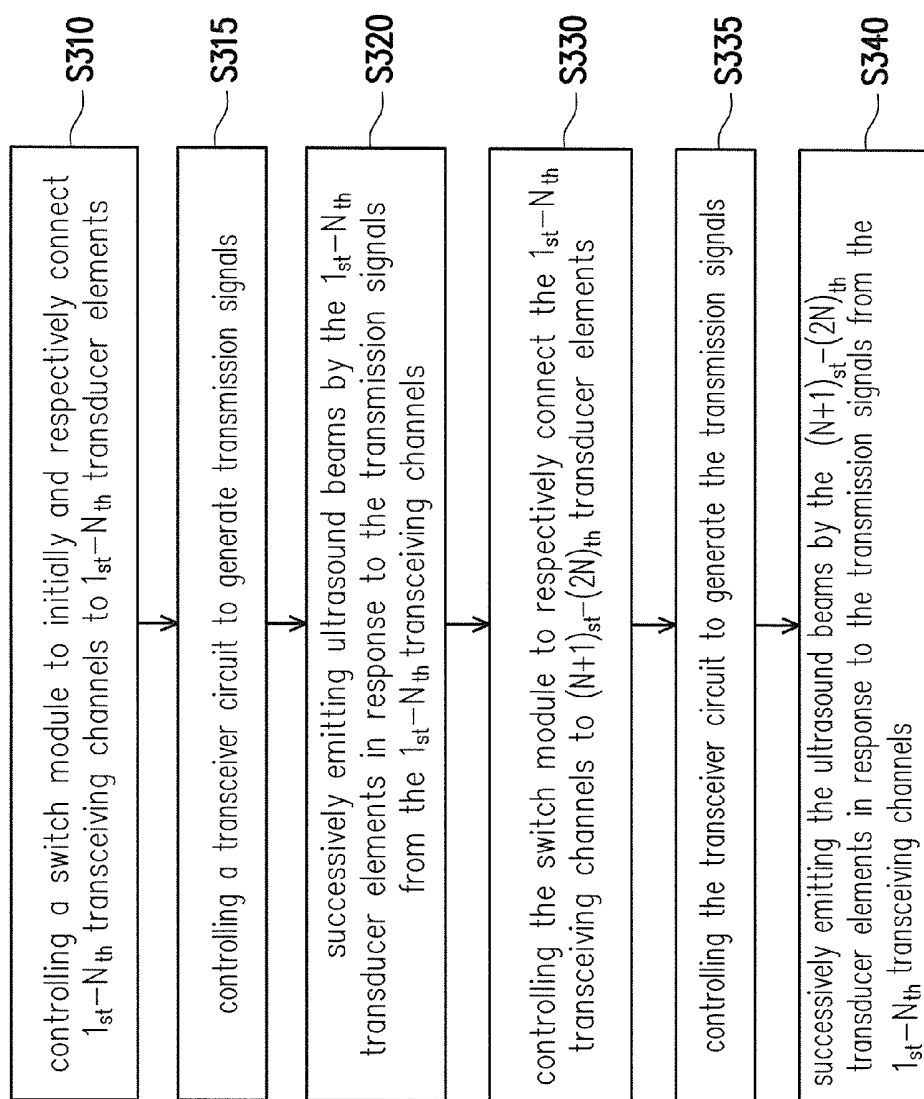


FIG. 3

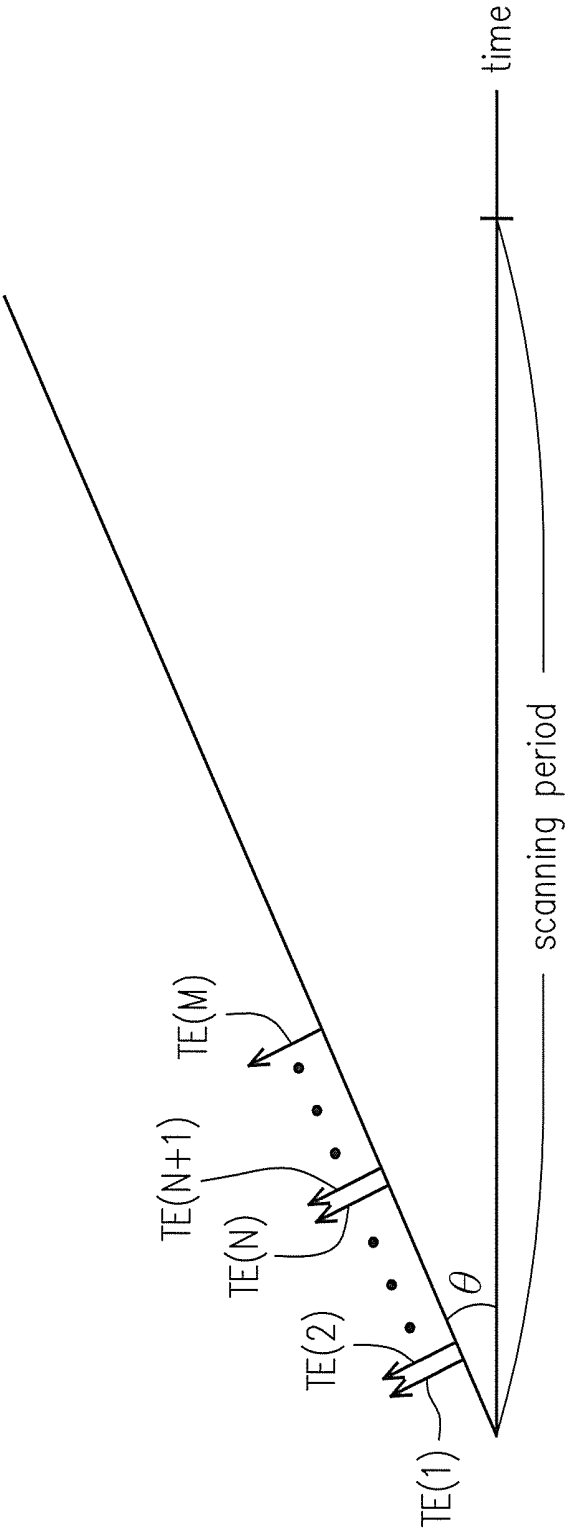


FIG. 4

ULTRASOUND APPARATUS AND ULTRASOUND EMISSION METHOD

BACKGROUND

Technical Field

[0001] The disclosure relates to an ultrasound apparatus and an ultrasound emission method adapted to the ultrasound apparatus.

Description of Related Art

[0002] Ultrasound has been widely used in medical diagnosis, military radar system and rusting detection. In the medical diagnosis system, the ultrasound is often used in imaging internal body structures such as tendons, muscles, joints, vessels and internal organs. Images obtained by the ultrasound may clearly show the internal body, which help medical personnel to correctly diagnose illness or disease of a patient. Thereafter, appropriate treatment could be chosen and performed to the patient.

[0003] In a traditional medical ultrasound apparatus, during the ultrasound scanning of an object, ultrasound beams are outputted by a plurality of transducer elements in a probe to form a plane wave, and echoes of the plane wave are detected and recorded for generating the image of the internal structure of the object. However, when using the probe for ultrasound scanning, the wave strength at the beginning and the end of the ultrasound plane wave is usually weaker than the wave strength at the other parts of the ultrasound plane wave. This usually leads to inaccurate ultrasound detection.

[0004] Therefore, compensation should be made in order to put the wave strength of the plane wave in consistency. It is still a goal of effort for those technicians of the field to provide an efficient and accurate ultrasound detection.

SUMMARY

[0005] The disclosure is directed to an ultrasound apparatus and an ultrasound emission method, by which ultrasound detection is precisely and accurately performed.

[0006] An embodiment of the disclosure provides an ultrasound apparatus. The ultrasound apparatus includes an ultrasound probe, a transceiver circuit, a switch module and a processor. The ultrasound probe has a 1_{st} transducer element to a M_{th} transducer element for respectively emitting ultrasound beams to form a plane wave, where M is a positive integer. The transceiver circuit has a 1_{st} transceiving channel to a N_{th} transceiving channel, where N is a positive integer, and M is a multiple of N . The switch module is switched between the ultrasound probe and the transceiver circuit, and the processor controls the switch module and the transceiver circuit. During a scanning period, the processor controls the switch module to initially and respectively connect the 1_{st} - N_{th} transceiving channels to the 1_{st} - N_{th} transducer elements and controls the transceiver circuit to generate transmission signals, such that the 1_{st} - N_{th} transducer elements successively emit the ultrasound beams in response to the transmission signals from the 1_{st} - N_{th} transceiving channels. After the ultrasound beam is emitted by the N_{th} transducer element, the processor controls the switch module to respectively connect the 1_{st} - N_{th} transceiving channels to the $(N+1)_{th}$ - $(2N)_{th}$ transducer elements and controls the transceiver circuit to generate the transmission signals, such that the

$(N+1)_{th}$ - $(2N)_{th}$ transducer elements successively emit the ultrasound beams in response to the transmission signals from the 1_{st} - N_{th} transceiving channels.

[0007] In an embodiment of the disclosure, every two of the ultrasound beams that are successively emitted are separated in time by an interval.

[0008] In an embodiment of the disclosure, operation of the switch module as to respectively connect the 1_{st} - N_{th} transceiving channels to the $(N+1)_{th}$ - $(2N)_{th}$ transducer elements is performed during the interval.

[0009] In an embodiment of the disclosure, when every two adjacent transducer elements are apart with a distance 1 , for emitting the plane wave with an incident angle θ , the interval is: $\text{interval} = 1 \times \sin \theta / V$, wherein V is a velocity of ultrasound.

[0010] In an embodiment of the disclosure, when M equals to $2N$, after the ultrasound beam is emitted by the $(2N)_{th}$ transducer element, the processor controls the switch module to respectively connect the 1_{st} - N_{th} transceiving channels to the 1_{st} - N_{th} transducer elements for detecting echoes of the ultrasound beams in rest of the scanning period. When the echoes of the ultrasound beams are detected, reception signals are generated by the 1_{st} - N_{th} transducer elements and transmitted to the 1_{st} - N_{th} transceiving channels. The reception signals are further transferred to Low-Voltage Differential Signaling (LVDS) signals by the transceiver circuit, and the LVDS signals are then sent to the processor.

[0011] In an embodiment of the disclosure, the switch module comprises at least one high voltage switch, and each of the at least one high voltage switch is switched between a portion of the transducer elements and a portion of the transceiving channels.

[0012] Another embodiment of the disclosure provides an ultrasound emission method, adapted to an ultrasound apparatus for emitting a plane wave during a scanning period. The ultrasound apparatus has an ultrasound probe, a transceiver circuit and a switch module switched between the ultrasound probe and the transceiver circuit. The ultrasound probe has a 1_{st} transducer element to a M_{th} transducer element for respectively emitting ultrasound beams to form the plane wave, the transceiver circuit has a 1_{st} transceiving channel to a N_{th} transceiving channel, M , N are positive integers, and M is a multiple of N . The method includes the following steps. The switch module is controlled to initially and respectively connect the 1_{st} - N_{th} transceiving channels to the 1_{st} - N_{th} transducer elements. The transceiver circuit is controlled to generate transmission signals. The ultrasound beams are successively emitted by the 1_{st} - N_{th} transducer elements in response to the transmission signals from the 1_{st} - N_{th} transceiving channels. After the ultrasound beam is emitted by the N_{th} transducer element, the switch module is controlled to respectively connect the 1_{st} - N_{th} transceiving channels to the $(N+1)_{th}$ - $(2N)_{th}$ transducer elements. The transceiver circuit is controlled to generate transmission signals. The ultrasound beams are successively emitted by the $(N+1)_{th}$ - $(2N)_{th}$ transducer elements in response to the transmission signals from the 1_{st} - N_{th} transceiving channels.

[0013] According to the above description, in the ultrasound apparatus and the ultrasound emission method, through the operation of the switch module, the total number of the emitted ultrasound beams during a single scanning period is at least twice of the number of the transceiving channels. Thus, energy of the emission is increased, so the

Signal-to-Noise Ratio (SNR) has been raised, such that the ultrasound detection is more precise and accurate, and the quality of the ultrasound image is also improved. Further, the total cycle time for a succeed scanning could be shortened, so as to lower the power consumption on ultrasound detection.

[0014] In order to make the aforementioned and other features and advantages of the disclosure comprehensible, several exemplary embodiments accompanied with figures are described in detail below.

BRIEF DESCRIPTION OF THE DRAWINGS

[0015] The accompanying drawings are included to provide a further understanding of the disclosure, and are incorporated in and constitute a part of this specification. The drawings illustrate embodiments of the disclosure and, together with the description, serve to explain the principles of the disclosure.

[0016] FIG. 1 is a block diagram illustrating an ultrasound apparatus according to an embodiment of the present disclosure.

[0017] FIG. 2 is a detailed diagram illustrating an ultrasound apparatus according to an embodiment of the present disclosure.

[0018] FIG. 3 is a flowchart illustrating an ultrasound emission method according to an embodiment of the present disclosure.

[0019] FIG. 4 is a schematic diagram of emitting a plane wave according to an embodiment of the present disclosure.

DESCRIPTION OF EMBODIMENTS

[0020] Reference will now be made in detail to the present preferred embodiments of the disclosure, examples of which are illustrated in the accompanying drawings. Wherever possible, the same reference numbers are used in the drawings and the description to refer to the same or like parts.

[0021] FIG. 1 is a block diagram illustrating an ultrasound apparatus according to an embodiment of the present disclosure. Referring to FIG. 1, in the present embodiment of the present disclosure, the ultrasound apparatus 100 includes an ultrasound probe 120, a transceiver circuit 140, a switch module 160 and a processor 180. The switch module 160 is switched between the ultrasound probe 120 and the transceiver circuit 140. The processor 180 is connected to the switch module 160 and the transceiver circuit 140, and thereby controls the switch module 160 and the transceiver circuit 140 for the ultrasound emission and detection. In an embodiment of the disclosure, the ultrasound apparatus 100 may be implemented in an electronic apparatus with computation ability, such as a personal computer, a laptop computer, a tabular computer, a server and a smart device, but it is not limited herein.

[0022] In an embodiment of the present disclosure, the ultrasound probe 120 includes a plurality of transducer elements, which emits ultrasound waves and receives echoes of the ultrasound waves. FIG. 2 is a detailed diagram illustrating an ultrasound apparatus according to an embodiment of the present disclosure. Referring to FIG. 1 and FIG. 2, in the present embodiment, a 1_{st} transducer elements to a M_{th} transducer elements TE(1)-TE(M) of the ultrasound probe 120 are arranged in a line, where M is a positive number, but the arrangement of the transducer elements TE(1)-TE(M) is not limited herein.

[0023] In the present embodiment, every two adjacent transducer elements, such as the transducer element TE(1) and the transducer element TE(2), are apart with a distance 1. The distance 1 is determined in accordance with the design of the ultrasound probe 120, and it could be several millimeters (mm) or less, though it is not limited herein. By respectively applying voltages (also called transmission signals) to the transducer elements TE(1)-TE(M), each of the transducer elements TE(1)-TE(M) is driven to output ultrasound beam, and those ultrasound beams are combined to form a plane wave traveling along a preferred direction.

[0024] After the emission of the ultrasound waves, the 1_{st} transducer elements to the M_{th} transducer elements TE(1)-TE(M) of the ultrasound probe 120 are further configured to listen for echoes that are produced when the emitted ultrasound waves are reflected by objects. Reception signals are generated by the transducer elements TE(1)-TE(M) when detecting and receiving the echoes.

[0025] Referring to FIG. 1 and FIG. 2, in an embodiment of the present disclosure, the transceiver circuit 140 includes a plurality of ultrasound transceivers 142 and a 1_{st} transceiving channel to a N_{th} transceiving channel CH(1)-CH(N), where N is a positive integer, and M is a multiple of N. Each of the ultrasound transceivers 142 may provide several transceiving channels. In the present embodiment shown in FIG. 2, the ultrasound transceivers 142 are octal ultrasound transceivers which respectively provides 8 transceiving channels CH(1)-CH(8), . . . , CH(N-8)-CH(N). However, the embodiment is not intended to limit the number of the transceiving channels for each of the ultrasound transceivers 142. In other embodiments, the each of the ultrasound transceivers 142 may provide various number of the transceiving channels.

[0026] In the present embodiment, the 1_{st} transceiving channel to the N_{th} transceiving channel CH(1)-CH(N) are responsible for generating and transmitting transmission signals to the ultrasound probe 120 under the control of the processor 180. The transmission signals are the voltage pulses that applied to the transducer elements TE(1)-TE(M) of the probe 120. Further, when receiving reception signals from the ultrasound probe 120 in response to the echoes of the ultrasound, the 1_{st} transceiving channel to the N_{th} transceiving channel CH(1)-CH(N) correspondingly transforms the reception signals to Low-Voltage Differential Signaling (LVDS) signals, and then send the LVDS signals to the processor 180.

[0027] Referring to FIG. 1 and FIG. 2, in an embodiment of the present disclosure, the switch module 160 includes at least one high voltage (HV) switch 162. In the embodiment, the high voltage switch 162 may be a multiplexer, however, the embodiment is not intended to limit the implement of the high voltage switch 162. Each high voltage switch 162 switches the connections between a portion of the transducer elements TE(1)-TE(M) and a portion of the transceiving channels CH(1)-CH(N). For example, the high voltage switch 162 switches the connection between the transducer elements TE(1)-TE(L), TE(N+1)-TE(N+L) and the transceiving channels CH(1)-CH(L), where L is a positive integer less than N.

[0028] Referring to FIG. 1 and FIG. 2, the processor 180 is a central processing unit (CPU), a programmable micro-processor, a digital signal processor (DSP), a programmable controller, an application specific integrated circuit (ASIC),

a Field-programmable gate array (FPGA) or a programmable logic device (PLD), for example, but not limited thereto.

[0029] In an embodiment of the disclosure, the ultrasound apparatus 100, for example, further includes a storage unit (not shown) and an input/output (I/O) interface (not shown). The storage unit is, for example, a hard disk, a random access memory (RAM) or a similar device having a storage function for storing various messages, programs and data. The I/O interface of the ultrasound apparatus 100 is, for example, a universal serial bus (USB) port, a wireless communication device or a similar device having a communication function for communicating with other apparatuses and devices.

[0030] FIG. 3 is a flowchart illustrating an ultrasound emission method according to an embodiment of the present disclosure. In the present embodiment, the ultrasound emission method is, for example, adapted to the ultrasound apparatus 100 shown in FIG. 1 and FIG. 2. Referring to FIG. 1, FIG. 2, and FIG. 3, during a scanning period, the switch module 160 is controlled by the processor 180 to initially and respectively connect the 1_{st} - N_{th} transceiving channels CH(1)-CH(N) to the 1_{st} - N_{th} transducer elements TE(1)-TE(N) (step S310). After the 1_{st} - N_{th} transceiving channels CH(1)-CH(N) are connected to the 1_{st} - N_{th} transducer elements TE(1)-TE(N), the processor 180 controls the transceiver circuit 140 to generate transmission signals (step S315) by transmitting control signals to the transceiver circuit 140. The transmission signals are further sent to the ultrasound probe 120 from the 1_{st} - N_{th} transceiving channels CH(1)-CH(N) of the transceiver circuit 140 through the switch module 160.

[0031] In response to the transmission signals from the 1_{st} - N_{th} transceiving channels CH(1)-CH(N), the ultrasound beams are successively emitted by the 1_{st} - N_{th} transducer elements TE(1)-TE(N) (step S320). It should be noted that, in an embodiment of the present disclosure, a time delay is adopted in successively emitting the ultrasound beams. In other words, every two of the ultrasound beams that are successively emitted, such as the ultrasound beams emitted by the 1_{st} transducer element TE(1) and the 2_{nd} transducer element TE(2), are separated in time by an interval.

[0032] FIG. 4 is a schematic diagram of emitting a plane wave according to an embodiment of the present disclosure. Referring to FIG. 4, when every two adjacent transducer elements, such as the 1_{st} transducer element TE(1) and the 2_{nd} transducer element TE(2), are apart with a distance 1, for emitting the plane wave with an incident angle θ , the interval mentioned above is shown as below.

$$\text{interval} = 1 \times \sin \theta / V \quad (1)$$

[0033] It should be noted that, V is a velocity of ultrasound which is approximately 1540 meters per second (m/s). Thus, for example, the ultrasound beam emitted by the 2_{nd} transducer element TE(2) is subsequent to the ultrasound beam emitted by the 1_{st} transducer element TE(1) for one interval mentioned above in time.

[0034] Referring to FIG. 1 to FIG. 4, after the ultrasound beam is emitted by the N_{th} transducer element, during the scanning period, the switch module 160 is controlled by the processor 180 to respectively connect the 1_{st} - N_{th} transceiving channels CH(1)-CH(N) to the $(N+1)_{th}$ -($2N$) $_{th}$ transducer elements TE(N+1)-TE(2N) (step S330). Then, the processor 180 controls the transceiver circuit 140 to generate the

transmission signals (step S335) by transmitting the control signals to the transceiver circuit 140. The transmission signals are further sent to the ultrasound probe 120 from the 1_{st} - N_{th} transceiving channels CH(1)-CH(N) of the transceiver circuit 140 through the switch module 160, such that the ultrasound beams are successively emitted by the $(N+1)_{th}$ -($2N$) $_{th}$ transducer elements TE(N+1)-TE(2N) (step S340) in response to the transmission signals from the 1_{st} - N_{th} transceiving channels CH(1)-CH(N).

[0035] In an embodiment of the present disclosure, since the ultrasound beams that are successively emitted by the N_{th} transducer element TE(N) and the $(N+1)_{th}$ transducer element TE(N+1) are also separated in time by the interval mentioned above, operation of the switch module 160 for respectively connecting the 1_{st} - N_{th} transceiving channels CH(1)-CH(N) to the $(N+1)_{th}$ -($2N$) $_{th}$ transducer elements TE(N+1)-TE(2N) should be performed during the interval. In other words, the operation of the switch module 160 for respectively connecting the 1_{st} - N_{th} transceiving channels CH(1)-CH(N) to the $(N+1)_{th}$ -($2N$) $_{th}$ transducer elements TE(N+1)-TE(2N) should be completed before the emission of the ultrasound beam performed by the $(N+1)_{th}$ transducer element TE(N+1).

[0036] Through the ultrasound emission method illustrated above, during one single scanning period, the total number of the emitted ultrasound beams is at least twice of the number of the transceiving channels CH(1)-CH(N). Thus, energy of the emission is increased, and the SNR of the ultrasound plane wave has been raised.

[0037] In an embodiment of the present disclosure, when M equals to $2N$ as shown in FIG. 2, after the ultrasound beam is emitted by the $(2N)_{th}$ transducer element TE(2N), the processor 180 controls the switch module 160 to respectively connect the 1_{st} - N_{th} transceiving channels CH(1)-CH(N) to the 1_{st} - N_{th} transducer elements TE(1)-TE(N) for detecting echoes of the ultrasound beams in rest of the scanning period. When the echoes of the ultrasound beams are detected, the reception signals are generated by the 1_{st} - N_{th} transducer elements TE(1)-TE(N) and transmitted to the 1_{st} - N_{th} transceiving channels CH(1)-CH(N). The reception signals are further transferred to LVDS signals by the transceiver circuit 140, and the LVDS signals are then sent to the processor 180.

[0038] However, in another embodiment of the present disclosure, when M equals to $3N$, the processor 180 controls switch module 160 to connect the 1_{st} - N_{th} transceiving channels CH(1)-CH(N) to the 1_{st} - N_{th} transducer elements, the $(N+1)_{st}$ -($2N$) $_{th}$ transducer elements, and the $(2N+1)_{st}$ -($3N$) $_{th}$ transducer elements in serial. After the ultrasound beam is emitted by the $(3N)_{th}$ transducer element, the processor 180 controls the switch module 160 to respectively connect the 1_{st} - N_{th} transceiving channels CH(1)-CH(N) to the 1_{st} - N_{th} transducer elements TE(1)-TE(N) for detecting echoes of the ultrasound beams in rest of the scanning period.

[0039] In the present disclosure, the numbers and the relationship of M and N may be varied. However, from the above description, the corresponding operation of the ultrasound apparatus 100 and the ultrasound emission method could still be deduced even when M and N are changed, so those are not illustrated herein.

[0040] A design of the ultrasound apparatus 100 in an embodiment of the present disclosure is provided below. In this embodiment, M is 128, N is 64, so the number of the transducer elements is twice of the number of the transceiv-

ing channels. Further, if the number of the high voltage switch 162 is 4, then L is 16. One single scanning period may be 200 microseconds (μ s), and ultrasound emission performed by all the transducer elements TE(1)-TE(M) may only cost a few microseconds (μ s). However, it should be noted that, the design of the ultrasound apparatus 100 may be varied in corresponding to the practical requirement on the ultrasound detection.

[0041] In summary, in the ultrasound apparatus and the ultrasound emission method, through the operation of the switch module, the total number of the emitted ultrasound beams during a single scanning period is at least twice of the number of the transceiving channels. Thus, energy of the emission is increased, so the Signal-to-Noise Ratio (SNR) has been raised, such that the ultrasound detection is more precise and accurate, and the quality of the ultrasound image is also improved. Further, the total cycle time for a succeed scanning could be shortened, so as to lower the power consumption on ultrasound detection.

[0042] It will be apparent to those skilled in the art that various modifications and variations can be made to the structure of the disclosure without departing from the scope or spirit of the disclosure. In view of the foregoing, it is intended that the disclosure cover modifications and variations of this invention provided they fall within the scope of the following claims and their equivalents.

What is claimed is:

1. An ultrasound apparatus, comprising:

an ultrasound probe, having a 1_{st} transducer element to a M_{th} transducer element for respectively emitting ultrasound beams to form a plane wave, where M is a positive integer;

a transceiver circuit, having a 1_{st} transceiving channel to a N_{th} transceiving channel, where N is a positive integer, and M is a multiple of N;

a switch module, switched between the ultrasound probe and the transceiver circuit; and

a processor, controlling the switch module and the transceiver circuit, wherein during a scanning period, the processor controls the switch module to initially and respectively connect the 1_{st} - N_{th} transceiving channels to the 1_{st} - N_{th} transducer elements and controls the transceiver circuit to generate transmission signals, such that the 1_{st} - N_{th} transducer elements successively emit the ultrasound beams through the 1_{st} - N_{th} transceiving channels in response to the transmission signals, and after the ultrasound beam is emitted by the N_{th} transducer element, the processor controls the switch module to respectively connect the 1_{st} - N_{th} transceiving channels to the $(N+1)_{th}$ -($2N$) $_{th}$ transducer elements and controls the transceiver circuit to generate the transmission signals, such that the $(N+1)_{th}$ -($2N$) $_{th}$ transducer elements successively emit the ultrasound beams in response to the transmission signals from the 1_{st} - N_{th} transceiving channels.

2. The ultrasound apparatus according to claim 1, wherein every two of the ultrasound beams that are successively emitted are separated in time by an interval.

3. The ultrasound apparatus according to claim 2, wherein operation of the switch module as to respectively connect the 1_{st} - N_{th} transceiving channels to the $(N+1)_{th}$ -($2N$) $_{th}$ transducer elements is performed during the interval.

4. The ultrasound apparatus according to claim 2, wherein when every two adjacent transducer elements are apart with a distance 1, for emitting the plane wave with an incident angle θ , the interval is:

$$\text{interval} = 1 \times \sin \theta / V,$$

wherein V is a velocity of ultrasound.

5. The ultrasound apparatus according to claim 1, wherein when M equals to $2N$, after the ultrasound beam is emitted by the $(2N)_{th}$ transducer element, the processor controls the switch module to respectively connect the 1_{st} - N_{th} transceiving channels to the 1_{st} - N_{th} transducer elements for detecting echoes of the ultrasound beams in rest of the scanning period,

when the echoes of the ultrasound beams are detected, reception signals are generated by the 1_{st} - N_{th} transducer elements and transmitted to the 1_{st} - N_{th} transceiving channels, the reception signals are further transferred to Low-Voltage Differential Signaling (LVDS) signals by the transceiver circuit, and the LVDS signals are then sent to the processor.

6. The ultrasound apparatus according to claim 1, wherein the switch module comprises at least one high voltage switch, and each of the at least one high voltage switch is switched between a portion of the transducer elements and a portion of the transceiving channels.

7. An ultrasound emission method, adapted to an ultrasound apparatus for emitting a plane wave during a scanning period, the ultrasound apparatus has an ultrasound probe, a transceiver circuit and a switch module switched between the ultrasound probe and the transceiver circuit, the ultrasound probe has a 1_{st} transducer element to a M_{th} transducer element for respectively emitting ultrasound beams to form the plane wave, the transceiver circuit has a 1_{st} transceiving channel to a N_{th} transceiving channel, M, N are positive integers, and M is a multiple of N, the method comprising:

controlling the switch module to initially and respectively connect the 1_{st} - N_{th} transceiving channels to the 1_{st} - N_{th} transducer elements;

controlling the transceiver circuit to generate transmission signals;

successively emitting the ultrasound beams by the 1_{st} - N_{th} transducer elements through the 1_{st} - N_{th} transceiving channels in response to the transmission signals;

after the ultrasound beam is emitted by the N_{th} transducer element,

controlling the switch module to respectively connect the 1_{st} - N_{th} transceiving channels to the $(N+1)_{th}$ -($2N$) $_{th}$ transducer elements;

controlling the transceiver circuit to generate the transmission signals; and

successively emitting the ultrasound beams by the $(N+1)_{th}$ -($2N$) $_{th}$ transducer elements in response to the transmission signals from the 1_{st} - N_{th} transceiving channels.

8. The method according to claim 7, wherein every two of the ultrasound beams that are successively emitted are separated in time by an interval.

9. The method according to claim 8, wherein step of controlling the switch module to respectively connect the 1_{st} - N_{th} transceiving channels to the $(N+1)_{th}$ -($2N$) $_{th}$ transducer elements is performed during the interval.

10. The method according to claim 8, wherein when every two adjacent transducer elements are apart with a distance 1, for emitting the plane wave with an incident angle θ , the interval is:

$$\text{interval} = 1 \times \sin \theta / V,$$

wherein V is a velocity of ultrasound.

11. The method according to claim 7, further comprising: when M equals to 2N, after the ultrasound beam is emitted by the $(2N)_{th}$ transducer element, controlling the switch module to respectively connect the 1_{st} - N_{th} transceiving channels to the 1_{st} - N_{th} transducer elements; and detecting echoes of the ultrasound beams in rest of the scanning period.

* * * * *

专利名称(译)	超声设备和超声发射方法		
公开(公告)号	US20180125454A1	公开(公告)日	2018-05-10
申请号	US15/347798	申请日	2016-11-10
[标]发明人	LIU YING YI PENG SHENG CHANG LIU KUO PING		
发明人	LIU, YING-YI PENG, SHENG-CHANG LIU, KUO-PING		
IPC分类号	A61B8/00 A61B8/14		
CPC分类号	A61B8/4488 A61B8/54 A61B8/4494 A61B8/145 A61B8/5207 G01S7/5202 G01S15/89 G01S15/8915		
外部链接	Espacenet USPTO		

摘要(译)

提供了一种超声设备和发射平面波的方法。超声设备包括超声探头，收发器电路，开关模块和处理器。超声探头具有1 st 至M th 换能器元件，用于分别发射超声波束以形成平面波，并且收发器电路具有1 st 到N th 收发信道。M，N是正整数，M是N的倍数。在扫描期间，处理器控制开关模块最初并分别连接1 st -N th 将信道收发到1 st -N th 换能器元件，使得1 st -N th 换能器元件连续发射超声波束。在N th 换能器元件发射超声波束之后，处理器控制开关模块分别连接1 st -N th 收发通道到 (N + 1) th - (2N) th 换能器元件，使得 (N + 1) th - (2N) th 换能器元件连续发射超声波束。

