




US 20040193051A1

(19) **United States**(12) **Patent Application Publication****Mandrusov et al.**(10) **Pub. No.: US 2004/0193051 A1**(43) **Pub. Date: Sep. 30, 2004**(54) **ULTRASOUND ENERGY DRIVEN
INTRAVENTRICULAR CATHETER TO
TREAT ISCHEMIA****Related U.S. Application Data**(63) Continuation of application No. 09/774,334, filed on
Jan. 30, 2001, now Pat. No. 6,740,040.(76) Inventors: **Evgenia Mandrusov**, Campbell, CA
(US); **Jeffrey Steward**, Lakewood, CO
(US); **Marshall Sherman**,
Cardiff-by-the-Sea, CA (US)**Publication Classification**(51) **Int. Cl.⁷** **A61B 8/00**(52) **U.S. Cl.** **600/439**

Correspondence Address:

Cameron Kerrigan**SQUIRE, SANDERS & DEMPSEY L.L.P.****Suite 300****One Maritime Plaza****San Francisco, CA 94111-3492 (US)****ABSTRACT**

A method and apparatus for improving blood flow to an ischemic region (e.g., myocardial ischemia) a patient is provided. An ultrasonic transducer is positioned proximate to the ischemic region. Ultrasonic energy is applied at a frequency at or above 1 MHz to create one or more thermal lesions in the ischemic region of the myocardium. The thermal lesions can have a gradient of sizes. The ultrasound transducer can have a curved shape so that ultrasound energy emitted by the transducer converges to a site within the myocardium, to create a thermal lesion without injuring the epicardium or endocardium.

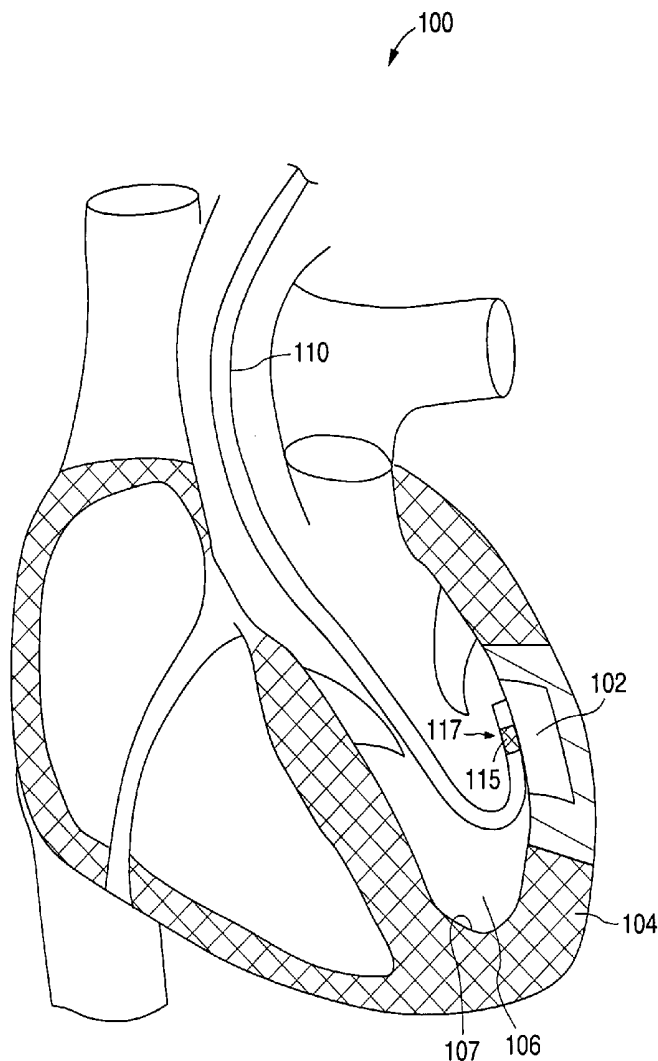(21) Appl. No.: **10/817,358**(22) Filed: **Apr. 1, 2004**

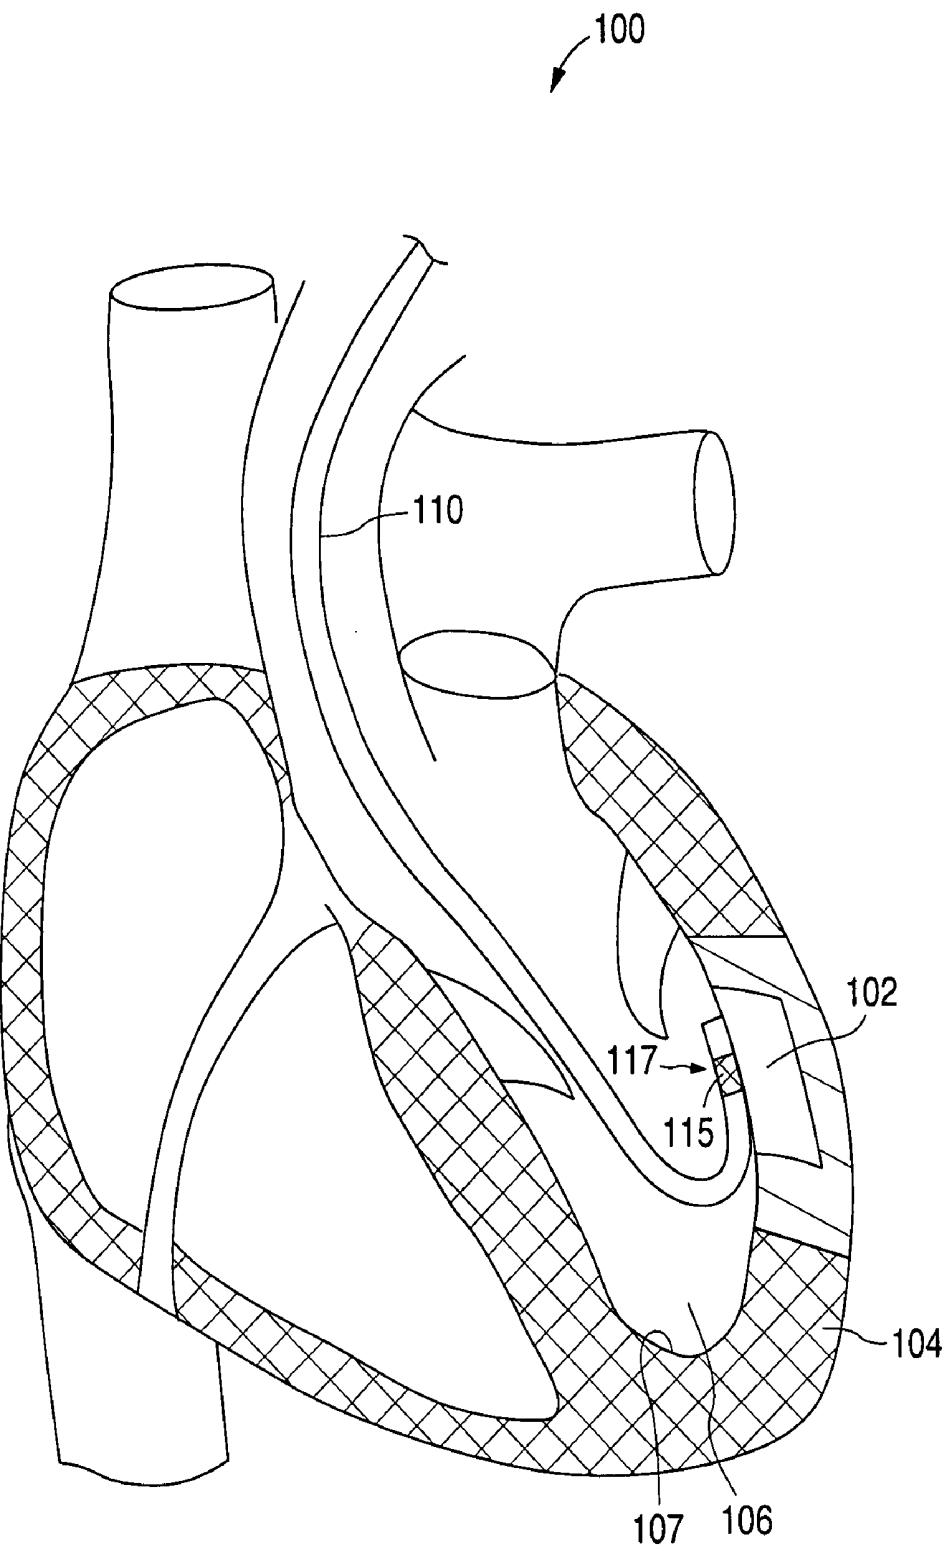


FIG. 1

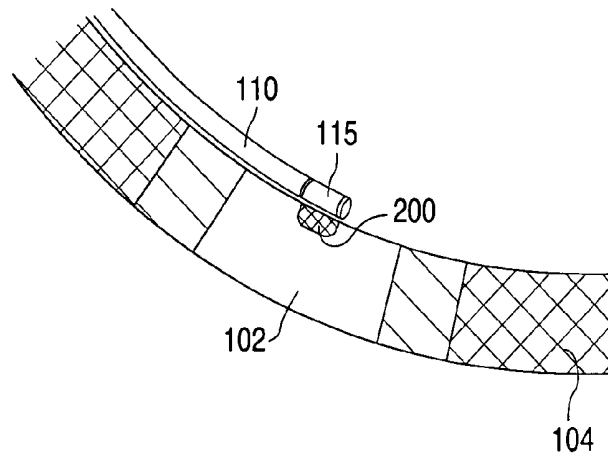


FIG. 2A

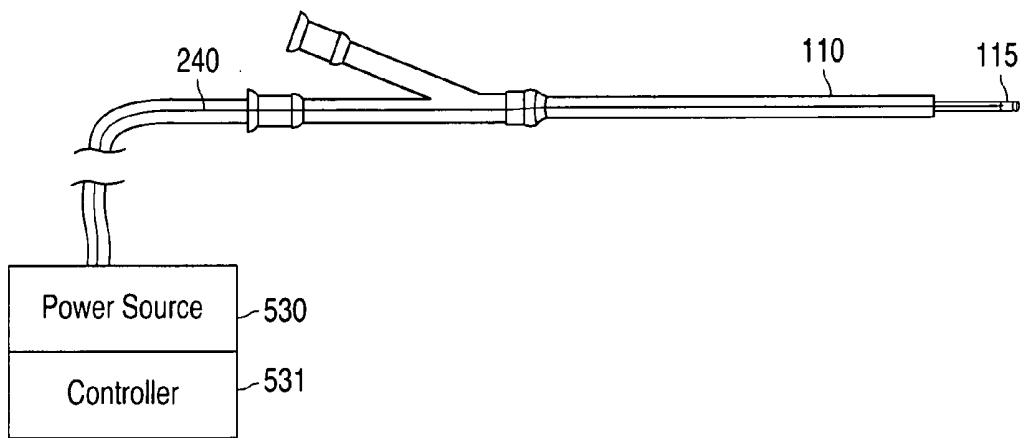


FIG. 2B

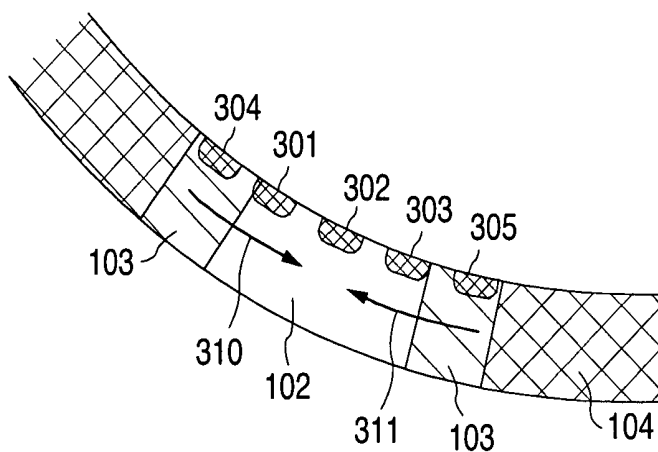


FIG. 3A

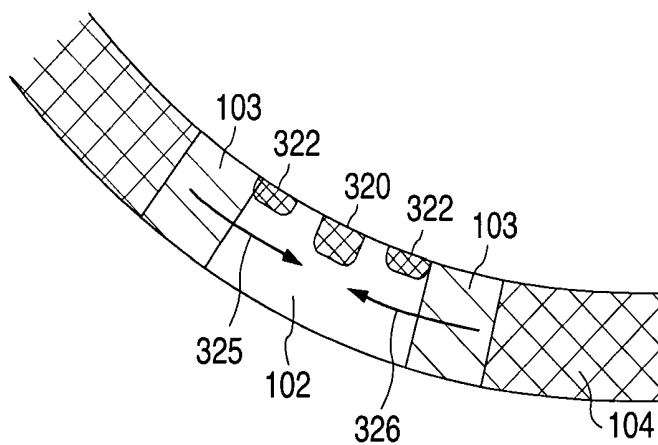


FIG. 3B

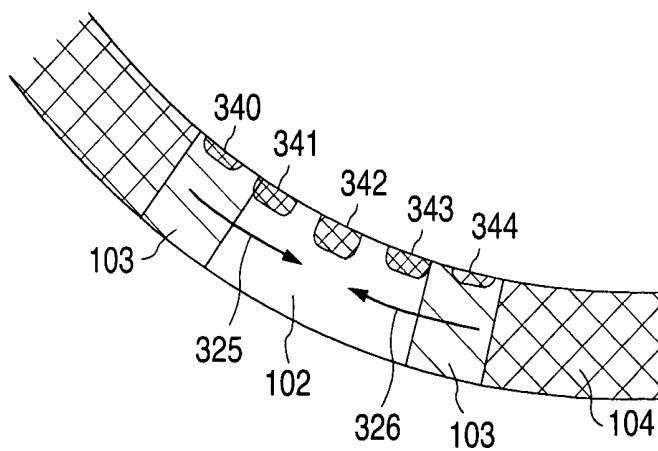


FIG. 3C

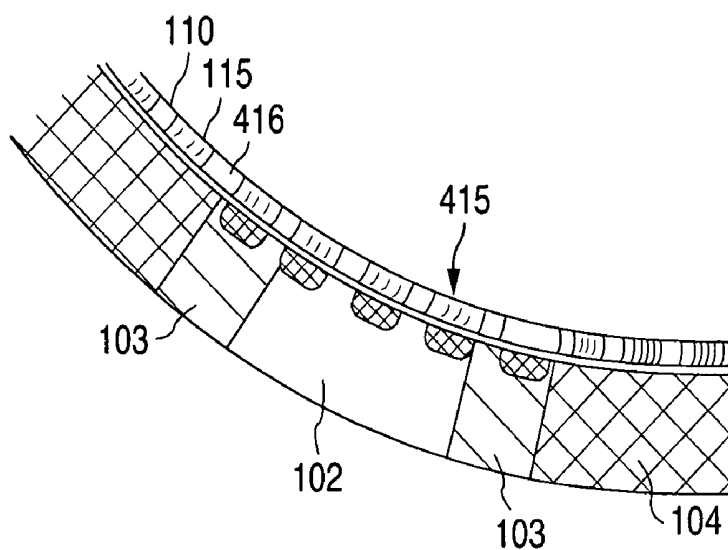


FIG. 4

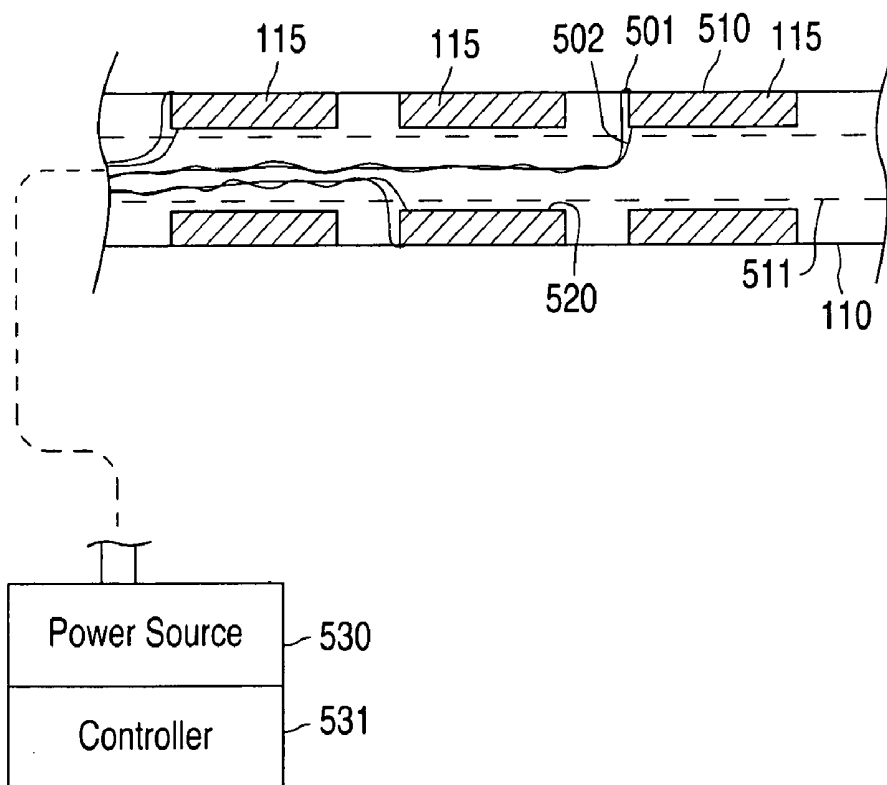


FIG. 5

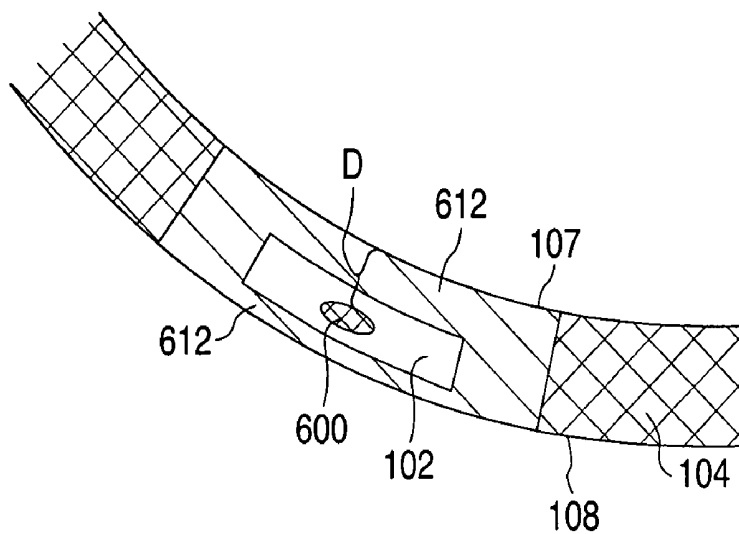


FIG. 6

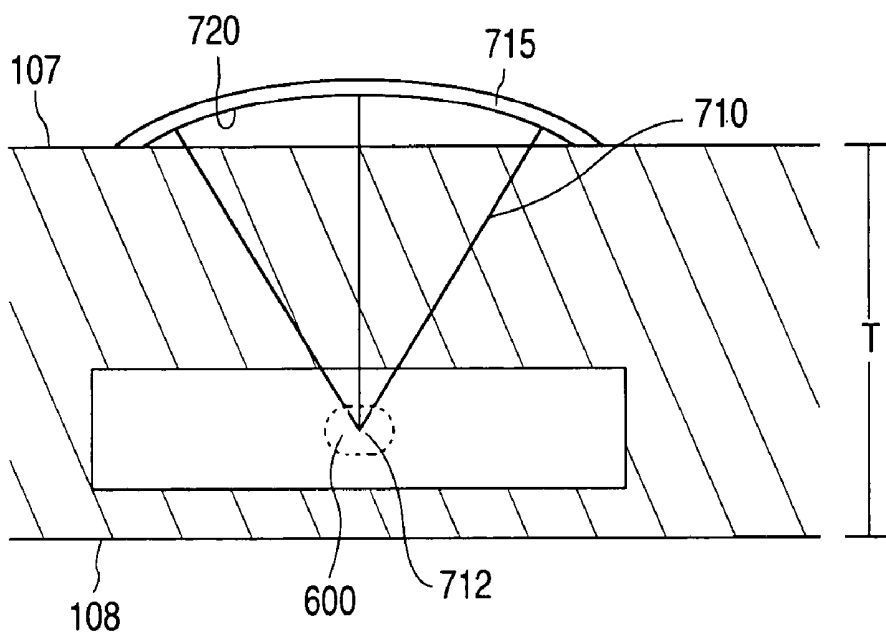


FIG. 7

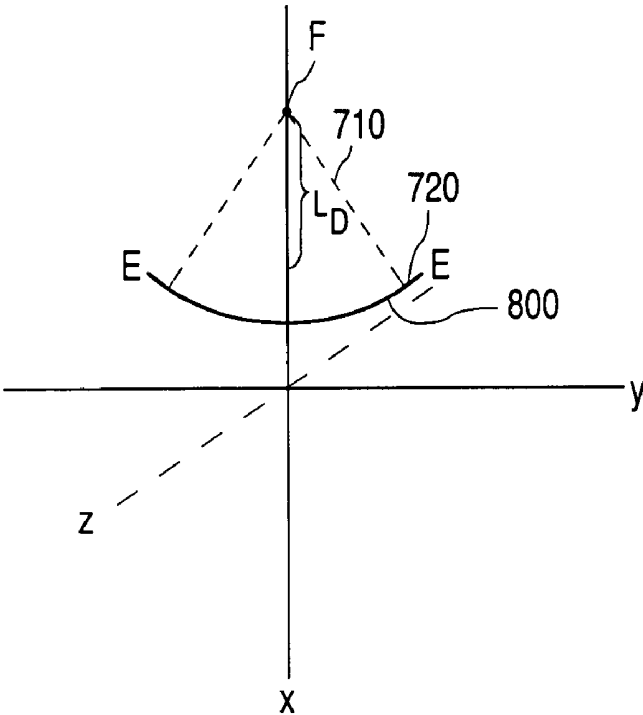


FIG. 8A

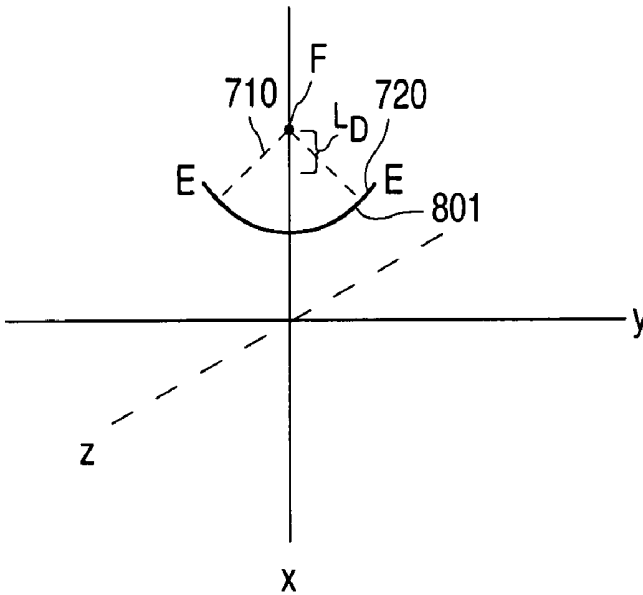


FIG. 8B

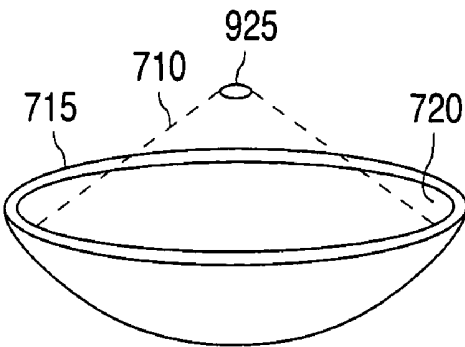


FIG. 9A

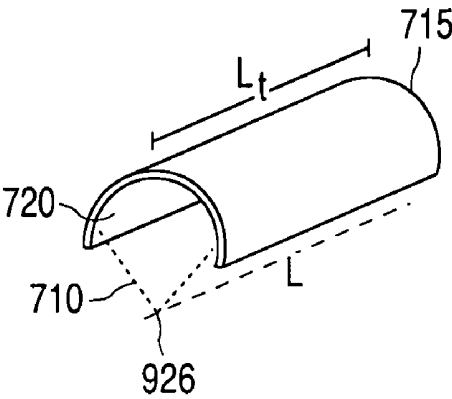


FIG. 9B

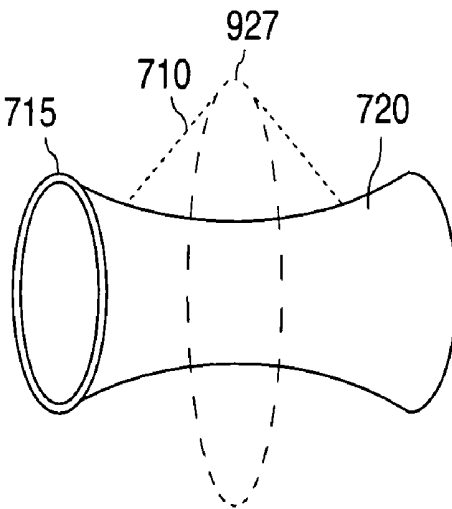


FIG. 9C

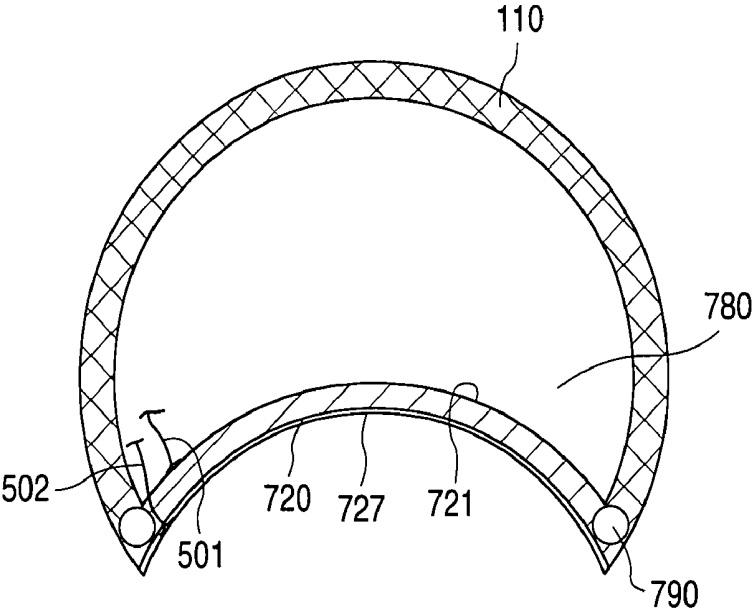


FIG. 10

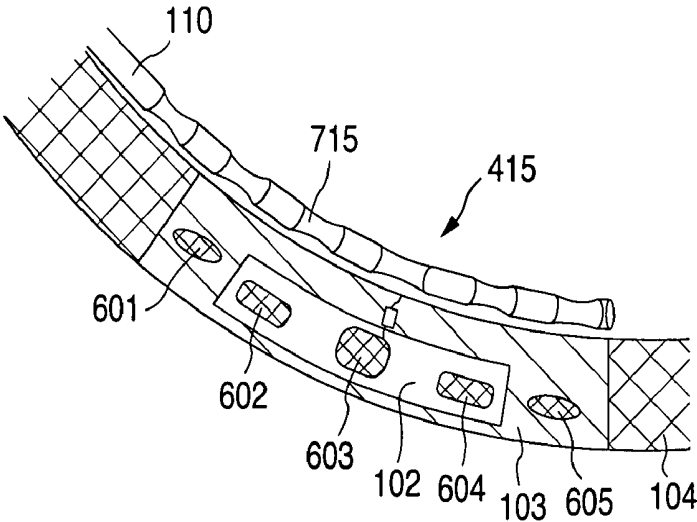


FIG. 11

ULTRASOUND ENERGY DRIVEN INTRAVENTRICULAR CATHETER TO TREAT ISCHEMIA

BACKGROUND

[0001] 1. Field of the Invention

[0002] The invention relates generally to treatment of heart disease. More particularly, the invention is directed to an ultrasonic method and apparatus to treat ischemic tissue.

[0003] 2. Description of the Background

[0004] Heart disease is a significant health problem and impairs the quality of life for millions of people. A common form of heart disease is ischemic heart disease, a condition in which parts of the heart muscle, or myocardium, do not receive an adequate supply of blood. Typically, this condition occurs when the arteries that carry blood to the myocardium become clogged by plaque build-up on their inner walls. The clogged arteries hinder blood flow, and the myocardium is deprived of oxygen and other nutrients. Ischemia results.

[0005] A number of methods are employed to improve blood flow to myocardium downstream of an arterial blockage. Many of these methods, such as coronary bypass surgery and balloon angioplasty, involve circumvention or removal of the arterial obstruction to re-establish blood flow. An alternate set of methods, known as transmyocardial revascularization (TMR) or percutaneous transmyocardial revascularization (PMR), involve the creation of small channels in the myocardium itself to reperfuse the ischemic tissue.

[0006] Channels created by the TMR or PMR procedures were initially believed to relieve ischemia by allowing blood to flow directly from the ventricle into the ischemic myocardium. More recent studies suggest that the channels do not remain open. Instead, the TMR or PMR procedures may stimulate angiogenesis, the creation of new blood vessels, and it is the new blood vessels that restore blood flow to the ischemic region. Angiogenesis is a natural response to cellular damage and results when injured cells alert the body to heal itself. It is believed that cells damaged by the TMR or PMR procedures produce and excrete special chemicals, such as cytokines and growth factors, which signal surrounding cells to initiate the formation of new blood vessels. The new blood vessels grow into the ischemic region, supplying the region with blood.

[0007] TMR and PMR methods used to create channels in the myocardium include mechanical coring, ultrasonic cutting, laser drilling, and using radio frequency (RF) energy to burn through the heart tissue. The mechanical, ultrasonic, laser, or RF device is typically positioned at the end of a catheter. The catheter is inserted either through the patient's cardiovascular system to place the device into the inside of the heart or through a small cavity in the patient's chest to place the device onto the outside of the heart.

[0008] Mechanical coring methods create channels in the myocardium by displacing or removing the heart tissue. Cutting devices such as needles or blades are employed.

[0009] Ultrasonic devices, such as those described in U.S. Pat. No. 5,827,203 to Nita and U.S. Pat. No. 5,989,274 to Davison et al., are also used to mechanically scrape or cut

channels into the heart tissue. With these devices, ultrasonic energy is applied at frequencies between 20 kHz and 100 kHz to a tip at the end of a catheter. The ultrasonic energy causes the tip to vibrate and pierce the surface of the heart to form a channel. A blade may be attached to the tip to facilitate cutting.

[0010] Lasers, such as CO₂ lasers, vaporize the heart tissue to bum channels in the myocardium. Myocardial revascularization using lasers is described, for example, in U.S. Pat. No. 6,074,384 to Brinkmann et al.

[0011] RF energy can also be used to burn holes in the myocardium, as described in U.S. Pat. No. 6,030,380 to Auth et al., U.S. Pat. No. 5,944,716 to Hektner, and U.S. Pat. No. 6,032,674 to Eggers et al.

[0012] A problem with the above procedures is that creating channels in the myocardium causes excessive trauma and damage to the heart tissue. The epicardium, endocardium, or both are punctured to form the channels, leading to a risk of complications such as hemorrhaging and scarring. The possibility that an embolus will form and cause, for instance, a stroke is another potential complication with the procedures.

[0013] As to problems with the particular methods described above, laser energy is known to kill healthy cells, which may worsen the patient's condition. The laser procedure may also cause denervation, which relieves the chest pain associated with ischemia, but permanently damages the heart muscle. In addition, controlling the location and depth of a channel formed by laser or RF energy is difficult, making accidental damage to healthy tissue more likely. RF energy is also diffuse, making it especially difficult to localize damage from the RF energy device, and creating problems such as the coagulation of surrounding blood.

[0014] U.S. Pat. No. 5,827,203 also describes using low frequency ultrasonic energy to massage the ischemic myocardium, without cutting or removing the tissue, as is required when creating channels. However, although massaging the tissue is less traumatic to the heart tissue than creating channels, massaging alone does not fully treat ischemia and does not cause the cellular damage necessary to stimulate angiogenesis.

SUMMARY

[0015] Embodiments of the present invention include methods and apparatuses for treating ischemic myocardium. The invention minimizes injury to the heart tissue and risk to the patient while still causing the cellular damage believed necessary for revascularization of ischemic tissue.

[0016] In one embodiment, an ultrasonic device is used to form localized, precisely placed thermal lesions in and near the ischemic tissue. Ultrasonic energy can be advantageously locally directed and is relatively easy to control. Therefore, the thermal lesions formed by ultrasonic energy can induce angiogenesis in myocardium without creating channels and without excessive damage and trauma to the tissue. Even beyond inducing angiogenesis, it is believed that the method will assist in increasing blood flow to the treated region and mitigates the progression and symptoms of ischemia.

[0017] In one particular embodiment, a catheter having a distal end is inserted into the patient. The catheter has at least

one ultrasonic transducer on the distal end. The ultrasonic transducer is positioned proximate to the ischemic region. Ultrasonic energy is applied at a frequency at or above 1 MHz to create a first thermal lesion in the ischemic region of the myocardium. For example, the ultrasonic energy can be applied at frequencies between 4 MHz and 15 MHz to create the thermal lesion.

[0018] The method may further include repositioning the ultrasonic transducer and applying ultrasonic energy at a frequency at or above 1 MHz to create one or more second thermal lesions in the myocardium. The second thermal lesion(s) may be created in the ischemic region adjacent the first thermal lesion or in myocardium adjacent the ischemic region. The first and second lesions can be created so as to have a gradient of sizes.

[0019] An embodiment of an ultrasonic catheter within the present invention can have an array of ultrasonic transducers. Ultrasonic energy at a frequency greater than approximately 1 MHz can be applied from the ultrasonic transducers in the array to create additional thermal lesions. The ultrasonic transducers of the array may be independently coupled to a power source and independently controlled by a controller, allowing ultrasonic energy of varying power and duration to be independently applied from each transducer in the array. The controller can control the duty cycle of the power source, so that higher powers can be applied to the tissue without overheating the transducer. The independently controlled transducers in the array can advantageously be used to create multiple thermal lesions that have a gradient of sizes.

[0020] The ultrasonic transducer can have a shape that causes the ultrasonic energy emitted by the transducer to converge in a region located internal to the myocardium and at a distance from the endocardium and epicardium. The transducer can have, for example, a bowl-like, partial cylinder, or hollow hyperboloid-like shape. Accordingly, the thermal lesions produced by the converging ultrasonic energy will be located internal to the myocardium and distal from the endocardium and epicardium. This allows ischemic region internal to the myocardium to be treated without injuring the endocardium or epicardium.

[0021] These and other embodiments and aspects of the present invention will be better understood in view of the attached drawings and the following detailed description.

BRIEF DESCRIPTION OF THE FIGURES

[0022] FIG. 1 is a diagrammatic view of a human heart in partial cross section showing a catheter with a distal end proximate to an ischemic region of the myocardium.

[0023] FIG. 2A illustrates a “side-fire” ultrasound transducer of a catheter that is located adjacent to an ischemic region of the myocardium, and a thermal lesion produced in the ischemic region by ultrasound energy from the transducer.

[0024] FIG. 2B is a plan view of a catheter with a transducer on the distal end. Electrical leads connect the transducer to a power supply and controller.

[0025] FIGS. 3A, 3B, and 3C illustrate multiple thermal lesions in the ischemic region and myocardium adjacent the ischemic region with arrows indicating the direction of

concentration gradients of growth factors and other angiogenesis stimulating substances. In FIG. 3A, the thermal lesions are approximately equivalent in size, in FIGS. 3B and 3C, the thermal lesions decrease in size from the center of the ischemic region.

[0026] FIG. 4 illustrates a catheter having an array of ultrasound transducers positioned over the ischemic region and the multiple lesions produced by the ultrasound energy from transducers in the array.

[0027] FIG. 5 is a sectional representation of a portion of the array of transducers illustrated in FIG. 4 and the electrical leads connecting the transducers to the power source and controller.

[0028] FIG. 6 is a sectional representation of an internal ischemic region that is located within the myocardium and a thermal lesion centered in the ischemic region. The lesion does not contact the endocardium or epicardium.

[0029] FIG. 7 is a sectional representation of a concave ultrasound transducer element located on the myocardium of FIG. 6, where ultrasound energy delivered from the concave transducer element is focused into the ischemic region.

[0030] FIGS. 8A and 8B illustrate exemplary curves that the transducer illustrated in FIG. 7 may be shaped as to focus the ultrasound energy.

[0031] FIGS. 9A, 9B, and 9C illustrate exemplary ultrasound transducers shaped to focus ultrasound energy.

[0032] FIG. 10 is a sectional end-on view of a concave ultrasound transducer mounted in a catheter.

[0033] FIG. 11 illustrates a catheter having multiple concave transducer elements and lesions produced in an internal ischemic region and adjacent myocardium by the ultrasound energy delivered by the transducers.

DETAILED DESCRIPTION

[0034] FIG. 1 illustrates a heart 100 having an ischemic region 102 in the myocardium 104 of the left ventricle 106. A catheter 110 has been inserted into the left ventricle 106. An ultrasound transducer 115 is mounted on distal portion 117 of catheter 110. Ultrasound transducer 115 is positioned adjacent to the endocardial surface 107 and proximate to ischemic region 102, where it is used to treat ischemic region 102, as described below. In particular, transducer 115 is positioned on the endocardial surface 107 laterally adjacent ischemic region 102.

[0035] Although FIG. 1 illustrates ischemic region 102 and catheter 110 in the left ventricle 106, which is particularly susceptible to ischemia, the beneficial effect of the procedures and devices described herein can be used to treat any ischemic area of the heart or other body tissue.

[0036] FIG. 2A illustrates a portion of myocardium 104 with an ischemic region 102. Ultrasound transducer 115 on catheter 110 is oriented toward ischemic region 102. A thermal lesion 200 has been created in ischemic region 102 by ultrasound energy that was emitted from ultrasound transducer 115 at a frequency at or above 1 MHz.

[0037] As defined herein, a “thermal lesion” is a localized injury to tissue caused by application of ultrasonic energy at frequencies at or above 1 MHz. In the various embodiments

of the invention, such thermal lesions are created to treat the ischemic tissue. Ultrasonic energy delivered to tissue at frequencies at or above 1 MHz heats the tissue to cause damage to cells within the area of the lesion. It is believed that the cells damaged by the high-frequency ultrasonic energy produce angiogenesis stimulating substances such as cytokines and growth factors. The angiogenesis stimulating substances promote the growth of new blood vessels, which may grow toward, away from, and/or in the vicinity of the angiogenesis stimulating substances. Thus, the tissue in and around the thermal lesion is revascularized.

[0038] By contrast, the above-described ultrasonic references (i.e., Nita and Davison et al.) use ultrasound energy having a frequency of 20 kHz to 100 kHz to shake an end effector against the tissue, thereby producing gross mechanical motion of the tissue. The gross mechanical motion massages and shakes the tissue, but does not cause revascularization. In the embodiments of the present invention, the ultrasonic transducer sends ultrasonic energy directly into the tissue at frequencies that begin at 1 MHz, e.g. 10 MHz, at least an order of magnitude higher than the above references, to obtain molecular motion and thus cause the requisite thermal cellular damage.

[0039] Such thermal lesions can be created using, for example, the ultrasound device described in U.S. Pat. No. 5,735,280 to Sherman and Castellano, which patent is incorporated herein by reference in its entirety. In the following discussion, aspects of such a device, and modifications thereto in accordance with the present invention are discussed in detail.

[0040] As illustrated in FIG. 2B, transducer 115 is connected to a power source 530 and controller 531 via electrical leads 240 that traverse the length of catheter 110. Power source 530 provides energy to transducer 115 through electrical leads 240. Controller 531 (typically containing a microprocessor) controls the power supplied to transducer 115 from power source 530. Ultrasound transducer 115 is typically a piezo-electric crystal that can deliver ultrasonic energy at frequencies greater than 1 MHz. In this embodiment, transducer 115 is a cylindrical, "side-fire" transducer. Ultrasonic energy is emitted radially from the sides of the transducer.

[0041] To create a thermal lesion, ultrasonic energy can be delivered to the tissue from transducer 115 at, for the example of a cylindrical transducer, a power of between 2 and 20 watts, typically 8-10 watts for a duration time in the range of 15 to 300 seconds, typically 120 seconds. The ultrasonic energy is delivered at a frequency at or above 1 MHz, e.g., between 1 MHz and 15 MHz, or more typically between 4 MHz and 10 MHz.

[0042] In creating the thermal lesion(s) in accordance with the present invention, it is desirable to control the temperature of the ultrasound transducer 115. In particular, it is desirable to keep the transducer from getting so hot as to boil or carbonize blood or tissue that directly contacts transducer 115. To avoid such a situation, the temperature of the transducer is kept at or below 70° C. to 80° C., as monitored by temperature sensors placed on the transducer crystal. The temperature sensors provide feedback to the controller, which accordingly adjusts the power supplied to transducer 115. The power supplied to the transducer may be controlled by appropriate setting of the voltage level. Alternatively, the

duty cycle of the power source can be regulated in a manner that achieves high peak power while maintaining a relatively low effective power level, as described in U.S. Pat. No. 5,971,980 to Sherman, which is incorporated herein by reference in its entirety. Because the transducer cools more quickly than the tissue, the duty cycle can be used to keep the transducer below the desired temperature while maintaining the peak power level needed to create the thermal lesions.

[0043] Catheter 110 can be any surgical tool capable of advancing and positioning ultrasound transducer 115. For example, catheter 110 can be a flexible guide catheter having a steerable tip, such as the catheter described in U.S. Pat. No. 5,857,997. Catheter 110 may be fitted with additional surgical equipment, such as a fiber optic scope for internal viewing, control circuitry for synchronizing delivery of ultrasound energy with the heartbeat cycle, or other devices for enhancing the safety and effectiveness of the surgical method.

[0044] Methods for accessing the heart with a surgical tool such as catheter 110 are well known. For example, catheter 110 can be inserted into the femoral artery and maneuvered through the aorta and into the left ventricle or into one of the main coronary arteries such as the left anterior descending or left circumflex. Alternatively, the heart can be externally accessed by inserting catheter 110 through an opening in the patient's chest, e.g., a sternotomy or mini-thoractomy, and positioning the ultrasound transducer 115 adjacent the epicardial surface or pericardial sac. Fluoroscopic, ultrasound, or other imaging techniques can be used to view catheter 110 and transducer 115 as they are guided through the body and positioned proximate to ischemic region 102. The location within the body of ischemic region 102 can be identified by known techniques, such as angiography. Note also that creation of thermal lesions in accordance with the embodiments of the invention may be performed in conjunction with other procedures, for example coronary artery bypass graft (CABG) surgery.

EXEMPLARY TREATMENT REGIMES

[0045] As mentioned above, we believe that, by creating thermal lesions in myocardium using ultrasonic energy applied at a frequency at or above 1 MHz without cutting or piercing the tissue, the tissue will be sufficiently damaged to release angiogenesis stimulating substances. The thermal lesions do not traumatize the tissue to the degree of conventional TMR and PMR procedures. In the description below, various treatment regimes are discussed which provide thermal lesions in various locations and amounts, as may be appropriate to particular clinical situations.

[0046] A. Creating Multiple Thermal Lesions

[0047] Multiple thermal lesions, as illustrated by exemplary thermal lesions 301, 302, and 303 of FIG. 3A, may be created throughout the ischemic region. We believe that the damaged cells in the thermal lesion will release angiogenesis stimulating substances, such as growth factors and cytokines, and that new blood vessels will grow in the vicinity of the substances so released. In a larger ischemic region, multiple thermal lesions throughout the ischemic region will cause angiogenesis stimulating substances to be released throughout the region, and thus promote revascularization of the entire region. The number of thermal lesions needed to

treat an ischemic area depends on factors such as the size of the ischemic area and degree of ischemia, as determined by the physician, and the size of the thermal lesions produced. The size of the thermal lesion produced, in terms of the surface area of the ischemic tissue covered by the thermal lesion, generally corresponds to the size of the transducer and the amount of contact the transducer has with the tissue. Typically, transducer **115** is 1 to 10 mm long and 1 to 10 mm in width (e.g., the diameter of a cylindrical transducer), creating thermal lesions that cover a surface area 1 to 10 mm in length and 1 to 10 mm in width. Typically, at least one thermal lesion is created for each square centimeter (cm²) of ischemic region.

[0048] FIG. 3A also illustrates thermal lesions **304** and **305**, which may be created in region **103** adjacent the ischemic region, where the heart tissue is healthier. New blood vessels may form more readily in the healthier tissue and may grow from the healthier tissue in region **103** toward the angiogenesis stimulating substances produced by the damaged cells in thermal lesions **301**, **302**, and **303**, as illustrated by the arrows **310** and **311**.

[0049] In another embodiment, illustrated by the example of FIG. 3B, the size of the thermal lesions is varied to produce a gradient of sizes of the thermal lesions. Larger thermal lesions, such as thermal lesion **320**, are created towards the center of the ischemic tissue. The larger thermal lesions **320** typically release larger amounts of angiogenesis stimulating substances than do the smaller thermal lesions **322** at the edges of the ischemic region. Thus, the size gradient of thermal lesions creates a concentration gradient of the released angiogenesis stimulating substances, illustrated by arrows **325**, **326**. It is believed that more new blood vessels may grow in the vicinity of the higher concentrations of the angiogenesis stimulating substances or that the higher concentration may stimulate the new blood vessels to grow over a larger distance. The gradient of sizes of the thermal lesions therefore may promote growth of new blood vessels in the center of ischemic region **102**.

[0050] For a given size of transducer **115**, the size of a thermal lesion can be varied by varying the power output of the ultrasound transducer. The power output can be varied either by varying the voltage applied to transducer **115**, the duty cycle (as described above), or the frequency of the ultrasound energy. In general, for transducer geometries such as cylindrical or flat, in which the ultrasound energy that radiates from the transducer does not converge (see below), more power creates a deeper lesion. The distance the transducer is from the myocardial tissue will also determine how deep into the tissue the ultrasonic energy penetrates and, hence, the size of the thermal lesion.

[0051] FIG. 3C illustrates an alternative embodiment that combines the methods illustrated in FIGS. 3A and 3B. Thermal lesions **340**, **341**, **342**, **343**, and **344** of varied size are created across ischemic region **102** and are also created in the area **103** adjacent the ischemic region.

[0052] To make the multiple thermal lesions illustrated in FIGS. 3A-3C with a catheter **110** having a single transducer element **115**, as illustrated in FIG. 2B, transducer **115** is repositioned each time a new thermal lesion is to be created. However, if multiple thermal lesions are to be created, single transducer **115** must be repositioned several times, which can make the procedure lengthy and may expose the patient to additional risk of complications.

[0053] An alternative apparatus that avoids or reduces the need to reposition transducer **115** several times is illustrated in FIG. 4. An array **415** of transducers **115** is provided at the distal end of catheter **110**. While ten transducers **115** are shown in array **415** of FIG. 4, the number of transducers may be more or less, and catheter **110** typically contains an array of between 5 and 15 ultrasound transducers **115** depending on the application. The spacing **416** between each transducer **115** can also vary with the application. For example, in one treatment regime, a thermal lesion is created for every one square centimeter of surface area of ischemic region **102** on the endocardium or epicardium. To treat an ischemic region **102** that has 25 cm² surface area and that is approximately square (5 cm×5 cm), a catheter **110** should have an array **415** of at least 5 transducers with, for instance, one transducer per cm in the array (e.g., transducers of 4 mm in length with a spacing **416** of 6 mm between them). To cover the 25 cm² ischemic area, such an array can be positioned five times to create five lines of five thermal lesions for a total of 25 thermal lesions. With respect to the spacing **416**, small, tightly spaced ultrasound transducers can be used to make small, tightly spaced thermal lesions, but may make distal end **117** of catheter **110** less flexible.

[0054] The transducer array **415** only needs to be positioned so that a portion of the transducers **115** overlies ischemic region **102**. Radiopaque or other markers on the catheter can be used to identify which of the transducers **115** are located over the ischemic region **102** and adjacent region **103**. The identified transducers can be selectively activated by the controller to produce thermal lesions in region **102** and, if desired, region **103**. The controller can also individually control the power output (by controlling the voltage, duty cycle, and/or frequency) of each transducer, to produce thermal lesions of varying sizes. Typically catheter **110** having an array **415** of transducers **115** will not need to be repositioned, or will only need to be repositioned a relatively small number of times, to create the desired pattern of thermal lesions across the entire ischemic region **102**. The size of ischemic region **102** typically will be a factor in determining whether any repositioning of array **415** will be necessary.

[0055] Typically, each transducer **115** of multi-transducer catheter **110** is individually coupled to the power source. As illustrated in the embodiment of FIG. 5, each of the multiple transducers **115** has an electrical lead **501** connected to the outer surface **510** of the transducer and an electrical lead **502** connected to the inner surface **520** of the transducer. Electrical leads **501**, **502** can be narrow (44-48 gauge) coaxial cable or twisted pair balanced feed line. The coaxial cable contains an inner wire for carrying the electrical signal, and a ground wire surrounding the inner wire to shield the inner wire from electrical noise. Coaxial cables or twisted pair balanced feed lines are typically used for electrical leads **501**, **502** instead of bare wire to minimize impedance loss over the length of the wire due to standing wave reflections. Electrical leads **501**, **502** run through an inner lumen **511** of catheter **110** to the power source, and are flexible, so as not to hinder plasticity of catheter **110**. Inner lumen **511** will also contain components (no shown) for steering and guiding catheter **110** through the body.

[0056] Electrical leads **501**, **502** deliver energy to the transducers **115** from a power source **530**. Controller **531** controls power source **530**. The controller **531** (typically

containing a microprocessor) can be programmed to selectively turn on and individually controlled each transducer 115. Transducers 115 can be activated simultaneously or sequentially, and power can be controlled to each using the amplitude of the voltage, duty cycle, or frequency as described above.

[0057] B. Creating Thermal Lesions Located Internal to the Myocardium

[0058] A method of treatment within the present invention uses ultrasonic energy having a frequency at or above 1 MHz to create thermal lesion(s) that are internal to the myocardium and advantageously do not damage the endocardium or epicardium. FIG. 6 illustrates an embodiment of this method, where a thermal lesion 600 has been created at a depth D within the myocardium 104. Thermal lesion 600 does not overlap the endocardium 107 or the epicardium 108. Likewise, thermal lesion 600 does not overlap healthy myocardium 612 between the endocardium 107 or epicardium 108 and the ischemic region 102.

[0059] FIG. 7 illustrates a curved ultrasonic transducer 715 for creating thermal lesion 600 of FIG. 6. Transducer 715 is similar to transducer 115, except that transducer 715 is shaped so that ultrasonic energy 710 radiates from the concave surface 720 and converges at a site 712 beyond the transducer. Transducer 715 can be positioned over ischemic region 102 and set on the endocardial 107 (or epicardial 108) surface of myocardium 104 with the concave surface 720 facing the myocardium. Ultrasound energy emitted from transducer 715 will be focused in the ischemic region to form thermal lesion 600.

[0060] Transducer 715 can have, for instance, a spherical curve, as illustrated in FIG. 8A by exemplary curve 800, a parabolic curve, as illustrated by exemplary curve 801 of FIG. 8B, or any other shape that focuses the ultrasound energy. For transducer 715 having a given shape, such as curve 800, ultrasonic energy 710 will radiate from the concave side 720 of the curve and converge at a focal site F. The depth D that thermal lesion 600 is created within myocardium 104 is determined by the length L_D that focal site F extends beyond the ends E of the curve. Length L_D is determined by the degree of curvature and arc length of the curve. Healthy myocardium has a thickness, T, (shown in FIG. 7) of approximately 1-2 mm, but the myocardium of diseased hearts can be thicker, for instance up to approximately 7 mm. Therefore, the depth D of thermal lesion 600 can be set to between, for example, 1 and 7 mm.

[0061] Curved transducer 715 can have a variety of shapes, including, but not limited to, the exemplary shapes illustrated in FIGS. 9A, 9B, and 9C. FIG. 9A illustrates transducer 715 in an exemplary bowl-like shape formed by the surface of rotation of a curve, such as curve 800 or 801, about the x-axis in FIGS. 8A and 8B, respectively. Ultrasonic energy 710 radiating from a transducer 715 of FIG. 9A converges in a central site, for example, site 925.

[0062] FIG. 9B illustrates transducer 715 having an exemplary shape that is a partial cylinder formed by the surface of translation of a curve, such as curve 800 or 801, along the z-axis of FIGS. 8A and 8B, respectively. Ultrasonic energy 710 emanating from transducer 715 of FIG. 9B converges along line 926, having a length L approximately equal to the length L_t of the transducer.

[0063] FIG. 9C illustrates transducer 715 having an exemplary hollow tubular shape with flared ends, such as a hyperboloid-like shape, formed by the surface of rotation of the curve, such as curve 800 or 801, about they-axis in FIGS. 8A and 8B, respectively. Ultrasonic energy 710 radiating from transducer 715 of FIG. 9C converges along a circle 927 surrounding the transducer. Therefore, ultrasound energy emitted from a hyperboloid-like shaped transducer 715 will form a thermal lesion in the form of an arc through the tissue, damaging the endocardial (or epicardial) surface at the point where the circle 927 intersects the endocardial (or epicardial) surface. However, a hyperboloid-like shaped transducer advantageously does not have to be oriented in a particular direction to irradiate ultrasound energy into the tissue.

[0064] Shaped transducer 715 can be formed by cutting, typically with an ultrasonic or mechanical machining process, sintering a powder of, or molding the ceramic material into the desired shape. The shaped ceramic is then polarized in a known process, for example exposing the ceramic to a high electric field, so that it will radiate ultrasound energy. Transducer 715 can be formed from, for example, LTZ2 (Staveley Sensors, Inc., East Hartford, Conn.), PZT, or other lead-ceramic materials, such as PbTiO_3 (lead titanate) or PbZrO_3 (lead zirconate).

[0065] The resonant frequency of the transducer is inversely proportional to the thickness of the ceramic material. Typically the ceramic material is between 0.006 inch (0.15 mm) to 0.015 inch (0.38 mm) thick, depending on the desired resonant frequency. The longest dimension of transducer 715 is typically between 1 and 10 mm.

[0066] FIG. 10 illustrates a sectional view of concave transducer 715 mounted in catheter 110. The front 720 and back 721 surfaces of the transducer 715 are typically coated with conductive material plating (not shown), such as gold, platinum or palladium, or other similar conductive materials. A thin layer of a bio-compatible coating 727, such as Epo-Tek 353 ND (Epo-Tek, Inc., Billerica, Mass.) or parylene is typically applied to concave surface 720. Coating 727 protects and strengthens the transducer, electrically isolates the conductive surfaces, and can be used to match impedance between the crystal and the tissue.

[0067] The transducer 715 is mounted to the catheter 110 through an o-ring 790, or other mechanical means that seals transducer 715 to catheter 110. Solder joints are used to mechanically attach and electrically connect the electrical leads 501, 502 to the transducer 715. In addition to solder joints, a conductive epoxy, cold solders, ultrasonic welds and other similar attachment techniques can be used. Electrical leads 501, 502 are generally connected at the edge of transducer 715 because solder may dampen the vibrations of the transducer.

[0068] There is a gap 780 between transducer 715 and catheter 110. Gap 780 may contain any suitable low-density material, including gaseous substances such as ambient air, oxygen, nitrogen, helium, an open-cell polymeric foam, a closed cell polymeric foam, and other similar polymeric materials and mixtures thereof. Ultrasonic energy does not travel through low-density material but instead is reflected by the low-density materials. Therefore, the ultrasonic energy that radiates inward from transducer 715, off back surface 721, is reflected rather than being absorbed by the

catheter. Gap **780** can be extremely thin, for example, $\frac{1}{1000}$ of an inch (0.025 mm), to leave room within catheter **110** for electrical leads **501, 502** and additional steering and guiding components (not shown). Catheter **110** is typically between 5 and 8 french in diameter.

[0069] Because the ultrasonic energy emitted from transducer **715** is focused, less power, for example, 2-3 Watts, is typically needed to create the thermal lesion **600** than to create a thermal lesion from an unfocused transducer. The duration of application of the ultrasonic energy will be similar to those listed above.

[0070] FIG. 11 illustrates a catheter **110** having an array **415** of curved transducers **715** at a distal end. Curved transducers **715**, illustrated here as having the exemplary hyperboloid-like shape illustrated in FIG. 9C, focuses ultrasonic energy as described above. The transducers **715** in array **415** are connected to a power source and controller as illustrated in FIG. 5 and operate in the same manner as described above with respect to FIG. 5.

[0071] In FIG. 11, multiple thermal lesions **601, 602, 603, 604, 605** have been created at a depth D within myocardium **104** by transducers **715** in array **415**. The thermal lesions have a gradient of sizes, as described above with respect to FIG. 3B, and lesions **601** and **605** have been created within the healthier tissue of region **103**, as describe above in reference to FIG. 3A.

[0072] While particular embodiments of the present invention have been shown and described, it will be clear to those of ordinary skill in the art that changes and modifications can be made without departing from this invention in its broader aspects and, therefore, the appended claims are to encompass all such changes and modifications as falling within the scope of this invention.

1.-20. (cancelled)

21. A method of treating an ischemic region of a patient, comprising creating a concentration gradient of an angiogenesis stimulating substance in the ischemic region and/or in tissue of a region adjacent the ischemic region.

22. The method of claim 21, wherein the tissue of the region adjacent the ischemic region is non-ischemic.

23. The method of claim 21, wherein the concentration of the angiogenesis stimulating substance is highest at about the center of the ischemic region.

24. The method of claim 21, wherein the concentration of the angiogenesis stimulating substance is higher in the ischemic region than in the tissue of the region adjacent the ischemic region.

25. The method of claim 24, wherein the tissue of the region adjacent the ischemic region is less ischemic than the tissue of the ischemic region.

26. The method of claim 24, wherein the tissue of the region adjacent the ischemic region is non-ischemic.

27. The method of claim 21, wherein the concentration of the angiogenesis stimulating substance is lower in the ischemic region than in the tissue of the region adjacent the ischemic region.

28. A method of treating a region of ischemic tissue in a patient, comprising triggering the release of angiogenesis stimulating substances to create a concentration gradient of the angiogenesis stimulating substances in the region of ischemic tissue and/or in tissue of a region adjacent the region of ischemic tissue.

29. The method of claim 28, wherein the angiogenesis stimulating substances are released by the region of ischemic tissue.

30. The method of claim 28, wherein the angiogenesis stimulating substances are released by the tissue of the region adjacent to the region of ischemic tissue.

31. A method of treating ischemic myocardial tissue of a patient, comprising:

inserting into the patient a catheter having a tissue stimulating device;

positioning the tissue stimulating device on or near the ischemic myocardial tissue; and

stimulating the ischemic myocardial tissue and/or myocardial tissue near the ischemic myocardial tissue without piercing or cutting the myocardial tissue to trigger the release of an angiogenic factor.

32. The method of claim 31, wherein the stimulation creates a concentration gradient of the angiogenic factor.

33. A method of claim 55, further comprising:

repositioning the tissue stimulating device; and

stimulating the ischemic myocardial tissue and/or myocardial tissue near the ischemic myocardial tissue without piercing or cutting the myocardial tissue to trigger the additional release of the angiogenic factor.

34. The method of claim 33, wherein the stimulation creates a concentration gradient of the angiogenic factor.

* * * * *

专利名称(译)	超声能量驱动脑室内导管治疗缺血		
公开(公告)号	US20040193051A1	公开(公告)日	2004-09-30
申请号	US10/817358	申请日	2004-04-01
[标]申请(专利权)人(译)	MANDRUSOV EVGENIA 管家JEFFREY SHERMAN MARSHALL		
申请(专利权)人(译)	MANDRUSOV EVGENIA 管家JEFFREY SHERMAN MARSHALL		
当前申请(专利权)人(译)	高级心血管系统公司.		
[标]发明人	MANDRUSOV EVGENIA STEWART JEFFREY SHERMAN MARSHALL		
发明人	MANDRUSOV, EVGENIA STEWART, JEFFREY SHERMAN, MARSHALL		
IPC分类号	A61B17/00 A61N7/02 A61B8/00		
CPC分类号	A61B2017/00247 A61N7/022 A61B2018/00392		
其他公开文献	US7001336		
外部链接	Espacenet USPTO		

摘要(译)

提供了一种用于改善患者向缺血区域(例如,心肌缺血)的血流的方法和装置。超声换能器位于缺血区域附近。以1MHz或更高的频率施加超声能量以在心肌的缺血区域中产生一个或多个热损伤。热损伤可具有大小梯度。超声换能器可以具有弯曲形状,使得换能器发射的超声能量会聚到心肌内的部位,从而产生热损伤而不会损伤心外膜或心内膜。

