



US007774933B2

(12) **United States Patent**
Wilson et al.

(10) **Patent No.:** **US 7,774,933 B2**
(45) **Date of Patent:** **Aug. 17, 2010**

(54) **METHOD OF MANUFACTURING
ULTRASOUND CATHETERS**

(75) Inventors: **Richard R. Wilson**, Seattle, WA (US);
Tim Abrahamson, Seattle, WA (US);
Leonard R. Oliver, Seattle, WA (US)

(73) Assignee: **Ekos Corporation**, Bothell, WA (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 1110 days.

(21) Appl. No.: **11/417,384**

(22) Filed: **May 4, 2006**

(65) **Prior Publication Data**

US 2006/0201604 A1 Sep. 14, 2006

Related U.S. Application Data

(60) Division of application No. 10/378,032, filed on Feb.
28, 2003, now abandoned, which is a continuation-in-
part of application No. 10/309,417, filed on Dec. 3,
2002, now Pat. No. 7,384,407.

(60) Provisional application No. 60/361,341, filed on Feb.
28, 2002.

(51) **Int. Cl.**
H01R 43/00 (2006.01)
H05K 13/00 (2006.01)

(52) **U.S. Cl.** **29/854**; 29/595; 29/825;
600/459; 600/463; 600/466; 600/467

(58) **Field of Classification Search** 29/854,
29/595, 825, 857, 874; 600/459, 463, 466,
600/467

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,433,226 A	3/1969	Boyd
4,040,414 A	8/1977	Suroff
4,176,662 A	12/1979	Frazer
4,319,580 A	3/1982	Colley et al.
4,531,943 A	7/1985	Van Tassel et al.

(Continued)

FOREIGN PATENT DOCUMENTS

DE 4005743 8/1991

(Continued)

OTHER PUBLICATIONS

Hynynen et al.; "Small Cylindrical Ultrasound Sources for Induction
of Hyperthermia Via Body Cavities or Interstitial Implants", Int. J.
Hyperthermia, 1993, vol. 9, No. 2, 263-274, Tucson, Arizona.

(Continued)


Primary Examiner—Thiem Phan

(74) *Attorney, Agent, or Firm*—Knobbe Martens Olson &
Bear, LLP

(57) **ABSTRACT**

An ultrasonic catheter is manufactured by providing an inner
tube having an inner diameter sufficient to accommodate a
guidewire, and mounting a tubular ultrasound radiating mem-
ber around a distal region of the inner tube. Two electrical
conductors are positioned along the inner tube, such that one
of the electrical conductors contacts an inner side of the
ultrasound radiating member while the other electrical con-
ductor contacts an outer side of the ultrasound radiating mem-
ber. An outer tube is then concentrically translated over the
inner tube and the ultrasound radiating member, and radially
shrunk onto the inner tube.

7 Claims, 11 Drawing Sheets

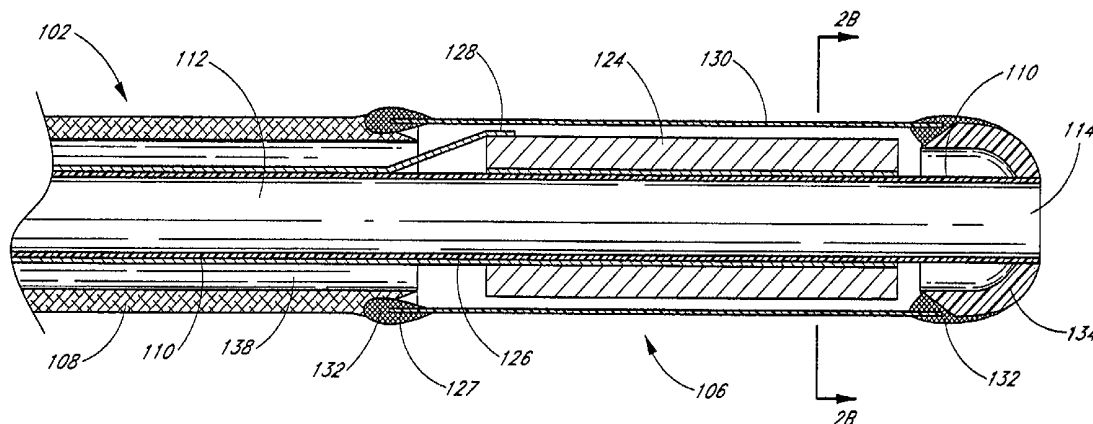

U.S. PATENT DOCUMENTS					
4,549,533 A	10/1985	Cain et al.	5,599,326 A	2/1997	Carter
4,739,768 A	4/1988	Engelson	5,603,694 A	2/1997	Brown et al.
4,750,902 A	6/1988	Wuchinich et al.	5,606,974 A	3/1997	Castellano et al.
4,808,153 A	2/1989	Parisi	5,609,574 A	3/1997	Kaplan et al.
4,841,977 A	6/1989	Griffith et al.	5,618,275 A	4/1997	Bock
4,870,953 A	10/1989	DonMichael et al.	5,620,479 A	4/1997	Diederich
4,906,238 A	3/1990	Greenfeld et al.	5,628,728 A	5/1997	Tachibana et al.
4,920,954 A	5/1990	Alliger et al.	5,628,730 A	5/1997	Shapland et al.
4,924,863 A	5/1990	Sterzer	5,630,837 A	5/1997	Crowley
4,936,281 A	6/1990	Stasz	5,713,848 A	2/1998	Dubrul et al.
4,948,587 A	8/1990	Cost et al.	5,725,494 A	3/1998	Briskin
5,021,044 A	6/1991	Sharkawy	5,728,062 A	3/1998	Briskin
5,059,851 A	10/1991	Corl et al.	5,735,811 A	4/1998	Briskin
5,108,369 A	4/1992	Ganguly et al.	5,759,173 A	6/1998	Preissman et al.
5,158,071 A	10/1992	Umemura et al.	5,782,811 A	7/1998	Samson et al.
5,163,421 A	11/1992	Bernsteing et al.	5,795,298 A	8/1998	Vesely et al.
5,197,946 A	3/1993	Tachibana	5,807,395 A	9/1998	Mulier et al.
5,226,421 A	7/1993	Frisbie et al.	5,827,313 A	10/1998	Ream
5,250,034 A	10/1993	Appling	5,827,529 A	10/1998	Ono et al.
5,267,954 A	12/1993	Nita	5,836,896 A	11/1998	Rosenschein
5,267,985 A	12/1993	Shimada et al.	5,836,946 A	11/1998	Diaz et al.
5,269,291 A	12/1993	Carter	5,842,994 A	12/1998	TenHoff et al.
5,269,297 A	12/1993	Weng et al.	5,895,398 A	4/1999	Wensel et al.
5,271,406 A	12/1993	Ganguly et al.	5,916,192 A	6/1999	Nita et al.
5,282,785 A	2/1994	Shapland et al.	5,928,186 A	7/1999	Homsma et al.
5,286,254 A	2/1994	Shapland et al.	5,931,805 A	8/1999	Briskin
5,295,484 A	3/1994	Marcus et al.	5,951,494 A	9/1999	Wang et al.
5,304,115 A	4/1994	Pflueger et al.	5,971,949 A	10/1999	Levin et al.
5,312,328 A	5/1994	Nita et al.	5,976,120 A	11/1999	Chow
5,318,014 A	6/1994	Carter	5,997,497 A	12/1999	Nita et al.
5,327,891 A	7/1994	Rammier	6,001,069 A	12/1999	Tachibana et al.
5,328,470 A	7/1994	Nabel et al.	6,024,703 A	2/2000	Zanell et al.
5,342,292 A	8/1994	Nita et al.	6,024,718 A	2/2000	Chen et al.
5,344,435 A	9/1994	Turner et al.	6,053,868 A	4/2000	Geistert et al.
5,345,940 A	9/1994	Seward et al.	6,096,000 A	8/2000	Tachibana et al.
5,348,481 A	9/1994	Ortiz et al.	6,110,314 A	8/2000	Nix et al.
5,353,798 A	10/1994	Sieben	6,113,558 A	9/2000	Rosenschein et al.
5,362,309 A	11/1994	Carter	6,120,454 A	9/2000	Suorsa et al.
5,363,853 A	11/1994	Lieber et al.	6,135,971 A	10/2000	Hutchinson et al.
5,368,036 A	11/1994	Tamaka et al.	6,176,842 B1	1/2001	Tachibana et al.
5,368,557 A	11/1994	Nita et al.	6,182,666 B1	2/2001	Dobak, III
5,380,273 A	1/1995	Dubrul et al.	6,206,831 B1	3/2001	Suorsa et al.
5,382,228 A	1/1995	Nita et al.	6,210,356 B1	4/2001	Anderson et al.
5,385,148 A	1/1995	Lesh et al.	6,228,046 B1	5/2001	Briskin
5,421,338 A	6/1995	Crowley et al.	6,235,024 B1	5/2001	Tu
5,423,797 A	6/1995	Adrian et al.	6,241,692 B1	6/2001	Tu et al.
5,427,118 A	6/1995	Nita et al.	6,241,703 B1	6/2001	Levin et al.
5,429,136 A	7/1995	Nilo et al.	6,258,080 B1	7/2001	Samson
5,431,663 A	7/1995	Carter	6,261,246 B1	7/2001	Pantages et al.
5,445,155 A	8/1995	Sieben	6,287,271 B1	9/2001	Dubrul et al.
5,447,509 A	8/1995	Mills et al.	6,296,619 B1	10/2001	Briskin et al.
5,447,510 A	9/1995	Jensen	6,361,500 B1	3/2002	Masters et al.
5,454,795 A	10/1995	Samson	6,361,531 B1	3/2002	Hissong
5,456,259 A	10/1995	Barlow et al.	6,368,315 B1	4/2002	Gillis et al.
5,458,568 A	10/1995	Racchini et al.	6,372,498 B2	4/2002	Newman et al.
5,462,523 A	10/1995	Samson et al.	6,379,320 B1	4/2002	Lafon et al.
5,465,726 A	11/1995	Dickinson et al.	6,387,035 B1	5/2002	Jung, Jr. et al.
5,474,531 A	12/1995	Carter	6,391,042 B1	5/2002	Cimino
5,496,267 A	3/1996	Drasler et al.	6,416,492 B1	7/2002	Nielson
5,496,294 A	3/1996	Hergenrother et al.	6,423,026 B1	7/2002	Gesswein et al.
5,498,238 A	3/1996	Shapland et al.	6,433,464 B2	8/2002	Jones
5,503,155 A	4/1996	Salmon et al.	6,437,487 B1	8/2002	Mohr, III et al.
5,509,896 A	4/1996	Carter	6,456,863 B1	9/2002	Levin et al.
5,514,092 A	5/1996	Forman et al.	6,461,314 B1	10/2002	Pant et al.
5,520,189 A	5/1996	Malinowski et al.	6,508,775 B2	1/2003	McKenzie et al.
5,531,715 A	7/1996	Engelson et al.	6,524,251 B2	2/2003	Rabiner
5,542,917 A	8/1996	Nita et al.	6,524,300 B2	2/2003	Meglin
5,546,948 A	8/1996	Hamm et al.	6,551,337 B1	4/2003	Rabiner et al.
5,569,197 A	10/1996	Helmus et al.	6,554,801 B1	4/2003	Steward et al.
5,571,086 A	11/1996	Kaplan et al.	6,562,021 B1	5/2003	Derbin et al.
5,588,432 A	12/1996	Crowley	6,582,392 B1	6/2003	Bennett et al.
			6,589,182 B1	7/2003	Lofman et al.
			6,599,288 B2	7/2003	Maguire et al.

6,607,502 B1 8/2003 Maguire et al.
 6,647,755 B2 11/2003 Rabiner et al.
 6,652,547 B2 11/2003 Rabiner et al.
 6,660,013 B2 12/2003 Rabiner et al.
 6,663,613 B1 12/2003 Evans et al.
 6,676,626 B1 1/2004 Bennett et al.
 6,692,494 B1 2/2004 Cooper et al.
 6,711,953 B2 3/2004 Hayashi et al.
 6,723,063 B1 4/2004 Zhang et al.
 6,740,040 B1 5/2004 Mandrusov et al.
 6,824,515 B2 11/2004 Suorsa et al.
 6,855,123 B2 2/2005 Nita
 6,979,293 B2 12/2005 Hansmann
 7,089,063 B2 8/2006 Lesh et al.
 2001/0037106 A1 11/2001 Shaddock
 2001/0041880 A1 11/2001 Briskin et al.
 2001/0047141 A1 11/2001 McKenzie et al.
 2002/0000763 A1 1/2002 Jones
 2002/0032394 A1 3/2002 Briskin et al.
 2002/0055747 A1 5/2002 Cano et al.
 2002/0087083 A1 7/2002 Nix et al.
 2002/0099292 A1 7/2002 Briskin et al.
 2002/0151825 A1 10/2002 Rubenchik et al.
 2002/0188276 A1 12/2002 Evans et al.
 2003/0023261 A1 1/2003 Tomaschko et al.
 2003/0028173 A1 2/2003 Forsberg
 2003/0036705 A1 2/2003 Hare et al.
 2003/0040698 A1 2/2003 Makin et al.
 2003/0109812 A1 6/2003 Corl et al.
 2003/0114878 A1 6/2003 Diederich et al.

2003/0236539 A1 12/2003 Rabiner et al.
 2004/0039311 A1 2/2004 Nita et al.
 2004/0068189 A1 4/2004 Wilson et al.

FOREIGN PATENT DOCUMENTS

EP 0746245 12/1988
 EP 0668052 8/1995
 EP 0774232 5/1997
 EP 1090658 A1 4/2001
 EP 1103281 A2 5/2001
 JP 2180275 7/1990
 JP H02-180275 7/1990
 WO WO 89/04142 5/1989
 WO WO 95/01751 1/1995
 WO WO 95/26777 12/1995
 WO WO 96/29935 3/1996
 WO WO 97/19645 5/1997
 WO WO 98/18391 5/1998
 WO WO 98/48711 11/1998
 WO WO 98/56462 12/1998
 WO WO 01/13357 2/2001
 WO WO 01/54754 A1 8/2001
 WO WO 03/051208 A1 6/2003

OTHER PUBLICATIONS

Lee et al.; "Arrays of Multielement Ultrasound Applications for Interstitial Hyperthermia"; IEEE Transactions on Biomedical Engineering; vol. 46, No. 7, Jul. 1999.
 PCT International Search Report; PCT/US02/38528.
 The International Search Report for PCT/US03/06462.

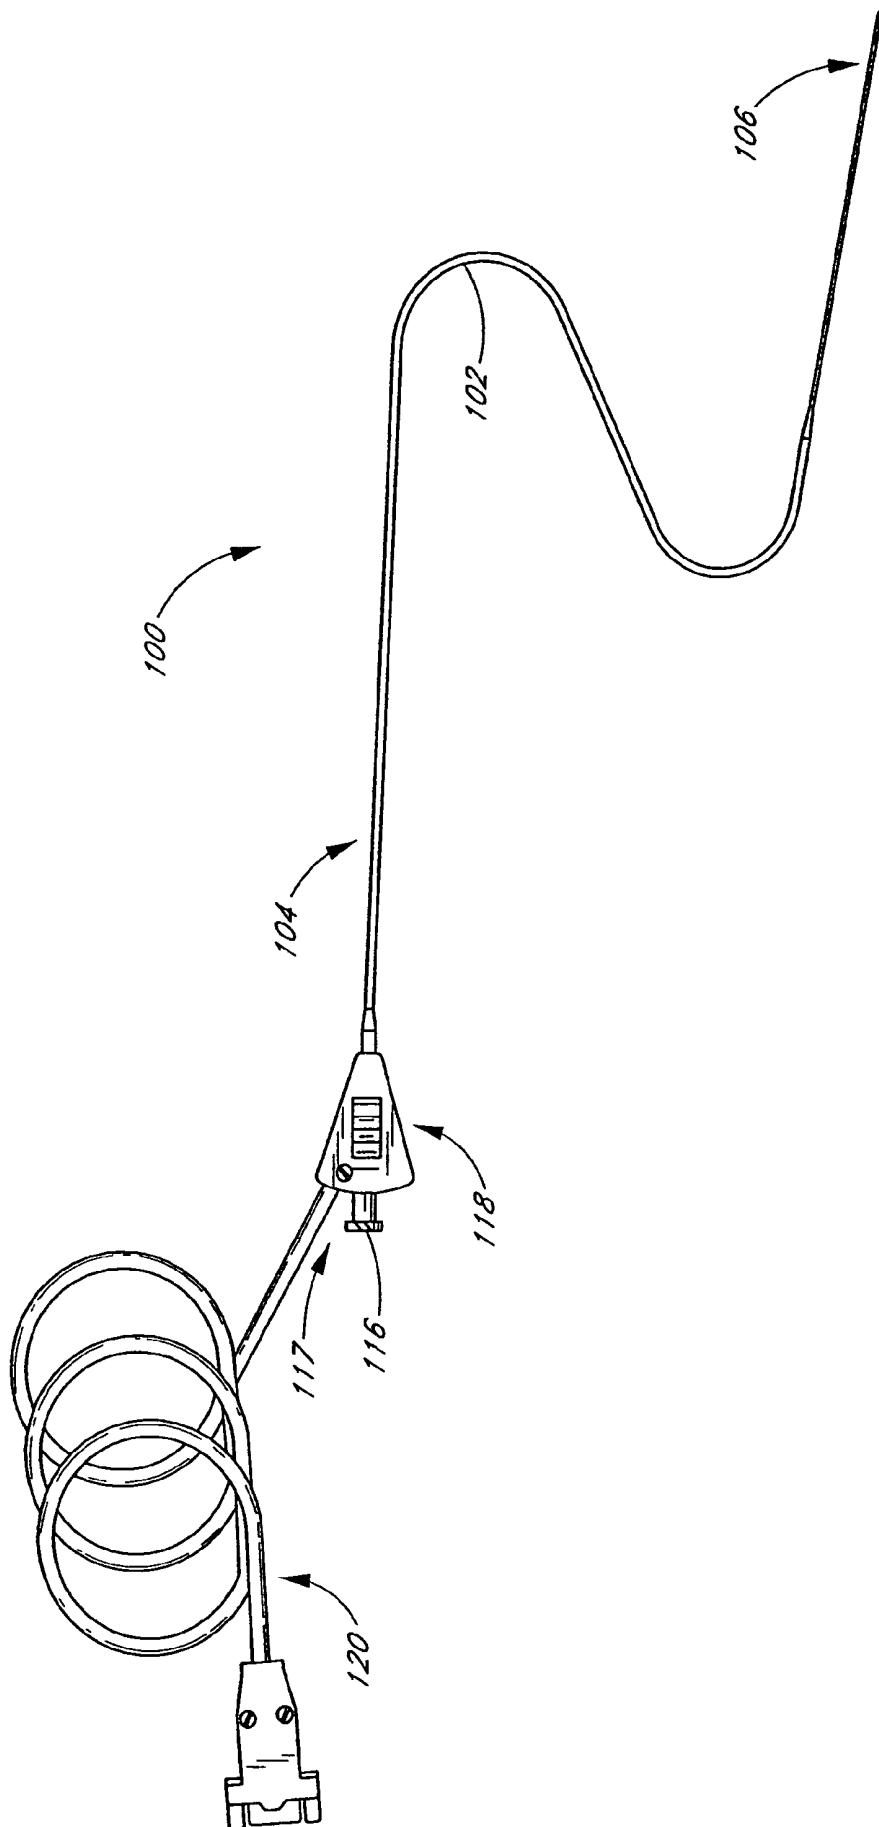


FIG. 1

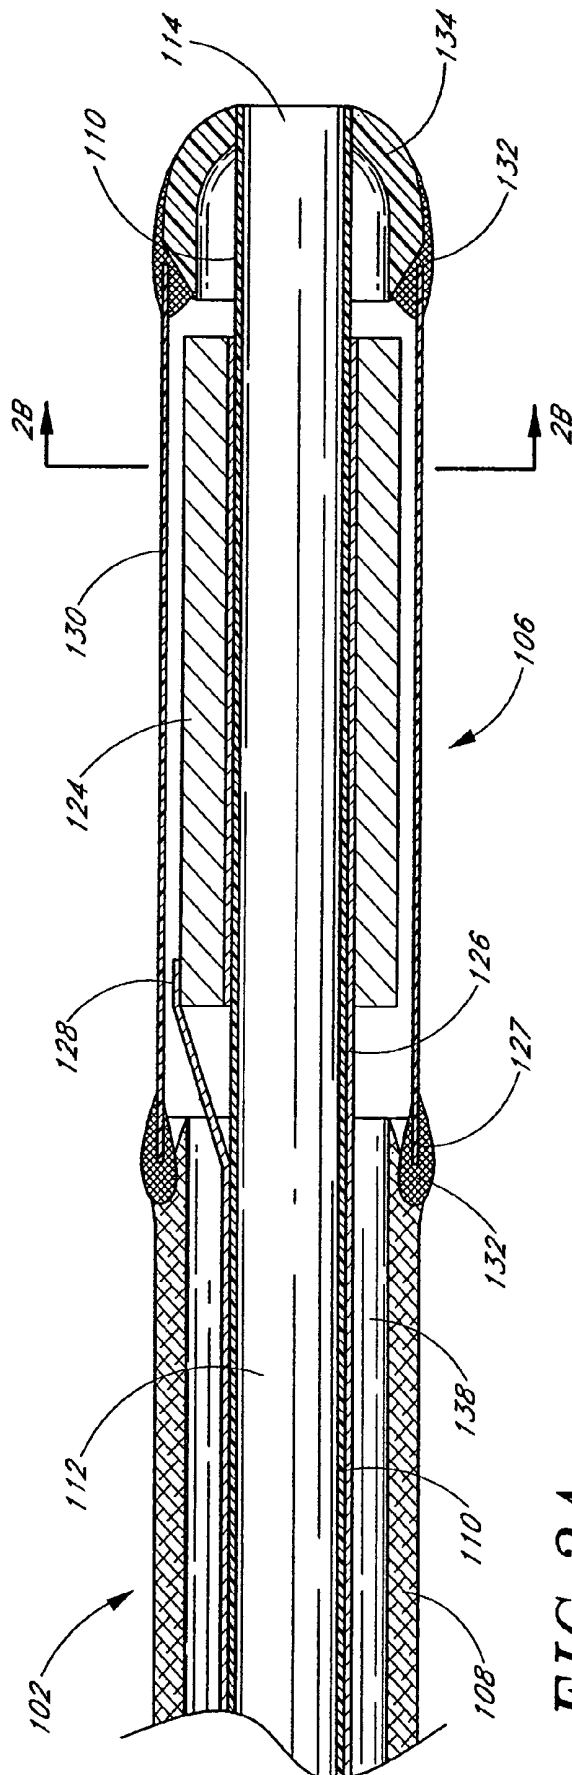


FIG. 2A

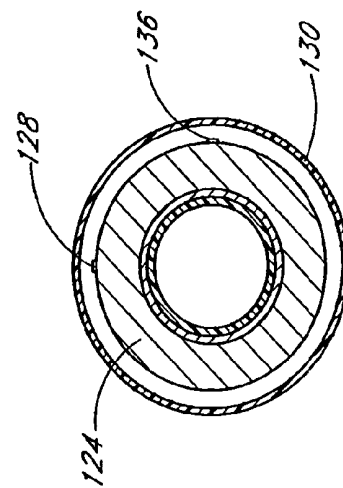


FIG. 2B

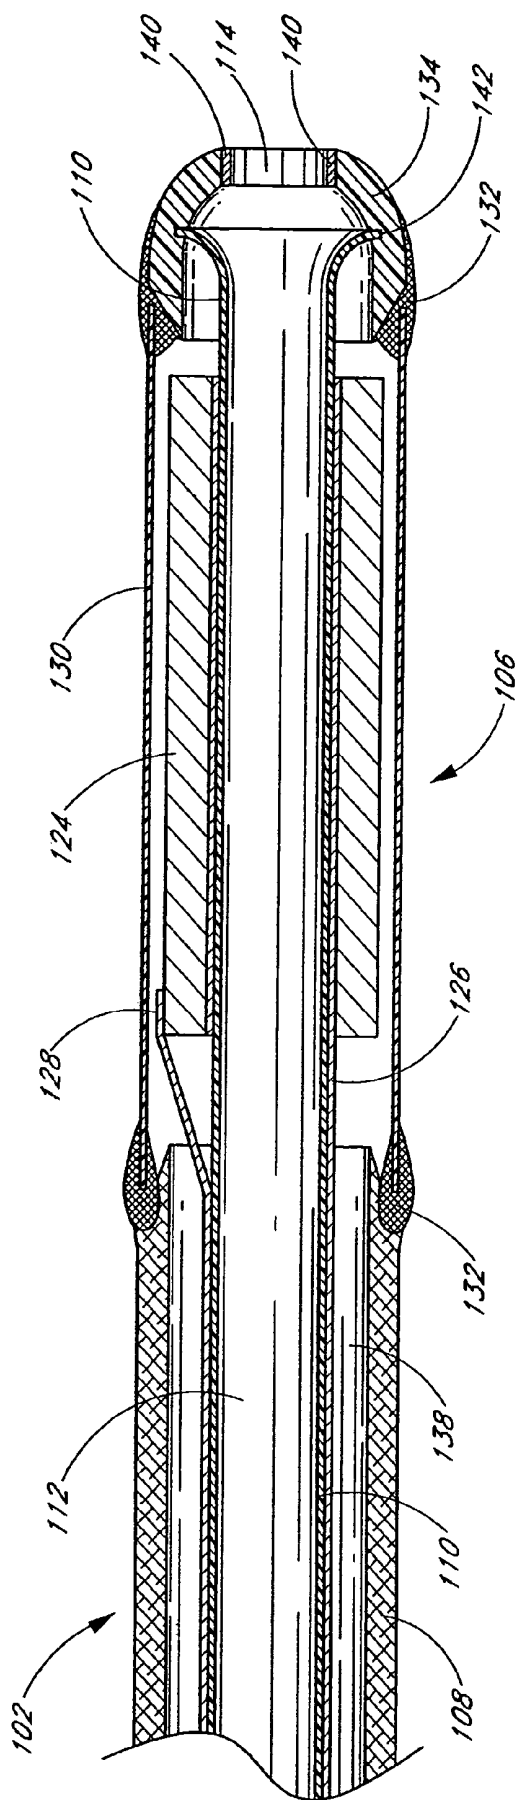


FIG. 3

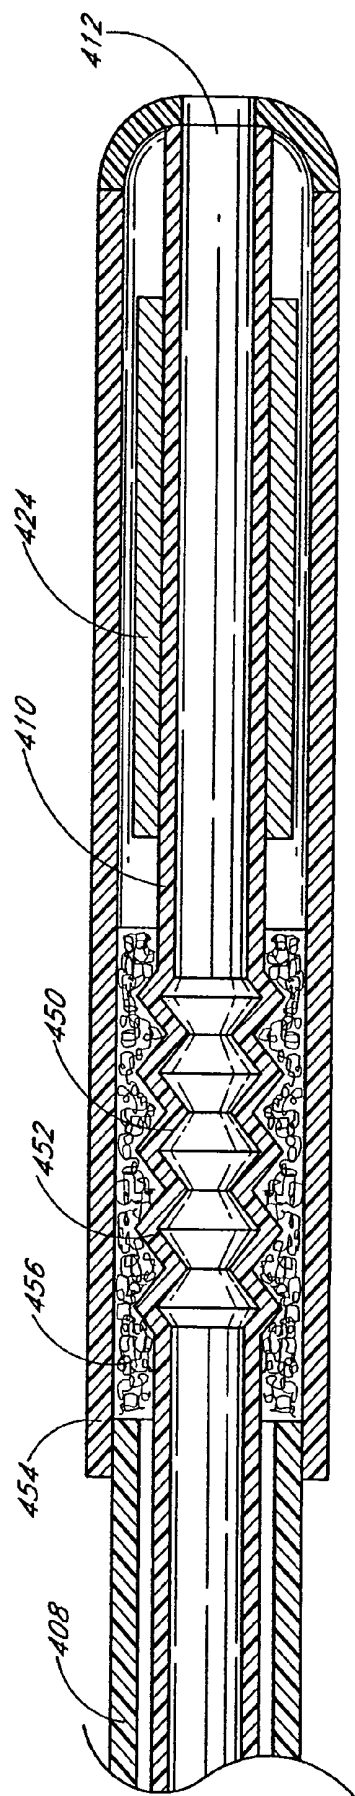


FIG. 4

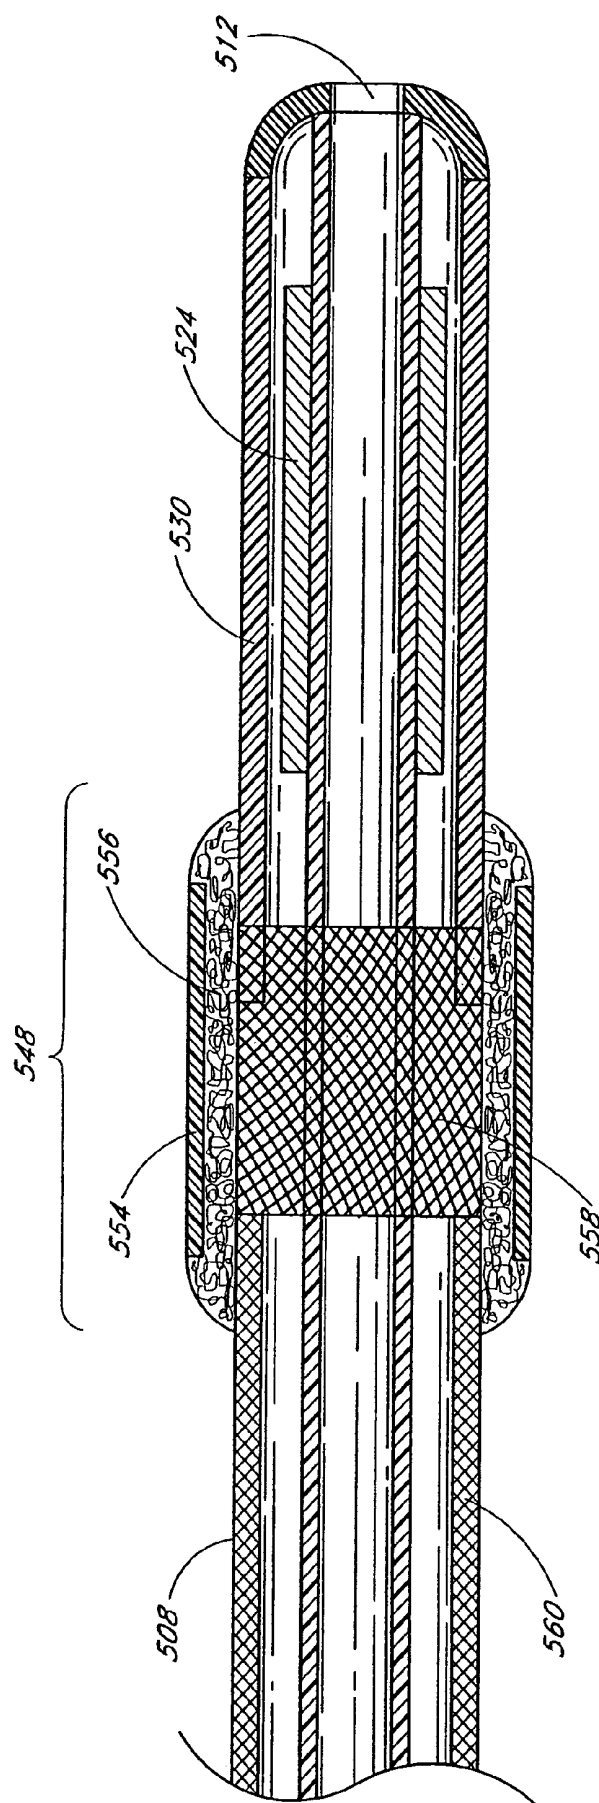


FIG. 5

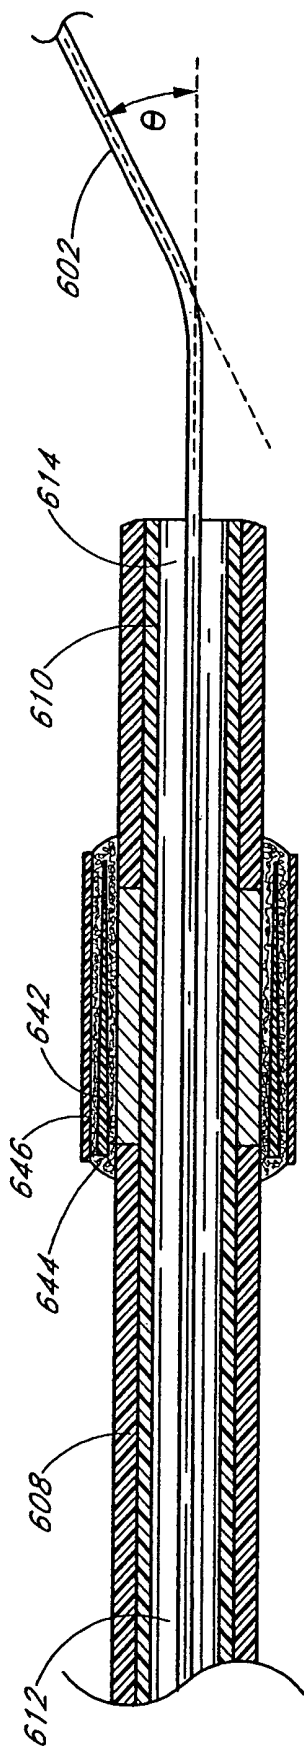


FIG. 6A

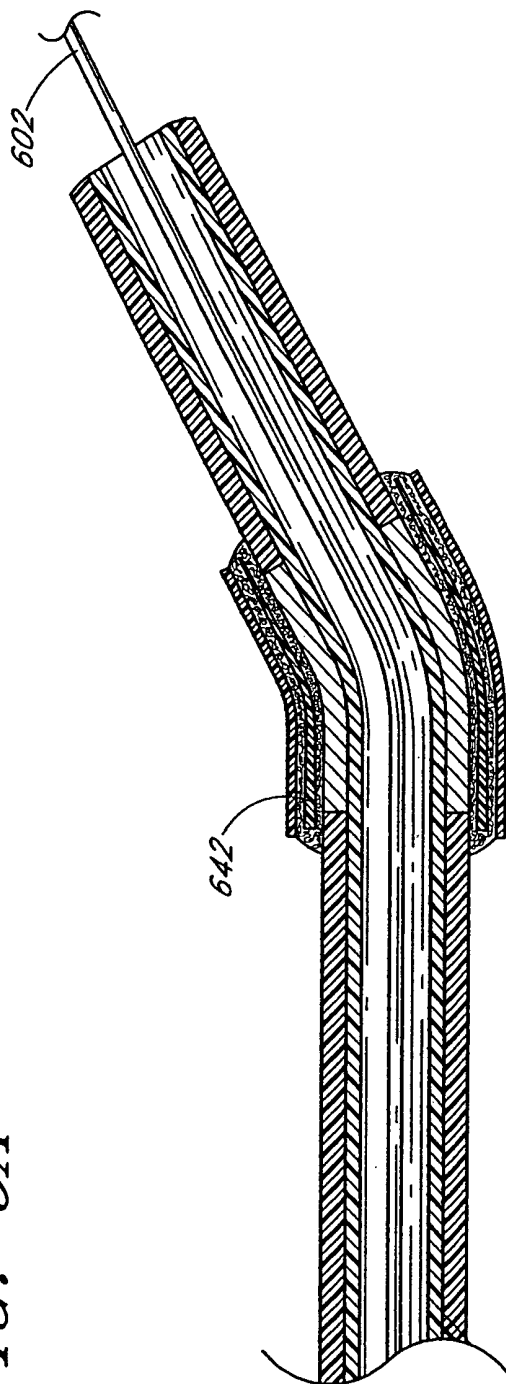


FIG. 6B

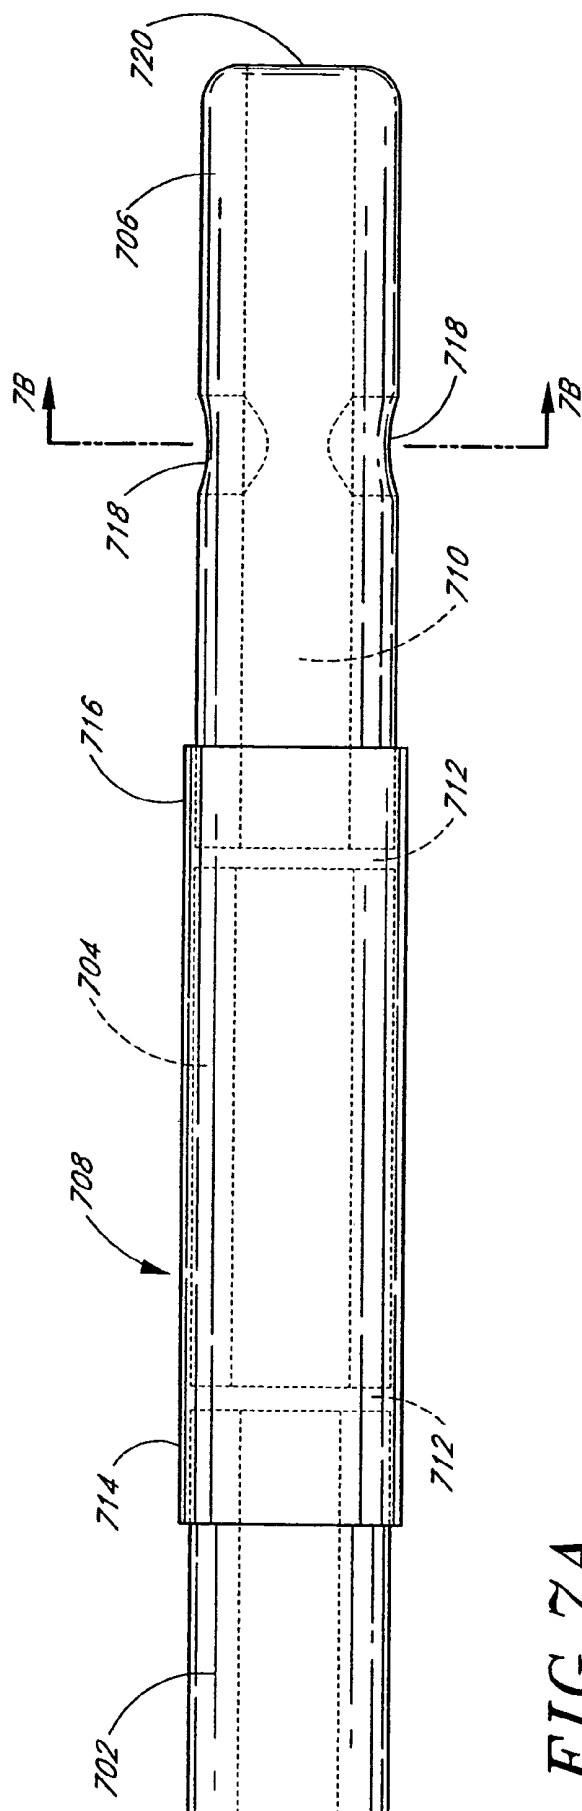


FIG. 7A

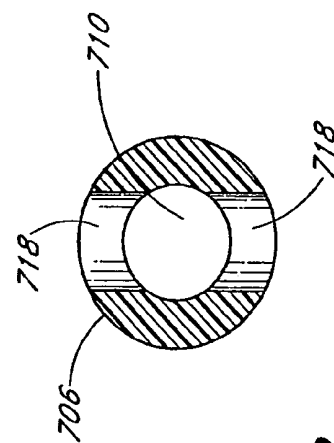


FIG. 7B

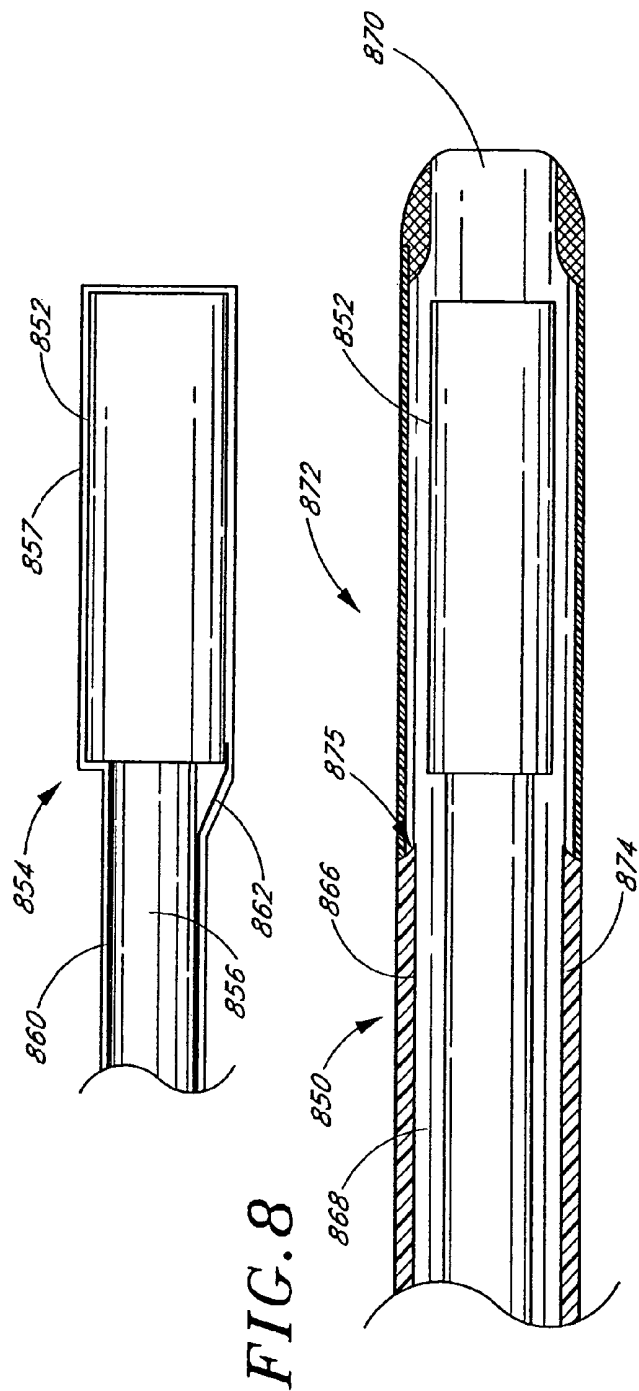


FIG. 8

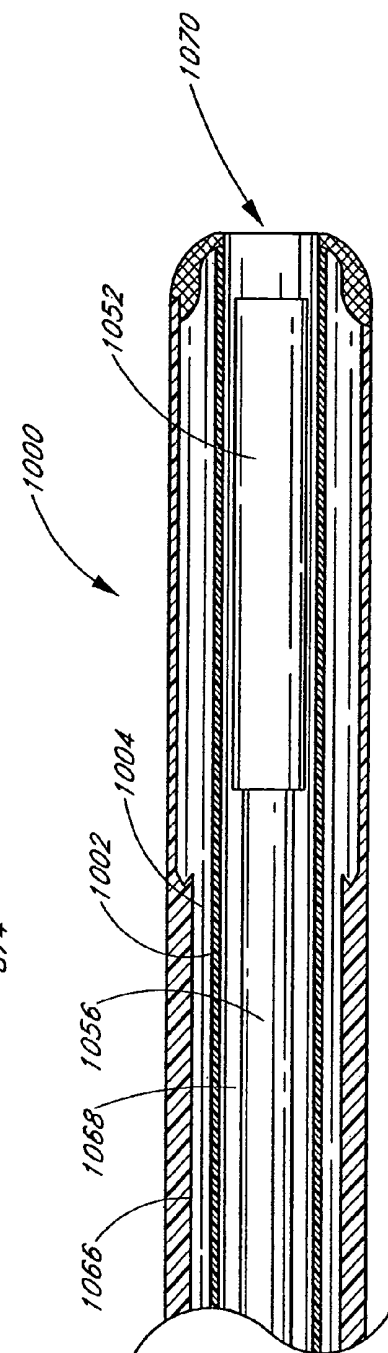
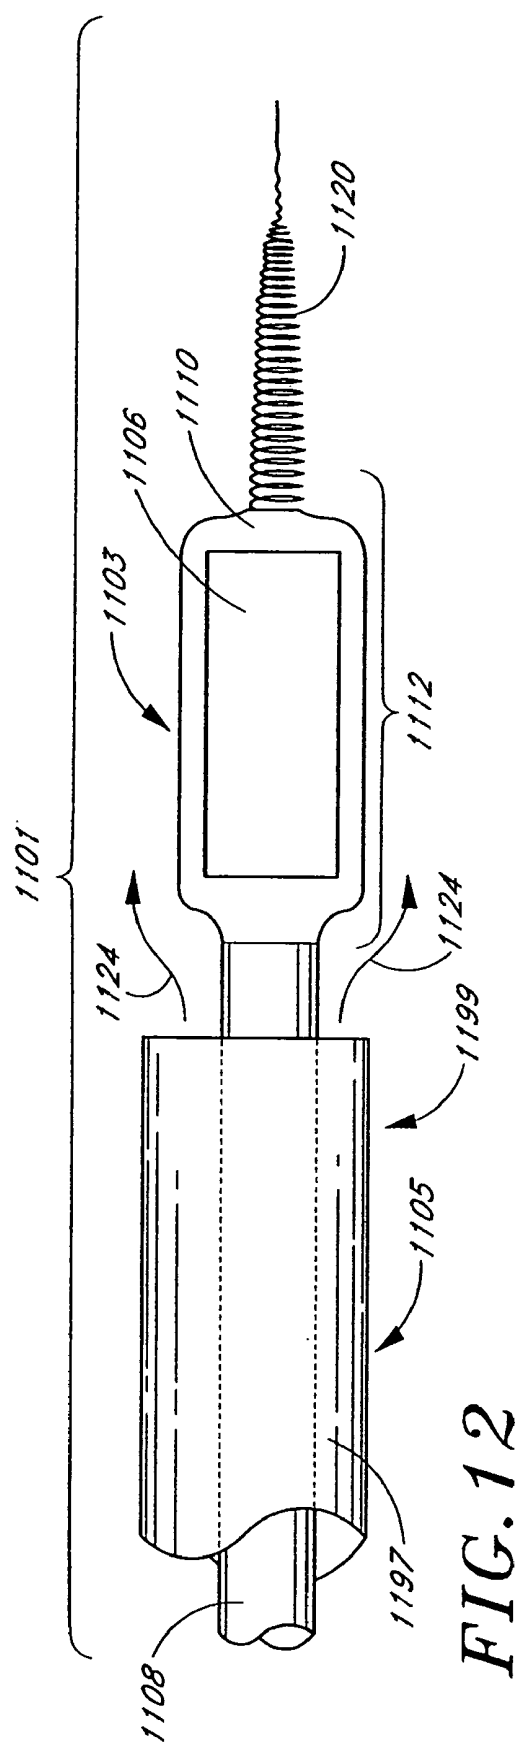
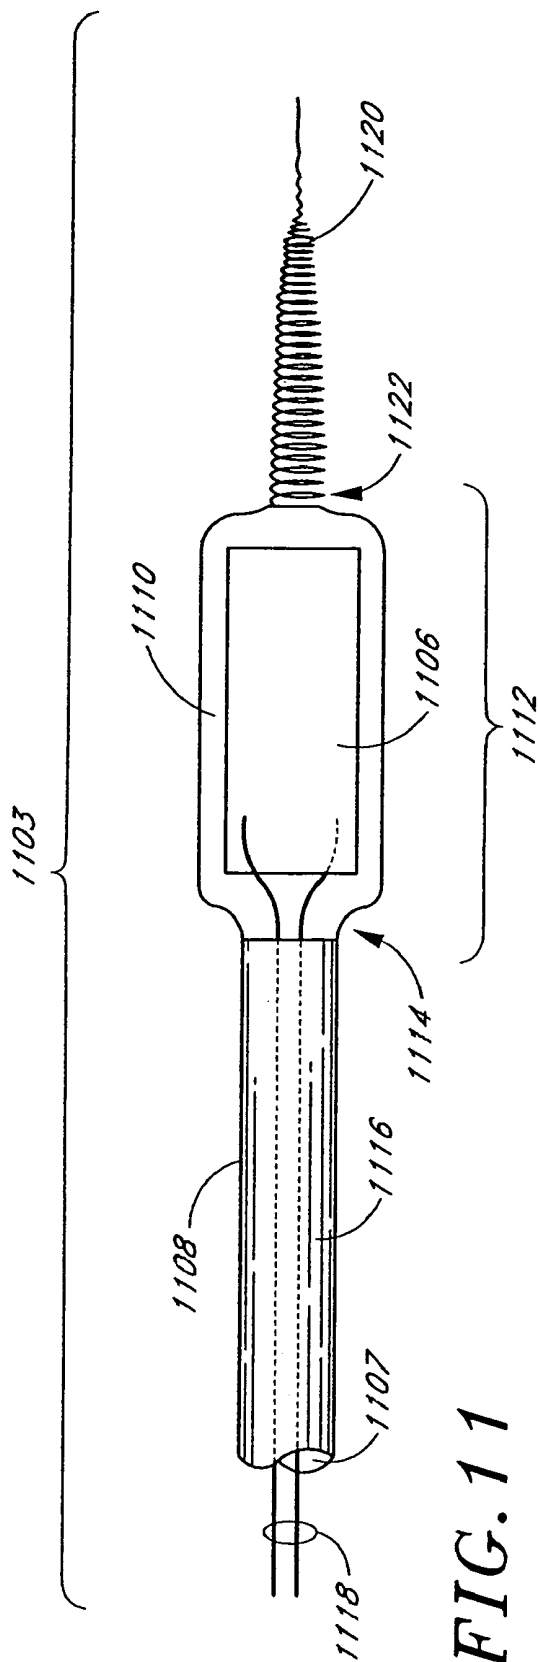


FIG. 9

FIG. 10



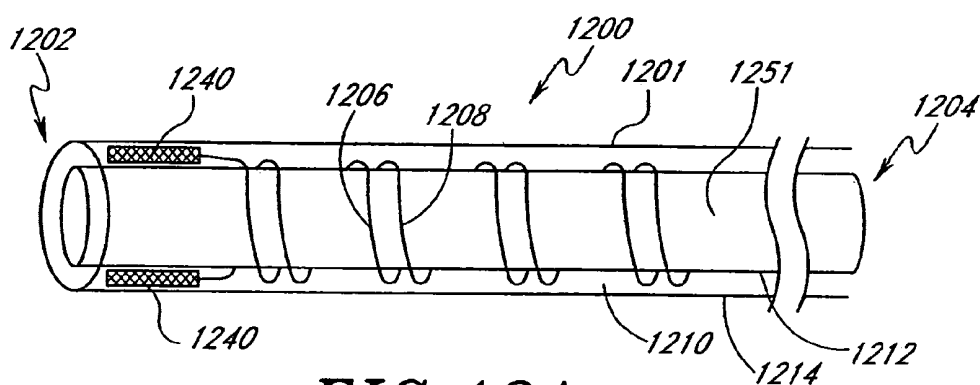


FIG. 13A

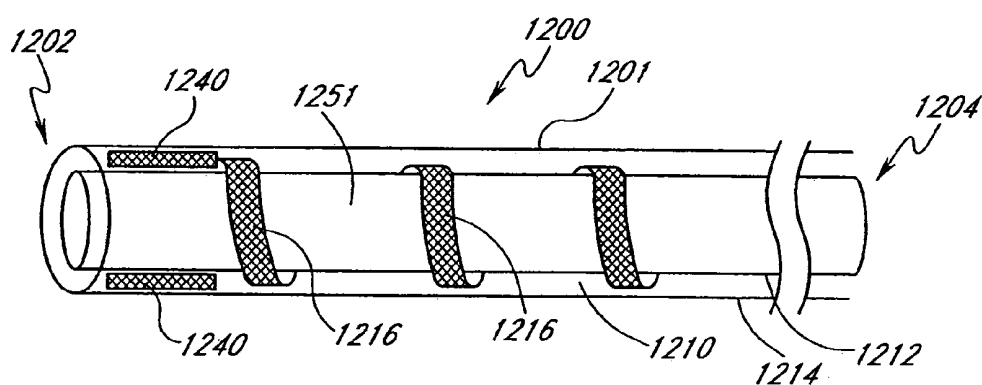


FIG. 13B

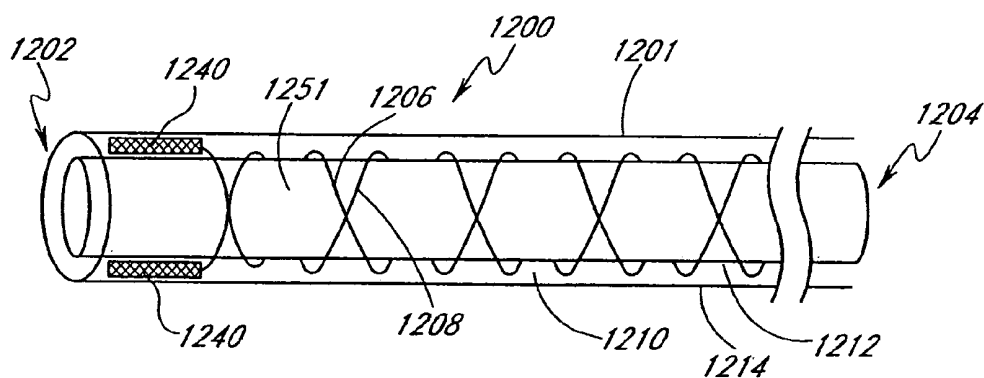


FIG. 14

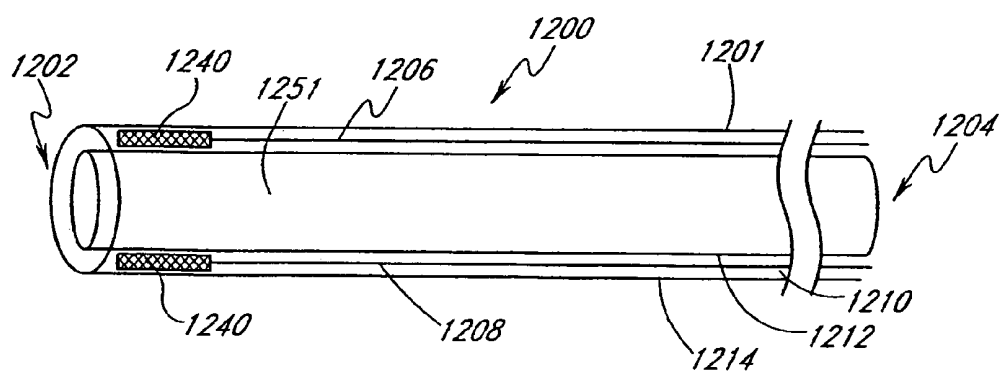


FIG. 15

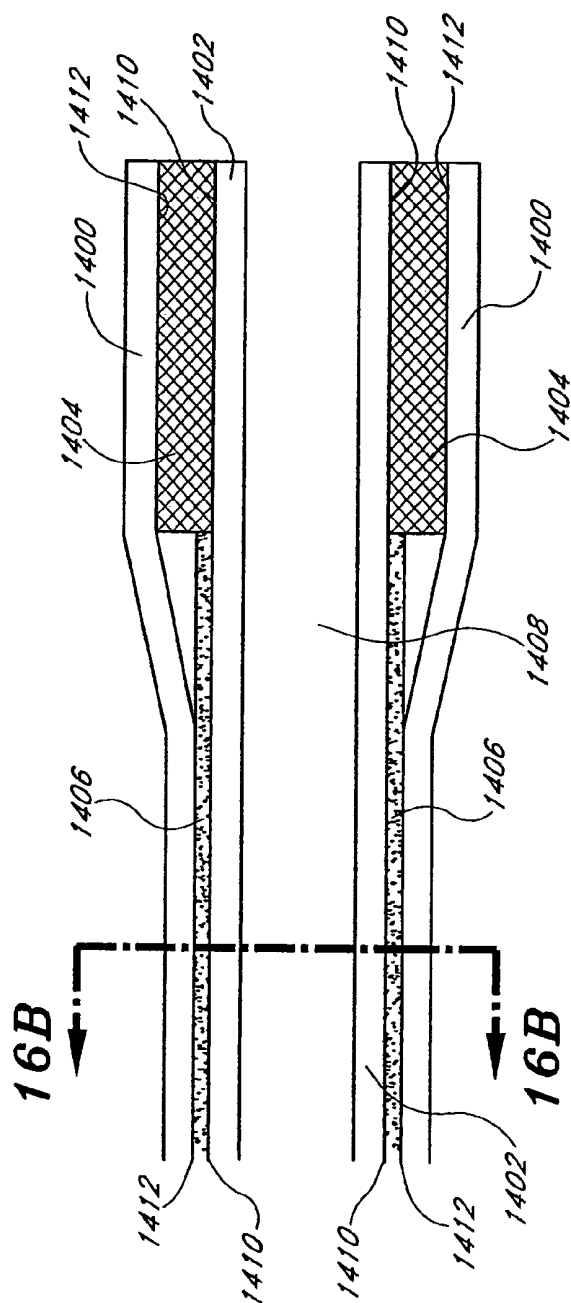


FIG. 16A

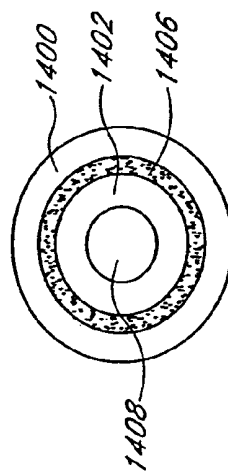


FIG. 16B

METHOD OF MANUFACTURING ULTRASOUND CATHETERS

PRIORITY INFORMATION

This application is a divisional of U.S. patent Ser. No. 10/378,032, filed Feb. 28, 2003 now abandoned, which claims priority under 35 U.S.C. §119(e) from U.S. Provisional Patent Application Ser. No. 60/361,341, entitled "Small Vessel Catheter with Embedded Conductors" and filed Feb. 28, 2002 and is a continuation-in-part of U.S. patent application Ser. No. 10/309,417, entitled "Small Vessel Ultrasonic Catheter" and filed Dec. 3, 2002 now U.S. Pat. No. 7,384,407, the entire contents of these applications are hereby incorporated by reference.

FIELD OF THE INVENTION

The present invention relates to a catheter having an ultrasound assembly useful for delivering ultrasound energy at a treatment site in a body. The apparatus is particularly well suited for delivering ultrasound energy at a treatment site located within a small blood vessel in the distal anatomy.

BACKGROUND OF THE INVENTION

Several therapeutic and diagnostic applications use ultrasound energy. For example, ultrasound energy can be used to enhance the delivery and therapeutic effect of various therapeutic compounds. See e.g., U.S. Pat. Nos. 4,821,740, 4,953,565 and 5,007,438, the entire disclosure of which is hereby incorporated by reference herein. In some applications, it is desirable to use an ultrasound catheter to deliver the ultrasound energy and/or therapeutic compound to a specific treatment site in the body. Such an ultrasound catheter typically comprises an elongate member configured for advancement through a patient's vasculature. An ultrasound assembly is mounted along the distal end portion of the elongate member and is adapted for emitting ultrasound energy. The ultrasound catheter may include a delivery lumen for delivering the therapeutic compound to the treatment site. In this manner, the ultrasound energy can be emitted at the treatment site to enhance the desired therapeutic effects and/or delivery of the therapeutic compound.

In one particular application, ultrasound catheters have been successfully used to treat human blood vessels that have become occluded by plaque, thrombi, emboli or other substances that reduce the blood carrying capacity of the vessel. See e.g., U.S. Pat. No. 6,001,069, the entire disclosure of which is hereby incorporated by reference herein. To remove the blockage, the ultrasound catheter is advanced through the patient's vasculature to deliver solutions containing dissolution compounds directly to the blockage site. To enhance the therapeutic effects of the dissolution compound, ultrasound energy is emitted into the compound and/or the surrounding tissue.

In another application, ultrasound catheters may be used to perform gene therapy on an isolated region of a blood vessel or other body lumen. For example, as disclosed in U.S. Pat. No. 6,135,976, the entire disclosure of which is hereby incorporated by reference herein, an ultrasound catheter can be provided with one or more expandable members for occluding a section of the body lumen at a treatment site. A gene therapy composition is delivered to the treatment site through the delivery lumen of the catheter. The ultrasound assembly is used to emit ultrasound energy at the treatment site to enhance the entry of the gene composition into the cells in the body lumen.

In addition to the applications discussed above, ultrasound catheters may be used for a wide variety of other purposes, such as, for example, delivering and activating light activated drugs with ultrasound energy (see e.g., U.S. Pat. No. 6,176,842, the entire disclosure of which is hereby incorporated by reference herein).

Over the years, numerous types of ultrasound catheters have been proposed for various therapeutic purposes. However, none of the existing ultrasound catheters is well adapted for effective use within small blood vessels in the distal anatomy. For example, in one primary shortcoming, the region of the catheter on which the ultrasound assembly is located (typically along the distal end portion) is relatively rigid and therefore lacks the flexibility necessary for navigation through difficult regions of the distal anatomy. Furthermore, it has been found that it is very difficult to manufacture an ultrasound catheter having a sufficiently small diameter for use in small vessels while providing adequate pushability and torqueability. Still further, it has been found that the distal tip of an ultrasound catheter can easily damage the fragile vessels of the distal anatomy during advancement through the patient's vasculature.

Accordingly, an urgent need exists for an improved ultrasound catheter that is capable of safely and effectively navigating small blood vessels. It is also desirable that such a device be capable of delivering adequate ultrasound energy to achieve the desired therapeutic purpose. It is also desirable that such a device be capable of accessing a treatment site in fragile distal vessels in a manner that is safe for the patient and that is not unduly cumbersome. The present invention addresses these needs.

SUMMARY OF THE INVENTION

In accordance with the foregoing, it is desired to provide an ultrasound catheter having increased flexibility and maneuverability. Such features are advantageous when a treatment is to be performed in the peripheral vasculature, and are especially advantageous when a treatment is to be performed in small vessels, such as in the neurovascular system.

As such, according to one embodiment of the present invention, an ultrasound catheter comprises an elongate tubular body. The elongate tubular body has a proximal region and a distal region opposite the proximal region. The tubular body defines a central lumen having a central lumen diameter. The ultrasound catheter further comprises an elongate, hollow inner core extending through the central lumen. The elongate, hollow inner core has an inner core outer diameter that is less than or equal to the central lumen diameter. The ultrasound catheter further comprises an ultrasound radiating member positioned within the distal region of the tubular body and between the tubular body and the inner core. The ultrasound catheter further comprises at least two electrical conductors extending between the tubular body proximal region and the tubular body distal region. The at least two electrical conductors are positioned between the tubular body and the inner core. The at least two electrical conductors are electrically connected to the ultrasound radiating member. The at least two electrical conductors are wrapped around the inner core a plurality of times in a region between the ultrasound radiating member and the tubular body proximal region.

According to another embodiment of the present invention, an ultrasound catheter comprises an elongate tubular body. The elongate tubular body has a proximal region and a distal region opposite the proximal region. The tubular body defines a central lumen having a central lumen diameter. The ultrasound catheter further comprises an elongate, hollow inner

core extending through the central lumen. The elongate, hollow inner core has an inner core outer diameter that is less than or equal to the central lumen diameter. The ultrasound catheter further comprises an ultrasound radiating member positioned within the distal region of the tubular body and between the tubular body and the inner core. The ultrasound catheter further comprises at least two electrical conductors extending between the tubular body proximal region and the tubular body distal region. The at least two electrical conductors are positioned between the tubular body and the inner core. The at least two electrical conductors are electrically connected to the ultrasound radiating member. The at least two electrical conductors are disposed substantially parallel to a catheter axis in a region between the ultrasound radiating member and the tubular body proximal region.

According to another embodiment of the present invention, an apparatus comprises an elongate, hollow body. The elongate, hollow body has a proximal region, a distal region opposite the proximal region, a body thickness, and an inner lumen. The apparatus further comprises an ultrasound radiating member positioned within the body thickness of the elongate, hollow body. The apparatus further comprises a plurality of elongate electrical conductors extending between the elongate, hollow body proximal region and the ultrasound radiating member. The plurality of elongate electrical conductors are positioned within the body thickness of the elongate, hollow body.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a side view of an ultrasound catheter that is particularly well suited for insertion into small blood vessels of the human body.

FIG. 2A is a cross-sectional view of a distal end of the ultrasound catheter of FIG. 1.

FIG. 2B is a cross-sectional view of the ultrasound catheter taken through line 2B-2B of FIG. 2A.

FIG. 3 is an alternative embodiment of the ultrasound catheter including a stiffener at the distal tip.

FIG. 4 is a cross-sectional view of the distal end of an ultrasound catheter wherein a portion of the inner core has a corrugated configuration for enhanced flexibility.

FIG. 5 is a cross-sectional view of the distal end of an ultrasound catheter wherein the proximal joint comprises braided sections for enhanced flexibility.

FIG. 6A is a cross-sectional view of the distal end of an ultrasound catheter including a bendable wire adapted for providing a shapeable tip.

FIG. 6B is a cross-sectional view of the embodiment of FIG. 6A with the shapeable tip pre-formed to facilitate advancement over a guidewire.

FIG. 7A is a top view of the distal end of an ultrasound catheter having a soft tip assembly.

FIG. 7B is a cross-sectional view of the soft tip assembly taken through line 7B-7B of FIG. 7A.

FIG. 8 is a side view an ultrasound element attached to the distal end of a guidewire.

FIG. 9 is a cross-sectional view of an ultrasound catheter used with the ultrasound element and guidewire of FIG. 8.

FIG. 10 is a cross-sectional view of a distal end of another modified embodiment of an ultrasound catheter that can be used with the ultrasound element and guidewire of FIG. 8.

FIG. 11 is a side view of a distal end of a treatment wire wherein an ultrasound element is provided along the distal end of a hypotube.

FIG. 12 is a side view of a distal end of an ultrasound catheter that incorporates the treatment wire of FIG. 11.

FIG. 13A is a partial cutaway view of one embodiment of an ultrasound catheter with embedded conductive wires that are spirally wrapped parallel to each other.

FIG. 13B is a partial cutaway view of one embodiment of an ultrasound catheter with embedded conductive wires that are spirally wrapped into a unitary cable.

FIG. 14 is a partial cutaway view of one embodiment of an ultrasound catheter with embedded conductive wires that are spirally wrapped in a nonparallel configuration.

FIG. 15 is a partial cutaway view of one embodiment of an ultrasound catheter with embedded conductive wires that are disposed substantially parallel to the catheter axis.

FIG. 16A illustrates a longitudinal cross-sectional view of an ultrasound catheter having internal surfaces that are electrically conductive.

FIG. 16B illustrates a cross-sectional view of the ultrasound catheter of FIG. 16A taken along line 16B-16B.

DETAILED DESCRIPTION OF PREFERRED EMBODIMENTS

The advancement of an ultrasound catheter through a blood vessel to a treatment site can be difficult and dangerous, particularly when the treatment site is located within a small vessel in the distal region of a patient's vasculature. To reach the treatment site, it is often necessary to navigate a tortuous path around difficult bends and turns. During advancement through the vasculature, bending resistance along the distal end portion of the catheter can severely limit the ability of the catheter to make the necessary turns. Moreover, as the catheter is advanced, the distal tip of the catheter is often in contact with the inner wall of the blood vessel. The stiffness and rigidity of the distal tip of the catheter may lead to significant trauma or damage to the tissue along the inner wall of the blood vessel. As a result, advancement of an ultrasound catheter through small blood vessels can be extremely hazardous. Therefore, a need exists for an improved ultrasound catheter design that allows a physician to more easily navigate difficult turns in small blood vessels while minimizing trauma and/or damage along the inner walls of the blood vessels.

To address this need, preferred embodiments of the present invention described herein provide an ultrasound catheter that is well suited for use in the treatment of small blood vessels or other body lumens having a small inner diameter. The ultrasound catheter can be used to enhance the therapeutic effects of drugs, medication and other pharmacological agents at a treatment site within the body. See e.g., U.S. Pat. Nos. 5,318, 014, 5,362,309, 5,474,531, 5,628,728, 6,001,069, and 6,210, 356. Certain preferred embodiments of the ultrasound catheter are particularly well suited for use in the treatment of thrombotic occlusions in small blood vessels, such as, for example, the cerebral arteries. In addition, preferred embodiments may also find utility in other therapeutic applications, such as, for example, performing gene therapy (see e.g., U.S. Pat. No. 6,135,976), activating light activated drugs for producing targeted tissue death (see e.g., U.S. Pat. No. 6,176, 842) and causing cavitation to produce various desirable biological effects (see e.g., U.S. Pat. No. RE36,939). Moreover, such therapeutic applications may be used in wide variety of locations within the body, such as, for example, in other parts of the circulatory system, solid tissues, duct systems and body cavities. It is also anticipated that the ultrasound catheters disclosed herein, and variations thereof, may find utility in other medical applications, such as, for example, diagnostic and imaging applications.

Ultrasound catheters and methods disclosed herein, and similar variations thereof, may also be useful for applications wherein the ultrasound energy provides a therapeutic effect by itself. For example, ultrasound energy may be effective for uses such as preventing and/or reducing stenosis and/or restenosis, tissue ablation, abrasion or disruption, promoting temporary or permanent physiological changes in intracellular or intercellular structures, or rupturing micro-balloons or micro-bubbles for drug delivery. See e.g., U.S. Pat. Nos. 5,269,291 and 5,431,663. In addition, the methods and devices disclosed herein may also find utility in applications that do not require the use of a catheter. For example the methods and devices may be used for enhancing hyperthermic drug treatment or using an external ultrasound source to enhance the therapeutic effects of drugs, medication and other pharmacological agents at a specific site within the body or to provide a therapeutic or diagnostic effect by itself. See e.g., U.S. Pat. Nos. 4,821,740, 4,953,565, 5,007,438 and 6,096,000. The entire disclosure of each of the patents mentioned in this paragraph and the previous paragraph is hereby incorporated by reference herein and made a part of this specification.

As used herein, the term "ultrasound energy" is a broad term and is used in its ordinary sense and means, without limitation, mechanical energy transferred through pressure or compression waves with a frequency greater than about 20 KHz. In one embodiment, the waves of the ultrasound energy have a frequency between about 500 KHz and 20 MHz and in another embodiment between about 1 MHz and 3 MHz. In yet another embodiment, the waves of the ultrasound energy have a frequency of about 3 MHz.

As used herein, the term "catheter" is a broad term and is used in its ordinary sense and means, without limitation, an elongate flexible tube configured to be inserted into the body of a patient, such as, for example, a body cavity, duct or vessel.

Preferred Features of an Ultrasound Catheter

Referring now to FIGS. 1 through 2B, for purposes of illustration, preferred embodiments of the present invention provide an ultrasound catheter 100 that is particularly well suited for use within small vessels of the distal anatomy, such as, for example, in the remote, small diameter, neurovasculature in the brain.

As shown in FIG. 1 and 2A, the ultrasound catheter 100 generally comprises a multi-component tubular body 102 having a proximal end 104 and a distal end 106. The tubular body 102 and other components of the catheter 100 can be manufactured in accordance with any of a variety of techniques well known in the catheter manufacturing field. As discussed in more detail below, suitable material dimensions can be readily selected taking into account the natural and anatomical dimensions of the treatment site and of the desired percutaneous access site.

Preferably, the tubular body 102 can be divided into at least three sections of varying stiffness. The first section, which preferably includes the proximal end 104, is generally more stiff than a second section, which lies between the proximal end 104 and the distal end 106 of the catheter. This arrangement facilitates the movement and placement of the catheter 102 within small vessels. The third section, which includes ultrasound radiating element 124, is generally stiffer than the second section due to the presence of the ultrasound radiating element 124.

In each of the embodiments described herein, the assembled ultrasound catheter preferably has sufficient struc-

tural integrity, or "pushability," to permit the catheter to be advanced through a patient's vasculature to a treatment site without buckling or kinking. In addition, the catheter has the ability to transmit torque, such that the distal portion can be rotated into a desired orientation after insertion into a patient by applying torque to the proximal end.

The elongate flexible tubular body 102 comprises an outer sheath 108 (see FIG. 2A) that is positioned upon an inner core 110. In an embodiment particularly well suited for small vessels, the outer sheath 108 comprises extruded PEBAX, PTFE, PEEK, PE, polyimides, braided polyimides and/or other similar materials. The distal end portion of the outer sheath 108 is adapted for advancement through vessels having a very small diameter, such as those in the neurovasculature of the brain. Preferably, the distal end portion of the outer sheath 108 has an outer diameter between about 2 and 5 French. More preferably, the distal end portion of the outer sheath 108 has an outer diameter of about 2.8 French. In one preferred embodiment, the outer sheath 108 has an axial length of approximately 150 centimeters.

In other embodiments, the outer sheath 108 can be formed from a braided tubing formed of, by way of example, high or low density polyethylenes, urethanes, nylons, etc. Such an embodiment enhances the flexibility of the tubular body 102. For enhanced pushability and torqueability, the outer sheath 108 may be formed with a variable stiffness from the proximal to the distal end. To achieve this, a stiffening member may be included along the proximal end of the tubular body 102.

The inner core 110 defines, at least in part, a delivery lumen 112, which preferably extends longitudinally along the entire length of the catheter 100. The delivery lumen 112 has a distal exit port 114 and a proximal axis port 116. Referring again to FIG. 1, the proximal access port 116 is defined by drug inlet port 117 of a back end hub 118, which is attached to the proximal end 104 of the outer sheath 108. The illustrated back end hub 118 is preferably attached to a control box connector 120, the utility of which will be described in more detail below.

The delivery lumen 112 is preferably configured to receive a guide wire (not shown). Preferably, the guidewire has a diameter of approximately 0.008 to 0.012 inches. More preferably, the guidewire has a diameter of about 0.010 inches. The inner core 110 is preferably formed from polyimide or a similar material which, in some embodiments, can be braided to increase the flexibility of the tubular body 102.

With particular reference to FIGS. 2A and 2B, the distal end 106 of the catheter 102 preferably includes the ultrasound radiating element 124. In the illustrated embodiment, the ultrasound radiating element 124 comprises an ultrasound transducer, which converts, for example, electrical energy into ultrasound energy. In a modified embodiment, the ultrasound energy can be generated by an ultrasound transducer that is remote from the ultrasound radiating element 124 and the ultrasound energy can be transmitted via, for example, a wire to the ultrasound radiating element 124.

In the embodiment illustrated in FIGS. 2A and 2B, the ultrasound radiating element 124 is configured as a hollow cylinder. As such, the inner core 110 can extend through the lumen of the ultrasound radiating element 124. The ultrasound radiating element 124 can be secured to the inner core 110 in any suitable manner, such as with an adhesive. A potting material may also be used to further secure the mounting of the ultrasound radiating element along the central core.

In other embodiments, the ultrasound radiating element 124 can be configured with a different shape without departing from the scope of the invention. For example, the ultrasound radiating element may take the form of a solid rod, a

disk, a solid rectangle or a thin block. Still further, the ultrasound radiating element **124** may comprise a plurality of smaller ultrasound radiating elements. The illustrated arrangement is the generally preferred configuration because it provides for enhanced cooling of the ultrasound radiating element **124**. For example, in one preferred embodiment, a drug solution can be delivered through the delivery lumen **112**. As the drug solution passes through the lumen of the ultrasound radiating element, the drug solution may advantageously provide a heat sink for removing excess heat generated by the ultrasound radiating element **124**. In another embodiment, a return path can be formed in the space **138** between the outer sheath and the inner core such that coolant from a coolant system can be directed through the space **138**.

The ultrasound radiating element **40** is preferably selected to produce ultrasound energy in a frequency range that is well suited for the particular application. Suitable frequencies of ultrasound energy for the applications described herein include, but are not limited to, from about 20 KHz to about 20 MHz. In one embodiment, the frequency is between about 500 KHz and 20 MHz and in another embodiment from about 1 MHz and about 3 MHz. In yet another embodiment, the ultrasound energy has a frequency of about 3 MHz.

As mentioned above, in the illustrated embodiment, ultrasound energy is generated from electrical power supplied to the ultrasound radiating element **124**. The electrical power can be supplied through the controller box connector **120**, which is connected to a pair of wires **126**, **128** that extend through the catheter body **102**. The electrical wires **126**, **128** can be secured to the inner core **110**, lay along the inner core **110** and/or extend freely in the space between the inner core **110** and the outer sheath **108**. In the illustrated arrangement, the first wire **126** is connected to the hollow center of the ultrasound radiating element **124** while the second wire **128** is connected to the outer periphery of the ultrasound radiating element **124**. The ultrasound radiating element **124** is preferably, but is not limited to, a transducer formed of a piezoelectric ceramic oscillator or a similar material.

With continued reference to FIGS. 2A and 2B, the distal end **104** of the catheter **100** preferably includes a sleeve **130**, which is generally positioned about the ultrasound radiating element **124**. The sleeve **130** is preferably constructed from a material that readily transmits ultrasound energy. Suitable materials for the sleeve **130** include, but are not limited to, polyolefins, polyimides, polyester and other materials having a relatively low impedance to ultrasound energy. Low ultrasound impedance materials are materials that readily transmit ultrasound energy with minimal absorption of the ultrasound energy. The proximal end of the sleeve **130** can be attached to the outer sheath **108** with an adhesive **132**. To improve the bonding of the adhesive **132** to the outer sheath **108**, a shoulder **127** or notch may be formed in the outer sheath for attachment of the adhesive thereto. Preferably, the outer sheath **108** and the sleeve **130** have substantially the same outer diameter.

In a similar manner, the distal end of the sleeve **130** can be attached to a tip **134**. In the illustrated arrangement, the tip **134** is also attached to the distal end of the inner core **110**. Preferably, the tip is between about 0.5 and 4.0 millimeters in length. More preferably, the tip is about 2.0 millimeters in length. As illustrated, the tip is preferably rounded in shape to reduce trauma or damage to tissue along the inner wall of a blood vessel or other body structure during advancement toward a treatment site.

With continued reference to FIG. 2B, the catheter **100** preferably includes at least one temperature sensor **136** along the distal end **106**. The temperature sensor **136** is preferably

located on or near the ultrasound radiating element **124**. Suitable temperature sensors include but are not limited to, diodes, thermistors, thermocouples, resistance temperature detectors (RTDs), and fiber optic temperature sensors that used thermochromic liquid crystals. The temperature sensor is preferably operatively connected to a control box (not shown) through a control wire, which extends through the catheter body **102** and back end hub **118** and is operatively connected to a control box through the control box connector **120**. The control box preferably includes a feedback control system having the ability to monitor and control the power, voltage, current and phase supplied to the ultrasound radiating element. In this manner, the temperature along the relevant region of the catheter can be monitored and controlled for optimal performance. Details of the control box can be found in Assignee's co-pending provisional application entitled CONTROL POD FOR ULTRASONIC CATHETER, Application Ser. No. 60/336,630, filed Dec. 3, 2001, which is incorporated by reference in its entirety.

In one exemplary application of the ultrasound catheter **100** described above, the apparatus may be used to remove a thrombotic occlusion from a small blood vessel. In one preferred method of use, a free end of a guidewire is percutaneously inserted into the patient's vasculature at a suitable first puncture site. The guidewire is advanced through the vasculature toward a treatment site wherein the blood vessel is occluded by the thrombus. The guidewire wire is preferably then directed through the thrombus.

After advancing the guidewire to the treatment site, the catheter **100** is thereafter percutaneously inserted into the vasculature through the first puncture site and is advanced along the guidewire towards the treatment site using traditional over-the-guidewire techniques. The catheter **100** is advanced until the distal end **106** of the catheter **100** is positioned at or within the occlusion. The distal end **106** of the catheter **100** may include one or more radiopaque markers (not shown) to aid in positioning the distal end **106** within the treatment site.

After placing the catheter, the guidewire can then be withdrawn from the delivery lumen **112**. A drug solution source (not shown), such as a syringe with a Luer fitting, is attached to the drug inlet port **117** and the controller box connector **120** is connected to the control box. As such, the drug solution can be delivered through the delivery lumen **112** and out the distal access port **114** to the thrombus. Suitable drug solutions for treating a thrombus include, but are not limited to, an aqueous solution containing Heparin, Urokinase, Streptokinase, and/or tissue Plasminogen Activator (TPA).

The ultrasound radiating element **124** is activated to emit ultrasound energy from the distal end **106** of the catheter **100**. As mentioned above, suitable frequencies for the ultrasound radiating element **124** include, but are not limited to, from about 20 KHz to about 20 MHz. In one embodiment, the frequency is between about 500 KHz and 20 MHz and in another embodiment between about 1 MHz and 3 MHz. In yet another embodiment, the ultrasound energy is emitted at a frequency of about 3 MHz. The drug solution and ultrasound energy are applied until the thrombus is partially or entirely dissolved. Once the thrombus has been dissolved to the desired degree, the catheter **100** is withdrawn from the treatment site.

Stiffening Component

Referring again to FIG. 2A, because the diameter of the distal exit port **114** is often relatively large compared with the diameter of the guidewire (not shown), a gap may exist

between the inner rim of the tip **134** and the guidewire. If sufficiently large, this gap may cause the tip **134** of the catheter to catch or snag on an object along the exit port **114**. If the tip **134** catches on an object, the exit port **114** may stretch (i.e., increase in diameter) as the catheter is pushed forward. This effect is particularly likely to occur at vessel bifurcations and will hereinafter be referred to as “fish-mouthing.”

FIG. 3 illustrates an embodiment adapted to reduce the likelihood of fish-mouthing wherein a circular stiffening component **140** is provided along the distal tip **134**. The circular stiffening component **140** reduces the gap between the tip **134** and the guidewire, and is preferably made of a stiff material, such as, for example, aluminum, that will prevent the tip **134** from fish-mouthing. Additionally, if the guidewire is formed with a variable diameter, cooperation of the guidewire and the circular stiffening component **140** may be advantageously used as a valve. By adjusting the relative positions of the guidewire and catheter, it is possible to control the delivery of drugs, medications, or other therapeutic compounds through the exit port **114** along the tip **134**. As seen in FIG. 3, this embodiment also includes a variation of the inner core **110A** having a flared end that may be inserted into a circumferential notch **142** formed in the distal tip **134**. Insertion of the flared end into the circumferential notch provides for enhanced structural integrity.

In alternative embodiments, fish-mouthing may be prevented by increasing the thickness of the tip **134**, or by manufacturing the tip **134** using a material with increased stiffness. In such embodiments, the tip **134** will have decreased flexibility, and therefore will be less susceptible to fish-mouthing.

Flexible Joint

Referring again to FIG. 2A, in modified embodiments of the present invention, the rigidity of the catheter along the joint (hereinafter referred to as the “proximal element joint”) between the outer sheath **108** and sleeve **130** may be reduced significantly. The rigidity of the proximal element joint is reduced to further enhance flexibility, prevent kinking of the flexible support section of the catheter, and to facilitate tracking of the catheter over the guidewire.

In such embodiments, the use of an adhesive may be eliminated, and the proximal end of the sleeve **130** may be attached to the outer sheath **108** at the proximal element joint using a direct bonding method adapted to create a more flexible proximal element joint. Examples of such direct bonding methods include, but are not limited to, the use of heat, a solvent, a mold, or a cast. Alternatively, a reflow, or “die wiping” technique may be employed wherein an extruded catheter shaft is covered with a heat shrink tube and heated to reflow and bond the polymers within the catheter shaft. An external heat source may be employed in a reflow technique, or if the catheter includes metal components at the proximal element joint, radio frequency (“RF”) energy may be used to heat and bond the polymers within the catheter shaft.

FIG. 4 illustrates yet another alternative embodiment for reducing the rigidity of the proximal element joint to thereby enhance the flexibility of the ultrasound catheter. As illustrated in FIG. 4, the inner core **410** includes a corrugated portion **452** along the proximal element joint just proximal of the ultrasound radiating element **424**. In such embodiments, a Teflon® liner **450** may be adapted to surround the inner surface of the corrugated portion **452** of the inner core **410** to prevent the guidewire from catching on the corrugations. Additionally, a flexible filler material **456** and a flexible cover sleeve **454** may be adapted to cover the exterior surface of the corrugated portion **452** of the catheter to prevent the catheter

from catching on the interior walls of the vessel anatomy. A corrugated portion **452** of the inner core **410** may be created by placing a close-fitting pin within a portion of the polyimide material used to form the inner core, and applying a compressive force to the polyimide material on either side of the pin. When the pin is removed from the inner core **410**, the corrugated portion **452** of the inner core **410** will have enhanced flexibility and will thereby increase the flexibility of the ultrasound catheter.

In still other embodiments, the rigidity of the proximal element joint may be further reduced by forming the inner core **410** of the delivery lumen **412** of a material with increased flexibility and resistance to kinking. For example, the inner core **410** of the delivery lumen **412** may comprise a Teflon®-lined polyimide shaft. Additionally, a coil or braid may be incorporated into the delivery lumen **412**, thereby further reducing susceptibility to kinking without increasing the rigidity of the catheter.

FIG. 5 illustrates yet another alternative embodiment wherein the rigidity of the proximal element joint **548** is reduced by providing an outer sheath **508** that includes an embedded braid **560**. Furthermore, the outer sheath **508** is attached to the sleeve **530** using a flexible exposed braided portion **558**. A flexible filler material **556** and a flexible cover sleeve **554** are used to bond the outer sheath **508**, the sleeve **530** and the exposed braided portion **558** together. This embodiment provides the catheter with a flexible region just proximal to the ultrasound radiating member **524**. In various preferred embodiments, the braided sections may be formed of high or low density polyethylenes, urethanes or nylons.

Sharpeable Tip

FIG. 6A illustrates yet another modified embodiment wherein the ultrasound catheter provides improved tracking over the guidewire **602**. Prolapsing of a guidewire is most likely to occur at small vessel radii, where the guidewire **602** follows a sharp turn, and where the angle θ formed by the intersection between the guidewire **602** and the catheter body is large. In order to reduce the incident angle θ between the guidewire and catheter body, a tapered wire **642** is provided along the exterior of the outer sheath **608** for shaping the distal end of the catheter. The tapered wire **642** may be set in a flexible potting or filler material **644**, which is contained within a flexible sleeve **646**. The tapered wire **642** is preferably comprised of a pliable material, such that it may be pre-formed into a selectable desired orientation before use. Pre-forming of the tapered wire **642** assists the physician in steering the catheter to follow the guidewire **602** reliably around small vessel radii by reducing the angle θ formed by the intersection between the guidewire **602** and the catheter body. The tapered wire is preferably provided in the region surrounding the ultrasound radiating element **624**. FIG. 6B illustrates the embodiment of FIG. 6A in use with the tip pre-formed for improved tracking over the guidewire.

Soft Tip Assembly

In addition to having excellent flexibility, it is also desirable for an ultrasound catheter to have a rounded and/or soft tip assembly for minimizing trauma or damage to the tissue along the inner wall of the blood vessel. This feature is particularly important during advancement through small blood vessels in the neurovasculature.

FIG. 7A illustrates an alternative embodiment wherein the distal end portion of an ultrasound catheter is provided with a soft tip assembly **700**. In the illustrated embodiment, the

ultrasound catheter generally comprises an elongate shaft body **702**, an ultrasound radiating element **704**, an elongate soft tip **706** and a connecting sleeve **708**. The soft tip **706** of the catheter is constructed to be softer and more flexible than the shaft body **702** for the purpose of minimizing or eliminating damage to the tissue along the inner wall of a blood vessel. In the illustrated embodiment, the soft tip **706** is configured as a substantially hollow member including a delivery lumen **710**. The lumen **710** may be used for receiving a guidewire and/or for delivering drugs to a treatment site. Preferably, the shaft body **702** and the soft tip **706** have substantially the same outer diameter. The delivery lumen **710** terminates at an exit port **720** at the extreme distal tip of the soft tip assembly.

Still referring to FIG. 7A, the ultrasound radiating element **704** is provided at a location just distal to the shaft body **702** and just proximal of the soft tip **710**. Preferably, a small gap **712** is provided between the ultrasound radiating element **704** and the elongate body **702** and also between the ultrasound radiating element **704** and the soft tip **706**. In the illustrated embodiment, a single cylindrical ultrasound radiating element **704** is provided, however, in alternative embodiments, others variations may be used, such as, for example a plurality of smaller ultrasound radiating elements.

In the illustrated embodiment, the shaft body **702**, ultrasound radiating element **704** and soft tip **706** are secured together by the sleeve **708**. The ultrasound radiating element **704** is contained within the lumen of the sleeve **708**. The proximal end **714** of the sleeve **708** extends over the distal portion of the shaft body **702**. The distal end **716** of the sleeve **708** extends over the proximal end of the soft tip **706**. In one embodiment, the sleeve **708** is formed of heat shrink tubing. To maximize effectiveness of the ultrasound catheter, the sleeve **708** is preferably constructed of a material having a low impedance to ultrasound energy. FIG. 7B illustrates a cross-sectional view of the soft tip assembly of FIG. 7A as seen through line 7B-7B.

Referring again to FIG. 7A, the illustrated embodiment of the soft tip assembly **706** is formed with a plurality of side holes **718**. The side holes **718** are in communication with the delivery lumen **710** and are provided for enhancing the delivery of drugs to the treatment site. Using the side holes **718**, the therapeutic agent can be delivered radially at a location closer to the ultrasound radiating element **704**. The illustrated embodiment includes two side holes, however, in alternative embodiments, any number of side holes may be used without departing from the spirit and scope of the invention. Alternatively, the soft tip assembly may be configured without any side holes.

In alternative embodiments, the soft tip assembly may have a solid tip wherein drugs exit the tip assembly only through side ports. In the embodiments with a solid tip, the guidewire exits the catheter through a side port, such as in a rapid exchange or monorail catheter design. In another embodiment, the soft tip assembly includes a radiopaque material to provide for high visibility under fluoroscopy. In various alternative embodiments, the soft tip assembly may have a variety of different lengths, such as, for example, 1 mm, 3 mm and 6 mm.

In operation, the ultrasound catheter is advanced over a guidewire that extends through the delivery lumen **710**. As the ultrasound catheter is advanced through a small blood vessel, the soft tip assembly bends and conforms to the shape of the blood vessel to reduce the pressure applied along the inner wall. The rounded tip of the soft tip assembly also minimizes trauma to the tissue as it is advanced along the inner walls of the blood vessels. The soft tip assembly can bend to facilitate the advancement of the catheter, yet will return to substan-

tially its original shape. After the ultrasound element is positioned in the desired location, the guidewire may be removed and the delivery lumen **710** used for the delivery of a therapeutic agent to the treatment site.

The soft tip assembly is preferably made of a soft polymer extrusion, such as, for example, polyimide. In one preferred method of construction, the soft tip assembly is constructed by first cutting the extruded soft tubular body into a length of approximately 3 to 6 mm. The distal tip is then rounded and smoothed using a heated die with the desired contour. In the embodiments wherein side holes are provided, the side holes are created using a 0.010 inch hole plunger. The soft tip assembly is then attached to the elongate shaft body using an adhesive or by thermal bonding. Alternatively, a length of heat shrink tubing may be used to secure the shaft body to the soft tip assembly.

Ultrasound Element on a Guidewire

FIGS. 8 and 9 illustrate another modified embodiment of an ultrasound catheter **850**. As shown in FIG. 8, in this embodiment, an ultrasound radiating element **852** is connected to or mounted on a distal end **854** of a guidewire **856**. In the illustrated arrangement, the ultrasound radiating element **852** is in the shape of a hollow cylinder. As such, the guidewire **856** can extend through the ultrasound radiating element **852**, which is positioned over the guidewire **856**. The ultrasound radiating element **852** can be secured to the guidewire **856** in any suitable manner, such as with an adhesive. In other embodiments, the ultrasound radiating element **856** can be of a different shape, such as, for example, a solid cylinder, a disk, a solid rectangle or a plate attached to the guidewire **856**. The ultrasound radiating element **852** can also be formed from a plurality of smaller ultrasound elements.

In the illustrated embodiment, ultrasound energy is generated from electrical power supplied to the ultrasound radiating element **852**. As such, the ultrasound radiating element **852** is connected to a pair of wires **860**, **862** that can extend through the catheter body. In the illustrated embodiment, the wires **860**, **862** are preferably secured to the guidewire **856** with the first wire **860** is connected to the hollow center of the ultrasound radiating element **852** and the second wire **862** connected to the outer periphery of the ultrasound radiating element **852**. As with the previous embodiments, the ultrasound radiating element **852** is preferably formed from, but is not limited to, a piezoelectric ceramic oscillator or a similar material. Other wiring schemes include wires connected to both ends of a solid transducer or both sides of a block. The ultrasound radiating element **852** and the wires **860**, **862** are preferably covered with a thin insulating material **857**.

FIG. 9 illustrates one embodiment of a catheter **850** that can be used with the guidewire **856** described above. In this embodiment, the catheter **850** includes an outer sheath **866**, which defines the delivery lumen **868**. As such, the illustrated embodiment does not include an inner core. The delivery lumen **868** includes a distal opening **870**. As will be explained below, in one arrangement, the distal opening **870** can be configured such that the guidewire **856** and the ultrasound radiating element **852** can be withdrawn into the catheter **850** through the distal opening **870**. In such an arrangement, a distal end **872** of the catheter **850** preferably includes a sleeve **874**, that is constructed from a material that readily transmits ultrasound energy as described above. In another arrangement, the distal opening **870** can be configured such that ultrasound radiating element **852** can not be withdrawn into the catheter **850** through the distal opening **870**. In such an

arrangement, the ultrasound radiating element **852** is configured to operate outside the catheter **850** near the distal opening **870**.

In one embodiment, the distal end **854** of the guidewire **856** is percutaneously inserted into the arterial system at a suitable first puncture site. The guidewire **856** and the ultrasound radiating element **852** are advanced through the vessels towards a treatment site, which includes a thrombotic occlusion. The guidewire **856** is preferably then directed through the thrombotic occlusion.

The catheter **850** is thereafter percutaneously inserted into the first puncture site and advanced along the guidewire **856** towards the treatment site using traditional over-the-guidewire techniques. The catheter **850** is advanced until the distal end of the catheter **856** is positioned at or within the occlusion. Preferably, the distal end includes radio opaque markers to aid positioning the distal end within the treatment site.

In one embodiment, the guidewire **856** can then be withdrawn until the ultrasound radiating element **852** is positioned within the distal end **874** of the catheter **850**. In such an arrangement, the catheter **850** can include a proximal stop **875** to aid the positioning of the ultrasound radiating element **852**. In another embodiment, the guidewire can be withdrawn until the ultrasound radiating element **852** is located near or adjacent the distal opening **870**. The catheter **850** can then be operated as described above.

In another modified embodiment, a standard guidewire (not shown) is percutaneously inserted into the first puncture site and advanced through the vessels towards and preferably through the occlusion. The catheter **850** is thereafter percutaneously inserted into the first puncture site and advanced along the standard guidewire towards the treatment site using traditional over-the-guidewire techniques. The catheter **850** preferably is advanced until the distal end of the catheter **850** is positioned at or within the occlusion. The standard guidewire can then be withdrawn from the delivery lumen. The guidewire **856** and ultrasound radiating element **852** of FIG. **8** can then be inserted into the delivery lumen. In one embodiment, the ultrasound radiating element **852** is advanced until it is positioned in the distal end of the catheter **850**. In another embodiment, the ultrasound radiating element **852** is advanced until it exits the distal end **870** of the delivery lumen **868**. The catheter can then be operated as describe above.

FIG. **10** illustrates yet another modified embodiment of an ultrasound catheter **1000** that can be used with the guidewire **1056** and ultrasound radiating element **1052**, as described above. In this embodiment, the guidewire lumen **1068** is defined by an inner sleeve or tube **1002**. The distal end **1070** of the delivery lumen **1068** can be configured as described above for preventing or withdrawing the ultrasound radiating element **1052** into catheter **1050**. In the illustrated arrangement, the delivery lumen **1068** can be used to transport the drug solution. In another arrangement, the space **1004** between the inner core **1002** and the outer sheath **1066** can be used to transport the drug solution. In such an arrangement, the outer sheath **1066** preferably includes one or more holes positioned at the distal end **1072** of the outer sheath **1066**. The catheter can be advanced on the guidewire **856** of FIG. **8** or a standard guidewire as described above.

Ultrasound Element on a Hypotube

FIGS. **11** and **12** illustrate yet another embodiment of an ultrasound catheter **1101** that is particularly well suited for use with small vessels of the distal anatomy. As shown in FIG.

12, this embodiment of the ultrasound catheter **1101** generally comprises a treatment wire **1103** and a microcatheter **1105**.

FIG. **11** illustrates a preferred embodiment of a treatment wire **1103**. As shown in FIG. **11**, in this embodiment, an ultrasound radiating element **1106** is connected to the distal tip of a hypotube **1108**. As discussed with reference to the small vessel catheters described above, the ultrasound radiating element can take many shapes and forms. The ultrasound radiating element **1106** is potted in an insulating material either as a conformal coating or potted inside an outer sleeve. The potting **1110** over the ultrasound radiating element **1106** sections is optimized for transmission of ultrasound energy. In the embodiment illustrated in FIG. **11**, the width of the potted ultrasound radiating element **1112** is approximately 0.018 inches. An epoxy or similar adhesive known in the catheter manufacturing field connects the potted ultrasound radiating element **1112** with the hypotube **1108** at junction **1114**.

The hypotube **1108** is made from Nitinol or stainless steel or other suitable material in accordance with the techniques and materials known in the catheter manufacturing field. In one embodiment, the hypotube has a diameter of approximately 0.014 to 0.015 inches. The hypotube **1108** provides an insulated lumen **1116** through which one can run power wires **1118** for the ultrasound radiating element **1106** or wires for temperature sensors (not shown) in the microcatheter **1105**. The microcatheter **1105**, into which the treatment wire **1103** is inserted, has a diameter greater than the width of the potted ultrasound radiating element **1112**.

As shown in FIG. **11**, in this embodiment, a flexible nose **1120** is connected to the distal end of the potted ultrasound radiating element **1112**. An epoxy or similar adhesive known in the catheter manufacturing field connects the flexible nose **1120** to the potted ultrasound radiating element **1112** at junction **1122**. The flexible nose **1120** is at least approximately 3 millimeters in length and functions as a guidewire when the treatment wire **1103** is inserted into a microcatheter **1105**. In the embodiment illustrated in FIG. **11**, the flexible nose **1120** is a soft coil made of metal or another suitable material known in the art. The flexible nose **1120** facilitates the delivery of the potted ultrasound radiating element **1112** through the microcatheter **1105** and into the vessel lumen of the treatment site. Preferably, the flexible nose **1120** is tapered in a manner so that the distal end of the nose has a smaller diameter than the proximal end.

In use, a free end of a guidewire is percutaneously inserted into the arterial system at a suitable first puncture site. The guidewire is advanced through the vessels toward a treatment site, such as, for example, a thrombotic occlusion in the middle cerebral artery.

The microcatheter **1105** is thereafter percutaneously inserted into the first puncture site and advanced along the guidewire towards the treatment site using traditional over-the-guidewire techniques. The catheter **1105** is advanced until the distal end **1199** of the catheter **1105** is positioned at or within the occlusion. Preferably, the distal end **1199** includes radio opaque markers to aid positioning the distal end **1199** within the treatment site.

The guidewire can then be withdrawn from the delivery lumen **1197** of the microcatheter **1105**. As illustrated in FIG. **12**, the treatment wire **1103** is then inserted and advanced through the microcatheter **1105** to the treatment site. The potted ultrasound radiating element **1112** of the treatment wire **1103** is advanced beyond the distal end **1199** of the

microcatheter and into lumen of the vessel. Once at the target site, the ultrasound radiating element **1106** provides ultrasound energy.

Preferably, drugs **1124**, including but not limited to drugs having thrombolytic effects, are infused through the microcatheter **1105** and delivered into the vessel around the ultrasound radiating element **1106** at the same time the ultrasound radiating element **1106** emits energy. It is believed that the transmission of ultrasound energy at the treatment site enhances drug uptake and activity and has other therapeutic effects. Preferably, the potted ultrasound radiating element **1112** extends far enough away from the distal tip **1199** of the microcatheter **1105** to facilitate the infusion of drugs (shown by arrow **1124**) through the microcatheter **1105** and into the vessel.

Overview of Ultrasound Catheter with Embedded Conductors

In certain embodiments, wherein an ultrasound radiating member is positioned between an inner elongate tubular body and an outer elongate tubular body, it is desired to pass elongate electrical conductors to the ultrasound radiating member from the proximal end of the catheter, thereby allowing an externally-generated driving signal to be provided to the ultrasound radiating member. In addition, in embodiments wherein a temperature sensor is positioned in the distal region of the catheter, it is desired to pass one or more elongate electrical conductors to the temperature sensor from the proximal end of the catheter, thereby allowing a distal temperature signal to be monitored at the proximal end of the catheter. The configuration of such elongate electrical conductors can be manipulated to affect the stiffness, torqueability, pushability, flexibility and other mechanical parameters of the catheter, thereby affecting accessibility of remote targets in the patient's vasculature.

Such embedded conductor configurations are discussed in greater detail in this section. These embodiments are particularly well-suited for use with small vessels of the distal anatomy, such as, for example, the vessels of the neurovascular system. However, such embodiments are also well-suited for the treatment of long segment peripheral arterial occlusions.

Referring now to FIG. **13A**, an ultrasonic catheter **1200** generally comprises a multi-component tubular body **1201** having a proximal end **1204** and a distal end **1202**. The tubular body **1201** and other components of the catheter **1200** can be manufactured in accordance with any of a variety of techniques well known in the catheter manufacturing field, and as explained above.

The ultrasonic catheter **1200** also comprises one or more ultrasound radiating members **1240** at its distal end **1202**. Suitable material dimensions for the ultrasound radiating member **1240** can be readily selected taking into account the natural and anatomical dimensions of the treatment site and of the desired percutaneous access site, as explained above. In other embodiments, the ultrasonic catheter **1200** further comprises a temperature sensor (not shown) positioned within the catheter distal region, as described above. In one preferred embodiment of an ultrasonic catheter **1200**, a central lumen **1251** can be concentrically placed over a guidewire (not shown) which has been previously navigated to the target area under, for example, fluoroscopic localization by a skilled surgeon or medical practitioner.

The ultrasonic catheter **1200** generally comprises one or more electrically conductive wires or fibers **1206**, **1208** that extend along the length of the catheter **1200**. In certain

embodiments, the conductive wires **1206**, **1208** generally reside within the wall **1210** of the tubular body **1201**. In such embodiments, the wall **1210** of the tubular body **1201** comprises an inner portion **1212** and an outer portion **1214**. In such embodiments, the conductive wires **1206**, **1208** can be located in between the inner portion **1212** and outer portion **1214** of the wall **1210**.

The inner portion **1212** provides a barrier against the contents of the central lumen **1251**, such as, for example, therapeutic drugs infused through the central lumen **1251** and out the distal end **1202** of the catheter to a treatment site within the patient's vasculature. The outer portion **1214** provides a barrier against the environment in which the catheter **1200** resides, which may include, for example, blood or other bodily fluids.

The inner portion **1212** and outer portion **1214** of the wall **1210**, and the wall **1210** in general, with the exception of the conductive wires **1206**, **1208** embedded in the wall **1210**, is made of insulating material, such as, for example, polyimide, high or low density polyethylenes, urethanes, nylons, and the like. Consequently, the conductive wires **1206**, **1208** are electrically isolated from the central lumen **1251** and the environment in which the catheter **1200** resides.

The conductive wires **1206**, **1208** are also preferably electrically isolated from each other. In one embodiment, the wires **1206**, **1208** are arranged and configured in a manner to prevent contact between them. For example, the wires **1206**, **1208** may be arranged along and/or around the central lumen in a manner which prevents any contact between the wires **1206**, **1208**. Also, electrically insulating material may be placed between the wires **1206**, **1208** to prevent contact between them. In another embodiment, the wires **1206**, **1208** are covered with insulating coating material either in addition to or in lieu of placing insulating material between the wires **1206**, **1208** or making the wall **1210** from insulating material.

The physical configuration or layout of the conductive wires **1206** and **1208** embedded within the wall **1210** of the tubular body **1201** can be adjusted to determine the mechanical attributes of the catheter **1200**. The conductive wires **1206**, **1208** may be arranged in various architectures such as, for example, linear arrays, weaving, spiraling, and other patterns which modulate stiffness, torqueability, pushability, flexibility and other mechanical parameters of the catheter which relate to accessibility of remote targets.

In one embodiment, shown in FIG. **13A**, both conductive wires **1206**, **1208** spiral around the central lumen **1251** and remain substantially parallel to each other at all times along the length of the catheter **1200**. In a modified embodiment, the wires **1206**, **1208** are covered with insulating coating material. In another modified embodiment, illustrated in FIG. **13B**, the conductive wires **1206**, **1208** are covered with insulating coating material or separated with insulating material and are contained in a unitary cable **1216**. In such embodiments, the cable **1216** spirals around the central lumen **1251** along the length of the catheter **1200**.

In another embodiment, illustrated in FIG. **14**, the conductive wires **1206**, **1208** are covered with insulating coating material and are spiraled in opposite directions, thereby forming a helix or helical pattern around the central lumen **1251**. In forming a helical pattern, the wires **1206**, **1208** cross each other, but remain electrically isolated from each other due to the insulating coating material around each wire.

In another embodiment, illustrated in FIG. **15**, the conductive wires **1206**, **1208** run in a generally straight line along the length of the catheter **1200**, and do not spiral around the

central lumen **1251** or cross each other. In such embodiments, the wires **12606**, **12608** can optionally be covered with an insulating coating material.

In a modified embodiment, illustrated in FIGS. **16A** and **16B**, the ultrasound catheter comprises an outer tubular body **1400** surrounding an inner core **1402**. The inner core **1402** defines a central lumen **1408** that can be used to pass a guidewire, a cooling fluid or a therapeutic compound through the ultrasonic catheter. In a distal region of the ultrasound catheter, a tubular ultrasound radiating member **1404** is positioned between the outer tubular body **1400** and the inner core **1402**. In regions proximal to the ultrasound radiating member **1404**, the outer tubular body **1400** and the inner core **1402** are separated by an insulating layer **1406**. Preferably, the inner core outer surface **1410** and the outer tubular body inner surface **1412** are electrically conductive, and are electrically connected to opposite poles of a power supply (not shown). Such electrically conductive surfaces can be created by depositing an electrically conductive material onto the desired surface.

In such embodiments, the conductive surfaces are separated by the insulating layer **1406** along the length of the catheter, and the presence of the ultrasound radiating member **1404** in the catheter distal region completes the electric circuit. In particular, because opposite surfaces of the ultrasound radiating member contact conductive surfaces of opposite polarity **1410**, **1412**, a voltage difference is created across the ultrasound radiating member, thereby causing ultrasonic vibrations to be created.

Such embodiments allow the ultrasound radiating member **1404** to be driven while eliminating any wires passing along the catheter body, such as illustrated in FIGS. **13A** through **15**. Elimination of wiring in the catheter body reduces manufacturing costs and reduces overall catheter dimensions, thereby increasing catheter maneuverability. Elimination of wiring can also increase catheter flexibility. Thus, in applications where the ultrasound catheter is to be passed through a small or tortuous portion of the vasculature, it may be desired to use such embodiments.

Small vessel ultrasonic catheters with conducting wires or fibers embedded in the walls of the catheter, as described above, can be assembled in a number of ways. See, for example, U.S. Pat. Nos. 4,277,432 and 6,030,371, both of which are incorporated by reference herein. In one method, the catheter is made from tubing which is fabricated from a polymer material that is extruded through a dye in a molten state and that is solidified while being drawn. In one preferred embodiment of the present invention, an electrically insulating material is extruded through the dye.

Conventionally, manufacturing equipment is used to co-extrude polymer support fibers, such as, for example, Kevlar, into the tubing wall in a linear, spiral, or woven pattern. In certain embodiments of the present invention, electrically conductive wires or fibers are used in lieu of polymer support fibers. Examples of conductive fibers include, but are not limited to, copper, carbon, steel, and stainless steel. In a modified embodiment, the conductive fibers are pre-coated with an insulating coating before they are co-extruded.

In another method of assembling small vessel catheters with conducting wires or fibers embedded in the walls of the catheter, the wires are sandwiched between two concentric tubes, an inner tube and an outer tube, both of which initially have approximately half the wall thickness of the final assembled catheter. The inner diameter of the inner tube determines the diameter of the final assembled catheter. The inner diameter of the outer tube is significantly greater than the outer diameter of the inner tube. For example, the inner and outer tubes can be made from an electrically isolating material.

In such embodiments, the catheter is assembled by winding or placing conductive fiber or wire over the inner tube; concentrically translating the outer tube over the inner tube and the fiber wrapping or abutting the inner tube; and radially shrinking the outer tube onto the inner tube such that the conductive fiber is trapped between the inner and outer tubes. In a modified embodiment, the conductive fibers are pre-coated with an insulating coating before they are incorporated into the above described sandwich construction.

As described above, the various configurations and arrangements of the elongate electrical conductors described herein can be used regardless of whether such elongate electrical conductors are connected to an ultrasound radiating member or a temperature sensor at the catheter distal end.

CONCLUSION

While the foregoing detailed description has described several embodiments of the apparatus and methods of the present invention, it is to be understood that the above description is illustrative only and not limiting of the disclosed invention. It will be appreciated that the specific dimensions of the various catheters and guidewires can differ from those described above, and that the methods described can be used within any biological conduit within the body and remain within the scope of the present invention. Thus, the invention is to be limited only by the claims which follow.

We claim:

1. A method of manufacturing an ultrasonic catheter comprising:

providing an inner tube having an inner diameter sufficient to accommodate a guidewire;

mounting a tubular ultrasound radiating member around a distal region of the inner tube;

positioning a first and a second electrical conductor along the inner tube, such that the first electrical conductor contacts an inner side of the ultrasound radiating member, and the second electrical conductor contacts an outer side of the ultrasound radiating member;

concentrically translating an outer tube over the inner tube and the ultrasound radiating member; and

radially shrinking the outer tube onto the inner tube, so that the first and the second electrical conductors are located in between the inner tube and the outer tube along the length of the ultrasonic catheter.

2. The method of claim 1, further comprising:

mounting a temperature sensor adjacent to the distal region of the inner tube; and

positioning at least one temperature sensor wire along the inner tube, such that the temperature sensor wire is electrically connect to the temperature sensor.

3. The method of claim 1, wherein the first and second electrical conductors are positioned along the inner tube in a substantially parallel configuration.

4. The method of claim 3, wherein the first and second electrical conductors are positioned along the inner tube at substantially radially opposite points.

5. The method of claim 1, further comprising integrating the first and second electrical conductors into a unitary cable.

6. The method of claim 1, wherein the first and second electrical conductors are wrapped around the inner core in opposite directions.

7. The method of claim 1, further comprising connecting the first and second electrical conductors to opposite poles of a power supply at a proximal end of the ultrasonic catheter.

