

(19)



(11)

EP 1 942 810 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
08.08.2012 Bulletin 2012/32

(51) Int Cl.:
A61B 19/00 (2006.01) A61B 17/02 (2006.01)

(21) Application number: **06813458.4**

(86) International application number:
PCT/US2006/031793

(22) Date of filing: **16.08.2006**

(87) International publication number:
WO 2007/022159 (22.02.2007 Gazette 2007/08)

(54) SYSTEM FOR POSITIONING A LAPAROSCOPIC DEVICE

SYSTEM ZUR POSITIONIERUNG EINES LAPAROSKOPIEGERÄTS

SYSTEME DE POSITIONNEMENT D'UN DISPOSITIF LAPAROSCOPIQUE

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HU IE IS IT LI LT LU LV MC NL PL PT RO SE SI
SK TR**

(30) Priority: **18.08.2005 US 709098 P
28.10.2005 US 730853 P
14.02.2006 US 772863 P
16.02.2006 US 773638 P
07.08.2006 US 821692 P
15.08.2006 US 464804**

(43) Date of publication of application:
16.07.2008 Bulletin 2008/29

(73) Proprietor: **Civco Medical Instruments Co., Inc.
Kalona, IA 52247-9589 (US)**

(72) Inventors:
• **WILSON, Roger, F.
Sarasota, FL 34240 (US)**

• **WHITMORE III, Willet, F.
Longboat Key, FL 34228 (US)**

(74) Representative: **Moreland, David et al
Marks & Clerk LLP
Aurora
120 Bothwell Street
Glasgow
G2 7JS (GB)**

(56) References cited:
**WO-A2-02/087420 WO-A2-2005/089113
GB-A- 2 354 559 US-A- 3 285 099
US-A- 3 858 578 US-A- 4 867 404
US-A- 4 867 404 US-A- 5 372 147
US-A- 5 555 897 US-A- 5 571 072
US-A- 5 704 900 US-A- 5 899 425
US-A1- 2003 208 207**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 1 942 810 B1

Description

FIELD OF THE INVENTION

[0001] The invention relates to a system for positioning a laparoscopic device. In particular, the invention relates to a holder and curvilinear articulating arm for positioning a laparoscopic device such as an endoscopic camera.

BACKGROUND OF THE INVENTION

[0002] During laparoscopy, a minimally invasive surgical procedure in which tissue for example may be removed from the abdomen or chest through a small puncture wound, the laparoscopic surgery is performed with the aid of an endoscopic camera. The camera is placed through a port in the skin into a working cavity and may be used for example to visually examine the interior of the cavity such as the peritoneum or surgical planes or spaces created for purposes of dissection. Typically, the camera includes a light source. Correct positioning and aim of the laparoscopic camera and light throughout a procedure are fundamental to laparoscopy.

[0003] Most commonly, the endoscopic camera is held by an assistant who must continually watch the video monitor and hold a steady position until the surgeon requests a change in the field of view. Alternatively, a variety of robotic arms have been designed to hold the camera and move for example on voice command by the surgeon. Such systems include the AESOP® (Automated Endoscopic System for Optimal Positioning) voice controlled robot system and the Zeus® minimal invasive surgical robot system from Computer Motion Inc. / Intuitive Surgical Inc. Mechanical/electrical servomotor controlled systems that move by foot controls, palm and fingertip controls include the LAPMAN® by MedSys s.a. of Belgium, while a remote, manual control system da Vinci® is available from Intuitive Surgical Inc.

[0004] In addition, a variety of known mechanical frameworks that have multiple adjustment and locking points can be used to hold an endoscopic camera including a laparoscopic retractor from Thompson Surgical Instruments, the Martin Arm System from Gebrüder Martin GmbH & Co. KG, and the Omni-Tract® surgical retractors from Minnesota Scientific Inc. These devices have the capability of holding other laparoscopic instruments as well, although different connections at the instrument interface may be required depending on the instrument and the application.

[0005] The first choice for any surgeon is to have a good human assistant, who can continuously and accurately aim and focus the camera and light on the moving surgical field. Unfortunately, good assistance, or any assistance for that matter, is frequently unavailable, and the surgeon must work solo. Also, occasions frequently arise where an assistant's hands may be occupied by other tasks, such as retraction and suction, and in these circumstances other means for holding the camera also

are required. The alternatives for holding and positioning the camera cited above then come into play. However, these alternatives each have one or more troublesome drawbacks. The high end robotic arms (such as da Vinci) are expensive, have high maintenance requirements, are time consuming and cumbersome to set up and may have high cost disposable components. They also require an experienced assistant or technician to be present. The simpler, voice controlled (AESOP) or palm radio controlled (LAPMAN) robotic arms also require significant maintenance and set up time, move too slowly for many surgeons, and are hard to precisely control. The mechanical arms and frameworks that are available typically have too many movable parts that require adjustment, require two hands for re-positioning, may have a large footprint near the surgical field, and are very slow to reposition because of the several joints that must be loosened and retightened.

[0006] Thompson Surgical Instruments also offers a Flexbar Scope Holder (product #42133C). This device has a clamp to the bedside railing and a set of stainless steel rods that may be clamped at a desired length with right angle clamps to position the base attachment of a curvilinear flexible arm. The arm uses a combination of a screw and cam locking mechanism to achieve an adjustable friction lock of the arm. In this device, the clamp that holds the laparoscopic camera at the free end of the flexible arm has limited capabilities; the clamp becomes locked dimensionally with the arm and is not a universal joint. The design of the scope holder generally requires a user to loosen and then retighten the locking mechanism for the arm whenever it is necessary to reposition the laparoscope.

[0007] Thus, there remains a need for better holding and positioning devices for laparoscopic instruments in general and for the laparoscopic camera (laparoscope) in particular. In particular there is a need for a device that will hold a laparoscope steady when it is not in hand, may be quickly re-positioned using one hand, allows quick engagement and disengagement to a laparoscopic instrument, and has a minimal and movable footprint on the surgical field.

[0008] A system according to the preamble of claim 1 is disclosed in US 5 571 072.

SUMMARY OF THE INVENTION

[0009] The invention relates to a system for positioning a laparoscopic device, the system having a holder. The holder includes a central portion having a first member operatively associated with a second member, the members selectively movable with respect to one another along a central axis, the central portion having a proximal end defined by the first member and a distal end defined by the second member. The holder also has at least three proximal rotational joints coupled to the first member proximate the proximal end, at least two distal rotational joints coupled to the second member proximate the distal

end, a clamp configured and dimensioned for retaining a laparoscopic device, and a coupling portion proximate a first of the proximal rotational joints. A first of the distal rotational joints is coupled to the distal end of the central portion and a second of the distal rotational joints is coupled to the clamp.

[0010] Each proximal rotational joint and each distal rotational joint permits 360° of rotation about an axis thereof.

[0011] In some embodiments, the members may telescope with respect to one another. The second member may be slidably received in the first member. The first member may have a slot and the second member may have a protrusion, the protrusion movable within the slot. For example, the protrusion may include a roller key. Also, in some embodiments, the second member may include a piston member proximate an end thereof, the piston member disposed within the first member. The piston member may be spring-loaded with a spring oriented transverse to the central axis.

[0012] The first member may include a receiving end for receiving the second member and a bushing coupled to the receiving end, with the bushing having a plurality of fingers disposed radially with respect to the central axis.

[0013] Each of the proximal and distal rotational joints may include a thrust bearing which may be a steel ball thrust bearing. In addition, each of the proximal rotational joints may include a washer abutting a spacer and rotatable with respect to each other. In some embodiments, the spacer may be formed of a material that is polytetrafluoroethylene-based. Each of the distal rotational joints may include a washer abutting a spacer and rotatable with respect to each other. In some embodiments, the spacer may be formed of a material comprising acetal homopolymer. Each of the proximal and distal rotational joints may include a spacer, each of the spacers of the proximal rotational joints having a first thickness and each of the spacers of the distal rotational joints having a second thickness, the first thickness being smaller than the second thickness.

[0014] The at least three proximal rotational joints may be three proximal rotational joints that each permit movement in a separate plane, and at least two of the planes may be parallel to one another.

[0015] The first of the distal rotational joints may permit rotation about an axis coinciding with the main axis and the second of the distal rotational joints may permit rotation about an axis transverse to the main axis. Also, the second of the distal rotational joints may permit rotation about an axis generally perpendicular to the main axis.

[0016] The clamp may include a pair of spring-biased jaw members each having a cover formed of a material softer than aluminum, the clamp being configured and dimensioned to retain the laparoscopic device while contacting the covers. For example, each cover may be formed of polyurethane.

[0017] The laparoscopic device may have a cylindrical

portion. The first member may be tubular. Each of the proximal and distal rotational joints may have a first portion rotatable with respect to a second portion about a fixed axis. The first and second members may be movable with respect to each other along the central axis but may not be rotatable with respect to each other.

[0018] The system may further include a curvilinear articulating arm, the holder being coupled to the curvilinear articulating arm. In addition, the system may further include a tray configured and dimensioned for supporting a mammal, the curvilinear articulating arm being coupled to the tray.

[0019] The coupling portion may include a clamp for coupling to a support, wherein the support is selected from the group consisting of a rail of a table and a rail of a bed.

[0020] The invention also relates to a system for positioning a laparoscopic device including a curvilinear articulating arm and a holder having at least two rotational regions and a clamping portion for receiving the laparoscopic device, the holder being coupled to the curvilinear articulating arm. The at least two rotational regions are permitted to articulate. The holder may further include a central portion with a selectively adjustable length along a central axis, wherein the at least two rotational regions are disposed between the central portion and the clamping portion. In some embodiments, the holder further includes a central portion with a selectively adjustable length along a central axis, the central portion having a proximal end and a distal end, wherein the at least two rotational regions includes at least three proximal rotational joints disposed proximate the proximal end and at least two distal rotational joints disposed between the distal end and the clamping portion. The at least two rotational regions may include a thrust bearing.

[0021] In addition, the invention relates to a method of positioning a laparoscopic device in a skin port of a mammal, the method including: coupling the laparoscopic device to a holder comprising a clamping portion and five rotational joints, the laparoscopic device being partially retained in the clamping portion; disposing the laparoscopic device partially within the skin port; positioning the laparoscopic device by selectively rotating portions of the holder with respect to one another. The method may further include positioning the laparoscopic device by selectively adjusting a length of the holder along a central axis. The holder may further include first and second members selectively movable with respect to one another. The length may be selectively adjustable by moving the first and second members with respect to each other. The length may be selectively adjustable by telescoping the first member with respect to the second member. Movement of the first and second members may be restricted to linear movement along the central axis, and the holder may be manually operated.

[0022] In some embodiments, the method may further include: coupling the holder to a curvilinear articulating arm; and articulating the curvilinear articulating arm. Al-

so, the method may further include: coupling the curvilinear articulating arm to a tray configured and dimensioned for supporting the mammal. Moreover, the method may further include: coupling the curvilinear articulating arm to a support, wherein the support may be selected from the group consisting of a rail of a table and a rail of a bed. The laparoscopic device may be held in a selected position while disposed partially within the skin port without locking movement of the rotational joints of the holder.

[0023] The invention also relates to a method of positioning a laparoscopic device in a skin port of a mammal, the method including: securing the laparoscopic device to a holder comprising at least two rotational joints; coupling the holder to a curvilinear articulating arm; disposing the laparoscopic device partially within the skin port; positioning the laparoscopic device by selectively articulating the curvilinear articulating arm and selectively rotating portions of the holder with respect to one another.

[0024] The method may further include: positioning the laparoscopic device by selectively adjusting a length of the holder along a central axis, wherein the holder further comprises first and second members selectively movable with respect to one another, and wherein the length is selectively adjustable by moving the first and second members with respect to each other. Also, the laparoscopic device may be held in a selected position while disposed partially within the skin port without locking movement of the rotational joints of the holder.

[0025] The invention further relates to a system for positioning a laparoscopic device such as a camera, the system including a curvilinear articulating arm and a holder that has at least two rotational regions as well as a clamping portion for receiving the laparoscopic device. The holder is coupled to the curvilinear articulating arm, and wherein the at least two rotational regions are permitted to articulate. The at least two rotational regions may be provided by one or more types of structures selected from the group consisting of a rotational joint, a rocking joint, and a living hinge. The at least two rotational regions may be permitted to freely articulate.

[0026] The invention also relates to a method of positioning a laparoscopic device in a skin port of a patient, the method including: securing the device in a holder permitted to articulate about at least two rotational regions; coupling the holder to a curvilinear articulating arm; disposing the device partially within the skin port; positioning the device by articulating the curvilinear articulating arm with the device moving in response to the articulation. The orientation of the device, such as a laparoscopic camera, thus may be set. The holder may be permitted to freely articulate about at least two rotational regions.

[0027] The present invention further relates to a new set of devices and a method that is particularly suited for holding, positioning and repositioning a laparoscopic camera throughout a laparoscopic surgical procedure. The device includes a holder with joints for permitting rotational movement and positioning of a clamping end

for securing a laparoscopic instrument. Fixed positioning and manual re-positioning may be quickly accomplished by simply overcoming the modest frictional resistance to movement within the devices without any mechanical adjustments after the initial set up. The joints of the holder may remain free to move at all times. When the holder is static it preferably will not move, and thus, in effect, becomes self locking because of the physical/mechanical relationship of the various system components including the laparoscopic instrument such as an endoscopic camera which is secured in the holder and extending through the skin of the patient. In addition, the multi-modality holder has alternative functionality for holding and positioning other laparoscopic instruments.

[0028] In one exemplary embodiment, the present invention comprises an articulating arm that may be attached at one end to a surgical table, and that has the capability of movement in three dimensions (i.e., at least three degrees (x, y and z) of freedom) at a free end. This arm has a receiving mechanism at the free end that can accept a variety of instrument holding devices one of the main ones of which is a laparoscopic instrument holder for coupling to the free end of the articulating arm and for positioning a laparoscopic device such as an endoscopic camera.

BRIEF DESCRIPTION OF THE DRAWINGS

[0029] Preferred features of the present invention are disclosed in the accompanying drawings, wherein:

FIG. 1 is a perspective view of a laparoscopic instrument holder system showing an exemplary arrangement with a holder **100** although the other exemplary holders disclosed herein may instead be used in such a system in place of holder **100**;

FIGS. 2A-2I show a laparoscopic instrument holder including **(2A)** a perspective view, **(2B)** a partial cross-sectional front view of a portion of the holder, **(2C)** a front view, **(2D)** a back view, **(2E)** a first side view, **(2F)** a second side view, **(2G)** a bottom view, **(2H)** a top view, and **(2I)** a perspective view of the mating of movable clamping jaws **122** and finger rest portion **126**;

FIGS. 3A-3G show a laparoscopic instrument holder, including **(3A)** a perspective view, **(3B)** a front view, **(3C)** a back view, **(3D)** a first side view, **(3E)** a second side view, **(3F)** a bottom view, and **(3G)** a top view;

FIGS. 3H-3N show yet another a laparoscopic instrument holder, including **(3H)** a perspective view, **(3I)** a front view, **(3J)** a back view, **(3K)** a first side view, **(3L)** a second side view, **(3M)** a bottom view, and **(3N)** a top view;

FIG. 3-O shows a perspective view of the holder of **FIGS. 3H-3N** with a modified member and clamping portion mounted thereon;

FIG. 3P-3Q show another laparoscopic instrument

holder, including (3P) a perspective view and (3Q) a front view;

FIG. 3R shows a perspective view of a portion of another clamping system for use with the present invention;

FIG. 3S shows a partial cross-sectional side view of the clamping system of **FIG. 3Q**;

FIGS. 3AA-3EE show a laparoscopic instrument holder including (3AA) a perspective view with a laparoscopic instrument retained by said holder, (3BB) a partial perspective view, (3CC) a partial cross-sectional perspective view, (3DD) another perspective view, and (3EE) another partial cross-sectional perspective view;

FIGS. 3FF-3UU show another laparoscopic instrument holder, including (3FF) a perspective view with a laparoscopic instrument retained by said holder, (3GG) a partial perspective view including several rotational joints, (3HH) a partial cross-sectional perspective view including the rotational joints of the previous figure, (3II) another partial perspective view including the rotational joints of the previous figure, (3JJ) a partial bottom view of the linear length adjustment portion of the holder, (3KK) a partial top view thereof, and (3LL) a partial cross-sectional side view thereof, (3MM) a partial cross-sectional side view of a coupling assembly, (3NN) a partial perspective view of several rotational joints, (3OO) another partial cross-sectional perspective view of several rotational joints and clamp, (3PP) a side view of a clamp, (3QQ) another side view of the clamp, and (3RR to 3UU) partial perspective views of the clamp; **FIGS. 3W-3WW** show an embodiment of a rotational joint for use with laparoscopic instrument holders of the present invention, including (3W) a partial side view and (3WW) a partial cross-sectional side view; **FIGS. 3XX-3ZZ** show another exemplary embodiment of a coupling portion for use with laparoscopic instrument holders of the present invention, including (3XX) a first side view, (3YY) a second side view, and (3ZZ) a partial cross-sectional perspective view; **FIGS. 3AAA-3HHH** show an embodiment of a laparoscopic instrument holder according to the present invention, including (3AAA) a perspective view with a laparoscopic instrument retained by said holder, (3BBB) a first partial side view, (3CCC) a second partial side view, (3DDD) a third partial side view, (3EEE) a partial cross-sectional side view of a piston member couple to a sliding member, (3FFF) a partial perspective view of several rotational joints, (3GGG) a partial perspective view of a rotational joint with joint members, and (3HHH) a partial perspective view of a clamp;

FIGS. 4A-4C show the curvilinear articulating arm assembly of **FIG. 1**, including (4A) a perspective view, (4B) a partial cross-sectional perspective view, and (4C) a partial side view;

FIGS. 4D-4L show the base handle of **FIG. 1**, includ-

ing (4D) a first side view, (4E) a second side view, (4F) a partial perspective view of a first set of components thereof, (4G) a partial side view of a second set of components thereof, (4H) another partial side view of the second set of components thereof, (4I) a front view, (4J) a back view, (4K) a top view, and (4L) a bottom view;

FIG. 4M shows a perspective view of a rail clamp for use with the present invention;

FIGS. 4N-4T show the free handle of **FIG. 1**, including (4N) a first side perspective view showing a portion of a tensioning wire therewith, (4O) a second side perspective view, (4P) a partial perspective view showing a first set of components thereof, (4Q) a front perspective view, (4R) a back perspective view, (4S) a top perspective view, and (4T) a bottom perspective view;

FIG. 4U shows a side perspective view of the interface lock of the free handle of **FIGS. 4N-4T**;

FIG. 5 shows a perspective view of a support system according to the present invention; and

FIGS. 6A-6C show the tray of **FIG. 5**, including (6A) a top view, (6B) a cross-section taken perpendicular to the central axis of the tray, and (6C) a partial cross-section showing detail taken at **VIC**.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

[0030] The instrument holders described herein are particularly useful in minimally invasive surgical procedures using a laparoscope (laparoscopic camera), which is a type of endoscope (endoscopic camera). It should be understood that each of the terms laparoscope, laparoscopic camera, endoscope, and endoscopic camera as individually used with respect to any particular embodiment are not meant to limit that embodiment to a laparoscopic or endoscopic context.

[0031] Referring initially to **FIG. 1**, a laparoscopic instrument holder system 10 is shown. Holder system 10 includes a curvilinear articulating arm assembly 12 and a laparoscopic instrument holder 14 coupled to assembly 12 as indicated by arrow A. As will be further described, arm assembly 12 includes a clamp 16 at a first free end thereof for coupling system 10 to a structure such as the rail 18 (shown schematically in phantom) of an operating room table.

[0032] Turning next to **FIGS. 2A-2G**, a first exemplary laparoscopic instrument holder 100 is shown. Holder 100 includes a coupling portion 102 in the form of a post. Coupling portion 102 preferably is configured to be received in portion 681 of free handle 662 of articulating arm assembly 12, as will be described later. Holder 100 includes a body portion 104 with a shaft portion 106 extending from an end thereof and forming a first rotational joint. As shown in the partial cross-sectional side view of **FIG. 2B**, shaft portion 106 may be formed as a screw with a head 106a, a cylindrical shaft 106b, and a threaded

end **106c** that may be received in threaded hole **104a** in body portion **104**. A first member **108** is mounted on shaft portion **106** and particularly cylindrical shaft **106b** so that shaft portion **106** extends within a bore **108a** in first member **108**. In the preferred exemplary embodiment, there is minimal frictional resistance to rotational movement of portion **106** and first member **108** with respect to one another so that these components are freely rotatable with respect to one another. However, the tolerance between the components preferably is selected to minimize other play therebetween, and the coupling between the components preferably is such that minimal translation of one component with respect to the other component is permitted along their central axis of rotation.

[0033] In alternate devices, portion **106** and first member **108** are mechanically associated with each other such that frictional engagement of these components provides limited resistance to rotational movement of portion **106** and first member **108** with respect to each other. However, the frictional engagement preferably permits relative rotation of portion **106** and first member **108** when sufficient manual, external force is applied as by a surgeon using holder **100** during a medical procedure.

[0034] Shaft portion **106** and first member **108** are disposed preferably at right angles with respect to each other. First member **108** preferably includes a shaft portion **110** that may be formed as a screw with a head **110a**, a cylindrical shaft **110b**, and a threaded end **110c** that may be received in threaded hole **108b** in first member **108**. Shaft portion **110** forms a second rotational joint.

[0035] Holder **100** further includes a second member **112** that is mounted on shaft portion **110** and particularly cylindrical shaft **110b** so that shaft portion **110** extends within a bore **112a** in second member **112**. In the preferred exemplary embodiment, there is minimal frictional resistance to rotational movement of second member **112** and portion **110** with respect to one another so that these components are freely rotatable with respect to one another. However, the tolerance between the components preferably is selected to minimize other play therebetween, and the coupling between the components preferably is such that minimal translation of one component with respect to the other component is permitted along their central axis of rotation.

[0036] In alternate devices, portion **110** and second member **112** are mechanically associated with each other such that frictional engagement of these components provides limited resistance to rotational movement of portion **110** and second member **112** with respect to each other. However, the frictional engagement preferably permits relative rotation of portion **110** and second member **112** when sufficient manual, external force is applied as by a surgeon using holder **100** during a medical procedure. Shaft portion **110** and second member **112** are disposed preferably at right angles with respect to each other.

[0037] In one preferred exemplary device the joints formed by rotational movement of portion **106** and first

member **108** with respect to each other, and by rotational movement of portion **110** and second member **112** with respect to each other, do not lock and are disposed at about 90° to each other. Preferably, the joints provide loose coupling between the components so that they may freely rock back and forth and be angulated.

[0038] In a preferred exemplary device a stop **104b** is created at the transition from a first circumference of body portion **104** to a smaller circumference of cylindrical shaft **106b**. Preferably, the length of cylindrical shaft **106b** is chosen to be approximately the length of bore **108a** in first member **108** so that a portion of first member **108** may be retained between head **106a** and body portion **104**.

[0039] In some alternate embodiments, portion **106** optionally may be tightened to provide substantial resistance to rotational movement of body portion **104** and first member **108** with respect to one another.

[0040] Similarly, a stop **108c** is created at the transition from a first circumference of first member **108** to a smaller circumference of cylindrical shaft **110b**. Stop **108c** may include washer **113** disposed between first member **108** and second member **112**. Preferably, the length of cylindrical shaft **110b** is chosen to be approximately the length of bore **112a** in second member **112** so that a portion of second member **112** may be retained between head **110a** and first member **108**. In the preferred embodiment, portion **110** provides minimal frictional resistance to rotational movement. However, in an alternate embodiment, portion **110** optionally may be tightened to provide substantial resistance to rotational movement of first member **108** and second member **112** with respect to one another.

[0041] Second member **112** includes a preferably arcuate clamping portion **114**. In addition, a pair of holes **116** extend into second member **112** and are disposed on either side of central longitudinal axis **118** thereof. Holes **116** are configured and dimensioned to receive end portions of springs **120**, which extend out of holes **116** and each may partially be disposed in a groove **120a** in second member **112**. Movable clamping jaws **122** are "spring loaded," with end faces **122a** abutting ends of respective springs **120**. Thus, springs **120** bias clamping jaws **122** so that face **122f** is biased toward clamping portion **114**. The slot formed between face **122f** and clamping portion **114** is designed so that the spring loading alone is sufficient to hold a laparoscope securely in place therein, but also to let the laparoscope rotate with sufficient frictional resistance to prevent undesired movement.

[0042] A set screw assembly **124** releasably and adjustably couples movable clamping jaws **122** to second member **112**. Preferably, only slight rotation of assembly **124** is permitted, e.g., one-quarter turn clockwise or counterclockwise. Such turning may loosen or tighten the engagement of movable clamping jaws **122** and finger rest portion **126** with respect to one another thus respectively permitting or hindering movement of spring-

loaded clamping jaws **122**.

[0043] In alternate devices, set screw assembly **124** may be any component(s) or manner of fixedly coupling finger rest portion **126** to second member **112**.

[0044] As shown for example in **FIG. 2I**, a finger rest portion **126** includes a central raised portion **126a** on a lower face **126b**. Central raised portion **126a** is slidably received in a slot **122b** in movable clamping jaws **122**. Travel of clamping jaws **122** is limited and governed by slot **122b** which includes a stop portion **122e**. Slot **122b** is symmetrically disposed with respect to axis **118**. Finger rests **122c, 122d** are disposed at a free end of movable clamping jaws **122**. Finger rest portion **126** is positionally fixed with respect to second member **112**, with a threaded screw **124a** of screw assembly **124** extending through hole **126c**. A knurled knob **124b** may be provided as well as a set screw **124c** (shown in **FIG. 2E**) extending into the shaft of screw **124a**.

[0045] Finger rest portion **126** includes a finger rest surface **126d** which provides sufficient surface area for accommodating a portion of a user's finger such as the fleshy tip of a user's thumb. Similarly, finger rests **122c, 122d** of movable clamping jaws **122** each provide sufficient surface area for accommodating a portion of another of a user's fingers. Thus, in use, in order to adjust the spacing between arcuate clamping portion **114** and clamping face **122f** of movable clamping jaws **122**, a user may grasp finger rest portion **126** with his or her thumb disposed on surface **126d** and two other fingers disposed on rests **122c, 122d**, and squeeze so that the spacing **d** between arcuate clamping portion **114** and clamping face **122f** is increased. Movement of clamping jaws **122** also is limited by the combined lateral distance defined by spacings **d, e**, particularly because of the fixed position of finger rest portion **126** with respect to second member **112** as well as the maximum travel of surfaces **122a** of movable clamping jaws **122** with respect to surfaces **112b** of second member **112**.

[0046] Thus, an object such as an endoscopic camera may be releasably retained in the space between portion **114** and clamping face **122f**. Finger rest portion **126** thus serves as a quick-release for such an object. Because clamping end face **122f** is movable with respect to arcuate clamping portion **114** of second member **112**, a variety of sizes and geometries of laparoscopic devices such as an endoscopic camera may be releasably retained within the region between clamping portion **114** and clamping end face **132a, 132b**. Although a single end face **132a** is shown, other configurations may be used including a bifurcated arrangement of clamping faces, or more than two distinct end faces or extensions such as a three "tine" fork configuration.

[0047] In use, when an object such as an endoscopic camera is secured by holder **100**, the rotational joints thereof are freely movable. However, once the camera is passed through a hole in a patient's skin, the camera may be aligned to provide the desired view through the use of curvilinear articulating arm assembly **12**. Because

the size of the entry hole in the patient's skin is limited, such an object disposed therein is unable to move substantially laterally, but may be angulated as by using arm assembly **12**.

[0048] Arm assembly **12** and holder **100** may be disposed in a sterile sleeve cover so that a sterile environment may be maintained for example when an endoscopic camera is coupled thereto and in use. Sterile covers for holder systems such as system **10** preferably are designed to cover the entire apparatus and slide on easily when articulating arm assembly **12** is in the semi-rigid "gooseneck lamp" mode (i.e. with only lever **682** locked, as will be explained). Such covers, preferably formed of transparent or semitransparent flexible polymer as known in the art, obviate the need for much cleaning and enable full function and use of system **10** in a sterile field. The scope retained by holder **100** is engaged by opening the spring-loaded slot between face **122f** and clamping portion **114** and working the mechanism of holder **100** through the cover, invaginating the cover into this slot with the scope then retained. The cover preferably withstands repeated engage/disengage cycles and scope rotations.

[0049] A variety of materials may be used to form the holder systems of the present invention. For example, components may be formed of polymer such as injection molded polymer, or metallic materials such as aluminum. Wherein springs are used, the springs for example may be formed of steel.

[0050] Although the center of second member **112** of holder **100** may be offset a distance d_1 from the central longitudinal axis of coupling portion **102** and body portion **104**, in some embodiments first member **108** may be configured so that the center of second member **112** may be aligned to be coaxial with the central longitudinal axis of coupling portion **102** and body portion **104**.

[0051] Turning to **FIGS. 3A-3G**, a second exemplary laparoscopic instrument holder **300** is shown. Holder **300** includes a coupling portion **302** in the form of a post that optionally may include a circumferential groove therein (not shown). Coupling portion **302** preferably is configured to be received in portion **82** of free handle **62** of articulating arm assembly **14**, as will be described later. Holder **300** includes a body portion **304** with a preferably cylindrical free end portion **306** forming a first rotational joint. In particular, a first member **308** is mounted on end portion **306** so that end portion **306** extends within a bore **308a** in first member **308**. In the preferred exemplary embodiment, there is minimal frictional resistance to rotational movement of portion **306** and first member **308** with respect to one another so that these components are freely rotatable with respect to one another. However, the tolerance between the components preferably is selected to minimize other play therebetween, and the coupling between the components preferably is such that minimal translation of one component with respect to the other component is permitted along their central axis of rotation.

[0052] In alternate devices, portion **306** and first member **308** are mechanically associated with each other such that frictional engagement of these components resists rotational movement of portion **306** and first member **308** with respect to each other. However, the frictional engagement preferably permits relative rotation of portion **306** and first member **308** when sufficient manual, external force is applied as by a using holder **300** surgeon during a medical procedure.

[0053] End portion **306** and first member **308** are disposed preferably at right angles with respect to each other. First member **308** preferably includes a cylindrical free end portion **310** forming a second rotational joint.

[0054] Holder **300** further includes a second member **312** that is mounted on end portion **310** so that end portion **310** extends within a bore **312a** in second member **312**. Again, in the preferred exemplary embodiment, there is minimal frictional resistance to rotational movement of portion **310** and second member **312** with respect to one another so that these components are freely rotatable with respect to one another. However, the tolerance between the components preferably is selected to minimize other play therebetween, and the coupling between the components preferably is such that minimal translation of one component with respect to the other component is permitted along their central axis of rotation.

[0055] In alternate devices, portion **310** and second member **312** are mechanically associated with each other such that frictional engagement of these components resists rotational movement of portion **310** and second member **312** with respect to each other. However, the frictional engagement preferably permits relative rotation of portion **310** and second member **312** when sufficient manual, external force is applied as by a surgeon using holder **300** during a medical procedure.

[0056] End portion **310** and second member **312** are disposed preferably at right angles with respect to each other.

[0057] Second member **312** includes a clamping portion **314** that may be arcuate such as U-shaped or may be another retaining shape such as V-shaped. In addition, a pair of holes **316** extend into second member **312** and are disposed on either side of central longitudinal axis **318** thereof. Holes **316** are configured and dimensioned to receive end portions of springs **320**, which extend out of holes **316**. Movable clamping jaws **322** are "spring loaded," with end faces **322a**, **322b** abutting ends of respective springs **320**. A set screw assembly **324** and respective washer **326** releasably and adjustably couples movable clamping jaws **322** to second member **312**. As shown for example in FIG. 3E, which shows a view with screw assembly **324** and washer **326** removed, a slot **328** guides movement of movable clamping jaws **322** along axis **318**, with the shaft portion of screw assembly **324** being threadably received in central threaded hole **330** in second member **312**. Oval shaped slot **328** permits limited movement, with the shaft of screw assembly **324**

being stopped from further movement at either end of slot **328**.

[0058] Clamping end faces **332a**, **332b** that are movable with respect to arcuate clamping portion **314** of second member **312**, and thus a variety of sizes and geometries of laparoscopic devices such as an endoscopic camera may be releasably retained within the region between clamping portion **314** and clamping end faces **332a**, **332b**. Although end faces **332a**, **332b** are shown in a bifurcated arrangement, other configurations may be used including a single clamping face such as a larger end face **332a** or **332b**, or more than two distinct end faces or extensions such as a three "tine" fork configuration.

[0059] In some devices, screw assembly **324** may include a threaded screw **324a**, a knurled thumb portion **324b**, and a set screw **324c** (shown in FIG. 3D) extending into the shaft of screw **324a**.

[0060] Holders **100**, **300** thus each incorporate a system of freely articulating joints and that supports a clamp for a laparoscope which may be aligned and attached along the long axis of the laparoscope. The instrument shaft may be held in alignment within the clamp opening by the spring-loaded clamp or in an alternate embodiment by using elastic band(s). The clamping mechanism of holders **100**, **300** preferably is of sufficient tension to hold the laparoscope in fixed alignment with the clamp body and yet allow rotation of the laparoscope about its long axis within the clamp. Proper functioning of this mechanism will allow for simple fixation of holder **100**, **300** to secure the laparoscope in a steady position without actually locking the individual joints in the universal system. Such a retention is permitted because the laparoscope shaft is firmly attached in three dimensions to the joint at the end of holder **100**, **300** and also passes through a second joint (the laparoscopic port) that is fixed in two dimensions at the skin. By positioning holder **100**, **300**, the camera may be positionally fixed unless the various frictional resistances previously set and controlled are overcome.

[0061] This design and method allows instantaneous and free movement and instant "re-locking" of the laparoscope position merely by relying on frictional resistance of the arm and clamp that is easily overcome for example by articulation by a surgeon, when desired, preferably by one handed positioning and re-positioning. Advantageously, this laparoscope holder system **100**, **300** is very simple mechanically, yet quick, reliable and easy to use. Also, it is a very quick and simple process to engage or disengage the laparoscope when desired.

[0062] The rotational joint provided, for example, by the coupling of end portion **310** and second member **312** preferably allows a 360° range of rotation, because the range of motion required for the laparoscope is extreme. Offsetting the points of rotation of the joints is one preferred design solution.

[0063] In use, a straight, rod-like laparoscope extends both above and below the point of attachment of any

clamp that is used to grasp it. Typically the laparoscope has power/light cords attached at the outer end that increase bulk in that region. Offsetting the rotational joints advantageously may permit better clearance between the outer end of holder **100, 300** proximate second member **112, 312** and the bulkier external end of the laparoscope.

[0064] Referring next to **FIGS. 3H to 3-O**, a third exemplary laparoscopic instrument holder **400** according to the present invention is shown.

[0065] Holder **400** includes a coupling portion **402** in the form of a post that optionally may include a circumferential groove therein (not shown). Coupling portion **402** preferably is configured to be received in portion **82** of free handle **62** of articulating arm assembly **14**, as will be described later. Holder **400** includes a body portion **404** with a preferably threaded hole **406** formed therein. A rotatable cradle **408** is mounted on a free end **404a** of body portion **404**, with a washer **410** disposed therebetween. A hole **412** with a upper broadened portion **412a** is disposed in cradle **408** and is configured and dimensioned to receive the shaft and head of a threaded screw **414**. Rotation of cradle **408** about longitudinal axis **416** is permitted.

[0066] In one exemplary devices, body portion **404**, washer **410**, and cradle **408** are mechanically associated with each other such that there is minimal frictional resistance to rotational movement between components so that cradle **408** and screw **414** are freely rotatable with respect to one another (screw **414** includes an unthreaded portion for this purpose). However, the tolerance between the components preferably is selected to minimize other play therebetween, and the coupling between the components preferably is such that minimal translation of one component with respect to the other component is permitted along their central axis of rotation. In alternate embodiments, frictional engagement of these components resists rotational movement of these components with respect to each other. However, the frictional engagement preferably permits relative rotation of portion **404** and first member **408** when sufficient manual, external force is applied as by a surgeon using holder **400** during a medical procedure.

[0067] Cradle **408** includes spaced, preferably parallel extensions **418** defining a space **420**. Aligned holes **422a, 422b** in respective extensions **418** receive a rod-shaped member **424** that extends therethrough. Member **424**, for example, may be press-fit in holes **422a, 422b** so as to be fixed therein. A first clamping portion **426** with a preferably generally C-shaped or arcuate face **426a** is mounted on member **424**, such as by member **424** extending through a hole in portion **426**. First clamping portion **426** is disposed between extensions **418** and is permitted to swivel on member **424** about swivel or rotational axis **428**.

[0068] In one exemplary, preferred device, there is minimal frictional resistance to rotational movement of member **424** and first clamping portion **426** with respect

to one another so that these components are freely rotatable with respect to one another. However, the tolerance between the components preferably is selected to minimize other play therebetween, and the coupling between the components preferably is such that minimal translation of one component with respect to the other component is permitted along their central axis of rotation.

[0069] In alternate devices, member **424** and first clamping portion **426** may be mechanically associated with each other such that frictional engagement of these components resists rotational movement of these components with respect to each other. However, the frictional engagement preferably permits relative rotation of member **424** and first clamping portion **426** when sufficient manual, external force is applied as by a surgeon using holder **400** during a medical procedure.

[0070] In a preferred device, axes **416, 428** are oriented perpendicular to one another.

[0071] Angulation of first clamping portion **426** on member **424** permits a laparoscopic device such as an endoscopic camera, schematically shown in **FIG. 3H** as component **430**, to be selectively positioned by a surgeon in a desired orientation.

[0072] Finally, a second clamping portion **432** is provided. Portion **432** preferably is elastic, and in one preferred exemplary embodiment is a resilient rubber o-ring. Advantageously, member **424** extends outward from extensions **418** such that a clamping portion **432** in the form of an o-ring may be demountably coupled proximate ends thereof. Member **424** may include a head or lip at each free end thereof to further assist in captivating clamping portion **432**. Thus, a component **430** may be releasably secured to holder **400** by: resting component **430** against first clamping portion **426** on surface **426a**, coupling a first loop section **434a** of second clamping portion **432** to member **424**, extending second clamping portion **432** over component **430**, and coupling a second loop section **434b** of second clamping portion **432** to member **424**.

[0073] Although a resilient o-ring is shown, other alternate embodiments include for example a flexible clip.

[0074] An alternate version of holder **400** is shown in **FIG. 3-O**. In this version, member **424** comprises a pair of opposing, aligned set screws **440**. Thus, clamping portion **426** swivels on an axis defined by screws **440**, with the screws extending in holes in clamping portion **426**. In addition, clamping portion **426** further includes a recessed portion **442** and a raised portion **444** separated by arcuate transition **446** on the outer sides of each extension **418**. Movement of clamping portion **426**, in some embodiments, may in part be guided by transition **446**, which also may provide a stop to prevent over-rotation of clamping portion **426** on member **440** but otherwise permits free and loose movement.

[0075] Another version of a holder **500** is shown in **FIG. 3P**. Holder **500** is similar to holder **400** with the rotatable body, however a one-piece Y-shaped cradle or yoke **508** is provided for use with an elastic clamping band as de-

scribed above. Rotation is permitted about axis **510** as indicated by **R₁**, and additional rotation is permitted about pivot region **P** disposed proximate axis **510** at and proximate the center of yoke **512**. In particular, an object such as an endoscopic camera **514** may rock transverse to axis **510**, for example in a plane through axis **510** and extending into and out of the page. As shown for example in **FIG. 3K**, an elastic band may be retained proximate regions **512a**, **512b**, extending over object **514**. In the preferred exemplary embodiment, tines **512** are rigid. However, in some alternate embodiments, tines **512** may have limited flexibility in positioning. In particular, a laparoscopic device such as an endoscopic camera could be held in the Y-axis using the elastic band.

[0076] In yet another device, shown in **FIGS. 3R-3S**, a holder system **550** includes a holder **551** with a clamping portion **552** for receiving a laparoscopic device such as an endoscopic camera (shown schematically as object **558**). Clamping portion **552** is mounted at one end of a body **554** with a split shaft **556**. Holder **551** is formed of unitary construction, and for example could be mounted on body portion **560** having a preferably unthreaded hole **562**. In particular, split shaft **556** may be releasably disposed in hole **562** so that body **554** and clamping portion **552** may rotate with respect to body portion **560**. Portion **556a** may be used to engage a suitably configured region in hole **562** (such as a ledge **564**) to releasably lock clamping system **550** in hole **562**. A coupling portion **566** in the form of a post may be provided as previously described with respect to other embodiments. Body **554** may rotate about central axis **567** in direction **R₂** as shown. In addition, further rotation may be provided by preferably rigid member **568** extending from body **554** to clamping portion **552**. Member **568** forms a living hinge and permits rotation in the form of rocking transverse to axis **567** and preferably in the plane of the page for the orientation shown in **FIG. 3S**. In a preferred exemplary embodiment, member **568** is rigid such that torsion about axis **567** is substantially resisted. Arms **570** serve as levers upon which a user may grasp with his or her fingers to assist in stabilizing the assembly during insertion or withdrawal of an object **558** such as an endoscopic camera from clamping portion **552**.

[0077] Portions of the holders described above, such as holder **551**, for example, could be made injection molded parts that could be made to function as described. Holder **551**, for example, may be a single-use, sterile, disposable component and thus in some embodiments a sterile drape for use with system **550** need only cover body portion **560** thereof and not holder **551**.

[0078] Referring next to **FIGS. 3AA-3EE**, another exemplary embodiment of a laparoscopic instrument holder **800** according to the present invention is shown. Holder **800** includes a coupling portion **802** in the form of a post that optionally may include a circumferential groove therein (not shown). Coupling portion **802** preferably is configured to be received in portion **82** of free handle **62** of articulating arm assembly **14**, as will be described later.

Holder **800** includes a body portion **804** coupled along axis **806** at a first rotational joint **808** to a first joint member **810**. In the exemplary embodiment, first rotational joint **808** may permit a 360° range of rotation about axis **806**.

[0079] In some devices, a series of rotational joints may be provided. In the exemplary device, first member **810** is coupled along an axis **812** at a second rotational joint **814** to a second joint member **816**. Second rotational joint **814** may permit a 360° range of rotation about axis **812**. Second joint member **816** is coupled along an axis **818** at a third rotational joint **820** to a third joint member **822**. Third rotational joint **820** may permit a 360° range of rotation about axis **818**.

[0080] Holder **800** further includes a linear length adjustment portion **824**, which will be described shortly. In the exemplary embodiment, portion **824** is coupled along an axis **826** at a fourth rotational joint **828** to third joint member **822**. Preferably, fourth rotational joint **828** is disposed proximate a free end of portion **824**.

[0081] In one preferred exemplary device, axes **806**, **812** are disposed at about 90° with respect to each other, axes **812**, **818** are disposed at about 90° with respect to each other, and axes **818**, **826** are disposed at about 90° with respect to each other. In addition, the combination of rotational joints **808**, **814**, **820**, **828** permit movement in four separate planes, it being possible for at least one pair of said planes (e.g., as defined by joints **808**, **820** or as defined by joints **814**, **828**) to be parallel to one another and it also being possible for there to be two pairs of parallel planes provided by the joints (e.g., as defined by joints **808**, **820** and as defined by joints **814**, **828**). The combination of rotational joints **808**, **814**, **820**, **828** also preferably permits movement in four separate planes which may be nonparallel to one another.

[0082] In the exemplary device, linear length adjustment portion **824** forms a sliding mechanism in which a first sliding member **830** is coupled to a second sliding member **832** and slidably associated with one another. Preferably, constant friction sliding is provided by members **830**, **832**. Also in the exemplary embodiment, members **830**, **832** are restricted to move with respect to one another along central sliding axis **834**.

[0083] Member **830** for example may be coupled to a coupling portion **836** such as with a plurality of screws **838**. Preferably, coupling portion **836** is configured and dimensioned to be received and slide in a grooved portion or track **832a** formed in member **832**. Members **830**, **832** may be coupled to one another with a set screw **839** which extends through and is permitted to translate along the length of slot **840** in member **832**. The shaft of set screw **839** extends into member **834**. In some embodiments, set screw **839** may be tightened so that the head thereof bears against member **832** to adjust the friction between the members **830**, **832** with respect to each other.

[0084] In alternate devices, the shaft of set screw **839** and the width of slot **840** may be sized so that if no coupling portion **836** is provided, movement of members **830**,

832 is guided along axis **834**.

[0085] Another rotational joint **842** is disposed proximate the free end of portion **824** opposite the free end at which rotational joint **828** is disposed. Joint **842** is disposed along an axis **844**. In particular, an extension **830a** of member **830** is coupled along axis **844** at rotational joint **842** to a joint member **846**. Rotational joint **842** may permit a 360° range of rotation about axis **844**. Preferably, axes **834**, **844** are parallel and disposed in different planes.

[0086] Joint member **846** is coupled along an axis **848** at yet another rotational joint **850** to a laparoscopic device retaining portion **852**. Rotational joint **850** may permit a 360° range of rotation about axis **848**. Laparoscopic device retaining portion **852** for example may be a clamp formed by a pair of jaw members **852a**, **852b** that are spring biased toward one another with a spring **852c** at a laparoscopic device grasping region **852d**. Preferably, laparoscopic device grasping region **852d** is sized to receive a laparoscopic device such as an endoscopic camera, shown schematically as device **854**. Thus, grasping region **852d** may be sized, for example, to grasp a 5 mm and/or 10 mm laparoscope. In the exemplary embodiment, axes **844**, **848** are disposed at about 90° with respect to each other.

[0087] Retaining portion **852** preferably may be used to secure the shaft portion of a laparoscopic device such as an endoscopic camera. A sterile sleeve drape may be used to cover the entire apparatus and to be imbricated into grasping region **852d**. Preferably, while spring-biased jaw members are configured to hold the laparoscopic device securely, they also permit the device to be manually rotated about its linear axis with enough frictional resistance to prevent undesired rotational movement.

[0088] The rotational joints of holder **800** such as rotational joints **814**, **816** for example may be formed as follows. A threaded screw **856** is disposed with the head thereof abutting a first washer **858a** which optionally rests on a second washer **858b**. Washers **858a**, **858b** rest on a ledge such as ledge **860** in member **816**. The shaft of screw **856** extends through coaxial holes **862**, **864** in adjacent components such as members **810**, **816**, and is threadably received in a nut **866** that rests against a washer **868** abutting ledge **870** in member **810**. Members **810**, **816** may be separated from one another with a washer **872**. A sleeve **874** optionally may be provided with a hole therein through which the shaft of screw **856** extends and is guided. Sleeve **874** may be disposed proximate the head of screw **856** or remote from the head.

[0089] Thus, laparoscopic device **854** may be positioned as desired using the combined freedom of movement provided by rotational joints **808**, **814**, **820**, **828**, **842**, **850**, linear length adjustment portion **824**, as well as the rotation provided by coupling portion **802** when received in portion **82** of free handle **62** of articulating arm assembly **14**.

[0090] In one preferred exemplary device, holder **800**

moves with five degrees of freedom, with the sixth degree being accommodated by rotation of laparoscopic device **854** within laparoscopic device retaining portion **852**. Preferably, frictional movement is provided by rotational joints **808**, **814**, **820**, **828**, **842**, **850**, linear length adjustment portion **824**, as well as coupling portion **802** when received in portion **82** of free handle **62** of articulating arm assembly **14**. Preferably, the friction is sufficient to hold the laparoscopic device regardless of orientation but selected so that the device is easily movable for re-orientation through manual manipulation by a user. Higher frictional resistance to allow for movement of the working envelope may be provided by curvilinear articulating arm assembly **12**, as described herein. It should be noted, however, that the ease of movement between relatively moving components may be selected as desired as a function of the friction between said components. Thus, different embodiments of holder **800** may be provided with different amounts of friction for rotational joints **808**, **814**, **820**, **828**, **842**, **850**, linear length adjustment portion **824**, as well as coupling portion **802**.

[0091] Turning next to FIGS. 3FF to 3-UU, yet another exemplary device of a laparoscopic instrument holder **900** is shown. Holder **900** includes a coupling portion **902** in the form of a post that optionally may include a circumferential groove therein (not shown). Coupling portion **902** preferably is configured to be received in portion **82** of free handle **62** of articulating arm assembly **14**, as will be described later. Holder **900** includes a body portion **904** coupled along axis **906** at a first rotational joint **908** to a first joint member **910**. In the exemplary embodiment, first rotational joint **908** may permit a 360° range of rotation about axis **906**.

[0092] In some devices, a series of rotational joints may be provided. In the exemplary embodiment, first member **910** is coupled along an axis **912** at a second rotational joint **914** to a second joint member **916**. Second rotational joint **914** may permit a 360° range of rotation about axis **912**. Second joint member **916** is coupled along an axis **918** at a third rotational joint **920** to a linear length adjustment portion **924**, which will be described shortly. Third rotational joint **920** may permit a 360° range of rotation about axis **918**. Preferably, third rotational joint **914** is disposed proximate a free end of portion **924**.

[0093] In one preferred exemplary device, axes **906**, **912** are disposed at about 90° with respect to each other, and axes **912**, **918** are disposed at about 90° with respect to each other. In addition, the combination of rotational joints **908**, **914**, **920** permits movement in three separate planes, it being possible for at least one pair of said planes (e.g., as defined by joints **908**, **920**) to be parallel to one another. The combination of rotational joints **908**, **914**, **920** also preferably permits movement in three separate planes which may be nonparallel to one another.

[0094] In the exemplary device, linear length adjustment portion **924** forms a sliding mechanism in which a first sliding member **930** is coupled to a second sliding member **932** and slidably associated with one another.

Preferably, constant friction sliding is provided by members **930**, **932**. Also in the exemplary embodiment, members **930**, **932** are restricted to move with respect to one another along central sliding axis **934**. Advantageously, linear length adjustment portion **924** permits a user to reposition a laparoscopic device **954**, for example into and out of an opening in a patient, with gross movement in a linear direction, as compared to angulation. For example, linear length adjustment portion **924** may permit about 6 inches of linear movement of a device **954** held by holder **900**.

[0095] Member **930** may be provided with a first slot **930a** and member **932** may be provided with a second slot **932a**, with each of slots **930a**, **932a** being disposed centrally along axis **934**. First and second slots **930a**, **932a** each may have a length S_1 , S_2 , respectively, along axis **934**, and lengths S_1 , S_2 may be about the same as one another. In an exemplary preferred embodiment, lengths S_1 , S_2 each may be about 5.5 inches. In the preferred exemplary embodiment, members **930**, **932** are coupled to each other by coupling assemblies **936** extending from fixed positions with respect to and proximate free ends **930b**, **932b** thereof.

[0096] Each coupling assembly **936** includes a female threaded round standoff **936a** that threadably receives truss head Phillips machine screws **936b**, **936c** at opposing ends thereof. Standoff **936a** extends through a plain bearing **936d** which is sized to slide and be guided in a respective slot **930a**, **930b** generally constrained for movement along axis **934**. Bearing **936d** extends through a plastic thrust bearing **936e** positioned between members **930**, **932**. A member **930**, **932** is captivated between plastic thrust bearing **936e** and a second plastic thrust bearing **936f**. A stainless steel round flat washer **936g** and a curved disc spring **936h** are provided between bearing **936f** and the head of screw **936c** as shown, with bearing **936d** abutting washer **936f**. Spring **936h** maintains tension between thrust bearings **936e**, **936g**. Finally, another curved disc spring **936i** is provided and seats in a recess **930c** or **932c** of a member **930**, **932**, respectively. Curved disc spring **936i** allows for greater machining tolerances for recesses **930c**, **932c** and preferably keeps bearing **936d** in contact with washer **936f**. Coupling assemblies **936** thus allow some adjustment of tensioning so that a desired level of force permits movement of members **930**, **932** with respect to one another. By loosening or tightening each of assemblies **936**, frictional resistance to sliding or telescoping of members **930**, **932** with respect to each other may be selected.

[0097] Another rotational joint **942** is disposed proximate the free end of portion **924** opposite the free end at which rotational joint **920** is disposed. Joint **942** is disposed along an axis **944**. In particular, an extension **930a** of member **930** is coupled along axis **944** at rotational joint **942** to a joint member **946**. Rotational joint **942** may permit a 360° range of rotation about axis **944**. Preferably, axes **934**, **944** are parallel and disposed in different

planes.

[0098] Joint member **946** is coupled along an axis **948** at yet another rotational joint **950** to a laparoscopic device retaining portion **952**. Rotational joint **950** may permit a 360° range of rotation about axis **948**. Laparoscopic device retaining portion **952**, for example, may be a clamp formed by a pair of jaw members **952a**, **952b** with a laparoscopic device grasping region **952d** formed by jaw portions that are spring biased toward one another and handle regions that are spring biased away from one another, the biasing accomplished using a spring **952c**. Preferably, laparoscopic device grasping region **952d** is sized to receive a laparoscopic device such as an endoscopic camera, shown schematically as device **954**. Thus, grasping region **952d** may be sized, for example, to grasp a 5 mm and/or 10 mm laparoscope (as shown in FIG. 3-OO, two cylindrical regions are sized for this purpose). In the exemplary embodiment, axes **944**, **948** are disposed at about 90° with respect to each other.

[0099] In order to provide sufficient clamping strength so that a laparoscopic device **954** may be securely and releasably retained within grasping region **952d** of retaining portion **952**, without undesired slippage or rotation, a strong spring mechanism is provided. In particular, as shown in FIGS. 3PP-3UU, spring **952c** in part elastically biases jaw members **952a**, **952b** toward one another so that grasping region **952d** is in a closed position. In the preferred exemplary device, spring **952c** is a Type 302 stainless steel torsion spring providing a torque of about 21 in.-lbs. (McMaster-Carr part number 9287K103 with the following characteristics: 90° deflection angle clockwise wound, spring outer diameter about 0.9 inch, wire diameter about 0.1 inch, length about 3.5 inches, maximum rod outer diameter about 0.5 inch, body length/spring length at torque about 0.6 inch, and about 3.25 active coils). However, in alternate embodiments, other elastic members instead of a torsion spring may be used and other spring characteristics may be specified as long as proper retention is provided in region **952d**. Thus, even forces due to power cords, etc., that may be associated with a laparoscopic device **954** may be sufficiently countered while device **954** is disposed in grasping region **952d**.

[0100] Because of the substantial torque provided by spring **952c** to securely retain a laparoscopic device **954** in grasping region **952d**, a user may need very significant hand strength to be able to compress the handle portions of jaw members **952a**, **952b** toward one another. To enhance usability in view of the torque of spring **952c**, jaw member **952a** has a forked, bifurcated design with a first portion **952a₁** having a U-shaped region that receives a second portion **952a₂**. A first pin **953a** pivotally associates portions **952a₁** and **952a₂** to one another, while a second pin **953b** pivotally associates second portion **952a₂** to lever link **955**. Lever link **955** is further pivotally associated with jaw member **952b** with a third pin **953c**. A boss **959a** of first portion **952a₁** with a through hole therein is received in the through hole of a boss **959b** of

jaw member **952b** and these jaw members **952a**, **952b** are coupled to one another with a screw **957a** that extends in the through hole of boss **959a** and tightly abuts a coaxial set screw **957b**. Spring **952c** is disposed about boss **959b** with one leg resting against ledge **961a** and the other leg resting against ledge **961b** of jaw members **952a**, **952b**, respectively. During operation, in order to open grasping region **952d**, a user may grasp in one hand and squeeze (1) portion **952a₁** of jaw **952a** which forms a first handle region and (2) jaw member **952b** which forms a second handle region. The use of a jaw member **952a** having portions **952a₁** and **952a₂** as well as lever link **955** provides a mechanical advantage to the user when changing the size of the openings in grasping region **952d**, e.g. to allow insertion or release of a laparoscopic device **954** therein. Preferably, the mechanical advantage is such that the turning force applied by a user to move jaw members **952a**, **952b** with respect to one another is less than half the turning force otherwise required for the spring **952c**.

[0101] In an exemplary preferred devices, when jaw members **952a**, **952b** are closed as shown in FIGS. 3PP and 3QQ, portion **952a₂** is separated from portion **952b** by an angle **J** of about 35°.

[0102] Retaining portion **952** preferably may be used to secure the shaft portion of a laparoscopic device such as an endoscopic camera. A sterile sleeve drape may be used to cover the entire apparatus and to be imbricated into grasping region **952d**. Preferably, while spring-biased jaw members are configured to hold the laparoscopic device securely, they also permit the device to be manually rotated about its linear axis with enough frictional resistance to prevent undesired rotational movement.

[0103] The rotational joints of holder **900** such as rotational joints **914**, **920** for example may be formed as follows. An internally threaded bolt **956** is disposed with the head thereof abutting a first washer **958a**. The washer **958a** abuts a first side of a joint member such as member **916** while a second washer **958b** abuts an opposite side of member **916** with bolt **956** extending therethrough. The shaft of bolt **956** extends through hole **962** and a coaxial hole in an adjacent component such as member **932**. An externally threaded bolt **964** is threadably received in internally threaded bolt **956**.

[0104] In another exemplary device, the rotational joints of holder **900** such as rotational joints **908**, **914**, **920**, **942**, **950** for example may be formed with thrust bearings as follows. Although in FIGS. 3W and 3WW an exemplary rotational joint **920** is shown, the construction of this joint also may reflect the construction of exemplary rotational joints **908**, **914**, **942**, **950** according to this embodiment. Rotational joint **920** couples joint member **916** and sliding member **932** (shown in phantom). Joint **920** includes a central screw **970** which is threadably received in a threaded hole **916a** in joint member **916**. A Belleville or conical washer **972** abuts head **970a** of screw **970** as well as a steel ball thrust bearing **974** (which for example

may be carbon steel or stainless steel). Washer **972** creates a spring tension to broaden the window of adjustability of holder **900** during assembly and accommodates slight wear that may occur in operation of holder **900**. In turn, thrust bearing **974** is mounted on a sleeve **976** which extends from within a central opening in thrust bearing **974** to within a recessed region in joint member **916**. Rotational joint **920** further includes a pair of washers **978**, **980**, preferably formed of stainless steel, and a spacer **982** disposed therebetween, together mounted on sleeve **976**. Washer **978** abuts and preferably is bonded to joint member **916** while washer **980** abuts and preferably is bonded to sliding member **932**. Washers **978**, **980** may rotate freely with respect to spacer **982**. Spacer **982** for example may be formed of Delrin® AF Blend (Acetal homopolymer, PTFE-filled). As is known in the art, a high performance miniature steel ball thrust bearing **974** for example may be formed of a pair of precision chrome-steel washers **974a**, **974b** and a ball cage **974c** that is bronze or stainless steel with steel balls **974d** disposed therein (e.g., McMaster-Carr part number 7806K63). In use, rotational joint **920** advantageously accommodates thrust loads - it can accommodate axial thrust along the axis of the "shaft" it supports - while also providing desired rotational movement between joint member **916** and sliding member **932**. Although a steel ball thrust bearing **972** is shown, other types of thrust bearing constructions instead may be used, and also other types of bearings instead may be used. Moreover, although rotational joint **920** with thrust bearing **972** has been shown in the exemplary context of joint member **916** and sliding member **932**, in the present embodiment such joint constructions with thrust bearings may be used in one or more, and preferably each of rotational joints **908**, **914**, **920**, **942**, **950**.

[0105] While holder **900** for example is shown in FIGS. 3FF and 3GG with a coupling portion **902** in the form of a post that couples to body portion **904**, another exemplary embodiment of a coupling portion **990** coupled to body portion **904** is shown in FIGS. 3XX-3ZZ. Coupling portion **990** is configured, for example, as an adaptor for coupling holder **900** to other types of arrangements as known in the art. Thus, holder **900** may be attached to a variety of positioning arms not limited for example to the curvilinear articulating arm assembly **12** in FIG. 1. Portion **990** includes a central hole **992** that receives a projection **904a** extending from an end of body portion **904**. Body portion **904** and coupling portion **990** are further aligned with a pin **994** extending in holes in portions **904**, **990** that are coaxial when in alignment with one another. An interface lock **996** extends into member **990a** of coupling portion **990** and is rotatably associated with projection **904a** of body portion **904**. Interface lock **996** for example may include a knurled knob portion **996a**, a cylindrical post **996b**, a sleeve **996c**, and a set screw **996d**. Exemplary operation of such an interface lock **996** is described elsewhere herein with respect to an interface lock **683** shown in FIG. 4U.

[0106] Thus, laparoscopic device **954** may be positioned as desired using the combined freedom of movement provided by rotational joints **908, 914, 920, 942, 950**, linear length adjustment portion **924**, as well as the rotation provided by coupling portion **902** when received in portion **82** of free handle **62** of articulating arm assembly **14**.

[0107] Preferably, frictional movement is provided by rotational joints **908, 914, 920, 942, 950**, linear length adjustment portion **924**, as well as coupling portion **902** when received in portion **82** of free handle **62** of articulating arm assembly **14**, as described with respect to holder **800** above. Preferably the friction is sufficient to hold the laparoscopic device regardless of orientation but selected so that the device is easily movable for re-orientation through manual manipulation by a user. Preferably, when a user positions a laparoscopic device **954** using holder **900**, the rotational and linear movements provided by the components of holder **900** provide a generally uniform feel to the user. In other words, during manual manipulation of a device **954** coupled to holder **900**, it feels to the user as though the user encounters the same degree of resistance to movement of the laparoscopic device **954** regardless of the direction in which device **954** is moved/oriented. In one exemplary preferred embodiment, rotational joints **908, 914, 920** proximate coupling portion **902** for interfacing with articulating arm assembly **14** may have about two times the frictional resistance to movement as rotational joints **942, 950** proximate laparoscopic device retaining portion **952**.

[0108] Next, with reference to **FIGS. 3AAA-3HHH**, embodiment of a laparoscopic instrument holder **1000** according to the present invention is shown. As with previous embodiments, in an exemplary embodiment holder **1000** includes three rotational axes at a proximal end and two rotational axes at a distal end. Holder **1000** includes a coupling portion **1002** in the form of a post. Coupling portion **1002** preferably is configured to be received in portion **82** of free handle **62** of articulating arm assembly **14**, as will be described later. Holder **1000** includes a body portion **1004** coupled along axis **1006** at a first rotational joint **1008** to a first joint member **1010**. In the exemplary embodiment, first rotational joint **1008** may permit a 360° range of rotation about axis **1006**.

[0109] In the embodiments, a series of rotational joints are provided. In the exemplary embodiment, first member **1010** is coupled along an axis **1012** at a second rotational joint **1014** to a second joint member **1016**. Second rotational joint **1014** may permit a 360° range of rotation about axis **1012**. Second joint member **1016** is coupled along an axis **1018** at a third rotational joint **1020** to a linear length adjustment portion **1024**, which will be described shortly. Third rotational joint **1020** may permit a 360° range of rotation about axis **1018**. Preferably, third rotational joint **1014** is disposed proximate a free end of portion **1024**.

[0110] In one preferred exemplary embodiment, axes **1006, 1012** are disposed at about 90° with respect to

each other, and axes **1012, 1018** are disposed at about 90° with respect to each other. In addition, the combination of rotational joints **1008, 1014, 1020** permits movement in three separate planes, it being possible for at least one pair of said planes (e.g., as defined by joints **1008, 1020**) to be parallel to one another. The combination of rotational joints **1008, 1014, 1020** may permit movement in three separate planes which may be non-parallel to one another.

[0111] In the exemplary embodiment, linear length adjustment portion **1024** forms a sliding mechanism in which a generally tubular first sliding member **1030** is coupled to a generally tubular second sliding member **1032** and are slidably associated with one another. Portion **1024** forms an extendable section of holder **1000** that for example provides adjustability to the length of holder **1000**. In the exemplary embodiment, members **1030, 1032** are restricted to move with respect to one another along central sliding axis **1034**. Advantageously, linear length adjustment portion **1024** permits a user to reposition a laparoscopic device **1054**, for example into and out of an opening in a patient, with gross movement in a linear direction, as compared to angulation. For example, linear length adjustment portion **1024** may permit about 5 or about 6 inches of linear movement of a device **1054** held by holder **1000**.

[0112] Member **1030** preferably is received within, and telescopes with respect to member **1032**. As shown in **FIG. 3CCC**, member **1032** is hollow and is provided with a slot **1032a**. A roller key **1034a** is secured to member **1030** with a rivet **1034b**; a piston member **1036** is coupled to a free end of member **1030** (see **FIG. 3EEE**) and rivet **1034b** extends in a coaxially disposed holes **1036a, 1030a** in members **1036, 1030** respectively. Roller key **1034a** coupled to member **1030** is movable within slot **1032a** of member **1032** and preferably is a miniature high precision stainless steel ball bearing. A cover **1037** may be secured to member **1032** over slot **1032a**, for example, for safety and aesthetic reasons. Member **1032** also may be provided with a bushing **1038** to provide support for member **1030** and to assist in preventing a sterile sleeve drape covering holder **1000** from being caught during movement of member **1030** with respect to member **1032**. Bushing **1038** includes a plurality of fingers **1038a** disposed radially with respect to axis **1034**. Advantageously, the use of fingers **1038a** allows an adequate interference fit to be provided with minimal drag between fingers **1038a** and the outer surface of member **1030** to prevent the sterile sleeve drape covering holder **1000** from being inadvertently caught during movement. Bushing **1038** may be formed, for example, of Delrin® AF Blend (Acetal homopolymer, PTFE-filled).

[0113] As shown in **FIG. 3EEE**, piston member **1036** is spring-loaded. In particular, a spring **1036b** and a plunger **1036c** are disposed within a hollow cylindrical region **1036d** in piston member **1036** for movement along axis **1036e**. Preferably axis **1036e** is disposed perpendicular to axis **1034**. By providing the spring/plunger ar-

rangement, a consistent drag force by may be provided for movement of members **1030**, **1032** with respect to each other as plunger **1036c** bears against the inner wall of member **1032**. In an exemplary embodiment, the following components and materials may be used: spring **1036b** may be stainless, 1/2" long x 0.36" OD x 0.032" wire; the plunger may be 0.43" long with an OD of 0.375 and may be made of Delrin® AF Blend; the depth of the hole in the piston may be 3/4" and the diameter of the piston may be 0.86", sized for clearance to the ID of member **1032**.

[0114] Turning back to **FIG. 3AAA**, another rotational joint **1042** is disposed proximate the free end of member **1030** opposite the free end of member **1032** at which rotational joint **1020** is disposed. Joint **1042** is disposed along axis **1034**. Rotational joint **1042** may permit a 360° range of rotation about axis **1034**. Joint member **1046** is coupled along an axis **1048** at yet another rotational joint **1050** to a laparoscopic device retaining portion **1052**. Rotational joint **1050** may permit a 360° range of rotation about axis **1048**. Laparoscopic device retaining portion **1052**, for example as shown in **FIG. 3HHH**, may be a clamp formed by a pair of jaw members **1052a**, **1052b** with a laparoscopic device grasping region **1052d** formed by jaw portions that are spring biased toward one another and handle regions that are spring biased away from one another, the biasing accomplished using a spring **1052c**. Preferably, laparoscopic device grasping region **1052d** is sized to receive a laparoscopic device such as an endoscopic camera, shown schematically as device **1054**. Preferably, grasping region **1052d** is formed by material softer than aluminum to prevent marring or denting of surfaces of delicate laparoscopic device **1054** which typically is thin-walled. In the exemplary preferred embodiment, polyurethane covers **1052e** are provided. Covers **1052e** for example may be formed of 85 or 95 durometer polyurethane, permitting devices **1054** to even be twisted out of grasping region **1052d** without damage occurring. In the exemplary embodiment, axes **1034**, **1048** are disposed at about 90° with respect to each other.

[0115] Further details concerning retaining portion **1052** were previously provided in the context of retaining portion **952** of a previous embodiment.

[0116] Thus, retaining portion **1052** preferably may be used to secure the shaft portion of a laparoscopic device such as an endoscopic camera. A sterile sleeve drape may be used to cover the entire apparatus and to be imbricated into grasping region **1052d**. Preferably, while spring-biased jaw members are configured to hold the laparoscopic device securely, they also permit the device to be manually rotated about its linear axis with enough frictional resistance to prevent undesired rotational movement.

[0117] An exemplary rotational joint **1014** is shown in **FIG. 3GGG**. Each of joints **1008**, **1014**, **1020** for example may have the same construction, and joint **1014** is described in particular. Although similar to these joints, the joints **1042**, **1050** proximate retaining portion **1052** have

similar constructions to joint **920** shown in **FIGS. 3VV-3WW** a previously described (e.g., with two stainless steel washers and a Delrin® AF Blend spacer therebetween that is not bonded to its surroundings). However, as will be described, components in these various joints may be formed of different materials depending on whether the joint is located near the proximal or distal end of holder **1000**.

[0118] In a preferred exemplary embodiment, joint **1014** may include a thrust bearing. Rotational joint **1014** couples joint member **1010** to joint member **1016** (shown in phantom). Joint **1014** includes a central screw **1070** which is threadably received in a threaded hole **1010a** in joint member **1010**. A pair of Belleville or conical washers **1072** are disposed proximate head **1070a** of screw **1070** as well as a high performance miniature steel ball thrust bearing **1074** that for example may be formed of a pair of precision chrome-steel washers **974a**, **974b** and a ball cage **974c** that is bronze or stainless steel with steel balls **974d** disposed therein (e.g., McMaster-Carr part number 7806K63). In turn, thrust bearing **1074** is mounted on a sleeve **1076** which extends from within a central opening in thrust bearing **1074** to within a recessed region in joint member **1016**. Rotational joint **1014** further includes a washer **1078** preferably formed of stainless steel and a spacer **1082** adjacent sleeve **1076**. Washer **1078** abuts joint member **1010**. Washer **1078** preferably is bonded to joint member **1010** while spacer **1082** preferably is bonded to joint member **1016**, it being possible for washer **1078** and spacer **1082** to rotate with respect to each other. The use of such a joint with a thrust bearing was described previously with respect to joint **920** of another embodiment, and the previous description also applies to this embodiment.

[0119] In a preferred exemplary embodiment, members **1030**, **1032** are formed of 6061-T6 aluminum due to the strength to weight ratio of this material. However, other materials could be used for example thin wall steel. Washers such as washers **1072** may be formed of stainless steel.

[0120] The spacers such as spacer **1082** in rotational joints **1008**, **1014**, **1020** at the proximal end may be formed of Multifil™ sliding bearing material which is polytetrafluoroethylene (PTFE)-based and available from GGB North America LLC. Advantageously, the Multifil material has low stiction for the present application - it shows almost no signs of "sticking" in the operating conditions of holder **1000**. On the other hand, the spacers in the rotational joints at the distal end such as joints **1042**, **1050** may be formed of Delrin® AF Blend (Acetal homopolymer, PTFE-filled). Different materials were used for the spacers at the proximal and distal ends for several reasons. First, Multifil was only available in a limited range of thicknesses. Because the spacers at the proximal end were of relatively large diameters (11/8 inch), forces against the spacers could be spread over this relatively large area thus allowing a "smaller" thickness of spacer to be used without risking plastic defor-

mation. The spacers at the distal end proximate retaining portion **1052** have comparatively small diameters (3/4 inch), and thus "larger" spacer thickness was needed to accommodate forces on these spacers without risking plastic deformation. Multifil was not available in the thickness needed for the spacers at the distal end and thus another material (Delrin® AF Blend) was chosen. Second, stiction appeared to be more of an issue in joints at the proximal end near body portion **1004** (than in joints proximate retaining portion **1052**); Multifil thus was the preferred material for addressing stiction concerns.

[0121] In an exemplary embodiment, holder **1000** may have a fully telescoped length of about 19.5 inches as measured from the first rotational joint **1008** at the proximal end proximate body portion **1004** to the center of the clamp jaw cover **1052e**; the unextended length of holder **1000** may be about 14.25 inches. Thus, telescoping action may provide about 5 to about 5.5 inches of adjustment in length of holder **1000**.

[0122] Joints **1008, 1014**, and **1020** each are set to about 2 ft-lbs of torque, while joint **1042** is set to about 0.8 ft-lbs of torque and joint **1050** is set to about 1.2 ft-lbs of torque. The telescoping action of members **1030, 1032** may be set to have about an axial force of about 1 lb.

[0123] In use, the port in a patient into which a device **1054** is introduced may serve as a fulcrum. The clamp of holder **1000** preferably is capable of holding about 1/4 lb. of weight from device **1054** when holder **1000** is fully extended. Although a typical endoscopic scope may weigh about 1/4 lb., various cables associated with the scope increase the weight that must be supported. However, support is further provided by the port formed in the body into which the scope is inserted, helping to assist in accommodating the additional weight.

[0124] The rotational joints described herein, for example, may permit limited rotation such as rotation through an angle of about 180° or an angle of about 270°, or may permit about 360° of rotation about an axis of the rotational joint.

[0125] Next, an exemplary method of using holder **900** is described although this method applies to other holders described herein such as holder **1000**. In use, the position of holder **900** should be checked for suitable working range near the planned camera port site. The optimum attachment point for the articulating arm assembly **14** for example on a surgical bed railing should be determined after the patient is positioned and asleep and before the prep. Initially, linear length adjustment portion **924** need not be telescoped, although portion **924** should be fully extended for draping. Assembly **14** should be oriented to near vertical for prepping and draping the patient and the arm. The drape for assembly **14** preferably should be placed after the skin prep but before the final large procedure drape is placed. A separate skirt/ half-sheet drape may be clipped around the base of the system after the large patient drape is placed. Assembly **14** then should be contoured closely to the patient to mini-

mize its footprint and brought adjacent to the camera port. In use, the assembly **14** should be closely contoured to the patient and holder **900** disposed approximately parallel to the skin (perpendicular to the port) to minimize interference and clutter. Also, although it is possible that in one combination joints **910, 914, 920** may be aligned generally in the same plane, it is desirable to have at least one of these joint out of plane relative to the others to start. If the laparoscopic device **954** is an endoscopic camera, preferably the shaft of the device is grasped in clamp **952** as close as possible to the camera body. A laparoscopic device **954** coupled to holder **900** may be moved, for example, in six degrees of freedom with the combination of rotational joints **942, 950** and grasping region **952d** of clamp **952** which permits rotation of device **954** therein.

[0126] Holders **100, 300, 400, 500, 800, 900, 1000** and clamping system **550** preferably may be provided with a full cover sleeve drape. Devices **100, 300, 400, 500, 550, 800, 900, 1000** may be formed as a single use, pre-sterilized device, or as a sterilizable, re-usable device, or as a non-sterile re-usable device that is covered by a sterile drape/cover when required. Portions of devices **100, 300, 400, 500, 550, 800, 900, 1000** may be disposable.

[0127] In one exemplary, preferred embodiment, the holders of the present invention may be designed to create a minimum footprint or minimum interference within the surgical field and be easily sterilized or protected by a sterile cover. The holders preferably are long enough to reach from an attachment point on or proximate the location of a bedside railing to well past the skin entry port of a patient to allow for a full range of movement of the laparoscope, and to have enough pathway variability to clear other objects in the surgical field.

[0128] Some embodiments of holders may have several modes of operation. One mode may be free movement with little resistance at the free end. A second mode may be moderate resistance at the free end. This may be most useful when holding an endoscopic camera. In this instance, the resistance in this second mode preferably should be sufficient to maintain camera position in the absence of additional external force while at the same time being weak enough to allow a complete range of three-dimensional manipulation by the surgeon or assistant using only one hand without the need to adjust any locking or unlocking mechanism. A third mode may be fully locked with high resistance to movement at the free end. This mode may be particularly useful in the case where greater force may be required, such as retraction of an internal structure or organ. In this circumstance, an instrument connection other than, or in addition to the rotational joints disclosed herein, may be used.

[0129] As described above, coupling portion **302** of holder **300** and coupling portion **402** of holder **400** preferably are configured to be received in portion **82** of free handle **62** of articulating arm assembly **14**. This articulating arm assembly now will be described.

[0130] Turning to **FIGS. 4A-4C**, an exemplary pre-

ferred curvilinear articulating arm assembly **12** is shown for use with a laparoscopic instrument holder **14**. Arm assembly includes a central arm **652** with a ball-sleeve arrangement that forms joints. In particular, central arm **652** includes a plurality of sleeves **654** with spherical balls **656** disposed therebetween thus forming ball and socket connections. In the exemplary device shown in the figures, three balls **656a** of a first size are disposed adjacent one another proximate one end of arm **652**, while the remaining balls **656b** are of a second size smaller than the first size. Sleeves **654a** of a first size and sleeves **654c** of a second size smaller than the first size are provided for accommodating balls **656a**, **656b**, respectively, while a transition sleeve **654b** is provided intermediate sleeves **654a**, **654c** as shown for accommodating a ball **656a** on one side and a ball **656b** on the other side thereof. Sleeves **654** are configured and dimensioned to receive balls **656a**, **656b** at ends thereof and thus permit articulating of sleeves with respect to each other. A tensioning wire **658** runs generally centrally through sleeves **654** and balls **656**, as will be further described shortly. Preferably, wire **658** is formed of metal. In an exemplary preferred embodiment, wire **658** is Type 302 stainless steel wire rope, 1x19 strand, 5/32 inch diameter, with a breaking strength of 3300 lb. (McMaster-Carr part number 3458T27). One exemplary operation of a wire tensioning mechanism is shown and described in U.S. Patent No. 3,858,578 to Milo, which is expressly incorporated herein by reference thereto. Preferably, curvilinear articulating arm assembly **12** may move with six degrees of freedom.

[0131] In the exemplary preferred device, three additional balls **656a** and three additional sleeves **654a** are provided to the arm assembly **12** shown in FIGS. 4A-4C, with arm assembly **12** having a fully extended (straightened) length of about 40 inches. End effector **14**, for example, may add about 4 inches to the length of the arm assembly **12**. In other embodiments, other desired lengths of arm assembly **12** may be accomplished by changing the number of balls and sleeves. For example, without the three additional balls **656a** and three additional sleeves **654a**, arm assembly **12** may have a length of about 32 inches.

[0132] A base handle **660** is coupled to central arm **652** on a first end thereof, preferably adjacent a ball **656a**. In addition, a free handle **662** is coupled to central arm **652** on a second end thereof, preferably adjacent a ball **656b**.

[0133] In one preferred exemplary device, a series of larger balls **656a** is provided proximate base handle **660** to provide stability to curvilinear articulating arm assembly **12**. If for example a user such as a surgeon orients assembly **12** by grasping it proximate free handle **662**, substantial bending forces may be exerted on central arm **652** proximate base handle **660**. Thus, the use of larger balls **656a** proximate base handle **660** as compared to smaller balls **656b** proximate free handle **662** provides a system with larger surface area balls near base handle

660 for additional resistance to rotational movement in that portion of central arm **652** and thus more stability. In alternate embodiments, more than two different sizes of balls **656** or more than two sets of sizes of balls **656** may be used, preferably increasing in size toward base handle **660**. In one alternate embodiment, each of the balls **656** in central arm **652** is of increasingly larger size from free handle **662** to base handle **660**. The use of only two sizes of balls **656** advantageously facilitates manufacture and construction of arm assembly **12** because of the need to only stock two sizes as compared to a larger number of sizes and concomitantly greater ease of construction because only two sizes need be assembled to form central arm **652**. In yet another alternate embodiment, central arm **652** may be formed of balls **656** that all are the same size.

[0134] Turning to FIG. 4D-4L, base handle **660** will be described. Base handle **660** includes a body portion **660a** with levers **666**, **668** pivotably associated therewith, as well as an extension **660b** that turns screw coupling **663** and rotates in relation to and independent of body portion **660a**. Base handle **660** further includes cam mechanisms **670**, **672** as will be described. Portion **663b** of coupling **663** preferably is noncircular and mechanically engages and is fixed to a like-shaped and sized non-circular opening in portion **660c** of extension **660b** so that rotation of extensions **660b** as by gripping and turning by a user imparts like-rotation of coupling **663** for example for demountable coupling to clamp **16** and further coupling to a surgical table rail **18**, as shown for example in FIG. 1. In the preferred exemplary embodiment, coupling **663** comprises a threaded portion **663d** which may be threadably received in a threaded hole **16a** disposed in clamp **16**.

[0135] Coupling **663** is disposed proximate a first free end **664a** of a stainless steel shaft **664** which extends therethrough and is provided with a head that abuts a shoulder disposed in end **663c** of coupling **663**. Preferably, rotation of coupling **663** is independent of rotation of shaft **664**. Shaft **664** preferably extends through a hole in extension **660b**.

[0136] Lever **666** is pivotably coupled to rocker arm **672** with a pin **666a** that is disposed such that rotation of lever **666** results in eccentric movement of rocker arm **672**. As shown for example in FIGS. 4D-4E, cylindrical projections **666b** of lever **666** are received and rotate in arcuate cradle portions **660a₁** of body portion **660a**, while cylindrical projections **672b** of rocker arm **672** are received and rotate in arcuate cradle portions **660a₂** of body portion **660a**. Rotation of lever **666** toward screw coupling **663** in direction **K** lifts pin **666a**, and because rocker arm **672** rests on pin **666a**, rocker arm **672** is rotated in direction **L** in an eccentric fashion.

[0137] As seen particularly in FIG. 4F, shaft **664** includes a threaded portion **664b** the free end of which is threadably associated with a nut **665a**. Shaft **664** extends through a hole in rocker arm **672** and an unthreaded insert **665b** with a hole therein which assists in guiding

travel of rod **664** along the longitudinal axis thereof. Pivoting of lever **666** in direction **K** causes rotation of rocker arm **672**, and with shaft **664** coupled to nut **665a** and nut **665a** abutting insert **665b**, rod **664** is translated in direction **M**.

[0138] When coupling **663** is threaded into a like threaded hole by rotation of extension **660b**, arm assembly **12** is relatively loosely coupled by the connection of coupling **663** to the hole. To firmly couple arm assembly **12**, lever **666** may be pivoted in direction **K** so that threaded portion **663d** of coupling **663** also moves in direction **M** and bears against the threads of the hole in which it is received. The leverage created by even slight movement of the threads against the threaded holes, on the order of tens of thousandths of an inch, creates a wedging effect that strongly locks arm assembly **12** to the hole.

[0139] Lever **668** of base handle **660** also is pivotably coupled to a rocker arm **670** with a pin **668a** that is disposed such that rotation of lever **668** results in eccentric movement of rocker arm **670**. As shown for example in FIGS. 4D-4H, cylindrical projections **668b** of lever **668** are received and rotate in arcuate cradle portions **660a₃** of body portion **660a**, while cylindrical projections **670b** of rocker arm **670** are received and rotate in arcuate cradle portions **660a₄** of body portion **660a**. Rotation of lever **668** toward screw coupling **663** in direction **N** lifts pin **668a**, and because rocker arm **670** rests on pin **668a**, rocker arm **670** is rotated in direction **P** in an eccentric fashion.

[0140] A forked member **676**, which for example may be formed of stainless steel, is coupled to rocker **670** and includes substantially parallel prongs **676a**, **676b** which mate with side walls of rocker **670** as shown. Rocker **670** is pivotably associated with forked member **676**, with a shaft **677** extending through aligned holes in prongs **676a**, **676b** and rocker **670**. Shaft **677** may be provided with a head **677a** and an external retaining ring **677b** secured in a shaft groove proximate an end opposite head **677a** to retain forked member **676** in association therewith and thus with rocker **670**. An axial through hole **676c** is provided in tubular portion **676d** of forked member **676**. Tensioning wire **658** is coupled to forked member **676** by inserting an end portion of wire **658** in hole **676c** and swaging tubular portion **676d** so that wire **658**, which extends out of open end **660a₅** of body portion **660a**, is retained by compression within tubular portion **676d**.

[0141] When lever **668** is rotated in direction **N**, shaft **676** translates along the longitudinal axis **M₁** toward coupling **663** creating substantial tension in tensioning wire **658** such that movement of curvilinear articulating arm assembly **12** may be substantially resisted. In particular, actuation of second lever **668** may increase or decrease the tension in wire **658** as desired by acting on rocker arm **670**. By increasing tension in wire **658**, central arm **652** preferably becomes increasingly resistant to movement although central arm **652** preferably still may be moved through its full range of motion. Thus, a user may

orient curvilinear articulating arm assembly **12** as desired, and then increase the tension of wire **658** so that the orientation of arm **652** is releasably fixed. Lever **668** preferably has an angular range of movement about pin **668a** of up to about 180° to permit substantial tension to be generated in tensioning wire **658**.

[0142] Rockers **670**, **672** preferably are associated with each other as with a spring plunger **679** extending from within one rocker **670** into a hole in the other rocker **672**. Spring plunger for example may be a stainless steel spring plunger with a round Delrin nose, without a lock element, with ¼"-20 threading, and 3-13 1b. end force (McMaster-Carr part number 84765A33). Spring plunger **679** is used as shown because under the force of gravity, first lever **666** may otherwise tend to move toward a closed position with in the direction of arrow **K**. Instead, spring plunger **679** applies pressure to rocker arm **672** to set lever **666** to tend to a default open position in which shaft **664** has not otherwise been raised toward open end **660a₅** of body portion **660a**.

[0143] In a preferred exemplary device, rocker **670** moves with substantially greater eccentricity than rocker **672**.

[0144] Clamp **16** for use with base handle **660** may be demountably attached to surgical table rail **18**. As previously discussed, actuation of first lever **666** permits a user to apply a force on coupling **663** so that movement is resisted (e.g., in response to an 8 or 10 pound force applied to arm **652**). In an alternate embodiment which will be further described later, screw coupling **664** as shown in FIG. 4A proximate base handle **660** of arm assembly **12** may be threadably associated with a threaded hole in another support surface.

[0145] A preferred exemplary of clamp **16** is shown in FIG. 4M. Clamp **16** includes a threaded hole **16a** for threadably receiving threaded portion **664** of base handle **660**. In addition, clamp **16** includes fixed jaw portion **16b** and movable jaw portion **16c** which is pivotable about axle **16d** and lockable in place using screw mechanism **16e** to firmly couple clamp **16** to a rail **18** secured between jaw portions **16b**, **16c**.

[0146] Next turning to FIGS. 4N-4U, free handle **662** will be described. Free handle **662** includes a wire receiving portion **680** and an end effector receiving portion **681**. In particular, wire receiving portion **680** preferably is configured to receive a ball **656b** therein, along with an end portion of wire **658**. As described previously with respect to base handle **660**, a pivotable lever **682** is associated with free handle **662** and preferably is coupled to tensioning wire **658** so that actuation of lever **682** may increase or decrease the tension in wire **658** as desired by acting on rocker arm **684**. By increasing tension in wire **658**, central arm **652** preferably becomes less flexible. Thus, a user may orient curvilinear articulating arm assembly **12** as desired, and then increase the tension of wire **658** so that the orientation of arm **652** is releasably fixed. Free handle **662** has a body portion **662a**, and lever **682** is rotatable with respect thereto. An interface lock

683 also is rotatably associated with body portion **662a** proximate end effector receiving portion **681**, as will be described shortly.

[0147] Lever **682** is pivotably coupled to rocker arm **684** with a pin **686a** that is disposed such that rotation of lever **682** results in eccentric movement of rocker arm **684**. Cylindrical projections **682a** of lever **682** are received and rotate in arcuate cradle portions **662a₁** of body portion **662a**, while cylindrical projections **684a** of rocker arm **684** are received and rotate in arcuate cradle portions **662a₂** of body portion **662a**. Rotation of lever **682** toward wire receiving portion **680** in direction **T** lifts pin **686a**, and because rocker arm **684** rests on pin **686a**, rocker arm **684** is rotated in direction **U** in an eccentric fashion.

[0148] Rocker arm **684** includes a hole in which a self-aligning setup washer **690** (a two-piece washer with one portion that rocks in another portion) is disposed. Setup washer **690** for example may be an 18-8 stainless steel self-aligning setup washer, ¼ inch in size, 17/64 inch inner diameter, ½ inch outer diameter, and 0.250 inch to 0.281 inch thick (McMaster-Carr part number 91944A028). A nut **692** also may abut setup washer **690** on the flat upper surface thereof and rock thereon. A threaded stud (not shown) may be swaged to the end of tensioning wire **658** opposite the end attached to forked member **676**, thus coupling wire **658** to the threaded stud by compression. The threaded stud may in turn be threadably associated with nut **692**. Wire **658** is provided with suitable length to span from forked member **676** to nut **692**.

[0149] Pivoting of lever **682** in direction **T** causes rotation of rocker arm **684**, and with tensioning wire **658** coupled to nut **692** and nut **692** abutting insert **690**, tension in wire **658** may be increased. In particular, actuation of lever **682** may increase or decrease the tension in wire **658** as desired. By increasing tension in wire **658**, central arm **652** preferably becomes increasingly resistant to movement although central arm **652** preferably still may be moved through its full range of motion. Thus, a user may orient curvilinear articulating arm assembly **12** as desired, and then increase the tension of wire **658** so that the orientation of arm **652** is releasably fixed. Lever **668** preferably has an angular range of movement about pin **686a** of up to about 90° to permit tension to be generated in tensioning wire **658**.

[0150] In the preferred exemplary device, actuation of lever **682** free handle **662** permits initial tensioning of central arm **652** while still permitting restricted movement. And, actuation of lever **668** of base handle **660** permits substantially greater tensioning of central arm **652** while also still permitting restricted movement thereof. Advantageously, with tension created in wire **658** of central arm **652** to restrict movement thereof, the orientation of lever **668** such as with respect to a patient still may readily be reset or adjusted before lever **666** in base handle **660** is actuated to create sufficient force to prevent rotation of threaded portion **663d** of coupling **663** in

the hole in which it is received.

[0151] As shown in FIG. 4U, interface lock **683** includes a knurled knob portion **683a** and a cylindrical post **683b** that is provided with an arcuate cutout **683c**. Interface lock **683** is coupled to body portion **662a** with set screw **683d** which is threadably received in a threaded hole **662b** in body portion **662a**. Set screw **683d** is further received in a slot **683e** in post **683b** to lock post **683b** in a position with arcuate cutout **683c** oriented to be movable along the longitudinal axis of cylindrical post **683b**. Cylindrical post **683b** may be disposed in a disengaged position in which the axial position of post **683b** is such that arcuate cutout **683c** generally follows the inner cylindrical contour of end effector receiving portion **681**. Also, cylindrical post **683b** may be disposed in an engaged position in which the axial position of post **683b** is such that a portion of cylindrical post **683b** other than arcuate cutout **683c** extends past the inner cylindrical contour of end effector receiving portion **681** toward the central longitudinal axis of end effector receiving portion **681**.

[0152] In use, in order for example to couple articulating arm assembly **12** to an end effector such as a holder **100**, by capturing post **102** of holder **100** in end effector receiving portion **681** of free handle **662**, post **102** is inserted therein while interface lock **683** is disposed in the aforementioned disengaged position. While lock **683** is in the disengaged position, post **102** may freely rotate about the central axis of receiving portion **681**. Once a desired orientation is set, lock **683** may be translated along the major axis defined by slot **683a** so that a portion of cylindrical post **683b** of lock **683** is disposed in an engaged position and bears against post **102**. Such interference between post **102** of holder **100** and post **683b** of lock **683** provides sufficient pressure so that post **102** will remain fixed in rotational position and translation along the longitudinal axis thereof against the inner cylindrical contour of end effector receiving portion **681**.

[0153] In one method of conducting a laparoscopic procedure, a curvilinear articulating arm assembly **12** with base attachment **16** is releasably secured to a surgical table rail **18**. Holder system **100** is demountably coupled to the free end of arm assembly **12** at free handle **662**, and a laparoscope is releasably retained in holder system **100** by locking it in the slot defined between face **122f** and clamping portion **114**, with the laparoscope being frictionally held in the slot in the desired rotational orientation. By articulating the lever **682** at the free end to a locked position, arm assembly **12** will hold position when left alone but can be easily repositioned with one hand without having to loosen or unclamp any other mechanisms. In this mode, arm assembly **12** should have sufficient resistance to hold the laparoscope in position absent other external forces, much like a gooseneck lamp. If locking lever **668** near the base of arm assembly **12** is also locked then arm assembly **12** will hold position against a much greater force, but this lever **668** will then have to be released when ready movement of the arm/

scope combination is required.

[0154] Preferably, the two rotating joints of holder **100** have complete freedom of motion and cannot be locked, and the scope is engaged by the slot defined between face **122f** and clamping portion **114** that opens via a syringe-like spring mechanism as previously described. Free movement of the scope is allowed by the freely rotating joints of holder **100** that respond to user-selected positioning of articulating arm assembly **12** while the scope is in the skin port of the patient.

[0155] In normal use, knob **124** preferably is backed off so that the spring loading of movable clamping jaws **122** operates freely and the scope may be engaged and disengaged quickly at will.

[0156] Once curvilinear articulating arm assembly **12** is fixed in position, the geometry of the swivel joints of holder **100** in combination with the curvilinear articulating arm assembly **12** and the laparoscope passing through a skin port is designed to result in reliable position holding for the scope, yet allow complete freedom of movement by manual repositioning. There is no need to adjust any locking or tensioning mechanisms because of the geometry of the setup and the resistance provided by the arm in its "goose-neck lamp" mode.

[0157] In some methods, gross movements of the scope may be accomplished by grabbing the articulating arm assembly **12** proximate the swivel joints and reorient the device from that gripping point. For smaller movements, it is possible to simply grab and torque the scope itself.

[0158] In one method of use, curvilinear articulating arm assembly **12** is closely contoured to the patient (approximately parallel to the skin) to minimize interference and clutter, and with the holder such as holder **800** extended nearby the endoscopic camera port. The position of arm assembly **12** is checked for suitable working range near the planned port site. The optimum attachment point for the base of the arm assembly **12** for example on a surgical bed railing is determined after the patient is positioned and asleep and before the next preparation phase. Arm assembly **12** may be oriented out of the way for prepping and draping. An arm drape may be placed after the skin prep but before the final large procedure drape is placed. A separate skirt/sheet drape may be clipped around the base after the large drape is placed. Arm assembly **12** may be contoured to the patient and brought adjacent to the camera port. The scope may be engaged working through the drape for example by pinching open the spring loaded clamp of holder **800** and simply invaginating the cover with the scope into the slot. The cover preferably is tough and stretchy and withstands repeated engage/disengage cycles and scope rotation.

[0159] Each of the holder systems described herein may be used in accordance with the aforementioned methods, regardless of spring-loading of the clamping arrangements.

[0160] Also, although an exemplary curvilinear articulating arm assembly is described herein, it should be understood that other preferably, curvilinear articulating arm assemblies instead may be used which preferably provide six degrees of freedom of movement and permit relatively rigid positioning such as described herein.

5

10

15

20

25

30

35

40

45

50

55

lating arm assembly is described herein, it should be understood that other preferably, curvilinear articulating arm assemblies instead may be used which preferably provide six degrees of freedom of movement and permit relatively rigid positioning such as described herein.

[0161] In some embodiments of the present invention, an instrument holder system such as system **10** may be coupled to a patient support other than a rail of a table. For example, referring next to **FIG. 5**, an exemplary support system **710** according to the present invention is shown with a variety of components coupled thereto. Support system **710** includes a tray **712**, curvilinear articulating arm assemblies **12**, **716** having respective end effectors **100**, **720**, an IV pole **722**, an arm board **724**, and rail assemblies **726**, **728**. A variety of end effectors may be demountably attached for example to articulating arm assembly **716** to assist a technician or practitioner with a medical/imaging procedure or provide other features useful with respect to a patient. End effector **720**, for example, is configured as a self-centering abdominal probe bracket.

[0162] In one preferred exemplary embodiment, tray **712** may include two pairs of hold regions **730**, each pair being disposed proximate a free cranial end **732** or free caudal end **734** of tray **712**. In alternate embodiments, other numbers of hold regions **730** may be provided such as two or more, and hold regions **730** may be provided in other regions of tray **712** such as intermediate ends **732**, **734** proximate sides **736**, **738**. Hold regions **730** may be configured as hand holds, or alternatively may be configured to receive strapping so that tray **712** may be releasably coupled to another object such as an ambulance stretcher, hospital bed, operating room table, or imaging scanner table. In some embodiments, handles may be coupled to tray **712**. As also shown in **FIG. 5**, attachment regions **740** are provided proximate sides **736**, **738** for demountably coupling components as previously described to tray **712**, as will be further described below. In the exemplary preferred embodiment, tray **712** is provided with thirteen attachment regions **740**, although in alternate embodiments another number of regions **740** may be provided such as at least one or tray **712** may be provided with a surgical rail or track permitting substantial freedom of coupling of components along the length thereof.

[0163] Turning to **FIGS. 6A-6C**, additional features of tray **712** are shown. Although hand hold regions **730** are not included in the figure, such regions may be provided as shown in **FIG. 5**. Attachment regions **740** are provided in spaced arrangement along the perimeter of tray **712**. Preferably, tray **712** includes a central arcuate portion **742** disposed between outer ledge portions **744**. Preferably, regions **740** are provided on outer ledge portions **744**. Central arcuate portion **742** preferably has an upper concave surface **742a** for receiving a patient and optionally a cushion (not shown) for the patient to rest against, and optionally includes a lower convex surface **742b**. Preferably, outer ledge portions **744** include upper and

lower surfaces **744a**, **744b** connected by a sidewall **744c** at an angle α with respect to surface **744b**. In a preferred exemplary embodiment, sidewall **744c** is disposed at an angle α between about 60° and about 100°, more preferably between about 70° and about 90°, and most preferably at about 80°.

[0164] In a preferred exemplary embodiment, tray **712** is formed of natural finish carbon fiber, R-51 foam core, and phenolic. Attenuation preferably is less than 1 mm Al equivalency. Thus, tray **712** is radiolucent and suitable for use with computed axial tomography (CT) scanners. In other embodiments, tray **712** is formed of a material suitable for use with magnetic resonance imaging (MR) scanners. In addition, tray **712** preferably supports a load of 900 lbs. evenly distributed along centerline **746**, about which tray **712** may be substantially symmetric as shown. Indicia **748** optionally may be provided, as shown for example proximate ends **732**, **734**. The indicia may for example indicate preferred orientation of tray **712** with respect to a patient lying thereon.

[0165] In the preferred exemplary embodiment, attachment regions **740** on each side of tray **712** are evenly spaced from each other by about 6 inches between centers thereof. To accommodate patients and equipment attached to tray **12**, in one preferred embodiment tray **712** has a length of about **78** inches, a width of about 21 inches, a generally uniform thickness of about 0.9 inch, and a height **h** of about 2.5 inches. Corners may be provided with a radius **R₁** of about 2 inches. In the preferred exemplary embodiment, attachment regions **740** preferably accommodate threaded inserts, which may be formed of aluminum.

[0166] In some embodiments, tray **712** is sized to hold an adult patient, and may be between about 180 cm and about 200 cm long. However, it will be appreciated that longer and shorter trays may be provided. In order to accommodate an adult patient, tray **712** may support an overall weight capacity of at least about 200 pounds, and preferably at least about 300 pounds. However, if a tray **712** is sized for use with a pediatric patient, tray **712** may only accommodate weights that do not exceed 200 pounds, and more preferably do not exceed 100 pounds.

[0167] Although the surface of portion **742** of tray **712** is substantially smooth in the preferred exemplary embodiment, in alternate embodiments the surface may be textured to provide additional resistance to motion of objects and/or a patient placed thereon.

[0168] Tray **712** thus is suitable for use in multiple environments, and thus may "move" with the patient from one environment (e.g., ambulance) to the next (e.g., CT scanner) without removing a patient supported thereon.

[0169] While various descriptions of the present invention are described above, it should be understood that the various features can be used singly or in any combination thereof. Therefore, this invention is not to be limited to only the specifically preferred embodiments depicted herein. For example, although the holders described herein are described in the context of laparoscopic

ic instrument holder systems that may place a camera through a port in the skin into a working cavity, the holders also may be used for example in the context of procedures that examine the interior of a bodily canal or hollow organ such as the colon, bladder, or stomach. The present invention may be applied in a variety of fields including but not limited to general surgery, orthopedics, gynecology, urology, and cardiology. In the context of laparoscopy, the systems of the present invention for example may be used to assist in surgical procedures involving the intestines, stomach, or gallbladder which may benefit from the visual inspection made possible by a laparoscope.

[0170] The scope of the present invention is accordingly defined as set forth in the appended claims.

Claims

1. A system (10) for positioning a laparoscopic device (1054), the system having a holder (1000) comprising:
 - a central portion (1024) comprising a first member (1032) operatively associated with a second member (1030), the members selectively movable with respect to one another along a central axis (1034), the central portion having a proximal end defined by the first member and a distal end defined by the second member;
 - at least three proximal rotational joints (1008, 1014, 1020) coupled to the first member proximate the proximal end;
 - at least two distal rotational joints (1042, 1050) coupled to the second member proximate the distal end;
 - a clamp (1052) configured and dimensioned for retaining a laparoscopic device; and
 - a coupling portion (1002) proximate a first of the proximal rotational joints;
- wherein a first of the distal rotational joints is coupled to the distal end of the central portion and a second of the distal rotational joints is coupled to the clamp, and in that each proximal rotational joint and each distal rotational joint permits 360° of rotation about an axis thereof.
2. The system of claim 1, wherein the members telescope with respect to one another.
3. The system of claim 2, wherein the second member (1030) is slidably received in the first member (1032).
4. The system of claim 3, wherein the first member comprises a slot (1032a) and the second member comprises a protrusion (1034a), the protrusion movable within the slot.

5. The system of claim 4, wherein the protrusion comprises a roller key (1034a).
6. The system of claim 4, wherein the second member (1030) comprises a piston member (1036) proximate an end thereof, the piston member disposed within the first member (1032).
7. The system of claim 6, wherein the piston member is spring-loaded with a spring (1036b) oriented transverse to the central axis.
8. The system of claim 2, wherein the first member comprises a receiving end for receiving the second member and a bushing (1038) coupled to the receiving end.
9. The system of claim 8, wherein the bushing comprises a plurality of fingers (1038a) disposed radially with respect to the central axis (1034).
10. The system of claim 1, wherein each of the proximal and distal rotational joints comprises a thrust bearing (1074).
11. The system of claim 10, wherein the thrust bearing is a steel ball thrust bearing.
12. The system of claim 10, wherein each of the proximal rotational joints comprises a washer (1078) abutting a spacer (1082) and rotatable with respect to each other.
13. The system of claim 12, wherein the spacer (1082) is formed of a material that is polytetrafluoroethylene-based.
14. The system of claim 10, wherein each of the distal rotational joints comprises a washer (1078) abutting a spacer (1082) and rotatable with respect to each other.
15. The system of claim 14, wherein the spacer (1082) is formed of a material comprising acetal homopolymer.
16. The system of claim 10, wherein each of the proximal and distal rotational joints comprises a spacer, each of the spacers of the proximal rotational joints having a first thickness and each of the spacers of the distal rotational joints having a second thickness, the first thickness being smaller than the second thickness.
17. The system of claim 1, wherein the at least three proximal rotational joints comprises three proximal rotational joints that each permit movement in a separate plane.
18. The system of claim 17, wherein at least two of the planes are parallel to one another.
19. The system of claim 1, wherein:
 - the first of the distal rotational joints (1042) permits rotation about an axis coinciding with the main axis (1034); and
 - the second of the distal rotational joints (1050) permits rotation about an axis (1048) transverse to the main axis.
20. The system of claim 19, wherein the second of the distal rotational joints (1050) permits rotation about an axis generally perpendicular to the main axis.
21. The system of claim 1, wherein the clamp (1052) comprises a pair of spring-biased jaw members (1052a, 1052b) each having a cover (1052e) formed of a material softer than aluminium, the clamp being configured and dimensioned to retain the laparoscopic device while contacting the covers.
22. The system of claim 21, wherein each cover is formed of polyurethane.
23. The system of claim 22, wherein the laparoscopic device (1054) comprises a cylindrical portion.
24. The system of claim 1, wherein the first member (1032) is tubular.
25. The system of claim 1, wherein each of the proximal and distal rotational joints comprises a first portion rotatable with respect to a second portion about a fixed axis.
26. The system of claim 1, wherein the first and second members are movable with respect to each other along the central axis but are not rotatable with respect to each other.
27. The system of claim 1, further comprising a curvilinear articulating arm (12), the holder being coupled to the curvilinear articulating arm.
28. The system of claim 27, further comprising a tray configured and dimensioned for supporting a mammal, the curvilinear articulating arm being coupled to the tray.
29. The system of claim 1, wherein the coupling portion (1002) comprises a clamp 16 for coupling to a support (18).
30. The system of claim 29, wherein the support (18) is selected from the group consisting of a rail of a table and a rail of a bed.

31. The system of claim 5, wherein the roller key (1034a) is a miniature high precision stainless steel ball bearing.

Patentansprüche

1. System (10) zum Positionieren eines laparoskopischen Geräts (1054), wobei das System einen Halter (1000) hat, der Folgendes umfasst:

einen Mittelabschnitt (1024), der ein erstes Element (1032) umfasst, das wirksam mit einem zweiten Element (1030) verknüpft ist, wobei die Elemente selektiv in Bezug aufeinander entlang einer Mittelachse (1034) bewegt werden können, wobei der Mittelabschnitt ein proximales Ende, das durch das erste Element definiert wird, und ein distales Ende, das durch das zweite Element definiert wird, hat, wenigstens drei proximale Drehgelenke (1008, 1014, 1020), die nahe dem proximalen Ende an das erste Element gekoppelt sind, wenigstens zwei proximale Drehgelenke (1042, 1050), die nahe dem distalen Ende an das zweite Element gekoppelt sind, eine Klemme (1052), die dafür konfiguriert und bemessen ist, ein laparoskopisches Gerät festzuhalten, und einen Kopplungsabschnitt (1002) nahe einem ersten der proximalen Drehgelenke,

wobei ein erstes der distalen Drehgelenke an das distale Ende des Mittelabschnitts gekoppelt ist und ein zweites der distalen Drehgelenke an die Klemme gekoppelt ist, und **dadurch gekennzeichnet, dass** jedes proximale Drehgelenk und jedes distale Drehgelenk eine Drehung von 360° um eine Achse desselben ermöglicht.

2. System nach Anspruch 1, wobei sich die Elemente in Bezug aufeinander ineinanderschieben.
3. System nach Anspruch 2, wobei das zweite Element (1030) verschiebbar in dem ersten Element (1032) aufgenommen wird.
4. System nach Anspruch 3, wobei das erste Element einen Schlitz (1032a) umfasst und das zweite Element einen Vorsprung (1034a) umfasst, wobei der Vorsprung innerhalb des Schlitzes bewegt werden kann.
5. System nach Anspruch 4, wobei der Vorsprung einen Rollenkeil (1034a) umfasst.
6. System nach Anspruch 4, wobei das zweite Element (1030) ein Kolbenelement (1036) nahe einem proxi-

malen Ende desselben umfasst, wobei das Kolbenelement innerhalb des ersten Elements (1032) angeordnet ist.

- 5 7. System nach Anspruch 6, wobei das Kolbenelement mit einer Feder (1036b), die quer zu der Mittelachse ausgerichtet ist, federgespannt ist.
- 10 8. System nach Anspruch 2, wobei das erste Element ein Aufnahmeende zum Aufnehmen des zweiten Elements und eine Buchse (1038), die an das Aufnahmeende gekoppelt ist, umfasst.
- 15 9. System nach Anspruch 8, wobei die Buchse eine Vielzahl von Fingern (1038a) umfasst, die in Radialrichtung in Bezug auf die Mittelachse (1034) angeordnet sind.
- 20 10. System nach Anspruch 1, wobei jedes der proximalen und distalen Drehgelenke ein Axiallager (1074) umfasst.
- 25 11. System nach Anspruch 10, wobei das Axiallager ein Stahlkugel-Axiallager ist.
- 30 12. System nach Anspruch 10, wobei jedes der proximalen Drehgelenke eine Scheibe (1078) umfasst, die an ein Abstandsstück (1082) anstößt, und sie in Bezug aufeinander drehbar sind.
- 35 13. System nach Anspruch 12, wobei das Abstandsstück (1082) aus einem Werkstoff geformt ist, der auf Polytetrafluorethylen beruht.
- 40 14. System nach Anspruch 10, wobei jedes der distalen Drehgelenke eine Scheibe (1078) umfasst, die an ein Abstandsstück (1082) anstößt, und sie in Bezug aufeinander drehbar sind.
- 45 15. System nach Anspruch 14, wobei das Abstandsstück (1082) aus einem Werkstoff geformt ist, der Acetal-Homopolymer umfasst.
- 50 16. System nach Anspruch 10, wobei jedes der proximalen und distalen Drehgelenke ein Abstandsstück umfasst, wobei jedes der Abstandsstücke der proximalen Drehgelenke eine erste Dicke hat und jedes der Abstandsstücke der distalen Drehgelenke eine zweite Dicke hat, wobei die erste Dicke kleiner ist als die zweite Dicke.
- 55 17. System nach Anspruch 1, wobei die wenigstens drei proximalen Drehgelenke drei proximale Drehgelenke umfassen, deren jedes eine Bewegung in einer gesonderten Ebene ermöglicht.
18. System nach Anspruch 17, wobei wenigstens zwei der Ebenen parallel zueinander sind.

19. System nach Anspruch 1, wobei:

das erste der distalen Drehgelenke (1042) eine Drehung um eine Achse, die mit der Hauptachse (1034) zusammenfällt, ermöglicht und das zweite der distalen Drehgelenke (1050) eine Drehung um eine Achse (1048), quer zu der Hauptachse, ermöglicht.

20. System nach Anspruch 19, wobei das zweite der distalen Drehgelenke (1050) eine Drehung um eine Achse, im Wesentlichen senkrecht zu der Hauptachse, ermöglicht.

21. System nach Anspruch 1, wobei die Klemme (1052) ein Paar von federvorgespannten Klemmbackenelementen (1052a, 1052b) umfasst, deren jedes eine Abdeckung (1052e), die aus einem Werkstoff, weicher als Aluminium, geformt ist, hat, wobei die Klemme dafür konfiguriert und bemessen ist, das laparoskopische Gerät festzuhalten, während die Abdeckungen berührt werden.

22. System nach Anspruch 21, wobei jede Abdeckung aus Polyurethan geformt ist.

23. System nach Anspruch 22, wobei das laparoskopische Gerät (1054) einen zylindrischen Abschnitt umfasst.

24. System nach Anspruch 1, wobei das erste Element (1032) röhrenförmig ist.

25. System nach Anspruch 1, wobei jedes der proximalen und distalen Drehgelenke einen ersten Abschnitt umfasst, der in Bezug auf einen zweiten Abschnitt um eine feststehende Achse gedreht werden kann.

26. System nach Anspruch 1, wobei das erste und das zweite Element in Bezug aufeinander entlang der Mittelachse bewegt werden können, aber nicht in Bezug aufeinander gedreht werden können.

27. System nach Anspruch 1, das ferner einen krummlinigen Gelenkarm (12) umfasst, wobei der Halter an den krummlinigen Gelenkarm gekoppelt ist.

28. System nach Anspruch 27, das ferner eine Ablage umfasst, die dafür konfiguriert und bemessen ist, ein Säugetier zu tragen, wobei der krummlinige Gelenkarm an die Ablage gekoppelt ist.

29. System nach Anspruch 1, wobei der Kopplungsabschnitt (1002) eine Klemme (16) zum Koppeln an eine Stütze (18) umfasst.

30. System nach Anspruch 29, wobei die Stütze (18) aus der Gruppe ausgewählt ist, die aus einer Quer-

stange eines Tisches und einer Querstange eines Betts besteht.

31. System nach Anspruch 5, wobei der Rollenkeil (1034a) ein hochpräzises Miniatur-Edelstahl-Kugellager ist.

Revendications

1. Système (10) de positionnement d'un dispositif laparoscopique (1054), le système comportant un support (1000), comprenant :

une partie centrale (1024), comprenant un premier élément (1032) associé en service à un deuxième élément (1030), les éléments pouvant être déplacés sélectivement l'un par rapport à l'autre le long d'un axe central (1034), la partie centrale comportant une extrémité proximale définie par le premier élément et une extrémité distale définie par le deuxième élément ;
au moins trois joints rotatifs proximaux (1008, 1014, 1020) accouplés au premier élément près de l'extrémité proximale ;
au moins deux joints rotatifs distaux (1042, 1050), accouplés au deuxième élément près de l'extrémité distale ;
une bride de serrage (1052), configurée et dimensionnée de sorte à retenir un dispositif laparoscopique ; et
une partie d'accouplement (1002) près d'un premier des joints rotatifs proximaux ; un premier joint des joints rotatifs distaux étant accouplé à l'extrémité distale de la partie centrale, et un deuxième joint des joints rotatifs distaux étant accouplé à la bride de serrage, et **caractérisé en ce que** chaque joint rotatif proximal et chaque joint rotatif distal permet une rotation de 360° sur un axe correspondant.

2. Système selon la revendication 1, dans lequel les éléments sont télescopés l'un par rapport à l'autre.

3. Système selon la revendication 2, dans lequel le deuxième élément (1030) est reçu de manière coulissante dans le premier élément (1032).

4. Système selon la revendication 3, dans lequel le premier élément comprend une fente (1032a), le deuxième élément comprenant une saillie (1034a), la saillie pouvant se déplacer dans la fente.

5. Système selon la revendication 4, dans lequel la saillie comprend une clavette de roulement (1034a).

6. Système selon la revendication 4, dans lequel le deuxième élément (1030) comprend un élément de

- piston (1036) près de l'une de ses extrémités, l'élément de piston étant agencé dans le premier élément (1032).
7. Système selon la revendication 6, dans lequel l'élément de piston est chargé par ressort, par un ressort (1036b) orienté de manière transversale par rapport à l'axe central.
8. Système selon la revendication 2, dans lequel le premier élément comprend une extrémité de réception pour recevoir le deuxième élément, et une douille (1038) accouplée à l'extrémité de réception.
9. Système selon la revendication 8, dans lequel la douille comprend plusieurs doigts (1038a) agencés radialement par rapport à l'axe central (1034).
10. Système selon la revendication 1, dans lequel chacun des joints rotatifs proximaux et distaux comprend un palier de butée (1074).
11. Système selon la revendication 10, dans lequel le palier de butée est un palier de butée à billes en acier.
12. Système selon la revendication 10, dans lequel chacun des joints rotatifs proximaux comprend une rondelle (1078) butant contre une entretoise (1082), les joints pouvant tourner les uns par rapport aux autres.
13. Système selon la revendication 12, dans lequel l'entretoise (1082) est composée d'un matériau à base de polytétrafluoréthylène.
14. Système selon la revendication 10, dans lequel chacun des joints rotatifs proximaux comprend une rondelle (1078) butant contre une entretoise (1082), les joints pouvant tourner les uns par rapport aux autres.
15. Système selon la revendication 14, dans lequel l'entretoise (1082) est composée d'un matériau comprenant un homopolymère d'acétal.
16. Système selon la revendication 10, dans lequel chacun des joints rotatifs proximaux et distaux comprend une entretoise, chacune des entretoises des joints rotatifs proximaux ayant une première épaisseur et chacune des entretoises des joints rotatifs distaux ayant une deuxième épaisseur, la première épaisseur étant inférieure à la deuxième épaisseur.
17. Système selon la revendication 1, dans lequel les au moins trois joints rotatifs proximaux comprennent trois joints rotatifs proximaux permettant chacun un déplacement dans un plan séparé.
18. Système selon la revendication 17, dans lequel au moins deux des plans sont parallèles l'un à l'autre.
19. Système selon la revendication 1, dans lequel :
- le premier joint des joints rotatifs distaux (1042) permet une rotation sur un axe coïncidant avec l'axe principal (1034) ; et
- le deuxième joint des joints rotatifs distaux (1050) permet la rotation sur un axe (1048) transversal à l'axe principal.
20. Système selon la revendication 19, dans lequel le deuxième joint des joints rotatifs distaux (1050) permet la rotation sur un axe généralement perpendiculaire à l'axe principal.
21. Système selon la revendication 1, dans lequel la bride de serrage (1052) comprend une paire d'éléments de mâchoire sollicités par ressort (1052a, 1052b), comportant chacun un couvercle (1052e) composé d'un matériau plus mou que l'aluminium, la bride de serrage étant configurée et dimensionnée de sorte à retenir le dispositif laparoscopique en contactant les couvercles.
22. Système selon la revendication 21, dans lequel chaque couvercle est composé de polyuréthane.
23. Système selon la revendication 22, dans lequel le dispositif laparoscopique (1054) comprend une partie cylindrique.
24. Système selon la revendication 1, dans lequel le premier élément (1032) est tubulaire.
25. Système selon la revendication 1, dans lequel chacun des joints rotatifs proximaux et distaux comprend une première partie pouvant tourner par rapport à une deuxième partie sur un axe fixe.
26. Système selon la revendication 1, dans lequel les premier et deuxième éléments peuvent être déplacés l'un par rapport à l'autre le long de l'axe central, mais ne peuvent pas tourner l'un par rapport à l'autre.
27. Système selon la revendication 1, comprenant en outre un bras d'articulation curviligne (12), le support étant accouplé au bras d'articulation curviligne.
28. Système selon la revendication 27, comprenant en outre un plateau configuré et dimensionné de sorte à supporter un mammifère, le bras d'articulation curviligne étant accouplé au plateau.
29. Système selon la revendication 1, dans lequel la partie d'accouplement (1002) comprend une bride de serrage (16) en vue de l'accouplement à un support (18).
30. Système selon la revendication 29, dans lequel le

support (18) est sélectionné dans le groupe constitué d'un rail d'une table et d'un rail d'un lit.

- 31.** Système selon la revendication 5, dans lequel la clavette de roulement (1034a) est un roulement à billes en acier inoxydable miniature haute précision.

10

15

20

25

30

35

40

45

50

55

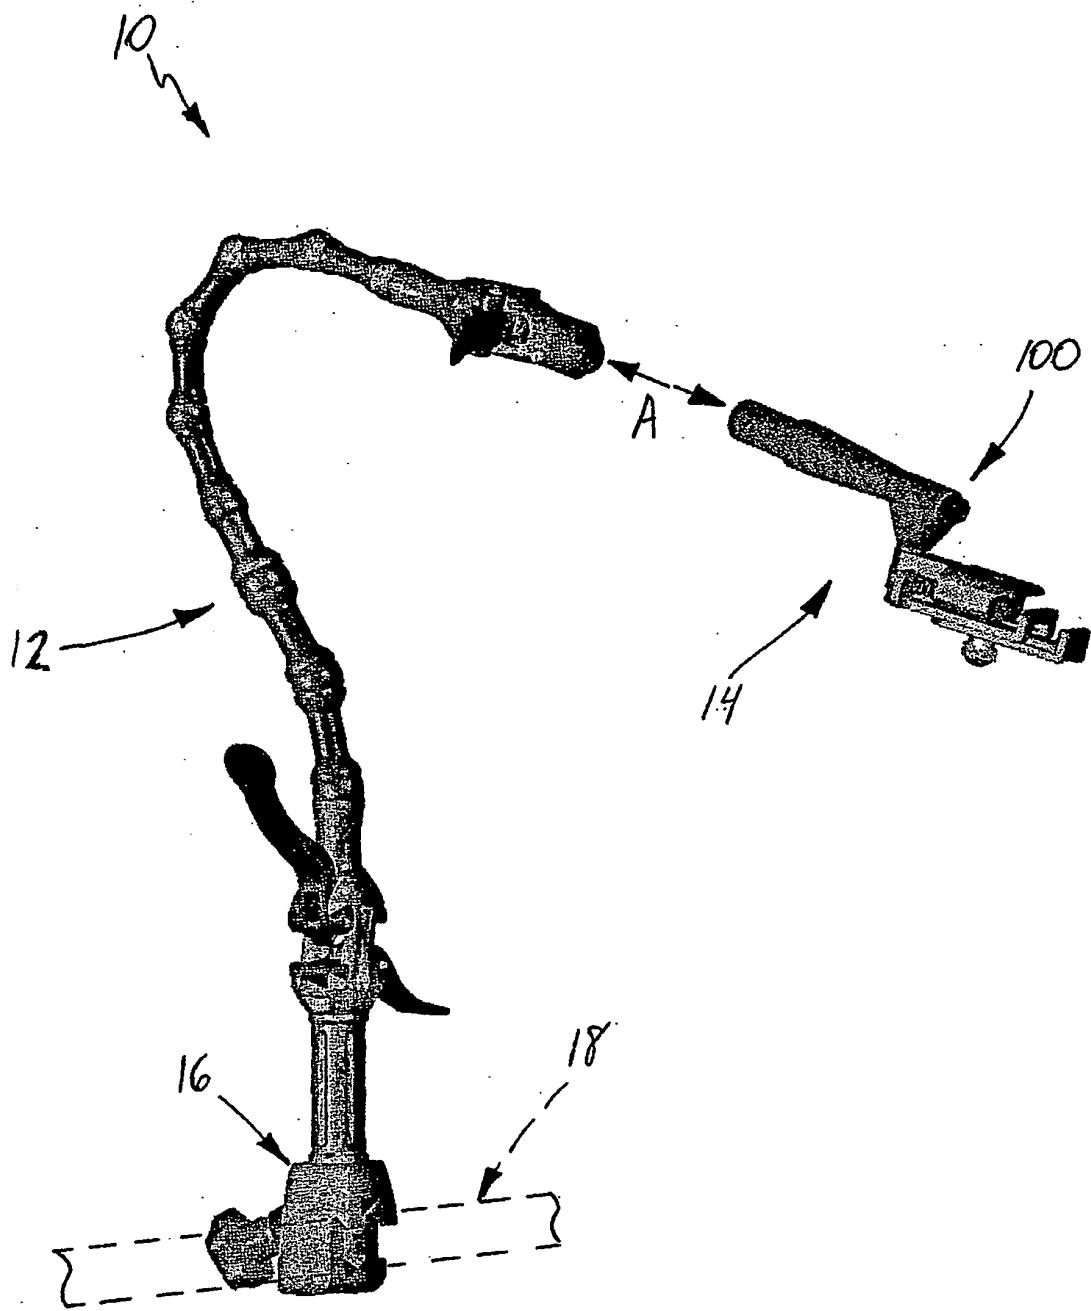


FIG. 1

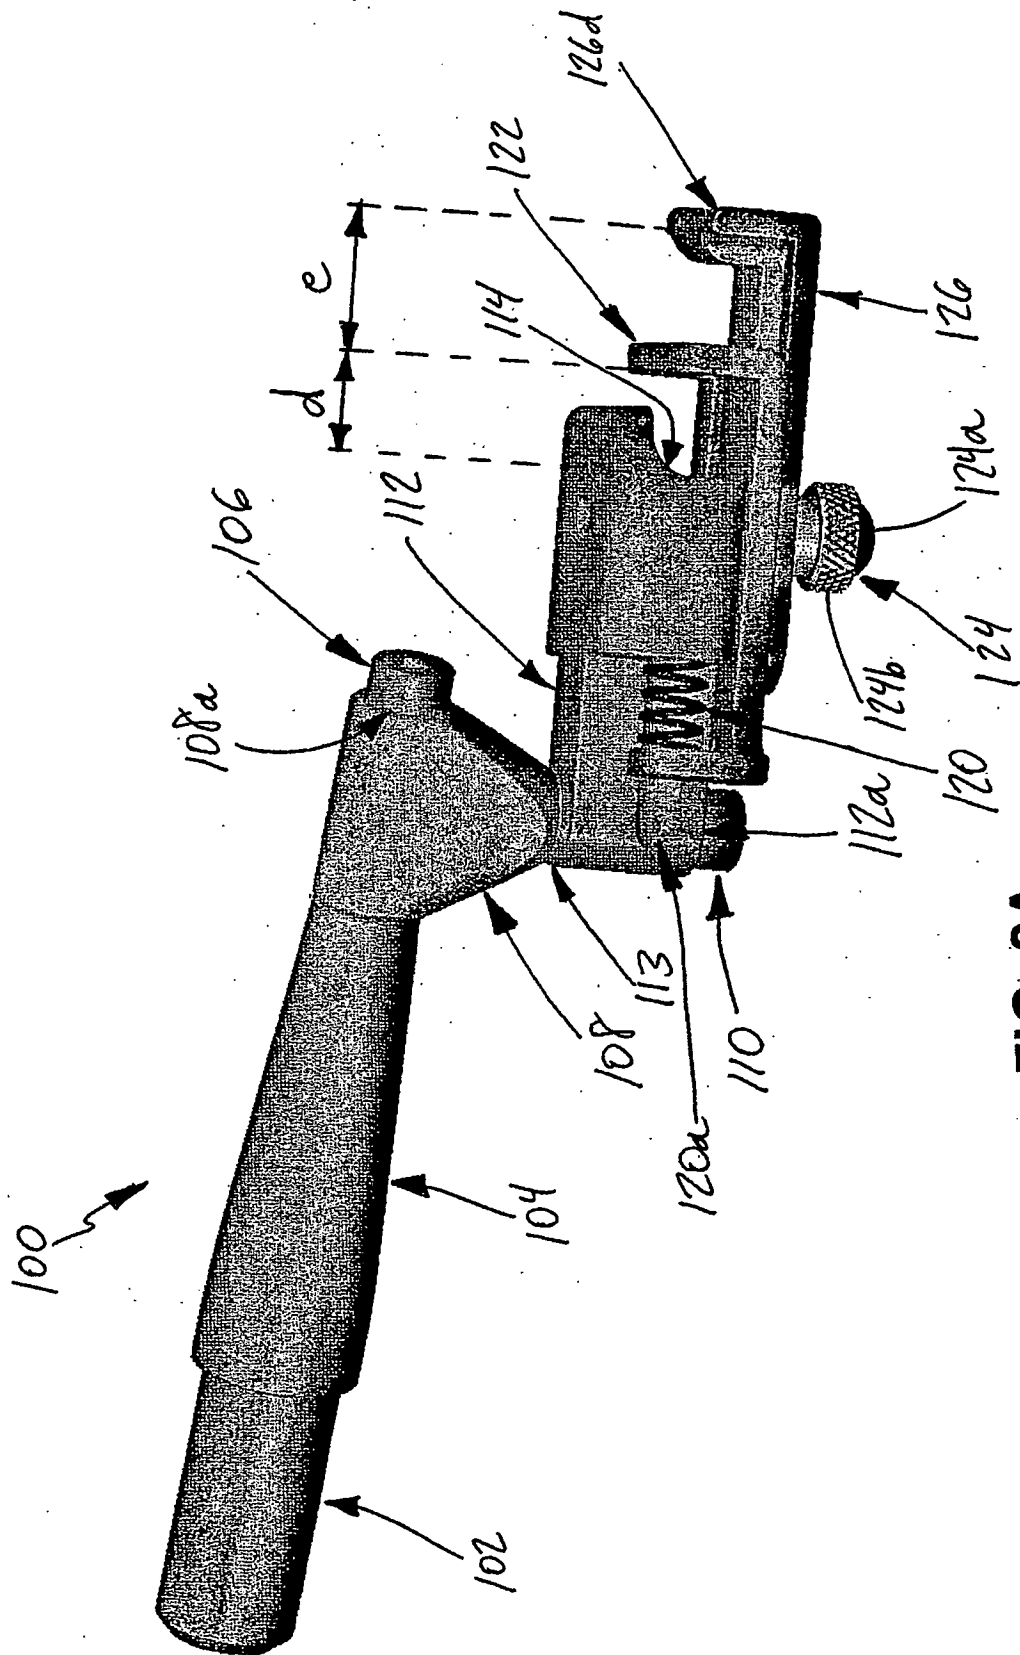


FIG. 2A

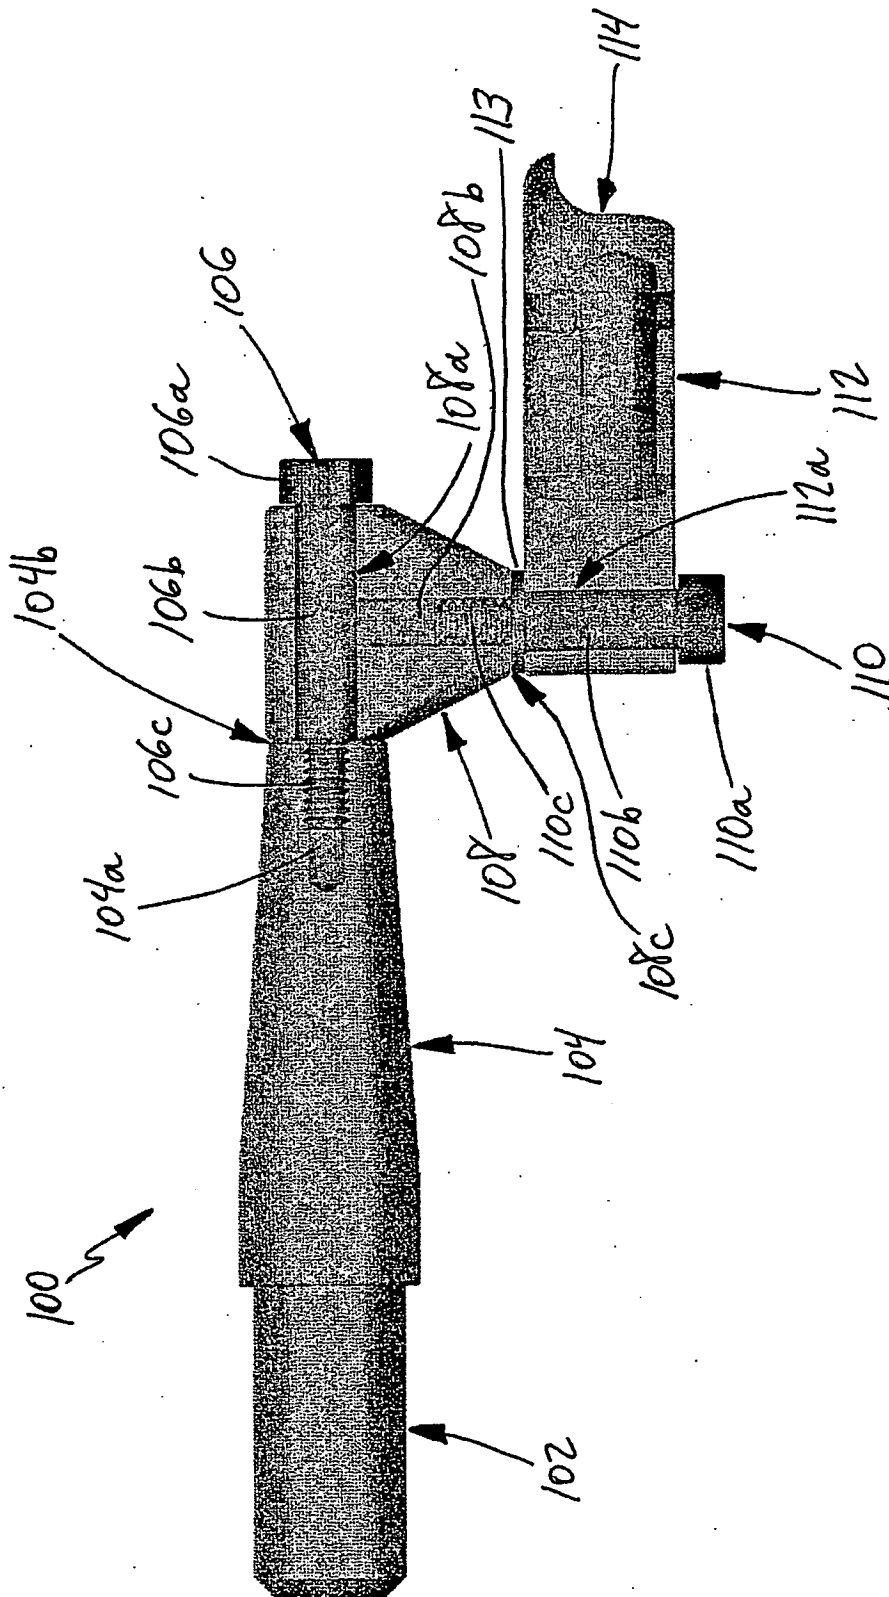


FIG. 2B

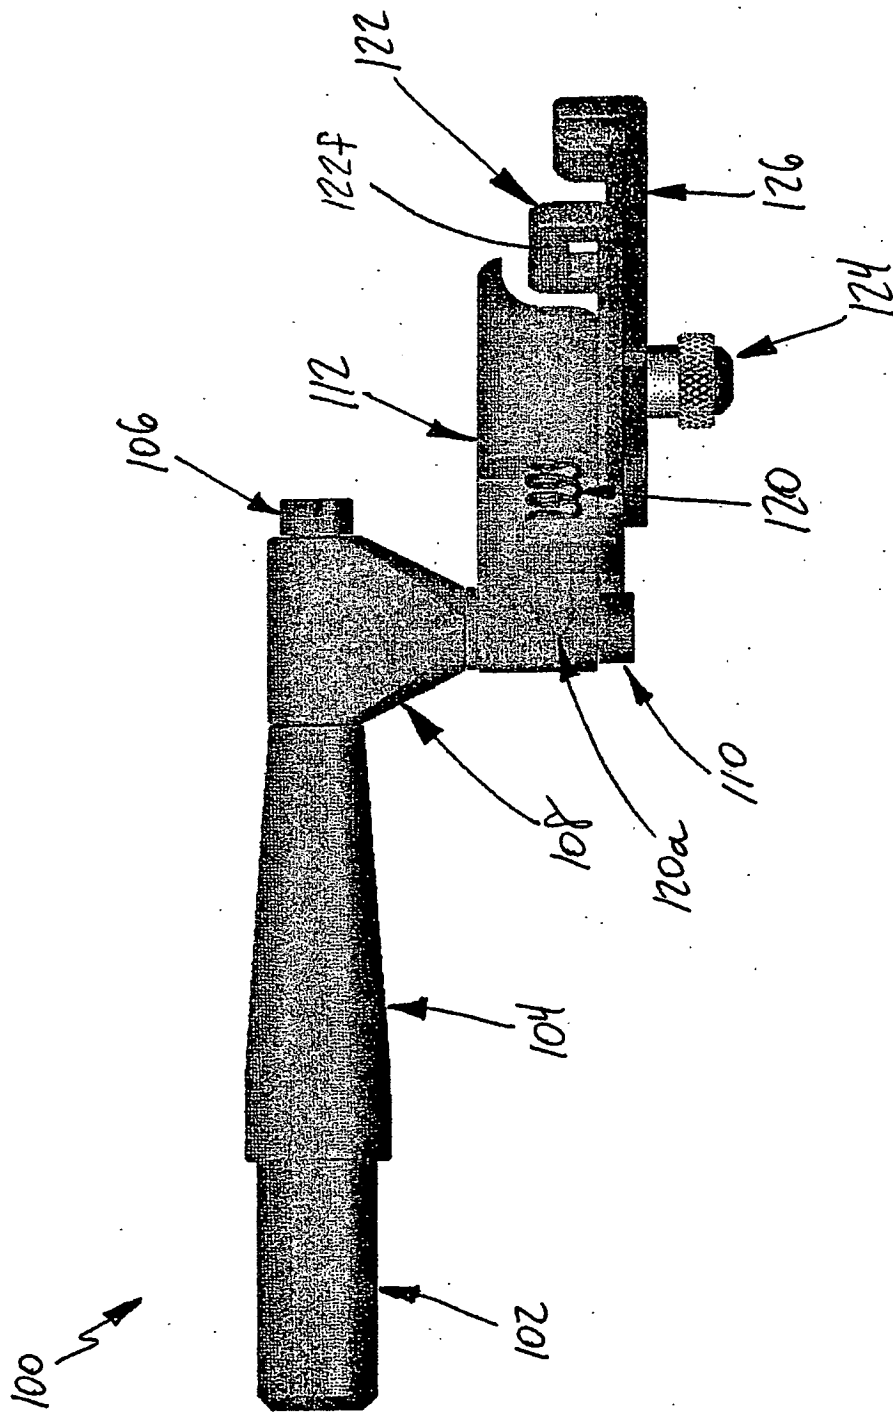


FIG. 2C

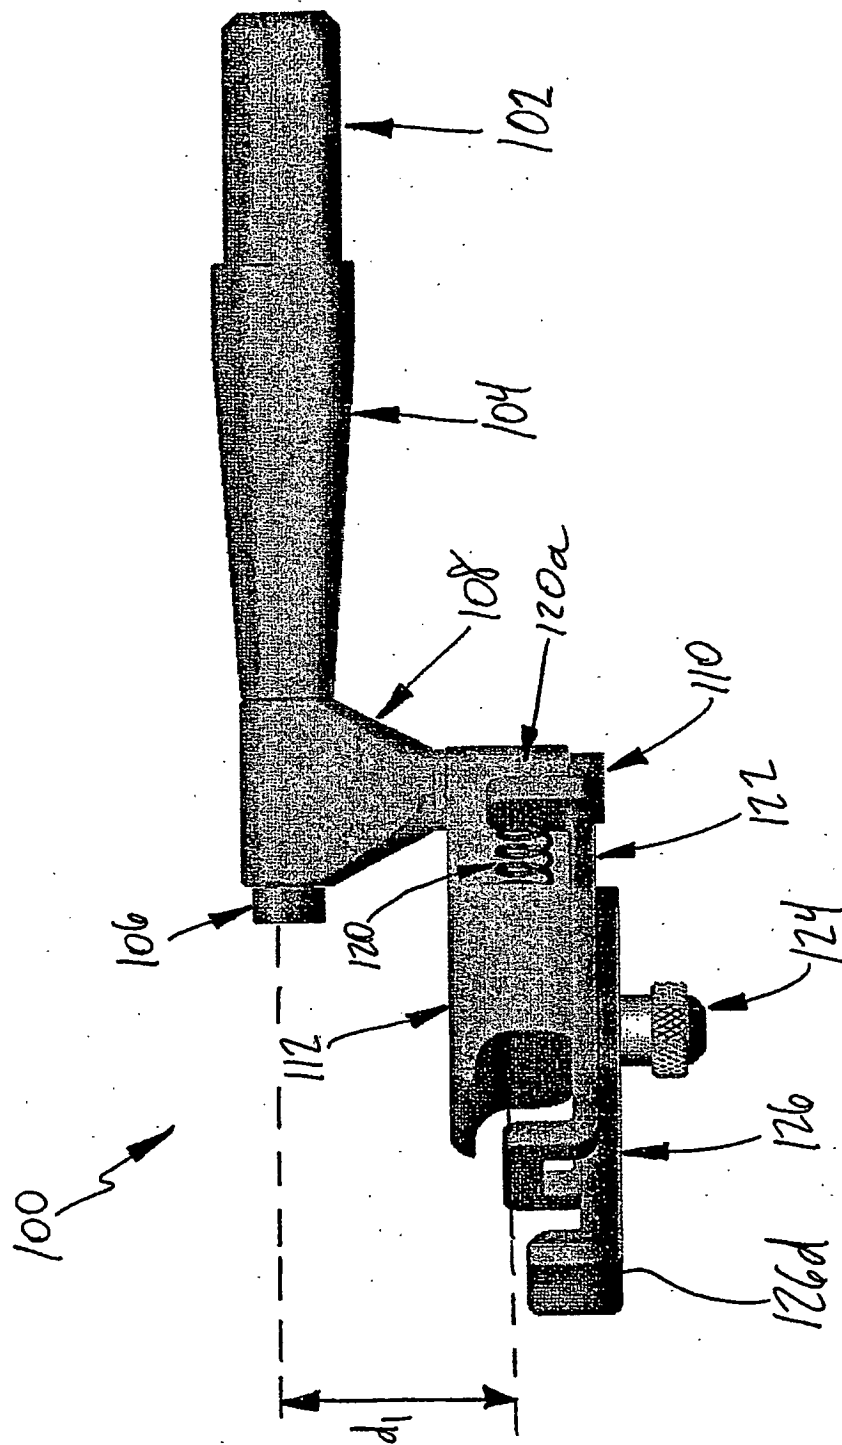


FIG. 2D

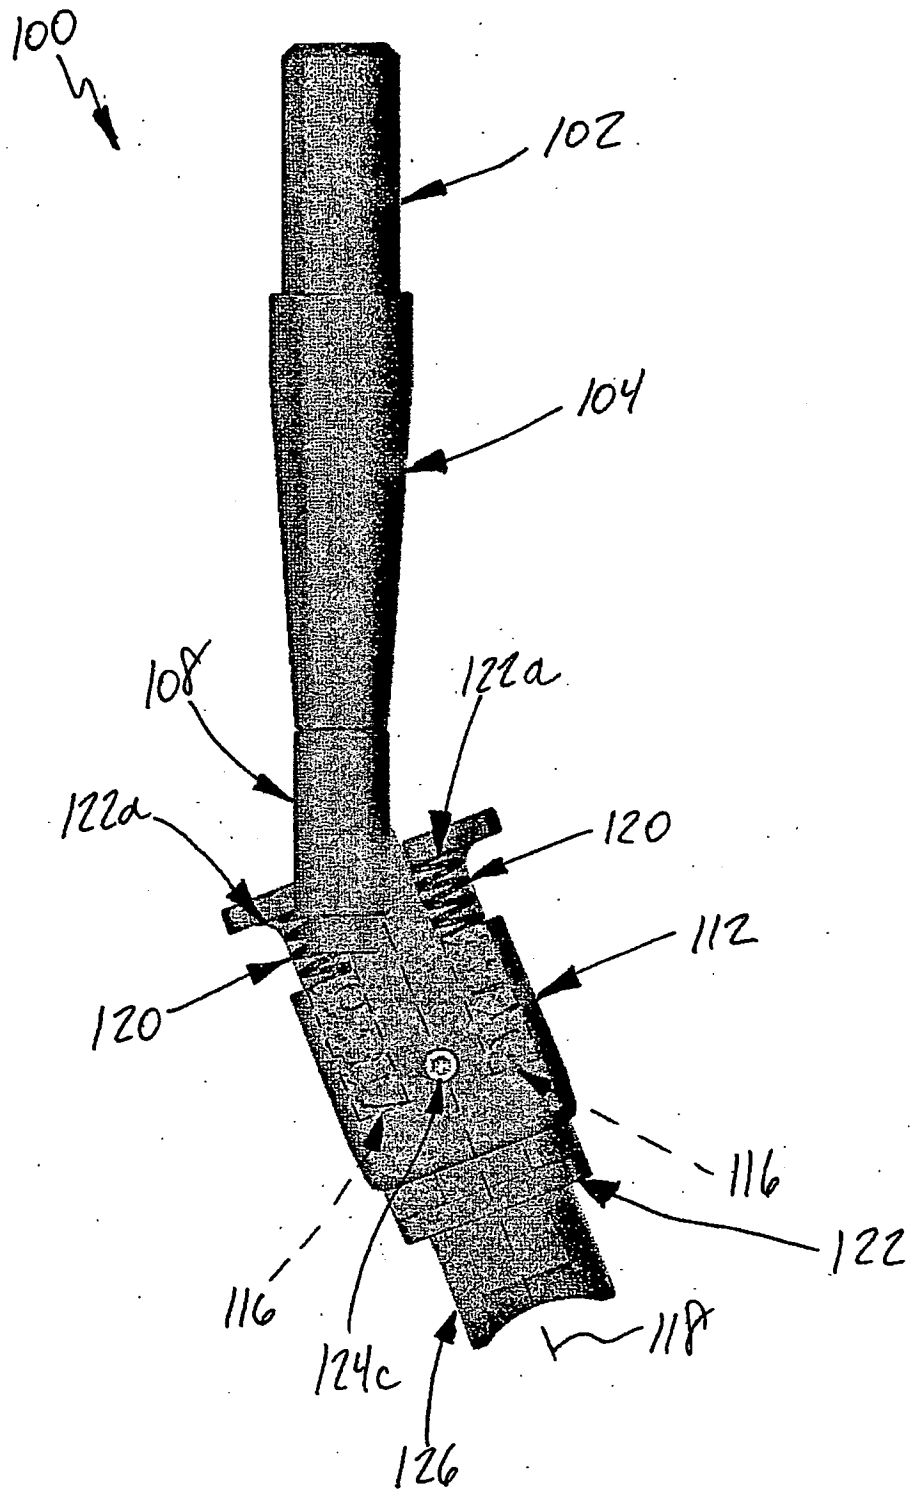


FIG. 2E

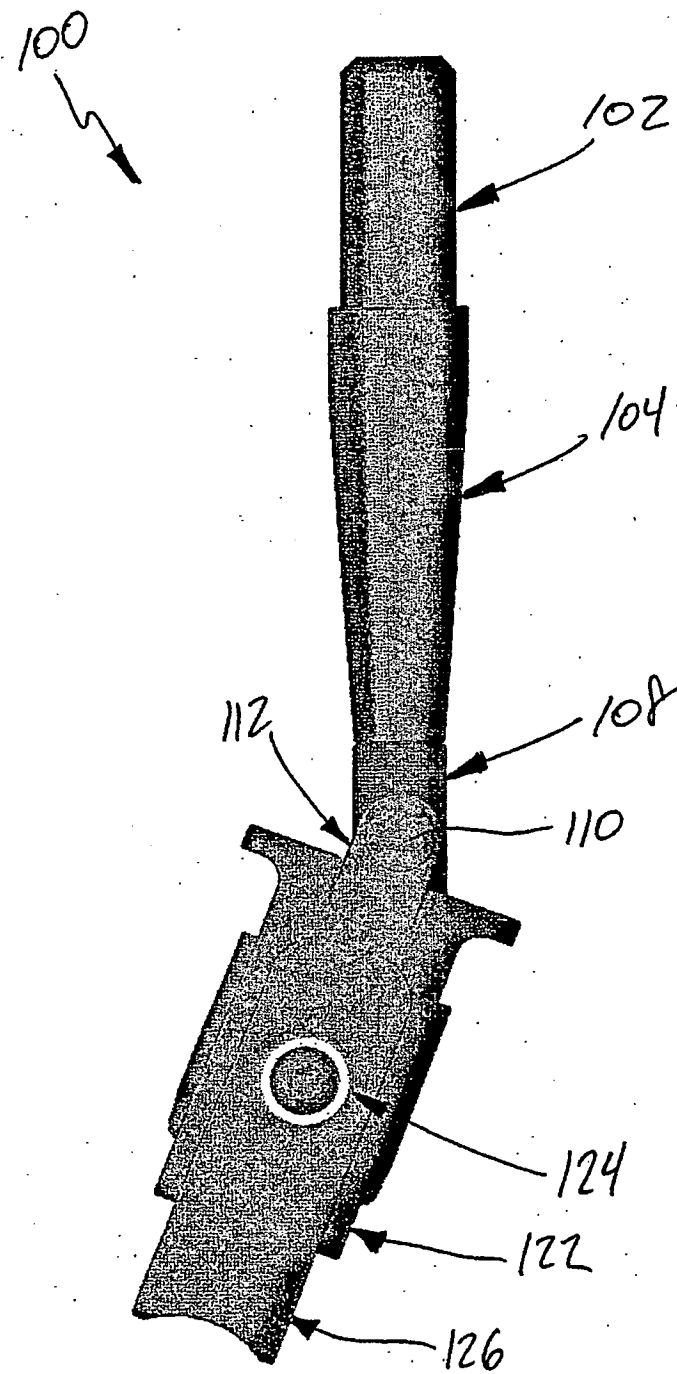


FIG. 2F

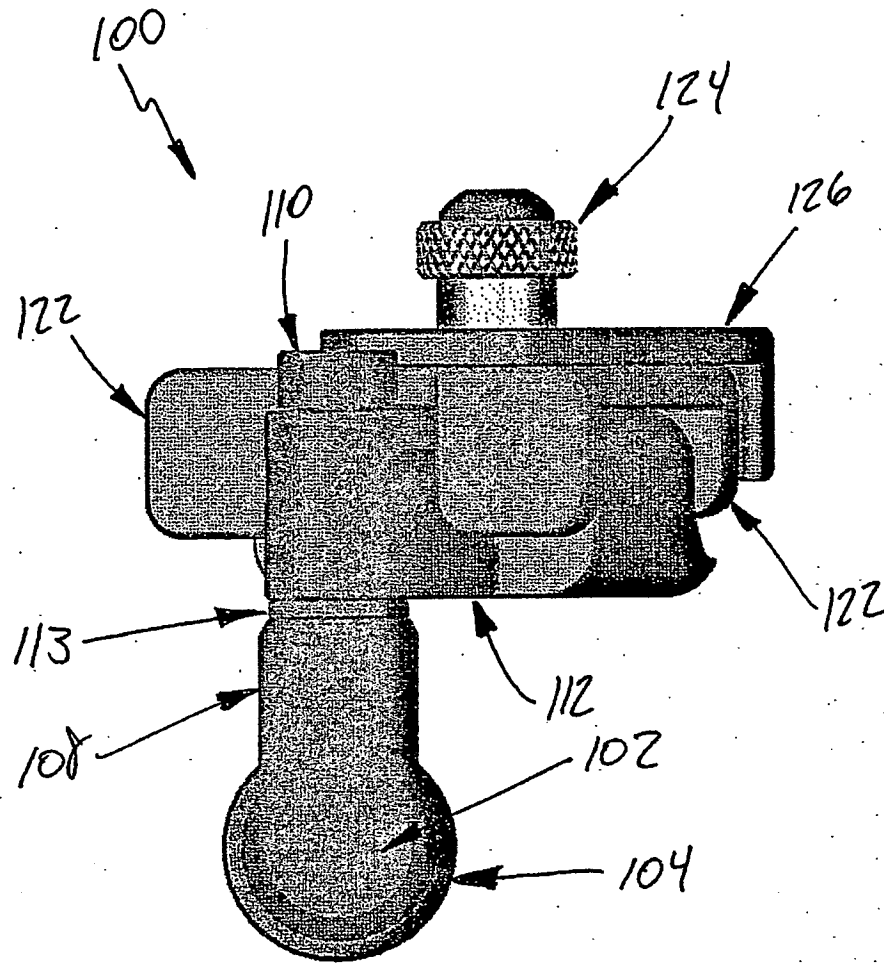


FIG. 2G

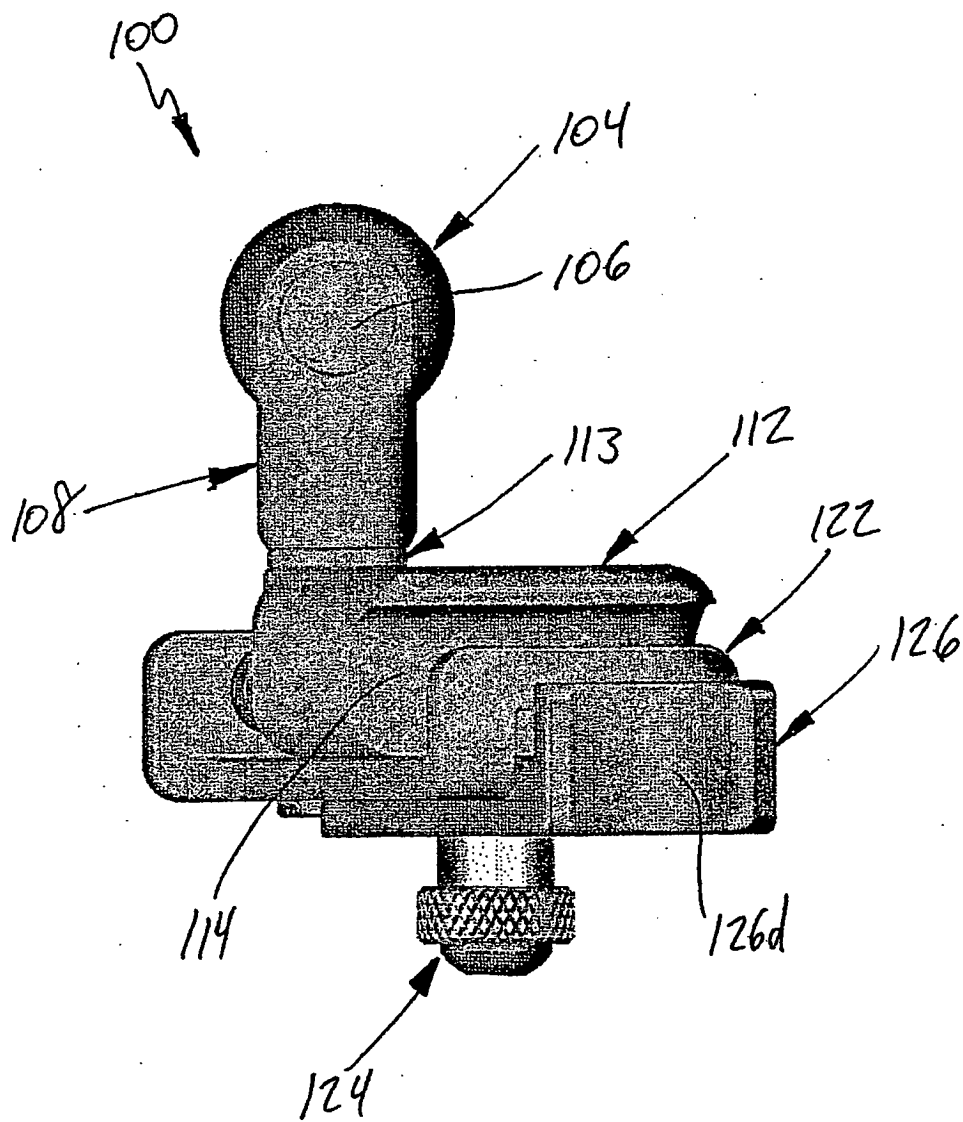


FIG. 2H

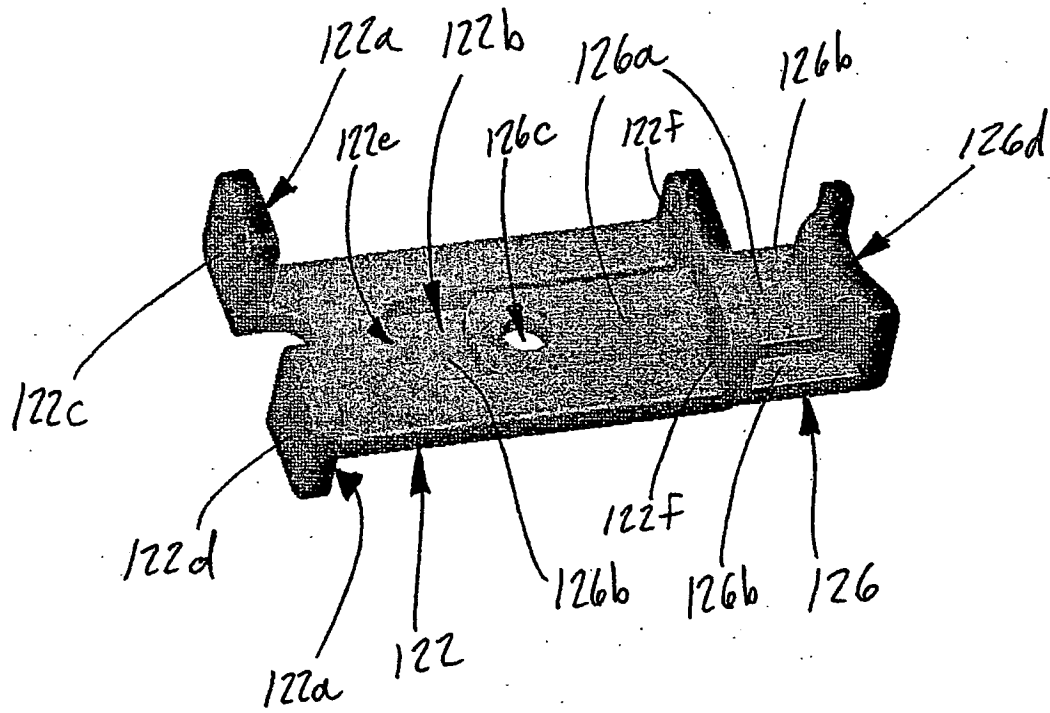


FIG. 2I

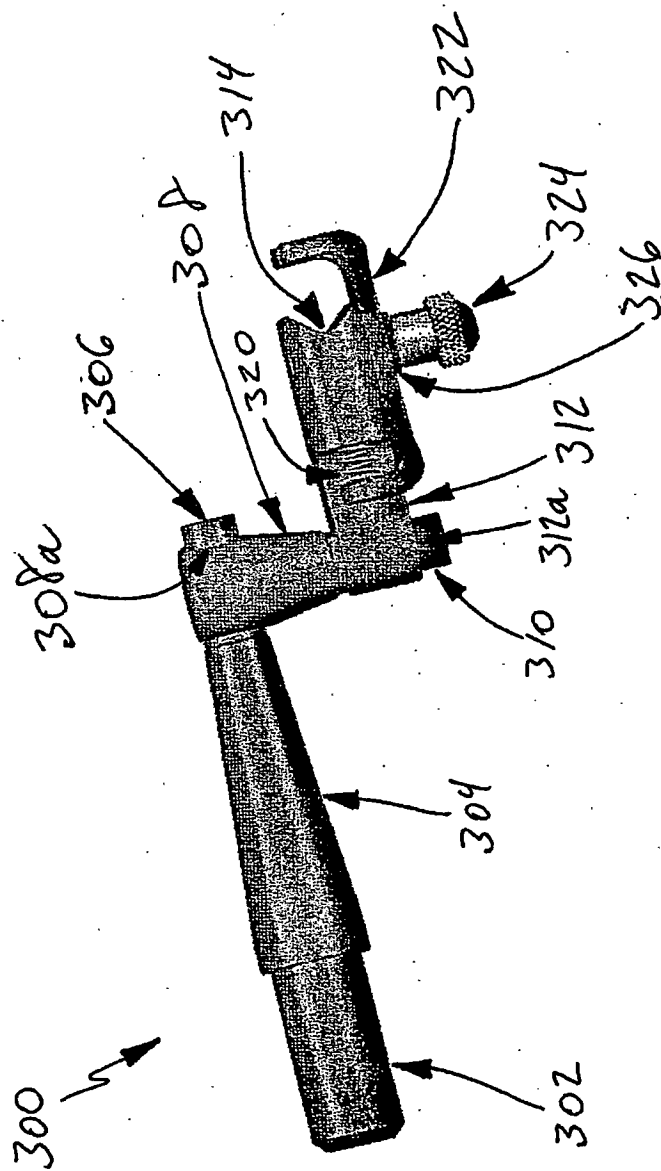


FIG. 3A

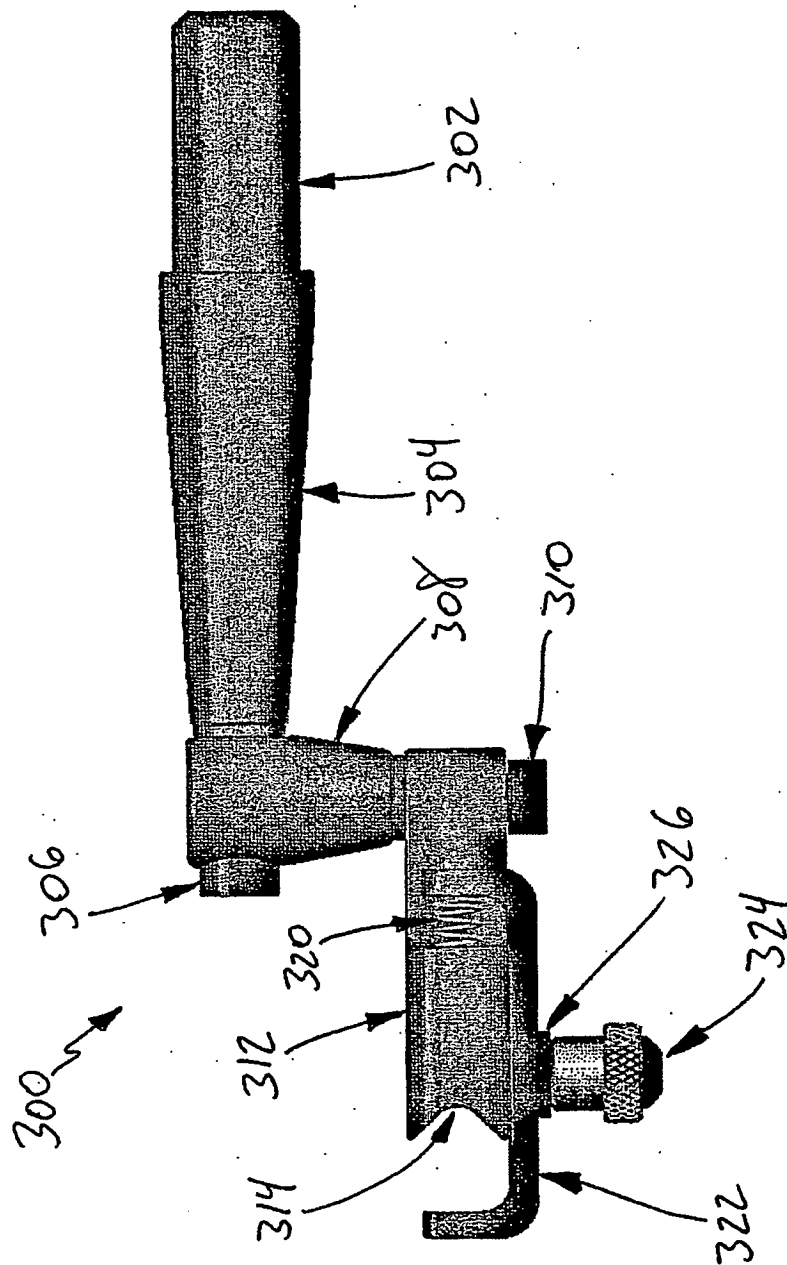
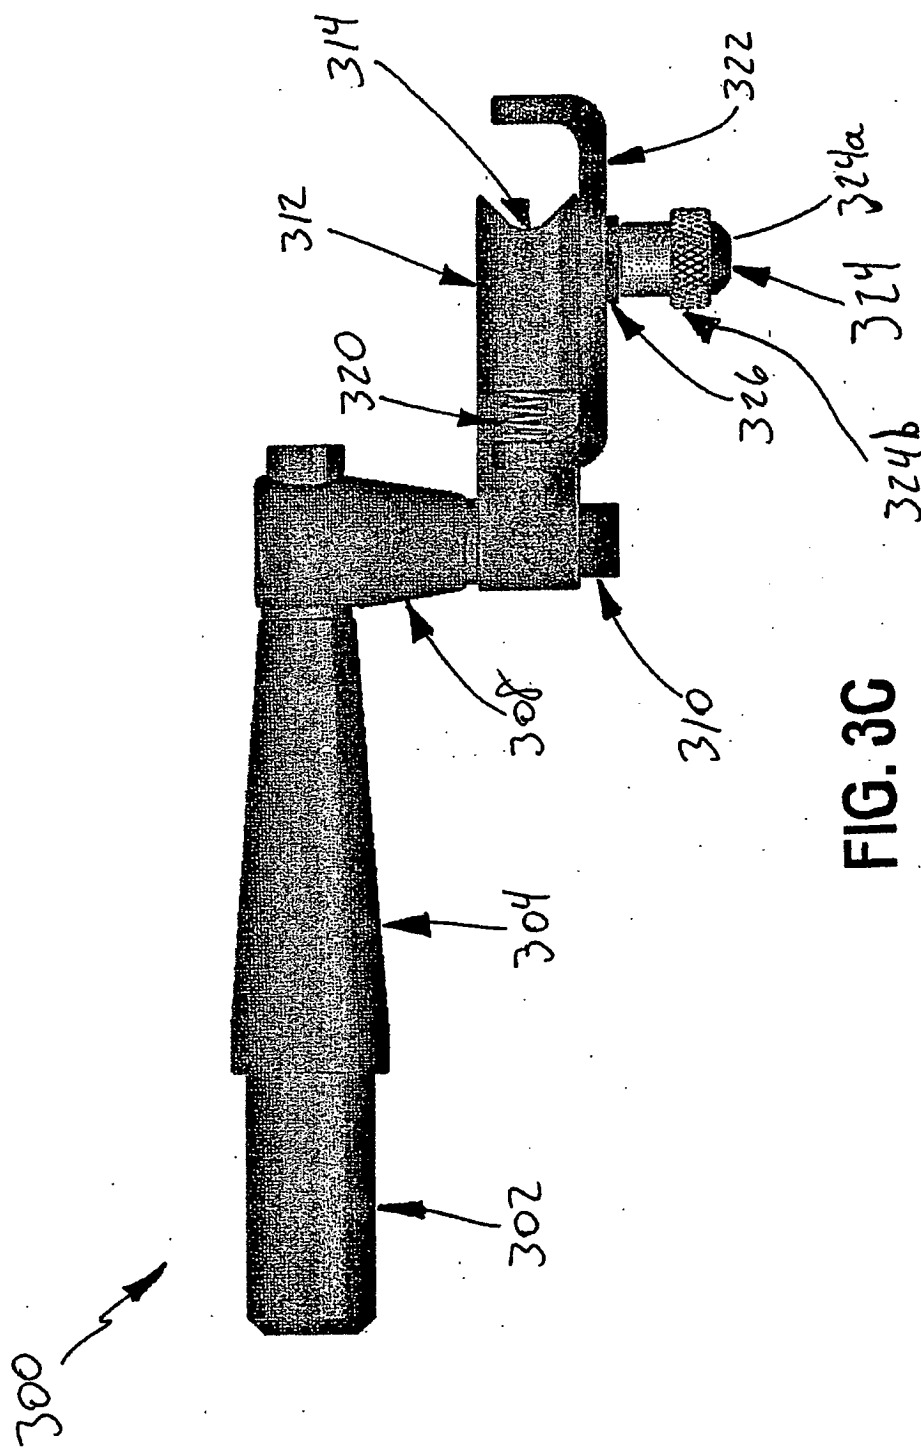


FIG. 3B



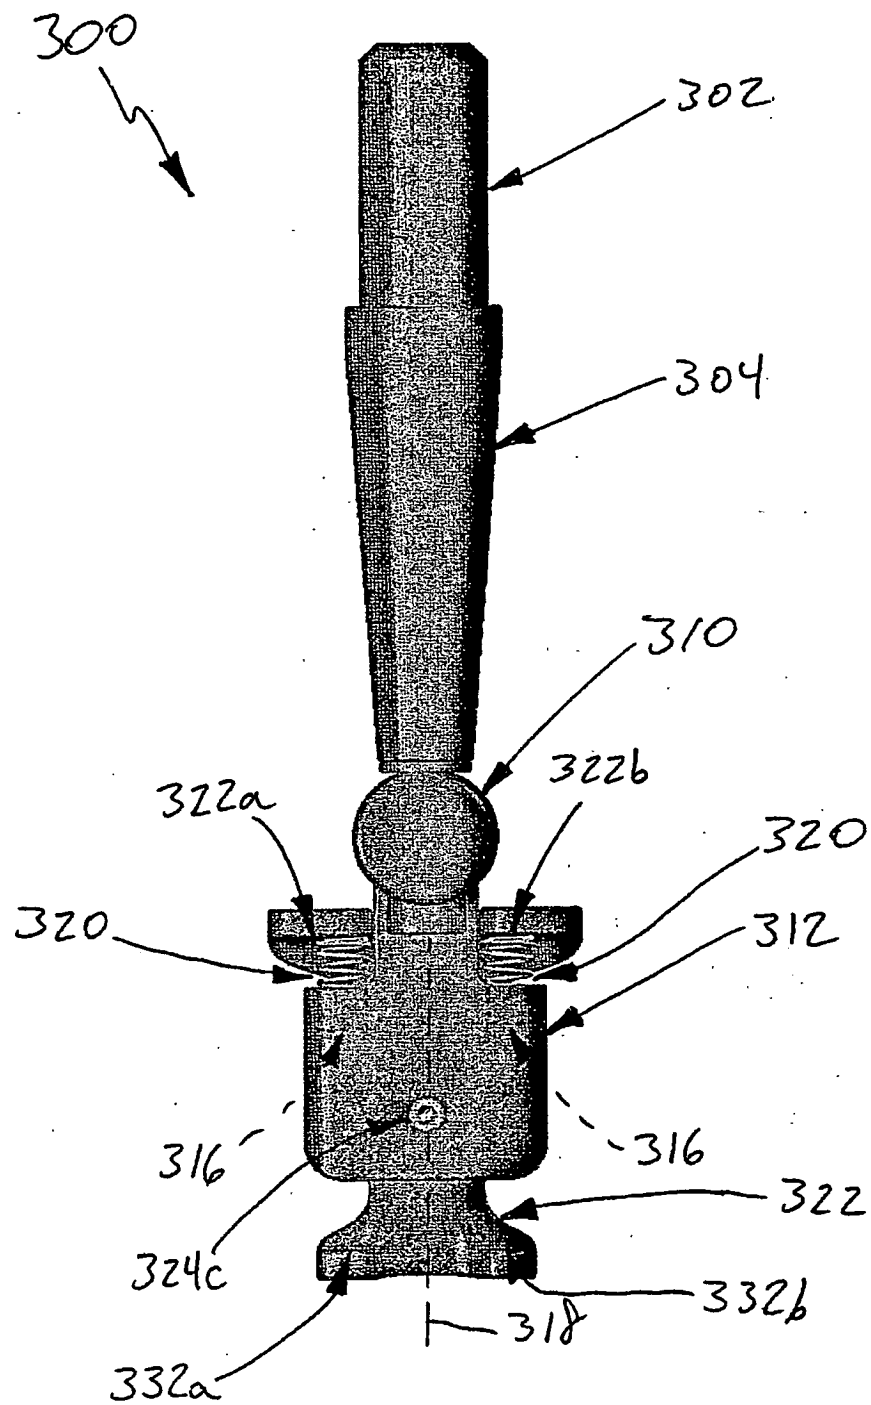


FIG. 3D

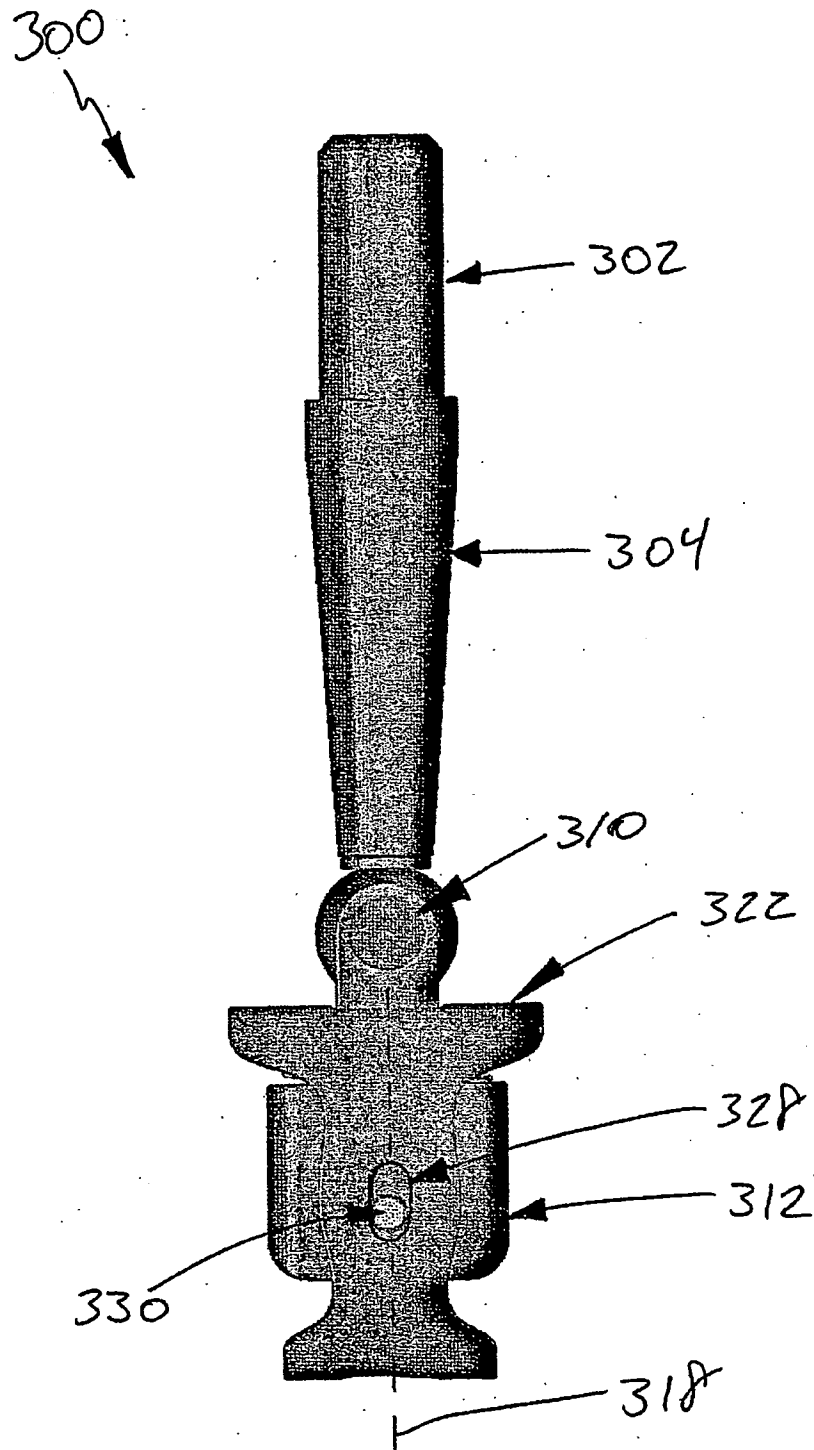


FIG. 3E

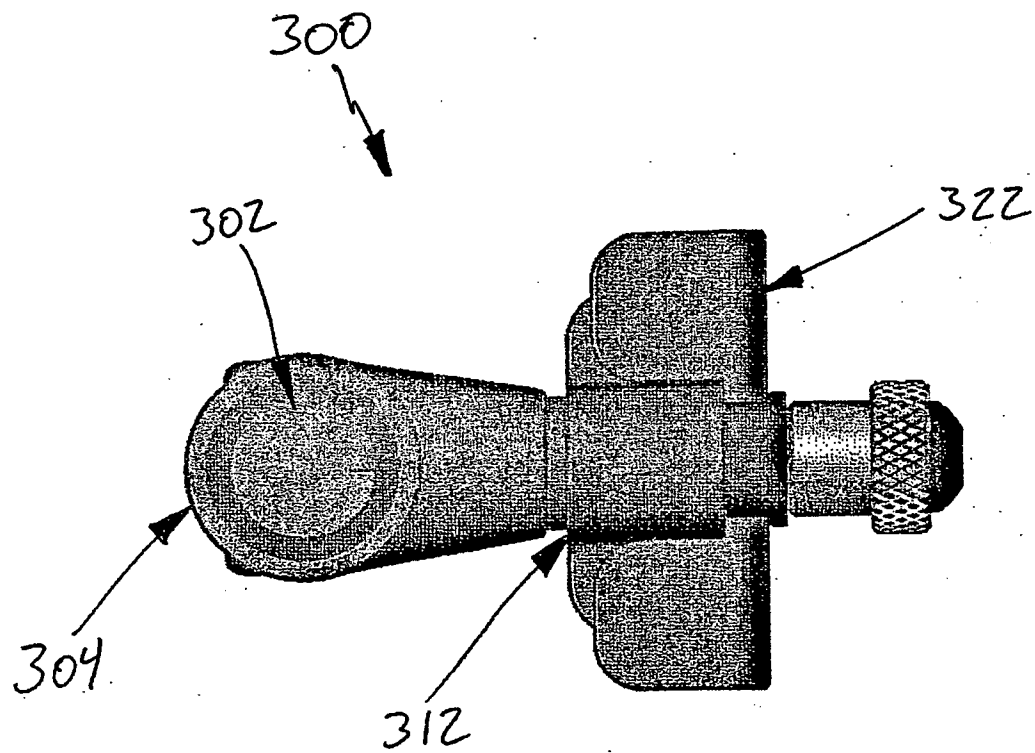


FIG. 3F

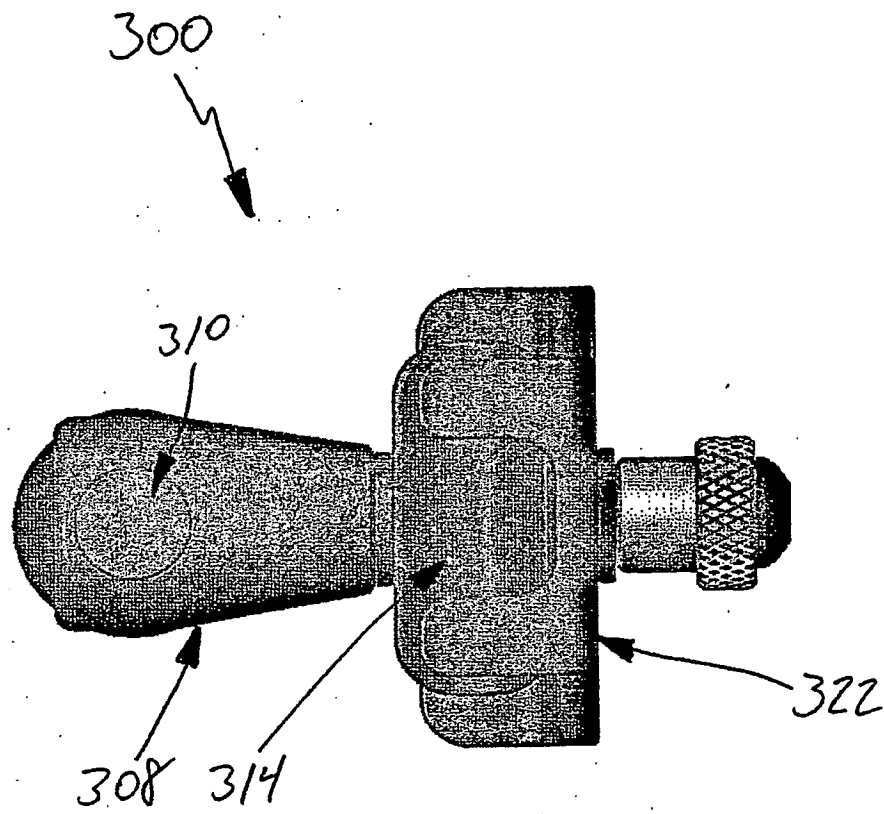


FIG. 3G

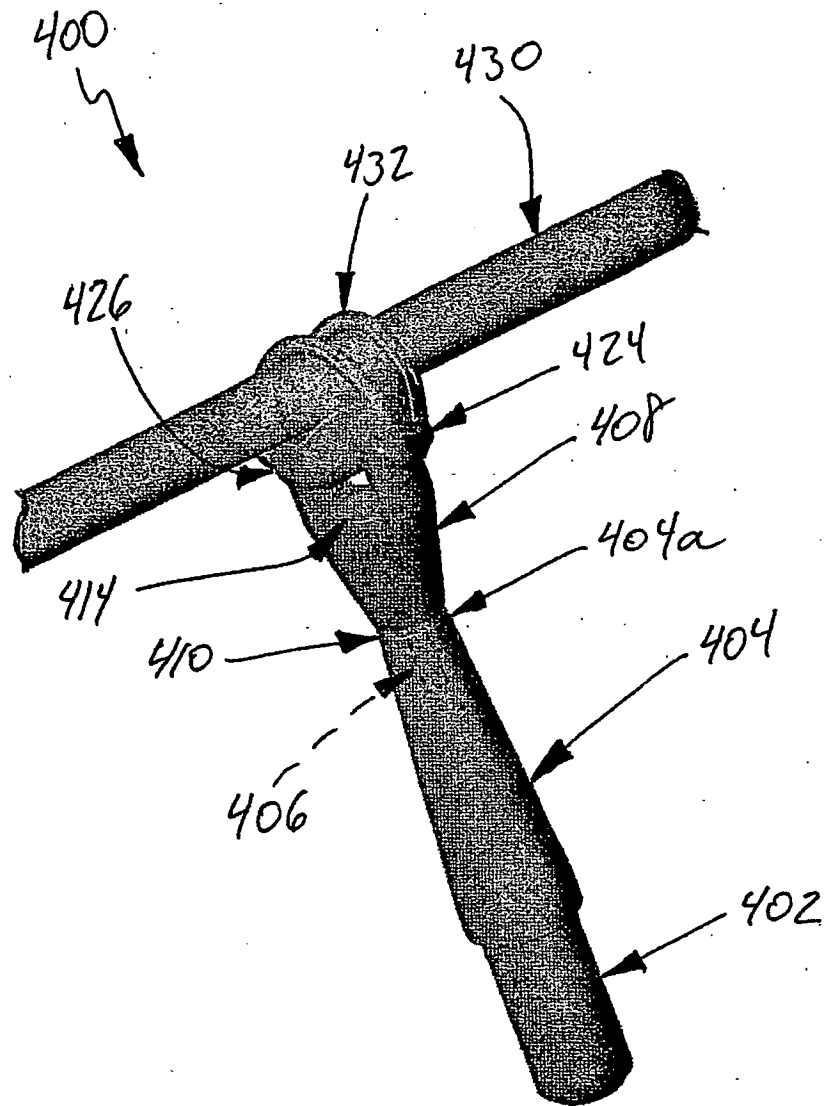


FIG. 3H

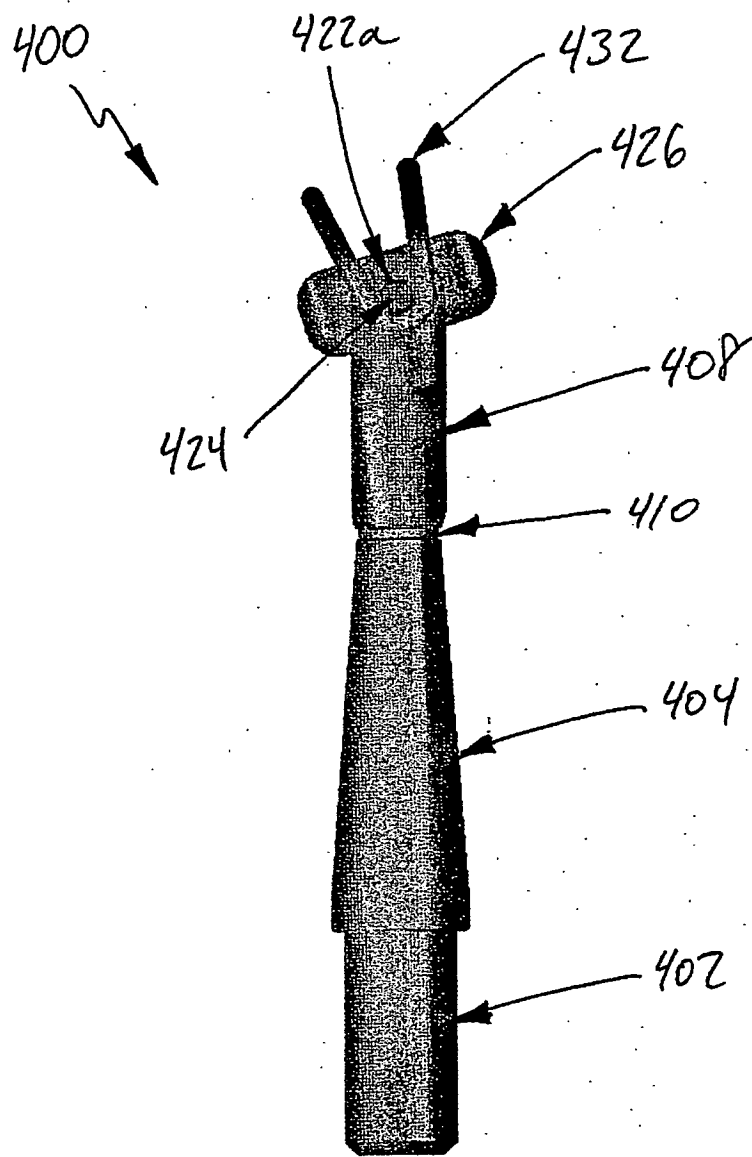


FIG. 3I

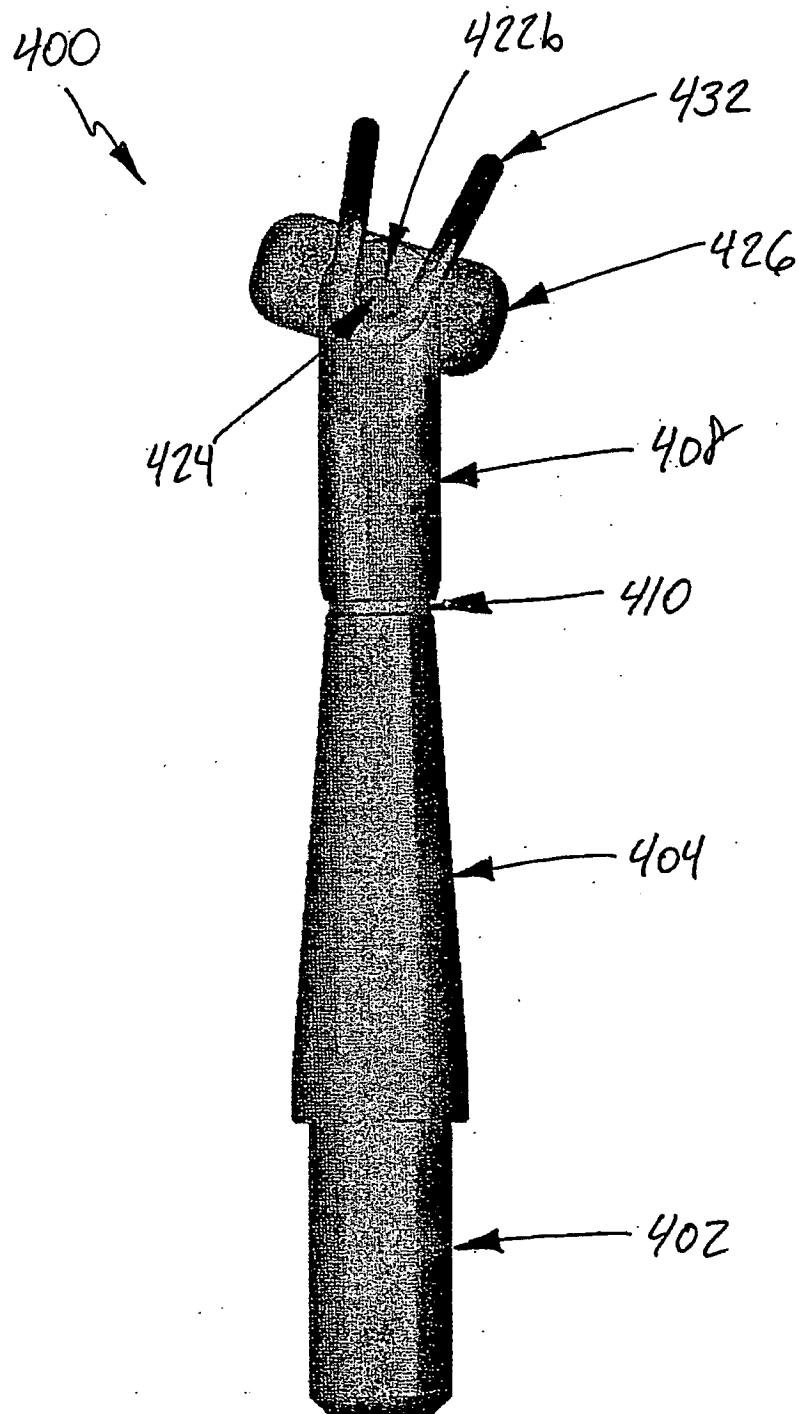


FIG. 3J

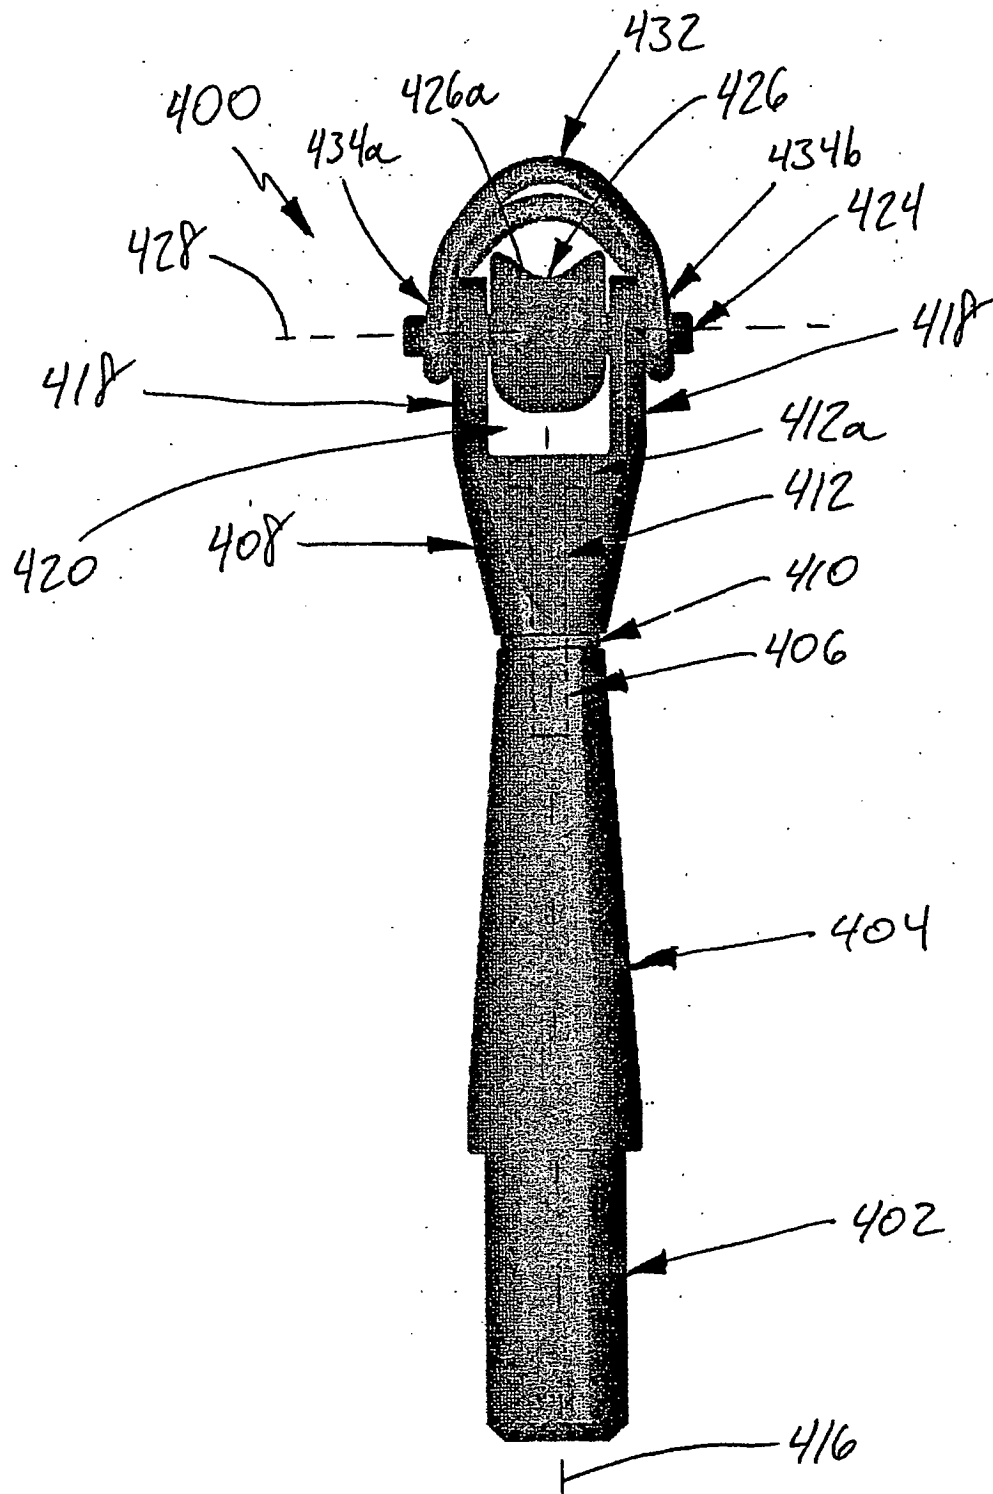


FIG. 3K

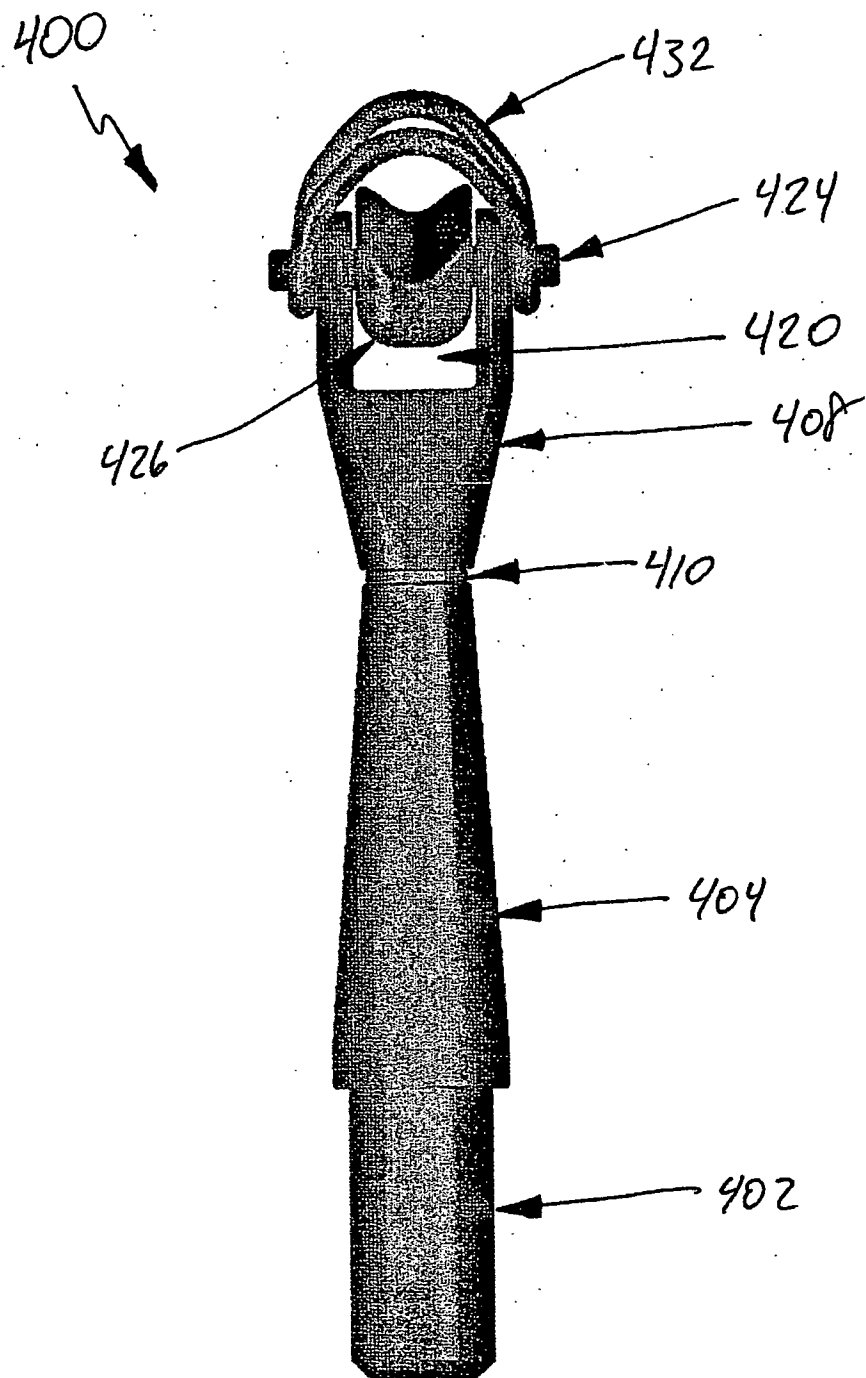


FIG. 3L

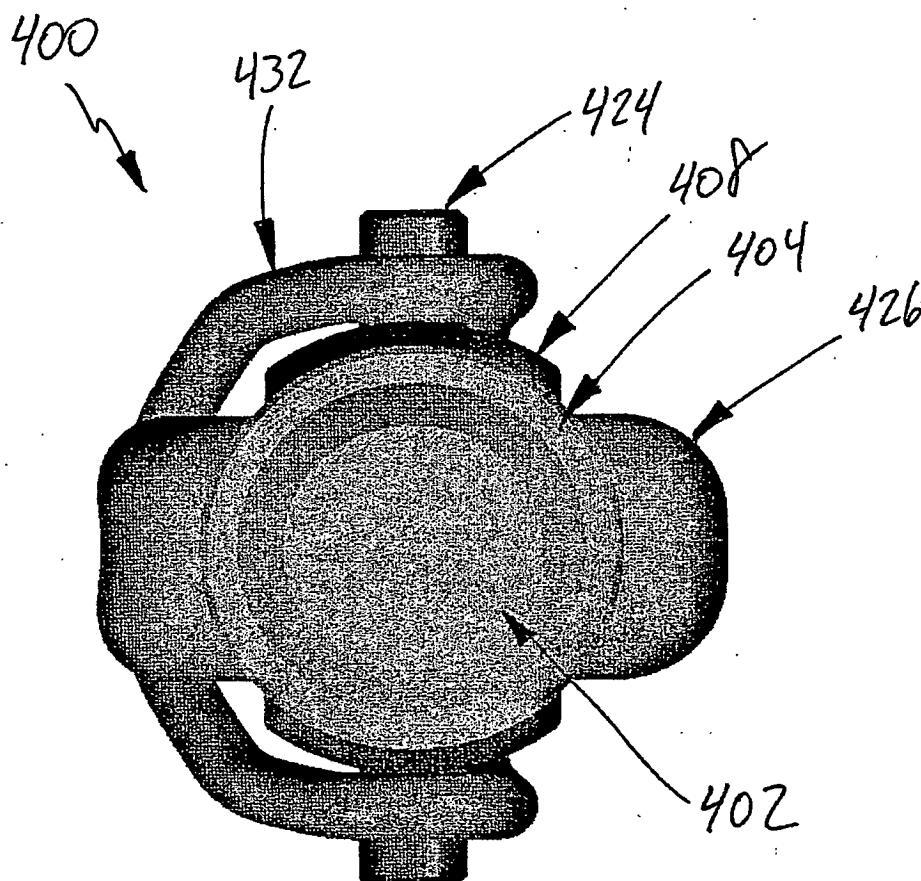


FIG. 3M

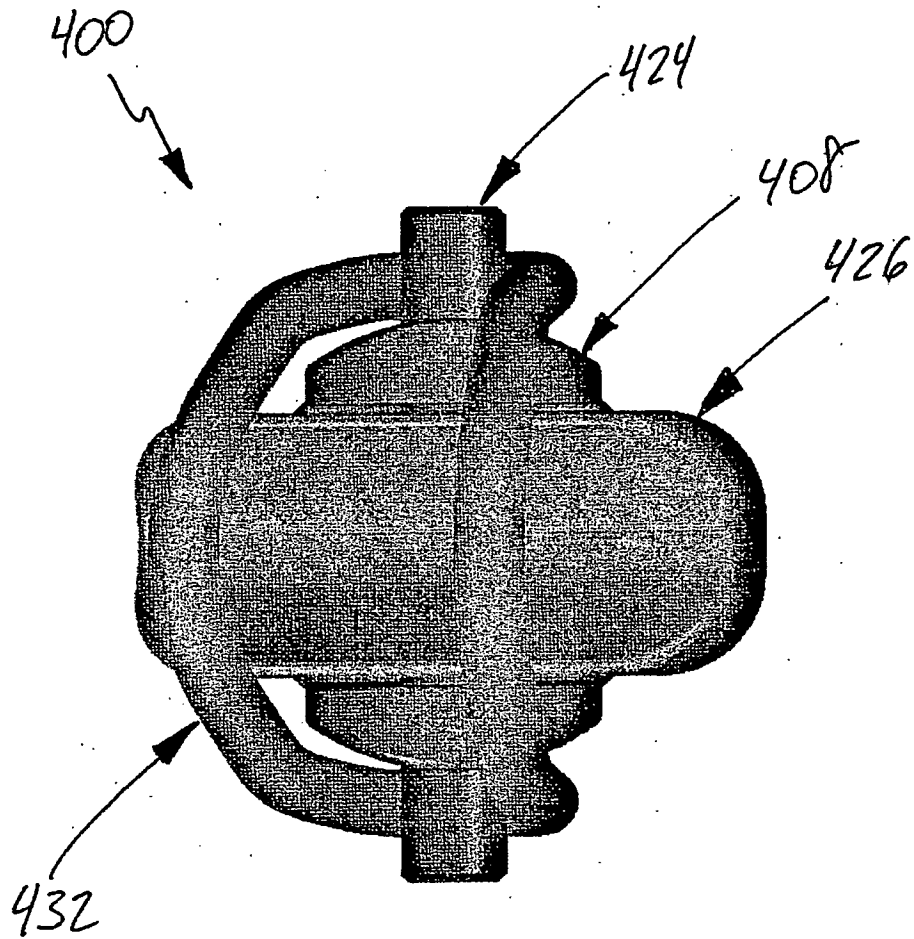


FIG. 3N

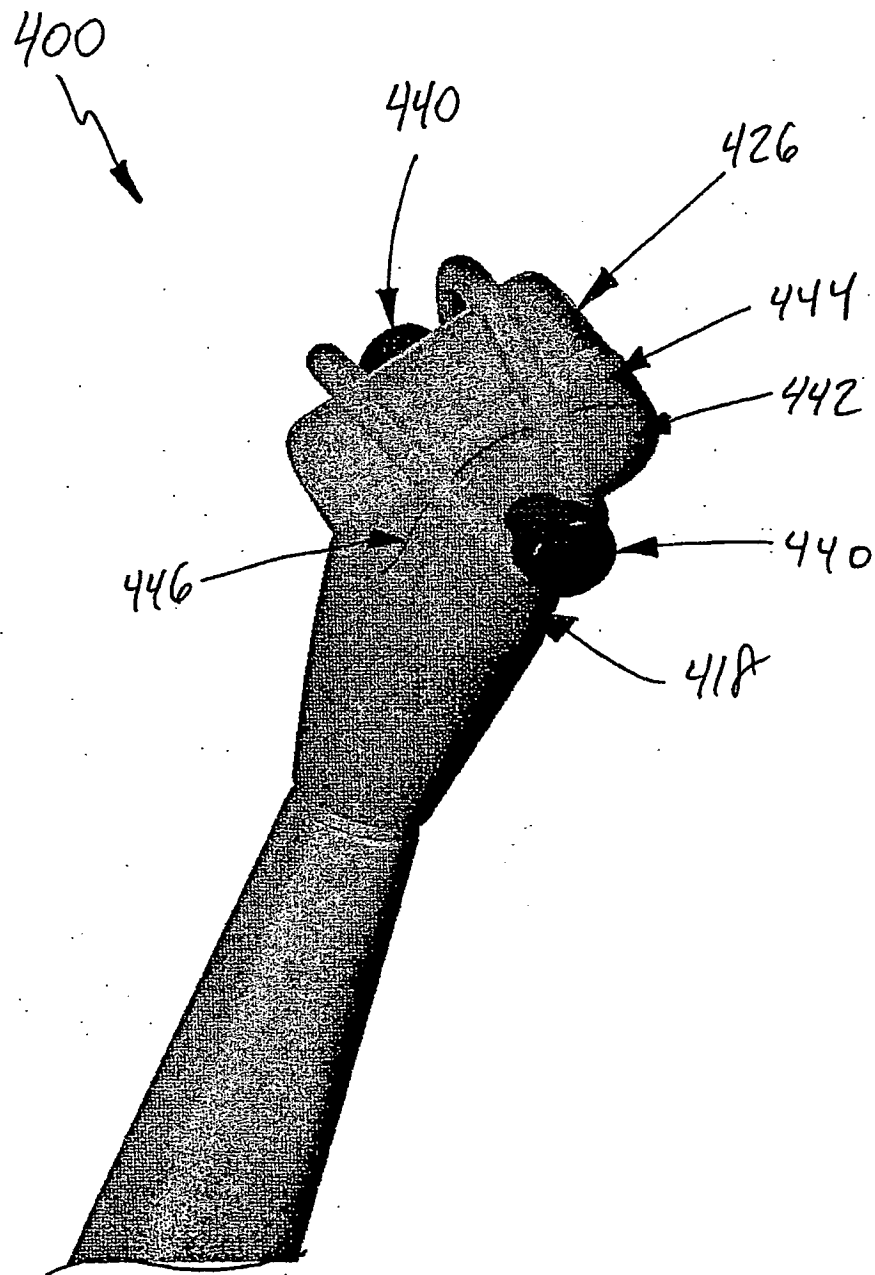


FIG. 3-O

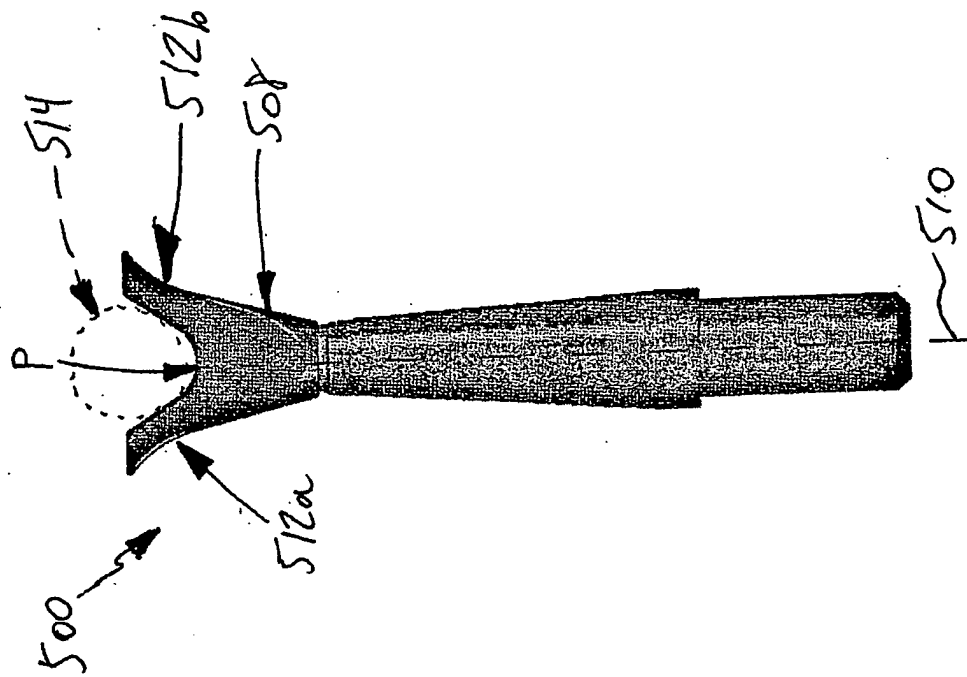


FIG. 3Q

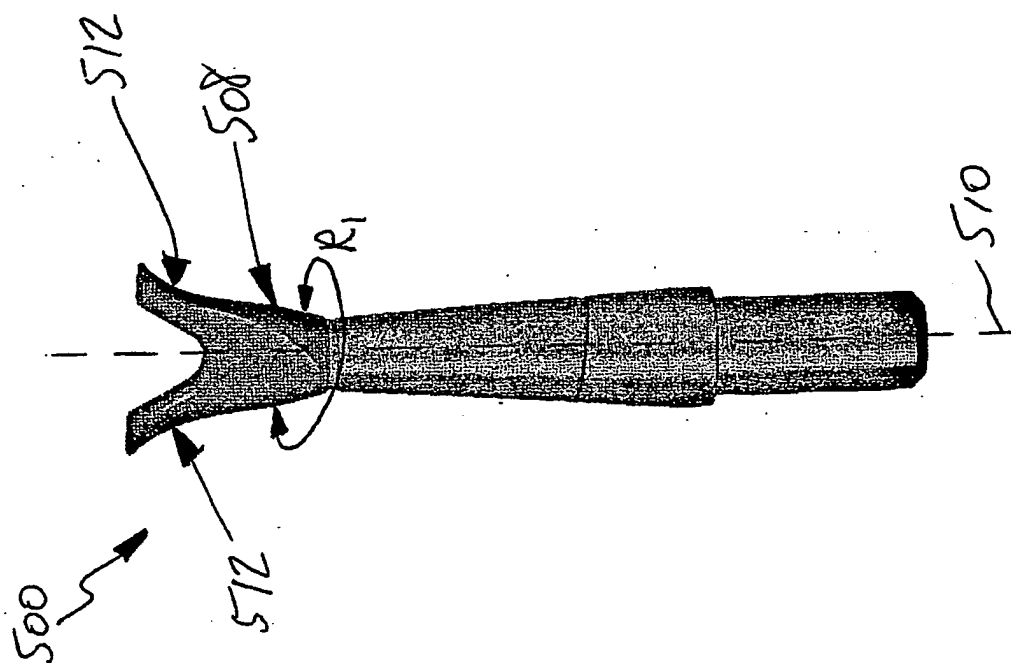


FIG. 3P

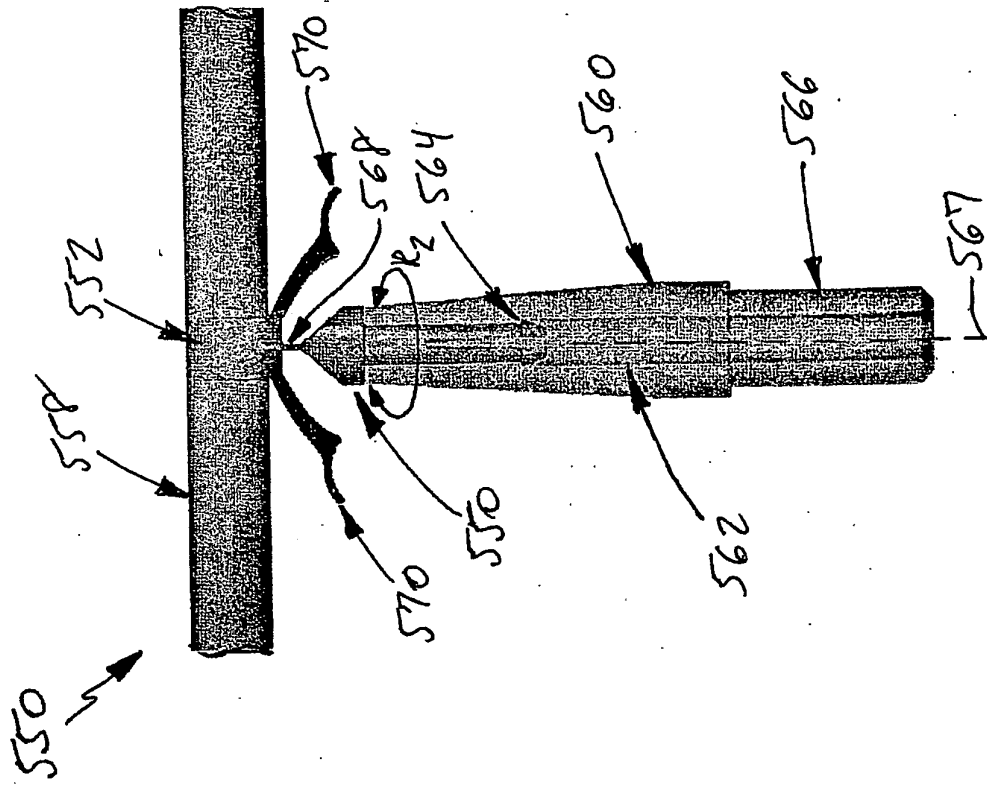


FIG. 35

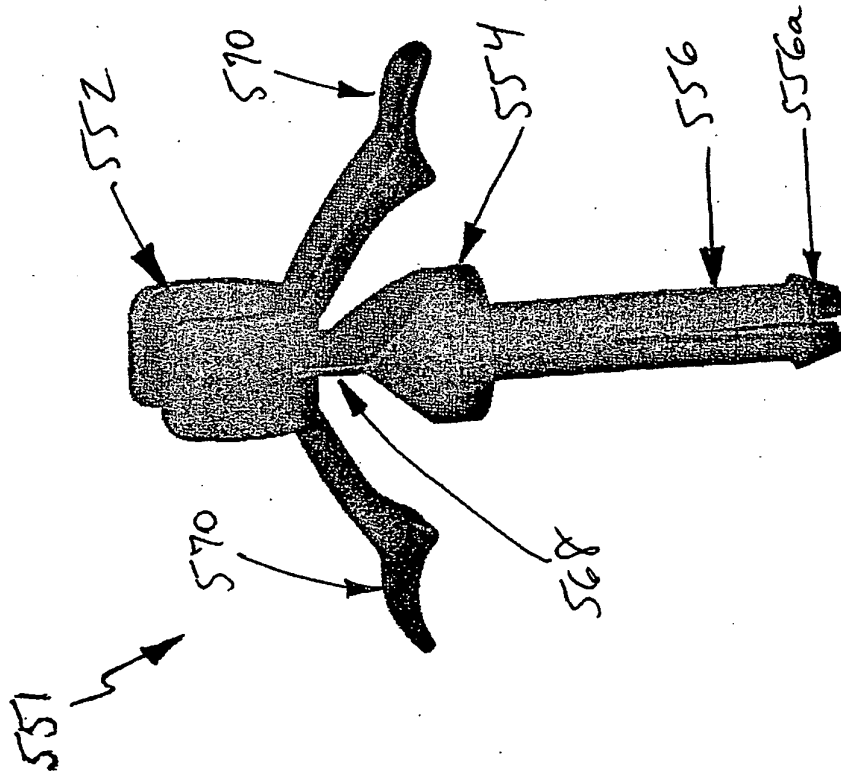
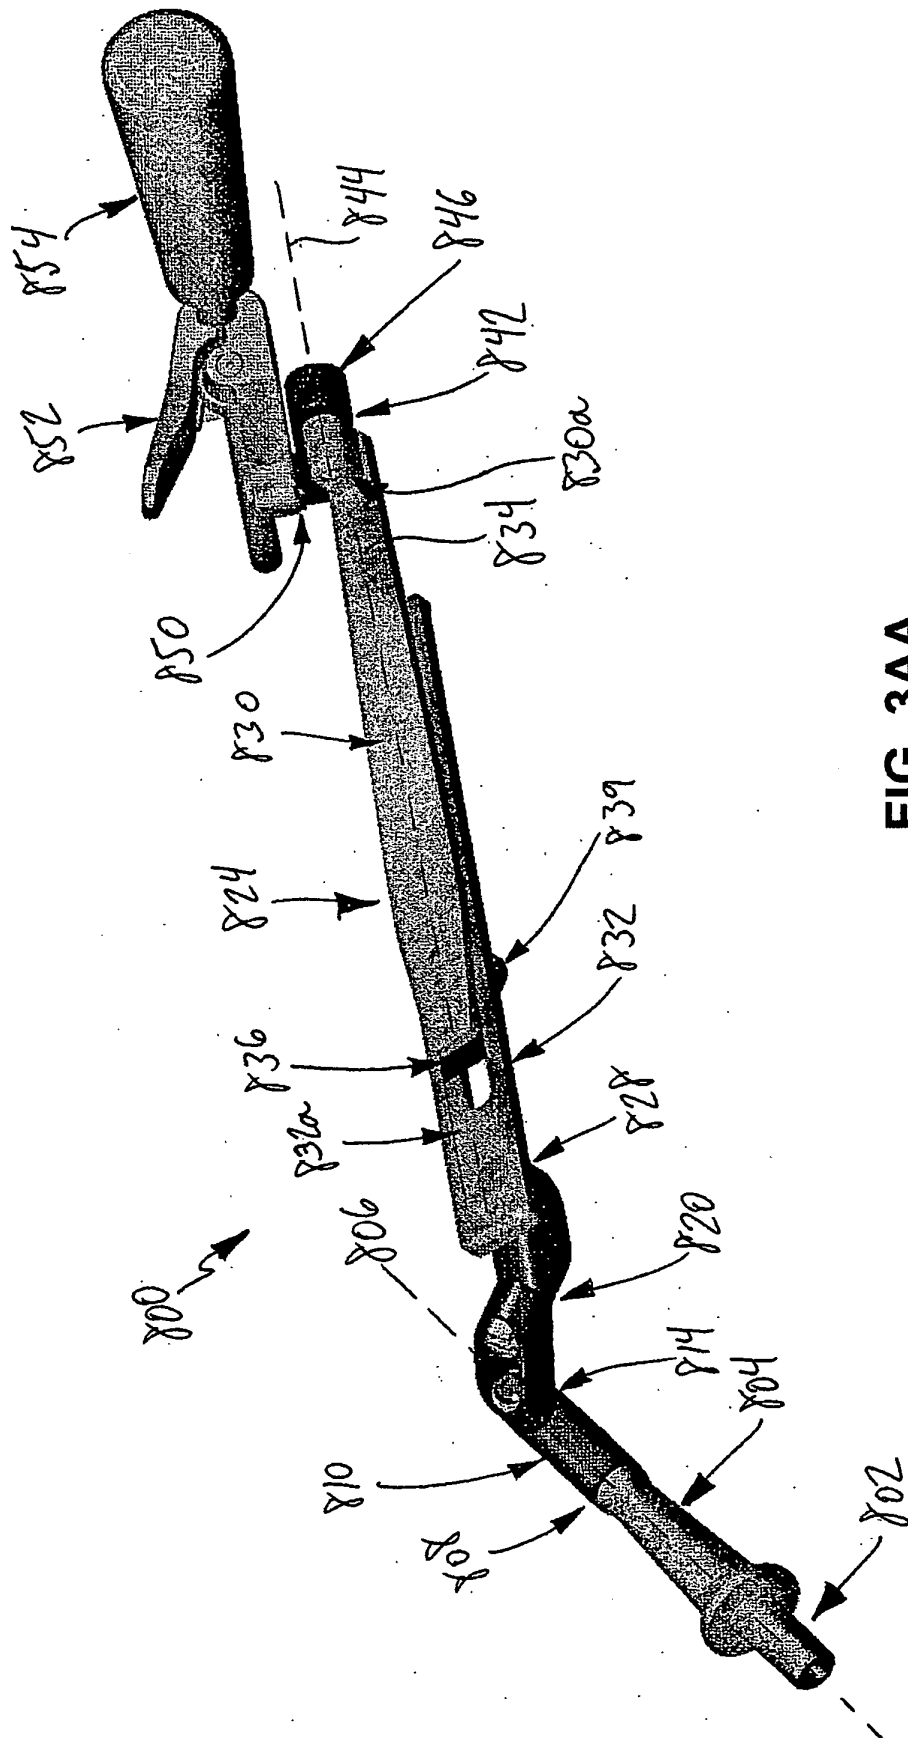


FIG. 3R



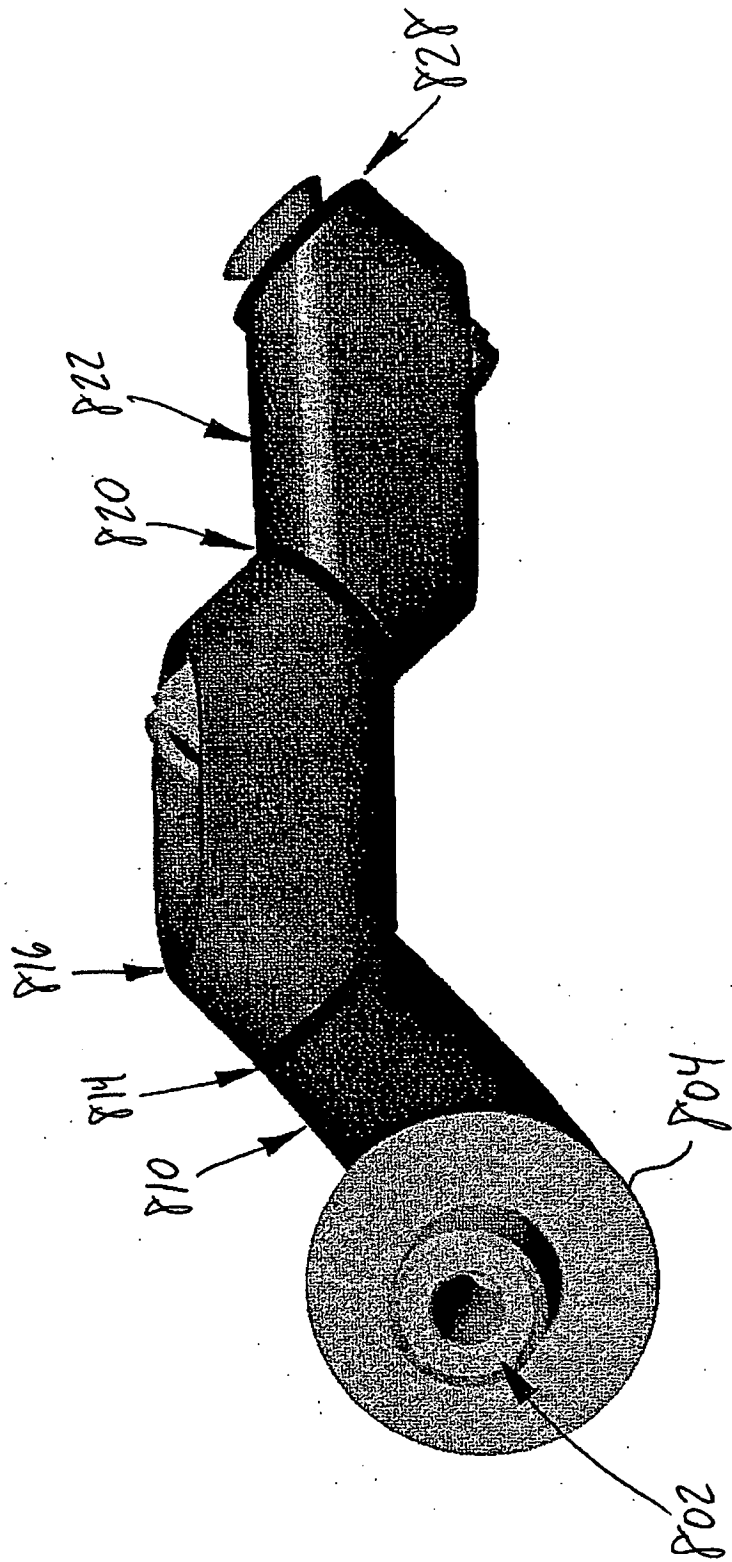


FIG. 3BB

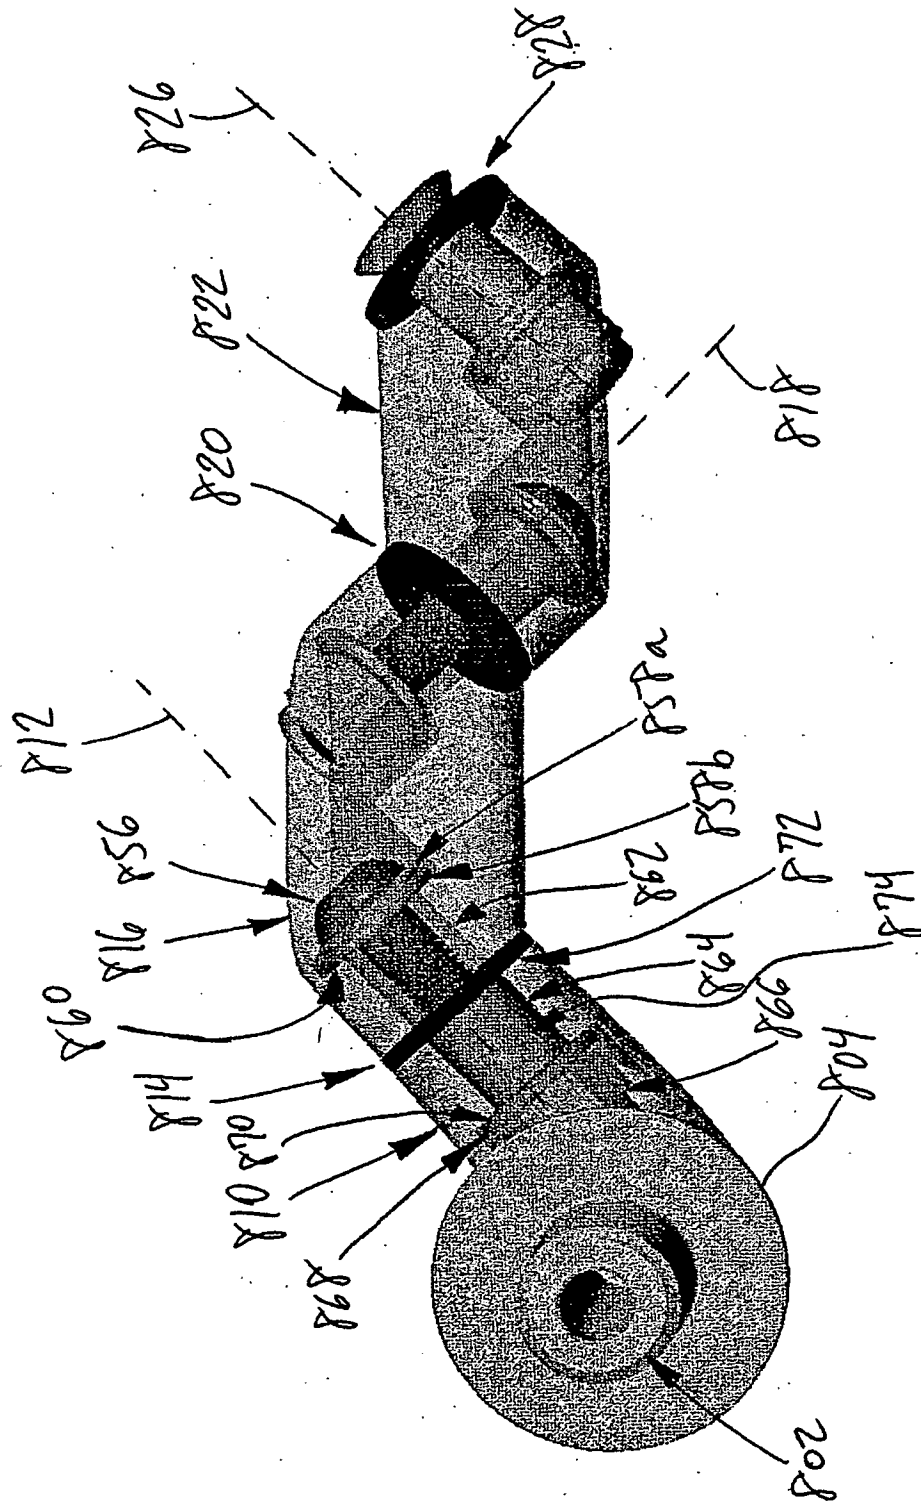


FIG. 3CC

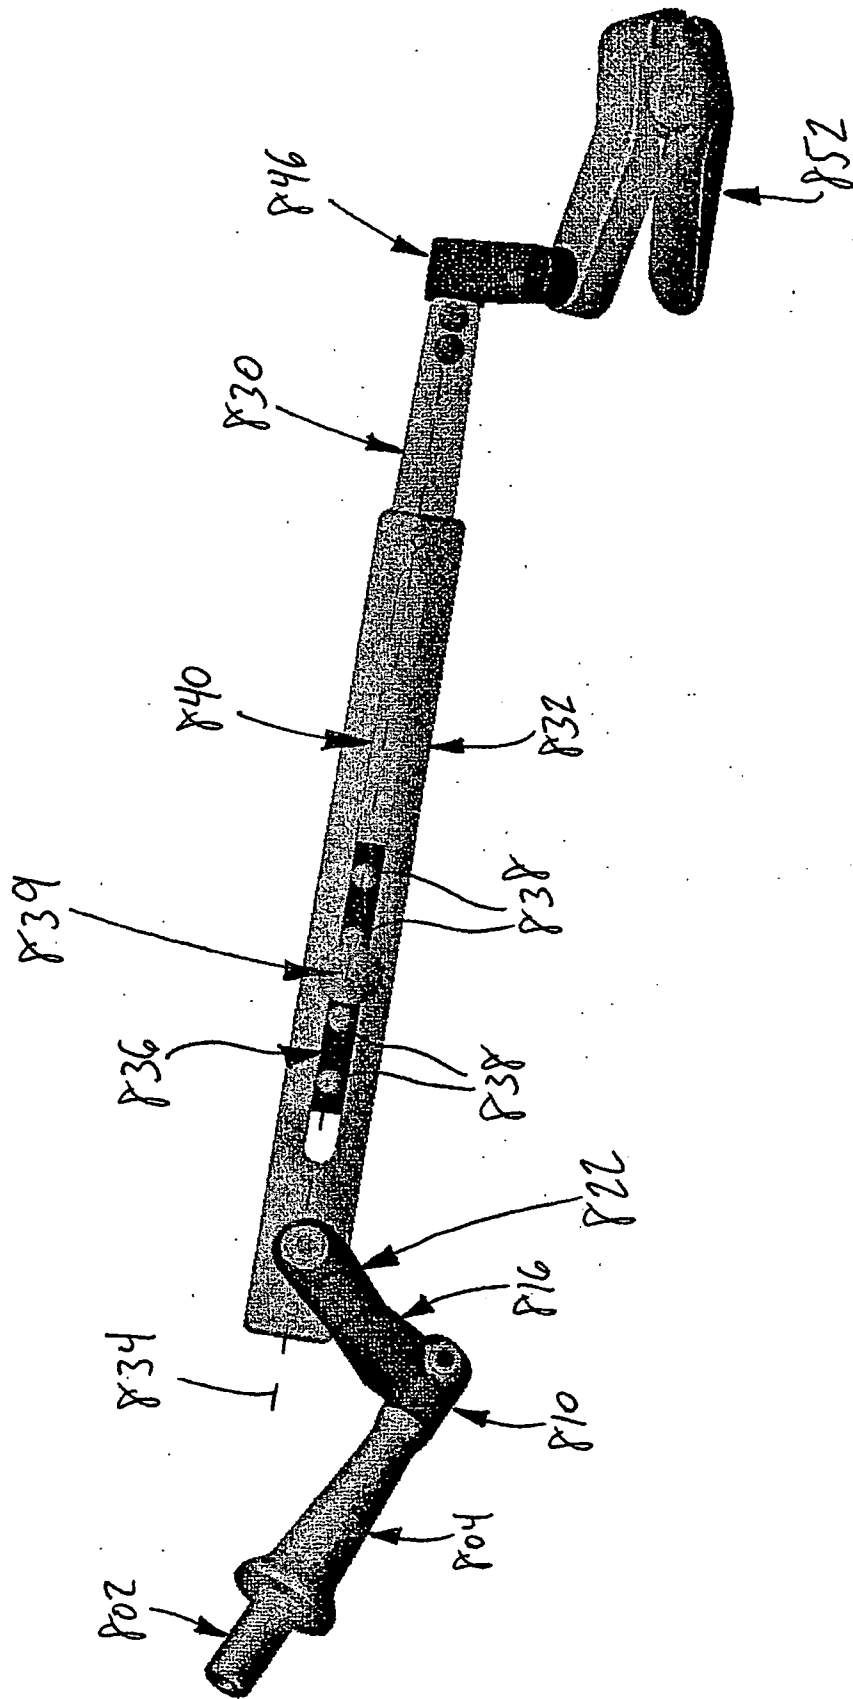


FIG. 3DD

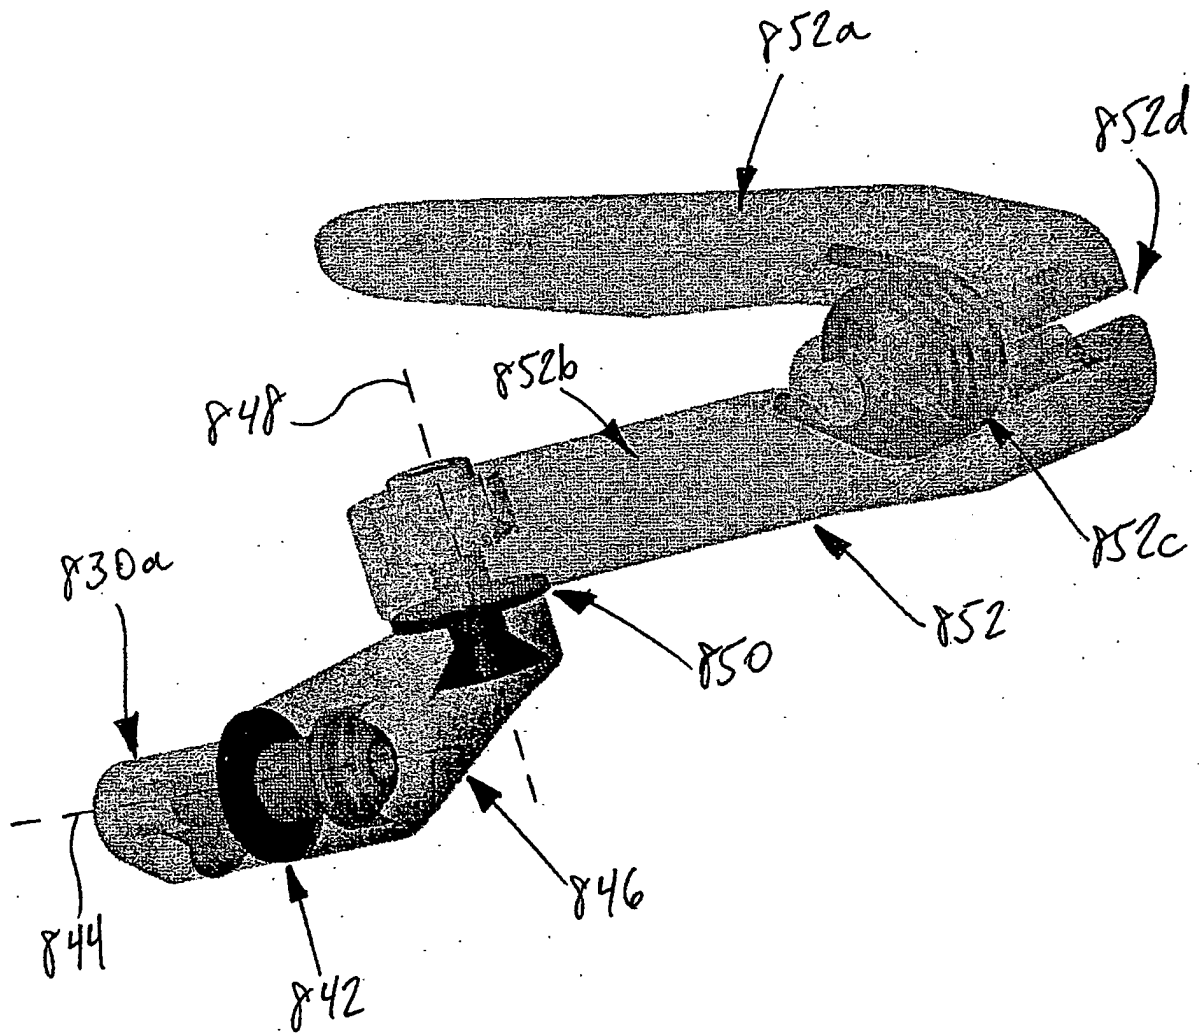


FIG. 3EE

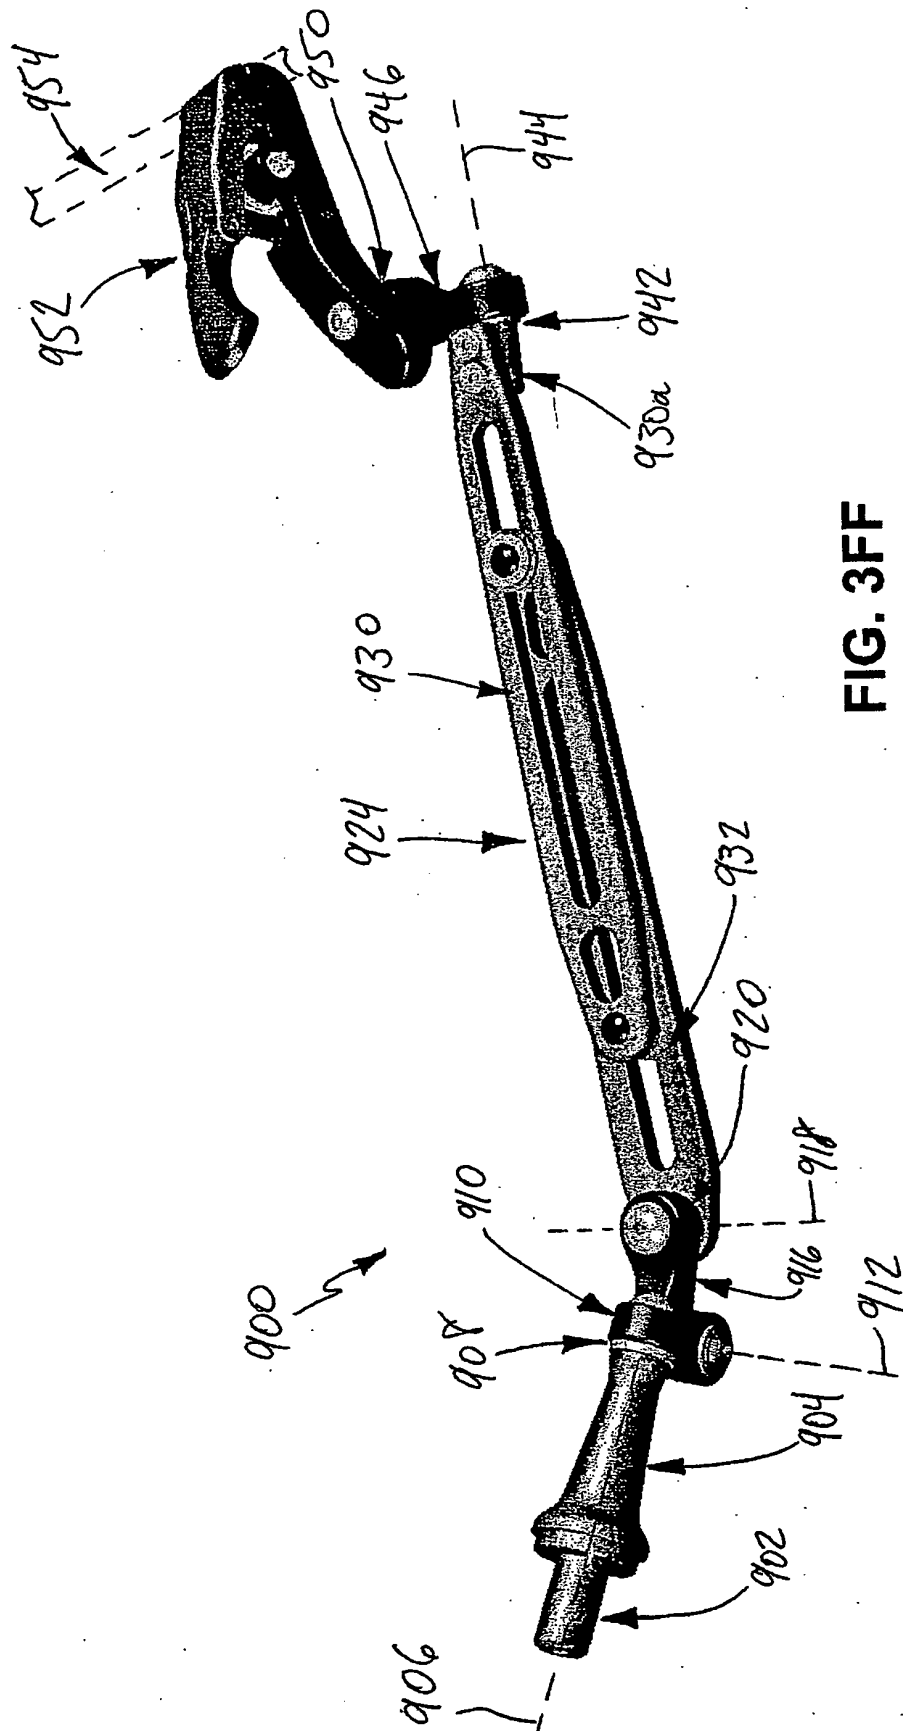
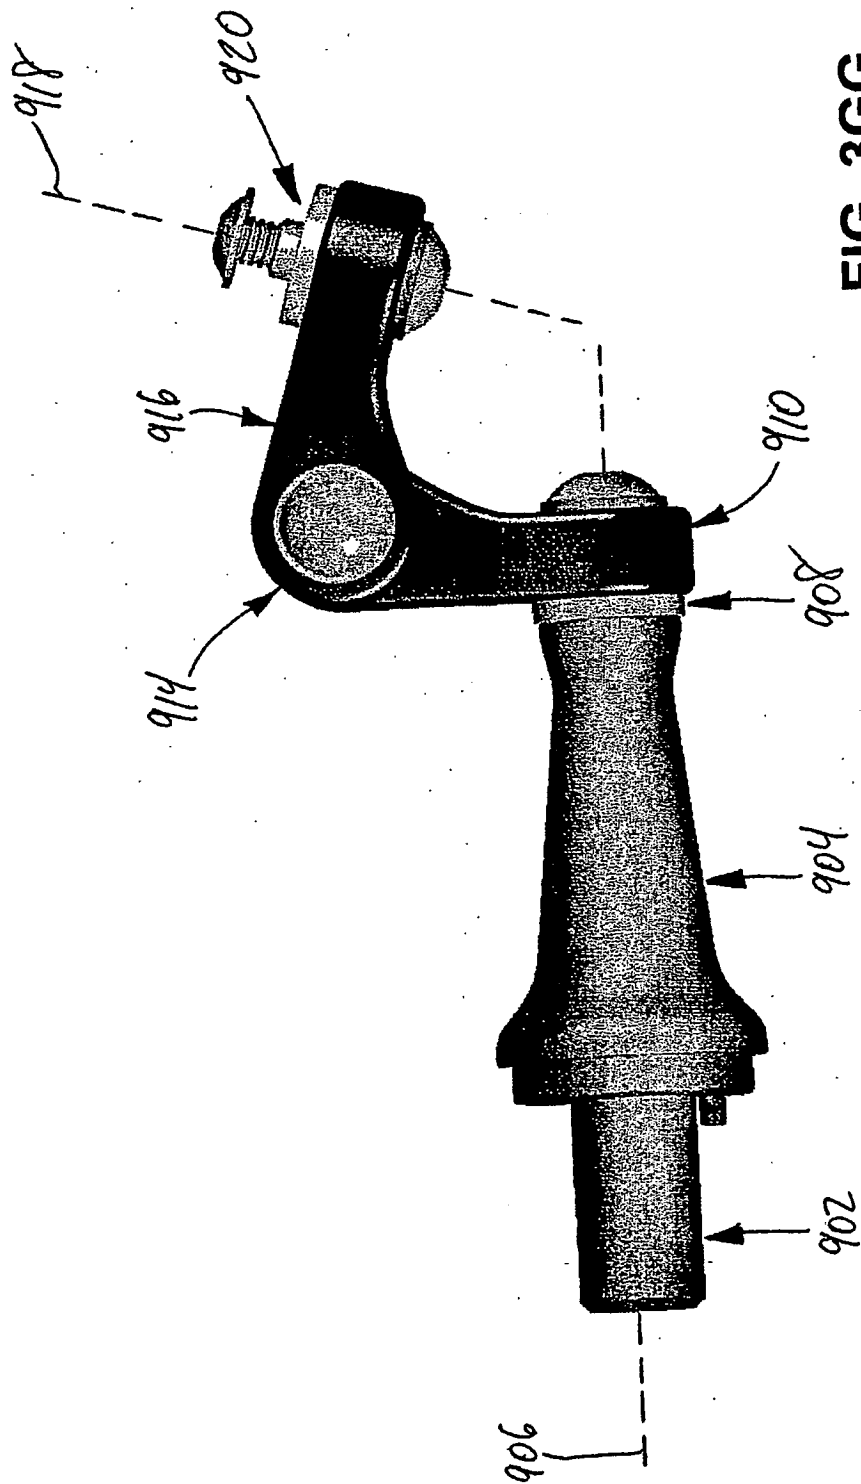


FIG. 3FF



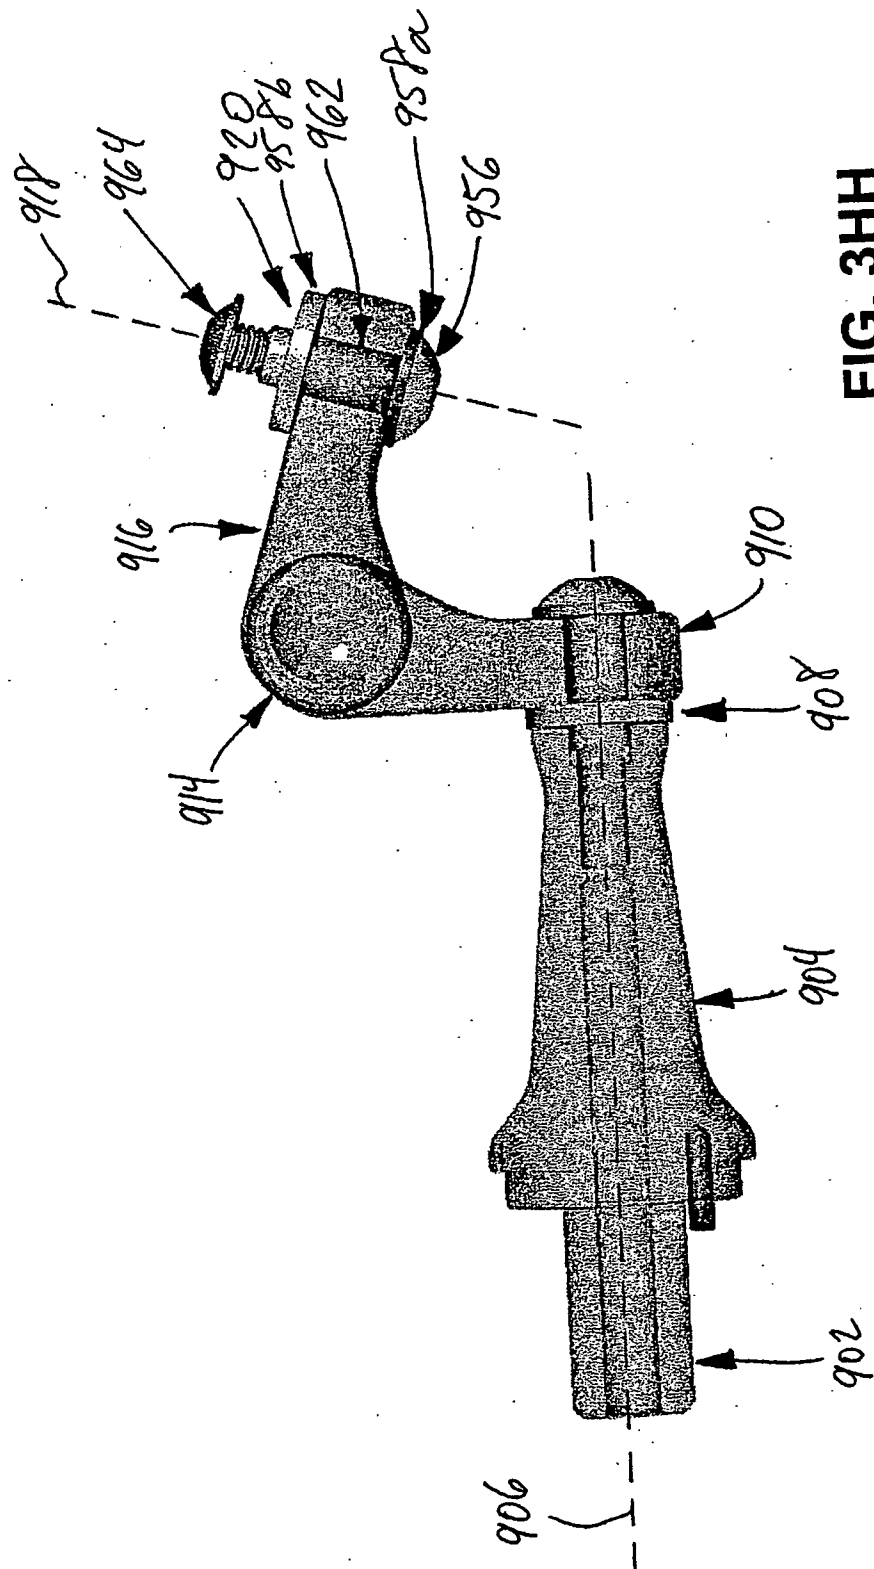


FIG. 3HH

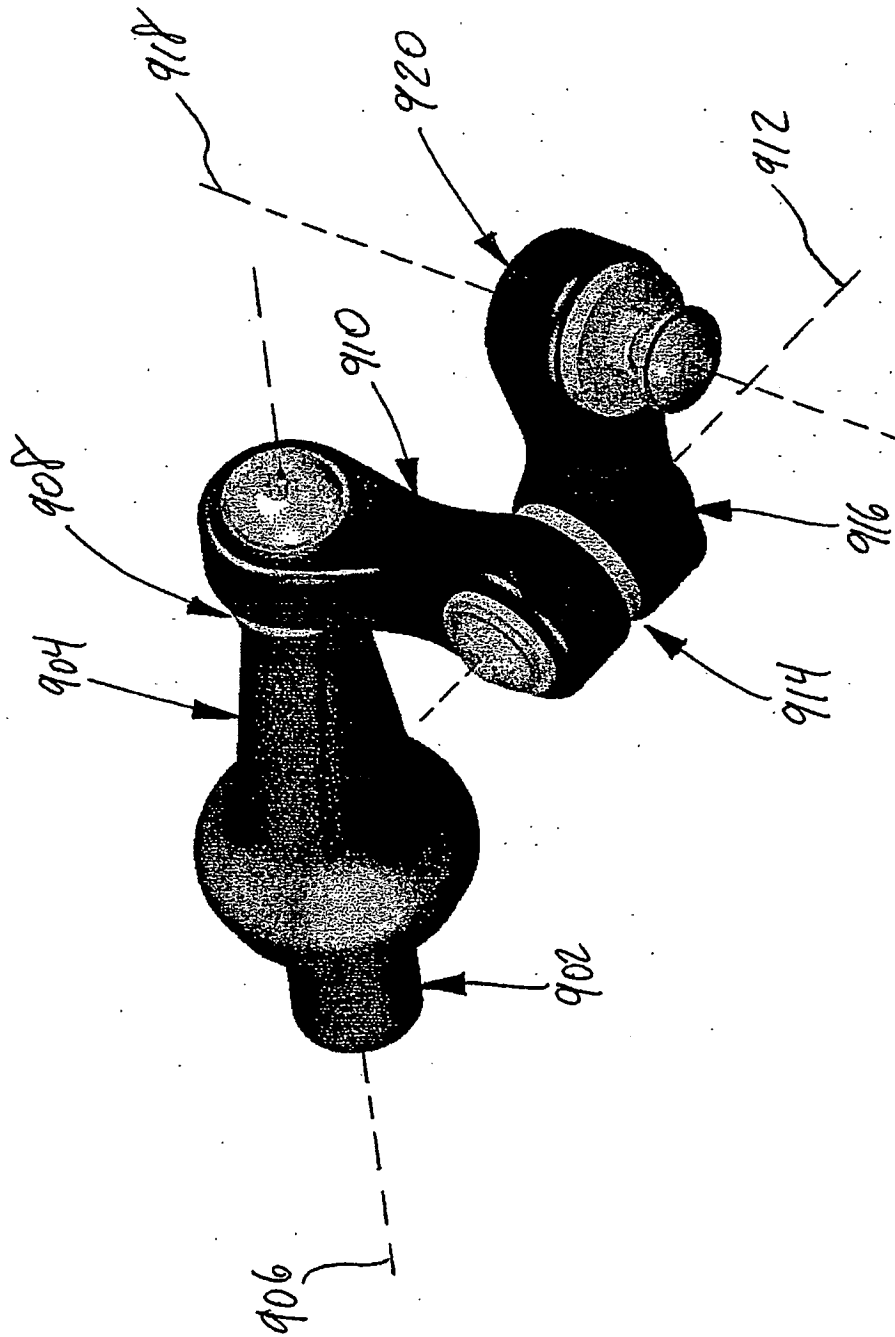
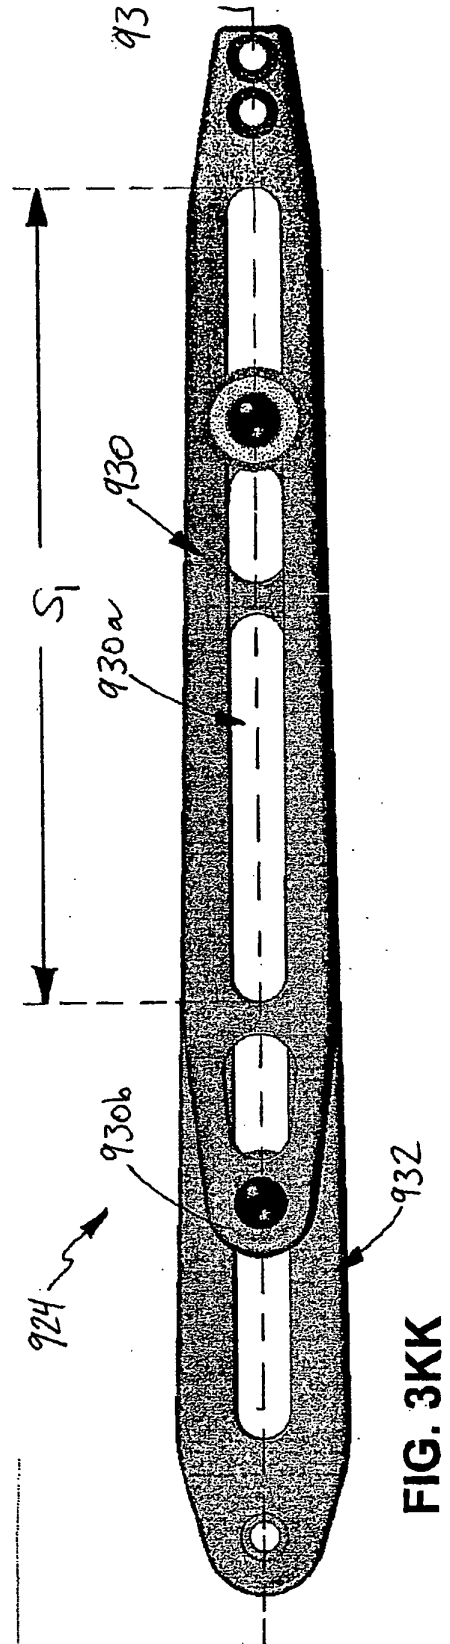
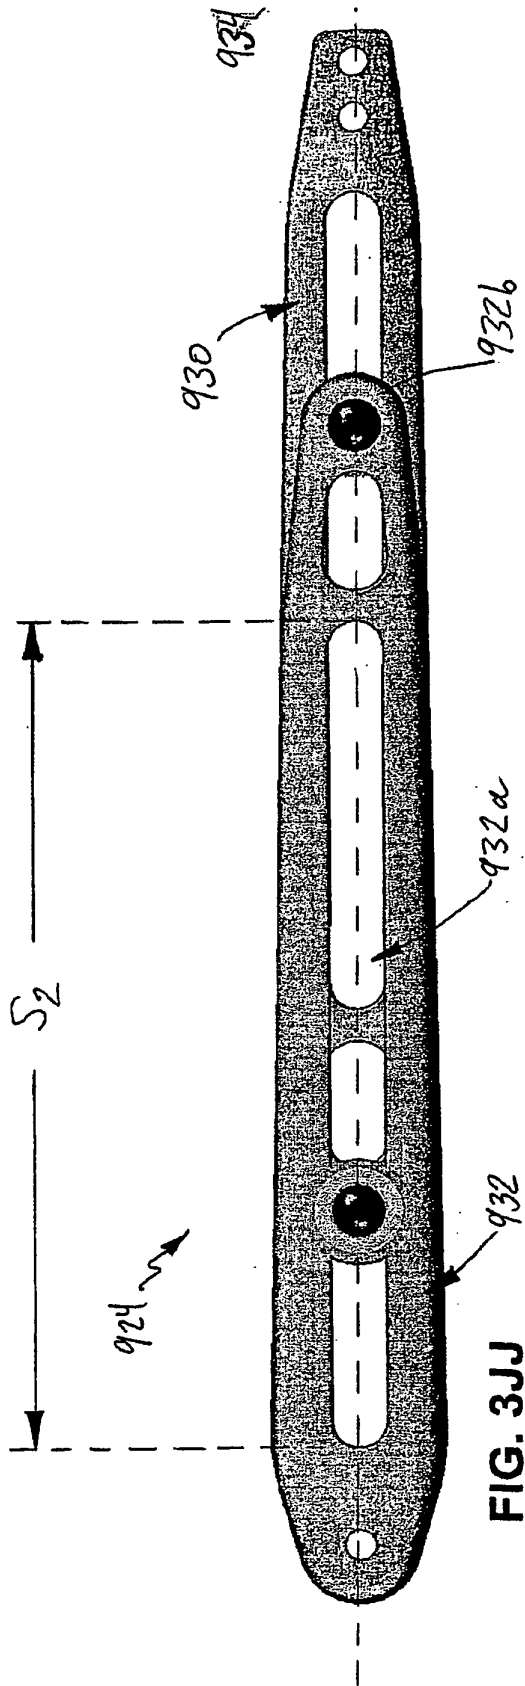


FIG. 3II



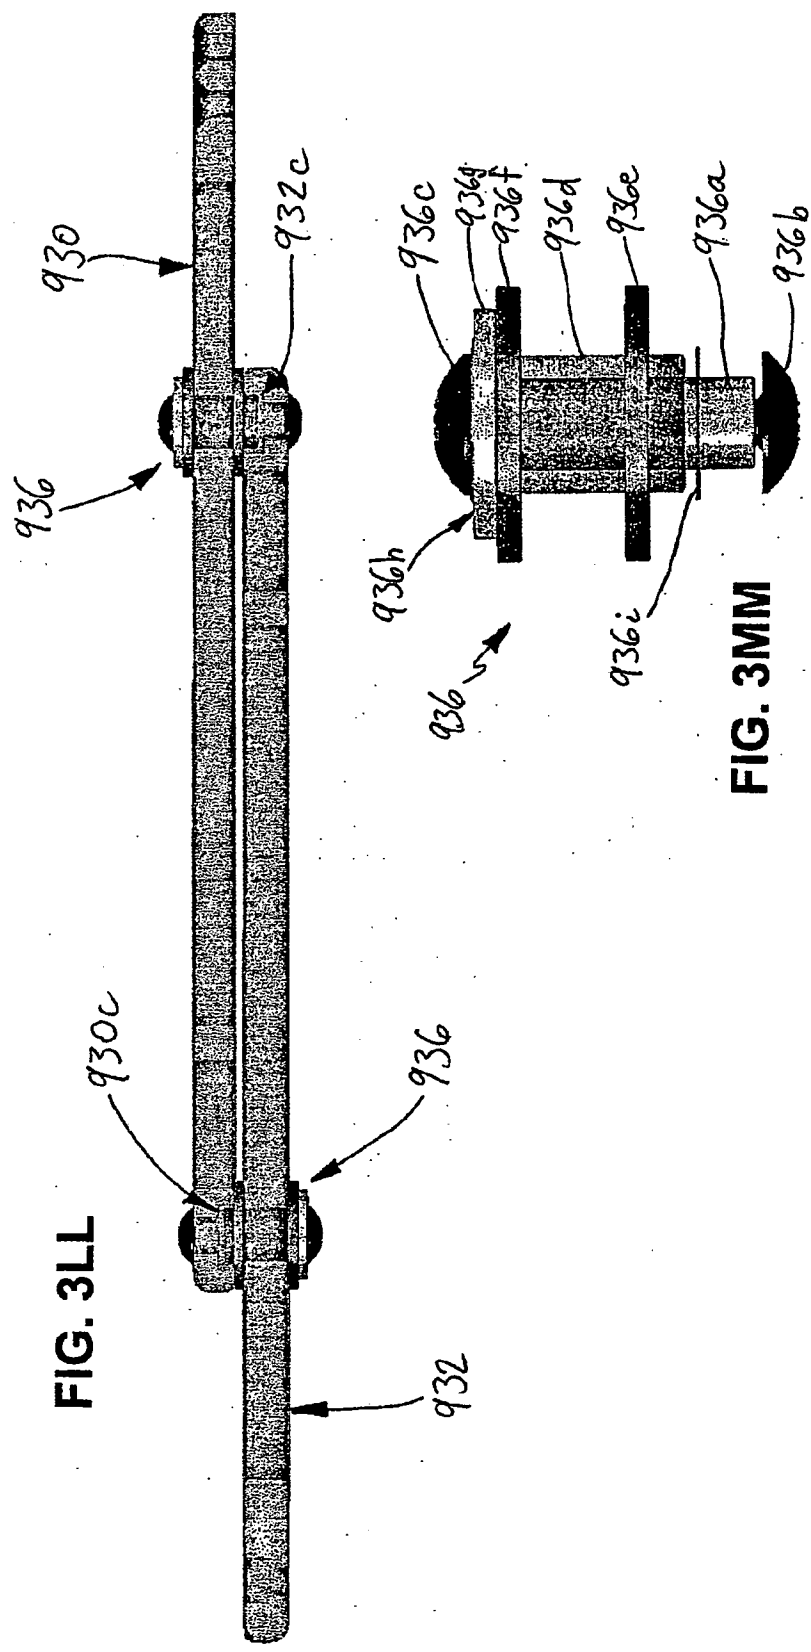


FIG. 3LL

FIG. 3MM

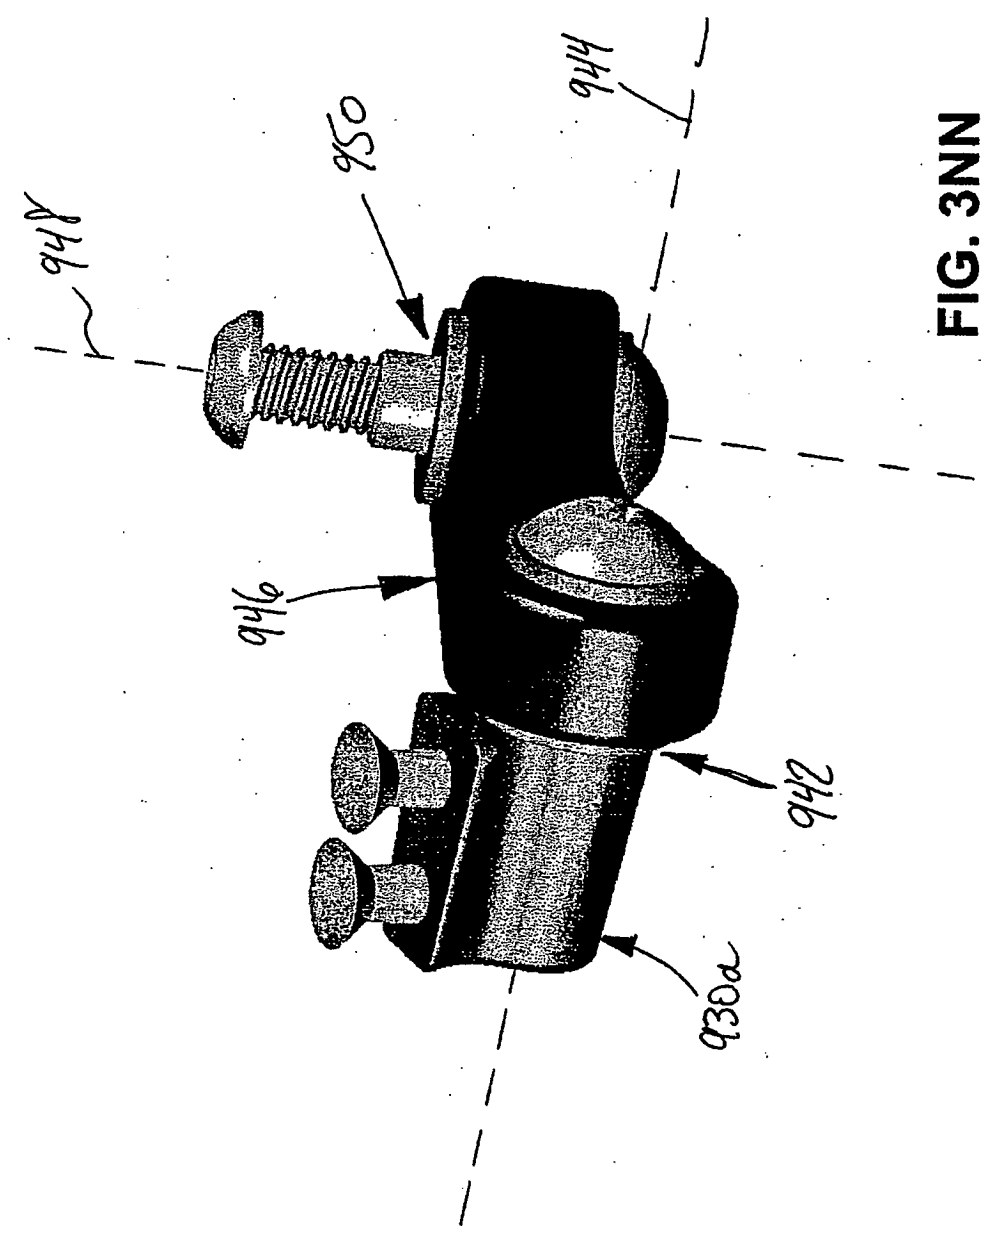


FIG. 3NN

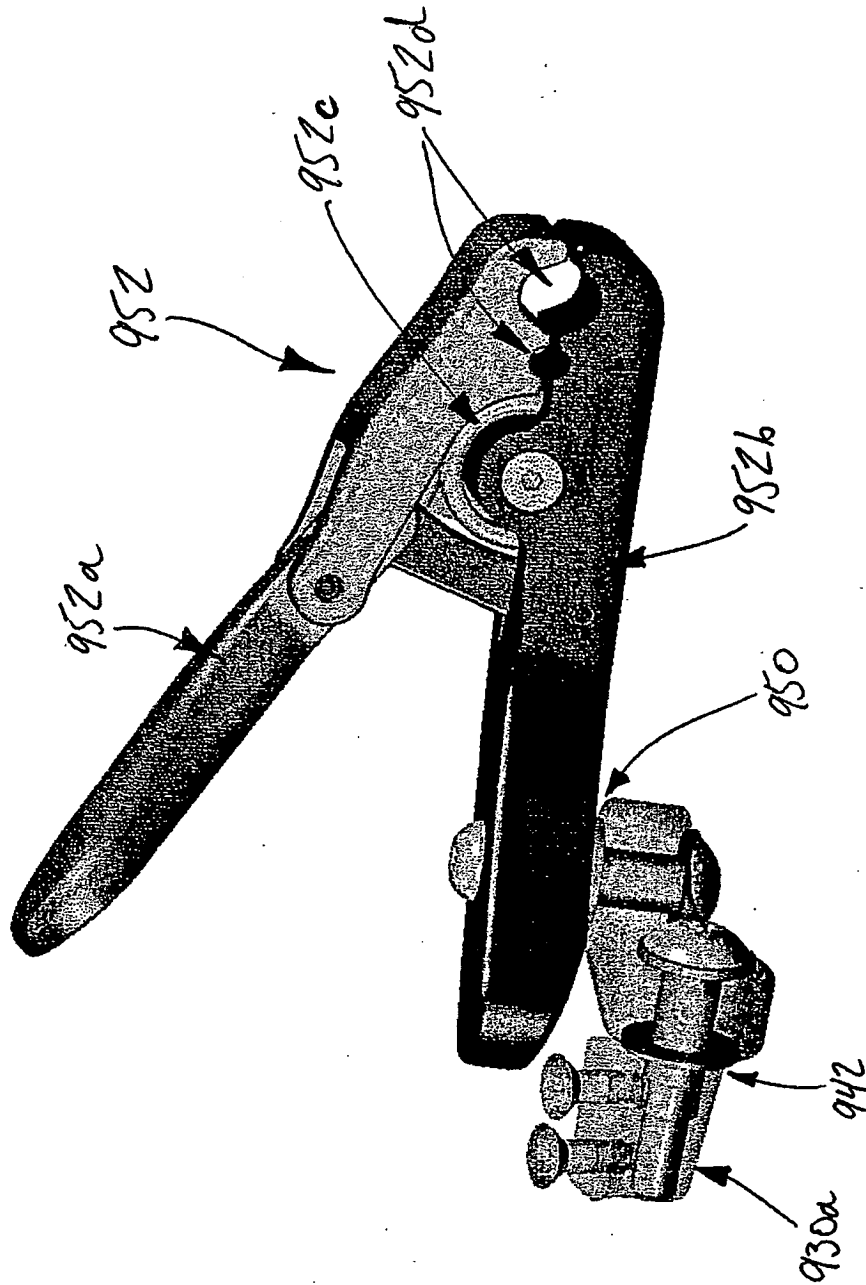


FIG. 3-00

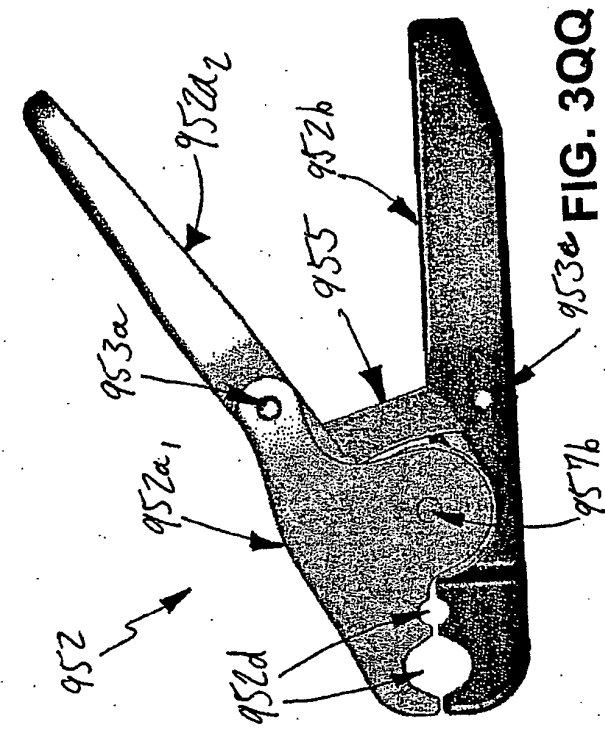


FIG. 3QQ

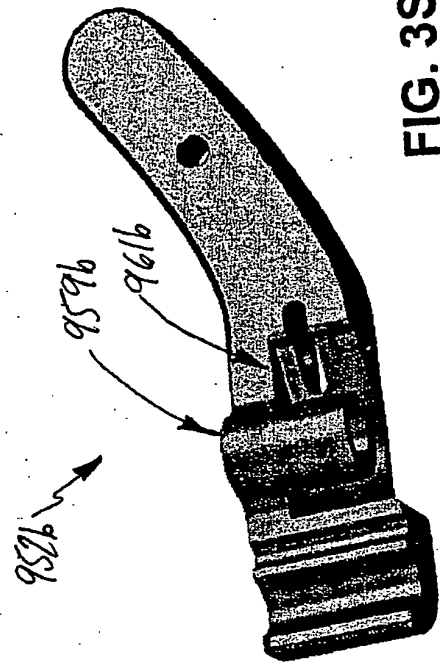


FIG. 3SS

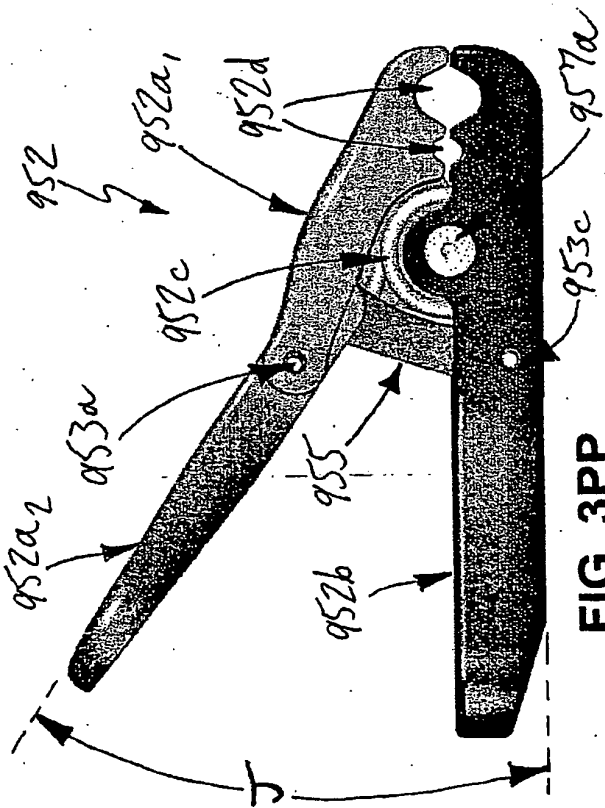


FIG. 3PP

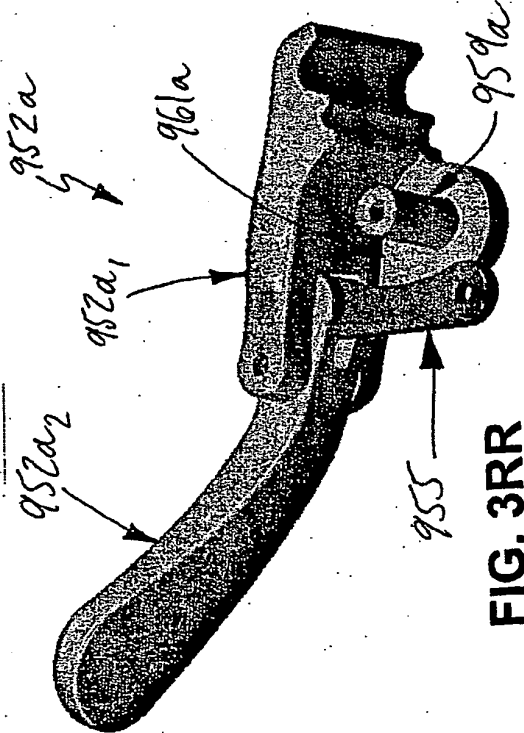


FIG. 3RR

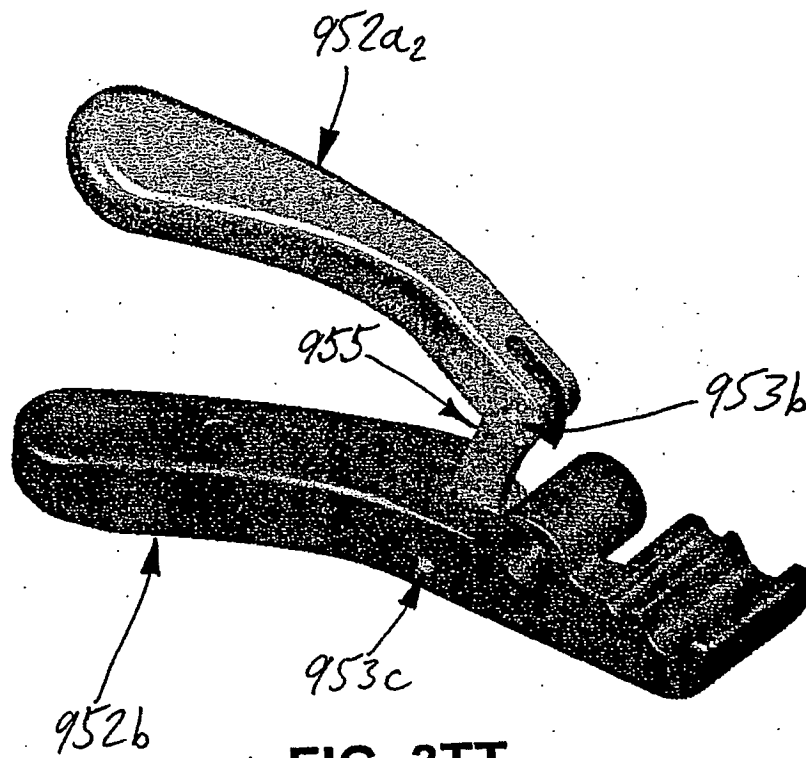


FIG. 3TT

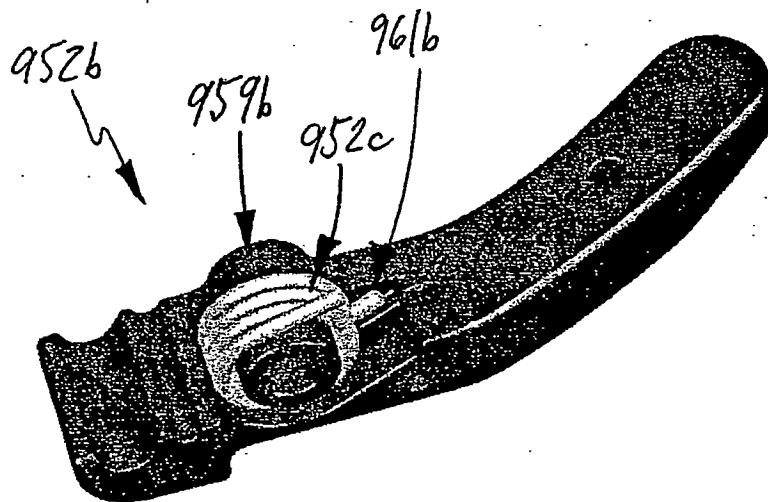
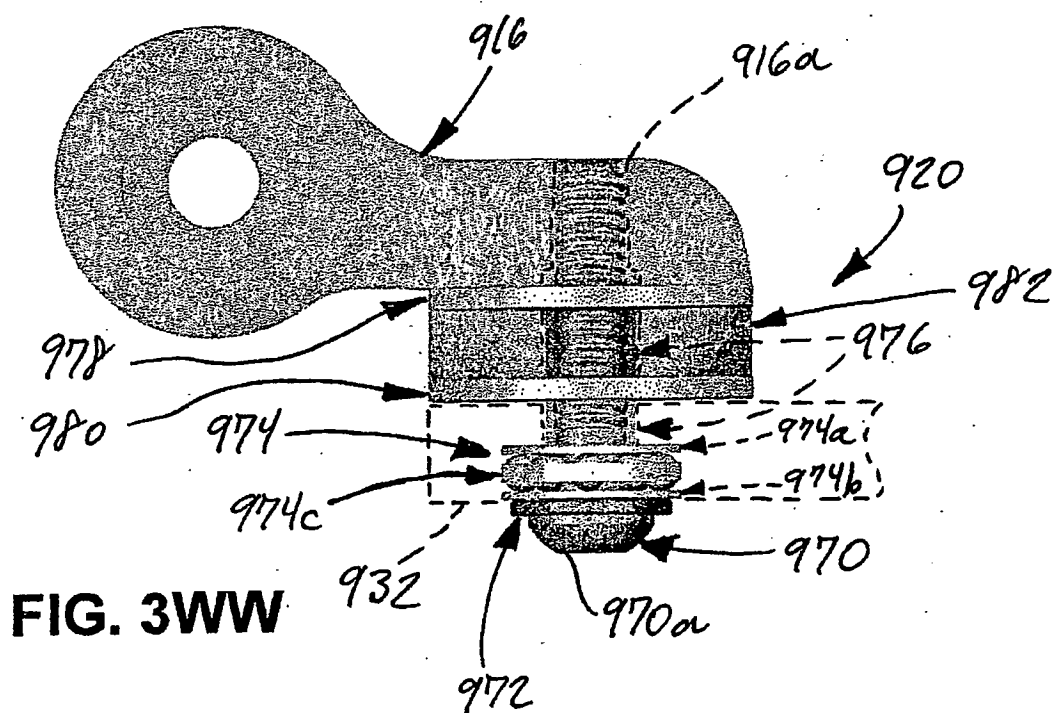
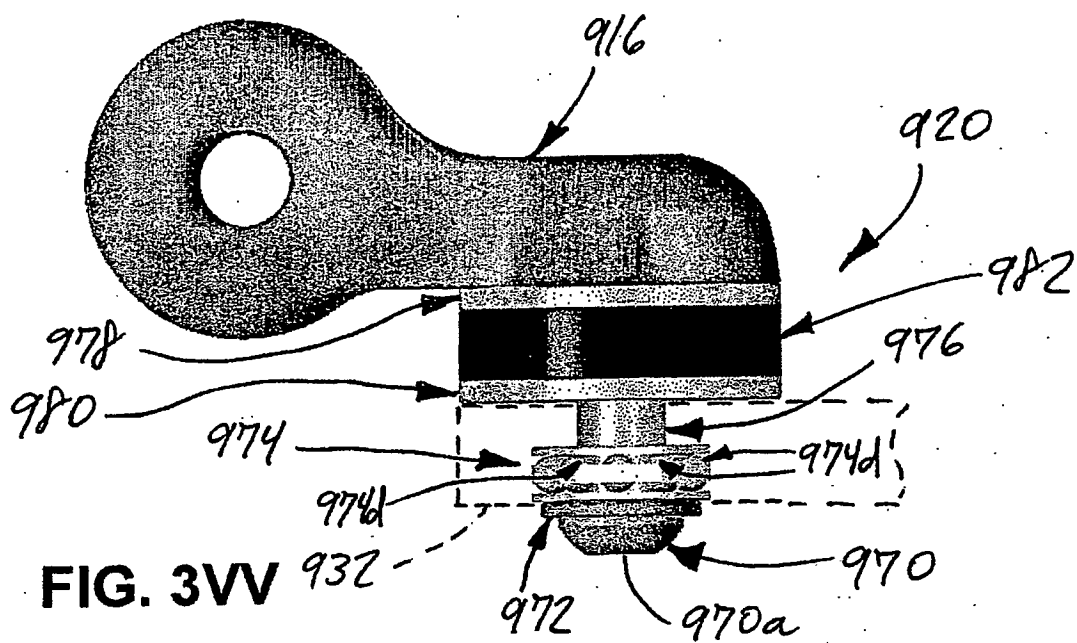


FIG. 3UU



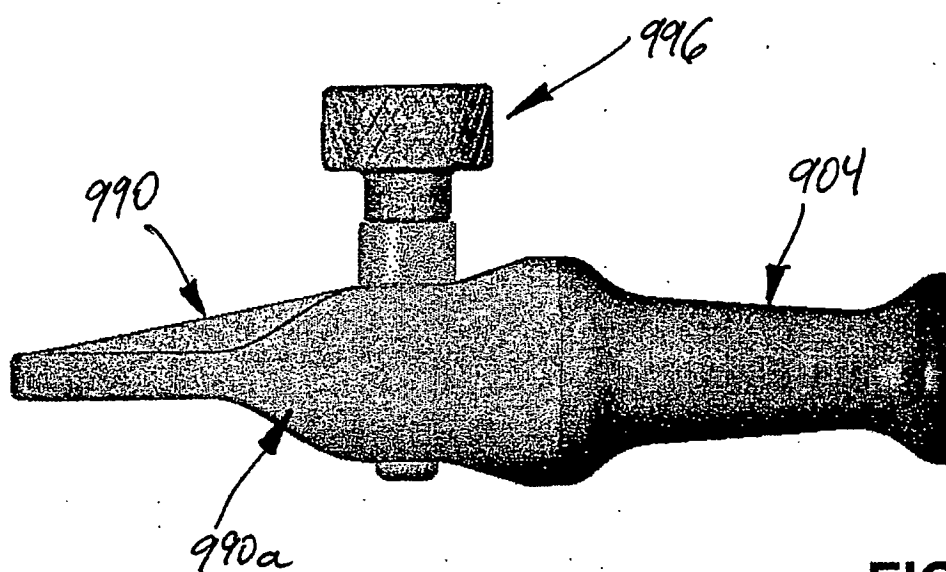


FIG. 3XX

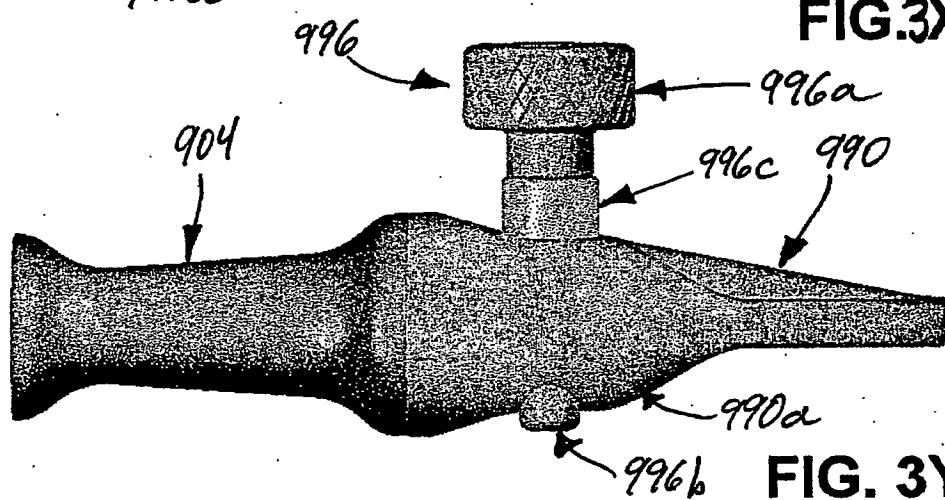


FIG. 3YY

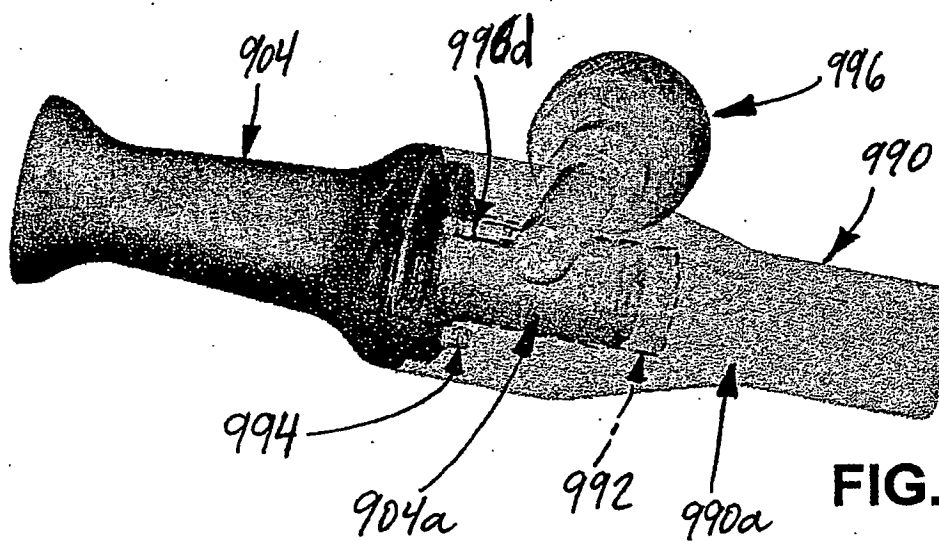


FIG. 3ZZ

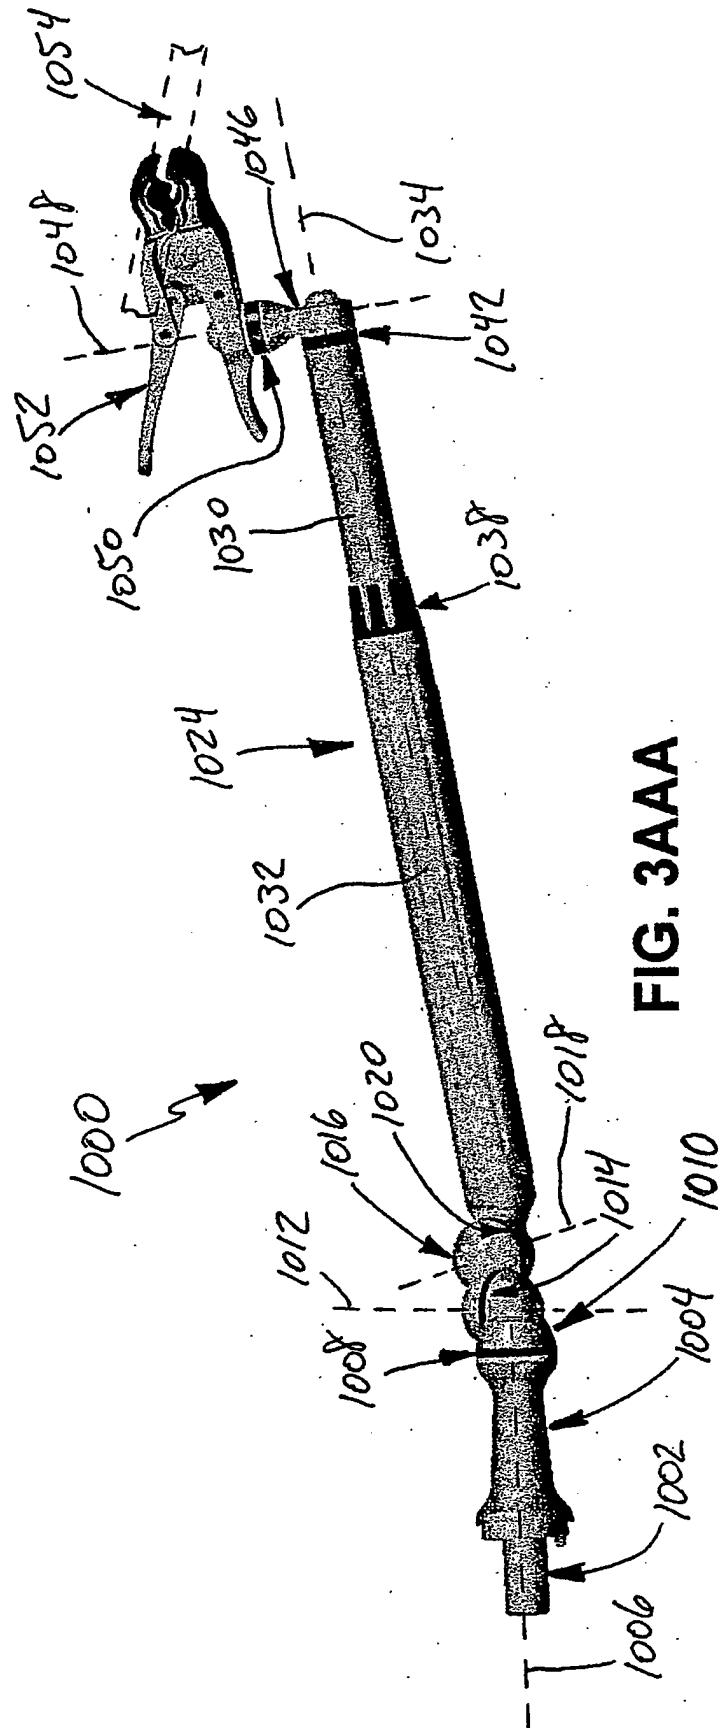


FIG. 3AAA

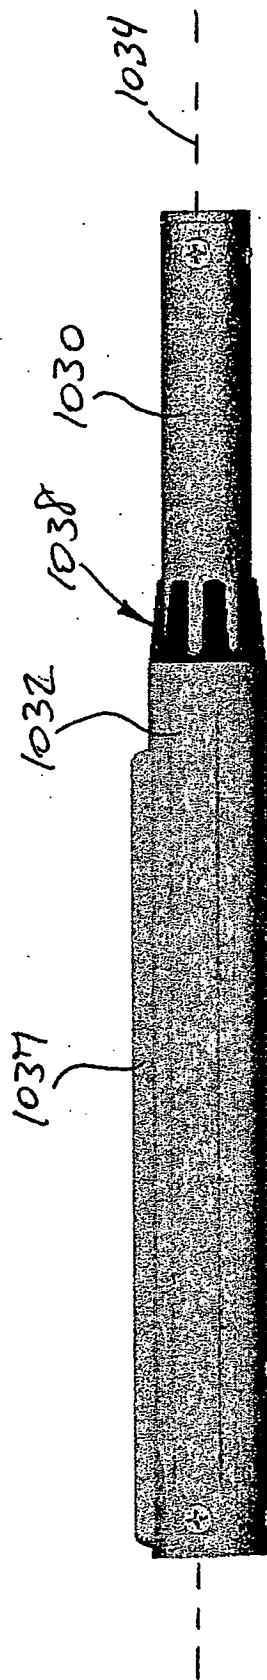


FIG. 3BBB

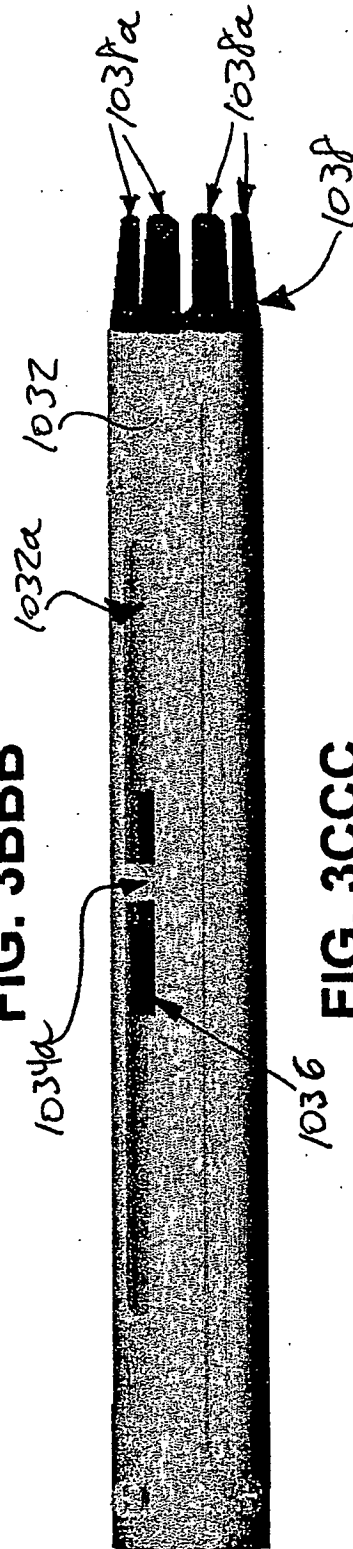


FIG. 3CCC

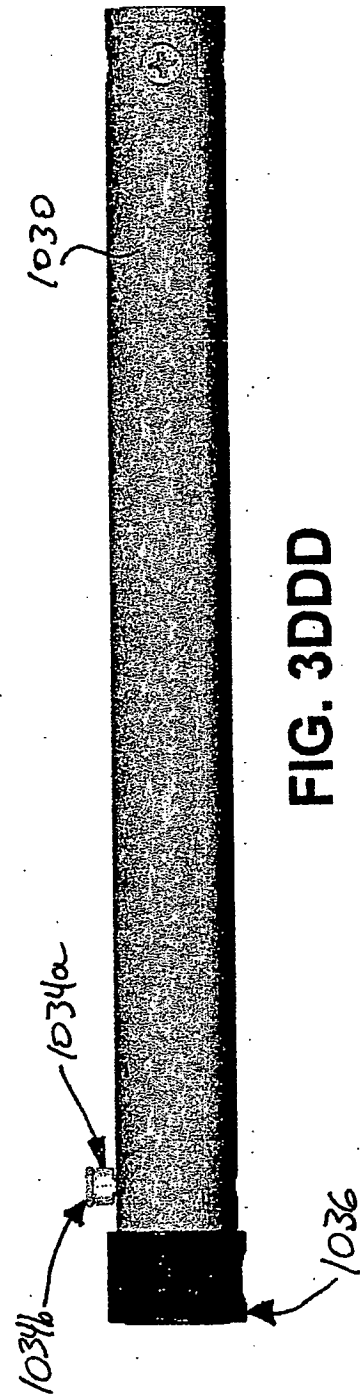
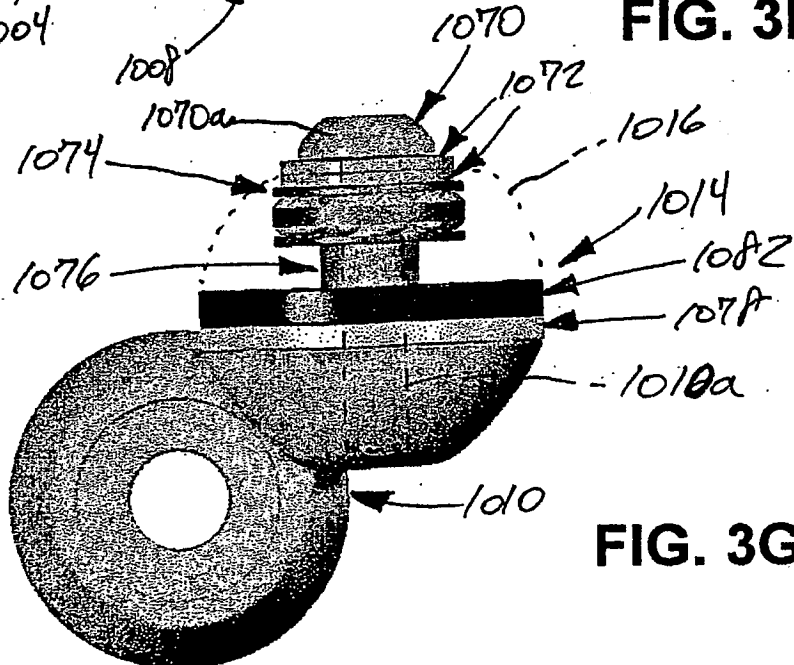
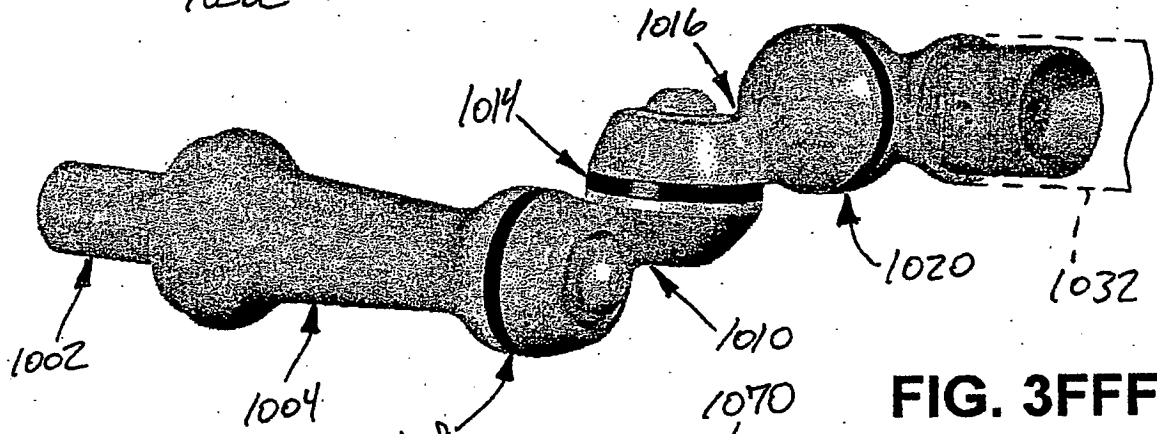
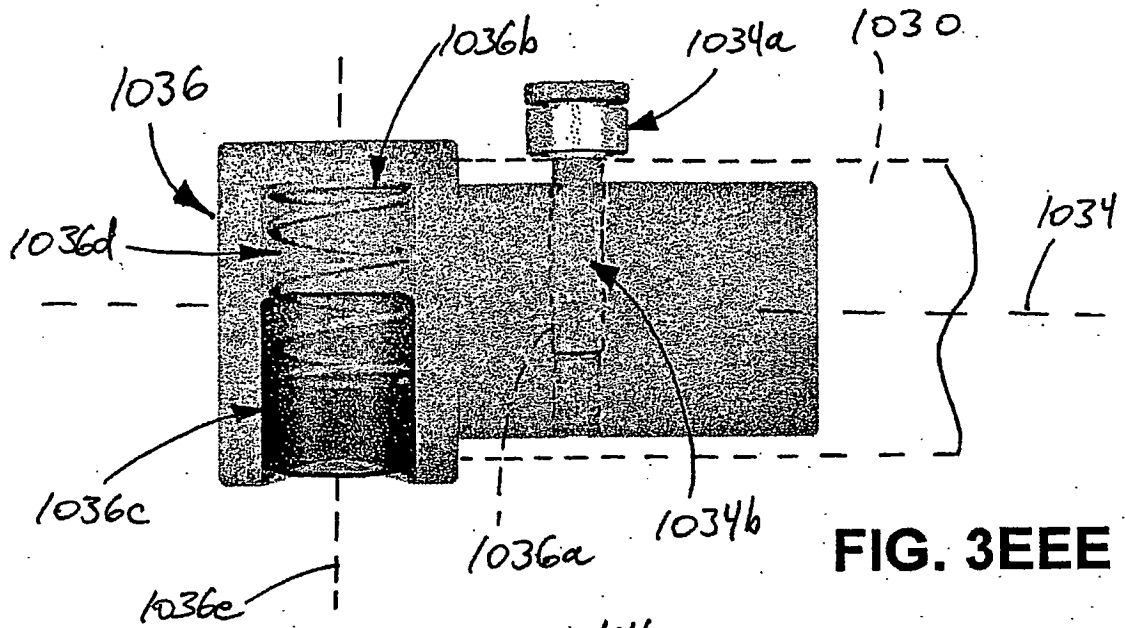


FIG. 3DDD



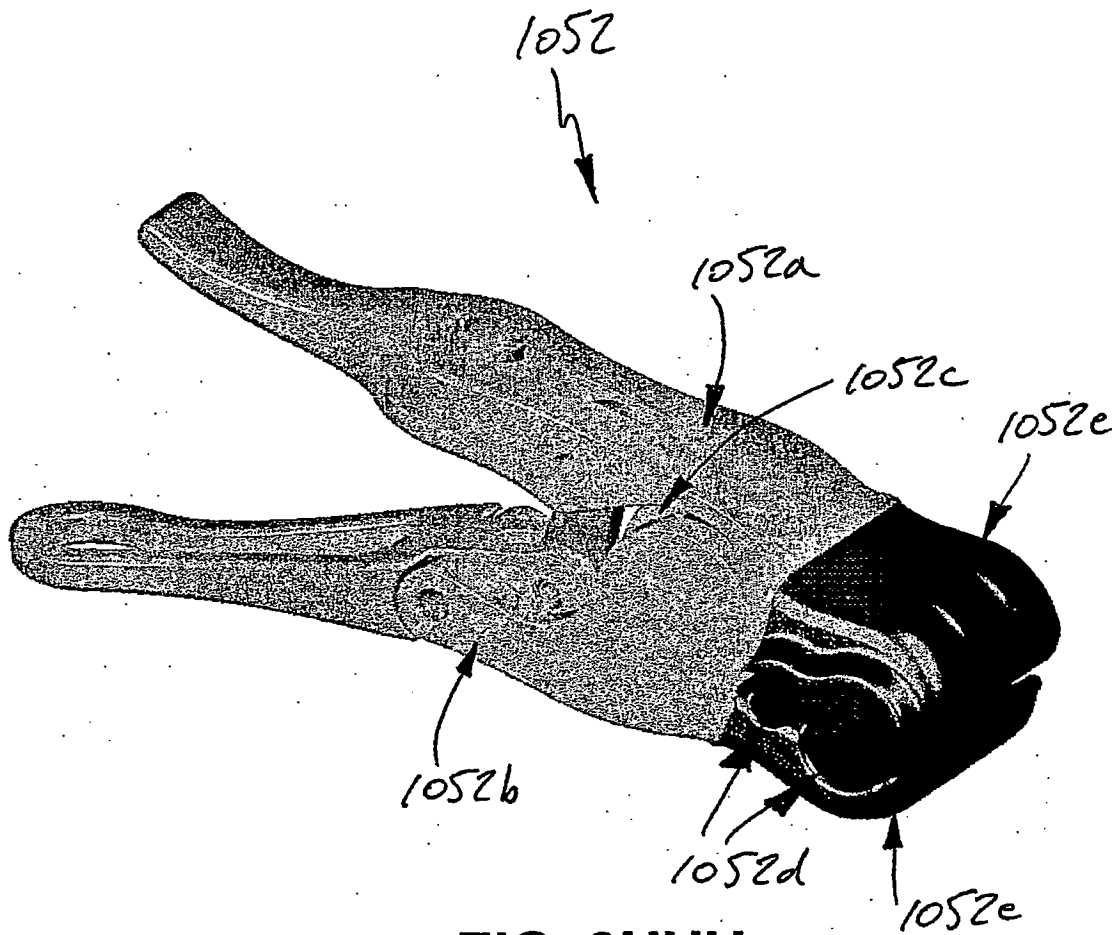


FIG. 3HHH

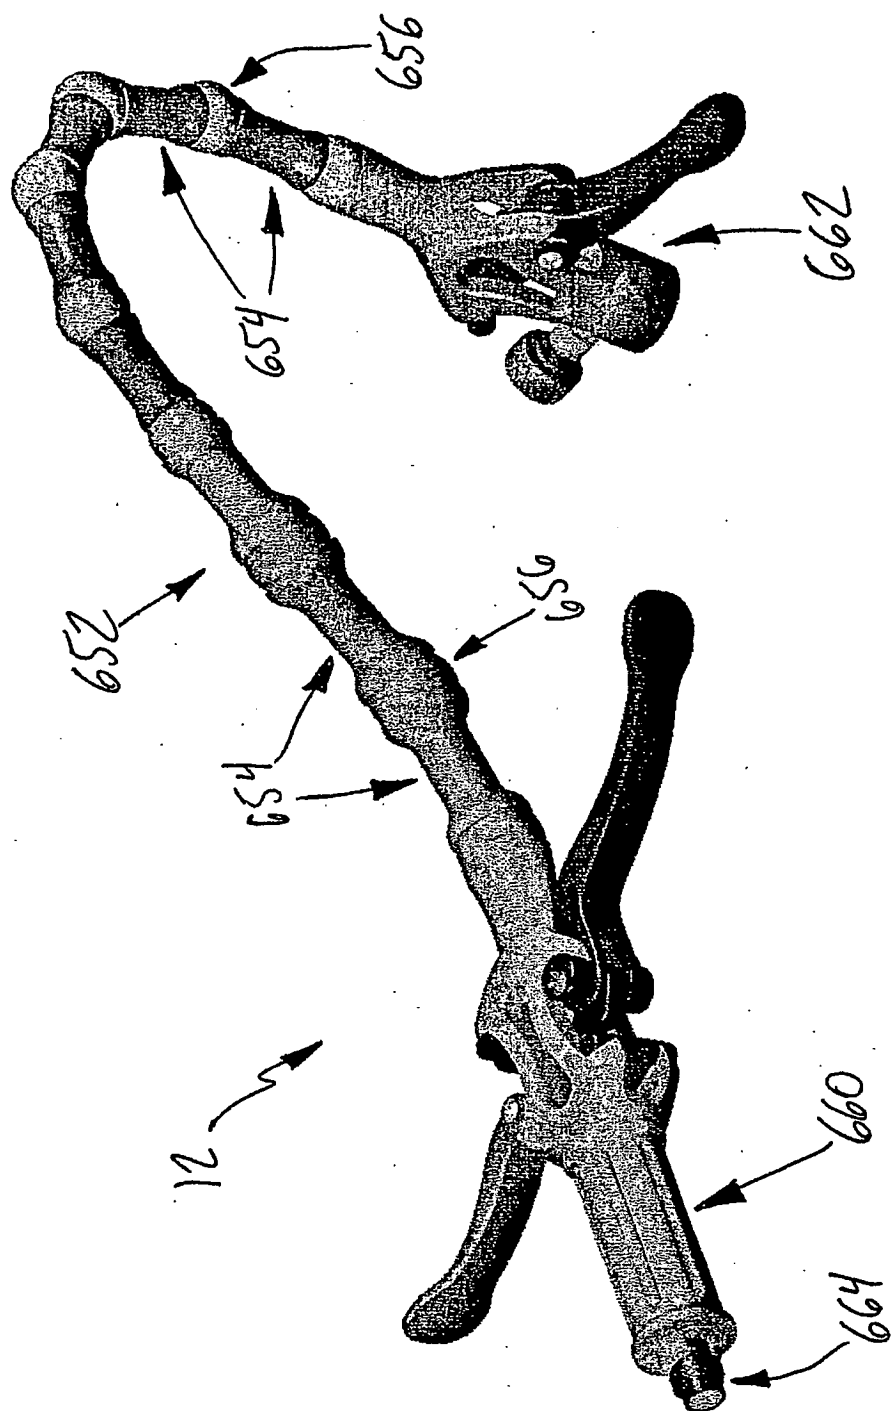


FIG. 4A

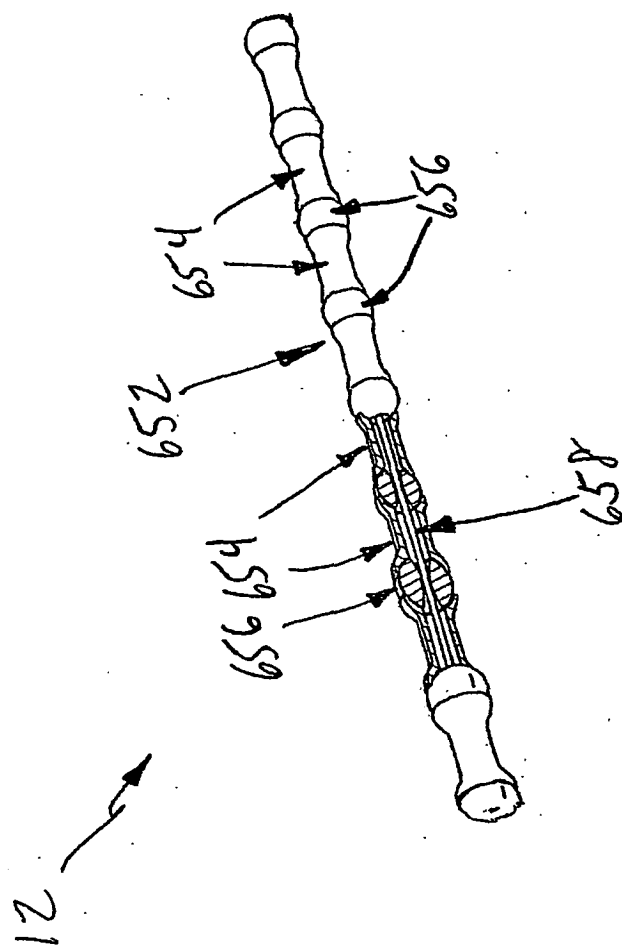


FIG. 4B

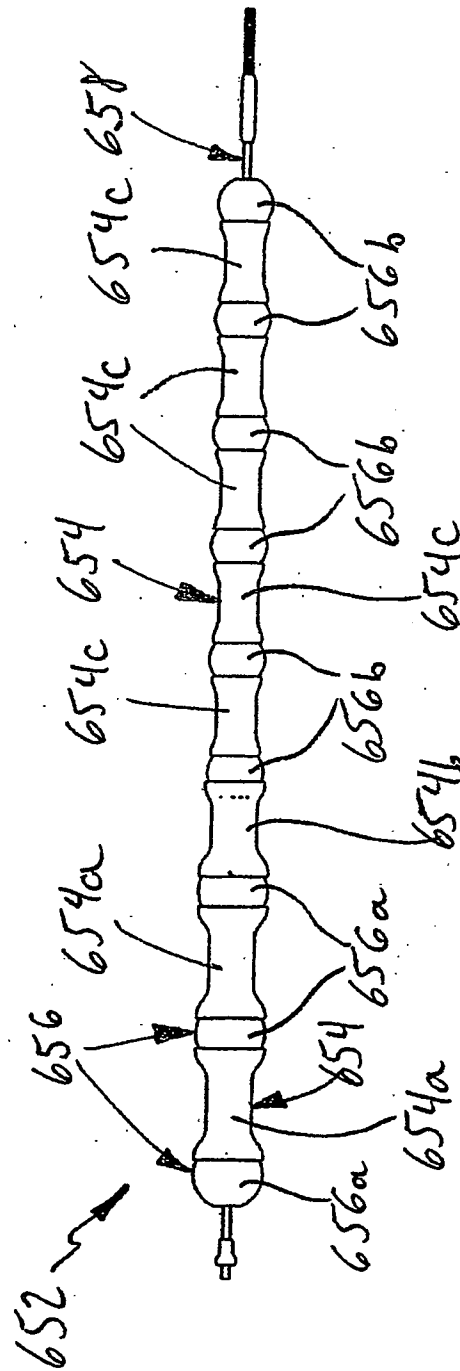


FIG. 4C

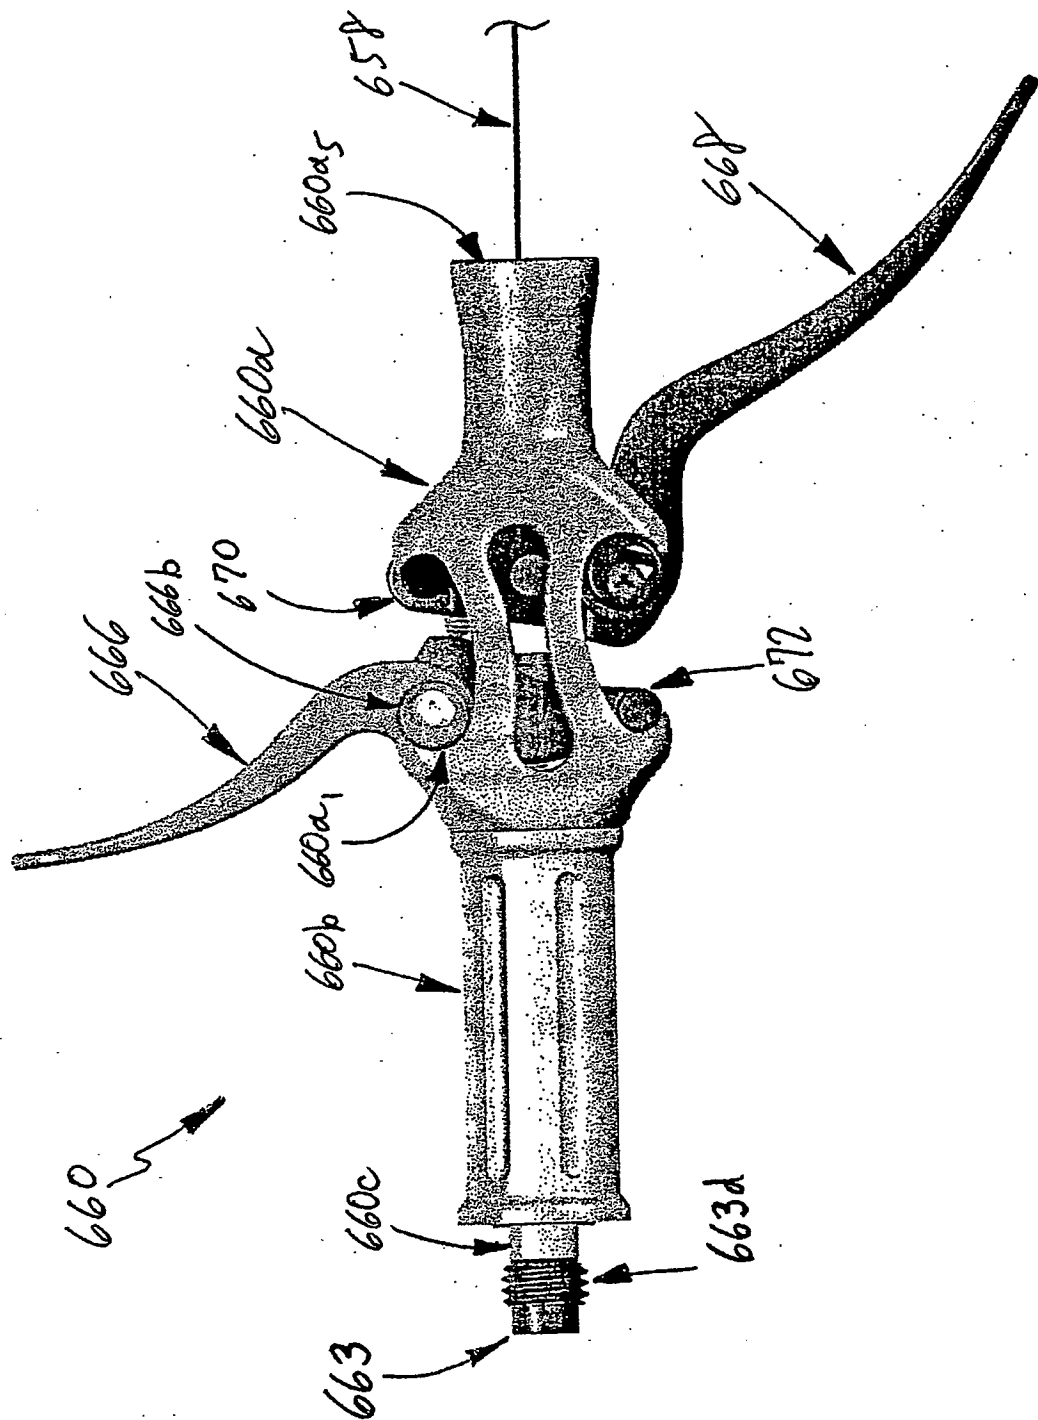


FIG. 4D

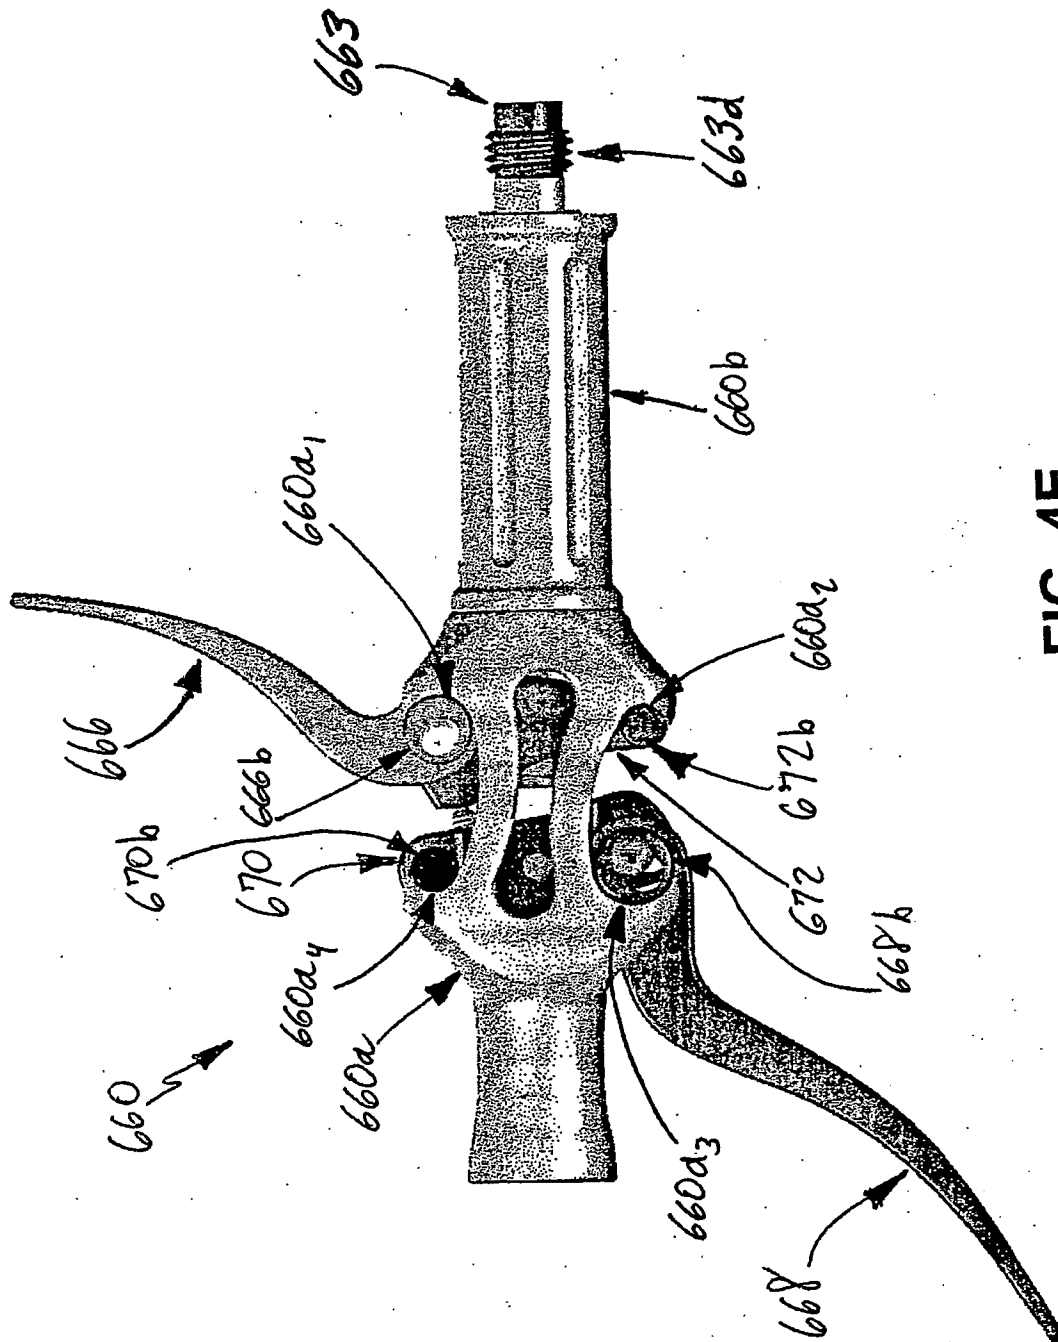


FIG. 4E

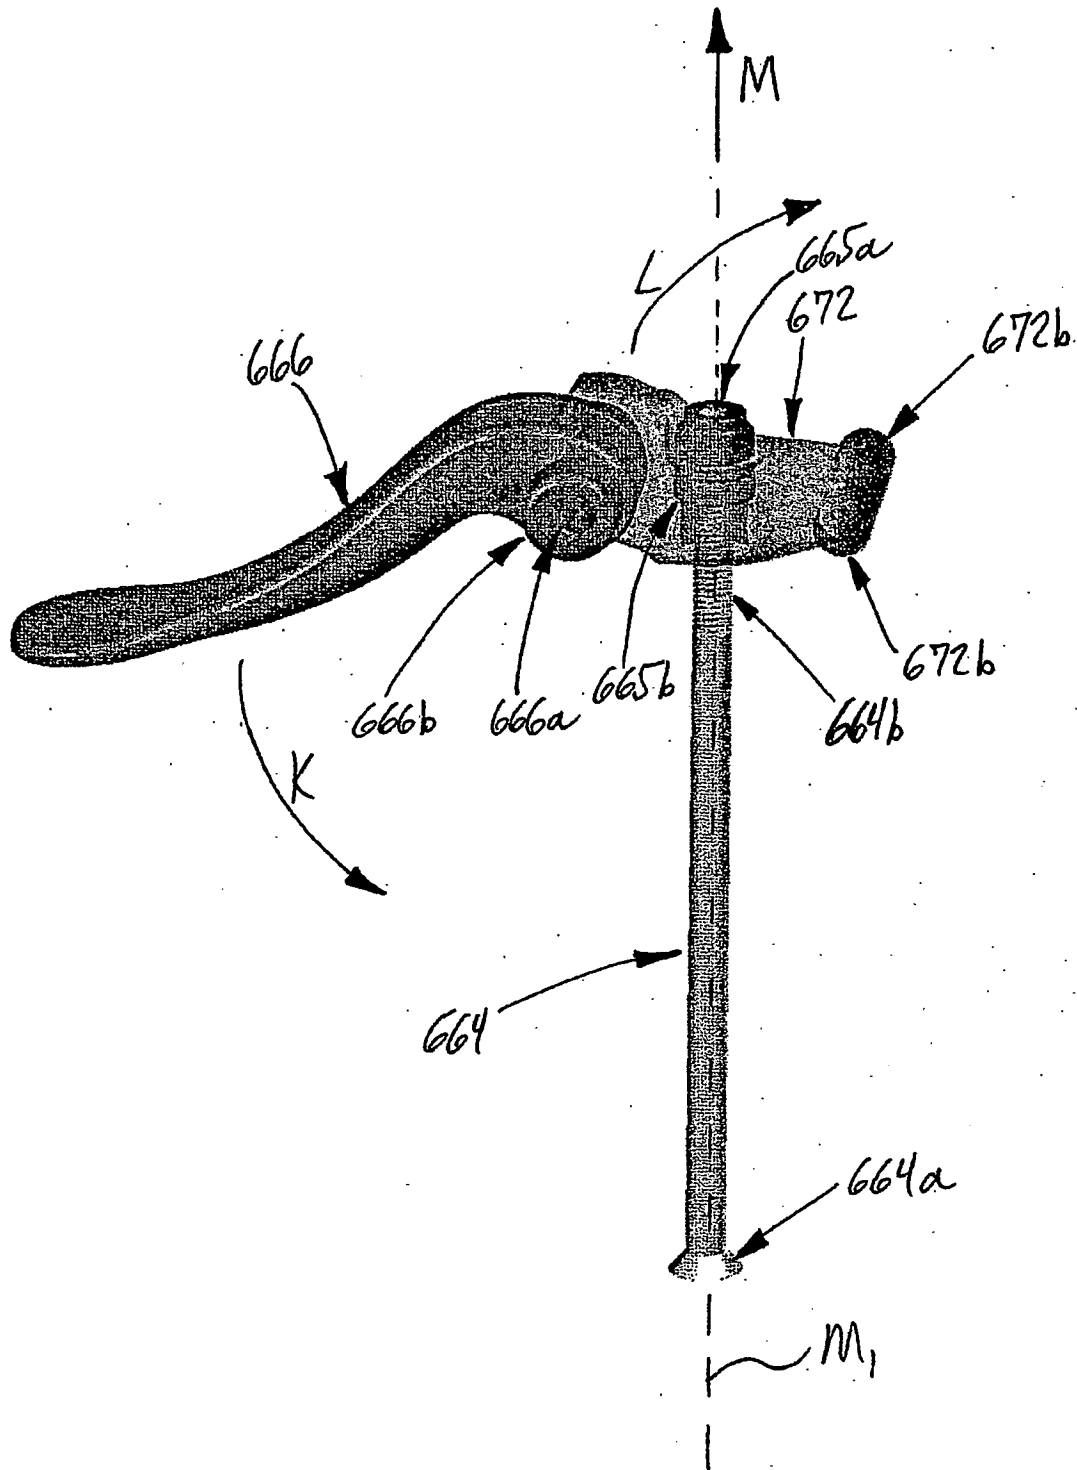


FIG. 4F

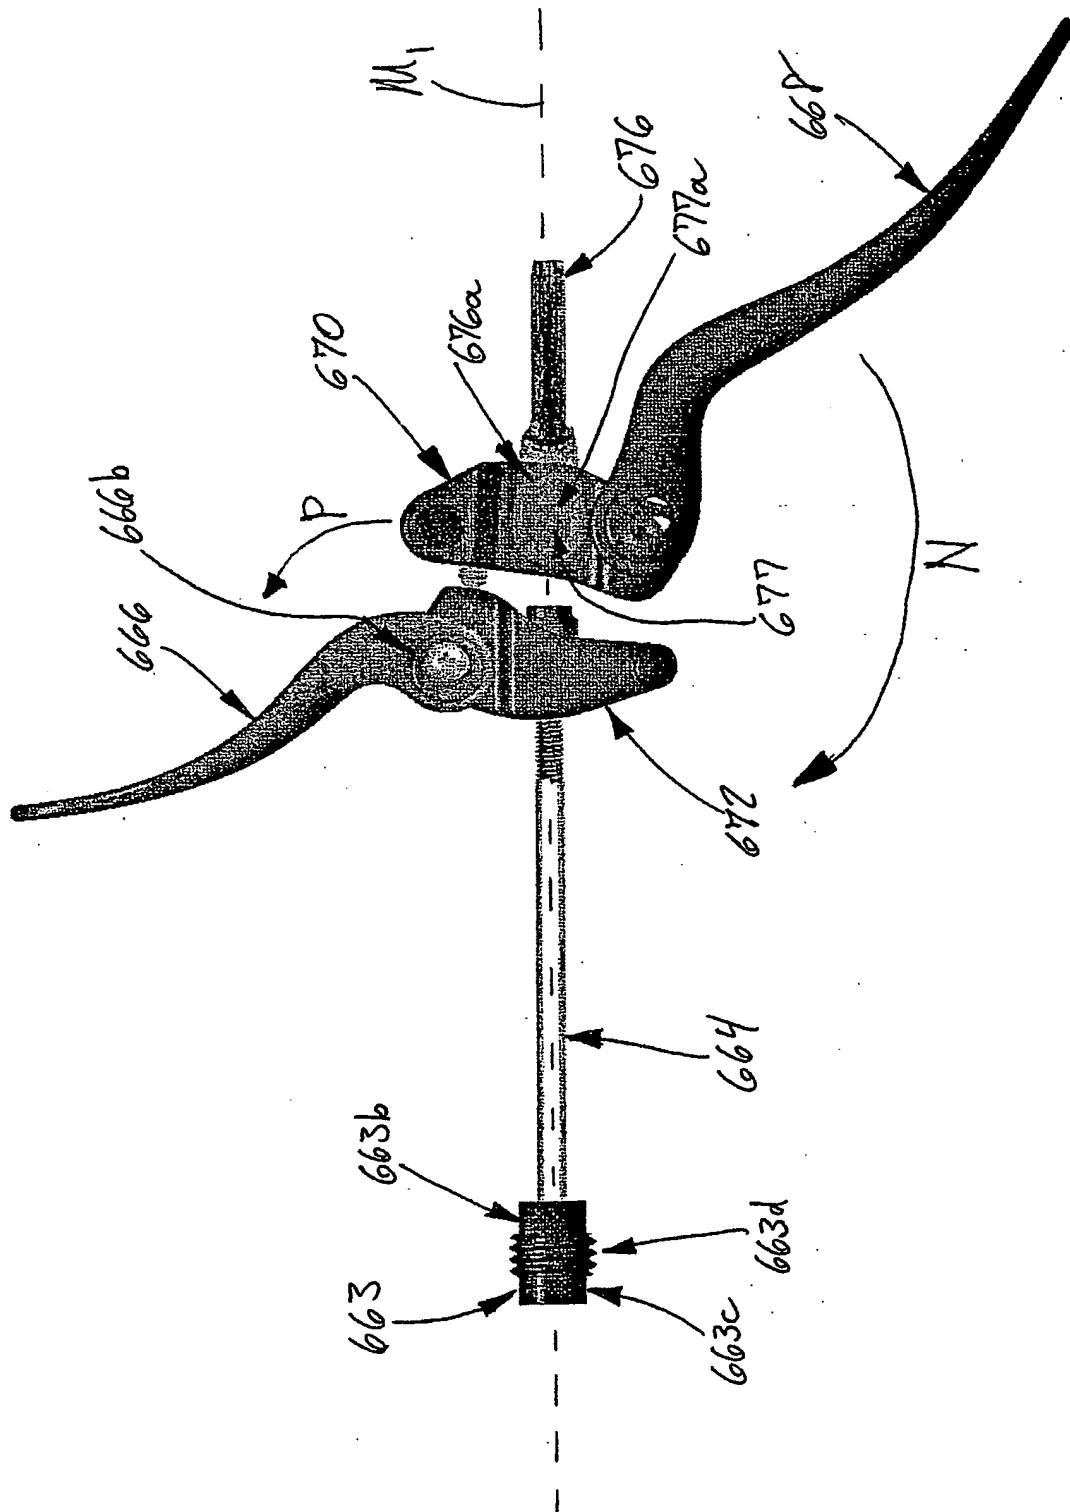


FIG. 4G

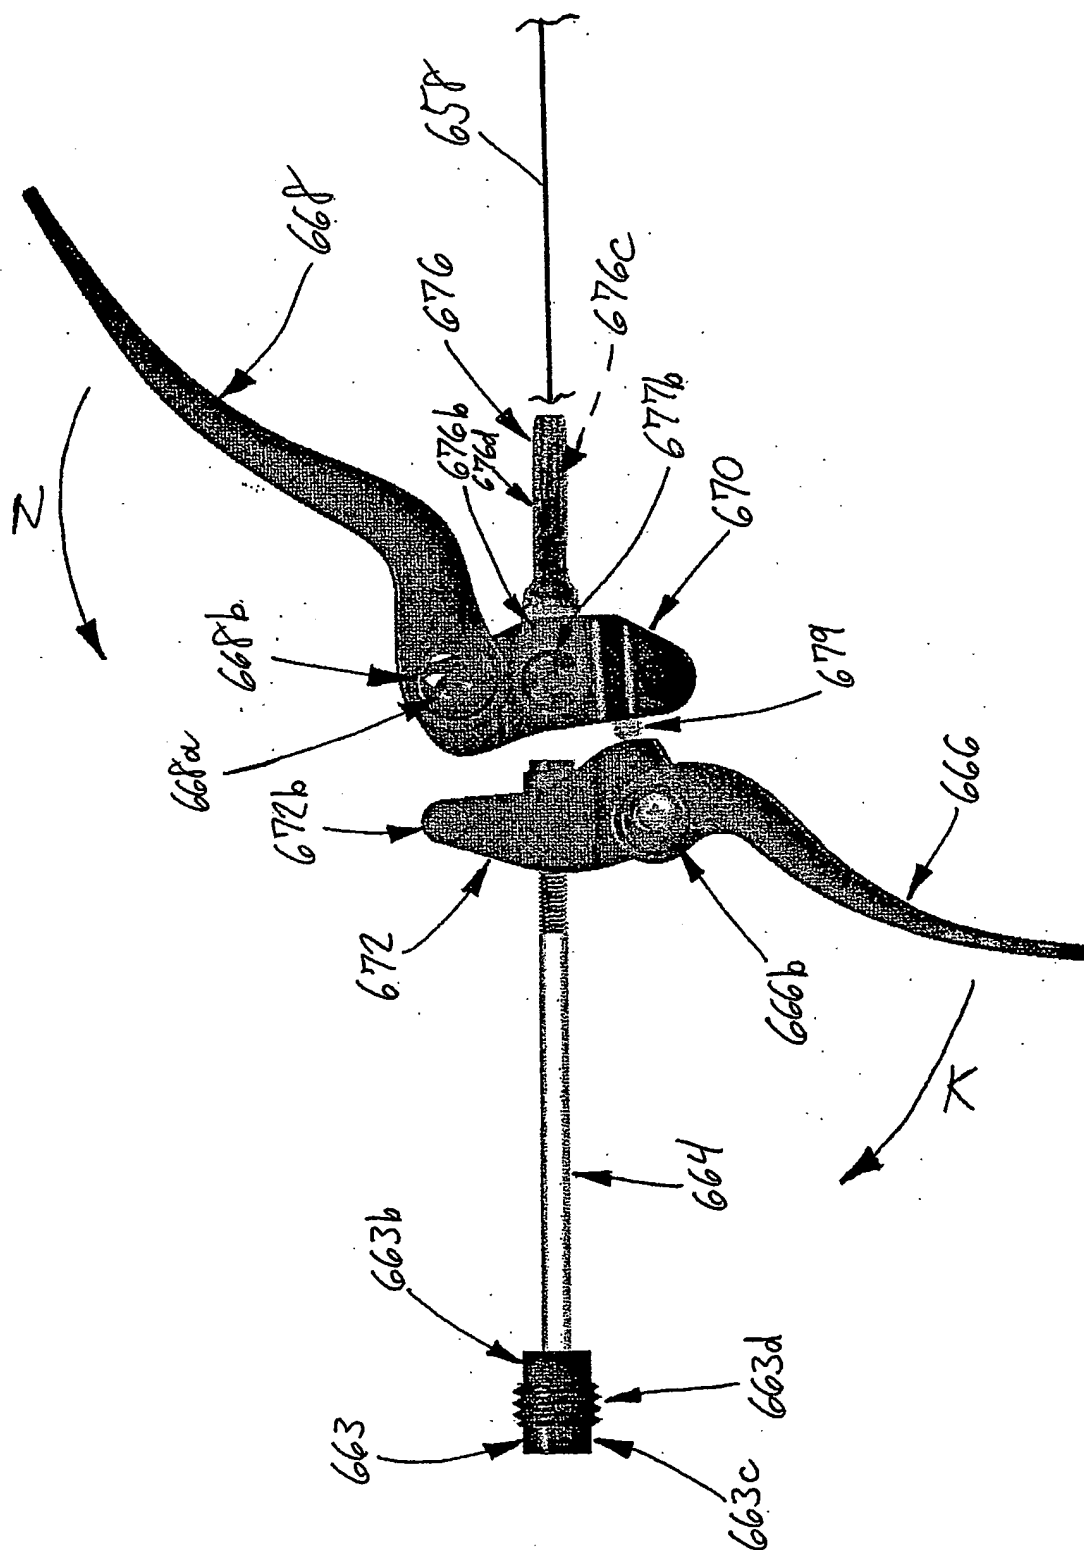


FIG. 4H

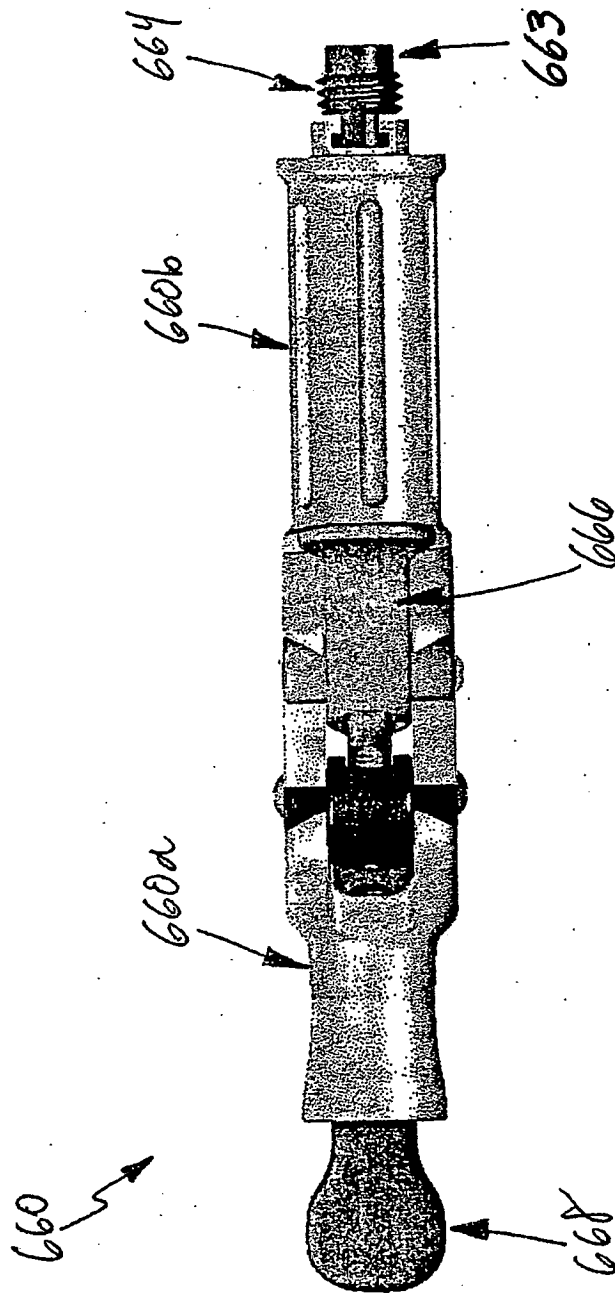


FIG. 41

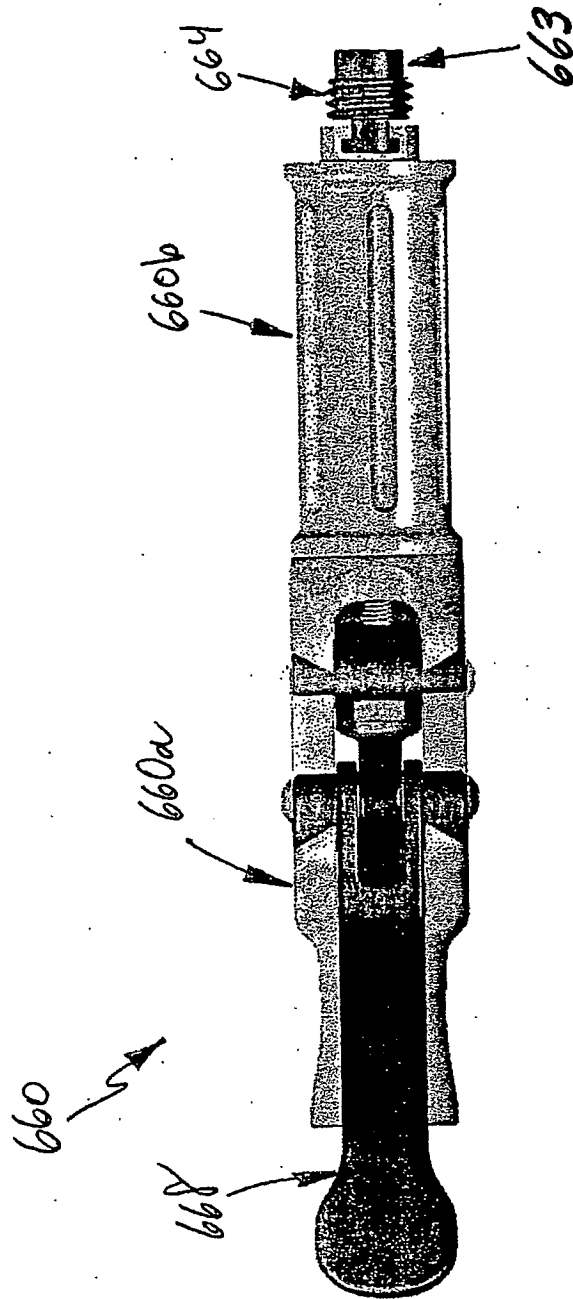


FIG. 4J

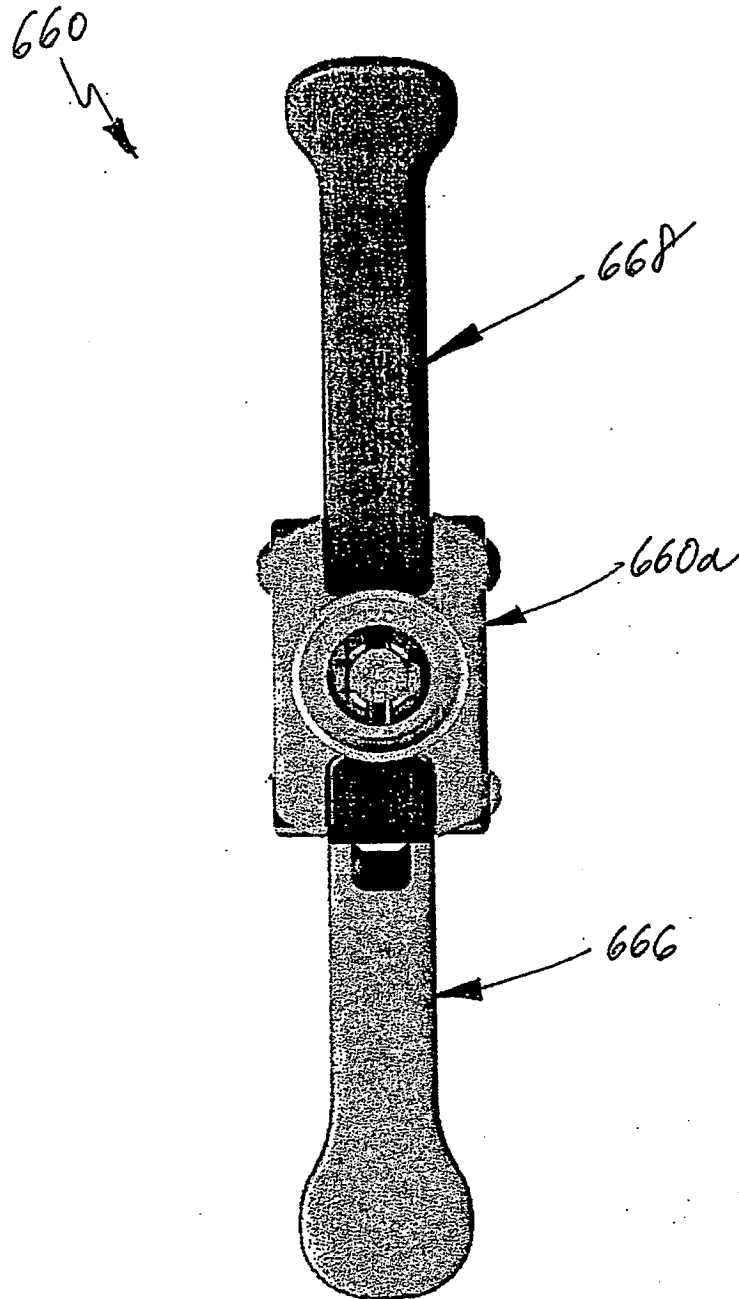


FIG. 4K

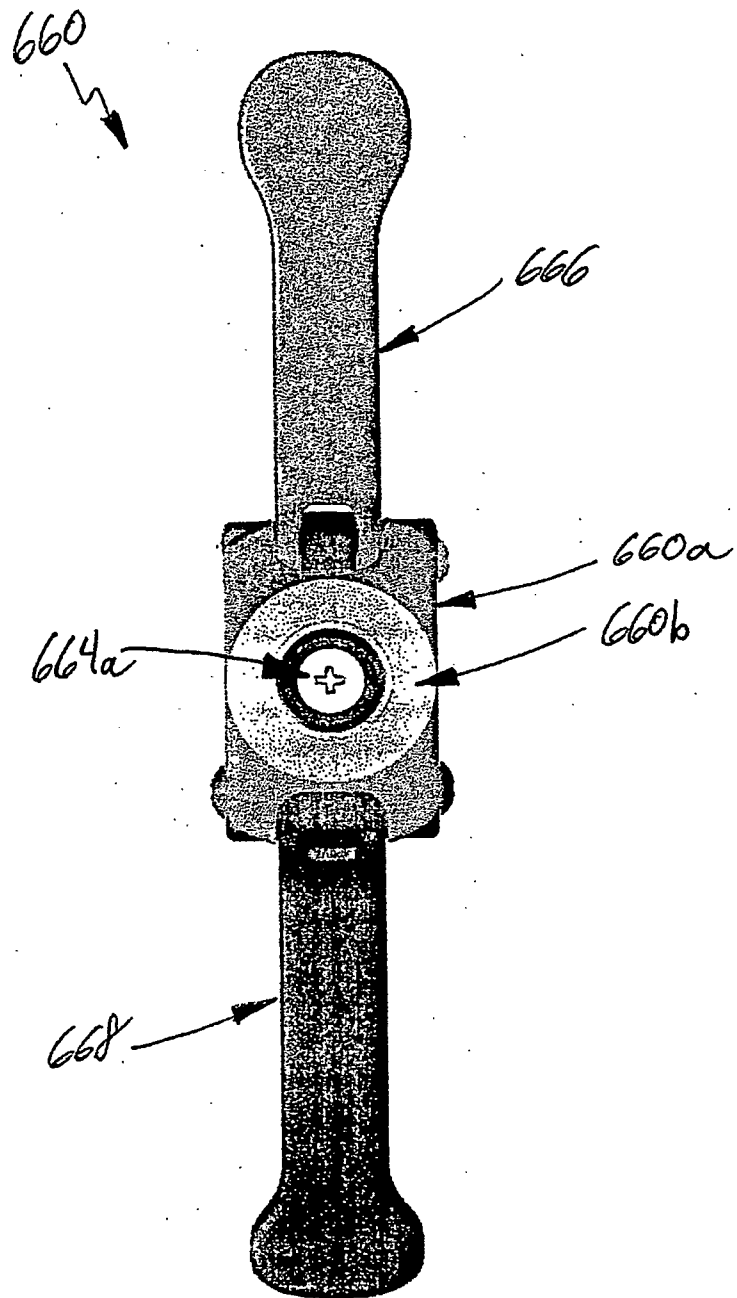


FIG. 4L

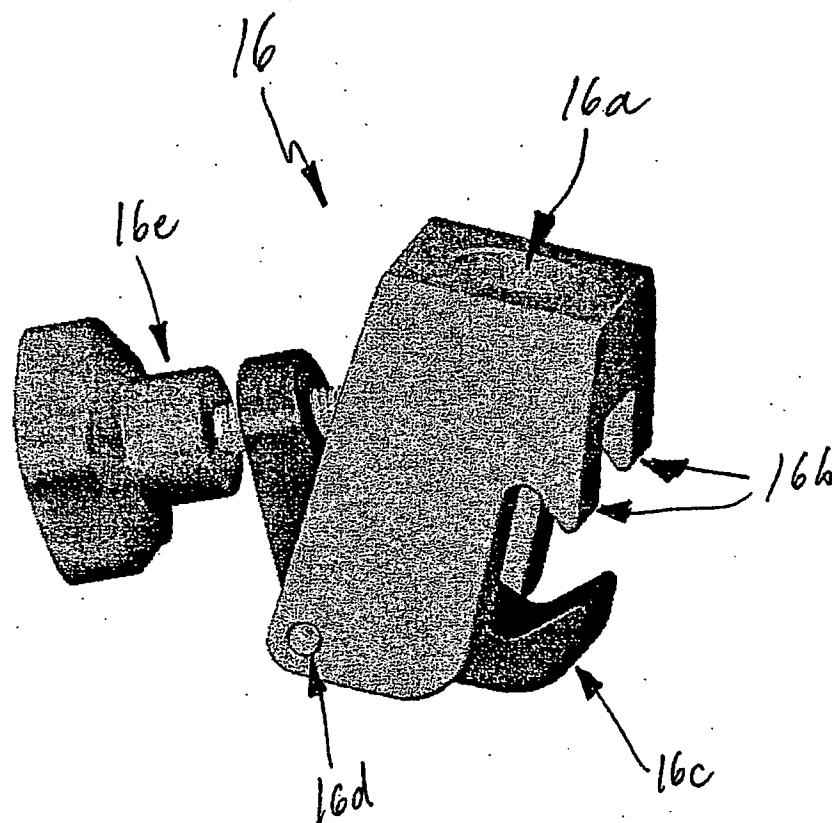


FIG. 4M

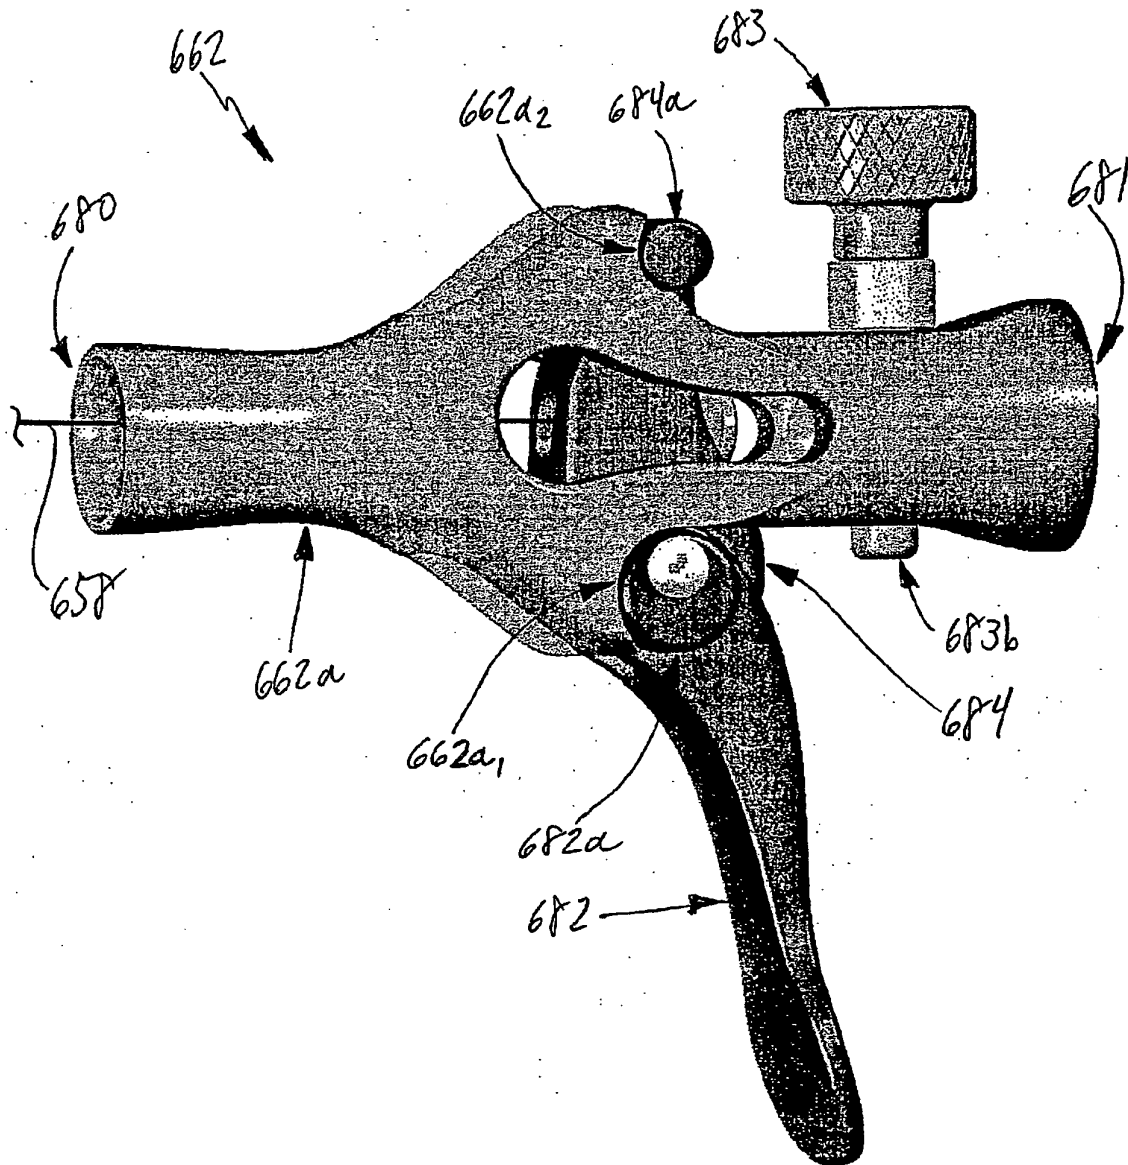


FIG. 4N

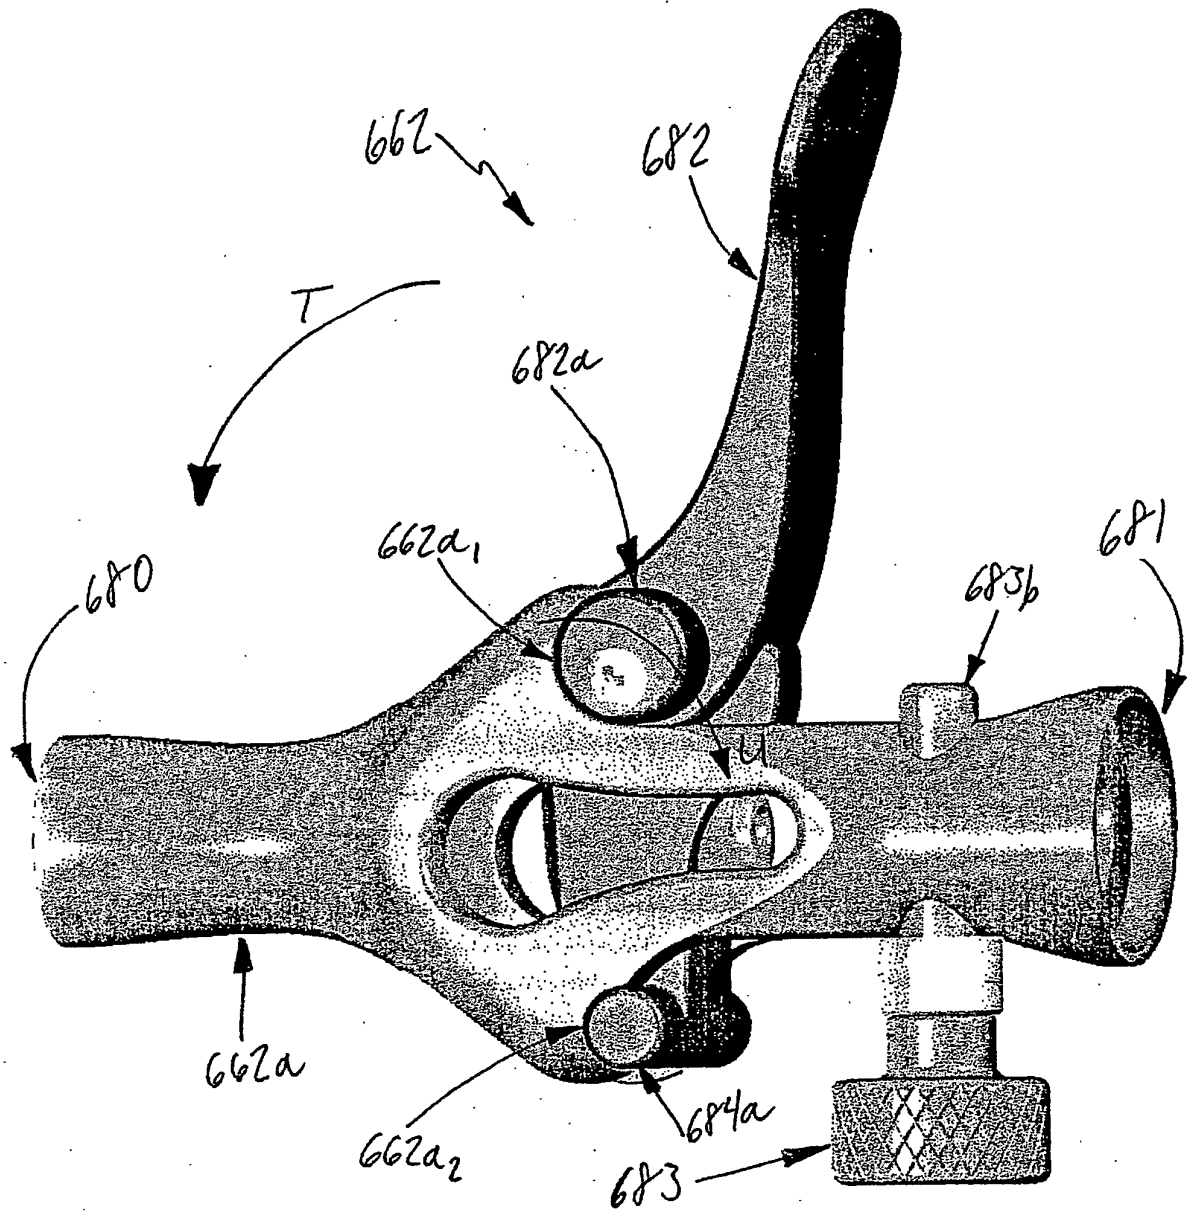


FIG. 4-O

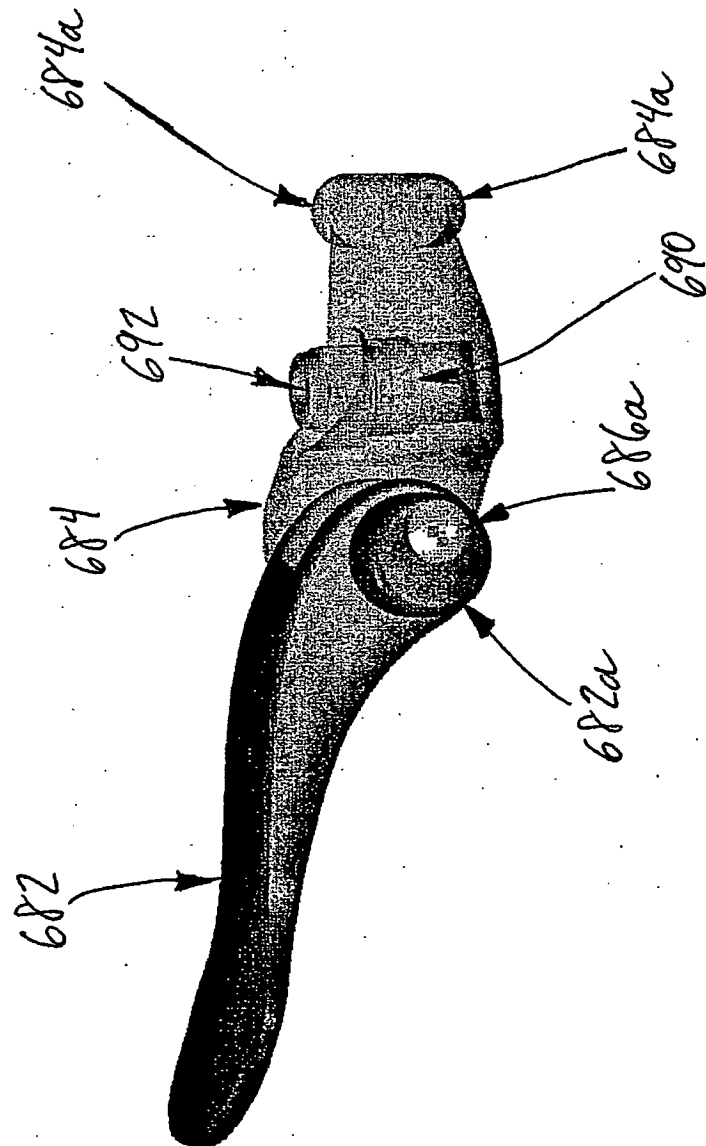


FIG. 4P

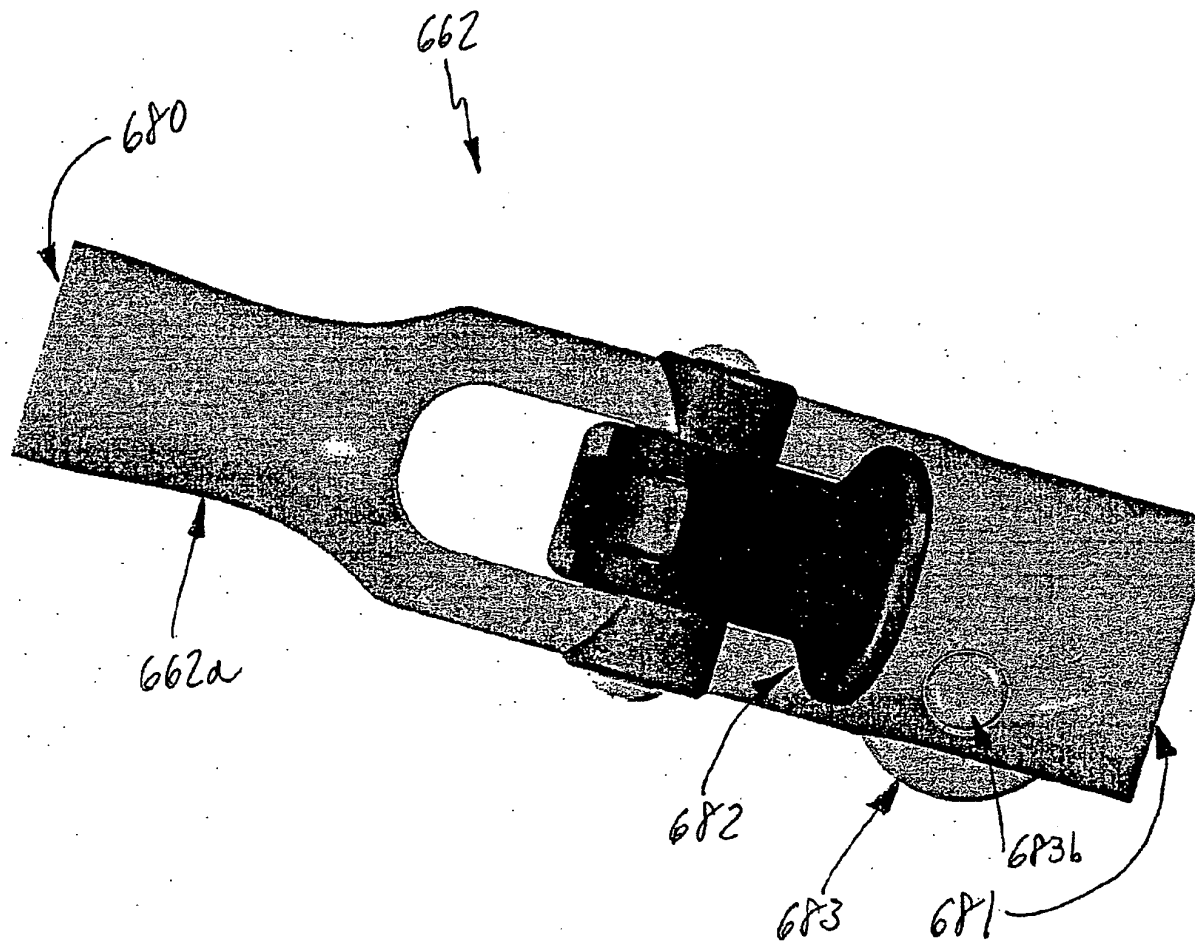


FIG. 4Q

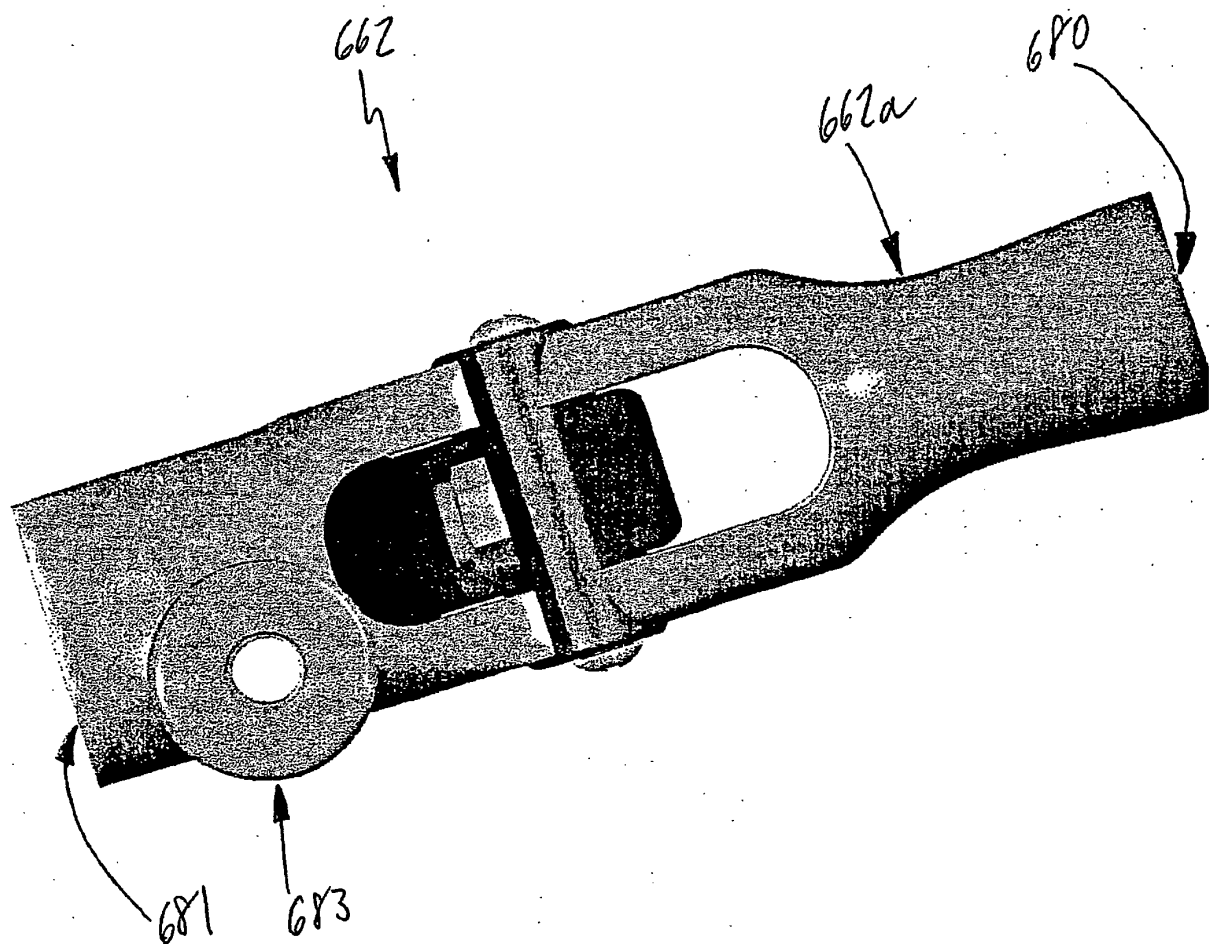


FIG. 4R

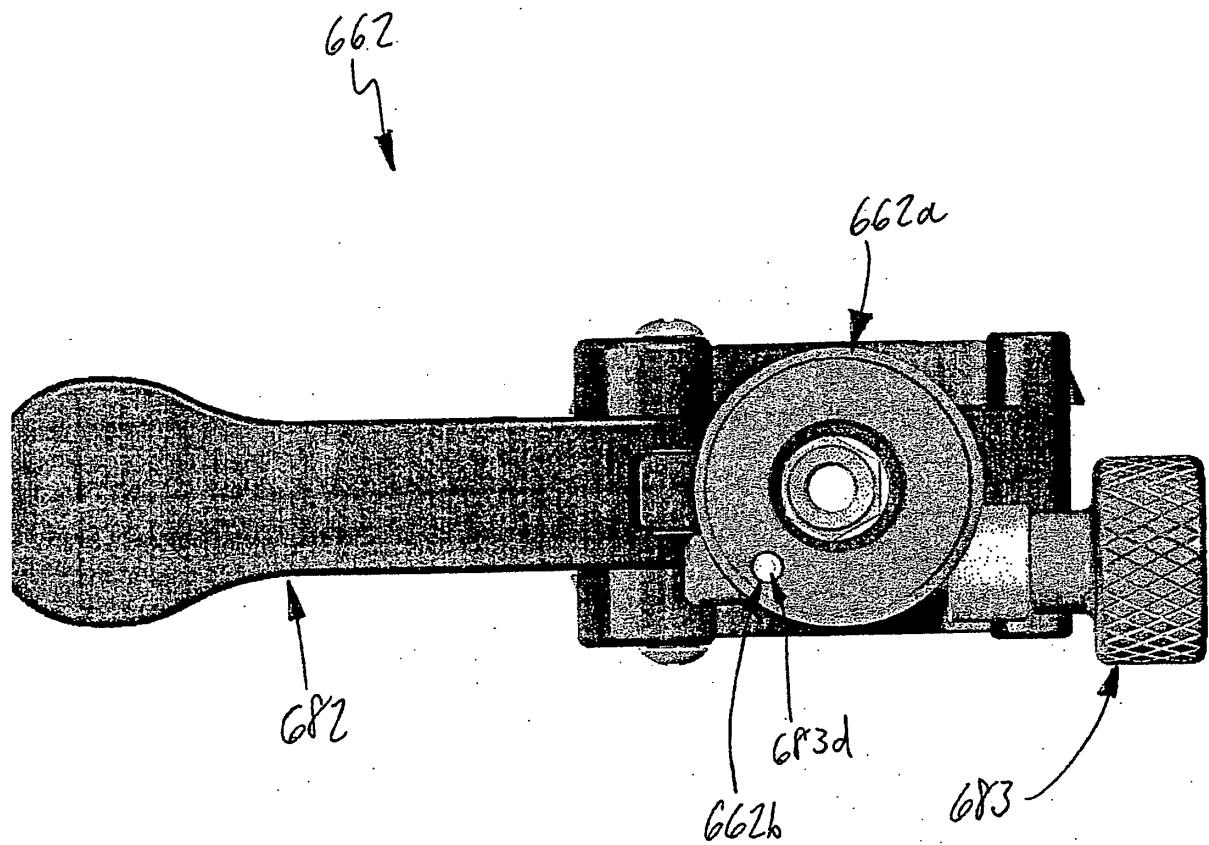


FIG. 4S

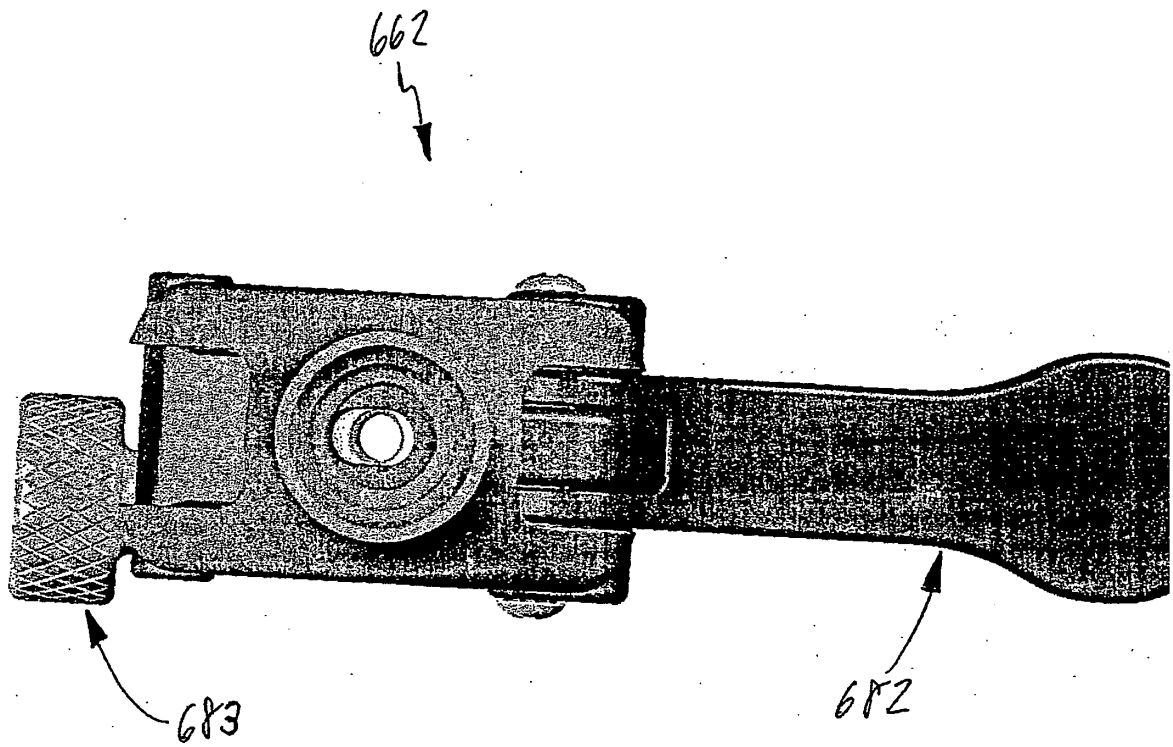


FIG. 4T

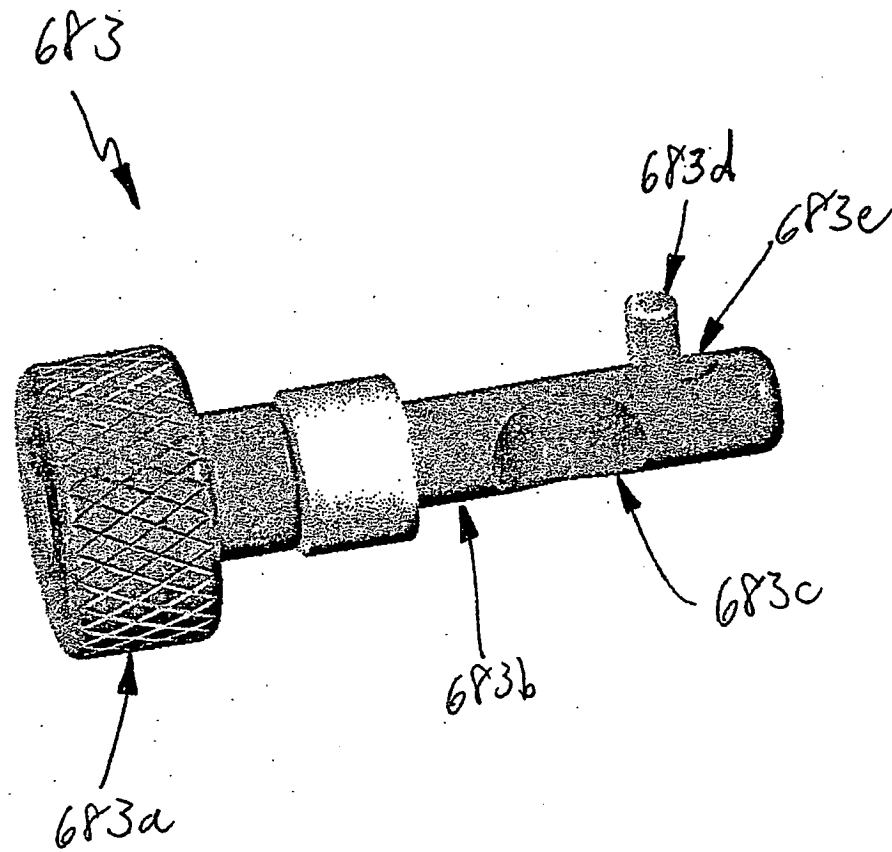


FIG. 4U


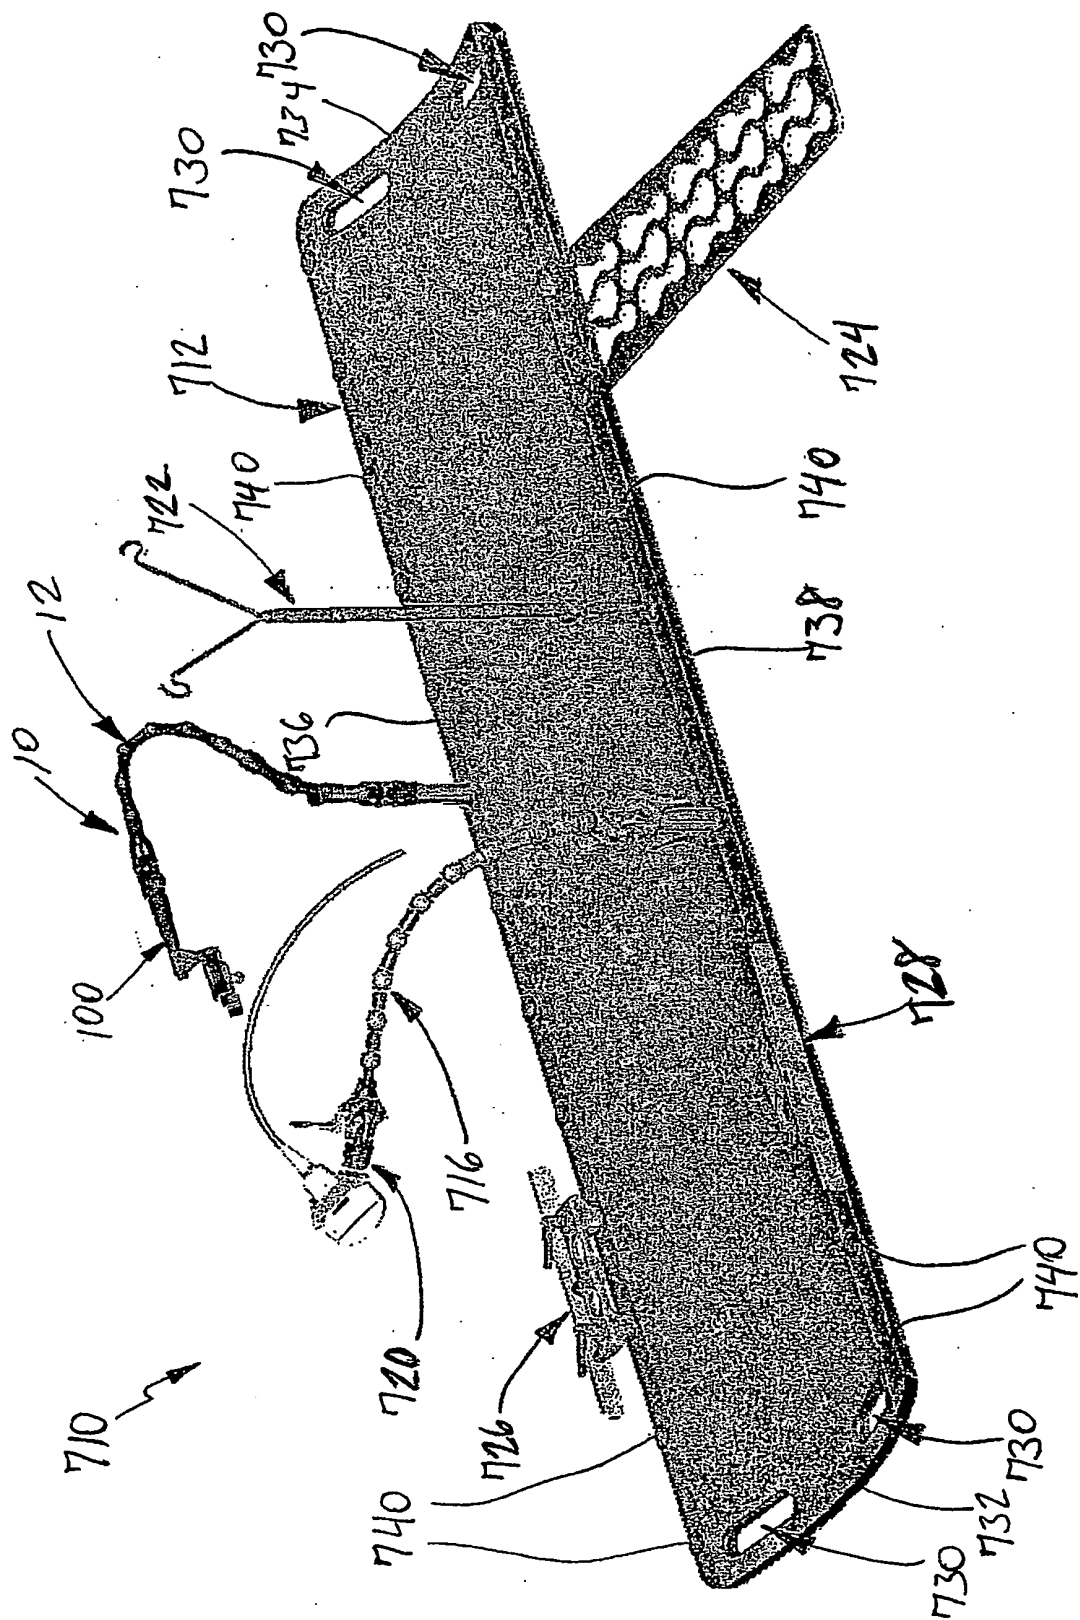


FIG. 5

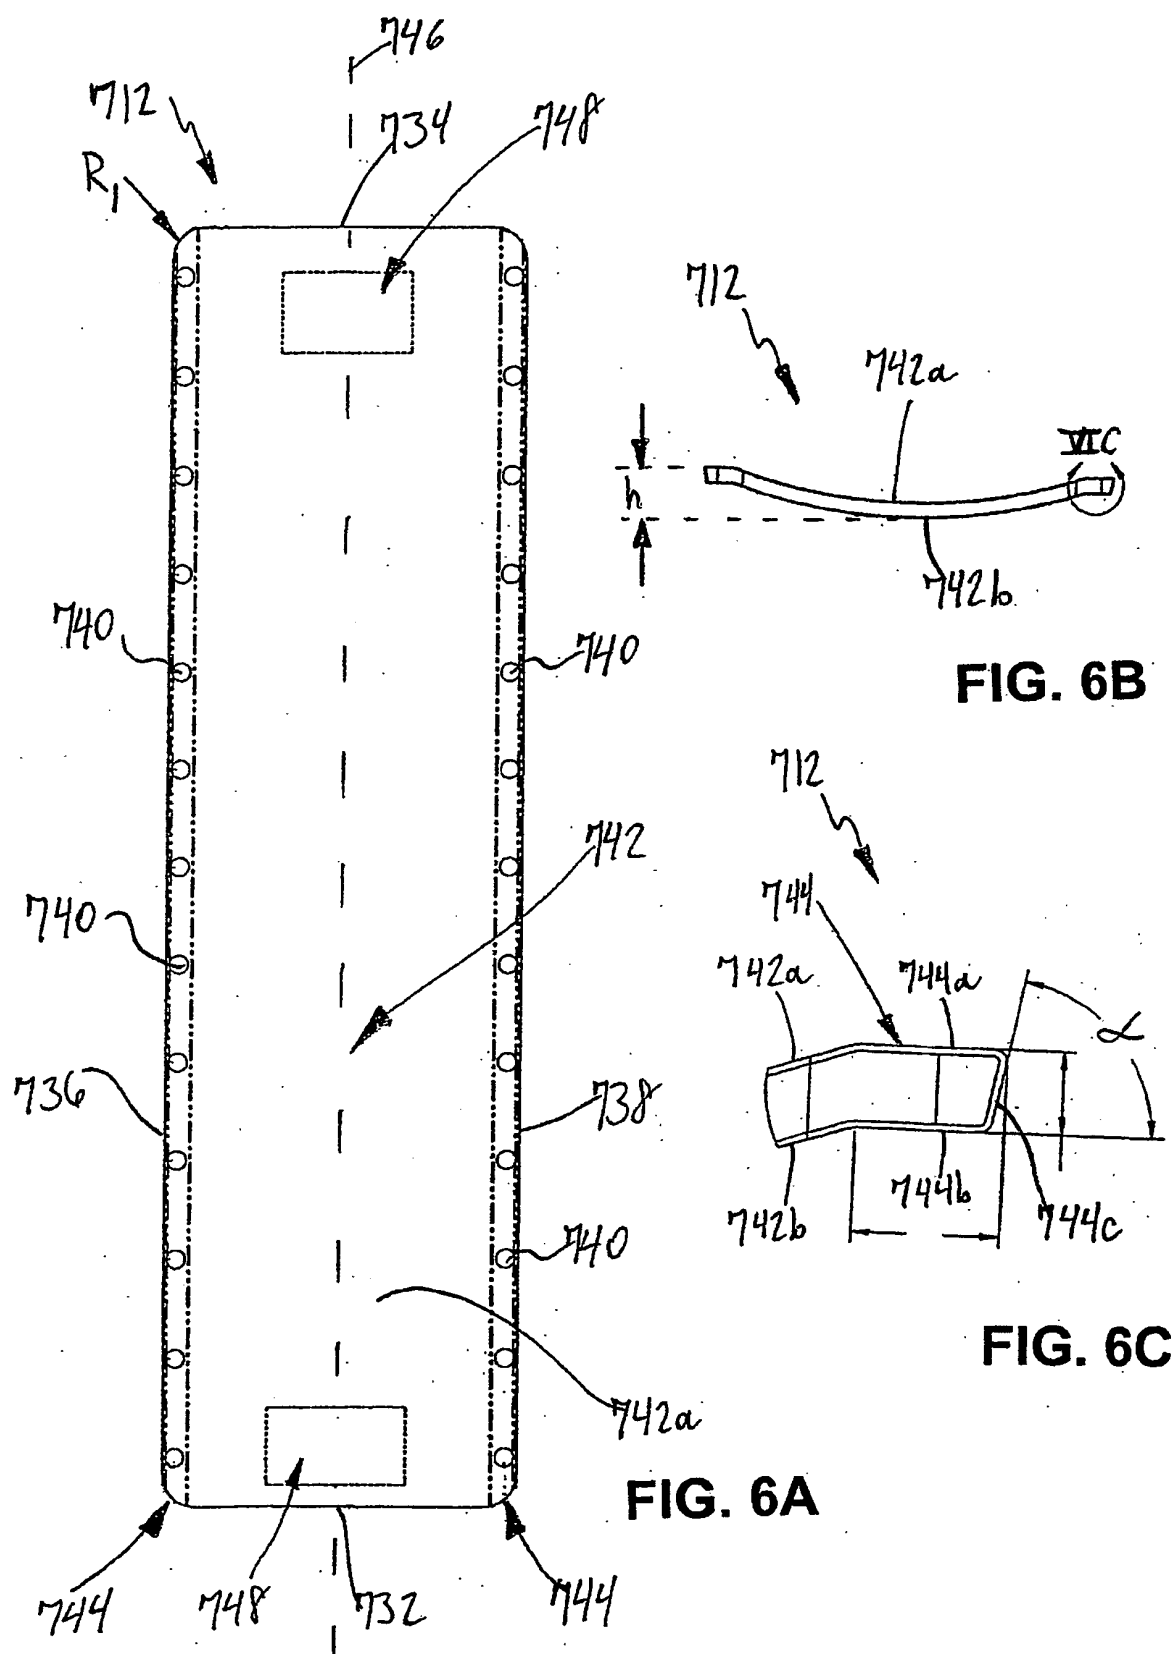

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 5571072 A [0008]
- US 3858578 A, Milo [0130]

专利名称(译)	用于定位腹腔镜装置的系统		
公开(公告)号	EP1942810B1	公开(公告)日	2012-08-08
申请号	EP2006813458	申请日	2006-08-16
申请(专利权)人(译)	CIVCO医疗器械CO. , INC.		
当前申请(专利权)人(译)	CIVCO医疗器械CO. , INC.		
[标]发明人	WILSON ROGER F WHITMORE III WILLET F		
发明人	WILSON, ROGER, F. WHITMORE III, WILLET, F.		
IPC分类号	A61B19/00 A61B17/02		
CPC分类号	A61B17/02 A61B90/50 A61B90/57 A61B2017/00858 A61B2017/00862 A61B2017/00991 A61B2090/571		
代理机构(译)	莫兰 , DAVID		
优先权	60/709098 2005-08-18 US 60/772863 2006-02-14 US 60/773638 2006-02-16 US 60/821692 2006-08-07 US 60/730853 2005-10-28 US 11/464804 2006-08-15 US		
其他公开文献	EP1942810A2 EP1942810A4		
外部链接	Espacenet		

摘要(译)

用于定位腹腔镜装置的系统包括曲线关节臂和支架。保持器具有至少两个旋转区域和用于接收腹腔镜装置的夹持部分，并且保持器联接到曲线关节臂。允许至少两个旋转区域进行关节运动。另外，将腹腔镜装置定位在哺乳动物的皮肤端口中的方法包括：将腹腔镜装置固定到具有至少两个旋转关节的支架上；将支架连接到曲线铰接臂；将腹腔镜装置部分地设置在皮肤端口内；通过选择性地铰接曲线关节臂并选择性地使支架的部分相对于彼此旋转来定位腹腔镜装置。

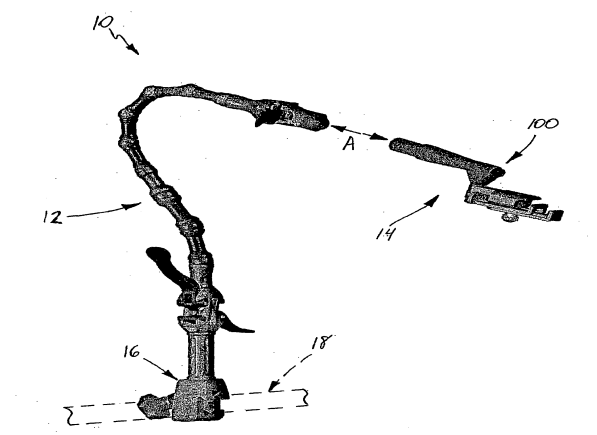


FIG. 1