

(19)



(11)

EP 2 043 499 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention of the grant of the patent:
21.10.2015 Bulletin 2015/43

(51) Int Cl.:
A61B 1/04 (2006.01)

(21) Application number: **07784896.8**

(86) International application number:
PCT/BE2007/000079

(22) Date of filing: **09.07.2007**

(87) International publication number:
WO 2008/006180 (17.01.2008 Gazette 2008/03)

(54) ENDOSCOPIC VISION SYSTEM

ENDOSKOPISCHES VISIONSSYSTEM
SYSTÈME DE VISION ENDOSCOPIQUE

(84) Designated Contracting States:
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IS IT LI LT LU LV MC MT NL PL PT RO SE SI SK TR

- **KONINCKX, Thomas**
3000 Leuven (BE)
- **VAN GOOL, Luc**
2170 Antwerpen (BE)

(30) Priority: **10.07.2006 GB 0613576**

(74) Representative: **Wauters, Davy Erik Angelo**
DenK iP bvba
Leuvensesteenweg 203
3190 Boortmeerbeek (BE)

(43) Date of publication of application:
08.04.2009 Bulletin 2009/15

(73) Proprietor: **Katholieke Universiteit Leuven**
3000 Leuven (BE)

(56) References cited:
WO-A-2005/039391 **WO-A-2005/084525**
US-A- 5 653 677 **US-A1- 2002 007 110**
US-A1- 2005 014 994 **US-A1- 2005 234 294**

(72) Inventors:
• **KONINCKX, Philippe**
3360 Bierbeek (BE)

EP 2 043 499 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

Background and Summary

BACKGROUND OF THE INVENTION

A. Field of the Invention

[0001] The present invention relates to a novel endoscope or an optical large view endoscopic system with improved depth perception. In particular, a multiple viewpoint endoscope system comprising a multiple viewpoint camera setup and/or an intelligent or cognitive image control system and display device particularly adapted for localising internal structures within a cavity or an enclosing structure, such as an animal body, for instance the abdomen of an animal or human, or for localising a real or synthetic image of such internal structures within an overview image or on an overview 3D model.

B. Description of the Related Art

[0002] Endoscopy refers to techniques used to inspect or to look into internal cavities or hollow structures. Endoscopy is used today for medical applications and for industrial applications such as for instance in the visual inspection of aircraft, diesel and automotive engines by so called borescopes (horoscopes). In the medical field endoscopes are used for life saving inspections and interventions such as endoscopic surgery on organs in a patient's body cavity. Borescopes allow preventive maintenance or inspection work where the area to be inspected is inaccessible by other means. They can for instance be used for preventive maintenance and inspection tasks on targets within an enclosed structure such as aircraft engines and others which require particular attention because of safety requirements. In the remainder of this text only the medical field will be used to illustrate the new apparatus. Its applicability, however, extends without limitations to the industrial working domain.

[0003] Medical endoscopic surgery, also called minimal access surgery has become widely used over the last decade because of clear-cut advantages such as a decreased postoperative morbidity, less pain and a shorter hospitalisation. Endoscopic surgery, however, is technically more demanding than 'classical open surgery' for several reasons such as smaller instruments, and the limitation of the smaller entry ports. The learning curve of endoscopic surgery is much longer than expected a decade ago.

[0004] A crucial problem remains the monocular vision with limited depth perception, together with a small field of view also referred to as 'tunnel vision'. Normally surgeons work with a camera acquiring video data through the endoscope, and perform surgery on a video display. This causes most depth of vision cues to be lost. The small field of view leads to difficulties of orientation and surgical mistakes. Experimentally, we were able to dem-

onstrate in a rabbit nephrectomy model that the duration of surgery, bleeding and accidents increase when the fields of view becomes smaller. This increase in duration of surgery and in accidents as a consequence of the small field of view decreases with the experience of the surgeon, suggesting that with experience and training the human brain is capable of reconstructing to a certain extent a broader field of view from the video data given. Unexperienced surgeons perceive this problem much more since they are not able to mentally reconstruct such an overview of the working field. Another limitation of the small field of view is the difficulty to position instruments into the field of view : surgery is performed with the lens at a short distance of the target tissue, eg 2 to 3 cm in order to obtain a sharp enlarged image. To position an instrument 'blindly' in this field of view requires a lot of experience and training. The alternative is to zoom out to visualize the instrument and then to zoom in again maintaining the instrument in the field of view. It is obvious, that this requires time, slowing down the surgery. During emergency cases eg an important bleeding, this becomes crucial : the artery should be clamped within seconds with the camera at short distance for visualization. If this fails, the operating field is flooded with blood, making things more difficult. This is the main reason why in gynaecologic surgery, for hysterectomies the conversion rates (ie to change from laparoscopy to laparotomy) range from 0 to 30 % according to the experience of the surgeon.

[0005] Implementations of non-monocular vision through an endoscope are in general embodied as a stereo setup. Two nearby optical pathways provide a baseline and therefore show two different real, but nearby viewpoints. If presented respectively to the left and right eye, this leads to depth perception for a human observer. However, this approach has several drawbacks, like eg. the need for an endoscope with a larger cross section or with smaller optical pathways. Moreover, stereoscopic visualization has no transparent implementation yet and requires eg shutter glasses, auto-stereoscopic displays or head mounted displays. Today these approaches to 3D visualization have failed to become widely accepted in endoscopic surgery because too cumbersome and too expensive without real demonstrable benefits.

[0006] The limitation of a restricted view has been addressed historically by building wide angle lenses. These have the drawback, however, that a close up view can only be obtained with the lens at a short distance from the tissue, thus making the working distance, ie the distance between lens and tissue limited. Another approach is by using with the endoscopes a varifocal camera unit or by using lenses with different focal lengths. This provides a surgeon with an optical zoom, and allows to restrict or enlarge the working field. However, zooming and refocusing is not straightforward per-operatively and is no real option to get a quick overview of the scene. Indeed if one hand holds a camera with a lens, a second hand is needed to adjust the angle of view ; this second hand

this is no longer available for surgery, A zoomed out camera view -even if used with larger monitors- is not practical to work with.

[0007] The problem thus narrows down to the dilemma, that we need a high resolution essential to work. This requires either a wide angle at short distance or a narrow view at larger distance. The former solution limits the working space, the latter solution makes an overview picture practically impossible. Today lenses and camera units with a variable field of view exist but are not really used for practical reasons.

[0008] More recently so called 'capsule endoscopy' has been introduced. This technique normally refers to the concept of 'a camera in a pill'. The device is swallowed and travels independently the internal digestive system. During this passage video data (and eventually supplementary data) are being collected and either stored in local memory or send to a receiver using a wireless link. One of the promoter applications of this technique is the inspection of the small intestine eg to check whether anemia could be caused by intestinal bleeding.

Problem summary

[0009] Despite the advanced stage of current systems for video endoscopy there is a need in the art for videoendoscopes or videoboscopes that ascertain ease and safety of critical operations by providing an accurate depth perception and ease of positioning the instruments in the field of view. Moreover the working field is limited and there is no means to visualize instruments outside this field of view and still keep a high resolution image of the local working field. No method or apparatus currently can generate either an overview image of the endoscopic working volume, or multiple different viewpoints of the endoscopic working volume. Neither are there existing systems for endoscopic 3D acquisition, which can generate quantitative 3D measurements, and this through an unmodified mono focal endoscope, even in case of a deformable environment. The difference with stereo endoscopy or stereoscopic endoscopy and visualisation will be explained later in this text and mainly relate to the relative distance between the different lenses and the size of the object. In endoscopic stereo systems the lenses are near to each other when compared to the relative size of the objects, in the system of present invention this is no longer the case. In a stereo endoscope the two centers of the lenses are typically some 10 mm apart, whereas now we can separate the lenses up to 50mm or more. Moreover the distance between the lenses is not fixed at construction time, as is the case in a stereoendoscope but can be fixed at deployment time, or even can be changed during operation. This is by no means possible in case of a stereo system. Also the system is by no means limited to the use of two lenses or cameras only, as is the case in a stereo endoscope, but can use multiple different cameras at the same time.

[0010] Known from prior art are US patent 5,653,677,

US patent application 2005/234294 and US patent application 2005/014994. US 5,653,677 describes an electronic endoscope apparatus having an imaging unit separable from the distal end portion of an endoscope and allowing easily handling and operating the separated imaging unit. An imaging device is arranged as a separate member so that the imaging unit can be separated from the distal end portion of the endoscope. Observing means may be provided with the endoscope main body independently of the imaging unit and further a stereoscopic image may be formed by the imaging device and the observing means. US patent application 2005/234294 describes methods and apparatus for obtaining endoluminal access. An elongate body is configured for insertion within a body lumen, conduit, organ, orifice, passageway or cavity, the elongate body having a working axis and a distal region, and an articulating element disposed near the distal region, the articulating element configured to articulate off-axis from the working axis of the elongate body. The elongate may achieve access in an endoluminal or a laparoscopic fashion. US patent application 2005/014994 describes an insertable device for insertion in a bodily cavity, the insertable device being configured such that the functional elements have various degrees of freedom of movement to provide access to the site from multiple and different orientations/perspectives as the procedure dictates, e.g., to provide multiple selectable views of the site, and may provide a stereoscopic view of the site of interest.

[0011] Present invention provides solutions to the aforementioned problems by combining a high resolution video stream of the local working field (local zoom in) together with a general overview of the overall scene (zoom out) and this without the need for additional incisions and the possibility to shift the region of interest without physically moving the optics. Moreover it can generate 3D information of a moving and deformable endoscopic scene with an unmodified mono focal endoscope and the multi view camera setup.

SUMMARY OF THE INVENTION

[0012] The present invention relates to the process or a system according to the independent claims of the present invention. It relates to a process or system which allows to synthesise (extreme) wide angle mosaic images (also referred to as panoramas or synthetic overview images) of internal structures in a body, for instance the internal organs in the body of an animal or human subject.

[0013] The system comprises a multiple viewpoint camera setup and an intelligent or cognitive image control system integrated into an endoscope -a device for endoscopic surgery - , to generate synthetic viewpoints or overview images. The system of present invention provides a solution to localise the current real or synthetic image of such internal structures with respect to these overview images.

[0014] Moreover the system can generate endoscopic

3D measurements and visualisations, through an unmodified mono focal endoscope and the multiple viewpoint camera setup, or by means of mono focal endoscopic pattern projection and the multiple viewpoint camera setup. This is again different from any prior endoscopic pattern projection systems, where the baselines (camera - projector lens distance) is typically in order of 10mm whereas now we can increase it upto 50mm or more.

[0015] The system of present invention can be integrated in existing (video)endoscopic systems. A video endoscopic system that is particularly suitable to be adapted for the present invention is a video endoscopic system comprising an endoscopic optical system and a camera. In such a system the endoscopic optical system having an elongated shaft through which an optical image guide and a fiber light guide extend, and an end housing, which is proximally connected to the shaft and has an image exit window and a light entry window, the camera portion including a camera housing, extending from which are an image signal cable and a light guide cable, and an image entry window and a light exit window. The end housing and the camera housing carrying co-operating rotationally lockable coupling means, arranged to couple the housings together and to lock the housing in a relative rotational position in which the image entry and exit windows are in alignment and the light entry and exit windows are in alignment. The coupling means including a cylinder with an end wall on one of the housings and a complementary bore with a base wall in the other housing, the windows being arranged in the end wall of the cylinder and the base wall of the bore. Such has been described in US20050191046.

[0016] The imaging system of present for receiving selected images of said selected portion of a field of view of a internal structure of an enclosing body and for producing output signals corresponding to said selected images to the image capture circuitry of present invention for receiving and providing digitized signals from said output signals from said imaging system and the image transform circuitry of present invention for processing said digitized signals from said image capture circuitry can be integrated in or connected to a (microtelescopic) laparoscope, endoscope or borescope. Such a laparoscope, endoscope or borescope can be for instance of the type that comprise a) an elongated tube with an observation head in wich the image capture circuitry can be integrated; b) elongated optical conduit means connecting said head and image capture circuitry to said image capture circuitry. The elongated insertion tube can contain optical means for conducting an optical image of the target on an enclosed structure (eg internal structure in a patient's body) from an imaging system at a proximal end (from the target) of the insertion tube to an image acquiring circuitry at a distal end thereof and it may also comprise a light conduit means therein for conducting illumination for a distal light tube fitting to said proximal end (proximal to the target) of the insertion tube to illu-

minate said target.

[0017] Other systems of videoendoscopy which can be adapted by the system of present invention are disclosed in U.S. Pat. No. 5,682, 199 and U.S. Pat. No. 6,494,826 B1. These prior systems both consist of an endoscope optical system and a camera housing which may be connected by means of a coupling, whereby both the image is coupled in one direction and the light is coupled in the other direction through the coupling point with appropriate windows. Separate elements suitable for the videoendoscopic system of present invention have been described in US4697577, US5313306, US5524180, US5776050, US5876325, US5907664, US5954634, US6097423, US6371909, US6428470 and US20020022767.

[0018] An apparently related system with respect to the endoscopic 3D depth extraction has been described in

[0019] US6503195. The major differences with respect to the 3D computation relates to the baseline(s) (cfr inf) being used (the multiple view endoscopic setup is a so-called 'wide baseline' setup) and therefore the different system for 3D computation and the number of viewpoints (the multiple view endoscopic setup is by no means restricted to a single camera, or to a single camera and projection device). Moreover, the system referenced above uses an adapted endoscope whereas the present invention can work with an unmodified mono focal endoscope. In other words there is no need for a stereo camera or stereo acquisition device for the multi-view setup to work, and generate 3D information. This said the system still can work with images coming from a stereo camera.

[0020] Further scope of applicability of the present invention will become apparent from the detailed description given hereinafter. However, it should be understood that the detailed description and specific examples, while indicating preferred embodiments of the invention, are given by way of illustration only, since various changes and modifications within the spirit and scope of the invention will become apparent to those skilled in the art from this detailed description. It is to be understood that both the foregoing general description and the following detailed description are exemplary and explanatory only and are not restrictive of the invention, as claimed.

[0021] Present invention comprises an endoscopic method that instructs one or more persons carrying out surgery respectively on the primary camera providing a picture of an internal part of the body, on the secondary camera(s) providing a picture of another internal part of the body to another display means, both pictures being integrated in an overview picture or model, shown on the displays of the internal body or being shown independently. In a particular embodiment a control system transforms the multiple video streams of the cameras into a synthetic wide angle overview image. In yet another embodiment the method extracts 3D information from multiple images, not all coming from a camera mounted to the endoscope. In the remainder of the text the camera

mounted to the endoscope will be mostly referred to as the principal or primary camera, whereas the other are referred to as secondary or multi-view cameras. The latter can be inserted into a cavity through the entry port of the primary camera, without the need for additional entry ports. Insertion can also be done comparable to the primary camera using secondary entry ports and cameras outside the cavity, with a lens protruding the cavity wall. Alternatively the method generates 3D information based on the projection of structured light through a regular unmodified mono focal endoscope, while imaging the scene through a multi-view endoscopic camera network or the method generates 3D information based on the projection of structured light through a stereo endoscope, while imaging the scene through one optical channel of the endoscope, and projection through the other optical channel. In yet another embodiment the method extracts 3D information without active illumination, and only uses the different camera images therefore. In the latter embodiment one of the cameras can also be moving with respect to the set of other cameras, which comprises at least two non moving cameras. The endoscopic method of present invention can also be used to localize a moving endoscope w.r.t. a real or synthetic wide angle camera image. Furthermore it can determine the constellation of an N-camera multi-view setup, and to derive automatically a camera calibration for this setup

[0022] By the invention of present method it also is possible to generate one or more virtual, possibly moving, camera images, without the need for motion of any optical components in an endoscopic working domain.

[0023] The method of present invention is particularly suitable to implement a safety procedure to warn a user when a real or imaginary boundary is crossed. This is done using the above technique for localisation of the moving endoscope wrt the overview image.

[0024] The present invention can be an endoscopic or borescopic vision system for inspecting the inside of a cavity or guiding operation on enclosed structures in said cavity, comprising an imaging system for receiving selected images of a target object and to create said output signals of the object image which is characterised in that the imaging system comprises a camera system designed to create said output signals of different object images of portions of the target structure or the direct environment thereof, whereby the camera system comprises a first ocular system (lens or camera) and at least a second ocular system (lens or camera) of which the distances between the both ocular systems are not fixed but whereby at deployment or in operational working state the optical distance is above 10 mm, preferably above 20 mm, more preferably between 20 and 200 mm, yet more preferably above 40 mm, for instance between 40 and 200 mm and most preferably above 50 mm for instance 50 and 100 mm..

[0025] Yet another embodiment of present invention is an endoscopic or borescopic vision system for inspecting the inside of a cavity or guiding operation on enclosed

structures in said cavity, comprising an imaging system for receiving selected images of a target object and to create said output signals of the object image which is characterised in that the imaging system comprises a camera system designed to create said output signals of different object images of portions of the target structure or the direct environment thereof, whereby the camera system comprises a first ocular system (lens or camera) and at least a second ocular system (lens or camera) whereby at deployment or in operational working the relative viewpoints of said ocular systems can be modified to generate views which do not share any common structures in the scene. In a preferred embodiment this is achieved by changing the ocular distances between the ocular systems or the orientation of one or more ocular systems. This is under normal working situations not possible with for instance a stereo system.

Drawing Description

BRIEF DESCRIPTION OF THE DRAWINGS

[0026] The present invention will become more fully understood from the detailed description given herein below and the accompanying drawings which are given by way of illustration only, and thus are not limitative of the present invention, and wherein:

Fig. 1 is a schematic view showing a normal endoscopic working volume, using an external camera (A) and an endoscopic telescope to provide an image of the internal cavity. The hatched region is a representation of the camera frustum, indicating the part of the working volume visible in the camera images without moving the optics.

Fig. 2 is a schematic view showing the same endoscopic working volume of figure 1 but with a N-view endoscopic multi-view setup, with N=5. The regular endoscopic camera (A) is referred to as the primary camera, whereas cameras (B-E) are secondary multi-view cameras. The working volume visible in a camera feed now is the envelope of all camera frusta, and spans a much larger visible area. Signal and power wiring is transferred through the cavity wall, and can be used as a means to provide fixation.

Fig. 3 is a schematic view showing the same endoscopic working volume of figure 1 and figure 2 but with the wiring guided as a single string through the trocar.

Fig. 4 displays in the top row a schematic representation of the individual camera images from the cameras indicated in figure 1- 3. The bottom row shows an illustration of a synthesised wide angle image combining all individual camera images or camera video streams. It will be the control unit which provides a solution to this integration problem. As the viewpoints of the different cameras are different, the images will have to be deformed in order to construct

this overall integrated synthetic camera image. By sliding a synthetic aperture over this integrated synthetic wide angle camera image, a moving camera with new viewpoints can be generated without moving optics.

Fig. 5 shows a possible configuration which allows fixating the secondary multi-view cameras referenced in figure 3. The drawing represents a perforated base plate with centrally the secondary multi-view camera. This is a more convenient means of fixating this secondary camera, than a regular capsule device. However, this is by no means the only way of providing such fixation.

Fig. 6 is a schematic view showing the endoscopic working setup in laparoscopy, indicating the major units related to the field of this invention and its embodiment in laparoscopy, and their relationship to the patient. It is intended to provide a better understanding of the overall endoscopic working circumstances.

Fig. 7 is a flowchart explaining the initial setup, calibration and verification of the N-view constellation. Its implementation will be explained in more detail in the remainder of this text.

Fig. 8 is a schematic view showing the main functional steps required by the 'Cognitive Control Unit' in order to generate the synthetic overview image, the 3D information derived from the endoscopic scene or the localisation of the moving primary camera wrt the overview image or 3D model.

DETAILED DESCRIPTION OF EMBODIMENTS OF THE INVENTION

[0027] It will be apparent to those skilled in the art that various modifications and variations can be made in process and methods of the present invention of a multiple viewpoint endoscopic camera system, or simply multi view endoscope and its use for generating of synthetic overview images or for generating endoscopic 3D information, and in construction of the system and method without departing from the scope or spirit of the invention. Examples of such modifications have been previously provided.

[0028] Other embodiments of the invention will be apparent to those skilled in the art from consideration of the specification and practice of the invention disclosed herein. It is intended that the specification and examples be considered as exemplary only.

[0029] *Image (based) correspondences* for the meaning of present invention are points in two or more different views which correspond to the projection of the same physical world point into these views. Their representation is a vector of M position coordinates in the different images, with M the number of images between which the 'correspondence' for this point could be established. The process of establishing correspondences is also referred to as '*matching*'. In case a corresponding point for every

image pixel is searched, the latter is referred to as '*dense marching*'. The image data can originate from still pictures or from video. The same definition is used if one or more cameras are replaced by projection devices. In this case the correspondences refer to points in two or more views or projection patterns, which project upon or are the projection of the same physical world point.

[0030] *interocular distance* for the meaning of present invention is the distance between the oculars of optical instruments or the distance between the lens or camera centers.

[0031] *Camera calibration* for the meaning of present invention is the process of deriving the set of parameters which describes the image formation process of an imaging device (a camera, a video camera, an endoscopic imaging unit, ...). The complete set of techniques presented here for extended image based scene interpretation only become feasible after a successful camera calibration.

[0032] A *3D model* for the meaning of present invention is a geometric description of a scene which provides a three-dimensional location of a discrete set of points with respect to a reference point (reference of the coordinate system). Depending on the application the colour data is considered part of, or supplementary data wrt the 3D model. In the latter case the resolution of both can be different. When compared to an image (which only stores colour information), this is a richer representation of the scene. An integrated 3D model can combine more data than what can be represented in a single camera view (eg the back and frontal side of an object). Although a 3D model can be used to generate a stereo visualisation, it is fundamentally different from mere stereo acquisition. The former refers to a 3D scene analysis (a measurement), the latter is only a recording from two slightly different viewpoints and provides no scene interpretation or analysis (stereo). Terminology however can be misleading, as a stereo acquisition when presented to a human observer offers depth perception. Therefore a stereo endoscope together with a stereoscopic visualisation unit, is often referred to as a '3D endoscopic system', although it does not provide any 3D measurement or analysis of the endoscopic scene other than by the human brain. Within this text we refer to quantitative measurements.

[0033] *Frame rate, or frame frequency*, for the meaning of present invention is the measurement of how quickly an imaging device, such as computer graphics, video cameras, film cameras, and motion capture systems, produces unique consecutive images called frames. The term applies equally well to an endoscopic imaging device. Frame rate is most often expressed in frames per second or simply, hertz (Hz).

[0034] A *Cognitive Control Unit* for the meaning of the present invention is a unit which transforms raw image data coming from one or multiple cameras into a single enhanced representation. Instead of presenting the user with more information, it combines and offers enriched

information. The latter avoids flooding the human observer with too many individual streams of information such that interpretation becomes infeasible. An illustration where the latter typically can happen is a control wall for video surveillance. Presenting the different raw video streams of the multi-view camera network could lead to a similar situation. A key element which distinguishes this unit from alternative implementations is that it uses (local or distributed) intelligence to do this merging of video data based on scene interpretation. Therefore it is referred to as a cognitive unit. It is a control unit, as it introduces feedback based on its computed output to adapt or control the camera system. The level of image based interpretation needed to do so is comparable to what a human observer mentally does, and surpasses any straightforward regulatory action like eg intensity control and similar actions found in nowadays so called 'endoscopic video processors'. Illustrative examples are the construction of an integrated overview image or mosaic (sometimes also referred to as a 'panorama') of the scene, measuring a 3D model of the scene, etc

[0035] Mono focal refers to an optical system with a single optical pathway, whereas in stereo two optical pathways are used.

[0036] The baseline for the meaning of the present invention is the translation vector, (or its magnitude, depending on the context) relating the individual effective optical camera centers as obtained by the camera calibration of the different devices in a system comprising multiple cameras, or multiple cameras and a projector or multiple cameras and projectors. Effective optical camera center hereby refers to the location of the lens center as computed during the camera calibration using eg a calibration technique as described in "An Efficient and Accurate Camera Calibration Technique for 3D Machine Vision, Roger Y. Tsai, Proceedings of IEEE Conference on Computer Vision and Pattern Recognition, Miami Beach, FL, 1986, pages 364-374". Such a system is referred to as a wide baseline system if the baseline or baselines is/are of comparable size when compared to the structures in the scenes being imaged or projected on. Such condition may also imply a large rotation angle between the optical axes of the different cameras, in order to have the same scene in the field of view.

[0037] Mono focal refers to an optical system with a single optical pathway, whereas in stereo two optical pathways are used.

[0038] The baseline for the meaning of the present invention is the translation vector, (or its magnitude, depending on the context) relating the individual camera centers of the different devices in a system comprising multiple cameras, or multiple cameras and a projector or multiple cameras and projectors. Such a system is referred to as a wide baseline system if the baseline or baselines is/are of comparable size when compared to the structures in the scenes being imaged or projected on. Such condition may also imply a large rotation angle between the optical axes of the different cameras, in or-

der to have the same scene in the field of view.

[0039] A system has been developed to generate multiple (minimal two) internal views, with a difference in viewpoint which is much larger than available in stereo endoscopy. More specifically a regular stereo endoscope will have a baseline which is an order of magnitude (scale factor $\times 10$) smaller than the internal structures imaged. The current invention envisions baselines which can be of similar sizes compared to the structures being imaged and which moreover is adaptable. For medical applications this boils down to be an increase in baseline from the range of 5 to 20 mm to an extended range of 5 to 250 mm. This allows the system to generate much more fundamentally different viewpoints. The latter means that the images generated are not just similar with only a slight deformation with respect to each other, but really visualise a different part of the scene. Whereas in case of stereo imaging, typically about 75% or more of all image pixels can be related to a pixel of the secondary image by computing the corresponding local image deformation, this will no longer be the case. Hence we refer to 'fundamentally different viewpoints', originating from the relative so called 'wide baseline' setup. This said, as the baseline is adaptable and the relative orientation of the different cameras can be changed, the multi-view system can, but is not enforced to be used as a wide-baseline setup. In combination with the aforementioned cognitive image control system, this leads to a completely new endoscopic visualization.

[0040] This endoscopic system works with minimally two different cameras. The system can function with multiple cameras. For instance, it can use an extended camera array if the working field allows for their insertion. The use of up to six cameras seems to provide a reasonable trade-off between quality and system complexity. However, there is no theoretical upper bound of the maximum numbers of cameras that can be used. The latter rather is restricted by practical issues like e.g. the amount of computing power available. This said neither the implementation nor the application of present invention targets the implementation or application of image processing to achieve only stereo acquisition or visualization. But the system of present invention has as a particular advantage that availability of multiple different video sources makes it possible to carry out an operation based on a principal or primary camera image, while the secondary cameras provide a different image of another part of the targeted internal structures. The system of present invention does not have to be limited to two viewpoints only, but it extends to N viewpoints. Moreover, the secondary camera or cameras can have a different zoom and orientation and such can provide an overview image. For the secondary cameras either capsule based devices are used or (regular) endoscopic lenses and cameras, inserted through secondary entry ports. In the latter case the secondary endoscopes will preferably have a smaller section (eg 2 mm) than the primary endoscope (eg 10 mm). The original images can be presented to the sur-

geon and her/his staff as independent video streams, or are fed into the control unit which combines the different streams into a single new composite overview video image. This provides an enhanced visualization in which both a high resolution video of the working field is combined with a larger overview image (see figure 2). This enhanced view is equipped with a steerable region of interest, which makes the working field selectable without moving optical components. This functionality is provided through the cognitive control unit, and is only feasible using the multi-view camera setup. This cognitive aspect of the overall endoscopic system and the implementation by which it can be achieved is the core of the invention embodied within this apparatus. It comprises the interpretation of the scene necessary to generate the overview image. Moreover it can additionally provide an approximate or accurate dense 3D scene analysis.

[0041] The cognitive control unit is a device implementing distributed or local intelligence, and such provides a means for image analysis. The most straightforward implementation comprises a software implementation and a processor for its execution, given the real-time constraint introduced by the processing of streaming video is respected. The latter is dependent on the number of parallel camera feeds to be processed. To this end a software implementation of the logic and intelligence in combination with dedicated, or configurable signal processors is advisory. Optimally the control unit can even be completely hard coded in a dedicated signal processor, requiring limited or no software configuration. Essential for the implementation, however, is the streaming processing which requires real-time performance, without introducing noticeable input-output delay. A guideline for the former is a minimal framerate of 15hz, whereas the delay should be reduced to be smaller than approx. 30 msec. Otherwise we found out during experiments that the videostream is not perceived as being fluent enough by medical users. Moreover tests demonstrated that in case of larger delays, a human observer notices the de-synchronisation between hand movements and visual appearance while performing surgery. This said, whatever the concrete implementation of the control unit is -software & processor, software processor and signal processor, hard coded implementation, or a combination- can be selected on the basis of other considerations, as long as the real-time constraints are respected, and the image based logic is correctly executed

[0042] An embodiment of present invention is thus an endoscopic or borescopic vision system for inspecting the inside of a cavity or guiding operation on enclosed structures in said cavity, comprising an imaging system for receiving selected images of a target object and to create said output signals of the object image that is characterised in that the imaging system comprises a camera system designed to create said output signals of different object images of portions of the target structure or the direct environment thereof, whereby the camera system comprises a first ocular system (lens or camera) and at

least a second ocular system (lens or camera) whereby at deployment or in operational working the ocular distances between the ocular systems are controllable to change the different viewpoints relatively to each other.

5 This ocular systems may controllable to change the different viewpoints relatively to each in such to generate views which do not have image correspondences or which do not share any common structures or which do not share in the scene.

10 **[0043]** A particularly suitable endoscopic or borescopic vision system is such as above but whereby the distances between the both ocular systems can change but whereby at deployment or in operational working state the optical distance is above 20 mm. In a preferred embodiment such endoscopic or borescopic vision system is characterised in that the distances between the both ocular systems can change but whereby at deployment or in operational working state the optical distance is above 50 mm

20 EXAMPLES OF SELECTED ILLUSTRATIVE EMBODIMENTS OF A MULTI VIEW ENDOSCOPIC SETUP AND THE OPERATION OF THE COGNITIVE CONTROL UNIT

25 Example 1: multiview endoscopic visualisation with fine tuning of the multi view camera network **Embodiment of the invention in laparoscopy**

[0044] In laparoscopy, being endoscopy in the abdominal cavity, endoscopes are normally rigid with a camera outside the body. The endoscope is inserted through a single small incision. Additional incisions allow to insert specific endoscopic (surgical) instruments. The working field contains considerably large variations in depth, relatively to the standoff (distance between tissue and lens) of the endoscopic telescopic lens. The telescope is used to visualize a particular region of interest within the abdominal cavity. This means that secondary regions are not visible to the surgeon or her/his staff. Nevertheless it often occurs that one or more assistants are keeping structures away outside the field of view. In such case this is done without any vision based feedback for neither the surgeon nor her/his assistants. The same reasoning applies when surgery is performed very close to vital or fragile organs and structure (eg the ureters, veins, nerves, etc...)

[0045] The apparatus of present invention implements a way to avoid this partially blind operation. To this end one or more secondary cameras are inserted into the body through the same incision as used to insert the regular endoscope (see figure 3). Devices derived from endoscopic capsule cameras with a 40 degree re-orientable head are suitable as secondary cameras. Alternatively secondary entry ports to the body can be used, with regular -possibly thin cross section- endoscopes.

[0046] For low frame rates or frame frequencies wireless transmission is used in case of capsule devices, whereas for fluent video rates the same devices in a wired

configuration are used. In laparoscopy or borescopy the wiring is guided as a joined string through the trocar or entry shaft to the cavity (see figure 3), or as per camera signal wire (see figure 2) directly through the abdominal wall or cavity wall. In the latter case the signal and power wiring provides also fixation. In the wireless case this fixation is done using one or more stitches. To this end the camera housing provides a ways to fixate them, and the shape is adapted for adhesion to the abdominal wall (see figure 5 for an illustration). The internal configuration of the secondary cameras loosely defines the new overall integrated working field that will become available. The re-orientable camera heads allow the system to automatically fine-tune its configuration (e.g. its field of view). The fine tuning is steered by a new algorithm minimising the distance between the intersection points of the different optical axes (center lines) of the lenses in the multi view camera system (cfr. inf.). It is executed by the cognitive control unit. Internally the cognitive control unit will extend the outcome of, and work further on, algorithms known within the community of computer vision, and which are commonly referred to as 'wide base line matching', 'dense matching', 'affine invariance', 'camera auto calibration', 'camera auto calibration with internal pre calibration' and 'shape from video'.

[0047] In case the implementation uses the same devices with fixed camera heads, or in case of use of regular endoscopes through secondary entry ports, the additional fine tuning is not longer possible but the overall functionality would be still available, albeit in a restricted form. After insertion the apparatus first runs a self configuration, during which an image based mutual localisation of the N cameras is performed followed by the fine tuning of the configuration.

[0048] Therefore the optical endoscopic or borescopic system of present invention comprises a turnkey technique to find corresponding regions, eventually refined to corresponding points between the different cameras. To this end the control unit performs a so called wide baseline matching using 'invariant regions'. By a combination of multiple different techniques (SIFT / SURF / affine invariance) better performance and robustness is obtained, due to self checking and voting based on this algorithmic redundancy. The resulting feature vectors of corresponding points lead unambiguously to an initial orientation of the internal camera network. The latter is done based on a decomposition of the so called essential matrix, which is derived from the initial set of matches. This process is executed taking into account the statistical relevance of each of the hypotheses of the solution, using only a minimal set of points to obtain this solution. The latter asks for respectively 5 or 8 corresponding points between two cameras, depending on whether internal camera parameters (cfr camera calibration) are known. The robust estimation process (eg a RANSAC implementation) provides optimal robustness against outliers.

[0049] When available, the camera-to-camera view geometry (the 2-view epipolar geometry) is used to start

a constrained image matching process by searching for corresponding points only when they also respect the multiple-view geometry.

[0050] Based on this primary orientation the camera heads are adjusted and can be directed towards the shared working volume. This is done by a joined minimisation of the distances between the optical axis of the different cameras and their 3D intersection. The latter is obtained by executing a numerical solver (eg Levenberg-Marquardt) which minimises this cost function. As the optical axes of the different cameras will never intersect in a single point in space but will cross, the center of gravity of the point cloud generated by the midpoints of the shortest (L2 distance) connecting vectors between the different optical axes is used. A valid initialisation is one which, with enough freedom to reorient the camera heads, will converge to a unique solution. Under normal circumstances the outcome, however, will only be an approximation due to a limited number of iterations and finite motion of the heads. After reorienting the camera heads, the cameras self-localisation is re-executed and refined. Given the initial localisation and the knowledge of how the camera heads are re-oriented, the matching process becomes less demanding every iteration, and therefore can be executed faster. This finishes the initial setup of this so called internal camera network. The computation of this initial setup is illustrated in the flowchart of figure 7. In figure 7 it is also indicated that in case the system can not be bootstrapped the user is asked to take a decision, and eventually will have to adapt the initial multi-view camera network.

[0051] In case of a non rigid environment this setup procedure is automatically re-executed whenever necessary. To this end a procedure to self check decides when the latter is necessary. During experiments this was done by checking the back projection error on the computed 3D geometry in the N-view cameras. As a practical threshold an average deviation of 1 pixel can be used. In case no underlying 3D is computed, similarly the deviation wrt the epipolar geometry can be used as a self check mechanism.

[0052] Based on the resulting set of high quality correspondences, the camera configuration or constellation is determined using either auto calibration (if no pre-calibration is available), either the above derived 6 DOF camera mutual localisation is used as an external calibration. A bundle adjustment finalizes the calibration (see figure 7 'multi view calibration'). Again, if the calibration is not successful the user is informed about this. At this point the system know the location of the multi view cameras, has possibly adapted the viewing directions of the camera heads, and has performed a full camera calibration.

[0053] Secondly a regular endoscope is inserted through the standard entry port. The system of present invention configured so far can be used already as a multi view endoscopic view system. The normal regular endoscopic view is available to the surgeon, whereas on sim-

ple request the control unit either switches the view to that of one of the secondary cameras, or shows a tiled overview of one or more cameras on top of the primary image.

[0054] The true performance of the system however is only unleashed when the image data is not directly presented to the medical staff, but if it is used as the input for the control unit (cfr. inf.).

Example 2: multiview endoscopic visualisation and generation of a synthetic overview image or panorama

Implementation of the optical large view endoscopic systems of present invention

[0055] It is explained beforehand that scene interpretation and analysis --or the 'intelligence' offered by the endoscopic control unit-- is what this apparatus really distinguishes from any other endoscopic imaging system.

[0056] On the one hand the apparatus can generate a regular endoscopic view, on the other hand the underlying scene model opens the way to a massive set of new technical/medical applications. The presentation of this enhanced information can be done transparently (ie a surgeon is presented subtly enriched information without s/he even realising it) or very explicitly. Examples of both will be provided as an illustration of the application domain. However an exhaustive description of the complete set of possible applications simply is not feasible. We hereunder as embodiments rather provide pointers to general examples and a high level description of the methodology used to implement them:

First embodiment:

[0057] Integrating the different video feeds coming from the system described under 'Example 1' leads to a truly enlarged field of view, as a new virtual overview camera can be build. This virtual camera view interpolates smoothly between the real cameras and their real resolutions. This can not only make the new overview possibly an extremely wide angle, but also provides a movable viewpoint without the need for moving cameras. The same is true for adapted resolutions. The exact size of the wide angle is determined by the area of the scene covered by the multi view cameras.

[0058] To this end a set of 'secondary cameras' (minimal two) is inserted, and attached so that the working field can be imaged (see also the description earlier). It is not a prerequisite for these cameras to be fully calibrated beforehand, but having a pre-calibration available increases robustness. Such a pre-calibration is performed using one of the standard techniques described in the literature (eg a "Tsai camera calibration" method). The locations of the cameras and their view directions roughly define the enlarged multi-view volume that will become available.

[0059] After insertion, the constellation of the multi-view setup is determined using the techniques of 'Example 1'. If no calibration can be determined, the system falls back to become a mere N-view visualisation unit.

5 The user is informed of this more restricted performance, which in this case is limited to scenes with relatively limited variation in depth. To test this, experiments are performed during which extended retinal overview images are synthesised , without first obtaining a calibration.

10 Extension of the embodiment: continuous matching and generating of 3D information

[0060] Given the constellation and calibration of the system is known, the orientation of the cameras is adapted to visualise a more overlapping part of the scene as described earlier. This will be done each time the system detects a deviation of the last known constellation. (see figure 8 'determine corresponding regions/points', 'verify constellation')

20 **[0061]** From now on the system perpetually will start to generate a set of correspondences based on each image of the cameras. In case of fluent video, the matching process takes also time continuity into account. This operation is executed online, ie the execution of this process is not postponed to a later stage but is done in parallel with the video acquisition. In case of the calibrated setup, 3D localisation of the corresponding feature points now also is performed.

25 **[0062]** Extension of the embodiment: generating of an extended overview image (see figure 4 and figure 8) Given the correspondences between the N views and a sparse set of 3D points, an integrated overview image is generated, and updated at a fixed rate. The latter framerate can be adapted, but can be limited by the amount of computing power available or the use of an excessive number of cameras. The reference implementation can run at 15hz for 6 cameras. Extended optimisation and further parallelism can improve this framerate.

30 **[0063]** This generating of an overview image, can be compared to solving a puzzle: each of the multi-view cameras generates a piece of a puzzle. The correspondences determined earlier indicate how to put the pieces together. This however only works if the puzzle has relatively limited depth variation. In all other cases the different pieces can not be outlined consistently anymore. This is overcome by modulating the surface on which we reconstruct this puzzle, based on the 3D information derived earlier. This also explains why, if no calibration could be obtained, the technique will only work for scenes which have relatively limited variation in depth. The implementation uses texture blending with illumination correction on a depth modulated projection surface. These operations can be speeded up using techniques for so called accelerated 3D graphics on a programmable Graphics Programming Unit (GPU).

35 **[0064]** Extension of the embodiment: localisation of the primary endoscopic lens wrt the synthetic overview im-

age (see figure 8 'track feature points', 'rough localisation moving camera', 'fine localisation on overview')

[0065] Whereas the earlier described multi view cameras are relatively stable, the primary endoscopic lens inserted can be very mobile. This source of video data can be thought of as a 'spotlight' wandering over the surface being built up. By tracking an extended set of points within the video data generated by this 'primary endoscopic video source' a continuous approximate self localisation can be performed and updated using a standard ego-motion algorithm (sometimes referred to as 'visual odometry'). By relating this to the extended overview images generated, we obtain an accurate localisation within a single coordinate system. The latter is done by pixel based matching, and using a 'position from structure' technique to update the position of the moving camera.

Extension of the embodiment: visualisation

[0066] The new multi-view image data can be visualised in multiple ways. Either the overview and primary endoscopic image are displayed independently, either an integrated visualisation is shown. In the latter case the localisation relatively wrt the overview can be seamlessly hidden, or in contrary, indicated explicitly on the overview image. The latter can be done using a border indication, or by highlighting of the primary image on the overview. The integrated visualisation is done by showing fine registered textures aligned on the approximate 3D model, or on a (3D modulated) projection surface.

[0067] In case of the integrated visualisation, the relative motion and zoom of the visualised video data is no longer restricted to what the real primary endoscopic camera can generate, but extends to the full size of the multi-view endoscopic working volume. This can be considered an example of the subtle (or transparent) visualisation of the enriched information. If it doesn't affect safety considerations (eg in an industrial application) the difference between real and synthetic camera data can be made less apparent.

Example 3: Additional application options of the optical large view endoscopic systems of present invention

[0068]

3.1) If not the synthetic overview images are of primary interest, but the 3D information than the system can generate, the apparatus can be switched to a so called 'dense 3D' modus. Now dense matching at reduced framerates is performed, but depth measurements for as many points as possible are generated. The number of generated points/image strongly depends on the scene under consideration. However, if less than 20% of the image points result in a 3D measurement, the system indicates failure of operation under the current working circumstances.

The 3D information in this case results from N (partially) matched views, possibly using a wide baseline constellation. The depth is computed using a standard 2 or 3 view optimal triangulation technique. The technique is called passive 3D reconstruction, as no explicit structured illumination is needed.

3.2.) If example 3.1 fails to generate robust data or if higher accuracy is desired, the system can operate in an 'active dense 3D' modus. To this end a source of structured light (or active illumination) is introduced through the (primary) endoscope. The secondary multi-view cameras now are presented a very apparent set of visual features which facilitate the matching process. It is important to state that the baseline in this system -now between camera and projection system- is again considerably larger than what can be obtained by any other system. By generating adaptable patterns system robustness can be improved, through projection of so called (adaptively) coded structured light. This technique is a so called active technique for 3D reconstruction, again possibly using an extreme wide-baseline setup. Experiments showed an accuracy using this modus which can be better than 100 micrometer, whereas the average accuracy of the regular 'dense 3D' modus is about 10 times lower.

3.3.) The availability of the dense 3D model asks for new visualisation techniques, or at least makes this possible. A particular new application wrt visualisation is the merging of synthetic 3D data and models with the data obtained online through the endoscope. This can be considered an example of an explicit visualisation of the enriched information. In the literature these techniques are mostly referred to as augmented reality or enhanced reality. The availability of the (dense) 3D measurements makes it possible to implement them using endoscopic imaging.

SURGICAL APPLICATIONS AND ADVANTAGES

[0069] The endoscopic system of present invention has applications and advantages for critical operations on structures in an enclosed body such as surgery.

1. The enlarged view is demonstrably more important for surgeons with less experience, ie during training, and for those assisting the main surgeon. In animal models it has been shown that it decreases operating time, accidents, bleedings and errors of judgments. Pilot experiments suggest that this will also be true in human surgery.
2. The enlarged view helps with the positioning of instruments in the field of view of the operating camera, thus reducing the problems of stereotaxis and thus decreasing time loss. We anticipate that in randomized trials the conversion rate for eg hysterec-

tomy will be lower. This will constitute a proof that control of bleeding is faster and more accurate.

3. The enlarged view will visualize all the instruments : this will prevent to a large extend the rare accidents caused by this blind manipulation and certainly the accidents, if they occur, will have a much higher probability to be visualized and recognized. We recently reported large and small bowel perforations, with subsequent severe peritonitis, probably caused by a blind instrument since on the video of the surgery itself no injury to the bowel could be seen. If a wide angel view would have been available, the assistant would have had visual control thus preventing accidents, and if nevertheless they would occur, they would have been recognized.

4. The depth enhanced view and localization offers new tools to implement intelligence to increase safety and permit disaster recovery procedures. Firstly regions in which no activity (cutting, clamping, or simply motion...) is to be tolerated can be indicated. The system can give a warning when such an imaginary or real boundary is crossed. Similarly since the synthetic overview image has generated a model of the scene this overview image can be used if the image from the primary camera fails, eg by a vessel pumping blood over the lens. Even if all cameras in the multi-view system would become unavailable (which is unlikely) still the underlying model or synthetic overview image remains available as a good approximation of the real image.

5. The possibly dense depth computation allows for implementing enhanced reality in endoscopy, visualizing and aligning structures generated by other imaging modalities such as CT, MRI etc. The applicability of these enhanced reality techniques is greatly improved by the multi view cameras, as the system becomes also less dependent on external motion tracker systems, and can do better registration. Moreover it offers a means to obtain quantitative 3D information in endoscopy and such to make measurements within a cavity.

An additional difference between the present invention and existing stereo endoscopes or more generally systems used for stereoscopic endoscopy, is that present invention can deduce 3D information from images which for a human observer do not generate a 3D stereo impression when viewed by the observer directly. The latter, however, is the main target of any stereoscopic system.

6. The present system allows to the user or surgeon to per-operatively reorient the lenses and thereby to change the view or field of view of the endoscopic imaging system, which is not possible with a stereo endoscope, as the lenses are rigidly attached to each other at construction time.

7. During surgery orientation of the image remains problematic, since rotation of the camera will rotate the image. Moreover, the restricted field of view (tun-

5

10

15

20

25

30

35

40

45

50

55

nel vision) without clear landmarks indicating horizontal or vertical directions, leads to a situation where a rotated camera view is not perceived as being obviously 'incorrect': there are no visual clues indicating that the perceived situation does not reflect reality in terms of horizontality. Since the camera, and thus also its orientation, generally is controlled by the assistant, this can lead to important errors of judgment. If the camera is, as an example, rotated 45 deg to the left, it results in a situation where the upward direction in the resulting images in fact is pointing to the right side in reality. If the images of the fixed cameras or the points of reference are used to rotate the image of the main camera back to its normal position, a new and effective means of orientation correction is obtained. Also in case of the mono focal setup, a single camera system can be corrected for rotational orientation using the techniques described in present invention. In case the multi camera setup can be used, this correction can be done in a more effective way, which risks to be less error prone.

[0070] In other words, present invention allows to do rotational orientation correction of a endoscopic camera view such that the visualized horizontal direction corresponds to the horizontal direction in reality, and this without any external rotation sensor but by image processing only.

[0071] The system is very cost effective: the original endoscopic image is available the same way and quality as beforehand as the original imaging pipeline is not modified. Moreover the implementation can run completely transparently.

Claims

1. An endoscopic or borescopic vision system for inspecting the inside of a cavity or guiding operation on enclosed structures in said cavity, comprising an imaging system for receiving selected images of a target object and to create output signals of the object image, the imaging system comprising a camera system designed to create output signals of different object images of portions of the target structure or the direct environment thereof, the camera system comprising a first ocular system, the first ocular system being a lens or a camera, and at least a second ocular system, the second ocular system being a lens or a camera, at deployment or in operational working the ocular distances between the ocular systems or the relative orientation of the ocular systems being controllable to change the different viewpoints relatively to each other, wherein the distance between the ocular systems is changeable, wherein the system is adapted for determining a con-

figuration or constellation of the camera system and the baseline between the ocular systems is selectable at deployment or in operational working state in the range 20 to 250mm,

wherein the system is adapted for combining the output signals into integrated video data taking into account said configuration or constellation,

characterised in that

said integrated video data comprises a synthetic overview image, in which generating the synthetic overview image comprises using texture blending with illumination correction on a depth modulated projection surface.

2. The endoscopic or borescopic vision system of claim 1, whereby the distances between the ocular systems can change but whereby at deployment or in operational working state the optical distance is above 50 mm, resulting in a wide baseline vision system, given the size of structures in a scene being imaged during endoscopy.
3. The vision system of any of the previous claims, wherein the imaging system comprises a camera system that comprises a first and a second camera or multiple secondary cameras designed to create said output signals of different object images of portions of the target structure or the direct environment thereof based on multiple viewpoint wide baseline imaging, and further comprises an image processing or control means, communicatively coupled to the image acquiring circuitry configured to process the received digitized signals object, which cannot be seen by the principal camera, which is under normal working situations not possible with a stereo system.
4. The vision system of any of the previous claims, further comprising a multi view camera system designed to generate different viewpoints by each of the cameras or to provide several viewpoints of the internal object each by different cameras, whereby the cameras have a different zoom and orientation.
5. The vision system of any of the previous claims, whereby the first camera is a principal camera designed to create an object image of the target object on the internal structure to be operated and the second camera or cameras is or are secondary camera or cameras designed to provide image of another portion of the object.
6. The vision system of any of the previous claims, whereby the image processing means is adapted to find the corresponding image points between the images from different cameras based on a wide baseline matching system.
7. The vision system of any of the previous claims,

whereby the image processing means comprises a computer program code to carry out a turnkey technique to find corresponding regions of object images from separate cameras and to direct the cameras of the image system towards the shared working volume.

8. The vision system of any of the previous claims, whereby the image processing means is designed to transform the multiple video streams of the cameras into a synthetic wide angle overview image in real time and present this synthetic data to the user, and, for generating one or more virtual camera images, without the need for motion of any optical components.
9. The vision system of any of the previous claims, whereby the image processing means is designed to extract 3D information from multiple images of which some are obtainable from a camera that is not mounted to the endoscope.
10. The vision system of any of the previous claims, whereby the image processing means is designed to generate 3D information based on the projection of structured light through a regular unmodified mono focal endoscope, while imaging the scene through a multi-view endoscopic camera network.
11. The vision system of any of the previous claims, whereby the image processing means is designed to generate 3D information based on the projection of structured light through a stereo endoscope, while imaging the scene through one optical channel of the endoscope, and projection through the other optical channel.
12. The vision system of any of the previous claims, whereby the image processing means is designed to implement a disaster recovery procedure or a safety procedure using the underlying model or synthetic overview image as a good approximation of the real image.
13. The vision system of any of the previous claims, whereby the image processing means is designed to implement enhanced reality visualisation merging endoscopic video data with data coming from another modality based on the interpreted scene data by the cognitive processing means.

Patentansprüche

1. Endoskopisches oder boreskopisches Bildverarbeitungssystem zum Inspizieren der Innenseite eines Hohlraumes oder zum Führen einer Operation an einer geschlossenen Struktur im besagten Hohl-

raum, ein Abbildungssystem zum Empfangen von ausgewählten Bildern eines Zielgegenstandes und zur Erzeugung von Ausgangssignalen des Gegenstandsbildes umfassend,

wobei das Abbildungssystem ein Kamerasystem umfasst, das dazu bestimmt ist, Ausgangssignale von verschiedenen Gegenstandsbildern von Abschnitten der Zielstruktur oder der unmittelbaren Umgebung davon zu erzeugen, wobei das Kamerasystem ein erstes Okularsystem umfasst und das erste Okularsystem eine Linse oder eine Kamera ist, und zumindest ein zweites Okularsystem, wobei das zweite Okularsystem eine Linse oder eine Kamera ist, wobei die okularen Abstände zwischen den Okularsystemen oder die relative Ausrichtung der Okularsysteme beim Einsatz oder in betrieblicher Bearbeitung steuerbar sind, um die verschiedenen Blickpunkte zueinander zu ändern, wobei der Abstand zwischen den Okularsystemen geändert werden kann,

wobei sich das System dazu eignet, eine Konfiguration oder Konstellation des Kamerasystems zu bestimmen und die Basislinie zwischen den Okularsystemen beim Einsatz oder im betrieblichen Bearbeitungsstatus im Bereich von 20 bis 250 mm eingestellt werden kann,

wobei sich das System dazu eignet, die Ausgangssignale unter Berücksichtigung der besagten Konfiguration oder Konstellation in integrierte Videodaten zu kombinieren,

dadurch gekennzeichnet, dass

die besagten integrierten Videodaten ein synthetisches Übersichtsbild umfassen, wobei die Generierung des synthetischen Übersichtsbilds die Verwendung von Überlagerungen mit Beleuchtungskorrektur auf einer tiefenmodulierten Projektionsfläche umfasst.

2. Endoskopisches oder boreskopisches Bildverarbeitungssystem nach Anspruch 1, wobei sich die Abstände zwischen den Okularsystemen ändern können, wobei der optische Abstand beim Einsatz oder im betrieblichen Bearbeitungsstatus jedoch über 50 mm liegt, was angesichts der Größe der Strukturen in einer Szene, die während der Endoskopie abgebildet werden, ein breitgefächertes Basislinien-Bildverarbeitungssystem ergibt.
3. Bildverarbeitungssystem nach irgendeinem der vorherigen Ansprüche, wobei das Abbildungssystem ein Kamerasystem umfasst, das eine erste und eine zweite Kamera oder mehrere sekundäre Kameras umfasst, die konzipiert wurden, um die besagten Ausgangssignale von verschiedenen Gegenstandsbildern von Abschnitten der Zielstruktur oder der unmittelbaren Umgebung davon basierend auf einer breitgefächerten Basislinien-Bildverarbeitung mit mehreren Blickpunkten zu erzeugen, und darüber

hinaus Mittel zur Bildverarbeitung oder Steuermittel umfasst, die kommunikativ mit der Bilderfassungsschaltung gekoppelt sind, die konfiguriert ist, um den empfangenen digitalisierten Signalgegenstand zu verarbeiten, der von der Hauptkamera nicht gesehen werden kann, was in normalen Arbeitssituationen mit einem Stereosystem nicht möglich ist.

4. Bildverarbeitungssystem nach irgendeinem der vorherigen Ansprüche, das darüber hinaus ein Mehrfachansicht-Kamerasystem umfasst, das dazu bestimmt ist, um verschiedene Blickpunkte von jeder der Kameras zu generieren, oder um verschiedene Blickpunkte des internen Gegenstands jeweils durch verschiedene Kameras beizusteuern, wobei die Kameras unterschiedliche Zooms und Ausrichtungen aufweisen.
5. Bildverarbeitungssystem nach irgendeinem der vorherigen Ansprüche, wobei die erste Kamera eine Hauptkamera ist, die dazu bestimmt ist, ein Gegenstandsbild des Zielobjekts der zu operierenden internen Struktur zu erzeugen, und die zweite Kamera oder Kameras eine Sekundärkamera oder Sekundärkameras sind, die dazu bestimmt sind, um ein Bild eines anderen Abschnitts des Gegenstands beizusteuern.
6. Bildverarbeitungssystem nach irgendeinem der vorherigen Ansprüche, wobei die Bildverarbeitungsmittel dazu bestimmt sind, um basierend auf einem breitgefächerten Basislinien-Abgleichungssystem die entsprechenden Bildpunkte aus den Bildern von verschiedenen Kameras herauszufinden.
7. Bildverarbeitungssystem nach irgendeinem der vorherigen Ansprüche, wobei die Bildverarbeitungsmittel einen Computerprogrammcode umfassen, um eine schlüsselfertige Technik auszuführen, um die entsprechenden Regionen der Gegenstandsbilder aus getrennten Kameras zu finden, und um die Kameras des Bildsystems zum gemeinsamen Arbeitsvolumen anzuordnen.
8. Bildverarbeitungssystem nach irgendeinem der vorherigen Ansprüche, wobei die Bildverarbeitungsmittel konzipiert sind, um die verschiedenen Videostreams der Kameras in Echtzeit in ein synthetisches Weitwinkel-Übersichtsbild zu verwandeln, und um diese synthetischen Daten dem Benutzer zu präsentieren, und zum Generieren von einem oder mehreren virtuellen Kamerabildern ohne dafür optische Bauteile bewegen zu müssen.
9. Bildverarbeitungssystem nach irgendeinem der vorherigen Ansprüche, wobei die Mittel zur Bildverarbeitung konzipiert sind, um eine 3D Information aus mehreren Bildern zu extrahieren, von denen einige

aus einer Kamera erhalten werden können, die auf dem Endoskop montiert ist.

10. Bildverarbeitungssystem nach irgendeinem der vorherigen Ansprüche, wobei die Mittel zur Bildverarbeitung konzipiert sind, um eine 3D Information basierend auf der Projektion von strukturiertem Licht durch ein reguläres unverändertes monofokales Endoskop zu generieren, während die Szene durch ein endoskopisches Kameranetzwerk mit mehreren Ansichten abgebildet wird. 5
11. Bildverarbeitungssystem nach irgendeinem der vorherigen Ansprüche, wobei die Mittel zur Bildverarbeitung konzipiert sind, um eine 3D Information basierend auf der Projektion von strukturiertem Licht durch ein Stereo-Endoskop zu generieren, während die Szene durch einen optischen Kanal des Endoskops und die Projektion durch den anderen optischen Kanal abgebildet wird. 10
12. Bildverarbeitungssystem nach irgendeinem der vorherigen Ansprüche, wobei die Mittel zur Bildverarbeitung konzipiert sind, um einen Notfallplan oder ein Sicherheitsverfahren unter Verwendung des zugrundeliegenden Modells oder des synthetischen Übersichtsbildes als gute Annäherung an das echte Bild umzusetzen. 15
13. Bildverarbeitungssystem nach irgendeinem der vorherigen Ansprüche, wobei die Mittel zur Bildverarbeitung konzipiert sind, um Darstellungen erweiterter Realität, die endoskopische Videodaten mit Daten zusammenlegen, die aus anderen Modalitäten stammen, umzusetzen, die auf den durch die kognitiven Verarbeitungsmittel interpretierten Szenendaten basieren. 20

Revendications

1. Un système de vision boroscopique ou endoscopique destiné à l'inspection de l'intérieur d'une cavité ou au guidage d'une opération sur des structures enfermées dans ladite cavité, comprenant un système d'imagerie destiné à la réception d'images sélectionnées d'un objet cible et à la création de signaux en sortie de l'image d'objet, le système d'imagerie comprenant un système de caméra conçu de façon à créer des signaux en sortie de différentes images d'objet de parties de la structure cible ou de l'environnement direct de celle-ci, le système de caméra comprenant un premier système oculaire, le premier système oculaire étant une lentille ou une caméra, et au moins un deuxième système oculaire, le deuxième système oculaire étant une lentille ou une caméra, au déploiement ou en état de fonctionnement opérationnel, les distances 25

oculaires entre les systèmes oculaires ou l'orientation relative des systèmes oculaires pouvant être commandées de façon à modifier les différents points de vue relativement les uns aux autres, où la distance entre les systèmes oculaires est modifiable, où le système est adapté de façon à déterminer une configuration ou une constellation du système de caméra et la ligne de base entre les systèmes oculaires est sélectionnable au déploiement ou en état de fonctionnement opérationnel dans la plage 20 à 250 mm, où le système est adapté de façon à combiner les signaux en sortie en données vidéo intégrées prenant en compte ladite configuration ou constellation, **caractérisé en ce que** lesdites données vidéo intégrées contiennent une image globale synthétique, la génération de l'image globale synthétique comprenant l'utilisation d'un mélange de textures avec une correction d'éclairage sur une surface de projection modulée en profondeur.

2. Le système de vision boroscopique ou endoscopique selon la Revendication 1, où les distances entre les systèmes oculaires peuvent changer mais où, au déploiement ou en état de fonctionnement opérationnel, la distance optique est supérieure à 50 mm, résultant en un système de vision à large ligne de base, compte tenu de la taille de structures dans une scène qui est imagée au cours d'une endoscopie. 30
3. Le système de vision selon l'une quelconque des Revendications précédentes, où le système d'imagerie comprend un système de caméra qui comprend une première et une deuxième caméras ou une pluralité de caméras secondaires conçues de façon à créer lesdits signaux en sortie de différentes images d'objet de parties de la structure cible ou de l'environnement direct de celle-ci en fonction d'une imagerie de large ligne de base à points de vue multiples, et comprend en outre un moyen de commande ou de traitement d'images, couplé en communication avec le circuit d'acquisition d'images configuré de façon à traiter l'objet signaux numérisés reçu, qui ne peut pas être vu par la caméra principale, ce qui n'est pas possible dans des situations de fonctionnement normales avec un système stéréo. 35
4. Le système de vision selon l'une quelconque des Revendications précédentes, comprenant en outre un système de caméra à vues multiples conçu de façon à générer différents points de vue par chacune des caméras ou à fournir plusieurs points de vue de l'objet interne, chacun d'eux par une caméra différente, les caméras possédant un zoom et une orientation différents. 40
5. Le système de vision selon l'une quelconque des 45

- Revendications précédentes, où la première caméra est une caméra principale conçue de façon à créer un objet image de l'objet cible sur la structure interne à actionner et la deuxième caméra ou les deuxièmes caméras est ou sont une caméra secondaire ou des caméras secondaires conçues de façon à fournir une image d'une autre partie de l'objet.
6. Le système de vision selon l'une quelconque des Revendications précédentes, où le moyen de traitement d'images est adapté de façon à trouver les points d'image correspondants entre les images provenant de différentes caméras en fonction d'un système de mise en correspondance à large ligne de base.
7. Le système de vision selon l'une quelconque des Revendications précédentes, où le moyen de traitement d'images contient du code de programme informatique destiné à exécuter une technique clés en main de façon à trouver des zones correspondantes d'images d'objet provenant de caméras distinctes et à diriger les caméras du système d'images vers le volume de travail partagé.
8. Le système de vision selon l'une quelconque des Revendications précédentes, où le moyen de traitement d'images est conçu de façon à transformer la pluralité de flux vidéo des caméras en une image globale à grand angle synthétique en temps réel et à présenter ces données synthétiques à l'utilisateur, et à générer une ou plusieurs images de caméra virtuelles sans avoir à déplacer un composant optique quelconque.
9. Le système de vision selon l'une quelconque des Revendications précédentes, où le moyen de traitement d'images est conçu de façon à extraire des informations 3D à partir d'une pluralité d'images, dont certaines peuvent être obtenues à partir d'une caméra qui n'est pas montée sur l'endoscope.
10. Le système de vision selon l'une quelconque des Revendications précédentes, où le moyen de traitement d'images est conçu de façon à générer des informations 3D en fonction de la projection d'une lumière structurée au travers d'un endoscope monofocal non modifié courant au cours de l'imagerie de la scène par l'intermédiaire d'un réseau de caméras endoscopiques à vues multiples.
11. Le système de vision selon l'une quelconque des Revendications précédentes, où le moyen de traitement d'images est conçu de façon à générer des informations 3D en fonction de la projection d'une lumière structurée au travers d'un endoscope stéréo, au cours de l'imagerie de la scène par l'intermédiaire d'un canal optique de l'endoscope, et une projection par l'intermédiaire de l'autre canal optique.
12. Le système de vision selon l'une quelconque des Revendications précédentes, où le moyen de traitement d'images est conçu de façon à mettre en oeuvre une procédure de reprise après catastrophe ou une procédure de sécurité au moyen du modèle sous-jacent ou d'une image globale synthétique en tant que bonne approximation de l'image réelle.
13. Le système de vision selon l'une quelconque des Revendications précédentes, où le moyen de traitement d'images est conçu de façon à mettre en oeuvre une visualisation en réalité augmentée fusionnant des données vidéo endoscopiques avec des données provenant d'une autre modalité en fonction des données de scène interprétées par le moyen de traitement cognitif.

Fig 1

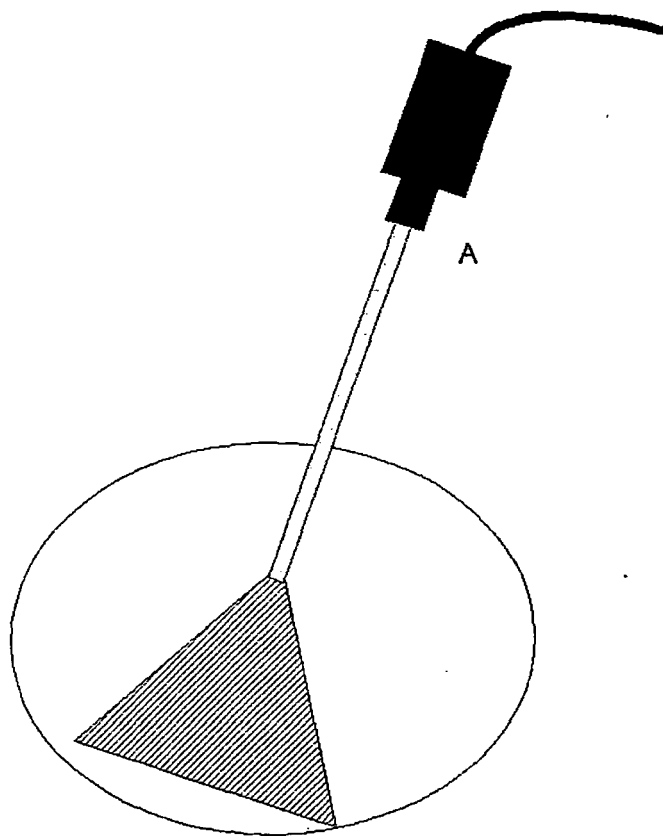


Fig 2

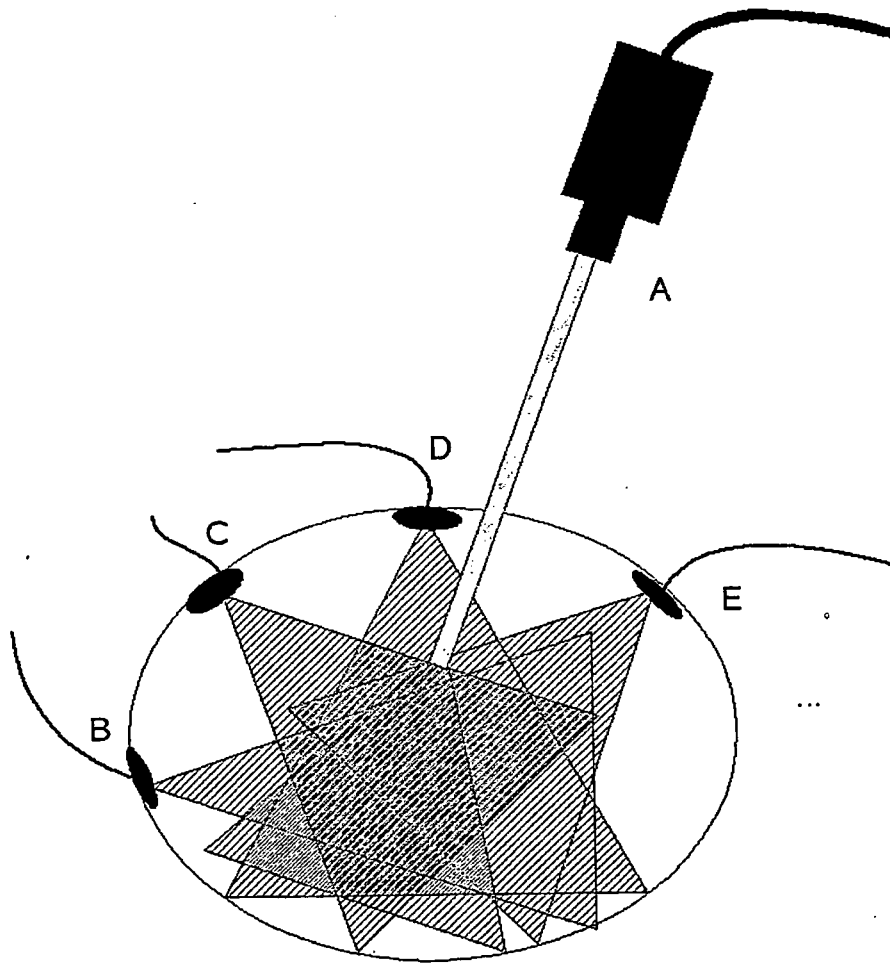


Fig 3

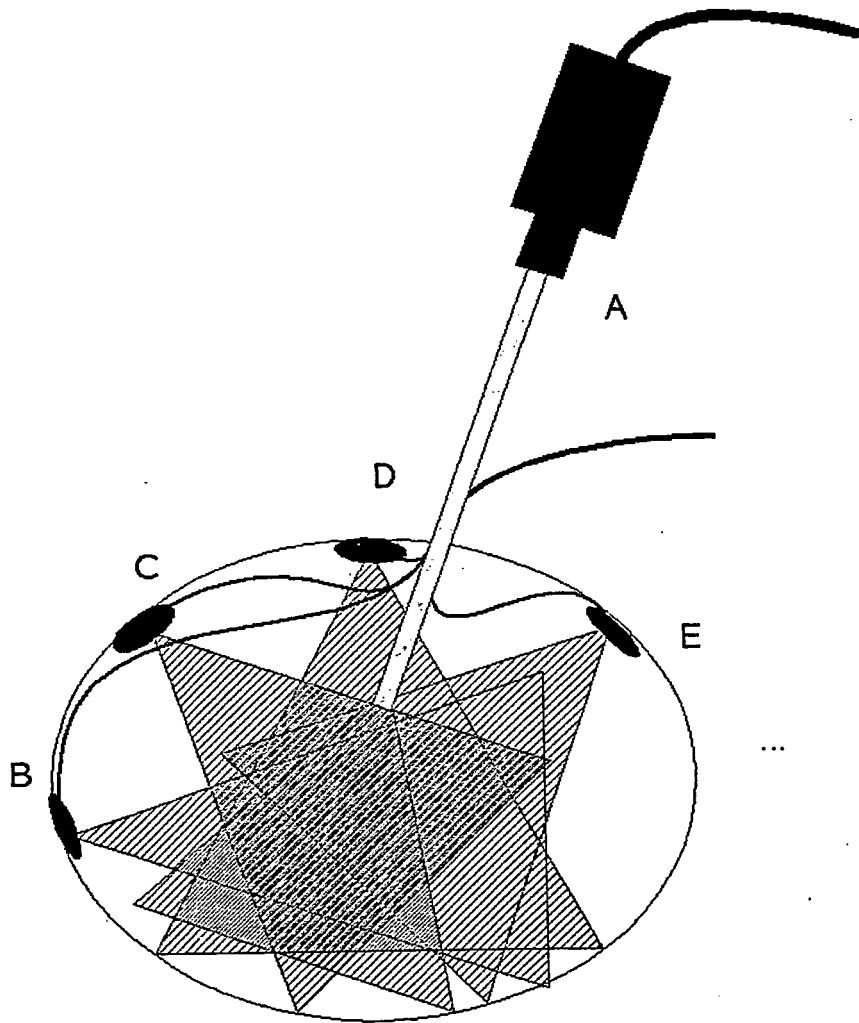


Fig 4

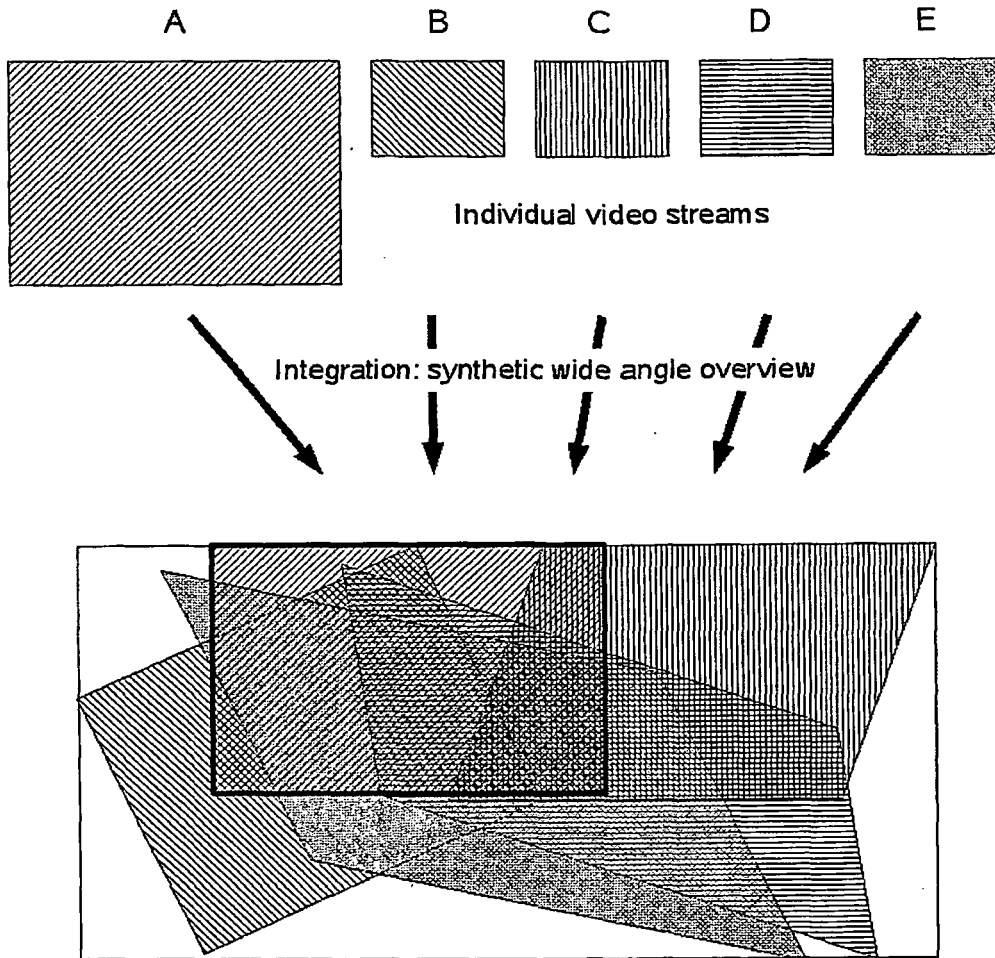


Fig 5


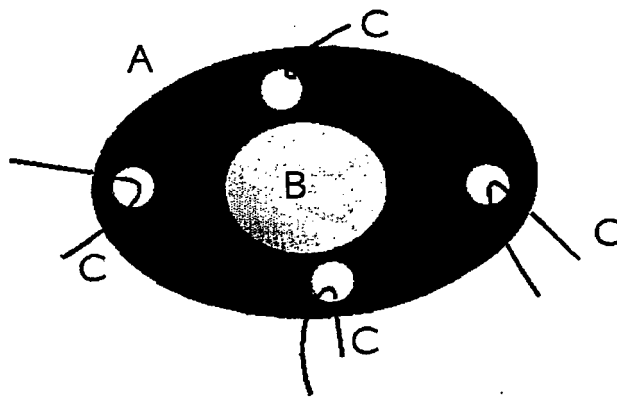


Fig 6

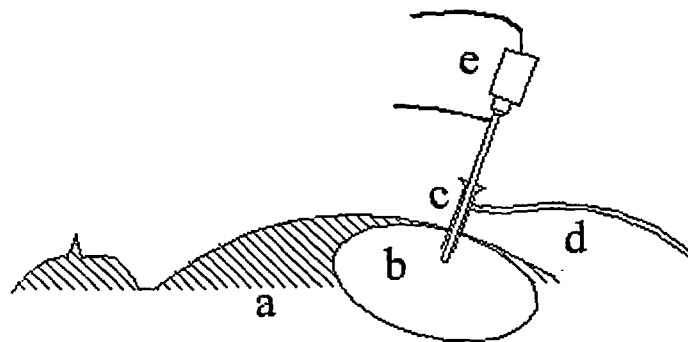

- | | |
|----|-----------------------------|
| a: | patient |
| b: | intra-abdominal cavity |
| c: | trocar |
| d: | insufflation |
| e: | endoscope, camera, lighting |

Fig 7

Initialization multi-view setup


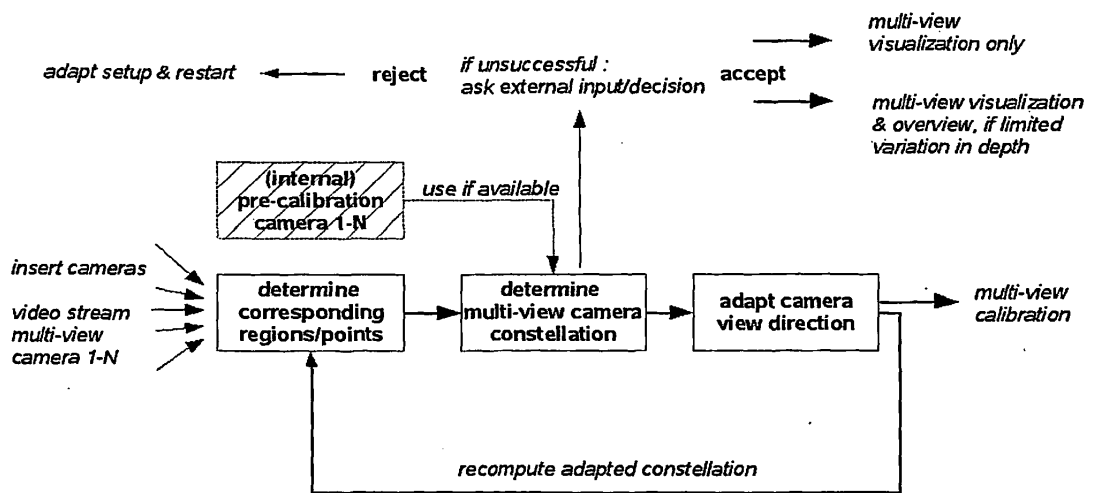


Fig 8

Synthetic overview

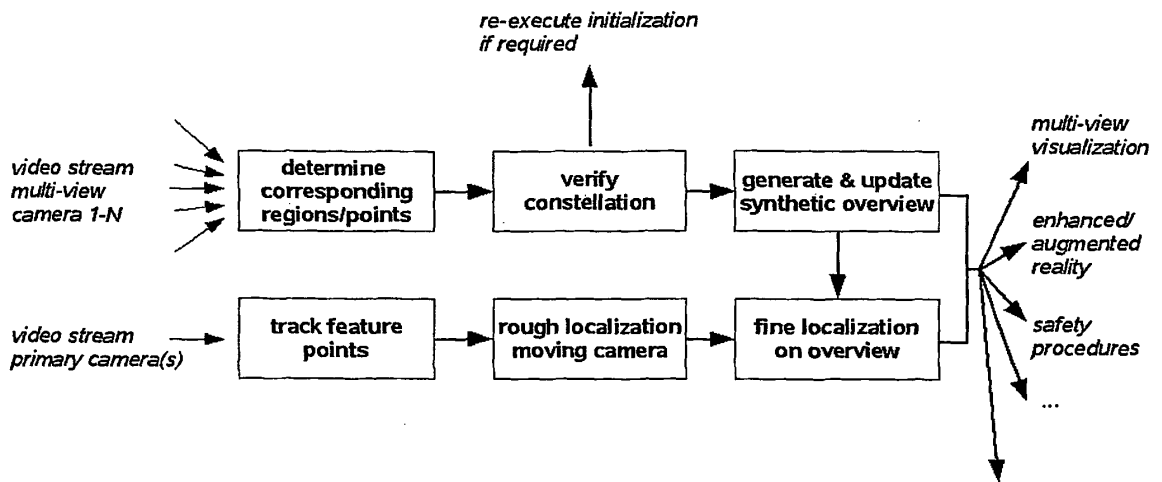

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 5653677 A [0010]
- US 2005234294 A [0010]
- US 2005014994 A [0010]
- US 20050191046 A [0015]
- US 5682199 A [0017]
- US 6494826 B1 [0017]
- US 4697577 A [0017]
- US 5313306 A [0017]
- US 5524180 A [0017]
- US 5776050 A [0017]
- US 5876325 A [0017]
- US 5907664 A [0017]
- US 5954634 A [0017]
- US 6097423 A [0017]
- US 6371909 B [0017]
- US 6428470 B [0017]
- US 20020022767 A [0017]
- US 6503195 B [0019]

Non-patent literature cited in the description

- **ROGER Y. TSAI.** An Efficient and Accurate Camera Calibration Technique for 3D Machine Vision. *Proceedings of IEEE Conference on Computer Vision and Pattern Recognition*, 1986, 364-374 [0036]

专利名称(译)	内窥镜视觉系统		
公开(公告)号	EP2043499B1	公开(公告)日	2015-10-21
申请号	EP2007784896	申请日	2007-07-09
[标]申请(专利权)人(译)	天主教鲁汶大学		
申请(专利权)人(译)	鲁汶大学		
当前申请(专利权)人(译)	鲁汶大学		
[标]发明人	KONINCKX PHILIPPE KONINCKX THOMAS VAN GOOL LUC		
发明人	KONINCKX, PHILIPPE KONINCKX, THOMAS VAN GOOL, LUC		
IPC分类号	A61B1/04		
CPC分类号	A61B1/042 A61B1/0005 A61B1/00181 A61B1/00193 H04N2005/2255		
优先权	2006013576 2006-07-10 GB		
其他公开文献	EP2043499A1		
外部链接	Espacenet		

摘要(译)

本发明涉及一种具有改进的深度感知的新型内窥镜或光学大视野内窥镜系统。具体地，多视点内窥镜系统包括多视点照相机设置和/或智能或认知图像控制系统和显示装置，其特别适用于定位空腔或封闭结构（例如动物体）内的内部结构，例如动物或人的腹部，或用于在概览图像内或概观3D模型上定位这种内部结构的真实或合成图像。

Fig 1

