



(11) **EP 1 479 346 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:  
**10.01.2007 Bulletin 2007/02**

(51) Int Cl.:  
**A61B 17/072 (2006.01)**

(21) Application number: **04252976.8**

(22) Date of filing: **20.05.2004**

(54) **Surgical stapling instrument incorporating keyed firing mechanism**

Chirurgisches Klammersetzgerät mit schlussförmigem Auslösemechanismus

Agrafeuse chirurgicale avec un mécanisme claveté de déclenchement

(84) Designated Contracting States:  
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IT LI LU MC NL PL PT RO SE SI SK TR**

(30) Priority: **20.05.2003 US 443617**

(43) Date of publication of application:  
**24.11.2004 Bulletin 2004/48**

(73) Proprietor: **ETHICON ENDO-SURGERY Cincinnati, Ohio 45242 (US)**

(72) Inventors:  
• **Shelton, Frederick E. IV Hillsboro Ohio 45133 (US)**

- **Setser, Michael E. Burlington Kentucky 41005 (US)**
- **Weisenburgh, William B. Maineville Ohio 45039 (US)**

(74) Representative: **Tunstall, Christopher Stephen et al Carpmaels & Ransford, 43-45 Bloomsbury Square London WC1A 2RA (GB)**

(56) References cited:  
**US-A- 5 465 895 US-A- 6 109 500**

**EP 1 479 346 B1**

Note: Within nine months from the publication of the mention of the grant of the European patent, any person may give notice to the European Patent Office of opposition to the European patent granted. Notice of opposition shall be filed in a written reasoned statement. It shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

## Description

### Cross Reference to Related Applications

**[0001]** The present application is related to four co-pending and commonly-owned applications, these four applications being respectively entitled:

- (1) "SURGICAL STAPLING INSTRUMENT HAVING A SINGLE LOCKOUT MECHANISM" to Frederick E. Shelton IV, Mike Setser, and Bruce Weisenburgh (EP 1479348)
- (2) "SURGICAL STAPLING INSTRUMENT HAVING SEPARATE DISTINCT CLOSING & FIRING SYSTEMS" to Frederick E. Shelton, Mike Setser, and Brian J. Hemmelgam; (EP 1479349)
- (3) "SURGICAL STAPLING INSTRUMENT HAVING A SPENT CARTRIDGE LOCKOUT" to Frederick E. Shelton IV, Mike Setser, Bruce Weisenburgh (EP 1479345); and
- (4) "SURGICAL STAPLING INSTRUMENT HAVING A FIRING LOCKOUT FOR AN UNCLOSED ANVIL" to Frederick E. Shelton IV, Mike Setser, and Bruce Weisenburgh (EP 1479347).

### Field of the Invention

**[0002]** The present invention relates in general to surgical stapler instruments that are capable of applying lines of staples to tissue while cutting the tissue between those staple lines and, more particularly, to improvements relating to stapler instruments and improvements in processes for forming various components of such stapler instruments.

### Background of the Invention

**[0003]** Surgical staplers have been used in the prior art to simultaneously make a longitudinal incision in tissue and apply lines of staples on opposing sides of the incision. Such instruments commonly include a pair of cooperating jaw members that, if the instrument is intended for endoscopic or laparoscopic applications, are capable of passing through a cannula passageway. One of the jaw members receives a staple cartridge having at least two laterally spaced rows of staples. The other jaw member defines an anvil having staple-forming pockets aligned with the rows of staples in the cartridge. The instrument includes a plurality of reciprocating wedges which, when driven distally, pass through openings in the staple cartridge and engage drivers supporting the staples to effect the firing of the staples toward the anvil.

**[0004]** The simultaneous severing of tissue while forming rows of staples on each side of the cut reduces bleeding and simplifies the surgical procedure. However, an appropriate amount of tissue should be clamped between the jaws so that proper staple formation is achieved and so that a cutting member does not bind or otherwise fail

to fully cut the clamped tissue.

**[0005]** A stapling and severing instrument that maintains a maximum jaw spacing is described in U.S. Pat. No. 4,429,695. In particular, a central knife carrier has an upper shoe that enters an upper passageway through an opening when the upper jaw is closed and has a lower shoe that is received within a lower passageway of the lower jaw. Thus, as the knife carrier is advanced distally, the shoes vertically and laterally position the upper and lower jaws. U.S. Pat. No. 4,429,695 teaches that the shoes are attached to the central knife carrier to resist vertical deflection (opening) of the jaws during ejection and forming of staples. As taught, the forces tend to vertically open the jaws during stapling. However, no mention is made of resisting forces that might be applied to vertically close the jaws. Additionally, this reference teaches that the device described therein is assembled from two separate, unconnected elements that are brought together and clamped onto tissue. The two elements form a device suitable only for an open procedure that has no size limitations.

**[0006]** Increasingly, endoscopic and laparoscopic procedures are preferred over open procedures due to their reduced post-operative recovery times and other advantages. Endoscopic stapling and severing instruments use a long slender jaw member that tends to deflect upwardly when clamped onto thick tissues. On thick tissue, this upward deflection of the free (distal) end of the jaw can cause differences in height of the formed staples as the distal gap between the anvil and cartridge is larger than the proximal gap. To ensure more uniform proximal to distal staple formation, the anvil is frequently cambered or bent inwardly toward the staple cartridge. This camber is better for thick tissue and can cause tighter staple forms at the distal end when used on thin tissue. To overcome this tight distal closure, pins or bumps have been added to the clamping surface of the cartridge adjacent to the distal end of the cartridge. The closure of the anvil onto the pin ensures a minimum gap at the distal end. However, surgeons were concerned about the pins or bumps causing tissue trauma. What is needed is a mechanism for maintaining a minimal gap between the anvil and cartridge and a mechanism for maintaining a maximum gap between the anvil and cartridge.

**[0007]** An example of a surgical stapler suitable for endoscopic applications is described in U.S. Pat. No. 5,465,895, which advantageously provides distinct closing and firing actions. Thereby, a clinician is able to close the jaw members upon tissue to position the tissue prior to firing. Once the clinician has determined that the jaw members are properly gripping tissue, the clinician can then fire the surgical stapler, thereby severing and stapling the tissue. The simultaneous severing and stapling avoids complications that may arise when performing such actions sequentially with different surgical tools that respectively only sever or staple.

**[0008]** One specific advantage of being able to close upon tissue before firing is that the clinician is able to

verify via an endoscope that a sufficient amount of tissue has been captured between opposing jaws. Otherwise, opposing jaws may be drawn too close together, especially pinching at their distal ends, and thus not effectively forming closed staples in the severed tissue. Moreover, a firing bar that traverses between opposing jaws to sever the tissue and to drive the wedges that drive the staples may encounter resistance due to the pinched opposing jaws.

[0009] Thus, while such surgical staplers have been a significant advance in surgical procedures, an opportunity has been recognized for enhancing their effectiveness. In particular, it would be desirable to affirmatively maintain proper spacing between the opposing jaws during firing, both opening and closing deflections. In particular, endoscopic devices need to fit into an access device such a trocar, and must maintain a small shaft diameter. To date, no endoscopic stapling device has been provided that has room for a pair for longitudinal passageways for shoes on a cutter that resists both tensile and compressive jaw loadings.

[0010] Furthermore, it is desirable to maintain other advantages of U.S. Pat. No. 5,465,895 to include a wedge sled integral to a staple cartridge, rather than having camming surfaces attached to a cutter. Thereby, fabrication of the cutter is simplified, as is installation of the staple cartridge. Significantly, an integral wedge sled may be designed specifically for each size and application of a staple cartridge, allowing the stapling and severing instrument increased number of uses. In particular, the thickness of the staple cartridge may be based on the desired tissue thickness. Also, the number and spacing of rows of staples may vary.

[0011] US 6,109,500 is considered to represent the closest prior art with respect to the present invention and discloses a surgical device that applies parallel rows of surgical fasteners to body tissue and concomitantly forms an incision between the rows of staples during an endoscopic or laparoscopic surgical procedure.

[0012] This device is generally similar to the device of the present invention, but the anvil slot does not define upper and lower inner surfaces, nor is a middle member disclosed which is slidable against the upper surface of the elongate channel.

[0013] Consequently, a significant need exists for an improved surgical stapling and severing instrument that maintains proper spacing in its end effector to achieve proper stapling of the severed tissue, yet retains the advantages of a staple cartridge having an integral wedge sled.

### **Brief Summary of the Invention**

[0014] The invention overcomes the above-noted and other deficiencies of the prior art by providing a firing mechanism that affirmatively vertically spaces an end effector of a surgical stapling and severing instrument. Thus, the instrument structurally assures adequate spac-

ing to achieve proper stapling, even in instances where too little tissue is clamped in the end effector.

[0015] The present invention provides a surgical instrument as in appended claim 1.

[0016] These and other objects and advantages of the present invention shall be made apparent from the accompanying drawings and the description thereof.

### **Brief Description of the Figures**

[0017] The accompanying drawings, which are incorporated in and constitute a part of this specification, illustrate embodiments of the invention, and, together with the general description of the invention given above, and the detailed description of the embodiments given below, serve to explain the principles of the present invention.

[0018] FIG. 1 depicts a partially cut-away side elevational view of a surgical stapling and severing instrument in an open position.

[0019] FIG. 2 depicts a cross-sectional side elevational detail view along the line 2-2 of FIG. 1 of an end effector of the surgical stapling and severing instrument.

[0020] FIG. 3 depicts an enlarged side elevational view of the firing bar of the surgical stapling and severing instrument of FIG. 2.

[0021] FIG. 4 depicts an enlarged front view of the firing bar of the surgical stapling and severing instrument of FIG. 2.

[0022] FIG. 5 depicts a cross-sectional side elevational detail view of an alternative end effector for the surgical stapling and severing instrument of FIG. 1, incorporating a firing bar that lacks a middle pin for preventing pinching of the end effector.

[0023] FIG. 6 depicts a side elevational view of a handle portion of a proximal end of the surgical stapling and severing instrument of FIG. 1 with a left side removed to expose interior parts in an unclamped, unfired ("start") position.

[0024] FIG. 7 depicts a perspective, exploded view of the handle portion of the proximal end of the surgical stapling and severing instrument of FIG. 1.

[0025] FIG. 8 depicts a side elevational view of the handle portion of the proximal end of the surgical stapling and severing instrument of FIG. 1 with the left side removed to expose interior parts in the closed ("clamped") position.

[0026] FIG. 9 depicts a side elevational view of the handle portion of proximal end of surgical stapling and severing instrument of FIG. 1 with the left side removed to expose interior parts in the stapled and severed ("fired") position.

[0027] FIG. 10 depicts an isometric view of the end effector at the distal end of the surgical stapling and severing instrument of FIG. 1 with the anvil in the up or open position exposing the staple cartridge and cutting edge of the firing bar.

[0028] FIG. 11 depicts an isometric, exploded view of the implement portion of the surgical stapling and sever-

ing instrument of FIG. 1.

[0029] FIG. 12 depicts an isometric view of the end effector at the distal end of the surgical stapling and severing instrument of FIG. 1 with the anvil in the up or open position with the cartridge largely removed exposing a single staple driver and a double staple driver as exemplary and the wedge sled in its start position against a middle pin of the firing bar.

[0030] FIG. 13 depicts an isometric view of the distal end of the surgical stapling and severing instrument of FIG. 1 with the anvil in the up or open position with the staple cartridge completely removed and a portion of an elongate channel removed to expose a lowermost pin of the firing bar.

[0031] FIG. 14 depicts a side elevation view in section showing a mechanical relationship between the anvil, elongate channel, and staple cartridge in the closed position of the surgical stapling and severing instrument of FIG. 1, the section generally taken along lines 14-14 of FIG. 10 to expose wedge sled, staple drivers and staples but also depicting the firing bar along the longitudinal centerline.

[0032] FIG. 15 depicts a section view of the end effector of the surgical stapling and severing instrument with the cartridge and firing bar in the start position taken along line 15-15 of FIG. 10.

[0033] FIG. 16 depicts a section view taken along line 16-16 of Fig. 15 showing the cross-sectional relationship between the firing bar, elongate channel, wedge sled, staple drivers, staples and staple cartridge.

[0034] FIG. 17 depicts a side elevation section view of the surgical stapling and severing instrument of FIG. 1 taken along the longitudinal centerline of the end effector in a partially closed but unclamped position gripping tissue.

[0035] FIG. 18 depicts a partially cut-away side elevational view of the surgical stapling and severing instrument of FIG. 1 in the closed or clamped position.

[0036] FIG. 19 depicts a side elevation view in centerline section of the distal end of the surgical stapling and severing instrument of FIG. 1 in the closed or clamped position with tissue properly compressed.

[0037] FIG. 20 depicts a partially cut-away side elevation view of the surgical stapling and severing instrument of FIG. 1 in a partially fired position.

[0038] FIG. 21 depicts a view in centerline section of the distal end of the surgical stapling and severing instrument of FIG. 1 in a partially fired position.

[0039] FIG. 22 depicts a partially cut-away side elevation view of the surgical stapling and severing instrument of FIG. 1 in a fully fired position.

[0040] FIG. 23 depicts a view in centerline section of the distal end of the surgical stapling and severing instrument of FIG. 1 in a fully fired position.

### Detailed Description of the Invention

[0041] Turning to the Drawings, wherein like numerals

denote like components throughout the several views, FIG. 1 and 2 depict a surgical stapling and severing instrument 10 that is capable of practicing the unique benefits of the present invention. The surgical stapling and severing instrument 10 incorporates an end effector 12 having an E-beam firing mechanism ("firing bar") 14 that advantageously controls the spacing of the end effector 12. In particular, an elongate channel 16 and a pivotally translatable anvil 18 are maintained at a spacing that assures effective stapling and severing. The problems are avoided associated with varying amounts of tissue being captured in the end effector 12.

[0042] The surgical and stapling and severing instrument 10 includes a handle portion 20 connected to an implement portion 22, the latter further comprising a shaft 23 distally terminating in the end effector 12. The handle portion 20 includes a pistol grip 24 toward which a closure trigger 26 is pivotally drawn by the clinician to cause clamping, or closing, of the anvil 18 toward the elongate channel 16 of the end effector 12. A firing trigger 28 is farther outboard of the closure trigger 26 and is pivotally drawn by the clinician to cause the stapling and severing of clamped tissue in the end effector 12.

[0043] It will be appreciated that the terms "proximal" and "distal" are used herein with reference to a clinician gripping a handle of an instrument. Thus, the end effector 12 is distal with respect to the more proximal handle portion 20. It will be further appreciated that for convenience and clarity, spatial terms such as "vertical" and "horizontal" are used herein with respect to the drawings. However, surgical instruments are used in many orientations and positions, and these terms are not intended to be limiting and absolute.

[0044] Closure trigger 26 is actuated first. Once the clinician is satisfied with the positioning of the end effector 12, the clinician may draw back the closure trigger 26 to its fully closed, locked position proximate to the pistol grip 24. Then, the firing trigger 28 is actuated. The firing trigger 28 springedly returns when the clinician removes pressure. A release button 30 when depressed on the proximal end of the handle portion 20 releases any locked closure trigger 26.

[0045] A closure sleeve 32 encloses a frame 34, which in turn encloses a firing drive member 36 that is positioned by the firing trigger 28. The frame 34 connects the handle portion 20 to the end effector 12. With the closure sleeve 32 withdrawn proximally by the closure trigger 26 as depicted, the anvil 18 springedly opens, pivoting away from the elongate channel 16 and translating proximally with the closure sleeve 32.

[0046] The elongate channel 16 receives a staple cartridge 37 that is responsive to the firing bar 14 to drive staples into forming contact with the anvil 18. It will be appreciated that although a readily replaceable staple cartridge 37 is advantageously described herein, a staple cartridge 37 consistent with aspects of the present invention may be permanently affixed or integral to the elongate channel 16, for instance when a larger portion of

the end effector 12 is replaced after each firing.

**[0047] E-BEAM FIRING MECHANISM**

**[0048]** Of particular relevance to the presently claimed invention and with particular reference to FIGS. 2-4, the firing bar 14 includes three vertically spaced pins that control the spacing of the end effector 12 during firing. In particular, an upper pin 38 is staged to enter an anvil pocket 40 near the pivot between the anvil 18 and elongate channel 16. When fired with the anvil 18 closed, the upper pin 38 advances distally within a longitudinal anvil slot 42 extending distally through anvil 18. Any minor upward deflection in the anvil 18 is overcome by a downward force imparted by the upper pin 38.

**[0049]** Firing bar 14 also includes a lower most pin, or firing bar cap, 44 that upwardly engages the elongate channel 16, adjacent a channel slot 45 thereby cooperating with the upper pin 38 to draw the anvil 18 and the elongate channel 16 slightly closer together in the event of excess tissue clamped therebetween.

**[0050]** The firing bar 14 advantageously includes a middle pin 46 that passes through a firing drive slot 47 formed in a lower surface of the cartridge 37 and an upward surface of the elongate channel 16, thereby driving the staples therein as described below. The middle pin 46, by sliding against the elongate channel 16, advantageously resists any tendency for the end effector 12 to be pinched shut at its distal end. To illustrate an advantage of the middle pin 46, FIG. 5 depicts an alternative end effector 12' that lacks a middle pin on a firing bar 14'. In this depiction, the end effector 12' is allowed to pinch shut at its distal end, which tends to impair desired staple formation.

**[0051]** Returning to FIGS. 2-4, a distally presented cutting edge 48 between the upper and middle pins 38, 46 on the firing bar 14 traverses through a proximally presented, vertical slot 49 in the cartridge 37 to sever clamped tissue. The affirmative positioning of the firing bar 14 with regard to the elongate channel 16 and anvil 18 assure that an effective cut is performed:

**[0052] CAMBERED ANVIL WITH SELECTED CARTRIDGE GAP**

**[0053]** The affirmative vertical spacing provided by the E-Beam firing bar 14 is suitable for the limited size available for endoscopic devices. Moreover, the E-Beam firing bar 14 enables fabrication of an anvil 16 with a camber imparting a vertical deflection at its distal end, similar to the position depicted in FIG. 5. This cambered anvil 16 advantageously assists in achieving the desired gap in the end effector 12 even with an anvil 16 reduced thickness, which is thus more suited to the size limitations of an endoscopic device.

**[0054]** The E-Beam firing bar 14 further enables increased applications, especially in combination with a range of configurations of staple cartridges. For instance, a clinician may select a gray staple cartridge yielding a 0.02 mm tissue gap, a white staple cartridge yielding a 0.04 mm tissue gap, a blue cartridge yielding a 0.06 mm tissue gap, or a green cartridge yielding a 0.10 mm tissue

gap. The vertical height of each respective staple cartridge in combination with the length of staples and an integral wedge sled (described in more detail below) pre-determines this desired tissue thickness with the anvil 18 appropriately vertically spaced by the E-Beam firing bar 14.

**[0055] TWO-AXIS HANDLE**

**[0056]** With reference to FIGS. 6-9, the handle portion 20 is comprised of first and second base sections 50 and 52, which are molded from a polymeric material such as a glass-filled polycarbonate. The first base section 50 is provided with a plurality of cylindrical-shaped pins 54. The second base section 52 includes a plurality of extending members 56, each having a hexagonal-shaped opening 58. The cylindrical-shaped pins 54 are received within the hexagonal-shaped openings 58 and are frictionally held therein for maintaining the first and second base sections 50 and 52 in assembly.

**[0057]** A rotating knob 60 has a bore 62 extending completely through it for engaging and rotating the implement portion 22 about its longitudinal axis. The rotating knob 60 includes an inwardly protruding boss 64 extending along at least a portion of the bore 62. The protruding boss 64 is received within a longitudinal slot 66 formed at a proximal portion of the closure sleeve 32 such that rotation of the rotating knob 60 effects rotation of the closure sleeve 32. It will be appreciated that the boss 64 further extends through frame 34 and into contact with a portion of the firing drive member 36 to effect their rotation as well. Thus, the end effector 12 (not shown in FIGS. 6-9) rotates with the rotating knob 60.

**[0058]** A proximal end 68 of the frame 34 passes proximally through the rotating knob 60 and is provided with a circumferential notch 70 that is engaged by opposing channel securement members 72 extending respectively from the base sections 50 and 52. Only the channel securement member 72 of the second base section 52 is shown. The channel securement members 72 extending from the base sections 50, 52 serve to secure the frame 34 to the handle portion 20 such that the frame 34 does not move longitudinally relative to the handle portion 20.

**[0059]** The closure trigger 26 has a handle section 74, a gear segment section 76, and an intermediate section 78. A bore 80 extends through the intermediate section 78. A cylindrical support member 82 extending from the second base section 52 passes through the bore 80 for pivotably mounting the closure trigger 26 on the handle portion 20. A second cylindrical support member 83 extending from the second base section 52 passes through a bore 81 of firing trigger 28 for pivotally mounting on the handle portion 20. A hexagonal opening 84 is provided in the cylindrical support member 83 for receiving a securement pin (not shown) extending from the first base section 50.

**[0060]** A closure yoke 86 is housed within the handle portion 20 for reciprocating movement therein and serves to transfer motion from the closure trigger 26 to the closure sleeve 32. Support members 88 extending from the

second base section 52 and securement member 72, which extends through a recess 89 in the yoke 86, support the yoke 86 within the handle portion 20.

**[0061]** A proximal end 90 of the closure sleeve 32 is provided with a flange 92 that is snap-fitted into a receiving recess 94 formed in a distal end 96 of the yoke 86. A proximal end 98 of the yoke 86 has a gear rack 100 that is engaged by the gear segment section 76 of the closure trigger 26. When the closure trigger 26 is moved toward the pistol grip 24 of the handle portion 20, the yoke 86 and, hence, the closure sleeve 32 move distally, compressing a spring 102 that biases the yoke 86 proximally. Distal movement of the closure sleeve 32 effects pivotal translation movement of the anvil 18 distally and toward the elongate channel 16 of the end effector 12 and proximal movement effects closing, as discussed below.

**[0062]** The closure trigger 26 is forward biased to an open position by a front surface 130 interacting with an engaging surface 128 of the firing trigger 28. Clamp first hook 104 that pivots top to rear in the handle portion 20 about a pin 106 restrains movement of the firing trigger 28 toward the pistol grip 24 until the closure trigger 26 is clamped to its closed position. Hook 104 restrains firing trigger 28 motion by engaging a lockout pin 107 in firing trigger 28. The hook 104 is also in contact with the closure trigger 26. In particular, a forward projection 108 of the hook 104 engages a member 110 on the intermediate section 78 of the closure trigger 26, the member 110 being outward of the bore 80 toward the handle section 74. Hook 104 is biased toward contact with member 110 of the closure trigger 26 and engagement with lockout pin 107 in firing trigger 28 by a release spring 112. As the closure trigger 26 is depressed, the hook 104 is moved top to rear, compressing the release spring 112 that is captured between a rearward projection 114 on the hook 104 and a forward projection 116 on the release button 30.

**[0063]** As the yoke 86 moves distally in response to proximal movement of the closure trigger 26, an upper latch arm 118 of the release button 30 moves along an upper surface 120 on the yoke 86 until dropping into an upwardly presented recess 122 in a proximal, lower portion of the yoke 86. The release spring 112 urges the release button 30 outward, which pivots the upper latch arm 118 downwardly into engagement with the upwardly presented recess 122, thereby locking the closure trigger 26 in a tissue clamping position, such as depicted in FIG. 8.

**[0064]** The latch arm 118 can be moved out of the recess 122 to release the anvil 18 by pushing the release button 30 inward. Specifically, the upper latch arm 118 pivots upward about pin 123 of the second base section 52. The yoke 86 is then permitted to move proximally in response to return movement of the closure trigger 26.

**[0065]** A firing trigger return spring 124 is located within the handle portion 20 with one end attached to pin 106 of the second base section 52 and the other end attached

to a pin 126 on the firing trigger 28. The firing return spring 124 applies a return force to the pin 126 for biasing the firing trigger 28 in a direction away from the pistol grip 24 of the handle portion 20. The closure trigger 26 is also biased away from pistol grip 24 by engaging surface 128 of firing trigger 28 biasing front surface 130 of closure trigger 26.

**[0066]** As the closure trigger 26 is moved toward the pistol grip 24, its front surface 130 engages with the engaging surface 128 on the firing trigger 28 causing the firing trigger 28 to move to its "firing" position. When in its firing position, the firing trigger 28 is located at an angle of approximately 45° to the pistol grip 24. After staple firing, the spring 124 causes the firing trigger 28 to return to its initial position. During the return movement of the firing trigger 28, its engaging surface 128 pushes against the front surface 130 of the closure trigger 26 causing the closure trigger 26 to return to its initial position. A stop member 132 extends from the second base section 52 to prevent the closure trigger 26 from rotating beyond its initial position.

**[0067]** The surgical stapling and severing instrument 10 additionally includes a reciprocating section 134, a multiplier 136 and a drive member 138. The reciprocating section 134 comprises a wedge sled in the implement portion 22 (not shown in FIG. 6-9) and a metal drive rod 140.

**[0068]** The drive member 138 includes first and second gear racks 141 and 142. A first notch 144 is provided on the drive member 138 intermediate the first and second gear racks 141, 142. During return movement of the firing trigger 28, a tooth 146 on the firing trigger 28 engages with the first notch 144 for returning the drive member 138 to its initial position after staple firing. A second notch 148 is located at a proximal end of the metal drive rod 140 for locking the metal drive rod 140 to the upper latch arm 118 of the release button 30 in its unfired position.

**[0069]** The multiplier 136 comprises first and second integral pinion gears 150 and 152. The first integral pinion gear 150 is engaged with a first gear rack 154 provided on the metal drive rod 140. The second integral pinion gear 152 is engaged with the first gear rack 141 on the drive member 138. The first integral pinion gear 150 has a first diameter and the second integral pinion gear 152 has a second diameter which is smaller than the first diameter.

**[0070]** FIGS. 6, 8 and 9 depict respectively the handle portion 20 in the start position (open and unfired), a clamped position (closed and unfired) and a fired position. The firing trigger 28 is provided with a gear segment section 156. The gear segment section 156 engages with the second gear rack 142 on the drive member 138 such that motion of the firing trigger 28 causes the drive member 138 to move back and forth between a first drive position, shown in FIG. 8, and a second drive position, shown in FIG. 9. In order to prevent staple firing before tissue clamping has occurred, the upper latch arm 118 on the release button 30 is engaged with the second

notch 148 on the drive member 138 such that the metal drive rod 140 is locked in its proximal-most position, as depicted in FIG. 6. When the upper latch arm 118 falls into the recess 122, the upper latch arm 118 disengages with the second notch 148 to permit distal movement of the metal drive rod 140, as depicted in FIG. 9.

**[0071]** Because the first gear rack 141 on the drive member 138 and the gear rack 154 on the metal drive rod 140 are engaged with the multiplier 136, movement of the firing trigger 28 causes the metal drive rod 140 to reciprocate between a first reciprocating position, shown in FIG. 8, and a second reciprocating position, shown in FIG. 9. Since the diameter of the first pinion gear 150 is greater than the diameter of the second pinion gear 152, the multiplier 136 moves the reciprocating section 134 a greater distance than the drive member 138 is moved by the firing trigger 28. The diameters of the first and second pinion gears 150 and 152 may be changed to permit the length of the stroke of the firing trigger 28 and the force required to move it to be varied.

**[0072]** It will be appreciated that the handle portion 20 is illustrative and that other actuation mechanisms may be employed. For instance, the closing and firing motions may be generated by automated means.

#### **[0073] SEPARATE AND DISTINCT CLOSING AND FIRING END EFFECTOR**

**[0074]** The end effector 12 of the surgical stapling and severing instrument 10 is depicted in further detail in FIGS. 10-16. As described above, the handle portion 20 produces separate and distinct closing and firing motions that actuate the end effector 12. The end effector 12 advantageously maintains the clinical flexibility of this separate and distinct closing and firing (i.e., stapling and severing). In addition, the end effector 12 introduces the aforementioned ability to affirmatively maintain the closed spacing during firing after the clinician positions and clamps the tissue. Both features procedurally and structurally enhance the ability of the surgical stapling and severing instrument 10 by ensuring adequate spacing for instances where an otherwise inadequate amount of tissue is clamped and to enhance the clamping in instances where an otherwise excessive amount of tissue has been clamped.

**[0075]** FIG. 10 depicts the end effector 12, which is in an open position by a retracted closure sleeve 32, with a staple cartridge 37 installed in the elongate channel 16. On a lower surface 200 of the anvil 18, a plurality of stapling forming pockets 202 are arrayed to correspond to a plurality of stapler apertures 204 in an upper surface 206 of the staple cartridge 37. The firing bar 14 is at its proximal position, with the upper pin 38 aligned in a non-interfering fashion with the anvil pocket 40. The anvil pocket 40 is shown as communicating with the longitudinal anvil slot 42 in the anvil 18. The distally presented cutting edge 48 of the firing bar 14 is aligned with and proximally from removed from the vertical slot 49 in the staple cartridge 37, thereby allowing removal of a spent cartridge and insertion of an unfired cartridge, which is

snapfit into the elongate channel 16. Specifically, extension features 208, 210 of the staple cartridge 37 engage recesses 212, 214 (shown in FIG. 12) of the elongate channel 16.

**[0076]** FIG. 11 shows the implement portion 22 of the surgical stapling and severing instrument 10 in disassembled form. The staple cartridge 37 is shown as being comprised of a cartridge body 216, a wedge sled 218, single and double drivers 220, staples 222, and a cartridge tray 224. When assembled, the cartridge tray 224 holds the wedge sled 218, single and double drivers 220, and staples 222 inside the cartridge body 216.

**[0077]** Having a wedge sled 218 integral to the staple cartridge 37 enables a number of flexible design options as compared to incorporating camming surfaces onto a firing bar itself. For instance, a number of different staple cartridges may be selected for use in the instrument 10 with each staple cartridge having a different configuration of rows of staples, each thus having a unique wedge sled configured to contact the middle pin 46 of the firing bar 14 while causing the driving of the staples 222. As another example, the integral wedge sled 218 provides an opportunity for a number of lockout features, described in greater detail in the first and third aforementioned co-pending applications.

**[0078]** The elongate channel 16 has a proximally placed attachment cavity 226 that receives a channel anchoring member 228 on the distal end of the frame 34 for attaching the end effector 12 to the handle portion 20. The elongate channel 16 also has an anvil cam slot 230 that pivotally receives an anvil pivot 232 of the anvil 18. The closure sleeve 32 that encompasses the frame 34 includes a distally presented tab 234 that engages an anvil feature 236 proximate but distal to the anvil pivot 232 on the anvil 18 to thereby effect opening and closing of the anvil 18. The firing drive member 36 is shown as being assembled from the firing bar 14 attached to a firing connector 238 by pins 240, which in turn is rotatably and proximally attached to the metal drive rod 140. The firing bar 14 is guided at a distal end of the frame by a slotted guide 239 inserted therein.

**[0079]** With particular reference to FIG. 12, a portion of the staple cartridge 37 is removed to expose portions of the elongate channel 16, such as recesses 212, 214 and to expose some components of the staple cartridge 37 in their unfired position. In particular, the cartridge body 216 (shown in FIG. 11) has been removed. The wedge sled 218 is shown at its proximal, unfired position with a pusher block 242 contacting the middle pin 46 (not shown in FIG. 12) of the firing bar 14. The wedge sled 218 is in longitudinal sliding contact upon the cartridge tray 224 and includes wedges 228 that force upward the single and double drivers 220 as the wedge sled 218 moves distally. Staples 222 (not shown in FIG. 12) resting upon the drivers 220 are thus also forced upward into contact with the anvil forming pockets 202 on the anvil 18 to form closed staples. Also depicted is the channel slot 45 in the elongate channel 16 that is aligned with the

vertical slot 49 in the staple cartridge 37.

**[0080]** FIG. 13 depicts the end effector 12 of FIG. 12 with all of the staple cartridge 37 removed to show the middle pin 46 of the firing bar 14 as well as portion of the elongate channel 16 removed adjacent to the channel slot 45 to expose the firing bar cap 44. In addition, portions of the shaft 23 are removed to expose a proximal portion of the firing bar 14. Projecting downward from the anvil 18 near the pivot, a pair of opposing tissue stops 244 prevent tissue being positioned too far up into the end effector 12 during clamping.

**[0081]** FIG. 14 depicts the end effector 12 closed in a tissue clamping position with the firing bar 14 unfired. The upper pin 38 is in the anvil pocket 40, vertically aligned with the anvil slot 42 for distal longitudinal movement of the firing bar 14 during firing. The middle pin 46 is positioned to push the wedge sled 218 distally so that wedge 228 sequentially contacts and lifts double drivers 220 and the respective staples 222 into forming contact with staple forming pockets 202 in the lower surface 200 of the anvil 18.

**[0082]** FIG. 15 depicts the upper surface 206 of the staple cartridge 37 with the firing bar 14 in its unfired, proximal position. The stapler apertures 204 are arrayed on each side of the vertical slot 49 in the staple cartridge 37.

**[0083]** FIG. 16 depicts the end effector 12 near the pivot showing that the elongate channel 16 has opposing ramp portions 246 to thereby cooperate with the tissue stops 244 of the anvil 18 (not shown in FIG. 16) to prevent tissue from jamming the end effector 12. Also depicted in greater detail are the double drivers 220 and their relation to the staples 222.

#### **[0084] OPERATION**

**[0085]** In use, the surgical stapling and severing instrument 10 is used as depicted in FIGS 1, 2, and 17-23. In FIGS. 1-2, the instrument 10 is in its start position, having had an unfired, fully loaded staple cartridge 37 snap-fitted into the distal end of the elongate channel 16. Both triggers 26, 28 are forward and the end effector 12 is open, such as would be typical after inserting the end effector 12 through a trocar or other opening into a body cavity. The instrument 10 is then manipulated by the clinician such that tissue 248 to be stapled and severed is positioned between the staple cartridge 37 and the anvil 18, as depicted in FIG. 17.

**[0086]** With reference to FIGS. 18-19, next, the clinician moves the closure trigger 26 proximally until positioned directly adjacent to the pistol grip 24, locking the handle portion 20 into the closed and clamped position. The retracted firing bar 14 in the end effector 12 does not impede the selective opening and closing of the end effector 12, but rather resides within the anvil pocket 40. With the anvil 18 closed and clamped, the E-beam firing bar 14 is aligned for firing through the end effector 12. In particular, the upper pin 38 is aligned with the anvil slot 42 and the elongate channel 16 is affirmatively engaged about the channel slot 45 by the middle pin 46 and the

firing bar cap 44.

**[0087]** With reference to FIGS. 20-21, after tissue clamping has occurred, the clinician moves the firing trigger 28 proximally causing the firing bar 14 to move distally into the end effector 12. In particular, the middle pin 46 enters the staple cartridge 37 through the firing drive slot 47 to effect the firing of the staples 222 (not shown in FIGS. 20-21) via wedge sled 218 toward the anvil 18. The lower most pin, or firing bar cap 44, cooperates with the middle pin 46 to slidably position cutting edge 48 of the firing bar 14 to sever tissue. The two pins 44, 46 also position the upper pin 38 of the firing bar 14 within longitudinal anvil slot 42 of the anvil 18, affirmatively maintaining the spacing between the anvil 18 and the elongate channel 16 throughout its distal firing movement.

**[0088]** With reference to FIGS. 22-23, the clinician continues moving the firing trigger 28 until brought proximal to the closure trigger 26 and pistol grip 24. Thereby, all of the ends of the staples 222 are bent over as a result of their engagement with the anvil 18. The firing bar cap 44 is arrested against a firing bar stop 250 projecting toward the distal end of the channel slot 45. The cutting edge 48 has traversed completely through the tissue. The process is complete by releasing the firing trigger 28 and by then depressing the release button 30 while simultaneously squeezing the closure trigger 26 to open the end effector 12.

**[0089]** While the present invention has been illustrated by description of several embodiments and while the illustrative embodiments have been described in considerable detail, it is not the intention of the applicant to restrict or in any way limit the scope of the appended claims to such detail. Additional advantages and modifications may readily appear to those skilled in the art.

**[0090]** For example, the affirmative spacing of the anvil 18 and elongate channel 16 is achieved in part with two pins 44, 46 on the firing bar 14 engaging opposite sides of a channel slot 47 and a single upper pin 38 entrained within an anvil slot 42.

**[0091]** For another example, although the E-beam firing beam 14 has advantages for an endoscopically employed surgical severing and stapling instrument 10, a similar E-Beam may be used in other clinical procedures. It is generally accepted that endoscopic procedures are more common than laparoscopic procedures. Accordingly, the present invention has been discussed in terms of endoscopic procedures and apparatus. However, use herein of terms such as "endoscopic", should not be construed to limit the present invention to a surgical stapling and severing instrument for use only in conjunction with an endoscopic tube (i.e., trocar). On the contrary, it is believed that the present invention may find use in any procedure where access is limited to a small incision, including but not limited to laparoscopic procedures, as well as open procedures.

**[0092]** For yet another example, although an illustrative handle portion 20 described herein is manually operated by a clinician, it is consistent with aspects of the



invention for some or all of the functions of a handle portion to be powered (e.g., pneumatic, hydraulic, electro-mechanical, ultrasonic, etc.). Furthermore, controls of each of these functions may be manually presented on a handle portion or be remotely controlled (e.g., wireless remote, automated remote console, etc.).

## Claims

### 1. A surgical stapling instrument (10) comprising:

a handle portion (20) operable to produce a firing motion;

an implement portion (22) responsive to the firing motions from the handle portion (20), the implement portion (22) comprising:

an elongate channel (16) coupled to the handle portion (20) and including a channel slot (45),

a staple cartridge (37) received by the elongate channel (16) and incorporating a proximally positioned wedge member aligned to cam upward a driver (220) supporting a staple (222),

an anvil (18) pivotally coupled to the elongate channel (16) and including an anvil slot (42) defining upper and lower inner surfaces extending substantially along the longitudinal length of the anvil (18),

a firing device including a distally presented cutting edge (48) longitudinally received between the elongate channel (16) and the anvil (18), an upper member (38) comprised of an upper pin slidably engageable with the upper and lower inner surfaces of the anvil channel (18), a lower member (44) upwardly engagable with the elongate channel (16) adjacent the channel slot (45), and a middle member (46) operable to actuate the staple cartridge (37) by distally translating the wedge member of the staple cartridge (37) and slidable against an upper surface of the elongate channel (16), such that the firing device positively engages both the elongate channel (16) and the anvil (18) during longitudinal firing travel to maintain vertical spacing between the elongate channel (16) and the anvil (18), thus resisting both a pinching together and a forcing apart of the elongate channel (16) and the anvil (18).

### 2. The surgical instrument of claim 1, wherein:

the handle portion is further operable to produce a closing motion;

the implement portion is diametrically dimen-

sioned for endo-surgical use, and the implement portion further comprises:

a shaft coupled to the handle portion operable to separately transfer the firing motion and the closing motion; wherein the elongate channel is coupled to the shaft, and the anvil is responsive to the closing motion from the shaft.

3. The surgical instrument of claim 2, wherein the staple cartridge includes a proximally opened slot for receiving the cutting edge of the firing device, the staple cartridge including a plurality of staples arranged so as to be cammed upwardly by the distal longitudinal movement of the firing mechanism.

4. The surgical instrument of claim 3, wherein the staple cartridge further includes a plurality of drivers supporting the plurality of staples and the wedge member comprises a wedge sled responsive to the distal longitudinal movement of the firing mechanism to cam upwardly the drivers and thus form the plurality of staples against the anvil.

5. The surgical instrument of claim 3, wherein the wedge member comprises a wedge sled (218) having a plurality of connected camming wedges (228) each having a preselected height configured for a selected type of staple cartridge (37), the middle member (46) of the firing device oriented to abut each of the plurality of staple cartridge types.

## Patentansprüche

### 1. Chirurgisches Klammerinstrument (10), enthaltend:

einen Handgriff (20), mit dem eine Feuerbewegung zu erzeugen ist;

einen Werkzeugabschnitt (22), der auf die Feuerbewegungen des Handgriffes (20) anspricht, enthaltend:

einen länglichen Kanal (16), der an den Handgriff (20) gekuppelt ist, und einen Kanalschlitz (45) aufweist,

eine Klammerpatrone (37), die von dem länglichen Kanal (16) aufgenommen ist, und ein proximal angeordnetes Keilteil aufweist, welches so ausgerichtet ist, daß es einen Treiber (220) nach oben drückt, welcher eine Klammer (222) abstützt,

einen Amboß (18), der schwenkbar an den länglichen Kanal (16) gekuppelt ist, und einen Amboßschlitz (42) aufweist, welcher obere und untere Innenseiten bildet, welche sich im wesentlichen entlang der in Längsrichtung gerichteten

- Länge des Amboßes (18) erstrecken, eine Feueleinrichtung mit einer distal angeordneten Schneidkante (48), welche in Längsrichtung zwischen dem länglichen Kanal (16) und dem Amboß (18) aufgenommen ist, einem Oberteil (38), welches einen oberen Stift aufweist, welcher gleitbar mit den oberen und unteren Innenseiten des Amboßkanals (18) in Eingriff zu bringen ist, einem Unterteil (44), welches nach oben mit dem länglichen Kanal (16) benachbart zu dem Kanalschlitz (45) in Eingriff zu bringen ist, und einem Mittelteil (46), mit dem die Klammerpatrone (37) durch distales Übertragen des Keilteils der Klammerpatrone (37) und Gleiten gegen eine Oberseite des länglichen Kanals (16) zu betätigen ist, so daß die Feueleinrichtung während der längsgerichteten Feuerbewegung sowohl mit dem länglichen Kanal (16) als auch mit dem Amboß (18) in Eingriff ist, um einen vertikalen Zwischenraum bzw. Abstand zwischen dem länglichen Kanal (16) und dem Amboß (18) aufrechtzuerhalten, und auf diese Weise sowohl ein Aneinanderschlagen als auch ein Auseinanderbewegen des länglichen Kanals (16) und des Amboßes (18) zu verhindern.
2. Chir urgisches Instrument nach Anspruch 1, wobei:
- der Handgriff weiterhin so zu betätigen ist, daß er eine Schließbewegung erzeugt;  
 der Werkzeugabschnitt diametral für einen endo-chirurgischen Gebrauch dimensioniert ist, und weiterhin aufweist:  
 eine an den Handgriff gekuppelte Welle, mittels welcher die Feuerbewegung und die Schließbewegung separat zu übertragen sind; wobei der längliche Kanal an die Welle gekuppelt ist, und  
 der Amboß auf die Schließbewegung der Welle anspricht.
3. Chir urgisches Instrument nach Anspruch 2, wobei die Klammerpatrone einen proximal offenen Schlitz zur Aufnahme der Schneidkante der Feueleinrichtung aufweist, und wobei die Klammerpatrone eine Mehrzahl von Klammern aufweist, die so angeordnet sind, daß sie durch die distale Längsbewegung der Feueleinrichtung nach oben bewegt werden.
4. Chir urgisches Instrument nach Anspruch 3, wobei die Klammerpatrone weiterhin eine Mehrzahl von Treibern aufweist, welche die Mehrzahl von Klammern abstützt, und das Keilteil einen Keilschlitten aufweist, welcher auf die distale Längsbewegung der Feueleinrichtung anspricht, um die Treiber nach oben zu bewegen, und somit die Mehrzahl von Klammern gegen den Amboß zu bewegen.

5. Chir urgisches Instrument nach Anspruch 3, wobei das Keilteil einen Keilschlitten (218) aufweist, welcher eine Mehrzahl von verbundenen Keilen (228) aufweist, welche jeweils eine vorgewählte Höhe aufweisen, welche für einen ausgewählten Typ einer Klammerpatrone (37) ausgebildet ist, und wobei das Mittelteil (46) der Feueleinrichtung so orientiert ist, daß es an jede der mehreren Typen von Klammerpatronen anschlägt.

## Revendications

1. Instrument d'agrafage chirurgical (10) comprenant:

une partie servant de poignée (20) actionnable de façon à produire un mouvement d'amorçage; une partie d'exécution (22) répondant aux mouvements d'amorçage de la partie servant de poignée (20), la partie d'exécution (22) comprenant :

un canal allongé (16) couplé à la partie servant de poignée (20) et comprenant une fente de canal (45),

une cartouche d'agrafes (37) reçue par le canal allongé (16) et comprenant un élément à clavette placé de façon proximale, aligné de façon à mettre en prise vers le haut, un pilote (220) soutenant une agrafe (222),

une enclume (18) couplée de façon à pivoter, au canal allongé (16) et comprenant une fente d'enclume (42) définissant des surfaces internes supérieure et inférieure s'étendant essentiellement le long de l'axe longitudinal de l'enclume (18),

un dispositif d'amorçage comprenant un bord coupant présenté sur le plan distal (48) reçu longitudinalement entre le canal allongé (16) et l'enclume (18), un élément supérieur (38) constitué d'une broche supérieure en prise de manière à coulisser avec les surfaces intérieures supérieure et inférieure du canal de l'enclume (18), un élément inférieur (44) en prise vers le haut avec le canal allongé (16) adjacent à la fente de canal (45) et un élément médian (46) fonctionnant de manière à actionner la cartouche d'agrafes (37) par translation distale de l'élément à clavette de la cartouche d'agrafes (37) et pouvant coulisser contre une surface supérieure du canal allongé (16) de sorte que le dispositif d'amorçage soit positivement en prise avec à la fois le canal allongé (16) et l'enclume (18) pendant le déplacement d'amorçage longitudinal pour maintenir un espacement vertical entre le canal allongé

- (16) et l'enclume (18), résistant ainsi à la fois à un pincement conjoint et à un forçage séparé du canal allongé (16) et de l'enclume (18). 5
2. Instrument chirurgical selon la revendication 1, dans lequel : 5
- la partie servant de poignée peut en outre être actionnée pour produire un mouvement de fermeture; 10
- la partie d'exécution est diamétralement dimensionnée pour une utilisation endo-chirurgicale et la partie d'exécution comprend en outre : 15
- une tige couplée à la partie servant de poignée, actionnable afin de transférer séparément le mouvement d'amorçage et le mouvement de fermeture; dans lequel 20
- le canal allongé est couplé à la tige, et l'enclume répond au mouvement de fermeture venant de la tige.
3. Instrument chirurgical selon la revendication 2, dans lequel la cartouche d'agrafes comprend une fente ouverte de façon proximale pour recevoir le bord coupant du dispositif d'amorçage, la cartouche d'agrafes comprenant une pluralité d'agrafes disposées de façon à être en prise vers le haut par le mouvement longitudinal distal du mécanisme d'amorçage. 25 30
4. Instrument chirurgical selon la revendication 3, dans lequel la cartouche d'agrafes comprend en outre une pluralité de pilotes soutenant la pluralité d'agrafes et l'élément à clavette comprend un traîneau de clavette répondant au mouvement longitudinal distal du mécanisme d'amorçage pour mettre en prise vers le haut des pilotes et former ainsi la pluralité d'agrafes contre l'enclume. 35 40
5. Instrument chirurgical selon la revendication 3, dans lequel l'élément à clavette comprend un traîneau à clavette (218) présentant une pluralité de clavettes reliées en prise (228), chacune ayant une hauteur présélectionnée, configurée pour un type choisi de cartouche d'agrafes (37) l'élément médian (46) du dispositif d'amorçage étant orienté de façon à mettre bout à bout chacun des multiples types de cartouches d'agrafes. 45 50

55

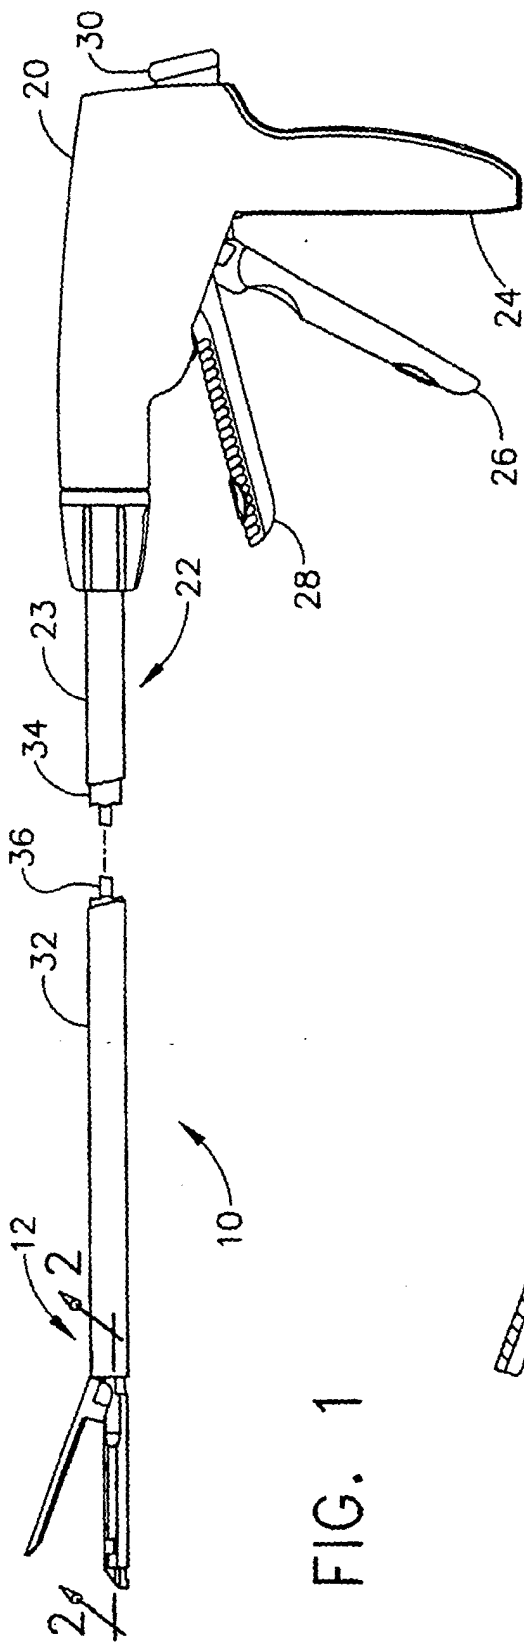


FIG. 1

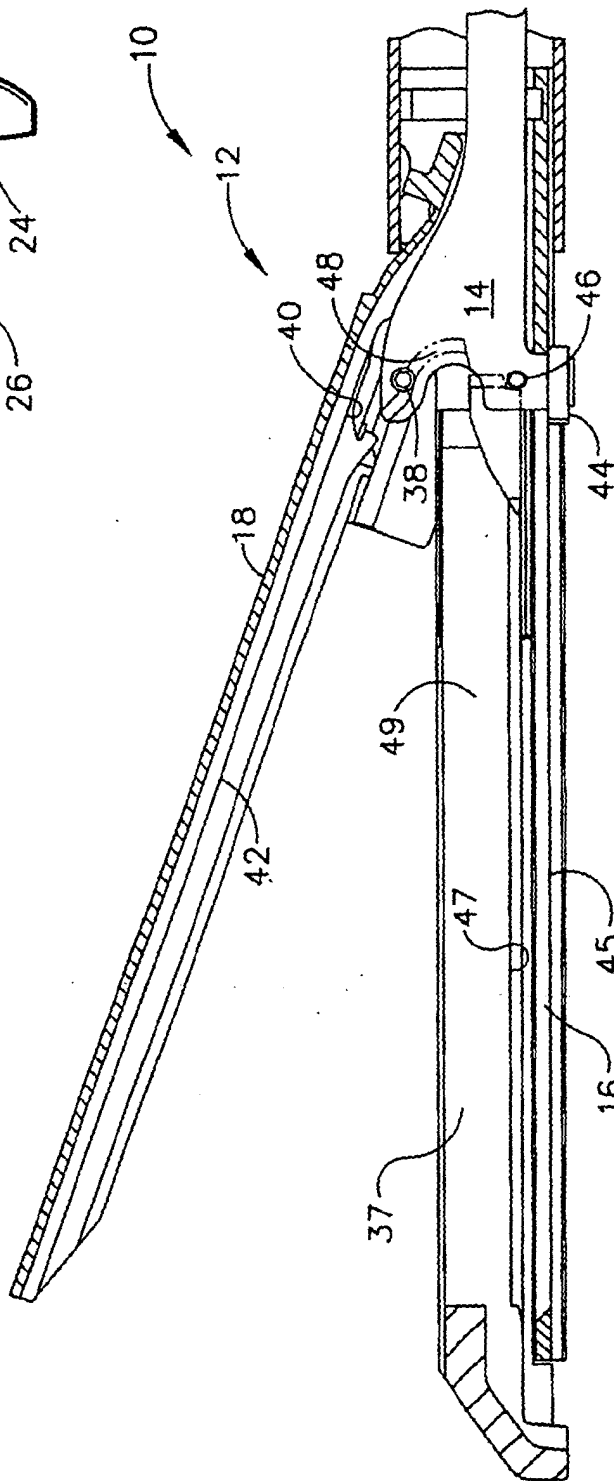
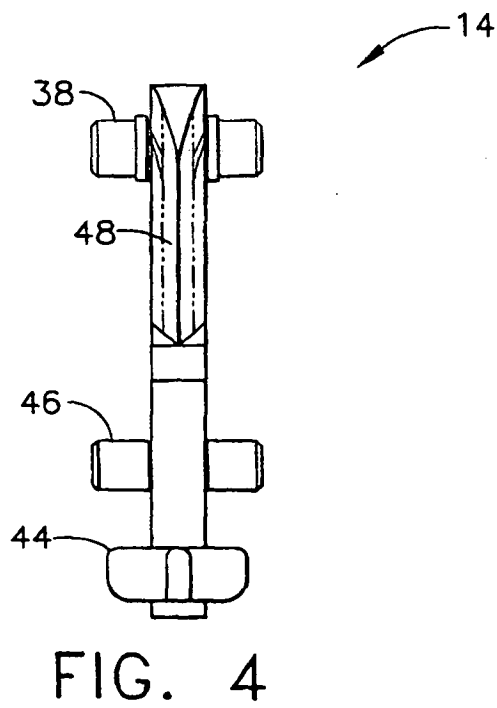
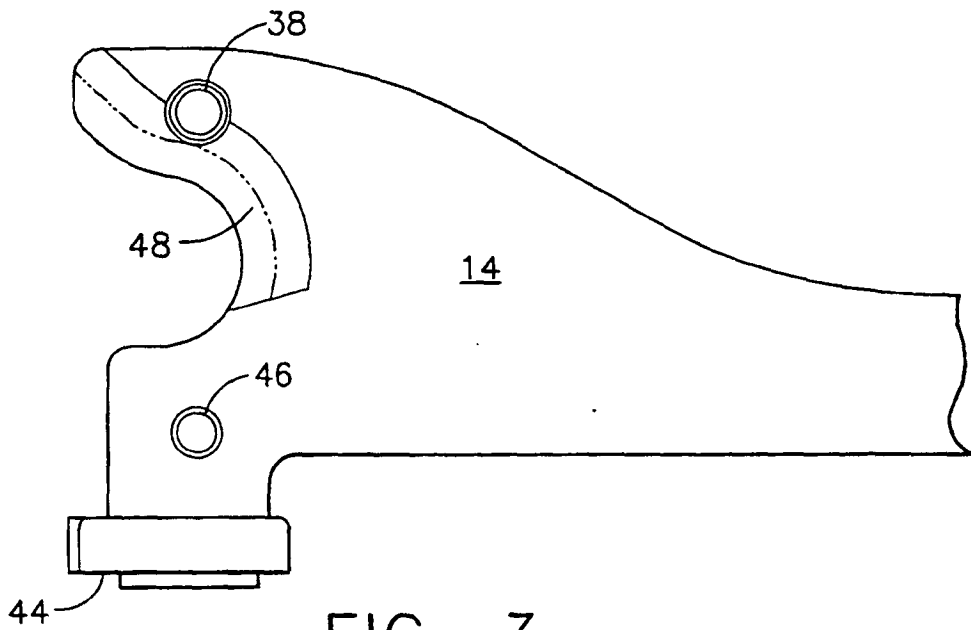


FIG. 2



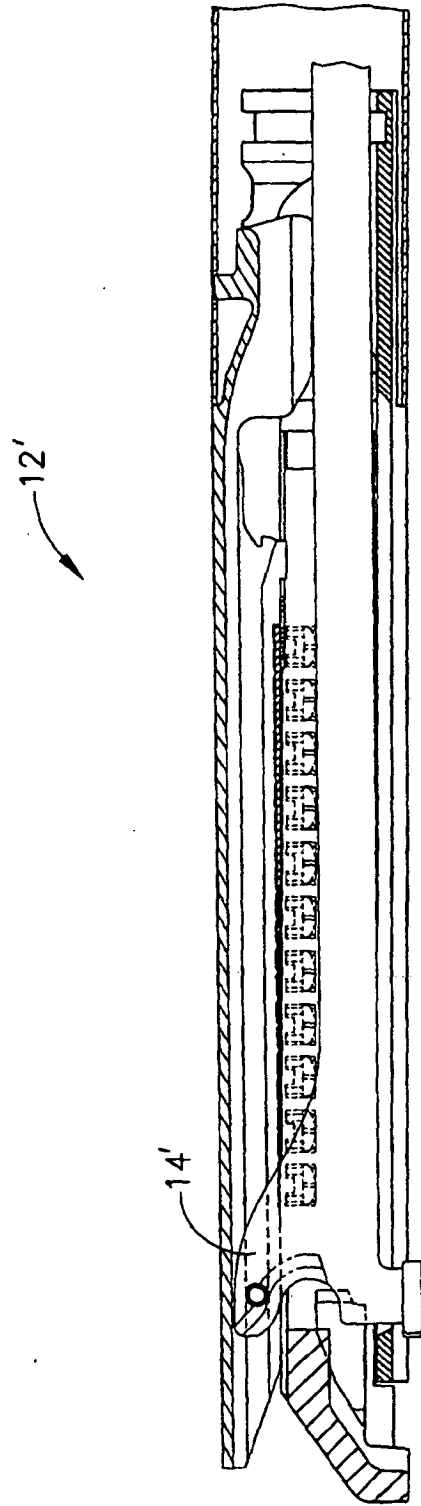


FIG. 5

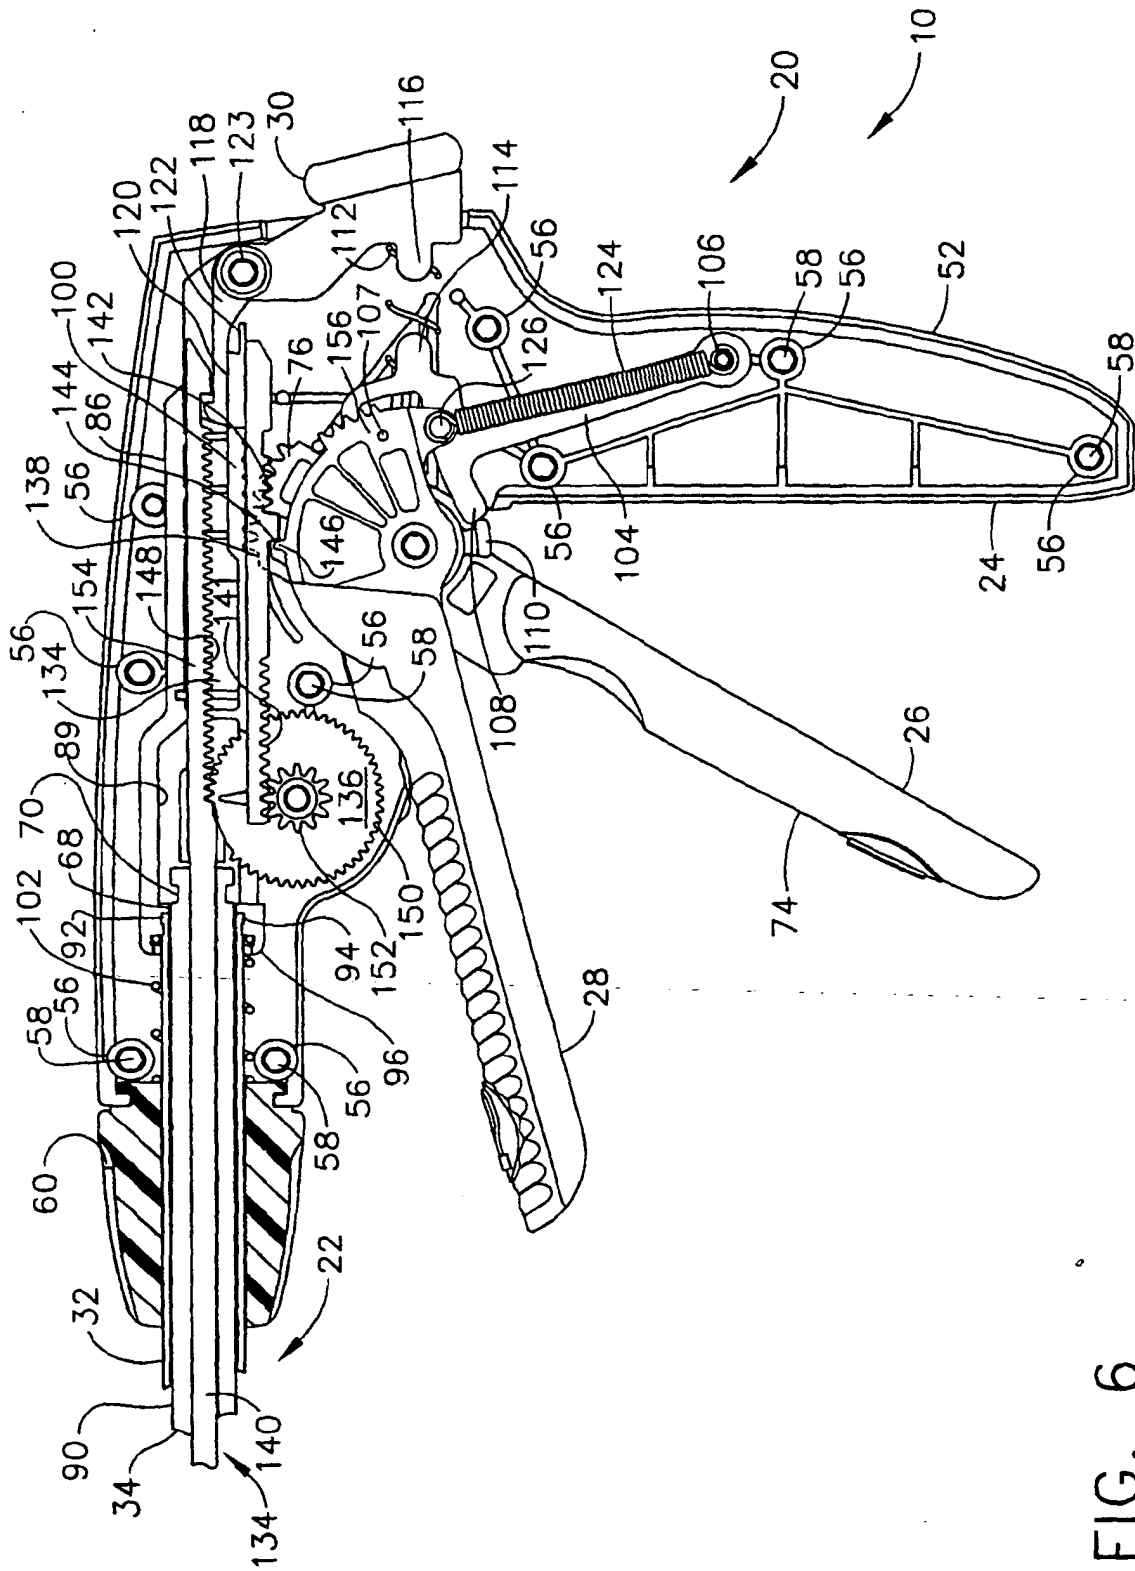


FIG. 6

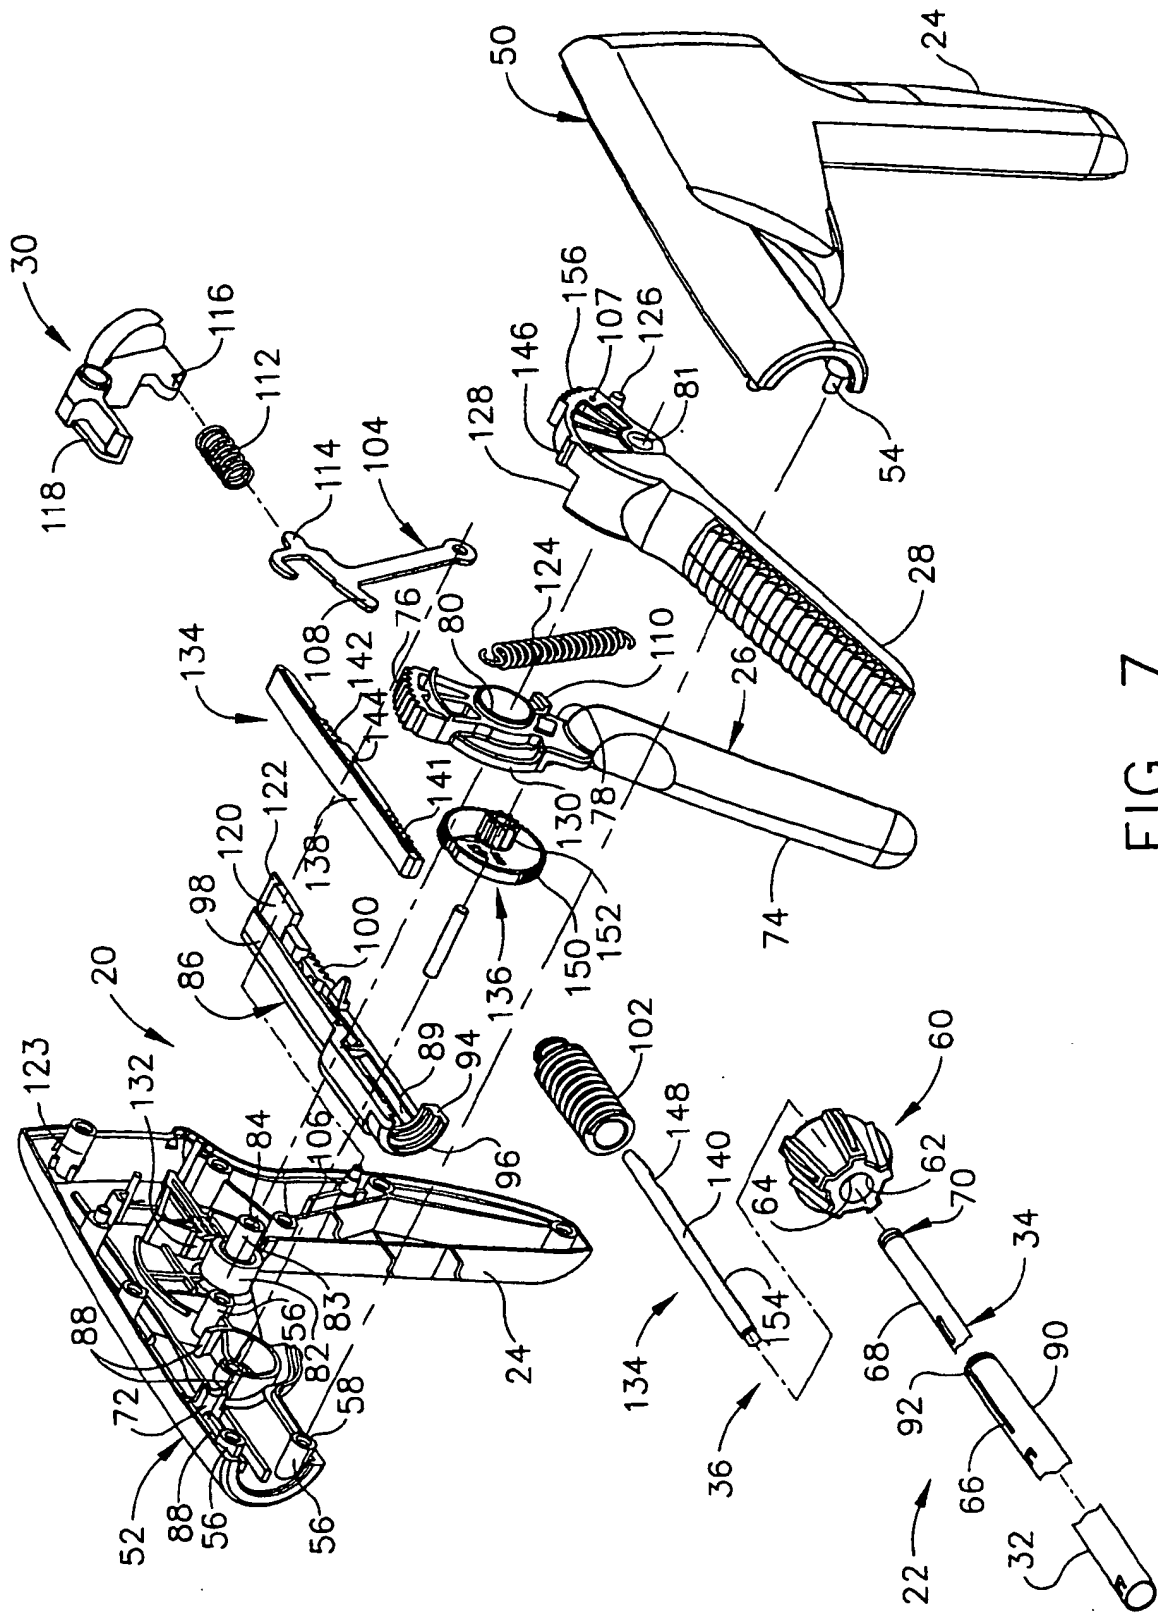


FIG. 7



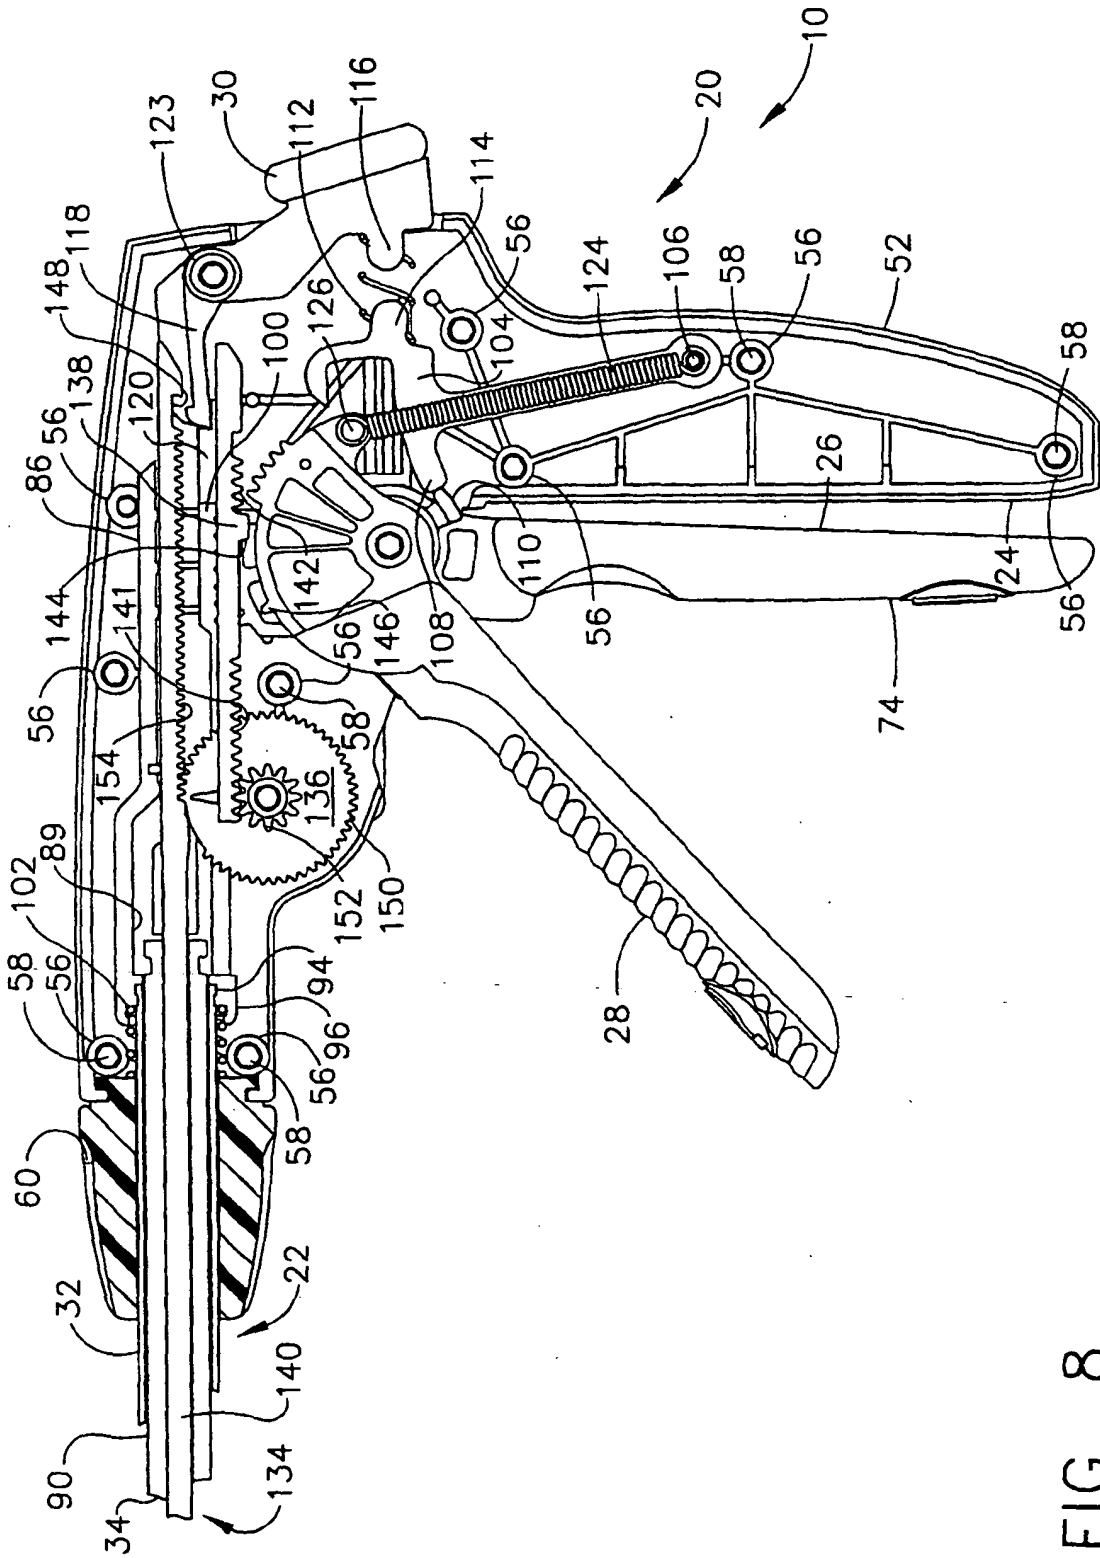


FIG. 8

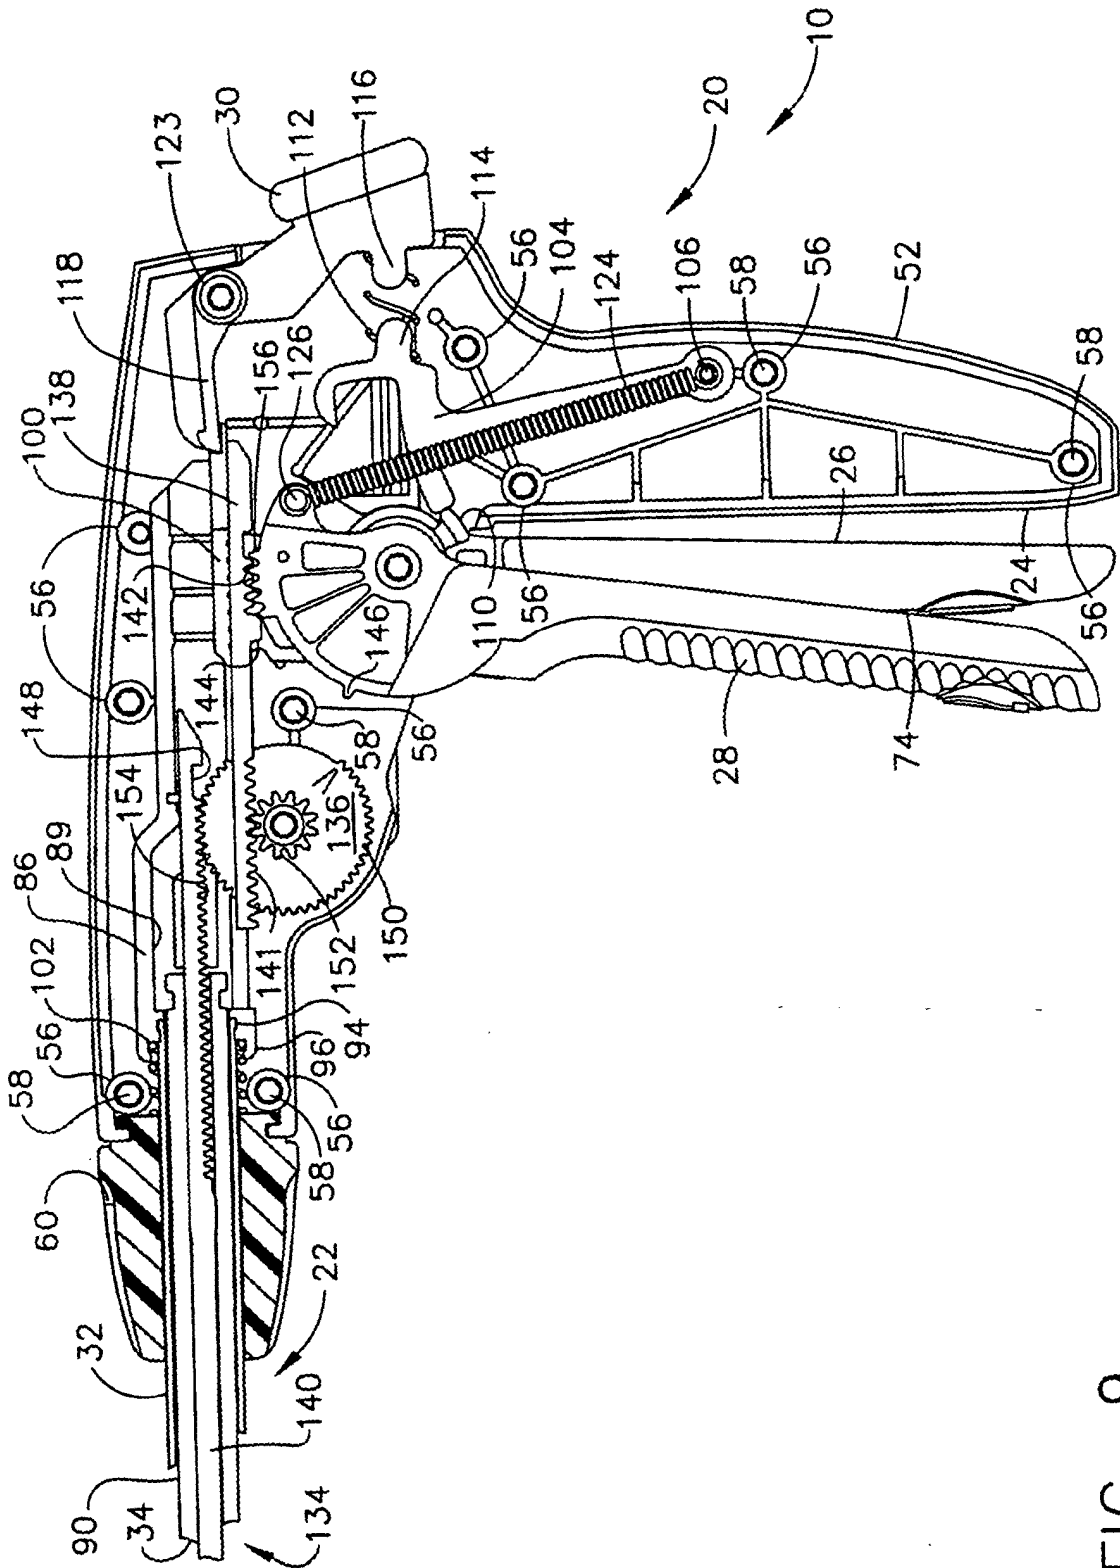


FIG. 9

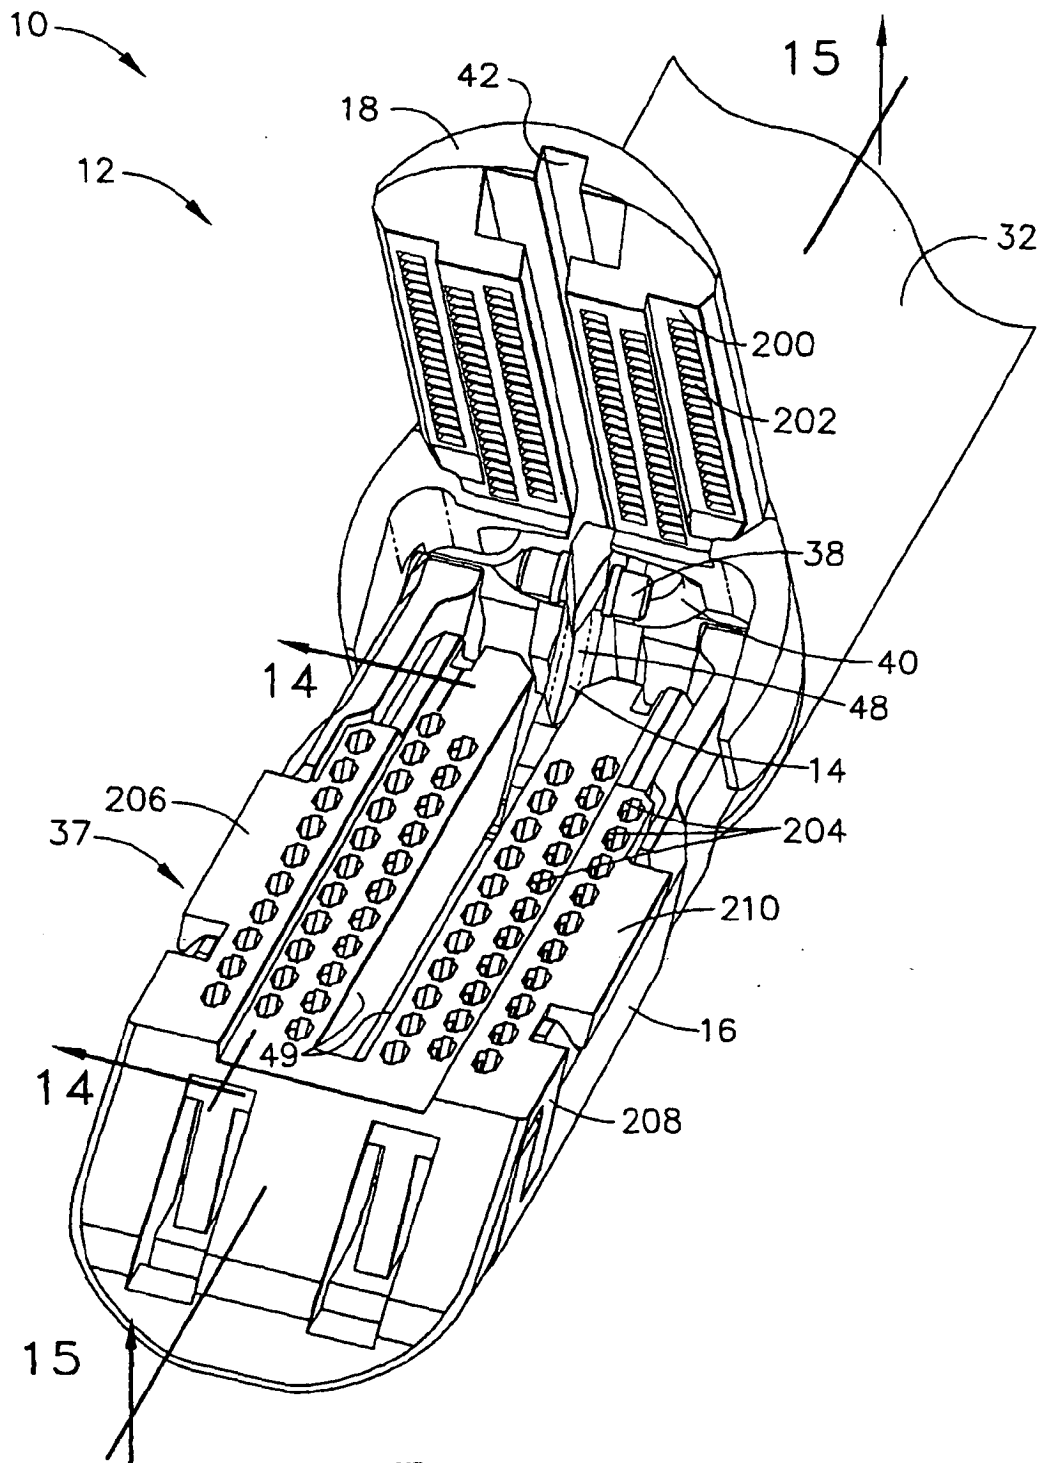


FIG. 10

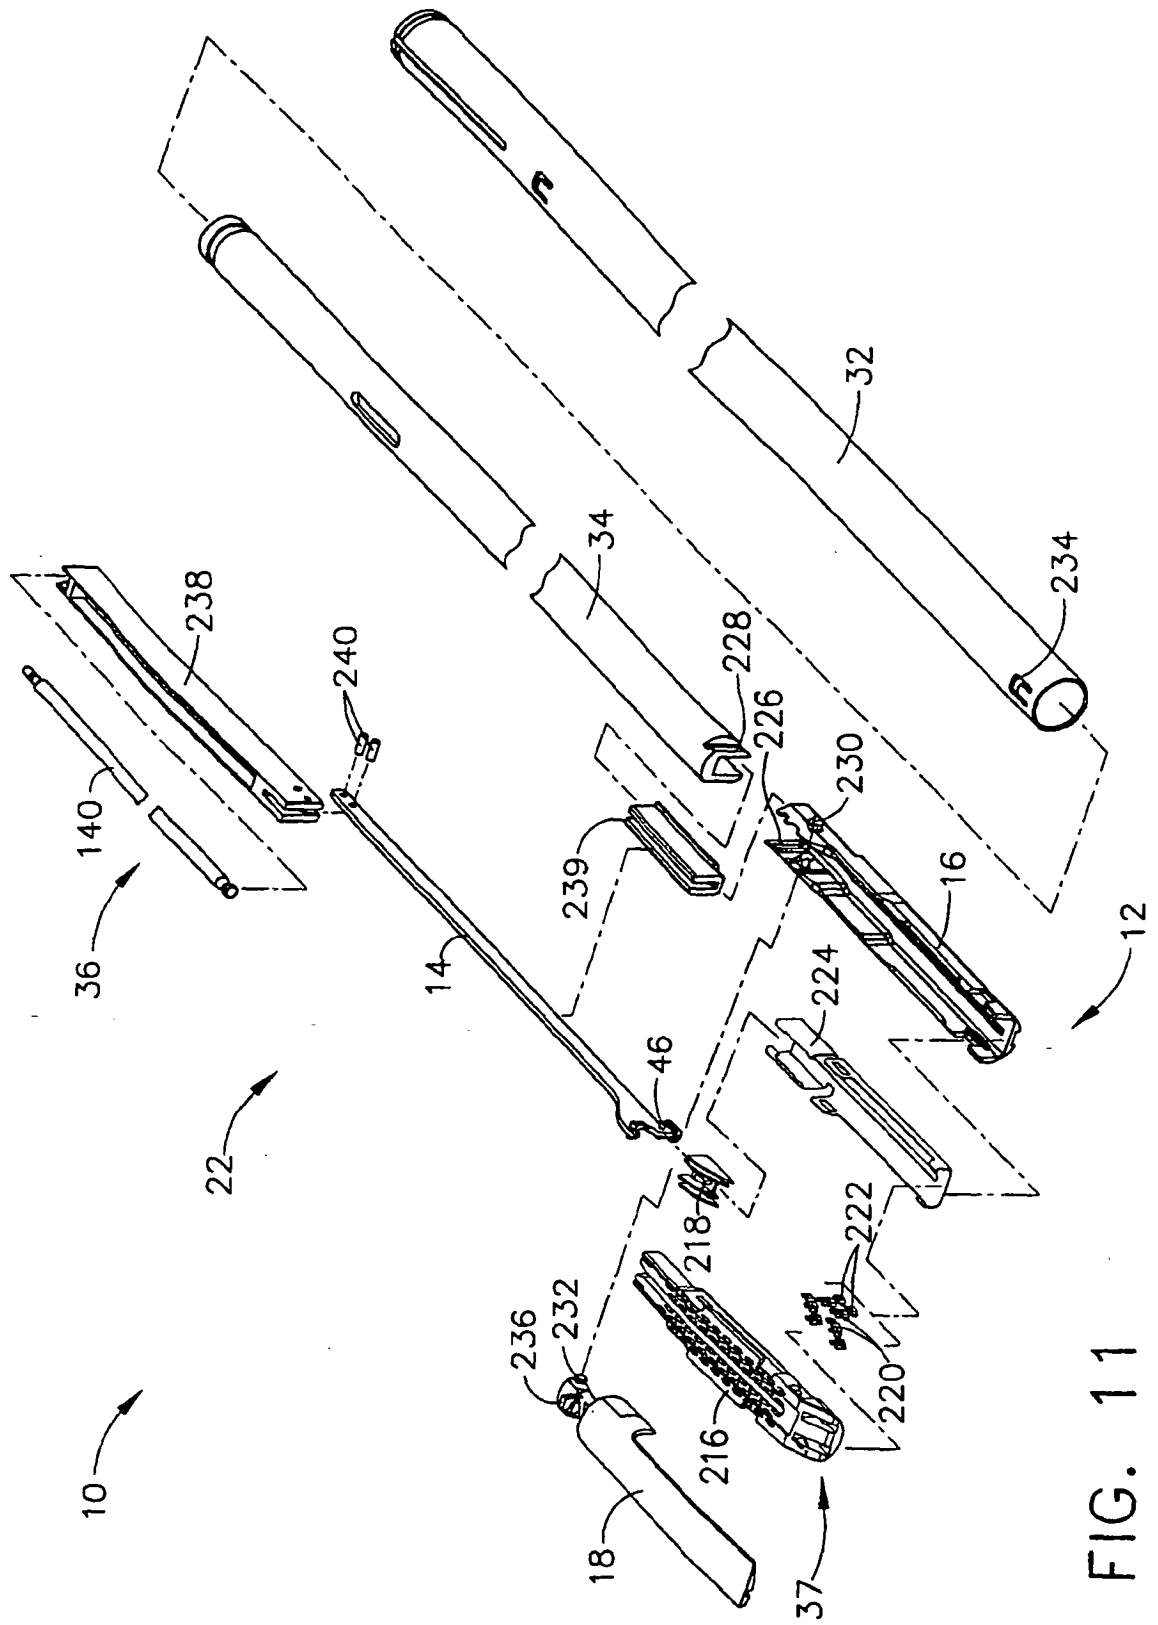


FIG. 11

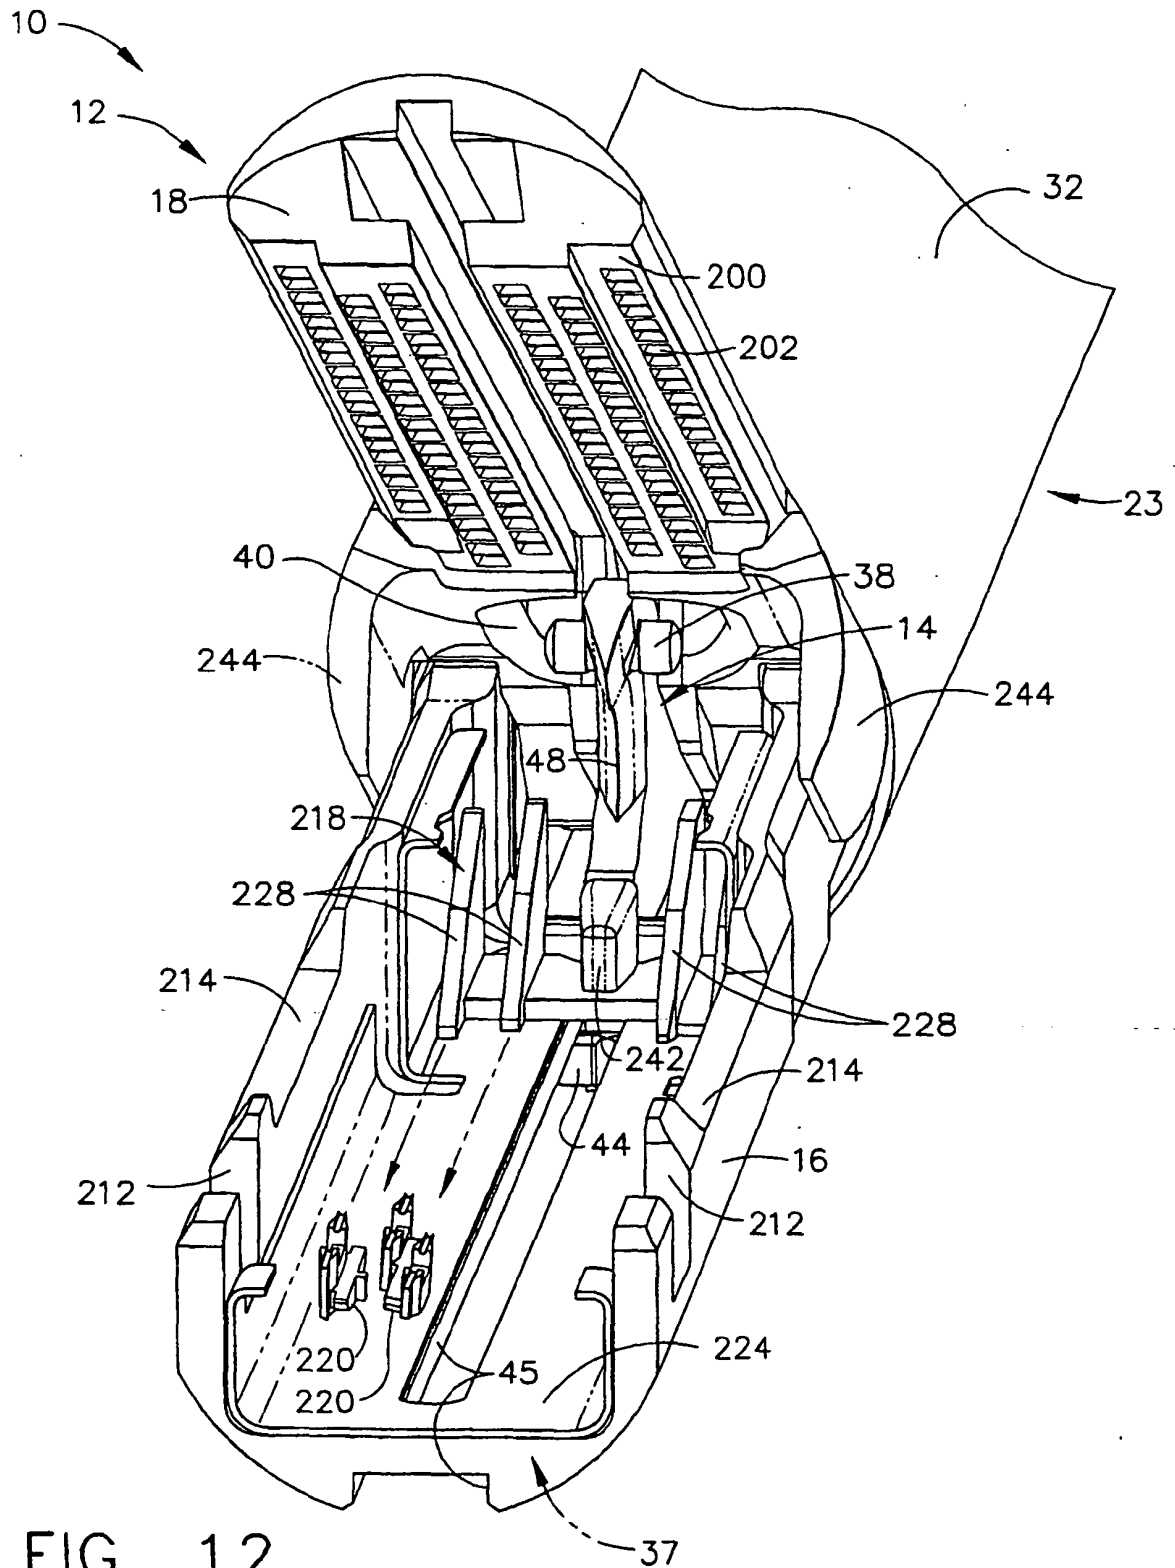


FIG. 12

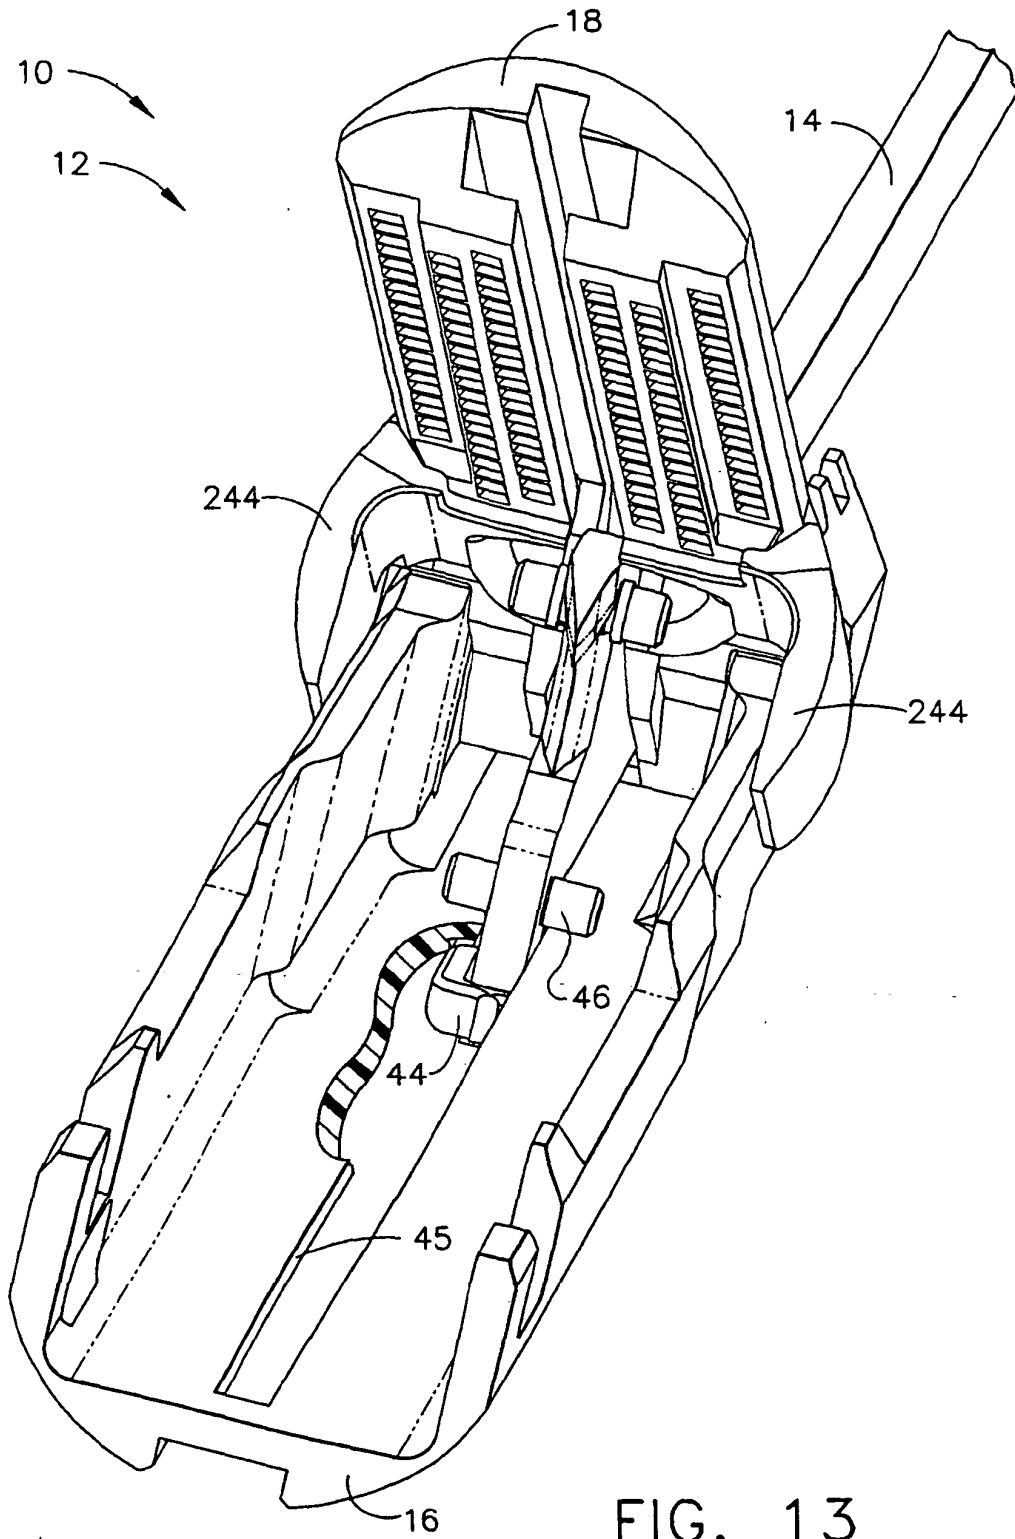


FIG. 13

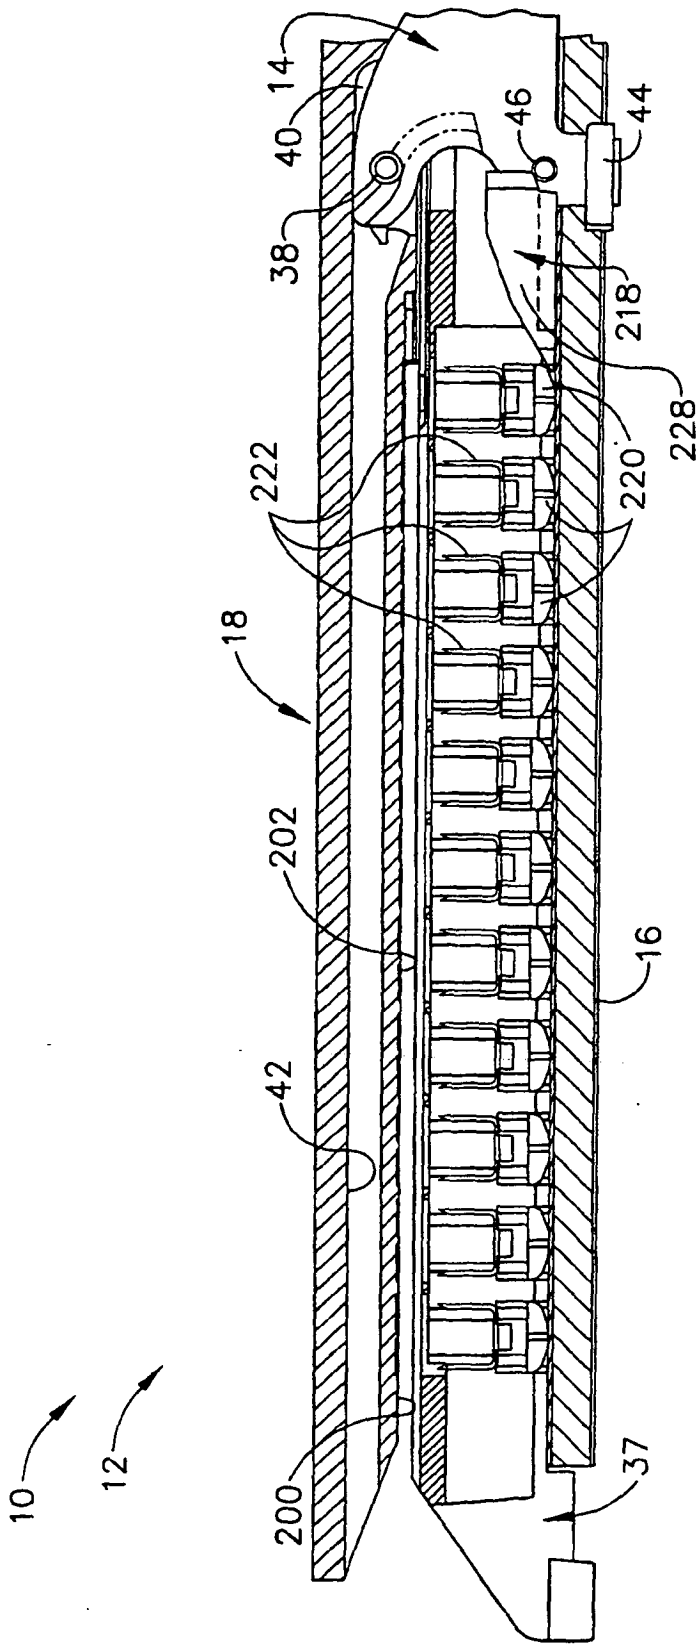


FIG. 14

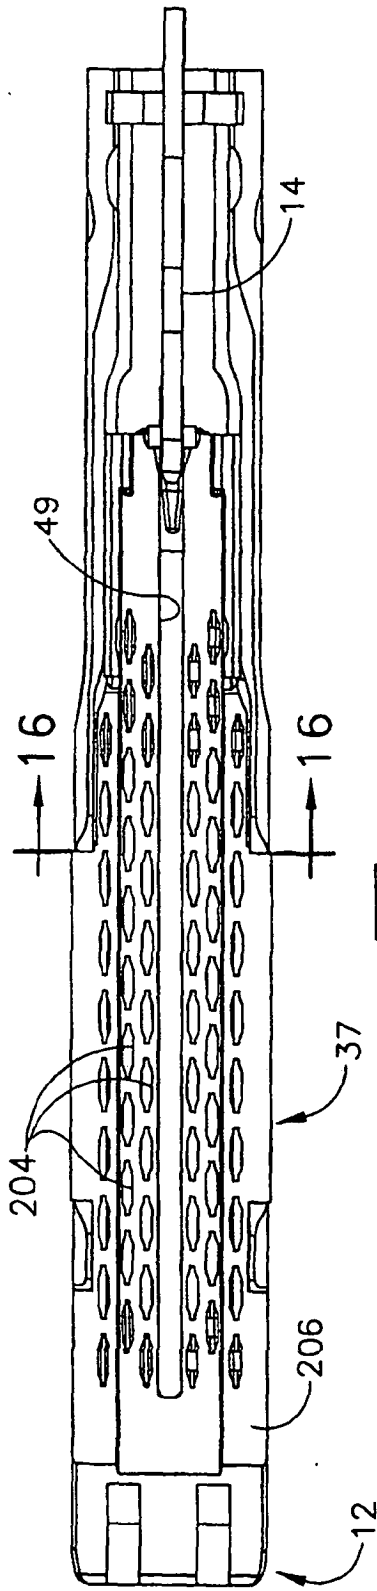


FIG. 15

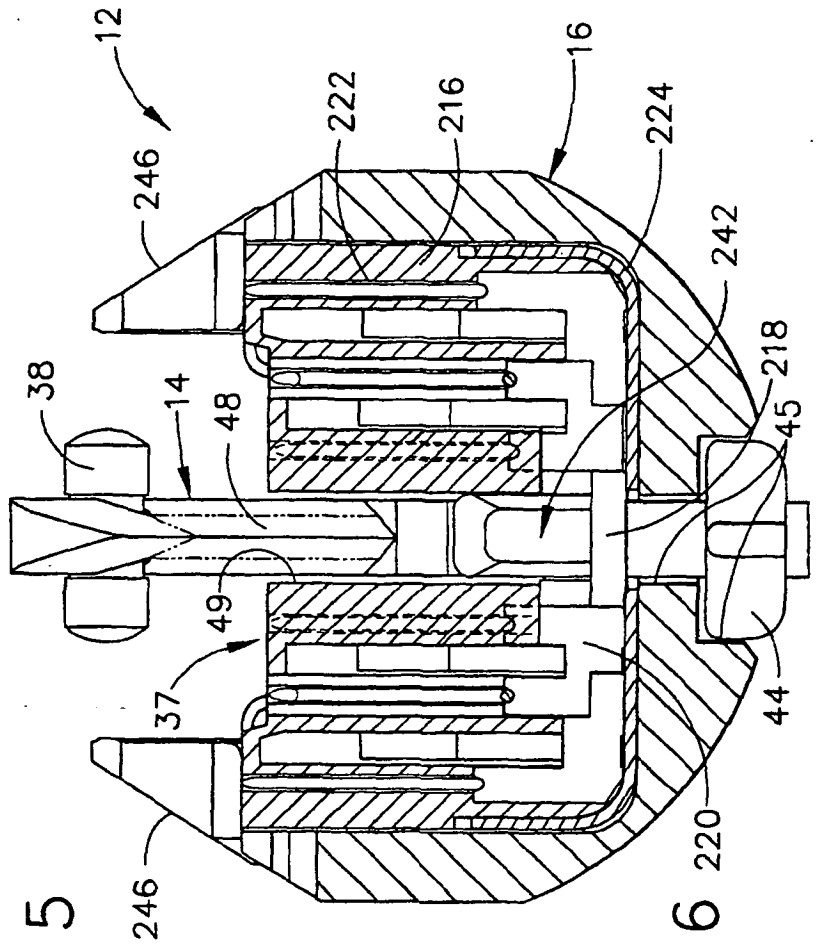


FIG. 16



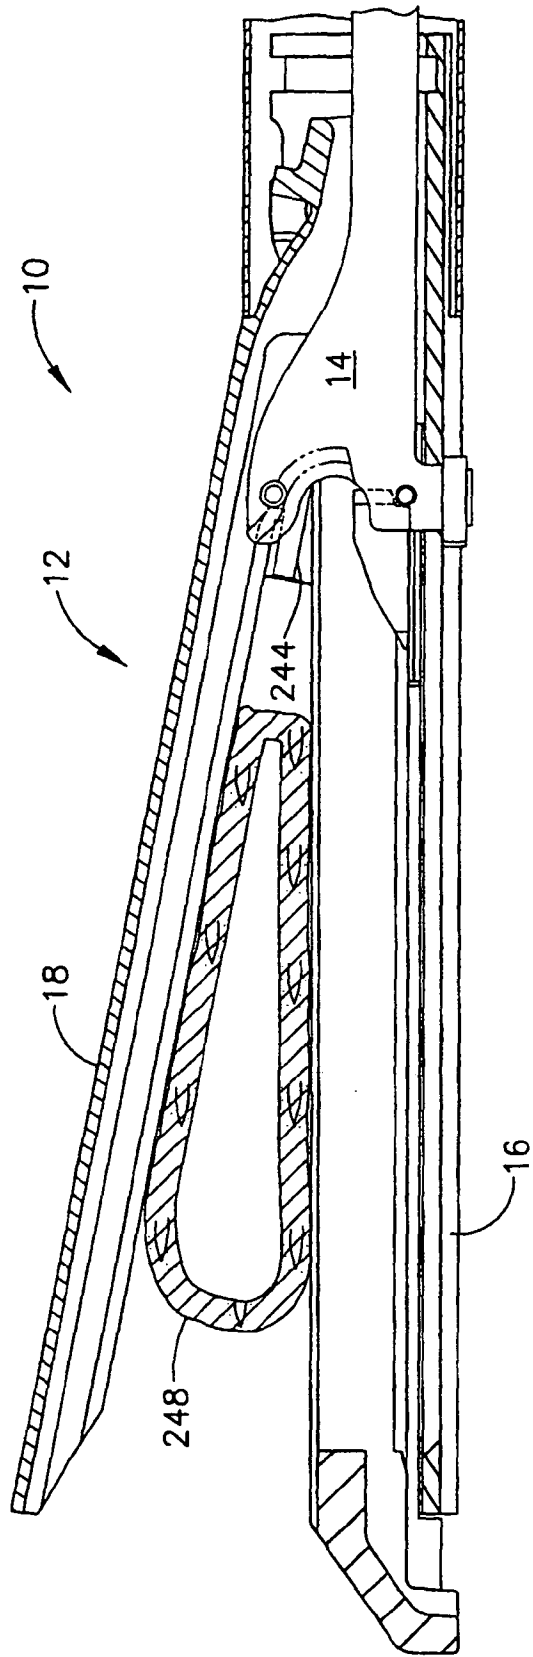
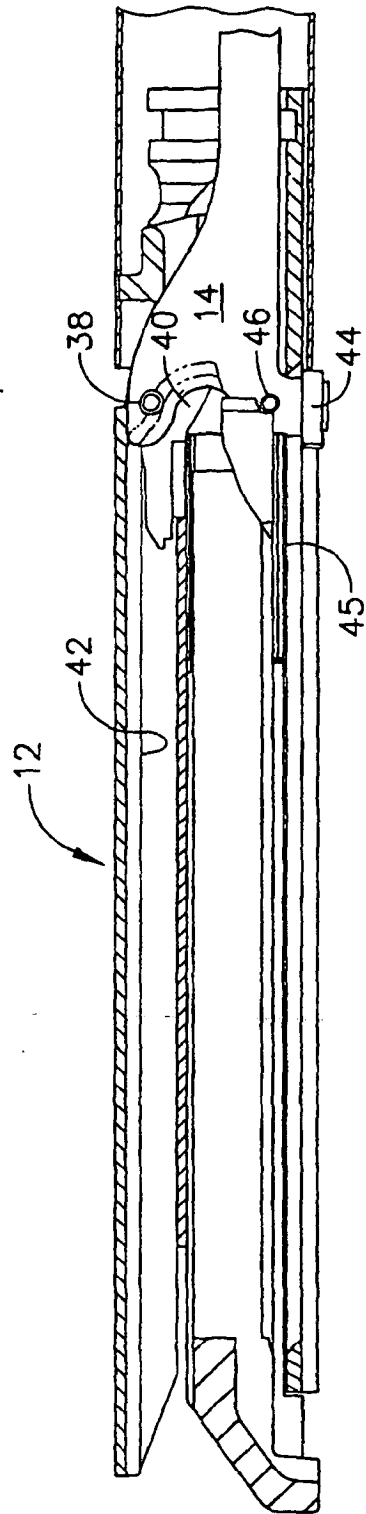
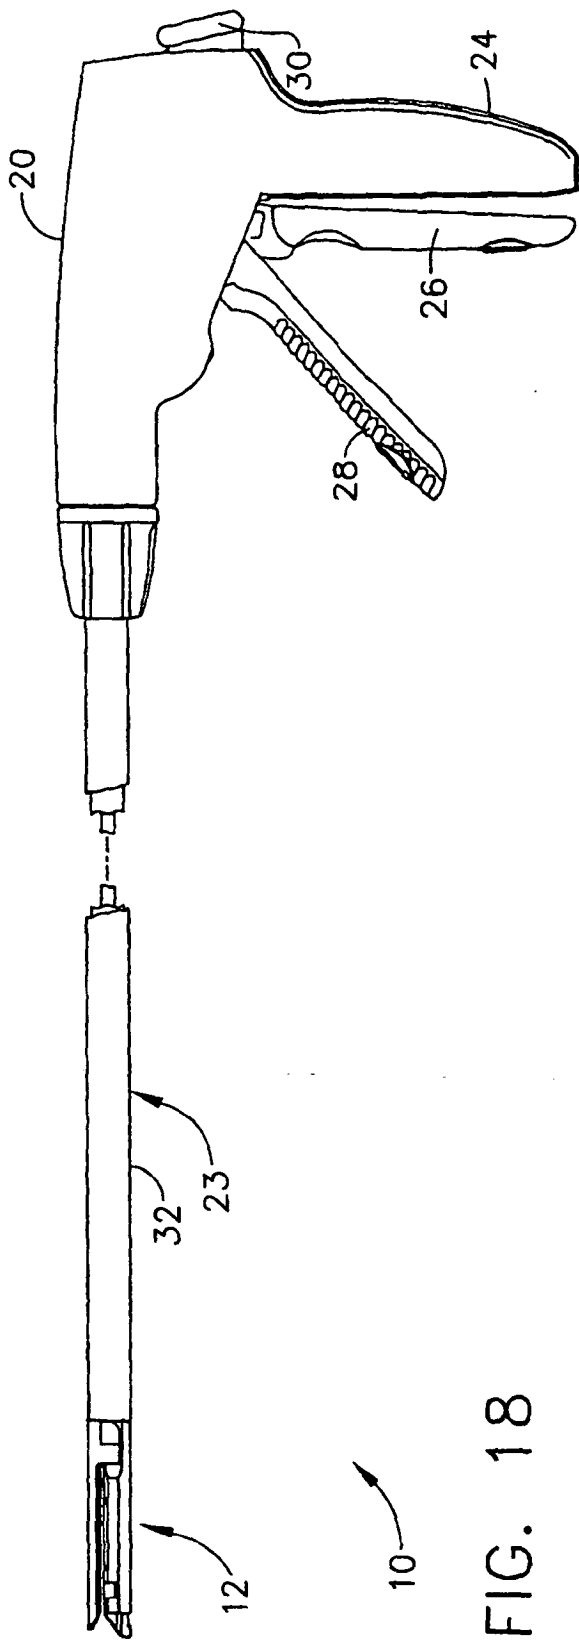


FIG. 17



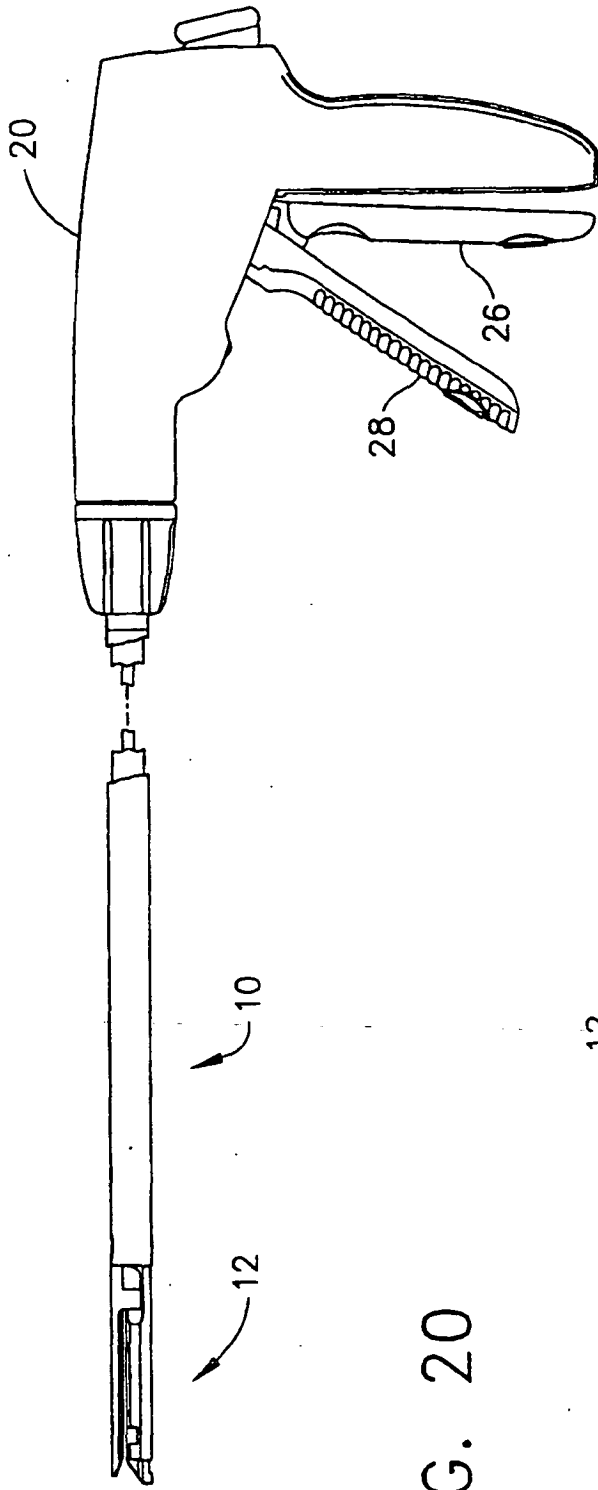


FIG. 20

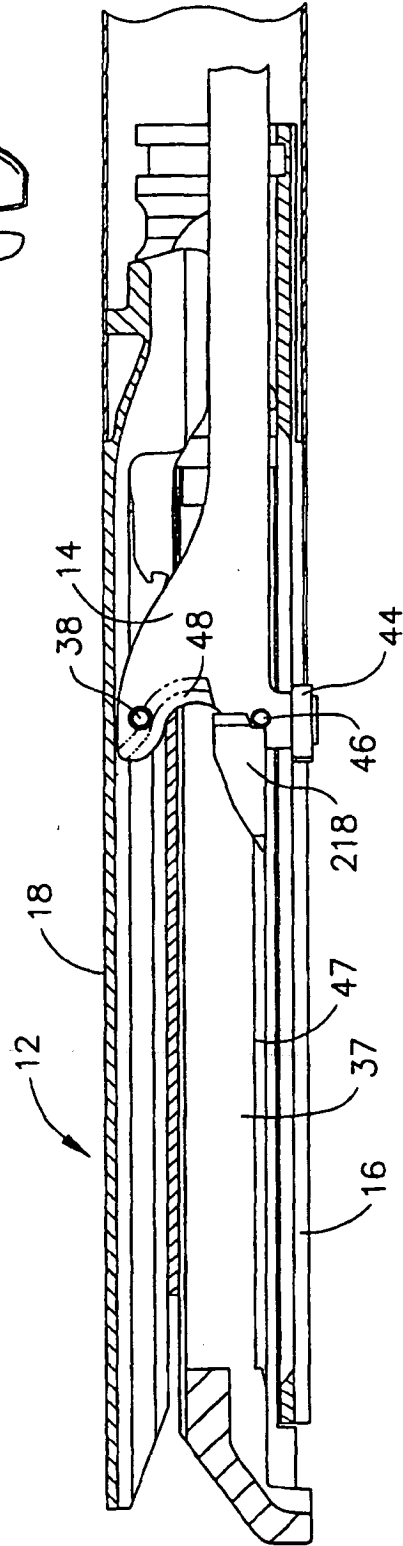


FIG. 21

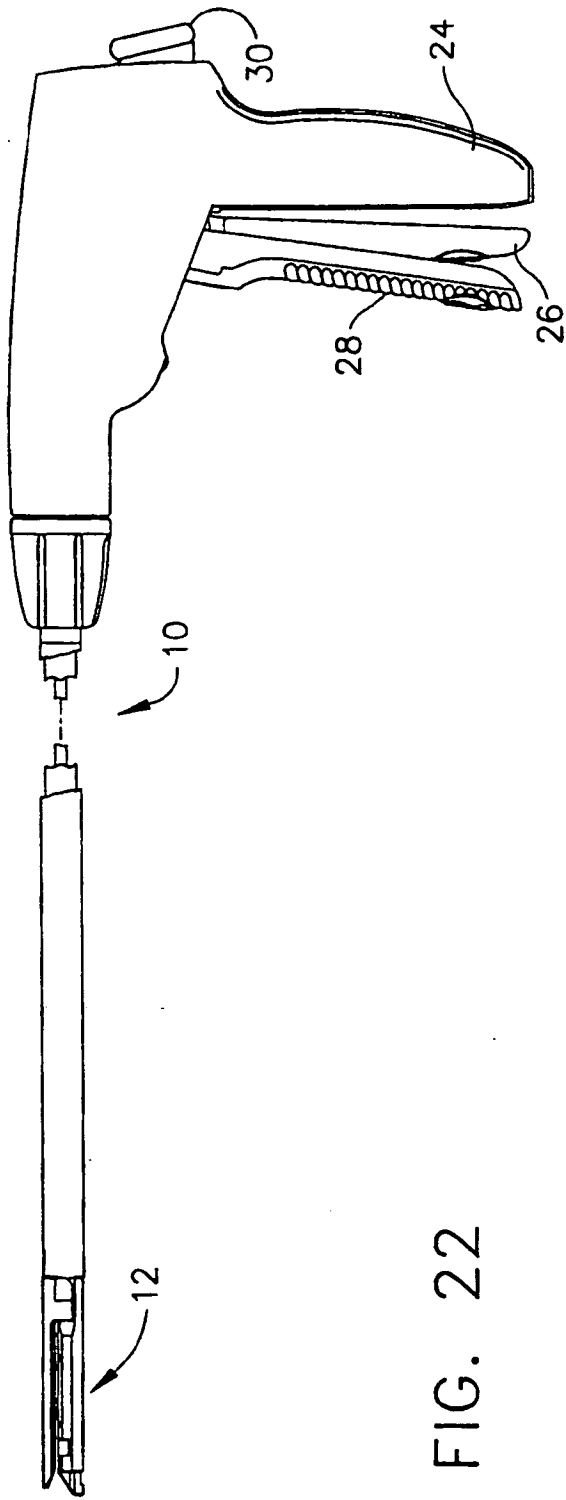


FIG. 22

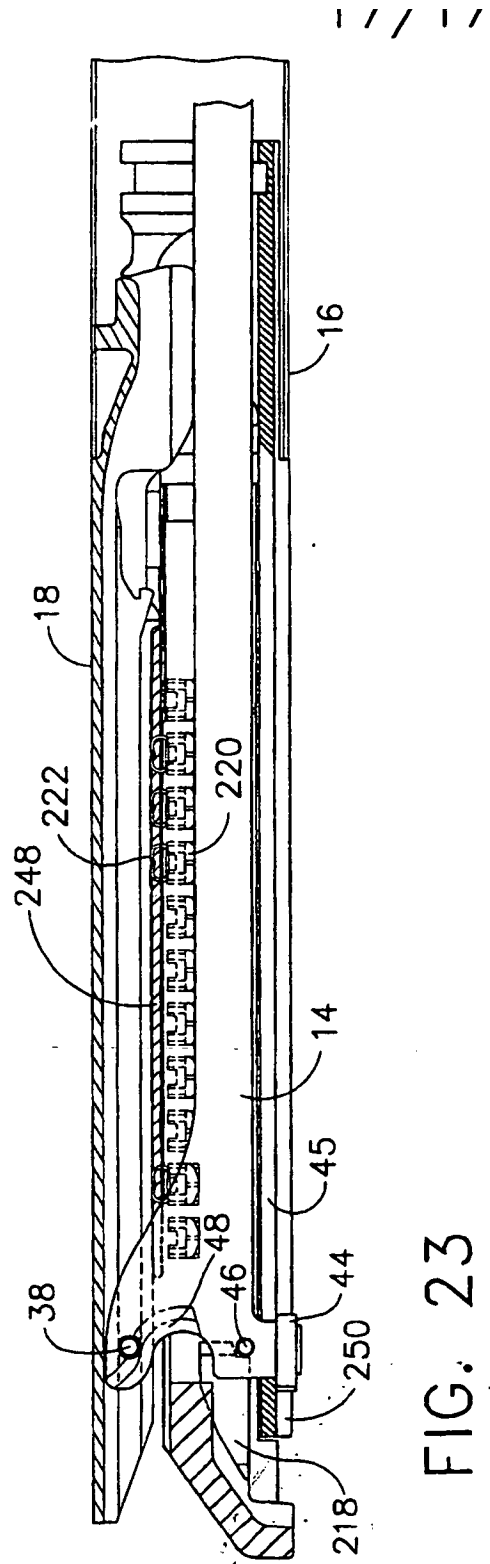


FIG. 23

专利名称(译)	包含键控发射机制的外科缝合器械		
公开(公告)号	<a href="#">EP1479346B1</a>	公开(公告)日	2007-01-10
申请号	EP2004252976	申请日	2004-05-20
[标]申请(专利权)人(译)	伊西康内外科公司		
申请(专利权)人(译)	爱惜康内镜外科		
当前申请(专利权)人(译)	爱惜康内镜外科		
[标]发明人	SHELTON FREDERICK E IV SETSER MICHAEL E WEISENBURGH WILLIAM B		
发明人	SHELTON, FREDERICK E. IV SETSER, MICHAEL E. WEISENBURGH, WILLIAM B.		
IPC分类号	A61B17/072 A61B17/32 A61B17/068		
CPC分类号	A61B17/07207 A61B2017/07214 A61B2017/07242 A61B2017/07285		
优先权	10/443617 2003-05-20 US 10/441632 2003-05-20 US		
其他公开文献	EP1479346B8 EP1479346A1		
外部链接	<a href="#">Espacenet</a>		

摘要(译)

适用于腹腔镜和内窥镜临床手术的外科切断和缝合器械夹具将组织夹在由砧座枢转地相对的细长通道的末端执行器内。电子束击发杆向远侧移动通过夹紧的末端执行器以切断组织并在切口的每一侧驱动钉。电子束击发杆肯定地将砧座与细长通道隔开，以确保适当形成的闭合钉，特别是当夹紧一定量的组织时，不足以使端部执行器间隔开。特别地，击发杆的上销纵向移动通过砧座槽，并且通道凝块被捕获在击发杆的下帽和中间销之间，以确保最小间距。

