



(51) International Patent Classification:

A61B 5/00 (2006.01) G01B 9/02 (2006.01)
A61B 17/24 (2006.01)

(21) International Application Number:

PCT/US2012/027261

(22) International Filing Date:

1 March 2012 (01.03.2012)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

61/448,345 2 March 2011 (02.03.2011) US

(71) Applicant (for all designated States except US): **DIAGNOSTIC PHOTONICS, INC.** [US/US]; 20 N. Wacker Drive, Suite 1201, Chicago, IL 60606 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **BOPPART, Stephen, A.** [US/US]; 4306 Stonebridge Court, Champaign, IL 61822 (US). **CARNEY, Paul, Scott** [US/US]; 292 Church Street, Urbana, IL 61821 (US). **CITTADINE, Andrew** [US/US]; 2119 North Magnolia Avenue, Chicago, IL 60614 (US).

(74) Agents: **ASHER, Robert, M.** et al.; Sunstein Kann Murphy & Timbers LLP, 125 Summer Street, Boston, MA 02110 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available):

AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available):

ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— without international search report and to be republished upon receipt of that report (Rule 48.2(g))

(54) Title: HAND-HELD FIXED-FOCUS OPTICAL PROBE

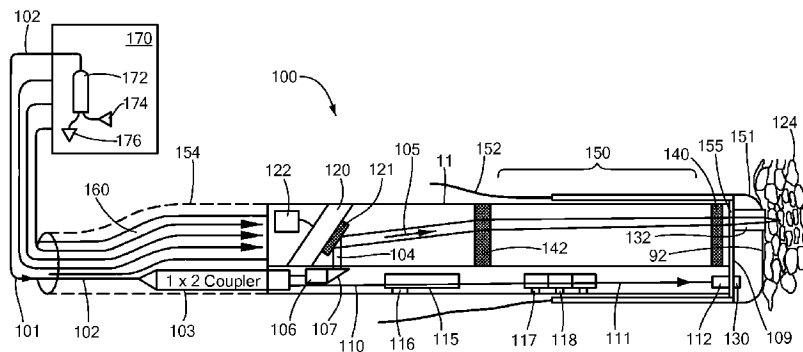


FIG. 1

(57) Abstract: An intraoperative probe and a system for optically imaging a surgically significant volume of tissue or other scattering medium. An illumination source generates an illuminating beam that is conveyed to the vicinity of the tissue and a beam splitter, that may be no more than an optical phase reference, splits the illuminating beam into a sample beam along a sample beam path and a reference beam along a reference beam path. A scanning mechanism scans a portion of the sample beam across a section of the scattering medium, while a detector detects return beams from both the reference beam path and the sample beam path and generates an interference signal. A processor computationally moves an effective focus of the sample beam without physical variation of focus of the sample beam. The probe may have a sterilizable fairing that may be detachable.



Hand-Held Fixed-Focus Optical Probe

[0001] The present Application claims the priority of US Provisional Patent Application Serial No. 61/448,345, filed March 2, 2011, which is incorporated herein by reference.

Technical Field

[0002] The present invention relates to an apparatus and methods for optically imaging a surgically significant volume of tissue by means of a hand-held probe without requiring active focusing.

Background Art

[0003] Optical coherence tomography (OCT) has proven to be an advantageous modality for noninvasive optical imaging in scattering media such as biological tissue, and is increasingly finding application in clinical diagnosis and research. Its application in surgery and microsurgery is suggested by the high resolution OCT can afford in a compact and readily integrated format. Such a probe is addressed in WO 2006/084279 (University of Florida), for example, which is incorporated herein by reference.

[0004] A major limitation attendant to existing OCT probes, however, is that the depth of focus is typically far shorter than the available imaging depth. Imaging is limited to the available confocal volume, which is smaller than the volume physically accessible to the imaging illumination. In order for the entire imaging depth to be available using existing techniques, the distance to focus must be varied relative to the body of the probe, and some focal technique must be implemented, as taught, for example, by Xie, *et al.*, *GRIN lens rod based probe for endoscopic spectral domain optical coherence tomography with fast dynamic focus tracking*, Opt. Express, vol. 14, pp. 3238-46 (2006), which is incorporated herein by reference.

[0005] Consequently, a probe that allows for three-dimensional imaging of a volume within the scattering medium without requiring that the focus be mechanically varied over the useful imaging depth would be highly desirable.

Summary of Embodiments of the Invention

[0006] In accordance with various embodiments of the present invention, a tomographic imaging system is provided for imaging a volume within a scattering medium. The system has an illumination source for generating an illuminating beam and an optical fiber for conveying the illuminating beam generated by the illumination source to the vicinity of the scattering medium. A beam splitter, which may be no more than a phase reference surface, splits the illuminating beam into a sample beam along a sample beam path and a reference beam along a reference beam path. A transverse scanning mechanism, disposed within an intraoperative probe, is provided for scanning the sample beam across a section of the scattering medium while a reflective element returns the reference beam along the reference beam path. A detector detects return beams from both the reference beam path and the sample beam path and generates an interference signal. Finally, a processor computationally moves an effective focus of the sample beam without physical variation of focus of the sample beam.

[0007] In accordance with alternate embodiments of the present invention, the sample path of the tomographic imaging may be characterized by a fixed focal depth into the scattering medium, and the fixed focal depth, in turn, may be determined in part by a fairing covering at least a portion of the intraoperative probe. The intraoperative probe may be hand-held by an operator, and may also be adapted for endoscopic or laparoscopic manipulation.

[0008] In certain embodiments of the invention, the beam splitter may be disposed within the intraoperative probe. A reflective element may be provided for returning the reference beam along the reference beam path, and it, too, may be disposed within the intraoperative probe.

[0009] In accordance with some embodiments of the invention, the sample path and the reference path coincide in part. The optical fiber may be mode-preserving, and the transverse scanning mechanism may be microelectromechanical.

[0010] In accordance with other embodiments of the present invention, a fairing may cover a portion of the intraoperative probe. The fairing may be adapted to serve as a sterile barrier between components of the intraoperative probe and the scattering medium. A focusing element may be disposed within the intraoperative probe for focusing the sample beam into the scattering medium, and the fairing may be adapted to provide a fixed offset distance between the focusing element and the scattering medium. The portion of the intraoperative probe covered by the fairing may include the entirety of the hand-held probe.

[0011] In further embodiments of the present invention, the fairing may include a distal tip disposed at an end of the hand-held probe proximate the scattering medium, and the distal tip may be substantially transparent to the sample beam and may include a focusing element of the sample beam. The distal tip may be adapted to serve as an optical phase reference for the interferometric tomography system, moreover a reflective element, or a plurality of reflective elements, may be integral with the distal tip of the fairing. An effective reflectivity of the reflective element may be varied by virtue of orientation of the reflective element with respect to a lens disposed within the reference beam path, where the lens may be a graded index lens.

[0012] In yet further embodiments of the present invention, the processor may be of a kind generating an extended-region image, more particularly, the processor may be of a kind employing interferometric synthetic aperture microscopy for generating an extended-region image without physical variation of focus of the sample beam. A camera may provide a real-time visual image of a surface of the scattering medium being tomographically imaged.

[0013] In accordance with a further aspect of the present invention, an intraoperative probe is provided for imaging a volume within a scattering medium. The intraoperative probe has an optical fiber for receiving an illuminating beam, a transverse scanning mechanism for scanning the sample beam across a section of the scattering medium, and a detachable sterile fairing extending over an end of the hand-held probe proximate the scattering medium, wherein the sterile fairing includes a distal tip which is substantially transparent to the sample beam.

[0014] In some, but not all, embodiments of the present invention, the intraoperative probe is hand-held. The intraoperative probe may also have a beam splitter for splitting the illuminating beam into a sample beam along a sample beam path and a reference beam along

a reference beam path, as well as a reflective element for returning the reference beam along the reference beam path. A portion of the distal tip may be substantially reflective of the reference beam. In various embodiments, the sample beam path and the reference beam path may coincide in part, up to substantially an entirety of the respective paths. A single optic may serve both to transmit the sample beam and to reflect the reference beam. The transverse scanning mechanism may be microelectromechanical, and the intraoperative probe may also have an intensity adjustment mechanism, or a polarization adjustment mechanism, within the reference beam path. The detachable sterile fairing may enclose the hand-held probe in substantial entirety.

[0015] In accordance with a further aspect of the present invention, a disposable fairing is provided for enclosing an intraoperative probe of a tomographic imaging system. The disposable fairing is characterized by substantial transparency to a scanning sample beam transmitted from the intraoperative probe to a volume within an imaged scattering medium. The disposable fairing may have an integral reflector for reflecting a reference beam, as well as a hard distal tip covering an end of the intraoperative probe proximate to the imaged scattering medium. The fairing may include a film jacket covering connecting cables that couple the intraoperative probe to a source of illumination and to a detector.

Brief Description of the Drawings

[0016] The foregoing features of the invention will be more readily understood by reference to the following detailed description, taken with reference to the accompanying drawings, in which:

[0017] Fig. 1 depicts an intraoperative imaging probe, in accordance with an embodiment of the present invention;

[0018] Fig. 2 is a cross sectional view of a fairing tip with multiple mirrors providing selectable reflectivity for the reference beam, in accordance with an embodiment of the present invention and

[0019] Fig. 3 is a cross-sectional view of an embodiment of the present invention in which an optical camera is attached to a hand-held intraoperative imaging probe.

Detailed Description of Embodiments of the Invention

[0020] *Definitions:* As used herein and in any appended claims, the term “image,” used as a noun or as a verb, and unless otherwise required by context, refers to the creation of a holomorphic mapping of values characterizing points in space such that the values may, thereafter, be associated, one-to-one, with particular points in space. The values may be stored in a memory, or displayed on a monitor, or fixed in a medium. The values mapped in the creation of an image are typically scalar, such as the scalar susceptibility associated with each point in the volume of the imaged sample. However, the mapping of a vector (or tensor) property of the sample, whether in two or three dimensions, and whether also incorporating other dimensions such as frequency or time (or some other experimental value, such as temperature, for that matter), will also be considered “imaging” for purposes of the following description and claims.

[0021] The term “interferometric tomography system,” as used herein and in any appended claims, shall be comprehensive and shall subsume systems referred to as low-coherence imaging systems, and of optical coherence tomography (OCT), whether time-domain, spectral-domain, or swept-source, and all other interferometric tomography systems currently known or subsequently invented of which the hand-held probe described herein may form a part.

[0022] The term “beam splitter,” as used herein and in any appended claims, shall include any element, or feature of an element, that serves to split differential between distinct components of a beam. Thus, for example, the beam splitter may include a dedicated component such as a directional coupler or circulator, and may also include the polished end of a fiber which gives rise to a distinguishable reflection of a beam component, along a common path, where that beam component may serve as a reference beam. A device feature, such as the surface of an optic, that provides an optical phase reference serves as a “beam splitter.”

[0023] The adjective “intraoperative” describes an imaging probe that may be positioned, or repositioned, by an operator, such as a surgeon, based upon an image that is being displayed in real time, or near real time. An intraoperative probe may include a probe

that is directly hand-held by a surgeon, pathologist, or other healthcare professional, and, additionally, a probe that is manipulated endoscopically or laparoscopically.

[0024] The term “fairing,” as used herein and in any appended claims, refers to a cover used to encase a portion, or all, of a hand-held probe, which cover may be transparent, in whole or in part, and may have segments of varying degrees of flexibility and conformance with the surface contour of the underlying probe or portions thereof. A fairing, as defined herein, may also be referred to by other terms.

[0025] The term “transverse scanning,” or any mechanism associated therewith, is not limited to linear scanning of a beam to positions within a plane but encompasses scanning along any line or surface, including Cartesian, helical, or circular scanning, such as by rotation transverse to the axis of an endoscope, for example.

[0026] The expression “in part,” as used herein and in any appended claims, shall encompass within its scope both a proper subset of the entirety and also the entirety.

[0027] Interferometric synthetic aperture microscopy (ISAM) is one of a class of methods of tomographic optical microscopy. ISAM brings together the power of computed imaging and inverse scattering together with interferometric broadband optical imaging. Solution of an inverse scattering problem entails two steps. In preparation for applying inverse scattering technique, a forward model is derived, as described, for example, in US Patent No. 7,643,155 (to Marks et al., hereinafter, “Marks ’155”) based on scattering of light by inhomogeneities in the sample susceptibility. In a second step, a signal based on coherent detection of scattering from the sample is used to infer a three-dimensional susceptibility of the sample based on comparing the detected signal to data predicted from the forward scattering model. Thus, the objective in formulating the forward model is to derive an expression for the data in terms of the unknown object susceptibility. Coherent detection of the scattering signal is performed using a device that interferes the scattering return from the sample against a reference signal derived from the same source as the sample signal. Hand-held probes in accordance with embodiments of the present invention are such devices.

[0028] Detailed practice of ISAM principles may be understood with reference to the following articles and patent literature, all of which are incorporated herein by reference:

- Ralston *et al.*, “Inverse scattering for optical coherence tomography,” *J. Opt. Soc. Am. A*, vol. **23**, pp. 1027-37 (2006).
- Ralston *et al.*, “Inverse scattering for high-resolution interferometric microscopy,” *Opt. Lett.*, vol. **31**, pp. 3585–87 (2006).
- Ralston *et al.*, “Interferometric synthetic aperture microscopy,” *Nat. Phys.*, vol. **5**, pp. 129–34, (2007).
- Marks *et al.*, “Inverse scattering for frequency-scanned full-field optical coherence tomography,” *J. Opt. Soc. Am. A*, vol. **24**, pp. 1034–41 (2007), hereinafter, “Marks (2007).”.
- Ralston *et al.*, US Patent No. 7,602,501 (October 13, 2009).
- Marks *et al.*, US Patent No. 7,643,155 (January 5, 2010).

[0029] In accordance with preferred embodiments of the present invention, an intraoperative probe, designated generally by numeral **100**, is provided, and is now described with reference to Fig. 1. For heuristic convenience, descriptions are provided herein in terms of a hand-held probe, although it is to be understood that endoscopically and laparoscopically manipulable probes are similarly within the scope of the invention presently described and claimed. Embodiments of the present invention allow the physical focus of the tomographic imaging system to be maintained within a single “plane” disposed within sample **124** while imaging information is derived for the entirety of a sample volume by application of ISAM or any other software approach that reconstructs the three-dimensional susceptibility of the sample. It is to be understood that, within the scope of the present invention, the “plane” of focus may, in fact, refer to a curved two-dimensional surface that departs, to some degree, from geometrical planarity.

[0030] An interferometric tomography system, in accordance with embodiments of the present invention, employs the following basic components:

- a source of illumination **174**, provided by a source of incoherent, or partially coherent, light, and conveyed to the hand-held probe **100** as an illumination beam **101** by a coherence-preserving optical fiber **102**, typically a single-mode fiber;
- a beam splitter **103** for splitting the illumination beam **101** propagating through optical fiber **102** into a sample beam path **104** and a reference beam path **110**. The function of beam splitter **103** is fulfilled, for example, by means of a fiber optical

directional 1×2 coupler, although any beam splitter known, or invented in the future, is within the scope of the present invention as described or claimed herein. By way of another example, a 2×2 fiber optical coupler may be employed, as further discussed below. Beam splitter **103** is preferably mode- (and thus also polarization-) preserving. The beam propagating along sample beam path **104** may be referred to herein as a sample beam **105**, while the beam propagating along reference beam path **110** (which is preferably an optical fiber) may be referred to as reference beam **111**. Additionally, the sample beam path may be referred to herein as the “sample arm,” and, *mutatis mutandis*, the reference path and “reference arm” are the same.

- a transverse scanning mechanism, designated generally by numeral **120**, that sweeps sample beam **105** across an areal section **92** of sample **124**. Sample **124** may be biological tissue, typically *in situ*. Transverse scanning mechanism **120** is discussed below. Sample beam **105** is attenuated and scattered as it propagates into sample **124**.
- a reflector **130** that reflects reference beam **111** back to beam splitter **103** for recombination, and interference, at a detector (not shown), with the scatter from sample **124**.

[0031] In embodiments of the invention in accordance with Fig. 1, the source of illumination and the detector are both disposed in a remote unit **170** distinct from the hand-held probe, which may be referred to as the interferometric tomography engine, or, in the case where the interferometric tomography system employs ISAM, the remote unit may be referred to as the “ISAM engine” **170**. In accordance with the embodiment of Fig. 1, an additional directional coupler **172** is provided within the remote unit **170**, coupling the source of illumination **174** and the detector **176**, respectively, to coherence-preserving optical fiber **102**. In alternate embodiments of the invention, there may be a single 2 × 2 directional coupler in the hand-held unit **110**, in which case there are two fibers **102** running from the probe **110** back to the ISAM engine, not just the one shown in Fig. 1. In yet another embodiment of the invention, hand-held probe **110** may contain a 2 × 2 directional coupler as well as the detector. It is preferred, however, in the case where a spectral-domain ISAM system is employed, that a spectrometer and detector array be disposed remotely from the probe as part of the ISAM engine.

[0032] As used herein, incoherence, or partial coherence, as applied to the source of illumination 174, refers to the fact that the electromagnetic field associated with different parts of the emitting surface of the source produce mutually incoherent electromagnetic fields, and do not interfere when averaged over a pertinent time scale such as the inverse bandwidth of the detection system. An example of a spatially incoherent source is the filament of an incandescent light bulb. The spatially incoherent source may be a source of visible or near-infrared light.

[0033] In embodiments implementing full-field imaging, the rigorous treatment of which was developed in Marks (2007), the source of illumination of the interferometric imaging system is preferably a spatially incoherent, quasimonochromatic source. In scanned embodiments, on the other hand, typically employing single-mode fiber (SMF), light illuminating the sample is typically spatially coherent. The source of illumination 174 may be characterized by a tunable temporal frequency (or, equivalently, wavelength). In accordance with various methods of employing the hand-held probe taught herein for interferometric imaging, the source may be of a fixed and narrow wavelength band, or may be a broadband source or a swept source. Data may be acquired by any of the foregoing interferometric modalities, with the intensity of interferograms on the detector recorded and processed. From these interferograms, the susceptibility of the sample is inferred.

[0034] It should be understood that, in accordance with alternate embodiments of the present invention, sample beam 105 and reference beam 111 may share a common path, and may share the same, or orthogonal, polarization. In one common-path embodiment of the invention, beamsplitter 103 is “degenerate” in that sample beam 105 and reference beam 111 are not physically separated. In that case, a surface of a focusing element 140 or of fairing tip 151, to be discussed below, may serve as reflector 130 while, at the same time, transmitting sample beam 105 into the sample. Reference beam 111 need not be present within hand-held probe 100 at all, within the scope of the present invention, in which case sample beam 105 alone is coupled via optical fiber 102 to the probe.

[0035] Referring further to Fig. 1 for other details of embodiments of the present invention, sample beam 105 may be coupled out of directional coupler 103 by means of an optic such as graduated index (GRIN) lens 106. Transverse scanning mechanism 120 may be a microelectromechanical (MEMS) –driven reflector 121 with attendant MEMS-driving

electronics **122**. Alternatively, sample beam **105** may be scanned electro-optically, or by any other scanning mechanism known in the art or subsequently invented. Transfer optics, such as right angle prism **107** – shown by way of example, and focusing elements **140** and **142** may be employed for conveying sample beam **105** onto sample **124** using any means known in the optical arts. A stand-off volume **155** may be provided between focusing optic **140** and cover surface **109** of the hand-held probe **100**, the optical path through which constitutes a portion of the fixed distance between optic **140** and a focal plane (or surface). Stand-off volume **155**, also referred to as an “air gap,” may, alternatively, also be filled with a liquid, glass or other optically transparent material of specified refractive index, as a matter of design choice. Air gap **155**, in combination with the thickness of the transparent window **132** (optionally such window may be a focusing element in which case the focusing properties – i.e. a lens focal distance – would also be included) within probe tip **151**, defines the focal distance of the instrument.

[0036] Focusing element **140** may serve to form a seal against liquid ingress into probe **100**. Optionally, an additional optical element, such as glass window **109**, may be inserted between the focusing element **140** and the probe tip **151** to seal the probe from liquid ingress. Preferably such element is sufficiently removed from the tissue surface to avoid reflections in the imaging plane. Such optical element may also be coated with an anti-reflective material or aligned off-parallel to a transparent window **132** to minimize internal reflections.

[0037] Transparent window **132** in the probe tip **151** may be positioned such that it is in contact with the tissue. Moreover, the optical element designated by numeral **132** may be a powered optic (*i.e.*, a lens), and, as such, serve to focus sample beam **105** into the sample **124** (or scattering medium). As stated above, the hardened plastic end, distal tip **151**, may serve to provide a fixed offset distance between lens **140** and imaged tissue **124** to ensure proper path length and/or optical properties. This is true also with glass **132** on tissue surface and an “air gap” **155** between focusing element **140** and window **132**.

[0038] Similarly, within reference path **110**, a GRIN lens **112** may be provided to couple reference beam **111** from optical fiber to free space, and, more particularly, to reflector **130**. An in-line fiber attenuator **115** may be provided for maintaining detector signals within a desired dynamic range, or to optimize signal to noise.

[0039] An outer fairing (which is preferably sterilizable, and disposable after a single use, but which may also be fixed, within the scope of the invention) covers a portion, or all, of the hand-held probe **100**, and is designated generally, in Fig. 1, by numeral **150**. Fairing **150**, in turn, may include a distal tip **151**, otherwise referred to as a “cap,” typically a hard section adapted to cover surface **109** of hand-held probe **100** proximate to sample **124**. Distal tip **151** (also referred to, herein, without limitation, as a hard-plastic end), may, for example, be acrylic or polymethylpentene (PMP, or TPX[®]) or other functional polymer, and may include integrated optical elements such as a window **132** and one or more mirrors **130** necessary for probe function. The distal tip **151** of fairing **150** is, thus, typically, a cylindrical rigid plastic element with an integral end closure that slides over housing **11** of hand-held probe **100**. Housing **11** of hand-held probe **100** is preferably machined metal, such as aluminum, while fairing **150** may advantageously provide sterile covering, and serve as a sterile barrier, when used in the sterile surgical field. The disposable fairing **150** preferably allows control with good tactile feedback of the probe controls.

[0040] The hardened plastic end, distal tip **151**, may serve to provide a fixed offset distance between lens **140** and imaged tissue **124** to ensure proper path length and/or optical properties. Distal tip **151** may extend over hand-held probe **100** and may transition to a sheath **152** of plastic film, or elastomer, or other material. Sheath **152** may, in turn, transition to a semi-flexible jacket **154** that encases optical fiber **101** and power and control electrical leads **160** that couple hand-held probe **100** to fairing **150**.

[0041] The distal tip **151** includes an optically transparent window through which sample beam **105** passes for imaging tissue **124**. Transparent window **132**, may be glass or plastic, for example, or other transparent material appropriate to the wavelength being employed for imaging. Distal tip **151**, may also provide the needed phase reference for common-path Doppler, or ISAM data collection, by virtue of a partial reflection from one of the surfaces of transparent window **132**. (A description of a common-path Doppler imaging system to which aspects of the present invention may be advantageously applied is provided by Koch *et al.*, *Resonant Doppler Imaging with Common Path OCT*, Optical Coherence Tomography and Coherence Techniques IV (Andersen *et al.*, eds.) (SPIE-OSA, 2009), incorporated herein by reference.) One or more small partially-reflective mirrors **130** may be integrated into distal tip **151**, serving as an optical phase reference for the interferometric

system.. Multiple mirrors **130** (shown in Fig. 2) may be integrated into distal tip **151** and may be of various reflectivities and available for selection for different tissue types or to optimize the signal-to-noise of the interferometric imaging system. Mirrors may be selectable by sliding distal tip **151** with respect to metal probe housing **11** along various grooves or détentes, each for a different mirror. Distal tip **151** is preferably characterized by a smooth rounded end that facilitates contact and movement across tissue **124** during imaging.

[0042] The rigid plastic distal tip **151** of the probe covering fairing **150** is connected to, and/or transitions to a plastic tube-like sheath **152** and jacket **154** that extend proximally from the probe cover tip **151**, typically for several meters. This sterile sheath **154** covers the wires/cables **160** of the hand-held probe **110** to maintain sterility when used in the surgical field. This single-use disposable fairing **150**, inclusive of the hardened distal tip **151** and flexible sheath **152** and jacket **154** (which may form a single integral part, or multiple parts) is placed over the probe **110** and wires **160** prior to each surgical procedure.

[0043] The fairing **150** may also have integrated irrigation and aspiration channels, with connecting plastic tubing integrated into the sheath and exiting at the proximal end, where the irrigation and aspiration channels may be connected to a room saline/water supply and pump, and to vacuum. A footpedal switch, or a button on the probe cover/unit controls irrigation/aspiration, intended to be used to rinse the end of the probe face, and to clear blood/fluids from the probe **110** and/or the tissue **124** to be imaged.

[0044] As now described with reference to Fig. 3, a clip-on video camera **164** may be attached to the hand-held probe **110** to provide a CCD-based real-time video image of the surface of the tissue **124**, the volume of which is being imaged using the interferometric tomography system **110**, using ISAM, or otherwise. Thus, the surgeon, or other operator, may advantageously visualize the location of the scanning ISAM beam **162**, relative to tissue structures. The cylindrical-shaped CCD camera unit **164**, when attached to the probe **110**, is either angled slightly, such that its field of view **166** allows visualization of the scanned tissue region **124**, or uses mirrors to view the tissue surface while keeping the camera unit closer to the probe.

[0045] Buttons **115**, **117** within the rigid end **151** of the probe fairing **150**, may provide for electrical or capacitive control, whether by means of wires running back and integrated with the long sheath or via pass-through buttons that when pressed, contact

respective buttons on the probe unit to activate functions such as irrigation/aspiration, CCD video capture, ISAM scan modes, image acquisition/storage, etc.

[0046] Housing **11** of hand-held probe **100** is preferably constructed from machined aluminum or hard plastic, and integrates the optical elements and 2-axis MEMS mirror for near common-path interferometry. Various possible beam splitter configurations are discussed above. The reference path fiber passes through an in-line fiber attenuator **115** and can be adjusted manually via set-screw adjustments **116** on the exterior of the probe. The reference fiber then passes through a fiber-based polarization controller **117** with similar set-screw adjustments **118**. The reference fiber ends with a GRIN lens **112** to collimate light to be reflected off the variable reflectivity mirrors **130** in the probe cover.

[0047] The sample-arm fiber from the coupler is attached to a GRIN lens **106** with right-angle prism **107** to collimate and direct light on to the mirror mounted on the 2-axis MEMS scanner **120**. The MEMS scanner **120** directs this light through a series of lens elements **140**, **142** to focus the light through the distal tip and probe cover **150** and into the tissue **124**. The 2-axis MEMS scanner **120** permits arbitrary scan patterns on the tissue, but the scan patterns are preferably linear/rectangular for 2-D ISAM imaging, square for 3-D ISAM imaging, and cross-shaped, for alignment purposes prior to 3-D imaging.

[0048] This distal end of hand-held probe **110** has an optically transparent front face **109** to allow the sample beam **105** and the reference arm beam **111** to pass through with limited attenuation and dispersion.

[0049] Controls for operating functions of probe can either be integrated in the probe itself, or operated via foot pedal switches or computer console.

[0050] Fiber-optic cable **101** and electrical control and power lines **160** for the MEMS scanner **120** pass out the proximal end of the probe **100**, and run back to the main unit console (not shown). All of the foregoing interconnections to the main unit console are covered by disposable jacket **154** when the probe is being used.

[0051] A surface of probe tip **151** (whether disposable or permanent) may be used as a signal phase reference for image computation. Either back- or front surfaces may serve that purpose, with the back surface reflectively, or anti-reflectively, coated, as appropriate.

[0052] Operation of a probe with a fixed focal plane, in accordance with the present invention, and application of software compensation to computationally move the focus, may

advantageously provide a more compact probe. Operation near the focus and far from the focus are discussed in detail in the Marks '155 Patent. It is to be understood that the probe **110** described herein may also be implemented in an endoscopic or transendoscopic modality within the scope of the present invention.

[0053] The described embodiments of the invention are intended to be merely exemplary and numerous variations and modifications will be apparent to those skilled in the art. All such variations and modifications are intended to be within the scope of the present invention as defined in the appended claims.

[0054] Where examples presented herein involve specific combinations of method acts or system elements, it should be understood that those acts and those elements may be combined in other ways to accomplish the same objective of interferometric tomography. Additionally, single device features may fulfill the requirements of separately recited elements of a claim. By way of specific example, the term “reflective element” need not comprise a distinct component within the scope of the present invention, in that the polished end of a fiber, or a generally transmissive optic, may also provide the reflectivity required to serve as a “reflective element.”

[0055] The embodiments of the invention described herein are intended to be merely exemplary; variations and modifications will be apparent to those skilled in the art. All such variations and modifications are intended to be within the scope of the present invention as defined in any appended claims.

What is claimed is:

1. A tomographic imaging system for imaging a volume within a scattering medium, the system comprising:
 - a. an illumination source for generating an illuminating beam;
 - b. an optical fiber for conveying the illuminating beam generated by the illumination source;
 - c. a beam splitter for splitting the illuminating beam into a sample beam along a sample beam path and a reference beam along a reference beam path;
 - d. a transverse scanning mechanism for scanning a portion of the sample beam across a section of the scattering medium;
 - e. a reflective element for returning a second portion of the illuminating toward reference beam along the reference beam path;
 - f. a detector for detecting return beams from both the reference beam path and the sample beam path and for generating an interference signal; and
 - g. a processor for computationally moving an effective focus of the sample beam without physical variation of focus of the sample beam,wherein the scanning mechanism is disposed within an intraoperative probe.
2. A tomographic imaging system in accordance with claim 1, wherein the sample path is characterized by a fixed focal depth into the scattering medium.
3. A tomographic imaging system in accordance with claim 2, wherein the fixed focal depth is determined in part by a fairing covering at least a portion of the intraoperative probe.
4. A tomographic imaging system in accordance with claim 1, wherein the intraoperative probe is hand-held by an operator.

5. A tomographic imaging system in accordance with claim 1, wherein the intraoperative probe is adapted for endoscopic or laparoscopic manipulation.
6. A tomographic imaging system in accordance with claim 1, wherein the beam splitter is disposed within the intraoperative probe.
7. A tomographic imaging system in accordance with claim 1, further comprising a reflective element for returning the reference beam along the reference beam path.
8. A tomographic imaging system in accordance with claim 7, wherein the reflective element for returning the reference beam is disposed within the intraoperative probe.
9. A tomographic imaging system in accordance with claim 1, wherein the sample path and the reference path coincide in part.
10. A tomographic imaging system in accordance with claim 1, wherein the optical fiber is mode-preserving.
11. A tomographic imaging system in accordance with claim 1, wherein the transverse scanning mechanism is microelectromechanical.
12. A tomographic imaging system in accordance with claim 1, further comprising a fairing covering a portion of intraoperative probe.
13. A tomographic imaging system in accordance with claim 12, wherein the fairing is adapted to serve as a sterile barrier between components of the intraoperative probe and the scattering medium.
14. A tomographic imaging system in accordance with claim 1, further comprising a focusing element disposed within the intraoperative probe for focusing the sample beam into the scattering medium.

15. A tomographic imaging system in accordance with claim 12, wherein the fairing is adapted to provide a fixed offset distance between the focusing element and the scattering medium.
16. A tomographic imaging system in accordance with claim 12, wherein the portion of the intraoperative probe covered by the fairing includes the entirety of the hand-held probe.
17. A tomographic imaging system in accordance with claim 12, wherein the fairing includes a distal tip disposed at an end of the hand-held probe proximate the scattering medium.
18. A tomographic imaging system in accordance with claim 17, wherein the distal tip is substantially transparent to the sample beam.
19. A tomographic imaging system in accordance with claim 17, wherein the distal tip includes a focusing element of the sample beam.
20. A tomographic imaging system in accordance with claim 17, wherein the distal tip is adapted to serve as an optical phase reference for the interferometric tomography system.
21. A tomographic imaging system in accordance with claim 17, wherein a reflective element is integral with the distal tip of the fairing.
22. A tomographic imaging system in accordance with claim 17, wherein a plurality of reflective elements are integral with the distal tip of the fairing.

23. A tomographic imaging system in accordance with claim 1, further comprising a lens disposed within the reference beam path.
24. A tomographic imaging system in accordance with claim 23, adapted for variation of an effective reflectivity of the reflective element by virtue of orientation of the reflective element with respect to a lens disposed within the reference beam path.
25. A tomographic imaging system in accordance with claim 24, wherein the lens is a graded index lens.
26. A tomographic imaging system in accordance with claim 1, wherein the processor is of a kind employing interferometric synthetic aperture microscopy for generating an extended-region image without physical variation of focus of the sample beam.
27. A tomographic imaging system in accordance with claim 1, wherein the processor is further adapted for generating an extended-region image.
28. A tomographic imaging system in accordance with claim 1, further comprising a camera for providing a real-time visual image of a surface of the scattering medium being tomographically imaged.
29. An intraoperative probe for imaging a volume within a scattering medium, the intraoperative probe comprising:
 - a. an optical fiber for receiving an illuminating beam;
 - b. a transverse scanning mechanism for scanning the sample beam across a section of the scattering medium; and
 - c. a detachable sterile fairing extending over an end of the hand-held probe proximate the scattering medium, wherein the sterile fairing includes a distal tip which is substantially transparent to the sample beam.

30. An intraoperative probe in accordance with claim 29, wherein the intraoperative probe is hand-held.
31. An intraoperative probe in accordance with claim 29, further comprising a beam splitter for splitting the illuminating beam into a sample beam along a sample beam path and a reference beam along a reference beam path.
32. An intraoperative probe in accordance with claim 31, further comprising a reflective element for returning the reference beam along the reference beam path.
33. An intraoperative probe in accordance with claim 31, wherein a portion of the distal tip is substantially reflective of the reference beam.
34. An intraoperative probe in accordance with claim 31, wherein the sample beam path and the reference beam path coincide in part, up to substantially an entirety of the respective paths.
35. An intraoperative probe in accordance with claim 31, wherein a single optic transmits the sample beam and reflects the reference beam.
36. An intraoperative probe in accordance with claim 29, wherein the transverse scanning mechanism is microelectromechanical.
37. An intraoperative probe in accordance with claim 31, further comprising an intensity adjustment mechanism for attenuating the reference beam.
38. An intraoperative probe in accordance with claim 31, further comprising a polarization adjustment mechanism for adjusting the polarization of the reference beam.

39. An intraoperative probe in accordance with claim 29, wherein the fairing encloses the hand-held probe in substantial entirety.
40. A disposable fairing for enclosing an intraoperative probe of a tomographic imaging system, the disposable fairing characterized by substantial transparency to a scanning sample beam transmitted from the intraoperative probe to a volume within an imaged scattering medium.
41. A disposable fairing in accordance with claim 40, the fairing having an integral reflector for reflecting a reference beam.
42. A disposable fairing in accordance with claim 40, the fairing including a hard distal tip covering an end of the intraoperative probe proximate to the imaged scattering medium.
43. A disposable fairing in accordance with claim 40, the fairing including a film jacket covering connecting cables that couple the intraoperative probe to a source of illumination and to a detector.

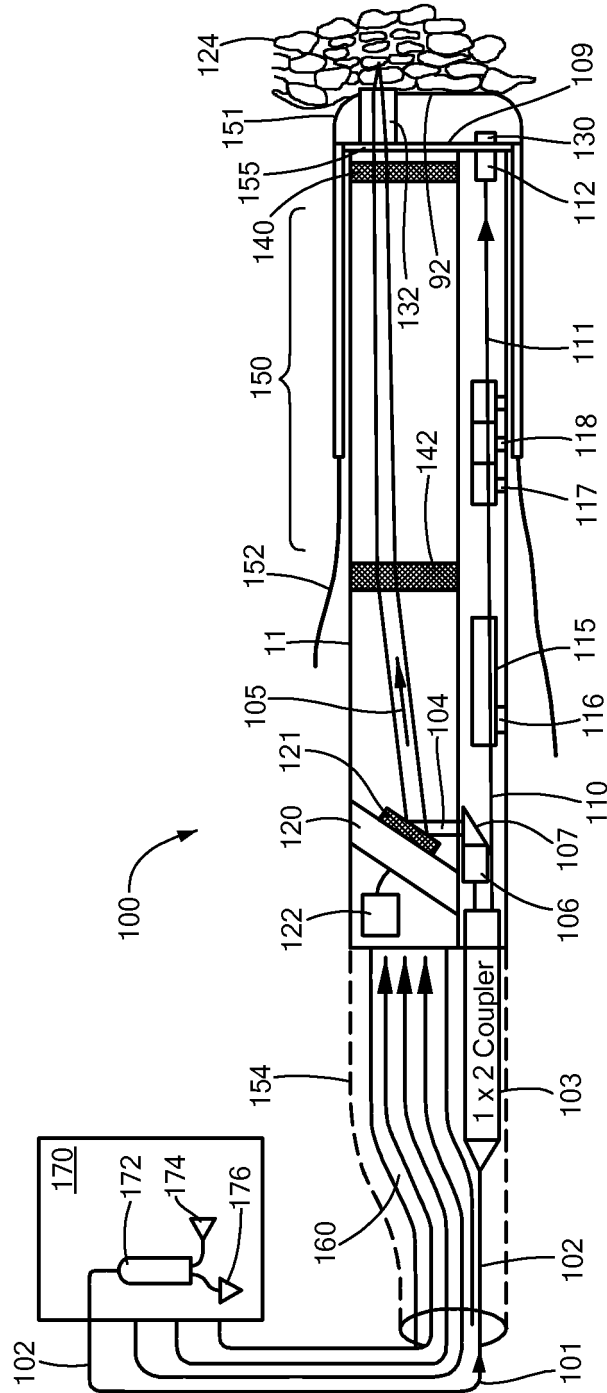


FIG. 1

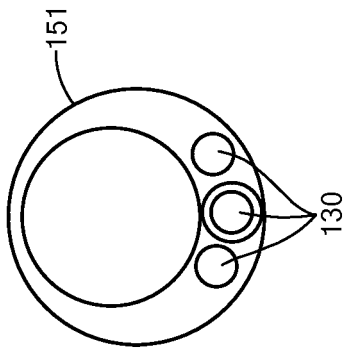


FIG. 2

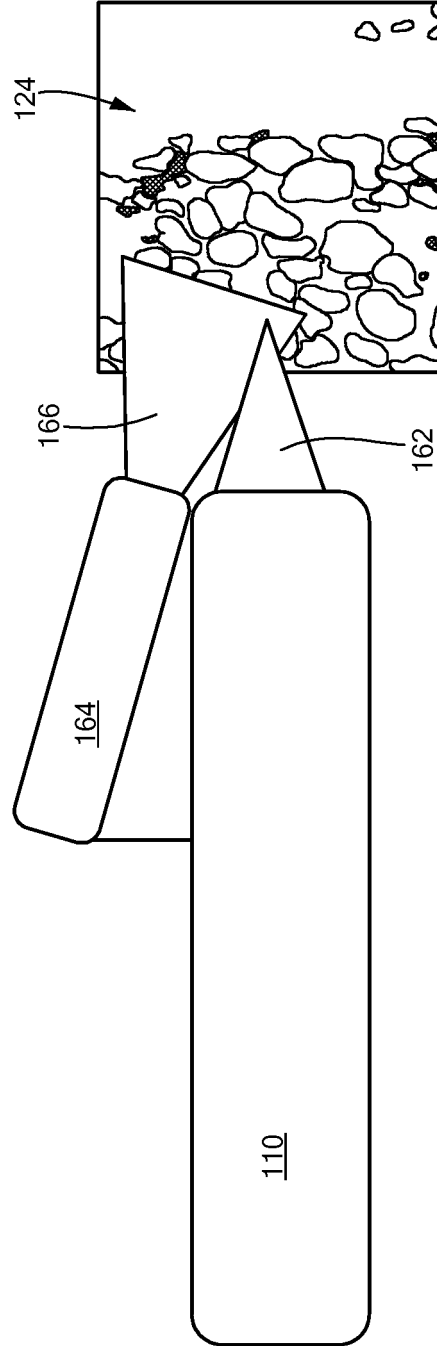


FIG. 3

专利名称(译)	手持式定焦光学探头		
公开(公告)号	EP2680743A4	公开(公告)日	2014-08-13
申请号	EP2012752521	申请日	2012-03-01
[标]申请(专利权)人(译)	诊断PHOTONICS		
申请(专利权)人(译)	诊断PHOTONICS , INC.		
当前申请(专利权)人(译)	诊断PHOTONICS , INC.		
[标]发明人	BOPPART STEPHEN A CARNEY PAUL SCOTT CITTADINE ANDREW		
发明人	BOPPART, STEPHEN, A. CARNEY, PAUL, SCOTT CITTADINE, ANDREW		
IPC分类号	A61B5/00 A61B17/24 G01B9/02		
CPC分类号	A61B5/0066 A61B5/0084 G01B9/0203 G01B9/0205 G01B9/02063 G01B9/02083 G01B9/02091 G01B2290/65 A61B5/0073 G01B9/02 G01B9/02049 G01B9/02054 G01B9/02087 G01B11/00		
代理机构(译)	范尼、PETER JOHN		
优先权	61/448345 2011-03-02 US		
其他公开文献	EP2680743A2		
外部链接	Espacenet		

摘要(译)

术中探针和用于对手术显着体积的组织或其他散射介质进行光学成像的系统。照明光源产生传送到组织附近的照明光束和分束器，其可以是光学相位参考，将照射光束沿着样本光束路径和参考光束分成样本光束。参考光束路径。扫描机构扫描一部分样本光束穿过散射介质的一部分，而检测器检测来自参考光束路径和样本光束路径的返回光束并产生干涉信号。处理器计算地移动样本光束的有效焦点而没有样本光束的焦点的物理变化。探针可具有可拆卸的可消毒整流罩。