

(19)



(11)

**EP 1 945 106 B1**

(12)

**EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:  
**07.11.2018 Bulletin 2018/45**

(51) Int Cl.:  
**A61B 17/10 (2006.01) A61B 17/04 (2006.01)**

(21) Application number: **06803567.4**

(86) International application number:  
**PCT/US2006/035804**

(22) Date of filing: **13.09.2006**

(87) International publication number:  
**WO 2007/033314 (22.03.2007 Gazette 2007/12)**

(54) **SUTURING DEVICE**

NAHTVORRICHTUNG

DISPOSITIF DE SUTURE

(84) Designated Contracting States:  
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IS IT LI LT LU LV MC NL PL PT RO SE SI SK TR**

- **BELMAN, Yuri**  
Mountain View, California 94043 (US)
- **ZATYURYUKIN, Alexander, Borisovich**  
Moscow (RU)
- **MOORE, Patricia, A.**  
Incline Village, California 89451 (US)

(30) Priority: **14.09.2005 US 227981**

(43) Date of publication of application:  
**23.07.2008 Bulletin 2008/30**

(74) Representative: **Clark, Jane Anne et al**  
**Mathys & Squire LLP**  
**The Shard**  
**32 London Bridge Street**  
**London SE1 9SG (GB)**

(60) Divisional application:  
**11192491.6 / 2 441 397**

(73) Proprietor: **Rhaphis Medical, Inc.**  
**Incline Village, NV 89451 (US)**

(56) References cited:  
**US-A- 5 897 563 US-A- 5 938 668**  
**US-A- 5 954 733 US-A- 5 957 937**  
**US-A- 5 993 466 US-A- 6 071 289**  
**US-A- 6 126 665**

(72) Inventors:  
• **HAMILTON, Henry, H.**  
**Hillsborough, California 94010 (US)**

**EP 1 945 106 B1**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

## Description

### BACKGROUND OF THE INVENTION

**[0001]** The present invention relates to a suturing device for use with a suturing needle. In specific embodiments, the devices are provided for suturing tissues in open surgery, minimally invasive surgical procedures, and the like.

**[0002]** Although many aspects of surgery have changed radically over the last several decades, some surgical techniques have remained remarkably constant. For example, as was true fifty years ago, suturing remains a common technique for approximation of tissues, ligation of tissues, affixing tissues together, and the like.

**[0003]** Suture has been used in open surgical procedures for generations to therapeutically treat diseased tissue and to close surgical access sites and other wounds. More recently, the use of minimally invasive surgical techniques has expanded, with surgical therapies often being performed at internal surgical sites. Although a wide variety of visualization techniques (including laparoscopes and other endoscopic viewing devices, fluoroscopy and other remote imaging modalities, and the like) have been developed to allow surgeons to view these internal surgical sites, and although a large variety of new tissue treatment techniques have been developed (including ultrasound techniques, electrosurgical techniques, cryosurgical techniques, and the like) and are now widely available, many modern surgical interventions continue to rely on suturing.

**[0004]** A wide variety of alternatives to suturing of tissues have been developed, and have gained varying degrees of acceptance in certain surgical procedures. Staples and tissue adhesives are used quite frequently in many open and minimally invasive surgical settings, and a variety of tissue welding techniques have also been proposed. Nonetheless, suturing remains ubiquitous in surgery, as suturing provides a number of advantages over many of the alternatives.

**[0005]** Suture's advantages include the large knowledge and skill base that surgeons have developed over the years. Additionally, a variety of off-the-shelf, pre-packaged surgical needles with suture are available from a large number of suppliers at very reasonable cost. Surgeons are able to precisely control the location of suture stitches by grasping the suture needle and first pushing it and then pulling it through the target tissue. In open surgery the surgeon may manually grasp the suture needle directly with his or her hand, although both open and minimally invasive procedures are often performed by grasping the needle with a needle grasping tool and manipulating the tool to place the suture stitches. The results obtained using suture are highly predictable, although dependent on the skill of the surgeon. In light of its advantages, the use of suture does not appear likely to disappear any time soon, with even modern robotic surgical techniques often making use of suture.

**[0006]** Although suture remains popular in surgery at least in part due to its significant advantages, suturing is not without disadvantages. In particular, placing a large number of suture stitches can be tiring and quite time-consuming. Manipulation of a suture needle can be difficult even in open surgery due to the limited space that is often available around the target tissues. The challenges of manipulating suture needles may be even greater in minimally invasive surgical procedures, where the needles are often manipulated using long-handled tools extending through a small aperture, typically while viewing the procedure on a display which is offset from the surgical site. Tying knots with a desired amount of tension and the like may call for intricate and precise manipulation of the suture, further complicating and delaying open and minimally-invasive surgeries. In fact, the time spent closing/suturing the access site may be significantly greater than the time spent treating the underlying target tissues for many procedures.

**[0007]** There have been a variety of proposals for modifications to standard surgical suturing structures and methods to try to address the above disadvantages. At least some of these proposals may seek to rely on specialized and/or proprietary suturing needle systems, which could increase costs and preclude their wide acceptance, especially in third world countries. Unfortunately, many proposals for modifying existing suturing techniques may also decrease the surgeon's control over the placement of the suture, such as by relying on an automated or indirect mechanical movement of a device to drive a suture needle into and/or through tissues. While these new proposals have in the past or may in the future gain varying degrees of acceptance in one or more surgical procedures, standard suturing techniques continue to predominate throughout surgery in general.

**[0008]** In light of the above, it would be desirable to provide improved suturing devices, systems, and methods. It would be generally desirable to maintain some, most, or all of the advantages of standard suturing techniques, preferably while decreasing the time required for suturing, the strain on the surgeon, the training involved in achieving competence or time-efficiency in suturing techniques, or the like. It would be particularly advantageous if these improvements could be provided without requiring extensive capital investments for new equipment, without significant increases in complexity of the suturing process, or without having to resort to specialized or proprietary suturing needles and the like. Alternative needle grasper structures which increased the ease and accuracy of stitching, and/or which are readily adapted for a variety of different procedures and patient physiologies would also be desirable.

**[0009]** US 6126665 discloses an instrument for manipulating anatomical tissue having a barrel with two drivers therein which can be manipulated from a proximal end of the barrel. The end effector of each driver is offset from a shaft by a transverse arm. In an insertion position, the end effectors are confined within the diametrical dimen-

sion of the barrel at a distal end thereof. After insertion, the end effectors can be manipulated by rotationally or arcuately moving the shafts to extend beyond the diametrical dimension of the barrel to provide a large working span in which a tissue procedure can be accomplished.

**[0010]** US 5954733 discloses an instrument for suturing anatomical tissue with a suture needle including a handle, a needle driver mounted by the handle for rotation along a first arcuate path having a radius of curvature commensurate with a radius of curvature of the suture needle, and a needle catcher mounted by the handle for rotation along a second arcuate path coplanar with the first arcuate path and having a radius of curvature commensurate with the radius of curvature of the suture needle. The needle driver and the needle catcher each include needle holding members selectively operable to grasp and release the suture needle.

**[0011]** US 6,071,289 describes a surgical device for assisting a surgeon in suturing bodily tissue using a curved surgical needle with a suture filament attached. The device has a stationary arm having a first holder fixedly attached to and extending from the distal end of the shaft for operationally engaging with the needle. The device also has a moveable arm having a second holder extending from the distal end of the shaft and rotatable about the longitudinal axis of the device. The moveable arm is also operationally engageable with the needle. An actuator is provided for cooperatively activating the first and second holders so as to pass a needle along a circular path transverse to the longitudinal axis of the device through the tissue, and thus place the suture filament into the tissue.

**[0012]** US 5,938,668 describes a surgical suturing apparatus having a pair of jaws extending distally from an elongate tubular portion and each individually longitudinally moveable with respect to the elongate tubular portion and with respect to each other. Each of the jaw structures includes a jaw and a securing mechanism for tightly holding the surgical needle within the jaw. Parts of the securing mechanism engaging the needle also move longitudinally with respect to the associated jaw and the associated tubular portion. Various control structures are provided to advance the securing mechanism relative to its associated jaw to secure the surgical needle therein and to move the entire jaw structure longitudinally with respect to the suturing apparatus.

**[0013]** US 5,957,937 describes an instrument for suturing anatomical tissue with a suture needle in which a needle holder is coupled with a housing for arcuate movement about a longitudinal axis of an elongate tubular member mounted by the housing such that a corresponding distal end of the needle holder is caused to move along an arcuate path extending outwardly of the peripheral edge and having a radius of curvature commensurate with the radius of curvature of the suture needle.

**[0014]** US 5,897,563 describes a method for using a needle holder to assist in the suturing in which the device has right and left arms extending distally from a handle,

the arms having proximal ends attached to the handle and distal ends having grippers attached thereto for gripping and releasing a needle. The device includes at least one mechanism for moving the distal ends of the arms closely adjacent to one another and for passing the needle from one gripper to the other and thereafter moving the distal ends of the arms further apart from one another. The described method involves first moving the distal ends of the arms apart from one another and manually inserting the needle into the tissue and back out again. Thereafter the method involves actuating the mechanism so as to move the arms closely adjacent one another so that the left gripper holds the needle and the right gripper releases the needle. The method then involves moving the distal ends of the arms further apart from one another and lastly removing the needle from the tissue.

#### BRIEF SUMMARY OF THE INVENTION

**[0015]** The present invention is set out in the appended claims. Described herein are suturing devices and methods that maintain some or all of the advantages of standard open and/or minimally invasive suturing techniques while providing enhanced speed and ease of use. Exemplary suturing devices may hold a suture needle at a fixed location relative to a handle of the device, allowing the surgeon to grasp and manipulate the handle so as to insert the needle through the tissues to be sutured in a manner closely analogous to use of a standard needle gripper. Cycling of the handle of the device from a closed position to an open position and back to the closed position may result in the needle being alternately gripped by a first clamp (for example, along a proximal portion of the needle, suitable for insertion of the tip of the needle into and through tissue), and then by a second clamp (for example, along a distal portion of the needle, suitable for pulling the protruding needle out from the tissue), and optionally again by the first clamp (ready for initiation of the next stitch). The needle will often remain at a substantially fixed location relative to the body and handle of the suturing device during at least the insertion and/or pulling of the needle through the tissue, allowing the surgeon to maintain precise control over needle movement and positioning of the suture. Advantageously, standard off-the-shelf suturing needles with their attached suture may be used, and the device may be employed in an open surgical setting or a minimally invasive procedure. Needle grasping devices and methods are also provided which can be bent plastically by a surgeon for use in a particular patient, and/or having advantageous ergonomics for use in surgery, these needle graspers optionally having only a single clamp for grasping of an associated needle.

**[0016]** A suturing method described herein comprises inserting a distal portion of a suturing needle distally through a tissue by moving a body of a suturing device. The body is moved while a clamp of the suturing device holds the needle at a fixed location relative to the body.

The distal portion of the needle is grasped with a second clamp of the suturing device, and the proximal portion of the needle is released from the first clamp. The proximal portion of the needle is pulled through the tissue by moving the body while the second clamp holds the needle.

**[0017]** The second clamp will often hold the needle at a fixed location relative to the body of the suturing device while the needle is pulled free. The needle may also remain at a substantially fixed location relative to the body of the suturing device while alternating the clamps, for example, by grasping the proximal portion of the needle with the first clamp and only then releasing the distal portion of the needle from the second clamp. The inserting of the distal portion of the needle into the tissue with the first clamp, switching clamps, and then pulling the proximal portion of the needle through the tissue with the second clamps can significantly facilitate forming a plurality of suture stitches, and may avoid completely releasing the needle and/or re-aligning the needle with the device each time a stitch is formed. Handing the needle back and forth between the first and second clamps will often be effected by actuating a handle of the suturing device with a hand of a surgeon, the handle typically moving from an open handed configuration to a closed grasp configuration. Preferably, the handle will be in the closed grasp configuration at least while inserting the distal portion of the needle into tissues.

**[0018]** In the exemplary embodiments, cycling the handle (for example, from closed to open, and back to closed) alternates which clamp of the suturing device is supporting the needle from the first clamp, to the second clamp, and back (optionally) to the first clamp. By having both clamps supporting the needle for at least a portion of the handle actuation cycle, unintended movement of the needle relative to the body of the device (and the handle) can be inhibited.

**[0019]** The suturing device body will often include a housing containing a linkage, and the linkage may include an alternatable drive element. The linkage will often drivingly couple the handle to the first and second clamps. With each handle actuation cycle, the alternatable drive element may move back and forth between a first configuration and a second configuration, in its first configuration, the alternatable drive element may drive a first portion of the linkage coupled to the first clamp. In its second configuration the alternatable drive element may drive a second portion of the linkage coupled to the second clamp.

**[0020]** In an exemplary embodiment, the handle actuation cycle may effect rotation of a drive wheel. The first and second linkage portions may each comprise a driven wheel, and the alternatable drive element in the first configuration may drivingly couple the drive wheel with the driven wheel of the first linkage portion. In the second configuration of the alternatable drive element, it may drivingly couple the drive wheel with a driven wheel of the second linkage portion. The alternatable drive element may be, for example, slidingly or pivotally attached

to the drive wheel and may move back and forth so as to engage surfaces of the driven wheels on either side of the drive wheel, with the wheels being driven about a common axis. Other linkage embodiments may employ an alternatable drive element in the form of a slider having alternative positions during axial movement, or the like. Still further alternative linkage embodiments may employ rack and pinion gears and cams, cables, and/or the like, with or without alternatable drive elements.

**[0021]** In many embodiments, the first clamp will be displaced laterally from around an axis of the needle when the second clamp is used to move the needle through tissue. Similarly, the second clamp may be displaced laterally from around the needle when the first clamp is used to move the needle through tissue. Each clamp may, for example, be mounted to an associated shaft, and these shafts may reciprocate so as to extend distally from a housing of the body before closing of the clamp around the needle. In some embodiments, the clamp may also pivot about an axis of the shaft while moving between a retracted position and an extended needle grasping position. A spring or other biasing means may inhibit closing of the clamp before the clamp is properly disposed around the needle, or the linkage may otherwise be configured to extend the shaft before closing of the clamp. In some embodiments, the shafts, clamps, and needle may move axially slightly relative to the housing of the body when the handle is cycled.

**[0022]** Conveniently, a release input may be provided on the suturing device so as to release the needle from both the first and second clamps. The needle may comprise an off-the-shelf needle which is sold primarily for standard open or laparoscopic procedures. These needles often come prepackaged with suture, and are available in a large variety of needle sizes and configuration, suture types (including resorbable and non-resorbable sutures), and the like, often at very modest costs. Alternatively, specialized needles may also be employed. An alternatable latch may optionally maintain either of the clamps closed over the needle during needle manipulation. The body and handle may be configured so that a rigid portion of the body can be comfortably grasped by the hand while a portion of the hand (such as the fingers) articulates the handle, so that inadvertent movement of the body and needle relative to the hand is inhibited. The surgeon may optionally plastically bend a distal extension of the body along its longitudinal axis for use with a particular patient physiology. In such embodiments, drive components within the body will typically be sufficiently flexible to allow operation of the clamps through the bent body

**[0023]** Described herein is a suturing device for use with a suture needle. The device comprises a body having a proximal end and a distal end. A first clamp is disposed near the distal end of the body. A second clamp is also disposed near the distal end of the body. A linkage effects movement of the first and second clamps between a grasping configuration and a displaced configuration.

Each clamp grasps the needle at an associated grasping location in the grasping configuration, and is laterally displaced from the needle in the displaced configuration. The grasping locations are substantially fixed relative to the body.

**[0024]** Described herein is a suturing device for use with a suturing needle. The device comprises a body having a proximal end and a distal end. A handle is disposed near the proximal end of the body. The handle is actuatable from a first configuration to a second configuration and back to the first configuration so as to define an actuation cycle. A first clamp and a second clamp are disposed near the distal end of the body, and the clamps are coupled to the handle so that an actuation cycle initiated while the first clamp is grasping the needle results in grasping of the needle with the second clamp and release of the needle from the first clamp, and (optionally) then in the first clamp grasping the needle and the needle being released from the second clamp.

**[0025]** In yet another aspect, the invention provides a suturing device for use with a suturing needle. The suturing device comprises a body having a proximal end and a distal end, with a clamp extendable distally of the body. Biasing means is coupled to the clamp to urge the clamps closed sufficiently to grasp the needle therein for suturing with the needle. An articulatable handle is disposed near the proximal end of the body, and a linkage couples the handle to the clamp so that manual articulation of the handle opens the clamp to release the needle. Such suturing devices may optionally have only a single needle-grasping clamp.

**[0026]** Described herein is a suturing device for use with a suturing needle. The suturing device comprises a rigid body having a proximal end and a distal end, and a clamp extendable distally of the body. An articulatable handle near the proximal end of the body is configured for manipulation by fingers of a hand while the hand engages the body near the proximal end. A linkage coupling the handle to the clamp so that manual articulation of the handle by the fingers effects opening and closing of the clamp to grasp and release the needle. Only a single clamp maybe provided, or a plurality of clamps, with the device ideally enhancing control over movement of the needle by the hand by inhibiting movement of the needle relative to the hand during opening and closing of the clamp.

**[0027]** Described herein is a method for securing suture using a needle driver. The method comprises placing a suture through a tissue by grasping a proximal end of a needle with the needle driver and inserting the needle into the tissue at a first insertion point. The needle is inserted with the needle driver so that a distal end of the needle protrudes from the tissue at a first exit point. The distal end of the needle is grasped by the needle driver and pulled distally from the tissue, with the suture being coupled to the needle. A first suture loop is formed in the tissue by, after the suture has been placed through the tissue, again supporting the proximal end of the needle

with the needle driver, inserting the needle into the tissue at a second insertion point and removing the needle from a second exit point in a manner similar to that used to first place the suture through the tissue. A second loop is formed in a similar manner, resulting in a third insertion point and a third exit point, and a third loop is also formed. The third loop extends across at least one (and preferably both) of the first and second loops between a third exit point and the fourth insertion point so as to define crossed loops in the suture. The needle is pulled from the fourth exit point sufficiently that the crossed loops secure the suture to the tissue. Advantageously, this knot may be formed without releasing the needle driver from the hand of the surgeon. The needle grasping and driving devices described herein are particularly advantageous for use in this method.

#### BRIEF DESCRIPTION OF THE DRAWINGS

#### **[0028]**

Fig. 1 is a perspective view of a suturing device with one of the clamps of the suturing device grasping a suturing needle.

Fig. 2 is a perspective view of a proximal portion of the suturing device of Fig. 1, with a cover removed from a proximal housing of the suturing device to show a portion of a linkage coupling a handle of the suturing device to the clamps of the suturing device.

Fig. 3 is an exploded perspective view of components of the linkage shown in Fig. 2.

Fig. 4 is an exploded view of a distal portion of the suturing device of Fig. 1, showing components of a clamp along with a reciprocable shaft and elements of the linkage that effect movement of the reciprocable shaft and actuation of the clamp.

Figs. 5-9 are perspective views showing use of the device of Fig. 1 for suturing tissues.

Fig. 10 is a perspective view of an alternative suturing device having first and second clamps which both reciprocate and rotate away from a suturing needle after releasing of the needle from the clamp.

Fig. 11 is an exploded view of the suturing device of Fig. 10 showing some of the components of its drive linkage.

Figs. 12-14 are partially exploded perspective views showing a portion of an actuation cycle of the suturing device of Fig. 10, and showing how the clamps both reciprocate and rotate away from the suturing needle.

Figs. 15-17 are perspective views of components of the suturing device of Fig. 10, showing how rotation of the reciprocable shaft is effected.

Fig. 18 is a perspective view of another an alternative suturing device which holds a suture needle so that an axis of the needle extends along an actuation plane of a handle of the device.

Fig. 19 is a perspective view of a suturing system including the suturing device and needle of Fig. 18, with a cover removed so as to show components of a linkage coupling the actuatable handles of the device to clamps for holding the needle.

Figs. 20 and 21 are detailed views illustrating reciprocable shafts and drive linkages configured to effect movement and actuation of the clamps in the suturing device of Fig. 18.

Fig. 22 is a perspective view of yet another alternative suturing device and system having a drive system including a rack and cams.

Fig. 23 is a perspective view of the suturing device of Fig. 22 with a cover removed so as to show components of the drive system of the device.

Figs. 24A and 24B illustrate an exemplary suturing device in which the clamps are releasably coupled to the body of the device, allowing the clamps to be disposable to avoid cross contamination between differing patients without having to sterilize the clamp structures.

Figs. 25A and 25B are a side view and top cross-sectional view, respectively, of another embodiment of a suturing device having a drive linkage with an alternatable drive element for moving first one clamp and then the other, and also having an alternatable latch for inhibiting movement of the clamp that is not being driven.

Fig. 26 is an exploded view schematically showing some of the components of the drive linkage of the suturing device of Figs. 25A and 25B.

Figs. 26A-26M are cross-sectional views schematically illustrating actuation of the linkage of the suturing device of Figs. 25A and 25B.

Figs. 27A-27C are perspective views of a distal portion of an alternative suturing mechanism in which axially offset clamps alternately grasp proximal and distal portions of a ski-jump suturing needle.

Fig. 28 is a perspective view of an alternative suturing device having a single needle-grasping clamp.

Fig. 29 is a side view schematically illustrating a suturing device similar to that of Fig. 25A in which an extension of the body between the clamps and proximal housing has been manually bent for a particular patient, in which the clamps are actuatable through the bent extension, and which is being grasped by a hand of a surgeon.

Figs. 30A-30D are perspective views schematically illustrating steps in tying a knot, where the knot can optionally be tied by manipulating the two-clamp suture devices described herein without the surgeon releasing the suturing device from his or her hand.

Figs. 31A and 31B schematically illustrate a suture knot tied according to the method of Figs. 30A-30D.

Embodiments can significantly increase the speed and ease of suturing, particularly when suturing of long incisions or where large numbers of stitches are to be deployed.

**[0029]** The invention should find a wide variety of applications for stitching anatomical tissues in both humans and animals. Along with endoscopic operations (for example, in laparoscopy) these structures and methods may find use in other areas of surgery where tissues are to be stitched, providing particular advantages for stitching of large incisions by increasing the ease and speed with which each individual stitch may be placed, as well as facilitating and expediting the formation of knots in the suture. The suturing devices and associated methods described herein may, for example, be used suture a wide variety of strata of anatomical tissues, including (but not limited to) subcutaneous layers, fascia, the outer skin, various organs (including the uterus), and the like. While exemplary embodiments are set forth below, these suturing devices and methods may be applicable to a wide variety of suturing operations, including open surgery, large and small cavity procedures, endoscopic procedures, microsurgeries (including for suturing of veins, arteries, and the like), and many specialized surgeries. Embodiments of these devices may be particularly useful for surgeries involving long incisions, including plastic surgeries. A wide variety of blood vessels, including both veins and arteries, may also be stitched using the techniques described herein, for formation of anastomoses and the like. Along with increasing the speed and/or ease of forming surgical suture stitches, embodiments will often maintain the control a doctor has over the placement of the sutures by maintaining a fixed relationship between the movements of the doctor's hand and the insertion and withdrawal of the suturing needle. Hence, among the procedures which may benefit from the invention are subcuticular peritoneum, fascia closure, and skin closure.

**[0030]** While embodiments may include (or be used within) a powered or automated system, optionally making use of electromechanical power, hydraulic power, or

the like (for example, with some embodiments being included within a robotic system), other embodiments may be configured for manual manipulation by one or more hands of a surgeon, often without having to resort to complex subsystems or external power.

**[0031]** Many embodiments of the devices described herein will be sterilizable so as to allow repeated use. Sterilization may be effected using autoclave techniques, chemical sterilization, irradiation, or the like, with most or all of the structures of the suturing device being formed of materials suitable for repeated sterilization (such as stainless steel, other metals and alloys, and the like). In general, the suturing device may comprise one or more plastics and/or metals common to surgical devices. Although specialized or proprietary suturing needles may be employed in some embodiments (for example, needles having flat gripping surfaces so as to maintain an alignment between the needle and an associated clamp), many embodiments of the suturing device will be suitable for use with standard off-the-shelf suture needles such as those packaged with any of a wide variety of permanent or resorbable suture materials in a hermetically sealed package. In fact, the invention may find some of its most immediate applications for facilitating surgical procedures performed manually in Third World countries, allowing physicians to treat a larger number of patients with greater ease than can be done using standard suturing techniques, but without the cost or complexity of recently-proposed automated suturing systems.

**[0032]** Referring now to Fig. 1, an exemplary suturing system 100 generally includes a suturing device 102 and a needle 1. Needle 1 generally has a proximal end 104 and a distal end 106, with at least the distal end being sharpened to facilitate insertion of the needle distally into and through tissues. Surgical needles are often formed with a curving shape between the proximal and distal ends, and are often packaged with a suture extending from proximal end 104, with the needle sometimes being referred to as an acus.

**[0033]** Suturing device 102 generally has a body 112 having a proximal end 108 and a distal end 110. A pair of clamps 3 are disposed near the distal end 110, while first and second handles 6, 8 are disposed near proximal end 108. Body 112 may include a proximal housing 7 and a distal extension 4. The distal extension may have a pair of channels, with each channel reciprocatably receiving a shaft 2 supporting an associated clamp 3.

**[0034]** In this exemplary suturing system, clamps 3 are mirror-symmetric, although they may alternatively have differing shapes. Clamps 3 are generally offset so as to grip axially offset portions of needle 1, with one of the clamps gripping a more proximal portion of the needle and the other clamp gripping a more distal portion of the needle. When handles 6, 8 are in a close-handed configuration as illustrated in Fig. 1, only one of clamps 3 will typically grip needle 1, the other clamp being retracted proximally away from the needle. Handles 6, 8 have openings for receiving fingers of the surgeon's hand, and

the surgeon will typically actuate the handles by opening them from the closed-handed configuration shown to an open-handed configuration 114. Starting with handles 6, 8 in the closed (as shown in Fig. 1), when the handle is moved to open-handed configuration 114 and is then returned to the closed-handed configuration, the handle may be described as having completed an actuation cycle.

**[0035]** With each actuation cycle of handles 6, 8, the clamp 3 supporting needle 1 is alternated so that a needle initially supported by grasping the needle in first clamp along a proximal portion of the needle will, when handles 6,8 are in open-handed configuration 114, instead be supported by the second clamp along a more distal portion of the needle. As handles 6,8 move back to the closed-handed configuration to complete the cycle, the clamps again alternate, so that closing of the handle results in extension of the proximal clamp, gripping of needle 1 with that proximal clamp, release of the needle from the distal clamp, and retraction of the distal clamp. The position of needle 1 relative to body 112 may remain substantially fixed throughout the handle actuation cycle, although the shafts may move axially slightly as the needle goes from being held by one clamp, to both clamps, and then to the other clamp, with this movement of the needle being less than a length of the needle.

**[0036]** Referring now to Figs. 1 and 2, handles 6, 8 are pivotally attached to housing 7 of body 112. Housing 7 generally includes at least one lid 9 (the top lid shown removed in Fig. 2), with the proximal housing preferably including opposed first and second lids 9 on opposed major surfaces of the body. Lids 9 and the other structures of housing 7 generally enclose a drive linkage 116 coupling handles 6, 8 to clamps 3. In the example of Figs. 1-9, drive linkage 116 generally includes a drive wheel 11 and two driven wheels 10 and 12. The driven wheels 10 and 12 are mirror-symmetric and joined by tie rods 14 and 21 to clamps 3.

**[0037]** Referring now to Figs. 1-3, driven wheel 10 has a thrust surface 24, while driven wheel 12 has a stop surface 23 and an incline 22. The driving wheel is supported so as to rotate about an axle 20, the driving wheel also having a lug 13. The driving wheel 11 is coupled to handles 6, 8 by ties 18 and 19, so that actuation of the handles relative to the body 7 induces rotation of driving wheel 11 about the axle. The driven wheels 10, 12 rotate coaxially with driven wheel 11.

**[0038]** Lug 13 generally comprises an alternatable configuration driving element. Lug 13 either drivingly couples driving wheel 11 with driven wheel 10, or with driven wheel 12, depending on the configuration of lug 13 at the time. More specifically, when lug 13 is disposed above a guide 15 as shown in Fig. 2, the lug drivingly couples the driving wheel 11 with the upper driven wheel 10. When lug 13 is disposed below guide 15, the lug drivingly engages driven wheel 12, and is disengaged from driven wheel 10. A reset or release input button 16 interacts with guide 15 and a spring-loaded positioning arm 17 so as

to allow both clamps 3 to release needle 1.

**[0039]** As can be understood with reference to Figs. 1-4, each clamp 3 is connected by an associated shaft 2 to the remaining components of drive linkage 116. Shafts 2 each include a lengthwise slot 118 (see Fig. 4), which allows the shaft to move within the channels of body extension 4. Guiding pins 32 ride in slots 118, and the guiding pins 32 are also fixed in extensions 4 within openings 5.

**[0040]** Moving wedges 31 within shafts 2 also have lengthwise slots 118 for receiving guiding pins 32. The wedge surfaces of moving wedges 32 engage corresponding surfaces of working jaws 25, with the working jaws forming the open and closable structure of clamps 3. More specifically, distal movement of moving wedge 31 against a corresponding surface of working jaws 25 closes clamps 3, the working jaws being attached to a distal clevis of shaft 2 by axle 27. A spring ring 30 biases working jaws 25 to an open configuration, allowing them to move around and capture needle 1 before the working jaws are forced shut by the moving wedges.

**[0041]** Working jaws 25 may have a variety of surfaces for holding needle 1, the clamps preferably holding the needle so that movement of the needle relative to suturing device 100 is inhibited during stitching. The surfaces of working jaws 25 may be hardened by deposition of diamond or a diamond-like carbon, or inserts 26 of a material harder than that of working jaws 25 may be provided. Optionally, working jaws 25 may have hard-surfaced inserts comprising tungsten and/or cobalt, with the inserts optionally being fabricated using powder sintering or the like.

**[0042]** A return spring 29 extends between pin 28 in working jaws 25 and the guiding pin 32, with the return spring partially fixed within a lumen of moving wedge 31. A spring 34 in the proximal portion of moving wedge 31 is held by a plug 37, with the distal end of spring 34 interacting with shaft 2 via thrust ring 33. Spring 34 can bring the moving wedge 31 into a position suitable for releasing the working jaws. A compensation spring 36 pressed against plug 37 writes on a rod 35 of a pusher 42 so as to maintain a desired axial force. Pusher 42 has an insert 40, which is connected with the pusher 42 by pin 39 and lug 38. The lug rotates about axle 41.

**[0043]** When handles 6 and 8 are moved apart to an open-handed configuration 114, a retracted clamp 3 and its associated shaft 2 moves from within a channel of body extension 4. While retracted, the moving wedge 31 is biased by spring 34 away from working jaws 25, so that spring ring 30 is free to open the clamp to allow it to extend around needle 1. Extension of compensating spring 34 may be at its greatest point while the associated clamp 3 is retracted, and insert 40 extends from pusher 42 with lug 38 in the insert.

**[0044]** As handles 6 and 8 are brought together, driving wheel 11 is turned by connector ties 18, 19. Lug 38 interacts with thrust surface 24 of driven wheel 10 and moves the driven wheel 10 in rotation. The motion of

driven wheel 10 is transferred by tie rod 14 so as to move insert 40 axially along body extension 4. The insert, in turn, moves the pusher 42 along body extension 4, the relative position of the insert 40 and pusher 42 being maintained by an inner surface of shaft 2 interacting with plug 30 so as to inhibit rotation of the plug about axle 41. Pusher 42 presses spring 34 and compensation spring 32, and via plug 37 and thrust ring 33, moves shaft 2. The movement of shaft 2 overcomes spring 29 and extends the shaft from the channel of body extension 4.

**[0045]** During distal movement of pusher 42, spring 34 and compensating spring 36 are sufficiently stiff so as to inhibit elongation, as their spring coefficients are significantly higher than that of return spring 29. However, engagement between an end of slot 118 in shaft 2 and guiding pin 32 eventually inhibits further distal movement of the shaft.

**[0046]** Once shaft 2 has stopped its distal movement (due to engagement of lengthwise slot 118 with guiding pin 32), spring 34 begins to contract, its rigidity being lower than that of compensating spring 26. As a result, moving wedge 31 begins to extend distally relative to working jaws 25, the corresponding surfaces of the wedge and working jaws sliding against each other so as to move the proximal ends of the working jaws apart and bringing the distal needle gripping inserts 26 of working jaws 25 together so as to grasp needle 1. As spring 34 contracts, contraction of compensation spring 36 also begins and the insert 40 moves. When lug 38 extends into and/or engages window 2a of shaft 2, pusher 42 engages a surface of body extension 4 or proximal housing 7, and axial movement of the pusher stops. Insert 40 continues moving, so that lug 38 rotates around axle 41. The lug interacts with an edge of shaft 2 and, overcoming compensation spring 36, starts to draw shaft 2 and its contents into body extension 4.

**[0047]** The clamping force on needle 1 by clamps 3 may be determined by the spring characteristics of compensating spring 36 so as to remain within a desired range. Advantageously, the clamping force imposed by suturing device 100 on needle 1 may correspond to forces applied by standard needle holders. Thrust surface 23 of driven wheel 12 approaches a tooth of spring-loaded fixing arm 17, and overcoming the spring, the thrust surface passes under the tooth, releasing the tooth so that the tooth and thrust surface are positioned for neutral engagement. After the thrust surface 23 of the driven wheel 12 passes beyond the tooth of spring loaded fixing arm 17, engagement of the thrust surface and tooth inhibit the return of the driving linkage 116 to its prior configuration, thereby inhibiting the release of needle 1 from the closed working jaws 25 so that the needle is not dropped.

**[0048]** As handles 6, 8 continue to move toward the open-handed configuration of the handle actuation cycle, movement of driven wheel 12 is inhibited by spring-loaded fixing arm 17. Driving wheel 11 nonetheless turns, and is reset. More specifically, incline 22 of driven wheel 12 moves lug 13 from a configuration above guide 15 to

a configuration in which the lug is disposed under the guide. Hence, when handles 6, 8 continue to move, here towards a closed-handed configuration, the lug 13 will interact with thrust surface 24 of the driven wheel 10. The description above regarding driven wheel 12 is thus repeated but with driven wheel 10 instead. When moving under the spring-loaded fixing arm 17, the thrust surface 23 of driven wheel 12 lifts the spring-loaded fixing arm 17 and releases driven wheel 10.

**[0049]** By action of spring 34, moving wedge 31 is retracted proximally from between the proximal ends of working jaws 25, so that the proximal ends of the working jaws are brought together by spring-loaded ring 30. Distal ends of working jaws 25 thereby move apart and the needle is released.

**[0050]** Each repeated opening and closing actuating cycle of handles 6, 8 alternates the needle between being held by one, and then the other of clamps 3, and often back to the first clamp. In other embodiments, each handle actuation cycle effects transfer of the needle from one clamp to the other, with the needle returning to be held solely by the first clamp only with a second handle actuation cycle. Regardless, during each cycle each retracted clamp is preferably extended around an associated portion of needle 1 and is closed before the previously extended clamp opens, so that the needle is held continuously by at least one of clamps 3 throughout the handle actuation cycle.

**[0051]** If it is desired to release needle 1 from suturing device 112 at any time during, before, or after a handle actuation cycle, release can be effected by pressing on release input button 16. Pressing on button 16 causes spring-loaded fixing arm 17 to lift away from driven wheels 10 and 12, thereby resetting the clamps in their proximal opened configuration.

**[0052]** Referring now to Figs. 5-9, the use of suturing device 102 for suturing an incision I in tissue T can be understood. Initially, handles 6, 8 (see Fig. 1) are in a closed-handed configuration and the handles are grasped by a hand of a surgeon. Needle 1 is supported by a first clamp 3a, with the first clamp grasping a proximal portion of the needle adjacent a suture S. The second clamp 3b is retracted proximally away from needle 1, so that a distal portion of the needle is free and exposed, as illustrated in Fig. 5.

**[0053]** As can be understood with reference to Fig. 6, the surgeon manually moves suturing device 102 by manipulating handles 6, 8 so as to insert a distal portion of suturing needle 1 through tissue T. Advantageously, body 112 and linkage 116 (see Fig. 2) of suturing device 102 inhibits relative movement of needle 1 relative to the body and handles 6, 8 of the suturing device while the handles are closed. This allows the surgeon to precisely control movement of the needle 1 as it is inserted through the tissue, in a manner analogous to manual manipulation of the needle using a standard needle grasper or forceps. As can be understood with reference to Figs. 6 and 7, once the distal portion of needle 1 extends suffi-

ciently through the tissue, handles 6, 8 can be cycled through at least a portion of their actuation cycle. Through the linkage 116, second clamp 3b is extended distally from body 112 of suturing device 102, grasping the distal portion of needle 1. The first clamp 3a then releases needle 1 and is withdrawn proximally from around the needle, as illustrated in Fig. 8.

**[0054]** As can be understood with reference to Figs. 8 and 9, once needle 1 is held by second clamp 3b, the surgeon can again manipulate the needle by moving handles 6, 8. In some embodiments, the surgeon can grasp the handles in an open-handed configuration while pulling the needle free from the tissue, while in other embodiments the needle will be pulled after the handle has returned to the closed-handed configuration. Regardless, the surgeon uses the handles, body, and clamp 3b to pull the proximal portion of needle 1 through tissue T, thereby leaving suture S inserted across incision I.

**[0055]** Prior to initiating a second stitch, the surgeon can cycle handles 6, 8 by closing the handles with his/her hand, or by opening and closing the handles through a full actuation cycle. This results in grasping of needle 1 by first clamp 3a and release of the needle by second clamp 3b, exposing the distal portion of the needle and displacing the second clamp from the needle so that the needle is ready to again insert through tissue T, as can be understood with reference to Fig. 5. The process can then be repeated without ever having to completely release needle 1, and by simply actuation of handles 6, 8 after insertion of the distal portion of the needle through the tissue and again after each pulling of the needle free. The process is repeated to form as many stitches as is desired. Analogous insertion of the distal portion of the needle through loops of suture, actuation of the handle, and pulling the needle free can be used to quickly and easily form knots.

**[0056]** As can be understood from the illustrations in Figs. 5-9, and as may be indicated by the detailed description above of the articulation of the drive linkage, shafts 2 extending distally from body 112 to clamps 3a, 3b may move slightly during the handle actuation cycle, for example, with the shaft supporting the clamp initially holding needle 1 retracting slightly into body 112 as the other shaft extends. Nonetheless, each clamp holds the needle at a fixed location while the surgeon holds the handles 6, 8 in the closed configuration and inserts or withdraws the needle into or from the tissue.

**[0057]** Referring now to Figs. 10-22, a wide variety of alternative linkage mechanisms, clamp structures, housing, handles, and the like may be employed. Referring first to Fig. 10, an alternative suturing device 130 may include clamps 43, 44 which both retract proximally and rotate away from needle when not used to hold the needle. Referring now to Figs. 10-17, and avoiding describing structures which are substantially similar to those described above, clamps 43 and 44 have bent-shaped inserts 54 made of a hard alloy (see Fig. 15). Proximal ends of clamps 43 and 44 may have conical surfaces 55

which are located, sized, and configured so as to interact with a distal port of shaft 47, and more specifically, so that proximally withdrawing the working jaws of clamps 43, 44 into sleeve 47 closes the working jaws of these clamps.

**[0058]** Shaft 47 has a lengthwise slot 52 for receiving a guiding pin, while a proximal extension of the working jaws of clamps 43, 44 has a spiral lengthwise slot 51 receiving guiding pin 48. Shafts 47 are connected with pushers 53, and ride in distal body extension 45, with the distal body extension again having openings for receiving the guiding pins.

**[0059]** In alternative suturing device 120, as the guiding pins 45 ride within spiral slot 51 due to axial motion of clamps 43, 44, the clamp rotates away from a needle 1 about the axis of shaft 47 when the clamp retracts proximally.

**[0060]** The rotation of clamps 43, 44 with axial movement of shafts 47 as effected by actuation of handles 6, 8 can be understood with reference to Figs. 12-13. As can be seen in Fig. 12, a first rotatable clamp 43 holds a proximal portion of needle 1 while handles 6, 8 are in a closed-handed configuration, while second rotatable clamp 44 is both withdrawn proximally and rotated clear of the needle. As the handles begin to open, as illustrated in Fig. 13, distal movement of shaft 47 of second rotatable clamp 44 imparts a twisting motion to the clamp due to the interaction between the guiding pin 48 and the helical slot 51 (see Fig. 11). The second rotatable clamp 44 can rotate into position and extend around needle 1, with the second clamp 44 grasping needle 1 and first clamp 43 withdrawn proximally and rotated free from the needle when the handles are in their fully opened configuration. Once again, a full actuation cycle from a closed configuration to an open configuration and back to a closed configuration may result in the needle alternating from being grasped by the first clamp along a proximal portion of the needle, then being grasped by the second clamp along a more distal portion of the needle (with the handles in the open configuration), and with the needle again being grasped solely by the first clamp when the handles are returned to the closed configuration. The structure and rotation of rotatable clamps 43, 44, along with the associated interaction between shaft 47 and guiding pin 48 are also illustrated in Figs. 15-17.

**[0061]** Referring now to Figs. 18-21, a still further alternative suturing device 140 has first and second clamps 142, 144 formed by working jaws 56, 57 connected at an axle 58. The shafts supporting clamps 142, 144 here comprise flattened structures 60 located within channels of body extension 61. Shafts 60 interact with rods 67 of pusher 63. This linkage couples handles 62 to clamps 142, 144 using a moveable rod 65 and an immovable fixing arm 66, along with a flat spring 64. Rods 67 of pushers 63 have inclines 68 which function to open and close the clamps, as can be understood with reference to Figs. 20 and 21.

**[0062]** Note that in example 140, needle 1 generally

extends along a plane of actuation of handle 62. In contrast, in suturing device 102, illustrated in Fig. 1, needle 1 generally extends across the handle actuation plane. Ergonomically, there may be advantages in orienting the needle so that it traverses the handle actuation plane as shown in Fig. 1. Such a configuration may conveniently be used by either a right hand or a left hand of the surgeon, although embodiments configured for use by only one or the other may also be provided.

**[0063]** Referring now to Figs. 22 and 23, yet another alternative suturing device 160 has an external appearance somewhat similar to suturing device 140 of Figs. 18 and 19, but makes use of a significantly different linkage mechanism for coupling handle 72 to clamps 69, 70. The clamps again extend from associated channels in body 71, but the linkage here makes use of a rack 77 actuated by a rod 84.

**[0064]** First clamp 69 has elongate levers 73 and 74, while second clamp 70 has levers 75 and 76. Tie rods 83 and 85 axially actuate rack 77 via rod 84, resulting in rotation of cams 78, 79, and large cams 81, 82. The large cams axially extend associated levers 74 and 75 so as to axially extend their associated clamps, while a spring 80 proximally withdraws the clamps when allowed by their cams. The small cams open and close the clamps via levers 73 and 76, with the levers generally acting as followers along the cam surfaces.

**[0065]** Referring now to Figs. 24A and 24B, an alternative suturing device system 202 may include many functional components which are similar to those described above, but can generally be separated into a reusable drive unit 204 and a disposable clamp unit 206. A releasable coupler 208 releasably couples clamp unit 206 to the drive unit 204. The exemplary coupler includes an interface that provides rigid coupling between extensions 210 of the clamp unit 206 and proximal housing 212 of drive unit 204, and also provides moving engagement surfaces between the shafts of the clamp unit and axially moving elements of the drive linkage. While the exemplary releasable coupler 208 includes axial positioning surfaces (in the form of a pin of drive unit 204 and corresponding aperture of clamp unit 206) and a releasable latch to avoid inadvertent decoupling, a wide variety of alternative releasable couplers might also be employed. The exemplary clamp unit includes two clamps. In some embodiments, each clamp may be individually attached to a drive unit 204. Regardless, allowing the clamps to be detached from the drive unit can avoid any need for making the clamps sterilizable, decreasing overall costs of the suturing system and helping to ensure that cross-contamination between patients is inhibited. A plurality of clamp units 206 will often be used with each drive unit 204, with each clamp being used for a single patient and then being disposed of.

**[0066]** A suturing device embodiment 220 can be seen in side and cross-sectional top views in Figs. 25A and 25B. An elongate extension 222 coupling proximal housing 224 to clamps 226 may facilitate use of suturing de-

vice 220 in endoscopic surgery or the like. In this embodiment, actuation of drive linkage 228 is generally effected by movement of a single articulatable handle 230a relative to a grasping base 232 that is affixed to proximal housing 224. By allowing the surgeon to grasp a structure that remains rigidly affixed relative to the suturing device body with one portion of the hand, and articulate handle 230a with the fingers of that hand, the overall position of suturing device 220 (and clamps 226, along with any needle supported therein) can be accurately maintained. As with the other embodiments described herein, a release 233 will often be provided that, when actuated, releases a needle from both clamps and sets the two clamps in a needle-receiving configuration.

**[0067]** The components and use of drive linkage 228 of suturing device 220 can be understood with reference to Fig. 26 and Figs. 26A-26M. As generally described above, drive linkage 228 includes an alternatable drive element 230 for alternating the driving of first one and then the other of the two clamps. Additionally, drive mechanism 228 includes an alternating latch or anchor 232 for inhibiting axial movement of the clamp that is not currently being driven. Drive linkage 228 further makes use of a channel casing 234 in which a movable tubular shaft 236 slides along an axis 238. First and second pushers 240, 242 and a cone with a rod 244 are disposed along axis 238, while a striker 246 and a stop pin with a spring 248 are disposed off of axis 238.

**[0068]** Reviewing the sequence of actuation of these components schematically, Figs. 26A shows the components of drive linkage 228 at a beginning configuration (such as after actuation of the release), with both clamps 226 in a configuration that is open and ready to receive a needle. In Fig. 26B, alternatable drive element 230 drives a first shaft 236 distally along its axis till the shaft engages pin 248. Needle 250 is disposed within the clamp, with the alternatable drive element 230 continuing to move axially with movement of the handle.

**[0069]** In Fig. 26C, continuing movement of drive element 230 has produced axial movement of pin 248 so as to compress its spring, so that the pin stops moving axially. As a result, continuing movement of drive element 230 does not produce additional movement of shaft 236, but instead causes the cone with its rod 244 to move within the shaft 236 till it reaches its distal position, as shown in Fig. 26D.

**[0070]** Additional movement by drive element 230 results in axial movement of pushers 240, 242, causing the striker 246 to move into alignment with a window in the shaft 236, and thus allowing the striker to engage and reposition latch 232. As the reconfigured latch 232 inhibits proximal movement of shaft 236, the handle may be returned (often to its extended position, as can be understood with reference to Fig. 26F) without movement of shaft 236.

**[0071]** Once the handle returns to its starting or extended position, needle 250 may be inserted into and through the tissue. Returning of the handle also recon-

figures alternatable drive element 230 to engage the other, previously non-driven clamp actuation components, with the other shaft 236 again moving distally along its axis due to movement of the handle to engage and compress pin 248 (as seen in Figs. 26H and 26I), inducing axial movement of the cone and rod 244 and allowing the associated striker to again reconfigure the alternatable latch 232 (see Figs. 26J and 26K). Reconfiguring the latch allows the extended, non-driven clamp 226 to retract proximally to the configuration shown in Fig. 26L under the influence of its proximal return spring, this retraction optionally occurring quite quickly. The handle may now again be released, with the reconfigurable drive element 230 again being reset to alternate the driven and latched clamps, as shown in Fig. 26M.

**[0072]** Structures and methods which inhibit gradual displacement of needle 250 relative to suturing device 220 during repeated cycling of drive linkage 228 can be understood with reference to Figs. 26I and 26K. As each clamp 226 is extended to grasp needle 250, the clamp advances distally slightly beyond the eventual location at which the clamp will hold the needle for suturing. This stresses and/or displaces the needle slightly, and the clamp then grasps the needle at the extended location. The extended location will typically be less than 20 diameters of the needle past the other clamp, typically being a few needle diameters distal of the other clamp (smaller needles generally employing smaller stress-inducing distances). The grasping clamp that is to retain needle 250 is retracted slightly to the grasping location and the other clamp is opened, so that needle 250 is positioned for the next cycle, i.e., so that the other clamp will again stress the needle before it is grasped. This slight alternating overshoot during grasping of the needle helps maintain the needle near the proximal end of the grasping jaws during cycling. The needle may also be manually pre-angled by the surgeon, either proximally or distally, to facilitate proximal or distal suturing. For example, the distal tip of the needle may extend or angle distally of the grasping clamps, rather than the needle being disposed perpendicular relative to the axes of the shafts. Cycling of drive linkage 228 will largely reproduce and maintain the grasping angle as the clamps alternately grasp the needle, with some gradual trend toward a perpendicular needle induced by the alternating overshoot during large numbers of actuator linkage cycles (for example, with movement of the distal portion of the needle proximally along the jaws by a few needle diameters or less with each cycle). Hard metal inserts with small protrusions or teeth along the grasping jaw surface may also be beneficial to limit inadvertent movement of the needle relative to the jaws.

**[0073]** Referring now to Figs. 27A-27C, a wide variety of alternative suturing device clamping arrangements may also be employed. An axially concentric suturing device 260 is particularly well suited for use with a ski-jump needle 262. Such needles may comprise a proximal straight section and a distal curving section, and may be

commercially available from a number of suppliers with suture affixed thereto (not shown). A proximal clamp 264 and distal clamp 266 have clamping jaw members which separate and rotate away from needle 262 to allow the needle to be inserted into tissue (in the configuration of Fig. 27A). The drive system may transfer the needle between the two clamps (Fig. 27B), and allow the needle to be pulled distally free of the tissue (in the configuration of Fig. 27C), with the clamps opening and closing with the cycling of a handle using drive elements that may be similar to, analogous to, or quite different than at least some of the drive components described above.

**[0074]** Referring now to Fig. 28, an alternative suturing device 270 may make use of many of the drive components described above, but may include a single clamp 272. Rather than passing a needle back and forth between two clamps, suturing device 270 may be used in a manner analogous to standard needle drivers, and may be particularly well suited for use in the endoscopic or other minimally invasive surgeries.

**[0075]** Fig. 29 schematically illustrates a suturing device 280 similar to that of Figs. 25A and 25B, with extension 282 between clamps 284 and proximal body housing 286 here having a bend 288. While such suturing devices may optionally be sold in a pre-bent configuration, bend 288 may alternatively be imposed by a surgeon, with the surgeon manually (or optionally, with the assistance of one or more tools) bending the extension (or another structure supporting the clamps) to a desired configuration for use in a surgical procedure on a particular patient. Extension 282 may be formed of a material (typically comprising a metal or polymer) which can withstand bend 288 while maintaining structural integrity of the suturing device, and the drive components which move within bend 288 (such as the axially movable shaft, rod with a cone, or the like) may be formed of a material (or having a configuration) which can accommodate lateral deflection within the bent tubular extension during the actuation, such as by forming drive components of a suitable polymer, making use of at least a portion of the drive components which are formed as a helical coil, including thin, flexible sheet metal components, or the like. In general, reconfiguring the drive components or support structures to employ bent sheet metal parts may also help reduce manufacturing costs, and the like. Hence, the shaft may (for example) comprise a sheet metal structure with end tabs having openings to receive components therein, and/or the like. The positive control or positioning of clamps 284 which can be available using a grasping base that's originally affixed to the body housing 286 when suturing device 280 is held by a hand H of a surgeon can also be understood with reference to Fig. 29.

**[0076]** Referring now to Figs. 30A-30D and Figs. 31A and 31B, methods for tying a knot 302 can be understood. Knot 302 may be particularly advantageous for tying with any of the suturing devices described herein, and may also be employed with other needle drivers and/or suturing devices.

**[0077]** As seen in Figs. 30A and 30D, a first tissue portion T1 may be affixed to a second tissue portion T2 using a needle 304 and a suture 306 affixed thereto. The needle has a sharpened distal end and suture 306 is affixed to a proximal end of the needle, with the needle and suture typically comprising any of the commercially available surgical structures. The needle is inserted distally through the tissue portions as shown in Fig. 30A, for example, on either side of an incision or the like, with the needle entering the tissue at a first insertion point 308a and exiting the tissue at a first exit point 310a. A first clamp of the suturing device may effect movement of the needle from the proximal end portion during insertion, while a second clamp of the suturing device may grasp and pull the distal end portion while the needle is pulled from the tissue, as explained above. The suturing device or other needle driver will not be shown for simplicity.

**[0078]** As seen in Fig. 30B, a first loop 312a is completed by again passing the needle through the tissue T1, T2, with the needle entering the tissue at a second insertion point 308b and exiting from a second exit point 310b that are near the first insertion point and first exit point, respectively. As seen in Fig. 30C, a second loop 312b is similarly formed using an adjacent third insertion point 308c and third exit point 310c.

**[0079]** Referring now to Figs. 30D and 31B, a third loop 312c (with associated fourth entry point 308d and fourth exit point 310d) are formed, with the external portion of the third loop crossing an exposed portion of at least one of the first loop 312a and the second loop 312b. Third loop 312c preferably crosses both first loop 312a and second loop 312b, as shown. Additional loops may be formed before, between, and/or after the first, second, and third loops 312a-312c, and the suture loops may be pulled tight after each is formed or only after more than one is formed.

**[0080]** After forming of the third loop, the needle and/or suture distal of the third loop is pulled sufficiently tight to bring the crossing sutures into firm engagement. The suture tension on the outer third loop presses against the inner first and/or second loop, which is counteracted by the compression of the encircled tissue within the inner loops. This, with the friction between suture and the tissue, can effectively anchor the suture to the tissue and prevent axial movement of the suture when the suture proximal of knot 302 is pulled proximally, and/or when the suture distal of the knot is pulled distally.

**[0081]** Advantageously, knot 302 can be tied using motions similar to those used to form basic stitches, preferably without having to remove a needle driver or grasper such as the suturing devices described herein from the hand of the surgeon, optionally using only one hand of the surgeon (often that holds the suturing device) to completely form the knot. Additionally, deleterious abrasion of the suture (such as that which can occur when other knots are tied away from the tissue and then moved down the suture to the tissue) can be reduced or effectively eliminated.

**[0082]** While exemplary embodiments of the invention have been described in detail, by way of example and for clarity of understanding, a variety of modifications, changes, and adaptations will be obvious to those of skill in the art. For example, along with the exemplary drive linkages described herein, still further drive linkages may be provided, including those making use of cables and pulleys, worm gears, and the like. Hence, the scope of the present invention is limited solely by the appended claims.

**Claims**

1. A suturing device for use with a suturing needle (1), the device comprising:

a body (112) having a proximal end (108) and a distal end (110);  
 a first clamp (226) near the distal end of the body;  
 a second clamp (226) near the distal end of the body;  
 a linkage (228) effecting movement of the first and second clamps between a grasping configuration and a displaced configuration, each clamp grasping the needle at an associated grasping location in the grasping configuration and laterally displaced from an axis of the needle in the displaced configuration, the grasping locations substantially fixed relative to the body; wherein the body extends along an axis from the proximal end to the distal end adjacent the first and second clamps, and further comprising an alternatable drive element (230) movable laterally from the axis of the body between a first configuration and a second configuration, the alternatable drive element drivingly coupled to the first clamp in the first configuration, the alternatable drive element drivingly coupled to the second clamp in the second configuration; the alternatable drive element movable axially along the axis of the body so as to actuate and displace the driven clamp from about the needle.

2. The suturing device of claim 1, further comprising a handle (230a) disposed at the proximal end of the body and coupled to the first and second clamps (226) by the linkage so that actuation of the handle alternates between:

the first clamp (226) in the grasping configuration and the second clamp (226) in the displaced configuration, and  
 the second clamp (226) in the grasping configuration and the first clamp (226) in the displaced configuration.

3. The suturing device of claim 2, wherein the handle

(230a) is configured for grasping by a hand of a surgeon and is actuatable between a closed hand configuration and an open hand configuration, movement of the handle (230a) from the closed-hand configuration to the open-hand configuration and back to the closed-hand configuration defining a handle actuation cycle, and wherein support for the needle alternates once between the first clamp (226) and the second clamp (226) during each handle actuation cycle, and wherein the surgeon can insert the needle into tissue by closing his hand on the handle and manipulating the handle (230a) while the needle is grasped by one of the clamps.

4. The suturing device of claim 3, wherein each clamp (226) opens after the other clamp has closed during the handle actuation cycle so that the clamps maintain the needle at a substantially fixed location relative to the body.

5. The suturing device of claim 2, wherein the linkage (228) comprises the alternatable drive element, the alternatable drive element moving between the first configuration and the second configuration with each handle actuation cycle, the alternatable drive element driving a first linkage (228) coupled to the first clamp in the first configuration and driving a second linkage (228) coupled to the second clamp in the second configuration.

6. The suturing device of claim 5, wherein the handle actuation cycle rotates a drive wheel (11), wherein the first and second linkages each comprise a driven wheel (10, 12), wherein the alternatable drive element in the first configuration drivingly couples the drive wheel with the driven wheel of the first linkage, and wherein the alternatable drive element in the second configuration drivingly couples the drive wheel with the driven wheel of the second linkage.

7. The suturing device of claim 1, wherein during actuation the linkage displaces the first clamp (226) laterally from around the needle after the second clamp (226) grasps the needle, and wherein during actuation the linkage displaces the second clamp laterally from around the needle after the first clamp grasps the needle.

8. The suturing device of claim 7, wherein each clamp (226) has a reciprocable shaft extending proximally from the clamp to the body, wherein the linkage (228) reciprocates the shafts relative to the body during the actuation cycle so as to move each clamp distally, and wherein the linkage thereafter closes the distally extended clamp around the needle.

9. The suturing device of claim 8, wherein the linkage (228) rotates each clamp (226) about an axis of the

- shaft between a retracted position and an extended grasping position.
10. The suturing device of claim 8, wherein at least one associated spring inhibits closing of each clamp before the clamp is adjacent the needle. 5
11. The suturing device of claim 1, further comprising a release input coupled to the linkage (228) so as to release the needle from the first and second clamps. 10
12. The suturing device of claim 1, further comprising the needle, wherein the needle comprises an off-the-shelf needle sold primarily for standard open or laparoscopic surgery. 15
13. The suturing device of claim 1, wherein the clamping locations of the first and second clamps (226) are axially offset along a length of the needle and angularly offset so as to accommodate axial curvature of the needle. 20
14. The suturing device of claim 1, further comprising a proximal handle coupled to the body so as to actuate along a handle actuation plane, wherein the first and second clamps are oriented to support the needle so that an axis of the needle traverses the handle actuation plane. 25
15. The suturing device of claim 1, wherein the suturing device is composed of chemically sterilizable materials. 30
16. The suturing device of claim 1, further comprising an alternatable latch (232) movable laterally between a first configuration and a second configuration in response to movement of the drive element, wherein the alternatable latch (232) in the first configuration inhibits movement of the first clamp (226), and wherein the alternatable latch (232) in the second configuration inhibits movement of the second clamp (226). 35
17. The suturing device of claim 1, wherein the body extends from a proximal handle of the body distally toward the first and second clamps, and further comprising a handle articulatably coupled to the body so that a hand can grasp and move the body while fingers of the hand articulate the handle, and wherein the articulation of the handle effects grasping and releasing of the needle by the clamps. 40
18. The suturing device of claim 1, wherein an extension (282) of the body (112) is disposed between the clamps (284) and a proximal housing (296) of the body, the extension extending along an axis, wherein the body is plastically bendable to have an axial bend (288) desired for a particular patient while the clamps 45
- are supported thereby, and wherein a drive member is articulatable from within the housing and through the bent extension so that the clamps can grasp and release the needle while the body has the bend.
19. The suturing device of claim 1, wherein an actuation axis extends between each clamp and the body, each clamp (226) comprising a pair of opposed driven surfaces which angle laterally outwardly along the axis, wherein the driven surfaces of each clamp are moved axially by pushing engagement of corresponding driving surfaces of a drive mechanism so that the clamp moves along the axis, and are driven laterally by sliding engagement between the driving surfaces and the driven surfaces so that the clamp opens and closes.
20. The suturing device of claim 1, wherein the first and second clamps (226) are alternately latched by an alternatable latch (232), and further comprising moving the alternatable latch laterally between a first configuration and a second configuration in response to movement of the drive element, wherein the alternatable latch in the first configuration inhibits movement of the first clamp, and wherein the alternatable latch in the second configuration inhibits movement of the second clamp.
21. The suturing device of claim 1, wherein the suturing device is configured for manually grasping and manipulation of the body with a hand of a surgeon, wherein the body comprises a rigid grasping base (232), and wherein the clamps (226) are operatively coupled to an articulatable handle (230a) so that grasping and releasing of the needle can be effected by articulating the handle with fingers of the hand while the hand grasps the grasping base (232) of the body.
22. The suturing device of claim 1, further comprising a detachable coupler (208) releasably coupling the first and second clamps to the body, the first and second clamps being disposable, and third and fourth disposable clamps for releasably coupling to the body in place of the first and second clamps so that each clamp can be used to suture tissue of only a single patient.
23. The suturing device of claim 1, wherein cycling of the linkage effects grasping of the needle with each clamp by:
- extending the clamp (226) slightly beyond the grasping location of the grasping configuration; closing the extended clamp (226) on the needle; and withdrawing the needle with the clamp to the grasping location;

so that gradual displacement of the needle relative to the body during repeated cycling of the linkage is inhibited.

24. The suturing device of claim 1, wherein the clamps (226) accommodate a range of oblique angles between the needle and a shaft of the clamp for proximal or distal suturing, and wherein cycling of the linkage substantially maintains the oblique angle.

### Patentansprüche

1. Nahtvorrichtung zur Verwendung mit einer Nähnaedel (1), wobei die Vorrichtung Folgendes umfasst:

einen Körper (112) mit einem proximalen Ende (108) und einem distalen Ende (110);  
eine erste Klemme (226) nahe dem distalen Ende des Körpers;  
eine zweite Klemme (226) nahe dem distalen Ende des Körpers;  
eine Getriebekette (228), die eine Bewegung der ersten und zweiten Klemmen zwischen einer Greifkonfiguration und einer verschobenen Konfiguration bewirkt, wobei jede Klemme die Nadel an einer damit assoziierten Greifstelle in der Greifkonfiguration fasst und seitlich von einer Achse der Nadel in die verschobene Konfiguration verschiebt, wobei die Greifstellen im Wesentlichen relativ zum Körper fixiert sind;  
wobei sich der Körper entlang einer Achse vom proximalen Ende bis zum distalen Ende, benachbart von den ersten und zweiten Klemmen erstreckt und weiter Folgendes umfasst: ein alternierbares Antriebselement (230), das seitlich beweglich von der Achse des Körpers zwischen einer ersten Konfiguration und einer zweiten Konfiguration ist, das alternierbare Antriebselement, das zum Antrieb an die erste Klemme in der ersten Konfiguration gekoppelt ist, das alternierbare Antriebselement zum Antrieb an die zweite Klemme in der zweiten Konfiguration gekoppelt ist; das alternierbare Antriebselement entlang der Achse des Körpers dergestalt axial beweglich ist, dass die angetriebene Klemme um die Nadel herum betätigt und verschoben wird.

2. Nahtvorrichtung nach Anspruch 1, weiter umfassend einen Griff (230a), der am proximalen Ende des Körpers angebracht ist und durch die Getriebekette an die ersten und zweiten Klemmen (226) dergestalt gekoppelt ist, dass die Betätigung des Griffs wie folgt alterniert zwischen:

der ersten Klemme (226) in der Greifkonfiguration und der zweiten Klemme (226) in der ver-

schobenen Konfiguration, und der zweiten Klemme (226) in der Greifkonfiguration und der ersten Klemme (226) in der verschobenen Konfiguration.

3. Nahtvorrichtung nach Anspruch 2, wobei der Griff (230a) zum Fassen mit einer Hand eines Chirurgen konfiguriert ist und zwischen einer geschlossenen Handkonfiguration und einer offenen Handkonfiguration, Bewegung des Griffs (230a) von der geschlossenen Handkonfiguration in die offene Handkonfiguration und zurück in die geschlossene Handkonfiguration betätigt werden kann, definierend einen Griffbetätigungszyklus, und wobei die Stütze für die Nadel während jedem Griffbetätigungszyklus einmal zwischen der ersten Klemme (226) und der zweiten Klemme (226) alterniert, und wobei der Chirurg durch Schließen seiner Hand auf dem Griff und Manipulieren des Griffs (230a) mit der Nadel das Gewebe durchdringen kann, während die Nadel von einer der Klemmen gefasst wird.
4. Nahtvorrichtung nach Anspruch 3, wobei sich jede Klemme (226) öffnet, nachdem sich die andere Klemme während des Griffbetätigungszyklus dergestalt geschlossen hat, dass die Klemmen die Nadel an einer im Wesentlichen fixierten Stelle relativ zum Körper halten.
5. Nahtvorrichtung nach Anspruch 2, wobei die Getriebekette (228) das alternierbare Antriebselement umfasst, wobei sich das alternierbare Antriebselement mit jedem Griffbetätigungszyklus zwischen der ersten Konfiguration und der zweiten Konfiguration bewegt, das alternierbare Antriebselement, das eine erste Getriebekette (228) antreibt, an die erste Klemme in der ersten Konfiguration gekoppelt ist und eine zweite Getriebekette (228) antreibt, die an die zweite Klemme in der zweiten Konfiguration gekoppelt ist.
6. Nahtvorrichtung nach Anspruch 5, wobei der Griffbetätigungszyklus ein Antriebsrad (11) dreht, wobei die ersten und zweiten Getriebeketten jeweils ein angetriebenes Rad (10, 12) umfassen, wobei das alternierbare Antriebselement in der ersten Konfiguration das Antriebsrad mit dem angetriebenen Rad der ersten Getriebekette zum Antrieb koppelt, und wobei das alternierbare Antriebselement in der zweiten Konfiguration das Antriebsrad mit dem angetriebenen Rad der zweiten Getriebekette zum Antrieb koppelt.
7. Nahtvorrichtung nach Anspruch 1, wobei während der Betätigung die Getriebekette die erste Klemme (226) seitlich um die Nadel herum verschiebt, nachdem die zweite Klemme (226) die Nadel fasst, und wobei während der Betätigung der Getriebekette die zweite Klemme seitlich um die Nadel herum verscho-

- ben wird, nachdem die erste Klemme die Nadel fasst.
8. Nahtvorrichtung nach Anspruch 7, wobei jede Klemme (226) einen hin und her beweglichen Schaft aufweist, der sich proximal von der Klemme zum Körper erstreckt, wobei die Getriebekette (228) während des Betätigungszyklus die Schäfte relativ zum Körper dergestalt hin und her bewegt, um jede Klemme distal zu bewegen, und wobei die Getriebekette danach die distal ausgezogene Klemme um die Nadel herum schließt.
9. Nahtvorrichtung nach Anspruch 8, wobei die Getriebekette (228) jede Klemme (226) um eine Achse des Schafts zwischen einer zurückgezogenen Position und einer ausgezogenen Greifposition dreht.
10. Nahtvorrichtung nach Anspruch 8, wobei mindestens eine damit assoziierte Feder das Schließen jeder Klemme inhibiert, bevor sich die Klemme benachbart zur Nadel befindet.
11. Nahtvorrichtung nach Anspruch 1, weiter umfassend einen an die Getriebekette (228) gekoppelten Freigabeeingang dergestalt, dass die Nadel von den ersten und zweiten Klemmen freigegeben wird.
12. Nahtvorrichtung nach Anspruch 1, weiter umfassend die Nadel, wobei die Nadel eine in erster Linie für übliche offene und laparoskopische chirurgische Eingriffe verkaufte Standardnadel umfasst.
13. Nahtvorrichtung nach Anspruch 1, wobei die Klemmstellen der ersten und zweiten Klemmen (226) entlang einer Länge der Nadel axial versetzt und winklig versetzt sind, dergestalt, um sie der axialen Biegung der Nadel anzupassen.
14. Nahtvorrichtung nach Anspruch 1, weiter umfassend einen proximalen Griff, der an den Körper dergestalt gekoppelt ist, um ihn entlang einer Griffbetätigungsebene zu betätigen, wobei die ersten und zweiten Klemmen zur Stütze der Nadel dergestalt ausgerichtet sind, dass eine Achse der Nadel die Griffbetätigungsebene transversal durchläuft.
15. Nahtvorrichtung nach Anspruch 1, wobei die Nahtvorrichtung aus chemisch sterilisierbaren Materialien zusammengesetzt ist.
16. Nahtvorrichtung nach Anspruch 1, weiter umfassend eine alternierbare Sperre (232), die zwischen einer ersten Konfiguration und einer zweiten Konfiguration als Reaktion auf die Bewegung des Antriebselements seitlich beweglich ist, wobei die alternierbare Sperre (232) in der ersten Konfiguration die Bewegung der ersten Klemme (226) inhibiert, und wobei
- die alternierbare Sperre (232) in der zweiten Konfiguration die Bewegung der zweiten Klemme (226) inhibiert.
17. Nahtvorrichtung nach Anspruch 1, wobei sich der Körper von einem proximalen Griff des Körpers distal in Richtung der ersten und zweiten Klemmen erstreckt, und weiter einen Griff umfasst, der gelenkig an den Körper dergestalt gekoppelt ist, dass eine Hand den Körper fassen und bewegen kann, während die Finger der Hand den Griff gelenkig bewegen, und wobei die Gelenkverbindung des Griffs das Fassen und Freigeben der Nadel durch die Klemmen bewirkt.
18. Nahtvorrichtung nach Anspruch 1, wobei eine Verlängerung (282) des Körpers (112) zwischen den Klemmen (284) und einem proximalen Gehäuse (296) des Körpers angeordnet ist, wobei sich die Verlängerung entlang einer Achse erstreckt, wobei der Körper plastisch biegsam ist, um eine axiale Biegung (288) aufzuweisen, die für einen bestimmten Patienten erwünscht ist, während die Klemmen dadurch unterstützt werden, und wobei ein Antriebsglied vom Gehäuseinneren und durch die gebogene Verlängerung dergestalt gelenkig verbunden ist, dass die Klemmen die Nadel fassen und freigegeben können, während der Körper die Biegung aufweist.
19. Nahtvorrichtung nach Anspruch 1, wobei sich eine Betätigungsachse zwischen jeder Klemme und dem Körper erstreckt, wobei jede Klemme (226) ein Paar gegenläufig angetriebene Oberflächen umfasst, welche entlang der Achse seitlich nach außen gewinkelt sind, wobei die angetriebenen Oberflächen von jeder Klemme durch Eingreifen mittels Schieben der entsprechenden Antriebsoberflächen eines Antriebsmechanismus dergestalt axial bewegt werden, dass sich die Klemme entlang der Achse bewegt, und durch gleitenden Eingriff zwischen den Antriebsoberflächen und den angetriebenen Oberflächen dergestalt seitlich angetrieben werden, dass sich die Klemme öffnet und schließt.
20. Nahtvorrichtung nach Anspruch 1, wobei die ersten und zweiten Klemmen (226) durch eine alternierbare Sperre (232) alternierend gesperrt werden, und weiter umfassend die alternierbare Sperre seitlich zwischen einer ersten Konfiguration und einer zweiten Konfiguration als Reaktion auf Bewegung des Antriebselements bewegen, wobei die alternierbare Sperre in der ersten Konfiguration die Bewegung der ersten Klemme inhibiert, und wobei die alternierbare Sperre in der zweiten Konfiguration die Bewegung der zweiten Klemme inhibiert.
21. Nahtvorrichtung nach Anspruch 1, wobei die Nahtvorrichtung zum manuellen Greifen und zur Manipu-

lation des Körpers mit einer Hand eines Chirurgen konfiguriert ist, wobei der Körper eine steife Greifbasis (232) umfasst, und wobei die Klemmen (226) an einen gelenkig beweglichen Griff (230a) dergestalt operativ gekoppelt sind, dass das Fassen und Freigeben der Nadel durch gelenkiges Bewegen des Griffs mit den Fingern der Hand bewirkt werden kann, während die Hand die Greifbasis (232) des Körpers fasst.

22. Nahtvorrichtung nach Anspruch 1, weiter umfassend einen abnehmbaren Koppler (208) zum lösbaren Koppeln der ersten und zweiten Klemmen an den Körper, wobei die ersten und zweiten Klemmen zum Einweggebrauch vorgesehen sind, und dritte und vierte Einwegklemmen zur lösbaren Kopplung an den Körper anstelle der ersten und zweiten Klemmen dergestalt vorgesehen sind, dass jede Klemme zum Anlegen einer Naht im Gewebe von nur einem einzigen Patienten verwendet werden kann.

23. Nahtvorrichtung nach Anspruch 1, wobei das Zyklieren der Getriebekette das Fassen der Nadel mit jeder Klemme bewirkt durch:

Ausziehen der Klemme (226) ein wenig über die Greifstelle der Greifkonfiguration hinausgehend;  
Schließen der ausgezogenen Klemme (226) auf der Nadel; und  
Zurückziehen der Nadel mit der Klemme in die Greifstelle;  
dergestalt, dass eine allmähliche Verschiebung der Nadel relativ zum Körper während wiederholtem Zyklieren der Getriebekette inhibiert wird.

24. Nahtvorrichtung nach Anspruch 1, wobei die Klemmen (226) an eine Reihe von schiefen Winkeln zwischen der Nadel und einem Schaft der Klemme zum proximalen oder distalen Anlegen einer Naht angepasst sind, und wobei das Zyklieren der Getriebekette im Wesentlichen den schiefen Winkel beibehält.

## Revendications

1. Dispositif de suture destiné à une utilisation avec une aiguille de suture (1), le dispositif comprenant :

un corps (112) ayant une extrémité proximale (108) et une extrémité distale (110) ;  
une première pince (226) près de l'extrémité distale du corps ;  
une deuxième pince (226) près de l'extrémité distale du corps ;  
une liaison (228) réalisant un déplacement des

première et deuxième pinces entre une configuration de préhension et une configuration déplacée, chaque pince saisissant l'aiguille à un emplacement de préhension associé dans la configuration de préhension et déplacé latéralement par rapport à un axe de l'aiguille dans la configuration déplacée, les emplacements de préhension étant sensiblement fixes par rapport au corps ;

dans lequel le corps s'étend le long d'un axe de l'extrémité proximale à l'extrémité distale adjacente aux première et deuxième pinces, et comprenant en outre un élément d'entraînement à mouvement alternatif (230) capable de se déplacer latéralement à partir de l'axe du corps entre une première configuration et une deuxième configuration, l'élément d'entraînement à mouvement alternatif étant couplé de façon à transmettre un entraînement à la première pince dans la première configuration, l'élément d'entraînement à mouvement alternatif étant couplé de façon à transmettre un entraînement à la deuxième pince dans la deuxième configuration ; l'élément d'entraînement à mouvement alternatif étant capable de se déplacer axialement le long de l'axe du corps de façon à actionner et déplacer la pince entraînée à partir du pourtour de l'aiguille.

2. Dispositif de suture selon la revendication 1, comprenant en outre une poignée (230a) disposée à l'extrémité proximale du corps et couplée aux première et deuxième pinces (226) par la liaison de façon à ce que l'actionnement de la poignée alterne entre :

la première pince (226) dans la configuration de préhension et la deuxième pince (226) dans la configuration déplacée, et  
la deuxième pince (226) dans la configuration de préhension et la première pince (226) dans la configuration déplacée.

3. Dispositif de suture selon la revendication 2, dans lequel la poignée (230a) est configurée pour être saisie par une main d'un chirurgien et peut être actionnée entre une configuration à main fermée et une configuration à main ouverte, le déplacement de la poignée (230a) de la configuration à main fermée à la configuration à main ouverte et le retour à la configuration à main fermée définissant un cycle d'actionnement de la poignée, et dans lequel le support de l'aiguille alterne une fois entre la première pince (226) et la deuxième pince (226) durant chaque cycle d'actionnement de la poignée, et dans lequel le chirurgien peut insérer l'aiguille dans le tissu en fermant sa main sur la poignée et en manipulant la poignée (230a) tandis que l'aiguille est saisie par une des pinces.

4. Dispositif de suture selon la revendication 3, dans lequel chaque pince (226) s'ouvre après que l'autre pince s'est fermée durant le cycle d'actionnement de la poignée, de telle sorte que les pinces maintiennent l'aiguille à un emplacement sensiblement fixe par rapport au corps.
5. Dispositif de suture selon la revendication 2, dans lequel la liaison (228) comprend l'élément d'entraînement à mouvement alternatif, l'élément d'entraînement à mouvement alternatif se déplaçant entre la première configuration et la deuxième configuration à chaque cycle d'actionnement de la poignée, l'élément d'entraînement à mouvement alternatif entraînant une première liaison (228) couplée à la première pince dans la première configuration et entraînant une deuxième liaison (228) couplée à la deuxième pince dans la deuxième configuration.
6. Dispositif de suture selon la revendication 5, dans lequel le cycle d'actionnement de la poignée fait tourner un disque d'entraînement (11), dans lequel les première et deuxième liaisons comprennent chacune un disque entraîné (10, 12), dans lequel l'élément d'entraînement à mouvement alternatif dans la première configuration couple de façon à transmettre un entraînement le disque d'entraînement avec le disque entraîné de la première liaison, et dans lequel l'élément d'entraînement à mouvement alternatif dans la deuxième configuration couple de façon à transmettre un entraînement le disque d'entraînement avec le disque entraîné de la deuxième liaison.
7. Dispositif de suture selon la revendication 1, dans lequel, durant l'actionnement, la liaison déplace la première pince (226) latéralement à partir du pourtour de l'aiguille après que la deuxième pince (226) a saisi l'aiguille et dans lequel, durant l'actionnement, la liaison déplace la deuxième pince latéralement à partir du pourtour de l'aiguille après que la première pince a saisi l'aiguille.
8. Dispositif de suture selon la revendication 7, dans lequel chaque pince (226) comporte une tige capable de se déplacer en va-et-vient qui s'étend proximale de la pince au corps, dans lequel la liaison (228) provoque un déplacement en va-et-vient des tiges par rapport au corps durant le cycle d'actionnement de façon à déplacer chaque pince distalement, et dans lequel la liaison ferme ensuite la pince allongée distalement autour de l'aiguille.
9. Dispositif de suture selon la revendication 8, dans lequel la liaison (228) fait pivoter chaque pince (226) autour d'un axe de la tige entre une position rétractée et une position de préhension allongée.
10. Dispositif de suture selon la revendication 8, dans lequel au moins un ressort associé empêche la fermeture de chaque pince avant que la pince ne soit adjacente à l'aiguille.
11. Dispositif de suture selon la revendication 1, comprenant en outre une commande de libération couplée à la liaison (228), de façon à libérer l'aiguille des première et deuxième pinces.
12. Dispositif de suture selon la revendication 1, comprenant en outre l'aiguille, dans lequel l'aiguille comprend une aiguille standard vendue principalement pour une chirurgie standard ouverte ou laparoscopique.
13. Dispositif de suture selon la revendication 1, dans lequel les emplacements de serrage des première et deuxième pinces (226) sont décalés axialement sur une longueur de l'aiguille et décalés angulairement de façon à tenir compte de la courbure axiale de l'aiguille.
14. Dispositif de suture selon la revendication 1, comprenant en outre une poignée proximale couplée au corps pour un actionnement le long d'un plan d'actionnement de la poignée, dans lequel les première et deuxième pinces sont orientées pour supporter l'aiguille de telle sorte qu'un axe de l'aiguille traverse le plan d'actionnement de la poignée.
15. Dispositif de suture selon la revendication 1, le dispositif de suture se composant de matériaux stérilisables chimiquement.
16. Dispositif de suture selon la revendication 1, comprenant en outre un blocage alternatif (232) capable de se déplacer latéralement entre une première configuration et une deuxième configuration en réponse à un déplacement de l'élément d'entraînement, dans lequel le blocage alternatif (232) dans la première configuration empêche le déplacement de la première pince (226), et dans lequel le blocage alternatif (232) dans la deuxième configuration empêche le déplacement de la deuxième pince (226).
17. Dispositif de suture selon la revendication 1, dans lequel le corps s'étend à partir d'une poignée proximale du corps distalement vers les première et deuxième pinces, et comprenant en outre une poignée couplée au corps de façon articulable de telle sorte qu'une main puisse saisir et déplacer le corps tandis que les doigts de la main articulent la poignée, et dans lequel l'articulation de la poignée provoque la préhension et la libération de l'aiguille par les pinces.
18. Dispositif de suture selon la revendication 1, dans lequel un prolongement (282) du corps (112) est dis-

- posé entre les pinces (284) et un logement proximal (296) du corps, le prolongement s'étendant le long d'un axe, dans lequel le corps peut être courbé plastiquement afin de présenter une courbure axiale (288) désirée pour un certain patient quand les pinces sont supportées ainsi, et dans lequel un élément d'entraînement peut être articulé à partir de l'intérieur du logement et par l'intermédiaire du prolongement courbé, de telle sorte que les pinces puissent saisir et relâcher l'aiguille quand le corps est courbé.
19. Dispositif de suture selon la revendication 1, dans lequel un axe d'actionnement s'étend entre chaque pince et le corps, chaque pince (226) comprenant une paire de surfaces entraînées opposées qui s'inclinent latéralement vers l'extérieur le long de l'axe, dans lequel les surfaces entraînées de chaque pince sont déplacées axialement sous l'effet d'une sollicitation par poussée par les surfaces d'entraînement correspondantes d'un mécanisme d'entraînement de telle sorte que la pince se déplace le long de l'axe, et sont entraînées latéralement par une coopération glissante entre les surfaces d'entraînement et les surfaces entraînées de telle sorte que la pince s'ouvre et se ferme.
20. Dispositif de suture selon la revendication 1, dans lequel les première et deuxième pinces (226) sont bloquées alternativement par un blocage alternatif (232), et comprenant en outre un déplacement du blocage alternatif latéralement entre une première configuration et une deuxième configuration en réponse à un déplacement de l'élément d'entraînement, dans lequel le blocage alternatif dans la première configuration empêche le déplacement de la première pince, et dans lequel le blocage alternatif dans la deuxième configuration empêche le déplacement de la deuxième pince.
21. Dispositif de suture selon la revendication 1, le dispositif de suture étant configuré pour une préhension manuelle et une manipulation du corps par une main d'un chirurgien, dans lequel le corps comprend une base de préhension rigide (232), et dans lequel les pinces (226) sont fonctionnellement couplées à une poignée articulable (230a) de telle sorte que la préhension et la libération de l'aiguille puissent être effectuées en articulant la poignée avec les doigts de la main tandis que la main saisit la base de préhension (232) du corps.
22. Dispositif de suture selon la revendication 1, comprenant en outre un coupleur amovible (208), couplant de façon amovible les première et deuxième pinces au corps, les première et deuxième pinces étant jetables, et des troisième et quatrième pinces jetables destinées à être couplées de façon amovible au corps à la place des première et deuxième pinces
- de telle sorte que chaque pince puisse être utilisée pour suturer les tissus d'un seul patient.
23. Dispositif de suture selon la revendication 1, dans lequel les cycles auxquels est soumise la liaison ont pour effet la préhension de l'aiguille par chaque pince, comme il est indiqué ci-dessous :
- allongement de la pince (226) légèrement au-delà de l'emplacement de préhension de la configuration de préhension ;  
fermeture de la pince allongée (226) sur l'aiguille ; et  
retrait de l'aiguille avec la pince jusqu'à l'emplacement de préhension ;  
de façon à empêcher un déplacement progressif de l'aiguille par rapport au corps lors de la répétition des cycles auxquels est soumise la liaison.
24. Dispositif de suture selon la revendication 1, dans lequel les pinces (226) sont compatibles avec une gamme d'angles obliques entre l'aiguille et une tige de la pince pour une suture proximale ou distale, et dans lequel les cycles auxquels est soumise la liaison maintiennent sensiblement l'angle oblique.

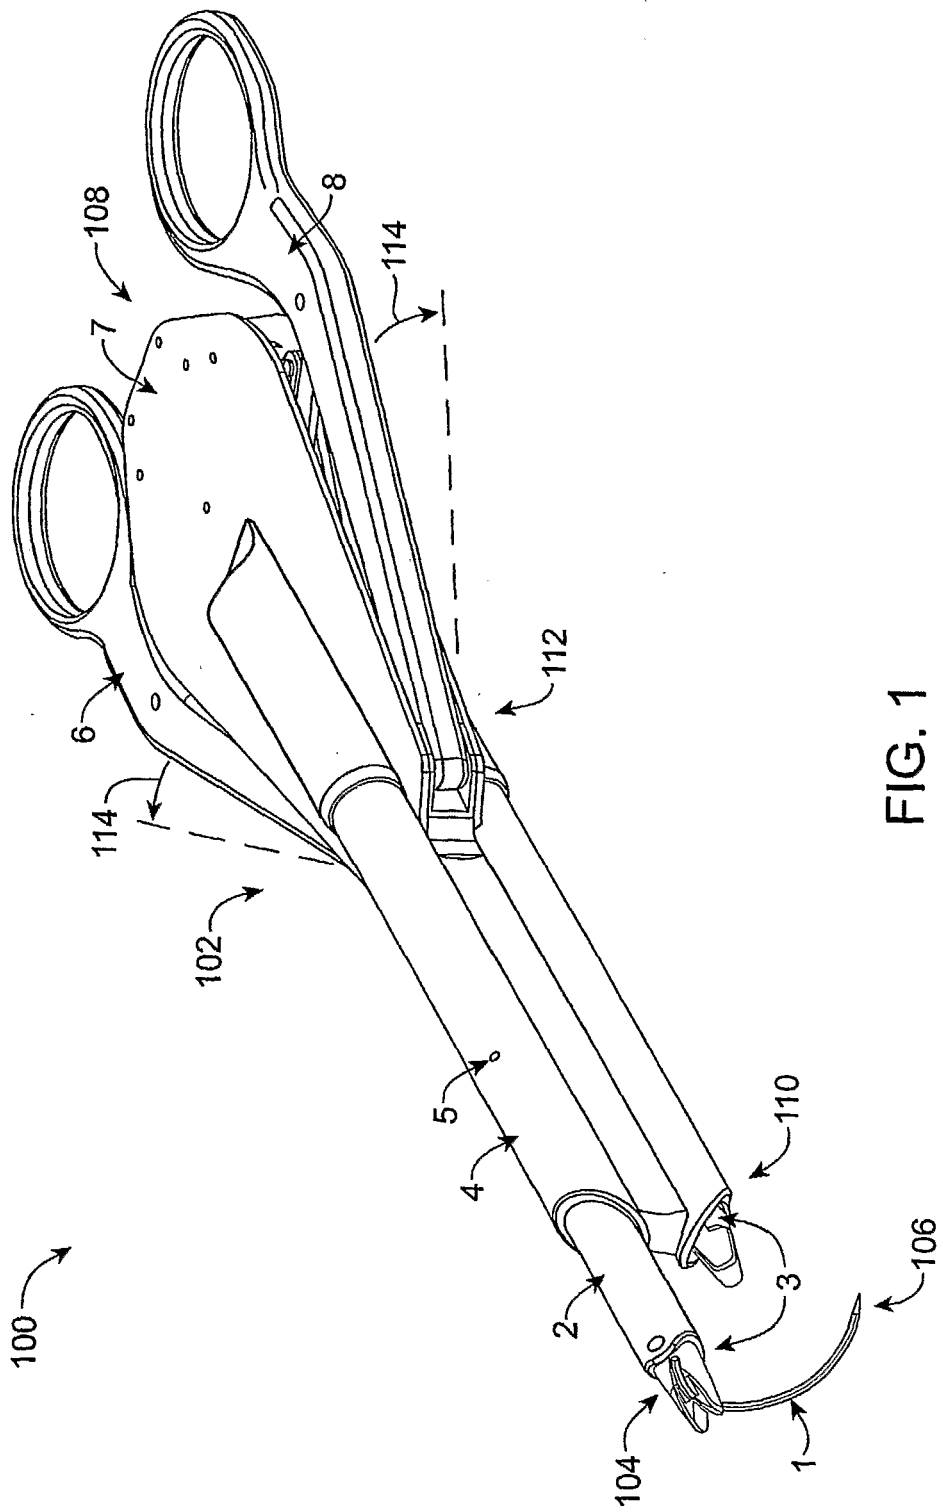


FIG. 1

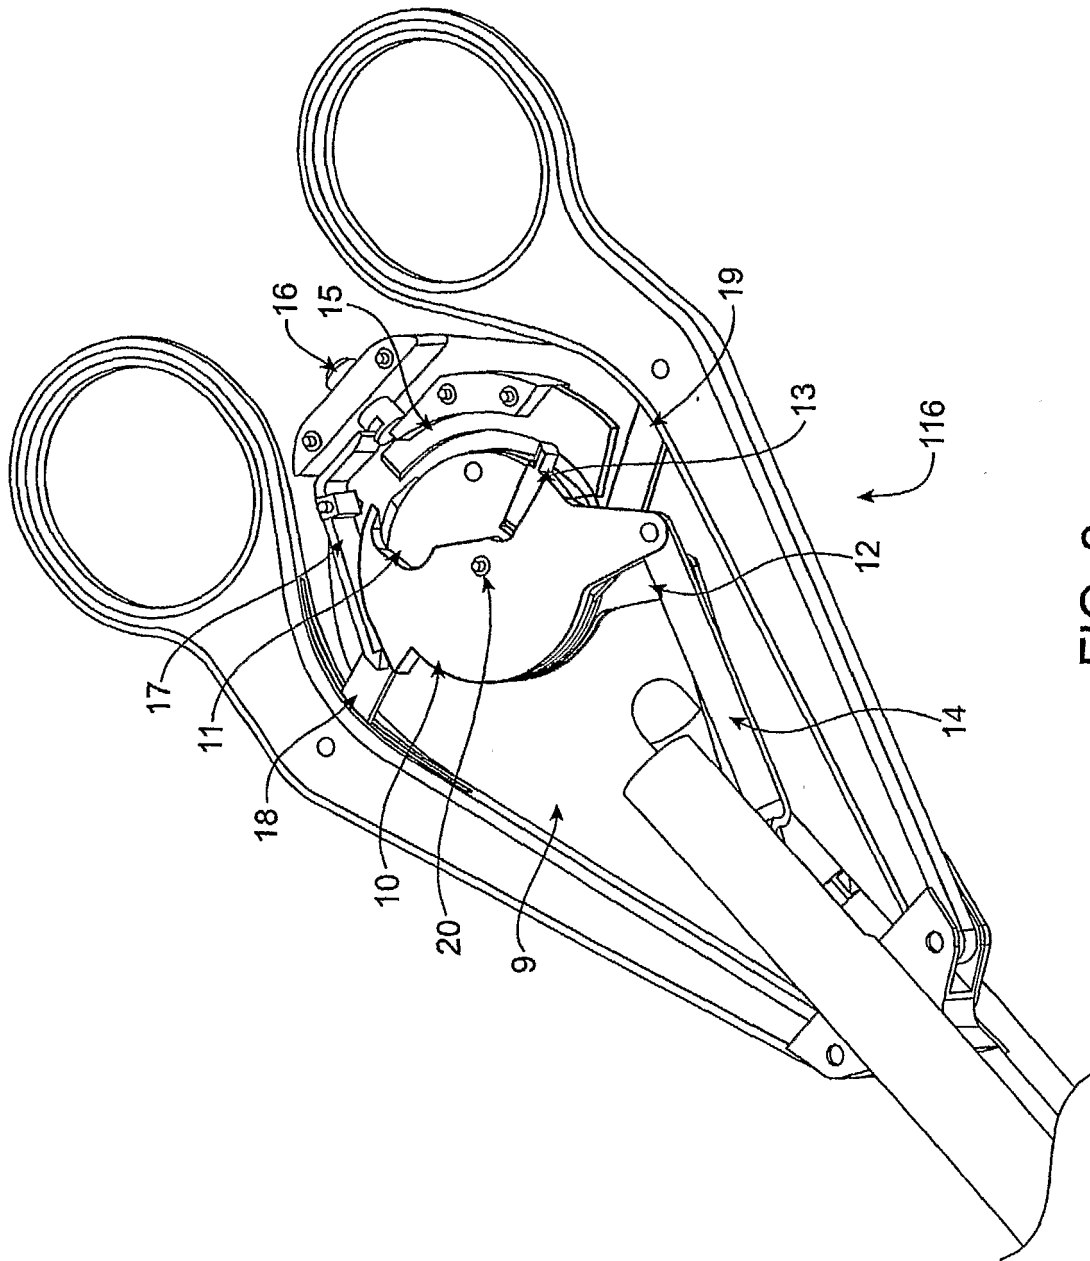


FIG. 2

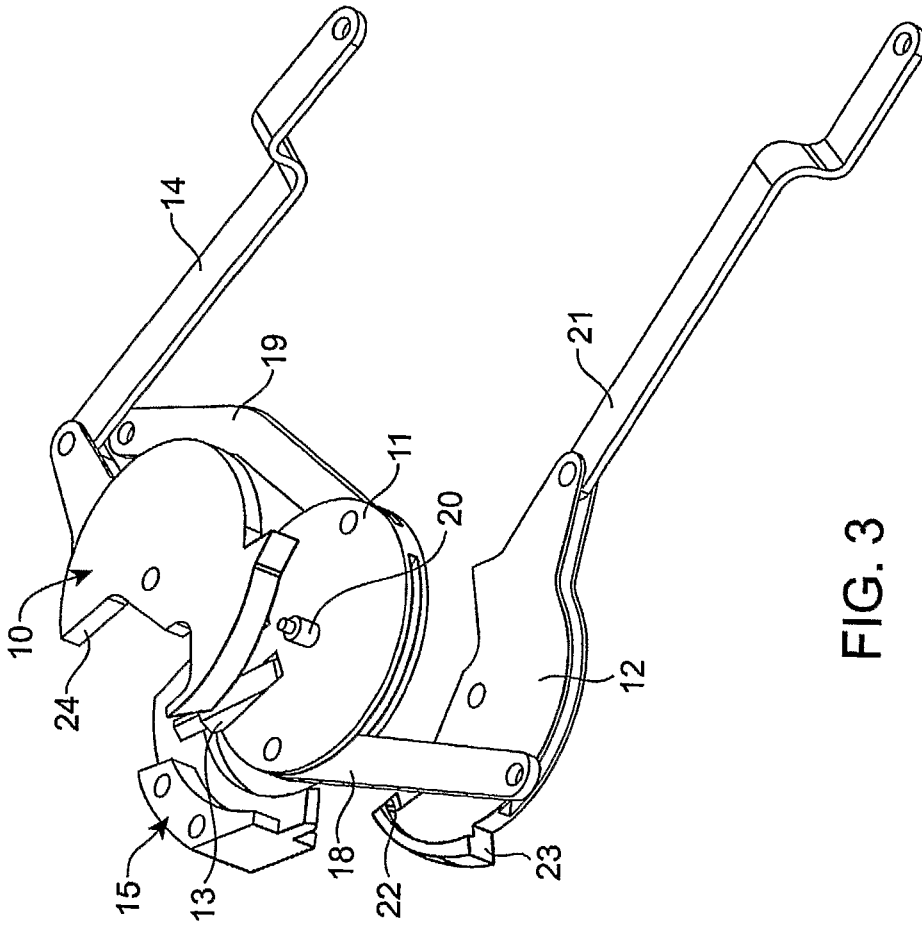


FIG. 3

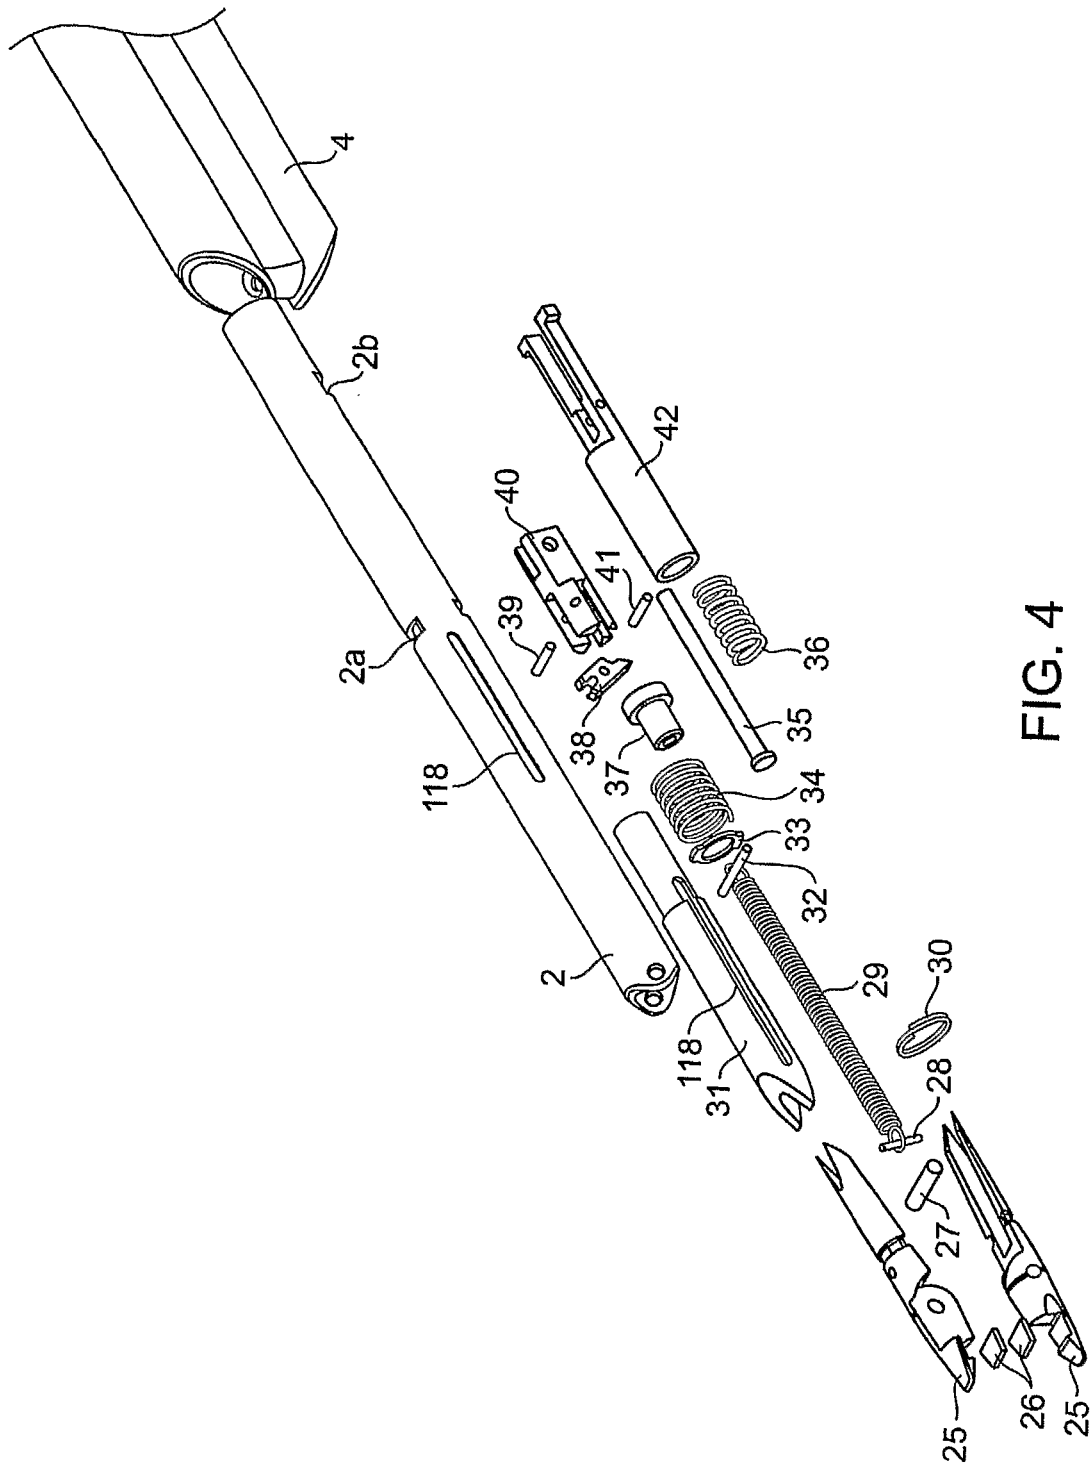


FIG. 4

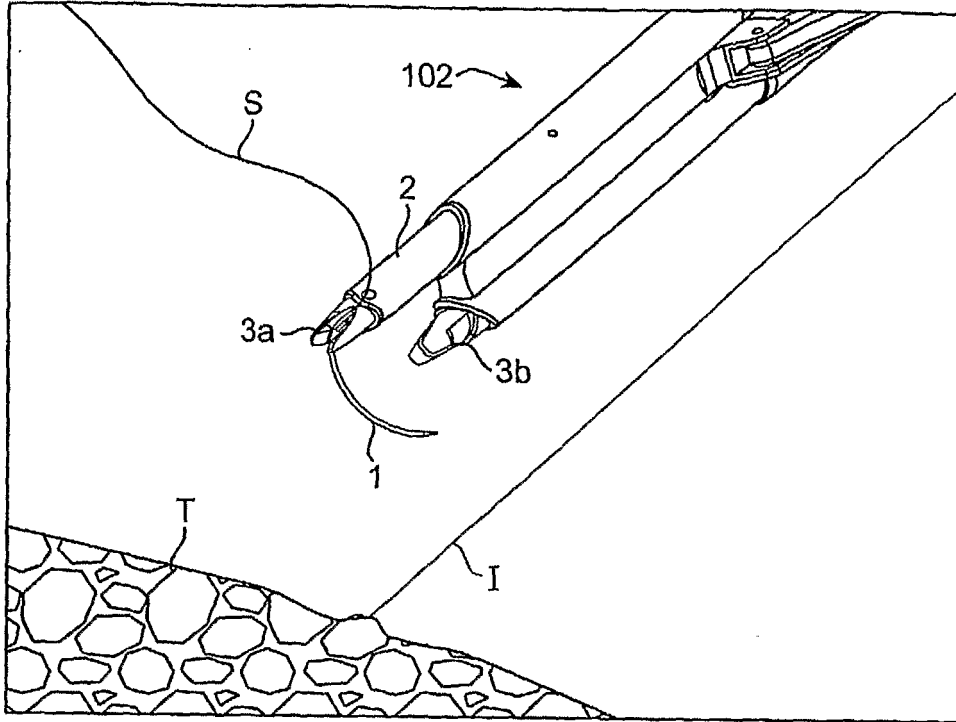


FIG. 5

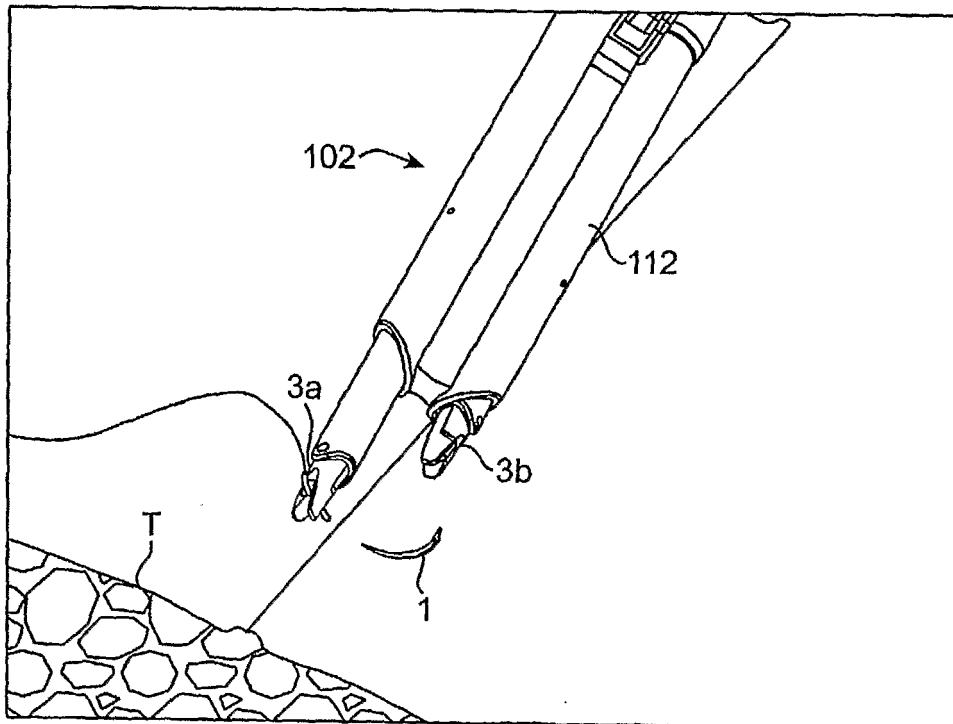


FIG. 6

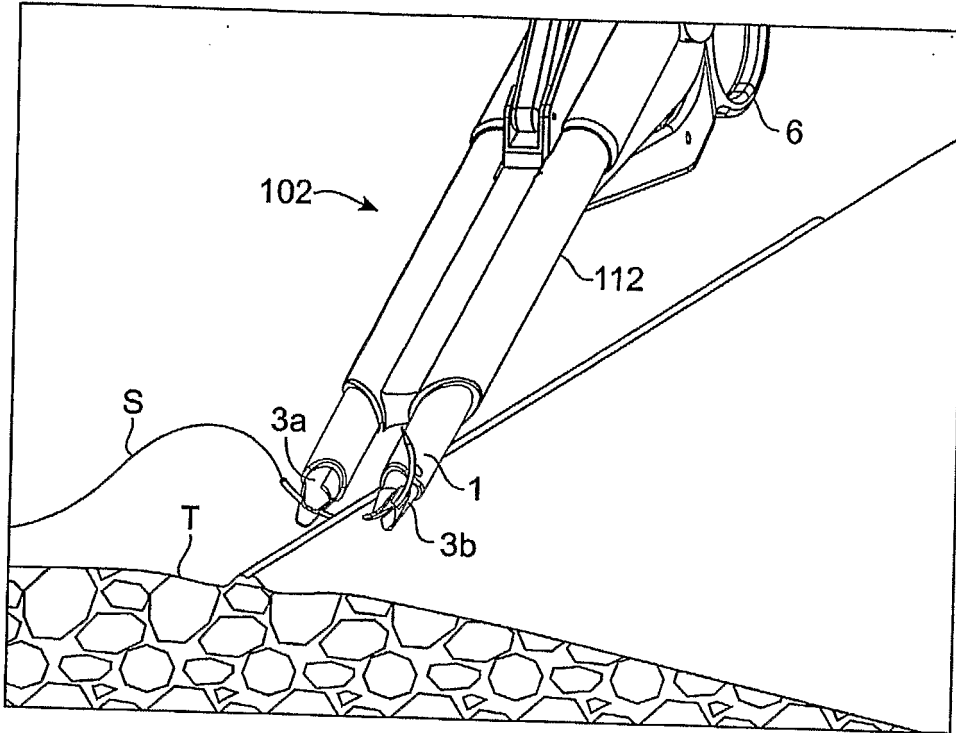


FIG. 7

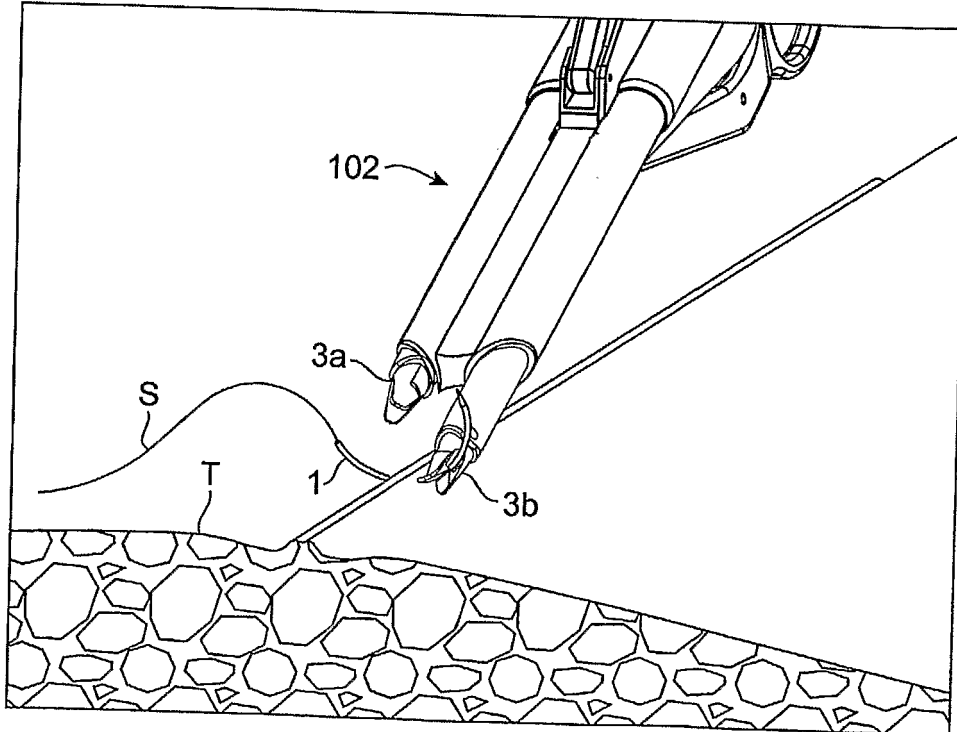


FIG. 8

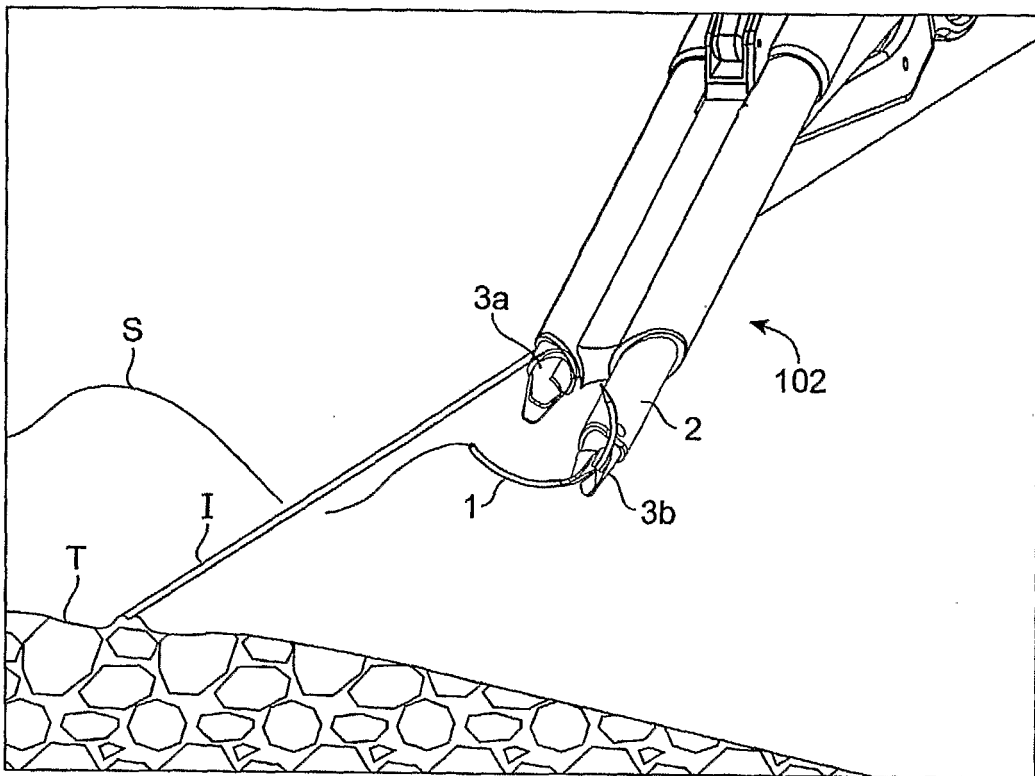
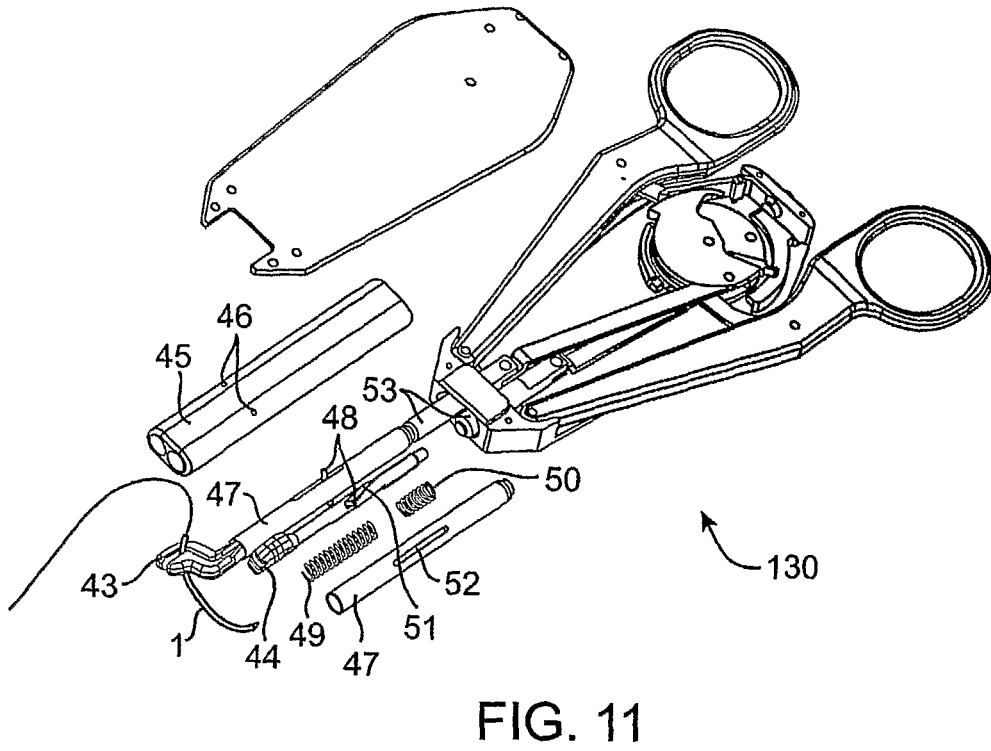
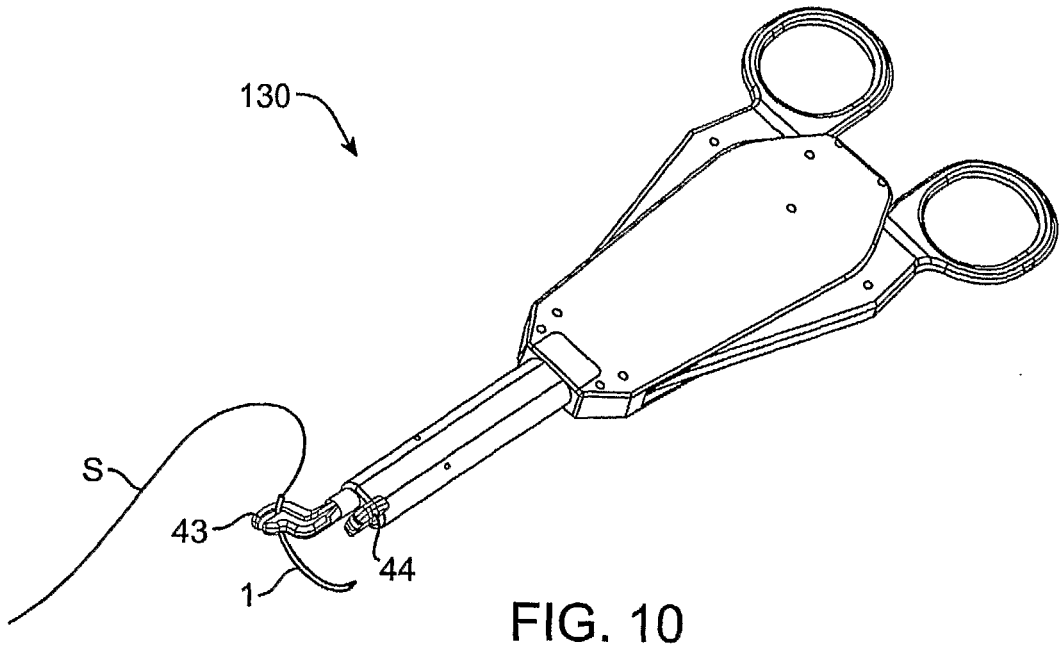


FIG. 9



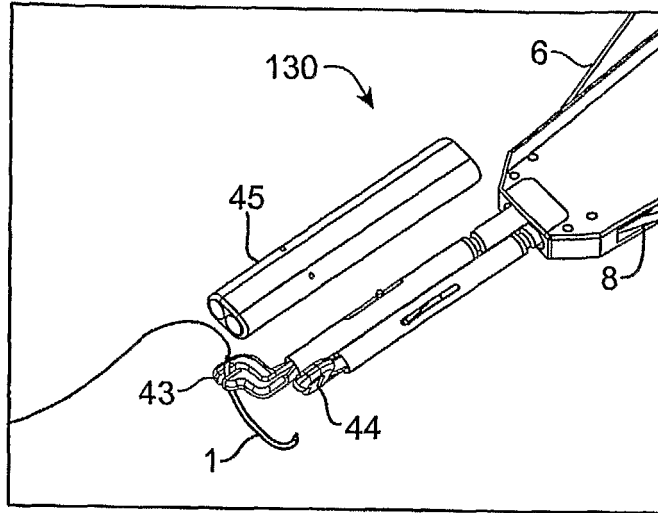


FIG. 12

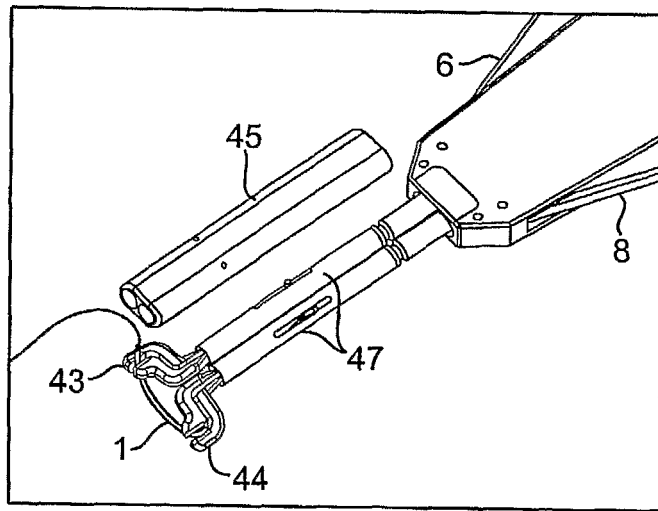


FIG. 13

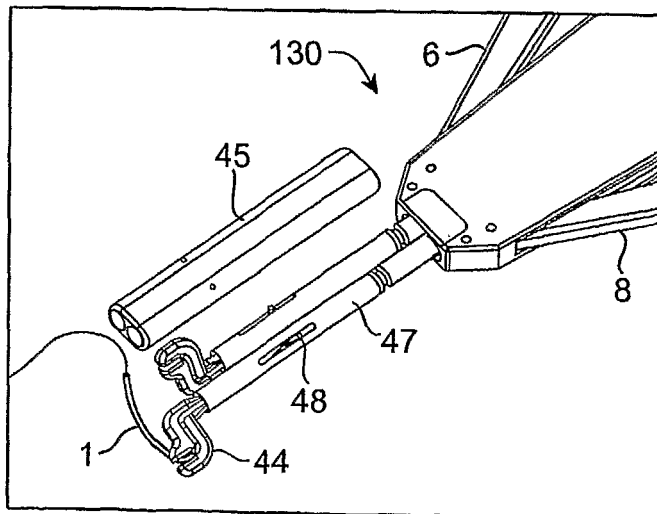


FIG. 14

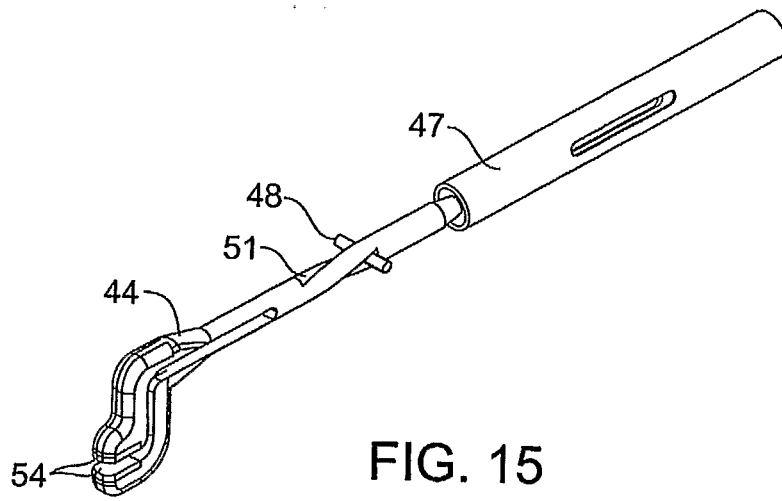


FIG. 15

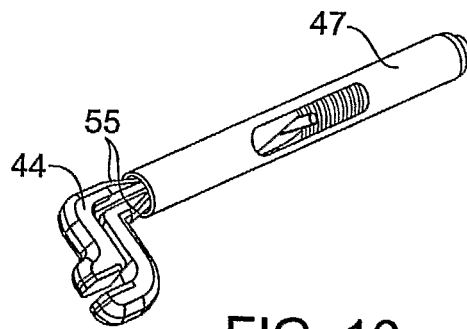


FIG. 16

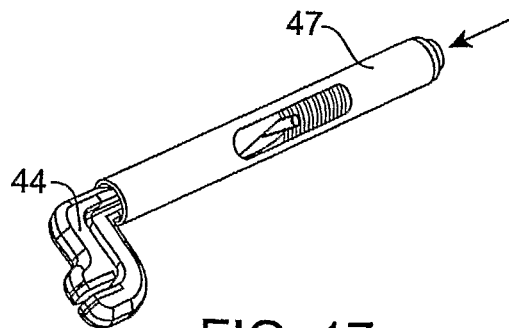
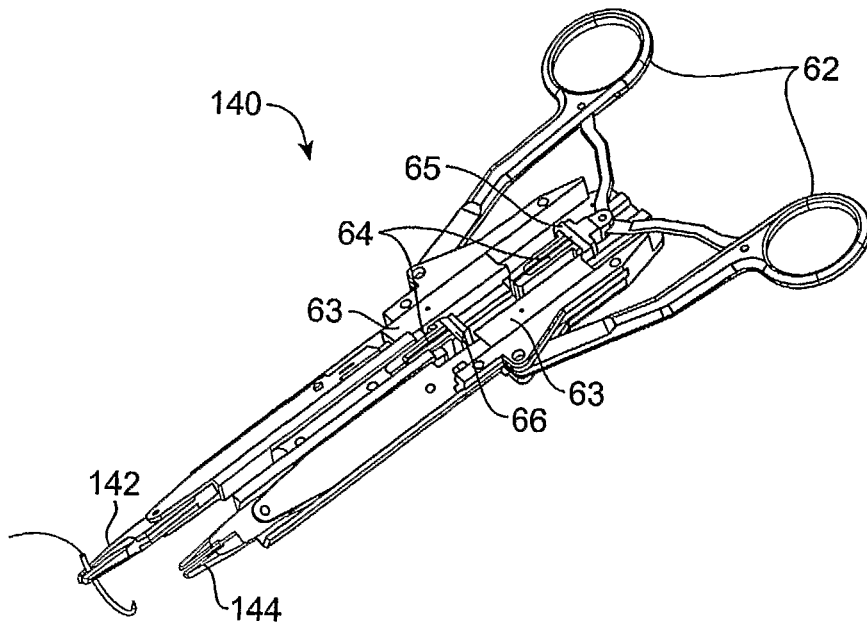
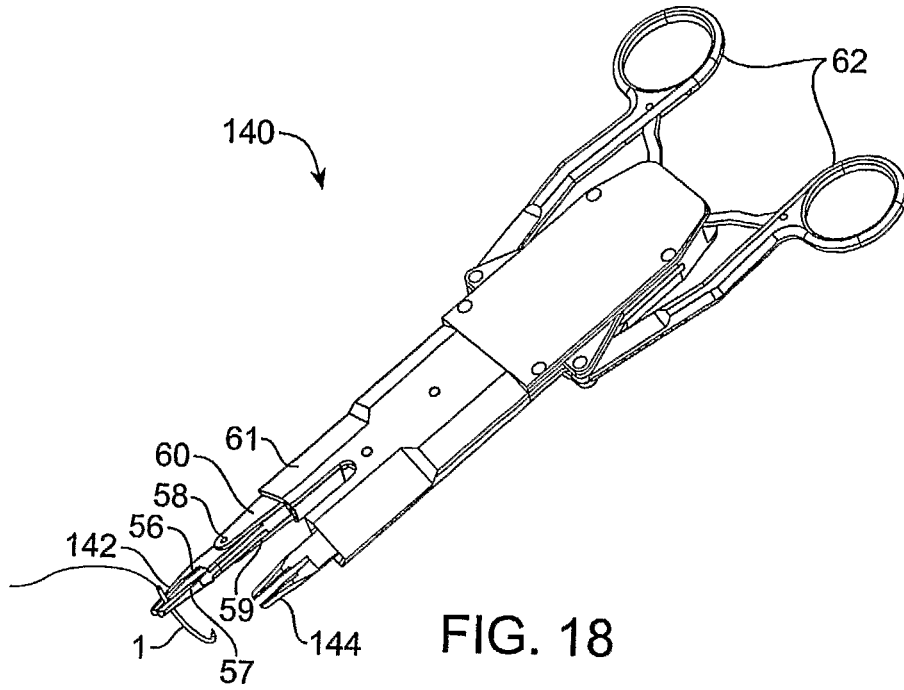
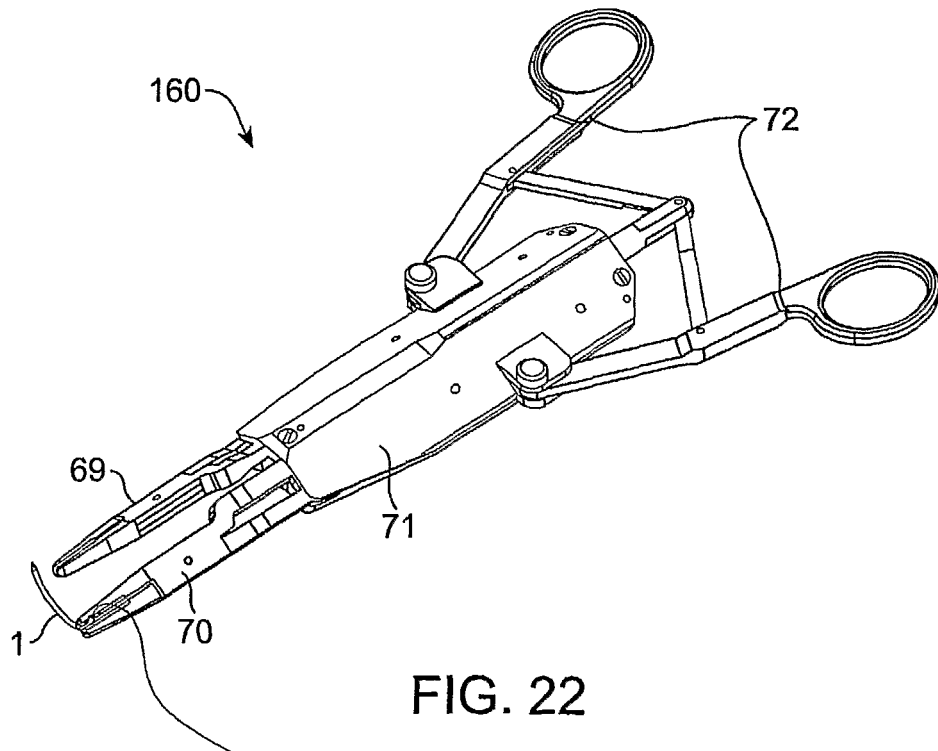
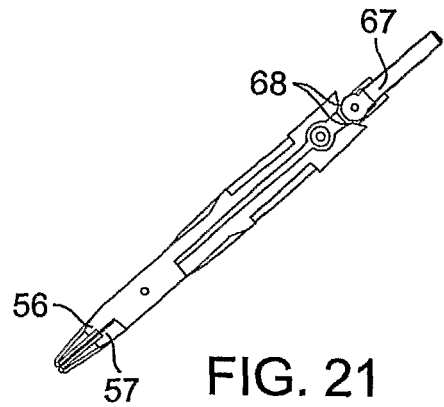
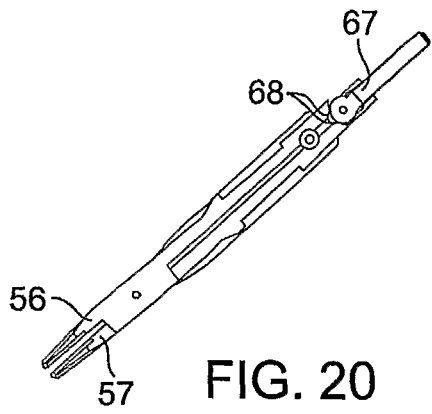


FIG. 17





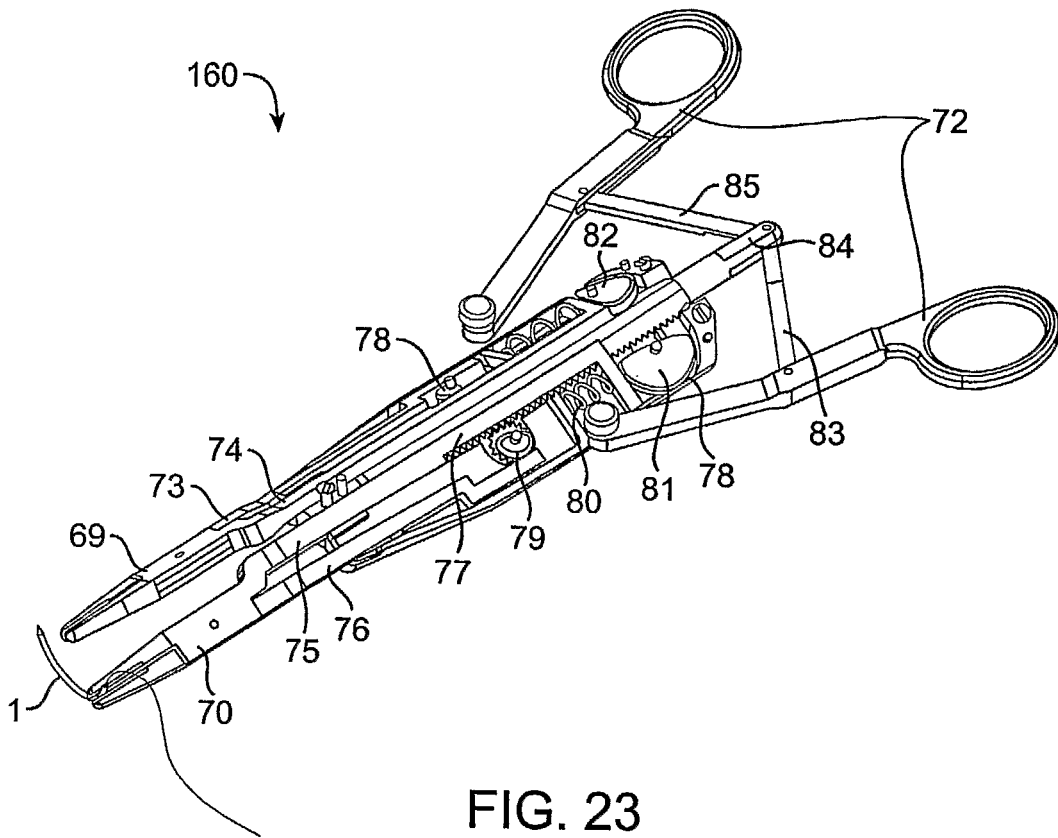


FIG. 23

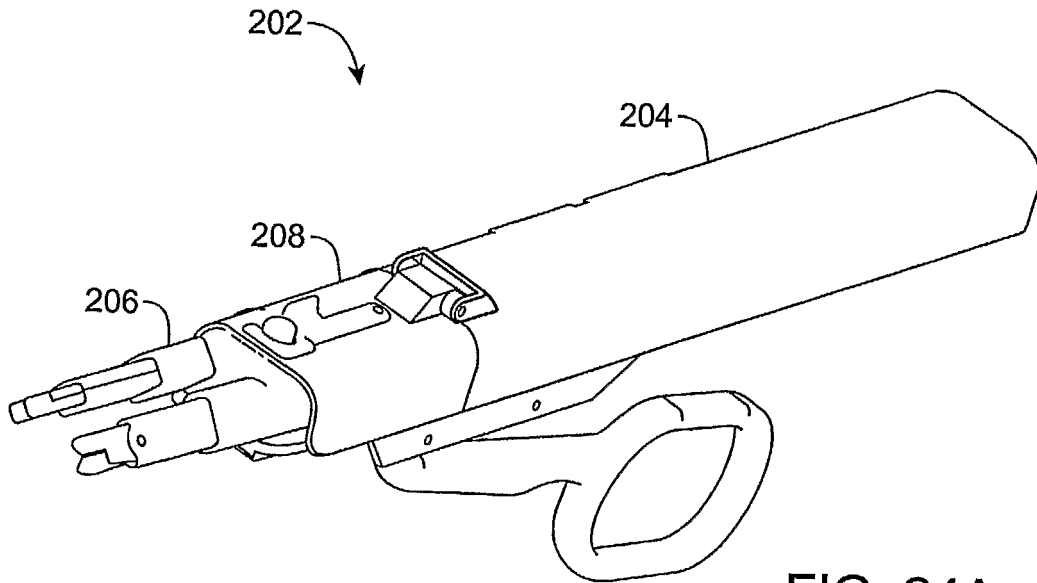


FIG. 24A

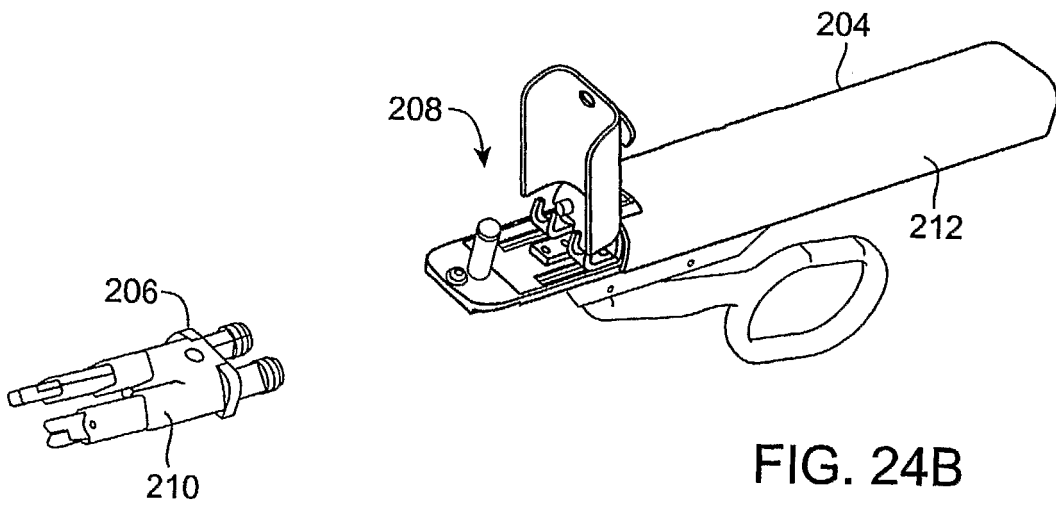


FIG. 24B

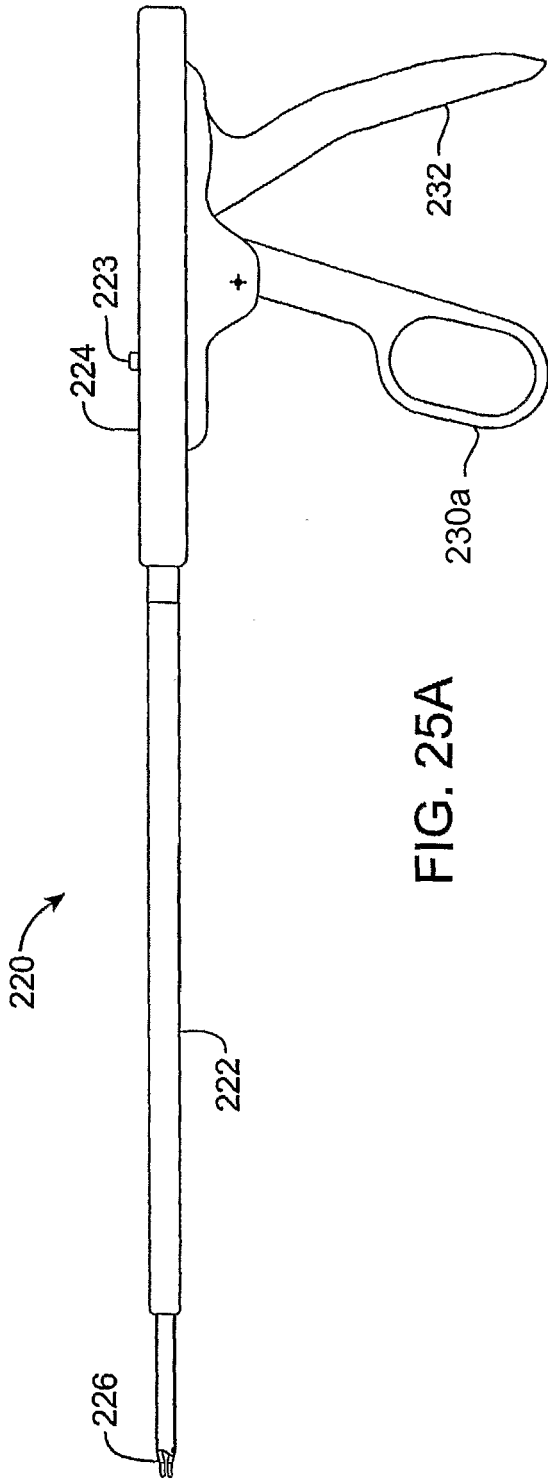


FIG. 25A

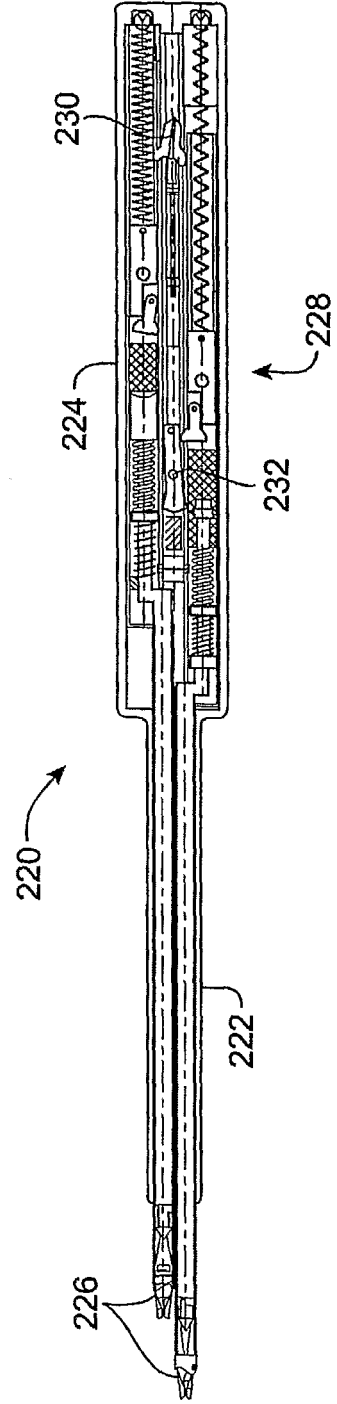


FIG. 25B

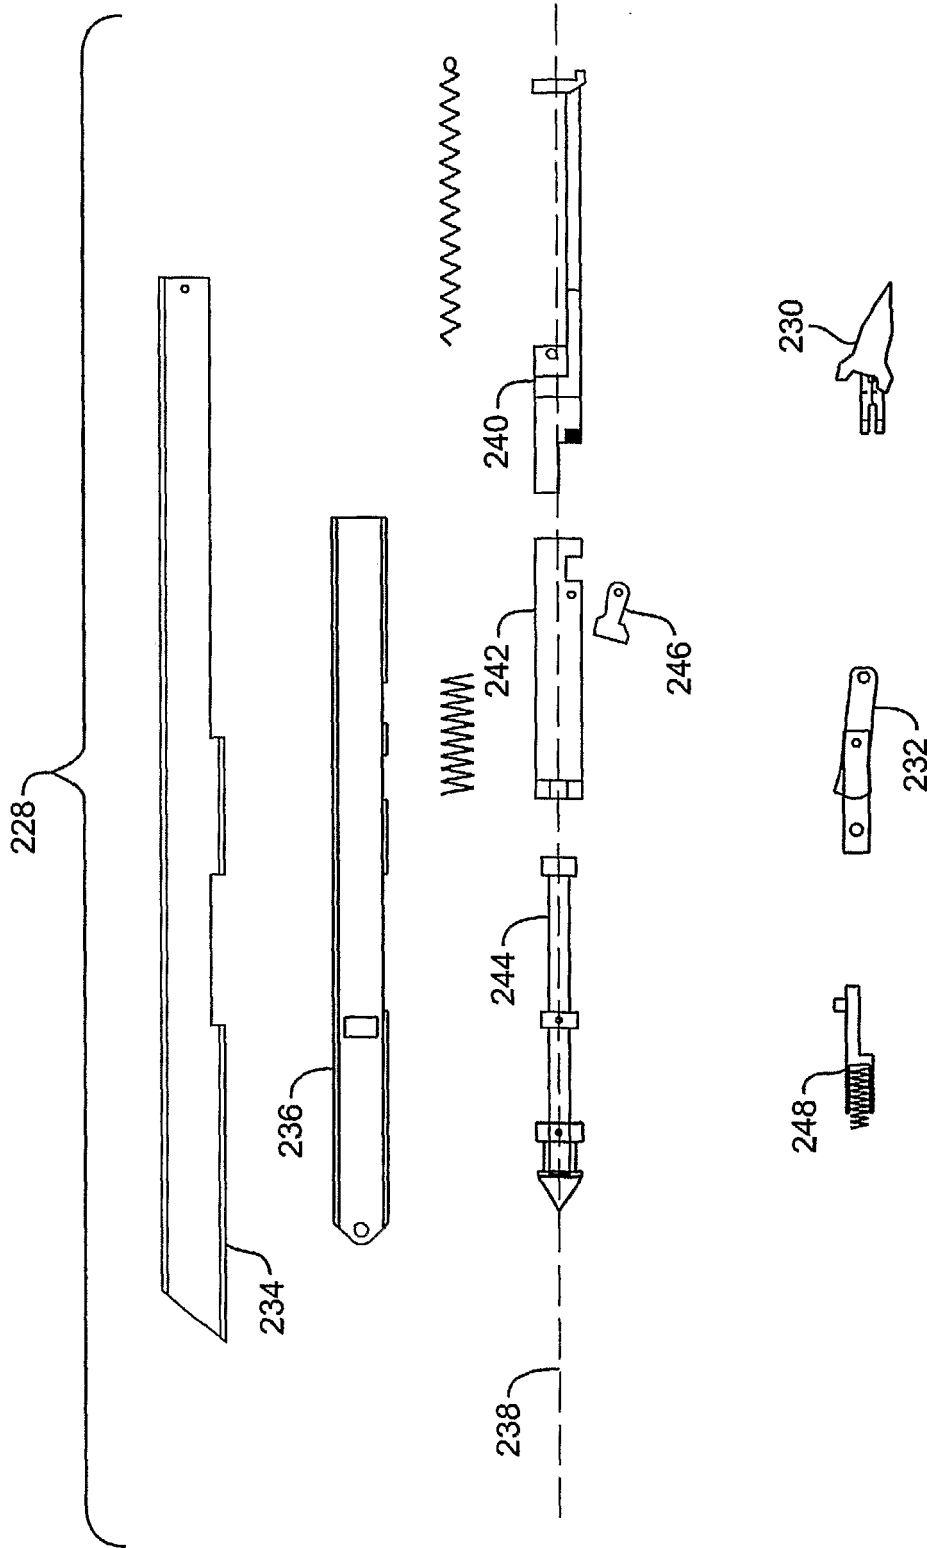


FIG. 26

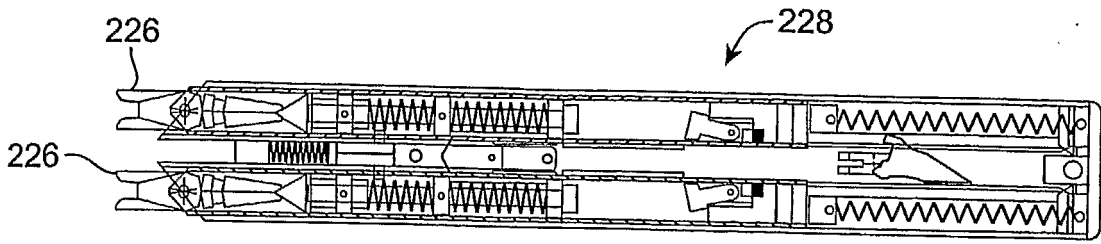


FIG. 26A

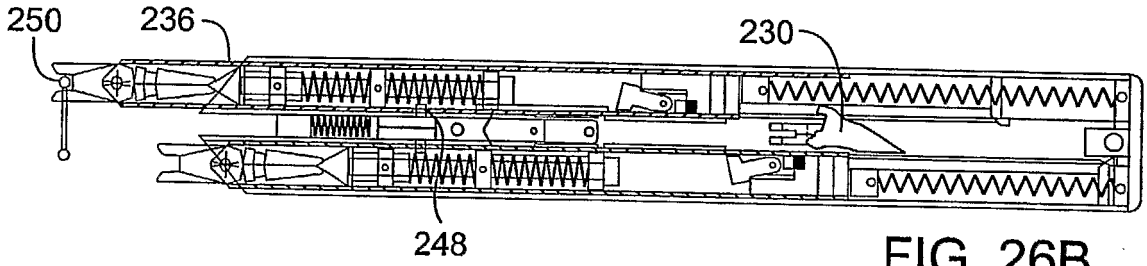


FIG. 26B

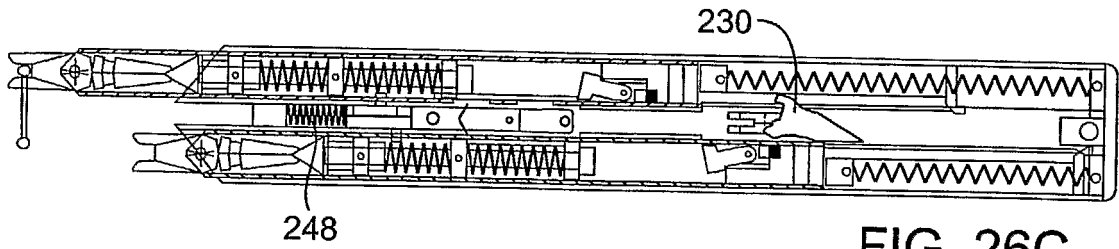


FIG. 26C

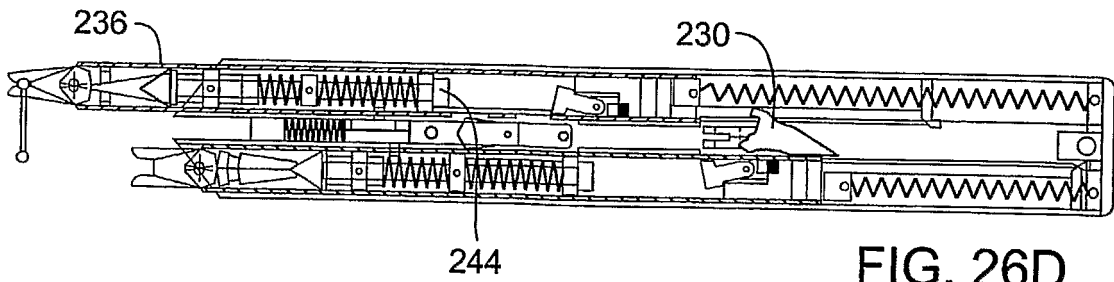


FIG. 26D

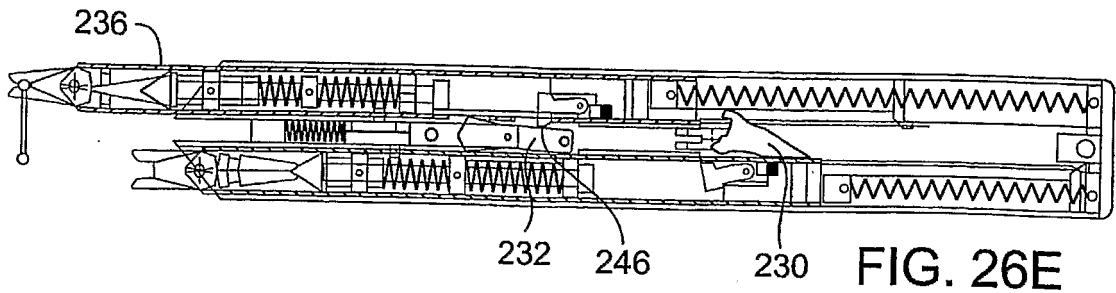


FIG. 26E

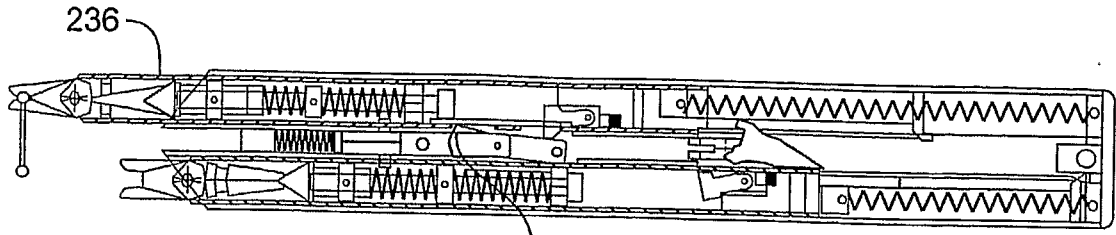


FIG. 26F

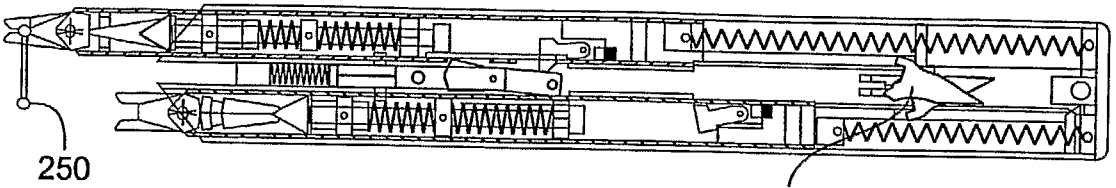


FIG. 26G

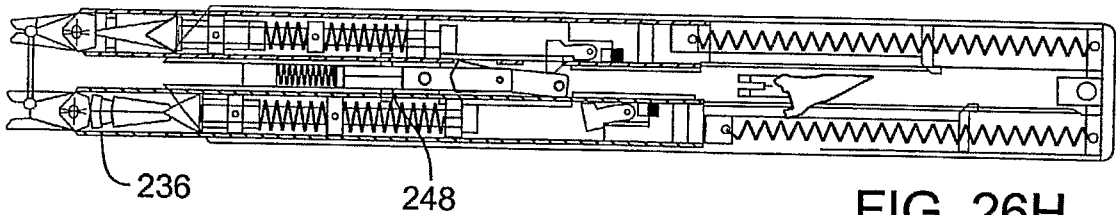


FIG. 26H

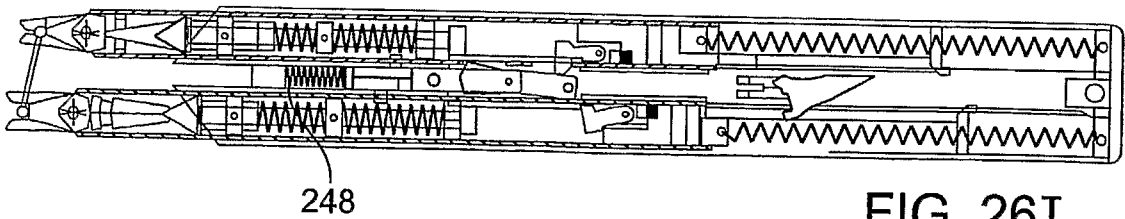


FIG. 26I

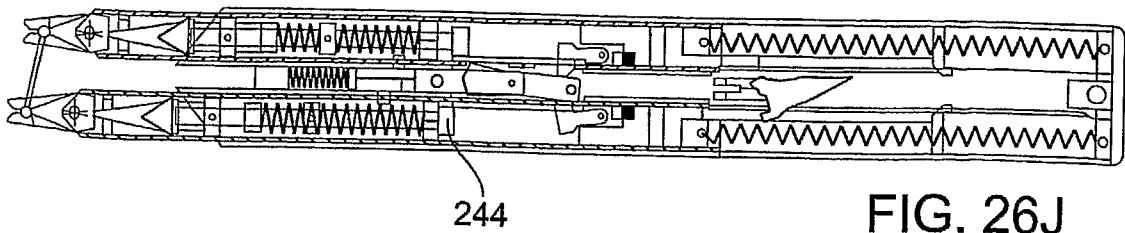


FIG. 26J

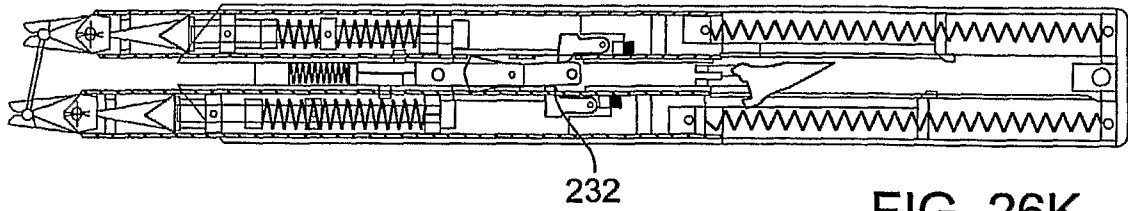


FIG. 26K

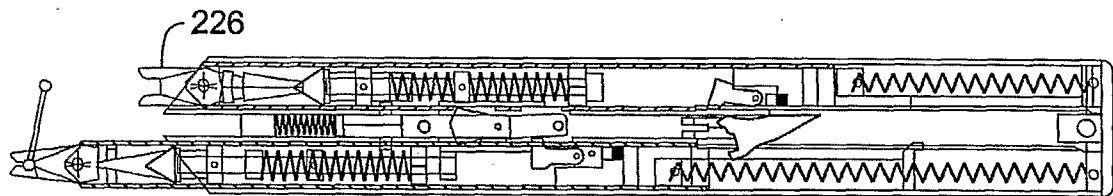


FIG. 26L

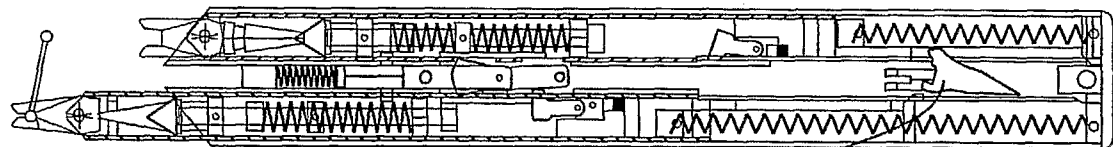
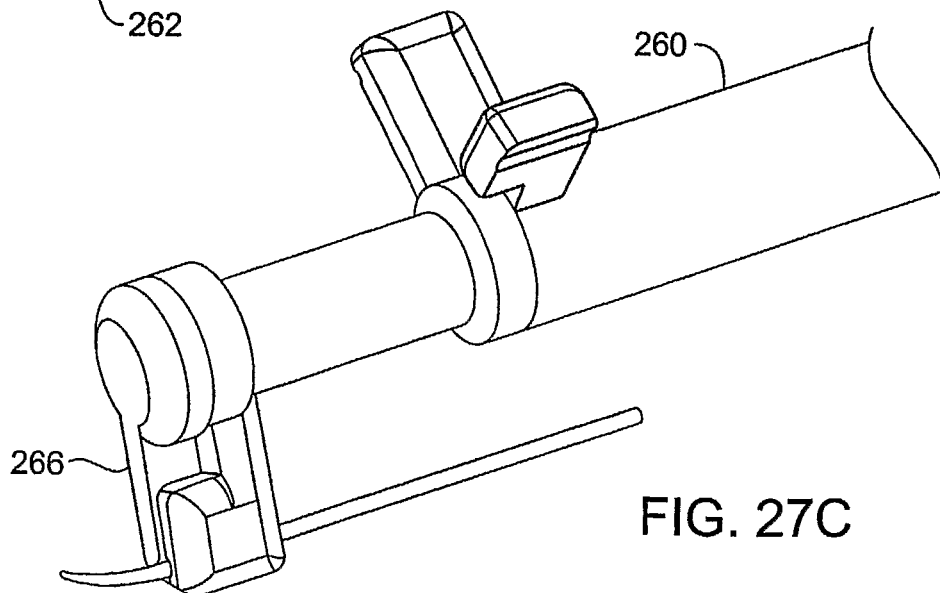
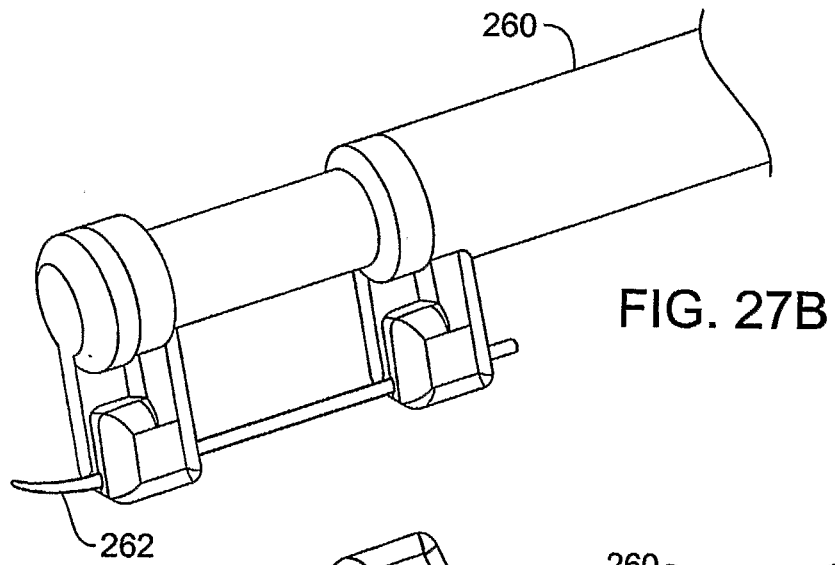
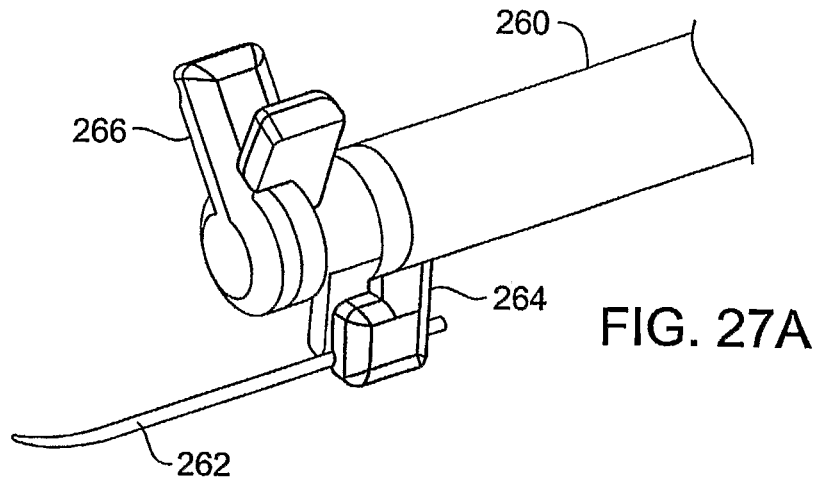


FIG. 26M



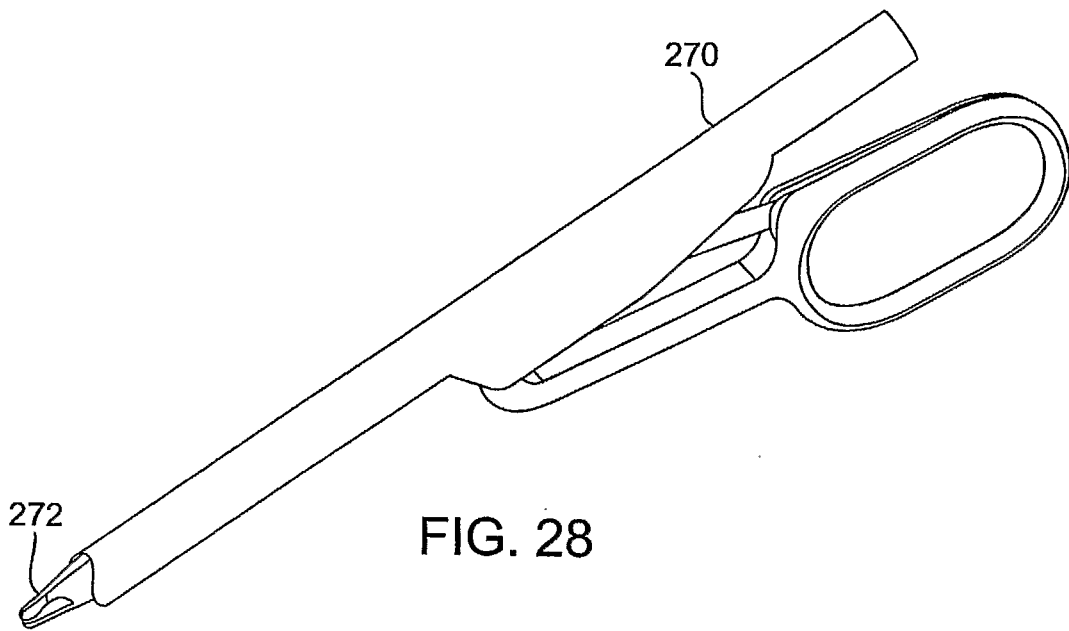


FIG. 28

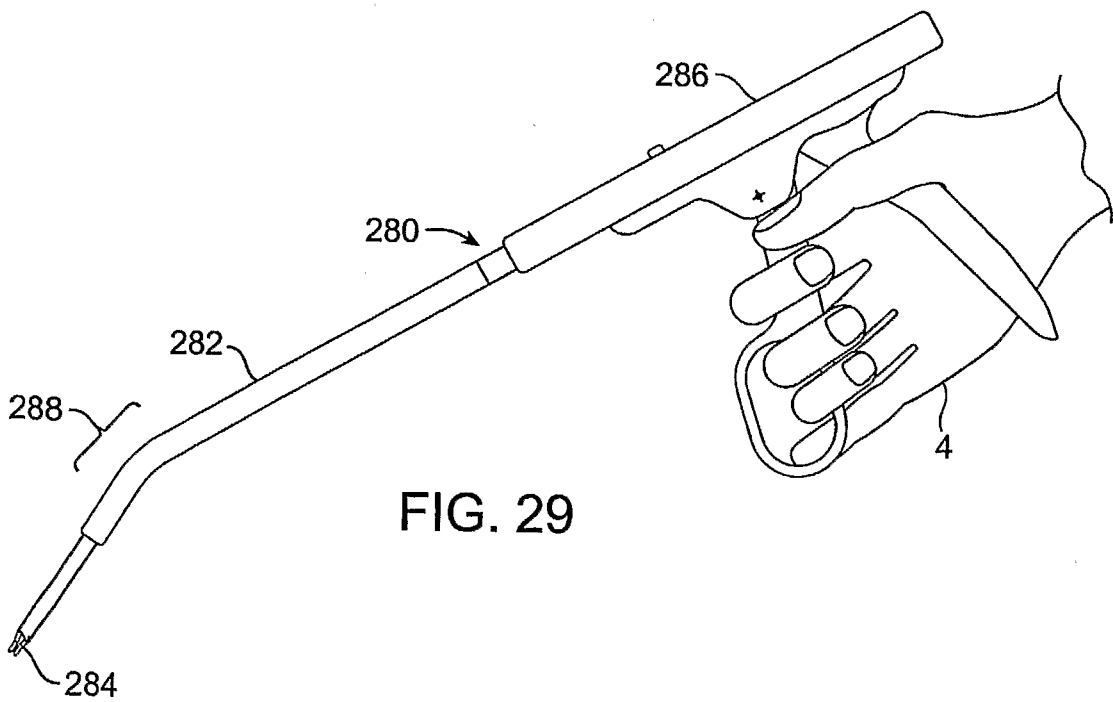


FIG. 29

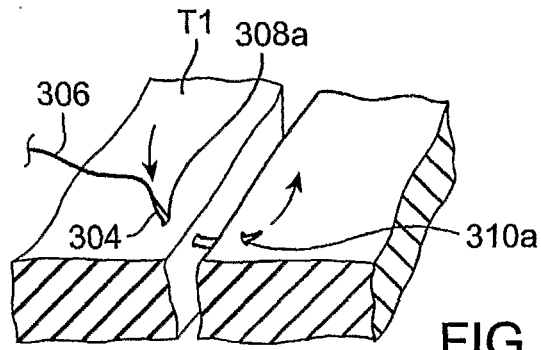


FIG. 30A

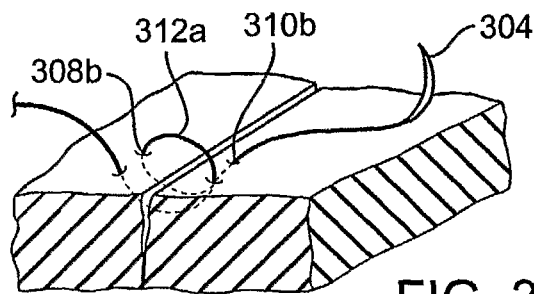


FIG. 30B

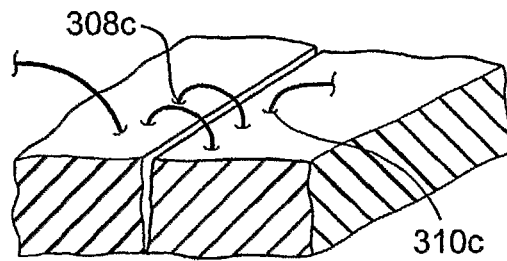


FIG. 30C

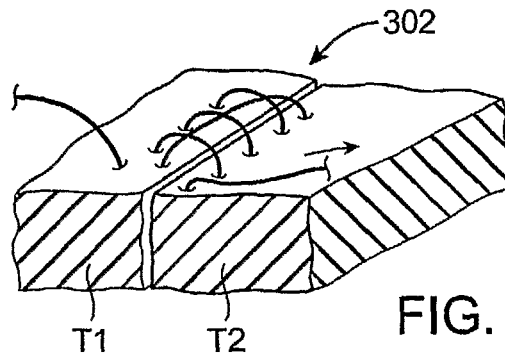


FIG. 30D

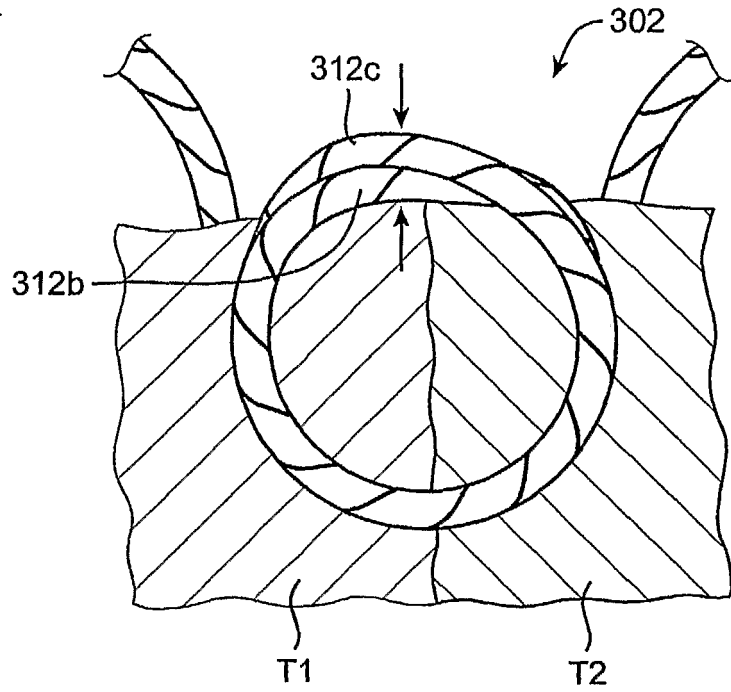


FIG. 31A

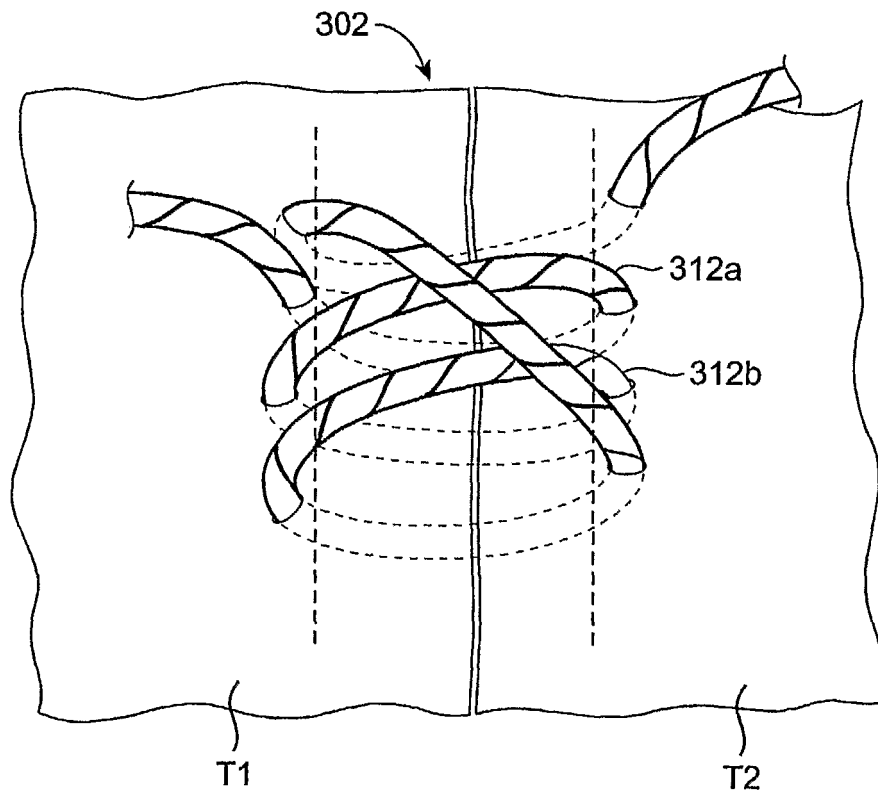


FIG. 31B

**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- US 6126665 A [0009]
- US 5954733 A [0010]
- US 6071289 A [0011]
- US 5938668 A [0012]
- US 5957937 A [0013]
- US 5897563 A [0014]

专利名称(译)	缝合装置，系统和方法		
公开(公告)号	<a href="#">EP1945106A2</a>	公开(公告)日	2008-07-23
申请号	EP2006803567	申请日	2006-09-13
申请(专利权)人(译)	RHAPHIS MEDICAL , INC.		
当前申请(专利权)人(译)	RHAPHIS MEDICAL , INC.		
[标]发明人	HAMILTON HENRY H BELMAN YURI ZATYURYUKIN ALEXANDER BORISOVICH MOORE PATRICIA A		
发明人	HAMILTON, HENRY, H. BELMAN, YURI ZATYURYUKIN, ALEXANDER, BORISOVICH MOORE, PATRICIA, A.		
IPC分类号	A61B17/04 A61B17/10		
CPC分类号	A61B17/062 A61B17/0469 A61B17/2841 A61B2017/00367		
代理机构(译)	WORK , 伊利亚		
优先权	11/227981 2005-09-14 US		
其他公开文献	EP1945106B1 EP1945106A4		
外部链接	<a href="#">Espacenet</a>		

#### 摘要(译)

改进的医疗缝合装置，系统和方法可以将缝合针保持在相对于装置的手柄的固定位置，允许外科医生抓握并操纵缝合装置的手柄以便以类似于以下的方式将针插入组织。使用标准针夹。将手柄从闭合位置循环到打开位置并返回到闭合位置可以在用第一夹子（例如，沿着针的近端部分）夹持针头之间交替装置以用第二夹子夹住针头（例如，沿着针的远端部分并且可选地返回到用第一夹具夹持，其中针通常相对于缝合装置主体停留在基本固定的位置。相关的单夹钳针抓取装置可由外科医生塑性弯曲，和/或具有用手抓住的身体，同时手的一部分致动手柄。