



(11) **EP 3 030 171 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:
01.11.2017 Bulletin 2017/44

(21) Application number: **14756174.0**

(22) Date of filing: **08.08.2014**

(51) Int Cl.:
A61B 17/34^(2006.01) A61M 5/178^(2006.01)

(86) International application number:
PCT/US2014/050446

(87) International publication number:
WO 2015/021448 (12.02.2015 Gazette 2015/06)

(54) **INJECTION DEVICE FOR MINIMALLY INVASIVE PROCEDURES**

INJEKTIONSVORRICHTUNG FÜR MINIMAL INVASIVE EINGRIFFE

DISPOSITIF D'INJECTION POUR INTERVENTIONS PEU INVASIVES

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR
Designated Extension States:
BA ME

(30) Priority: **08.08.2013 US 201361863888 P**

(43) Date of publication of application:
15.06.2016 Bulletin 2016/24

(73) Proprietor: **Global Bio Therapeutics, Inc.**
San Diego, CA 92122 (US)

(72) Inventors:
• **CABRERA AQUINO, Jose Gustavo**
Del. Tlalpan
C.P. 14260 Mexico D.F. (MX)

• **SEGURA PACHECO, Blanca Angelica**
C.P. 18900 Mexico D.F. (MX)
• **GERKEN, Steven**
Encinitas, CA 92024 (US)
• **MASTERSON, Steven**
Encinitas, CA 92024 (US)

(74) Representative: **Boult Wade Tennant**
Verulam Gardens
70 Gray's Inn Road
London WC1X 8BT (GB)

(56) References cited:
WO-A1-2013/107068 US-A- 4 763 667
US-A- 6 004 295 US-A1- 2006 200 083
US-A1- 2009 270 806 US-A1- 2010 048 990
US-A1- 2010 217 073 US-A1- 2010 312 173
US-A1- 2011 160 533 US-B1- 6 723 082
US-B1- 6 743 206

EP 3 030 171 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

predetermined depths.

FIELD OF THE INVENTION

[0001] Provided herein is an injection device that can be used in minimally invasive procedures, including surgeries such as laparoscopic surgeries, for direct administration of a fluid, such as a therapeutic, to a target tissue or organ.

BACKGROUND

[0002] Many medical procedures, including minimally invasive procedures, can require direct injection of a fluid, such as a therapeutic, to a target tissue. Such procedures can require that the needle is inserted through a port at a distance far from the operator. This can create safety concerns, since it can be easy to puncture non-target tissues and/or to inadvertently puncture or pierce through tissues or organs with the needle. Thus, there is a need for injection devices that can be used in minimally invasive procedures that overcome these problems.

[0003] US2010/0312173 describes injection devices for delivering a medical agent to a plurality of locations within a patient tissue volume such as the interior space of a spinal disc, and removing material from the space during delivery. The medical agent is delivered to multiple sites using a plurality of curved needles without the need to reposition the device. A cannulated sleeve is positioned at the desired location and a syringe is moved proximally or distally in relation to the sleeve, driving the needles into the tissue. The two part form of claim 1 is based on this document. US 4,763,667 describes a tissue-penetrating catheter device that includes an inner catheter assembly attached to a needle at one end and a shaft at the other, and an outer catheter assembly through which the inner catheter is movable.

[0004] US 6,723,082 describes a tissue-penetrating catheter device for delivering an angiogenic agent to a site within the heart. The needle is extended distally beyond the distal end of a sheath by repositioning a slider, and a desired therapeutic substance can be injected into the tissue by the injector.

[0005] US 2011/0160533 describes a catheter device for delivery of a drug to uterine tissue. The device includes a first elongate member, a second elongate member and a stopper device, which is configured to control movement of the second elongate member within the first elongate member, thereby defining the retracted and extended positions. The device can include a needle within an outer sheath to deliver the drug to the tissue.

[0006] US 2010/048990 describes transluminal access devices that include a catheter, an inflatable member, a hollow needle, a stylet and a guide wire. The movement of the endoscopic needle shaft can be used to move the needle tip between a retracted position and an extended position. The needle shaft can include a depth gauge to control the extension of the needle to various

REFERENCE NUMERALS LIST

[0007] The following list indicates the terms used and the corresponding reference numerals. Reference to each should be made with respect to the description below and the accompanying Drawings. Reference numerals should not however be seen as limiting the extent of the matter protected by the claims.

5	60, 60' or 60" -	laparoscopic injection device
	71 or 71' -	needle sheath controller
	710 -	needle sheath controller housing
	711 -	positioner
	711a -	positioner - forward position
	711b -	positioner - intermediate position
	711c -	positioner - rearward position
	712 -	lock and release element
	713 -	connection member
	715 -	distal sheath stop
	716 -	proximal sheath stop
	717 -	controller lumen
	72, 72' or 72" -	needle sheath
	72a -	needle sheath - sheathed position
	72b -	needle sheath - transitional position
	72c -	needle sheath - unsheathed position
	720 -	proximal portion of the needle sheath
	723 -	needle sheath lumen
	724 -	visibility window
	725 -	visibility window
	726 -	open cavity
	73 or 73' -	needle sheath distal tip
	733 -	needle channel
	76 -	needle groove
	81 -	injection needle
	82 -	coupling member
	83 -	injection tube
	84 -	needle hub
	85 -	needle coupler
	900a -	standard syringe - detached position
	900b -	standard syringe - connected position
	910 -	dockable syringe
	910a -	dockable syringe - undocked position
	910b -	dockable syringe - docked position
	91, 91' or 91" -	syringe barrel
	92, 92' or 92" -	plunger
	920 -	auxiliary plunger
	93 -	Luer fit adaptor

- 94 - syringe barrel base
 95 or 95' - plunger head
 951 - plunger adaptor
 96 - syringe adaptor lining
 960 - plunger rest cavity
 961 - barrel dock
 962 - barrel rest cavity
 963 - barrel dock

SUMMARY

[0008] The present invention provides an injection device, comprising: a syringe barrel (91), wherein the syringe barrel provides a fluid reservoir; a plunger (92) configured to be controlled by the operator of the device and to move within the syringe barrel for loading and releasing fluid from the fluid reservoir in the syringe barrel; and is characterized by further comprising:

- a) an injection needle (81) that is fixed and operably coupled to the syringe barrel (91) providing a fluid pathway for fluid contained in the syringe barrel to be injected into a target tissue when the plunger (92) is depressed, wherein extraction or retraction of the needle is independent of movement of the plunger; b) an elongate sheath (72), comprising an internal lumen (723) that contains the injection needle and having a distal tip that contains an opening for the injection needle, wherein: the sheath is movable around the injection needle; and control of the sheath is independent from movement of the plunger; and c) a controller (71) for positioning the sheath, comprising:

a housing (710), comprising at least a first (715) and second (716) stop to control exposure of the injection needle and that are provided within the housing at a predetermined distance from each other, wherein the stops can be locked; a central lumen (717) in the housing comprising a connection member, wherein the connection member (713) is configured to be movable in the central lumen in the housing and is coupled to the sheath, wherein the proximal end of the sheath is coupled to the distal end of the connection member so that movement of the connection member controls movement of the sheath; and

a positioner (711) mounted within the housing configured to move forward towards the distal end of the controller and rearward towards the proximal end of the controller, between the stops in the housing, wherein the positioner is operatively connected to the connection member to guide movement of the connection member in the same direction, whereby movement of the positioner forward towards the distal end engages the first stop and moves the sheath to enclose

the injection needle inside the lumen of the sheath (711a, 72a), and movement of the positioner rearward towards the proximal end engages the second stop and moves the sheath to expose no more than a predetermined length of the distal tip of the injection needle (711c, 72c) through the opening in the injection needle for injection into the tissue.

[0009] Provided herein are injection devices according to the present claims used for direct injection of a fluid, such as a therapeutic, to a target site of a subject, such as a target tissue or organ. The injection device can be used in minimally invasive procedures, such as surgeries and other procedures, for example in laparoscopic surgery. Also provided herein are injection devices according to the present claims for use in a method, including in medical applications to treat diseases and conditions. As provided herein, the injection device includes a) a syringe barrel, in which the syringe barrel provides a fluid reservoir; b) a plunger configured to be controlled by the operator of the device and to move within the syringe barrel for loading and releasing fluid from the fluid reservoir in the syringe barrel; c) an injection needle that is operably coupled to the syringe barrel providing a fluid pathway for fluid contained in the syringe barrel to be injected into a target tissue when the plunger is depressed; d) an elongate sheath, which includes an internal lumen that contains the injection needle and having a distal tip that contains an opening for the injection needle; and e) a controller for positioning the sheath, which includes a housing, including at least a first and second stop to control exposure of the injection needle and that are provided within the housing at a predetermined distance from each other; a central lumen in the housing including a connection member, in which the connection member is configured to be movable in the central lumen in the housing and is coupled to the sheath, in which the proximal end of the sheath is coupled to the distal end of the connection member so that movement of the connection member controls movement of the sheath; and a positioner mounted within the housing configured to move forward towards the distal end of the controller and rearward towards the proximal end of the controller, between the stops in the housing, in which the positioner is operatively connected to the connection member to guide movement of the connection member in the same direction, whereby movement of the positioner forward towards the distal end engages the first stop and moves the sheath to enclose the injection needle inside the lumen of the sheath, and movement of the positioner rearward towards the proximal end engages the second stop and moves the sheath to expose no more than a predetermined length of the distal tip of the injection needle through the opening in the injection needle for injection into the tissue.

[0010] In examples of any of the injection devices here-

in, the elongate sheath has a sufficient length and width to reach an organ through an endoscopic port. For example, the elongate sheath generally has a length from its proximal to distal end of from or from about 200 mm to 600 mm and a diameter of from or from about 2 mm to 15 mm, and typically a length from its proximal to distal end of from or from about 250 to 400 mm and a diameter of 4 mm to 12 mm. For example, the elongate sheath has a length from its proximal to distal end of at least or about at least 300 mm and a diameter of at least or about at least 5 mm, 6 mm, 7 mm, 8 mm, 9 mm or 10 mm.

[0011] In examples of any of the injection devices herein, the predetermined length of the distal tip of the injection needle is generally 1 mm to 10 mm, 2 mm to 8 mm, 4 mm to 6 mm or 2 mm to 3 mm, and typically less than 10 mm, 9 mm, 8 mm, 7 mm, 6 mm, 5 mm, 4 mm, 3 mm, 2 mm or less. For example, the predetermined length is less than 5 mm.

[0012] In examples of any of the injection devices herein, the injection device can include at least 3 stops, 4 stops or 5 stops, in which the second stop is the most proximal stop and the first stop is the most distal stop and the other stop or stops are positioned between the first stop and the second stop; and each stop is positioned at a predetermined distance from adjacent stop or stops to control exposure of the needle to different predetermined lengths, in which the second stop controls exposure of the needle its longest predetermined length, whereby the positioner can move between the adjacent stops to engage with the stop to expose different predetermined lengths of the injection needle. Generally, the predetermined distance between stops is substantially the same as the predetermined length of the exposed injection needle.

[0013] In examples of any of the injection devices herein, the positioner can include a lock and release element that is configured in the positioner to engage the positioner with the stops. Typically, the lock and release element is a spring that provides an upward force against the positioner and a downward force against the connection member to lock the positioner into the stop, and is capable of being compressed to release the positioner from the stop.

[0014] In examples of any of the injection devices herein, the injection needle typically is 5 mm to 40 mm in length, and 25 gauge to 34 gauge, 25 gauge to 30 gauge or 26 gauge to 28 gauge. For example, injection needle is or is about 27 gauge.

[0015] In examples of any of the injection devices herein, the syringe barrel can be either proximal or distal to the controller.

[0016] In particular examples of the injection devices provided herein, the syringe barrel is proximal to the controller and is operably coupled to the injection needle by an injection tube, in which: the injection tube includes a proximal and a distal end, in which the proximal end is connected to the syringe barrel and the distal end connected to the injection needle; and the controller is con-

figured to hold the injection tube and includes an opening at the proximal end so that the injection tube extends out of the controller to connect to the syringe barrel. In particular examples, the syringe barrel is configured to be connected to the injection tube so that the syringe barrel is detachable from the device. The syringe barrel can be connected to the injection tube, which includes a hub on its proximal end that is compatible with an adaptor on the distal end of the syringe barrel, and the hub of the injection tube connects to the adaptor of the syringe barrel.

[0017] In particular examples herein, the injection tube is fixed in the controller; the connection member in the controller includes a recess by which the injection tube is routed to pass from the controller into the sheath at the junction where the connection member is coupled to the sheath; and the connection member is movable around the injection tube. In some examples, the injection tube is connected directly to the injection needle. In other examples, the injection tube is connected indirectly to the injection needle via a coupler, the coupler having a proximal and distal end, the proximal end connected to the distal end of the injection tube and the distal end connected to the proximal end of the injection needle. The injection tube and injection needle can be the same gauge or a different gauges. In particular examples provided herein, the injection tube has a larger outer diameter than the injection needle; the injection needle can be 25 gauge to 34 gauge, 25 gauge to 30 gauge or 26 gauge to 28 gauge; and the injection tube can be 15 gauge to 25 gauge or 20 gauge to 25 gauge. For example, the injection needle is or is about 27 gauge and the injection tube is or is about 21 gauge.

[0018] In examples of any of the injection devices herein, the sheath can be opaque or transparent. In some examples of the injection devices provided herein, the coupler is opaque or transparent. In particular examples, the sheath is opaque; the coupler is transparent; and the sheath includes a window configured in the sheath to view the coupler.

[0019] In examples of any of the injection devices herein, the injection device can include a) a syringe barrel, in which the syringe barrel provides a fluid reservoir; b) a plunger configured to be controlled by the operator of the device and to move within the syringe barrel for loading and releasing fluid from the fluid reservoir in the syringe barrel; c) an injection needle that is operably coupled to the syringe barrel providing a fluid pathway for fluid contained in the syringe barrel to be injected into a target tissue when the plunger is depressed, in which: the injection needle is operably coupled to the syringe barrel by an injection tube, the injection tube includes a proximal and a distal end, the proximal end connected to the syringe barrel and the distal end directly or indirectly connected to the injection needle; the injection needle is 25 gauge to 34 gauge and has a length in the range from 5 mm to 40 mm; and the injection tube has a larger diameter than the injection needle that is has a smaller diameter than 25 gauge and is connected to the syringe barrel; d)

an elongate sheath, which includes an internal lumen that contains the injection tube and injection needle and having a distal tip that contains an opening for the injection needle, in which the sheath is movable around the injection needle; and e) a controller for positioning the sheath, in which the controller is distal to the syringe barrel and plunger and which includes: a housing, including at least a first and second stop to control exposure of the injection needle and that are provided within the housing at a predetermined distance from each other; a cavity for the injection tube and an opening at the proximal end so that the injection tube extends out of the controller to connect to the syringe barrel, in which the injection tube is fixed in the controller; a central lumen in the housing which includes a connection member, in which: the connection member in the controller includes a recess by which the injection tube is routed to pass from the controller into the distal lumen of the sheath at the junction where the connection member is coupled to the sheath; the connection member is configured to be movable in the central lumen in the housing around the injection tube and is coupled to the sheath, in which the proximal end of the sheath is coupled to the distal end of the connection member so that movement of the connection member controls movement of the sheath; and a positioner mounted within the housing configured to move forward towards the distal end of the controller and rearward towards the proximal end of the controller, between the stops in the housing, in which the positioner is operatively connected to the connection member to guide movement of the connection member in the same direction, whereby movement of the positioner forward towards the distal end engages the first stop and moves the sheath to enclose the injection needle inside the lumen of the sheath, and movement of the positioner rearward towards the proximal end engages the second stop and moves the sheath to expose no more than a predetermined length of the distal tip of the injection needle through the opening in the injection needle for injection into the tissue

[0020] In some examples provided herein, the total length of the injection tube and injection needle is as long as the controller and sheath. For example, the total length of the injection tube and injection needle can be 100 mm to 600 mm or 200 mm to 400 mm.

[0021] In some examples of the injection device provided herein, the syringe barrel is positioned distal to the controller and the internal lumen of the sheath includes the syringe barrel in its distal end; and the syringe barrel is configured in the lumen so that the sheath is movable around the syringe barrel. In particular examples, the sheath encloses the syringe barrel. In particular examples, the sheath can include a window to view the syringe barrel. In particular examples, the sheath includes an open cavity that includes the syringe barrel, where the open cavity of the sheath includes a lining that is configured in the sheath so that the sheath is movable around the lining; and the syringe barrel is mounted into the lining in the open cavity. In some examples, the open cavity

extends the length of the sheath. The sheath can be enclosed at its proximal end and provides a conduit for the plunger and the open cavity is present at the distal end of the sheath.

5 **[0022]** In some examples provided herein, the plunger is extended to engage with the syringe barrel in the distal end of the lumen of the sheath and arranged so that the plunger is movable through the controller and within the lumen of the sheath.

10 **[0023]** In some examples provided herein, the plunger is longer than the sheath and has a length that is from or from about 100 mm to 600 mm or 200 mm to 500 mm.

[0024] In some examples provided herein, the plunger is operably connected to an auxiliary plunger provided in the lumen of the sheath; and the plunger is extended to engage with the auxiliary plunger in the lumen of the sheath and arranged so that the plunger is movable through the controller and sheath and the auxiliary plunger is movable through the sheath and configured to move within the syringe barrel, whereby depressing the plunger depresses the auxiliary plunger into the syringe barrel releasing fluid from the fluid reservoir in the syringe barrel and pulling back on the plunger pulls back on the auxiliary plunger to load fluid into the fluid reservoir in the syringe barrel. In particular examples, the plunger includes an adaptor at its distal end to connect to the proximal end of the auxiliary plunger. The sheath can include an open cavity which includes a detachable syringe; and the detachable syringe includes the syringe barrel, the auxiliary plunger having a distal end configured to be movable in the syringe barrel and a proximal end coupled to the plunger, and the injection needle that is operably coupled to the syringe. The open cavity of the sheath can include a lining that is configured in the sheath so that the sheath is movable around the lining; and the detachable syringe is mounted into the lining in the open cavity. In particular examples, the controller is configured to hold the plunger so that the plunger is movable within the controller, and the controller that includes: an opening at its proximal end to receive the plunger; and a recess in the connection member of the controller by which the plunger is routed to pass from the controller into the lumen of the sheath at the junction where the connection member is coupled to the sheath, in which the plunger and connection member move independently with respect to each other.

45 **[0025]** In some examples provided herein, the injection device includes a) a syringe barrel, in which the syringe barrel provides a fluid reservoir; b) an extended plunger configured to be controlled by the operator of the device and coupled to an auxiliary plunger to move within the syringe barrel for loading and releasing fluid from the fluid reservoir in the syringe barrel, whereby depressing the plunger depresses the auxiliary plunger into the syringe barrel releasing fluid from the fluid reservoir in the syringe barrel and pulling back on the plunger pulls back on the auxiliary plunger to load fluid into the fluid reservoir in the syringe barrel; c) an injection needle that is operably coupled to the syringe barrel providing a fluid pathway for

fluid contained in the syringe barrel to be injected into a target tissue when the plunger is depressed, in which the injection needle is 25 gauge to 34 gauge and has a length in the range from 5 mm to 40 mm; d) an elongate sheath, which includes an internal lumen that contains the plunger, the auxiliary plunger, the syringe barrel and the injection needle and having a distal tip that contains an opening for the injection needle, in which: the sheath is enclosed at its proximal end and provides a conduit for the plunger, in which the plunger is movable through the sheath; the sheath includes an open cavity at the distal end, the open cavity which includes the auxiliary plunger, syringe barrel and injection needle, in which: the open cavity of the sheath includes a lining that is configured in the sheath so that the sheath is movable around the lining; the auxiliary plunger, syringe barrel and injection needle are mounted into the lining in the open cavity; and the auxiliary plunger, syringe barrel and injection needle are detachable as a unit from the open cavity; the sheath is movable around the plunger, auxiliary plunger, syringe barrel and injection needle; and e) a controller for positioning the sheath, which includes: a housing, including at least a first and second stop to control exposure of the injection needle and that are provided within the housing at a predetermined distance from each other; an opening at its proximal end to receive the plunger and which includes a cavity configured to hold the plunger so that the plunger is movable within the controller; a central lumen in the housing including a connection member, in which: the connection member includes a recess by which the plunger is routed to pass from the controller into the distal lumen of the sheath at the junction where the connection member is coupled to the sheath, in which the plunger and connection member move independently with respect to each other; the connection member is configured to be movable in the central lumen in the housing and is coupled to the sheath, in which the proximal end of the sheath is coupled to the distal end of the connection member so that movement of the connection member controls movement of the sheath; and a positioner mounted within the housing configured to move forward towards the distal end of the controller and rearward towards the proximal end of the controller, between the stops in the housing, in which the positioner is operatively connected to the connection member to guide movement of the connection member in the same direction, whereby movement of the positioner forward towards the distal end engages the first stop and moves the sheath to enclose the injection needle inside the lumen of the sheath, and movement of the positioner rearward towards the proximal end engages the second stop and moves the sheath to expose no more than a predetermined length of the distal tip of the injection needle through the opening in the injection needle for injection into the tissue.

[0026] In some examples provided herein, the injection device includes a) a syringe barrel, in which the syringe barrel provides a fluid reservoir; b) an extended plunger configured to be controlled by the operator of the device

to move within the syringe barrel for loading and releasing fluid from the fluid reservoir in the syringe barrel; c) an injection needle that is operably coupled to the syringe barrel providing a fluid pathway for fluid contained in the syringe barrel to be injected into a target tissue when the plunger is depressed, in which the injection needle is 25 gauge to 34 gauge and has a length in the range from 5 mm to 40 mm; d) an elongate sheath, which includes an internal lumen that contains the plunger, the syringe barrel and the injection needle and having a distal tip that contains an opening for the injection needle, in which: the sheath is enclosed to provide a conduit for the plunger, in which the plunger is movable through the sheath; the sheath includes an a window to view the syringe barrel; the sheath is movable around the plunger, syringe barrel and injection needle; and e) a controller for positioning the sheath, which includes: a housing, including at least a first and second stop to control exposure of the injection needle and that are provided within the housing at a predetermined distance from each other; an opening at its proximal end to receive the plunger and including a cavity configured to hold the plunger so that the plunger is movable within the controller; a central lumen in the housing including a connection member, in which: the connection member includes a recess by which the plunger is routed to pass from the controller into the distal lumen of the sheath at the junction where the connection member is coupled to the sheath, in which the plunger and connection member move independently with respect to each other; the connection member is configured to be movable in the central lumen in the housing and is coupled to the sheath, in which the proximal end of the sheath is coupled to the distal end of the connection member so that movement of the connection member controls movement of the sheath; and a positioner mounted within the housing configured to move forward towards the distal end of the controller and rearward towards the proximal end of the controller, between the stops in the housing, in which the positioner is operatively connected to the connection member to guide movement of the connection member in the same direction, whereby movement of the positioner forward towards the distal end engages the first stop and moves the sheath to enclose the injection needle inside the lumen of the sheath, and movement of the positioner rearward towards the proximal end engages the second stop and moves the sheath to expose no more than a predetermined length of the distal tip of the injection needle through the opening in the injection needle for injection into the tissue.

[0027] In examples of any of the injection devices herein, the syringe barrel can be transparent and configured to hold 0.2 mL to 10 mL of fluid, 0.5 mL to 5 mL of fluid or 0.5 to 2 mL of fluid. For example, the syringe barrel holds at least or about at least or about 1 mL of fluid. The syringe barrel can be disposable or is re-usable.

[0028] In examples of any of the injection devices herein, the device can be disposable or is re-usable. The device is for delivering a therapeutic to an organ or tissue.

The therapeutic can be a biologic, chemotherapeutic or gene therapy agent. For example, the therapeutic is a small molecule drug, prodrug, protein, peptide, DNA, RNA, virus, antibody, organic molecule, saccharide, polysaccharide, lipid and combinations or conjugates thereof.

[0029] Also provided herein are injection devices according to the present claims for use in a method of directly administering a fluid to a tissue or an organ in a subject during a minimally invasive procedure, which includes: inserting any of the injection devices provided herein into a port or cannula configured to provide access to the tissue or organ during the minimally invasive procedure; and depressing the plunger to inject the fluid into the tissue. Methods provided herein include providing the device for inserting into the port with the positioner moved forward towards the distal end to engage with the first stop to move the sheath to enclose the injection needle inside the lumen of the sheath; and prior to depressing the plunger, moving the positioner rearward toward the proximal end to engage the second stop to move the sheath to expose the injection needle. In any of the methods provided herein, the tissue or organ is selected from among liver, brain spinal cord, pancreas, heart, skin, kidney, lung, blood vessel, bone, muscle, uterus, cervix, prostate, urethra, and intestine.

[0030] In any of the methods described herein, the fluid is a composition including a therapeutic, which can be a biologic, chemotherapeutic or gene therapy agent. In any of the methods provided herein, the composition is a pharmaceutical composition.

[0031] In any of the methods described herein, the therapeutic is a small molecule drug, prodrug, protein, peptide, DNA, RNA, virus, antibody, organic molecule, saccharide, polysaccharide, lipid and combinations or conjugates thereof. For example, the therapeutic can be a gene therapy agent, a chemotherapeutic agent, an analgesic agent, an anti-inflammatory agent, an antimicrobial agent, an amoebicidal agent, a trichomonocidal agent, an anti-parkinson agent, an anti-malarial agent, an anticonvulsant agent, an anti-depressant agent, and antiarthritics agent, an anti-fungal agent, an antihypertensive agent, antipyretic agent, an anti-parasite agent, an antihistamine agent, an alpha-adrenergic agonist agent, an alpha blocker agent, an anesthetic agent, a bronchi dilator agent, a biocide agent, a bactericide agent, a bacteriostat agent, a beta-adrenergic blocker agent, a calcium channel blocker agent, a cardiovascular drug agent, a contraceptive agent, a decongestant agent, a diuretic agent, a depressant agent, a diagnostic agent, an electrolyte agent, a hypnotic agent, a hormone agent, a hyperglycemic agent, a muscle relaxant agent, a muscle contractant agent, an ophthalmic agent, a parasympathomimetic agent, a psychic energizer agent, a sedative agent, a sympathomimetic agent, a tranquilizer agent, a urinary agent, a vaginal agent, a viricide agent, a vitamin agent, a non-steroidal anti-inflammatory agent, an angiotensin converting enzyme inhibitor agent, an al-

cohol, or a sleep inducer. The therapeutic can be a polypeptide selected from among an enzyme, a hormone, a coagulation or clotting factor, a cytokine, a growth factor or active portion thereof, an antibody or antigen binding portions of antibodies, an angiogenesis modulator, an immunomodulator, a pain modulator, a receptor or active portion thereof, a transport protein, a regulatory protein, an antigen or an allergen.

[0032] In any of the methods described herein, the therapeutic can be a nucleic acid molecule for gene therapy, and the nucleic acid molecule can encode a polypeptide. The encoded polypeptide can be an enzyme, a hormone, a coagulation or clotting factor, a cytokine, a growth factor or active portion thereof, an antibody or antigen binding portions of antibodies, an angiogenesis modulator, an immunomodulator, a pain modulator, a receptor or active portion thereof, a transport protein, a regulatory protein, an antigen and an allergen. For example, the encoded polypeptide can be adenosine deaminase, cystic fibrosis transmembrane conductance regulator (CTFR), galsulfase, laronidase, N-acetylgalactosamine 6-sulfatase, phenylalanine ammonia lyase, acid alpha glucosidase, imiglucerase, alglucosidase alpha, thyrotropin, growth hormone, insulin, thyroid hormone, erythropoietin (EPO), interleukin-1 (IL-1), IL-2, IL-3, IL-4, IL-5, IL-7, interferon- α (IFN- α), IFN- β , IFN- γ , tumor necrosis factor (TNF), IL-12, IL-18, Fms-Related Tyrosine Kinase 3 (flt3), neuropilin-2 (NP2), bone morphogenic protein (BMPs), epidermal growth factor (EGF), erythropoietin (EPO), fibroblast growth factor (FGF), granulocyte colony stimulating factor (G-CSF), granulocyte macrophage colony stimulating factor (GM-CSF), hepatocyte growth factor (HGF), insulin-like growth factor (IGF), platelet derived growth factor (PDGF), transforming growth factor α or β , vascular endothelial growth factor (VEGF), epidermal growth factor receptor (EGFR), fibroblast growth factor receptor (FGFR), FGFR antagonist (sFGFR) transforming growth factor receptor (TGFR), vascular endothelial growth factor receptor (VEGFR), plasminogen activator, urokinase, Factor VIII, Factor IX, von Willebrand factor, growth hormone, metalloproteinase thrombospondin motifs 1 (METH-1), METH -2, tryptophanyl-tRNA synthetase (TrpRS) fragments, proliferin-related protein, prolactin fragment, pigment epithelium-derived factor (PEDF), vasostatin, angiostatin, endostatin, kininostatin, fibrinogen-E fragment, thrombospondin, tumstatin, canstatin, restin, soluble fms-like tyrosine kinase-1 (sFlt-1), soluble vascular endothelial growth factor receptors (sFlk), soluble Neuropilin 1 (sNRP1), Interferon gamma-induced protein 10 (IP-10), Platelet factor 4 (PF-4), Gro-beta, soluble Ephrin type-B receptor 4 (sEphB4), sephrinB2, IGF-1, herpes simplex virus thymidine kinase (HSV-TK), carboxypeptidase G2 (CPG2), carboxylesterase (CA), cytosine deaminase (CD), cytochrome P450 (cyt-450), deoxycytidine kinase (dCK), nitroreductase (NR), purine nucleoside phosphorylase (PNP), thymidine phosphorylase (TP), varicella zoster virus thymidine kinase (VZV-TK), xan-

thine-guanine phosphoribosyl transferase (XGPRT), Aspartylglucosaminidase, α -Galactosidase A, Palmitoyl Protein Thioesterase, Tripeptidyl Peptidase, Lysosomal transmembrane protein, cysteine transporter, Acid ceramidase, acid α -L-fucosidase, protective protein/cathepsin A, acid β -glucosidase or glucocerebrosidase, acid β -galactosidase, iduronate-2-sulfatase, α -L-Iduronidase, galactocerebrosidase, acid α -mannosidase, acid β -mannosidase, arylsulfatase B, arylsulfatase A, N-Acetylgalactosamine-6-sulfate sulfatase, N-Acetylglucosamine-1-phosphotransferase, Acid sphingomyelinase, Niemann-Pick disease, type C1 (NPC-1), β -Hexosaminidase B, Heparan N-sulfatase, α -N-Acetylglucosaminidase (NaGlu), Acetyl-CoA: α glucosaminidase N-acetyltransferase, N-Acetylglucosamine-6-sulfate sulfatase, β -Glucuronidase, acid lipase, neprilysin, the insulin-degrading enzyme insulysin, thimet oligopeptidase, calbindin D28, parvalbumin, hypoxia induced factor 1-alpha (HIF1-alpha), sirtuin-2 (SIRT-2), survival motor neuron protein-1 (SMN-1), SMN-2, glial cell-derived neurotrophic factor (GDNF), ciliary neurotrophic factor (CNTF), low density lipoprotein receptor (LDLR), lipoprotein lipase (LPL), Alpha-1-Antitrypsin (AAT), UDP-glucuronyltransferase (UGT), UGT1A1, glucose-6 phosphatase, phosphoenolpyruvate-carboxykinase, galactose-1 phosphate uridyl transferase, phenylalanine hydroxylase, branched chain alpha-ketoacid dehydrogenase, fumarlylacetate hydrolase, methylmalonyl-CoA mutase, ornithine transcarbamylase, argininosuccinic acid synthetase, adenosine deaminase, hyposanthine guanine phosphoribosyl transferase, biotinidase, betagluco-cerebrosidase, beta-glucuronidase, porphobilinogen deaminase (PBDG) or p53.

[0033] In any of the methods described herein, the nucleic acid molecule can be a therapeutic nucleic acid molecule that encodes a therapeutic product, whereby delivery of the nucleic acid molecule effects treatment of a disease or condition. The disease or condition can be an arthritis, chronic pain, HIV-related AIDS, atherosclerosis, restenosis, inherited enzyme deficiency, inherited immune deficiency, cancer, a retrovirus infection, hemophilia, diabetes, a muscular dystrophy, a cardiovascular disorder, cystic fibrosis, a neurodegenerative disorder, trauma, pain, sickle cell anemia, autoimmune disease, inflammatory disease, and hypertension. In particular examples, the nucleic acid encoded polypeptide can be a Factor VIII for the treatment of hemophilia A; a Factor IX for the treatment of hemophilia B; an insulin gene for treatment of type I diabetes mellitus; an alpha-1-antitrypsin (AAT) for the treatment of alpha-1-antitrypsin (AAT) deficiency; a hemochromatosis protein (HFE) for treatment of hemochromatosis; a copper-transporting ATPase 2 for treatment of Wilson's disease; UDP glucuronosyltransferase 1A1 (UGT1A1) for the treatment of Crigler-Najjar syndrome type I; ornithine transcarbamylase (OTC) for the treatment of ornithine transcarbamylase deficiency, type II; low density lipoprotein receptor (LDLR) for the treatment of familial hypercholesterolem-

ia; fibrinogen alpha (FGA), beta (FGB) or gamma (FGB) for the treatment of afibrinogenemia; glucose-6-phosphate- α for the treatment of glycogen storage disease (GSD) type Ia; G6PT for the treatment of GSD type Ib; acid- α -glucosidase for the treatment of GSD type II (Pompe); α -L-iduronidase for the treatment of mucopolysaccharidosis (MPSI); sulphamidase for the treatment of MPS IIIA; α -N-acetylglucosaminidase (NaGlu) for the treatment of MPS IIIB; β -glucuronidase for the treatment of MPS VII; α -galactosidase A for the treatment of Fabry disease; glucocerebrosidase for the treatment of Gaucher's disease; acid sphingomyelinase for the treatment of Niemann-Pick syndrome; phenylalanine hydroxylase for the treatment of phenylketonuria; TIMP antagonist or anti-HSC molecules for the treatment of liver fibrosis; anti-ROS molecules for the treatment of liver ischemia reperfusion injury; amyloid-beta degrading enzyme neprilysin, the insulin-degrading enzyme insulysin, or thimet oligopeptidase for the treatment of Alzheimer's disease; insulin growth factor-1 (IGF-1), calbindin D28, parvalbumin, HIF1-alpha, SIRT-2, VEGF, SMN-1, SMN-2, GDNF or ciliary neurotrophic factor (CNTF) for the treatment of Amyotrophic Lateral Sclerosis (ALS); galactose-1 phosphate uridyl transferase for the treatment of galactosemia; branched chain alpha-ketoacid dehydrogenase for the treatment of maple syrup urine disease; fumarlylacetate hydrolase for the treatment of tyrosinemia type 1; methylmalonyl-CoA mutase for the treatment of methylmalonic acidemia; argininosuccinic acid synthetase for the treatment of citrullinemia; hyposanthine guanine phosphoribosyl transferase for the treatment of Gout and Lesch Nyan syndrome; beta-glucuronidase for the treatment of Sly syndrome; peroxisome membrane protein 70 kDa for the treatment of Zellweger syndrome, enfuvirtide for the treatment of Human immunodeficiency virus (HIV) infection; adenosine deaminase (ADA) for the treatment of combined immunodeficiency disease (SCID); CFTR for the treatment of cystic fibrosis; porphobilinogen deaminase (PBDG) for the treatment of acute intermittent porphyria; interferon-beta for the treatment of multiple sclerosis; lipoprotein lipase for the treatment of lipoprotein lipase deficiency (LPLD), p53 for the treatment of cancer; and glutamic acid decarboxylase (GAD) for the treatment of Parkinson's Disease.

[0034] For example, the nucleic acids molecules can encode a protein for treatment of a cancer. For example, the cancer can be a solid tumor, including, but not limited to, breast cancer, melanoma, head and neck cancer, colon cancer, renal carcinoma and sarcoma. Such cancers can be treated with any molecule that inhibits angiogenesis. Hence, a nucleic acid molecule can encode a protein that inhibits angiogenesis, including, but not limited to, endostatin, angiostatin, vasculostatin, thrombospondin-1, tissue inhibitor of metalloprotease (TIMP), soluble vascular endothelial growth factor (VEGF) receptor and vasostatin (calreticulin fragment). Such anti-angiogenic agents also can be used in the treatment of other angiogenic diseases or conditions, such as ocular diseases.

[0035] In any of the methods described herein, the nucleic acid molecule can encode a polypeptide that increases muscle production in an animal, increases hair production in an animal, increases wool production in an animal, increases growth of an animal, or is involved in nutrient synthesis or utilization. For example, the encoded polypeptide can be: a polypeptide that increases muscle production in an animal that is a myostatin inhibitor; a polypeptide that increases growth in an animal that is a growth hormone, IGF-1, a growth hormone releasing factor or chicken Ski; or a polypeptide that is involved in nutrient synthesis or utilization that is a serine transacetylase and o-acetylserine sulphhydrylase. In particular examples, the myostatin inhibitor is follistatin.

[0036] In any of the methods described herein, the nucleic acid molecule can be a DNA molecule, a RNA molecule, or an aptamer. For example, the nucleic acid molecule can be a microRNA, a small interfering RNA, a ribozyme or an antisense nucleic acid. The nucleic acid can be delivered in a vehicle, which can be lipid vesicle, a virus or a microorganism. For example, the lipid vesicle can be a liposome or micelle. In other examples, the vehicle is a virus, and the virus can be an adenovirus, an adeno-associated virus (AAV), a retrovirus, a vaccinia virus or a herpes simplex virus. The retrovirus can be a lentivirus. In particular examples, the virus is an adenovirus, and the adenovirus can include a deletion in an E1, E2a, E2b, E3, or E4 coding region and have a serotype of adenovirus type 2 or adenovirus type 5. In some of the examples of methods provided herein, the amount of virus administered can be from or from about 10 to 1 x 10¹² particles, 10 to 1 x 10⁶ particles, 1 x 10³ to 1 x 10¹² particles, 1 x 10⁶ to 1 x 10¹⁰ particles, or 1 x 10⁷ to 1 x 10⁹ particles; or is or is from or from about 10 to 1 x 10¹² pfu, 10 to 1 x 10⁶ pfu, 1 x 10³ to 1 x 10¹² pfu, 1 x 10⁶ to 1 x 10¹⁰ pfu, or 1 x 10⁷ to 1 x 10⁹ pfu; or less than 1 x 10¹² particles, 1 x 10¹¹ particles, 1 x 10¹⁰ particles, 1 x 10⁹ particles, 1 x 10⁸ particles, 1 x 10⁷ particles, 1 x 10⁶ particles, 1 x 10⁵ particles, 1 x 10⁴ particles, 1 x 10³ particles or less; or is less than 1 x 10¹² pfu, 1 x 10¹¹ pfu, 1 x 10¹⁰ pfu, 1 x 10⁹ pfu, 1 x 10⁸ pfu, 1 x 10⁷ pfu, 1 x 10⁶ pfu, 1 x 10⁵ pfu, 1 x 10⁴ pfu, 1 x 10³ pfu or less.

[0037] In any of the methods described herein, the subject can be a mouse, rat, cow, pig, sheep, goat, horse and human. For example, subject can be a human child under the age of 18 or is a human fetus.

[0038] In any of the methods described herein includes removing the device from the port, in which prior to removing the device from the port, the positioner is moved forward towards the distal end to engage with the first stop to move the sheath to enclose the injection needle inside the lumen of the sheath.

BRIEF DESCRIPTION OF THE DRAWINGS

[0039] The drawings described herein are for illustrative purposes only of selected embodiments and not all possible implementations, and are not intended to limit

the scope of the present disclosure.

FIGS. 1A and 1B illustrate a standard syringe injection device. **FIG. 1A** shows a perspective view of an exemplary embodiment of an injection device containing a standard syringe at the proximal end of the device. **FIG. 1B** illustrates connection of the syringe barrel to the needle sheath controller.

FIG. 2 shows a perspective view of an exemplary embodiment of an integrated syringe injection device in which a syringe barrel is integrated into the needle sheath lumen at the distal end of the device.

FIG. 3 shows a perspective view of an exemplary embodiment of a dockable syringe injection device in which a syringe containing an auxiliary plunger, barrel and injection needle are adapted to be docked onto a syringe adaptor within the needle sheath lumen at the distal end of the device

FIGS. 4A-C illustrate the movement of the needle sheath of the injection device between the sheathed and unsheathed position as controlled by the positioner. **FIG. 4A** is a birds-eye view showing the positioner positioned towards the distal end so that the needle sheath is in the sheathed position. **FIG. 4B** is a birds-eye view showing the positioner in an intermediate or middle position with the needle sheath in the transitioning position moving between the sheathed and unsheathed position. **FIG. 4C** is a birds-eye view showing the positioner position towards the proximal end so that the needle sheath is in the unsheathed position.

FIG. 5 is an enlarged sectional view of the needle sheath controller of the device depicted in FIG. 1A and 1B.

FIG. 6 is an enlarged sectional view of the needle sheath controller of the device depicted in FIG. 2.

FIG. 7 is an enlarged sectional view of the needle sheath controller of the device depicted in FIG. 3.

FIGS. 8A-8B show an enlarged sectional view of the tip of the needle sheath in the device shown in FIG. 1A and 1B. **FIG. 8A** shows the needle sheath in the sheathed position. **FIG. 8B** shows the needle sheath in the unsheathed position.

FIGS. 9A-9D show enlarged perspective views of the needle sheath in the device shown in FIG. 1A and 1B. **FIG. 9A** illustrates the needle sheath in the sheathed position in a windowless needle sheath shaft. **FIG. 9B** illustrates the needle sheath in the unsheathed position in a windowless needle sheath shaft. **FIG. 9C** illustrates the needle sheath in the sheathed position in a needle shaft with a visibility window. **FIG. 9D** illustrates the needle sheath in the unsheathed position in a needle shaft with a visibility window.

FIGS. 10A-10D illustrate enlarged views of the device shown in FIG. 2. **FIG. 10A** is a sectional view of the needle sheath in the sheathed position. **FIG. 10B** is a sectional view of the needle sheath in the

unsheathed position. **FIG. 10C** is a perspective view of the needle sheath in the sheathed position. **FIG. 10D** is a perspective view of the needle sheath in the unsheathed position.

FIGS. 11A-11D illustrate enlarged views of the device shown in FIG. 3. **FIG. 11A** is a perspective view of the distal end of the device illustrating the syringe adaptor cavity and the syringe adaptor with the dockable syringe in the undocked position. **FIG. 11B** is a perspective view of the distal end of the device, with the dockable syringe docked onto the syringe adaptor and the needle sheath in the sheathed position. **FIG. 11C** is a perspective view of the distal end of the device, with the dockable syringe docked onto the syringe adaptor and the needle sheath in the unsheathed position. **FIG. 11D** is a perspective view of the distal end of the device, with the dockable syringe docked onto the syringe adaptor, the needle sheath in the unsheathed position and the dockable syringe plunger in the depressed position.

[0040] Corresponding reference numerals indicate corresponding parts throughout the several views of the drawings. For parts which are similar but not the same as parts originally specified with a given number, a prime (') of the original numbers is used. A lowercase reference numeral (e.g. a, b, etc.) refers to the same part but in different positions or states.

DETAILED DESCRIPTION

[0041]

A. Definitions

B. Injection Device

1. Standard Injection Device
2. Integrated Injection Device
3. Dockable Injection Device

C. Applications and Uses

1. Treating Diseases and Disorders

D. Examples

A. DEFINITIONS

[0042] Unless defined otherwise, all technical and scientific terms used herein have the same meaning as is commonly understood by one of skill in the art to which the invention(s) belong. In the event that there are a plurality of definitions for terms herein, those in this section prevail. Where reference is made to a URL or other such identifier or address, it is understood that such identifiers can change and particular information on the internet can come and go, but equivalent information can be found by searching the internet. Reference thereto evidences

the availability and public dissemination of such information.

[0043] As used herein, reference to a "minimally invasive surgery" or a "minimally invasive procedure," also sometimes referred to as endoscopy, refers to any procedure (surgical or otherwise) that is less invasive than open surgery used for the same purpose. A minimally invasive procedure is carried out through the skin or through a body cavity or anatomical opening. The procedure typically involves use of devices suitable for the procedure, such as arthroscopic devices (for joints and the spine) or laparoscopic devices (for surgeries of abdomen). Minimally invasive procedures can be carried out with indirect observation of the surgical field through an endoscope or large scale display panel, and can involve manual or remote-control manipulation of instruments. Exemplary of a minimally invasive procedure is laparoscopy. Other minimally invasive procedures include, but are not limited to, refractive surgery, percutaneous surgery, arthroscopic surgery, cryosurgery, microsurgery, keyhole surgery, thoracoscopic surgery, endovascular surgery (such as angioplasty), coronary catheterization, stereotactic surgery, image-guided surgery, and ultrasound guided percutaneous ethanol treatment.

[0044] As used herein, "laparoscopy" or "laparoscopic surgery" refers to a minimally invasive surgical procedure in which operations in the abdomen are performed through small incisions. The incisions are typically 5 millimeters (mm) to 20 mm in length. One or several incisions are made, and laparoscopic ports, typically 5 mm to 12 mm in diameter, are inserted into the incisions. Laparoscopic surgical instruments are inserted or withdrawn through the laparoscopic ports.

[0045] As used herein, endoscope refers to an instrument that can be introduced into the body to give a view of its internal parts. A "laparoscope" refers to an instrument that can be introduced into the abdomen to give a view of its internal parts.

[0046] As used herein, "endoscopic port" refers to a medical appliance inserted into an incision for a minimally invasive procedure that provides a pathway that allows a minimally invasive device to pass through the skin or body cavity. With reference to laparoscopy, a "laparoscopic port" is a medical appliance inserted into an incision for a laparoscopic procedure that provides a pathway that allows a laparoscopic device to pass through the skin into the abdominal cavity.

[0047] As used herein, a device for minimally invasive procedures is a device that is sufficiently long and narrow to permit access to a tissue or an organ during minimally invasive procedures.

[0048] As used herein, a laparoscopic device is a device that is sufficiently long and narrow to permit access to a tissue or an organ during minimally invasive procedures.

[0049] As used herein, injection device refers to a device that can be used to deliver fluids into the body or its cavities, such as a tissue or an organ or a portion

thereof. The device generally contains a hollow barrel or syringe fitted with a plunger and a hollow needle for penetrating the target. For purposes herein, an injection device is one that can be used for minimally invasive procedures, such as laparoscopic surgeries or procedures.

[0050] As used herein, direct injection refers to injections given straight into the target, for example, straight into the tissue or organ or portion thereof.

[0051] As used herein, an organ or a tissue refers to differentiated parts of the body of a subject that performs a specific function. Tissues generally are a group of specialized cells that group together to form a specialized function. For example, muscle tissue is a specialized tissue that can contract. Organs are made up of tissues that perform a function. Examples of organs, include but are not limited to, the eyes, ears, lungs, liver, kidney, heart, or skin.

[0052] As used herein, reference to a "portion of a tissue or an organ" refers to part of a tissue or an organ of the body of a subject. The part can be a region, segment, lobe, section or other part of a tissue or an organ. The portion is one that can be mobilized or isolated separate from the rest of the tissue or organ. It also is a portion that is sufficient to effect delivery of the agent. It is within the skill of one in the art to determine the appropriate size of a portion of a tissue or an organ sufficient to effect delivery of the agent, and it depends upon the particular organ, the indication treated, the dosage, the size of the subject and other parameters. Typically, a portion of a tissue or an organ has a volume of at least about 5 mm³, 10 mm³ or more. For example, the portion can be any area of a tissue or an organ that has a length ranging from 0.5 cm to 25 cm, a height (or thickness) of 0.5 cm to 20 cm and/or a depth from 0.5 cm to 15 cm. As an example, a portion of a liver lobe or segment is one that has a length of 5 cm to 10 cm, a height of 1 cm to 3 cm and a depth (from the tip) of 1.5 cm to 3 cm. Smaller regions or portions are also contemplated so long as the portion is of a sufficient size to deliver a therapeutic or other agent.

[0053] As used herein, parenchyma refers to the portions of the tissue and associated cells of an organ that conducts the specific function of the organ and that makes up the bulk of the organ. Hence, the parenchyma is the main underlying functional tissue of an organ. These can include the epithelial tissue, muscle tissue, nervous tissue and associated cells thereof. Parenchyma is distinct from the stroma, which is the connective tissue, blood vessels, nerves and ducts. Hence, parenchyma does not include connective tissue, blood vessels, nerves and ducts. For example, the parenchyma of the liver includes hepatocytes, the parenchyma of the heart includes cardiac muscle cells such as myocytes, the parenchyma of the kidney includes nephrons. The parenchyma of the skin is the epidermis.

[0054] As used herein, "parenchymal cells" refers to the cells that are contained in or that make up the parenchyma of a tissue or an organ. For example, hepatocytes

are cells of the main tissue of the liver, which make up 70-80% of the liver's mass. In the lung, 75% of all lung cells are contained in the parenchyma. These include, for example, fibroblasts of the interstitium and epithelial cells that line that alveoli, such as type 1 and type 2 cells (pneumocytes) and brush cells. In the skin, cells found in the parenchyma include epidermal cells such as keratinocytes. One of skill in the art is familiar with the parenchyma of various tissue and organs and cells therein.

[0055] As used herein, parenchymal injection refers to administration to the parenchyma of a tissue or an organ.

[0056] As used herein, "proximal" with reference to a component of the device or the device refers to the end of the component or the device that is closest to the medical professional operating the device during use of the device. It is understood that the proximal portion need not be the end of the component, but includes the entire portion of the component that is closest to the medical professional operating the device during use of the device.

[0057] As used herein, "distal" with reference to a component of the device or the device refers to the end of the device furthest from the medical professional during use of the device.

[0058] As used herein, "operably" or "operatively" when referring to two components means that the segments are arranged so that they function in concert for their intended purposes, e.g., movement of one component by another component.

[0059] As used herein, "engaged" refers to the condition in which two members that are designed to be contacted or connected are physically contacted to connected to each other in a manner in which they are designed to be contacted or connected. For example, an adaptor and a hub, such as Luer connectors, can be engaged when they are physically connected to each other in a manner in which they are designed to be connected. A groove (e.g. in sheath stops) and a notch that fits in the groove (e.g. in positioner), can be engaged when they are physically contacted to each other in a manner in which they are designed to be contacted.

[0060] As used herein, "male" with reference to a thread (e.g. of a Luer connector) refers to a member that includes a thread on its outer surface.

[0061] As used herein, "female" with reference to a thread (e.g. of a Luer connector) refers to a connecting member that includes a thread on its inner surface.

[0062] As used herein, elongate with reference to the sheath means that the sheath is long in relation to width or diameter. The elongate structure permits use of the device through ports to access the body cavity in minimally invasive procedures, such as laparoscopic procedures or surgeries.

[0063] As used herein, extended with reference to the plunger means that the proximal end of the plunger is not in proximity to the syringe barrel, such that the plunger is expanded or increased in length to cover a larger area so that it is able to operably connect with the syringe

barrel.

[0064] As used herein, "substantially the same" with reference to the length of the exposed needle compared to the distance between sheath stops means that the length and distance are for the most part the same or essentially the same, but can differ slightly in a manner that is not significant. For example, the length of the exposed needle and the distance between sheath stops is substantially the same if the length of the exposed needle is longer or shorter than the distance between the sheath stops by no more than 1 mm, and generally less than 1 mm, 0.8 mm, 0.6 mm, 0.5 mm, 0.4 mm or less.

[0065] As used herein, sheath stop with reference to the needle sheath controller refers to an opening or groove formed in the controller to cease or halt or prevent the movement of the sheath. The engagement of the sheath with the stops need not be direct, but can be indirect. For example, the sheath can be operably coupled to a component that itself engages with stop. In examples of the device herein, the sheath is connected to a connection member that is connected to a positioner that engages directly with the stop to cease, halt or prevent the movement of the sheath. Hence, the stops lock the sheath from moving. The stops can be positioned at different distances from each other so that the sheath can be movably locked into more than one position (e.g. the sheathed and unsheathed position).

[0066] As used herein, "sheathed" or "the sheathed position" with reference to the injection needle means that the sheath is enclosed over the needle so that the sheath is not extended or exposed outside of the blunt end of the sheath.

[0067] As used herein, "unsheathed" or "the unsheathed position" with reference to the injection needle means that the distal tip of the needle extended or exposed outside of the sheath, and the sheath does not enclose the distal tip of the needle. The extent by which the distal tip of the needle is unsheathed is dependent on the particular device (e.g. sheath stops).

[0068] As used herein, axial force with reference to the plunger refers to force that directly acts on the center axis of an object. The axial force used herein is applied along the longitudinal axis. For example, axial force must be applied to depress or pull back the plunger. Axial force is typically compression force, e.g. depression of a plunger, or a stretching force, e.g. pulling back of a plunger.

[0069] As used herein, lumen refers to the inside space of a tubular structure. The tubular structure can have a regular tubular or cylindrical shape, or irregular tubular or cylindrical shape.

[0070] As used herein, cavity refers to an empty or hollow space or an opening leading to an empty space within an object.

[0071] As used herein, recess refers to an empty or hollow space created by part of an object which is constructed further back from the rest. It can be a hollow space created by walls surrounding the space. For example, a recess can be a groove with openings at one

or both ends so that an item can pass through.

[0072] As used herein, predetermined length refers to a length that is set by the configuration of the device. Once the device has been constructed and configured, the predetermined length cannot be changed.

[0073] As used herein, loading a syringe refers to filling the syringe barrel, the fluid reservoir, with fluid. The syringe barrel is typically loaded or filled by pulling the plunger backward/rearward, toward the proximal end of the device.

[0074] As used herein, releasing, dispelling, expelling or ejecting a fluid from the syringe refers to emptying the fluid content of the syringe through the distal end of the syringe by depressing the plunger.

[0075] As used herein, lining refers to a separate layer of different material positioned on the inside surface of an object. For example, if a hollow tubular structure has another hollow tubular structure with a slightly smaller diameter fitted on the inside surface, the inner tubular structure is a lining for the outer tubular structure.

[0076] As used herein, integrated describes a part which is physically enclosed or encased with another part. Integrated parts cannot be separated from the part that encases or encloses the integrated part. With reference to the integrated injection device, the syringe barrel is enclosed or encased by the sheath and cannot be separated from the sheath.

[0077] As used herein, dockable or detachable describes a part which can be attached, docked, snap-fitted or placed into an adaptor of another part. Dockable parts can be attached docked, snap-fitted or placed into an adaptor in a reversible manner. For example, the part can be undocked or removed, i.e. separated from the part. Hence, the part is not physically bonded to the other part which contains the dock or the adaptor. With reference to the dockable syringe injection device, the syringe can be removed or undocked from the sheath. Likewise, with reference to the standard injection device, the syringe barrel can be detached from the device.

[0078] As used herein, dead volume refers to the volume of fluid that is loaded into the syringe barrel but cannot be expelled from the device and remains in the syringe barrel or needle. Factors that influence the amount of dead volume include the length of the needle, the diameter of the needle, and the diameter of the syringe barrel.

[0079] As used herein, injection pressure refers to the pressure required to inject the fluid out of the fluid reservoir into the target. Required injection pressure may differ depending on the properties of the composition of the fluid (e.g. viscosity), the length of the needle and the target site (e.g. hardness).

[0080] As used herein, pressure drop refers to the decrease in pressure as fluid flows through the fluid path, due to factors such as drag and frictional effect. Factors that can influence pressure drop include length of the needle, the diameter of the needle, and the viscosity of the fluid. If significant pressure drop occurs, the axial

force applied to the plunger does not result in sufficient injection pressure at the needle.

[0081] As used herein, a composition refers to any mixture. It can be a solution, a suspension, fluid, powder, a paste, aqueous, non-aqueous or any combination thereof.

[0082] As used herein, fluid refers to any composition that can flow. Fluids thus encompass compositions that are in the form of semi-solids, pastes, solutions, aqueous mixtures, gels, lotions, creams and other such compositions. For purposes herein, a fluid generally is injectable.

[0083] As used herein, a therapeutic refers to an agent, a product, a compound or a composition that is capable of producing a therapeutic effect. The agent, product, compound or composition can comprise small molecule drugs, prodrugs, proteins, peptides, DNA, RNA, viruses, antibodies, organic molecules, saccharides, polysaccharides, lipids and combinations or conjugates thereof. The agent, product, compound or composition can include other pharmaceutically effective agents known in the general art to be of value in treating one or more of the diseases or medical conditions. Exemplary therapeutics are described herein.

[0084] As used herein, therapeutic effect means an effect resulting from treatment of a subject that alters, typically improves or ameliorates the symptoms of a disease or condition or that cures a disease or condition. A therapeutically effective amount refers to the amount of a composition, molecule or compound which results in a therapeutic effect following administration to a subject.

[0085] As used herein, "genetic therapy" or "gene therapy" involves the transfer of a nucleic acid molecule, such as heterologous DNA to certain cells, target cells, of a mammal, particularly a human, with a disorder or condition for which such therapy is sought. The DNA is introduced into the selected target cells in a manner such that the heterologous DNA is expressed and a therapeutic product encoded thereby is produced. Alternatively, the heterologous DNA can in some manner mediate expression of DNA that encodes the therapeutic product, it can encode a product, such as a peptide or RNA that in some manner mediates, directly or indirectly, expression of a therapeutic product. Genetic therapy also can be used to deliver nucleic acid encoding a gene product to replace a defective gene or supplement a gene product produced by the mammal or the cell in which it is introduced. The introduced nucleic acid can encode a therapeutic compound (e.g. a growth factor inhibitor thereof, or a tumor necrosis factor or inhibitor thereof, such as a receptor therefor), that is not normally produced in the mammalian host or that is not produced in therapeutically effective amounts or at a therapeutically useful time. The heterologous DNA encoding the therapeutic product can be modified prior to introduction into the cells of the afflicted host in order to enhance or otherwise alter the product or expression thereof.

[0086] As used herein, nucleic acid molecule refers to single-stranded and/or double-stranded polynucle-

otides, such as deoxyribonucleic acid (DNA) and ribonucleic acid (RNA), as well as analogs or derivatives of either RNA or DNA. Also included in the term "nucleic acid" are analogs of nucleic acids such as peptide nucleic acid (PNA), phosphorothioate DNA, and other such analogs and derivatives. Nucleic acids can encode gene products, such as, for example, polypeptides, regulatory RNAs, microRNAs, small inhibitory RNAs (siRNAs) and functional RNAs. Hence, nucleic acid molecule is meant to include all types and sizes of DNA molecules including siRNA, aptamers, ribozymes, complementary DNA (cDNA), plasmids and DNA including modified nucleotides and nucleotide analogs.

[0087] As used herein, a therapeutic nucleic acid is a nucleic acid molecule that encodes a therapeutic or is capable of producing a therapeutic effect. The product can be nucleic acid, such as a regulatory sequence or gene, or can encode a protein that has a therapeutic activity or effect. For example, therapeutic nucleic acid can be a ribozyme, antisense, double-stranded RNA, a nucleic acid encoding a protein and others.

[0088] As used herein, "vehicle" refers to the agent or conduit, such as vector or construct, that contains a nucleic acid molecule for gene therapy and that facilitates entry of the nucleic acid molecule into cells and/or expression thereof. Hence, the vehicle containing the nucleic acid is the delivered agent that is administered to a subject and that contains the nucleic acid molecule packaged therein or associated therewith. Examples of vehicles include, but are not limited to, a virus, virus-like particles, mini-circles, a plasmid or vector, a liposome and/or nanoparticle. For example, a vehicle can include a lipid-based or other polymer-based composition, such as liposome, micelle or reverse micelle, that is associated with a nucleic acid molecule or other agent, such as a non-viral vector or virus provided herein, for delivery into a host subject. The uptake of vehicles can be further increased or facilitated using various mechanical techniques such as electroporation, sonoporation or "gene gun."

[0089] As used herein, a heterologous nucleic acid (also referred to as exogenous nucleic acid or foreign nucleic acid) with reference to nucleic acid contained in the genome of a virus refers to a nucleic acid that is not normally produced *in vivo* by an organism or virus from which it is expressed or that is produced by an organism or a virus but is at a different locus, or that mediates or encodes mediators that alter expression of endogenous nucleic acid, such as DNA, by affecting transcription, translation, or other regulatable biochemical processes. Hence, heterologous nucleic acid is often not normally endogenous to an organism or a virus into which it is introduced. Heterologous nucleic acid can refer to a nucleic acid molecule from another virus in the same organism or another organism, including the same species or another species. Heterologous nucleic acid, however, can be endogenous, but is nucleic acid that is expressed from a different locus or altered in its expression or se-

quence (e.g., a plasmid). Thus, heterologous nucleic acid includes a nucleic acid molecule not present in the exact orientation or position as the counterpart nucleic acid molecule, such as DNA, is found in a genome. Generally, although not necessarily, such nucleic acid encodes RNA and proteins that are not normally produced by the organism or virus or in the same way in the virus in which it is expressed. Any nucleic acid, such as DNA, that one of skill in the art recognizes or considers as heterologous, exogenous or foreign to the virus in which the nucleic acid is expressed is herein encompassed by heterologous nucleic acid. Examples of heterologous nucleic acid include, but are not limited to, nucleic acid that encodes exogenous peptides/proteins, including diagnostic and/or therapeutic agents. Proteins that are encoded by heterologous nucleic acid can be expressed within the virus, secreted, or expressed on the surface of the virus in which the heterologous nucleic acid has been introduced.

[0090] As used herein, a DNA construct is a single or double stranded, linear or circular DNA molecule that contains segments of DNA combined and juxtaposed in a manner not found in nature. DNA constructs exist as a result of human manipulation, and include clones and other copies of manipulated molecules.

[0091] As used herein, vector (or plasmid) refers to discrete elements that are used to introduce a heterologous nucleic acid into cells for either expression or replication thereof. The vectors typically remain episomal, but can be designed to effect integration of a gene or portion thereof into a chromosome of the genome. Vectors include non-viral vectors, such as non-viral expression vectors. Also contemplated are vectors that are artificial chromosomes, such as yeast artificial chromosomes and mammalian artificial chromosomes. Vectors also include "virus vectors" or "viral vectors." Selection and use of such vehicles are well known to those of skill in the art.

[0092] As used herein, an expression vector includes vectors capable of expressing DNA that is operatively linked with regulatory sequences, such as promoter regions, that are capable of effecting expression of such DNA fragments. Such additional segments can include promoter and terminator sequences, and optionally can include one or more origins of replication, one or more selectable markers, an enhancer, a polyadenylation signal, and the like. Expression vectors are generally derived from plasmid or viral DNA, or can contain elements of both. Thus, an expression vector refers to a recombinant DNA or RNA construct, such as a plasmid, a phage, recombinant virus or other vector that, upon introduction into an appropriate host cell, results in expression of the cloned DNA. Appropriate expression vectors are well known to those of skill in the art and include those that are replicable in eukaryotic cells and/or prokaryotic cells and those that remain episomal or those which integrate into the host cell genome.

[0093] As used herein, "virus," refers to any of a large group of infectious entities that cannot grow or replicate

without a host cell. Viruses typically contain a protein coat surrounding an RNA or DNA core of genetic material, but no semipermeable membrane, and are capable of growth and multiplication only in living cells. Viruses include those that are formed when, such as when a vector containing all or a part of a viral genome, is transduced into an appropriate cell or cell line for the generation of such particles. The resulting viral particles have a variety of uses, including, but not limited to, transferring nucleic acids into cells either *in vitro* or *in vivo*. Thus, a virus is a packaged viral genome. A virus can refer to a single particle, a stock of particles or a viral genome.

[0094] As used herein, viral vector refers to a nucleic acid vector construct that includes at least one element of viral origin and can be packaged into a viral vector particle or virus. Reference to viral vector herein is used interchangeably with virus when it is packaged inside a protein coat. The viral vector particles or virus can be used for the purpose of transferring DNA, RNA or other nucleic acids into cells either *in vitro* or *in vivo*. Viral vectors include, but are not limited to, retroviral vectors, vaccinia vectors, lentiviral vectors, herpes virus vectors (e.g., HSV), baculoviral vectors, cytomegalovirus (CMV) vectors, papillomavirus vectors, simian virus (SV40) vectors, Sindbis vectors, Semliki Forest virus vectors, phage vectors, adenoviral vectors, and adeno-associated viral (AAV) vectors. Suitable viral vectors are described, for example, in U.S. Patent Nos. 6,057,155, 5,543,328 and 5,756,086. Viral vectors typically include engineered viruses that are operatively linked to exogenous genes to transfer (as vehicles or shuttles) the exogenous genes into cells.

[0095] As used herein, "adenovirus vector" and "adenoviral vector" are used interchangeably and are well understood in the art to mean a polynucleotide containing all or a portion of an adenovirus genome. An adenoviral vector, refers to nucleic acid encoding a complete genome or a modified genome or one that can be used to introduce heterologous nucleic acid when transferred into a cell, particularly when packaged as a particle. An adenoviral vector can be in any of several forms, including, but not limited to, naked DNA, DNA encapsulated in an adenovirus capsid, DNA packaged in another viral or viral-like form (such as herpes simplex, and AAV), DNA encapsulated in liposomes, DNA complexed with polylysine, complexed with synthetic polycationic molecules, conjugated with transferrin, complexed with compounds such as PEG to immunologically "mask" the molecule and/or increase half-life, or conjugated to a non-viral protein.

[0096] As used herein, the term "adenovirus" or "adenoviral particle" is used to include any and all viruses that can be categorized as an adenovirus, including any adenovirus that infects a human or an animal, including all groups, subgroups, and serotypes. Depending upon the context reference to "adenovirus" can include adenoviral vectors. There are at least 51 serotypes of adenovirus that are classified into several subgroups. For example,

subgroup A includes adenovirus serotypes 12, 18, and 31. Subgroup B includes adenovirus serotypes 3, 7, 11a, 11p, 14, 16, 21, 34, 35 and 50. Subgroup C includes adenovirus serotypes 1, 2, 5, and 6. Subgroup D includes adenovirus serotypes 8, 9, 10, 13, 15, 17, 19, 19p, 20, 22-30, 32, 33, 36-39, 42-49 and 51. Subgroup E includes adenovirus serotype 4. Subgroup F includes adenovirus serotypes 40 and 41. Thus, as used herein an adenovirus or adenovirus particle is a packaged vector or genome. For purposes herein, the viruses typically are recombinant adenoviruses containing a heterologous nucleic acid molecule in its genome and formed when an adenovirus vector is encapsulated in an adenovirus capsid.

[0097] Included among adenoviruses are any and all viruses that can be categorized as an adenovirus, including any adenovirus that infects a human or an animal, including all groups, subgroups, and serotypes. Thus, as used herein, "adenovirus" and "adenovirus particle" refer to the virus itself and derivatives thereof and cover all serotypes and subgroups and naturally occurring and recombinant forms, except where indicated otherwise. Included are adenoviruses that infect human cells. Adenoviruses can be wildtype or can be modified in various ways known in the art or as disclosed herein. Such modifications include, but are not limited to, modifications to the adenovirus genome that is packaged in the particle in order to make an infectious virus. Exemplary modifications include deletions known in the art, such as deletions in one or more of the E1a, E1b, E2a, E2b, E3, or E4 coding regions. Other exemplary modifications include deletions of all of the coding regions of the adenoviral genome. Such adenoviruses are known as "gutless" adenoviruses. The terms also include replication conditional adenoviruses, which are viruses that preferentially replicate in certain types of cells or tissues but to a lesser degree or not at all in other types.

[0098] As used herein, subject can be a vertebrate, more specifically a mammal (e.g., a human, horse, cat, dog, cow, pig, sheep, goat, mouse, rabbit, rat, and guinea pig), birds, reptiles, amphibians, fish, and any other animal. The term does not denote a particular age or sex. Thus, adult and newborn subjects, whether male or female, are intended to be covered. As used herein, patient or subject may be used interchangeably and can refer to a subject in need of a therapeutic agent. The term patient or subject includes human and veterinary subjects. Both therapeutic, industrial, veterinary and agricultural (e.g., meat production) uses are disclosed herein.

[0099] As used herein, a patient refers to a human subject.

[0100] As used herein, a combination refers to any association between or among two or more items. The combination can be two or more separate items, such as two compositions or two collections, can be a mixture thereof, such as a single mixture of the two or more items, or any variation thereof. The elements of a combination are generally functionally associated or related.

[0101] As used herein, the singular forms "a," "an" and

"the" include plural referents unless the context clearly dictates otherwise.

[0102] As used herein, the term "or" is used to mean "and/or" unless explicitly indicated to refer to alternatives only or the alternatives are mutually exclusive.

[0103] As used herein, ranges and amounts can be expressed as "about" a particular value or range. About also includes the exact amount. Hence "about 5 grams" means "about 5 grams" and also "5 grams." It also is understood that ranges expressed herein include whole numbers within the ranges and fractions thereof. For example, a range of between 5 grams and 20 grams includes whole number values such as 5, 6, 7, 8, 9, 10, 11, 12, 13, 14, 15, 16, 17, 18, 19 and 20 grams, and fractions within the range including, but not limited to, 5.25, 6.72, 8.5 and 11.95 grams.

[0104] As used herein, "optional" or "optionally" means that the subsequently described event or circumstance does or does not occur and that the description includes instances where said event or circumstance occurs and instances where it does not.

B. INJECTION DEVICE

[0105] Provided herein are injection devices in accordance with the present claims that can be used in minimally invasive procedures, such as laparoscopic procedures, for use in delivering fluids, such as therapeutics, by direct injection into a target locus, such as by direct injection into a target tissue. The device has an elongated needle sheath with a small diameter, and can be inserted through an endoscopic port, such as a laparoscopic ports, trocars or cannulas, to reach the internal target site. The device provided herein can deliver small and accurate doses of the fluid directly into the target tissue, without the need of large standard syringes and open surgery. The device can optionally deliver multiple doses to the same or different target sites.

[0106] The device can be used in any method that requires direct injection of an agent into a target site, in which access to the target site is limited, such as in minimally invasive procedures. For example, in addition to laparoscopic surgeries, the device provided herein can also be used for direct injection of a fluid, such as a therapeutic, during other minimally invasive medical or surgical procedures, such as thoracoscopic surgery. As described elsewhere herein, any fluid, such as a therapeutic, can be administered, including but not limited to, protein, nucleic acid, small molecule, virus, antibodies or other fluids. The device can be used in conjunction with other minimally invasive surgical devices using single-port or multiport endoscopic (e.g. laparoscopic) surgery. The device can also be used to deliver multiple discrete doses to the same or different sites of injection without removing or after removing the device from the laparoscopic port.

[0107] As described further below, in all embodiments of the device, the device contains a movable sheath en-

closing a fixed needle. The sheath contains an opening to expose the needle, whereby movement of the sheath is controlled by stops in a controller that can be adjusted by a positioner that moves between stops in the controller. The stops are positioned a predetermined distance so that movement of the positioner forward towards the distal end engages the first stop and moves the sheath to enclose the injection needle inside the lumen of the sheath, and movement of the positioner rearward towards the proximal end engages the second stop to move the sheath to expose no more than a predetermined length of the distal tip of the injection needle. Hence, the sheath moves around the fixed needle and is able to retract from its enclosed position to expose a desired length of needle for penetration of a tissue or organ. The particular length of the needle that is exposed is a function of the predetermined distance between the stops in the controller. The stops also can be locked to prevent movement of the needle once it is placed.

[0108] The ability to control movement of the sheath to fully enclose the needle or to expose the needle only a desired length, are features of the injection device that permit its use for direct administration to a parenchymal tissue or other desired locus. For example, the ability to enclose the needle by the sheath prevents unwanted exposure of the needle where its penetration into target tissues is not desired, which can occur when the device is being positioned for direct injection or when it is being removed from a subject. Also, the ability to control the extent or length of needle that is exposed ensures that the needle is no longer than the thickness of the tissue or organ so that the needle cannot puncture through the tissue or organ when it is injected.

[0109] Further, because the needle is fixed and does not move relative to the needle sheath controller, the positioner only controls the movement of the needle sheath, while the injection needle and other components of the device are stationary regardless of the position of the positioner. Thus, control of the movable sheath, and hence needle retraction or extension, is independent from movement of the plunger. This ensures precise injection into the tissue by the plunger without disturbing the placement of the needle in the tissue. In addition, because the needle is fixed and independent of the plunger, movement of the plunger only controls the drawing up and dispelling of fluids. This means that the plunger can be pulled back at the site of injection to draw up fluids to test needle placement (e.g. to confirm injection is not into a blood vessel), without disturbing placement of the needle. As described herein, embodiments of the injection device also can contain a visibility window (e.g. a transparent syringe barrel or needle coupler) to visualize the fluid that is drawn up by the plunger.

[0110] The injection devices provided herein include devices that are configured to minimize dead volume and/or avoid problems in pressure drops, which are problems with injection devices for minimally invasive, such as laparoscopic, surgeries. Thus, the injection devices

generally avoid loss of the fluid, such as a therapeutic, that is being injected by the device. Also, because the injection devices provided herein are configured so that any problems with pressure drop are minimized, the injection devices provided herein also do not require undue axial force to depress the plunger to compensate for pressure drops. Therefore, the devices are safe to use and efficient to use.

[0111] The device, including exemplary embodiments of the device, will be described with reference to the accompanying drawings. As indicated, the use of a prime (') designation with a number indicates that the element shown or described is the same as the non-prime element, except as shown or described differently.

[0112] The device generally has two ends, the needle tip end and the plunger end. For clarity of description, it should be noted that the exemplary devices are depicted with the needle tip end generally towards the right side in the drawings, and the plunger end generally towards the left side of the drawing. The needle tip end will be generally described as the "distal end," and the plunger end will be generally described as the "proximal end." The term "distal end" is intended to refer to the end of the injection device furthest from the person holding the device, and the term "proximal end" is intended to refer to the end of the device closest to the holder of the device. If a component is described to be more "proximal" to another component, the component is closer to the proximal (plunger) end. If a component is described to be more "distal" to another component, the component is closer to the distal (needle tip) end.

[0113] Some components of the injection device can move in two general directions along the longitudinal axis relative to other components. For example, components can generally move towards the proximal end or distal end, or move in the proximal direction or the distal direction. Components that move towards the distal direction (needle tip) are described as moving forward, and components that move toward the proximal direction (plunger) are described as moving rearward/backward. The exemplary devices are also generally depicted with needle sheath controller positioned so that the positioner is pointing upward, with the exception of **FIGS. 4A-4C**, which are birds-eye views looking down on the device. Some of the components, such as the positioner, can move parallel to the vertical axis. The components can move in the upward direction or the downward direction. Pressing of the positioner toward the needle sheath controller will be described as pressing "downward" and releasing the positioner will be described as the positioner moving "upward."

[0114] In a general embodiment, the injection device, or apparatus, provided herein, includes a needle sheath and needle sheath controller, an injection needle with a needle tip that can be sheathed and unsheathed, a syringe barrel used as a reservoir for the fluid, such as a therapeutic, that is being delivered to the target tissue and a plunger that controls loading and release of the

fluid. The needle sheath generally is a rigid shaft, but a flexible or steerable shaft can also be used depending on the purpose of use.

[0115] For example, with reference to FIG. 1A and 1B, which illustrate a first exemplary embodiments provided herein, the syringe injection device is indicated generally by the reference numeral 60, and includes the needle sheath 72 and needle sheath controller 71, the injection needle 81, the syringe barrel 91 and the plunger 92. Other embodiments of the syringe device are described in FIG. 2 and FIG. 3, and other Figures as described below. For example, FIG. 2 shows a further embodiment indicated generally by the reference numeral 60', and includes the needle sheath 72', needle sheath controller 71', the injection needle 81, the syringe barrel 91' and the plunger 92'. In this embodiment, the needle sheath 72', needle sheath controller 71', the syringe barrel 91' and the plunger 92' are substantially the same as the embodiment of FIG. 1A and 1B, except that the syringe barrel 91' is located at the distal end of the device and is integrated with the needle sheath 72' and therefore the plunger 92' traverses through the needle sheath controller 71'. FIG. 3 shows a further embodiment indicated generally by the reference numeral 60'', and includes the needle sheath 72'', the needle sheath controller 71'', the injection needle 81, the syringe barrel 91'' and the plunger 92''. In this embodiment, the needle sheath 72'', needle sheath controller 71'', syringe barrel 91'' and plunger 92'' are substantially the same as the embodiment of FIG. 1A and 1B, except that the syringe barrel 91'' is located at the distal end of the device and is adapted so that it is dockable into the needle sheath 72''. Further, the plunger 92'' traverses the needle sheath controller 71'', and is further adapted to associate with an auxiliary plunger 920 located distal to the needle sheath controller 71' where the auxiliary plunger 920 is adapted to move within the syringe barrel 91''.

[0116] In all embodiments of the laparoscopic device provided herein, the dimensions of the laparoscopic device permits its use through typical ports for laparoscopic surgery or other minimally invasive surgical procedures. For example, typical ports for laparoscopic surgery, through which the instruments or devices enter the patient, is about 5 to 10 mm in diameter. The device is used to reach and inject into the target tissue, which is typically an internal tissue or organ of the body, including the parenchyma of an organ. The length of the device is sufficiently long to permit access to the particular desired target tissue through a laparoscopic port, while not being so unwieldy that it is difficult to control. The choice of dimension of the device is dependent on the particular user, the target tissue, the subject being treated, the agent being administered, and other factors within the level of a skilled artisan. Generally, the needle sheath 72, 72' or 72'' of the injection device is of a sufficient length to permit laparoscopic access to the target of interest, and is generally a length of 200 mm to 600 mm, such as 250 to 400 mm, and generally at least or about

at least or 300 mm.

[0117] In all aspects of the device provided herein, the syringe barrel 91, 91' or 91'' is cylindrical in shape with a hollow center that can fit the plunger 92, 92' or 92'' so that the plunger can move back and forth inside the syringe barrel. The syringe can be made out of plastic or glass or other suitable material. Generally, the syringe is made out of glass or plastic, such as polypropylene, polyethylene, or polycarbonate. Other types of biocompatible materials may also be used. The syringe barrel can contain calibrations or markings on the outer surface in order to measure or detect the volume of solution. The calibrations can be marked in any measurement such as in cubic centimeters (cc), milliliters (mL), tenths of a milliliter, hundredths of a milliliter or other measurement. The volume of the syringe barrel can be selected by the operator depending on the particular application, the agent being administered, the type of device that is being used and other similar factors. For example, the volume of the syringe barrel can depend on the desired amount of fluid, such as a therapeutic, to be delivered, which is generally between 200 μ L and 10 mL, more typically 500 μ L to 2.5 mL, such as at least 500 μ L, 1 milliliter (mL), 2 mL, 2.5 mL, 3 mL, 4 mL, 5 mL, 6 mL, 7 mL, 8 mL, 9 mL, 10 mL or more. For example, the syringe barrel can be 0.5 mL to 20 mL (i.e. 0.5 cc to 20 cc), and generally is 0.5 mL to 3 mL (i.e. 0.5 cc to 3 cc), such as at least or about a 1 mL (i.e. 1 cc) syringe. The syringe barrel also can have unit calibrations, such as present on standard insulin syringes (e.g. 100 units correlates to 1 mL). Typically, 200 μ L to 600 μ L of the fluid, such as a therapeutic, is delivered to the target locus, and the volume of syringe barrel is 1 mL.

[0118] The syringe barrel 91, 91' or 91'' is always positioned on the proximal side of the injection needle, but can be positioned on either side of the needle sheath controller and in a manner that is on the proximal or distal side of the needle sheath controller. For example, the syringe barrel can be positioned on the proximal side of the needle sheath controller, or inside the needle sheath 72, 72' or 72''. In particular aspects, with reference to the Figures and description below, FIG. 1A and 1B depict a device 60 where the syringe barrel 91 is proximal to the needle sheath controller 71. In contrast, FIG. 2 depicts a device 60' where the syringe barrel 91' is distal to the needle sheath controller 71' and is integrated with the needle sheath at its distal end. FIG. 3 depicts a device 60'' where the syringe barrel 91'' is distal to the needle sheath controller 71'' and is dockable, and hence removable from, the needle sheath at the distal end.

[0119] In cases where sterile injections are required, the syringe barrel can be loaded with the fluid, such as a therapeutic, in a sterile environment, such as a sterile operating room, or a sterile pre-loaded syringe can be used. For example, a sterile standard or dockable syringe can be connected to the device after loading with the fluid, such as a therapeutic, in a sterile environment. In other cases, the entire device is loaded, manipulated and

operated in a sterile environment.

[0120] The plunger is located at the proximal end of the device and is movable so that it can be pulled and pushed along the inside the syringe barrel. Portions of the plunger travel within the syringe barrel along the longitudinal axis of the device. The plunger is cylindrical to move through the syringe barrel, and is made of a material that permits ease of movement through the syringe barrel. For example, the plunger generally is made of a plastic, such as polypropylene or polyethylene. The plunger also contains a head at the proximal end of the device that can be conveniently grasped by the operator to manipulate the plunger. The plunger head can transmit axial force from the operator in both the distal or proximal directions, leading to depression and drawing back, respectively, of the plunger. The plunger can be drawn back to load the syringe barrel with the fluid, such as a therapeutic, or depressed to inject the fluid, such as a therapeutic, in the target tissue. Pulling back on the plunger draws in the fluid, such as a therapeutic, or air into the syringe barrel. Pushing in the plunger forces air or the fluid or air out of the syringe barrel. The plunger can also be pulled back at the site of injection to test needle placement.

[0121] The length of the plunger is sufficiently long to permit its association with the inside of the syringe barrel directly or indirectly in order to effect dispelling of the fluid, such as a therapeutic, or composition or solution through the distal end of the syringe (and into a needle or tube if connected thereto). For example, in some aspects herein, a control plunger that is accessible to the operator can be adapted to be used with an auxiliary plunger when the syringe barrel is distally located. The length of the plunger can be 5 mm to 500 mm, such as 10 mm to 300 mm, 10 mm to 200 mm or 10 mm to 100 mm. Depending on the positioning of the syringe barrel with reference to the needle sheath controller, in some aspects the plunger also traverses through the needle sheath controller. In particular aspects, with reference to the Figures and description below, **FIG. 1A** and **1B** depict a device **60** where the plunger **92** is a standard plunger that is sized to move only within the syringe barrel **91** located at the proximal end of the device relative to the needle sheath controller. In contrast, **FIG. 2** depicts a device **60'** where the plunger **92'** is elongated to traverse through the needle sheath controller **71'** and hollow lumen of the needle sheath before traveling through the syringe barrel **91'** at the distal end of the device. In another aspect, **FIG. 3** depicts a device **60''** where the plunger **92''** is elongated to traverse through the needle sheath controller **71'** and hollow lumen of the needle sheath, but does not travel through the syringe barrel **92''** at the distal end of the device. Instead, the plunger is adaptable with an auxiliary plunger **920** that is sized to move only with the syringe barrel located at the distal end of the device.

[0122] The plunger **92**, **92'** or **92''** can be manually depressed or pulled back, or an automatic controller can

be used to control the plunger. An automatic or mechanical plunger mechanism can deliver several fixed or variable doses of the fluid, such as a therapeutic, with or without having to remove the injection device from the laparoscopic port. For example, a means of depressing the plunger **92**, **92'** or **92''** can include hydraulic components, such as mechanically or electronically actuated piston and cylinder assemblies operatively connected, via hydraulic fluid lines, to the respective plunger **92**, **92'** or **92''** elements. The device can be used to deliver a single dose of the fluid, such as a therapeutic, or multiple injections to the same patient without withdrawing the device from the laparoscopic port. Multiple doses can be delivered at different injection sites, if the multiple sites are reasonably close to each other that removal from the laparoscopic port is not necessary. The injection of several discrete doses can be achieved using different controls, such as mechanical controls and hydraulic mechanisms. For example, hydraulic components, such as mechanically and/or electronically actuated piston/cylinder assemblies or hydraulic plunger actuators can be used to control the plunger, which permits the use of a stroke or a force multiplier, and also permits a flexible shaft for the plunger mechanism, to transmit axial force. For multiple injections, an indexed injection trigger is used to deliver discrete doses of the fluid, such as a therapeutic, for example 100 microliter (μL), upon each pull of the trigger. The doses for multiple injections can be fixed or variable, and a volume control or a feedback mechanism for dose control for multiple injections can be used. Multiple doses provide an advantage over a single large dose in that they can be manipulated by parameters such as the location of the tissue, geometrical parameters and temporal parameters.

[0123] In all aspects of the devices provided herein, the device contains an injection needle **81** that is located inside the sheath at the proximal end of the needle and can be sheathed and unsheathed at its distal tip. The injection needle typically contains a beveled tip sufficient to penetrate or pierce a tissue or an organ. The injection needle **81** can be directly or indirectly connected to the distal end of the syringe barrel in a manner that permits passage of a fluid or solution in the syringe barrel through the needle to its distal tip. For example, in some aspects, the injection needle **81** can be indirectly connected to the syringe barrel by an intermediary tube **83** that, together with the injection needle, form a continuous sealed fluid pathway for solution to move through. The intermediary tube can be a plastic or metal tube that is coupled directly or indirectly to the injection needle **81** by welding, bonding or molding. The intermediary injection tube **83** can be indirectly coupled to the injection tube **81** by a needle coupler **85**. The needle coupler **85** can be made of any biocompatible and drug compatible rigid material, including metals, plastics, and ceramics, and is typically made of plastics such as polycarbonate or Acrylonitrile butadiene styrene (ABS). An optional coupling member **82** can be present inside the cavity of the needle coupler **85**. The

needle coupler **85** is coupled to each of the intermediary injection tube **83** and injection tube **81** by welding, bonding, molding or other procedure that creates a secure and reliable seal.

[0124] In some variations, the distal end of the syringe barrel can contain an adaptor that is compatible with a needle hub on the proximal end of the injection needle **81** or other intermediary tube **83** that itself is coupled to the injection needle **81**. For example, with reference to **FIG. 1A**, and as described further below, the distal end of the syringe barrel **91** can contain a Luer fit adaptor **93** that is compatible with a needle hub **84** on the proximal end of intermediary injection tube **83**, which itself is directly or indirectly connected to the injection needle **81**. In other variations of the devices herein, the proximal portion of the injection needle **81** or other intermediary tube **83** that couples to the injection needle is directly affixed to the distal end of the syringe barrel and extends out of the syringe barrel. For example, with reference to **FIGS. 2** and **3**, the injection needle **81** is directly connected to the syringe barrel.

[0125] The size and diameter of the injection needle **81** is selected depending on the ease of insertion into tissue, damage to tissue that can be tolerated, shear/flow parameters of the fluid such as viscosity, injection force and injection rate required for the fluid, properties of the target tissue, amount of dead volume that remains in the device after injection, and other factors considered by persons skilled in the art. Typically, a small diameter needle **81** is employed to reduce the force required to insert the needle into the target tissue or organ, and to reduce trauma to the target tissue or organ. Generally, injection needle **81** is between 25 and 34 gauge, such as 25 gauge, 26 gauge, 27 gauge, 28 gauge, 29 gauge, 30 gauge or 31 gauge, and typically is 27 gauge.

[0126] The length of the injection needle **81** is dependent on the configuration of the syringe barrel in the device (i.e. whether the syringe barrel is located at the proximal or distal end of the device). The length of the injection needle **81** also is dependent on whether the needle is coupled directly to an intermediary injection tube **83** or is indirectly coupled to an intermediary injection tube **83** by a needle coupler **85**. Such parameters can be related to the pressure drop that can be tolerated, the viscosity of fluid, the dead volume that can be tolerated, and other similar factors. For example, factors that influence pressure drop include the length of the needle, the diameter of the needle, and the viscosity of the fluid. A certain amount of injection pressure can be needed to deliver a fluid, such as a therapeutic, to a specific tissue. A specific injection pressure can be needed for delivery of certain fluid compositions. The injection pressure required can depend on factors such as parameters of the fluid being delivered such as viscosity, injection rate, and target tissue pressure.

[0127] For example, in some variations of the device, the injection needle **81** can be long and extend from the distal tip of the device through the sheath controller **71**

where it is connected to syringe barrel **91** at the proximal end of the device. Hence, the length of the injection needle can range from 5 mm to 500 mm or more, such as 10 mm to 300 mm. Generally, in examples of the devices herein, the injection needle is shorter, which avoids problems in pressure drop that can occur when a solution is injected through a long needle. For example, the length of the injection needle generally can range from 5 mm and 40 mm, such as 10 mm to 40 mm. For example, common needle lengths that are widely available include for example, 12.7 mm, 25.4 mm or 38.1 mm needles. If a longer path is required for solution or fluid to travel (i.e. the syringe barrel is located at the proximal end of the device, e.g. **FIGS. 1A** and **1B**), a smaller injection needle **81** can still be employed, but a pressure drop can be avoided by directly or indirectly coupling a smaller diameter injection needle **81** to an intermediary injection tube **83** of a greater diameter. For example, if the injection needle **81** is 27 gauge, the intermediary injection tube can be 15 gauge to 25 gauge, such as generally 20 gauge to 25 gauge, for example 21 gauge.

[0128] The injection needle **81** of the device is protected by a blunt, elongated needle sheath, which can sheathe and protect the needle prior to injection and un-sheathe the needle at the site of injection. Hence, in all embodiments of the laparoscopic injection device provided herein, such as devices set forth in **FIGS. 1A**, **1B**, **2** or **3**, the needle sheath **72**, **72'** or **72''** is adapted so that the injection needle **81** can be sheathed and un-sheathed. The ability to sheathe or un-sheathe the injection needle **81** permits the operator of the device to control when the injection needle is exposed or when the injection needle is protected. For example, sheathing of the needle can prevent accidental injections or penetrations, damages to the patient's tissue, including the target tissue and non-target tissues, damages to the laparoscopic surgical instruments, such as damages to the elastomeric seals and valves of the laparoscopic port, damage to the needle, and accidental drip of the fluid, such as a therapeutic, during the insertion of the device into the laparoscopic port or removal of the device from the laparoscopic port. At the site of injection, the needle can be un-sheathed, exposing the injection needle **81** to allow the needle tip to penetrate the target site and deliver the agent to the target site, such as the parenchyma of a target organ. The injection needle **81** can be sheathed again after injection to prevent accidental needle puncture of tissue other than the injection site.

[0129] In particular, the needle sheath **72**, **72'** or **72''** is adapted to be controlled by the needle sheath controller **71** or **71'**. The needle sheath controller **71** or **71'** contains the components that control movement of the needle sheath **72**, **72'** or **72''**, connects the proximal and distal ends of the device, and is the conduit by which inner tubings, plungers or other components can travel between the proximal and distal ends of the device. The needle sheath controller **71** or **71'** includes a controller housing **710** that encloses components internal to the

needle sheath controller **71** or **71'**, and the proximal end of the needle sheath **72**, **72'** or **72''**. The needle sheath controller housing **710** can be made of any suitably resilient and rigid material, such as any polymeric material, including plastics, or rubber, metals, ceramics, composites, or other suitable material known to one of skill in the art. Typically, the needle sheath controller housing **710** is made from a plastic, including medical-grade plastics such as polypropylene, polystyrene, polyethylene, polyvinyl chloride, polyurethane, or silicone, rubber or acrylic. The needle sheath controller housing **710** can be molded using any technique known in the art, including compression-molding, thermoforming or injection-molding. The housing **710** can be made of one singular piece, using methods such as by an injection molding. Alternatively, the housing **710** can include multiple pieces that are separately manufactured and attached in a secondary process, such as with adhesive, locking joints, or other fasteners.

[0130] As shown in **FIGS. 1A, 1B, 2** and **3**, the needle sheath controller **71** or **71'** is positioned on the proximal side of the needle sheath **72**, **72'** or **72''**. The needle sheath controller **71** or **71'** is configured to be held and manipulated by an operator, such as a surgeon. The needle sheath controller **71** or **71'** can be any shape and size that is convenient to permit the operator to hold and manipulate the device. Generally, the needle sheath controller **71** or **71'** is cylindrical and can fit into the palm of an average person. The diameter of the needle sheath controller **71** or **71'** is larger than the diameter of the needle sheath **72**, **72'** or **72''** in order to accommodate the proximal end of the needle sheath **72**, **72'** or **72''**. For example, the diameter can be 15 mm to 100 mm, and is generally 20 to 35 mm. The diameter can be uniform or variable. For example, the outside of the needle sheath controller **71** or **71'** can be graduated, contoured, beveled or grooved. The needle sheath controller **71** or **71'** generally has a length of 30 mm to 225 mm, such as 50 mm to 75 mm. On the outside of the needle sheath controller **71** or **71'**, an optional grip can be present to facilitate the manipulation and handling of the device.

[0131] The needle sheath controller **71** or **71'** contains an externally accessible positioner **711**, which controls the position of the needle sheath **72** relative to the injection needle **81**. As can be seen in **FIGS. 1A, 1B, 2** and **3**, the needle sheath controller **71** or **71'** is a cylindrical ring having a positioner **711** extending out of the needle sheath controller **71** or **71'** so that it is accessible to the operator. The positioner **711** can be integrally formed with the housing **710**, or alternatively can be a separate piece coupled to the housing during assembly.

[0132] The positioner **711** is configured in the needle sheath controller **71** or **71'** so that it is movable both forward and rearward relative to the needle sheath controller **71** or **71'**. Movement of the positioner **711** forward or rearward controls movement of the needle sheath **72**, **72'** or **72''** between two fixed or locked positions, the sheathed position **72a** and unsheathed positions **72c**.

When sheathed, the injection needle **81** is hidden inside the needle sheath, and when unsheathed, the injection needle **81** is exposed outside of the needle sheath. The injection needle **81**, however, is fixed and does not move relative to the needle sheath controller **71** or **71'**. Thus, the positioner **711** only controls the movement of the needle sheath **72**, **72'** or **72''**, while the position of the injection needle **81** and other components of the device are stationary regardless of the position of the positioner **711**. The relative position of the injection needle **81**, however, changes with the movement of the needle sheath **72**, **72'** or **72''**, as the needle sheath **71** or **71'** moves in the distal direction or the proximal direction, hiding or exposing the injection needle **81**.

[0133] As shown in **FIG. 4A**, positioning of the positioner in a forward **711a** position moves the needle sheath over the injection needle in the sheathed position **72a** so that the injection needle is hidden inside the shaft of the needle sheath. As shown in **FIG. 4B**, positioning or moving the positioner to an intermediate position **711b**, that is not fully locked forward or rearward, transitions the needle from outside of the needle sheath shaft to a transitional position **72b** that exposes less of the needle than its maximum extent or length. As shown in **FIG. 4C**, positioning of the positioner in the rearward **711c** position moves the needle sheath proximally towards the needle sheath controller to its fully unsheathed position **72c**, thereby permitting maximum exposure of the injection needle **81**.

[0134] The positioner **711** is engaged with the needle sheath and slides the needle sheath. As can be seen in **FIGS. 5-7**, the movement of the needle sheath **72**, **72'** or **72''** by the positioner **711** is facilitated by a connection member **713**. The connection member **713** is connected to the proximal end of the needle sheath **72**, **72'** or **72''** and the lower part of the positioner **711**. The positioner **711** and the needle sheath connector **713** can be connected to each other by welding, adhesive, locking joints, fasteners or other suitable means. The distal end of the connection member **713** is connected to the proximal end of the needle sheath **72**, **72'** or **72''**, such that the sheath is longitudinally movable relative to the controller housing **710** and the injection needle **81**. In particular, the distal end of the outside of the connection member **713** is engaged with the proximal inside lumen **723** of the needle sheath around its circumference. The needle sheath **72**, **72'** or **72''** can be connected to the connection member **713** by welding, adhesive, locking joints, fasteners or other suitable means.

[0135] The lower portion of the positioner **711**, the connection member **713** and proximal end of the needle sheath **72**, **72'** or **72''** are enclosed by the controller housing **710**. With reference to **FIGS. 5-7**, the needle sheath controller housing **710** is molded with an internal needle sheath controller lumen **717** that is a hollow cavity inside the needle sheath controller **71** or **71'** of a sufficient length and diameter to accommodate forward and rearward movement of the connection member **713**. The length

and diameter of the controller lumen 717, however, is always less than the total length and diameter of the needle sheath controller 71 or 71", thereby restricting movement of the needle sheath connector 713 within the inside of the needle sheath controller 71 or 71'. The controller lumen 717 is generally longitudinal along the housing body. The shape of the internal or central lumen 717 of the controller can be any of a variety of shapes and configurations, so long as it provides a tracking means along which the connection member 713 slides. For example, the controller lumen 717 can be cylindrical or rectangular. The controller lumen 717 also can be uniform or non-uniform in shape, size or diameter. For example, the distal and proximal ends can be the same diameter or different diameters.

[0136] The needle sheath controller housing 710 also contains cut-out grooves to serve as sheath stops 715 and 716 that provide a means to engage with the positioner 711. As shown in FIGS. 5-7, the positioner 711 contains a projected top portion or head that juts out of the needle sheath controller 71 or 71' where it can be moved forward or rearward by the operator. Internal to the needle sheath controller 71 or 71', the body of the positioner 711 is notched on its sides or is otherwise configured to engage with sheath stops. The sheath stops 715 and 716 are grooves in the needle sheath controller housing 710 that fit the notched body of the positioner and trap the positioner 711 so that it cannot be moved without external force.

[0137] The positioner 711 is configured to be lockable and releasable in the sheath stops 715 and 716, such that when the positioner is engaged in a sheath stop it is secure to prevent the sheath from moving, but can be conveniently repositioned to control the movement of the sheath. For example, the sheath stops can be configured in a manner that creates a cradle for the positioner so that the positioner 711 is secured within the sheath stop and is not able to fall out of the cradle in the stop. To move the positioner 711 out of the cradle in the stop, the positioner must be physically moved outward from the cradle, so that the positioner 711 can be repositioned. To lock the positioner, the positioner must be physically moved inward (towards the grooves or cradle in the stop) to engage with the cradle created in the stop. Thus, the positioner 711 can also be pivoted to move outward (away from the grooves or cradle in the stop) to unlock from the sheath stops 715 and 716, then slid along the longitudinal axis to change positions, and pivoted again to move inward (towards the grooves or cradle in the stop) to engage with and lock into the sheath stops 715 and 716 to lock the positioner 711 and the needle sheath 72.

[0138] As an alternative, the positioner 711 can contain a lock and release element that facilitates lock and release of the positioner with the grooves of the sheath stops. FIG. 5 depicts an optional lock and release element 712 that can be contained in the positioner to facilitate lock and release of the positioner 711 with the

grooves of the sheath stops. For example, the lock and release element 712 can be a spring or other resilient means. When the positioner 711 is moved or fit into the grooves of a stop it is locked into place by a vertically upward force against the positioner 711 and a downward force against the connection member 713. Pressing the positioner 711 vertically downwards releases the vertically upward force applied by the lock and release element 712, and releases the positioner from the stops.

[0139] Because the positioner 711 and the connection member 713 are connected, the movement of the positioner 711 can control the movement of the connection member 713 and the connected needle sheath 72, 72' or 72". Therefore, movement of the positioner 711 between the sheath stops 715 and 716 moves the needle sheath 72, 72' or 72" between the sheathed and un-sheathed positions. In other variations, the lock and release mechanism can be a latch or switch that can be selectively engaged or disengaged according to its mechanical nature, for example, by sliding a latch or pivoting a lever attached to the head of the positioner 711, thereby moving it out of the way of a notch or other fastening mechanisms in the groove of the sheath stops.

[0140] For example, with reference to FIGS. 5-7, the needle sheath controller housing 710 contains two sheath stops 715 and 716 that are arranged into the needle sheath controller housing 710 on the proximal and distal sides of the positioner 711. With reference to FIG. 5, when the positioner 711 is engaged in either of the sheath stops 715 or 716, the lock and release element 712, such as a spring, can exert a force against the positioner 711 in the vertically upward direction, and the connection member 713 in the downward direction. Unless force is applied against the lock and release element 712 by pressing the positioner 711 down, the positioner 711 and connection member 713 have a tendency to be pushed away from each other in the vertical direction, due to the force exerted by the lock and release element 712. The force that pushes the positioner 711 in the upward direction permits the positioner 711 to be locked in place in either the distal sheath stop 715 or the proximal sheath stop 716. If the positioner 711 is pressed vertically downward, the positioner 711 is freed from the grooves and can move in the forward or rearward direction longitudinally.

[0141] FIGS. 5-7 demonstrate the alternative positions of the positioner 711 relative to the sheath stops. For example, FIG. 5 depicts the positioner 711 in the forward position 711a where it is engaged or fit into the distal sheath stop 715. When the positioner 711 is engaged with distal stop 715, the connection member 713 is longitudinally moved to the furthest distal position within the controller lumen 717 and the sheath is in the extended position hiding the needle tip. FIG. 6 depicts the positioner 711 in the rearward position 711c where it is engaged or fit into the proximal sheath stop 716. When the positioner 711 is engaged with proximal stop 716, the connection member is longitudinally moved towards the

proximal end of the needle sheath lumen, thereby exposing the injection needle. **FIG. 7** depicts the positioner **711** in an intermediate position **711b** after releasing the positioner from its locked position in either sheath stop and sliding the positioner along the longitudinal axis. In this position, the injection needle **81** is in an intermediate unsheathed position, but is not fully exposed.

[0142] The extent or length of the injection needle **81** that can be exposed or unsheathed at the distal end of the device is related to the distance along the longitudinal axis between a first sheath stop and a second sheath stop, which is the distance that the positioner **711**, and hence connection member **713** controlling the position of the sheath, moves between locked positions. For example, with reference to **FIGS. 5-7**, the extent or length of the injection needle **81** that can be exposed or unsheathed at the distal end of the device can be substantially the same as the distance between the distal sheath stop **715** and the proximal sheath stop **716**. It is understood, however, that the extent or length of the injection needle that is exposed can be somewhat longer or shorter than the distance between the first and second groove stop due to a slight recess of the distal tip of the injection needle in the distal tip of the needle sheath when it is unsheathed. For example, if the distal tip of the injection needle **81** is recessed from the distal tip of the needle sheath **73** in the fully sheathed position **72c**, the extent or length the injection needle that can be exposed is shorter than the distance between a first sheath stop and a second sheath stop. A needle that is exposed substantially the same as the distance between the sheath stops is recessed only slightly and no more than 1 mm, such that the difference in the distance of the sheath stop and the length that the injection needle that can be exposed is less than 1 mm or 0.5 mm or less. As an example, if the distal tip of the injection needle **81** is slightly recessed from the distal tip of the needle sheath **73** in the fully sheathed position **72c**, the maximum extent or length of the injection needle that can be exposed or unsheathed at the distal end of the device is the distance between the distal sheath stop **715** and the proximal sheath stop **716**, minus the slight distance between the tip of the injection needle **81** and the distal tip of the needle sheath **73** in the fully sheathed position.

[0143] In other examples, the length of the injection needle that is exposed or extended is appreciably shorter than the distance between the sheath stops. In this case, the injection needle can be positioned so that it is recessed inside the distal tip of the needle sheath **73** in the unsheathed position **72c** more than 1 mm, and generally 2 mm to 5 mm, from the distal tip of the needle sheath **73** in the unsheathed position **72c**. Thus, if the distal tip of the injection needle **81** is recessed from the distal tip of the needle sheath **73** in the fully sheathed position **72c**, the maximum extent or length of the injection needle that can be exposed or unsheathed at the distal end of the device is the distance between the distal sheath stop **715** and the proximal sheath stop **716**, minus the distance

between the tip of the injection needle **81** and the distal tip of the needle sheath **73** in the fully sheathed position.

[0144] The extent or length of the injection needle **81** that is exposed when unsheathed can be empirically determined, and is a function of the target tissue, the particular subject being treated, the agent being administered and other factors within the level of a skilled artisan. For example, the extent of the injection needle that is unsheathed is of a sufficient length so that the needle tip can penetrate the parenchyma of the target tissue of interest, but not so long that it can easily pass through or puncture the target tissue through to the other side. Typically, the desired length of the exposed injection needle when unsheathed is from or from about 2 mm to 10 mm, such as generally 5 mm to 10 mm. For example, general adult tissues, such as the liver, have a thickness of 10 mm to 30 mm. The thickness of the tissue can vary depending on the anatomical dimensions of the subject, such as age, height, weight, and/or the type of tissue or organ. Hence, the distance between the distal sheath stop **715** and the proximal sheath stop **716** is 2 mm to 15 mm, such as 2 mm to 12 mm, 2 mm to 10 mm, such as generally 5 mm to 10 mm.

[0145] In variations of the injection devices herein, more than two sheath stops, such as 3, 4, 5 or more sheath stops, can be configured into the needle sheath controlling housing **710** that can each engage separately with the positioner **711** to lock the sheath. Engagement of the positioner with the most distal sheath stop locks the sheath in its fullest extended position to completely hide the injection needle inside the needle sheath. Engagement of the positioner with the most proximal sheath stop locks the sheath in its fullest retracted or opened position to maximally expose the injection needle outside of the needle sheath. The other sheath stops provide means to vary the length of the exposed injection needle from its fully sheathed or unsheathed positions. Hence, the length of the exposed injection needle **81** can be varied with use of multiple needle sheath lock grooves. For example, in addition to the proximal **715** and distal **716** needle sheath stops, several additional sheath stops can be present, between the proximal and distal stops, permitting the positioner **711** and the needle sheath **72**, **72'** or **72''** to be locked in several different positions, with different lengths of the injection needle **81** exposed. As an example, the controller housing **710** can contain four sheath stops that are separated along the longitudinal axis by a distance of 2 mm. Thus, the positioner **711** can be locked in four different positions, resulting in positioning of the injection needle so that it can be sheathed, or exposed by 2 mm, 4 mm or 6 mm.

[0146] The connection member **713** contains a central cavity that is also longitudinal along the housing body and is of a sufficient size to slide around and independently from components of the device that traverse through the needle sheath controller **71**, **71'** or **71''**. For example in **FIGS. 5-7**, an injection tube or plunger can traverse through the inside of the needle sheath control-

ler across its longitudinal axis. In particular, **FIG. 5** shows an intermediary injection tube **83** that traverses through the inside of the needle sheath controller, and the connection member **713** contains a central cavity that slides around and independently from the injection tube **83**. The injection tube **83** is fixed to the needle sheath controller **71** at its proximal end. As shown in **FIGS. 6-7**, the plunger **92'** or **92"**, respectively, longitudinally traverses through the inside of the needle sheath controller **71'**, and the connection member **713** contains a central cavity that accommodates and slides around and independently from the plunger **92'** or **92"**. The plunger is movable within the needle sheath controller **71'** and is not fixed thereto. The particular width or size of the cavity is dependent on the particular component that traverses through it. The connection member **713** is disengaged from and moves independently with respect to the components (e.g. injection tube or plunger) that run through its internal central cavity.

[0147] In aspects of the injection device provided herein, the needle sheath optionally has a visibility window, allowing visualization of the drawback fluids to test needle placement in target organs. For injections into the parenchyma of a target organ that has extensive vasculature, the drawback fluid can be used to confirm needle placement into the parenchyma, and avoid injections into the vasculature or the bile duct. At the site of injection, the plunger can be pulled back slightly to draw a small amount of fluids, in order to determine whether the needle was placed at a blood vessel or the target organ. Once the needle **81** is positioned and has penetrated the target injection site, the plunger **92, 92' or 92"** can be depressed to deliver the fluid, such as a therapeutic, contained in the syringe barrel to the target site.

[0148] The syringe barrel **91, 91' or 91"** and/or the device can be disposable or reusable. For example, except if the syringe is integrated with the device, the syringe barrel can be removed after injection or exhaustion of the fluid, such as a therapeutic, replaced with a new loaded syringe, or reloaded and re-connected. If the syringe barrel is at the outside the laparoscopic port, such as described with device **60**, this can be achieved without the need to withdraw the device from the laparoscopic port. In some cases, the device can be withdrawn from the laparoscopic port and disposed of after one use. The method of loading and the type of syringe and syringe format employed can be empirically determined and is a function of factors considered by persons of skill in the art, such as the objective of the injection, target tissue or organ, dose and frequency of injections needed, properties of the fluid, such as a therapeutic, composition, and surgical environment.

[0149] For clarity of description, exemplary embodiments of the injection device are described below. It is understood that for the described embodiments, general aspects and components of the device are the same, and that different aspects or components are so described. Thus, except as noted, the description of the various ex-

emplary embodiments and the structures of the embodiments described above apply to all embodiments of the injection device. Additionally, the methods of using the injection device, for example for injection of a fluid, such as a therapeutic, to a target tissue during a minimally invasive procedure, apply to all embodiments as well. The particular injection device employed can be empirically determined and is a function of factors considered by persons of skill in the art, such as the objective of the injection, target tissue or organ, dose and frequency of injections needed, properties of the fluid, such as a therapeutic, composition, and surgical environment.

1. STANDARD INJECTION DEVICE

[0150] **FIGS. 1A-B, 5, 8A-B, and 9A-D** depict the injection device **60** and components and features thereof. The injection device as shown in **FIGS. 1A** and **1B** includes needle sheath **72**, needle sheath controller **71**, injection needle **81**, syringe barrel **91** and plunger **92**. With reference to **FIG. 1A**, generally, the needle sheath **72** of the injection device is of a sufficient length to permit laparoscopic access to the target of interest, and is generally a length of 200 mm to 600 mm, such as 250 to 400 mm, and generally at least or about at least or 300 mm. The device is generally cylindrical around the longitudinal axis, generally having a smaller diameter in the needle sheath **72** region and the plunger **92** region, and a larger diameter in the needle controller **71** region. The needle sheath **72** portion of the device is typically inserted through the laparoscopic port. The diameter of the needle sheath **72** is typically between 3 mm to 12 mm in size, and typically from 5 mm to 10 mm. It is understood that the portions of the device external to the laparoscopic port can have a diameter greater than 10 mm. For example, the needle sheath controller body **71** can have a diameter sufficiently large, so long as it can be easily gripped or handled by the operator. The needle sheath controller body **71** is held by the operator, typically a surgeon, to manipulate and position the device **60**, control the needle sheath **72**, and support the device while manipulating the plunger **92**.

[0151] The syringe barrel **91** is cylindrical in shape with a hollow center that can fit plunger **92** so that the plunger can move back and forth inside the syringe barrel. The syringe barrel is generally clear and transparent. The syringe barrel **91** can be made out of plastic or glass or other suitable material, and in particular is made out of plastic such as polypropylene, polyethylene, polycarbonate or other clear material. As described above, the syringe barrel **91** can contain calibrations or marking on the outer surface to indicate the volume of the agent within the barrel. As described above, the syringe barrel **91** can have a volume capacity that is from the range of 0.5 mL to 20 mL (i.e. 0.5 cc to 20 cc), and generally is 0.5 mL to 3 mL (i.e. 0.5 cc to 3 cc), such as at least or about a 1 mL (i.e. 1 cc) syringe. Typically, 200 μ L to 600 μ L of the fluid, such as a therapeutic, is delivered to the target

locus, and the volume of syringe barrel is 1 mL.

[0152] The syringe barrel **91** is positioned proximal to the injection needle **81**, and on the proximal side of the needle sheath controller **71**. As shown in **FIG. 1A**, the distal end of the syringe barrel **91** contains a Luer fit adaptor **93** that is compatible with a needle hub **84** on the proximal side of the needle sheath controller **71**. The syringe barrel **91** is removable and attachable with the needle sheath controller **71** and the connected needle sheath **72** by manipulation of the Luer fit locking mechanisms. **FIG. 1A** shows the syringe in the detached position **900a**. Thus, a sterile syringe barrel **91** can conveniently be used when drawing up or loading the syringe with a fluid, such as a therapeutic, compositions or other solutions into the syringe barrel. If desired, a separately sterile needle can be fitted on the Luer fit adaptor **93** to permit loading of the syringe barrel **91** with a fluid, such as a therapeutic. After the agent is drawn up into the syringe, the syringe barrel **91** (without needle) can be secured to the needle sheath controller **71** through the Luer fit adaptor **93** on the distal end of the syringe barrel **91** and the needle hub **84** on the proximal end of the needle sheath controller **71**. In some cases, a pre-loaded syringe with standard Luer fit adaptor **93** can be connected. **FIG. 1B** shows injection device **60** with the syringe barrel **91** secured to the needle sheath controller, in the connected position **900b**. Advantages of device **60** having a removable and attachable syringe barrel **91** include the ease of loading the syringe barrel and exchange of loaded syringe. Since standard syringes can be used to connect to the needle sheath control **71**, a variety of syringe types can be used, and several different types of syringes can be used for one patient, if necessary. In cases where the syringe must be re-loaded or additional fluid is needed, new or re-loaded syringes can easily be connected.

[0153] The plunger **92** is located on the proximal end of the device **60** and is movable so that it can be pulled and pushed along the inside of the syringe barrel **91**. The plunger **92** can be drawn back to load the syringe barrel **91** with the fluid or depressed to inject the fluid in the target tissue. The plunger **92** can also be pulled back at the site of injection to test needle placement. The plunger is cylindrical to move through the syringe barrel **91**, and is made of a material that permits ease of movement through the syringe barrel, such as a plastic, for example polypropylene or polyethylene. The plunger contains a head **95** at the proximal end of the device that can be conveniently grasped by the operator to manipulate the plunger. The plunger head **95** also is generally made of plastic. The distal tip of the plunger **92** is generally made of silicone or other natural or synthetic rubber to provide a tight seal within the syringe barrel **91** when traveling within the syringe barrel **91**.

[0154] The plunger **92** is long enough in length to permit its association with the inside of the syringe barrel **91** in order to dispel the fluid through the distal end of the syringe (and into a needle or tube if connected thereto). For example, the plunger is 5 cm to 50 cm, such as 5 cm

to 30 cm or 10 cm to 20 cm. Pulling back on the plunger **92** draws in the fluid, such as a therapeutic, or air, and pushing the plunger **92** forces the fluid, such as a therapeutic, or air out of the syringe barrel. Optionally, the plunger can contain syringe barrel base **94** that can aid manipulation of the syringe barrel **91** with respect to the plunger **92**.

[0155] The syringe barrel **91** and/or the device **60** can be disposable or reusable. For example, the syringe barrel **91** connected to the proximal side of the needle sheath controller **71** through a Luer fit adaptor **93**, can be removed after injection of the fluid, such as a therapeutic, replaced with a new loaded syringe, or reloaded and re-connected, with or without the need to withdraw the device from the laparoscopic port. The device **60** can be withdrawn from the laparoscopic port and disposed of after one use.

[0156] The device **60** contains an injection needle **81** that is located inside the needle sheath **72** that can be sheathed and unsheathed at the distal tip of the needle **81**. With reference to **FIG. 1A**, the distal tip of the needle sheath **73** contains a needle channel **733** that guides the needle outside of the needle sheath **72** when it is unsheathed as shown in **FIG. 1B**. As shown in **FIG. 1B**, the injection needle **81** contains a beveled tip sufficient to penetrate or pierce a tissue or an organ.

[0157] **FIG. 5** depicts an enlarged cross section view of the distal end of the syringe barrel **91** and the needle sheath controller **71**. As shown in **FIG. 5**, the plunger **92** is contained within the syringe barrel **91**, which optionally can contain a syringe base **94**, where it can movably travel. The needle sheath controller **71** is positioned on the proximal side of the needle sheath **72**. The needle sheath controller **71** contains the components that control movement of the needle sheath **72**, connect the proximal and distal ends of the device, and is the conduit by which the injection needle **81**, directly or indirectly connected to an intermediary injection tube **83**, travel between the proximal and distal ends of the device. The needle sheath controller **71** is configured to be held and manipulated by an operator, such as a surgeon. As discussed above, the needle sheath controller **71** can be any shape and size that is convenient to permit the operator to hold and manipulate the device, and typically is cylindrical in shape. The diameter of the needle sheath controller **71** is such that it can be held in the palm of an average adult, and is generally 20 mm to 100 mm in diameter with a length of 50 mm to 225 mm. The needle sheath controller **71** optionally can contain an outside grip for handling.

[0158] As shown in **FIG. 1A-B** and **FIG. 5**, the needle sheath controller **71** includes a controller housing **710** that encloses components internal to the needle sheath controller **71**, and the proximal end of the needle sheath **72**. As discussed above, the needle sheath controller housing **710** can be made of any suitably resilient and rigid material, such as any polymeric material, including plastics, or rubber, metals, ceramics, composites, or other suitable material known to one of skill in the art. The

controller housing **710** is typically made of polypropylene, polystyrene, polyethylene, polyvinyl chloride, polyurethane, silicone, rubber or acrylic. As discussed above, the housing **710** can be made by any manufacturing known to a skilled artisan, and can be made as one singular piece or can be made of two or more pieces that are attached together, such as with adhesive, locking joints or fasteners.

[0159] As shown in **FIG. 1A** and **1B**, the needle sheath controller **71** contains an externally accessible positioner **711**. As described above, the positioner **711** is configured in the needle sheath controller **71** so that it is movable both forward and rearward relative to the needle sheath controller **71**. As described above, the positioner **711** is engaged with the needle sheath **72** through a connection member **713**, and can be used to slide the needle sheath **72**. This connection permits movement of the positioner **711** between the forward or rearward positions to control movement of the needle sheath between two fixed or locked positions, the sheathed and unsheathed positions. The sheathed position protects or hides the injection needle, while the unsheathed position exposes the needle.

[0160] With reference to **FIG. 5**, the connection member **713** is connected to the proximal end of the needle sheath **72**, and the lower part of the positioner **711**. The connection of the connection member **713** with the proximal end of the needle sheath is such that the needle sheath **72** is longitudinally movable relative to the controller housing **710** and the injection needle **81**. For example, the distal end of the outside of the connection member **713** is engaged with the proximal inside cavity of the needle sheath **72** around its circumference. The connections of the control member **713** with the positioner **711** and needle sheath **72** can be by welding, adhesive, locking joints, fasteners or other suitable means.

[0161] As described above generally, the connection member **713** moves inside a hollow cavity or lumen **717** contained inside the housing **710** of the needle sheath controller **71** that is closed at both ends relative to the housing **710**. The controller lumen **717** accommodates the connection member **713** such that the connection member **713** can easily glide or move forward or rearward in a restricted manner. For example, the connection member **713** can be cylindrical and fit inside a cylindrical hollow lumen cavity **717**. As shown in **FIG. 5**, and discussed further below, the connection member **713** contains an internal hollow cavity to fit the injection tube **83** that passes through.

[0162] Movement of the connection member **713** is controlled by the positioner **711**. As shown in **FIGS. 1A, 1B** and **5**, the positioner **711** contains a projected top portion or head that juts out of the needle sheath controller **71** where it can be moved forward or rearward by the operator. As shown in **FIG. 5**, internal to the needle sheath controller **71**, the body of the positioner **711** is notched on its sides or is otherwise configured to engage with sheath stops **715** or **716**. Sheath stops **715** and **716**

are grooves in the needle sheath controller housing **710** that fit the notched body of the positioner and trap the positioner **711** so that it cannot be moved.

[0163] **FIG. 5** depicts the optional lock and release element **712** configured in the positioner **711** to facilitate lock and release of the positioner with the grooves of the sheath stop **715** or **716**. For example, the lock and release element **712** can be a spring or other resilient means. The mechanism controlling lock and release of the positioner **711** with the grooves of the sheath stop **715** or **716** by the lock and release element **712** is as described above, whereby downward, vertical or lateral forces release or lock the positioner **711** from the sheath stops **715** or **716**. Pushing downward on the positioner **711** permits the positioner to slide and to fit it into either of sheath stops **715** or **716**.

[0164] Movement of the positioner **711** between the sheath stops **715** and **716** moves the connection member **713**, and thereby also moves the needle sheath **72** so that it can transition from the sheathed and unsheathed positions by control of the positioner by the operator. When the positioner is in the forward position **711a** as exemplified in **FIG. 5**, proximal sheath stop **716** is free and the positioner **711** is fit into the distal sheath stop **715**, thereby sheathing the injection needle so that it is protected. While not shown in **FIG. 5**, the positioner **711** also can be in the rearward position **711c** as exemplified in **FIG. 6**, where the distal sheath stop **715** is free and the positioner **711** is fit into the proximal sheath stop **716**, thereby unsheathing the injection needle so that it is exposed. As a further position, the positioner **711** also can be in an intermediate position **711b** as exemplified in **FIG. 7**, where both the distal sheath stop **715** and the proximal sheath stop **716** are free and not engaged with the positioner **711**.

[0165] The injection needle **81** shown in **FIG. 1B** is indirectly connected to the syringe barrel **91** through an intermediary injection tube **83** as shown in **FIG. 1A** and **5**. The injection tube **83** contains a proximal needle hub **84** that is secured with the Luer fit adaptor **93** of the syringe barrel **91**. The injection tube **83** is fixed directly to the needle sheath controller housing **710** so that the injection tube, and hence injection needle coupled thereto at the distal end of the device, is not movable.

[0166] As shown in **FIG. 5**, the injection tube **83** passes through the inside lumen **717** of the needle sheath controller **71** and passes through a central cavity of the connection member **713**, but is not directly attached to the connection member. Hence, the connection member **713** can move independently around the fixed injection tube **83**. As discussed above, because the needle sheath **72** is directly connected to the connection member **713** contained in the controller lumen **717**, the injection tube **83** enters the lumen **723** of the needle sheath **72** inside the needle sheath controller **71**. The injection tube **83** exits the distal end of the needle sheath controller **71** where it is contained within the hollow cavity of the needle sheath **72**.

[0167] With reference to **FIGS. 8A** and **8B**, the injection tube **83** runs distally and longitudinally through the needle sheath **72** where it is connected to the injection needle **81**. The injection tube **83** and the injection needle **81** can be made of one piece, or made of more than one separate pieces. When the injection tube and injection needle **81** are made of one piece, the injection tube **83** can also be an elongated tapered needle, having a larger diameter in the proximal region, and a smaller diameter in the distal region near the injection needle **81**. Optionally, a needle coupler **85**, made of the same or different material, can be used to indirectly connect the two parts. The injection tube **83** and injection needle **81** can be made of the same material, or of different material. The injection tube **83** and the injection needle **81** have the same diameter, or a different diameter.

[0168] As shown in **FIGS. 8A** and **8B**, the injection tube **83** is indirectly coupled to the injection needle **81** through a needle coupler **85**. The coupler **85** connects the injection tube **83** to the injection needle **81** to form a continuous sealed fluid pathway for solution to move through. The connection can be by welding, bonding, molding or other procedure that creates a secure and reliable seal. The coupler **85** can be made of any biocompatible and drug compatible material suitable to provide a seal, and generally is made of a plastic. The coupler **85** can be clear or transparent or opaque. For example, the coupler **85** can be made of polycarbonate or other clear material. As discussed further below, in embodiments where the needle sheath **72** contains an optional visibility window **724** to view drawn up fluids, the needle coupler **85** generally is clear or transparent to permit visualization of the fluid or solution through the window.

[0169] The injection needle **81** contains a beveled tip sufficient to penetrate or pierce a tissue or an organ. The injection needle **81** is typically made of metal or alloy, such as surgical stainless steel or other medical grade metal. The size and diameter of the injection needle **81** is selected based on parameters described above. As described above, typically a small diameter needle **81** is employed to reduce the force required to insert the needle into the target tissue or organ, and to reduce trauma to the target tissue or organ. For example, the injection needle **81** is between 25 and 34 gauge, such as a 25 gauge, 26 gauge, 27 gauge, 28 gauge, 29 gauge, 30 gauge or 31 gauge needle, and typically is 27 gauge.

[0170] The gauge of the injection tube **83** can be the same or different than the injection needle **81**. The device provided herein is generally designed, however, to minimize pressure drop throughout the path that the fluid traverses. Factors that influence the pressure within the column of fluid includes the length of the needle, viscosity of the fluid contained within, rate of delivery of the fluid, and the gauge of the needle. The device is designed to have reasonable axial force requirements to depress the plunger **92**, thereby permitting delivery of the fluid in a laparoscopic manner with sufficient injection pressure. For example, the axial force required to depress the

plunger **92** in order to inject the fluid to the target organ is typically less than 2 pounds of force (lbf), preferably less than 1 lbf. The axial force required to depress the plunger **92** can also depend on the desired rate of delivery of the fluid, and the optimal pressure can also depend on the operator. In some cases, a significant injection force can be required to inject the fluid through a long needle of the laparoscopic device. To prevent an immediate significant pressure drop when the fluid traverses the injection tube **83**, a larger gauge injection tube can be used. Thus, in order to reduce pressure drops that can occur due to the long path created by the continuous sealed fluid pathway made up of the injection tube **83**, coupler **85** and injection needle **81**, the injection tube **83** generally has a larger diameter than the injection needle **81**.

[0171] For example, if the syringe barrel **91** is positioned at least 300 mm proximal to the injection needle **81**, and the fluid, such as a therapeutic, must traverse a long path through the needle sheath shaft **72**, a significant pressure drop can occur. In this case, an injection tube **83** of a larger diameter can be used, coupled to an injection needle **81** with a smaller diameter, to prevent the large pressure drop when traversing through a narrow needle **80**. An optional needle coupler **85** can be used to join the injection tube **83** with the injection needle **81**. The needle coupler **85** contains a recess by which the injection tube **83** and the injection needle **81** can be press fit to stably hold the position of the needle components in place within the needle sheath lumen **723**. The needle coupler **85**, can optionally contain a coupling member **82** to facilitate coupling of the injection tube **83** and the injection needle **81** in the recess of the needle coupler **85**.

[0172] If the gauge of the injection tube **83** and injection needle **81** are different, the coupler **85** can be sized to fit the opposing diameters, for example, it can be beveled on its proximal or distal end. In particular examples, the injection tube **83** is 15 gauge to 25 gauge, and the injection needle **81** is 25 gauge to 34 gauge. For example, the injection tube **83** is 21 gauge and the injection needle **81** is 27 gauge. The injection tube **83** can be made of metal or plastic, such as any surgical grade materials. The combined length of the injection tube **83**, coupler **85** and injection needle **81** is sufficiently long to pass from the distal end of the syringe barrel **91** to the distal end of the needle sheath **72**, for example is 100 mm to 600 mm long, and generally at least or about at least 300 mm. The particular size of the injection tube **83**, coupler **85** and injection needle **81** can be chosen by the user and can depend, for example, on the convenience of available injection needles. For example, commonly used injection needles are sized as 12.7 mm, 25.4 mm or 38.1 mm needles.

[0173] The continuous sealed fluid pathway formed by the injection tube **83**, coupler **85** and injection needle **81** pass through and traverse the central inside hollow cavity or lumen **723** of the needle sheath **72**. The needle coupler **85** also holds the injection tube **83**, and injection needle

81, so that the needle sheath 72 can slide over the injection tube 83, needle coupler 85 and injection needle 81 when the sheath is moved between the sheathed position 72a and unsheathed position 72c. For example, the needle coupler 85 is loosely fit into the hollow circular sheath lumen 723. Thus, the needle sheath 72 moves independently from the needle coupler 85. The needle coupler 85 can be made of any biocompatible and drug compatible rigid material, including metals, plastics, and ceramics, and is typically made of plastics such as polycarbonate or Acrylonitrile butadiene styrene (ABS). The injection tube 83 and injection needle 81 can be press fit into the recess of the needle coupler to create a stable fixed relationship with the needle coupler 85, and hence also the housing 710. An optional coupling member 82 can be present inside the recess of the needle coupler 85 and can be connected to the injection tube 83 and injection needle 81. The coupling member 82 is coupled to each of the intermediary injection tube 83 and injection tube 81 by welding, bonding, molding or other procedure that creates a secure and reliable seal. The coupling member 82 can be made of any biocompatible and drug compatible rigid material, including metals, plastics, and ceramics, and is typically made of plastics such as polycarbonate or Acrylonitrile butadiene styrene (ABS).

[0174] At the distal end of the device 60, the needle sheath 72 ends in a distal tip of the needle sheath 73 that contains a needle channel 733. The needle channel 733 is sufficiently sized to fit the injection needle 81 so that the injection needle can extend and retract through the needle channel 733 as the needle sheath 72 moves. In FIG. 8A, the injection needle 81 is covered by the needle sheath 72 and does not traverse through the distal portion of the needle channel 733. With reference to FIG. 4A, the device 60 in FIG. 8A is in the sheathed position 72a. In FIG. 8B, the injection needle 81 is extended out of the needle sheath 72 and does traverse through the distal portion of the needle channel 733. With reference to FIG. 4C, the device 60 in FIG. 8B is in the unsheathed position 72c.

[0175] In the unsheathed position, the needle sheath 72 is pulled back, but the injection tube 83, needle coupler 85 and injection needle 81 are fixed and do not move. For example, as shown in FIG. 8B, because the needle sheath 72 is pulled back, the size of the sheath lumen 723 between the distal end of the needle coupler 85 and the distal tip 73 of the device is shortened compared to the size of the corresponding sheath lumen shown in FIG. 8A. This demonstrates that movement of the sheath, as described with reference to FIG. 5 above using the positioner 711, only controls the movement of the needle sheath 72, while the position of the injection needle 81 and other components of the device are stationary regardless of the position of the positioner 711.

[0176] As described above, in the unsheathed position, the extent by which the injection needle 81 is extended or exposed out of the device 60 is a function of the distance between the sheath stops 715 and 716 as

shown in FIG. 5. This distance is a function of the particular application of the device, the particular target tissue, the subject being treated and other considerations. For example, unsheathed needle that is exposed should not be so long that it can easily penetrate through to the other side of a target tissue. Generally, with reference to most target tissues (e.g. liver), the portion of the injection needle 81 shown in FIGS. 8B, 9B and 9D that can be unsheathed or exposed is generally less than 1 cm, such as 2 mm to 10 mm, and generally no more than 5 mm. For a child, the length can be smaller, and is generally less than 4 mm. For applications *in utero*, the length can be 2 mm to 3 mm.

[0177] The needle sheath 72 can be solid or can be transparent or clear. In some cases, the needle sheath 72 contains an optional visibility window 724. As described above, the presence of the visibility window 724 allows visualization of the administered agent or solution as well as the drawback fluids. For example, since some applications require injection directly into the parenchyma, and not into a vessel or bile duct, the ability to drawback and visualize fluid from the area the needle has penetrated can be used to confirm needle placement into the parenchyma, while avoiding injections into the vasculature or bile ducts. Since device 60 is long and the plunger 92 is outside of the body it is helpful to visualize the fluid path closer to the injection site and within the view of the laparoscope. To achieve this, a visibility window 724 can optionally be present in the needle sheath 72 to visualize the fluid path through a clear or transparent needle coupler 85. FIGS. 9A and 9C provide corresponding perspective views of the needle sheath shown in FIG. 8A in the sheathed position 72a. In FIG. 9A, the needle sheath 72 is solid and the injection needle inside the sheath cannot be visualized. In FIG. 9C, the needle sheath 72 contains a visibility window 724 that permits visualization of the inside components of the needle sheath 72, including the injection needle. Likewise, FIGS. 9B and 9D provide corresponding perspective views of the needle sheath shown in FIG. 8B in the unsheathed position 72c. In FIG. 9B, the needle sheath 72 is solid and the injection needle 81 inside the sheath is extended, but otherwise cannot be visualized inside the needle sheath 72. In FIG. 9D, the needle sheath 72 contains a visibility window 724 that permits visualization of the inside components of the needle sheath 72, including the portion of the injection needle 81 that is not extended out of the sheath. It is understood that the visualization window 724 in FIGS. 9B and 9D is for exemplification only, and that the visualization window can be any desired size. For example, the visualization window can extend the entire sheath. It also can extend distally and include portions of the distal tip of the needle sheath 73. Other variations also are contemplated and can be easily envisioned by a skilled artisan in view of this description.

[0178] The syringe barrel and/or the device can be disposable or reusable. For example, the syringe barrel 91 connected to the proximal side of the needle sheath con-

troller **71** through a Luer fit adaptor **93**, can be removed after injection or exhaustion of the fluid, such as a therapeutic, replaced with a new loaded syringe, or reloaded and re-connected, without the need to withdraw the device from the laparoscopic port. In some cases, the device **60** can be withdrawn from the laparoscopic port and disposed of after one use, or can be re-used.

[0179] With reference to the above Figures, exemplary of the mode of operation of the injection device **60** involves loading a standard syringe (e.g. 1 mL insulin syringe) containing a syringe barrel **91** and plunger **92** with a fluid, such as a therapeutic, prior to connecting the syringe to the needle sheath controller **71** via the Luer fit adaptor **93** of the syringe barrel **91** and the needle hub **84** connected to the injection tube **83**. Once the syringe barrel **91** is loaded and connected to the needle sheath controller **71**, the needle sheath **72** can be positioned in the sheathed position **72a**, and the device can be inserted into a laparoscopic port to be placed near the site of injection. At the site of injection (target tissue), the needle sheath **72** can be unsheathed **72c**, and the injection needle **81** can be exposed for injection. If necessary, the plunger **92** can be pulled back to draw fluids from the site of injection, to test the placement of the injection needle **81** at the injection site. The optional visibility window **724** can be used to visualize the drawback fluid from the injection site. Once the site of needle placement is determined, the plunger **92** can be depressed, to inject the fluid, such as a therapeutic, at the target tissue. After injection, the needle sheath **72** can be positioned in the sheathed position **72a**, to protect the non-target organs and prevent accidental needle puncture, prior to removing the laparoscopic device from the injection site and through the laparoscopic port.

2. INTEGRATED INJECTION DEVICE

[0180] **FIGS. 2, 6** and **10A-D** depict the injection device **60'** and components and features thereof. The injection device as shown in **FIG. 2** includes needle sheath **72'**, needle sheath controller **71'**, injection needle **81**, syringe barrel **91'** and plunger **92'**. The needle sheath **72'** of the injection device is of a sufficient length to permit laparoscopic access to the target of interest, and is generally a length of 200 mm to 600 mm, such as 250 to 400 mm, and generally at least or about at least or 300 mm. The device is generally cylindrical around the longitudinal axis, generally having a smaller diameter in the needle sheath **72'** region and the plunger **92'** region and a larger diameter in the sheath controller **71'** region. The needle sheath **72'** of the device is typically inserted through the port (e.g. laparoscopic port). The diameter of the needle sheath **72'** is typically from 3 mm to 12 mm in size, and typically from 5 mm to 10 mm. It is understood that portions of the device external to the laparoscopic port can have a diameter greater than 10 mm. For example, the needle sheath controller body **71'** can have a diameter sufficiently large, so long as it can be easily gripped or

handled by the operator. The needle sheath controller body **71'** is held by the operator, typically a surgeon, to manipulate and position the device **60'**, control the needle sheath **72'** and support the device while manipulating the plunger **92'**.

[0181] The syringe barrel **91'** is cylindrical in shape with a hollow center that can fit plunger **92'** so that the plunger can move back and forth inside the syringe barrel. The syringe barrel is generally clear and transparent. The syringe barrel can be made out of plastic or glass or other suitable material, and in particular is made of plastic such as polypropylene, polyethylene, polycarbonate or other clear material. As described generally above, the syringe barrel **91'** can contain calibrations or markings on the outer surface to indicate the volume of the agent within the barrel. As described above, the syringe barrel **91'** can have a volume capacity that is from the range of 0.5 mL to 20 mL (i.e. 0.5 cc to 20 cc), and generally is 0.5 mL to 3 mL (i.e. 0.5 cc to 3 cc), such as at least or about a 1 mL (i.e. 1 cc) syringe. Typically, 200 μ L to 600 μ L of the fluid, such as a therapeutic, is delivered to the target locus, and the volume of syringe barrel is 1 mL.

[0182] The syringe barrel **91'** is positioned on the distal side of the needle sheath controller **71'**. As shown in **FIG. 2**, the syringe barrel **91'** is integrated and contained within the distal most lumen end of the needle sheath **72'**. Thus, the syringe barrel is enclosed by the needle sheath **72'**. As shown in **FIG. 10A** and **10B**, described in more detail below, the syringe barrel **91'** is not directly connected to the lumen **723** of the sheath cavity, but is positioned so that it is immovable in relation to the needle sheath controller **71'**. Thus, in this embodiment, the syringe barrel **91'** is not removable from the needle sheath **72'**.

[0183] The needle sheath **72'** can be opaque or can be transparent or clear. Generally, the needle sheath **72'** is opaque, but contains a visibility window **725** for visualization of the integrated syringe barrel **91'**. Since device **60'** contains a syringe barrel **91'** that is enclosed within the needle sheath **72'**, and that would not otherwise be visible, the presence of the visibility window **725** permits visualization of the graduated markings on the syringe barrel to aid in drawing up agents or solutions. In addition to permitting visualization of the administered agent or solutions, the presence of the visibility window **725** allows visualization of drawback fluids. For example, since some applications require injection directly into the parenchyma, and not into a vessel or bile duct, the ability to drawback and visualize fluid from the area the needle has penetrated can be used to confirm needle placement into the parenchyma, while avoiding injections into the vasculature or bile ducts. The visibility window **725** can be made of glass or clear plastic such as polycarbonate. The visibility window **725** is integrated directly into the body of the needle sheath **72'**. The visibility window can surround the entire circumference of the needle sheath **72'** or can partially surround the circumference of needle sheath **72'**. The visibility window **725** can be any desired length, and located anywhere along the needle sheath

72' so long as a portion of the syringe barrel 91' is exposed under the visibility window 725. Generally, the visibility window 725 exposes the distal portion of the syringe barrel 91', but can expose the entire syringe barrel 91'. The visibility window 725 can be 10 cm to 300 mm, and generally is 20 mm to 100 mm in length.

[0184] The plunger 92' is located on the proximal end of the device 60' and passes through the needle sheath controller 71' and the needle sheath 72' where it can engage with and pass into the syringe barrel 91'. The plunger 92' is movable through the needle sheath controller 71', needle sheath 72' and syringe barrel 91' so that it can be pulled and pushed along inside the syringe barrel 91'. The plunger 92' can be drawn back to load the syringe barrel 91' with the fluid, such as a therapeutic, or depressed to inject the fluid, such as a therapeutic, in the target tissue. The plunger 92' also can be pulled back at the site of injection to test needle placement. The plunger is cylindrical to move through the syringe barrel 91', and is made of material that permits ease of movement through the needle sheath controller 71', needle sheath 72' and syringe barrel 91'. Typically, the plunger 92' is made of plastic, for example polypropylene or polyethylene. The plunger contains a head 95 at the proximal end of the device that can be conveniently grasped by the operator to manipulate the plunger. The plunger head 95 also is generally made of plastic. The distal tip of the plunger 92' is generally made of silicone or other natural or synthetic rubber to provide a tight seal within the syringe barrel 91' when traveling within the syringe barrel 91'.

[0185] The plunger 92' is long enough in length to permit its association with the inside of the syringe barrel 91' in order to dispel the fluid, such as a therapeutic through the distal end of the syringe and into the needle 81 connected thereto. Since the plunger essentially extends the length of the device, the plunger is generally at least as long as the sheath, and generally longer since it extends outside of the laparoscopic port. For example, the plunger 92' can be 200 mm to 800 mm, such as 300 to 600 mm, and generally at least or about at least or 300 to 400 mm. Pulling back on the plunger 92' draws in the fluid, such as a therapeutic, or air, and pushing the plunger 92' forces the fluid, such as a therapeutic, or air out of the syringe barrel.

[0186] The device 60' contains an injection needle 81 that is located inside the needle sheath 72' that can be sheathed and unsheathed at the distal tip of the needle 81. With reference to FIG. 10A, described in more detail below, the distal tip of the needle sheath 73 contains a needle channel 733 that guides the needle outside of the needle sheath 72' when it is unsheathed as shown in FIG. 2. As shown in FIG. 2, the injection needle contains a beveled tip sufficient to penetrate or pierce a tissue or an organ.

[0187] As discussed further below, because the injection needle 81 is directly attached to the syringe barrel 91' at the distal end of the device, the injection needle is

relatively short. This avoids problems in pressure drop that can occur with longer needles. This also means that the dead volume in the device 60', which is the volume of fluid that is loaded into the syringe barrel 91', but cannot be expelled from the device and injected into the tissue, is generally small. Since therapeutics are often costly or limited, an injection device that minimizes amount of dead volume is advantageous. Factors that influence the amount of dead volume include the length of the needle, the diameter of the needle, and the diameter of the syringe barrel. In case of a long needle, the amount of air in the needle often is not tolerable in the patient and the target tissue and/or organ. Hence, the air needs to be removed from the needle and the needle is sometimes "primed." After the injection, the amount of fluid remaining in the fluid path between the tip of the plunger and the tip of the injection needle 81 cannot be expelled completely, and thus results in dead volume. In case of a long needle, the amount of dead volume is thus larger. In device 60', the syringe barrel 91' is located close to the tip of the needle sheath 72', and the dead volume occurs only in the tip of the syringe barrel 91' and the injection needle 81.

[0188] FIG. 6 depicts an enlarged cross section view of the needle sheath controller 71' and the plunger 92' extended through the needle sheath controller 71'. The needle sheath controller 71' is positioned on the proximal side of the needle sheath 72'. The needle sheath controller 71' contains the components that control movement of the needle sheath 72', connect the proximal and distal end of the device, and is the conduit by which the plunger 92' travels between the proximal and distal ends of the device. The needle sheath controller 71' is configured to be held and manipulated by an operator, such as a surgeon. As discussed above, the needle sheath controller 71' can be any shape and size that is convenient to permit the operator to hold and manipulate the device, and typically is cylindrical in shape. The diameter of the needle sheath controller 71' is such that it can be held in the palm of an average adult, and is generally 20 mm to 100 mm in diameter with a length of 50 mm to 225 mm. The needle sheath controller optionally can contain an outside grip for handling.

[0189] As shown in FIG. 2 and FIG. 6, the needle sheath controller 71' includes a controller housing 710 that encloses components internal to the needle sheath controller 71', and the proximal end of the needle sheath 72'. As discussed above, the needle sheath controller housing 710 can be made of any suitably resilient and rigid material, such as any polymeric material, including plastics, or rubber, metals, ceramics, composites, or other suitable material known to one of skill in the art. The controller housing 710 is typically made of polypropylene, polystyrene, polyethylene, polyvinyl chloride, polyurethane, silicone, rubber or acrylic. As discussed above, the housing 710 can be made by any manufacturing known to a skilled artisan, and can be made as one singular piece or can be made of two or more pieces that

are attached together, such as with adhesive, locking joints or fasteners.

[0190] As shown in **FIG. 2** and **FIG. 6**, the needle sheath controller **71'** contains an externally accessible positioner **711**. As described above, the positioner **711** is configured in the needle sheath controller **71'** so that it is movable both forward and rearward relative to the needle sheath controller **71'**. As described above, the positioner **711** is engaged with the needle sheath **72'** through a connection member **713**, and can be used to slide the needle sheath **72'**. This connection permits movement of the positioner **711** between the forward or rearward positions to control movement of the needle sheath between two fixed or locked positions, the sheathed and unsheathed positions. The sheathed position protects or hides the injection needle, while the unsheathed position exposes the needle.

[0191] With reference to **FIG. 6**, the connection member **713** is connected to the proximal end of the needle sheath **72'**, and the lower part of the positioner **711**. The connection of the connection member **713** with the proximal end of the needle sheath is such that the needle sheath **72'** is longitudinally movable relative to the controller housing **710** and the injection needle **81**. For example, the distal end of the outside of the connection member **713** is engaged with the proximal inside cavity of the needle sheath **72'** around its circumference. The connections of the control member with the positioner **711** and needle sheath **72'** can be by welding, adhesive, locking joints, fasteners or other suitable means.

[0192] As described above generally, the connection member **713** moves inside a hollow cavity or lumen **717** contained inside the housing **710** of the needle sheath controller **71'** that is closed at both ends relative to the housing **710**. The controller lumen **717** accommodates the connection member **713** such that the connection member **713** can easily glide or move forward or rearward in a restricted manner. For example, the connection member **713** can be cylindrical and fit inside a cylindrical hollow lumen cavity **717**. As shown in **FIG. 6**, and discussed further below, the connection member **713** contains an internal hollow cavity sized to fit the plunger **92'** that passes through.

[0193] Movement of the connection member **713** is controlled by the positioner **711**. As shown in **FIGS. 2** and **6**, the positioner **711** contains a projected top portion or head that juts out of the needle sheath controller **71'** where it can be moved forward or rearward by the operator. As shown in **FIG. 6**, internal to the needle sheath controller **71'**, the body of the positioner **711** is notched on its sides or is otherwise configured to engage with sheath stops **715** or **716**. Sheath stops **715** and **716** are grooves in the needle sheath controller housing **710** that fit the notched body of the positioner and trap the positioner **711** so that it cannot be moved.

[0194] As exemplified in **FIG. 5** with the exemplary device **60**, device **60'** also contains an optional lock and release element **712** configured in the positioner **711** to

facilitate lock and release of the positioner with the grooves of the sheath stop **715** or **716**. For example, the lock and release element **712** can be a spring or other resilient means. The mechanism controlling lock and release of the positioner **711** with the grooves of the sheath stop **715** or **716** by the lock and release element **712** is as described above, whereby downward, vertical or lateral forces release or lock the positioner **711** from the sheath stops **715** or **716**. Pushing downward on the positioner **711** permits the positioner to slide and to fit it into either of sheath stops **715** or **716**.

[0195] Movement of the positioner **711** between the sheath stops **715** and **716** moves the connection member **713**, and thereby also moves the needle sheath **72'** so that it can transition from the sheathed and unsheathed positions by control of the positioner by the operator. When the positioner is in the rearward position **711c** as exemplified in **FIG. 6**, distal sheath stop **715** is free and the positioner **711** is fit into the proximal sheath stop **716**, thereby unsheathing the injection needle so that it is exposed. While not shown in **FIG. 6**, the positioner **711** also can be in the forward position **711a** as exemplified in **FIG. 5**, where the proximal sheath stop **716** is free and the positioner **711** is fit into the distal sheath stop **715**, thereby sheathing the injection needle so that it is protected. As a further position, the positioner **711** also can be in an intermediate position **711b** as exemplified in **FIG. 7**, where both the distal sheath stop **715** and the proximal sheath stop **716** are free and not engaged with the positioner **711**.

[0196] As shown in **FIG. 6**, the plunger **92'** passes through the inside lumen **717** of the needle sheath controller **71'** and passes through a central cavity of the connection member **713**, but is not directly attached to the needle sheath controller **71'** or connection member **713**. Hence, the connection member **713** can move independently around the plunger **92'**, and the plunger **92'** can move independently through the connection member **713**. As discussed above, because the needle sheath **72'** is directly connected to the connection member **713** contained in the controller lumen **717**, the plunger **92'** enters the inside cavity of the needle sheath **72'** inside the needle sheath controller **71'**. The plunger **92'** exists the distal end of the needle sheath controller **71'** where it is contained within the lumen **723** of the needle sheath **72'**.

[0197] With reference to **FIG. 10A** and **10B**, the plunger **92'** runs distally and longitudinally through the needle sheath **72'** where it engages with the proximal end of the syringe barrel **91'**. The injection needle **81** is directly connected to the inside of the syringe barrel **91'** at the distal end of the syringe barrel **91'**. The injection needle **81** contains a beveled tip sufficient to penetrate or pierce a tissue or an organ. The injection needle **81** is typically made of metal or alloy, such as surgical stainless steel or other medical grade metal. The size and diameter of the injection needle **81** is selected based on parameters generally describe above. As described above, typically

a small diameter needle **81** is employed to reduce the force required to insert the needle into the target tissue or organ, and to reduce trauma to the target tissue or organ. For example, the injection needle **81** is between 25 and 34 gauge, such as a 25 gauge, 26 gauge, 27 gauge, 28 gauge, 29 gauge, 30 gauge or 31 gauge needle, and typically is 27 gauge.

[0198] At the distal end of the device **60'**, the needle sheath **72'** ends in a distal tip **73** that contains a needle channel **733**. The needle channel **733** is sufficiently sized to fit the injection needle **81** so the injection needle can extend and retract through the needle channel **733** as the needle sheath **72'** moves. In **FIG. 10A**, the injection needle **81** is covered by the needle sheath **72'** and does not traverse through needle channel **733**. With reference to **FIG. 4A**, the device **60'** in **FIG. 10A** is in the sheathed position **72a**. In **FIG. 10B**, the injection needle **81** is extended out of the needle sheath **72'** and does traverse through needle channel **733**. With reference to **FIG. 4C**, the device **60'** in **FIG. 10B** is in the unsheathed position **72c**.

[0199] As shown in **FIGS. 10A** and **10B**, because the syringe barrel **91'** is not connected to the needle sheath **72'**, the needle sheath **72'** moves independently around the syringe **91'**. In the unsheathed position, the needle sheath **72'** is pulled back, but the syringe barrel **91'** and injection needle **81** are fixed and do not move. For example, as shown in **FIG. 10B**, because the needle sheath **72'** is pulled back, the size of the sheath lumen **723** is shortened compared to **FIG. 10A** when the needle sheath **72'** is not pulled back. In the unsheathed position shown in **FIG. 10B**, the distal end of the syringe barrel **91'** touches the distal tip of the sheath **73**. A notch can be configured in the distal tip **73** in order to accommodate the syringe barrel **91'** as it is positioned in the unsheathed position **72c**. This demonstrates that movement of the sheath, as described with reference to **FIG. 6** above using the positioner **711**, only controls the movement of the needle sheath **72'**, while the position of the syringe barrel **91'** and injection needle **81** of the device are stationary regardless of the position of the positioner **711**.

[0200] As described above, in the unsheathed position, the extent by which the injection needle **81** is extended or exposed out of the device **60'** is a function of the distance between the sheath stops **715** and **716** as shown in **FIG. 6**. This distance is a function of the particular application of the device, the particular target tissue, the subject being treated and other considerations. For example, unsheathed needle that is exposed should not be so long that it can easily penetrate through to the other side of a target tissue. Generally, with reference to most target tissues (e.g. liver), the portion of the injection needle **81** shown in **FIG. 10B** that can be unsheathed or exposed is generally less than 1 cm, such as 2 mm to 10 mm, and generally no more than 5 mm. For a child, the length can be smaller, and is generally less than 4 mm. For applications *in utero*, the length can be 2 mm to 3 mm. Generally, the total length of the injection needle **81**

in device **60'** is slightly longer than the unsheathed needle tip that extends out of the device. As shown in **FIG. 10B**, the extent of the extra length is sufficient to account for the distance of the distal sheath tip **73** and the extent to which the proximal end of the needle is connected to syringe barrel **91'**. For example, the total length of the injection needle **81** can range from 5 mm to 40 mm, such as 10 mm to 40 mm, such as a 12.7 mm, 25.4 mm or 38.1 mm needle.

[0201] **FIG. 10C** provides a corresponding perspective view of the needle sheath shown in **FIG. 10A** in the sheathed position **72a**. **FIG. 10D** provides a corresponding perspective view of the needle sheath shown in **FIG. 10B** in the unsheathed position **72c**. In **FIG. 10A** and **D**, the needle sheath **72'** is opaque, but contains a visibility window **725** in order to view the syringe barrel **91'** and injection needle **81** whether sheathed or unsheathed.

[0202] The device **60'** can be disposable or reusable. For example, the device **60'** can be withdrawn from the laparoscopic port and disposed of, or reloaded and reused. The device **60'** also can be a sterile device. For example, the device **60'** can be loaded through the injection needle **81** in a sterile environment, such as a sterile operating room. The device **60'** can be pre-loaded with the fluid, such as a therapeutic, and provided as a sterile pre-loaded syringe. Furthermore, distribution of sterile disposable pre-loaded devices is easily achieved using this device **60'** due to the complete integration of the syringe barrel into the needle shaft, thereby minimizing contamination that can occur when the syringe barrel and device must be packaged or stored separately. Alternatively, the injection needle **81** can be inserted into a container with the fluid, such as a therapeutic, composition, and the plunger **92'** can be pulled back to load the fluid, such as a therapeutic, in the syringe barrel **91'**.

[0203] With reference to the above Figures and description, exemplary of the mode of operation of the injection device **60'** involves first loading the device **60'** with a fluid, such as a therapeutic. With the needle sheath **72'** in the unsheathed position **72c**, the injection needle **81** can be inserted into a vial or a container of fluid, such as a therapeutic, and the integrated syringe plunger **92'** can be pulled back to load the syringe with the fluid, such as a therapeutic. Optionally, a vial adaptor can be used when loading the syringe with the therapeutic compound, such that the long device can be stabilized over a vial or container of fluid, such as a therapeutic, loading the syringe barrel **92'**. Once the syringe is loaded, the needle sheath **72'** can be positioned in the sheathed position **72a**, and the device can be inserted into a laparoscopic port to place the device near the site of injection. At the site of injection (target tissue), the needle sheath **72'** can be unsheathed **72c**, and the injection needle **81** can be exposed for injection. If necessary, the integrated syringe plunger **92'** can be pulled back to draw fluids from the site of injection, to test the placement of the injection needle **81** at the injection site. The syringe visibility window **725** can be used to visualize the drawback and the move-

ment of the plunger **92'**. Once the site of needle placement is determined, the plunger **92'** can be depressed, to inject the fluid, such as a therapeutic, at the target tissue. After injection, the needle sheath **72'** can be positioned in the sheathed position **72a**, to protect the non-target organs and prevent accidental needle puncture, prior to removing the laparoscopic device from the injection site and through the laparoscopic port.

3. DOCKABLE INJECTION DEVICE

[0204] FIGS. 3, 7 and 11A-D depict the injection device **60"** and components and features thereof. The injection device as shown in FIG. 3 includes needle sheath **72"**, needle sheath controller **71'**, plunger **92"** and a dockable syringe **910** containing injection needle **81**, syringe barrel **91"**, and associated auxiliary plunger **920**. The needle sheath **72"** of the injection device is of a sufficient length to permit laparoscopic access to the target of interest, and is generally a length of 200 mm to 600 mm, such as 250 to 400 mm, and generally at least or about at least or 300 mm. The device is generally cylindrical around the longitudinal axis, generally having a smaller diameter in the needle sheath region **72"** and the plunger region **92"** and a larger diameter in the needle controller region **71'**. The needle sheath **72"** of the device is typically inserted through the port (e.g. laparoscopic port). The diameter of the needle sheath **72"** is typically between 3 mm to 12 mm in size, and typically from 5 mm to 10 mm. It is understood that portions of the device external to the laparoscopic port can have a diameter greater than 10 mm. For example, the needle sheath controller body **71'** can have a diameter sufficiently large, so long as it can be easily gripped or handled by the operator. The needle sheath controller body **71'** is held by the operator, typically a surgeon, to manipulate and position the device **60"**, control the needle sheath **72"** and support the device while manipulating the plunger **92"**.

[0205] Injection device **60"** is adapted so that a dockable syringe **910** containing injection needle **81**, syringe barrel **91"** and associated auxiliary plunger **920** can be temporarily docked therewith. As shown in FIG. 3, the syringe barrel **91"** is cylindrical in shape with a hollow center that can fit auxiliary plunger **920** so that the plunger can move back and forth inside the syringe barrel. The auxiliary plunger **920** is located on the proximal side of the syringe barrel **91"** and is movable so that it can be pulled and pushed along inside of the syringe barrel **91"**. The auxiliary plunger **920** can be drawn back to load the syringe barrel **91"** with the fluid, such as a therapeutic, or depressed to dispel or inject the fluid in the target tissue. The auxiliary plunger **920** can also be pulled back at the site of injection to test needle placement. As discussed below, movement of the auxiliary plunger **920** when docked in the device is controlled by the plunger **92"**. The auxiliary plunger **920** is cylindrical to move through the syringe barrel **91"**, and is made of material that permits ease of movement through the syringe bar-

rel, such as a plastic, for example, polypropylene or polyethylene.

[0206] The auxiliary plunger **920** contains a plunger head **95** at the proximal end of the plunger that can be conveniently grasped by the operator to manipulate the plunger, or otherwise configured to control movement of auxiliary plunger **920**. For example, the auxiliary plunger **920** can be independently moved and controlled, for example, when the dockable syringe **910** is in the undocked position (discussed further below). In other instances, when the dockable syringe **910** is docked in device **60"**, movement of the auxiliary plunger **920** is controlled by plunger **92"** at the proximal end of device **60"** through a plunger adaptor **951** (discussed further below). The plunger head **95** also is generally made of plastic. The distal tip of the auxiliary plunger **920** is generally made of silicone or other natural or synthetic rubber to provide a tight seal within the syringe barrel **91"** when traveling within the syringe barrel **91"**.

[0207] The auxiliary plunger **920** is long enough in length to permit its association with the inside of syringe barrel **91"** in order to dispel the fluid, such as a therapeutic, through the distal end of the syringe barrel **91"** and into injection needle **81** connected thereto. For example, the auxiliary plunger **920** can have a length between 50 mm and 100 mm, typically 70 mm to 90 mm. Pulling back on the auxiliary plunger **920** draws in the fluid or air, and pushing the auxiliary plunger **920** forces the fluid or air out of the syringe barrel.

[0208] The syringe barrel **91"** is generally clear and transparent. The syringe barrel **91"** can be made out of plastic or glass or other suitable material, and in particular is made out of plastic such as polypropylene, polyethylene, polycarbonate or other clear material. As described above, the syringe barrel **91"** can contain calibrations or marking on the outer surface to indicate the volume of the agent within the barrel. As described above, the syringe barrel **91"** can have a volume capacity that is from the range of 0.5 mL to 20 mL (i.e. 0.5 cc to 20 cc), and generally is 0.5 mL to 3 mL (i.e. 0.5 cc to 3 cc), such as at least or about a 1 mL (i.e. 1 cc) syringe. Typically, 200 μ L to 600 μ L of the fluid, such as a therapeutic, is delivered to the target locus, and the volume of syringe barrel is 1 mL.

[0209] The dockable syringe **910** of device **60"** contains an injection needle **81** that is located on the distal end of the syringe barrel **91"**, and hence the distal end of the device **60"** when the dockable syringe **910** is docked into device **60"** (discussed further below). The injection needle **81** can be connected directly or indirectly to syringe barrel **91"**. For example, the injection needle **81** can be directly affixed, such as by an adhesive, bonding or molding, to the inside of syringe barrel **91"** at the distal end of syringe barrel **91"**. In other examples, the distal end of syringe barrel **91"** can contain a Luer fit or other adaptor that is compatible with a hub on the proximal end of injection needle **81**.

[0210] As shown FIG. 3, the injection needle contains

a beveled tip sufficient to penetrate or pierce a tissue or an organ. The injection needle **81** is typically made of metal or alloy, such as surgical stainless steel or other medical grade metal. The size and diameter of the injection needle **81** is selected based on parameters generally describe above. As described above, typically a small diameter needle **81** is employed to reduce the force required to insert the needle into the target tissue or organ, and to reduce trauma to the target tissue or organ. For example, the injection needle **81** is between 25 and 34 gauge, such as a 25 gauge, 26 gauge, 27 gauge, 28 gauge, 29 gauge, 30 gauge or 31 gauge needle, and typically is 27 gauge.

[0211] Because the injection needle **81** is directly attached to the syringe barrel **91''**, the injection needle is relatively short. This avoids problems in pressure drop that can occur with longer needles. Similar to device **60'** discussed above, this also means that there is generally a small dead volume created by device **60''**. For example, the total length of the injection needle **81** can range from 5 mm to 40 mm, such as 10 mm to 40 mm, such as a 12.7 mm, 25.4 mm or 38.1 mm needle. Generally, the use of shorter needle is desired in order to avoid problems related to dead volume and pressure drops.

[0212] The needle sheath **72''** can be opaque or can be transparent or clear. The needle sheath **72''** is generally solid at the proximal portion of the needle sheath **720**, but contains an open cavity **726** at its distal portion. The dockable syringe **910** containing auxiliary plunger **920**, syringe barrel **91''** and injection needle **81** is configured so that it can be docked and undocked in the open cavity of the sheath, and in a manner in which the needle sheath **72''** is movable around the dockable syringe **910**. As shown in **FIG. 3** and **FIG. 11A**, the open cavity **726** is a cut out in the top half of the needle sheath **72''**. The inner side of the open cavity **726** of the sheath can be lined with a syringe adaptor lining **96** in a manner so that the sheath moves independently from the syringe adaptor lining **96**. The syringe adaptor lining **96** also has an open cavity of substantially similar size.

[0213] For example, as shown in **FIGS. 11A** and **11B**, a syringe adaptor lining **96** can run through the sheath, such that the sheath moves independently around the syringe adaptor lining **96**. The syringe adaptor lining **96** can be connected or fixed at its proximal end to the needle sheath controller **71'** and have an open cavity at its distal end to form a nest for the dockable syringe. For example, the syringe adaptor lining **96** can be a hypodermic tubing that has a distal section removed to form a nest for the dockable syringe. The tubing can have a diameter smaller than the inside portion of the needle sheath **72''** so that the tubing can run into and through the sheath where it can be connected to the needle sheath controller **71'** in a fixed position.

[0214] The open cavity of the syringe adaptor lining **96** can contain a plunger rest cavity **960**, a barrel rest cavity **962**, and two barrel docks **961** and **963**. The barrel rest cavity **962** is flanked by two barrel docks **961** and **963**,

which are clasps or fitting that are adapted to seat or secure the syringe barrel **91''** at its proximal and distal end, respectively. The size of the barrel rest cavity **962** and the distance between the two barrel docks **961** and **963** permit engagement with the syringe barrel **91''**. If the syringe barrel **91''** contains grooves to fit into the barrel docks **961** and **963**, the length between the two barrel docks **961** and **963** is the same as the length between the corresponding grooves in the syringe barrel **91''**. The portion of the syringe barrel **91''** that can dock with barrel docks **961** and **963** can be restricted by configuring syringe barrel **91''** with narrow grooves at its proximal and distal ends that fit dock **961** and **963**, respectively. This ensures that the syringe barrel **91''**, when fitted in the open cavity **726**, is properly lined up for sheathing and unsheathing injection needle **81**.

[0215] The barrel docks **961** and **963** can be similarly sized, or can be different sizes depending on the particular size and configuration of syringe barrel **91''**. The barrel docks **961** or **963** can be rigid or flexible, and can be made out of metal or polymeric materials such as plastics. The barrel docks **961** and **963** can be features extruding from the syringe adaptor lining **96**, or can be separate parts that are attached to the exposed part of the syringe adaptor lining **96**. The barrel rest cavity **962** and the docks **961** and **963** are not directly connected to the needle sheath so that the needle sheath **72''** moves around and independently from the syringe adaptor lining **96**, including the barrel rest cavity and docks.

[0216] A plunger adaptor **951** that is part of the distal end of plunger **92''** is located at the proximal end of the cavity **726**. The plunger adaptor **951** rests inside open cavity of the syringe adaptor lining **96** when the plunger **92''** is pulled back in an extended position. As discussed below, the plunger **92''** is movable within the lumen of the syringe adaptor lining **96** in order to control movement of auxiliary plunger **920**. The distance between barrel dock **961** and plunger adaptor **951** when the plunger **92''** is in its extended position (i.e. pulled out to maximum length outside of syringe barrel) creates a plunger rest cavity **960** within the syringe adaptor lining **96** sufficiently sized to fit the auxiliary plunger **920** in its extended position.

[0217] Hence, the length of the open cavity **726** of the needle sheath **72''** and the open cavity of the syringe adaptor lining **96** is sufficient to fit dockable syringe **910**. In some instances, the cavity can span the entire length of the needle sheath **72''**, except for the distal tip of the needle sheath **73'** discussed below. Typically, the open cavity **726** is 50 mm to 250 mm in length. Accordingly, the open cavity of the syringe adaptor lining **96**, which has a substantially similar length to the open cavity **726** of the needle sheath, is 50 mm to 250 mm in length. The length of the open cavities also depends on the diameter of the needle sheath **72''**, the volume, length and diameter of the dockable syringe **910**. If a larger volume of syringe barrel **91''** is needed for a specific injection, the length of the syringe barrel **91''** and the open cavities can

be made larger. However, the stroke length of the auxiliary plunger **920** is limited to less than half of the entire length of the needle sheath **72"**, as both the fully extended auxiliary plunger **920** and the syringe barrel **91"** must fit in the length of the needle sheath **72"** and the open cavities. The stroke length of the plunger **92"** is also limited to the maximum stroke length of the auxiliary plunger **920**. Hence, if a larger volume of syringe barrel **91"** is needed, the diameter of the needle sheath **72"** can be larger. The optimal length and diameter of the syringe barrel **91"** in relation to the stroke length and the length of the needle sheath **72"**, including the length of the proximal portion of the needle sheath **720**, can be empirically determined based on the diameter of the laparoscopic ports, type of surgery, and the volume of syringe barrel required.

[0218] The open cavities terminate at the distal tip of the needle sheath **73'**. The distal tip of the needle sheath **73'** is solid, except that it contains an open needle groove **76** on its top side. The needle groove **76** is a narrow opening sufficient for injection needle **81** to drop into the distal tip of needle sheath **73'** where it can line up with needle channel **733** to guide the injection needle **81** outside when unsheathed. The length and diameter of the groove **76** is sufficient to fit injection needle **81**. For example, the needle groove **76** is 5 mm to 40 mm long, such as 10 mm to 40 mm. The width of the needle groove is 0.2 to 2 mm, such as 0.3 to 1 mm.

[0219] **FIGS. 11A** and **11B** depict the dockable and undocked configurations of dockable syringe **910** with the syringe adaptor lining **96** and the needle sheath **72"**. For example, **FIG. 11A** shows the dockable syringe **910** in the undocked position **910a**. As shown in **FIG. 11A**, a syringe adaptor lining **96** is inside the needle sheath **72"**. An open cavity of the syringe adaptor lining **96** configured into the open cavity **726** of the needle sheath **72"** is configured to fit the dockable syringe **910** as described above. **FIG. 11B** shows the dockable syringe **910** in the docked position **910b**. In the docked position **910b**, the dockable syringe **910** is positioned on the distal side of the needle sheath controller **71'**. When in the docked position **910b**, the injection needle **81** is located inside the needle sheath **72"** and can be sheathed and unsheathed at the distal tip of the needle **81** as discussed below.

[0220] The ability to dock into syringe dock accessible by the open cavity **726** of the needle sheath **72"** and the open cavity of the syringe adaptor lining **96** permits visualization of the syringe barrel in device **60"** so that the administered agent or drawback fluids can be visualized. For example, as discussed above, since some applications require injection directly into the parenchyma, and not into a vessel or bile duct, the ability to drawback and visualize fluid from the area the needle has penetrated can be used to confirm needle placement into the parenchyma, while avoiding injections into the vasculature or bile ducts.

[0221] In addition, the ability to remove or dock the

syringe **910** in injection device **60"** also provides advantages, including the ease of loading the syringe barrel, exchange of loaded syringe, and sterility of syringe. For example, a sterile syringe barrel **91"** can conveniently be used when drawing up or loading the syringe with a fluid, such as a therapeutic, compositions or other solutions into the syringe barrel. If desired, a separately sterile needle **81** can be fitted to the syringe barrel **91"**, such as by a Luer fit adaptor, to permit loading of the syringe barrel **91"** with a fluid, such as a therapeutic. Syringe barrel **91"** also can be separately loaded prior to use of device **60"**, or a pre-loaded syringe barrel **91"** can be used. Also, a variety of syringe types and sizes can be used so long as they are dockable with the device **60"**. In some cases, several different types of syringes can be used for one patient, if necessary. In cases where the syringe must be re-loaded or additional fluid, such as a therapeutic, is needed, new or re-loaded syringes can be docked.

[0222] As shown in **FIG. 3**, plunger **92"** is located on the proximal end of the device **60"** where it can be controlled and operated by the operator outside of the laparoscopic port. Plunger **92"** passes through the needle sheath controller **71'** and the proximal portion of the needle sheath **72"**. The plunger **92"** is generally cylindrical and movable within needle sheath controller **71'** and needle sheath **72"**. The plunger **92"** is made of material that permits ease of movement through the needle sheath controller **71'** and needle sheath **72"**. Typically, the plunger **92"** is made of plastic, for example polypropylene or polyethylene. The distal end of the plunger **92"** contains a plunger adaptor **951** that is exposed through open cavity **726** in the needle sheath **72"** where it associates with auxiliary plunger **920**. The plunger **92"** is long enough in length to permits its association with auxiliary plunger **920** in needle sheath **72"** when auxiliary plunger **920** is docked in cavity **726**. For example, the length of plunger **92"** can range from 50 mm to 500 mm, such as 100 mm to 400 mm or 100 mm to 200 mm. Plunger **92"** is generally longer than auxiliary plunger **920**.

[0223] The plunger adaptor **951** contains a groove or notch to connect with auxiliary plunger **920** through plunger head **95'** of auxiliary plunger **920**. The plunger adaptor **951** is of a sufficient size and shape so that plunger head **95'** of auxiliary plunger **920** can be seated or secured in the plunger rest cavity **960**. As shown in **FIG. 11B**, when plunger head **95'** of auxiliary plunger **920** is fitted or secured in plunger adaptor **951**, the auxiliary plunger **920** and the plunger **92"** are connected, such that movement of the plunger **92"** controls movement of auxiliary plunger **920**. The plunger **92"** also contains a plunger head **95** at the proximal end of the device that can be conveniently grasped by the operator to manipulate plunger **92"**, and thus also auxiliary plunger **920**. For example, pushing the plunger **92"** also pushes the auxiliary plunger **920** and forces the fluid or air out of the syringe barrel **91"**.

[0224] **FIG. 7** depicts an enlarged cross section view

of the needle sheath controller 71' and the plunger 92" extended through the needle sheath controller 71'. The needle sheath controller 71' is positioned on the proximal side of the needle sheath 72". The needle sheath controller 71' contains the components that control movement of the needle sheath 72", connect the proximal and distal end of the device, and is the conduit by which the plunger 92" travels between the proximal and distal ends of the device. The needle sheath controller 71' is configured to be held and manipulated by an operator, such as a surgeon. As discussed above, the needle sheath controller 71' can be any shape and size that is convenient to permit the operator to hold and manipulate the device, and typically is cylindrical in shape. The diameter of the needle sheath controller 71' is such that it can be held in the palm of an average adult, and is generally 20 mm to 100 mm in diameter with a length of 50 mm to 225 mm. The needle sheath controller optionally can contain an outside grip for handling.

[0225] As shown in FIG. 3 and FIG. 7, the needle sheath controller 71' includes a controller housing 710 that encloses components internal to the needle sheath controller 71', and the proximal end of the needle sheath 72". As discussed above, the needle sheath controller housing 710 can be made of any suitably resilient and rigid material, such as any polymeric material, including plastics, or rubber, metals, ceramics, composites, or other suitable material known to one of skill in the art. The controller housing 710 is typically made of polypropylene, polystyrene, polyethylene, polyvinyl chloride, polyurethane, silicone, rubber or acrylic. As discussed above, the housing 710 can be made by any manufacturing known to a skilled artisan, and can be made as one singular piece or can be made of two or more pieces that are attached together, such as with adhesive, locking joints or fasteners.

[0226] As shown in FIG. 3 and FIG. 7, the needle sheath controller 71' contains an externally accessible positioner 711. As described above, the positioner 711 is configured in the needle sheath controller 71' so that it is movable both forward and rearward relative to the needle sheath controller 71'. As described above, the positioner 711 is engaged with the needle sheath 72" through a connection member 713, and can be used to slide the needle sheath 72". This connection permits movement of the positioner 711 between the forward or rearward positions to control movement of the needle sheath 72" between two fixed or locked positions, the sheathed and unsheathed positions. The sheathed position protects or hides the injection needle, while the unsheathed position exposes the needle.

[0227] With reference to FIG. 7, the connection member 713 is connected to the proximal end of the needle sheath 72", and the lower part of the positioner 711. The connection of the connection member 713 with the proximal end of the needle sheath is such that the needle sheath 72" is longitudinally movable relative to the controller housing 710 and the injection needle 81. For ex-

ample, the distal end of the outside of the connection member 713 is engaged with the proximal inside lumen 723 of the needle sheath 72" around its circumference. The connections of the control member with the positioner 711 and needle sheath 72" can be by welding, adhesive, locking joints, fasteners or other suitable means.

[0228] As described above generally, the connection member 713 moves inside a hollow cavity or lumen 717 contained inside the housing 710 of the needle sheath controller 71' that is closed at both ends relative to the housing 710. The controller lumen 717 accommodates the connection member 713 such that the connection member 713 can easily glide or move forward or rearward in a restricted manner. For example, the connection member 713 can be cylindrical and fit inside a cylindrical hollow lumen cavity 717. As shown in FIG. 7, and discussed further below, the connection member 713 contains an internal hollow cavity sized to fit the plunger 92" that passes through.

[0229] Movement of the connection member 713 is controlled by the positioner 711. As shown in FIGS. 3 and 7, the positioner 711 contains a projected top portion or head that juts out of the needle sheath controller 71' where it can be moved forward or rearward by the operator. As shown in FIG. 7, internal to the needle sheath controller 71', the body of the positioner 711 is notched on its sides or is otherwise configured to engage with sheath stops 715 or 716. Sheath stops 715 and 716 are grooves in the needle sheath controller housing 710 that fit the notched body of the positioner and trap the positioner 711 so that it cannot be moved.

[0230] As exemplified in FIG. 5 with the exemplary device 60, device 60" also contains an optional lock and release element 712 configured in the positioner 711 to facilitate lock and release of the positioner with the grooves of the sheath stops 715 or 716. For example, the lock and release element 712 can be a spring or other resilient means. The mechanism controlling lock and release of the positioner 711 with the grooves of the sheath stops 715 or 716 by the lock and release element 712 is as described above, whereby downward, vertical or lateral forces release or lock the positioner 711 from the sheath stops 715 or 716. Pushing downward on the positioner 711 permits the positioner to slide and to fit it into either of sheath stops 715 or 716.

[0231] Movement of the positioner 711 between the sheath stops 715 and 716 moves the connection member 713, and thereby also moves the needle sheath 72" so that it can transition from the sheathed and unsheathed positions by control of the positioner by the operator. When the positioner is in the intermediate position as exemplified in FIG. 7, both distal sheath stop 715 and the proximal sheath stop 716 are free and not engaged with the positioner 711. While not shown in FIG. 7, the positioner 711 also can be in the forward position 711a as exemplified in FIG. 5, where the proximal sheath stop 716 is free and the positioner 711 is fit into the distal sheath stop 715, thereby sheathing the injection needle

so that it is protected. As a further position, while not shown in FIG. 7, the positioner also can be in the rearward position 711c as shown in FIG. 6, where distal sheath stop 715 is free and the positioner 711 is fit into the proximal sheath stop 716, thereby unsheathing the injection needle so that it is exposed.

[0232] As shown in FIG. 7, the plunger 92" passes through the inside lumen 717 of the needle sheath controller 71' and passes through a central cavity of the connection member 713, but is not directly attached to the needle sheath controller 71' or connection member 713. Hence, the connection member 713 can move independently around the plunger 92", and the plunger 92" can move independently through the connection member 713. As discussed above, because the needle sheath 72" is directly connected to the connection member 713 contained in the controller lumen 717, the plunger 92" enters the inside cavity of the needle sheath 72" inside the needle sheath controller 71'. The plunger 92" exits the distal end of the needle sheath controller 71' where it is contained within the hollow cavity of the needle sheath 72".

[0233] At the distal end of the device 60", the needle sheath 72" ends in a distal tip of the needle sheath 73' that contains a needle channel 733 that is sufficiently sized to fit injection needle 81. When the dockable syringe 910 is docked in the device in the docked position 910b as shown in FIGS. 11B-D, injection needle 81 fits through groove 76 where it is lined up to pass through needle channel 733 so that injection needle 81 can extend and retract through needle channel 733 as the needle sheath 72" moves. In FIG. 11B, injection needle 81 is fit into the groove 76 and contained in needle sheath 72", but does not traverse through the distal portion of needle channel 733. With reference to FIG. 4A, the device 60" in FIG. 11B is in the sheathed position 72a. In FIG. 11C, injection needle 81 is extended out of needle sheath 72" and does traverse through the distal portion through needle channel 733. With reference to FIG. 4C, the device 60" in FIG. 11C is in the unsheathed position.

[0234] As shown in FIGS. 11B and 11C, because syringe barrel 91" is not connected to needle sheath 72", the needle sheath 72" moves independently around syringe barrel 91". In the unsheathed position 72c as shown in FIG. 11C, the needle sheath 72" is pulled back, but the syringe barrel 91" and injection needle 81 are fixed and do not move. For example, as shown in FIG. 11C, because the needle sheath 72" is pulled back, the distal portion of the syringe barrel 91" is covered up by the distal tip of the needle sheath 73. In contrast, in the sheathed position 72a as shown in FIG. 11B, the sheath is not pulled back, such that the distal end of the syringe barrel 91" is not covered up by the distal tip of needle sheath 73. Hence, movement of the needle sheath 72" between sheathed and unsheathed positions, shortens the amount of syringe barrel 91" that is exposed in the docked cavity of device 60".

[0235] As described above, in the unsheathed position

72c as shown in FIG. 11C, the extent by which injection needle 81 is extended or exposed out of the device 60" is a function of the distance between sheath stops 715 and 716 as shown in FIG. 7 (and related FIG. 5 and 6).

5 This distance is a function of the particular application of the device, the particular target tissue, the subject being treated and other considerations. For example, unsheathed needle that is exposed should not be so long that it can easily penetrate through to the other side of a target tissue. Generally, with reference to most target tissues (e.g. liver), the portion of the injection needle 81 shown in FIG. 11C that can be unsheathed or exposed is generally less than 1 cm, such as 2 mm to 10 mm, and generally no more than 5 mm. For a child, the length can be smaller, and is generally less than 4 mm. For applications in utero, the length can be 2 mm to 3 mm. Generally, the total length of the injection needle 81 in device 60" is slightly longer than the unsheathed needle tip that can extend out of the device in the fully unsheathed position. As shown in FIG. 11C, the extent of the extra length is sufficient to account for the portion of the proximal end of the injection needle 81 still contained in the distal tip of sheath 73' and distal end of syringe barrel 91" when device is in the unsheathed position. For example, as described above, the total length of the injection needle 81 can range from 5 mm to 40 mm, such as 10 mm to 40 mm, such as a 12.7 mm, 25.4 mm or 38.1 mm needle.

[0236] Dispelling or ejecting a fluid, such as a therapeutic, or other solution through the injection needle is controlled by depressing plunger 92", which effects depression of auxiliary plunger 920 because of the connection achieved by plunger adaptor 951. With reference to FIG. 11C, plunger 92" is in an extended position, such that auxiliary plunger 920 also is in an extended position. In contrast, FIG. 11D illustrates plunger 92" in the depressed position, such that auxiliary plunger 920 also is in the depressed position. This allows the delivery of the fluid, such as a therapeutic, to the target tissue. The plunger 92" also can be used to control draw back of fluids from the injection site if drawback is required to test the needle placement. This is achieved by pulling or drawing back on plunger 92", which, through its connection with auxiliary plunger 920, also draws back auxiliary plunger 920. The drawback fluid can be visible in syringe barrel 91" where it is not covered by needle sheath 72".

[0237] The dockable syringe 910 (containing auxiliary plunger 920, syringe barrel 91" and injection needle 81) and/or the device 60" can be disposable or reusable. For example, after injection or exhaustion of the fluid, such as a therapeutic, from the syringe barrel 91", or when otherwise desirable, dockable syringe 910 can be withdrawn from the laparoscopic port. A newly loaded dockable syringe 910 can be docked into device 60". The newly loaded dockable syringe 910 can contain the previously used dockable syringe barrel 91" that can be reloaded, or it can be new pre-loaded dockable syringe 910. Alternatively, the device 60" can be withdrawn from the laparoscopic port and disposed of after one use. In

cases where sterile injections are required, the syringe barrel **91**" can be loaded with the fluid, such as a therapeutic, in a sterile environment, such as a sterile operating room, and then docked into device **60**". Alternatively, a sterile pre-loaded dockable syringe **910** can be used, which can be docked into device **60**".

[0238] With reference to the above Figures and description, exemplary of the mode of operation of the injection device **60**" involves first loading dockable syringe **910** with fluid, such as a therapeutic, prior to docking the syringe into the syringe adaptor in the syringe adaptor lining **96** located inside the needle sheath **72**". Once the dockable syringe **910** is loaded, the syringe is docked into the syringe dock by engagement with barrel docks **961** and **963** and plunger adaptor **951**. The needle sheath **72**" can be positioned in the sheathed position **72a**, and the device can be inserted into a laparoscopic port to be positioned close to the target site. At the site of injection (target tissue), the needle sheath **72**" can be unsheathed **72c**, and the injection needle **81** can be exposed for injection. If necessary, the control plunger **92**" can be pulled back to draw fluids from the site of injection, for example, to test the placement of injection needle **81** at the injection site. The drawback fluid is visible at the distal end of syringe barrel **91**" in needle sheath **72**". The control plunger **92**" can be depressed, to inject the fluid, such as a therapeutic, at the target tissue. After injection, the needle sheath **72**" can be positioned in the sheathed position **72a**, to protect the non-target organs and prevent accidental needle puncture, prior to removing the laparoscopic device from the injection site and through the laparoscopic port.

C. APPLICATIONS AND USES

[0239] The injection devices provided herein permits direct delivery of fluids, such as a therapeutic, into a specific target site, such as the parenchyma of an organ internal to the body of the subject, in minimally invasive procedures, such as surgeries, for example as laparoscopic surgeries. Accordingly, the injection device can be used in diverse applications, including, but not limited to, medical applications, including applications to exogenously administer a fluid, such as a therapeutic, for the treatment of a disease or condition, or other applications such as agricultural, veterinary and industrial applications that require direct delivery of a fluid to a target site in minimally invasive procedures. For example, the device can be used to deliver chemotherapeutic agents to a specific target organ, or the device can be used to deliver nucleic acids or viral agents to a specific organ targeted for gene therapy, without the need of invasive open surgery. In some examples, the injection device can be useful in delivering fluids, such as a therapeutic in settings where the fluid treats or ameliorates a disorder or condition in a subject or otherwise improves the quality of life in a subject. In other examples, the injection device can be useful in agricultural settings, for example, for

applications that improve the quality or quantity of meat production.

[0240] The injection device can be used in any subject or patient that is in need of direct delivery of a fluid, such as a therapeutic, into a target site in a minimally invasive manner. Exemplary of such subjects include, but are not limited to, mice, rats, cows, pigs, sheep, goats, horses and humans. In particular examples, children under age 18, including infants, toddlers or young children, are contemplated herein for the delivery of fluids, such as therapeutics, for the treatment of diseases or conditions. In particular examples, *in utero* delivery of a fluid, such as a therapeutic, to the fetus is contemplated herein, for the treatment of diseases or conditions.

[0241] Exemplary applications of the method herein are provided below. It is understood that other applications exist depending on the particular fluid delivered, setting or subject. It is within the level of a person skilled in the art choose a fluid, setting, or subject of interest based on any desired application. The description herein below is for exemplification only.

1. TREATING DISEASES AND DISORDERS

[0242] Provided herein are applications of treating a disease, disorder or condition by delivering a fluid, such as a therapeutic, directly into a target injection site in a subject using the injection device provided herein. The disease, disorder or condition that is treated is any that is amenable to treatment by an exogenously delivered fluid, such as a therapeutic, directly to the target site, such as the parenchyma of an internal organ of a subject. In any of such examples herein, the fluid, such as a therapeutic, is delivered directly and specifically to the target injection site during a minimally invasive procedure. Thus, provided herein is an injection device that is used to deliver an accurate amount of fluid to the target injection site of the subject in a minimally invasive procedure without accidental puncture of non-target sites or damage to the apparatuses used for minimally invasive procedures. The particular device used has an injection needle that when unsheathed also cannot puncture through the tissue or organ in which the direct injection is effected.

[0243] The fluid used for injection can be any fluid used for injection. In particular examples, the fluid contains a therapeutic used for treating a disease, disorder or a condition. The therapeutic can include a fluid comprising small molecule drugs, prodrugs, proteins, peptides, DNA, RNA, viruses, antibodies, organic molecules, saccharides, polysaccharides, lipids and combinations or conjugates thereof. In particular examples, the fluid can comprise a therapeutic including, but not limited to, a gene therapy agent, a chemotherapeutic agent, an analgesic agent, an anti-inflammatory agent, an antimicrobial agent, an amoebicidal agent, a trichomonocidal agent, an anti-parkinson agent, an anti-malarial agent, an anticonvulsant agent, an antidepressant agent, an antiarthritics agent, an anti-fungal agent, an antihyperten-

sive agent, antipyretic agent, an anti-parasite agent, an antihistamine agent, an alpha-adrenergic agonist agent, an alpha blocker agent, an anesthetic agent, a bronchi dilator agent, a biocide agent, a bactericide agent, a bacteriostat agent, a betadrenergic blocker agent, a calcium channel blocker agent, a cardiovascular drug agent, a contraceptive agent, a decongestant agent, a diuretic agent, a depressant agent, a diagnostic agent, an electrolyte agent, a hypnotic agent, a hormone agent, a hyperglycemic agent, a muscle relaxant agent, a muscle contractant agent, an ophthalmic agent, a parasympathomimetic agent, a psychic energizer agent, a sedative agent, a sympathomimetic agent, a tranquilizer agent, a urinary agent, a vaginal agent, a viricide agent, a vitamin agent, a non-steroidal anti-inflammatory agent, an angiotensin converting enzyme inhibitor agent, an alcohol and a sleep inducer.

[0244] For example, the therapeutic can be a polypeptide, such as an enzyme, a hormone, a coagulation or clotting factor, a cytokine, a growth factor or active portion thereof, an antibody or antigen binding portions of antibodies, an angiogenesis modulator, an immunomodulator, a pain modulator, a receptor or active portion thereof, a transport protein, a regulatory protein, an antigen and an allergen.

[0245] In another example, the therapeutic can be a nucleic acid molecule for gene therapy, wherein the nucleic acid molecule encodes a polypeptide. The encoded polypeptide can include an enzyme, a hormone, a coagulation or clotting factor, a cytokine, a growth factor or active portion thereof, an antibody or antigen binding portions of antibodies, an angiogenesis modulator, an immunomodulator, a pain modulator, a receptor or active portion thereof, a transport protein, a regulatory protein, an antigen or an allergen. In a particular example, the polypeptides encoded can include adenosine deaminase, cystic fibrosis transmembrane conductance regulator (CTFR), galsulfase, laronidase, N-acetylgalactosamine 6-sulfatase, phenylalanine ammonia lyase, acid alpha glucosidase, imiglucerase, alglucosidase alpha, thyrotropin, growth hormone, insulin, thyroid hormone, erythropoietin (EPO), interleukin-1 (IL-1), IL-2, IL-3, IL-4, IL-5, IL-7, interferon- α (IFN- α), IFN- β , IFN- γ , tumor necrosis factor (TNF), IL-12, IL-18, Fms-Related Tyrosine Kinase 3 (flt3), neuropilin-2 (NP2), bone morphogenic protein (BMPs), epidermal growth factor (EGF), erythropoietin (EPO), fibroblast growth factor (FGF), granulocyte colony stimulating factor (G-CSF), granulocyte macrophage colony stimulating factor (GM-CSF), hepatocyte growth factor (HGF), insulin-like growth factor (IGF), platelet derived growth factor (PDGF), transforming growth factor α or β , vascular endothelial growth factor (VEGF), epidermal growth factor receptor (EGFR), fibroblast growth factor receptor (FGFR), FGFR antagonist (sFGFR) transforming growth factor receptor (TGFR), vascular endothelial growth factor receptor (VEGFR), plasminogen activator, urokinase, Factor VIII, Factor IX, von Willebrand factor, growth hormone, met-

alloproteinase thrombospondin motifs 1 (METH-1), METH -2, tryptophanyl-tRNA synthetase (TrpRS) fragments, proliferin-related protein, prolactin fragment, pigment epithelium-derived factor (PEDF), vasostatin, angiostatin, endostatin, kininostatin, fibrinogen-E fragment, thrombospondin, tumstatin, canstatin, restin, soluble fms-like tyrosine kinase-1 (sFlt-1), soluble vascular endothelial growth factor receptors (sFlk), soluble Neuropilin 1 (sNRP1), Interferon gamma-induced protein 10 (IP-10), Platelet factor 4 (PF-4), Gro-beta, soluble Ephrin type-B receptor 4 (sEphB4), sephrinB2, IGF-1, herpes simplex virus thymidine kinase (HSV-TK), carboxypeptidase G2 (CPG2), carboxylesterase (CA), cytosine deaminase (CD), cytochrome P450 (cyt-450), deoxycytidine kinase (dCK), nitroreductase (NR), purine nucleoside phosphorylase (PNP), thymidine phosphorylase (TP), varicella zoster virus thymidine kinase (VZV-TK), xanthine-guanine phosphoribosyl transferase (XGPRT), Aspartylglucosaminidase, α -Galactosidase A, Palmitoyl Protein Thioesterase, Tripeptidyl Peptidase, Lysosomal transmembrane protein, cysteine transporter, Acid ceramidase, acid α -L-fucosidase, protective protein/cathepsin A, acid β -glucosidase or glucocerebrosidase, acid β -galactosidase, iduronate-2-sulfatase, α -L-Iduronidase, galactocerebrosidase, acid α -mannosidase, acid β -mannosidase, arylsulfatase B, arylsulfatase A, N-Acetylgalactosamine-6-sulfate sulfatase, N-Acetylglucosamine-1-phosphotransferase, Acid sphingomyelinase, Niemann-Pick disease, type C1 (NPC-1), β -Hexosaminidase B, Heparan N-sulfatase, α -N-Acetylglucosaminidase (NaGlu), Acetyl-CoA: α glucosaminide N-acetyltransferase, N-Acetylglucosamine-6-sulfate sulfatase, β -Glucuronidase, acid lipase, neprilysin, the insulin-degrading enzyme insulysin, thimet oligopeptidase, calbindin D28, parvalbumin, hypoxia induced factor 1-alpha (HIF1-alpha), sirtuin-2 (SIRT-2), survival motor neuron protein-1 (SMN-1), SMN-2, glial cell-derived neurotrophic factor (GDNF), ciliary neurotrophic factor (CNF), low density lipoprotein receptor (LDLR), lipoprotein lipase (LPL), Alpha-1-Antitrypsin (AAT), UDP-glucuronyl-transferase (UGT), UGT1A1, glucose-6 phosphatase, phosphoenolpyruvate-carboxykinase, galactose-1 phosphate uridyl transferase, phenylalanine hydroxylase, branched chain alpha-ketoacid dehydrogenase, fumarlylacetate hydrolase, methylmalonyl-CoA mutase, ornithine transcarbamylase, argininosuccinic acid synthetase, adenosine deaminase, hyposanthine guanine phosphoribosyl transferase, biotinidase, beta-glucocerebrosidase, beta-glucuronidase, porphobilinogen deaminase (PBDG) and p53.

[0246] For example, diseases or conditions for which the injection device provided herein can be used include any in which treatment is effected by increasing or decreasing the activity of a specific protein or other cellular targets, decreasing or increasing expression of a gene associated with the condition, decreasing or increasing the activity of a gene product associated with the condition or otherwise countering the alteration associated

with the condition (e.g. signs, symptoms or effects associated with the disease or condition), by direct delivery of the therapeutic to a target organ. For example, non-specific or targeted chemotherapeutic agents can be delivered directly and specifically to the parenchyma of a solid tumor to kill rapidly dividing cells. The diseases or conditions for which the injection device provided can be used for include an arthritis, chronic pain, HIV-related AIDS, atherosclerosis, restenosis, inherited enzyme deficiency, inherited immune deficiency, cancer, a retrovirus infection, hemophilia, diabetes, a muscular dystrophy, a cardiovascular disorder, cystic fibrosis, a neurodegenerative disorder, trauma, pain, sickle cell anemia, autoimmune disease, inflammatory disease, and hypertension.

[0247] In another example, the device can be used to deliver fluids that include gene therapy agents, such as nucleic acids, vectors or viruses. Gene therapy can be used to treat diseases or conditions associated with genetic deficiencies, including monogenic diseases, (e.g. hemophilia A and B, type I diabetes mellitus, alpha-1-antitrypsin (AAT), cystic fibrosis, muscular dystrophy and numerous others) or can be used to treat diseases or conditions by encoding a therapeutic protein associated with ameliorating the disease or condition (e.g. cancers).

[0248] The injection device provided herein can be used in methods to inject a wide variety of fluids in medical applications. The delivered fluid, and the therapeutic agent therein, is selected based on the disorder or disease to be addressed, and the particular organ affected. As described elsewhere herein, one of skill in the art can determine the type of therapeutic agent depending on the particular disease or disorder that is being treated. As further exemplification, the injection device can be used to deliver anti-angiogenesis agents, such as angiostatin or endostatin for the treatment of cancer, insulin for the treatment of diabetes mellitus, soluble tumor necrosis factor (TNF) receptor for the treatment of rheumatoid arthritis, angiostatin for the treatment of renal failure, anti-human immunodeficiency virus (HIV) agents for the treatment of HIV infection and acquired immunodeficiency syndrome (AIDS), ethanol for the treatment of papillary thyroid carcinoma (PTC), and Factor VIII or Factor IX for hemophilia. The therapeutic agents can also be in the form of nucleic acids that encode a protein required to ameliorate the disease symptoms or treat the disease. In other examples, the injection device can be used to deliver a nucleic acid encoding a Factor VIII for the treatment of hemophilia A; a Factor IX for the treatment of hemophilia B; an insulin gene for treatment of type I diabetes mellitus; an alpha-1-antitrypsin (AAT) for the treatment of alpha-1-antitrypsin (AAT) deficiency; a hemochromatosis protein (HFE) for treatment of hemochromatosis; a copper-transporting ATPase 2 for treatment of Wilson's disease; UDP glucuronosyltransferase 1A1 (UGT1A1) for the treatment of Crigler-Najjar syndrome type I; ornithine transcarbamylase (OTC) for the treatment of ornithine transcarbamylase deficiency, type II;

low density lipoprotein receptor (LDLR) for the treatment of familial hypercholesterolemia; fibrinogen alpha (FGA), beta (FGB) or gamma (FGB) for the treatment of afibrinogenemia; glucose-6-phosphate- α for the treatment of glycogen storage disease (GSD) type Ia; G6PT for the treatment of GSD type Ib; acid- α -glucosidase for the treatment of GSD type II (Pompe); α -L-iduronidase for the treatment of mucopolysaccharidosis (MPSI); sul-
 5 phamidase for the treatment of MPS IIIA; α -N-acetylglucosaminidase (NaGlu) for the treatment of MPS IIIB; β -glucuronidase for the treatment of MPS VII; α -galactosidase A for the treatment of Fabry disease; glucocerebrosidase for the treatment of Gaucher's disease; acid sphingomyelinase for the treatment of Niemann-Pick
 10 syndrome; phenylalanine hydroxylase for the treatment of phenylketonuria; TIMP antagonist or anti-HSC molecules for the treatment of liver fibrosis; anti-ROS molecules for the treatment of liver ischemia reperfusion injury; amyloid-beta degrading enzyme neprilysin, the insulin-degrading enzyme insulysin, or thimet oligopeptidase for the treatment of Alzheimer's disease; insulin
 20 growth factor-1 (IGF-1), calbindin D28, parvalbumin, HIF1-alpha, SIRT-2, VEGF, SMN-1, SMN-2, GDNF or ciliary neurotrophic factor (CNF) for the treatment of
 25 Amyotrophic Lateral Sclerosis (ALS); galactose-1 phosphate uridyl transferase for the treatment of galactosemia; branched chain alpha-ketoacid dehydrogenase for the treatment of maple syrup urine disease; fumarylacetoacetate hydrolase for the treatment of tyrosinemia type 1;
 30 methylmalonyl-CoA mutase for the treatment of methylmalonic acidemia; argininosuccinic acid synthetase for the treatment of citrullinemia; hyposanthine guanine phosphoribosyl transferase for the treatment of Gout and Lesch Nyan syndrome; beta-glucuronidase for the treatment of Sly syndrome; peroxisome membrane protein
 35 70 kDa for the treatment of Zellweger syndrome, enfuvirtide for the treatment of Human immunodeficiency virus (HIV) infection; adenosine deaminase (ADA) for the treatment of combined immunodeficiency disease
 40 (SCID); cystic fibrosis transmembrane conductance regulator (CFTR) for the treatment of cystic fibrosis; porphobilinogen deaminase (PBDG) for the treatment of acute intermittent porphyria; interferon-beta for the treatment of multiple sclerosis; lipoprotein lipase for the treatment of lipoprotein lipase deficiency (LPLD), p53 for the treatment of cancer; glutamic acid decarboxylase (GAD) for the treatment of Parkinson's Disease; neuropilin-2 (NP2) for treatment of pain; a nucleic acid encoding an angiogenesis inhibitor or tumor suppressor for the treatment
 45 of cancer; and a nucleic acid encoding an insulin or exendin-4 for treatment of diabetes.

[0249] Further, it is known to one of skill in the art the particular target tissue or organ for direct injection of the fluid based on the disease or disorder to be treated, and the particular delivered therapeutic agent that is administered. In some cases, the delivered fluid such as a therapeutic does not exhibit specific tissue targeting when systemically administered, and thus is delivered directly

to the affected target site, such as a tissue or an organ.

[0250] For specific target tissues or organs for delivery of fluids, such as a therapeutic, the lung is an important target organ for direct injection of therapeutics to treat or ameliorate many acute and chronic diseases, including cancer, asthma, cystic fibrosis, alpha-1-antitrypsin deficiency and respiratory distress syndrome, among others. The muscle is a target organ for direct injection of therapeutics for treatment of muscular or motor disorders like muscular dystrophy or charcot-Marie-Tooth (CMT) disease. The brain is an important target organ for direct injection of therapeutics of motor neuron diseases (e.g. spinal muscular atrophy (AMA), amyotrophic lateral sclerosis (ALS), X-linked adrenoleukodystrophy (ALD)), Parkinson's Disease, or diseases and conditions associated with a missing or defective gene, including metabolic or lysosomal disorders such as Sanfilippo (mucopolysaccharidosis type III; MSPIII) or Canavan disease. The skin is a target organ for direct injection of therapeutics for chronic wounds, hypertrophic scars, keloids, cancer, genetic diseases and systemic diseases. The liver is a target organ for direct injection of therapeutics of numerous liver diseases and disorders including, but not limited to, hemochromatosis, hemophilia A and B, alpha 1 antitrypsin deficiency, Wilson's disease, Crigler-Najjar syndrome type I, ornithine transcarbamylase deficiency, type IIa familial hypercholesterolemia, afibrinogenemia, lysosomal storage diseases, glycogen storage diseases, phenylketonuria, Tay-Sachs disease, induced hepatitis.

[0251] This list is not intended to be limiting, as any disease or condition that can be addressed with a therapeutic agent that is directly and specifically delivered to a target injection site could be addressed. Exemplary methods of treating various diseases and conditions are described below.

D. EXAMPLES

[0252] The following examples are included for illustrative purposes only and are not intended to limit the scope of the invention.

Example 1

Construction of Syringe Injection Device

[0253] A syringe injection device **60** of the type depicted in FIGS. 1A, 1B, 5, 8A-B and 9A-D and as described in the detailed description was constructed. The device contains a plunger **92** and syringe barrel **91**, a needle sheath controller **71**, a needle sheath **72**, and an injection needle **81**. The device was configured so that a standard 1 cc syringe barrel **91** containing plunger **92**, but without needle, is able to be separately attached to needle sheath controller **71**. To permit laparoscopic access to a portion of the liver, the diameter of the needle sheath **72** was 5 mm and the length of the needle sheath **72** was 300 mm (see e.g. FIG. 1A showing syringe barrel removed from

needle sheath controller, position **900a**, and FIG. 1B showing syringe barrel attached to needle sheath controller, position **900b**).

[0254] As constructed, when the syringe barrel **91** is connected to the needle sheath controller **71**, the injection needle **81** is connected to syringe barrel **91** via an injection tube **83**. The injection needle was a standard 27 gauge of 10 mm in length and was connected directly to a 27 gauge injection tube **83**. The injection tube **83** and injection needle **81** were made of stainless steel. The injection tube **83** contained a needle hub **84** at proximal end, and the injection tube **83** and needle hub **84** were directly affixed to needle sheath controller **71** at the proximal end of the inside of the needle sheath controller **71** (see e.g. FIG. 1A and 1B).

[0255] A standard 1 cc insulin syringe containing a syringe barrel **91** and plunger **92**, but without a needle, was filled with 0.7 mL solution and purged. The syringe was attached to the proximal end of the needle hub **84** outside of the needle sheath controller **71** using a Luer fit adaptor **93** (see FIG. 1A and 1B). The injection needle **81** was sheathed and locked by sliding the positioner **711** forward.

Example 2

Compartmentalized Transduction of The Liver in a Laparoscopic Simulator

[0256] A clamp device and the injection device **60** described in Example 1 were utilized in a laparoscopic simulator by a skilled surgeon/physician to effect clamping of a portion of the left median lobe of a liver to compartmentalize the region for delivery of an injectable solution. The laparoscopic simulator (*Lapa-Pro, Mexico*) was positioned at a 35° to 45° angle inclination to simulate the Semi-Fowlers position of a subject. The Semi-Fowlers position facilitates the access to the distal portion of the left lobe of the human liver using gravity to distally displace the abdominal organs. With respect to a subject, the entry ports of the simulator were positioned as follows: one entry port in the epigastric abdominal region; one entry port in the umbilical abdominal region; and two entry ports in the left lumbar abdominal region.

[0257] A freshly obtained cadaveric pig liver was positioned inside the laparoscopic simulator. The laparoscope was inserted through the umbilical entry port. A laparoscopic clamp was inserted through the epigastric entry port and was used to clamp a 5 cm portion of the distal portion of the left median lobe of the cadaveric pig liver.

[0258] A standard 1 cc insulin syringe was filled with 0.7 mL tap water solution and purged. The filled syringe containing a syringe barrel **91** and plunger **92** was attached to a needle hub **84** on the proximal end of the needle sheath controller **71** as depicted in FIG. 1B. The positioner **711** on the needle sheath controller **71** was slid backward to unlock the positioner **711** and to un-

sheathe the injection needle **81**. The entire syringe injection device was purged by pressing the plunger until fluid was observed at the tip of the needle (approximately 200 μL). The positioner **711** on the needle sheath controller **71** was then slid forward to lock the positioner **711** in the forward position **711a** and to sheathe the injection needle **81**. The injection device with the needle sheathed was introduced into the simulator through the proximal left lumbar entry port. Using the laparoscope monitor, the tip of the injection device was positioned close to the site of injection. The injection needle **81** on the injection device was unsheathed by sliding the positioner **711** backward and locking the positioner in the rearward position **711c**. The tip of the injection needle **81** was introduced into the parenchymal tissue making sure that it did not go through the tissue. Once the tip of the injection needle **81** was carefully positioned inside the parenchyma, the plunger **92** was pressed until 500 μL of fluid was injected.

[0259] The positioner **711** on the needle sheath controller **71** was slid forward to lock the positioner **711** in the forward position **711a** and to sheathe the needle. The injection device **60** was removed from the simulator. The clamp also was released from the liver. Once released, the procedure was over, and the clamp also was removed from the simulator.

[0260] Since modifications will be apparent to those of skill in the art, it is intended that this invention be limited only by the scope of the appended claims.

Claims

1. An injection device, comprising:

a syringe barrel (91), wherein the syringe barrel provides a fluid reservoir;
 a plunger (92) configured to be controlled by the operator of the device and to move within the syringe barrel for loading and releasing fluid from the fluid reservoir in the syringe barrel; and
 is **characterized by** further comprising:

a) an injection needle (81) that is fixed and operably coupled to the syringe barrel (91) providing a fluid pathway for fluid contained in the syringe barrel to be injected into a target tissue when the plunger (92) is depressed, wherein extraction or retraction of the needle is independent of movement of the plunger;

b) an elongate sheath (72), comprising an internal lumen (723) that contains the injection needle and having a distal tip that contains an opening for the injection needle, wherein:

the sheath is movable around the injection needle; and

control of the sheath is independent from movement of the plunger; and

c) a controller (71) for positioning the sheath, comprising:

a housing (710), comprising at least a first (715) and second (716) stop to control exposure of the injection needle and that are provided within the housing at a predetermined distance from each other, wherein the stops can be locked;

a central lumen (717) in the housing comprising a connection member, wherein the connection member (713) is configured to be movable in the central lumen in the housing and is coupled to the sheath, wherein the proximal end of the sheath is coupled to the distal end of the connection member so that movement of the connection member controls movement of the sheath; and
 a positioner (711) mounted within the housing configured to move forward towards the distal end of the controller and rearward towards the proximal end of the controller, between the stops in the housing, wherein the positioner is operatively connected to the connection member to guide movement of the connection member in the same direction, whereby movement of the positioner forward towards the distal end engages the first stop and moves the sheath to enclose the injection needle inside the lumen of the sheath (711a, 72a), and movement of the positioner rearward towards the proximal end engages the second stop and moves the sheath to expose no more than a predetermined length of the distal tip of the injection needle (711c, 72c) through the opening in the injection needle for injection into the tissue.

2. The injection device of claim 1, wherein the elongate sheath (72) is of a sufficient length and width to reach an organ through an endoscopic port.

3. The injection device of claim 1 or claim 2, comprising at least 3 stops, 4 stops or 5 stops, wherein:

the second (716) stop is the most proximal stop and the first (715) stop is the most distal stop and the other stop or stops are positioned between the first stop and the second stop; and
 each stop is positioned at a predetermined distance from adjacent stop or stops to control exposure of the needle to different predetermined lengths, wherein the second stop controls exposure of the needle to its longest predetermined

- length, whereby the positioner (711) can move between the adjacent stops to engage with the stop to expose different predetermined lengths of the injection needle (81).
4. The injection device of any of claims 1-3, wherein the positioner (711) comprises a lock and release element (712) that is configured in the positioner to engage the positioner with the stops.
5. The injection device of claim 4, wherein the lock and release element (712) is a spring that provides an upward force against the positioner (711) and a downward force against the connection member (713) to lock the positioner into the stop, and is capable of being compressed to release the positioner from the stop.
6. The injection device of any of claims 1-5, wherein the syringe barrel (91) is proximal or distal to the controller (71).
7. The injection device of any of claims 1-6, wherein the syringe barrel (91) is proximal to the controller (71) and is operably coupled to the injection needle (81) by an injection tube (83), wherein:
- the injection tube comprises a proximal and a distal end, the proximal end connected to the syringe barrel and the distal end connected to the injection needle; and
- the controller is configured to hold the injection tube and comprises an opening at the proximal end so that the injection tube is operably connected to the syringe barrel.
8. The injection device of claim 7, wherein the syringe barrel (91) is configured to be connected to the injection tube (83) so that the syringe barrel is detachable from the device.
9. The injection device of claim 7 or claim 8, wherein the injection tube (83) comprises a hub (84) on its proximal end that is compatible with an adaptor (93) on the distal end of the syringe barrel and the hub of the injection tube connects to the adaptor of the syringe barrel.
10. The injection device of any of claims 7-9, wherein:
- the injection tube (83) is fixed in the controller (71);
- the connection member (713) in the controller comprises a recess by which the injection tube is routed to pass from the controller into the sheath (72) at the junction where the connection member is coupled to the sheath; and
- the connection member is movable around the
- injection tube.
11. The injection device of any of claims 7-10, wherein the injection tube (83) is connected directly to the injection needle (81).
12. The injection device of any of claims 7-10, wherein the injection tube (83) is connected indirectly to the injection needle (81) via a coupler (85), the coupler having a proximal and distal end, the proximal end connected to the distal end of the injection tube and the distal end connected to the proximal end of the injection needle.
13. The injection device of any of claims 7-12, wherein the injection tube (83) and injection needle (81) are the same gauge or different gauges.
14. The injection device of any of claims 1-13, further comprising an injection tube (83) by which the injection needle (81) is operably coupled to the syringe barrel (91), wherein:
- the injection tube comprises a proximal and a distal end, the proximal end connected to the syringe barrel and the distal end directly or indirectly connected to the injection needle;
- the injection needle has a diameter of 25 gauge or less or is 25 gauge to 34 gauge and has a length in the range from 5 mm to 40 mm; and
- the injection tube has a larger diameter than the injection needle, wherein the injection needle is connected to the syringe barrel;
- the controller (71) is distal to the syringe barrel and plunger (92) and comprises:
- a cavity for the injection tube and an opening at the proximal end so that the injection tube extends out of the controller to connect to the syringe barrel, wherein the injection tube is fixed in the controller; and
- a central lumen (717) in the housing (710) comprising a connection member (713), wherein:
- the connection member in the controller comprises a recess by which the injection tube is routed to pass from the controller into the distal lumen of the sheath at the junction where the connection member is coupled to the sheath (71); and
- the connection member is configured to be movable in the central lumen in the housing around the injection tube and is coupled to the sheath, wherein the proximal end of the sheath is coupled to the distal end of the connection member so that movement of

the connection member controls movement of the sheath.

15. The injection device of any of claims 7-14, wherein the total length of the injection tube (83) and injection needle (81) is as long as the controller (71) and sheath (72).

16. The injection device of any of claims 1-6, wherein:
the syringe barrel (91) is positioned distal to the controller (71) and the internal lumen (723) of the sheath comprises the syringe barrel in its distal end; and
the syringe barrel is configured in the lumen so that the sheath is movable around the syringe barrel.

17. The injection device of claim 16, wherein:
the open cavity (726) of the sheath (72) comprises a lining (96) that is configured in the sheath so that the sheath is movable around the lining; and
the syringe barrel (91) is mounted into the lining in the open cavity.

18. The injection device of claim 17, wherein the open cavity (726) extends the length of the sheath (72).

19. The injection device of any of claims 16-18, wherein the plunger (92) is operably connected to the syringe barrel (91) in the distal end of the lumen of the sheath and arranged so that the plunger is movable through the controller (71) and within the lumen of the sheath.

20. The injection device of any of claims 16-18, wherein; the plunger (92) is operably connected to the syringe barrel (91) by an auxiliary plunger (920) provided in the lumen of the sheath; and
the plunger is adapted to couple with the auxiliary plunger in the lumen of the sheath and arranged so that the plunger is movable through the controller (71) and sheath (72) and the auxiliary plunger is movable through the sheath and configured to move within the syringe barrel, whereby depressing the plunger depresses the auxiliary plunger into the syringe barrel releasing fluid from the fluid reservoir in the syringe barrel and pulling back on the plunger pulls back on the auxiliary plunger to load fluid into the fluid reservoir in the syringe barrel.

21. The injection device of claim 20, wherein:
the sheath (72) comprises an open cavity (726) comprising a detachable syringe (900a, 900b); and
the detachable syringe comprises the syringe

barrel (91), the auxiliary plunger (920) having a distal end configured to be movable in the syringe barrel and a proximal end coupled to the plunger, and the injection needle (81) that is operably coupled to the syringe.

22. The injection device of any of claims 16-21, wherein the controller (71) is configured to hold the plunger (92) so that the plunger is movable within the controller, the controller comprising:

an opening at its proximal end to receive the plunger; and
a recess in the connection member (713) of the controller by which the plunger is routed to pass from the controller into the lumen of the sheath at the junction where the connection member is coupled to the sheath, wherein the plunger and connection member move independently with respect to each other.

23. An injection device of any of claims 16-22, further comprising:

an auxiliary plunger (920) attached to the plunger (92) to form an extended plunger configured to be controlled by the operator of the device to move within the syringe barrel (91) for loading and releasing fluid from the fluid reservoir in the syringe barrel, whereby depressing the plunger depresses the auxiliary plunger into the syringe barrel releasing fluid from the fluid reservoir in the syringe barrel and pulling back on the plunger pulls back on the auxiliary plunger to load fluid into the fluid reservoir in the syringe barrel; an opening at the proximal end of the controller (71) to receive the plunger and comprising a cavity configured to hold the plunger so that the plunger is movable within the controller; and
a recess in the connection member (713) by which the plunger is routed to pass from the controller into the distal lumen of the sheath at the junction where the connection member is coupled to the sheath, wherein the plunger and connection member move independently with respect to each other;

wherein:

the injection needle (81) is 25 gauge to 34 gauge and has a length in the range from 5 mm to 40 mm; and
the elongate sheath (72) comprises an internal lumen (723) that contains the plunger, the auxiliary plunger, the syringe barrel and the injection needle and having a distal tip (73) that contains an opening for the injection needle, wherein:

the sheath is enclosed at its proximal end and provides a conduit for the plunger, wherein the plunger is movable through the sheath;

the sheath comprises an open cavity (726) at the distal end, the open cavity comprising the auxiliary plunger, syringe barrel and injection needle, wherein:

the open cavity of the sheath comprises a lining that is configured in the sheath so that the sheath is movable around the lining;

the auxiliary plunger, syringe barrel and injection needle are mounted into the lining in the open cavity; and the auxiliary plunger, syringe barrel and injection needle are detachable as a unit from the open cavity; and the sheath is movable around the plunger, auxiliary plunger, syringe barrel and injection needle.

24. An injection device of any of claims 1-23 for use for delivering a therapeutic to the parenchyma of an organ or tissue.

25. An injection device of any of claims 1-23 for use in delivering a therapeutic to an organ or tissue during a surgery.

26. The injection device for use of claim 25, wherein surgery is minimally invasive surgery.

27. The injection device for use of any of claims 24-26, wherein:

the therapeutic is a nucleic acid; and the surgery effects delivery of nucleic acid for gene therapy.

Patentansprüche

1. Injektionsvorrichtung, die aufweist:

einen Spritzenzylinder (91), wobei der Spritzenzylinder ein Fluidreservoir ausbildet; einen Kolben (92), der ausgebildet ist von einer Bedienperson der Vorrichtung bedient zu werden und sich innerhalb des Spritzenzylinders zu bewegen, um das Fluidreservoir in dem Spritzenzylinder zu füllen und zu entleeren; und **dadurch gekennzeichnet ist, dass** sie ferner aufweist:

a) eine Injektionskanüle (81), die an dem Spritzenzylinder (91) befestigt und mit die-

sem funktionell verbunden ist und die einen Fluidweg für ein in dem Spritzenzylinder enthaltenes Fluid ausbildet, das beim Herunterdrücken des Kolbens (92) in ein Zielgewebe injiziert werden soll, wobei eine Extraktion oder Retraktion der Kanüle unabhängig von einer Bewegung des Kolbens erfolgt;

b) eine längliche Hülle (72), die ein internes Lumen (723) aufweist, das die Injektionskanüle enthält und eine distale Spitze besitzt, die eine Öffnung für die Injektionskanüle aufweist, wobei:

die Hülle um die Injektionskanüle herum beweglich ist; und eine Bedienung der Hülle unabhängig von einer Bewegung des Kolbens erfolgt; und

c) eine Bedieneinrichtung (71) zum Positionieren der Hülle, die aufweist:

ein Gehäuse (710), das zumindest einen ersten (715) und einen zweiten (716) Anschlag zum Steuern einer Exposition der Injektionskanüle aufweist, wobei diese innerhalb des Gehäuses in einem vorgegebenen Abstand zueinander angeordnet sind und wobei die Anschläge arretiert werden können; ein zentrales Lumen (717), das in dem Gehäuse ausgebildet ist und ein Verbindungselement aufweist, wobei das Verbindungselement (713) so ausgebildet ist, dass es in dem zentralen Lumen in dem Gehäuse beweglich ist und mit der Hülle gekoppelt ist, wobei das proximale Ende der Hülle an das distale Ende des Verbindungselements gekoppelt ist, sodass die Bewegung des Verbindungselements die Bewegung der Hülle steuert; und

eine Positioniereinrichtung (711), die innerhalb des Gehäuses befestigt und so ausgebildet ist, dass sie zwischen den Anschlängen in dem Gehäuse nach vorne in Richtung des distalen Endes der Bedieneinrichtung und nach hinten in Richtung des proximalen Endes der Bedieneinrichtung bewegt werden kann, wobei die Positioniereinrichtung funktionell mit dem Verbindungselement verbunden ist, um eine Bewegung des Verbindungselements in dieselbe Richtung zu führen, wobei eine Bewegung der Positioniereinrichtung nach vorne in Richtung des distalen En-

- des den ersten Anschlag aktiviert und die Hülle bewegt, um die Injektionskanüle innerhalb des Lumens der Hülle (711a, 72a) zu umschließen, und eine Bewegung der Positioniereinrichtung nach hinten in Richtung zum proximalen Ende den zweiten Anschlag aktiviert und die Hülle bewegt, sodass nicht mehr als eine vorgegebene Länge der distalen Spitze der Injektionskanüle (711c, 72c) durch die Öffnung für die Injektionskanüle zur Injektion in das Gewebe freigelegt wird.
2. Injektionsvorrichtung nach Anspruch 1, wobei die Länge und Breite der länglichen Hülle (72) ausreicht, um ein Organ durch einen endoskopischen Kanal zu erreichen.
3. Injektionsvorrichtung nach Anspruch 1 oder Anspruch 2, die zumindest 3 Anschläge, 4 Anschläge oder 5 Anschläge aufweist, wobei:
- der zweite (716) Anschlag der am weitesten proximal gelegene Anschlag ist und der erste (715) Anschlag der am weitesten distal gelegene Anschlag ist und der andere Anschlag oder die anderen Anschläge zwischen dem ersten Anschlag und dem zweiten Anschlag angeordnet sind; und
- jeder Anschlag in einem vorgegebenen Abstand zu einem benachbarten Anschlag oder benachbarten Anschlägen angeordnet ist, um eine Exposition der Kanüle auf unterschiedliche vorgegebene Längen zu steuern, wobei der zweite Anschlag die Exposition der Kanüle auf ihre längste vorgegebene Länge steuert, wobei die Positioniereinrichtung (711) zwischen den einander benachbarten Anschlägen zum Aktivieren des Anschlags bewegt werden kann, um unterschiedliche vorgegebene Längen der Injektionskanüle (81) zu exponieren.
4. Injektionsvorrichtung nach einem der Ansprüche 1 bis 3, wobei die Positioniereinrichtung (711) ein Arretier- und Löseelement (712) aufweist, das in der Positioniereinrichtung ausgebildet ist, um die Positioniereinrichtung mit den Anschlägen in Eingriff zu bringen.
5. Injektionsvorrichtung nach Anspruch 4, wobei das Arretier- und Löseelement (712) eine Feder ist, die eine nach oben gerichtete Kraft gegen die Positioniereinrichtung (711) und eine nach unten gerichtete Kraft gegen das Verbindungselement (713) aufbringt, um die Positioniereinrichtung in dem Anschlag zu arretieren, und die komprimiert werden kann, um die Positioniereinrichtung von dem Anschlag zu lösen.
6. Injektionsvorrichtung nach einem der Ansprüche 1 bis 5, wobei sich der Spritzenzylinder (91) proximal oder distal zur Bedieneinrichtung (71) befindet.
7. Injektionsvorrichtung nach einem der Ansprüche 1 bis 6, wobei sich der Spritzenzylinder (91) proximal zur Bedieneinrichtung (71) befindet und über ein Injektionsrohr (83) mit der Injektionskanüle (81) funktionell gekoppelt ist, wobei:
- das Injektionsrohr ein proximales und ein distales Ende aufweist, wobei das proximale Ende mit dem Spritzenzylinder und das distale Ende mit der Injektionskanüle verbunden ist; und die Bedieneinrichtung zum Halten des Injektionsrohrs ausgebildet ist und am proximalen Ende eine Öffnung aufweist, sodass das Injektionsrohr funktionell mit dem Spritzenzylinder verbunden ist.
8. Injektionsvorrichtung nach Anspruch 7, wobei der Spritzenzylinder (91) so zur Verbindung mit dem Injektionsrohr (83) ausgebildet ist, dass der Spritzenzylinder von der Vorrichtung abgenommen werden kann.
9. Injektionsvorrichtung nach Anspruch 7 oder Anspruch 8, wobei das Injektionsrohr (83) an seinem proximalen Ende eine Nabe (84) aufweist, die mit einem Adapter (93) am distalen Ende des Spritzenzylinders kompatibel ist, wobei die Nabe des Injektionsrohrs mit dem Adapter des Spritzenzylinders verbunden werden kann.
10. Injektionsvorrichtung nach einem der Ansprüche 7 bis 9, wobei:
- das Injektionsrohr (83) in der Bedieneinrichtung (71) befestigt ist;
- das Verbindungselement (713) in der Bedieneinrichtung eine Ausnehmung aufweist, über die das Injektionsrohr geführt wird, um an der Verbindungsstelle, an der das Verbindungselement an die Hülle gekoppelt ist, von der Bedieneinrichtung in die Hülle (72) zu gelangen; und das Verbindungselement um das Injektionsrohr herum beweglich ist.
11. Injektionsvorrichtung nach einem der Ansprüche 7 bis 10, wobei das Injektionsrohr (83) direkt mit der Injektionskanüle (81) verbunden ist.
12. Injektionsvorrichtung nach einem der Ansprüche 7 bis 10, wobei das Injektionsrohr (83) über einen Koppler (85) indirekt mit der Injektionskanüle (81) verbunden ist, wobei der Koppler ein proximales und

ein distales Ende aufweist, das proximale Ende mit dem distalen Ende des Injektionsrohrs und das distale Ende mit dem proximalen Ende der Injektionskanüle verbunden ist.

13. Injektionsvorrichtung nach einem der Ansprüche 7 bis 12, wobei das Injektionsrohr (83) und die Injektionskanüle (81) denselben Durchmesser oder unterschiedliche Durchmesser aufweisen.

14. Injektionsvorrichtung nach einem der Ansprüche 1 bis 13, die ferner ein Injektionsrohr (83) aufweist, über das die Injektionskanüle (91) funktionell mit dem Spritzenzylinder (91) verbunden ist, wobei:

das Injektionsrohr ein proximales und ein distales Ende aufweist, wobei das proximale Ende mit dem Spritzenzylinder und das distale Ende direkt oder indirekt mit der Injektionskanüle verbunden ist;

die Injektionskanüle einen Durchmesser von 25 Gauge oder weniger oder von 25 bis 34 Gauge und eine Länge im Bereich von 5 bis 40 mm aufweist; und

das Injektionsrohr einen größeren Durchmesser als die Injektionskanüle aufweist, wobei die Injektionskanüle mit dem Spritzenzylinder verbunden ist;

sich die Bedieneinrichtung (71) distal zu dem Spritzenzylinder und dem Kolben (92) befindet und aufweist:

einen Hohlraum für das Injektionsrohr und eine Öffnung am proximalen Ende, sodass das Injektionsrohr zur Verbindung mit dem Spritzenzylinder aus der Bedieneinrichtung ragt, wobei das Injektionsrohr in der Bedieneinrichtung befestigt ist; und ein zentrales Lumen (717) in dem Gehäuse (710), das ein Verbindungselement (713) umfasst, wobei:

das Verbindungselement in der Bedieneinrichtung eine Ausnehmung aufweist, über die das Injektionsrohr geführt wird, um an der Verbindungsstelle, an der das Verbindungselement an die Hülle (71) gekoppelt ist, von der Bedieneinrichtung in das distale Lumen der Hülle zu gelangen; und

das Verbindungselement so ausgebildet ist, dass es in dem zentralen Lumen in dem Gehäuse um das Injektionsrohr herum beweglich ist und mit der Hülle gekoppelt ist, wobei das proximale Ende der Hülle an das distale Ende des Verbindungselements gekoppelt ist, sodass die Bewegung des Verbindungselements die Be-

wegung der Hülle steuert.

15. Injektionsvorrichtung nach einem der Ansprüche 7 bis 14, wobei die Gesamtlänge des Injektionsrohrs (83) und der Injektionskanüle (81) der Länge der Bedieneinrichtung (71) und der Hülle (72) entspricht.

16. Injektionsvorrichtung nach einem der Ansprüche 1 bis 6, wobei:

der Spritzenzylinder (91) distal zur Bedieneinrichtung (71) angeordnet ist und das interne Lumen (723) der Hülle an seinem distalen Ende den Spritzenzylinder aufweist; und der Spritzenzylinder so in dem Lumen angeordnet ist, dass die Hülle um den Spritzenzylinder herum beweglich ist.

17. Injektionsvorrichtung nach Anspruch 16, wobei:

der offene Hohlraum (726) der Hülle (72) eine Auskleidung (96) aufweist, die in der Hülle so ausgebildet ist, dass die Hülle um die Auskleidung herum bewegt werden kann; und der Spritzenzylinder (91) in der Auskleidung in dem offenen Hohlraum montiert ist.

18. Injektionsvorrichtung nach Anspruch 17, wobei sich der offene Hohlraum (726) über die Länge der Hülle (72) erstreckt.

19. Injektionsvorrichtung nach einem der Ansprüche 16 bis 18, wobei der Kolben (92) am distalen Ende des Lumens der Hülle funktionell mit dem Spritzenzylinder (91) verbunden und so ausgebildet ist, dass der Kolben durch die Bedieneinrichtung (71) und innerhalb des Lumens der Hülle bewegt werden kann.

20. Injektionsvorrichtung nach einem der Ansprüche 16 bis 18, wobei:

der Kolben (92) funktionell mit dem Spritzenzylinder (91) über einen Hilfskolben (920) verbunden ist, der in dem Lumen der Hülle vorgesehen ist; und

der Kolben zur Kopplung mit dem Hilfskolben in dem Lumen der Hülle ausgebildet und so angeordnet ist, dass der Kolben durch die Bedieneinrichtung (71) und die Hülle (72) bewegt werden kann und der Hilfskolben durch die Hülle bewegt werden kann und ausgebildet ist, sich innerhalb des Spritzenzylinders zu bewegen, wobei ein Herunterdrücken des Kolbens den Hilfskolben in den Spritzenzylinder drückt, wodurch Fluid aus dem Fluidreservoir in dem Spritzenzylinder ausgegeben wird und ein Zurückziehen des Kolbens den Hilfskolben zurückzieht, um Fluid in das Fluidreservoir in dem Spritzenzylinder zu

füllen.

21. Injektionsvorrichtung nach Anspruch 20, wobei:

die Hülle (72) einen offenen Hohlraum (726) aufweist, der eine abnehmbare Spritze (900a, 900b) aufweist; und
 die abnehmbare Spritze den Spritzenzylinder (91), den Hilfskolben (920), der ein distales Ende aufweist, das so ausgebildet ist, dass es in dem Spritzenzylinder beweglich ist, und ein proximales Ende aufweist, das an den Kolben gekoppelt ist, und die Injektionskanüle (81) aufweist, die mit der Spritze funktionell verbunden ist.

22. Injektionsvorrichtung nach einem der Ansprüche 16 bis 21, wobei die Bedieneinrichtung (71) so zum Halten des Kolbens (92) ausgebildet ist, dass der Kolben innerhalb der Bedieneinrichtung beweglich ist, wobei die Bedieneinrichtung aufweist:

eine Öffnung an ihrem proximalen Ende zum Aufnehmen des Kolbens; und
 eine Ausnehmung in dem Verbindungselement (713) der Bedieneinrichtung durch die der Kolben geführt wird, um an der Verbindungsstelle, an der das Verbindungselement an die Hülle gekoppelt ist, von der Bedieneinrichtung in das Lumen der Hülle zu gelangen, wobei sich der Kolben und das Verbindungselement unabhängig voneinander bewegen.

23. Injektionsvorrichtung nach einem der Ansprüche 16 bis 22, die ferner aufweist:

einen Hilfskolben (920), der an dem Kolben (92) angebracht ist, um einen verlängerten Kolben zu bilden, der ausgebildet ist, von der Bedienungsperson der Vorrichtung bedient zu werden, um innerhalb des Spritzenzylinders (91) zum Füllen und Entleeren von Fluid aus dem Fluidreservoir in dem Spritzenzylinder bewegt zu werden, wobei ein Herunterdrücken des Kolbens den Hilfskolben in den Spritzenzylinder drückt, wodurch Fluid aus dem Fluidreservoir in dem Spritzenzylinder ausgegeben wird und ein Zurückziehen des Kolbens den Hilfskolben zurückzieht, um Fluid in das Fluidreservoir in dem Spritzenzylinder zu füllen;
 eine Öffnung am proximalen Ende der Bedieneinrichtung (71) zum Aufnehmen des Kolbens und mit einem Hohlraum, der zum Halten des Kolbens so ausgebildet ist, dass der Kolben innerhalb der Bedieneinrichtung beweglich ist; und
 eine Ausnehmung in dem Verbindungselement (713), durch die der Kolben geführt wird, um an

der Verbindungsstelle, an der das Verbindungselement an die Hülle gekoppelt ist, von der Bedieneinrichtung in das distale Lumen der Hülle zu gelangen, wobei sich der Kolben und das Verbindungselement unabhängig voneinander bewegen;

wobei:

die Injektionskanüle (81) einen Durchmesser von 25 bis 34 Gauge und eine Länge im Bereich von 5 bis 40 mm aufweist; und
 die längliche Hülle (72) ein internes Lumen (723) aufweist, das den Kolben, den Hilfskolben, den Spritzenzylinder und die Injektionskanüle enthält, und eine distale Spitze (73) besitzt, die eine Öffnung für die Injektionskanüle umfasst, wobei:

die Hülle an ihrem proximalen Ende umschlossen ist und einen Kanal für den Kolben bietet, wobei der Kolben durch die Hülle bewegt werden kann;
 die Hülle an ihrem distalen Ende einen offenen Hohlraum (726) aufweist, wobei der offene Hohlraum den Hilfskolben, den Spritzenzylinder und die Injektionskanüle enthält, wobei:

der offene Hohlraum der Hülle eine Auskleidung aufweist, die in der Hülle so ausgebildet ist, dass die Hülle um die Auskleidung herum bewegt werden kann;

der Hilfskolben, der Spritzenzylinder und die Injektionskanüle in der Auskleidung in dem offenen Hohlraum montiert sind; und
 der Hilfskolben, der Spritzenzylinder und die Injektionskanüle als Einheit von dem offenen Hohlraum abgenommen werden können; und
 die Hülle um den Kolben, den Hilfskolben, den Spritzenzylinder und die Injektionskanüle bewegt werden kann.

24. Injektionsvorrichtung nach einem der Ansprüche 1 bis 23 zur Verwendung bei der Verabreichung eines therapeutischen Wirkstoffes an das Parenchym eines Organs oder Gewebes.

25. Injektionsvorrichtung nach einem der Ansprüche 1 bis 23 zur Verwendung bei der Verabreichung eines therapeutischen Wirkstoffes an ein Organ oder Gewebe während eines chirurgischen Eingriffs.

26. Injektionsvorrichtung zur Verwendung nach Anspruch 25, wobei es sich bei dem chirurgischen Eingriff um einen minimalinvasiven chirurgischen Ein-

griff handelt.

27. Injektionsvorrichtung zur Verwendung nach einem der Ansprüche 24 bis 26, wobei:

es sich bei dem therapeutischen Wirkstoff um eine Nucleinsäure handelt;
und der chirurgische Eingriff die Verabreichung der Nucleinsäure zur Gentherapie bewirkt.

Revendications

1. Dispositif d'injection comprenant :

un corps cylindrique de seringue (91), dans lequel le corps cylindrique de seringue fournit un réservoir de fluide ;
un piston plongeur (92) configuré pour être commandé par l'opérateur du dispositif et pour se déplacer à l'intérieur du corps de cylindrique de seringue afin de charger et de libérer le fluide du réservoir de fluide dans le corps cylindrique de seringue ; et est **caractérisé en ce qu'il** comprend en outre :

a) une aiguille d'injection (81) qui est fixe et couplée de manière opérationnelle au corps cylindrique de seringue (91) fournissant une voie de passage de fluide pour le fluide contenu dans le corps cylindrique de seringue à injecter dans un tissu cible lorsque le piston plongeur (92) est enfoncé, dans lequel l'extraction ou la rétraction de l'aiguille est indépendante du mouvement du piston plongeur ;

b) une gaine allongée (72) comprenant une lumière interne (723) qui contient l'aiguille d'injection et ayant une pointe distale qui contient une ouverture pour l'aiguille d'injection, dans lequel :

la gaine est mobile autour de l'aiguille d'injection ; et

la commande de la gaine est indépendante du mouvement du piston plongeur ; et

c) un organe de commande (71) pour positionner la gaine, comprenant :

un boîtier (710) comprenant au moins une première (715) et une seconde (716) butée pour contrôler l'exposition de l'aiguille d'injection et qui sont prévues à l'intérieur du boîtier à une distance prédéterminée l'une de l'autre, dans lequel les butées peuvent être

verrouillées ;

une lumière centrale (717) dans le boîtier comprenant un élément de raccordement,

dans lequel l'élément de raccordement (713) est configuré pour être mobile dans la lumière centrale dans le boîtier et est couplé à la gaine, dans lequel l'extrémité proximale de la gaine est couplée à l'extrémité distale de l'élément de raccordement de sorte que le mouvement de l'élément de raccordement contrôle le mouvement de la gaine ; et

un dispositif de positionnement (711) monté à l'intérieur du boîtier, configuré pour se déplacer vers l'avant, vers l'extrémité distale de l'organe de commande et vers l'arrière, vers l'extrémité proximale de l'organe de commande, entre les butées dans le boîtier, dans lequel le dispositif de positionnement est raccordé de manière opérationnelle à l'élément de raccordement pour guider le mouvement de l'élément de raccordement dans la même direction, moyennant quoi le mouvement du dispositif de positionnement vers l'avant, vers l'extrémité distale met en prise la première butée et déplace la gaine pour enfermer l'aiguille d'injection à l'intérieur de la lumière de la gaine (711a, 72a) et le mouvement du dispositif de positionnement vers l'arrière, vers l'extrémité proximale met en prise la deuxième butée et déplace la gaine pour ne pas exposer plus d'une longueur prédéterminée de la pointe distale de l'aiguille d'injection (711c, 72c) à travers l'ouverture dans l'aiguille d'injection pour l'injection dans le tissu.

2. Dispositif d'injection selon la revendication 1, dans lequel la gaine allongée (72) a une longueur et une largeur suffisante pour atteindre un organe à travers un orifice endoscopique.

3. Dispositif d'injection selon la revendication 1 ou la revendication 2, comprenant au moins 3 butées, 4 butées ou 5 butées, dans lequel :

la deuxième butée (716) est la butée la plus proximale et la première butée (715) est la butée la plus distale et l'autre butée ou les autres butées sont positionnées entre la première butée et la deuxième butée ; et
chaque butée est positionnée à une distance prédéterminée d'une butée ou des butées adja-

- centes pour contrôler l'exposition de l'aiguille à différentes longueurs prédéterminées, dans lequel la deuxième butée contrôle l'exposition de l'aiguille jusqu'à sa longueur prédéterminée la plus longue, moyennant quoi le dispositif de positionnement (711) peut se déplacer entre les butées adjacentes pour se mettre en prise avec la butée afin d'exposer différentes longueurs prédéterminées de l'aiguille d'injection (81).
- 5
4. Dispositif d'injection selon l'une quelconque des revendications 1 à 3, dans lequel le dispositif de positionnement (711) comprend un élément de verrouillage et de libération (712) qui est configuré, dans le dispositif de positionnement, pour mettre en prise le dispositif de positionnement avec les butées.
- 10
5. Dispositif d'injection selon la revendication 4, dans lequel l'élément de verrouillage et de libération (712) est un ressort qui fournit une force ascendante contre le dispositif de positionnement (711) et une force descendante contre l'élément de raccordement (713) pour verrouiller le dispositif de positionnement dans la butée, et peut être comprimé pour libérer le dispositif de positionnement de la butée.
- 15
6. Dispositif d'injection selon l'une quelconque des revendications 1 à 5, dans lequel le corps cylindrique de seringue (91) est proximal ou distal par rapport à l'organe de commande (71).
- 20
7. Dispositif d'injection selon l'une quelconque des revendications 1 à 6, dans lequel le corps cylindrique de seringue (91) est à proximité de l'organe de commande (71) et est couplé, de manière opérationnelle, à l'aiguille d'injection (81) par un tube d'injection (83), dans lequel :
- 25
- le tube d'injection comprend une extrémité proximale et une extrémité distale, l'extrémité proximale étant raccordée au corps cylindrique de seringue et l'extrémité distale étant raccordée à l'aiguille d'injection ; et l'organe de commande est configuré pour maintenir le tube d'injection et comprend une ouverture au niveau de l'extrémité proximale de sorte que le tube d'injection est raccordé, de manière opérationnelle, au corps cylindrique de seringue.
- 30
8. Dispositif d'injection selon la revendication 7, dans lequel le corps cylindrique de seringue (91) est configuré pour être raccordé au tube d'injection (83) de sorte que le corps cylindrique de seringue peut se détacher du dispositif.
- 35
9. Dispositif d'injection selon la revendication 7 ou la revendication 8, dans lequel le tube d'injection (83) comprend un raccord (84) sur son extrémité proximale qui est compatible avec un adaptateur (93) sur l'extrémité distale du corps cylindrique de seringue et le raccord du tube d'injection se raccorde à l'adaptateur du corps cylindrique de seringue.
- 40
10. Dispositif d'injection selon l'une quelconque des revendications 7 à 9, dans lequel :
- 45
- le tube d'injection (83) est fixé dans l'organe de commande (71) ; l'élément de raccordement (713) dans l'organe de commande comprend un évidement par lequel le tube d'injection est acheminé pour passer de l'organe de commande dans la gaine (72) au niveau de la jonction où l'élément de raccordement est couplé à la gaine ; et l'élément de raccordement est mobile autour du tube d'injection.
- 50
11. Dispositif d'injection selon l'une quelconque des revendications 7 à 10, dans lequel le tube d'injection (83) est directement raccordé à l'aiguille d'injection (81).
- 55
12. Dispositif d'injection selon l'une quelconque des revendications 7 à 10, dans lequel le tube d'injection (83) est indirectement raccordé à l'aiguille d'injection (81) via un coupleur (85), le coupleur ayant une extrémité proximale et une extrémité distale, l'extrémité proximale étant raccordée à l'extrémité distale du tube d'injection et l'extrémité distale étant raccordée à l'extrémité proximale de l'aiguille d'injection.
13. Dispositif d'injection selon l'une quelconque des revendications 7 à 12, dans lequel le tube d'injection (83) et l'aiguille d'injection (81) ont le même calibre ou des calibres différents.
14. Dispositif d'injection selon l'une quelconque des revendications 1 à 13, comprenant en outre un tube d'injection (83) grâce auquel l'aiguille d'injection (81) est couplée de manière opérationnelle au corps cylindrique de seringue (91), dans lequel :
- le tube d'injection comprend une extrémité proximale et une extrémité distale, l'extrémité proximale étant raccordée au corps cylindrique de seringue et l'extrémité distale étant directement ou indirectement raccordée à l'aiguille d'injection ; l'aiguille d'injection a un diamètre de calibre 25 ou inférieur ou un calibre de 25 à 34 et a une longueur dans la plage de 5 mm à 40 mm ; et le tube d'injection a un plus grand diamètre que l'aiguille d'injection, dans lequel l'aiguille d'injection est raccordée au corps cylindrique de seringue ;

l'organe de commande (71) est distal par rapport au corps cylindrique de seringue et au piston plongeur (92) et comprend :

une cavité pour le tube d'injection et une ouverture au niveau de l'extrémité proximale de sorte que le tube d'injection s'étend hors de l'organe de commande pour se raccorder au corps cylindrique de seringue, dans lequel le tube d'injection est fixé dans l'organe de commande ; et une lumière centrale (717) dans le boîtier (710) comprenant un élément de raccordement (713), dans lequel :

l'élément de raccordement dans l'organe de commande comprend un évidement grâce auquel le tube d'injection est acheminé pour passer de l'organe de commande dans la lumière distale de la gaine au niveau de la jonction où l'élément de raccordement est couplé à la gaine (71) ; et l'élément de raccordement est configuré pour être mobile dans la lumière centrale dans le boîtier autour du tube d'injection et est couplé à la gaine, dans lequel l'extrémité proximale de la gaine est couplée à l'extrémité distale de l'élément de raccordement de sorte que le mouvement de l'élément de raccordement commande le mouvement de la gaine.

15. Dispositif d'injection selon l'une quelconque des revendications 7 à 14, dans lequel la longueur totale du tube d'injection (83) et de l'aiguille d'injection (81) est aussi longue que l'organe de commande (71) et la gaine (72).

16. Dispositif d'injection selon l'une quelconque des revendications 1 à 6, dans lequel :

le corps cylindrique de seringue (91) est positionné de manière distale par rapport à l'organe de commande (71) et la lumière interne (723) de la gaine comprend le corps cylindrique de seringue dans son extrémité distale ; et le corps cylindrique de seringue est configuré dans la lumière de sorte que la gaine est mobile autour du corps cylindrique de seringue.

17. Dispositif d'injection selon la revendication 16, dans lequel :

la cavité ouverte (726) de la gaine (72) comprend un revêtement (96) qui est configuré dans la gaine de sorte que la gaine est mobile autour

du revêtement ; et

le corps cylindrique de seringue (91) est monté dans le revêtement dans la cavité ouverte.

5 18. Dispositif d'injection selon la revendication 17, dans lequel la cavité ouverte (726) étend la longueur de la gaine (72).

10 19. Dispositif d'injection selon l'une quelconque des revendications 16 à 18, dans lequel le piston plongeur (92) est raccordé, de manière opérationnelle au corps cylindrique de seringue (91) dans l'extrémité distale de la lumière de la gaine et agencé de sorte que le piston plongeur est mobile à travers l'organe de commande (71) et à l'intérieur de la lumière de la gaine.

15 20. Dispositif d'injection selon l'une quelconque des revendications 16 à 18, dans lequel ;
20 le piston plongeur (92) est raccordé, de manière opérationnelle, au corps cylindrique de seringue (91) par un piston plongeur auxiliaire (920) prévu dans la lumière de la gaine ; et
25 le piston plongeur est adapté pour se coupler avec le piston plongeur auxiliaire dans la lumière de la gaine et agencé de sorte que le piston plongeur est mobile à travers l'organe de commande (71) et la gaine (72) et le piston plongeur auxiliaire est mobile à travers la gaine et configuré pour se déplacer à l'intérieur du corps cylindrique de seringue, moyennant quoi l'enfoncement du piston plongeur enfonce le piston plongeur auxiliaire dans le corps cylindrique de seringue, libérant le fluide du réservoir de fluide dans le corps cylindrique de seringue et la traction sur le piston plongeur ramène le piston plongeur auxiliaire pour charger le fluide dans le réservoir de fluide dans le corps cylindrique de seringue.

35 40 21. Dispositif d'injection selon la revendication 20, dans lequel :

la gaine (72) comprend une cavité ouverte (726) comprenant une seringue détachable (900a, 900b) ; et

45 la seringue détachable comprend un corps cylindrique de seringue (91), le piston plongeur auxiliaire (920) ayant une extrémité distale configurée pour être mobile dans le corps cylindrique de seringue et une extrémité proximale couplée au piston plongeur, et l'aiguille d'injection (81) est couplée, de manière opérationnelle, à la seringue.

50 55 22. Dispositif d'injection selon l'une quelconque des revendications 16 à 21, dans lequel l'organe de commande (71) est configuré pour maintenir le piston plongeur (92) de sorte que le piston plongeur est mobile à l'intérieur de l'organe de commande, l'or-

gane de commande comprenant :

une ouverture au niveau de son extrémité proximale pour recevoir le piston plongeur ; et
 un évidement dans l'élément de raccordement (713) de l'organe de commande grâce auquel le piston plongeur est acheminé pour passer de l'organe de commande dans la lumière de la gaine, au niveau de la jonction où l'élément de raccordement est couplé à la gaine, dans lequel le piston plongeur et l'élément de raccordement se déplacent indépendamment l'un de l'autre.

- 23.** Dispositif d'injection selon l'une quelconque des revendications 16 à 22, comprenant en outre :

un piston plongeur auxiliaire (920) fixé au piston plongeur (92) pour former un piston plongeur étendu configuré pour être commandé par l'opérateur du dispositif afin de se déplacer à l'intérieur du corps cylindrique de seringue (91) pour charger et libérer le fluide du réservoir de fluide dans le corps cylindrique de seringue, moyennant quoi l'enfoncement du piston plongeur enfonce le piston plongeur auxiliaire dans le corps cylindrique de seringue libérant le fluide du réservoir de fluide dans le corps cylindrique de seringue et la traction sur le piston plongeur ramène le piston plongeur auxiliaire pour charger le fluide dans le réservoir de fluide dans le corps cylindrique de seringue ; une ouverture au niveau de l'extrémité proximale de l'organe de commande (71) pour recevoir le piston plongeur et comprenant une cavité configurée pour maintenir le piston plongeur de sorte que le piston plongeur est mobile à l'intérieur de l'organe de commande ; et
 un évidement dans l'élément de raccordement (713) grâce auquel le piston plongeur est acheminé pour passer de l'organe de commande dans la lumière distale de la gaine au niveau de la jonction où l'élément de raccordement est couplé à la gaine, dans lequel le piston plongeur et l'élément de raccordement se déplacent indépendamment l'un de l'autre ;

dans lequel :

l'aiguille d'injection (81) a un calibre de 25 à 34 et a une longueur dans la plage de 5 mm à 40 mm ; et
 la gaine allongée (72) comprend une lumière interne (723) qui contient le piston plongeur, le piston plongeur auxiliaire, le corps cylindrique de seringue et l'aiguille d'injection et ayant une pointe distale (73) qui contient une ouverture pour l'aiguille d'injection, dans lequel :

la gaine est enfermée au niveau de son extrémité proximale et fournit un conduit pour le piston plongeur, dans lequel le piston plongeur est mobile à travers la gaine ;
 la gaine comprend une cavité ouverte (726) au niveau de l'extrémité distale, la cavité ouverte comprenant le piston plongeur auxiliaire, le corps cylindrique de seringue et une aiguille d'injection,

dans lequel :

la cavité ouverte de la gaine comprend un revêtement qui est configuré dans la gaine de sorte que la gaine est mobile autour du revêtement ; le piston plongeur auxiliaire, le corps cylindrique de seringue et l'aiguille d'injection sont montés dans le revêtement dans la cavité ouverte ; et le piston plongeur auxiliaire, le corps cylindrique de seringue et l'aiguille d'injection sont détachables sous la forme d'une unité, de la cavité ouverte ; et
 la gaine est mobile autour du piston plongeur, du piston plongeur auxiliaire, du corps cylindrique de seringue et de l'aiguille d'injection.

- 24.** Dispositif d'injection selon l'une quelconque des revendications 1 à 23, destiné à être utilisé pour administrer un traitement au parenchyme d'un organe ou d'un tissu.
- 25.** Dispositif d'injection selon l'une quelconque des revendications 1 à 23, destiné pour être utilisé afin d'administrer un traitement à un organe ou un tissu pendant une chirurgie.
- 26.** Dispositif d'injection destiné à être utilisé selon la revendication 25, dans lequel la chirurgie est une chirurgie minimalement invasive.
- 27.** Dispositif d'injection destiné à être utilisé selon l'une quelconque des revendications 24 à 26, dans lequel :

le traitement est un acide nucléique ;
 et la chirurgie effectue l'administration de l'acide nucléique pour la thérapie génique.

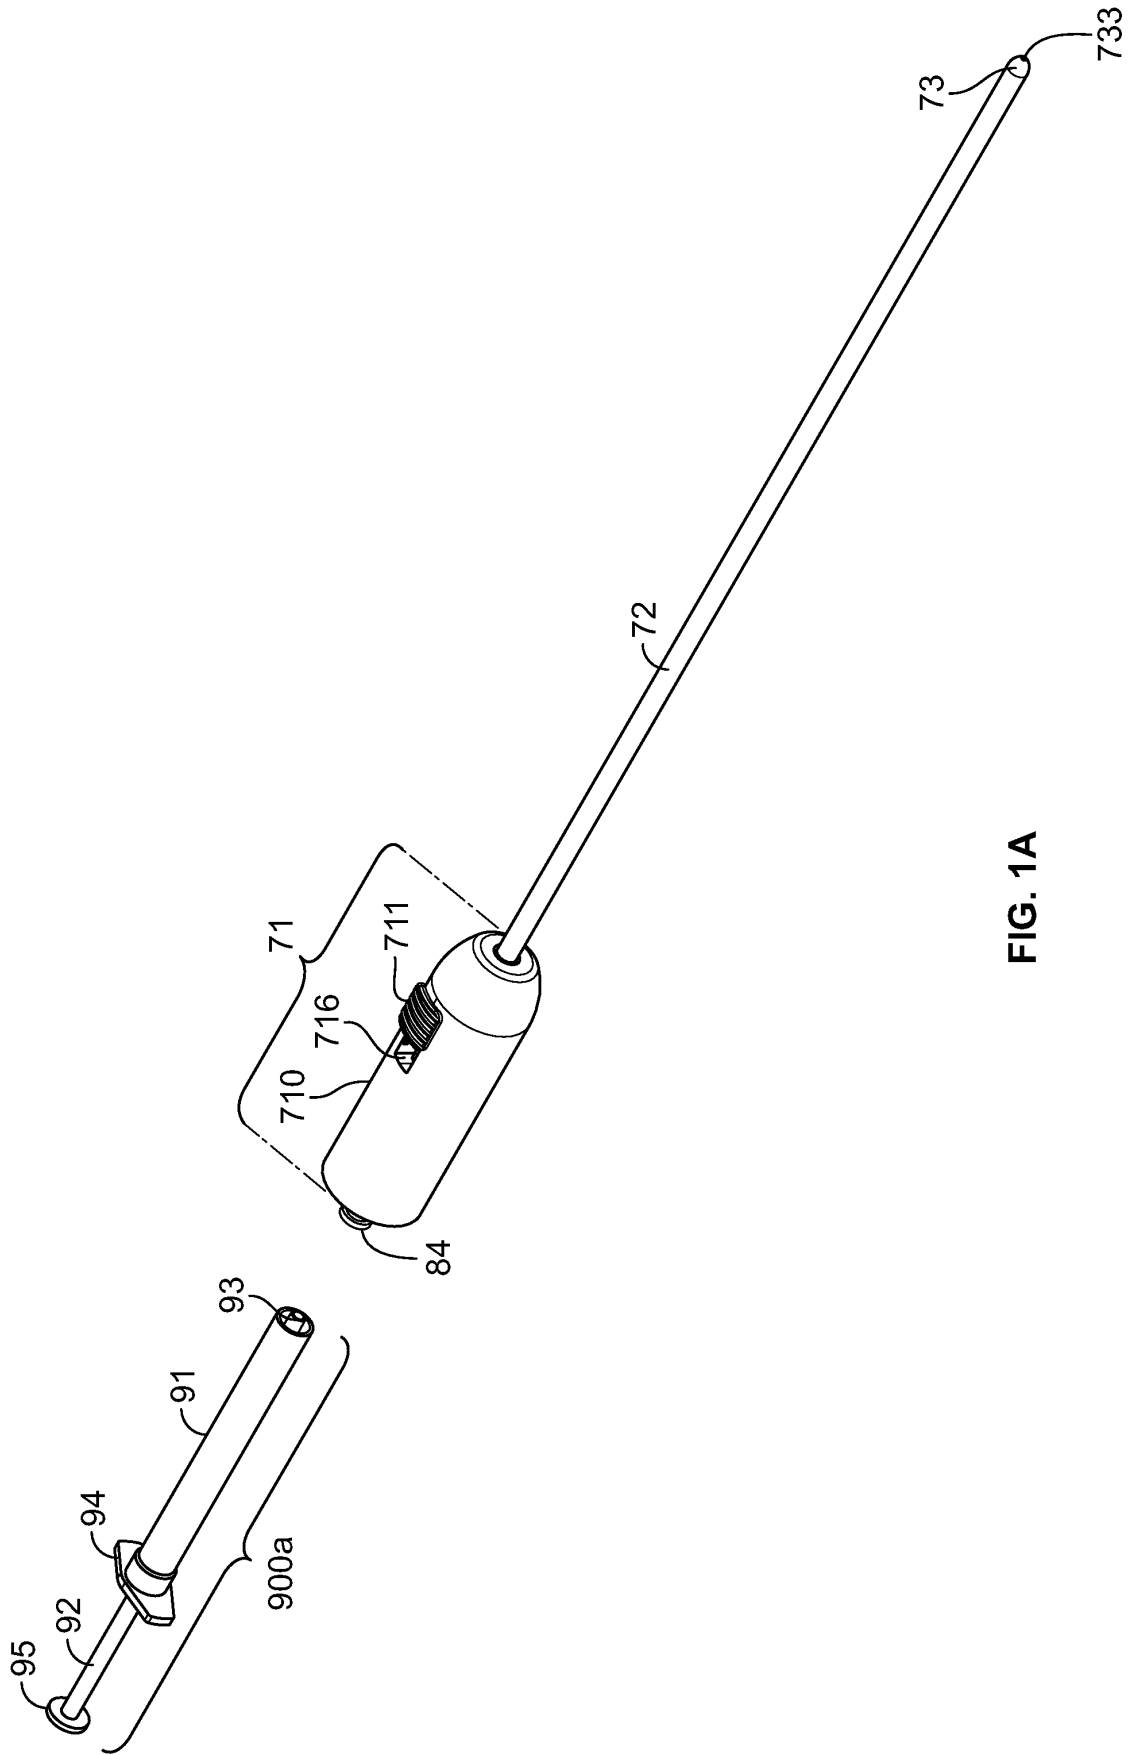


FIG. 1A

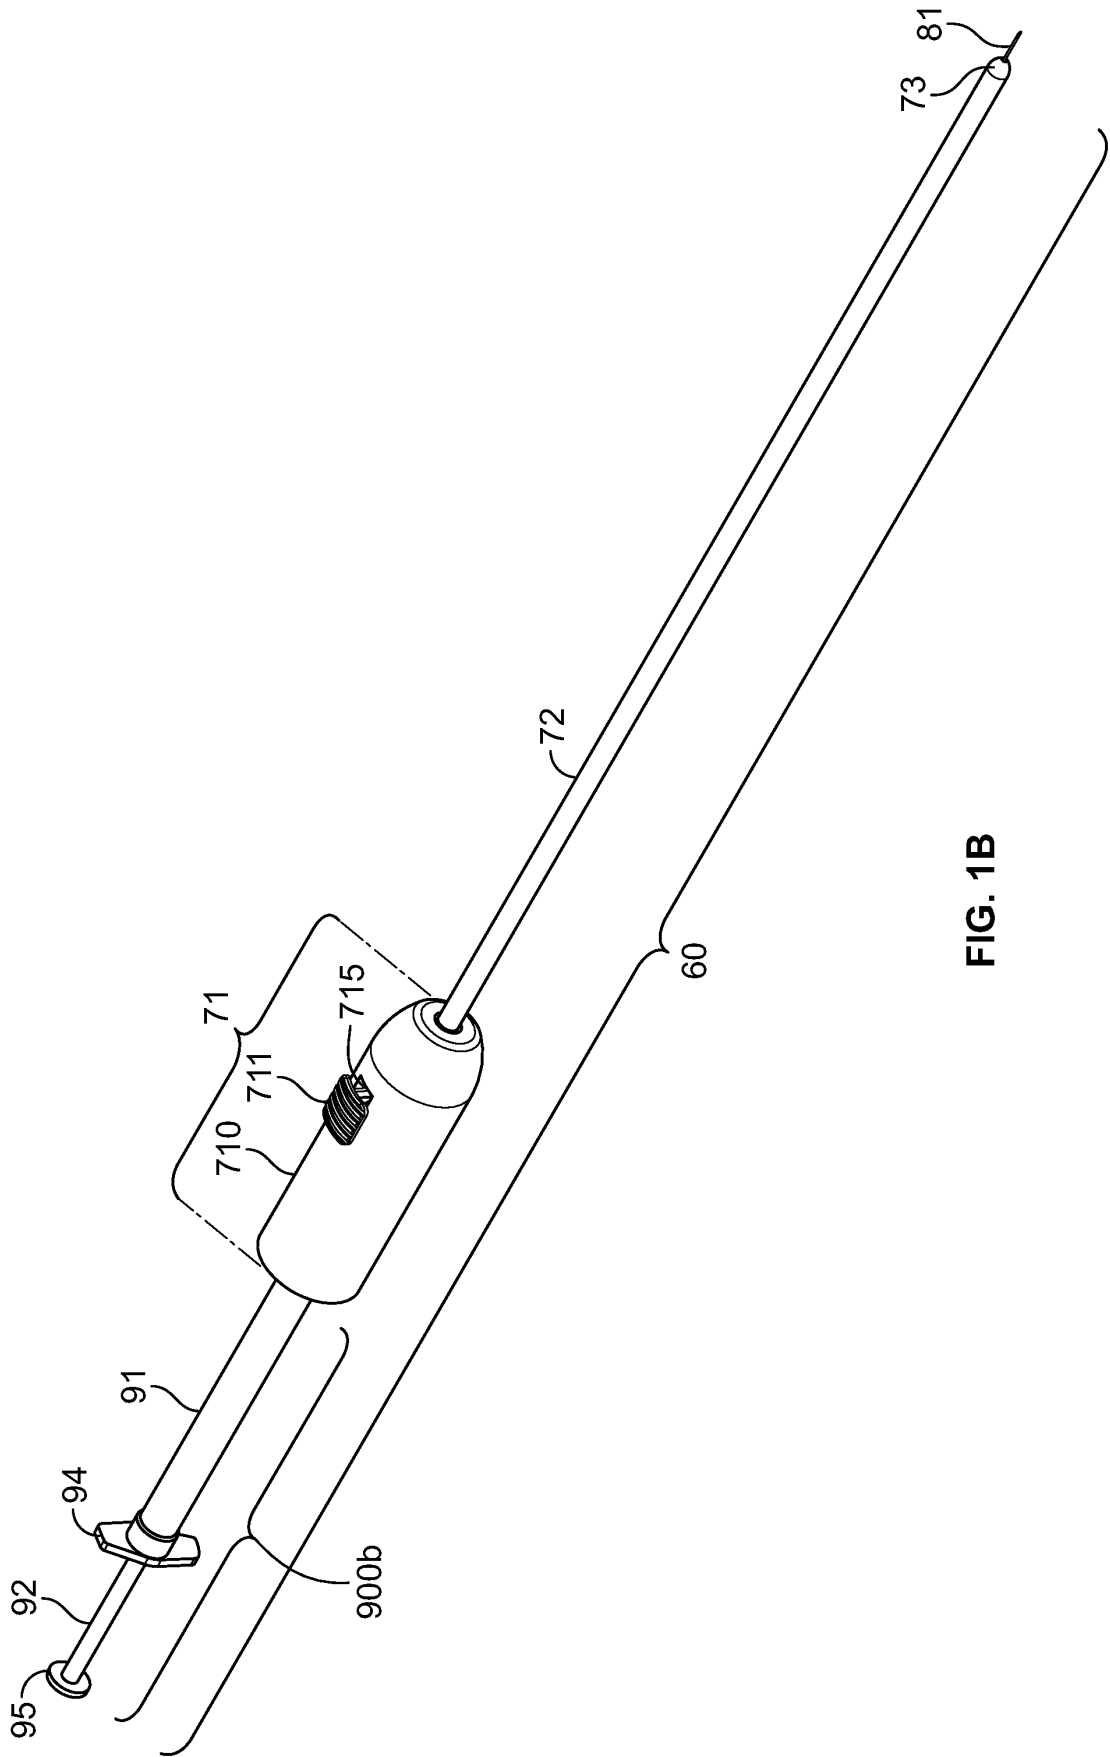


FIG. 1B

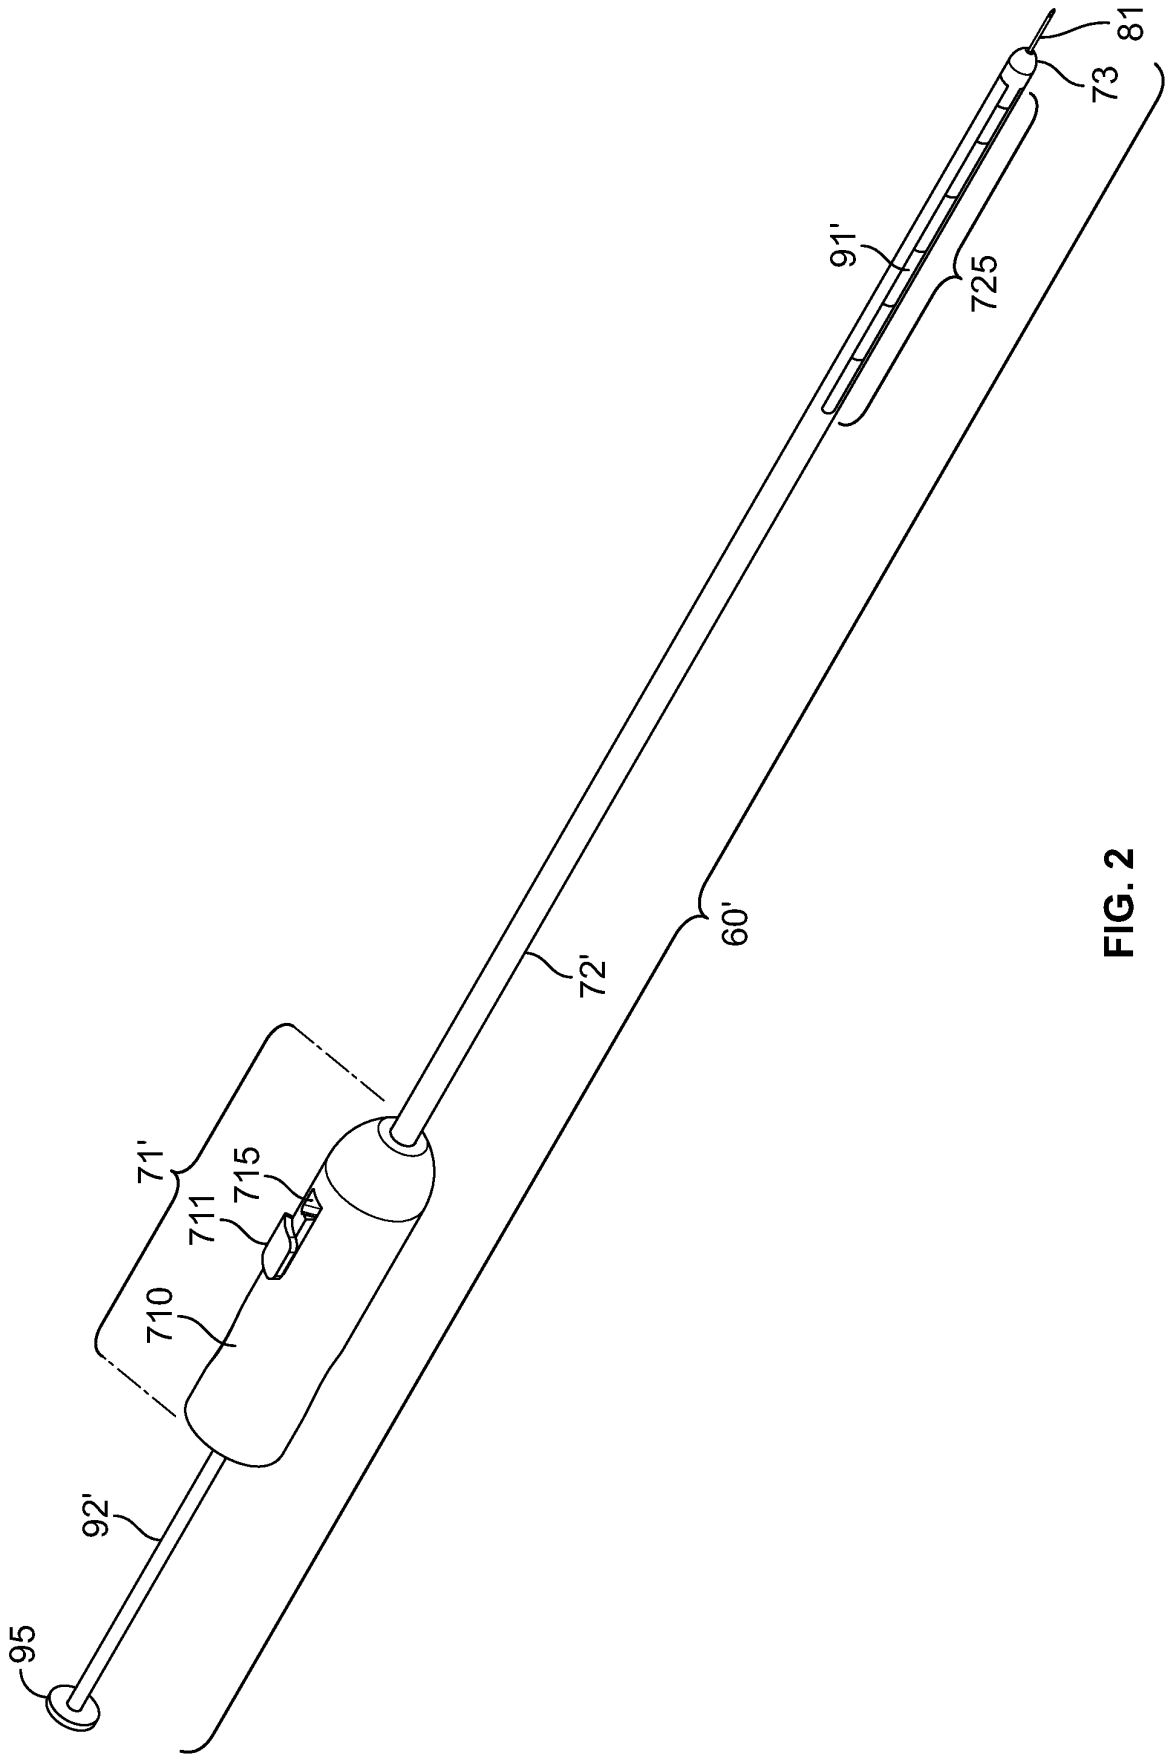


FIG. 2

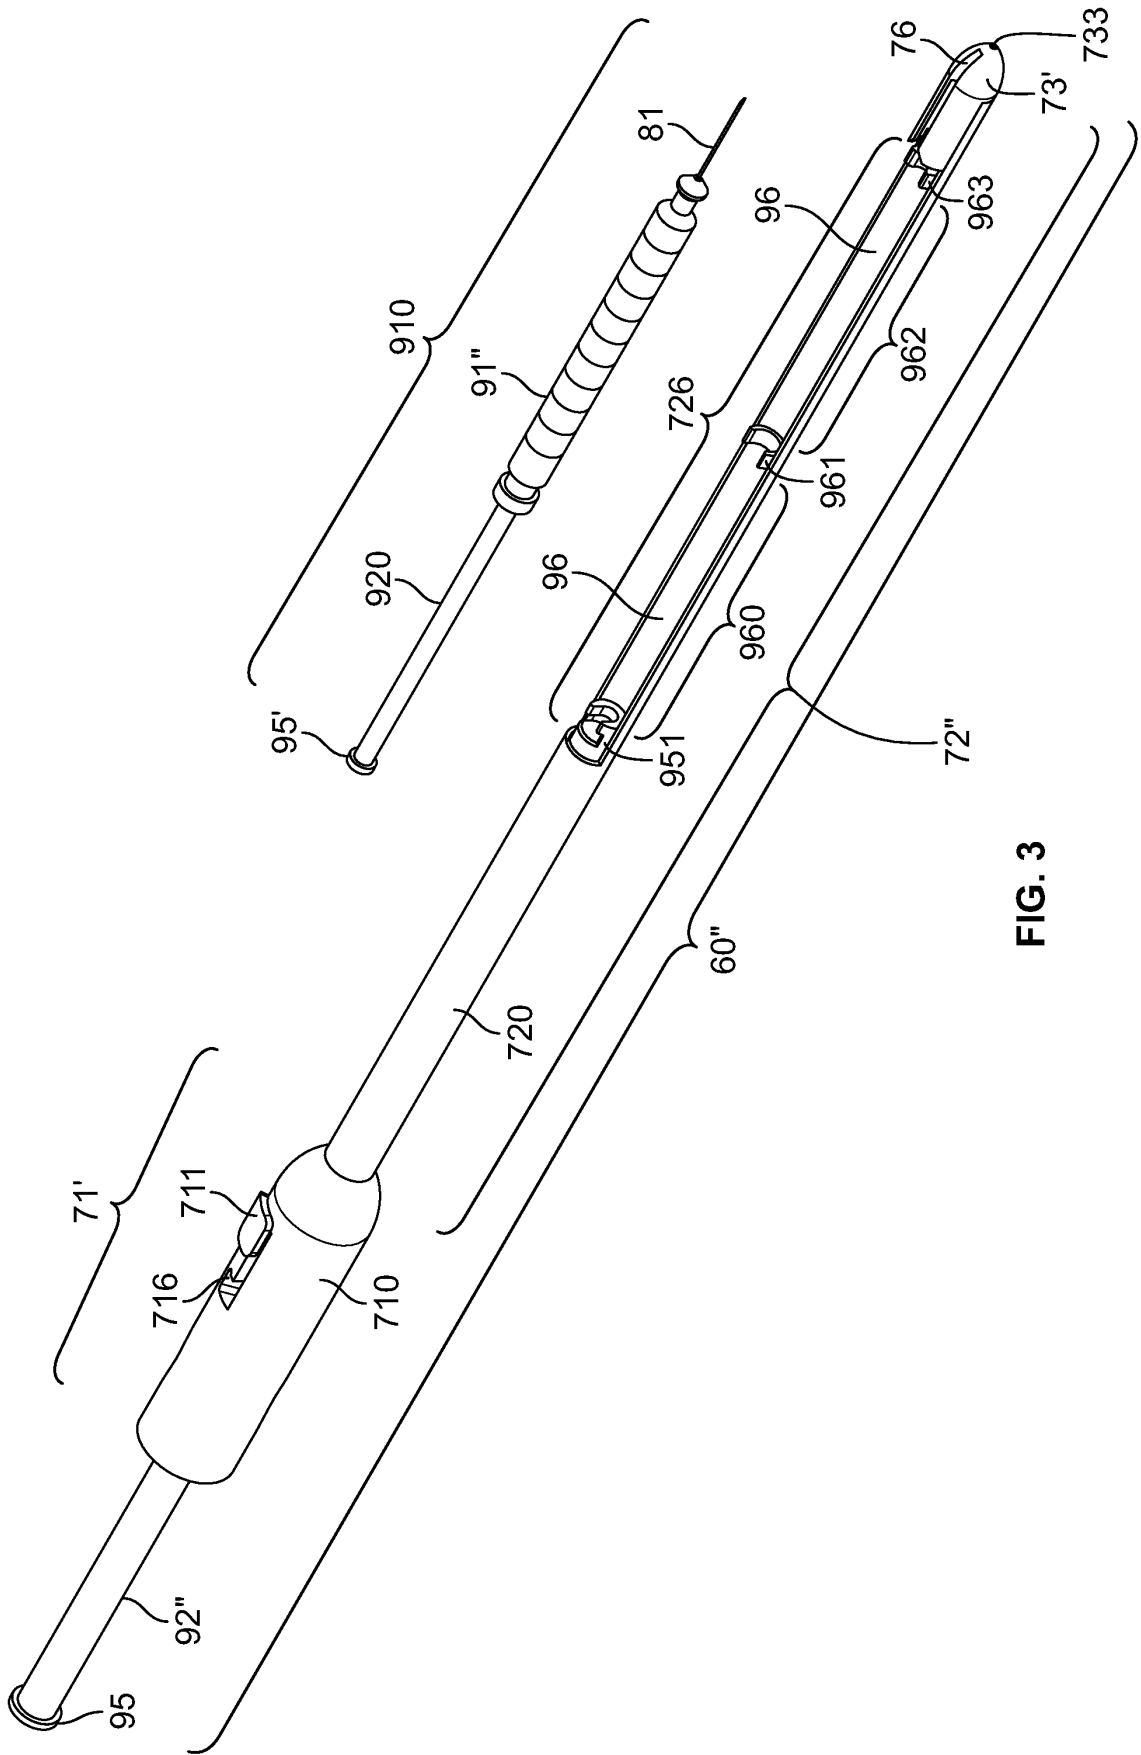


FIG. 3

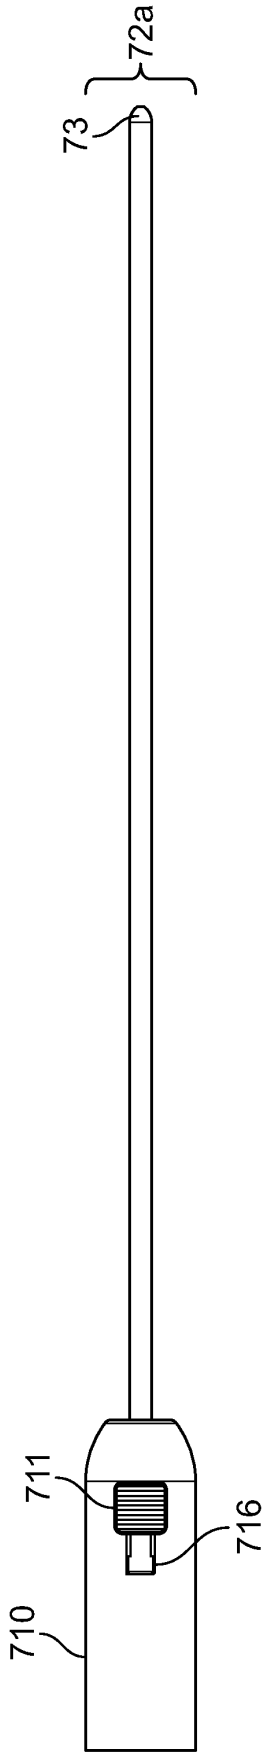


FIG. 4A

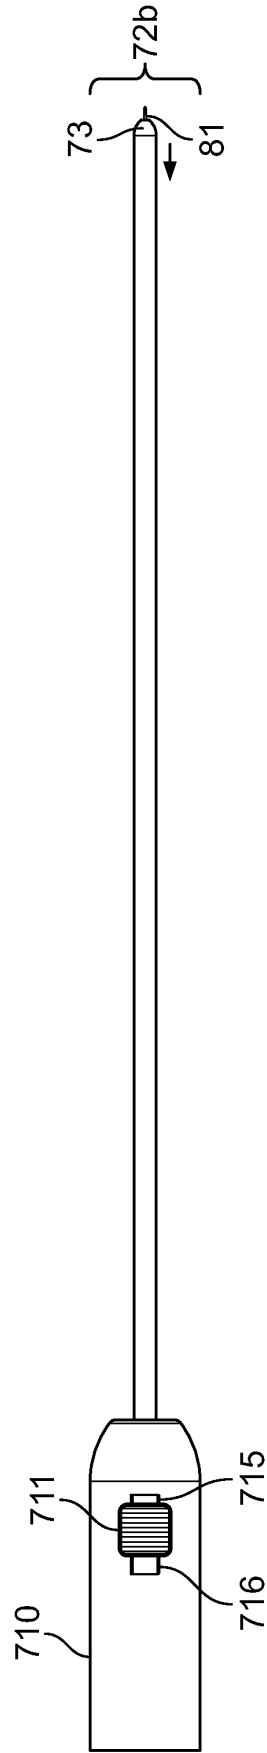


FIG. 4B

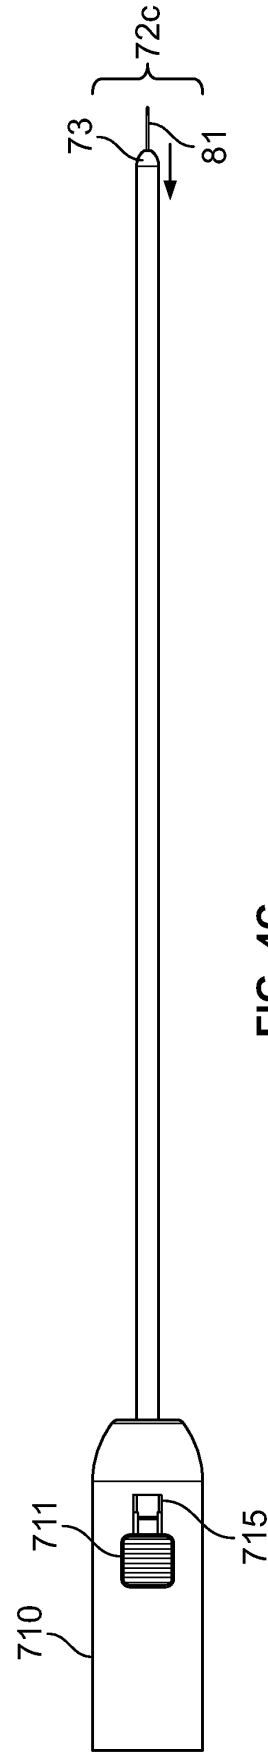


FIG. 4C

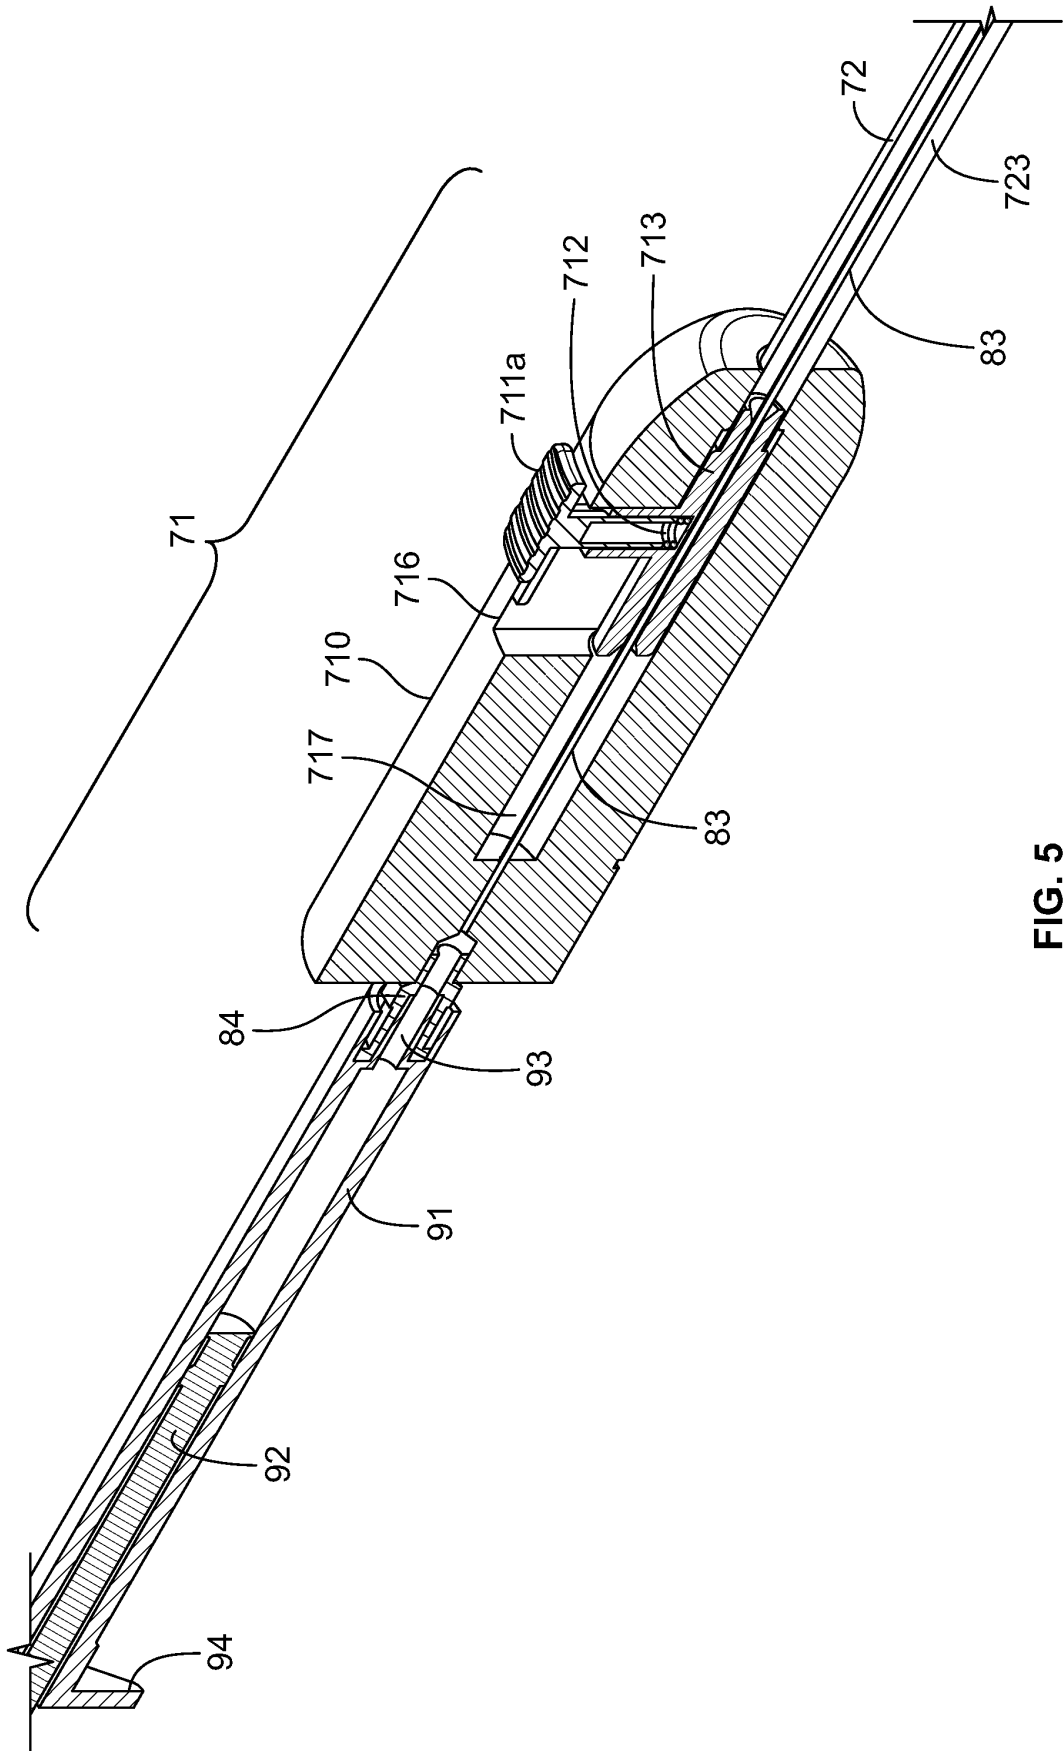


FIG. 5

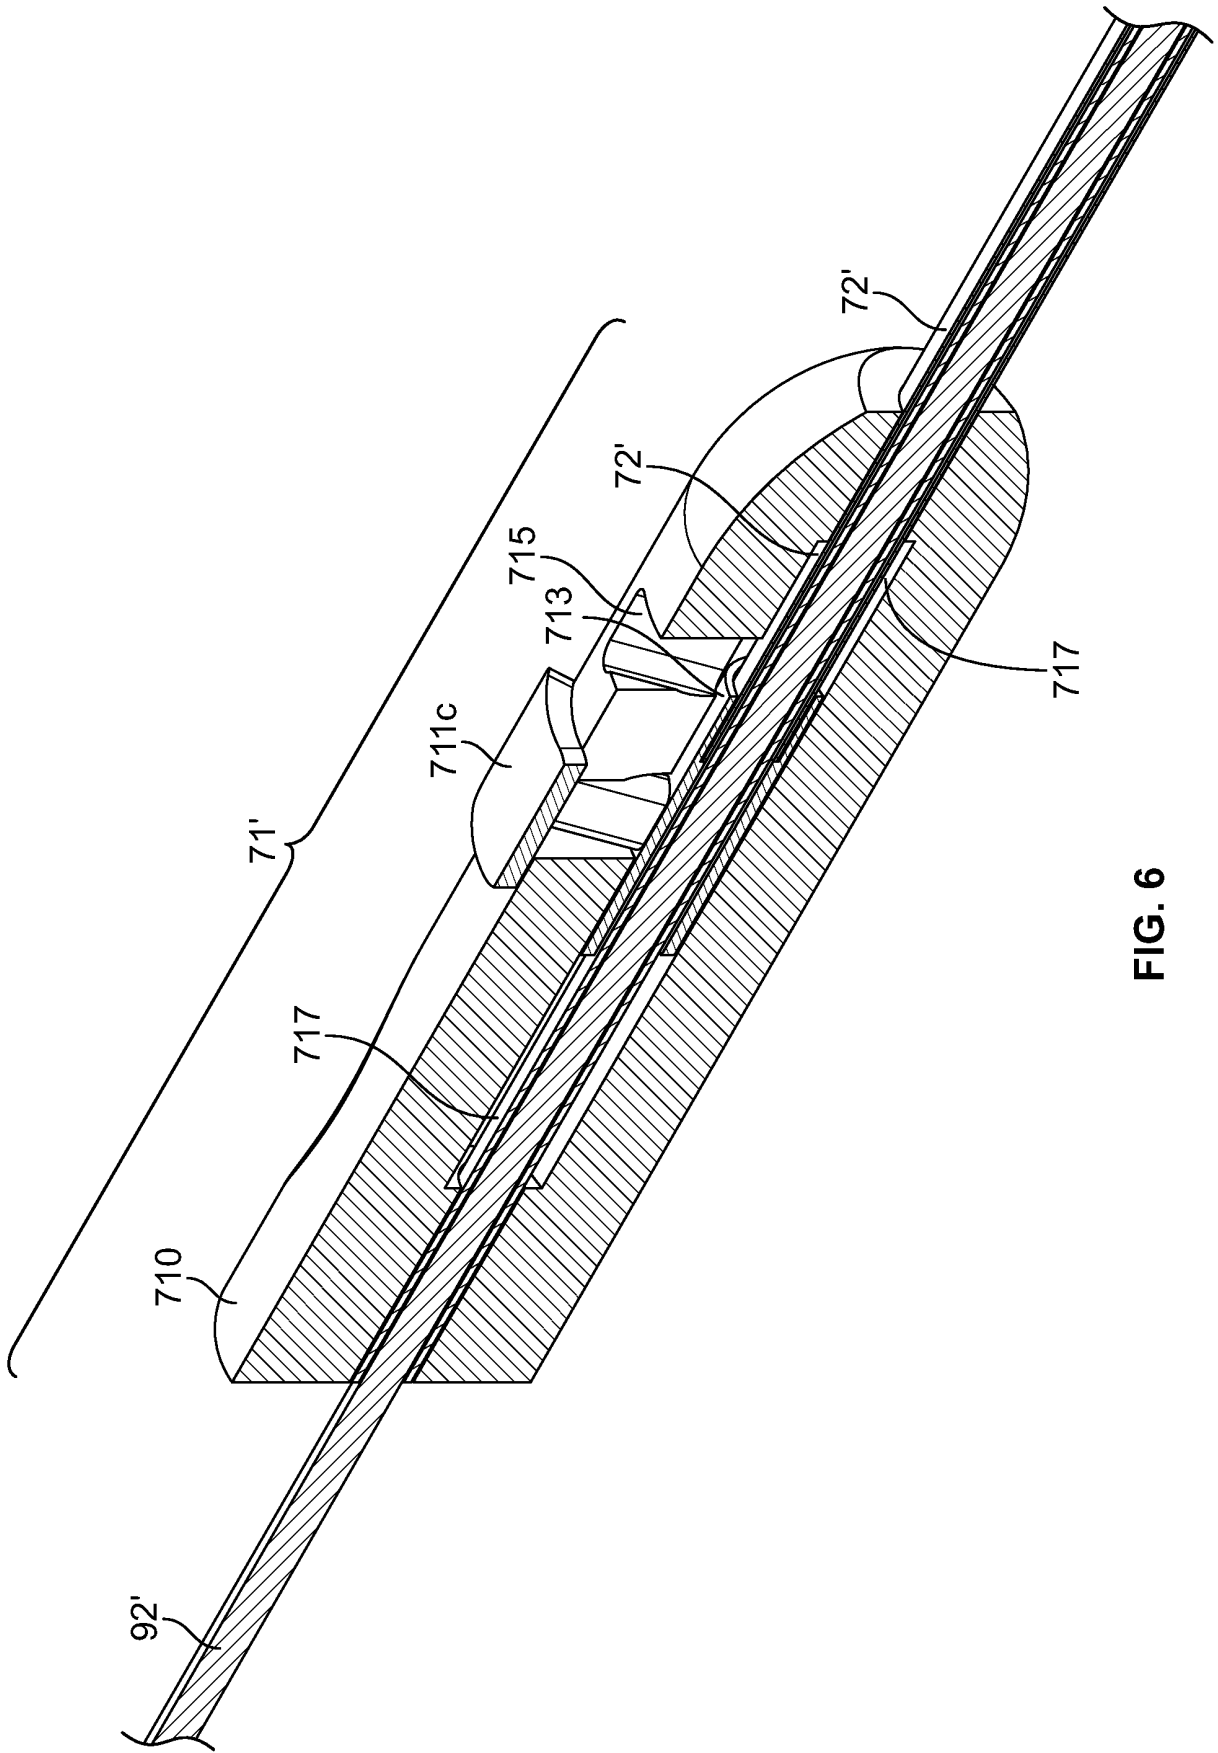


FIG. 6

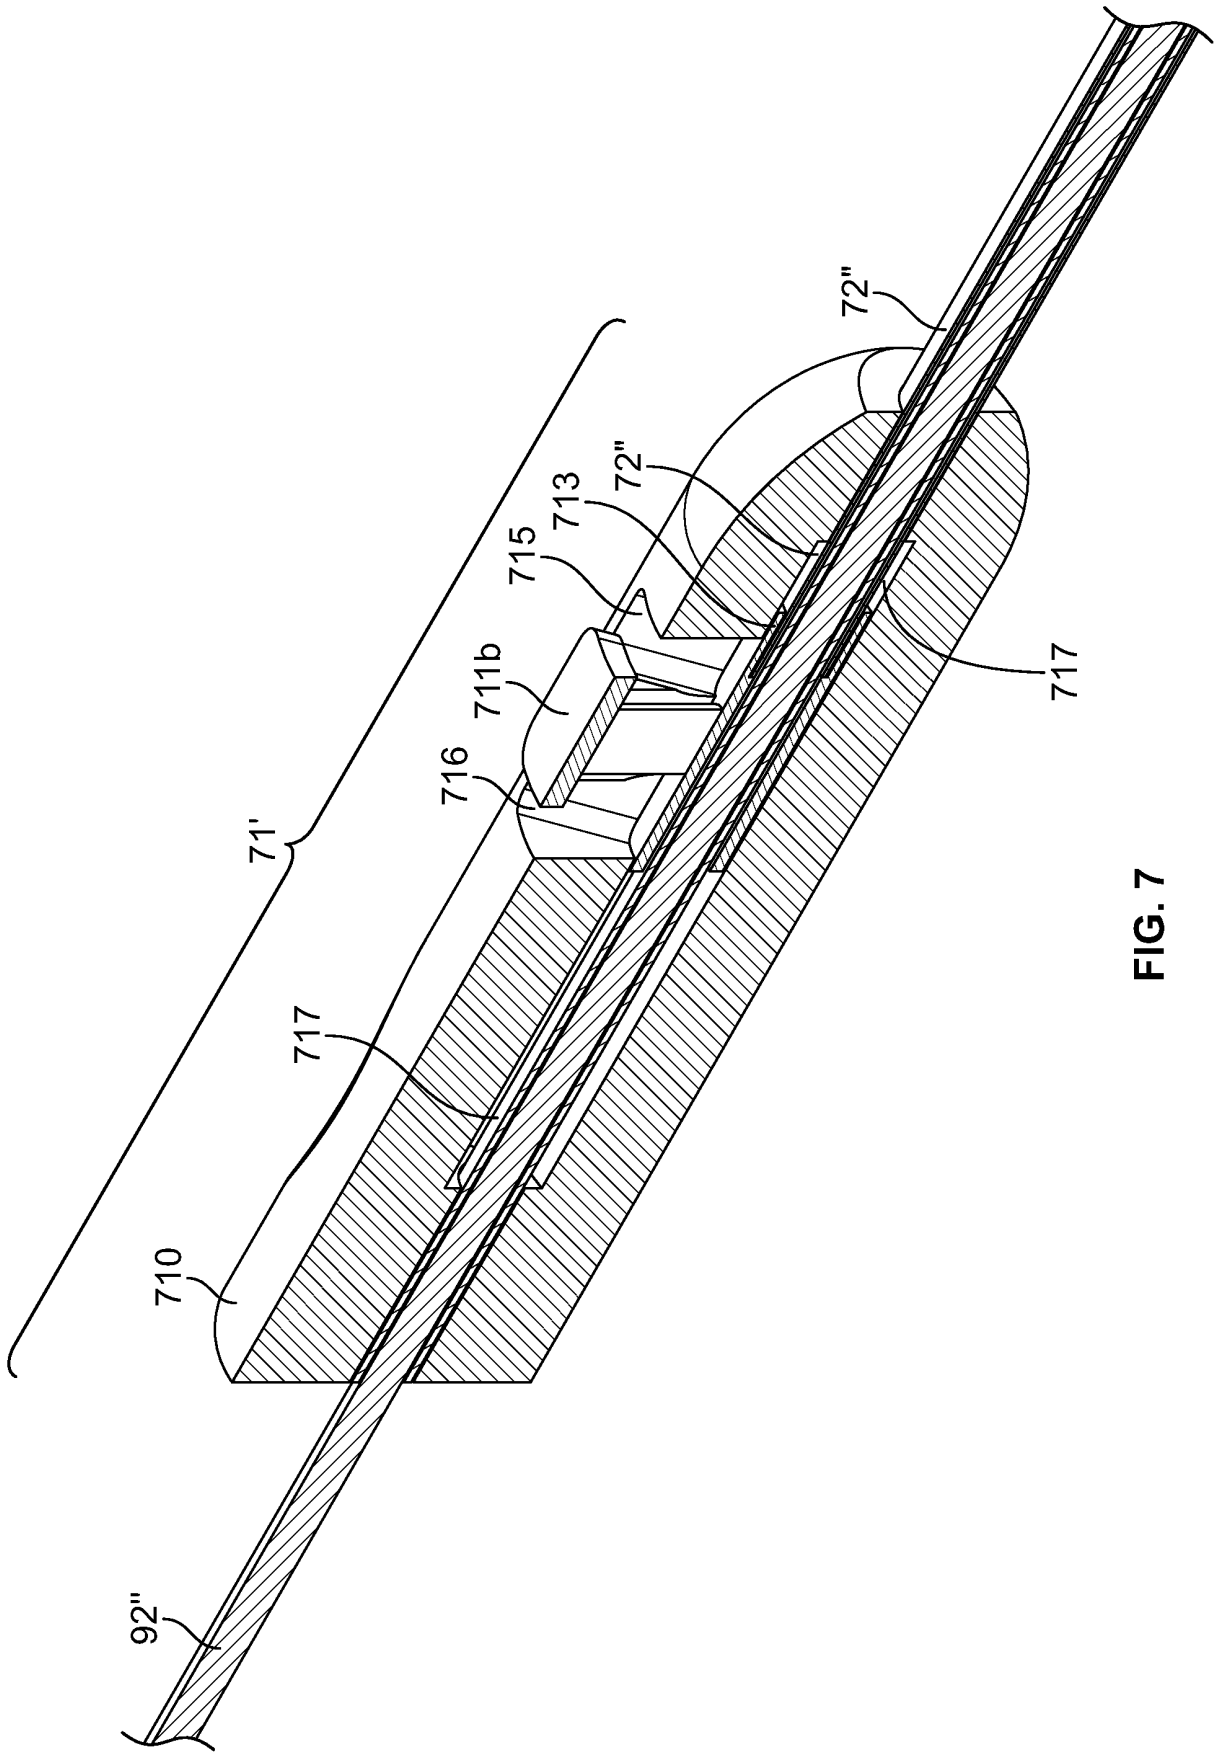
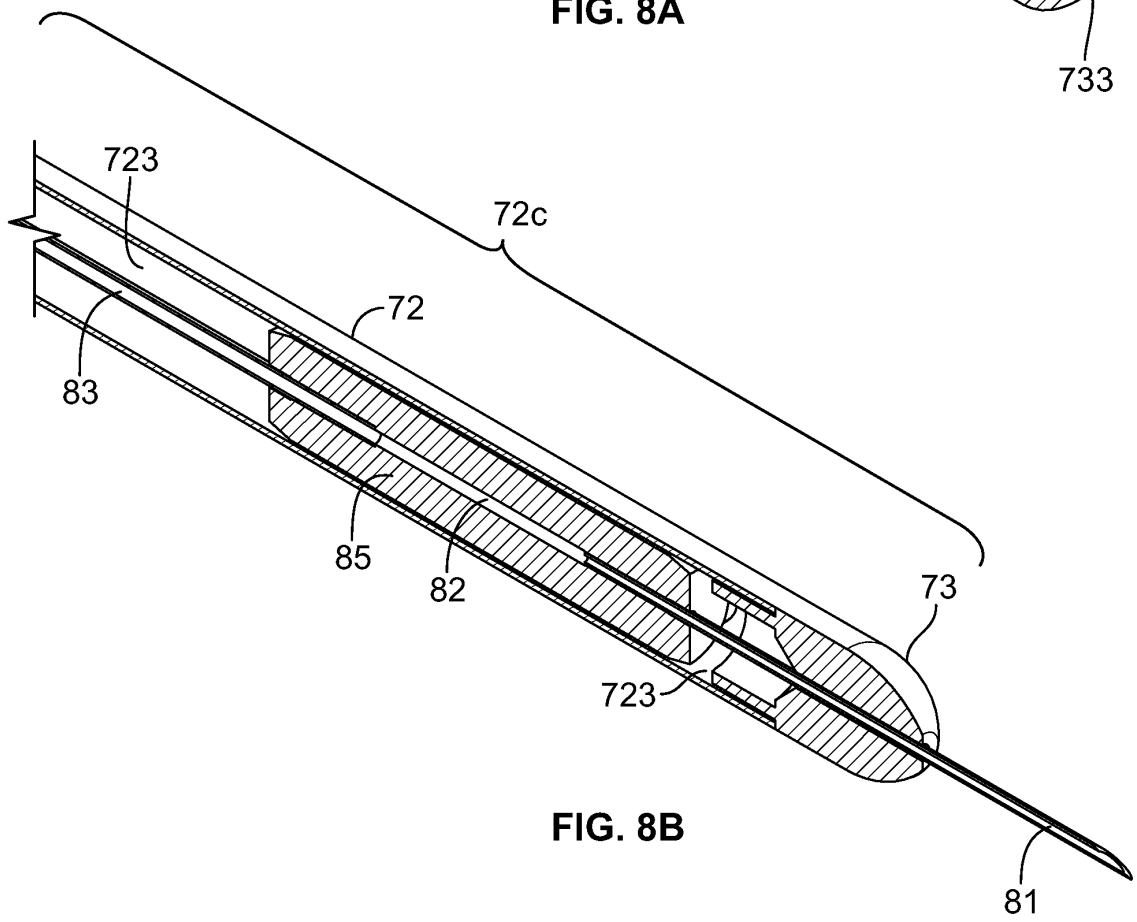
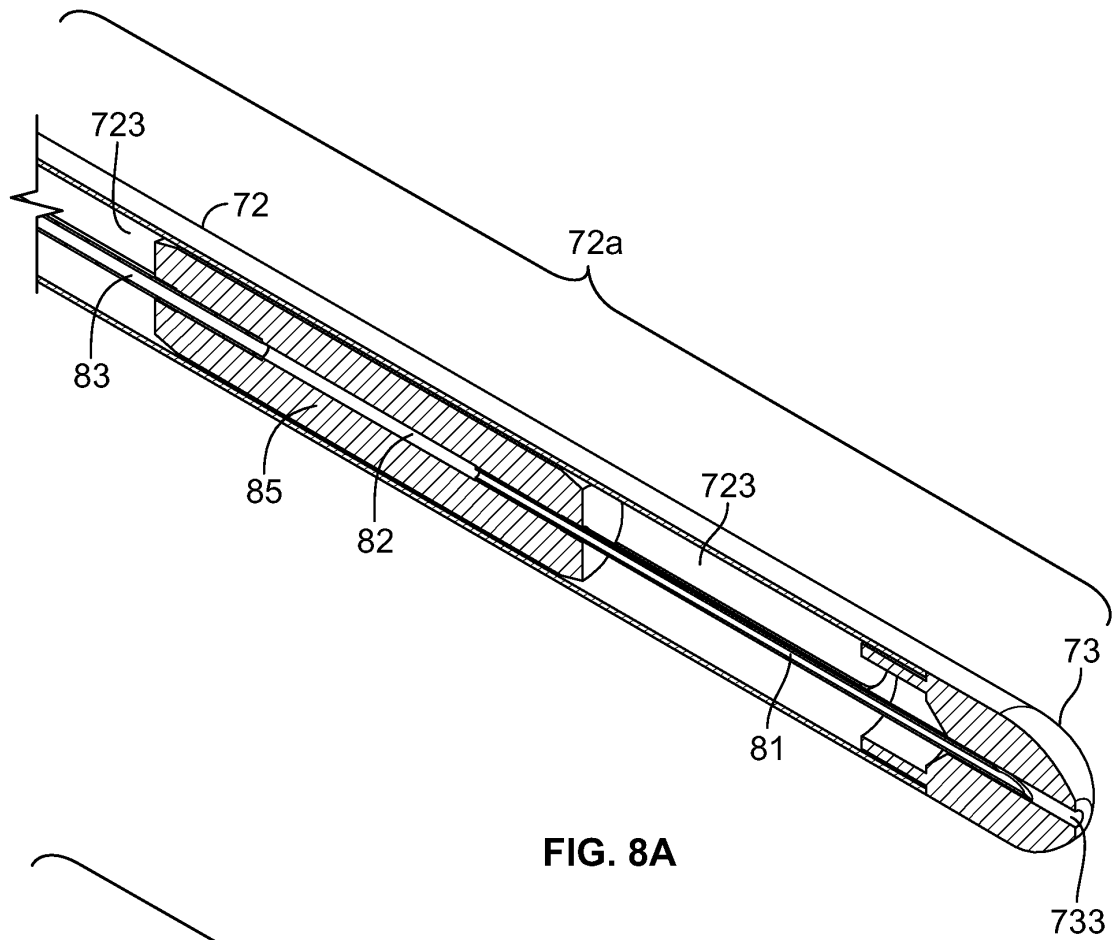


FIG. 7



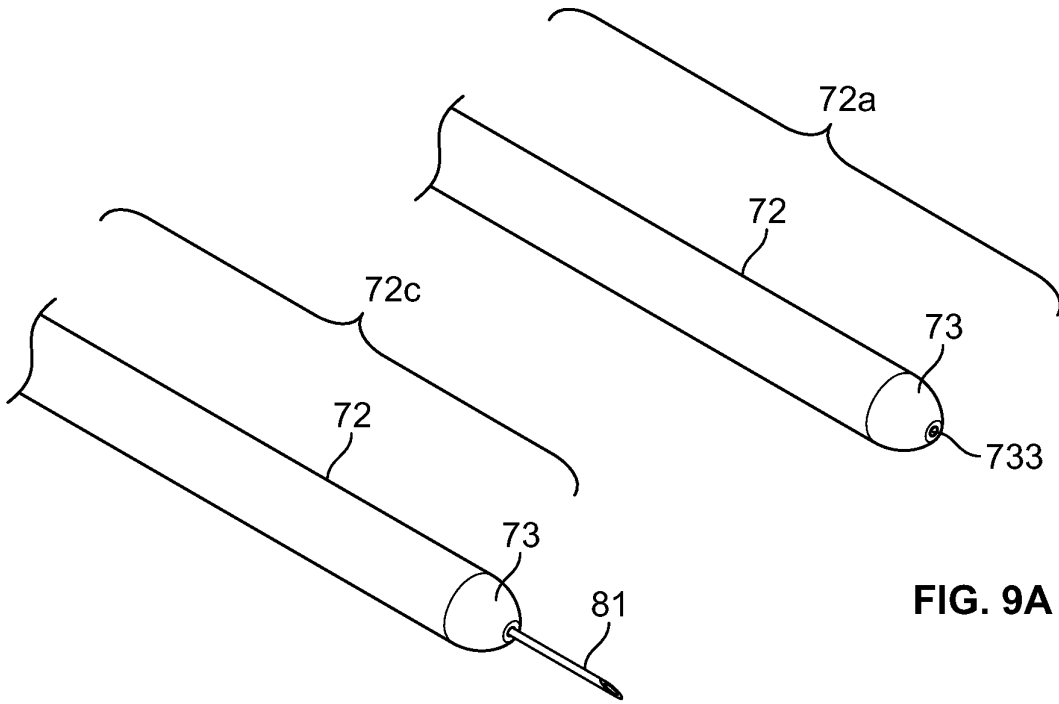


FIG. 9A

FIG. 9B

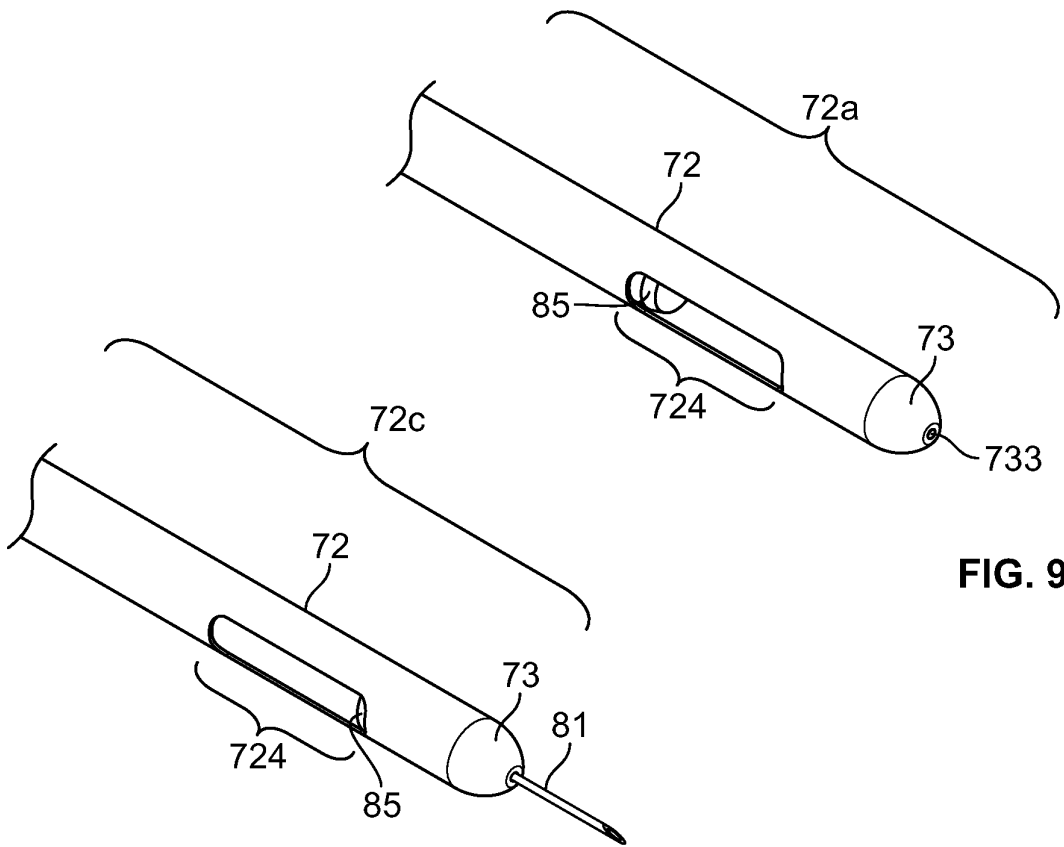


FIG. 9C

FIG. 9D

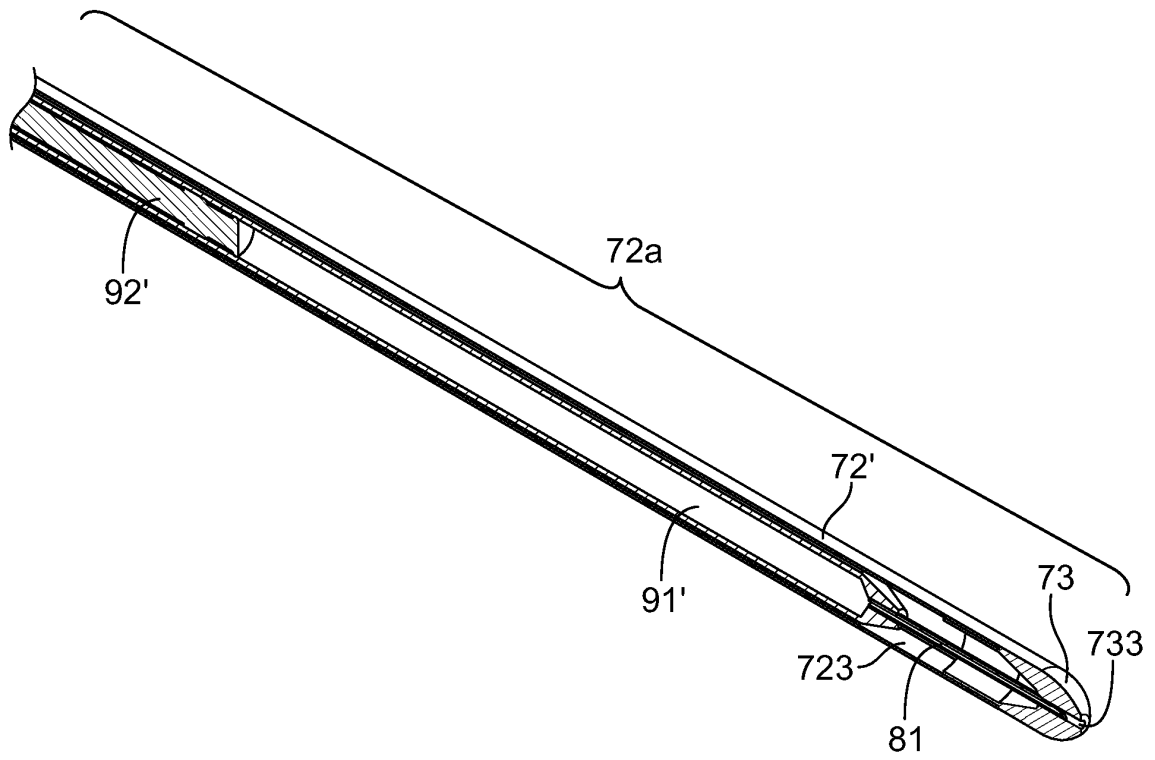


FIG. 10A

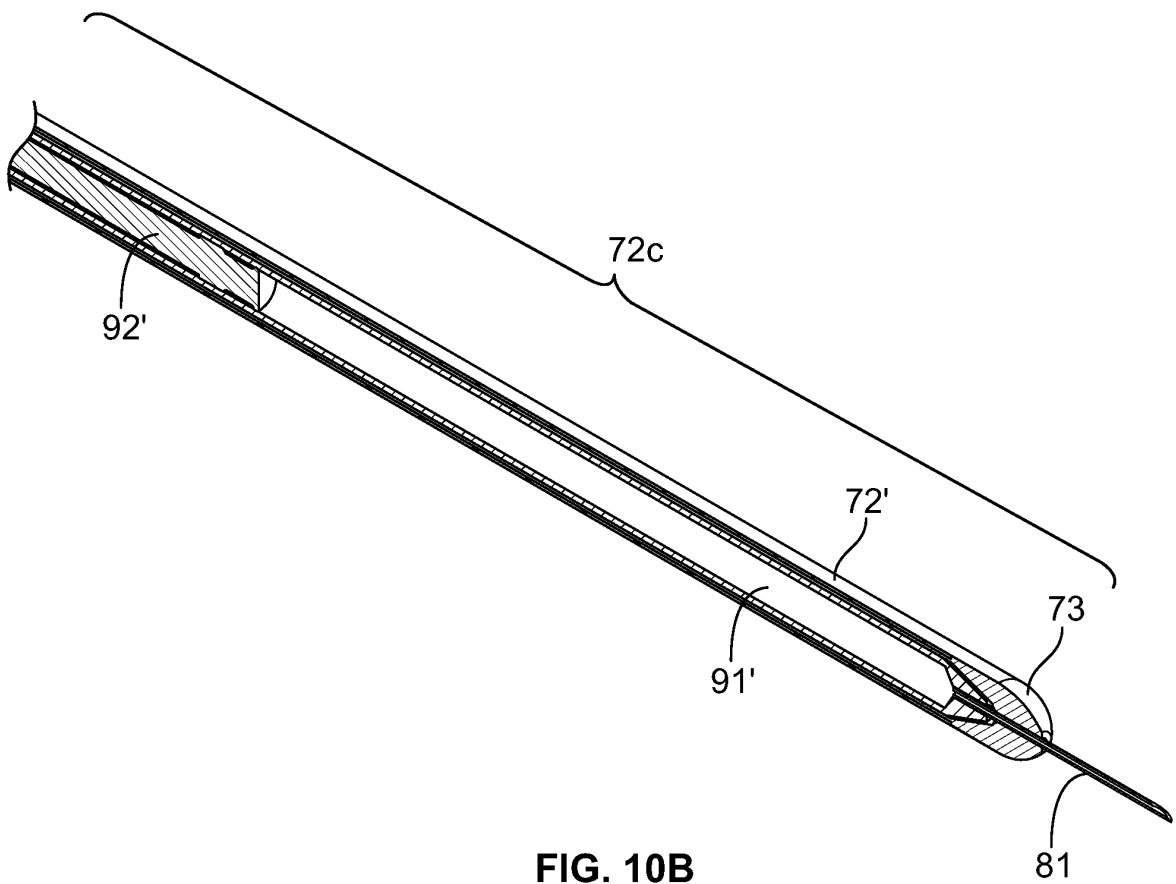


FIG. 10B

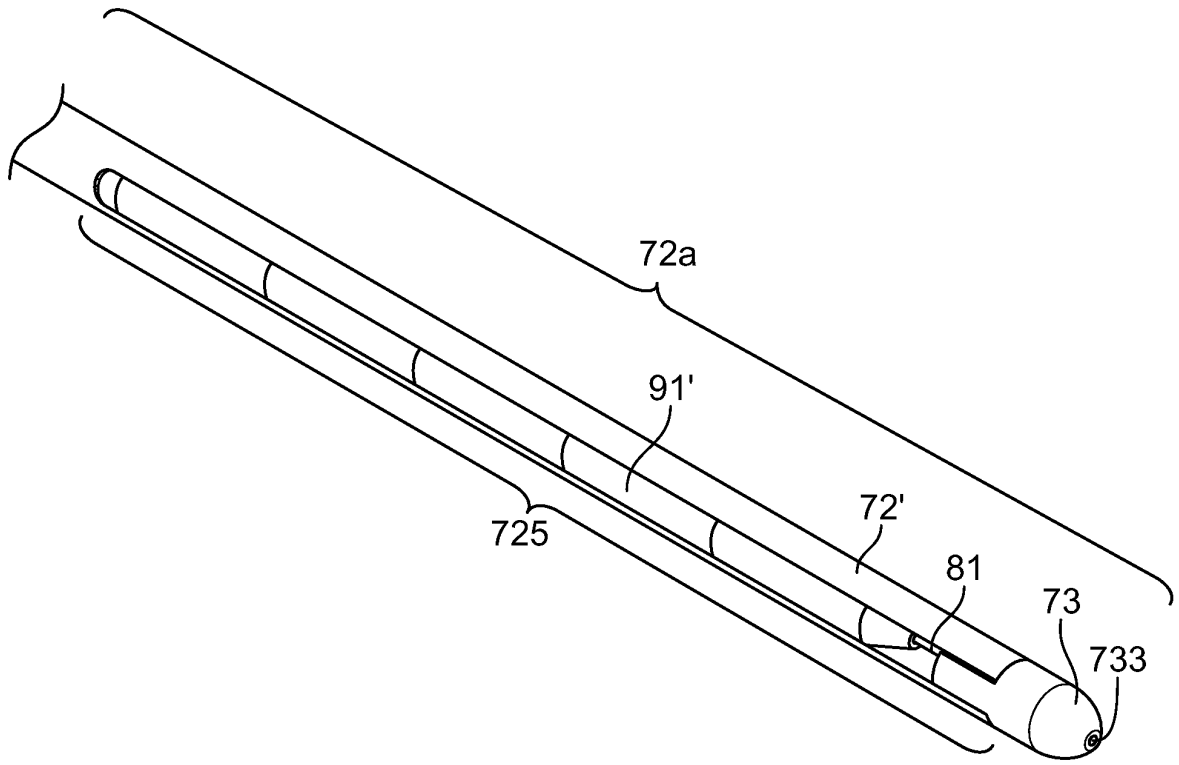


FIG. 10C

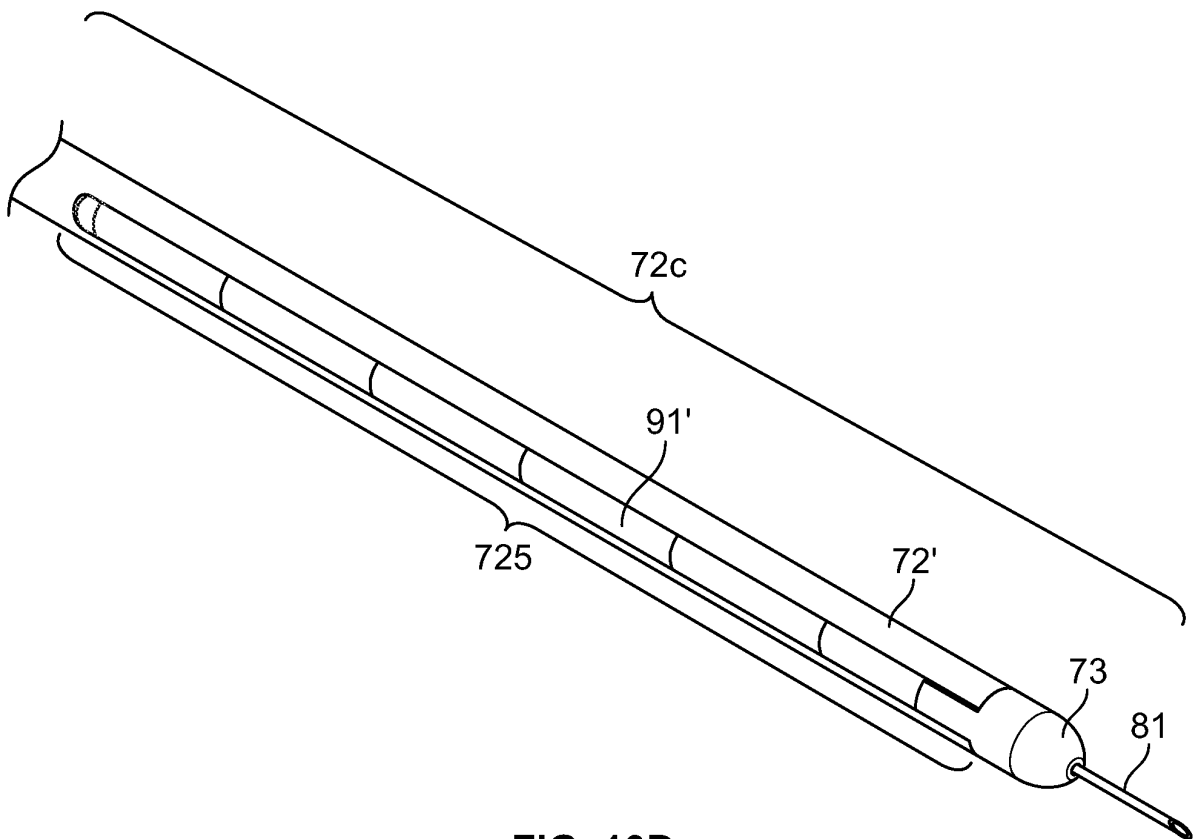


FIG. 10D

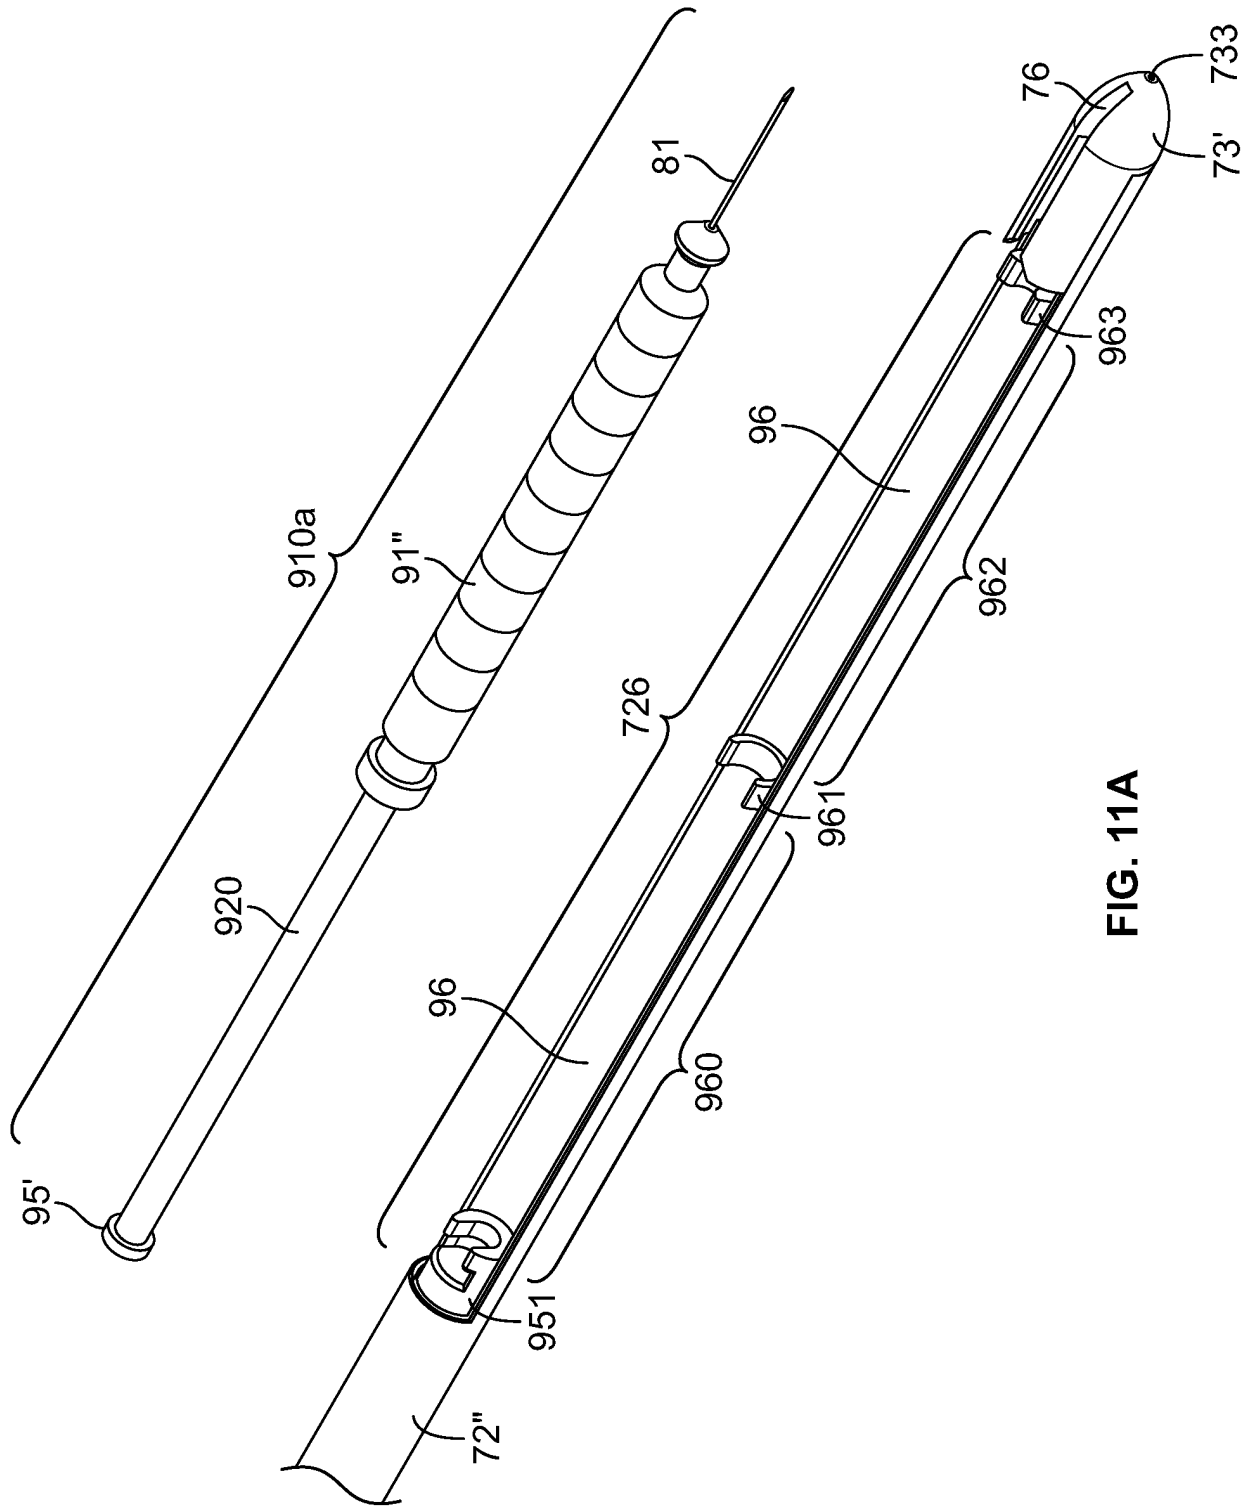


FIG. 11A

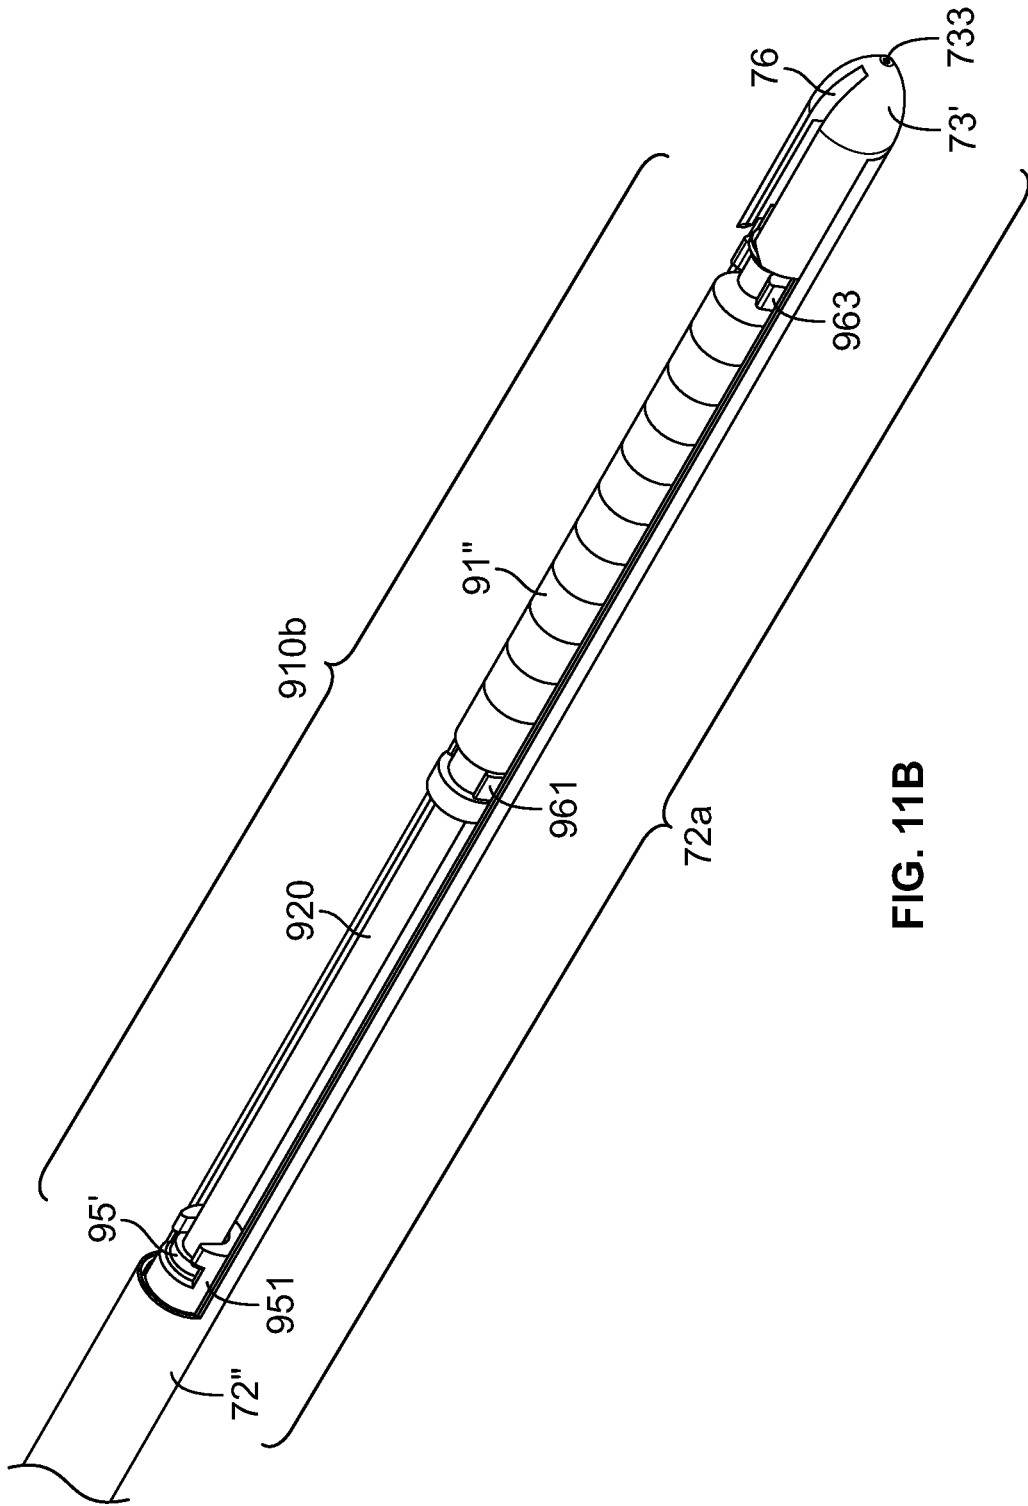


FIG. 11B

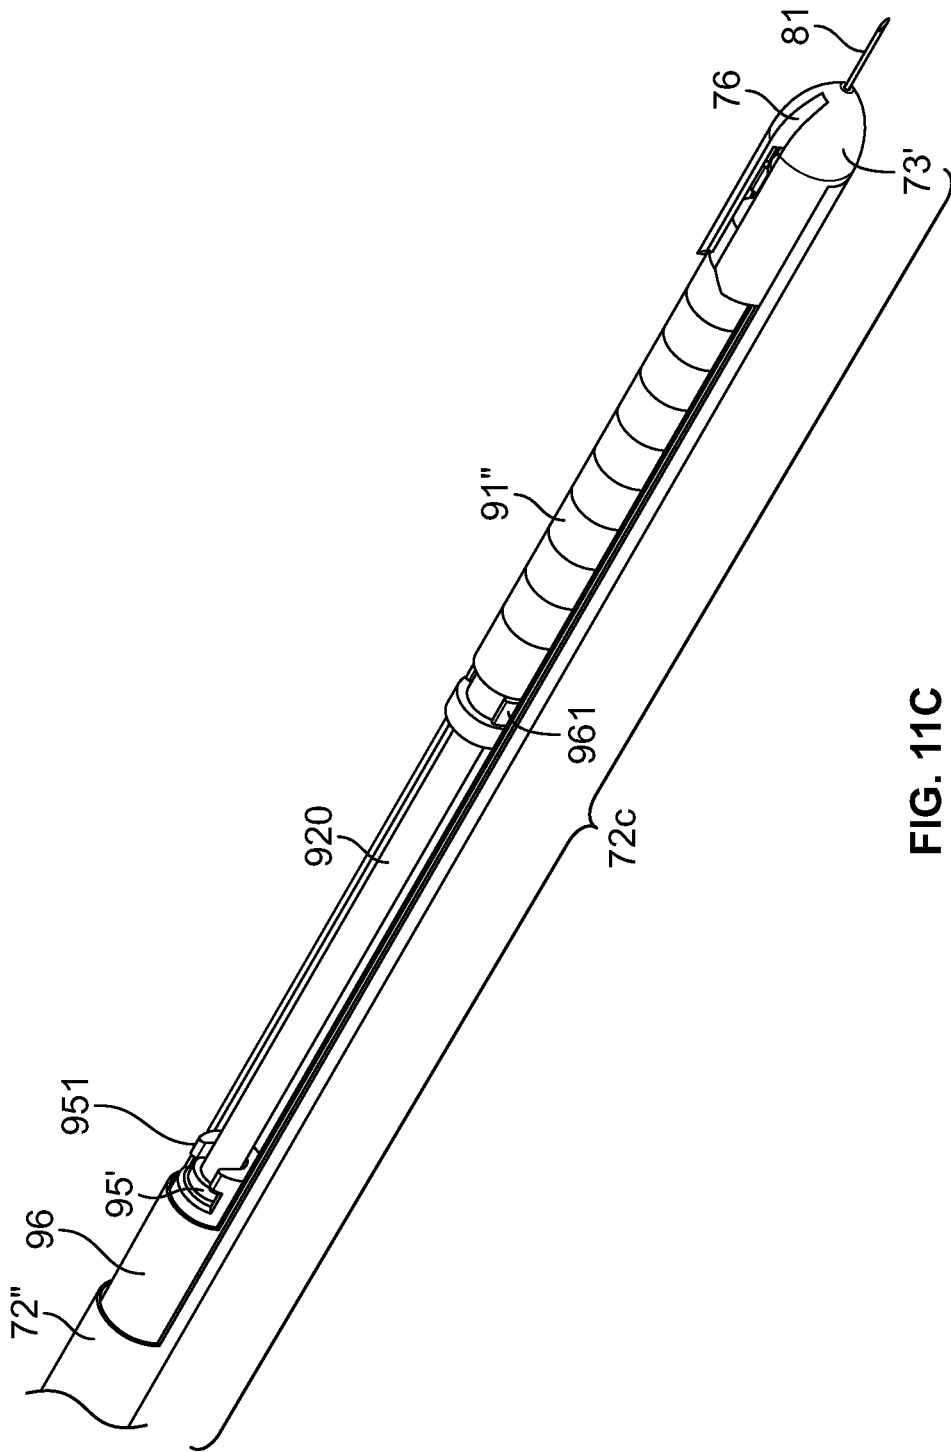


FIG. 11C

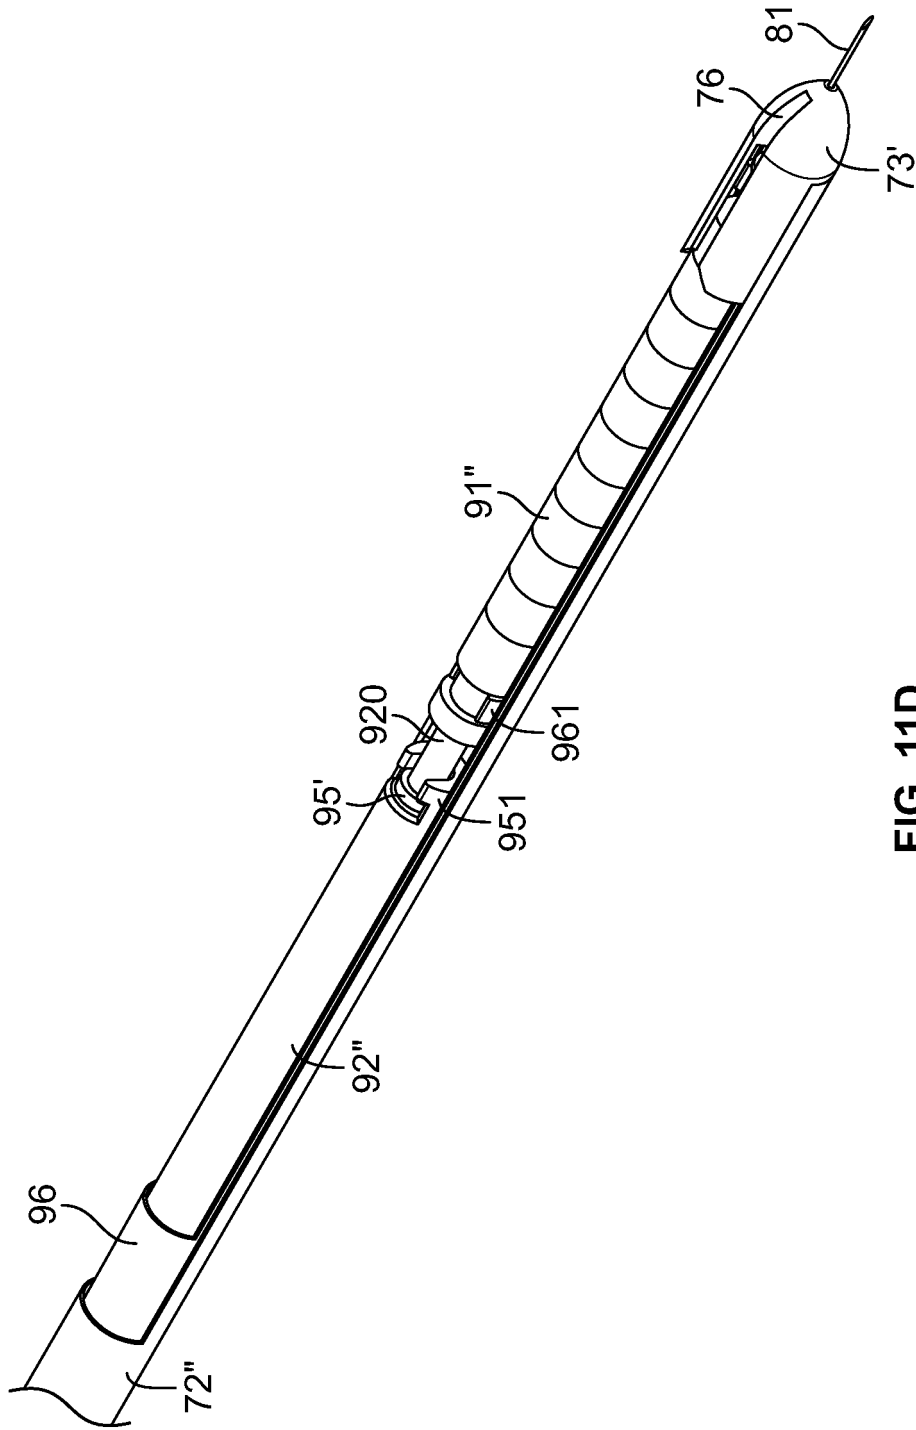


FIG. 11D

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 20100312173 A [0003]
- US 4763667 A [0003]
- US 6723082 B [0004]
- US 20110160533 A [0005]
- US 2010048990 A [0006]
- US 6057155 A [0094]
- US 5543328 A [0094]
- US 5756086 A [0094]

专利名称(译)	注射装置用于微创手术		
公开(公告)号	EP3030171B1	公开(公告)日	2017-11-01
申请号	EP2014756174	申请日	2014-08-08
[标]申请(专利权)人(译)	全球生物疗法有限公司		
申请(专利权)人(译)	全球生物治疗学, INC.		
当前申请(专利权)人(译)	全球生物治疗学, INC.		
[标]发明人	CABRERA AQUINO JOSE GUSTAVO SEGURA PACHECO BLANCA ANGELICA GERKEN STEVEN MASTERSON STEVEN		
发明人	CABRERA AQUINO, JOSE GUSTAVO SEGURA PACHECO, BLANCA ANGELICA GERKEN, STEVEN MASTERSON, STEVEN		
IPC分类号	A61B17/34 A61M5/178		
CPC分类号	A61B17/3478 A61B2017/00247 A61B2090/034 A61B2090/08021 A61D7/00 A61M5/31511 A61M5/3202 A61M5/46 A61M2005/31598 A61M2202/206 A61M2210/02 A61M2210/04 A61M2210/0693 A61M2210/1003 A61M2210/1039 A61M2210/1071 A61M2210/1089 A61M2210/125 A61M2210/1433 A61M2210/166 A61P11/00 A61P17/14 A61P19/02 A61P21/00 A61P21/02 A61P25/00 A61P25/04 A61P29/00		
代理机构(译)	博尔特WADE TENNANT		
优先权	61/863888 2013-08-08 US		
其他公开文献	EP3030171A2		
外部链接	Espacenet		

摘要(译)

本文提供了一种注射装置, 其可用于微创手术, 例如腹腔镜手术, 用于将流体(例如治疗剂)直接施用于靶组织或器官。

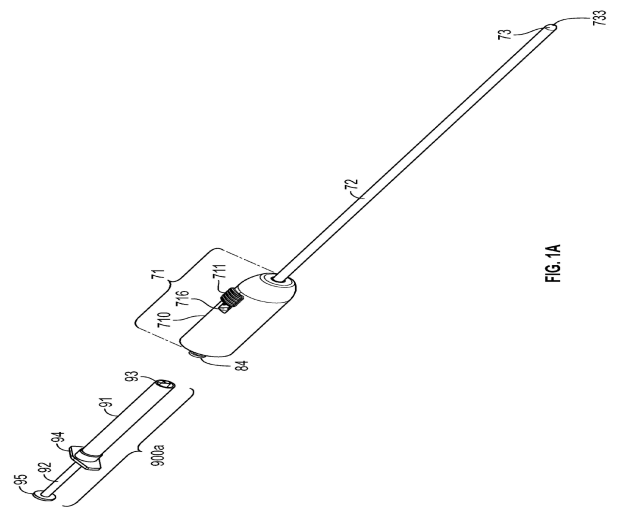


FIG. 1A