



(51) International Patent Classification:
A61B 1/00 (2006.01)

(21) International Application Number:

PCT/US20 13/040992

(22) International Filing Date:

14 May 2013 (14.05.2013)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

61/61 1,182	15 March 2012 (15.03.2012)	US
61/623,376	12 April 2012 (12.04.2012)	u s
PCT/US20 12/34698	23 April 2012 (23.04.2012)	u s
61/646,887	14 May 2012 (14.05.2012)	u s
13/474,429	17 May 2012 (17.05.2012)	u s
61/664,143	25 June 2012 (25.06.2012)	u s
61/667,341	2 July 2012 (02.07.2012)	u s
61/681,129	8 July 2012 (08.07.2012)	u s
61/672,733	17 July 2012 (17.07.2012)	u s
61/676,444	27 July 2012 (27.07.2012)	u s
61/692,701	23 August 2012 (23.08.2012)	u s
61/709,022	2 October 2012 (02. 10.2012)	u s
61/709,033	2 October 2012 (02. 10.2012)	u s
61/803,672	20 March 2013 (20.03.2013)	u s
61/803,664	20 March 2013 (20.03.2013)	u s
61/813,635	18 April 2013 (18.04.2013)	u s
61/818,341	1 May 2013 (01.05.2013)	u s

Merced Drive, San Bruno, CA 94066 (US). **WANG, Shih-Ping** [US/US]; 38 Third Street #307, Los Altos, CA 94022 (US).

(74) Agent: **KAVRUKOV, Ivan, S**; Cooper & Dunham LLP, 30 Rockefeller Plaza, 20th Floor, New York, NY 101 12 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

(71) Applicant (for all designated States except US): **EN-DOSEE CORPORATION** [US/US]; 4984 El Camino Real, Suite 115, Los Altos, CA 94022 (US).


(72) Inventors; and

(71) Applicants (for US only): **OUYANG, Xiaolong** [US/US]; 969 Lawrence Lane, Palo Alto, CA 94303 (US). **END-MAN, Paul, D.** [US/US]; 1415 Mercer Avenue, San Jose, CA 95032 (US). **DECKMAN, Robert, K.** [US/US]; 126

Published:

- with international search report (Art. 21(3))
- with information concerning one or more priority claims considered void (Rule 26bis.2(d))
- the filing date of the international application is within two months from the date of expiration of the priority period (Rule 26bis.3)

(54) Title: METHOD AND APPARATUS FOR HYSTEROSCOPY AND COMBINED HYSTEROSCOPY AND ENDOMETRIAL BIOPSY

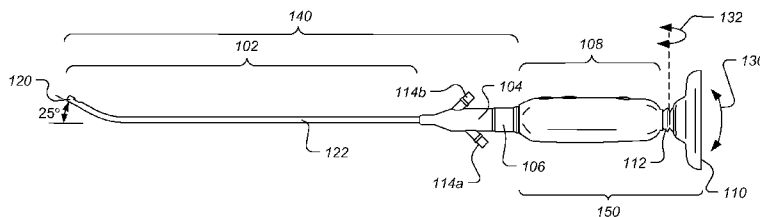

(57) Abstract: Instruments and methods are described for performing hysteroscopy and/or combined hysteroscopy and endometrial biopsy. According to some embodiments, the handle, electronics and integrated display screen form a re-usable portion of the instrument while the fluid hub and cannula which includes a CMOS imaging module and LED lighting, form a single use portion of the instrument. The cannula is semi-flexible such that the operator can easily grasp the cannula at some intermediate point along the shaft (e.g. 5 inches from the distal tip) to bend and/or steer the cannula during use. According to some embodiments, the distal tip has a larger diameter than the shaft which has been found to improve fluid management during use in some applications.



METHODS AND APPARATUSES FOR
HYSTEROSCOPY AND COMBINED HYSTEROSCOPY AND ENDOMETRIAL
BIOPSY

5

REFERENCE TO RELATED APPLICATIONS

[0001] This patent application claims the priority benefit of and incorporates by reference each of the following applications:

- U.S. Prov. Ser. No. 61/646,887 filed May 14, 2012;
- 10 U.S. Prov. Ser. No. 61/667,341 filed July 2, 2012;
- U.S. Prov. Ser. No. 61/664,143 filed June 25, 2012;
- U.S. Prov. Ser. No. 61/672,733 filed July 17, 2012;
- U.S. Prov. Ser. No. 61/676,444 filed July 27, 2012;
- U.S. Prov. Ser. No. 61/681,129 filed August 8, 2012;
- 15 U.S. Prov. Ser. No. 61/692,701 filed August 23, 2012;
- U.S. Prov. Ser. No. 61/709,022 filed October 2, 2012;
- U.S. Prov. Ser. No. 61/709,033 filed October 2, 2012;
- U.S. Ser. No. 13/474,429 filed May 17, 2012;
- U.S. Prov. Ser. No. 61/803,664 filed March 20, 2013;
- 20 U.S. Prov. Ser. No. 61/803,672 filed March 20, 2013;
- U.S. Prov. Ser. No. 61/813,635 filed April 18, 2013; and
- U.S. Prov. Ser. No. 61/818,341 filed May 1, 2013;

The subject matter of this patent specification relates to the subject matter of the following applications, each of which is incorporated by reference herein:

- 25 U.S. Ser. No. 12/911,297 filed October 25, 2010;
- U.S. Prov. Ser. No. 61/415,771 filed November 19, 2010;
- U.S. Prov. Ser. No. 61/418,248, filed November 30, 2010;
- U.S. Prov. Ser. No. 61/429,093 filed December 31, 2010;
- U.S. Prov. Ser. No. 61/431,316 filed January 10, 2011;
- 30 U.S. Prov. Ser. No. 61/437,687, filed January 30, 2011;
- U.S. Prov. Ser. No. 61/444,098, filed February 17, 2011;
- U.S. Prov. Ser. No. 61/450,115, filed March 7, 2011;
- U.S. Prov. Ser. No. 61/453,533, filed March 16, 2011;
- U.S. Prov. Ser. No. 61/476,754, filed April 18, 2011;
- 35 U.S. Prov. Ser. No. 61/482,200 filed May 3, 2011;

- 2 -

U.S. Prov. Ser. No. 61/482,309 filed May 4, 201 1;
U.S. Prov. Ser. No. 61/485,601 filed May 12, 201 1;
U.S. Prov. Ser. No. 61/490,029 filed May 25, 201 1;
U.S. Prov. Ser. No. 61/494,400 filed June 7, 201 1;
5 U.S. Prov. Ser. No. 61/506,074 filed July 9, 201 1;
U.S. Prov. Ser. No. 61/515,092 filed August 4, 201 1;
U.S. Prov. Ser. No. 61/539,736 filed September 27, 201 1;
U.S. Prov. Ser. No. 61/544,280 filed October 7, 201 1;
U.S. Prov. Ser. No. 61/550,391 filed October 22, 201 1;
10 U.S. Prov. Ser. No. 61/555,470 filed November 3, 201 1;
U.S. Prov. Ser. No. 61/556,167 filed November 4, 201 1;
International Patent Appl. No. PCT/US1 1/51982 filed September 16, 201 1;
U.S. Prov. Ser. No. 61/570,816 filed December 14, 201 1;
U.S. Prov. Ser. No. 61/599,981 filed February 17, 2012;
15 U.S. Prov. Ser. No. 61/600,593 filed February 18, 2012;
U.S. Prov. Ser. No. 61/61 1,182 filed March 15, 2012;
U.S. Prov. Ser. No. 61/623,376 filed April 12, 2012; and
International Patent Appl. No. PCT/US201 2/34698 filed April 23, 2012.

The above-referenced provisional and non-provisional patent applications are
20 collectively referenced herein as "the commonly assigned incorporated
applications."

FIELD

25 **[0002]** The present invention generally relates mainly to a medical device for
use in hysteroscopic examinations of the uterus. More particularly, some
embodiments relate to a medical device having integrated visualization and
endometrial sampling components.

BACKGROUND

30 **[0003]** Hysteroscopy, or direct vision of the inside of the uterus (referred to
herein as the "uterine cavity" and/or "endometrial cavity"), has been shown to
greatly improve diagnostic accuracy. Few gynecologists do office hysteroscopy,
however, because of the complexity and expense of the equipment and supplies

- 3 -

required. Conventional endoscopes are typically tethered and cumbersome to use. They require skilled staff to operate and maintain. This makes it especially difficult in time critical locations such as an emergency room, operating room, and other areas of a medical facility where multiple devices and instruments are being used
5 simultaneously.

[0004] Office-based endometrial biopsy is a standard diagnostic procedure used by gynecologists. While efficacious in detection of cancer, endometrial biopsy frequently will not detect endometrial polyps, submucous myomas, and other endometrial pathology. While it is possible to take tiny biopsies through
10 some hysteroscopes that have operating channels, the surgeon usually needs to remove the hysteroscope and then do an endometrial biopsy with a different instrument. The repeated insertion and removal of multiple instruments into the patient's uterine cavity can be uncomfortable for the patient and/or may prolong the time required to complete the hysteroscopy and endometrial sampling procedures
15 compared to performing both procedures without the repeated insertion and removal of different instruments. And, such use of multiple instruments for the same inspection/biopsy procedure requires the expense and inconvenience of buying, stocking and sterilizing such instruments.

[0005] The subject matter claimed herein is not limited to embodiments that
20 solve any specific disadvantages or that operate only in environments such as those described above. Rather, this background is only provided to illustrate one exemplary technology area where some embodiments described herein may be practiced.

25

SUMMARY

[0006] According to some embodiments, a low-cost medical instrument is described for examining a patient's uterus. The instrument includes a single-use portion configured to in a single insertion distend and image a patient's uterus. The single-use portion includes: an elongated conduit having a distal portion
30 configured and dimensioned for insertion into the patient's uterus, and a proximal portion; a fluid connection port formed at the proximal portion of the conduit; one or more distal openings at the distal portion of the conduit configured to provide fluid from the conduit and into the uterus; an imaging system at the distal portion of the

- 4 -

conduit configured to image the uterus and provide video signals; an illumination system at the distal portion of the conduit configured to illuminate the uterus at an illumination field viewed by the imaging system; and an electrical cable extending from a proximal end of the conduit to the imaging system and configured to carry
5 video signals, control signals and electrical power. The instrument also includes a multiple-use portion having interior and exterior surfaces, the multiple-use portion being configured to be attached to the single-use portion for a single use and then detached after a single use, and to be re-used with a second single-use portion without sterilization of the interior surfaces. The multiple-use portion includes an
10 integral image display that is electrically coupled with the imaging system at least in part by the electrical cable, the display being configured to display images provided by the imaging system for viewing by a user. The instrument also includes one or more seals configured to keep fluid in the conduit from contacting any of the interior surfaces of the multiple-use portion.

15 **[0007]** According to some embodiments, an integrated endoscopic instrument is described for examining a patient's uterus. The instrument includes an elongate member having a proximal end and a distal end. The elongate member is dimensioned and configured to facilitate insertion of the distal end through a patient's cervix and into the uterus. The elongate member is semi-flexible such
20 that when fixedly held at 5 inches from the distal end and a 50 gram mass is applied two inches from the distal end the distal end bends in a downwards direction between 10mm and 80mm. The instrument further includes: an imaging system at the distal portion of the conduit configured to image the uterus and provide video signals; an illumination system at the distal portion of the conduit
25 configured to illuminate the uterus at an illumination field viewed by the imaging system; a fluid opening positioned at the distal end of the elongate member to improve visual inspection using the electronic imaging module by delivering fluid to flow in a distal direction thereby clearing debris close to the imaging module; a handle that is configured and dimensioned to be grasped by a user's hand and
30 manipulated by a user; and an integral image display that is electrically coupled with the imaging system at least in part an electrical cable. The display is configured to display images provided by the imaging system for viewing by the user.

- 5 -

[0008] According to some embodiments, an integrated endoscopic instrument is described for examining a patient's uterus. The instrument includes: an elongate member having a proximal end, a distal end, and a shaft extending from the distal end to the proximal end. The shaft houses a fluid channel and a plurality of
5 electrical conductors. The conductors are configured to carry video and control signals. The shaft has a first outer diameter of less than 5mm and the distal end has a second outer diameter greater than the first outer diameter. The instrument further includes: an imaging system at the distal portion of the conduit configured to
10 image the uterus and provide video signals; an illumination system at the distal portion of the conduit configured to illuminate the uterus at an illumination field viewed by the imaging system; and a distal facing fluid opening at the distal end of the elongate member and in fluid communication with the fluid channel. The opening is positioned to improve visual inspection using the electronic imaging module by delivering fluid to flow in a distal direction thereby clearing debris close
15 to the imaging module. The instrument further includes: a handle that is configured and dimensioned to be grasped by a user's hand and manipulated by a user; and an integral image display that is electrically coupled with the imaging system at least in part by at least some of the plurality of electrical conductors. The display is configured to display images provided by the imaging system for viewing by the
20 user.

BRIEF DESCRIPTION OF THE DRAWINGS

[0009] To further clarify the above and other advantages and features of the subject matter of this patent specification, specific examples of embodiments
25 thereof are illustrated in the appended drawings. It should be appreciated that these drawings depict only illustrative embodiments and are therefore not to be considered limiting of the scope of this patent specification or the appended claims. The subject matter hereof will be described and explained with additional specificity and detail through the use of the accompanying drawings in which:

30 **[001 0]** Fig. 1 is a left side view of a device for hysteroscopy and/or combined hysteroscopy and endometrial biopsy, according to some embodiments;

[001 1] Fig. 2 is a distal end view of a device for hysteroscopy and/or combined hysteroscopy and endometrial biopsy, according to some embodiments;

- 6 -

- [0012]** Fig. 3 is a proximal end view of a device for hysteroscopy and/or combined hysteroscopy and endometrial biopsy, according to some embodiments;
- [0013]** Fig. 4 is a perspective view of a device for hysteroscopy and/or combined hysteroscopy and endometrial biopsy, according to some embodiments;
- 5 **[0014]** Fig. 5 is a cross section showing details of a sealed sliding connector for a device for hysteroscopy and/or combined hysteroscopy and endometrial biopsy, according to some embodiments;
- [0015]** Figs. 6A-6F illustrate various aspects of a cannula for a device configured for combined hysteroscopy and endometrial biopsy, according to some
10 embodiments;
- [0016]** Figs. 7A-C show further detail of a distal tip of a device configured for combined hysteroscopy and endometrial biopsy, according to some embodiments;
- [0017]** Fig. 8 is a flow chart illustrating aspects of using a multi-lumen cannula with simultaneous in-flow and out-flow for a hysteroscopy procedure, according to
15 some embodiments;
- [0018]** Figs. 9A-9G illustrate a single-use portion that includes a cannula configured for fluid-in flow and visualization, according to some embodiments;
- [0019]** Fig. 10 is a cross section showing details of a sealed sliding connector for a device for hysteroscopy, according to some embodiments;
- 20 **[0020]** FIG. 11 is a flow chart showing aspects of using a variable dimension cannula for visual inspection of a patient's uterus, according to some embodiments;
- [0021]** Figs. 12A-12C illustrate a test setup to measure flexibility of a cannula shafts used in a device for hysteroscopy and/or combined hysteroscopy and endometrial biopsy, according to some embodiments;
- 25 **[0022]** Fig. 13 is a cross section showing an example of a different internal shaft structures within a cannula for a device for hysteroscopy and/or combined hysteroscopy and endometrial biopsy, according to some embodiments;
- [0023]** Figs. 14A-14B illustrate aspects of a cannula for a device configured for combined hysteroscopy and endometrial biopsy, according to some alternative
30 embodiments; and
- [0024]** Figs. 15A-15C illustrate a device for hysteroscopy and/or combined hysteroscopy and endometrial biopsy having a single use cannula, fluid hub and handle, and a re-usable display screen, according to some embodiments.

DETAILED DESCRIPTION

[0025] A detailed description of examples of preferred embodiments is provided below. While several embodiments are described, it should be understood that the new subject matter described in this patent specification is not limited to any one embodiment or combination of embodiments described herein, but instead encompasses numerous alternatives, modifications, and equivalents. In addition, while numerous specific details are set forth in the following description in order to provide a thorough understanding work, some embodiments can be practiced without some or all of these details. Moreover, for the purpose of clarity, certain technical material that is known in the related art has not been described in detail in order to avoid unnecessarily obscuring the new subject matter described herein. It should be clear that individual features of one or several of the specific embodiments described herein can be used in combination with features or other described embodiments. Further, like reference numbers and designations in the various drawings indicate like elements.

[0026] Fig. 1 is a left side view of a device for hysteroscopy and/or combined hysteroscopy and endometrial biopsy, according to some embodiments. Many of the elements of the embodiments of hysteroscope 100 shown in Fig. 1 are the same as or similar to those discussed in the embodiments described in the commonly assigned incorporated applications, and such elements may not be described or may only briefly be described. It will also be appreciated that the aspects of the embodiments described in the commonly assigned incorporated applications may also apply to the embodiments described herein.

[0027] The device 100 is particularly advantageous for enabling a physician to perform an efficient combined hysteroscopic examination and an endometrial biopsy, although it is to be appreciated that other uses for hysteroscope 100 are within the scope of the present teachings. For example, as will be described in further detail, *infra*, the hysteroscope 100 can be fitted with other types of cannulas that are configured for other types of procedures such as hysteroscopy without biopsy. The hysteroscope 100 can bring about substantial efficiencies in terms of keeping equipment costs low and keeping the time required to perform the

- 8 -

procedure modest, while at the same time providing the opportunity for better endometrial sample quality over conventional "blind" endometrial sample collection methods. Hysteroscope 100 includes a sampling cannula 102, fluid hub 104, sliding connector 106, handle body 108, display mount 112 and display 110. The biopsy sampling cannula 102 is made of a distal tip 120 and a shaft 122. The fluid hub in this case includes two fluid ports 114a and 114b. In the example shown in Fig. 1, fluid port 114a is configured to deliver fluid into the device and thus into the uterus, and fluid port 114b is configured to apply suction to extract fluid and tissue samples from the uterus. As shown, the shaft 122 is curved near its distal end, for example having a 25 degree bend as shown. According to some embodiments, a bend of between 15 and 35 degrees near the distal end has been found to be suitable for many applications. The distal tip 120 includes a video camera assembly, lighting elements and fluid ports for in-flow (i.e. out of the device 100 and into the patient) and out-flow (i.e. into the device 100 and out of the patient). A sampling port on the upper side of the distal tip 120 also includes a cutting portion, which aids in tissue sample collection, as described in more detail below. According to some embodiments, the outer shell of tip 120 and shaft 122 are constructed of the same material, for example a heat and UV stabilized nylon 12 grade for tube extrusion such as Grilamid® L25. According to some embodiments the display 110 is a touch-screen display, and is able to tilt upwards and downwards by, for example, about 60 degrees each (total range of motion of 120 degrees), and pivot, or "pan" left and right by, for example, 45 degrees each (total range of motion 90 degrees) as shown by arrows 130 and 132 respectively. According to some embodiments, the cannula 102 (including the camera assembly, LED lighting and fluid ports integrated into the distal tip 120), fluid hub 104 and sliding connector 106 together form a single-use portion 140, which is designed for a single-use. According to these embodiments the single-use portion 140 is delivered to the medical practitioner in pre-sterilized package and are intended to be disposed of after a single-use, and the handle 108 and display 110 form a reusable portion 150, which is designed to be re-used many times.

[0028] According to some embodiments, the device 100 shown for example in Figs. 1 is a hand-held, compact single use endoscope. In these cases, endoscope 100 is provided in a sterile package, so is ready for immediate use without

- 9 -

requiring any preparation for diagnostic or therapeutic procedures. According to some embodiments the single use device 100 needs no sophisticated connectors such that the entire endoscope is supplied in a sterile package ready for use.

[0029] Fig. 2 is a distal end view of a device for hysteroscopy and/or combined hysteroscopy and endometrial biopsy, according to some embodiments. The tip 120 and shaft 122 can be seen, as well as the fluid hub 104, fluid ports 114a and 114b, as well as handle body 108. Also shown, according to some embodiments is photo/video processing circuitry 210 that can be used to enhance or otherwise manipulate standard video signals and/or images received from the camera module in tip 120. According to some embodiments, in Fig. 2 as in other figures herein, various dimensions are shown that have been found to be suitable for many applications, but those skilled in the art may vary those dimensions without departing from the teachings of this patent specification.

[0030] Fig. 3 is a proximal end view of a device for hysteroscopy and/or combined hysteroscopy and endometrial biopsy, according to some embodiments. Touch-sensitive screen 110 is preferably 3.5 inches (diagonally) in size.

[0031] Fig. 4 is a perspective view of a device for hysteroscopy and/or combined hysteroscopy and endometrial biopsy, according to some embodiments. In Fig. 4 the single-use portion 140 is shown disconnected from the re-usable portion 150. The sliding connector 106 is shown and has an outer shell 470 that includes a lip 472 that fits over an o-ring seal 462 and a protruding mating portion 450 of the handle assembly 108. Multiple similar seals can be provided along the length of connector 106 to further isolate handle 108 from patient matter and/or fluids that could otherwise contaminate and/or cause connection failure such as electrical failures on handle 108. Also within connector 106 is a seal which forms a barrier between the proximal end of electrical cable 480 and fluid and/or patient matter. The cable 480 carries video signals and control signals between the camera module and LEDs at distal tip 120 to connection pins housed within sleeve 460. The sleeve 460 fits into a closed channel on the handle 108 while the connection pins mate with pin receptacles 452 as to form electrical connections with the pins.

[0032] Also visible in Fig. 4 is ON/OFF button 410 is used to toggle the device 100 on or off. According to some embodiments, the power ON/OFF button 410 is

- 10 -

backlit using two differently colored LEDs to indicate the status of rechargeable battery 420 to the user. For example, green backlighting can be used to indicate the battery level is OK and red backlighting can be used to indicate the battery 420 is low. According to some embodiments the capacity of battery 420 is about
5 2500mAh. According to some embodiments, the LED lighting of button 412 can also be used to indicate battery charging status during re-charging of the battery 420 from an external power source. In this case, the backlighting LED shows red while charging the battery and green when the battery 420 is fully charged. According to some embodiments, the ON/OFF button 410 doubles as a "home"
10 button, such that a shorter press, such as 1 second or less, of button 410 brings up a home screen menu on the display 110.

[0033] LED brightness control button 412 is used to control the brightness of the LEDs on the distal tip 120. According to some embodiments a total of four different LED illumination levels has been found to be suitable and the single
15 button 412 controls the level by cycling through the levels, changing the illumination level with each button press. The Snap/Video button 414 is used to capture still images and/or video from the camera in tip 120. According to some embodiments, pressing Snap/Video button 414 for three seconds or less captures a single still photo, while pressing button 414 for longer than three seconds starts
20 video recording. When video is being recorded, a single press of button 414 stops video capture. According to some embodiments, an audible acknowledgement signal is associated with presses of the buttons 410, 412 and 414. For example, a single "beep" is sounded when any of the buttons except for double beeps when either the Snap/Video button 414 or an OK software button is pressed.

25 **[0034]** It has been found that providing dedicated hardware buttons on the handle itself have several advantages over touch-screen implemented "soft buttons" and/or hardware buttons located in locations other than the the handle. The handle located hardware buttons, such as shown in Fig. 4, allow for one-handed operation as well as for operation with gloved and/or wet hands. With one-
30 handed operation, a user can use a single hand to both manipulation of scope and operate buttons such as the "snap" and/or the "LED" buttons. The user's other hand is then free for other procedures or for manipulating the cannula (e.g. bending of cannula and/or steering the cannula). In other examples, for some

- 11 -

reason the user's other hand may not be sterile. Furthermore, it has been found that the use of touch-screen implemented soft buttons on touch screen display 110 may not reliably work with gloved and/or wet fingers.

[0035] Fig. 5 is a cross section showing details of a sealed sliding connector for a device for hysteroscopy and/or combined hysteroscopy and endometrial biopsy, according to some embodiments. The sliding connector 106 is shown here with an outer shell 470 that includes a lip 472 that fits over an o-ring seal 462 and a protruding mating portion 480 of the handle assembly 108. Other seals can be provided along the length of connector 106 to further isolate handle 108 from patient matter and/or fluids that could otherwise contaminate and/or cause connection failure such as electrical failures on handle 108. The cable 480 carries video signals, control signals and electrical power between the camera module and LEDs at distal tip 120 to connection pins housed within sleeve 460. The sleeve 460 fits into a closed channel on the handle 108 while the connection pins 552 mate with pin receptacles 452 as to form electrical connections the pins. The sliding connector 106 includes a barrier 530 that fits tightly inside outer shell 470. According to some embodiments, a transparent sealing glue 550 is applied between the barrier 530 and shell 470 as shown in Fig. 5. Barrier 530 terminates at its proximal end in an extended sleeve 460 that fits into a closed channel 560 in handle 108 such that an outwardly facing bump 572 releasably fits into an inward facing depression 562 in channel 560. Barrier 530 further includes a distal portion that terminates in a first seal 532 having an opening 534 through which cable 480 passes. An intermediate portion of barrier 530 provides an additional seal by including an inner indentation 536 tightly enveloping a radial projection 540 of the proximal portion of cable 480. Barrier 530 further includes at its proximal portion a lip 538 that helps form another additional seal by bearing against o-ring 462 to further help ensure that fluid and tissue matter will not reach interior portions of handle 108 when the instrument is in use. According to some embodiments glue 554 is used to enhance the seal between barrier 530 and cable 480 as shown. According to some other embodiments, glue 554 additionally is used to mostly or fully fill the inner void 556 of barrier 530 as well. According to some embodiments, other techniques and/or combinations of techniques are used to implement the fluid barrier between the single use portion 140 and multi-use portion 150 of the

- 12 -

device 100. For example, the seal or seals can be implemented using structures such as gaskets, caps, o-rings alone, with each other and/or in combination with glues and/or ultrasonic welding or bonding techniques.

[0036] Also visible in Fig. 5 is a fluid cap 510 and gasket 512 that are shaped and positioned to provide fluid communication between a cutout 520 in shaft 122 to fluid port 114b. For simplicity, the shaft 122 is shown with two fluid lumens. One fluid lumen 502 is in fluid communication with fluid port 114b and the other fluid lumen 504 is in fluid communication with fluid port 114a. A plug 514 is inserted in the end of lumen 502 to prevent fluid communication between lumen 502 and fluid port 114a. As is described *infra*, the actual cross section of the shaft 122 can be of other layouts and the cut-outs and/or plug shapes and locations depends on the design of the fluid hub and shaft being used. According to some embodiments, transparent sealing glue 506 is used between the outer shell of the fluid hub 104 and the cap 510 and gasket 512.

[0037] According to some embodiments the fluid barrier and sealing can be implemented by one or more ultrasonic welding processes. In these cases, the outer shell 470 is manufactured as two pre-molded halves (for example split along the central longitudinal axis). Assembling two halves enhances the ability to effectively and evenly apply the glue, such as glue 506 and glue 550. According to some embodiments, certain interior structural components, such as barrier 530, gasket 512 and/or cap 510, are bonded or welded ultrasonically directly to the shell 470. In such cases, the use of glue 506 and/or 550 can be eliminated or at least supplemented. According to some embodiments, a some or all of barrier 530 is also manufactured as two halves. During assembly the placement of the glue 554 is more easily and robustly applied to form a seal between opening 534 of barrier 530 and cable 480.

[0038] Figs. 6A-6F illustrate various aspects of a cannula for a device configured for combined hysteroscopy and endometrial biopsy, according to some embodiments. Fig. 6A shows a right side view of shaft 122 of cannula 102, such a shown in device 100 of Fig. 1. The shaft 122 configured for hysteroscopy using LED lighting, camera module and forward facing fluid ports on distal tip 120 as well as for taking biopsy tissue samples using a sampling port 610. The proximal end of shaft 122 includes a cutout section 520 for making fluid communication with one

- 13 -

of the fluid lumens to a fluid port located in a fluid hub. By constructing the cannula shaft 122 from a single piece of extruded tubing, the need for additional tubes is eliminated, and it has been found that assembly yield rates are significantly improved. According to some embodiments the shaft 122 is
5 constructed of a heat and UV stabilized nylon 12 grade for tube extrusion such as Grilamid® L25. Fig. 6B is a cross sectional view along A-A', according to some embodiments. In this case, the shaft 122 is elliptical such that it is slightly taller than it is wide. In the embodiment shown, the outer walls 620 and inner walls 622 and 624 are 0.008" thick and define a central lumen 502 and two side lumens 504a and 504b. According to some embodiments, each of the side lumens 504a and 504b have a cross sectional area of 1.22mm². Also shown in Fig. 6B is the approximate location of the cutout 520. As can be seen the central lumen 502 can be connected to a fluid port via the cutout 520. According to some embodiments, the central lumen 502 is used for both the electrical cable 480 (shown in Fig. 4), as
10 well as for drawing fluid ("out-flow) so as to aid in taking tissue samples by being in fluid communication with fluid port 114b (shown in Fig. 5). The two side lumens 504a and 504b are both in fluid communication with the in-flow fluid port 114a. Note that according to this embodiment, the plug 514 shown in Fig. 5 would be used to plug the proximal end of central lumen 502, and the plug 514 has a hole for
15 allowing cable 480 to pass through it. On the distal end of the shaft 122, the two side lumens 504a and 504b are each in fluid communication with a forward facing fluid port on distal tip 120, as shown in Fig. 7B, *infra*. Fig. 6C shows another example of a cross section of shaft 122 which in this case is round, having a outer diameter of 4.3mm. Also visible in Fig. 6C is the electrical cable 480 which is
20 enclosed in a waterproof jacket.

[0039] Fig. 6D is a top view of the distal area of shaft 122, according to some embodiments. Near the distal tip 120, the sampling port 610 includes a cutting edge 612, which is sharp and positioned so as to facilitate collection of the endometrial sample by scraping. Fig. 6E is a side view showing further details of
30 the shape of distal tip 120 of shaft 122, according to some embodiments. Fig. 6F shows details of the proximal end of shaft 122 including the cut out 520, according to some embodiments.

- 14 -

[0040] Figs. 7A-C show further detail of a distal tip of a device configured for combined hysteroscopy and endometrial biopsy, according to some embodiments. Visible in Fig. 7A, on top side of distal tip 120 is the sampling port 610 used to draw fluid out of the patient's uterus as well as collect tissue. On the distal end of the tip
5 120 is lens sensor stack 750. According to some embodiments, lens sensor stack 750 consists of a lens set (which includes an iris) precisely positioned on top of a CMOS sensor. Lens sensor stack 750 is held together by a plastic (or in some embodiments stainless steel) housing or holder block 740. Glass 752 in some
10 embodiments is simply a protective glass cover, and according to some other embodiments is the first element of the lens set. Glass 752 is coated with hydrophobic or hydrophilic film. The lens sensor stack 750, holder 740 and glass 752 together are referred to herein as camera module 754. According to some embodiments the camera module 754 also includes a shield (not shown) to block direct entry of light from LEDs 730 and 732 into the sensor lens stack 750.
15 According to some embodiments, camera module 754 is about 2.2mm x 2.2mm in cross sectional size.

[0041] According to some embodiments, the CMOS sensor within lens sensor stack 750 includes a low voltage color CMOS image sensor core, image sensor processing and image output interface circuitry on a single chip such as the
20 OmniVision 7675. According to some other embodiments, an additional chip can be used to carry out video processing which is mounted on the same mini-PCB as the CMOS sensor. By providing integrated digital video processing within the sensor module, all video processing can be performed directly on the same PCB as the CMOS sensor, or on the same substrate in which the CMOS is formed such
25 that the imaging plane of the CMOS and the plane along which the video processing circuits extend substantially coincide. In this example, the video signal from the sensor module can be in any suitable video format, such as NTSC, PAL, or another common video format, so that no further video processing would be required to drive widely available displays for common video formats such as TV
30 displays, tablets, computers and hospital workstations.

[0042] Two LEDs 730 and 732 are positioned above and below and mounted to the camera module 754 to evenly illuminate the uterine tissue for visual inspection. According to some embodiments each of the LEDs 730 and 732 are

- 15 -

about 1.0mm x 0.5mm in frontal area. One problem in performing visual inspections of endometrial tissues, and particularly in situations where the endometrial medium, consisting of free tissue, loosely attached tissue and/or fluid, is relatively thick, is that light reflected from tissue particles suspended close to the lens can appear overly-bright and therefore impair imaging of other tissue surfaces. As can be seen in Fig. 7B, which is a front view of distal tip 120, two forward facing fluid ports, 720 and 722 are provided to allow fluid to exit the tip and tend to push suspended particulate matter away from the camera so as to enhance image and video capture by camera module 754. In some cases some tissue debris may collect on the distal surface such that imaging would be impaired in such cases the forward facing ports are useful in clearing away such collected tissue. Also it has been found that the forward facing ports are helpful in aiding insertion of the cannula in many cases as the fluid provides lubrication as well as a partial distending of tissues just ahead of the distal tip during insertion. Since the forward facing ports improve visualization, the risk of accidental damage to the uterus is greatly reduced. Fig. 7C is a perspective view of the holder block 740 which according to some embodiments is made of a suitable plastic material, such as liquid crystal polymer. The distal tip 120 in this case includes separated fluid channels for fluid in-flow and out-flow. In particular, the central fluid lumen 502 is in fluid communication with the sampling port 610, and is blocked via the holder block 740 from being in fluid communication with the forward facing ports 720 and 722. Similarly, the two side fluid lumens 504a and 504b are in fluid communication with forward facing fluid ports 722 and 720, respectively.

[0043] In performing a hysteroscopy procedure, it has been found that providing a device that has separated fluid flow channels for in-flow and out-flow has certain benefits including allowing for simultaneous in-flow and out-flow. Fig. 8 is a flow chart illustrating aspects of using a multi-lumen cannula with simultaneous in-flow and out-flow for a hysteroscopy procedure, according to some embodiments. In step 810, the cannula 102 is inserted through the cervix into the patient's uterus while in-flowing fluid through the in-flow lumen(s) such as lumens 504a and 504b shown in Fig. 6B or 6C, and through forward facing ports such as ports 720 and 722 shown in Fig. 7B. In step 812, the endometrial cavity is visually examined by viewing live images from the sensor in the camera module 754

- 16 -

(shown in Fig. 7A) and on the integrated display 110 shown in Figs. 1 and 3.

Suction is applied to the out-flow port (port 114b, shown in Fig. 1, 2 and 5) to allow for a continuous flow of fluid which maintains clear visibility by removing blood mucus and other opaque material such as tissue debris. In an optional step 814,

5 after visualization is completed, one or more endometrial tissue samples can be obtained by turning off the inflow port and applying suction to the outflow port.

Samples can be obtained from a side facing port such as port 610 shown in Figs.

6A, 6D and 6E. The location of the biopsy sampling be based on the areas of pathology identified by the visual inspection step 812 to allow for a directed biopsy.

10 Additionally according to some embodiments where conditions allow it, visualization can continue during step 814 allowing for further visual confirmation of the location of the biopsy. In step 816 the cannula is withdrawn from the patient.

[0044] It has been found that it is very useful to provide the device 100 as

divided into two portions: a single use portion, such a portion 140 in Fig. 1, and a

15 re-usable portion 150 in Fig. 1. According to some embodiments, the re-usable portion includes the handle and integrated display, where some of the more costly components (such as the display) as well as some of the components that may be difficult or impractical to be re-sterilized (such as some of the electronic

components) are located. According to some embodiments the separable design

20 shown allows for different types of single-use portions to be provided that each are configured to operate with a single re-usable portion. Examples of different types

of single use portions include cannulas having different port configurations

(including the presence or absence of a side-facing port), different fluid hub layout

configurations (including the number of fluid ports), as well cannulas having

25 different bend locations and amount, as well as different flexibility characteristics.

The selection of which cannula design to use can be a matter of preference by the

user but can also be influenced by anatomical variables, as well as what type of

procedure is being performed. For example, according to some embodiments at

least three main types of single-use cannula are provided that are all compatible

30 with a re-usable handle and display portion: (1) a diagnostic cannula having in-flow

capability for distention and visualization, but without a dedicated out-flow port for

sampling; (2) a combined visualization and biopsy cannula which is configured for

both visualization and taking tissue samples (for example single-use portion 140);

- 17 -

and (3) an operative cannula that includes visualization as well as a working channel for performing one or more different types of surgical procedures.

[0045] Figs. 9A-9G illustrate a single-use portion that includes a cannula configured for fluid-in flow and visualization, according to some embodiments. As shown in Fig. 9A, the hysteroscopy device 900 comprises a single-use portion 940 with a sliding connector 906 that is configured to mate with re-useable portion 150 that has been shown and described elsewhere herein. The single use portion 940 also includes a fluid hub 904 having a single fluid port 914 that is in fluid communication with a single fluid lumen within shaft 922. Cannula 902 includes a shaft 922 and a distal tip 920 which includes one more more forward facing in-flow ports, a camera module and LED lighting as will be described in further detail herein. Fig. 9B is a right side view of the shaft 922, and Fig. 9C is a cross section along A-A'. As can be seen in Fig. 9C, there is two lumens in shaft 922. Circular lumen 902 has an inner diameter of 1.5mm that contains the electrical cable 980 between the distal tip 920 and the connector 906. Crescent-shaped fluid lumen 904 is in fluid communication with the fluid port 914 at the proximal end of shaft 922 and with forward facing in-flow ports on the distal tip 920. According to some embodiments, the cross sectional area of fluid lumen 904 is about 2.43mm². Providing a hysteroscopy device having fluid in-flow capabilities with an outer diameter of less than about 4mm has been found to be desirable, and according to even more preferred embodiments the outer diameter of shaft 922 is less than about 3.6mm. In the example shown in Fig. 9C, the outer diameter of shaft 922 is 3.4mm, and an outer wall thickness of 0.016 inches. Fig. 9D is a right side view showing further detail of the distal end of shaft 922, according to some embodiments. According to some embodiments, shaft 922 is constructed of a heat and UV stabilized nylon 12 grade for tube extrusion such as Grilamid® L25.

[0046] Fig. 9E is a left side view of the distal end of device 900, showing a separate distal tip shell 942 that surrounds a holder block 940. Shell 942 can be made, for example, of acrylic or other suitable material. The holder block 940 houses lens sensor stack 950 which can be of the same design as lens sensor stack 750 described herein. According to some embodiments, the distal tip shell 942 is tapered as shown such that the most distal end is of larger dimension than the proximal end (where it mates with the shaft 922). It has been found that

- 18 -

providing a device with variable dimensions, in particular larger distal tip paired with a narrower shaft, allow for certain advantages in facilitating fluid management (which is described in greater detail with respect to Fig. 11), as well as providing for more frontal area for the front facing fluid ports, LEDs and camera module.

5 According to some embodiments the diameter of the distal end of tip shell 942 is 4.0mm. It has been found that a differential of 0.4mm is beneficial for fluid management during many applications. Fig. 9F is a perspective view of the distal tip 920, and shows the lens 952, which may be covered by a glass cover, as well as two LEDs 930 and 932. Two forward facing in-flow fluid ports 934 and 936 are
10 also provided on the distal end of tip 920 as shown, and are in fluid communication with the fluid lumen 904 in shaft 922 and also to fluid port 914 on fluid hub 904. Fig. 9G is a perspective view of holder block 940 which according to some embodiments is made of a suitable plastic material, such as liquid crystal polymer.

[0047] Fig. 10 is a cross section showing details of a sealed sliding connector
15 for a device for hysteroscopy, according to some embodiments. As described, the sliding connector 906 is compatible with the re-useable handle 108. The fluid hub 904 and connector 906 are similar or identical to hub 104 and connector 106 in many respects other than being configured for only a single fluid-carrying lumen in the cannula shaft as well as a single fluid port on hub 904. A fluid cap 1010 and
20 gasket 1012 that are shaped and positioned to provide fluid communication between lumen 904 shaft 922 to fluid port 914. According to some embodiments, transparent sealing glue 1006 is used between the outer shell of the fluid hub 904 and the cap 1010 and gasket 1012. The sliding connector 906 is shown here with an outer shell 1070 that includes a lip 472 that fits over an o-ring seal 462 and a
25 protruding mating portion 460 of the handle assembly 108. Other seals can be provided along the length of connector 906 to further isolate handle 108 from patient matter and/or fluids that could otherwise contaminate and/or cause connection failure such as electrical failures on handle 108. The cable 980 carries video signals and control signals between the camera module and LEDs at distal
30 tip 920 to connection pins housed within sleeve 460. The sleeve 460 fits into a closed channel on the handle 108 while the connection pins 552 mate with pin receptacles 452 as to form electrical connections the pins. The sliding connector 906 includes a barrier 530 that fits tightly inside outer shell 1070. According to

- 19 -

some embodiments, a transparent sealing glue 550 is applied between the barrier 530 and shell 470. Barrier 530 terminates at its proximal end in an extended sleeve 460 that fits into a closed channel 560 in handle 108 such that an outwardly facing bump 572 releasably fits into an inward facing depression 562 in channel 560. Barrier 530 further includes a distal portion that terminates in a first seal 532 having an opening 534 through which cable 480 passes. An intermediate portion of barrier 530 provides an additional seal by including an inner indentation 536 tightly enveloping a radial projection 1040 of the proximal portion of cable 980. Barrier 530 further includes at its proximal portion a lip 538 that helps form another additional seal by bearing against o-ring 462 to further help ensure that fluid and tissue matter will not reach interior portions of handle 108 when the instrument is in use.

[0048] FIG. 11 is a flow chart showing aspects of using a variable dimension cannula for visual inspection of a patient's uterus, according to some embodiments. The steps shown in Fig. 11 assume that a variable dimension cannula is being used for the visual inspection, such as cannula 902 in which the shaft of the cannula has a smaller diameter than the distal tip. By using a smaller shaft, fluid can be allowed to drain from the uterus. This is because after larger diameter tip is inserted through the cervix, the portion of the cannula that is in touch with the cervix is kept small which allows the fluid to drain.

[0049] In step 1110, the patient is on the exam table. In step 1112 the packaging enclosing the sterile single-use portion (e.g. portion 940 in Fig. 9A) is opened and the single-use portion is attached to the re-usable portion (e.g. portion 150 in Fig. 1 and 9A). In step 1114 the device (e.g. device 900 in Fig. 9A) is turned on and a manual white balance procedure is carried out if desired or needed. In step 1116 a fluid tube and syringe or pressurized fluid bag containing saline or other distending fluid is attached to the fluid port of the device (e.g. port 914 in Fig. 9A). In step 1118, the distal end of the cannula is inserted into the cavity, such as through the cervix to the uterus, under direct vision using the camera module and integrated display screen while fluid is being infused. In step 1120, the uterus is visually inspected, again under direct vision using the camera module and integrated display screen. In step 1122, if the view is impaired by blood or debris in the cavity the cannula can be advanced into the cavity so that the narrow portion is

- 20 -

in the entrance (e.g. the cervix), thus allowing leakage of fluid around the cannula shaft while fluid is infused through the forward facing ports at the distal end of the cannula. This allows for continuous flow of fluid, which aids in obtaining improved visual images from the camera module. In step 1124, if there is more leakage than is
5 needed in order to maintain the desired distension of the uterus, then the cannula can be withdrawn so that the wider diameter distal tip is within the entrance so as to effectively block a significant portion of leakage from the uterus. In step 1126, optionally, the syringe can be used to draw fluid out (out-flow) to obtain samples from the uterus. In step 1128, the cannula is withdrawn from the uterus and the
10 procedure is completed. According to some embodiments, as mentioned in optional step 1126, sampling and/or biopsy can be carried out via the two forward facing ports on the distal end.

[0050] Conventional video endoscopes are typically either rigid or flexible. The rigid scopes have a rigid, non-bendable elongated body with a precision rod lens
15 set inside as relay optics. On the other hand, flexible endoscopes are made of flexible elongated body. The tip portion of a flexible endoscope can be bendable or steerable by embedded cable wire that is attached to the levers at the proximal end. The rigid scope is rigidly attached to the scope body and handle so it can be moved in a fashion as a typical rigid body can be moved. On the other hand, the
20 flexible endoscope is weakly coupled to the scope handle or body, and therefore has limited control by the handle and endoscope body. In either case, the handle or scope body has to be moved which is often undesirable.

[0051] According to some embodiments, a semi-flexible (or semi-rigid) endoscope is provided. In one embodiment, the elongated body (the scope
25 cannula) can be easily manipulated spatially to achieve the best visualization of cavity such as a distended uterus or knee joint. Optimal flexibility (or stiffness/rigidity) of the cannula allow the operator clinician to bend or steer the cannula without moving the scope handle or scope body. For example, using a device such as device 100 of Fig. 1 or device 900 of Fig. 9A, the operator can use
30 one hand to hold the handle 108, using one finger to control visualization using the LED lighting and/or snap buttons, while the operator uses the other hand to grasp the cannula at some intermediate point along the shaft (e.g. 5 inches from the distal tip) to bend and/or steer the cannula. According to some other

embodiments, a selection from multiple cannulas having different lengths is made according to the size of the cavity which is being evaluated.

[0052] Figs. 12A-12C illustrate a test setup to measure flexibility of a cannula shafts used in a device for hysteroscopy and/or combined hysteroscopy and endometrial biopsy, according to some embodiments. Fig. 12A shows a test set up in which the cannula shaft 122 is held firmly at a point 10 inches from the distal tip, while a force from a mass of 10 grams is applied to a point that is 2 inches from the distal tip. Fig. 12B shows shaft 122 in a bent state (in dotted lines) under the force applied as shown. In this example the distal tip was moved 35mm from the applied force. Fig. 12C show the shaft 122 held at a different point, 5 inches from the distal tip, while a force from a different mass, 30 grams, is applied to a point 2 inches from the distal tip. In this example, the distal tip is deflected 10 mm under the applied force. Tables 1 and 2 show the tip deflections for a cannula shaft 122 which includes separated in-flow and out-flow fluid paths such as for shown in Fig. 6A. Table 1 shows the measured tip deflections when the shaft is held 10 inches from the distal tip and Table 2 shows the measured tip deflections when the shaft is held 5 inches from the distal tip.

Weight (g)	Tip down (mm)
10	35
20	70
30	100
40	130
50	145

Table 1. Cannula Having Separate In-flow and Out-flow Paths. Held at 10 inches from distal tip, and loading weight at 2 inches from distal tip.

Weight (g)	Tip down (mm)
10	2
20	6
30	10
40	14
50	17
70	25
90	35

100	39
150	60
170	70
200	80

Table 2. Cannula Having Separate In-flow and Out-flow Paths.
Held at 5 inches from distal tip, and loading weight at 2 inches from distal tip.

5

[0053] Similarly, Tables 3 and 4 show the tip deflections for a cannula shaft 922 which includes a single fluid path such as for shown in Fig. 9B. Table 3 shows the measured tip deflections when the shaft is held 10 inches from the distal tip and Table 4 shows the measured tip deflections when the shaft is held 5 inches 10 from the distal tip.

Weight (g)	Tip down (mm)
5	75
10	100
15	135
20	150

Table 3. Cannula Having Single Fluid Paths.
Held at 10 inches from distal tip, and loading weight at 2 inches from distal tip.

Weight (g)	Tip down (mm)
5	4
10	8
15	13
20	18
30	26
40	32
50	41
70	55
90	70
100	75
120	85

150	95
170	100
200	105

Table 4. Cannula Having Single Fluid Path.

Held at 5 inches from distal tip, and loading weight at 2 inches from distal tip.

[0054] It has been found that multiple fluid path cannulas having flexibilities of
 5 between 60% less deflection (i.e. more stiff), and 40% greater deflection (i.e. less
 stiff) than the examples shown in Tables 1-2 are suitable for many applications,
 according to some embodiments. More preferably, cannulas having multiple fluid
 paths should have flexibilities of between 30% less deflection and 25% greater
 deflection than the examples shown in Tables 1-2. Even more preferably,
 10 cannulas having multiple fluid paths should have flexibilities of between 15% less
 deflection and 10% greater deflection than the examples shown in Tables 1-2. It
 has been found that single fluid path cannulas having flexibilities of between 75%
 less deflection (i.e. more stiff), and 50% greater deflection (i.e. less stiff) than the
 examples shown in Tables 3-4 are suitable for many applications, according to
 15 some embodiments. More preferably, cannulas having a single fluid path should
 have flexibilities of between 50% less deflection and 25% greater deflection than
 the examples shown in Tables 3-4. Even more preferably, cannulas having a
 single fluid path should have flexibilities of between 25% less deflection and 10%
 greater deflection than the examples shown in Tables 3-4. Another advantage of
 20 providing flexibility and stiffness characteristics as described is a potential
 reduction in risks of injury such as by perforation of the uterine wall.

[0055] Although internal shaft structures shown in Figs. 6A, 6B, and 9C have
 been shown and described herein, other internal structures can be provided
 according to some other embodiments. Fig. 13 is a cross section showing an
 25 example of a different internal shaft structures within a cannula for a device for
 hysteroscopy and/or combined hysteroscopy and endometrial biopsy, according to
 some embodiments. In Fig. 13, cannula shaft 1322 includes two fluid lumens are
 provides for separated in-flow and out-flow channels. The wall 1330 defines and
 upper lumen 1304 that, for example can be used for out-flow, as well as a lower

- 24 -

lumen 1302 that can be used for both in-flow as well as housing the electrical cable 1380 which is enclosed in a waterproof jacket.

[0056] Figs. 14A-14B illustrate aspects of a cannula for a device configured for combined hysteroscopy and endometrial biopsy, according to some alternative
5 embodiments. A cannula 1402 is shown that has a variable diameter (a wider distal tip 1420 and narrower shaft 1422). The cannula 1402 also includes a fluid hub 1404 and sliding connector (not shown) that mates with a re-usable portion that can include a handle and integrated display screen (such as portion 150 in
10 Figs. 1 and 9A). In this case, for purposes of fluid management, a slideable sleeve 1430 is positioned surrounding cannula shaft 1422 can be used to plug the entrance of the body cavity to prevent fluid from draining out of the cavity. The sleeve 1430 can be a soft material and cylindrical in shape disposed such that it surrounds the cannula shaft 1422, or according to some embodiments sleeve 1430 can be a piece that can be mounted on the shaft 1422 after insertion of the tip
15 1420.

[0057] Although the junction between the single use portion 140 and the re-usable portion 150 is shown between the fluid hub and handle 108 in Figs. 1 and 9A, according to some embodiments the junction can be positioned in other locations. It has been found that the most costly components of the endoscopic
20 device are associated with the integrated display. As such, according to some embodiments, the single use portion can include the handle, while the re-usable portion includes the display. Figs. 15A-15C illustrate a device for hysteroscopy and/or combined hysteroscopy and endometrial biopsy having a single use cannula, fluid hub and handle, and a re-usable display screen, according to some
25 embodiments. Figs. 15A and 15B show a device 1500 having a single use portion 1550 and a re-usable display screen 110 in a display screen assembly 1510. The single use portion includes: a cannula 102 that has a distal tip 120 and shaft 122; a fluid hub 140 that has a fluid port 114; a handle 1508 and a sliding connector 1506. According to some embodiments, the cannula 102 and fluid hub 104 can be as
30 described herein with reference to Figs. 1-5, 6A-F and 7A-C. According to some other embodiments the cannula and fluid hub can be identical or similar to the cannula 902 and fluid hub 904 shown in Figs. 9A-G and 10. The handle 1508 can include the control buttons, electronics and battery, such as handle 108 described

- 25 -

herein. According to some embodiments in-order to reduce the cost of the single-use portion 1550, some or all of the system electronics 1522 and/or the battery 1520 can be located in the display screen assembly 1510. A sliding connector 1506 forms a connection between the display assembly 1510 and the handle 1508.

5 The sliding connector 1506 preferably includes some or all of the fluid barriers and seals described with respect to connector 106, in order to prevent fluid from entering mating portion of the connector 1506 and/or the system electronics and LCD display in display assembly 1510.

[0058] Fig. 15C is a perspective view of device 1500 with the sliding
10 connector 1506 disconnected. The sliding connector mates with a connector 1550 on display assembly 1510. According to some embodiments, one or more of on/off button 1530, LED lighting control button 1532 and "snap" button 1534 can be located on the display assembly 1510 so that the user can control the device 1500 using hardware buttons, which may be easier to use with gloved or wet hands, for
15 example, while maintaining a low-cost single-use portion 1550. According to some other embodiments, soft-buttons can be used on touch screen 110 on display assembly 1510.

[0059] Although the foregoing has been described in some detail for purposes of clarity, it will be apparent that certain changes and modifications may be made
20 without departing from the principles thereof. It should be noted that there are many alternative ways of implementing both the processes and apparatuses described herein, including for using the described devices or certain aspects thereof for hysteroscopy but not for endometrial biopsy, or for endometrial biopsy but not for hysteroscopy, or for endoscopy and/or biopsy other than of the uterus.
25 For example, in some applications the device shown in Figs. 50-51 could also be used for taking fluid and/or fluid/tissue endometrial samples through the forward facing fluid parts. Accordingly, the present embodiments are to be considered as illustrative and not restrictive, and the body of work described herein is not to be limited to the details given herein, which may be modified within the scope and
30 equivalents of the appended claims.

- 26 -

CLAIMS

What it claimed is:

1. A low-cost medical instrument for examining a patient's uterus, said instrument comprising:
 - a single-use portion configured to in a single insertion distend and image a patient's uterus, the single-use portion including:
 - an elongated conduit having a distal portion configured and dimensioned for insertion into the patient's uterus, and a proximal portion;
 - a fluid connection port formed at the proximal portion of the conduit;
 - one or more distal openings at the distal portion of the conduit configured to provide fluid from the conduit and into the uterus;
 - an imaging system at the distal portion of the conduit configured to image the uterus and provide video signals;
 - an illumination system at the distal portion of the conduit configured to illuminate the uterus at an illumination field viewed by said imaging system; and
 - an electrical cable extending from a proximal end of the conduit to the imaging system and configured to carry video signals and control signals;
 - a multiple-use portion having interior and exterior surfaces, the multiple-use portion being configured to be attached to the single-use portion for a single use and then detached after a single use, and to be re-used with a second single-use portion without sterilization of the interior surfaces, said multiple-use portion comprising an integral image display that is electrically coupled with said imaging system at least in part by the electrical cable, the display being configured to display images provided by the imaging system for viewing by a user; and
 - one or more seals configured to keep fluid in the conduit from contacting any of the interior surfaces of said multiple-use portion.

- 27 -

2. An instrument according to claim 1 wherein said multiple-use portion further comprises a handle having an off-axis profile so as to facilitate grasping by the user's hand and for rotation and tilting of the instrument in use, the handle including a plurality of buttons to control a plurality of features of the instrument, wherein when said single-use and multiple-use portions are attached to one another, the display, handle, elongate member and imaging system are mounted in a fixed relationship so as to rotate about a longitudinal axis of the elongate member in rotational alignment.
3. An instrument according to claim 1 wherein said single-use portion further comprises a handle having an off-axis profile so as to facilitate grasping by the user's hand and for rotation and tilting of the instrument in use.
4. An instrument according to claim 3 wherein said multiple-use portion includes a rechargeable battery and electronics disposed along with said integral image display within a multi-use display housing, and said multi-use display housing is configured to slidably attach to said handle of said single-use portion.
5. An instrument according to claim 1 wherein the conduit comprises:
a first fluid channel in fluid communication with at least a first of the one or more distal openings and with said fluid connection port; and
a second fluid channel in fluid communication with at least a second of the one or more distal openings and with a second fluid connection port formed at the proximal portion of the conduit.
6. An instrument according to claim 5 wherein the instrument is configured for a medical procedure in which said distal portion is inserted into the patient's uterus to simultaneously provide (a) improved visual inspection using the electronic imaging system by delivering fluid flow in a distal direction by introducing fluid under positive pressure into said fluid connection port, which fluid passes through said first fluid channel and enters the uterus through at least the first distal opening, (b) drawing fluid under negative

- 28 -

pressure from said second fluid connection port, which fluid is drawn from the uterus and into the instrument through at least the second distal opening and passes through said second fluid channel and out of said second fluid connection port, and (c) image of the uterus by illuminating the uterus with said illumination system and imaging the illuminated uterus with said imaging system.

7. An instrument according to claim 1 wherein said elongated conduit being semi-flexible such that when fixedly held at 5 inches from a tip of the distal portion and a 50 gram mass is attached at a location two inches from the tip, the distal portion bends in a downwards direction between 10mm and 80mm.
8. An instrument according to claim 1 wherein at least on of the one or more seals is at least partially formed by one or more ultrasonic welding processes during manufacture.
9. An integrated endoscopic instrument for examining a patient's uterus, said instrument comprising:
 - an elongate member having a proximal end and a distal end, said elongate member being dimensioned and configured to facilitate insertion of the distal end through a patient's cervix and into the uterus, and said elongate member being semi-flexible such that when fixedly held at 5 inches from the distal end and a 50 gram mass is applied two inches from the distal end the distal end bends in a downwards direction between 2mm and 60mm;
 - an imaging system at the distal portion of the conduit configured to image the uterus and provide video signals;
 - an illumination system at the distal portion of the conduit configured to illuminate the uterus at an illumination field viewed by said imaging system;
 - a fluid opening positioned at the distal end of the elongate member to improve visual inspection using the electronic imaging module by

- 29 -

delivering fluid to flow in a distal direction thereby clearing debris close to the imaging module;

a handle that is configured and dimensioned to be grasped by a user's hand and manipulated by a user; and

an integral image display and an electrical cable, wherein the display is electrically coupled with said imaging system at least in part through the electrical cable, the display being configured to display images provided by the imaging system for viewing by the user.

10. An instrument according to claim 9 wherein the elongate member includes a fluid port at the proximal end and a shaft extending from the distal end to the proximal end, the shaft housing the electrical cable and a first fluid channel in fluid communication with the fluid opening at the distal end and with the fluid port at the proximal end, and wherein the elongate member when fixedly held at 5 inches from the distal end and a 50 gram mass is applied two inches from the distal end the distal end bends in a downwards direction between 4mm and 55mm.
11. An instrument according to claim 10 wherein the shaft has an outer diameter of less than 4mm, and the elongate member when fixedly held at 5 inches from the distal end and a 50 gram mass is applied two inches from the distal end the distal end bends in a downwards direction between 10mm and 50mm.
12. An instrument according to claim 11 wherein the shaft has an outer diameter of less than 3.6mm, and the elongate member when fixedly held at 5 inches from the distal end and a 50 gram mass is applied two inches from the distal end the distal end bends in a downwards direction between 20mm and 45mm.
13. An instrument according to claim 10 wherein the shaft further includes a second fluid opening at the distal end and a second fluid port at the proximal end and has an outer diameter of greater than 4mm, and further includes a

- 30 -

second fluid channel in fluid communication with the second fluid opening positioned at the distal end of the elongate member and with the second fluid port at the proximal end, and wherein the elongate member when fixedly held at 5 inches from the distal end and a 50 gram mass is applied two inches from the distal end the distal end bends in a downwards direction between 4mm and 34mm.


14. An instrument according to claim 13 wherein the elongate member when fixedly held at 5 inches from the distal end and a 50 gram mass is applied two inches from the distal end the distal end bends in a downwards direction between 8mm and 21mm.
15. An instrument according to claim 13 wherein the second fluid opening is a side-facing sampling opening in the elongate member located and dimensioned and configured to facilitate in collection of endometrial tissues.
16. An instrument according to claim 11 wherein the instrument is configured for a medical procedure in which said distal portion is inserted into the patient's uterus to simultaneously provide (a) improved visual inspection using the electronic imaging system by delivering fluid flow in a distal direction by introducing fluid under positive pressure into said fluid port, which fluid passes through said first fluid channel and enters the uterus through at least the fluid opening at the distal end, (b) drawing fluid under negative pressure from said second fluid port, which fluid is drawn from the uterus and into the instrument through at least the second fluid opening and passes through said second fluid channel and out of said second fluid port, and (c) image of the uterus by illuminating the uterus with said illumination system and imaging the illuminated uterus with said imaging system.
17. An integrated endoscopic instrument for examining a patient's uterus, said instrument comprising:
an elongate member having a proximal end, a distal end, and a shaft extending from the distal end to the proximal end, said shaft housing

- 31 -

a fluid channel and a plurality of electrical conductors, said conductors configured to carry video and control signals, said shaft having a first outer diameter of less than 5mm and said distal end having a second outer diameter greater than the first outer diameter; an imaging system at the distal portion of the conduit configured to image the uterus and provide video signals; an illumination system at the distal portion of the conduit configured to illuminate the uterus at an illumination field viewed by said imaging system; a distal facing fluid opening at the distal end of the elongate member and in fluid communication with the fluid channel, said opening being positioned to improve visual inspection using the electronic imaging module by delivering fluid to flow in a distal direction thereby clearing debris close to the imaging module; a handle that is configured and dimensioned to be grasped by a user's hand and manipulated by a user; and an integral image display that is electrically coupled with said imaging system at least in part by at least some of the plurality of electrical conductors, the display being configured to display images provided by the imaging system for viewing by the user.

18. An instrument according to claim 17 wherein the first outer diameter is less than 3.8mm.
19. An instrument according to claim 18 wherein the second outer diameter is at least 0.4mm greater than the first outer diameter.
20. An instrument according to claim 17 wherein the second outer diameter is greater than 3.5mm.
21. An instrument according to claim 20 wherein the second outer diameter is at least 0.4mm greater than the first outer diameter.

Fig. 1

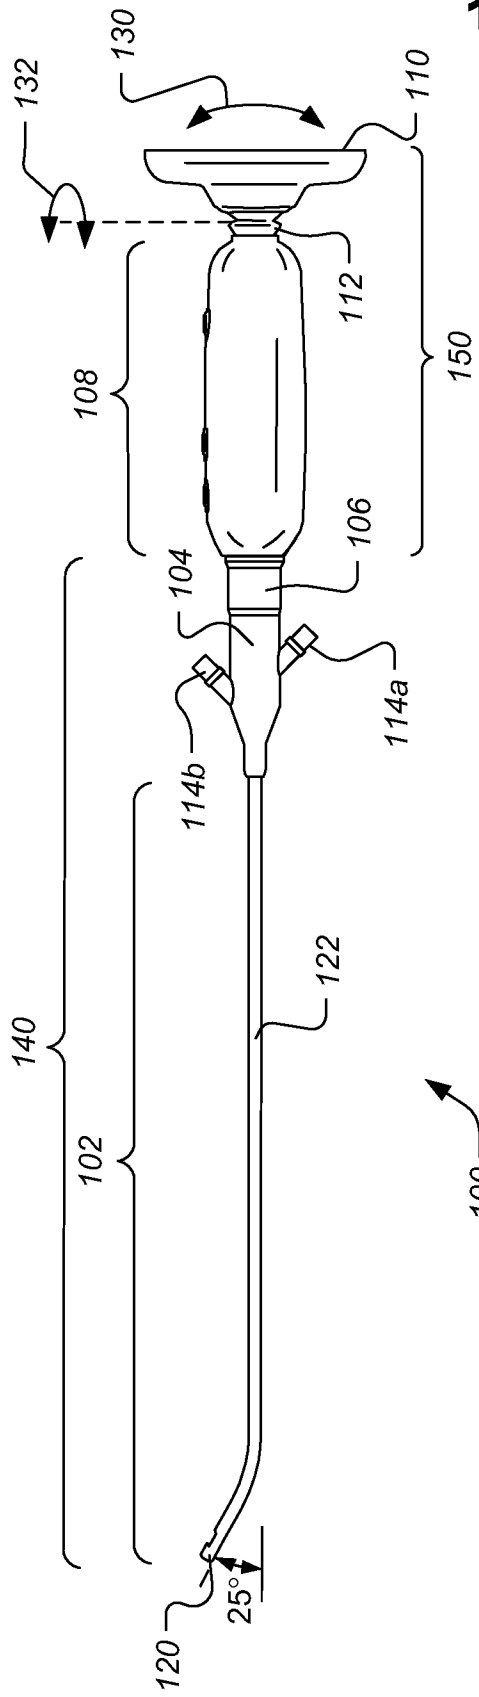

1 / 16

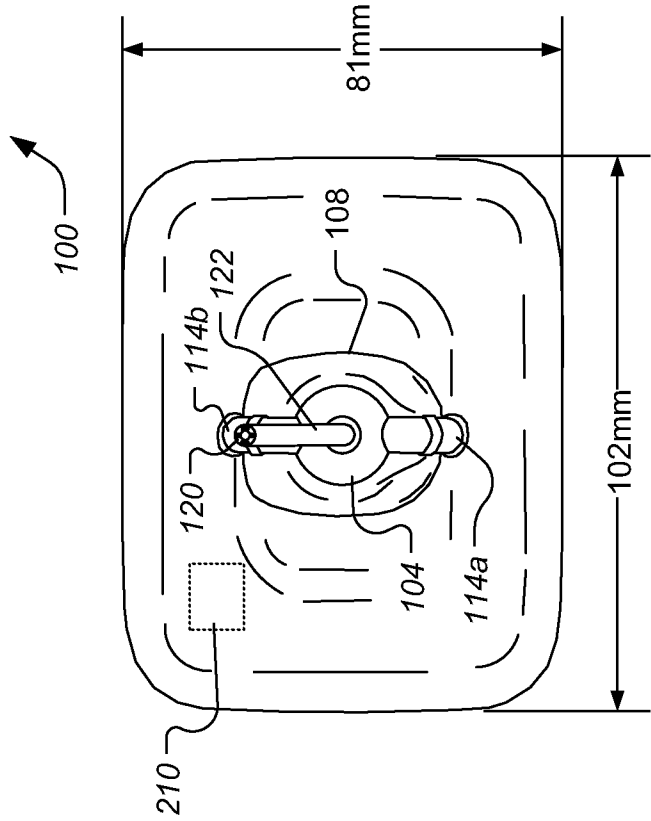


Fig. 3

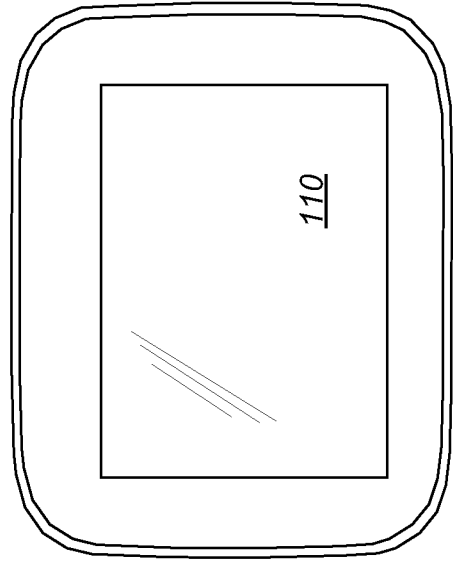
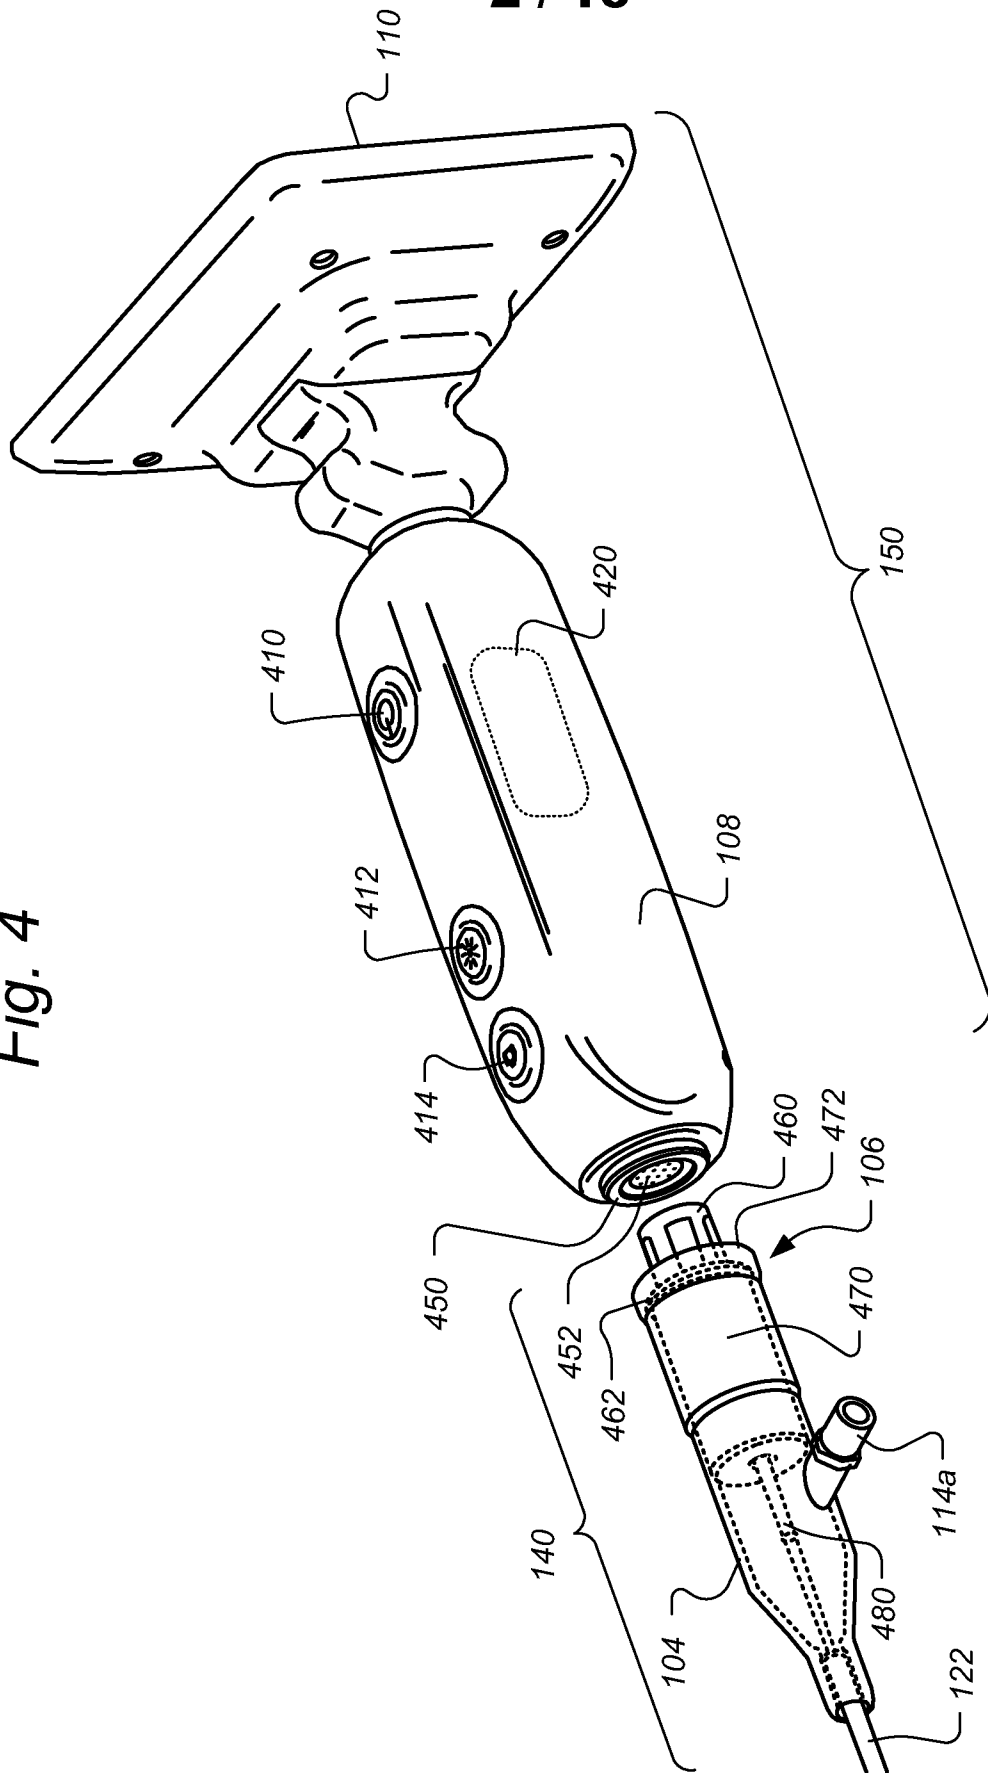


Fig. 2

Fig. 4



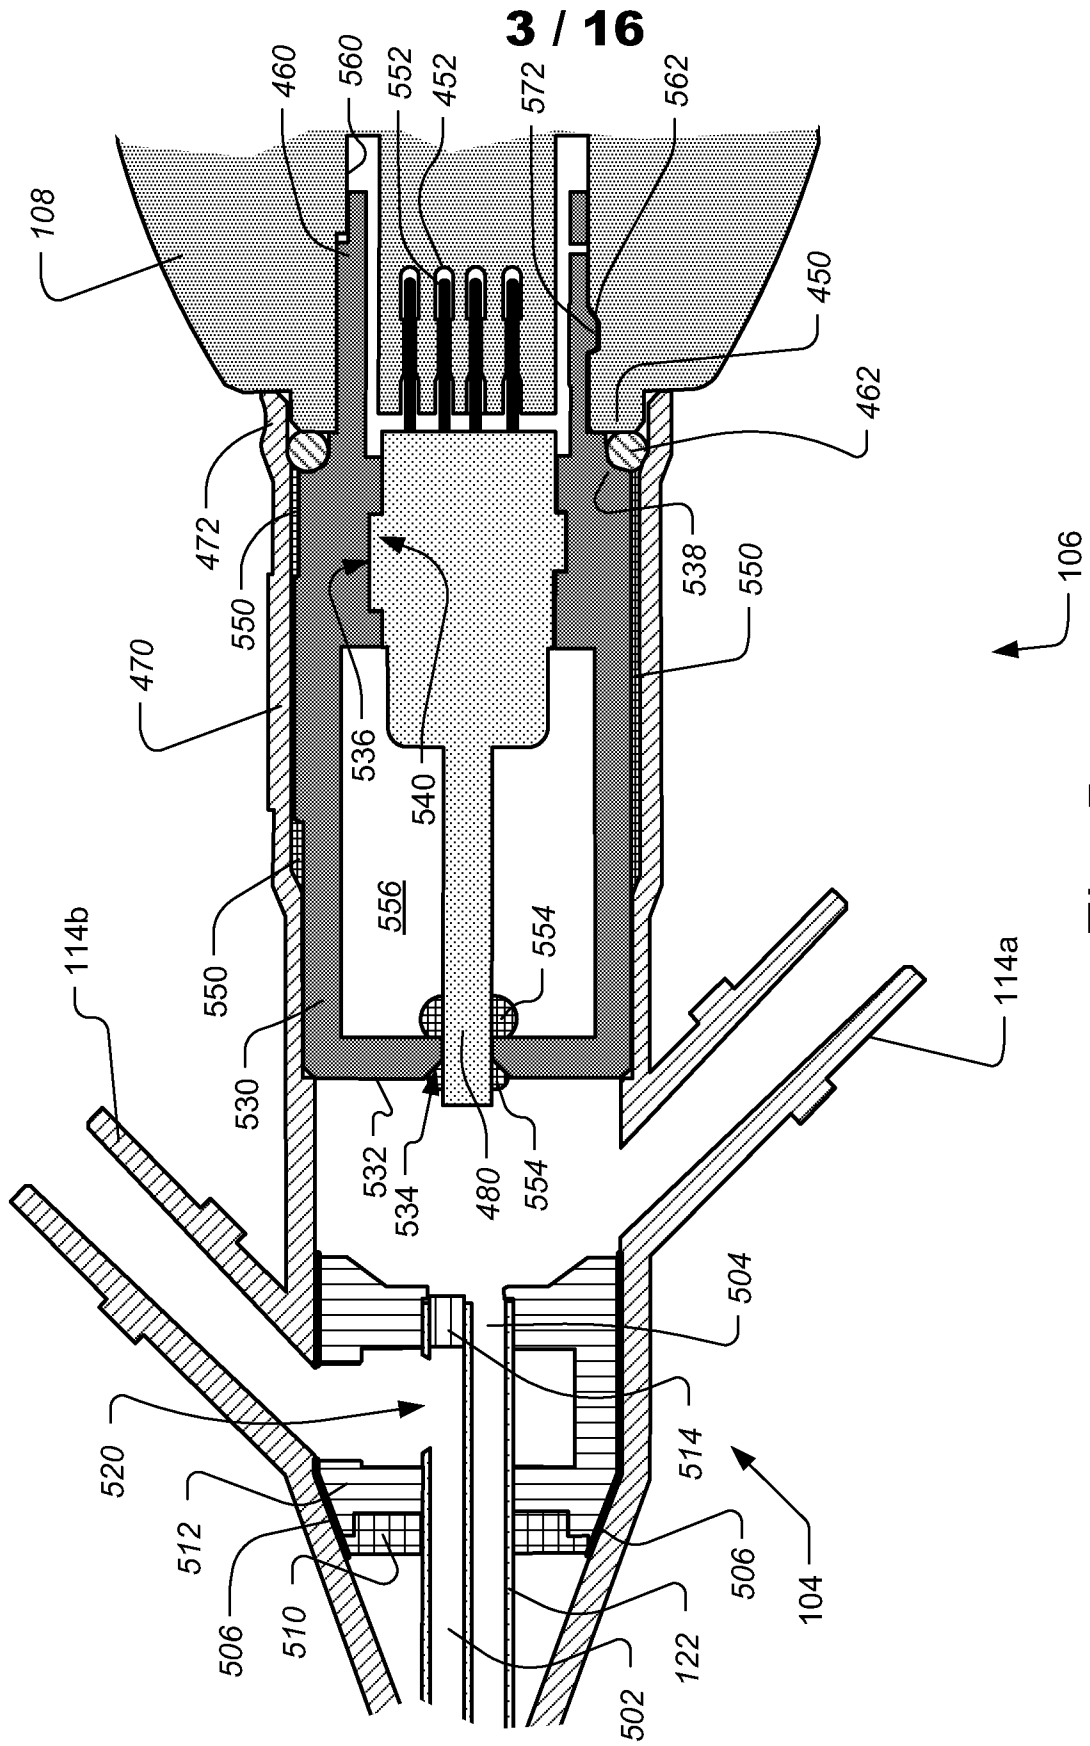


Fig. 5

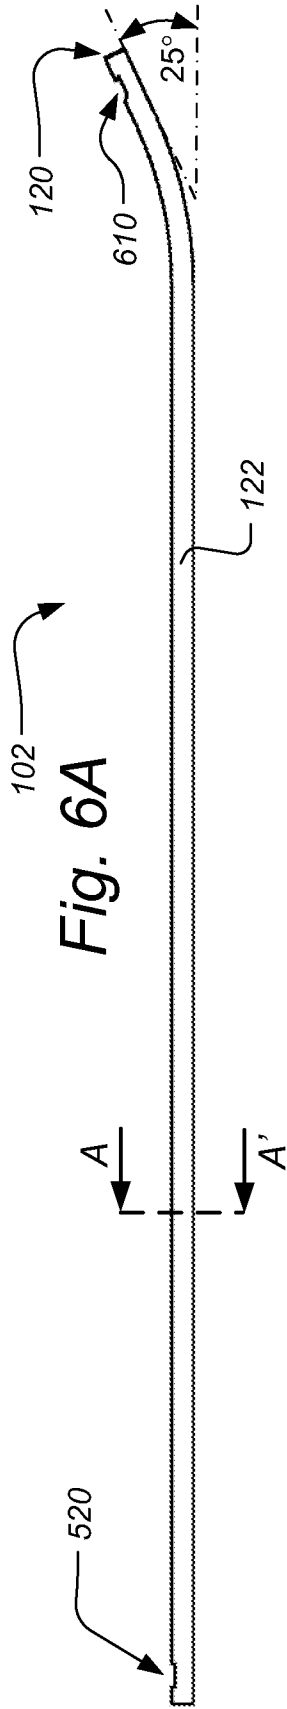


Fig. 6B (A-A')





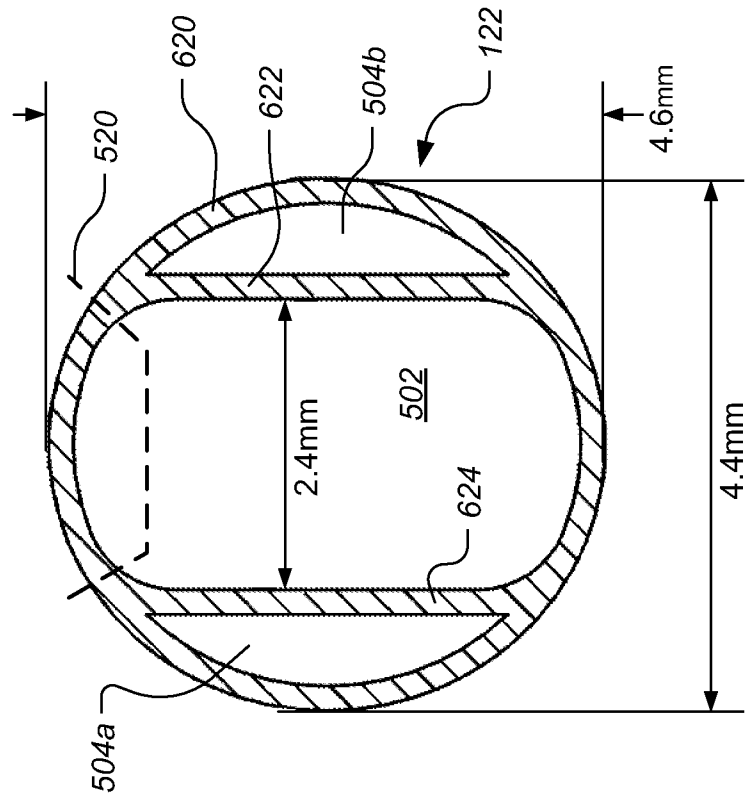


Fig. 6C

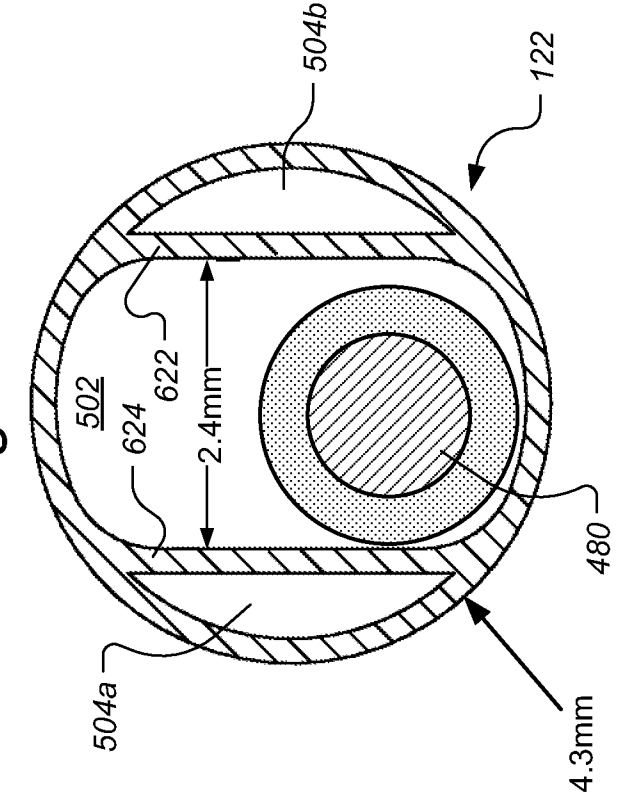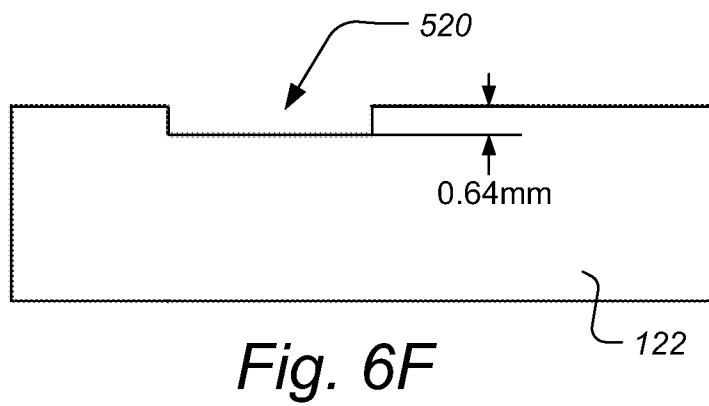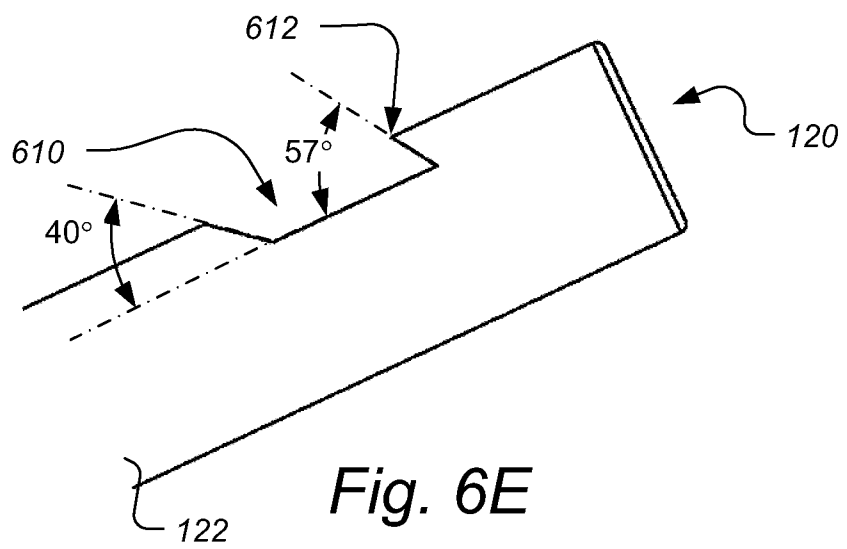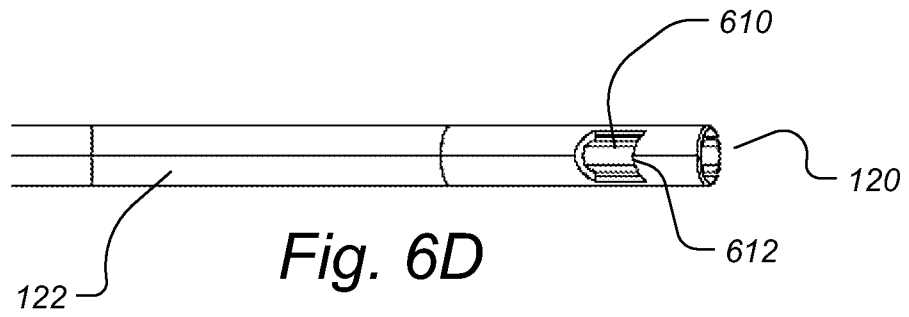

5 / 16



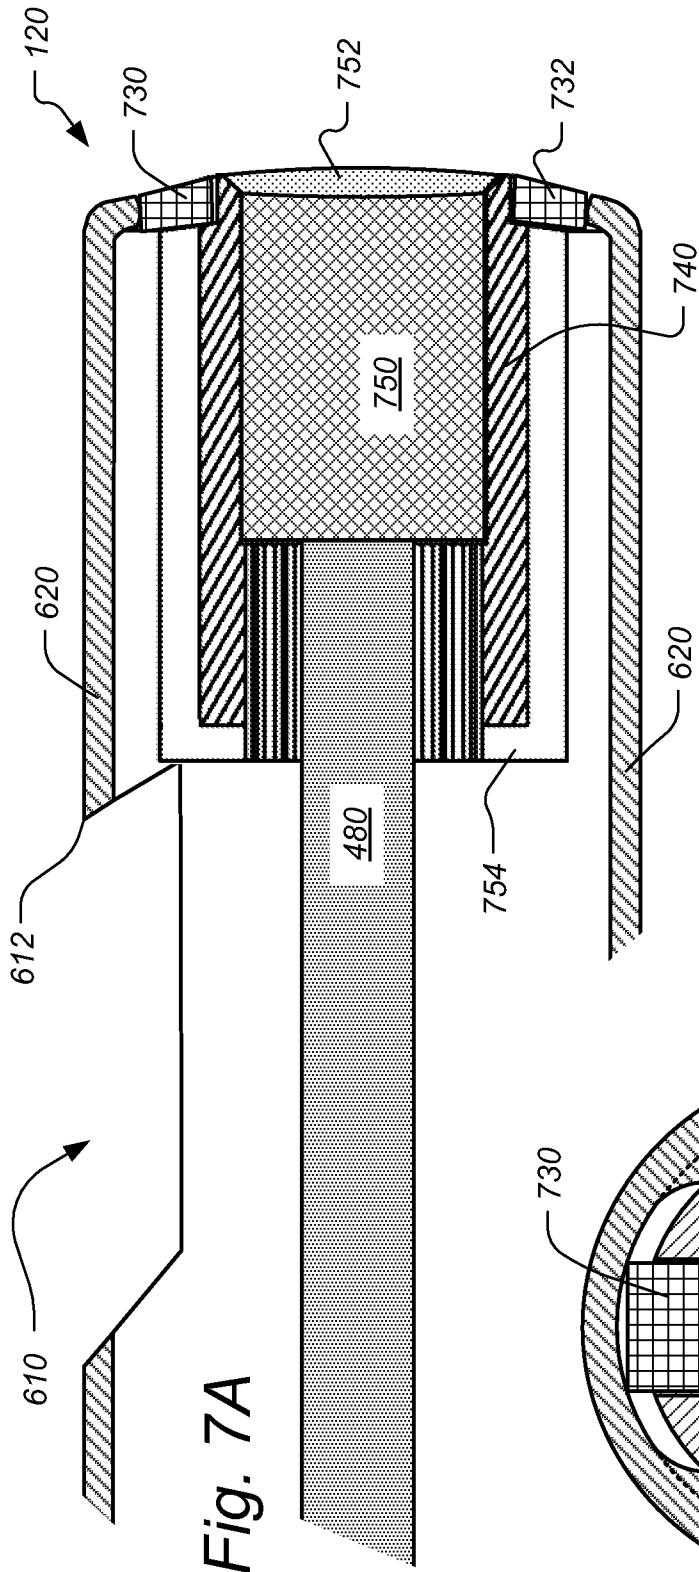


Fig. 7A

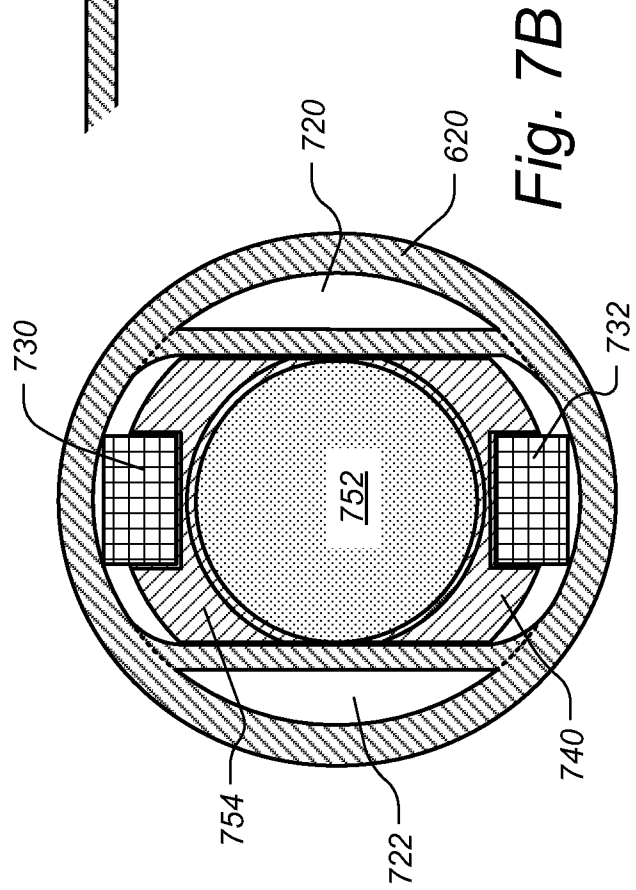


Fig. 7B

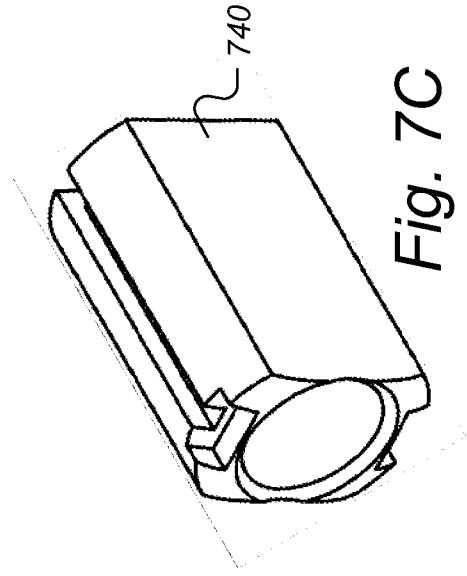
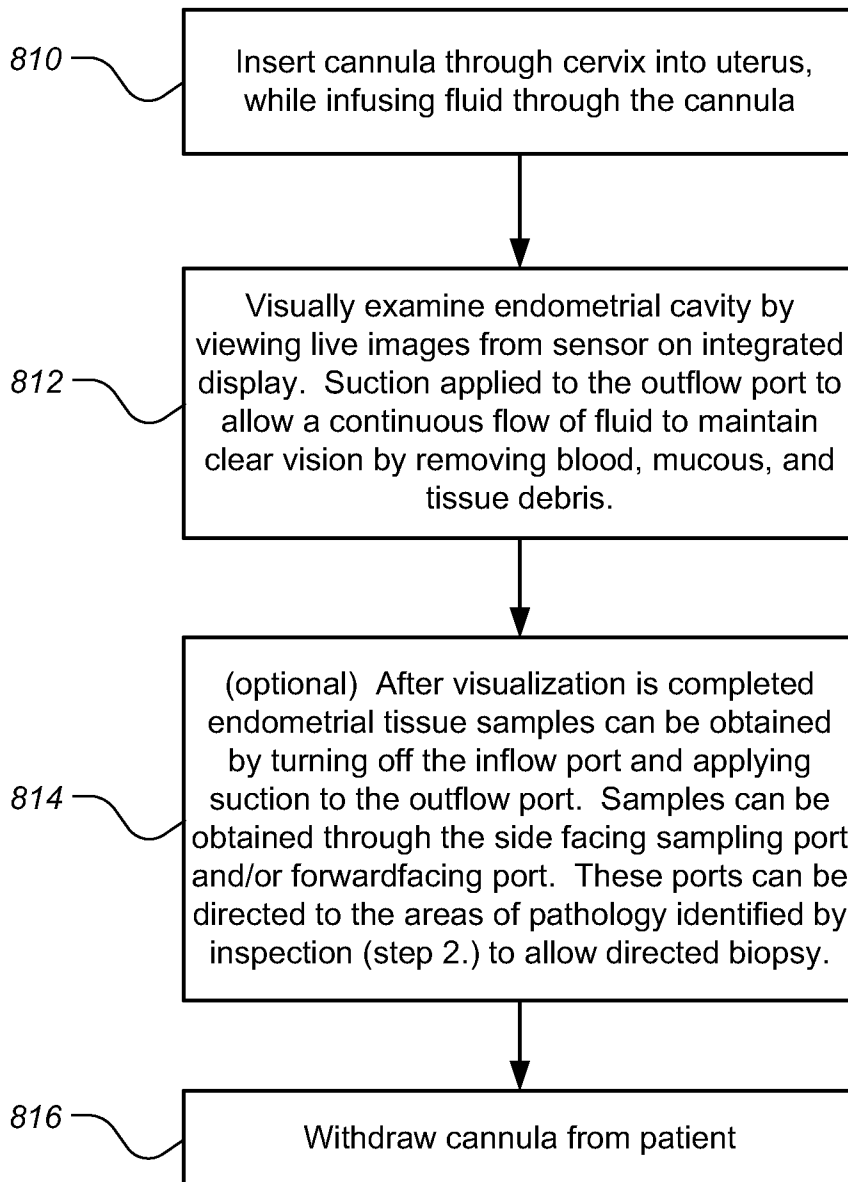


Fig. 7C

7 / 16*Fig. 8*



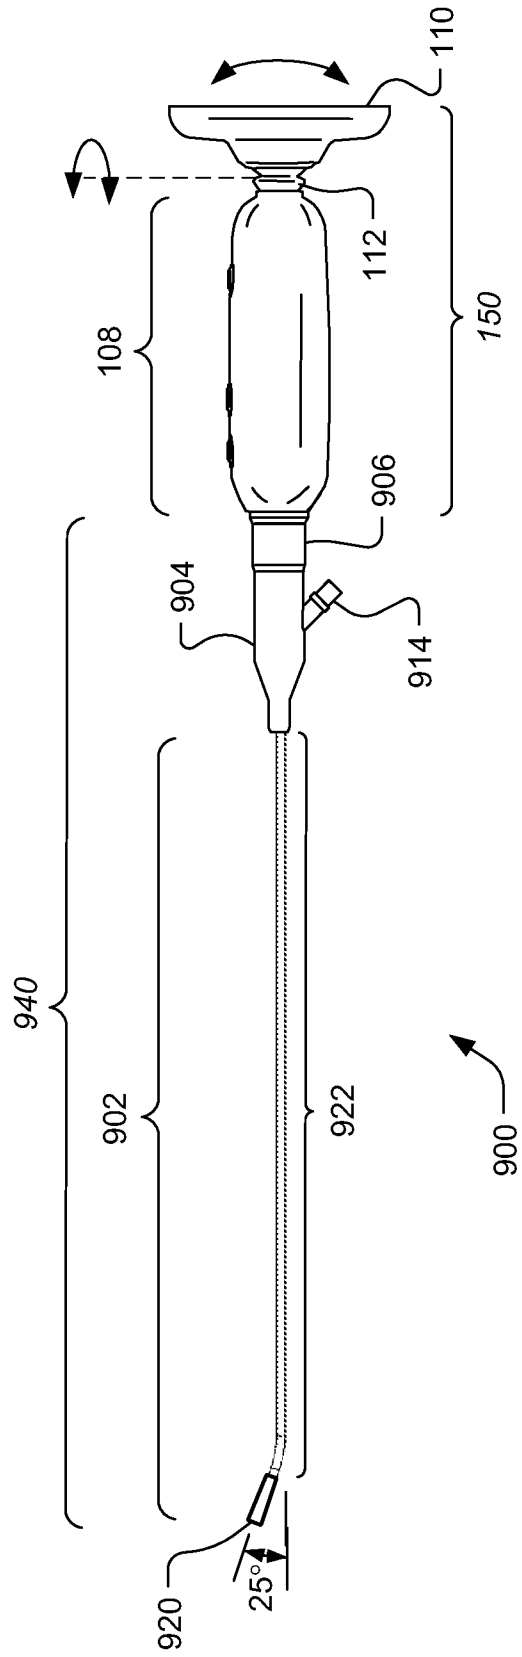


Fig. 9A

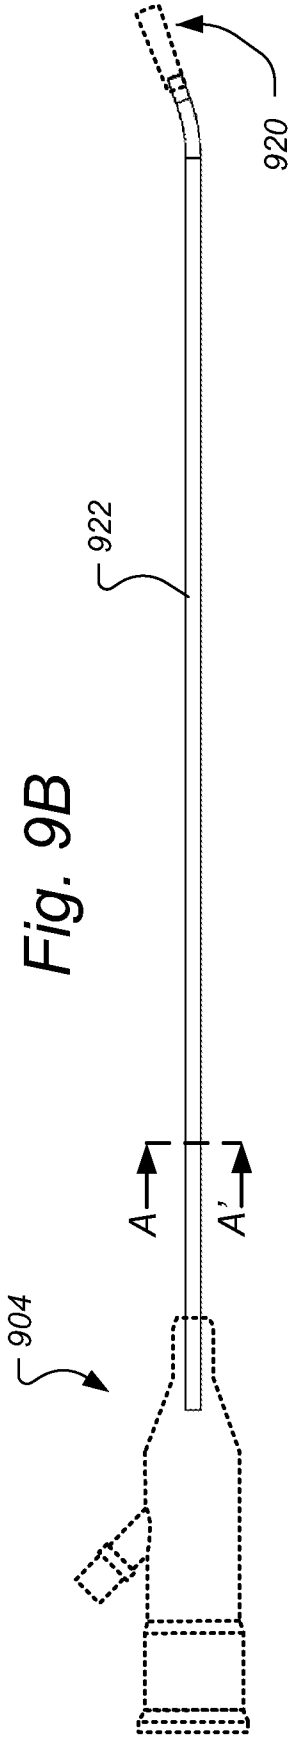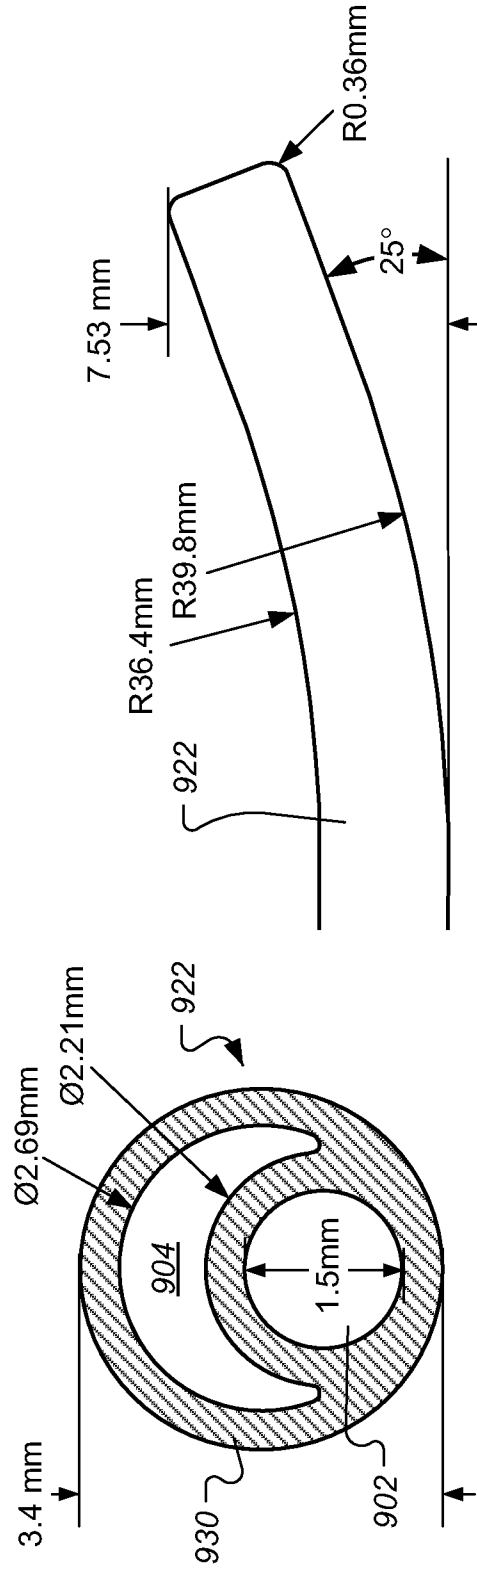

9 / 16



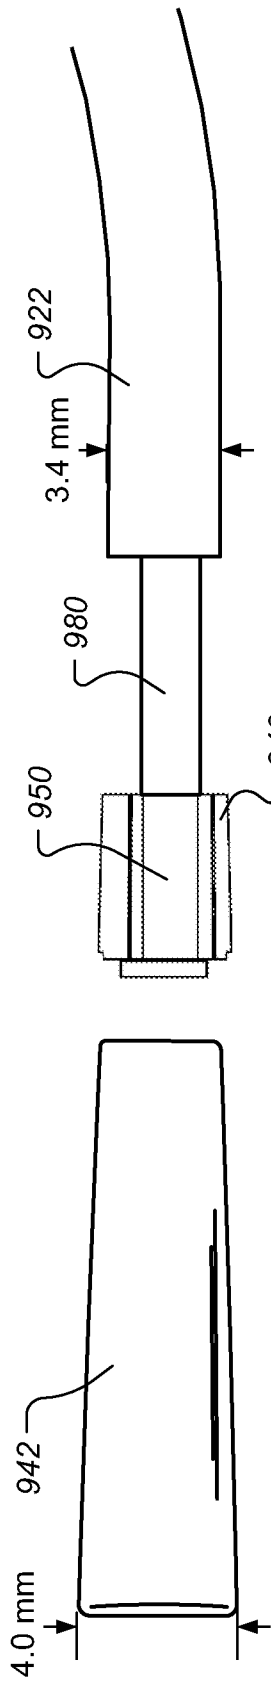


Fig. 9E

920

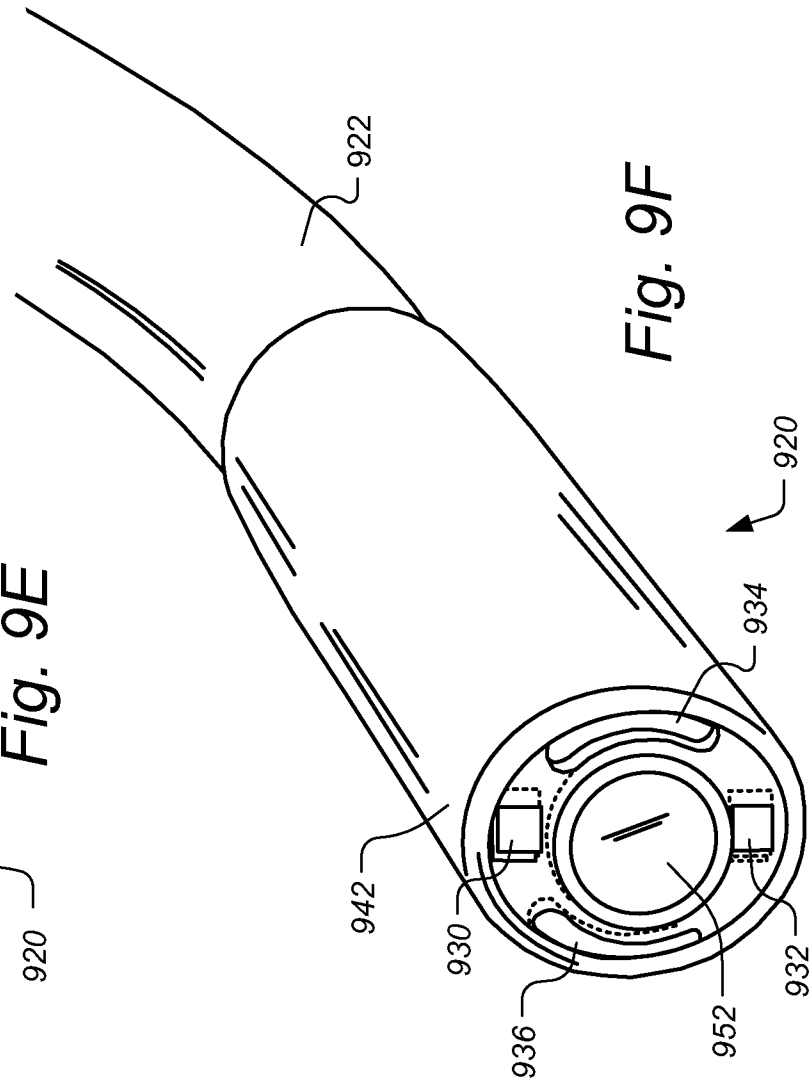


Fig. 9F

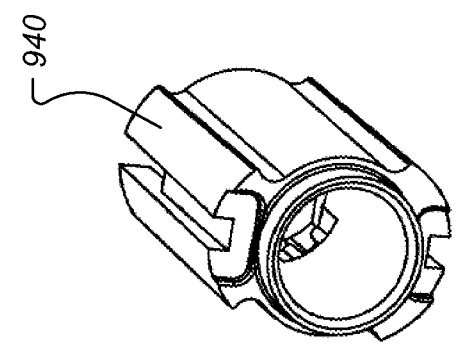
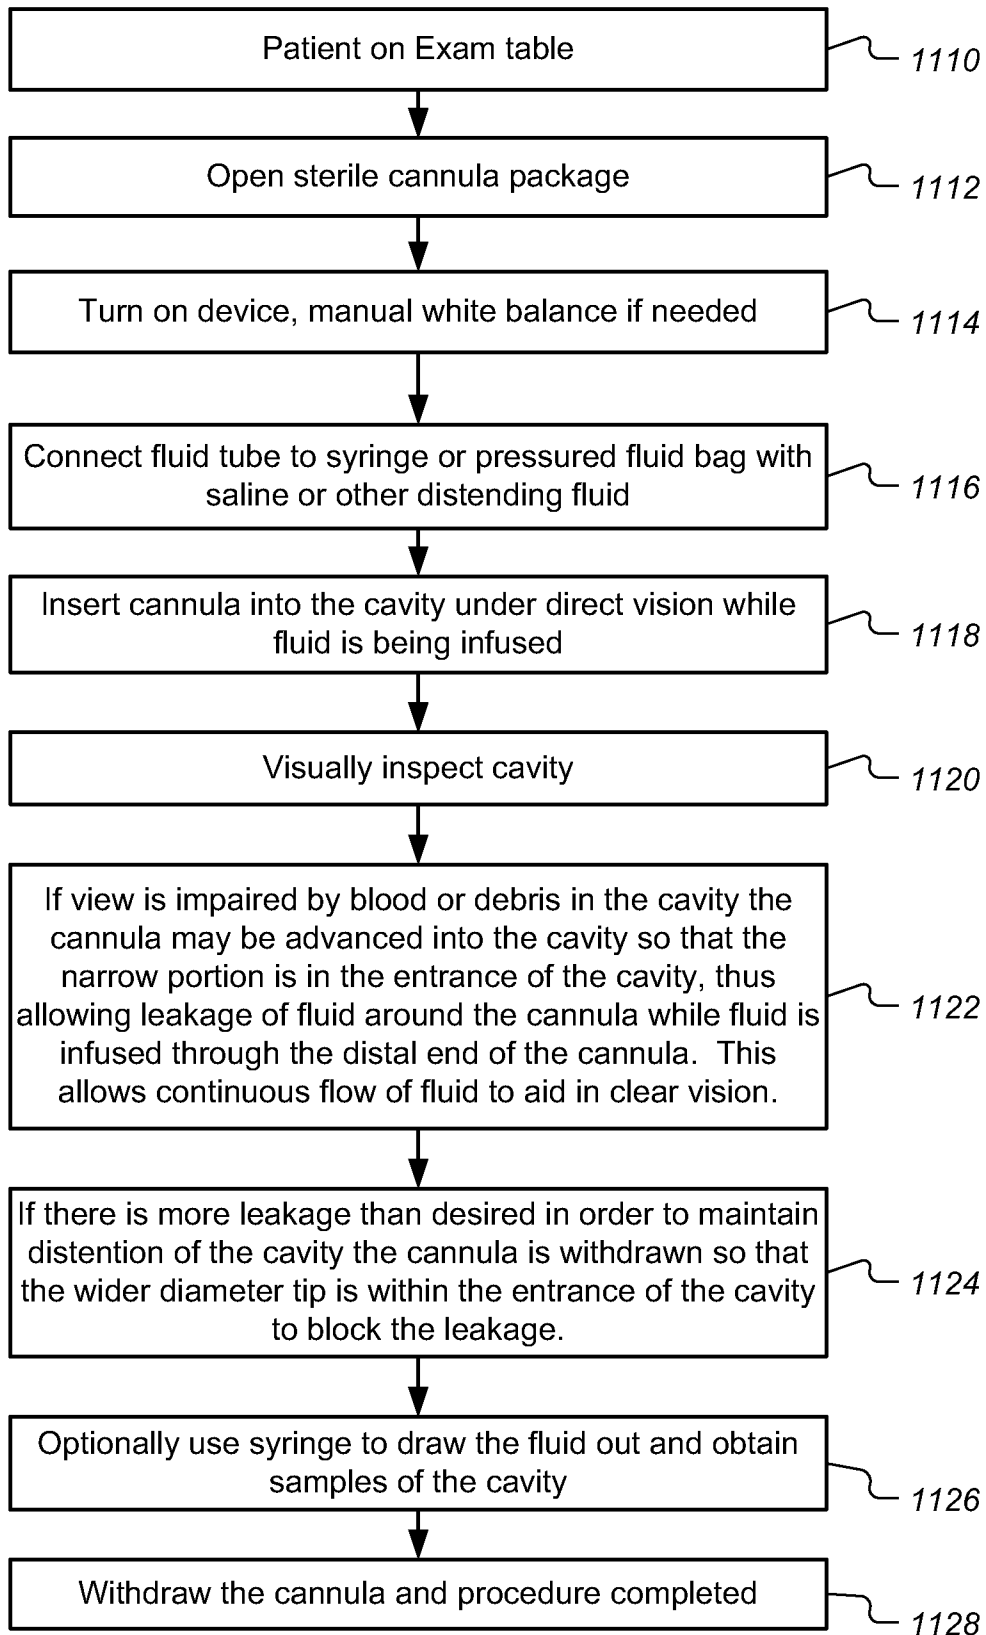


Fig. 9G

12 / 16*Fig. 11*

13 / 16

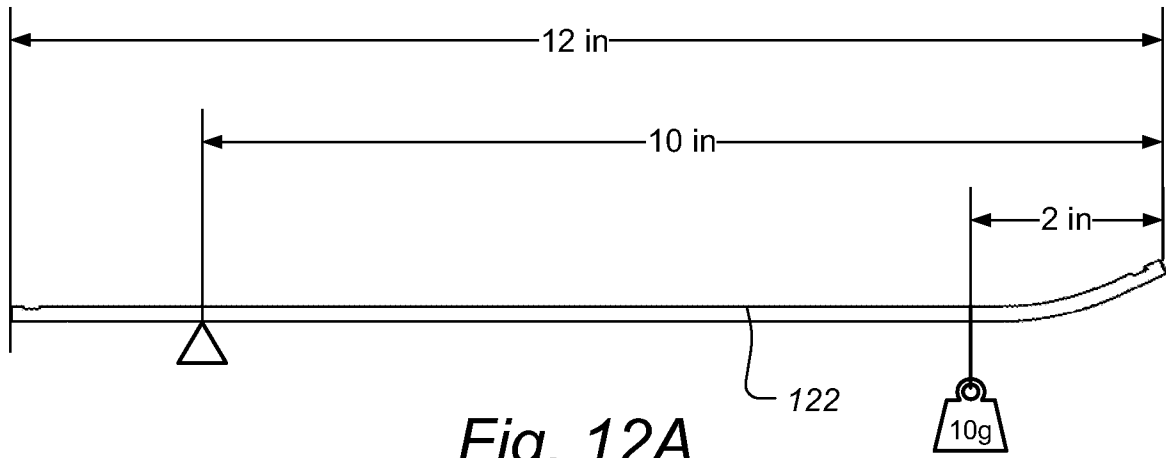


Fig. 12A

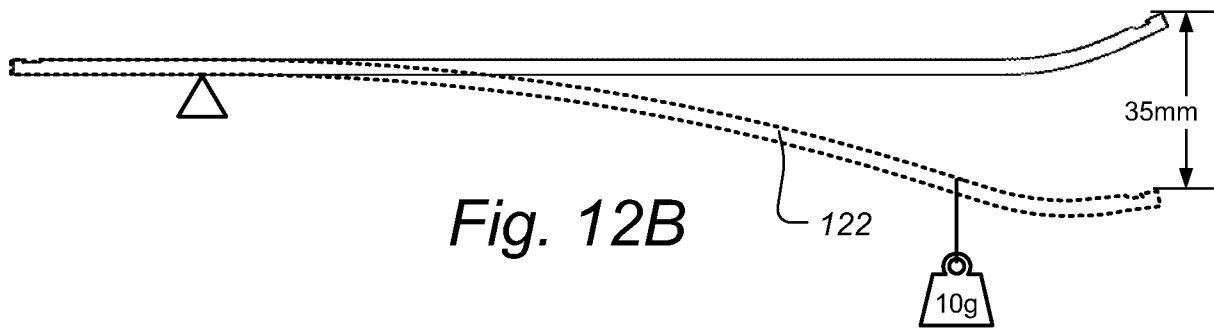


Fig. 12B

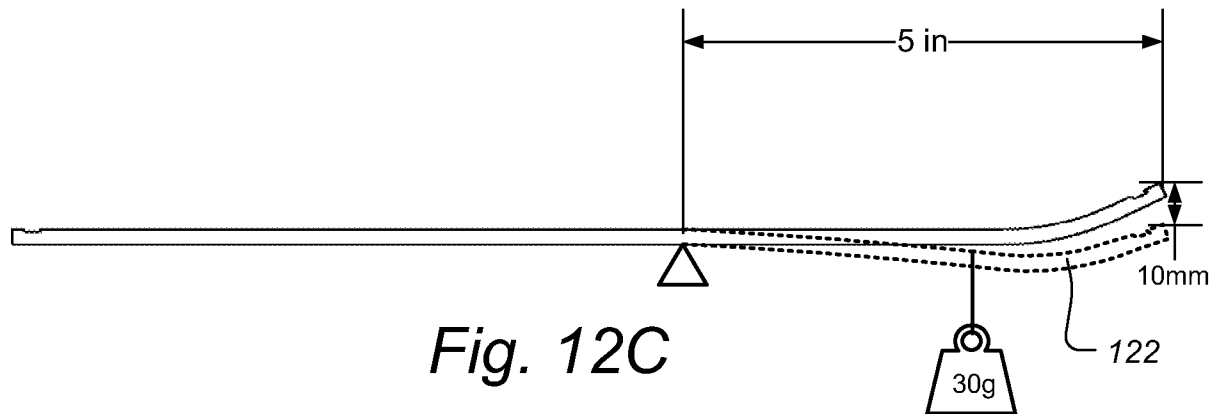


Fig. 12C

14 / 16


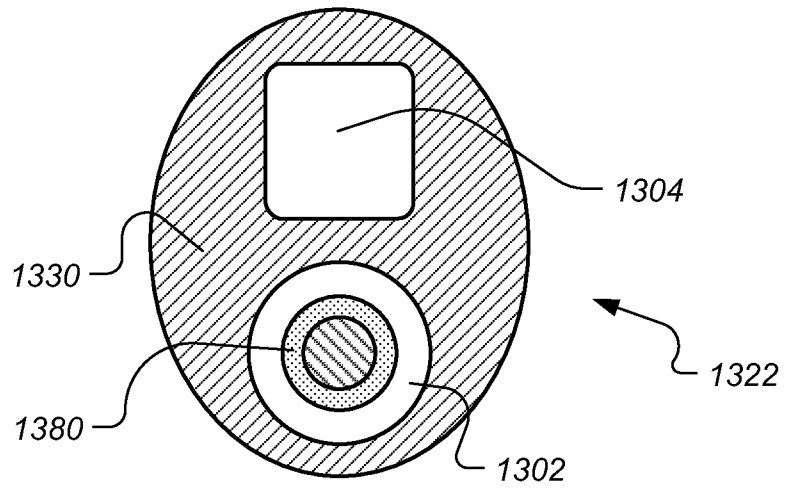


Fig. 13

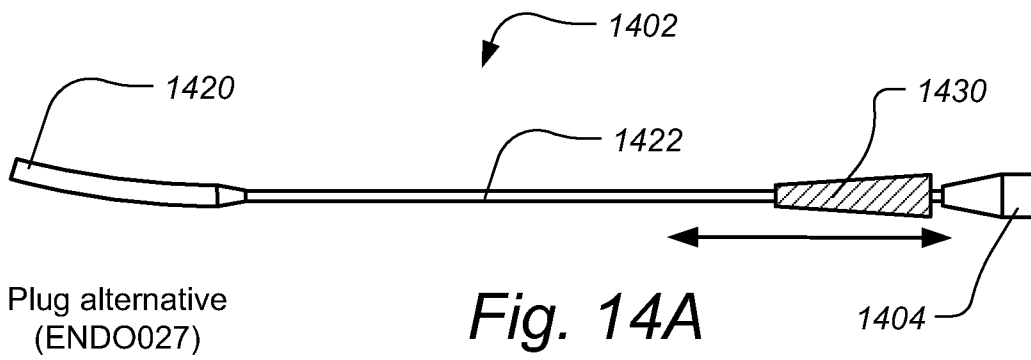

Plug alternative
(ENDO027)

Fig. 14A

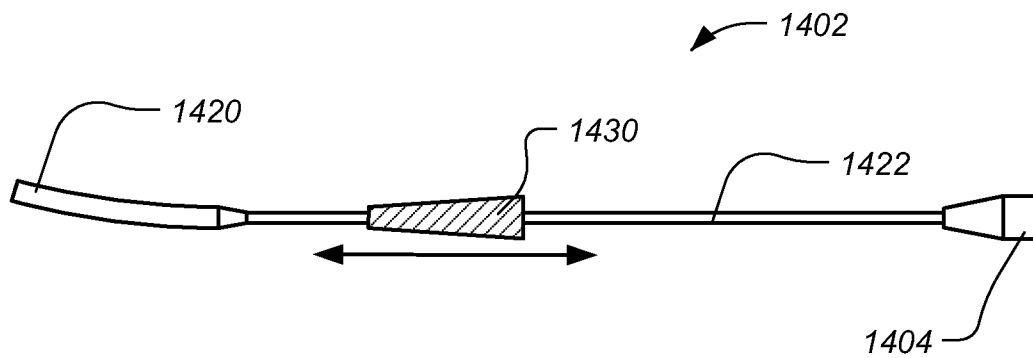
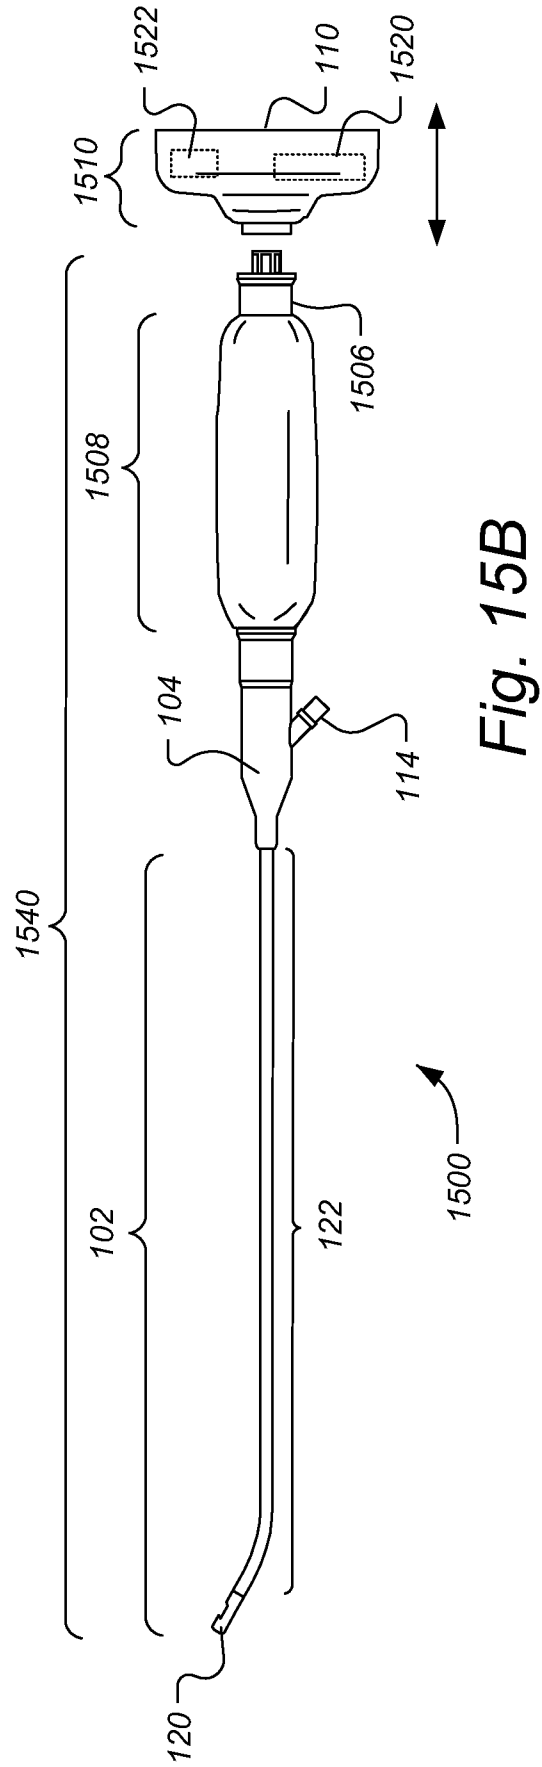
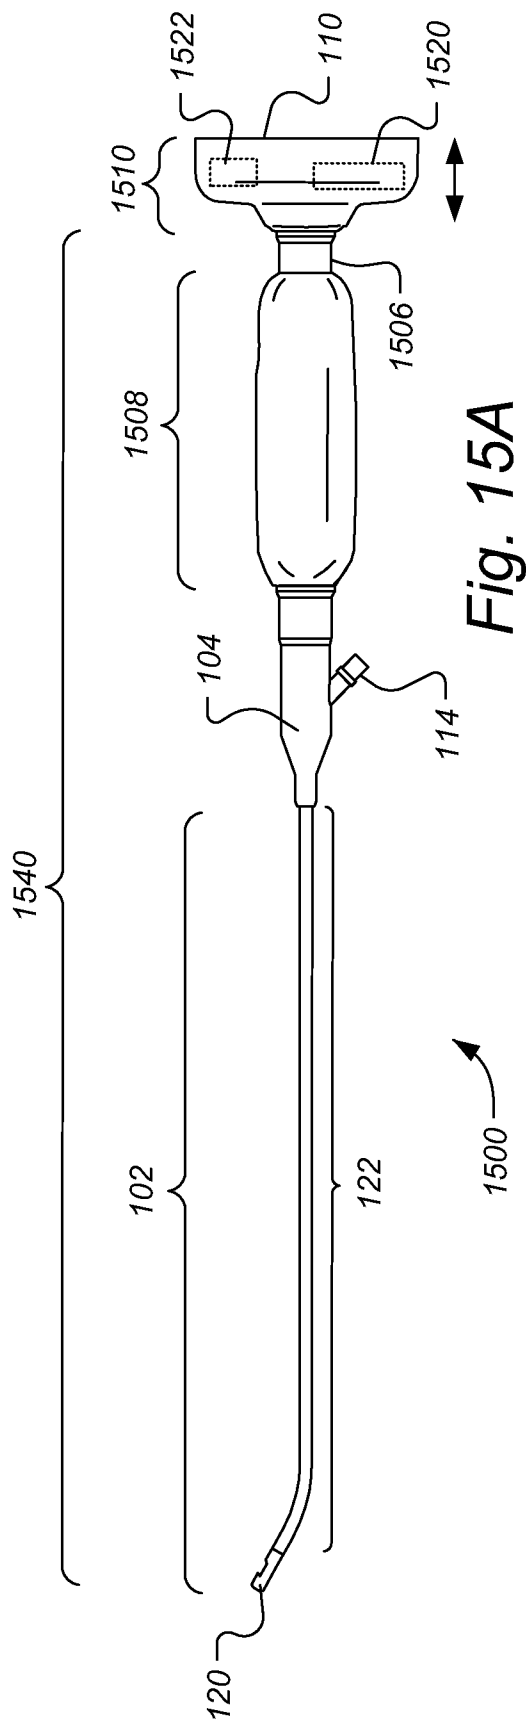


Fig. 14B

15 / 16



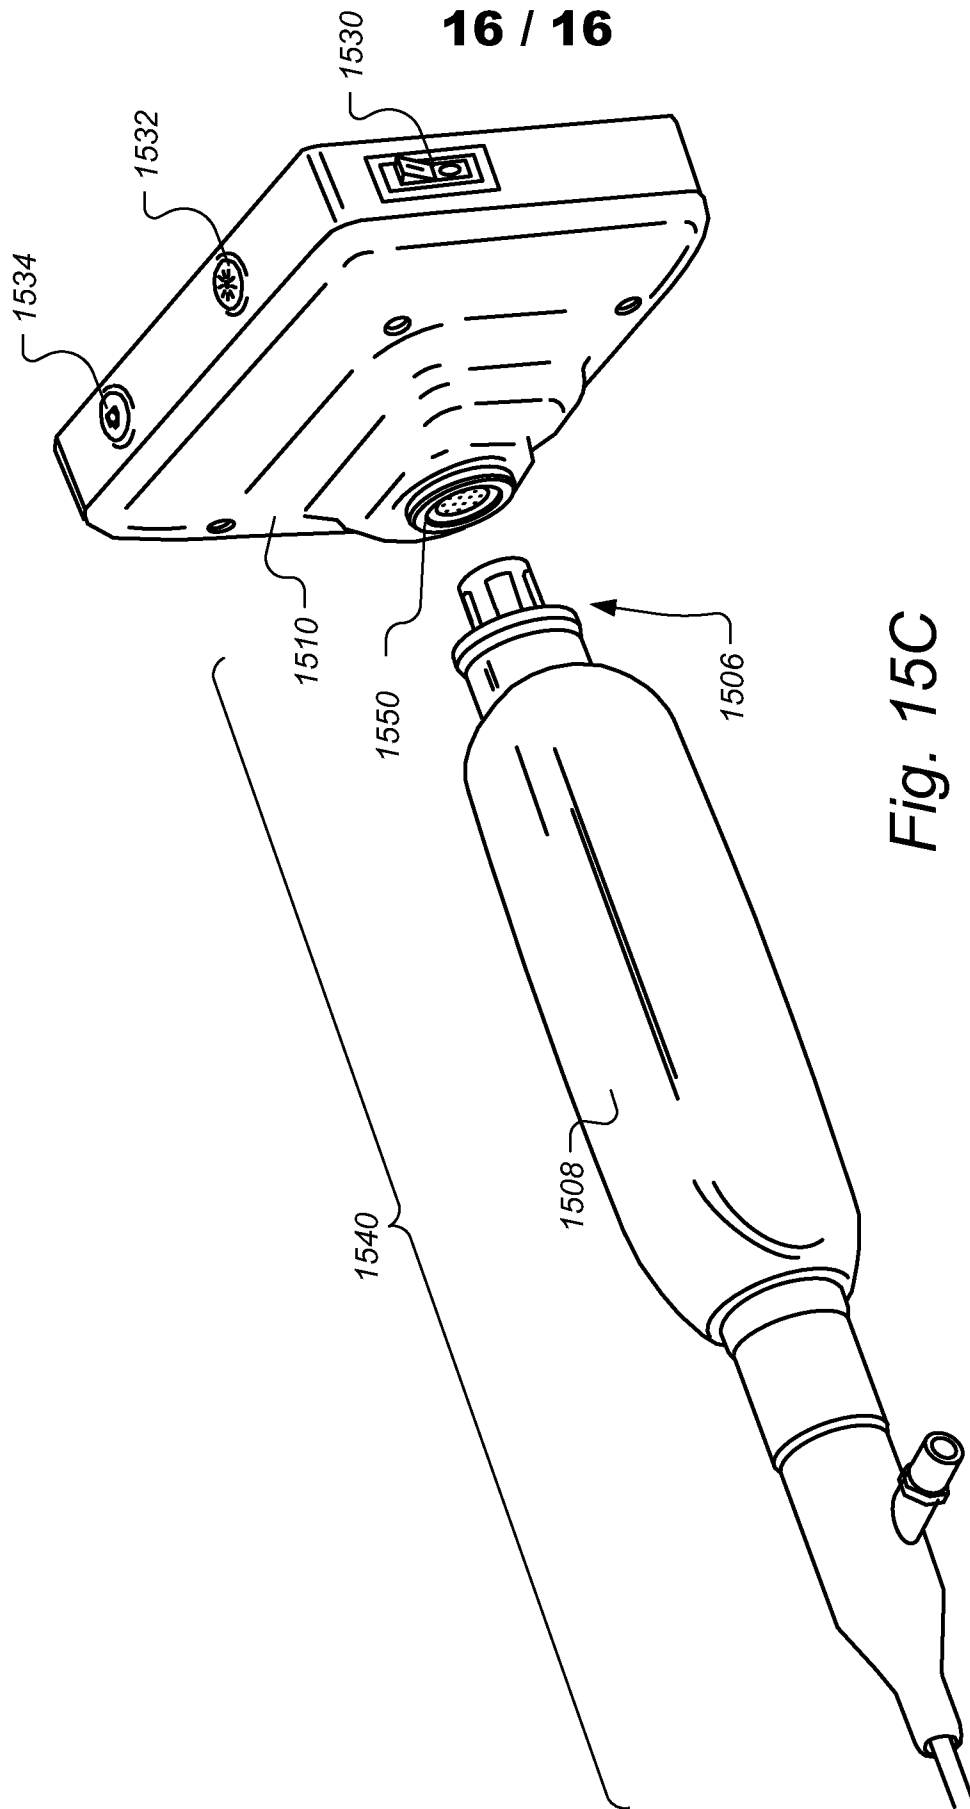


Fig. 15C

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US 13/40992

<p>A. CLASSIFICATION OF SUBJECT MATTER IPC(8) - A61B 1/00 (2013.01) USPC - 600/104, 101 According to International Patent Classification (IPC) or to both national classification and IPC</p>																										
<p>B. FIELDS SEARCHED</p> <p>Minimum documentation searched (classification system followed by classification symbols) IPC(8) - A61B 1/00, 1/015, 1/018, 1/04, 1/06, 1/303; H04N 7/18 (2013.01) USPC: 348/077; 600/101, 103, 104, 131, 136, 156</p> <p>Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched</p> <p>Electronic data base consulted during the international search (name of data base and, where practicable, search terms used) MicroPatent (US-G, US-A, EP-A, EP-B, WO, JP-bib, DE-C.B, DE-A, DE-T, DE-U, GB-A, FR-A); DialogPRO; Google; Google Scholar; Medline/PubMed. conduit, detach, endoscope, fluid, hyster*, illuminate, image, irrigate, probe, separable, separate, tube, tubular, uterus, video</p>																										
<p>C. DOCUMENTS CONSIDERED TO BE RELEVANT</p> <table border="1"> <thead> <tr> <th>Category*</th> <th>Citation of document, with indication, where appropriate, of the relevant passages</th> <th>Relevant to claim No.</th> </tr> </thead> <tbody> <tr> <td>Y</td> <td>US 2008/0058595 A1 (SNOKE, PJ, et al.) March 6, 2008 figures 10, 11, 17; paragraph [0044], [0063], [0091], [0099]-[0105], [0108]-[0111]</td> <td>1-8</td> </tr> <tr> <td>Y</td> <td>WO 201 1/038310 A1 (ZIARNO, WA, et al.) March 31, 2011 figure 30; page 32, lines 23-25; page 33, lines 1-3; page 70, lines 20-27; page 71, lines 1-3</td> <td>1-8</td> </tr> <tr> <td>Y</td> <td>US 2008/0045791 A1 (GAL, E, et al.) February 21, 2008 figure 1; paragraph [0071]-[0078], [0081], [0089]</td> <td>1-8</td> </tr> <tr> <td>Y</td> <td>US 4836189 A (ALFRED, III, JB, et al.) June 6, 1989 column 4, lines 49-57</td> <td>7</td> </tr> <tr> <td>Y</td> <td>US 2010/0191050 A1 (ZWOLINSKI, AM) July 29, 2010 figures 22B, 23B; paragraph [0071].</td> <td>8</td> </tr> <tr> <td>A</td> <td>US 2010/0030020 A1 (SANDERS, GJ, et al.) February 4, 2010 paragraphs [0044]-[0053]</td> <td>1-8</td> </tr> <tr> <td>A</td> <td>US 7033314 B2 (KAMRAVA, MM, et al.) April 25, 2006 columns 4-6</td> <td>1-8</td> </tr> </tbody> </table>			Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.	Y	US 2008/0058595 A1 (SNOKE, PJ, et al.) March 6, 2008 figures 10, 11, 17; paragraph [0044], [0063], [0091], [0099]-[0105], [0108]-[0111]	1-8	Y	WO 201 1/038310 A1 (ZIARNO, WA, et al.) March 31, 2011 figure 30; page 32, lines 23-25; page 33, lines 1-3; page 70, lines 20-27; page 71, lines 1-3	1-8	Y	US 2008/0045791 A1 (GAL, E, et al.) February 21, 2008 figure 1; paragraph [0071]-[0078], [0081], [0089]	1-8	Y	US 4836189 A (ALFRED, III, JB, et al.) June 6, 1989 column 4, lines 49-57	7	Y	US 2010/0191050 A1 (ZWOLINSKI, AM) July 29, 2010 figures 22B, 23B; paragraph [0071].	8	A	US 2010/0030020 A1 (SANDERS, GJ, et al.) February 4, 2010 paragraphs [0044]-[0053]	1-8	A	US 7033314 B2 (KAMRAVA, MM, et al.) April 25, 2006 columns 4-6	1-8
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.																								
Y	US 2008/0058595 A1 (SNOKE, PJ, et al.) March 6, 2008 figures 10, 11, 17; paragraph [0044], [0063], [0091], [0099]-[0105], [0108]-[0111]	1-8																								
Y	WO 201 1/038310 A1 (ZIARNO, WA, et al.) March 31, 2011 figure 30; page 32, lines 23-25; page 33, lines 1-3; page 70, lines 20-27; page 71, lines 1-3	1-8																								
Y	US 2008/0045791 A1 (GAL, E, et al.) February 21, 2008 figure 1; paragraph [0071]-[0078], [0081], [0089]	1-8																								
Y	US 4836189 A (ALFRED, III, JB, et al.) June 6, 1989 column 4, lines 49-57	7																								
Y	US 2010/0191050 A1 (ZWOLINSKI, AM) July 29, 2010 figures 22B, 23B; paragraph [0071].	8																								
A	US 2010/0030020 A1 (SANDERS, GJ, et al.) February 4, 2010 paragraphs [0044]-[0053]	1-8																								
A	US 7033314 B2 (KAMRAVA, MM, et al.) April 25, 2006 columns 4-6	1-8																								
<p><input type="checkbox"/> Further documents are listed in the continuation of Box C. <input type="checkbox"/></p>																										
<p>* Special categories of cited documents:</p> <table border="0"> <tr> <td>"A" document defining the general state of the art which is not considered to be of particular relevance</td> <td>"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention</td> </tr> <tr> <td>"E" earlier application or patent but published on or after the international filing date</td> <td>"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone</td> </tr> <tr> <td>"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)</td> <td>"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art</td> </tr> <tr> <td>"O" document referring to an oral disclosure, use, exhibition or other means</td> <td>"&" document member of the same patent family</td> </tr> <tr> <td>"P" document published prior to the international filing date but later than the priority date claimed</td> <td></td> </tr> </table>			"A" document defining the general state of the art which is not considered to be of particular relevance	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention	"E" earlier application or patent but published on or after the international filing date	"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone	"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art	"O" document referring to an oral disclosure, use, exhibition or other means	"&" document member of the same patent family	"P" document published prior to the international filing date but later than the priority date claimed															
"A" document defining the general state of the art which is not considered to be of particular relevance	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention																									
"E" earlier application or patent but published on or after the international filing date	"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone																									
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art																									
"O" document referring to an oral disclosure, use, exhibition or other means	"&" document member of the same patent family																									
"P" document published prior to the international filing date but later than the priority date claimed																										
<p>Date of the actual completion of the international search 30 September 2013 (30.09.2013)</p>		<p>Date of mailing of the international search report 17 OCT 2013</p>																								
<p>Name and mailing address of the ISA/US Mail Stop PCT, Attn: ISA/US, Commissioner for Patents P.O. Box 1450, Alexandria, Virginia 22313-1450 Facsimile No. 571-273-3201</p>		<p>Authorized officer: Shane Thomas PCT Helpdesk: 571-272-4300 PCT OSP: 571-272-7774</p>																								

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US 13/40992

Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:

2. Claims Nos.:
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:

3. Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

This application contains the following inventions or groups of inventions which are not so linked as to form a single general inventive concept under PCT Rule 13.1.

Group I: Claims 1-8 are directed toward a low-cost medical instrument for examining a patient's uterus.

Group II: Claims 9-16 are directed toward an integrated endoscopic instrument for examining a patient's uterus, with an elongate member being semi-flexible such that when fixedly held at 5 inches from the distal end and a 50 gram mass is applied two inches from the distal end the distal end bends in a downwards direction between 2mm and 60mm.

-***-See extra sheet for details-***-

1. As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. As all searchable claims could be searched without effort justifying additional fees, this Authority did not invite payment of additional fees.
3. As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:

4. No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:
1-8

Remark on Protest

- The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- No protest accompanied the payment of additional search fees.

-***- Continued from Box No. III - Observations where unity of invention is lacking -***-

Group III: Claims 17-21 are directed toward an integrated endoscopic instrument for examining a patient's uterus, with a shaft housing a fluid channel and a plurality of electrical conductors, said conductors configured to carry video and control signals, said shaft having a first outer diameter of less than 5mm and said distal end having a second outer diameter greater than the first outer diameter.

The inventions listed as Groups I-III do not relate to a single general inventive concept under PCT Rule 13.1 because, under PCT Rule 13.2, they lack the same or corresponding special technical features for the following reasons: the special technical features of Group I include a single-use portion configured to in a single insertion distend and image a patient's uterus, the single-use portion including: an elongated conduit having a distal portion configured and dimensioned for insertion into the patient's uterus, and a proximal portion; a fluid connection port formed at the proximal portion of the conduit; one or more distal openings at the distal portion of the conduit configured to provide fluid from the conduit and into the uterus; an electrical cable extending from a proximal end of the conduit to the imaging system and configured to carry video signals and control signals; a multiple-use portion having interior and exterior surfaces, the multiple-use portion being configured to be attached to the single-use portion for a single use and then detached after a single use, and to be re-used with a second single-use portion without sterilization of the interior surfaces; and one or more seals configured to keep fluid in the conduit from contacting any of the interior surfaces of said multiple-use portion, which are not present in Groups II-III; the special technical features of Group II include said elongate member being dimensioned and configured to facilitate insertion of the distal end through a patient's cervix and into the uterus, and said elongate member being semi-flexible such that when fixedly held at 5 inches from the distal end and a 50 gram mass is applied two inches from the distal end the distal end bends in a downwards direction between 2mm and 60mm, which are not present in Groups I and III; the special technical features of Group III include a shaft extending from the distal end to the proximal end, said shaft housing a fluid channel and a plurality of electrical conductors, said conductors configured to carry video and control signals, said shaft having a first outer diameter of less than 5mm and said distal end having a second outer diameter greater than the first outer diameter, which are not present in Groups I-II.

The common technical features of Groups I-III are an elongate member with a proximal end and a distal end; an imaging system; an illumination system; a fluid opening; and an image display with electrical connection.

These common technical features are disclosed by US 7,033,314 B2 to Kamrava, et al. (hereinafter 'Kamrava'). Kamrava discloses an elongate member with a proximal end and a distal end (elongate tubular body having a proximal end and a distal end; claim 1); an imaging system (video camera may be coupled about lumen 36 to provide video images of the uterus; column 4, lines 1-2); an illumination system (illumination within uterus may be provided via illumination train extending through lumen 35 of hysteroscope; column 3, lines 38-40); a fluid opening (microcatheter is used to introduce gas or transfer embryo; column 5, lines 10-21; column 6, lines 1-12); and an image display with electrical connection (system (video camera may be coupled about lumen 36 to provide video images of the uterus; column 4, lines 1-2).

Since the common technical features are previously disclosed by the Kamrava reference, the common features are not special and so Groups I-III lack unity.

专利名称(译)	用于宫腔镜检查 and 组合宫腔镜检查 and 子宫内膜活组织检查的方法和设备		
公开(公告)号	EP2900118A4	公开(公告)日	2016-04-20
申请号	EP2013830519	申请日	2013-05-14
[标]申请(专利权)人(译)	ENDOSEE 股份有限公司		
申请(专利权)人(译)	ENDOSEE CORPORATION		
当前申请(专利权)人(译)	ENDOSEE CORPORATION		
[标]发明人	OUYANG XIAOLONG INDMAN PAUL D DECKMAN ROBERT K WANG SHIH PING		
发明人	OUYANG, XIAOLONG INDMAN, PAUL, D. DECKMAN, ROBERT, K. WANG, SHIH-PING		
IPC分类号	A61B1/00		
CPC分类号	A61B1/303 A61B1/00006 A61B1/00032 A61B1/00034 A61B1/00048 A61B1/00052 A61B1/00057 A61B1/00066 A61B1/00071 A61B1/00078 A61B1/00091 A61B1/00094 A61B1/00103 A61B1/00105 A61B1/00114 A61B1/00124 A61B1/005 A61B1/0055 A61B1/015 A61B1/05 A61B1/06 A61B1/0676 A61B1/0684 A61B1/126 A61B1/307 A61B1/317 A61B10/0291 A61B10/04		
代理机构(译)	康罗伊, JOHN		
优先权	61/692701 2012-08-23 US 61/646887 2012-05-14 US 61/709022 2012-10-02 US 61/709033 2012-10-02 US 61/676444 2012-07-27 US 61/664143 2012-06-25 US 61/818341 2013-05-01 US 61/667341 2012-07-02 US 61/803672 2013-03-20 US 61/813635 2013-04-18 US 61/803664 2013-03-20 US 13/474429 2012-05-17 US 61/672733 2012-07-17 US		
其他公开文献	EP2900118A1		
外部链接	Espacenet		

摘要(译)

描述了用于执行宫腔镜检查和/或组合宫腔镜检查和子宫内膜活组织检查的器械和方法。根据一些实施例，手柄，电子设备和集成显示屏形成器械的可重复使用部分，而包括CMOS成像模块和LED照明的流体鞘和套管形成器械的单次使用部分。套管是半柔性的，使得操作者可以在沿轴的某个中间点（例如距离远端尖端5英寸）处容易地抓住套管，以在使用期间弯曲和/或操纵套管。根据一些实施例，远端尖端具有比轴更大的直径，已经发现在一些应用中使用期间改善了流体管理。

