



(51) International Patent Classification:

A61B 34/32 (2016.01) A61B 34/20 (2016.01)
A61B 34/00 (2016.01) A61B 17/00 (2006.01)

(21) International Application Number:

PCT/US2018/031302

(22) International Filing Date:

07 May 2018 (07.05.2018)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

62/510,938 25 May 2017 (25.05.2017) US

(71) Applicant: **COVIDIEN LP** [US/US]; 15 Hampshire Street, Mansfield, Massachusetts 02048 (US).


(72) Inventors: **CHOWANIEC, Matthew**; 35 Blueberry Hill Drive, Madison, Connecticut 06443 (US). **CHEN, Xingrui**; 36 Meadowrue Drive, Glastonbury, Connecticut 06033 (US).

(74) Agent: **AKYUZ, Ishak** et al.; Medtronic, 60 Middletown Avenue, c/o Legal Mailstop MS 54, North Haven, Connecticut 06473 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JO, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,

(54) Title: ROBOTIC SURGICAL SYSTEM WITH AUTOMATED GUIDANCE

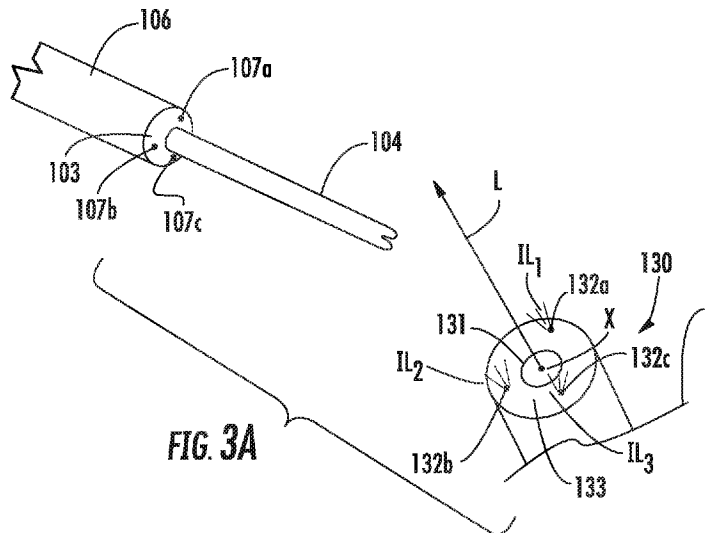

(57) Abstract: A robotic surgical system includes at least one robot arm, at least one instrument, and a plurality of drive motors configured to drive the at least one robot arm and at least one instrument. The system also includes a laparoscopic port having a plurality of fiducials, a sensor configured to detect the plurality of fiducials, and a controller configured to control the plurality of drive motors. The controller includes a processor that determines a current distance between each fiducial among the plurality of fiducials, determines a location of the laparoscopic port based on the distance between each fiducial, determines a position of the at least one robot arm and the at least one instrument relative to the location of the laparoscopic port, and controls the plurality of drive motors to align the at least one robot arm or the at least one instrument with the laparoscopic port.



TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,
KM, ML, MR, NE, SN, TD, TG).

Published:

— *with international search report (Art. 21(3))*

ROBOTIC SURGICAL SYSTEM WITH AUTOMATED GUIDANCE

BACKGROUND

[1] Robotic surgical systems such as teleoperative systems are used to perform minimally invasive surgical procedures that offer many benefits over traditional open surgery techniques, including less pain, shorter hospital stays, quicker return to normal activities, minimal scarring, reduced recovery time, and less injury to tissue.

[2] Robotic surgical systems can have a number of robotic arms that move attached instruments or tools, such as an image capturing device, a stapler, an electrosurgical instrument, etc., in response to movement of input devices by a surgeon viewing images captured by the image capturing device of a surgical site. During a surgical procedure, each of the tools may be inserted through an opening, e.g., a laparoscopic port, into the patient and positioned to manipulate tissue at a surgical site. The openings are placed about the patient's body so that the surgical instruments may be used to cooperatively perform the surgical procedure and the image capturing device may view the surgical site.

[3] During the surgical procedure, the tools are manipulated in multiple degrees of freedom by a clinician. In order to manipulate the tool through the laparoscopic port, the clinician has to position the robotic arm correctly to facilitate insertion and/or removal of the tool. However, obtaining the correct position may be a relatively time consuming step. Further, manual positioning of the robotic arm by the clinician adds further time and complexity to this step of the surgical procedure.

[4] Accordingly, there is a need for guiding the robotic arms of the robotic surgical system to reduce the complexity and duration of a surgical procedure, as well as increase the outcome and/or results of the surgical procedure.

SUMMARY

[5] The present disclosure relates generally to guiding of a robotic surgical system and, in particular, guiding a robotic arm of the robotic surgical system to automatically insert and/or remove tools through an opening or laparoscopic port.

[6] In an aspect of the present disclosure, a robotic surgical system is provided. The system includes at least one robot arm, at least one instrument coupled to the robot arm, and a plurality of drive motors configured to drive the at least one robot arm and at least one instrument. The system also includes a laparoscopic port having a plurality of fiducials and a sensor configured to detect the plurality of fiducials. A controller that is configured to control the plurality of drive motors includes a processor configured to determine a current distance between each fiducial among the plurality of fiducials, determine a location of the laparoscopic port based on the distance between each fiducial, determine a position of the at least one robot arm and the at least one instrument relative to the location of the laparoscopic port, and control the plurality of drive motors to align the at least one robot arm or the at least one instrument with the laparoscopic port.

[7] In embodiments, the processor is also configured to obtain a predetermined distance between each fiducial among the plurality of fiducials and obtain a predetermined distance between each fiducial and the laparoscopic port. The processor may determine the location of the laparoscopic port based on the current distance between each fiducial among the plurality of

fiducials, the predetermined distance between each fiducial among the plurality of fiducials, and the predetermined distance between each fiducial and the laparoscopic port.

[8] In embodiments, the processor is configured to obtains a length of the at least one instrument and a length of the at least one robot arm. Control of the plurality of drive motors may be based on the position of the at least one robot arm and the at least one instrument relative to the location of the laparoscopic port, the length of the at least one instrument, and the length of the at least one robot arm.

[9] In some embodiments, the plurality of fiducials is active light emitting diodes.

[10] In some embodiments, the robotic surgical system includes a light source configured to emit light directed at the plurality of fiducials. The plurality of fiducials may include a reflective material and the light emitted from the light source may be reflected by the plurality of fiducials and detected by the sensor.

[11] In another aspect of the present disclosure, a method for guiding a robot arm and/or instrument toward a laparoscopic port is provided. The method includes determining a current distance between each fiducial among a plurality of fiducials disposed around the laparoscopic port and determining a location of the laparoscopic port based on the distance between each fiducial. The method also includes determining a position of the robot arm and the instrument relative to the location of the laparoscopic port and controlling a plurality of drive motors associated with the robot arm and the instrument to align the robot arm or the instrument with the laparoscopic port.

[12] In embodiments, the method includes obtaining a predetermined distance between each fiducial among the plurality of fiducials and obtaining a predetermined distance between each fiducial and the laparoscopic port. The method also includes determining the location of the laparoscopic port based on the current distance between each fiducial among the plurality of fiducials, the predetermined distance between each fiducial among the plurality of fiducials, and the predetermined distance between each fiducial and the laparoscopic port.

[13] In embodiments, the method includes obtaining a length of the instrument and obtaining a length of the robot arm. Controlling the plurality of drive motors is based on the position of the robot arm and the instrument relative to the location of the laparoscopic port, the length of the instrument, and the length of the robot arm.

BRIEF DESCRIPTION OF THE DRAWINGS

[14] Various aspects of the present disclosure are described hereinbelow with reference to the drawings, which are incorporated in and constitute a part of this specification, wherein:

[15] Fig. 1 is a schematic illustration of a user interface and a robotic system of a robotic surgical system in accordance with the present disclosure;

[16] Fig. 2A is a top view of a laparoscopic port in accordance with the present disclosure;

[17] Fig. 2B is a perspective view of a portion of robotic arm of the robot system of Fig. 1 with a surgical instrument attached to the robotic arm;

[18] Fig. 3A is a perspective view of an exemplary outside-looking-in optical system in accordance with the present disclosure;

[19] Fig. 3B is a perspective view of an exemplary inside-looking-out optical system in accordance with the present disclosure;

[20] Fig. 3C is a perspective view of an exemplary optical system in accordance with the present disclosure including sensors disposed about an operating theater; and

[21] Fig. 4 is a flowchart depicting operation of an automated guidance system of the present disclosure including an optical system of Fig. 3A, 3B, or 3C.

DETAILED DESCRIPTION

[22] The present disclosure is directed to systems and methods for guiding one or more robotic arms in a robotic surgical system utilizing images captured during a surgical procedure. Image data captured during a surgical procedure may be analyzed to guide a robotic arm having a device or tool coupled thereto to insert and/or remove the tool from a laparoscopic port. In the systems described herein, one or more laparoscopic ports have three (3) fiducials, e.g., active infrared light emitting diodes (LEDs), with known distances between the fiducials and known distances between the fiducials and a center of the laparoscopic port. The positions of each fiducial may be analyzed using motion analyzing techniques to establish a plane defined by the fiducials and establish the steps necessary to move the robot arm in position. The position of the center of the laparoscopic port relative to the three (3) fiducials determines where to insert and/or remove the tool, and an orientation angle for the tool.

[23] In the systems described herein, aligning and orienting the robotic arm to insert and/or remove the tool through the laparoscopic port relies on one or more variables. The variable(s) may include, but is/are not limited to, distance(s) between three (3) or more fiducials,

distance(s) between the fiducials and the center of the laparoscopic port, the port plane defined by the fiducials, and/or the length of the interchangeable tool and robotic arm.

[24] The systems described herein permit quicker installation of robotic instrumentation into laparoscopic ports, less intervention on the part of a clinician during a surgical procedure, and/or potentially lower incidents of impact with a laparoscopic port site.

[25] Turning to Fig. 1, a robotic surgical system 100 may be employed with one or more consoles 102 that are next to the operating theater or located in a remote location. In this instance, one team of clinicians or nurses may prep the patient for surgery and configure the robotic surgical system 100 with one or more tools 104 while another clinician (or group of clinicians) remotely controls the instruments via the robotic surgical system. As can be appreciated, a highly skilled clinician may perform multiple operations in multiple locations without leaving his/her remote console which can be both economically advantageous and a benefit to the patient or a series of patients.

[26] The robotic arms 106 of the surgical system 100 are typically coupled to a pair of master handles 108 by a controller 110. Controller 110 may be integrated with the console 102 or provided as a standalone device within the operating theater. The handles 106 can be moved by the clinician to produce a corresponding movement of the working ends of any type of tools 104 (e.g., probes, mechanical or electrosurgical end effectors, graspers, knives, scissors, etc.) attached to the robotic arms 106. For example, tool 104 may be a probe that includes an image capture device.

[27] The console 102 includes a display device 112 which is configured to display two-dimensional or three-dimensional images. The display device 112 displays the images of the

surgical site which may include data captured by tool 104 positioned on the ends 114 of the arms 106 and/or include data captured by imaging devices that are positioned about the surgical theater (e.g., an imaging device positioned within the surgical site, an imaging device positioned adjacent the patient, imaging device positioned at a distal end of an imaging arm). The imaging devices may capture visual images, infra-red images, ultrasound images, X-ray images, thermal images, and/or any other known real-time images of the surgical site. The imaging devices transmit captured imaging data to the controller 110 which creates the images of the surgical site in real-time from the imaging data and transmits the images to the display device 112 for display.

[28] The movement of the master handles 108 may be scaled so that the working ends have a corresponding movement that is different, smaller or larger, than the movement performed by the operating hands of the clinician. The scale factor or gearing ratio may be adjustable so that the operator can control the resolution of the working ends of the surgical instrument(s) 104.

[29] During operation of the surgical system 100, the master handles 108 are operated by a clinician to produce a corresponding movement of the robotic arms 106 and/or surgical instruments 104. The master handles 108 provide a signal to the controller 110 which then provides a corresponding signal to one or more drive motors 114. The one or more drive motors 114 are coupled to the robotic arms 106 in order to move the robotic arms 106 and/or surgical instruments 104.

[30] The master handles 108 may include various haptics 116 to provide feedback to the clinician relating to various tissue parameters or conditions, e.g., tissue resistance due to manipulation, cutting or otherwise treating, pressure by the instrument onto the tissue, tissue temperature, tissue impedance, etc. As can be appreciated, such haptics 116 provide the clinician

with enhanced tactile feedback simulating actual operating conditions. The haptics 116 may include vibratory motors, electroactive polymers, piezoelectric devices, electrostatic devices, subsonic audio wave surface actuation devices, reverse-electrovibration, or any other device capable of providing a tactile feedback to a user. The master handles 108 may also include a variety of different actuators (not shown) for delicate tissue manipulation or treatment further enhancing the clinician's ability to mimic actual operating conditions.

[31] The controller 110 includes a transceiver 118 and a processor 120. Transceiver 118 receives a signal from infrared sensors 122 which will be described in more detail below. The signal from infrared sensors may be transmitted to transceiver 118 via any conventional wired or wireless methods. Transceiver 118 provides the signal to a motion analysis unit 124 in processor 120 which performs a motion analysis on the signal in order to control the one or more drive motors 114 to move the robotic arms 106 and/or surgical instruments 104 into the correct position and/or orientation. A memory 126 may store an algorithm used to perform the motion analysis. In some embodiments, memory 126 may store a look up table (LUT) that includes information pertaining to instruments 104, robot arms 106, and laparoscopic ports discussed below.

[32] As will be discussed in more detail below, infrared sensors receive light from infrared light sources. The infrared sensors may be disposed on the robotic arm 106, the surgical instrument 104, the laparoscopic port 130, or may be disposed anywhere in the surgical environment. The infrared light sources may be incorporated in the robotic arm 106, the surgical instrument 104, the laparoscopic port 130, or may be disposed anywhere in the surgical environment.

[33] With reference to Fig. 2A, the laparoscopic port 130 has at least three (3) port fiducials 132a-c positioned in a port plane about a port opening 131 of the laparoscopic port 130. The port plane may be defined by an outer surface 133 (Fig. 3A) of the laparoscopic port 130. The port fiducials 132a-c are positioned about the port opening 131 with distances D_{1-3} between the port fiducials 132a-c and distances P_{1-3} between the port fiducials 132a-c and a center "X" of the port opening 131 being known.

[34] Referring to Fig. 2B, the robotic arm 106 has at least three (3) arm fiducials 107a-c positioned in an arm plane orthogonal to a longitudinal axis of the robotic arm 106. The arm plane may be defined by a distal surface 103 of the robotic arm 106. Similar to the port fiducials 132a-c, distances between the arm fiducials 107a-c and distances between each of the arm fiducials 107a-c and the longitudinal axis of the robotic arm 106 are known.

[35] Turning to Fig. 3A, an outside-looking-in optical system is shown according to an embodiment of the present disclosure including the robotic arm 106 and the laparoscopic port 130. In such an embodiment, the port fiducials 132a-c of laparoscopic port 130 are infrared light sources (e.g., active infrared light emitting diodes (LEDs)) which each emit infrared light IL_{1-3} having a distinctive characteristic (e.g., wavelength, phase) and the arm fiducials 107a-c are infrared sensors (e.g., infrared cameras) in communication with the transceiver 118 (FIG. 1). The arm fiducials 107a-c determine the time it takes for infrared light (e.g., IL_{1-3}) from the port fiducials 132a-c to reach the respective arm fiducial 107a-c and provides a signal indicative of the time to motion analysis unit 124.

[36] Referring to Fig. 3B, an inside-looking-out optical system is shown according to an embodiment of the present disclosure including the robotic arm 106 and the laparoscopic port 130.

The at least three (3) arm fiducials 107a-c are infrared light sources (e.g., active infrared light emitting diodes (LEDs)) which each emit infrared light EL_{1-3} having a distinctive characteristic (e.g., wavelength, phase) and the at least three (3) of laparoscopic port 130 are infrared sensors (e.g., infrared cameras) in communication with the transceiver 118 (FIG. 1). The port fiducials 132a-c determine the time it takes for the infrared light (e.g., EL_{1-3}) from the arm fiducials 107a-c to reach the respective port fiducial 132a-c and provides a signal indicative of the motion analysis unit 124.

[37] Referring to Fig. 3C, a fixed optical system is shown according to an embodiment of the present disclosure including the robotic arm 106 and the laparoscopic port 130. In such an embodiment, at least three (3) infrared sensors 192a-c (e.g., infrared cameras) are positioned about the operating theater and are in communication with the transceiver 118 (FIG. 1). The port fiducials 132a-c of laparoscopic port 130 are infrared light sources (e.g., active infrared light emitting diodes (LEDs)) which each emit infrared light IL_{1-3} having a distinctive characteristic (e.g., wavelength, phase) and the arm fiducials 107a-c and the arm fiducials 107a-c are infrared light sources (e.g., active infrared light emitting diodes (LEDs)) which each emit infrared light EL_{1-3} having a distinctive characteristic (e.g., wavelength, phase). The positions of the infrared sensors 192a-c within the operating theater are known such that the position of the arm and port fiducials 107a-c, 132a-c relative to the infrared sensors 192a-c can be determined as detailed below. The infrared sensors 192a-c determine the time it takes for infrared light (e.g., IL_{1-3} or EL_{1-3}) from the arm fiducials 107a-c and the port fiducials 132a-c to reach the respective infrared sensor 192a-c and provides a signal indicative of the time to motion analysis unit 124.

[38] As detailed below with reference to FIG. 4, the motion analysis unit 124 (FIG. 1) determines the position of the robotic arm 106 relative to the laparoscopic port 130 based on signals

from the fiducials 107a-c, 132a-c. Fig. 4 will be described while making references to Figs. 1-3A. As shown in Fig. 4, a user enters a laparoscopic port identification number in step s202. Based on the laparoscopic port identification number, the motion analysis unit queries the memory 126 in step s204 to obtain the distances between port fiducials 132a-c (D_1 , D_2 , and D_3 as shown in Fig. 2A) and the distances between each port fiducial 132a-c and the port center "X" of the port opening 131 (P_1 , P_2 , and P_3 as shown in Fig. 2A) that correspond to the laparoscopic port 130. In step s206, an instrument identification number is obtained. The instrument identification number of an instrument 104 coupled to the robotic arm 106 may be obtained via a user input or it may be obtained from an integrated circuit (IC) included in the instrument 104. In step s208, the length of the instrument 104 is obtained based on the instrument identification number, either from the memory 124 or the IC included in the instrument 104. In step s210, a robot arm identification number is obtained. The robot arm identification number may be obtained via a user input or it may be obtained from an IC included in the robot arm 106. In step s212, the geometry of the robot arm 106 is obtained based on the robot arm identification number, either from memory 124 or the IC included in the robot arm 106.

[39] In step s214, the motion analysis unit 124 receives signals from the arm fiducials 107a-c representing the time that the respective infrared light (e.g., IL_{1-3}) from a respective one of the port fiducials 132a-c reached a respective arm fiducial 107a-c. Based on the signals from the arm fiducials 107a-c, the motion analysis unit 124 uses three-dimensional spherical trilateration to determine the distance between each of the port fiducials 132a-c and each of the arm fiducials 107a-c in step s216.

[40] For a detailed discussion of three-dimensional spherical trilateration used to determine the location of points in three dimensions, reference can be made to MURPHY JR.,

WILLIAM S. & HEREMAN, WILLY, DETERMINATION OF A POSITION IN THREE DIMENSIONS USING TRILATERATION AND APPROXIMATE DISTANCES, November 28, 1999, available at <http://inside.mines.edu/~whereman/papers/Murphy-Hereman-Trilateration-1995.pdf>, the entire contents of which are hereby incorporated by reference.

[41] In step s218, the distances between each of the port fiducials 132a-c relative to each of the arm fiducials 107a-c, the port plane defined by the port fiducials 132a-c is determined relative to the arm fiducials 107a-c.

[42] It will be appreciated that the at least three port fiducials (e.g., port fiducials 132a-c) are required to define the port plane relative to the arm fiducials 107a-c which can be determined as follows:

1. Solving for the vector from 132a, 132b and the vector from 132a, 132c as follows:

$$\overrightarrow{AB} = (x_B - x_A) \hat{i} + (y_B - y_A) \hat{j} + (z_B - z_A) \hat{k}$$

$$\overrightarrow{AC} = (x_C - x_A) \hat{i} + (y_C - y_A) \hat{j} + (z_C - z_A) \hat{k}$$

2. Determining the normal vector as follows:

$$\overrightarrow{AB} \times \overrightarrow{AC} = \begin{bmatrix} \hat{i} & \hat{j} & \hat{k} \\ (x_B - x_A) & (y_B - y_A) & (z_B - z_A) \\ (x_C - x_A) & (y_C - y_A) & (z_C - z_A) \end{bmatrix}$$

3. Determine the equation of the plane from the normal vector as follows:

$$((x_B - x_A) + (x_C - x_A))x + ((y_B - y_A) + (y_C - y_A))y + ((z_B - z_A) + (z_C - z_A))z + d = 0$$

4. Use any known point on the plane to solve for d .

[43] As detailed above, the arm fiducials 107a-c are sensors and the port fiducials 132a-c are light sources. Alternatively, the arm fiducials 107a-c can be light sources and the port fiducials 132a-c can be sensors in communication with the motion analysis unit 124. In addition, as detailed above, the arm and port fiducials 107a-c, 132a-c can be light sources and the sensors 192a-c can be sensors in communication with the motion analysis unit 124.

[44] In addition, during step s218, the motion analysis unit 124 determines the port center “X” on the port plane from the position of the three arm fiducials 107a-c. To determine the port center “X”, the motion analysis unit 124 solves the following system of equations:

$$\begin{aligned}(X_x-X_A)^2+(Y_x-Y_A)^2+(Z_x-Z_A)^2&=R_A^2 \\(X_x-X_B)^2+(Y_x-Y_B)^2+(Z_x-Z_B)^2&=R_B^2 \\(X_x-X_C)^2+(Y_x-Y_C)^2+(Z_x-Z_C)^2&=R_C^2\end{aligned}$$

where R_{A-C} are the distances each port fiduciary 132a-c is from a given one of the arm fiduciaries 107a-c.

[45] In step s220, from the position of the port fiducials 132a-c and the port center “X”, a vector “V” normal to the port plane defined by the port fiducials 132a-c and passing through the port center “X” provides the orientation of the port opening 131 relative to the arm fiducials 107a-c.

[46] In step s222, the motion analysis unit 124 determines the current position of the robot arm 106 and the instrument 104 relative to the laparoscopic port 130. To determine the current position of the instrument 104, the motion analysis unit 124 can use inverse kinematics based on the known geometry of links of the robot arm 106, the instrument 104, and measured angles between the links of the robot arm 106.

[47] In step s224, the length of the instrument 104 obtained in step s208, the geometry of the robot arm 106 obtained in steps s212, the location of the laparoscopic port 130 determined in step s220, and the current position of the robot arm 106 (e.g., angles between links) and the instrument 104 determined in step s222 are used to determine how to control the drive motors 114 in order to align the instrument 104 with the vector “V” so that the robot arm 106 and/or instrument 104 may be inserted and/or removed from the laparoscopic port 130. It will be appreciated that by determining the vector “V” relative to the arm fiducials 107a-c the movement of the robot arm 106, and thus instrument 104, are relative to the port fiducials 132a-c. In step s226, the drive motors 114 are controlled to perform insertion and/or removal of the instrument 104.

[48] The embodiments disclosed herein are examples of the disclosure and may be embodied in various forms. Specific structural and functional details disclosed herein are not to be interpreted as limiting, but as a basis for the claims and as a representative basis for teaching one skilled in the art to variously employ the present disclosure in virtually any appropriately detailed structure. Like reference numerals may refer to similar or identical elements throughout the description of the figures.

[49] The phrases “in an embodiment,” “in embodiments,” “in some embodiments,” or “in other embodiments,” which may each refer to one or more of the same or different embodiments in accordance with the present disclosure. A phrase in the form “A or B” means “(A), (B), or (A and B)”. A phrase in the form “at least one of A, B, or C” means “(A), (B), (C), (A and B), (A and C), (B and C), or (A, B and C)”. A clinician may refer to a surgeon or any medical professional, such as a doctor, nurse, technician, medical assistant, or the like performing a medical procedure.

[50] The systems described herein may also utilize one or more controllers to receive various information and transform the received information to generate an output. The controller may include any type of computing device, computational circuit, or any type of processor or processing circuit capable of executing a series of instructions that are stored in a memory. The controller may include multiple processors and/or multicore central processing units (CPUs) and may include any type of processor, such as a microprocessor, digital signal processor, microcontroller, or the like. The controller may also include a memory to store data and/or algorithms to perform a series of instructions.

[51] The systems described herein utilize optical or visual motion tracking technology; however, it is envisioned that other motion tracking technologies can be used in place of or in conjunction with the optical motion tracking technologies detailed above including, but not limited to, accelerometer, gyroscopic, ultrasound, magnetic, radio frequency, or other light based (e.g., laser) motion tracking technologies.

[52] Any of the herein described methods, programs, algorithms, or codes may be converted to, or expressed in, a programming language or computer program. A “Programming Language” and “Computer Program” includes any language used to specify instructions to a computer, and includes (but is not limited to) these languages and their derivatives: Assembler, Basic, Batch files, BCPL, C, C+, C++, Delphi, Fortran, Java, JavaScript, Machine code, operating system command languages, Pascal, Perl, PL1, scripting languages, Visual Basic, metalanguages which themselves specify programs, and all first, second, third, fourth, and fifth generation computer languages. Also included are database and other data schemas, and any other meta-languages. No distinction is made between languages which are interpreted, compiled, or use both compiled and interpreted approaches. No distinction is also made between compiled and source

versions of a program. Thus, reference to a program, where the programming language could exist in more than one state (such as source, compiled, object, or linked) is a reference to any and all such states. Reference to a program may encompass the actual instructions and/or the intent of those instructions.

[53] Any of the herein described methods, programs, algorithms or codes may be contained on one or more machine-readable media or memory. The term “memory” may include a mechanism that provides (e.g., stores and/or transmits) information in a form readable by a machine such a processor, computer, or a digital processing device. For example, a memory may include a read only memory (ROM), random access memory (RAM), magnetic disk storage media, optical storage media, flash memory devices, or any other volatile or non-volatile memory storage device. Code or instructions contained thereon can be represented by carrier wave signals, infrared signals, digital signals, and by other like signals.

[54] It should be understood that the foregoing description is only illustrative of the present disclosure. Various alternatives and modifications can be devised by those skilled in the art without departing from the disclosure. For instance, any of the augmented images described herein can be combined into a single augmented image to be displayed to a clinician. Accordingly, the present disclosure is intended to embrace all such alternatives, modifications and variances. The embodiments described with reference to the attached drawing figures are presented only to demonstrate certain examples of the disclosure. Other elements, steps, methods, and techniques that are insubstantially different from those described above and/or in the appended claims are also intended to be within the scope of the disclosure.

WHAT IS CLAIMED IS:

1. A robotic surgical system comprising:
 - at least one robot arm;
 - at least one instrument coupled to the robot arm;
 - a plurality of drive motors configured to drive the at least one robot arm;
 - a laparoscopic port;
 - a plurality of fiducials;
 - a plurality of sensors configured to detect the plurality of fiducials; and
 - a controller configured to control the plurality of drive motors, the controller including a processor configured to:
 - determine a current distance between each sensor of the plurality of sensors and each fiducial of the plurality of fiducials;
 - determine a port plane based on the distance between the each sensor and each fiducial;
 - determine a vector normal to the port plane passing through a center of the laparoscopic port based on the distance between each sensor and each fiducial;
 - determine a position of the at least one robot arm and the at least one instrument relative to the vector; and
 - control the plurality of drive motors to align the at least one robot arm or the at least one instrument with the vector.
2. The robotic surgical system of claim 1, wherein the processor is also configured to:
 - obtain a predetermined distance between each fiducial among the plurality of fiducials; and

obtain a predetermined distance between each fiducial and the center of the laparoscopic port.

3. The robotic surgical system of claim 2, wherein the processor determines the port plane based on the current distance between each fiducial among the plurality of fiducials, the predetermined distance between each fiducial among the plurality of fiducials, and the predetermined distance between each fiducial and the center of the laparoscopic port.

4. The robotic surgical system of claim 3, wherein the processor is configured to obtain a length of the at least one instrument.

5. The robotic surgical system of claim 4, wherein the processor is configured to obtain a geometry of the at least one robot arm.

6. The robotic surgical system of claim 5, wherein controlling the plurality of drive motors is based on the position of the at least one robot arm and the at least one instrument relative to the vector, the length of the at least one instrument, and the geometry of the at least one robot arm.

7. The robotic surgical system of claim 1, wherein the plurality of fiducials are active light emitting diodes.

8. The robotic surgical system of claim 1, wherein the plurality of sensors are disposed on the robot arm.

9. The robotic surgical system of claim 1, wherein the plurality of fiducials are disposed on the laparoscopic port.
10. The robotic surgical system of claim 1, wherein the plurality of fiducials are disposed on the robot arm.
11. The robotic surgical system of claim 1, wherein the plurality of sensors are disposed on the laparoscopic port.
12. The robotic surgical system of claim 1, wherein the plurality of drive motors are configured to drive the at least one instrument.
13. A method for guiding a robot arm and/or instrument toward a laparoscopic port, the method comprising:
- determining a position of each fiducial among a plurality of fiducials disposed around the laparoscopic port;
 - determining a port plane of the laparoscopic port based on the position of each fiducial;
 - determining a vector normal to the port plane passing through a center of the laparoscopic port based on the position of each fiducial;
 - determining a position of the robot arm and the instrument relative to the vector; and
 - controlling a plurality of drive motors associated with the robot arm and the instrument to align the robot arm or the instrument with the vector.
14. The method of claim 13, further comprising:

obtaining a predetermined distance between each fiducial among the plurality of fiducials;
and
obtaining a predetermined distance between each fiducial and the center of the laparoscopic port.

15. The method of claim 14, further comprising determining the vector based on the position of each fiducial among the plurality of fiducials, the predetermined distance between each fiducial among the plurality of fiducials, and the predetermined distance between each fiducial and center of the laparoscopic port.

16. The method of claim 15, further comprising obtaining a length of the instrument.

17. The method of claim 16, further comprising obtaining a length of the robot arm.

18. The method of claim 17, wherein controlling the plurality of drive motors is based on the position of the robot arm and the instrument relative to the vector, the length of the instrument, and the length of the robot arm.

19. The method of claim 13, wherein determining the position of each fiducial among a plurality of fiducials includes determining a distance between each sensor of a plurality of sensors and each fiducial of the plurality of fiducials.

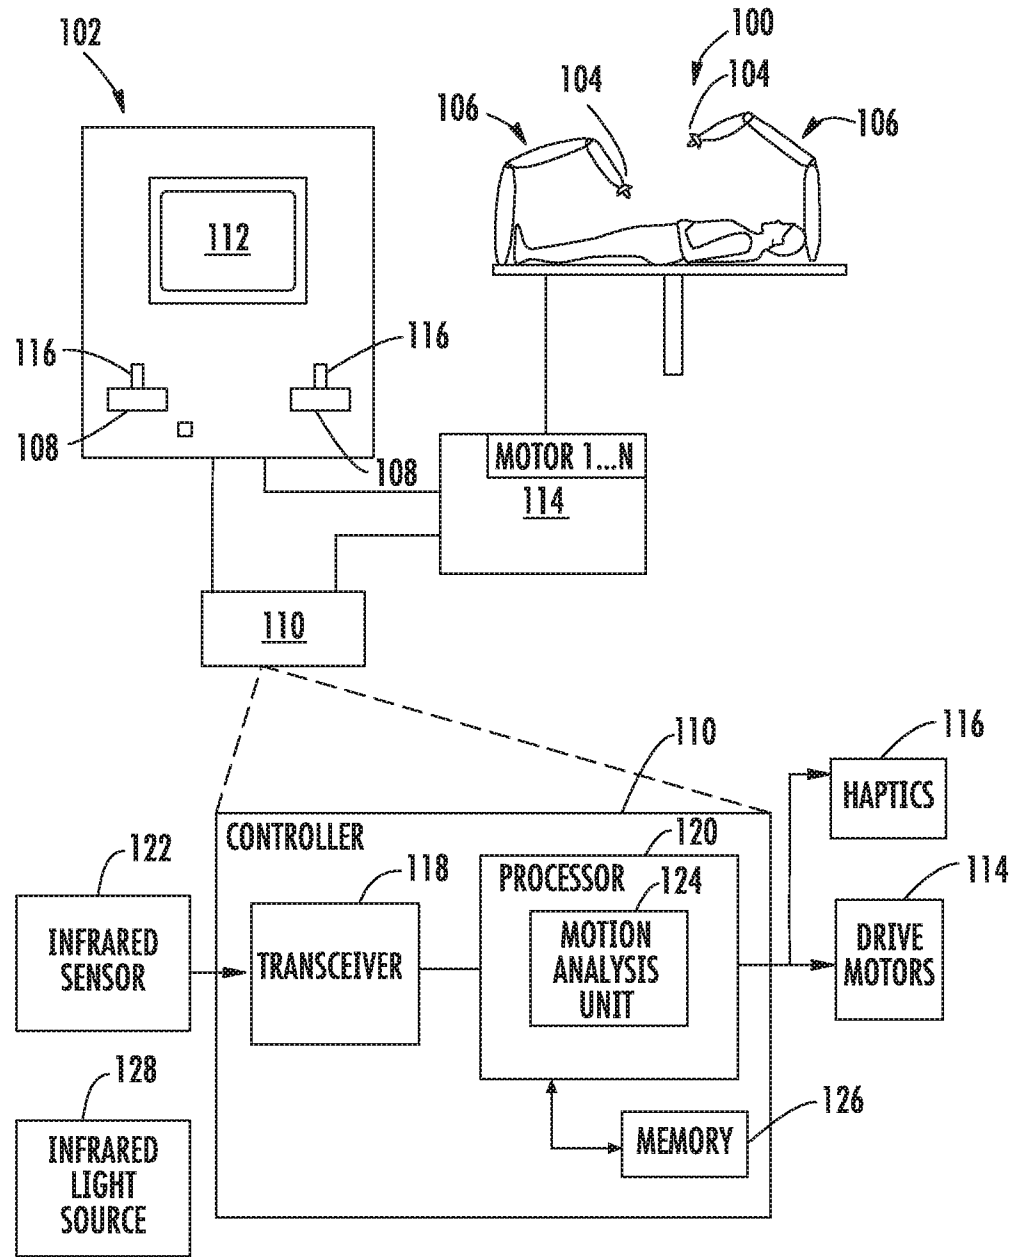


FIG. 1

2/5

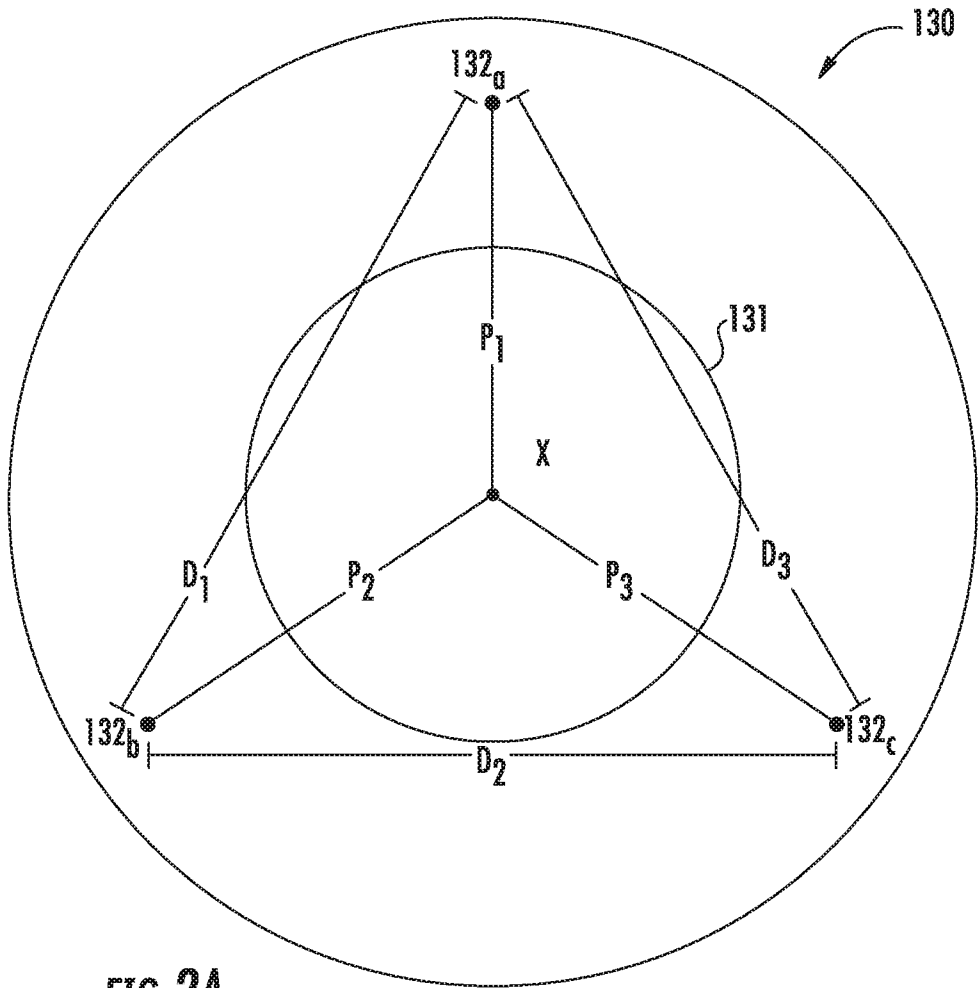


FIG. 2A

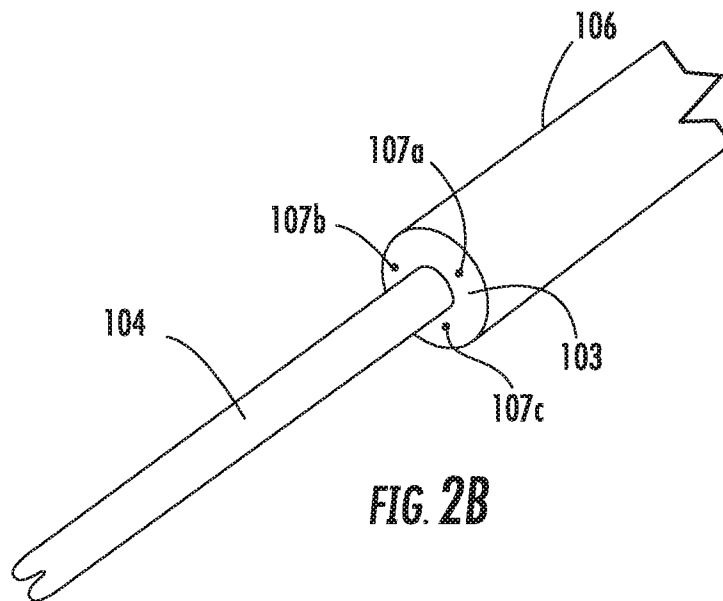
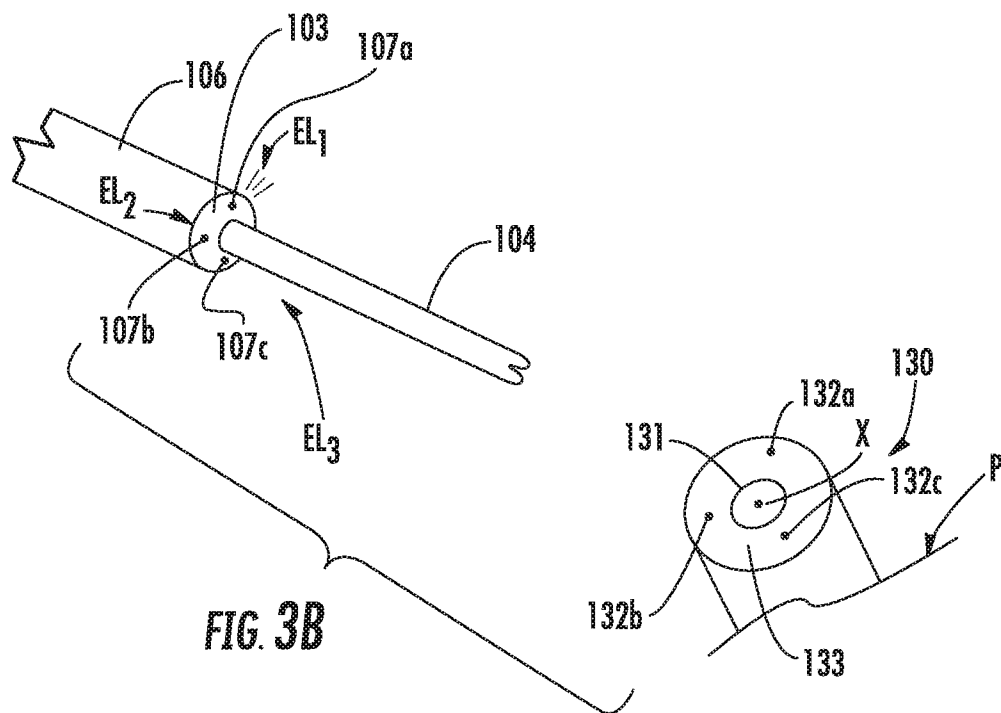
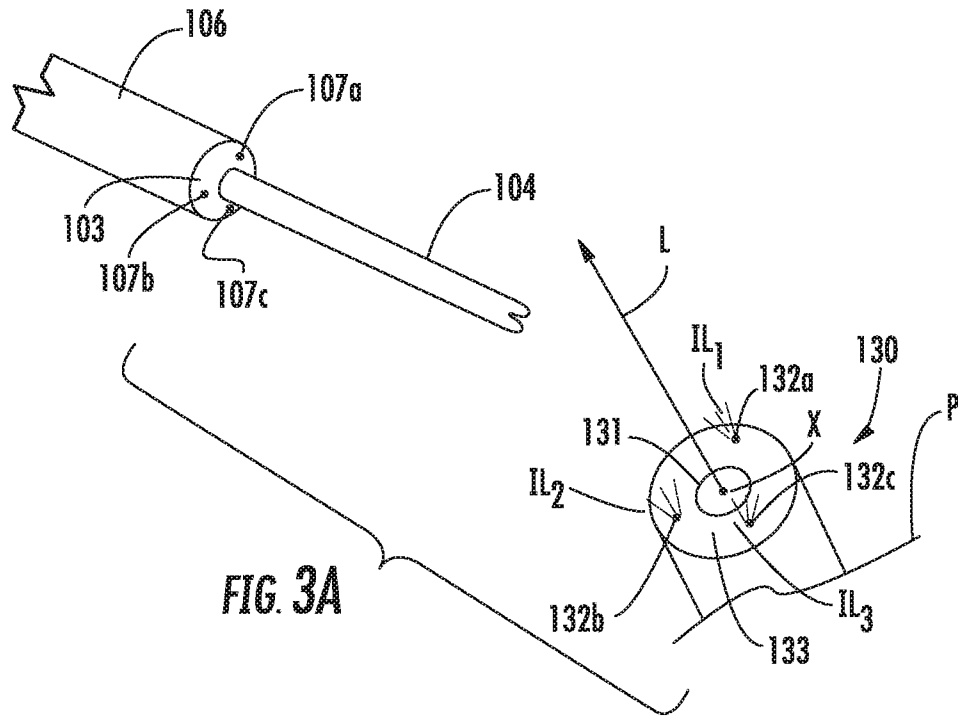


FIG. 2B



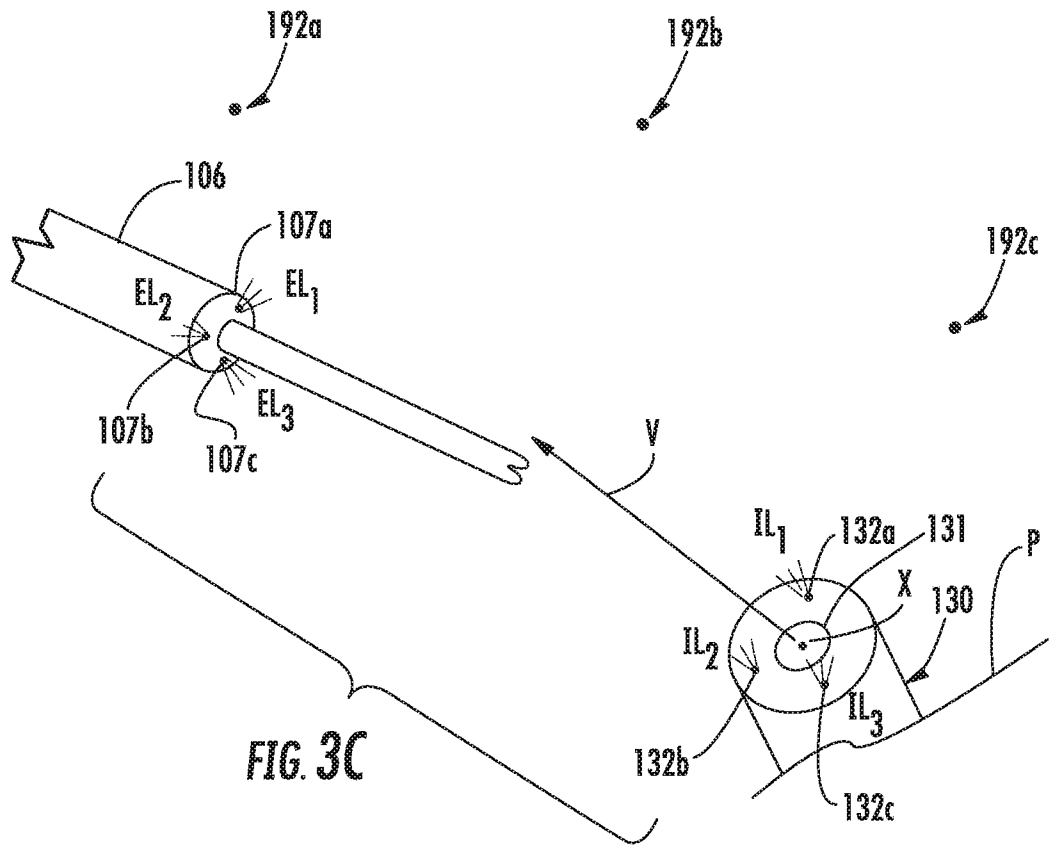


FIG. 3C

5/5

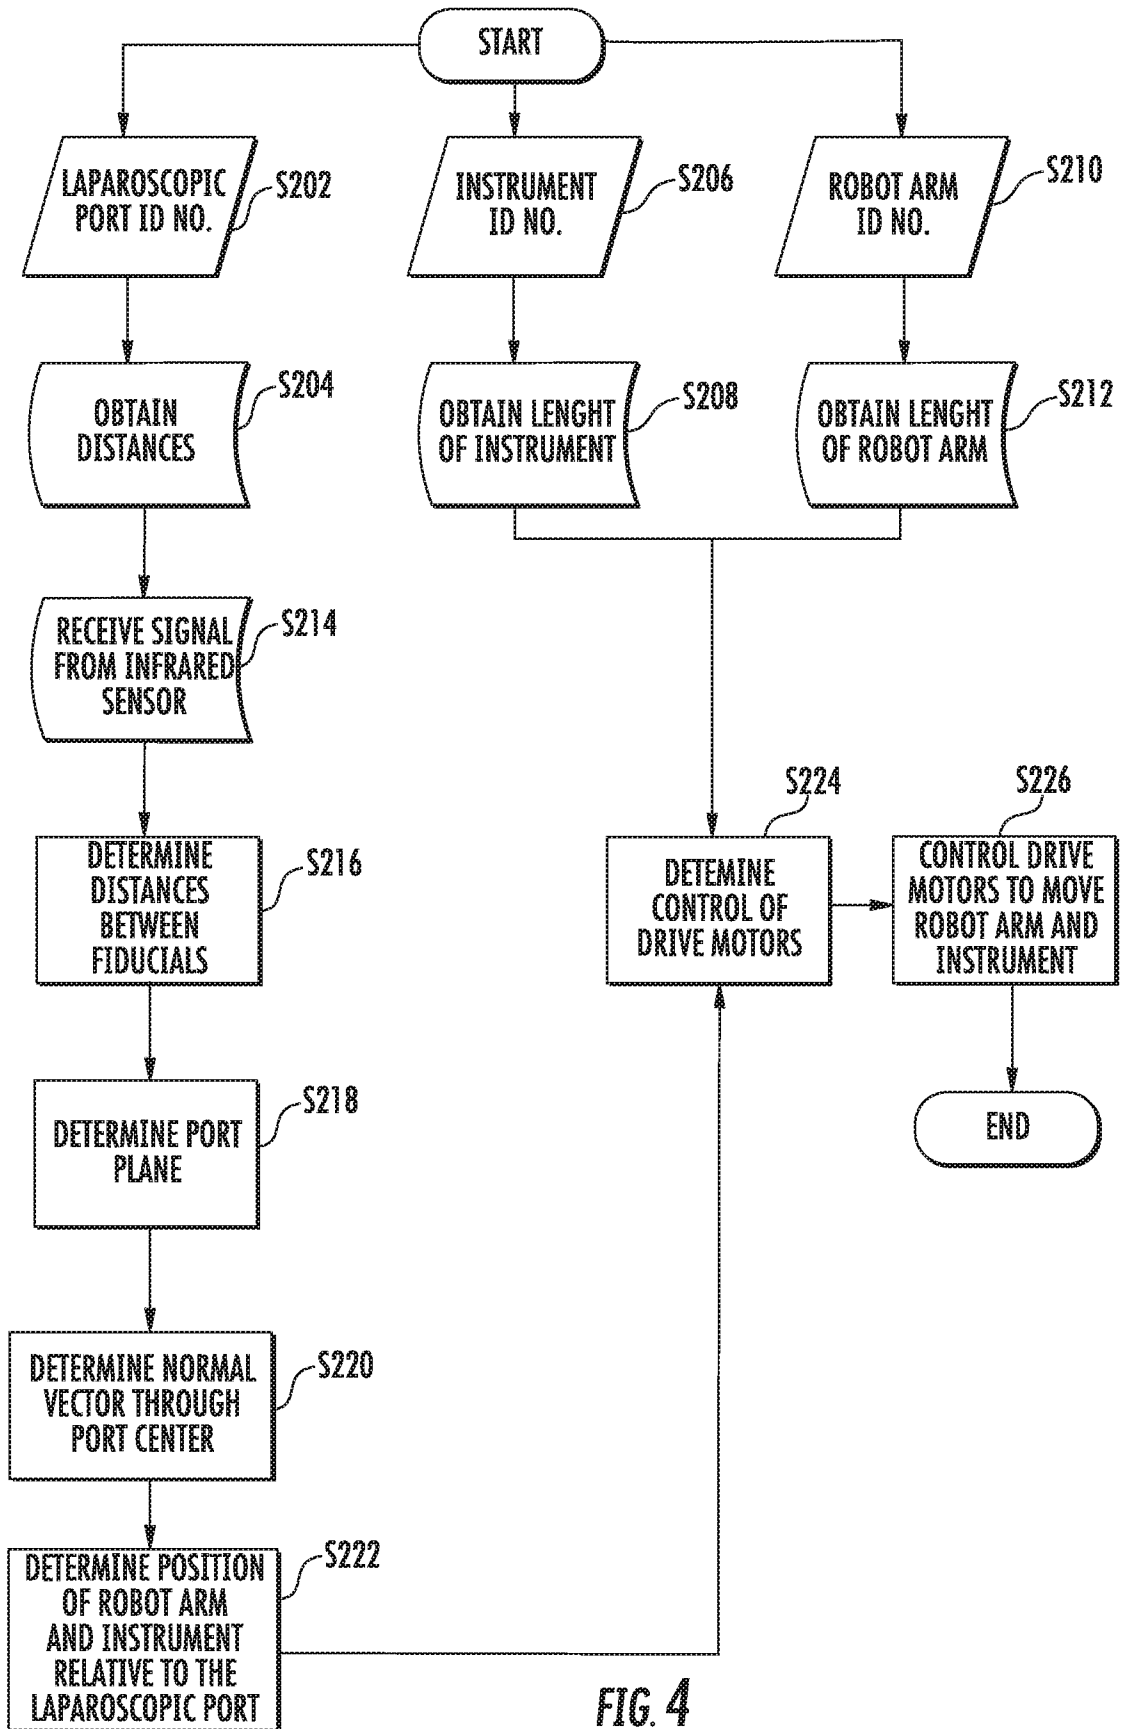


FIG. 4

A. CLASSIFICATION OF SUBJECT MATTER**A61B 34/32(2016.01)i, A61B 34/00(2016.01)i, A61B 34/20(2016.01)i, A61B 17/00(2006.01)i**

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61B 34/32; A61B 34/20; A61B 17/34; A61B 19/00; A61B 90/11; B25J 9/04; A61B 5/06; A61B 34/00; A61B 17/00

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Korean utility models and applications for utility models

Japanese utility models and applications for utility models

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

eKOMPASS(KIPO internal) & Keywords: robotic surgical system, arm, instrument, laparoscopic port, fiducial, sensors, controller, port plane, distance, vector

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 2013-0066335 A1 (BARWINKEL, R. et al.) 14 March 2013 See paragraphs [0037]-[0051]; claims 11-20; figures 1, 2.	1-19
A	US 2014-0276007 A1 (SYNAPTIVE MEDICAL (BARBADOS) INC.) 18 September 2014 See the whole document.	1-19
A	US 2017-0007349 A1 (SOLAR, M. S. et al.) 12 January 2017 See the whole document.	1-19
A	US 2010-0241079 A1 (ABRAMS, M. E.) 23 September 2010 See the whole document.	1-19
A	WO 2007-088206 A2 (THE EUROPEAN ATOMIC ENERGY COMMUNITY (EURATOM), REPRESENTED BY THE EUROPEAN COMMISSION et al.) 09 August 2007 See the whole document.	1-19

 Further documents are listed in the continuation of Box C. See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

29 August 2018 (29.08.2018)

Date of mailing of the international search report

03 September 2018 (03.09.2018)

Name and mailing address of the ISA/KR

International Application Division

Korean Intellectual Property Office

189 Cheongsu-ro, Seo-gu, Daejeon, 35208, Republic of Korea



Facsimile No. +82-42-481-8578

Authorized officer

HAN, Inho

Telephone No. +82-42-481-3362



INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2018/031302

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2013-0066335 A1	14/03/2013	CN 102905642 A EP 2575662 A1 EP 2575662 B1 US 9066737 B2 WO 2011-147651 A1	30/01/2013 10/04/2013 18/10/2017 30/06/2015 01/12/2011
US 2014-0276007 A1	18/09/2014	CA 2846729 A1	15/09/2014
US 2017-0007349 A1	12/01/2017	US 2013-0096570 A1 US 2014-0288578 A1 US 8747419 B2 US 9445793 B2 WO 2011-156701 A2 WO 2011-156701 A3	18/04/2013 25/09/2014 10/06/2014 20/09/2016 15/12/2011 10/05/2012
US 2010-0241079 A1	23/09/2010	AU 2010-201013 A1 CA 2696485 A1 EP 2229899 A1 JP 2010-221030 A US 8137319 B2	07/10/2010 20/09/2010 22/09/2010 07/10/2010 20/03/2012
WO 2007-088206 A2	09/08/2007	CA 2635135 A1 CN 101421080 A CN 101421080 B EP 1815949 A1 EP 1984150 A2 EP 1984150 B1 JP 2009-525097 A JP 5148512 B2 KR 10-1306215 B1 KR 10-2008-0100211 A US 2010-0204713 A1 US 9358682 B2 WO 2007-088206 A3	09/08/2007 29/04/2009 21/12/2011 08/08/2007 29/10/2008 04/07/2018 09/07/2009 20/02/2013 09/09/2013 14/11/2008 12/08/2010 07/06/2016 20/09/2007

专利名称(译)	具有自动向导的机器人手术系统		
公开(公告)号	EP3629980A1	公开(公告)日	2020-04-08
申请号	EP2018806526	申请日	2018-05-07
[标]申请(专利权)人(译)	柯惠有限合伙公司		
申请(专利权)人(译)	COVIDIEN LP		
当前申请(专利权)人(译)	COVIDIEN LP		
[标]发明人	CHOWANIEC MATTHEW CHEN XINGRUI		
发明人	CHOWANIEC, MATTHEW CHEN, XINGRUI		
IPC分类号	A61B34/32 A61B34/00 A61B34/20 A61B17/00		
CPC分类号	A61B34/32 A61B2034/302 A61B2090/3979 A61B90/36 A61B2034/301 A61B2090/363		
代理机构(译)	MASCHIO , ANTONIO		
优先权	62/510938 2017-05-25 US		
外部链接	Espacenet		

摘要(译)

一种机器人手术系统，包括至少一个机器人臂，至少一个器械以及多个驱动马达，所述多个驱动马达被配置为驱动所述至少一个机器人臂和至少一个器械。该系统还包括具有多个基准的腹腔镜端口，被配置为检测多个基准的传感器以及被配置为控制多个驱动马达的控制器。该控制器包括处理器，该处理器确定多个基准中的每个基准之间的当前距离，基于每个基准之间的距离确定腹腔镜端口的位置，确定至少一个机械臂和至少一个器械的位置。相对于腹腔镜端口的位置，并且控制多个驱动马达以使至少一个机械臂或至少一种器械与腹腔镜端口对准。