



US010136881B2

(12) **United States Patent**
Mariani

(10) **Patent No.:** **US 10,136,881 B2**
(45) **Date of Patent:** **Nov. 27, 2018**

(54) **LAPAROSCOPIC RETRACTOR DEVICES**

5,271,385 A 12/1993 Bailey
5,353,784 A * 10/1994 Nady-Mohamed
A61B 17/0218
600/205

(71) Applicant: **Mayo Foundation for Medical
Education and Research**, Rochester,
MN (US)

5,439,476 A 8/1995 Frantzides
5,441,044 A 8/1995 Tovey et al.
6,913,610 B2 7/2005 Nakao
7,052,502 B2 5/2006 Le Huec
7,112,172 B2 9/2006 Orban et al.
7,122,003 B2 10/2006 Nakao

(72) Inventor: **Andrea Mariani**, Rochester, MN (US)

(73) Assignee: **Mayo Foundation for Medical
Education and Research**, Rochester,
MN (US)

(Continued)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 648 days.

FOREIGN PATENT DOCUMENTS

EP 2088934 8/2009
EP 3075322 10/2016
(Continued)

(21) Appl. No.: **14/614,616**

(22) Filed: **Feb. 5, 2015**

(65) **Prior Publication Data**

US 2015/0223795 A1 Aug. 13, 2015

Related U.S. Application Data

(60) Provisional application No. 61/938,234, filed on Feb.
11, 2014.

(51) **Int. Cl.**

A61B 1/32 (2006.01)

A61B 17/02 (2006.01)

(52) **U.S. Cl.**

CPC **A61B 17/0218** (2013.01)

(58) **Field of Classification Search**

CPC combination set(s) only.

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,178,133 A 1/1993 Pena
5,267,554 A 12/1993 Wilk

OTHER PUBLICATIONS

“Comparison of EZ Surgical A-Lap™ and Diamond Flex Retractor,” Eisner USA.com [online] modified Nov. 1, 2010. Retrieved from the Internet: <URL: http://www.eisnerusa.com/download/comparison/Comparison+Table_A+Lap+Diamond+Flex+retractor.pdf>, 2 pages.

(Continued)


Primary Examiner — Sameh Boles

(74) *Attorney, Agent, or Firm* — Fish & Richardson P.C.

(57) **ABSTRACT**

Devices for performing medical procedures such as laparoscopic surgery are provided herein. For example, this document provides laparoscopic retractor devices. In some embodiments, the laparoscopic retractor devices provided herein include two retractor blades that can be expanded or contracted. Further, in some embodiments an elastic covering is included, and the retractor blades are disposed within the elastic covering.

17 Claims, 7 Drawing Sheets

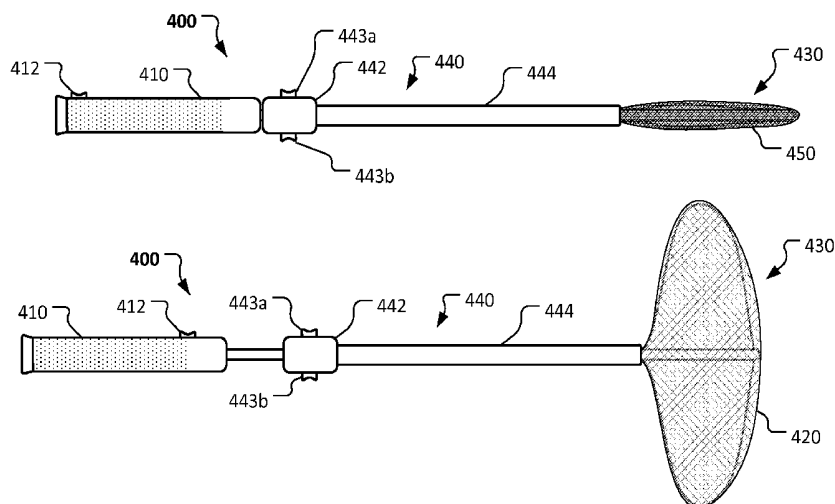

(56)

References Cited

U.S. PATENT DOCUMENTS

7,766,823 B2	8/2010	Moll et al.
8,007,508 B2	8/2011	Cox
8,097,008 B2	1/2012	Henderson
8,562,522 B2	10/2013	Antanaitis
8,840,638 B2	9/2014	Sherwinter
9,107,648 B2	8/2015	Ransden et al.
9,314,153 B2	4/2016	Stein et al.
9,326,757 B2	5/2016	Ravikumar et al.
9,445,800 B2	9/2016	Nguyen
2003/0225432 A1	12/2003	Baptiste et al.
2005/0043750 A1	2/2005	Scott, III et al.
2007/0213595 A1	9/2007	Ravikumar
2008/0146881 A1	6/2008	Alimi et al.
2009/0192360 A1	7/2009	Riess et al.
2010/0174149 A1	7/2010	Moll et al.
2010/0228093 A1	9/2010	Voegelé et al.
2010/0292718 A1	11/2010	Sholev et al.
2011/0082479 A1*	4/2011	Friedlander A61F 2/0063 606/151
2011/0105848 A1	5/2011	Sadovsky et al.
2011/0144450 A1	6/2011	Paolitto et al.
2012/0046525 A1	2/2012	Russell et al.
2012/0059225 A1	3/2012	Gostout et al.
2012/0088978 A1	4/2012	Park et al.
2012/0123215 A1	5/2012	Begg
2012/0238824 A1	9/2012	Widenhouse et al.
2012/0245417 A1	9/2012	Winterberg et al.
2013/0066155 A1	3/2013	Keating et al.
2013/0172682 A1	7/2013	Ransden et al.
2014/0039264 A1	2/2014	Heiman
2014/0316209 A1	10/2014	Overes et al.
2015/0065805 A1	3/2015	Edmondson et al.
2015/0245828 A1	9/2015	Harari et al.
2016/0256147 A1	9/2016	Jeong et al.
2016/0278756 A1	9/2016	Aho et al.

FOREIGN PATENT DOCUMENTS

GB	245990	11/2009
WO	WO2008068405	6/2008
WO	WO 2010094799	8/2010

OTHER PUBLICATIONS

"iLap: A New Laparoscopic Retractor," 2011 [retrieved on Sep. 11, 2015]. Retrieved from the Internet: <URL: <http://blogs.ucc.ie/wordpress/biodesign/biodesign-2011/>>, 4 pages.

"UZit A-Lap™," ezsurgical.com [online], archived Aug. 29, 2014 [retrieved on Sep. 23, 2015]. Retrieved from the Internet: <URL: <https://web.archive.org/web/20140829004856/http://ezsurgical.com/Products.asp?Page=UZit>>, 2 pages.

Alimi et al., "Intestinal retractor for transperitoneal laparoscopic aortoiliac reconstruction: experimental study on human cadavers and initial clinical experience," *Surg Endosc.*, 14(10):915-919, Oct. 2000.

Autosuture, "Endo Retract™ II 10 mm Retractor," Bio-Medicine.org [online] archived Sep. 2, 2014. Retrieved from the Internet: <URL: <https://web.archive.org/web/20140902102146/http://www.bio-medicine.org/medicine-products/ENDO-RETRACT-26trade-3B-II-10-mm-Retractor-11126-1/>>.

Autosuture, "Endo Mini-Retract™ 5 mm Retractor," Bio-Medicine.org [online] archived Jan 15, 2009. Retrieved from the Internet: <URL: <https://web.archive.org/web/20090115091133/http://www.bio-medicine.org/medicine-products/ENDO-MINI-RETRACT-26trade-3B-5-mm-Retractor-11124-1/>>, 1 page.

Autosuture, "Endo Paddle Retract™ 12 mm Retractor," Bio-Medicine.org [online] archived Nov. 26, 2014. Retrieved from the Internet: <URL: <https://web.archive.org/web/20141126231117/http://bio-medicine.org/medicine-products/ENDO-PADDLE-RETRACT-26trade-3B-12-mm-Retractor-11122-1/>>, 1 page.

Autosuture, "Endo Peanut™ 5 mm Retractor," Bio-Medicine.org [online] archived Dec. 3, 2008. Retrieved from the Internet: <URL: <https://web.archive.org/web/20081203114049/http://www.bio-medicine.org/medicine-products/ENDO-PEANUT-26trade-3B-5-mm-Retractor-11121-1/>>, 1 page.

Autosuture, "Endo Retract™ 10 mm Retractor," bio-medicine.org [online] archived Dec. 3, 2008. Retrieved from the Internet: <URL: <https://web.archive.org/web/20081203113738/http://www.bio-medicine.org/medicine-products/ENDO-RETRACT-26trade-3B-10-mm-Retractor-11125-1/>>, 1 page.

Autosuture, "Endo Retract™ Maxi 10 mm Retractor," Bio-Medicine.org [online] archived Dec. 3, 2008. Retrieved from the Internet: <URL: <https://web.archive.org/web/20081203113912/http://www.bio-medicine.org/medicine-products/ENDO-RETRACT-26trade-3B-Maxi-10-mm-Retractor-11123-1/>>, 1 page.

Autosuture, "Extrahand™ Balloon Retractor," Bio-Medicine.org [online] archived Sep. 2, 2014. Retrieved from the Internet: <URL: <https://web.archive.org/web/20140902110631/http://www.bio-medicine.org/medicine-products/EXTRAHAND-26trade-3B-Balloon-Retractor-11131-1/>>, 1 page.




Barbera et al., "Newly designed retraction devices for intestine control during laparoscopic aortic surgery: a comparative study in an animal model," *Surg Endosc.*, 14(1):63-66, Jan. 2000.

CareFusion, "Snowden-Pencer® laparoscopic articulating retractors," Carefusion.com [online] 2012 [retrieved on Sep. 14, 2015]. Retrieved from the Internet: <http://www.carefusion.com/pdf/Surgical_Instrumentation/Articulating_retractors_brochure.pdf>, 4 pages.

Gyms ACMI, "Soft-Wand™ Balloon Retractor," [product catalog] 2 pages, 2008.

Paolucci et al., "Exposure of the operative field in laparoscopic surgery," *Surg Endosc.*, 11(8):856-863, Aug. 1997.

* cited by examiner

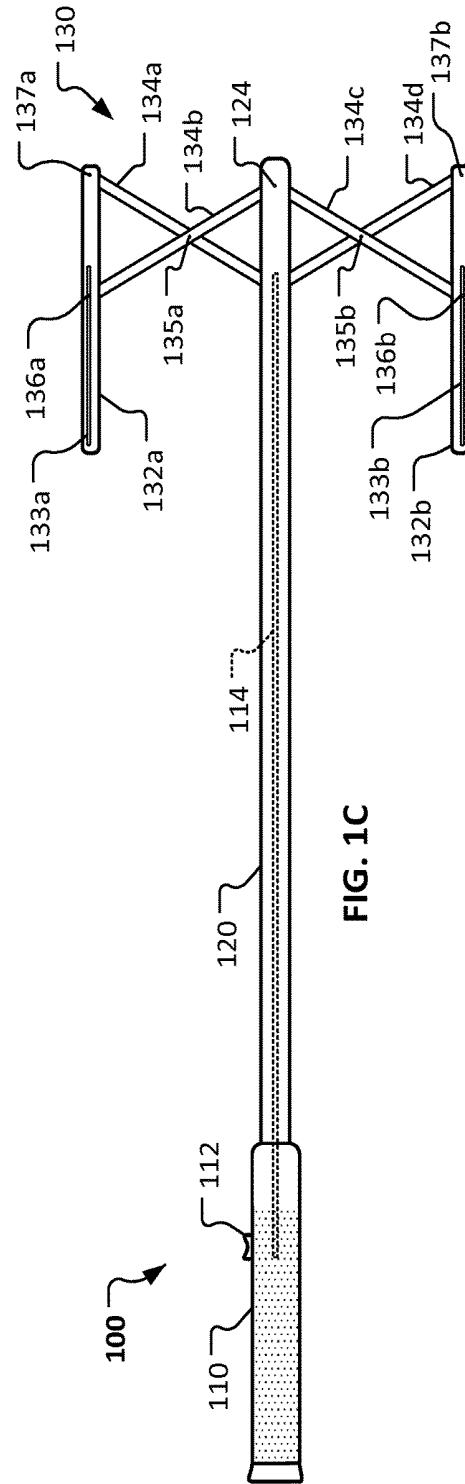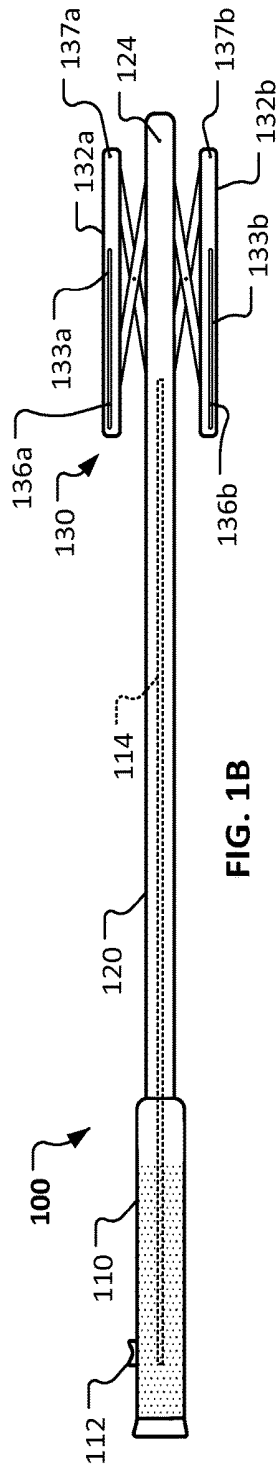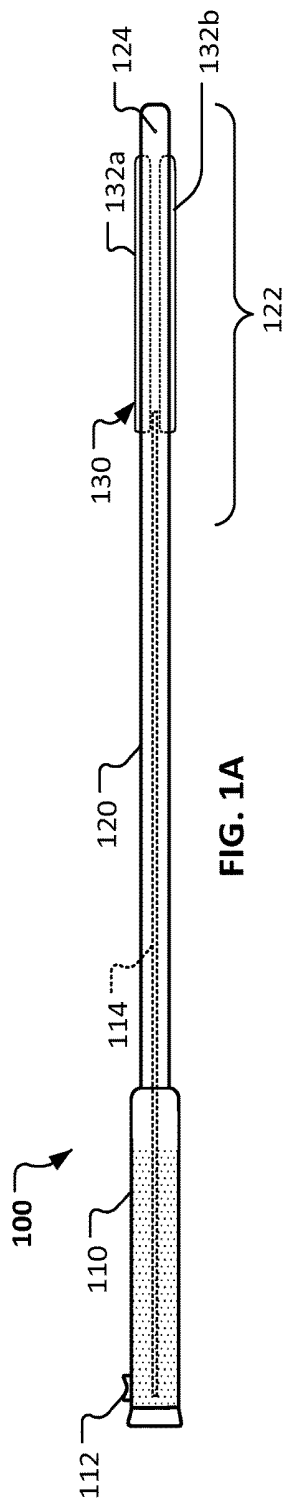

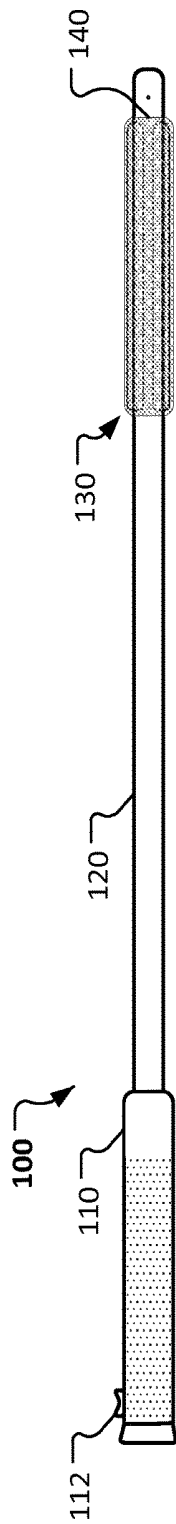


FIG. 2A

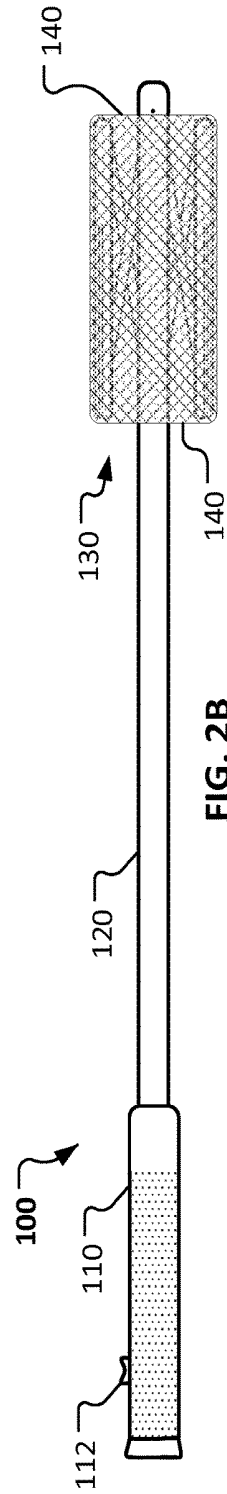


FIG. 2B

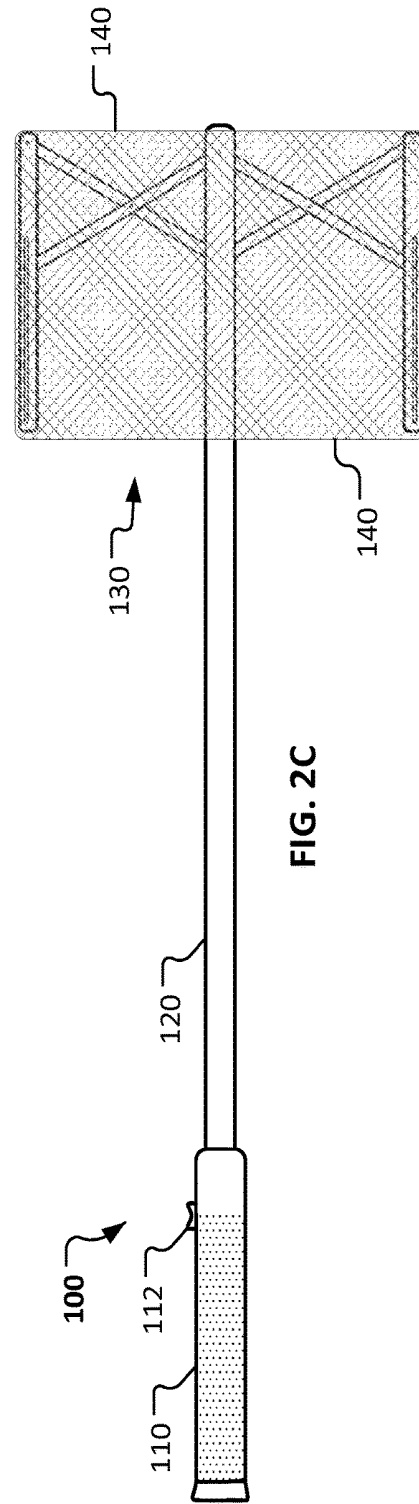


FIG. 2C

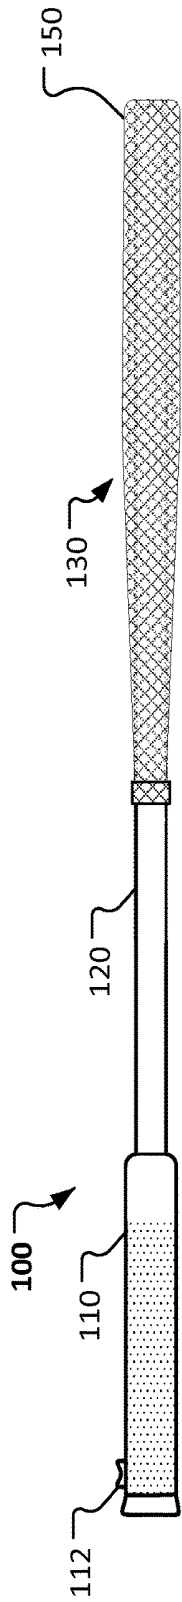


FIG. 3A

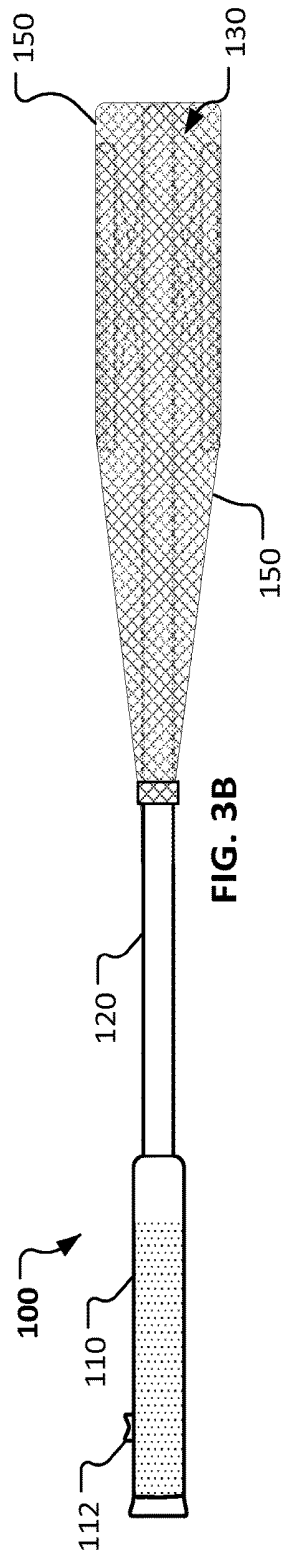


FIG. 3B

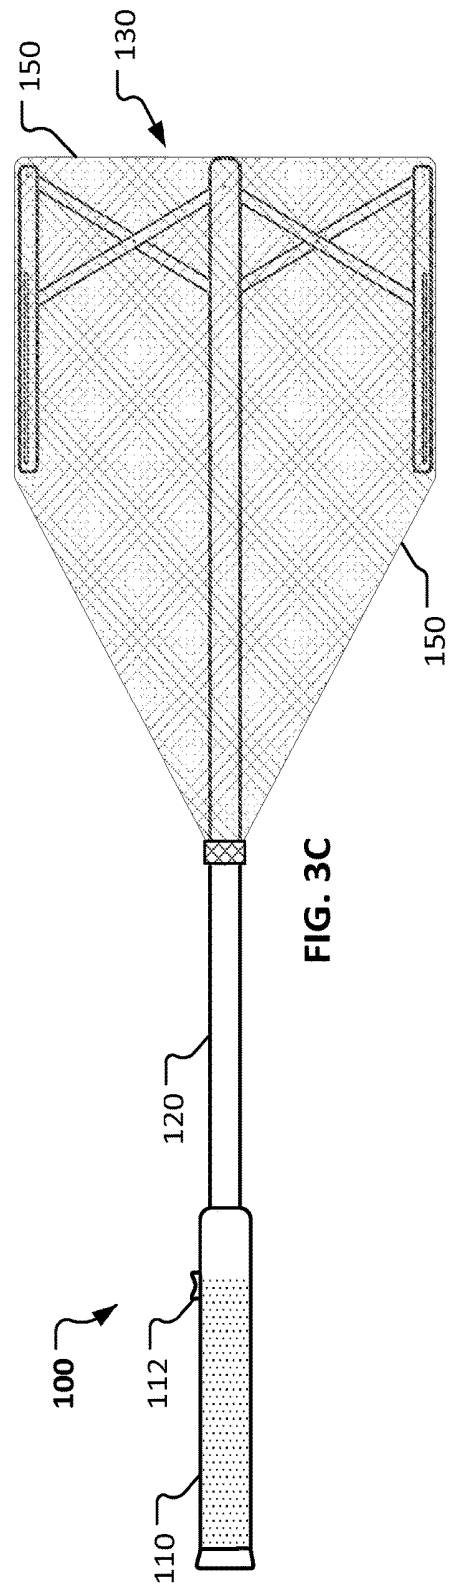
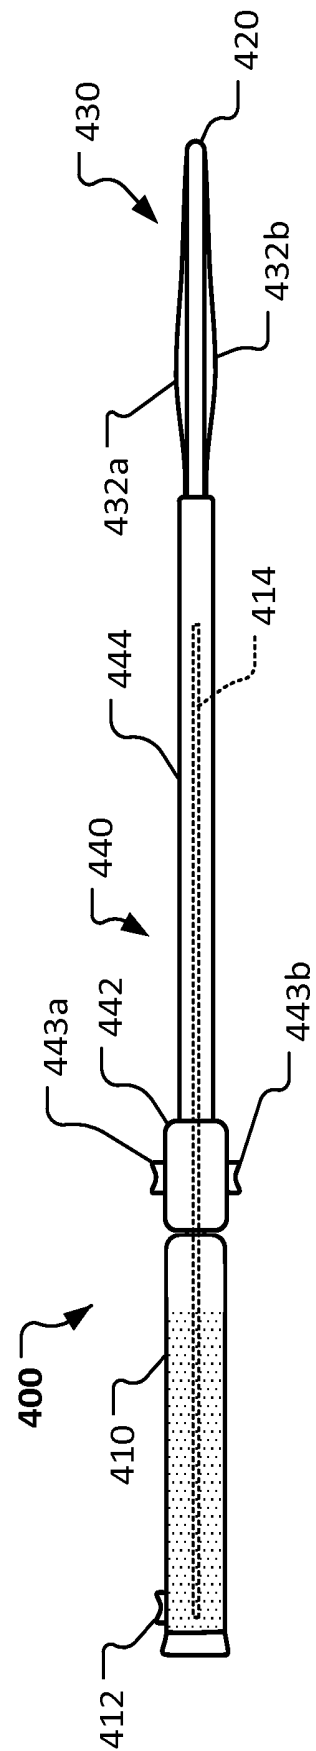
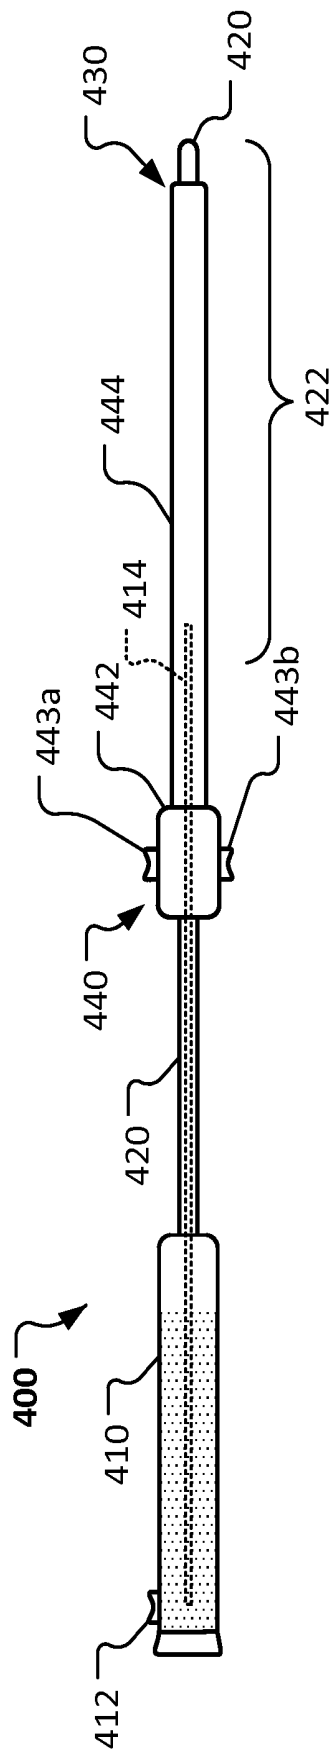
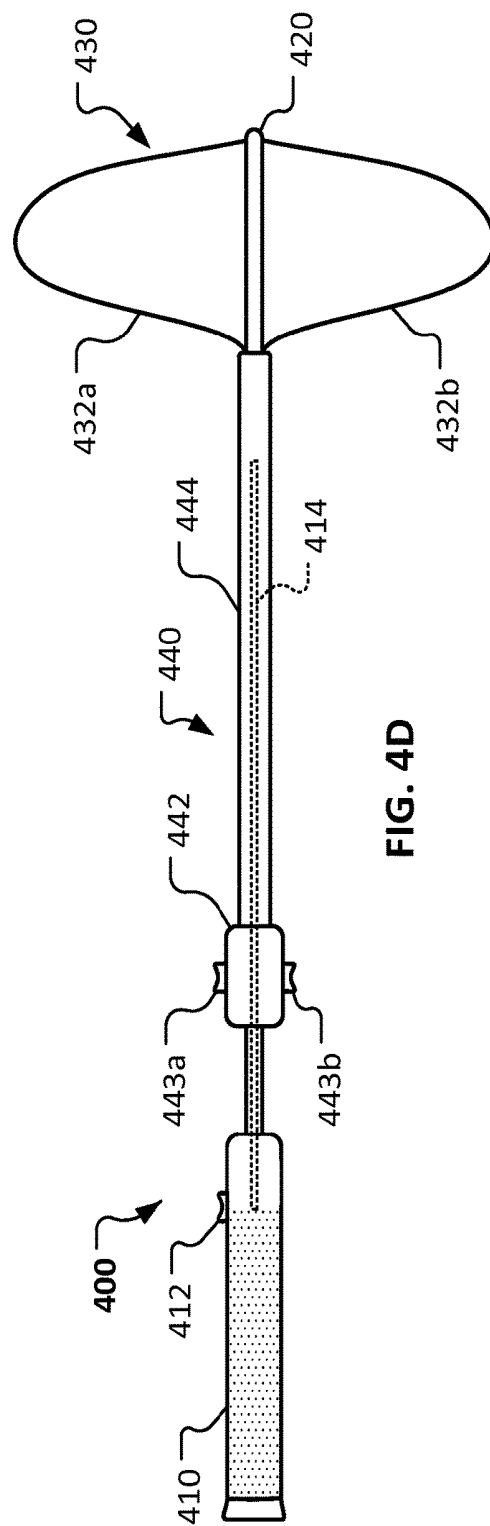
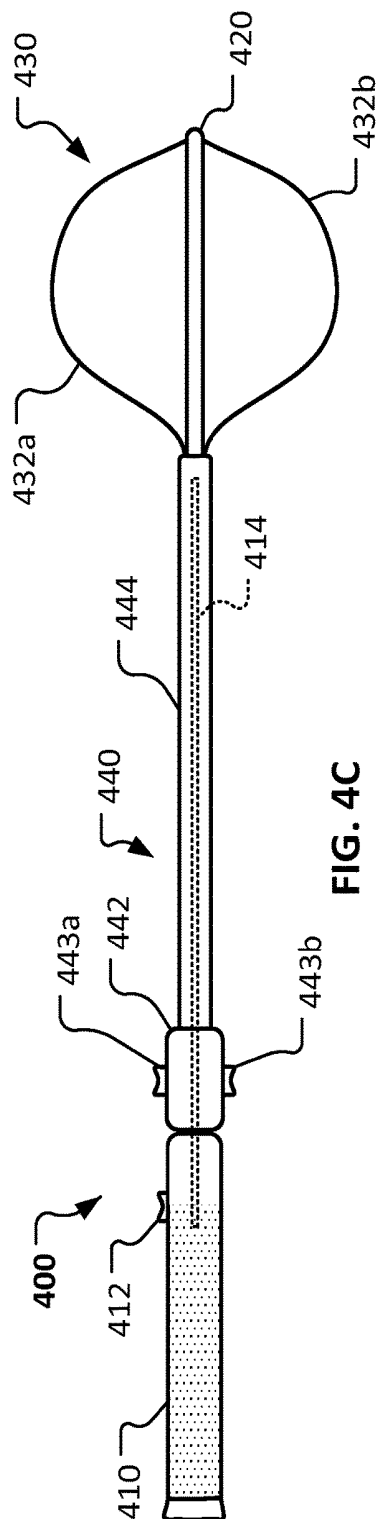


FIG. 3C





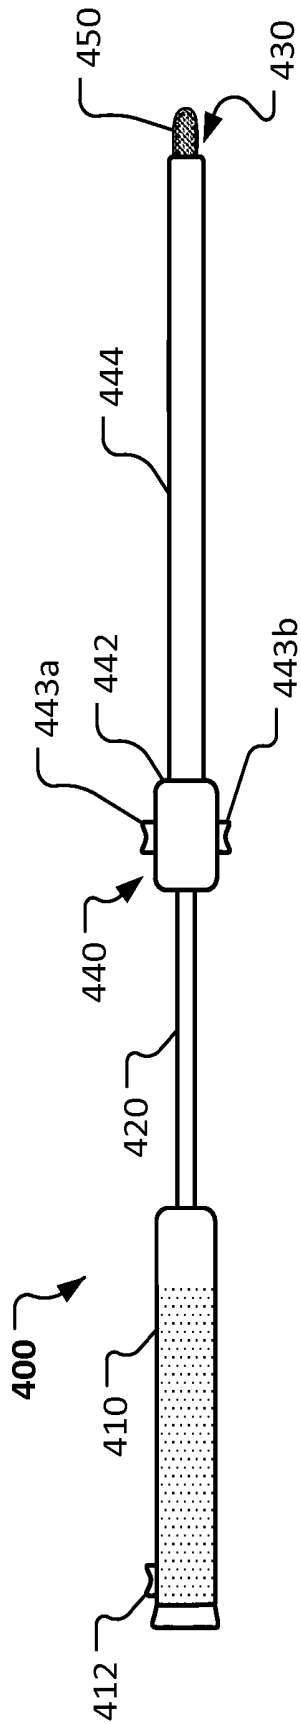


FIG. 5A



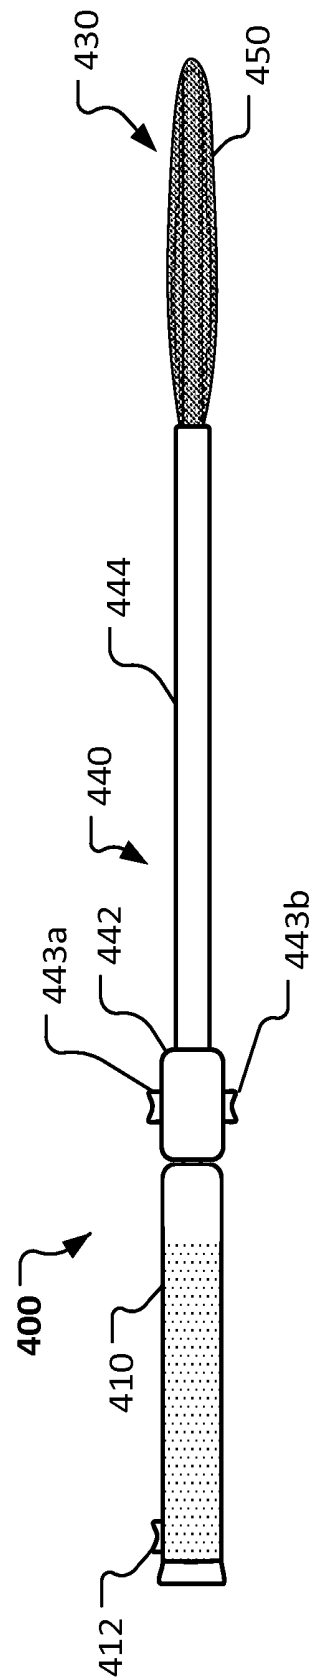


FIG. 5B

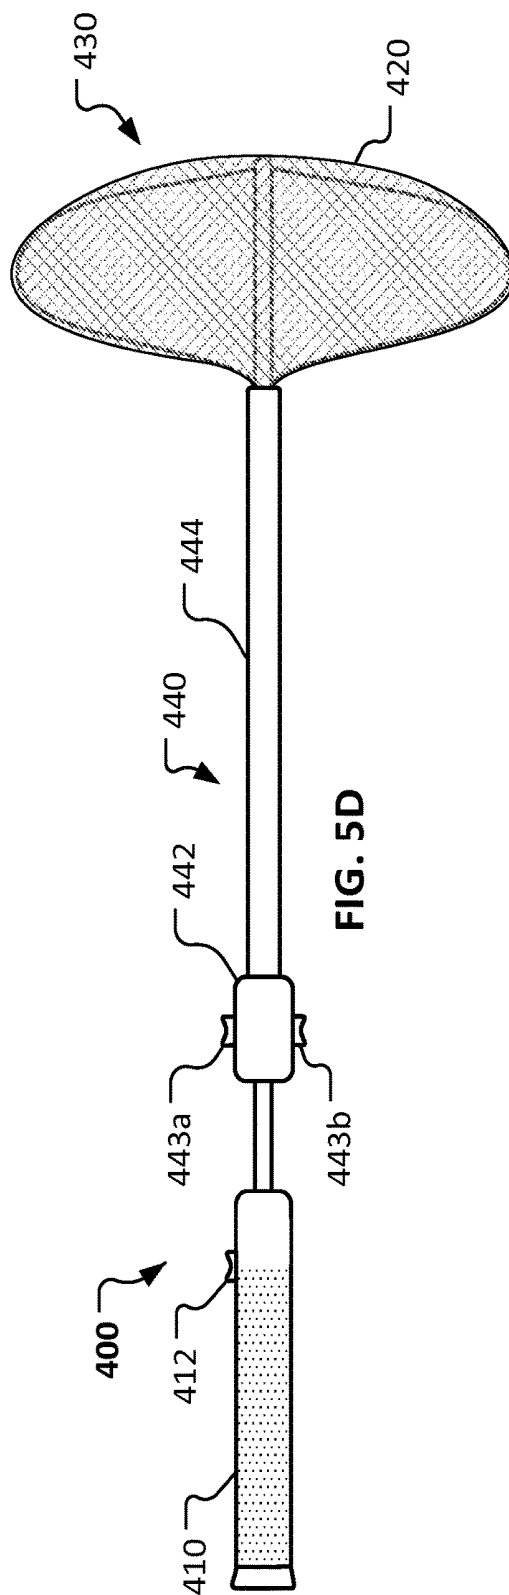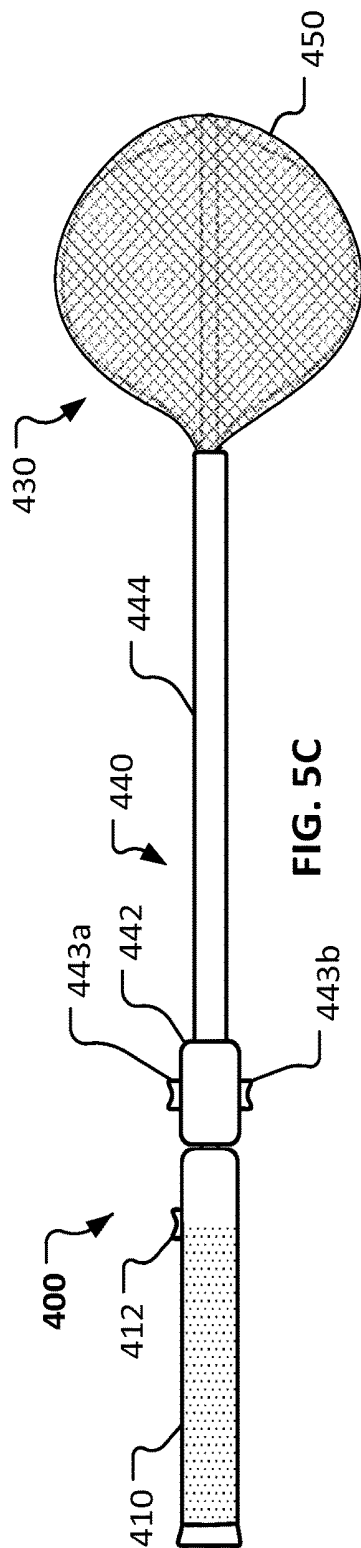

LAPAROSCOPIC RETRACTOR DEVICES**CROSS-REFERENCE TO RELATED APPLICATIONS**

This application claims the benefit of U.S. Provisional Application Ser. No. 61/938,234, filed Feb. 11, 2014. The disclosure of the prior application is considered part of (and is incorporated by reference in) the disclosure of this application.

BACKGROUND**1. Technical Field**

This document relates to devices for performing medical procedures such as laparoscopic surgery. For example, this document relates to retractor devices such as laparoscopic bowel retractors for use in performing intra-abdominal surgery.

2. Background Information

Optimal visualization of the operative field is a fundamental principle in surgery. Any technique that improves intra-operative visualization has the potential to make surgery safer and more cost efficient. With the advent of minimally invasive surgery, the utilization of laparoscopic or robotic surgery is becoming the standard of care for many abdominal surgeries. However, there are areas of the abdominal cavity, like the paraaortic area, in which the minimally invasive approach is still challenging. In fact, small bowel loops frequently obscure the paraaortic surgical field, especially in obese patients.

Endometrial cancer is the fourth most prevalent malignancy in the United States. It is estimated that approximately 40% of endometrial cancer patients need to have a paraaortic lymphadenectomy, which involves surgery in the area of the aorta and vena cava. In 70% of such cases, the surgical site is either partially or completely obstructed by the small bowel, making the procedure sometimes impractical to perform by minimally invasive robotic surgery.

Some intestinal retraction devices are either too small for the amount of bowel that needs to be restrained, too cumbersome to use, or too difficult to retrieve. There is a need for an improved bowel retractor device that is convenient to operate and effective for keeping the bowel away from the operative field, including for obese patients.

SUMMARY

This document provides devices for performing medical procedures such as laparoscopic surgery. For example, this document provides laparoscopic retractor devices. In some embodiments, the laparoscopic retractor devices provided herein include two retractor blades that can be expanded or contracted. Further, in some embodiments an elastic covering is included, and the retractor blades are disposed within the elastic covering.

In general, one aspect of this document features a laparoscopic retractor device. The laparoscopic retractor device comprises a handle and an elongate shaft with a proximal end portion that is attached to the handle. The shaft extends from the handle and terminates at a distal free end portion. The shaft includes a first lumen therethrough. The laparoscopic retractor device further comprises an elongate shaft linkage disposed within the first lumen. The shaft linkage has a proximal end and a distal end. The laparoscopic retractor device further comprises an actuator located at the handle and coupled to the proximal end of the shaft linkage,

and an expandable portion coupled to the shaft at the distal free end portion and coupled to the distal end of the shaft linkage. In some embodiments, moving the actuator causes the expandable portion to move radially outward from the shaft or radially inward toward the shaft.

Some implementations of the laparoscopic retractor device may further comprise an elastic covering that is disposed around the expandable portion. In various implementations of the laparoscopic retractor device the actuator may be slidable in relation to the handle. In some implementations, sliding the actuator distally may cause the expandable portion to expand, and sliding the actuator proximally may cause the expandable portion to contract. The expandable portion may comprise at least two retractor blades in some embodiments. In some such embodiments, causing the expandable portion to expand may comprise causing the at least two retractor blades to move radially outward from the shaft, and causing the expandable portion to contract may comprise causing the at least two retractor blades to move radially inward toward the shaft. Further, in some implementations the at least two retractor blades may be elongate blades that include axes that are substantially parallel to a longitudinal axis of the shaft and remain substantially parallel to the axis of the shaft while moving radially outward from and inward toward the shaft. Still further, in some implementations the expandable portion may further comprise scissor arms, and the scissor arms may be pivotably coupled to the at least two retractor blades and to the shaft. Some such implementations may further comprise an elastic covering that may be disposed around the at least two retractor blades.

In another general aspect, this document features another laparoscopic retractor device embodiment comprising: a handle; an elongate shaft with a proximal end portion that is attached to the handle, the shaft extending from the handle and terminating at a distal free end portion, the shaft including a first lumen therethrough; an elongate shaft linkage disposed within the first lumen, the shaft linkage having a proximal end and a distal end; a first actuator located at the handle and coupled to the proximal end of the shaft linkage; an expandable portion coupled to the shaft at the distal free end portion and coupled to the distal end of the shaft linkage, wherein moving the actuator causes the expandable portion to move radially outward from the shaft or radially inward toward the shaft; and a sheath with a lumen therethrough, at least a portion of the shaft being disposed within the lumen, the sheath being slidable distally and proximally along the shaft.

Some implementations of the laparoscopic retractor device may further comprise an elastic covering that is disposed around the expandable portion of the another laparoscopic retractor device embodiment. In various implementations of the laparoscopic retractor device embodiment the sheath may include a hub that is connected to a proximal end of the sheath, and the hub may include a second actuator whereby the hub can be locked and unlocked from being coupled to the shaft. In some embodiments, the first actuator may be slidable in relation to the handle. In particular embodiments, sliding the first actuator distally may cause the expandable portion to expand, and sliding the first actuator proximally may cause the expandable portion to contract. Optionally, the expandable portion may comprise at least two retractor blades. In some implementations, causing the expandable portion to expand may comprise causing the at least two retractor blades to bend and to move radially outward from the shaft, and causing the expandable portion to contract may comprise causing the at least two

retractor blades unbend and to move radially inward toward the shaft. In particular implementations, by sliding the sheath distally at least some portion of the at least two retractor blades can be made to move further radially away from the shaft. Further, by sliding the sheath proximally at least some portion of the at least two retractor blades can be made to move further radially inward toward the shaft in some implementations. The laparoscopic retractor device may further comprise an elastic covering that is disposed around the at least two retractor blades.

Particular embodiments of the subject matter described in this document can be implemented to realize one or more of the following advantages. In some embodiments, the laparoscopic retractor devices provided herein are readily adjustable in size from a low profile contracted configuration to a substantially wider expanded configuration for performing retraction of tissue and organs. The laparoscopic retractor devices provided herein have intuitive and easy to operate designs. In some embodiments, various surgeries can be performed in a minimally invasive fashion using the devices and methods provided herein. Such minimally invasive techniques can reduce recovery times, patient discomfort, and treatment costs. In some embodiments, the laparoscopic retractor devices provided herein are designed to minimize the risk of pinching or impinging tissue during the adjustment of the retractors between the contracted and expanded configurations. Further, the laparoscopic retractor devices provided herein do not include separable pieces. As such, clinicians can operate the retractor devices without a risk of pieces becoming detached within a body cavity.

Unless otherwise defined, all technical and scientific terms used herein have the same meaning as commonly understood by one of ordinary skill in the art to which this invention pertains. Although methods and materials similar or equivalent to those described herein can be used to practice the invention, suitable methods and materials are described herein. All publications, patent applications, patents, and other references mentioned herein are incorporated by reference in their entirety. In case of conflict, the present specification, including definitions, will control. In addition, the materials, methods, and examples are illustrative only and not intended to be limiting.

The details of one or more embodiments of the invention are set forth in the accompanying drawings and the description herein. Other features, objects, and advantages of the invention will be apparent from the description and drawings, and from the claims.

DESCRIPTION OF THE DRAWINGS

FIG. 1A is a side view of a laparoscopic bowel retractor device, shown in a contracted configuration, in accordance with some embodiments provided herein.

FIG. 1B is a side view of the laparoscopic retractor device of FIG. 1A shown in a partially expanded configuration.

FIG. 1C is a side view of the laparoscopic retractor device of FIG. 1A shown in an expanded configuration.

FIGS. 2A-2C show the laparoscopic retractor device of FIG. 1A in the same configurations of FIGS. 1A-1C, and with the addition of an example elastic covering on the expandable portion, in accordance with some embodiments provided herein.

FIGS. 3A-3C show the laparoscopic retractor device of FIG. 1A in the same configurations of FIGS. 1A-1C, and with the addition of another example elastic covering on the expandable portion, in accordance with some embodiments provided herein.

FIG. 4A is a side view of another laparoscopic bowel retractor device, shown in a contracted configuration, in accordance with some embodiments provided herein.

FIG. 4B is a side view of the laparoscopic retractor device of FIG. 4A showing a revealed expandable portion.

FIG. 4C is a side view of the laparoscopic retractor device of FIG. 4A shown in an expanded configuration.

FIG. 4D is a side view of the laparoscopic retractor device of FIG. 4A shown in another expanded configuration.

FIGS. 5A-5D show the laparoscopic retractor device of FIG. 4A in the same configurations of FIGS. 4A-4D, and with the addition of an example elastic covering on the expandable portion, in accordance with some embodiments provided herein.

Like reference numbers represent corresponding parts throughout.

DETAILED DESCRIPTION

This document provides devices for performing medical procedures such as laparoscopic surgery. For example, this document provides laparoscopic retractor devices. In some embodiments, the laparoscopic retractor devices provided herein include two retractor blades that can be expanded or contracted. Further, in some embodiments an elastic covering is included, and the retractor blades are disposed within the elastic covering.

In one example implementation, the laparoscopic retractor devices provided herein can be used for performing surgeries such as, but not limited to, paraaortic lymphadenectomy procedures to treat endometrial cancer. Also, the laparoscopic bowel retractors provided herein may help to gain exposure and visualization of the surgical field in other areas of the abdomen that are obscured by the bowel, including other types of laparoscopic or robotic surgeries. In addition to such intra-abdominal surgeries, in some cases the laparoscopic bowel retractor devices provided herein may be used for procedures in other medical specialties such as, but not limited to, urology, vascular surgery, and general surgery.

Referring to FIG. 1A, an example laparoscopic retractor device **100** in accordance with some embodiments provided herein includes a handle **110**, a shaft **120**, and an expandable portion **130**. The proximal end of shaft **120** is fixedly coupled to handle **110**. As will be explained further below, expandable portion **130** is movably coupled to shaft **120** at a distal end portion **122** of shaft **120** where shaft **120** terminates with a free end. It should be understood that the figures included in this disclosure are not necessarily to scale. However, the figures appropriately depict the design concepts so as to facilitate one of ordinary skill in the art to practice the inventive laparoscopic bowel retractor devices provided herein.

Laparoscopic retractor device **100** is shown in a contracted configuration. This contracted configuration may be used, for example, when inserting distal portion **122** of laparoscopic retractor device **100** into an internal space such as an abdomen of a patient, and thereafter when withdrawing laparoscopic retractor device **100**. In some implementations, distal portion **122** of laparoscopic retractor device **100** is inserted into a patient, while a proximal portion of laparoscopic retractor device **100** remains external to the patient.

In some circumstances, a trocar device is utilized as a portal to provide access to the patient's internal space such as the abdominal space. In such cases, distal portion **122** of laparoscopic retractor device **100** can be passed through the trocar. In some such cases, a trocar with an inner diameter

of about 1 centimeter (cm) is used, and distal portion **122** of laparoscopic retractor device **100** can be passed there-through when distal portion **122** is in the contracted configuration. In other implementations, laparoscopic retractor device **100** can be used with trocars having other inner diameter sizes, such as about 0.7 cm, about 0.8 cm, about, 0.9 cm, about 1.1 cm, about 1.2 cm, about 1.3 cm, about 1.4 cm, about 1.5 cm, about 1.6 cm, about 1.7 cm, about 1.8 cm, about 1.9 cm, or about 2.0 cm. Laparoscopic retractor device **100** can be provided in a range of sizes (diameters and lengths), and the suitably sized laparoscopic retractor device **100** can be selected for use in such various implementations. It should be understood that the use of a trocar may not be required in some implementations. In some other implementations, laparoscopic retractor device **100** can be passed through an incision.

Laparoscopic retractor device **100** includes shaft **120**. In some embodiments, shaft **120** is comprised of a metallic material. For example, metallic materials including, but not limited to, stainless steels (e.g., austenitic 316 stainless steel or martensitic 440 and 420 stainless steels), titanium, titanium alloys (e.g., Ti6Al4V), and the like, can be used for shaft **120**. In other embodiments, shaft **120** can be comprised of a polymeric material. For example, polymeric materials including, but limited to, polyvinyl chloride (PVC), PEBEX, PICOFLEX, TECOFLEX, PTFE, ePTFE, FEP, PEEK, silicone, urethane, polyethylene, polypropylene, and the like, can be used for shaft **120**. In some embodiments, at least portions of shaft **120** can be malleable or articulable.

As will be explained further below, shaft **120** includes at least one lumen. A shaft linkage **114** that extends from handle **110** to expandable portion **130** runs through the lumen and is slidable therein. In some embodiments, shaft linkage **114** is a solid metallic rod (e.g., stainless steel), or a solid polymeric rod (e.g., TEFLON, DELRIN, polyurethane, and the like). In other embodiments, a Bowden cable is used for shaft linkage **114**.

In some embodiments, shaft **120** includes more than one lumen. For example, one or more additional lumens can be optionally included in shaft **120** for purposes such as, but not limited to, suction, irrigation, and the like. In some cases, the optional lumen(s) has a diameter of about 5 millimeters (mm), but other smaller or larger sized lumens can be included in some embodiments.

Referring now to FIGS. 1A-1C, distal portion **122** of laparoscopic retractor device **100** can be expanded in situ (e.g., after insertion of laparoscopic retractor device **100** into the patient) to facilitate the retraction of internal tissue, such as the patient's intestines in the case of an intra-abdominal implementation. Such expansion of distal portion **122** is depicted in FIGS. 1B (partial expansion) and 1C (nearly full expansion).

Laparoscopic retractor device **100** also includes handle **110**. Handle **110** can be comprised of any suitable metallic or polymeric material such as, but not limited to, polymethyl methacrylate, polystyrene, acrylonitrile butadiene styrene (ABS), PVC, polyethylene, polypropylene, polycarbonate, and the like. Handle **110** can include a textured or contoured surface so that a clinician can get a good grip on handle **110**.

Handle **110** includes a sliding actuator knob **112**. Sliding actuator knob **112** can be used by an operator of laparoscopic retractor device **100** to expand or retract expandable portion **130**. That is, in some embodiments sliding actuator knob **112** can be depressed and slid distally or proximally in relation to handle **110**. Such sliding of sliding actuator knob **112** can expand or retract expandable portion **130** because of shaft linkage **114** that is connected therebetween. Sliding actuator

knob **112** can lock in place on the handle when the operator is no longer depressing sliding actuator knob **112**. In other embodiments, other types of actuators can be used as alternatives to sliding actuator knob **112**. For example, a rotary actuator, a lever, a trigger, and other types of actuators can be used in some embodiments.

Laparoscopic retractor device **100** also includes expandable portion **130**. Expandable portion **130** includes retractor blades **132a** and **132b** that are movably coupled to shaft **120** and shaft linkage **114** via scissor arms **134a**, **134b**, **134c**, and **134d**. Using such a mechanical arrangement, retractor blades **132a** and **132b** can be moved radially inward and outward from shaft **120** while remaining essentially parallel to shaft **120**.

One end of scissor arm **134a** is pivotably coupled to retractor blade **132a** using a pin **137a**. The other end of scissor arm **134a** is pivotably coupled to shaft linkage **114**.

One end of scissor arm **134b** is pivotably coupled to retractor blade **132a** using a pin **136a** that can translate in a slot **133a** located in retractor blade **132a**. The other end of scissor arm **134b** is pivotably coupled to shaft **120** using a pin **124**.

One end of scissor arm **134c** is pivotably coupled to retractor blade **132b** using a pin **137b**. The other end of scissor arm **134c** is pivotably coupled to shaft linkage **114**.

One end of scissor arm **134d** is pivotably coupled to retractor blade **132b** using a pin **136b** that can translate in a slot **133b** located in retractor blade **132b**. The other end of scissor arm **134d** is pivotably coupled to shaft **120** using a pin **124**.

Scissor arms **134a** and **134b** are pivotably coupled together near their midpoints using a pin **135a**. Similarly, scissor arms **134c** and **134d** are pivotably coupled together near their midpoints using a pin **135b**.

The components of expandable portion **130** can be metallic or polymeric. For example, in some embodiments some or all of the components of expandable portion **130** can be metals such as, but not limited to, stainless steels, titanium, titanium alloys, NiTi, and the like. In some embodiments, some or all of the components of expandable portion **130** can be polymers such as, but not limited to, DELRIN, TEFLON, polyurethane, polyethylene, polypropylene, and the like. In some embodiments, a combination of metallic and polymeric materials can be used to construct expandable portion **130**.

In some embodiments, retractor blades **132a** and **132b** are double-sided. In some such embodiments, retractor blades **132a** and **132b** have a U-shaped cross-section (like a channel) and the ends of scissor arms **134a-b** are within the channels (or between the double-sided retractor blades **132a** and **132b**).

Referring now to FIGS. 2A-2C, laparoscopic retractor device **100** can include an elastic covering **140** on expandable portion **130**. Elastic covering **140** can be a sleeve of stretchable material that surrounds and conforms to retractor blades **132a** and **132b**.

When retractor blades **132a** and **132b** are in the contracted configuration as shown in FIG. 2A, elastic covering **140** is also contracted such that it snugly conforms to retractor blades **132a** and **132b**. As retractor blades **132a** and **132b** are expanded radially outward from shaft **120**, elastic covering **140** stretches to remain surrounding and conforming to retractor blades **132a** and **132b** (as shown in FIGS. 2B and 2C). In some embodiments, elastic covering **140** is attached to retractor blades **132a** and **132b**, such as by using a biocompatible adhesive, clips, barbs, or another type of

fastening means. In some embodiments, elastic covering **140** simply elastically surrounds retractor blades **132a** and **132b**.

Elastic covering **140** can be comprised of various materials. For example, in some embodiments elastic covering **140** can be made of materials including, but not limited to, polypropylene, natural latex, polyester, spandex, silicone, and the like. In some embodiments, elastic covering **140** can comprise nitinol. In some embodiments, a combination of such materials can be used to make elastic covering **140**. The materials used to make elastic covering **140** can be knitted, woven, spun, extruded, molded, and the like. In some embodiments, elastic covering **140** is a mesh or netting type of material. In some embodiments, elastic covering **140** is a fabric, sheet, membrane, film, or the like. In particular embodiments, elastic covering **140** can be porous or at least partially porous so as to let fluids pass through some or all portions of elastic covering **140**.

Elastic covering **140** can provide functional benefits for laparoscopic retractor device **100** in some situations. For example, elastic covering **140** can enlarge the area that expandable portion **130** comprises. Accordingly, laparoscopic retractor device **100** with elastic covering **140** can provide additional retraction capabilities as compared to laparoscopic retractor device **100** without elastic covering **140**, in some situations. Additionally, in some situations the use of elastic covering **140** can reduce the likelihood of pinching tissue such as bowels when laparoscopic retractor device **100** with elastic covering **140** is being expanded or retracted, as compared to laparoscopic retractor device **100** without elastic covering **140**.

Referring now to FIGS. 3A-3C, some embodiments of laparoscopic retractor device **100** can include an elastic covering **150** of another type on expandable portion **130**. Elastic covering **150** can be a sleeve of stretchable material that is attached to shaft **120** and that surrounds and conforms to retractor blades **132a** and **132b**.

When retractor blades **132a** and **132b** are in the contracted configuration as shown in FIG. 3A, elastic covering **150** is also contracted such that it snugly conforms to retractor blades **132a** and **132b**. As retractor blades **132a** and **132b** are expanded radially outward from shaft **120**, elastic covering **150** stretches to remain surrounding and conforming to retractor blades **132a** and **132b** (as shown in FIGS. 3B and 3C). In some embodiments, elastic covering **150** is attached to retractor blades **132a** and **132b**, such as by using a biocompatible adhesive, clip, barbs, or another type of fastening means. In some embodiments, elastic covering **150** simply elastically surrounds retractor blades **132a** and **132b**.

Elastic covering **150** can be comprised of the same materials and made using the same construction techniques as elastic covering **140** described above. Additionally, the uses and advantages of elastic covering **150** are analogous to those of elastic covering **140** described above.

Referring now to FIG. 4A, another example laparoscopic retractor device **400** in accordance with some embodiments provided herein includes a handle **410**, a shaft **420**, an expandable portion **430**, and a sheath **440**. Expandable portion **430** is located at a distal end portion **422** of shaft **420** where shaft **420** terminates at a free end. The proximal end of shaft **420** is fixedly coupled to and extending from handle **410**. Sheath **440** is slidably disposed over shaft **420** and expandable portion **430**. As will be explained further below, a shaft linkage **414** is coupled to a sliding actuator knob **412** and to expandable portion **430**.

Laparoscopic retractor device **400** is shown in a contracted configuration. This contracted configuration may be used, for example, when inserting distal portion **422** of

laparoscopic retractor device **400** into an internal space of a patient, and when withdrawing laparoscopic retractor device **400**. In some implementations, distal portion **422** of laparoscopic retractor device **400** is inserted into a patient, while a proximal portion of laparoscopic retractor device **400** remains external to the patient.

In some circumstances, a trocar device is utilized as a portal to provide access to an internal space of the patient, such as the patient's abdominal space. In such cases, distal portion **422** of laparoscopic retractor device **400** can be passed through the trocar. In some such cases, a trocar with an inner diameter of about 1 cm is used, and distal portion **422** of laparoscopic retractor device **400** can be passed therethrough. In other implementations, trocars with other inner diameter sizes are used (and the laparoscopic retractor device **400** can be passed therethrough), such as about 0.7 cm, about 0.8 cm, about 0.9 cm, about 1.1 cm, about 1.2 cm, about 1.3 cm, about 1.4 cm, about 1.5 cm, about 1.6 cm, about 1.7 cm, about 1.8 cm, about 1.9 cm, or about 2.0 cm. Laparoscopic retractor device **400** can be provided in a range of sizes (diameters and lengths), and the suitably sized laparoscopic retractor device **400** can be selected for use in such various implementations. It should be understood that the use of a trocar may not be required in all implementations. In some other implementations, laparoscopic retractor device **400** can be passed through an incision.

Laparoscopic retractor device **400** includes shaft **420**. Shaft **420** can be constructed of the same types of materials as shaft **120** described above. As will be explained further below, shaft **420** includes at least one lumen. Shaft linkage **414** extends from handle **410** to expandable portion **430**, running through the lumen and being slidable therein. In some embodiments, shaft linkage **414** is a solid metallic rod (e.g., stainless steel), or a solid polymeric rod (e.g., TEF-LON, DELRIN, polyurethane, and the like). In other embodiments, a Bowden cable is used for shaft linkage **414**.

In some embodiments, shaft **420** includes more than one lumen. For example, one or more additional lumens can be optionally included in shaft **420** for purposes such as, but not limited to, suction, irrigation, and the like. In some cases, the optional lumen(s) has a diameter of about 5 mm, but other smaller or larger sized lumens can be included in some embodiments.

Laparoscopic retractor device **400** also includes sheath **440**. Sheath **440** includes a hub **442**, and a tube **444** that is attached to and extending from hub **442**. Sheath **440** has a lumen within which at least a portion of shaft **420** and expandable portion **430** can be positioned, as desired, when sheath **440** is positioned at a distal location as shown in FIG. 4A. Sheath **440** can be slid proximally and distally along shaft **420** by a clinician operator. Hub **442** includes buttons **443a-b** that can be depressed to unlock sheath **440** from shaft **420** such that sheath **440** can be slid along shaft **420**. When buttons **443a-b** are released, sheath **440** is locked to shaft **420**. Accordingly, an operator can slide sheath **440** proximally or distally along shaft **420** and then release sheath **440** in a desired location, at which sheath **440** will stay. In other embodiments, buttons **443a-b** can be replaced by other types of mechanisms that are lockable and releasable, such as an eccentric locking ring, a set screw or thumb screw, a friction fitting arrangement, a ratchet and pawl mechanism, a threaded arrangement, and the like.

In some embodiments, sheath **440** is comprised of a metallic material. For example, metallic materials including, but not limited to, stainless steels (e.g., austenitic 316 stainless steel or martensitic 440 and 420 stainless steels), titanium, titanium alloys (e.g., Ti6Al4V), and the like, can

be used for sheath **440**. In other embodiments, sheath **440** can be comprised of a polymeric material. For example, polymeric materials including, but limited to, polyvinyl chloride (PVC), PEBEX, PICOFLEX, TECOFLEX, PTFE, ePTFE, FEP, PEEK, silicone, urethane, polyethylene, polypropylene, and the like, can be used for sheath **440**. In some embodiments, sheath **440** can be malleable.

Referring now to FIGS. **4A-4D**, distal portion **422** of laparoscopic retractor device **400** can be expanded in situ (e.g., after insertion of laparoscopic retractor device **400** into the patient) to facilitate the retraction of internal tissue, such as the patient's intestines in the case of an intra-abdominal implementation. Such expansion of distal portion **422** is depicted in FIGS. **4B** (partial expansion), **4C** (nearly full expansion), and **4D** (full expansion).

Laparoscopic retractor device **400** also includes handle **410**. Handle **410** can be comprised of any suitable polymeric material such as, but not limited to, polymethyl methacrylate, polystyrene, acrylonitrile butadiene styrene (ABS), PVC, polyethylene, polypropylene, polycarbonate, and the like. Handle **410** can include a textured or contoured surface so that a clinician can get a good grip on handle **410**.

Handle **410** includes sliding actuator knob **412**. Sliding actuator knob **412** can be used by an operator of laparoscopic retractor device **400** to expand or retract expandable portion **430**. That is, in some embodiments sliding actuator knob **412** can be depressed and slid distally or proximally in relation to handle **410**. Such sliding of sliding actuator knob **412** can expand or retract expandable portion **430** because of shaft linkage **414** therebetween. Sliding actuator knob **412** can lock in place on the handle when the operator is no longer depressing sliding actuator knob **412**. In other embodiments, other types of actuators can be used as alternatives to sliding actuator knob **412**. For example, a rotary actuator, a level, a trigger, and other types of actuators can be used in some embodiments.

Laparoscopic retractor device **400** also includes expandable portion **430**. Expandable portion **430** includes retractor blades **432a** and **432b** that are movably coupled to shaft **420** and shaft linkage **414**. Using such a mechanical arrangement, retractor blades **432a** and **432b** can be moved radially inward and outward from shaft **420** by moving sliding actuator knob **412** along handle **410**.

The retractor blades **432a** and **432b** can be metallic or polymeric. For example, in some embodiments retractor blades **432a** and **432b** can be made of metals such as, but not limited to, stainless steels, titanium, titanium alloys, NiTi, and the like. In some embodiments, retractor blades **432a** and **432b** can be made of polymers such as, but not limited to, DELRIN, TEFLON, graphite, nylon, silicone, polyurethane, polyethylene, polypropylene, and the like. In some embodiments, a combination of metallic and polymeric materials can be used to construct retractor blades **432a** and **432b**.

Retractor blades **432a-b** are slender, and very flexible and resilient in bending. Accordingly, retractor blades **432a-b** can be moved radially outward from shaft **420** and radially inward toward shaft **420** by compressing and uncompressing retractor blades **432a-b** by the linear action of shaft linkage **414**.

In FIG. **4B**, sheath **440** has been slid proximally so as to reveal expandable portion **430**. Retractor blades **432a-b** are visible but generally laying close to shaft **420** in a contracted configuration.

In FIG. **4C**, sliding actuator knob **412** has been slid distally along handle **410**. Accordingly, shaft linkage **414** translates distally in coordination with movement of sliding

actuator knob **412**. The distal end of shaft linkage **414** being coupled to retractor blades **432a-b**, as shaft linkage **414** translates distally retractor blades **432a-b** become extended from shaft **420**. In this expanded configuration, laparoscopic retractor device **400** can be used for retraction.

In FIG. **4D**, sheath **440** has been slid distally along shaft **420**. Accordingly, retractor blades **432a-b** are reshaped to a flatter but wider arrangement. During this step, sliding actuator knob **412** may also be moved further distally if so desired. It should be understood from the description herein, that an operator can configure retractor blades **432a-b** in a variety of distinct shapes or configurations by moving sliding actuator knob **412** and sheath **440** in various positions to create the shape of retractor blades **432a-b** as desired.

Retractor blades **432a-b** can be expanded and retracted with little risk of impinging tissue, such as the bowels in the case of intra-abdominal use. This feature can be advantageous for patient safety and ease of use for laparoscopic retractor device **400**.

Referring now to FIGS. **5A-5D**, laparoscopic retractor device **400** can include an elastic covering **450** on expandable portion **430**. Elastic covering **450** can be a sleeve of stretchable material that surrounds and conforms to retractor blades **432a** and **432b**.

When expandable portion **430** is in the contracted configuration as shown in FIG. **5A**, elastic covering **450** is also contracted such that it snugly conforms to retractor blades **432a** and **432b** (inside of elastic covering **450**). As retractor blades **432a** and **432b** are expanded radially outward from shaft **420**, elastic covering **450** stretches to remain surrounding and conforming to retractor blades **432a** and **432b** (as shown in FIGS. **5C** and **5D**). In some embodiments, elastic covering **450** is attached to retractor blades **432a** and **432b**, such as by using a biocompatible adhesive, clips, barbs, or another type of fastening means. In some embodiments, elastic covering **450** simply elastically surrounds retractor blades **432a** and **432b**.

Elastic covering **450** can be comprised of various materials. For example, in some embodiments elastic covering **450** can be made of materials including, but not limited to, polypropylene, natural latex, polyester, Spandex, silicone, and the like. In some embodiments, elastic covering **450** can comprise nitinol. In some embodiments, a combination of such materials can be used to make elastic covering **450**. The materials used to make elastic covering **450** can be knitted, woven, spun, extruded, molded, and the like. In some embodiments, elastic covering **450** is a mesh or netting type of material. In some embodiments, elastic covering **450** is a fabric, sheet, membrane, film, or the like. In particular embodiments, elastic covering **450** can be porous or at least partially porous so as to let fluids pass through some or all portions of elastic covering **450**.

Elastic covering **450** can provide functional benefits for laparoscopic retractor device **400** in some situations. For example, elastic covering **450** can enlarge the area that expandable portion **430** comprises. Accordingly, laparoscopic retractor device **400** with elastic covering **450** can provide additional retraction capabilities as compared to laparoscopic retractor device **400** without elastic covering **450**, in some situations. Additionally, in some situations the use of elastic covering **450** can reduce the likelihood of pinching tissue such as bowels when laparoscopic retractor device **400** with elastic covering **450** is being expanded or retracted, as compared to laparoscopic retractor device **400** without elastic covering **450**.

While this specification contains many specific implementation details, these should not be construed as limitations on the scope of any invention or of what may be claimed, but rather as descriptions of features that may be specific to particular embodiments of particular inventions. Certain features that are described in this specification in the context of separate embodiments can also be implemented in combination in a single embodiment. Conversely, various features that are described in the context of a single embodiment can also be implemented in multiple embodiments separately or in any suitable subcombination. Moreover, although features may be described herein as acting in certain combinations and even initially claimed as such, one or more features from a claimed combination can in some cases be excised from the combination, and the claimed combination may be directed to a subcombination or variation of a subcombination.

Similarly, while operations are depicted in the drawings in a particular order, this should not be understood as requiring that such operations be performed in the particular order shown or in sequential order, or that all illustrated operations be performed, to achieve desirable results. In certain circumstances, multitasking and parallel processing may be advantageous. Moreover, the separation of various system modules and components in the embodiments described herein should not be understood as requiring such separation in all embodiments, and it should be understood that the described program components and systems can generally be integrated together in a single product or packaged into multiple products.

Particular embodiments of the subject matter have been described. Other embodiments are within the scope of the following claims. For example, the actions recited in the claims can be performed in a different order and still achieve desirable results. As one example, the processes depicted in the accompanying figures do not necessarily require the particular order shown, or sequential order, to achieve desirable results. In certain implementations, multitasking and parallel processing may be advantageous.

What is claimed is:

1. A laparoscopic retractor device comprising:

a handle;

an elongate shaft with a proximal end portion that is attached to the handle, the shaft extending from the handle and terminating at a distal free end portion, the shaft defining a first lumen;

an elongate shaft linkage disposed within the first lumen, the shaft linkage having a proximal end and a distal end;

a first actuator located at the handle and coupled to the proximal end of the shaft linkage;

an expandable portion including: (i) a distal end portion coupled to the distal free end portion of the shaft and (ii) a proximal end portion coupled to the distal end of the shaft linkage, wherein moving the actuator causes the expandable portion to move radially outward from the shaft or radially inward toward the shaft; and

a sheath with a lumen therethrough, at least a portion of the shaft being disposed within the lumen, the sheath being slidable distally and proximally along the shaft.

2. The laparoscopic retractor device of claim 1, wherein the sheath includes a hub that is connected to a proximal end of the sheath, and wherein the hub includes a second actuator whereby the hub can be locked and unlocked from being coupled to the shaft.

3. The laparoscopic retractor device of claim 2, wherein the second actuator whereby the hub can be locked and unlocked from being coupled to the shaft is at least one of a button, an eccentric locking ring, a set screw, a thumb screw, a friction fitting arrangement, a ratchet and pawl mechanism, and a threaded arrangement.

4. The laparoscopic retractor device of claim 1, wherein the first actuator is slidable in relation to the handle.

5. The laparoscopic retractor device of claim 4, wherein sliding the first actuator distally causes the expandable portion to expand, and wherein sliding the first actuator proximally causes the expandable portion to contract.

6. The laparoscopic retractor device of claim 4, the first actuator comprising a knob, wherein the first actuator is locked into place when the knob is released.

7. The laparoscopic retractor device of claim 1, wherein the expandable portion comprises at least two retractor blades.

8. The laparoscopic retractor device of claim 7, wherein causing the expandable portion to expand comprises causing the at least two retractor blades to bend and to move radially outward from the shaft, and wherein causing the expandable portion to contract comprises causing the at least two retractor blades unbend and to move radially inward toward the shaft.

9. The laparoscopic retractor device of claim 8, wherein by sliding the sheath distally at least some portion of the at least two retractor blades can be made to move further radially away from the shaft.

10. The laparoscopic retractor device of claim 8, wherein by sliding the sheath proximally at least some portion of the at least two retractor blades can be made to move further radially inward toward the shaft.

11. The laparoscopic retractor device of claim 10, further comprising an elastic covering that is disposed around the at least two retractor blades.

12. The laparoscopic retractor device of claim 11, wherein the elastic covering is attached to the retractor blades via at least one of adhesive, clops, and barbs.

13. The laparoscopic retractor device of claim 1, further comprising an elastic covering that is disposed around the expandable portion.

14. The laparoscopic retractor device of claim 13, wherein the elastic covering is attached to the retractor blades via at least one of adhesive, clops, and barbs.

15. The laparoscopic retractor device of claim 1, wherein the first actuator is at least one of a rotary actuator, a lever, and a trigger.

16. The laparoscopic retractor device of claim 1, wherein the handle comprises at least one of a textured surface and a contoured surface.

17. The laparoscopic retractor device of claim 1, wherein the shaft defines a second lumen for at least one of suction and irrigation.

* * * * *

专利名称(译)	腹腔镜牵开器装置		
公开(公告)号	US10136881	公开(公告)日	2018-11-27
申请号	US14/614616	申请日	2015-02-05
[标]申请(专利权)人(译)	梅约医学教育与研究基金会		
申请(专利权)人(译)	梅奥基金会的医学教育和研究		
当前申请(专利权)人(译)	梅奥基金会的医学教育和研究		
[标]发明人	MARIANI ANDREA		
发明人	MARIANI, ANDREA		
IPC分类号	A61B1/32 A61B17/02		
CPC分类号	A61B17/0218		
代理机构(译)	FISH & RICHARDSON P.C.		
优先权	61/938234 2014-02-11 US		
其他公开文献	US20150223795A1		
外部链接	Espacenet		

摘要(译)

本文提供了用于执行诸如腹腔镜手术的医疗程序的装置。例如，该文献提供了腹腔镜牵开器装置。在一些实施例中，本文提供的腹腔镜牵开器装置包括两个可伸展或收缩的牵开器刀片。此外，在一些实施例中，包括弹性覆盖物，并且牵开器叶片设置在弹性覆盖物内。

