



US010368905B2

(12) **United States Patent**
Rosenbaum et al.

(10) **Patent No.:** **US 10,368,905 B2**
(45) **Date of Patent:** **Aug. 6, 2019**

(54) **TROCAR ASSEMBLY WITH A CLEANING ELEMENT FOR USE DURING A LAPAROSCOPIC PROCEDURE**

(71) Applicant: **CareFusion 2200, Inc.**, San Diego, CA (US)

(72) Inventors: **Joanna L. Rosenbaum**, Evanston, IL (US); **Jeanny Chung**, Deerfield, IL (US); **Patrick Hubbard**, Vernon Hills, IL (US); **Joseph Prybell**, Mundelein, IL (US); **Corrie Threlkeld**, Vernon Hills, IL (US); **Sara Tillman**, Vernon Hills, IL (US); **Brandon Toth**, Vernon Hills, IL (US); **Andrew P. VanDeWeghe**, Grayslake, IL (US); **Thomas Wilschke**, Chicago, IL (US); **Jesse Charles Darley**, Madison, WI (US); **Christopher Alan Harris**, Madison, WI (US); **Curtis B. Irwin**, Madison, IL (US); **Stephen A. Latham**, Sun Prairie, WI (US); **Daniel J. Lee**, Princeton Junction, NJ (US); **Douglas Rodenkirch**, Sun Prairie, WI (US); **Jeffrey R. Staszak**, Deerfield, WI (US)

(73) Assignee: **Carefusion 2200, Inc.**, San Diego, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) Appl. No.: **15/452,211**

(22) Filed: **Mar. 7, 2017**

(65) **Prior Publication Data**

US 2018/0256203 A1 Sep. 13, 2018

(51) **Int. Cl.**
A61B 17/34 (2006.01)
A61B 1/12 (2006.01)

(Continued)

(52) **U.S. Cl.**
CPC **A61B 17/3415** (2013.01); **A61B 1/00154** (2013.01); **A61B 1/126** (2013.01);
(Continued)

(58) **Field of Classification Search**
CPC **A61B 90/70**; **A61B 1/00154**; **A61B 1/122**; **A61B 1/3132**; **A61B 17/0218**;
(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,274,874 A 1/1994 Cercone et al.
5,351,675 A 10/1994 Brodsky
(Continued)

FOREIGN PATENT DOCUMENTS

EP 2111782 A2 10/2009
EP 2111808 A2 10/2009
(Continued)

OTHER PUBLICATIONS

International Search Report and Written Opinion in Application No. PCT/US2018/020850, dated May 17, 2018, 12 pages.
(Continued)

Primary Examiner — Pedro Philogene


Assistant Examiner — David C Comstock

(74) *Attorney, Agent, or Firm* — Dinsmore & Shohl LLP

(57) **ABSTRACT**

The present disclosure relates to a housing for a laparoscopic trocar assembly with an integrated scope-cleaning structure. The housing may include a shell forming a wall portion of a chamber and a cleaning element forming at least a portion of an internal surface of the chamber, the cleaning element configured to remove debris from a distal end of a scope upon contact between the cleaning element and the distal end of the scope. The cleaning element may be movable with respect to the shell of the housing in response to an input force upon the shell that moves a portion of the shell and a

(Continued)

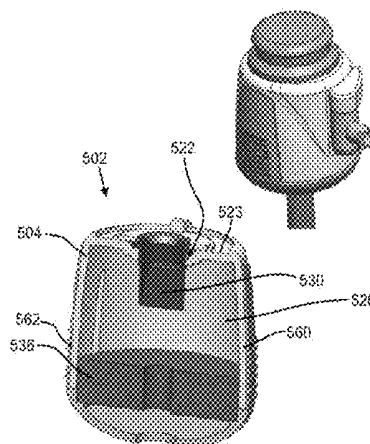

portion of the cleaning element between a default state and a displaced state.

20 Claims, 12 Drawing Sheets

- (51) **Int. Cl.**
A61B 1/00 (2006.01)
A61B 1/313 (2006.01)
- (52) **U.S. Cl.**
 CPC **A61B 1/3132** (2013.01); **A61B 17/34** (2013.01); **A61B 17/3462** (2013.01); **A61B 17/3474** (2013.01); **A61B 2017/3437** (2013.01)
- (58) **Field of Classification Search**
 CPC A61B 17/3423; A61B 2090/701; A61B 2017/00367; A61L 317/0218; A61L 317/3423
 USPC 600/204, 206, 184, 188, 127, 157
 See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

5,365,267	A	11/1994	Edwards
5,382,297	A	1/1995	Valentine et al.
5,549,543	A	8/1996	Kim
5,643,227	A	7/1997	Stevens
5,651,757	A	7/1997	Meckstroth
5,842,971	A	12/1998	Yoon
5,880,779	A	3/1999	Rhynes
5,910,106	A	6/1999	Morgan et al.
5,916,145	A	6/1999	Chu et al.
5,980,493	A	11/1999	Smith et al.
6,197,041	B1	3/2001	Schichman et al.
6,319,266	B1	11/2001	Stellon et al.
6,482,181	B1	11/2002	Racenet et al.
6,497,716	B1	12/2002	Green et al.
6,685,630	B2	2/2004	Sauer et al.
6,976,957	B1 *	12/2005	Chin A61B 1/313 600/157
6,981,966	B2	1/2006	Green et al.
7,025,747	B2	4/2006	Smith
7,294,136	B2	11/2007	Dubruil et al.
7,367,960	B2	5/2008	Stellon et al.
7,390,315	B2	6/2008	Stellon et al.
7,537,563	B2	5/2009	Temple
7,691,089	B2	4/2010	Gresham
7,771,384	B2	8/2010	Ravo
7,811,225	B2	10/2010	Sauer et al.
7,811,251	B2	10/2010	Wenchell et al.
7,988,670	B2	8/2011	Smith
8,070,730	B2	12/2011	Rockrohr
8,092,423	B2	1/2012	Gresham
8,123,682	B2	2/2012	Wenchell et al.
8,152,717	B2	4/2012	Gomez
8,202,290	B2	6/2012	Smith
8,206,411	B2	6/2012	Thompson et al.
8,211,135	B2	7/2012	Heinrich et al.
8,223,193	B2	7/2012	Zhao et al.
8,241,251	B2	8/2012	Gresham
8,257,253	B2	9/2012	Piskun
8,257,254	B2	9/2012	Piskun
8,257,315	B2	9/2012	Franer et al.
8,267,896	B2 *	9/2012	Hartoumbekis A61B 1/126 604/167.01
8,394,018	B2	3/2013	Piskun
8,449,460	B2	5/2013	Duke et al.
8,458,971	B2	7/2013	Smith et al.
8,491,545	B2	7/2013	Shelton, IV
8,496,622	B2	7/2013	Shelton, IV

8,535,220	B2	9/2013	Mondschein
D700,326	S	2/2014	Minnelli et al.
8,708,889	B2	4/2014	Feuer et al.
8,726,037	B2	5/2014	Franer
8,728,109	B2	5/2014	Piskun
8,764,648	B2	7/2014	Piskun
8,771,307	B2	7/2014	Franer
8,870,747	B2	10/2014	Moreno, Jr. et al.
8,911,463	B2	12/2014	Fischvogt
8,932,249	B2	1/2015	Parihar et al.
8,961,552	B2	2/2015	Fischvogt et al.
8,968,250	B2	3/2015	McGinley et al.
9,039,604	B2	5/2015	Yoshida
9,078,562	B2	7/2015	Poll et al.
D736,926	S	8/2015	Minnelli et al.
9,211,059	B2	12/2015	Drach et al.
9,265,899	B2	2/2016	Albrecht et al.
9,289,115	B2	3/2016	Dang et al.
D753,303	S	4/2016	Dannaher
9,314,266	B2	4/2016	Kahle et al.
9,314,267	B2	4/2016	Piskun et al.
9,358,040	B2	6/2016	Kahle et al.
2002/0022762	A1	2/2002	Beane et al.
2005/0043683	A1	2/2005	Ravo
2006/0293559	A1 *	12/2006	Grice, III A61B 1/00135 600/102
2008/0194915	A1	8/2008	Blackhurst et al.
2008/0200765	A1	8/2008	Mondschein
2009/0112057	A1	4/2009	Kammer et al.
2009/0240111	A1 *	9/2009	Kessler A61B 1/00032 600/155
2009/0270686	A1	10/2009	Duke et al.
2010/0012152	A1	1/2010	Hansen
2011/0149057	A1	6/2011	Beck et al.
2012/0101337	A1	4/2012	Clark et al.
2012/0187104	A1	7/2012	Heymann et al.
2013/0041230	A1	2/2013	Hartoumbekis et al.
2013/0053639	A1 *	2/2013	Ihde, II A61B 1/04 600/109
2013/0085329	A1	4/2013	Morrisette et al.
2013/0102843	A1	4/2013	Feuer et al.
2013/0150670	A1	6/2013	O'Prey et al.
2014/0171739	A1	6/2014	Nguyen
2014/0215736	A1 *	8/2014	Gomez A61B 1/00154 15/104.05
2014/0235944	A1	8/2014	Feuer et al.
2014/0249370	A1 *	9/2014	Hurst A61B 1/126 600/114
2016/0015573	A1 *	1/2016	Ihde, II A61B 90/70 604/385.01
2016/0113484	A1	4/2016	Nakaguchi
2016/0166135	A1	6/2016	Fiset
2018/0035988	A1 *	2/2018	Lau A61B 17/00008


FOREIGN PATENT DOCUMENTS


EP	2113215	A1	11/2009
EP	2193742	A1	6/2010
EP	2238928	A1	10/2010
EP	2111782	B1	8/2016
WO	WO2010/011563	A2	7/2009
WO	WO2010/011563	A3	7/2009
WO	WO2013/012790	A2	7/2012
WO	WO2013/012790	A3	7/2012
WO	WO2013/063153	A2	5/2013
WO	WO2014/185334	A1	5/2014


OTHER PUBLICATIONS

International Search Report and Written Opinion in Application No. PCT/US2018/020856, dated May 17, 2018, 15 pages.
 International Search Report and Written Opinion in Application No. PCT/US2018/020853, dated Jun. 18, 2018, 16 pages.

* cited by examiner

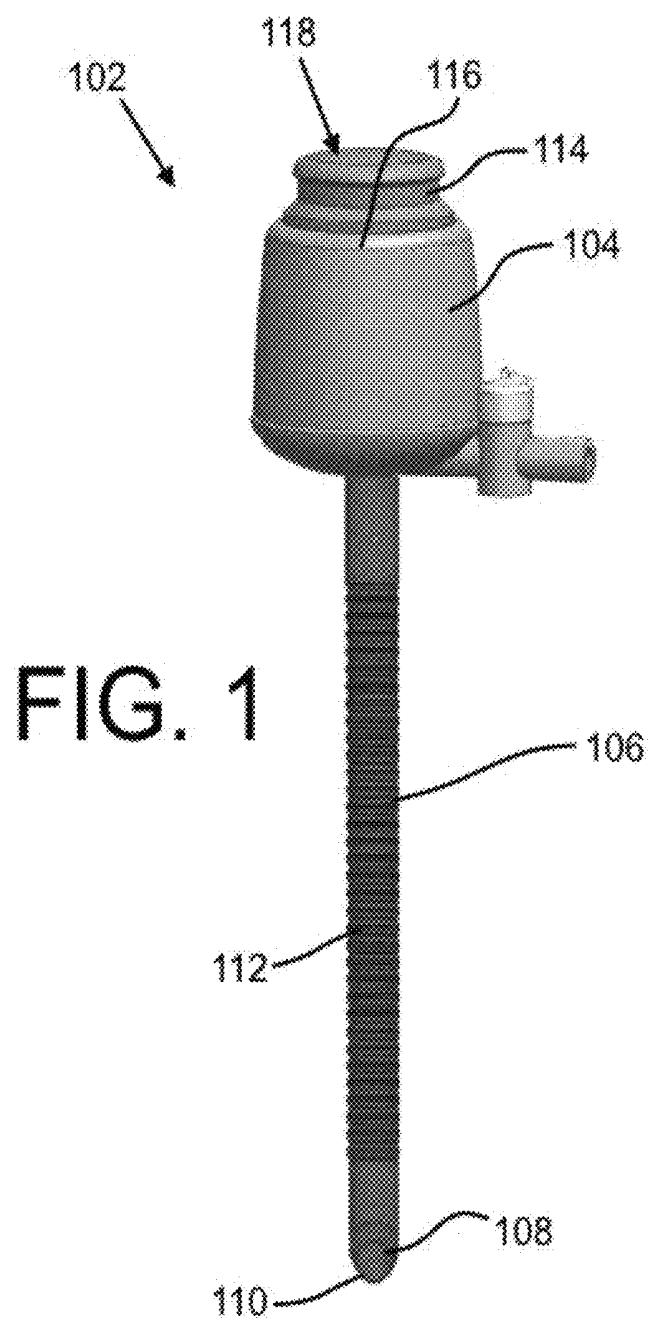

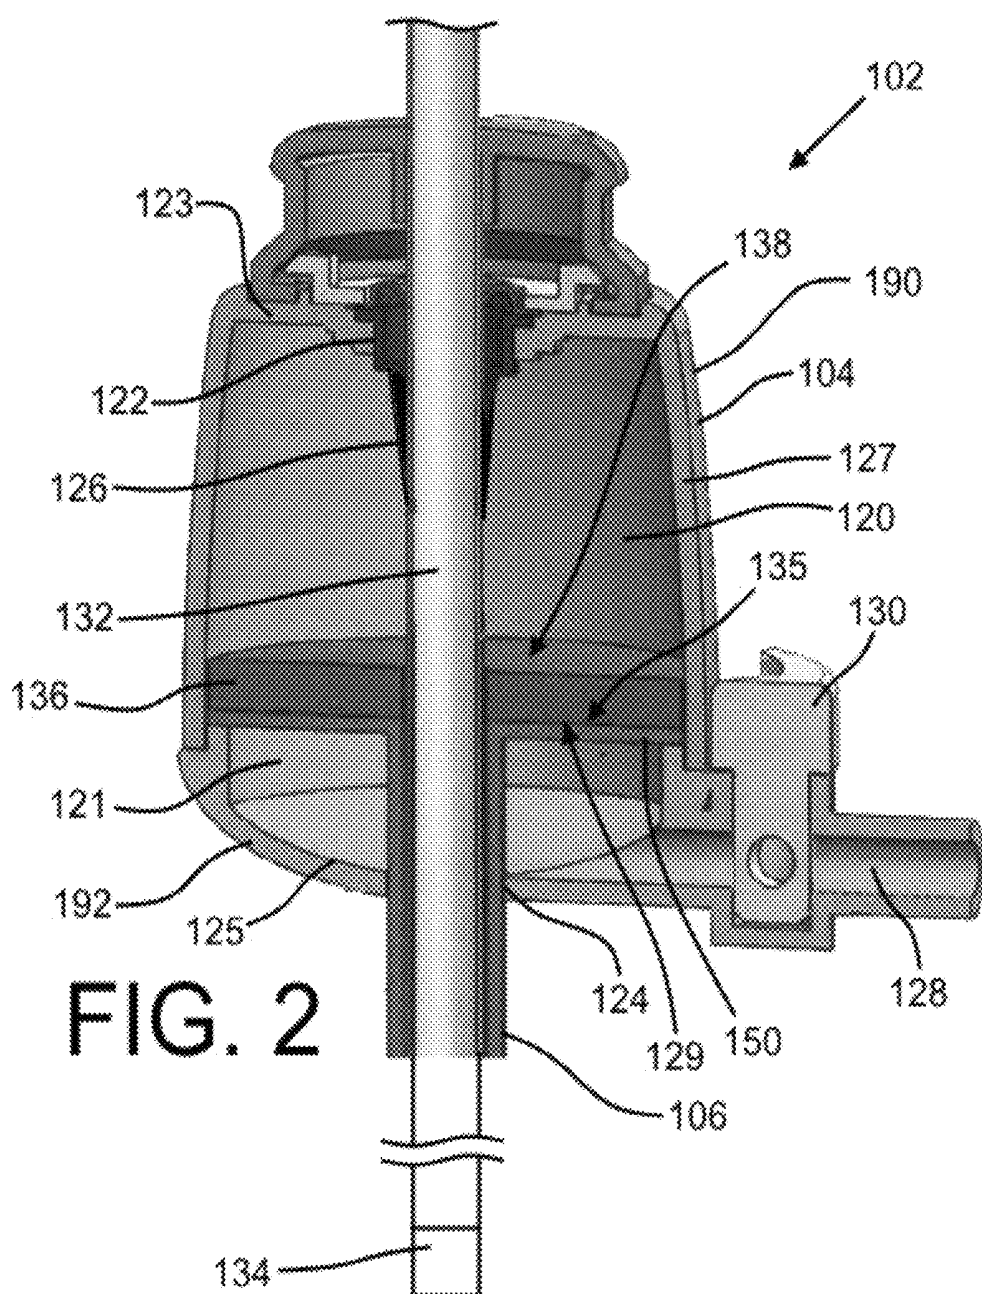

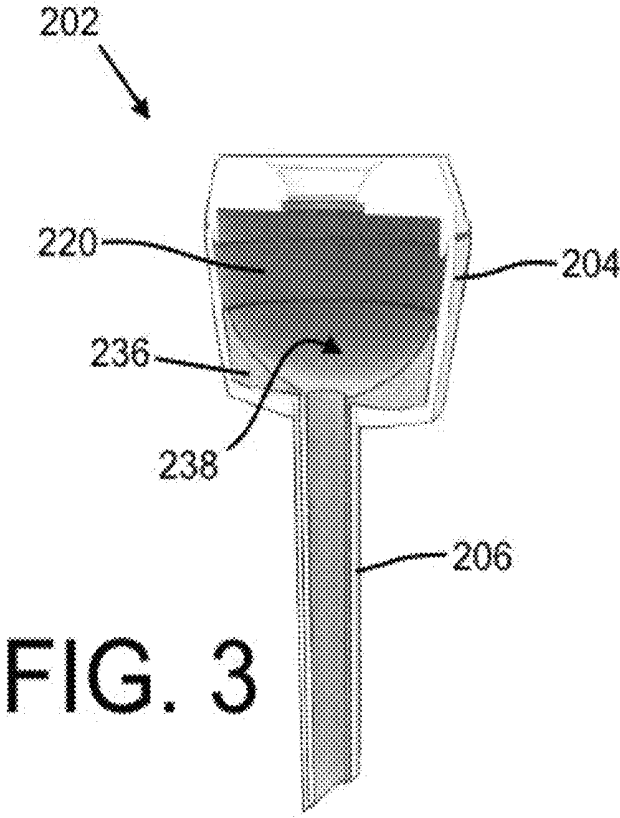

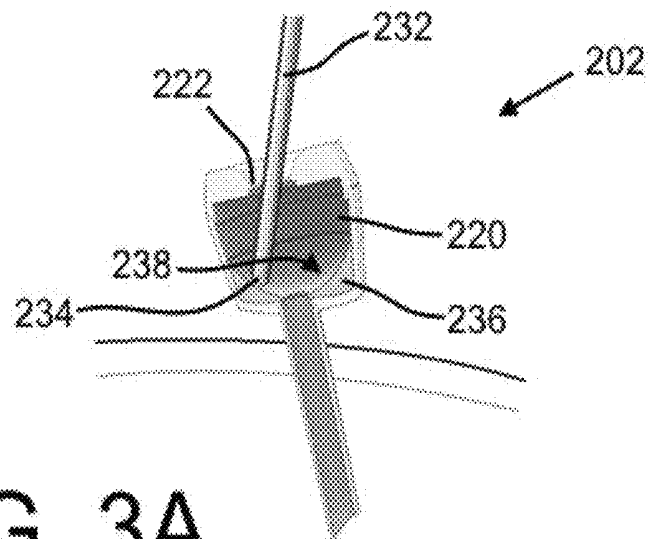


FIG. 3A

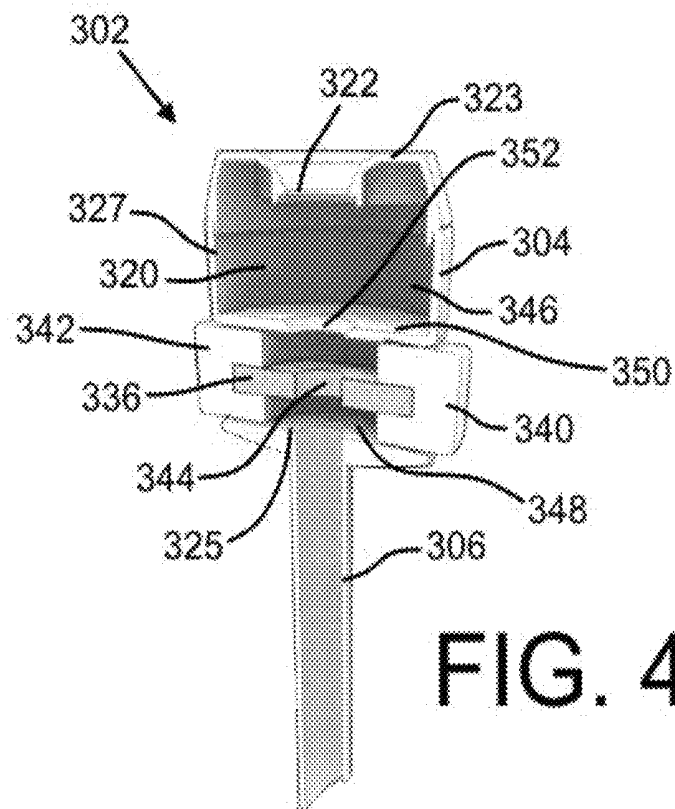


FIG. 4

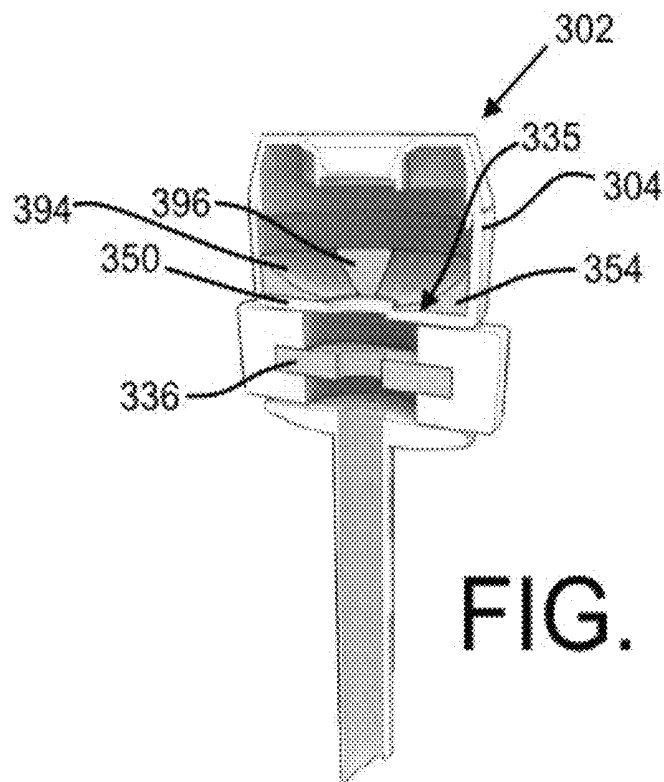
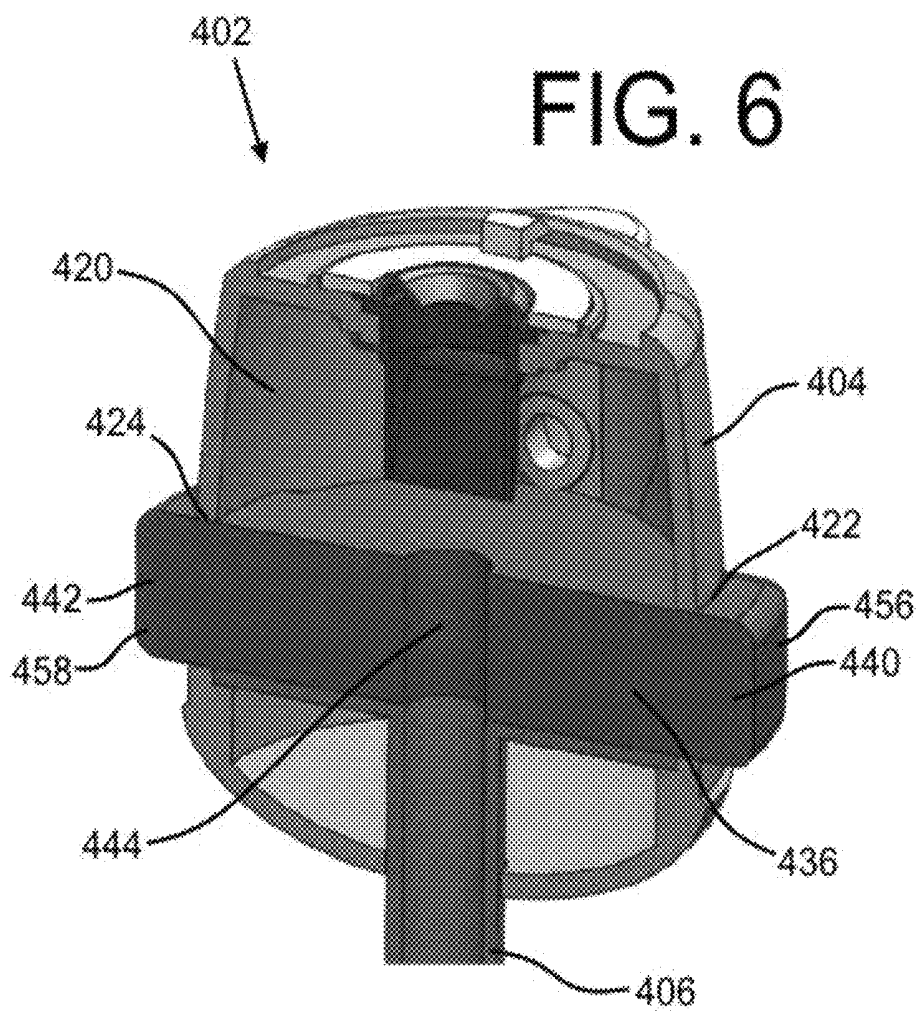


FIG. 5

FIG. 6



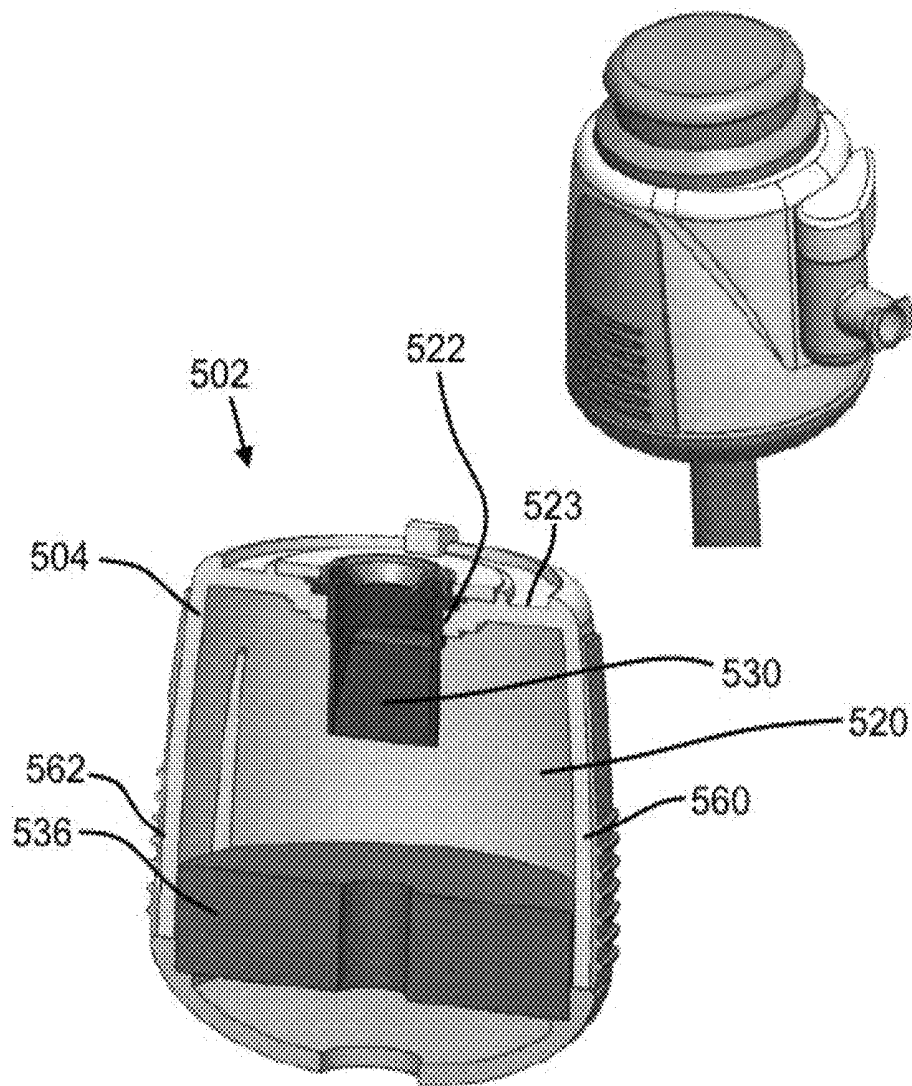
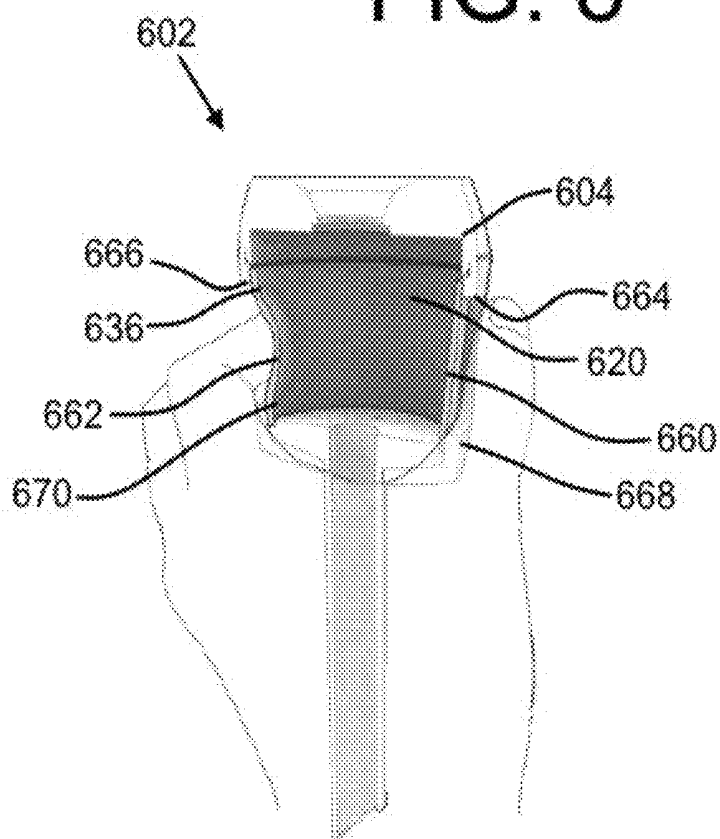


FIG. 7

FIG. 8





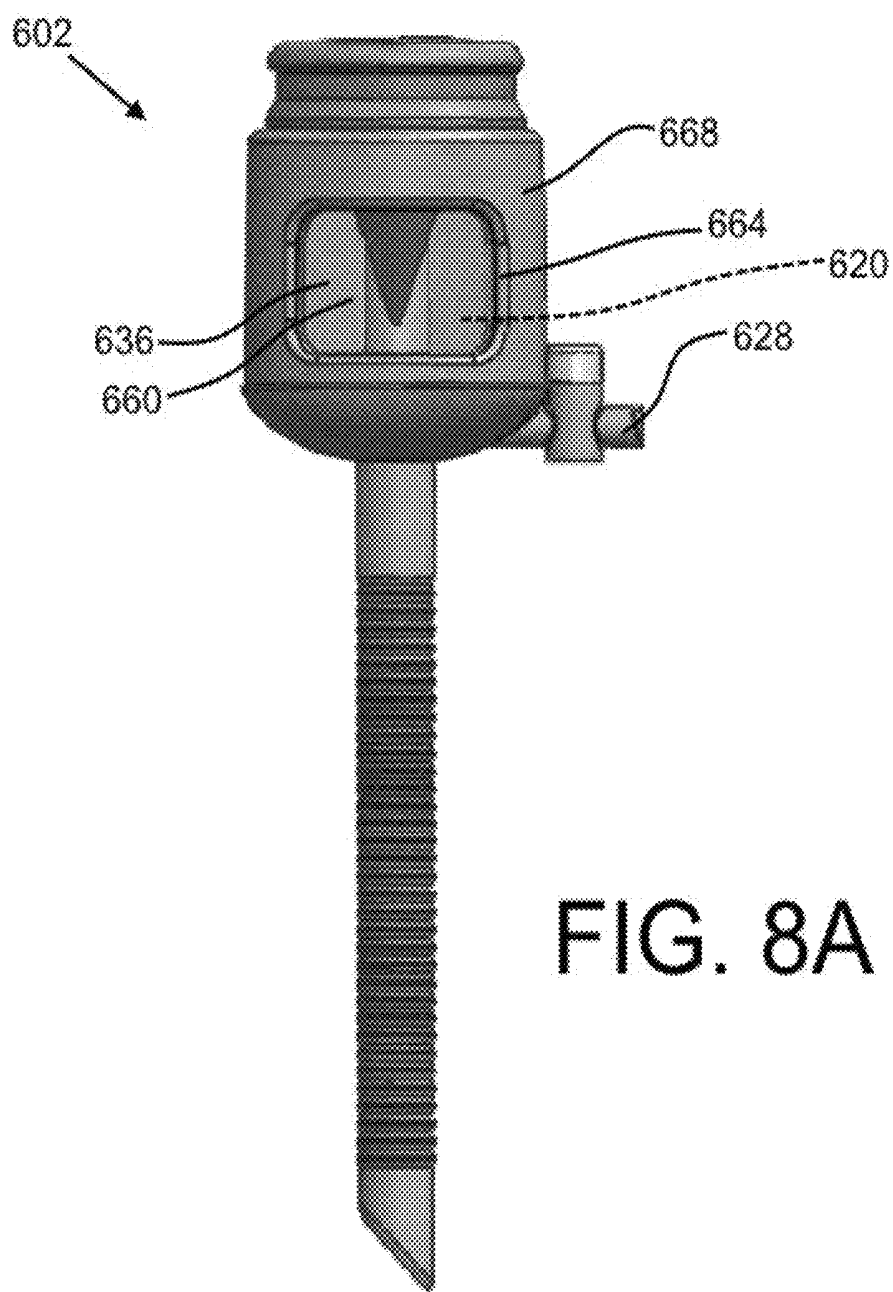


FIG. 8A

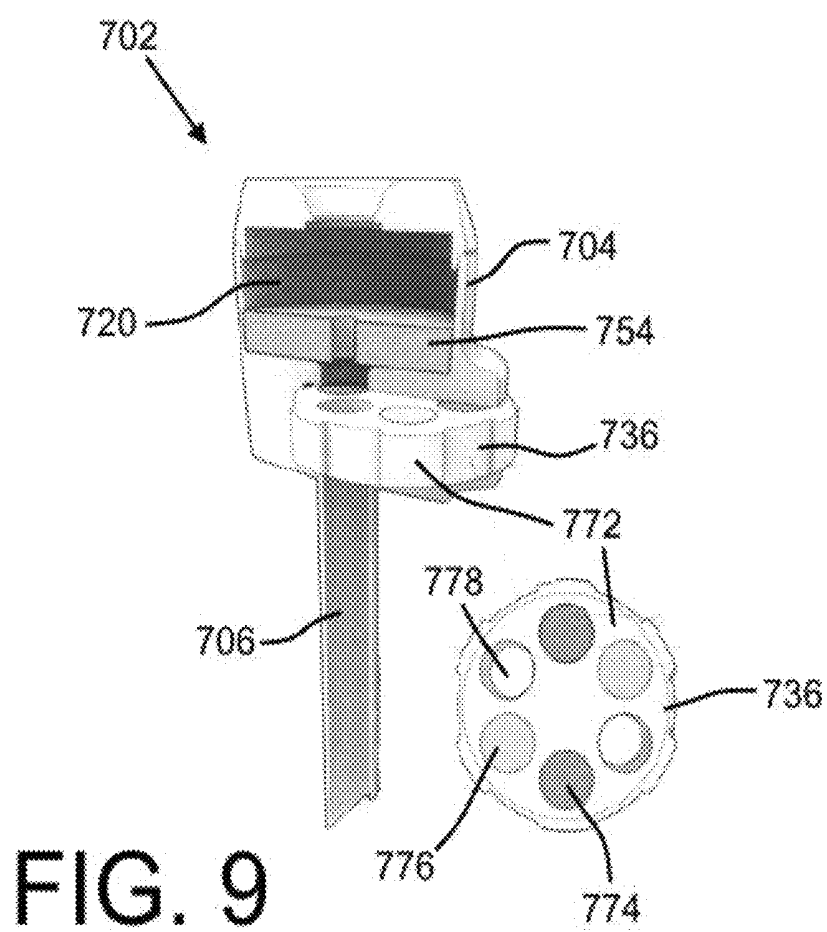

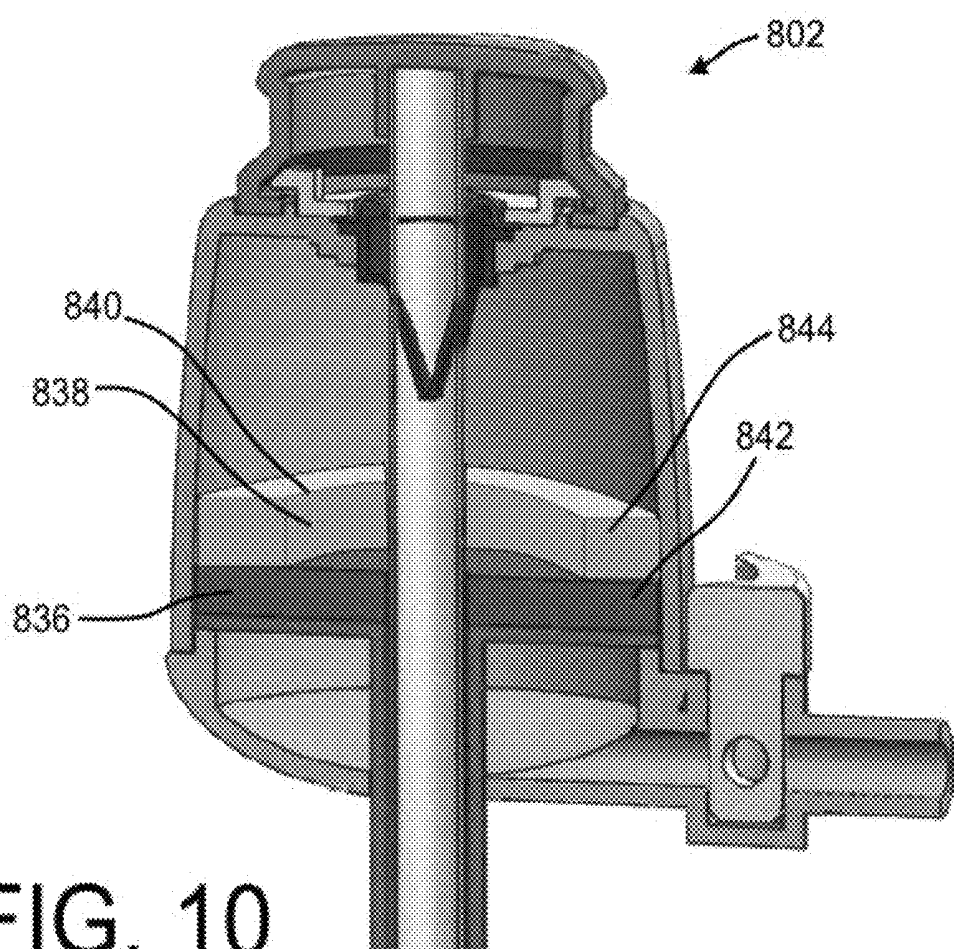

1

TROCAR ASSEMBLY WITH A CLEANING ELEMENT FOR USE DURING A LAPAROSCOPIC PROCEDURE

FIELD OF TECHNOLOGY

The present disclosure relates generally to trocar assemblies and related devices, and more specifically, to trocar assemblies which can be utilized in laparoscopic medical procedures.

BACKGROUND

Laparoscopic surgery is a minimally-invasive surgical technique typically performed with the assistance of one or more medical instruments inserted through a small incision in a patient's body. Laparoscopic surgery is often preferred to traditional and more invasive surgical procedures because of the reduced frequency and degree of certain postoperative side effects, such as postoperative pain, swelling, internal bleeding, and infection risk. The minimally-invasive nature of laparoscopic procedures may also result in decreased recovery times and shorter hospital stays.

Typical medical devices utilized during laparoscopic procedures have instruments mounted on an elongated metal or plastic body that are inserted into the patient's body and maneuvered to a target area within a body cavity (e.g., the abdominal, pelvic, thoracic, or chest cavity, where insufflation may be used to provide additional space in which to maneuver, which requires a fluid-patent barrier to maintain insufflation pressure in the cavity). One or more trocar assemblies are typically first inserted into the patient body at an incision site (for each), and the instruments access the patient body through the trocar assembly(ies).

Often, a medical device including a camera or other image-transmitting device is inserted through a trocar to transmit one or more images or a live video feed from within the body cavity to a medical professional (such as the surgeon). The device may be referred to as a scope or a laparoscope, and its transmission may guide the medical professional's actions during the laparoscopic procedure.

A problem typically experienced during laparoscopic procedures involves a compromised image or video feed due to an obstructed lens of the laparoscope. This obstruction may be caused by condensation (e.g., fog) and/or debris such as bodily fluids or displaced tissue encountered by the lens during the procedure. Such obstruction is problematic because the lens of the laparoscope preferably remains contained in a pressurized and sterile environment (e.g., insufflated body cavity), and removing the lens from that environment for cleaning purposes may cause lengthy interruptions prolonging patient anesthesia and increasing a risk of compromised sterility.

DESCRIPTION

In one aspect, the present disclosure relates to a housing for a laparoscopic trocar assembly with an integrated scope-cleaning structure. The housing may include a shell forming a wall portion of a chamber and a cleaning element forming at least a portion of an internal surface of the chamber, the cleaning element configured to remove debris from a distal end of a scope upon contact between the cleaning element and the distal end of the scope. The cleaning element may be movable with respect to the shell of the housing in response

2

to an input force upon the shell that moves a portion of the shell and a portion of the cleaning element between a default state and a displaced state.

The housing may include an external surface at least partially formed by the shell, where an external facing surface of the cleaning element forms at least a portion of the external surface of the housing.

The cleaning element may be formed of a resilient material such that the cleaning element includes a tendency to assume the default state in the absence of an input force, and where the default state forms an external shape that is generally continuous with the shell, or that extends from the shell in a visually-contrasting manner.

At least one button may be coupled to the cleaning element, where the input force is applied to the at least one button, and where the at least one button is movable with respect to the chamber in response to the input force. The cleaning element may include a stepped portion with an edge.

The cleaning element may include an opening longitudinally aligned with a longitudinal axis of a cannula, the cannula extending distally from the housing when the cleaning element is in the default state. A divider may separate the chamber into a proximal portion and a distal portion, the divider including an opening aligned with the opening of the cleaning element. The divider may include a second cleaning element located in the proximal portion of the chamber. The second cleaning element may include a curved concave proximal-facing surface.

In another aspect, the present disclosure provides a housing for a laparoscopic trocar assembly with an integrated scope-cleaning structure with an outer shell having a proximal entry opening through a proximal wall, a distal exit opening to a trocar lumen through a distal wall, and a generally cylindrical wall therebetween, the generally cylindrical wall circumferentially defining a chamber and being deformable. An inner surface of the generally cylindrical wall may have at least one cleaning element with a cleaning surface within the chamber, the cleaning surface configured to contact and to remove debris from at least a viewing element of a scope when the generally cylindrical wall is deformed and the at least a viewing element is within the chamber.

The outer shell proximal entry opening may form a fluid-patent seal around a scope directed therethrough. The cleaning surface may be formed by a more-flexible wall portion of the generally cylindrical wall, immediately adjacent a less-flexible outermost periphery of the proximal wall of the outer shell, the more-flexible wall portion configured to displace inwards with respect to the chamber in response to an input force directed toward a central region of the generally cylindrical wall.

The cleaning surface may be formed of a compliant material continuous with the generally cylindrical wall.

The cleaning element may form at least a portion of an inner-facing longitudinal and circumferential surface of the housing.

The cleaning element may be movable with respect to the outer shell of the housing in response to an input force between a generally cylindrical default state and a displaced state. The cleaning element may be formed of a resilient material such that the cleaning element includes a tendency to assume the default state in the absence of an input force.

The cleaning element may include a stepped portion with an edge.

In another aspect, the present disclosure provides a method for cleaning a scope. The method may include

maneuvering a distal end of the scope to a location within a chamber of a trocar assembly, the chamber at least partially formed by a shell where a cleaning element has a surface within the chamber, moving the cleaning element from a default state to a displaced state by displacing an external-facing surface of the chamber inwardly, and removing debris from at least a distal-facing surface of the scope moving the scope and in contact with a cleaning element.

Moving the cleaning element may include applying an input force to a button formed by the external-facing surface of the chamber, where the button is coupled to the cleaning element.

The cleaning element may be formed of a resilient material such that the cleaning element includes a tendency to assume the default state in the absence of an input force.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 shows a trocar assembly for use during a laparoscopic procedure in accordance with the present disclosure.

FIG. 2 shows a section view of the trocar assembly of FIG. 1.

FIG. 3 shows another embodiment of a trocar assembly with a curved convex cleaning surface and lined cannula in accordance with the present disclosure.

FIG. 3A shows the trocar assembly of FIG. 3 during a cleaning procedure in accordance with the present disclosure.

FIG. 4 shows a trocar assembly with movable buttons for displacing a cleaning element in response to an input force in accordance with the present disclosure.

FIG. 5 shows the trocar assembly of FIG. 4 with a second cleaning element in accordance with the present disclosure.

FIG. 6 shows another embodiment of a trocar assembly having a cleaning element with portions extending to a location outside of a housing in accordance with the present disclosure.

FIG. 7 shows another embodiment of a trocar assembly with a housing having flexible wall portions in accordance with the present disclosure.

FIG. 8 shows another embodiment of a trocar assembly with flexible wall portions formed by an inner shell including a cleaning element in accordance with the present disclosure.

FIG. 8A shows a second illustration of the trocar assembly of FIG. 8.

FIG. 9 shows another embodiment of a trocar assembly with an adjustable cleaning element in accordance with the present disclosure.

FIG. 10 shows another embodiment of a trocar assembly with disclosure cleaning element having two disk portions.

DETAILED DESCRIPTION

Various embodiments are described below with reference to the drawings in which like elements generally are referred to by like numerals. The relationship and functioning of the various elements of the embodiments may better be understood by reference to the following detailed description. However, embodiments are not limited to those illustrated in the drawings. It should be understood that the drawings may or may not be to scale, and in certain instances details may have been omitted that are not necessary for an understanding of embodiments disclosed herein, such as—for example—conventional fabrication and assembly.

The invention is defined by the claims, may be embodied in many different forms, and should not be construed as

limited to the embodiments set forth herein; rather, these embodiments are provided so that this disclosure will be thorough and complete, and will fully convey enabling disclosure to those skilled in the art. As used in this specification and the claims, the singular forms “a,” “an,” and “the” include plural referents unless the context clearly dictates otherwise. Reference herein to any industry and/or governmental standards (e.g., ASTM, ANSI, IEEE, HIPAA, FDA standards) is defined as complying with the currently published standards as of the original filing date of this disclosure concerning the units, measurements, and testing criteria communicated by those standards unless expressly otherwise defined herein.

The terms “proximal” and “distal” are used herein in the common usage sense where they refer respectively to a handle/doctor-end of a device or related object and a tool/patient-end of a device or related object. The terms “about,” “substantially,” “generally,” and other terms of degree, when used with reference to any volume, dimension, proportion, or other quantitative or qualitative value, are intended to communicate a definite and identifiable value within the standard parameters that would be understood by one of skill in the art (equivalent to a medical device engineer with experience in this field), and should be interpreted to include at least any legal equivalents, minor but functionally-insignificant variants, standard manufacturing tolerances, and including at least mathematically significant figures (although not required to be as broad as the largest range thereof).

FIG. 1 shows a trocar assembly 102 for use during a laparoscopic procedure. The trocar assembly 102 may include a housing 104 with a cannula 106 extending distally from the housing 104. The cannula 106 may include a distal end 108 for placement into a patient body during the laparoscopic procedure. The distal end 108 of the cannula 106 may include a beveled or sharpened end 110 to facilitate entry of the cannula 106 into the patient body. An obturator may additionally or alternatively be included. The cannula 106 may include certain surface characteristics, such as threads or ridges 112, to enhance the stability of the trocar assembly 102 when inserted into a body incision. In some embodiments, a removable bayonet fitting 114 or other suitable securement mechanism may be placed on a proximal side 116 of the housing 104 during deployment of the trocar assembly 102. The bayonet fitting 114 may be configured to secure an obturator to the housing 104 and may provide a surface 118 for receiving an input force from a medical professional intended to direct the cannula 106 into the patient body, for example. The bayonet fitting 114 may be removed once the trocar assembly 102 is deployed.

FIG. 2 shows a section view of the trocar assembly 102 of FIG. 1. As shown, the cannula 106 may be in fluid communication with a chamber 120 formed by the housing 104. The chamber 120 may be defined by a proximal or top wall 123, a distal or bottom wall 125, and a generally cylindrical side wall 327 extending from the top wall 123 to the bottom wall 125 and defining inner and outer chamber perimeters (i.e., circumferences, when the chamber is rounded but otherwise applicable to any geometry). The chamber 120 may have a proximal opening 122 configured to receive medical devices used during laparoscopic surgery, including but not limited to graspers, dissectors, needles, scissors, clamps, electrodes, forceps, a camera or laparoscope (a “scope”), etc. The proximal opening 122 may be located in a top wall 123 of the housing 104. A valve 126 may be located in the proximal opening 122 and may form a seal or fluid barrier between the chamber 120 and an

external environment (e.g., the ambient room environment). Alternatively or in addition, the valve 126 may be located in another location (such as at the opening 124). It may be advantageous for at least one valve 126 to be located at a the proximal opening 122 such that a lens of a scope does not have to pass through the valve 126 prior to cleaning, thereby reducing or eliminating the chance of materials from the valve 126 dirtying the scope's lens. The inner and outer chamber perimeters each is greater than an outer perimeter of the cannula 106.

The chamber 120 may be subjected to a continuous sterile and pressurized environment that extends through the cannula 106 and to the body cavity (herein referred to as the "internal environment" even though the continuous region may extend external of the patient body wall, e.g., within trocar assembly 102). This may be advantageous if maintaining insufflation of the body cavity is desired during all operation—including cleaning—of a trans-trocar-located scope or other device. Further, the controlled environment of the chamber 120 may reduce fogging of a scope by eliminating or reducing temperature changes and/or changes in humidity.

The valve 126 (which may include more than one valve) may include a particular structure that allows certain medical devices to pass through the proximal opening 122 and into the chamber while maintaining the seal or fluid barrier. For example, the valve 126 may include the depicted duck-bill seal, an annular seal structure, or both, but other suitable structures may additionally or alternatively be included. The valve 126 may be formed with a compliant material such that it expands or contracts as necessary for compatibility with scopes of different sizes. For example, on the Shore Hardness Scale, the valve 126 may be formed of a material with a hardness between about Shore A 20 to about Shore A 80, such as from about Shore A 30 to about Shore A 60.

An insufflation inlet 128 may communicate with the chamber and may be configured to control the pressure and other characteristics (e.g., temperature, composition of the atmosphere), which may be advantageous for providing precise control of insufflation of a body cavity during the laparoscopic procedure. The insufflation inlet 128 may include an insufflation valve 130, and may be in fluid communication with a pump or other suitable pressure source. As shown, the insufflation inlet 128 may communicate with a distal chamber portion 121 (which is a portion of the chamber 120) that is separated from the remainder of the chamber 120 by a divider 150, and the cleaning element 136 may be located on a proximal face of the divider 150, as shown. Advantageously, the flow of gasses or other contents received into the chamber 120 through the insufflation inlet 128 may be introduced in a manner such that the effect of the flow across cleaning element 136 is reduced or eliminated. For example, when the cleaning element 136 (which is described in detail below) is wetted with a cleaning fluid, concerns of increased evaporation due to fluid flow over the cleaning element 136 may be alleviated.

The trocar assembly 102 may provide an entry or point of access into the body for a scope 132. In non-limiting embodiments, the scope 132 may include a commercially-available rigid laparoscope with a 5 mm or a 10 mm diameter (or any other suitable diameter) with either a non-angled lens or an angled lens, which may be angled at 30 degrees, 45 degrees, 50 degrees, etc. with respect to the longitudinal axis of the scope 132. At least a distal end 134 of the scope 132 may include one or more elements designed to magnify, reflect, illuminate, and/or capture images of internal body areas under treatment, and then transmit those

images back to the medical professional controlling the procedure (herein referred to as a "viewing element"). The scope 132 may be inserted into proximal opening 122 of the chamber 120, may extend through the chamber 120, and may extend through into the cannula 106 through a distal opening 124 in the bottom wall 125 of the chamber 120, where the distal opening 124 is in fluid and mechanical communication with the cannula 106. The scope 132 may further extend distally to the cannula's distal end 108 (shown in FIG. 1) and into the body cavity. In some embodiments, a sleeve (not shown, but readily understood as a lining layer) may be located within the cannula 106, and the scope 132 may pass through the sleeve. Once deployed, the scope 132 may be manipulated by the medical professional moving it distally/proximally, angling it, and/or by rotating it into a particular orientation. Typically, during laparoscopic procedures, scopes can become obstructed when debris (e.g., condensation, displaced tissue, bodily fluids) are encountered and accumulate on a lens of the scope, which may compromise the image or video feed provided to the medical professional.

As shown in FIG. 2, the trocar assembly 102 may include the cleaning element 136 forming a surface 138 at a location within the internal environment. The housing 104 may include a cleaning element receiving surface 135 configured (e.g., sized and shaped) to receive, and attach to, the cleaning element 136. The cleaning element may have a surface (such as the bottom surface 129) configured to secure to the cleaning element receiving surface 135. For example, the bottom surface 129 may have an adhesive or other tacky/sticky substance to adhere to the cleaning element receiving surface 135, but additional and/or alternative securement devices are contemplated. The surface 138 of the cleaning element 136 may facilitate removal of obstructions from the scope 132 without necessitating removal of the scope 132 from the internal environment. Advantageously, lengthy interruptions (and therefore increased surgical and anesthesia time) due to removing and/or replacing an obstructed scope may be reduced or eliminated. Further, the distal end of the scope 132 may remain in the sterile internal environment during cleaning, which may advantageously alleviate concerns related to loss of sterility within the internal environment due to the removal and re-entry of the scope 132 one or more times for cleaning purposes. Keeping the scope 132 within the internal environment may also reduce or eliminate debris in the form of fogging or condensation caused by exposure to pressure and/or temperature changes when switching between environments. It should also be understood that certain advantages of the present embodiments are generally described as relating to a scope for explanation purposes and may also extend to other types of instruments used during surgical procedures, and therefore "scope" should be understood as including any suitable medical device used during laparoscopic surgery when described in the context of the present embodiments, unless clearly excluded.

The cleaning element 136 may incorporate any suitable structures, materials, and/or cleaning solutions for moving obstructions from the scope 132. The cleaning element may have a unitary construction, or alternatively may have multiple surfaces or layers with different cleaning characteristics or properties for facilitating multiple treatments. For example, it is contemplated that the cleaning element 136 may have a first region with an abrasive surface for breaking up potential obstructions, a second region including a liquid, a gel, or other material for dissolving or washing away the

obstructions, and a third region with an absorbent or adsorbent surface for removing any remaining residue.

The cleaning element **136** may include any suitable cleaning structures or materials, such as sponges, foams (e.g., reticulated or non-reticulated foamed plastic polymers forming open-cell, semi-open cell, or closed-cell foam structures), fibrous materials (e.g., materials with natural (e.g., cellulosic) and/or synthetic fibers), microfiber or wipe materials (e.g., polyethers, polyamides, polyesters, and/or blends of each in a woven or non-woven construction with split or non-split fibers), hydrophilic or hydrophobic materials, fluids, gases, bristles, films, etc. The structures and/or materials of the cleaning element **136** may include and hydrophobic properties to assist in absorbing and wicking of various bodily fluids and/or lipophilic characteristics for increased absorption of oils or fats. The cleaning element **136** may be capable of absorbing at least 5 times its original weight of fluids, such as about 15 times its original weight (or more). When the cleaning element **136** includes pores, consistent or variable pore sizes may be consistently or randomly dispersed (or layered) in certain configurations for suitable absorption properties (for example, a the cleaning element **136** may include a micro-porous foam with about 4 pores per inch to about 100 pores per inch). The cleaning element **136** may have a firmness/compliance of about 2 lbs/50 in² to about 80 lbs/50 in², and preferably about 6 lbs/50 in² to about 45 lbs/50 in² (when tested at 25% deflection on a 20 inch by 20 inch by 4 inch specimen). The material(s) of the cleaning element **136** may be formed of a material suitable for use in a medical device (e.g., with suitable biocompatibility, non-linting/no particulate, tear resistance, sterilization or other chemical/solvent compatibility, and radiation stability).

The cleaning element **136** may be multi-layered in some embodiments. For example, a first layer may be configured to absorb a fluid obstruction located on the scope **132**, and a second layer may be configured to retain or discard that fluid. In some embodiments, the first layer may include an open-cell foam with relatively low density (such as polyurethane or silicone foam) that may be used to effectively and quickly absorb (or wick, etc.) the obstructing fluid, and the second layer may include higher-density foam for effectively retaining the fluid. The second layer may be located beneath (e.g., covered by) the first layer, for example. Fibrous materials such as terrycloth and microfiber cloths may additionally or alternatively be used and may be advantageous for providing a streak-free lens surface when wiped against the scope **132**. The solid materials of the cleaning element **136** may be combined or “wetted” with a cleaning fluid, such as an anti-fog fluid, sterile water, saline, a detergent, etc., which may facilitate the removal of fatty smudges and dried-on debris.

Referring to the trocar assembly **102** of FIG. 2, in the event the medical professional’s visibility becomes compromised due to obstruction of the scope **132** during surgery, the scope **132** may be retracted proximally such that the distal end of the scope **132** is located within the chamber **120**. The distal end **134** (or other location) may then be wiped or swept by pressing and/or rubbing the distal end **134** of the scope **132** on the cleaning element **136** to remove obstructions. As explained above, this cleaning procedure may advantageously be completed without removing the scope **132** from the internal environment in the trocar assembly **102**. In some embodiment, the housing **104** may be formed of a transparent or translucent material such that a user has a visual perspective of the cleaning element **136**, the scope **132**, and other objects in the chamber **120** during the

cleaning procedure. Similarly, the cannula **106** may be formed of a transparent or translucent material. When the scope **132** is located in the trocar assembly **102**, the scope **132** (which often includes a light) may illuminate the chamber **120** to increase visibility, even if the housing **104** is not fully transparent. While the housing **104** may be fully formed of a transparent or translucent material, the housing **104** may alternatively include an opaque material and also include at least one viewport formed of transparent or translucent material.

In some embodiments, the cleaning element **136** may be selectable, removable, and/or replaceable. Thus, the trocar assembly **102** may be capable of allowing access into the chamber **120** (e.g., in an operating room prior to a surgery) such that a medical professional can select an appropriate version of the cleaning element **136** and then use that cleaning element **136** with the trocar assembly **102** during the procedure. The access may be provided by separating an upper portion **190** of the housing from a lower portion **192** of the housing, for example. The cleaning element **136** may additionally or alternatively be replaced during a medical procedure (e.g., if it becomes soiled), and/or may be replaced between medical procedures during reprocessing of the trocar assembly **102** if the trocar assembly **102** is reusable.

After completion of the cleaning procedure, the distal end **134** of the scope **132** may be again advanced through the cannula **106** and out beyond the cannula distal end to restore the image or video feed provided by the scope. Those of skill in the art will appreciate that existing scopes and potential scope designs include at least one non-longitudinal, distal-end-facing surface of the distal end **134** that may be generally or exactly perpendicular to the longitudinal axis of the scope **132**, or which distal-facing surface may be configured at a non-perpendicular angle relative to the longitudinal axis (e.g., 30 degrees off-perpendicular, 45 degrees off-perpendicular). It is further contemplated that the distal-facing surface of the scope **132** may be flat/planar, concave, or convex relative to the major plane of that face. The term “non-longitudinal, distal-end-facing surface” is meant to include the operative end face(s) of a scope in distinction from the longitudinal lateral sides of the scope, which will generally be columnar cylindrical. Thus, as described in more detail below, the surface characteristics of the cleaning element **136** may be shaped or otherwise configured for compatibility with a variety of distal-facing surfaces of the scope **132**.

FIG. 3 shows a trocar assembly **202** with a housing **204**, a chamber **220**, and a cannula **206**. The trocar assembly **202** includes a cleaning element **236** with a concave surface **238** (or other curved surface) within the chamber **220**. The concave surface **238** may be advantageous for providing a cleaning profile that matches a profile of a scope with a distal non-perpendicular face, such as a curved (e.g., convex) or angled lens, or other curved instrument, for example. The concave surface **238** may advantageously increase the total surface area of the cleaning element **236** when compared to a flat cleaning element, which may be advantageous when more than one cleaning procedure will take place without replacing or reprocessing the trocar assembly **202**, particularly if previously-used areas of the cleaning element **236** cannot be reused without reprocessing (e.g., due to buildup of debris).

The cleaning element **236** may also line the cannula **206** or otherwise extend through the cannula **206**, as depicted by FIG. 3. Advantageously, this embodiment may provide the ability to clean a scope while retracting it through the

cannula 206 and/or without necessitating retraction of the distal end 234 of the scope the entire way to the chamber 220, particularly when the obstructed instrumentation is located on an outer-diameter surface along the elongated body of the scope. The cleaning element 236 may extend all the way to the distal end of the cannula 206, or not. While not shown, it is contemplated that the entirety of the inner surface area of the trocar assembly 202 within the internal environment may include one or more cleaning element(s) 236.

FIG. 3A shows the embodiment of the trocar assembly 202 of FIG. 3 during a cleaning procedure in accordance with the present disclosure. As shown, the scope 232 may be received into the chamber 220 of the housing 204 through the top opening 222. While not shown, a valve may be located at the top opening 222 to form a fluid barrier at the top opening 222, thereby sealing the environment inside the chamber 220 from an external environment. The cleaning element 236 may include the curved concave surface 238, which is particularly advantageous when the scope 232 has angled distal end 234 as depicted, a curved distal end, or another non-planar distal end. To clean the distal end 234 of the scope 232, the user may wipe the distal end 234 of the scope 232 against the concave surface 238 of the cleaning element 236 to remove debris. At least a portion of the cleaning element 236 may be relatively compliant such that when the user presses the distal end of the scope 232 against the cleaning element 236 with sufficient force, the contact portion of the cleaning element 236 yields and at least partially assumes the shape of the distal end 234 of the scope 232 to thereby provide a larger surface area of contact.

Another embodiment of a trocar assembly 302 is depicted in FIG. 4. Like other embodiments described herein, the trocar assembly 302 includes a housing 304 with a chamber 320 and a cannula 306 extending from the chamber 320. A proximal or top wall 323 of the housing 304 may include an opening 322, which may be configured to receive a scope and which may be associated with a valve (not shown) for sealing the chamber 320 from an external environment. The chamber 320 may be defined by the top wall 323, a distal or bottom wall 325, and a generally cylindrical side wall 327 extending from the top wall 323 to the bottom wall 325. The housing 304 includes a first button 340 and a second button 342. Herein, a "button" may be a structure that moves in response to an input force applied by a user. The buttons 340, 342 may form a portion of the side wall 327 such that the chamber 320 is deformable (e.g., inwardly). The first button 340 and the second button 342 are secured to a cleaning element 336 such that movement of the first button 340 and/or the second button 342 effects displacement of the cleaning element 336. The buttons 340, 342 may be configured to move in response to an input force applied to one or more of the buttons 340, 342. So, the cleaning element 336 may displace from a default state (shown in FIG. 4) to a displaced state (not shown) when one of the buttons 340, 342 is moved in response to the applied input force. The input force may result from a medical professional intentionally applying pressure on one of the buttons 340, 342, for example. While two buttons are depicted, more or fewer than two buttons may be included. The buttons may be coupled to a spring or other biasing element such that the cleaning element 336 returns to the default state when the input force is removed from the buttons 340, 342. It is contemplated that the resiliency of the cleaning element 336 may provide the biasing/spring force, particularly when the cleaning element 336 includes a resilient material, such as a particular foam, rubber, or plastic. Therefore, the cleaning

element 336 may include a tendency to assume the default state in the absence of an input force (shown, in the non-limiting illustration of FIG. 4 as a flat circular disc with a center-hole, but able to be embodied differently within the scope of the present disclosure).

The cleaning element 336 may have an opening 344 to provide access from a proximal portion 346 of the chamber 320 to a distal portion 348 of the chamber, and/or from the proximal portion 346 of the chamber 320 to the cannula 306.

The opening 344 may be aligned with a longitudinal axis of the cannula 306 such that substantially straight elongated instruments extending through the cannula 306 also may extend proximally through the opening 344. The diameter (or other cross-sectional dimension) of the opening 344 may be approximately equal to, or slightly larger than, the inner diameter of the cannula 306 and/or an outer diameter of a scope, which may be advantageous for allowing the scope to pass through the opening 344 without catching or creating friction when being manipulated during the laparoscopic procedure. Alternatively, it may be advantageous for the diameter of the opening 344 to be less than the diameter of certain instruments (and therefore less than the inner diameter of the cannula 306) such that the cleaning element 336 contacts the outer diameter of those instruments, thereby cleaning the outer diameter surface of those instruments and/or providing a friction to give a medical professional precise control, including a braking-like control, of the distal/proximal movement and rotation of that instrument.

In some embodiments, the opening 344 allows certain instruments, such as a scope, access to the cannula 306 when the cleaning element 336 is in the default state, and then restricts access to the cannula 306 when the cleaning element is in the displaced state. Advantageously, when the scope becomes obstructed by debris, the scope may be withdrawn proximally through the opening 344 such that a distal end of the scope is within the proximal portion 346 of the chamber 320. Then, the cleaning element 336 may be displaced as a result of an input force applied to one or more buttons, as described above. The displacement of the cleaning element 336 may change the location and/or the dimensions of the opening 344 such that when the scope is advanced distally towards the cannula 306, it does not proceed through the opening 344 but instead contacts the cleaning element 336. Accordingly, the scope may contact the cleaning element 336 for cleaning purposes. After cleaning, the input force may be removed from the buttons, the cleaning element 336 may then return to the default state providing access to the cannula 306 through the opening 344, and the scope may then be advanced distally through the cannula 306 to again resume its function inside the body cavity.

While not required, the housing 304 may include a divider 350 separating the proximal portion 346 of the chamber 320 from the distal portion 348 of the chamber 320. The divider 350 may provide suitable support and guidance for the buttons 340, 342, for example. The divider 350 may include a guide opening 352, which may retain the distal end of the scope such that it remains approximately aligned with the cannula 306 during the cleaning process. This may facilitate efficient re-entry into the cannula 306 after cleaning. While not required, the opening 352 of the divider 350 may include a valve or other suitable device for creating a seal between the distal portion 348 of the chamber 320 and the proximal portion 346 of the chamber 320. In other embodiments, the distal portion 348 of the chamber 320 may be in fluid communication with the proximal portion 346 of the chamber 320, which may be advantageous for eliminating or

reducing pressure and/or temperature change when a distal end of a scope is moved between chamber portions. The divider **350** is not required in all embodiments.

As shown an embodiment illustrated in FIG. 5, the divider **350** may include cleaning element receiving surface **335** configured (e.g., sized and shaped) to receive and attach to a second cleaning element **354**. The second cleaning element **354** may include one or more of the features of at least one of the cleaning elements described above with respect to FIG. 2 and FIG. 3. The two cleaning elements **336**, **354** may be intended for different degrees of debris removal, or may otherwise have at least one different cleaning property. For example, it is contemplated that more efficient, but potentially less effective cleaning may be performed with the cleaning element **336**, while more extensive cleaning may be carried out by the second cleaning element **354** (e.g., “rough cleaning” and “fine cleaning,” respectively, analogous in such an example to a coarse filter for removing larger elements, and fine filter for polishing and removing smaller elements). Further, the first cleaning element **336** may be better suited for debris removal on side surfaces of a scope, while the second cleaning element **354** may be better suited for removing debris on a distal-face surface.

It is also contemplated that a single cleaning element may have two surface-area portions that are configured differently (i.e., have at least one different cleaning property). For example, a first surface area portion **394** of the second cleaning element **354** may be configured for cleaning without a cleaning fluid, and a second surface area portion **396** may be wetted or may otherwise be configured for a different cleaning function than the first surface area portion **394**. The two surface area portions may have different colors or other visual characteristics such that a user can readily distinguish between the surface area portions visually (particularly when the housing **304** is transparent or translucent). Alternatively (or in addition), the scope may provide visual feedback to an external screen or other device to facilitate distinguishing between surface area portions. It is also contemplated that the surface area portions may have different textures or otherwise provide a tactical indication that a user can sense when rubbing or otherwise contacting a scope with the surface area portions, which may be advantageous for ensuring completion of the proper cleaning function(s).

FIG. 6 shows a trocar assembly **402** with a cleaning element **436** having a first portion **456** and a second portion **458** extending to a location outside of a housing **404**. The first portion **456** and the second portion **458** of the cleaning element **436** may respectively form a first button **440** and a second button **442** for receiving an input force. The first portion **456** and the second portion **458** may form a portion of the shell of the housing **404** that defines the chamber **420** and retains a pressure differential between the chamber **420** and the external environment. The cleaning element **436** may further include an opening **444** providing access to a cannula **406** at least when the cleaning element **436** is in a default state. Similar to as described above with reference to FIG. 4 and FIG. 5, that access may be restricted when an input force is applied to at least one of the first button **440** and the second button **442**, thereby moving the cleaning element **436** and the opening **444** into a displaced state. Natural resiliency of a material forming the cleaning element **436** may ensure the cleaning element **436** is in the default state when no input force is provided. The portions of the cleaning element **436** forming the first button **440** and/or the second button **442** may include a compressible/compliant material slightly larger (when/where not com-

pressed) than corresponding openings **422**, **424** of the housing **404**, which may advantageously retain a fluid barrier between the chamber and an external environment by contacting the chamber in a sealing/compliant manner (when still and when being moved/displaced) so as to prevent or at least inhibit loss of fluid from the chamber **420** (e.g., positive insufflation pressure, liquids from cleaning and/or medical procedures).

Another embodiment of a trocar assembly **502** is shown in FIG. 7. The trocar assembly **502** may include a housing **504** and a cleaning element **536** forming a cleaning surface within the housing **504**, as shown. As in certain embodiments described above, the housing **504** may form a chamber **520** that is sealed from an external environment. A scope or other medical device may be received by the trocar assembly **502** through a top wall **523** of the housing **504**, and specifically through an opening **522** of the top wall **523** of the housing **504**. A valve **530** may form a fluid-barrier around an outer surface of the scope to retain the seal between the chamber **520** and the external environment when the scope is received by the trocar assembly **502**. The housing **504** may include one or more flexible wall portions **560**, **562**, which may act as (and be referred to) as buttons for receiving an input force. The input force may cause the flexible wall portions **560**, **562** to flex, thereby forcing the cleaning element **536** from the depicted default state to a displaced state. The resiliency of the flexible wall portions **560**, **562** and/or the resiliency of the cleaning element **536** may cause movement back to the default state when the input force is removed.

Similarly, a trocar assembly **602** depicted in FIG. 8 has a first flexible wall portion **660** and a second flexible wall portion **662**. Here, the first flexible wall portion **660** and the second flexible wall portion **662** are formed by openings **664**, **666** within an outer shell **668** of the housing **604**, where a cleaning element **636** at least partially forms an inner shell **670** of the housing **604**. It is contemplated that the inner shell **670** may be formed entirely by the cleaning element **636**. The inner shell **670** may cover the openings **664**, **666** such that a fluid barrier between a chamber **620** of the housing **604** and the external environment is not compromised. As shown, the inner shell **670** may form at least a portion of an external surface of the housing **604**, and may be substantially surrounded by the outer shell **668**.

When a scope is located in the chamber **620**, an input force may be applied to at least one of the first flexible wall portion **660** and the second flexible wall portion **662** such that the cleaning element **636** deflects towards the center of the chamber for easier and more comprehensive cleaning of the scope. Further, when the inner shell **670** is relatively thin and compliant, this embodiment may be advantageous for providing a medical professional with a sense of feel (i.e., tactile indication) with respect to the scope by allowing the medical professional to indirectly touch the scope (through the inner shell **670**), which may provide for efficient and effective wiping or sweeping of debris from the scope. While not shown in FIG. 8, a second cleaning element may be included on another surface of the chamber **620** (e.g., a bottom or distal surface, which may be a cleaning element receiving surface), which may have features described in certain embodiments above with reference to FIG. 4 and FIG. 5, for example.

FIG. 8A shows a second illustration of the embodiment of the trocar assembly **602** of FIG. 8 (but also with an insufflation inlet **628**). As shown, the outer shell **668** may include the opening **664**, and the cleaning element **636** (and particularly the flexible wall portion **660**, shown as partially

transparent in FIG. 8A) may be aligned with the opening 664 such that it is accessible by a user and such that a user can press the flexible wall portion 660 by reaching/pressing through the opening 664. The cleaning element 636 may also cover the opening 664 and function as seal or fluid barrier between the chamber 620 and the external environment. Thus, the cleaning element 636 may include a material that is not permeable or is substantially impermeable by air or other gasses/fluids. It is contemplated that only an outer layer or portion of the cleaning element 636 forms the seal, while an inner layer or portion is configured for absorption and retention of a liquid or other fluid (as described in more detail above). Additionally or alternatively, a fluid-impermeable cover or other element may be placed on the cleaning element 636 and over the opening 664 for forming the seal between the chamber 620 and the external environment.

FIG. 9 shows a trocar assembly 702 with an adjustable cleaning element 736 and a second cleaning element 754. The second cleaning element 754 may form a surface within a chamber 720 of the housing 704 and may be similar to the cleaning element 136 of FIG. 2, for example. The adjustable cleaning element 736 may be configured to rotate, slide, or otherwise move to adjust its position and/or orientation relative to the housing 704. In the depicted embodiment, the adjustable cleaning element 736 includes a wheel 772 with a pair of first cleaning surfaces 774, a pair of second cleaning surfaces 776, and a pair of openings 778. Alternatively, more or fewer than two types of cleaning surfaces may be included. When in a first setting (depicted), the cleaning element 736 may restrict access to a cannula, and the first cleaning surface 774 may be located along a longitudinal axis of the cannula 706 such that a scope will contact the first cleaning surface 774 when moving distally within the chamber 720 and towards the cannula 706. The first cleaning surface 774 may include certain surface characteristics and/or incorporate a cleaning material (e.g., a cleaning liquid) for carrying out a first cleaning treatment. For example, the first cleaning surface 774 may include a cleaning liquid or other fluid that may dissolve and loosen debris from the scope.

Next, the cleaning element 736 may be rotated to a second setting such that the second cleaning surface 776 is positioned to contact the scope. The second cleaning surface 776 may include certain surface characteristics and/or materials for carrying out a second cleaning treatment. For example, the second cleaning surface 776 may include an abrasive and/or absorbent surface that removes debris and absorbs residue (which is also considered debris herein) that remain on the scope after the first cleaning step. In this example, the two cleaning steps can be repeated as necessary by rotating the cleaning element 736 and repeating contact between particular cleaning surfaces and the scope. A cleaning surface may additionally or alternatively include a rubber or other material suitable for squeegeeing or otherwise wiping away fluid debris from a lens.

When the cleaning processes are complete, the cleaning element 736 may be rotated or otherwise moved to a third setting such that the opening 778 is aligned with the cannula 706 to provide the scope with access to the cannula 706. The opening 778 is depicted as a round hole in FIG. 9, but other suitable openings are contemplated (e.g., a wedge or pie-shaped or other-shaped gap in the wheel 772, a hole of a different shape, etc.). The cleaning element 736 may include openings of different shapes and sizes (and also cleaning surfaces of different shapes and sizes) for compatibility with multiple types of scopes and other medical instruments. It is contemplated, for example, that certain cleaning surfaces of

the movable cleaning element 736 are concave in shape for interaction with a convex instrument surface, while others are flat for interaction with a flat instrument surface.

FIG. 10 shows a trocar assembly 802 similar to the trocar assembly 202 of FIG. 2, but with a different embodiment of a cleaning element 836. As shown in FIG. 10, the cleaning element 836 may include a stepped portion 838. Advantageously, during a cleaning procedure, the stepped portion 838 may provide an edge 840 (which may be a sharp corner or a rounded edge) that can be used as a scraping edge and/or that can be used to ensure suitable contact of a scope with an angled lens, for example. The stepped portion 838 may be formed by including two portions of the cleaning element 836: a first disk portion 842 and a second disk portion 844, where the second disk portion 844 is located on a proximal surface of the first disk portion 842, and where the second disk portion 844 has a larger inner diameter than the first disk portion 842 such that the proximal surface of the first disk portion 842 remains accessible. Alternative constructions are also contemplated for forming the stepped portion 838. In one non-limiting example, the cleaning element 836 may include an outer disk with a first height and an inner disk with a second height, where the first height is greater than the second height, and wherein an inner diameter of the outer disk surrounds an inner diameter of the second disk (i.e., such that the second disk is "inside" the first disk). A cleaning element 836 with a stepped portion may be included in any of the embodiments of trocar assemblies described above. Cleaning elements with other surface characteristics are also contemplated. For example, a cleaning surface may be flat (e.g., as in FIG. 2), curved concavely (e.g., as in FIG. 3), curved convexly, stepped (e.g., as in FIG. 10), sloped or angled, wavy, spiked, etc.

Those of skill in the art will appreciate that embodiments not expressly illustrated herein may be practiced within the scope of the claims, including that features described herein for different embodiments may be combined with each other and/or with currently-known or future-developed technologies while remaining within the scope of the claims. This specifically includes that the structure, location, and mechanisms of the disclosed cleaning elements and related structures in the different embodiments illustrated and described with reference to the drawing figures may be combined and elements interchanged within the level of skill in the art as informed by this application, and within the scope of the present claims, which includes that a variety of disclosed individual cleaning element components dimensioned for use encompassed within in laparoscopy trocars may be configured as separable/replaceable components of a larger trocar assembly. Although specific terms are employed herein, they are used in a generic and descriptive sense only and not for purposes of limitation unless specifically defined by context, usage, or other explicit designation. It is therefore intended that the foregoing detailed description be regarded as illustrative rather than limiting. And, it should be understood that the following claims, including all equivalents, are intended to define the spirit and scope of this invention. Furthermore, the advantages described above are not necessarily the only advantages of the invention, and it is not necessarily expected that all of the described advantages will be achieved with every embodiment. In the event of any inconsistent disclosure or definition from the present application conflicting with any document incorporated by reference, the disclosure or definition herein shall be deemed to prevail.

15

We claim:

1. A housing for a laparoscopic trocar assembly with an integrated scope-cleaning structure, the housing comprising: a shell forming a wall portion of a chamber; and a cleaning element that is located proximal a cannula with the cannula extending distally away from the chamber, the cleaning element forming at least a portion of an internal surface of the chamber, the cleaning element configured to remove debris from a distal end of a scope upon contact between the cleaning element and the distal end of the scope,

wherein the cleaning element is movable with respect to the shell of the housing in response to an input force upon the shell that moves a portion of the shell and a portion of the cleaning element between a default state and a displaced state.

2. The housing of claim 1, further comprising an external surface at least partially formed by the shell, wherein an external facing surface of the cleaning element forms at least a portion of the external surface of the housing.

3. The housing of claim 1, wherein the cleaning element is formed of a resilient material such that the cleaning element includes a tendency to assume the default state in the absence of an input force, and wherein the default state forms an external shape that is generally continuous with the shell, or that extends from the shell in a visually-contrasting manner.

4. The housing of claim 1, further comprising at least one button coupled to the cleaning element, wherein the input force is applied to the at least one button, and wherein the at least one button is movable with respect to the chamber in response to the input force.

5. The housing of claim 1, wherein the cleaning element includes an opening longitudinally aligned with a longitudinal axis of a cannula extending distally from the housing when the cleaning element is in the default state.

6. The housing of claim 5, further comprising a divider separating the chamber into a proximal portion and a distal portion, the divider including an opening aligned with the opening of the cleaning element.

7. The housing of claim 6, wherein the divider comprises a second cleaning element located in the proximal portion of the chamber.

8. The housing of claim 7, wherein the second cleaning element includes a curved concave proximal-facing surface.

9. The housing of claim 1, wherein the cleaning element includes a stepped portion with an edge.

10. A housing for a laparoscopic trocar assembly with an integrated scope-cleaning structure, the housing comprising: an outer shell with a proximal entry opening through a proximal wall, a distal exit opening to a cannula that extends distally from a distal wall of the outer shell, and a generally cylindrical wall therebetween, the generally cylindrical wall circumferentially defining a chamber at least partially proximal the cannula and being deformable; and

16

an inner surface of the generally cylindrical wall comprising at least one cleaning element with a cleaning surface within the chamber, the cleaning surface configured to contact and to remove debris from at least a viewing element of a scope when the generally cylindrical wall is deformed and the at least a viewing element is within the chamber.

11. The housing of claim 10, wherein the outer shell proximal entry opening forms a fluid-patent seal around a scope directed therethrough.

12. The housing of claim 11, wherein the cleaning surface is comprised by a more-flexible wall portion of the generally cylindrical wall, immediately adjacent a less-flexible outermost periphery of the proximal wall of the outer shell, the more-flexible wall portion configured to displace inwards with respect to the chamber in response to an input force directed toward a central region of the generally cylindrical wall.

13. The housing of claim 10, wherein the cleaning surface is formed of a compliant material continuous with the generally cylindrical wall.

14. The housing of claim 10, wherein the cleaning element forms at least a portion of an inner-facing longitudinal and circumferential surface of the housing.

15. The housing of claim 10, wherein the cleaning element is movable with respect to the outer shell of the housing in response to an input force between a generally cylindrical default state and a displaced state.

16. The housing of claim 15, wherein the cleaning element is formed of a resilient material such that the cleaning element includes a tendency to assume the default state in the absence of an input force.

17. The housing of claim 10, wherein the cleaning element includes a stepped portion with an edge.

18. A method for cleaning a scope, the method comprising:

maneuvering a distal end of the scope proximally out of a cannula to a location within a chamber of a trocar assembly, the chamber at least partially formed by a shell wherein a cleaning element comprises a surface within the chamber;

moving the cleaning element from a default state to a displaced state by displacing an external-facing surface of the chamber inwardly; and

removing debris from at least a distal-facing surface of the scope moving the scope and in contact with a cleaning element.

19. The method of claim 18, wherein moving the cleaning element includes applying an input force to a button comprised by the external-facing surface of the chamber, wherein the button is coupled to the cleaning element.

20. The method of claim 18, wherein the cleaning element is formed of a resilient material such that the cleaning element includes a tendency to assume the default state in the absence of an input force.

* * * * *

专利名称(译)	带有清洁元件的套管组件，用于腹腔镜手术		
公开(公告)号	US10368905	公开(公告)日	2019-08-06
申请号	US15/452211	申请日	2017-03-07
[标]申请(专利权)人(译)	CAREFUSION 2200		
申请(专利权)人(译)	CAREFUSION 2200 , INC.		
当前申请(专利权)人(译)	CAREFUSION 2200 , INC.		
[标]发明人	ROSENBAUM JOANNA L CHUNG JEANNY HUBBARD PATRICK PRYBELL JOSEPH THRELKELD CORRIE TILLMAN SARA TOTH BRANDON VANDEWEGHE ANDREW P WILSCHKE THOMAS DARLEY JESSE CHARLES HARRIS CHRISTOPHER ALAN IRWIN CURTIS B LATHAM STEPHEN A LEE DANIEL J RODENKIRCH DOUGLAS STASZAK JEFFREY R		
发明人	ROSENBAUM, JOANNA L. CHUNG, JEANNY HUBBARD, PATRICK PRYBELL, JOSEPH THRELKELD, CORRIE TILLMAN, SARA TOTH, BRANDON VANDEWEGHE, ANDREW P. WILSCHKE, THOMAS DARLEY, JESSE CHARLES HARRIS, CHRISTOPHER ALAN IRWIN, CURTIS B. LATHAM, STEPHEN A. LEE, DANIEL J. RODENKIRCH, DOUGLAS STASZAK, JEFFREY R.		
IPC分类号	A61B17/34 A61B1/12 A61B1/00 A61B1/313		
CPC分类号	A61B17/3415 A61B1/00154 A61B1/126 A61B17/34 A61B17/3462 A61B17/3474 A61B1/3132 A61B2017/3437 A61B17/3421 A61B17/3478 A61B17/3498 A61B90/70 A61B2090/701		
其他公开文献	US20180256203A1		
外部链接	Espacenet		
摘要(译)			

本公开涉及一种用于腹腔镜套管针组件的壳体，其具有集成的范围清洁结构。壳体可包括形成腔室的壁部分的壳体和形成腔室的内表面的至少一部分的清洁元件，清洁元件构造成在清洁元件之间接触时从窥镜的远端移除碎屑。和范围的远端。响应于壳体上的输入力，清洁元件可相对于壳体的壳体移动，壳体的一部分使壳体的一部分和清洁元件的一部分在默认状态和移位状态之间移动。

