



US 20080009858A1

(19) **United States**

(12) **Patent Application Publication**  
**Rizvi**

(10) **Pub. No.: US 2008/0009858 A1**

(43) **Pub. Date: Jan. 10, 2008**

(54) **LAPAROSCOPIC INSTRUMENT TIP AND METHOD OF SPECIMEN COLLECTION**

**Publication Classification**

(75) Inventor: **Syed Rizvi, Bakersfield, CA (US)**

(51) **Int. Cl.**  
**A61B 18/14** (2006.01)

Correspondence Address:  
**FURR LAW FIRM**  
**2622 DEBOLT ROAD**  
**UTICA, OH 43080**

(52) **U.S. Cl.** ..... **606/48; 606/51**


(73) Assignee: **CENTUM RESEARCH LLC,**  
**Bakersfield, CA (US)**

(57) **ABSTRACT**

(21) Appl. No.: **11/428,836**

A unique laparoscopy instrument tip and method which allows simultaneous gasping, cauterization, dissection, containment, enclosure and removal of body tissue. Mechanisms for grasping, holding, manipulating, cauterizing, dissecting, encasement in an enclosed cavity and removing the tissue are provided in one implement allowing easy, safe and quick performance of the procedure.

(22) Filed: **Jul. 6, 2006**

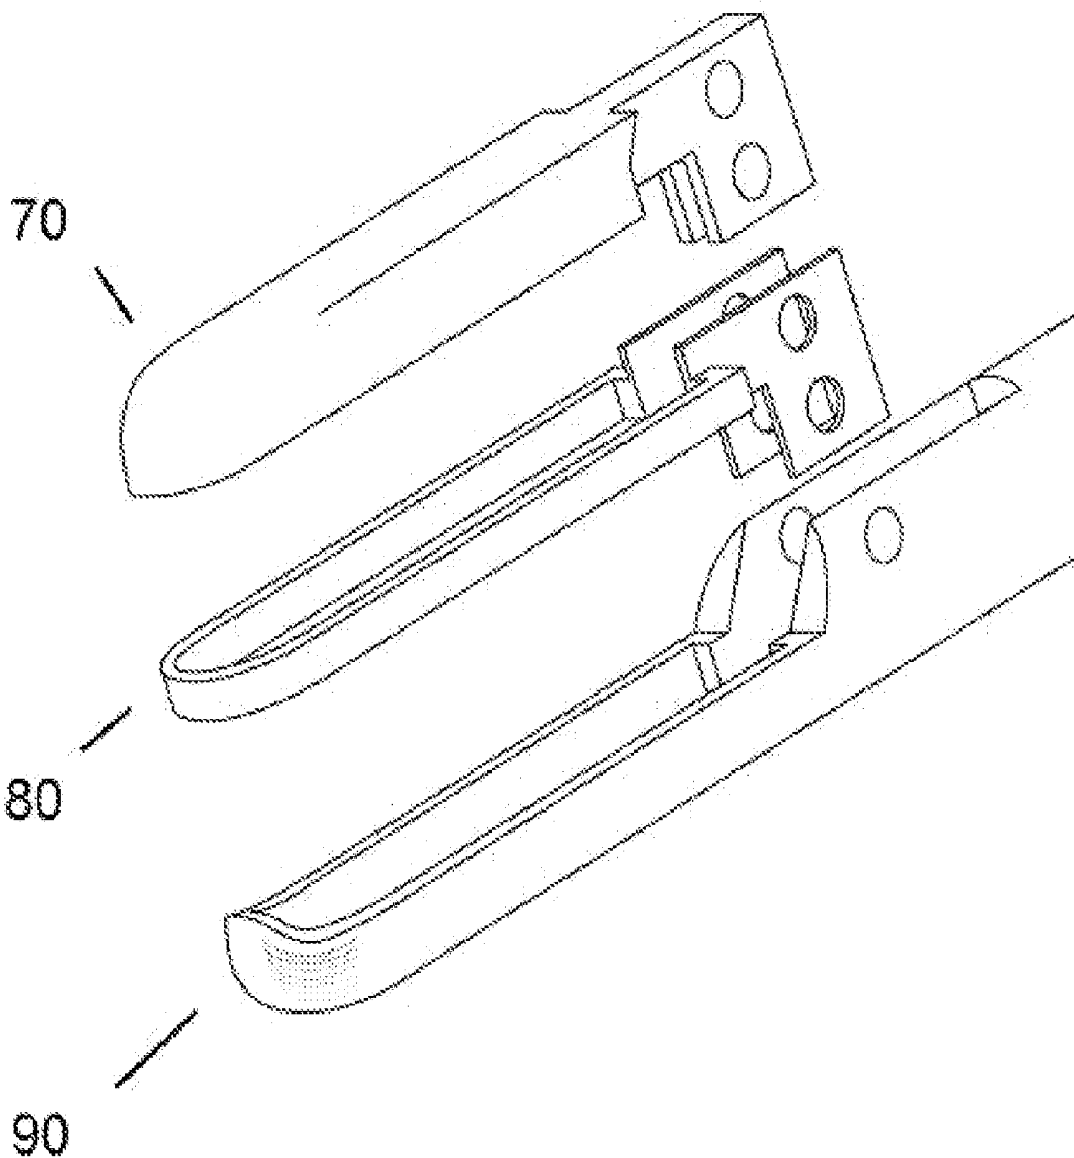

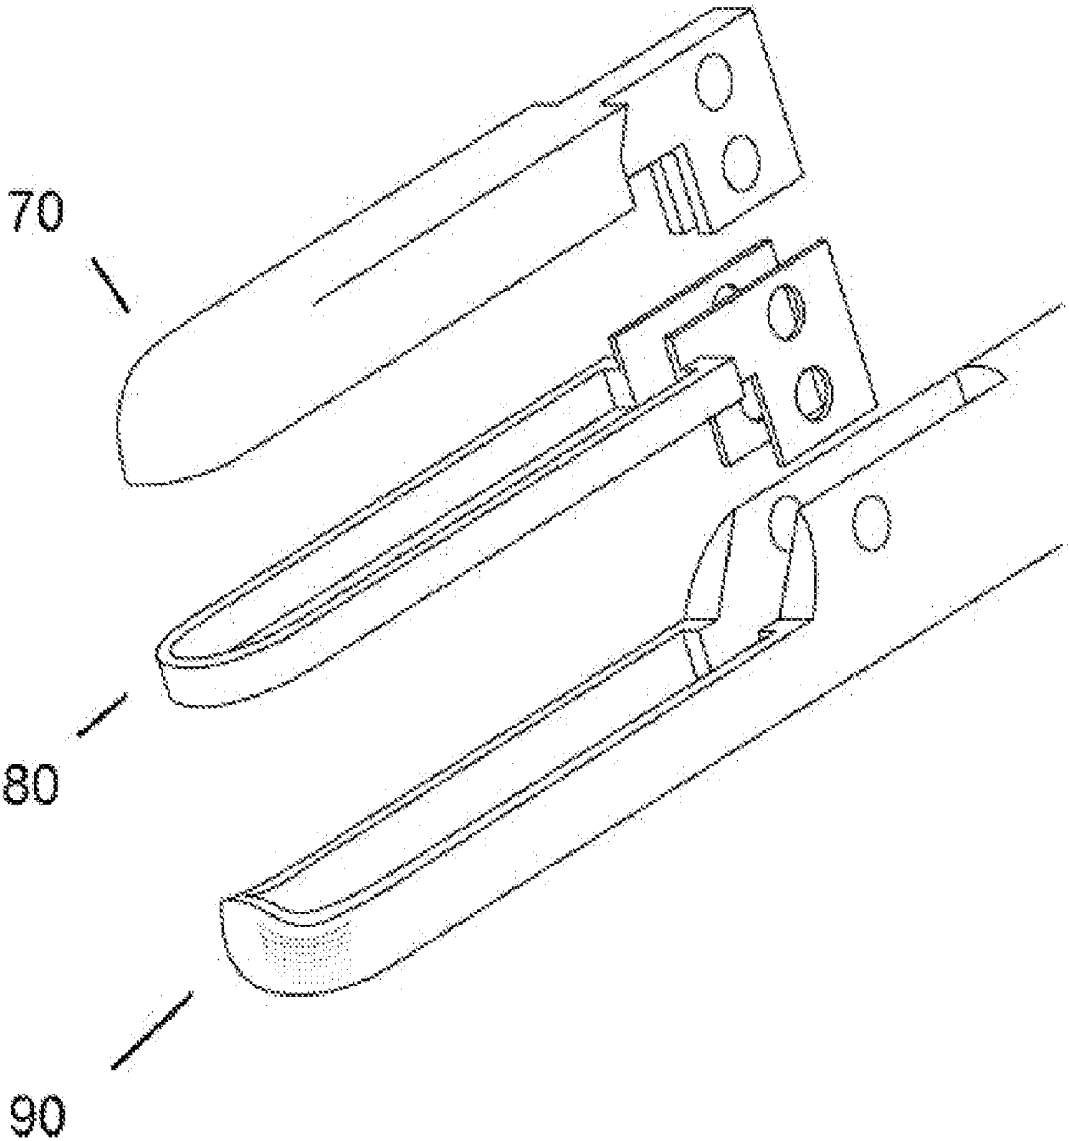


Figure 1

## LAPAROSCOPIC INSTRUMENT TIP AND METHOD OF SPECIMEN COLLECTION

### FIELD OF THE INVENTION

[0001] This invention relates to a laparoscopy instrument tip and method of use thereof, which prevents slippage of the tissue and allows simultaneous manipulation, cauterization, dissection and encasement of the tissue prior to the removal from the body.

### STATEMENT OF THE INVENTION

[0002] A unique laparoscopy instrument tip and method, which allows simultaneous manipulation, cauterization, dissection, encasement and removal of the body tissue. The tip is located at the distal end of the instrument, which allows lifting and grasping the tissue, cauterizing, cutting and encasing it. The raised outer edge of the fixed lower jaw prevents the slippage of the tissue during the procedure. The ring shape jaw allows cauterizing the tissue. The cup shape part dissects and protects the tissue until it is removed. The tip can be used on any part of the body where simultaneous manipulation, cauterization, tissue dissection and protected removal of the dissected tissue are desired. Any mechanism on the laparoscopy device can be used to open/close the jaws, manipulate the device and to operate the cautery/cutting mechanisms. The sources of energy used include but are not limited to electrical, ultrasonic, laser or radio energy.

[0003] The tip can be permanent or a disposable modular laparoscopic instrument tip. Disposable modular tip can provide surgical efficiency, convenience, precision, durability and cost effectiveness by replacing only the disposable modular tip and reusing the non-disposable laparoscopy instrument.

### BACKGROUND OF THE INVENTION

[0004] Technical advances, particularly the use of the laparoscopy, have significantly affected the setting in which procedures can be performed. Several laparoscopic instruments have been described in prior art. Many of these instruments provide multifunctionality such as simultaneous grasping, coagulation and cutting of the tissue. Slippage of the tissue from the tip is a problem during laparoscopic surgeries. It is difficult to hold the tissue for cautery or cutting adding to the technical difficulties, frustration, operating time, cost and risk of complications. Laparoscopic instrumentation in prior art does not provide for the prevention of the slippage of the tissue from the tip. Furthermore prior art does not provide for complete encasement and containment of the dissected tissue along with the cautery and active cutting mechanism before the removal. Lack of instrumentation and methods of preventing slippage of the tissue during the procedure and lack of adequate all in one cautery, cutting and containment mechanism prior to removal make it challenging for surgeons to perform operations using minimally invasive techniques.

[0005] During unipolar cautery, which can be performed with or without the laparoscopic instrument, patient's body is part of the circuit. This method has been associated with dangerous and fatal consequences due to injuries to other organs.

[0006] The bipolar cautery technique is the safest and simplest to perform. The poles of the tip of the instrument conduct the electricity between them, with no current flow

beyond the instrument tip, so the patient is not part of the circuit eliminating the risk of injury to other organs.

[0007] Tischer (U.S. Pat. No. 4,655,216) is a surgical combination instrument for grasping tissue, coagulating it and removing the tissue between the coagulated areas. This device does not provide for a mechanism to prevent the slippage of the tissue. This device also does not provide for complete encasement of the dissected tissue.

[0008] Ryan (U.S. Pat. No. 6,152,923) device is merely a grasping bipolar forceps with active passive cutting mechanism, which does not provide for preventing the slippage of the tissue. This device also does not provide for complete encasement of the dissected tissue. Furthermore this device does not provide an independent cutting mechanism.

[0009] Lands (U.S. Pat. No. 6,960,210) described a laparoscopic bipolar electro-surgical instrument that can just apply a large closure force between its jaw.

[0010] Ryan (U.S. Pat. No. 6,932,810) described an axial elongate bipolar tissue sealer/cutter.

[0011] Truckai (U.S. Pat. No. 6,929,644) described a working end of a surgical instrument that carries first and second jaws for delivering energy to tissue.

[0012] Truckai (U.S. Pat. No. 6,913,579) described an electro-surgical working end and method for obtaining a tissue sample for biopsy purposes with curved jaw members that are positioned on opposing sides.

[0013] Morley (U.S. Pat. No. 6,840,938) described a bipolar surgical instrument that includes opposing grips that can engage the tissue.

[0014] Frazier (U.S. Pat. No. 6,682,528) described an endoscopic bipolar forceps for clamping and sealing tissue includes first and second jaw members pivotally attached in opposing relation.

[0015] Dycus (U.S. Pat. D457,958) described a vessel sealer and divider.

[0016] Rioux (U.S. Pat. No. 3,938,527) described a laparoscopic electrocautery instrument for tubal cauterization.

[0017] Yoon (U.S. Pat. No. 3,967,625) described a method for sterilizing the female by tubal ligation comprising the use of a ring and an applicator device.

[0018] Polk (U.S. Pat. No. 4,226,239) described a surgical ligating instrument for tubal ligation by the application of two or more elastic rings.

[0019] Yoon (U.S. Pat. No. 4,374,523) describes a two cylinder ring applicator device and method for applying an elastic occluding ring on fallopian tubes.

[0020] Young (U.S. Pat. No. 5,300,081) describes an apparatus for applying surgical clips on the fallopian tubes.

[0021] Koros (U.S. Pat. No. 5,352,235) describes a monopolar laparoscopic instrument with scissor like blades to cut the tissue.

[0022] McQuilkin (U.S. Pat. No. 5,575,802) described a clip suitable for sexual sterilization.

[0023] Koros (U.S. Pat. No. 5,578,052) describes insulated laparoscopic grasper with removable shaft.

[0024] Whitfield (U.S. Pat. No. 5,833,696) described a surgical clip applying instrument.

[0025] Jones (U.S. Pat. No. 6,112,747) describes a method of female sterilization with the application of laser energy through the hysteroscope.

[0026] Davis (U.S. Pat. No. 6,241,740) describes an instrument and method for ligating with a clip and cutting the tissue.

[0027] Harrington (U.S. Pat. No. 6,309,384) describes a method, which involves thermally damaging the lining of the utero-tubal junction followed by placement of a foam plug.

[0028] It is therefore an object of the present invention to provide a tip for a bipolar laparoscopic instrument, which prevents the tissue from slippage during the procedure.

[0029] Another object is to provide a mechanism for the containment of the dissected tissue by complete encasement in an enclosed cavity during removal from the body.

[0030] A further object of the invention is provision of a multifunction tip for the bipolar laparoscopic instrument, which allows simultaneous cautery, dissection and retention of the dissected tissue in an enclosed cavity.

#### SUMMARY

[0031] A unique laparoscopy instrument tip and method which allows simultaneous gasping, cauterization, dissection, containment, enclosure and removal of body tissue. Mechanisms for grasping, holding, manipulating, cauterizing, dissecting, encasement in an enclosed cavity and removing the tissue are provided in one implement allowing easy, safe and quick performance of the procedure.

#### BRIEF DESCRIPTION OF THE DRAWINGS

[0032] Without restricting the full scope of this invention, the preferred form of this invention is illustrated in the following drawings:

[0033] FIG. 1 shows the overview of all components of the tip.

#### DESCRIPTION OF THE PREFERRED EMBODIMENT

[0034] FIG. 1 shows the overview of all components of the tip.

[0035] The cup shape movable cutting jaw 70 is connected to the handle of the laparoscopy instrument. This movable cutting part of the tip is approximately 1.5 centimeters long. This part can be opened or closed by operating the handle and functions to dissect and encase the dissected tissue along with the fixed jaw 90.

[0036] The cautery ring 80 is connected to the handle of the laparoscopic instrument. This ring can be opened or closed by operating the handle and is attached to the bipolar electrical circuit. Total length of this part is approximately 2.2 centimeters.

[0037] The fixed jaw 90 is connected to the shaft of the laparoscopic instrument and is approximately 2.2 centimeters long. This jaw is also attached to the bipolar electrical circuit. This part is fixed to the instrument and cannot be opened or closed by operating the handle but functions to dissect and encase the dissected tissue along with the movable cutting jaw 70.

[0038] The preferred diameter of the tip is 7 millimeters. Fixed lower jaw 90 is 7 millimeters wide. Ring shape cautery jaw 80 is 7 millimeters wide and the cup shape movable cutting jaw 70 is 5 millimeters wide. Difference in the width of the ring shape cautery jaw 80 and cup shape cutting jaw 70 allows for at least one-millimeter margin.

#### OPERATION OF THE INVENTION

[0039] Jaws of the tip device are opened. Tissue is grasped assuring that the entire tissue is in the jaws of the device. The cauterizing jaw is closed.

[0040] The surgeon then actuates the bipolar cautery and cauterizes the tissue. The surgeon then engages the cutting mechanism until the tissue is completely dissected and traps the dissected portion of the tissue into the jaws. The cautery jaw is then opened slightly, instrument is pulled back and the jaw is closed. The specimen is removed by pulling the device back and bringing it out of the body. The specimen is retrieved after jaws are opened.

[0041] It is to be understood that both the foregoing general description and the following detailed description are exemplary and explanatory but are not restrictive of the invention.

[0042] The invention in its broader aspects is not limited to the specific details shown and described, and departures may be made from such details without departing from the principles of the invention and without sacrificing its chief advantages.

What is claimed is:

1. A tip for bipolar laparoscopy instrument comprising; a fixed jaw with raised outer edge and connected to the power source for bipolar cautery; a movable ring shape jaw connected to the power source for bipolar cautery; a movable cup shape cutting jaw.
2. A laparoscopy instrument tip as in claim 1 which allows simultaneous manipulation, cauterization, dissection, encasement and removal of entire specimen of body tissue.
3. A laparoscopy instrument tip as in claim 1 which completely encases and protects the dissected tissue until it is removed from the body.
4. A laparoscopy instrument tip as in claim 1 which prevents slippage of body tissue during the procedure.
5. A laparoscopy instrument tip as in claim 1 which contains the dissected tissue in an enclosed cavity prior to the removal from the body.
6. A method of dissecting the tissue comprising; grasping the tissue, cauterizing, dissecting, encasing and removing the specimen with the laparoscopy instrument tip as in claim 1.

\* \* \* \* \*

专利名称(译)	腹腔镜器械尖端和标本采集方法		
公开(公告)号	<a href="#">US20080009858A1</a>	公开(公告)日	2008-01-10
申请号	US11/428836	申请日	2006-07-06
[标]申请(专利权)人(译)	CENTUM RES		
申请(专利权)人(译)	CENTUM研究有限责任公司		
当前申请(专利权)人(译)	CENTUM研究有限责任公司		
[标]发明人	RIZVI SYED		
发明人	RIZVI, SYED		
IPC分类号	A61B18/14		
CPC分类号	A61B18/1445 A61B10/06		
其他公开文献	US8012166		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

摘要(译)

独特的腹腔镜检查仪器尖端和方法，允许同时喘气，烧灼，解剖，收容，封闭和移除身体组织。在一个工具中提供了用于在封闭腔中抓握，保持，操纵，烧灼，解剖，包裹和移除组织的机构，从而允许容易，安全和快速地执行该过程。

