


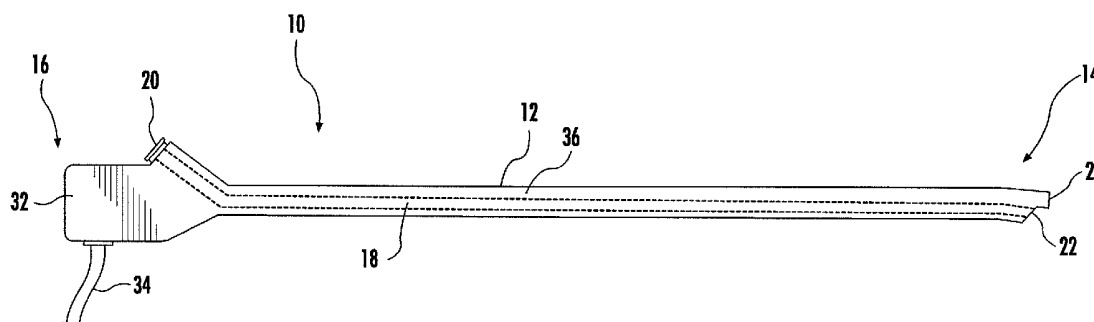

US 20140275762A1

(19) **United States**(12) **Patent Application Publication**
Irby, III(10) **Pub. No.: US 2014/0275762 A1**(43) **Pub. Date: Sep. 18, 2014**(54) **URETEROSCOPE AND ASSOCIATED
METHOD FOR THE MINIMALLY INVASIVE
TREATMENT OF URINARY STONES**(71) Applicant: **The Charlotte-Mecklenburg Hospital
Authority d/b/a Carolinas Healthcare
System, Charlotte, NC (US)**(72) Inventor: **Pierce B. Irby, III, Charlotte, NC (US)**(21) Appl. No.: **13/827,045**(22) Filed: **Mar. 14, 2013****Publication Classification**(51) **Int. Cl.**
A61B 18/26 (2006.01)
A61B 1/005 (2006.01)
A61M 25/09 (2006.01)
A61B 1/06 (2006.01)
A61B 1/00 (2006.01)
A61B 1/307 (2006.01)
A61B 1/018 (2006.01)
A61B 1/04 (2006.01)(52) **U.S. Cl.**CPC **A61B 18/26** (2013.01); **A61B 1/018**
(2013.01); **A61B 1/005** (2013.01); **A61B 1/042**
(2013.01); **A61B 1/0669** (2013.01); **A61B**
1/00071 (2013.01); **A61B 1/00016** (2013.01);
A61B 1/00045 (2013.01); **A61B 1/307**
(2013.01); **A61M 25/09** (2013.01)
USPC **600/103**; 600/104; 600/108(57) **ABSTRACT**

A passively flexible ureteroscope having a diameter of less than about 2.5 millimeters is provided. The ureteroscope may help overcome many of the problems associated with the prior art devices and methods for removing kidney stones. The ureteroscope includes an elongate member having a distal portion, a proximal portion, and an inner conduit that extends longitudinally between the proximal and distal portions. The elongate member is made from a passively flexible material that is capable of being inserted and directed through a patient's body cavity, such as the ureter, by manual direction and pressure so that minimal, if any, additional mechanical or steering mechanisms are present. An imaging device and light source are provided at the distal portion of the elongate member to allow for positioning the device with respect to the stone. A laser fiber can be directed through the conduit to destroy a targeted stone.



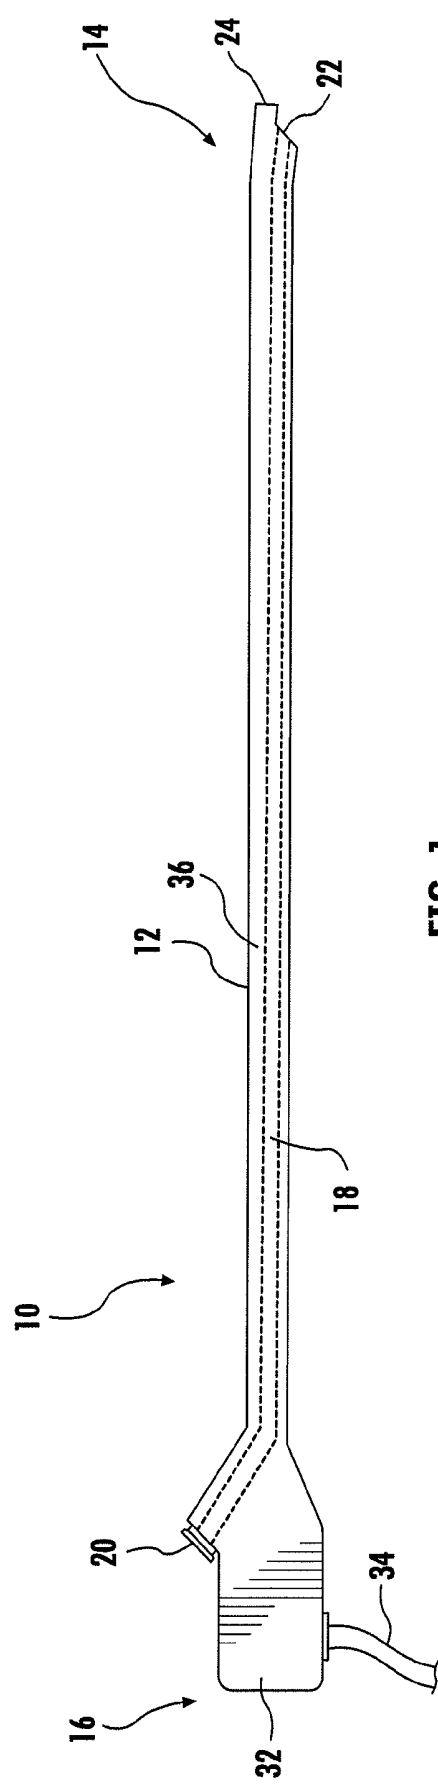


FIG. 1

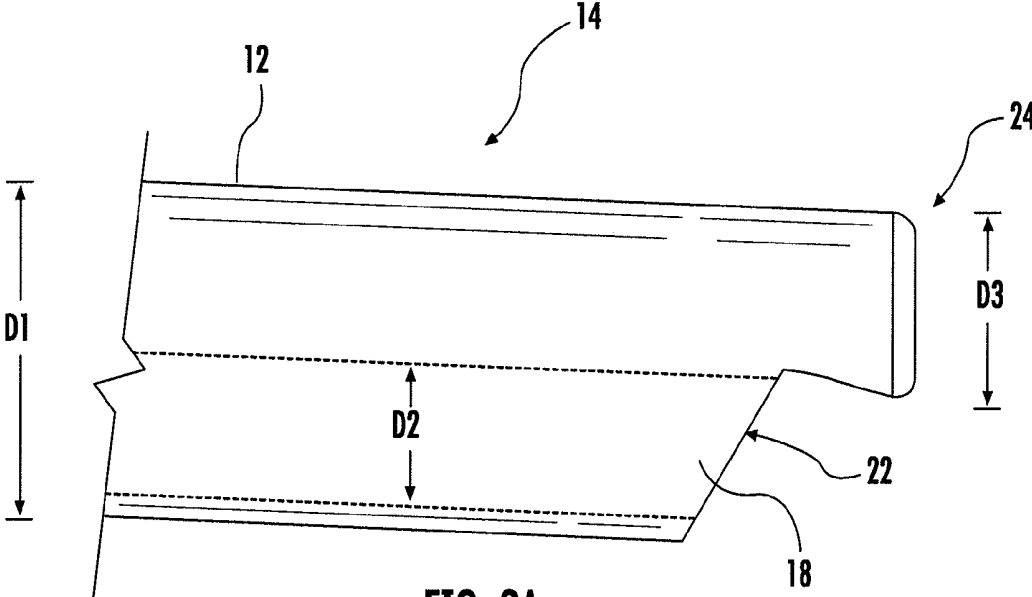


FIG. 2A


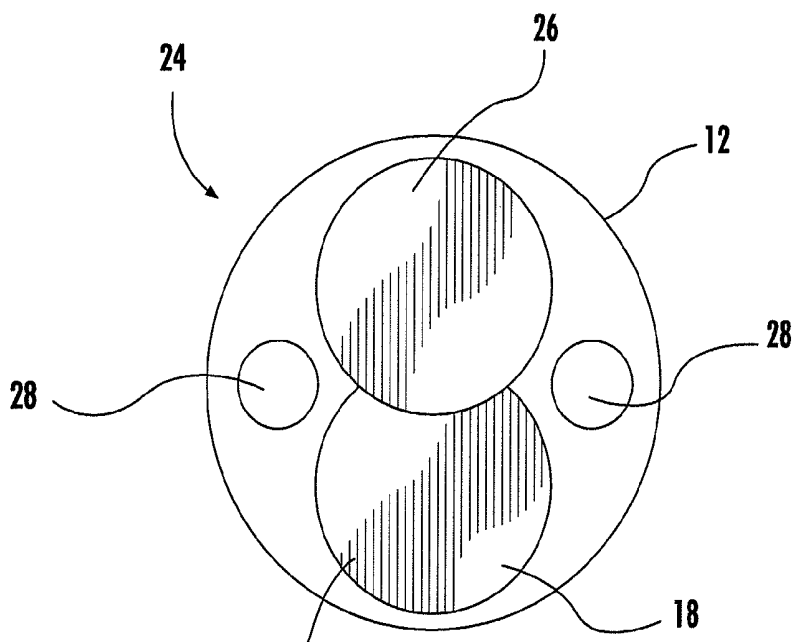


FIG. 2B

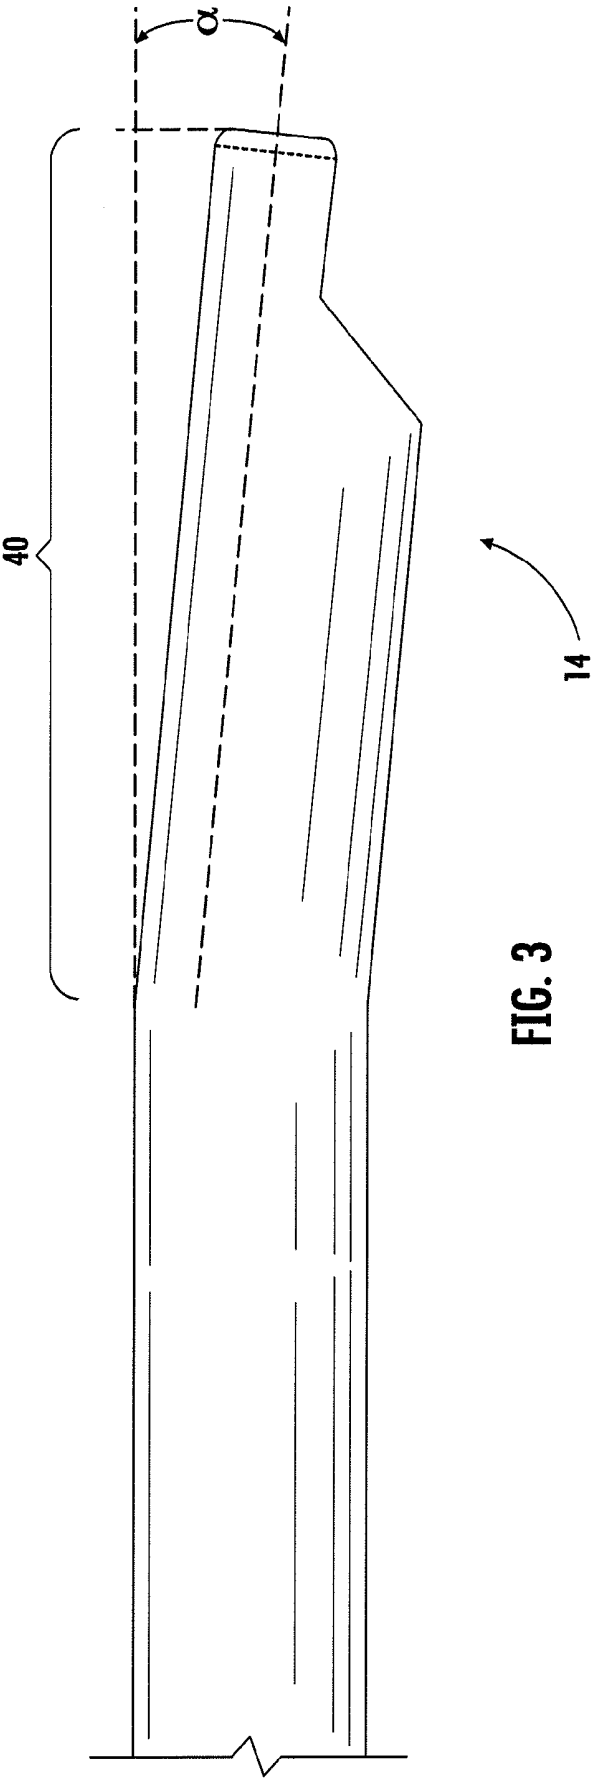

URETEROSCOPE AND ASSOCIATED METHOD FOR THE MINIMALLY INVASIVE TREATMENT OF URINARY STONES

FIELD

[0001] The present invention relates generally to devices and associated methods for the removal of urinary stones from a body cavity, and in particular, to devices and associated methods for removal of urinary stones as a truly outpatient procedure (non-hospital or office).

BACKGROUND

[0002] Kidney stones, which are also commonly known as urinary stones, are solid accumulations and aggregations of matter formed in the kidneys from minerals in the urine.

[0003] Urinary stones are typically classified by their location in the kidney, ureter, or bladder, or by their chemical composition. About 66% of those with kidney stones are men.

[0004] Kidney stones typically leave the body by passage in the urine stream, and many stones are formed and passed without causing symptoms. If stones grow to sufficient size (usually at least 3 millimeters (0.12 in)) they can cause obstruction of the ureter. Ureteral obstruction has many adverse side effects including discomfort, pain, and spasm of the ureter. In many cases, the pain is commonly felt in the flank (the area between the ribs and hip), lower abdomen, and groin (a condition called renal colic). In some instances, renal colic can be associated with nausea, vomiting, fever, blood in the urine, pus in the urine, and painful urination.

[0005] Currently, there are three primary treatment options that account for over 99% of the surgical treatments of kidney stones: 1) percutaneous nephrolithotomy (PNL), 2) shock wave lithotripsy (SWL), and 3) ureteroscopic stone removal (URS).

[0006] PNL is generally used for stones larger than about 20 mm in diameter, and is performed almost exclusively for large stones within the kidneys. SWL is generally used to treat moderate sized stones, for example, stones having diameters ranging from 5 to 20 mm. URS is commonly used for stones having diameters of less than 20 mm. While PNL is used exclusively in the kidneys, SWL and URS can be used to treat kidney stones in the kidney and the ureter.

[0007] In addition to the above techniques, medical expulsion therapy (MET) employs medications to assist in the natural passage of the stone. MET may improve the statistical likelihood of small stone (2-6 mm) passage provided the patient remains comfortable and stable. However, this may require days to weeks of observation in an outpatient mode, waiting with uncertainty for a stone to pass. In the event the stone fails to pass, the patient will often require an operative treatment using URS or SWL. To date, no medications exist to dissolve stones, and stones 7 mm diameter or greater have less than 10% chance of passage.

[0008] SWL and URS are both typically outpatient procedures, as opposed to PNL, which requires a hospitalization of 1-2 days after surgery. SWL is typically performed with intravenous sedation (no formal anesthesia) with no instrumentation inserted into the patient. However, success rates, defined as stone-free with a single treatment session, generally do not exceed 75%. SWL typically depends on the availability of an expensive mobile machine that is rarely hospital owned, traveling around on a scheduled circuit, typically once weekly for most hospitals.

[0009] In contrast, URS is performed in the hospital operating room almost always with general anesthesia. URS is normally available on a daily 24/7 basis, with the insertion of a small fiberoptic telescope into the patient through the natural urinary channels (no incisions). The telescope is advanced up the ureter to the stone, where, if small enough (2-5 mm), it may be extracted intact. Otherwise the stone is fragmented in place with a laser fiber passed through the telescope. Fragments are then irrigated out or extracted mechanically with miniature instruments. Success or stone free rates for URS are 95-98% in experienced hands.

[0010] Due to the outpatient scheduling requirement for SWL, patient selection must be limited to those whose pain is well controlled and who have no other relatively common co-existent emergent contraindications that a stone may present, such as infection or kidney failure. These complicating factors demand a more urgent intervention than SWL can provide.

[0011] Unfortunately, there are currently no surgical treatments that are available as an outpatient in the urologist's office. Each of the above techniques requires formal sedation or anesthesia and the support of in-hospital environment (URS) or mobile lithotripsy unit (SWL). Both of these treatments also require the use of radiologic support in the form of fluoroscopy to monitor the treatment and technical progress during the procedure.

[0012] The relative status quo of the above surgical techniques for urologic stone disease has been the case now for approximately 15 years in the U.S. There have been no significant technological changes in PNL or SWL technology in over 20 years and no new advances are advertised or anticipated from known current research efforts. The most recent innovations in the triad of stone surgery occurred with URS, with the introduction of the first miniaturized flexible ureteroscope around 1995.

[0013] However, current ureteroscopes generally include a requisite mechanical structure so that they can be actively steered and directed through the ureter to the location of the stone, and into the kidney where active steerability of the ureteroscope is mandatory. As a consequence, the sizes of these ureteroscopes have been limited to minimum diameters ranging from 2.5 to 3.0 mm diameter (7.5-9 F). Currently, no passively flexible exists exclusively for ureteral stone surgery.

[0014] Current ureteroscopes rely on the use of laser lithotripsy to destroy stones by passing a tiny laser fiber through a channel within the telescope. The laser fiber transmits laser energy from a separate laser source located in proximity to the surgical field. The laser fiber then is placed in contact with a stone under direct vision and the surgeon reduces the stone to dust and tiny passable fragments. The ureteroscope is removed and the patient awakens, goes to a recovery nursing unit and is discharged home. The sizes of current ureteroscopes are such that the technique of introduction and manipulation would not be tolerated by an un-anesthetized patient.

[0015] Accordingly, there still exists a need for devices and associated methods that can be used to remove urinary stones as a truly outpatient procedure that can be performed in a non-hospital, office environment.

SUMMARY

[0016] Embodiments of the present invention are directed to passively flexible ureteroscopes having diameters of less than about 2.5 millimeters (mm), and in particular is about 2

mm or less. As a result, devices in accordance with embodiments of the present invention may help overcome many of the problems associated with the prior art devices and methods for removing kidney stones. In particular, the availability to surgically treat patients suffering from kidney stones as a non-hospital, truly outpatient procedure may help minimize patient pain and suffering as well as significantly reduce costs typically associated with the surgical treatment of kidney stones.

[0017] In one embodiment, the present invention is directed to a device for removing a stone from a body cavity comprising an elongate member having a distal portion, a proximal portion, and an inner conduit that extends longitudinally between the proximal and distal portions. The elongate member comprises a passively flexible material that is capable of being inserted and directed through a patient's body cavity, such as the ureter, by manual direction and pressure so that minimal, if any, additional mechanical or steering mechanisms are present. As a result, the diameter of the elongate member can be significantly reduced in comparison to conventional ureteroscopes, which in turn, may permit the surgeon to surgically remove kidney stones from the ureter in a truly outpatient process. That is, without the need for hospitalization and anesthetization of the patient.

[0018] Suitable materials for the elongate member may include a wide variety of polymers including silicone rubber, nitinol, nylon, polyurethane, and polyethylene terephthalate (PETE) latex, polytetrafluoroethylene (TEFLON®), hydrophilic polymers, and thermoplastic elastomers. In one particular embodiment, the elongate member comprises a flexible silicone material, wherein the elongate member is passively flexible and has a diameter that is less than about 2.5 mm.

[0019] In one embodiment, the device also includes a port disposed towards the proximal portion of the elongate member and an opening disposed at the distal portion of the elongate member. The port and opening are in communication with each other via the conduit. The conduit, which functions as a working channel, can be used to introduce various devices, such as an irrigation tube, laser fiber, basket, and the like, into a desired location with respect to a targeted kidney stone. In one embodiment, the optical device comprises a charged coupled device or fiber optics.

[0020] In addition, the device includes an optical device disposed towards the proximal portion of the elongate member, and at least one light source disposed towards the proximal portion of the elongate member. The optical device and the light source cooperate to provide the surgeon images of the stone so that the laser fiber can be properly positioned and the surgeon can monitor the status of the procedure.

[0021] In some embodiments, the elongate member may include an outer coating comprising a hydrophilic material, such as polyurethane.

[0022] In a further aspect, the invention is directed to a method of removing a kidney stone from a patient in need thereof, the method comprising the steps of: inserting a cystoscope into a bladder of a patient; identifying a kidney stone in a ureter of the patient; positioning a guidewire in close proximity to the stone; providing a ureteroscope in accordance with at least one embodiment of the present invention; traveling the ureteroscope over the guidewire to position the ureteroscope in close proximity to the stone; removing the guidewire; obtaining an image of the ureter with the optical device of the ureteroscope; positioning the ureteroscope so

that a center of mass of the stone is centered in the image; passing a laser fiber through the ureteroscope so that the laser fiber is in close proximity to the stone; activating the laser fiber to fragment the stone.

[0023] In some embodiments, the step of identifying the kidney stone may be performed with the assistance of an imaging procedure, such as fluoroscopic imaging.

[0024] Aspects of the present invention may provide advantages over currently available treatment methods for the treatment of kidney stones. In particular, the availability to surgically treat patients suffering from kidney stones as a non-hospital, truly outpatient procedure may help minimize patient pain and suffering as well as significantly reduce costs typically associated with the surgical treatment of kidney stones.

BRIEF DESCRIPTION OF THE SEVERAL VIEWS OF THE DRAWING(S)

[0025] Having thus described the invention in general terms, reference will now be made to the accompanying drawings, which are not necessarily drawn to scale, and wherein:

[0026] FIG. 1 is a side view of a device in accordance with at least one embodiment of the present invention;

[0027] FIG. 2A is a partial side view of the distal portion of the device of FIG. 1;

[0028] FIG. 2B is a front view of the distal portion of the device of FIG. 1; and

[0029] FIG. 3 is a partial side view on alternative embodiment of the device of FIG. 1.

DETAILED DESCRIPTION

[0030] The present invention now will be described more fully hereinafter with reference to the accompanying drawings, in which some, but not all embodiments of the inventions are shown. Indeed, these inventions may be embodied in many different forms and should not be construed as limited to the embodiments set forth herein; rather, these embodiments are provided so that this disclosure will satisfy applicable legal requirements. Like numbers refer to like elements throughout.

[0031] With reference to FIG. 1, a device for removing a stone from a body cavity that is in accordance with at least one embodiment of the present invention is illustrated and designated with reference number 10. The device 10 comprises an elongate member 12 having a distal portion 14 and a proximal portion 16. The interior of the elongate member 12 includes a longitudinally extending conduit 18 (represented by the dashed lines in FIG. 1) that extends from a port 20 located towards the proximal portion 16 of the elongate member 12 and an opening 22 disposed at the distal portion 14 of the elongate member 12. The conduit is configured to provide communication between the port and the opening.

[0032] The elongate member comprises a passively flexible material so that the device can be inserted and directed through a patient's body cavity, such as the ureter, with minimal, if any, additional mechanical or steering mechanisms that are present in conventional ureteroscopes and cystoscopies. In other words, the term passively flexible means that the elongate material has sufficient flexibility so that it can be maneuvered through the ureter, or other body cavity, without the need for additional steering devices or associated mechanical structures. As a result, the diameter of the elon-

gate member can be significantly reduced in comparison to conventional ureteroscopes. Suitable materials for the elongate member may include a wide variety of polymers including silicone rubber, nitinol, nylon, polyurethane, and polyethylene terephthalate (PETE) latex, polytetrafluoroethylene (TEFLON®), hydrophilic polymers, and thermoplastic elastomers. In one particular embodiment, the elongate member comprises a flexible silicone material. It should be recognized that in some embodiments, the elongate member may include some minimal steering devices and associated structures provided that the minimal size and flexibility of the device is maintained.

[0033] Turning now to FIGS. 2A and 2B, a partial view of the elongate member is shown. As shown in FIG. 2A, the diameter D1 (or width) of the elongate member is generally less than about 2.5 millimeters (mm), and in particular is about 2 mm or less. In some embodiments, the diameter D1 is from about 1.7 to 2.2 mm, and more particularly, about 2 mm.

[0034] The diameter D2 (or width) of the conduit 18 is desirably large enough to allow for irrigation as well as the insertion of a guide wire or laser fiber. In some embodiments, the diameter D2 is less than 1.25 mm, and preferably less than about 1 mm, and more preferably, about 0.7 to 1 mm, with a size of about 1 mm being most preferred.

[0035] The overall length of the elongate member is desirably sufficient so that it can be inserted and directed to a desired location in a body cavity. For example, in applications directed to the removal of a kidney stone in the ureter, the length of the elongate member may range from about 35 to 55 centimeters (cm), and in particular, about 40 to 45 cm.

[0036] The distal portion of the elongate member defines a tip portion 24 of the device in which an optical device 26, such as a charged coupled device (CCD), camera, or optical fiber, and a light source 28 is positioned. In this regard, FIG. 2B shows a front view of the medical device 10 in which the light source 28 and optical device 26 are positioned in the tip portion 24 of the elongate member. The optical device and light source will typically be connected to an external power source, control device (e.g., a processor) via one or more connectors, such as wires, that extend through one or more additional conduits (not shown) that extend longitudinally through the elongate member.

[0037] In the illustrated embodiment, the light source and optical device are shown as being disposed above the opening 22 to the conduit. However, it should be recognized that other configurations may be utilized in the practice of the invention. As shown in FIG. 2A, the overall diameter D3 (or width) of the optical device may be about 1 to 1.5 mm, and in particular, about 1.1 to 1.3 mm. Preferably, the diameter D3 is about 1.2 mm or less.

[0038] The optical device 26 is generally positioned such that it is located for enabling imaging of forward regions of the body cavity in which the device is positioned. In one embodiment, optical device may be arranged for focusing incident light onto a CCD for generation of a signal which is communicated to an external display, for example a monitor, television or the like. The signal provided by the optical device is preferably digital, although other formats such as analogue signals may be used. In one embodiment, the signal is communicated to the display by conductors such as electrical wires or an optical fiber carrying a modulated signal.

[0039] Other embodiments may include wireless transmission means, for example a miniature radio transmitter, which is adapted to receive a signal from the optical device and

transmit the signal through the body of the patient to a receiver located externally of the patient. This embodiment advantageously dispenses with the requirement for electrical conductors to connect the optical device to a display. In still other embodiments, the device may include a transmitter positioned towards a proximal portion of the device, such as in a handle, so that the signal can be transmitted from the transmitter to the display, such as through a radio transceiver or similar device. In this embodiment, the optical device may be connected to the transmitter through conductors, such as electrical wires.

[0040] In some embodiments, the optical device may comprise an optical fiber. In particular, visualization within the body cavity may be achieved utilizing one or more optic fibers arranged in the same manner as the electrical conductors associated with a CCD. Preferably, a bundle of optic fibers will be used. Generally, the optic fibers will terminate at the distal tip of the elongate member. In one embodiment, the distal ends of the optical fibers are arranged with one or more lenses held in the casing, for feeding light incident upon the lens into the fibers. The light is transmitted by means of internal reflection along the length of the optical fiber to proximal ends. Light processing means, such as processor, disposed at the proximal ends of the optical fibers receive the light and derive therefrom an image for display upon the display device in a manner known to those skilled in the art.

[0041] The light source is preferably disposed proximate the optical device, or is integral therewith, so as to illuminate the region of the body cavity to be imaged. In exemplary embodiments the light source takes the form of a miniature globe, a diode, or for instance an optical fiber positioned so as to communicate light from an external light source. In the case of optical fibers, the size of a bundle of optical fibers may generally have a diameter from about 0.25 to 0.6 mm and, in particular, from about 0.4 to 0.5 mm.

[0042] Referring back to FIG. 1, the device 10 may include a handle 32 disposed towards the proximal end of the elongate member. The handle may also include an inlet/outlet 34 for one or more conductors, such as wires, for providing power and communications to the light source and optical device. In an alternative embodiment, the handle may include a power source, such as a battery, and a transceiver for facilitating wireless communication between the optical device and an external display device.

[0043] In one embodiment, the outer surface 36 of the elongate member may include an outer sheath, such as a polymeric coating, that substantially covers the outer surface of the elongate member. In one embodiment, the sheath may comprise a polymer coating including but not limited to such substances as polyurethane (e.g., polyurethane 55D and 90A) or polytetrafluoroethylene, or silicone. In a preferred embodiment, the sheath includes a hydrophilic coating.

[0044] As noted previously, the conduit 18 is desirably large enough to allow for irrigation as well as the insertion of a guide wire or laser fiber. In particular, the conduit also commonly referred to as a "working channel" provides a means through which the body cavity can be irrigated via a saline or similar solution, and means for positioning a laser fiber in close proximity to a stone to be targeted for removal. The port 20 through which access to the conduit is obtained, can be any conventional port, such as a standard Luer-lok. In one embodiment, an irrigation tubing can be introduced into the conduit via the port.

[0045] In some embodiments, the distal portion of the elongate member may be slightly angled so as to provide better maneuvering and positioning of the medical device within the body cavity. In this regard, FIG. 3 illustrates an embodiment of the invention in which the distal portion of the elongate member includes an angled portion 40 that is slightly angled relative to the remaining portion of the elongate member. As shown in FIG. 3 the angle defined by the angled portion is identified as angle α . Angle α can generally range from about 3° to 8° , and in particular is about 5° . With rotational manipulation of the slightly angled tip, the tip may be directed in a 360° fashion to address a stone in the lumen of the ureter.

[0046] Advantageously, medical devices in accordance with the present invention can be used to treat patients suffering from kidney stones of less than 20 mm. As a result, the invention may help avoid problems associated with prior treatment methods that typically require hospitalization.

[0047] In a typical procedure according to the present invention, the patient undergoes conscious sedation (with or without supplemental oral sedation) while in the supine position (male patient) or lithotomy position (female patient). Initial endoscopy on the patient is then performed with a standard flexible cystoscope, also using local gel anesthesia as per standard current outpatient or office protocol. The cystoscope is advanced per urethra into the bladder and the bladder is inspected. The location of the stone within the ureter is identified and confirmed. Preferably, the location is confirmed by pre-procedural imaging.

[0048] In some embodiments, it may also be desirable to perform this part of the procedure with the assistance of fluoroscopic imaging. Radiographic (fluoroscopic) study of the involved ureter may be performed by the gentle retrograde injection of contrast into the ureteral orifice in the bladder through a standard ureteral catheter, such as a 5 F catheter (retrograde ureterogram).

[0049] After the stone has been located and identified, a guidewire is advanced through the working channel of the cystoscope. In one particular embodiment, the guidewire (e.g., a standard GLIDEWIRE®) may be advanced through the previously inserted catheter. Preferably the guidewire is a standard 0.035" or less (e.g., from 0.025"-0.035") hydrophilic guidewire. Once the guidewire is positioned in the desired location relative to the stone, the catheter is removed leaving the guidewire in place. In an alternative embodiment, the cystoscope may also be removed at this time.

[0050] The device 10 (also referred to herein as a ureteroscope) is now passed over the guidewire and into the bladder and up the ureter until the stone is encountered. In a preferred embodiment, positioning of the ureteroscope is assisted with fluoroscopic imaging. The guidewire is now removed and irrigation (normal saline) is initiated through the conduit of the ureteroscope.

[0051] The ureteroscope may now be manipulated either forward or backward by the surgeon's hand. Rotational manipulation may be achieved by the use of a modified torque device (e.g., Cook Urological) applied to the ureteroscope. The optical device of the ureteroscope can now be used to obtain images of the patient's ureter with the assistance of the light source. As noted previously, the optical device is configured to provide images via a display device.

[0052] By a combination of longitudinal and rotational manipulation, the stone will be engaged in a "center of mass" view. Once a satisfactory "sight picture" is achieved with the optical device wherein the stone is centered in view, a laser

fiber (e.g., standard 270 micron holmium laser fiber) will be passed through the conduit of the ureteroscope. With the laser fiber in direct contact with the stone, the laser is activated and fired at standard energy settings (typically 6-10 Hz at 600-800 mJ). Once the stone is fragmented sufficiently, the laser will be discontinued and removed from the ureteroscope. Stone fragments may be cleared by passage of a 1.9 F stone basket through the conduit and withdrawing the fragments into the bladder. At this point, the ureteroscope can be removed from within the patient.

[0053] In a further aspect of the invention, a ureteral stent (6 F) can be positioned in the patient's ureter. In this aspect, (the cystoscope is reintroduced if previously removed) and a guidewire is then passed into the ureter under fluoroscopic imaging. The guidewire is then advanced to the level of the kidney. A ureteral stent (6 F) is then passed over the guidewire until a proximal end of the stent is in the kidney, and a distal end of the stent remains in the bladder. At this point the cystoscope is removed and the procedure is completed.

[0054] Generally, it may be desirable to monitor the patient in a holding area for up to one hour and discharged home to follow-up in one week. The stent ensures that the ureter remains patent in the post-procedure period until the patient returns to the office for follow-up. This is typically after one week for a brief removal of the stent in similar fashion using the cystoscope, requiring only local topical gel anesthesia.

[0055] From the foregoing discussion, it is evident that the present invention provides many advantages over currently available treatment methods for the treatment of kidney stones. In particular, the availability to surgically treat patients suffering from kidney stones as a non-hospital, truly outpatient procedure may help minimize patient pain and suffering as well as significantly reduce costs typically associated with the surgical treatment of kidney stones.

[0056] Many modifications and other embodiments of the inventions set forth herein will come to mind to one skilled in the art to which these inventions pertain having the benefit of the teachings presented in the foregoing descriptions and the associated drawings. Therefore, it is to be understood that the inventions are not to be limited to the specific embodiments disclosed and that modifications and other embodiments are intended to be included within the scope of the appended claims. Although specific terms are employed herein, they are used in a generic and descriptive sense only and not for purposes of limitation.

That which is claimed:

1. A device for removing a stone from a body cavity comprising:

an elongate member having a distal portion, a proximal portion, and an inner conduit extending longitudinally between the proximal and distal portions, wherein the elongate member is passively flexible and has a diameter that is less than about 2.5 mm;

a port disposed towards the proximal portion of the elongate member and in communication with the conduit;

an opening disposed at the distal portion of the elongate member and in communication with the conduit;

an optical device disposed towards the proximal portion of the elongate member; and

at least one light source disposed towards the proximal portion of the elongate member.

2. The device according to claim 1, wherein the elongate member includes an outer coating comprising a hydrophilic material.

3. The device according to claim 1, wherein the coating comprises polyurethane.

4. The device according to claim 1, wherein the diameter of the elongate member is from about 1.7 to 2.2 mm.

5. The device according to claim 1, wherein the optical device is positioned above the conduit.

6. The device according to claim 1, wherein the optical device comprises a charged coupled device or fiber optics.

7. The device according to claim 1, wherein the diameter of the elongate member is 2 mm or less, and the diameter of the conduit is about 1 mm or less.

8. The device according to claim 1, wherein the optical device is in wireless communication with a display device.

9. The device according to claim 1, wherein the elongate member comprises silicone rubber, nitinol, nylon, polyurethane, polyethylene terephthalate (PETE) latex, polytetrafluoroethylene, a hydrophilic polymer, a thermoplastic elastomer, or combinations thereof.

10. A method of removing a kidney stone from a patient in need thereof, the method comprising the steps of:

inserting a cystoscope into a bladder of a patient;

identifying a kidney stone in a ureter of the patient;

positioning a guidewire in close proximity to the stone;

providing a ureteroscope in accordance with the device of claim 1;

traveling the ureteroscope over the guidewire to position the ureteroscope in close proximity to the stone;

removing the guidewire;

obtaining an image of the ureter with the optical device of the ureteroscope;

positioning the ureteroscope so that a center of mass of the stone is centered in the image;

passing a laser fiber through the ureteroscope so that the laser fiber is in close proximity to the stone;

activating the laser fiber to fragment the stone.

* * * * *

专利名称(译)	输尿管镜及相关方法治疗泌尿系结石的微创治疗		
公开(公告)号	US20140275762A1	公开(公告)日	2014-09-18
申请号	US13/827045	申请日	2013-03-14
[标]申请(专利权)人(译)	夏洛特-梅克伦堡医院(商业用名：卡罗来纳保健系统)		
申请(专利权)人(译)	夏洛特 - 梅克伦堡医院管理局D / B / A卡罗来纳州的医疗系统		
当前申请(专利权)人(译)	夏洛特 - 梅克伦堡医院管理局D / B / A卡罗来纳州的医疗系统		
[标]发明人	IRBY III PIERCE B		
发明人	IRBY, III, PIERCE B.		
IPC分类号	A61B18/26 A61B1/005 A61M25/09 A61B1/06 A61B1/00 A61B1/307 A61B1/018 A61B1/04		
CPC分类号	A61B1/04 A61M25/09 A61B2017/22074 A61B2017/22084 A61B2019/5217 A61B2217/007 A61B18/26 A61B1/00016 A61B1/00045 A61B1/00071 A61B1/005 A61B1/018 A61B1/042 A61B1/0669 A61B1/307 A61B17/22 A61B1/01 A61B17/221 A61B2018/00511 A61B2018/00982 A61B2090/3614		
其他公开文献	US9775675		
外部链接	Espacenet USPTO		

摘要(译)

提供了一种直径小于约2.5毫米的被动柔性输尿管镜。输尿管镜可以帮助克服与现有技术装置和用于去除肾结石的方法相关的许多问题。输尿管镜包括细长构件，细长构件具有远端部分，近端部分和在近端部分和远端部分之间纵向延伸的内导管。细长构件由被动柔性材料制成，该材料能够通过手动方向和压力插入并引导通过患者的体腔，例如输尿管，从而存在最小的（如果有的话）额外的机械或转向机构。成像装置和光源设置在细长构件的远端部分处，以允许装置相对于石头定位。可以引导激光纤维穿过导管以破坏目标石头。

