



US010363055B2

(12) **United States Patent**
Beira et al.

(10) **Patent No.:** **US 10,363,055 B2**
(45) **Date of Patent:** **Jul. 30, 2019**

(54) **ARTICULATED HAND-HELD INSTRUMENT**

(71) Applicant: **DistalMotion SA**, Lausanne (CH)

(72) Inventors: **Ricardo Daniel Rita Beira**, Lausanne (CH); **Michael Urs Friedrich**, Bern (CH)

(73) Assignee: **DistalMotion SA**, Epalinges (CH)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 104 days.

(21) Appl. No.: **15/564,194**

(22) PCT Filed: **Apr. 11, 2016**

(86) PCT No.: **PCT/IB2016/000542**

§ 371 (c)(1),

(2) Date: **Oct. 3, 2017**

(87) PCT Pub. No.: **WO2016/162751**

PCT Pub. Date: **Oct. 13, 2016**

(65) **Prior Publication Data**

US 2018/0125519 A1 May 10, 2018

Related U.S. Application Data

(60) Provisional application No. 62/280,736, filed on Jan. 20, 2016, provisional application No. 62/145,454, filed on Apr. 9, 2015.

(51) **Int. Cl.**

A61B 17/29 (2006.01)

A61B 34/00 (2016.01)

(Continued)

(52) **U.S. Cl.**

CPC **A61B 17/2909** (2013.01); **A61B 17/00234** (2013.01); **A61B 17/29** (2013.01);

(Continued)

(58) **Field of Classification Search**

CPC **A61B 2017/291**; **A61B 2017/2927**; **A61B 17/2909**; **A61B 34/71**; **A61B 17/29**;

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,764,301 A 9/1956 Goertz et al.

2,771,199 A 11/1956 Jelatis

(Continued)

FOREIGN PATENT DOCUMENTS

CN 101584594 A 11/2009

CN 101637402 A 2/2010

(Continued)

OTHER PUBLICATIONS

U.S. Appl. No. 13/878,924, filed May 17, 2013.

(Continued)


Primary Examiner — Katherine M Shi

(74) *Attorney, Agent, or Firm* — Foley & Lardner LLP; Christopher C. Bolten; Nicola A. Pisano

(57) **ABSTRACT**

An articulated hand-held medical instrument is provided. The instrument is primarily intended to be used in minimally invasive surgical procedures. The articulated instrument comprises a master-slave architecture whereby user hand movements on a proximal handle element are replicated on a distal end-effector. The proximal handle comprises a number of handle links joined by handle joints that correspond to a number of end-effector links joined by end-effector joints. The articulated hand-held medical instrument can be used in standard laparoscopic procedures in various port arrangements and through the use of standard equipment such as trocars, and movements inside the patient's body may be tracked using available endoscopic cameras.

20 Claims, 43 Drawing Sheets

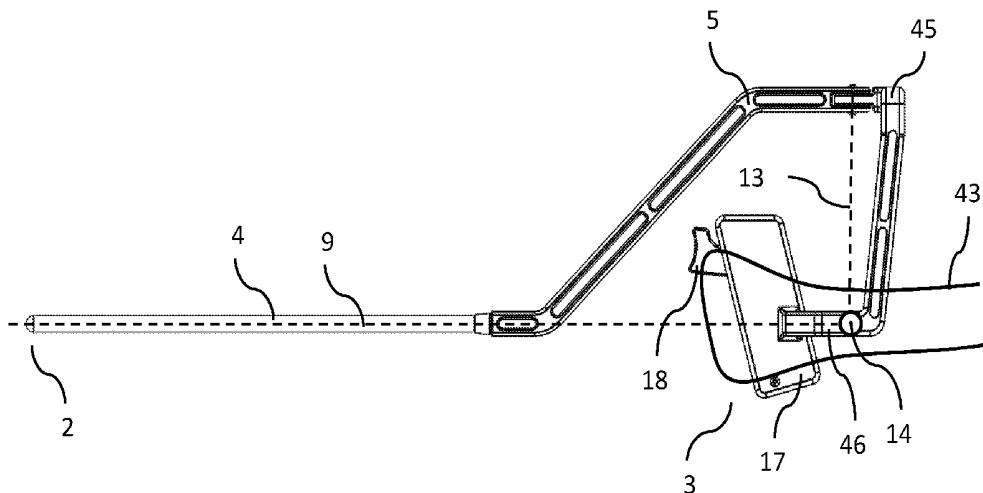

- (51) **Int. Cl.**
A61B 17/00 (2006.01)
A61B 90/00 (2016.01)
- (52) **U.S. Cl.**
 CPC *A61B 34/71* (2016.02); *A61B 2017/0046*
 (2013.01); *A61B 2017/00424* (2013.01); *A61B*
2017/00738 (2013.01); *A61B 2017/291*
 (2013.01); *A61B 2017/2927* (2013.01); *A61B*
2017/2929 (2013.01); *A61B 2017/2948*
 (2013.01); *A61B 2090/0813* (2016.02)
- (58) **Field of Classification Search**
 CPC *A61B 34/70*; *A61B 17/00234*; *A61B*
2017/00424; *A61B 2017/00738*; *A61B*
34/25; *A61B 34/37*; *A61B 34/77*; *A61B*
90/50; *B25J 13/02*; *B25J 3/02*
 USPC 606/1, 130, 205
 See application file for complete search history.
- (56) **References Cited**
 U.S. PATENT DOCUMENTS
- | | | | | | |
|--------------|---------|---------------------|--------------|---------|-------------------|
| 2,774,488 A | 12/1956 | Goertz | 6,587,750 B2 | 7/2003 | Gerbi et al. |
| 2,846,084 A | 8/1958 | Goertz et al. | 6,594,552 B1 | 7/2003 | Nowlin et al. |
| 3,065,863 A | 11/1962 | Saunders, Jr. | 6,671,581 B2 | 12/2003 | Niemeyer et al. |
| 3,095,096 A | 6/1963 | Chesley | 6,699,177 B1 | 3/2004 | Wang et al. |
| 3,212,651 A | 10/1965 | Specht et al. | 6,786,896 B1 | 9/2004 | Madhani et al. |
| 3,261,480 A | 7/1966 | Haaker et al. | 6,788,999 B2 | 9/2004 | Green |
| 3,297,172 A | 1/1967 | Haaker et al. | 6,840,938 B1 | 1/2005 | Morley et al. |
| 3,391,801 A | 7/1968 | Haaker | 6,850,817 B1 | 2/2005 | Green |
| 3,425,569 A | 2/1969 | Haaker | 6,852,107 B2 | 2/2005 | Wang et al. |
| 4,221,516 A | 9/1980 | Haaker et al. | 6,879,880 B2 | 4/2005 | Nowlin et al. |
| 4,756,655 A | 7/1988 | Jameson | 6,902,560 B1 | 6/2005 | Morley et al. |
| 5,147,357 A | 9/1992 | Rose et al. | 6,951,535 B2 | 10/2005 | Ghodoussi et al. |
| 5,176,352 A | 1/1993 | Braun | 6,991,627 B2 | 1/2006 | Madhani et al. |
| 5,207,114 A | 5/1993 | Salisbury et al. | 6,994,708 B2 | 2/2006 | Manzo |
| 5,209,747 A | 5/1993 | Knoepfler | 7,048,745 B2 | 5/2006 | Tierney et al. |
| 5,304,203 A | 4/1994 | El-Mallawany et al. | 7,083,571 B2 | 8/2006 | Wang et al. |
| 5,308,358 A | 5/1994 | Bond et al. | 7,090,637 B2 | 8/2006 | Danitz et al. |
| 5,330,502 A | 7/1994 | Hassler et al. | 7,101,363 B2 | 9/2006 | Nishizawa et al. |
| 5,368,606 A | 11/1994 | Marlow et al. | 7,204,836 B2 | 4/2007 | Wagner et al. |
| 5,383,888 A | 1/1995 | Zvenyatsky et al. | 7,232,440 B2 | 6/2007 | Dumbauld et al. |
| 5,484,435 A | 1/1996 | Fleenor et al. | 7,306,597 B2 | 12/2007 | Manzo |
| 5,599,151 A | 2/1997 | Daum et al. | 7,316,681 B2 | 1/2008 | Madhani et al. |
| 5,603,723 A | 2/1997 | Aranyi et al. | 7,338,513 B2 | 3/2008 | Lee et al. |
| 5,631,973 A | 5/1997 | Green | 7,364,582 B2 | 4/2008 | Lee |
| 5,649,956 A | 7/1997 | Jensen et al. | 7,373,219 B2 | 5/2008 | Nowlin et al. |
| 5,710,870 A | 1/1998 | Ohm et al. | 7,398,707 B2 | 7/2008 | Morley et al. |
| 5,716,352 A | 2/1998 | Viola et al. | 7,481,824 B2 | 1/2009 | Boudreaux et al. |
| 5,735,874 A | 4/1998 | Measamer et al. | 7,594,912 B2 | 9/2009 | Cooper et al. |
| 5,784,542 A | 7/1998 | Ohm et al. | 7,608,039 B1 | 10/2009 | Todd |
| 5,797,900 A | 8/1998 | Madhani et al. | 7,615,002 B2 | 11/2009 | Rothweiler et al. |
| 5,810,716 A | 9/1998 | Mukherjee et al. | 7,615,067 B2 | 11/2009 | Lee et al. |
| 5,810,805 A | 9/1998 | Sutcu et al. | 7,674,255 B2 | 3/2010 | Braun |
| 5,828,813 A | 10/1998 | Ohm | 7,699,855 B2 | 4/2010 | Anderson et al. |
| 5,908,436 A | 6/1999 | Cuschieri et al. | 7,756,036 B2 | 7/2010 | Druke et al. |
| 5,951,587 A | 9/1999 | Qureshi et al. | 7,819,894 B2 | 10/2010 | Mitsuishi et al. |
| 5,976,122 A | 11/1999 | Madhani et al. | 7,824,401 B2 | 11/2010 | Manzo et al. |
| 6,026,701 A | 2/2000 | Reboulet | 7,828,798 B2 | 11/2010 | Buysse et al. |
| 6,132,368 A | 10/2000 | Cooper | 7,890,211 B2 | 2/2011 | Green |
| 6,197,017 B1 | 3/2001 | Brock et al. | 7,914,521 B2 | 3/2011 | Wang et al. |
| 6,206,903 B1 | 3/2001 | Ramans | 7,976,458 B2 | 7/2011 | Stefanchik et al. |
| 6,233,504 B1 | 5/2001 | Das et al. | 8,048,084 B2 | 11/2011 | Schneid |
| 6,281,651 B1 | 8/2001 | Haanpaa et al. | 8,105,320 B2 | 1/2012 | Manzo |
| 6,312,435 B1 | 11/2001 | Wallace et al. | 8,114,017 B2 | 2/2012 | Bacher |
| 6,331,181 B1 | 12/2001 | Tierney et al. | 8,137,263 B2 | 3/2012 | Marescaux et al. |
| 6,358,249 B1 | 3/2002 | Chen et al. | 8,142,447 B2 | 3/2012 | Cooper et al. |
| 6,361,534 B1 | 3/2002 | Chen et al. | 8,224,485 B2 | 7/2012 | Unsworth |
| 6,364,879 B1 | 4/2002 | Chen et al. | 8,287,469 B2 | 10/2012 | Stefanchik et al. |
| 6,371,952 B1 | 4/2002 | Madhani et al. | 8,292,889 B2 | 10/2012 | Cunningham et al. |
| 6,394,998 B1 | 5/2002 | Wallace et al. | 8,306,656 B1 | 11/2012 | Schaible et al. |
| 6,435,794 B1 | 8/2002 | Springer | 8,308,738 B2 | 11/2012 | Nobis et al. |
| 6,459,926 B1 | 10/2002 | Nowlin et al. | 8,332,072 B1 | 12/2012 | Schaible et al. |
| 6,491,701 B2 | 12/2002 | Tierney et al. | 8,336,751 B2 | 12/2012 | Scirica |
| 6,554,844 B2 | 4/2003 | Lee et al. | 8,347,754 B1 | 1/2013 | Veltri et al. |
| | | | 8,353,898 B2 | 1/2013 | Lutze et al. |
| | | | 8,357,161 B2 | 1/2013 | Mueller |
| | | | 8,382,742 B2 | 2/2013 | Hermann et al. |
| | | | 8,403,832 B2 | 3/2013 | Cunningham et al. |
| | | | 8,418,904 B2 | 4/2013 | Wenchell et al. |
| | | | 8,423,186 B2 | 4/2013 | Itkowitz et al. |
| | | | 8,496,152 B2 | 7/2013 | Viola |
| | | | 8,523,900 B2 | 9/2013 | Jinno et al. |
| | | | 8,540,748 B2 | 9/2013 | Murphy et al. |
| | | | 8,562,592 B2 | 10/2013 | Conlon et al. |
| | | | 8,568,444 B2 | 10/2013 | Cunningham |
| | | | 8,579,176 B2 | 11/2013 | Smith et al. |
| | | | 8,591,397 B2 | 11/2013 | Berkelman et al. |
| | | | 8,603,077 B2 | 12/2013 | Cooper et al. |
| | | | 8,617,203 B2 | 12/2013 | Stefanchik et al. |
| | | | 8,663,270 B2 | 3/2014 | Donnigan et al. |
| | | | 8,668,689 B2 | 3/2014 | Dumbauld et al. |
| | | | 8,668,702 B2 | 3/2014 | Awtar et al. |
| | | | 8,696,666 B2 | 4/2014 | Sanai et al. |
| | | | 8,709,000 B2 | 4/2014 | Madhani et al. |
| | | | 8,761,930 B2 | 6/2014 | Nixon |
| | | | 8,768,509 B2 | 7/2014 | Unsworth |
| | | | 8,792,688 B2 | 7/2014 | Unsworth |
| | | | 8,801,752 B2 | 8/2014 | Fortier et al. |
| | | | 8,816,628 B2 | 8/2014 | Nowlin et al. |
| | | | 8,818,560 B2 | 8/2014 | Kishi |

(56)

References Cited

U.S. PATENT DOCUMENTS

8,821,480	B2	9/2014	Burbank	2010/0305595	A1	12/2010	Hermann
8,828,046	B2	9/2014	Stefanchik et al.	2010/0318099	A1	12/2010	Itkowitz et al.
8,845,517	B2	9/2014	Russo	2010/0318101	A1	12/2010	Choi
8,845,622	B2	9/2014	Paik et al.	2010/0331859	A1	12/2010	Omori
8,870,867	B2	10/2014	Walberg et al.	2011/0087236	A1	4/2011	Stokes et al.
8,887,979	B2	11/2014	Mastri et al.	2011/0087238	A1	4/2011	Wang et al.
8,894,674	B2	11/2014	Balanev et al.	2011/0213346	A1	9/2011	Morley et al.
8,930,027	B2	1/2015	Schaible et al.	2011/0230867	A1	9/2011	Hirschfeld et al.
8,945,098	B2	2/2015	Seibold et al.	2011/0275901	A1	11/2011	Shelton, IV
8,961,499	B2	2/2015	Paik et al.	2011/0276084	A1	11/2011	Shelton, IV
8,961,514	B2	2/2015	Garrison	2011/0290854	A1	12/2011	Timm et al.
8,968,187	B2	3/2015	Kleyman et al.	2011/0301419	A1	12/2011	Craft et al.
8,989,844	B2	3/2015	Cinquin et al.	2012/0027762	A1	2/2012	Schofield
8,992,564	B2	3/2015	Jaspers	2012/0031114	A1	2/2012	Mueller et al.
9,023,015	B2	5/2015	Penna	2012/0049623	A1	3/2012	Nakayama
9,033,998	B1	5/2015	Schaible et al.	2012/0095298	A1	4/2012	Stefanchik et al.
9,044,238	B2	6/2015	Orszulak	2012/0116163	A1	5/2012	Lutze et al.
9,084,606	B2	7/2015	Greep	2012/0132018	A1	5/2012	Tang et al.
9,113,861	B2	8/2015	Martin et al.	2012/0143173	A1	6/2012	Steege et al.
9,149,339	B2	10/2015	Unsworth	2012/0158014	A1	6/2012	Stefanchik et al.
9,307,894	B2	4/2016	Von Grunberg et al.	2012/0191245	A1	7/2012	Fudaba et al.
9,474,580	B2	10/2016	Hannaford et al.	2012/0209292	A1	8/2012	Devengenzo et al.
9,480,531	B2	11/2016	Von Grunberg	2012/0253326	A1	10/2012	Kleyman
9,492,240	B2	11/2016	Itkowitz et al.	2012/0277762	A1	11/2012	Lathrop et al.
9,696,700	B2	7/2017	Beira et al.	2012/0283745	A1	11/2012	Goldberg et al.
10,071,488	B2	9/2018	Robinson et al.	2012/0289973	A1	11/2012	Prisco et al.
10,092,359	B2	10/2018	Beira et al.	2012/0289974	A1	11/2012	Rogers et al.
10,265,129	B2	4/2019	Beira	2012/0296341	A1	11/2012	Seibold et al.
2002/0040217	A1	4/2002	Jinno	2013/0123805	A1	5/2013	Park et al.
2002/0049367	A1	4/2002	Irion et al.	2013/0144274	A1	6/2013	Stefanchik et al.
2002/0072736	A1	6/2002	Tierney et al.	2013/0172713	A1	7/2013	Kirschenman
2003/0155747	A1	8/2003	Bridges	2013/0245643	A1	9/2013	Woodard et al.
2003/0208186	A1	11/2003	Moreyra	2013/0245647	A1	9/2013	Martin et al.
2004/0049205	A1	3/2004	Lee et al.	2013/0282027	A1	10/2013	Woodard et al.
2004/0116906	A1	6/2004	Lipow	2013/0303408	A1	11/2013	Indermuhle
2004/0236316	A1	11/2004	Danitz et al.	2013/0304083	A1	11/2013	Kaercher et al.
2004/0253079	A1	12/2004	Sanchez	2013/0304084	A1	11/2013	Epfl
2005/0096502	A1	5/2005	Khalili	2014/0005681	A1	1/2014	Gee et al.
2005/0204851	A1	9/2005	Morley et al.	2014/0018447	A1	1/2014	McGovern et al.
2005/0240078	A1	10/2005	Kwon et al.	2014/0018780	A1	1/2014	Hirschfeld
2006/0043698	A1	3/2006	Bridges	2014/0076088	A1	3/2014	Berkelman et al.
2006/0178559	A1	8/2006	Kumar et al.	2014/0114481	A1	4/2014	Ogawa et al.
2006/0183975	A1	8/2006	Saadat et al.	2014/0142595	A1	5/2014	Awatar et al.
2006/0219065	A1	10/2006	Jinno et al.	2014/0166023	A1	6/2014	Kishi
2006/0235436	A1	10/2006	Anderson et al.	2014/0180308	A1	6/2014	Von Grunberg
2006/0253109	A1	11/2006	Chu	2014/0188091	A1	7/2014	Vidal et al.
2007/0088340	A1	4/2007	Brock et al.	2014/0188159	A1	7/2014	Steege
2007/0137371	A1	6/2007	Devengenzo et al.	2014/0195010	A1	7/2014	Epfl
2007/0156123	A1	7/2007	Moll et al.	2014/0200561	A1	7/2014	Ingmanson et al.
2007/0208375	A1	9/2007	Nishizawa et al.	2014/0207150	A1	7/2014	Rosa et al.
2007/0299387	A1	12/2007	Williams et al.	2014/0230595	A1	8/2014	Butt et al.
2008/0039255	A1	2/2008	Jinno et al.	2014/0249546	A1	9/2014	Shvartsberg et al.
2008/0046122	A1	2/2008	Manzo et al.	2014/0263541	A1	9/2014	Leimbach et al.
2008/0058776	A1	3/2008	Jo et al.	2014/0263553	A1	9/2014	Leimbach et al.
2008/0071208	A1	3/2008	Voegele et al.	2014/0276950	A1	9/2014	Smaby et al.
2008/0103492	A1	5/2008	Morley et al.	2014/0276951	A1	9/2014	Hourtash et al.
2008/0177285	A1	7/2008	Brock et al.	2014/0276956	A1	9/2014	Crainich et al.
2008/0243106	A1	10/2008	Coe et al.	2014/0350570	A1	11/2014	Lee
2008/0314181	A1	12/2008	Schena	2015/0057499	A1	2/2015	Erden et al.
2009/0036902	A1	2/2009	Dimairo et al.	2015/0057702	A1	2/2015	Edmondson et al.
2009/0198253	A1	8/2009	Omori	2015/0060517	A1	3/2015	Williams
2009/0216248	A1	8/2009	Uenohara et al.	2015/0066018	A1	3/2015	Doll et al.
2009/0216249	A1	8/2009	Jinno et al.	2015/0105821	A1	4/2015	Ward et al.
2009/0247821	A1	10/2009	Rogers	2015/0113933	A1	4/2015	Markt
2009/0248039	A1	10/2009	Cooper et al.	2015/0142018	A1	5/2015	Sniffin et al.
2009/0299141	A1	12/2009	Downey et al.	2015/0150575	A1	6/2015	Hartoumbekis et al.
2010/0004508	A1	1/2010	Naito et al.	2015/0250547	A1	9/2015	Fukushima et al.
2010/0011900	A1	1/2010	Burbank	2015/0265355	A1	9/2015	Prestel et al.
2010/0023025	A1	1/2010	Zeiner et al.	2016/0022365	A1	1/2016	Jensen et al.
2010/0094130	A1	4/2010	Ninomiya et al.	2016/0051274	A1	2/2016	Howell et al.
2010/0121347	A1	5/2010	Jaspers	2016/0151115	A1	6/2016	Karguth et al.
2010/0160929	A1	6/2010	Rogers et al.	2016/0346053	A1	12/2016	Beira
2010/0160940	A1	6/2010	Lutze et al.	2016/0374766	A1	12/2016	Schuh
2010/0170519	A1	7/2010	Romo et al.	2017/0245954	A1	8/2017	Beira
2010/0225209	A1	9/2010	Goldberg et al.	2017/0273749	A1	9/2017	Grover et al.
				2017/0308667	A1	10/2017	Beira et al.
				2017/0360522	A1	12/2017	Beira
				2017/0367778	A1	12/2017	Beira
				2018/0000472	A1	1/2018	Beira

(56)

References Cited

U.S. PATENT DOCUMENTS

2018/0000544 A1 1/2018 Beira
 2018/0000550 A1 1/2018 Beira
 2018/0055583 A1 3/2018 Schuh et al.
 2018/0125519 A1 5/2018 Beira et al.
 2018/0125592 A1 5/2018 Beira
 2018/0242991 A1 8/2018 Beira
 2018/0353252 A1 12/2018 Chassot et al.

FOREIGN PATENT DOCUMENTS

CN 101732093 A 6/2010
 CN 103717355 A 4/2014
 DE 43 03 311 A1 8/1994
 DE 19652792 C2 5/1999
 DE 10314827 B3 4/2004
 DE 10314828 B3 7/2004
 DE 10 2012 222 755 6/2014
 DE 10 2014 205 036 A1 9/2015
 DE 10 2014 205 159 A1 9/2015
 EP 0 595 291 A1 5/1994
 EP 0 621 009 A1 10/1994
 EP 0 677 275 A2 10/1995
 EP 0 776 739 A2 6/1997
 EP 1 254 642 A1 11/2002
 EP 1 279 371 B1 12/2004
 EP 1 886 630 A2 2/2008
 EP 1 889 579 A2 2/2008
 EP 2 058 090 A2 5/2009
 EP 1 977 677 B1 8/2009
 EP 2 095 778 A1 9/2009
 EP 1 889 583 B1 4/2011
 EP 2 377 477 B1 5/2012
 EP 2 473 119 A2 7/2012
 EP 2 305 144 B1 10/2012
 EP 2 044 893 B1 7/2013
 EP 2 653 110 A1 10/2013
 EP 2 679 192 A2 1/2014
 EP 2 736 680 A2 6/2014
 EP 2 777 561 A1 9/2014
 EP 2 783 643 A1 10/2014
 EP 2 837 340 A1 2/2015
 EP 2 837 354 A1 2/2015
 EP 2 554 131 B1 8/2015
 EP 2 979 657 A1 2/2016
 GB 0 969 899 A 9/1964
 JP 2004-041580 A 2/2004
 JP 2007-290096 A 11/2007
 JP 2008-104620 A 5/2008
 JP 2009-018027 A 1/2009
 KR 20110032444 A 3/2011
 KR 20130031403 A 3/2013
 WO WO-82/00611 A1 3/1982
 WO WO-97/43942 A1 11/1997
 WO WO-98/25666 A1 6/1998
 WO WO-03/067341 A2 8/2003
 WO WO-03/086219 A2 10/2003
 WO WO-2004/052171 A2 6/2004
 WO WO-2005/009482 A2 2/2005
 WO WO-2005/046500 A1 5/2005
 WO WO-2006/086663 A2 4/2006
 WO WO-2007/133065 A1 11/2007
 WO WO-2008/130235 A2 10/2008
 WO WO-2009/091497 A2 7/2009
 WO WO-2009/095893 A2 8/2009
 WO WO-2009/145572 A2 12/2009
 WO WO-2009/157719 A2 12/2009
 WO WO-2010/019001 A2 2/2010
 WO WO-2010/030114 A2 3/2010
 WO WO-2010/050771 A2 5/2010
 WO WO-2010/083480 A2 7/2010
 WO WO-2010/096580 A1 8/2010
 WO WO-2010/130817 A1 11/2010
 WO WO-2011/027183 A2 3/2011
 WO WO-2011/123669 A1 10/2011
 WO WO-2012/020386 A1 2/2012

WO WO-2012/049623 A1 4/2012
 WO WO-2013/007784 A1 1/2013
 WO WO-2013/014621 A1 1/2013
 WO WO-2013/014621 A2 1/2013
 WO WO-2014/012780 A1 1/2014
 WO WO-2014/018447 A1 1/2014
 WO WO-2014/067804 A1 5/2014
 WO WO-2014/094716 A1 6/2014
 WO WO-2014/094717 A1 6/2014
 WO WO-2014/094718 A1 6/2014
 WO WO-2014/094719 A1 6/2014
 WO WO-2014/145148 A2 9/2014
 WO WO-2014/156221 A1 10/2014
 WO WO-2014/201010 A1 12/2014
 WO WO-2014/201538 A1 12/2014
 WO WO-2015/081946 A1 6/2015
 WO WO-2015/081947 A1 6/2015
 WO WO-2015/088647 A1 6/2015
 WO WO-2015/088655 A1 6/2015
 WO WO-2015/111475 A1 7/2015
 WO WO-2015/113933 A1 8/2015
 WO WO-2015/129383 A1 8/2015
 WO WO-2015/139674 A1 9/2015
 WO WO-2015/175200 A1 11/2015
 WO WO-2016/030767 A9 3/2016
 WO WO-2016/083189 A1 6/2016
 WO WO-2016/097861 A1 6/2016
 WO WO-2016/097864 A2 6/2016
 WO WO-2016/097868 A1 6/2016
 WO WO-2016/097871 A1 6/2016
 WO WO-2016/097873 A2 6/2016
 WO WO-2016/162751 A1 10/2016
 WO WO-2016/162752 A1 10/2016
 WO WO-2016/183054 A1 11/2016
 WO WO-01/6189284 A1 12/2016
 WO WO-2016/189284 A1 12/2016
 WO WO-2017/015599 A1 1/2017
 WO WO-2017/064301 A1 4/2017
 WO WO-2017/064303 A1 4/2017
 WO WO-2017/064305 A1 4/2017
 WO WO-2017/064306 A1 4/2017

OTHER PUBLICATIONS

U.S. Appl. No. 14/233,184 / U.S. Pat. No. 9,696,700, filed Jan. 16, 2014 / Jul. 4, 2017.
 U.S. Appl. No. 15/116,509, filed Aug. 3, 2016.
 U.S. Appl. No. 15/506,659, filed Feb. 24, 2017.
 U.S. Appl. No. 15/536,539, filed Jun. 15, 2017.
 U.S. Appl. No. 15/536,562, filed Jun. 15, 2017.
 U.S. Appl. No. 15/536,568, filed Jun. 15, 2017.
 U.S. Appl. No. 15/536,573, filed Jun. 15, 2017.
 U.S. Appl. No. 15/536,576, filed Jun. 15, 2017.
 U.S. Appl. No. 15/564,193, filed Oct. 3, 2017.
 U.S. Appl. No. 15/633,611, filed Jun. 26, 2017.
 International Search Report & Written Opinion dated Jul. 10, 2018 in Int'l PCT Patent Appl. Serial No. PCT/IB2018/053272.
 Abbott, et al., "Design of an Endoluminal NOTES Robotic System," IEEE/RSJ International Conference on Intelligent Robots and Systems, San Diego, CA, pp. 410-416 (2007).
 Aesculap Surgical Technologies, Aesculap® Caiman®, Advanced Bipolar Seal and Cut Technology Brochure, 6 pages (retrieved Aug. 31, 2015).
 Arata, et al., "Development of a dexterous minimally-invasive surgical system with augmented force feedback capability," IEEE/RSJ International Conference on Intelligent Robots and Systems, pp. 3207-3212 (2005).
 Ç avuş oğlu, et al., "Laparoscopic Telesurgical Workstation," IEEE Transactions on Robotics and Automation,(15)4:728-739 (1999).
 Charles, et al., Dexterity-enhanced Telerobotic Microsurgery, Advanced Robotics, ICAR '97. Proceedings, 8th Int'l Conference (1997).
 Dachs, et al., "Novel Surgical Robot Design: Minimizing the Operating Envelope Within the Sterile Field," 28th International Conference, IEEE Engineering in Medicine Biology Society, New York, pp. 1505-1508 (2006).

(56)

References Cited

OTHER PUBLICATIONS

- Dario, et al., "Novel Mechatronic Tool for Computer-Assisted Arthroscopy," IEEE Transactions on Information Technology in Biomedicine, 4(1):15-29 (Mar. 2000).
- Focacci, et al., "Lightweight Hand-held Robot for Laparoscopic Surgery," IEEE International Conference on Robotics & Automation, Rome, Italy, pp. 599-604 (2007).
- Guthart, et al., "The Intuitive™ Telesurgery System: Overview and Application," IEEE International Conference on Robotics & Automation, San Francisco, CA, pp. 618-621 (2000).
- Ikuta, et al., "Development of Remote Microsurgery Robot and New Surgical Procedure for Deep and Narrow Space," IEEE International Conference on Robotics & Automation, Taipei, Taiwan, pp. 1103-1108 (2003).
- Ikuta, et al., "Hyper Redundant Miniature Manipulator 'Hyper Finger' for Remote Minimally Invasive Surgery in Deep Area," IEEE International Conference on Robotics & Automation, Taipei, Taiwan, pp. 1098-1102 (2003).
- International Search Report & Written Opinion dated Feb. 2, 2017 in Int'l PCT Patent Appl. Serial No. PCT/IB2016/001286.
- International Search Report & Written Opinion dated Jan. 18, 2013 in Int'l PCT Patent Appl Serial No. PCT/IB2012/053786.
- International Search Report dated Jan. 18, 2013 in Int'l PCT Patent Appl Serial No. PCT/IB2012/053786.
- International Search Report dated Mar. 23, 2012 in Int'l PCT Patent Appl Serial No. PCT/IB2011/054476.
- Ishii, et al., "Development of a New Bending Mechanism and Its Application to Robotic Forceps Manipulator," IEEE International Conference on Robotics & Automation, Rome, Italy, pp. 238-243 (2007).
- International Search Report & Written Opinion dated Feb. 17, 2016 in Int'l PCT Patent Appl Serial No. PCT/IB2015/002095.
- International Search Report & Written Opinion dated May 23, 2016 in Int'l PCT Patent Appl Serial No. PCT/IB2015/002524.
- International Search Report & Written Opinion dated Mar. 23, 2012 in Int'l PCT Patent Appl Serial No. PCT/IB2011/054476.
- International Search Report & Written Opinion dated Mar. 30, 2015 in Int'l PCT Patent Appl Serial No. PCT/EP2015/051473.
- International Search Report & Written Opinion dated Apr. 26, 2016 in Int'l PCT Patent Appl Serial No. PCT/IB2015/002512.
- International Search Report & Written Opinion dated May 24, 2016 in Int'l PCT Patent Appl Serial No. PCT/IB2015/002487.
- International Search Report & Written Opinion dated Jun. 10, 2016 in Int'l PCT Patent Appl Serial No. PCT/IB2015/002533.
- International Search Report & Written Opinion dated Jun. 13, 2016 in Int'l PCT Patent Appl Serial No. PCT/IB2015/002493.
- International Search Report & Written Opinion dated Aug. 25, 2016 in Int'l PCT Patent Appl Serial No. PCT/IB2016/000542.
- International Search Report & Written Opinion dated Sep. 2, 2016 in Int'l PCT Patent Appl Serial No. PCT/IB2016/000543.
- Kobayashi, et al., "Small Occupancy Robotic Mechanisms for Endoscopic Surgery," International Conference on Medical Image Computing and Computer assisted Interventions, pp. 75-82 (2002).
- Lang, et al., Intra-operative robotics: NeuroArm., Acta Neurochir Suppl, 109:231-236 (2011).
- Mayer, et al., "The Endo[PA]R System for Minimally Invasive Robotic Surgery," IEEE/RSJ International Conference on Intelligent Robots and Systems, Sendai, Japan, pp. 3637-3642 (2004).
- Mitsuishi, et al., "Development of a Remote Minimally Invasive Surgical System with Operational Environment Transmission Capability," IEEE International Conference on Robotics & Automation, Taipei, Taiwan, pp. 2663-2670 (2003).
- Mitsuishi, et al., Master-slave robotic platform and its feasibility study for micro-neurosurgery, Int. J. Med. Robot., 9(2):180-9 (2013).
- Morita, et al., Microsurgical robotic system for the deep surgical field: development of a prototype and feasibility studies in animal and cadaveric models, J. Neurosurg., 103(2):320-7 (2005).
- Nakamura, et al., "Multi-DOF Forceps Manipulator System for Laparoscopic Surgery-Mechanism miniaturized & Evaluation of New Interface," 4th International Conference on Medical Image Computing and Computer assisted Interventions (MICCAI2001), pp. 606-613 (2001).
- Peirs, et al., "Design of an advanced tool guiding system for robotic surgery," IEEE International Conference on Robotics & Automation, Taipei, Taiwan, pp. 2651-2656 (2003).
- Sallé, et al., "Optimal Design of High Dexterity Modular MIS Instrument for Coronary Artery Bypass Grafting," IEEE International Conference on Robotics & Automation, New Orleans, LA, pp. 1276-1281 (2004).
- Seibold, et al., "Prototype of Instrument for Minimally Invasive Surgery with 6-Axis Force Sensing Capability," IEEE International Conference on Robotics & Automation, Barcelona, Spain, pp. 496-501 (2005).
- Simaan, et al., "Dexterous System for Laryngeal Surgery: Multi-Backbone Bending Snake-like Slaves for Teleoperated Dexterous Surgical Tool Manipulation," IEEE International Conference on Robotics & Automation, New Orleans, LA, pp. 351-357 (2004).
- Stryker®, Endoscopy, Take a Look Around, Ideal Eyes™ FFD122 HD, Articulating Laparoscope Brochure, 2 pages (2009).
- Swiss Search Report dated Jun. 4, 2012 in Swiss Patent Application No. CH 00702/12.
- Tavakoli, et al., "Force Reflective Master-Slave System for Minimally Invasive Surgery," IEEE/RSJ International Conference on Intelligent Robots and Systems, Las Vegas, NV, pp. 3077-3082 (2003).
- Taylor, et al., "Steady-Hand Robotic System for Microsurgical Augmentation," The International Journal of Robotics Research, 18(12):1201-1210 (1999).
- www.cttc.co/technologies/maestro-non-robotic-dexterous-laposcopic-instrument-writes-providing-seven-degrees, "Maestro: Non-Robotic Dexterous Laproscopic Instrument With a Wrist Providing Seven Degrees of Freedom", accessed Nov. 12, 2015, 4 pages.
- Yamashita, et al., "Development of Endoscopic Forceps Manipulator Using Multi-Slider Linkage Mechanisms," The 1st Asian Symposium on Computer Aided Surgery-Robotic and Image-Guided Surgery, Ibaraki, Japan, 4 pages (2005).
- Zeus, "Robotic Surgical System" available at <http://al-labourboticsurgery.com/zeusrobot.html>.

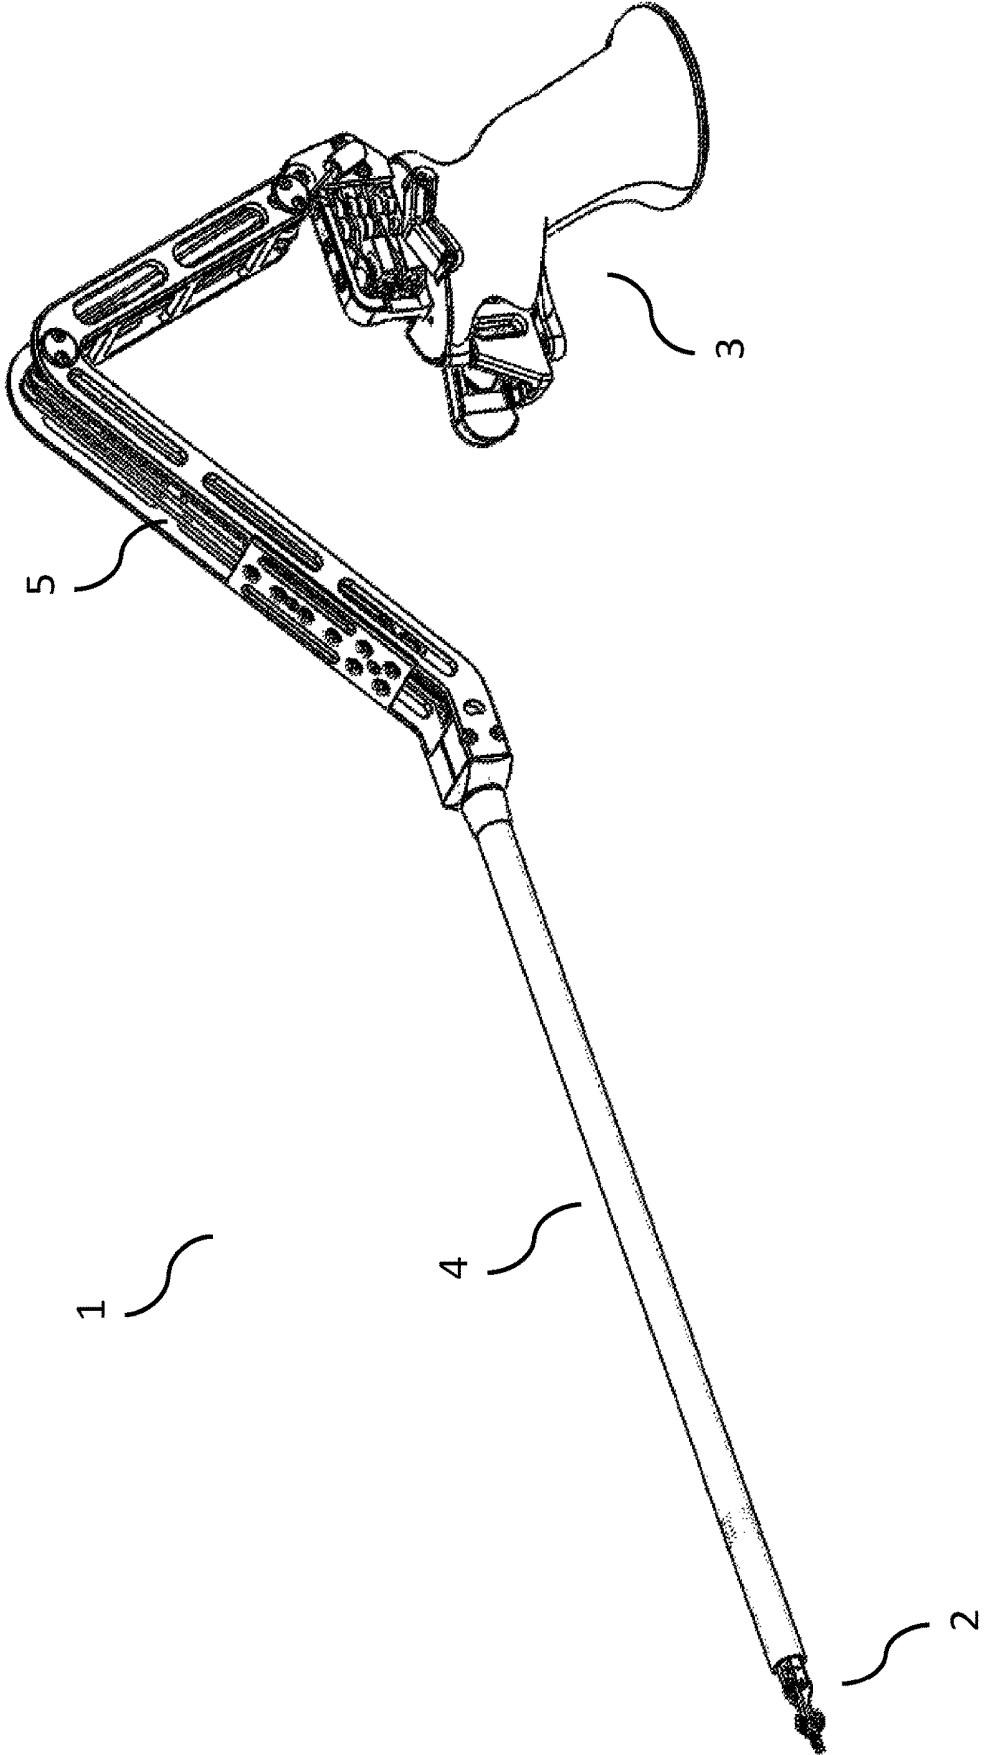


Figure 1

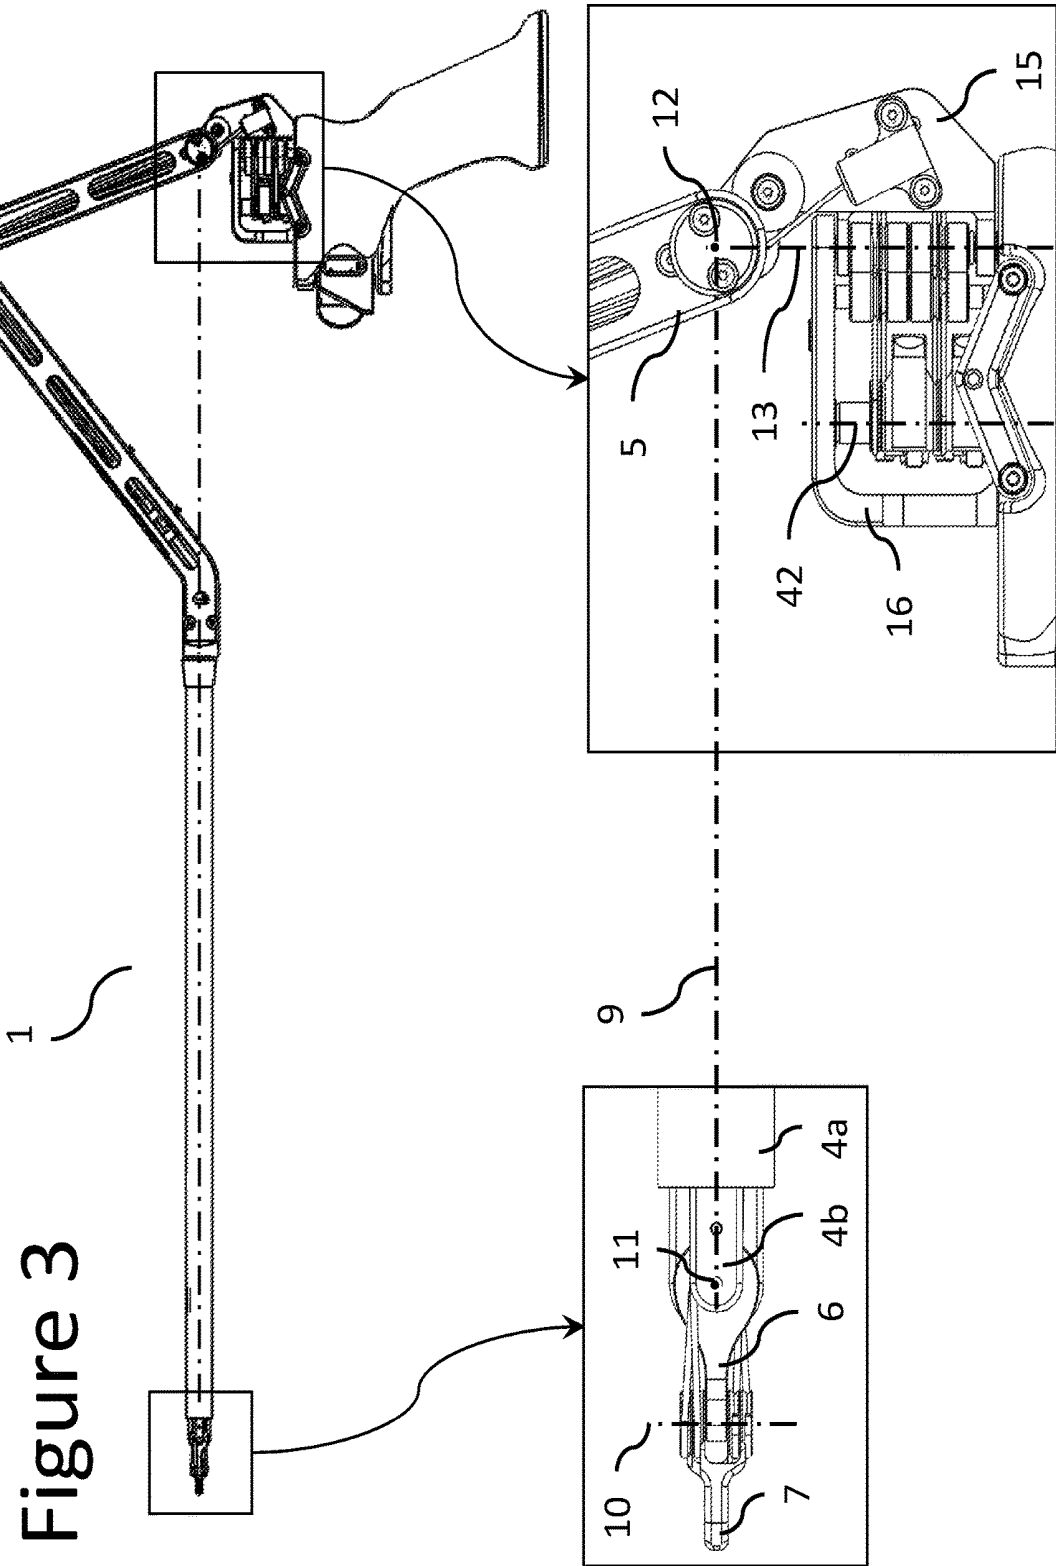


Figure 4

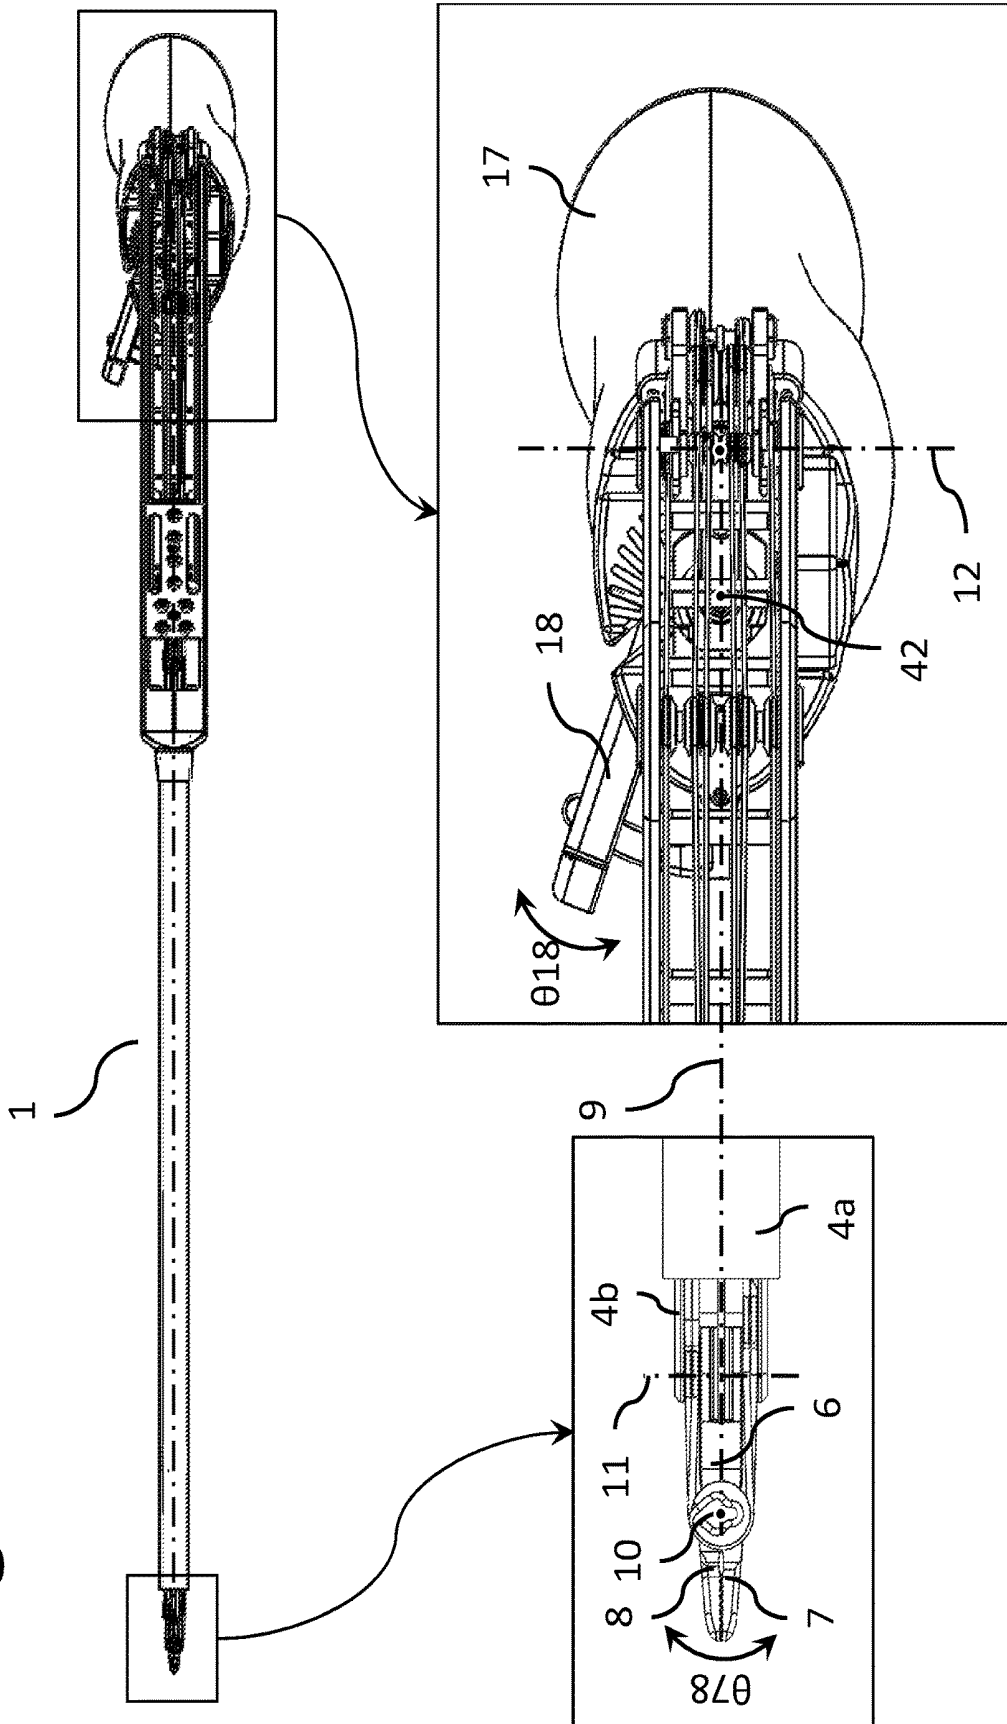


Figure 6

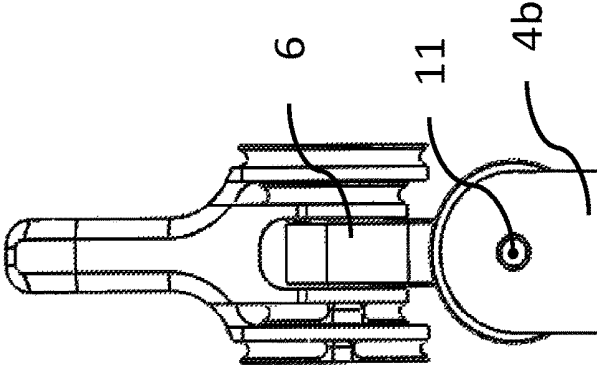


Figure 7

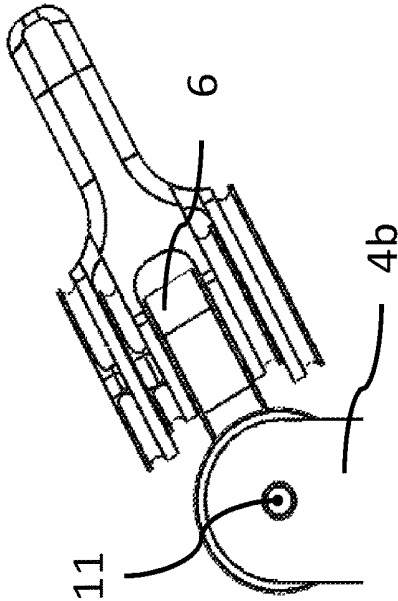


Figure 5

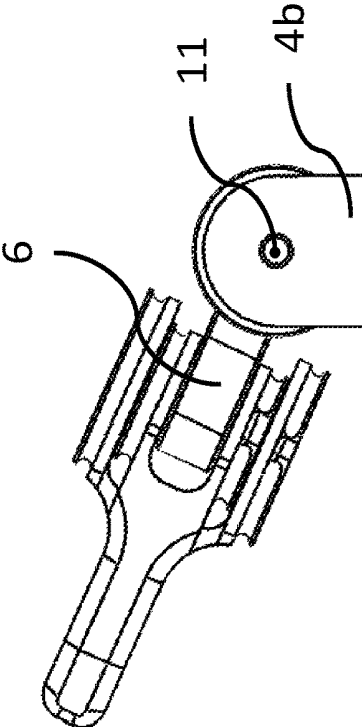


Figure 9

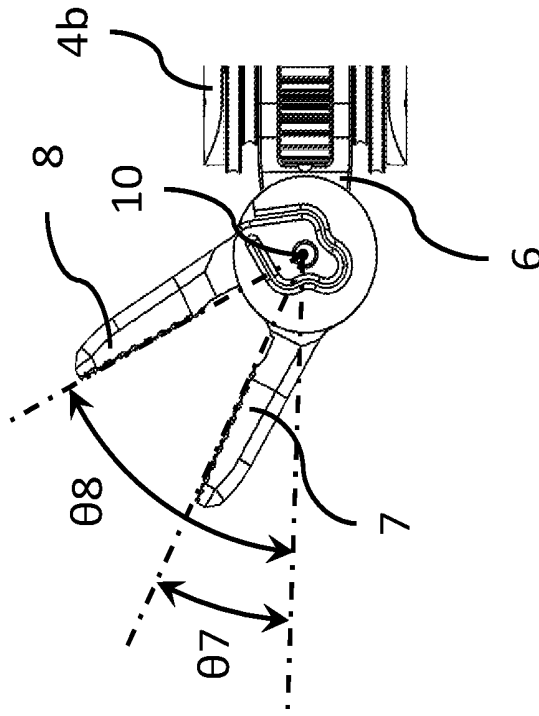


Figure 8

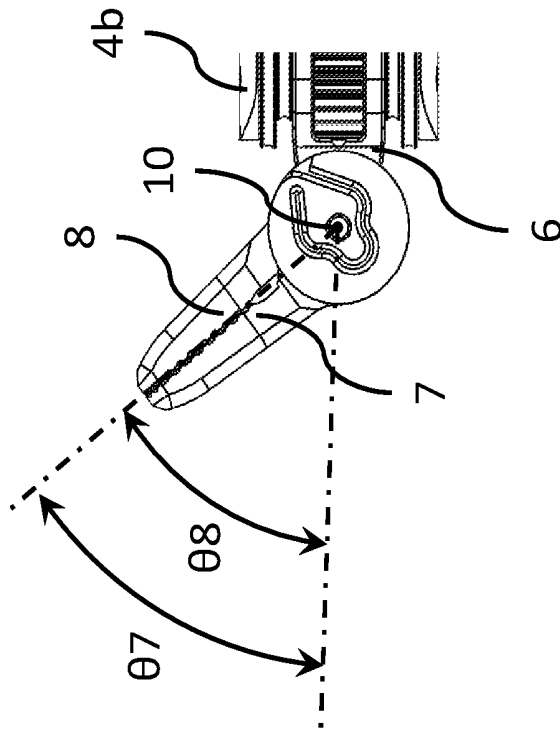


Figure 10

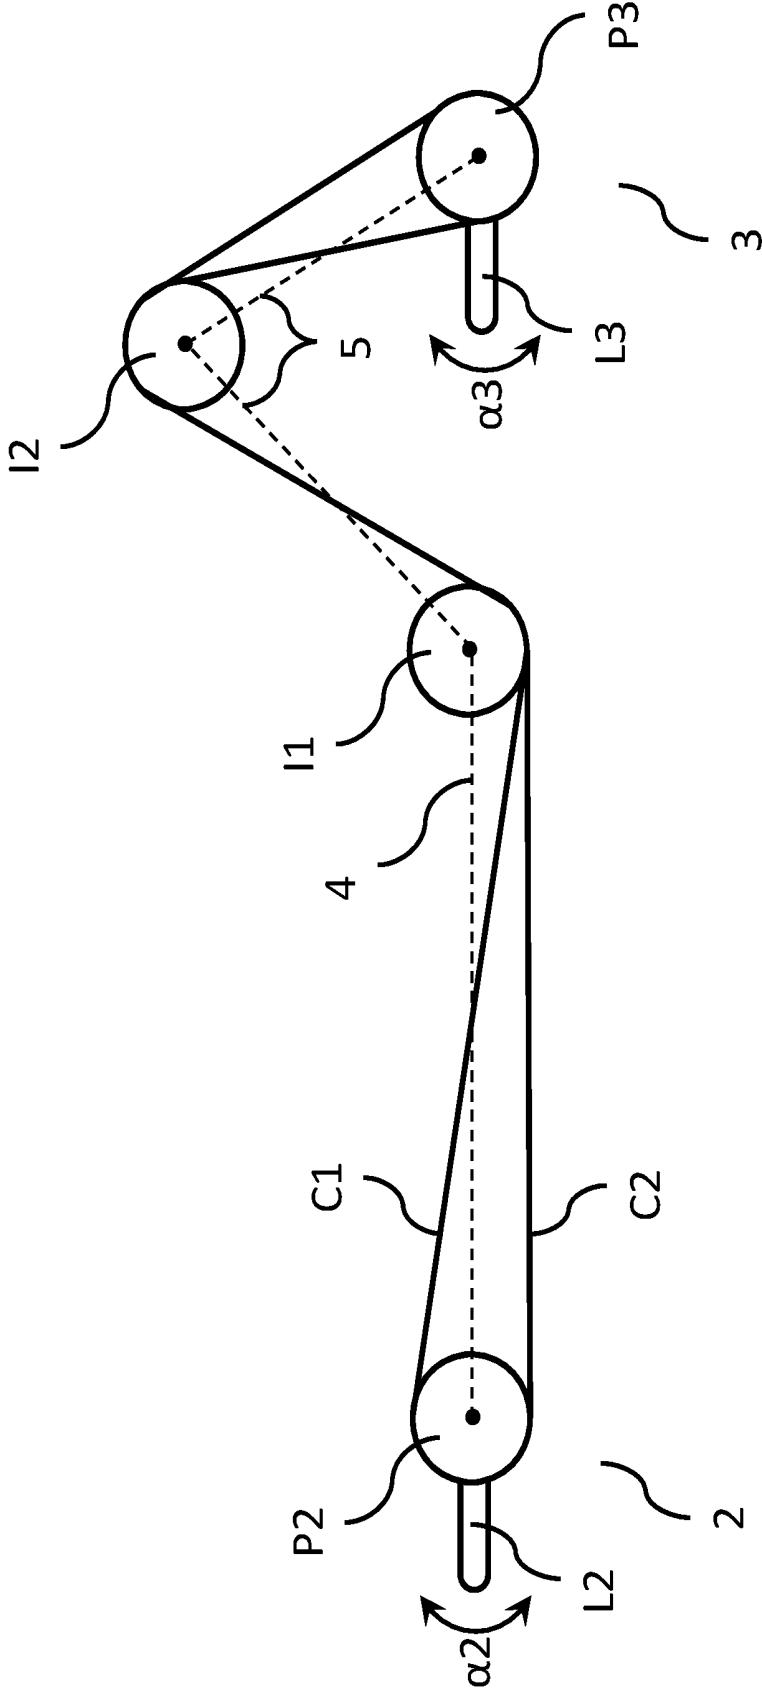
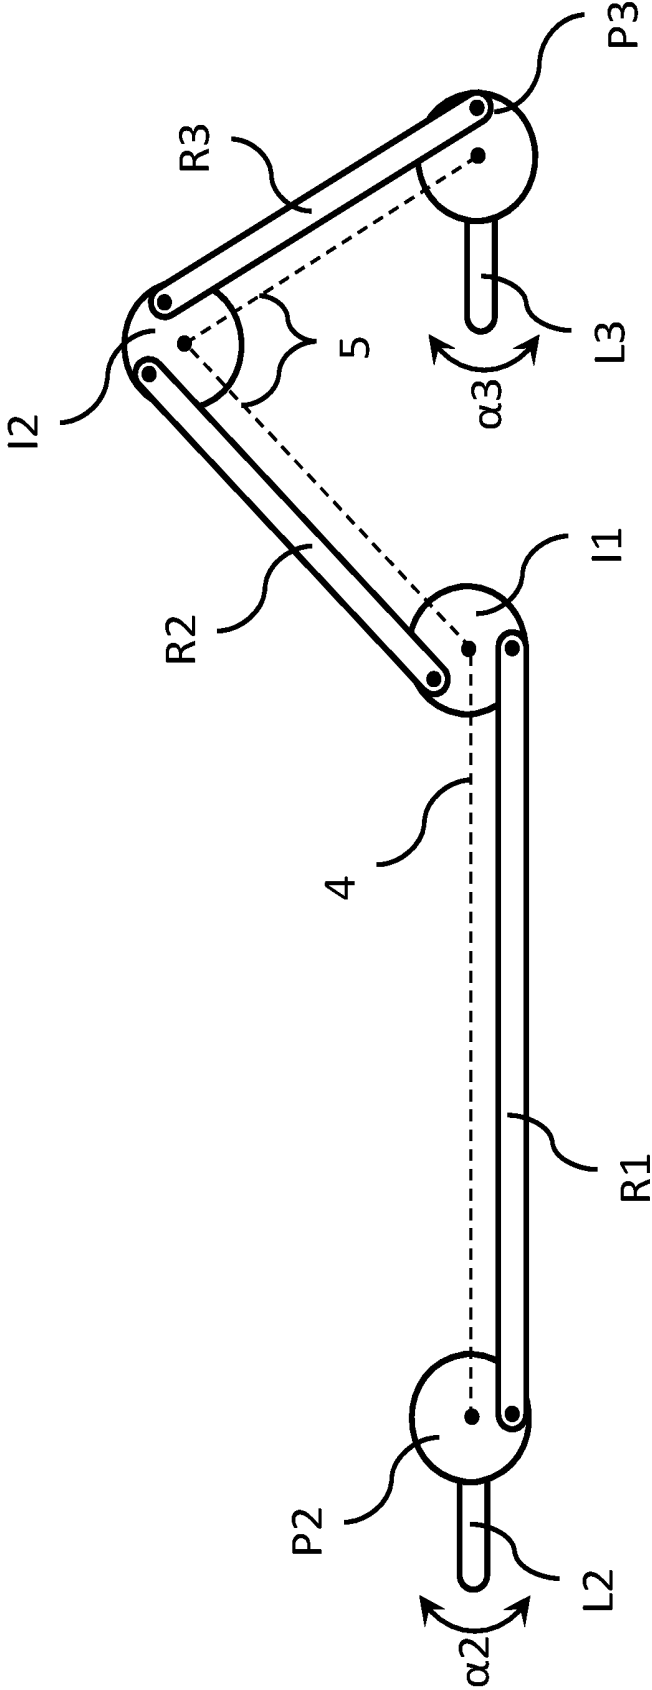


Figure 11



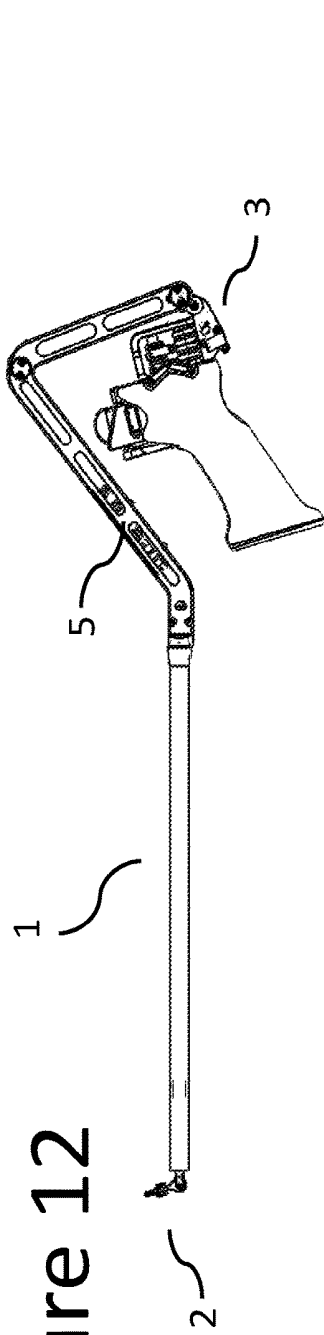


Figure 12

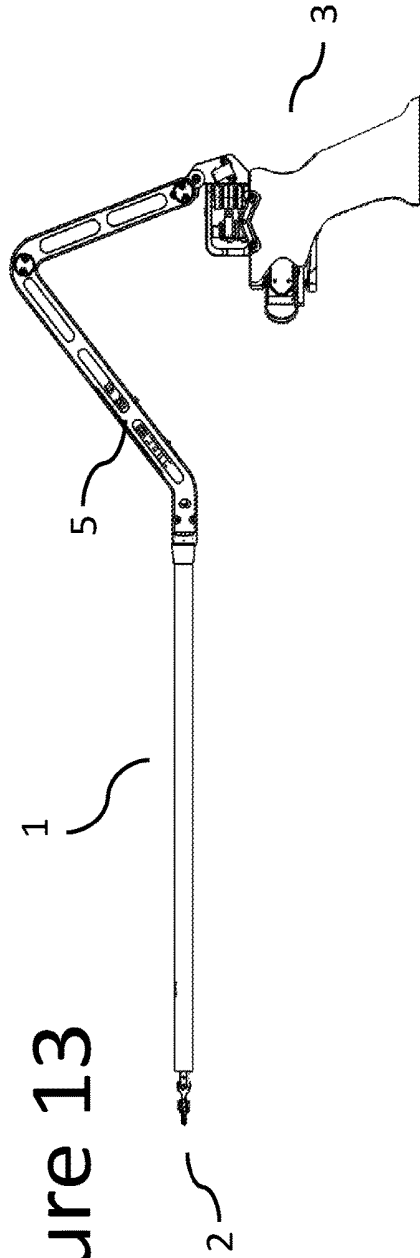


Figure 13

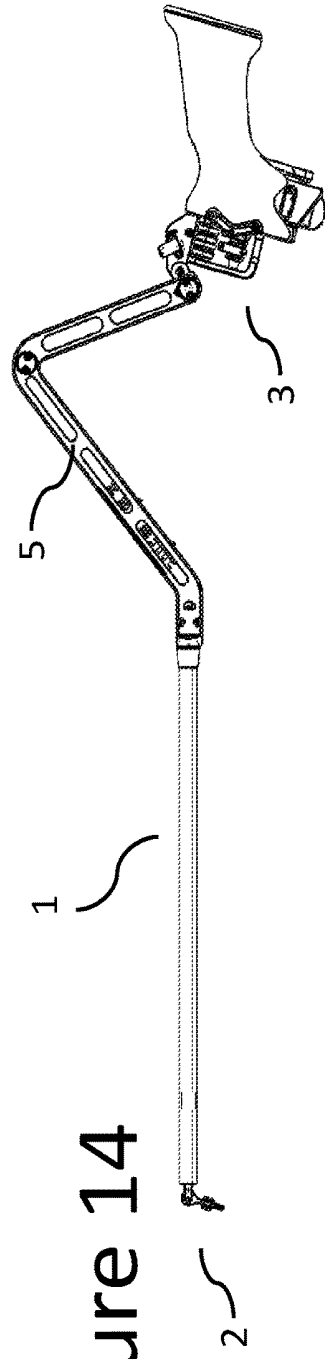


Figure 14

Figure 15

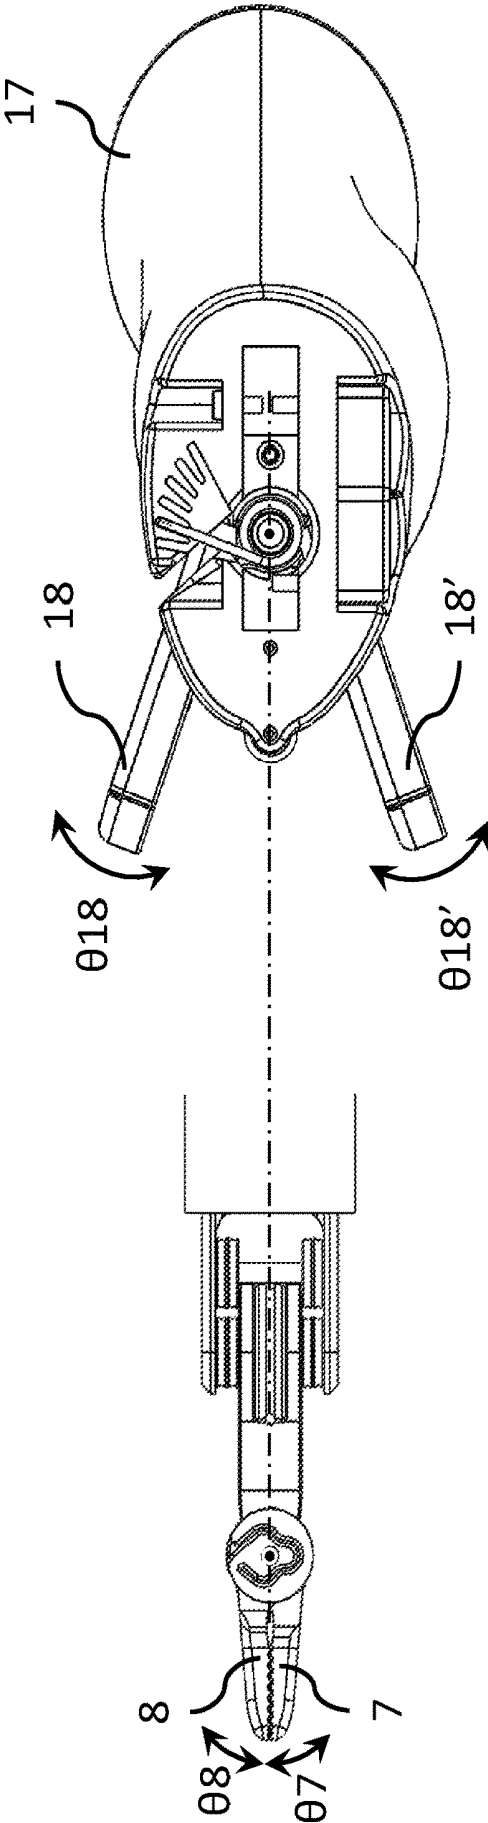
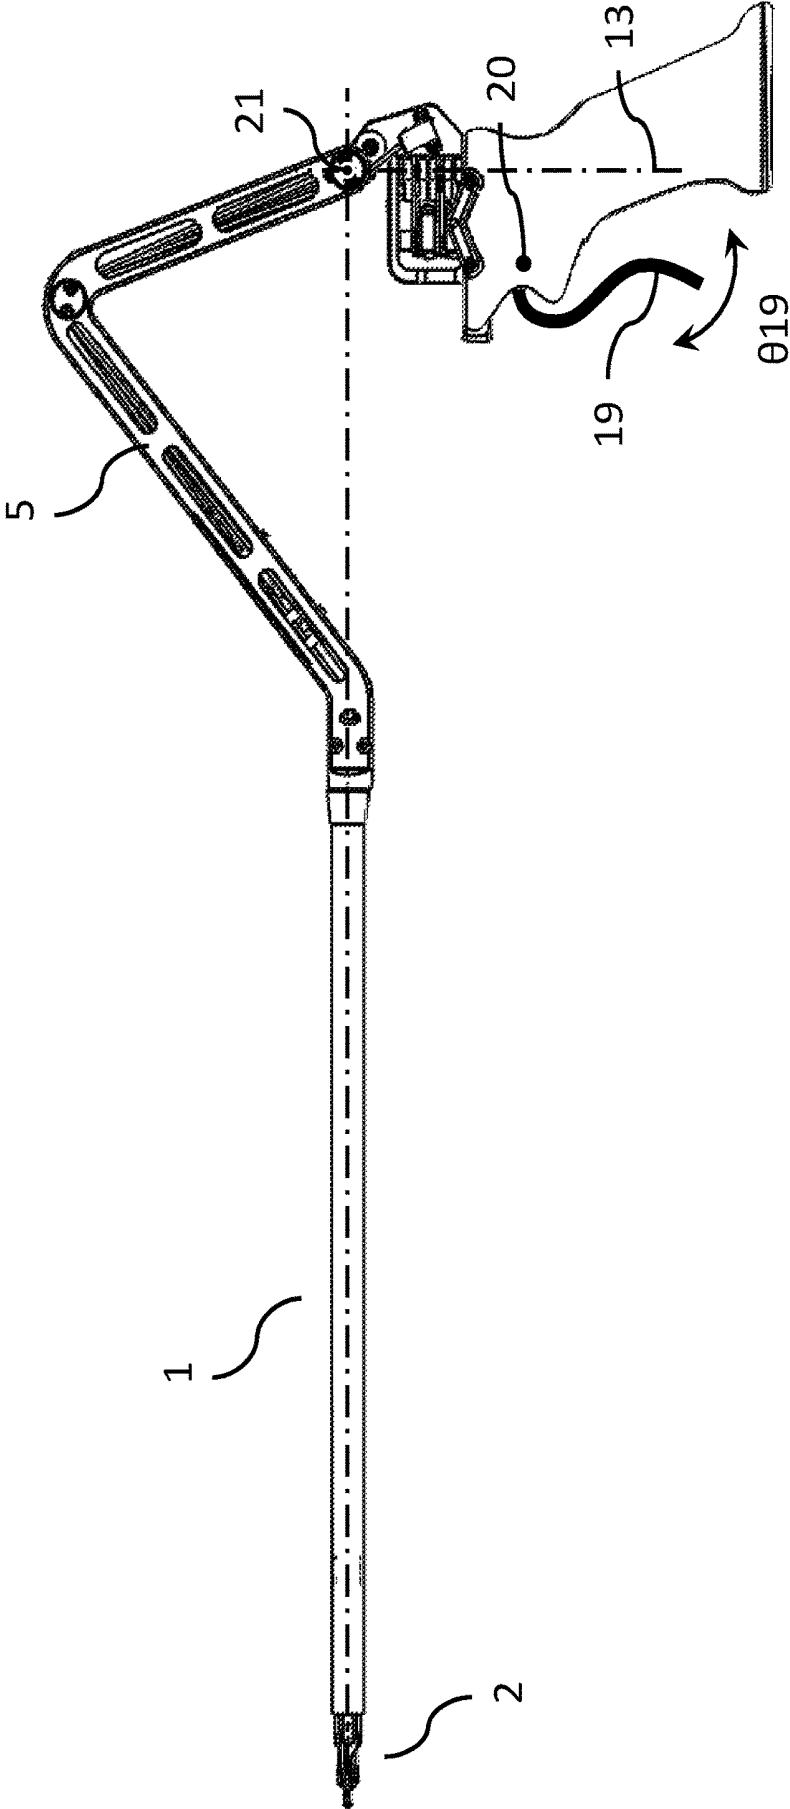


Figure 16



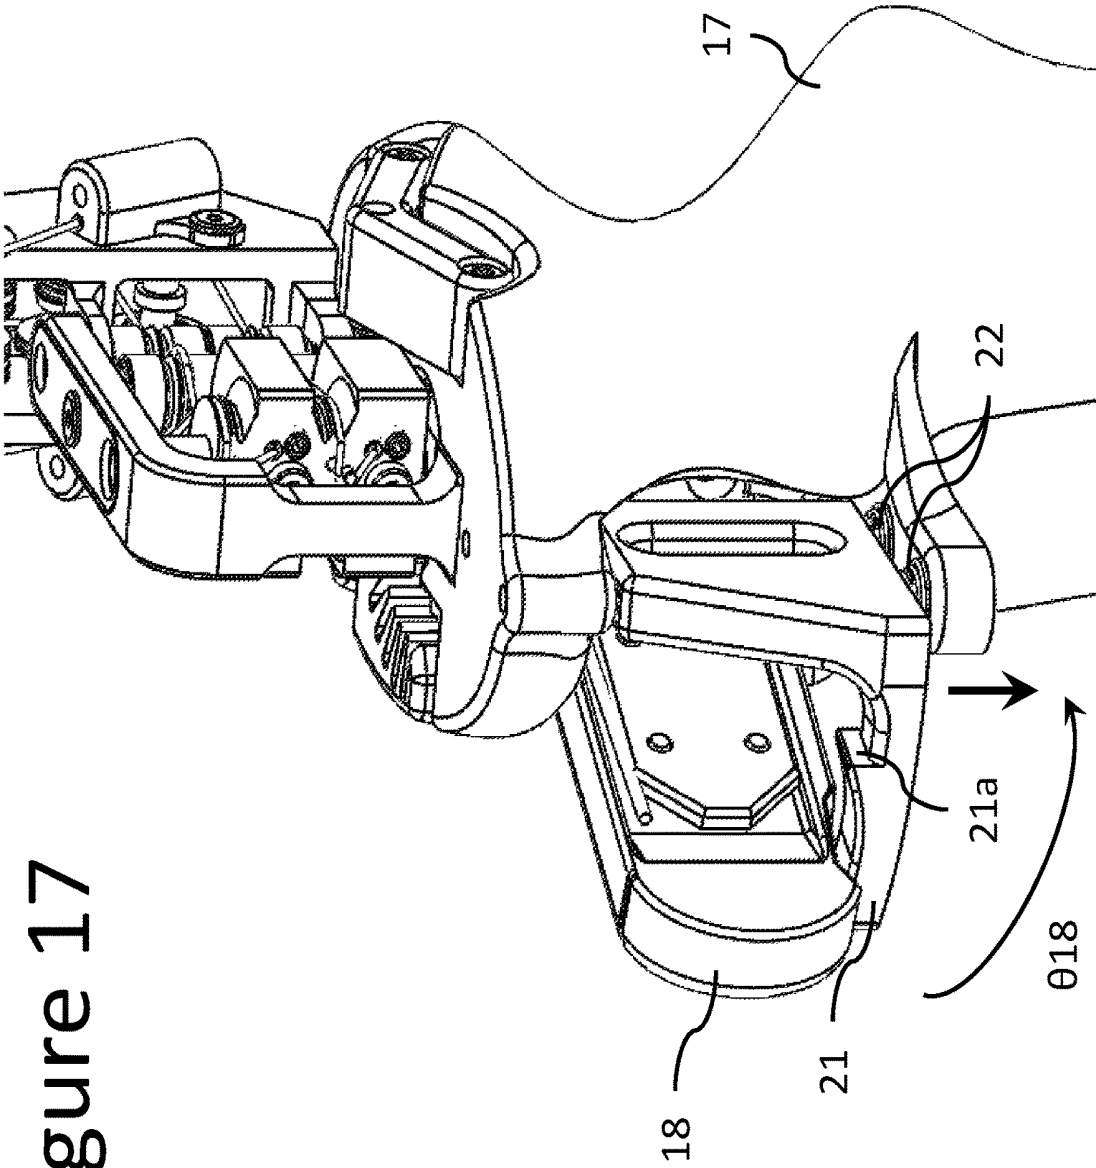
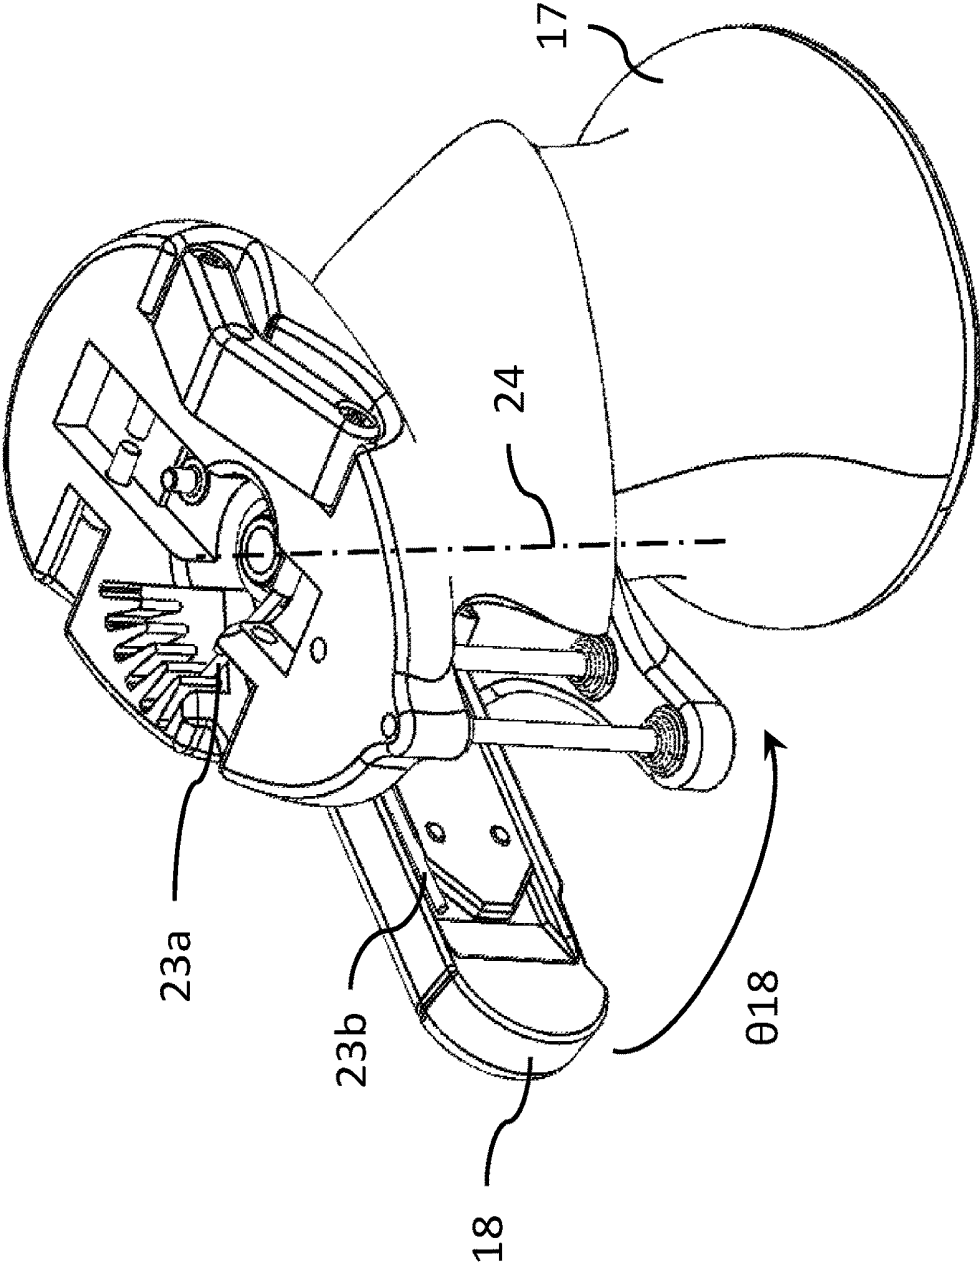


Figure 17

Figure 18



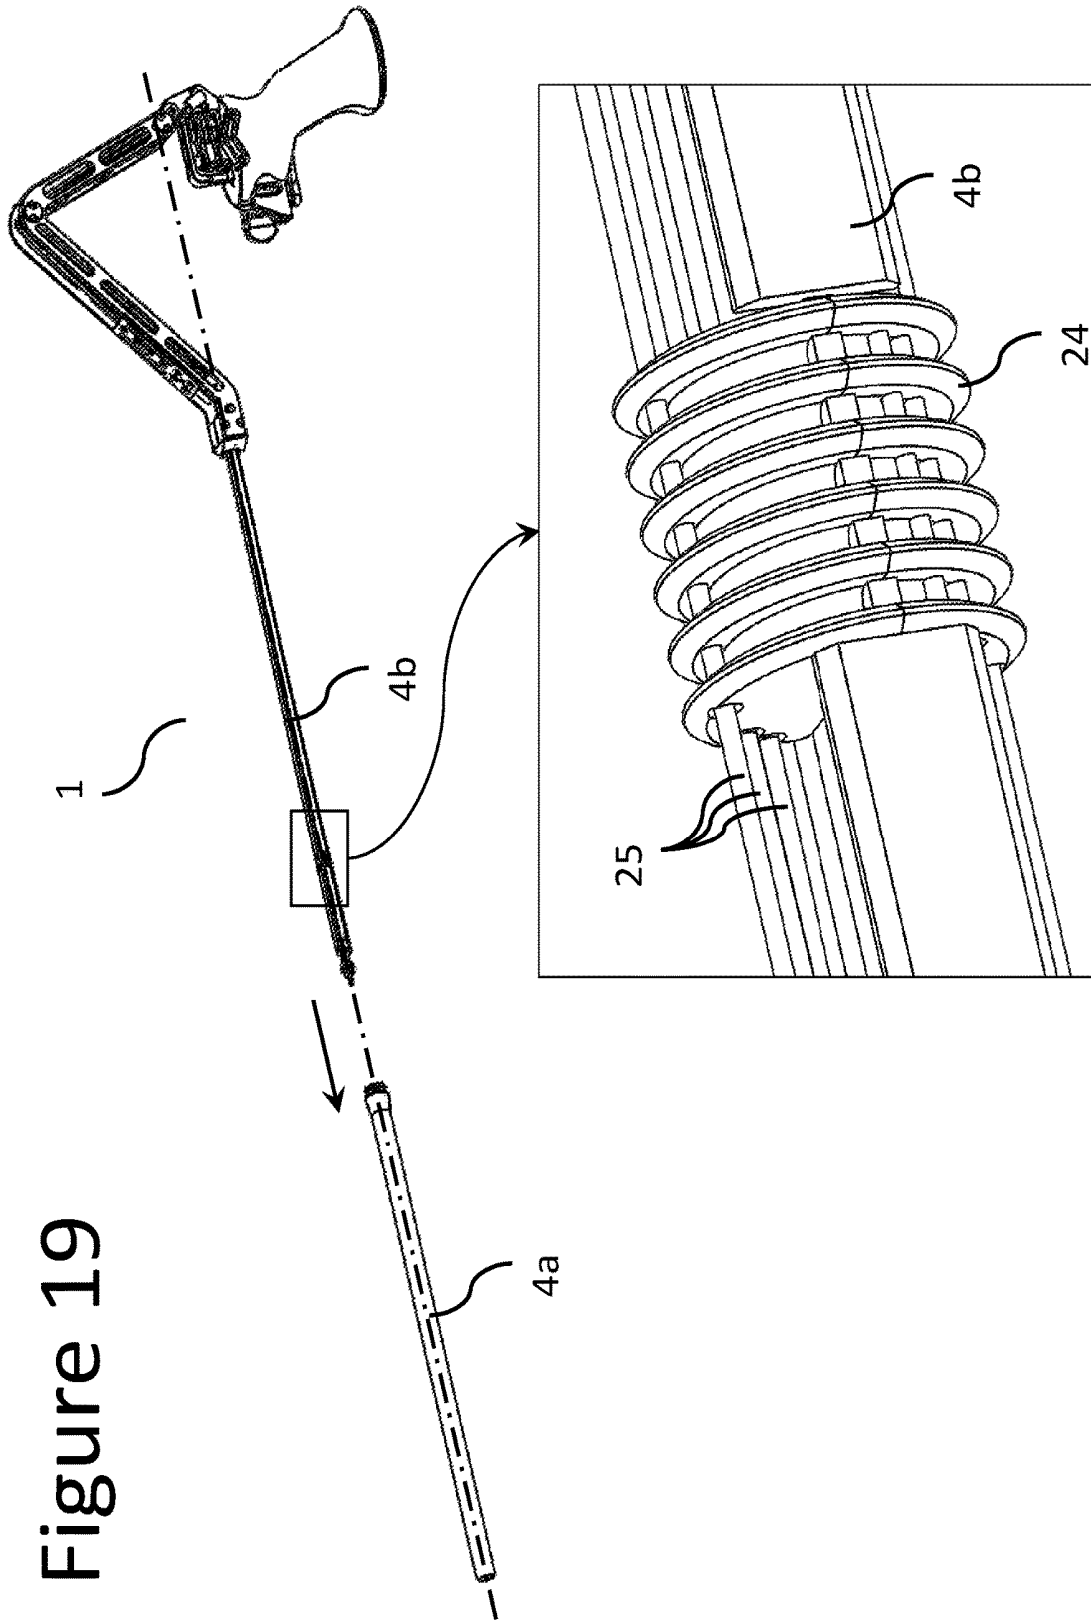


Figure 19

Figure 20

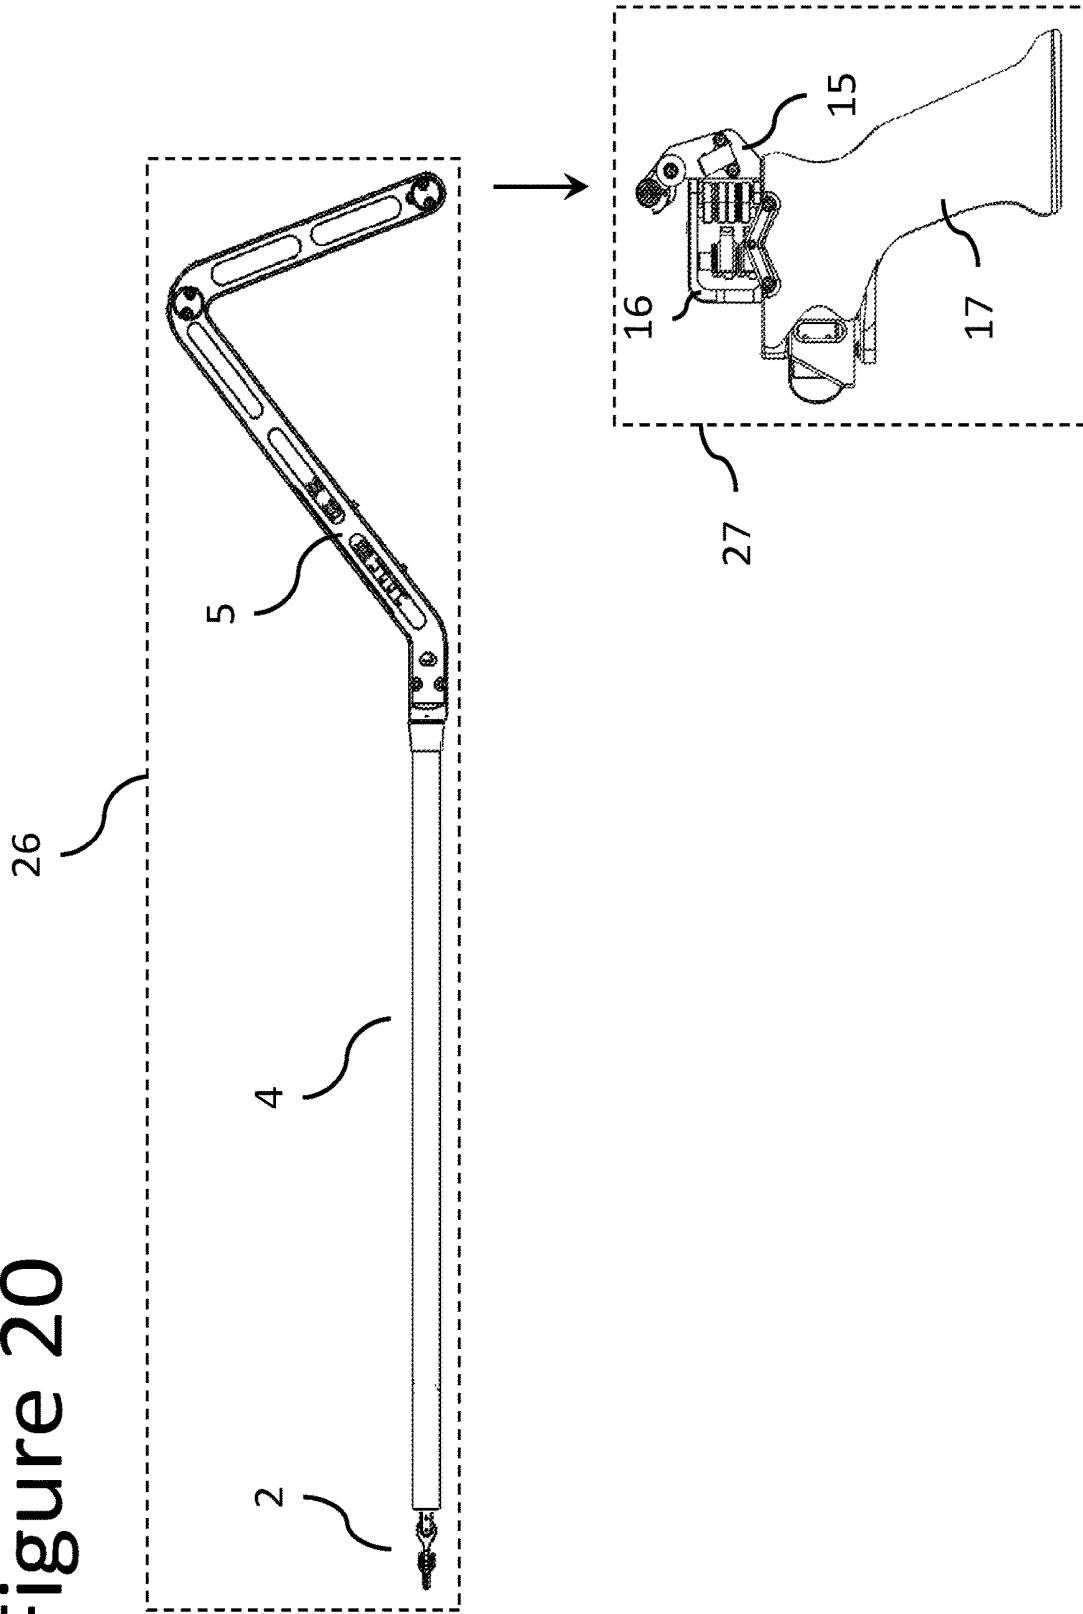


Figure 21

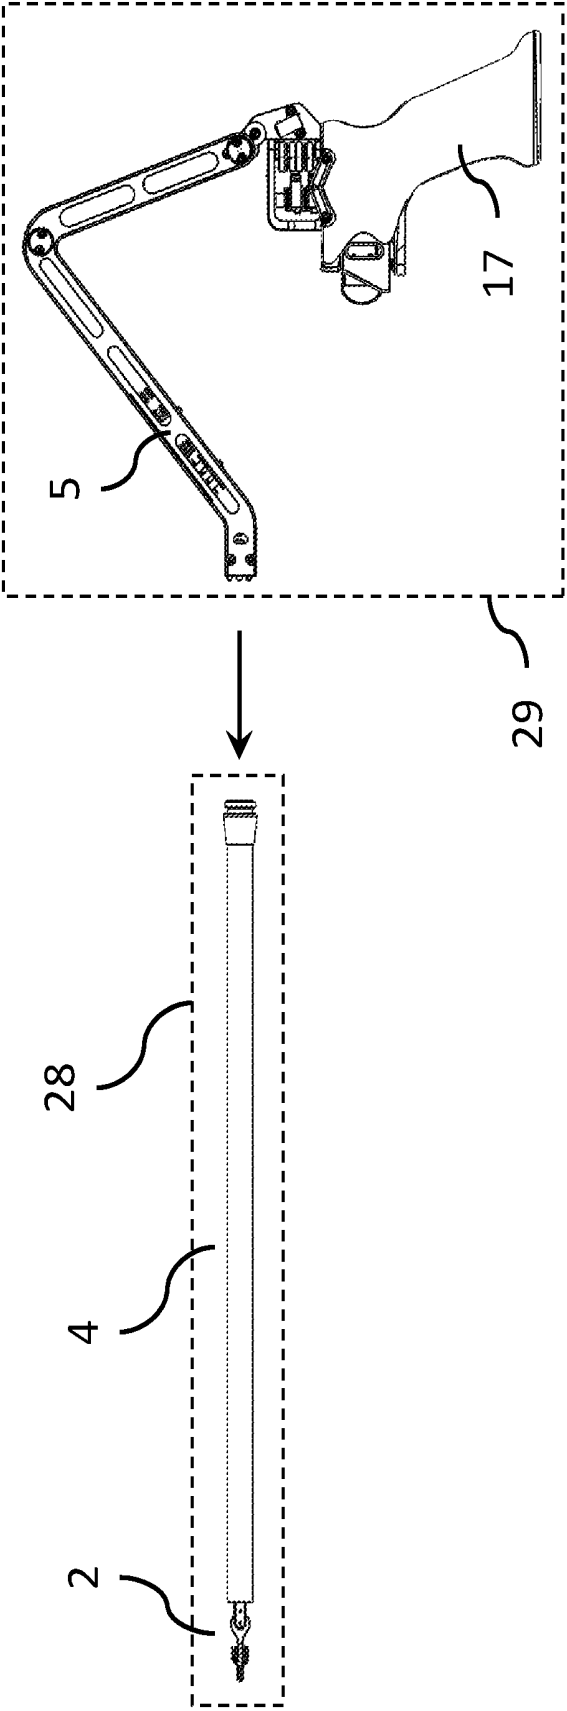


Figure 22

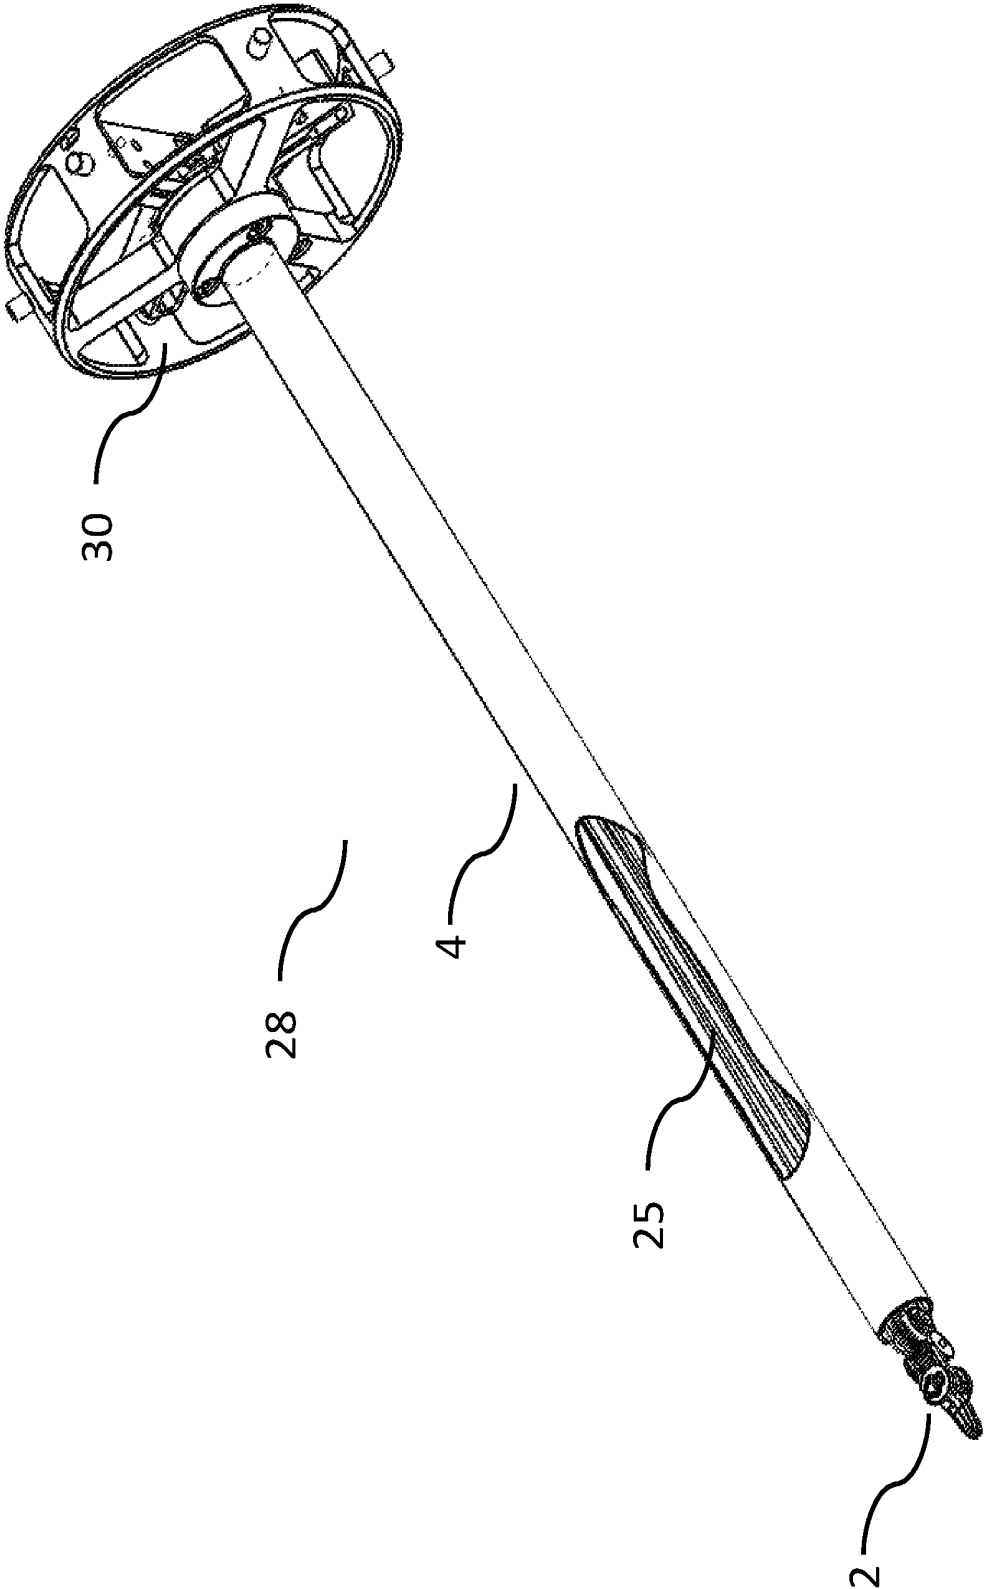


Figure 23

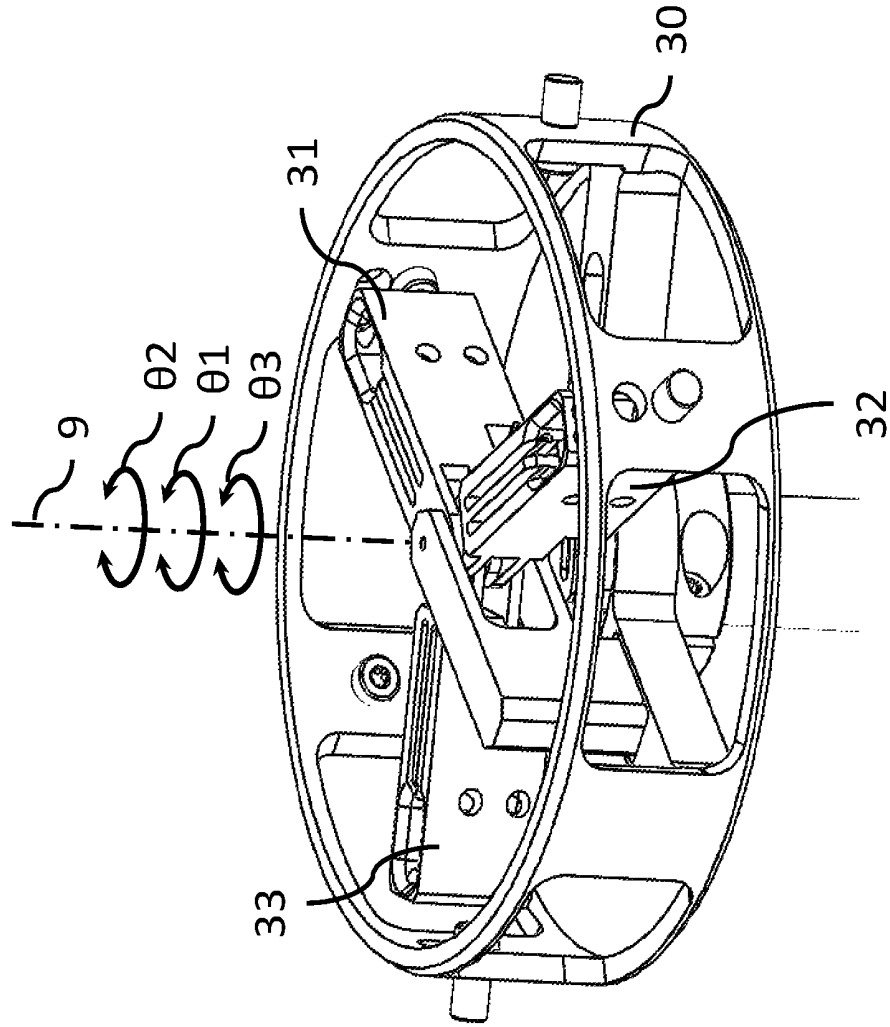


Figure 24

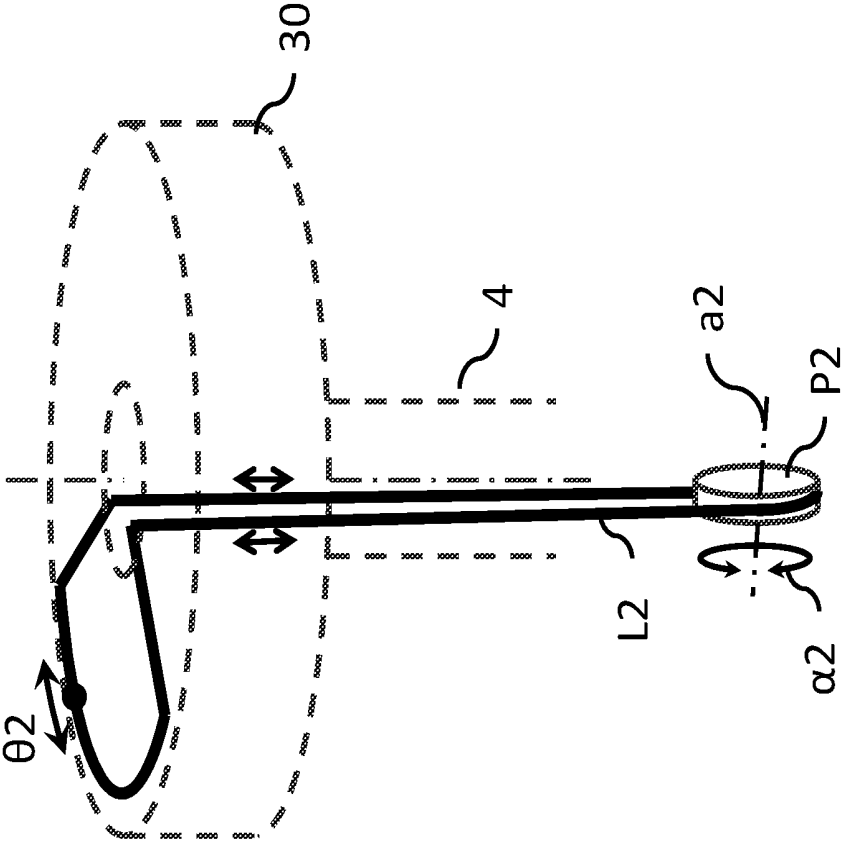


Figure 25

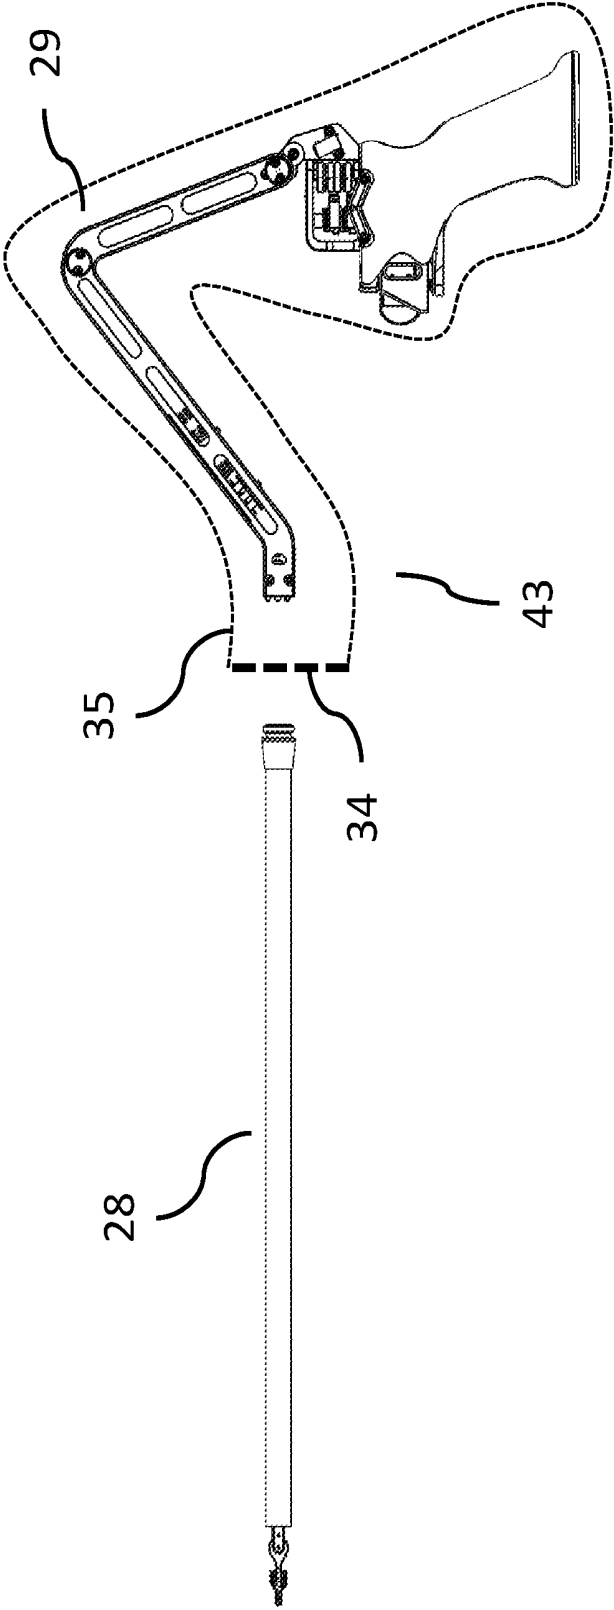


Figure 26

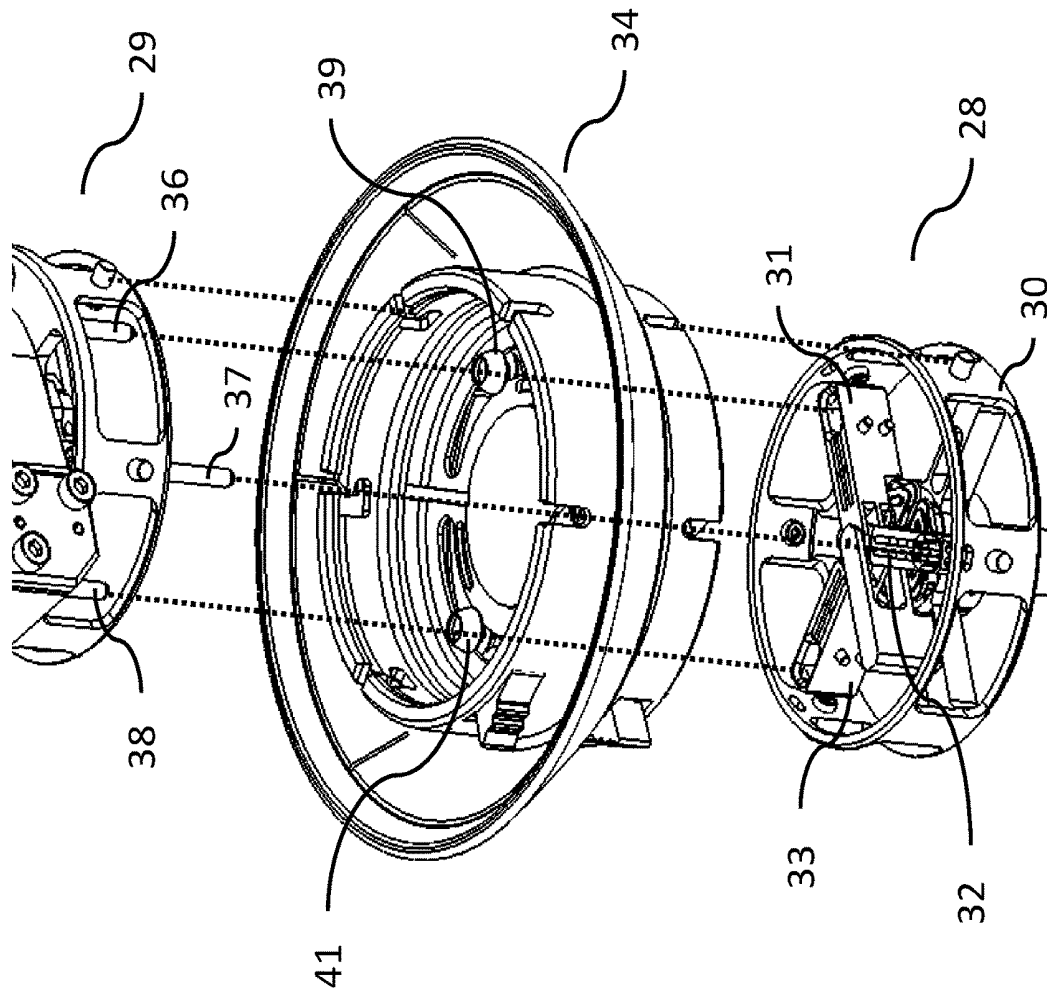


Figure 27

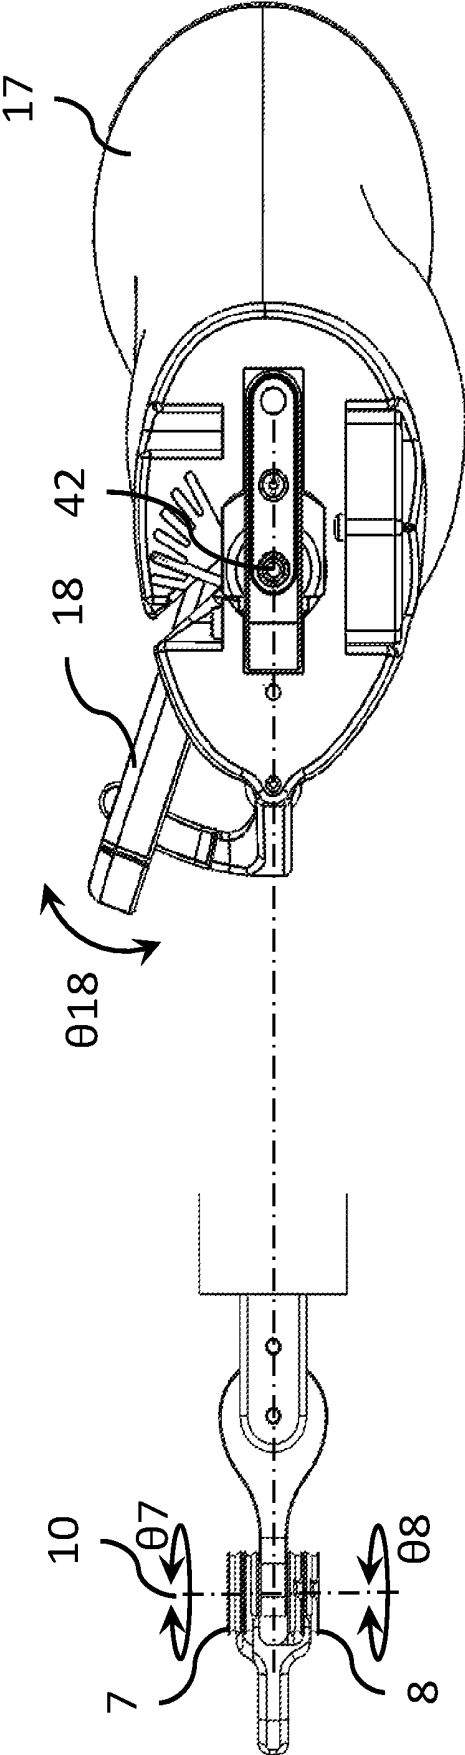


Figure 28

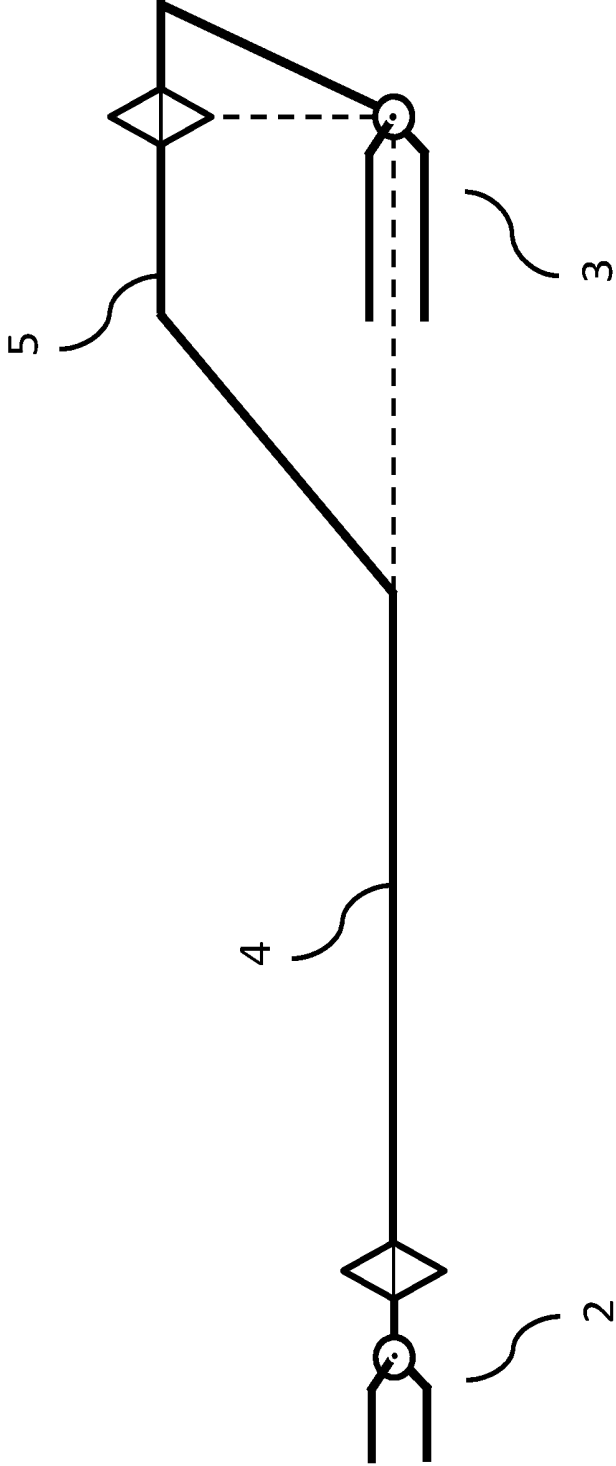


Figure 29

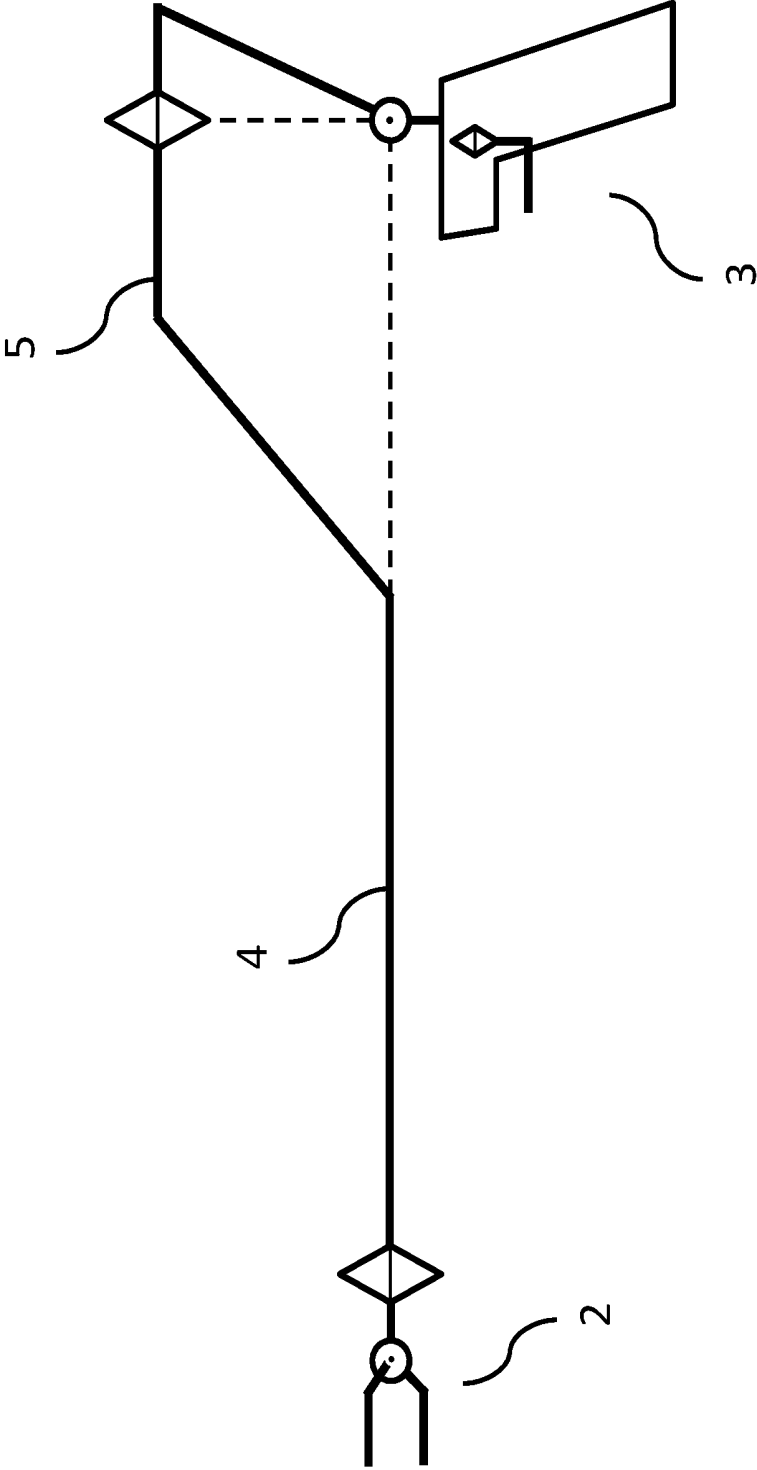


Figure 30

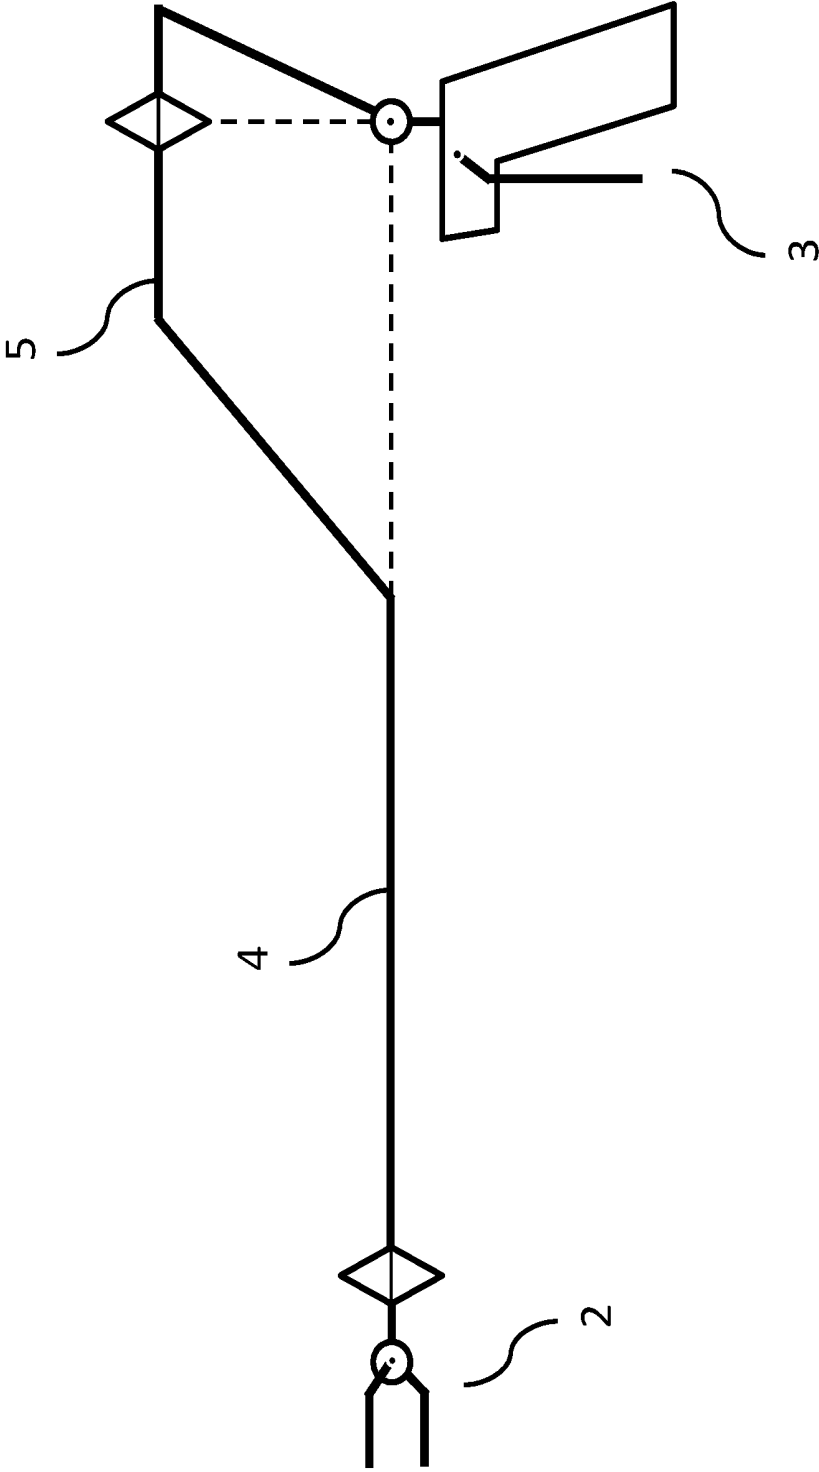


Figure 31

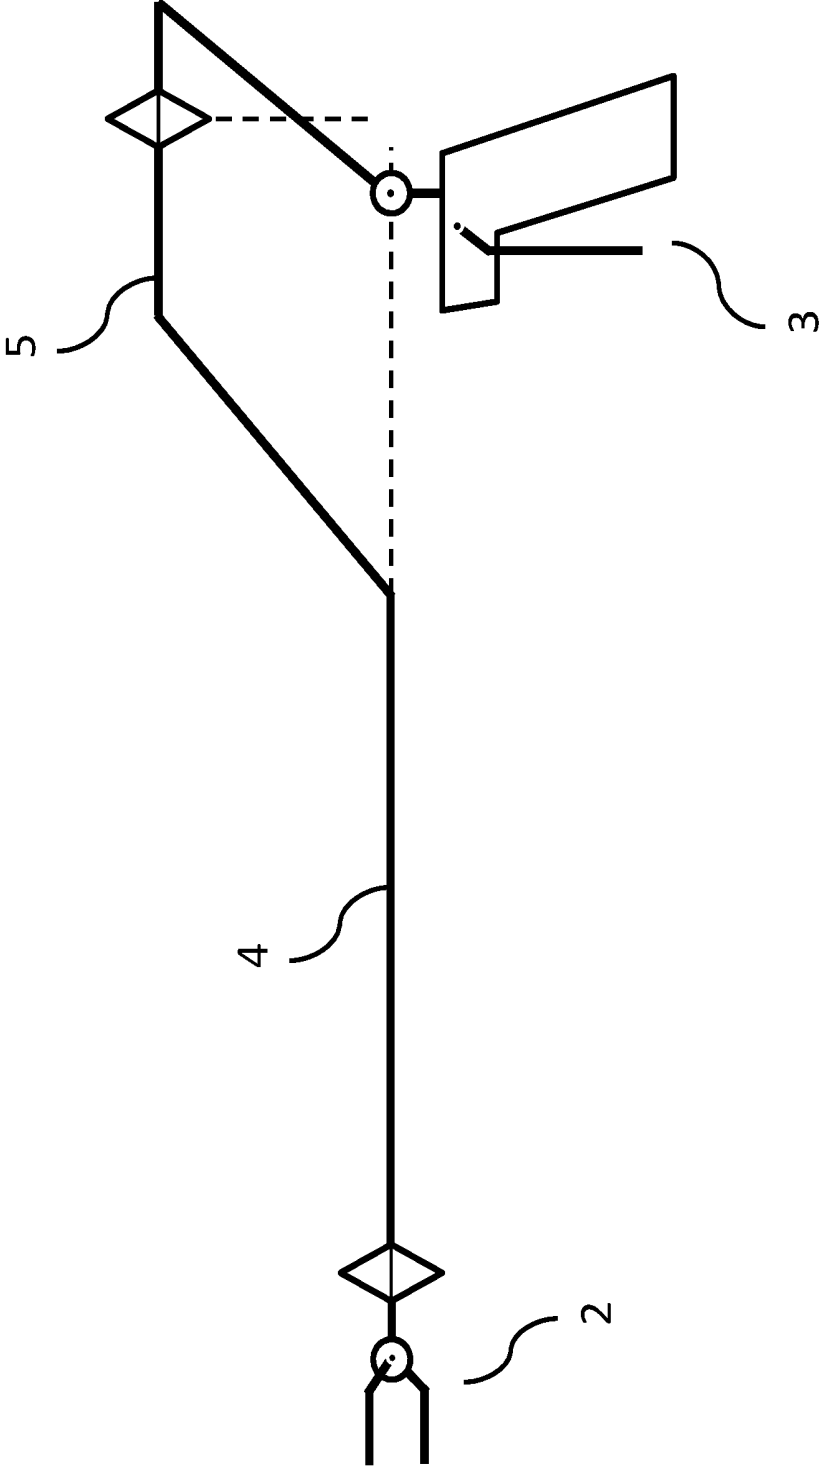


Figure 32

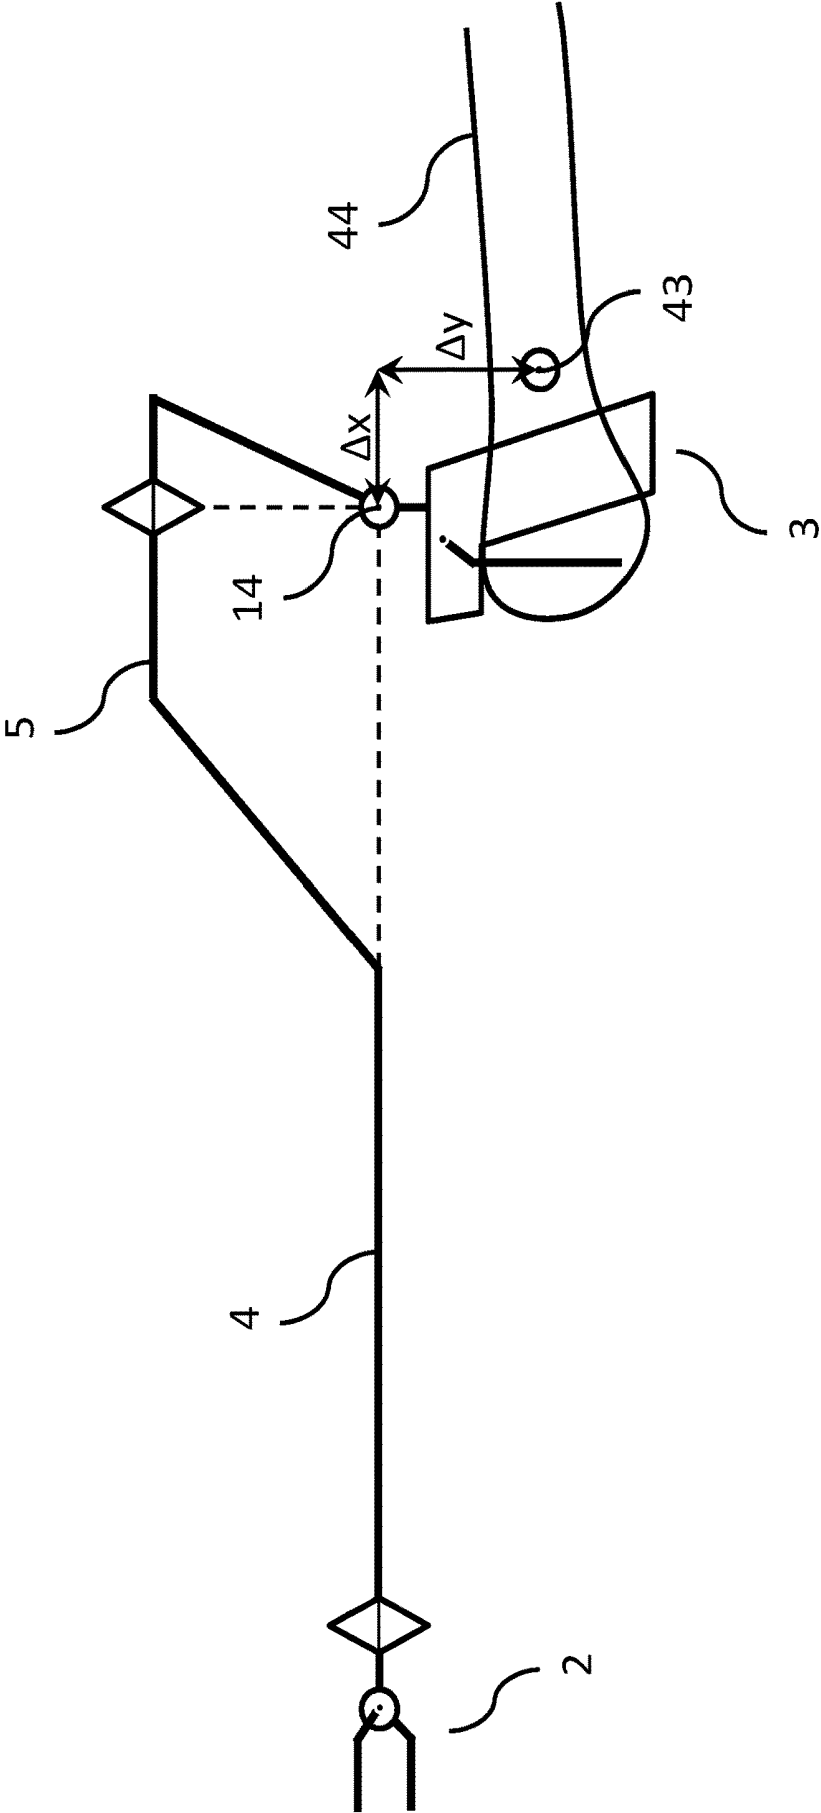


Figure 33

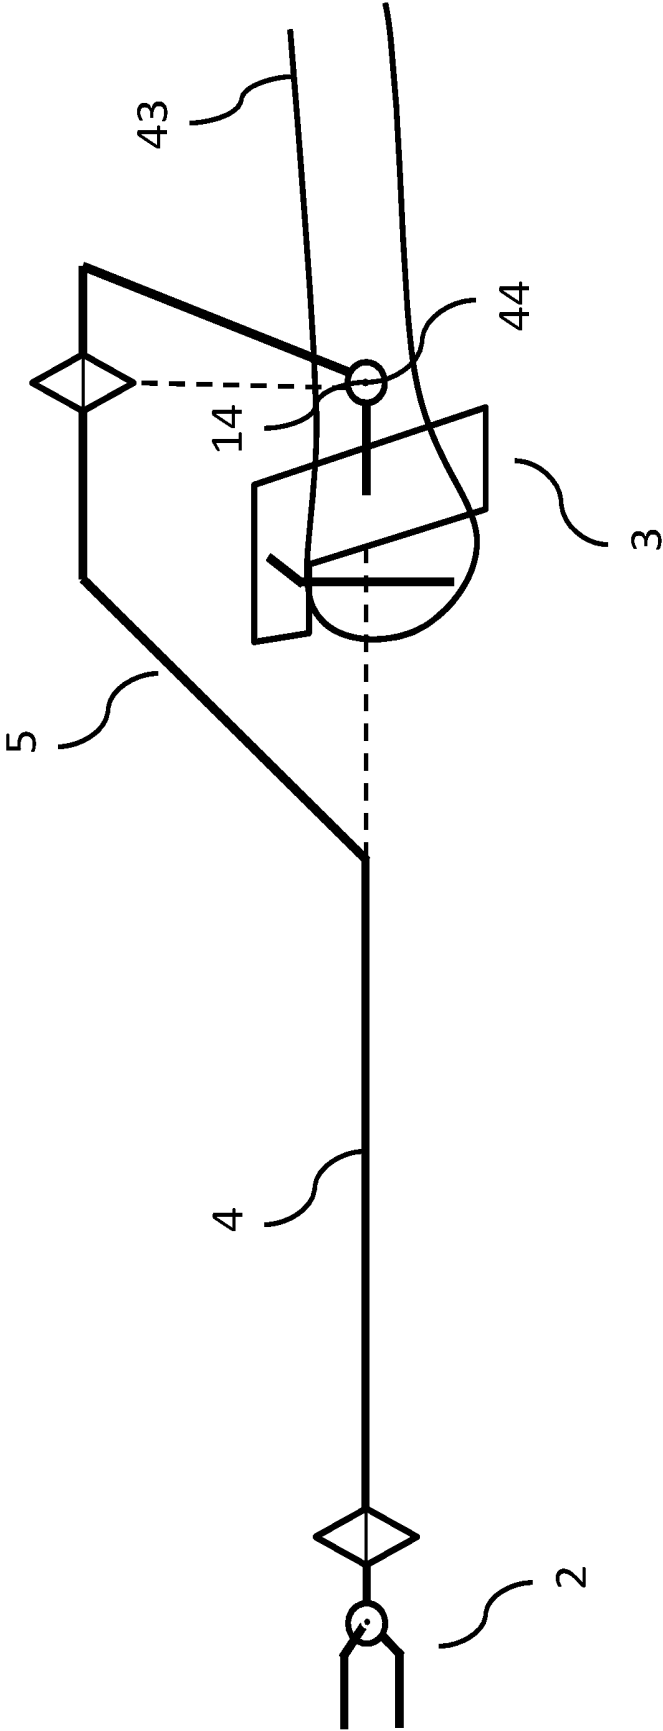


Figure 34

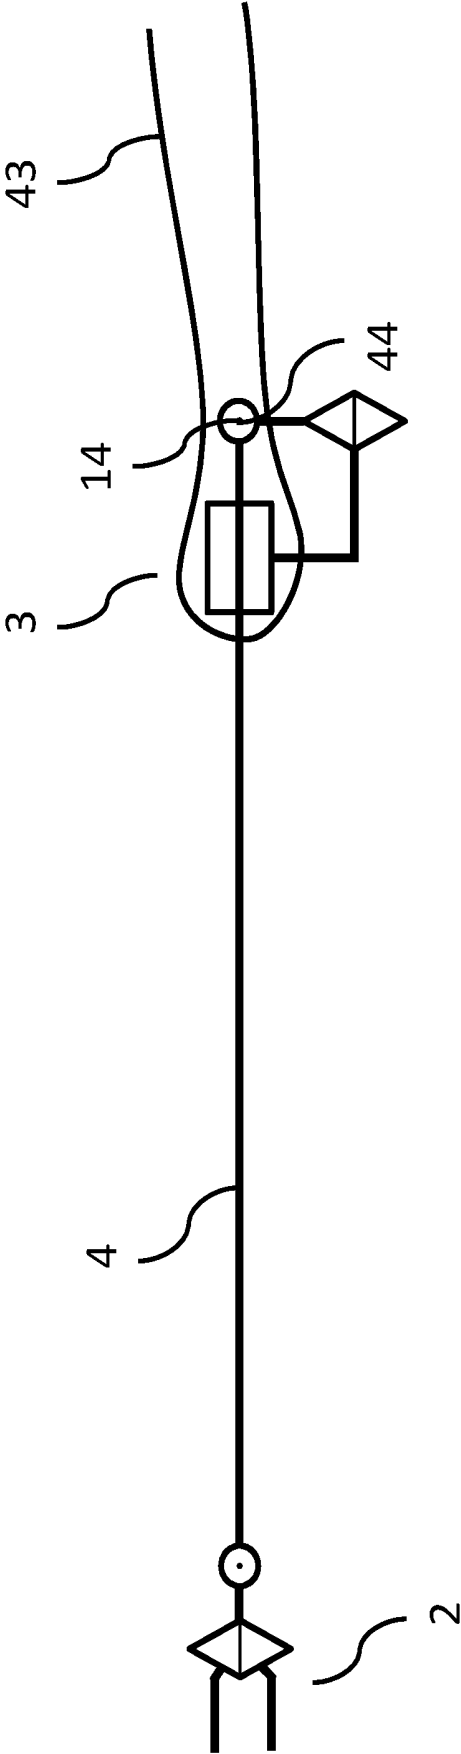


Figure 35

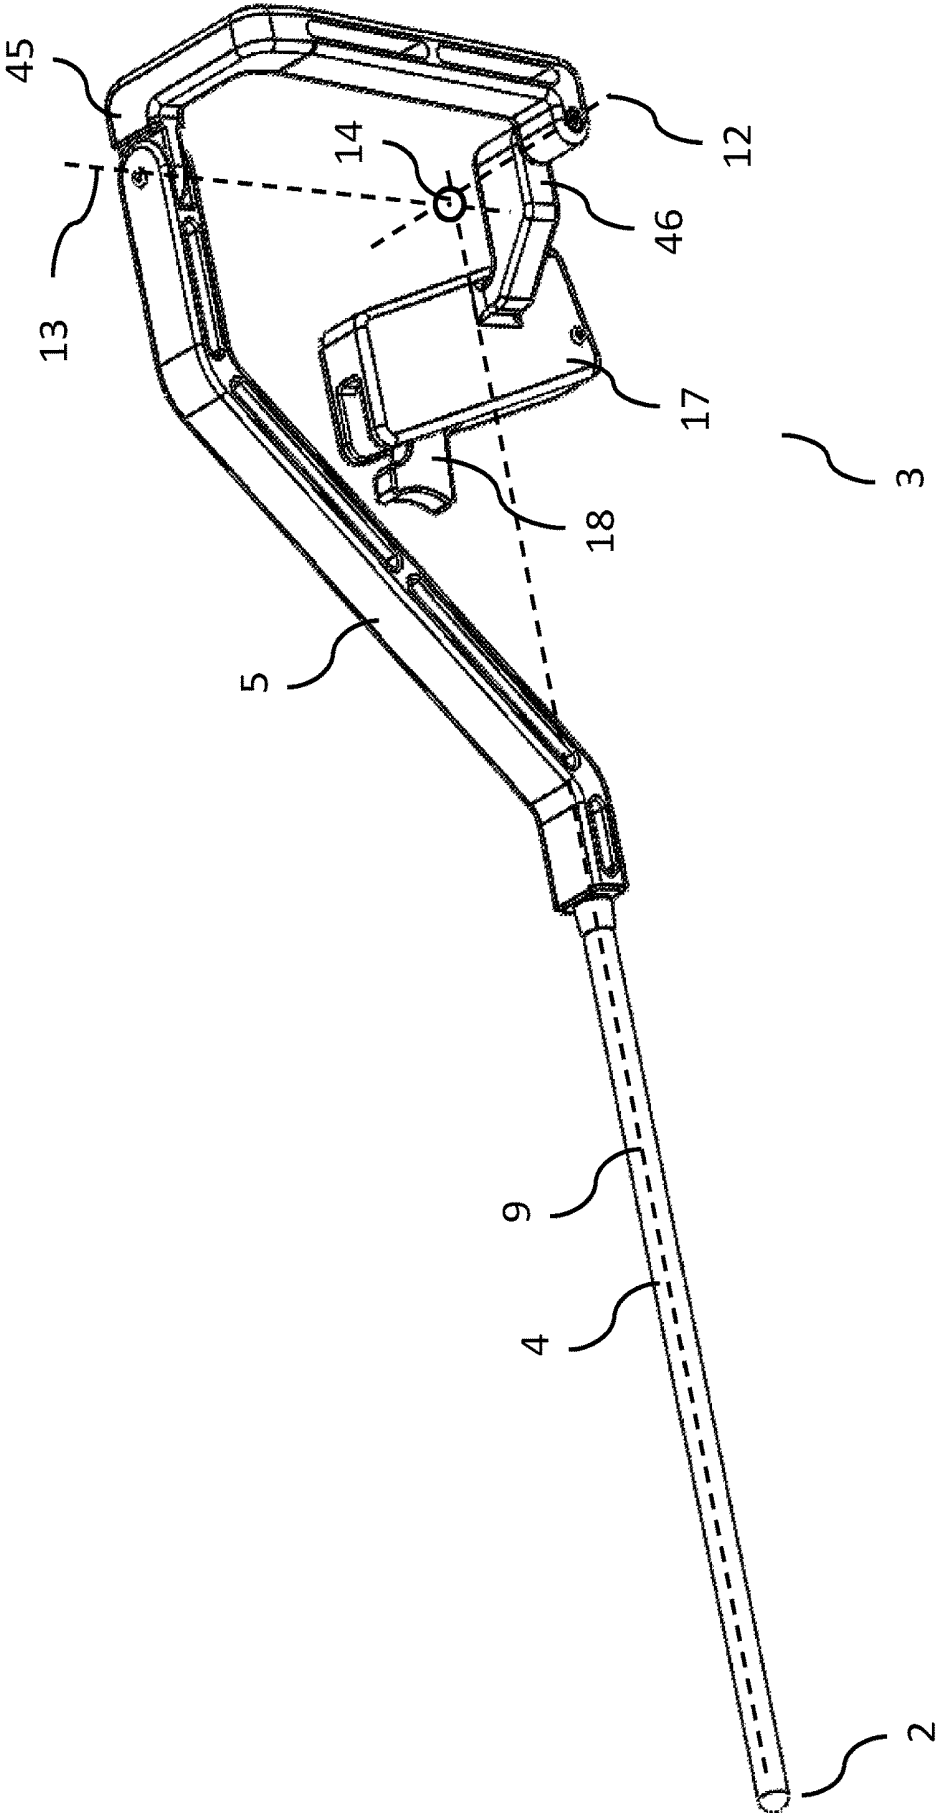


Figure 36

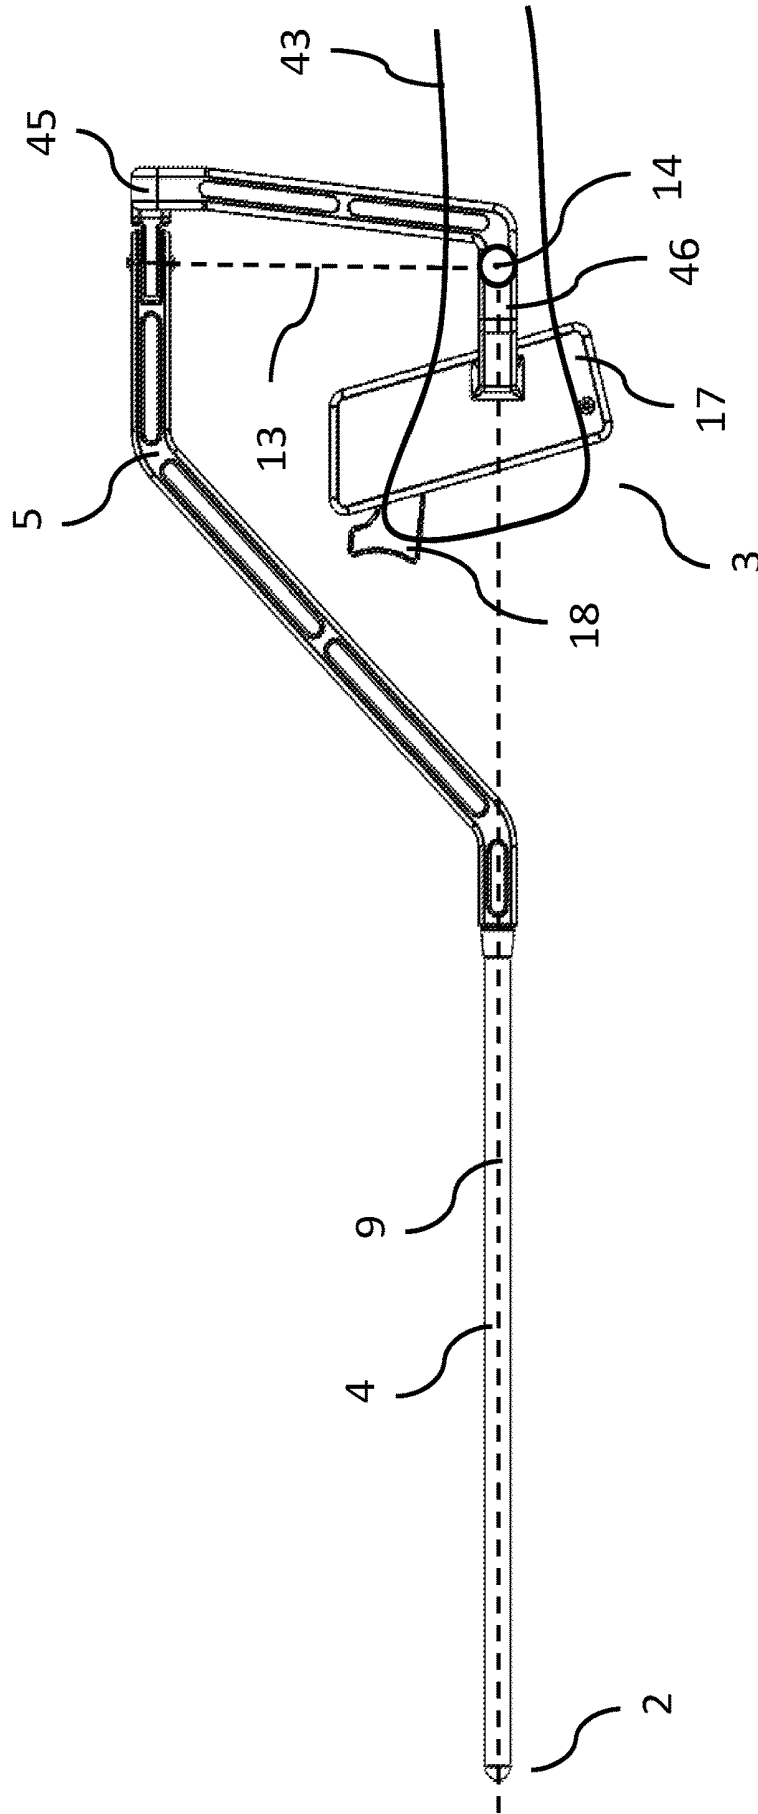
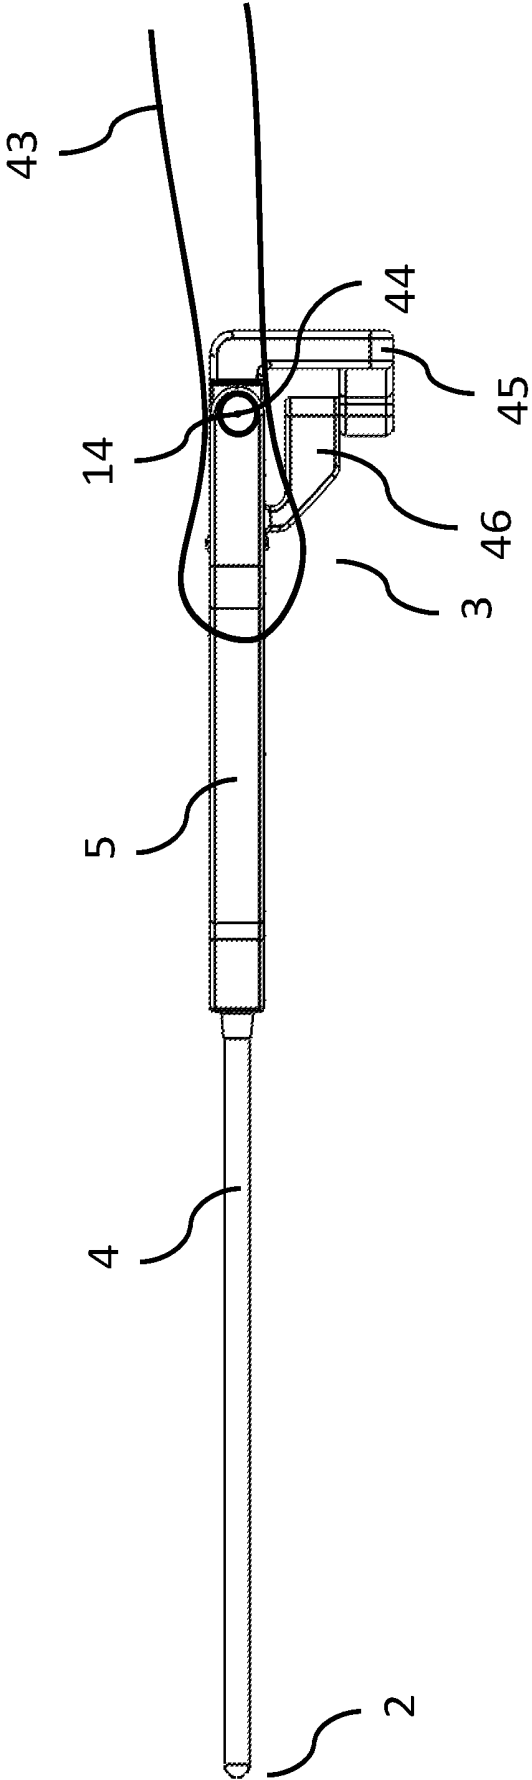


Figure 37



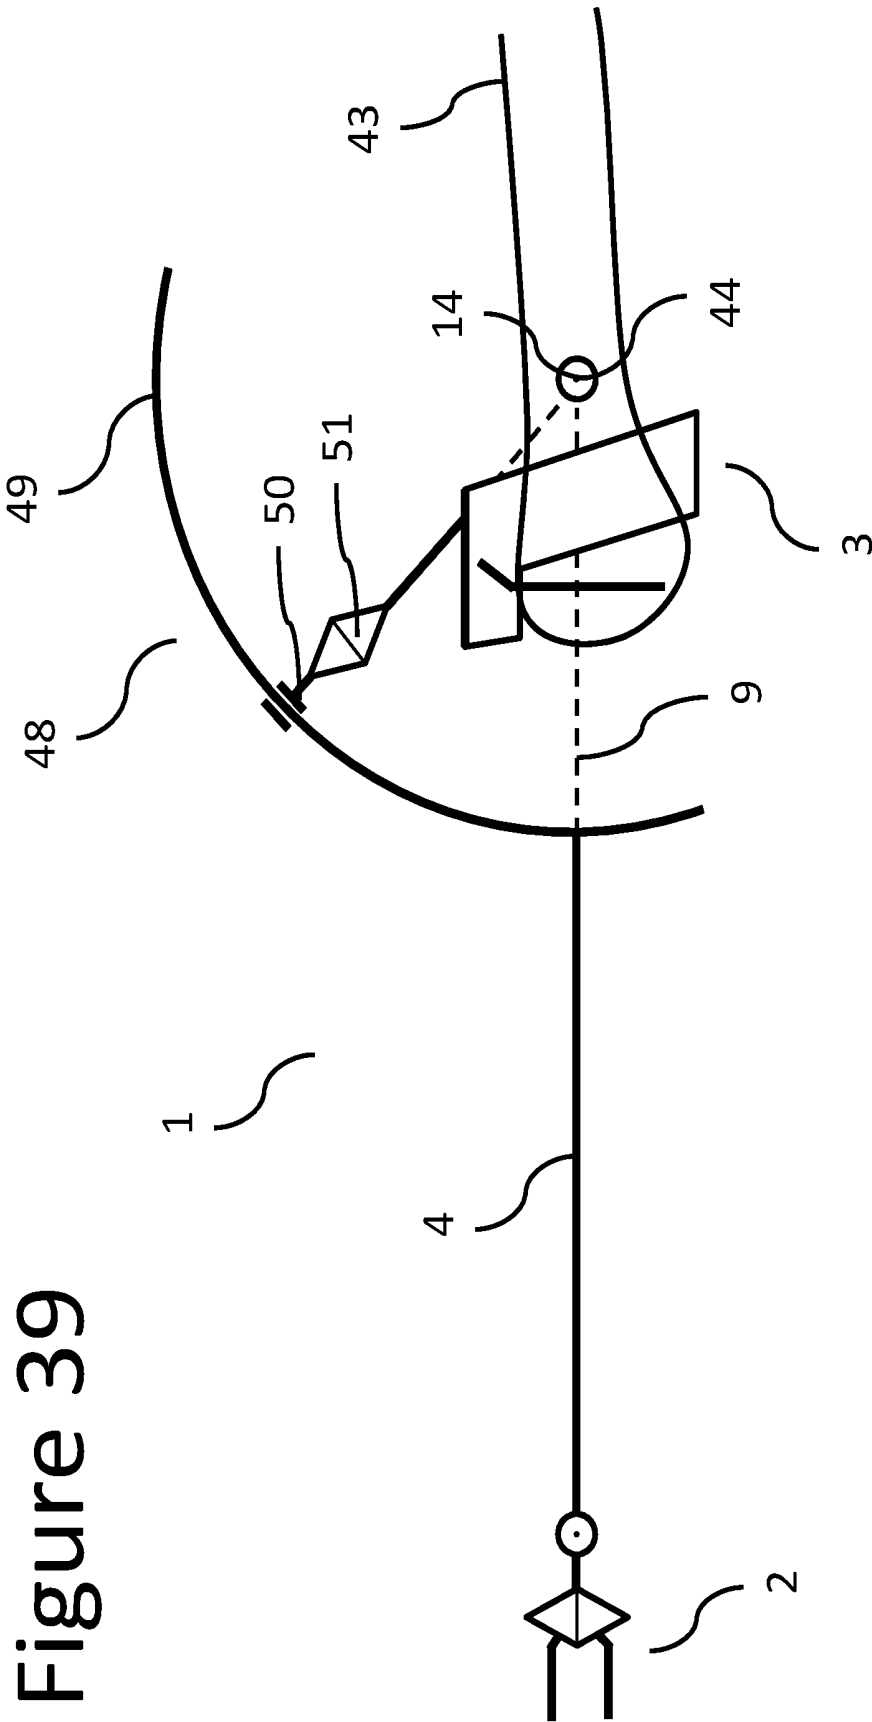


Figure 39

Figure 41

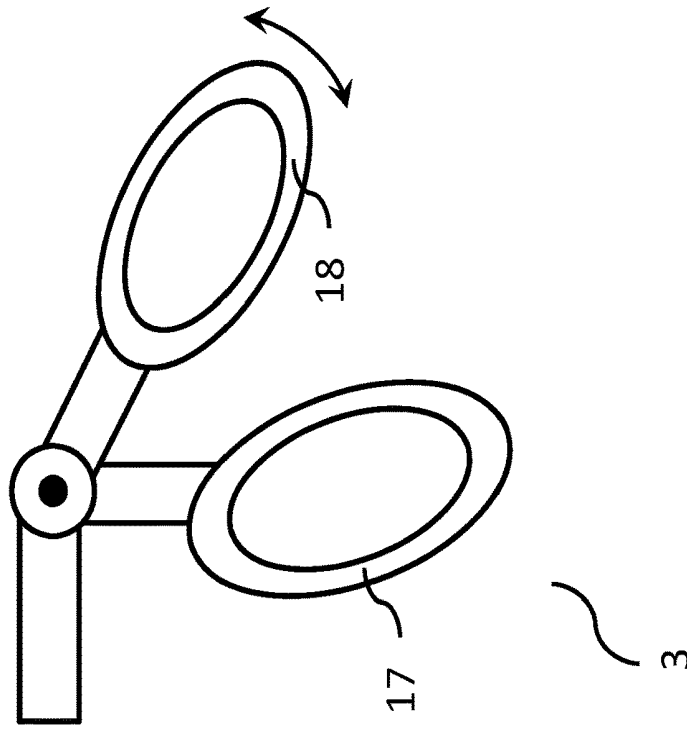


Figure 40

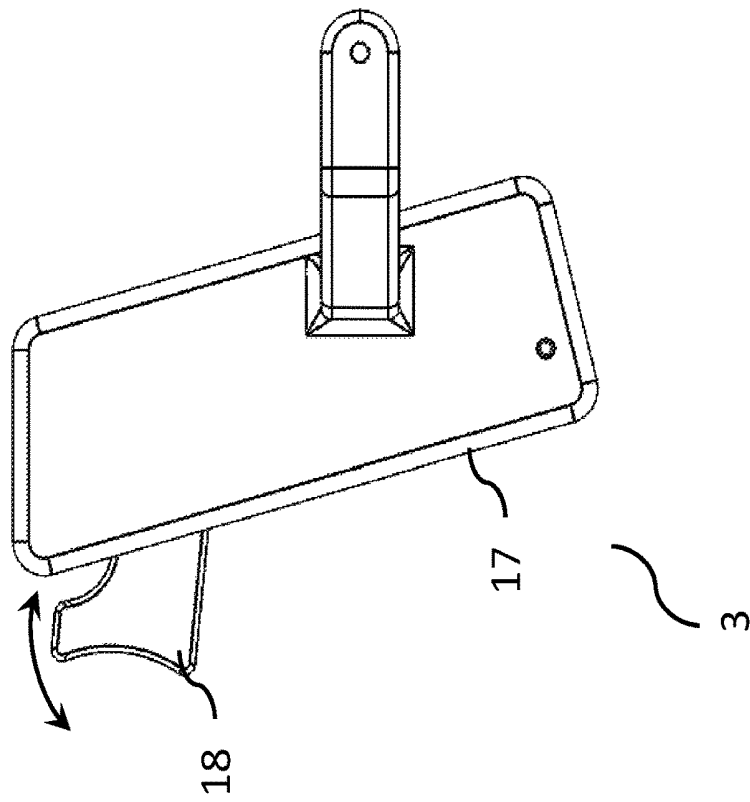


Figure 42

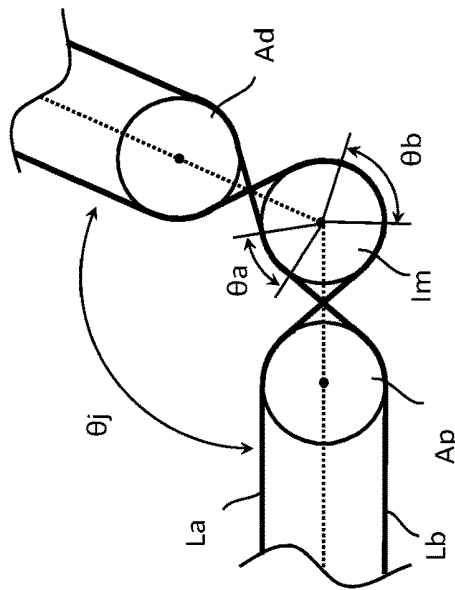


Figure 43

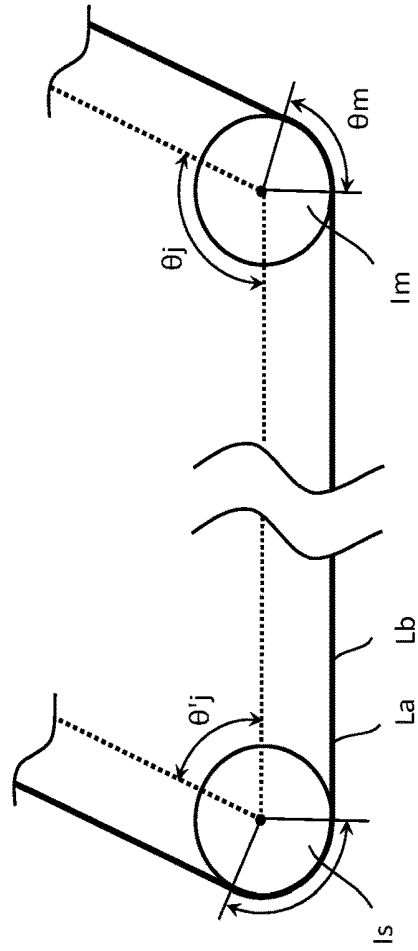


Figure 44

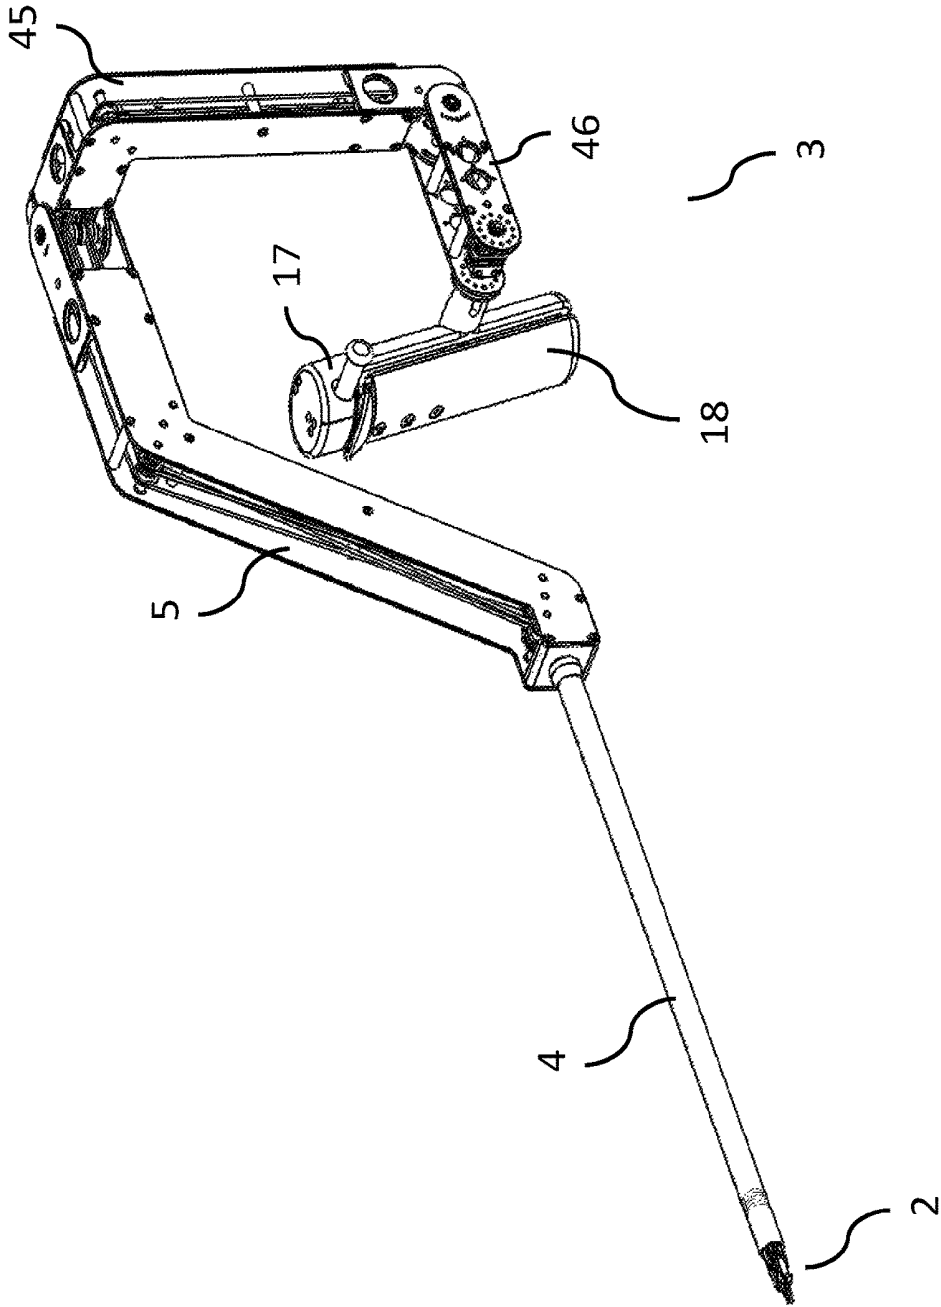


Figure 45

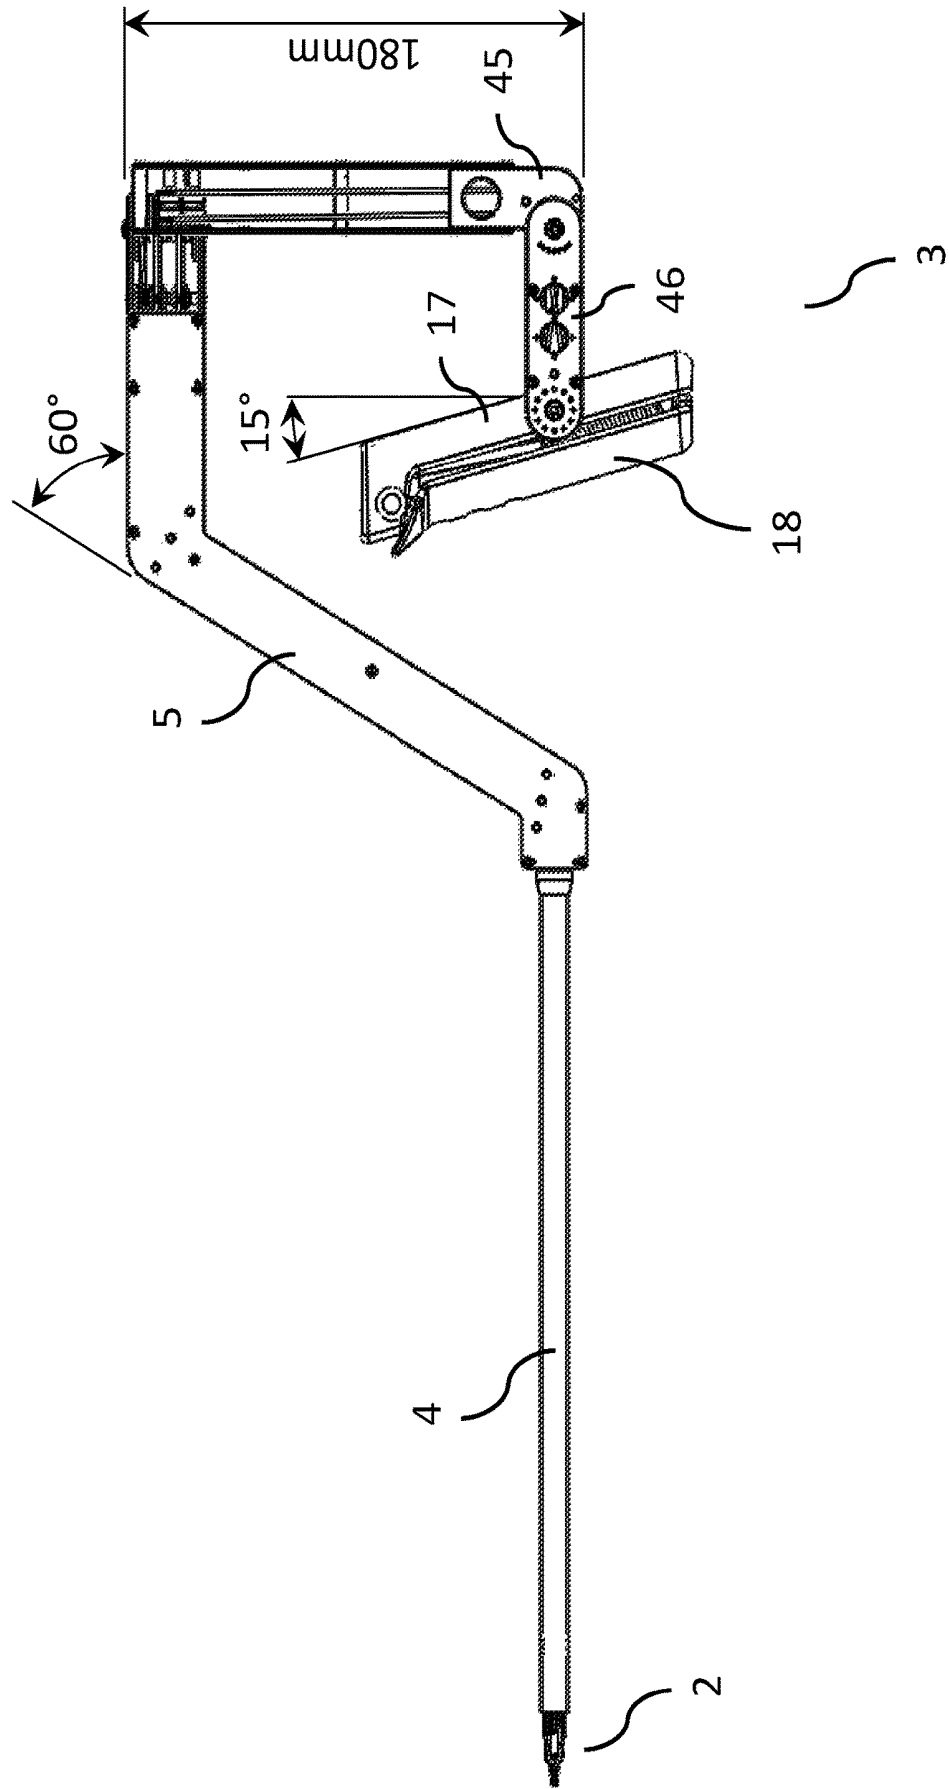


Figure 46

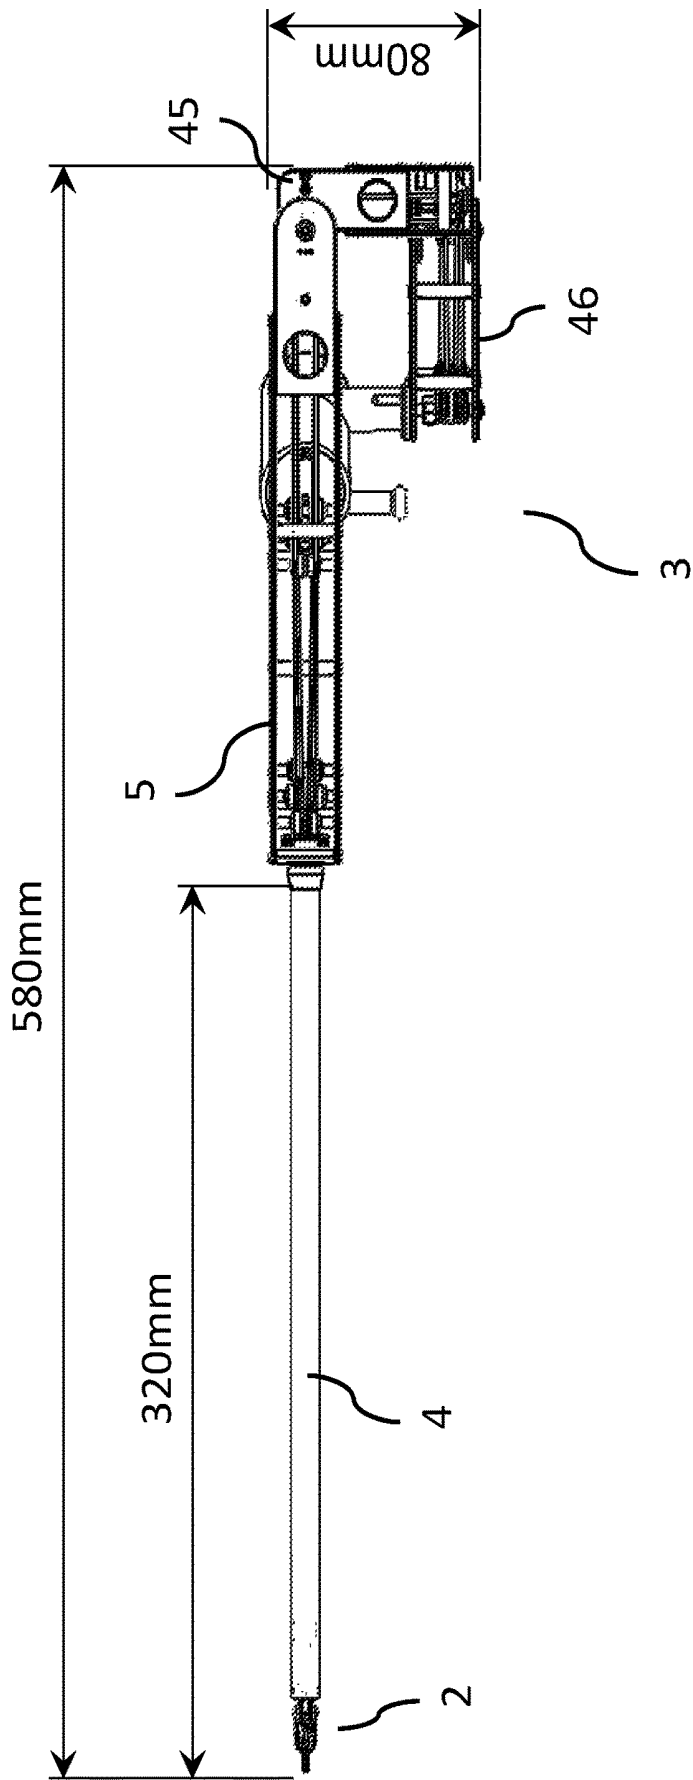
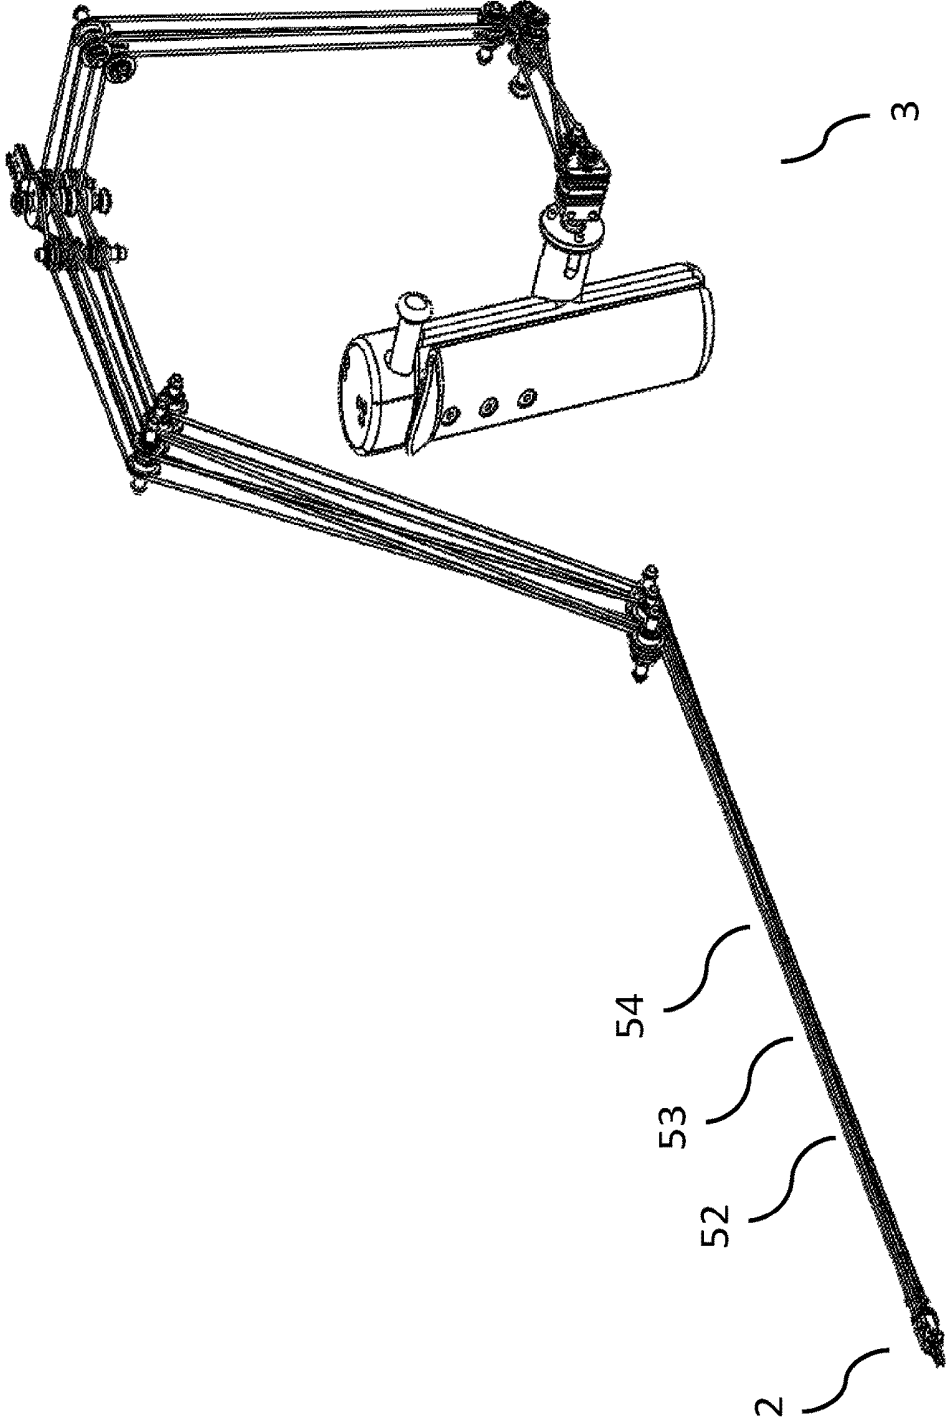


Figure 47



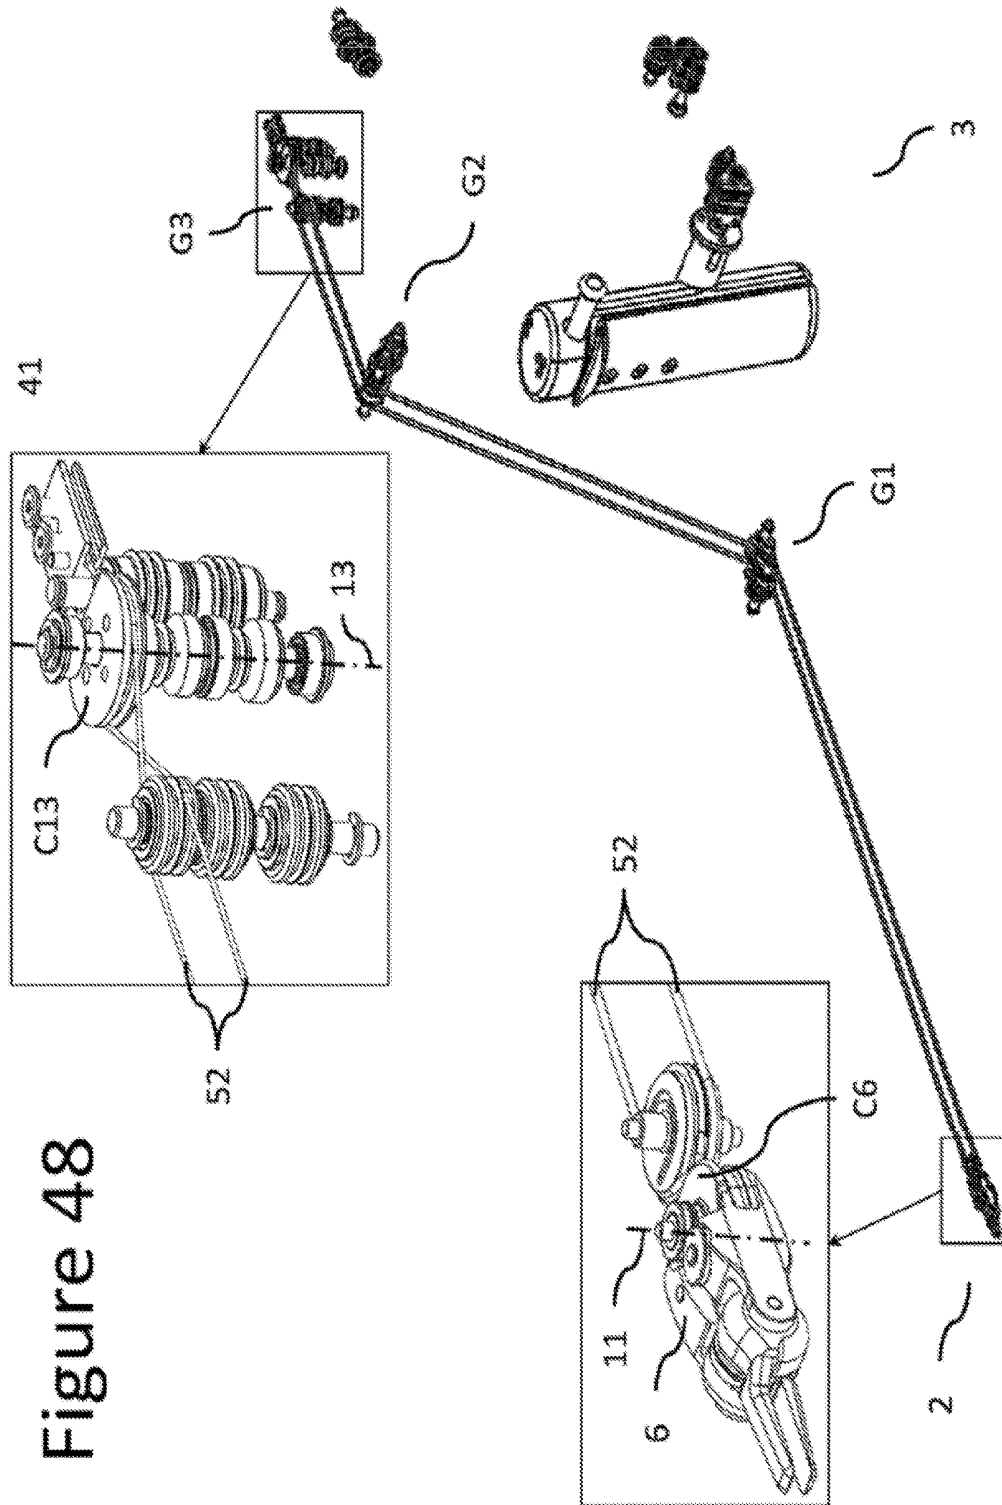


Figure 48

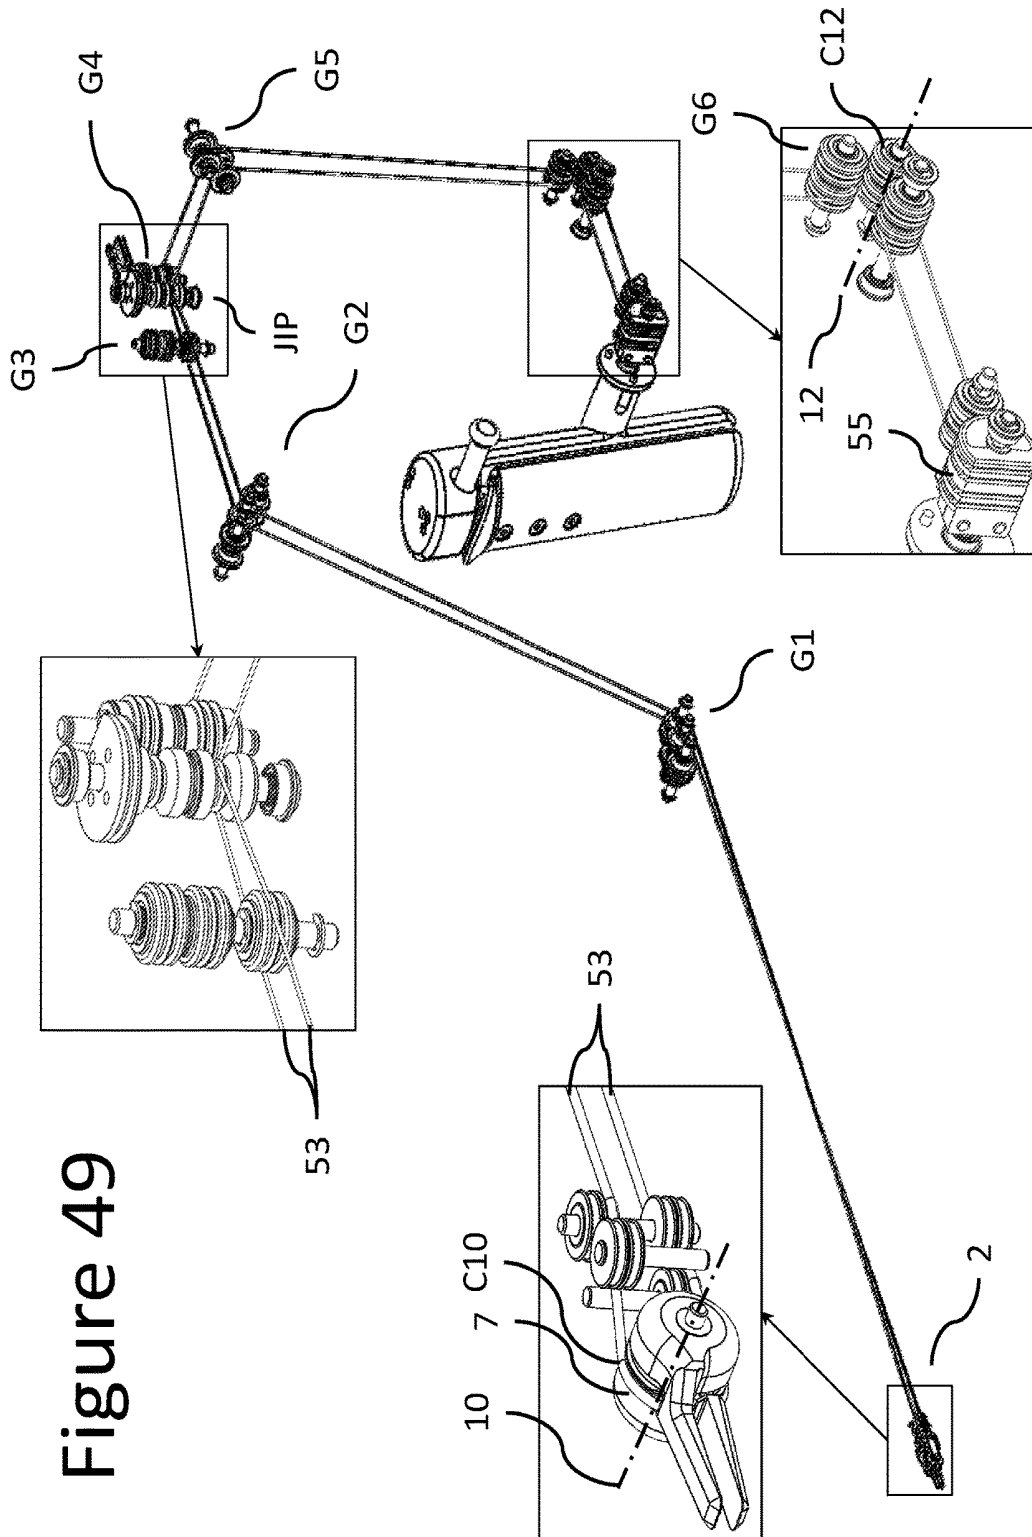


Figure 49

Figure 51


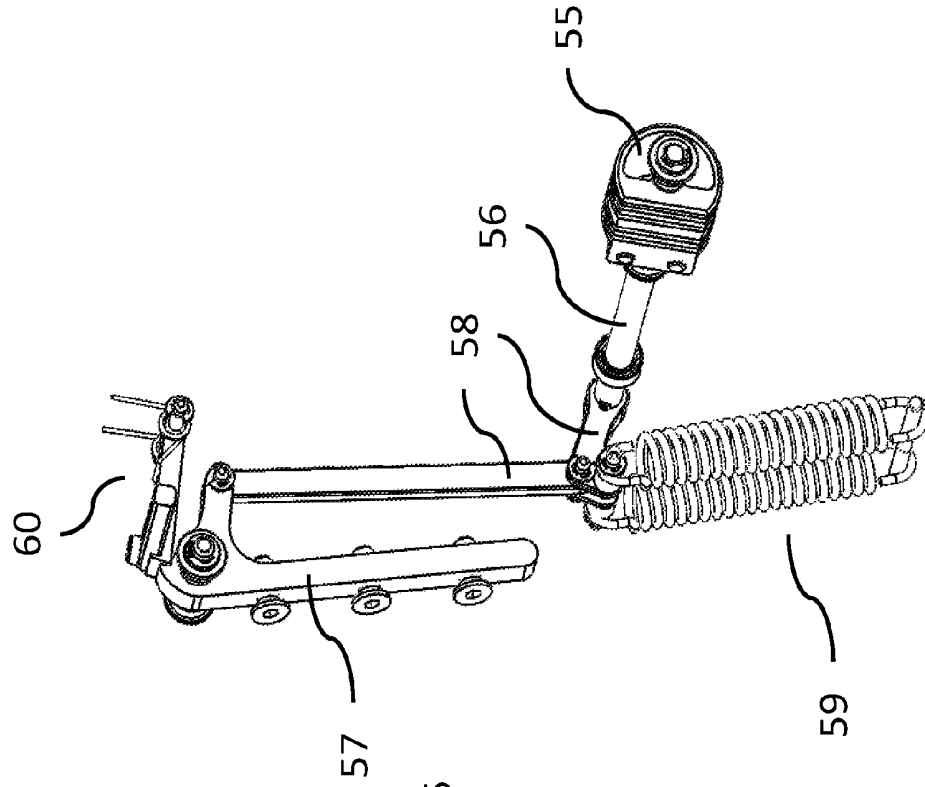


Figure 50

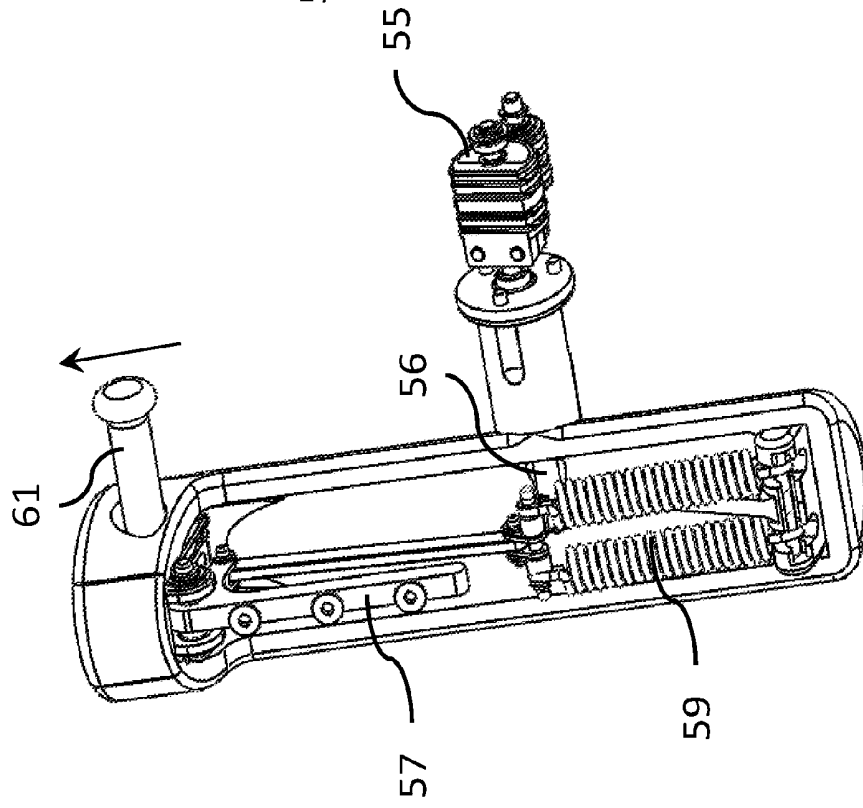

ARTICULATED HAND-HELD INSTRUMENT**CROSS-REFERENCE TO RELATED APPLICATIONS**

This application is a national phase of International PCT Patent Application No. PCT/IB2016/000542, filed Apr. 11, 2016, which claims priority to U.S. Provisional Patent Application Nos. 62/280,736, filed Jan. 20, 2016, and 62/145,454, filed Apr. 9, 2015, the entire contents of each of which are incorporated herein by reference.

FIELD OF THE INVENTION

The present invention relates to the field of remotely actuated mechanical systems, more particularly to surgical instruments, and most particularly to articulated hand-held surgical instruments. More specifically, this invention relates to articulated hand-held surgical instruments primarily designed to be used in minimally invasive surgical procedures. The inventive surgical instruments are designed to be used in a full range of minimally invasive surgical procedures and with standard equipment, such as trocars and endoscopic cameras. The articulated hand-held surgical instruments are designed to provide greater reach, range of motion and dexterity than that accessible with the use of standard laparoscopic instruments.

BACKGROUND OF THE INVENTION

Open surgery is still the standard technique for most surgical procedures. It has been used by the medical community for several decades and consists of performing the surgical tasks through a long incision in the abdomen, through which traditional surgical tools are inserted. However, due to the long incision, this approach is extremely invasive for the patients, resulting in substantial blood loss during the surgery and long and painful recovery periods at the hospital.

In order to reduce the invasiveness of open surgery, laparoscopy, a minimally invasive technique, was developed. Instead of a single long incision, four to five small incisions are made in the patient through which appropriately sized surgical instruments and endoscopic cameras are inserted. Because of the low invasiveness, this technique reduces blood loss and shortens hospital stays and pain. When performed by experienced surgeons, this technique can attain clinical outcomes similar to open surgery. However, despite the above-mentioned advantages, laparoscopy requires extremely advanced surgical skills to manipulate the rigid and long instrumentation. The entry incision acts as a point of rotation, decreasing the surgeon's freedom for positioning and orientating the instruments inside the patient. The movements of the surgeon's hand about this incision are inverted and scaled-up relative to the instrument tip ("fulcrum effect"), which removes dexterity, sensibility and magnifies the tremors of the surgeon's hands. In addition, these long and straight instruments force surgeons to work in an uncomfortable posture, which can be tremendously tiring during several hours of operation and result in stress and discomfort for hands, arms and body. Therefore, due to these drawbacks of laparoscopic instrumentation, these minimally invasive techniques are mainly limited to use in simple surgeries, while only a small minority of surgeons is able to use them in complex procedures.

To overcome these limitations, surgical robotic systems were developed to provide an easier-to-use approach to

complex minimally invasive surgeries. By means of a computerized robotic interface, these systems enable the performance of remote laparoscopy wherein the surgeon sits at a console manipulating two master manipulators to perform the operation through several small incisions. Like laparoscopy, the robotic approach is also minimally invasive, bringing several advantages over open surgery in terms of pain, blood loss, and recovery time. In addition, it also offers better ergonomics for the surgeon compared to open and laparoscopic techniques. However, although being technically easier, robotic surgery brings several negative aspects. A major disadvantage of these systems is related to the extremely high complexity of existing robotic devices, which are composed of complex mechanical and electronic systems, leading to huge costs of acquisition and maintenance, which are not affordable for the majority of surgical departments worldwide. Another drawback of these systems comes from the fact that current surgical robots are very large, competing for precious space within the operating room environment and significantly increasing preparation time. Access to the patient is thus impaired, which, together with a lack of force-feedback, raises safety concerns.

In addition to robotic systems, several hand-held laparoscopic instruments are known. These instruments provide access to the surgical field without the need for an expensive and cumbersome robotic system, but they often provide poor ergonomics to the user.

There are known examples of hand-held, articulated surgical instruments. However, they present significant drawbacks in their designs. For example, one known articulated instrument (ref) must be attached to the user's forearm by a frame, making its use cumbersome and likely tiring, given that every movement must involve the user moving his entire forearm, which needs to be geometrically aligned with the instrument's shaft. Other known articulated instruments (refs) require the manipulation of knobs or similar elements on the device handle to produce corresponding movements in an end-effector. Such arrangement does not allow for a natural replication of user hand movements.

Accordingly, an aim of the present invention is to provide an articulated hand-held medical instrument that allows for a natural replication of user hand movements on the instrument handle at an end effector. The instrument is to allow for good ergonomics and ease of use as compared to known hand-held articulated instruments.

SUMMARY OF THE INVENTION

These aims and other advantages are achieved by a new articulated hand-held medical instrument. The articulated hand-held medical instrument of the present invention is primarily intended to be used in minimally invasive surgical procedures.

The articulated hand-held medical instrument comprises a frame, a proximal handle and a distal end-effector. The proximal handle is joined to the distal end-effector by an instrument tube and a structural frame. The instrument tube may optionally be introduced to the patient's body during a minimally invasive surgical procedure through a trocar or other standard piece of equipment.

The proximal handle of the articulated hand-held surgical instrument is made up of a series of handle links connected by handle joints. The distal end-effector element is generally made up of a number of end-effector links connected by end-effector joints. Mechanical transmission means transmit user motions performed on the proximal handle to the distal end-effector. In this way, the articulated hand-held surgical

instrument has a master-slave architecture allowing for the replication of user hand movements on the proximal handle at the distal end-effector. Taken in conjunction with the multiple links and degrees of freedom, this architecture allows for greater dexterity and ergonomics than that accessible with standard laparoscopic instruments.

BRIEF DESCRIPTION OF FIGURES

The invention will be better understood according to the following detailed description of several embodiments with reference to the attached drawings, in which:

FIG. 1 shows a perspective view of the articulated instrument according to an embodiment of the present invention.

FIG. 2 shows a detailed perspective view of the articulated instrument according to an embodiment of the present invention;

FIG. 3 shows a detailed side view of the articulated instrument according to an embodiment of the present invention;

FIG. 4 shows a detailed top view of the articulated instrument according to an embodiment of the present invention;

FIG. 5 shows the distal end-effector of the articulated instrument according to an embodiment of the present invention in a first active position;

FIG. 6 shows the distal end-effector of the articulated instrument according to an embodiment of the present invention in a second active position;

FIG. 7 shows the distal end-effector of the articulated instrument according to an embodiment of the present invention in a third active position;

FIG. 8 shows the distal end-effector of the articulated instrument according to an embodiment of the present invention in a fourth active position;

FIG. 9 shows the distal end-effector of the articulated instrument according to an embodiment of the present invention in a fifth active position;

FIG. 10 shows a simplified path of a flexible transmission system actuating a distal end-effector articulation of the articulated instrument according to an embodiment of the present invention;

FIG. 11 shows a simplified path of a rigid transmission system actuating a distal end-effector articulation of the articulated instrument according to a different embodiment of the present invention;

FIG. 12 shows the articulated instrument according to an embodiment of the present invention in a first active position;

FIG. 13 shows the articulated instrument according to an embodiment of the present invention in a second active position;

FIG. 14 shows the articulated instrument according to an embodiment of the present invention in a third active position;

FIG. 15 illustrates the actuation of the two distal end-effector links of the articulated instrument according to an embodiment of the present invention;

FIG. 16 shows a schematic side view of the articulated instrument, according to an embodiment of the current invention;

FIG. 17 shows a perspective view of a clamp system used in the proximal handle of the articulated instrument, according to an embodiment of the current invention;

FIG. 18 shows a perspective view of a spring system used in the proximal handle of the articulated instrument, according to an embodiment of the current invention;

FIG. 19 shows a procedure through which an external tube of an instrument shaft can be assembled and disassembled on the articulated instrument according to an embodiment of the present invention;

FIG. 20 shows a distal part of an articulated instrument detached from the proximal part of the articulated instrument according to an embodiment of the present invention;

FIG. 21 shows a distal part of an articulated instrument detached from the proximal part of the articulated instrument according to another embodiment of the present invention;

FIG. 22 shows a detachable distal part of an articulated instrument according to an embodiment of the present invention;

FIG. 23 shows the rotational elements of an interface portion of a distal part of the articulated instrument according to an embodiment of the present invention;

FIG. 24 shows the rotational kinematics of an interface portion of a distal part of the articulated instrument according to an embodiment of the present invention;

FIG. 25 shows schematically the sterile interface between the distal and proximal parts of the articulated instrument according to an embodiment of the current invention;

FIG. 26 shows a perspective view of a rigid connector composing a sterile interface operationally mounted between the distal and proximal parts of the articulated instrument according to an embodiment of the current invention;

FIG. 27 illustrates the actuation of the two distal end-effector links of the articulated instrument according to an embodiment of the present invention;

FIG. 28 shows an alternative kinematics of the articulated instrument according to an embodiment of the present invention;

FIG. 29 shows an alternative kinematics of the articulated instrument according to an embodiment of the present invention;

FIG. 30 shows an alternative kinematics of the articulated instrument according to an embodiment of the present invention;

FIG. 31 shows an alternative kinematics of the articulated instrument according to an embodiment of the present invention.

FIG. 32 shows a kinematic model of an embodiment of the present invention displaying the position of the user's wrist joint relative to that of a centre of rotation of the handle.

FIGS. 33 and 34 show alternative kinematic models of embodiments of the present invention displaying alignment of the user's wrist joint relative to the centre of rotation of the handle.

FIGS. 35, 36 and 37 show embodiments of the present invention where the user's wrist is in alignment with the centre of rotation of the handle.

FIGS. 38 and 39 show kinematic models of embodiments of the present invention including a wrist alignment concept in accordance with the invention.

FIGS. 40 and 41 show representative handle links that may be used in accordance with embodiments of the present invention.

FIG. 42 shows a schematic view of a cable rooting method to maintain a closed loop with a constant length, shown at the joint level, in accordance with various embodiments of the present invention;

FIG. 43 shows a schematic view of another cable rooting method to maintain a closed loop with a constant length,

shown at the level of equivalent handle/end-effector joints, in accordance with various embodiments of the present invention;

FIGS. 44, 45 and 46 show different views, with main dimensions, of a detailed design of an embodiment of the present invention.

FIGS. 47, 48 and 49 show the mechanical transmission elements of the different degrees-of-freedom of the instrument, in accordance with various embodiments of the present invention.

FIGS. 50 and 51 show detailed views of the instrument's actuation system, in accordance with various embodiments of the present invention.

DETAILED DESCRIPTION OF THE INVENTION

The articulated instrument 1 of FIG. 1, according to an embodiment of the present invention, is intended to be used in minimally invasive surgical procedures.

One of the key features of this type of articulated instrument 1 lies in its master-slave architecture, which enables the replication of the user hand movements, on a proximal handle 3 (the master), by a distal end-effector 2 (the slave) inside the patient's body.

According to FIGS. 1, 2, 3 and 4, the articulated instrument 1 comprises: i) a proximal handle 3 having a number of handle links 15, 17, 18 interconnected by a plurality of handle joints, represented by rotations over the axes 12, 13, 42; a ii) a frame 5, structurally connecting the proximal handle 3 to the distal portion of the articulated instrument 1; iii) a distal end-effector 2 having a number of end-effector links 6, 7, 8 interconnected by a plurality of end-effector joints, corresponding to the handle links, and represented by rotations over the axes 11 and 10; and iv) an instrument shaft 4, connecting the distal end of the frame 5 to the distal end-effector 2. More particularly, the kinematic chain formed by the plurality of articulated end-effector links 6, 7, 8 and corresponding end-effector joints 11, 10 of the end-effector 2, may be substantially identical to the kinematic chain formed by the plurality of articulated handle links 15, 17, 18 and corresponding handle joints 12, 13, 42 of the proximal handle 3. As can be seen in FIG. 2, in some embodiments of the present invention, the axes 9, 12, and 13 are perpendicular to each other and intersection at a central rotation point 14, which is kinematically equivalent to a spherical joint.

Referring to FIGS. 2, 3 and 4, the end-effector 2 is connected to the distal extremity of the instrument shaft 4 by a proximal end-effector joint, which allows the rotation of the proximal end-effector link 6 by the proximal axis 11 in such a manner that the orientation of the proximal end-effector link 6 with respect to the main axis 9 of the instrument shaft 4 can be changed. The distal end-effector links 7, 8 are pivotally connected to the proximal end-effector link 6 by two distal joints, having coincident axes of rotation, which are represented by the distal axis 10. This distal axis 10 is substantially perpendicular and non-intersecting with the proximal axis 11 and substantially intersects the main axis 9 of the instrument shaft 9. FIGS. 5 to 7 show the end-effector 2 with different angular displacements at the proximal end-effector link 6.

By actuating the two distal joints, the two distal end-effector links 7, 8 can be angulated over the distal axis 10, with respect to the plane containing the main axis 9 and the distal axis 10, by the angles θ_7 , θ_8 . Consequently, through the combination of rotations θ_7 and θ_8 , it is possible to

operate the surgical instrument 1, in such a manner as to provide orientation motions between the end effector and the instrument shaft 4 (FIG. 8) and to accomplish its "open/close" function (FIG. 9).

The articulated instrument 1 further comprises mechanical transmission systems arranged to kinematically connect the distal end-effector 2 with the proximal handle 3 such that the movement (angle of joint) applied on each handle joint of the proximal handle 3 is reproduced by the corresponding end-effector joint of the distal end-effector 2.

For each degree of freedom of the articulated instrument 1, different types of mechanical transmission can be used. In order to minimize the system's overall friction and inertia, certain embodiments of the current invention may use a mechanical transmission in the form of pulley-routed flexible elements, where each driven pulley of the distal end-effector 2 is connected to the respective driving pulley of the proximal handle 2, by a closed cable loop transmission. As can be seen in FIG. 10, the action of the user creating a rotation α_3 on a general handle link L3 produces a rotation α_3 on the handle pulley P3, which is directly connected to the handle link L3. Then, the mechanical transmission system, composed by the closed cable loop comprising cables C1 and C2, passes by the frame 5 and the instrument shaft 4 and is able to kinematically connect the handle pulley P3 to the end-effector pulley P2 (a system of idle pulleys I1, I2 is used to guide the cables C1, C2 on their path). As a result, the user actuation α_3 on the handle link L3 is reproduced by the rotation α_2 of the handle link L2. Depending of the use of amplification elements, α_2 may be smaller, bigger or the same as α_3 .

The transmission of the movement between each handle pulley and the corresponding end-effector pulley in the aforementioned embodiments, by using this kind of mechanical transmission, may present certain drawbacks pertaining to kinematic and dynamic coupling between the driven and the driving pulleys. Furthermore, the adoption of a closed loop cable transmission requires that the overall length of the cable route must be kept constant, for all possible handle/end-effector configurations, independently of the motion performed by the driving pulleys of the articulated handle 2. In this sense, the aforementioned embodiments of the present invention will be operational but may not accommodate all possible use cases.

Therefore, cables must be routed through joint idler pulleys while maintaining constant cable length. The basics of the cable routing method used in this invention is illustrated in FIG. 42 for the general case of having both cables La and Lb, composing the closed loop L, being routed through a general pivot joint. The cables La and Lb are wrapped around a set of pulleys, Im, called the "joint idler pulleys," which are concentric with the joint's axis of rotation. To maintain constant cable length of the closed loop, cables La, Lb must remain in contact with the joint idler pulleys at all times. In this way, if the joint angle θ_j is reduced, the length of the superior segment of La, in contact with the idler pulley Im will decrease and the inferior segment of Lb will increase, by the same value, guaranteeing the constant length of the cable closed loop. In addition, in order to keep a permanent contact between the cables La and Lb with the idler pulleys Im, auxiliary pulleys Ap and Ad may be added.

Another solution to keep a constant cable length of the closed loop consists in compensating the length change not at the joint level but between the equivalent idler pulleys Im and Is of respective handle and end-effector as schematically shown in FIG. 43. In this case, both cables La, Lb are

passing under I_m and I_s and, when the joint angle θ_j , θ'_j , is changed, the constant length of the closed loop is guaranteed because the increase/reduction of θ_s is compensated by the reduction/increase of θ_m .

In a different embodiment, as is conceptually illustrated in FIG. 11, the mechanical transmission may comprise rigid elements R1, R2, R3, instead of flexible elements C1, C2, to transmit motion between the handle link L3 and the end-effector link L2. Other embodiments can be achieved by combining flexible elements with rigid elements and/or geared components.

FIGS. 12 to 14 show the articulated instrument 1 with different angular displacements at the proximal handle link 15 (and therefore, proximal end-effector link 6). The geometry of frame 5 allows for the movement of the handle 3 in its full range of motion.

In the preferred embodiment of the current invention, the actuation θ_{18} of the handle link 18 is able to produce simultaneous rotations θ_7 , θ_8 on both the end-effector links 7, 8, with a certain movement amplification ratio. However, as shown in FIG. 15, a second distal handle link 18' may exist, so that its actuation θ_{18}' can actuate the end-effector link 7 by a rotation θ_7 and the actuation θ_{18} of the handle link 18 is actuating uniquely the end-effector link 8 by a rotation θ_8 .

In a different embodiment of the current invention, as shown in FIG. 27, the axis 42, around which the handle link 18 is able to rotate θ_{18} might be not parallel to the axis 10 around which the distal end-effector links 7, 8 are moving θ_7 , θ_8 , providing a different ergonomic position to the user. FIGS. 28 to 31 show alternative kinematics of the articulated instrument 1 according to different embodiments of the present invention.

In another embodiment of the current invention, the handle link 18 may be replaced by another handle link 19, whose axis of rotation 20 is perpendicular and non-intersecting with the axis 13 (FIG. 16), providing a different ergonomomy to the user.

As can be seen in FIG. 17, a clamp element 21 may be used on the handle 3 in order to block the movement of the handle link 18 when it is brought to the "closed" position. This is particularly useful when the end-effector comprises a needle holder instrument and the user wants to apply high and constant gripping forces on needles when performing suturing tasks. Therefore, when the handle link 18 is brought θ_{18} to its "closed" position, its movement is blocked by a wedge/step geometry 21a (actuated by a system of miniature springs 22) of the clamp element 21 (FIG. 17). Then, in order to unlock the movement of the handle link 18, the user should press the clamp element 21 downwards, so that the handle link 18 can pass back through the wedge/step geometry 21a of the clamp element 21.

In another embodiment, the handle 3 may be provided with a spring element 23 that can bring the handle link 18 to an "opened" default position (FIG. 18) and apply a resistance torque when the handle link 18 is moving towards a "closing" direction.

As can be seen in FIG. 19, the external tube 4a, composing the instrument shaft 4, can be easily and individually detached and attached to the articulated instrument 1 after each procedure. Referring to FIG. 19, the internal structural element 4b is fixed directly to the frame 5 and the external tube 4a can be connected and disconnected from the internal structural element 4b by threaded surfaces or any other attachment mechanism. Therefore, with this architecture, the external tube 4a can be removed from the articulated instrument 1, without the need to disassemble other parts of the

system, like the articulated end-effector 2 or the mechanical transmission elements 25, which remain completely operational without the external tube 4a. This feature facilitates tremendously the procedure to effectively clean and sterilize the articulated instrument 1, which can easily be performed by the hospital staff.

Towards a more distal region of the instrument shaft 4, the external tube 4a is in contact with a sealing element 24, which fills the gap between the internal surface of the external tube 4a and the internal structural element 4b. This sealing element 24 has little channels through which the transmission elements 25 can pass, guaranteeing the airtightness of the articulated instrument 1.

In order to farther facilitate the cleaning and sterilization procedure, the distal part of the articulated instrument 1 may be able to be easily attached and detached to the proximal part of the articulated instrument 1. In one possible embodiment of the current invention, the attachment/detachment between the distal 26 and the proximal 27 parts of the articulated instrument 1 can be done between the frame 5 and the handle 3 (FIG. 20). However, in another embodiment of the current invention, the attachment/detachment between the distal 28 and the proximal 29 parts of the articulated instrument 1 can be done between the instrument shaft 4 and the frame 5 (FIG. 21).

In the above mentioned embodiment, the detachable distal instrument 28 may be provided with a distal articulated end-effector 2, a proximal hub 30 and the instrument shaft 4, through which different mechanical elements 25 may pass, delivering motion to the different end-effector links 6, 7, 8 (FIG. 22) from the proximal hub 30.

With reference to FIGS. 23 and 24, the movement is transmitted to each one of the three distal articulations of the articulated instrument 1 by a rotating element 31, 32, 33, which is able to rotate about the axis 9 and is connected to one of the transmission elements 25. As a result, when the rotating element 31, 32, 33 rotates a certain angle θ_1 , θ_2 , θ_3 about the axis 9, a rotation α_1 , α_2 , α_3 is transmitted to the respective end-effector link 6, 7, 8.

Since the distal part 28 of the surgical instrument 1 is partially entering the patient's body, it has to be sterile, just like the area in the vicinity of the patient. On the other hand, the proximal part 29 of the articulated instrument 1 may not be sterile and therefore should be separated from the sterile instrument portions 28 by a sterile interface 43 which protects the sterile area from the non-sterile components 29 of the articulated instrument 1 (FIG. 25).

The sterile interface 43 comprises two main components: a flexible sleeve 35, which covers the moving links of the proximal part 29 of the articulated instrument 1 and a rigid connector 35, which i) guarantees that the sterile distal part 28 of the articulated instrument 1 is not directly touching the non-sterile components of the proximal part 29, ii) enables attachment/detachment between the distal 28 and the proximal 29 parts of the articulated instrument 1, and iii) ensures the connection/disconnection of the mechanical transmission systems that deliver motion to the end-effector links 6, 7, 8.

FIG. 26 shows how the rigid connector 34 can be disposed and operationally mounted between the proximal hub 30 and the proximal part 29 of the articulated instrument 1. In order to connect/disconnect the mechanical transmission systems that deliver motion to the end-effector links 6, 7, 8, three cylindrical elements 36, 37, 38, from the proximal part 29 of the articulated instrument 1, are inserted on three miniature cups 39, 40, 41 of the rigid connector 34, which are then inserted on the rotating elements 31, 32, 33. In this way, it

can be guaranteed that the sterile surgical instrument **28** is not directly touching non-sterile components.

In other embodiments of the current invention, the movement of some of the three cylindrical elements **36**, **37**, **38**, from the proximal part **29** of the articulated instrument **1**, may be constrained so that some degrees-of-freedom of the end-effector **2** can be locked/unlocked in their range of movement, allowing for instance the use of the articulated instrument **1** as a standard laparoscopic instrument, with a single degree-of-freedom at the end-effector.

The articulated hand-held medical instrument of the present invention is designed to be used in a full range of minimally invasive surgical procedures in combination with standard laparoscopic equipment. For example, the inventive instrument may optionally be inserted through a trocar and its movements inside the patient's body may be tracked with an available endoscopic camera. In addition, the articulated hand-held medical instrument may be used in a range of port arrangements in minimally invasive surgical procedures.

The articulated instrument **1** can assume other kinematics, like the kinematic models shown in FIGS. **28** to **31**.

As illustrated in FIG. **32**, in most of the embodiments (and kinematic models) described up to this point, the central rotation point **14** of the articulated handle **3** is not coincident with the central wrist point **43** of the user **44**. However, these positional offsets Δx , Δy (and possibly Δz) can create positional mismatches (also known as "parasitic movements") between the movements applied to the handle **3** and the movements generated at the end-effector **2**. In particular, a pure rotation performed by the user's hand at the handle **3** might create a composed movement, of rotation plus a translation, of the end-effector **2**. Therefore, in order to compensate for that, the central rotation point **14** and the central wrist point **43** have to be aligned. In order to achieve this, other kinematic models (like the ones of FIGS. **33**, **38** and **39**) can be used on the articulated instrument **1** of the current invention so that the central rotation point **14** is located in the free space and not within the structure of the moving links **5**, **45**, **46** (this kinematic feature may also be designated by Remote Center of Motion, RCM). In some of these embodiments, like the one of FIGS. **35**, **36** and **37**, there are three revolute joints whose axes **9**, **12**, **13** intersect at the RCM. Thus, the kinematics of the articulated instrument **1** can be set so that the central rotation point **14** (or RCM) is substantially coincident to the central wrist point **44** of the user **43**. FIGS. **36** and **37** show a side and top view of this alignment.

FIGS. **38** and **39** show two additional embodiments of the current invention using two different kinematic models. The articulated instrument **1** of FIG. **38** uses a double parallelogram mechanism **47** to achieve its RCM, where the central rotation point **14** is set to be substantially coincident to the central wrist point **44** of the user **43**. The articulated instrument **1** of FIG. **39** uses a spherical mechanism, having a circular track **49** as the movement base, whose center is aligned with the axis **9** of the instrument shaft **4**. Mounted on the circular track **49**, a radial sliding element **50** comprises a collinear rotational joint **51** and is always aligned with the RCM (the central rotation point **14**) at the center of the circular track **49**.

In order to provide an ergonomic manipulation and gripping functionality to the user, the handle **3** of the articulated instrument **1** may be compatible with handle links **17** and **18** of multiple shapes and sizes. Therefore, while in the embodiment of FIG. **40**, the handle links **17** and **18** may have a joystick-like or pistol-grip-like shape, in the embodiment

shown in FIG. **41**, the handle links **17** and **18** have a scissors-like or needle-holder-like configuration.

FIGS. **44** to **46** show three different views (with main dimensions) of a possible embodiment of the current invention. These figures show a detailed design version of the embodiment of FIGS. **35** to **37**, with the kinematic model of FIGS. **33** and **34**.

In order to be as light in weight as possible, the articulated instrument **1** may be, in the main, constructed of aluminum components, although the invasive part of the instrument should be mainly constructed of medical grade stainless steel and polymers. The mechanical transmission is essentially constructed of tungsten ropes, although steel or polymeric ropes could also be used in some specific situations, depending on the target number of cleaning and sterilization cycles that the instrument should support.

The mechanical transmission elements for each one of the three degrees of freedom of the instrument are shown are shown in FIG. **47** to FIG. **49**, as described in more detail below.

FIG. **48** shows the transmission of motion between the handle **3** and end-effector **2** for the proximal degree of freedom. Joints around the axes **11** and **13** are connected by a cable **52** in a single closed loop configuration (in some embodiments, it may comprise two segments of cable **52a** and **52b**) which runs from a driving pulley **C13** connected to the proximal handle link **45** and passing through 3 sets of guiding pulleys **G1**, **G2** and **G3** up to a driven pulley **C6**, connected to the proximal end-effector link **6**. The sets of guiding pulleys are used to shape the path of the transmission cables to the geometry of the frame **5** or handle links.

FIG. **49** shows the transmission of motion between the handle **3** and end-effector **2** for a first distal degree of freedom. Joints around the axes **10** and **12** are connected by a cable **53** in a single closed loop configuration (in some embodiments, it may comprise two segments of cable **53a** and **53b**) which runs from a driving pulley **C12** up to a driven pulley **C10**, connected to the proximal end-effector link **7**. On their path from the driving pulley **C12** to the driven pulley **C6**, the closed loop cable **53** passes through 6 sets of guiding pulleys **G1**, **G2**, **G3**, **G4**, **G5**, **G6** and a set of joint idle pulleys **JIP**. Although this degree-of-freedom is driven by pulley **C12**, the closed cable loop is not directly attached to it. Instead they are attached to a distal actuation pulley **55**, which couples the movement of the two distal degrees-of-freedom (shown in FIGS. **8** and **9**) so that they perform the actuation of the instrument in parallel. The motion transmission between the handle **3** and end-effector **2** for the second distal degree of freedom is analogous, with a similar arrangement of cable loops and pulleys.

Attached to the distal actuation pulley **55**, there is an actuation shaft **56** (FIGS. **50** and **51**), which transmits the actuation input movement from the handle link **18**. Handle link **18** is rigidly attached to an actuation link **57**, which is connected by a linkage system **58** to the actuation shaft **56**. A spring system **59** is permanently acting on the linkage system **58**, bringing the actuation link **57** to a default open position. When brought to its maximum closed position, the actuation link **57** can be temporarily blocked by a spring-actuated ratcheting mechanism **60**, which can be deactivated by pressing up the thumb trigger **61**.

While this invention has been shown and described with reference to particular embodiments thereof, it will be understood by those skilled in the art that various changes in form and details may be made therein without departing from the spirit and scope of the invention as defined by the appended claims.

The invention claimed is:

1. A handheld surgical instrument comprising:
an instrument shaft having a proximal end and a distal end;
an articulated handle;
an articulated end effector connected to the distal end of the instrument shaft;
a structural frame having a proximal end mounted on the articulated handle and a distal end coupled to the proximal end of the instrument shaft, the structural frame comprising three joints, each of the three joints having an axis that intersects at a remote center of motion of the handheld surgical instrument, the remote center of motion configured to be coincident to a central point of a user's wrist; and
a flexible mechanical transmission system connecting the articulated handle to the articulated end effector such that motion applied to the articulated handle is reproduced at the articulated end effector,
wherein the articulated end effector comprises at least three orientation or actuation degrees of freedom, and wherein the flexible mechanical transmission system follows a continuous path from a proximal end of the articulated handle to the distal end of the articulated handle and then from the proximal to the distal end of the structural frame and then from the proximal to the distal end of the instrument shaft and then from a proximal end of the articulated end-effector to a distal end of the articulated end effector.
2. The handheld surgical instrument of claim 1, wherein the flexible mechanical transmission system comprises a system of cables and pulleys disposed at the articulated handle and articulated end effector.
3. The handheld surgical instrument of claim 2, wherein the flexible mechanical transmission system comprises a closed loop configuration.
4. The handheld surgical instrument of claim 3, wherein at least one of the cables of the system of cables and pulleys runs from a driving pulley coupled to the articulated handle, through a plurality of guiding pulleys, to a driven pulley coupled to the articulated end effector.
5. The handheld surgical instrument of claim 1, wherein the handle comprises a joystick-like or pistol-grip-like shape.
6. The handheld surgical instrument of claim 1, wherein a geometry of the structural frame allows alignment of the human user's wrist with the remote center of motion of the handheld surgical instrument.
7. The handheld surgical instrument of claim 6, wherein the geometry of the structural frame allows the articulated handle a full range of movement without colliding with the instrument shaft.
8. The handheld surgical instrument of claim 1, wherein the articulated handle comprises a plurality of handle links connected by a corresponding plurality of handle joints and wherein the articulated end effector comprises a plurality of end-effector links connected by a corresponding plurality of end effector joints, and wherein the number of handle links is equal to the number of end-effector links.
9. The handheld surgical instrument of claim 1, wherein the handle comprises a scissors-like or needle-holder-like configuration.
10. The handheld surgical instrument of claim 1, wherein the at least three degrees of freedom of the articulated end effector comprise at least two orientational degrees of freedom and at least one actuation degree of freedom.

11. The handheld surgical instrument of claim 10, wherein at least two of the orientational degrees of freedom have a serial kinematic disposition.

12. The handheld surgical instrument of claim 10, wherein the at least one actuation degree of freedom is disposed in parallel to the orientational degrees of freedom.

13. The handheld surgical instrument of claim 1, wherein the flexible mechanical transmission system comprises cables made from steel or tungsten.

14. A method for performing a minimally invasive, remotely actuated surgical procedure using the handheld surgical instrument of claim 1, the method comprising:

positioning the user's hand at the articulated handle such that the remote center of motion of the handheld surgical instrument is coincident with the central point of the user's wrist;

laparoscopically introducing the articulated end effector into a patient to a desired location for the surgical procedure; and

actuating the articulated handle such that motion applied to the articulated handle is reproduced at the articulated end effector in at least one orientation or actuation degrees of freedom via the flexible mechanical transmission system for performing the surgical procedure.

15. The method of claim 14, wherein the motion reproduced at the articulated end effector comprises a composed movement of rotation and translation.

16. The method of claim 14, wherein the at least one orientation or actuation degrees of freedom comprises at least two orientational degrees of freedom and at least one actuation degree of freedom.

17. The method of claim 14, wherein a geometry of the structural frame allows the user to articulate the articulated handle in a full range of movement without colliding with the instrument shaft.

18. A handheld surgical instrument comprising:
an instrument shaft having a proximal end and a distal end;

an articulated handle;

an articulated end effector connected to the distal end of the instrument shaft;

a structural frame having a proximal end mounted on the articulated handle and a distal end coupled to the proximal end of the instrument shaft, the structural frame comprising three joints, each of the three joints having an axis that intersects at a remote center of motion of the handheld surgical instrument, the remote center of motion configured to be coincident to a central point of a user's wrist; and

a flexible mechanical transmission system connecting the articulated handle to the articulated end effector such that motion applied to the articulated handle is reproduced at the articulated end effector,

wherein the articulated end effector comprises at least three orientation or actuation degrees of freedom, and wherein the articulated handle comprises a plurality of handle links connected by a corresponding plurality of handle joints and wherein the articulated end effector comprises a plurality of end-effector links connected by a corresponding plurality of end effector joints, and wherein the number of handle links is equal to the number of end-effector links.

19. The handheld surgical instrument of claim 18, wherein motion applied to a particular handle link is reproduced at the corresponding end-effector link.

20. A handheld surgical instrument comprising:
an instrument shaft having a proximal end and a distal
end;
an articulated handle;
an articulated end effector connected to the distal end of 5
the instrument shaft;
a structural frame having a proximal end mounted on the
articulated handle and a distal end coupled to the
proximal end of the instrument shaft, the structural
frame comprising three joints, each of the three joints 10
having an axis that intersects at a remote center of
motion of the handheld surgical instrument, the remote
center of motion configured to be coincident to a
central point of a user's wrist; and
a flexible mechanical transmission system connecting the 15
articulated handle to the articulated end effector such
that motion applied to the articulated handle is repro-
duced at the articulated end effector,
wherein the articulated end effector comprises at least
three orientation or actuation degrees of freedom, 20
wherein the flexible mechanical transmission system
comprises a system of cables and pulleys disposed at
the articulated handle and articulated end effector and
the flexible mechanical transmission system comprises
a closed loop configuration, and 25
wherein at least one of the cables of the system of cables
and pulleys runs from a driving pulley coupled to the
articulated handle, through a plurality of guiding pul-
leys, to a driven pulley coupled to the articulated end
effector. 30

* * * * *

专利名称(译)	铰接式手持式仪器		
公开(公告)号	US10363055	公开(公告)日	2019-07-30
申请号	US15/564194	申请日	2016-04-11
[标]申请(专利权)人(译)	DISTALMOTION		
申请(专利权)人(译)	DISTALMOTION SA		
当前申请(专利权)人(译)	DISTALMOTION SA		
[标]发明人	BEIRA RICARDO DANIEL RITA FRIEDRICH MICHAEL URS		
发明人	BEIRA, RICARDO DANIEL RITA FRIEDRICH, MICHAEL URS		
IPC分类号	A61B17/29 A61B34/00 A61B17/00 A61B90/00		
CPC分类号	A61B17/2909 A61B17/00234 A61B17/29 A61B34/71 A61B2017/0046 A61B2090/0813 A61B2017/00738 A61B2017/291 A61B2017/2927 A61B2017/2929 A61B2017/2948 A61B2017/00424		
优先权	62/280736 2016-01-20 US 62/145454 2015-04-09 US		
其他公开文献	US20180125519A1		
外部链接	Espacenet		

摘要(译)

提供一种铰接式手持式医疗器械。该仪器主要用于微创外科手术。铰接式器械包括主从结构，其中近侧手柄元件上的使用者手部运动被复制在远端末端执行器上。近端手柄包括由手柄关节连接的多个手柄连杆，手柄连接件对应于由末端执行器关节连接的多个末端执行器连杆。铰接式手持式医疗器械可以在各种端口布置的标准腹腔镜手术中使用，并且通过使用诸如套管针的标准设备，并且可以使用可用的内窥镜摄像机跟踪患者体内的运动。

