



US010595978B2

(12) **United States Patent**
Lavigne et al.

(10) **Patent No.:** **US 10,595,978 B2**
(45) **Date of Patent:** **Mar. 24, 2020**

(54) **SYSTEM AND METHOD OF
LAPAROSCOPIC USE OF HEMOSTATIC
PATCH**

(71) Applicant: **Covidien LP**, Mansfield, MA (US)

(72) Inventors: **Kevin Lavigne**, Hamden, CT (US);
Steven Bennett, Cheshire, CT (US);
Nathaniel Mast, Hamden, CT (US)

(73) Assignee: **Covidien LP**, Mansfield, MA (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 445 days.

(21) Appl. No.: **15/423,625**

(22) Filed: **Feb. 3, 2017**

(65) **Prior Publication Data**

US 2017/0143464 A1 May 25, 2017

Related U.S. Application Data

(62) Division of application No. 12/791,534, filed on Jun.
1, 2010, now Pat. No. 9,592,108.

(60) Provisional application No. 61/229,333, filed on Jul.
29, 2009.

(51) **Int. Cl.**

A61F 2/00 (2006.01)
A61L 27/34 (2006.01)
A61L 27/52 (2006.01)
A61L 27/56 (2006.01)
A61B 17/34 (2006.01)
A61B 17/00 (2006.01)

(52) **U.S. Cl.**

CPC **A61F 2/0063** (2013.01); **A61L 27/34**
(2013.01); **A61L 27/52** (2013.01); **A61L 27/56**
(2013.01); **A61B 17/3468** (2013.01); **A61B**
2017/00287 (2013.01); **A61F 2002/0072**
(2013.01)

(58) **Field of Classification Search**

CPC . A61F 2/0036; A61F 2002/0072; A61B 17/08

USPC 606/151

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,364,200 A 1/1968 Ashton et al.
4,626,253 A 12/1986 Broadnax, Jr.
5,201,745 A 4/1993 Tayot et al.
5,397,332 A * 3/1995 Kammerer A61B 17/0057
604/14

(Continued)

FOREIGN PATENT DOCUMENTS

EP 1707130 A1 10/2006
EP 2177239 A2 4/2010

(Continued)

OTHER PUBLICATIONS

European Search Report for EP 09252417.2-1219 dated Dec. 12,
2010.

(Continued)


Primary Examiner — Julie A Szpira

(74) *Attorney, Agent, or Firm* — Carter, DeLuca & Farrell
LLP

(57) **ABSTRACT**

The present disclosure includes systems and a method for in
situ application of a surgical patch during minimally inva-
sive surgery. The method includes the steps of inserting a
surgical patch into a bag; transferring a polymeric bag
containing a hemostatic patch into a body cavity; removing
the surgical patch from the polymeric bag while the poly-
meric bag is within the body cavity; and applying the
surgical patch to a tissue within the body cavity.

16 Claims, 5 Drawing Sheets

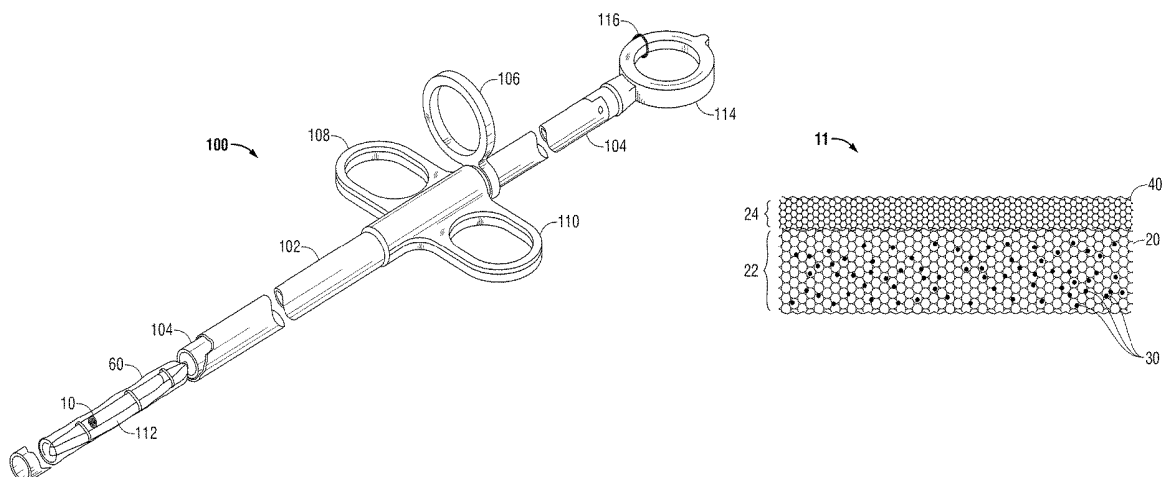

(56)

References Cited

U.S. PATENT DOCUMENTS

5,484,913 A 1/1996 Stilwell et al.
 6,152,943 A 11/2000 Sawhney
 6,165,201 A 12/2000 Sawhney et al.
 6,179,862 B1 1/2001 Sawhney
 6,443,964 B1 9/2002 Ory et al.
 6,500,777 B1 12/2002 Wiseman et al.
 6,514,534 B1 2/2003 Sawhney
 6,566,406 B1 5/2003 Pathak et al.
 6,605,294 B2 8/2003 Sawhney
 6,673,093 B1 1/2004 Sawhney
 6,703,047 B2 3/2004 Sawhney et al.
 6,818,018 B1 11/2004 Sawhney
 6,946,003 B1 * 9/2005 Wolowacz A61F 2/08
 623/23.72
 7,009,034 B2 3/2006 Pathak et al.
 7,021,086 B2 4/2006 Ory et al.
 7,347,850 B2 3/2008 Sawhney
 9,592,108 B2 3/2017 Lavigne et al.
 2002/0106409 A1 8/2002 Sawhney et al.
 2003/0031697 A1 2/2003 Chudzik et al.
 2004/0028655 A1 * 2/2004 Nelson A61K 47/6953
 424/93.2
 2004/0092970 A1 * 5/2004 Xavier A61B 17/00234
 606/151
 2006/0200169 A1 9/2006 Sniffin

2006/0200170 A1 9/2006 Aranyi
 2006/0229640 A1 10/2006 Whitfield
 2008/0082113 A1 * 4/2008 Bishop A61B 17/06166
 606/151
 2010/0042045 A1 * 2/2010 Splvey A61F 2/0063
 604/93.01
 2011/0070288 A1 3/2011 Andjelic

FOREIGN PATENT DOCUMENTS

EP 2179753 A2 4/2010
 GB 2459902 A 11/2009
 WO 2004037123 A1 5/2004
 WO 2007081940 A2 7/2007
 WO 2010019655 A1 2/2010
 WO 2010043980 A2 4/2010

OTHER PUBLICATIONS

European Search Report for EP 09252421.4-1219 dated Dec. 12, 2010.
 Canadian Office Action issued in corresponding Canadian Application No. 2,709,046 dated Mar. 29, 2016.

* cited by examiner

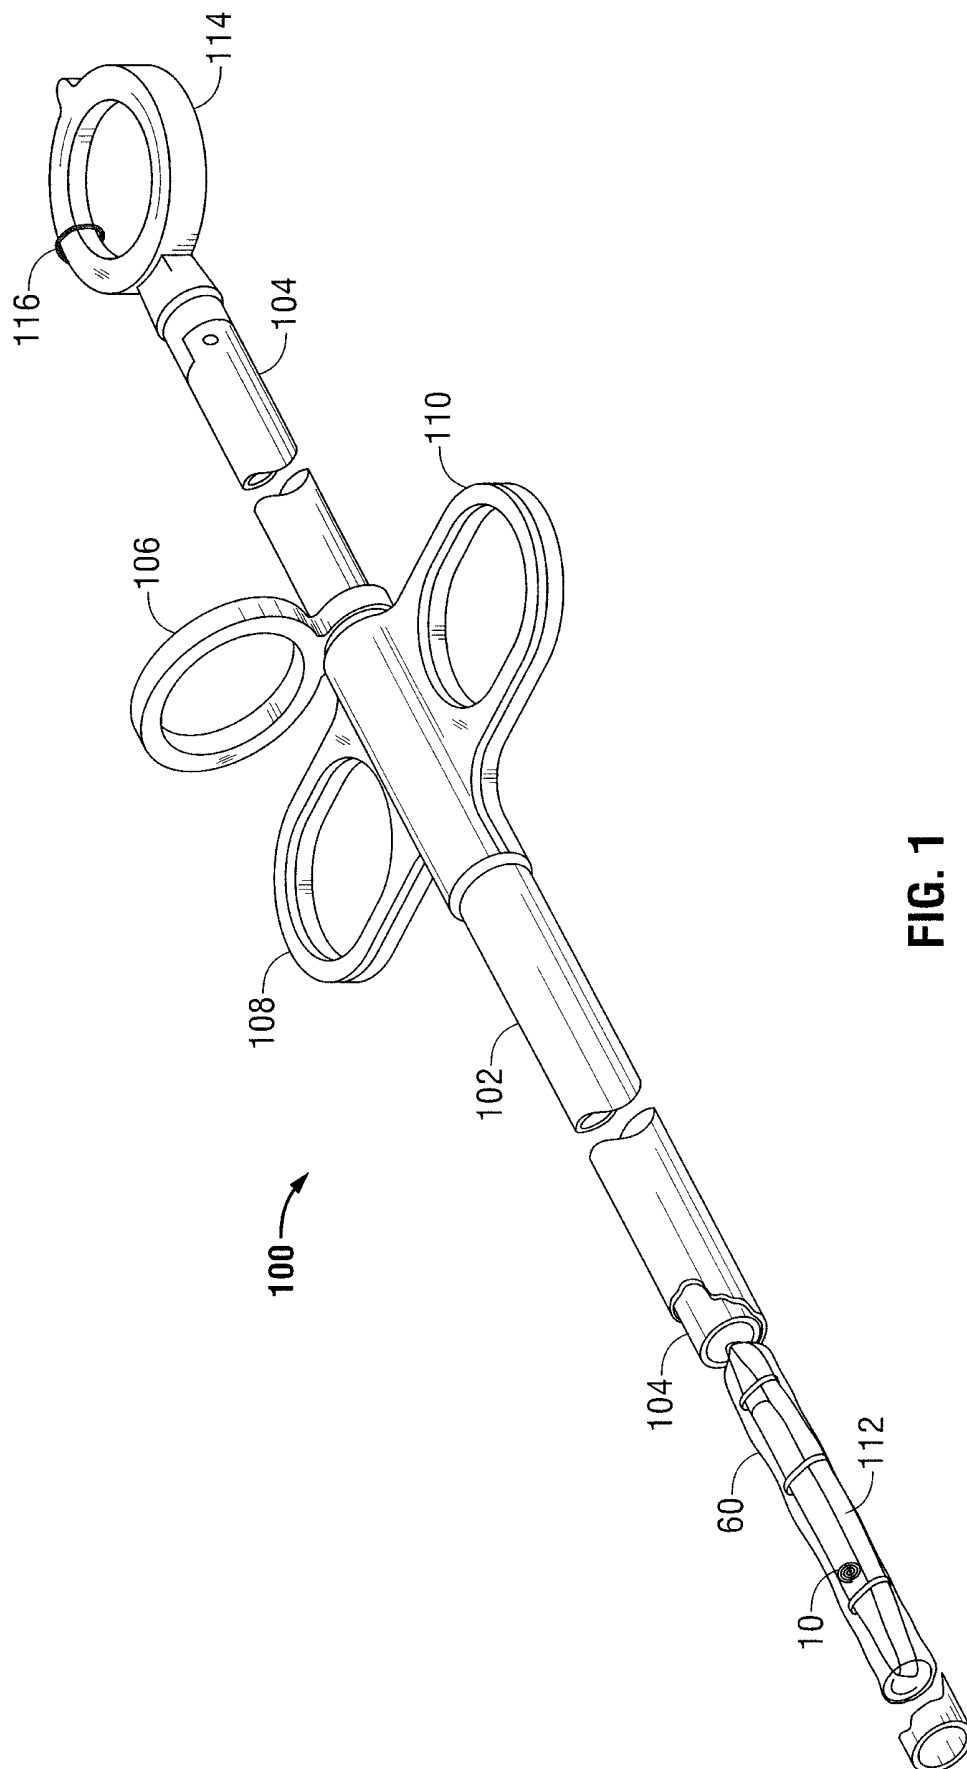


FIG. 1

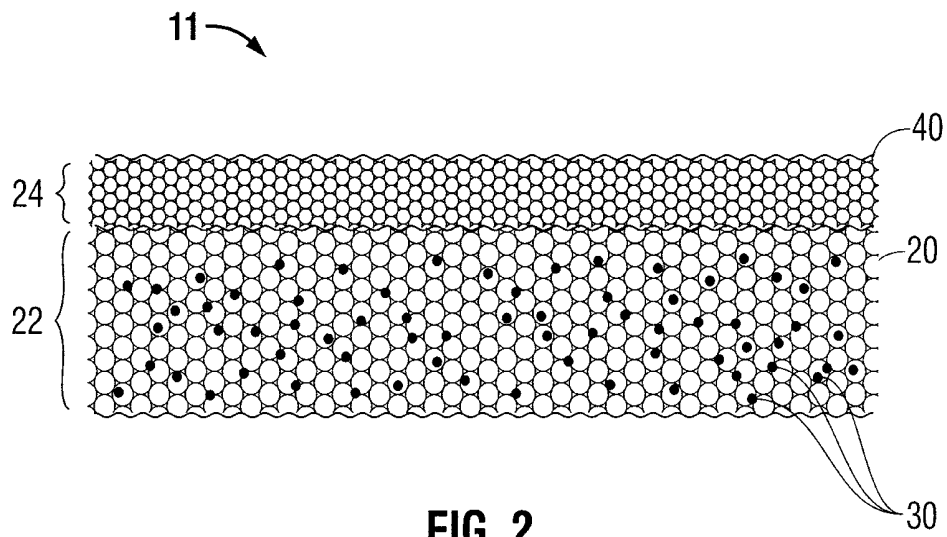


FIG. 2

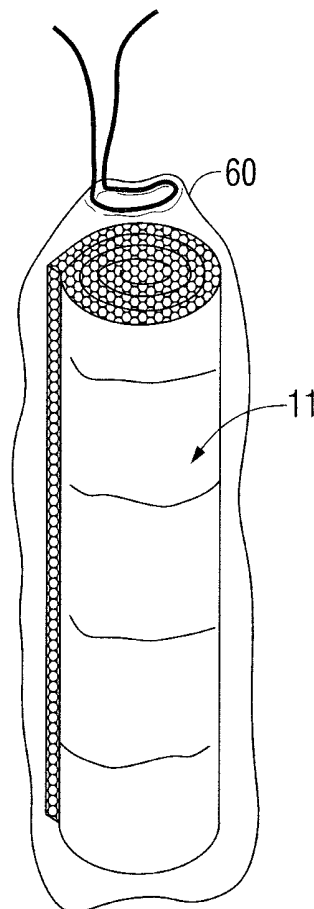


FIG. 3

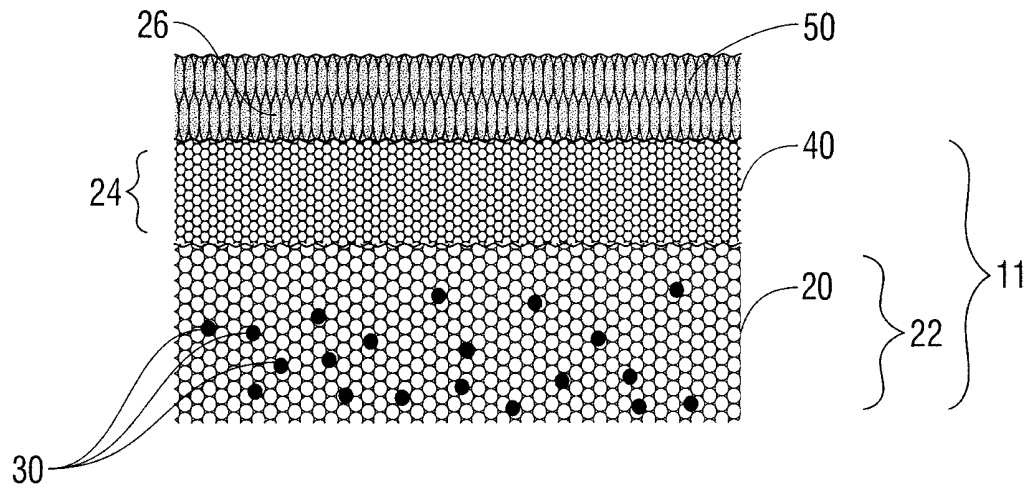


FIG. 4A

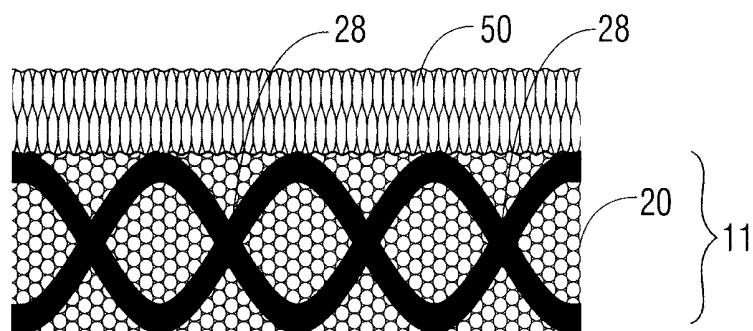


FIG. 4B

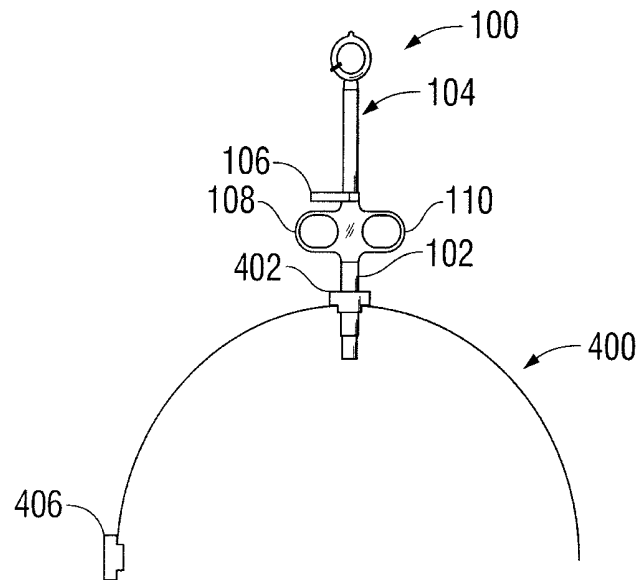


FIG. 5A

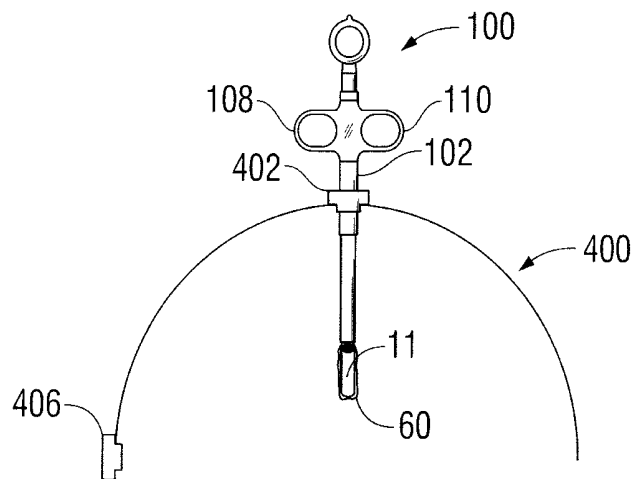


FIG. 5B

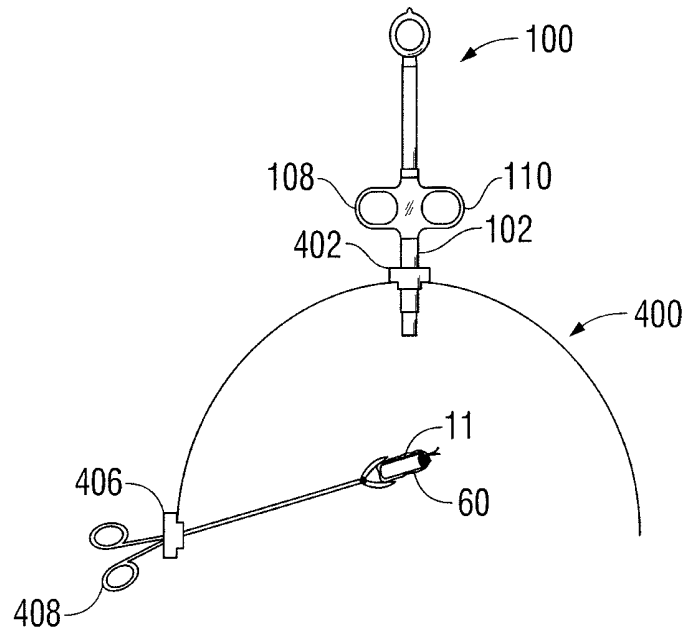


FIG. 5C

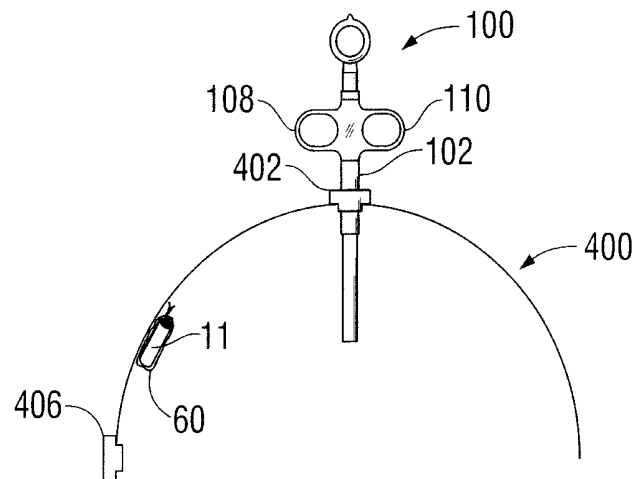


FIG. 5D

1

SYSTEM AND METHOD OF LAPAROSCOPIC USE OF HEMOSTATIC PATCH

CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a divisional of U.S. patent application Ser. No. 12/791,534 filed Jun. 1, 2010, which claims benefit of and priority to U.S. Provisional Application No. 61/229,333 filed Jul. 29, 2009, and the disclosures of each of the above-identified applications are hereby incorporated by reference in their entirety.

BACKGROUND

Technical Field

The present disclosure relates to apparatus and methods for the application of a surgical patch. More particularly, the present disclosure relates to systems and methods for the in situ application of a surgical patch during minimally invasive surgery.

Background

Surgical patches, such as hemostatic patches, are used in repair of defective tissues or organs to establish hemostasis. Hemostatic patches can be used as a supplement to or in conjunction with sutures, staples, or other medical attachment or fastening devices. Hemostatic patches can be used to provide hemostasis to the tissue or organ in need of treatment.

Self-affixing surgical patches are useful for application during open surgery where the surgical patch is applied in the form, i.e., shape, in which it is packaged. However, certain types of absorbable medical devices may be moisture sensitive, that is, they will prematurely react if exposed to moisture in the atmosphere or in the body. Therefore, an apparatus and method of transporting these patches without exposure to ambient or interstitial moisture is needed.

SUMMARY

The present disclosure is directed to the application of a surgical patch during minimally invasive surgery. The method includes laparoscopically transferring a polymeric bag containing a surgical patch into a body cavity followed by removing said surgical patch from the polymeric bag within the body cavity, and applying said surgical patch to a site in the body cavity in need of hemostasis. The method may also include the step of providing a hemostatic patch. The hemostatic patch may include a substrate having a first hydrogel precursor applied to a first portion of the substrate; and a second hydrogel precursor applied to a second portion of the substrate. The method may also include the step of providing a polymeric bag comprising a material selected from polyurethane and latex.

In another embodiment the surgical patch is transferred to a polymeric bag. The polymeric bag containing the surgical patch is then laparoscopically transferred into a body cavity. This embodiment may further include providing a hemostatic patch. The hemostatic patch may include a substrate having a first hydrogel precursor applied to a first portion of the substrate; and a second hydrogel precursor applied to a second portion of the substrate. The polymeric bag may include a material selected from polyurethane and latex.

The present disclosure further includes an apparatus for transferring an item into a body cavity during laparoscopic

2

surgery. The apparatus may include a surgical patch in a polymeric bag sized and dimensioned to be received within a deployment device.

The present disclosure is also directed to an apparatus for performing a surgical procedure. The apparatus includes: an elongated tube; a drive rod; a spring; and a surgical patch received with a polymeric bag. The drive rod, spring, and surgical patch are slidably housed within the elongated tube. The distal end of the drive rod may be connected to the spring. The proximal end of the drive rod may include a handle.

BRIEF DESCRIPTION OF THE DRAWINGS

The foregoing objects and advantages of the disclosure will become more apparent from the reading of the following description in connection with the accompanying drawings, in which:

FIG. 1 is a perspective view of a laparoscopic deployment device, shown in a non-deployed condition, in accordance with the present disclosure;

FIG. 2 is an illustration of a hemostatic patch in accordance with the present disclosure;

FIG. 3 is an illustration of a hemostatic patch retained within a polymeric bag in accordance with the present disclosure;

FIGS. 4A-4B are a schematic illustration of the effect of fluid on the hemostatic patch in situ in accordance with the present disclosure; and

FIGS. 5A-5D are schematic illustrations of the use of the laparoscopic deployment device of FIG. 1 deploying the hemostatic patch retained within a bag of FIG. 2 in accordance with the present disclosure.

DETAILED DESCRIPTION

The present disclosure relates to devices, systems and methods for minimally invasive surgeries such as, endoscopic, laparoscopic, arthroscopic, endoluminal and/or transluminal placement of a surgical patch at a surgical site. As used herein the term "surgical patch" is used to refer to any type of patch for use in surgical procedures, such as, for example, patches that react in situ and those that react upon exposure to moisture. As used herein the term "laparoscopic deployment device" is used to refer to a deployment device that may be used during minimally invasive surgeries described above.

In the drawings and in the description that follows, the term "proximal," as is traditional, will refer to an end of a device that is closer to the user, while the term "distal" will refer to the end of the device that is further from the user.

Laparoscopic surgical procedures are minimally invasive procedures which are carried out within the body cavity through use of access ports in conjuncture with elongated surgical devices. An initial opening in the body tissue enables passage of the endoscopic or laparoscopic device to the interior of the body. Openings include natural passageways of the body or openings which are created by a tissue piercing device such as a trocar. During laparoscopic procedures, narrow punctures or incisions are made minimizing trauma to the body cavity and reducing patient recovery time.

Referring now in specific detail to the drawings, in which like numbers identify similar or identical elements, FIG. 1 illustrates a laparoscopic deployment/collection device and is generally designated as **100**. The deployment device **100** includes an elongated tube **102**, which is of such dimensions

and/or diameter to be insertable through an access device, such as a trocar cannula, for endoscopic or laparoscopic procedures. The tube **102** is generally between about 0.25 inches to 0.50 inches in diameter, and about 10 inches to about 15 inches long, although other dimensions may also be used if appropriate. Tube **102** slidably houses a drive rod **104** and, when undeployed, a polymeric bag **60**, containing a surgical patch **10**.

The laparoscopic deployment device **100** includes a drive rod or bar **104** that is an elongated generally cylindrical member slidably disposed through the bore of tube **102**. A distal end of the drive rod **104** is attached to the bag **60** to move the bag **60** from a non-deployed position contained within the outer tube **102** to a deployed position distal to the outer tube **102**.

A locking tab **106** may be included to prevent premature actuation of the device. The locking tab **106** includes snap fit engagement structure to engage a slot of the drive rod **104**. When thus engaged, the drive rod **104** cannot be pushed distally beyond the point where the locking tab **106** engages the proximal end of handle portions **108**, **110**.

In addition, the laparoscopic deployment device **100** may include a finger loop **114** for engagement by a user's finger. One end of a drawstring **116** is attached to the finger loop **114** while an opposing end of the drawstring **116** is attached to the bag **60**. In an initial, unused condition, bag **60** will be rolled up (or otherwise folded) and contain a spring **112** and surgical patch **10** in a relatively straight position within tube **102**. When the drive rod **104** is advanced, the spring **112** connected thereto will exit a distal end of tube **102** and resiliently open, thereby deploying and opening the bag **60** to allow access to the surgical patch **10**. In some embodiments the bag **60** will remain closed following deployment. Tube **102** is preferably formed from a metal such as stainless steel and is preferably coated with a shrink-wrap plastic such as shrinkable polyethylene fiberglass, or polyvinyl chloride of a grade suitable for use in surgical procedures.

Such devices are known in the art and include, for example, the devices disclosed in U.S. Patent Application Publication No. 2006/0229640, filed Mar. 29, 2005; U.S. Patent Application Publication No. U.S. 2006/0200170, filed Mar. 7, 2005; and U.S. Patent Application Publication No. 2006/0200169, filed Mar. 7, 2005, the entire contents of which are incorporated by reference herein.

FIG. 2 illustrates one embodiment of a surgical patch, according to the present disclosure. A hemostatic patch **11** is used with laparoscopic deployment device **100**. The hemostatic patch **11** includes a porous substrate **20** having a first hydrogel precursor **30** applied to a first portion **22** of the porous substrate and a second hydrogel precursor **40** applied to a second portion **24** of the porous substrate. Such a hemostatic patch **11** is disclosed in U.S. Provisional Patent Application No. 61/196,543, filed Oct. 17, 2008, the entire contents of which are incorporated by reference herein.

During use, the hemostatic patch **11** is oriented with the portion **24** to which the second hydrogel precursor **40** is applied being closer to the tissue and the portion **22** having the first hydrogel precursor **30** applied thereto further from the tissue. In embodiments, the first and second portions **22**, **24** may be distinguishable from one another by the addition of contrast dyes, surface texturing, coloring or other visual cues. Upon contact with tissue, such as, for example, injured tissue, the hemostatic patch **11** will soak up physiological fluid and the second hydrogel precursor **40** may be dissolved by the fluid. As the fluid wicks into and migrates across the hemostatic patch **11**, it will carry the dissolved second hydrogel precursor **40** along through the hemostatic patch

11. Eventually, the fluid will migrate through the hemostatic patch **11** sufficiently to reach the portion **22** to which the first hydrogel precursor **30** is applied, thereby contacting the first hydrogel precursor **30**. The first and second hydrogel precursors **30**, **40** will then react to form a biocompatible cross-linked material, thereby creating hemostasis at the injury site. In some embodiments, the biocompatible cross-linked material produced by reaction of the first and second hydrogel precursors **30**, **40** not only provide hemostatic properties but also provide a portion of the hemostatic patch **11** with anti-adhesive properties.

The porous substrate **20** of the hemostatic patch **11** has openings or pores over at least a portion of a surface thereof. The pores may be formed in the substrate either before or after implantation. As described in more detail below, suitable materials for forming the porous substrate **20** include, but are not limited to fibrous structures (e.g., knitted structures, woven structures, non-woven structures, etc.) and/or foams (e.g., open or closed cell foams). In embodiments, the pores may be in sufficient number and size so as to interconnect across the entire thickness of the porous substrate **20**. Woven fabrics, knitted fabrics and open cell foam are illustrative examples of structures in which the pores can be in sufficient number and size so as to interconnect across the entire thickness of the porous substrate **20**. In embodiments, the pores do not interconnect across the entire thickness of the porous substrate **20**. Closed cell foam or fused non-woven materials are illustrative examples of structures in which the pores may not interconnect across the entire thickness of the porous substrate **20**. The pores of the foam porous substrate **20** may span across the entire thickness of porous substrate **20**. In yet other embodiments, the pores do not extend across the entire thickness of the porous substrate **20**, but rather are present at a portion of the thickness thereof. In embodiments, the openings or pores are located on a portion of the surface of the porous substrate **20**, with other portions of the porous substrate **20** having a non-porous texture. In other embodiments, the pores may be formed after implantation in situ. The in situ pore formation may be performed using any suitable method. Some non-limiting examples include the use of contact lithography, living radical photopolymer (LRPP) systems and salt leaching. Those skilled in the art reading the present disclosure will envision other pore distribution patterns and configurations for the porous substrate **20**.

Where the porous substrate **20** is fibrous, the fibers may be filaments or threads suitable for knitting or weaving or may be staple fibers, such as those frequently used for preparing non-woven materials. The fibers may be made from any biocompatible material. Thus, the fibers may be formed from a natural material or a synthetic material. The material from which the fibers are formed may be bioabsorbable or non-bioabsorbable. It should be understood that any combination of natural, synthetic, bioabsorbable and non-bioabsorbable materials may be used to form the fibers. Some non-limiting examples of materials from which the fibers may be made include, but are not limited to polyesters such as poly(lactic acid) and poly(glycolic acid) poly(trimethylene carbonate), poly(dioxanone), poly(hydroxybutyrate), poly(phosphazene), polyethylene terephthalate, ultra-high molecular weight polyethylene, polyethylene glycols, polyethylene oxides, polyacrylamides, polyhydroxyethylmethacrylate (pHEMA), polyvinylpyrrolidone, polyvinyl alcohols, polyacrylic acid, polyacetate, polycaprolactone, polypropylene, aliphatic polyesters, glycerols, poly(amino acids), copoly(ether-esters), polyalkylene oxalates, poly(saccharides), polyamides, poly(iminocar-

bonates), polyalkylene oxalates, polyoxaesters, polyorthoesters, polyphosphazenes, biopolymers, polymer drugs and copolymers, block copolymers, homopolymers, blends and combinations thereof.

Where the porous substrate **20** is fibrous, the porous substrate **20** may be formed using any method suitable to forming fibrous structures, including but not limited to knitting, weaving, non-woven techniques, wet-spinning, electro-spinning, extrusion, co-extrusion, and the like. Suitable techniques for making fibrous structures are within the purview of those skilled in the art. In embodiments, the textile has a three dimensional structure, such as the textiles described in U.S. Pat. Nos. 7,021,086 and 6,443,964, the contents of which are incorporated by reference herein.

In some embodiments, the porous substrate **20** is made from fibers of oxidized cellulose. Such materials are known and include oxidized cellulose hemostat materials commercially available under the trade name SURGICEL®. Methods for preparing oxidized cellulose hemostat materials are known to those skilled in the art and are disclosed, for example in U.S. Pat. Nos. 3,364,200; 4,626,253; 5,484,913; and 6,500,777, the disclosures of which are incorporated herein by this reference in their entirety.

Where the porous substrate **20** is a foam, the porous substrate **20** may be formed using any method suitable to forming a foam or sponge including, but not limited to the lyophilization or freeze-drying of a composition. The foam may be cross-linked or non-cross-linked, and may include covalent or ionic bonds. Suitable techniques for making foams are within the purview of those skilled in the art.

As mentioned above, the porous substrate **20** has a first and second hydrogel precursor **30, 40** applied thereto. The terms “first hydrogel precursor” and “second hydrogel precursor” each mean a polymer, functional polymer, macromolecule, small molecule, or crosslinker that can take part in a reaction to form a network of crosslinked molecules, e.g., a hydrogel.

In embodiments, each of the first and second hydrogel precursors **20, 30**, includes only one category of functional groups, either only nucleophilic groups or only electrophilic functional groups, so long as both nucleophilic and electrophilic precursors are used in the crosslinking reaction. Thus, for example, if the first hydrogel precursor **30** has nucleophilic functional groups such as amines, the second hydrogel precursor **40** may have electrophilic functional groups such as N-hydroxysuccinimides. On the other hand, if first hydrogel precursor **30** has electrophilic functional groups such as sulfosuccinimides, then the second hydrogel precursor **40** may have nucleophilic functional groups such as amines or thiols. Thus, functional polymers such as proteins, poly(allyl amine), styrene sulfonic acid, or amine-terminated di- or multifunctional poly(ethylene glycol) (“PEG”) can be used.

The first and second hydrogel precursors **30, 40** may have biologically inert and water soluble cores. When the core is a polymeric region that is water soluble, preferred polymers that may be used include: polyether, for example, polyalkylene oxides such as polyethylene glycol (“PEG”), polyethylene oxide (“PEO”), polyethylene oxide-co-polypropylene oxide (“PPO”), co-polyethylene oxide block or random copolymers, and polyvinyl alcohol (“PVA”); poly(vinyl pyrrolidone) (“PVP”); poly(amino acids); poly(saccharides), such as dextran, chitosan, alginates, carboxymethylcellulose, oxidized cellulose, hydroxyethylcellulose, hydroxyethylcellulose, hyaluronic acid, and proteins such as albumin, collagen, casein, and gelatin. The polyethers and more particularly poly(oxyalkylenes) or poly(ethylene glycol) or polyethylene glycol are especially useful. When the core is

small molecular in nature, any of a variety of hydrophilic functionalities can be used to make the first and second hydrogel precursors **30, 40** water soluble. For example, functional groups like hydroxyl, amine, sulfonate and carboxylate, which are water soluble, maybe used to make the precursor water soluble. In addition, N-hydroxysuccinimide (“NHS”) ester of subaric acid is insoluble in water, but by adding a sulfonate group to the succinimide ring, the NHS ester of subaric acid may be made water soluble, without affecting its reactivity towards amine groups.

The first and second hydrogel precursors **30, 40** may be applied to the porous substrate **20** using any suitable method known to those skilled in the art. For example, the first and second hydrogel precursors **30, 40**, may be incorporated into the porous substrate **20** prior to forming the porous substrate **20**. In another non-limiting example, the first or second hydrogel precursors **30, 40** may be positioned in the pores of the porous substrate **20** or onto a surface of the porous substrate **20** following formation of the substrate. In additional embodiments, the porous substrate **20** may be calendared prior to application of the first hydrogel precursor **30** thereby allowing the first or second hydrogel precursors **30, 40** to penetrate into openings on the substrate which were created by the calendaring process.

In other embodiments, the first or second hydrogel precursors **30, 40** may be in the form of a coating which is applied to the substrate in any concentration, dimension and configuration capable of forming the hemostatic patch **11**. The coating may form a non-porous layer or a porous layer. In embodiments, at least one of the first and second hydrogel precursors **30, 40** is a cross-linker. In embodiments, at least one of the first and second hydrogel precursors **30, 40** is a macromolecule, and is referred to as a “functional polymer”.

Each of the first and second hydrogel precursors **30, 40** is multifunctional, meaning that it comprises two or more electrophilic or nucleophilic functional groups, such that, for example, a nucleophilic functional group on the first hydrogel precursor **30** may react with an electrophilic functional group on the second hydrogel precursor **40** to form a covalent bond. At least one of the first or second hydrogel precursors **30, 40** includes more than two functional groups, so that, as a result of electrophilic-nucleophilic reactions, the precursors combine to form cross-linked polymeric products.

In embodiments, a multifunctional nucleophilic polymer such as tryllysine may be used as a first hydrogel precursor **30** and a multifunctional electrophilic polymer such as a multi-arm PEG functionalized with multiple NHS groups may be used as a second hydrogel precursor **40**. The multi-arm PEG functionalized with multiple NHS groups can for example have four, six or eight arms and have a molecular weight of from about 5,000 to about 25,000. Many other examples of suitable first and second hydrogel precursors **30, 40** are described in U.S. Pat. Nos. 6,152,943; 6,165,201; 6,179,862; 6,514,534; 6,566,406; 6,605,294; 6,673,093; 6,703,047; 6,818,018; 7,009,034; and 7,347,850, the entire content of each of which is incorporated herein by reference.

While the present disclosure may involve a hemostatic patch, any surgical patch may be used in the method disclosed herein. The hemostatic patch may be any size and dimension capable of transport in the laparoscopic deployment device of the disclosure. In one embodiment, the hemostatic patch is about 2 inches square, although it is envisioned that the patch may be of varying shapes and sizes. Additionally, while the substrate used in forming the patch is described as “porous” the substrate may be porous or non-porous in various embodiments.

Upon application to a site of bleeding tissue, the hemostatic patch may affect hemostasis of said tissue. As used herein, the term “hemostasis” means the arrest of bleeding. It is believed, without being limited thereto, that the hemostatic effect of the hemostatic patch is due to both intrinsic and extrinsic factors. In some embodiments, the substrate may be comprised of a hemostatic agent providing an intrinsic hemostatic effect. In embodiments, the cross-linking between the hydrogel precursors creates a physical barrier to blood flow providing an extrinsic hemostatic effect. Hemostasis may occur, at the site of application of the hemostatic patch, within less than about 2 minutes. As stated above, upon contact with tissue, such as, for example, injured or bleeding tissue, the hemostatic patch **11** soaks up interstitial and physiological fluid (e.g., blood, lymph-fluid, etc.) and the first and second hydrogel precursors **30**, **40** are mixed by the fluid. In order to prevent the hemostatic patch **11** from taking up fluid prior to use at the location in need of hemostasis, the hemostatic patch **11** is retained or sealed in packaging until the time it is needed for its application.

As shown in FIG. 3, to provide for moisture resistant transport of the hemostatic patch **11** during laparoscopic surgery, the hemostatic patch **11** is enclosed in a polymeric bag **60**, which is moisture resistant. The term “moisture” as used herein means physiological fluids and humidity. As used herein, the term “sterile” means that the bag is free from living organisms such as microorganisms in addition to endotoxins, viruses, and the like. The bag **60** may be formed of material that resists moisture/humidity. Exemplary materials which may be used in accordance with the present disclosure include, for example, a substantially transparent polymeric material such as a polyurethane sheet or latex. In embodiments, the bag **60** may include a metallized layer disposed on a plastic film backing in order to reduce the incidence and degree of porosity thereof. In one embodiment, the bag **60** is formed from aromatic polyester type thermoplastic polyurethane such as Dureflex®, a product of Deerfield Urethane, Inc., located in Whately, Mass. In some embodiments, the bag **60** is transparent to permit viewing of the hemostatic patch **11**. The thickness of the bag **60** can be from about 0.001 to about 0.005 inches although other thicknesses are also envisioned. The bag **60** should also be impervious to penetration by disease-causing cells, such as cancer cells. The bag **60** may be of any dimension suitable to enclose the hemostatic patch **11**, and prevent the hemostatic patch from contacting moisture. The bag **60** may be folded or rolled to a size sufficient to be inserted into the laparoscopic deployment device **100**. In some embodiments, the bag **60** may have a diameter from about 1.5 inches to about 6.0 inches, a depth of from about 2 inches to about 10 inches, and a cubic capacity of up to about 2.0 liters of water. In some embodiments, the bag **60** is an Endobag™ manufactured by Covidien AG, Mansfield, Mass. As seen in FIG. 3, hemostatic patch **11** may be rolled or folded for placement within bag **60**. In some embodiments, when folded or rolled, the hemostatic patch **11**, in the bag **60**, is preferably less than about 0.50 inches in diameter. In another embodiment, the rolled or folded hemostatic patch **11**, in the bag **60**, is less than about 0.25 inches in diameter.

The polymeric bag **60** may be sealed in such a manner as to protect the hemostatic patch **11** from exposure to moisture during and after deployment thereof from a laparoscopic device **100**. In embodiments, the bag **60** may be open following deployment from the device.

The hemostatic patch **11**, in the sterile polymeric bag **60**, may be transferred to a body cavity during laparoscopic surgery utilizing laparoscopic deployment device **100**. As

seen in FIGS. 4A-4B, during use, the hemostatic patch **11** is oriented with second portion **24**, to which the second hydrogel precursor **40** is applied, being closer to tissue **50** and with the first portion **22**, to which the first hydrogel precursor **30** is applied, being disposed further from the tissue **50**. Upon contact with tissue **50**, such as, for example, injured or bleeding tissue, hemostatic patch **11**, soaks up physiological fluid or blood **26** and the second portion **24**, having the second hydrogel precursor **40**, is dissolved by the fluid or blood **26**. As the fluid or blood **26** wicks into and migrates across the hemostatic patch **11**, the fluid or blood carries the dissolved second hydrogel precursor **40** along through the hemostatic patch **11** sufficiently to reach the first portion **22** to which the first hydrogel precursor **30** is applied, thereby initiating the cross-linking reaction between the first and second hydrogel precursors **30**, **40**. At this point, as seen in FIG. 4B, first and second hydrogel precursors **30**, **40**, then react to form a biocompatible cross-linked material **28** thereby assisting with the hemostasis of the tissue **50**.

In one embodiment, the laparoscopic deployment device **100** may contain the hemostatic patch **11** encased in the polymeric bag **60** for delivery during a single use of the laparoscopic deployment device. In another embodiment, a hemostatic patch **11**, encased in the polymeric bag **60**, may be provided for insertion into a laparoscopic deployment device **100**.

According to another method of use, as shown in FIGS. 5A-5C, a laparoscopic deployment device **100** is shown inserted into a body cavity **400** through a trocar **402** and additional trocar **406** is inserted in the side of the body cavity **400**, for later use. As shown in FIGS. 5A-5B, locking tab **106** is removed and drive rod **104** is pushed to the proximal end of handle portions **108**, **110**. As seen in FIG. 5B, the hemostatic patch **11**, encased in the polymeric bag **60** is deployed through the laparoscopic deployment device **100** into the body cavity **400**. At this point, as seen in FIG. 5C, the encased hemostatic patch **11** can then be removed from laparoscopic deployment device **100** using pinchers **408** through trocar **406** and held to the side of the body cavity **400** as shown in FIG. 5D, until needed. At the point in time of the procedure/operation, when the hemostatic patch **11** is needed, various laparoscopic tools known to those skilled in the art can be utilized to remove the hemostatic patch **11** from the polymeric bag **60** and place the hemostatic patch **11** in the location it is needed or desired, e.g., the injured or bleeding tissue.

While the above description contains many specifics, these specifics should not be construed as limitations on the scope of the present disclosure, but merely as exemplifications of preferred embodiments thereof. Those skilled in the art will envision many other possible variations that are within the scope and spirit of the present disclosure.

What is claimed is:

1. An apparatus for delivering a surgical patch into a body cavity during laparoscopic surgery, the apparatus comprising:

a surgical patch including a first hydrogel precursor and a second hydrogel precursor on the first hydrogel precursor, the first hydrogel precursor including one of nucleophilic functional groups or electrophilic functional groups, and the second hydrogel precursor including the other of the nucleophilic functional groups or the electrophilic functional groups, the first and second hydrogel precursors configured to react with one another to form a biocompatible cross-linked material; and
a polymeric bag,

9

the surgical patch disposed in the polymeric bag, the surgical patch and polymeric bag configured to be received within a deployment device for delivering the surgical patch and the polymeric bag into a body cavity.

2. The apparatus according to claim 1, wherein the polymeric bag and the surgical patch are configured to be delivered together into the body cavity.

3. The apparatus according to claim 2, wherein the surgical patch is selectively removable from the polymeric bag while the surgical patch and the polymeric bag are within the body cavity.

4. The apparatus according to claim 1, wherein the surgical patch is configured to wick fluid for migration across the surgical patch to enable the first and second hydrogel precursors to react with one another.

5. The apparatus according to claim 1, wherein the surgical patch is sealed inside the polymeric bag.

6. A system for performing a surgical procedure, the system comprising:

a polymeric bag;

a surgical patch within the polymeric bag, the surgical patch including a first hydrogel precursor and a second hydrogel precursor on the first hydrogel precursor, the first hydrogel precursor including one of nucleophilic functional groups or electrophilic functional groups, and the second hydrogel precursor including the other of the nucleophilic functional groups or the electrophilic functional groups, the first and second hydrogel precursors configured to react with one another to form a biocompatible cross-linked material; and

a deployment device including:

an elongated tube; and

a drive rod supported within the elongated tube and slidable to advance the polymeric bag and surgical

10

patch along the elongated tube to dispense the polymeric bag and surgical patch from the elongated tube.

7. The system according to claim 6, wherein the drive rod is connected to a spring.

8. The system according to claim 6, wherein the drive rod includes a handle.

9. The system according to claim 6, wherein the surgical patch comprises:

a substrate having the first hydrogel precursor applied to a first portion of the substrate; and

the second hydrogel precursor applied to a second portion of the substrate.

10. The system according to claim 9, wherein the first and second hydrogel precursors are configured to react with one another to form a biocompatible cross-linked material while the surgical patch is positioned in a body cavity.

11. The system according to claim 10, wherein the surgical patch is configured to wick fluid for migration across the surgical patch to enable the first and second hydrogel precursors to react with one another.

12. The system according to claim 6, wherein the surgical patch is sealed inside the polymeric bag.

13. The system according to claim 6, wherein the polymeric bag is constructed, at least in part, from polyurethane.

14. The system according to claim 6, wherein the surgical patch is rolled or folded within the polymeric bag.

15. The system according to claim 9, wherein the substrate is nonporous.

16. The system according to claim 9, wherein the substrate is porous.

* * * * *

专利名称(译)	止血药的腹腔镜使用的系统和方法		
公开(公告)号	US10595978	公开(公告)日	2020-03-24
申请号	US15/423625	申请日	2017-02-03
[标]申请(专利权)人(译)	柯惠有限合伙公司		
申请(专利权)人(译)	COVIDIEN LP		
当前申请(专利权)人(译)	COVIDIEN LP		
[标]发明人	LAVIGNE KEVIN BENNETT STEVEN MAST NATHANIEL		
发明人	LAVIGNE, KEVIN BENNETT, STEVEN MAST, NATHANIEL		
IPC分类号	A61F2/00 A61L27/52 A61L27/34 A61L27/56 A61B17/34 A61B17/00		
CPC分类号	A61F2/0063 A61L27/34 A61L27/52 A61L27/56 A61F2002/0072 A61B17/3468 A61B2017/00287		
优先权	61/229333 2009-07-29 US		
其他公开文献	US20170143464A1		
外部链接	Espacenet		

摘要(译)

本公开包括用于在微创手术期间原位施加手术贴片的系统和方法。该方法包括将手术贴片插入袋中的步骤；将装有止血贴的聚合物袋转移到体腔中；当聚合物袋在体腔内时，从聚合物袋上取下手术贴片；将手术贴片施加到体腔内的组织上。

