


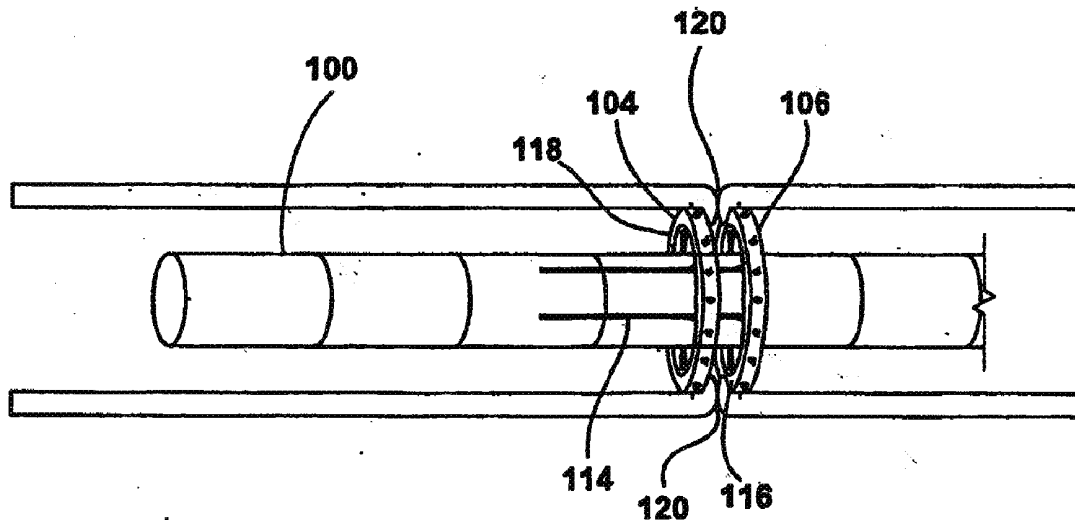

US 20130116712A1

(19) **United States**(12) **Patent Application Publication**
Belson(10) **Pub. No.: US 2013/0116712 A1**(43) **Pub. Date: May 9, 2013**(54) **APPARATUS AND METHOD FOR
ENDOSCOPIC COLECTOMY****Publication Classification**(71) Applicant: **Intuitive Surgical Operations, Inc.**,
Sunnyvale, CA (US)(72) Inventor: **Amir Belson**, Los Altos, CA (US)(73) Assignee: **Intuitive Surgical Operations, Inc.**,
Sunnyvale, CA (US)(21) Appl. No.: **13/729,602**(22) Filed: **Dec. 28, 2012****Related U.S. Application Data**(62) Division of application No. 12/027,739, filed on Feb.
7, 2008, now Pat. No. 8,361,090, which is a division of
application No. 10/327,370, filed on Dec. 20, 2002,
now Pat. No. 7,338,505.(60) Provisional application No. 60/347,674, filed on Jan.
9, 2002.(51) **Int. Cl.**
A61B 17/11 (2006.01)(52) **U.S. Cl.**
CPC **A61B 17/1114** (2013.01)
USPC **606/153**(57) **ABSTRACT**

Apparatus and methods for endoscopic colectomy are described herein. A colectomy device having a first and a second tissue approximation device is mounted on a colonoscope separated from one another. During deployment of the colectomy device, a diseased portion of the colon is positioned inbetween the tissue approximation devices. The tissue approximation devices are radially expanded such that they contact and grasp the colon wall at two sites adjacent to the diseased portion of the colon. The diseased portion is separated from the omentum and is transected using a laparoscope or is drawn into the colonoscope for later removal. The tissue approximation devices are then urged towards one another over the colonoscope to approximate the two free edges of the colon into contact together where they are fastened to one another using the tissue approximation device as a surgical stapler to create an end-to-end anastomosis.



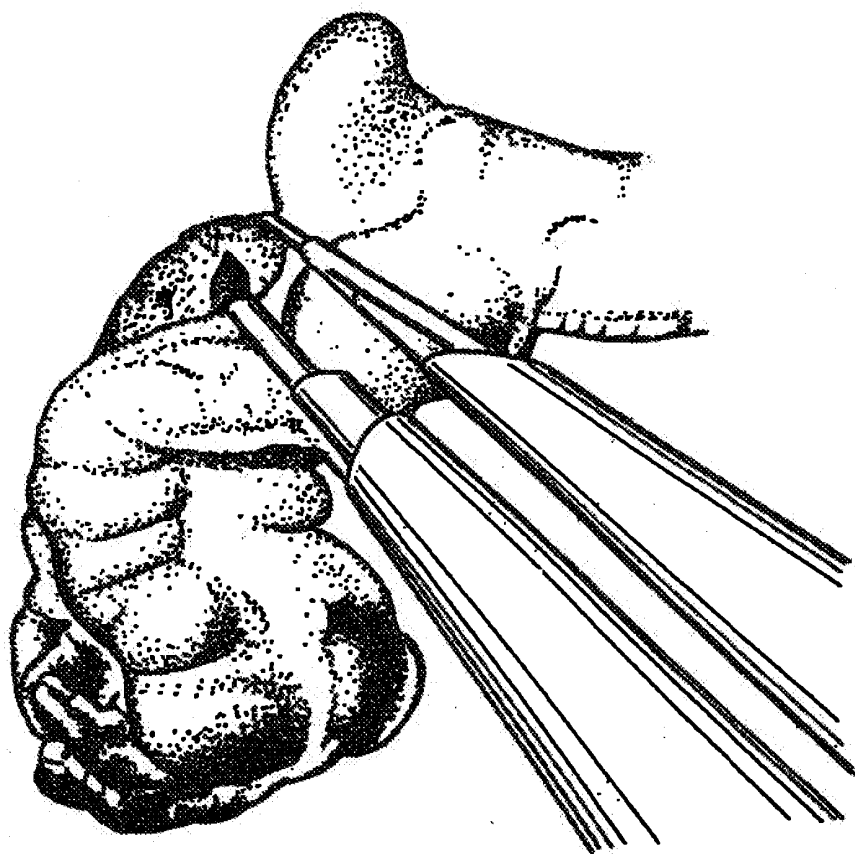


FIG. 1

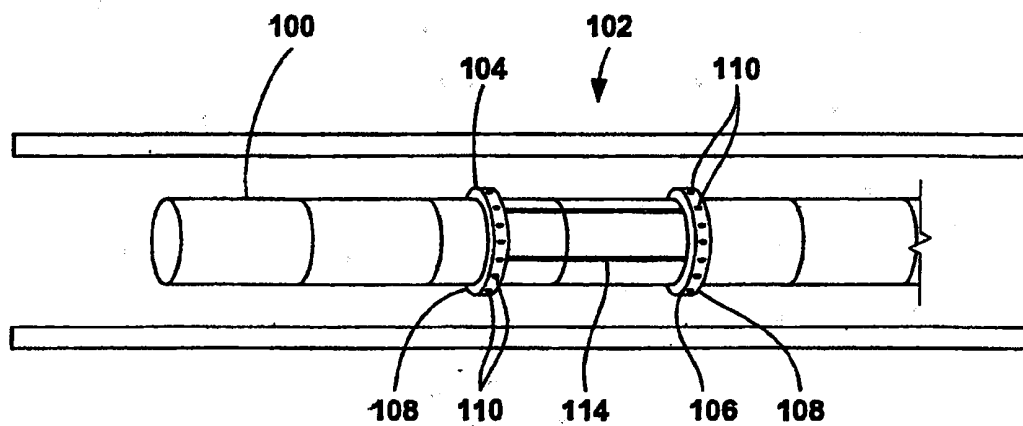


FIG 2

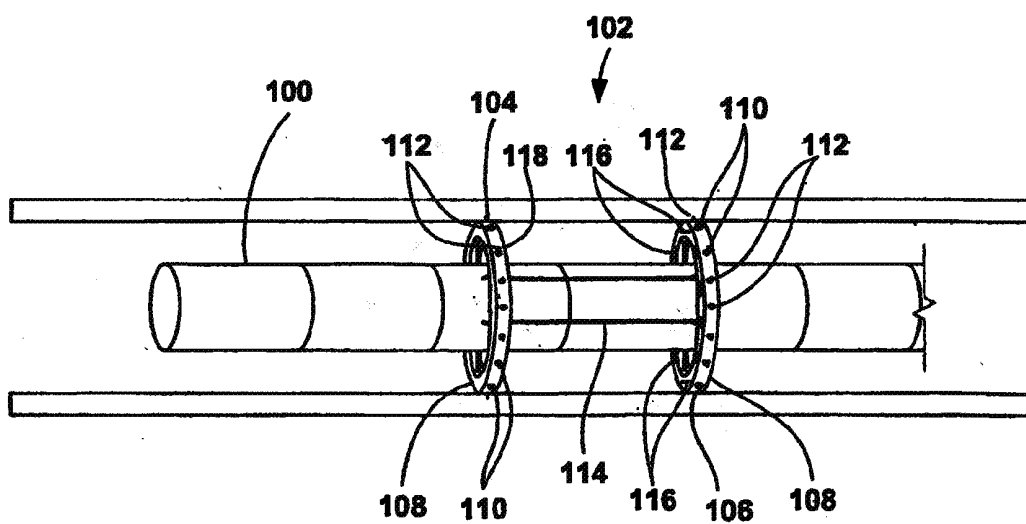


FIG 3

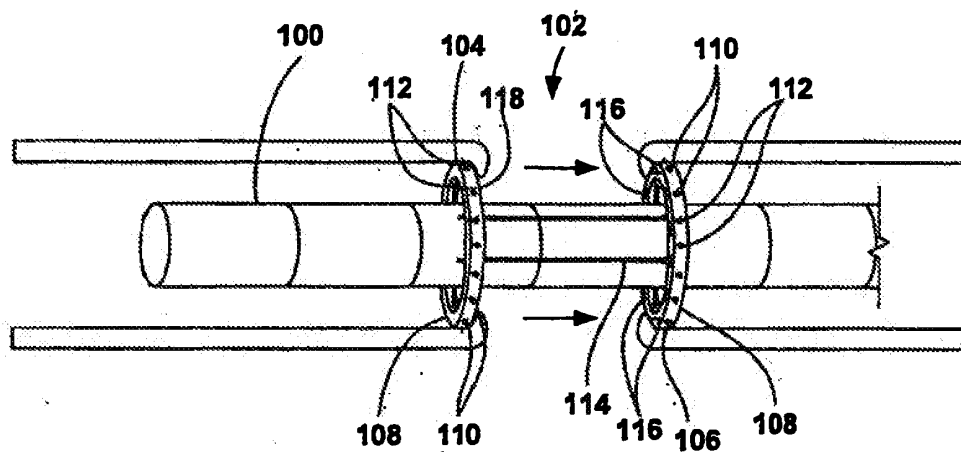


FIG 4

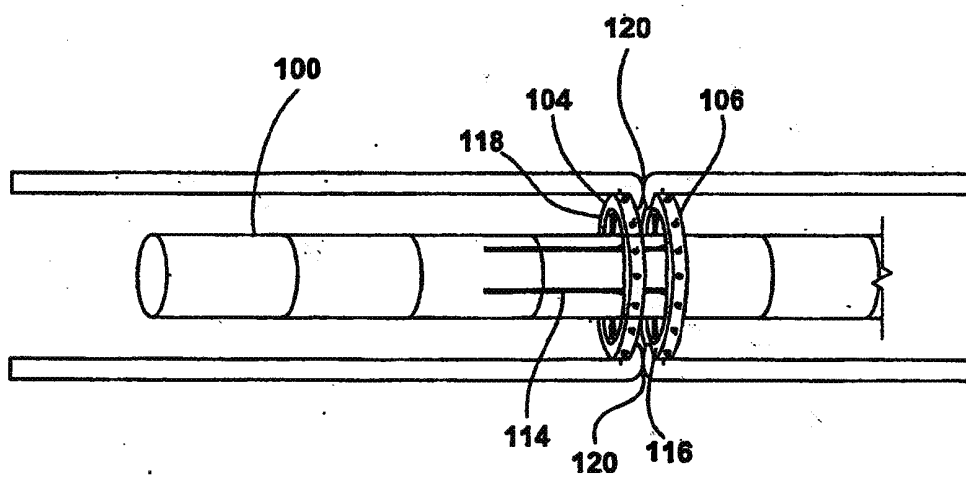


FIG 5

FIG. 6

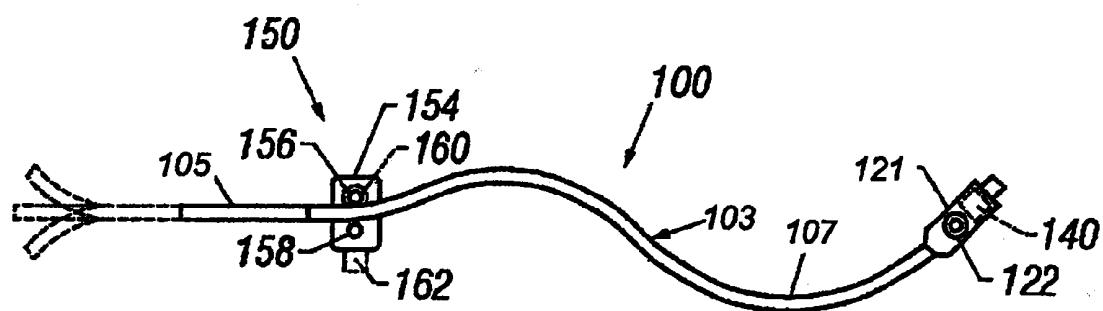


FIG. 7

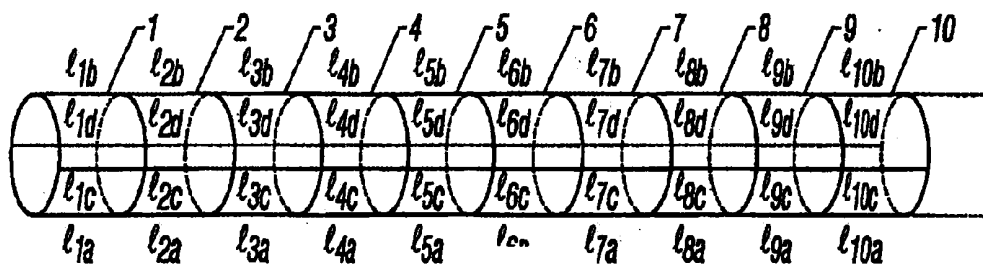


FIG. 8

103

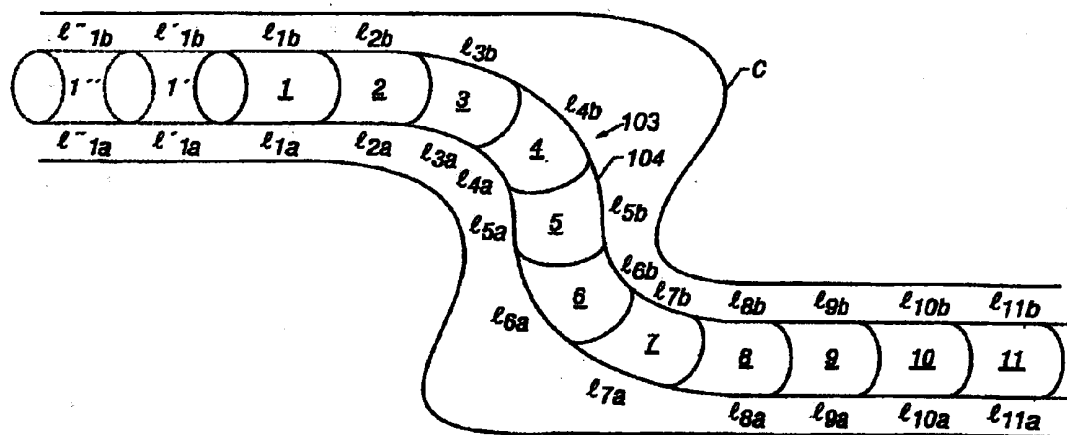


FIG. 9

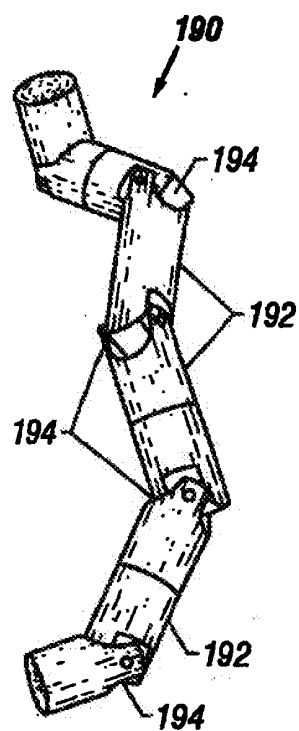


FIG. 10

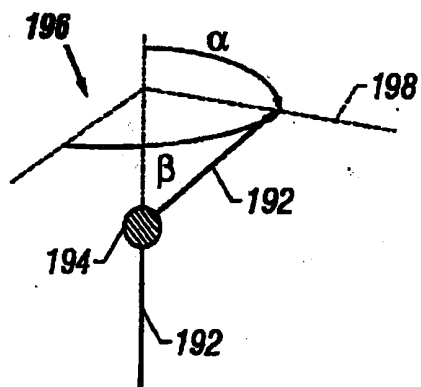


FIG. 11

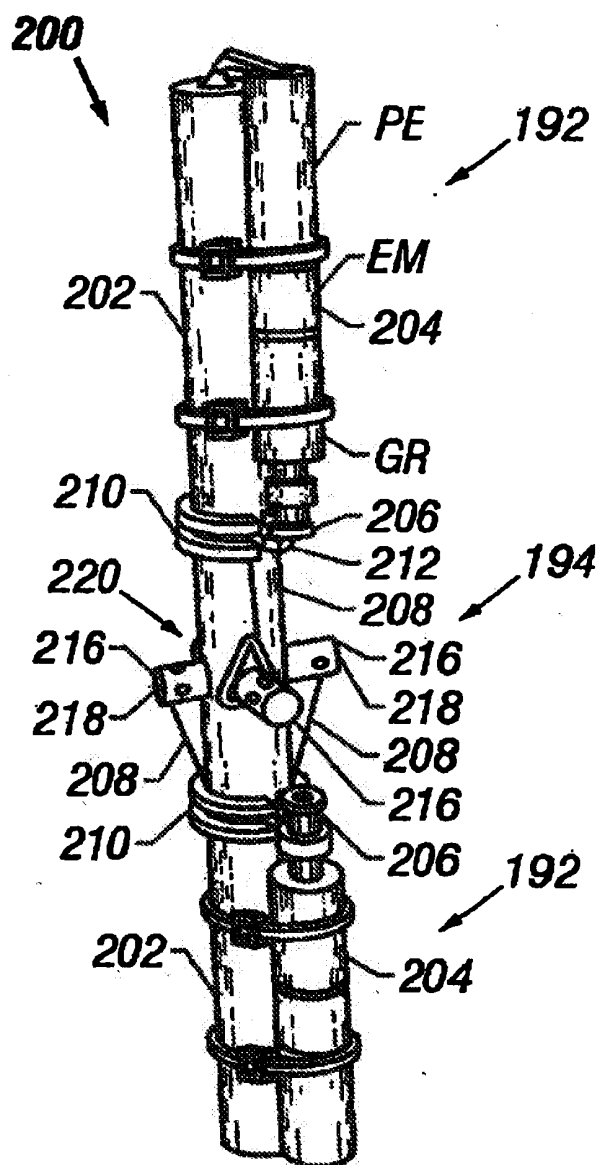


FIG. 12

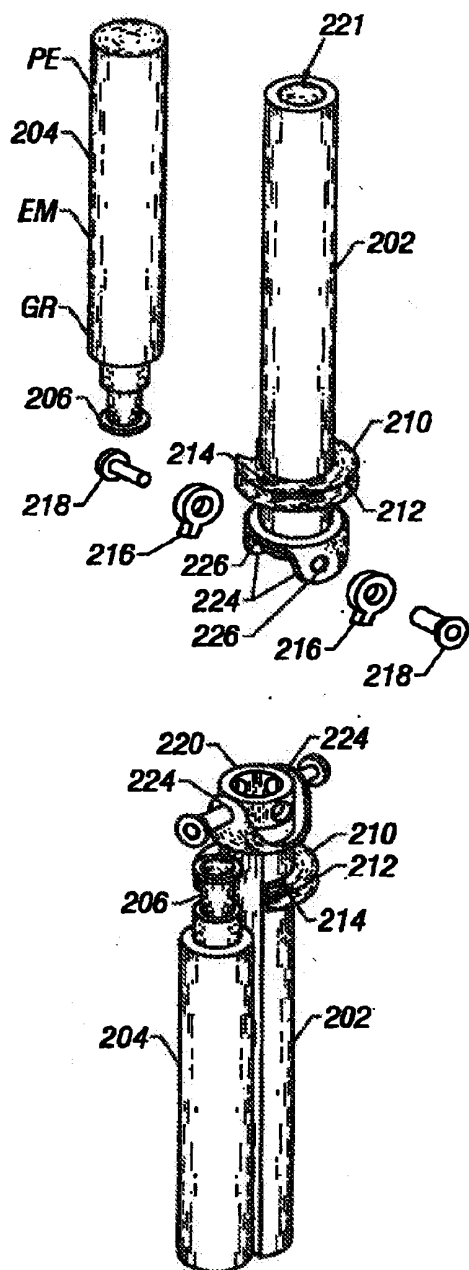


FIG. 13A

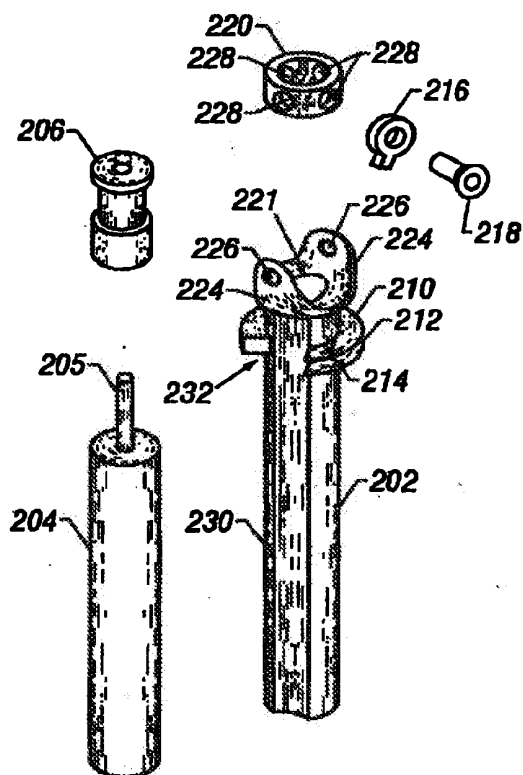


FIG. 13B

FIG. 14

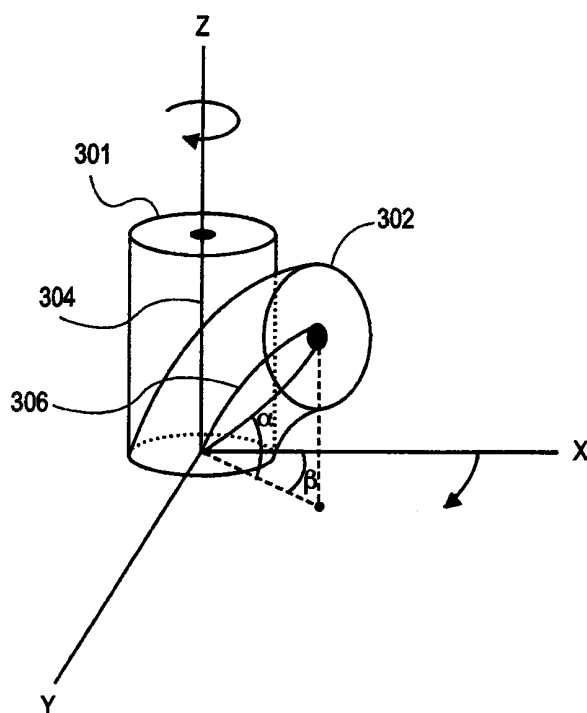


FIG. 15A

FIG. 15B

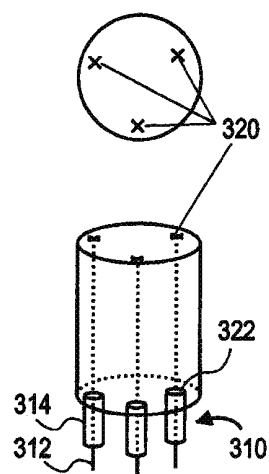


FIG. 15C

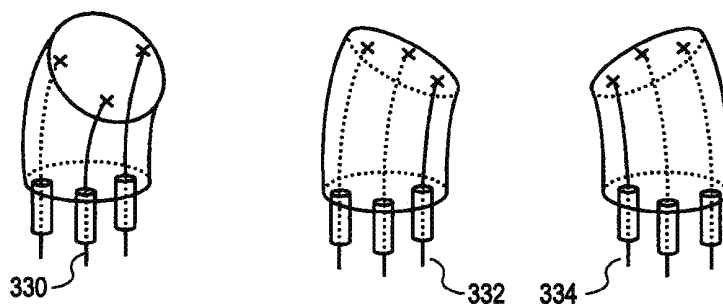


FIG. 15D

FIG. 15E

FIG. 15F

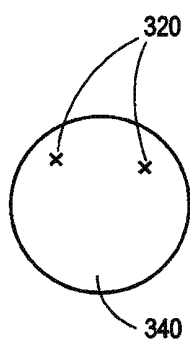


FIG. 16A

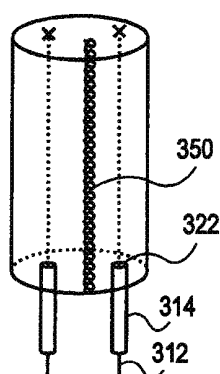


FIG. 16B

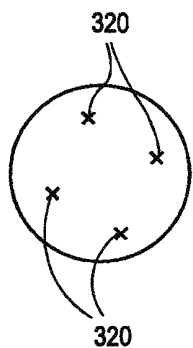


FIG. 16C

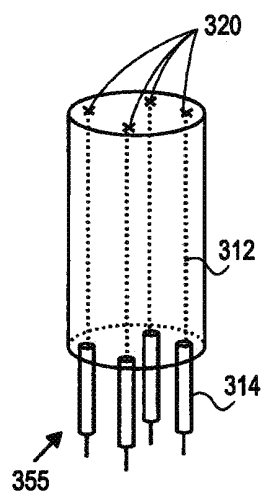
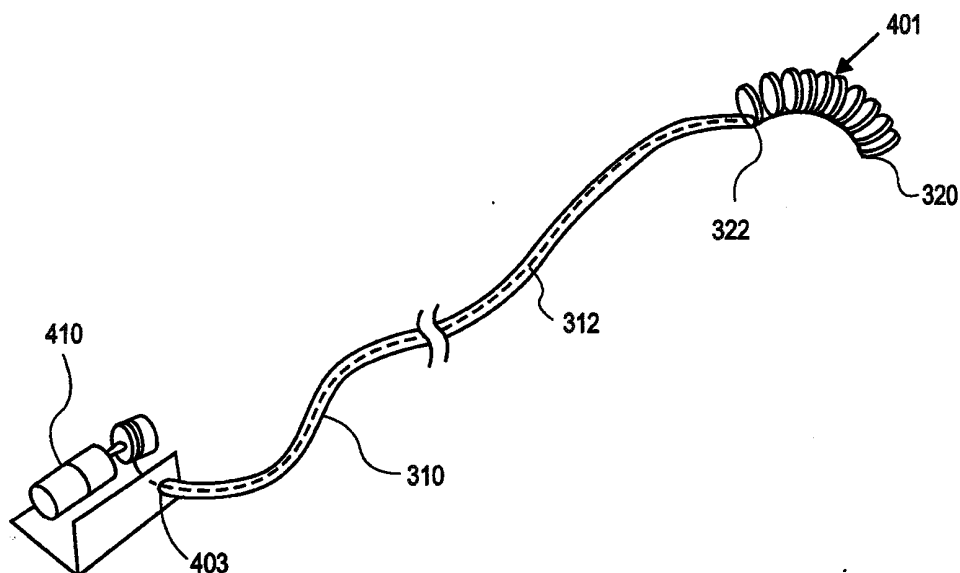


FIG. 16D

FIG. 17



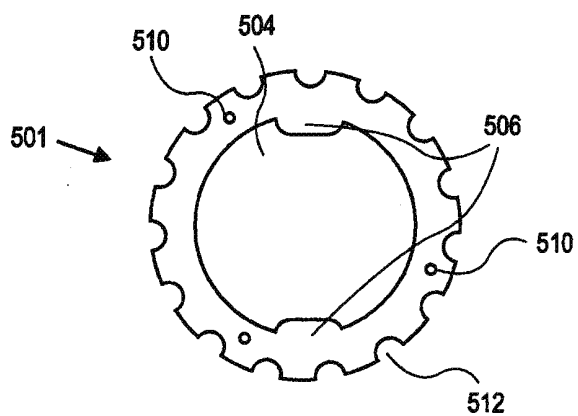


FIG. 18A

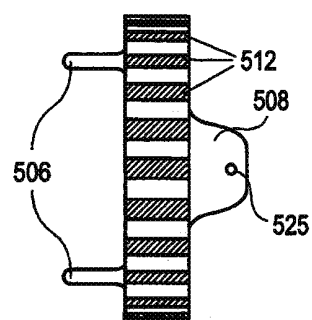


FIG. 18B

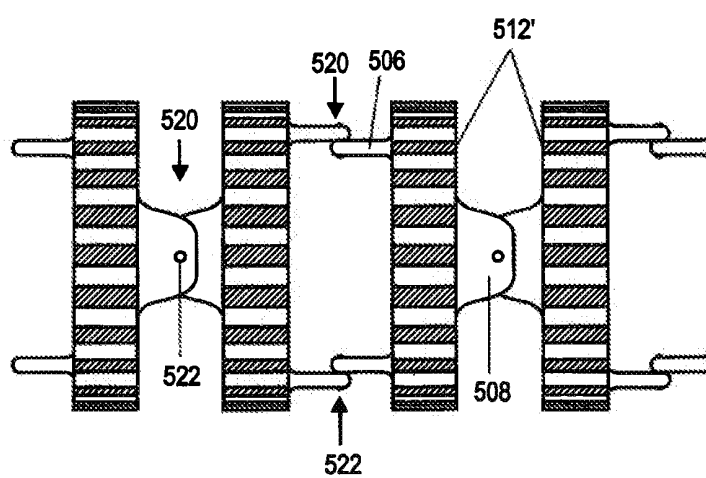


FIG. 18C

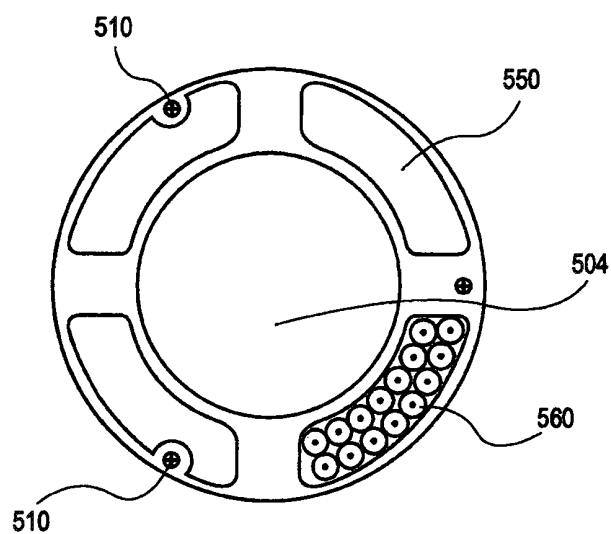


FIG. 18D

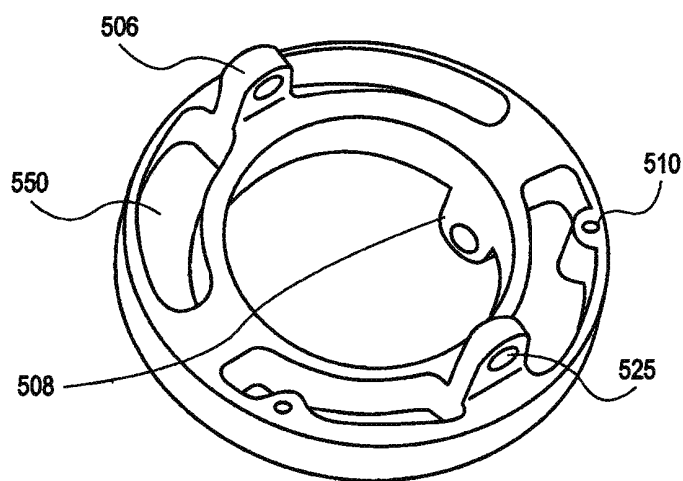


FIG. 18E

FIG. 19A

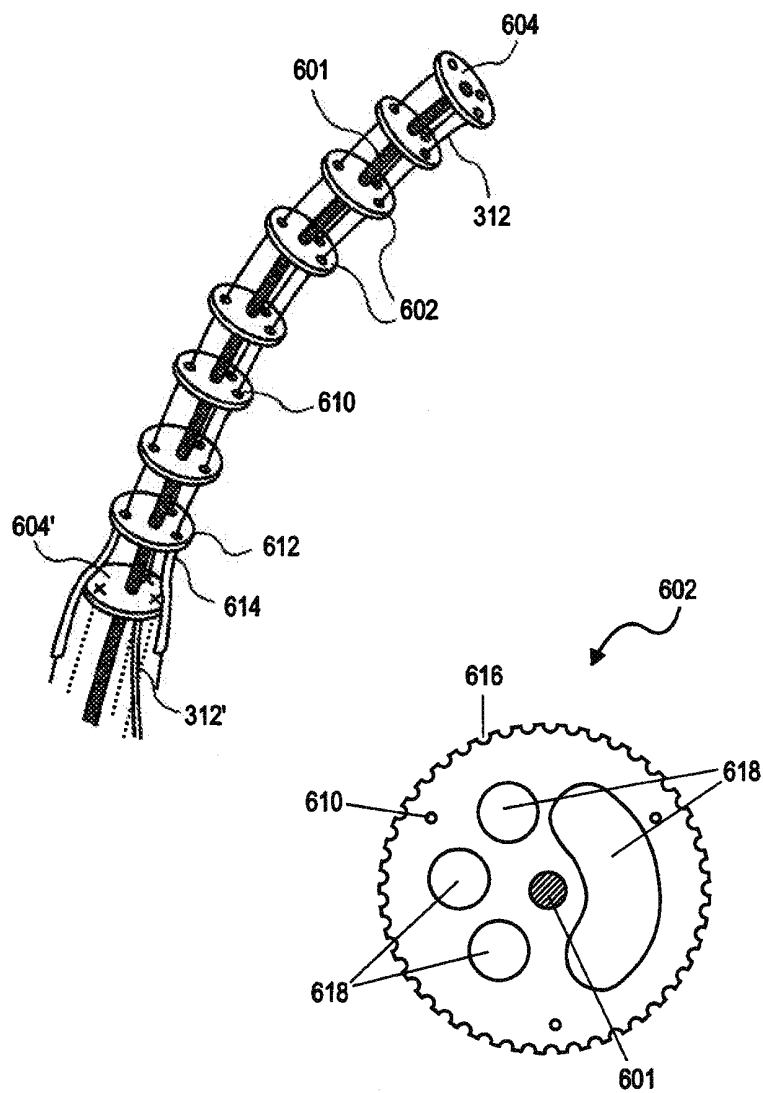


FIG. 19B

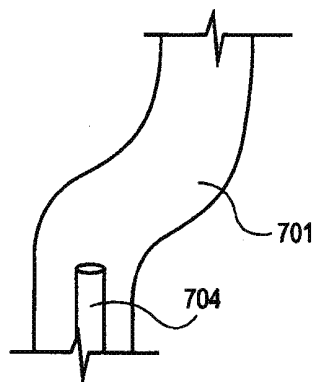


FIG. 20A

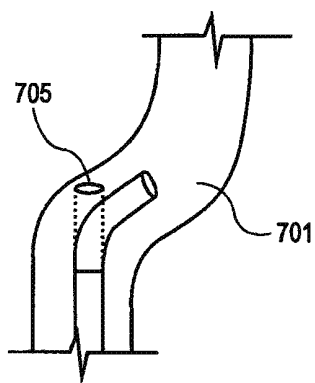


FIG. 20B

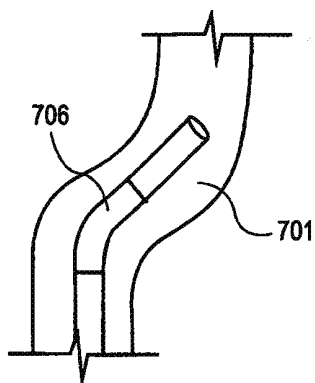


FIG. 20C

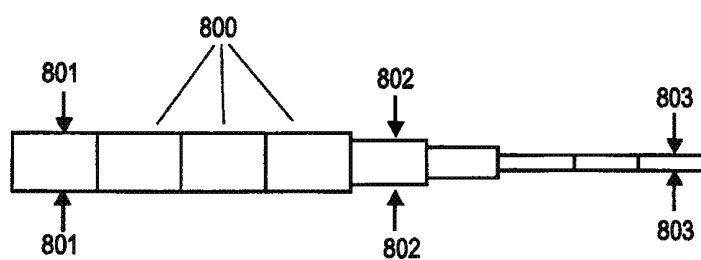


FIG. 21

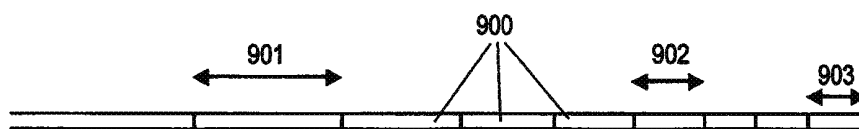


FIG. 22

APPARATUS AND METHOD FOR ENDOSCOPIC COLECTOMY

CROSS REFERENCE TO RELATED APPLICATIONS

[0001] This is a divisional application of U.S. patent application Ser. No. 10/327,370 filed Dec. 20, 2002, which claims the benefit of priority U.S. Provisional Patent Application Ser. No. 60/347,674 filed Jan. 9, 2002, the entirety of which is incorporated herein by reference.

FIELD OF THE INVENTION

[0002] The present invention relates generally to surgical methods and apparatus. More particularly, it relates to methods and apparatus for performing endoscopic colectomy.

BACKGROUND OF THE INVENTION

[0003] Endoscopy studies the intraluminal aspects of hollow organs of the upper and lower intestine including the esophagus, stomach and the colon through cannulation of the lumen via the mouth or anus. Endoscopic polypectomy is presently limited to a submucosal resection. The endoscopist is often unable to completely resect a sessile polyp or lesion and therefore the patient is subjected to subsequent definitive surgery, i.e. resection of the base of the tumor. Endoscopic polypectomy can be used to debulk sessile masses but it is unable to resect mural disease. Incomplete resection of a sessile polyp may destroy the biopsy specimen and alter the relationship of the gross specimen given to the pathologist thereby resulting in the pathologist possibly providing incorrect or incomplete study results. The endoscopist is also unable to correct uncommon, but life threatening, procedural complications such as perforations. Other cases where resection is required are invasive tumors, perforation from different causes, inflammatory bowel disease, diverticulosis and others.

[0004] Surgical approaches for resecting diseased tissue are largely practiced by making large laparotomy incisions or using minimally invasive techniques such as laparoscopic surgery in which tissues are resected and repaired through small incisions.

[0005] There are numerous surgical devices enabling surgeons to resect diseased tissue and subsequently anastomose remaining tissue either through a conventional incision or using a laparoscope and making one or more relatively small incisions. Additionally, endoscopically assisted stapling devices are known which enable surgeons to remotely anastomose luminal structures such as the bowel. Endoscopically assisted bowel anastomosis nevertheless typically requires extraluminal assistance via a traditional laparotomy incision or use of a laparoscope.

[0006] Trends in surgery are towards minimally invasive procedures as evidenced by developments including laparoscopic cholecystectomy, laparoscopic appendectomy and laparoscopically assisted partial colectomies and hernia repairs. All of these minimally invasive procedures involve introducing a laparoscope through the abdominal wall and creating other associated openings to gain access to the peritoneal cavity in order to perform the necessary surgical procedure. Typically, general anesthesia is required. Endoscopically possible procedures include polypectomy, mucosectomy, and cauterization. During "laparoscopic colectomy" today the colon is separated from its omentum

laparoscopically and then the colon is exteriorized out of the abdominal cavity, through a laparotomy incision where the resection and anastomosis are performed extracorporeally.

[0007] Disadvantages of the laparoscopic method include the need to traverse the abdominal wall, increased operating time secondary to the lack of exposure for the procedure and possibly the need to convert to an "open" laparotomy in the course of performing the procedure.

[0008] Present stapling techniques in surgery are for the most part functionally adequate but limited. Devices exist including the GIA and EEA staplers which can be used to transect tissue in a linear or circular fashion, respectively, with subsequent anastomosis with staples. The linear GIA is relatively versatile. The EEA is primarily suited for lower colonic circular anastomosis after a lesion has been surgically removed (via laparotomy or laparoscopically) or during a colectomy takedown procedure.

[0009] The rigid post of the EEA stapler severely limits its use, as well as requiring that an open procedure be utilized. The steerable endoscopic stapler is useful in allowing for more bowel accessibility; however, it remains dependent upon transabdominal surgical exposure prior to utilization. While laparoscopic surgical instruments have been used for bowel anastomosis, in such procedures the bowel is exteriorized through the laparoscopic incision and anastomosed extracorporeally or in an augmented stapled side-to-side fashion.

[0010] U.S. Pat. Nos. 5,868,760 and 6,264,086 describe a method and apparatus for performing endolumenal resection of tissue, in particular for removal of diseased portions of a patient's colon. This purely endolumenal approach to colectomy does not fully address the surgical anatomy of the colon. As is well known, the colon and other viscera are connected and supported within the abdomen by the omentum, a membranous extension of the peritoneum that carries the blood supply to the colon. Resection of more than a small portion of the colon requires mobilization of the colon from the omentum and ligation or cauterization of the blood vessels supplying that portion of the colon. This aspect is not addressed by the endolumenal approach described; therefore it would be suitable for resecting only small portions of the colon.

[0011] Commonly owned and copending U.S. patent application Ser. Nos. 09/790,204 filed Feb. 20, 2001 (now U.S. Pat. No. 6,468,203); 09/969,927 filed Oct. 2, 2001; and 10/229,577 filed Aug. 27, 2002, describe steerable colonoscopes that uses serpentine motion to facilitate rapid and safe insertion of the colonoscope into a patient's colon. The technology described therein can also be used in conjunction with the methods and apparatus of the present invention to facilitate endoscopic colectomy or resection of any other part of the gastrointestinal system including, but not limited to, the esophagus, duodenum, jejunum and ileum or any other tubular organ like the bronchus. These patents and patent applications, and all other patents and patent applications referred to herein, are hereby incorporated by reference in their entirety.

SUMMARY OF THE INVENTION

[0012] In keeping with the foregoing discussion, the present invention takes the form of methods and apparatus for performing endoscopic colectomy that combine the advantages of the laparoscopic and endolumenal approaches. The diseased portion of the colon to be resected is identified using either laparoscopic and/or colonoscopic techniques or using

another imaging modality. A colectomy device mounted on a colonoscope grasps the colon wall at two sites adjacent to a diseased portion of the colon. Using laparoscopic techniques, the diseased portion of the colon is separated from the omentum and the blood vessels supplying it are ligated or cauterized. The colon wall is transected to remove the diseased portion and the excised tissue is removed using the laparoscope or drawn into the colectomy device for later removal upon withdrawal of the colonoscope. The colectomy device approximates the two ends of the colon and performs an end-to-end anastomosis. If the part to be resected is a tumor, prior to the resection, the edges of the segment to be resected will be stapled to seal it and prevent spillage of malignant cells to the healthy tissue.

[0013] The methods and apparatus of the present invention provide a number of benefits not realized by the prior art approaches to colectomy. As stated above, the purely endoluminal approach does not provide for separation of the colon from the omentum, which is necessary when resecting more than just a small portion of the colon wall. By combining laparoscopic techniques with a colonoscope-mounted colectomy device, the present invention overcomes this deficiency in the prior art allowing a more comprehensive approach to colectomy. Unlike prior art laparoscopic techniques, however, the colon does not need to be exteriorized for excision of the diseased portion or anastomosis of the remaining colon. The colonoscope-mounted colectomy device approximates the ends of the colon and performs an anastomosis from the interior of the lumen of the colon. The excised tissue can be drawn into the colectomy device for removal through the lumen of the colon along with the colonoscope or can be taken out by the laparoscope, which can be done through a very small incision in the patient's skin. The prior art approach also does not protect from leaking of malignant cells to the periphery. This idea will enable sealing of the tissue with staples at its ends to prevent such leakage. Optionally, it will be done with the help of a laparoscopic device that will serve as an anvil. Unlike the prior art procedure, the present invention will optionally use a balloon inflated in the lumen of the colon or any other resected organ before stapling, and by this assure the anastomosis will be ideal with the best possible approximation of the edges.

[0014] The use of colonoscopic techniques in the present invention provides another benefit not realized by a purely laparoscopic approach. Since colonoscopic examination is at present the most definitive diagnostic method for identifying diseases of the colon, locating the lesions through the exterior of the colon by laparoscopy or even by direct visualization can be somewhat problematic. Using the colonoscope to identify and isolate the diseased portion of the colon from within the lumen helps assure that the correct portions of the colon wall are excised and makes clean surgical margins without residual disease more assured as well.

[0015] In a preferred embodiment, the present invention utilizes a steerable colonoscope as described in U.S. patent application Ser. Nos. 09/790,204 (now U.S. Pat. No. 6,468,203); 09/969,927; and 10/229,577, which have been incorporated by reference. The steerable colonoscope described therein provides a number of additional benefits for performing endoscopic colectomy according to the present invention. The steerable colonoscope uses serpentine motion to facilitate rapid and safe insertion of the colonoscope into the patient's colon, which allows the endoscopic colectomy method to be performed more quickly and more safely.

Beyond this however, the steerable colonoscope has the capability to create a three-dimensional mathematical model or map of the patient's colon and the location of any lesions identified during the initial examination. Lesions found during a previous examination by CT, MRI or any other imaging technology can also be mapped onto the three-dimensional mathematical model of the colon. By generating a three-dimensional map of the colon, the system knows where each part of the endoscope is in the colon and will be able to localize the two parts of the dissecting and stapling system exactly in the desired location. During surgery, this information can be used to quickly and accurately return the colonoscope to the location of the identified lesions where the colonoscope-mounted colectomy device will be used to complete the endoscopic colectomy procedure.

BRIEF DESCRIPTION OF THE DRAWINGS

[0016] FIG. 1 is a phantom drawing illustrating a diseased portion of the colon being separated from the omentum using laparoscopic techniques through a small incision in a patient's abdomen.

[0017] FIG. 2 is a cutaway drawing illustrating a steerable colonoscope with a colectomy device mounted thereon being inserted through the lumen of a patient's colon.

[0018] FIG. 3 is a cutaway drawing showing the gripping mechanism of the colonoscope-mounted colectomy device expanded within the lumen of the colon.

[0019] FIG. 4 illustrates the colon after the diseased portion has been excised and removed with the colonoscope-mounted colectomy device in position to approximate the transected ends of the colon.

[0020] FIG. 5 illustrates the colonoscope-mounted colectomy device performing an end-to-end anastomosis to complete the endoscopic colectomy procedure.

[0021] FIG. 6 shows a first embodiment of the steerable endoscope of the present invention.

[0022] FIG. 7 shows a second embodiment of the steerable endoscope of the present invention.

[0023] FIG. 8 shows a wire frame model of a section of the body of the endoscope in a neutral or straight position.

[0024] FIG. 9 shows the wire frame model of the endoscope body shown in FIG. 8 passing through a curve in a patient's colon.

[0025] FIG. 10 shows a representative portion of an alternative endoscopic body embodiment having multiple segments interconnected by joints.

[0026] FIG. 11 shows a partial schematic representation of the embodiment of FIG. 10 showing two segments being pivotable about two independent axes.

[0027] FIG. 12 shows a preferable endoscope embodiment having motorized segmented joints.

[0028] FIGS. 13A-13B show exploded isometric assembly views of two adjacent segments and an individual segment, respectively, from the embodiment shown in FIG. 12.

[0029] FIG. 14 shows a variation of the tendon driven endoscope of the present invention.

[0030] FIG. 15A shows the range of motion of a controllable segment of the present invention actuated by three tendons.

[0031] FIGS. 15B to 15F show the use of three tendons to actuate a controllable segment used in the endoscope of the present invention.

[0032] FIGS. 16A and 16B show the use of two tendons to actuate a controllable segment in the endoscope of the present invention.

[0033] FIGS. 16C and 16D show the use of four tendons to actuate a controllable segment in the endoscope of the present invention.

[0034] FIG. 17 shows a partial schematic representation of a single tendon bending a segment.

[0035] FIGS. 18A and 18B show an end view and a side view, respectively, of a vertebra-type control ring which may be used to form the controllable segments of the endoscope of the present invention.

[0036] FIG. 18C shows a side view of interconnected vertebra-type control rings used to form the controllable segments of the endoscope of the present invention.

[0037] FIGS. 18D and 18E show a side view and a perspective view, respectively, of another embodiment of a vertebra-type control ring.

[0038] FIG. 19A shows a perspective view of an endoscope device variation with the outer layers removed to reveal the control rings and backbone.

[0039] FIG. 19B shows an end view of a variation of the control ring for an endoscope of the present invention.

[0040] FIGS. 20A to 20C illustrate advancing the tendon driven endoscope of the present invention through a tortuous path.

[0041] FIG. 21 shows a variation of the tendon driven endoscope of the present invention that has segments of differing diameters.

[0042] FIG. 22 shows a variation of the tendon-driven endoscope of the present invention that has segments of different length.

DETAILED DESCRIPTION OF THE INVENTION

[0043] FIG. 2 is a cutaway drawing illustrating a steerable colonoscope 100 with a colectomy device 102 mounted thereon being inserted through the lumen of a patient's colon. As mentioned before, the same technique may apply for every other tubular shaped organ. Preferably, the steerable colonoscope 100 is constructed as described in U.S. patent application Ser. Nos. 09/790,204 (now U.S. Pat. No. 6,468,203); 09/969,927 (now U.S. Pat. No. 6,610,007); and 10/229,577 (now U.S. Pat. No. 6,858,005), with multiple articulating segments that are controlled to move with a serpentine motion that facilitates insertion and withdrawal of the colonoscope with a minimum of contact and stress applied to the colon walls. Additional details and various embodiments of the steerable colonoscope 100 are described below with reference to FIGS. 6-22. In addition, the control system of the steerable colonoscope 100 has the capability to construct a three-dimensional mathematical model or map of the colon as it advances through lumen under control of the operator. The three-dimensional mathematical model of the colon and the location and nature of any lesions identified in the course of an initial colonoscopic examination can be stored and used in performance of the endoscopic colectomy procedure. In alternate embodiments, the colectomy device 102 of the present invention may be mounted on a colonoscope of a different design and construction.

[0044] The colectomy device 102 can be permanently or removably mounted on the steerable colonoscope 100. The colectomy device 102 has a distal component 104 and a proximal component 106. The distal component 104 and the proximal component 106 each have an expandable member

108 and a gripping mechanism 110 for gripping the wall of the colon. The expandable member 108 may be an inflatable balloon or a mechanically expandable mechanism. The gripping mechanism 110 may comprise a plurality of circumferentially located ports within which attachment points 112, e.g., needles, hooks, barbs, etc., may be retractably positioned about an exterior surface of the expandable member 108. Alternatively, the gripping mechanism 110 may utilize a vacuum gripper through a plurality of circumferentially located ports around the distal component 104 and/or the proximal component 106 or other known gripping mechanisms. In the case of the vacuum gripper, gripping mechanism 110 is in fluid communication through the ports and through the colonoscope 100 to the proximal end of the colonoscope 100 to a vacuum pump (not shown). At least one, and optionally both, of the distal component 104 and the proximal component 106 are movable longitudinally with respect to the body of the steerable colonoscope 100. Rails, grooves or the like 114 may be provided on the body of the steerable colonoscope 100 for guiding the longitudinal movement of the distal component 104 and the proximal component 106.

[0045] In addition, the colectomy device 102 includes a surgical stapler 116 or other anastomosis mechanism. The surgical stapler 116 is carried on either the distal component 104 or the proximal component 106 and a stapler anvil 118 is carried on the other of these components. The surgical stapler 116 may be configured similarly to any number of conventional stapling devices which are adapted to actuate staples into tissue. Another option is that there is a stapler and an anvil on both components for stapling and sealing the edges. Optionally, the colectomy device 102 may include a cutting device and/or electrocautery and/or a laser device for transecting the colon wall. Optionally, the colectomy device 102 may also include a vacuum mechanism or the like for drawing the excised tissue into the colectomy device 102 for later removal along with the steerable colonoscope 100.

[0046] FIG. 2 shows the steerable colonoscope 100 with the expandable members 108 of the distal component 104 and the proximal component 106 in a contracted or deflated condition for easy passage through the lumen of the patient's colon. The control system of the steerable colonoscope 100 monitors the position of each segment of the colonoscope 100 as it is advanced within the colon and can signal to the operator when the segments carrying the distal component 104 and the proximal component 106 of the colectomy device 102 are correctly positioned with respect to a previously detected lesion in the colon. Alternatively, the control system of the steerable colonoscope 100 can be programmed to advance the colonoscope 100 automatically through the lumen of the colon and to stop it when the distal component 104 and the proximal component 106 of the colectomy device 102 are correctly positioned with respect to the lesion in the colon. Alternatively, the control system will be able to automatically guide and deliver the two components to the desired location after the colonoscope has been inserted to the colon.

[0047] FIG. 3 is a cutaway drawing showing the expandable members 108 of the distal component 104 and the proximal component 106 of the colonoscope-mounted colectomy device 102 expanded within the lumen of the colon so that the gripping mechanism 110 grips the wall of the colon. The distal component 104 and the proximal component 106 may be expanded through any number of expansion devices. For instance, they may be radially expanded upon spoke-like support structures or they may be configured to radially

expand in a rotational motion until the desired expansion diameter is attained. At this point, with the diseased portion of the colon identified and isolated by the colonoscope-mounted colectomy device **102**, the diseased portion is separated from the omentum and the blood vessels supplying it are ligated and/or cauterized using laparoscopic techniques. FIG. **1** is a phantom drawing illustrating a diseased portion of the colon being separated from the omentum using laparoscopic techniques through a small incision in a patient's abdomen.

[0048] Next, the diseased portion of the colon is excised by transecting the colon at the proximal and distal end of the diseased portion. The colon may be transected using laparoscopic techniques or using a cutting mechanism and/or electrocautery drawing mounted on the colectomy device **102**. The excised tissue is removed using the laparoscope or drawn into the colectomy device **102** for later removal upon withdrawal of the steerable colonoscope **100**. FIG. **4** illustrates the colon after the diseased portion has been excised and removed with the colonoscope-mounted colectomy device **102** in position to approximate the transected ends of the colon.

[0049] The remaining ends of the colon are approximated one to the other by moving the distal component **104** and/or the proximal component **106** longitudinally with respect to the body of the steerable colonoscope **100**, as shown by the arrows. Optionally, the proximal component **106** may be longitudinally translated towards the distal component **104** or both components **104**, **106** may be approximated simultaneously towards one another. The ends of the colon are stapled to one another to create an end-to-end anastomosis **120** using the surgical stapler **116** and stapler anvil **118** on the colectomy device **102**. Once the ends of the tissue have been approximated, staples or other fastening devices, e.g., clips, screws, adhesives, sutures, and combinations thereof, etc., may be actuated through the surgical stapler **116** such that they pierce both ends of the tissue against the stapler anvil **118**. FIG. **5** illustrates the colonoscope-mounted colectomy device performing an end-to-end anastomosis **120** to complete the endoscopic colectomy procedure. Once the anastomosis **120** is complete, the expandable members **108** of the distal component **104** and the proximal component **106** are deflated or contracted and the steerable colonoscope **100** and the colectomy device **102** are withdrawn from the patient's body. The expanded members will assure a very accurate end-to-end anastomosis and prevent stenosis that can happen as a result of inaccurate approximation of the two ends.

[0050] In an alternative method using the colonoscope-mounted colectomy device **102**, the diseased portion of the colon may be excised using a cutting device within the colectomy device **102** after the ends of the diseased portion have been approximated and anastomosed. The excised tissue is drawn into the colectomy device **102** and removed when the steerable colonoscope **100** is withdrawn from the patient.

[0051] In another alternative method, the colectomy procedure may be performed entirely from the endolumenal approach using the colonoscope-mounted colectomy device **102** without laparoscopic assistance. This method would be particularly advantageous for resection of small portions of the colon where it may not be necessary to mobilize an extended portion of the colon from the omentum to achieve successful approximation and anastomosis. The three-dimensional mapping capability of the steerable colonoscope **102** would be used to locate previously identified lesions without laparoscopic assistance.

Steerable Colonoscope

[0052] FIG. **6** shows a first embodiment of the steerable endoscope **100** of the present invention. The endoscope **100** has an elongate body **103** with a manually or selectively steerable distal portion **105** and an automatically controlled proximal portion **107**. The selectively steerable distal portion **105** can be selectively steered or bent up to a full 180 degree bend in any direction. A fiberoptic imaging bundle **113** and one or more illumination fibers **115** extend through the body **103** from the proximal end **111** to the distal end **109**. Alternatively, the endoscope **100** can be configured as a video endoscope with a miniaturized video camera, such as a CCD camera, positioned at the distal end **109** of the endoscope body **103**. The images from the video camera can be transmitted to a video monitor by a transmission cable or by wireless transmission. Optionally, the body **103** of the endoscope **100** may include one or two instrument channels **117**, **119** that may also be used for insufflation or irrigation. The body **103** of the endoscope **100** is highly flexible so that it is able to bend around small diameter curves without buckling or kinking. When configured for use as a colonoscope, the body **103** of the endoscope **100** is typically from 135 to 185 cm in length and approximately 12-13 mm in diameter. The endoscope **100** can be made in a variety of other sizes and configurations for other medical and industrial applications.

[0053] A proximal handle **121** is attached to the proximal end **111** of the elongate body **103**. The handle **121** includes an ocular **124** connected to the fiberoptic imaging bundle **113** for direct viewing and/or for connection to a video camera **126**. The handle **121** is connected to an illumination source **128** by an illumination cable **134** that is connected to or continuous with the illumination fibers **115**. A first luer lock fitting **130** and a second luer lock fitting **132** on the handle **121** are connected to the instrument channels **117**, **119**.

[0054] The handle **121** is connected to an electronic motion controller **140** by way of a controller cable **136**. A steering control **122** is connected to the electronic motion controller **140** by way of a second cable **138**. The steering control **122** allows the user to selectively steer or bend the selectively steerable distal portion **105** of the body **103** in the desired direction. The steering control **122** may be a joystick controller as shown, or other known steering control mechanism. The electronic motion controller **140** controls the motion of the automatically controlled proximal portion **107** of the body **103**. The electronic motion controller **140** may be implemented using a motion control program running on a micro-computer or using an application-specific motion controller. Alternatively, the electronic motion controller **140** may be implemented using a neural network controller.

[0055] An axial motion transducer **150** is provided to measure the axial motion of the endoscope body **103** as it is advanced and withdrawn. The axial motion transducer **150** can be made in many possible configurations. By way of example, the axial motion transducer **150** in FIG. **6** is configured as a ring **152** that surrounds the body **103** of the endoscope **100**. The axial motion transducer **150** is attached to a fixed point of reference, such as the surgical table or the insertion point for the endoscope **100** on the patient's body. As the body **103** of the endoscope **100** slides through the axial motion transducer **150**, it produces a signal indicative of the axial position of the endoscope body **103** with respect to the fixed point of reference and sends a signal to the electronic motion controller **140** by telemetry or by a cable (not shown). The axial motion transducer **150** may use optical, electronic

or mechanical means to measure the axial position of the endoscope body 103. Other possible configurations for the axial motion transducer 150 are described below.

[0056] FIG. 7 shows a second embodiment of the endoscope 100 of the present invention. As in the embodiment of FIG. 6, the endoscope 100 has an elongate body 103 with a selectively steerable distal portion 105 and an automatically controlled proximal portion 107. The steering control 122 is integrated into proximal handle 121 in the form of one or two dials for selectively steering the selectively steerable distal portion 105 of the endoscope 100. Optionally, the electronic motion controller 140 may be miniaturized and integrated into proximal handle 121, as well. In this embodiment, the axial motion transducer 150 is configured with a base 154 that is attachable to a fixed point of reference, such as the surgical table. A first roller 156 and a second roller 158 contact the exterior of the endoscope body 103. A multi-turn potentiometer 160 or other motion transducer is connected to the first roller 156 to measure the axial motion of the endoscope body 103 and to produce a signal indicative of the axial position.

[0057] The endoscope 100 may be manually advanced or withdrawn by the user by grasping the body 103 distal to the axial motion transducer 150. Alternatively, the first roller 156 and/or second roller 158 may be connected to a motor 162 for automatically advancing and withdrawing the body 103 of the endoscope 100.

[0058] FIG. 8 shows a wire frame model of a section of the body 103 of the endoscope 100 in a neutral or straight position. Most of the internal structure of the endoscope body 103 has been eliminated in this drawing for the sake of clarity. The endoscope body 103 is divided up into sections 1, 2, 3 . . . 10, etc. The geometry of each section is defined by four length measurements along the a, b, c and d axes. For example, the geometry of section 1 is defined by the four length measurements l_{1a} , l_{1b} , l_{1c} , l_{1d} , and the geometry of section 2 is defined by the four length measurements l_{2a} , l_{2b} , l_{2c} , l_{2d} , etc. Preferably, each of the length measurements is individually controlled by a linear actuator (not shown). The linear actuators may utilize one of several different operating principles. For example, each of the linear actuators may be a self-heating NiTi alloy linear actuator or an electrorheological plastic actuator, or other known mechanical, pneumatic, hydraulic or electromechanical actuator. The geometry of each section may be altered using the linear actuators to change the four length measurements along the a, b, c and d axes. Preferably, the length measurements are changed in complementary pairs to selectively bend the endoscope body 103 in a desired direction. For example, to bend the endoscope body 103 in the direction of the a axis, the measurements l_{1a} , l_{2a} , l_{3a} . . . l_{10a} , would be shortened and the measurements l_{1b} , l_{2b} , l_{3b} . . . l_{10b} , would be lengthened an equal amount. The amount by which these measurements are changed determines the radius of the resultant curve.

[0059] In the selectively steerable distal portion 105 of the endoscope body 103, the linear actuators that control the a, b, c and d axis measurements of each section are selectively controlled by the user through the steering control 122. Thus, by appropriate control of the a, b, c and d axis measurements, the selectively steerable distal portion 105 of the endoscope body 103 can be selectively steered or bent up to a full 180° in any direction.

[0060] In the automatically controlled proximal portion 107, however, the a, b, c and d axis measurements of each section are automatically controlled by the electronic motion

controller 140, which uses a curve propagation method to control the shape of the endoscope body 103. To explain how the curve propagation method operates, FIG. 9 shows the wire frame model of a part of the automatically controlled proximal portion 107 of the endoscope body 103 shown in FIG. 8 passing through a curve in a patient's colon C. For simplicity, an example of a two-dimensional curve is shown and only the a and b axes will be considered. In a three-dimensional curve all four of the a, b, c and d axes would be brought into play.

[0061] In FIG. 9, the endoscope body 103 has been maneuvered through the curve in the colon C with the benefit of the selectively steerable distal portion 105 (this part of the procedure is explained in more detail below) and now the automatically controlled proximal portion 107 resides in the curve. Sections 1 and 2 are in a relatively straight part of the colon C, therefore $l_{1a}=l_{1b}$, and $l_{2a}=l_{2b}$. However, because sections 3-7 are in the S-shaped curved section, $l_{3a}<l_{3b}$, $l_{4a}<l_{4b}$, and $l_{5a}<l_{5b}$, but $l_{6a}>l_{6b}$, $l_{7a}>l_{7b}$ and $l_{8a}>l_{8b}$. When the endoscope body 103 is advanced distally by one unit, section 1 moves into the position marked 1', section 2 moves into the position previously occupied by section 1, section 3 moves into the position previously occupied by section 2, etc. The axial motion transducer 150 produces a signal indicative of the axial position of the endoscope body 103 with respect to a fixed point of reference and sends the signal to the electronic motion controller 140. Under control of the electronic motion controller 140, each time the endoscope body 103 advances one unit, each section in the automatically controlled proximal portion 106 is signaled to assume the shape of the section that previously occupied the space that it is now in. Therefore, when the endoscope body 103 is advanced to the position marked 1', $l_{1a}=l_{1ab}$, $l_{2a}=l_{2b}$, $l_{3a}=l_{3b}$, $l_{4a}<l_{4b}$, $l_{5a}<l_{5b}$, $l_{6a}>l_{6b}$, $l_{7a}>l_{7b}$, $l_{8a}>l_{8b}$, and $l_{9a}>l_{9b}$, and, when the endoscope body 103 is advanced to the position marked 1'', $l_{1a}=l_{1b}$, $l_{2a}=l_{2b}$, $l_{3a}=l_{3b}$, $l_{4a}=l_{4b}$, $l_{5a}<l_{5b}$, $l_{6a}<l_{6b}$, $l_{7a}<l_{7b}$, $l_{8a}>l_{8b}$, $l_{9a}>l_{9b}$, and $l_{10a}>l_{10b}$. Thus, the S-shaped curve propagates proximally along the length of the automatically controlled proximal portion 107 of the endoscope body 103. The S-shaped curve appears to be fixed in space, as the endoscope body 103 advances distally.

[0062] Similarly, when the endoscope body 103 is withdrawn proximally, each time the endoscope body 103 is moved proximally by one unit, each section in the automatically controlled proximal portion 107 is signaled to assume the shape of the section that previously occupied the space that it is now in. The S-shaped curve propagates distally along the length of the automatically controlled proximal portion 107 of the endoscope body 103, and the S-shaped curve appears to be fixed in space, as the endoscope body 103 withdraws proximally.

[0063] Whenever the endoscope body 103 is advanced or withdrawn, the axial motion transducer 150 detects the change in position and the electronic motion controller 140 propagates the selected curves proximally or distally along the automatically controlled proximal portion 107 of the endoscope body 103 to maintain the curves in a spatially fixed position. This allows the endoscope body 103 to move through tortuous curves without putting unnecessary force on the wall of the colon C.

[0064] FIG. 10 shows a representative portion of an alternative endoscopic body embodiment 190 which has multiple segments 192 interconnected by joints 194. In this embodiment, adjacent segments 192 can be moved or angled relative to one another by a joint 194 having at least one degree-of-

freedom, and preferably having multiple degrees-of-freedom, preferably about two axes as shown here. As seen further in FIG. 4, a partial schematic representation 196 of the embodiment 190 is shown where two segments 192 may be rotated about joint 194 about the two independent axes. The range of motion may be described in relation to spherical axes 198 by angles α and β .

[0065] As mentioned above, such a segmented body may be actuated by a variety of methods. A preferable method involves the use of electromechanical motors individually mounted on each individual segment to move the segments relative to one another. FIG. 12 shows a preferable embodiment 200 having motorized segmented joints. Each segment 192 is preferably comprised of a backbone segment 202, which also preferably defines at least one lumen running through it to provide an access channel through which wires, optical fibers, air and/or water channels, various endoscopic tools, or any variety of devices and wires may be routed through. The backbone segment may be made of a variety of materials which are preferably biocompatible and which provide sufficient strength to support the various tools and other components, e.g., stainless steel. Although much of the description is to an individual segment 192, each of the segments 192 are preferably identical, except for the segment (or first few segments) located at the distal tip, and the following description readily applies to at least a majority of the segments 192.

[0066] A single motor, or multiple motors depending upon the desired result and application, may be attached to at least a majority of the segments. An embodiment having a single motor on a segment is illustrated in FIG. 12 where an individual motor 204 is preferably attached to backbone 202 and is sufficiently small and compact enough so as to present a relatively small diameter which is comfortable and small enough for insertion into a patient without trauma. Motor 204, which is shown here as being a small brushed DC motor, may be used for actuating adjacent segments 192 and may be controlled independently from other motors. Various motors, aside from small brushed DC motors, may also be used such as AC motors, linear motors, etc. Each motor 204 also preferably contains within the housing not only the electromechanical motor assembly EM itself, but also a gear reduction stage GR, and a position encoder PE. A gear reduction stage GR attached to the motor assembly EM will allow for the use of the motor 204 in its optimal speed and torque range by changing high-speed, low-torque operating conditions into a more useful low-speed, high-torque output. The position encoder PE may be a conventional encoder to allow the controlling computer to read the position of the segment's joint 194 by keeping track of the angular rotational movement of the output shaft of the motor 204.

[0067] Each motor 204 has a rotatable shaft which extends from an end of the motor 204 to provide for the transmission of power to actuate the segments 192. Upon this shaft, a spool 206 may be rotatably attached with a first end of the cable 208 further wound about the spool 206. The cable 208 may then be routed from spool 206 through a channel 212 which is defined in the cable guide 210 and out through opening 214 (as seen in greater detail in FIGS. 13A-13B) to cable anchor 216, to which the second end of the cable 208 is preferably attached, e.g., by crimping and/or soldering. The cable guide 210 serves to capture the cable 208 that is wound about the spool 206. The cable anchor 216 is attached across a universal joint pivot 220 to an adjacent segment 192 via a pin 218 and

may be shaped like a conventional electronic ring connector having a round section defining a hole therethrough for mounting to the segment 192 and an extension protruding from the anchor 216 for attaching the second end of the cable 208. Cable 208 may comprise a wide variety of filaments, strands, wires, chains, braids, etc. any of which may be made of a wide variety of biocompatible materials, e.g., metals such as stainless steel, polymers such as plastics and Nylon, etc.

[0068] In operation, when the motor 204 is operated to spin the shaft in a first direction, e.g., clockwise, the spool 206 rotates accordingly and the cable 208 pulls in a corresponding direction on the adjacent segment 192 and transmits the torque to subsequently actuate it along a first axis. When the motor 204 is operated to spin the shaft in a second direction opposite to the first, e.g., counter-clockwise, the spool 206 again rotates accordingly and the cable 208 would then pull in the corresponding opposing direction on the adjacent segment 192 to subsequently transmit the torque and actuate it in the opposite direction.

[0069] FIGS. 13A and 13B show exploded isometric assembly views of two adjacent segments and an individual segment, respectively, from the embodiment shown in FIG. 12. As seen in FIG. 13A, backbone 202 is seen with the lumen 221, which may be used to provide a working channel, as described above. Also seen are channel 212 defined in cable guide 210 as well as opening 214 for the cable 208 to run through. In interconnecting adjacent segments and to provide the requisite degree-of-freedom between segments, a preferable method of joining involves using the universal joint pivot 220. However, other embodiments, rather than using a universal joint pivot 220, may use a variety of joining methods, e.g., a flexible tube used to join two segments at their respective centers, a series of single degree-of-freedom joints that may be closely spaced, etc. This particular embodiment describes the use of the universal joint pivot 220. At the ends of backbone 202 adjacent to other segments, a pair of universal yoke members 224 may be formed with a pair of corresponding pin openings 226. As the universal joint pivot 220 is connected to a first pair of yoke members 224 on one segment, a corresponding pair of yoke members 224 from the adjacent segment may also be attached to the joint pivot 220.

[0070] As seen further in FIG. 13B, the universal joint pivot 220 is shown in this embodiment as a cylindrical ring having two sets of opposing receiving holes 228 for pivotally receiving corresponding yoke members 224. The receiving holes 228 are shown as being spaced apart at 90.degree. intervals, however, in other variations, receiving holes may be spaced apart at other angles depending upon the desired degree-of-freedom and application. Also seen is an exploded assembly of spool 206 removed from motor 204 exposing drive shaft 205. With motor 204 displaced from backbone 202, the groove 230 is revealed as formed in the backbone 202. This groove 230 may be depressed in backbone 202 to preferably match the radius of the motor 204 housing not only to help locate the motor 204 adjacent to backbone 202, but also to help in reducing the overall diameter of the assembled segment. The motor 204 may be attached to the backbone 202 by various methods, e.g., adhesives, clamps, bands, mechanical fasteners, etc. A notched portion 232 may also be formed in the cable guide 210 as shown to help in further reducing segment diameter.

[0071] Prior to insertion into a patient, the endoscope 200 may optionally be configured to have a diagnostic check performed automatically. When the endoscope 200 is wound

onto a drum, adjacent segments **192** will have a predetermined angle relative to one another, as determined initially by the diameter of the drum and the initial configuration of the storage unit in which the endoscope **200** may be positioned. During a diagnostic check before insertion, a computer may be configured to automatically sense or measure the angles between each adjacent segments **192**. If any of the adjacent segments **192** indicate a relative measured angle out of a predetermined acceptable range of angles, this may indicate a segment **192** being out of position and may indicate a potential point of problems during endoscope **200** use. Accordingly, the computer may subsequently sound an audible or visual alarm and may also place each of the segments **192** into a neutral position to automatically prevent further use or to prevent any trauma to the patient.

[0072] FIG. **14** shows a variation of the tendon driven endoscope **20** of the present invention. The endoscope **20** has an elongate body **21** with a manually or selectively steerable distal portion **24**, an automatically controlled portion **28**, and a flexible and passively manipulated proximal portion **22**, which may be optionally omitted from the device. The steerable distal portion **24** can be articulated by hand or with mechanical assistance from actuators. The automatically controlled portion **28** is segmented, and each segment is capable of bending through a full range of steerable motion. The distal portion **24** is also a controllable segment.

[0073] The selectively steerable distal portion **24** can be selectively steered or bent up to, e.g., a full 180.degree. bend in any direction **26**, as shown. A fiberoptic imaging bundle **40** and one or more illumination fibers **42** may extend through the body **21** from the proximal portion **22** to the distal portion **24**. Alternatively, the endoscope **20** may be configured as a video endoscope with a miniaturized video camera, such as a CCD or CMOS camera, positioned at the distal portion **24** of the endoscope body **21**. The images from the video camera can be transmitted to a video monitor by a transmission cable or by wireless transmission where images may be viewed in real-time and/or recorded by a recording device onto analog recording medium, e.g., magnetic tape, or digital recording medium, e.g., compact disc, digital tape, etc. LEDs or other light sources could also be used for illumination at the distal tip of the endoscope.

[0074] The body **21** of the endoscope **20** may also include one or more access lumens **38** that may optionally be used for illumination fibers for providing a light source, insufflation or irrigation, air and water channels, and vacuum channels. Generally, the body **21** of the endoscope **20** is highly flexible so that it is able to bend around small diameter curves without buckling or kinking while maintaining the various channels intact. When configured for use as a colonoscope, the body **21** of the endoscope **20** may range typically from 135 to 185 cm in length and about 13-19 mm in diameter. The endoscope **20** can be made in a variety of other sizes and configurations for other medical and industrial applications.

[0075] The controllable portion **28** is composed of at least one segment **30**, and preferably several segments **30**, which are controllable via a computer and/or electronic controller (controller) **45** located at a distance from the endoscope **20**. Each of the segments **30** has tendons mechanically connected to actuators to allow for the controlled motion of the segments **30** in space. The actuators driving the tendons may include a variety of different types of mechanisms capable of applying a force to a tendon, e.g., electromechanical motors, pneumatic and hydraulic cylinders, pneumatic and hydraulic

motors, solenoids, shape memory alloy wires, electronic rotary actuators or other devices or methods as known in the art. If shape memory alloy wires are used, they are preferably configured into several wire bundles attached at a proximal end of each of the tendons within the controller. Segment articulation may be accomplished by applying energy, e.g., electrical current, heat, etc., to each of the bundles to actuate a linear motion in the wire bundles which in turn actuate the tendon movement. The linear translation of the actuators within the controller may be configured to move over a relatively short distance, e.g., within a few inches or less such as $\pm .1$ inch, to accomplish effective articulation depending upon the desired degree of segment movement and articulation.

[0076] It is preferable that the length of the insertable portion of the endoscope comprises controllable segments **30**, although a passive proximal portion **22** can also be used. This proximal portion **22** is preferably a flexible tubing member that may conform to an infinite variety of shapes, and may be made from a variety of materials such as thermoset and thermoplastic polymers which are used for fabricating the tubing of conventional endoscopes.

[0077] Each segment **30** preferably defines at least one lumen running throughout to provide an access channel through which wires, optical fibers, air and/or water channels, various endoscopic tools, or any variety of devices and wires may be routed. A polymeric covering, or sheath, **39** may also extend over the body of the endoscope **21** including the controllable portion **28** and steerable distal portion **24**. This sheath **39** can preferably provide a smooth transition between the controllable segments **30**, the steerable distal portion **24**, and the flexible tubing of proximal portion **22**.

[0078] A handle **32** may be attached to the proximal end of the endoscope. The handle **32** may include an ocular connected to the fiberoptic imaging bundle **42** for direct viewing. The handle **32** may otherwise have a connector **54** for connection to a video monitor, camera, e.g., a CCD or CMOS camera, or a recording device **52**. The handle **32** may be connected to an illumination source **43** by an illumination cable **44** that is connected to or continuous with the illumination fibers **42**. Alternatively, some or all of these connections could be made at the controller **45**. Luer lock fittings **34** may be located on the handle **32** and connected to the various instrument channels.

[0079] The handle **32** may be connected to a motion controller **45** by way of a controller cable **46**. A steering controller **47** may be connected to the motion controller **45** by way of a second cable **48** or it may optionally be connected directly to the handle **32**. Alternatively, the handle may have the steering control mechanism integrated directly into the handle, e.g., in the form of a joystick, conventional disk controllers such as dials, pulleys or wheels, etc. The steering controller **47** allows the user to selectively steer or bend the selectively steerable distal portion **24** of the body **21** in the desired direction **26**. The steering controller **47** may be a joystick controller as shown, or other steering control mechanism, e.g., dual dials or rotary knobs as in conventional endoscopes, track balls, touchpads, mouse, or sensory gloves. The motion controller **45** controls the movement of the segmented automatically controlled proximal portion **28** of the body **21**. This controller **45** may be implemented using a motion control program running on a microcomputer or using an application-specific motion controller. Alternatively, the controller **45** may be implemented using, e.g., a neural network controller.

[0080] The actuators applying force to the tendons may be included in the motion controller unit 45, as shown, or may be located separately and connected by a control cable. The tendons controlling the steerable distal portion 24 and the controllable segments 30 extend down the length of the endoscope body 21 and connect to the actuators. FIG. 14 shows a variation in which the tendons pass through the handle 32 and connect directly to the motion controller 45 via a quick-release connector 60. In this variation, the tendons are part of the control cable 46, although they could independently connect to the actuators, so long as the actuators are in communication with the controller 45.

[0081] An axial motion transducer (also called a depth referencing device or datum) 49 may be provided for measuring the axial motion, i.e., the depth change, of the endoscope body 21 as it is advanced and withdrawn. The depth referencing device 49 can be made in many possible configurations. For example, the axial motion transducer 49 in FIG. 14 is configured as a ring 49 that may surround the body 21 of the endoscope 20. The axial motion transducer 49 is preferably attached to a fixed point of reference, such as the surgical table or the insertion point for the endoscope 20 on the patient's body. As the body 21 of the endoscope 20 slides through the axial motion transducer 49, it indicates the axial position of the endoscope body 21 with respect to the fixed point of reference and sends a signal to the electronic controller 45 by telemetry or by a cable. The axial motion transducer 49 may use optical, electronic, magnetic, radio frequency or mechanical methods to measure the axial position of the endoscope body 21.

[0082] When the endoscope body 21 is advanced or withdrawn, the axial motion transducer 49 detects the change in position and signals the motion controller 45. The controller can use this information to propagate the selected curves proximally or distally along the controllable portion 28 of the endoscope body 21 to keep the endoscope actively following the pathway selected by the user steering the distal portion 24. The axial motion transducer 49 also allows for the incrementing of a current depth within the colon C by the measured change in depth. This allows the endoscope body 21 to be guided through tortuous curves without putting unnecessary force on the wall of the colon C.

[0083] FIG. 15A shows an example of the resulting segment articulation which may be possible through the use of two or three tendons to articulate the controllable segments, including the steerable distal section. FIG. 15A shows one example of a possible range of motion of a controllable segment of the present invention actuated, in this example, by three tendons. A segment in the relaxed, upright position 301 can be bent in virtually any direction relative to the x-y plane. The figure, as an illustrative example, shows a segment 302 that has been bent down and at an angle relative to its original position 301. The angles α and β describe the bend assumed by the segment. Angle β gives the angle in the x-y plane, while α is the angle describing the motion in the x-z plane. In one variation, the controllable segments of the endoscope can bend through all 360° in the β angle and up to 90° in the α angle. An angle a greater than 90° would result in looping of the endoscope. In FIG. 15A, the segment is shown bent approximately 45° along angle α . The freedom of movement of a segment is, in part, determined by the articulation method, the size of the segment, the materials from which it is constructed, and the manner in which it is constructed, among others. Some of these factors are discussed herein.

[0084] The steerable distal portion, as well as the endoscope and the controllable segments are bendable but preferably not compressible or expansible. Thus, in FIG. 15A, the centerline 304 of the relaxed segment 301 is approximately the same length as the centerline 306 of the segment after bending 302.

[0085] FIGS. 15B to 15F show the use of three tendons to actuate a controllable segment used in an endoscope of the present invention. The tendons shown in this example are all Bowden type cables 310 that have an internal cable 312 coaxially surrounded by a housing or sleeve 314 in which the cable is free to move. Bowden cables can be used to apply either tensile or compressive forces, i.e., they may be pushed or pulled, to articulate the endoscope and can be actuated remotely to deliver forces as desired at locations along the endoscope. Force from a tendon is exerted across or through the segment by attaching the tendon cable at the distal end of the segment 320 and the tendon housing 314 at the proximal end of the segment 322. FIG. 15B shows a view of the top of the segment with three attachment sites for the tendon cables indicated 320.

[0086] In one variation, three tendons are used to actuate each segment, including the steerable distal portion, although four or more tendons could be used. Three tendons can reliably articulate a segment in any direction without having to rotate the segment or endoscope about its longitudinal axis. The three cable tendons 312 are preferably attached at the distal end of the segment 320 close to the segment's edge, spaced equally apart. In FIG. 15B, tendons are attached at the two o'clock, six o'clock and 10 o'clock positions. It is desirable to use fewer tendons, because of space concerns, since the tendons controlling each segment project proximally to the actuators. Thus, two tendons could be used to control a segment. It may also be desirable to include one or more biasing element, e.g., a spring, to assist in articulating a segment in three dimensions. In another variation, two tendons may be used to articulate a segment in three dimensional space by controlling motion in two directions while rotating the segment about its longitudinal axis.

[0087] FIG. 15C shows a relaxed segment with three tendons attached. The tendon sleeves 314 are shown attached to the proximal end of the segment 322 directly below the corresponding cable attachment sites. FIGS. 15D to 15F show this segment bent by each of the controlling tendons 310 separately.

[0088] As shown in FIG. 15D, applying tension by pulling on the first tendon 330 results in a bending in the direction of the first tendon 330. That is, looking down on the top of the unbent segment (as in FIG. 15B), if the first tendon is attached at the six o'clock position, then pulling on just this tendon results in bending the segment towards the six o'clock position. Likewise, in FIG. 15E, putting tension only on a second tendon 332 attached at the two o'clock position results in bending the segment towards the two o'clock direction. Finally, pulling on the tendon in the ten o'clock position 334 bends the segment towards the ten o'clock direction. In all cases, the bending is continuous; the greater the tension applied, the further the bending (the α angle, in the x-z plane of FIG. 15A). A segment can be bent in any direction by pulling on individual tendons or a combination of two tendons. Thus, to bend the segment in the twelve o'clock direction, both the second 332 and the third 334 tendon could be pulled with equal force. Alternatively, first tendon 330 in the six o'clock position may be pushed either alone or in combi-

nation with second **332** and third tendons **334** being pulled to result in the same configuration.

[0089] FIGS. **16A** and **16B** show a variation in which a segment is articulated by two tendons and one biasing element. FIG. **16A** shows a planar top view of the segment. The attachment sites for the biasing element **340** and the two tendons **320** are spaced around the perimeter of the distal end of the segment as shown. The tendons **320** may be attached at the two o'clock and ten o'clock positions, looking down on the top of the section, and the biasing element **340** is attached at the six o'clock position. FIG. **16B** shows a perspective view of the segment in the unbent configuration. In this variation, the biasing element is configured to apply tension to the side of the segment such that it will bend towards the six o'clock position. The biasing element can be any element that can apply compressive or tensile forces across the segment, e.g., a spring, elastic element, a piston, etc. The segment is held in the neutral or unbent position shown in FIG. **16B** by applying tension from both tendons **312**. Controlling the amount of tension applied by the tendons results in bending of the segment in three dimensional space. More than one biasing element could also be used with two or more tendons. For example, a biasing element could be located opposite each tendon.

[0090] Alternatively, if the tendon is a push-pull cable, and each tendon can apply compression as well as tension, then two tendons can control the motion of segment without any biasing element at all.

[0091] More than three tendons can also be used to control the bending of a segment. FIG. **16C** shows a top planar view of a segment that is controlled by four tendons attached in the eleven o'clock, two o'clock, five o'clock and eight o'clock positions. As with the three-tendon embodiment, tension applied on one or a combination of the tendons results in shortening the side of the segment. Thus, if tension is applied only on the tendon attached distally at the eleven o'clock position **355**, the corresponding side of the tendon will shorten, and the segment will bend in the eleven o'clock direction.

[0092] In all these variations, the circumferential locations of the tendons and/or biasing elements are illustrative and are not intended to be limited to the examples described herein. Rather, they may be varied according to the desired effects as understood by one of skill in the art.

[0093] FIG. **17** shows a partial schematic representation of a single tendon bending a segment. For clarity, the other parts of a complete endoscope, including other tendons and segments, have been omitted from FIG. **17**. Tension applied to a tendon cable is transferred across the entire segment, resulting in bending. By using a Bowden cable **310** whose sleeve **314** is attached to the base **322** of the segment and also fixed at the proximal actuator end **403**, only the intended segment **401** is bent by applying tension to the tendon **312**, and more proximal segments are unaffected. The tendon is placed in tension by the actuator **410**, which is shown, in this variation, as a motor pulling on the tendon cable **312**.

[0094] Linked control rings may provide the flexible structure needed to construct the steerable distal portion and the controllable segments. Two examples of the types of control rings that may be utilized are shown. The first is shown in FIG. **18A** which shows a vertebra-type control ring that forms the controllable segments of the present invention. FIG. **18A** shows an end view of a single vertebra. Each ring-shaped vertebra **501** can define a central channel or aperture **504** or

apertures that can collectively form the internal lumen of the device as previously described. The vertebrae may have two pairs of hinges; the first pair **506** projecting perpendicularly from a first face of the vertebra and a second pair **508**, located 90° around the circumference from the first pair, projecting perpendicularly away from the face of the vertebra on a second face of the vertebra opposite to the first face. The hinges shown in FIGS. **18A** and **18B** are tab-shaped, however other shapes may also be used.

[0095] The vertebra control ring in FIG. **18A** is shown with three holes **510** through the edge of the vertebra that may act, e.g., as attachment sites for the tendon cable **312** if the vertebra is the most distal vertebra in a segment, or as a throughway for a tendon cable that can actuate the segment in which the vertebra is used. These holes **510** can also be used to attach the sleeve of the Bowden-type tendon cable **314** when the vertebra is the most proximal control disk in a segment. Alternatively, rather than a hole **510**, the attachment sites could be a recess or other specialized shape. Although FIG. **18A** shows three holes **510**, the number of holes may depend upon the number of tendons used to control the segment to which the vertebra belongs. Since the holes **510** may be used as attachment sites for the tendons, there are as many holes as there are tendons controlling the segment.

[0096] The outer edge of the vertebra in FIG. **18A** may be scalloped to provide spaces **512** for tendon housings of tendons that control more distal segments and bypass the vertebra. These tendon bypass spaces preferably conform to the outer diameter of the tendons used. The number of tendon bypass spaces **512** may vary depending on the number of tendons. Also, the orientation of the tendon bypass spaces may be varied if it is desirable to vary the way in which the bypassing tendons are wound around the endoscope. For example, the spaces **512'** in FIG. **18C** are oriented at an angle relative to the longitudinal axis of the vertebra, allowing the tendons to wind around the body of the endoscope as they project proximally. Furthermore, the tendon bypass spaces could be lubricated or composed of a lubricious material in order to facilitate free movement of the bypassing tendons across the segment, and prevent interference between the bending of the segment and the bypassing tendons.

[0097] FIGS. **18B** and **18C** show side views of the same vertebra as FIG. **18A**. The two pairs of hinge joints **508**, **506** are shown. Hinge joints **508**, **506** are preferably located 90° apart and extend axially so that the hinge joints can pivotally mate with hinge joints from adjacent vertebrae. This mating **520** with adjacent vertebrae is more clearly seen in FIG. **18C**. These hinges can be joined, pinned, or connected through the holes **525** as shown **522**. Alternatively, hinges may also be made from materials utilizing, e.g., thermoplastics, shape memory alloys, etc. Once hinged, each vertebra can rotate relative to an adjoining vertebra in one axis. However, because vertebrae are hinged to each other in directions alternating by 90°, an assembly of multiple vertebrae is able to move in virtually any direction. The greater the number of vertebrae joined in this manner, the greater the range of motion. In one embodiment, two to ten vertebrae are used to comprise one segment, achieving a length of around 4 cm to 10 cm per segment. The dimensions of both the vertebrae and the hinge joints can be varied, e.g., longer hinge joints will have a greater bending radius when joined to another vertebra. Furthermore, the number of vertebrae per segment can vary, e.g. more than ten vertebrae could be used.

[0098] FIGS. 18D and 18E show another variation of a vertebra in sectional and perspective views, respectively. In FIGS. 18D and 18E, the tendons that bypass the segment may be contained within the body of the vertebra in a tendon bypassing space 550 rather than along the outer edge of the vertebra as shown in FIG. 18A. The vertebra of FIGS. 18D and 18E show four tendon bypassing spaces 550, and each space can hold approximately fifteen bypassing tendon sleeves. The number, shape and sizes of the tendon bypassing spaces can be varied. For example, a vertebra could have two tendon bypassing spaces that could hold more than thirty-five tendon sleeves. Moreover, the tendon bypassing space could also be located on the inside of the central aperture or lumen of the vertebra 504.

[0099] Although FIG. 18D shows tendon sleeves holding only a single tendon cable 560, more than one tendon cable could be contained in a tendon housing or sleeve. For example, if three tendons articulate a segment, all three tendons could be contained in a single tendon housing. Such a combined tendon housing could further utilize lubrication to accommodate independent movement by individual tendon cables and/or could be divided into compartments that isolate the tendons within the housing.

[0100] FIG. 18E also shows a perspective view of the hinge joints 506, 508 that can pivotally mate with pairs of hinge joints from adjacent vertebrae. Although FIGS. 18A and 18B shows two pairs of hinge joints projecting axially, a single hinge joint on each face of the vertebra could also be used. Moreover, as long as the hinge joints can pivotally mate with adjacent vertebrae, the hinge joints can be located at different radial locations from the center of the vertebra. For example, the pairs of hinge joints shown in FIGS. 18A to 18C are located closer to the center of the vertebra than the hinge joints in FIGS. 18D and 18E.

[0101] FIG. 19A and 19B illustrate a second variation of control ring. The variation shown in the figure utilizes a flexible backbone 601 preferably made of a material that is relatively non-compressible and non-extensible, to which control rings 602 are attached at intervals. This structure allows bending in a continuous curve in any desired direction. FIG. 19A shows a side view of one controllable segment of this variation with the outer layers removed to show the control rings and backbone. Multiple control rings 602 may be attached to the flexible backbone at regular intervals. Fewer or more control rings could be used to comprise a single segment depending upon the desired degree of articulation. The tendon cable 312 attaches to the most distal control ring of the segment 604. As with the vertebra-type variation, this central backbone embodiment is shown actuated by three tendons 310 attached at sites equally spaced around the edge of the most distal control ring of the segment 604. The tendon cables controlling the segment 312 pass through spaces or holes 610 defined in the control rings 602 through which they are free to move. These holes 610 could be lubricated, lined with a lubricious material or the control rings 602 may be composed of some lubricious material to facilitate cable motion through the holes 610. The tendon sleeve preferably attaches at a location 614 to the most proximal control ring in the segment 612. When a tendon 312 is placed under tension, this force is distributed along the entire segment. Because the inner tendon cable 312 is freely slidable within the tendon sleeve 314, and the tendon sleeve is fixed at both ends of the tendon 614, pulling on the tendon cable causes bending only in the selected segment.

[0102] FIG. 19A also shows the first control ring of a more proximal segment 604'. The tendons controlling the more distal segment may pass over the outside of the more proximal segments as they project proximally to the actuators. The outer edge of the control rings for the flexible backbone embodiment are shown with channels or tendon bypassing spaces 616 for bypassing tendons, as seen in FIG. 19B. As with the vertebra-type control rings, these tendon bypassing spaces could also be located within the control ring, for example, in an enclosed tendon bypassing space.

[0103] FIG. 19B shows an end view of control ring 602 which may be used with the flexible backbone embodiment of the endoscope. The center of the control ring contains a channel through which the flexible backbone 601 can be attached. A number of additional channels through the control ring 618 are also shown. These channels can be aligned with channels in neighboring control rings to form an internal lumen or channel for a fiber optic imaging bundle, illumination fibers, etc. as discussed above. Moreover, adjacent control rings may be spaced adjacently to one another at uniform or various distances depending upon the desired degree of bending or control. FIG. 19B shows three equally spaced holes 610 through which the tendon cable can pass; these holes 610 could also be used as attachment sites for the tendon cable, e.g., when the control ring is the most distal control ring in the segment 604, or for the tendon cable sleeve, e.g., when the control ring is the most proximal control ring in the segment 612. These holes 610 could be shaped specifically to receive either the tendon end or the tendon sleeve. Control rings of other designs could be used for different regions of the segment, or for different segments.

[0104] FIGS. 20A to 20C illustrate a variation of the tendon driven endoscope navigating a tortuous path. The path 701 is shown in FIG. 20A. This pathway may represent a portion of colon, for example. In FIG. 20A, the distal tip of the device 704 approaches the designated bend. FIG. 20B shows the distal tip being steered 705 to assume the appropriate curve. This steering could be performed manually by the user, e.g., a doctor, or automatically using an automatic detection method that could determine the proximity of the walls of the pathway. As described, the bending of the steerable tip is performed by placing tension on the tendon, or combination of tendons that results in the appropriate bending.

[0105] The device is then advanced again in FIG. 20C; as it is advanced, the selected curve is propagated down the proximal length of the endoscope, so that the bend of the endoscope remains in relatively the same position with respect to the pathway 701. This prevents excessive contact with the walls, and allows the endoscope to move more easily along the tortuous pathway 701. The endoscope is in continuous communication with the motion controller, and the motion controller can monitor the location of the endoscope within the pathway, e.g., depth of insertion, as well as the selected bends or curves that define the pathway of the endoscope. Depth can be determined by, e.g., the axial motion transducer 49 previously described, or by more direct measurement techniques. Likewise, the shape of each segment could be determined by the tension applied to the tendons, or by direct measurement, such as direct measurement of displacement of the tendon cables. The motion controller can propagate the selected shape of a segment at a specified location, or depth, within the body, e.g., by setting the lengths of the sides of more proximal segments equal to the corresponding lengths of the sides of more distal segments as the device is moved

distally. The controller can also use this information to automatically steer the body of the endoscope, or for other purposes, e.g. creating a virtual map of the endoscope pathway for analytic use.

[0106] In addition to measuring tendon displacement, the motion controller can also adjust for tendon stretch or compression. For example, the motion controller can control the “slack” in the tendons, particularly in tendons that are not actively under tension or compression. Allowing slack in inactive tendons reduces the amount of force that is required to articulate more proximal segments. In one variation, the umbilicus at the distal end of the endoscope may contain space to allow slack in individual tendons.

[0107] The bending and advancing process can be done in a stepwise or continuous manner. If stepwise, e.g., as the tendon is advanced by a segment length, the next proximal segment **706** is bent to the same shape as the previous segment or distal steerable portion. A more continuous process could also result by bending the segment incrementally as the tendon is advanced. This could be accomplished by the computer control, for example when the segments are smaller than the navigated curve.

[0108] Controllable segments, including the steerable distal portion, can be selected to have different dimensions, e.g., different diameters or lengths, even within the same endoscope. Segments of different dimensions may be desirable because of considerations of space, flexibility and method of bending. For example, the more segments in an endoscope, the further it can be steered within a body cavity; however, more segments require more tendons to control the segments. FIGS. **21** and **22** illustrate two variations on tendon driven endoscopes.

[0109] FIG. **21** shows a tendon driven endoscope variation that has segments **800** of differing diameters. More distal segments may have a smaller diameter **803** than more proximal segments, e.g., **802**, **801**. The diameter of a typical endoscope could decrease from, e.g., 20 mm, down to, e.g., 12.5 mm. The endoscope shown in FIG. **21** appears telescoped, as the diameter decreases distally in a stepwise manner. This design would be responsive, e.g., to internal body structures that become increasingly narrow. This design would also help accommodate bypassing tendons from more distal segments as they proceed towards the proximal actuators because of the larger diameter of the more proximal segments. FIG. **21** shows four differently sized segments; however, virtually any number of differently sized segments could be used. Moreover, although the segments appear stepped in this variation, the outer surface may be gently tapered to present a smooth outer surface decreasing in diameter towards the distal end.

[0110] FIG. **22** shows another variation of the tendon driven endoscope that has segments of different lengths. Using segments of different lengths may require fewer overall segments **900** to construct an equivalent length of articulatable endoscope. As shown in FIG. **22**, more proximal segments **901** are increasingly longer than more distal, e.g., **902**, **903**, segments. For example, segment length could be decreased from 20 cm at a proximal segment down to 6 cm at a distal most segment. The lengths may be decreased incrementally segment to segment by a constant factor; alternatively, lengths may be decreased geometrically, exponentially, or arbitrarily depending upon the desired articulation. In practice this results in an “averaging” of curves by more distal segments as bends and turns are propagated proximally. In order to accomplish this, the motion controller may be

configured to accommodate the differently sized segments accordingly. Alternatively, endoscopes could be comprised of a combination of segments of different length and thickness, depending upon the application.

[0111] The tendons that articulate the segments are in mechanical communication with the actuators. However, it may be desirable to have the insertable distal portion of the endoscope be removable from the actuators and controller, e.g., for cleaning or disinfecting. A quick-release mechanism between the proximal end of the endoscope and the actuators is an efficient way to achieve an endoscope that is easily removable, replaceable or interchangeable. For example, the proximal ends of the tendons can be organized to allow predictable attachment to corresponding actuators. The tendons may be organized into a bundle, array, or rack. This organization could also provide other advantages to the endoscope, such as allowing active or passive control of the tendon slack. Furthermore, the proximal ends of each tendon can be modified to allow attachment and manipulation, e.g., the ends of the tendons may be held in a specially configured sheath or casing.

[0112] While the present invention has been described herein with respect to the exemplary embodiments and the best mode for practicing the invention, it will be apparent to one of ordinary skill in the art that many modifications, improvements and subcombinations of the various embodiments, adaptations and variations can be made to the invention without departing from the spirit and scope thereof.

1. An endoscopic device for approximating tissue within a hollow body organ, comprising: an elongated body having a plurality of articulatable segments and a steerable distal portion, wherein each of the segments are configurable to assume a selected shape along an arbitrary path when the elongated body is advanced distally or proximally; a first tissue approximation component positioned about the elongated body, wherein the first component is adapted to radially expand and adhere a first region of tissue to a plurality of tissue gripping regions circumferentially located about the first component; and a second tissue approximation component positioned about the elongated body proximally of the first component, wherein the second component is adapted to radially expand and adhere a second region of tissue to a plurality of tissue gripping regions circumferentially located about the second component, wherein the first component and the second component are adapted to approximate and securely fasten the first region to the second region of tissue.

2. The endoscopic device of claim 1 wherein the first and the second tissue approximation components each comprise a radially expandable ring.

3. The endoscopic device of claim 1 wherein the first and the second tissue approximation components each comprise a radially expandable balloon.

4. The endoscopic device of claim 1 wherein the plurality of tissue gripping regions on each of the first and the second tissue approximation components comprise vacuum ports.

5. The endoscopic device of claim 1 wherein the plurality of tissue gripping regions on each of the first and the second tissue approximation components comprise retractable fasteners.

6. The endoscopic device of claim 5 wherein the retractable fasteners are selected from the group consisting of needles, hooks, and barbs.

7. The endoscopic device of claim 1 wherein the first tissue approximation component is adapted to slide longitudinally

towards the second tissue approximation component along at least a portion of the elongated body within rails or grooves defined along the elongated body such that the first region is adjacent to the second region of tissue.

8. The endoscopic device of claim 1 wherein the second tissue approximation component is adapted to slide longitudinally towards the first tissue approximation component along at least a portion of the elongated body within rails or grooves defined along the elongated body such that the first region is adjacent to the second region of tissue.

9. The endoscopic device of claim 1 wherein the first and the second tissue approximation components are each adapted to slide longitudinally towards one another along at least a portion of the elongated body within rails or grooves defined along the elongated body such that the first region is adjacent to the second region of tissue.

10. The endoscopic device of claim 1 wherein the first or the second tissue approximation component contains a plurality of fasteners adapted to fasten the first region to the second region of tissue.

11. The endoscopic device of claim 10 wherein the fasteners are selected from the group consisting of staples, clips, screws, adhesives, sutures, and combinations thereof.

12. A method of endoscopically approximating tissue within a hollow body organ, comprising:

positioning an elongated body adjacent to a portion of tissue to be excised from the hollow body organ;

releasably fastening a first region of tissue circumferentially about a first tissue approximation component and a second region of tissue circumferentially about a second tissue approximation component such that the tissue to be excised is positioned between the first and the second tissue approximation components;

removing the tissue to be excised from between the first and the second tissue approximation components;

approximating the first and the second tissue approximation components such that the first and the second regions of tissue are adjacent to one another; and fastening the first region of tissue to the second region of tissue.

13. The method of claim 12 wherein the first and the second regions of tissue are releasably fastened to the first and the second tissue approximation components, respectively, via a vacuum force.

14. The method of claim 12 wherein the first and the second regions of tissue are releasably fastened to the first and the second tissue approximation components, respectively, via a plurality of fasteners.

15. The method of claim 14 wherein the fasteners are retractable.

16. The method of claim 12 wherein releasably fastening comprises radially expanding the first and the second tissue approximation components into contact with the first and the second regions of tissue, respectively.

17. The method of claim 12 wherein removing the tissue to be excised comprises laparoscopically excising the tissue from between the first and the second tissue approximation components.

18. The method of claim 12 wherein approximating the first and the second tissue approximation components comprises longitudinally translating the first and the second tissue approximation components towards one another along the elongated body.

19. The method of claim 12 wherein fastening the first region of tissue to the second region of tissue comprises stapling or suturing the first region to the second region via the first or the second tissue approximation component.

20. The method of claim 12 further comprising radially reducing a diameter of the first and the second tissue approximation components.

* * * * *

专利名称(译)	用于内窥镜结肠切除术的装置和方法		
公开(公告)号	US20130116712A1	公开(公告)日	2013-05-09
申请号	US13/729602	申请日	2012-12-28
[标]申请(专利权)人(译)	直观外科手术操作公司		
当前申请(专利权)人(译)	Intuitive Surgical公司运营, INC.		
[标]发明人	BELSON AMIR		
发明人	BELSON, AMIR		
IPC分类号	A61B17/11 A61B17/32 A61B A61B1/00 A61B1/31 A61B17/00 A61B17/08 A61B17/115 A61B17/22		
CPC分类号	A61B1/00147 A61B1/0055 A61B1/0058 A61B1/31 A61B17/1114 A61B2019/5259 A61B2017/00557 A61B2017/1103 A61B2017/22034 A61B2017/22054 A61B2017/003 A61B2034/2059 A61B17/00234 A61B17/1155 A61B2017/00296 A61B2017/00314 A61B2017/00349 A61B2017/00353 A61B2017/1132		
优先权	60/347674 2002-01-09 US		
其他公开文献	US8696694		
外部链接	Espacenet USPTO		

摘要(译)

本文描述了用于内窥镜结肠切除术的装置和方法。具有第一和第二组织接近装置的结肠切除装置安装在彼此分离的结肠镜上。在结肠切除术装置的展开期间,结肠的患病部分位于组织接近装置之间。组织接近装置径向扩张,使得它们在与结肠的疾病部分相邻的两个部位处接触并抓握结肠壁。将病变部分与网膜分离,并使用腹腔镜进行横切,或将其拉入结肠镜中以便以后取出。然后在结肠镜上朝向彼此推动组织接近装置,以使结肠的两个自由边缘接近在一起,在那里它们使用组织接近装置作为外科吻合器固定到彼此,以产生端对端吻合。

