



US 20150119646A1


(19) **United States**(12) **Patent Application Publication**
Sharma et al.(10) **Pub. No.: US 2015/0119646 A1**(43) **Pub. Date: Apr. 30, 2015**(54) **LEAD IMPLANTATION METHOD**(71) Applicant: **EndoStim, Inc.**, St. Louis, MO (US)(72) Inventors: **Virender K. Sharma**, Paradise Valley, AZ (US); **Shai Policker**, Redmond, WA (US); **Paul V. Goode**, Round Rock, TX (US); **Ofer Glasberg**, Zichron Ya'akov (IL)(21) Appl. No.: **14/548,855**(22) Filed: **Nov. 20, 2014****Related U.S. Application Data**

(63) Continuation-in-part of application No. 13/602,184, filed on Sep. 2, 2012.

(60) Provisional application No. 61/906,825, filed on Nov. 20, 2013, provisional application No. 61/530,781, filed on Sep. 2, 2011.

Publication Classification(51) **Int. Cl.****A61N 1/05** (2006.01)**A61N 1/08** (2006.01)**A61B 1/06** (2006.01)**A61B 1/313** (2006.01)(52) **U.S. Cl.**CPC **A61N 1/0509** (2013.01); **A61B 1/3132** (2013.01); **A61N 1/08** (2013.01); **A61B 1/06** (2013.01); **A61N 2001/083** (2013.01)(57) **ABSTRACT**

A method of laparoscopically implanting an electrically stimulating lead proximate the lower esophageal sphincter (LES) of a patient includes delivering the lead through a port of a laparoscope inserted into the abdominal cavity of the patient through an incision in the abdominal wall. The stimulating electrode is implanted in or proximate the muscularis layer of the lower esophageal wall to treat esophageal reflux disease (GERD). The lead includes a needle and suture at its distal end for pulling the electrode into the muscular wall of the LES. Clips are applied to the suture attached to the distal end of the lead to prevent retrograde movement of the electrode. The lead also includes an anchoring member for anchoring the portion of the lead proximal to the electrode. The method and lead used with the method allow the surgeon to work within the confined anatomy present at the gastro-esophageal junction and prevents backwards movement and dislodgment of the electrode. The implantation procedure can be combined with a hiatal hernia repair to repair the hernia and prevent recurrence of a hiatal hernia.

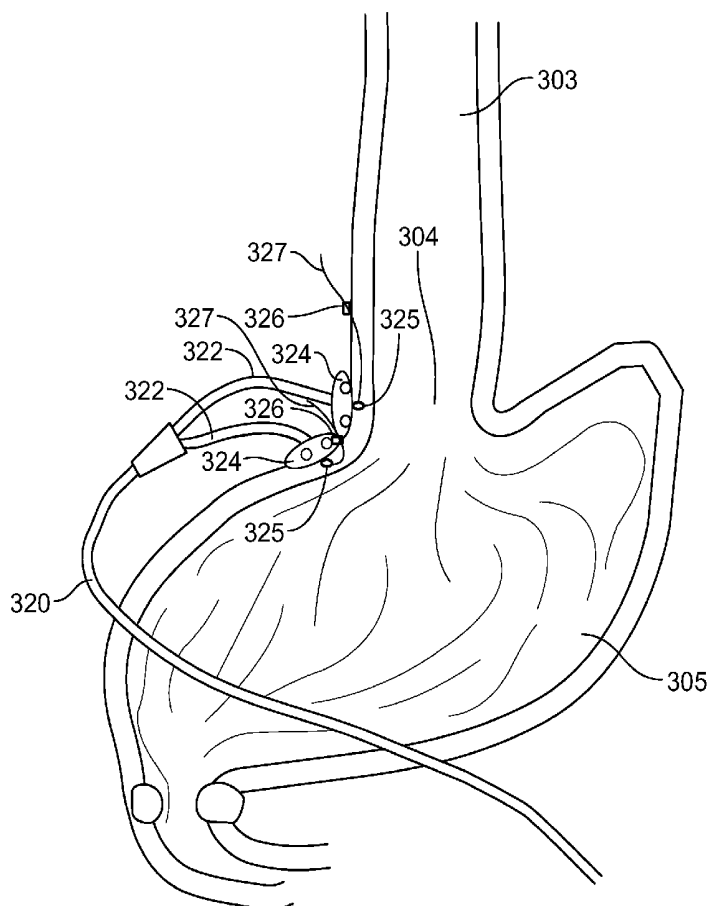

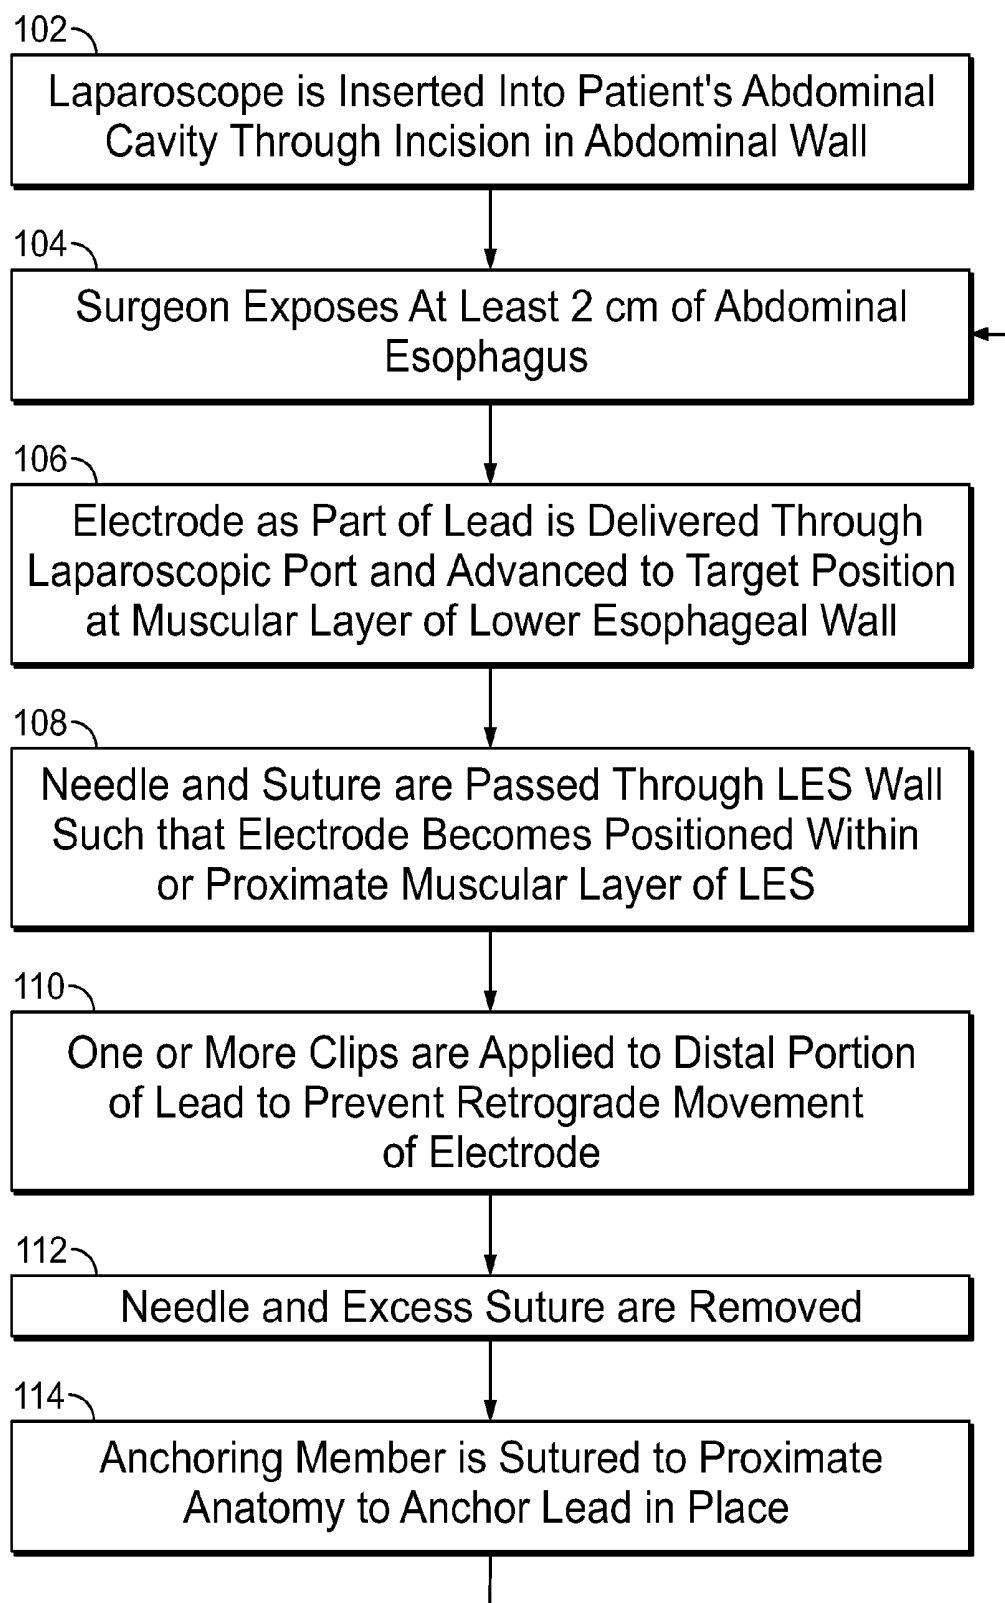


FIG. 1A

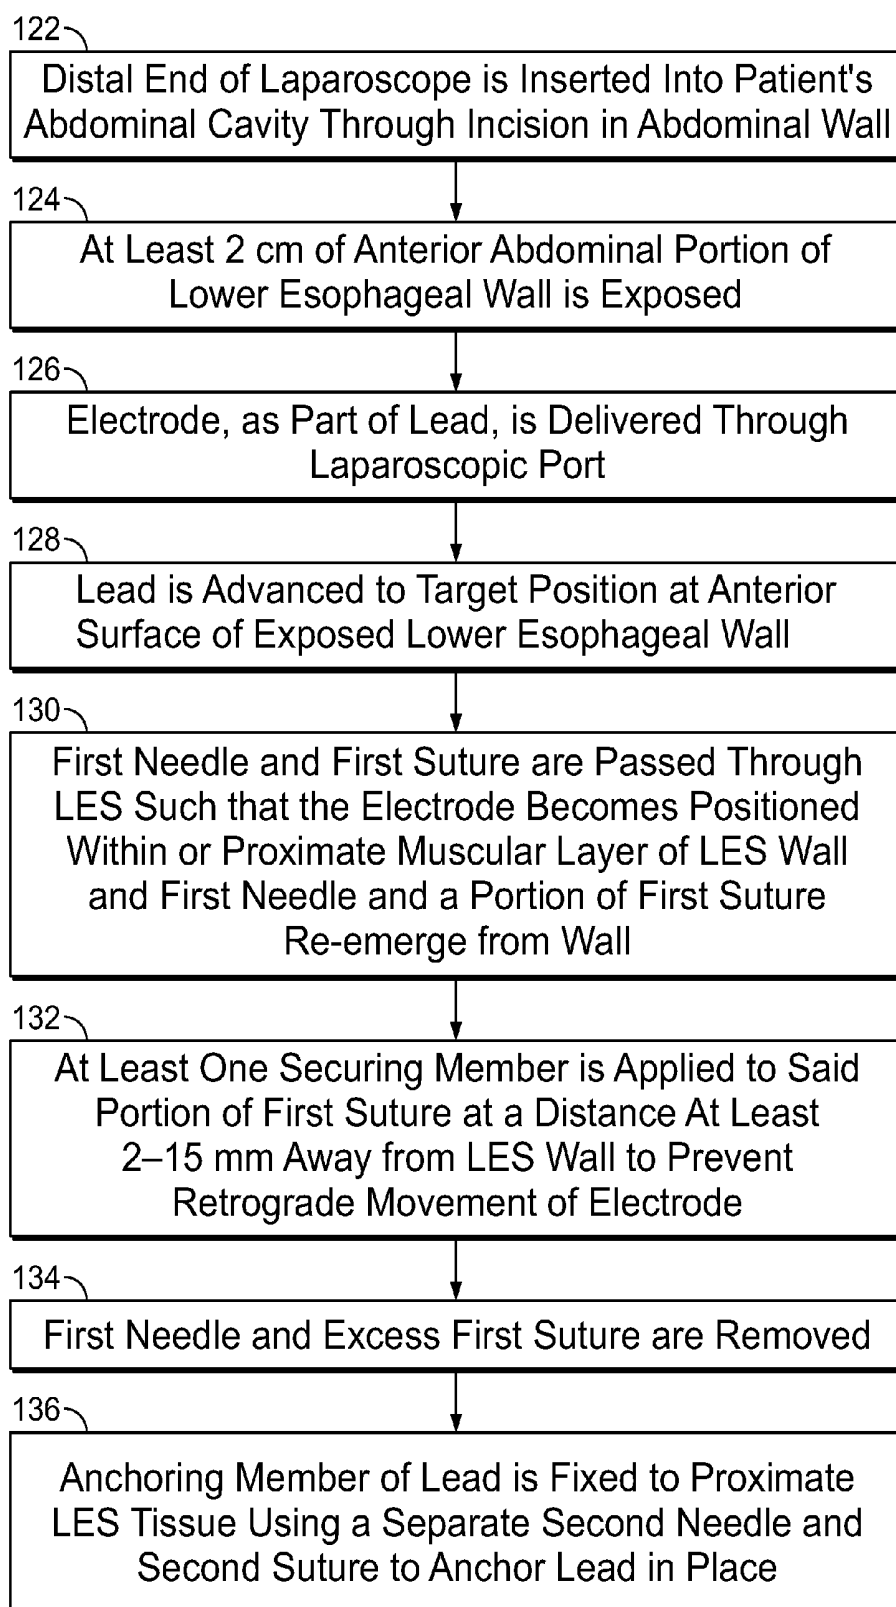


FIG. 1B

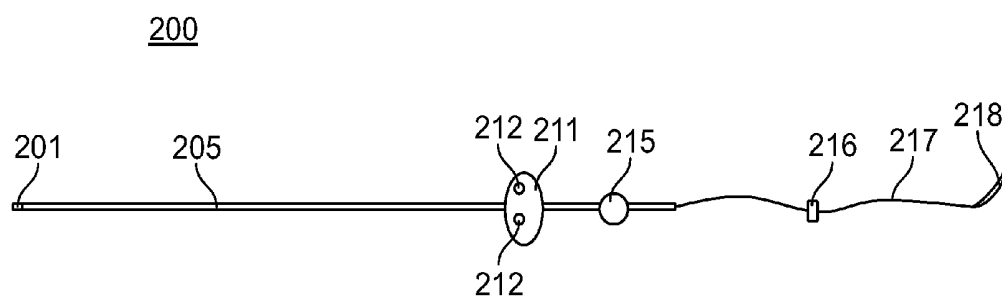


FIG. 2A

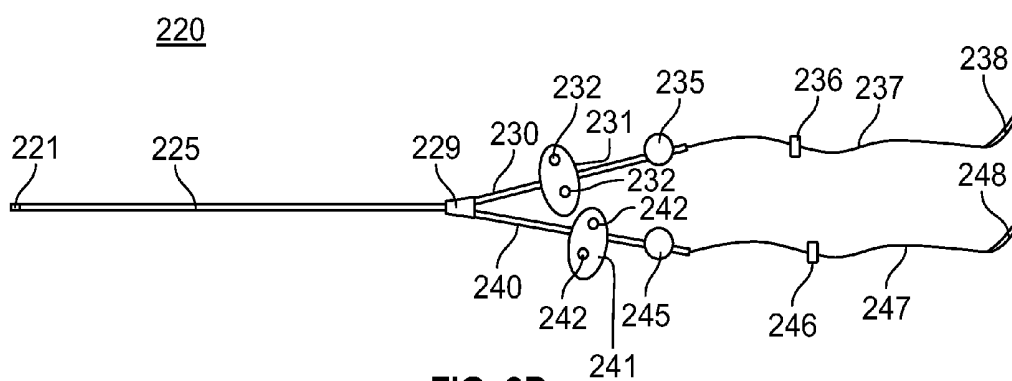


FIG. 2B

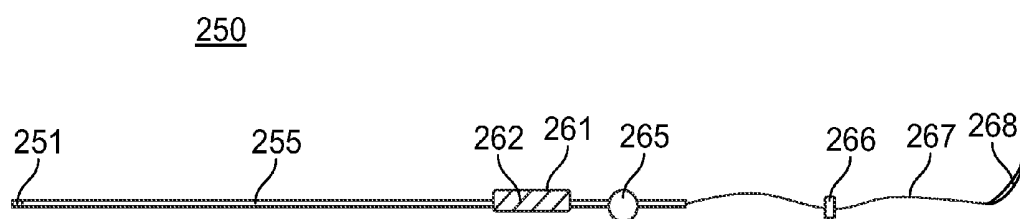


FIG. 2C

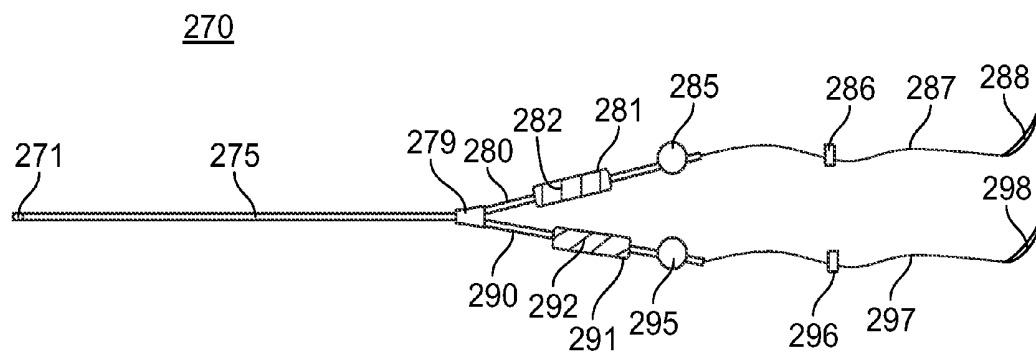
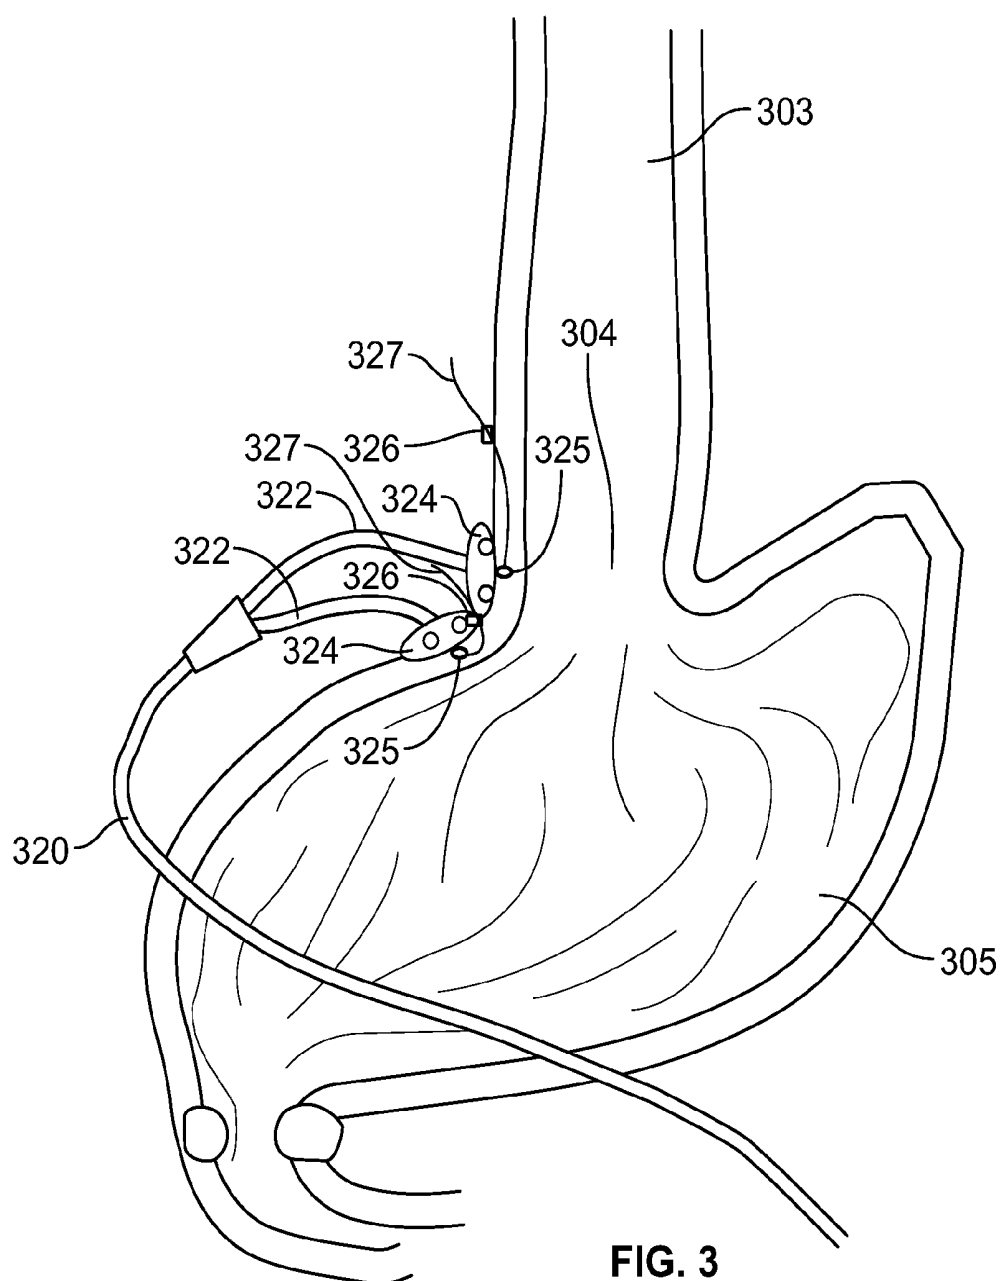
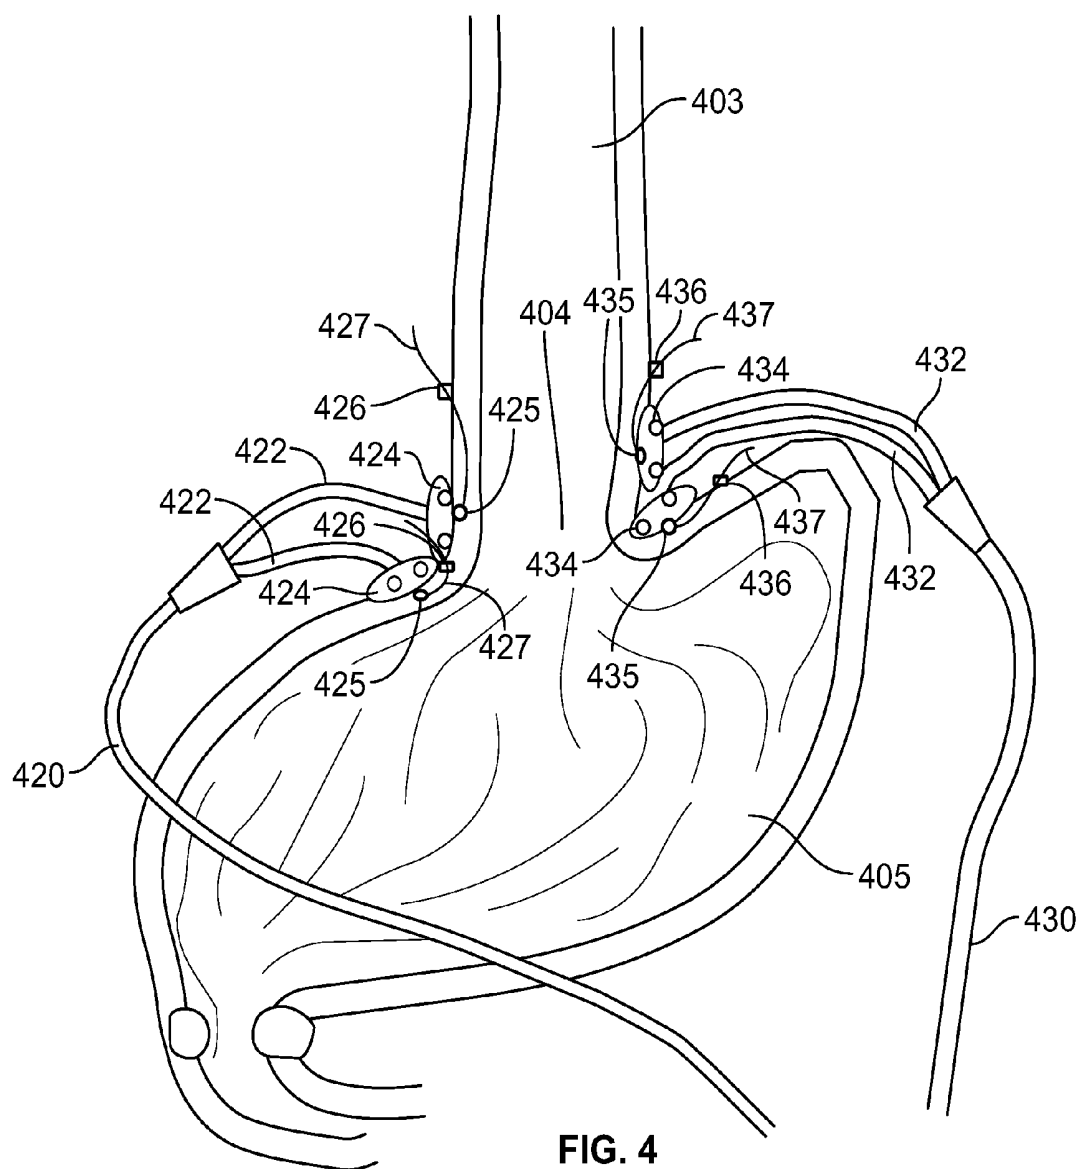


FIG. 2D





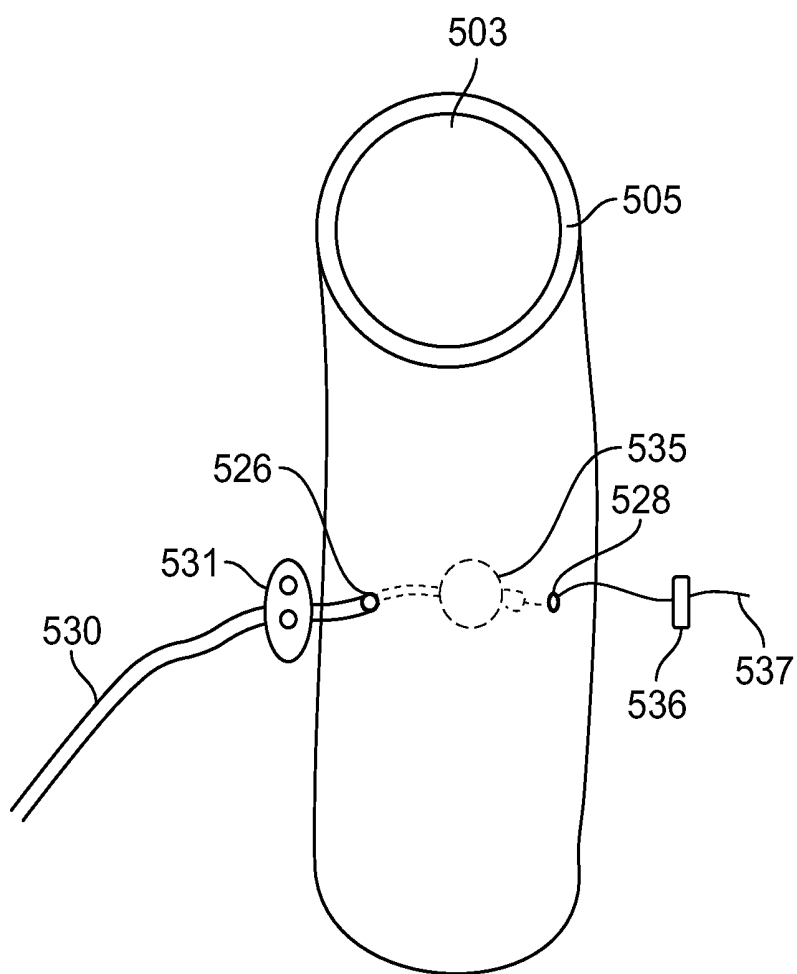


FIG. 5

LEAD IMPLANTATION METHOD

CROSS-REFERENCE

[0001] The present application relies on U.S. Provisional Patent Application No. 61/906,825, entitled “Lead Implantation Method” and filed on Nov. 20, 2013, for priority.

[0002] The present application is also a continuation-in-part application of U.S. patent application Ser. No. 13/602,184, entitled “Endoscopic Lead Implantation Method” and filed on Sep. 2, 2012, which relies on U.S. Provisional Patent Application No. 61/530,781, of the same title and filed on Sep. 2, 2011, for priority.

[0003] The present application is also related to U.S. patent application Ser. No. 14/191,085, entitled “Implantable Electrical Stimulation Leads” and filed on Feb. 26, 2014, which relies on U.S. Provisional Patent Application No. 61/769,732, of the same title and filed on Feb. 26, 2013, for priority.

[0004] All of the aforementioned applications are herein incorporated by reference in their entirety.

FIELD

[0005] The present specification relates generally to the electrical stimulation of biological tissues to provide therapy for physiological disorders. More particularly, the present specification relates to a method of laparoscopic implantation of electrically conductive leads proximate the lower esophageal sphincter (LES).

BACKGROUND

[0006] Electrical stimulation of nerves and surrounding tissue is used to treat a variety of conditions. For example, electrical stimulation can be used to restore partial function to limbs or organs following traumatic injury. Electrical stimulation can also be used to reduce pain. Specifically, electrical stimulation can be used to treat disorders associated with the gastrointestinal (GI) system, such as, obesity and gastroesophageal reflux disease (GERD).

[0007] Obesity is a common condition and a major public health problem in developed nations including the United States of America. As of 2009, more than two thirds of American adults, approximately 127 million people, were either overweight or obese. Data suggest that 300,000 Americans die prematurely from obesity-related complications each year. Many children in the United States are also either overweight or obese. Hence, the overall number of overweight Americans is expected to rise in the future. It has been estimated that obesity costs the United States approximately \$100 billion annually in direct and indirect health care expenses and in lost productivity. This trend is also apparent in many other developed countries.

[0008] For adults, the body mass index (BMI) is used to determine if one is overweight or obese. A person's BMI is calculated by multiplying body weight in pounds by 703 and then dividing the total by height in inches squared. A person's BMI is expressed as kilograms per meter squared. An adult is considered overweight if his or her BMI is between 25 and 30 kg/m². Obesity is defined as possessing a BMI between 30 and 40 kg/m². A BMI greater than 30 kg/m² is associated with significant co-morbidities. Morbid obesity is defined as possessing either a body weight more than 100 pounds greater than ideal or a body mass index (BMI) greater than 40 kg/m². Approximately 5% of the U.S. population meets at least one of the criteria for morbid obesity. Morbid obesity is associ-

ated with many diseases and disorders including, for example: diabetes; hypertension; heart attacks; strokes; dyslipidemia; sleep apnea; pickwickian syndrome; asthma; lower back and disc disease; weight-bearing osteoarthritis of the hips, knees, ankles and feet; thrombophlebitis and pulmonary emboli; intertriginous dermatitis; urinary stress incontinence; gastroesophageal reflux disease (GERD); gallstones; and, sclerosis and carcinoma of the liver. In women, infertility, cancer of the uterus, and cancer of the breast are also associated with morbid obesity. Taken together, the diseases associated with morbid obesity markedly reduce the odds of attaining an average lifespan. The sequelae raise annual mortality in affected people by a factor of 10 or more.

[0009] Gastro-esophageal reflux disease (GERD) is another common health problem and is expensive to manage in both primary and secondary care settings. This condition results from exposure of esophageal mucosa to gastric acid as the acid refluxes from the stomach into the esophagus. The acid damages the esophageal mucosa resulting in heartburn, ulcers, bleeding, and scarring, and long term complications such as Barrett's esophagus (pre-cancerous esophageal lining) and adeno-cancer of the esophagus.

[0010] Gastric electrical stimulation (GES) is aimed at treating both obesity and GERD. GES employs an implantable, pacemaker-like device to deliver low-level electrical stimulation to the gastrointestinal tract. For obesity, GES operates by disrupting the motility cycle and/or stimulating the enteric nervous system, thereby increasing the duration of satiety experienced by the patient. The procedure involves the surgeon suturing electrical leads to the outer lining of the stomach wall. The leads are then connected to the device, which is implanted just under the skin in the abdomen. Using an external programmer that communicates with the device, the surgeon establishes the level of electrical stimulation appropriate for the patient. The Abiliti® implantable gastric stimulation device, manufactured by IntraPace, is currently available in Europe for treatment of obesity.

[0011] In another example, Medtronic offers for sale and use the Enterra™ Therapy, which is indicated for the treatment of chronic nausea and vomiting associated with gastroparesis when conventional drug therapies are not effective. The Enterra™ Therapy uses mild electrical pulses to stimulate the stomach. According to Medtronic, this electrical stimulation helps control the symptoms associated with gastroparesis, including nausea and vomiting.

[0012] Electrical stimulation has also been suggested for use in the treatment of GERD, wherein the stimulation is supplied to the lower esophageal sphincter (LES). For example, in U.S. Pat. No. 6,901,295, assigned to the applicant of the current invention, “A method and apparatus for electrical stimulation of the lower esophageal sphincter (LES) is provided. Electrode sets are placed in the esophagus in an arrangement that induce contractions of the LES by electrical stimulation of the surrounding tissue and nerves. The electrical stimulus is applied by a pulse generator for periods of varying duration and varying frequency so as to produce the desired contractions. The treatment may be short-term or may continue throughout the life of the patient in order to achieve the desired therapeutic effect. The stimulating electrode sets can be used either alone or in conjunction with electrodes that sense esophageal peristalsis. The electrode sets can be placed endoscopically, surgically or radiologically.” The referenced invention relies on sensing certain physiological changes in the esophagus, such as changes in esophageal pH, to detect

acid reflux. Once a change in esophageal pH is recognized, the system generates an electrical stimulation in an attempt to instantaneously close the LES and abort the episode of acid reflux. U.S. Pat. No. 6,901,295 is hereby incorporated by reference in its entirety.

[0013] Typically, the leads for LES stimulation are implanted in the lower esophageal wall using a laparoscopic approach. Lead implantation in the LES poses unique challenges different from implantation in any other part of the human body, including the stomach. One of the major challenges is the scarcity of space proximate the LES for the surgeon to maneuver. Another major challenge is exposure of the muscle tissue of the LES. The LES muscle tissue is covered by overlying fat tissue and the location of the gastroesophageal junction is difficult to identify. In addition, in a patient having a pre-existing gastrointestinal structural disorder, such as, a hiatal hernia, proper lead placement can be difficult to achieve. Often times the electrodes of the leads are not optimally positioned proximate the target tissue. Also, if a lead is not properly anchored, it can become dislodged and therapy will become ineffective. Therefore, what is needed is an effective and accurate method of implantation within the confined anatomy of the LES wherein the lead is securely fixed and/or anchored proximate the target tissue. What is also needed is an effective and accurate method of lead implantation that includes a hiatal closure as part of the implantation method.

SUMMARY

[0014] The present specification discloses a method of laparoscopically implanting at least one electrically conductive electrode, as part of an electrically conductive lead, proximate a lower esophageal sphincter (LES) of a patient, said method comprising the steps of: inserting the distal end of a laparoscope into an abdominal cavity of a patient through an incision in an abdominal wall of said patient; surgically exposing at least 2 cm of an anterior abdominal portion of a lower esophageal wall of said patient; delivering said electrically conductive electrode through a port on said laparoscope, wherein said lead comprises an elongate metal body having a proximal end and a distal end, said elongate body being covered in an electrically insulating material, said proximal end having a connector for connection to an implantable pulse generator and said distal end including said at least one exposed electrode and an anchoring member, said lead further comprising a first suture having a first end and a second end opposite said first end, wherein said first end is attached to a said distal end of said lead body and a first needle is attached to said second end; advancing said electrically conductive lead to a target position at an anterior surface of said exposed lower esophageal wall; using said first needle and said first suture to pass said electrode through said LES such that said exposed electrode comes to rest within or proximate a muscular layer of a wall of said LES and said first needle and a portion of said second end of said first suture re-emerge from said wall of said LES; applying at least one securing member to said portion of said second end of said suture at a distance at least 2-15 mm away from said wall of said LES; removing said first needle and excess first suture; and, fixing said anchoring member to proximate LES tissue by using a separate second needle to couple a second suture to said anchoring member.

[0015] The at least one securing member may comprise any one of a clip, suture, u-clip, or anchor.

[0016] Optionally, the at least one anchoring member comprises a butterfly tab having at least one opening and said step of coupling said second suture to said anchoring member comprises passing said second suture through said at least one opening. Optionally, the at least one anchoring member comprises a suture sleeve having at least one groove and said step of coupling said second suture to said anchoring member comprises passing said second suture around said at least one groove.

[0017] Optionally, the first suture comprises a barbed micro-architecture of a suture.

[0018] Optionally, the method further comprises the steps of repeating the steps of surgically exposing at least 2 cm of an anterior abdominal portion of a lower esophageal wall of said patient through fixing said anchoring member to proximate LES tissue by using a separate second needle to couple a second suture to said anchoring member to implant additional electrically stimulating leads.

[0019] The method further may comprise the step of using an external device to assess the impedance between each electrode to ensure accurate positioning of the electrodes within the muscularis layer of the lower esophageal wall.

[0020] The method further may comprise the step of endoscopically illuminating the lower esophageal sphincter to identify the appropriate location for dissection and placement of said at least one electrode.

[0021] The method may further comprise the step of endoscopically assessing lead placement to rule out perforation of said lower esophageal wall. The method may also further comprise the step of repositioning said lead if perforation of said lower esophageal wall has occurred.

[0022] Optionally, the implantation is combined with a hiatal hernia repair procedure to repair a hiatal hernia and prevent recurrence of a hiatal hernia in said patient.

[0023] The method may further comprise the steps of: exposing a diaphragmatic crura of said patient; and, applying at least one suture to said diaphragmatic crura.

[0024] The method may further comprise the step of attaching said proximal end of said lead to an implanted pulse generator.

[0025] The method may be used to implant a lead to treat esophageal disorders such as gastroesophageal reflux disease (GERD), achalasia, and esophageal dysmotility.

[0026] The present specification also discloses an electrically conductive lead for implanting proximate a lower esophageal sphincter of a patient, said lead comprising: an electrically conductive, elongate body having a proximal end and a distal end and covered in an insulating material; a connector at said proximal end for connecting to a pulse generator; at least one anchoring member positioned proximate said distal end of said lead body; at least one electrode positioned proximate said distal end of said lead body and distal to said at least one anchoring member; at least one length of suture having a first end and a second end opposite said first end, wherein said first end is attached to said distal end of said lead body; a needle attached to said second end of said at least one length of suture; and, at least one securing member removably applicable to said at least one length of suture.

[0027] Optionally, the elongate body comprises a straight metal wire. Optionally, the elongate body comprises a coiled metal wire. Optionally, the elongate body comprises a conducting cable.

[0028] The at least one securing member may comprise any one of a clip, suture, u-clip, or anchor.

[0029] Optionally, the at least one anchoring member comprises a butterfly tab having at least one opening. Optionally, the at least one anchoring member comprises a suture sleeve having at least one groove.

[0030] The present specification also discloses an electrically conductive lead for implanting proximate a lower esophageal sphincter of a patient, said lead comprising: an electrically conductive, elongate body having a proximal end and a distal end and covered in an insulating material; a connector at said proximal end for connecting to a pulse generator; a splitting element at said distal end for splitting said elongate body into two or more branches; two or more branches emanating from said splitting element, each branch having a proximal end and a distal end; at least one anchoring member positioned proximate said proximal end of each branch; at least one electrode positioned proximate said distal end of each branch; at least one length of suture having a first end and a second end opposite said first end, wherein said first end is attached to said distal end of each branch; a needle attached to said second end of said at least one length of suture; and, at least one securing member removably applicable to said at least one length of suture.

[0031] Optionally, the elongate body comprises a straight metal wire. Optionally, the elongate body comprises a coiled metal wire. Optionally, the elongate body comprises a conducting cable.

[0032] The at least one securing member may comprise any one of a clip, suture, u-clip, or anchor.

[0033] Optionally, the at least one anchoring member comprises a butterfly tab having at least one opening. Optionally, the at least one anchoring member comprises a suture sleeve having at least one groove.

[0034] The aforementioned and other embodiments of the present invention shall be described in greater depth in the drawings and detailed description provided below.

BRIEF DESCRIPTION OF THE DRAWINGS

[0035] These and other features and advantages of the present invention will be further appreciated, as they become better understood by reference to the detailed description when considered in connection with the accompanying drawings:

[0036] FIG. 1A is a flowchart illustrating the steps involved in one embodiment of a method of laparoscopically implanting at least one stimulating lead in the muscularis of a lower esophageal wall of a patient;

[0037] FIG. 1B is a flowchart illustrating the steps involved in another embodiment of a method of laparoscopically implanting at least one stimulating lead in the muscular layer of a lower esophageal wall of a patient;

[0038] FIG. 2A is an illustration of an in-line electrically stimulating lead in accordance with one embodiment of the present specification;

[0039] FIG. 2B is an illustration of bipolar electrically stimulating lead in accordance with one embodiment of the present specification;

[0040] FIG. 2C is an illustration of an in-line electrically stimulating lead in accordance with another embodiment of the present specification;

[0041] FIG. 2D is an illustration of bipolar electrically stimulating lead in accordance with another embodiment of the present specification;

[0042] FIG. 3 is an illustration of the anatomical area proximate the lower esophageal sphincter (LES) of a patient depicting a single bipolar electrically stimulating lead that has been laparoscopically implanted using a method in accordance with one embodiment of the present specification;

[0043] FIG. 4 is an illustration of the anatomical area proximate the lower esophageal sphincter (LES) of a patient depicting two bipolar electrically stimulating leads that have been laparoscopically implanted using a method in accordance with one embodiment of the present specification; and,

[0044] FIG. 5 is a close up illustration of a distal end portion of an electrically stimulating lead depicting an electrode implanted within the muscular wall of the LES in accordance with one embodiment of the present specification.

DETAILED DESCRIPTION

[0045] The present specification discloses a method of laparoscopically implanting one or more stimulating leads in the esophageal wall to be used with an electrical stimulation system directed toward treating at least one gastrointestinal disorder, such as gastroesophageal reflux disease (GERD). In various embodiments, the stimulating lead is defined as a lead having one or more stimulating electrodes. In one embodiment, the stimulating lead comprises an in-line lead having one stimulating electrode. In one embodiment, the stimulating lead comprises a bipolar lead having two stimulating electrodes. It should be appreciated that a stimulating lead having any number of stimulating electrodes can be used with the method of the present specification. The distal end of a laparoscope is inserted into the abdominal cavity of a patient through an incision in the patient's abdominal wall. A surgeon then exposes at least 2 cm of the abdominal esophagus. At least one stimulating lead is delivered through a laparoscopic port and the electrode(s) are advanced to a target position at the muscular portion of the esophageal wall. The lead comprises an elongate metal wire with an electrically insulating covering having a proximal end and a distal end. With respect to the lead, distal is used to describe the end that is positioned proximate the target tissue and proximal is used to describe the end that is connected to an implantable pulse generator (IPG), as described below.

[0046] In one embodiment, the elongate body comprises a straight metal wire. In another embodiment, the elongate body comprises a coiled metal wire. In yet another embodiment, the elongate body comprises a conducting cable. In one embodiment, the distal end of the lead comprises at least one branch or distal end wherein each branch or distal end includes an anchoring member and an exposed electrode. In various embodiments, the anchoring member comprises a butterfly tab with at least one opening. In one embodiment, each butterfly tab comprises two openings. In other embodiments, the anchoring mechanism comprises a suture sleeve with at least one groove. A length of non-absorbable suture (monofilament or multifilament) continues from the distal end of each branch or distal end of the lead and includes a stitching needle at its end opposite its attachment to the distal end of the branch. In one embodiment, the suture is comprised of nylon. In one embodiment, the suture comprises a barbed micro-architecture of a suture, such as the Covidien V-Lock™. The needle and suture are used to pass the exposed electrode into the muscularis of the LES. The electrode comes to rest within or proximate the muscularis of the LES. In various other embodiments, the electrode is positioned within or proximate the anterior gastric wall, gastric cardia or within

3 cm of the LES. For example, in one embodiment, the lead includes two electrodes wherein one is positioned within or proximate the anterior gastric wall and the other is positioned within or proximate the gastric cardia or the LES. The needle and suture re-emerge out of the LES wall. A portion of the lead proximate the distal end of the suture has at least one clip or securing member applied to it to prevent retrograde movement and/or dislodgement. In various embodiments, the clip is comprised of a metal. In one embodiment, the clip is titanium. In various embodiments, the clip is applied to the suture at least 2-15 mm away from the LES wall to allow for some slack between the clip and the LES. The clip acts as a distal stopper to prevent the electrode from sliding too far backwards and out of the LES muscular layer. The slack is provided to allow for gentle distension of surrounding GI tissues as a food bolus passes, thereby reducing the chances for tension or injury. The needle and excess suture are then removed. A separate needle with suture is used to stitch through the openings in the butterfly tab or around the grooves in the suture sleeve to hold the lead in place. During the application of these anchoring sutures to the butterfly tab or suture sleeve, the implanted electrode tends to move backwards, resulting in the first use of the clip in preventing backwards slippage of the electrode. The proximal end of the lead is then connected to an IPG that has been implanted in a subcutaneous pocket in the patient's abdomen.

[0047] In various embodiments, a length of up to 10 cm of suture remains distal to the clip. This provides several advantages. In the event that the clips are not tightly applied to the suture, they will tend to slide. It is preferable if the clips slide along the suture and not get lost in the abdominal cavity. A short suture end is stiff and traumatic to the surrounding organs, such as, the liver. A short suture end can easily puncture and damage surrounding tissues. In addition, a long suture is beneficial during removal of the lead. The long suture end acts as a locator of the distal end of the electrode and clip. Cutting the clip from the distal end of the suture is the first step in removing the electrode.

[0048] In one embodiment, a first stimulating lead is implanted with its electrodes positioned in the muscularis of the lower esophageal wall on the anterior surface of the esophagus. In various embodiments, additional stimulating leads are implanted into the muscularis of the lower esophageal wall in additional anatomical locations proximate the lower esophageal sphincter (LES).

[0049] In various embodiments, the method described above further includes using an external device to assess the impedance between each electrode implanted to ensure accurate positioning of the electrodes within the muscular layer of the target anatomy.

[0050] In many patients suffering from GERD, the anatomical area of the LES is "pushed up" or raised due to chronic esophagitis. In various embodiments, a light source is inserted endoscopically into these patients and the light is directed toward the anterior surface of the LES to assist with implantation by helping to direct the surgeon to the LES while minimizing the dissection.

[0051] In various embodiments, the method described above further includes endoscopically assessing lead placement to rule out perforation of the gastric wall or lower esophageal wall. If perforation is detected, the leads are withdrawn and repositioned.

[0052] In various embodiments, the method described above is used to implant leads in a patient having a hiatal

hernia. The method further includes surgical dissection and exposure of the anatomy proximate the diaphragmatic crura. The surgeon surgically dissects the surrounding anatomy from the laparoscopic approach to implant the electrodes. In one embodiment, an area including at least 100 mm² of esophageal tissue proximate the LES is used for implantation. In various embodiments, the methods above are performed during a hiatal hernia repair to repair said hernia and prevent recurrence of a hiatal hernia as described with reference to co-pending U.S. patent application Ser. No. 13/975,162, filed Aug. 23, 2013 and entitled "Device and Implantation System for Electrical Stimulation of Biological Systems", which is hereby incorporated by reference in its entirety.

[0053] The present invention is directed toward multiple embodiments. The following disclosure is provided in order to enable a person having ordinary skill in the art to practice the invention. Language used in this specification should not be interpreted as a general disavowal of any one specific embodiment or used to limit the claims beyond the meaning of the terms used therein. The general principles defined herein may be applied to other embodiments and applications without departing from the spirit and scope of the invention. Also, the terminology and phraseology used is for the purpose of describing exemplary embodiments and should not be considered limiting. Thus, the present invention is to be accorded the widest scope encompassing numerous alternatives, modifications and equivalents consistent with the principles and features disclosed. For purpose of clarity, details relating to technical material that is known in the technical fields related to the invention have not been described in detail so as not to unnecessarily obscure the present invention.

[0054] FIG. 1A is a flowchart illustrating the steps involved in one embodiment of a method of laparoscopically implanting at least one stimulating lead in the muscularis of the lower esophageal wall of a patient. At step **102**, a laparoscope is inserted with its distal end into a patient's abdominal cavity through an incision in the patient's abdominal wall. A surgeon exposes at least 2 cm of abdominal esophagus at step **104**. An electrode, as part of a stimulating lead, is then delivered through a laparoscopic port and advanced to a target position at the muscular layer of the lower esophageal wall at step **106**. Then, at step **108**, a needle and suture attached to the distal end of the lead is used to pass through the LES wall and pull the electrode into the muscular layer of the LES. One or more clips are then applied to the suture of the lead at a position proximate the lead's distal end to prevent retrograde movement of the electrode at step **110**. The needle and excess suture are removed at step **112**. Then, at step **114**, using a separate needle and suture, an anchoring member is sutured to the proximate anatomy to anchor the lead in place. In some embodiments, the anchoring member comprises a butterfly tab with at least one opening and the separate needle is used to pass the separate suture through the proximate anatomy and the at least one opening to secure the anchoring member in place. In other embodiments, the anchoring member comprises a suture sleeve with at least one groove and the separate needle is used to pass the separate suture through the proximate anatomy and around the groove to secure the anchoring member in place. Step **112** is typically performed prior to step **114** due to the traumatic nature of the needle. Optionally, in another embodiment, the original needle and suture are removed after securing the anchoring member. If additional leads are to be implanted, steps **104** through **114** are then repeated for each additional lead.

[0055] FIG. 1B is a flowchart illustrating the steps involved in another embodiment of a method of laparoscopically implanting at least one stimulating lead in the muscular layer of a lower esophageal wall of a patient. At step 122, the distal end of a laparoscope is inserted into a patient's abdominal cavity through an incision in an abdominal wall of the patient. At least 2 cm of an anterior abdominal portion of a lower esophageal wall is then exposed at step 124. At least one electrode, as part of an electrically conducting lead, is delivered through a port on the laparoscope at step 126. At step 128, the lead is advanced to a target position at an anterior surface of the exposed lower esophageal wall. Then, at step 130, a first needle and first suture of the lead are passed through the LES such that the electrode becomes positioned within or proximate the muscular layer of the LES wall and the first needle and a portion of the first suture re-emerge from the wall. At least one securing member is then applied to the portion of the first suture at a distance at least 2-15 mm away from the LES wall to prevent retrograde movement of the electrode at step 132. The first needle and excess first suture are then removed at step 134. At step 136, an anchoring member on the lead is fixed to the proximate LES tissue using a separate second needle and second suture to anchor the lead in place.

[0056] FIG. 2A is an illustration of an in-line electrically stimulating lead 200 in accordance with one embodiment of the present specification. The lead 200 includes an elongate lead body 205 having a proximal end and a distal end. A connector 201 is positioned at the proximal end for connection to an implantable pulse generator. The distal end includes an anchoring member 211 and an electrode 215. Referring to FIG. 2A, the anchoring member 211 comprises a butterfly tab having two openings 212 for anchoring to body tissues after implantation. In other embodiments, the butterfly tab includes one or three or more openings. A suture 217 having a proximal end and a distal end is attached to the distal end of the lead body 205. A needle 218 is attached to the distal end of the suture 217. After implantation, at least one clip 216 is applied to the suture 217 emerging from the LES wall to prevent backward movement of the electrode 215.

[0057] FIG. 2B is an illustration of bipolar electrically stimulating lead 220 in accordance with one embodiment of the present specification. The lead 220 includes an elongate lead body 225 having a proximal end and a distal end. A connector 221 is positioned at the proximal end for connection to an implantable pulse generator. The distal end comprises a bifurcation point 229 that splits the lead body 225 into two branches or distal ends 230, 240. Each branch 230, 240 comprises an anchoring member 231, 241 and an electrode 235, 245. Referring to FIG. 2B, each anchoring member 231, 241 comprises a butterfly tab having two openings 232, 242 for anchoring to body tissues after implantation. In other embodiments, each butterfly tab includes one or three or more openings. A suture 237, 247 having a proximal end and a distal end is attached to the distal end of each branch 230, 240 of the lead 220. A needle 238, 248 is attached to the distal end of each suture 237, 247. After implantation, at least one clip 236, 246 is applied to each suture 237, 247 emerging from the LES wall to prevent backward movement of each electrode 235, 245.

[0058] FIG. 2C is an illustration of an in-line electrically stimulating lead 250 in accordance with another embodiment of the present specification. The lead 250 includes an elongate lead body 255 having a proximal end and a distal end. A

connector 251 is positioned at the proximal end for connection to an implantable pulse generator. The distal end includes an anchoring member 261 and an electrode 265. Referring to FIG. 2C, the anchoring member 261 comprises a suture sleeve having a groove 262 for anchoring to body tissues after implantation. In other embodiments, the suture sleeve includes more than one groove. A suture 267 having a proximal end and a distal end is attached to the distal end of the lead body 255. A needle 268 is attached to the distal end of the suture 267. After implantation, at least one clip 266 is applied to the suture 267 emerging from the LES wall to prevent backward movement of the electrode 265.

[0059] FIG. 2D is an illustration of bipolar electrically stimulating lead 270 in accordance with another embodiment of the present specification. The lead 270 includes an elongate lead body 275 having a proximal end and a distal end. A connector 271 is positioned at the proximal end for connection to an implantable pulse generator. The distal end comprises a bifurcation point 279 that splits the lead body 275 into two branches or distal ends 280, 290. Each branch 280, 290 comprises an anchoring member 281, 291 and an electrode 285, 295. Referring to FIG. 2D, each anchoring member 281, 291 comprises a suture sleeve having a groove 282, 292 for anchoring to body tissues after implantation. In other embodiments, each suture sleeve includes more than one groove. A suture 287, 297 having a proximal end and a distal end is attached to the distal end of each branch 280, 290 of the lead 270. A needle 288, 298 is attached to the distal end of each suture 287, 297. After implantation, at least one clip 286, 296 is applied to each suture 287, 297 emerging from the LES wall to prevent backward movement of each electrode 285, 295.

[0060] FIG. 3 is an illustration of the anatomical area proximate the lower esophageal sphincter (LES) 304 of a patient depicting a single bipolar electrically stimulating lead 320 that has been laparoscopically implanted using a method in accordance with one embodiment of the present specification. The anatomical area of the LES 304 is depicted at the junction between the esophagus 303 and the stomach 305. Each lead 320 comprises two branches 322 wherein each branch 322 includes a butterfly tab 324 and an exposed electrode 325. The lead 320 has been implanted such that its electrodes 325 are positioned on a first side of the esophagus 303 within the muscular layer proximate the LES 304. Extending from the distal end of each branch 322 are the suture 327 and clip 326 preventing backward movement of the electrode 325.

[0061] FIG. 4 is an illustration of the anatomical area proximate the lower esophageal sphincter (LES) 404 of a patient depicting two bipolar electrically stimulating leads 420, 430 that have been laparoscopically implanted using a method in accordance with one embodiment of the present specification. The anatomical area of the LES 404 is depicted at the junction between the esophagus 403 and the stomach 405. Each lead 420, 430 comprises two branches 422, 432 wherein each branch 422, 432 includes a butterfly tab 424, 434 and an exposed electrode 425, 435. A first lead 420 has been implanted such that its electrodes 425 are positioned on a first side of the esophagus 403 within the muscular layer proximate the LES 404. A second lead 430 has been implanted such that its electrodes 435 are positioned on a second side of the esophagus 403, away and distinct from said first side, within the muscular layer proximate the LES 404. Extending

from the distal end of each branch **422**, **432** are the suture **427**, **437** and clip **426**, **436** preventing backward movement of the electrode **425**, **435**.

[0062] FIG. 5 is a close up illustration of a distal end portion **530** of an electrically stimulating lead depicting an electrode **535** implanted within the muscular wall **505** of the LES **503** in accordance with one embodiment of the present specification. The distal end portion **530** of the lead includes a butterfly tab **531** for anchoring to nearby anatomy. The butterfly tab **531** is depicted positioned proximal to an insertion point **526** of the distal end portion **530** of the lead into the wall of the LES **503**. A suture **537** extends from the electrode **535** and emerges from the wall of the LES **503** at an exit point **528**. The suture **537** includes a clip **536** applied to its distal end. The clip **537** cannot re-enter the wall of the LES **503** at the exit point **528** and thereby prevents backwards slippage of the electrode **535** out the insertion point **526**. In one embodiment, anchoring of the distal end portion **530** of the lead with the butterfly tab **531** prevents slippage of the electrode **535** in the forward direction.

[0063] The above examples are merely illustrative of the many applications of the system of the present invention. Although only a few embodiments of the present invention have been described herein, it should be understood that the present invention might be embodied in many other specific forms without departing from the spirit or scope of the invention. Therefore, the present examples and embodiments are to be considered as illustrative and not restrictive, and the invention may be modified within the scope of the appended claims.

We claim:

1. A method of laparoscopically implanting at least one electrically conductive electrode, as part of an electrically conductive lead, proximate the lower esophageal sphincter (LES) of a patient, said method comprising the steps of:

inserting the distal end of a laparoscope into an abdominal cavity of a patient through an incision in an abdominal wall of said patient;

surgically exposing at least 2 cm of an anterior abdominal portion of a lower esophageal wall of said patient;

delivering said electrically conductive lead through a port on said laparoscope, wherein said lead comprises an elongate metal body having a proximal end and a distal end, said elongate body being covered in an electrically insulating material, said proximal end having a connector for connection to an implantable pulse generator and said distal end including said at least one exposed electrode and an anchoring member, said lead further comprising a first suture having a first end and a second end opposite said first end, wherein said first end is attached to said distal end of said lead body and a first needle is attached to said second end;

advancing said electrically conductive lead to a target position at an anterior surface of said exposed lower esophageal wall;

using said first needle and said first suture to pass said electrode through said LES such that said exposed electrode comes to rest within or proximate a muscular layer of a wall of said LES and said first needle and a portion of said second end of said first suture re-emerge from said wall of said LES;

applying at least one securing member to said portion of said second end of said suture at a distance at least 2-15 mm away from said wall of said LES;

removing said first needle and excess first suture; and, fixing said anchoring member to proximate LES tissue by using a separate second needle to couple a second suture to said anchoring member.

2. The method of claim 1, wherein said at least one securing member comprises any one of a clip, suture, u-clip, or anchor.

3. The method of claim 1, wherein said at least one anchoring member comprises a butterfly tab having at least one opening and said step of coupling said second suture to said anchoring member comprises passing said second suture through said at least one opening.

4. The method of claim 1, wherein said at least one anchoring member comprises a suture sleeve having at least one groove and said step of coupling said second suture to said anchoring member comprises passing said second suture around said at least one groove.

5. The method of claim 1, wherein said first suture comprises a barbed micro-architecture of a suture.

6. The method of claim 1, further comprising the steps of repeating the steps of surgically exposing at least 2 cm of an anterior abdominal portion of a lower esophageal wall of said patient through fixing said anchoring member to proximate LES tissue by using a separate second needle to couple a second suture to said anchoring member to implant additional electrically stimulating leads.

7. The method of claim 1, further comprising the step of using an external device to assess the impedance between each electrode to ensure accurate positioning of the electrodes within the muscularis layer of the lower esophageal wall.

8. The method of claim 1, further comprising the step of endoscopically illuminating the lower esophageal sphincter to identify the appropriate location for dissection and placement of said at least one electrode.

9. The method of claim 1, further comprising the step of endoscopically assessing lead placement to rule out perforation of said lower esophageal wall.

10. The method of claim 9, further comprising the step of repositioning said lead if perforation of said lower esophageal wall has occurred.

11. The method of claim 1, wherein said implantation is combined with a hiatal hernia repair procedure to repair a hiatal hernia and prevent recurrence of a hiatal hernia in said patient.

12. The method of claim 1, further comprising the steps of: exposing a diaphragmatic crura of said patient; and, applying at least one suture to said diaphragmatic crura.

13. The method of claim 1, further comprising the step of attaching said proximal end of said lead to an implanted pulse generator.

14. The method of claim 1, wherein said implanted lead is used to treat esophageal disorders such as gastroesophageal reflux disease (GERD), achalasia, and esophageal dysmotility.

15. An electrically conductive lead for implanting proximate a lower esophageal sphincter of a patient, said lead comprising:

an electrically conductive, elongate body having a proximal end and a distal end and covered in an insulating material;

a connector at said proximal end for connecting to a pulse generator;

at least one anchoring member positioned proximate said distal end of said lead body;

at least one electrode positioned proximate said distal end of said lead body and distal to said at least one anchoring member;

at least one length of suture having a first end and a second end opposite said first end, wherein said first end is attached to said distal end of said lead body;

a needle attached to said second end of said at least one length of suture; and,

at least one securing member removably applicable to said at least one length of suture.

16. The lead of claim 15, wherein said elongate body comprises a straight metal wire.

17. The lead of claim 15, wherein said elongate body comprises a coiled metal wire.

18. The lead of claim 15, wherein said elongate body comprises a conducting cable.

19. The lead of claim 15, wherein said at least one securing member comprises any one of a clip, suture, u-clip, or anchor.

20. The lead of claim 15, wherein said at least one anchoring member comprises a butterfly tab having at least one opening.

21. The lead of claim 15, wherein said at least one anchoring member comprises a suture sleeve having at least one groove.

22. An electrically conductive lead for implanting proximate a lower esophageal sphincter of a patient, said lead comprising:

an electrically conductive, elongate body having a proximal end and a distal end and covered in an insulating material;

a connector at said proximal end for connecting to a pulse generator;

a splitting element at said distal end for splitting said elongate body into two or more branches;

two or more branches emanating from said splitting element, each branch having a proximal end and a distal end;

at least one anchoring member positioned proximate said proximal end of each branch;

at least one electrode positioned proximate said distal end of each branch;

at least one length of suture having a first end and a second end opposite said first end, wherein said first end is attached to said distal end of each branch;

a needle attached to said second end of said at least one length of suture; and,

at least one securing member removably applicable to said at least one length of suture.

23. The lead of claim 22, wherein said elongate body comprises a straight metal wire.

24. The lead of claim 22, wherein said elongate body comprises a coiled metal wire.

25. The lead of claim 22, wherein said elongate body comprises a conducting cable.

26. The lead of claim 22, wherein said at least one securing member comprises any one of a clip, suture, u-clip, or anchor.

27. The lead of claim 22, wherein said at least one anchoring member comprises a butterfly tab having at least one opening.

28. The lead of claim 22, wherein said at least one anchoring member comprises a suture sleeve having at least one groove.

* * * * *

专利名称(译)	铅植入法		
公开(公告)号	US20150119646A1	公开(公告)日	2015-04-30
申请号	US14/548855	申请日	2014-11-20
[标]申请(专利权)人(译)	恩多斯蒂姆股份有限公司		
申请(专利权)人(译)	ENDOSTIM INC.		
当前申请(专利权)人(译)	ENDOSTIM INC.		
[标]发明人	SHARMA VIRENDER K POLICKER SHAI GOODE PAUL V GLASBERG OFER		
发明人	SHARMA, VIRENDER K. POLICKER, SHAI GOODE, PAUL V. GLASBERG, OFER		
IPC分类号	A61N1/05 A61N1/08 A61B1/06 A61B1/313		
CPC分类号	A61N1/0509 A61B1/3132 A61N2001/083 A61B1/06 A61N1/08 A61B17/0401 A61B2017/00818 A61B2017/00827 A61B2017/0417 A61N1/0517		
优先权	61/906825 2013-11-20 US 61/530781 2011-09-02 US		
其他公开文献	US9925367		
外部链接	Espacenet USPTO		

摘要(译)

一种在患者的下食道括约肌 (LES) 附近腹腔镜植入电刺激引线的方法包括通过腹壁中的切口将导线穿过插入患者腹腔的腹腔镜的端口。将刺激电极植入下食管壁的肌层中或附近以治疗食管反流病 (GERD)。引线包括在其远端的针和缝合线, 用于将电极拉入LES的肌肉壁。将夹子施加到连接到引线远端的缝合线上, 以防止电极逆行移动。引线还包括锚固构件, 用于将引线的一部分锚固在电极附近。该方法使用的方法和引线允许外科医生在胃食管连接处存在的受限解剖结构内工作并防止电极向后移动和移位。植入手术可以与食管裂孔疝修复相结合, 以修复疝气并防止食管裂孔疝的复发。

