



US 20160157698A1

(19) **United States**(12) **Patent Application Publication**
SHOLEV(10) **Pub. No.: US 2016/0157698 A1**(43) **Pub. Date: Jun. 9, 2016**(54) **DEVICE AND METHODS OF IMPROVING
LAPAROSCOPIC SURGERY***A61B 34/00* (2006.01)*A61B 1/313* (2006.01)(71) Applicant: **M.S.T. MEDICAL SURGERY
TECHNOLOGIES LTD., Nazereth (IL)**(52) **U.S. Cl.**CPC *A61B 1/00016* (2013.01); *A61B 1/00149*
(2013.01); *A61B 1/3132* (2013.01); *A61B*
1/00006 (2013.01); *A61B 17/00234* (2013.01);
A61B 34/25 (2016.02); *A61B 1/00045*
(2013.01); *A61B 2034/301* (2016.02)(72) Inventor: **Mordehai SHOLEV, Amikam (IL)**(21) Appl. No.: **15/046,862**(22) Filed: **Feb. 18, 2016****Related U.S. Application Data**

(63) Continuation of application No. 11/874,534, filed on Oct. 18, 2007, now Pat. No. 9,295,379, which is a continuation of application No. PCT/IL2006/000478, filed on Apr. 20, 2006.


(60) Provisional application No. 60/672,010, filed on Apr. 18, 2005, provisional application No. 60/705,199, filed on Aug. 4, 2005, provisional application No. 60/716,953, filed on Sep. 15, 2005, provisional application No. 60/716,951, filed on Sep. 15, 2005.

Publication Classification(51) **Int. Cl.***A61B 1/00* (2006.01)*A61B 17/00* (2006.01)

(57)

ABSTRACT

An improved interface between the surgeon and an endoscope system for laparoscopic surgery, holding a laparoscopic camera and/or controlling an automated endoscope assistant includes at least one wireless transmitter with at least one operating key, at least one wireless receiver, at least one conventional laparoscopy computerized system loaded with conventional surgical instrument spatial location software, and conventional automated assistant maneuvering software, software loaded onto the conventional laparoscopy system that enables a visual response to the depression of at least one key on the wireless transmitter as well as an interface with the conventional automated assistant maneuvering software so as to achieve movement of the endoscope, and at least one video screen.

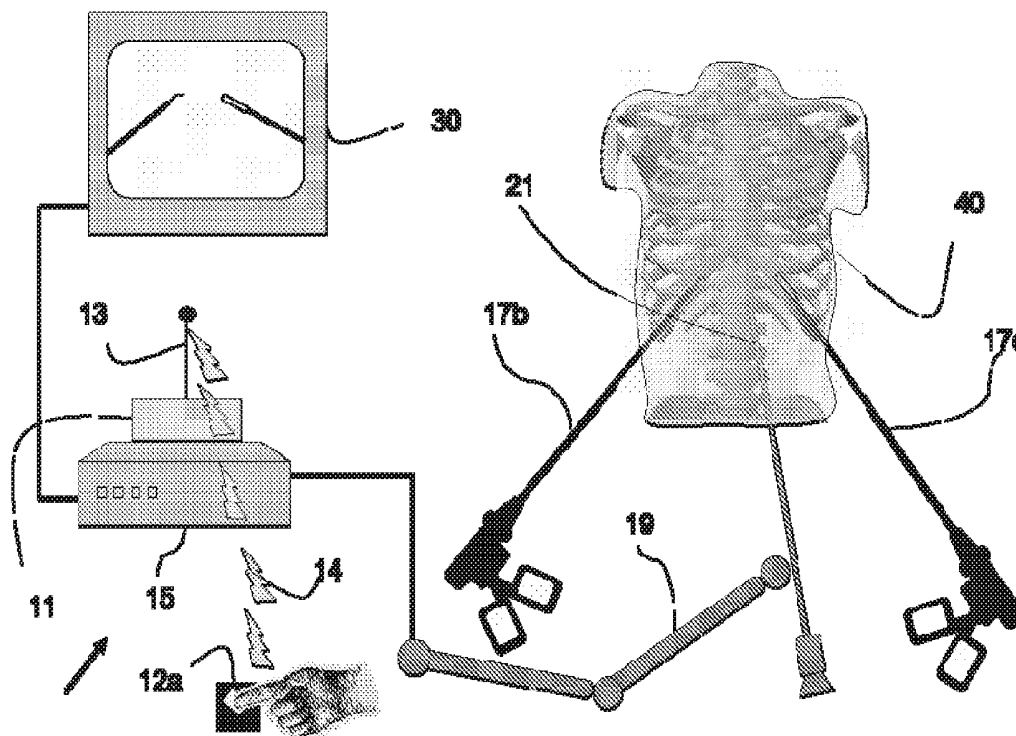

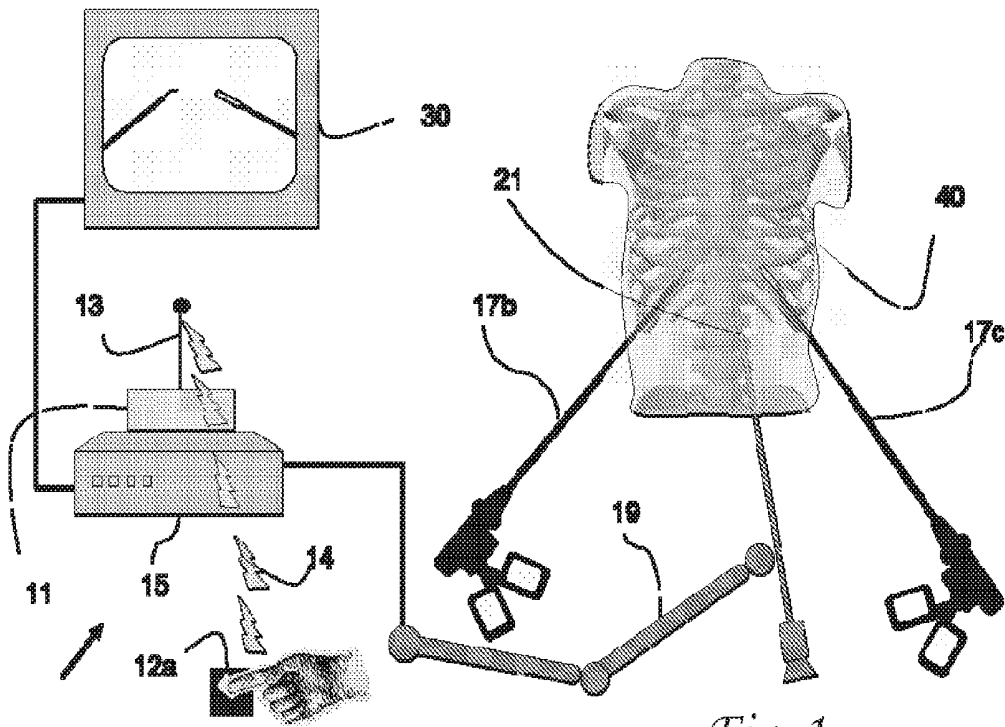


Fig. 1

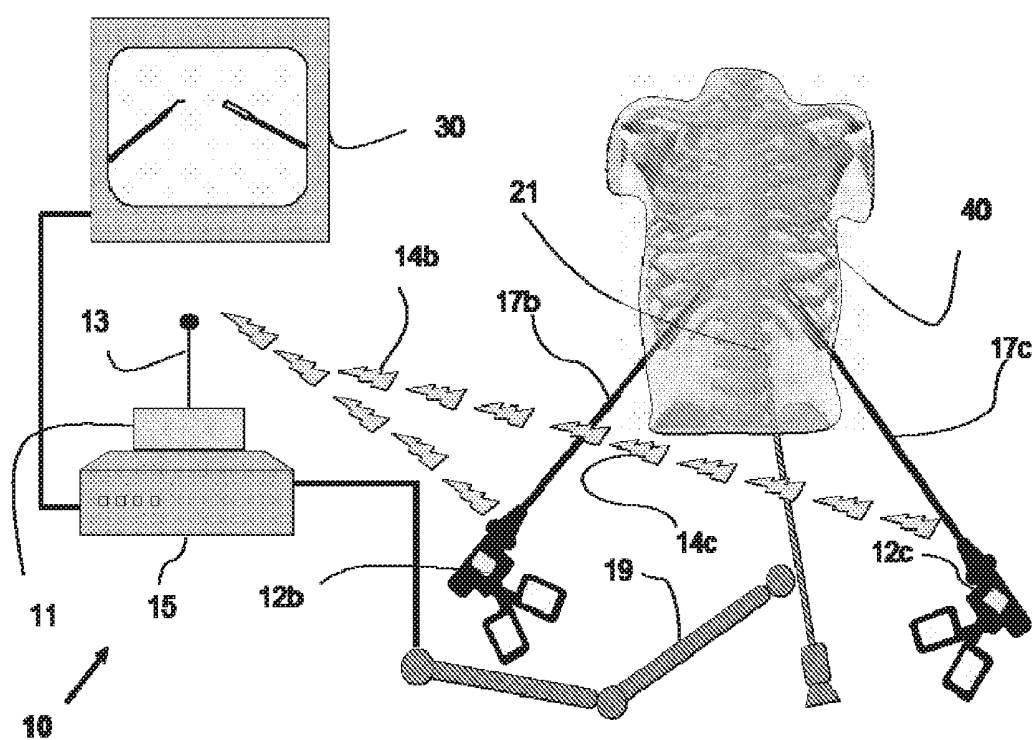


Fig. 2

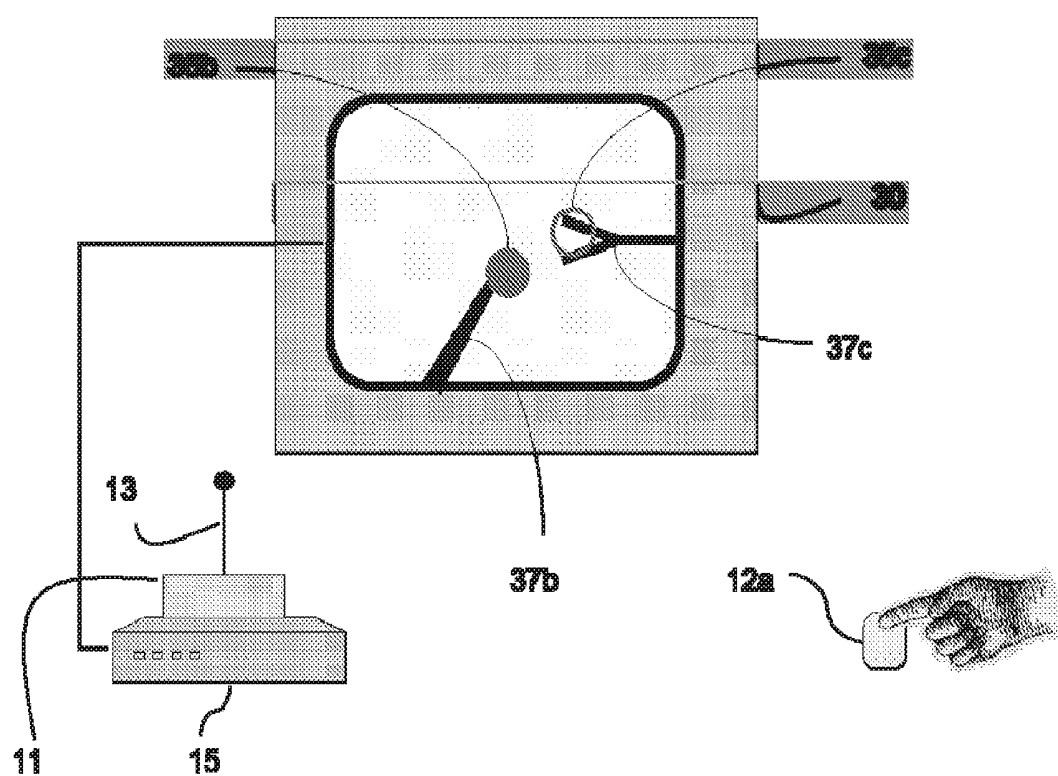


Fig. 3

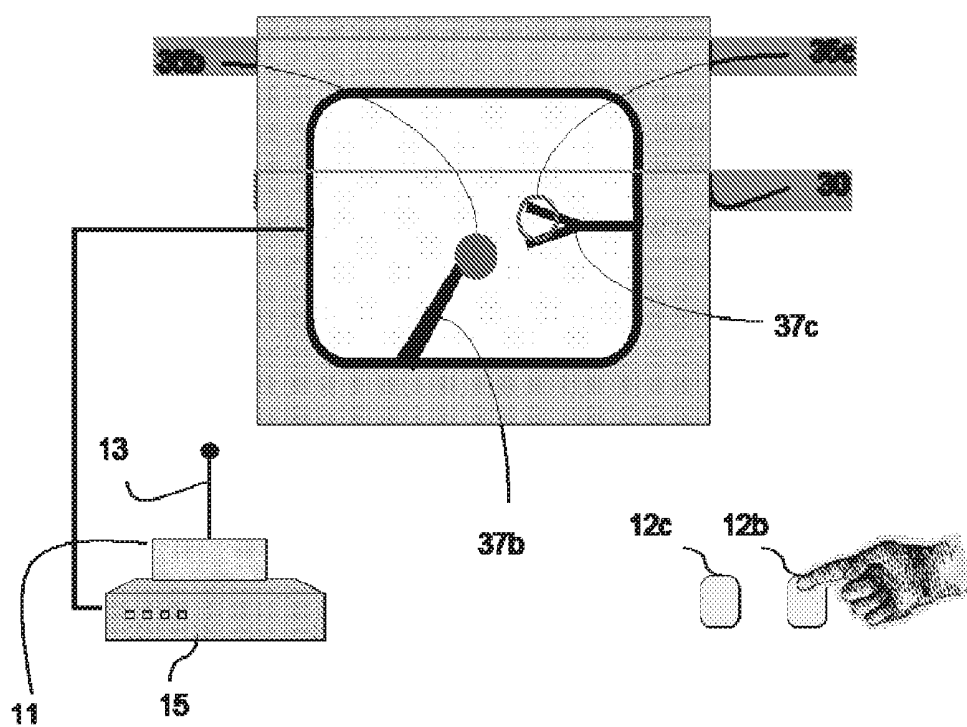


Fig. 4

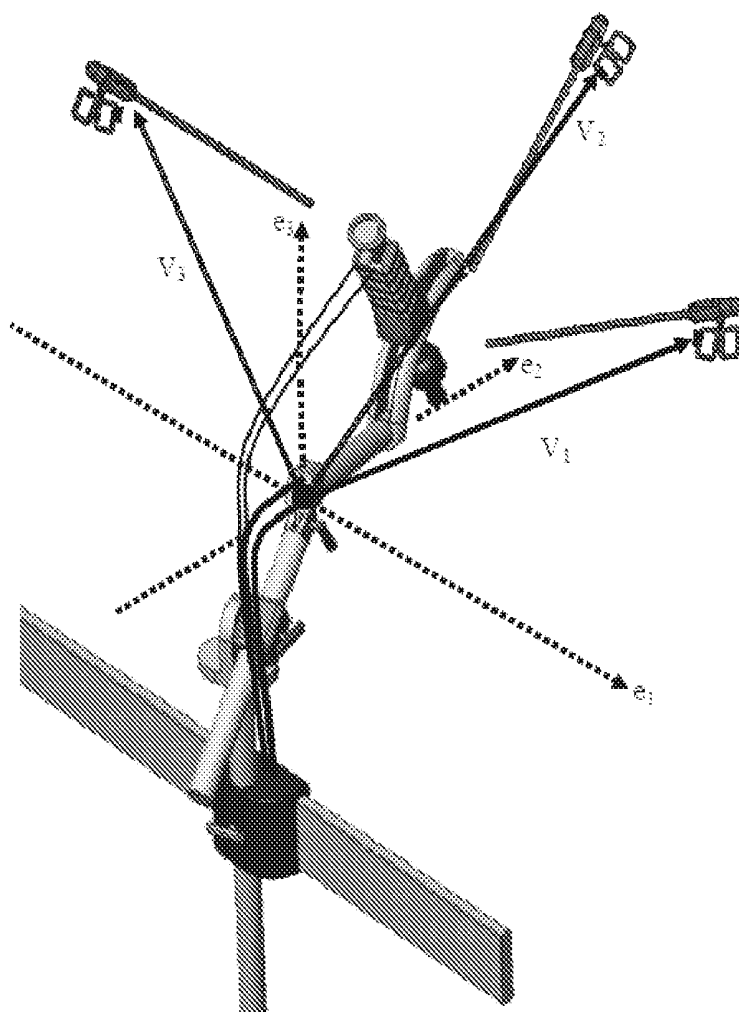


Fig. 5

DEVICE AND METHODS OF IMPROVING LAPAROSCOPIC SURGERY

FIELD OF THE INVENTION

[0001] The present invention generally relates to means and methods for improving the interface between the surgeon and the operating medical assistant or between the surgeon and an endoscope system for laparoscopic surgery. Moreover, this present invention discloses a device useful for controlling an endoscope system for laparoscopic surgery, in which the endoscope is inserted through a small incision into the body's cavities.

BACKGROUND OF THE INVENTION

[0002] In laparoscopic surgery, the surgeon performs the operation through small holes using long instruments and observing the internal anatomy with an endoscope camera. The endoscope is conventionally held by a camera human assistant (i.e. operating medical assistant) since the surgeon must perform the operation using both hands. The surgeon performance is largely dependent on the camera position relative to the instruments and on a stable image shown at the monitor. The main problem is the difficulty for the operating medical assistant to hold the endoscope steadily, keeping the scene upright.

[0003] Laparoscopic surgery is becoming increasingly popular with patients because the scars are smaller and their period of recovery is shorter. Laparoscopic surgery requires special training of the surgeon or gynecologist and the theatre nursing staff. The equipment is often expensive and not available in all hospitals.

[0004] During laparoscopic surgery it is often required to shift the spatial placement of the endoscope in order to present the surgeon with the optimal view. Conventional laparoscopic surgery makes use of either human assistants that manually shift the instrumentation or alternatively robotic automated assistants. Automated assistants utilize interfaces that enable the surgeon to direct the mechanical movement of the assistant, achieving a shift in the camera view.

[0005] U.S. Pat. No. 6,714,841 discloses an automated camera endoscope in which the surgeon is fitted with a head mounted light source that transmits the head movements to a sensor, forming an interface that converts the movements to directions for the mechanical movement of the automated assistant. Alternative automated assistants incorporate a voice operated interface, a directional key interface, or other navigational interfaces. The above interfaces share the following drawbacks:

[0006] a. Single directional interface that provide limited feedback to the surgeon

[0007] b. Cumbersome serial operation for starting and stopping movement directions that requires the surgeon's constant attention, preventing the surgeon from keeping the flow of surgical procedure.

[0008] Research has suggested that these systems divert the surgeons focus from the major task at hand. Therefore technologies assisted by magnets and image processing have been developed to simplify interfacing control. However these improved technologies still fail to address another complicating interface aspect of laparoscopic surgery, they do not allow the surgeon to signal to both the automated assistant and to human assistants or to surgical colleagues, which instrument his attention is focused on.

[0009] Hence, there is still a long felt need for a improving the interface between the surgeon and an endoscope system, surgical colleagues or human assistants for laparoscopic surgery.

SUMMARY OF THE INVENTION

[0010] It is one object of the present invention to disclose a device useful for the surgeon and the automated assistant interface, and/or said surgeon and the operating medical assistant interface, during laparoscopic surgery; wherein said device is adapted to control and/or direct said automated endoscope assistant to focus said endoscope on the desired instrument of said surgeon; further wherein said device is adapted to focus said operating medical assistant on said desired instrument of said surgeon.

[0011] It is another object of the present invention to disclose the device as defined above, wherein said device additionally comprising:

[0012] a. at least one wireless transmitter with at least one operating key;

[0013] b. at least one wireless receiver;

[0014] c. at least one conventional laparoscopy computerized system; said conventional laparoscopy computerized system is adapted to load a surgical instrument spatial locating software, and an automated assistant maneuvering software; said locating software enables a visual response to the depression of said at least one key on said wireless transmitter; said maneuvering software enables the movement of said endoscope; and

[0015] d. at least one video screen.

[0016] It is another object of the present invention to disclose the device as defined above, wherein each said instrument is fitted with a wireless transmitter.

[0017] It is another object of the present invention to disclose the device as defined above, wherein said wireless transmitter is freestanding.

[0018] It is another object of the present invention to disclose the device as defined above, wherein said wireless transmitter is adapted to locate the position of each instrument.

[0019] It is another object of the present invention to disclose the device as defined above, wherein said selection of said desired instrument is confirmed by clicking on said at least one key.

[0020] It is another object of the present invention to disclose the device as defined above, wherein said selection of said desired instrument is confirmed by depression of said at least one key on said wireless transmitter.

[0021] It is another object of the present invention to disclose the device as defined above, wherein said depression of said at least one key is a prolonged depression.

[0022] It is another object of the present invention to disclose a method useful for surgeon and the automated assistant interface, and/or said surgeon and the operating medical assistant interface, during laparoscopic surgery. The method comprises step selected inter alia from (a) obtaining a device as defined above; (b) selecting said desired instrument; and (c) displaying said desired instrument on a screen; wherein said device controlling and/or directing said automated endoscope assistant and thereby focusing said endoscope on said desired instrument of said surgeon.

[0023] It is another object of the present invention to disclose the method as defined above, additionally comprising the step of confirming by the selection of said desired instrument.

[0024] It is another object of the present invention to disclose the method as defined above, additionally comprising the step of extracting said desired instrument from said screen.

[0025] It is another object of the present invention to disclose the method as defined above, additionally comprising the step of instructing said automated assistant to focus said endoscope on said desired instrument.

[0026] It is another object of the present invention to disclose the method as defined above, wherein said step of selecting said desired instrument additionally comprising the steps of (a) depressing of said at least one key on said wireless transmitter; (b) transmitting a generic code to said receiver; (c) communicating said signal to the computer.

[0027] It is another object of the present invention to disclose the method as defined above, wherein said step of selecting said desired instrument additionally comprising the step confirming the selection of said desired instrument by clicking on said at least one key.

[0028] It is another object of the present invention to disclose the method as defined above, wherein said step of selecting said desired instrument additionally comprising the step confirming the selection of said desired instrument by a prolonged depression on said at least one key.

[0029] It is another object of the present invention to disclose the method as defined above, additionally comprising the step of re-selecting said desired instrument until said desired instrument is selected.

[0030] It is another object of the present invention to disclose the method as defined above, additionally comprising the step of identifying each of said instrument to said computerized system.

[0031] It is another object of the present invention to disclose the method as defined above, additionally comprising the step of attaching said wireless transmitter to said surgical instrument.

[0032] It is another object of the present invention to disclose the method as defined above, additionally comprising the step of matching each transmitted code from said depressed wireless transmitter to said surgical instrument.

[0033] It is another object of the present invention to disclose the method as defined above, wherein said step of matching each transmitted code additionally comprising the step of storing said matching database on a computer.

[0034] It is another object of the present invention to disclose the method as defined above, additionally comprising the step of signing said surgical instrument by a temporary onscreen graphic symbol and presenting upon the onscreen depiction of the surgical instrument.

[0035] It is another object of the present invention to disclose the method as defined above, additionally comprising the step of continuously displaying said selection graphic symbol.

[0036] It is still an object of the present invention to disclose the method as defined above, wherein the selection of the surgical instrument is signified by a continuous onscreen graphic symbol presented upon the onscreen depiction of the surgical instrument.

[0037] It is lastly an object of the present invention to disclose the method as defined above, additionally comprising the step of calculating the position of each said instrument.

BRIEF DESCRIPTION OF THE FIGURES

[0038] In order to understand the invention and to see how it may be implemented in practice, and by way of non-limiting example only, with reference to the accompanying drawing, in which

[0039] FIG. 1 is a general schematic view of an enhanced interface laparoscopic system that relies on a single wireless code signal to indicate the instrument on which to focus the endoscope constructed in accordance with the principles of the present invention in a preferred embodiment thereof;

[0040] FIG. 2 is a general schematic view of an enhanced interface laparoscopic system that relies on at least two wireless signals to indicate the instrument on which to focus the endoscope;

[0041] FIG. 3 is a schematic view of the method in which the single wireless code signal choice instrumentation focus is represented on the viewing apparatus;

[0042] FIG. 4 is a schematic view of the method in which multiple wireless code signal choice of instrumentation is operated;

[0043] FIG. 5 represents the relative position of each tool in respect to the mechanism;

DETAILED DESCRIPTION OF THE EMBODIMENTS

[0044] The following description is provided, alongside all chapters of the present invention, so as to enable any person skilled in the art to make use of the invention and sets forth the best modes contemplated by the inventor of carrying out this invention. Various modifications, however, will remain apparent to those skilled in the art, since the generic principles of the present invention have been defined specifically to provide means and methods for improving the interface between the surgeon and an endoscope system for laparoscopic surgery.

[0045] The present invention can be also utilized to improve the interface between the surgeon and the operating medical assistant and/or the surgeon colleagues. Moreover, the present invention can be also utilized to control and/or direct an automated endoscope assistant to focus the endoscope to the desired instrument of the surgeon. Furthermore, the device is adapted to focus the operating medical assistant on the desired instrument of the surgeon.

[0046] The term "conventional laparoscopy computerized system" refers herein to system or/software conventionally used in the market such as Lapman, Endo assist or AESOP.

[0047] In preferred embodiment of the invention a single wireless emission code is utilized and choice is achieved by a visible graphic representation upon the conventional viewing screen.

[0048] In another preferred embodiment each instrument is fitted with a unique code wireless transmitter, and selection is achieved by depressing its button.

[0049] The present invention discloses also a device joined with conventional camera assisted laparoscopic surgery systems comprising at least one wireless transmitter that may or may not be attached to the maneuvering control end of surgical instruments. Upon depression of at least one button on the transmitters either a generic or a unique code is transmitted to a receiving device connected to a computer that presents (e.g. displays) the selected surgical tool on a connected video screen. Confirmation of the selection by the depression of at least one button on wireless transmitter transmits a code

to the receiver connected to the computer that instructs the automated surgical assistant to move the endoscope achieving a view on the screen that is focused on the selected instrument area.

[0050] It would thus be desirable to achieve a device that allows the surgeon to identify to the laparoscopic computing system as well as to surgical colleagues to which surgical instrument attention is to be directed. By identifying the surgical instrument by the laparoscopic computing system the endoscope directs the view to the selected focus of attention.

[0051] Therefore, in accordance with a preferred embodiment of the present invention an enhanced interface laparoscopy device is provided. The device comprising:

[0052] a. At least one wireless transmitter with at least one operating key.

[0053] b. At least one wireless receiver.

[0054] c. at least one conventional laparoscopy computerized system; said conventional laparoscopy computerized system is adapted to load a surgical instrument spatial locating software, and an automated assistant maneuvering software; said locating software enables a visual response to the depression of said at least one key on said wireless transmitter; said maneuvering software enables the movement of said endoscope.

[0055] d. At least one video screen.

[0056] e. At least one automated assistant.

[0057] In a preferred embodiment of the enhanced interface laparoscopy device the wireless transmitter or transmitters are either freestanding or attached to the maneuvering end of the surgical instruments and emit the same single code that upon the depression of at least one key on them emits a signal to the receiver that communicates with the connected computer that displays a graphic symbol upon a random choice of one of the onscreen surgical instruments depicted or extracted by the computer on the screen. If needed the surgeon repeats the depression of at least one key resulting in a shift in the displayed graphic designator from one onscreen depiction of surgical instrument to another until the desired instrument is reached and thereby selected.

[0058] Subsequently the computer directs the automated assistant to focus the endoscope on the desired instrument area.

[0059] In a further preferred embodiment the selection of the instrument requires confirmation by varying the form of click on at least one key, such as a prolonged depression. Only upon confirmation is the computer authorized to instruct the automated assistant to focus the endoscope on the desired instrument area.

[0060] In another preferred embodiment of the invention each relevant surgical instruments is fitted at its maneuvering control end with a wireless transmitter with at least one key that transmits a unique code. In the initial stage of the procedure the surgeon identifies each of the instruments to the computerized system by depressing at least one key on each of the wireless transmitters fitted to the surgical instruments and matching their characteristics with a prepared database, thereby forming within the computerized system a unique signature for each of the transmitters. Thereon, upon depression of at least one key on the wireless transmitter attached to each surgical instrument, the receiver receives the unique code communicates it to the computer that identifies it with

the preprogrammed signature and instructs the automated assistant to move the endoscope so as to achieve the desired focus.

[0061] In another preferred embodiment of the invention each relevant surgical instruments is fitted at its maneuvering control end with a wireless transmitter with at least one key that transmits a unique code. While performing the surgery procedure, whenever the surgeon inserts, a surgical instrument at the first time, he signals by depressing at least one key on each of the wireless transmitters fitted to the surgical instruments.

[0062] Then the computer software identifies the instrument, while it is being inserted, analyzes the characteristics of the surgical instrument and keeps it in a database, thereby forming within the computerized system a unique signature for each of the transmitters. Thereon, upon depression of at least one key on the wireless transmitter attached to each surgical instrument, the receiver receives the unique code, communicates it to the computer that identifies it with the signature stored at the insertion step and instructs the automated assistant to move the endoscope so as to achieve the desired focus.

[0063] In a further preferred embodiment the selection is signified on the connected screen by displaying a graphic symbol upon the onscreen depiction of the surgical.

[0064] In a further preferred embodiment the selection is confirmed by an additional mode of depression of at least one key on the wireless transmitter, such as a prolonged depression of the key, authorizing the computer to instruct the automated assistant to change view provided by the endoscope.

[0065] The device of the present invention has many technological advantages, among them:

[0066] Simplifying the communication interface between surgeon and mechanical assistants.

[0067] Seamless interaction with conventional computerized automated endoscope systems.

[0068] Simplicity of construction and reliability.

[0069] User-friendliness

[0070] Additional features and advantages of the invention will become apparent from the following drawings and description.

[0071] Reference is made now to FIG. 1, which is a general schematic view of an enhanced interface laparoscopic system comprising one or more button operated wireless transmitters **12a**, that may or may not be attached to the maneuvering end of surgical instruments **17b** and **17c**, which once depressed aerially transmit a single code wave **14** through aerial **13** to connected receiver **11** that produces a signal processed by computer **15** thereby assigning a particular one of two or more surgical instruments **17b** and **17c** as the focus of the surgeons attention. Accordingly a conventional automated endoscope **21** is maneuvered by means of conventional automated arm **19** according to conventional computational spatial placement software contained in computer **15**.

[0072] Reference is made now to FIG. 2, which is a general schematic view of an enhanced interface laparoscopic system comprising one or more button operated wireless transmitters **12b** and **12c** are attached respectfully to the maneuvering means at the end of surgical instruments **17b** and **17c**, which once depressed aerially, each transmit a unique code wave **14b** and **14c** through aerial **13** to connected receiver **11** that produces a signal processed by computer **15** thereby assigning a particular one of two or more surgical instruments **17b** and **17c** as the focus of the surgeons attention. Accordingly a

conventional automated endoscope **21** is maneuvered by means of conventional automated arm **19** according to conventional computational spatial placement software contained in computer **15**.

[0073] Reference is made now to FIG. **3**, which is a schematic view of the method in which single wireless signal code choice of instrumentation focus is achieved, by means of video representation, **35b** and **35c** of the actual surgical instruments (not represented in FIG. **3**) displayed by graphic symbols. Wherein a light depression of the button on generic code emitting wireless transmitter **12a** transmits a code that is received by receiver aerial **13** communicated through connected receiver **11** to computer **15** that shifts the graphically displayed symbol of choice **35b** on video screen **30** from instrument to instrument until the required instrument is reached. A prolonged depression of the button on transmitter **12a** confirms the selection thereby signaling computer **15** to instruct the automated mechanical assistant (not represented in FIG. **4**) to move the endoscope (not represented in FIG. **3**) and achieving a camera view of the instrument area on screen **30**.

[0074] Reference is made now to FIG. **4**, which is a schematic view of the method in which multiple wireless signal code choice of instrumentation focus is achieved, by means of video representation **35b** and **35c** of the actual surgical instruments (not represented in FIG. **4**) displayed by graphic symbols. Wherein when buttons on unique code emitting wireless transmitters **12b** and **12c** attached respectfully to actual operational instruments (not represented in FIG. **4**) displays graphic symbol **35b** on respectful video representation **37b**. A prolonged depression of the button on transmitter **12b** and **12c** confirms the selection thereby signaling computer **15** to instruct the automated mechanical assistant (not represented in FIG. **4**) to move the endoscope (not represented in FIG. **4**) and achieving a camera view of the instrument area on screen **30**.

[0075] In another embodiment of this invention, when a prolonged depression of the buttons on transmitter **12b** and **12c** confirms the selection, the computer software analyze the characteristics of the surgical instrument and stores it in a database, thereby forming within the computerized system, a database, used for matching between each transmitting code and a surgical instrument.

[0076] From now on, when the surgeon presses again on this button, the receiver that receives the transmitted code, communicates it to the computer software that identifies the code as a "known" code and matching it, to the known parameters that were stored earlier in database of the surgical tools, and extracts the surgical tool tip. When the position tool tip is known, then the tracking software instructs the automated assistant to move the endoscope so as to achieve the desired focus.

[0077] Reference is made now to FIG. **5** illustrating the relative position of each tool. While performing the surgery, the surgeon often changes the position of his tools and even their insertion point. The wireless switches then may be use to locate the relative angle in which each tool is being held in respect to the camera holder mechanism. This is another advantage of the system that is used to calculate the position of the tool in the frame captured by the video camera. In that manner the surgeon does not have to inform the system where the insertion point of every tool is. The exact location of the wireless switch is not measured: the information about the relative positions of the tools in respect to each other contains

in most cases enough data for the software to maintain the matching between the switches and the tools. In this figure the positioning sensors of the system are placed near or on the camera holder and the signals they receive can be utilize in order to calculate the vectors $V_1 V_2 \dots V_n$ representing the range and the 3 angles needed to define a point in a 3D space.

[0078] In order to realize a position and range system, many well known technologies may be used. For example if the switches emit wireless signals then an array of antennas may be used to compare the power of the signal received at each antenna in order to determine the angle of the switch and it's approximate range to the camera holder mechanism. If the switch emits ultra sound wave then US microphones can be used to triangulate the position of the switch. The same is for light emitting switch.

1. A device for joining with an endoscope system for laparoscopic surgery to improve an interface between the endoscope system for laparoscopic surgery and a user of the endoscope system for laparoscopic surgery, the device comprising:

at least one wireless transmitter having at least one depressable, operating key, the at least one wireless transmitter configured to send at least one signal to a wireless receiver;

at least one surgical instrument in communication with the wireless transmitter;

at least one wireless receiver configured to receive the at least one signal;

an automated assistant in a form of at least one automated arm for moving the endoscope in at least two directions; and for enabling the endoscope to rotate around an insertion point into a body of a subject; and wherein the endoscope can pivot at the insertion point;

wherein the at least one wireless receiver is in communication with the computer and the computer is in communication with the automated assistant,

wherein the automated assistant initiates movement based on a human action of depressing the at least one depressable key, and

wherein the automated assistant mechanically maneuvers the endoscope in response to the at least one signal.

2. The device according to claim 1, wherein said device additionally comprising at least one computer.

3. The device according to claim 1, wherein said device additionally comprising at least one viewing screen.

4. The device according to claim 1, wherein the at least one wireless transmitter is manually activated.

5. The device according to claim 1, wherein the at least one wireless transmitter is freestanding.

6. The device according to claim 1, wherein the at least one wireless transmitter is attached to a maneuvering end of the at least one surgical instrument.

7. The device according to claim 1, wherein said selection of said desired instrument is confirmed by clicking on said at least one key.

8. The device according to claim 1, wherein said selection of said desired instrument is confirmed by depression of said at least one key on said wireless transmitter.

9. The device according to claim 8, wherein said depression of said at least one key is a prolonged depression.

10. An improved endoscope system for laparoscopic surgery, the improved endoscope system comprising:

an endoscope;

a pivoting support configured to be pivotally attached to the endoscope, thereby enabling the endoscope to pivot around the pivoting support;

an automated assistant in a form of at least one automated arm for moving the endoscope in at least two directions; and for enabling the endoscope to rotate around an insertion point into a body of a subject,

wherein the endoscope can pivot at the insertion point;

at least one wireless transmitter having at least one depressable, operating key, the wireless transmitter transmitting a first signal when the at least one depressable, operating key is pressed by human action;

one or more surgical instruments, each of the surgical instruments in communication with at least one of the wireless transmitter, wherein when the at least one depressable, operating key is pressed the surgical instrument that the depressable, operating key is in communication with is selected as a surgical instrument that attention of a user of the improved endoscope system is focused on;

a computer in communication with the automated assistant in the form of an automated arm;

at least one wireless receiver that receives the first signal, wherein upon receipt of the first signal produces a second signal and transmits the second signal to the computer; and

wherein when the computer receives the second signal the computer:

- (i) selects the surgical instrument that attention of a user of the improved endoscope system is focused on;
- (ii) displays the selected surgical instrument on the viewing screen; and
- (iii) directs the automated assistant to mechanically position the endoscope on the selected surgical instrument.

11. The improved endoscope system according to claim 10, additionally comprising a viewing screen.

12. The improved endoscope system according to claim 10, wherein the at least one wireless transmitter is manually activated.

13. The improved endoscope system according to claim 10, wherein the at least one wireless transmitter is freestanding.

14. The improved endoscope system according to claim 10, wherein the at least one wireless transmitter is attached to a maneuvering end of the one or more surgical instruments.

15. The device according to claim 10, wherein said selection of said desired instrument is confirmed by clicking on said at least one key.

16. The device according to claim 10, wherein said selection of said desired instrument is confirmed by depression of said at least one key on said wireless transmitter.

17. The device according to claim 16, wherein said depression of said at least one key is a prolonged depression.

18. A method for using an improved endoscope system for laparoscopic surgery, the method comprising:

providing an improved endoscope system according to claim 10;

pressing the at least one depressable, operating key to transmit a first signal to the at least one wireless receiver;

transmitting a second signal from the wireless receiver to select a surgical instrument on which to focus attention; and,

and

directing the automated assistant to mechanically position the endoscope on the selected surgical instrument.

19. The method according to claim 18, further comprising step of providing viewing screen and displaying the selected surgical instrument on the viewing screen.

20. The method according to claim 18, further comprising attaching the at least one wireless transmitter to a surgical instrument.

21. The method according to claim 18, wherein said selection of said desired instrument is confirmed by clicking on said at least one key.

22. The method according to claim 18, wherein said selection of said desired instrument is confirmed by depression of said at least one key on said wireless transmitter.

23. The method according to claim 22, wherein said depression of said at least one key is a prolonged depression.

24. The method according to claim 18, wherein the at least one wireless transmitter is freestanding.

25. The improved endoscope system according to claim 10, wherein each of the surgical instruments is assigned with a dedicated first signal; such that upon receipt of said second signal being sent to the computer, said computer is configured to perform at least one action selected from a group consisting of:

- selects the surgical instrument with which said first signal is assigned;
- (ii) displays the selected surgical instrument on the viewing screen; and
- (iii) directs the automated assistant to mechanically position the endoscope on the selected surgical instrument;
- (vi) any combination thereof.

26. The improved endoscope system according to claim 10, wherein when the computer receives the second signal, the computer is configured to perform at least one action selected from a group consisting of:

- displays each of the surgical instruments on the viewing screen until the user of the improved endoscope system selected surgical instrument on the viewing screen; and
- (ii) directs the automated assistant to mechanically position the endoscope on the selected surgical instrument;
- (iii) any combination thereof.

27. The device according to claim 1, wherein each of the surgical instruments is assigned with a dedicated signal; such that upon receipt of said signal being sent to the computer, said computer is configured to perform at least one action selected from a group consisting of:

- selects the surgical instrument with which said signal is assigned;
- (ii) displays the selected surgical instrument on the viewing screen; and
- (iii) directs the automated assistant to mechanically position the endoscope on the selected surgical instrument;
- (vi) any combination thereof.

28. The device according to claim 1, wherein when the computer receives the signal, the computer is configured to perform at least one action selected from a group consisting of:

- displays each of the surgical instruments on the viewing screen until the user of the improved endoscope system selected surgical instrument on the viewing screen; and

- (ii) directs the automated assistant to mechanically position the endoscope on the selected surgical instrument;
- (iii) any combination thereof.

29. The method according to claim 18, further comprising a step of assigning each of the surgical instruments a dedicated signal; such that upon receipt of said signal being sent to the computer, said computer is configured to perform at least one action selected from a group consisting of:

- selects the surgical instrument with which said signal is assigned;
- (ii) displays the selected surgical instrument on the viewing screen; and
- (iii) directs the automated assistant to mechanically position the endoscope on the selected surgical instrument;
- (vi) any combination thereof.

30. The method according to claim 18, further comprising a step of once the computer receives the signal, the computer is configured to perform at least one action selected from a group consisting of:

- displays each of the surgical instruments on the viewing screen until the user of the improved endoscope system selected surgical instrument on the viewing screen; and
- (ii) directs the automated assistant to mechanically position the endoscope on the selected surgical instrument;
- (iii) any combination thereof.

31. The method according to claim 18, additionally comprising a step of confirming a selection of said desired instrument.

32. The method according to claim 18, additionally comprising a step of extracting said desired instrument from said screen.

33. The method according to claim 18, wherein said step of selecting said desired instrument additionally comprising the steps of (a) depressing of said at least one key on said wireless transmitter; (b) transmitting a generic code to said receiver; (c) and communicating said signal to the computer.

34. The method according to claim 18, wherein said step of selecting said desired instrument additionally comprises the step of confirming the selection of said desired instrument by clicking on said at least one key.

35. The method according to claim 18, wherein said step of selecting said desired instrument additionally comprises the step of confirming the selection of said desired instrument by a prolonged depression on said at least one key.

36. The method according to claim 18, additionally comprising the step of re-selecting said desired instrument until said desired instrument is selected.

37. The method according to claim 18, additionally comprising the step of identifying each of said instruments to said computerized system.

38. The method according to claim 18, additionally comprising the step of attaching said wireless transmitter to said surgical instrument.

39. The method according to claim 18, additionally comprising the step of matching each transmitted code from said depressed wireless transmitter to said surgical instrument.

40. The method according to claim 18, wherein said step of matching each transmitted code additionally comprises the step of storing said matching database on a computer.

41. The method according to claim 18, additionally comprising the step of signing said surgical instrument by a temporary onscreen graphic symbol and presenting upon the onscreen depiction of the surgical instrument.

42. The method according to claim 18, additionally comprising the step of continuously displaying said selection graphic symbol.

43. The method according to claim 18, wherein the selection of the surgical instrument is signified by a continuous onscreen graphic symbol presented upon the onscreen depiction of the surgical instrument.

* * * * *

专利名称(译)	改善腹腔镜手术的装置和方法		
公开(公告)号	US20160157698A1	公开(公告)日	2016-06-09
申请号	US15/046862	申请日	2016-02-18
[标]申请(专利权)人(译)	M.S.T.医学外科技术有限公司		
申请(专利权)人(译)	M.S.T.医疗手术TECHNOLOGIES LTD.		
当前申请(专利权)人(译)	M.S.T.医疗手术TECHNOLOGIES LTD.		
[标]发明人	SHOLEV MORDEHAI		
发明人	SHOLEV, MORDEHAI		
IPC分类号	A61B1/00 A61B17/00 A61B34/00 A61B1/313		
CPC分类号	A61B1/00016 A61B1/00149 A61B1/3132 A61B1/00006 A61B2017/00225 A61B34/25 A61B1/00045 A61B2034/301 A61B17/00234 A61B34/30 A61B34/70 A61B34/74 A61B90/361 A61B2017/00221 A61B2034/2051		
优先权	60/672010 2005-04-18 US 60/705199 2005-08-04 US 60/716953 2005-09-15 US 60/716951 2005-09-15 US		
其他公开文献	US10456010		
外部链接	Espacenet USPTO		

摘要(译)

用于腹腔镜手术的外科医生和内窥镜系统之间的改进的接口，保持腹腔镜相机和/或控制自动内窥镜助手包括至少一个具有至少一个操作键的无线发射器，至少一个无线接收器，至少一个传统的腹腔镜检查装载有传统手术器械空间定位软件的计算机化系统，以及传统的自动辅助操纵软件，加载到传统腹腔镜系统上的软件，其能够对无线发射器上的至少一个按键的按压进行视觉响应以及传统的接口相接自动辅助操纵软件，以实现内窥镜的移动，以及至少一个视频屏幕。

