



US006960210B2

(12) **United States Patent**
Lands et al.

(10) **Patent No.:** **US 6,960,210 B2**
(45) **Date of Patent:** ***Nov. 1, 2005**

(54) **LAPAROSCOPIC BIPOLAR
ELECTROSURGICAL INSTRUMENT**

(75) Inventors: **Michael John Lands**, Clearwater, FL (US); **Stephen Wade Lukianow**, Boulder, CO (US); **Donald Robert Loeffler**, Louisville, CO (US); **James Steven Cunningham**, Boulder, CO (US); **Kate Ryland Lawes**, Superior, CO (US); **Daniel Lee Trimberger, II**, Greeley, CO (US); **Mathew Erle Mitchell**, Boulder, CO (US); **Jenifer Serafin Kennedy**, Boulder, CO (US)

(73) Assignee: **Sherwood Services AG**, Schaffhausen (CH)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **10/243,274**

(22) Filed: **Sep. 13, 2002**

(65) **Prior Publication Data**

US 2003/0032956 A1 Feb. 13, 2003

Related U.S. Application Data

(63) Continuation of application No. 09/591,330, filed on Jun. 9, 2000, now Pat. No. 6,451,018, which is a continuation of application No. 08/970,472, filed on Nov. 14, 1997, now Pat. No. 6,228,083.

(51) Int. Cl.⁷ **A61B 18/14**

(52) U.S. Cl. **606/50**; 606/46; 606/48; 606/51; 606/207; 606/208

(58) Field of Search 606/46, 48-52, 606/170, 207, 208

(56) **References Cited**

U.S. PATENT DOCUMENTS

371,664 A	10/1887	Brannan et al.
702,472 A	6/1902	Pignolet
728,883 A	5/1903	Downes

(Continued)

FOREIGN PATENT DOCUMENTS

CA	2104423	2/1994
DE	19608716	4/1997
EP	0364216 A1	4/1990

(Continued)

OTHER PUBLICATIONS

US 6,090,109, 7/2000, Lands et al. (withdrawn)


(Continued)

Primary Examiner—Lee S. Cohen

(57) **ABSTRACT**

A laparoscopic bipolar electrosurgical instrument can apply a large closure force between its jaw without damaging the small yoke assembly. The instrument comprises: a first jaw having a first flange with a first slot, and a second jaw having a second flange with a second slot, wherein the first and second jaws are located at a distal end of the instrument and comprise an electrically conductive material for conducting bipolar electrosurgical current therebetween; a yoke attached to a pushrod and positioned to electrically insulate the first flange from the second flange, the yoke having a first side facing the first flange and a second side facing the second flange, the yoke further comprising a first shoulder and a second shoulder; a first pin located on the first side and movably engaged with the first slot; a second pin located on the second side and movably engaged with the second slot; the first slot and the second slot shaped such that an angle, subtended by the first and second jaws, decreases with distal motion of the pushrod, and first and second cul-de-sacs positioned respectively in the first and second slots to relieve shear stresses on the first and second pins approximately when the first and second shoulders respectively engage the first and second flanges to provide a closure force between the first and second jaws.

5 Claims, 5 Drawing Sheets

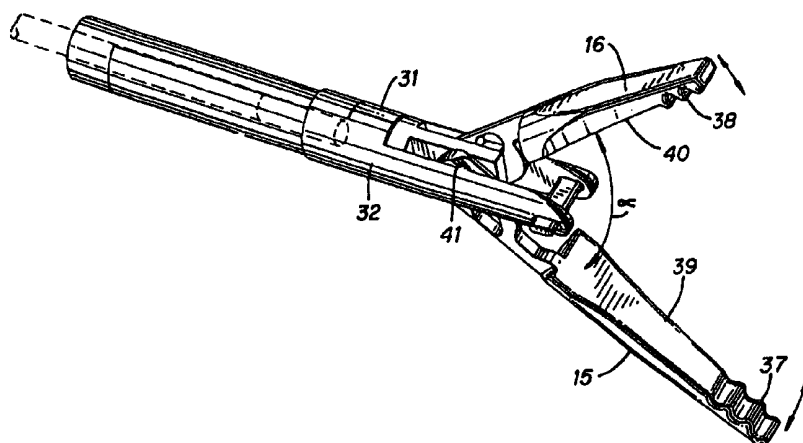

U.S. PATENT DOCUMENTS

1,586,645 A	6/1926	Bierman	5,389,098 A	2/1995	Tsuruta et al.
2,002,594 A	5/1935	Wappler et al.	5,389,104 A	2/1995	Hahnen et al.
2,011,169 A	5/1935	Wappler	5,391,166 A	2/1995	Eggers
2,176,479 A	10/1939	Willis	5,391,183 A	2/1995	Janzen et al.
2,305,156 A	12/1942	Grubel	5,403,312 A	4/1995	Yates et al.
2,632,661 A	12/1953	Cristofv	5,411,519 A	5/1995	Tovey et al.
2,668,538 A	2/1954	Baker	5,411,520 A	5/1995	Nash et al.
2,796,065 A	6/1957	Kapp	5,413,571 A	5/1995	Katsaros et al.
3,459,187 A	8/1969	Pallotta	5,415,657 A	5/1995	Taymor-Luria
3,643,663 A	2/1972	Sutter	5,423,810 A	6/1995	Goble et al.
3,651,811 A	3/1972	Hildebrandt et al.	5,425,739 A	6/1995	Jessen
3,862,630 A	1/1975	Balamuth	5,429,616 A	7/1995	Schaffer
3,866,610 A	2/1975	Kletschka	5,431,674 A	7/1995	Basile et al.
3,911,766 A	10/1975	Fridolph et al.	5,437,292 A	8/1995	Kipshidze et al.
3,920,021 A	11/1975	Hitebrandt	5,438,302 A	8/1995	Goble
3,921,641 A	11/1975	Hulka	5,441,517 A	8/1995	Kensey et al.
3,938,527 A	2/1976	Rioux et al.	5,443,463 A	8/1995	Stern et al.
3,952,749 A	4/1976	Fridolph et al.	5,443,464 A	8/1995	Russell et al.
4,005,714 A	2/1977	Hiltebrandt	5,443,480 A	8/1995	Jacobs et al.
4,074,718 A	2/1978	Morrison, Jr.	5,445,638 A	8/1995	Rydell
4,088,134 A	5/1978	Mazzariello	5,445,658 A	8/1995	Durrfeld et al.
4,165,746 A	8/1979	Burgin	5,451,224 A	9/1995	Goble et al.
4,300,564 A	11/1981	Furihata	5,456,684 A	10/1995	Schmidt et al.
4,370,980 A	2/1983	Lottick	5,458,598 A	10/1995	Feinberg et al.
D276,790 S	12/1984	Laske	5,460,629 A	10/1995	Shlain et al.
4,492,231 A	1/1985	Auth	5,462,546 A	10/1995	Rydell
4,552,143 A	11/1985	Lottick	5,472,443 A	12/1995	Cordis et al.
4,574,804 A	3/1986	Kurwa	5,478,351 A	12/1995	Meade et al.
4,597,379 A	7/1986	Kihn et al.	5,484,436 A	1/1996	Eggers et al.
4,657,016 A	4/1987	Garito et al.	5,496,317 A	3/1996	Goble et al.
4,671,274 A	6/1987	Sorochenko	5,499,997 A	3/1996	Sharpe et al.
4,685,459 A	8/1987	Koch et al.	5,509,922 A	4/1996	Aranyi et al.
4,763,669 A	8/1988	Jaeger	5,514,134 A	5/1996	Rydell et al.
4,827,929 A	5/1989	Hodge	5,527,313 A	6/1996	Scott et al.
4,887,612 A	12/1989	Esser et al.	5,531,744 A	7/1996	Nardella et al.
4,938,761 A	7/1990	Ensslin	5,540,684 A	7/1996	Hassler, Jr.
5,007,908 A	4/1991	Rydell	5,540,685 A	7/1996	Parins et al.
5,026,370 A	6/1991	Lottick	5,540,715 A	7/1996	Katsaros et al.
5,099,840 A	3/1992	Goble et al.	5,558,672 A	9/1996	Edwards et al.
5,116,332 A	5/1992	Lottick	5,569,241 A	10/1996	Edwards
5,151,102 A	9/1992	Kamiyama et al.	5,569,243 A	10/1996	Kortenbach et al.
5,176,695 A	1/1993	Dulebohn	5,571,100 A	11/1996	Goble et al.
5,197,964 A	3/1993	Parins	5,573,535 A	11/1996	Viklund
5,215,101 A	6/1993	Jacobs et al.	5,585,896 A	12/1996	Yamazaki et al.
5,217,457 A	6/1993	Delahuerga et al.	5,590,570 A	1/1997	LeMaire, III et al.
5,217,458 A	6/1993	Parins	5,603,711 A	2/1997	Parins et al.
5,244,462 A	9/1993	Delahuerga et al.	5,603,723 A	2/1997	Aranyi et al.
5,250,047 A	10/1993	Rydell	5,626,578 A	5/1997	Tihon
5,258,006 A	11/1993	Rydell et al.	5,630,833 A	5/1997	Katsaros et al.
5,261,918 A	11/1993	Phillips et al.	5,637,110 A	6/1997	Pennybacker et al.
5,275,615 A	1/1994	Rose	5,643,294 A	7/1997	Tovey et al.
5,277,201 A	1/1994	Stern	5,647,869 A	7/1997	Goble et al.
5,282,799 A	2/1994	Rydell	5,649,959 A	7/1997	Hannam et al.
5,290,286 A	3/1994	Parins	5,658,281 A	8/1997	Heard
5,304,203 A	4/1994	El-Mallawany et al.	5,667,526 A	9/1997	Levin
5,308,357 A	5/1994	Lichtman	5,674,220 A	10/1997	Fox et al.
5,318,589 A	6/1994	Lichtman	5,693,051 A	12/1997	Schulze et al.
5,324,289 A	6/1994	Eggers	5,695,522 A	12/1997	LeMaire, III et al.
5,330,471 A	7/1994	Eggers	5,700,261 A	12/1997	Brinkerhoff
5,334,183 A	8/1994	Wuchinich	5,702,390 A	12/1997	Austin et al.
5,334,215 A	8/1994	Chen	5,707,369 A	1/1998	Vaitekunas et al.
5,336,221 A	8/1994	Anderson	5,709,680 A	1/1998	Yates et al.
5,342,359 A	8/1994	Rydell	5,727,428 A	3/1998	LeMaire, III et al.
5,342,381 A	8/1994	Tidemand	5,743,906 A	4/1998	Parins et al.
5,342,393 A	8/1994	Stack	5,755,717 A	5/1998	Yates et al.
5,352,222 A	10/1994	Rydell	5,766,166 A	6/1998	Hooven
5,354,271 A	10/1994	Voda	5,766,170 A	6/1998	Eggers
5,356,408 A	10/1994	Rydell	5,769,849 A	6/1998	Eggers
5,366,477 A	11/1994	LeMarie, III et al.	5,776,128 A	7/1998	Eggers
5,383,897 A	1/1995	Wholey	5,776,130 A	7/1998	Buyse et al.
			5,779,701 A	7/1998	McBrayer et al.

5,792,137 A 8/1998 Carr et al.
 5,792,177 A 8/1998 Kaseda
 5,797,958 A 8/1998 Yoon
 5,800,449 A 9/1998 Wales
 5,810,808 A 9/1998 Eggers
 5,810,811 A 9/1998 Yates et al.
 5,814,043 A 9/1998 Shapeton
 5,827,271 A 10/1998 Buysse et al.
 5,827,279 A 10/1998 Hughett et al.
 5,827,281 A 10/1998 Levin
 5,833,690 A 11/1998 Yates et al.
 5,843,080 A 12/1998 Fleenor et al.
 5,849,022 A 12/1998 Sakashita et al.
 5,853,412 A 12/1998 Mayenberger
 5,876,401 A 3/1999 Schulze et al.
 5,891,141 A 4/1999 Rydell
 5,891,142 A 4/1999 Eggers et al.
 5,893,863 A 4/1999 Yoon
 5,893,875 A 4/1999 Oconnor et al.
 5,902,301 A 5/1999 Olig
 5,908,420 A 6/1999 Parins et al.
 5,913,874 A 6/1999 Berns et al.
 5,921,984 A 7/1999 Sutcu et al.
 5,935,126 A 8/1999 Riza
 5,951,549 A 9/1999 Richardson et al.
 5,954,720 A 9/1999 Wilson et al.
 5,976,132 A 11/1999 Morris
 5,989,277 A 11/1999 LeMaire, III et al.
 6,004,335 A 12/1999 Vaitekunas et al.
 6,024,744 A 2/2000 Kese et al.
 6,033,399 A 3/2000 Gines
 6,039,733 A 3/2000 Buysse et al.
 6,050,996 A 4/2000 Schmaltz et al.
 6,053,914 A 4/2000 Eggers et al.
 6,053,933 A 4/2000 Balazs et al.
 D424,694 S 5/2000 Tetzlaff et al.
 D425,201 S 5/2000 Tetzlaff et al.
 RE36,795 E 7/2000 Rydell
 6,083,223 A 7/2000 Baker
 6,086,586 A 7/2000 Hooven
 6,090,107 A 7/2000 Borgmeier et al.
 6,099,550 A 8/2000 Yoon
 6,102,909 A 8/2000 Chen et al.
 6,110,171 A 8/2000 Rydell
 6,113,596 A 9/2000 Hooven et al.
 6,113,598 A 9/2000 Baker
 H1904 H 10/2000 Yates et al.
 6,126,658 A 10/2000 Baker
 6,152,923 A 11/2000 Ryan
 6,174,309 B1 1/2001 Wrublewski et al.
 6,179,834 B1 1/2001 Buysse et al.
 6,179,837 B1 1/2001 Hooven
 6,183,467 B1 2/2001 Shapeton et al.
 6,187,003 B1 2/2001 Buysse et al.
 6,190,386 B1 2/2001 Rydell
 6,193,718 B1 2/2001 Kortenbach et al.
 6,206,877 B1 3/2001 Kese et al.
 6,224,593 B1 5/2001 Ryan et al.
 6,228,080 B1 5/2001 Gines
 6,228,083 B1 5/2001 Lands et al.
 6,267,761 B1 7/2001 Ryan
 6,273,887 B1 8/2001 Yamauchi et al.
 6,277,117 B1 8/2001 Tetzlaff et al.
 D449,886 S 10/2001 Tetzlaff et al.
 6,334,861 B1 1/2002 Chandler et al.
 6,350,264 B1 2/2002 Hooven
 6,352,536 B1 3/2002 Buysse et al.
 6,409,728 B1 6/2002 Ehr et al.
 H2037 H 7/2002 Yates et al.
 6,443,970 B1 9/2002 Schulze et al.
 6,451,018 B1 * 9/2002 Lands et al. 606/50

6,458,128 B1 10/2002 Schulze
 6,458,130 B1 10/2002 Frazier et al.
 6,511,480 B1 1/2003 Tetzlaff et al.
 6,585,735 B1 7/2003 Frazier et al.
 6,620,161 B2 9/2003 Schulze et al.
 6,682,528 B2 1/2004 Frazier et al.
 2003/0018331 A1 1/2003 Dycus et al.

FOREIGN PATENT DOCUMENTS


EP 0 518 230 A1 12/1992
 EP 0541930 B1 5/1993
 EP 0572131 A1 12/1993
 EP 0 584 787 A1 3/1994
 EP 0623316 A1 11/1994
 EP 0650701 A1 5/1995
 EP 0694290 A3 3/1996
 EP 0754437 A3 3/1997
 EP 0717966 A1 6/1998
 EP 0 853 922 A1 7/1998
 EP 0887046 A3 1/1999
 EP 0923907 A1 6/1999
 EP 1034747 A1 9/2000
 EP 1034748 A1 9/2000
 EP 1025807 A3 10/2000
 EP 1034746 A3 10/2000
 EP 1050278 A1 11/2000
 EP 1053719 A1 11/2000
 EP 1053720 A1 11/2000
 EP 1055399 A1 11/2000
 EP 1055400 A1 11/2000
 EP 1080694 A1 3/2001
 EP 1082944 A1 3/2001
 GB 2214430 A 6/1989
 JP 5-40112 2/1993
 JP 06343644 A2 12/1994
 JP 07265328 A2 10/1995
 JP 08056955 A2 3/1996
 JP 08252263 A2 10/1996
 JP 09010223 A2 1/1997
 JP 11249298 A2 9/1999
 JP 2000342599 A2 12/2000
 JP 2000350732 A2 12/2000
 JP 2001008944 A2 1/2001
 JP 2001029356 A2 2/2001
 JP 2001128990 A2 5/2001
 SU 401367 10/1973
 WO WO 92/06642 4/1992
 WO WO 95/02369 1/1995
 WO WO 97/00646 1/1997
 WO WO97/00647 1/1997
 WO WO 97/24073 7/1997
 WO WO 97/24993 7/1997
 WO WO 98/27880 7/1998
 WO WO 99/03407 1/1999
 WO WO 99/03408 1/1999
 WO WO 99/03409 1/1999
 WO WO 99/40857 8/1999
 WO WO 99/51158 10/1999
 WO WO 00/24330 5/2000
 WO WO 00/41638 7/2000
 WO WO 00/53112 9/2000
 WO WO 01/54604 A1 8/2001
 WO WO 02/080796 A1 10/2002

OTHER PUBLICATIONS

Bergdahl et al., Studies on Coagulation and the Development of an Automatic Computerized Bipolar Conagulator, J. Neurosurg. vol. 75, Jul. 1991 pp 148-151.
 Sigel et al., The Mechanism of Blood Vessel Closure By High Frequency Electrocoagulation, Surgery & Gynecology and Obstetrics, Oct. 1965 pp. 832-831.

- Kennedy et al. "High-burst-strength, feedback-controlled bipolar vessel sealing", *Surgical Endoscopy* (1998) 12:876-878.
- Peterson et al. "Comparison of Healing Process Following Ligation with Sutures and Bipolar Vessel Sealing", *Surgical Technology International* (2001).
- Linehan et al. "A Phase I Study of the LigaSure Vessel Sealing System in Hepatic Surgery", Section of HPB Surgery, Washington University School of medicine, St. Louis MO, Presented at AHPBA, Feb. 2001.
- Johnson et al. "Evaluation of the LigaSure Vessel Sealing System in Hemorrhoidectomy", American College of Surgeons (ACS) Clinical Congress Poster (2000).
- Sayfan et al. "Sutureless Closed Hemorrhoidectomy: A New Technique", *Annals of Surgery* vol. 234 No. 1 Jul. 2001 pp. 21-24.
- Henlford et al. "Initial Results with an Electrothermal Bipolar Vessel Sealer", *Surgical Endoscopy* (2000) 15:799-801.
- Henlford et al. "Initial Research and Clinical results with an Electrothermal Bipolar Vessel Sealer", Oct. 1999.
- McLellan et al. "Vessel Sealing for Hemostasis During pelvic Surgery", Int'l Federation of Gynecology and Obstetrics FIGO World Congress 2000, Washington, D.C.
- Levy et al. "Use of a New Energy-based Vessel Ligation Device During Vaginal Hysterectomy", Int'l Federation of Gynecology and Obstetrics (FIGO) World Congress.
- Crawford et al. "Use of the LigaSure Vessel Sealing System in Urologic Cancer Surgery", *Grand Rounds in Urology* 1999 vol. 1 Issue 4 pp. 10-17.
- Rothenberg et al. "Use of the LigaSure Vessel Sealing System in Minimally Invasive Surgery in Children", Int'l Pediatric Endosurgery Group (IPEG) 2000.
- Palazzo et al. "Randomized clinical trial of Ligasure versus open haemorrhoidectomy", *British Journal of Surgery* 2002, 89, 154-157.
- "Innovative in Electrosurgery" Sales/Product Literature.
- LigaSure Vessel Sealing System, the Seal of Confidence in General, Gynecologic, Urologic, and Laparoscopic Surgery Sales/Product Literature.
- Carbonell et al., "Comparison of the Gyrus PlasmaKinetic Sealer and the Valleylab LigaSure Device in the Hemostasis of Small, Medium, and Large-Sized Arteries" Carolinas Laparoscopic and Advanced Surgery Program, Carolinas Medical Center, Charlotte, NC.
- "Reducing Needlestick Injuries in the Operating Room" Sales/Product Literature.
- Chung et al., "Clinical Experience of Sutureless Closed Hemorrhoidectomy with LigaSure" *Diseases of the Colon & Rectum* vol. 46, No. 1 Jan. 2003.
- Strasberg et al., "Use of a Bipolar Vessel-Sealing Device for Parenchymal Transaction During Liver Surgery" *Journal of Gastrointestinal Surgery*, vol. 6, No. 4, Jul./Aug. 2002 pp. 569-574.
- Paul G. Horgan, "A Novel Technique for Parenchymal Division During Hepatectomy" *The American Journal of Surgery*, vol. 181, No. 3, Apr. 2001 pp. 236-237.
- W. Scott Helton, "LigaSure Vessel Sealing System: Revolutionary Hemostasis Product for General Surgery" Sales/Product Literature.
- Michael Choti, "Abdominoperineal Resection with the LigaSure Vessel Sealing System and LigaSure Atlas 20 cm Open Instrument" *Innovations That Work*, Jun. 2003.
- Craig Johnson, "Use of the LigaSure Vessel Sealing System in Bloodless Hemorrhoidectomy" *Innovations that Work*, Mar. 2000.
- Mueller et al., "Extended Left Hemicolectomy Using the LigaSure Vessel Sealing System" *Innovations that Work*, Sep. 1999.
- Herman et al., "Laparoscopic Intestinal Resection With the LigaSure Vessel Sealing System: A Case Report" *Innovations that Work*, Feb. 2002.
- Carus et al., "Initial Experience With The LigaSure Vessel Sealing System in Abdominal Surgery" *Innovations That Work*, Jun. 2002.
- Levy et al. "Randomized Trial of Suture Versus Electrosurgical Bipolar Vessel Sealing in Vaginal Hysterectomy" *Obstetrics & Gynecology*, vol. 102, No. 1, Jul. 2003.
- Levy et al., "Update on Hysterectomy—New Technologies and Techniques" *OBG Management*, Feb. 2003.
- Barbara Levy, "Use of a New Vessel Ligation Device During Vaginal Hysterectomy" FIGO 2000, Washington, D.C.
- McLellan et al. "Vessel Sealing For Hemostasis During Gynecologic Surgery" Sales/Product Literature.
- Sengupta et al., "Use of a Computer-Controlled Bipolar Diathermy System in Radical Prostatectomies and Other Open Urological Surgery" *ANZ Journal of Surgery* (2001) 71.9 pp. 538-540.
- Olsson et al. "Radical Cystectomy in Females" *Current Surgical Techniques in Urology*, vol. 14, Issue 3.
- E. David Crawford "Use of a Novel Vessel Sealing Technology in Management of the Dorsal Venous Complex" sales Product Literature.
- Jarrett et al., "Use of the LigaSure Vessel Sealing System for Peri-Hilar Vessels in Laparoscopic Nephrectomy" Sales Product Literature.
- E. David Crawford "Evaluation of a New Vessel Sealing Device in urological Cancer Surgery" Sales Product Literature.
- Joseph Ortenberg "LigaSure System used in Laparoscopic 1st and 2nd Stage Orchiopaxy" *Innovations That Work*, Nov. 2002.
- Koyle et al., "Laparoscopic Palomo Varicocele Ligation in Children and Adolescents" *Pediatric Endosurgery & innovative Techniques*, vol. 6, No. 1, 2002.
- Dulemba et al. "Use of a Bipolar Electrothermal Vessel Sealer in Laparoscopically Assisted Vaginal Hysterectomy" Sales Product Literature.
- Johnson et al. "Evaluation of a Bipolar electrothermal Vessel Sealing Device in Hemorrhoidectomy" Sales Product Literature.

* cited by examiner

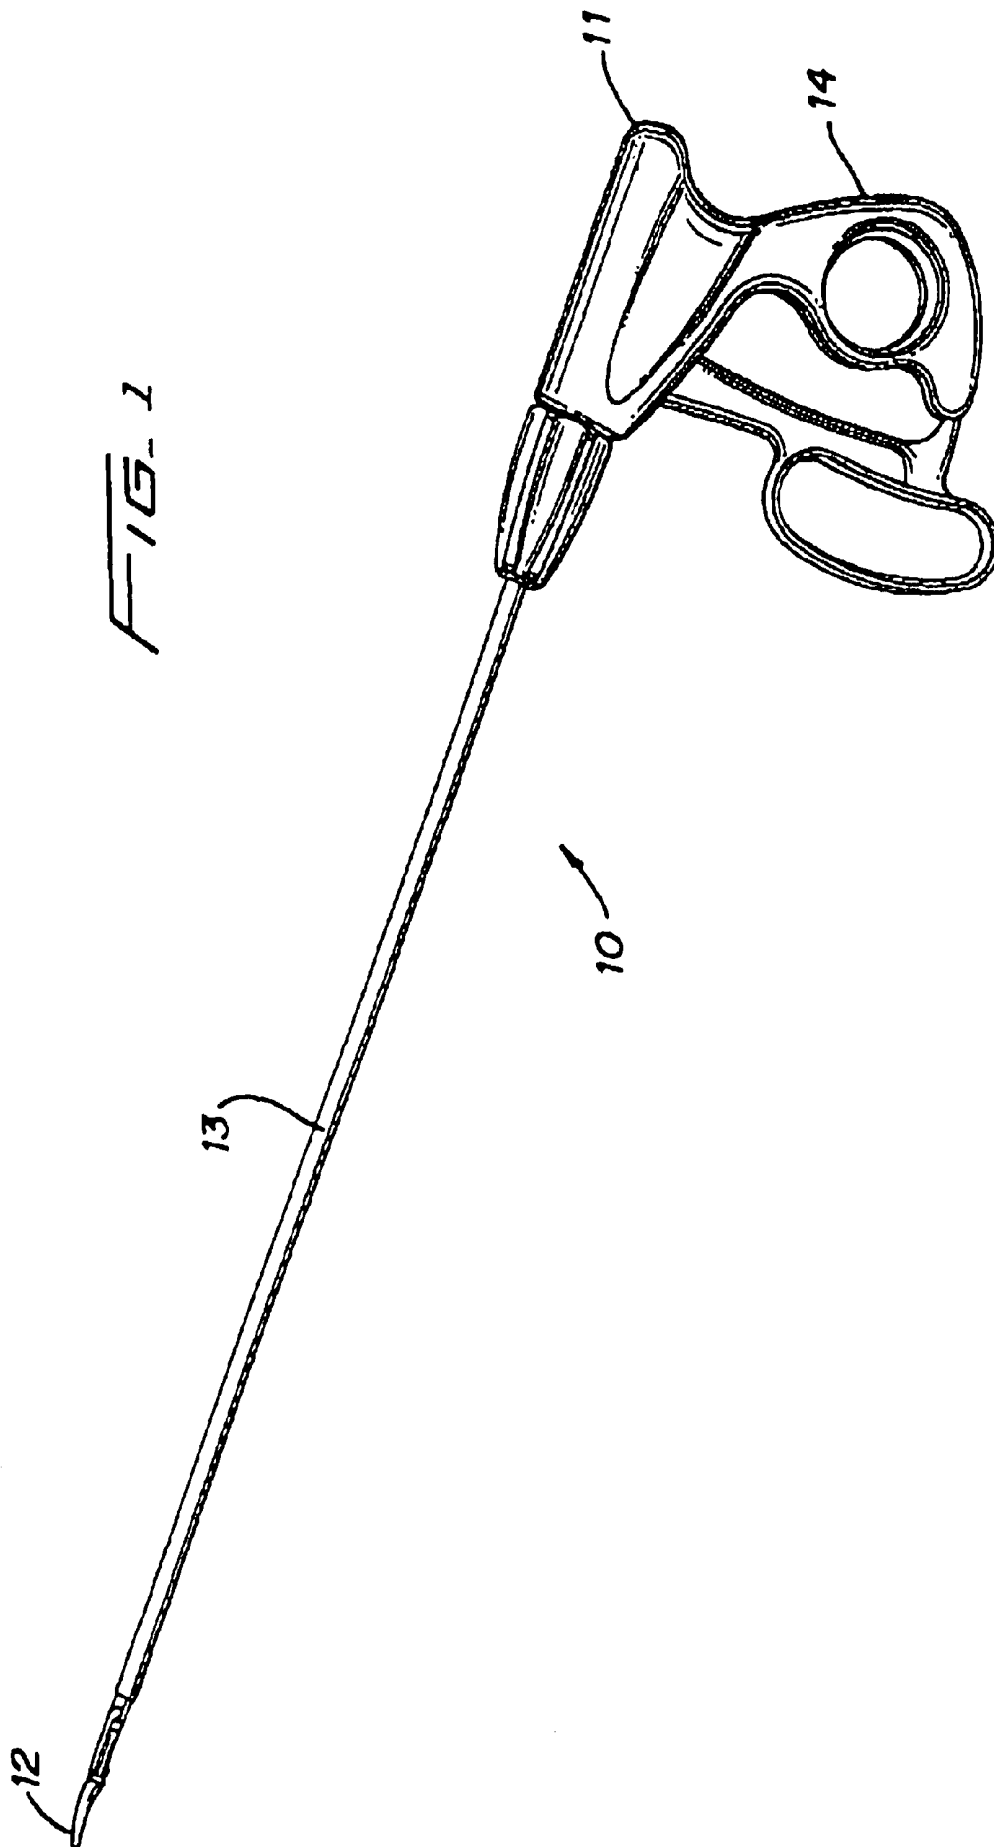

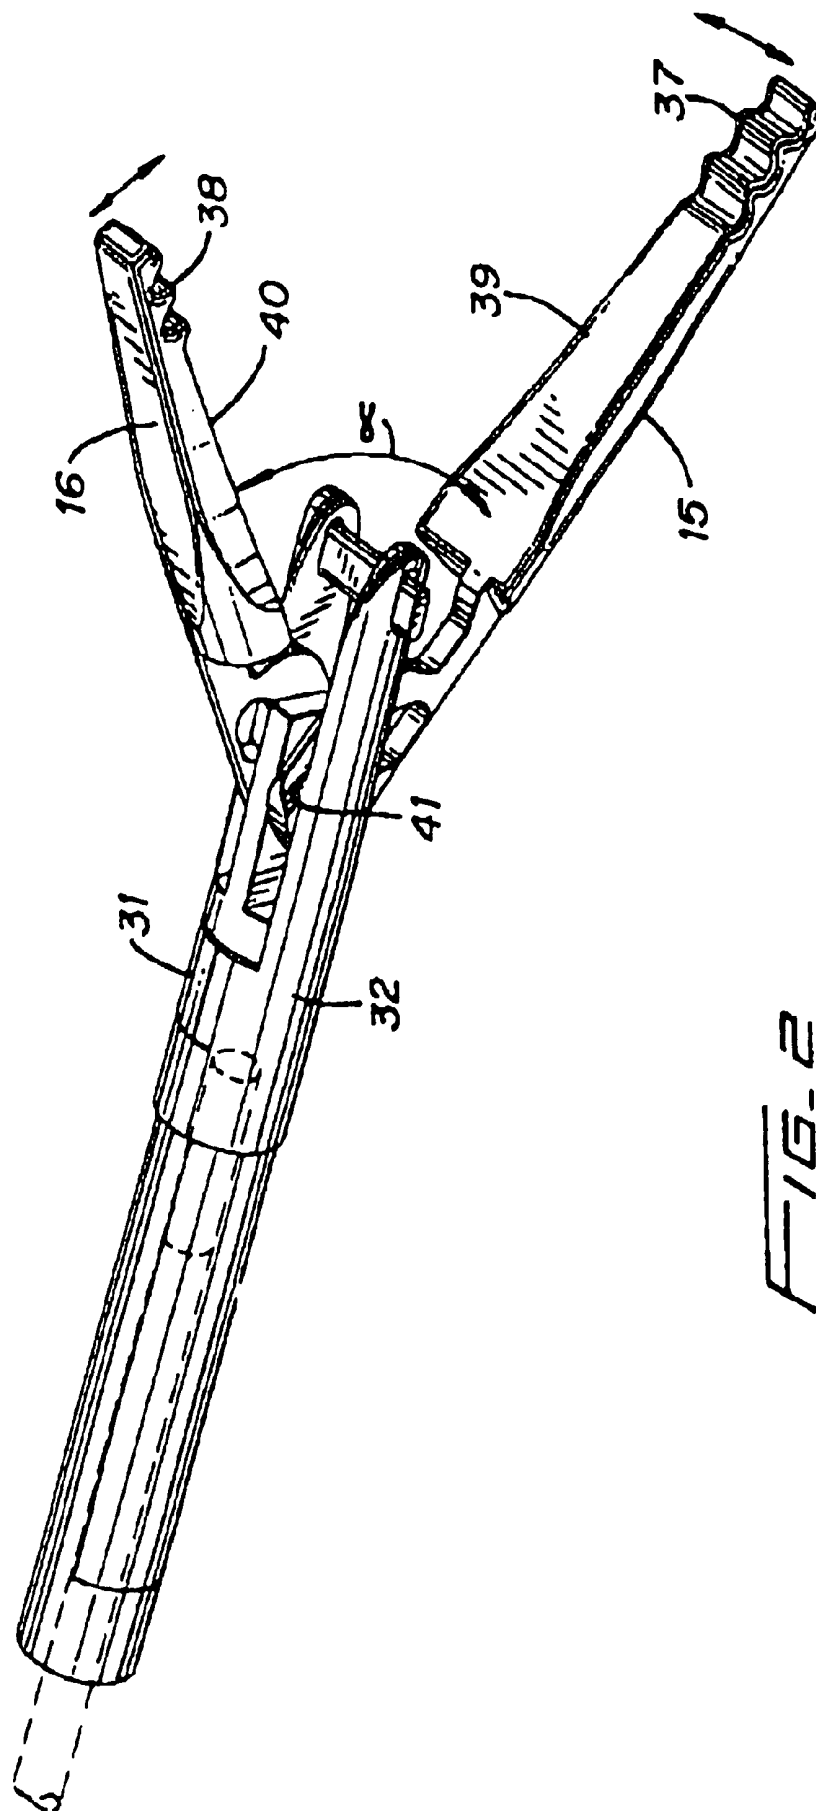


FIG. 2

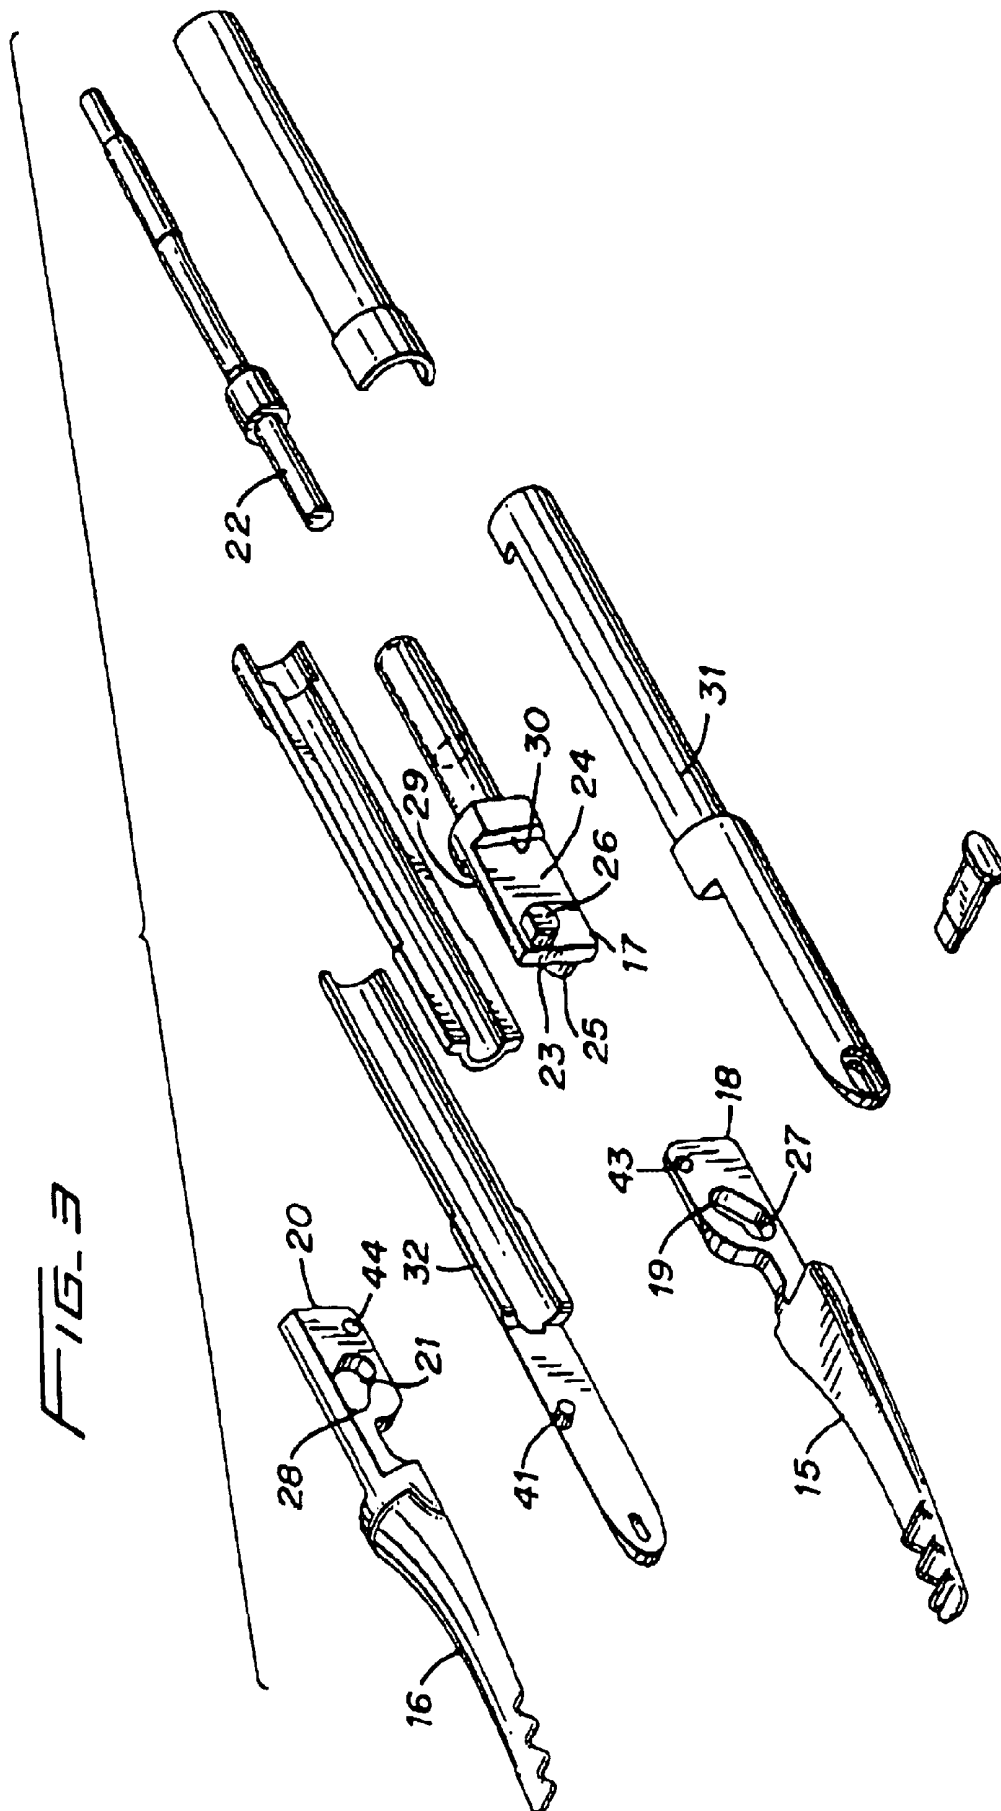


FIG. 4

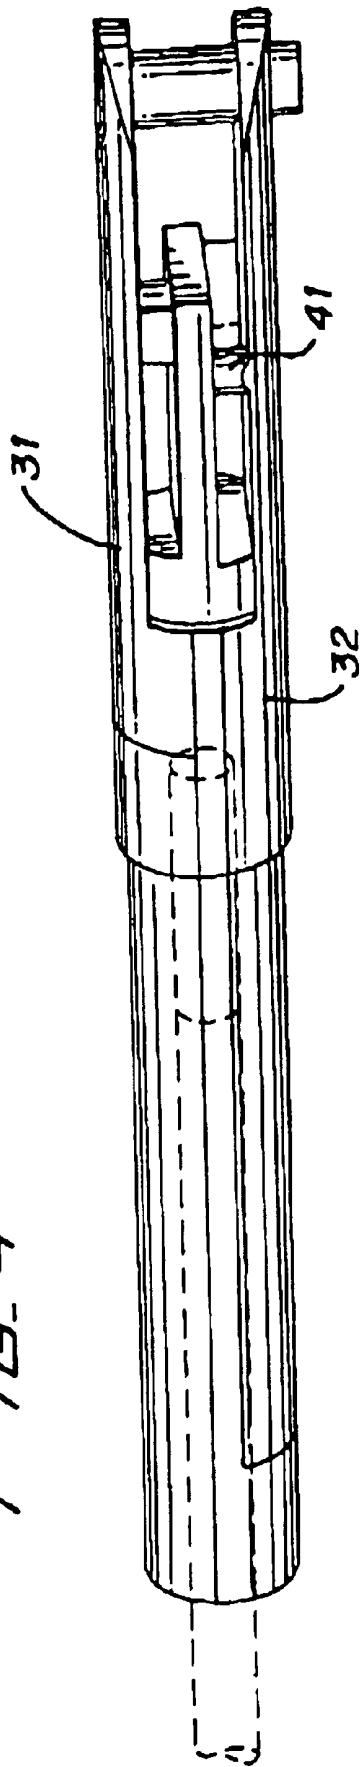


FIG. 5

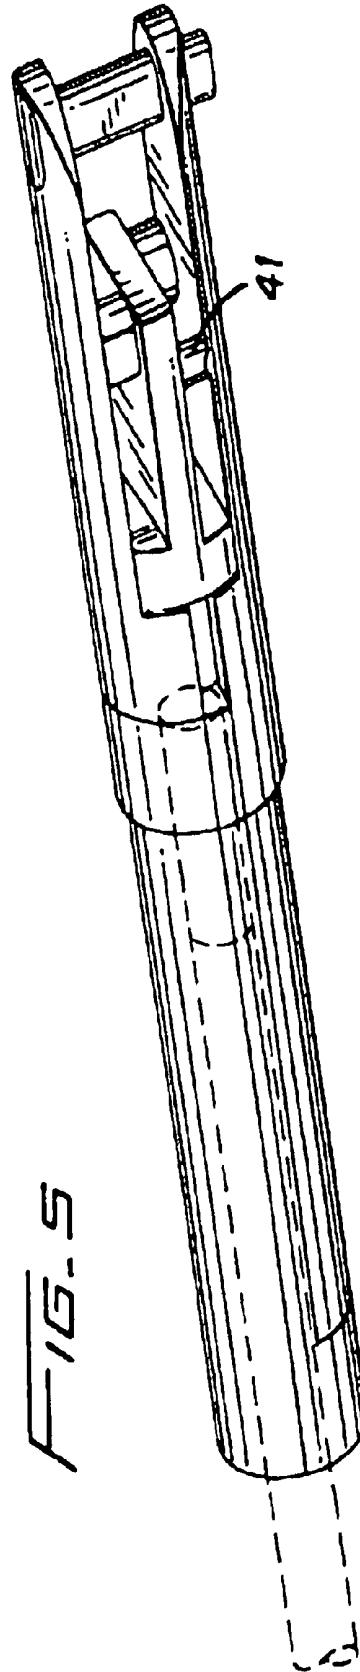


FIG. 6


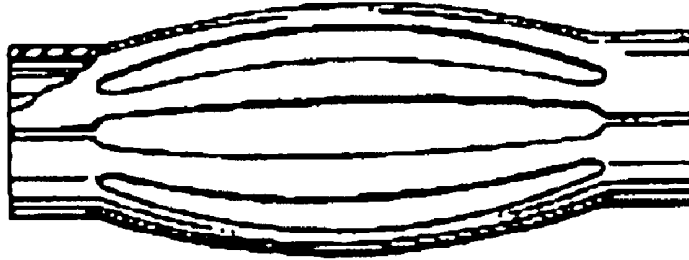


FIG. 7



LAPAROSCOPIC BIPOLAR ELECTROSURGICAL INSTRUMENT

This application is a continuation of U.S. application Ser. No. 09/591,330 filed on Jun. 9, 2000, now U.S. Pat. No. 6,451,018, which is a continuation of U.S. application Ser. No. 08/970,472 filed on Nov. 14, 1997, now U.S. Pat. No. 6,228,083.

FIELD OF THE INVENTION

This relates to an electrosurgical instrument for performing laparoscopic surgical procedures, and more particularly to a laparoscopic electrosurgical instrument that is capable of grasping vessels and vascular tissue with sufficient force between two bipolar jaws to seal the vessel or vascular tissue.

BACKGROUND OF THE DISCLOSURE

Laparoscopic surgical instruments are used to perform surgical operation without making large incisions in the patient. The laparoscopic instruments are inserted into the patient through a cannula, or port, that has been made with a trocar. Typical sizes for cannulas range from three millimeters to twelve millimeters. Smaller cannulas are usually preferred, and this presents a design challenge to instrument manufacturers who must find ways to make surgical instruments that fit through cannulas.

Certain surgical procedures require cutting blood vessels or vascular tissue. This sometimes presents a problem for surgeons because it is difficult to suture blood vessels using laparoscopic tools. Very small blood vessels, in the range below two millimeters in diameter, can often be closed using standard electrosurgical Techniques. If a larger vessel is severed, it may be necessary for the surgeon to convert the laparoscopic procedure into an open-surgical procedure and thereby abandon the benefits of laparoscopy.

Several journal articles have disclosed methods for sealing small blood vessels using electrosurgery. An article entitled *Studies on Coagulation and the Development of an Automatic Computerized Bipolar Coagulator*, J. Neurosurg., Volume 75, Jul. 1991, describes a bipolar coagulator which is used to seal small blood vessels. The article states that it was not possible to safely coagulate arteries with a diameter larger than 2 to 2.5 mm. A second article entitled *Automatically Controlled Bipolar Electrocoagulation—"COA—COMP"*, Neurosurg. Rev. (1984), pp.187-190. This article describes a method for terminating electrosurgical power to the vessel so that charring of the vessel walls can be avoided.

It has been recently determined that electrosurgical methods may be able to seal larger vessels using an appropriate electrosurgical power curve, coupled with an instrument capable of applying a large closure force to the vessel walls. It is thought that the process of coagulating small vessels is fundamentally different than electrosurgical vessel sealing. Coagulation is defined as a process of desiccating tissue wherein the tissue cells are ruptured and dried. Vessel sealing is defined as the process of liquefying the collagen in the tissue so that it crosslinks and reforms into a fused mass. Thus, coagulation of small vessels is sufficient to permanently close them. Larger vessels need to be sealed to assure permanent closure.

It would be desirable to have a surgical tool capable of applying electrosurgical energy, capable of applying a large closure force to the vessel walls, and also capable of fitting through a cannula. A large closure force between the jaws typically requires a large moment about the pivot for each

jaw. This presents a challenge because the first and second pins have a small moment arm with respect to the pivot of each jaw. A large force, coupled with a small moment arm, is undesirable because the large forces may shear the first and second pins. It is also undesirable to increase the moment arm of the first and second pins because the physical size of the yoke might not fit through a cannula.

Several bipolar laparoscopic instruments are known. For example, U.S. Pat. No. 3,938,527 discloses a bipolar laparoscopic instrument for tubal cauterization. U.S. Pat. No. 5,250,047 discloses a bipolar laparoscopic instrument with a replaceable electrode tip assembly. U.S. Pat. No. 5,445,638 discloses a bipolar coagulation and cutting forceps with first and second conductors extending from the distal end. U.S. Pat. No. 5,391,166 discloses a bipolar endoscopic instrument having a detachable working end. U.S. Pat. No. 5,342,359 discloses a bipolar coagulation device.

The present invention solves the problem of providing a large closure force between the jaws of a laparoscopic bipolar electrosurgical instrument, using a compact design that fits through a cannula, without risking structural failure of the instrument yoke.

SUMMARY OF THE INVENTION

The present invention is an instrument for applying bipolar electrosurgical current to tissue in a laparoscopic operation with the added benefit of providing a large closure force between the instrument jaws. The large closure force may be particularly useful for vessel sealing operations. An advantage of the present invention is that tissue can be grasped and clamped with a relatively large closure force without damage to the yoke. The yoke is capable of transmitting the large closure force to the instrument jaws while being small enough to fit through a cannula.

The laparoscopic bipolar electrosurgical instrument comprises first and second jaws having, respectively, first and second flanges with first and second slots. The instrument is electrically connected to an electrosurgical generator, and conducts bipolar electrosurgical current to the first and second jaws. A yoke is attached to a pushrod and positioned to electrically insulate the first flange from the second flange. First and second pins on the yoke are designed to engage the first and second slots, respectively, in a cam-follower arrangement that opens and closes the jaws with linear motion of the yoke. The yoke is preferably a "push yoke" which means that linear motion of the yoke in the direction of the distal end of the instrument will cause the jaws to close together.

The yoke has first and second shoulders that are spaced apart from the first and second flanges until the jaws are in close arcuate proximity to each other. At that point, the first and second shoulders engage the first and second flanges, whereby further distal motion of the yoke applies a force to the first and second flanges that creates a moment about the pivot of each jaw. In general, the cam-follower arrangement of pins and slots may be designed to provide coarse motion of the jaws with relatively small forces. Large closure forces, once the jaws are relatively close together, may be obtained by pressing the shoulders against the flanges. The first and second pins move into cul-de-sacs in the first and second slots to protect them from large shear stresses when the shoulders are applying relatively large forces to the flanges. Thus, the first and second pins may be made from an electrically insulative material that is not designed to handle large shear stresses, large closure forces may be obtained, and the entire assembly may be compact and fit through a cannula.

A method of making the laparoscopic bipolar electrosurgical instrument is described, comprising the following steps: forming a first jaw having a first flange with a first slot, and a second jaw having a second flange with a second slot; attaching the yoke to a pushrod; electrically insulating the first flange from the second flange with the yoke; engaging first and second pins with the first and second slots; positioning first and second cul-de-sacs respectively in the first and second slots to relieve shear stresses on the first and second pins at a subtended angle and approximately wherein first and second shoulders engage the first and second flanges.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a perspective view of a laparoscopic bipolar electrosurgical instruments.

FIG. 2 is a perspective view of the distal end and jaws of the instrument in FIG. 1.

FIG. 3 is an exploded view of the distal end shown in FIG. 2.

FIG. 4 is perspective view of the distal end of the instrument with the jaws removed.

FIG. 5 is another perspective of FIG. 4.

FIG. 6 is a side view of an electrical spring contact.

FIG. 7 is a front view of the spring contact shown in FIG. 6.

DETAILED DESCRIPTION OF THE INVENTION

A laparoscopic bipolar electrosurgical instrument 10 is shown in FIG. 1. The instrument 10 has a proximal end 11 with a handle 14 for holding and manipulating the instrument 10. A distal end 12 on the instrument 10 is used for surgical manipulation of tissue. The instrument 10 comprises an elongate tube 13 that is sized to fit through a cannula for laparoscopic operations, and in different embodiments may be sized to fit through either a five or seven millimeter cannula.

A portion of the distal end 12 of the instrument 10 is shown in FIG. 2. A first jaw 15 and a second jaw 16 are shown in an open position. An angle α is subtended by the jaws 15 and 16. Closing of the jaws 15 and 16 is defined as reduction of the angle α subtended by the jaws 15 and 16. Similarly, opening of the jaws 15 and 16 is defined as an enlargement of the angle α . The angle α is zero when the jaws 15 and 16 are closed together. The center of rotation for the first jaws 15 is at the first pivot 41, and the center of rotation for the second jaw 16 is at the second pivot 42. The first pivot 41 is located on an outer nose piece 32, and fits in a first pivot hole 43 located on the first flange 18. The second pivot 42 is located on an inner nose piece 31, and fits in a second pivot hole 44 located on the second flange 20.

Pieces that comprise the distal end 12 of the instrument 10 are shown in an exploded view in FIG. 3. The first jaw 15 and the second jaw 16 are shown separated from a yoke 17. The first jaw 15 has a first flange 18 and a first slot 19 therewithin. The second jaw 16 has a second flange 20 and a second slot 21 therewithin. Each jaw 15 and 16 is preferably formed from a single piece of stainless steel or other electrically conductive material.

Referring again to FIG. 3, the yoke 17 is attached to a pushrod 22. The yoke 17 is preferably formed from an electrically insulative material such as plastic. A first side 23 of the yoke 17 faces the first flange 18. A second side 24 of the yoke 17 faces the second flange 20. When the yoke 17

is positioned between the flanges 18 and 20, the yoke 17 also acts to electrically insulate the first jaw 15 from the second jaw 16. In this manner, bipolar electrosurgical current can be conducted through tissue grasped by the jaws 15 and 16 without short circuiting between the flanges 18 and 20.

A first pin 25 is located on the first side 23 to movably engage with the first slot 19. Similarly, a second pin 26 is located on the second side 24 to movably engage with the second slot 21. Each pin and slot combination works as a cam-follower mechanical linkage. Motion of the pushrod 22 moves the yoke 17 causing pins 25 and 26 to slide within their respective slots 19 and 21. The slots 19 and 21 are angled with respect to the distal ends of the jaws 15 and 16 such that the jaws 15 and 16 move in an arcuate fashion toward and away from each other. The pins 25 and 26 are different from the pivots 41 and 42. The pins 25 and 26 provide a force against the walls of the slots 19 and 21, creating a moment about the pivots 41 and 42.

The slots 19 and 21 are arranged such that distal motion of the pushrod 22 causes the jaws 15 and 16 to move together. Distal motion of the pushrod 22 is defined as motion in the direction of the distal end 12 of the instrument 10. Once the jaws 15 and 16 are closed together, the present invention holds the jaws 15 and 16 together with a compressive force on the pushrod 22.

One of the advantages of this invention is that shear forces on the pins 25 and 26 can be offloaded to prevent mechanical failure when large forces are being transmitted to the jaws 15 and 16. Each slot 19 and 20 has a cul-de-sac 27 and 28, respectively, as shown in FIG. 3. The first cul-de-sac 28 is an enlargement of the second slot 21 near its distal end. The cam-follower motion of the pins 25 and 26 in the slots 19 and 21 will bring the pins 25 and 26 into their respective cul-de-sac 27 and 28. This position of the pins 25 and 26 leaves a very small moment arm between the pins 25 and 26 and the pivots 41 and 42. The yoke 17 has shoulders 29 and 30 that can provide a relatively large moment about the pivots 41 and 42 to effect a high closure force between the jaws 15 and 16 without a high shear forces on the pins 25 and 26, as described below.

Once the pins 25 and 26 are in the cul-de-sacs 27 and 28, the force from the yoke is transmitted to the flanges 18 and 20 by a first shoulder 29 and a second shoulder 30. The shoulders 29 and 30 abut the proximal end of the flanges 18 and 20 to cause the jaws 15 and 16 to close together. The pivots 41 and 42 are preferably made of metal and can withstand relatively high shear forces. In contrast, pins 25 and 26 are preferably made of plastic and will break under relatively high shear forces. Thus, the shoulders 29 and 30 provide a moment about the pivots 41 and 42, thereby avoiding the necessity of applying high shear forces to the pins 25 and 26 when the moment arm from the pins 25 and 26 would be small. There is an angle α at which the pins 25 and 26 enter their respective cul-de-sacs 27 and 28 and the shoulders 29 and 30 abut the flanges 18 and 20. Then angle α at which the forgoing occurs is preferably around three degrees.

The bipolar electrosurgical instrument 10 has first and second poles of alternating potential that are conducted along the instrument 10 and through tissue that is grasped between the jaws 15 and 16. The first pole is conducted from the proximal end 11 toward the distal end 12 along the pushrod 22. The second pole is conducted from the proximal end 11 toward the distal end 12 along the tube 13. The outer surface of the tube 13 is preferably coated with an electrically insulative material. There is also preferably an elec-

5

trically insulative barrier between the pushrod 22 and the tube 13 to prevent short circuits in the instrument 10.

In the preferred embodiment, the distal end of the instrument 10 comprises an inner nose piece 31 and an outer nose piece 32, as shown in FIG. 2. The inner nose piece 31 is electrically connected with the pushrod 22, while the outer nose piece is electrically connected with tube 13. The inner nose piece 31 and the outer nose piece 32 capture the yoke 17, along with the first and second flanges 18 and 20, as shown in FIG. 2. The yoke 17 moves axially, along an axis defined by the tube, in a space between the inner and outer nose pieces 31 and 32. A spacer 33 maintains the separation of the nose pieces 31 and 32 at their distal ends. The nose pieces 31 and 32 provide lateral support for the flanges 18 and 20 to help ensure that the pins 25 and 26 remain within the slots 19 and 21.

The preferred embodiment also comprises an inner insulator 34 and an outer insulator 35 for maintaining electrical insulation between the poles. The outer insulator 35 is seated between the tube 13 and the inner nose 31, as shown in FIGS. 2 and 4. The inner insulator 34 is seated between the tube 13 and the pushrod 22. In this manner, the outer nose piece 32 can provide electrical continuity between the tube 13 and the second jaw 16, while the inner nose piece 34 can provide electrical continuity between the pushrod 22 and the first jaw 15. Since the pushrod 22 is slidably mounted within the tube 13, the preferred embodiment has a spring contact 36, as shown in FIGS. 6 and 7, mounted on the pushrod 22 to maintain an electrical connection with the inner nose piece 34 during axial motion.

The first and second jaws 15 and 16 each have ridges 37 and 38 at their distal ends that preferably nest together. The jaws 15 and 16 also have seal surfaces 39 and 40, as shown in FIG. 2. The width of the seal surfaces 39 and 40 is a parameter that affects the quality of the surgical outcome. The closure force between the jaws 15 and 16 varies along the length of the seal surfaces 39 and 40, with the largest force at the distal tip and the smallest force at the proximal end of the seal surfaces 39 and 40. It has been found through experimentation that good vessel sealing results are obtained when the closure force in grams divided by the width in millimeters is in the range of 400 to 650. Since the closure force varies with the length of the seal surfaces 39 and 40, it has been found to be advantageous to taper the width of the seal surfaces 39 and 40 along their length, with the widest width at the proximal end and the narrowest width at the distal end. This design allows the jaws 15 and 16 to apply a relatively constant closure force per unit width, preferably 525 grams per millimeter width.

A method of making a laparoscopic bipolar electrosurgical instrument 10 is also herein described. The method comprises the step of forming a first jaw 15 having a first flange 18 with a first slot 19, and a second jaw 16 having a second flange 20 with a second slot 21. The jaws 15 and 16 are preferably formed in a casting process, although it is also possible to machine the jaws 15 and 16 from stock. The casting process may include injecting powdered metal under pressure into a mold, and then applying heat.

Other steps in the method include attaching a yoke 17 to a push rod 22, and electrically insulating the first flange 18 from the second flange 20 with the yoke 17. The yoke 17 is preferably an injection molded plastic part with features including a first shoulder 29 and a second shoulder 30.

During assembly of the distal portion of the instrument 10, steps in the method include engaging a first pin 25 with

6

the first slot 19, and engaging a second pin 26 with the second slot 21. The slots 19 and 21 are shaped such that a subtended angle α between the first and second jaws 15 and 16 decreases with distal motion of the pushrod 17, and the slots 19 and 20 are formed with cul-de-sacs 27 and 28 positioned to relieve shear stresses on the first and second pins 25 and 26 at the subtended angle α approximately wherein the first and second shoulder 29 and 30 engage the first and second flanges 18 and 20.

Further steps in the method comprise: surrounding at least a portion of the pushrod 22 with an electrically conductive tube 13; electrically insulating the tube 13 from the pushrod 22; electrically connecting an inner nose piece 31 to the pushrod 22, and electrically connecting an outer nose piece 32 to the tube 13, wherein the inner nose piece 31 and the outer nose piece 32 capture the yoke 17 along with the first and second flanges 18 and 20 to conduct bipolar electrosurgical current to the first and second jaws 15 and 16. In the preferred embodiment, there is a step of electrically connecting the pushrod 22 and the inner nose piece 31 with a spring contact 36.

The method of making the instrument 10, in some embodiments, includes the step of tapering the width of the seal surfaces 29 and 40 along the length of each of the first and second jaws 15 and 16.

While a particular preferred embodiment has been illustrated and described, the scope of the protection sought is in the claims that follow.

What is claimed is:

1. A bipolar endoscopic instrument, comprising:

a first jaw member adapted to be connected to a first electrical potential and a second jaw member adapted to be connected to a second electrical potential, the first and second jaw members being movable from a first position in spaced relation relative to one another to a second position wherein the first and second jaw members cooperate to conduct bipolar energy through tissue held therebetween;

a yoke which electrically insulates the first and second jaw members during activation, the yoke including:

a pair of pins which initially rotate the first and second jaw members from the first to second positions upon linear reciprocation of the yoke; and

a pair of shoulder portions which are configured to abut the first and second jaw members in the second position and offload pressure on the pins during clamping and sealing of tissue.

2. The bipolar electrosurgical instrument of claim 1 further comprising:

inner and outer nose pieces which are configured to capture the yoke and conduct bipolar electrosurgical energy to the first and second jaw members.

3. The bipolar electrosurgical instrument of claim 1 wherein the first and second jaw members include ridges which nest when the jaw members are disposed in the second position.

4. The bipolar electrosurgical instrument of claim 1 wherein each of the first and second jaw members includes a seal surface which is tapered along its respective length.

5. The bipolar electrosurgical instrument of claim 4 wherein the closure force is approximately constant along a length between the jaw members.

* * * * *

专利名称(译)	腹腔镜双极电外科仪器		
公开(公告)号	US6960210	公开(公告)日	2005-11-01
申请号	US10/243274	申请日	2002-09-13
[标]申请(专利权)人(译)	地政迈克尔·约翰· LUKIANOW STEPHEN WADE LOEFFLER DONALD ROBERT CUNNIGHAM JAMES 史蒂芬 劳斯KATE RYLAND TRIMBERGER 李仁 米切尔MATHEW ERLE KENNEDY 珍妮弗SERAFIN		
申请(专利权)人(译)	地政迈克尔·约翰· LUKIANOW STEPHEN WADE LOEFFLER DONALD ROBERT CUNNIGHAM JAMES 史蒂芬 劳斯KATE RYLAND TRIMBERGER 李仁 米切尔MATHEW ERLE KENNEDY 珍妮弗SERAFIN		
当前申请(专利权)人(译)	COVIDIEN AG		
[标]发明人	LANDS MICHAEL JOHN LUKIANOW STEPHEN WADE LOEFFLER DONALD ROBERT CUNNIGHAM JAMES STEVEN LAWES KATE RYLAND TRIMBERGER II DANIEL LEE MITCHELL MATHEW ERLE KENNEDY JENIFER SERAFIN		
发明人	LANDS, MICHAEL JOHN LUKIANOW, STEPHEN WADE LOEFFLER, DONALD ROBERT CUNNIGHAM, JAMES STEVEN LAWES, KATE RYLAND TRIMBERGER, II, DANIEL LEE MITCHELL, MATHEW ERLE KENNEDY, JENIFER SERAFIN		
IPC分类号	A61B18/14 A61B19/00 A61B18/12		
CPC分类号	A61B18/1445		
审查员(译)	COHEN , LEE S.		
其他公开文献	US20030032956A1		
外部链接	Espacenet USPTO		
摘要(译)			

腹腔镜双极电外科器械可在其钳口之间施加大的闭合力而不损坏小轭组件。该器械包括：第一钳口，具有带有第一槽的第一凸缘；以及第二钳口，具有带有第二槽的第二凸缘，其中第一和第二钳口位于器械的远端并包括导电材料用于在其间传导双极电外科电流；轭连接到推杆并且定位成使第一凸缘与第二凸缘电绝缘，轭具有面向第一凸缘的第一侧和面向第二凸缘的第二侧，轭还包括第一肩部和第二肩部；第一销位于第一侧并可移动地与第一槽接合；第二销位于第二侧并可移动地与第二槽接合；第一狭槽和第二狭槽成形为使得第一和第二钳口对向的角度随着推杆的远侧运动而减小，并且第一和第二穹窿分别定位在第一和第二狭槽中以重现剪切应力当第一和第二肩部分别接合第一和第二凸缘以在第一和第二夹爪之间提供闭合力时，在第一和第二销上。

