


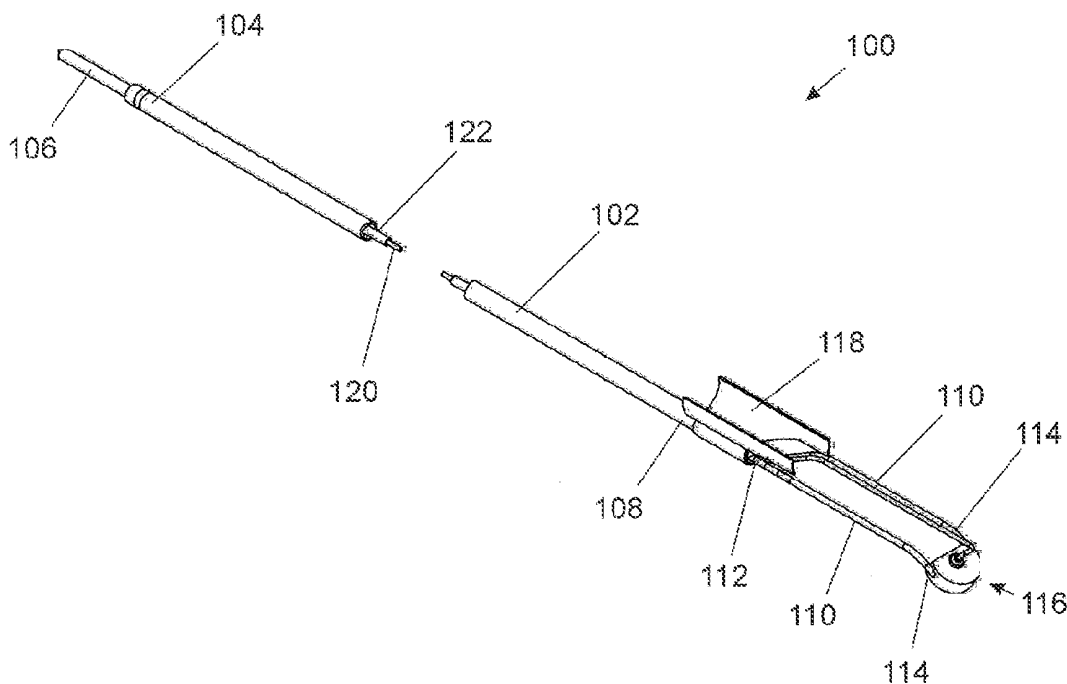

US 20120245578A1

(19) **United States**(12) **Patent Application Publication**
Van Wyk et al.(10) **Pub. No.: US 2012/0245578 A1**(43) **Pub. Date: Sep. 27, 2012**(54) **ELECTROSURGICAL DEVICE HAVING
FLOATING-POTENTIAL ELECTRODE FOR
OBSTRUCTION REMOVAL**(75) Inventors: **Robert A. Van Wyk**, St. Pete
Beach, FL (US); **Yuval Carmel**,
Rockville, MD (US); **Anatoly**
Shkvarunets, Rockville, MD (US)(73) Assignee: **ElectroMedical Associates LLC**,
Bethesda, MD (US)(21) Appl. No.: **13/493,975**(22) Filed: **Jun. 11, 2012****Related U.S. Application Data**(62) Division of application No. 13/451,138, filed on Apr.
19, 2012, which is a division of application No.
11/859,297, filed on Sep. 21, 2007, now Pat. No.
8,177,784.(60) Provisional application No. 60/847,496, filed on Sep.
27, 2006.**Publication Classification**(51) **Int. Cl.**
A61B 18/14 (2006.01)
A61B 18/18 (2006.01)(52) **U.S. Cl.** **606/33; 606/41; 606/46**(57) **ABSTRACT**

Disclosed herein are embodiments of an electrosurgical device that include one or more floating electrodes and are specifically adapted to remove, cut, resect, ablate, vaporize, denaturize, drill, coagulate and form lesions in soft tissues, with or without externally supplied liquids, preferably in combination with a resectoscope, particularly in the context of urological, gynecological, laparoscopic, arthroscopic, and ENT procedures. Specific adaptations for urological and gynecological applications, for example kidney stone removal and BPH treatment, are also described.



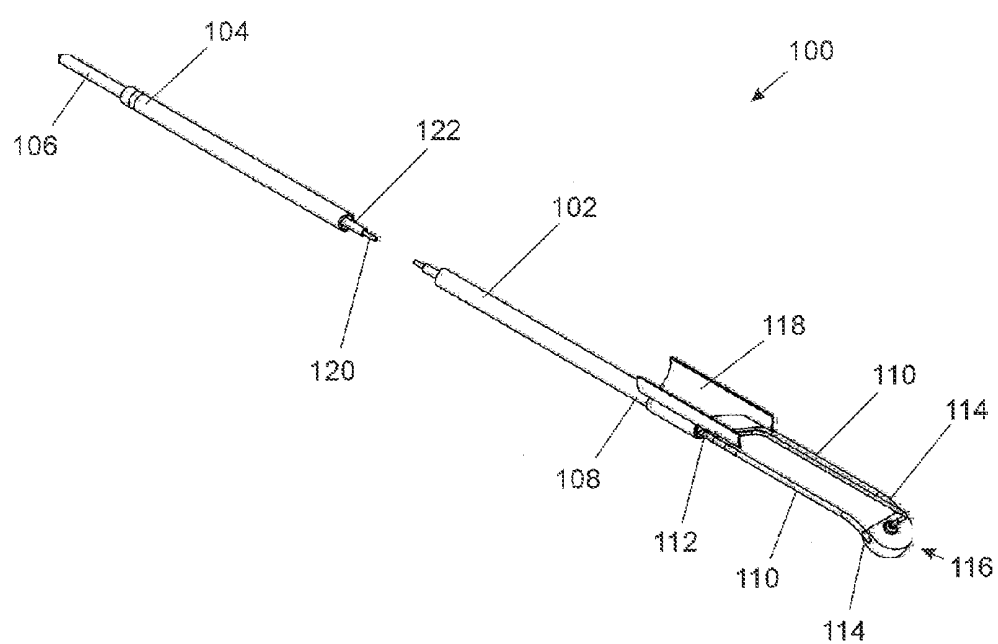


Fig. 1

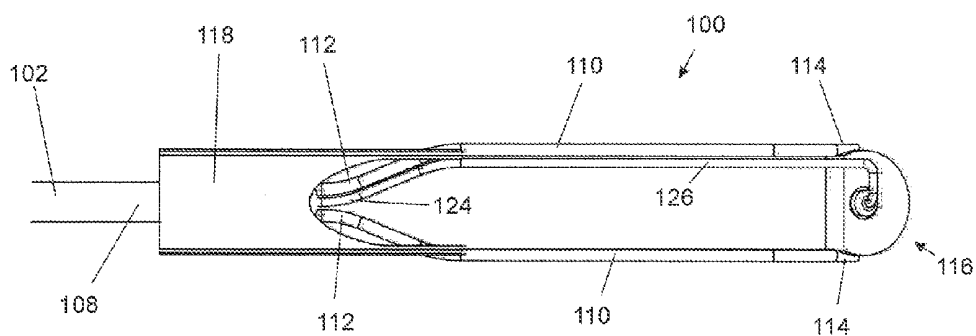


Fig. 2

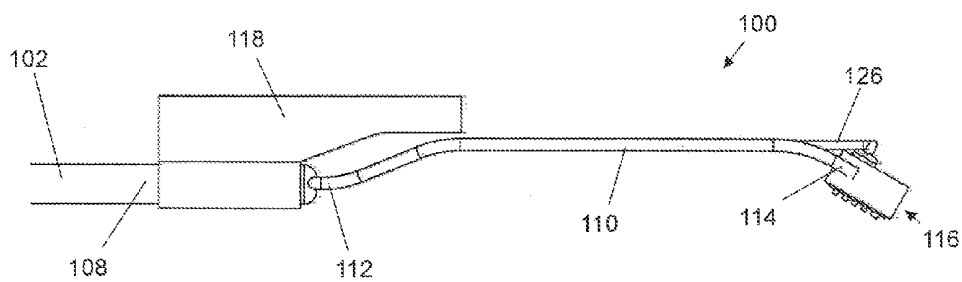


Fig. 3

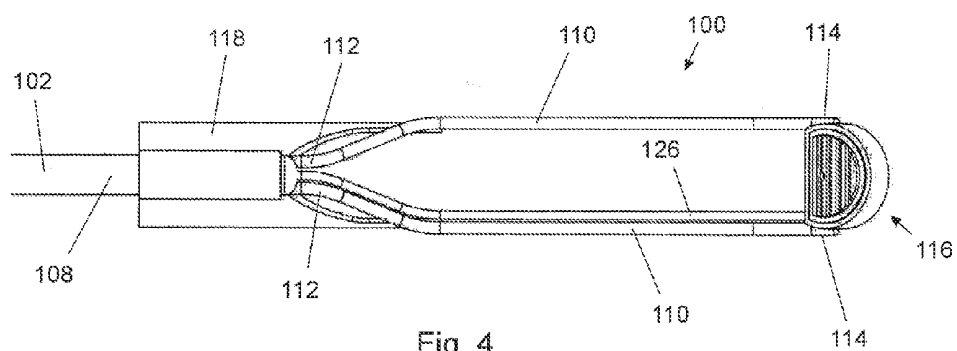
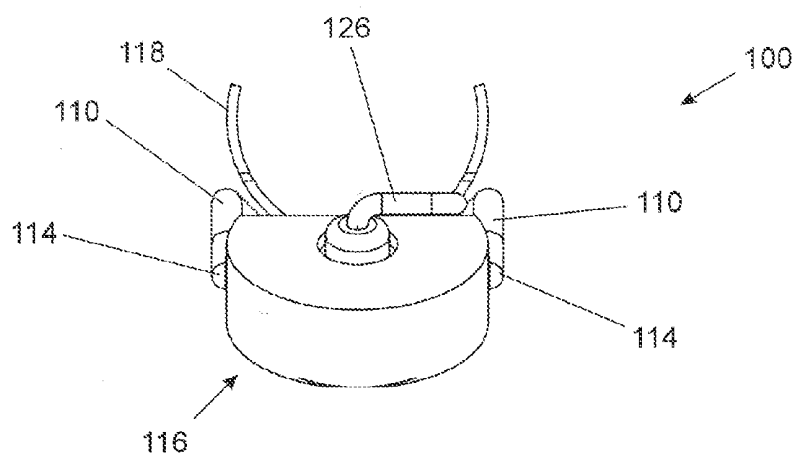
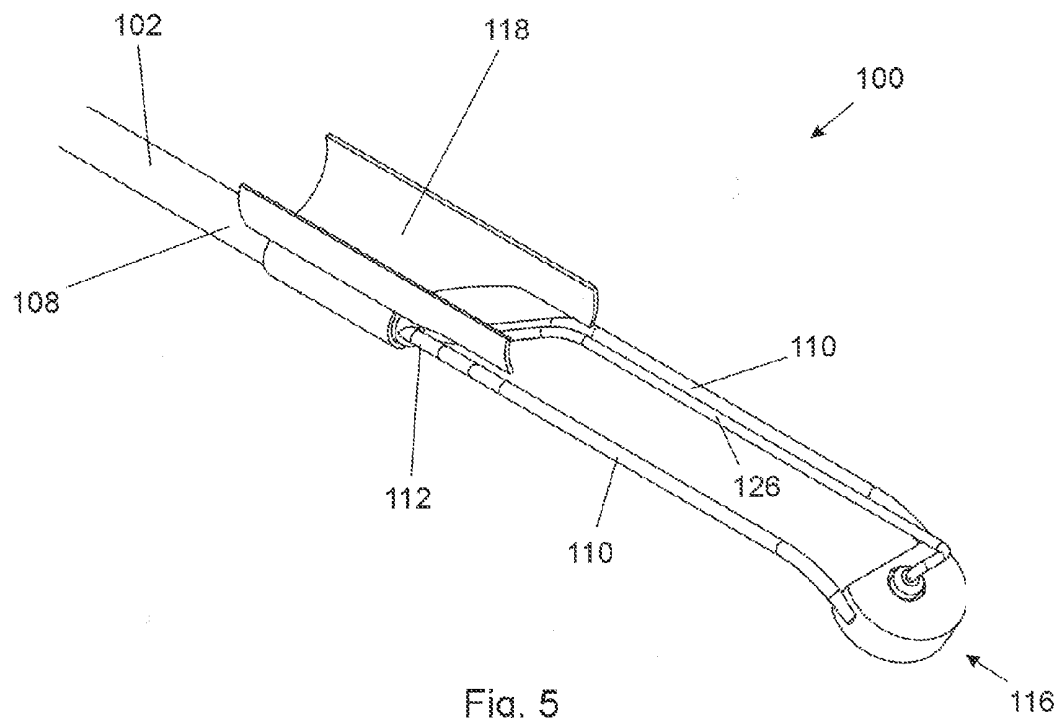


Fig. 4



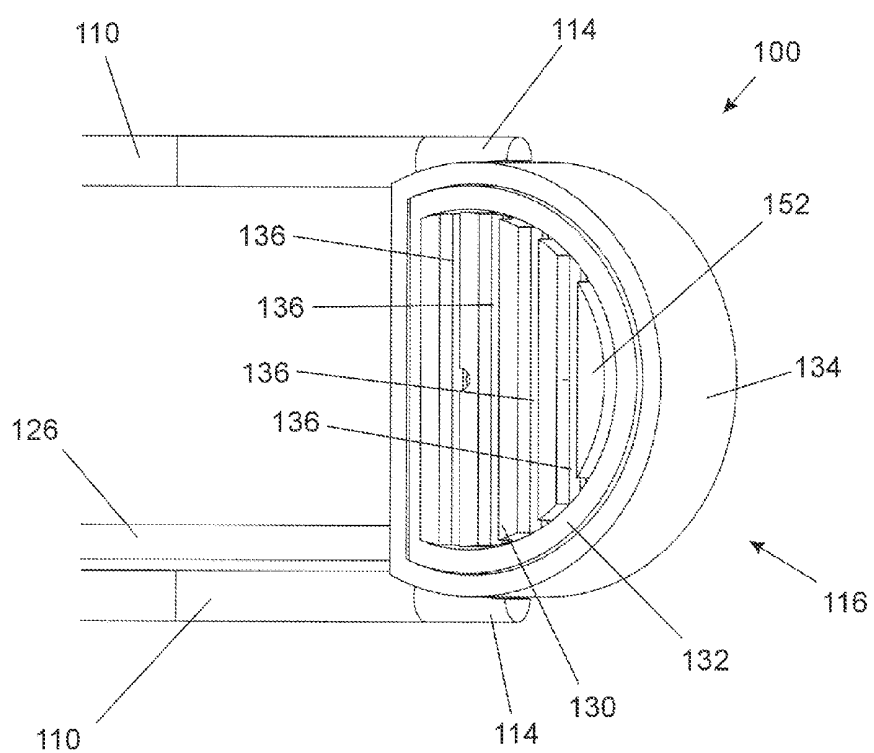


Fig. 7

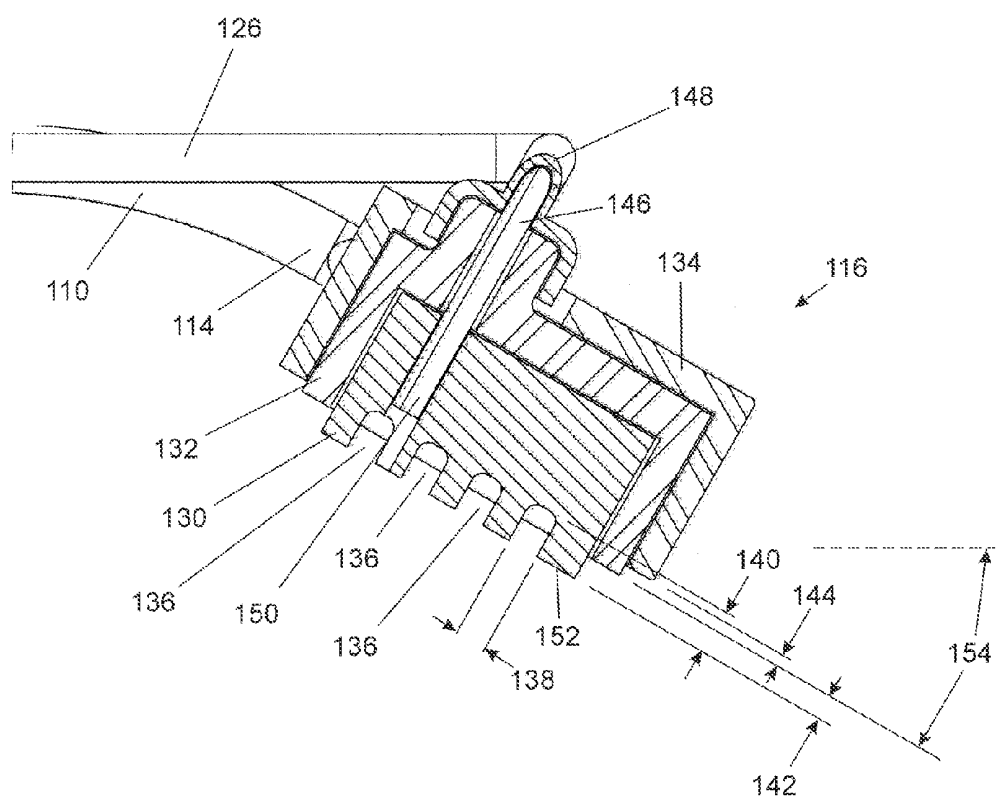


Fig. 8

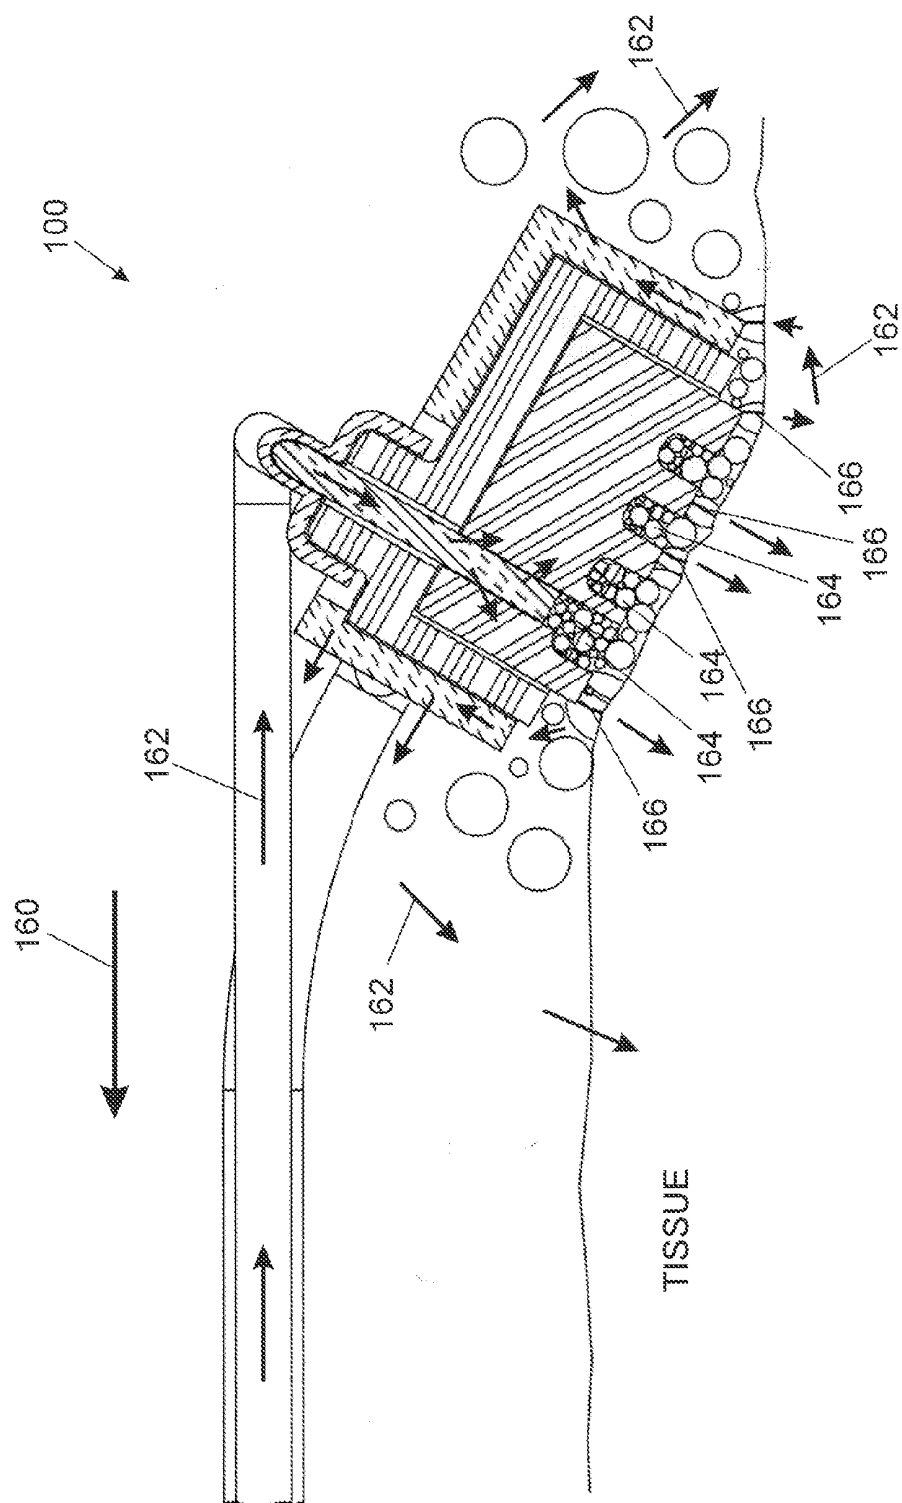


Fig. 9

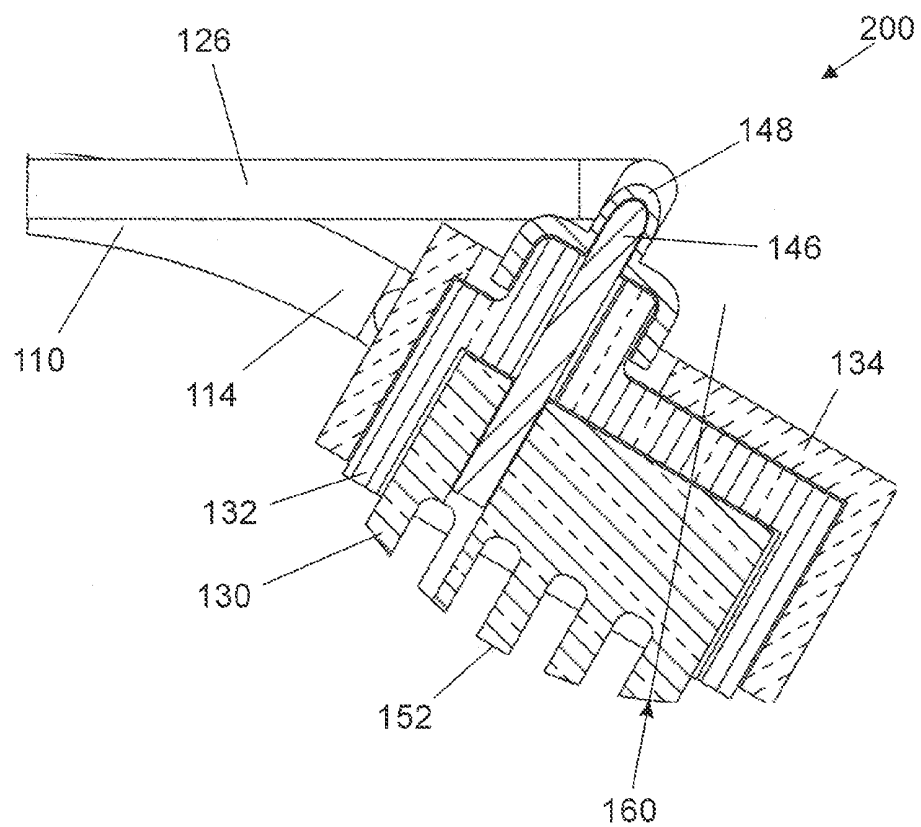


Fig. 10

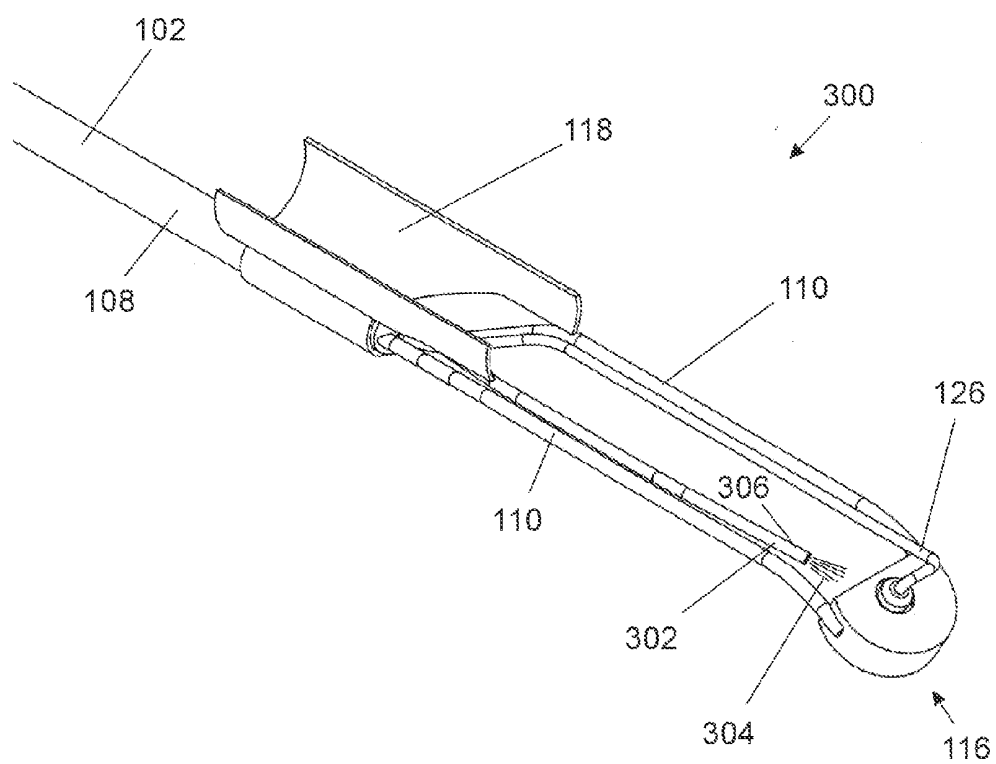


Fig. 11

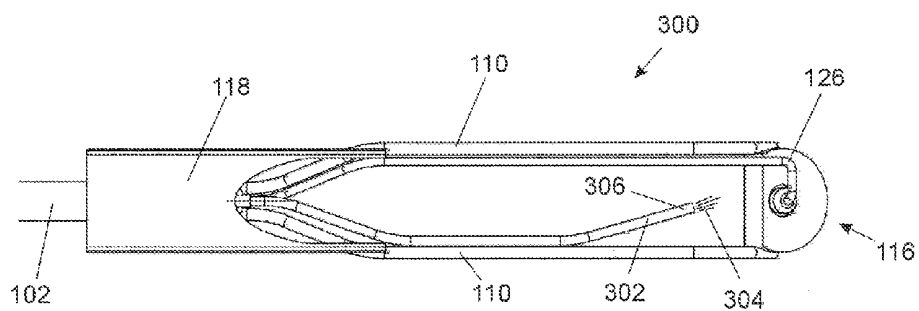


Fig. 12

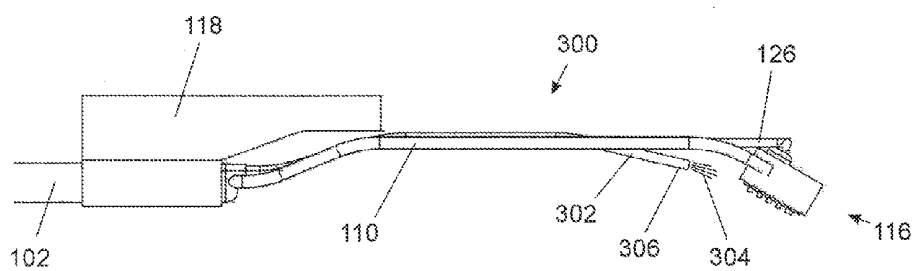


Fig. 13

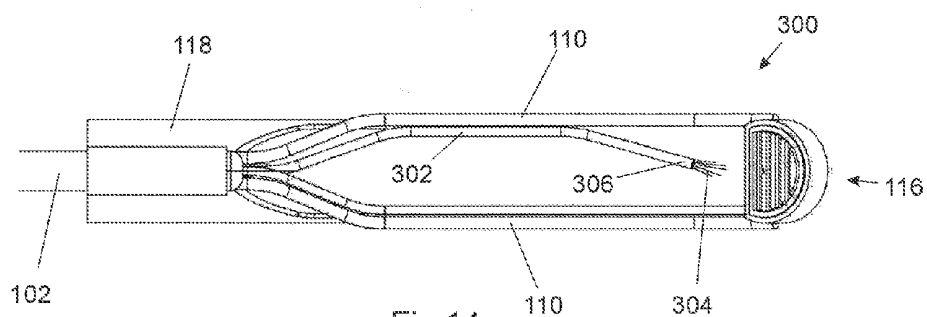


Fig. 14

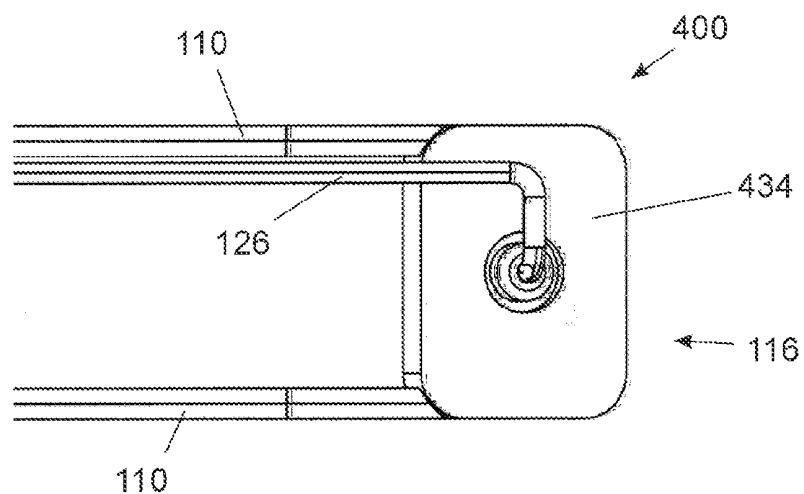


Fig. 15

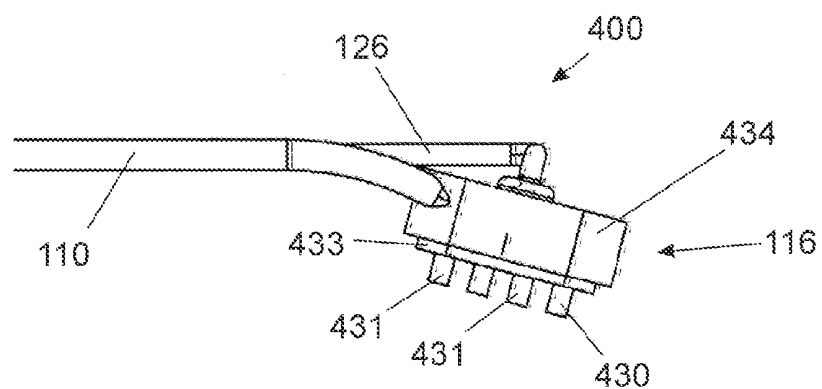


Fig. 16

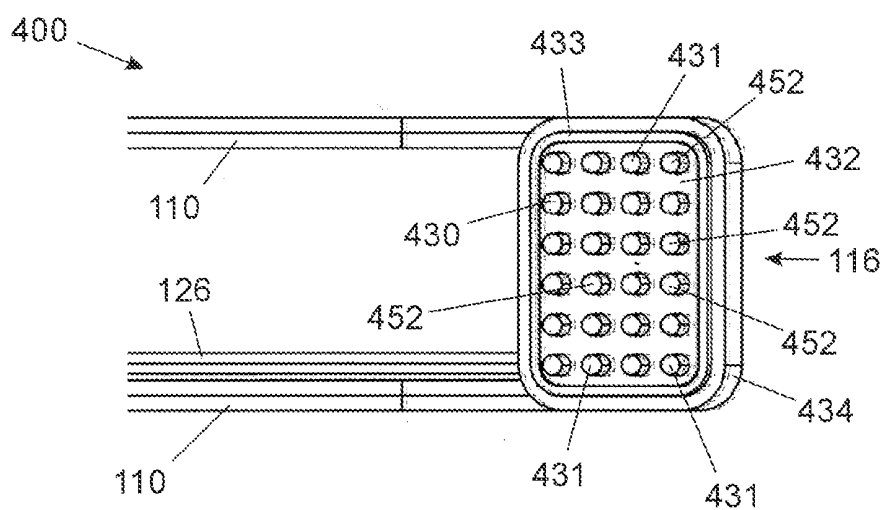


Fig. 17

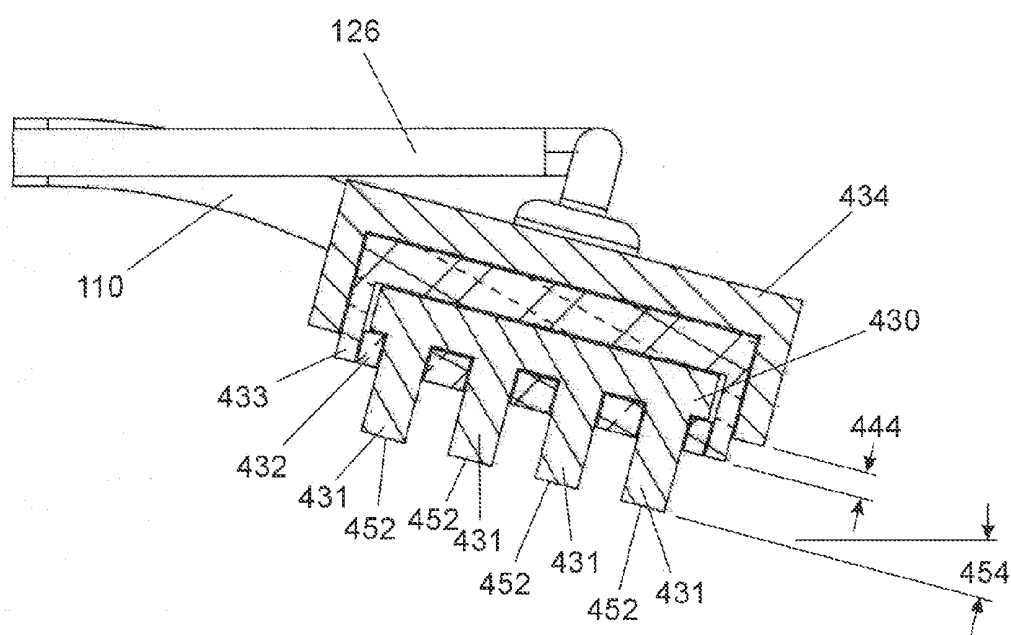


Fig. 18

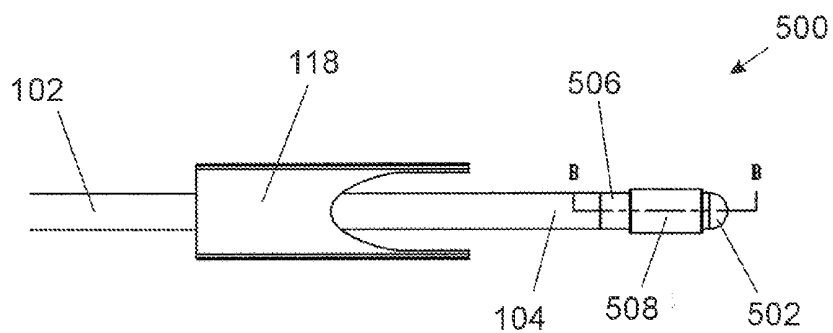


Fig. 19

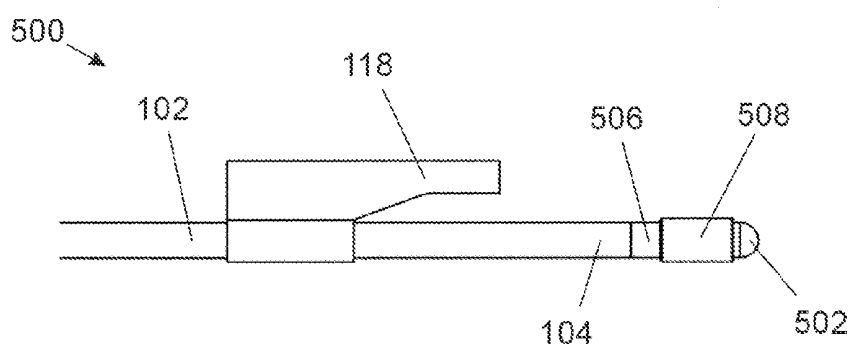


Fig. 20

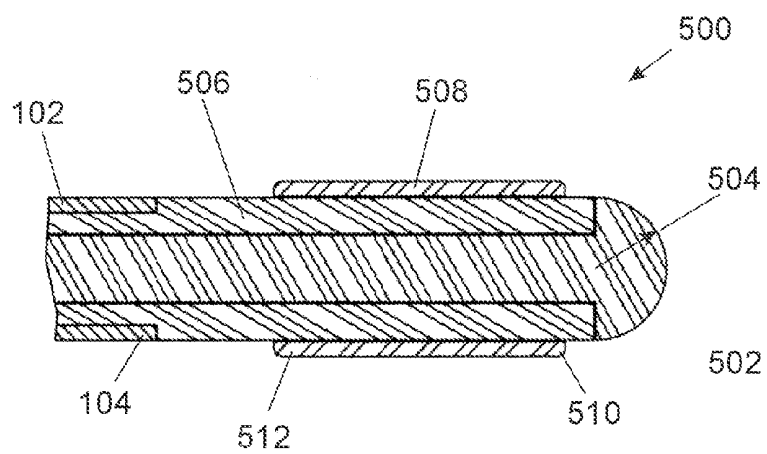


Fig. 21

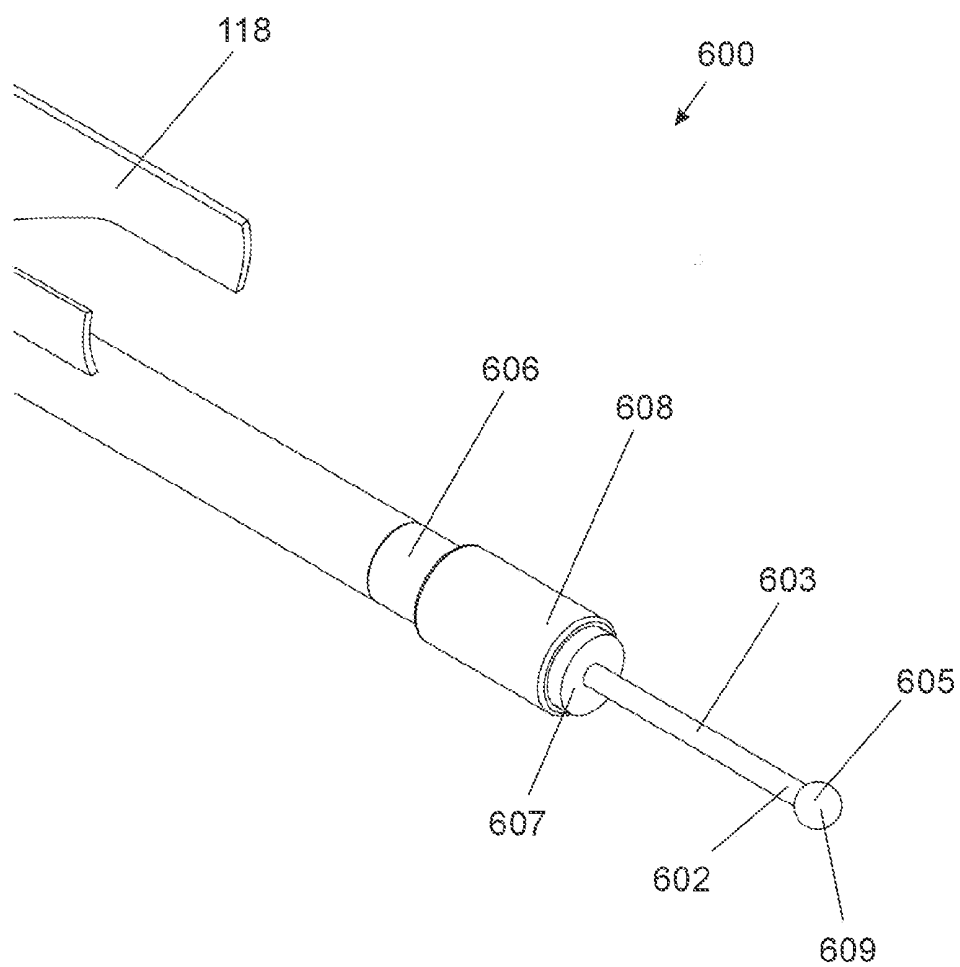


Fig. 22

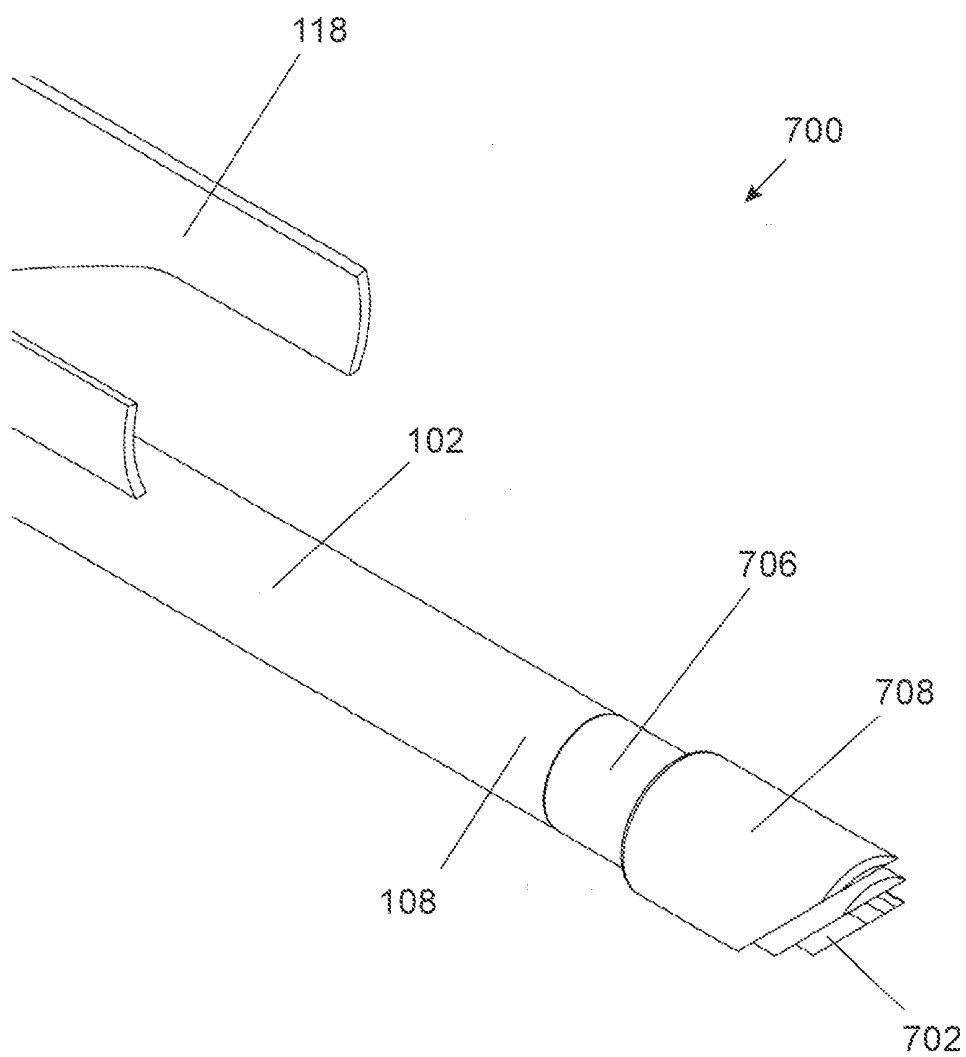


Fig. 23

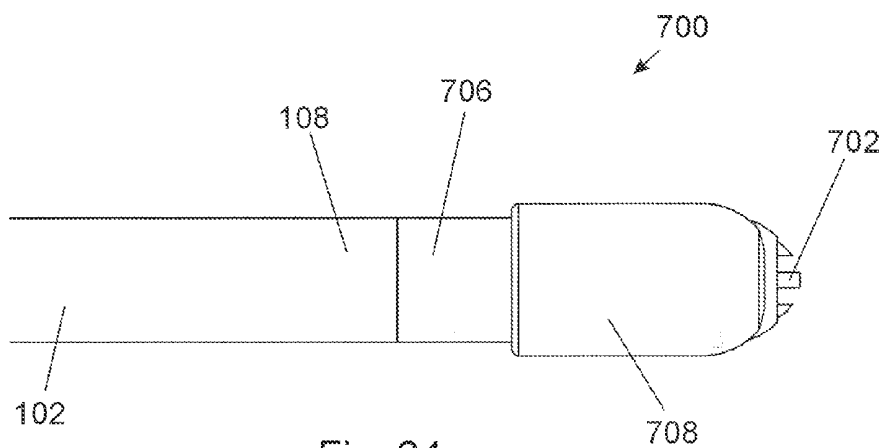


Fig. 24

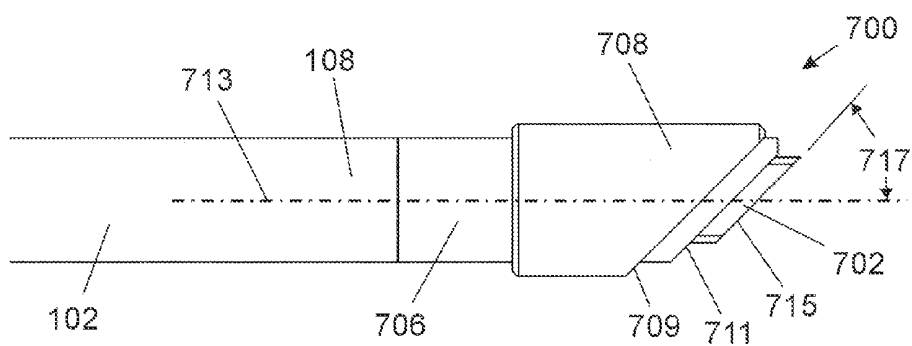


Fig. 25

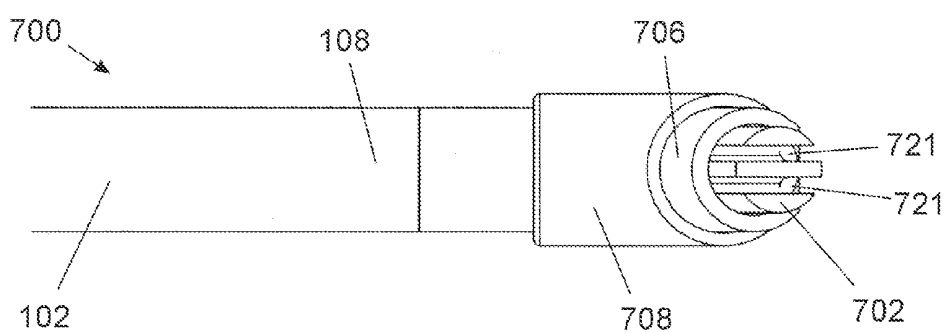


Fig. 26

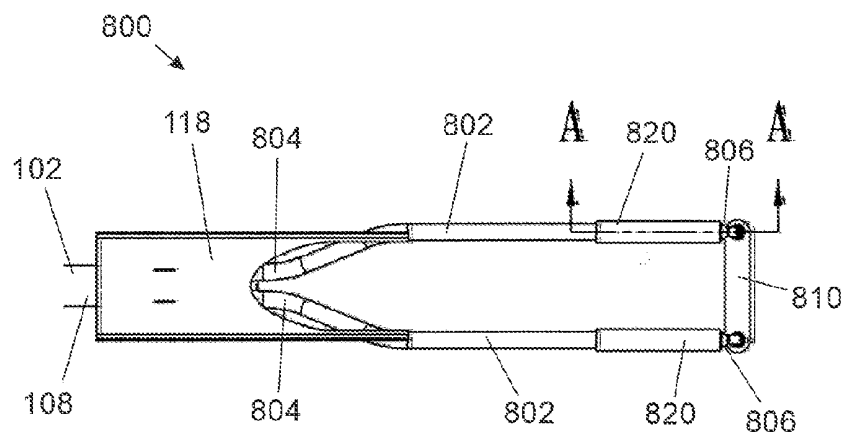


FIG. 27

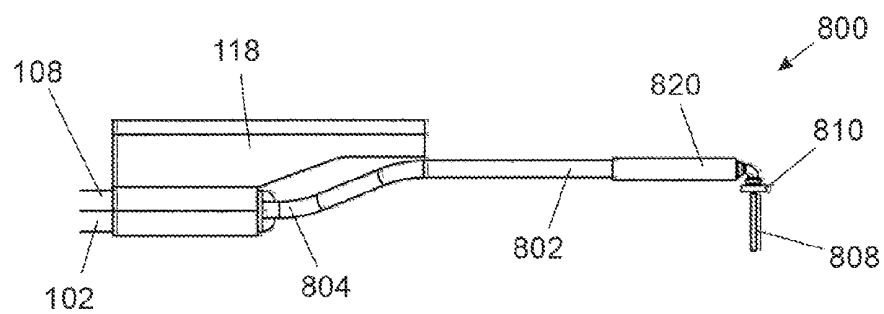


FIG. 28

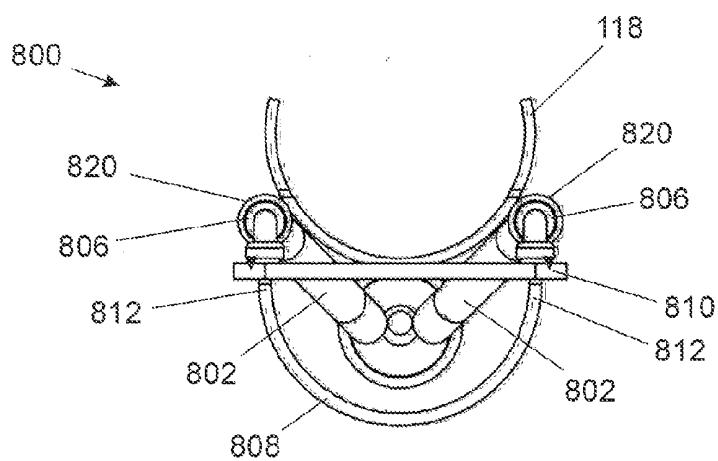


FIG. 29

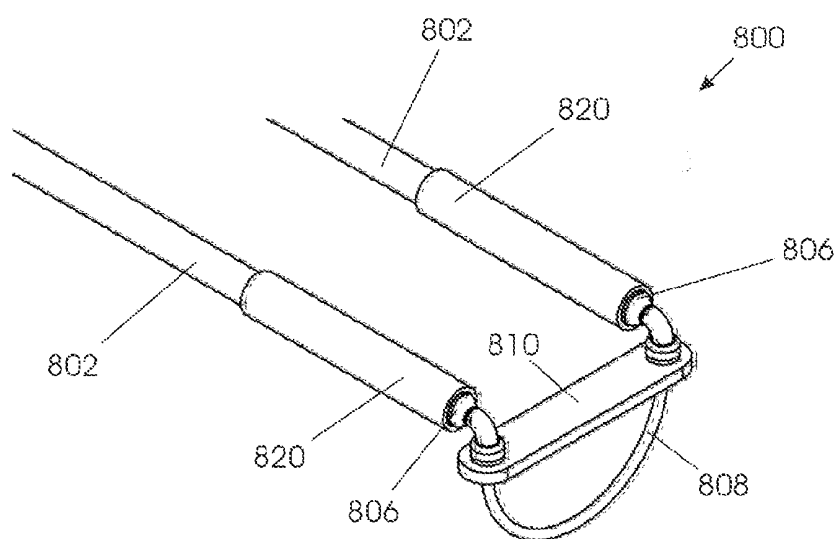


FIG. 30


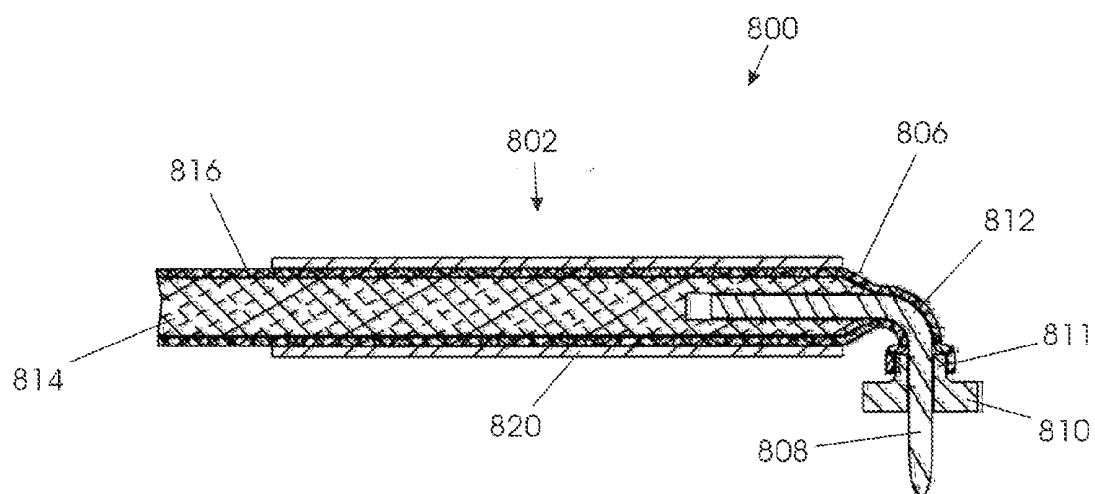


FIG. 31

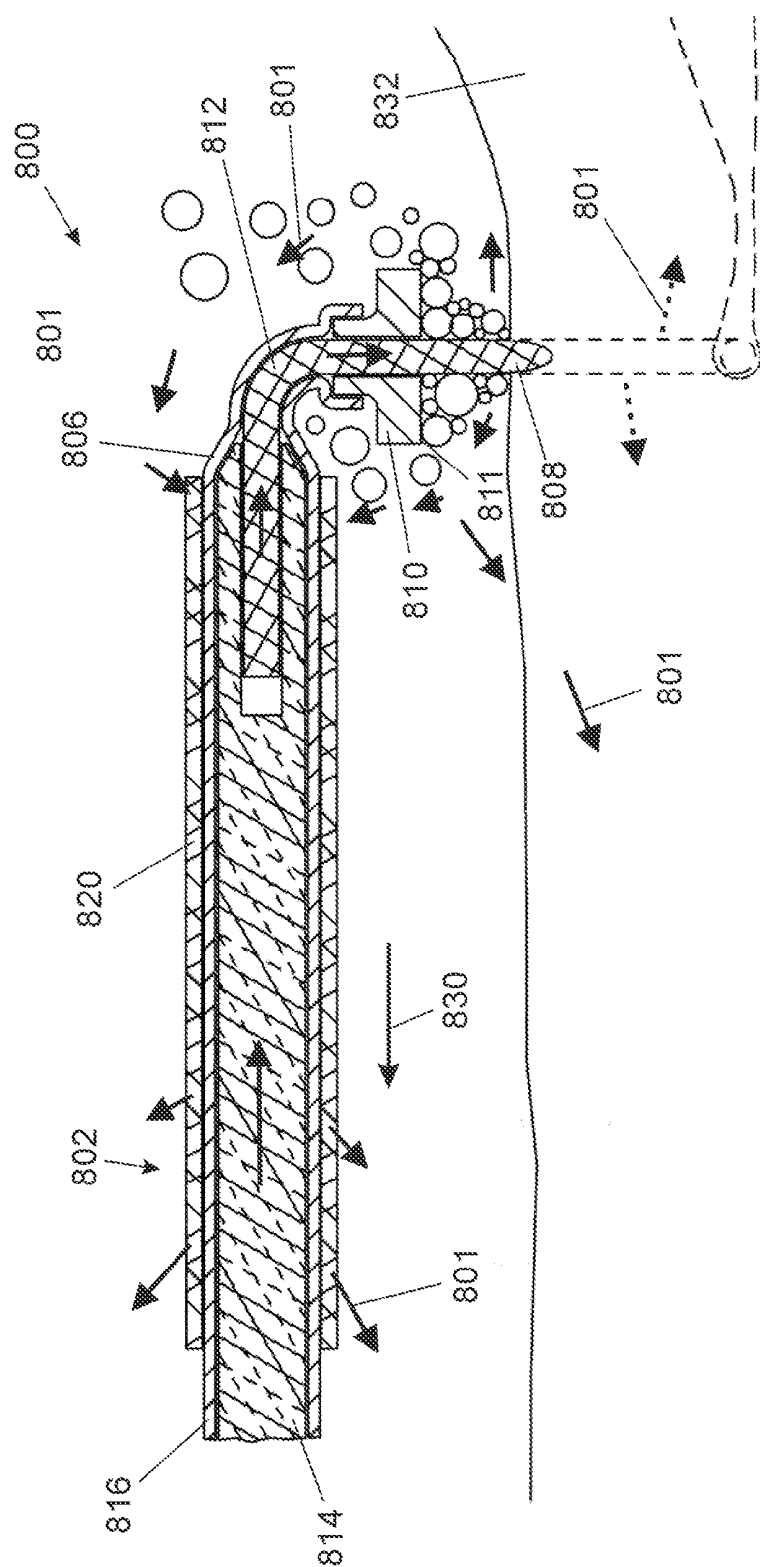

32
19
L

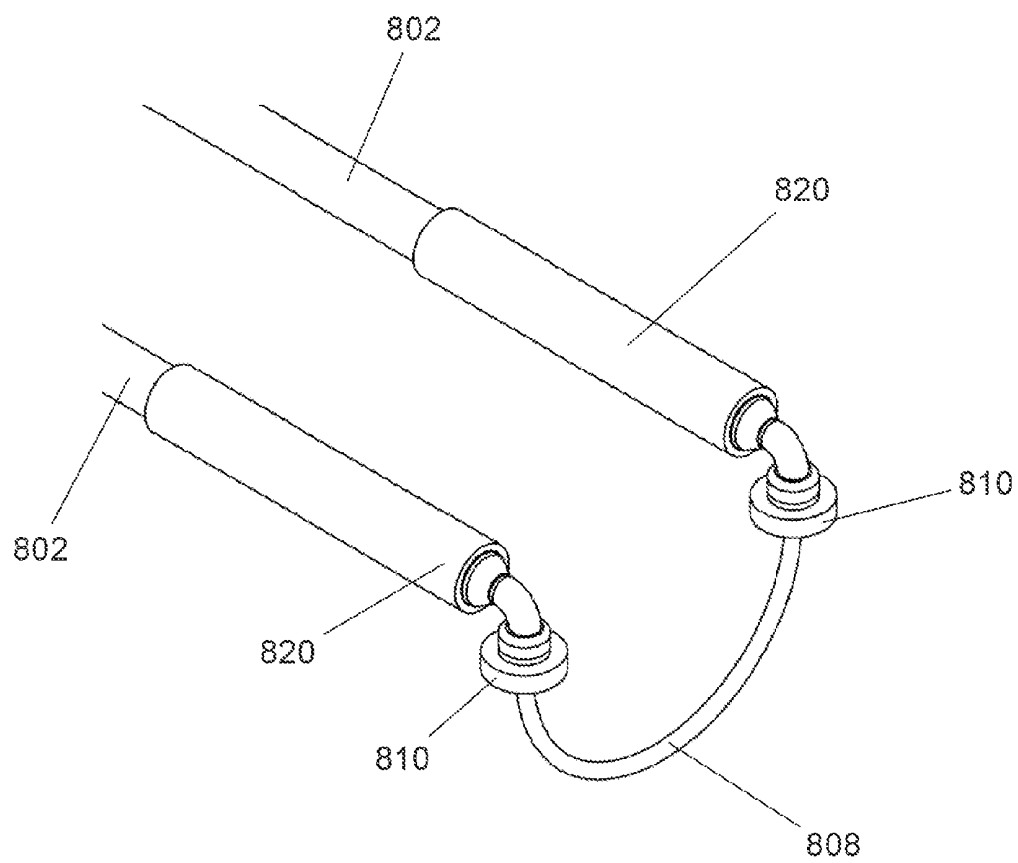


FIG. 33

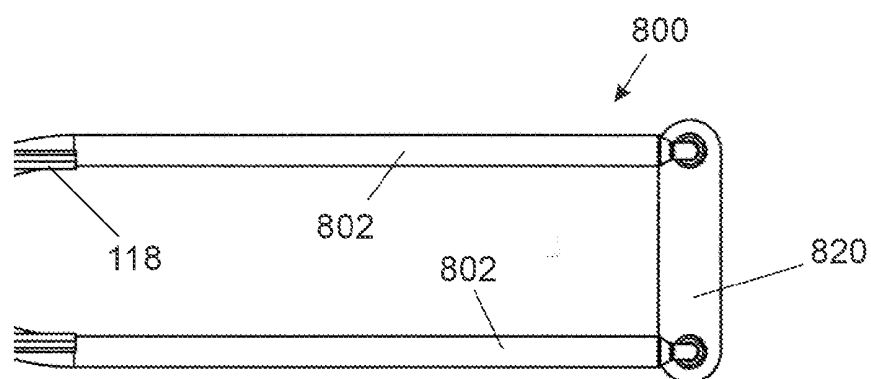


Fig. 34

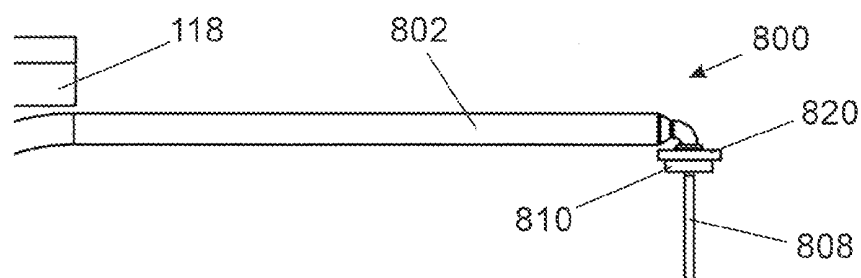


Fig. 35

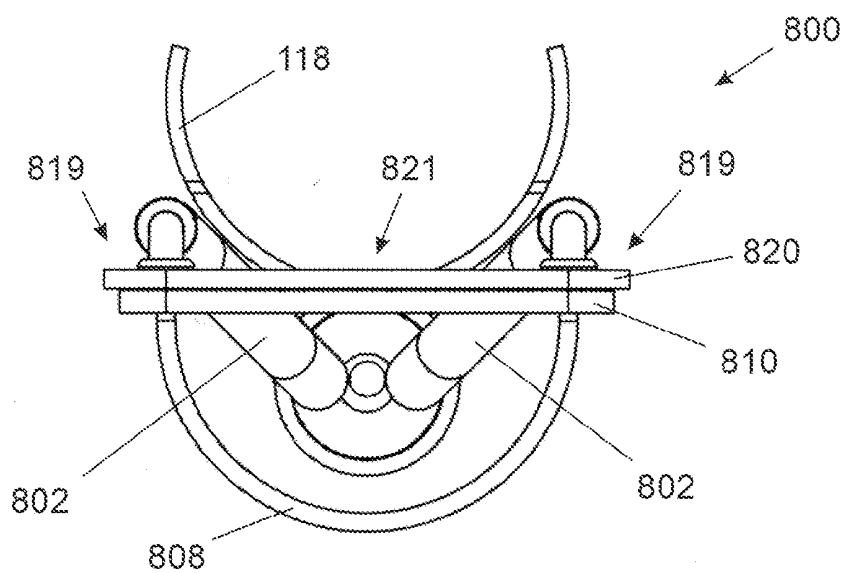


Fig. 36

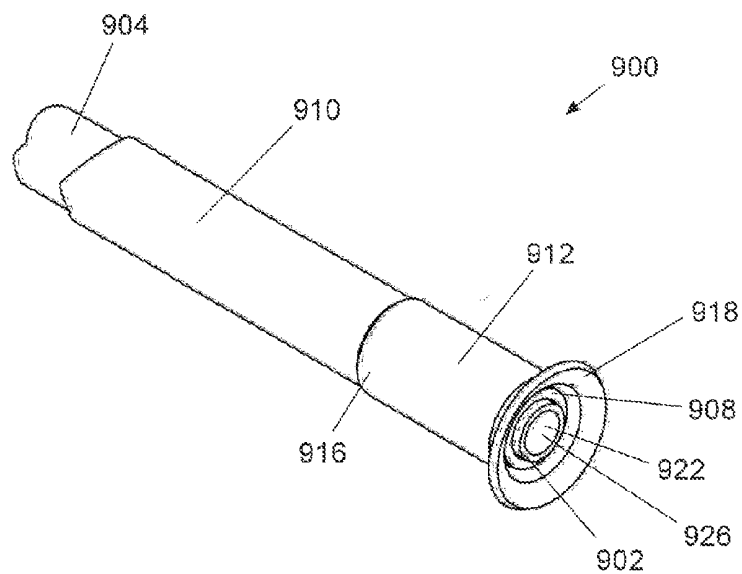


Fig. 37

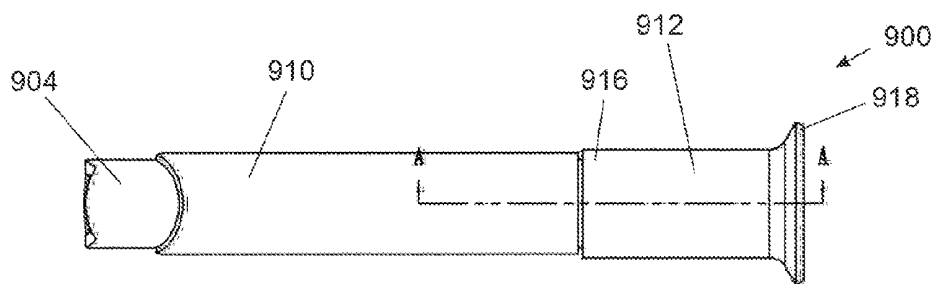


Fig. 38

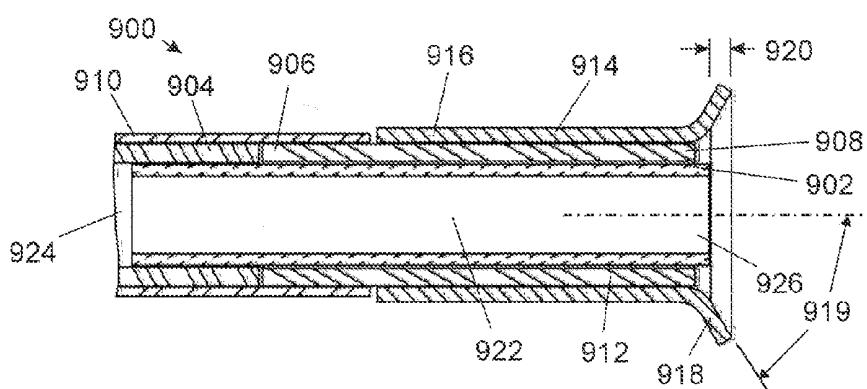


Fig. 39

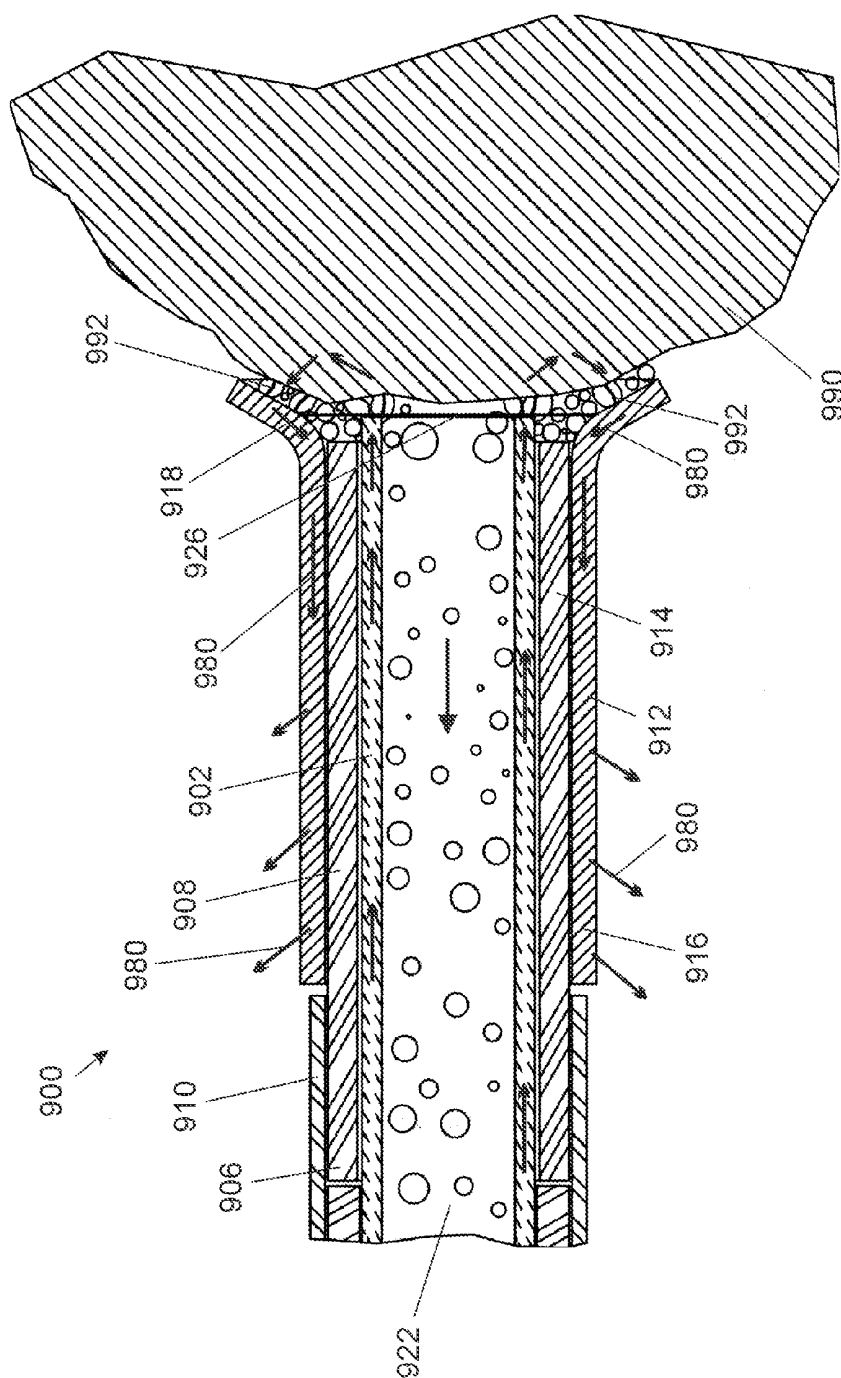


Fig. 40

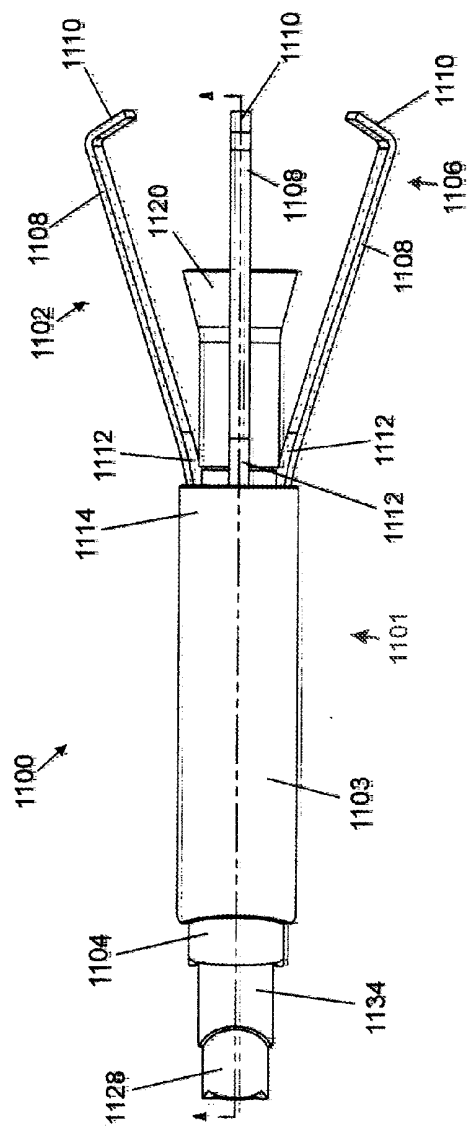


Fig. 41

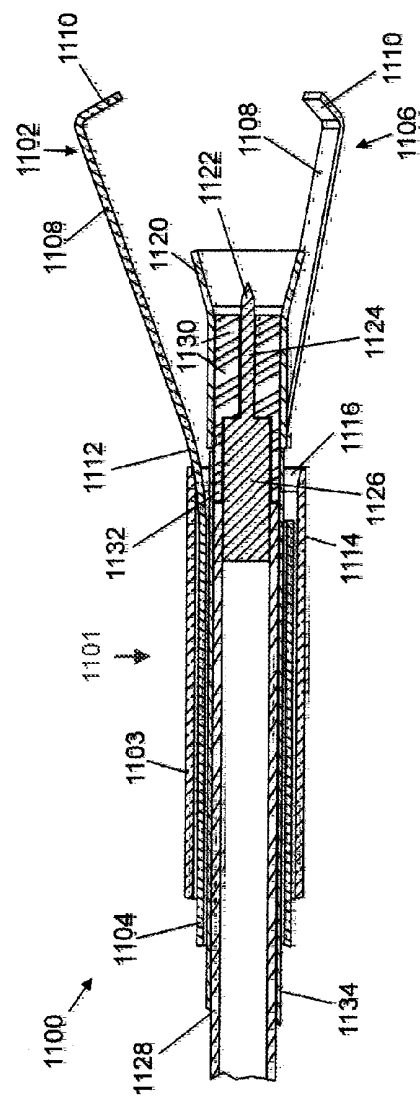


Fig. 42

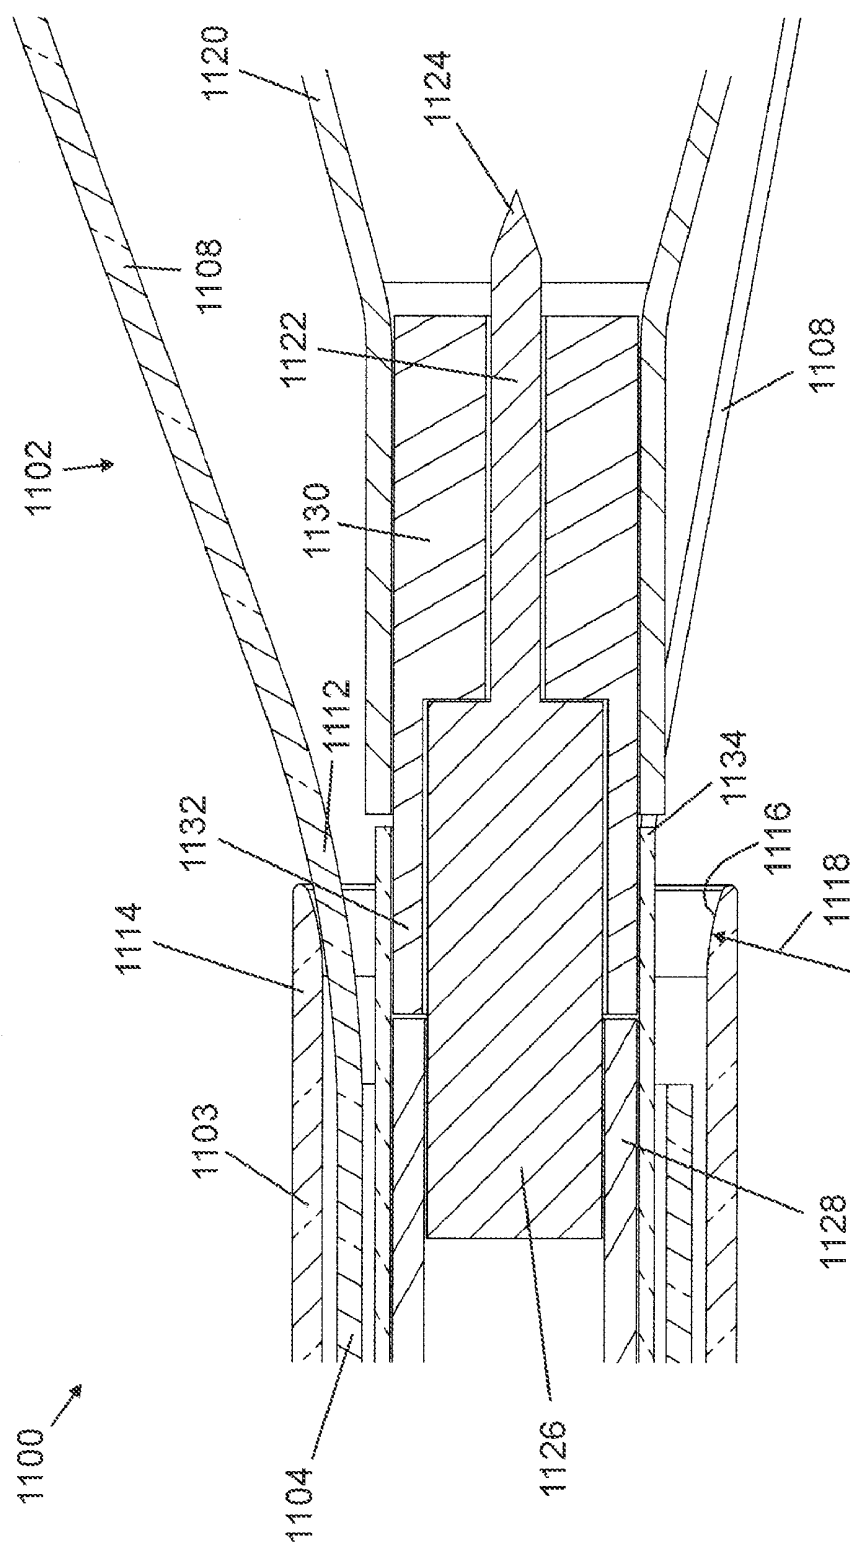


Fig. 43

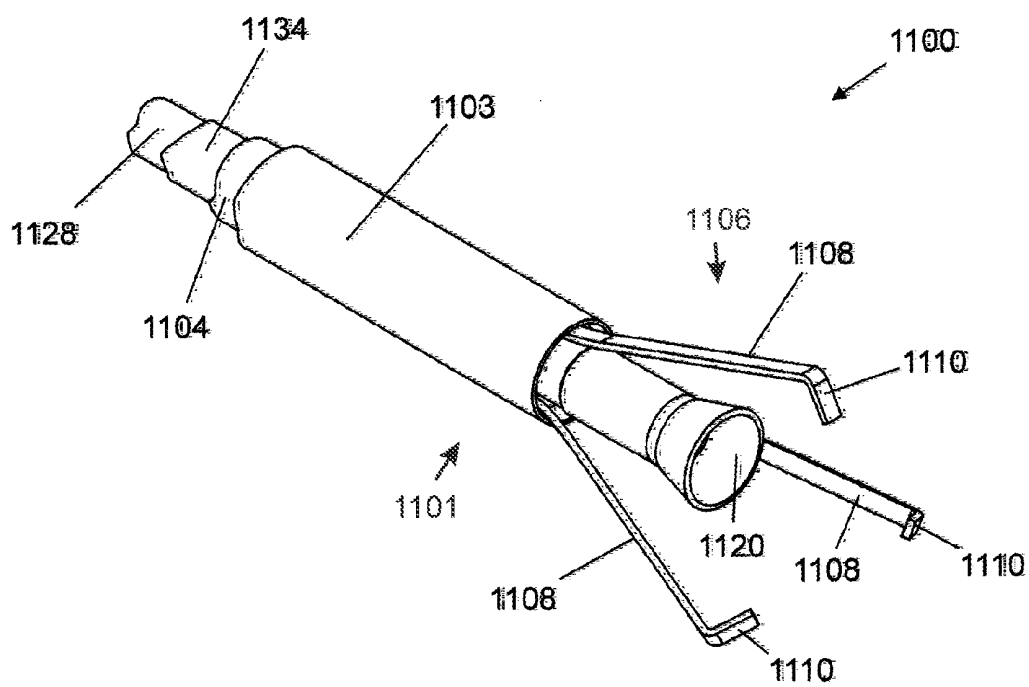


Fig. 44

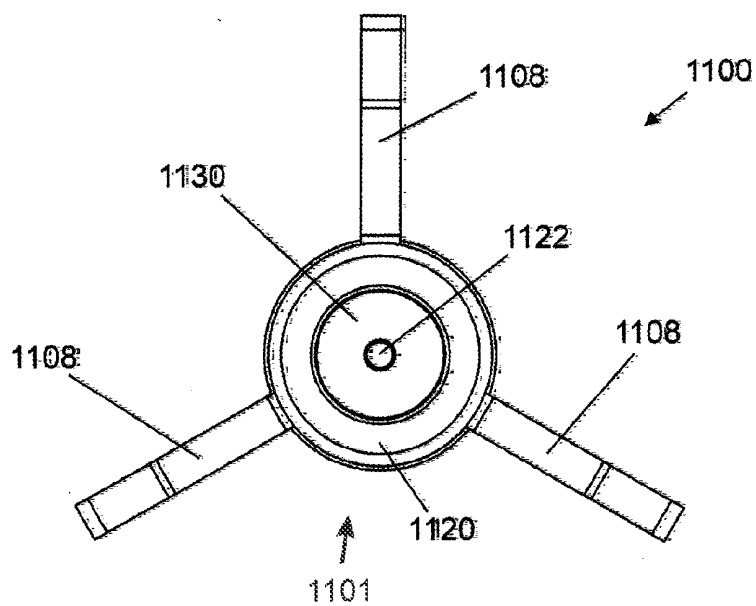


Fig. 45

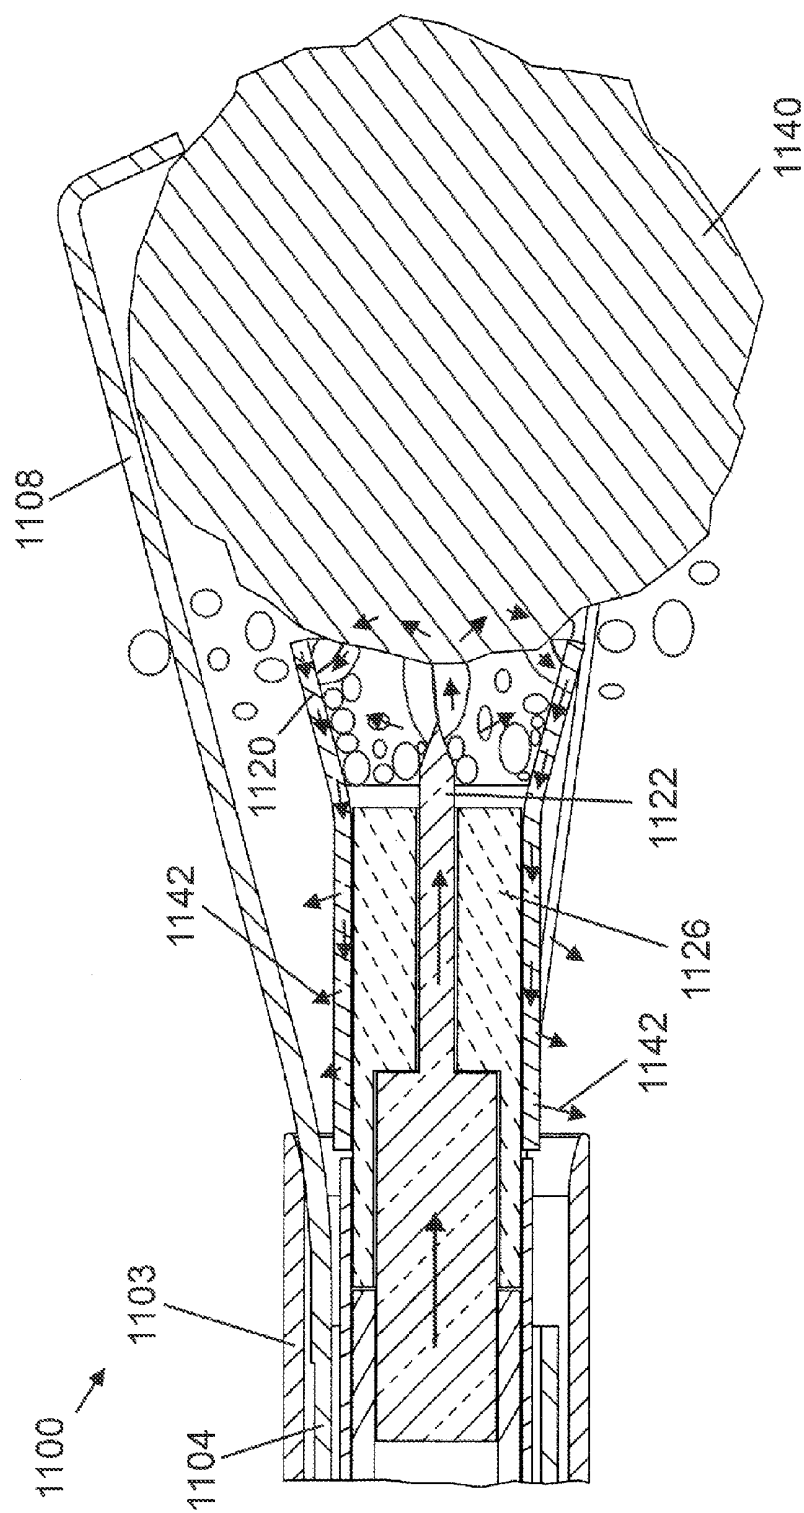


Fig. 46

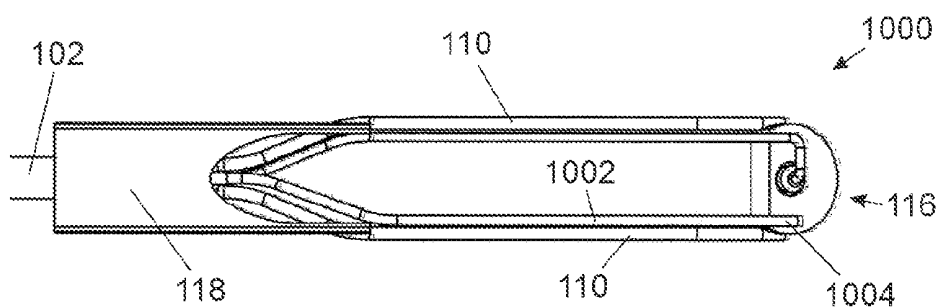


Fig. 47

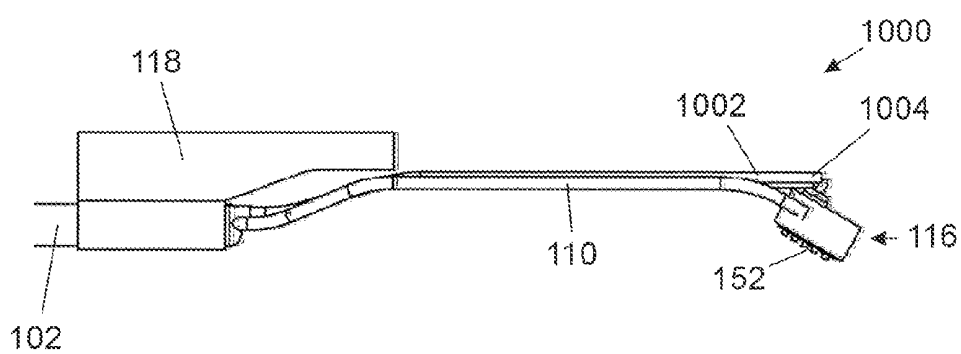


Fig. 48

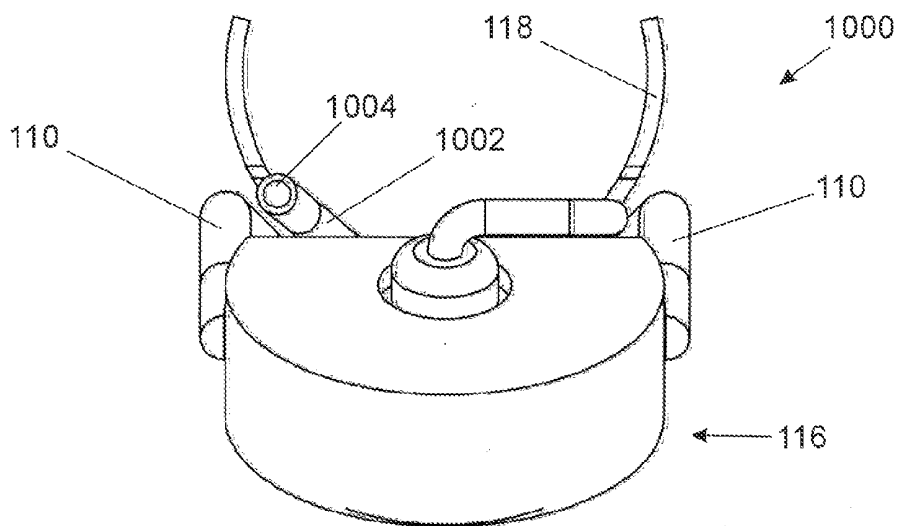


Fig. 49

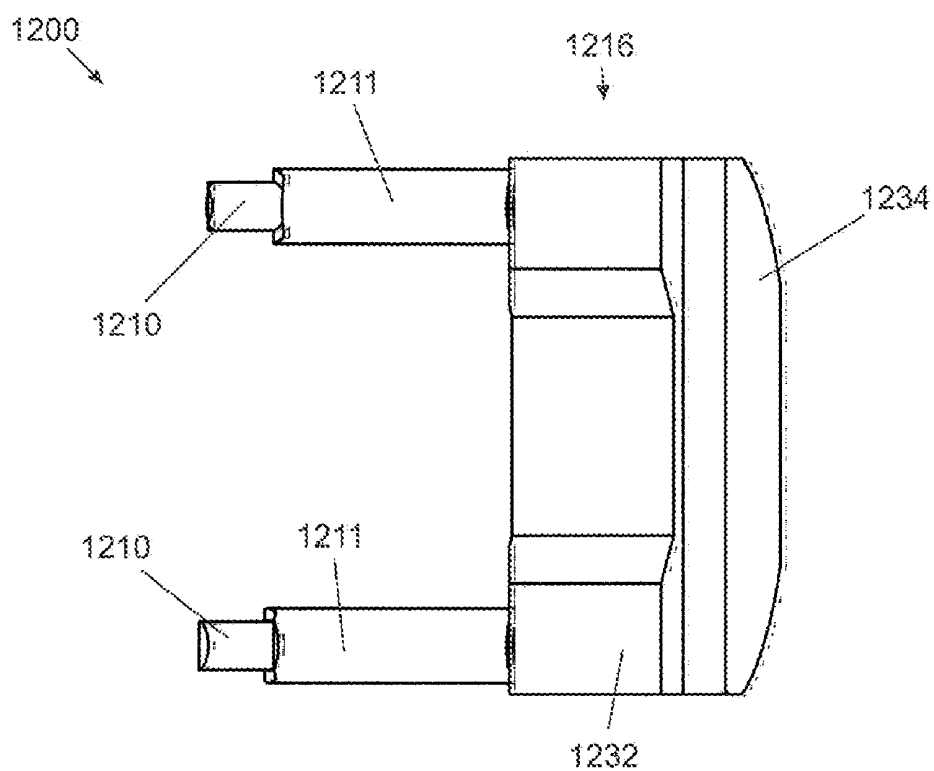


Fig. 50a

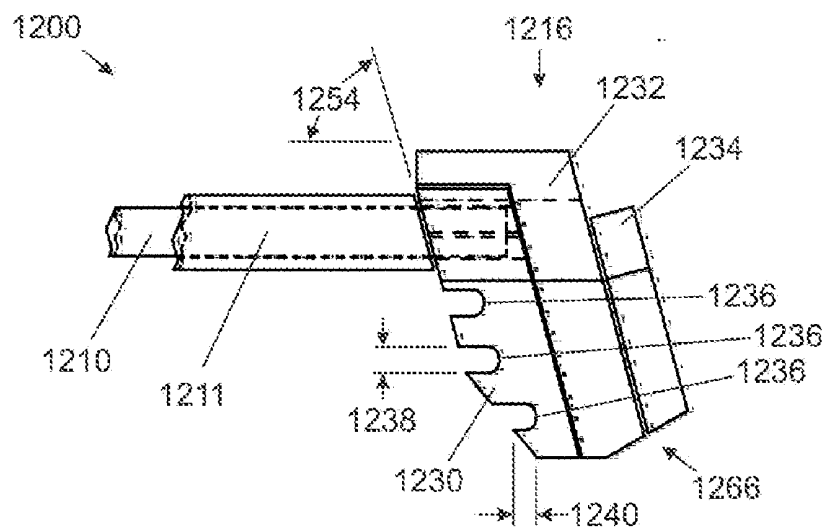


Fig. 51a

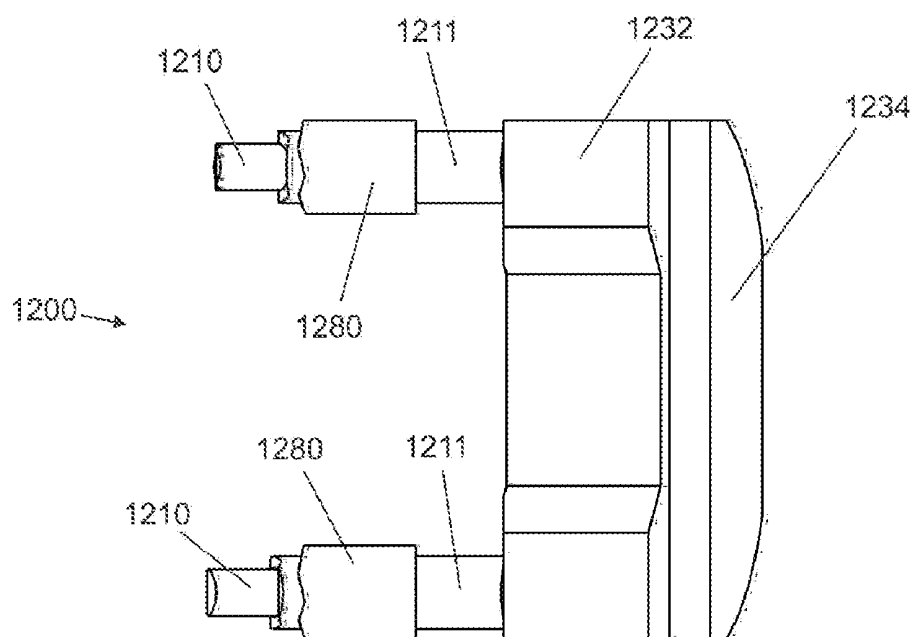


Fig. 50b

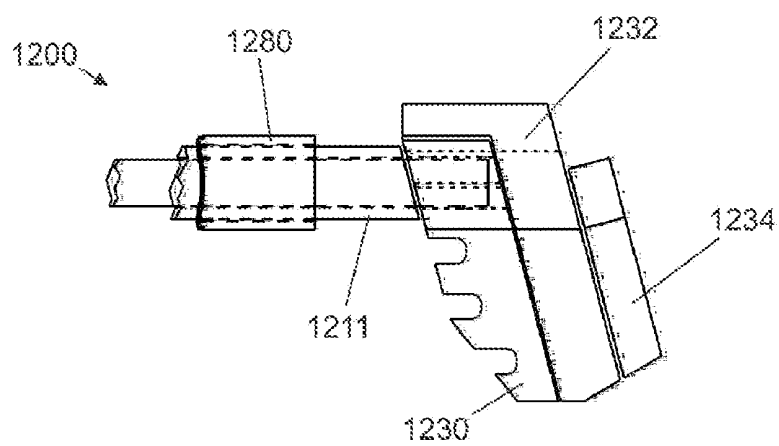


Fig. 51b

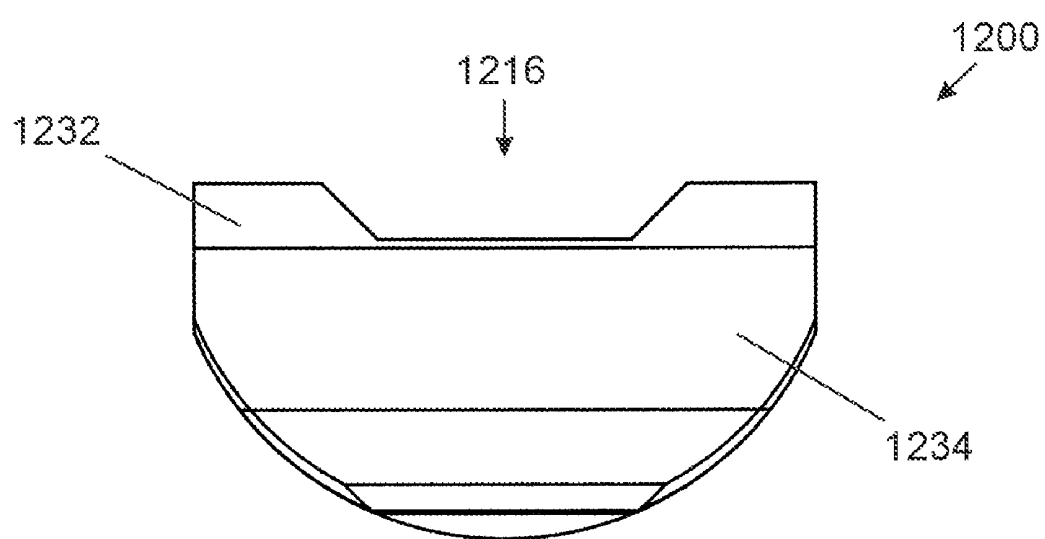


Fig. 52

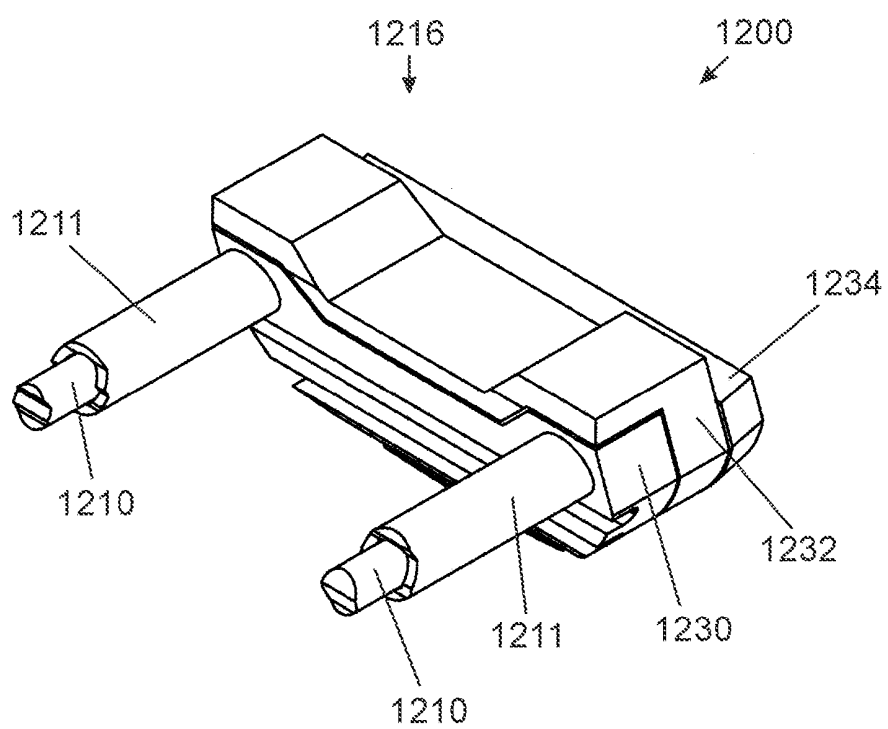


Fig. 53

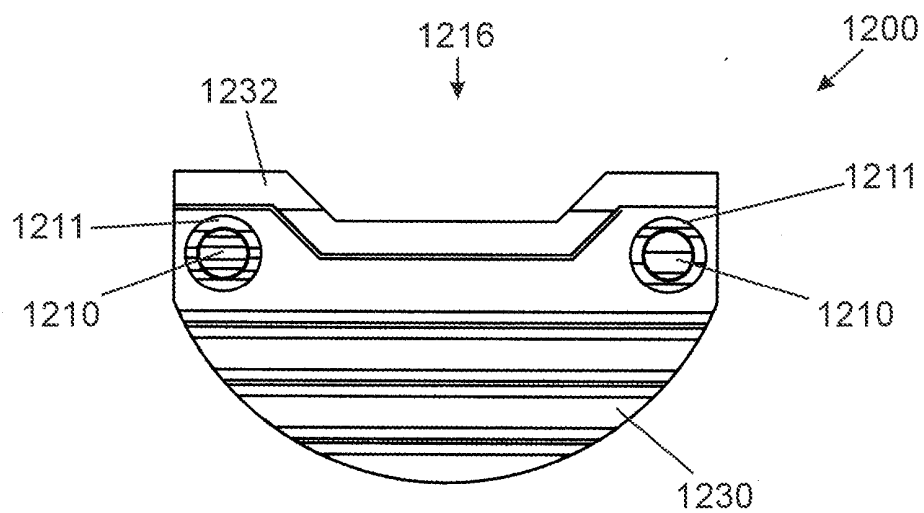


Fig. 54

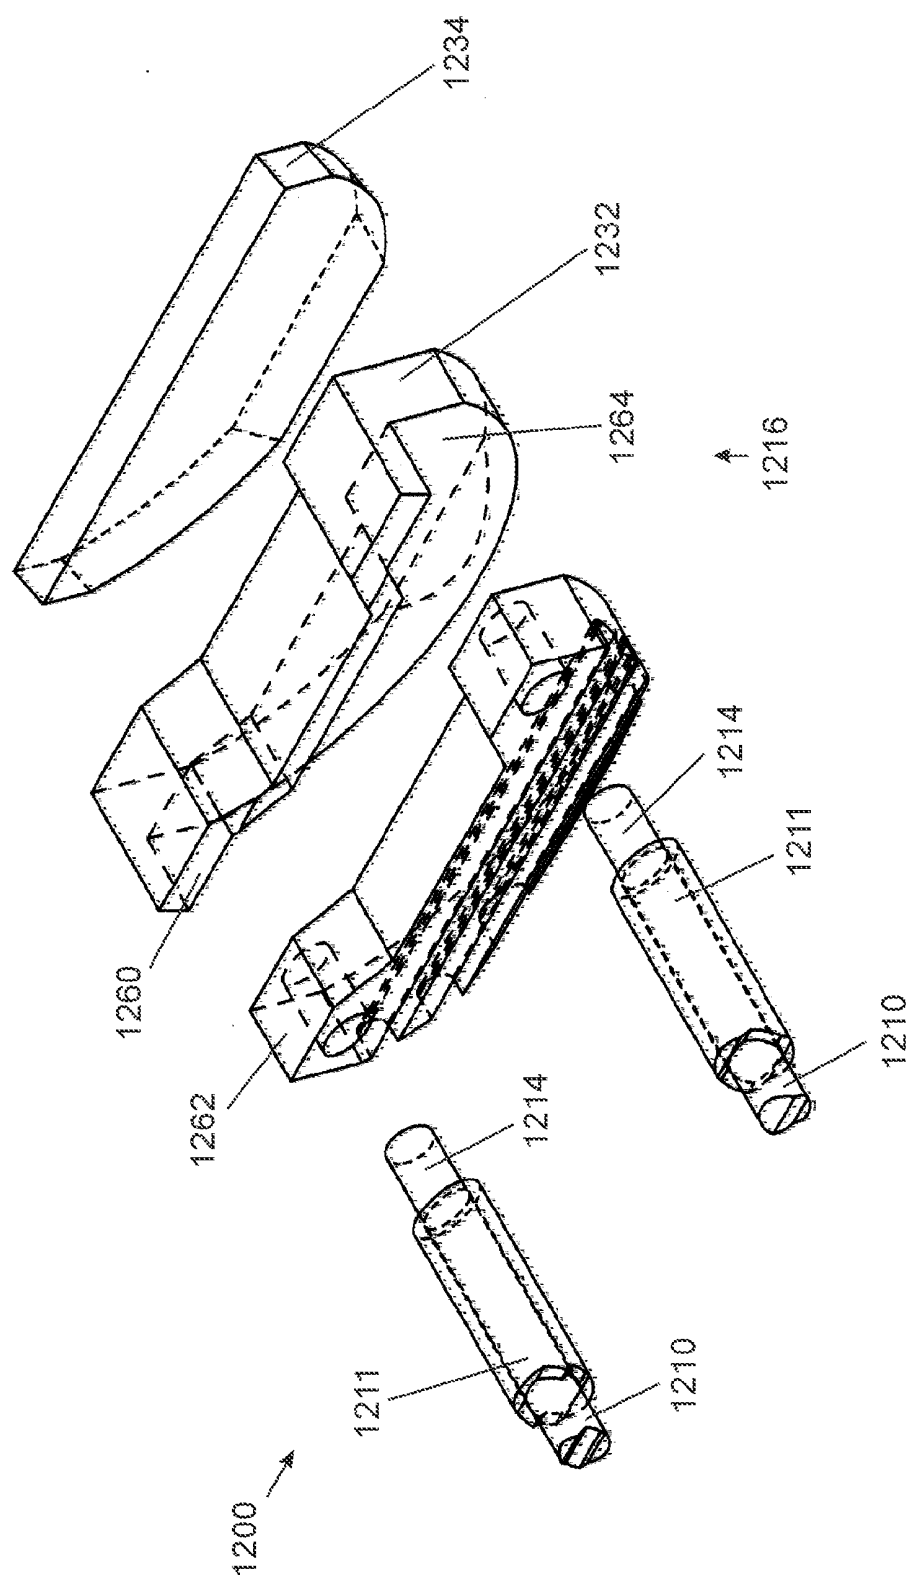


Fig. 55

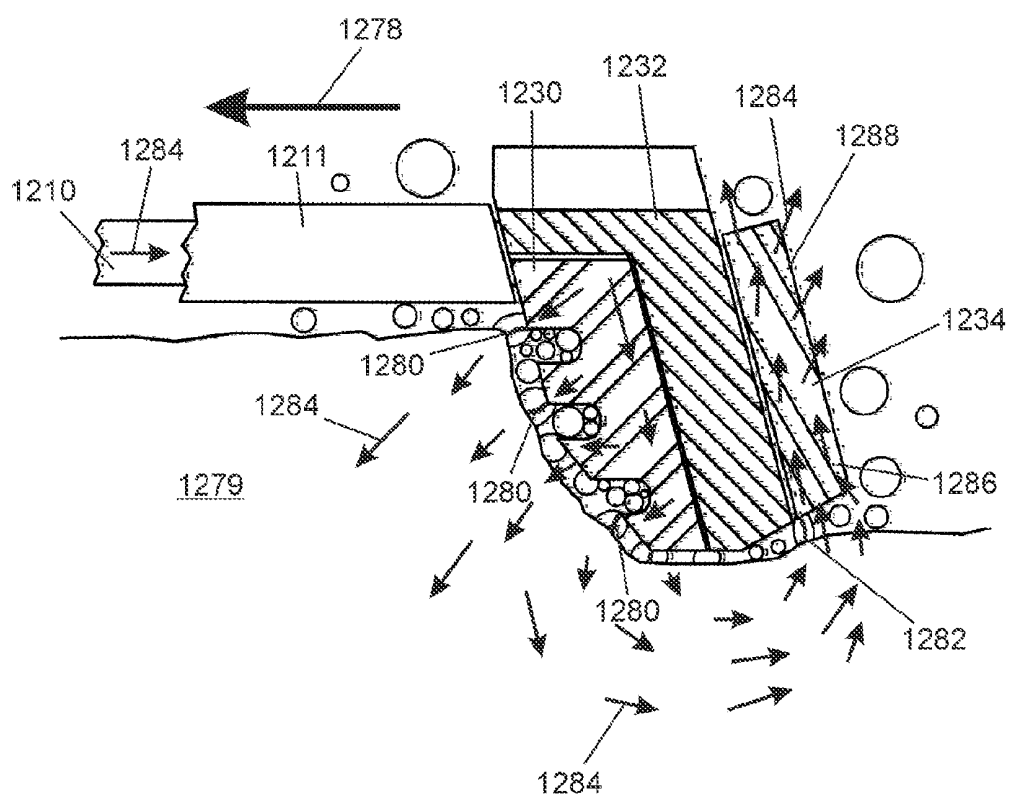


Fig. 56

**ELECTROSURGICAL DEVICE HAVING
FLOATING-POTENTIAL ELECTRODE FOR
OBSTRUCTION REMOVAL**

PRIORITY

[0001] This application is a divisional of U.S. patent application Ser. No. 13/451,138 filed Apr. 19, 2012, which, in turn, is a divisional of U.S. patent application Ser. No. 11/859,297 filed Sep. 21, 2007, now U.S. Pat. No. 8,177,784, issued May 15, 2012, which, in turn, claims the benefit of U.S. Provisional Application No. 60/847,496 filed Sep. 27, 2006, the entire contents of which are incorporated by reference herein.

FIELD OF THE INVENTION

[0002] The present invention relates generally to the field of electrosurgery, and more particularly, to high efficiency electrosurgical devices and methods which use radio frequency (RF) energy to cut, resect, ablate, vaporize, denaturize, drill, coagulate and form lesions in soft tissues, with or without externally supplied liquids. The electrosurgical devices of the instant invention find particular utility in combination with a resectoscope, in the context of urological, gynecological, laparoscopic, arthroscopic, and ENT procedures.

BACKGROUND OF THE INVENTION

[0003] As compared to conventional tissue removal techniques, electrosurgical procedures are advantageous in that they generally reduce patient bleeding and trauma. More recently, electrosurgical devices have gained significant popularity due to their ability to accomplish outcomes with reduced patient pain and accelerated return of the patient to normal activities. Such instruments are electrically energized, typically using an RF generator operating at a frequency between 100 kHz to over 4 MHz.

[0004] Many types of electrosurgical devices are currently in use. They can be divided to two general categories—monopolar devices and bipolar devices. When monopolar electrosurgical devices are used, the RF current generally flows from an exposed active electrode, through the patient's body, to a passive, return current electrode that is externally attached to a suitable location on the patient body. In this manner, the patient's body becomes part of the return current circuit. In the context of bipolar electrosurgical devices, both the active and the return current electrodes are exposed, and are typically positioned in close proximity to each other, preferably mounted on the same instrument. In bipolar procedures, the RF current flows from the active electrode to the return electrode through the nearby tissue and conductive fluids.

[0005] High frequency electrosurgical instruments, both monopolar and bipolar, have been used in the context of many surgical procedures in such fields as urology, gynecology, laparoscopy, general surgery, arthroscopy, ear nose and throat and more. In many fields of electrosurgery, monopolar and bipolar instruments operate according to the same principles. For example, the electrosurgical interventional instrument, whether monopolar or bipolar, may be introduced through a cannula, a resectoscope, or alternatively directly to perform the needed surgical procedure in the target area of the patient's body. In some cases, an externally supplied liquid (often referred to as an "irrigant"), either electrically conductive or non-conductive, is applied. In other electrosurgical procedures, the instruments rely only on locally available

bodily fluids, without requiring an external source of fluid. Procedures performed in this manner are often referred to as performed in "dry-field". When necessary, the electrosurgical instruments may be equipped with irrigation, aspiration or both.

[0006] Even though the benefits are well recognized, current electrosurgical instruments and procedures suffer from very significant deficiencies. For example, monopolar devices require the use of an additional external component, namely one or more grounding plates, remotely attached to a suitable location on the skin of the patient. Thus, in that monopolar devices require current to flow from the active electrode through the patient's body, they invariably allow for the possibility that some of the current will flow through undefined paths in the patient's body, particularly when the instrument is not properly designed and positioned.

[0007] Bipolar electrosurgical devices have their own inherent drawbacks, often resulting from the close orientation of the return and active electrodes. The return electrode necessarily has a small area and, as a result, can cause undesired tissue heating, coagulating or evaporation at its contact point with the patient's tissue due to the relatively high current densities present thereon. In addition, with the bipolar configuration, the close proximity of the active and return electrodes creates the danger that the current will short across the electrodes. For this reason, bipolar devices normally operate at relatively low voltage (typically 100 to 500 V) to decrease the chances that a spark will bridge the gap between the active and return electrodes.

[0008] Electrosurgical procedures which cut or vaporize tissue rely on generation of sparks in the vicinity of the active electrodes to vaporize the tissue. Sparking is often referred to as "arcing" within gaseous bubbles in liquid, or alternatively as plasmas. Operation at relatively low voltage, as is necessary with bipolar instruments, leads to less efficient sparking, reduced efficiency of the instrument, undesirable overheating of nearby tissue, and longer procedure time. Moreover, the use of electrosurgical bipolar procedures in electrically conductive environments is inherently problematic. For example, many arthroscopic procedures require flushing of the region to be treated with saline, both to maintain an isotonic environment, to carry away process heat and debris, and to keep the field of view clear. The presence of saline, which is a highly conductive electrolyte, can also cause electrical shorting of a bipolar electrosurgical probe, thereby causing probe destruction and unintended and unnecessary heating in the treatment environment which, in turn, can result in unintended and uncontrolled tissue destruction.

[0009] In addition, current monopolar and bipolar instruments used to cut or vaporize tissue often do not have effective means for controlling bubbles, which is essential to the safety and efficiency of many procedures. As a result, the efficiency of the instruments is often low and the procedure length is increased. Electrosurgical instruments that lack an effective means for trapping of bubbles include, for example, cutting loops, rollers, needles and knives, resection instruments and ablaters. Furthermore, many current monopolar and bipolar instruments are not designed to take full advantage of either the electrical properties of the fluids present in the vicinity of the procedure site (bodily fluids, including blood, as well as irrigation fluids, either electrically conductive or non-conductive) or the electrical properties of the tissue itself.

[0010] Vaporizing electrodes (ablaters) currently available for use in conductive liquids, whether monopolar or bipolar, have an active electrode surrounded by an insulator that is significantly larger in size than the ablating surface of the electrode. For ablaters with a circular geometry, the diameter of the portion of the probe which generates ablative arcs (i.e., the “working” diameter) is generally not greater than 70 to 80 percent of the diameter of the insulator (i.e., the “physical” diameter). Accordingly, only about 50% of the physical probe area can be considered effective. This increases the size of the distal end of the electrode necessary to achieve a given ablative surface size, and necessitates the use of cannulae, often with unnecessarily large lumens, an undesirable condition.

[0011] As noted above, it is well known in the prior art to use high frequency current in electrosurgical instruments, both monopolar and bipolar, introduced via a cannula, resectoscope, endoscope or directly, to perform the desired surgical procedure in such fields as urology, gynecology, laparoscopy, general surgery, arthroscopy, ear nose and throat and more. In fact, a number of radio frequency devices, both monopolar and bipolar, and techniques, both in conductive and non-conductive fluids, are described in the art for urological and gynecological purposes. Illustrative examples include: Alschibaja et al. [(2006) *BJU Int.* 97(2):243-6]; Botto [(2001) *J. of Endourology*, 15 (3) 313-316]; and Keoghane (pinpointmedical.com/urology) as well as U.S. Pat. Nos. 3,856,015 (Iglesias), 3,901,242 (Storz), and 2,448,741 (Scott et al.), which illustrate prior art cutting electrode assemblies for urology, gynecology and endoscopy. Other examples include: Smith (U.S. Pat. No. 5,195,959) and Pao (U.S. Pat. No. 4,674,499), which describe monopolar and bipolar electrosurgical devices, respectively, that include irrigation channels. Finally, Eggers et al. (U.S. Pat. No. 6,113,597) describes bipolar instruments for resecting and/or ablating tissue within the urethra, prostate and bladder.

[0012] Endoscopic transurethral resection and/or thermal treatment of tissue is generally accomplished using a resectoscope, a device which allows the scope and other instruments to pass easily into the urethra. Resectoscopes are well known in the art. For example, in U.S. Pat. No. 4,726,370, Karasawa et al. describe a conventional resectoscope device and electrodes suited for use therewith. Various elongated probes are used to cut, vaporize, coagulate, or otherwise thermally treat tissue. Additional electrosurgical probes for use with a resectoscope are disclosed by Grossi et al. in U.S. Pat. Nos. 4,917,082, 6,033,400, and 6,197,025. Resectoscopes, along with their associated electrosurgical probes, are also used in various laparoscopic and gynecological procedures.

[0013] Endoscopic electrosurgical probes of the type used with a resectoscope may be used with conductive or nonconductive irrigants. When conductive irrigants are used, current flows and/or arcing from any uninsulated portion of the active electrode which contacts the conductive fluid. Due to this reality, probes for use in conductive fluids must be insulated except for portions which will give the desired clinical effect during use. In a nonconductive fluid environment, conduction occurs only from portions of the active electrode which are in sufficiently close proximity to tissue to cause current flows and/or arcing between the electrode and the tissue, or from portions of the electrode which are in contact with tissue. During a surgical procedure, however, even non-conductive irrigants can achieve some level of conductivity, for example as a result of bodily fluids seeping from the patient's tissue

into the irrigant. This contamination may increase the local conductivity to a degree sufficient to cause significant current flow from uninsulated portions of a probe designed for use in a non-conductive irrigant. Accordingly, it may be presumed that all fluids have some level of conductivity during laparoscopic electrosurgery, and that all probes which are used partially or completely submerged in a liquid will benefit from a construction that maximizes electrode efficiency by maximizing the portion of the RF energy which provides clinical benefit.

[0014] Probes may be used for vaporization or for thermal modification, such as lesion formation. Vaporization occurs when the current density at the active electrode is sufficient to cause localized boiling of the fluid at the active electrode, and arcing within the bubbles formed. When the current density is insufficient to cause boiling, the tissue in proximity to the active electrode is exposed to high-temperature liquid and high current density. The temperature of the liquid and tissue is affected by the current density at the active electrode, and the flow of fluid in proximity to the electrode. The current density is determined by the probe design and by the power applied to the probe. Any given probe, therefore, can function as either a vaporizing probe or a thermal treatment probe, depending on the choice of the power applied to the probe. Lower powers will cause a probe to operate in a thermal treatment mode rather than in the vaporizing mode possible if higher power is applied.

[0015] The bubbles which form at the active electrode when a probe is used in vaporizing mode, form first in regions of the highest current density and lowest convection of the liquid. When they reach a critical size, these bubbles support arcing within and allow for vaporization of tissue. Bubbles also form in areas of lower current density as the conductive liquid in these regions reaches sufficient temperature. While these bubbles generally do not support arcing, they cover portions of the exposed electrode surface, thereby insulating these portions of the surface. This insulation of non-productive regions of the electrode decreases non-beneficial current flow into the liquid thereby allowing the electrode to achieve its clinically beneficial results at lower power levels. It is possible to increase electrode efficiency by managing these bubbles so as to retain them in regions in which their presence insulates the electrode.

[0016] In summary, the geometry, shape and materials used for the design and construction of electrosurgical instruments greatly affect the performance. Electrodes with inefficient designs will require substantially higher power levels than those with efficient designs. While currently available electrodes are capable of achieving desired surgical effects, they are not efficient for accomplishing these tasks and may result in undesired side effects to the patient.

SUMMARY OF THE INVENTION

[0017] In view of the everpresent need in the art for more efficient electrode design, it is accordingly an object of the present invention to provide an electrosurgical device which has high efficiency.

[0018] It is also an object of the present invention to provide an electrosurgical device which may be readily used in combination with a resectoscope

[0019] It is further an object of the present invention to provide an electrosurgical device which may be used in applications in which the target tissue is not submerged in a liquid environment.

[0020] It is additionally an object of the present invention to provide an electrosurgical device capable of operating in electrically conductive and non-conductive fluid environments, as well as in dry fields (bodily fluids).

[0021] These and other objects are accomplished in the invention herein disclosed, which is directed to an advanced, high efficiency, electrosurgical device designed for use with a resectoscope, and equipped with one or more additional metallic electrodes which are not connected directly to any part of power supply circuit. This disconnected electrode may contact the surrounding conducting liquid and/or tissue. The electrical potential of this disconnected electrode is “floating” and is determined by the size and position of the electrode, the tissue type and properties, and the presence or absence of bodily fluids or externally supplied fluid. “Floating” electrodes for electrosurgery are described in co-pending U.S. patent application Ser. Nos. 10/911,309 (published as US 2005-0065510) and 11/136,514 (published as US 2005-023446), the contents of which are incorporated by reference herein in their entirety. In the context of the present invention, the “floating” electrode is preferably mounted in such a way that one portion of the electrode is in close proximity to the tip of the active electrode, in the region of high potential. Another portion of the floating electrode is preferably placed farther away, in a region of otherwise low potential. This region of low potential may be in contact with the fluid environment, in contact with tissue, or both.

[0022] In the context of the present invention, the floating electrode generates and concentrates high power density in the vicinity of the active region, and results in more efficient liquid heating, steam bubble formation and bubble trapping in this region. This increases the probe efficiency, which, in turn, allows the surgeon to substantially decrease the applied RF power and thereby reduce the likelihood of patient burns and unintended local tissue injury. The probe may be operated so that the portion of the floating electrode in close proximity to the active electrode has sufficient current density to produce vaporization of the liquid and arcing so as to vaporize tissue. Alternatively, the probe may be operated so that the floating electrode contacts tissue, wherein those portions of the floating electrode in contact with the tissue have sufficient current density to thermally coagulate blood vessels and tissue. This is particularly useful for achieving hemostasis in vascular tissue, such as, for instance, that present when performing tonsillectomies.

[0023] The innovative electrosurgical devices with floating electrodes of the present invention may be very effective in other medical procedures, other than those involving tissue evaporation (ablation), including, for instance, for thermal tissue treatment, lesion formation, tissue sculpting, tissue “drilling”, and coagulation with or without externally supplied liquids.

[0024] Accordingly, in view of these noted needs and objectives, the present invention provides in one embodiment an electrosurgical instrument comprising:

- [0025]** (a) an elongate shaft having a proximal end configured for connection to an electrosurgical power source and a distal end having an electrode assembly mounted thereto;
- [0026]** (b) a conductive member coupled to the elongate shaft and extending between the proximal and distal ends thereof; and
- [0027]** (c) an electrode assembly having an active surface that forms an acute angle with the longitudinal axis

of the shaft and comprises conductive active and floating electrodes positioned in close proximity to each other and separated by a non-conductive dielectric insulator;

[0028] wherein the active surface includes a continuous or discontinuous array of raised and recessed portions that creates regions of high current density for high efficiency vaporization of tissue.

[0029] In another preferred embodiment, the present invention provides an electrosurgical instrument as described above, with the exception that the electrode assembly has a layered construction (referred to as a sandwich construction) comprised of (i) an active electrode having upper and lower surfaces; (ii) an insulator having upper and lower surfaces, wherein the upper surface of the insulator is adhered to the lower surface of the active electrode; and (iii) a floating electrode having upper and lower surfaces, wherein the upper surface of the floating electrode adhered to the lower surface of the insulator.

[0030] In a further preferred embodiment, the present invention provides an electrosurgical instrument as described above, with the exception that the electrode assembly comprises an active electrode, a floating electrode, and an insulator separating the active and floating electrodes, wherein the insulator is concentrically disposed about the active electrode, and the floating electrode is concentrically disposed about the insulator;

[0031] In the context of the present invention, the electrosurgical device herein disclosed may take the form of a probe for use with a resectoscope, wherein the probe has an elongated proximal portion and an active distal portion, the distal portion having at its distal end at least one active electrode and at least one floating electrode. The active electrode is preferably connected via cabling disposed within the elongated proximal portion to an externally disposed electrosurgical generator. At least a portion of the distal-most portion of at least one floating electrode should be positioned in close proximity to at least one active electrode. In a preferred embodiment, the active electrode has an ablating surface (often referred to herein as the “active surface” or “working surface”) composed of an array of raised and recessed regions particularly configured to maximize bubble retention and concentrate power density. The array may take the form of, for example, a plurality of walls and grooves, a plurality of elevated pins, a plurality of bumps and pockets, or a combination thereof. So long as the array performs the desired function (e.g., bubble retention, power density concentration), the specific design, geometry, arrangement and configuration of the array or its components is not particularly limited. For example, the array be continuous or discontinuous, evenly or unevenly spaced, composed of raises and recesses that are linear or non-linear (e.g., curvilinear, wavy, zigzagged, angled, etc.), parallel or circumferential positioned, or the like. In one particularly preferred embodiment, the array is composed of a plurality of grooves etched into the ablating surface of the active electrode, such grooves being of a depth and width for maximal retention of bubbles within the grooves.

[0032] The floating electrode preferably surrounds the active electrode and is separated therefrom by a dielectric member. The floating electrode intensifies the electric field in proximity to the active electrode and aids bubble retention when the probe is used to vaporize tissue. In other embodiments, the probe has irrigation supplied to the probe tip. In still other embodiments, the active electrode has a plurality of

protuberances formed on its ablating surface. These electrodes may be used for vaporizing tissue by applying sufficient voltage for bubble formation and arcing, or may be used for thermal treatment of tissue by applying lower voltages.

[0033] Other embodiments include small-diameter, elongated active electrodes having distal ends forming spherical radii, cylindrical radii, conical points or other shapes.

[0034] In another embodiment, the device may be configured exclusively for thermal treatment by providing an active electrode with a hemispherical shape.

[0035] In still other embodiments, a shaped wire electrode may be used to resect rather than vaporize tissue from a body. In this manner, the electrode functions as a cutting instrument. An illustrative embodiment of such an electrosurgical instrument may comprise:

[0036] (a) an elongate shaft having a proximal end configured for connection to an electrosurgical power source and a distal end having an electrode assembly mounted thereto;

[0037] (b) a conductive member coupled to the elongate shaft and extending between the proximal and distal ends thereof;

[0038] (c) first and second laterally opposed, distally extending, insulated conductive members mounted to the distal end of the shaft;

[0039] (d) a pair of floating electrodes, one concentrically disposed about the distal end of the first conductive member and the other concentrically disposed about the distal end of the second of conductive member;

[0040] (e) a bubble trap mounted to the distal ends of the first and second conductive members; and

[0041] (f) an active loop electrode mounted to the bubble trap, extending between the first and second conductive members;

[0042] wherein the bubble trap is formed from a non-conductive dielectric material while the active loop and floating electrodes are formed from an electrically conductive material;

[0043] further wherein the at least one active electrode is electrically connected to the conductive member while the at least one floating electrode is not connected to either the conductive member or the electrosurgical power source.

[0044] In another embodiment, the device may be configured for the treatment of kidney stones.

[0045] The present invention also provides electrosurgical methods which utilize radio frequency (RF) energy to cut, resect, ablate, vaporize, denaturize, drill, coagulate and form lesions in soft tissues, with or without externally supplied liquids, for example, in the context of urological, gynecological, laparoscopic, arthroscopic, and ENT procedures. In an illustrative embodiment, the present invention provides a method of treating benign prostatic hyperplasia (BPH) in a subject in need thereof, comprising the steps of:

[0046] (a) inserting a resectoscope outer sheath into the urethra of a subject;

[0047] (b) advancing the resectoscope outer sheath until the distal end is adjacent a target site of the prostate of the subject;

[0048] (c) advancing a resectoscope working element with telescope and an electrosurgical instrument of the present invention through the resectoscope outer sheath to the target site;

[0049] (d) introducing an irrigant to the target site so as to submerge the active and floating electrodes of the electrosurgical instrument; and

[0050] (e) applying current to the active electrode of the electrosurgical instrument and moving the electrosurgical instrument in a proximal direction relative to the prostate tissue;

[0051] wherein step (e) results in vaporization, thermal modification and hemostatic dessication of adjacent prostate tissue.

[0052] These and other objects and features of the invention will become more fully apparent when the following detailed description is read in conjunction with the accompanying figures and examples. However, it is to be understood that both the foregoing summary of the invention and the following detailed description are of a preferred embodiment, and not restrictive of the invention or other alternate embodiments of the invention.

BRIEF DESCRIPTION OF THE FIGURES

[0053] FIG. 1 is a perspective view of an electrosurgical probe constructed in accordance with the principles of this invention.

[0054] FIG. 2 is an expanded plan view of the distal portion of the object of FIG. 1.

[0055] FIG. 3 is a side elevational view of the objects of FIG. 2.

[0056] FIG. 4 is a bottom side plan view of the objects of FIG. 2.

[0057] FIG. 5 is an expanded perspective view of the distal portion of the objects of FIG. 1.

[0058] FIG. 6 is an expanded distal axial view of the objects of FIG. 1.

[0059] FIG. 7 is an expanded bottom side plan view of the distal-most portion of the objects of FIG. 2.

[0060] FIG. 8 is a side elevational sectional view of the objects of FIG. 5.

[0061] FIG. 9 is a side elevational sectional view of the objects of FIG. 5 during use.

[0062] FIG. 10 is a side elevational sectional view of the distal-most portion of an alternate embodiment.

[0063] FIG. 11 is a perspective view of another alternate embodiment.

[0064] FIG. 12 is a plan view of the objects of FIG. 11.

[0065] FIG. 13 is a side elevational view of the objects of FIG. 11.

[0066] FIG. 14 is a bottom side plan view of the objects of FIG. 11.

[0067] FIG. 15 is a plan view of an alternate embodiment.

[0068] FIG. 16 is a side elevational view of the objects of FIG. 15.

[0069] FIG. 17 is a bottom side plan view of the objects of FIG. 15.

[0070] FIG. 18 is an expanded side elevational sectional view of the distal-most portion of the objects of FIG. 15.

[0071] FIG. 19 is a plan view of another alternate embodiment.

[0072] FIG. 20 is a side elevational view of the objects of FIG. 19.

[0073] FIG. 21 is an expanded side elevational sectional view of the distal-most portion of the objects of FIG. 19.

[0074] FIG. 22 is a perspective view of another alternate embodiment.

[0075] FIG. 23 is a perspective view of yet another alternate embodiment.

[0076] FIG. 24 is an expanded plan view of the distalmost portion of the objects of FIG. 23.

[0077] FIG. 25 is a side elevational view of the objects of FIG. 24.

[0078] FIG. 26 is a bottom side plan view of the objects of FIG. 24.

[0079] FIG. 27 is a plan view of the distal portion of an alternate embodiment.

[0080] FIG. 28 is a side elevational view of the objects of FIG. 27.

[0081] FIG. 29 is an expanded distal end view of the objects of FIG. 27.

[0082] FIG. 30 is a perspective view of the objects of FIG. 27.

[0083] FIG. 31 is a side elevational sectional view of the objects of FIG. 27 at location A-A of FIG. 27.

[0084] FIG. 32 is a side elevational sectional view of the objects of FIG. 27 in use.

[0085] FIG. 33 is a perspective view of the distal portion of an alternate embodiment.

[0086] FIG. 34 is a plan view of the distal portion of an alternate embodiment.

[0087] FIG. 35 is a side elevational view of the objects of FIG. 34.

[0088] FIG. 36 is an expanded distal end view of the objects of FIG. 34.

[0089] FIG. 37 is a perspective view of the distal portion of an alternate embodiment for ablating kidney stones.

[0090] FIG. 38 is a plan view of the objects of FIG. 37.

[0091] FIG. 39 is an expanded side elevational sectional view of the objects of FIG. 37 at location A-A of FIG. 38.

[0092] FIG. 40 is an expanded side elevational sectional view of the objects of FIG. 37 during use.

[0093] FIG. 41 is a plan view of the distal portion of an alternate embodiment for removal of kidney stones.

[0094] FIG. 42 is a side elevational sectional view of the objects of FIG. 41 at location A-A of location 41.

[0095] FIG. 43 is an expanded side sectional elevational view of the mid-portion of the objects of FIG. 41 as depicted in FIG. 42.

[0096] FIG. 44 is a perspective view of the objects of FIG. 41.

[0097] FIG. 45 is an expanded distal end view of the objects of FIG. 41.

[0098] FIG. 46 is a side elevational sectional view of the objects of FIG. 41 during use.

[0099] FIG. 47 is a plan view of an alternate embodiment having aspiration.

[0100] FIG. 48 is a side elevational view of the objects of FIG. 47.

[0101] FIG. 49 is an expanded axial end view of the objects of FIG. 47.

[0102] FIG. 50a is a plan view of the distal end electrode assembly of an alternate embodiment with simplified construction. FIG. 50b is alternate view of embodiment depicted in FIG. 50a, with optional return electrodes (1280) included.

[0103] FIG. 51a is a side elevational view of the objects of FIG. 50a. FIG. 51b is alternate view of embodiment depicted in FIG. 51a, with optional return electrode (1280) included.

[0104] FIG. 52 is a distal axial view of the objects of FIG. 50a.

[0105] FIG. 53 is a perspective view of the objects of FIG. 50a.

[0106] FIG. 54 is a proximal axial view of the objects of FIG. 50a.

[0107] FIG. 55 is an exploded view of the objects of FIG. 50a.

[0108] FIG. 56 is a sectional elevational side view of the probe of FIG. 50a during use.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

[0109] In the context of the present invention, the following definitions apply:

[0110] The words “a”, “an”, and “the” as used herein mean “at least one” unless otherwise specifically indicated.

[0111] In common terminology and as used herein, the term “electrode” may refer to one or more components of an electrosurgical device (such as an active electrode or a return electrode) or to the entire device, as in an “ablator electrode” or “cutting electrode”. Such electrosurgical devices are often interchangeably referred to herein as “probes” or “instruments”.

[0112] The term “proximal” refers to that end or portion which is situated closest to the user; in other words, the proximal end of the electrosurgical device of the instant invention will typically comprise the handle portion.

[0113] The term “distal” refers to that end or portion situated farthest away from the user; in other words, the distal end of the electrosurgical device of the instant invention will typically comprise the active electrode portion.

[0114] The instant invention has both human medical and veterinary applications. Accordingly, the terms “subject” and “patient” are used interchangeably herein to refer to the person or animal being treated or examined. Exemplary animals include house pets, farm animals, and zoo animals. In a preferred embodiment, the subject is a mammal.

[0115] Unless otherwise defined, all technical and scientific terms used herein have the same meaning as commonly understood by one of ordinary skill in the art to which this invention belongs. In case of conflict, the present specification, including definitions, will control.

[0116] As noted above, the present invention is directed to high efficiency monopolar or bipolar electrosurgical devices and methods which utilize radio frequency (RF) energy to cut, resect, ablate, vaporize, denaturize, drill, coagulate and form lesions in soft tissues, with or without externally supplied liquids, having particular utility in the context of urological, gynecological, laparoscopic, arthroscopic, and ENT procedures. At its most basic, the device of the present invention is comprised of electrosurgical probe having a metallic electrode coated entirely with dielectric, with the exception of an exposed portion located at the electrode tip. This exposed tip is referred to herein as the “active element” or “active electrode” of the probe. When placed into conductive liquid-tissue media and energized, the probe induces electrical current in the conducting liquid and nearby tissue. This current deposits energy into the liquid and tissue, thereby raising the local temperature and creating the desired clinical effect. The highest energy deposition occurs in areas closely proximate to the active tip where current density is largest.

[0117] Power density in close proximity to the tip depends primarily on the applied power, the shape and size of the exposed portion of the electrode, the surrounding liquid/tissue electrical conductivity as well as the presence of bubbles.

In the sparking regime, the power density also depends on the spark distribution and conductivity (i.e., the plasma conductivity). It is further affected by the size, shape, and position of the return current electrode. In most cases, positioning the return electrode in closer proximity to the active electrode increases the power density in the region near the electrode tip.

[0118] In the case of a monopolar probe, the return current is collected by a large return electrode (sometimes called dispersive electrode or return pad) placed on the patient's body, remote from the probe tip. The power concentration capability of a monopolar probe is determined by the shape of the exposed electrode: the smaller and sharper the tip is, the better its power concentration capability.

[0119] In the case of bipolar probes, the return current electrode is placed in moderate proximity to the active electrode (generally from 1 to 10 mm). In comparison with a monopolar probe having an active electrode of approximately the same shape, some additional power concentration takes place. The power concentration capability can be further controlled by the shape and position of the return electrode. Decreasing the distance between the return electrode and the active electrode increases the power concentration. A problem arises when the probe is generating sparks. (Recall that this is the goal of probe operation in ablation-tissue evaporation or cutting, for example). If the return electrode is placed sufficiently close to the tip to achieve a substantial increase of power concentration, the breakdown (arcing within bubbles) takes place between the tip and return electrode. The spark conductive channel connects the active electrode to the return current electrode and the power supply is loaded directly by the spark. Usually this leads to an extra high-energy deposition in the spark between metallic electrodes, thereby resulting in localized melting and vaporization of the electrodes themselves. In turn, this results in shorting of the power supply and destruction of both the active and return electrodes with little clinical benefit to the patient.

[0120] A good bipolar probe design must therefore avoid arcing between the active and return electrodes. Usually this is achieved by placing the return electrode a sufficiently large distance away from the active electrode to prevent direct breakdown between electrodes. Nevertheless, periodic arcing may take place such that both electrodes are eroded and eventually destroyed, especially in an aggressive mode of operation. Therefore, the additional degree of power concentration achievable by bipolar probes is severely limited.

[0121] In contrast, the electrosurgical device of the present invention has one or more additional metallic electrodes which are not connected directly to any part of the power supply circuit, and therefore are called "floating". These floating electrodes are in contact with the tissue and/or liquid in proximity to the active electrode. The electrical potential of these additional electrodes is not fixed, but rather is "floating" and is determined by size and position of the electrode and the electrical conductivity of the tissue and/or liquid surrounding the distal end of the device. This electrode is positioned in such a way that one end of the electrode is in close proximity to the active electrode. Another portion of the floating electrode is positioned in a region of low potential in the liquid and/or tissue. The addition of this floating electrode thereby substantially modifies the electrical field distribution, and energy deposition, in the vicinity of the active electrode with-

out the possibility of electrode destruction since the floating electrode is not directly connected to the electrical power supply.

[0122] The floating electrode therefore serves to concentrate the electric field in the region of the active electrode, but it does not provide a current path back to the RF generator that powers the electrosurgical device. In monopolar electrosurgical devices, there is an additional dispersive return electrode that is in contact with a remote portion of the patient's body and is coupled to the RF generator in order to complete the return path. In bipolar electrosurgical devices, there is a return electrode mounted near the active electrode near the distal end of the device, and this return electrode is coupled to the RF generator in order to complete the return path to ground. In either configuration, a floating electrode may be used to shape the electric field near the active electrode; however, the floating electrode should not be confused with the return electrode, as the floating electrode has no connection to the RF generator and is, in fact, isolated from the electrical circuit of the device.

[0123] In the absence of sparking (arcing within bubbles), the "floating" electrode increases power density in the vicinity of the probe tip. This is because the floating electrode extends from a high potential region (near the active electrode), to a region with low potential (farther from the active electrode), and "shorts" these points together. The probe's floating will be between the potentials of these points. The presence of the electrode decreases the potential near the active electrode, and thereby increases the electric field, current and power density in the region near the active electrode. A floating electrode works about the same way as any extended conductive object in an electrostatic field. The higher power density results in more efficient liquid heating and steam bubble formation, which, in turn, allows one to decrease the power applied to probe for a given effect. In the presence of the "floating" electrode, more sparks are generated in the active region, since this region is larger. Bubble trapping (the retention of bubbles in selected areas to insulate these areas for improved ablator efficiency) is greatly enhanced with proper design of the floating electrode, insulator and the active electrode.

[0124] Sparks are an active element of the electrosurgical process. A spark is generated in a steam bubble if the electrical field in the bubble (voltage difference across a bubble) is sufficient for breakdown. Usually sparks are generated in bubbles that are close to the active electrode of the probe because current density and field intensity are largest in this region.

[0125] The breakdown or spark inside a bubble is an electrically conductive channel of partly ionized pressurized gas. This medium is called highly collisional plasma. The basic property of this plasma is that the conductivity is proportional to the plasma density. Higher plasma temperatures are associated with higher ionization rates, plasma densities and conductivity.

[0126] Usually energy is deposited into highly collisional plasmas by electric current driven by voltage applied to electrodes at the ends of a plasma channel. In the case of a plasma channel formed inside of a bubble, the inner parts of the bubble surface having the largest voltage difference act as the "electrodes" to which the channel is connected. More frequently, but not always, one of these electrodes is a metallic surface of the active electrode and the other is the opposite surface of the bubble or the surface of the tissue.

[0127] Electrically, the plasma channel is characterized by its impedance. The efficiency of energy deposition strongly depends on the ratio between the plasma channel and the power supply impedance. Efficiency (the portion of applied energy deposited to the plasma) as high as 50% can be achieved for matched conditions in which the power supply impedance equals the spark (plasma channel) impedance. If the channel impedance is too large or too small, the power deposition in the plasma is decreased.

[0128] As described previously herein, the additional “floating” electrode can significantly increase the energy density in the region surrounding the active electrode. This makes it possible to substantially increase the power deposited into the spark. Since the floating electrode can be placed very close to the probe tip, the largest probability is for breakdown and plasma channel formation in the region between the two electrodes—the active electrode and the floating electrode. The plasma channel current can now be supported not by a bubble size fraction of the induced current, but by a much larger volume of current flow that is determined by the size of floating electrode. This floating electrode additionally concentrates current delivered to the spark. The optimum spark current can be controlled by adjusting the size and position of the floating electrode. Arcing, then, can occur through bubbles between the active and floating electrodes, or from either electrode through bubbles in contact with that electrode.

[0129] In summary, the present invention provides an advanced, electrosurgical probe equipped with one or more “floating electrodes” coupled with one or more active electrode uniquely designed and configured for thermal tissue treatment, including tissue ablation and vaporization, preferably in combination with a resectoscope. The floating electrode concentrates the power (i.e., increases the power density) in the active region, which leads to more efficient liquid heating, steam bubble formation, and spark generation in this region. Arcing occurs from the floating electrode as well as the active electrode, thereby resulting in a probe in which the distal tip has a “working” area equal to the “physical” area. This is in contrast to other prior art probes used in electrically conductive liquids which generally have an electrically active area that is significantly smaller than the physical area of the device.

[0130] The floating electrode favorably affects bubble formation and trapping, and therefore enhances the probe’s performance. This results in high efficiency operation, allowing the surgeon to substantially decrease the applied RF power and thereby reduce the likelihood of patient burns and injury, while at the same time maintaining high performance operation.

[0131] The method of the present invention includes the step of positioning the electrosurgical probe adjacent to target tissue at a surgical site so that at least one of the active electrodes and at least a portion of at least one of the floating electrodes are in close proximity to the target tissue. Conductive or non-conductive irrigant may be supplied to the probe distal tip in the region between the active electrode(s) and the target tissue, and between the portion of the floating electrode in close proximity to the tissue, and the target tissue itself. Other portions of the floating electrode(s) may be in contact with target tissue, adjacent tissue, or fluid environment. Vacuum may be supplied via means within the elongated distal portion to the probe distal tip so as to remove excess irrigant as well as ablation products. The probe is energized

producing high current density and arcing in portions of the active electrode and floating electrode in close proximity to the target tissue. Lower density current flow from regions of the floating electrode(s) in contact with adjacent target tissue results in desiccation of the adjacent tissue so as to achieve hemostasis. While energized, the probe may be moved across the target tissue with a brushing or sweeping motion, or intermittently energized for a brief period of time and repositioned so as to affect the target tissue. When used with a resectoscope, the probe may be extended axially, energized and retracted proximally so as to cut a groove in the tissue. The process may be repeated until the desired volume of tissue is removed. The movement of the probe relative to the tissue may be manually achieved or alternatively automated, for example, according to the principles outlined in U.S. Pat. No. 6,921,398 or U.S. Patent Publication No. 2003-0065321, the contents of which are incorporated by reference herein in their entirety.

[0132] The current invention is also useful for medical procedures in which tissue is thermally treated rather than removed by vaporization, such as, for instance, cardiology, oncology and treatment of tumors, a process sometimes referred to as lesion formation for coagulation and/or denaturing of tissue. In these applications, the device is brought into close proximity, or contact, with tissue with or without the presence of externally applied irrigant at the site for thermal treatment. The voltage applied to the active electrode is reduced to a level which produces current densities insufficient for forming sparks and the associated bubbles. Tissue is heated to a desired temperature for a predetermined time sufficient for lesion formation. The floating electrode intensifies the electric field in the region surrounding the active electrode so as to produce a larger, more controlled and more uniform lesion.

EXAMPLES

[0133] Hereinafter, the present invention is described in more detail by reference to the exemplary embodiments. However, the following examples only illustrate aspects of the invention and in no way are intended to limit the scope of the present invention. As such, embodiments similar or equivalent to those described herein can be used in the practice or testing of the present invention.

[0134] Referring to FIGS. 1 through 4, which depict an electrosurgical probe specifically configured for use with a resectoscope (not shown) and constructed in accordance with the principles of this invention, probe **100** has an elongated tubular member **102** with a proximal end **104** having an electrical connector **106** suitable for connecting via an electrical cable to an electrosurgical generator, and a distal end **108**. Members **110** have proximal ends **112** mounted to distal end **108** of elongated tubular member **102**, and distal ends **114** to which are mounted electrode assembly **116**. Optional electrode stabilizer **118** for stabilizing the distal end of probe **100** is intended to be proximally disposed to a distal region of a telescope mounted in a resectoscope working element. However, it is envisioned that stabilizer **118** is not required to practice this invention. Conductive member **120** covered by insulation **122** extends from electrical connector **106** to proximal end **124** of insulated conductive member **126**.

[0135] Referring now to FIGS. 5-8, which depict the distal-most portion of probe **100**, referred to herein as the active head, electrode assembly **116** includes active electrode **130**, insulator **132** and floating electrode **134**. Active electrode **130**

has a plurality of grooves **136** of width **138** and depth **140**, width **138** and depth **140** being selected to trap bubbles in the grooves. However, as noted previously, the present invention is not limited to the grooved design depicted but encompasses any active electrode ablating surface specifically configured to maximize bubble retention and concentrate power density. So long as the ablating surface performs the desired function (e.g., bubble retention, power density concentration), the specific design, geometry, arrangement and configuration of the array or its components is not particularly limited. Accordingly, the ablating surface may be composed of an array of raised and recessed regions, e.g., a plurality of walls and grooves, a plurality of elevated pins, a plurality of bumps and pockets, or a combination thereof. As noted previously, the array be continuous or discontinuous, evenly or unevenly spaced, composed of raises and recesses that are linear or non-linear (e.g., curvilinear, wavy, zigzagged, angled, etc.), parallel or circumferential positioned, or the like.

[0136] Active electrode **130** and floating electrode **134** are preferably formed from a suitable metallic material, examples of which include, but are not limited to, stainless steel, nickel, titanium, tungsten, and the like. Insulator **132** is preferably formed from a suitable dielectric material, example of which include, but are not limited to, alumina, zirconia, and high-temperature polymers. As shown in FIG. 8, active electrode **130** preferably protrudes beyond insulator **132** a distance **142**. In turn, insulator **132** preferably protrudes beyond floating electrode **134** a distance **144**. Insulated conductive member **126** has a conductive portion **146** coated with dielectric material **148**. Distal end **150** portion **146** is connected to active electrode **130**. Active electrode **130** has surface **152** segmented by grooves **136**. Surface **136** forms an acute angle **154** with the axis of tubular member **102**. Angle **154** is preferably between 0 and 90 degrees, more preferably between 5 and 80 degrees, more preferably between 10 and 70 degrees, more preferably between 15 and 60 degrees, even more preferably between 20 and 50 degrees.

[0137] Referring now to FIG. 9, which depicts a probe **100** in use in a conductive liquid environment, probe **100** is moved axially in direction **160** relative to the tissue which is connected to a return electrode at a remote location. Current (depicted by arrows **162**) flows from conductor **126** to active electrode **130**, and then from active electrode **130** through the conductive fluid to the tissue and the return electrode. A portion of the current flows through the floating electrode, the current entering the portion of the floating electrode in the high-potential portion of the electric field in close proximity to the active electrode, and exiting in portions of the floating electrode in low-potential regions farther removed from the active electrode. Current flowing through the conductive liquid heats the liquid, the heating at a location being proportional to the current density at that location. Where the current density is sufficient, the conductive liquid boils, forming steam bubbles. Some of the bubbles **164** are trapped in grooves **136** where their presence decreases current flow from the surfaces of the groove, thereby effectively insulating the groove. Other bubbles form at surface **152**. When these bubbles reach a sufficient size, arcing **166** occurs within some of these bubbles, the resistance to arcing being less than the resistance of the alternate path for current flow around the bubble. In some cases, the bubbles at surface **152** intersect portions of tissue that are in close proximity. When arcing occurs within these bubbles, the arc is between active electrode **130** and the tissue, and in this manner a portion of the

tissue is vaporized. Current density at the portions of the floating electrode in high-potential portion of the electric field, in close proximity to the active electrode, also may be sufficient to cause boiling of the liquid, bubble formation, arcing within bubbles, and arcing between the floating electrode and tissue so as to vaporize tissue.

[0138] The active or ablating surface **152** of active electrode **130** of probe **100** is preferably planar. However, in some circumstances, it may be advantageous to have surface **152** take other, non-planar forms. For example, in an alternate embodiment shown in FIG. 10, active surface **152** of probe **200** is curved, preferably in a cylindrical manner having a radius **160**. In other embodiments, surface **152** may have other curvilinear profiles. In still other embodiments, surface **152** may have a non-uniform cross-section and take the shape of, for example, a convex spherical segment or a concave spherical segment.

[0139] Probe **100** is intended for use at a surgical site which is submerged in liquid environment or in which the region surrounding the distal end of the probe is irrigated with a irrigant. Probe **300**, shown in FIGS. 11 through 14, is identical in construction to probe **100**, and additionally has a means for providing irrigant to a surgical site, particularly the region surrounding the distal portion of the probe. Tubular member **302** is connected via means within tubular member **102** to an external irrigant source. Flow **304** from distal end **306** of member **302** causes puddling of irrigant in the region surrounding electrode assembly **116** and tissue in contact with it.

[0140] FIGS. 15 through 18 depict an alternate embodiment, including an active electrode configured for thermal treatment or vaporization of tissue in a fluid environment. Probe **400**, the distal portion of which is depicted in FIGS. 15 through 18, is constructed a fashion analogous to that of probe **100**, with the exception of electrode assembly **116**. Active electrode **430** forms an array of cylindrical pins **431** which protrude through holes in insulator portion **432**, which with insulator portion **433** electrically isolate active electrode **430**. Insulator portion **432** protrudes from floating electrode **434** distance **444**. Axial surfaces **452** of pins **431** are coplanar and form an acute angle **454** with the axis of tubular portion **102** (FIG. 1). In this context, the acute angle may range between 0 and 90 degrees, more preferably between 5 and 80 degrees, more preferably between 10 and 70 degrees, more preferably between 15 and 60 degrees, even more preferably between 20 and 50 degrees.

[0141] It is frequently desirable to precisely vaporize or thermally treat small regions of tissue. The embodiment shown in FIGS. 19 through 21 has an active electrode that forms a hemispherical portion of radius **504**. Probe **500** is analogous in construction to probe **100**, including an elongated tubular portion **102** with a proximal end electrical connector **106** connected by means within portion **102** to the active electrode, and a scope support **118**. Active electrode **502** forms a hemisphere of radius **504**. Insulator **506** is mounted to distal end **104** of tubular portion **102**. Tubular floating electrode **508** is mounted to insulator **506**. When energized in a conductive fluid environment, floating electrode **508** intensifies the field in close proximity to active electrode **502**. Distal end **510** of floating electrode **508** is in a high potential region of the field. Proximal end **512** of floating electrode **508** is in a lower potential portion of the field such that current flows through floating electrode **508** from distal end **510** to lower potential portions. This current flow increases the field intensity thereby increasing the efficiency

of the probe. This, in turn, allows procedures to be performed with less power or more quickly.

[0142] A further embodiment, intended for cutting, vaporizing or thermally treating tissue, is depicted in FIG. 22. Probe 600 is constructed like probe 500 except that active electrode 602 forms an elongated portion 603 protruding from distal surface 607 of insulator 606. Elongated portion 603 has a distal end 605 forming a spherical portion 609. In other embodiments, portion 603 may be cylindrical throughout its entire length. In still other embodiments, distal end 605 forms a conical point. Floating electrode 608 functions in the same manner as with probe 500. That is, floating electrode 608 intensifies the electric field so as to increase the efficiency of probe 600 when vaporizing or thermally treating tissue.

[0143] Another embodiment, the distal portion of which is depicted in FIGS. 23 through 26, uses bubble trapping and a floating electrode to aggressively vaporize tissue. Probe 700 is analogous in construction to probes 500 and 600, comprised of an insulator 706 mounted to distal end 108 of tubular portion 102, a tubular floating electrode 708 mounted to insulator 706, and an active electrode 702 protruding from the distal portion of insulator 706. Active electrode 702 has a distal-most surface 715 inclined at angle 717 to axis 713. Angle 717 preferably ranges between 0 and 90 degrees, more preferably ranges between 5 and 60 degrees, more preferably between 10 and 55 degrees, even more preferably between 30 and 50. Distal-most surfaces 709 of floating electrode 708 and 711 of insulator 706 are approximately parallel to distal-most surface 715 of active electrode 702. Grooves 721 are of a depth and width suitable for trapping bubbles as taught in the description of probe 100.

[0144] Cutting loop electrodes are well known in the art. For example, Grossi et al, in U.S. Pat. No. 4,917,082, describes a resectoscope electrode that utilizes a formed wire cutting loop as the active electrode. The electrode, intended for use in non-conductive liquids, has insulating tubes (elements 51 and 53 of Grossi FIG. 2) which cover inner sleeves (elements 50 and 52 of Grossi FIG. 2) but cover no portion of the cutting loop (element 48 of Grossi FIG. 2). This is typical of probes designed for use with non-conductive irrigants since, if the irrigant is ideally non-conductive, current flows only from those portions of the uninsulated portions which are in contact with or sufficiently close proximity to tissue. If such a probe is placed in a conductive fluid environment, current flows from all uninsulated surfaces, both those of the formed wire electrode and uninsulated portions of the conductive members. A large portion of the power applied to the probe would flow into the fluid so as to heat the fluid with no clinical benefit. This power loss would necessitate the use of high power levels to achieve the desired cutting action.

[0145] FIGS. 27 through 31 depict a cutting loop electrode configured for use in a liquid environment and constructed in accordance with the principles of this invention. Probe 800, the distal portions of which are shown in the figures, has a pair of laterally opposed, distally extending, insulated conductive members 802 having proximal ends 804 assembled to distal end 108 of tubular member 102. Conductive members 802 are connected via conductive member 120 to proximal end connector 106 (FIG. 1). Distal ends 806 of members 802 have mounted thereto formed electrode 808. Bubble trap 810, made from a suitable dielectric material, is mounted to upper portions 812 of electrode 808. As best seen in FIG. 31, members 802 have a conductive inner portion 814, an insulating coating 816 which covers distal ends 806, upper portion 812

of electrode 808, and portion 811 of bubble trap 810. Tubular floating electrodes 820 are mounted to members 802 adjacent to distal ends 806 of members 802.

[0146] Referring now to FIG. 32 which depicts loop electrode 800 in use, electrode 800 is moved in a proximal direction 830 relative to tissue at the surgical site such that electrode 808 removes a portion of tissue 832. Where electrode 808 is in contact with tissue, current 801 flows from active electrode 808 into the tissue, the high current density present causing vaporization of tissue so as to allow portion 832 to be separated from the remaining tissue. Current also flows from portions of electrode 808 which are uninsulated and in contact with the liquid environment, the current density being sufficient to cause boiling of the fluid adjacent to the wire, and arcing within some of the bubbles. The arcing begins when a bubble reaches a critical size, and stops when the bubble reaches a size which will no longer support arcing. Bubbles which are too large to support arcing may remain in contact with the active electrode due to surface tension, such bubbles thereby insulating the portion of the electrode surface to which they adhere. The buoyancy of the bubbles, and natural convection currents resulting from the heating of the water, act on the bubbles causing them to dislodge from the electrode surface. Conductive flow along the surface of electrode 808 must flow around bubble trap 810, the deflection of the flow causing a region to form beneath bottom surface of bubble trap 810 which is shielded from the convective flow. Bubbles are retained against surface by surface tension, and by the buoyancy of the bubbles. Bubbles beneath these bubbles tend to remain in the region because of surface tension, shielding from convection currents, and buoyancy of the bubbles. The presence of the bubbles, particularly large bubbles, partially insulates the portions of electrode 808 above the tissue so as to reduce current flow from these portions thereby increasing the efficiency of probe 800.

[0147] During use, current (represented by arrows 801) flows from 808 active electrode to the tissue or to the liquid environment. A portion of the current flows through floating electrode 820, entering distal portion which is in a high-potential portion of the electric field formed by active electrode 808, and leaving from floating electrode 820 in more proximal portions which are in lower potential portions of the electric field. The current then flows to the return which may be a dispersive pad, or a return electrode located on the instrument. As with other embodiments, the current flow through the floating electrodes increases the current density in the portions of the field around the floating electrodes. This increased current density increases current flow at the active electrode thereby increasing the electrode efficiency.

[0148] Other configurations of the bubble trap and floating electrode are contemplated in the present invention. For instance, FIG. 33 shows an alternate embodiment in which bubble traps 810 are circular members attached to upper portions 812 (see FIG. 31) of electrode 808. Bubble traps 810 function in the same manner as those of the embodiment depicted in FIGS. 27 through 32. In other embodiments, bubble traps 810 have other shapes such as, for instance, elliptical, oblong, or an irregular shape when viewed in plan view as in FIG. 27. In other embodiments, surface 811 may be non-planar, for example concave, or with raised edges so as to better retain bubbles in contact with surface 811. FIGS. 34 through 36 depict an alternate embodiment in which floating electrode 820 is a planar plate mounted to the upper surface of bubble trap 810. Lateral portions 819 of floating electrode

820 in close proximity to active electrode **808** are in high-potential regions of the electric field. Medial portion **821** of floating electrode **820** is in a lower potential region of the electric field. Current flow in the floating electrode is from the high-potential regions in close proximity to active electrode **808** to medial regions in lower potential regions. This current flow, as with previous embodiments, increases current density in region of the active electrode thereby increasing the instrument efficiency.

[**0149**] Yet another disclosed embodiment may be used to reduce the size of kidney stones so that they can be aspirated from the patient. Referring to FIGS. **37** through **39** which depict the distal portion of an ablator probe for eroding kidney stones, probe **900** has a tubular active electrode **902** which is assembled to tubular member **904** such that active electrode **902** is electrically connected to proximal electrical connector **106** (FIG. **1**). Tubular member **904** and proximal end **906** of ceramic insulator **908** are covered by dielectric coating **910**. Floating electrode **912** is mounted to distal portion **914** of insulator **908**. Floating electrode **912** has a cylindrical proximal portion **916**, and a flared distal portion **918** protruding beyond active electrode **902** by a distance **920**. Lumen **922** of active electrode **902** and lumen **924** of tubular member **904** together form an aspiration path between the distal opening **926** of active electrode **902** and an external vacuum source. In a preferred embodiment, the external vacuum source has a means for controlling the vacuum level.

[**0150**] Referring now to FIG. **40**, depicting probe **900** in use eroding a kidney stone **990**, a slight vacuum applied to opening **926** of active electrode **902** draws conductive liquid down the aspiration path and holds stone **990** in contact with or close proximity to the distal end of probe **900**. Current (represented by arrows **980**) flows from active electrode **902** to the conductive fluid and therefrom to a return electrode, the return electrode being either a dispersive pad (e.g., a monopolar application) or a return electrode on the probe (e.g., a bipolar application). A large portion of the current flows through floating electrode **912**, entering in the distal portion **918** which is in close proximity to active electrode **902**, and exiting in the portions of proximal portion **916** which are in lower potential portions of the electric field. High current density occurs in the conductive liquid in close proximity to both active electrode **902** and floating electrode **912**. This causes rapid localized heating of the fluid, boiling of the fluid, and, when the bubbles formed reach a critical size, arcing within some of the bubbles. Some of the bubbles which intersect the active electrode and the surface of the stone, or which intersect the floating electrode and surface of the stone, support arcs **992** which affect the surface of the stone, vaporizing material in proximity to the arcs. This vaporization, along with fracturing of the stone caused by intense thermal gradients, creates debris which is aspirated from the site via lumen **922** of active electrode **902** and lumen **924** of tubular member **904**. The process continues until stone **990** is sufficiently eroded for aspiration via probe **900** or other means.

[**0151**] In another embodiment configured for removal of kidney stones, a mechanism is provided for grasping a stone, and positioning and retaining it in proximity to the active and floating electrodes. Specifically FIGS. **41** through **45** depict the distal portion of probe **1100** having a subassembly **1101** for grasping stones slidably assembled thereto. Subassembly **1101** has a grasping element **1102** and a tubular control element **1103**. Grasping element **1102** has a tubular proximal portion **1104** and a distal grasping portion **1106** having arms

1108. Arms **1108** have angled distal portions **1110** to aid in grasping a stone, and proximal portions **1112** formed to a radius and attached to the distal end of tubular proximal portion **1104** of element **1102**. Tubular control element **1103** has at its distal end **1114** internal surface portion **1116** of radius **1118**. Control element **1103** is slidably positioned on grasping element **1102** such that, when element **1103** is advanced distally relative to element **1102**, surface **1116** acts on proximal portions **1112** of arms **1108** so as to deflect arms **1108** inwardly so as to grasp a stone in proximity to the distal end of probe **1100**. When a stone has been grasped by arms **1108**, subassembly **1101** (elements **1102** and **1103**) is moved proximally until the stone is in contact with floating electrode **1120**. Active electrode **1122** has a sharpened distal portion **1124** and a proximal portion **1126** which is assembled to conductive tubular member **1128**. Insulator **1130** is assembled to active electrode **1122**. Tubular member **1128** and proximal portion **1132** of insulator **1130** are covered with dielectric coating **1134**.

[**0152**] Referring now to FIG. **46**, which depicts probe **1100** in use, stone **1140** is positioned in close proximity to or contact with floating electrode **1120**. Current (depicted by arrows **1142**) flows from active electrode **1122** to a return electrode located at a remote location (e.g., a monopolar application) or on the instrument (e.g., a bipolar application). A portion of the current flows from active electrode **1122** to portions of floating electrode **1120** in close proximity to the active electrode, and then floating electrode **1120** via the surrounding conductive liquid to the return electrode. A portion of the current flowing to floating electrode **1120** flows through stone **1140**. A portion of this current causes arcing at active electrode **1122** and/or arcing at floating electrode **1120**, the arcing causing erosion and fracturing of stone **1140**.

[**0153**] Aspiration may also be advantageous when vaporizing tissue. Bubbles formed during ablation of tissue may obscure the view of the surgeon and form pockets which displace conductive liquid from the surgical site. An electro-surgical probe formed in accordance with the principles of this invention and having ablation is depicted in FIGS. **47** through **49**. Probe **1000** is constructed identically to probe **100** shown in FIGS. **1** through **9**, but has added thereto aspiration tube **1002** which is in communication with an external vacuum source by means within tubular member **102**. Distal end **1004** of tube **1002** is positioned on the back side of electrode assembly **116** so that liquid aspirated from the site contains only waste heat, rather than process heat as would be the case if distal end **1004** were in close proximity to active electrode **152**.

[**0154**] Referring now to FIGS. **50a** through **55**, which depict the distal-most portion of probe **1200**, referred to herein as the active head, electrode assembly **1216** includes active electrode **1230**, insulator **1232** and floating electrode **1234**. Active electrode **1230** has a plurality of grooves **1236** of width **1238** and depth **1240**, width **1238** and depth **1240** being selected to trap bubbles in the grooves. Active electrode **1230** and floating electrode **1234** are preferably formed from a suitable metallic material, examples of which include, but are not limited to, such as stainless steel, nickel, titanium, tungsten, and the like. Insulator **1232** is preferably formed from a suitable dielectric material, example of which include, but are not limited to, alumina, zirconia, and high-temperature polymers. Members **1210**, insulated by dielectric coating **1211**, have affixed to distal ends **1214** of active electrode **1230** such that electrical power may be conducted by members **1210** to

active electrode **1230**. Members **1210** are connected by at least one conductive member of probe **1200** and external cabling to a suitable RF generator.

[0155] As with previously described embodiments, current flows from active electrode **1230** to the tissue or to the liquid environment, with a portion of the current flowing through floating electrode **1234**. The current then flows to a return which may be a dispersive pad (not shown), or one or more return electrode **1280** located on the probe that are electrically connected to the electrosurgical generator (not shown). As with other embodiments, the current flow through the floating electrodes increases the current density in the portions of the field around the floating electrodes. This increased current density increases current flow at the active electrode thereby increasing the electrode efficiency.

[0156] As best seen in FIG. 55, insulator **1232** has a first portion **1260** which insulates top surfaces **1262** of active electrode **1230**, and a second portion **1264** which electrically isolates floating electrode **1234** from active electrode **1230**. As best seen in FIG. 51, electrode assembly **1216** has a beveled lower portion **1266** formed on the lower distal portion of portion **1264** of insulator **1232** and the lower portion of floating electrode **1234**. When viewed axially in the distal direction as in FIG. 54, floating electrode **1234** and second portion **1264** of insulator **1232** are flush with, or recessed behind active electrode **1230**. Surface **1236** forms an acute angle **1254** with the axis of member **1210**. Angle **1254** is preferably between 0 and 90 degrees, more preferably between 20 and 60 degrees.

[0157] Electrode assembly **1216** of probe **1200** has a simple construction which may be produced at low cost. Active electrode **1230** may be formed by machining using wire Electrical Discharge Machining and conventional machining, or by metal injection molding. Floating electrode **1234** may be stamped at low cost from sheet material. Insulator **1232** may be made by pressing and sintering, or by ceramic injection molding. Active electrode **1230** is joined to insulator **1232**, and insulator **1232** is joined to floating electrode **1234** by a suitable biocompatible adhesive such as, for instance, EP62-1 MED or EP3HTMED epoxies by Master Bond Incorporated (Hackensack, N.J.) or Cement **31** by Sauereisen Incorporated (Pittsburgh, Pa.), all of which maintain their adhesive properties at the temperatures to which assembly **1216** may be heated during use. Alternatively, assembly **1216** may be held together by mechanical means, for example using fasteners such as screws, nuts, rivets or the like. Because members **1210** conduct power to active electrode **1230**, it is not necessary to have a separate conductor such as conductor **126** of probe **100** (FIGS. 5 through 8), thereby further reducing the cost of probe **1200**.

[0158] Probe **1200** is particularly useful for treating Benign Prostatic Hyperplasia (BPH), commonly referred to as enlarged prostate. Surgical treatment of this condition is commonly accomplished using a resectoscope in a procedure referred to as Transurethral Resection of the Prostate (TURP). The resectoscope outer sheath is inserted into the urethra and the distal end advanced until it is near the prostate. The resectoscope working element with telescope and RF probe are inserted into the outer sheath such that the distal end of the probe can be used to modify or remove tissue. Most commonly, a cutting loop electrode (like that taught by Grossi et al in U.S. Pat. No. 4,917,082) is used to cut strips of tissue from the interior of the prostate, the site being filled with non-conductive irrigant. When sufficient tissue has been removed, the site

including the bladder is flushed with irrigant to remove tissue strips that may remain at the site. The time required to flush the tissue from the site is frequently a significant portion of the total procedure time. Additionally, the use of non-conductive irrigant may lead to TUR syndrome, a potentially serious low blood sodium level. Gyms ACMI (Southboro, Mass.) has developed bipolar RF devices which operate in conductive irrigant. One of the products removes tissue by bulk vaporization so as to make removal of remaining tissue strips after resection unnecessary. Because the system is bipolar, its efficiency is low. As a result, high power levels are required to achieve acceptably high tissue removal rates. As noted previously, excessive power levels can lead to unintended injury to local tissue. The bipolar products are usable with conductive irrigants only.

[0159] Probe **1200** may be used to efficiently perform TURP procedures using either non-conductive or conductive irrigants. When non-conductive irrigant is introduced into the body, blood and other highly conductive bodily fluids contaminate the irrigant thereby making it conductive, the level of conductivity depending on the degree of contamination. When probe **1200** is submerged in an irrigant with any level of conductivity, floating electrode **1234** intensifies the electric field in close proximity to active electrode **1230** thereby increasing the current density and making conditions more favorable for tissue vaporization. This allows probe **1200** to be effectively used when either conductive or non-conductive irrigants are supplied to the site, the selection being based on surgeon preference.

[0160] Referring to FIG. 56 depicting probe **1200** in the context of a TURP procedure, probe **1200** is moved in a proximal direction **1278** relative to tissue **1279**. Current (indicated by arrows **1284**) from the RF generator, is supplied to active electrode **1230** by elements **1210**. The current **1284** then flows from active electrode **1230** to a return electrode and therefrom to the generator. A portion of the current flows through tissue **1279** to tissue in close proximity to region **1286** of floating electrode **1234** in close proximity to active electrode **1230**. This current flows through floating electrode **1234** to portion **1288** of floating electrode **1234** in a lower potential region of the electric field, and from floating electrode **1234** to the irrigant and therethrough to the return electrode. Some of the current flowing from active electrode **1230** to tissue **1279** causes boiling of irrigant in close proximity, arcing with the bubbles formed, and vaporization of tissue in the manner previously herein described. A portion of the current flow at region **1286** of floating electrode **1234** may have sufficient density to cause boiling, arcing and vaporization of tissue. A larger portion of the current flow has insufficient density to causing boiling of the irrigant, but does cause heating of the irrigant to elevated temperatures less than 100° C. The heated irrigant in these regions of lower current density causes thermal modification of adjacent tissue, specifically dessication of the tissue resulting in hemostasis.

[0161] When using probe **1200** to perform a TURP, a resectoscope sheath is introduced to the site in the standard manner. The working element with telescope and probe **1200** is inserted into the resectoscope sheath. Probe **1200** is extended distally past the end of the prostate slightly into the bladder. The distal end of the resectoscope is lowered somewhat such that when probe **1200** is energized and retracted proximally into the resectoscope, tissue intersected by active electrode assembly **1216** is vaporized so as to form a channel or groove in the prostate tissue. The scope position is adjusted and the

process repeated to remove additional tissue. The process is repeated until the required volume of tissue is removed. Current flowing between active electrode 1230 and floating electrode 1234 thermally coagulates adjacent tissue thereby producing hemostasis.

[0162] All publications, patent applications, patents and other references mentioned herein are incorporated by reference in their entirety.

[0163] While the invention has been described in detail and with reference to specific embodiments thereof, it will be apparent to one skilled in the art that various changes and modifications can be made therein without departing from the spirit and scope of the invention.

What is claimed:

1. An electrosurgical instrument comprising:
 - a. an elongate conductive shaft having a proximal end configured for connection to an electrosurgical power source and a distal end configured for connection to an electrode assembly;
 - b. an electrode assembly mounted to the distal end of the elongate shaft and comprising an active electrode, a floating electrode, and an insulator separating said active and floating electrodes, wherein:
 - i. said insulator is disposed around said active electrode, and said floating electrode is disposed around said insulator;
 - ii. said insulator is formed from a nonconductive dielectric material whereas said active and floating electrodes are formed from an electrically conductive material;
 - iii. said active and floating electrodes are positioned in close proximity to each other;
 - iv. said active electrode is electrically connected to said conductive member whereas said floating electrode is not directly connected to either the conductive member or the electrosurgical power source;
 - c. a grasping subassembly slidably mounted to a distal portion of the shaft, said assembly comprising a plurality of grasping arms and a tubular control element positioned and axially slidable over said arms, wherein advancement of said control element in a distal direction causes said plurality of arms to deflect inwardly and capture tissue retained therebetween.
2. The electrosurgical instrument of claim 1, each of said grasping arms comprises a radially projecting proximal portion assembled to an angled distal portion.
3. The electrosurgical instrument of claim 1, wherein said grasping subassembly comprises at least three of said grasping arms.
4. The electrosurgical instrument of claim 1, wherein said active electrode further comprises a sharpened distal tip.
5. The electrosurgical instrument of claim 1, wherein said floating electrode comprises a cylindrical proximal portion and a flared distal portion that extends distally past said active electrode.
6. The electrosurgical instrument of claim 1, wherein said instrument comprises a monopolar radiofrequency device.
7. The electrosurgical instrument of claim 1, wherein said instrument comprises a bipolar radiofrequency device.
8. The electrosurgical instrument of claim 7, wherein said bipolar radiofrequency device further comprises a return electrode mounted to said tubular member.

9. The electrosurgical instrument of claim 1, wherein said active electrode and conductive shaft comprise mating lumen for aspirating liquid and ablation products from regions distal to said instrument.

10. A method of removing an obstruction comprising the steps of:

- a. introducing the electrosurgical instrument of claim 1 into a biological vessel or organ of a patient containing an obstruction;
- b. manipulating the instrument such that the distal end of the instrument is proximate to said obstruction;
- c. advancing the control element in a distal direction relative to said grasping arms so as to deflect arms inwardly and capture said obstruction therebetween;
- d. retracting the grasping subassembly in a proximal direction until the obstruction is in contact with or in close proximity to said floating electrode;
- e. applying a high frequency energy to said active electrode so to generate regions of high current density, arcing and thermal gradients that vaporize and fracture the obstruction into smaller particles; and
- f. aspirating the smaller particles via the continuous aspiration path.

11. An ablator probe for eroding an obstruction comprising:

- a. a tubular member having a proximal end configured for connection to an electrosurgical power source and an external vacuum source and a distal end configured for connection to one or more electrodes, wherein said tubular member comprises a first aspiration lumen having proximal and distal openings that extends between the proximal and distal ends of said tubular member;
- b. an insulator disposed about a distal portion of said tubular member;
- c. a tubular active electrode assembled to the distal end of said tubular member, in electrical communication with said electrosurgical power source, and comprising a second aspiration lumen having proximal and distal openings, wherein said second aspiration lumen is in fluid communication with said first aspiration lumen so as to form a continuous aspiration path between the distal opening of said second aspiration lumen and said vacuum source; and
- d. a floating electrode that is not in electrical communication with said electrosurgical power source, wherein said floating electrode is mounted to the distal portion of said tubular member about which said non-conductive coating is disposed.

12. The ablator probe of claim 10, further comprising a grasping subassembly slidably mounted to the distal portion of the tubular member, said assembly comprising a plurality of grasping arms and a tubular control element positioned and axially slidable over said arms, wherein advancement of said control element in a distal direction causes said plurality of arms to deflect inwardly and capture tissue retained therebetween.

13. The electrosurgical instrument of claim 10, each of said grasping arms comprises a radially projecting proximal portion assembled to an angled distal portion.

14. The electrosurgical instrument of claim 10, wherein said grasping subassembly comprises at least three of said grasping arms.

15. The ablator probe of claim **10**, wherein said floating electrode comprises a cylindrical proximal portion and a flared distal portion that extends distally past said active electrode.

16. The ablator probe of claim **10**, wherein said insulator comprises a dielectric coating.

17. The ablator probe of claim **10**, wherein said ablator probe comprises a monopolar radiofrequency device.

18. The ablator probe of claim **10**, wherein said ablator probe comprises a bipolar radiofrequency device.

19. The ablator probe of claim **18**, wherein said bipolar radiofrequency device comprises a return electrode mounted to said tubular member.

20. A method of eroding an obstruction comprising the steps of:

- a. introducing the ablator probe of claim **10** into a biological vessel or organ of a patient containing an obstruction;
- b. manipulating the probe such that the distal end of the probe is proximate to said obstruction;
- c. applying a vacuum to the continuous aspiration path so as to draw conductive liquid down said aspiration path and pull the obstruction into contact or close proximity with the distal opening of said second aspiration lumen;
- d. applying a high frequency energy between said active electrode and said return electrode so to generate regions of high current density, arcing and thermal gradients that vaporize and fracture the obstruction into smaller particles; and
- e. aspirating the smaller particles via the continuous aspiration path.

* * * * *

专利名称(译)	具有浮动电位电极的电外科装置，用于阻塞物移除		
公开(公告)号	US20120245578A1	公开(公告)日	2012-09-27
申请号	US13/493975	申请日	2012-06-11
[标]申请(专利权)人(译)	电子医疗ASSOCS		
申请(专利权)人(译)	电子医疗Associates LLC公司		
当前申请(专利权)人(译)	电子医疗ASSOCIATES, LLC		
[标]发明人	VAN WYK ROBERT A CARMEL YUVAL SHKVARUNETS ANATOLY		
发明人	VAN WYK, ROBERT A. CARMEL, YUVAL SHKVARUNETS, ANATOLY		
IPC分类号	A61B18/14 A61B18/18		
CPC分类号	A61B18/149 A61B2018/00053 A61B2018/0016 A61B2018/00505 A61B2018/00559 A61B18/1482 A61B2018/1213 A61B2018/1407 A61B2018/1427 A61B2218/002 A61B2018/00625		
优先权	60/847496 2006-09-27 US		
其他公开文献	US8790340		
外部链接	Espacenet USPTO		

摘要(译)

本文公开了包括一个或多个浮动电极的电外科装置的实施例，并且特别适于在有或没有外部供应的液体的情况下去除，切割，切除，消融，蒸发，变性，钻孔，凝结和形成软组织中的损伤，优选地。结合切除镜，特别是在泌尿科，妇科，腹腔镜，关节镜和耳鼻喉科手术的背景下。还描述了对泌尿科和妇科应用的具体改编，例如肾结石移除和BPH治疗。

