



US008459520B2

(12) **United States Patent**
Giordano et al.

(10) **Patent No.:** **US 8,459,520 B2**
(45) **Date of Patent:** **Jun. 11, 2013**

(54) **SURGICAL INSTRUMENT WITH WIRELESS
COMMUNICATION BETWEEN CONTROL
UNIT AND REMOTE SENSOR**

(75) Inventors: **James R. Giordano**, Milford, OH (US);
Jeffrey S. Swayze, Hamilton, OH (US);
Frederick E. Shelton, IV, New Vienna,
OH (US)

(73) Assignee: **Ethicon Endo-Surgery, Inc.**, Cincinnati,
OH (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 941 days.

(21) Appl. No.: **11/651,807**

(22) Filed: **Jan. 10, 2007**

(65) **Prior Publication Data**

US 2008/0167672 A1 Jul. 10, 2008

(51) **Int. Cl.**
A61B 17/32 (2006.01)

(52) **U.S. Cl.**
USPC **227/175.1**; 227/180.1; 227/181.1;
227/2; 227/19; 606/219; 606/50; 606/51;
606/52; 606/45; 606/46; 606/47

(58) **Field of Classification Search**
USPC 227/175.1, 180.1, 181.1, 2, 19; 606/219,
606/50–52, 45, 46–47, 159; 74/DIG. 7
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

66,052 A 6/1867 Smith
662,587 A 11/1900 Blake
951,393 A 3/1910 Hahn

2,037,727 A 4/1936 La Chapelle
2,132,295 A 10/1938 Hawkins
2,161,632 A 6/1939 Nattenheimer
2,211,117 A 8/1940 Hess
2,214,870 A 9/1940 West
2,441,096 A 5/1948 Happe
2,526,902 A 10/1950 Rublee
2,674,149 A 4/1954 Benson
2,804,848 A 9/1957 O'Farrell et al.
2,808,482 A 10/1957 Zanichkowsky et al.
2,853,074 A 9/1958 Olson

(Continued)

FOREIGN PATENT DOCUMENTS

CA 2458946 A1 3/2003
CA 2512960 A1 1/2006

(Continued)

OTHER PUBLICATIONS

European Search Report, Application No. 08250080.2, dated Nov. 4,
2009 (7 pages).


(Continued)

Primary Examiner — Brian D Nash
Assistant Examiner — Michelle Lopez

(57) **ABSTRACT**

A surgical instrument, such as an endoscopic or laparoscopic instrument. The surgical instrument may comprise an end effector comprising at least one sensor. The surgical instrument may also comprise an electrically conductive shaft having a distal end connected to the end effector wherein the sensor is electrically insulated from the shaft. The surgical instrument may also comprise a handle connected to a proximate end of the shaft. The handle may comprise a control unit electrically coupled to the shaft such that the shaft radiates signals as an antenna from the control unit to the sensor and receives radiated signals from the sensor. Other components electrically coupled to the shaft may also radiate the signals.

21 Claims, 21 Drawing Sheets

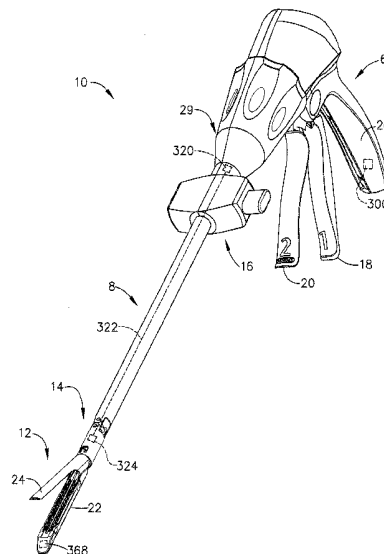

US 8,459,520 B2

Page 2

U.S. PATENT DOCUMENTS

3,032,769	A	5/1962	Palmer	4,606,343	A	8/1986	Conta et al.
3,075,062	A	1/1963	Iaccarino	4,607,638	A	8/1986	Crainich
3,078,465	A	2/1963	Bobrov	4,608,981	A	9/1986	Rothfuss et al.
3,166,072	A	1/1965	Sullivan, Jr.	4,610,250	A	9/1986	Green
3,266,494	A	8/1966	Brownrigg et al.	4,610,383	A	9/1986	Rothfuss et al.
3,269,630	A	8/1966	Fleischer	4,619,262	A	10/1986	Taylor
3,357,296	A	12/1967	Lefever	4,629,107	A	12/1986	Fedotov et al.
3,490,675	A	1/1970	Green et al.	4,632,290	A	12/1986	Green et al.
3,551,987	A	1/1971	Wilkinson	4,633,874	A	1/1987	Chow et al.
3,598,943	A	8/1971	Barrett	4,641,076	A	2/1987	Linden
3,643,851	A	2/1972	Green et al.	4,646,722	A	3/1987	Silverstein et al.
3,662,939	A	5/1972	Bryan	4,655,222	A	4/1987	Florez et al.
3,717,294	A	2/1973	Green	4,663,874	A	5/1987	Sano et al.
3,734,207	A	5/1973	Fishbein	4,664,305	A	5/1987	Blake, III et al.
3,740,994	A	6/1973	DeCarlo, Jr.	4,665,916	A	5/1987	Green
3,744,495	A	7/1973	Johnson	4,667,674	A	5/1987	Korthoff et al.
3,746,002	A	7/1973	Haller	4,671,445	A	6/1987	Barker et al.
3,751,902	A	8/1973	Kingsbury et al.	4,676,245	A	6/1987	Fukuda
3,819,100	A	6/1974	Noiles et al.	4,693,248	A	9/1987	Failla
3,821,919	A	7/1974	Knohl	4,709,120	A	11/1987	Pearson
3,885,491	A	5/1975	Curtis	4,715,520	A	12/1987	Roehr, Jr. et al.
3,892,228	A	7/1975	Mitsui	4,719,917	A	1/1988	Barrows et al.
3,894,174	A	7/1975	Cartun	4,728,020	A	3/1988	Green et al.
3,940,844	A	3/1976	Colby et al.	4,728,876	A	3/1988	Mongeon et al.
RE28,932	E	8/1976	Noiles et al.	4,729,260	A	3/1988	Dudden
4,060,089	A	11/1977	Noiles	4,741,336	A	5/1988	Failla et al.
4,129,059	A	12/1978	Van Eck	4,752,024	A	6/1988	Green et al.
4,213,562	A	7/1980	Garrett et al.	4,754,909	A	7/1988	Barker et al.
4,250,436	A	2/1981	Weissman	4,767,044	A	8/1988	Green
4,261,244	A	4/1981	Becht et al.	4,777,780	A	10/1988	Holzwarth
4,272,662	A	6/1981	Simpson	4,787,387	A	11/1988	Burbank, III et al.
4,275,813	A	6/1981	Noiles	4,790,225	A	12/1988	Moody et al.
4,289,133	A	9/1981	Rothfuss	4,805,617	A	2/1989	Bedi et al.
4,305,539	A	12/1981	Korolkov et al.	4,805,823	A	2/1989	Rothfuss
4,317,451	A	3/1982	Cerwin et al.	4,809,695	A	3/1989	Gwathmey et al.
4,321,002	A	3/1982	Froehlich	4,817,847	A	4/1989	Redtenbacher et al.
4,331,277	A	5/1982	Green	4,819,853	A	4/1989	Green
4,340,331	A	7/1982	Savino	4,821,939	A	4/1989	Green
4,347,450	A	8/1982	Colligan	4,827,911	A	5/1989	Broadwin et al.
4,349,028	A	9/1982	Green	4,844,068	A	7/1989	Arata et al.
4,353,371	A *	10/1982	Cosman 606/42	4,869,414	A	9/1989	Green et al.
4,379,457	A	4/1983	Gravener et al.	4,869,415	A	9/1989	Fox
4,380,312	A	4/1983	Landrus	4,880,015	A	11/1989	Nierman
4,383,634	A	5/1983	Green	4,890,613	A	1/1990	Golden et al.
4,396,139	A	8/1983	Hall et al.	4,892,244	A	1/1990	Fox et al.
4,402,445	A	9/1983	Green	4,915,100	A	4/1990	Green
4,408,692	A	10/1983	Siegel et al.	4,930,503	A	6/1990	Pruitt
4,415,112	A	11/1983	Green	4,932,960	A	6/1990	Green et al.
4,428,376	A	1/1984	Mericle	4,938,408	A	7/1990	Bedi et al.
4,429,695	A	2/1984	Green	4,941,623	A	7/1990	Pruitt
4,434,796	A	3/1984	Karapetian et al.	4,944,443	A	7/1990	Odds et al.
4,442,964	A	4/1984	Becht	4,955,959	A	9/1990	Tompkins et al.
4,451,743	A	5/1984	Suzuki et al.	4,978,049	A	12/1990	Green
4,454,887	A	6/1984	Krüger	4,986,808	A	1/1991	Broadwin et al.
4,467,805	A	8/1984	Fukuda	4,988,334	A	1/1991	Hornlein et al.
4,475,679	A	10/1984	Fleury, Jr.	5,002,553	A	3/1991	Shiber
4,485,816	A	12/1984	Krumme	5,009,661	A	4/1991	Michelson
4,489,875	A	12/1984	Crawford et al.	5,014,899	A	5/1991	Presty et al.
4,500,024	A	2/1985	DiGiovanni et al.	5,015,227	A	5/1991	Broadwin et al.
4,505,273	A	3/1985	Braun et al.	5,027,834	A	7/1991	Pruitt
4,505,414	A	3/1985	Filipi	5,031,814	A	7/1991	Tompkins et al.
4,506,671	A	3/1985	Green	5,040,715	A	8/1991	Green et al.
4,520,817	A	6/1985	Green	5,042,707	A	8/1991	Taheri
4,522,327	A	6/1985	Korthoff et al.	5,061,269	A	10/1991	Muller
4,526,174	A	7/1985	Froehlich	5,062,563	A	11/1991	Green et al.
4,527,724	A	7/1985	Chow et al.	5,065,929	A	11/1991	Schulze et al.
4,530,453	A	7/1985	Green	5,071,052	A	12/1991	Rodak et al.
4,548,202	A	10/1985	Duncan	5,071,430	A	12/1991	de Salis et al.
4,565,189	A	1/1986	Mabuchi	5,074,454	A	12/1991	Peters
4,566,620	A	1/1986	Green et al.	5,080,556	A	1/1992	Carreno
4,573,469	A	3/1986	Golden et al.	5,083,695	A	1/1992	Foslien et al.
4,573,622	A	3/1986	Green et al.	5,084,057	A	1/1992	Green et al.
4,576,167	A	3/1986	Noiles et al.	5,088,979	A	2/1992	Filipi et al.
4,580,712	A	4/1986	Green	5,088,997	A	2/1992	Delahuerga et al.
4,589,416	A	5/1986	Green	5,094,247	A	3/1992	Hernandez et al.
4,591,085	A	5/1986	Di Giovanni	5,100,420	A	3/1992	Green et al.
4,604,786	A	8/1986	Howie, Jr.	5,104,025	A	4/1992	Main et al.
4,605,001	A	8/1986	Rothfuss et al.	5,106,008	A	4/1992	Tompkins et al.
				5,111,987	A	5/1992	Moeinzadeh et al.

US 8,459,520 B2

Page 3

5,116,349 A	5/1992	Aranyi	5,359,231 A	10/1994	Flowers et al.
5,129,570 A	7/1992	Schulze et al.	D352,780 S	11/1994	Glaeser et al.
5,137,198 A	8/1992	Nobis et al.	5,360,428 A	11/1994	Hutchinson, Jr.
5,139,513 A	8/1992	Segato	5,364,003 A	11/1994	Williamson, IV
5,141,144 A	8/1992	Foslien et al.	5,366,134 A	11/1994	Green et al.
5,156,315 A	10/1992	Green et al.	5,366,479 A	11/1994	McGarry et al.
5,156,614 A	10/1992	Green et al.	5,368,015 A *	11/1994	Wilk 600/104
5,158,567 A	10/1992	Green	5,370,645 A	12/1994	Klicek et al.
D330,699 S	11/1992	Gill	5,372,596 A	12/1994	Klicek et al.
5,163,598 A	11/1992	Peters et al.	5,372,602 A	12/1994	Burke
5,171,247 A	12/1992	Hughett et al.	5,374,277 A	12/1994	Hassler
5,171,249 A	12/1992	Stefanchik et al.	5,379,933 A	1/1995	Green et al.
5,188,111 A	2/1993	Yates et al.	5,381,782 A	1/1995	DeLaRama et al.
5,190,517 A	3/1993	Zieve et al.	5,382,247 A	1/1995	Cimino et al.
5,195,968 A	3/1993	Lundquist et al.	5,383,880 A	1/1995	Hooven
5,197,648 A	3/1993	Gingold	5,383,881 A	1/1995	Green et al.
5,200,280 A	4/1993	Karasa	5,383,888 A	1/1995	Zvenyatsky et al.
5,205,459 A	4/1993	Brinkerhoff et al.	5,383,895 A	1/1995	Holmes et al.
5,207,697 A	5/1993	Carusillo et al.	5,389,098 A	2/1995	Tsuruta et al.
5,209,747 A	5/1993	Knoepfler	5,391,180 A	2/1995	Tovey et al.
5,211,649 A	5/1993	Kohler et al.	5,392,979 A	2/1995	Green et al.
5,217,457 A	6/1993	Delahuerga et al.	5,395,030 A	3/1995	Kuramoto et al.
5,217,478 A	6/1993	Rexroth	5,395,033 A	3/1995	Byrne et al.
5,219,111 A	6/1993	Bilotti et al.	5,395,312 A	3/1995	Desai
5,221,036 A	6/1993	Takase	5,397,046 A	3/1995	Savage et al.
5,221,281 A	6/1993	Klicek	5,397,324 A	3/1995	Carroll et al.
5,222,963 A	6/1993	Brinkerhoff et al.	5,403,312 A	4/1995	Yates et al.
5,222,975 A	6/1993	Crainich	5,405,072 A	4/1995	Zlock et al.
5,222,976 A	6/1993	Yoon	5,405,344 A	4/1995	Williamson et al.
5,223,675 A	6/1993	Taft	5,407,293 A	4/1995	Crainich
5,234,447 A	8/1993	Kaster et al.	5,409,498 A	4/1995	Braddock et al.
5,236,440 A	8/1993	Hlavacek	5,411,508 A	5/1995	Bessler et al.
5,239,981 A	8/1993	Anaplotis	5,413,267 A	5/1995	Solyntjes et al.
5,240,163 A	8/1993	Stein et al.	5,413,268 A	5/1995	Green et al.
5,242,457 A	9/1993	Akopov et al.	5,413,272 A	5/1995	Green et al.
5,244,462 A	9/1993	Delahuerga et al.	5,415,334 A	5/1995	Williamson, IV et al.
5,246,156 A	9/1993	Rothfuss et al.	5,415,335 A	5/1995	Knodell, Jr.
5,246,443 A	9/1993	Mai	5,417,361 A	5/1995	Williamson, IV
5,253,793 A	10/1993	Green et al.	5,421,829 A	6/1995	Olichney et al.
5,258,009 A	11/1993	Connors	5,422,567 A	6/1995	Matsunaga
5,258,012 A	11/1993	Luscombe et al.	5,423,809 A	6/1995	Klicek
5,259,366 A	11/1993	Reydel et al.	5,425,745 A	6/1995	Green et al.
5,260,637 A	11/1993	Pizzi	5,431,322 A	7/1995	Green et al.
5,263,629 A	11/1993	Trumbull et al.	5,431,668 A	7/1995	Burbank, III et al.
5,263,973 A	11/1993	Cook	5,433,721 A	7/1995	Hooven et al.
5,268,622 A	12/1993	Philipp	5,438,302 A	8/1995	Goble
5,271,543 A	12/1993	Grant et al.	5,439,479 A	8/1995	Shichman et al.
5,271,544 A	12/1993	Fox et al.	5,441,193 A	8/1995	Gravener
RE34,519 E	1/1994	Fox et al.	5,441,494 A	8/1995	Ortiz
5,275,323 A	1/1994	Schulze et al.	5,445,304 A	8/1995	Plyley et al.
5,275,608 A	1/1994	Forman et al.	5,445,644 A	8/1995	Pietrafitta et al.
5,281,216 A	1/1994	Klicek	5,447,417 A	9/1995	Kuhl et al.
5,282,806 A	2/1994	Haber et al.	5,447,513 A	9/1995	Davison et al.
5,282,829 A	2/1994	Hermes	5,449,355 A	9/1995	Rhum et al.
5,297,714 A	3/1994	Kramer	5,449,365 A	9/1995	Green et al.
5,304,204 A	4/1994	Bregen	5,452,836 A	9/1995	Huitema et al.
5,307,976 A	5/1994	Olson et al.	5,452,837 A	9/1995	Williamson, IV et al.
5,309,927 A	5/1994	Welch	5,454,827 A	10/1995	Aust et al.
5,312,023 A	5/1994	Green et al.	5,456,401 A	10/1995	Green et al.
5,312,329 A	5/1994	Beaty et al.	5,458,579 A	10/1995	Chodorow et al.
5,314,424 A	5/1994	Nicholas	5,462,215 A	10/1995	Viola et al.
5,318,221 A	6/1994	Green et al.	5,464,300 A	11/1995	Crainich
5,330,502 A	7/1994	Hassler et al.	5,465,894 A	11/1995	Clark et al.
5,332,142 A	7/1994	Robinson et al.	5,465,895 A	11/1995	Knodel et al.
5,333,422 A	8/1994	Warren et al.	5,465,896 A	11/1995	Allen et al.
5,334,183 A	8/1994	Wuchinich	5,466,020 A	11/1995	Page et al.
5,336,232 A	8/1994	Green et al.	5,467,911 A	11/1995	Tsuruta et al.
5,339,799 A	8/1994	Kami et al.	5,470,006 A	11/1995	Rodak
5,341,724 A	8/1994	Vatel	5,470,007 A	11/1995	Plyley et al.
5,341,810 A	8/1994	Dardel	5,472,132 A	12/1995	Savage et al.
5,342,395 A	8/1994	Jarrett et al.	5,472,442 A	12/1995	Klicek
5,342,396 A	8/1994	Cook	5,473,204 A	12/1995	Temple
5,344,060 A	9/1994	Gravener et al.	5,474,057 A	12/1995	Makower et al.
5,350,400 A	9/1994	Esposito et al.	5,474,566 A	12/1995	Alesi et al.
5,352,235 A	10/1994	Koros et al.	5,476,206 A	12/1995	Green et al.
5,352,238 A	10/1994	Green et al.	5,476,479 A	12/1995	Green et al.
5,354,303 A	10/1994	Spaeth et al.	5,478,003 A	12/1995	Green et al.
5,356,006 A	10/1994	Alpern et al.	5,478,354 A	12/1995	Tovey et al.
5,358,510 A	10/1994	Luscombe et al.	5,480,089 A	1/1996	Blewett

US 8,459,520 B2

Page 4

5,480,409 A	1/1996	Riza	5,588,581 A	12/1996	Conlon et al.
5,482,197 A	1/1996	Green et al.	5,591,170 A	1/1997	Spievack et al.
5,484,095 A	1/1996	Green et al.	5,591,187 A	1/1997	Dekel
5,484,398 A	1/1996	Stoddard	5,597,107 A	1/1997	Knodel et al.
5,484,451 A	1/1996	Akopov et al.	5,599,151 A	2/1997	Daum et al.
5,485,947 A	1/1996	Olson et al.	5,599,344 A	2/1997	Paterson
5,485,952 A	1/1996	Fontayne	5,599,350 A	2/1997	Schulze et al.
5,487,499 A	1/1996	Sorrentino et al.	5,601,224 A	2/1997	Bishop et al.
5,487,500 A	1/1996	Knodel et al.	5,603,443 A	2/1997	Clark et al.
5,489,058 A	2/1996	Plyley et al.	5,605,272 A	2/1997	Witt et al.
5,489,256 A	2/1996	Adair	5,605,273 A	2/1997	Hamblin et al.
5,496,312 A	3/1996	Klicek	5,607,094 A	3/1997	Clark et al.
5,496,317 A	3/1996	Goble et al.	5,607,095 A	3/1997	Smith et al.
5,497,933 A	3/1996	DeFonzo et al.	5,607,450 A	3/1997	Zvenyatsky et al.
5,503,320 A	4/1996	Webster et al.	5,609,285 A	3/1997	Grant et al.
5,503,635 A	4/1996	Sauer et al.	5,611,709 A	3/1997	McAnulty
5,503,638 A	4/1996	Cooper et al.	5,613,966 A	3/1997	Makower et al.
5,505,363 A	4/1996	Green et al.	5,618,294 A	4/1997	Aust et al.
5,507,426 A	4/1996	Young et al.	5,618,303 A	4/1997	Marlow et al.
5,509,596 A	4/1996	Green et al.	5,620,289 A	4/1997	Curry
5,509,916 A	4/1996	Taylor	5,620,452 A	4/1997	Yoon
5,511,564 A	4/1996	Wilk	5,624,452 A	4/1997	Yates
5,514,129 A	5/1996	Smith	5,626,587 A	5/1997	Bishop et al.
5,514,157 A	5/1996	Nicholas et al.	5,628,446 A	5/1997	Geiste et al.
5,518,163 A	5/1996	Hooven	5,628,743 A	5/1997	Cimino
5,518,164 A	5/1996	Hooven	5,630,539 A	5/1997	Plyley et al.
5,520,678 A	5/1996	Heckele et al.	5,630,540 A	5/1997	Blewett
5,520,700 A	5/1996	Beyar et al.	5,630,782 A	5/1997	Adair
5,522,817 A	6/1996	Sander et al.	5,632,432 A	5/1997	Schulze et al.
5,527,320 A	6/1996	Carruthers et al.	5,632,433 A	5/1997	Grant et al.
5,529,235 A	6/1996	Boiarski et al.	5,634,584 A	6/1997	Okorocho et al.
D372,086 S	7/1996	Grasso et al.	5,636,779 A	6/1997	Palmer
5,531,744 A	7/1996	Nardella et al.	5,636,780 A	6/1997	Green et al.
5,533,521 A	7/1996	Granger	5,639,008 A	6/1997	Gallagher et al.
5,533,581 A	7/1996	Barth et al.	5,643,291 A	7/1997	Pier et al.
5,533,661 A	7/1996	Main et al.	5,645,209 A	7/1997	Green et al.
5,535,934 A	7/1996	Boiarski et al.	5,647,526 A	7/1997	Green et al.
5,535,935 A	7/1996	Vidal et al.	5,647,869 A	7/1997	Goble et al.
5,535,937 A	7/1996	Boiarski et al.	5,649,937 A	7/1997	Bito et al.
5,540,375 A	7/1996	Bolanos et al.	5,651,491 A	7/1997	Heaton et al.
5,541,376 A	7/1996	Ladtchow et al.	5,653,373 A	8/1997	Green et al.
5,542,594 A	8/1996	McKean et al.	5,653,374 A	8/1997	Young et al.
5,543,119 A	8/1996	Sutter et al.	5,653,677 A	8/1997	Okada et al.
5,547,117 A	8/1996	Hamblin et al.	5,653,721 A	8/1997	Knodel et al.
5,549,621 A	8/1996	Bessler et al.	5,655,698 A	8/1997	Yoon
5,549,628 A	8/1996	Cooper et al.	5,657,921 A	8/1997	Young et al.
5,549,637 A	8/1996	Crainich	5,658,281 A	8/1997	Heard
5,553,675 A	9/1996	Pitzen et al.	5,658,300 A	8/1997	Bito et al.
5,553,765 A	9/1996	Knodel et al.	5,662,258 A	9/1997	Knodel et al.
5,554,169 A	9/1996	Green et al.	5,662,260 A	9/1997	Yoon
5,556,416 A	9/1996	Clark et al.	5,662,662 A	9/1997	Bishop et al.
5,558,665 A	9/1996	Kieturakis	5,667,517 A	9/1997	Hooven
5,558,671 A	9/1996	Yates	5,667,526 A	9/1997	Levin
5,560,530 A	10/1996	Bolanos et al.	5,667,527 A	9/1997	Cook
5,560,532 A	10/1996	DeFonzo et al.	5,669,544 A	9/1997	Schulze et al.
5,562,239 A *	10/1996	Boiarski et al. 227/175.2	5,669,904 A	9/1997	Platt, Jr. et al.
5,562,241 A	10/1996	Knodel et al.	5,669,907 A	9/1997	Platt, Jr. et al.
5,562,682 A	10/1996	Oberlin et al.	5,669,918 A	9/1997	Balazs et al.
5,562,701 A	10/1996	Huitema et al.	5,673,840 A	10/1997	Schulze et al.
5,562,702 A	10/1996	Huitema et al.	5,673,841 A	10/1997	Schulze et al.
5,564,615 A	10/1996	Bishop et al.	5,673,842 A	10/1997	Bittner et al.
5,569,161 A	10/1996	Ebling et al.	5,678,748 A	10/1997	Plyley et al.
5,571,090 A	11/1996	Sherts	5,680,981 A	10/1997	Mililli et al.
5,571,100 A	11/1996	Goble et al.	5,680,982 A	10/1997	Schulze et al.
5,571,116 A	11/1996	Bolanos et al.	5,680,983 A	10/1997	Plyley et al.
5,573,543 A	11/1996	Akopov et al.	5,683,349 A	11/1997	Makower et al.
5,574,431 A	11/1996	McKeown et al.	5,685,474 A	11/1997	Seeber
5,575,789 A	11/1996	Bell et al.	5,688,270 A	11/1997	Yates et al.
5,575,799 A	11/1996	Bolanos et al.	5,690,269 A	11/1997	Bolanos et al.
5,575,803 A	11/1996	Cooper et al.	5,692,668 A	12/1997	Schulze et al.
5,577,654 A	11/1996	Bishop	5,693,042 A	12/1997	Boiarski et al.
5,579,978 A	12/1996	Green et al.	5,693,051 A	12/1997	Schulze et al.
5,580,067 A	12/1996	Hamblin et al.	5,695,494 A	12/1997	Becker
5,582,611 A	12/1996	Tsuruta et al.	5,695,504 A	12/1997	Gifford, III et al.
5,582,617 A	12/1996	Klieman et al.	5,695,524 A	12/1997	Kelley et al.
5,584,425 A	12/1996	Savage et al.	5,697,543 A	12/1997	Burdorff
5,586,711 A	12/1996	Plyley et al.	5,697,943 A	12/1997	Sauer et al.
5,588,579 A	12/1996	Schnut et al.	5,700,270 A	12/1997	Peyser et al.
5,588,580 A	12/1996	Paul et al.	5,702,387 A	12/1997	Arts et al.

5,702,408 A	12/1997	Wales et al.	5,817,109 A	10/1998	McGarry et al.
5,702,409 A	12/1997	Rayburn et al.	5,817,119 A	10/1998	Klieman et al.
5,704,087 A	1/1998	Strub	5,820,009 A	10/1998	Melling et al.
5,704,534 A	1/1998	Huitema et al.	5,823,066 A	10/1998	Huitema et al.
5,706,997 A	1/1998	Green et al.	5,826,776 A	10/1998	Schulze et al.
5,706,998 A	1/1998	Plyley et al.	5,827,271 A	10/1998	Buyse et al.
5,707,392 A	1/1998	Kortenbach	5,829,662 A	11/1998	Allen et al.
5,709,334 A	1/1998	Sorrentino et al.	5,833,690 A	11/1998	Yates et al.
5,709,680 A	1/1998	Yates et al.	5,833,695 A	11/1998	Yoon
5,711,472 A	1/1998	Bryan	5,833,696 A	11/1998	Whitfield et al.
5,713,128 A	2/1998	Schrenk et al.	5,836,503 A	11/1998	Ehrenfels et al.
5,713,505 A	2/1998	Huitema	5,836,960 A	11/1998	Kolesa et al.
5,713,895 A	2/1998	Lontine et al.	5,839,639 A	11/1998	Sauer et al.
5,715,987 A	2/1998	Kelley et al.	5,843,132 A	12/1998	Ilvento
5,715,988 A	2/1998	Palmer	5,846,254 A	12/1998	Schulze et al.
5,716,366 A	2/1998	Yates	5,849,011 A	12/1998	Jones et al.
5,718,359 A	2/1998	Palmer et al.	5,855,311 A	1/1999	Hamblin et al.
5,718,360 A	2/1998	Green et al.	5,855,583 A	1/1999	Wang et al.
5,718,548 A	2/1998	Cotellessa	5,860,975 A	1/1999	Goble et al.
5,720,744 A	2/1998	Eggleston et al.	5,865,361 A	2/1999	Milliman et al.
D393,067 S	3/1998	Geary et al.	5,868,760 A	2/1999	McGuckin, Jr.
5,725,536 A	3/1998	Oberlin et al.	5,871,135 A	2/1999	Williamson, IV et al.
5,725,554 A	3/1998	Simon et al.	5,873,885 A	2/1999	Weidenbenner
5,728,121 A	3/1998	Bimbo et al.	5,876,401 A	3/1999	Schulze et al.
5,730,758 A	3/1998	Allgeyer	5,878,193 A	3/1999	Wang et al.
5,732,871 A	3/1998	Clark et al.	5,878,937 A	3/1999	Green et al.
5,732,872 A	3/1998	Bolduc et al.	5,878,938 A	3/1999	Bittner et al.
5,735,445 A	4/1998	Vidal et al.	5,891,160 A	4/1999	Williamson, IV et al.
5,735,848 A	4/1998	Yates et al.	5,893,506 A	4/1999	Powell
5,735,874 A	4/1998	Measamer et al.	5,894,979 A	4/1999	Powell
5,738,474 A	4/1998	Blewett	5,897,562 A	4/1999	Bolanos et al.
5,738,648 A	4/1998	Lands et al.	5,899,914 A	5/1999	Zirps et al.
5,743,456 A	4/1998	Jones et al.	5,901,895 A	5/1999	Heaton et al.
5,747,953 A	5/1998	Philipp	5,902,312 A	5/1999	Frater et al.
5,749,889 A	5/1998	Bacich et al.	5,904,693 A	5/1999	Dicesare et al.
5,749,893 A	5/1998	Vidal et al.	5,906,625 A	5/1999	Bitto et al.
5,752,644 A	5/1998	Bolanos et al.	5,908,402 A	6/1999	Blythe
5,752,965 A	5/1998	Francis et al.	5,908,427 A	6/1999	McKean et al.
5,755,717 A	5/1998	Yates et al.	5,911,353 A	6/1999	Bolanos et al.
5,758,814 A	6/1998	Gallagher et al.	5,915,616 A	6/1999	Viola et al.
5,762,255 A	6/1998	Chrisman et al.	5,918,791 A	7/1999	Sorrentino et al.
5,762,256 A	6/1998	Mastri et al.	5,919,198 A	7/1999	Graves, Jr. et al.
5,766,188 A	6/1998	Igaki	5,928,256 A	7/1999	Riza
5,766,205 A	6/1998	Zvenyatsky et al.	5,931,847 A	8/1999	Bittner et al.
5,769,892 A	6/1998	Kingwell	5,931,853 A	8/1999	McEwen et al.
5,772,379 A	6/1998	Evensen	5,937,951 A	8/1999	Izuchukwu et al.
5,772,578 A	6/1998	Heimberger et al.	5,938,667 A	8/1999	Peyser et al.
5,772,659 A	6/1998	Becker et al.	5,941,442 A	8/1999	Geiste et al.
5,776,130 A	7/1998	Buyse et al.	5,944,172 A	8/1999	Hannula
5,779,130 A	7/1998	Alesi et al.	5,944,715 A	8/1999	Goble et al.
5,779,131 A	7/1998	Knodel et al.	5,948,030 A	9/1999	Miller et al.
5,779,132 A	7/1998	Knodel et al.	5,951,552 A	9/1999	Long et al.
5,782,396 A	7/1998	Mastri et al.	5,951,574 A	9/1999	Stefanchik et al.
5,782,397 A	7/1998	Koukline	5,954,259 A	9/1999	Viola et al.
5,782,749 A	7/1998	Riza	5,964,774 A	10/1999	McKean et al.
5,782,859 A	7/1998	Nicholas et al.	5,971,916 A	10/1999	Koren
5,784,934 A	7/1998	Izumisawa	5,988,479 A	11/1999	Palmer
5,785,232 A	7/1998	Vidal et al.	6,003,517 A	12/1999	Sheffield et al.
5,787,897 A	8/1998	Kieturakis	6,004,319 A	12/1999	Goble et al.
5,792,135 A	8/1998	Madhani et al.	6,010,054 A	1/2000	Johnson et al.
5,792,165 A	8/1998	Klieman et al.	6,012,494 A	1/2000	Balazs
5,794,834 A	8/1998	Hamblin et al.	6,013,076 A	1/2000	Goble et al.
5,796,188 A	8/1998	Bays	6,015,406 A	1/2000	Goble et al.
5,797,536 A	8/1998	Smith et al.	6,017,322 A	1/2000	Snoke et al.
5,797,537 A	8/1998	Oberlin et al.	6,017,356 A	1/2000	Frederick et al.
5,797,538 A	8/1998	Heaton et al.	6,022,352 A	2/2000	Vandewalle
5,797,906 A	8/1998	Rhum et al.	6,024,741 A	2/2000	Williamson, IV et al.
5,797,959 A	8/1998	Castro et al.	6,024,748 A	2/2000	Manzo et al.
5,799,857 A	9/1998	Robertson et al.	6,027,501 A	2/2000	Goble et al.
5,807,378 A	9/1998	Jensen et al.	6,032,849 A	3/2000	Mastri et al.
5,807,393 A	9/1998	Williamson, IV et al.	6,033,378 A	3/2000	Lundquist et al.
5,809,441 A	9/1998	McKee	6,033,399 A	3/2000	Gines
5,810,811 A	9/1998	Yates et al.	6,033,427 A	3/2000	Lee
5,810,855 A	9/1998	Rayburn et al.	6,039,733 A	3/2000	Buyse et al.
5,813,813 A	9/1998	Daum et al.	6,039,734 A *	3/2000	Goble 606/41
5,814,057 A	9/1998	Oi et al.	6,045,560 A	4/2000	McKean et al.
5,817,084 A	10/1998	Jensen	6,050,472 A	4/2000	Shibata
5,817,091 A	10/1998	Nardella et al.	6,053,390 A	4/2000	Green et al.
5,817,093 A	10/1998	Williamson, IV et al.	6,056,746 A	5/2000	Goble et al.

US 8,459,520 B2

Page 6

6,063,097	A	5/2000	Oi et al.	6,358,224	B1	3/2002	Tims et al.
6,063,098	A	5/2000	Houser et al.	6,364,877	B1	4/2002	Goble et al.
6,068,627	A	5/2000	Orszulak et al.	6,364,888	B1	4/2002	Niemeyer et al.
6,071,233	A	6/2000	Ishikawa et al.	6,373,152	B1	4/2002	Wang et al.
6,074,386	A	6/2000	Goble et al.	6,387,113	B1	5/2002	Hawkins et al.
6,077,286	A	6/2000	Cuschieri et al.	6,387,114	B2	5/2002	Adams
6,079,606	A	6/2000	Milliman et al.	6,391,038	B2	5/2002	Vargas et al.
6,082,577	A	7/2000	Coates et al.	6,398,781	B1	6/2002	Goble et al.
6,083,234	A	7/2000	Nicholas et al.	6,398,797	B2	6/2002	Bombard et al.
6,083,242	A	7/2000	Cook	6,406,440	B1	6/2002	Stefanchik
6,086,600	A	7/2000	Kortenbach	6,409,724	B1	6/2002	Penny et al.
6,090,106	A	7/2000	Goble et al.	H2037	H	7/2002	Yates et al.
6,093,186	A	7/2000	Goble	6,416,486	B1	7/2002	Wampler
6,099,537	A	8/2000	Sugai et al.	6,416,509	B1	7/2002	Goble et al.
6,099,551	A	8/2000	Gabbay	6,419,695	B1	7/2002	Gabbay
6,102,271	A	8/2000	Longo et al.	RE37,814	E	8/2002	Allgeyer
6,109,500	A	8/2000	Alli et al.	6,436,097	B1	8/2002	Nardella
6,117,158	A	9/2000	Measamer et al.	6,436,107	B1	8/2002	Wang et al.
6,119,913	A	9/2000	Adams et al.	6,436,122	B1	8/2002	Frank et al.
6,120,433	A	9/2000	Mizuno et al.	6,439,446	B1	8/2002	Perry et al.
6,123,241	A	9/2000	Walter et al.	6,440,146	B2	8/2002	Nicholas et al.
H1904	H	10/2000	Yates et al.	6,443,973	B1	9/2002	Whitman
6,126,058	A	10/2000	Adams et al.	6,450,391	B1	9/2002	Kayan et al.
6,126,670	A	10/2000	Walker et al.	6,468,275	B1	10/2002	Wampler et al.
6,131,789	A	10/2000	Schulze et al.	6,471,106	B1	10/2002	Reining
6,132,368	A	10/2000	Cooper	6,482,200	B2	11/2002	Shippert
6,139,546	A	10/2000	Koenig et al.	6,485,490	B2	11/2002	Wampler et al.
6,155,473	A	12/2000	Tompkins et al.	6,488,196	B1	12/2002	Fenton, Jr.
6,156,056	A	12/2000	Kearns et al.	6,488,197	B1	12/2002	Whitman
6,159,146	A	12/2000	El Gazayerli	6,491,201	B1	12/2002	Whitman
6,159,200	A	12/2000	Verdura et al.	6,491,690	B1	12/2002	Goble et al.
6,162,208	A	12/2000	Hipps	6,491,701	B2	12/2002	Tierney et al.
6,165,175	A	12/2000	Wampler et al.	6,492,785	B1	12/2002	Kasten et al.
6,165,184	A	12/2000	Verdura et al.	6,494,896	B1	12/2002	D'Alessio et al.
6,168,605	B1	1/2001	Measamer et al.	6,503,257	B2	1/2003	Grant et al.
6,171,316	B1	1/2001	Kovac et al.	6,503,259	B2	1/2003	Huxel et al.
6,171,330	B1	1/2001	Benchetrit	6,505,768	B2	1/2003	Whitman
6,174,308	B1	1/2001	Goble et al.	6,510,854	B2	1/2003	Goble
6,174,309	B1	1/2001	Wrublewski et al.	6,511,468	B1	1/2003	Cragg et al.
6,179,776	B1	1/2001	Adams et al.	6,517,535	B2	2/2003	Edwards
6,181,105	B1	1/2001	Cutolo et al.	6,517,565	B1	2/2003	Whitman et al.
6,193,129	B1	2/2001	Bittner et al.	6,517,566	B1	2/2003	Hovland et al.
6,197,042	B1	3/2001	Ginn et al.	6,522,101	B2	2/2003	Malackowski
6,202,914	B1	3/2001	Geiste et al.	6,543,456	B1	4/2003	Freeman
6,214,028	B1	4/2001	Yoon et al.	6,547,786	B1	4/2003	Goble
6,220,368	B1	4/2001	Ark et al.	6,550,546	B2	4/2003	Thurler et al.
6,223,835	B1	5/2001	Habedank et al.	6,551,333	B2	4/2003	Kuhns et al.
6,228,081	B1	5/2001	Goble	6,554,861	B2	4/2003	Knox et al.
6,228,084	B1	5/2001	Kirwan, Jr.	6,558,379	B1	5/2003	Batchelor et al.
6,231,565	B1	5/2001	Tovey et al.	6,565,560	B1	5/2003	Goble et al.
6,234,178	B1	5/2001	Goble et al.	6,569,085	B2	5/2003	Kortenbach et al.
6,241,139	B1	6/2001	Milliman et al.	6,569,171	B2	5/2003	DeGuillebon et al.
6,241,723	B1	6/2001	Heim et al.	6,578,751	B2	6/2003	Hartwick
6,249,076	B1	6/2001	Madden et al.	6,582,427	B1	6/2003	Goble et al.
6,250,532	B1	6/2001	Green et al.	6,588,643	B2	7/2003	Bolduc et al.
6,258,107	B1	7/2001	Balázs et al.	6,589,164	B1	7/2003	Flaherty
6,261,286	B1	7/2001	Goble et al.	6,592,597	B2	7/2003	Grant et al.
6,264,086	B1	7/2001	McGuckin, Jr.	6,596,432	B2	7/2003	Kawakami et al.
6,264,087	B1	7/2001	Whitman	D478,665	S	8/2003	Isaacs et al.
6,270,508	B1	8/2001	Klieman et al.	D478,986	S	8/2003	Johnston et al.
6,273,897	B1	8/2001	Dalessandro et al.	6,601,749	B2	8/2003	Sullivan et al.
6,277,114	B1	8/2001	Bullivant et al.	6,602,252	B2	8/2003	Mollenauer
6,293,942	B1	9/2001	Goble et al.	6,605,078	B2	8/2003	Adams
6,296,640	B1	10/2001	Wampler et al.	6,605,669	B2	8/2003	Awokola et al.
6,302,311	B1	10/2001	Adams et al.	6,616,686	B2	9/2003	Coleman et al.
6,306,134	B1	10/2001	Goble et al.	6,619,529	B2	9/2003	Green et al.
6,309,403	B1	10/2001	Minor et al.	6,620,166	B1	9/2003	Wenstrom, Jr. et al.
6,315,184	B1	11/2001	Whitman	6,629,630	B2	10/2003	Adams
6,320,123	B1	11/2001	Reimers	6,629,974	B2	10/2003	Penny et al.
6,324,339	B1	11/2001	Hudson et al.	6,629,988	B2	10/2003	Weadock
6,325,799	B1	12/2001	Goble	6,636,412	B2	10/2003	Smith
6,325,810	B1	12/2001	Hamilton et al.	6,638,108	B2	10/2003	Tachi
6,330,965	B1	12/2001	Milliman et al.	6,638,285	B2	10/2003	Gabbay
6,331,181	B1	12/2001	Tierney et al.	6,641,528	B2	11/2003	Torii
6,331,761	B1	12/2001	Kumar et al.	6,644,532	B2	11/2003	Green et al.
6,334,860	B1	1/2002	Dorn	6,648,816	B2	11/2003	Irion et al.
6,336,926	B1	1/2002	Goble	D484,243	S	12/2003	Ryan et al.
6,346,077	B1	2/2002	Taylor et al.	D484,595	S	12/2003	Ryan et al.
6,352,503	B1	3/2002	Matsui et al.	D484,596	S	12/2003	Ryan et al.

6,656,193	B2	12/2003	Grant et al.	6,913,613	B2	7/2005	Schwarz et al.
6,666,875	B1	12/2003	Sakurai et al.	6,923,803	B2	8/2005	Goble
6,669,073	B2	12/2003	Milliman et al.	6,929,641	B2	8/2005	Goble et al.
6,671,185	B2	12/2003	Duval	6,931,830	B2	8/2005	Liao
D484,977	S	1/2004	Ryan et al.	6,936,042	B2	8/2005	Wallace et al.
6,676,660	B2	1/2004	Wampler et al.	6,939,358	B2	9/2005	Palacios et al.
6,679,410	B2	1/2004	Würsch et al.	6,942,662	B2	9/2005	Goble et al.
6,681,978	B2	1/2004	Geiste et al.	6,945,444	B2	9/2005	Gresham et al.
6,681,979	B2	1/2004	Whitman	6,953,138	B1	10/2005	Dworak et al.
6,682,527	B2	1/2004	Strul	6,953,139	B2	10/2005	Milliman et al.
6,682,528	B2	1/2004	Frazier et al.	6,959,851	B2	11/2005	Heinrich
6,685,727	B2	2/2004	Fisher et al.	6,959,852	B2	11/2005	Shelton, IV et al.
6,692,507	B2	2/2004	Pugsley et al.	6,960,163	B2	11/2005	Ewers et al.
6,695,199	B2	2/2004	Whitman	6,960,220	B2	11/2005	Marino et al.
6,698,643	B2	3/2004	Whitman	6,964,363	B2	11/2005	Wales et al.
6,699,235	B2	3/2004	Wallace et al.	6,966,907	B2	11/2005	Goble
6,704,210	B1	3/2004	Myers	6,966,909	B2	11/2005	Marshall et al.
6,705,503	B1	3/2004	Pedicini et al.	6,972,199	B2 *	12/2005	Lebouitz et al. 438/5
6,716,223	B2	4/2004	Leopold et al.	6,974,462	B2	12/2005	Sater
6,716,232	B1	4/2004	Vidal et al.	6,978,921	B2	12/2005	Shelton, IV et al.
6,716,233	B1	4/2004	Whitman	6,978,922	B2	12/2005	Bilotti et al.
6,722,552	B2	4/2004	Fenton, Jr.	6,981,628	B2	1/2006	Wales
6,723,087	B2	4/2004	O'Neill et al.	6,981,941	B2	1/2006	Whitman et al.
6,723,091	B2	4/2004	Goble et al.	6,981,978	B2	1/2006	Gannoe
6,726,697	B2	4/2004	Nicholas et al.	6,984,203	B2	1/2006	Tartaglia et al.
6,740,030	B2	5/2004	Martone et al.	6,984,231	B2	1/2006	Goble et al.
6,747,121	B2	6/2004	Gogolewski	6,986,451	B1	1/2006	Mastri et al.
6,749,560	B1	6/2004	Konstorum et al.	6,988,649	B2	1/2006	Shelton, IV et al.
6,752,768	B2	6/2004	Burdorff et al.	6,988,650	B2	1/2006	Schwemberger et al.
6,752,816	B2	6/2004	Culp et al.	6,990,796	B2	1/2006	Schnipke et al.
6,755,195	B1	6/2004	Lemke et al.	6,994,708	B2	2/2006	Manzo
6,755,338	B2	6/2004	Hahnen et al.	6,997,931	B2	2/2006	Sauer et al.
6,758,846	B2	7/2004	Goble et al.	7,000,818	B2	2/2006	Shelton, IV et al.
6,761,685	B2	7/2004	Adams et al.	7,000,819	B2	2/2006	Swayze et al.
6,767,352	B2	7/2004	Field et al.	7,001,380	B2	2/2006	Goble
6,767,356	B2	7/2004	Kanner et al.	7,001,408	B2	2/2006	Knodel et al.
6,769,594	B2	8/2004	Orban, III	7,008,435	B2	3/2006	Cummins
6,773,438	B1	8/2004	Knodel et al.	7,018,390	B2	3/2006	Turovskiy et al.
6,780,151	B2	8/2004	Grabover et al.	7,025,743	B2	4/2006	Mann et al.
6,780,180	B1	8/2004	Goble et al.	7,029,435	B2	4/2006	Nakao
6,783,524	B2	8/2004	Anderson et al.	7,032,798	B2	4/2006	Whitman et al.
6,786,382	B1	9/2004	Hoffman	7,032,799	B2	4/2006	Viola et al.
6,786,864	B2	9/2004	Matsuura et al.	7,033,356	B2	4/2006	Latterell et al.
6,786,896	B1	9/2004	Madhani et al.	7,036,680	B1	5/2006	Flannery
6,790,173	B2	9/2004	Saadat et al.	7,037,344	B2	5/2006	Kagan et al.
6,793,652	B1	9/2004	Whitman et al.	7,044,352	B2	5/2006	Shelton, IV et al.
6,805,273	B2	10/2004	Bilotti et al.	7,044,353	B2	5/2006	Mastri et al.
6,806,808	B1	10/2004	Watters et al.	7,048,687	B1	5/2006	Reuss et al.
6,808,525	B2	10/2004	Latterell et al.	7,052,494	B2	5/2006	Goble et al.
6,814,741	B2	11/2004	Bowman et al.	7,055,730	B2	6/2006	Ehrenfels et al.
6,817,508	B1	11/2004	Racenet et al.	7,055,731	B2	6/2006	Shelton, IV et al.
6,817,509	B2	11/2004	Geiste et al.	7,056,284	B2	6/2006	Martone et al.
6,817,974	B2	11/2004	Cooper et al.	7,056,330	B2	6/2006	Gayton
6,821,273	B2	11/2004	Mollenauer	7,059,508	B2	6/2006	Shelton, IV et al.
6,821,284	B2	11/2004	Sturtz et al.	7,063,712	B2	6/2006	Vargas et al.
6,827,725	B2	12/2004	Batchelor et al.	7,066,879	B2	6/2006	Fowler et al.
6,828,902	B2	12/2004	Casden	7,066,944	B2	6/2006	Laufer et al.
6,830,174	B2	12/2004	Hillstead et al.	7,070,083	B2	7/2006	Jankowski
6,832,998	B2	12/2004	Goble	7,070,559	B2	7/2006	Adams et al.
6,834,001	B2	12/2004	Myono	7,071,287	B2	7/2006	Rhine et al.
6,835,199	B2	12/2004	McGuckin, Jr. et al.	7,075,770	B1	7/2006	Smith
6,843,403	B2	1/2005	Whitman	7,077,856	B2	7/2006	Whitman
6,843,789	B2	1/2005	Goble	7,080,769	B2	7/2006	Vresh et al.
6,846,307	B2	1/2005	Whitman et al.	7,081,114	B2	7/2006	Rashidi
6,846,308	B2	1/2005	Whitman et al.	7,083,073	B2	8/2006	Yoshie et al.
6,846,309	B2	1/2005	Whitman et al.	7,083,075	B2	8/2006	Swayze et al.
6,849,071	B2	2/2005	Whitman et al.	7,083,571	B2	8/2006	Wang et al.
RE38,708	E	3/2005	Bolanos et al.	7,083,615	B2	8/2006	Peterson et al.
6,866,178	B2	3/2005	Adams et al.	7,087,071	B2	8/2006	Nicholas et al.
6,866,671	B2	3/2005	Tierney et al.	7,090,637	B2	8/2006	Danitz et al.
6,872,214	B2	3/2005	Sonnenschein et al.	7,090,673	B2	8/2006	Dycus et al.
6,874,669	B2	4/2005	Adams et al.	7,090,684	B2	8/2006	McGuckin, Jr. et al.
6,877,647	B2	4/2005	Green et al.	7,094,202	B2	8/2006	Nobis et al.
6,878,106	B1	4/2005	Herrmann	7,097,089	B2	8/2006	Marczyk
6,889,116	B2	5/2005	Jinno	7,098,794	B2	8/2006	Lindsay et al.
6,893,435	B2	5/2005	Goble	7,104,741	B2	9/2006	Krohn
6,905,057	B2	6/2005	Swayze et al.	7,108,695	B2	9/2006	Witt et al.
6,905,497	B2	6/2005	Truckai et al.	7,108,701	B2	9/2006	Evens et al.
6,913,608	B2	7/2005	Liddicoat et al.	7,108,709	B2	9/2006	Cummins

7,111,769 B2	9/2006	Wales et al.	7,328,828 B2	2/2008	Ortiz et al.
7,112,214 B2	9/2006	Peterson et al.	7,328,829 B2	2/2008	Arad et al.
RE39,358 E	10/2006	Goble	7,330,004 B2	2/2008	DeJonge et al.
7,114,642 B2	10/2006	Whitman	7,334,717 B2	2/2008	Rethy et al.
7,118,582 B1	10/2006	Wang et al.	7,336,184 B2	2/2008	Smith et al.
7,121,446 B2	10/2006	Arad et al.	7,338,513 B2	3/2008	Lee et al.
7,122,028 B2	10/2006	Looper et al.	7,343,920 B2	3/2008	Toby et al.
7,128,253 B2	10/2006	Mastri et al.	7,348,763 B1	3/2008	Reinhart et al.
7,128,254 B2	10/2006	Shelton, IV et al.	7,351,258 B2	4/2008	Ricotta et al.
7,128,748 B2	10/2006	Mooradian et al.	7,354,447 B2	4/2008	Shelton, IV et al.
7,131,445 B2	11/2006	Amoah	7,357,287 B2	4/2008	Shelton, IV et al.
7,133,601 B2	11/2006	Phillips et al.	7,364,060 B2	4/2008	Milliman
7,140,527 B2	11/2006	Ehrenfels et al.	7,364,061 B2	4/2008	Swayze et al.
7,140,528 B2	11/2006	Shelton, IV	7,377,928 B2	5/2008	Zubik et al.
7,143,923 B2	12/2006	Shelton, IV et al.	7,380,695 B2	6/2008	Doll et al.
7,143,924 B2	12/2006	Scirica et al.	7,380,696 B2	6/2008	Shelton, IV et al.
7,143,925 B2	12/2006	Shelton, IV et al.	7,388,217 B2	6/2008	Buschbeck et al.
7,143,926 B2	12/2006	Shelton, IV et al.	7,396,356 B2	7/2008	Mollenauer
7,147,138 B2	12/2006	Shelton, IV	7,398,907 B2	7/2008	Racenet et al.
7,147,139 B2	12/2006	Schwemberger et al.	7,398,908 B2	7/2008	Holsten et al.
7,147,637 B2	12/2006	Goble	7,404,508 B2	7/2008	Smith et al.
7,147,650 B2	12/2006	Lee	7,404,509 B2	7/2008	Ortiz et al.
7,150,748 B2	12/2006	Ebbutt et al.	7,407,075 B2	8/2008	Holsten et al.
7,153,300 B2	12/2006	Goble	7,407,078 B2	8/2008	Shelton, IV et al.
7,156,863 B2 *	1/2007	Sonnenschein et al. 606/219	7,410,086 B2	8/2008	Ortiz et al.
7,159,750 B2	1/2007	Racenet et al.	7,416,101 B2	8/2008	Shelton, IV et al.
7,160,299 B2	1/2007	Baily	7,418,078 B2	8/2008	Blanz et al.
7,161,036 B2	1/2007	Oikawa et al.	7,419,080 B2	9/2008	Smith et al.
7,168,604 B2	1/2007	Milliman et al.	7,422,136 B1	9/2008	Marczyk
7,172,104 B2	2/2007	Scirica et al.	7,422,139 B2	9/2008	Shelton, IV et al.
7,179,223 B2	2/2007	Motoki et al.	7,424,965 B2	9/2008	Racenet et al.
7,179,267 B2	2/2007	Nolan et al.	7,431,188 B1	10/2008	Marczyk
7,182,239 B1	2/2007	Myers	7,431,189 B2	10/2008	Shelton, IV et al.
7,188,758 B2	3/2007	Viola et al.	7,431,694 B2	10/2008	Stefanchik et al.
7,195,627 B2	3/2007	Amoah et al.	7,431,730 B2	10/2008	Viola
7,204,835 B2	4/2007	Latterell et al.	7,434,715 B2	10/2008	Shelton, IV et al.
7,207,233 B2	4/2007	Wadge	7,434,717 B2	10/2008	Shelton, IV et al.
7,207,471 B2	4/2007	Heinrich et al.	7,438,209 B1	10/2008	Hess et al.
7,207,472 B2	4/2007	Wukusick et al.	7,439,354 B2	10/2008	Lenges et al.
7,208,005 B2	4/2007	Freckler et al.	7,441,684 B2	10/2008	Shelton, IV et al.
7,210,609 B2	5/2007	Leiboff et al.	7,441,685 B1	10/2008	Boudreaux
7,211,081 B2	5/2007	Goble	7,442,201 B2	10/2008	Pugsley et al.
7,211,084 B2	5/2007	Goble et al.	7,448,525 B2	11/2008	Shelton, IV et al.
7,213,736 B2	5/2007	Wales et al.	7,455,208 B2	11/2008	Wales et al.
7,214,224 B2	5/2007	Goble	7,461,767 B2	12/2008	Viola et al.
7,217,285 B2	5/2007	Vargas et al.	7,464,846 B2	12/2008	Shelton, IV et al.
7,220,260 B2	5/2007	Fleming et al.	7,464,847 B2	12/2008	Viola et al.
7,220,272 B2	5/2007	Weadock	7,464,849 B2	12/2008	Shelton, IV et al.
7,225,963 B2	6/2007	Scirica	7,467,740 B2	12/2008	Shelton, IV et al.
7,225,964 B2	6/2007	Mastri et al.	7,467,849 B2	12/2008	Silverbrook et al.
7,234,624 B2	6/2007	Gresham et al.	7,472,814 B2	1/2009	Mastri et al.
7,235,089 B1	6/2007	McGuckin, Jr.	7,472,815 B2	1/2009	Shelton, IV et al.
7,235,302 B2	6/2007	Jing et al.	7,473,253 B2	1/2009	Dycus et al.
7,237,708 B1	7/2007	Guy et al.	7,479,608 B2	1/2009	Smith
7,238,195 B2	7/2007	Viola	7,481,347 B2	1/2009	Roy
7,241,288 B2	7/2007	Braun	7,481,349 B2	1/2009	Holsten et al.
7,246,734 B2	7/2007	Shelton, IV	7,481,824 B2	1/2009	Boudreaux et al.
7,247,161 B2	7/2007	Johnston et al.	7,485,133 B2	2/2009	Cannon et al.
7,252,660 B2	8/2007	Kunz	7,490,749 B2	2/2009	Schall et al.
7,255,696 B2	8/2007	Goble et al.	7,494,039 B2	2/2009	Racenet et al.
7,258,262 B2	8/2007	Mastri et al.	7,494,499 B2	2/2009	Nagase et al.
7,260,431 B2	8/2007	Libbus et al.	7,500,979 B2	3/2009	Hueil et al.
7,265,374 B2	9/2007	Lee et al.	7,501,198 B2	3/2009	Barlev et al.
7,267,679 B2	9/2007	McGuckin, Jr. et al.	7,506,790 B2	3/2009	Shelton, IV
7,273,483 B2	9/2007	Wiener et al.	7,506,791 B2	3/2009	Omaitis et al.
7,278,562 B2	10/2007	Mastri et al.	7,510,107 B2	3/2009	Timm et al.
7,278,563 B1	10/2007	Green	7,524,320 B2	4/2009	Tierney et al.
7,278,994 B2	10/2007	Goble	7,530,985 B2	5/2009	Takemoto et al.
7,282,048 B2	10/2007	Goble et al.	7,546,940 B2	6/2009	Milliman et al.
7,295,907 B2	11/2007	Lu et al.	7,547,312 B2	6/2009	Bauman et al.
7,296,724 B2	11/2007	Green et al.	7,549,563 B2	6/2009	Mather et al.
7,297,149 B2	11/2007	Vitali et al.	7,549,564 B2	6/2009	Boudreaux
7,300,450 B2	11/2007	Vleugels et al.	7,552,854 B2	6/2009	Wixey et al.
7,303,106 B2	12/2007	Milliman et al.	7,556,185 B2	7/2009	Viola
7,303,107 B2	12/2007	Milliman et al.	7,556,186 B2	7/2009	Milliman
7,303,108 B2	12/2007	Shelton, IV	7,559,450 B2	7/2009	Wales et al.
7,303,556 B2	12/2007	Metzger	7,559,452 B2	7/2009	Wales et al.
7,308,998 B2	12/2007	Mastri et al.	7,563,862 B2	7/2009	Sieg et al.
7,324,572 B2	1/2008	Chang	7,566,300 B2	7/2009	Devierre et al.

7,568,603 B2	8/2009	Shelton, IV et al.	7,963,963 B2	6/2011	Francischelli et al.
7,568,604 B2	8/2009	Ehrenfels et al.	7,967,180 B2	6/2011	Scirica
7,575,144 B2	8/2009	Ortiz et al.	7,972,298 B2	7/2011	Wallace et al.
7,588,175 B2	9/2009	Timm et al.	8,002,795 B2	8/2011	Beetel
7,588,176 B2	9/2009	Timm et al.	8,011,551 B2	9/2011	Marczyk et al.
7,597,229 B2	10/2009	Boudreaux et al.	8,011,555 B2	9/2011	Tarinelli et al.
7,600,663 B2	10/2009	Green	8,028,883 B2	10/2011	Stopek
7,604,150 B2	10/2009	Boudreaux	8,034,077 B2	10/2011	Smith et al.
7,604,151 B2	10/2009	Hess et al.	8,038,045 B2	10/2011	Bettuchi et al.
7,607,557 B2	10/2009	Shelton, IV et al.	8,038,046 B2	10/2011	Smith et al.
7,611,038 B2	11/2009	Racenet et al.	8,062,330 B2	11/2011	Prommersberger et al.
7,615,003 B2	11/2009	Stefanchik et al.	D650,074 S	12/2011	Hunt et al.
7,624,902 B2	12/2009	Marczyk et al.	8,091,756 B2	1/2012	Viola
7,631,793 B2	12/2009	Rethy et al.	8,097,017 B2	1/2012	Viola
7,637,409 B2	12/2009	Marczyk	8,108,072 B2	1/2012	Zhao et al.
7,641,092 B2	1/2010	Kruszynski et al.	8,123,103 B2	2/2012	Milliman
7,641,093 B2	1/2010	Doll et al.	8,152,041 B2	4/2012	Kostrzewski
7,644,848 B2	1/2010	Swayze et al.	8,157,152 B2	4/2012	Holsten et al.
7,651,498 B2	1/2010	Shifrin et al.	8,167,895 B2	5/2012	D'Agostino et al.
7,656,131 B2	2/2010	Embrey et al.	8,211,125 B2	7/2012	Spivey
7,658,312 B2	2/2010	Vidal et al.	8,220,468 B2	7/2012	Cooper et al.
7,665,646 B2	2/2010	Prommersberger	8,225,799 B2	7/2012	Bettuchi
7,674,255 B2	3/2010	Braun	8,241,271 B2	8/2012	Millman et al.
7,682,307 B2	3/2010	Danitz et al.	8,245,898 B2	8/2012	Smith et al.
7,686,826 B2	3/2010	Lee et al.	8,245,901 B2	8/2012	Stopek
7,691,098 B2	4/2010	Wallace et al.	8,256,654 B2	9/2012	Bettuchi et al.
7,699,204 B2	4/2010	Viola	8,257,391 B2	9/2012	Orban, III et al.
7,699,859 B2	4/2010	Bombard et al.	2002/0022836 A1	2/2002	Goble et al.
7,708,180 B2	5/2010	Murray et al.	2002/0029036 A1	3/2002	Goble et al.
7,708,758 B2	5/2010	Lee et al.	2002/0117534 A1	8/2002	Green et al.
7,714,239 B2	5/2010	Smith	2002/0134811 A1	9/2002	Napier et al.
7,721,930 B2	5/2010	McKenna et al.	2002/0165541 A1	11/2002	Whitman
7,722,610 B2	5/2010	Viola et al.	2003/0093103 A1	5/2003	Malackowski et al.
7,726,537 B2	6/2010	Olson et al.	2003/0105478 A1	6/2003	Whitman et al.
7,726,538 B2	6/2010	Holsten et al.	2003/0130677 A1	7/2003	Whitman et al.
7,743,960 B2	6/2010	Whitman et al.	2003/0139741 A1	7/2003	Goble et al.
7,744,627 B2	6/2010	Orban, III et al.	2003/0153908 A1	8/2003	Goble et al.
7,766,821 B2	8/2010	Brunnen et al.	2003/0195387 A1	10/2003	Kortenbach et al.
7,766,894 B2	8/2010	Weitzner et al.	2003/0205029 A1	11/2003	Chapolini et al.
7,771,396 B2	8/2010	Stefanchik et al.	2003/0216732 A1	11/2003	Truckai et al.
7,772,720 B2	8/2010	McGee et al.	2003/0220660 A1	11/2003	Kortenbach et al.
7,776,060 B2	8/2010	Mooradian et al.	2004/0002726 A1	1/2004	Nunez et al.
7,780,054 B2	8/2010	Wales	2004/0006335 A1	1/2004	Garrison
7,780,055 B2	8/2010	Scirica et al.	2004/0006340 A1	1/2004	Latterell et al.
7,780,663 B2	8/2010	Yates et al.	2004/0006372 A1	1/2004	Racenet et al.
7,780,685 B2	8/2010	Hunt et al.	2004/0030333 A1	2/2004	Goble
7,784,662 B2	8/2010	Wales et al.	2004/0034357 A1	2/2004	Beane et al.
7,803,151 B2	9/2010	Whitman	2004/0034369 A1	2/2004	Sauer et al.
7,806,891 B2	10/2010	Nowlin et al.	2004/0044364 A1	3/2004	DeVries et al.
7,815,565 B2	10/2010	Stefanchik et al.	2004/0068161 A1	4/2004	Couvillon, Jr.
7,824,401 B2	11/2010	Manzo et al.	2004/0068307 A1	4/2004	Goble
7,828,794 B2	11/2010	Sartor	2004/0078037 A1	4/2004	Batchelor et al.
7,828,808 B2	11/2010	Hinman et al.	2004/0093024 A1	5/2004	Lousararian et al.
7,832,611 B2	11/2010	Boyden et al.	2004/0094597 A1	5/2004	Whitman et al.
7,836,400 B2	11/2010	May et al.	2004/0097987 A1	5/2004	Pugsley et al.
7,837,081 B2	11/2010	Holsten et al.	2004/0101822 A1	5/2004	Weisner et al.
7,845,533 B2	12/2010	Marczyk et al.	2004/0108357 A1	6/2004	Milliman et al.
7,845,534 B2	12/2010	Viola et al.	2004/0111081 A1	6/2004	Whitman et al.
7,846,149 B2	12/2010	Jankowski	2004/0115022 A1	6/2004	Albertson et al.
7,870,989 B2	1/2011	Viola et al.	2004/0116952 A1	6/2004	Sakurai et al.
7,887,530 B2	2/2011	Zemlok et al.	2004/0147909 A1	7/2004	Johnston et al.
7,905,380 B2	3/2011	Shelton, IV et al.	2004/0164123 A1	8/2004	Racenet et al.
7,905,381 B2	3/2011	Baxter, III et al.	2004/0167572 A1	8/2004	Roth et al.
7,909,191 B2	3/2011	Baker et al.	2004/0173659 A1	9/2004	Green et al.
7,909,221 B2	3/2011	Viola et al.	2004/0181219 A1	9/2004	Goble et al.
7,913,891 B2	3/2011	Doll et al.	2004/0186470 A1	9/2004	Goble et al.
7,914,543 B2	3/2011	Roth et al.	2004/0193189 A1	9/2004	Kortenbach et al.
7,918,377 B2	4/2011	Measamer et al.	2004/0222268 A1	11/2004	Bilotti et al.
7,922,061 B2	4/2011	Shelton, IV et al.	2004/0230214 A1	11/2004	Donofrio et al.
7,922,063 B2	4/2011	Zemlok et al.	2004/0232201 A1	11/2004	Wenchell et al.
7,934,630 B2	5/2011	Shelton, IV et al.	2004/0243151 A1	12/2004	Demmy et al.
7,938,307 B2	5/2011	Bettuchi	2004/0243163 A1	12/2004	Casiano et al.
7,942,303 B2	5/2011	Shah	2004/0243176 A1	12/2004	Hahnen et al.
7,942,890 B2	5/2011	D'Agostino et al.	2004/0254566 A1	12/2004	Plicchi et al.
7,950,560 B2	5/2011	Zemlok et al.	2004/0254608 A1	12/2004	Huitema et al.
7,954,682 B2	6/2011	Giordano et al.	2004/0267310 A1	12/2004	Racenet et al.
7,954,684 B2	6/2011	Boudreaux	2005/0032511 A1	2/2005	Malone et al.
7,954,686 B2	6/2011	Baxter, III et al.	2005/0033357 A1	2/2005	Braun
7,959,050 B2	6/2011	Smith et al.	2005/0054946 A1	3/2005	Krzyzanowski

US 8,459,520 B2

Page 10

2005/0059997 A1	3/2005	Bauman et al.	2006/0161185 A1	7/2006	Saadat et al.
2005/0070929 A1	3/2005	Dallessandro et al.	2006/0173470 A1	8/2006	Oray et al.
2005/0080454 A1	4/2005	Drews et al.	2006/0180634 A1	8/2006	Shelton, IV et al.
2005/0085693 A1	4/2005	Belson et al.	2006/0183246 A1	8/2006	Wiesner et al.
2005/0090817 A1	4/2005	Phan	2006/0200123 A1	9/2006	Ryan
2005/0099290 A1 *	5/2005	Govari 340/539.13	2006/0212069 A1	9/2006	Shelton, IV
2005/0103819 A1	5/2005	Racenet et al.	2006/0217729 A1	9/2006	Eskridge et al.
2005/0107814 A1	5/2005	Johnston et al.	2006/0226196 A1	10/2006	Hueil et al.
2005/0107824 A1	5/2005	Hillstead et al.	2006/0235469 A1	10/2006	Viola
2005/0113820 A1	5/2005	Goble et al.	2006/0241655 A1	10/2006	Viola
2005/0119525 A1	6/2005	Takemoto	2006/0241692 A1	10/2006	McGuckin, Jr. et al.
2005/0119669 A1	6/2005	Demmy	2006/0244460 A1	11/2006	Weaver
2005/0124855 A1	6/2005	Jaffe et al.	2006/0245971 A1	11/2006	Burns et al.
2005/0125009 A1	6/2005	Perry et al.	2006/0258904 A1	11/2006	Stefanchik et al.
2005/0131173 A1	6/2005	McDaniel et al.	2006/0259073 A1	11/2006	Miyamoto et al.
2005/0131211 A1	6/2005	Bayley et al.	2006/0264927 A1	11/2006	Ryan
2005/0131390 A1	6/2005	Heinrich et al.	2006/0264929 A1	11/2006	Goble et al.
2005/0131436 A1	6/2005	Johnston et al.	2006/0271042 A1	11/2006	Latterell et al.
2005/0131437 A1	6/2005	Johnston et al.	2006/0271102 A1	11/2006	Bosshard et al.
2005/0131457 A1	6/2005	Douglas et al.	2006/0273135 A1	12/2006	Beetel
2005/0137454 A1	6/2005	Saadat et al.	2006/0278680 A1	12/2006	Viola et al.
2005/0137455 A1	6/2005	Ewers et al.	2006/0278681 A1	12/2006	Viola et al.
2005/0143759 A1	6/2005	Kelly	2006/0289602 A1	12/2006	Wales et al.
2005/0145675 A1	7/2005	Hartwick et al.	2006/0291981 A1	12/2006	Viola et al.
2005/0154258 A1	7/2005	Tartaglia et al.	2007/0023476 A1	2/2007	Whitman et al.
2005/0165419 A1	7/2005	Sauer et al.	2007/0023477 A1	2/2007	Whitman et al.
2005/0165435 A1	7/2005	Johnston et al.	2007/0027468 A1	2/2007	Wales et al.
2005/0169974 A1	8/2005	Tenerz et al.	2007/0027469 A1	2/2007	Smith et al.
2005/0171522 A1	8/2005	Christopherson	2007/0034668 A1	2/2007	Holsten et al.
2005/0177181 A1	8/2005	Kagan et al.	2007/0045379 A1	3/2007	Shelton, IV
2005/0182298 A1	8/2005	Ikeda et al.	2007/0055219 A1	3/2007	Whitman et al.
2005/0184121 A1	8/2005	Heinrich	2007/0070574 A1	3/2007	Nerheim et al.
2005/0187545 A1	8/2005	Hooven et al.	2007/0073341 A1	3/2007	Smith
2005/0187572 A1	8/2005	Johnston et al.	2007/0078484 A1	4/2007	Talarico et al.
2005/0187576 A1	8/2005	Whitman et al.	2007/0083193 A1	4/2007	Werneth et al.
2005/0189397 A1	9/2005	Jankowski	2007/0084897 A1	4/2007	Shelton, IV et al.
2005/0192609 A1	9/2005	Whitman et al.	2007/0102453 A1	5/2007	Morgan et al.
2005/0192628 A1	9/2005	Viola	2007/0102472 A1	5/2007	Shelton, IV
2005/0203550 A1	9/2005	Laufer et al.	2007/0102473 A1	5/2007	Shelton, IV et al.
2005/0216055 A1	9/2005	Scirica et al.	2007/0102474 A1	5/2007	Shelton, IV et al.
2005/0228224 A1	10/2005	Okada et al.	2007/0106113 A1	5/2007	Ravo
2005/0240222 A1	10/2005	Shipp	2007/0106317 A1	5/2007	Shelton, IV et al.
2005/0245965 A1	11/2005	Orban, III et al.	2007/0114261 A1	5/2007	Ortiz et al.
2005/0251128 A1	11/2005	Amoah	2007/0118175 A1	5/2007	Butler et al.
2005/0256522 A1	11/2005	Francischelli et al.	2007/0129605 A1	6/2007	Schaaf
2005/0261676 A1	11/2005	Hall et al.	2007/0135803 A1	6/2007	Belson
2005/0261677 A1	11/2005	Hall et al.	2007/0158358 A1	7/2007	Mason, II et al.
2005/0263563 A1	12/2005	Racenet et al.	2007/0158385 A1	7/2007	Hueil et al.
2005/0267455 A1	12/2005	Eggers et al.	2007/0170225 A1	7/2007	Shelton, IV et al.
2005/0274768 A1	12/2005	Cummins et al.	2007/0173806 A1 *	7/2007	Orszulak et al. 606/34
2006/0004407 A1	1/2006	Hiles et al.	2007/0173813 A1 *	7/2007	Odom 606/51
2006/0008787 A1	1/2006	Hayman et al.	2007/0175949 A1	8/2007	Shelton, IV et al.
2006/0011699 A1	1/2006	Olson et al.	2007/0175950 A1	8/2007	Shelton, IV et al.
2006/0015009 A1	1/2006	Jaffe et al.	2007/0175951 A1	8/2007	Shelton, IV et al.
2006/0020247 A1	1/2006	Kagan et al.	2007/0175953 A1	8/2007	Shelton, IV et al.
2006/0020336 A1	1/2006	Liddicoat	2007/0175955 A1	8/2007	Shelton, IV et al.
2006/0025811 A1	2/2006	Shelton, IV	2007/0175957 A1	8/2007	Shelton, IV et al.
2006/0025812 A1	2/2006	Shelton, IV	2007/0175958 A1	8/2007	Shelton, IV et al.
2006/0025813 A1	2/2006	Shelton et al.	2007/0175964 A1	8/2007	Shelton, IV et al.
2006/0047275 A1	3/2006	Goble	2007/0179476 A1	8/2007	Shelton, IV et al.
2006/0047303 A1	3/2006	Ortiz et al.	2007/0181632 A1	8/2007	Milliman
2006/0047307 A1	3/2006	Ortiz et al.	2007/0194079 A1	8/2007	Hueil et al.
2006/0049229 A1	3/2006	Milliman et al.	2007/0194080 A1	8/2007	Swayze et al.
2006/0052825 A1	3/2006	Ransick et al.	2007/0194081 A1	8/2007	Hueil et al.
2006/0060630 A1	3/2006	Shelton, IV et al.	2007/0194082 A1	8/2007	Morgan et al.
2006/0064086 A1	3/2006	Odom	2007/0203510 A1	8/2007	Bettuchi
2006/0079735 A1	4/2006	Martone et al.	2007/0213750 A1	9/2007	Weadock
2006/0085031 A1	4/2006	Bettuchi	2007/0221700 A1	9/2007	Ortiz et al.
2006/0085033 A1	4/2006	Criscuolo et al.	2007/0221701 A1	9/2007	Ortiz et al.
2006/0086032 A1	4/2006	Valencic et al.	2007/0225562 A1	9/2007	Spivey et al.
2006/0100643 A1	5/2006	Laufer et al.	2007/0233053 A1	10/2007	Shelton, IV et al.
2006/0108393 A1	5/2006	Heinrich et al.	2007/0239028 A1	10/2007	Houser et al.
2006/0111710 A1	5/2006	Goble et al.	2007/0246505 A1	10/2007	Pace-Florida et al.
2006/0111711 A1	5/2006	Goble	2007/0260278 A1	11/2007	Wheeler et al.
2006/0111723 A1	5/2006	Chapolini et al.	2007/0270784 A1	11/2007	Smith et al.
2006/0122636 A1	6/2006	Bailly et al.	2007/0270884 A1	11/2007	Smith et al.
2006/0129140 A1 *	6/2006	Todd et al. 606/1	2007/0288044 A1	12/2007	Jinno et al.
2006/0142772 A1	6/2006	Ralph et al.	2007/0295780 A1	12/2007	Shelton et al.
2006/0149163 A1	7/2006	Hibner et al.	2007/0299427 A1	12/2007	Yeung et al.

2008/0015598 A1	1/2008	Prommersberger	2009/0005808 A1	1/2009	Hess et al.
2008/0029570 A1	2/2008	Shelton et al.	2009/0005809 A1	1/2009	Hess et al.
2008/0029573 A1	2/2008	Shelton et al.	2009/0012534 A1	1/2009	Madhani et al.
2008/0029574 A1	2/2008	Shelton et al.	2009/0012556 A1	1/2009	Boudreaux et al.
2008/0029575 A1	2/2008	Shelton et al.	2009/0020958 A1	1/2009	Soul
2008/0029576 A1	2/2008	Shelton et al.	2009/0054908 A1 *	2/2009	Zand et al. 606/130
2008/0030170 A1	2/2008	Dacquay et al.	2009/0057369 A1	3/2009	Smith et al.
2008/0035701 A1	2/2008	Racenet et al.	2009/0076534 A1	3/2009	Shelton, IV et al.
2008/0041916 A1	2/2008	Milliman et al.	2009/0090763 A1	4/2009	Zemlok et al.
2008/0041917 A1	2/2008	Racenet et al.	2009/0093728 A1	4/2009	Hyde et al.
2008/0078800 A1	4/2008	Hess et al.	2009/0108048 A1	4/2009	Zemlok et al.
2008/0078801 A1	4/2008	Shelton et al.	2009/0114701 A1	5/2009	Zemlok et al.
2008/0078802 A1	4/2008	Hess et al.	2009/0143805 A1	6/2009	Palmer et al.
2008/0078803 A1	4/2008	Shelton et al.	2009/0149871 A9	6/2009	Kagan et al.
2008/0078804 A1	4/2008	Shelton et al.	2009/0157067 A1 *	6/2009	Kane et al. 606/33
2008/0078806 A1	4/2008	Omairs et al.	2009/0200355 A1	8/2009	Baxter, III et al.
2008/0078807 A1	4/2008	Hess et al.	2009/0206123 A1	8/2009	Doll et al.
2008/0078808 A1	4/2008	Hess et al.	2009/0206124 A1	8/2009	Hall et al.
2008/0082114 A1	4/2008	McKenna et al.	2009/0206125 A1	8/2009	Huitema et al.
2008/0082115 A1	4/2008	Morgan et al.	2009/0206126 A1	8/2009	Huitema et al.
2008/0082124 A1	4/2008	Hess et al.	2009/0206128 A1	8/2009	Hueil et al.
2008/0082125 A1	4/2008	Murray et al.	2009/0206129 A1	8/2009	Doll et al.
2008/0082126 A1	4/2008	Murray et al.	2009/0206130 A1	8/2009	Hall et al.
2008/0083813 A1	4/2008	Zemlok et al.	2009/0206131 A1	8/2009	Weisenburgh, II et al.
2008/0114385 A1	5/2008	Byrum et al.	2009/0206132 A1	8/2009	Hueil et al.
2008/0129253 A1	6/2008	Shiue et al.	2009/0206133 A1	8/2009	Morgan et al.
2008/0140115 A1	6/2008	Stopek	2009/0206134 A1	8/2009	Swayze et al.
2008/0164296 A1	7/2008	Shelton et al.	2009/0206135 A1	8/2009	Hall et al.
2008/0167522 A1	7/2008	Giordano et al.	2009/0206136 A1	8/2009	Moore et al.
2008/0167644 A1	7/2008	Shelton et al.	2009/0206137 A1	8/2009	Hall et al.
2008/0167670 A1	7/2008	Shelton et al.	2009/0206138 A1	8/2009	Smith et al.
2008/0167671 A1	7/2008	Giordano et al.	2009/0206139 A1	8/2009	Hall et al.
2008/0167672 A1	7/2008	Giordano et al.	2009/0206140 A1	8/2009	Scheib et al.
2008/0167736 A1	7/2008	Swayze et al.	2009/0206141 A1	8/2009	Huitema et al.
2008/0169328 A1	7/2008	Shelton	2009/0206142 A1	8/2009	Huitema et al.
2008/0169329 A1	7/2008	Shelton et al.	2009/0206143 A1	8/2009	Huitema et al.
2008/0169330 A1	7/2008	Shelton et al.	2009/0206144 A1	8/2009	Doll et al.
2008/0169331 A1	7/2008	Shelton et al.	2009/0209946 A1	8/2009	Swayze et al.
2008/0169332 A1	7/2008	Shelton et al.	2009/0209979 A1	8/2009	Yates et al.
2008/0169333 A1	7/2008	Shelton et al.	2009/0209990 A1	8/2009	Yates et al.
2008/0172087 A1	7/2008	Fuchs et al.	2009/0213685 A1	8/2009	Mak et al.
2008/0172088 A1	7/2008	Smith et al.	2009/0218384 A1	9/2009	Aranyi
2008/0185419 A1	8/2008	Smith et al.	2009/0242610 A1	10/2009	Shelton, IV et al.
2008/0197167 A1	8/2008	Viola et al.	2009/0255974 A1	10/2009	Viola
2008/0200835 A1	8/2008	Monson et al.	2009/0255975 A1	10/2009	Zemlok et al.
2008/0210738 A1	9/2008	Shelton et al.	2009/0255976 A1	10/2009	Marczyk et al.
2008/0228029 A1	9/2008	Mikkaichi et al.	2009/0255977 A1	10/2009	Zemlok
2008/0237296 A1	10/2008	Boudreaux et al.	2009/0255978 A1	10/2009	Viola et al.
2008/0245841 A1	10/2008	Smith et al.	2009/0289096 A1	11/2009	Shelton, IV et al.
2008/0251568 A1	10/2008	Zemlok et al.	2009/0292283 A1 *	11/2009	Odom 606/51
2008/0251569 A1	10/2008	Smith et al.	2009/0308907 A1	12/2009	Nalagatla et al.
2008/0255413 A1	10/2008	Zemlok et al.	2010/0001036 A1	1/2010	Marczyk et al.
2008/0262654 A1	10/2008	Omori et al.	2010/0012704 A1	1/2010	Tarinelli Racenet et al.
2008/0283570 A1	11/2008	Boyden et al.	2010/0023024 A1	1/2010	Zeiner et al.
2008/0287944 A1	11/2008	Pearson et al.	2010/0032470 A1	2/2010	Hess et al.
2008/0290134 A1	11/2008	Bettuchi et al.	2010/0049084 A1	2/2010	Nock et al.
2008/0296343 A1	12/2008	Schall et al.	2010/0065605 A1	3/2010	Shelton, IV et al.
2008/0296345 A1	12/2008	Shelton, IV et al.	2010/0065609 A1	3/2010	Schwemberger
2008/0296346 A1	12/2008	Shelton, IV et al.	2010/0069942 A1	3/2010	Shelton, IV
2008/0296347 A1	12/2008	Shelton, IV et al.	2010/0072251 A1	3/2010	Baxter, III et al.
2008/0300579 A1	12/2008	Broehl et al.	2010/0072252 A1	3/2010	Baxter, III et al.
2008/0300580 A1	12/2008	Shelton, IV et al.	2010/0072253 A1	3/2010	Baxter, III et al.
2008/0300613 A1	12/2008	Shelton, IV et al.	2010/0072254 A1	3/2010	Aranyi et al.
2008/0308601 A1	12/2008	Timm et al.	2010/0072256 A1	3/2010	Baxter, III et al.
2008/0308602 A1	12/2008	Timm et al.	2010/0076474 A1	3/2010	Yates et al.
2008/0308603 A1	12/2008	Shelton, IV et al.	2010/0076475 A1	3/2010	Yates et al.
2008/0308608 A1	12/2008	Prommersberger	2010/0089970 A1	4/2010	Smith et al.
2008/0314954 A1	12/2008	Boudreaux	2010/0089972 A1	4/2010	Marczyk
2008/0314955 A1	12/2008	Boudreaux et al.	2010/0089974 A1	4/2010	Shelton, IV
2008/0314957 A1	12/2008	Boudreaux	2010/0096431 A1	4/2010	Smith et al.
2008/0314960 A1	12/2008	Marczyk et al.	2010/0096435 A1	4/2010	Fuchs et al.
2009/0001121 A1	1/2009	Hess et al.	2010/0108740 A1	5/2010	Pastorelli et al.
2009/0001122 A1	1/2009	Prommersberger et al.	2010/0108741 A1	5/2010	Hessler et al.
2009/0001123 A1	1/2009	Morgan et al.	2010/0127042 A1	5/2010	Shelton, IV
2009/0001124 A1	1/2009	Hess et al.	2010/0133317 A1	6/2010	Shelton, IV et al.
2009/0001125 A1	1/2009	Hess et al.	2010/0133318 A1	6/2010	Boudreaux
2009/0001128 A1	1/2009	Weisenburgh, II et al.	2010/0145146 A1	6/2010	Melder
2009/0001130 A1	1/2009	Hess et al.	2010/0163598 A1	7/2010	Belzer
2009/0005807 A1	1/2009	Hess et al.	2010/0179382 A1	7/2010	Shelton, IV et al.

2010/0181364	A1	7/2010	Shelton, IV et al.	2011/0233258	A1	9/2011	Boudreaux
2010/0186219	A1	7/2010	Smith	2011/0253766	A1	10/2011	Baxter, III et al.
2010/0193566	A1	8/2010	Schieb et al.	2011/0275901	A1	11/2011	Shelton, IV
2010/0193567	A1	8/2010	Scheib et al.	2011/0276083	A1	11/2011	Shelton, IV et al.
2010/0193568	A1	8/2010	Scheib et al.	2011/0288573	A1	11/2011	Yates et al.
2010/0193569	A1	8/2010	Yates et al.	2011/0290851	A1	12/2011	Shelton, IV
2010/0198220	A1	8/2010	Boudreaux et al.	2011/0290853	A1	12/2011	Shelton, IV et al.
2010/0200637	A1	8/2010	Beetel	2011/0290854	A1	12/2011	Timm et al.
2010/0213241	A1	8/2010	Bedi et al.	2011/0290855	A1	12/2011	Moore et al.
2010/0222901	A1	9/2010	Swayze et al.	2011/0290856	A1	12/2011	Shelton, IV et al.
2010/0224669	A1	9/2010	Shelton, IV et al.	2011/0290857	A1	12/2011	Shelton, IV et al.
2010/0230465	A1	9/2010	Smith et al.	2011/0295242	A1	12/2011	Spivey et al.
2010/0237132	A1	9/2010	Measamer et al.	2011/0295269	A1	12/2011	Swensgard et al.
2010/0243707	A1	9/2010	Olson et al.	2011/0295270	A1	12/2011	Giordano et al.
2010/0243708	A1	9/2010	Aranyi et al.	2011/0295295	A1	12/2011	Shelton, IV et al.
2010/0243709	A1	9/2010	Hess et al.	2012/0022523	A1	1/2012	Smith et al.
2010/0258611	A1	10/2010	Smith et al.	2012/0024934	A1	2/2012	Shelton, IV et al.
2010/0264193	A1	10/2010	Huang et al.	2012/0024935	A1	2/2012	Shelton, IV et al.
2010/0264194	A1	10/2010	Huang et al.	2012/0024936	A1	2/2012	Baxter, III et al.
2010/0276471	A1	11/2010	Whitman	2012/0029272	A1	2/2012	Shelton, IV et al.
2010/0294827	A1	11/2010	Boyden et al.	2012/0029544	A1	2/2012	Shelton, IV et al.
2010/0294829	A1	11/2010	Giordano et al.	2012/0029547	A1	2/2012	Shelton, IV et al.
2010/0301095	A1	12/2010	Shelton, IV et al.	2012/0046692	A1	2/2012	Smith et al.
2010/0301096	A1	12/2010	Moore et al.	2012/0061448	A1	3/2012	Zingman
2010/0305552	A1	12/2010	Shelton, IV et al.	2012/0071711	A1	3/2012	Shelton, IV et al.
2010/0308100	A1	12/2010	Boudreaux	2012/0071866	A1	3/2012	Kerr et al.
2010/0312261	A1	12/2010	Suzuki et al.	2012/0074196	A1	3/2012	Shelton, IV et al.
2011/0006099	A1	1/2011	Hall et al.	2012/0074198	A1	3/2012	Huitema et al.
2011/0006101	A1	1/2011	Hall et al.	2012/0074200	A1	3/2012	Schmid et al.
2011/0006103	A1	1/2011	Laurent et al.	2012/0074201	A1	3/2012	Baxter, III et al.
2011/0011914	A1	1/2011	Baxter, III et al.	2012/0080332	A1	4/2012	Shelton, IV et al.
2011/0011915	A1	1/2011	Shelton, IV	2012/0080333	A1	4/2012	Woodard, Jr. et al.
2011/0017801	A1	1/2011	Zemlok et al.	2012/0080334	A1	4/2012	Shelton, IV et al.
2011/0022032	A1	1/2011	Zemlok et al.	2012/0080335	A1	4/2012	Shelton, IV et al.
2011/0024477	A1	2/2011	Hall et al.	2012/0080336	A1	4/2012	Shelton, IV et al.
2011/0024478	A1	2/2011	Shelton, IV	2012/0080337	A1	4/2012	Shelton, IV et al.
2011/0024479	A1	2/2011	Swensgard et al.	2012/0080338	A1	4/2012	Shelton, IV et al.
2011/0036887	A1	2/2011	Zemlok et al.	2012/0080339	A1	4/2012	Shelton, IV et al.
2011/0042441	A1	2/2011	Shelton, IV et al.	2012/0080340	A1	4/2012	Shelton, IV et al.
2011/0060363	A1	3/2011	Hess et al.	2012/0080344	A1	4/2012	Shelton, IV
2011/0062212	A1	3/2011	Shelton, IV et al.	2012/0080345	A1	4/2012	Morgan et al.
2011/0068145	A1	3/2011	Bedi et al.	2012/0080475	A1	4/2012	Smith et al.
2011/0068148	A1	3/2011	Hall et al.	2012/0080477	A1	4/2012	Leimbach et al.
2011/0084112	A1	4/2011	Kostrzewski	2012/0080478	A1	4/2012	Morgan et al.
2011/0084113	A1	4/2011	Bedi et al.	2012/0080479	A1	4/2012	Shelton, IV
2011/0084115	A1	4/2011	Bedi et al.	2012/0080480	A1	4/2012	Woodard, Jr. et al.
2011/0087276	A1	4/2011	Bedi et al.	2012/0080481	A1	4/2012	Widenhouse et al.
2011/0087279	A1	4/2011	Shah et al.	2012/0080482	A1	4/2012	Schall et al.
2011/0095068	A1	4/2011	Patel	2012/0080483	A1	4/2012	Riestenberg et al.
2011/0101065	A1	5/2011	Milliman	2012/0080484	A1	4/2012	Morgan et al.
2011/0114697	A1	5/2011	Baxter, III et al.	2012/0080485	A1	4/2012	Woodard, Jr. et al.
2011/0114698	A1	5/2011	Baxter, III et al.	2012/0080486	A1	4/2012	Woodard, Jr. et al.
2011/0114699	A1	5/2011	Baxter, III et al.	2012/0080487	A1	4/2012	Woodard, Jr. et al.
2011/0114700	A1	5/2011	Baxter, III et al.	2012/0080488	A1	4/2012	Shelton, IV et al.
2011/0118761	A1	5/2011	Baxter, III et al.	2012/0080489	A1	4/2012	Shelton, IV et al.
2011/0121051	A1	5/2011	Shelton, IV et al.	2012/0080490	A1	4/2012	Shelton, IV et al.
2011/0121052	A1	5/2011	Shelton, IV et al.	2012/0080491	A1	4/2012	Shelton, IV et al.
2011/0125176	A1	5/2011	Yates et al.	2012/0080493	A1	4/2012	Shelton, IV et al.
2011/0125177	A1	5/2011	Yates et al.	2012/0080496	A1	4/2012	Schall et al.
2011/0132962	A1	6/2011	Hall et al.	2012/0080498	A1	4/2012	Shelton, IV et al.
2011/0132963	A1	6/2011	Giordano et al.	2012/0080499	A1	4/2012	Schall et al.
2011/0132964	A1	6/2011	Weisenburgh, II et al.	2012/0080500	A1	4/2012	Morgan et al.
2011/0132965	A1	6/2011	Moore et al.	2012/0080501	A1	4/2012	Morgan et al.
2011/0139852	A1	6/2011	Zingman	2012/0080502	A1	4/2012	Morgan et al.
2011/0144430	A1	6/2011	Spivey et al.	2012/0080503	A1	4/2012	Woodard, Jr. et al.
2011/0147433	A1	6/2011	Shelton, IV et al.	2012/0083833	A1	4/2012	Shelton, IV et al.
2011/0147434	A1	6/2011	Hueil et al.	2012/0083834	A1	4/2012	Shelton, IV et al.
2011/0155780	A1	6/2011	Boudreaux	2012/0083835	A1	4/2012	Shelton, IV et al.
2011/0155781	A1	6/2011	Swensgard et al.	2012/0083836	A1	4/2012	Shelton, IV et al.
2011/0155785	A1	6/2011	Laurent et al.	2012/0132450	A1	5/2012	Timm et al.
2011/0155787	A1	6/2011	Baxter, III et al.	2012/0138660	A1	6/2012	Shelton, IV
2011/0163147	A1	7/2011	Laurent et al.	2012/0160721	A1	6/2012	Shelton, IV et al.
2011/0174860	A1	7/2011	Shelton, IV et al.	2012/0175399	A1	7/2012	Shelton et al.
2011/0174861	A1	7/2011	Shelton, IV et al.	2012/0187179	A1	7/2012	Gleiman
2011/0174863	A1	7/2011	Shelton, IV et al.	2012/0199630	A1	8/2012	Shelton, IV et al.
2011/0178536	A1	7/2011	Kostrzewski	2012/0199631	A1	8/2012	Shelton, IV et al.
2011/0192882	A1	8/2011	Hess et al.	2012/0199632	A1	8/2012	Spivey et al.
2011/0210156	A1	9/2011	Smith et al.	2012/0199633	A1	8/2012	Shelton, IV et al.
2011/0226837	A1	9/2011	Baxter, III et al.	2012/0203247	A1	8/2012	Shelton, IV et al.

2012/0205421	A1	8/2012	Shelton, IV	EP	0324636	B1	3/1994
2012/0211546	A1	8/2012	Shelton, IV	EP	0593920	A1	4/1994
2012/0234890	A1	9/2012	Aronhalt et al.	EP	0594148	A1	4/1994
2012/0234891	A1	9/2012	Aronhalt et al.	EP	0427949	B1	6/1994
2012/0234892	A1	9/2012	Aronhalt et al.	EP	0523174	B1	6/1994
2012/0234893	A1	9/2012	Schuckmann et al.	EP	0600182	A2	6/1994
2012/0234895	A1	9/2012	O'Connor et al.	EP	0310431	B1	11/1994
2012/0234896	A1	9/2012	Ellerhorst et al.	EP	0375302	B1	11/1994
2012/0234897	A1	9/2012	Shelton, IV et al.	EP	0376562	B1	11/1994
2012/0234898	A1	9/2012	Shelton, IV et al.	EP	0630612	A1	12/1994
2012/0234899	A1	9/2012	Scheib et al.	EP	0634144	A1	1/1995
2012/0234900	A1	9/2012	Swayze	EP	0646356	A2	4/1995
2012/0238823	A1	9/2012	Hagerty et al.	EP	0646357	A1	4/1995
2012/0238824	A1	9/2012	Widenhouse et al.	EP	0653189	A2	5/1995
2012/0238826	A1	9/2012	Yoo et al.	EP	0669104	A1	8/1995
2012/0238829	A1	9/2012	Shelton, IV et al.	EP	0511470	B1	10/1995
2012/0239009	A1	9/2012	Mollere et al.	EP	0679367	A2	11/1995
2012/0239010	A1	9/2012	Shelton, IV et al.	EP	0392547	B1	12/1995
2012/0239012	A1	9/2012	Laurent et al.	EP	0685204	A1	12/1995
2012/0239075	A1	9/2012	Widenhouse et al.	EP	0364216	B1	1/1996
2012/0239082	A1	9/2012	Shelton, IV et al.	EP	0699418	A1	3/1996
2012/0241491	A1	9/2012	Aldridge et al.	EP	0702937	A1	3/1996
2012/0241492	A1	9/2012	Shelton, IV et al.	EP	0705571	A1	4/1996
2012/0241493	A1	9/2012	Baxter, III et al.	EP	0711611	A2	5/1996
2012/0241496	A1	9/2012	Vasudevan et al.	EP	0484677	B2	6/1996
2012/0241497	A1	9/2012	Vasudevan et al.	EP	0541987	B1	7/1996
2012/0241498	A1	9/2012	Gonzalez et al.	EP	0667119	B1	7/1996
2012/0241499	A1	9/2012	Baxter, III et al.	EP	0708618	B1	3/1997
2012/0241500	A1	9/2012	Timmer et al.	EP	0770355	A1	5/1997
2012/0241501	A1	9/2012	Swayze et al.	EP	0503662	B1	6/1997
2012/0241502	A1	9/2012	Aldridge et al.	EP	0447121	B1	7/1997
2012/0241503	A1	9/2012	Baxter, III et al.	EP	0625077	B1	7/1997
2012/0241505	A1	9/2012	Alexander, III et al.	EP	0633749	B1	8/1997
2012/0248169	A1	10/2012	Widenhouse et al.	EP	0710090	B1	8/1997
2012/0253298	A1	10/2012	Henderson et al.	EP	0578425	B1	9/1997
2012/0265230	A1	10/2012	Yates et al.	EP	0625335	B1	11/1997
2012/0273551	A1	11/2012	Shelton, IV et al.	EP	0552423	B1	1/1998
2012/0283707	A1	11/2012	Giordano et al.	EP	0592244	B1	1/1998
2012/0286019	A1	11/2012	Hueil et al.	EP	0648476	B1	1/1998
2012/0292367	A1	11/2012	Morgan et al.	EP	0649290	B1	3/1998
2012/0292370	A1	11/2012	Hess et al.	EP	0598618	B1	9/1998
2012/0298719	A1	11/2012	Shelton, IV et al.	EP	0676173	B1	9/1998
2013/0012931	A1	1/2013	Spivey et al.	EP	0678007	B1	9/1998
2013/0012957	A1	1/2013	Shelton, IV et al.	EP	0603472	B1	11/1998

FOREIGN PATENT DOCUMENTS

CA	2514274	A1	1/2006	EP	0878169	A1	11/1998
CN	1634601	A	7/2005	EP	0879742	A1	11/1998
CN	1868411	A	11/2006	EP	0695144	B1	12/1998
CN	1915180	A	2/2007	EP	0722296	B1	12/1998
CN	101095621	A	1/2008	EP	0760230	B1	2/1999
DE	273689	C	5/1914	EP	0623316	B1	3/1999
DE	1775926	A	1/1972	EP	0650701	B1	3/1999
DE	3036217	A1	4/1982	EP	0537572	B1	6/1999
DE	3210466	A1	9/1983	EP	0923907	A1	6/1999
DE	9412228	U	9/1994	EP	0843906	B1	3/2000
DE	19509116	A1	9/1996	EP	0552050	B1	5/2000
DE	19851291	A1	1/2000	EP	0833592	B1	5/2000
DE	19924311	A1	11/2000	EP	0830094	B1	9/2000
DE	69328576	T2	1/2001	EP	1034747	A1	9/2000
DE	10052679	A1	5/2001	EP	1034748	A1	9/2000
DE	20112837	U1	10/2001	EP	0694290	B1	11/2000
DE	20121753	U1	4/2003	EP	1050278	A1	11/2000
DE	10314072	A1	10/2004	EP	1053719	A1	11/2000
DE	202007003114	U1	6/2007	EP	1053720	A1	11/2000
EP	0122046	A1	10/1984	EP	1055399	A1	11/2000
EP	0070230	B1	10/1985	EP	1055400	A1	11/2000
EP	0156774	A2	10/1985	EP	1080694	A1	3/2001
EP	0387980	B1	10/1985	EP	1090592	A1	4/2001
EP	0033548	B1	5/1986	EP	1095627	A1	5/2001
EP	0129442	B1	11/1987	EP	1256318	B1	5/2001
EP	0276104	A2	7/1988	EP	0806914	B1	9/2001
EP	0178941	B1	1/1991	EP	0768840	B1	12/2001
EP	0248844	B1	1/1993	EP	0908152	B1	1/2002
EP	0545029	A1	6/1993	EP	0872213	B1	5/2002
EP	0277959	B1	10/1993	EP	0862386	B1	6/2002
EP	0233940	B1	11/1993	EP	0949886	B1	9/2002
EP	0261230	B1	11/1993	EP	1238634	A2	9/2002
EP	0639349	A2	2/1994	EP	0858295	B1	12/2002
				EP	0656188	B1	1/2003

US 8,459,520 B2

Page 14

EP	1284120	A1	2/2003	EP	1767163	A1	3/2007
EP	1287788	A1	3/2003	EP	1769756	A1	4/2007
EP	0717966	B1	4/2003	EP	1769758	A1	4/2007
EP	0869742	B1	5/2003	EP	1581128	B1	5/2007
EP	0829235	B1	6/2003	EP	1785097	A2	5/2007
EP	0887046	B1	7/2003	EP	1790293	A2	5/2007
EP	0852480	B1	8/2003	EP	1800610	A1	6/2007
EP	0891154	B1	9/2003	EP	1300117	B1	8/2007
EP	0813843	B1	10/2003	EP	1813199	A1	8/2007
EP	0873089	B1	10/2003	EP	1813201	A1	8/2007
EP	0856326	B1	11/2003	EP	1813203	A2	8/2007
EP	1374788	A1	1/2004	EP	1813207	A1	8/2007
EP	0741996	B1	2/2004	EP	1813209	A1	8/2007
EP	0814712	B1	2/2004	EP	1487359	B1	10/2007
EP	1402837	A1	3/2004	EP	1599146	B1	10/2007
EP	0705570	B1	4/2004	EP	1839596	A1	10/2007
EP	0959784	B1	4/2004	EP	2110083	A2	10/2007
EP	1407719	A2	4/2004	EP	1857057	A2	11/2007
EP	1086713	B1	5/2004	EP	1402821	B1	12/2007
EP	0996378	B1	6/2004	EP	1872727	A1	1/2008
EP	1426012	A1	6/2004	EP	1897502	A1	3/2008
EP	0833593	B2	7/2004	EP	1330201	B1	6/2008
EP	1442694	A1	8/2004	EP	1702568	B1	7/2008
EP	0888749	B1	9/2004	EP	1943957	A2	7/2008
EP	0959786	B1	9/2004	EP	1943964	A1	7/2008
EP	1459695	A1	9/2004	EP	1943976	A2	7/2008
EP	1473819	A1	11/2004	EP	1593337	B1	8/2008
EP	1477119	A1	11/2004	EP	1970014	A1	9/2008
EP	1479345	A1	11/2004	EP	1980213	A2	10/2008
EP	1479347	A1	11/2004	EP	1759645	B1	11/2008
EP	1479348	A1	11/2004	EP	1990014	A2	11/2008
EP	0754437	B2	12/2004	EP	1693008	B1	12/2008
EP	1025807	B1	12/2004	EP	1759640	B1	12/2008
EP	1001710	B1	1/2005	EP	2000102	A2	12/2008
EP	1520521	A1	4/2005	EP	2008595	A2	12/2008
EP	1520523	A1	4/2005	EP	1736104	B1	3/2009
EP	1520525	A1	4/2005	EP	1749486	B1	3/2009
EP	1522264	A1	4/2005	EP	2039316	A2	3/2009
EP	1523942	A2	4/2005	EP	1721576	B1	4/2009
EP	1550408	A1	7/2005	EP	1733686	B1	4/2009
EP	1557129	A1	7/2005	EP	2044890	A1	4/2009
EP	1064883	B1	8/2005	EP	1550413	B1	6/2009
EP	1067876	B1	8/2005	EP	1745748	B1	8/2009
EP	0870473	B1	9/2005	EP	2090237	A1	8/2009
EP	1157666	B1	9/2005	EP	2090244	A2	8/2009
EP	0880338	B1	10/2005	EP	2090245	A1	8/2009
EP	1158917	B1	11/2005	EP	2090256	A2	8/2009
EP	1344498	B1	11/2005	EP	2095777	A2	9/2009
EP	1330989	B1	12/2005	EP	2110082	A1	10/2009
EP	0771176	B2	1/2006	EP	1813208	B1	11/2009
EP	1621138	A2	2/2006	EP	2116195	A1	11/2009
EP	1621139	A2	2/2006	EP	1607050	B1	12/2009
EP	1621141	A2	2/2006	EP	1815804	B1	12/2009
EP	1621145	A2	2/2006	EP	1566150	B1	4/2010
EP	1621151	A2	2/2006	EP	1813206	B1	4/2010
EP	1034746	B1	3/2006	EP	1769754	B1	6/2010
EP	1632191	A2	3/2006	EP	1535565	B1	10/2010
EP	1065981	B1	5/2006	EP	1702570	B1	10/2010
EP	1082944	B1	5/2006	EP	1785098	B1	10/2010
EP	1652481	A2	5/2006	EP	2030578	B1	11/2010
EP	1382303	B1	6/2006	EP	1627605	B1	12/2010
EP	1253866	B1	7/2006	EP	1813205	B1	6/2011
EP	1032318	B1	8/2006	EP	1785102	B1	1/2012
EP	1045672	B1	8/2006	FR	999646	A	2/1952
EP	1617768	B1	8/2006	FR	1112936	A	3/1956
EP	1693015	A2	8/2006	FR	2598905	A1	11/1987
EP	1400214	B1	9/2006	FR	2765794	A	1/1999
EP	1702567	A2	9/2006	GB	939929	A	10/1963
EP	1129665	B1	11/2006	GB	1210522	A	10/1970
EP	1400206	B1	11/2006	GB	1217159	A	12/1970
EP	1721568	A1	11/2006	GB	1339394	A	12/1973
EP	1256317	B1	12/2006	GB	2109241	A	6/1983
EP	1285633	B1	12/2006	GB	2272159	A	5/1994
EP	1728473	A1	12/2006	GB	2284242	A	5/1995
EP	1728475	A2	12/2006	GB	2336214	A	10/1999
EP	1479346	B1	1/2007	GB	2425903	A	11/2006
EP	1484024	B1	1/2007	JP	S 58500053	A	1/1983
EP	1754445	A2	2/2007	JP	61-98249	A	5/1986
EP	1759812	A1	3/2007	JP	63-203149		8/1988

US 8,459,520 B2

Page 15

JP	3-12126 A	1/1991	WO	WO 96/24301 A1	8/1996
JP	5-212039 A	8/1993	WO	WO 96/27337 A1	9/1996
JP	6007357 A	1/1994	WO	WO 96/31155 A1	10/1996
JP	7051273 A	2/1995	WO	WO 96/35464 A1	11/1996
JP	8033641 A	2/1996	WO	WO 96/39085 A1	12/1996
JP	8229050 A	9/1996	WO	WO 96/39086 A1	12/1996
JP	2000033071 A	2/2000	WO	WO 96/39087 A1	12/1996
JP	2000171730 A	6/2000	WO	WO 96/39088 A1	12/1996
JP	2000287987 A	10/2000	WO	WO 96/39089 A1	12/1996
JP	2000325303 A	11/2000	WO	WO 97/00646 A1	1/1997
JP	2001-514541 A	9/2001	WO	WO 97/00647 A1	1/1997
JP	2001286477 A	10/2001	WO	WO 97/06582 A1	2/1997
JP	2002143078 A	5/2002	WO	WO 97/10763 A1	3/1997
JP	2002369820 A	12/2002	WO	WO 97/10764 A1	3/1997
JP	2003-500153 A	1/2003	WO	WO 97/11648 A2	4/1997
JP	2004-344663	12/2004	WO	WO 97/11649 A1	4/1997
JP	2005-028149 A	2/2005	WO	WO 97/15237 A1	5/1997
JP	2005505322 T	2/2005	WO	WO 97/24073 A1	7/1997
JP	2005103293 A	4/2005	WO	WO 97/24993 A1	7/1997
JP	2005131163 A	5/2005	WO	WO 97/30644 A1	8/1997
JP	2005131164 A	5/2005	WO	WO 97/34533 A1	9/1997
JP	2005131173 A	5/2005	WO	WO 97/37598 A1	10/1997
JP	2005131211 A	5/2005	WO	WO 97/39688 A2	10/1997
JP	2005131212 A	5/2005	WO	WO 98/17180 A1	4/1998
JP	2005137423 A	6/2005	WO	WO 98/27880 A1	7/1998
JP	2005152416 A	6/2005	WO	WO 98/30153 A1	7/1998
JP	2005-523105 A	8/2005	WO	WO 98/47436 A1	10/1998
JP	2005524474 A	8/2005	WO	WO 99/03407 A1	1/1999
JP	2006-281405 A	10/2006	WO	WO 99/03408 A1	1/1999
RU	2008830 C1	3/1994	WO	WO 99/03409 A1	1/1999
RU	2187249 C2	8/2002	WO	WO 99/12483 A1	3/1999
RU	2225170 C2	3/2004	WO	WO 99/12487 A1	3/1999
SU	189517 A	1/1967	WO	WO 99/12488 A1	3/1999
SU	328636 A	9/1972	WO	WO 99/15086 A1	4/1999
SU	886900 A1	12/1981	WO	WO 99/15091 A1	4/1999
SU	1009439 A	4/1983	WO	WO 99/23933 A2	5/1999
SU	1333319 A2	8/1987	WO	WO 99/23959 A1	5/1999
SU	1377053 A1	2/1988	WO	WO 99/25261 A1	5/1999
SU	1561964 A1	5/1990	WO	WO 99/29244 A1	6/1999
SU	1722476 A1	3/1992	WO	WO 99/34744 A1	7/1999
WO	WO 82/02824 A1	9/1982	WO	WO 99/45849 A1	9/1999
WO	WO 91/15157 A1	10/1991	WO	WO 99/48430 A1	9/1999
WO	WO 92/20295 A1	11/1992	WO	WO 99/51158 A1	10/1999
WO	WO 92/21300 A1	12/1992	WO	WO 00/24322 A1	5/2000
WO	WO 93/08755 A1	5/1993	WO	WO 00/24330 A1	5/2000
WO	WO 93/13718 A1	7/1993	WO	WO 00/41638 A1	7/2000
WO	WO 93/14690 A1	8/1993	WO	WO 00/48506 A1	8/2000
WO	WO 93/15850 A1	8/1993	WO	WO 00/53112 A2	9/2000
WO	WO 9315648 A1 *	8/1993	WO	WO 00/54653 A1	9/2000
WO	WO 93/19681 A1	10/1993	WO	WO 00/57796 A1	10/2000
WO	WO 94/00060 A1	1/1994	WO	WO 00/64365 A1	11/2000
WO	WO 94/11057 A1	5/1994	WO	WO 00/72762 A1	12/2000
WO	WO 94/12108 A1	6/1994	WO	WO 00/72765 A1	12/2000
WO	WO 94/18893 A1	9/1994	WO	WO 01/03587 A1	1/2001
WO	WO 94/22378 A1	10/1994	WO	WO 01/05702 A1	1/2001
WO	WO 94/23659 A1	10/1994	WO	WO 01/10482 A1	2/2001
WO	WO 95/02369 A1	1/1995	WO	WO 01/35845 A1	5/2001
WO	WO 95/03743 A1	2/1995	WO	WO 01/54594 A1	8/2001
WO	WO 95/06817 A1	3/1995	WO	WO 01/58371 A1	8/2001
WO	WO 95/09576 A1	4/1995	WO	WO 01/62158 A2	8/2001
WO	WO 95/09577 A1	4/1995	WO	WO 01/62161 A1	8/2001
WO	WO 95/14436 A1	6/1995	WO	WO 01/62162 A1	8/2001
WO	WO 95/17855 A1	7/1995	WO	WO 01/62164 A2	8/2001
WO	WO 95/18383 A1	7/1995	WO	WO 01/62169 A2	8/2001
WO	WO 95/18572 A1	7/1995	WO	WO 01/78605 A2	10/2001
WO	WO 95/19739 A1	7/1995	WO	WO 01/91646 A1	12/2001
WO	WO 95/20360 A1	8/1995	WO	WO 02/07608 A2	1/2002
WO	WO 95/23557 A1	9/1995	WO	WO 02/07618 A1	1/2002
WO	WO 95/24865 A1	9/1995	WO	WO 02/17799 A1	3/2002
WO	WO 95/25471 A3	9/1995	WO	WO 02/19920 A1	3/2002
WO	WO 95/26562 A1	10/1995	WO	WO 02/19932 A1	3/2002
WO	WO 95/29639 A1	11/1995	WO	WO 02/30297 A2	4/2002
WO	WO 96/04858 A1	2/1996	WO	WO 02/32322 A2	4/2002
WO	WO 96/19151 A1	6/1996	WO	WO 02/36028 A1	5/2002
WO	WO 96/19152 A1	6/1996	WO	WO 02/43571 A2	6/2002
WO	WO 96/20652 A1	7/1996	WO	WO 02/058568 A1	8/2002
WO	WO 96/21119 A1	7/1996	WO	WO 02/060328 A1	8/2002
WO	WO 96/22055 A1	7/1996	WO	WO 02/067785 A2	9/2002
WO	WO 96/23448 A1	8/1996	WO	WO 02/098302 A1	12/2002

WO WO 03/000138 A2 1/2003
 WO WO 03/001329 A2 1/2003
 WO WO 03/013363 A1 2/2003
 WO WO 03/015604 A2 2/2003
 WO WO 03/020106 A2 3/2003
 WO WO 03/020139 A2 3/2003
 WO WO 03/024339 A1 3/2003
 WO WO 03/079909 A3 3/2003
 WO WO 03/030743 A2 4/2003
 WO WO 03/037193 A1 5/2003
 WO WO 03/047436 A3 6/2003
 WO WO 03/055402 A1 7/2003
 WO WO 03/057048 A1 7/2003
 WO WO 03/057058 A1 7/2003
 WO WO 03/063694 A1 8/2003
 WO WO 03/077769 A1 9/2003
 WO WO 03/079911 A1 10/2003
 WO WO 03/082126 A1 10/2003
 WO WO 03/088845 A2 10/2003
 WO WO 03/090630 A2 11/2003
 WO WO 03/094743 A1 11/2003
 WO WO 03/094745 A1 11/2003
 WO WO 03/094746 A1 11/2003
 WO WO 03/094747 A1 11/2003
 WO WO 03090630 A2 * 11/2003
 WO WO 03/101313 A1 12/2003
 WO WO 03/105698 A2 12/2003
 WO WO 03/105702 A2 12/2003
 WO WO 2004/006980 A2 1/2004
 WO WO 2004/011037 A2 2/2004
 WO WO 2004/019769 A1 3/2004
 WO WO 2004/021868 A2 3/2004
 WO WO 2004/028585 A2 4/2004
 WO WO 2004/032754 A2 4/2004
 WO WO 2004/032760 A2 4/2004
 WO WO 2004/032762 A1 4/2004
 WO WO 2004/032763 A2 4/2004
 WO WO 2004/034875 A2 4/2004
 WO WO 2004/047626 A1 6/2004
 WO WO 2004/047653 A2 6/2004
 WO WO 2004/049956 A2 6/2004
 WO WO 2004/052426 A2 6/2004
 WO WO 2004/056276 A1 7/2004
 WO WO 2004/056277 A1 7/2004
 WO WO 2004/062516 A1 7/2004
 WO WO 2004/078050 A2 9/2004
 WO WO 2004/078051 A2 9/2004
 WO WO 2004/086987 A1 10/2004
 WO WO 2004/096015 A2 11/2004
 WO WO 2004/096057 A2 11/2004
 WO WO 2004/103157 A2 12/2004
 WO WO 2004/105593 A1 12/2004
 WO WO 2004/105621 A1 12/2004
 WO WO 2004/112618 A2 12/2004
 WO WO 2004/112652 A2 12/2004
 WO WO 2005/027983 A2 3/2005
 WO WO 2005/037329 A2 4/2005
 WO WO 2005/044078 A2 5/2005
 WO WO 2005/055846 A1 6/2005
 WO WO 2005/072634 A2 8/2005
 WO WO 2005/078892 A1 8/2005
 WO WO 2005/079675 A2 9/2005
 WO WO 2005/096954 A2 10/2005
 WO WO 2005/112806 A2 12/2005
 WO WO 2005/112808 A1 12/2005
 WO WO 2005/115251 A2 12/2005
 WO WO 2005/115253 A2 12/2005
 WO WO 2005/117735 A1 12/2005
 WO WO 2005/122936 A1 12/2005
 WO WO 2006/027014 A1 3/2006
 WO WO 2006/044490 A2 4/2006
 WO WO 2006/044581 A2 4/2006
 WO WO 2006/044810 A2 4/2006
 WO WO 2006/051252 A1 5/2006
 WO WO 2006/059067 A1 6/2006
 WO WO 2006/083748 A1 8/2006
 WO WO 2006/092563 A1 9/2006

WO WO 2006/092565 A1 9/2006
 WO WO 2006/115958 A1 11/2006
 WO WO 2006/125940 A1 11/2006
 WO WO 2006/132992 A1 12/2006
 WO WO 2007/002180 A2 1/2007
 WO WO 2007/016290 A2 2/2007
 WO WO 2007/018898 A2 2/2007
 WO WO 2007/098220 A2 8/2007
 WO WO 2007/121579 A1 11/2007
 WO WO 2007/131110 A2 11/2007
 WO WO 2007/137304 A2 11/2007
 WO WO 2007/139734 A2 12/2007
 WO WO 2007/142625 A2 12/2007
 WO WO 2007/147439 A1 12/2007
 WO WO 2008/021969 A2 2/2008
 WO WO 2008/039249 A1 4/2008
 WO WO 2008/039270 A1 4/2008
 WO WO 2008/045383 A2 4/2008
 WO WO 2008/070763 A1 6/2008
 WO WO 2008/089404 A2 7/2008
 WO WO 2008/109125 A1 9/2008
 WO WO 2010/063795 A1 6/2010
 WO WO 2012/044844 A2 4/2012

OTHER PUBLICATIONS

Disclosed Anonymously, "Motor-Driven Surgical Stapler Improvements," Research Disclosure Database No. 526041, Published: Feb. 2008.

C.C. Thompson et al., "Peroral Endoscopic Reduction of Dilated Gastrojejunal Anastomosis After Roux-en-Y Gastric Bypass: A Possible New Option for Patients with Weight Regain," *Surg Endosc* (2006) vol. 20, pp. 1744-1748.

B.R. Coolman, DVM, MS et al., "Comparison of Skin Staples With Sutures for Anastomosis of the Small Intestine in Dogs," Abstract; <http://www.blackwell-synergy.com/doi/abs/10.1053/jvet.2000.7539?cookieSet=1&journalCode=vsu> which redirects to <http://www3.interscience.wiley.com/journal/119040681/abstract?CRETRY=1&SRETRY=0>; [online] accessed: Sep. 22, 2008 (2 pages).

The Soderm Aseptic Battery Transfer Kit, Soderm Systems, 2000, 3 pages.

"Biomedical Coatings," Fort Wayne Metals, Research Products Corporation, obtained online at www.fwmetals.com on Jun. 21, 2010 (1 page).

Van Meer et al., "A Disposable Plastic Compact Wrist for Smart Minimally Invasive Surgical Tools," *LAAS/CNRS* (Aug. 2005).

Breedveld et al., "A New, Easily Miniaturized Sterrable Endoscope," *IEEE Engineering in Medicine and Biology Magazine* (Nov./Dec. 2005).

D. Tuite, Ed., "Get the Lowdown on Ultracapacitors," Nov. 15, 2007; [online] URL: <http://electronicdesign.com/Articles/Print.cfm?ArticleID=17465>, accessed Jan. 15, 2008 (5 pages).

Datasheet for Panasonic TK Relays Ultra Low Profile 2 a Polarized Relay, Copyright Matsushita Electric Works, Ltd. (Known of at least as early as Aug. 17, 2010), 5 pages.

ASTM procedure D2240-00, "Standard Test Method for Rubber Property-Durometer Hardness," (Published Aug. 2000).

ASTM procedure D2240-05, "Standard Test Method for Rubber Property-Durometer Hardness," (Published Apr. 2010).

U.S. Appl. No. 13/488,903, filed Jun. 5, 2012.

European Examination Report, Application No. 08250080.2, dated Jun. 14, 2010 (4 pages).

International Search Report for PCT/US2012/026997, May 7, 2012 (5 pages).

Written Opinion for PCT/US2012/026997, May 7, 2012 (6 pages).

International Search Report for PCT/US2012/039156, Oct. 29, 2012 (4 pages).

Written Opinion for PCT/US2012/039156, Oct. 29, 2012 (6 pages).

European Search Report for Application No. 12173458.6, dated Dec. 6, 2012 (8 pages).

* cited by examiner

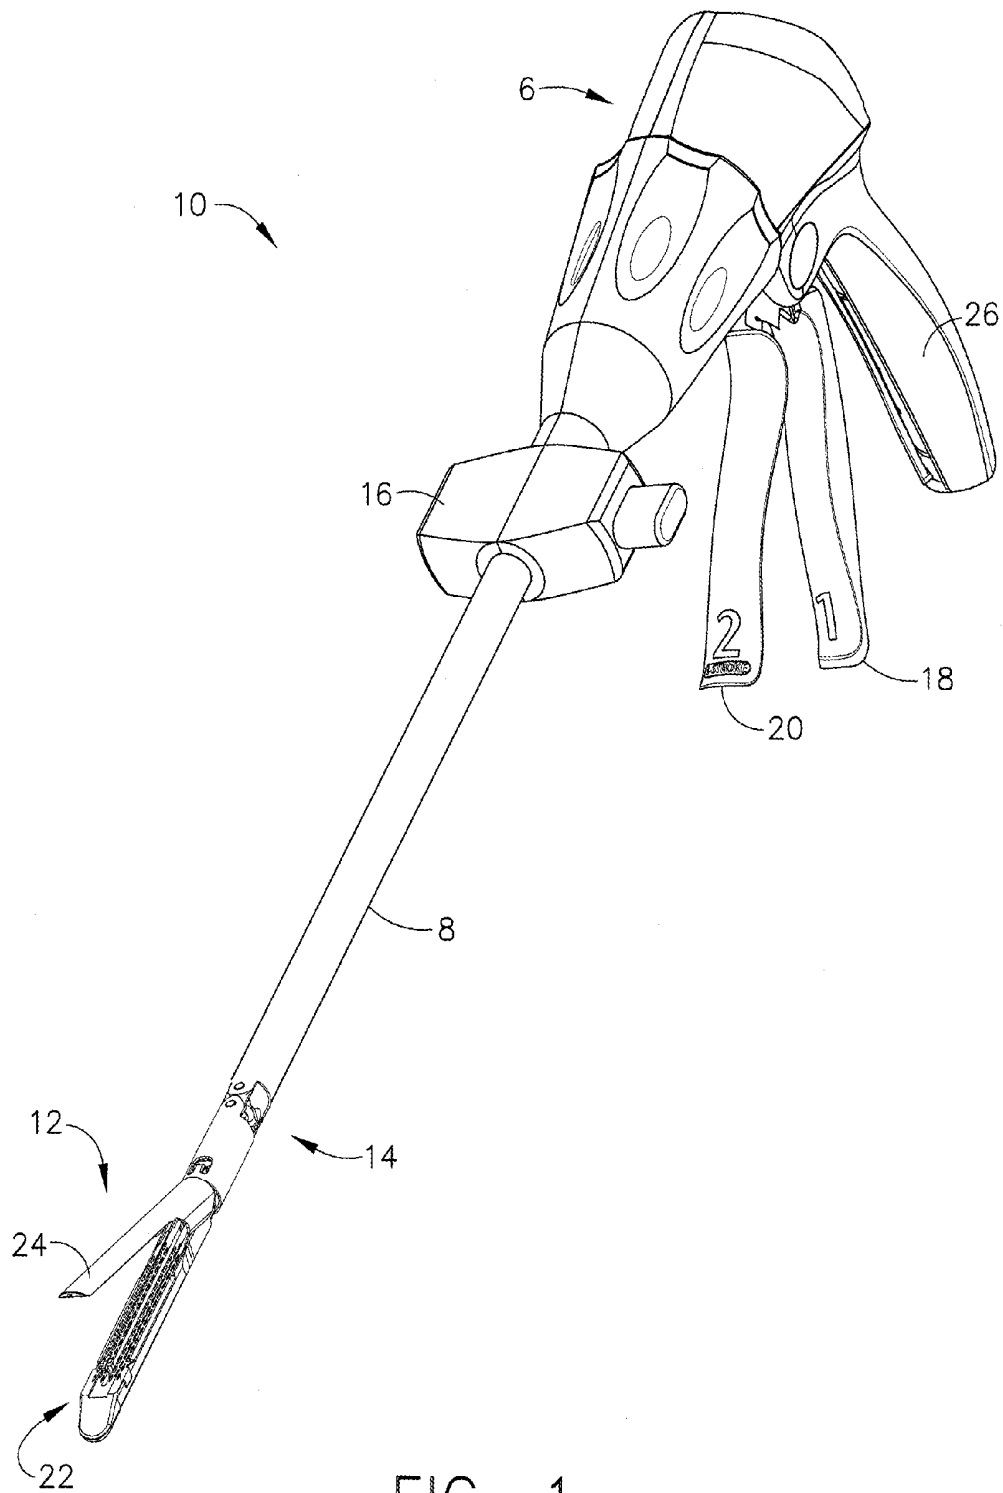


FIG. 1

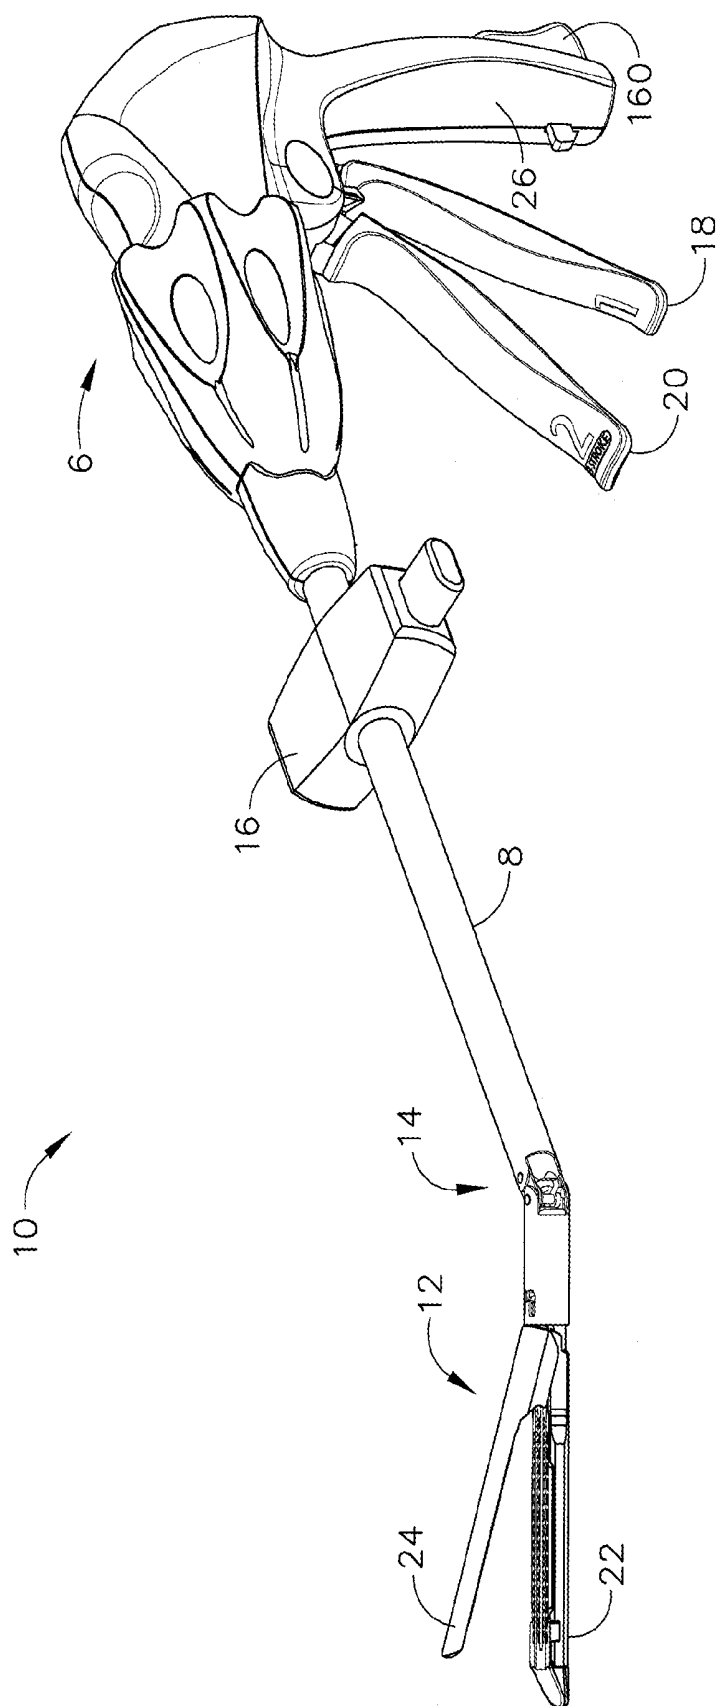


FIG. 2

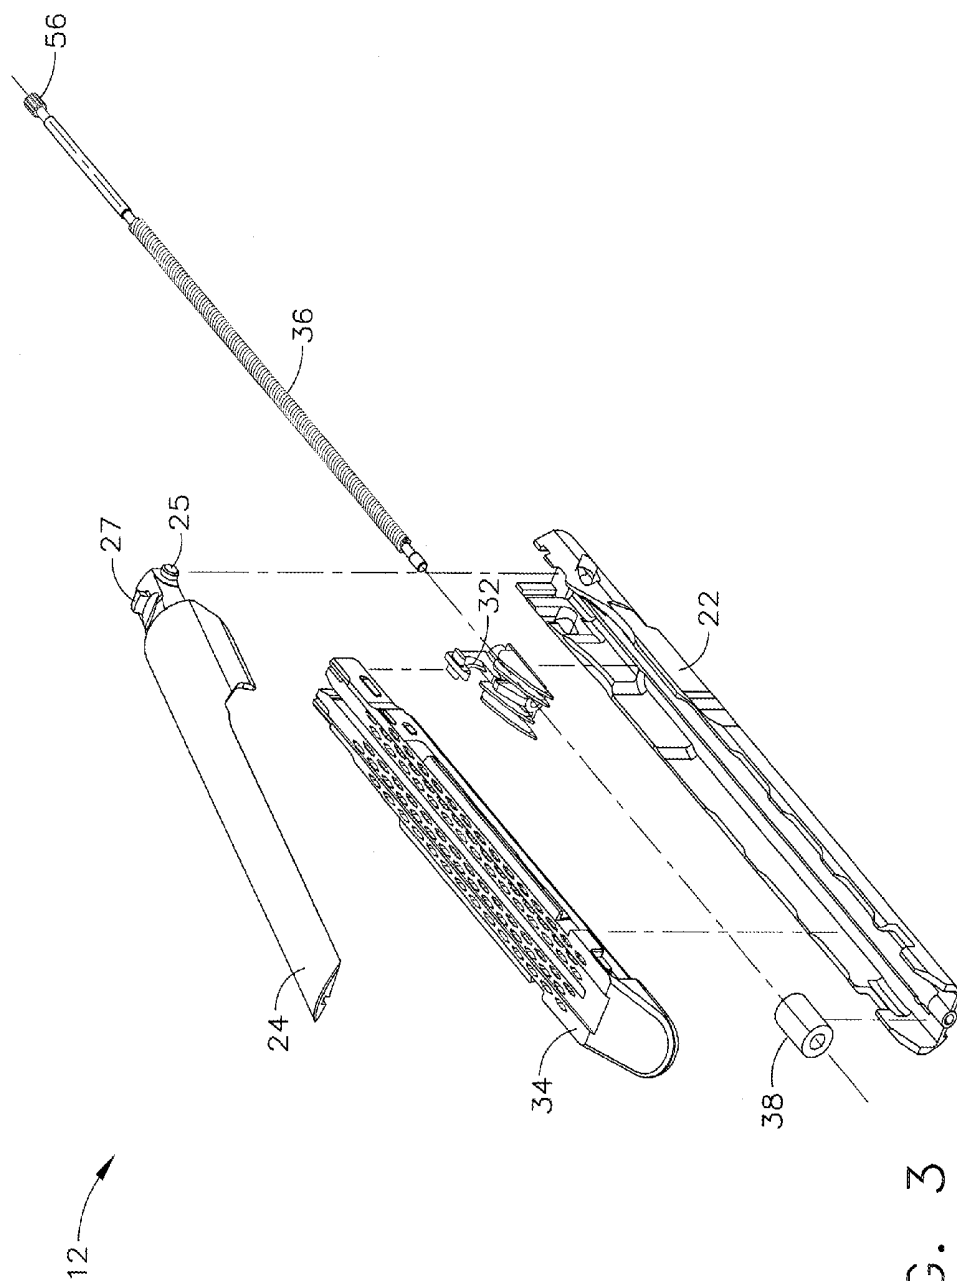


FIG. 3

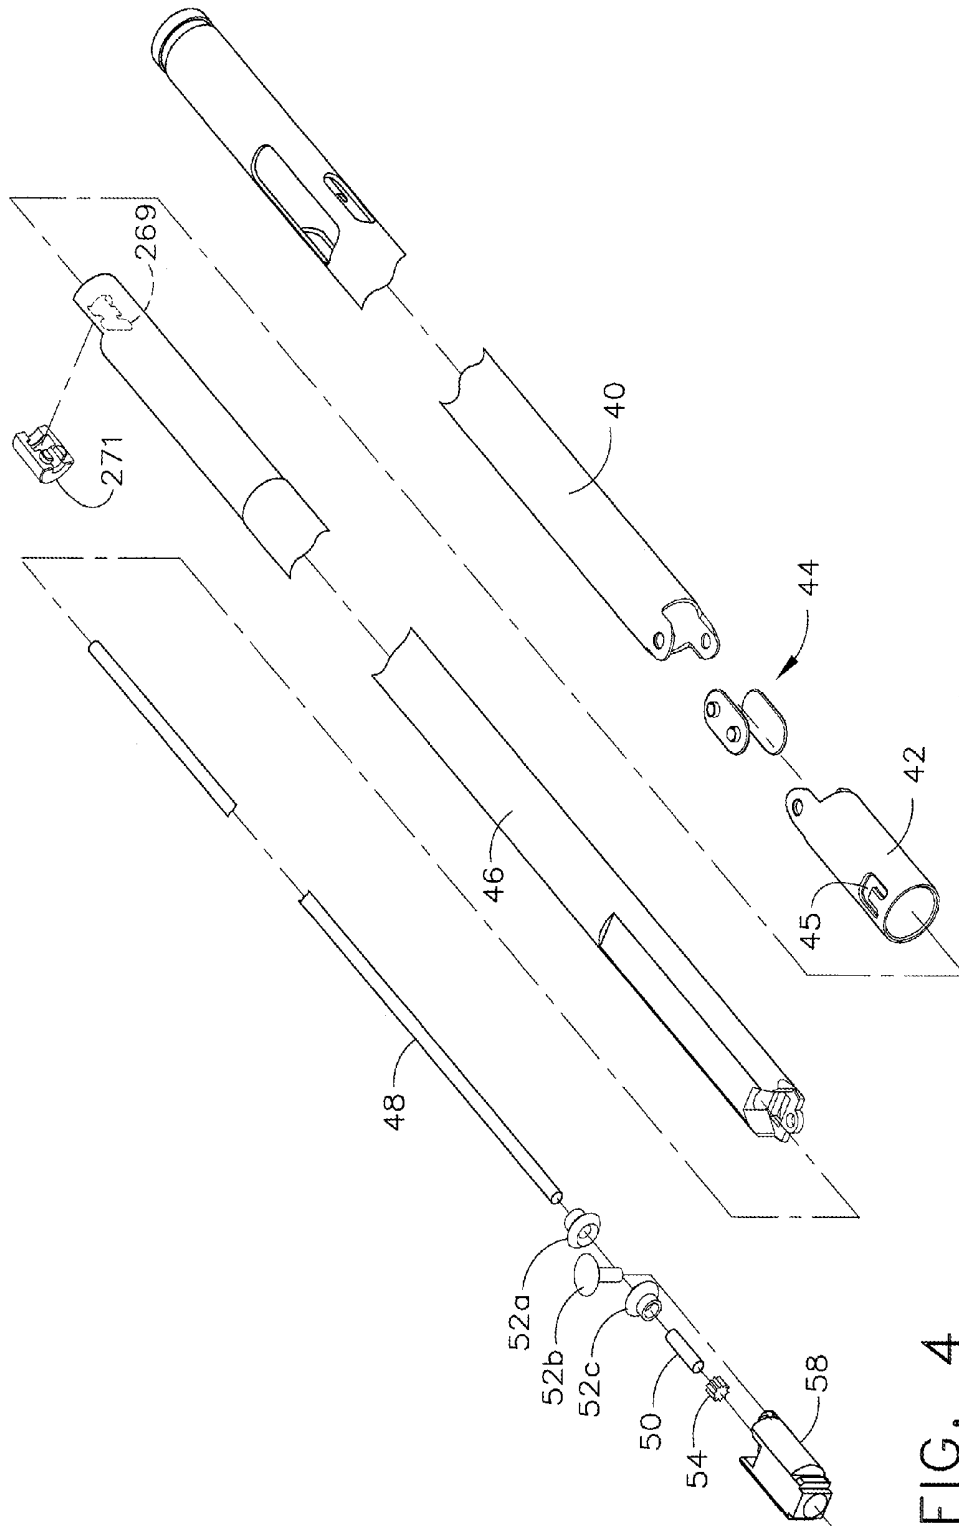


FIG. 4

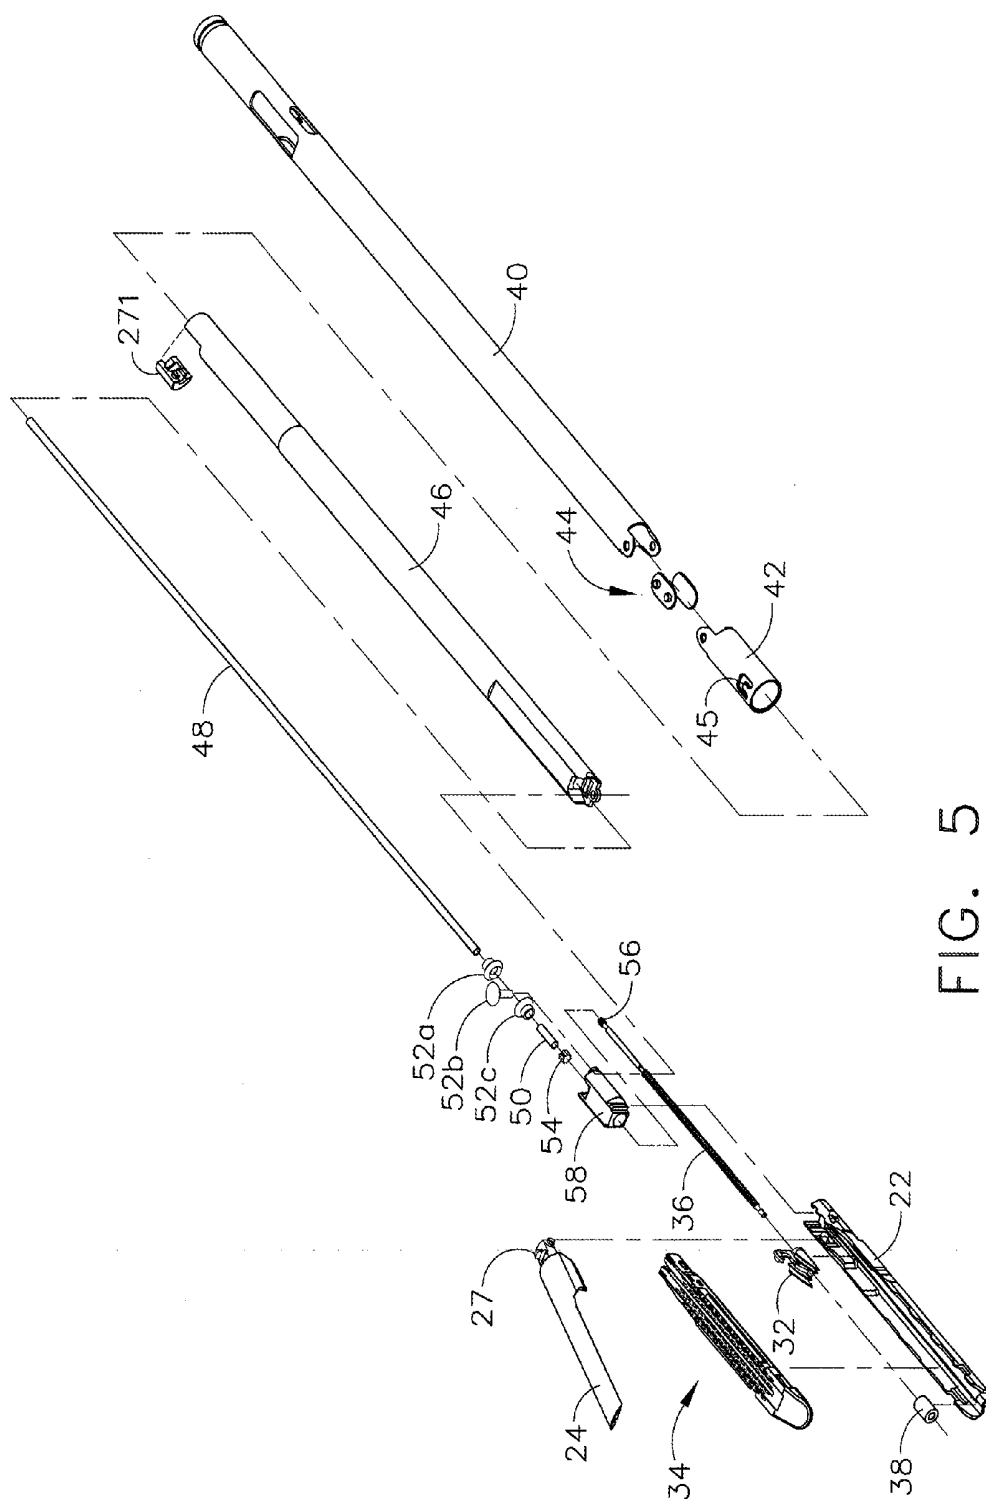


FIG. 5

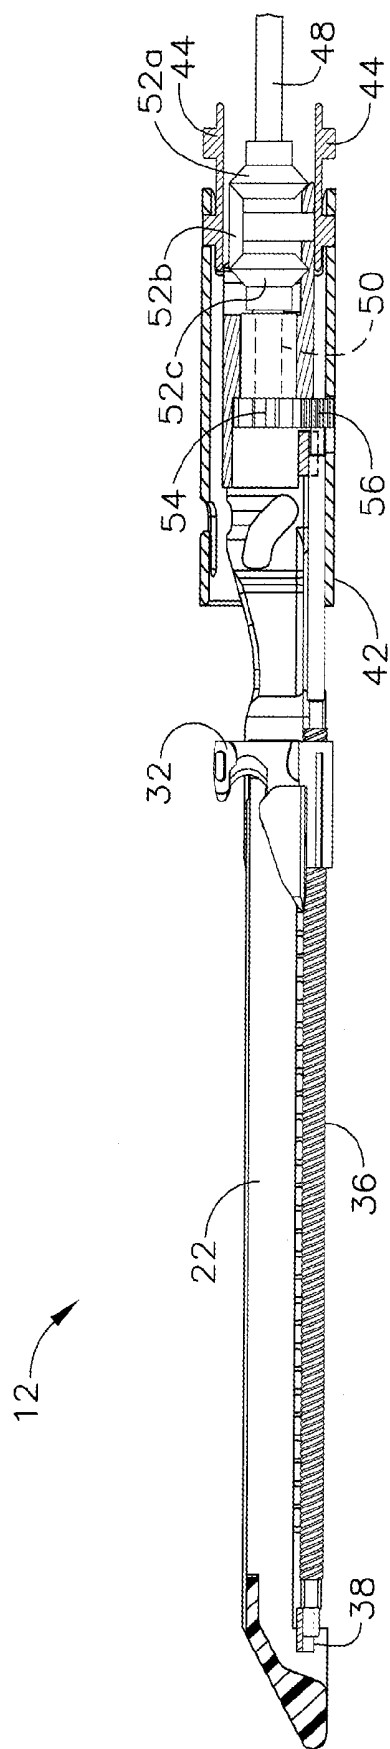
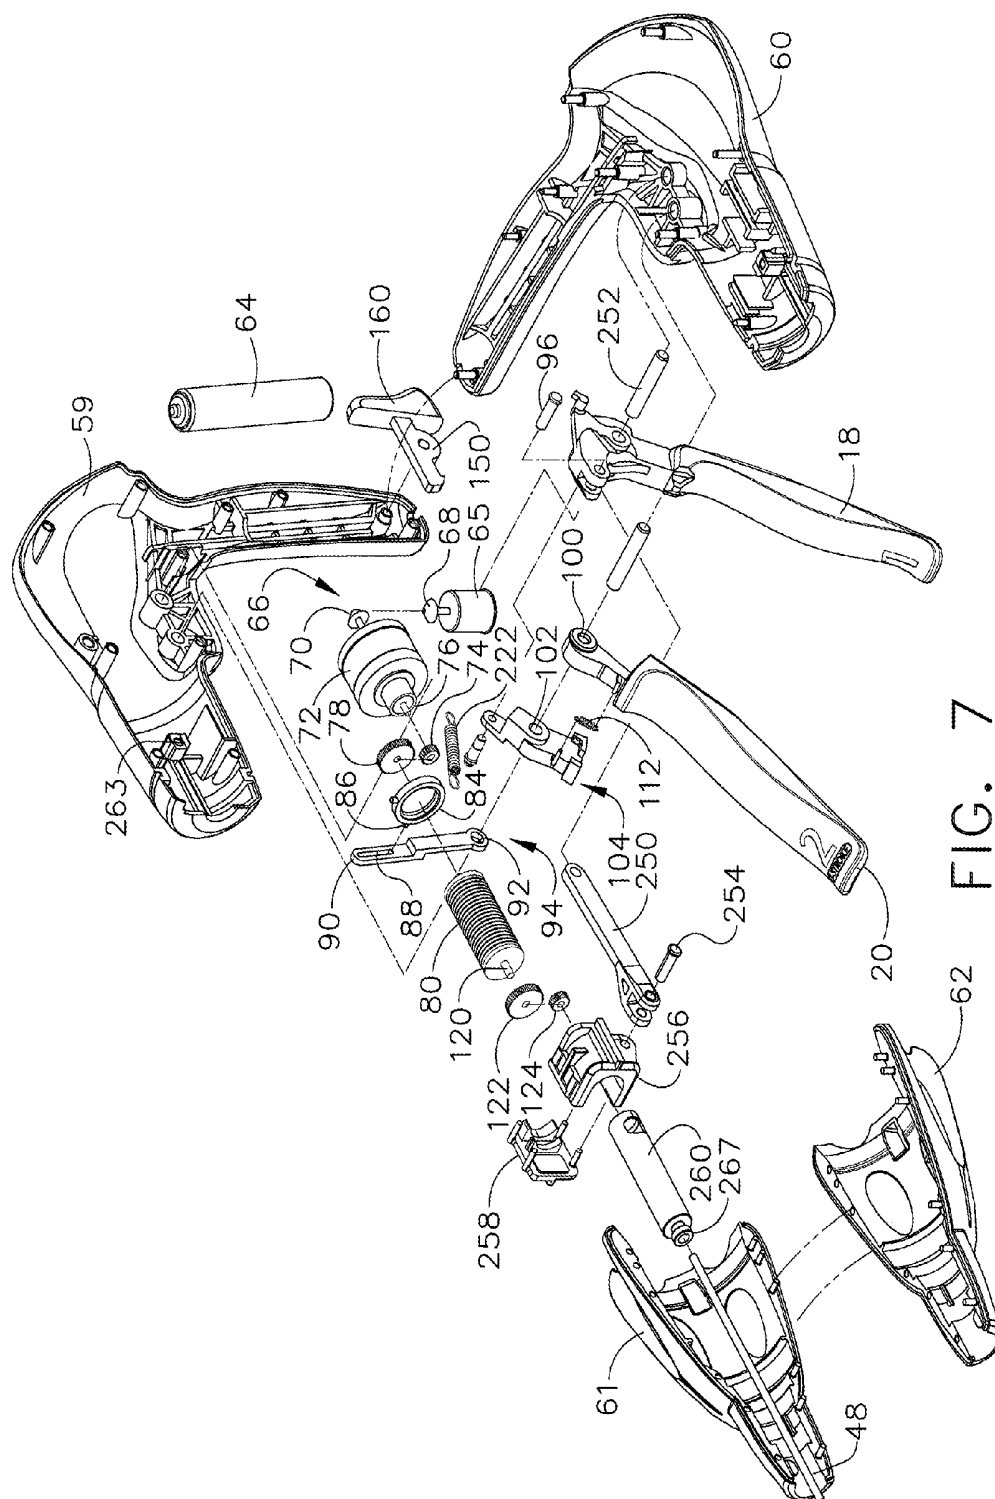


FIG. 6



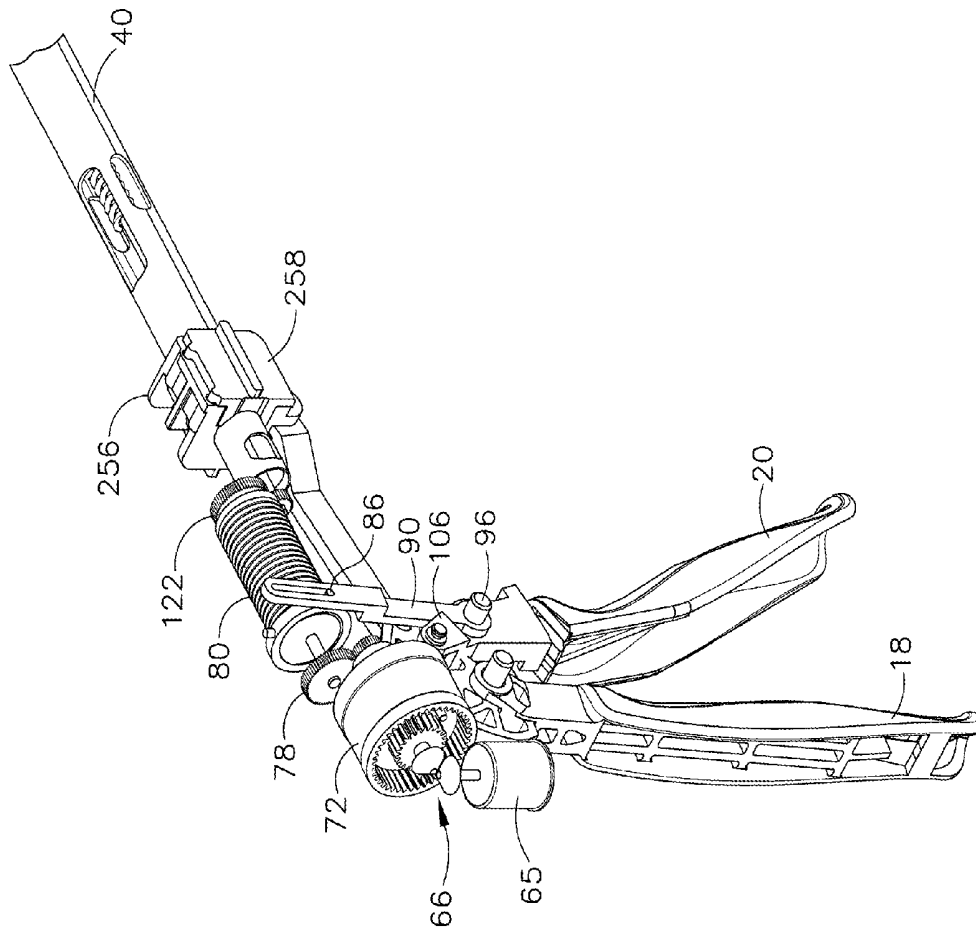


FIG. 8

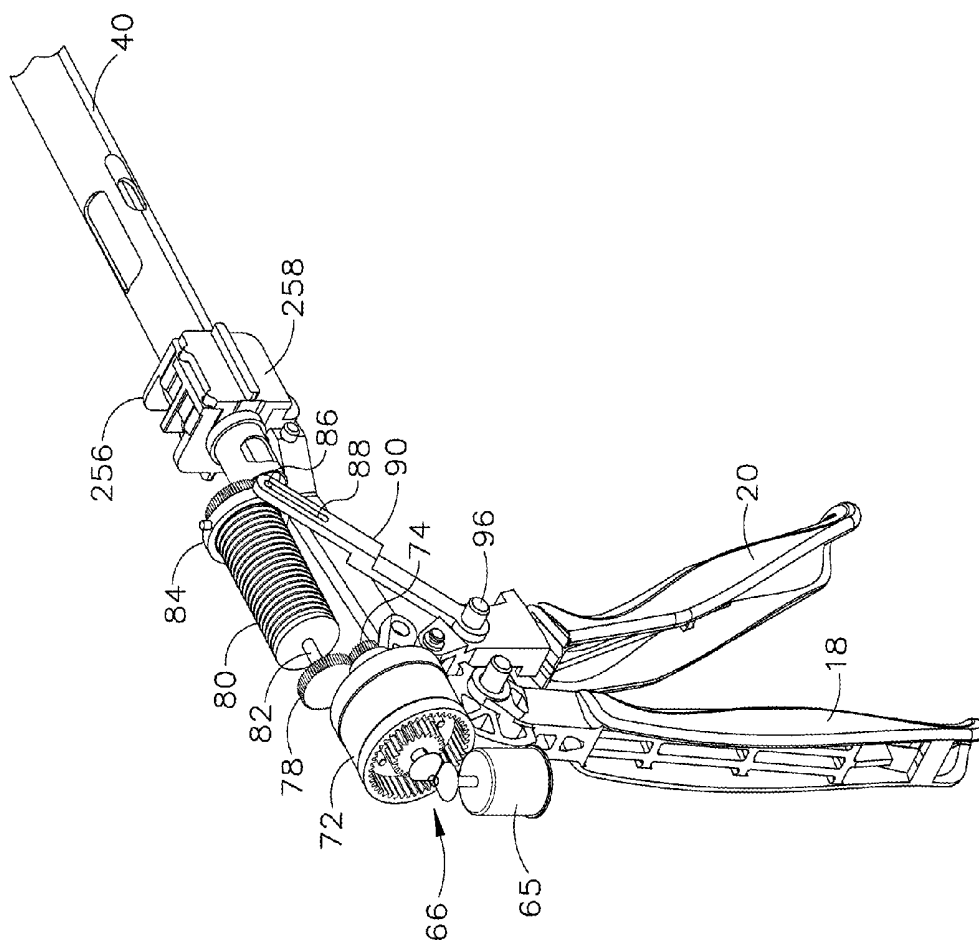


FIG. 9

FIG. 10

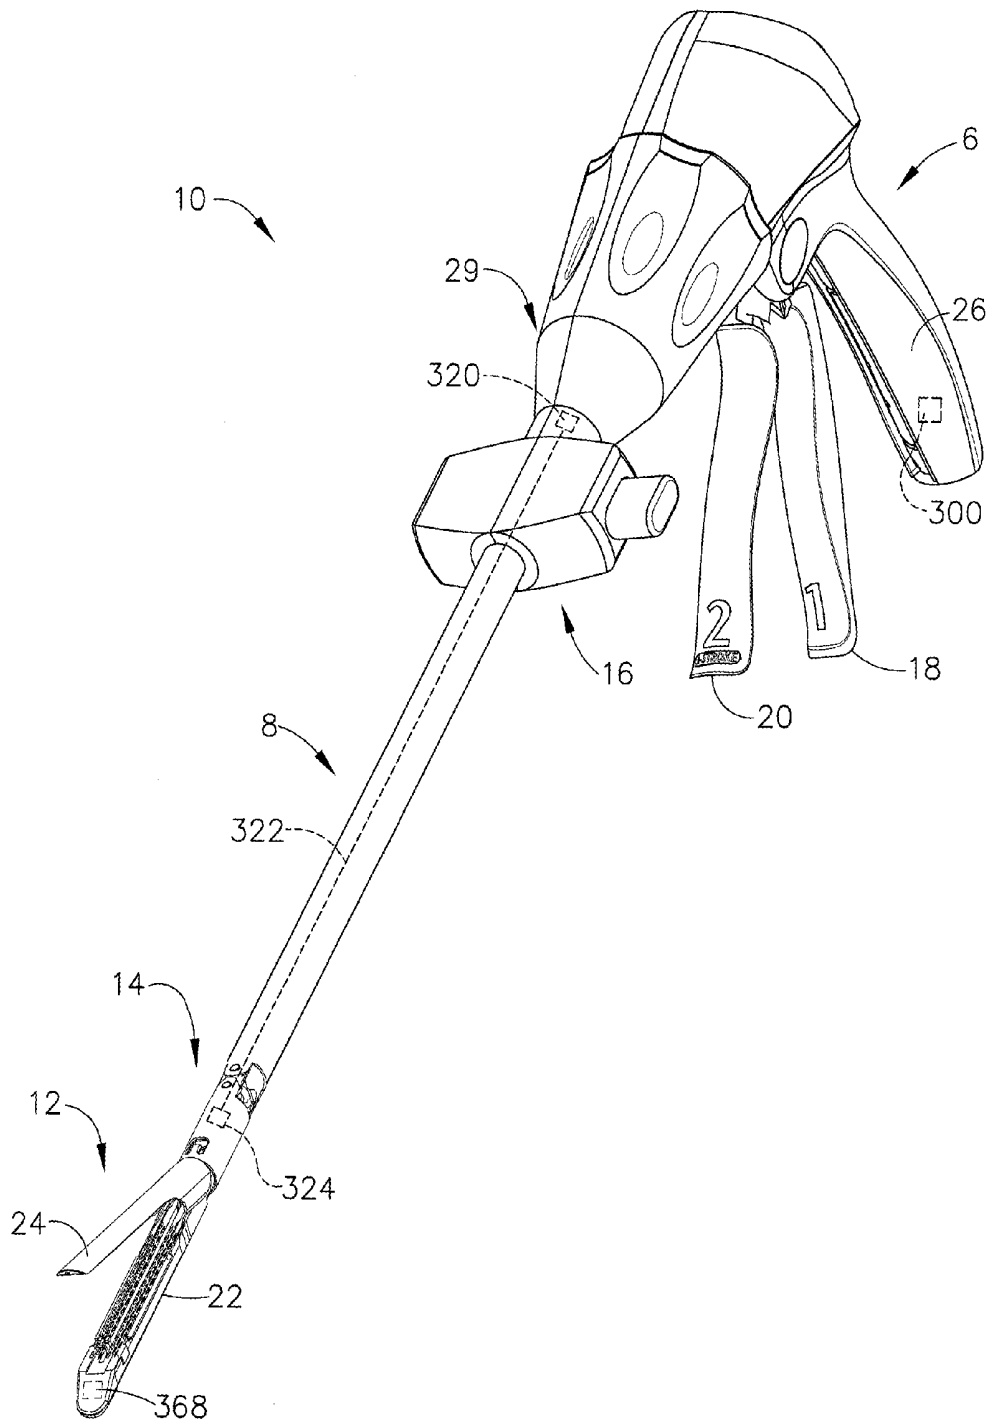


FIG. 11

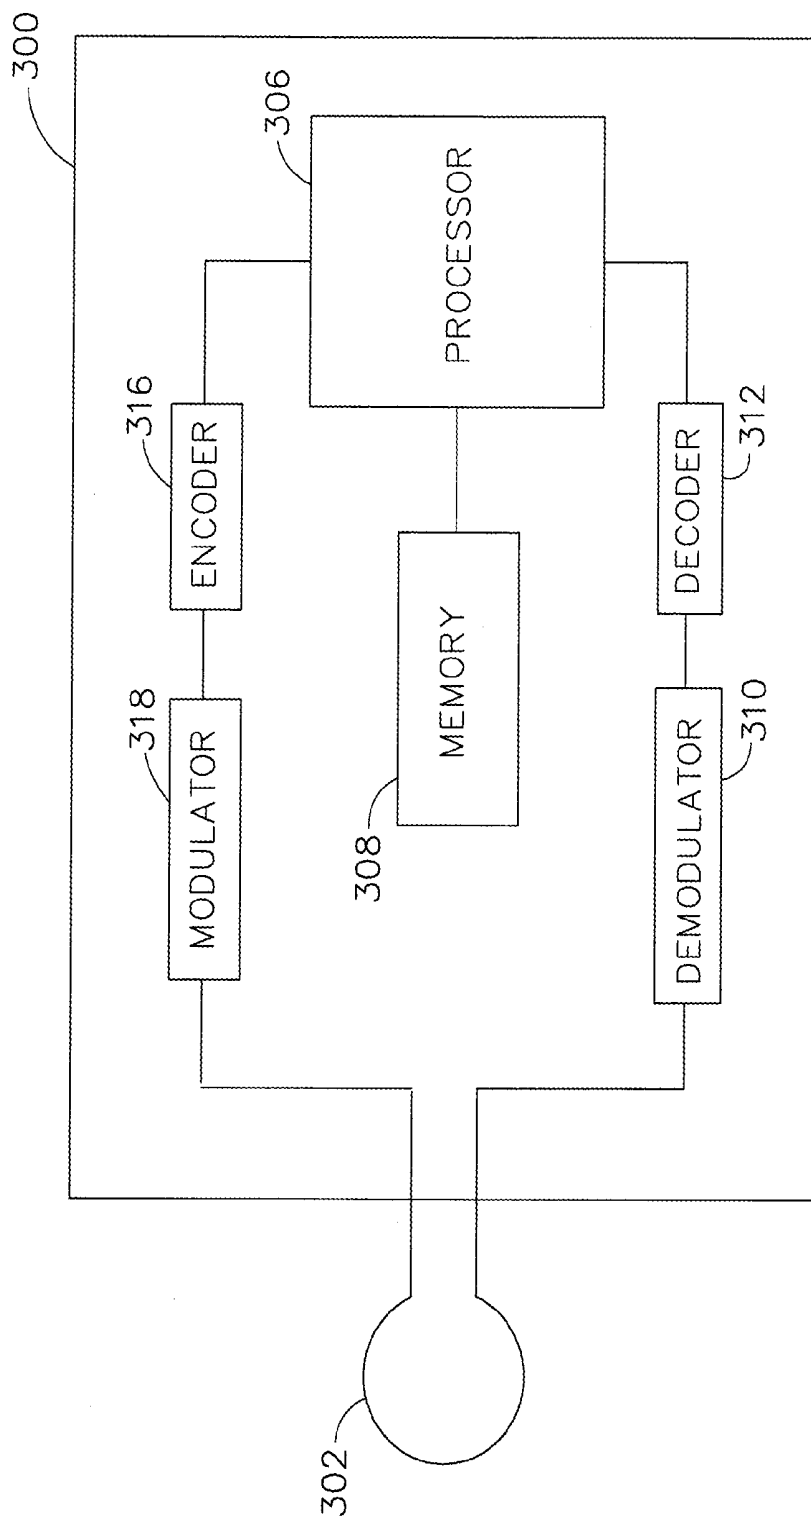


FIG. 12

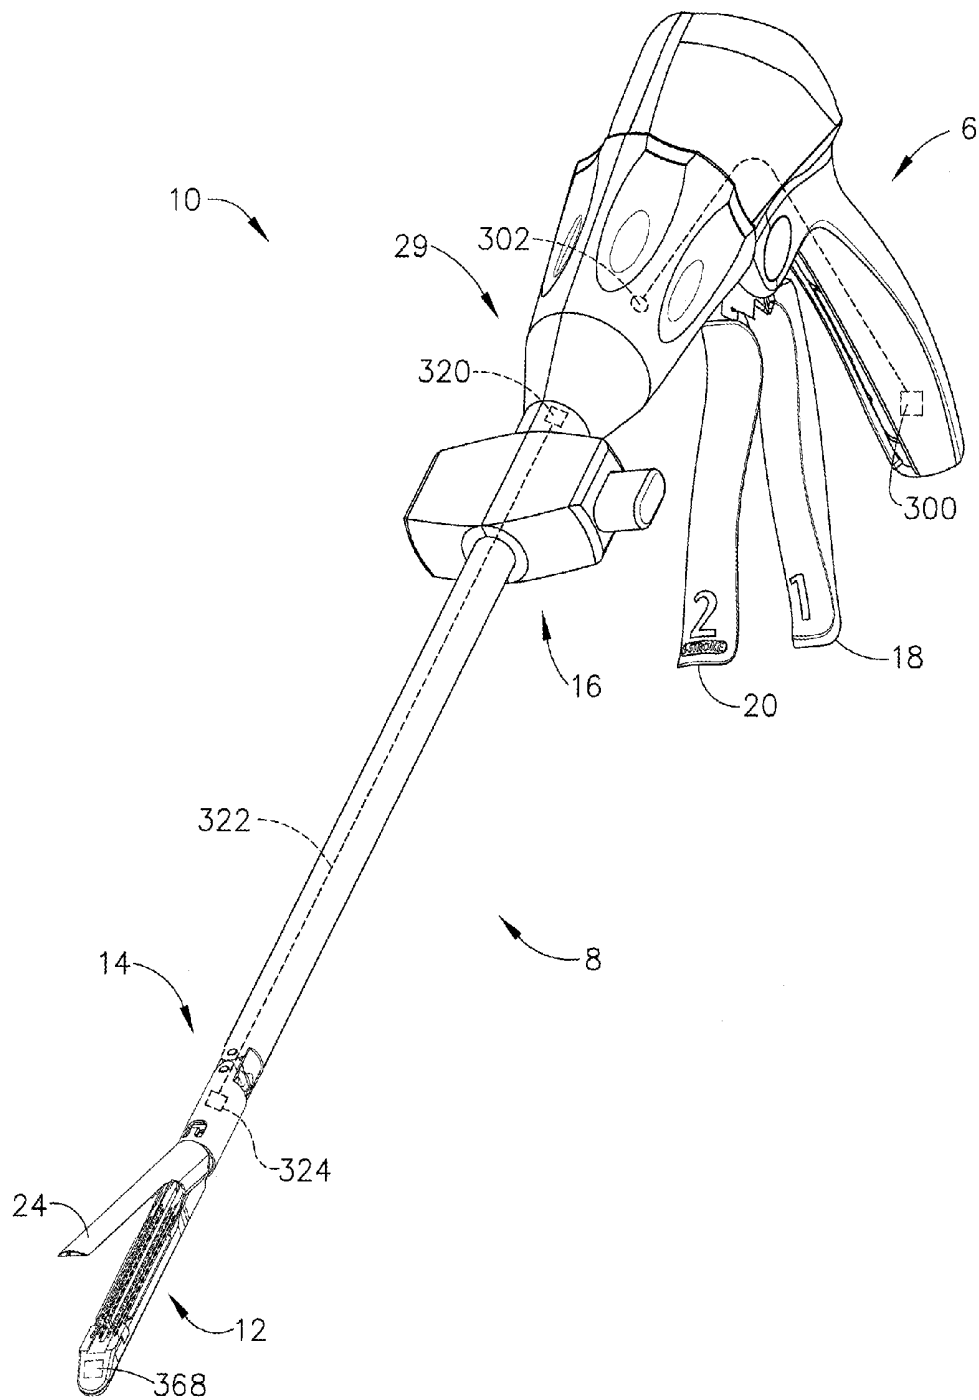


FIG. 13

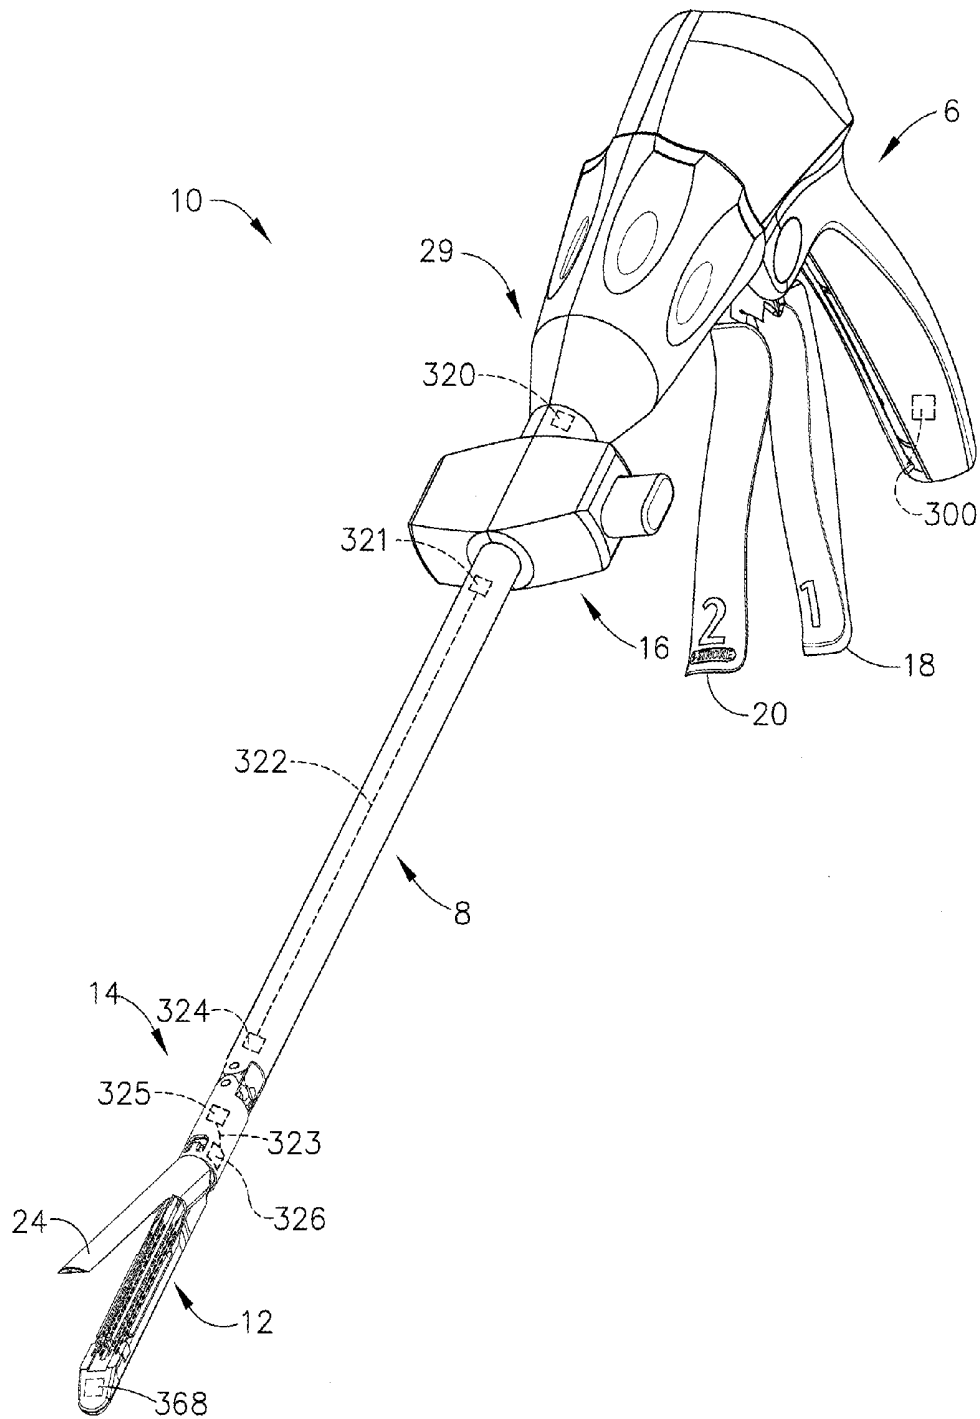


FIG. 14

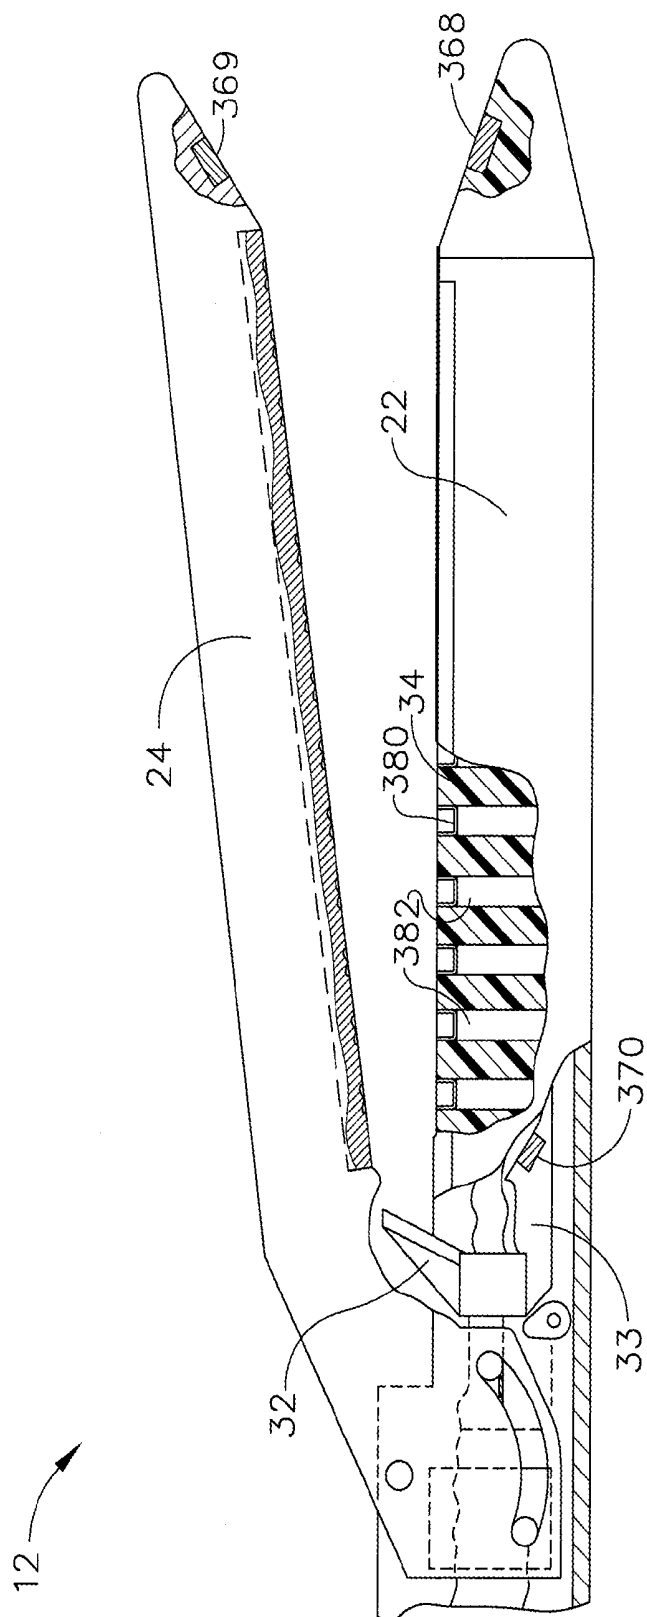


FIG. 15

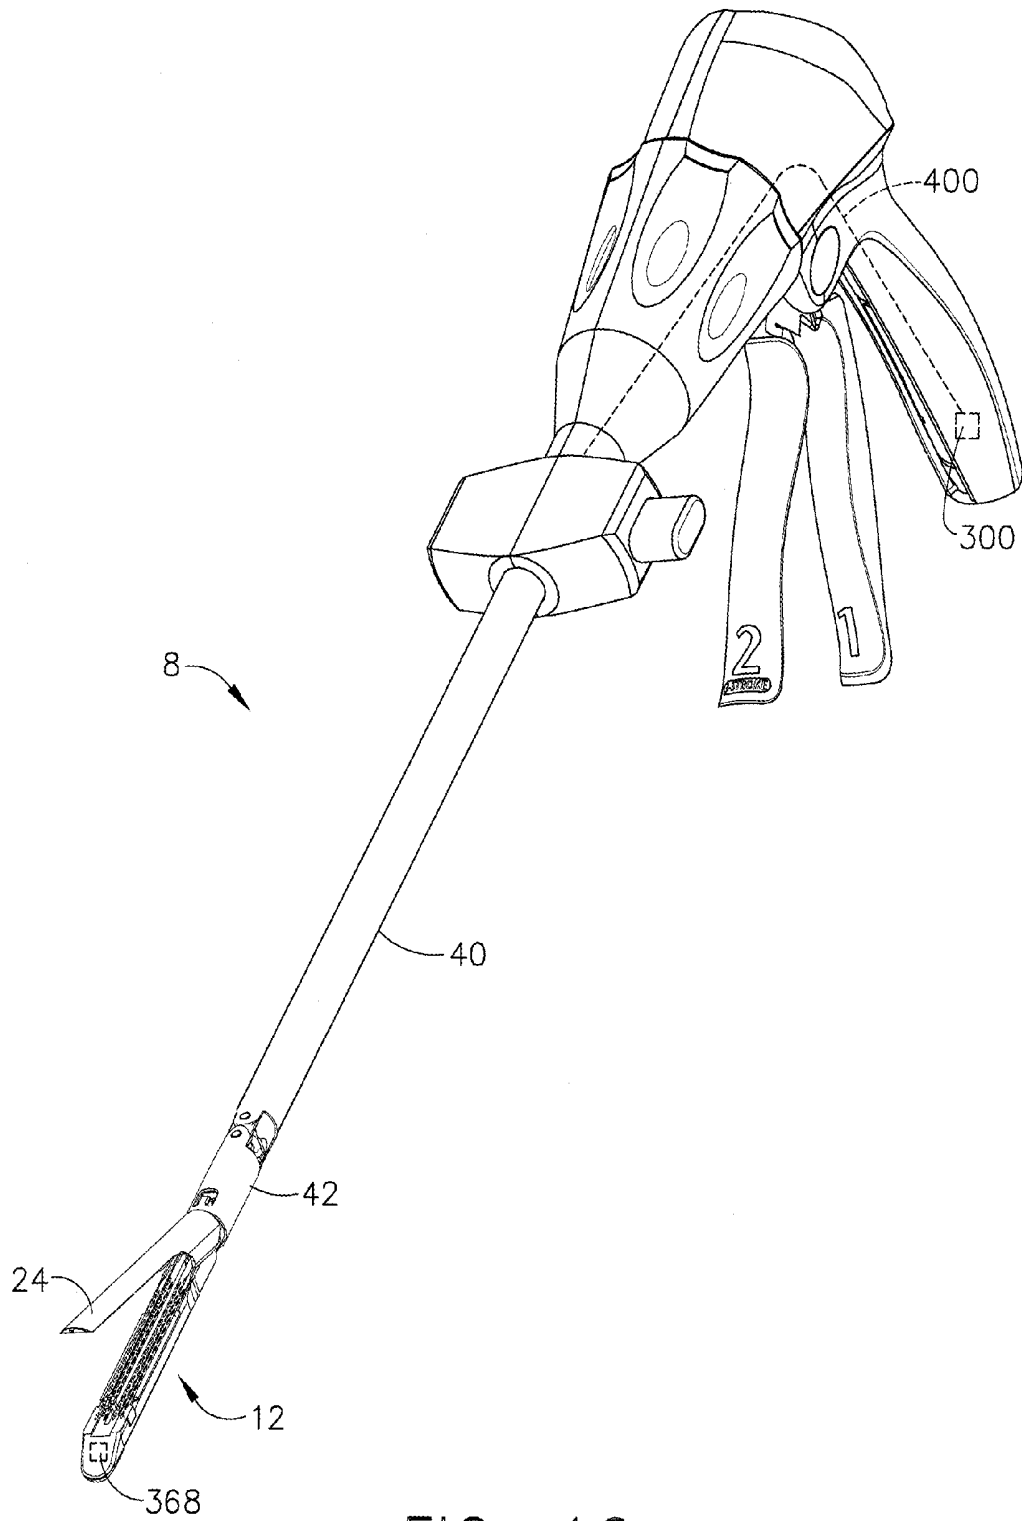


FIG. 16

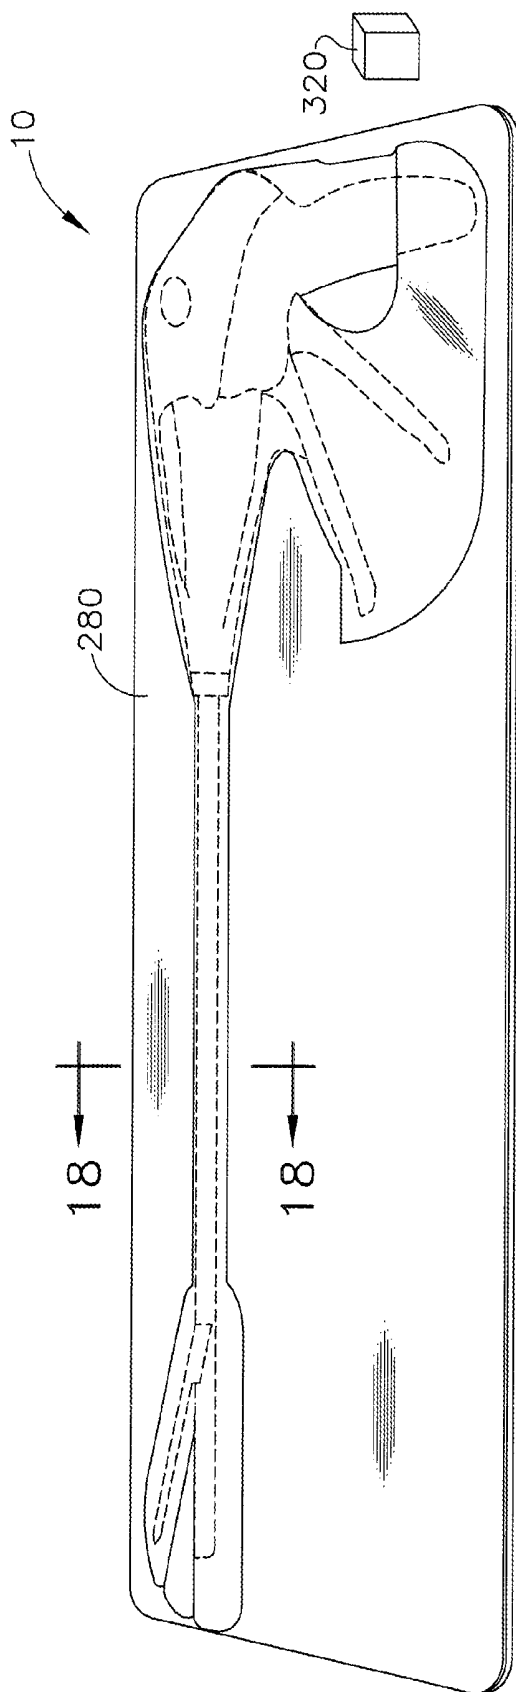


FIG. 17



FIG. 18

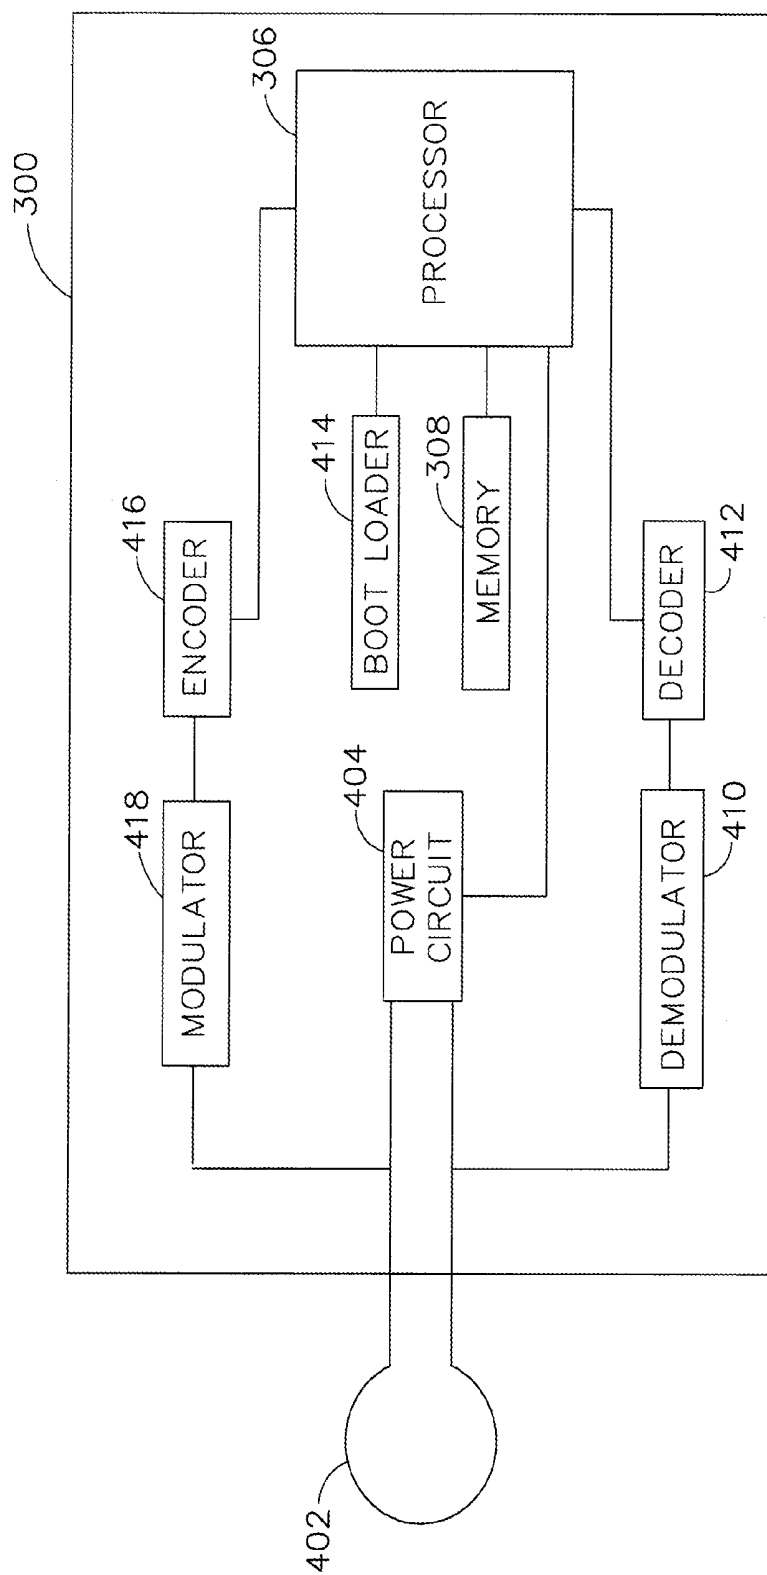


FIG. 19

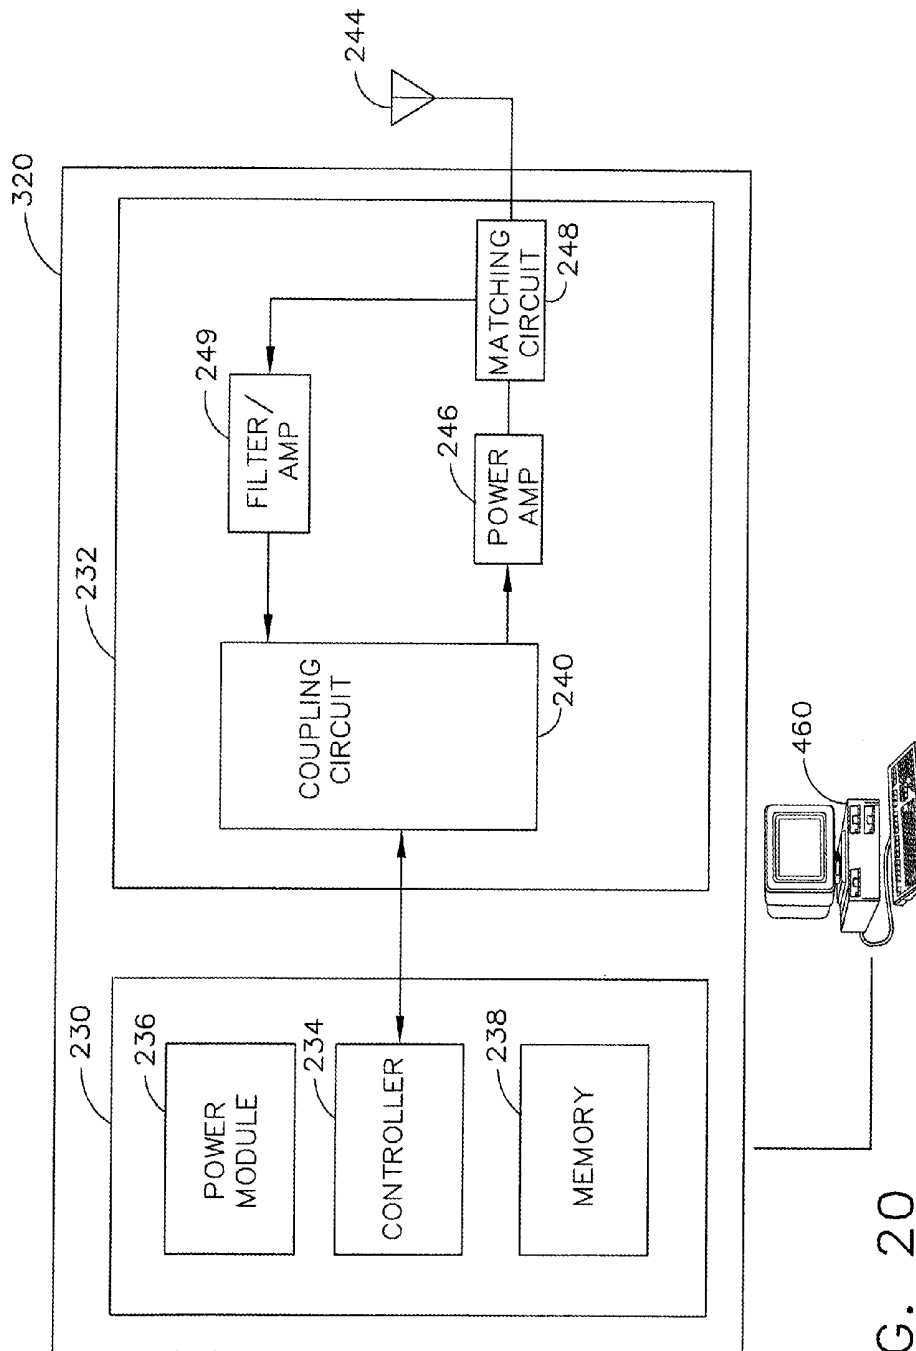


FIG. 20

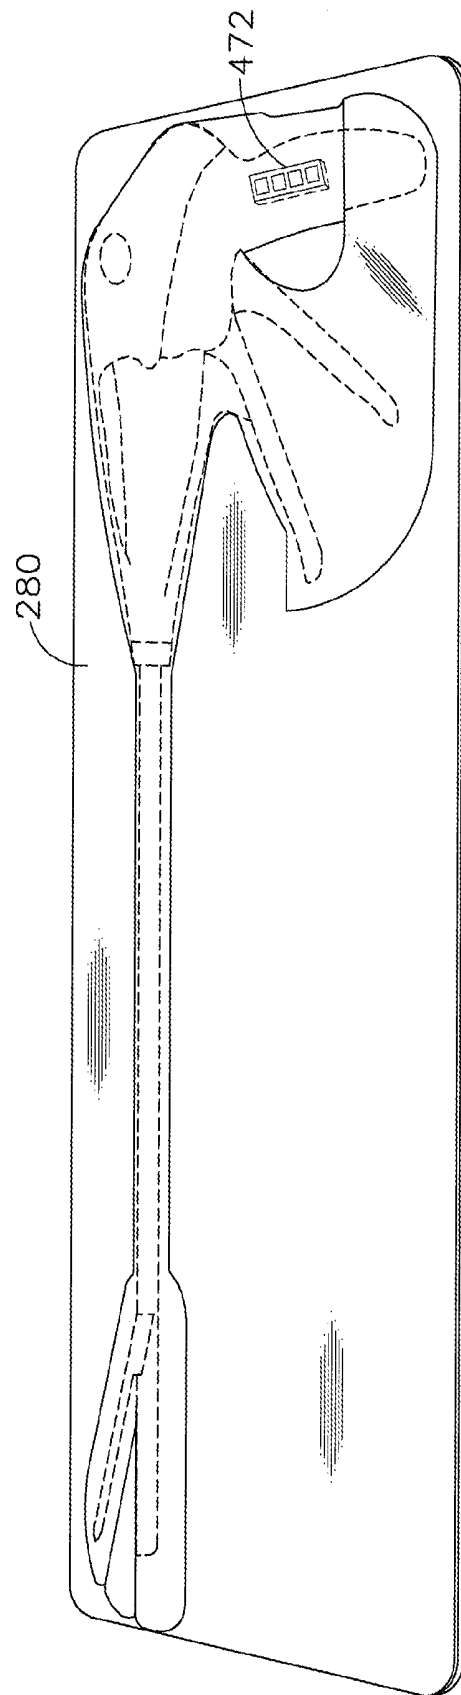


FIG. 21

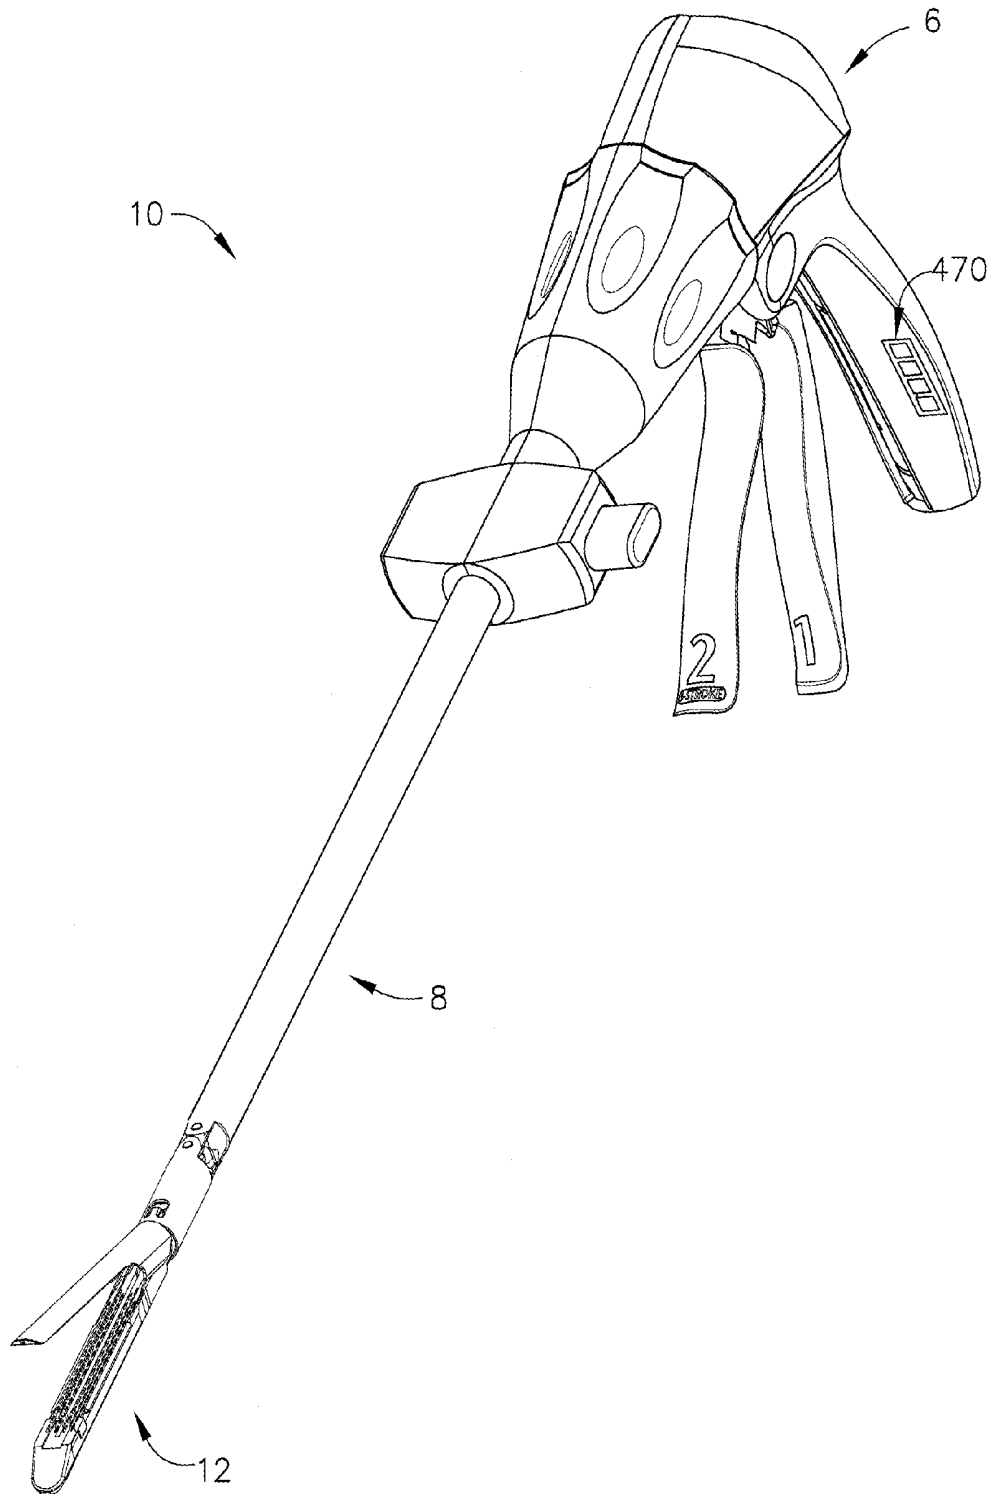


FIG. 22

SURGICAL INSTRUMENT WITH WIRELESS COMMUNICATION BETWEEN CONTROL UNIT AND REMOTE SENSOR

CROSS REFERENCE TO RELATED APPLICATIONS

The present application is related to the following, concurrently-filed U.S. patent applications, which are incorporated herein by reference:

(1) U.S. patent application Ser. No. 11/651,715, entitled "SURGICAL INSTRUMENT WITH WIRELESS COMMUNICATION BETWEEN CONTROL UNIT AND SENSOR TRANSPONDERS," by J. Giordano et al.;

(2) U.S. patent application Ser. No. 11/651,806, entitled "SURGICAL INSTRUMENT WITH ELEMENTS TO COMMUNICATE BETWEEN CONTROL UNIT AND END EFFECTOR," by J. Giordano et al.;

(3) U.S. patent application Ser. No. 11/651,768, entitled "PREVENTION OF CARTRIDGE REUSE IN A SURGICAL INSTRUMENT," by F. Shelton et al.;

(4) U.S. patent application Ser. No. 11/651,771, entitled "POST-STERILIZATION PROGRAMMING OF SURGICAL INSTRUMENTS," by J. Swayze et al.;

(5) U.S. patent application Ser. No. 11/651,788, entitled "INTERLOCK AND SURGICAL INSTRUMENT INCLUDING SAME," by F. Shelton et al.; and

(6) U.S. patent application Ser. No. 11/651,785, entitled "SURGICAL INSTRUMENT WITH ENHANCED BATTERY PERFORMANCE," by F. Shelton et al.

BACKGROUND

Endoscopic surgical instruments are often preferred over traditional open surgical devices since a smaller incision tends to reduce the post-operative recovery time and complications. Consequently, significant development has gone into a range of endoscopic surgical instruments that are suitable for precise placement of a distal end effector at a desired surgical site through a cannula of a trocar. These distal end effectors engage the tissue in a number of ways to achieve a diagnostic or therapeutic effect (e.g., endocutter, grasper, cutter, staplers, clip applier, access device, drug/gene therapy delivery device, and energy device using ultrasound, RF, laser, etc.).

Known surgical staplers include an end effector that simultaneously makes a longitudinal incision in tissue and applies lines of staples on opposing sides of the incision. The end effector includes a pair of cooperating jaw members that, if the instrument is intended for endoscopic or laparoscopic applications, are capable of passing through a cannula passageway. One of the jaw members receives a staple cartridge having at least two laterally spaced rows of staples. The other jaw member defines an anvil having staple-forming pockets aligned with the rows of staples in the cartridge. The instrument includes a plurality of reciprocating wedges which, when driven distally, pass through openings in the staple cartridge and engage drivers supporting the staples to effect the firing of the staples toward the anvil.

An example of a surgical stapler suitable for endoscopic applications is described in U.S. Pat. No. 5,465,895, which discloses an endocutter with distinct closing and firing actions. A clinician using this device is able to close the jaw members upon tissue to position the tissue prior to firing. Once the clinician has determined that the jaw members are properly gripping tissue, the clinician can then fire the surgical stapler with a single firing stroke, thereby severing and

stapling the tissue. The simultaneous severing and stapling avoids complications that may arise when performing such actions sequentially with different surgical tools that respectively only sever and staple.

One specific advantage of being able to close upon tissue before firing is that the clinician is able to verify via an endoscope that the desired location for the cut has been achieved, including that a sufficient amount of tissue has been captured between opposing jaws. Otherwise, opposing jaws may be drawn too close together, especially pinching at their distal ends, and thus not effectively forming closed staples in the severed tissue. At the other extreme, an excessive amount of clamped tissue may cause binding and an incomplete firing.

Endoscopic staplers/cutters continue to increase in complexity and function with each generation. One of the main reasons for this is the quest to lower force-to-fire (FTF) to a level that all or a great majority of surgeons can handle. One known solution to lower FTF is use CO₂ or electrical motors. These devices have not fared much better than traditional hand-powered devices, but for a different reason. Surgeons typically prefer to experience proportionate force distribution to that being experienced by the end effector in the forming of the staple to assure them that the cutting/stapling cycle is complete, with the upper limit within the capabilities of most surgeons (usually around 15-30 lbs). They also typically want to maintain control of deploying the staples and being able to stop at anytime if the forces felt in the handle of the device feel too great or for some other clinical reason.

To address this need, so-called "power-assist" endoscopic surgical instruments have been developed in which a supplemental power source aids in the firing of the instrument. For example, in some power-assist devices, a motor provides supplemental electrical power to the power input by the user from squeezing the firing trigger. Such devices are capable of providing loading force feedback and control to the operator to reduce the firing force required to be exerted by the operator in order to complete the cutting operation. One such power-assist device is described in U.S. patent application Ser. No. 11/343,573, filed Jan. 31, 2006 by Shelton et al., entitled "Motor-driven surgical cutting and fastening instrument with loading force feedback," ("the '573 application") which is incorporated herein by reference.

These power-assist devices often include other components that purely mechanical endoscopic surgical instruments do not, such as sensors and control systems. One challenge in using such electronics in a surgical instrument is delivering power and/or data to and from the sensors, particularly when there is a free rotating joint in the surgical instrument.

SUMMARY

In one general aspect, the present invention is directed to a surgical instrument, such as an endoscopic or laparoscopic instrument. According to one embodiment, the surgical instrument comprises an end effector comprising at least one sensor transponder that is passively powered. The surgical instrument also comprises a shaft having a distal end connected to the end effector and a handle connected to a proximate end of the shaft. The handle comprises a control unit (e.g., a microcontroller) that is in communication with the sensor transponder via at least one inductive coupling. Further, the surgical instrument may comprise a rotational joint for rotating the shaft. In such a case, the surgical instrument may comprise a first inductive element located in the shaft distally from the rotational joint and inductively coupled to the control unit, and a second inductive element located dis-

tally in the shaft and inductively coupled to the at least one sensor transponder. The first and second inductive elements may be connected by a wired, physical connection.

That way, the control unit may communicate with the transponder in the end effector without a direct wired connection through complex mechanical joints like the rotating joint where it may be difficult to maintain such a wired connection. In addition, because the distances between the inductive elements may be fixed and known, the couplings could be optimized for inductive transfer of energy. Also, the distances could be relatively short so that relatively low power signals could be used to thereby minimize interference with other systems in the use environment of the instrument.

In another general aspect of the present invention, the electrically conductive shaft of the surgical instrument may serve as an antenna for the control unit to wirelessly communicate signals to and from the sensor transponder. For example, the sensor transponder could be located on or disposed in a nonconductive component of the end effector, such as a plastic cartridge, thereby insulating the sensor from conductive components of the end effector and the shaft. In addition, the control unit in the handle may be electrically coupled to the shaft. In that way, the shaft and/or the end effector may serve as an antenna for the control unit by radiating signals from the control unit to the sensor and/or by receiving radiated signals from the sensor. Such a design is particularly useful in surgical instruments having complex mechanical joints (such as rotary joints), which make it difficult to use a direct wired connection between the sensor and control unit for communicating data signals.

In another embodiment, the shaft and/or components of the end effector could serve as the antenna for the sensor by radiating signals to the control unit and receiving radiated signals from the control unit. According to such an embodiment, the control unit is electrically insulated from the shaft and the end effector.

In another general aspect, the present invention is directed to a surgical instrument comprising a programmable control unit that can be programmed by a programming device after the instrument has been packaged and sterilized. In one such embodiment, the programming device may wirelessly program the control unit. The control unit may be passively powered by the wireless signals from the programming device during the programming operation. In another embodiment, the sterile container may comprise a connection interface so that the programming unit can be connected to the surgical instrument while the surgical instrument is in its sterilized container.

FIGURES

Various embodiments of the present invention are described herein by way of example in conjunction with the following figures wherein:

FIGS. 1 and 2 are perspective views of a surgical instrument according to various embodiments of the present invention;

FIGS. 3-5 are exploded views of an end effector and shaft of the instrument according to various embodiments of the present invention;

FIG. 6 is a side view of the end effector according to various embodiments of the present invention;

FIG. 7 is an exploded view of the handle of the instrument according to various embodiments of the present invention;

FIGS. 8 and 9 are partial perspective views of the handle according to various embodiments of the present invention;

FIG. 10 is a side view of the handle according to various embodiments of the present invention;

FIGS. 11, 13-14, 16, and 22 are perspective views of a surgical instrument according to various embodiments of the present invention;

FIGS. 12 and 19 are block diagrams of a control unit according to various embodiments of the present invention;

FIG. 15 is a side view of an end effector including a sensor transponder according to various embodiments of the present invention;

FIGS. 17 and 18 show the instrument in a sterile container according to various embodiments of the present invention;

FIG. 20 is a block diagram of the remote programming device according to various embodiments of the present invention; and

FIG. 21 is a diagram of a packaged instrument according to various embodiments of the present invention.

DETAILED DESCRIPTION

Various embodiments of the present invention are directed generally to a surgical instrument having at least one remote sensor transponder and means for communicating power and/or data signals to the transponder(s) from a control unit. The present invention may be used with any type of surgical instrument comprising at least one sensor transponder, such as endoscopic or laparoscopic surgical instruments, but is particularly useful for surgical instruments where some feature of the instrument, such as a free rotating joint, prevents or otherwise inhibits the use of a wired connection to the sensor(s). Before describing aspects of the system, one type of surgical instrument in which embodiments of the present invention may be used—an endoscopic stapling and cutting instrument (i.e., an endocutter)—is first described by way of illustration.

FIGS. 1 and 2 depict an endoscopic surgical instrument 10 that comprises a handle 6, a shaft 8, and an articulating end effector 12 pivotally connected to the shaft 8 at an articulation pivot 14. Correct placement and orientation of the end effector 12 may be facilitated by controls on the handle 6, including (1) a rotation knob 28 for rotating the closure tube (described in more detail below in connection with FIGS. 4-5) at a free rotating joint 29 of the shaft 8 to thereby rotate the end effector 12 and (2) an articulation control 16 to effect rotational articulation of the end effector 12 about the articulation pivot 14. In the illustrated embodiment, the end effector 12 is configured to act as an endocutter for clamping, severing and stapling tissue, although in other embodiments, different types of end effectors may be used, such as end effectors for other types of surgical instruments, such as graspers, cutters, staplers, clip appliers, access devices, drug/gene therapy devices, ultrasound, RF or laser devices, etc.

The handle 6 of the instrument 10 may include a closure trigger 18 and a firing trigger 20 for actuating the end effector 12. It will be appreciated that instruments having end effectors directed to different surgical tasks may have different numbers or types of triggers or other suitable controls for operating the end effector 12. The end effector 12 is shown separated from the handle 6 by the preferably elongate shaft 8. In one embodiment, a clinician or operator of the instrument 10 may articulate the end effector 12 relative to the shaft 8 by utilizing the articulation control 16, as described in more detail in pending U.S. patent application Ser. No. 11/329,020, filed Jan. 10, 2006, entitled "Surgical Instrument Having An Articulating End Effector," by Geoffrey C. Hueil et al., which is incorporated herein by reference.

The end effector 12 includes in this example, among other things, a staple channel 22 and a pivotally translatable clamping member, such as an anvil 24, which are maintained at a spacing that assures effective stapling and severing of tissue clamped in the end effector 12. The handle 6 includes a pistol grip 26 towards which a closure trigger 18 is pivotally drawn by the clinician to cause clamping or closing of the anvil 24 toward the staple channel 22 of the end effector 12 to thereby clamp tissue positioned between the anvil 24 and channel 22. The firing trigger 20 is farther outboard of the closure trigger 18. Once the closure trigger 18 is locked in the closure position, the firing trigger 20 may rotate slightly toward the pistol grip 26 so that it can be reached by the operator using one hand. Then the operator may pivotally draw the firing trigger 20 toward the pistol grip 12 to cause the stapling and severing of clamped tissue in the end effector 12. The '573 application describes various configurations for locking and unlocking the closure trigger 18. In other embodiments, different types of clamping members besides the anvil 24 could be used, such as, for example, an opposing jaw, etc.

It will be appreciated that the terms "proximal" and "distal" are used herein with reference to a clinician gripping the handle 6 of an instrument 10. Thus, the end effector 12 is distal with respect to the more proximal handle 6. It will be further appreciated that, for convenience and clarity, spatial terms such as "vertical" and "horizontal" are used herein with respect to the drawings. However, surgical instruments are used in many orientations and positions, and these terms are not intended to be limiting and absolute.

The closure trigger 18 may be actuated first. Once the clinician is satisfied with the positioning of the end effector 12, the clinician may draw back the closure trigger 18 to its fully closed, locked position proximate to the pistol grip 26. The firing trigger 20 may then be actuated. The firing trigger 20 returns to the open position (shown in FIGS. 1 and 2) when the clinician removes pressure. A release button 30 on the handle 6, and in this example, on the pistol grip 26 of the handle, when depressed may release the locked closure trigger 18.

FIG. 3 is an exploded view of the end effector 12 according to various embodiments. As shown in the illustrated embodiment, the end effector 12 may include, in addition to the previously-mentioned channel 22 and anvil 24, a cutting instrument 32, a sled 33, a staple cartridge 34 that is removably seated in the channel 22, and a helical screw shaft 36. The cutting instrument 32 may be, for example, a knife. The anvil 24 may be pivotally opened and closed at a pivot point 25 connected to the proximate end of the channel 22. The anvil 24 may also include a tab 27 at its proximate end that is inserted into a component of the mechanical closure system (described further below) to open and close the anvil 24. When the closure trigger 18 is actuated, that is, drawn in by a user of the instrument 10, the anvil 24 may pivot about the pivot point 25 into the clamped or closed position. If clamping of the end effector 12 is satisfactory, the operator may actuate the firing trigger 20, which, as explained in more detail below, causes the knife 32 and sled 33 to travel longitudinally along the channel 22, thereby cutting tissue clamped within the end effector 12. The movement of the sled 33 along the channel 22 causes the staples of the staple cartridge 34 to be driven through the severed tissue and against the closed anvil 24, which turns the staples to fasten the severed tissue. U.S. Pat. No. 6,978,921, entitled "Surgical stapling instrument incorporating an E-beam firing mechanism," which is incorporated herein by reference, provides more details about such two-stroke cutting and fastening instruments. The sled 33 may be part of the cartridge 34, such that when the knife 32 retracts

following the cutting operation, the sled 33 does not retract. The channel 22 and the anvil 24 may be made of an electrically conductive material (such as metal) so that they may serve as part of the antenna that communicates with the sensor(s) in the end effector, as described further below. The cartridge 34 could be made of a nonconductive material (such as plastic) and the sensor may be connected to or disposed in the cartridge 34, as described further below.

It should be noted that although the embodiments of the instrument 10 described herein employ an end effector 12 that staples the severed tissue, in other embodiments different techniques for fastening or sealing the severed tissue may be used. For example, end effectors that use RF energy or adhesives to fasten the severed tissue may also be used. U.S. Pat. No. 5,709,680, entitled "Electrosurgical Hemostatic Device" to Yates et al., and U.S. Pat. No. 5,688,270, entitled "Electrosurgical Hemostatic Device With Recessed And/Or Offset Electrodes" to Yates et al., which are incorporated herein by reference, discloses cutting instruments that use RF energy to fasten the severed tissue. U.S. patent application Ser. No. 11/267,811 to Morgan et al. and U.S. patent application Ser. No. 11/267,383 to Shelton et al., which are also incorporated herein by reference, disclose cutting instruments that use adhesives to fasten the severed tissue. Accordingly, although the description herein refers to cutting/stapling operations and the like, it should be recognized that this is an exemplary embodiment and is not meant to be limiting. Other tissue-fastening techniques may also be used.

FIGS. 4 and 5 are exploded views and FIG. 6 is a side view of the end effector 12 and shaft 8 according to various embodiments. As shown in the illustrated embodiment, the shaft 8 may include a proximate closure tube 40 and a distal closure tube 42 pivotably linked by a pivot links 44. The distal closure tube 42 includes an opening 45 into which the tab 27 on the anvil 24 is inserted in order to open and close the anvil 24. Disposed inside the closure tubes 40, 42 may be a proximate spine tube 46. Disposed inside the proximate spine tube 46 may be a main rotational (or proximate) drive shaft 48 that communicates with a secondary (or distal) drive shaft 50 via a bevel gear assembly 52. The secondary drive shaft 50 is connected to a drive gear 54 that engages a proximate drive gear 56 of the helical screw shaft 36. The vertical bevel gear 52b may sit and pivot in an opening 57 in the distal end of the proximate spine tube 46. A distal spine tube 58 may be used to enclose the secondary drive shaft 50 and the drive gears 54, 56. Collectively, the main drive shaft 48, the secondary drive shaft 50, and the articulation assembly (e.g., the bevel gear assembly 52a-c), are sometimes referred to herein as the "main drive shaft assembly." The closure tubes 40, 42 may be made of electrically conductive material (such as metal) so that they may serve as part of the antenna, as described further below. Components of the main drive shaft assembly (e.g., the drive shafts 48, 50) may be made of a nonconductive material (such as plastic).

A bearing 38, positioned at a distal end of the staple channel 22, receives the helical drive screw 36, allowing the helical drive screw 36 to freely rotate with respect to the channel 22. The helical screw shaft 36 may interface a threaded opening (not shown) of the knife 32 such that rotation of the shaft 36 causes the knife 32 to translate distally or proximally (depending on the direction of the rotation) through the staple channel 22. Accordingly, when the main drive shaft 48 is caused to rotate by actuation of the firing trigger 20 (as explained in more detail below), the bevel gear assembly 52a-c causes the secondary drive shaft 50 to rotate, which in turn, because of the engagement of the drive gears 54, 56, causes the helical screw shaft 36 to rotate, which causes the

knife 32 to travel longitudinally along the channel 22 to cut any tissue clamped within the end effector. The sled 33 may be made of, for example, plastic, and may have a sloped distal surface. As the sled 33 traverses the channel 22, the sloped forward surface may push up or drive the staples in the staple cartridge 34 through the clamped tissue and against the anvil 24. The anvil 24 turns the staples, thereby stapling the severed tissue. When the knife 32 is retracted, the knife 32 and sled 33 may become disengaged, thereby leaving the sled 33 at the distal end of the channel 22.

According to various embodiments, as shown FIGS. 7-10, the surgical instrument may include a battery 64 in the handle 6. The illustrated embodiment provides user-feedback regarding the deployment and loading force of the cutting instrument in the end effector 12. In addition, the embodiment may use power provided by the user in retracting the firing trigger 18 to power the instrument 10 (a so-called "power assist" mode). As shown in the illustrated embodiment, the handle 6 includes exterior lower side pieces 59, 60 and exterior upper side pieces 61, 62 that fit together to form, in general, the exterior of the handle 6. The handle pieces 59-62 may be made of an electrically nonconductive material, such as plastic. A battery 64 may be provided in the pistol grip portion 26 of the handle 6. The battery 64 powers a motor 65 disposed in an upper portion of the pistol grip portion 26 of the handle 6. The battery 64 may be constructed according to any suitable construction or chemistry including, for example, a Li-ion chemistry such as LiCoO₂ or LiNiO₂, a Nickel Metal Hydride chemistry, etc. According to various embodiments, the motor 65 may be a DC brushed driving motor having a maximum rotation of, approximately, 5000 RPM to 100,000 RPM. The motor 64 may drive a 90° bevel gear assembly 66 comprising a first bevel gear 68 and a second bevel gear 70. The bevel gear assembly 66 may drive a planetary gear assembly 72. The planetary gear assembly 72 may include a pinion gear 74 connected to a drive shaft 76. The pinion gear 74 may drive a mating ring gear 78 that drives a helical gear drum 80 via a drive shaft 82. A ring 84 may be threaded on the helical gear drum 80. Thus, when the motor 65 rotates, the ring 84 is caused to travel along the helical gear drum 80 by means of the interposed bevel gear assembly 66, planetary gear assembly 72 and ring gear 78.

The handle 6 may also include a run motor sensor 110 in communication with the firing trigger 20 to detect when the firing trigger 20 has been drawn in (or "closed") toward the pistol grip portion 26 of the handle 6 by the operator to thereby actuate the cutting/stapling operation by the end effector 12. The sensor 110 may be a proportional sensor such as, for example, a rheostat or variable resistor. When the firing trigger 20 is drawn in, the sensor 110 detects the movement, and sends an electrical signal indicative of the voltage (or power) to be supplied to the motor 65. When the sensor 110 is a variable resistor or the like, the rotation of the motor 65 may be generally proportional to the amount of movement of the firing trigger 20. That is, if the operator only draws or closes the firing trigger 20 in a little bit, the rotation of the motor 65 is relatively low. When the firing trigger 20 is fully drawn in (or in the fully closed position), the rotation of the motor 65 is at its maximum. In other words, the harder the user pulls on the firing trigger 20, the more voltage is applied to the motor 65, causing greater rates of rotation. In another embodiment, for example, the control unit (described further below) may output a PWM control signal to the motor 65 based on the input from the sensor 110 in order to control the motor 65.

The handle 6 may include a middle handle piece 104 adjacent to the upper portion of the firing trigger 20. The handle 6 also may comprise a bias spring 112 connected between posts

on the middle handle piece 104 and the firing trigger 20. The bias spring 112 may bias the firing trigger 20 to its fully open position. In that way, when the operator releases the firing trigger 20, the bias spring 112 will pull the firing trigger 20 to its open position, thereby removing actuation of the sensor 110, thereby stopping rotation of the motor 65. Moreover, by virtue of the bias spring 112, any time a user closes the firing trigger 20, the user will experience resistance to the closing operation, thereby providing the user with feedback as to the amount of rotation exerted by the motor 65. Further, the operator could stop retracting the firing trigger 20 to thereby remove force from the sensor 100, to thereby stop the motor 65. As such, the user may stop the deployment of the end effector 12, thereby providing a measure of control of the cutting/fastening operation to the operator.

The distal end of the helical gear drum 80 includes a distal drive shaft 120 that drives a ring gear 122, which mates with a pinion gear 124. The pinion gear 124 is connected to the main drive shaft 48 of the main drive shaft assembly. In that way, rotation of the motor 65 causes the main drive shaft assembly to rotate, which causes actuation of the end effector 12, as described above.

The ring 84 threaded on the helical gear drum 80 may include a post 86 that is disposed within a slot 88 of a slotted arm 90. The slotted arm 90 has an opening 92 at its opposite end 94 that receives a pivot pin 96 that is connected between the handle exterior side pieces 59, 60. The pivot pin 96 is also disposed through an opening 100 in the firing trigger 20 and an opening 102 in the middle handle piece 104.

In addition, the handle 6 may include a reverse motor (or end-of-stroke sensor) 130 and a stop motor (or beginning-of-stroke) sensor 142. In various embodiments, the reverse motor sensor 130 may be a limit switch located at the distal end of the helical gear drum 80 such that the ring 84 threaded on the helical gear drum 80 contacts and trips the reverse motor sensor 130 when the ring 84 reaches the distal end of the helical gear drum 80. The reverse motor sensor 130, when activated, sends a signal to the control unit which sends a signal to the motor 65 to reverse its rotation direction, thereby withdrawing the knife 32 of the end effector 12 following the cutting operation.

The stop motor sensor 142 may be, for example, a normally-closed limit switch. In various embodiments, it may be located at the proximate end of the helical gear drum 80 so that the ring 84 trips the switch 142 when the ring 84 reaches the proximate end of the helical gear drum 80.

In operation, when an operator of the instrument 10 pulls back the firing trigger 20, the sensor 110 detects the deployment of the firing trigger 20 and sends a signal to the control unit which sends a signal to the motor 65 to cause forward rotation of the motor 65 at, for example, a rate proportional to how hard the operator pulls back the firing trigger 20. The forward rotation of the motor 65 in turn causes the ring gear 78 at the distal end of the planetary gear assembly 72 to rotate, thereby causing the helical gear drum 80 to rotate, causing the ring 84 threaded on the helical gear drum 80 to travel distally along the helical gear drum 80. The rotation of the helical gear drum 80 also drives the main drive shaft assembly as described above, which in turn causes deployment of the knife 32 in the end effector 12. That is, the knife 32 and sled 33 are caused to traverse the channel 22 longitudinally, thereby cutting tissue clamped in the end effector 12. Also, the stapling operation of the end effector 12 is caused to happen in embodiments where a stapling-type end effector is used.

By the time the cutting/stapling operation of the end effector 12 is complete, the ring 84 on the helical gear drum 80 will

have reached the distal end of the helical gear drum 80, thereby causing the reverse motor sensor 130 to be tripped, which sends a signal to the control unit which sends a signal to the motor 65 to cause the motor 65 to reverse its rotation. This in turn causes the knife 32 to retract, and also causes the ring 84 on the helical gear drum 80 to move back to the proximate end of the helical gear drum 80.

The middle handle piece 104 includes a backside shoulder 106 that engages the slotted arm 90 as best shown in FIGS. 8 and 9. The middle handle piece 104 also has a forward motion stop 107 that engages the firing trigger 20. The movement of the slotted arm 90 is controlled, as explained above, by rotation of the motor 65. When the slotted arm 90 rotates CCW as the ring 84 travels from the proximate end of the helical gear drum 80 to the distal end, the middle handle piece 104 will be free to rotate CCW. Thus, as the user draws in the firing trigger 20, the firing trigger 20 will engage the forward motion stop 107 of the middle handle piece 104, causing the middle handle piece 104 to rotate CCW. Due to the backside shoulder 106 engaging the slotted arm 90, however, the middle handle piece 104 will only be able to rotate CCW as far as the slotted arm 90 permits. In that way, if the motor 65 should stop rotating for some reason, the slotted arm 90 will stop rotating, and the user will not be able to further draw in the firing trigger 20 because the middle handle piece 104 will not be free to rotate CCW due to the slotted arm 90.

Components of an exemplary closure system for closing (or clamping) the anvil 24 of the end effector 12 by retracting the closure trigger 18 are also shown in FIGS. 7-10. In the illustrated embodiment, the closure system includes a yoke 250 connected to the closure trigger 18 by a pin 251 that is inserted through aligned openings in both the closure trigger 18 and the yoke 250. A pivot pin 252, about which the closure trigger 18 pivots, is inserted through another opening in the closure trigger 18 which is offset from where the pin 251 is inserted through the closure trigger 18. Thus, retraction of the closure trigger 18 causes the upper part of the closure trigger 18, to which the yoke 250 is attached via the pin 251, to rotate CCW. The distal end of the yoke 250 is connected, via a pin 254, to a first closure bracket 256. The first closure bracket 256 connects to a second closure bracket 258. Collectively, the closure brackets 256, 258 define an opening in which the proximate end of the proximate closure tube 40 (see FIG. 4) is seated and held such that longitudinal movement of the closure brackets 256, 258 causes longitudinal motion by the proximate closure tube 40. The instrument 10 also includes a closure rod 260 disposed inside the proximate closure tube 40. The closure rod 260 may include a window 261 into which a post 263 on one of the handle exterior pieces, such as exterior lower side piece 59 in the illustrated embodiment, is disposed to fixedly connect the closure rod 260 to the handle 6. In that way, the proximate closure tube 40 is capable of moving longitudinally relative to the closure rod 260. The closure rod 260 may also include a distal collar 267 that fits into a cavity 269 in proximate spine tube 46 and is retained therein by a cap 271 (see FIG. 4).

In operation, when the yoke 250 rotates due to retraction of the closure trigger 18, the closure brackets 256, 258 cause the proximate closure tube 40 to move distally (i.e., away from the handle end of the instrument 10), which causes the distal closure tube 42 to move distally, which causes the anvil 24 to rotate about the pivot point 25 into the clamped or closed position. When the closure trigger 18 is unlocked from the locked position, the proximate closure tube 40 is caused to slide proximally, which causes the distal closure tube 42 to slide proximally, which, by virtue of the tab 27 being inserted in the window 45 of the distal closure tube 42, causes

the anvil 24 to pivot about the pivot point 25 into the open or unclamped position. In that way, by retracting and locking the closure trigger 18, an operator may clamp tissue between the anvil 24 and channel 22, and may unclamp the tissue following the cutting/stapling operation by unlocking the closure trigger 18 from the locked position.

The control unit (described further below) may receive the outputs from end-of-stroke and beginning-of-stroke sensors 130, 142 and the run-motor sensor 110, and may control the motor 65 based on the inputs. For example, when an operator initially pulls the firing trigger 20 after locking the closure trigger 18, the run-motor sensor 110 is actuated. If the staple cartridge 34 is present in the end effector 12, a cartridge lockout sensor (not shown) may be closed, in which case the control unit may output a control signal to the motor 65 to cause the motor 65 to rotate in the forward direction. When the end effector 12 reaches the end of its stroke, the reverse motor sensor 130 will be activated. The control unit may receive this output from the reverse motor sensor 130 and cause the motor 65 to reverse its rotational direction. When the knife 32 is fully retracted, the stop motor sensor switch 142 is activated, causing the control unit to stop the motor 65.

In other embodiments, rather than a proportional-type sensor 110, an on-off type sensor could be used. In such embodiments, the rate of rotation of the motor 65 would not be proportional to the force applied by the operator. Rather, the motor 65 would generally rotate at a constant rate. But the operator would still experience force feedback because the firing trigger 20 is geared into the gear drive train.

The instrument 10 may include a number of sensor transponders in the end effector 12 for sensing various conditions related to the end effector 12, such as sensor transponders for determining the status of the staple cartridge 34 (or other type of cartridge depending on the type of surgical instrument), the progress of the stapler during closure and firing, etc. The sensor transponders may be passively powered by inductive signals, as described further below, although in other embodiments the transponders could be powered by a remote power source, such as a battery in the end effector 12, for example. The sensor transponder(s) could include magnetoresistive, optical, electromechanical, RFID, MEMS, motion or pressure sensors, for example. These sensor transponders may be in communication with a control unit 300, which may be housed in the handle 6 of the instrument 10, for example, as shown in FIG. 11.

As shown in FIG. 12, according to various embodiments the control unit 300 may comprise a processor 306 and one or more memory units 308. By executing instruction code stored in the memory 308, the processor 306 may control various components of the instrument 10, such as the motor 65 or a user display (not shown), based on inputs received from the various end effector sensor transponders and other sensor(s) (such as the run-motor sensor 110, the end-of-stroke sensor 130, and the beginning-of-stroke sensor 142, for example). The control unit 300 may be powered by the battery 64 during surgical use of instrument 10. The control unit 300 may comprise an inductive element 302 (e.g., a coil or antenna) to pick up wireless signals from the sensor transponders, as described in more detail below. Input signals received by the inductive element 302 acting as a receiving antenna may be demodulated by a demodulator 310 and decoded by a decoder 312. The input signals may comprise data from the sensor transponders in the end effector 12, which the processor 306 may use to control various aspects of the instrument 10.

To transmit signals to the sensor transponders, the control unit 300 may comprise an encoder 316 for encoding the signals and a modulator 318 for modulating the signals

according to the modulation scheme. The inductive element **302** may act as the transmitting antenna. The control unit **300** may communicate with the sensor transponders using any suitable wireless communication protocol and any suitable frequency (e.g., an ISM band). Also, the control unit **300** may transmit signals at a different frequency range than the frequency range of the received signals from the sensor transponders. Also, although only one antenna (inductive element **302**) is shown in FIG. **12**, in other embodiments the control unit **300** may have separate receiving and transmitting antennas.

According to various embodiments, the control unit **300** may comprise a microcontroller, a microprocessor, a field programmable gate array (FPGA), one or more other types of integrated circuits (e.g., RF receivers and PWM controllers), and/or discrete passive components. The control units may also be embodied as system-on-chip (SoC) or a system-in-package (SIP), for example.

As shown in FIG. **11**, the control unit **300** may be housed in the handle **6** of the instrument **10** and one or more of the sensor transponders **368** for the instrument **10** may be located in the end effector **12**. To deliver power and/or transmit data to or from the sensor transponders **368** in the end effector **12**, the inductive element **302** of the control unit **300** may be inductively coupled to a secondary inductive element (e.g., a coil) **320** positioned in the shaft **8** distally from the rotation joint **29**. The secondary inductive element **320** is preferably electrically insulated from the conductive shaft **8**.

The secondary inductive element **320** may be connected by an electrically conductive, insulated wire **322** to a distal inductive element (e.g., a coil) **324** located near the end effector **12**, and preferably distally relative to the articulation pivot **14**. The wire **322** may be made of an electrically conductive polymer and/or metal (e.g., copper) and may be sufficiently flexible so that it could pass through the articulation pivot **14** and not be damaged by articulation. The distal inductive element **324** may be inductively coupled to the sensor transponder **368** in, for example, the cartridge **34** of the end effector **12**. The transponder **368**, as described in more detail below, may include an antenna (or coil) for inductive coupling to the distal coil **324**, a sensor and integrated control electronics for receiving and transmitting wireless communication signals.

The transponder **368** may use a portion of the power of the inductive signal received from the distal inductive element **326** to passively power the transponder **368**. Once sufficiently powered by the inductive signals, the transponder **368** may receive and transmit data to the control unit **300** in the handle **6** via (i) the inductive coupling between the transponder **368** and the distal inductive element **324**, (ii) the wire **322**, and (iii) the inductive coupling between the secondary inductive element **320** and the control unit **300**. That way, the control unit **300** may communicate with the transponder **368** in the end effector **12** without a direct wired connection through complex mechanical joints like the rotating joint **29** and/or without a direct wired connection from the shaft **8** to the end effector **12**, places where it may be difficult to maintain such a wired connection. In addition, because the distances between the inductive elements (e.g., the spacing between (i) the transponder **368** and the distal inductive element **324**, and (ii) the secondary inductive element **320** and the control unit **300**) are fixed and known, the couplings could be optimized for inductive transfer of energy. Also, the distances could be relatively short so that relatively low power signals could be used to thereby minimize interference with other systems in the use environment of the instrument **10**.

In the embodiment of FIG. **12**, the inductive element **302** of the control unit **300** is located relatively near to the control unit **300**. According to other embodiments, as shown in FIG. **13**, the inductive element **302** of the control unit **300** may be positioned closer to the rotating joint **29** so that it is closer to the secondary inductive element **320**, thereby reducing the distance of the inductive coupling in such an embodiment. Alternatively, the control unit **300** (and hence the inductive element **302**) could be positioned closer to the secondary inductive element **320** to reduce the spacing.

In other embodiments, more or fewer than two inductive couplings may be used. For example, in some embodiments, the surgical instrument **10** may use a single inductive coupling between the control unit **300** in the handle **6** and the transponder **368** in the end effector **12**, thereby eliminating the inductive elements **320**, **324** and the wire **322**. Of course, in such an embodiment, a stronger signal may be required due to the greater distance between the control unit **300** in the handle **6** and the transponder **368** in the end effector **12**. Also, more than two inductive couplings could be used. For example, if the surgical instrument **10** had numerous complex mechanical joints where it would be difficult to maintain a direct wired connection, inductive couplings could be used to span each such joint. For example, inductive couplers could be used on both sides of the rotary joint **29** and both sides of the articulation pivot **14**, with the inductive element **321** on the distal side of the rotary joint **29** connected by a wire **322** to the inductive element **324** of the proximate side of the articulation pivot, and a wire **323** connecting the inductive elements **325**, **326** on the distal side of the articulation pivot **14** as shown in FIG. **14**. In this embodiment, the inductive element **326** may communicate with the sensor transponder **368**.

In addition, the transponder **368** may include a number of different sensors. For example, it may include an array of sensors. Further, the end effector **12** could include a number of sensor transponders **368** in communication with the distal inductive element **324** (and hence the control unit **300**). Also, the inductive elements **320**, **324** may or may not include ferrite cores. As mentioned before, they are also preferably insulated from the electrically conductive outer shaft (or frame) of the instrument **10** (e.g., the closure tubes **40**, **42**), and the wire **322** is also preferably insulated from the outer shaft **8**.

FIG. **15** is a diagram of an end effector **12** including a transponder **368** held or embedded in the cartridge **34** at the distal end of the channel **22**. The transponder **368** may be connected to the cartridge **34** by a suitable bonding material, such as epoxy. In this embodiment, the transponder **368** includes a magnetoresistive sensor. The anvil **24** also includes a permanent magnet **369** at its distal end and generally facing the transponder **368**. The end effector **12** also includes a permanent magnet **370** connected to the sled **33** in this example embodiment. This allows the transponder **368** to detect both opening/closing of the end effector **12** (due to the permanent magnet **369** moving further or closer to the transponder as the anvil **24** opens and closes) and completion of the stapling/cutting operation (due to the permanent magnet **370** moving toward the transponder **368** as the sled **33** traverses the channel **22** as part of the cutting operation).

FIG. **15** also shows the staples **380** and the staple drivers **382** of the staple cartridge **34**. As explained previously, according to various embodiments, when the sled **33** traverses the channel **22**, the sled **33** drives the staple drivers **382** which drive the staples **380** into the severed tissue held in the end effector **12**, the staples **380** being formed against the anvil **24**. As noted above, such a surgical cutting and fastening instru-

13

ment is but one type of surgical instrument in which the present invention may be advantageously employed. Various embodiments of the present invention may be used in any type of surgical instrument having one or more sensor transponders.

In the embodiments described above, the battery 64 powers (at least partially) the firing operation of the instrument 10. As such, the instrument may be a so-called "power-assist" device. More details and additional embodiments of power-assist devices are described in the '573 application, which is incorporated herein. It should be recognized, however, that the instrument 10 need not be a power-assist device and that this is merely an example of a type of device that may utilize aspects of the present invention. For example, the instrument 10 may include a user display (such as a LCD or LED display) that is powered by the battery 64 and controlled by the control unit 300. Data from the sensor transponders 368 in the end effector 12 may be displayed on such a display.

In another embodiment, the shaft 8 of the instrument 10, including for example, the proximate closure tube 40 and the distal closure tube 42, may collectively serve as part of an antenna for the control unit 300 by radiating signals to the sensor transponder 368 and receiving radiated signals from the sensor transponder 368. That way, signals to and from the remote sensor in the end effector 12 may be transmitted via the shaft 8 of the instrument 10.

The proximate closure tube 40 may be grounded at its proximate end by the exterior lower and upper side pieces 59-62, which may be made of a nonelectrically conductive material, such as plastic. The drive shaft assembly components (including the main drive shaft 48 and secondary drive shaft 50) inside the proximate and distal closure tubes 40, 42 may also be made of a nonelectrically conductive material, such as plastic. Further, components of end effector 12 (such as the anvil 24 and the channel 22) may be electrically coupled to (or in direct or indirect electrical contact with) the distal closure tube 42 such that they may also serve as part of the antenna. Further, the sensor transponder 368 could be positioned such that it is electrically insulated from the components of the shaft 8 and end effector 12 serving as the antenna. For example, the sensor transponder 368 may be positioned in the cartridge 34, which may be made of a nonelectrically conductive material, such as plastic. Because the distal end of the shaft 8 (such as the distal end of the distal closure tube 42) and the portions of the end effector 12 serving as the antenna may be relatively close in distance to the sensor 368, the power for the transmitted signals may be held at low levels, thereby minimizing or reducing interference with other systems in the use environment of the instrument 10.

In such an embodiment, as shown in FIG. 16, the control unit 300 may be electrically coupled to the shaft 8 of the instrument 10, such as to the proximate closure tube 40, by a conductive link 400 (e.g., a wire). Portions of the outer shaft 8, such as the closure tubes 40, 42, may therefore act as part of an antenna for the control unit 300 by radiating signals to the sensor 368 and receiving radiated signals from the sensor 368. Input signals received by the control unit 300 may be demodulated by the demodulator 310 and decoded by the decoder 312 (see FIG. 12). The input signals may comprise data from the sensors 368 in the end effector 12, which the processor 306 may use to control various aspects of the instrument 10, such as the motor 65 or a user display.

To transmit data signals to or from the sensors 368 in the end effector 12, the link 400 may connect the control unit 300 to components of the shaft 8 of the instrument 10, such as the proximate closure tube 40, which may be electrically con-

14

nected to the distal closure tube 42. The distal closure tube 42 is preferably electrically insulated from the remote sensor 368, which may be positioned in the plastic cartridge 34 (see FIG. 3). As mentioned before, components of the end effector 12, such as the channel 22 and the anvil 24 (see FIG. 3), may be conductive and in electrical contact with the distal closure tube 42 such that they, too, may serve as part of the antenna.

With the shaft 8 acting as the antenna for the control unit 300, the control unit 300 can communicate with the sensor 368 in the end effector 12 without a direct wired connection. In addition, because the distances between shaft 8 and the remote sensor 368 is fixed and known, the power levels could be optimized for low levels to thereby minimize interference with other systems in the use environment of the instrument 10. The sensor 368 may include communication circuitry for radiating signals to the control unit 300 and for receiving signals from the control unit 300, as described above. The communication circuitry may be integrated with the sensor 368.

In another embodiment, the components of the shaft 8 and/or the end effector 12 may serve as an antenna for the remote sensor 368. In such an embodiment, the remote sensor 368 is electrically connected to the shaft (such as to distal closure tube 42, which may be electrically connected to the proximate closure tube 40) and the control unit 300 is insulated from the shaft 8. For example, the sensor 368 could be connected to a conductive component of the end effector 12 (such as the channel 22), which in turn may be connected to conductive components of the shaft (e.g., the closure tubes 40, 42). Alternatively, the end effector 12 may include a wire (not shown) that connects the remote sensor 368 the distal closure tube 42.

Typically, surgical instruments, such as the instrument 10, are cleaned and sterilized prior to use. In one sterilization technique, the instrument 10 is placed in a closed and sealed container 280, such as a plastic or TYVEK container or bag, as shown in FIGS. 17 and 18. The container and the instrument are then placed in a field of radiation that can penetrate the container, such as gamma radiation, x-rays, or high-energy electrons. The radiation kills bacteria on the instrument 10 and in the container 280. The sterilized instrument 10 can then be stored in the sterile container 280. The sealed, sterile container 280 keeps the instrument 10 sterile until it is opened in a medical facility or some other use environment. Instead of radiation, other means of sterilizing the instrument 10 may be used, such as ethylene oxide or steam.

When radiation, such as gamma radiation, is used to sterilize the instrument 10, components of the control unit 300, particularly the memory 308 and the processor 306, may be damaged and become unstable. Thus, according to various embodiments of the present invention, the control unit 300 may be programmed after packaging and sterilization of the instrument 10.

As shown in FIG. 17, a remote programming device 320, which may be a handheld device, may be brought into wireless communication with the control unit 300. The remote programming device 320 may emit wireless signals that are received by the control unit 300 to program the control unit 300 and to power the control unit 300 during the programming operation. That way, the battery 64 does not need to power the control unit 300 during the programming operation. According to various embodiments, the programming code downloaded to the control unit 300 could be of relatively small size, such as 1 MB or less, so that a communications protocol with a relatively low data transmission rate could be used if desired. Also, the remote programming unit 320 could

be brought into close physical proximity with the surgical instrument **10** so that a low power signal could be used.

Referring back to FIG. **19**, the control unit **300** may comprise an inductive coil **402** to pick up wireless signals from a remote programming device **320**. A portion of the received signal may be used by a power circuit **404** to power the control unit **300** when it is not being powered by the battery **64**.

Input signals received by the coil **402** acting as a receiving antenna may be demodulated by a demodulator **410** and decoded by a decoder **412**. The input signals may comprise programming instructions (e.g., code), which may be stored in a non-volatile memory portion of the memory **308**. The processor **306** may execute the code when the instrument **10** is in operation. For example, the code may cause the processor **306** to output control signals to various sub-systems of the instrument **10**, such as the motor **65**, based on data received from the sensors **368**.

The control unit **300** may also comprise a non-volatile memory unit **414** that comprises boot sequence code for execution by the processor **306**. When the control unit **300** receives enough power from the signals from the remote control unit **320** during the post-sterilization programming operation, the processor **306** may first execute the boot sequence code ("boot loader") **414**, which may load the processor **306** with an operating system.

The control unit **300** may also send signals back to the remote programming unit **320**, such as acknowledgement and handshake signals, for example. The control unit **300** may comprise an encoder **416** for encoding the signals to then be sent to the programming device **320** and a modulator **418** for modulating the signals according to the modulation scheme. The coil **402** may act as the transmitting antenna. The control unit **300** and the remote programming device **320** may communicate using any suitable wireless communication protocol (e.g., Bluetooth) and any suitable frequency (e.g., an ISM band). Also, the control unit **300** may transmit signals at a different frequency range than the frequency range of the received signals from the remote programming unit **320**.

FIG. **20** is a simplified diagram of the remote programming device **320** according to various embodiments of the present invention. As shown in FIG. **20**, the remote programming unit **320** may comprise a main control board **230** and a boosted antenna board **232**. The main control board **230** may comprise a controller **234**, a power module **236**, and a memory **238**. The memory **238** may store the operating instructions for the controller **234** as well as the programming instructions to be transmitted to the control unit **300** of the surgical instrument **10**. The power module **236** may provide a stable DC voltage for the components of the remote programming device **320** from an internal battery (not shown) or an external AC or DC power source (not shown).

The boosted antenna board **232** may comprise a coupler circuit **240** that is in communication with the controller **234** via an I²C bus, for example. The coupler circuit **240** may communicate with the control unit **300** of the surgical instrument via an antenna **244**. The coupler circuit **240** may handle the modulating/demodulating and encoding/decoding operations for transmissions with the control unit. According to other embodiments, the remote programming device **320** could have a discrete modulator, demodulator, encoder and decoder. As shown in FIG. **20**, the boost antenna board **232** may also comprise a transmitting power amp **246**, a matching circuit **248** for the antenna **244**, and a filter/amplifier **249** for receiving signals.

According to other embodiments, as shown in FIG. **20**, the remote programming device could be in communication with a computer device **460**, such as a PC or a laptop, via a USB

and/or RS232 interface, for example. In such a configuration, a memory of the computing device **460** may store the programming instructions to be transmitted to the control unit **300**. In another embodiment, the computing device **460** could be configured with a wireless transmission system to transmit the programming instructions to the control unit **300**.

In addition, according to other embodiments, rather than using inductive coupling between the control unit **300** and the remote programming device **320**, capacitively coupling could be used. In such an embodiment, the control unit **300** could have a plate instead of a coil, as could the remote programming unit **320**.

In another embodiment, rather than using a wireless communication link between the control unit **300** and the remote programming device **320**, the programming device **320** may be physically connected to the control unit **300** while the instrument **10** is in its sterile container **280** in such a way that the instrument **10** remains sterilized. FIG. **21** is a diagram of a packaged instrument **10** according to such an embodiment. As shown in FIG. **22**, the handle **6** of the instrument **10** may include an external connection interface **470**. The container **280** may further comprise a connection interface **472** that mates with the external connection interface **470** of the instrument **10** when the instrument **10** is packaged in the container **280**. The programming device **320** may include an external connection interface (not shown) that may connect to the connection interface **472** at the exterior of the container **280** to thereby provide a wired connection between the programming device **320** and the external connection interface **470** of the instrument **10**.

The various embodiments of the present invention have been described above in connection with cutting-type surgical instruments. It should be noted, however, that in other embodiments, the inventive surgical instrument disclosed herein need not be a cutting-type surgical instrument, but rather could be used in any type of surgical instrument including remote sensor transponders. For example, it could be a non-cutting endoscopic instrument, a grasper, a stapler, a clip applier, an access device, a drug/gene therapy delivery device, an energy device using ultrasound, RF, laser, etc. In addition, the present invention may be in laparoscopic instruments, for example. The present invention also has application in conventional endoscopic and open surgical instrumentation as well as robotic-assisted surgery.

The devices disclosed herein can be designed to be disposed of after a single use, or they can be designed to be used multiple times. In either case, however, the device can be reconditioned for reuse after at least one use. Reconditioning can include any combination of the steps of disassembly of the device, followed by cleaning or replacement of particular pieces, and subsequent reassembly. In particular, the device can be disassembled, and any number of the particular pieces or parts of the device can be selectively replaced or removed in any combination. Upon cleaning and/or replacement of particular parts, the device can be reassembled for subsequent use either at a reconditioning facility, or by a surgical team immediately prior to a surgical procedure. Those skilled in the art will appreciate that reconditioning of a device can utilize a variety of techniques for disassembly, cleaning/replacement, and reassembly. Use of such techniques, and the resulting reconditioned device, are all within the scope of the present application.

Although the present invention has been described herein in connection with certain disclosed embodiments, many modifications and variations to those embodiments may be implemented. For example, different types of end effectors may be employed. Also, where materials are disclosed for

certain components, other materials may be used. The foregoing description and following claims are intended to cover all such modification and variations.

Any patent, publication, or other disclosure material, in whole or in part, that is said to be incorporated by reference herein is incorporated herein only to the extent that the incorporated materials does not conflict with existing definitions, statements, or other disclosure material set forth in this disclosure. As such, and to the extent necessary, the disclosure as explicitly set forth herein supersedes any conflicting material incorporated herein by reference. Any material, or portion thereof, that is said to be incorporated by reference herein, but which conflicts with existing definitions, statements, or other disclosure material set forth herein will only be incorporated to the extent that no conflict arises between that incorporated material and the existing disclosure material.

What is claimed is:

1. A surgical instrument comprising:
an end effector comprising at least one sensor;
a shaft having a distal end connected to the end effector, wherein the shaft comprises:
at least one electrically conductive outer tube, wherein the sensor is electrically insulated from the at least one electrically conductive outer tube; and
a drive shaft disposed at least partially within the at least one electrically conductive outer tube;
a handle connected to a proximate end of the shaft, the handle housing a control unit, wherein the control unit is electrically coupled to the at least one electrically conductive outer tube such that the at least one electrically conductive outer tube wirelessly radiates communication signals from the control unit to the sensor and receives wirelessly radiated communication signals from the sensor.
2. The surgical instrument of claim 1, wherein the handle further houses:
a motor in communication with the control unit and for powering the end effector; and
a battery for powering the motor.
3. The surgical instrument of claim 1, wherein the at least one sensor comprises a magnetoresistive sensor.
4. The surgical instrument of claim 1, wherein the at least one sensor comprises a pressure sensor.
5. The surgical instrument of claim 1, wherein the at least one sensor comprises a RFID sensor.
6. The surgical instrument of claim 1, wherein the at least one sensor comprises a MEMS sensor.
7. The surgical instrument of claim 1, wherein the at least one sensor comprises an electromechanical sensor.
8. The surgical instrument of claim 1, wherein the at least one sensor is connected to a plastic cartridge of the end effector.
9. The surgical instrument of claim 1, wherein the end effector comprises an electrically conductive component coupled to the at least one electrically conductive outer tube, wherein the electrically conductive component is configured to radiate communication signals to and from the sensor.

10. The surgical instrument of claim 1, wherein the surgical instrument comprises an endoscopic surgical instrument.

11. The surgical instrument of claim 1, wherein the surgical instrument comprises a cutting and fastening surgical instrument.

12. The surgical instrument of claim 11, wherein the end effector comprises a cutting instrument.

13. The surgical instrument of claim 12, wherein the end effector comprises a plastic cartridge and the at least one sensor is disposed in the cartridge.

14. The surgical instrument of claim 1, wherein the communication signals radiated wirelessly from the shaft use a wireless communication protocol.

15. The surgical instrument of claim 1, wherein the wireless signals comprise RF wireless signals.

16. A surgical instrument comprising:
an end effector comprising at least one sensor;
an electrically conductive shaft having a distal end connected to the end effector wherein the shaft comprises at least one electrically conductive outer tube, wherein the sensor is electrically insulated from the at least one electrically conductive outer tube; and
a control unit electrically coupled to the shaft such that the at least one electrically conductive outer tube wirelessly radiates communication signals from the control unit to the sensor and to receives wirelessly radiated communication signals from the sensor.

17. The surgical instrument of claim 16, further comprising:
a motor in communication with the control unit and for powering the end effector; and
a battery for powering the motor.

18. The surgical instrument of claim 16, wherein the at least one sensor is connected to a plastic cartridge of the end effector.

19. The surgical instrument of claim 16, wherein the end effector comprises an electrically conductive component coupled to the at least one electrically conductive outer tube, wherein the electrically conductive component is configured to radiate wireless communication signals to and from the sensor.

20. The surgical instrument of claim 19, wherein the end effector comprises a plastic staple cartridge and the at least one sensor is disposed in the staple cartridge.

21. A surgical instrument comprising:
an end effector comprising at least one sensor;
an electrically conductive shaft having a distal end connected to the end effector, wherein the shaft comprises at least one electrically conductive outer tube, wherein the sensor is electrically coupled to the at least one electrically conductive outer tube; and
a control unit electrically insulated from the at least one electrically conductive outer tube, such that the at least one electrically conductive outer tube radiates wireless communication signals from the sensor to the control unit and receives wirelessly radiated communication signals from the control unit.

* * * * *

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : 8,459,520 B2
APPLICATION NO. : 11/651807
DATED : June 11, 2013
INVENTOR(S) : James R. Giordano et al.

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the Title Page:

The first or sole Notice should read --

Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b)
by 1106 days.

Signed and Sealed this
Twenty-third Day of December, 2014



Michelle K. Lee
Deputy Director of the United States Patent and Trademark Office

专利名称(译)	在控制单元和远程传感器之间进行无线通信的手术器械		
公开(公告)号	US8459520	公开(公告)日	2013-06-11
申请号	US11/651807	申请日	2007-01-10
[标]申请(专利权)人(译)	GIORDANO JAMES - [R] 斯韦兹JEFFREY小号 谢尔顿检基ê		
申请(专利权)人(译)	GIORDANO JAMES - [R] 斯韦兹JEFFREY小号 谢尔顿检基ê		
当前申请(专利权)人(译)	爱惜康内镜手术，INC.		
[标]发明人	GIORDANO JAMES R SWAYZE JEFFREY S SHELTON IV FREDERICK E		
发明人	GIORDANO, JAMES R. SWAYZE, JEFFREY S. SHELTON, IV, FREDERICK E.		
IPC分类号	A61B17/32		
CPC分类号	A61B17/068 A61B17/07207 A61B90/98 A61B2017/00022 A61B2017/00221 A61B2017/00398 A61B2017/00734 A61B2017/07271 A61B2017/2927 A61B2090/065 A61B2090/0814		
其他公开文献	US20080167672A1		
外部链接	Espacenet USPTO		

摘要(译)

手术器械，例如内窥镜或腹腔镜器械。手术器械可包括末端执行器，末端执行器包括至少一个传感器。手术器械还可包括导电轴，该导电轴具有连接到端部执行器的远端，其中传感器与轴电绝缘。手术器械还可包括连接到轴的近端的手柄。手柄可包括电连接到轴的控制单元，使得轴将信号作为天线从控制单元辐射到传感器并接收来自传感器的辐射信号。电耦合到轴的其他部件也可以辐射信号。

