



US008652120B2

(12) **United States Patent**
Giordano et al.

(10) **Patent No.:** **US 8,652,120 B2**
(45) **Date of Patent:** ***Feb. 18, 2014**

(54) **SURGICAL INSTRUMENT WITH WIRELESS COMMUNICATION BETWEEN CONTROL UNIT AND SENSOR TRANSPONDERS**

(75) Inventors: **James R. Giordano**, Milford, OH (US);
Frederick E. Shelton, IV, New Vienna, OH (US); **Jeffrey S. Swayze**, Hamilton, OH (US)

(73) Assignee: **Ethicon Endo-Surgery, Inc.**, Cincinnati, OH (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 1966 days.

This patent is subject to a terminal disclaimer.

2,161,632 A	6/1939	Nattenheimer
2,211,117 A	8/1940	Hess
2,214,870 A	9/1940	West
2,441,096 A	5/1948	Happe
2,526,902 A	10/1950	Rublee
2,674,149 A	4/1954	Benson
2,804,848 A	9/1957	O'Farrell et al.
2,808,482 A	10/1957	Zanichkowsky et al.
2,853,074 A	9/1958	Olson
3,032,769 A	5/1962	Palmer
3,075,062 A	1/1963	Iaccarino
3,078,465 A	2/1963	Bobrov

(Continued)

FOREIGN PATENT DOCUMENTS

CA	2458946 A1	3/2003
CA	2512960 A1	1/2006

(Continued)

OTHER PUBLICATIONS

European Examination Report, Application No. 08250093.5, dated Jun. 14, 2010 (5 pages).

(Continued)

Primary Examiner — Aaron Roane

(21) Appl. No.: **11/651,715**

(22) Filed: **Jan. 10, 2007**

(65) **Prior Publication Data**

US 2008/0167522 A1 Jul. 10, 2008

(51) **Int. Cl.**
A61B 18/00 (2006.01)

(52) **U.S. Cl.**
USPC **606/1; 700/245; 606/205**

(58) **Field of Classification Search**
USPC 606/1, 2-52, 205; 700/245-264
See application file for complete search history.

(56) **References Cited**


U.S. PATENT DOCUMENTS

66,052 A	6/1867	Smith
662,587 A	11/1900	Blake
951,393 A	3/1910	Hahn
2,037,727 A	4/1936	La Chapelle
2,132,295 A	10/1938	Hawkins

(57) **ABSTRACT**

A surgical instrument, such as an endoscopic or laparoscopic instrument, comprising, according to various embodiments, an end effector comprising at least one sensor transponder. The surgical instrument also comprises a shaft having a distal end connected to the end effector and a handle connected to a proximate end of the shaft. The handle comprises a control unit in communication with the sensor transponder via at least one inductive coupling. The surgical instrument may be a power-assist motorized device including a battery for powering (at least partially) the surgical instrument during use. The surgical instrument may be adapted to provide user feedback regarding the load being experienced by the end effector.

20 Claims, 21 Drawing Sheets

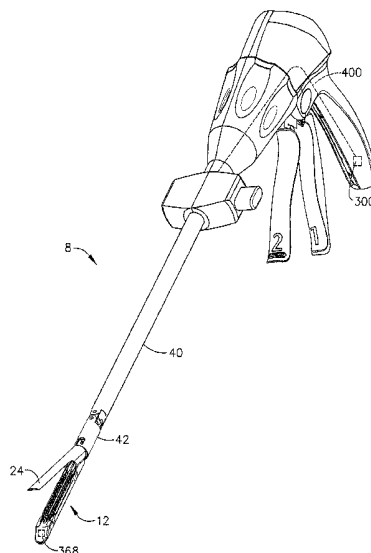

(56)

References Cited

U.S. PATENT DOCUMENTS

3,166,072 A	1/1965	Sullivan, Jr.	4,605,004 A	8/1986	Di Giovanni et al.
3,266,494 A	8/1966	Brownrigg et al.	4,606,343 A	8/1986	Conta et al.
3,269,630 A	8/1966	Fleischer	4,607,638 A	8/1986	Crainich
3,357,296 A	12/1967	Lefever	4,608,981 A	9/1986	Rothfuss et al.
3,490,675 A	1/1970	Green et al.	4,610,250 A	9/1986	Green
3,551,987 A	1/1971	Wilkinson	4,610,383 A	9/1986	Rothfuss et al.
3,598,943 A	8/1971	Barrett	4,619,262 A	10/1986	Taylor
3,643,851 A	2/1972	Green et al.	4,629,107 A	12/1986	Fedotov et al.
3,662,939 A	5/1972	Bryan	4,632,290 A	12/1986	Green et al.
3,717,294 A	2/1973	Green	4,633,874 A	1/1987	Chow et al.
3,734,207 A	5/1973	Fishbein	4,641,076 A	2/1987	Linden
3,740,994 A	6/1973	De Carlo, Jr.	4,646,722 A	3/1987	Silverstein et al.
3,744,495 A	7/1973	Johnson	4,655,222 A	4/1987	Florez et al.
3,746,002 A	7/1973	Haller	4,663,874 A	5/1987	Sano et al.
3,751,902 A	8/1973	Kingsbury et al.	4,664,305 A	5/1987	Blake, III et al.
3,819,100 A	6/1974	Noiles et al.	4,665,916 A	5/1987	Green
3,821,919 A	7/1974	Knohl	4,667,674 A	5/1987	Korthoff et al.
3,885,491 A	5/1975	Curtis	4,671,445 A	6/1987	Barker et al.
3,892,228 A	7/1975	Mitsui	4,676,245 A	6/1987	Fukuda
3,894,174 A	7/1975	Cartun	4,693,248 A	9/1987	Failla
3,940,844 A	3/1976	Colby et al.	4,709,120 A	11/1987	Pearson
RE28,932 E	8/1976	Noiles et al.	4,715,520 A	12/1987	Roehr, Jr. et al.
4,060,089 A	11/1977	Noiles	4,719,917 A	1/1988	Barrows et al.
4,129,059 A	12/1978	Van Eck	4,728,020 A	3/1988	Green et al.
4,213,562 A	7/1980	Garrett et al.	4,728,876 A	3/1988	Mongeon et al.
4,250,436 A	2/1981	Weissman	4,729,260 A	3/1988	Dudden
4,261,244 A	4/1981	Becht et al.	4,741,336 A	5/1988	Failla et al.
4,272,662 A	6/1981	Simpson	4,752,024 A	6/1988	Green et al.
4,275,813 A	6/1981	Noiles	4,754,909 A	7/1988	Barker et al.
4,289,133 A	9/1981	Rothfuss	4,767,044 A	8/1988	Green
4,305,539 A	12/1981	Korolkov et al.	4,777,780 A	10/1988	Holzwarth
4,317,451 A	3/1982	Cerwin et al.	4,787,387 A	11/1988	Burbank, III et al.
4,321,002 A	3/1982	Froehlich	4,790,225 A	12/1988	Moody et al.
4,331,277 A	5/1982	Green	4,805,617 A	2/1989	Bedi et al.
4,340,331 A	7/1982	Savino	4,805,823 A	2/1989	Rothfuss
4,347,450 A	8/1982	Colligan	4,809,695 A	3/1989	Gwathmey et al.
4,349,028 A	9/1982	Green	4,817,847 A	4/1989	Redtenbacher et al.
4,353,371 A	10/1982	Cosman	4,819,853 A	4/1989	Green
4,379,457 A	4/1983	Gravener et al.	4,821,939 A	4/1989	Green
4,380,312 A	4/1983	Landrus	4,827,911 A	5/1989	Broadwin et al.
4,383,634 A	5/1983	Green	4,844,068 A	7/1989	Arata et al.
4,396,139 A	8/1983	Hall et al.	4,869,414 A	9/1989	Green et al.
4,402,445 A	9/1983	Green	4,869,415 A	9/1989	Fox
4,408,692 A	10/1983	Siegel et al.	4,880,015 A	11/1989	Nierman
4,415,112 A	11/1983	Green	4,890,613 A	1/1990	Golden et al.
4,428,376 A	1/1984	Mericle	4,892,244 A	1/1990	Fox et al.
4,429,695 A	2/1984	Green	4,915,100 A	4/1990	Green
4,434,796 A	3/1984	Karapetian et al.	4,930,503 A	6/1990	Pruitt
4,442,964 A	4/1984	Becht	4,932,960 A	6/1990	Green et al.
4,451,743 A	5/1984	Suzuki et al.	4,938,408 A	7/1990	Bedi et al.
4,454,887 A	6/1984	Krüger	4,941,623 A	7/1990	Pruitt
4,467,805 A	8/1984	Fukuda	4,944,443 A	7/1990	Odds et al.
4,475,679 A	10/1984	Fleury, Jr.	4,955,959 A	9/1990	Tompkins et al.
4,485,816 A	12/1984	Krumme	4,978,049 A	12/1990	Green
4,489,875 A	12/1984	Crawford et al.	4,986,808 A	1/1991	Broadwin et al.
4,500,024 A	2/1985	DiGiovanni et al.	4,988,334 A	1/1991	Hornlein et al.
4,505,273 A	3/1985	Braun et al.	5,002,553 A	3/1991	Shiber
4,505,414 A	3/1985	Filipi	5,009,661 A	4/1991	Michelson
4,506,671 A	3/1985	Green	5,014,899 A	5/1991	Presty et al.
4,520,817 A	6/1985	Green	5,015,227 A	5/1991	Broadwin et al.
4,522,327 A	6/1985	Korthoff et al.	5,027,834 A	7/1991	Pruitt
4,526,174 A	7/1985	Froehlich	5,031,814 A	7/1991	Tompkins et al.
4,527,724 A	7/1985	Chow et al.	5,040,715 A	8/1991	Green et al.
4,530,453 A	7/1985	Green	5,042,707 A	8/1991	Taheri
4,548,202 A	10/1985	Duncan	5,061,269 A	10/1991	Muller
4,565,189 A	1/1986	Mabuchi	5,062,563 A	11/1991	Green et al.
4,566,620 A	1/1986	Green et al.	5,065,929 A	11/1991	Schulze et al.
4,573,469 A	3/1986	Golden et al.	5,071,052 A	12/1991	Rodak et al.
4,573,622 A	3/1986	Green et al.	5,071,430 A	12/1991	de Salis et al.
4,576,167 A	3/1986	Noiles et al.	5,074,454 A	12/1991	Peters
4,580,712 A	4/1986	Green	5,080,556 A	1/1992	Carreno
4,589,416 A	5/1986	Green	5,083,695 A	1/1992	Foslien et al.
4,591,085 A	5/1986	Di Giovanni	5,084,057 A	1/1992	Green et al.
4,604,786 A	8/1986	Howie, Jr.	5,088,979 A	2/1992	Filipi et al.
4,605,001 A	8/1986	Rothfuss et al.	5,088,997 A	2/1992	Delahuerga et al.
			5,094,247 A	3/1992	Hernandez et al.
			5,100,420 A	3/1992	Green et al.
			5,104,025 A	4/1992	Main et al.
			5,106,008 A	4/1992	Tompkins et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

5,111,987 A	5/1992	Moeinzadeh et al.	5,350,400 A	9/1994	Esposito et al.
5,116,349 A	5/1992	Aranyi	5,352,235 A	10/1994	Koros et al.
5,129,570 A	7/1992	Schulze et al.	5,352,238 A	10/1994	Green et al.
5,137,198 A	8/1992	Nobis et al.	5,354,303 A	10/1994	Spaeth et al.
5,139,513 A	8/1992	Segato	5,356,006 A	10/1994	Alpern et al.
5,141,144 A	8/1992	Foslien et al.	5,358,510 A	10/1994	Luscombe et al.
5,156,315 A	10/1992	Green et al.	5,359,231 A	10/1994	Flowers et al.
5,156,614 A	10/1992	Green et al.	D352,780 S	11/1994	Glaeser et al.
5,158,567 A	10/1992	Green	5,360,428 A	11/1994	Hutchinson, Jr.
D330,699 S	11/1992	Gill	5,364,003 A	11/1994	Williamson, IV
5,163,598 A	11/1992	Peters et al.	5,366,134 A	11/1994	Green et al.
5,171,247 A	12/1992	Hughett et al.	5,366,479 A	11/1994	McGarry et al.
5,171,249 A	12/1992	Stefanchik et al.	5,368,015 A	11/1994	Wilk
5,188,111 A	2/1993	Yates et al.	5,370,645 A	12/1994	Klicek et al.
5,190,517 A	3/1993	Zieve et al.	5,372,596 A	12/1994	Klicek et al.
5,195,968 A	3/1993	Lundquist et al.	5,372,602 A	12/1994	Burke
5,197,648 A	3/1993	Gingold	5,374,277 A	12/1994	Hassler
5,200,280 A	4/1993	Karasa	5,379,933 A	1/1995	Green et al.
5,205,459 A	4/1993	Brinkerhoff et al.	5,381,782 A	1/1995	DeLaRama et al.
5,207,697 A	5/1993	Carusillo et al.	5,382,247 A	1/1995	Cimino et al.
5,209,747 A	5/1993	Knoepfler	5,383,880 A	1/1995	Hooven
5,211,649 A	5/1993	Kohler et al.	5,383,881 A	1/1995	Green et al.
5,217,457 A	6/1993	Delahuerga et al.	5,383,888 A	1/1995	Zvenyatsky et al.
5,217,478 A	6/1993	Rexroth	5,383,895 A	1/1995	Holmes et al.
5,219,111 A	6/1993	Bilotti et al.	5,389,098 A	2/1995	Tsuruta et al.
5,221,036 A	6/1993	Takase	5,391,180 A	2/1995	Tovey et al.
5,221,281 A	6/1993	Klicek	5,392,979 A	2/1995	Green et al.
5,222,963 A	6/1993	Brinkerhoff et al.	5,395,030 A	3/1995	Kuramoto et al.
5,222,975 A	6/1993	Crainich	5,395,033 A	3/1995	Byrne et al.
5,222,976 A	6/1993	Yoon	5,395,312 A	3/1995	Desai
5,223,675 A	6/1993	Taft	5,397,046 A	3/1995	Savage et al.
5,234,447 A	8/1993	Kaster et al.	5,397,324 A	3/1995	Carroll et al.
5,236,440 A	8/1993	Hlavacek	5,403,312 A	4/1995	Yates et al.
5,239,981 A	8/1993	Anapliotis	5,405,072 A	4/1995	Zlock et al.
5,240,163 A	8/1993	Stein et al.	5,405,344 A	4/1995	Williamson et al.
5,242,457 A	9/1993	Akopov et al.	5,407,293 A	4/1995	Crainich
5,244,462 A	9/1993	Delahuerga et al.	5,409,498 A	4/1995	Braddock et al.
5,246,156 A	9/1993	Rothfuss et al.	5,411,508 A	5/1995	Bessler et al.
5,246,443 A	9/1993	Mai	5,413,267 A	5/1995	Solyntjes et al.
5,253,793 A	10/1993	Green et al.	5,413,268 A	5/1995	Green et al.
5,258,009 A	11/1993	Connors	5,413,272 A	5/1995	Green et al.
5,258,012 A	11/1993	Luscombe et al.	5,415,334 A	5/1995	Williamson, IV et al.
5,259,366 A	11/1993	Reydel et al.	5,415,335 A	5/1995	Knodell, Jr.
5,260,637 A	11/1993	Pizzi	5,417,361 A	5/1995	Williamson, IV
5,263,629 A	11/1993	Trumbull et al.	5,421,829 A	6/1995	Olichney et al.
5,263,973 A	11/1993	Cook	5,422,567 A	6/1995	Matsunaga
5,268,622 A	12/1993	Philipp	5,423,809 A	6/1995	Klicek
5,271,543 A	12/1993	Grant et al.	5,425,745 A	6/1995	Green et al.
5,271,544 A	12/1993	Fox et al.	5,431,322 A	7/1995	Green et al.
RE34,519 E	1/1994	Fox et al.	5,431,668 A	7/1995	Burbank, III et al.
5,275,323 A	1/1994	Schulze et al.	5,433,721 A	7/1995	Hooven et al.
5,275,608 A	1/1994	Forman et al.	5,438,302 A	8/1995	Goble
5,281,216 A	1/1994	Klicek	5,439,479 A	8/1995	Shichman et al.
5,282,806 A	2/1994	Haber et al.	5,441,193 A	8/1995	Gravener
5,282,829 A	2/1994	Hermes	5,441,494 A	8/1995	Ortiz
5,297,714 A	3/1994	Kramer	5,445,304 A	8/1995	Plyley et al.
5,304,204 A	4/1994	Bregen	5,445,644 A	8/1995	Pietrafitta et al.
5,307,976 A	5/1994	Olson et al.	5,447,417 A	9/1995	Kuhl et al.
5,309,927 A	5/1994	Welch	5,447,513 A	9/1995	Davison et al.
5,312,023 A	5/1994	Green et al.	5,449,355 A	9/1995	Rhum et al.
5,312,329 A	5/1994	Beaty et al.	5,449,365 A	9/1995	Green et al.
5,314,424 A	5/1994	Nicholas	5,452,836 A	9/1995	Huitema et al.
5,318,221 A	6/1994	Green et al.	5,452,837 A	9/1995	Williamson, IV et al.
5,330,502 A	7/1994	Hassler et al.	5,454,827 A	10/1995	Aust et al.
5,332,142 A	7/1994	Robinson et al.	5,456,401 A	10/1995	Green et al.
5,333,422 A	8/1994	Warren et al.	5,458,579 A	10/1995	Chodorow et al.
5,333,772 A	8/1994	Rothfuss et al.	5,462,215 A	10/1995	Viola et al.
5,334,183 A	8/1994	Wuchinich	5,464,300 A	11/1995	Crainich
5,336,232 A	8/1994	Green et al.	5,465,894 A	11/1995	Clark et al.
5,339,799 A	8/1994	Kami et al.	5,465,895 A	11/1995	Knodel et al.
5,341,724 A	8/1994	Vatel	5,465,896 A	11/1995	Allen et al.
5,341,810 A	8/1994	Dardel	5,466,020 A	11/1995	Page et al.
5,342,395 A	8/1994	Jarrett et al.	5,467,911 A	11/1995	Tsuruta et al.
5,342,396 A	8/1994	Cook	5,470,006 A	11/1995	Rodak
5,344,060 A	9/1994	Gravener et al.	5,470,007 A	11/1995	Plyley et al.
			5,470,009 A	11/1995	Rodak
			5,472,132 A	12/1995	Savage et al.
			5,472,442 A	12/1995	Klicek
			5,473,204 A	12/1995	Temple

(56)

References Cited

U.S. PATENT DOCUMENTS

5,474,057	A	12/1995	Makower et al.	5,575,789	A	11/1996	Bell et al.
5,474,566	A	12/1995	Alesi et al.	5,575,799	A	11/1996	Bolanos et al.
5,476,206	A	12/1995	Green et al.	5,575,803	A	11/1996	Cooper et al.
5,476,479	A	12/1995	Green et al.	5,577,654	A	11/1996	Bishop
5,478,003	A	12/1995	Green et al.	5,579,978	A	12/1996	Green et al.
5,478,354	A	12/1995	Tovey et al.	5,580,067	A	12/1996	Hamblin et al.
5,480,089	A	1/1996	Blewett	5,582,611	A	12/1996	Tsuruta et al.
5,480,409	A	1/1996	Riza	5,582,617	A	12/1996	Klieman et al.
5,482,197	A	1/1996	Green et al.	5,584,425	A	12/1996	Savage et al.
5,484,095	A	1/1996	Green et al.	5,586,711	A	12/1996	Plyley et al.
5,484,398	A	1/1996	Stoddard	5,588,579	A	12/1996	Schnut et al.
5,484,451	A	1/1996	Akopov et al.	5,588,580	A	12/1996	Paul et al.
5,485,947	A	1/1996	Olson et al.	5,588,581	A	12/1996	Conlon et al.
5,485,952	A	1/1996	Fontayne	5,591,170	A	1/1997	Spievack et al.
5,487,499	A	1/1996	Sorrentino et al.	5,591,187	A	1/1997	Dekel
5,487,500	A	1/1996	Knodel et al.	5,597,107	A	1/1997	Knodel et al.
5,489,058	A	2/1996	Plyley et al.	5,599,151	A	2/1997	Daum et al.
5,489,256	A	2/1996	Adair	5,599,344	A	2/1997	Paterson
5,496,312	A	3/1996	Kliceck	5,599,350	A	2/1997	Schulze et al.
5,496,317	A	3/1996	Goble et al.	5,601,224	A	2/1997	Bishop et al.
5,497,933	A	3/1996	DeFonzo et al.	5,603,443	A	2/1997	Clark et al.
5,503,320	A	4/1996	Webster et al.	5,605,272	A	2/1997	Witt et al.
5,503,635	A	4/1996	Sauer et al.	5,605,273	A	2/1997	Hamblin et al.
5,503,638	A	4/1996	Cooper et al.	5,607,094	A	3/1997	Clark et al.
5,505,363	A	4/1996	Green et al.	5,607,095	A	3/1997	Smith et al.
5,507,426	A	4/1996	Young et al.	5,607,450	A	3/1997	Zvenyatsky et al.
5,509,596	A	4/1996	Green et al.	5,609,285	A	3/1997	Grant et al.
5,509,916	A	4/1996	Taylor	5,611,709	A	3/1997	McAnulty
5,511,564	A	4/1996	Wilk	5,613,966	A	3/1997	Makower et al.
5,514,129	A	5/1996	Smith	5,618,294	A	4/1997	Aust et al.
5,514,157	A	5/1996	Nicholas et al.	5,618,303	A	4/1997	Marlow et al.
5,518,163	A	5/1996	Hooven	5,618,307	A	4/1997	Donlon et al.
5,518,164	A	5/1996	Hooven	5,620,289	A	4/1997	Curry
5,520,678	A	5/1996	Heckele et al.	5,620,452	A	4/1997	Yoon
5,520,700	A	5/1996	Beyar et al.	5,624,452	A	4/1997	Yates
5,522,817	A	6/1996	Sander et al.	5,626,587	A	5/1997	Bishop et al.
5,527,320	A	6/1996	Carruthers et al.	5,628,446	A	5/1997	Geiste et al.
5,529,235	A	6/1996	Boiarski et al.	5,628,743	A	5/1997	Cimino
D372,086	S	7/1996	Grasso et al.	5,630,539	A	5/1997	Plyley et al.
5,531,744	A	7/1996	Nardella et al.	5,630,540	A	5/1997	Blewett
5,533,521	A	7/1996	Granger	5,630,782	A	5/1997	Adair
5,533,581	A	7/1996	Barth et al.	5,632,432	A	5/1997	Schulze et al.
5,533,661	A	7/1996	Main et al.	5,632,433	A	5/1997	Grant et al.
5,535,934	A	7/1996	Boiarski et al.	5,634,584	A	6/1997	Okorocho et al.
5,535,935	A	7/1996	Vidal et al.	5,636,779	A	6/1997	Palmer
5,535,937	A	7/1996	Boiarski et al.	5,636,780	A	6/1997	Green et al.
5,540,375	A	7/1996	Bolanos et al.	5,639,008	A	6/1997	Gallagher et al.
5,541,376	A	7/1996	Ladtikow et al.	5,643,291	A	7/1997	Pier et al.
5,542,594	A	8/1996	McKean et al.	5,645,209	A	7/1997	Green et al.
5,543,119	A	8/1996	Sutter et al.	5,647,526	A	7/1997	Green et al.
5,547,117	A	8/1996	Hamblin et al.	5,647,869	A	7/1997	Goble et al.
5,549,621	A	8/1996	Bessler et al.	5,649,937	A	7/1997	Bito et al.
5,549,628	A	8/1996	Cooper et al.	5,651,491	A	7/1997	Heaton et al.
5,549,637	A	8/1996	Crainich	5,653,373	A	8/1997	Green et al.
5,553,675	A	9/1996	Pitzen et al.	5,653,374	A	8/1997	Young et al.
5,553,765	A	9/1996	Knodel et al.	5,653,677	A	8/1997	Okada et al.
5,554,169	A	9/1996	Green et al.	5,653,721	A	8/1997	Knodel et al.
5,556,416	A	9/1996	Clark et al.	5,655,698	A	8/1997	Yoon
5,558,665	A	9/1996	Kieturakis	5,657,921	A	8/1997	Young et al.
5,558,671	A	9/1996	Yates	5,658,281	A	8/1997	Heard
5,560,530	A	10/1996	Bolanos et al.	5,658,300	A	8/1997	Bito et al.
5,560,532	A	10/1996	DeFonzo et al.	5,662,258	A	9/1997	Knodel et al.
5,562,239	A	10/1996	Boiarski et al.	5,662,260	A	9/1997	Yoon
5,562,241	A	10/1996	Knodel et al.	5,662,662	A	9/1997	Bishop et al.
5,562,682	A	10/1996	Oberlin et al.	5,667,517	A	9/1997	Hooven
5,562,701	A	10/1996	Huitema et al.	5,667,526	A	9/1997	Levin
5,562,702	A	10/1996	Huitema et al.	5,667,527	A	9/1997	Cook
5,564,615	A	10/1996	Bishop et al.	5,669,544	A	9/1997	Schulze et al.
5,569,161	A	10/1996	Ebling et al.	5,669,904	A	9/1997	Platt, Jr. et al.
5,569,284	A	10/1996	Young et al.	5,669,907	A	9/1997	Platt, Jr. et al.
5,571,090	A	11/1996	Sherts	5,669,918	A	9/1997	Balazs et al.
5,571,100	A	11/1996	Goble et al.	5,673,840	A	10/1997	Schulze et al.
5,571,116	A	11/1996	Bolanos et al.	5,673,841	A	10/1997	Schulze et al.
5,573,543	A	11/1996	Akopov et al.	5,673,842	A	10/1997	Bittner et al.
5,574,431	A	11/1996	McKeown et al.	5,678,748	A	10/1997	Plyley et al.
				5,680,981	A	10/1997	Mililli et al.
				5,680,982	A	10/1997	Schulze et al.
				5,680,983	A	10/1997	Plyley et al.
				5,683,349	A	11/1997	Makower et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

5,685,474 A	11/1997	Seeber	5,794,834 A	8/1998	Hamblin et al.
5,688,270 A	11/1997	Yates et al.	5,796,188 A	8/1998	Bays
5,690,269 A	11/1997	Bolanos et al.	5,797,536 A	8/1998	Smith et al.
5,692,668 A	12/1997	Schulze et al.	5,797,537 A	8/1998	Oberlin et al.
5,693,042 A	12/1997	Boiarski et al.	5,797,538 A	8/1998	Heaton et al.
5,693,051 A	12/1997	Schulze et al.	5,797,906 A	8/1998	Rhum et al.
5,695,494 A	12/1997	Becker	5,797,959 A	8/1998	Castro et al.
5,695,504 A	12/1997	Gifford, III et al.	5,799,857 A	9/1998	Robertson et al.
5,695,524 A	12/1997	Kelley et al.	5,807,376 A	9/1998	Viola et al.
5,697,543 A	12/1997	Burdorff	5,807,378 A	9/1998	Jensen et al.
5,697,943 A	12/1997	Sauer et al.	5,807,393 A	9/1998	Williamson, IV et al.
5,700,270 A	12/1997	Peyser et al.	5,809,441 A	9/1998	McKee
5,702,387 A	12/1997	Arts et al.	5,810,811 A	9/1998	Yates et al.
5,702,408 A	12/1997	Wales et al.	5,810,855 A	9/1998	Rayburn et al.
5,702,409 A	12/1997	Rayburn et al.	5,813,813 A	9/1998	Daum et al.
5,704,087 A	1/1998	Strub	5,814,057 A	9/1998	Oi et al.
5,704,534 A	1/1998	Huitema et al.	5,817,084 A	10/1998	Jensen
5,706,997 A	1/1998	Green et al.	5,817,091 A	10/1998	Nardella et al.
5,706,998 A	1/1998	Plyley et al.	5,817,093 A	10/1998	Williamson, IV et al.
5,707,392 A	1/1998	Kortenbach	5,817,109 A	10/1998	McGarry et al.
5,709,334 A	1/1998	Sorrentino et al.	5,817,119 A	10/1998	Klieman et al.
5,709,680 A	1/1998	Yates et al.	5,820,009 A	10/1998	Melling et al.
5,711,472 A	1/1998	Bryan	5,823,066 A	10/1998	Huitema et al.
5,713,128 A	2/1998	Schrenk et al.	5,826,776 A	10/1998	Schulze et al.
5,713,505 A	2/1998	Huitema	5,827,271 A	10/1998	Buyse et al.
5,713,895 A	2/1998	Lontine et al.	5,829,662 A	11/1998	Allen et al.
5,713,896 A	2/1998	Nardella	5,833,690 A	11/1998	Yates et al.
5,715,987 A	2/1998	Kelley et al.	5,833,695 A	11/1998	Yoon
5,715,988 A	2/1998	Palmer	5,833,696 A	11/1998	Whitfield et al.
5,716,366 A	2/1998	Yates	5,836,503 A	11/1998	Ehrenfels et al.
5,718,359 A	2/1998	Palmer et al.	5,836,960 A	11/1998	Kolesa et al.
5,718,360 A	2/1998	Green et al.	5,839,639 A	11/1998	Sauer et al.
5,718,548 A	2/1998	Cotellessa	5,843,132 A	12/1998	Ilvento
5,720,744 A	2/1998	Eggleston et al.	5,846,254 A	12/1998	Schulze et al.
D393,067 S	3/1998	Geary et al.	5,849,011 A	12/1998	Jones et al.
5,725,536 A	3/1998	Oberlin et al.	5,855,311 A	1/1999	Hamblin et al.
5,725,554 A	3/1998	Simon et al.	5,855,583 A	1/1999	Wang et al.
5,728,121 A	3/1998	Bimbo et al.	5,860,975 A	1/1999	Goble et al.
5,730,758 A	3/1998	Allgeyer	5,865,361 A	2/1999	Milliman et al.
5,732,871 A	3/1998	Clark et al.	5,868,760 A	2/1999	McGuckin, Jr.
5,732,872 A	3/1998	Bolduc et al.	5,871,135 A	2/1999	Williamson, IV et al.
5,735,445 A	4/1998	Vidal et al.	5,873,885 A	2/1999	Weidenbenner
5,735,848 A	4/1998	Yates et al.	5,876,401 A	3/1999	Schulze et al.
5,735,874 A	4/1998	Measamer et al.	5,878,193 A	3/1999	Wang et al.
5,738,474 A	4/1998	Blewett	5,878,937 A	3/1999	Green et al.
5,738,648 A	4/1998	Lands et al.	5,878,938 A	3/1999	Bittner et al.
5,743,456 A	4/1998	Jones et al.	5,891,160 A	4/1999	Williamson, IV et al.
5,747,953 A	5/1998	Philipp	5,893,506 A	4/1999	Powell
5,749,889 A	5/1998	Bacich et al.	5,894,979 A	4/1999	Powell
5,749,893 A	5/1998	Vidal et al.	5,897,562 A	4/1999	Bolanos et al.
5,752,644 A	5/1998	Bolanos et al.	5,899,914 A	5/1999	Zirps et al.
5,752,965 A	5/1998	Francis et al.	5,901,895 A	5/1999	Heaton et al.
5,755,717 A	5/1998	Yates et al.	5,902,312 A	5/1999	Frater et al.
5,758,814 A	6/1998	Gallagher et al.	5,904,693 A	5/1999	Dicesare et al.
5,762,255 A	6/1998	Chrisman et al.	5,906,625 A	5/1999	Bito et al.
5,762,256 A	6/1998	Mastri et al.	5,908,402 A	6/1999	Blythe
5,766,188 A	6/1998	Igaki	5,908,427 A	6/1999	McKean et al.
5,766,205 A	6/1998	Zvenyatsky et al.	5,911,353 A	6/1999	Bolanos et al.
5,769,892 A	6/1998	Kingwell	5,915,616 A	6/1999	Viola et al.
5,772,379 A	6/1998	Evensen	5,918,791 A	7/1999	Sorrentino et al.
5,772,578 A	6/1998	Heimberger et al.	5,919,198 A	7/1999	Graves, Jr. et al.
5,772,659 A	6/1998	Becker et al.	5,928,256 A	7/1999	Riza
5,776,130 A	7/1998	Buyse et al.	5,931,847 A	8/1999	Bittner et al.
5,779,130 A	7/1998	Alesi et al.	5,931,853 A	8/1999	McEwen et al.
5,779,131 A	7/1998	Knodel et al.	5,937,951 A	8/1999	Izuchukwu et al.
5,779,132 A	7/1998	Knodel et al.	5,938,667 A	8/1999	Peyser et al.
5,782,396 A	7/1998	Mastri et al.	5,941,442 A	8/1999	Geiste et al.
5,782,397 A	7/1998	Koukline	5,944,172 A	8/1999	Hannula
5,782,749 A	7/1998	Riza	5,944,715 A	8/1999	Goble et al.
5,782,859 A	7/1998	Nicholas et al.	5,948,030 A	9/1999	Miller et al.
5,784,934 A	7/1998	Izumisawa	5,951,552 A	9/1999	Long et al.
5,785,232 A	7/1998	Vidal et al.	5,951,574 A	9/1999	Stefanchik et al.
5,787,897 A	8/1998	Kieturakis	5,954,259 A	9/1999	Viola et al.
5,792,135 A	8/1998	Madhani et al.	5,964,774 A	10/1999	McKean et al.
5,792,165 A	8/1998	Klieman et al.	5,971,916 A	10/1999	Koren
			5,988,479 A	11/1999	Palmer
			6,003,517 A	12/1999	Sheffield et al.
			6,004,319 A	12/1999	Goble et al.
			6,010,054 A	1/2000	Johnson et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,012,494 A	1/2000	Balazs	6,261,286 B1	7/2001	Goble et al.
6,013,076 A	1/2000	Goble et al.	6,264,086 B1	7/2001	McGuckin, Jr.
6,015,406 A	1/2000	Goble et al.	6,264,087 B1	7/2001	Whitman
6,017,322 A	1/2000	Snoke et al.	6,270,508 B1	8/2001	Klieman et al.
6,017,356 A	1/2000	Frederick et al.	6,273,897 B1	8/2001	Dallessandro et al.
6,022,352 A	2/2000	Vandewalle	6,277,114 B1	8/2001	Bullivant et al.
6,024,741 A	2/2000	Williamson, IV et al.	6,293,942 B1	9/2001	Goble et al.
6,024,748 A	2/2000	Manzo et al.	6,296,640 B1	10/2001	Wampler et al.
6,027,501 A	2/2000	Goble et al.	6,302,311 B1	10/2001	Adams et al.
6,032,849 A	3/2000	Mastri et al.	6,306,134 B1	10/2001	Goble et al.
6,033,378 A	3/2000	Lundquist et al.	6,309,403 B1	10/2001	Minor et al.
6,033,399 A	3/2000	Gines	6,315,184 B1	11/2001	Whitman
6,033,427 A	3/2000	Lee	6,320,123 B1	11/2001	Reimers
6,039,733 A	3/2000	Buyse et al.	6,324,339 B1	11/2001	Hudson et al.
6,039,734 A	3/2000	Goble	6,325,799 B1	12/2001	Goble
6,045,560 A	4/2000	McKean et al.	6,325,810 B1	12/2001	Hamilton et al.
6,050,472 A	4/2000	Shibata	6,330,965 B1	12/2001	Milliman et al.
6,053,390 A	4/2000	Green et al.	6,331,181 B1	12/2001	Tierney et al.
6,056,746 A	5/2000	Goble et al.	6,331,761 B1	12/2001	Kumar et al.
6,063,097 A	5/2000	Oi et al.	6,334,860 B1	1/2002	Dorn
6,063,098 A	5/2000	Houser et al.	6,336,926 B1	1/2002	Goble
6,066,132 A	5/2000	Chen et al.	6,338,737 B1	1/2002	Toledano
6,068,627 A	5/2000	Orszulak et al.	6,346,077 B1	2/2002	Taylor et al.
6,071,233 A	6/2000	Ishikawa et al.	6,352,503 B1	3/2002	Matsui et al.
6,074,386 A	6/2000	Goble et al.	6,358,224 B1	3/2002	Tims et al.
6,077,286 A	6/2000	Cuschieri et al.	6,364,877 B1	4/2002	Goble et al.
6,079,606 A	6/2000	Milliman et al.	6,364,888 B1	4/2002	Niemeyer et al.
6,082,577 A	7/2000	Coates et al.	6,373,152 B1	4/2002	Wang et al.
6,083,234 A	7/2000	Nicholas et al.	6,387,113 B1	5/2002	Hawkins et al.
6,083,242 A	7/2000	Cook	6,387,114 B2	5/2002	Adams
6,086,600 A	7/2000	Kortenbach	6,391,038 B2	5/2002	Vargas et al.
6,090,106 A	7/2000	Goble et al.	6,398,781 B1	6/2002	Goble et al.
6,093,186 A	7/2000	Goble	6,398,797 B2	6/2002	Bombard et al.
6,099,537 A	8/2000	Sugai et al.	6,406,440 B1	6/2002	Stefanchik
6,099,551 A	8/2000	Gabbay	6,409,724 B1	6/2002	Penny et al.
6,102,271 A	8/2000	Longo et al.	H2037 H	7/2002	Yates et al.
6,109,500 A	8/2000	Alli et al.	6,416,486 B1	7/2002	Wampler
6,117,158 A	9/2000	Measamer et al.	6,416,509 B1	7/2002	Goble et al.
6,119,913 A	9/2000	Adams et al.	6,419,695 B1	7/2002	Gabbay
6,120,433 A	9/2000	Mizuno et al.	RE37,814 E	8/2002	Allgeyer
6,123,241 A	9/2000	Walter et al.	6,436,097 B1	8/2002	Nardella
6,126,058 A	10/2000	Adams et al.	6,436,107 B1	8/2002	Wang et al.
6,126,670 A	10/2000	Walker et al.	6,436,122 B1	8/2002	Frank et al.
6,131,789 A	10/2000	Schulze et al.	6,439,446 B1	8/2002	Perry et al.
6,132,368 A	10/2000	Cooper	6,440,146 B2	8/2002	Nicholas et al.
6,139,546 A	10/2000	Koenig et al.	6,443,973 B1	9/2002	Whitman
6,155,473 A	12/2000	Tompkins et al.	6,450,391 B1	9/2002	Kayan et al.
6,156,056 A	12/2000	Kearns et al.	6,468,275 B1	10/2002	Wampler et al.
6,159,146 A	12/2000	El Gazayerli	6,471,106 B1	10/2002	Reining
6,159,200 A	12/2000	Verdura et al.	6,482,200 B2	11/2002	Shippert
6,162,208 A	12/2000	Hipps	6,485,490 B2	11/2002	Wampler et al.
6,165,175 A	12/2000	Wampler et al.	6,488,196 B1	12/2002	Fenton, Jr.
6,165,184 A	12/2000	Verdura et al.	6,488,197 B1	12/2002	Whitman
6,168,605 B1	1/2001	Measamer et al.	6,491,201 B1	12/2002	Whitman
6,171,316 B1	1/2001	Kovac et al.	6,491,690 B1	12/2002	Goble et al.
6,171,330 B1	1/2001	Benchetrit	6,491,701 B2	12/2002	Tierney et al.
6,174,308 B1	1/2001	Goble et al.	6,492,785 B1	12/2002	Kasten et al.
6,174,309 B1	1/2001	Wrublewski et al.	6,494,896 B1	12/2002	D'Alessio et al.
6,179,776 B1	1/2001	Adams et al.	6,503,257 B2	1/2003	Grant et al.
6,181,105 B1	1/2001	Cutolo et al.	6,503,259 B2	1/2003	Huxel et al.
6,193,129 B1	2/2001	Bittner et al.	6,505,768 B2	1/2003	Whitman
6,197,042 B1	3/2001	Ginn et al.	6,510,854 B2	1/2003	Goble
6,202,914 B1	3/2001	Geiste et al.	6,511,468 B1	1/2003	Cragg et al.
6,214,028 B1	4/2001	Yoon et al.	6,517,535 B2	2/2003	Edwards
6,220,368 B1	4/2001	Ark et al.	6,517,565 B1	2/2003	Whitman et al.
6,223,835 B1	5/2001	Habedank et al.	6,517,566 B1	2/2003	Hovland et al.
6,228,081 B1	5/2001	Goble	6,522,101 B2	2/2003	Malackowski
6,228,084 B1	5/2001	Kirwan, Jr.	6,543,456 B1	4/2003	Freeman
6,231,565 B1	5/2001	Tovey et al.	6,547,786 B1	4/2003	Goble
6,234,178 B1	5/2001	Goble et al.	6,550,546 B2	4/2003	Thurler et al.
6,241,139 B1	6/2001	Milliman et al.	6,551,333 B2	4/2003	Kuhns et al.
6,241,723 B1	6/2001	Heim et al.	6,554,861 B2	4/2003	Knox et al.
6,249,076 B1	6/2001	Madden et al.	6,558,379 B1	5/2003	Batchelor et al.
6,250,532 B1	6/2001	Green et al.	6,565,560 B1	5/2003	Goble et al.
6,258,107 B1	7/2001	Balázs et al.	6,569,085 B2	5/2003	Kortenbach et al.
			6,569,171 B2	5/2003	DeGuillebon et al.
			6,578,751 B2	6/2003	Hartwick
			6,582,427 B1	6/2003	Goble et al.
			6,588,643 B2	7/2003	Bolduc et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,589,164	B1	7/2003	Flaherty	6,814,741	B2	11/2004	Bowman et al.
6,592,597	B2	7/2003	Grant et al.	6,817,508	B1	11/2004	Racenet et al.
6,596,432	B2	7/2003	Kawakami et al.	6,817,509	B2	11/2004	Geiste et al.
D478,665	S	8/2003	Isaacs et al.	6,817,974	B2	11/2004	Cooper et al.
D478,986	S	8/2003	Johnston et al.	6,821,273	B2	11/2004	Mollenauer
6,601,749	B2	8/2003	Sullivan et al.	6,821,284	B2	11/2004	Sturtz et al.
6,602,252	B2	8/2003	Mollenauer	6,827,725	B2	12/2004	Batchelor et al.
6,605,078	B2	8/2003	Adams	6,828,902	B2	12/2004	Casden
6,605,669	B2	8/2003	Awokola et al.	6,830,174	B2	12/2004	Hillstead et al.
6,616,686	B2	9/2003	Coleman et al.	6,832,998	B2	12/2004	Goble
6,619,529	B2	9/2003	Green et al.	6,834,001	B2	12/2004	Myono
6,620,166	B1	9/2003	Wenstrom, Jr. et al.	6,835,199	B2	12/2004	McGuckin, Jr. et al.
6,629,630	B2	10/2003	Adams	6,843,403	B2	1/2005	Whitman
6,629,974	B2	10/2003	Penny et al.	6,843,789	B2	1/2005	Goble
6,629,988	B2	10/2003	Weadock	6,846,307	B2	1/2005	Whitman et al.
6,636,412	B2	10/2003	Smith	6,846,308	B2	1/2005	Whitman et al.
6,638,108	B2	10/2003	Tachi	6,846,309	B2	1/2005	Whitman et al.
6,638,285	B2	10/2003	Gabbay	6,849,071	B2	2/2005	Whitman et al.
6,638,297	B1	10/2003	Huitema	RE38,708	E	3/2005	Bolanos et al.
6,641,528	B2	11/2003	Torii	6,866,178	B2	3/2005	Adams et al.
6,644,532	B2	11/2003	Green et al.	6,866,671	B2	3/2005	Tierney et al.
6,648,816	B2	11/2003	Irion et al.	6,872,214	B2	3/2005	Sonnenschein et al.
D484,243	S	12/2003	Ryan et al.	6,874,669	B2	4/2005	Adams et al.
D484,595	S	12/2003	Ryan et al.	6,877,647	B2	4/2005	Green et al.
D484,596	S	12/2003	Ryan et al.	6,878,106	B1	4/2005	Herrmann
6,656,193	B2	12/2003	Grant et al.	6,889,116	B2	5/2005	Jinno
6,666,875	B1	12/2003	Sakurai et al.	6,893,435	B2	5/2005	Goble
6,669,073	B2	12/2003	Milliman et al.	6,905,057	B2	6/2005	Swayze et al.
6,671,185	B2	12/2003	Duval	6,905,497	B2	6/2005	Truckai et al.
D484,977	S	1/2004	Ryan et al.	6,913,608	B2	7/2005	Liddicoat et al.
6,676,660	B2	1/2004	Wampler et al.	6,913,613	B2	7/2005	Schwarz et al.
6,679,410	B2	1/2004	Würsch et al.	6,923,803	B2	8/2005	Goble
6,681,978	B2	1/2004	Geiste et al.	6,929,641	B2	8/2005	Goble et al.
6,681,979	B2	1/2004	Whitman	6,931,830	B2	8/2005	Liao
6,682,527	B2	1/2004	Strul	6,936,042	B2	8/2005	Wallace et al.
6,682,528	B2	1/2004	Frazier et al.	6,939,358	B2	9/2005	Palacios et al.
6,685,727	B2	2/2004	Fisher et al.	6,942,662	B2	9/2005	Goble et al.
6,692,507	B2	2/2004	Pugsley et al.	6,945,444	B2	9/2005	Gresham et al.
6,695,199	B2	2/2004	Whitman	6,953,138	B1	10/2005	Dworak et al.
6,698,643	B2	3/2004	Whitman	6,953,139	B2	10/2005	Milliman et al.
6,699,235	B2	3/2004	Wallace et al.	6,959,851	B2	11/2005	Heinrich
6,704,210	B1	3/2004	Myers	6,959,852	B2	11/2005	Shelton, IV et al.
6,705,503	B1	3/2004	Pedicini et al.	6,960,163	B2	11/2005	Ewers et al.
6,712,773	B1	3/2004	Viola	6,960,220	B2	11/2005	Marino et al.
6,716,223	B2	4/2004	Leopold et al.	6,964,363	B2	11/2005	Wales et al.
6,716,232	B1	4/2004	Vidal et al.	6,966,907	B2	11/2005	Goble
6,716,233	B1	4/2004	Whitman	6,966,909	B2	11/2005	Marshall et al.
6,722,552	B2	4/2004	Fenton, Jr.	6,972,199	B2	12/2005	Lebouitz et al.
6,723,087	B2	4/2004	O'Neill et al.	6,974,462	B2	12/2005	Sater
6,723,091	B2	4/2004	Goble et al.	6,978,921	B2	12/2005	Shelton, IV et al.
6,726,697	B2	4/2004	Nicholas et al.	6,978,922	B2	12/2005	Bilotti et al.
6,740,030	B2	5/2004	Martone et al.	6,981,628	B2	1/2006	Wales
6,747,121	B2	6/2004	Gogolewski	6,981,941	B2	1/2006	Whitman et al.
6,749,560	B1	6/2004	Konstorum et al.	6,981,978	B2	1/2006	Gannoe
6,752,768	B2	6/2004	Burdorff et al.	6,984,203	B2	1/2006	Tartaglia et al.
6,752,816	B2	6/2004	Culp et al.	6,984,231	B2	1/2006	Goble et al.
6,755,195	B1	6/2004	Lemke et al.	6,986,451	B1	1/2006	Mastri et al.
6,755,338	B2	6/2004	Hahnen et al.	6,988,649	B2	1/2006	Shelton, IV et al.
6,758,846	B2	7/2004	Goble et al.	6,988,650	B2	1/2006	Schwemberger et al.
6,761,685	B2	7/2004	Adams et al.	6,990,796	B2	1/2006	Schnipke et al.
6,767,352	B2	7/2004	Field et al.	6,994,708	B2	2/2006	Manzo
6,767,356	B2	7/2004	Kanner et al.	6,997,931	B2	2/2006	Sauer et al.
6,769,594	B2	8/2004	Orban, III	7,000,818	B2	2/2006	Shelton, IV et al.
6,773,438	B1	8/2004	Knodel et al.	7,000,819	B2	2/2006	Swayze et al.
6,780,151	B2	8/2004	Grabover et al.	7,001,380	B2	2/2006	Goble
6,780,180	B1	8/2004	Goble et al.	7,001,408	B2	2/2006	Knodel et al.
6,783,524	B2	8/2004	Anderson et al.	7,008,435	B2	3/2006	Cummins
6,786,382	B1	9/2004	Hoffman	7,018,390	B2	3/2006	Turovskiy et al.
6,786,864	B2	9/2004	Matsuura et al.	7,025,743	B2	4/2006	Mann et al.
6,786,896	B1	9/2004	Madhani et al.	7,029,435	B2	4/2006	Nakao
6,790,173	B2	9/2004	Saadat et al.	7,032,798	B2	4/2006	Whitman et al.
6,793,652	B1	9/2004	Whitman et al.	7,032,799	B2	4/2006	Viola et al.
6,805,273	B2	10/2004	Bilotti et al.	7,033,356	B2	4/2006	Latterell et al.
6,806,808	B1	10/2004	Watters et al.	7,036,680	B1	5/2006	Flannery
6,808,525	B2	10/2004	Latterell et al.	7,037,344	B2	5/2006	Kagan et al.
				7,044,352	B2	5/2006	Shelton, IV et al.
				7,044,353	B2	5/2006	Mastri et al.
				7,048,687	B1	5/2006	Reuss et al.
				7,052,494	B2	5/2006	Goble et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,055,730 B2	6/2006	Ehrenfels et al.	7,211,084 B2	5/2007	Goble et al.
7,055,731 B2	6/2006	Shelton, IV et al.	7,213,736 B2	5/2007	Wales et al.
7,056,284 B2	6/2006	Martone et al.	7,214,224 B2	5/2007	Goble
7,056,330 B2	6/2006	Gayton	7,217,285 B2	5/2007	Vargas et al.
7,059,508 B2	6/2006	Shelton, IV et al.	7,220,260 B2	5/2007	Fleming et al.
7,063,712 B2	6/2006	Vargas et al.	7,220,272 B2	5/2007	Weadock
7,066,879 B2	6/2006	Fowler et al.	7,225,963 B2	6/2007	Scirica
7,066,944 B2	6/2006	Laufer et al.	7,225,964 B2	6/2007	Mastri et al.
7,070,083 B2	7/2006	Jankowski	7,234,624 B2	6/2007	Gresham et al.
7,070,559 B2	7/2006	Adams et al.	7,235,089 B1	6/2007	McGuckin, Jr.
7,071,287 B2	7/2006	Rhine et al.	7,235,302 B2	6/2007	Jing et al.
7,075,770 B1	7/2006	Smith	7,237,708 B1	7/2007	Guy et al.
7,077,856 B2	7/2006	Whitman	7,238,195 B2	7/2007	Viola
7,080,769 B2	7/2006	Vresh et al.	7,241,288 B2	7/2007	Braun
7,081,114 B2	7/2006	Rashidi	7,246,734 B2	7/2007	Shelton, IV
7,083,073 B2	8/2006	Yoshie et al.	7,247,161 B2	7/2007	Johnston et al.
7,083,075 B2	8/2006	Swayze et al.	7,252,660 B2	8/2007	Kunz
7,083,571 B2	8/2006	Wang et al.	7,255,696 B2	8/2007	Goble et al.
7,083,615 B2	8/2006	Peterson et al.	7,256,695 B2	8/2007	Hamel et al.
7,087,071 B2	8/2006	Nicholas et al.	7,258,262 B2	8/2007	Mastri et al.
7,090,637 B2	8/2006	Danitz et al.	7,260,431 B2	8/2007	Libbus et al.
7,090,673 B2	8/2006	Dycus et al.	7,265,374 B2	9/2007	Lee et al.
7,090,683 B2	8/2006	Brock et al.	7,267,679 B2	9/2007	McGuckin, Jr. et al.
7,090,684 B2	8/2006	McGuckin, Jr. et al.	7,273,483 B2	9/2007	Wiener et al.
7,094,202 B2	8/2006	Nobis et al.	7,278,562 B2	10/2007	Mastri et al.
7,094,247 B2	8/2006	Monassevitch et al.	7,278,563 B1	10/2007	Green
7,097,089 B2	8/2006	Marczyk	7,278,994 B2	10/2007	Goble
7,098,794 B2	8/2006	Lindsay et al.	7,282,048 B2	10/2007	Goble et al.
7,104,741 B2	9/2006	Krohn	7,295,907 B2	11/2007	Lu et al.
7,108,695 B2	9/2006	Witt et al.	7,296,724 B2	11/2007	Green et al.
7,108,701 B2	9/2006	Evens et al.	7,297,149 B2	11/2007	Vitali et al.
7,108,709 B2	9/2006	Cummins	7,300,450 B2	11/2007	Vleugels et al.
7,111,769 B2	9/2006	Wales et al.	7,303,106 B2	12/2007	Milliman et al.
7,112,214 B2	9/2006	Peterson et al.	7,303,107 B2	12/2007	Milliman et al.
RE39,358 E	10/2006	Goble	7,303,108 B2	12/2007	Shelton, IV
7,114,642 B2	10/2006	Whitman	7,303,556 B2	12/2007	Metzger
7,118,582 B1	10/2006	Wang et al.	7,308,998 B2	12/2007	Mastri et al.
7,121,446 B2	10/2006	Arad et al.	7,322,975 B2	1/2008	Goble et al.
7,122,028 B2	10/2006	Looper et al.	7,324,572 B2	1/2008	Chang
7,128,253 B2	10/2006	Mastri et al.	7,328,828 B2	2/2008	Ortiz et al.
7,128,254 B2	10/2006	Shelton, IV et al.	7,328,829 B2	2/2008	Arad et al.
7,128,748 B2	10/2006	Mooradian et al.	7,330,004 B2	2/2008	DeJonge et al.
7,131,445 B2	11/2006	Amoah	7,334,717 B2	2/2008	Rethy et al.
7,133,601 B2	11/2006	Phillips et al.	7,336,184 B2	2/2008	Smith et al.
7,140,527 B2	11/2006	Ehrenfels et al.	7,338,513 B2	3/2008	Lee et al.
7,140,528 B2	11/2006	Shelton, IV	7,343,920 B2	3/2008	Toby et al.
7,143,923 B2	12/2006	Shelton, IV et al.	7,348,763 B1	3/2008	Reinhart et al.
7,143,924 B2	12/2006	Scirica et al.	7,351,258 B2	4/2008	Ricotta et al.
7,143,925 B2	12/2006	Shelton, IV et al.	7,354,447 B2	4/2008	Shelton, IV et al.
7,143,926 B2	12/2006	Shelton, IV et al.	7,357,287 B2	4/2008	Shelton, IV et al.
7,147,138 B2	12/2006	Shelton, IV	7,364,060 B2	4/2008	Milliman
7,147,139 B2	12/2006	Schwemmerberger et al.	7,364,061 B2	4/2008	Swayze et al.
7,147,637 B2	12/2006	Goble	7,377,928 B2	5/2008	Zubik et al.
7,147,650 B2	12/2006	Lee	7,380,695 B2	6/2008	Doll et al.
7,150,748 B2	12/2006	Ebbutt et al.	7,380,696 B2	6/2008	Shelton, IV et al.
7,153,300 B2	12/2006	Goble	7,388,217 B2	6/2008	Buschbeck et al.
7,156,863 B2	1/2007	Sonnenschein et al.	7,396,356 B2	7/2008	Mollenauer
7,159,750 B2	1/2007	Racenet et al.	7,397,364 B2	7/2008	Govari
7,160,299 B2	1/2007	Baily	7,398,907 B2	7/2008	Racenet et al.
7,161,036 B2	1/2007	Oikawa et al.	7,398,908 B2	7/2008	Holsten et al.
7,168,604 B2	1/2007	Milliman et al.	7,401,721 B2	7/2008	Holsten et al.
7,172,104 B2	2/2007	Scirica et al.	7,404,508 B2	7/2008	Smith et al.
7,179,223 B2	2/2007	Motoki et al.	7,404,509 B2	7/2008	Ortiz et al.
7,179,267 B2	2/2007	Nolan et al.	7,407,075 B2	8/2008	Holsten et al.
7,182,239 B1	2/2007	Myers	7,407,078 B2	8/2008	Shelton, IV et al.
7,188,758 B2	3/2007	Viola et al.	7,410,086 B2	8/2008	Ortiz et al.
7,189,207 B2	3/2007	Viola	7,416,101 B2	8/2008	Shelton, IV et al.
7,195,627 B2	3/2007	Amoah et al.	7,418,078 B2	8/2008	Blanz et al.
7,204,835 B2	4/2007	Latterell et al.	7,419,080 B2	9/2008	Smith et al.
7,207,233 B2	4/2007	Wadge	7,422,136 B1	9/2008	Marczyk
7,207,471 B2	4/2007	Heinrich et al.	7,422,139 B2	9/2008	Shelton, IV et al.
7,207,472 B2	4/2007	Wukusick et al.	7,424,965 B2	9/2008	Racenet et al.
7,208,005 B2	4/2007	Frecker et al.	7,431,188 B1	10/2008	Marczyk
7,210,609 B2	5/2007	Leiboff et al.	7,431,189 B2	10/2008	Shelton, IV et al.
7,211,081 B2	5/2007	Goble	7,431,694 B2	10/2008	Stefanchik et al.
			7,431,730 B2	10/2008	Viola
			7,434,715 B2	10/2008	Shelton, IV et al.
			7,434,717 B2	10/2008	Shelton, IV et al.
			7,438,209 B1	10/2008	Hess et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,439,354	B2	10/2008	Lenges et al.	7,714,239	B2	5/2010	Smith
7,441,684	B2	10/2008	Shelton, IV et al.	7,721,930	B2	5/2010	McKenna et al.
7,441,685	B1	10/2008	Boudreaux	7,722,610	B2	5/2010	Viola et al.
7,442,201	B2	10/2008	Pugsley et al.	7,726,537	B2	6/2010	Olson et al.
7,448,525	B2	11/2008	Shelton, IV et al.	7,726,538	B2	6/2010	Holsten et al.
7,455,208	B2	11/2008	Wales et al.	7,743,960	B2	6/2010	Whitman et al.
7,455,676	B2	11/2008	Holsten et al.	7,744,627	B2	6/2010	Orban, III et al.
7,461,767	B2	12/2008	Viola et al.	7,766,821	B2	8/2010	Brunnen et al.
7,464,846	B2	12/2008	Shelton, IV et al.	7,766,894	B2	8/2010	Weitzner et al.
7,464,847	B2	12/2008	Viola et al.	7,771,396	B2	8/2010	Stefanchik et al.
7,464,849	B2	12/2008	Shelton, IV et al.	7,772,720	B2	8/2010	McGee et al.
7,467,740	B2	12/2008	Shelton, IV et al.	7,776,060	B2	8/2010	Mooradian et al.
7,467,849	B2	12/2008	Silverbrook et al.	7,780,054	B2	8/2010	Wales
7,472,814	B2	1/2009	Mastri et al.	7,780,055	B2	8/2010	Scirica et al.
7,472,815	B2	1/2009	Shelton, IV et al.	7,780,663	B2	8/2010	Yates et al.
7,473,253	B2	1/2009	Dycus et al.	7,780,685	B2	8/2010	Hunt et al.
7,479,608	B2	1/2009	Smith	7,784,662	B2	8/2010	Wales et al.
7,481,347	B2	1/2009	Roy	7,803,151	B2	9/2010	Whitman
7,481,349	B2	1/2009	Holsten et al.	7,806,891	B2	10/2010	Nowlin et al.
7,481,824	B2	1/2009	Boudreaux et al.	7,815,092	B2	10/2010	Whitman et al.
7,485,133	B2	2/2009	Cannon et al.	7,815,565	B2	10/2010	Stefanchik et al.
7,490,749	B2	2/2009	Schall et al.	7,824,401	B2	11/2010	Manzo et al.
7,494,039	B2	2/2009	Racenet et al.	7,828,189	B2	11/2010	Holsten et al.
7,494,499	B2	2/2009	Nagase et al.	7,828,794	B2	11/2010	Sartor
7,500,979	B2	3/2009	Hueil et al.	7,828,808	B2	11/2010	Hinman et al.
7,501,198	B2	3/2009	Barlev et al.	7,832,611	B2	11/2010	Boyden et al.
7,506,790	B2	3/2009	Shelton, IV	7,836,400	B2	11/2010	May et al.
7,506,791	B2	3/2009	Omaits et al.	7,837,081	B2	11/2010	Holsten et al.
7,510,107	B2	3/2009	Timm et al.	7,845,533	B2	12/2010	Marczyk et al.
7,524,320	B2	4/2009	Tierney et al.	7,845,534	B2	12/2010	Viola et al.
7,530,985	B2	5/2009	Takemoto et al.	7,846,149	B2	12/2010	Jankowski
7,546,940	B2	6/2009	Milliman et al.	7,870,989	B2	1/2011	Viola et al.
7,547,312	B2	6/2009	Bauman et al.	7,871,418	B2	1/2011	Thompson et al.
7,549,563	B2	6/2009	Mather et al.	7,887,530	B2	2/2011	Zemlok et al.
7,549,564	B2	6/2009	Boudreaux	7,905,380	B2	3/2011	Shelton, IV et al.
7,552,854	B2	6/2009	Wixey et al.	7,905,381	B2	3/2011	Baxter, III et al.
7,556,185	B2	7/2009	Viola	7,909,191	B2	3/2011	Baker et al.
7,556,186	B2	7/2009	Milliman	7,909,221	B2	3/2011	Viola et al.
7,559,450	B2	7/2009	Wales et al.	7,913,891	B2	3/2011	Doll et al.
7,559,452	B2	7/2009	Wales et al.	7,914,543	B2	3/2011	Roth et al.
7,563,862	B2	7/2009	Sieg et al.	7,918,376	B1	4/2011	Knodel et al.
7,566,300	B2	7/2009	Devierre et al.	7,918,377	B2	4/2011	Measamer et al.
7,568,603	B2	8/2009	Shelton, IV et al.	7,922,061	B2	4/2011	Shelton, IV et al.
7,568,604	B2	8/2009	Ehrenfels et al.	7,922,063	B2	4/2011	Zemlok et al.
7,568,619	B2	8/2009	Todd et al.	7,934,630	B2	5/2011	Shelton, IV et al.
7,575,144	B2	8/2009	Ortiz et al.	7,938,307	B2	5/2011	Bettuchi
7,588,175	B2	9/2009	Timm et al.	7,941,865	B2	5/2011	Seman, Jr. et al.
7,588,176	B2	9/2009	Timm et al.	7,942,303	B2	5/2011	Shah
7,597,229	B2	10/2009	Boudreaux et al.	7,942,890	B2	5/2011	D'Agostino et al.
7,600,663	B2	10/2009	Green	7,944,175	B2	5/2011	Mori et al.
7,604,150	B2	10/2009	Boudreaux	7,950,560	B2	5/2011	Zemlok et al.
7,604,151	B2	10/2009	Hess et al.	7,954,682	B2	6/2011	Giordano et al.
7,607,557	B2	10/2009	Shelton, IV et al.	7,954,684	B2	6/2011	Boudreaux
7,611,038	B2	11/2009	Racenet et al.	7,954,686	B2	6/2011	Baxter, III et al.
7,615,003	B2	11/2009	Stefanchik et al.	7,959,050	B2	6/2011	Smith et al.
7,624,902	B2	12/2009	Marczyk et al.	7,963,963	B2	6/2011	Francischelli et al.
7,631,793	B2	12/2009	Rethy et al.	7,967,180	B2	6/2011	Scirica
7,635,074	B2	12/2009	Olson et al.	7,972,298	B2	7/2011	Wallace et al.
7,637,409	B2	12/2009	Marczyk	7,997,469	B2	8/2011	Olson et al.
7,641,092	B2	1/2010	Kruszynski et al.	8,002,795	B2	8/2011	Beetel
7,641,093	B2	1/2010	Doll et al.	8,011,551	B2	9/2011	Marczyk et al.
7,644,848	B2	1/2010	Swayze et al.	8,011,555	B2	9/2011	Tarinelli et al.
7,651,498	B2	1/2010	Shifrin et al.	8,025,199	B2	9/2011	Whitman et al.
7,656,131	B2	2/2010	Embrey et al.	8,028,883	B2	10/2011	Stopek
7,658,312	B2	2/2010	Vidal et al.	8,034,077	B2	10/2011	Smith et al.
7,665,646	B2	2/2010	Prommersberger	8,038,045	B2	10/2011	Bettuchi et al.
7,674,255	B2	3/2010	Braun	8,038,046	B2	10/2011	Smith et al.
7,682,307	B2	3/2010	Danitz et al.	8,062,330	B2	11/2011	Prommersberger et al.
7,686,826	B2	3/2010	Lee et al.	D650,074	S	12/2011	Hunt et al.
7,688,028	B2	3/2010	Phillips et al.	8,091,756	B2	1/2012	Viola
7,691,098	B2	4/2010	Wallace et al.	8,097,017	B2	1/2012	Viola
7,699,204	B2	4/2010	Viola	8,108,072	B2	1/2012	Zhao et al.
7,699,859	B2	4/2010	Bombard et al.	8,113,410	B2	2/2012	Hall et al.
7,708,180	B2	5/2010	Murray et al.	8,123,103	B2	2/2012	Milliman
7,708,758	B2	5/2010	Lee et al.	8,136,712	B2	3/2012	Zingman
				8,141,762	B2	3/2012	Bedi et al.
				8,152,041	B2	4/2012	Kostrzewski
				8,157,152	B2	4/2012	Holsten et al.
				8,157,153	B2	4/2012	Shelton, IV et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

8,167,185 B2	5/2012	Shelton, IV et al.	2005/0103819 A1	5/2005	Racenet et al.
8,167,895 B2	5/2012	D'Agostino et al.	2005/0107814 A1	5/2005	Johnston et al.
8,172,124 B2	5/2012	Shelton, IV et al.	2005/0107824 A1	5/2005	Hillstead et al.
8,196,795 B2	6/2012	Moore et al.	2005/0113820 A1	5/2005	Goble et al.
8,196,796 B2	6/2012	Shelton, IV et al.	2005/0119525 A1	6/2005	Takemoto
8,205,781 B2	6/2012	Baxter, III et al.	2005/0119669 A1	6/2005	Demmy
8,211,125 B2	7/2012	Spivey	2005/0124855 A1	6/2005	Jaffe et al.
8,220,468 B2	7/2012	Cooper et al.	2005/0125009 A1	6/2005	Perry et al.
8,225,799 B2	7/2012	Bettuchi	2005/0131173 A1	6/2005	McDaniel et al.
8,241,271 B2	8/2012	Millman et al.	2005/0131211 A1	6/2005	Bayley et al.
8,245,898 B2	8/2012	Smith et al.	2005/0131390 A1	6/2005	Heinrich et al.
8,245,901 B2	8/2012	Stopek	2005/0131436 A1	6/2005	Johnston et al.
8,256,654 B2	9/2012	Bettuchi et al.	2005/0131437 A1	6/2005	Johnston et al.
8,257,391 B2	9/2012	Orban, III et al.	2005/0131457 A1	6/2005	Douglas et al.
8,372,094 B2	2/2013	Bettuchi et al.	2005/0137454 A1	6/2005	Saadat et al.
2002/0022836 A1	2/2002	Goble et al.	2005/0137455 A1	6/2005	Ewers et al.
2002/0029036 A1	3/2002	Goble et al.	2005/0143759 A1	6/2005	Kelly
2002/0117534 A1	8/2002	Green et al.	2005/0145675 A1	7/2005	Hartwick et al.
2002/0134811 A1	9/2002	Napier et al.	2005/0154258 A1	7/2005	Tartaglia et al.
2002/0165541 A1	11/2002	Whitman	2005/0165419 A1	7/2005	Sauer et al.
2003/0093103 A1	5/2003	Malackowski et al.	2005/0165435 A1	7/2005	Johnston et al.
2003/0105478 A1	6/2003	Whitman et al.	2005/0169974 A1	8/2005	Tenerz et al.
2003/0130677 A1	7/2003	Whitman et al.	2005/0171522 A1	8/2005	Christopherson
2003/0139741 A1	7/2003	Goble et al.	2005/0177181 A1	8/2005	Kagan et al.
2003/0153908 A1	8/2003	Goble et al.	2005/0182298 A1	8/2005	Ikeda et al.
2003/0195387 A1	10/2003	Kortenbach et al.	2005/0184121 A1	8/2005	Heinrich
2003/0205029 A1	11/2003	Chapolini et al.	2005/0187545 A1	8/2005	Hooven et al.
2003/0216732 A1	11/2003	Truckai et al.	2005/0187572 A1	8/2005	Johnston et al.
2003/0220660 A1	11/2003	Kortenbach et al.	2005/0187576 A1	8/2005	Whitman et al.
2004/0002726 A1	1/2004	Nunez et al.	2005/0189397 A1	9/2005	Jankowski
2004/0006335 A1	1/2004	Garrison	2005/0192609 A1	9/2005	Whitman et al.
2004/0006340 A1	1/2004	Latterell et al.	2005/0192628 A1	9/2005	Viola
2004/0006372 A1	1/2004	Racenet et al.	2005/0203550 A1	9/2005	Laufer et al.
2004/0030333 A1	2/2004	Goble	2005/0216055 A1	9/2005	Scirica et al.
2004/0034357 A1	2/2004	Beane et al.	2005/0228224 A1	10/2005	Okada et al.
2004/0034369 A1	2/2004	Sauer et al.	2005/0240222 A1	10/2005	Shipp
2004/0044364 A1	3/2004	DeVries et al.	2005/0245965 A1	11/2005	Orban, III et al.
2004/0068161 A1	4/2004	Couvillon, Jr.	2005/0251128 A1	11/2005	Amoah
2004/0068307 A1	4/2004	Goble	2005/0256452 A1	11/2005	DeMarchi et al.
2004/0070369 A1	4/2004	Sakahibara	2005/0256522 A1	11/2005	Francischelli et al.
2004/0078037 A1	4/2004	Batchelor et al.	2005/0261676 A1	11/2005	Hall et al.
2004/0093024 A1	5/2004	Lousararian et al.	2005/0261677 A1	11/2005	Hall et al.
2004/0094597 A1	5/2004	Whitman et al.	2005/0263563 A1	12/2005	Racenet et al.
2004/0097987 A1	5/2004	Pugsley et al.	2005/0267455 A1	12/2005	Eggers et al.
2004/0101822 A1	5/2004	Weisner et al.	2005/0274768 A1	12/2005	Cummins et al.
2004/0108357 A1	6/2004	Milliman et al.	2006/0004407 A1	1/2006	Hiles et al.
2004/0111081 A1	6/2004	Whitman et al.	2006/0008787 A1	1/2006	Hayman et al.
2004/0115022 A1	6/2004	Albertson et al.	2006/0011699 A1	1/2006	Olson et al.
2004/0116952 A1	6/2004	Sakurai et al.	2006/0015009 A1	1/2006	Jaffe et al.
2004/0147909 A1	7/2004	Johnston et al.	2006/0020247 A1	1/2006	Kagan et al.
2004/0164123 A1	8/2004	Racenet et al.	2006/0020258 A1	1/2006	Strauss et al.
2004/0167572 A1	8/2004	Roth et al.	2006/0020336 A1	1/2006	Liddicoat
2004/0173659 A1	9/2004	Green et al.	2006/0025811 A1	2/2006	Shelton
2004/0181219 A1	9/2004	Goble et al.	2006/0025812 A1	2/2006	Shelton
2004/0186470 A1	9/2004	Goble et al.	2006/0025813 A1	2/2006	Shelton et al.
2004/0193189 A1	9/2004	Kortenbach et al.	2006/0041188 A1	2/2006	Dirusso et al.
2004/0222268 A1	11/2004	Bilotti et al.	2006/0047275 A1	3/2006	Goble
2004/0230214 A1	11/2004	Donofrio et al.	2006/0047303 A1	3/2006	Ortiz et al.
2004/0232197 A1 *	11/2004	Shelton et al. 227/175.1	2006/0047307 A1	3/2006	Ortiz et al.
2004/0232201 A1	11/2004	Wenchell et al.	2006/0049229 A1	3/2006	Milliman et al.
2004/0243151 A1	12/2004	Demmy et al.	2006/0052825 A1	3/2006	Ransick et al.
2004/0243163 A1	12/2004	Casiano et al.	2006/0060630 A1	3/2006	Shelton et al.
2004/0243176 A1	12/2004	Hahnen et al.	2006/0064086 A1	3/2006	Odom
2004/0254566 A1	12/2004	Plicchi et al.	2006/0079735 A1	4/2006	Martone et al.
2004/0254608 A1	12/2004	Huitema et al.	2006/0085031 A1	4/2006	Bettuchi
2004/0260315 A1	12/2004	Dell et al.	2006/0085033 A1	4/2006	Criscuolo et al.
2004/0267310 A1	12/2004	Racenet et al.	2006/0086032 A1	4/2006	Valencic et al.
2005/0032511 A1	2/2005	Malone et al.	2006/0100643 A1	5/2006	Laufer et al.
2005/0033357 A1	2/2005	Braun	2006/0108393 A1	5/2006	Heinrich et al.
2005/0054946 A1	3/2005	Krzyzanowski	2006/0111711 A1	5/2006	Goble
2005/0059997 A1	3/2005	Bauman et al.	2006/0111723 A1	5/2006	Chapolini et al.
2005/0070929 A1	3/2005	Dalessandro et al.	2006/0122636 A1	6/2006	Bailly et al.
2005/0080454 A1	4/2005	Drews et al.	2006/0142772 A1	6/2006	Ralph et al.
2005/0085693 A1	4/2005	Belson et al.	2006/0149163 A1	7/2006	Hibner et al.
2005/0090817 A1	4/2005	Phan	2006/0161185 A1	7/2006	Saadat et al.
			2006/0173470 A1	8/2006	Oray et al.
			2006/0180634 A1	8/2006	Shelton, IV et al.
			2006/0183246 A1	8/2006	Wiesner et al.
			2006/0200123 A1	9/2006	Ryan

(56)

References Cited

U.S. PATENT DOCUMENTS

2006/0212069	A1	9/2006	Shelton, IV	2008/0015598	A1	1/2008	Prommersberger
2006/0217729	A1	9/2006	Eskridge et al.	2008/0029570	A1	2/2008	Shelton et al.
2006/0226196	A1	10/2006	Hueil et al.	2008/0029573	A1	2/2008	Shelton et al.
2006/0235469	A1	10/2006	Viola	2008/0029574	A1	2/2008	Shelton et al.
2006/0241655	A1	10/2006	Viola	2008/0029575	A1	2/2008	Shelton et al.
2006/0241692	A1	10/2006	McGuckin, Jr. et al.	2008/0029576	A1	2/2008	Shelton et al.
2006/0244460	A1	11/2006	Weaver	2008/0030170	A1	2/2008	Dacquay et al.
2006/0245971	A1	11/2006	Burns et al.	2008/0035701	A1	2/2008	Racenet et al.
2006/0258904	A1	11/2006	Stefanchik et al.	2008/0041916	A1	2/2008	Milliman et al.
2006/0259073	A1	11/2006	Miyamoto et al.	2008/0041917	A1	2/2008	Racenet et al.
2006/0264927	A1	11/2006	Ryan	2008/0078800	A1	4/2008	Hess et al.
2006/0264929	A1	11/2006	Goble et al.	2008/0078801	A1	4/2008	Shelton et al.
2006/0271042	A1	11/2006	Latterell et al.	2008/0078802	A1	4/2008	Hess et al.
2006/0271102	A1	11/2006	Bosshard et al.	2008/0078803	A1	4/2008	Shelton et al.
2006/0273135	A1	12/2006	Beetel	2008/0078804	A1	4/2008	Shelton et al.
2006/0278680	A1	12/2006	Viola et al.	2008/0078806	A1	4/2008	Omaits et al.
2006/0278681	A1	12/2006	Viola et al.	2008/0078807	A1	4/2008	Hess et al.
2006/0284730	A1	12/2006	Schmid et al.	2008/0078808	A1	4/2008	Hess et al.
2006/0289602	A1	12/2006	Wales et al.	2008/0082114	A1	4/2008	McKenna et al.
2006/0291981	A1	12/2006	Viola et al.	2008/0082115	A1	4/2008	Morgan et al.
2007/0023476	A1	2/2007	Whitman et al.	2008/0082124	A1	4/2008	Hess et al.
2007/0023477	A1	2/2007	Whitman et al.	2008/0082125	A1	4/2008	Murray et al.
2007/0027468	A1	2/2007	Wales et al.	2008/0082126	A1	4/2008	Murray et al.
2007/0027469	A1	2/2007	Smith et al.	2008/0083813	A1	4/2008	Zemlok et al.
2007/0034668	A1	2/2007	Holsten et al.	2008/0114385	A1	5/2008	Byrum et al.
2007/0045379	A1	3/2007	Shelton, IV	2008/0129253	A1	6/2008	Shiue et al.
2007/0055219	A1	3/2007	Whitman et al.	2008/0140115	A1	6/2008	Stopek
2007/0070574	A1	3/2007	Nerheim et al.	2008/0164296	A1	7/2008	Shelton et al.
2007/0073341	A1	3/2007	Smith	2008/0167644	A1	7/2008	Shelton et al.
2007/0078484	A1	4/2007	Talarico et al.	2008/0167670	A1	7/2008	Shelton et al.
2007/0083193	A1	4/2007	Werneth et al.	2008/0167671	A1	7/2008	Giordano et al.
2007/0084897	A1	4/2007	Shelton, IV et al.	2008/0167672	A1	7/2008	Giordano et al.
2007/0102453	A1	5/2007	Morgan et al.	2008/0167736	A1	7/2008	Swayze et al.
2007/0102472	A1	5/2007	Shelton, IV	2008/0169328	A1	7/2008	Shelton
2007/0102473	A1	5/2007	Shelton, IV et al.	2008/0169329	A1	7/2008	Shelton et al.
2007/0102474	A1	5/2007	Shelton, IV et al.	2008/0169330	A1	7/2008	Shelton et al.
2007/0106113	A1	5/2007	Ravo	2008/0169331	A1	7/2008	Shelton et al.
2007/0106317	A1	5/2007	Shelton, IV et al.	2008/0169332	A1	7/2008	Shelton et al.
2007/0114261	A1	5/2007	Ortiz et al.	2008/0169333	A1	7/2008	Shelton et al.
2007/0118175	A1	5/2007	Butler et al.	2008/0172087	A1	7/2008	Fuchs et al.
2007/0129605	A1	6/2007	Schaaf	2008/0172088	A1	7/2008	Smith et al.
2007/0135803	A1	6/2007	Belson	2008/0183193	A1	7/2008	Omori et al.
2007/0158358	A1	7/2007	Mason et al.	2008/0185419	A1	8/2008	Smith et al.
2007/0158385	A1	7/2007	Hueil et al.	2008/0197167	A1	8/2008	Viola et al.
2007/0170225	A1	7/2007	Shelton, IV et al.	2008/0200835	A1	8/2008	Monson et al.
2007/0173806	A1	7/2007	Orszulak et al.	2008/0210738	A1	9/2008	Shelton et al.
2007/0173813	A1	7/2007	Odom	2008/0228029	A1	9/2008	Mikkaichi et al.
2007/0175949	A1	8/2007	Shelton, IV et al.	2008/0237296	A1	10/2008	Boudreaux et al.
2007/0175950	A1	8/2007	Shelton, IV et al.	2008/0245841	A1	10/2008	Smith et al.
2007/0175951	A1	8/2007	Shelton, IV et al.	2008/0251568	A1	10/2008	Zemlok et al.
2007/0175953	A1	8/2007	Shelton, IV et al.	2008/0251569	A1	10/2008	Smith et al.
2007/0175955	A1	8/2007	Shelton, IV et al.	2008/0255413	A1	10/2008	Zemlok et al.
2007/0175957	A1	8/2007	Shelton, IV et al.	2008/0262654	A1	10/2008	Omori et al.
2007/0175958	A1	8/2007	Shelton, IV et al.	2008/0283570	A1	11/2008	Boyden et al.
2007/0175964	A1	8/2007	Shelton, IV et al.	2008/0287944	A1	11/2008	Pearson et al.
2007/0179476	A1	8/2007	Shelton, IV et al.	2008/0290134	A1	11/2008	Bettuchi et al.
2007/0181632	A1	8/2007	Milliman	2008/0296343	A1	12/2008	Schall et al.
2007/0194079	A1	8/2007	Hueil et al.	2008/0296345	A1	12/2008	Shelton, IV et al.
2007/0194080	A1	8/2007	Swayze et al.	2008/0296346	A1	12/2008	Shelton, IV et al.
2007/0194081	A1	8/2007	Hueil et al.	2008/0296347	A1	12/2008	Shelton, IV et al.
2007/0194082	A1	8/2007	Morgan et al.	2008/0300579	A1	12/2008	Broehl et al.
2007/0203510	A1	8/2007	Bettuchi	2008/0300580	A1	12/2008	Shelton, IV et al.
2007/0213750	A1	9/2007	Weadock	2008/0300613	A1	12/2008	Shelton, IV et al.
2007/0221700	A1	9/2007	Ortiz et al.	2008/0308601	A1	12/2008	Timm et al.
2007/0221701	A1	9/2007	Ortiz et al.	2008/0308602	A1	12/2008	Timm et al.
2007/0225562	A1	9/2007	Spivey et al.	2008/0308603	A1	12/2008	Shelton, IV et al.
2007/0233053	A1	10/2007	Shelton, IV et al.	2008/0308608	A1	12/2008	Prommersberger
2007/0239028	A1	10/2007	Houser et al.	2008/0314954	A1	12/2008	Boudreaux
2007/0246505	A1	10/2007	Pace-Florida et al.	2008/0314955	A1	12/2008	Boudreaux et al.
2007/0260278	A1	11/2007	Wheeler et al.	2008/0314957	A1	12/2008	Boudreaux
2007/0270784	A1	11/2007	Smith et al.	2008/0314960	A1	12/2008	Marczyk et al.
2007/0270884	A1	11/2007	Smith et al.	2009/0001121	A1	1/2009	Hess et al.
2007/0288044	A1	12/2007	Jinno et al.	2009/0001122	A1	1/2009	Prommersberger et al.
2007/0295780	A1	12/2007	Shelton et al.	2009/0001123	A1	1/2009	Morgan et al.
2007/0299427	A1	12/2007	Yeung et al.	2009/0001124	A1	1/2009	Hess et al.
				2009/0001125	A1	1/2009	Hess et al.
				2009/0001128	A1	1/2009	Weisenburgh, II et al.
				2009/0001130	A1	1/2009	Hess et al.
				2009/0005807	A1	1/2009	Hess et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2009/0005808	A1	1/2009	Hess et al.	2010/0127042	A1	5/2010	Shelton, IV
2009/0005809	A1	1/2009	Hess et al.	2010/0133317	A1	6/2010	Shelton, IV et al.
2009/0012534	A1	1/2009	Madhani et al.	2010/0133318	A1	6/2010	Boudreaux
2009/0012556	A1	1/2009	Boudreaux et al.	2010/0145146	A1	6/2010	Melder
2009/0020958	A1	1/2009	Soul	2010/0147922	A1	6/2010	Olson
2009/0054908	A1	2/2009	Zand et al.	2010/0163598	A1	7/2010	Belzer
2009/0057369	A1	3/2009	Smith et al.	2010/0179382	A1	7/2010	Shelton, IV et al.
2009/0076534	A1	3/2009	Shelton, IV et al.	2010/0181364	A1	7/2010	Shelton, IV et al.
2009/0078736	A1	3/2009	Van Lue	2010/0186219	A1	7/2010	Smith
2009/0088774	A1	4/2009	Swarup et al.	2010/0193566	A1	8/2010	Scheib et al.
2009/0090763	A1	4/2009	Zemlok et al.	2010/0193567	A1	8/2010	Scheib et al.
2009/0093728	A1	4/2009	Hyde et al.	2010/0193568	A1	8/2010	Scheib et al.
2009/0108048	A1	4/2009	Zemlok et al.	2010/0193569	A1	8/2010	Yates et al.
2009/0112229	A1	4/2009	Omori et al.	2010/0198220	A1	8/2010	Boudreaux et al.
2009/0114701	A1	5/2009	Zemlok et al.	2010/0200637	A1	8/2010	Beetel
2009/0143805	A1	6/2009	Palmer et al.	2010/0213241	A1	8/2010	Bedi
2009/0149871	A9	6/2009	Kagan et al.	2010/0222901	A1	9/2010	Swayze et al.
2009/0157067	A1	6/2009	Kane et al.	2010/0224669	A1	9/2010	Shelton, IV et al.
2009/0200355	A1	8/2009	Baxter, III et al.	2010/0230465	A1	9/2010	Smith et al.
2009/0206123	A1	8/2009	Doll et al.	2010/0237132	A1	9/2010	Measamer et al.
2009/0206124	A1	8/2009	Hall et al.	2010/0243707	A1	9/2010	Olson et al.
2009/0206125	A1	8/2009	Huitema et al.	2010/0243708	A1	9/2010	Aranyi et al.
2009/0206126	A1	8/2009	Huitema et al.	2010/0243709	A1	9/2010	Hess et al.
2009/0206128	A1	8/2009	Hueil et al.	2010/0258611	A1	10/2010	Smith et al.
2009/0206129	A1	8/2009	Doll et al.	2010/0264193	A1	10/2010	Huang et al.
2009/0206130	A1	8/2009	Hall et al.	2010/0264194	A1	10/2010	Huang et al.
2009/0206131	A1	8/2009	Weisenburgh, II et al.	2010/0276471	A1	11/2010	Whitman
2009/0206132	A1	8/2009	Hueil et al.	2010/0294827	A1	11/2010	Boyden et al.
2009/0206133	A1	8/2009	Morgan et al.	2010/0294829	A1	11/2010	Giordano et al.
2009/0206134	A1	8/2009	Swayze et al.	2010/0301095	A1	12/2010	Shelton, IV et al.
2009/0206135	A1	8/2009	Hall et al.	2010/0305552	A1	12/2010	Shelton, IV et al.
2009/0206136	A1	8/2009	Moore et al.	2010/0308100	A1	12/2010	Boudreaux
2009/0206137	A1	8/2009	Hall et al.	2010/0312261	A1	12/2010	Suzuki et al.
2009/0206138	A1	8/2009	Smith et al.	2011/0006099	A1	1/2011	Hall et al.
2009/0206139	A1	8/2009	Hall et al.	2011/0006101	A1	1/2011	Hall et al.
2009/0206140	A1	8/2009	Scheib et al.	2011/0006103	A1	1/2011	Laurent et al.
2009/0206141	A1	8/2009	Huitema et al.	2011/0011914	A1	1/2011	Baxter, III et al.
2009/0206142	A1	8/2009	Huitema et al.	2011/0011915	A1	1/2011	Shelton, IV
2009/0206143	A1	8/2009	Huitema et al.	2011/0017801	A1	1/2011	Zemlok et al.
2009/0206144	A1	8/2009	Doll et al.	2011/0022032	A1	1/2011	Zemlok et al.
2009/0209946	A1	8/2009	Swayze et al.	2011/0024477	A1	2/2011	Hall et al.
2009/0209979	A1	8/2009	Yates et al.	2011/0024478	A1	2/2011	Shelton, IV
2009/0209990	A1	8/2009	Yates et al.	2011/0024479	A1	2/2011	Swensgard et al.
2009/0213685	A1	8/2009	Mak et al.	2011/0036887	A1	2/2011	Zemlok et al.
2009/0218384	A1	9/2009	Aranyi	2011/0042441	A1	2/2011	Shelton, IV et al.
2009/0242610	A1	10/2009	Shelton, IV et al.	2011/0060363	A1	3/2011	Hess et al.
2009/0255974	A1	10/2009	Viola	2011/0068145	A1	3/2011	Bedi et al.
2009/0255975	A1	10/2009	Zemlok et al.	2011/0068148	A1	3/2011	Hall et al.
2009/0255976	A1	10/2009	Marczyk et al.	2011/0084112	A1	4/2011	Kostrzewski
2009/0255977	A1	10/2009	Zemlok	2011/0084115	A1	4/2011	Bedi et al.
2009/0255978	A1	10/2009	Viola et al.	2011/0087276	A1	4/2011	Bedi et al.
2009/0289096	A1	11/2009	Shelton, IV et al.	2011/0087279	A1	4/2011	Shah et al.
2009/0292283	A1	11/2009	Odom	2011/0095068	A1	4/2011	Patel
2009/0308907	A1	12/2009	Nalagatla et al.	2011/0101065	A1	5/2011	Milliman
2010/0012704	A1	1/2010	Tarinelli Racenet et al.	2011/0114697	A1	5/2011	Baxter, III et al.
2010/0023024	A1	1/2010	Zeiner et al.	2011/0114698	A1	5/2011	Baxter, III et al.
2010/0032470	A1	2/2010	Hess et al.	2011/0114699	A1	5/2011	Baxter, III et al.
2010/0049084	A1	2/2010	Nock et al.	2011/0114700	A1	5/2011	Baxter, III et al.
2010/0065605	A1	3/2010	Shelton, VI et al.	2011/0118761	A1	5/2011	Baxter, III et al.
2010/0065609	A1	3/2010	Schwemmerger	2011/0125176	A1	5/2011	Yates et al.
2010/0069942	A1	3/2010	Shelton, IV	2011/0125177	A1	5/2011	Yates et al.
2010/0072251	A1	3/2010	Baxter, III et al.	2011/0132963	A1	6/2011	Giordano et al.
2010/0072252	A1	3/2010	Baxter, III et al.	2011/0132964	A1	6/2011	Weisenburgh, II et al.
2010/0072253	A1	3/2010	Baxter, III et al.	2011/0132965	A1	6/2011	Moore et al.
2010/0072254	A1	3/2010	Aranyi et al.	2011/0144430	A1	6/2011	Spivey et al.
2010/0072256	A1	3/2010	Baxter, III et al.	2011/0147433	A1	6/2011	Shelton, IV et al.
2010/0076474	A1	3/2010	Yates et al.	2011/0147434	A1	6/2011	Hueil et al.
2010/0076475	A1	3/2010	Yates et al.	2011/0155780	A1	6/2011	Boudreaux
2010/0089970	A1	4/2010	Smith et al.	2011/0155781	A1	6/2011	Swensgard et al.
2010/0089972	A1	4/2010	Marczyk	2011/0155785	A1	6/2011	Laurent et al.
2010/0089974	A1	4/2010	Shelton, IV	2011/0155787	A1	6/2011	Baxter, III et al.
2010/0096431	A1	4/2010	Smith et al.	2011/0163147	A1	7/2011	Laurent et al.
2010/0096435	A1	4/2010	Fuchs et al.	2011/0174861	A1	7/2011	Shelton, IV et al.
2010/0108740	A1	5/2010	Pastorelli et al.	2011/0174863	A1	7/2011	Shelton, IV et al.
2010/0108741	A1	5/2010	Hessler et al.	2011/0178536	A1	7/2011	Kostrzewski
				2011/0192882	A1	8/2011	Hess et al.
				2011/0210156	A1	9/2011	Smith et al.
				2011/0226837	A1	9/2011	Baxter, III et al.
				2011/0233258	A1	9/2011	Boudreaux

(56)

References Cited

U.S. PATENT DOCUMENTS

2011/0275901 A1 11/2011 Shelton, IV
 2011/0276083 A1 11/2011 Shelton, IV et al.
 2011/0288573 A1 11/2011 Yates et al.
 2011/0290851 A1 12/2011 Shelton, IV
 2011/0290853 A1 12/2011 Shelton, IV et al.
 2011/0290854 A1 12/2011 Timm et al.
 2011/0290855 A1 12/2011 Moore et al.
 2011/0290856 A1 12/2011 Shelton, IV et al.
 2011/0290857 A1 12/2011 Shelton, IV et al.
 2011/0295242 A1 12/2011 Spivey et al.
 2011/0295269 A1 12/2011 Swensgard et al.
 2011/0295270 A1 12/2011 Giordano et al.
 2011/0295295 A1 12/2011 Shelton, IV et al.
 2012/0022523 A1 1/2012 Smith et al.
 2012/0024934 A1 2/2012 Shelton, IV et al.
 2012/0024935 A1 2/2012 Shelton, IV et al.
 2012/0024936 A1 2/2012 Baxter, III et al.
 2012/0029272 A1 2/2012 Shelton, IV et al.
 2012/0029544 A1 2/2012 Shelton, IV et al.
 2012/0029547 A1 2/2012 Shelton, IV et al.
 2012/0046692 A1 2/2012 Smith et al.
 2012/0061448 A1 3/2012 Zingman
 2012/0071711 A1 3/2012 Shelton, IV et al.
 2012/0071866 A1 3/2012 Kerr et al.
 2012/0074196 A1 3/2012 Shelton, IV et al.
 2012/0074198 A1 3/2012 Huitema et al.
 2012/0074200 A1 3/2012 Schmid et al.
 2012/0074201 A1 3/2012 Baxter, III et al.
 2012/0080332 A1 4/2012 Shelton, IV et al.
 2012/0080333 A1 4/2012 Woodard, Jr. et al.
 2012/0080334 A1 4/2012 Shelton, IV et al.
 2012/0080335 A1 4/2012 Shelton, IV et al.
 2012/0080336 A1 4/2012 Shelton, IV et al.
 2012/0080337 A1 4/2012 Shelton, IV et al.
 2012/0080338 A1 4/2012 Shelton, IV et al.
 2012/0080339 A1 4/2012 Shelton, IV et al.
 2012/0080340 A1 4/2012 Shelton, IV et al.
 2012/0080344 A1 4/2012 Shelton, IV
 2012/0080345 A1 4/2012 Morgan et al.
 2012/0080475 A1 4/2012 Smith et al.
 2012/0080477 A1 4/2012 Leimbach et al.
 2012/0080478 A1 4/2012 Morgan et al.
 2012/0080479 A1 4/2012 Shelton, IV
 2012/0080480 A1 4/2012 Woodard, Jr. et al.
 2012/0080481 A1 4/2012 Widenhouse et al.
 2012/0080482 A1 4/2012 Schall et al.
 2012/0080483 A1 4/2012 Riestenberg et al.
 2012/0080484 A1 4/2012 Morgan et al.
 2012/0080485 A1 4/2012 Woodard, Jr. et al.
 2012/0080486 A1 4/2012 Woodard, Jr. et al.
 2012/0080487 A1 4/2012 Woodard, Jr. et al.
 2012/0080488 A1 4/2012 Shelton, IV et al.
 2012/0080489 A1 4/2012 Shelton, IV et al.
 2012/0080490 A1 4/2012 Shelton, IV et al.
 2012/0080491 A1 4/2012 Shelton, IV et al.
 2012/0080493 A1 4/2012 Shelton, IV et al.
 2012/0080496 A1 4/2012 Schall et al.
 2012/0080498 A1 4/2012 Shelton, IV et al.
 2012/0080499 A1 4/2012 Schall et al.
 2012/0080500 A1 4/2012 Morgan et al.
 2012/0080501 A1 4/2012 Morgan et al.
 2012/0080502 A1 4/2012 Morgan et al.
 2012/0080503 A1 4/2012 Woodard, Jr. et al.
 2012/0083833 A1 4/2012 Shelton, IV et al.
 2012/0083834 A1 4/2012 Shelton, IV et al.
 2012/0083835 A1 4/2012 Shelton, IV et al.
 2012/0083836 A1 4/2012 Shelton, IV et al.
 2012/0132450 A1 5/2012 Timm et al.
 2012/0138660 A1 6/2012 Shelton, IV
 2012/0160721 A1 6/2012 Shelton, IV et al.
 2012/0175399 A1 7/2012 Shelton et al.
 2012/0187179 A1 7/2012 Gleiman
 2012/0199630 A1 8/2012 Shelton, IV et al.
 2012/0199631 A1 8/2012 Shelton, IV et al.
 2012/0199632 A1 8/2012 Spivey et al.

2012/0199633 A1 8/2012 Shelton, IV et al.
 2012/0203247 A1 8/2012 Shelton, IV et al.
 2012/0205421 A1 8/2012 Shelton, IV
 2012/0211546 A1 8/2012 Shelton, IV
 2012/0234890 A1 9/2012 Aronhalt et al.
 2012/0234891 A1 9/2012 Aronhalt et al.
 2012/0234892 A1 9/2012 Aronhalt et al.
 2012/0234893 A1 9/2012 Schuckmann et al.
 2012/0234895 A1 9/2012 O'Connor et al.
 2012/0234896 A1 9/2012 Ellerhorst et al.
 2012/0234897 A1 9/2012 Shelton, IV et al.
 2012/0234898 A1 9/2012 Shelton, IV et al.
 2012/0234899 A1 9/2012 Scheib et al.
 2012/0234900 A1 9/2012 Swayze
 2012/0238823 A1 9/2012 Hagerty et al.
 2012/0238824 A1 9/2012 Widenhouse et al.
 2012/0238826 A1 9/2012 Yoo et al.
 2012/0238829 A1 9/2012 Shelton, IV et al.
 2012/0239009 A1 9/2012 Mollere et al.
 2012/0239010 A1 9/2012 Shelton, IV et al.
 2012/0239012 A1 9/2012 Laurent et al.
 2012/0239075 A1 9/2012 Widenhouse et al.
 2012/0239082 A1 9/2012 Shelton, IV et al.
 2012/0241491 A1 9/2012 Aldridge et al.
 2012/0241492 A1 9/2012 Shelton, IV et al.
 2012/0241493 A1 9/2012 Baxter, III et al.
 2012/0241496 A1 9/2012 Mandakolathur Vasudevan et al.
 2012/0241497 A1 9/2012 Mandakolathur Vasudevan et al.
 2012/0241498 A1 9/2012 Gonzalez et al.
 2012/0241499 A1 9/2012 Baxter, III et al.
 2012/0241500 A1 9/2012 Timmer et al.
 2012/0241501 A1 9/2012 Swayze et al.
 2012/0241502 A1 9/2012 Aldridge et al.
 2012/0241503 A1 9/2012 Baxter, III et al.
 2012/0241505 A1 9/2012 Alexander, III et al.
 2012/0248169 A1 10/2012 Widenhouse et al.
 2012/0253298 A1 10/2012 Henderson et al.
 2012/0265230 A1 10/2012 Yates et al.
 2012/0273551 A1 11/2012 Shelton, IV et al.
 2012/0283707 A1 11/2012 Giordano et al.
 2012/0286019 A1 11/2012 Hueil et al.
 2012/0292367 A1 11/2012 Morgan et al.
 2012/0292370 A1 11/2012 Hess et al.
 2012/0298719 A1 11/2012 Shelton, IV et al.
 2013/0012931 A1 1/2013 Spivey et al.
 2013/0012957 A1 1/2013 Shelton, IV et al.
 2013/0020376 A1 1/2013 Shelton, IV et al.
 2013/0023861 A1 1/2013 Shelton, IV et al.
 2013/0026208 A1 1/2013 Shelton, IV et al.
 2013/0026210 A1 1/2013 Shelton, IV et al.
 2013/0041371 A1 2/2013 Yates et al.
 2013/0048697 A1 2/2013 Shelton, IV et al.
 2013/0075443 A1 3/2013 Giordano et al.
 2013/0190733 A1 7/2013 Giordano et al.

FOREIGN PATENT DOCUMENTS

CA 2514274 A1 1/2006
 CN 2488482 Y 5/2002
 CN 1634601 A 7/2005
 CN 1868411 A 11/2006
 CN 1915180 A 2/2007
 CN 101011286 8/2007
 CN 101095621 A 1/2008
 DE 273689 C 5/1914
 DE 1775926 A 1/1972
 DE 3036217 A1 4/1982
 DE 3210466 A1 9/1983
 DE 9412228 U 9/1994
 DE 19509116 A1 9/1996
 DE 19851291 A1 1/2000
 DE 19924311 A1 11/2000
 DE 69328576 T2 4/2001
 DE 10052679 A 5/2001
 DE 20112837 U1 10/2001
 DE 20121753 U1 4/2003
 DE 10314072 A 10/2004
 DE 202007003114 U1 6/2007
 EP 0122046 A1 10/1984

(56)

References Cited

FOREIGN PATENT DOCUMENTS

EP 0070230 B1 10/1985
 EP 0156774 A2 10/1985
 EP 0387980 B1 10/1985
 EP 0033548 B1 5/1986
 EP 0129442 B1 11/1987
 EP 0276104 A2 7/1988
 EP 0178941 B1 1/1991
 EP 0248844 B1 1/1993
 EP 0545029 A1 6/1993
 EP 0277959 B1 10/1993
 EP 0233940 B1 11/1993
 EP 0261230 81 11/1993
 EP 0639349 A2 2/1994
 EP 0324636 B1 3/1994
 EP 0593920 A1 4/1994
 EP 0594148 A1 4/1994
 EP 0427949 B1 6/1994
 EP 0523174 B1 6/1994
 EP 0600182 A2 6/1994
 EP 0310431 B1 11/1994
 EP 0375302 B1 11/1994
 EP 0376562 B1 11/1994
 EP 0630612 A1 12/1994
 EP 0634144 A1 1/1995
 EP 0646356 A2 4/1995
 EP 0646357 A1 4/1995
 EP 0653189 A2 5/1995
 EP 0669104 A1 8/1995
 EP 0511470 B1 10/1995
 EP 0679367 A2 11/1995
 EP 0392547 B1 12/1995
 EP 0685204 A1 12/1995
 EP 0364216 B1 1/1996
 EP 0699418 A1 3/1996
 EP 0702937 A1 3/1996
 EP 0705571 A1 4/1996
 EP 0711611 A2 5/1996
 EP 0484677 B2 6/1996
 EP 0541987 B1 7/1996
 EP 0667119 B1 7/1996
 EP 0708618 B1 3/1997
 EP 0770355 A1 5/1997
 EP 0503662 B1 6/1997
 EP 0447121 B1 7/1997
 EP 0625077 B1 7/1997
 EP 0633749 B1 8/1997
 EP 0710090 B1 8/1997
 EP 0578425 B1 9/1997
 EP 0625335 B1 11/1997
 EP 0552423 B1 1/1998
 EP 0592244 B1 1/1998
 EP 0648476 B1 1/1998
 EP 0649290 B1 3/1998
 EP 0598618 B1 9/1998
 EP 0676173 B1 9/1998
 EP 0678007 B1 9/1998
 EP 0603472 B1 11/1998
 EP 0605351 B1 11/1998
 EP 0878169 A1 11/1998
 EP 0879742 A1 11/1998
 EP 0695144 B1 12/1998
 EP 0722296 B1 12/1998
 EP 0760230 B1 2/1999
 EP 0623316 B1 3/1999
 EP 0650701 B1 3/1999
 EP 0537572 B1 6/1999
 EP 0923907 A1 6/1999
 EP 0843906 B1 3/2000
 EP 0552050 B1 5/2000
 EP 0833592 B1 5/2000
 EP 0830094 B1 9/2000
 EP 1034747 A1 9/2000
 EP 1034748 A1 9/2000
 EP 0694290 B1 11/2000
 EP 1050278 A1 11/2000

EP 1053719 A1 11/2000
 EP 1053720 A1 11/2000
 EP 1055399 A1 11/2000
 EP 1055400 A1 11/2000
 EP 1080694 A1 3/2001
 EP 1090592 A1 4/2001
 EP 1095627 A1 5/2001
 EP 1256318 B1 5/2001
 EP 0806914 B1 9/2001
 EP 0768840 B1 12/2001
 EP 0908152 B1 1/2002
 EP 0872213 B1 5/2002
 EP 0862386 B1 6/2002
 EP 0949886 81 9/2002
 EP 1238634 A2 9/2002
 EP 0858295 B1 12/2002
 EP 0656188 B1 1/2003
 EP 1284120 A1 2/2003
 EP 1287788 A1 3/2003
 EP 0717966 B1 4/2003
 EP 0869742 B1 5/2003
 EP 0829235 B1 6/2003
 EP 0887046 B1 7/2003
 EP 0852480 81 8/2003
 EP 0891154 B1 9/2003
 EP 0813843 B1 10/2003
 EP 0873089 B1 10/2003
 EP 0856326 B1 11/2003
 EP 1374788 A1 1/2004
 EP 0741996 B1 2/2004
 EP 0814712 B1 2/2004
 EP 1402837 A1 3/2004
 EP 0705570 B1 4/2004
 EP 0959784 B1 4/2004
 EP 1407719 A2 4/2004
 EP 1086713 B1 5/2004
 EP 0996378 B1 6/2004
 EP 1426012 A1 6/2004
 EP 0833593 B2 7/2004
 EP 1442694 A1 8/2004
 EP 0888749 B1 9/2004
 EP 0959786 B1 9/2004
 EP 1459695 A1 9/2004
 EP 1473819 A1 11/2004
 EP 1477119 A1 11/2004
 EP 1479345 A1 11/2004
 EP 1479347 A1 11/2004
 EP 1479348 A1 11/2004
 EP 0754437 B2 12/2004
 EP 1025807 B1 12/2004
 EP 1001710 B1 1/2005
 EP 1520521 A1 4/2005
 EP 1520523 A1 4/2005
 EP 1520525 A1 4/2005
 EP 1522264 A1 4/2005
 EP 1523942 A2 4/2005
 EP 1550408 A1 7/2005
 EP 1557129 A1 7/2005
 EP 1064883 B1 8/2005
 EP 1067876 B1 8/2005
 EP 0870473 B1 9/2005
 EP 1157666 B1 9/2005
 EP 0880338 81 10/2005
 EP 1158917 B1 11/2005
 EP 1344498 B1 11/2005
 EP 1330989 B1 12/2005
 EP 0771176 B2 1/2006
 EP 1621138 A2 2/2006
 EP 1621139 A2 2/2006
 EP 1621141 A2 2/2006
 EP 1621145 A2 2/2006
 EP 1621151 A2 2/2006
 EP 1034746 B1 3/2006
 EP 1632191 A2 3/2006
 EP 1065981 B1 5/2006
 EP 1082944 B1 5/2006
 EP 1652481 A2 5/2006
 EP 1382303 B1 6/2006
 EP 1253866 B1 7/2006

(56)

References Cited

FOREIGN PATENT DOCUMENTS

EP	1032318	B1	8/2006	EP	1566150	B1	4/2010
EP	1045672	B1	8/2006	EP	1813206	B1	4/2010
EP	1617768	B1	8/2006	EP	1769754	B1	6/2010
EP	1693015	A2	8/2006	EP	1535565	B1	10/2010
EP	1400214	B1	9/2006	EP	1702570	B1	10/2010
EP	1702567	A2	9/2006	EP	1785098	B1	10/2010
EP	1129665	B1	11/2006	EP	2005896	B1	10/2010
EP	1400206	B1	11/2006	EP	2030578	B1	11/2010
EP	1721568	A1	11/2006	EP	1627605	B1	12/2010
EP	1256317	B1	12/2006	EP	1813205	B1	6/2011
EP	1285633	B1	12/2006	EP	2090243	B1	6/2011
EP	1728473	A1	12/2006	EP	1785102	B1	1/2012
EP	1728475	A2	12/2006	FR	999646	A	2/1952
EP	1479346	B1	1/2007	FR	1112936	A	3/1956
EP	1484024	B1	1/2007	FR	2598905	A1	11/1987
EP	1754445	A2	2/2007	FR	2765794	A	1/1999
EP	1759812	A1	3/2007	GB	939929	A	10/1963
EP	1767163	A1	3/2007	GB	1210522	A	10/1970
EP	1769756	A1	4/2007	GB	1217159	A	12/1970
EP	1769758	A1	4/2007	GB	1339394	A	12/1973
EP	1581128	B1	5/2007	GB	2109241	A	6/1983
EP	1780825	A1	5/2007	GB	2272159	A	5/1994
EP	1785097	A2	5/2007	GB	2284242	A	5/1995
EP	1790293	A2	5/2007	GB	2336214	A	10/1999
EP	1800610	A1	6/2007	GB	2425903	A	11/2006
EP	1300117	B1	8/2007	JP	50-33988	U	4/1975
EP	1813199	A1	8/2007	JP	S 58500053	A	1/1983
EP	1813201	A1	8/2007	JP	61-98249	A	5/1986
EP	1813202	A1	8/2007	JP	S 61502036	A	9/1986
EP	1813203	A2	8/2007	JP	63-203149		8/1988
EP	1813207	A1	8/2007	JP	3-12126	A	1/1991
EP	1813209	A1	8/2007	JP	5-212039	A	8/1993
EP	1487359	B1	10/2007	JP	6007357	A	1/1994
EP	1599146	B1	10/2007	JP	7051273		2/1995
EP	1839596	A1	10/2007	JP	7-124166	A	5/1995
EP	2110083	A2	10/2007	JP	7-255735	A	10/1995
EP	1857057	A2	11/2007	JP	8-33642	A	2/1996
EP	1402821	B1	12/2007	JP	8033641	A	2/1996
EP	1872727	A1	1/2008	JP	8-164141	A	6/1996
EP	1897502	A1	3/2008	JP	8229050	A	9/1996
EP	1330201	B1	6/2008	JP	2000033071	A	2/2000
EP	1702568	B1	7/2008	JP	2000171730	A	6/2000
EP	1943955	A2	7/2008	JP	2000287987	A	10/2000
EP	1943957	A2	7/2008	JP	2000325303	A	11/2000
EP	1943964	A1	7/2008	JP	2001-514541	A	9/2001
EP	1943976	A2	7/2008	JP	2001286477	A	10/2001
EP	1593337	B1	8/2008	JP	2002143078	A	5/2002
EP	1970014	A1	9/2008	JP	2002369820	A	12/2002
EP	1980213	A2	10/2008	JP	2003-500153	A	1/2003
EP	1759645	B1	11/2008	JP	2003-521301	A	7/2003
EP	1990014	A2	11/2008	JP	2004-532084	A	10/2004
EP	1552795	B1	12/2008	JP	2004-329624	A	11/2004
EP	1693008	B1	12/2008	JP	2004-344663		12/2004
EP	1759640	B1	12/2008	JP	2005-28148	A	2/2005
EP	2000102	A2	12/2008	JP	2005-028149	A	2/2005
EP	2008595	A2	12/2008	JP	2005505322	T	2/2005
EP	1736104	B1	3/2009	JP	2005103293	A	4/2005
EP	1749486	B1	3/2009	JP	2005131163	A	5/2005
EP	2039316	A2	3/2009	JP	2005131164	A	5/2005
EP	1721576	81	4/2009	JP	2005131173	A	5/2005
EP	1733686	B1	4/2009	JP	2005131211	A	5/2005
EP	2044890	A1	4/2009	JP	2005131212	A	5/2005
EP	1550409	A1	6/2009	JP	2005-144183	A	6/2005
EP	1550413	B1	6/2009	JP	2005137423	A	6/2005
EP	1745748	B1	8/2009	JP	2005152416	A	6/2005
EP	2090237	A1	8/2009	JP	2005-523105	A	8/2005
EP	2090244	A2	8/2009	JP	2005524474	A	8/2005
EP	2090245	A1	8/2009	JP	2006-034975	A	2/2006
EP	2090256	A2	8/2009	JP	2006-281405	A	10/2006
EP	2095777	A2	9/2009	JP	2009-506799	A	2/2009
EP	2110082	A1	10/2009	RU	2008830	C1	3/1994
EP	1813208	B1	11/2009	RU	2141279	C1	11/1999
EP	2116195	A1	11/2009	RU	2187249	C2	8/2002
EP	1607050	B1	12/2009	RU	2225170	C2	3/2004
EP	1815804	B1	12/2009	SU	189517	A	1/1967
				SU	328636	A	9/1972
				SU	886900	A1	12/1981
				SU	1009439	A	4/1983
				SU	1333319	A2	8/1987

(56)

References Cited

FOREIGN PATENT DOCUMENTS

SU	1377053	A1	2/1988	WO	WO 99/12487	A1	3/1999
SU	1561964	A1	5/1990	WO	WO 99/12488	A1	3/1999
SU	1708312	A1	1/1992	WO	WO 99/15086	A1	4/1999
SU	1722476	A1	3/1992	WO	WO 99/15091	A1	4/1999
SU	1752361	A1	8/1992	WO	WO 99/23933	A2	5/1999
WO	WO 82/02824	A1	9/1982	WO	WO 99/23959	A1	5/1999
WO	WO 91/15157	A1	10/1991	WO	WO 99/25261	A1	5/1999
WO	WO 92/20295	A1	11/1992	WO	WO 99/29244	A1	6/1999
WO	WO 92/21300	A1	12/1992	WO	WO 99/34744	A1	7/1999
WO	WO 93/08755	A1	5/1993	WO	WO 99/45849	A1	9/1999
WO	WO 93/13718	A1	7/1993	WO	WO 99/48430	A1	9/1999
WO	WO 93/14690	A1	8/1993	WO	WO 99/51158	A1	10/1999
WO	WO 93/15648	A1	8/1993	WO	WO 00/24322	A1	5/2000
WO	WO 93/15850	A1	8/1993	WO	WO 00/24330	A1	5/2000
WO	WO 93/19681	A1	10/1993	WO	WO 00/41638	A1	7/2000
WO	WO 94/00060	A1	1/1994	WO	WO 00/48506	A1	8/2000
WO	WO 94/11057	A1	5/1994	WO	WO 00/53112	A2	9/2000
WO	WO 94/12108	A1	6/1994	WO	WO 00/54653	A1	9/2000
WO	WO 94/18893	A1	9/1994	WO	WO 00/57796	A1	10/2000
WO	WO 94/22378	A1	10/1994	WO	WO 00/64365	A1	11/2000
WO	WO 94/23659	A1	10/1994	WO	WO 00/72762	A1	12/2000
WO	WO 95/02369	A1	1/1995	WO	WO 00/72765	A1	12/2000
WO	WO 95/03743	A1	2/1995	WO	WO 01/03587	A1	1/2001
WO	WO 95/06817	A1	3/1995	WO	WO 01/05702	A1	1/2001
WO	WO 95/09576	A1	4/1995	WO	WO 01/10482	A1	2/2001
WO	WO 95/09577	A1	4/1995	WO	WO 01/35845	A1	5/2001
WO	WO 95/14436	A1	6/1995	WO	WO 01/54594	A1	8/2001
WO	WO 95/17855	A1	7/1995	WO	WO 01/58371	A1	8/2001
WO	WO 95/18383	A1	7/1995	WO	WO 01/62158	A2	8/2001
WO	WO 95/18572	A1	7/1995	WO	WO 01/62161	A1	8/2001
WO	WO 95/19739	A1	7/1995	WO	WO 01/62162	A1	8/2001
WO	WO 95/20360	A1	8/1995	WO	WO 01/62164	A2	8/2001
WO	WO 95/23557	A1	9/1995	WO	WO 01/62169	A2	8/2001
WO	WO 95/24865	A1	9/1995	WO	WO 01/78605	A2	10/2001
WO	WO 95/25471	A3	9/1995	WO	WO 01/91646	A1	12/2001
WO	WO 95/26562	A1	10/1995	WO	WO 02/07608	A2	1/2002
WO	WO 95/29639	A1	11/1995	WO	WO 02/07618	A1	1/2002
WO	WO 96/04858	A1	2/1996	WO	WO 02/17799	A1	3/2002
WO	WO 96/19151	A1	6/1996	WO	WO 02/19920	A1	3/2002
WO	WO 96/19152	A1	6/1996	WO	WO 02/19932	A1	3/2002
WO	WO 96/20652	A1	7/1996	WO	WO 02/30297	A2	4/2002
WO	WO 96/21119	A1	7/1996	WO	WO 02/32322	A2	4/2002
WO	WO 96/22055	A1	7/1996	WO	WO 02/36028	A1	5/2002
WO	WO 96/23448	A1	8/1996	WO	WO 02/43571	A2	6/2002
WO	WO 96/24301	A1	8/1996	WO	WO 02/058568	A1	8/2002
WO	WO 96/27337	A1	9/1996	WO	WO 02/060328	A1	8/2002
WO	WO 96/31155	A1	10/1996	WO	WO 02/067785	A2	9/2002
WO	WO 96/35464	A1	11/1996	WO	WO 02/098302	A1	12/2002
WO	WO 96/39085	A1	12/1996	WO	WO 03/000138	A2	1/2003
WO	WO 96/39086	A1	12/1996	WO	WO 03/001329	A2	1/2003
WO	WO 96/39087	A1	12/1996	WO	WO 03/013363	A1	2/2003
WO	WO 96/39088	A1	12/1996	WO	WO 03/015604	A2	2/2003
WO	WO 96/39089	A1	12/1996	WO	WO 03/020106	A2	3/2003
WO	WO 97/00646	A1	1/1997	WO	WO 03/020139	A2	3/2003
WO	WO 97/00647	A1	1/1997	WO	WO 03/024339	A1	3/2003
WO	WO 97/06582	A1	2/1997	WO	WO 03/079909	A3	3/2003
WO	WO 97/10763	A1	3/1997	WO	WO 03/030743	A2	4/2003
WO	WO 97/10764	A1	3/1997	WO	WO 03/037193	A1	5/2003
WO	WO 97/11648	A2	4/1997	WO	WO 03/047436	A3	6/2003
WO	WO 97/11649	A1	4/1997	WO	WO 03/055402	A1	7/2003
WO	WO 97/15237	A1	5/1997	WO	WO 03/057048	A1	7/2003
WO	WO 97/24073	A1	7/1997	WO	WO 03/057058	A1	7/2003
WO	WO 97/24993	A1	7/1997	WO	WO 03/063694	A1	8/2003
WO	WO 97/30644	A1	8/1997	WO	WO 03/077769	A1	9/2003
WO	WO 97/34533	A1	9/1997	WO	WO 03/079911	A1	10/2003
WO	WO 97/37598	A1	10/1997	WO	WO 03/082126	A1	10/2003
WO	WO 97/39688	A2	10/1997	WO	WO 03/088845	A2	10/2003
WO	WO 98/17180	A1	4/1998	WO	WO 03/090630	A2	11/2003
WO	WO 98/27880	A1	7/1998	WO	WO 03/094743	A1	11/2003
WO	WO 98/30153	A1	7/1998	WO	WO 03/094745	A1	11/2003
WO	WO 98/47436	A1	10/1998	WO	WO 03/094746	A1	11/2003
WO	WO 99/03407	A1	1/1999	WO	WO 03/094747	A1	11/2003
WO	WO 99/03408	A1	1/1999	WO	WO 03/101313	A1	12/2003
WO	WO 99/03409	A1	1/1999	WO	WO 03/105698	A2	12/2003
WO	WO 99/12483	A1	3/1999	WO	WO 03/105702	A2	12/2003
				WO	WO 2004/006980	A2	1/2004
				WO	WO 2004/011037	A2	2/2004
				WO	WO 2004/019769	A1	3/2004
				WO	WO 2004/019803	A1	3/2004

(56) References Cited

FOREIGN PATENT DOCUMENTS

WO WO 2004/021868 A2 3/2004
 WO WO 2004/028585 A2 4/2004
 WO WO 2004/032754 A2 4/2004
 WO WO 2004/032760 A2 4/2004
 WO WO 2004/032762 A1 4/2004
 WO WO 2004/032763 A2 4/2004
 WO WO 2004/034875 A2 4/2004
 WO WO 2004/047626 A1 6/2004
 WO WO 2004/047653 A2 6/2004
 WO WO 2004/049956 A2 6/2004
 WO WO 2004/052426 A2 6/2004
 WO WO 2004/056276 A1 7/2004
 WO WO 2004/056277 A1 7/2004
 WO WO 2004/062516 A1 7/2004
 WO WO 2004/078050 A2 9/2004
 WO WO 2004/078051 A2 9/2004
 WO WO 2004/086987 A1 10/2004
 WO WO 2004/096015 A2 11/2004
 WO WO 2004/096057 A2 11/2004
 WO WO 2004/103157 A2 12/2004
 WO WO 2004/105593 A1 12/2004
 WO WO 2004/105621 A1 12/2004
 WO WO 2004/112618 A2 12/2004
 WO WO 2004/112652 A2 12/2004
 WO WO 2005/027983 A2 3/2005
 WO WO 2005/037329 A2 4/2005
 WO WO 2005/044078 A2 5/2005
 WO WO 2005/055846 A1 6/2005
 WO WO 2005/072634 A2 8/2005
 WO WO 2005/078892 A1 8/2005
 WO WO 2005/079675 A2 9/2005
 WO WO 2005/096954 A2 10/2005
 WO WO 2005/112806 A2 12/2005
 WO WO 2005/112808 A1 12/2005
 WO WO 2005/115251 A2 12/2005
 WO WO 2005/115253 A2 12/2005
 WO WO 2005/117735 A1 12/2005
 WO WO 2005/122936 A1 12/2005
 WO WO 2006/023486 A1 3/2006
 WO WO 2006/027014 A1 3/2006
 WO WO 2006/044490 A2 4/2006
 WO WO 2006/044581 A2 4/2006
 WO WO 2006/044810 A2 4/2006
 WO WO 2006/051252 A1 5/2006
 WO WO 2006/059067 A1 6/2006
 WO WO 2006/083748 A1 8/2006
 WO WO 2006/092563 A1 9/2006
 WO WO 2006/092565 A1 9/2006
 WO WO 2006/115958 A1 11/2006
 WO WO 2006/125940 A1 11/2006
 WO WO 2006/132992 A1 12/2006
 WO WO 2007/002180 A2 1/2007
 WO WO 2007/016290 A2 2/2007
 WO WO 2007/018898 A2 2/2007
 WO WO 2007/098220 A2 8/2007
 WO WO 2007/121579 A1 11/2007
 WO WO 2007/131110 A2 11/2007
 WO WO 2007/137304 A2 11/2007
 WO WO 2007/139734 A2 12/2007
 WO WO 2007/142625 A2 12/2007
 WO WO 2007/147439 A1 12/2007
 WO WO 2008/021969 A2 2/2008
 WO WO 2008/039249 A1 4/2008
 WO WO 2008/039270 A1 4/2008
 WO WO 2008/045383 A2 4/2008
 WO WO 2008/070763 A1 6/2008
 WO WO 2008/089404 A2 7/2008
 WO WO 2008/109125 A1 9/2008
 WO WO 2008/124748 A1 10/2008
 WO WO 2010/063795 A1 6/2010

WO WO 2010/098871 A2 9/2010
 WO WO 2012/021671 A1 2/2012
 WO WO 2012/044844 A2 4/2012

OTHER PUBLICATIONS

The Soderm Aseptic Battery Transfer Kit, Soderm Systems, 2000, 3 pages.
 "Biomedical Coatings," Fort Wayne Metals, Research Products Corporation, obtained online at www.fwmetals.com on Jun. 21, 2010 (1 page).
 European Search Report, Application No. 08250093.5, dated Nov. 4, 2009 (7 pages).
 Disclosed Anonymously, "Motor-Driven Surgical Stapler Improvements," Research Disclosure Database No. 526041, Published: Feb. 2008.
 C.C. Thompson et al., "Peroral Endoscopic Reduction of Dilated Gastrojejunal Anastomosis After Roux-en-Y Gastric Bypass: A Possible New Option for Patients with Weight Regain," *Surg Endosc* (2006) vol. 20, pp. 1744-1748.
 B.R. Coolman, DVM, MS et al., "Comparison of Skin Staples With Sutures for Anastomosis of the Small Intestine in Dogs," Abstract; <http://www.blackwell-synergy.com/doi/abs/10.1053/jvet.2000.7539?cookieSet=1&journalCode=vsu> which redirects to <http://www3.interscience.wiley.com/journal/119040681/abstract?CRETRY=1&SRETRY=0>; [online] accessed: Sep. 22, 2008 (2 pages).
 Reg. No. H1904, Oct. 3, 2000, Yates et al.
 Van Meer et al., "A Disposable Plastic Compact Wrist for Smart Minimally Invasive Surgical Tools," *LAAS/CNRS* (Aug. 2005).
 Breedveld et al., "A New, Easily Miniaturized Sterrable Endoscope," *IEEE Engineering in Medicine and Biology Magazine* (Nov./Dec. 2005).
 D. Tuite, Ed., "Get the Lowdown on Ultracapacitors," Nov. 15, 2007; [online] URL: <http://electronicdesign.com/Articles/Print.cfm?ArticleID=17465>, accessed Jan. 15, 2008 (5 pages).
 Datasheet for Panasonic TK Relays Ultra Low Profile 2 a Polarized Relay, Copyright Matsushita Electric Works, Ltd. (Known of at least as early as Aug. 17, 2010), 5 pages.
 ASTM procedure D2240-00, "Standard Test Method for Rubber Property-Durometer Hardness," (Published Aug. 2000).
 ASTM procedure D2240-05, "Standard Test Method for Rubber Property-Durometer Hardness," (Published Apr. 2010).
 U.S. Appl. No. 12/031,368, filed Feb. 14, 2008.
 U.S. Appl. No. 12/031,542, filed Feb. 14, 2008.
 U.S. Appl. No. 12/031,556, filed Feb. 14, 2008.
 U.S. Appl. No. 12/031,573, filed Feb. 14, 2008.
 U.S. Appl. No. 13/118,241, filed May 27, 2011.
 U.S. Appl. No. 13/488,903, filed Jun. 5, 2012.
 U.S. Appl. No. 13/310,107, filed Dec. 2, 2011.
 U.S. Appl. No. 13/369,561, filed Feb. 9, 2012.
 U.S. Appl. No. 13/369,569, filed Feb. 9, 2012.
 U.S. Appl. No. 13/369,584, filed Feb. 9, 2012.
 U.S. Appl. No. 13/369,588, filed Feb. 9, 2012.
 U.S. Appl. No. 13/369,594, filed Feb. 9, 2012.
 U.S. Appl. No. 13/369,601, filed Feb. 9, 2012.
 U.S. Appl. No. 13/369,609, filed Feb. 9, 2012.
 U.S. Appl. No. 13/369,629, filed Feb. 9, 2012.
 U.S. Appl. No. 13/369,666, filed Feb. 9, 2012.
 U.S. Appl. No. 13/372,195, filed Feb. 13, 2012.
 U.S. Appl. No. 13/486,175, filed Jun. 1, 2012.
 U.S. Appl. No. 13/480,263, filed May 24, 2012.
 Partial European Search Report, Application No. 08250085.1, dated Apr. 15, 2008 (7 pages).
 European Search Report for Application No. 12173438.8, dated Oct. 24, 2012 (8 pages).
 European Examination Report for Application No. 08250093.5, dated Jan. 19, 2012 (4 pages).

* cited by examiner

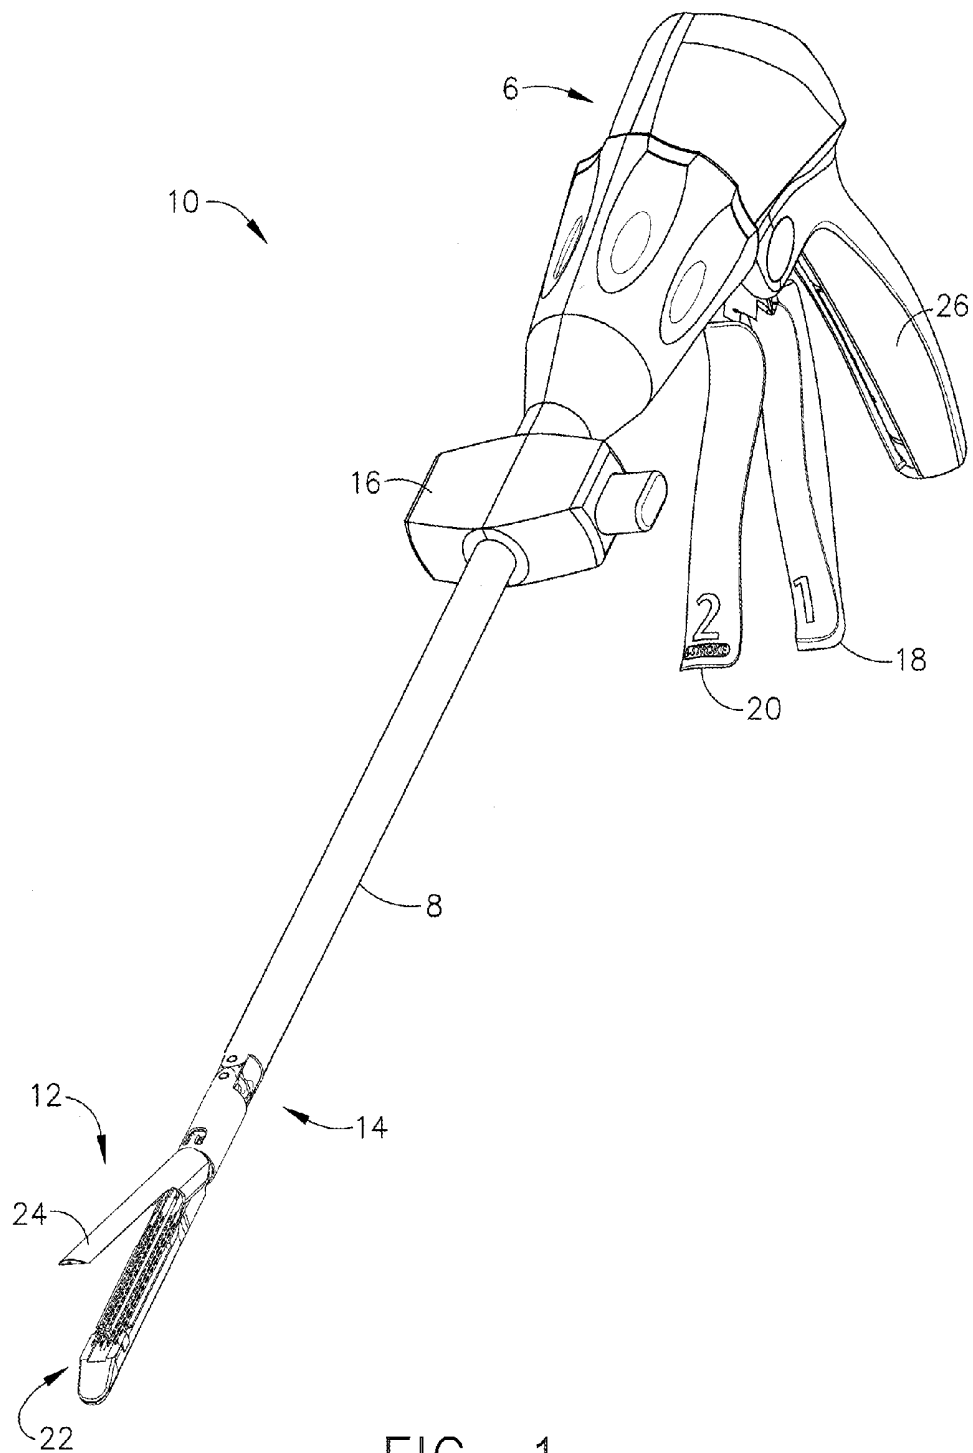


FIG. 1

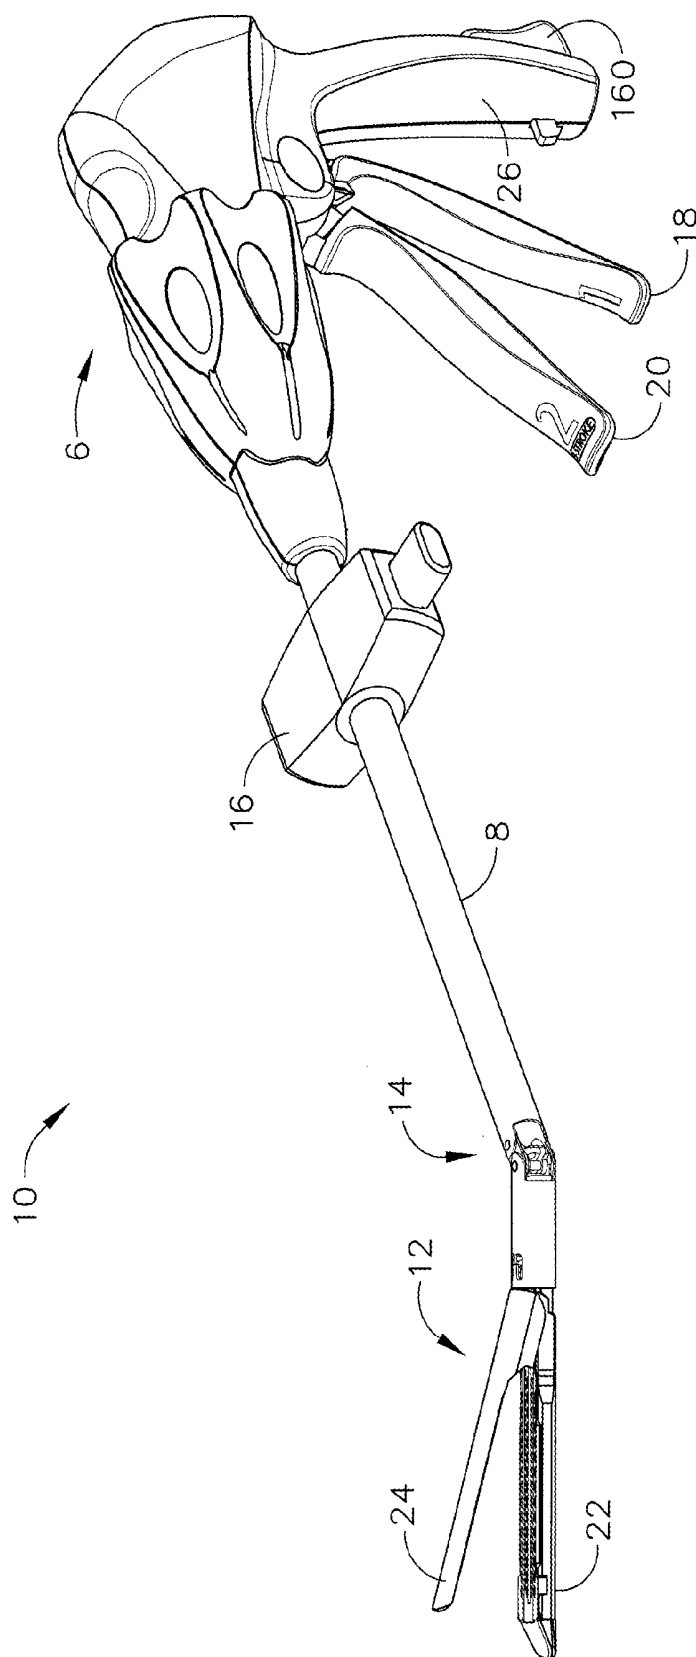


FIG. 2

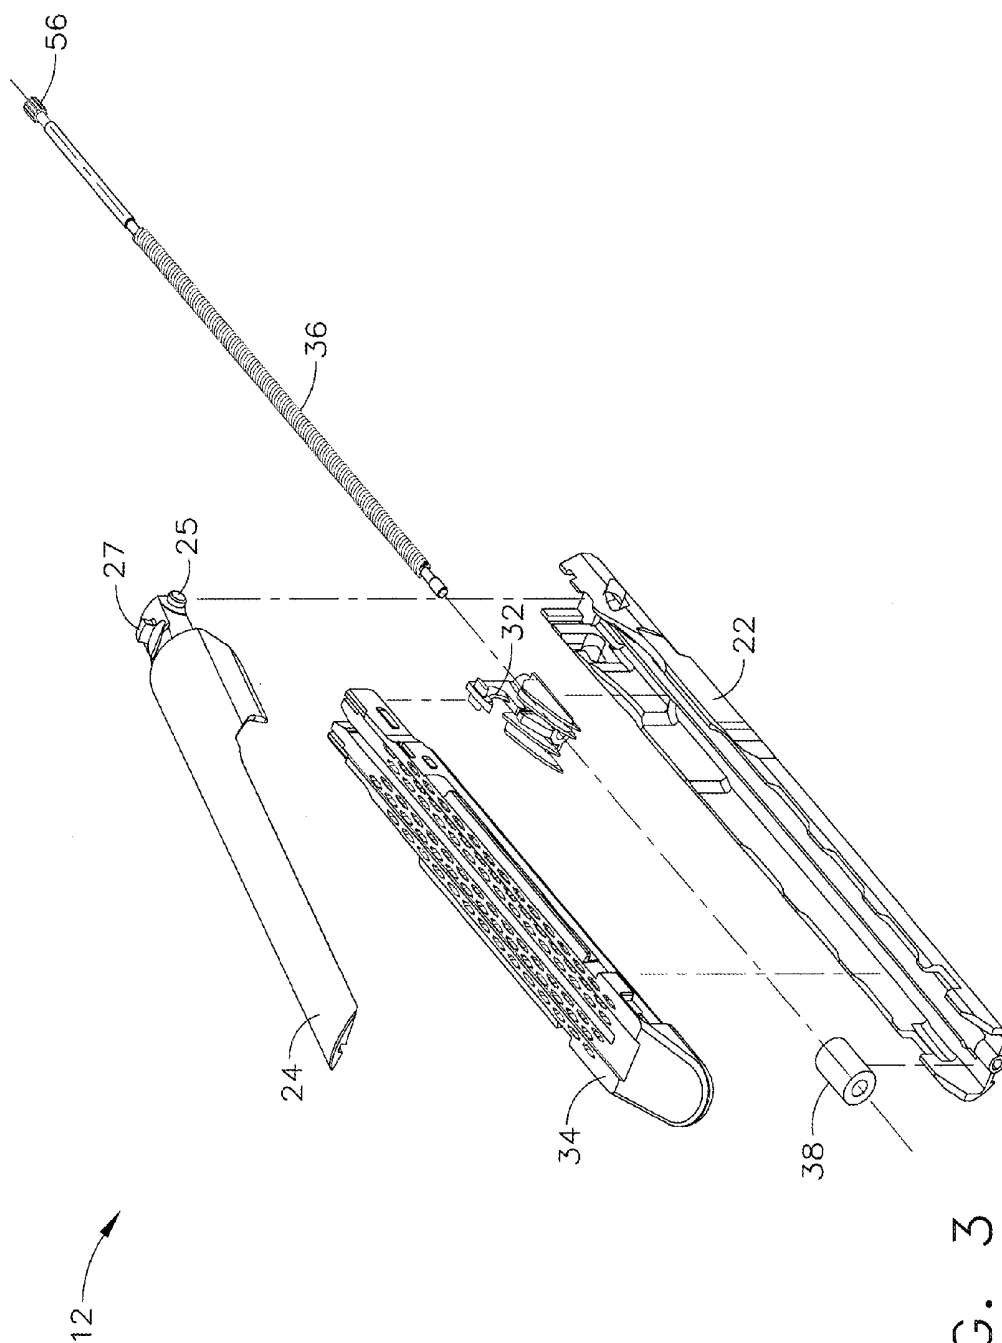


FIG. 3


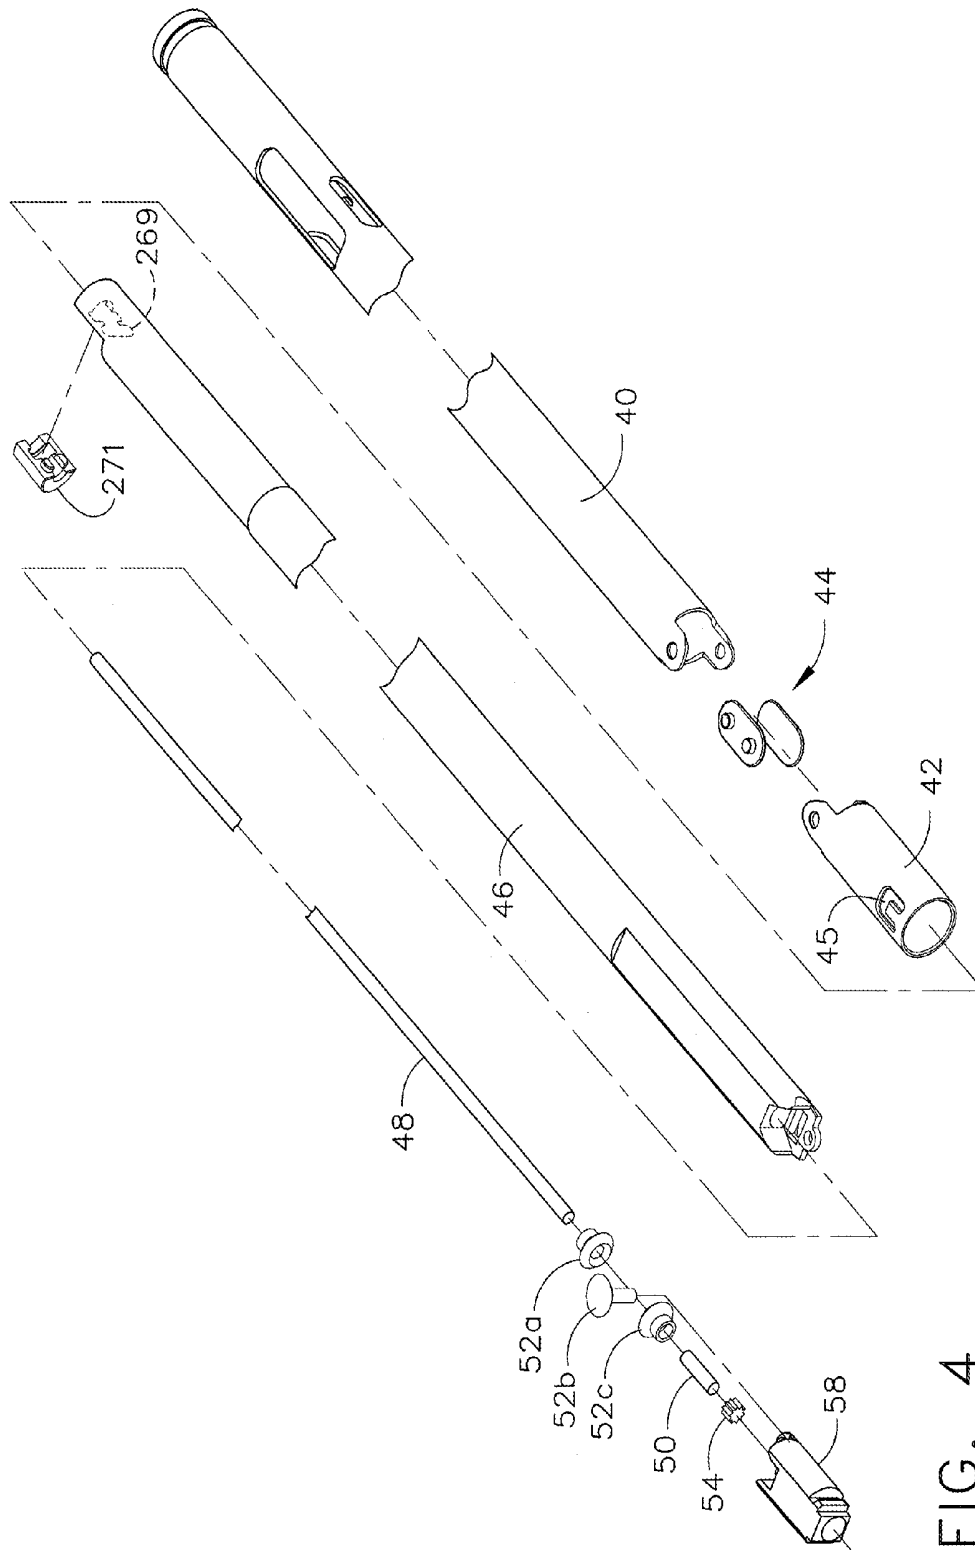


FIG. 4

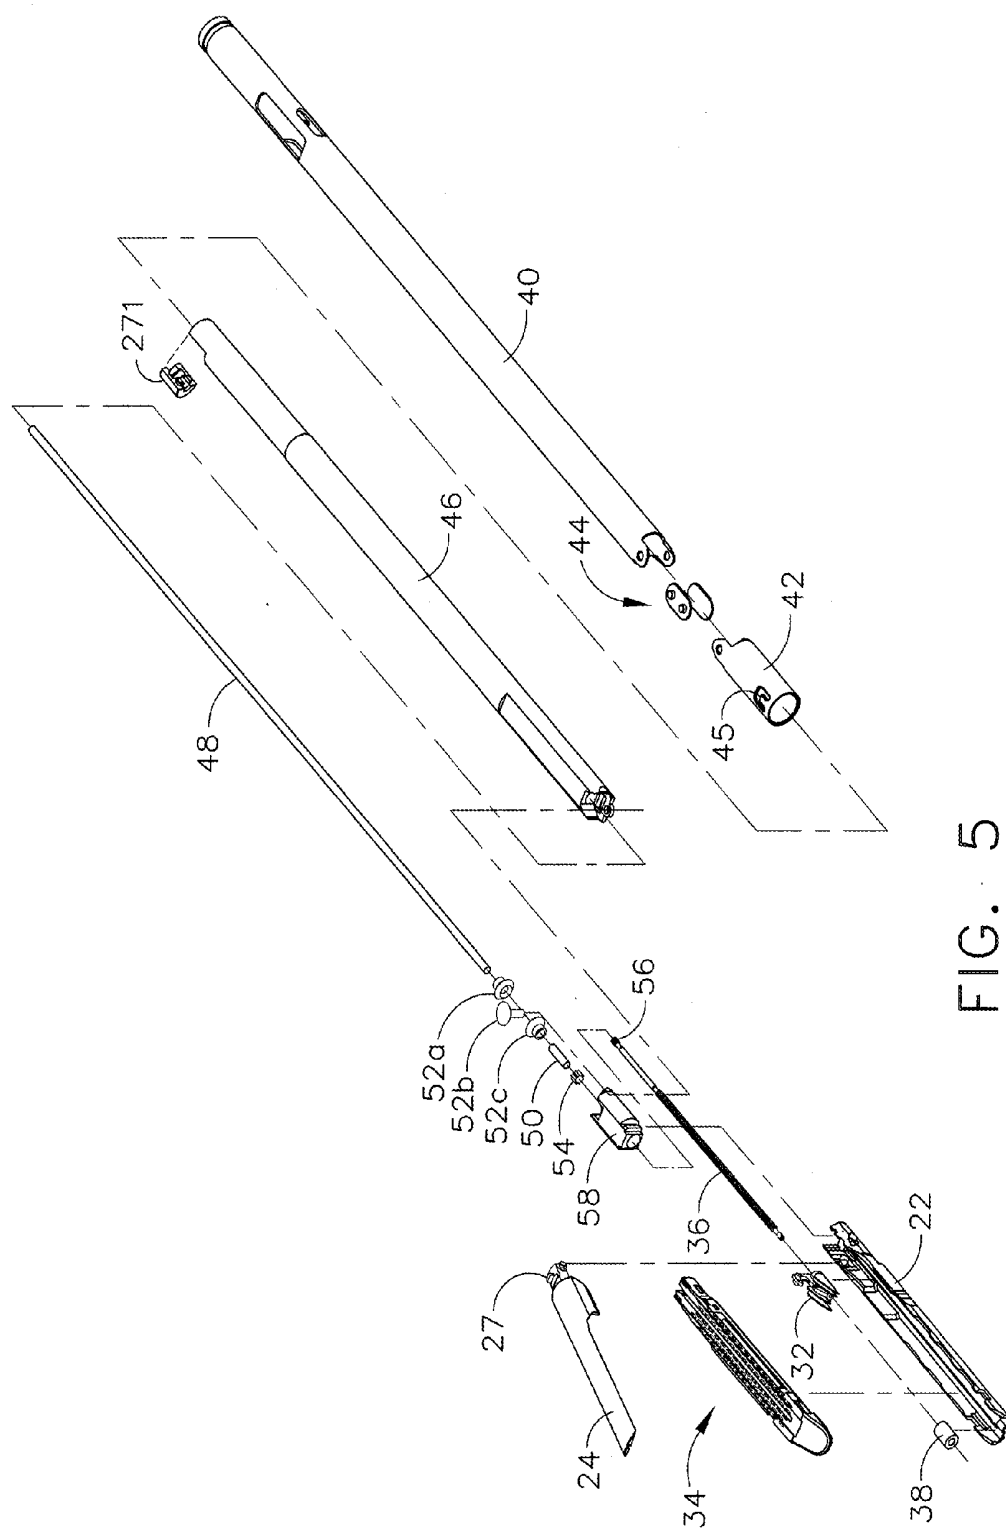

56

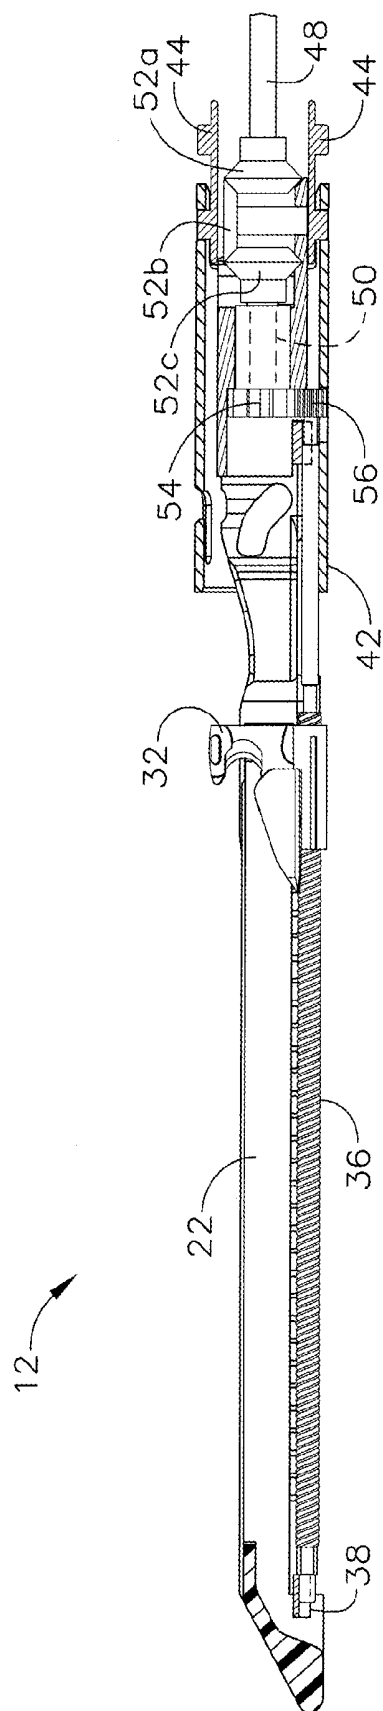


FIG. 6

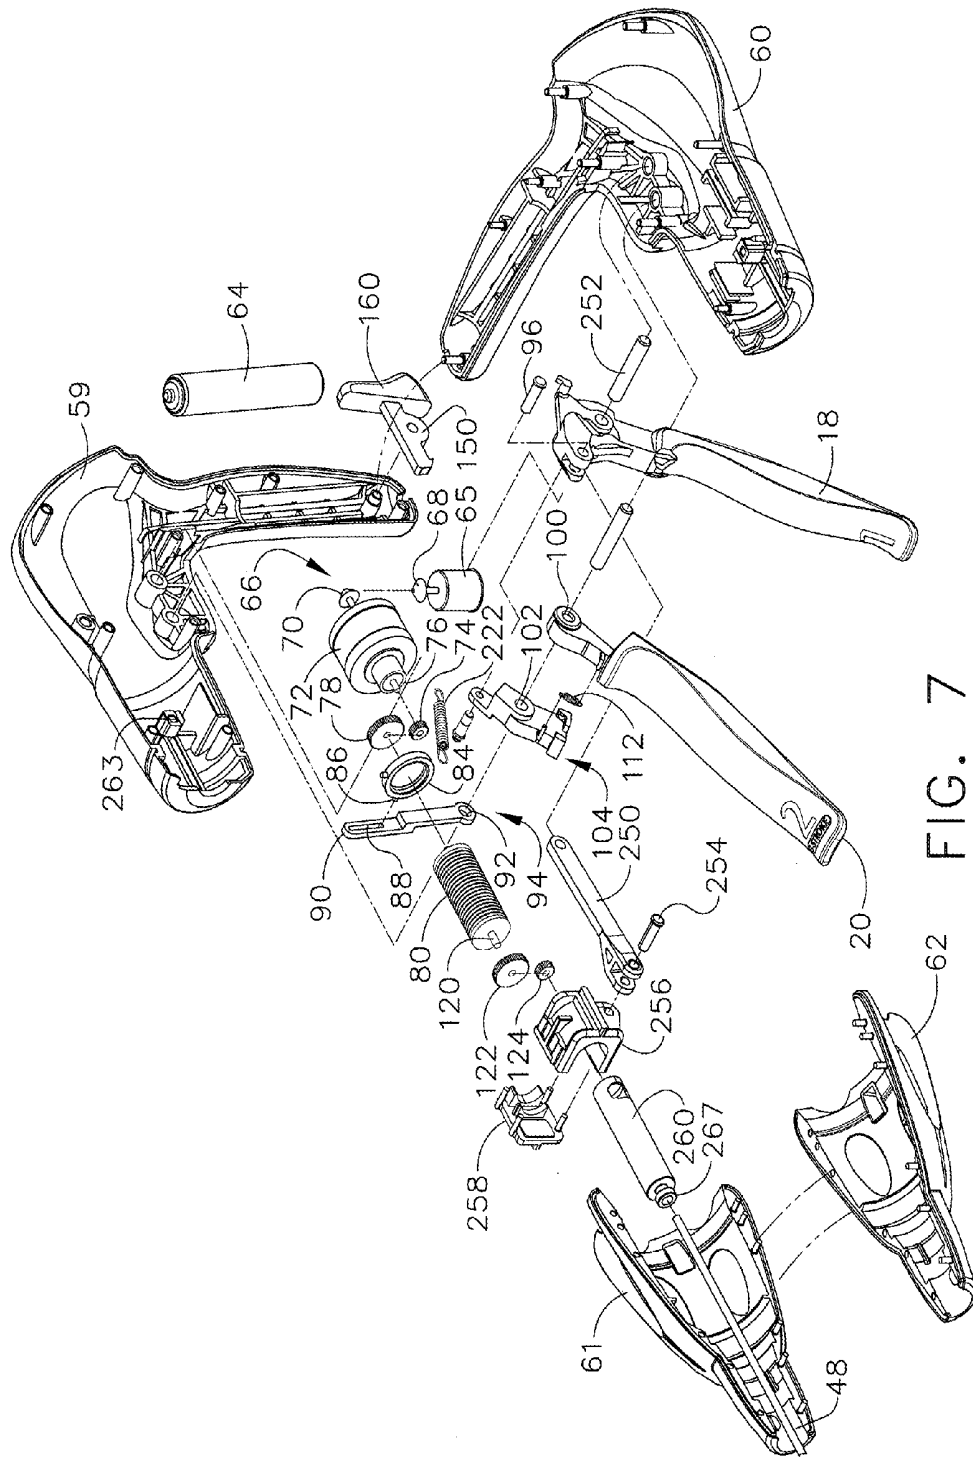


FIG. 7

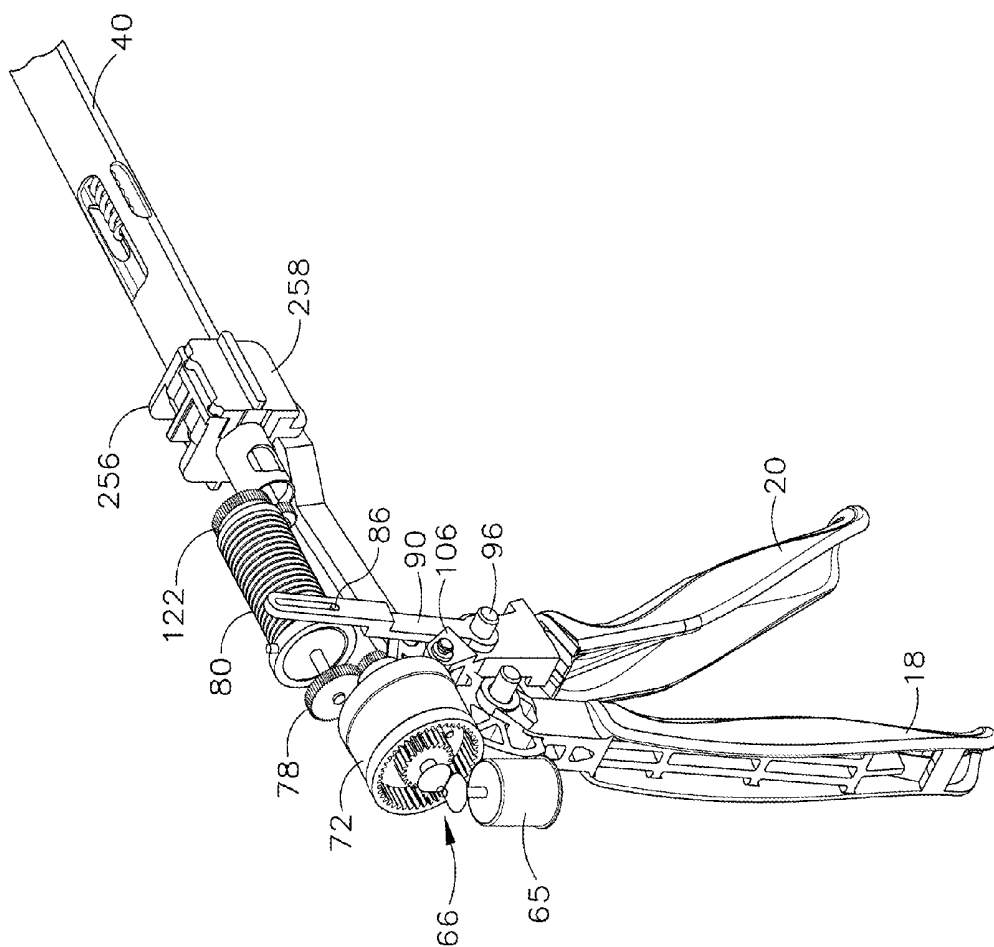


FIG. 8

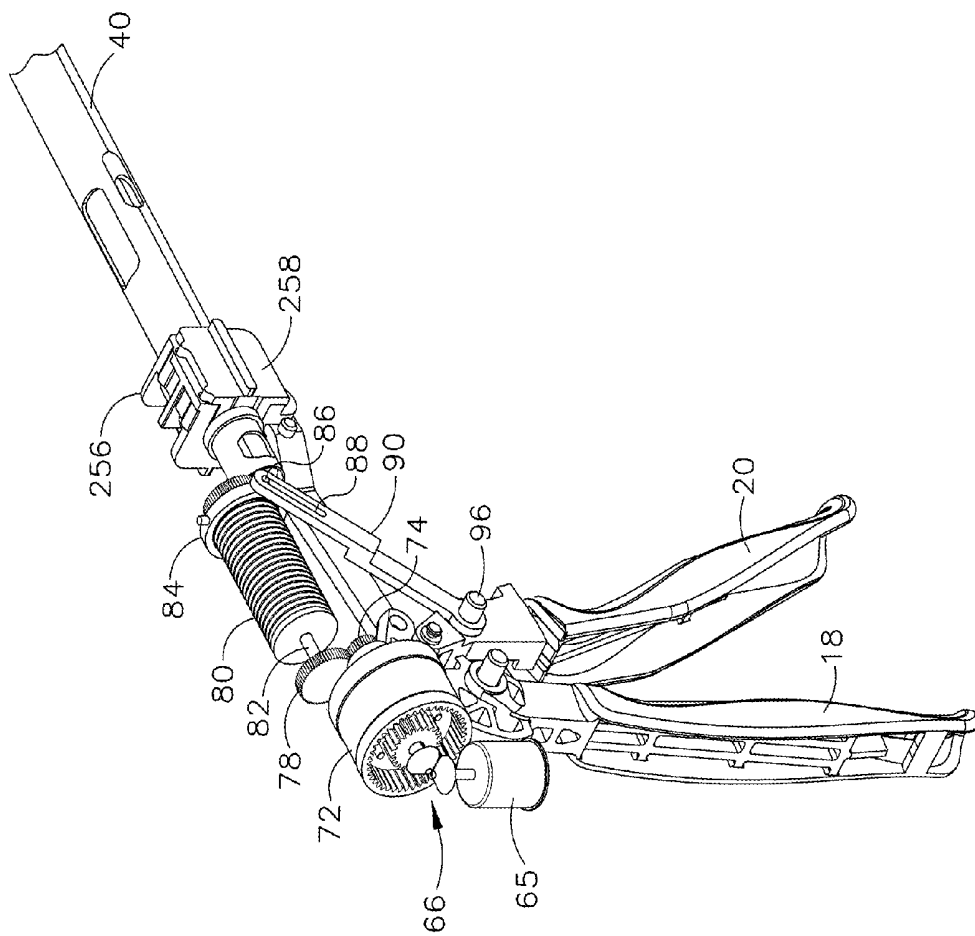


FIG. 9

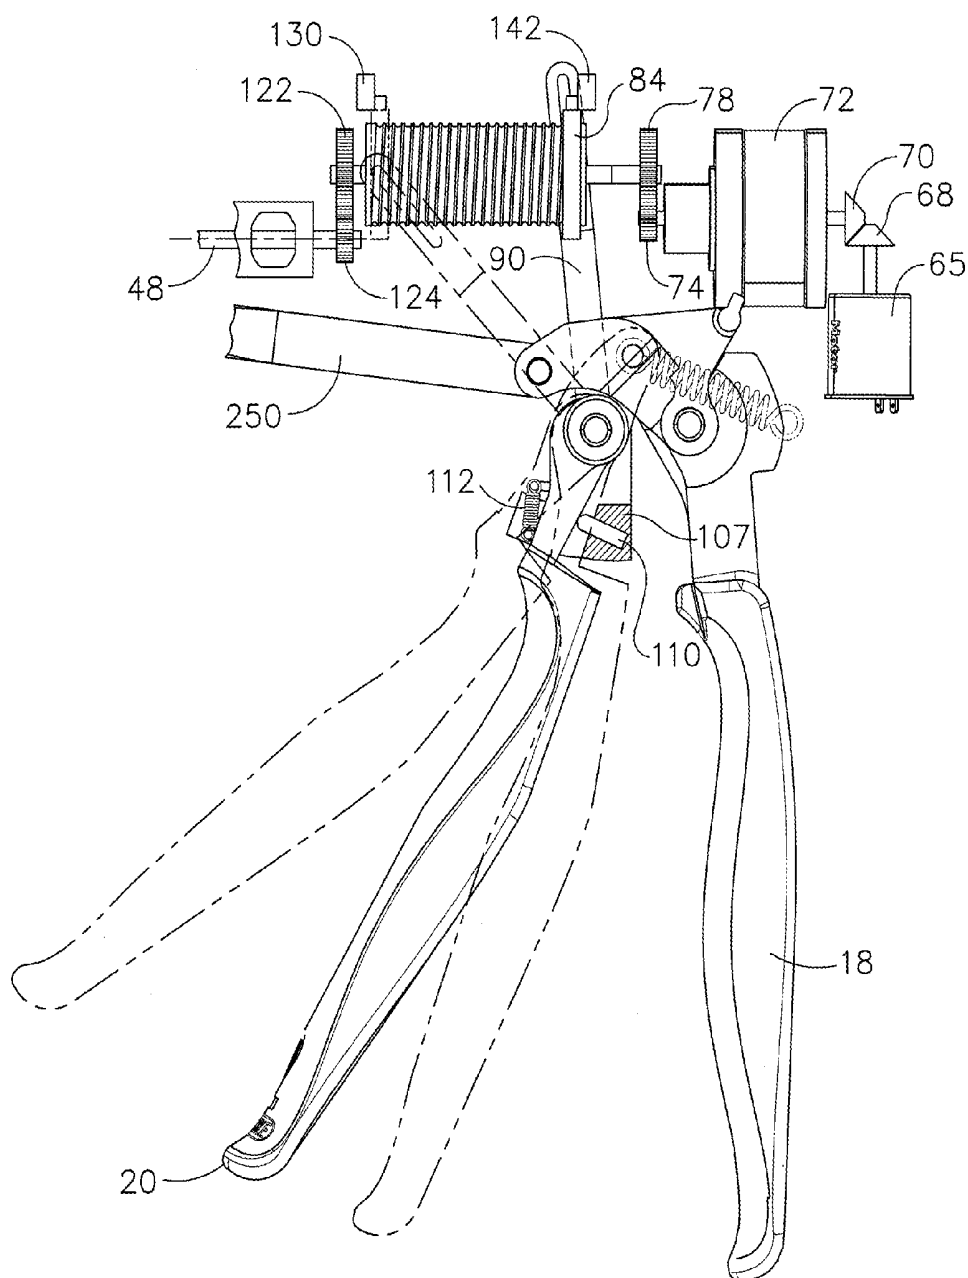


FIG. 10

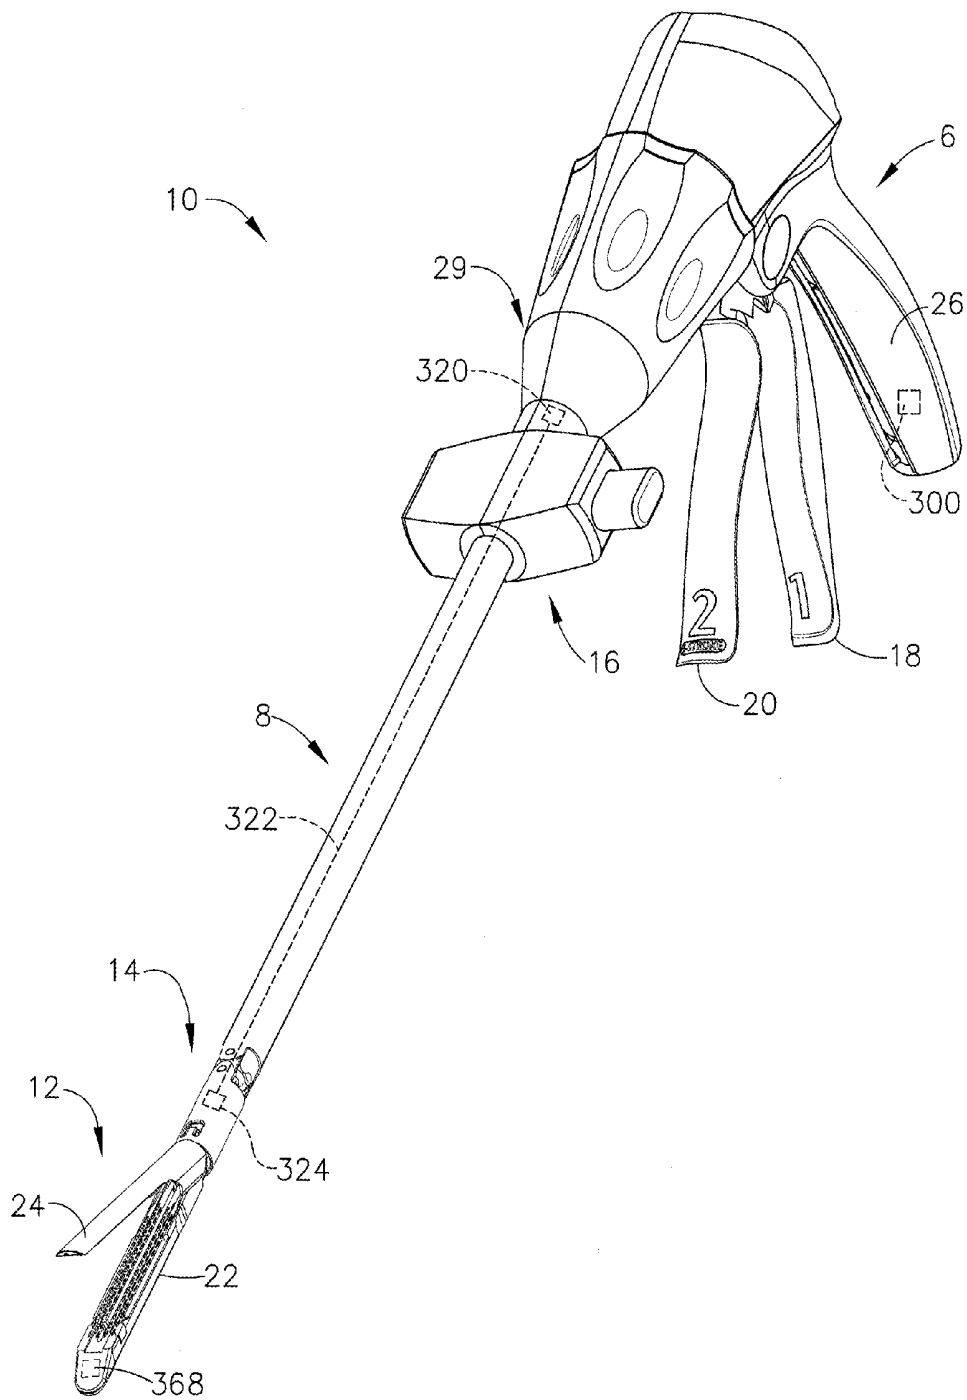


FIG. 11

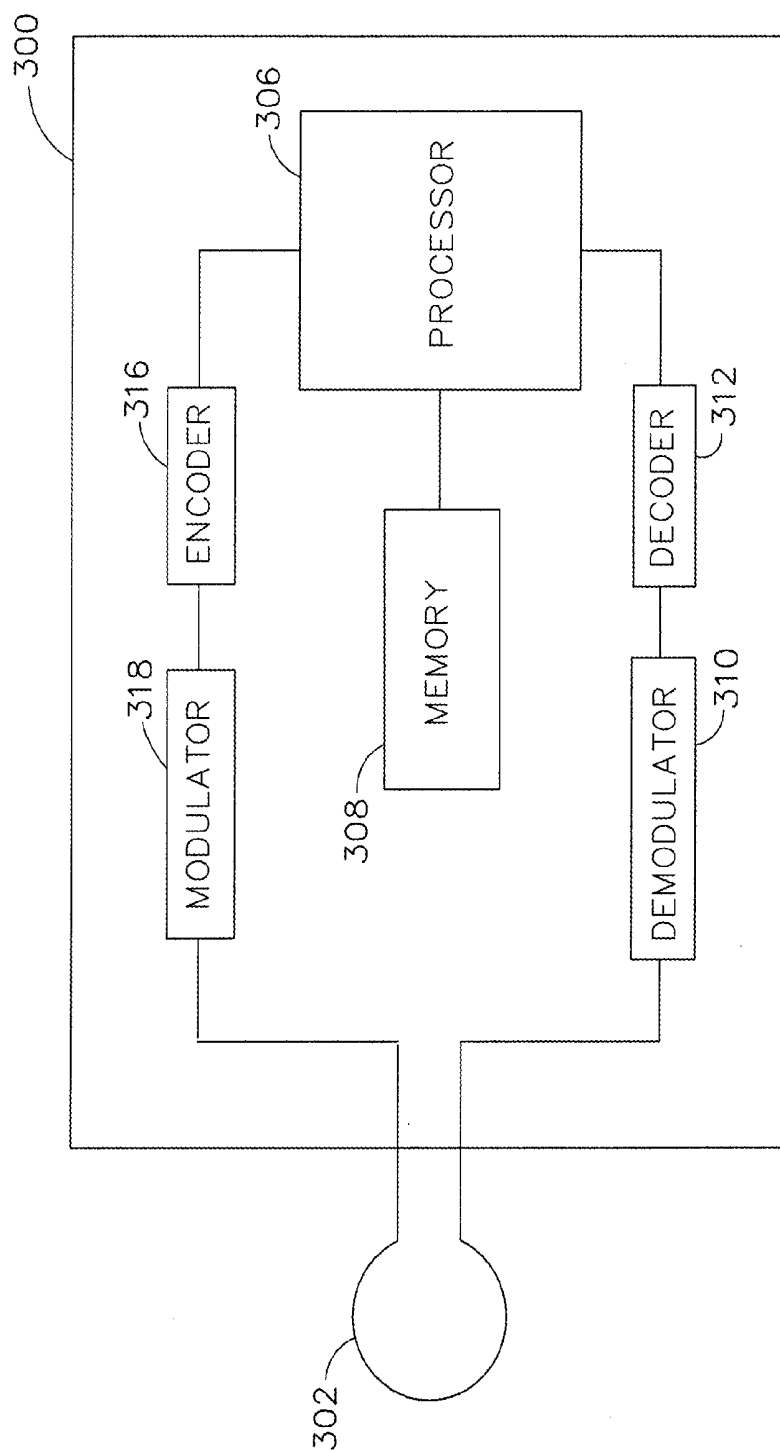


FIG. 12

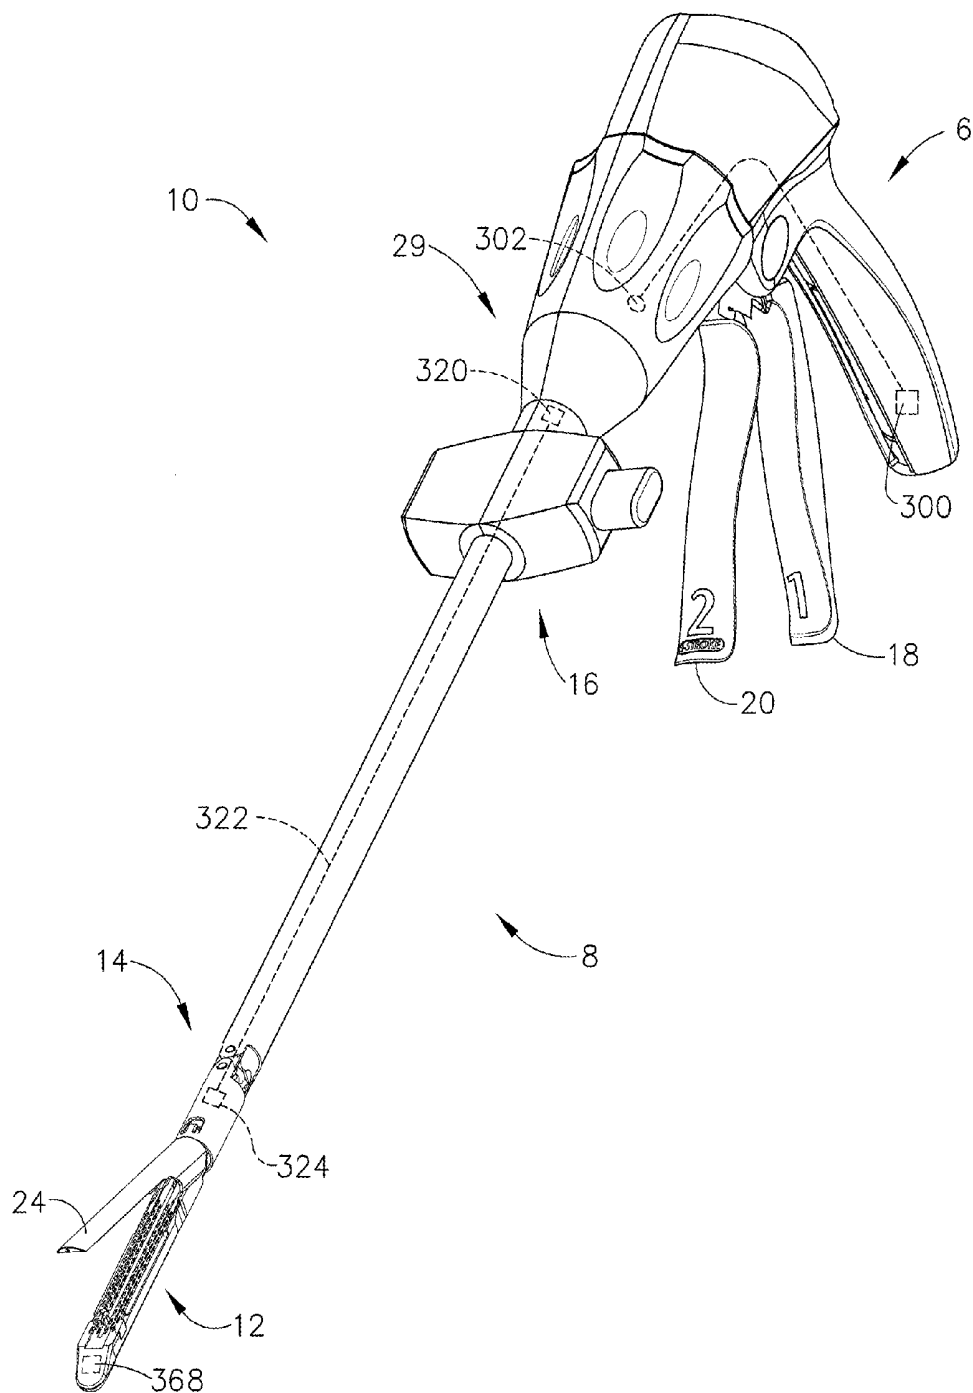


FIG. 13

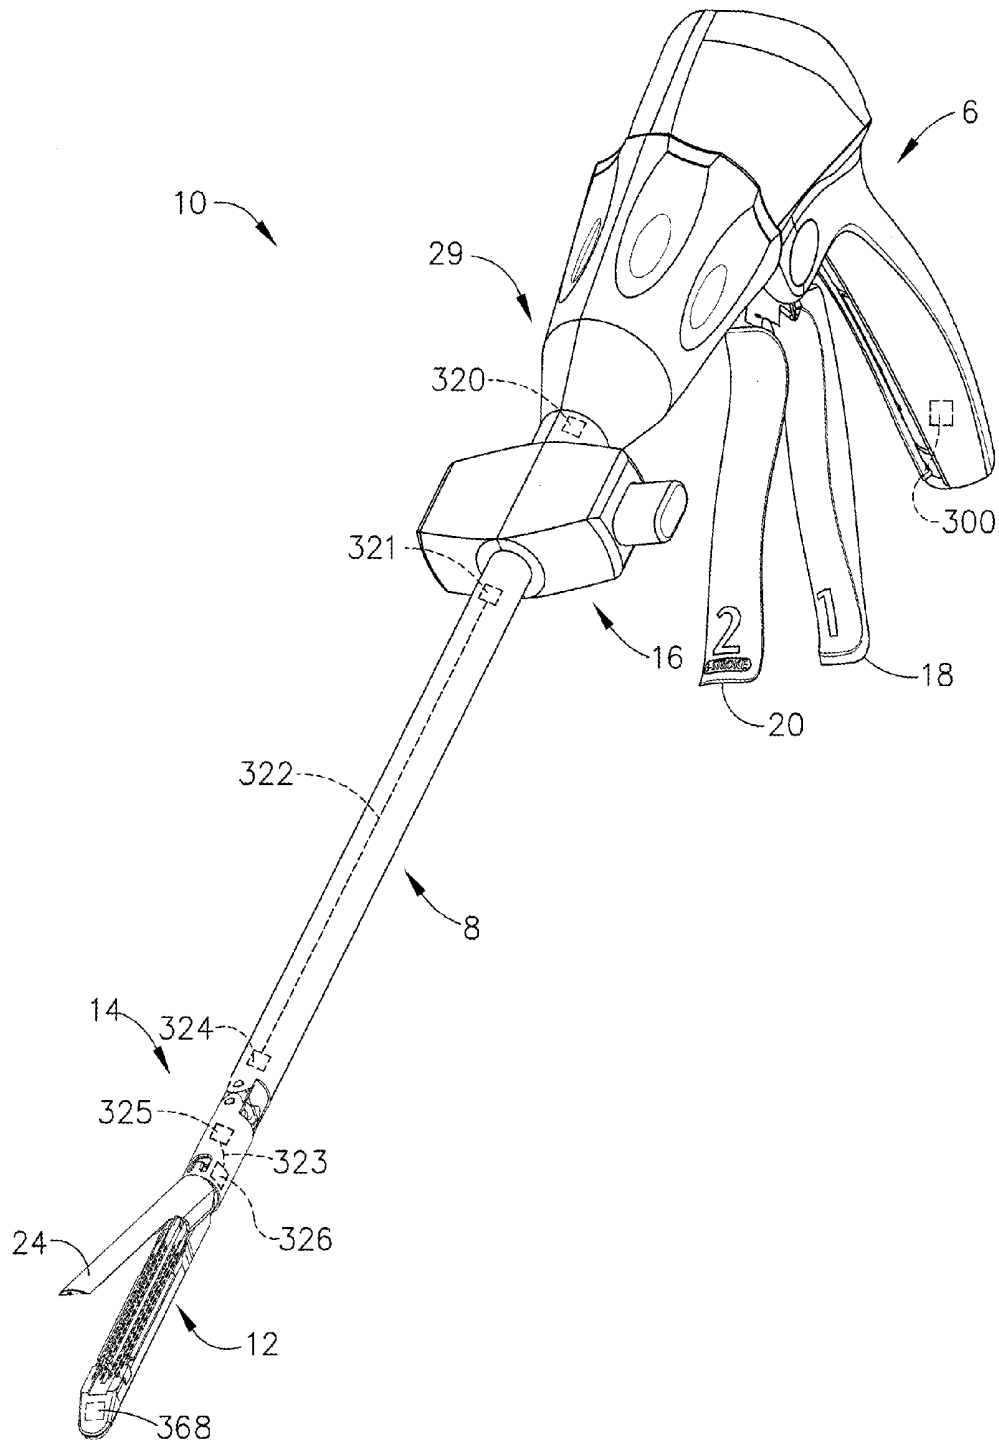


FIG. 14

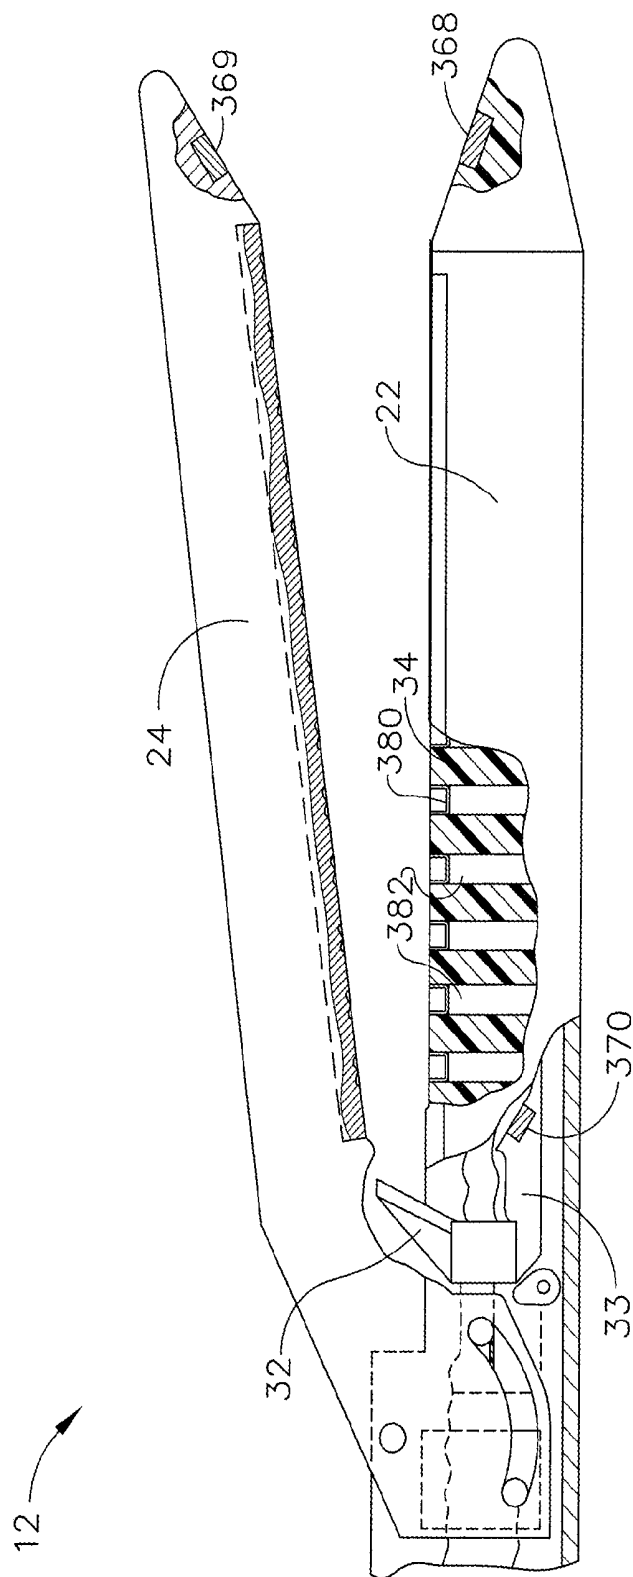


FIG. 15

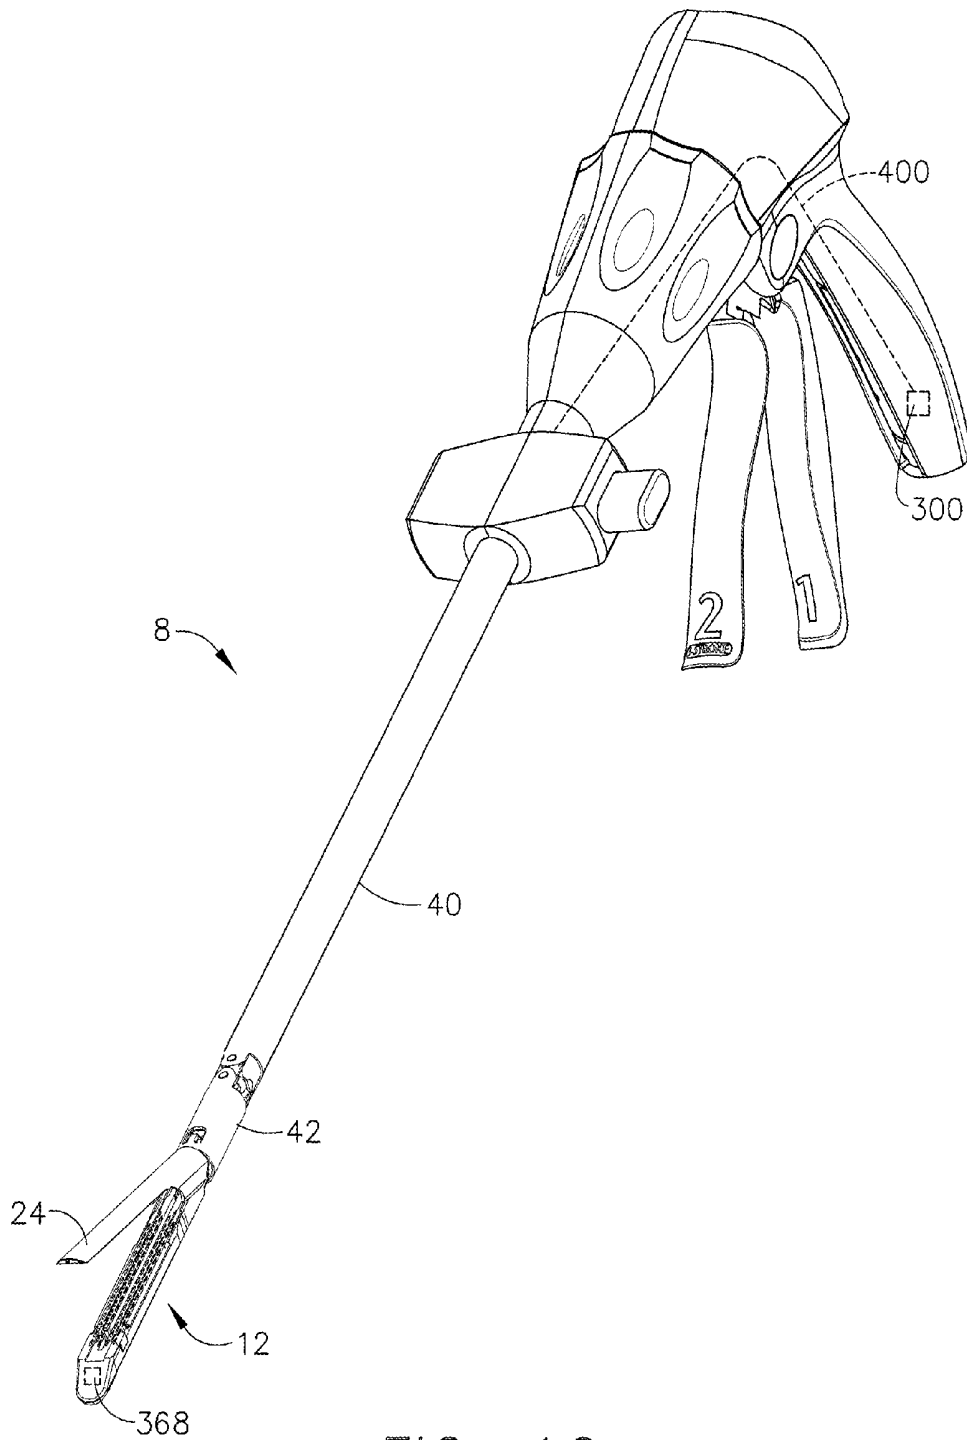


FIG. 16

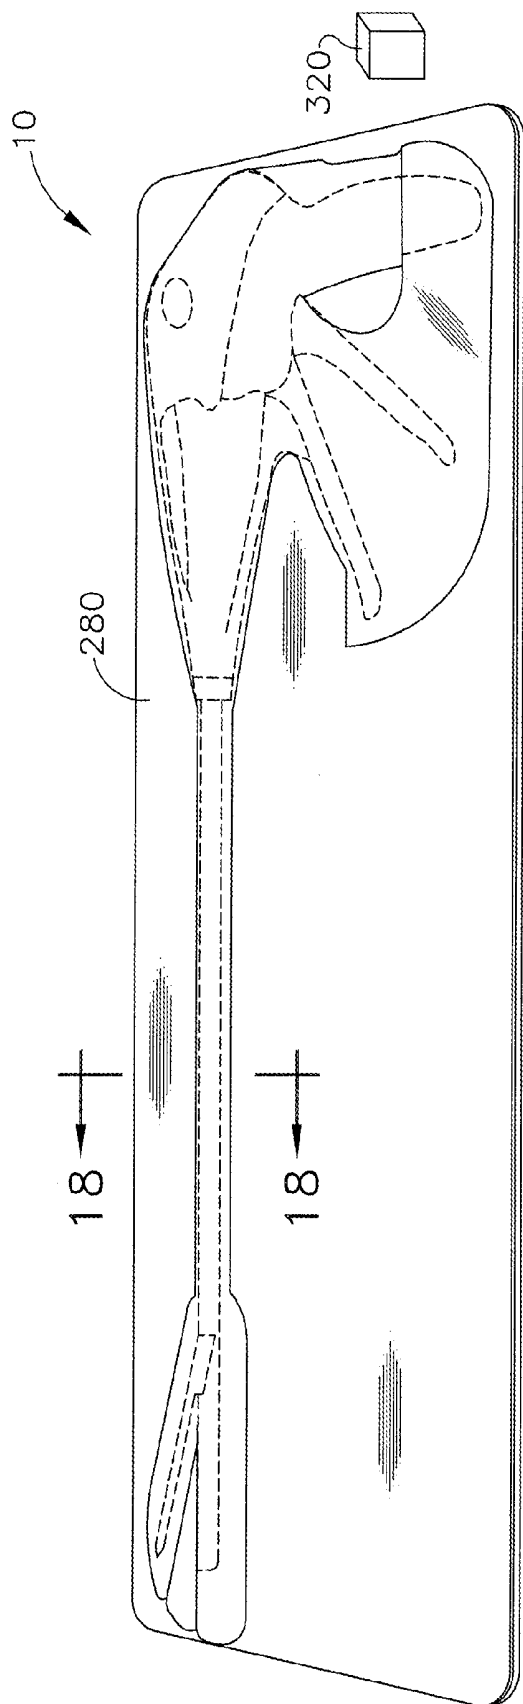


FIG. 18

FIG. 17

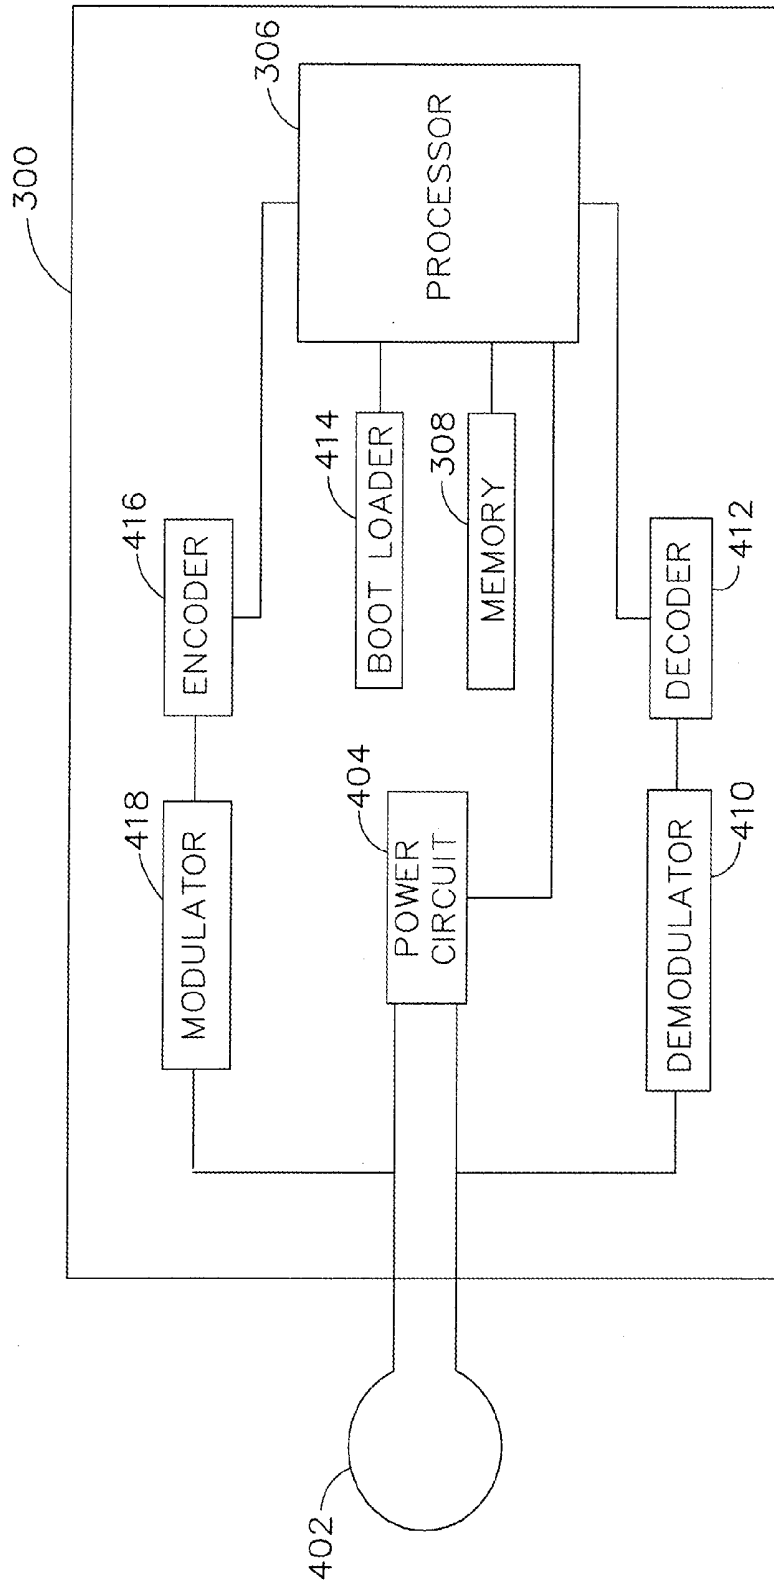
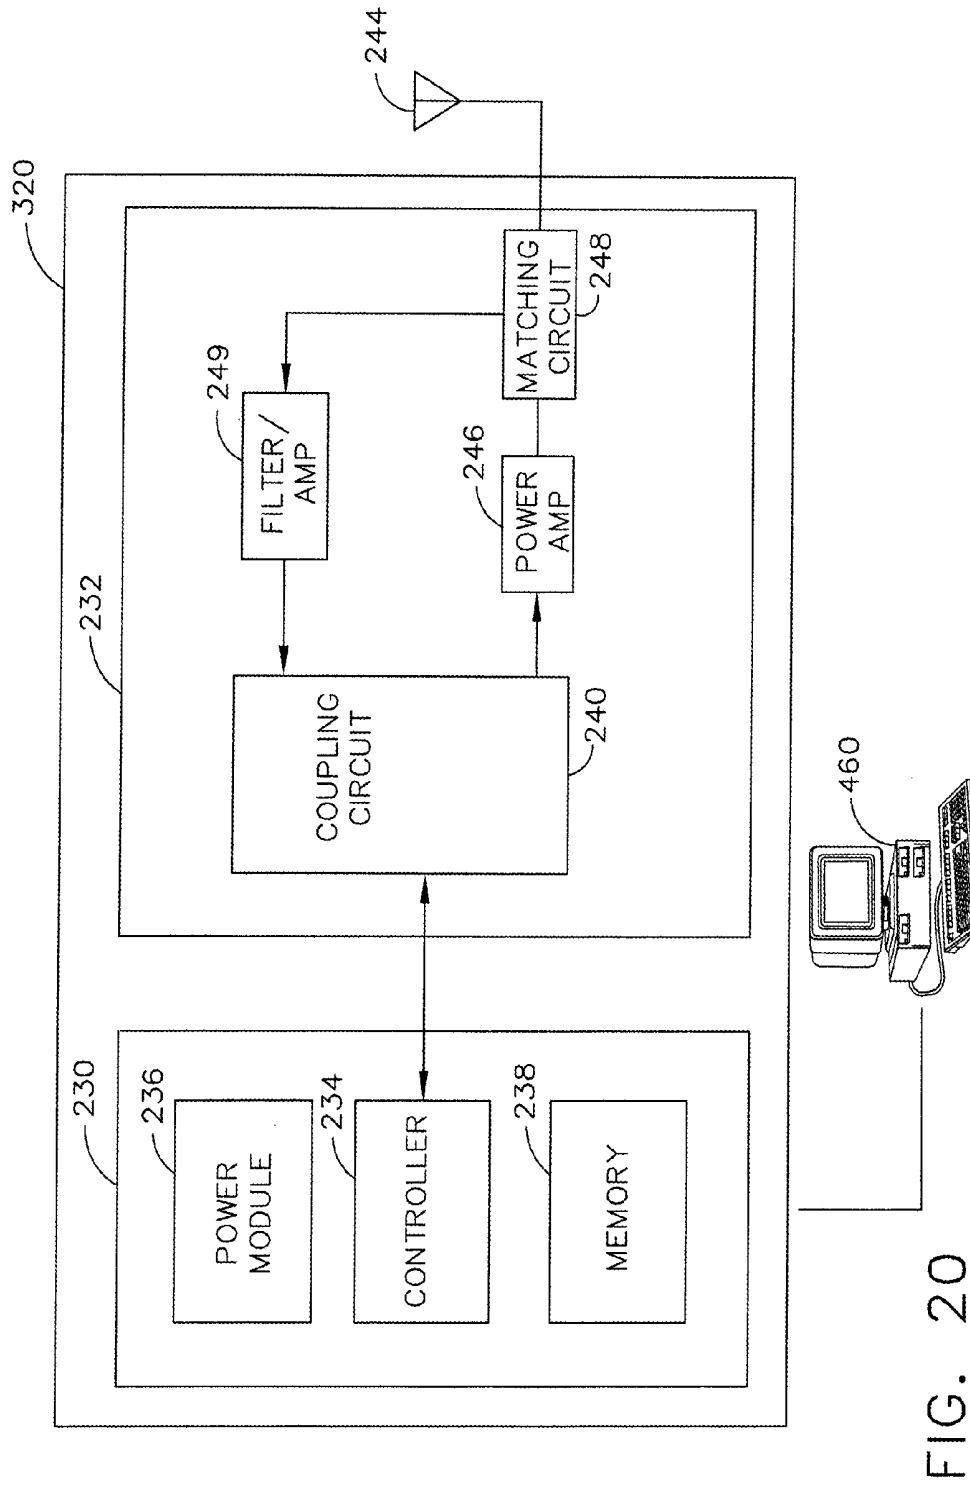


FIG. 19



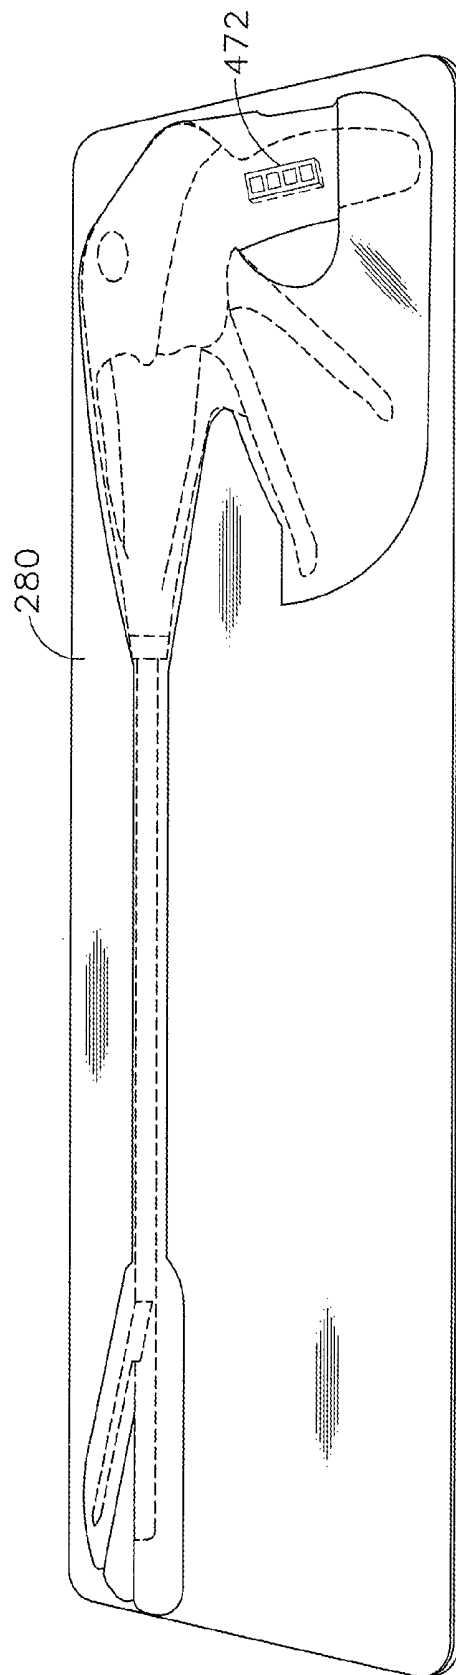


FIG. 21

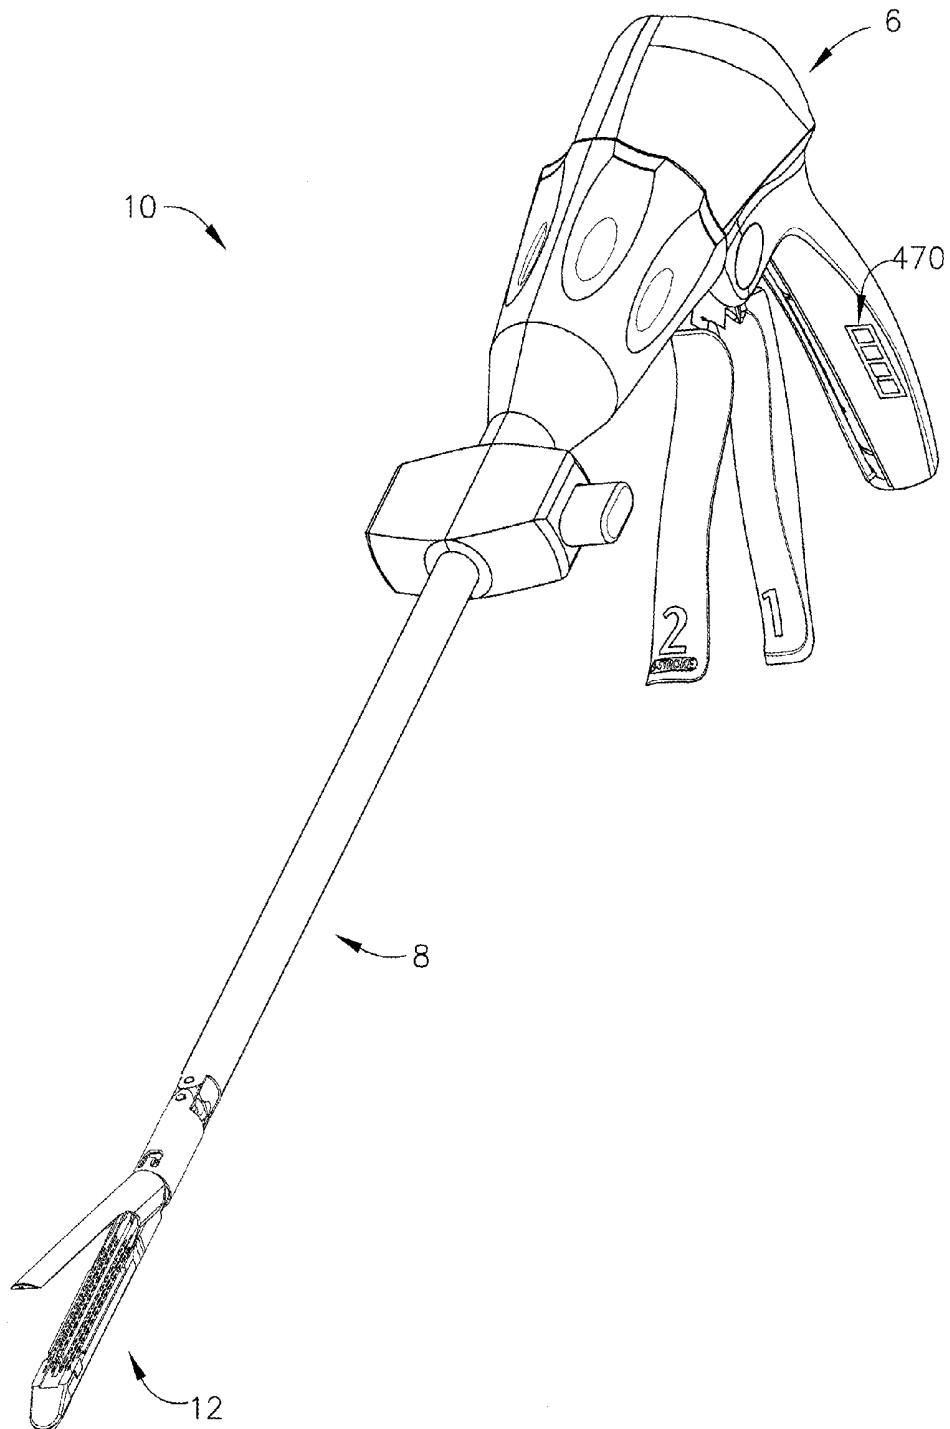


FIG. 22

SURGICAL INSTRUMENT WITH WIRELESS COMMUNICATION BETWEEN CONTROL UNIT AND SENSOR TRANSPONDERS

CROSS REFERENCE TO RELATED APPLICATION

The present application is related to the following, concurrently-filed U.S. patent applications, which are incorporated herein by reference:

(1) U.S. patent application Ser. No. 11/651,807, entitled "SURGICAL INSTRUMENT WITH WIRELESS COMMUNICATION BETWEEN CONTROL UNIT AND REMOTE SENSOR," by J. Giordano et al., now U.S. Pat. No. 8,459,520;

(2) U.S. patent application Ser. No. 11/651,806, entitled "SURGICAL INSTRUMENT WITH ELEMENTS TO COMMUNICATE BETWEEN CONTROL UNIT AND END EFFECTOR," by J. Giordano et al., now U.S. Pat. No. 7,954,682;

(3) U.S. patent application Ser. No. 11/651,768, entitled "PREVENTION OF CARTRIDGE REUSE IN A SURGICAL INSTRUMENT," by F. Shelton et al., now U.S. Pat. No. 7,721,931;

(4) U.S. patent application Ser. No. 11/651,771, entitled "POST-STERILIZATION PROGRAMMING OF SURGICAL INSTRUMENTS," by J. Swayze et al., now U.S. Pat. No. 7,738,971;

(5) U.S. patent application Ser. No. 11/651,788, entitled "INTERLOCK AND SURGICAL INSTRUMENT INCLUDING SAME," by F. Shelton et al., now U.S. Pat. No. 7,721,936; and

(6) U.S. patent application Ser. No. 11/651,785, entitled "SURGICAL INSTRUMENT WITH ENHANCED BATTERY PERFORMANCE," by F. Shelton et al., now U.S. Pat. No. 7,900,805.

BACKGROUND

Endoscopic surgical instruments are often preferred over traditional open surgical devices since a smaller incision tends to reduce the post-operative recovery time and complications. Consequently, significant development has gone into a range of endoscopic surgical instruments that are suitable for precise placement of a distal end effector at a desired surgical site through a cannula of a trocar. These distal end effectors engage the tissue in a number of ways to achieve a diagnostic or therapeutic effect (e.g., endocutter, grasper, cutter, staplers, clip applier, access device, drug/gene therapy delivery device, and energy device using ultrasound, RF, laser, etc.).

Known surgical staplers include an end effector that simultaneously makes a longitudinal incision in tissue and applies lines of staples on opposing sides of the incision. The end effector includes a pair of cooperating jaw members that, if the instrument is intended for endoscopic or laparoscopic applications, are capable of passing through a cannula passageway. One of the jaw members receives a staple cartridge having at least two laterally spaced rows of staples. The other jaw member defines an anvil having staple-forming pockets aligned with the rows of staples in the cartridge. The instrument includes a plurality of reciprocating wedges which, when driven distally, pass through openings in the staple cartridge and engage drivers supporting the staples to effect the firing of the staples toward the anvil.

An example of a surgical stapler suitable for endoscopic applications is described in U.S. Pat. No. 5,465,895, which

discloses an endocutter with distinct closing and firing actions. A clinician using this device is able to close the jaw members upon tissue to position the tissue prior to firing. Once the clinician has determined that the jaw members are properly gripping tissue, the clinician can then fire the surgical stapler with a single firing stroke, thereby severing and stapling the tissue. The simultaneous severing and stapling avoids complications that may arise when performing such actions sequentially with different surgical tools that respectively only sever and staple.

One specific advantage of being able to close upon tissue before firing is that the clinician is able to verify via an endoscope that the desired location for the cut has been achieved, including that a sufficient amount of tissue has been captured between opposing jaws. Otherwise, opposing jaws may be drawn too close together, especially pinching at their distal ends, and thus not effectively forming closed staples in the severed tissue. At the other extreme, an excessive amount of clamped tissue may cause binding and an incomplete firing.

Endoscopic staplers/cutters continue to increase in complexity and function with each generation. One of the main reasons for this is the quest to lower force-to-fire (FTF) to a level that all or a great majority of surgeons can handle. One known solution to lower FTF is use CO₂ or electrical motors. These devices have not fared much better than traditional hand-powered devices, but for a different reason. Surgeons typically prefer to experience proportionate force distribution to that being experienced by the end effector in the forming of the staple to assure them that the cutting/stapling cycle is complete, with the upper limit within the capabilities of most surgeons (usually around 15-30 lbs). They also typically want to maintain control of deploying the staples and being able to stop at anytime if the forces felt in the handle of the device feel too great or for some other clinical reason.

To address this need, so-called "power-assist" endoscopic surgical instruments have been developed in which a supplemental power source aids in the firing of the instrument. For example, in some power-assist devices, a motor provides supplemental electrical power to the power input by the user from squeezing the firing trigger. Such devices are capable of providing loading force feedback and control to the operator to reduce the firing force required to be exerted by the operator in order to complete the cutting operation. One such power-assist device is described in U.S. patent application Ser. No. 11/343,573, filed Jan. 31, 2006 by Shelton et al., entitled "Motor-driven surgical cutting and fastening instrument with loading force feedback," ("the '573 application") which is incorporated herein by reference.

These power-assist devices often include other components that purely mechanical endoscopic surgical instruments do not, such as sensors and control systems. One challenge in using such electronics in a surgical instrument is delivering power and/or data to and from the sensors, particularly when there is a free rotating joint in the surgical instrument.

SUMMARY

In one general aspect, the present invention is directed to a surgical instrument, such as an endoscopic or laparoscopic instrument. According to one embodiment, the surgical instrument comprises an end effector comprising at least one sensor transponder that is passively powered. The surgical instrument also comprises a shaft having a distal end connected to the end effector and a handle connected to a proximate end of the shaft. The handle comprises a control unit (e.g., a microcontroller) that is in communication with the

3

sensor transponder via at least one inductive coupling. Further, the surgical instrument may comprise a rotational joint for rotating the shaft. In such a case, the surgical instrument may comprise a first inductive element located in the shaft distally from the rotational joint and inductively coupled to the control unit, and a second inductive element located distally in the shaft and inductively coupled to the at least one sensor transponder. The first and second inductive elements may be connected by a wired, physical connection.

That way, the control unit may communicate with the transponder in the end effector without a direct wired connection through complex mechanical joints like the rotating joint where it may be difficult to maintain such a wired connection. In addition, because the distances between the inductive elements may be fixed and known, the couplings could be optimized for inductive transfer of energy. Also, the distances could be relatively short so that relatively low power signals could be used to thereby minimize interference with other systems in the use environment of the instrument.

In another general aspect of the present invention, the electrically conductive shaft of the surgical instrument may serve as an antenna for the control unit to wirelessly communicate signals to and from the sensor transponder. For example, the sensor transponder could be located on or disposed in a nonconductive component of the end effector, such as a plastic cartridge, thereby insulating the sensor from conductive components of the end effector and the shaft. In addition, the control unit in the handle may be electrically coupled to the shaft. In that way, the shaft and/or the end effector may serve as an antenna for the control unit by radiating signals from the control unit to the sensor and/or by receiving radiated signals from the sensor. Such a design is particularly useful in surgical instruments having complex mechanical joints (such as rotary joints), which make it difficult to use a direct wired connection between the sensor and control unit for communicating data signals.

In another embodiment, the shaft and/or components of the end effector could serve as the antenna for the sensor by radiating signals to the control unit and receiving radiated signals from the control unit. According to such an embodiment, the control unit is electrically insulated from the shaft and the end effector.

In another general aspect, the present invention is directed to a surgical instrument comprising a programmable control unit that can be programmed by a programming device after the instrument has been packaged and sterilized. In one such embodiment, the programming device may wirelessly program the control unit. The control unit may be passively powered by the wireless signals from the programming device during the programming operation. In another embodiment, the sterile container may comprise a connection interface so that the programming unit can be connected to the surgical instrument while the surgical instrument is in its sterilized container.

FIGURES

Various embodiments of the present invention are described herein by way of example in conjunction with the following figures wherein:

FIGS. 1 and 2 are perspective views of a surgical instrument according to various embodiments of the present invention;

FIGS. 3-5 are exploded views of an end effector and shaft of the instrument according to various embodiments of the present invention;

4

FIG. 6 is a side view of the end effector according to various embodiments of the present invention;

FIG. 7 is an exploded view of the handle of the instrument according to various embodiments of the present invention;

FIGS. 8 and 9 are partial perspective views of the handle according to various embodiments of the present invention;

FIG. 10 is a side view of the handle according to various embodiments of the present invention;

FIGS. 11, 13-14, 16, and 22 are perspective views of a surgical instrument according to various embodiments of the present invention;

FIGS. 12 and 19 are block diagrams of a control unit according to various embodiments of the present invention;

FIG. 15 is a side view of an end effector including a sensor transponder according to various embodiments of the present invention;

FIGS. 17 and 18 show the instrument in a sterile container according to various embodiments of the present invention;

FIG. 20 is a block diagram of the remote programming device according to various embodiments of the present invention; and

FIG. 21 is a diagram of a packaged instrument according to various embodiments of the present invention.

DETAILED DESCRIPTION

Various embodiments of the present invention are directed generally to a surgical instrument having at least one remote sensor transponder and means for communicating power and/or data signals to the transponder(s) from a control unit. The present invention may be used with any type of surgical instrument comprising at least one sensor transponder, such as endoscopic or laparoscopic surgical instruments, but is particularly useful for surgical instruments where some feature of the instrument, such as a free rotating joint, prevents or otherwise inhibits the use of a wired connection to the sensor(s). Before describing aspects of the system, one type of surgical instrument in which embodiments of the present invention may be used—an endoscopic stapling and cutting instrument (i.e., an endocutter)—is first described by way of illustration.

FIGS. 1 and 2 depict an endoscopic surgical instrument 10 that comprises a handle 6, a shaft 8, and an articulating end effector 12 pivotally connected to the shaft 8 at an articulation pivot 14. Correct placement and orientation of the end effector 12 may be facilitated by controls on the handle 6, including (1) a rotation knob 28 for rotating the closure tube (described in more detail below in connection with FIGS. 4-5) at a free rotating joint 29 of the shaft 8 to thereby rotate the end effector 12 and (2) an articulation control 16 to effect rotational articulation of the end effector 12 about the articulation pivot 14. In the illustrated embodiment, the end effector 12 is configured to act as an endocutter for clamping, severing and stapling tissue, although in other embodiments, different types of end effectors may be used, such as end effectors for other types of surgical instruments, such as graspers, cutters, staplers, clip applicators, access devices, drug/gene therapy devices, ultrasound, RF or laser devices, etc.

The handle 6 of the instrument 10 may include a closure trigger 18 and a firing trigger 20 for actuating the end effector 12. It will be appreciated that instruments having end effectors directed to different surgical tasks may have different numbers or types of triggers or other suitable controls for operating the end effector 12. The end effector 12 is shown separated from the handle 6 by the preferably elongate shaft 8. In one embodiment, a clinician or operator of the instrument 10 may articulate the end effector 12 relative to the shaft

8 by utilizing the articulation control 16, as described in more detail in pending U.S. patent application Ser. No. 11/329,020, filed Jan. 10, 2006, entitled "Surgical Instrument Having An Articulating End Effector," by Geoffrey C. Hueil et al., which is incorporated herein by reference.

The end effector 12 includes in this example, among other things, a staple channel 22 and a pivotally translatable clamping member, such as an anvil 24, which are maintained at a spacing that assures effective stapling and severing of tissue clamped in the end effector 12. The handle 6 includes a pistol grip 26 towards which a closure trigger 18 is pivotally drawn by the clinician to cause clamping or closing of the anvil 24 toward the staple channel 22 of the end effector 12 to thereby clamp tissue positioned between the anvil 24 and channel 22. The firing trigger 20 is farther outboard of the closure trigger 18. Once the closure trigger 18 is locked in the closure position, the firing trigger 20 may rotate slightly toward the pistol grip 26 so that it can be reached by the operator using one hand. Then the operator may pivotally draw the firing trigger 20 toward the pistol grip 12 to cause the stapling and severing of clamped tissue in the end effector 12. The '573 application describes various configurations for locking and unlocking the closure trigger 18. In other embodiments, different types of clamping members besides the anvil 24 could be used, such as, for example, an opposing jaw, etc.

It will be appreciated that the terms "proximal" and "distal" are used herein with reference to a clinician gripping the handle 6 of an instrument 10. Thus, the end effector 12 is distal with respect to the more proximal handle 6. It will be further appreciated that, for convenience and clarity, spatial terms such as "vertical" and "horizontal" are used herein with respect to the drawings. However, surgical instruments are used in many orientations and positions, and these terms are not intended to be limiting and absolute.

The closure trigger 18 may be actuated first. Once the clinician is satisfied with the positioning of the end effector 12, the clinician may draw back the closure trigger 18 to its fully closed, locked position proximate to the pistol grip 26. The firing trigger 20 may then be actuated. The firing trigger 20 returns to the open position (shown in FIGS. 1 and 2) when the clinician removes pressure. A release button 30 on the handle 6, and in this example, on the pistol grip 26 of the handle, when depressed may release the locked closure trigger 18.

FIG. 3 is an exploded view of the end effector 12 according to various embodiments. As shown in the illustrated embodiment, the end effector 12 may include, in addition to the previously-mentioned channel 22 and anvil 24, a cutting instrument 32, a sled 33, a staple cartridge 34 that is removably seated in the channel 22, and a helical screw shaft 36. The cutting instrument 32 may be, for example, a knife. The anvil 24 may be pivotably opened and closed at a pivot point 25 connected to the proximate end of the channel 22. The anvil 24 may also include a tab 27 at its proximate end that is inserted into a component of the mechanical closure system (described further below) to open and close the anvil 24. When the closure trigger 18 is actuated, that is, drawn in by a user of the instrument 10, the anvil 24 may pivot about the pivot point 25 into the clamped or closed position. If clamping of the end effector 12 is satisfactory, the operator may actuate the firing trigger 20, which, as explained in more detail below, causes the knife 32 and sled 33 to travel longitudinally along the channel 22, thereby cutting tissue clamped within the end effector 12. The movement of the sled 33 along the channel 22 causes the staples of the staple cartridge 34 to be driven through the severed tissue and against the closed anvil 24, which turns the staples to fasten the severed tissue. U.S. Pat.

No. 6,978,921, entitled "Surgical stapling instrument incorporating an E-beam firing mechanism," which is incorporated herein by reference, provides more details about such two-stroke cutting and fastening instruments. The sled 33 may be part of the cartridge 34, such that when the knife 32 retracts following the cutting operation, the sled 33 does not retract. The channel 22 and the anvil 24 may be made of an electrically conductive material (such as metal) so that they may serve as part of the antenna that communicates with the sensor(s) in the end effector, as described further below. The cartridge 34 could be made of a nonconductive material (such as plastic) and the sensor may be connected to or disposed in the cartridge 34, as described further below.

It should be noted that although the embodiments of the instrument 10 described herein employ an end effector 12 that staples the severed tissue, in other embodiments different techniques for fastening or sealing the severed tissue may be used. For example, end effectors that use RF energy or adhesives to fasten the severed tissue may also be used. U.S. Pat. No. 5,709,680, entitled "Electrosurgical Hemostatic Device" to Yates et al., and U.S. Pat. No. 5,688,270, entitled "Electrosurgical Hemostatic Device With Recessed And/Or Offset Electrodes" to Yates et al., which are incorporated herein by reference, discloses cutting instruments that use RF energy to fasten the severed tissue. U.S. patent application Ser. No. 11/267,811 to Morgan et al. and U.S. patent application Ser. No. 11/267,383 to Shelton et al., which are also incorporated herein by reference, disclose cutting instruments that use adhesives to fasten the severed tissue. Accordingly, although the description herein refers to cutting/stapling operations and the like, it should be recognized that this is an exemplary embodiment and is not meant to be limiting. Other tissue-fastening techniques may also be used.

FIGS. 4 and 5 are exploded views and FIG. 6 is a side view of the end effector 12 and shaft 8 according to various embodiments. As shown in the illustrated embodiment, the shaft 8 may include a proximate closure tube 40 and a distal closure tube 42 pivotably linked by a pivot links 44. The distal closure tube 42 includes an opening 45 into which the tab 27 on the anvil 24 is inserted in order to open and close the anvil 24. Disposed inside the closure tubes 40, 42 may be a proximate spine tube 46. Disposed inside the proximate spine tube 46 may be a main rotational (or proximate) drive shaft 48 that communicates with a secondary (or distal) drive shaft 50 via a bevel gear assembly 52. The secondary drive shaft 50 is connected to a drive gear 54 that engages a proximate drive gear 56 of the helical screw shaft 36. The vertical bevel gear 52b may sit and pivot in an opening 57 in the distal end of the proximate spine tube 46. A distal spine tube 58 may be used to enclose the secondary drive shaft 50 and the drive gears 54, 56. Collectively, the main drive shaft 48, the secondary drive shaft 50, and the articulation assembly (e.g., the bevel gear assembly 52a-c), are sometimes referred to herein as the "main drive shaft assembly." The closure tubes 40, 42 may be made of electrically conductive material (such as metal) so that they may serve as part of the antenna, as described further below. Components of the main drive shaft assembly (e.g., the drive shafts 48, 50) may be made of a nonconductive material (such as plastic).

A bearing 38, positioned at a distal end of the staple channel 22, receives the helical drive screw 36, allowing the helical drive screw 36 to freely rotate with respect to the channel 22. The helical screw shaft 36 may interface a threaded opening (not shown) of the knife 32 such that rotation of the shaft 36 causes the knife 32 to translate distally or proximally (depending on the direction of the rotation) through the staple channel 22. Accordingly, when the main drive shaft 48 is

caused to rotate by actuation of the firing trigger 20 (as explained in more detail below), the bevel gear assembly 52a-c causes the secondary drive shaft 50 to rotate, which in turn, because of the engagement of the drive gears 54, 56, causes the helical screw shaft 36 to rotate, which causes the knife 32 to travel longitudinally along the channel 22 to cut any tissue clamped within the end effector. The sled 33 may be made of, for example, plastic, and may have a sloped distal surface. As the sled 33 traverses the channel 22, the sloped forward surface may push up or drive the staples in the staple cartridge 34 through the clamped tissue and against the anvil 24. The anvil 24 turns the staples, thereby stapling the severed tissue. When the knife 32 is retracted, the knife 32 and sled 33 may become disengaged, thereby leaving the sled 33 at the distal end of the channel 22.

According to various embodiments, as shown FIGS. 7-10, the surgical instrument may include a battery 64 in the handle 6. The illustrated embodiment provides user-feedback regarding the deployment and loading force of the cutting instrument in the end effector 12. In addition, the embodiment may use power provided by the user in retracting the firing trigger 18 to power the instrument 10 (a so-called "power assist" mode). As shown in the illustrated embodiment, the handle 6 includes exterior lower side pieces 59, 60 and exterior upper side pieces 61, 62 that fit together to form, in general, the exterior of the handle 6. The handle pieces 59-62 may be made of an electrically nonconductive material, such as plastic. A battery 64 may be provided in the pistol grip portion 26 of the handle 6. The battery 64 powers a motor 65 disposed in an upper portion of the pistol grip portion 26 of the handle 6. The battery 64 may be constructed according to any suitable construction or chemistry including, for example, a Li-ion chemistry such as LiCoO_2 or LiNiO_2 , a Nickel Metal Hydride chemistry, etc. According to various embodiments, the motor 65 may be a DC brushed driving motor having a maximum rotation of, approximately, 5000 RPM to 100,000 RPM. The motor 64 may drive a 90° bevel gear assembly 66 comprising a first bevel gear 68 and a second bevel gear 70. The bevel gear assembly 66 may drive a planetary gear assembly 72. The planetary gear assembly 72 may include a pinion gear 74 connected to a drive shaft 76. The pinion gear 74 may drive a mating ring gear 78 that drives a helical gear drum 80 via a drive shaft 82. A ring 84 may be threaded on the helical gear drum 80. Thus, when the motor 65 rotates, the ring 84 is caused to travel along the helical gear drum 80 by means of the interposed bevel gear assembly 66, planetary gear assembly 72 and ring gear 78.

The handle 6 may also include a run motor sensor 110 in communication with the firing trigger 20 to detect when the firing trigger 20 has been drawn in (or "closed") toward the pistol grip portion 26 of the handle 6 by the operator to thereby actuate the cutting/stapling operation by the end effector 12. The sensor 110 may be a proportional sensor such as, for example, a rheostat or variable resistor. When the firing trigger 20 is drawn in, the sensor 110 detects the movement, and sends an electrical signal indicative of the voltage (or power) to be supplied to the motor 65. When the sensor 110 is a variable resistor or the like, the rotation of the motor 65 may be generally proportional to the amount of movement of the firing trigger 20. That is, if the operator only draws or closes the firing trigger 20 in a little bit, the rotation of the motor 65 is relatively low. When the firing trigger 20 is fully drawn in (or in the fully closed position), the rotation of the motor 65 is at its maximum. In other words, the harder the user pulls on the firing trigger 20, the more voltage is applied to the motor 65, causing greater rates of rotation. In another embodiment, for example, the control unit (described further below) may

output a PWM control signal to the motor 65 based on the input from the sensor 110 in order to control the motor 65.

The handle 6 may include a middle handle piece 104 adjacent to the upper portion of the firing trigger 20. The handle 6 also may comprise a bias spring 112 connected between posts on the middle handle piece 104 and the firing trigger 20. The bias spring 112 may bias the firing trigger 20 to its fully open position. In that way, when the operator releases the firing trigger 20, the bias spring 112 will pull the firing trigger 20 to its open position, thereby removing actuation of the sensor 110, thereby stopping rotation of the motor 65. Moreover, by virtue of the bias spring 112, any time a user closes the firing trigger 20, the user will experience resistance to the closing operation, thereby providing the user with feedback as to the amount of rotation exerted by the motor 65. Further, the operator could stop retracting the firing trigger 20 to thereby remove force from the sensor 100, to thereby stop the motor 65. As such, the user may stop the deployment of the end effector 12, thereby providing a measure of control of the cutting/fastening operation to the operator.

The distal end of the helical gear drum 80 includes a distal drive shaft 120 that drives a ring gear 122, which mates with a pinion gear 124. The pinion gear 124 is connected to the main drive shaft 48 of the main drive shaft assembly. In that way, rotation of the motor 65 causes the main drive shaft assembly to rotate, which causes actuation of the end effector 12, as described above.

The ring 84 threaded on the helical gear drum 80 may include a post 86 that is disposed within a slot 88 of a slotted arm 90. The slotted arm 90 has an opening 92 at its opposite end 94 that receives a pivot pin 96 that is connected between the handle exterior side pieces 59, 60. The pivot pin 96 is also disposed through an opening 100 in the firing trigger 20 and an opening 102 in the middle handle piece 104.

In addition, the handle 6 may include a reverse motor (or end-of-stroke sensor) 130 and a stop motor (or beginning-of-stroke) sensor 142. In various embodiments, the reverse motor sensor 130 may be a limit switch located at the distal end of the helical gear drum 80 such that the ring 84 threaded on the helical gear drum 80 contacts and trips the reverse motor sensor 130 when the ring 84 reaches the distal end of the helical gear drum 80. The reverse motor sensor 130, when activated, sends a signal to the control unit which sends a signal to the motor 65 to reverse its rotation direction, thereby withdrawing the knife 32 of the end effector 12 following the cutting operation.

The stop motor sensor 142 may be, for example, a normally-closed limit switch. In various embodiments, it may be located at the proximate end of the helical gear drum 80 so that the ring 84 trips the switch 142 when the ring 84 reaches the proximate end of the helical gear drum 80.

In operation, when an operator of the instrument 10 pulls back the firing trigger 20, the sensor 110 detects the deployment of the firing trigger 20 and sends a signal to the control unit which sends a signal to the motor 65 to cause forward rotation of the motor 65 at, for example, a rate proportional to how hard the operator pulls back the firing trigger 20. The forward rotation of the motor 65 in turn causes the ring gear 78 at the distal end of the planetary gear assembly 72 to rotate, thereby causing the helical gear drum 80 to rotate, causing the ring 84 threaded on the helical gear drum 80 to travel distally along the helical gear drum 80. The rotation of the helical gear drum 80 also drives the main drive shaft assembly as described above, which in turn causes deployment of the knife 32 in the end effector 12. That is, the knife 32 and sled 33 are caused to traverse the channel 22 longitudinally, thereby cutting tissue clamped in the end effector 12. Also,

the stapling operation of the end effector **12** is caused to happen in embodiments where a stapling-type end effector is used.

By the time the cutting/stapling operation of the end effector **12** is complete, the ring **84** on the helical gear drum **80** will have reached the distal end of the helical gear drum **80**, thereby causing the reverse motor sensor **130** to be tripped, which sends a signal to the control unit which sends a signal to the motor **65** to cause the motor **65** to reverse its rotation. This in turn causes the knife **32** to retract, and also causes the ring **84** on the helical gear drum **80** to move back to the proximate end of the helical gear drum **80**.

The middle handle piece **104** includes a backside shoulder **106** that engages the slotted arm **90** as best shown in FIGS. **8** and **9**. The middle handle piece **104** also has a forward motion stop **107** that engages the firing trigger **20**. The movement of the slotted arm **90** is controlled, as explained above, by rotation of the motor **65**. When the slotted arm **90** rotates CCW as the ring **84** travels from the proximate end of the helical gear drum **80** to the distal end, the middle handle piece **104** will be free to rotate CCW. Thus, as the user draws in the firing trigger **20**, the firing trigger **20** will engage the forward motion stop **107** of the middle handle piece **104**, causing the middle handle piece **104** to rotate CCW. Due to the backside shoulder **106** engaging the slotted arm **90**, however, the middle handle piece **104** will only be able to rotate CCW as far as the slotted arm **90** permits. In that way, if the motor **65** should stop rotating for some reason, the slotted arm **90** will stop rotating, and the user will not be able to further draw in the firing trigger **20** because the middle handle piece **104** will not be free to rotate CCW due to the slotted arm **90**.

Components of an exemplary closure system for closing (or clamping) the anvil **24** of the end effector **12** by retracting the closure trigger **18** are also shown in FIGS. **7-10**. In the illustrated embodiment, the closure system includes a yoke **250** connected to the closure trigger **18** by a pin **251** that is inserted through aligned openings in both the closure trigger **18** and the yoke **250**. A pivot pin **252**, about which the closure trigger **18** pivots, is inserted through another opening in the closure trigger **18** which is offset from where the pin **251** is inserted through the closure trigger **18**. Thus, retraction of the closure trigger **18** causes the upper part of the closure trigger **18**, to which the yoke **250** is attached via the pin **251**, to rotate CCW. The distal end of the yoke **250** is connected, via a pin **254**, to a first closure bracket **256**. The first closure bracket **256** connects to a second closure bracket **258**. Collectively, the closure brackets **256**, **258** define an opening in which the proximate end of the proximate closure tube **40** (see FIG. **4**) is seated and held such that longitudinal movement of the closure brackets **256**, **258** causes longitudinal motion by the proximate closure tube **40**. The instrument **10** also includes a closure rod **260** disposed inside the proximate closure tube **40**. The closure rod **260** may include a window **261** into which a post **263** on one of the handle exterior pieces, such as exterior lower side piece **59** in the illustrated embodiment, is disposed to fixedly connect the closure rod **260** to the handle **6**. In that way, the proximate closure tube **40** is capable of moving longitudinally relative to the closure rod **260**. The closure rod **260** may also include a distal collar **267** that fits into a cavity **269** in proximate spine tube **46** and is retained therein by a cap **271** (see FIG. **4**).

In operation, when the yoke **250** rotates due to retraction of the closure trigger **18**, the closure brackets **256**, **258** cause the proximate closure tube **40** to move distally (i.e., away from the handle end of the instrument **10**), which causes the distal closure tube **42** to move distally, which causes the anvil **24** to rotate about the pivot point **25** into the clamped or closed

position. When the closure trigger **18** is unlocked from the locked position, the proximate closure tube **40** is caused to slide proximally, which causes the distal closure tube **42** to slide proximally, which, by virtue of the tab **27** being inserted in the window **45** of the distal closure tube **42**, causes the anvil **24** to pivot about the pivot point **25** into the open or unclamped position. In that way, by retracting and locking the closure trigger **18**, an operator may clamp tissue between the anvil **24** and channel **22**, and may unclamp the tissue following the cutting/stapling operation by unlocking the closure trigger **18** from the locked position.

The control unit (described further below) may receive the outputs from end-of-stroke and beginning-of-stroke sensors **130**, **142** and the run-motor sensor **110**, and may control the motor **65** based on the inputs. For example, when an operator initially pulls the firing trigger **20** after locking the closure trigger **18**, the run-motor sensor **110** is actuated. If the staple cartridge **34** is present in the end effector **12**, a cartridge lockout sensor (not shown) may be closed, in which case the control unit may output a control signal to the motor **65** to cause the motor **65** to rotate in the forward direction. When the end effector **12** reaches the end of its stroke, the reverse motor sensor **130** will be activated. The control unit may receive this output from the reverse motor sensor **130** and cause the motor **65** to reverse its rotational direction. When the knife **32** is fully retracted, the stop motor sensor switch **142** is activated, causing the control unit to stop the motor **65**.

In other embodiments, rather than a proportional-type sensor **110**, an on-off type sensor could be used. In such embodiments, the rate of rotation of the motor **65** would not be proportional to the force applied by the operator. Rather, the motor **65** would generally rotate at a constant rate. But the operator would still experience force feedback because the firing trigger **20** is geared into the gear drive train.

The instrument **10** may include a number of sensor transponders in the end effector **12** for sensing various conditions related to the end effector **12**, such as sensor transponders for determining the status of the staple cartridge **34** (or other type of cartridge depending on the type of surgical instrument), the progress of the stapler during closure and firing, etc. The sensor transponders may be passively powered by inductive signals, as described further below, although in other embodiments the transponders could be powered by a remote power source, such as a battery in the end effector **12**, for example. The sensor transponder(s) could include magnetoresistive, optical, electromechanical, RFID, MEMS, motion or pressure sensors, for example. These sensor transponders may be in communication with a control unit **300**, which may be housed in the handle **6** of the instrument **10**, for example, as shown in FIG. **11**.

As shown in FIG. **12**, according to various embodiments the control unit **300** may comprise a processor **306** and one or more memory units **308**. By executing instruction code stored in the memory **308**, the processor **306** may control various components of the instrument **10**, such as the motor **65** or a user display (not shown), based on inputs received from the various end effector sensor transponders and other sensor(s) (such as the run-motor sensor **110**, the end-of-stroke sensor **130**, and the beginning-of-stroke sensor **142**, for example). The control unit **300** may be powered by the battery **64** during surgical use of instrument **10**. The control unit **300** may comprise an inductive element **302** (e.g., a coil or antenna) to pick up wireless signals from the sensor transponders, as described in more detail below. Input signals received by the inductive element **302** acting as a receiving antenna may be demodulated by a demodulator **310** and decoded by a decoder **312**. The input signals may comprise data from the sensor

11

transponders in the end effector 12, which the processor 306 may use to control various aspects of the instrument 10.

To transmit signals to the sensor transponders, the control unit 300 may comprise an encoder 316 for encoding the signals and a modulator 318 for modulating the signals according to the modulation scheme. The inductive element 302 may act as the transmitting antenna. The control unit 300 may communicate with the sensor transponders using any suitable wireless communication protocol and any suitable frequency (e.g., an ISM band). Also, the control unit 300 may transmit signals at a different frequency range than the frequency range of the received signals from the sensor transponders. Also, although only one antenna (inductive element 302) is shown in FIG. 12, in other embodiments the control unit 300 may have separate receiving and transmitting antennas.

According to various embodiments, the control unit 300 may comprise a microcontroller, a microprocessor, a field programmable gate array (FPGA), one or more other types of integrated circuits (e.g., RF receivers and PWM controllers), and/or discrete passive components. The control units may also be embodied as system-on-chip (SoC) or a system-in-package (SIP), for example.

As shown in FIG. 11, the control unit 300 may be housed in the handle 6 of the instrument 10 and one or more of the sensor transponders 368 for the instrument 10 may be located in the end effector 12. To deliver power and/or transmit data to or from the sensor transponders 368 in the end effector 12, the inductive element 302 of the control unit 300 may be inductively coupled to a secondary inductive element (e.g., a coil) 320 positioned in the shaft 8 distally from the rotation joint 29. The secondary inductive element 320 is preferably electrically insulated from the conductive shaft 8.

The secondary inductive element 320 may be connected by an electrically conductive, insulated wire 322 to a distal inductive element (e.g., a coil) 324 located near the end effector 12, and preferably distally relative to the articulation pivot 14. The wire 322 may be made of an electrically conductive polymer and/or metal (e.g., copper) and may be sufficiently flexible so that it could pass through the articulation pivot 14 and not be damaged by articulation. The distal inductive element 324 may be inductively coupled to the sensor transponder 368 in, for example, the cartridge 34 of the end effector 12. The transponder 368, as described in more detail below, may include an antenna (or coil) for inductive coupling to the distal coil 324, a sensor and integrated control electronics for receiving and transmitting wireless communication signals.

The transponder 368 may use a portion of the power of the inductive signal received from the distal inductive element 326 to passively power the transponder 368. Once sufficiently powered by the inductive signals, the transponder 368 may receive and transmit data to the control unit 300 in the handle 6 via (i) the inductive coupling between the transponder 368 and the distal inductive element 324, (ii) the wire 322, and (iii) the inductive coupling between the secondary inductive element 320 and the control unit 300. That way, the control unit 300 may communicate with the transponder 368 in the end effector 12 without a direct wired connection through complex mechanical joints like the rotating joint 29 and/or without a direct wired connection from the shaft 8 to the end effector 12, places where it may be difficult to maintain such a wired connection. In addition, because the distances between the inductive elements (e.g., the spacing between (i) the transponder 368 and the distal inductive element 324, and (ii) the secondary inductive element 320 and the control unit 300) and fixed and known, the couplings could be optimized

12

for inductive transfer of energy. Also, the distances could be relatively short so that relatively low power signals could be used to thereby minimize interference with other systems in the use environment of the instrument 10.

In the embodiment of FIG. 12, the inductive element 302 of the control unit 300 is located relatively near to the control unit 300. According to other embodiments, as shown in FIG. 13, the inductive element 302 of the control unit 300 may be positioned closer to the rotating joint 29 so that it is closer to the secondary inductive element 320, thereby reducing the distance of the inductive coupling in such an embodiment. Alternatively, the control unit 300 (and hence the inductive element 302) could be positioned closer to the secondary inductive element 320 to reduce the spacing.

In other embodiments, more or fewer than two inductive couplings may be used. For example, in some embodiments, the surgical instrument 10 may use a single inductive coupling between the control unit 300 in the handle 6 and the transponder 368 in the end effector 12, thereby eliminating the inductive elements 320, 324 and the wire 322. Of course, in such an embodiment, a stronger signal may be required due to the greater distance between the control unit 300 in the handle 6 and the transponder 368 in the end effector 12. Also, more than two inductive couplings could be used. For example, if the surgical instrument 10 had numerous complex mechanical joints where it would be difficult to maintain a direct wired connection, inductive couplings could be used to span each such joint. For example, inductive couplers could be used on both sides of the rotary joint 29 and both sides of the articulation pivot 14, with the inductive element 321 on the distal side of the rotary joint 29 connected by a wire 322 to the inductive element 324 of the proximate side of the articulation pivot, and a wire 323 connecting the inductive elements 325, 326 on the distal side of the articulation pivot 14 as shown in FIG. 14. In this embodiment, the inductive element 326 may communicate with the sensor transponder 368.

In addition, the transponder 368 may include a number of different sensors. For example, it may include an array of sensors. Further, the end effector 12 could include a number of sensor transponders 368 in communication with the distal inductive element 324 (and hence the control unit 300). Also, the inductive elements 320, 324 may or may not include ferrite cores. As mentioned before, they are also preferably insulated from the electrically conductive outer shaft (or frame) of the instrument 10 (e.g., the closure tubes 40, 42), and the wire 322 is also preferably insulated from the outer shaft 8.

FIG. 15 is a diagram of an end effector 12 including a transponder 368 held or embedded in the cartridge 34 at the distal end of the channel 22. The transponder 368 may be connected to the cartridge 34 by a suitable bonding material, such as epoxy. In this embodiment, the transponder 368 includes a magnetoresistive sensor. The anvil 24 also includes a permanent magnet 369 at its distal end and generally facing the transponder 368. The end effector 12 also includes a permanent magnet 370 connected to the sled 33 in this example embodiment. This allows the transponder 368 to detect both opening/closing of the end effector 12 (due to the permanent magnet 369 moving further or closer to the transponder as the anvil 24 opens and closes) and completion of the stapling/cutting operation (due to the permanent magnet 370 moving toward the transponder 368 as the sled 33 traverses the channel 22 as part of the cutting operation).

FIG. 15 also shows the staples 380 and the staple drivers 382 of the staple cartridge 34. As explained previously, according to various embodiments, when the sled 33 traverses

the channel 22, the sled 33 drives the staple drivers 382 which drive the staples 380 into the severed tissue held in the end effector 12, the staples 380 being formed against the anvil 24. As noted above, such a surgical cutting and fastening instrument is but one type of surgical instrument in which the present invention may be advantageously employed. Various embodiments of the present invention may be used in any type of surgical instrument having one or more sensor transponders.

In the embodiments described above, the battery 64 powers (at least partially) the firing operation of the instrument 10. As such, the instrument may be a so-called "power-assist" device. More details and additional embodiments of power-assist devices are described in the '573 application, which is incorporated herein. It should be recognized, however, that the instrument 10 need not be a power-assist device and that this is merely an example of a type of device that may utilize aspects of the present invention. For example, the instrument 10 may include a user display (such as a LCD or LED display) that is powered by the battery 64 and controlled by the control unit 300. Data from the sensor transponders 368 in the end effector 12 may be displayed on such a display.

In another embodiment, the shaft 8 of the instrument 10, including for example, the proximate closure tube 40 and the distal closure tube 42, may collectively serve as part of an antenna for the control unit 300 by radiating signals to the sensor transponder 368 and receiving radiated signals from the sensor transponder 368. That way, signals to and from the remote sensor in the end effector 12 may be transmitted via the shaft 8 of the instrument 10.

The proximate closure tube 40 may be grounded at its proximate end by the exterior lower and upper side pieces 59-62, which may be made of a nonelectrically conductive material, such as plastic. The drive shaft assembly components (including the main drive shaft 48 and secondary drive shaft 50) inside the proximate and distal closure tubes 40, 42 may also be made of a nonelectrically conductive material, such as plastic. Further, components of end effector 12 (such as the anvil 24 and the channel 22) may be electrically coupled to (or in direct or indirect electrical contact with) the distal closure tube 42 such that they may also serve as part of the antenna. Further, the sensor transponder 368 could be positioned such that it is electrically insulated from the components of the shaft 8 and end effector 12 serving as the antenna. For example, the sensor transponder 368 may be positioned in the cartridge 34, which may be made of a nonelectrically conductive material, such as plastic. Because the distal end of the shaft 8 (such as the distal end of the distal closure tube 42) and the portions of the end effector 12 serving as the antenna may be relatively close in distance to the sensor 368, the power for the transmitted signals may be held at low levels, thereby minimizing or reducing interference with other systems in the use environment of the instrument 10.

In such an embodiment, as shown in FIG. 16, the control unit 300 may be electrically coupled to the shaft 8 of the instrument 10, such as to the proximate closure tube 40, by a conductive link 400 (e.g., a wire). Portions of the outer shaft 8, such as the closure tubes 40, 42, may therefore act as part of an antenna for the control unit 300 by radiating signals to the sensor 368 and receiving radiated signals from the sensor 368. Input signals received by the control unit 300 may be demodulated by the demodulator 310 and decoded by the decoder 312 (see FIG. 12). The input signals may comprise data from the sensors 368 in the end effector 12, which the processor 306 may use to control various aspects of the instrument 10, such as the motor 65 or a user display.

To transmit data signals to or from the sensors 368 in the end effector 12, the link 400 may connect the control unit 300 to components of the shaft 8 of the instrument 10, such as the proximate closure tube 40, which may be electrically connected to the distal closure tube 42. The distal closure tube 42 is preferably electrically insulated from the remote sensor 368, which may be positioned in the plastic cartridge 34 (see FIG. 3). As mentioned before, components of the end effector 12, such as the channel 22 and the anvil 24 (see FIG. 3), may be conductive and in electrical contact with the distal closure tube 42 such that they, too, may serve as part of the antenna.

With the shaft 8 acting as the antenna for the control unit 300, the control unit 300 can communicate with the sensor 368 in the end effector 12 without a direct wired connection. In addition, because the distances between shaft 8 and the remote sensor 368 is fixed and known, the power levels could be optimized for low levels to thereby minimize interference with other systems in the use environment of the instrument 10. The sensor 368 may include communication circuitry for radiating signals to the control unit 300 and for receiving signals from the control unit 300, as described above. The communication circuitry may be integrated with the sensor 368.

In another embodiment, the components of the shaft 8 and/or the end effector 12 may serve as an antenna for the remote sensor 368. In such an embodiment, the remote sensor 368 is electrically connected to the shaft (such as to distal closure tube 42, which may be electrically connected to the proximate closure tube 40) and the control unit 300 is insulated from the shaft 8. For example, the sensor 368 could be connected to a conductive component of the end effector 12 (such as the channel 22), which in turn may be connected to conductive components of the shaft (e.g., the closure tubes 40, 42). Alternatively, the end effector 12 may include a wire (not shown) that connects the remote sensor 368 the distal closure tube 42.

Typically, surgical instruments, such as the instrument 10, are cleaned and sterilized prior to use. In one sterilization technique, the instrument 10 is placed in a closed and sealed container 280, such as a plastic or TYVEK container or bag, as shown in FIGS. 17 and 18. The container and the instrument are then placed in a field of radiation that can penetrate the container, such as gamma radiation, x-rays, or high-energy electrons. The radiation kills bacteria on the instrument 10 and in the container 280. The sterilized instrument 10 can then be stored in the sterile container 280. The sealed, sterile container 280 keeps the instrument 10 sterile until it is opened in a medical facility or some other use environment. Instead of radiation, other means of sterilizing the instrument 10 may be used, such as ethylene oxide or steam.

When radiation, such as gamma radiation, is used to sterilize the instrument 10, components of the control unit 300, particularly the memory 308 and the processor 306, may be damaged and become unstable. Thus, according to various embodiments of the present invention, the control unit 300 may be programmed after packaging and sterilization of the instrument 10.

As shown in FIG. 17, a remote programming device 320, which may be a handheld device, may be brought into wireless communication with the control unit 300. The remote programming device 320 may emit wireless signals that are received by the control unit 300 to program the control unit 300 and to power the control unit 300 during the programming operation. That way, the battery 64 does not need to power the control unit 300 during the programming operation. According to various embodiments, the programming code downloaded to the control unit 300 could be of relatively

small size, such as 1 MB or less, so that a communications protocol with a relatively low data transmission rate could be used if desired. Also, the remote programming unit 320 could be brought into close physical proximity with the surgical instrument 10 so that a low power signal could be used.

Referring back to FIG. 19, the control unit 300 may comprise an inductive coil 402 to pick up wireless signals from a remote programming device 320. A portion of the received signal may be used by a power circuit 404 to power the control unit 300 when it is not being powered by the battery 64.

Input signals received by the coil 402 acting as a receiving antenna may be demodulated by a demodulator 410 and decoded by a decoder 412. The input signals may comprise programming instructions (e.g., code), which may be stored in a non-volatile memory portion of the memory 308. The processor 306 may execute the code when the instrument 10 is in operation. For example, the code may cause the processor 306 to output control signals to various sub-systems of the instrument 10, such as the motor 65, based on data received from the sensors 368.

The control unit 300 may also comprise a non-volatile memory unit 414 that comprises boot sequence code for execution by the processor 306. When the control unit 300 receives enough power from the signals from the remote control unit 320 during the post-sterilization programming operation, the processor 306 may first execute the boot sequence code ("boot loader") 414, which may load the processor 306 with an operating system.

The control unit 300 may also send signals back to the remote programming unit 320, such as acknowledgement and handshake signals, for example. The control unit 300 may comprise an encoder 416 for encoding the signals to then be sent to the programming device 320 and a modulator 418 for modulating the signals according to the modulation scheme. The coil 402 may act as the transmitting antenna. The control unit 300 and the remote programming device 320 may communicate using any suitable wireless communication protocol (e.g., Bluetooth) and any suitable frequency (e.g., an ISM band). Also, the control unit 300 may transmit signals at a different frequency range than the frequency range of the received signals from the remote programming unit 320.

FIG. 20 is a simplified diagram of the remote programming device 320 according to various embodiments of the present invention. As shown in FIG. 20, the remote programming unit 320 may comprise a main control board 230 and a boosted antenna board 232. The main control board 230 may comprise a controller 234, a power module 236, and a memory 238. The memory 238 may store the operating instructions for the controller 234 as well as the programming instructions to be transmitted to the control unit 300 of the surgical instrument 10. The power module 236 may provide a stable DC voltage for the components of the remote programming device 320 from an internal battery (not shown) or an external AC or DC power source (not shown).

The boosted antenna board 232 may comprise a coupler circuit 240 that is in communication with the controller 234 via an I²C bus, for example. The coupler circuit 240 may communicate with the control unit 300 of the surgical instrument via an antenna 244. The coupler circuit 240 may handle the modulating/demodulating and encoding/decoding operations for transmissions with the control unit. According to other embodiments, the remote programming device 320 could have a discrete modulator, demodulator, encoder and decoder. As shown in FIG. 20, the boost antenna board 232 may also comprise a transmitting power amp 246, a matching circuit 248 for the antenna 244, and a filter/amplifier 249 for receiving signals.

According to other embodiments, as shown in FIG. 20, the remote programming device could be in communication with a computer device 460, such as a PC or a laptop, via a USB and/or RS232 interface, for example. In such a configuration, a memory of the computing device 460 may store the programming instructions to be transmitted to the control unit 300. In another embodiment, the computing device 460 could be configured with a wireless transmission system to transmit the programming instructions to the control unit 300.

In addition, according to other embodiments, rather than using inductive coupling between the control unit 300 and the remote programming device 320, capacitively coupling could be used. In such an embodiment, the control unit 300 could have a plate instead of a coil, as could the remote programming unit 320.

In another embodiment, rather than using a wireless communication link between the control unit 300 and the remote programming device 320, the programming device 320 may be physically connected to the control unit 300 while the instrument 10 is in its sterile container 280 in such a way that the instrument 10 remains sterilized. FIG. 21 is a diagram of a packaged instrument 10 according to such an embodiment. As shown in FIG. 22, the handle 6 of the instrument 10 may include an external connection interface 470. The container 280 may further comprise a connection interface 472 that mates with the external connection interface 470 of the instrument 10 when the instrument 10 is packaged in the container 280. The programming device 320 may include an external connection interface (not shown) that may connect to the connection interface 472 at the exterior of the container 280 to thereby provide a wired connection between the programming device 320 and the external connection interface 470 of the instrument 10.

The various embodiments of the present invention have been described above in connection with cutting-type surgical instruments. It should be noted, however, that in other embodiments, the inventive surgical instrument disclosed herein need not be a cutting-type surgical instrument, but rather could be used in any type of surgical instrument including remote sensor transponders. For example, it could be a non-cutting endoscopic instrument, a grasper, a stapler, a clip applier, an access device, a drug/gene therapy delivery device, an energy device using ultrasound, RF, laser, etc. In addition, the present invention may be in laparoscopic instruments, for example. The present invention also has application in conventional endoscopic and open surgical instrumentation as well as robotic-assisted surgery.

The devices disclosed herein can be designed to be disposed of after a single use, or they can be designed to be used multiple times. In either case, however, the device can be reconditioned for reuse after at least one use. Reconditioning can include any combination of the steps of disassembly of the device, followed by cleaning or replacement of particular pieces, and subsequent reassembly. In particular, the device can be disassembled, and any number of the particular pieces or parts of the device can be selectively replaced or removed in any combination. Upon cleaning and/or replacement of particular parts, the device can be reassembled for subsequent use either at a reconditioning facility, or by a surgical team immediately prior to a surgical procedure. Those skilled in the art will appreciate that reconditioning of a device can utilize a variety of techniques for disassembly, cleaning/replacement, and reassembly. Use of such techniques, and the resulting reconditioned device, are all within the scope of the present application.

Although the present invention has been described herein in connection with certain disclosed embodiments, many

modifications and variations to those embodiments may be implemented. For example, different types of end effectors may be employed. Also, where materials are disclosed for certain components, other materials may be used. The foregoing description and following claims are intended to cover all such modification and variations.

Any patent, publication, or other disclosure material, in whole or in part, that is said to be incorporated by reference herein is incorporated herein only to the extent that the incorporated materials does not conflict with existing definitions, statements, or other disclosure material set forth in this disclosure. As such, and to the extent necessary, the disclosure as explicitly set forth herein supersedes any conflicting material incorporated herein by reference. Any material, or portion thereof, that is said to be incorporated by reference herein, but which conflicts with existing definitions, statements, or other disclosure material set forth herein will only be incorporated to the extent that no conflict arises between that incorporated material and the existing disclosure material.

What is claimed is:

1. A surgical instrument comprising:
an end effector comprising at least one sensor transponder;
a shaft having a distal end connected to the end effector;
and
a handle connected to a proximate end of the shaft, the handle comprising a control unit, wherein the control unit is in communication with the at least one sensor transponder via at least one inductive coupling.
2. The surgical instrument of claim 1, wherein the handle further comprises:
a motor in communication with the control unit, wherein the motor is for powering a main drive shaft assembly in the shaft, wherein the main drive shaft assembly drives the end effector; and
a battery for powering the motor.
3. The surgical instrument of claim 2, wherein the handle further comprises:
a closure trigger for causing, when retracted by an operator, the end effector to clamp an object positioned in the end effector; and
a firing trigger, separate from the closure trigger, for causing, when retracted by the operator, actuation of the motor.
4. The surgical instrument of claim 1, wherein the control unit comprises:
a processor;
a memory in communication with the processor; and
an inductive element in communication with the processor for receiving and transmitting signals.
5. The surgical instrument of claim 1, wherein the surgical instrument comprises at least one rotational joint for rotating the shaft, and wherein the surgical instrument further comprises:
a first inductive element located in the shaft distally from the rotational joint and inductively coupled to the control unit; and
a second inductive element located in the shaft and inductively coupled to the at least one sensor transponder.
6. The surgical instrument of claim 5, wherein the second inductive element is located adjacent to the end effector, and

wherein the second inductive element is connected to the first inductive element via a flexible electrically conductive wire located inside the shaft.

7. The surgical instrument of claim 6, wherein the shaft comprises an articulation pivot between the first and second inductive elements.

8. The surgical instrument of claim 1, wherein the at least one sensor transponder comprises a magnetoresistive sensor.

9. The surgical instrument of claim 1, wherein the at least one sensor transponder comprises a RFID sensor.

10. The surgical instrument of claim 1, wherein the at least one sensor transponder comprises an electromechanical sensor.

11. The surgical instrument of claim 1, wherein the surgical instrument comprises an endoscopic surgical instrument.

12. The surgical instrument of claim 1, wherein the end effector comprises a moveable cutting instrument.

13. The surgical instrument of claim 12, wherein the end effector comprises a staple cartridge.

14. A surgical instrument comprising:
an end effector comprising at least one sensor transponder;
a shaft having a distal end connected to the end effector;
and
a control unit, wherein the control unit is in communication with the at least one sensor transponder via at least one inductive coupling.

15. The surgical instrument of claim 14, wherein the control unit comprises:
a processor;
a memory in communication with the processor; and
an inductive element in communication with the processor for receiving and transmitting signals.

16. The surgical instrument of claim 14, wherein the surgical instrument comprises at least one rotational joint for rotating the shaft, and wherein the surgical instrument further comprises:

a first inductive element located in the shaft distally from the rotational joint and inductively coupled to the control unit; and
a second inductive element located in the shaft and inductively coupled to the at least one sensor transponder.

17. The surgical instrument of claim 16, wherein the second inductive element is located adjacent to the end effector, and wherein the second inductive element is connected to the first inductive element via a flexible electrically conductive wire located inside the shaft.

18. The surgical instrument of claim 17, wherein the shaft comprises an articulation pivot between the first and second inductive elements.

19. The surgical instrument of claim 16, further comprising:

a motor for actuating the end effector; and
a battery connected to the motor for powering the motor.

20. The surgical instrument of claim 19, further comprising:

a closure trigger for causing, when retracted by an operator, the end effector to clamp an object positioned in the end effector; and
a firing trigger, separate from the closure trigger, for causing, when retracted by the operator, actuation of the motor.

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : 8,652,120 B2
APPLICATION NO. : 11/651715
DATED : February 18, 2014
INVENTOR(S) : Giordano et al.

Page 1 of 1


It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the Title Page:

The first or sole Notice should read --

Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b)
by 2112 days.

Signed and Sealed this
Second Day of June, 2015

A handwritten signature in black ink, reading "Michelle K. Lee". The signature is written in a cursive, flowing style.

Michelle K. Lee
Director of the United States Patent and Trademark Office

专利名称(译)	在控制单元和传感器发送应答器之间进行无线通信的手术器械		
公开(公告)号	US8652120	公开(公告)日	2014-02-18
申请号	US11/651715	申请日	2007-01-10
[标]申请(专利权)人(译)	GIORDANO JAMES - [R] 谢尔顿检基ê 斯韦兹JEFFREY小号		
申请(专利权)人(译)	GIORDANO JAMES - [R] 谢尔顿检基ê 斯韦兹JEFFREY小号		
当前申请(专利权)人(译)	爱惜康内镜手术，INC.		
[标]发明人	GIORDANO JAMES R SHELTON IV FREDERICK E SWAYZE JEFFREY S		
发明人	GIORDANO, JAMES R. SHELTON, IV, FREDERICK E. SWAYZE, JEFFREY S.		
IPC分类号	A61B18/00		
CPC分类号	A61B19/026 A61B2017/00221 A61B2017/00362 A61B2017/00212 A61B2019/448 A61B2017/00398 A61B2017/320052 A61B17/00 A61B2017/00734 A61B2019/0286 A61B2017/00022 A61B2017/07214 A61B17/07207 A61B2019/4857 A61B2017/00039 A61B2019/465 A61B2019/0267 A61B17/00234 A61B2017/2927 A61B2017/0688 A61B17/068 A61B2560/0266 A61B50/30 A61B90/98 A61B2050/3015 A61B2050/314 A61B2090/065 A61B2090/0811		
其他公开文献	US20080167522A1		
外部链接	Espacenet USPTO		

摘要(译)

一种外科手术器械，例如内窥镜或腹腔镜器械，根据各种实施例，包括末端执行器，该末端执行器包括至少一个传感器应答器。手术器械还包括轴，该轴具有连接到末端执行器的远端和连接到轴的近端的手柄。手柄包括控制单元，该控制单元通过至少一个电感耦合与传感器应答器通信。手术器械可以是动力辅助机动装置，其包括用于在使用期间（至少部分地）为手术器械供电的电池。手术器械可以适于提供关于末端执行器所经历的负载的用户反馈。

