



US008192455B2

(12) **United States Patent**
Brazzini et al.

(10) **Patent No.:** **US 8,192,455 B2**
(45) **Date of Patent:** **Jun. 5, 2012**

(54) **COMPRESSIVE DEVICE FOR PERCUTANEOUS TREATMENT OF OBESITY**

(75) Inventors: **Augusto Brazzini**, New Orleans, LA (US); **David S. Kirsch**, Jefferson, LA (US); **Wilfrido R. Castaneda-Zuniga**, New Orleans, LA (US); **Horacio D'Agostino**, Shreveport, LA (US)

(73) Assignee: **Board of Supervisors of Louisiana State University and Agricultural and Mechanical College**, Baton Rouge, LA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 1629 days.

(21) Appl. No.: **10/567,199**

(22) PCT Filed: **Jul. 30, 2004**

(86) PCT No.: **PCT/US2004/024612**

§ 371 (c)(1),
(2), (4) Date: **Aug. 14, 2006**

(87) PCT Pub. No.: **WO2005/018417**

PCT Pub. Date: **Mar. 3, 2005**

(65) **Prior Publication Data**

US 2007/0060940 A1 Mar. 15, 2007

Related U.S. Application Data

(60) Provisional application No. 60/494,698, filed on Aug. 13, 2003.

(51) **Int. Cl.**
A61M 29/00 (2006.01)

(52) **U.S. Cl.** **606/192; 606/191; 600/37; 128/898**

(58) **Field of Classification Search** 600/37;
606/191, 192, 195; 128/898
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

233,475 A 10/1880 Cook et al.

(Continued)

FOREIGN PATENT DOCUMENTS

EP 1 016 377 A2 7/2000

(Continued)

OTHER PUBLICATIONS

Brolin, R.E., "Gastric Bypass," *Surg. Clinics of North America*, vol. 81(5), pp. 1077-1096 (2001).

(Continued)

Primary Examiner — Gary Jackson


Assistant Examiner — Michael Mendoza

(74) *Attorney, Agent, or Firm* — Alan W. Cannon

(57) **ABSTRACT**

An apparatus and method for treating morbid obesity in mammals using a gastric reduction assembly that reduces the gastric volume of a stomach and induces early satiety. The gastric reduction assembly comprises at least two or more expandable devices, each able to be adjustably inflated with a fluid (e.g., a liquid or a gas) using a filling tube. In a preferred embodiment, the gastric reduction assembly is inserted through the abdominal wall and placed at a location exterior to the stomach body, avoiding an abdominal incision. Once positioned near the stomach body, the gastric reduction assembly allows for the external compression of the stomach body to limit food intake. The gastric reduction assembly also minimizes the potential for shifting of the expandable devices after insertion to the stomach body to revert to its pre-compressed state.

8 Claims, 3 Drawing Sheets

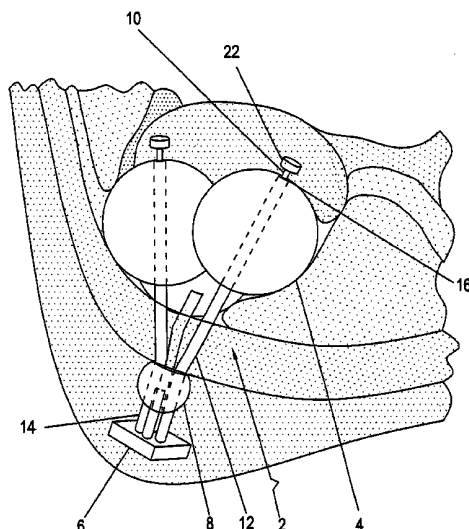

U.S. PATENT DOCUMENTS				
659,422 A	10/1900	Shidler	5,480,406 A	1/1996 Nolan et al.
780,392 A	1/1905	Wanamaker et al.	5,496,311 A	3/1996 Abele et al.
789,467 A	5/1905	West	5,507,754 A	4/1996 Green et al.
1,461,524 A	7/1923	Goddard	5,545,171 A	8/1996 Sharkey et al.
2,579,192 A	12/1951	Kohl et al.	5,545,178 A	8/1996 Kensey et al.
2,646,298 A	7/1953	Leary	5,549,621 A	8/1996 Bessler et al.
2,697,624 A	12/1954	Thomas et al.	5,554,162 A	9/1996 DeLange
2,734,299 A	2/1956	Masson	5,573,540 A	11/1996 Yoon
2,825,592 A	3/1958	Semple	5,591,177 A	1/1997 Lehrer
3,326,586 A	6/1967	Frost et al.	5,601,604 A	2/1997 Vincent
3,470,834 A	10/1969	Bone	5,626,614 A	5/1997 Hart
3,521,918 A	7/1970	Hammond	5,634,936 A	6/1997 Linden et al.
3,571,864 A	3/1971	Emile et al.	5,647,836 A	7/1997 Blake, III et al.
3,664,435 A	5/1972	Klessig	5,690,691 A	11/1997 Chen et al.
3,675,639 A	7/1972	Climber	5,716,368 A	2/1998 Torre et al.
3,713,680 A	1/1973	Pagano	5,725,557 A	3/1998 Gattuna et al.
3,756,638 A	9/1973	Stockberger	5,846,254 A	12/1998 Schulze et al.
3,873,140 A	3/1975	Bloch	5,888,196 A	3/1999 Bonutti
3,931,667 A	1/1976	Merser et al.	5,931,788 A	8/1999 Keen et al.
3,976,079 A	8/1976	Samuels et al.	5,938,669 A	8/1999 Klaiber et al.
4,006,747 A	2/1977	Kronenthal et al.	5,951,590 A	9/1999 Goldfarb
4,060,089 A	11/1977	Noiles	5,961,440 A	10/1999 Schweich, Jr. et al.
4,133,315 A	1/1979	Berman et al.	5,971,447 A	10/1999 Steck, III
4,210,148 A	7/1980	Stivala	5,993,473 A	11/1999 Chan et al. 606/192
4,246,893 A	1/1981	Berson 128/1 R	6,013,053 A	1/2000 Bower et al.
4,291,698 A	9/1981	Fuchs et al.	6,067,991 A	5/2000 Forsell
4,328,805 A	5/1982	Akopov et al.	6,080,160 A	6/2000 Chen et al.
4,416,267 A	11/1983	Garren et al.	6,097,984 A	8/2000 Douglas
4,458,681 A	7/1984	Hophins	6,102,922 A	8/2000 Jakobsson et al. 606/157
4,472,226 A	9/1984	Redinger et al.	6,113,609 A	9/2000 Adams
4,485,805 A	12/1984	Foster, Jr. et al.	6,143,006 A	11/2000 Chan
4,493,323 A	1/1985	Albright et al.	6,162,234 A	12/2000 Freedland et al.
4,558,699 A	12/1985	Bashour	6,186,149 B1	2/2001 Pacella et al.
4,592,339 A	6/1986	Kuzmak et al.	6,270,530 B1	8/2001 Eldridge et al.
4,592,342 A	6/1986	Salmasian	6,420,452 B1	7/2002 Gunatillake et al.
4,621,640 A	11/1986	Mulhollan et al.	6,437,073 B1	8/2002 Gunatillake et al.
4,669,473 A	6/1987	Richards et al.	6,447,533 B1	9/2002 Adams
4,694,827 A	9/1987	Weiner et al. 128/303 R	6,454,785 B2	9/2002 De Hoyos Garza
4,696,288 A	9/1987	Kuzmak et al.	6,475,136 B1	11/2002 Forsell 600/37
4,705,040 A	11/1987	Mueller et al.	6,488,691 B1	12/2002 Carroll et al.
4,714,281 A	12/1987	Peck	6,491,707 B2	12/2002 Makower et al.
4,723,547 A	2/1988	Kullas et al.	6,494,888 B1	12/2002 Laufer et al.
4,738,255 A	4/1988	Goble et al.	6,500,148 B1	12/2002 Pinchuk et al.
4,739,758 A	4/1988	Lai et al.	6,506,196 B1	1/2003 Laufer
4,744,364 A	5/1988	Kensey	6,511,490 B2	1/2003 Robert 606/151
4,750,492 A	6/1988	Jacobs	6,535,764 B2	3/2003 Imran et al.
4,803,985 A	2/1989	Hill	6,558,400 B2	5/2003 Deem et al.
4,823,794 A	4/1989	Pierce	6,656,182 B1	12/2003 Hayhurst
4,899,747 A	2/1990	Garren et al.	6,663,639 B1	12/2003 Laufer et al.
4,955,913 A	9/1990	Robinson	6,669,713 B2	12/2003 Adams
5,002,550 A	3/1991	Li	6,675,809 B2	1/2004 Stack et al.
5,033,481 A	7/1991	Heyler, III	6,736,793 B2	5/2004 Meyer et al.
5,041,129 A	8/1991	Hayhurst et al.	6,746,460 B2	6/2004 Gannoe et al.
5,084,061 A	1/1992	Gau et al.	6,755,869 B2	6/2004 Geitz
5,100,421 A	3/1992	Christoudias	6,773,441 B1	8/2004 Laufer et al.
5,112,310 A *	5/1992	Grobe 604/175	6,790,213 B2	9/2004 Cherok et al.
5,123,914 A	6/1992	Cope	6,821,285 B2	11/2004 Laufer et al.
5,129,912 A	7/1992	Noda et al.	6,835,200 B2	12/2004 Laufer et al.
RE34,021 E	8/1992	Mueller et al.	6,869,395 B2	3/2005 Page et al.
5,151,086 A *	9/1992	Duh et al. 604/506	6,900,055 B1	5/2005 Fuller
5,188,104 A	2/1993	Wernicke et al.	6,908,487 B2	6/2005 Cigaina
5,217,470 A	6/1993	Weston	6,981,978 B2	1/2006 Gannoe
5,234,454 A	8/1993	Bangs 606/191	6,994,715 B2	2/2006 Gannoe et al.
5,246,456 A	9/1993	Wilkinson	7,033,373 B2	4/2006 de la Torre et al.
5,258,015 A	11/1993	Li et al.	7,037,344 B2	5/2006 Kagan et al.
5,259,399 A	11/1993	Brown	7,153,314 B2	12/2006 Laufer et al.
5,269,809 A	12/1993	Hayhurst et al.	7,167,750 B2	1/2007 Knudson et al.
5,292,344 A	3/1994	Douglas	7,223,277 B2	5/2007 DeLegge
5,334,200 A	8/1994	Johnson	7,255,675 B2	8/2007 Gertner et al.
5,354,271 A	10/1994	Voda	7,338,433 B2	3/2008 Coe
5,364,408 A	11/1994	Gordon	7,354,454 B2	4/2008 Stack et al.
5,391,182 A	2/1995	Chin	7,374,565 B2	5/2008 Hassler et al.
5,405,352 A	4/1995	Weston	7,402,166 B2	7/2008 Feigl
5,423,872 A	6/1995	Cigaina	7,416,554 B2	8/2008 Lam et al.
5,428,123 A	6/1995	Ward et al.	7,618,426 B2	11/2009 Ewers et al.
5,445,608 A	8/1995	Chen et al.	7,666,195 B2	2/2010 Kelleher et al.
5,470,337 A	11/1995	Moss	7,670,279 B2	3/2010 Gertner
5,472,446 A	12/1995	Torre	7,841,978 B2	11/2010 Gertner
			7,862,546 B2	1/2011 Conlon et al.

7,988,617 B2	8/2011	Gertner	2007/0250103 A1	10/2007	Makower
2001/0010005 A1	7/2001	Kammerer et al.	2007/0255308 A1	11/2007	Williams et al.
2001/0011543 A1	8/2001	Forsell	2007/0270892 A1	11/2007	Makower
2001/0044639 A1	11/2001	Levinson	2007/0276293 A1	11/2007	Gertner
2002/0055757 A1	5/2002	Torre et al.	2007/0276432 A1	11/2007	Stock
2002/0128684 A1	9/2002	Foerster	2008/0015501 A1	1/2008	Gertner
2002/0161382 A1	10/2002	Neisz et al.	2008/0051823 A1	2/2008	Makower et al.
2002/0161414 A1	10/2002	Flesler et al.	2008/0051824 A1	2/2008	Gertner
2002/0188354 A1	12/2002	Peghini 623/23.65	2008/0051850 A1	2/2008	Sparks et al.
2003/0021822 A1	1/2003	Lloyd	2008/0058710 A1	3/2008	Wilk
2003/0055463 A1	3/2003	Gordon et al.	2008/0071306 A1	3/2008	Gertner et al.
2003/0055465 A1	3/2003	Ben-Haim et al.	2008/0086082 A1	4/2008	Brooks
2003/0093117 A1	5/2003	Saadat	2008/0091237 A1	4/2008	Schwartz et al.
2003/0208212 A1	11/2003	Cigaina	2008/0109027 A1	5/2008	Chen et al.
2004/0006351 A1	1/2004	Gannoe et al.	2008/0147002 A1	6/2008	Gertner
2004/0024386 A1	2/2004	Deem et al.	2008/0161717 A1	7/2008	Gertner
2004/0030347 A1	2/2004	Gannoe	2008/0167519 A1	7/2008	St-Germain
2004/0044353 A1	3/2004	Gannoe	2008/0167647 A1	7/2008	Gertner
2004/0044357 A1	3/2004	Gannoe	2008/0167648 A1	7/2008	Gertner
2004/0054352 A1	3/2004	Adams et al.	2008/0172074 A1	7/2008	Baker et al.
2004/0059289 A1	3/2004	Garza Alvarez	2008/0172079 A1	7/2008	Birk
2004/0068224 A1	4/2004	Couvillon et al.	2008/0208240 A1	8/2008	Paz
2004/0092892 A1	5/2004	Kagan et al.			
2004/0097986 A1	5/2004	Adams			
2004/0098060 A1	5/2004	Ternes			
2004/0116949 A1	6/2004	Ewers et al.	EP 1 520 563	4/2005	
2004/0122456 A1	6/2004	Saadat et al.	EP 1 602 392 A1	7/2005	
2004/0122473 A1	6/2004	Ewers et al.	EP 1 591 140 A1	11/2005	
2004/0148034 A1	7/2004	Kagan et al.	EP 1 547 642 B1	8/2007	
2004/0186503 A1	9/2004	Delegge	EP 1 607 071 B1	8/2007	
2004/0193194 A1	9/2004	Laufer et al.	EP 1 670 361 B1	4/2008	
2004/0194790 A1	10/2004	Laufer et al.	FR 2 907 665	2/2008	
2004/0243178 A1	12/2004	Haut et al.	WO WO 87/00034	1/1987	
2004/0243179 A1	12/2004	Foerster	WO WO 9925418	5/1999	
2004/0243180 A1	12/2004	Donnelly et al.	WO WO 9925418	5/1999	
2004/0260345 A1	12/2004	Foerster	WO WO 0009049	2/2000	
2004/0267378 A1	12/2004	Gazi et al.	WO WO 0018330	4/2000	
2005/0022827 A1	2/2005	Woo et al.	WO WO 00/74573 A1	12/2000	
2005/0049718 A1	3/2005	Dann et al.	WO WO 0147435	7/2001	
2005/0159769 A1	7/2005	Alverdy	WO WO 02/35980	5/2002	
2005/0197687 A1	9/2005	Molaei et al.	WO WO 02071951	9/2002	
2005/0203344 A1	9/2005	Orban, III et al.	WO WO 03/055420	7/2003	
2005/0216040 A1	9/2005	Gertner et al.	WO WO 03095015	11/2003	
2005/0216042 A1	9/2005	Gertner et al.	WO WO 2004004542	1/2004	
2005/0228415 A1	10/2005	Gertner	WO WO 2004014237	2/2004	
2005/0261712 A1	11/2005	Balbierz	WO WO 2004019765	3/2004	
2005/0267405 A1	12/2005	Shah	WO WO 2004021894	3/2004	
2005/0267406 A1	12/2005	Hassler, Jr.	WO WO 2004037064	5/2004	
2005/0267533 A1	12/2005	Gertner	WO WO 2005007232	1/2005	
2005/0267595 A1	12/2005	Chen et al.	WO WO 2005009288	2/2005	
2005/0267596 A1	12/2005	Chen et al.	WO WO 2005/018417 A2	3/2005	
2005/0277960 A1	12/2005	Hassler, Jr. et al.	WO WO 2005/018417 A3	3/2005	
2005/0277974 A1	12/2005	Hassler, Jr. et al.	WO WO 2005/094447 A2	10/2005	
2006/0009789 A1	1/2006	Gambale et al.	WO WO 2006020370	2/2006	
2006/0025789 A1	2/2006	Laufer et al.	WO WO 2006/049725 A2	5/2006	
2006/0058829 A1	3/2006	Sampson	WO WO 2006063593 A2	6/2006	
2006/0089571 A1	4/2006	Gertner	WO WO 2006108203	10/2006	
2006/0106288 A1	5/2006	Roth et al.	WO WO 2007017880 A2	2/2007	
2006/0161186 A1	7/2006	Hassler, Jr. et al.	WO WO 2007/067206 A2	6/2007	
2006/0161256 A1	7/2006	Ziegler et al.	WO WO 2007110866	10/2007	
2006/0195139 A1	8/2006	Gertner	WO WO 2008006084	1/2008	
2006/0212053 A1	9/2006	Gertner	WO WO 2008013814	1/2008	
2006/0253131 A1	11/2006	Wolniewicz			
2006/0264699 A1	11/2006	Gertner			
2007/0027358 A1	2/2007	Gertner et al.			
2007/0060940 A1	3/2007	Brazzini et al.			
2007/0073318 A1	3/2007	Carter et al.			
2007/0073323 A1	3/2007	Carter et al.			
2007/0088373 A1	4/2007	Baker			
2007/0112363 A1	5/2007	Adams			
2007/0129738 A1	6/2007	Kraemer et al.			
2007/0167982 A1	7/2007	Gertner et al.			
2007/0173869 A1	7/2007	Gannoe et al.			
2007/0173888 A1	7/2007	Gertner et al.			
2007/0179335 A1	8/2007	Gertner et al.			
2007/0203517 A1	8/2007	Williams et al.			
2007/0233170 A1	10/2007	Gertner, et al.			
2007/0235083 A1	10/2007	Dlugos			
2007/0239284 A1	10/2007	Skerven et al.			

FOREIGN PATENT DOCUMENTS

EP	1 520 563	4/2005
EP	1 602 392 A1	7/2005
EP	1 591 140 A1	11/2005
EP	1 547 642 B1	8/2007
EP	1 607 071 B1	8/2007
EP	1 670 361 B1	4/2008
FR	2 907 665	2/2008
WO	WO 87/00034	1/1987
WO	WO 9925418	5/1999
WO	WO 9925418	5/1999
WO	WO 0009049	2/2000
WO	WO 0018330	4/2000
WO	WO 00/74573 A1	12/2000
WO	WO 0147435	7/2001
WO	WO 02/35980	5/2002
WO	WO 02071951	9/2002
WO	WO 03/055420	7/2003
WO	WO 03095015	11/2003
WO	WO 2004004542	1/2004
WO	WO 2004014237	2/2004
WO	WO 2004019765	3/2004
WO	WO 2004021894	3/2004
WO	WO 2004037064	5/2004
WO	WO 2005007232	1/2005
WO	WO 2005009288	2/2005
WO	WO 2005/018417 A2	3/2005
WO	WO 2005/018417 A3	3/2005
WO	WO 2005/094447 A2	10/2005
WO	WO 2006020370	2/2006
WO	WO 2006/049725 A2	5/2006
WO	WO 2006063593 A2	6/2006
WO	WO 2006108203	10/2006
WO	WO 2007017880 A2	2/2007
WO	WO 2007/067206 A2	6/2007
WO	WO 2007110866	10/2007
WO	WO 2008006084	1/2008
WO	WO 2008013814	1/2008

OTHER PUBLICATIONS

Deitel, M., "Overview of Obesity Surgery," *World J. Surg.*, vol. 22, pp. 913-918 (1998).

DeMaria, E.J., "Laparoscopic Adjustable Silicone Gastric Banding," *Surg. Clinics of North America*, vol. 81(5), pp. 1129-1144 (2001).

Doherty, C., "Vertical Banded Gastroplasty," *Surg. Clinics of North America*, vol. 81(5), pp. 1097-1112 (2001).

Marceau, P. et al., "Malabsorptive Obesity Surgery," *Surg. Clinics of North America*, vol. 81(5), pp. 1113-1128 (2001).

McMillan, et al., Arthroscopic Knot-tying techniques. pp. 81-95, 2003.

Buchwald—Overview of Bariatric Surgery. *Journal of the American College of Surgeons*. pp. 367-375, Mar. 2002.

Sharp, et al., The 4-S Modification of the Roeder Knot: How to Tie It. pp. 1004-1006, vol. 90, No. 6, Dec. 1997.

- Akira., JP63277063, Japanese and English Abstract, Nov. 15, 1988, pp. 1-4.
- Abhyankar et al, Use of a tissue expander and a polyglactic acid (Vicryl) mesh to reduce radiation enteritis: case report and literature view, 21: pp. 755-757, Aug. 2005.
- Buchwald, Overview of Bariatric Surgery, vol. 194, No. 3, Mar. 2002, pp. 367-375.
- Burnett, et al., The Use of a Pelvic Displacement Prosthesis to Exclude the Small Intestine from the Radiation Field Following Radical Hysterectomy, 79, pp. 438-443, 2000. <http://www.idealibrary.com>.
- Cheng, Splenic Epidermoid Cyst, pp. 1-3, 1997.
- Doherty, Cornelius., Technique of Vertical Banded Gastroplasty. vol. 81, No. 5, Oct. 2001, pp. 1097-1111.
- Foglia et al., Management of giant omphalocele with rapid creation of abdominal domain, 41, pp. 704-709, 2006.
- Fried et al., Physical Principles of Available Adjustable Gastric Bands: How they Work. Obesity Surgery, 14, 2004, pp. 1118-1122.
- Geliebter et al; Extra-abdominal pressure alters food intake, intragastric pressure, and gastric emptying rate. 1986, pp. R549-R552.
- Hoffman et al., Morbidity after Intraperitoneal Insertion of Saline-Filled Tissue Expanders for Small Bowel Exclusion from Radiotherapy Treatment Fields: A Prospective Four Year Experience with 34 Patients, pp. 473-483, No. 7, vol. 60, Jul. 1994.
- Hainaux et al., Laparoscopic adjustable silicone gastric banding: radiological appearances of a new surgical treatment for morbid obesity. 1999, *Abdom Imaging* 24: 533-537.
- Konturek et al., Neuro-Hormonal Control of Food Intake; Basic Mechanisms and Clinical Implications, 2005, 56, Supp 6, 5-25. www.jpp.krakow.pl.
- Lam et al., Huge Splenic Epidemoid Cyst: A Case Report, 1997; 60:113-6.
- Lee et al., Laparoscopic Vertical Sleeve Gastrectomy: A Novel Bariatric Procedure—superior to Established Operations? pp. 1-27. 90th Annual Clinical Congress, New Orleans, LA, Oct. 10, 2004.
- Malassagne, et al., Intra-abdominal Sengstaken-Blakemore tube Placement for acute venous outflow obstruction in reduced-size Liver, Nov. 1996, 83, pp. 1086.
- Mera, et al., Use of the Breast Implant for Liver Graft Malposition. vol. 5, No. 6, Nov. 1999, pp. 534-535.
- Obesity Surgery Including Laparoscopy and Allied Care. vol. 16, No. 1, Jan. 2006, pp. 1-2. www.obesitysurgery.com.
- Pomerri et al., Adjustable Silicone Gastric Banding of Obesity. , 1992, *Gastrointest Radiol* 17:207-210.
- Schauer, et al., New applications for endoscopy: the emerging field of endoluminal and transgastric bariatric surgery, DOI:10.1007/s00464-006-9008-8, 2006.
- The Sleeve Gastrectomy (or 2-Stage Procedure). 2006, pp. 1-2. <http://surgicallyslim.com/sleeve.htm>.
- Walker, et al. Bladder Augmentation in Dogs Using the Tissue Capsule Formed Around a Perivesical tissue Expander, vol. 168, pp. 1534-1536, 2002.
- Zwart et al., Gastric Motility: Comparison of Assessment with Real-Time MR Imaging or Barostat Experience I., 224: pp. 592-597, Aug. 2002.
- About the Vertical Sleeve Gastrectomy. Mar. 24, 2006, pp. 1-1. <http://obesityhelp.com/forums/VSG/about.html>.
- Gertner MD, Stomach Restriction with an Extragastric Balloon, pp. 1, Abstract for 2007.
- Laparoscopic Duodenal Switch, Mar. 24, 2006, <http://wo-pub2.med.cornell.edu/cgi-bin/WebObjects/PublicA.woa/5/w...> p. 1-1.
- Med-4840, Product Profile , Mar. 30, 2007, pp. 1-2.
- Tucker, Diana, Medical Device Daily. vol. 10, No. 102, pp. 1-10, May 26, 2006.
- Trumble et al., "Method for measuring long-term function of muscle-powered implants via radiotelemetry" *J. Appl. Physiol.* 2001,90: pp. 1977-1985.
- Buchwald et al., "Evolution of Operative Procedures for the Management of Morbid Obesity 1950-2000", *Obesity Surgery* 2002, 12:705-717.
- Cummings et al., "Genetics and Pathophysiology of Human Obesity", *An Annual Review of Medicine*, 2003, 54:453-471.
- Johnston et al., The MagenstJohnston et al., "The Magenstrasse and Mill Operation for Morbid Obesity", *Obesity Surgery* 2003, 13:10-16.
- Smith et al., "Modification of the Gastric Partitioning Operation for Morbid Obesity", *Am. J. Surgery* 142, Dec. 1981, pp. 725-730.
- Smith et al., "Results and Complications of Gastric Partitioning: Four Years Follow-Up of 300 Morbidly Obese Patients", *The American Journal of Surgery*, 1983, (146) pp. 815-819.

* cited by examiner

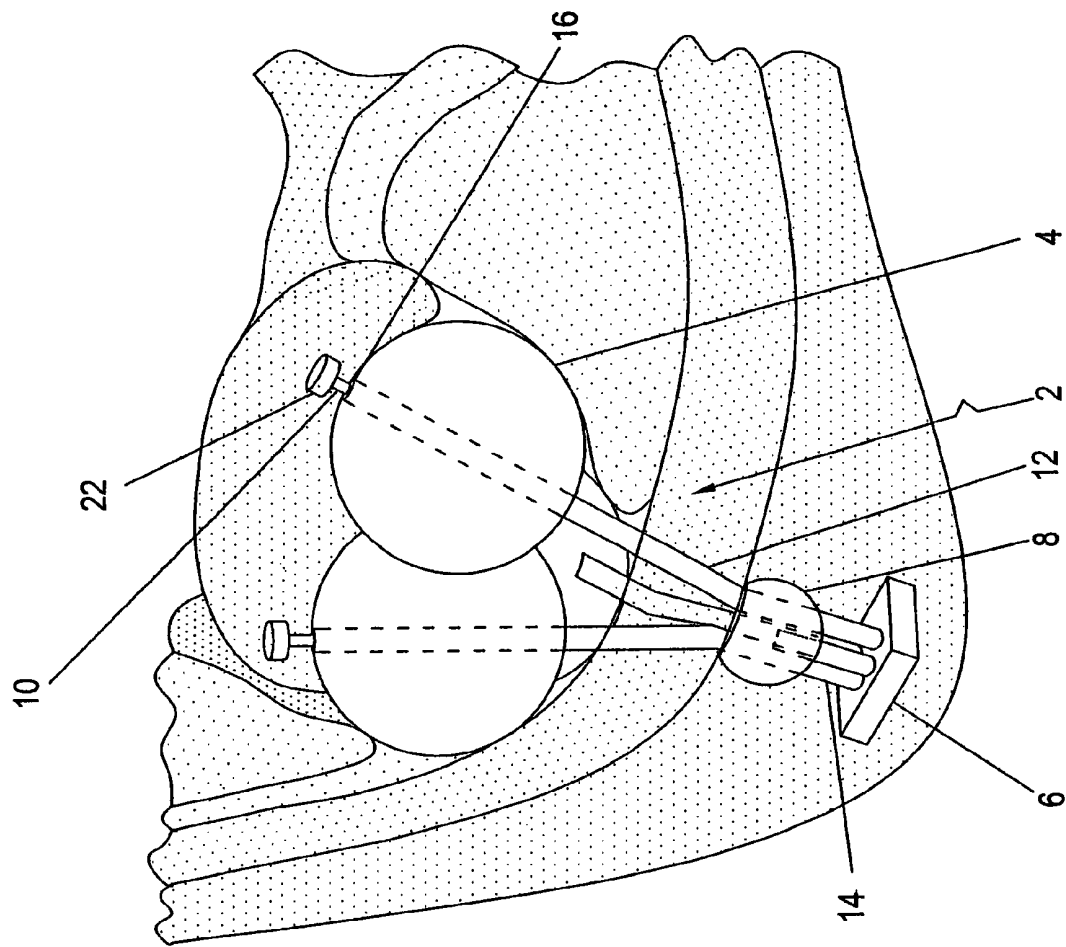


Fig. 1

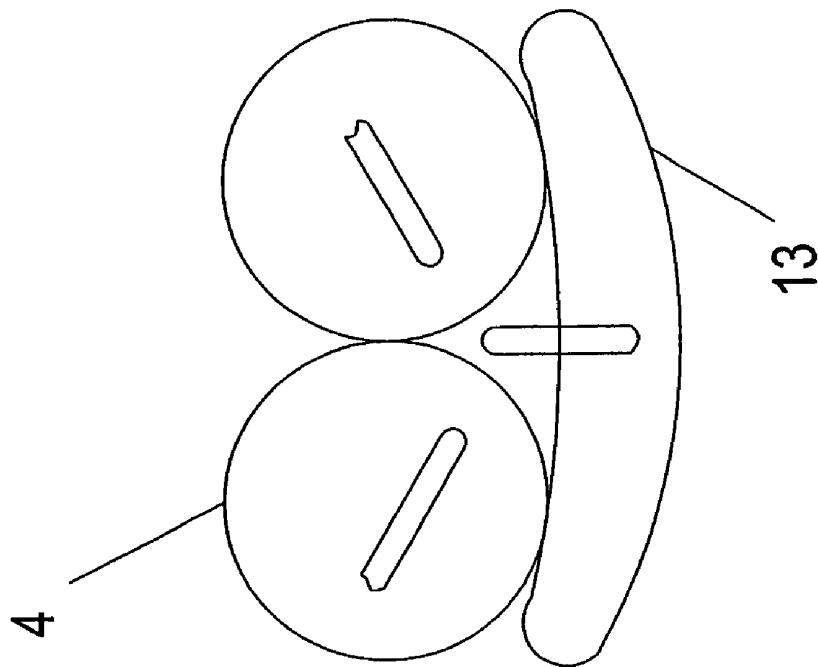


Fig. 2

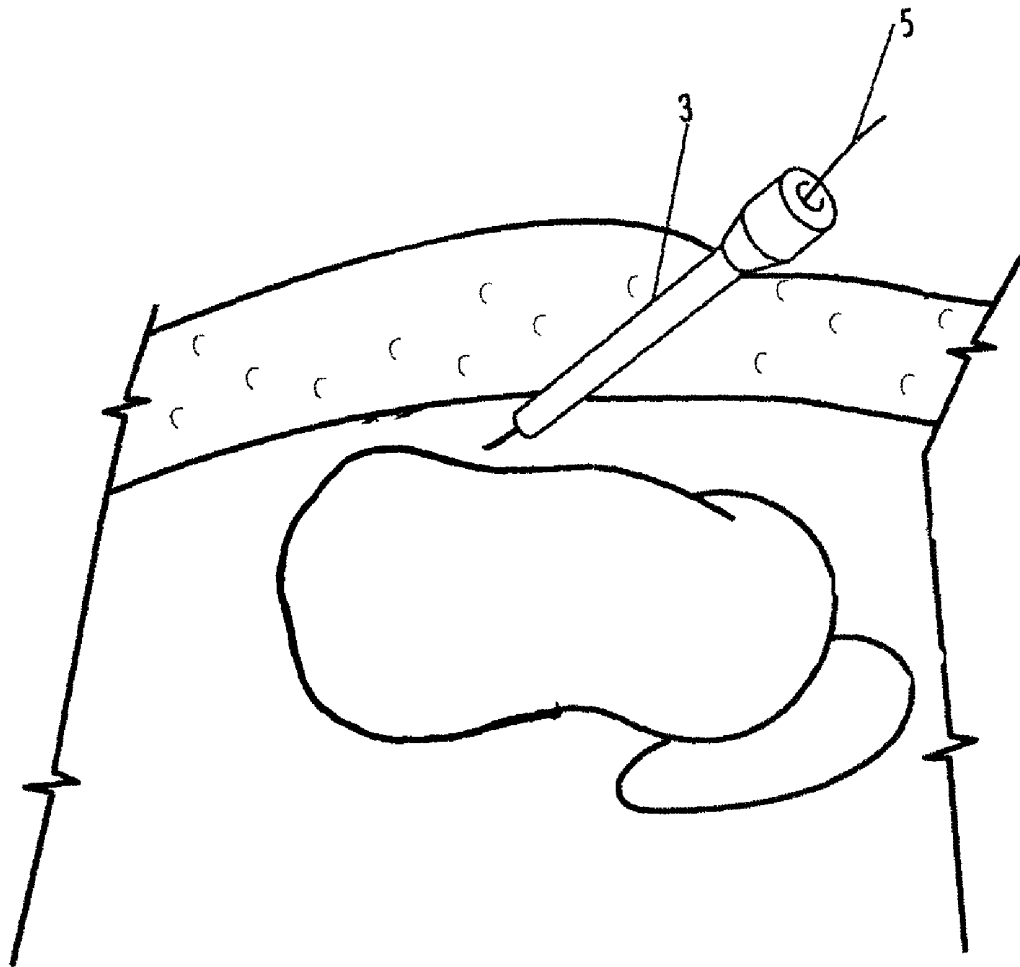


Fig. 3

COMPRESSIVE DEVICE FOR PERCUTANEOUS TREATMENT OF OBESITY

This is the United States national stage of International Application PCT/US04/24612, filed 30 Jul. 2004, which claims the priority filing date of U.S. provisional application 60/494,698, filed 13 Aug. 2003 under 35 U.S.C. §119(e).

TECHNICAL FIELD

This invention pertains to multiple expandable devices that can be implanted to treat obesity in mammals by reducing the volume of the stomach.

BACKGROUND ART

Obesity is a complex, medical disease affecting more than 30% of the population in the United States. Obesity affects an individual's personal quality of life and contributes significantly to morbidity and mortality. Obese patients, i.e. individuals having a body mass index ("BMI") greater than 30, often have a high risk of associated health problems (e.g., diabetes, hypertension, and respiratory insufficiency), including early death. In the United States, approximately 280,000 deaths annually are attributed to obesity and obesity-related diseases. In the case of morbid obesity, studies have shown that conservative treatment with diet and exercise may be ineffective for reducing excess body weight. In addition, specific diets, medications, behavioral modifications, and exercise programs have over a 95% failure rate in morbidly obese individuals. Consequently, surgery is often the most effective means of treatment. "Bariatric surgery" is the field of surgery that treats people who are so overweight that they are suffering health consequences due to the excess weight. The surgery usually involves operations on the stomach to restrict one's ability to eat, or on the small intestine to restrict the absorption of ingested food. See M. Deitel, "Overview of Obesity Surgery," *World J. Surg.*, vol. 22, pp. 913-918 (1998).

A successful bariatric surgery results in a maintained weight loss of greater than 50% of excess body weight and in an increase in patient wellness. An important factor for success is a long-term relationship between the patient and a medical team, which includes the doctor performing the procedure, a dietitian, a psychologist, and a physical therapist. While current bariatric surgery may assist patients in reducing food intake, it may also increase medical risks due to complications inherently associated with surgery, including complications of anesthesia, surgical procedure, wound infections, dehiscence, stomal stenosis, marginal ulcers, thrombophlebitis, and pulmonary problems.

There are several bariatric surgical procedures for treating morbid obesity. One procedure for treating morbid obesity is referred to as a "biliopancreatic diversion." Biliopancreatic diversion surgery is a reduction of the stomach volume and a diversion of food from the stomach to the final segment of the small intestine, bypassing the beginning and middle portions of the small intestine to limit the amount of nutrients and calories absorbed by the body. This procedure removes about one half of the stomach, and then connects the stomach to the last 250 cm of the small intestine. Disadvantages of this surgery include patients suffering from protein malnutrition, anemia, gastric retention, diarrhea, abdominal bloating, and intestinal obstruction. See P. Marceau, et al., "Malabsorptive Obesity Surgery," *Surg. Clinics of North America*, vol. 81(5), pp. 1113-28 (2001).

Another bariatric surgery, "gastric bypass," is a bypass connecting the lower compartment of the stomach to the

initial portion of the small intestine. This procedure limits the amount of food that can be ingested at one sitting and reduces absorption of food across the small intestine. In addition to surgical complications, patients may also suffer from acute gastric dilation, anastomotic leak, anemia, and dumping syndrome. See R. E. Brolin, "Gastric Bypass," *Surg. Clinics of North America*, vol. 81(5), pp. 1077-1096 (2001).

A third bariatric surgical procedure is "gastric banding," which constricts the stomach to form an hourglass shape. This procedure restricts the amount of food that passes from one section to the next, which induces a feeling of satiety. A band is placed around the stomach near the junction of the stomach and esophagus. The small upper stomach pouch is filled quickly, and slowly empties through the narrow outlet to produce a feeling of satiety. In addition to surgical complications, patients undergoing this procedure may also suffer from esophageal injury, splenic injury, band slippage, staple line disruption, reservoir deflation/leak, and persistent vomiting. See E. J. DeMaria, "Laparoscopic Adjustable Silicone Gastric Banding," *Surg. Clinics of North America*, vol. 81(5), pp. 1129-44 (2001).

A fourth bariatric surgical procedure is "vertical-banded gastroplasty," which restricts the volume of the stomach by using staples. In this procedure, staples are placed in the upper stomach region to create a small pouch with a narrow outlet to the remaining portion of the stomach. A lap-band is placed around the narrow outlet to provide support and inhibit stretching of the stomach. In addition to surgical complications, patients undergoing this procedure may suffer from vomiting, ulcers, band erosion, and leaks. See C. Doherty, "Vertical Banded Gastroplasty," *Surg. Clinics of North America*, vol. 81(5), pp. 1097-1112 (2001).

U.S. Pat. No. 6,102,922 describes a device and surgical method for reducing the food intake of a patient by forming a restriction in the stomach using a band. In one embodiment, the band is looped around the esophagus and a portion of the stomach is pulled up through the band loop. This forms a small stomach pouch and a narrow outlet to the remaining portion of the stomach. This allows for a quick filling of the small stomach pouch, and a slow emptying of the stomach through the narrow outlet to produce a feeling of satiety.

U.S. Pat. No. 6,475,136 describes a device for treating heartburn and reflux disease by restricting the amount of food flowing into a stomach or an esophagus, comprising a restriction device (a sphincter or a cuff) that can be adjusted. In one embodiment, the restriction device performs like an artificial sphincter that opens and closes the food passageway in the stomach. In an alternative embodiment, the restriction device comprises an adjustable cuff, a clamp, or a roller to bend or rotate the esophagus or stomach to close or almost close the junction between the stomach and esophagus.

U.S. Pat. No. 4,246,893 describes a device and method for treating obesity by compressing the stomach and reducing its capacity using a single adjustable distensible device (e.g., a balloon) whose volume can be adjusted from an external port.

U.S. Pat. No. 5,993,473 and WO 99/2418 describe a device and surgical method for treating obesity by decreasing the volume of the stomach by using a single expandable device placed inside the stomach cavity.

U.S. Pat. No. 4,694,827 describes a device and method for controlling obesity by deterring ingestion of food using a single balloon that is placed inside the stomach.

U.S. Publication No. 2002/0188354 describes a device for treating obesity by inserting an hourglass-shaped device into the junction between the stomach and the small bowel, which delays gastric emptying of food.

U.S. Pat. No. 6,511,490 describes a device for the treatment of morbid obesity by restricting food passage in the stomach by placing an inflatable band around the stomach to create a pouch with a small opening adjacent to the esophagus. The inflatable band is secured and then inflated until the appropriate sized opening is achieved.

DISCLOSURE OF INVENTION

We have discovered an apparatus and method for effectively treating morbid obesity in mammals, while minimizing the health risks associated with traditional surgery. The device reduces the gastric volume of the stomach and induces early satiety. The "gastric reduction assembly" comprises at least two or more expandable devices (e.g., balloons), each able to be independently inflated and adjusted from an external port. Each expandable device can be filled with a fluid (e.g., CO₂, isotonic dextrose solution, isotonic saline solution, etc.) using a filling tube (e.g., a catheter), which can be easily accessed externally. In a preferred embodiment, the gastric reduction assembly is inserted percutaneously through the antero-lateral abdominal wall, and placed at a location exterior to the stomach body, avoiding an abdominal incision. Laparoscopic guidance, optionally, may be used to assist in placing the gastric reduction assembly near the stomach body. Once positioned near the stomach body, the gastric reduction assembly can be inflated to compress the volume of the stomach and effectively limit food intake. The gastric reduction assembly, with multiple expandable devices, minimizes the potential for post-implantation movement. The expandable devices have a size and shape to complement each other, such that they form a barrier when inflated that minimizes post implantation movement.

To further minimize inferior migration, a subcutaneous anchor (e.g., a balloon or ring placed within the fatty layer between the skin and the abdominal wall), may be attached to the filling tubes to anchor the expandable devices to the abdominal wall. In addition, each expandable device may use an intragastric anchor (e.g., a collapsible fixation disc) to anchor the expandable device against the stomach body.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 illustrates a perspective view of one embodiment of the gastric reduction assembly, implanted in the peritoneal cavity around the stomach.

FIG. 2 illustrates a front view of one embodiment of the gastric reduction assembly which has three expandable devices: two spherical-shaped and one crescent-shaped.

FIG. 3 illustrates a guidewire having been inserted through a sheath according to an embodiment of the present invention described herein.

The invention provides a reliable, inexpensive method for treating obesity in mammals by reducing the volume of the stomach without abdominal surgery, thus reducing postoperative surgical complications. The gastric reduction assembly can provide either an intraperitoneal or an extraperitoneal method to compress the stomach. The placement depends on the surgeon's preference, and the physical condition and body habitus of the patient. In the intraperitoneal cavity, expandable devices can be placed either at pregastric location (i.e., either anterior or anterolateral to the stomach) or a retrogastric location (i.e., either posterior or posterolateral to the stomach), or both. In the extraperitoneal cavity, the expandable devices can be placed in any of the anatomical compartments, spaces, or layers of the abdominal wall. Candidates for this minimally invasive procedure include patients with a

BMI greater than 40, or patients with a BMI less than 40 and a debilitating disease related to the obesity such as diabetes, hypertension, and respiratory insufficiency.

MODES FOR CARRYING OUT THE INVENTION

The basic design comprises a gastric reduction assembly having at least two or more expandable devices (e.g., balloons), each able to be adjusted and independently inflated. Each device can be inflated with a fluid (e.g., CO₂, isotonic dextrose solution, isotonic saline solution, etc.) using a filling tube. The filling tube is accessed externally by way of an access device. To inflate each expandable device, the inlet of each filling tube is attached to a corresponding port, and fluid is injected into the inlet via a carrier (e.g., a hypodermic syringe). Fluid flows through the filling tube into each expandable device. Alternatively, fluid can be removed by reversing the process. The filling tubes may be locked together inside a single catheter or other large tubing such that only one tube crosses the abdominal wall to the access port.

In a preferred embodiment, compression of the stomach is achieved using two or more spherical-shaped expandable devices to form a compressive barrier that reduces the volume of the stomach and minimizes post-implantation movement. Optionally, at least one crescent-shaped expandable device may be used to support the spherical-shaped expandable devices. The shape of the barrier formed by the multiple expandable devices may be adjusted to complement that of surrounding tissues and organs of the patient by changing the volume of the devices.

To further minimize post-implantation movement, a subcutaneous anchor may be used to help anchor the expandable devices to the abdominal wall. In one embodiment, the subcutaneous anchor is a balloon-like device adapted to circumscribe the filling tubes subcutaneously or below the abdominal wall, at the muscular layer level. The volume of the subcutaneous anchor is adjusted by adding fluid. Alternatively, a ring lock may be placed around each filling tube at the muscular layer. In another embodiment, the expandable devices may be anchored to the stomach using an anchor e.g., a collapsible, fixation disc placed inside the stomach. One method of placement is to pass the intragastric anchor through a separate tube that crosses the expandable device and ends inside the stomach cavity. The tube can be accessed externally.

The expandable devices can be implanted bypassing through the skin and across the anterior abdominal wall via a larger tube to a predetermined implantation site. The expandable devices remain at the site, attached to filling tubes that can be accessed externally through a small single access port.

The gastric reduction assembly has several advantages. First, the potential for incisional hernia and wound infections is substantially reduced, since no surgical incision of the abdominal wall is needed. The expandable devices are inserted through the skin and across the anterior abdominal wall via a small puncture. The access device for refilling or deflating the expandable devices is placed in the fatty layers of the abdomen, between the skin and the anterior abdominal muscles. Second, post-implantation movement is substantially reduced, almost eliminating a need to re-orient the expandable devices following implantation. Third, modifications (e.g., inflation, deflation, reorientation, or removal) may easily be done without surgery.

FIG. 1 illustrates a perspective view of one embodiment of the gastric reduction assembly 2, in accordance with the present invention. In this embodiment, the device comprises an access device 6, a subcutaneous anchor 8, and at least two

or more expandable devices **4**, each having an intragastric anchor **10** and a filling tube **12**. Multiple expandable devices **4** are sized and shaped to complement each other such that when inflated, they cluster to form a compressive barrier capable of reducing the stomach volume and minimizing post-implantation movement. To adjustably inflate the expandable devices **4** in the peritoneal cavity, fluid is injected into each filling tube **12** of each expandable device **4** via the access device **6**.

As shown in FIG. 1, gastric reduction assembly **2** comprises three spherical-shaped expandable devices **4** (e.g., balloons) placed at a pregastric location. Alternatively, gastric reduction assembly **2** may comprise another number of expandable devices **4** (e.g., two, four, five, six, etc.). Optionally, at least one crescent-shaped expandable device **13** may be used, as shown in FIG. 2. This enhances the compressive barrier by forming a carrier ridge to support spherical-shaped expandable devices **4**. Expandable devices **4** can be made of any durable, distensible biocompatible material, such as rubber, latex, or polyurethane elastomer.

As shown in FIG. 1, each filling tube **12** has an inlet at the access device **6** and an outlet to the interior of each expandable device **4** to allow for inflation with fluid. In an alternative embodiment, a single filling tube **12** that has an inlet and outlet (not shown) for each expandable device **4** may be used. Filling tubes **12** should be made of a durable, flexible, biocompatible material, such as TYGON® tubing, polyurethane, or other plastics.

As shown in FIG. 1, subcutaneous anchor **8** is a distensible balloon-like device that circumscribes filling tubes **12** within the fatty layer between the skin and abdominal wall or at a subperitoneal (i.e., below the abdominal wall) region to anchor the expandable devices **4** to the abdominal wall. The balloon-like device is inflated via its own filling tube **14**. Alternatively, subcutaneous anchor **8** can be a ring lock (not shown) that joins all filling tubes **12** and advanced towards the abdominal wall, it forms an anchor against the muscular layer of the abdominal wall. Subcutaneous anchor **8** should be made of a durable, distensible biocompatible material, such as rubber, latex, or polyurethane elastomer.

As shown in FIG. 1, intragastric anchor **10** is a collapsible, fixation disc which can be inserted through the stomach wall via tube **12** with a second channel **16** that extends through each expandable device **4**. The disc, once opened in the stomach, anchors expandable device **4** against the stomach. Once intragastric anchor **10** is positioned within the stomach and unfolds, an attached suture may be pulled to form a snug fit between the exterior surface of the stomach body and expandable devices **4**. The size and shape of intragastric anchor **10** is chosen to complement the inner surface of the stomach, and to provide a sufficient surface area (when unfolded) to prevent intragastric anchor **10** from dislodging from the stomach when tension is applied. Intragastric anchor **10** should be made of a biocompatible material capable of shape memory, e.g., nitinol coated with polytetrafluoroethylene.

An access device **6** comprises ports (not shown) to filling tubes **12**. The size and shape of access device **6** is adapted to allow for a tight seal with filling tubes **12** and a fluid carrier (e.g., a hypodermic syringe). The number of ports is determined by the number of tubes (**12** and **14**) that need to be accessed from the outside.

A preferred method of implanting the gastric reduction assembly is to go through the skin with a minimally invasive puncture. For example, a nasogastric tube (Bard, Covington, Ga.) is inserted into the stomach. The stomach is then inflated to better visualize it under fluoroscopy so that the proper

location for an access site through the skin can be determined. The access site should be below the rib cage, near the gastric chamber. Once the access site is determined, a micropuncture needle (e.g., 22 g; Cook, Inc., Bloomington, Ind.) is inserted into the peritoneal cavity immediately in front of the anterior gastric wall. A microwire (e.g., 0.018 in; Cook, Inc., Bloomington, Ind.) is passed through the needle under fluoroscopic guidance and into the peritoneal cavity. Once the microwire reaches the peritoneal cavity, the micropuncture needle is removed over the wire.

An access sheath (e.g., 6 French introducer; Cook, Inc., Bloomington, Ind.), a hollow tube that fits through the skin to form a temporary pathway to the peritoneal cavity, is then inserted over the microwire. The microwire is then removed, leaving the access sheath in place. A guidewire (see FIG. 3) (e.g., 0.035 in stiff regular or hydrophilic; Boston Scientific, Natick, Mass.) is then inserted through the access sheath **3** to provide additional support. The opening in the abdominal wall is progressively dilated with dilators (Cook, Inc. Bloomington, Ind.) from 6-14 French. When the opening is sufficiently large, a larger access sheath (e.g., 14 Fr peel-away sheath; Cook, Inc. Bloomington, Ind.) is placed over the 0.035 in stiff guidewire, and the dilator and guidewire are removed. Air is then evacuated from the stomach through the nasogastric tube to provide space for the gastric compression assembly **2**.

Introducer tubes (e.g., catheters) containing expandable devices **4** (e.g., balloons) attached to filling tubes **12** are inserted through the access sheath to a predetermined position near the stomach. Expandable devices **4** are released from the introducer tubes. The expandable devices **4** are then partially inflated sequentially near the stomach using a syringe to introduce fluid (e.g., CO₂, isotonic saline solution, or isotonic dextrose solution) to the expandable devices **4** through the filling tubes **12**. Introducer tubes are slowly withdrawn, and each filling tube **12** is pulled until each partially inflated expandable device **4** contacts the abdominal wall. The access sheath is then removed, and a subcutaneous anchor **8** (e.g., a balloon or ring lock) is placed within the fatty layer between the skin and abdominal wall or the subperitoneal region (i.e., below the abdominal wall) to anchor expandable devices **4**. Expandable devices **4** are then inflated to a volume sufficient to compress the stomach, and filling tubes **12** cut to an appropriate length. The inlets to filling tubes **12** are then attached to the ports of access device **6**, and access device **6** is placed within the fatty layer between the skin and abdominal wall. The skin is then closed with sutures.

In an alternative embodiment, each expandable device **4** is individually introduced to a preselected stomach compression site near the stomach and then anchored to the stomach, as described below. In this embodiment, filling tube **12** to each expandable device **4** has at least two channels. Filling tube **12** is positioned to pass through expandable device **4** and abut the side of expandable device **4** that is near the stomach. One channel of filling tube **12** has an opening that allows fluid to flow into expandable device **4** to inflate the device. The second channel of filling tube **12** passes intact through expandable device **4** to the wall near the stomach. This channel allows an intragastric anchor **10** to be placed inside the stomach to help anchor expandable device **4** as described below. Initially, a needle (e.g., an 18-gauge needle; Cook, Inc. Bloomington, Ind.) is passed through the access sheath to puncture the stomach wall. A contrast medium (e.g. gastrograffin) is then injected into the stomach to determine the needle's location. Once the location is determined, a suture **22** is attached to intragastric anchor **10**, and the collapsed anchor is advanced through the needle into the stomach in a

collapsed form using a stiff guidewire (e.g., 0.035 cm guidewire; Boston Scientific Corp, Natick, Mass.). Upon exiting the needle outlet within the stomach, intragastric anchor **10** resumes its disc-shaped configuration. Intragastric anchor **10** can be covered with a biocompatible material (e.g., GORTEX®, DACRON®, polyethylene or silicone) to help seal the gastric puncture site. The 18-gauge needle is then removed, while the stiff guidewire and suture remain attached to the intragastric anchor **10**. Preferably, suture **22** is attached to the guidewire to allow for withdrawal. This process is repeated for each of the remaining expandable devices **4**. The stiff guidewire is then passed through the second channel of filling tube **12** for each expandable device **4**. Expandable devices **4** are then positioned at preselected stomach compression sites as described above. After verifying the compressive effects of each expandable device **4** on the gastric volume of the stomach, the stiff guidewires are disconnected from sutures **22** and removed. Each suture **22** is then pulled back through the second channel of filling tube **12** to anchor the device to the stomach wall. The access sheath is then removed, and filling tubes **12** are cut to an appropriate length. The ends of each suture are pulled through the second channel and attached to access device **6** to anchor expandable devices **4**. Expandable devices **4** can then be inflated or deflated through access device **6**, as necessary. Access device **6** is then placed within the fatty layer between the skin and the abdominal wall, and the skin is closed with sutures.

Clinical trials will initially involve testing two groups (a test and a control) of pigs weighing more than 50 kg. The gastric reduction assembly will be implanted into the test group. Once the gastric reduction assembly has been implanted, an upper gastrointestinal study (“UGI”) will be conducted with barium to check the gastric volume and passage of material through the stomach into the small intestine. The volume of the expandable devices will be adjusted in the test group based on the findings of the UGI. UGIs will be conducted at various intervals to check on the location and volume of the expandable devices. The two groups will be weighed weekly. After six months, the animals will be euthanized and the position of the gastric reduction assembly evaluated during necropsy. The data will be analyzed for differences in weight loss between the two groups.

The complete disclosures of all references cited in this specification are hereby incorporated by reference. In the event of an otherwise irreconcilable conflict, however, the present specification shall control.

We claim:

1. A method of treating obesity in a patient, said method comprising:
 - making a percutaneous opening to the abdominal cavity of the patient;

passing an expandable device, while in a contracted configuration, through said opening;

- positioning the expandable device adjacent the stomach of the patient;

- expanding the expandable device to occupy a volume of space and substantially prevent the stomach from expanding into the volume of space; and

- anchoring the expandable device to at least one structure in the abdominal cavity, wherein the expandable device is drawn into contact with a location of the at least one structure that the expandable device is anchored to.

2. A method of treating a patient, said method comprising:
 - passing a device including an expandable member in a collapsed configuration through an opening in the skin of the patient, and into the abdominal cavity of the patient;

- anchoring at least a portion of the expandable member, relative to at least one structure in the abdominal cavity without piercing the stomach, wherein the at least a portion is drawn into contact with a location of the at least one structure that the at least a portion is anchored to; and

- expanding the expandable member to an expanded configuration in a space in the abdominal cavity to perform at least one of: prevention of expansion of the stomach of the patient into the space; and compression of a portion of the stomach.

3. The method of claim **2**, wherein said method is performed as a percutaneous procedure.

4. The method of claim **2**, wherein said method is performed as a laparoscopic procedure.

5. The method of claim **2**, wherein a guidewire is passed through the skin of the patient, and into the abdominal cavity, and wherein the device is passed over the guidewire to guide the device to an intended location in the abdominal cavity.

6. The method of claim **2**, further comprising inserting a sheath through a minimally invasive opening made through the skin and the abdominal wall, wherein the guidewire is inserted through the sheath to pass the guidewire through the skin and abdominal wall and into the abdominal cavity.

7. The method of claim **2**, wherein said device further comprises a second expandable member, said method further comprising at least partially expanding the second expandable member.

8. The method of claim **2**, wherein the device is passed in a compact configuration, the compact configuration being achieved and maintained by compacting the expandable member and inserting the expandable member within a sheath.

* * * * *

专利名称(译)	用于经皮治疗肥胖症的压缩装置		
公开(公告)号	US8192455	公开(公告)日	2012-06-05
申请号	US10/567199	申请日	2004-07-30
[标]申请(专利权)人(译)	BRAZZINI AUGUSTO 基尔希戴维家 CASTANEDA祖尼加WILFRIDOř đAGOSTINO HORACIO		
申请(专利权)人(译)	BRAZZINI AUGUSTO 基尔希戴维家 CASTANEDA-祖尼加WILFRIDOř đAGOSTINO HORACIO		
当前申请(专利权)人(译)	董事局的路易斯安那州立大学与农业和机械大学监事		
[标]发明人	BRAZZINI AUGUSTO KIRSCH DAVID S CASTANEDA ZUNIGA WILFRIDO R DAGOSTINO HORACIO		
发明人	BRAZZINI, AUGUSTO KIRSCH, DAVID S. CASTANEDA-ZUNIGA, WILFRIDO R. D'AGOSTINO, HORACIO		
IPC分类号	A61M29/00 A61B A61F5/00 A61M5/00		
CPC分类号	A61F5/003 A61F5/0033 A61F5/0073		
代理机构(译)	CANNON , ALAN W.		
审查员(译)	JACKSON , GARY		
助理审查员(译)	MENDOZA , MICHAEL		
优先权	60/494698 2003-08-13 US		
其他公开文献	US20070060940A1		
外部链接	Espacenet USPTO		

摘要(译)

一种使用胃减容组件治疗哺乳动物中的病态肥胖症的装置和方法，所述胃减少组件减少胃的胃容积并诱导早期饱腹感。胃减容组件包括至少两个或更多个可膨胀装置，每个可膨胀装置能够使用填充管可调节地用流体（例如液体或气体）充气。在优选实施例中，胃减容组件穿过腹壁插入并放置在胃体外部的的位置，避免腹部切口。一旦定位在胃体附近，胃减容组件允许胃体的外部压缩以限制食物摄入。胃减容组件还使可膨胀装置在插入胃体后恢复其预压缩状态的可能性最小化。

