



US009345476B2

(12) **United States Patent**
Surti

(10) **Patent No.:** **US 9,345,476 B2**
(45) **Date of Patent:** **May 24, 2016**

(54) **TACKING DEVICE AND METHODS OF DEPLOYMENT**

- (75) Inventor: **Vihar C. Surti**, Winston-Salem, NC (US)
(73) Assignee: **COOK MEDICAL TECHNOLOGIES LLC**, Bloomington, IN (US)
(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 246 days.

(21) Appl. No.: **12/787,744**

(22) Filed: **May 26, 2010**

(65) **Prior Publication Data**

US 2010/0305591 A1 Dec. 2, 2010

Related U.S. Application Data

(60) Provisional application No. 61/181,946, filed on May 28, 2009.

(51) **Int. Cl.**
A61B 17/064 (2006.01)
A61B 17/00 (2006.01)

(52) **U.S. Cl.**
CPC **A61B 17/064** (2013.01); **A61B 2017/00862** (2013.01); **A61B 2017/00867** (2013.01); **A61B 2017/0649** (2013.01)

(58) **Field of Classification Search**
CPC A61F 2220/0008; A61F 2220/0016; A61B 17/12122; A61B 17/064; A61B 2017/0649
USPC 606/139, 142, 143, 151, 157, 158, 213, 606/215, 232; 623/23.72–23.76
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,199,025 A 4/1940 Conn
2,671,444 A 3/1954 Pease, Jr.
3,209,422 A 10/1965 Dritz
3,399,432 A 9/1968 Merser
3,470,834 A 10/1969 Bone
3,556,079 A 1/1971 Omizo

(Continued)

FOREIGN PATENT DOCUMENTS

EP 0310582 A1 4/1989
EP 0774237 A2 5/1997

(Continued)

OTHER PUBLICATIONS

Communication Pursuant to Rules 161(1) and 162EPC for European Patent Application Serial No. 09791618.3, dated Mar. 28, 2011, 2 pages.

(Continued)



Primary Examiner — Thomas McEvoy

(74) *Attorney, Agent, or Firm* — Brinks Gilson & Lione

(57) **ABSTRACT**

The present embodiments provide apparatus and methods suitable for coupling a graft member to tissue, closing a bodily opening, and the like. In one embodiment, a tacking device comprises a wire having first and second ends, and further having delivery and deployed states. In the contracted state, the wire comprises an elongated configuration that is substantially parallel to a central longitudinal axis. In the expanded state, the wire comprises a head region and a body region, the head region comprising at least one full turn having a first diameter, and the body region comprising at least two full turns having a second diameter, wherein the first diameter is greater than the second diameter. One or more of the tacking devices may be delivered using a laparoscopic, endoscopic or percutaneous approach.

5 Claims, 4 Drawing Sheets

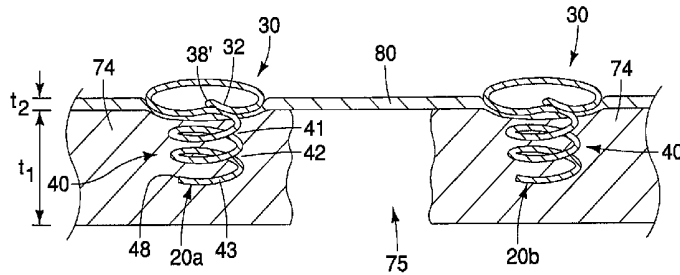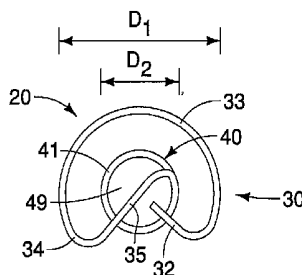

(56)

References Cited

U.S. PATENT DOCUMENTS

3,814,104 A	6/1974	Irnich et al.	6,228,055 B1	5/2001	Foerster et al.
3,856,016 A	12/1974	Davis	6,241,747 B1	6/2001	Ruff
3,954,108 A	5/1976	Davis	6,290,674 B1	9/2001	Roue et al.
3,958,576 A	5/1976	Komiya	6,306,150 B1	10/2001	Levinson
4,006,747 A	2/1977	Kronenthal et al.	6,328,727 B1	12/2001	Frazier et al.
4,204,541 A	5/1980	Kapitanov	6,371,963 B1	4/2002	Nishtala et al.
4,217,902 A	8/1980	March	6,375,671 B1 *	4/2002	Kobayashi et al. 606/213
4,235,238 A	11/1980	Ogiu et al.	6,402,765 B1	6/2002	Monassevitch et al.
4,485,816 A	12/1984	Krumme	6,419,669 B1	7/2002	Frazier et al.
4,621,639 A	11/1986	Transue et al.	6,425,887 B1	7/2002	McGuckin et al.
4,749,114 A	6/1988	Green	6,425,900 B1	7/2002	Knodel et al.
4,773,420 A	9/1988	Green	6,428,548 B1	8/2002	Durgin et al.
4,791,707 A	12/1988	Tucker	6,446,854 B1	9/2002	Remiszewski et al.
4,796,627 A	1/1989	Tucker	6,447,530 B1	9/2002	Ostrovsky et al.
4,821,939 A	4/1989	Green	6,468,290 B1	10/2002	Weldon et al.
4,832,027 A	5/1989	Utz	6,482,178 B1	11/2002	Andrews et al.
4,990,156 A	2/1991	Lefebvre	6,491,707 B2	12/2002	Makower et al.
4,994,069 A *	2/1991	Ritchart et al. 606/191	6,551,333 B2	4/2003	Kuhns et al.
5,015,249 A	5/1991	Nakao et al.	6,572,629 B2	6/2003	Kaloo et al.
5,049,153 A	9/1991	Nakao et al.	6,592,559 B1	7/2003	Pakter et al.
5,059,205 A	10/1991	El-Nounou et al.	6,623,510 B2	9/2003	Carley et al.
5,084,057 A	1/1992	Green et al.	6,641,557 B1	11/2003	Frazier et al.
5,099,827 A	3/1992	Melzer et al.	6,699,256 B1	3/2004	Logan et al.
5,100,420 A	3/1992	Green et al.	6,699,263 B2	3/2004	Cope
5,123,914 A	6/1992	Cope	6,712,804 B2	3/2004	Roue et al.
5,156,609 A	10/1992	Nakao et al.	6,719,777 B2	4/2004	Ginn et al.
5,192,303 A	3/1993	Gattorna et al.	6,746,458 B1	6/2004	Cloud
5,203,787 A	4/1993	Noblitt et al.	6,746,460 B2	6/2004	Gannoe et al.
5,242,456 A	9/1993	Nash et al.	6,746,472 B2	6/2004	Frazier et al.
5,324,307 A	6/1994	Jarrett et al.	6,776,783 B1	8/2004	Frantzen et al.
5,333,624 A	8/1994	Tovey	6,849,078 B2	2/2005	Durgin et al.
5,334,217 A	8/1994	Das	6,884,248 B2	4/2005	Bolduc et al.
5,350,385 A	9/1994	Christy	6,911,032 B2	6/2005	Jugenheimer et al.
5,366,480 A	11/1994	Corriveau et al.	6,913,607 B2	7/2005	Ainsworth et al.
5,368,600 A	11/1994	Failla et al.	6,966,916 B2	11/2005	Kumar
5,368,602 A	11/1994	de la Torre	6,994,713 B2	2/2006	Berg et al.
5,411,522 A	5/1995	Trott	7,001,398 B2	2/2006	Carley et al.
5,417,691 A	5/1995	Hayhurst	7,018,388 B2	3/2006	Yencho et al.
5,437,266 A	8/1995	McPherson	7,025,756 B2	4/2006	Frazier et al.
5,520,700 A	5/1996	Beyar et al.	7,056,325 B1	6/2006	Makower et al.
5,527,343 A	6/1996	Bonutti	7,060,084 B1	6/2006	Loshakove et al.
5,554,183 A	9/1996	Nazari	7,087,073 B2	8/2006	Bonutti
5,573,543 A	11/1996	Akopov et al.	7,112,214 B2	9/2006	Peterson et al.
5,582,615 A	12/1996	Foshee et al.	7,115,110 B2	10/2006	Frazier et al.
5,582,616 A	12/1996	Bolduc et al.	7,211,101 B2	5/2007	Carley et al.
5,593,414 A	1/1997	Shipp et al.	7,326,221 B2	2/2008	Sakamoto
5,662,683 A	9/1997	Kay	7,326,231 B2	2/2008	Phillips et al.
5,667,527 A	9/1997	Cook	7,331,968 B2	2/2008	Arp et al.
5,674,231 A	10/1997	Green et al.	7,410,460 B2	8/2008	Benderev
5,690,656 A	11/1997	Cope et al.	7,416,554 B2	8/2008	Lam et al.
5,695,525 A	12/1997	Mulhauser et al.	7,485,124 B2	2/2009	Kuhns et al.
5,728,116 A	3/1998	Rosenman	7,494,496 B2	2/2009	Swain et al.
5,741,278 A	4/1998	Stevens	7,601,159 B2	10/2009	Ewers et al.
5,779,720 A	7/1998	Walder-Utz et al.	7,608,091 B2	10/2009	Goldfarb et al.
5,810,848 A	9/1998	Hayhurst	7,618,426 B2	11/2009	Ewers et al.
5,865,791 A	2/1999	Wayne et al.	7,621,925 B2	11/2009	Saadat et al.
5,868,763 A	2/1999	Spence et al.	7,622,068 B2	11/2009	Li et al.
5,891,159 A	4/1999	Sherman et al.	7,641,836 B2	1/2010	Li et al.
5,968,078 A	10/1999	Grotz	7,655,015 B2	2/2010	Goldfarb et al.
5,972,002 A	10/1999	Bark et al.	7,666,197 B2	2/2010	Orban, III
5,972,022 A	10/1999	Huxel	7,670,362 B2	3/2010	Zergiebel
5,976,159 A	11/1999	Bolduc et al.	7,695,493 B2	4/2010	Saadat et al.
5,984,917 A	11/1999	Fleischman et al.	7,704,264 B2	4/2010	Ewers et al.
5,984,949 A	11/1999	Levin	7,722,628 B2	5/2010	Stokes et al.
6,110,183 A	8/2000	Cope	7,727,247 B2	6/2010	Kimura et al.
6,113,612 A	9/2000	Swanson et al.	7,727,248 B2	6/2010	Smith et al.
RE36,974 E	11/2000	Bonutti	7,736,376 B2	6/2010	Sato et al.
6,149,658 A	11/2000	Gardiner et al.	7,736,378 B2	6/2010	Maahs et al.
6,152,935 A	11/2000	Kammerer et al.	7,736,379 B2	6/2010	Ewers et al.
6,152,937 A	11/2000	Peterson et al.	7,736,388 B2	6/2010	Goldfarb et al.
6,156,044 A	12/2000	Kammerer et al.	7,744,613 B2	6/2010	Ewers et al.
6,159,223 A	12/2000	Danks et al.	7,758,598 B2	7/2010	Conlon et al.
6,171,321 B1	1/2001	Gifford, III et al.	7,758,612 B2	7/2010	Shipp
6,183,486 B1	2/2001	Snow et al.	7,799,040 B2	9/2010	Stokes et al.
6,193,732 B1	2/2001	Frantzen et al.	7,803,165 B2	9/2010	Stokes et al.
			7,803,166 B2	9/2010	Stokes et al.
			7,815,652 B2	10/2010	Messerly et al.
			7,815,653 B2	10/2010	Stokes et al.
			7,815,659 B2	10/2010	Conlon et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,815,662	B2	10/2010	Spivey et al.	2007/0276424	A1	11/2007	Mikkaichi et al.
7,828,811	B2	11/2010	Kortenbach et al.	2008/0015633	A1	1/2008	Abbott et al.
7,842,053	B2 *	11/2010	Chanduszeko et al. 606/157	2008/0086153	A1	4/2008	Sakamoto et al.
2001/0002250	A1	5/2001	Burbank et al.	2008/0091059	A1	4/2008	Machold
2001/0037130	A1	11/2001	Adams	2008/0097489	A1	4/2008	Goldfarb et al.
2001/0039435	A1	11/2001	Roue et al.	2008/0114378	A1	5/2008	Matsushita
2002/0010481	A1 *	1/2002	Jayaraman 606/151	2008/0114398	A1	5/2008	Phillips et al.
2002/0099437	A1 *	7/2002	Anson et al. 623/1.15	2008/0147116	A1	6/2008	Smith et al.
2003/0158578	A1	8/2003	Pantages et al.	2008/0154290	A1	6/2008	Golden et al.
2003/0195561	A1	10/2003	Carley et al.	2008/0172088	A1	7/2008	Smith et al.
2004/0009289	A1	1/2004	Carley et al.	2008/0177304	A1	7/2008	Westra et al.
2004/0039414	A1	2/2004	Carley et al.	2008/0200930	A1	8/2008	Saadat et al.
2004/0044364	A1	3/2004	Devries et al.	2008/0208161	A1	8/2008	Kaji et al.
2004/0073236	A1	4/2004	Carley et al.	2008/0208214	A1	8/2008	Sato et al.
2004/0087981	A1	5/2004	Berube et al.	2008/0208218	A1	8/2008	Shiono
2004/0087985	A1	5/2004	Loshakove et al.	2008/0208219	A1	8/2008	Suzuki
2004/0092975	A1	5/2004	Loshakove et al.	2008/0208220	A1	8/2008	Shiono et al.
2004/0097982	A1	5/2004	Jugenheimer et al.	2008/0208251	A1	8/2008	Weadock et al.
2004/0167539	A1	8/2004	Kuehn et al.	2008/0221619	A1	9/2008	Spivey et al.
2004/0186514	A1	9/2004	Swain et al.	2008/0228199	A1	9/2008	Cropper et al.
2004/0220596	A1	11/2004	Frazier et al.	2008/0228202	A1	9/2008	Cropper et al.
2005/0015141	A1	1/2005	Quiachon et al.	2008/0228203	A1	9/2008	Bell et al.
2005/0033313	A1	2/2005	Chu et al.	2008/0243148	A1	10/2008	Mikkaichi et al.
2005/0038370	A1	2/2005	Kuth et al.	2008/0255422	A1	10/2008	Kondoh et al.
2005/0113851	A1	5/2005	Swain et al.	2008/0255423	A1	10/2008	Kondo et al.
2005/0119695	A1	6/2005	Carley et al.	2008/0262525	A1	10/2008	Chang et al.
2005/0143763	A1	6/2005	Ortiz et al.	2008/0269566	A1	10/2008	Measamer
2005/0171562	A1	8/2005	Criscuolo et al.	2008/0275297	A1	11/2008	Bakos et al.
2005/0182445	A1	8/2005	Zamierowski	2008/0281354	A1	11/2008	Cropper et al.
2005/0192596	A1	9/2005	Jugenheimer et al.	2008/0294178	A1	11/2008	Kortenbach et al.
2005/0197594	A1	9/2005	Burbank et al.	2008/0296344	A1	12/2008	Cropper et al.
2005/0234512	A1	10/2005	Nakao	2008/0300547	A1	12/2008	Bakos
2005/0251154	A1 *	11/2005	Chanduszeko et al. 606/151	2008/0300608	A1	12/2008	Measamer
2005/0251165	A1	11/2005	Vaughan et al.	2008/0300624	A1	12/2008	Schwemberger et al.
2005/0273119	A1 *	12/2005	Widomski et al. 606/151	2008/0300627	A1	12/2008	Measamer et al.
2005/0277945	A1	12/2005	Saadat et al.	2008/0319257	A1	12/2008	Sato et al.
2005/0277981	A1	12/2005	Maahs et al.	2009/0005800	A1	1/2009	Franer et al.
2005/0283188	A1	12/2005	Loshakove et al.	2009/0018552	A1	1/2009	Lam et al.
2006/0004409	A1	1/2006	Nobis et al.	2009/0069822	A1	3/2009	Takahashi et al.
2006/0004410	A1	1/2006	Nobis et al.	2009/0088780	A1	4/2009	Shiono et al.
2006/0015006	A1	1/2006	Laurence et al.	2009/0088797	A1	4/2009	Crombie et al.
2006/0015125	A1	1/2006	Swain	2009/0125038	A1	5/2009	Ewers et al.
2006/0025788	A1	2/2006	Loshakove et al.	2009/0125039	A1	5/2009	Mikkaichi et al.
2006/0025819	A1	2/2006	Nobis et al.	2009/0204147	A1	8/2009	Rahmani
2006/0106279	A1	5/2006	Machold et al.	2009/0222029	A1	9/2009	Gordin et al.
2006/0106405	A1	5/2006	Fann et al.	2009/0254119	A1 *	10/2009	Sibbitt et al. 606/213
2006/0116605	A1	6/2006	Nakao	2009/0287080	A1	11/2009	Nishina et al.
2006/0135989	A1	6/2006	Carley et al.	2009/0299385	A1	12/2009	Stefanchik et al.
2006/0155288	A1	7/2006	Little et al.	2009/0299406	A1	12/2009	Swain et al.
2006/0167484	A1	7/2006	Carley et al.	2009/0306686	A1	12/2009	Ohdaira
2006/0190016	A1	8/2006	Onuki et al.	2009/0318936	A1	12/2009	Harris et al.
2006/0190038	A1	8/2006	Carley et al.	2009/0326578	A1	12/2009	Ewers et al.
2006/0206063	A1	9/2006	Kagan et al.	2010/0010457	A1	1/2010	Ewers et al.
2006/0207606	A1	9/2006	Roue et al.	2010/0010508	A1	1/2010	Takahashi et al.
2006/0217762	A1	9/2006	Maahs et al.	2010/0010509	A1	1/2010	Ishioka et al.
2006/0235447	A1	10/2006	Walshe	2010/0010511	A1	1/2010	Harris et al.
2006/0237022	A1	10/2006	Chen et al.	2010/0010514	A1	1/2010	Ishioka et al.
2006/0237023	A1	10/2006	Cox et al.	2010/0010520	A1	1/2010	Takahashi et al.
2006/0241662	A1	10/2006	Adams et al.	2010/0042115	A1	2/2010	Saadart et al.
2006/0241691	A1	10/2006	Wilk	2010/0042144	A1	2/2010	Bennett
2006/0253144	A1	11/2006	Mikkaichi et al.	2010/0049244	A1	2/2010	Cohen et al.
2006/0271073	A1	11/2006	Lam et al.	2010/0076462	A1	3/2010	Bakos et al.
2006/0271101	A1	11/2006	Saadat et al.	2010/0076488	A1	3/2010	Spivey et al.
2007/0010835	A1	1/2007	Breton et al.	2010/0094341	A1	4/2010	Raju
2007/0100375	A1	5/2007	Mikkaichi et al.	2010/0106166	A1	4/2010	Cropper et al.
2007/0100376	A1	5/2007	Mikkaichi et al.	2010/0113873	A1	5/2010	Suzuki et al.
2007/0112362	A1	5/2007	Mikkaichi et al.	2010/0121351	A1	5/2010	Whitfield et al.
2007/0123840	A1	5/2007	Cox	2010/0174312	A1	7/2010	Maahs et al.
2007/0129755	A1	6/2007	Abbott et al.	2010/0198192	A1	8/2010	Serina et al.
2007/0173868	A1	7/2007	Bachinski et al.	2010/0211086	A1	8/2010	Ewers et al.
2007/0208360	A1	9/2007	Demarais et al.	2010/0217292	A1	8/2010	Kimura et al.
2007/0219411	A1	9/2007	Dejima et al.	2010/0217293	A1	8/2010	Kimura et al.
2007/0270752	A1	11/2007	LaBombard	2010/0217294	A1	8/2010	Kimura et al.
2007/0270943	A1	11/2007	Solem et al.	2010/0249498	A1	9/2010	Wingardner et al.
2007/0276416	A1	11/2007	Ginn et al.	2010/0256658	A1	10/2010	Criscuolo et al.
				2010/0264192	A1	10/2010	Marczyk
				2010/0268253	A1	10/2010	Ahlberg et al.
				2010/0268270	A1	10/2010	Viola
				2011/0022065	A1	1/2011	Shipp

(56)

References Cited

U.S. PATENT DOCUMENTS

FOREIGN PATENT DOCUMENTS

EP	1317904	A1	11/2003
EP	1961388	A2	8/2008
JP	2000-514336		10/2000
JP	2010-17542		1/2010
WO	WO88/01486		3/1988
WO	WO90/02522		3/1990
WO	WO95/21575		8/1995
WO	WO96/14020		5/1996
WO	WO96/40356		12/1996
WO	WO 98/02100		1/1998
WO	WO98/18389		5/1998
WO	WO99/62408		12/1999
WO	WO00/07506		2/2000
WO	WO00/16701		3/2000
WO	WO00/21443		4/2000
WO	WO00/56223		9/2000
WO	WO00/56227		9/2000
WO	WO01/19256		3/2001
WO	WO01/35832		5/2001
WO	WO01/58363		8/2001
WO	WO2005/034729		4/2005
WO	WO2007/004228		1/2007
WO	WO2007/24615		3/2007
WO	WO2007/089843		8/2007
WO	WO2007/142977		12/2007

OTHER PUBLICATIONS

Response to Communication Pursuant to Rules 161(1) and 162EPC for European Patent Application Serial No. 09791618.3, dated May 6, 2011, 4 pages.

International Search Report for PCT/US2009/041415, dated Jul. 24, 2009, 4 pages.

International Preliminary Report on Patentability for PCT/US2009/041415, dated Nov. 4, 2010, 6 pages.

International Search Report for PCT/US2009/054176, dated Nov. 20, 2009, 16 pages.

International Preliminary Report on Patentability for PCT/US2009/054176, dated Mar. 3, 2011, 9 pages.

International Search Report for PCT/US2009/056512, dated Feb. 10, 2010, 5 pages.

Article 34 Demand and Amendment for PCT/US2009/056512, dated Jul. 6, 2010, 22 pages.

International Preliminary Report on Patentability for PCT/US2009/056512, dated Jan. 10, 2010, 31 pages.

International Search Report and Written Opinion for PCT/US2009/056604, dated May 4, 2010, 9 pages.

International Search Report for PCT/US2009/066983, dated Jan. 19, 2010, 4 pages.

International Search Report and Written Opinion for PCT/US2009/066992, dated Mar. 4, 2010, 15 pages.

International Search Report and Written Opinion for PCT/US2009/067992, Jul. 9, 2010, 20 pages.

International Search Report and Written Opinion for PCT/US2009/067994, dated Jun. 10, 2010, 18 pages.

International Search Report and Written Opinion for PCT/US2010/036188, dated Sep. 14, 2010, 18 pages.

Restriction Requirement for U.S. Appl. No. 12/428,226, dated Apr. 27, 2011, 7 pages.

Response to Restriction Requirement for U.S. Appl. No. 12/428,226, dated May 27, 2011, 10 pages.

Office Action for U.S. Appl. No. 12/428,226, dated Jun. 9, 2011, 8 pages.

Office Action for U.S. Appl. No. 12/543,000, dated Mar. 15, 2011, 14 pages.

Fritscher-Ravens, "Transgastric endoscopy—a new fashion, a new excitement!", *Endoscopy*, vol. 39, 2007, pp. 161-167.

Sporn et al., "Endoscopic colotomy closure after full thickness excision: comparison of T fastener with multclip applier", *Endoscopy*, vol. 40, 2008, pp. 589-594.

Voermans et al., "In vitro comparison and evaluation of seven gastric closure modalities for natural orifice transluminal endoscopic surgery", *Endoscopy*, vol. 40, 2008, pp. 595-601.

Sclabas et al., "Endoluminal Methods for Gastrotomy Closure in Natural Orifice TransEnteric Surgery", *Surgical Innovation*, vol. 13, No. 1, Mar. 2006, pp. 23-30.

Desilets et al., "Loop-anchor purse-string versus endoscopic clips for gastric closure: a natural orifice transluminal endoscopic surgery comparison study using burst pressures", *Gastrointestinal Endoscopy*, vol. 70, No. 6, 2009, pp. 1225-1230.

Sporn et al., "Endoscopic colotomy closure for natural orifice transluminal endoscopic surgery using a T-fastener prototype in comparison to conventional laparoscopic suture closure", *Gastrointestinal Endoscopy*, vol. 68, No. 4, 2008, pp. 724-730.

Dray et al., "Air and fluid leak tests after NOTES procedures: a pilot study in a live porcine model", *Gastrointestinal Endoscopy*, vol. 68, No. 3, 2008, pp. 513-519.

Shurr et al., "An over-the-scope clip (OTSC) system for closure of iatrogenic colon perforations: results of an experimental survival study in pigs", *Endoscopy*, vol. 40, 2008, pp. 584-588.

Romanelli et al., "Natural orifice transluminal endoscopic surgery gastrotomy closure in porcine explants with the Padlock-G clip using the Lock-It system", *Endoscopy*, vol. 42, 2010, pp. 306-310.

Bergström et al., "Early clinical experience with a new flexible endoscopic suturing method for natural orifice transluminal endoscopic surgery and intraluminal endosurgery", *Gastrointestinal Endoscopy*, vol. 67, No. 3, 2008, pp. 528-533.

Park et al., "Endoscopic sutured closure of a gastric natural orifice transluminal endoscopic surgery access gastronomy compared with open surgical closure in a porcine model. A randomized, multicenter controlled trial", *Endoscopy*, vol. 42, 2010 pp. 311-317.

Yasser M. Bhat, MD, "Transluminal Endosurgery: Novel Use of Endoscopic Tacks for the Closure of Access Sites in Natural Orifice Transluminal Endoscopic Surgery," *Gastrointestinal Endoscopy*, vol. 69, No. 6, p. 1161.

International Preliminary Report on Patentability for PCT/US2010/036188 dated Dec. 8, 2011, 10 pgs.

Communication Under Rules 161(1) and 162 EPC for European Patent Application 10726736.1 dated Jan. 30, 2012, 2 pgs.

Reply to Communication Under Rules 161(1) and 162 EPC for European Patent Application 10726736.1 dated Jul. 30, 2012, 13 pgs.

Communication Under Article 94(3) EPC for European Patent Application 10726736.1 dated Apr. 4, 2013, 4 pgs.

Office Action for Canadian Application 2,763,133 dated Oct. 1, 2013, 3 pgs.

Examination Report No. 1 for Australian Application 2010254151 dated Nov. 19, 2012, 3 pgs.

Reply to Examination Report No. 1 for Australian Application 2010254151 dated Jul. 16, 2013, 7 pgs.

Examination Report No. 2 for Australian Application 2010254151 dated Sep. 23, 2013, 3 pgs.

Reply to Examination Report No. 2 for Australian Application 2010254151 dated Nov. 13, 2013, 4 pgs.

Notice of Acceptance for Australian Application 2010254151 dated Nov. 19, 2013, 2 pgs.

Office Action dated Feb. 12, 2014 for Japanese Patent Application 2012-513205, 5 pgs. Including English translation.

Office Action dated Nov. 18, 2014 for Japanese Patent Application 2012-513205, 3 pgs. Including English translation.

* cited by examiner

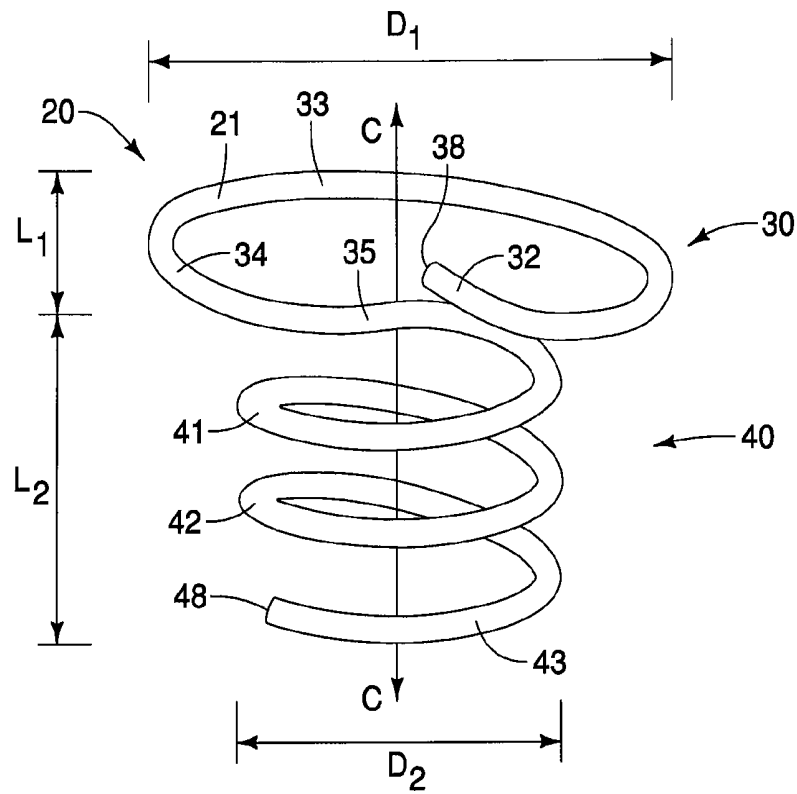


FIG. 1A

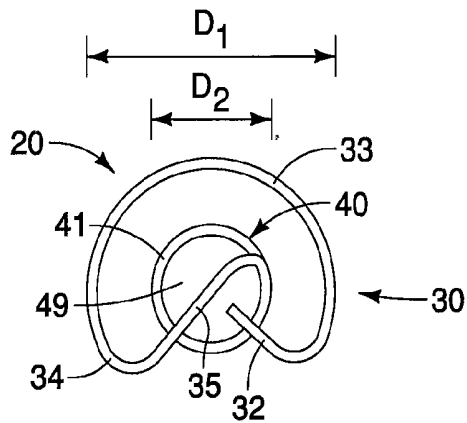


FIG. 1B

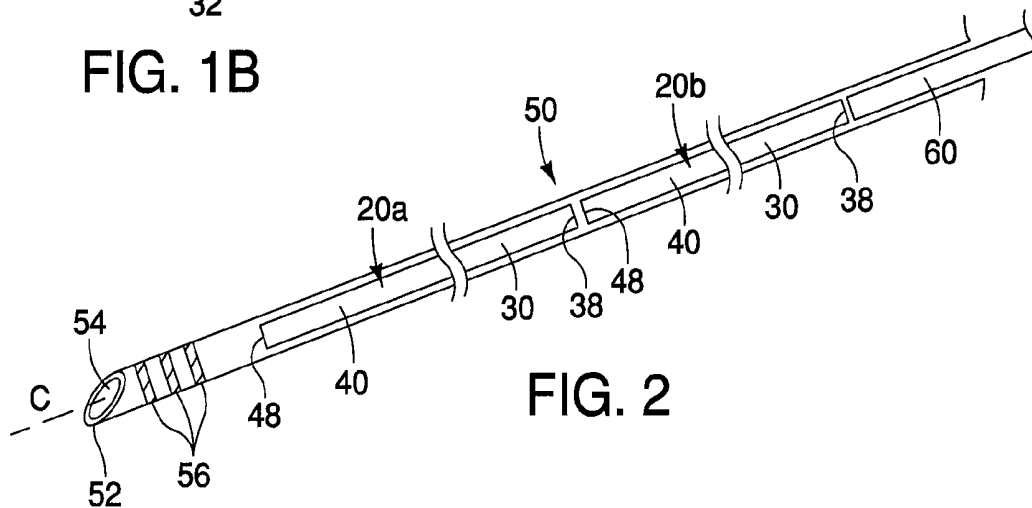


FIG. 2

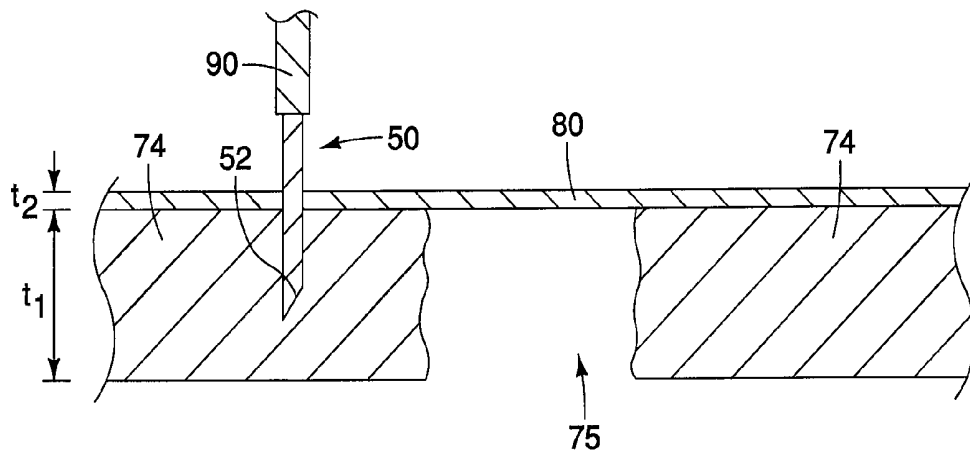


FIG. 3

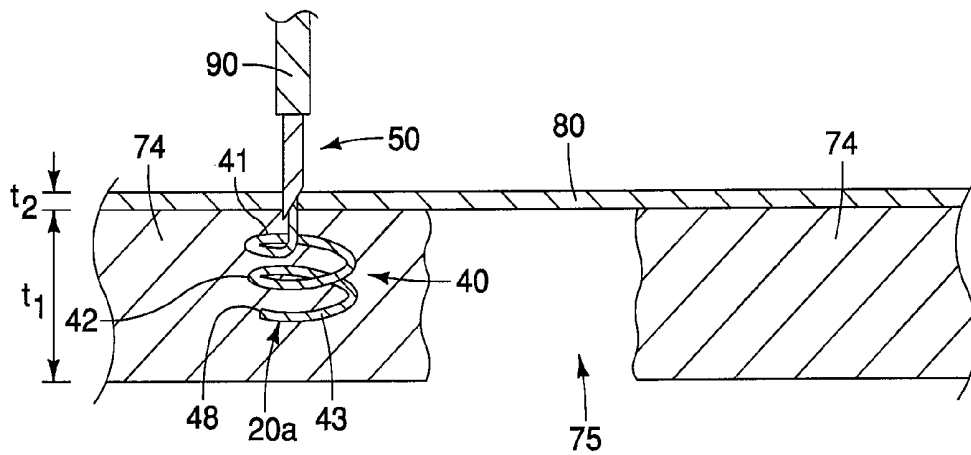


FIG. 4

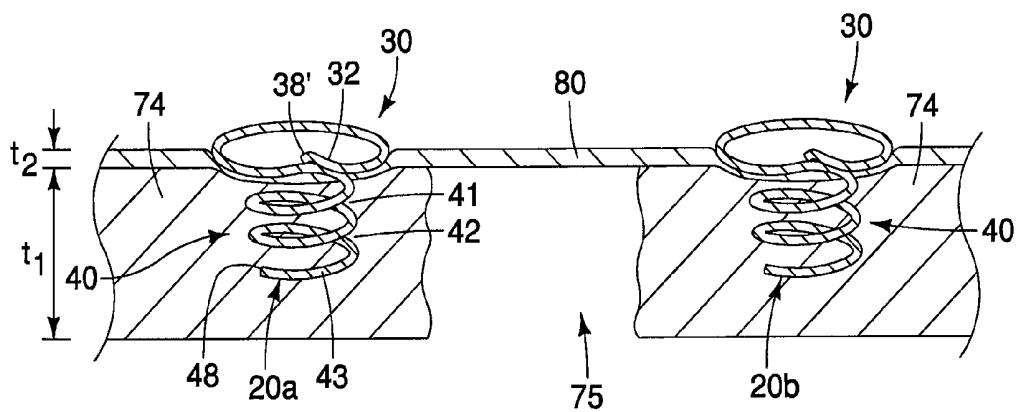


FIG. 5

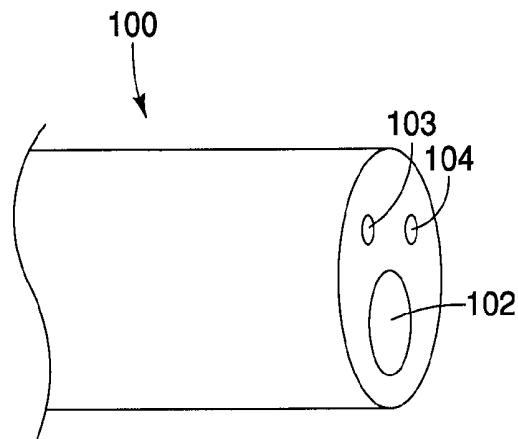


FIG. 6

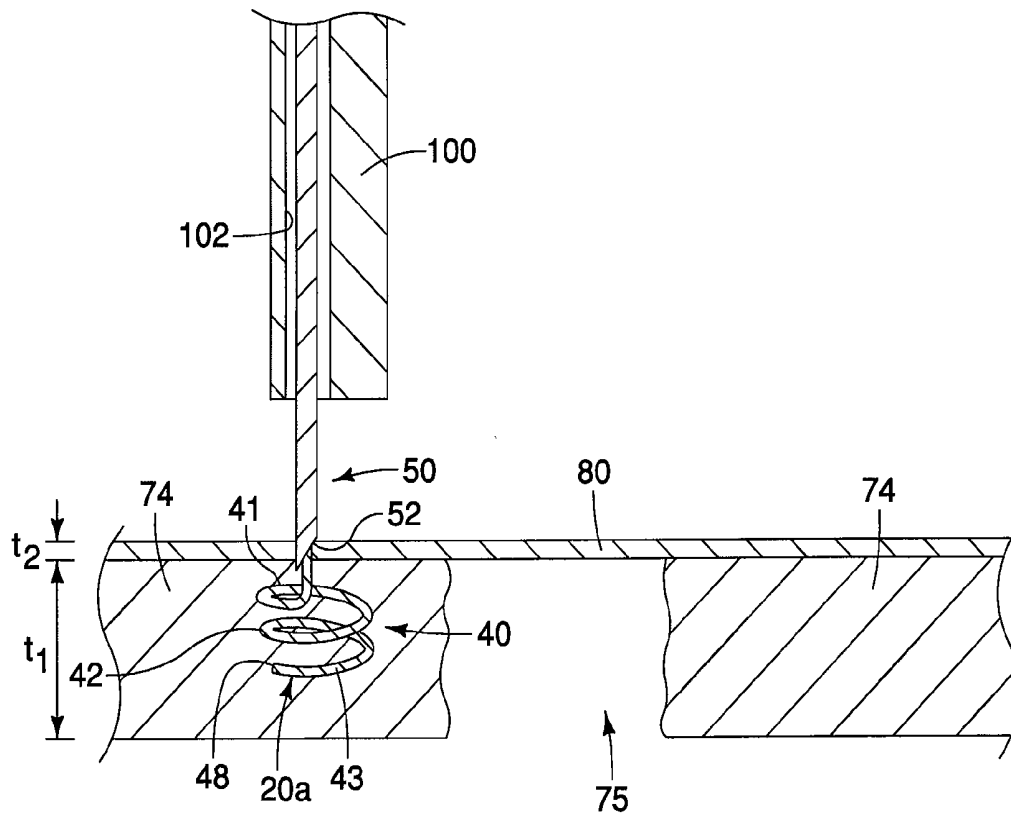


FIG. 7

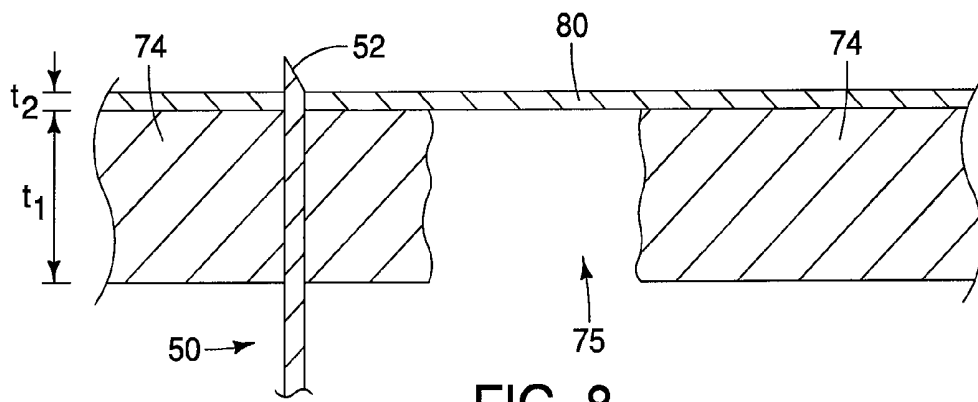


FIG. 8

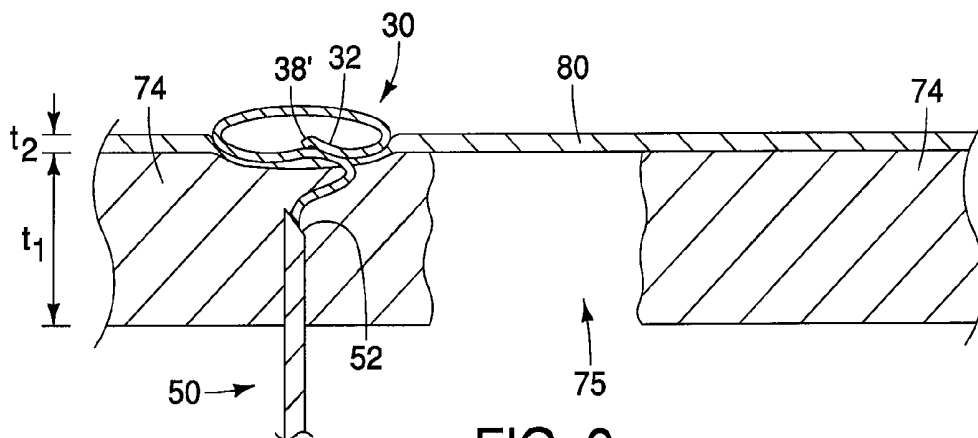


FIG. 9

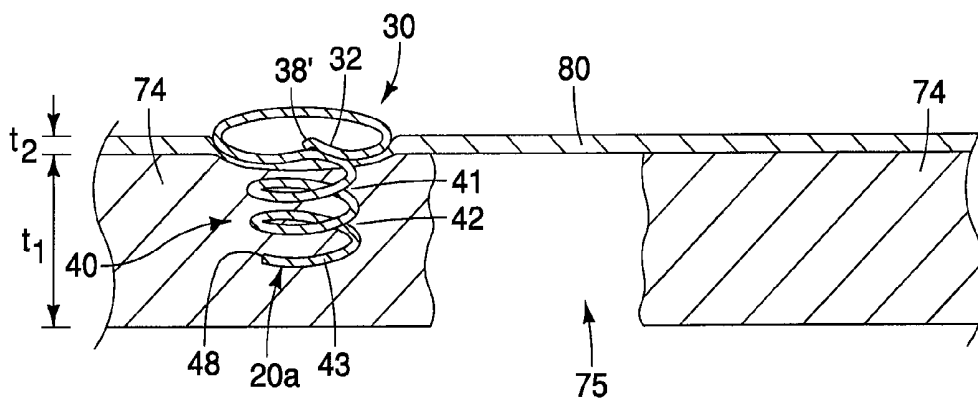


FIG. 10

TACKING DEVICE AND METHODS OF DEPLOYMENT**PRIORITY CLAIM**

This invention claims the benefit of priority of U.S. Provisional Application Ser. No. 61/181,946, entitled "Tacking Device and Methods of Deployment," filed May 28, 2009, the disclosure of which is hereby incorporated by reference in its entirety.

BACKGROUND

The present embodiments relate generally to medical devices, and more particularly, to apparatus and methods for coupling a graft member to tissue, closing a bodily opening, and the like.

Perforations in tissue or bodily walls may be formed intentionally or unintentionally. For example, an unintentional ventral abdominal hernia may be formed in the abdominal wall due to heavy lifting, coughing, strain imposed during a bowel movement or urination, fluid in the abdominal cavity, or other reasons. Intentional perforations may be formed, for example, during surgical procedures such as transluminal procedures. In a transluminal procedure, one or more instruments, such as an endoscope, may be inserted through a visceral wall, such as the stomach wall. During a transluminal procedure, a closure instrument may be used to close the perforation in the visceral wall. Depending on the structure comprising the perforation, it may be difficult to adequately close the perforation and prevent leakage of bodily fluids.

Attempts to seal perforations have been attempted by coupling a graft member to tissue. For example, during hernia repair, a graft material such as a mesh or patch may be disposed to cover the perforation. The graft material may completely overlap with the perforation, and the edges of the graft material may at least partially overlap with tissue surrounding the perforation. The graft material then may be secured to the surrounding tissue in an attempt to effectively cover and seal the perforation.

In order to secure the graft material to the surrounding tissue, sutures commonly are manually threaded through the full thickness of the surrounding tissue. In the case of a ventral abdominal hernia, the sutures may be threaded through the thickness of the abdominal wall, then tied down and knotted. However, such manual suturing techniques may be time consuming and/or difficult to perform.

In addition to covering and sealing perforations, there are various other instances in which it may be desirable to couple a graft material to tissue. For example, it may become necessary or desirable to couple the graft material to a region of tissue for purposes of reconstructing the local tissue. Whether a graft material is coupled to tissue to reconstruct local tissue, seal a perforation, or another purpose, it would be desirable to provide apparatus and methods for quickly and effectively coupling the graft material to the tissue.

Various tacking devices have been used to couple a graft to tissue during hernia procedures. Some of the tacking devices comprise spiral or threaded members. In some cases, a screwdriver may engage a head region of the tacking device to screw the tacking device into the tissue, or alternative, loosen its engagement with the tissue. However, such tacking devices comprise rigid members having a fixed profile, which therefore requires a relatively large delivery device and incision. Moreover, the inventor has discovered that tacking devices may permit slipping of the graft member relative to the tissue, and the head region may significantly protrude into

a body space and inadvertently snag on organs such as the intestines, causing surgical complications.

SUMMARY

The present embodiments provide a tacking device for engaging tissue, which may be useful for coupling a graft to tissue, facilitating closure of a bodily opening, and the like. In one embodiment, the tacking device comprises a wire having first and second ends, and further having delivery and deployed states. In the delivery state, the wire comprises an elongated configuration that is substantially parallel to a central longitudinal axis. In the deployed state, the wire comprises a head region and a body region, the head region comprising at least one full turn having a first diameter, and the body region comprising at least two full turns having a second diameter.

The first diameter of the full turn of the head region may be greater than the second diameter of the at least two full turns of the body region. Further, a longitudinal distance of the body region may be at least three times greater than a longitudinal distance of the head region. The wire of the tacking device may comprise a nickel-titanium alloy that is configured to self-expand from the delivery state to the deployed state.

A tacking device provided in accordance with the present embodiments may be used to treat an array of medical conditions. For example, when used to couple a graft member to tissue to treat a ventral hernia, the at least one full turn of the head region may abut the graft member, while the at least two full turns of the body region may engage the tissue.

The tacking device may be delivered within a hollow lumen of an insertion tool in the delivery state, and may be deployed using multiple techniques. For example, a laparoscopic delivery technique may be used in which the insertion tool is advanced through a laparoscopic device and the body region of the wire is deployed prior to the head region. Alternatively, an endoscopic delivery technique may be used in which the insertion tool is advanced through a lumen of an endoscope and the body region of the wire is deployed prior to the head region. Still further, a percutaneous delivery technique may be used in which the insertion tool is advanced directly through abdominal skin and the head region of the wire is deployed prior to the body region. In any of the above techniques, multiple tacking devices may be loaded in a sequential manner within the hollow lumen of the insertion tool, and then sequentially deployed to secure the graft member to the tissue at multiple different locations.

Advantageously, in the deployed state, the design of the head region of the tacking device may reduce the risk of complications such as inadvertent snagging on the intestines. Moreover, the enlarged diameter of the head region may reduce the likelihood of the graft member slipping off the tacking device and away from the tissue. Still further, since the tacking device can be delivered as an elongated wire in the delivery state, the profile of the insertion tool and bodily incision may be reduced.

Other systems, methods, features and advantages of the invention will be, or will become, apparent to one with skill in the art upon examination of the following figures and detailed description. It is intended that all such additional systems, methods, features and advantages be within the scope of the invention, and be encompassed by the following claims.

BRIEF DESCRIPTION OF THE DRAWINGS

The invention can be better understood with reference to the following drawings and description. The components in

the figures are not necessarily to scale, emphasis instead being placed upon illustrating the principles of the invention. Moreover, in the figures, like referenced numerals designate corresponding parts throughout the different views.

FIGS. 1A-1B illustrate a side view of a tacking device from a slightly elevated perspective, and a top view, respectively.

FIG. 2 is a perspective, cut-away view illustrating multiple tacking devices in a delivery configuration within an insertion tool.

FIGS. 3-5 are side-sectional views illustrating an exemplary laparoscopic deployment of one or more of the tacking devices of FIGS. 1-2 to treat a ventral hernia.

FIG. 6 is a perspective view of the distal region of an exemplary end-viewing endoscope.

FIG. 7 is a side-sectional view illustrating an endoscopic approach for treatment of a ventral hernia using one or more of the tacking devices of FIGS. 1-2.

FIGS. 8-10 are side-sectional views illustrating a percutaneous deployment of one or more of the tacking devices of FIGS. 1-2 to treat a ventral hernia.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

In the present application, the term “proximal” refers to a direction that is generally towards a physician during a medical procedure, while the term “distal” refers to a direction that is generally towards a target site within a patient’s anatomy during a medical procedure. Thus, “proximal” and “distal” portions of a device or bodily region may depend on the point of entry for the procedure (e.g., percutaneously versus endoscopically).

Referring now to FIGS. 1A-1B, a first embodiment of a tacking device 20 is shown in a deployed or expanded state. The tacking device 20 comprises a single wire 21 having first and second ends 38 and 48. As used herein, the term “wire” refers to a generally wire-like member, and is not limited to a metal member, but rather may include plastic or any other material. In the expanded state of FIGS. 1A-1B, the wire 21 comprises a head region 30 and a body region 40, and has a series of turns through both regions, as described in further detail below. For reference purposes, the tacking device 20 has a central longitudinal axis C, as illustrated in FIGS. 1-2.

The head region 30 generally extends from the first end 38 towards a junction 35, which separates the head region 30 from the body region 40. The first end 38 may be positioned such that it intersects with, or is adjacent to, the central longitudinal axis C, and may transition into a substantially straight segment 32 that extends in a radially outward direction away from the central longitudinal axis C. The substantially straight segment 32 then transitions into a curved segment 33, which preferably spans at least 360 degrees and terminates at the junction 35, as depicted in FIGS. 1A-1B.

The junction 35 may comprise a single point, or may comprise a short straight segment delineating a transition between the first and second regions 30 and 40. The junction 35 may effectively change the direction of curvature of the wire 21. For example, as shown in FIGS. 1A-1B, while the wire 21 extends in a generally counterclockwise direction through the head region 30, the junction 35 changes the direction so that the wire 21 extends in a clockwise direction through the body region 40.

In the exemplary embodiment of FIGS. 1A-1B, the curved segment 33 spans about 450 degrees, i.e., one full counterclockwise turn of 360 degrees, plus 90 additional degrees. More particularly, as shown in FIGS. 1A-1B, there is a portion 34 along the curved segment 33 that is parallel to the

substantially straight segment 32, thereby indicating a curvature of 360 degrees, and the wire 21 further extends about another 90 degrees from the portion 34 to the junction 35. Accordingly, in this example, the junction 35 is oriented approximately orthogonal to the substantially straight segment 32, as depicted in FIGS. 1A-1B. The junction 35 may extend laterally in a direction that intersects with, or nearly coincides with, a line defined by the central longitudinal axis C. The junction 35 therefore may be longitudinally and/or radially offset from the first end 38 of the wire 21, so that the junction 35 does not interfere with the first end 38 in the expanded state.

The curved segment 33, while not necessarily forming a perfectly enclosed circle, comprises a diameter D_1 , which may be defined as the maximum straight line extension away from the central longitudinal axis C, as depicted in FIGS. 1A-1B. As will be explained in further detail below, an increased diameter D_1 may enhance an engagement between the head region 30 and a graft member covering a perforation in tissue to thereby reduce the likelihood of the graft member slipping off the tacking device 20 and away from the tissue.

While the curved segment 33 is shown spanning approximately 450 degrees, the curved segment 33 may span a shorter or greater length. For example, the curved segment may extend in a counterclockwise direction through at least two full turns of 360 degrees or more. It may be noted, however, that by utilizing fewer than two full turns, a longitudinal distance L_1 of the head region 30 may be reduced, which advantageously may reduce protrusion of the head region 30 into the peritoneum during treatment of a ventral hernia, as explained further below.

Referring still to FIG. 1A, the body region 40 generally extends from the junction 35 towards the second end 48. As noted above, the junction 35 may change the direction of the wire to cause the body region 40 to extend in a clockwise direction. In the exemplary embodiment of FIG. 1A, the body region 40 comprises at least two full turns 41 and 42, each of which span 360 degrees. A partial turn 43 of less than 360 degrees extends between the full turn 42 and the second end 48 of the wire 21. However, the body region 40 may span two full turns or less, or alternatively, three full turns or more. Notably, the diameter D_2 of the turns 41 and 42 of the body region 40 is smaller than the diameter D_1 of the head region 30. The ratio of the diameter D_1 to the diameter D_2 may be about 2 to 1, although an increased or reduced ratio may be provided.

In the embodiment shown, the body region 40 defines a cylindrical shape in the deployed state in which the diameter D_2 of each of the turns is approximately equal. However, in an alternative embodiment, the diameter of the turn 41 may be larger than the diameter of the turn 42, such that the body region 40 tapers in a screw-like manner.

The at least two full turns 41 and 42 of the body region 40 rotate around the central longitudinal axis C, forming an interior space 49 therein, as shown in FIG. 1B. A portion of the head region 30 also rotates around the interior space 49, as shown in FIG. 1B. The junction 35 may extend through the interior space 49, longitudinally between the first and second regions 30 and 40, to effectively change the direction of curvature of the wire 21.

Based in part on the number of turns, as well as the diameter D_2 of the turns, the body region 40 spans a longitudinal distance L_2 , as depicted in FIG. 1A. The number of full turns may be selected based on the particular medical application. For example, during treatment of a ventral hernia, the number of turns along the body region 40 may be selected such that the body region 40 is disposed substantially within abdominal

5

tissue, as explained further below. Moreover, the longitudinal distances L_1 and L_2 , accounting for the entire longitudinal length of the tacking device **20**, may be dimensioned to be substantially equal to or less than the combined thickness t_1 and t_2 of a tissue **74** and a graft member **80**, respectively, as shown in the examples below.

In a preferred embodiment, the longitudinal distance L_2 of the body region **40** is at least three times greater than the longitudinal distance L_1 of the head region **30**. However, the longitudinal distance L_2 may range from about 1.5 to about 10.0 times greater than the longitudinal distance L_1 . Advantageously, a relatively short longitudinal distance L_1 of the head region **30** may reduce protrusion of the tacking device **20** into a body space such as the peritoneum, while a relatively long longitudinal distance L_2 of the body region **40** may increase engagement with the tissue **74**.

In addition to the expanded deployed state shown in FIGS. 1A-1B, the tacking device **20** comprises a contracted or delivery state, as shown in FIG. 2. In a preferred embodiment, the wire **21** of the tacking device **20** comprises a shape-memory material, such as a nickel-titanium alloy (nitinol). If a shape-memory material such as nitinol is employed, the wire **21** may be manufactured such that it can assume the preconfigured expanded state shown in FIGS. 1A-1B upon application of a certain cold or hot medium. More specifically, a shape-memory material may undergo a substantially reversible phase transformation that allows it to "remember" and return to a previous shape or configuration. For example, in the case of nitinol, a transformation between an austenitic phase and a martensitic phase may occur by cooling and/or heating (shape memory effect) or by isothermally applying and/or removing stress (superelastic effect). Austenite is characteristically the stronger phase and martensite is the more easily deformable phase.

In an example of the shape-memory effect, a nickel-titanium alloy having an initial configuration in the austenitic phase may be cooled below a transformation temperature (M_f) to the martensitic phase and then deformed to a second configuration. Upon heating to another transformation temperature (A_f), the material may spontaneously return to its initial, predetermined configuration, as shown in FIGS. 1A-1B. Generally, the memory effect is one-way, which means that the spontaneous change from one configuration to another occurs only upon heating. However, it is possible to obtain a two-way shape memory effect, in which a shape memory material spontaneously changes shape upon cooling as well as upon heating.

Alternatively, the wire **21** may be made from other metals and alloys that are biased, such that they may be restrained prior to deployment, but are inclined to return to their relaxed, expanded configuration upon deployment. Solely by way of example, the wire **21** may comprise other materials such as stainless steel, cobalt-chrome alloys, amorphous metals, tantalum, platinum, gold and titanium, or may be made from non-metallic materials, such as thermoplastics and other polymers.

As shown in FIG. 2, the wire **21** of the tacking device **20** comprises an elongated configuration in the contracted state, i.e., the wire **21** is oriented along the central longitudinal axis C. In this state, one or more tacking devices **20** may be delivered to a target site in a patient's anatomy using an insertion tool **50**. In one embodiment, the insertion tool **50** is capable of carrying multiple different tacking devices, such as first and second tacking devices **20a** and **20b**, as shown in FIG. 2 and described below.

In one embodiment, the insertion tool **50** comprises a needle-like body having a sharpened distal tip **52** and a hollow

6

lumen **54**. The insertion tool **50** may be manufactured from stainless steel or any other suitable material, and may comprise an endoscopic ultrasound (EUS), or echogenic, needle. Solely by way of example, the insertion tool **50** may comprise the EchoTip® Ultrasound Needle, or the EchoTip® Ultra Endoscopic Ultrasound Needle, both manufactured by Cook Endoscopy of Winston-Salem, N.C.

The hollow lumen **54** of the insertion tool **50** may comprise an inner diameter that is larger than an outer diameter of the wire **21** forming the tacking devices. Therefore, the first and second tacking devices **20a** and **20b** may be loaded into the hollow lumen **54** of the insertion tool **50** in a sequential manner, as shown in FIG. 2. The direction of loading of the wires **21** is important and may be determined based on the procedure and associated entry point, e.g., laparoscopic versus percutaneous, as described greater below. In FIG. 2, the loading of the first and second tacking devices **20a** and **20b** is suitable for a laparoscopic or endoscopic procedure, wherein the body region **40** is deployed prior to the head region **30**. Accordingly, the second end **48** of the first tacking device **20a** may be closest to the sharpened distal tip **52** of the insertion tool **50**, while the first end **38** of the first tacking device **20a** may abut the second end **48** of the second tacking device **20b**, as depicted in FIG. 2.

A stylet **60** may be disposed for longitudinal movement within the hollow lumen **52** of the insertion tool **50**, as shown in FIG. 2. The stylet **60** may comprise stainless steel or any other suitable material. The stylet **60** is disposed proximal to the second, or final, tacking device **20b**. During use, the insertion tool **50** may be proximally retracted, while the stylet **60** may be held longitudinally steady, to facilitate sequential deployment of the first and second tacking devices **20a** and **20b**, as explained further below.

The insertion tool **50** may comprise one or more markers **56**, as shown in FIG. 2, which may be disposed near the distal end of the insertion tool **50**. The markers **56** may be configured to be visualized under fluoroscopy or other imaging techniques to facilitate location of the distal end of the insertion tool, for example, so that a physician may determine how far the insertion tool **50** has penetrated into tissue **74**, as depicted in FIG. 3 below. As will be explained further below, the insertion tool **50** may be used in conjunction with another device, such as a laparoscopic device or an endoscope.

The dimensions of the tacking device **20** may be tailored based on a particular surgical procedure, a particular patient's anatomy and/or other factors. Advantageously, since the tacking device **20** can be delivered as an elongated wire prior to deployment into the shape of FIGS. 1A-1B, the overall profile of the insertion tool may be reduced, which may result in a smaller incision.

Referring now to FIGS. 3-5, one or more tacking devices **20** described above may be used to facilitate treatment of a perforation **75** using a graft member **80**. In the example shown, the perforation **75** is a ventral hernia located in the tissue **74** of the abdominal wall. While treatment of a ventral hernia is shown for illustrative purposes, it will be apparent that the tacking devices described herein may be used in a wide range of medical procedures, including but not limited to any exemplary procedures described herein.

The initial stages of the ventral hernia repair may be performed using techniques that are known. In the example of FIGS. 3-5, a laparoscopic technique is employed whereby multiple relatively small incisions are made to access the hernia site. A first laparoscopic device (not shown) may be used to visualize the peritoneum, while a second laparoscopic device **90** may be used to deliver the insertion tool **50**.

The graft member **80** may comprise any suitable material for covering the perforation **75** and substantially or entirely inhibiting the protrusion of abdominal matter. In one embodiment, the graft member **80** may comprise small intestinal submucosa (SIS), such as SURGISIS® BIODESIGN™ Soft Tissue Graft, available from Cook Biotech, Inc., West Lafayette, Ind., which provides smart tissue remodeling through its three-dimensional extracellular matrix (ECM) that is colonized by host tissue cells and blood vessels, and provides a scaffold for connective and epithelial tissue growth and differentiation along with the ECM components. Preferably, the graft member **80** would be a one to four layer lyophilized soft tissue graft made from any number of tissue engineered products. Reconstituted or naturally-derived collagenous materials can be used, and such materials that are at least bioresorbable will provide an advantage, with materials that are bioremodelable and promote cellular invasion and ingrowth providing particular advantage. Suitable bioremodelable materials can be provided by collagenous ECMs possessing biotropic properties, including in certain forms angiogenic collagenous extracellular matrix materials. For example, suitable collagenous materials include ECMs such as submucosa, renal capsule membrane, dermal collagen, dura mater, pericardium, fascia lata, serosa, peritoneum or basement membrane layers, including liver basement membrane. Suitable submucosa materials for these purposes include, for instance, intestinal submucosa, including small intestinal submucosa, stomach submucosa, urinary bladder submucosa, and uterine submucosa. The graft member **80** may also comprise a composite of a biomaterial and a biodegradable polymer. Additional details may be found in U.S. Pat. No. 6,206,931 to Cook et al., the disclosure of which is incorporated herein by reference in its entirety.

Referring now to FIG. 3, after the graft member **80** has been placed to cover the perforation **75** using known techniques, the laparoscopic device **90** may be maneuvered into a desired position within the peritoneum. The distal end of the laparoscopic device **90** may be positioned facing the graft member **80**, as shown in FIG. 3. In a next step, the insertion tool **50** may be advanced distally through a lumen of the laparoscopic device **90** to pierce through the graft member **80**, and further may pierce at least partially into the tissue **74** at a first location around the perimeter of the perforation **75**.

In this example, the insertion tool **50** is carrying two sequential tacking devices **20a** and **20b**, which may be disposed within the hollow lumen **54** of the insertion tool **50** as shown in FIG. 2 above. With the tacking devices **20a** and **20b** in the contracted delivery states, the sharpened tip **52** of the insertion tool **50** may be advanced to a predetermined depth into the tissue **74**. The markers **56** of FIG. 2 may facilitate in determining how far the insertion tool **50** has penetrated into the tissue **74**.

In a next step, the stylet **60** of FIG. 2 may be held steady with respect to the insertion tool **50**, while the insertion tool **50** is retracted in a proximal direction, i.e., away from the tissue **74** and towards the peritoneum. This causes the second end **48** of the most distal tacking device **20a** to extend distal to the sharpened tip **52** of the insertion tool **50**, and causes a progressive deployment of the partial turn **43**, followed by the second full turn **42** and the first full turn **41** of the body region **40**, as depicted in FIG. 4. When the body region **40** of the wire **21** is no longer radially constrained by the insertion tool **50**, the partial turn **43** and full turns **41** and **42** may assume their predetermined expanded configurations in which they may engage the tissue **74**. Preferably, the partial turn **43** and full turns **41** and **42** become embedded or interwoven with the

tissue **74**, e.g., the tissue may fill the open spaced between the turns of the wire **21**, thereby securing the body region **40** within the tissue **74**.

As the insertion tool **50** further is retracted proximally with respect to the first tacking device **20a**, the head region **30** may assume its predetermined expanded configuration when no longer radially constrained, as shown in FIG. 5. In the expanded configuration, the head region **30** may engage or abut the graft member **80**. In this manner, the tacking device **20a** helps secure the graft material **80** against the tissue **74**.

In an alternative deployment technique, the stylet **60** may be distally advanced, while the insertion tool **50** is held steady, to distally advance the first tacking device **20a** relative to the insertion tool **50**. Still further, the stylet **60** may be distally advanced while the insertion tool **50** is proximally retracted to deploy the first tacking device **20a**. Using either technique, the tacking device **20a** itself may be visualized using a desired modality, such as fluoroscopy, and in particular the junction **35**.

After the first tacking device **20a** has been deployed, the insertion tool **50** may be repositioned to deploy the second tacking device **20b** around the perimeter of the perforation **75**. The second tacking device **20b** may be deployed in the same manner as the first tacking device **20a**. In this manner, multiple tacking devices may secure the graft member **80** around the perimeter of the perforation **75**, as shown in FIG. 5. As will be apparent, greater than two tacking devices may be used, and the positioning of the tacking devices may be varied to optimize securing the graft member **80** to the tissue **74** in order to substantially seal the perforation **75**.

Advantageously, since the longitudinal distance L_1 of the head region **30** is relatively small, the head region **30** provides a relatively flat surface that may reduce protrusion of the tacking devices **20** into the peritoneum, as depicted in FIG. 5. Moreover, the head region **30** does not comprise any substantially sharp surfaces that can inadvertently snag on, or pierce through, bodily organs such as the intestines. If desired, an alternative first end **38'** of the head region **30** may be bent inward, i.e., towards the tissue **74** and the second end **48**, as shown in FIG. 5, to further reduce complications such as inadvertent snagging of the tacking device **20**. Further, the enlarged diameter D_1 of the head region **30** provides an enhanced surface contact with the graft member **80**, which may reduce the likelihood of the graft member **80** falling off the tacking device **20** and slipping away from the tissue **74**.

Optionally, the laparoscopic device **90** may be periodically pushed distally to abut the graft member **80** as the insertion tool **50** is retracted proximally to deploy the head region **30**. This technique may help ensure that the head region **30** is deployed entirely proximal to the graft member **80**, thereby sandwiching the graft member **80** between the head region **30** and the body region **40**. Alternatively, a blunt outer sheath may be advanced over the insertion tool **50**, via the annular space between the laparoscopic device **90** and the insertion tool **50**, to push against the tissue **74** as needed during deployment.

In a further alternative embodiment, where multiple tacking devices **20a** and **20b** are sequentially positioned around the perforation **75** in a semi-annular or annular shape, a suture may be disposed between the multiple tacking devices. For example, the suture may be looped under or around the head regions **30** of the first and second tacking devices **20a** and **20b**, with first and second ends of the suture being capable of manipulation by a physician. The first and second ends of the suture then may be tensioned in a purse-string manner to reduce the distance between the tacking devices and compress the tissue **74** around the perforation **75**. The suture ends

may be secured to maintain the compression of the tissue **74** using any suitable technique such as by forming a knot or using clamps, rivets and the like.

Referring now to FIGS. 6-7, an endoscopic approach for treatment of a ventral hernia is described. The endoscopic approach is similar to the laparoscopic approach described in FIGS. 3-5 above, however, an endoscope **100** is used instead of the laparoscopic devices, and no visible incisions may be made on the skin of the patient. In particular, the endoscope **100** may be advanced through a bodily lumen such as the alimentary canal, with an access hole being created through the alimentary canal, to obtain peritoneal access to the ventral hernia, as depicted in FIG. 7.

One or more components, such as the insertion tool **50**, may be advanced through a working lumen **102** of the endoscope. The distal end of the insertion tool **50** may be viewed via optical elements **103** and **104** of the endoscope **100**, which may comprise fiber optic components for illuminating and capturing an image distal to the endoscope **100**. Under suitable visualization using a light source and an eyepiece, a physician may deploy multiple tacking devices one at one time using the insertion tool **50**.

If this endoscopic approach is employed, the insertion tool **50** may carry additional tacking devices **20** to subsequently close the access hole in the alimentary canal. Specifically, a first set of multiple tacking devices **20** may be used to secure the graft member **80** to the tissue **74**, as described in detail in FIGS. 3-5 above, and then a second set of multiple tacking devices **20** may be used to facilitate closure of the access opening in the alimentary canal, with or without use of a graft member. It should be noted that while only one specific endoscopic deployment step is shown in FIG. 7, the other steps are shown and described in FIGS. 3-5 above, and the final deployment of the tacking devices **20a** and **20b** using an endoscopic approach will be substantially the same as depicted in FIG. 5 above.

Referring now to FIGS. 8-10, a percutaneous approach for treatment of a ventral hernia is described. The percutaneous approach is similar to the laparoscopic approach described in FIGS. 3-5 above, but with some notable differences. First, in the percutaneous technique, then insertion tool **50** is advanced in a direction from the abdominal tissue **74** towards the graft member **80**. Accordingly, the head region **30** is deployed prior to the body region **40**, as explained below. Further, the insertion tool **50** may be advanced directly through a patient's abdominal skin.

If a percutaneous approach is used, the tacking devices **20** must be loaded in an opposite direction within the insertion tool **50**, relative to loading for the laparoscopic and endoscopic approaches described above. More particularly, referring to FIG. 2 above, in a percutaneous approach the first end **38** of the head region **30** of the first tacking device **20a** would be located closest to the sharpened tip **52** of the needle. Further, the second end **48** of the first tacking device **20a** would abut the first end **38** of the second tacking device **20b**, and the stylet **60** would abut the second end **48** of the second tacking device **20b**.

With the components loaded as described, the insertion tool **50** then is advanced directly through a patient's abdominal skin, through the tissue **74**, and may be advanced just distal to the graft member **80** into the peritoneum, as shown in FIG. 8. In order to optimally visualize the insertion tool **50**, a laparoscopic viewing device may be positioned in the peritoneum, or an endoscope may be transluminally advanced in proximity to the target site, as noted in the embodiments

above. Alternatively, the insertion tool **50**, and markers **56** in particular, may be viewed using fluoroscopy of other suitable techniques.

In a next step, the stylet **60** of FIG. 2 may be held steady with respect to the insertion tool **50**, while the insertion tool **50** is retracted in a proximal direction, i.e., away from the peritoneum and towards the tissue **74**. This causes the first end **38** of the first tacking device **20a** to extend distal to the sharpened tip **52** of the insertion tool **50**, and causes the head region **30** to be deployed. By aligning the sharpened tip **52** of the insertion tool **50** with the graft member **80**, the head region **30** may be deployed into abutting contact with the graft member **80**, as shown in FIG. 9. As the insertion tool **50** further is retracted proximally with respect to the first tacking device **20a**, the first full turn **41** of the body region **40** is deployed, followed by the second full turn **42** and the partial turn **43**. As noted above, in the expanded state, the full turns **41** and **42** and the partial turn **43** may become embedded or interwoven with the tissue **74**, thereby securing the body region **40** into the tissue **74**. After the first tacking device **20a** has been deployed, the insertion tool **50** may be repositioned to deploy additional tacking devices around the perimeter of the perforation **75**, as generally described above.

As noted above, in an alternative embodiment, the diameter of the turn **41** may be larger than the diameter of the turn **42**, such that the body region **40** tapers in a screw-like manner. In a further alternative embodiment, there may be multiple relatively large diameter turns separated by multiple relatively small or intermediate diameter turns. For example, from the head region towards the body region, there may be a relatively large turn, followed by a relatively small turn, followed by a relatively large turn, followed by an intermediate turn, and followed by a relatively small turn. Several different such combinations of diameter turns are possible. Moreover, in yet a further alternative embodiment, the tacking device may comprise a uniform helical diameter throughout its entire longitudinal length.

While the exemplary embodiments herein have illustrated the use of one or more tacking devices **20** for covering a perforation **75** formed in the ventral abdominal wall, the tacking devices disclosed herein may be useful in many other procedures. Solely by way of example, one or more tacking devices **20** may be used to treat perforations in a visceral wall, such as the stomach wall. Further, the tacking devices **20** may be used to secure a graft member to tissue for reconstructing local tissue, and the like.

In yet further applications within the scope of the present embodiments, the tacking devices **20** need not be used for coupling a graft member to tissue. For example, the tacking devices **20** may be used in an anastomosis procedure. In order to create an anastomosis, for example, multiple tacking devices **20** may be deployed in a circular manner to couple a proximal vessel, duct or organ to a distal vessel, duct or organ. In such cases, a suitable insertion device, such as an endoscope, may be advanced through a bodily lumen such as the alimentary canal to a position proximate the target location. One or more components, such as the insertion tool **50**, may be advanced through a working lumen of the endoscope. The distal end of the insertion tool **50** may be viewed under fluoroscopy, or via optical elements of the endoscope, or by some other visualization technique. Under suitable visualization, multiple tacking devices then may be delivered at one time, for example, using the insertion tool **50**. Then, a hole may be punched through the middle of the deployed tacking devices to create a flow path between the proximal and distal vessels/ducts/organs.

11

It will be apparent that still further applications of the tacking devices **20** are possible. Finally, while exemplary laparoscopic, endoscopic and percutaneous delivery techniques have been described, it should be noted that one or more tacking devices **20** described herein may be deployed at a target site during an open medical procedure. 5

While various embodiments of the invention have been described, the invention is not to be restricted except in light of the attached claims and their equivalents. Moreover, the advantages described herein are not necessarily the only advantages of the invention and it is not necessarily expected that every embodiment of the invention will achieve all of the advantages described. 10

I claim:

1. A tacking device comprising:

a wire having first and second ends, and further having delivery and deployed states,

wherein, in the delivery state, the wire comprises an elongated configuration that is substantially parallel to a central longitudinal axis, 20

wherein, in the deployed state, the wire comprises a head region, a body region and a junction disposed therebetween, the head region comprising a curved portion substantially within a plane, a first diameter, and a substantially straight segment adjacent to the first end wherein

12

the first end is bent in a direction towards the second end and terminates adjacent to the plane in the deployed state, and the body region comprising at least two full turns having a second diameter,

wherein the first diameter is greater than the second diameter, wherein the junction changes a direction of curvature of the wire from clockwise to counterclockwise directions,

wherein a turn of the first diameter leads into the junction, and

wherein, in the deployed state, there is a curvature in one direction only along the head region, and the junction is substantially straight.

2. The tacking device of claim **1** wherein a longitudinal distance of the body region is at least three times greater than a longitudinal distance of the head region in the deployed state. 15

3. The tacking device of claim **1** wherein the first diameter is greater than the second diameter.

4. The tacking device of claim **1** wherein the head region curves between about 400 and 500 degrees total between the first end and the junction. 20

5. The tacking device of claim **1** wherein the curved portion comprises the first diameter and spans less than a full turn.

* * * * *

专利名称(译)	跟踪设备和部署方法		
公开(公告)号	US9345476	公开(公告)日	2016-05-24
申请号	US12/787744	申请日	2010-05-26
[标]申请(专利权)人(译)	SURTI VIHARÇ		
申请(专利权)人(译)	SURTI , VIHAR C.		
当前申请(专利权)人(译)	库克医疗技术有限责任公司		
[标]发明人	SURTI VIHAR C		
发明人	SURTI, VIHAR C.		
IPC分类号	A61B17/064 A61B17/00		
CPC分类号	A61B17/064 A61B2017/00862 A61B2017/00867 A61B2017/0649		
审查员(译)	MCEVOY , THOMAS		
优先权	61/181946 2009-05-28 US		
其他公开文献	US20100305591A1		
外部链接	USPTO		

摘要(译)

本实施例提供适合于将移植物构件联接到组织，闭合身体开口等的装置和方法。在一个实施例中，定位装置包括具有第一和第二端的线，并且还具有输送和展开状态。在收缩状态下，线材包括细长构造，该细长构造基本上平行于中心纵向轴线。在扩张状态下，导线包括头部区域和主体区域，头部区域包括至少一个具有第一直径的整圈，并且主体区域包括至少两个具有第二直径的整圈，其中第一直径是大于第二直径。可以使用腹腔镜，内窥镜或经皮方法递送一个或多个定位装置。

