



US009486341B2

(12) **United States Patent**
Shalev

(10) **Patent No.:** **US 9,486,341 B2**
(45) **Date of Patent:** **Nov. 8, 2016**

(54) **REDUCED-STRAIN EXTRA-VASCULAR
RING FOR TREATING AORTIC ANEURYSM**

(56) **References Cited**

U.S. PATENT DOCUMENTS

(75) Inventor: **Alon Shalev**, Ra'anana (IL)

4,355,426 A 10/1982 MacGregor
4,505,767 A 3/1985 Quin

(73) Assignee: **ENDOSPAN LTD.**, Herzilyia Pituach
(IL)

(Continued)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 378 days.

FOREIGN PATENT DOCUMENTS

CA 2 497 704 3/2004
EP 1 177 780 2/2002

(Continued)

(21) Appl. No.: **14/001,641**

(22) PCT Filed: **Mar. 1, 2012**

OTHER PUBLICATIONS

(86) PCT No.: **PCT/IL2012/000095**

§ 371 (c)(1),

(2), (4) Date: **Nov. 5, 2013**

Communication dated Nov. 10, 2014, issued by the European Patent
Office in counterpart Application No. 12752054.2.

(Continued)

(87) PCT Pub. No.: **WO2012/117395**

PCT Pub. Date: **Sep. 7, 2012**

Primary Examiner — Thomas McEvoy

(74) *Attorney, Agent, or Firm* — Sughrue Mion, PLLC

(65) **Prior Publication Data**

US 2014/0052236 A1 Feb. 20, 2014

Related U.S. Application Data

(60) Provisional application No. 61/448,199, filed on Mar.
2, 2011.

(51) **Int. Cl.**

A61F 2/93 (2013.01)

A61F 2/07 (2013.01)

(Continued)

(52) **U.S. Cl.**

CPC . **A61F 2/93** (2013.01); **A61F 2/07** (2013.01);
A61B 17/12013 (2013.01); **A61F 2/89**
(2013.01);

(Continued)

(58) **Field of Classification Search**

CPC **A61F 2/92**; **A61F 2/93**; **A61F 2/2409**;
A61F 2/07; **A61B 17/12013**


See application file for complete search history.

(57)

ABSTRACT

Apparatus (10) is provided that includes an extra-vascular
ring (12) and an endo vascular stent-graft (14). The ring (12)
comprises a structural member (30), which is configured to
assume an elongate hollow shape (32), which has first and
second longitudinal ends (40, 42), and is suitable for place-
ment at least partially around an aorta (20) so as to provide
a generally cylindrical landing zone. The endovascular
stent-graft (14) is suitable for endovascular placement inside
the aorta (20) such that a portion of the stent-graft (14) is
positioned against an internal wall of the aorta (20) at the
landing zone provided by the structural member (30). If the
structural member (30) is unrolled to a planar shape (82),
one side (90) of the planar shape (82) is defined by the first
longitudinal end (40), and at least the first longitudinal end
(40) has a profile that defines a series of curved portions and
has no singularities or discontinuities, which profile extends
along at least 50% of the first longitudinal end (40).

21 Claims, 10 Drawing Sheets

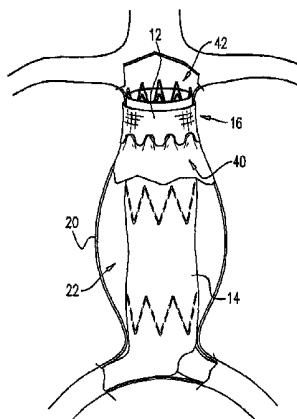

- (51) **Int. Cl.**
A61B 17/12 (2006.01)
A61F 2/89 (2013.01)
- (52) **U.S. Cl.**
 CPC .. *A61F 2220/005* (2013.01); *A61F 2220/0025*
 (2013.01); *A61F 2220/0041* (2013.01); *A61F*
2220/0066 (2013.01); *A61F 2220/0075*
 (2013.01); *A61F 2220/0083* (2013.01); *A61F*
2230/0054 (2013.01)
- (56) **References Cited**
 U.S. PATENT DOCUMENTS
- | | | | | | |
|-------------|---------|------------------|--------------|---------|----------------------|
| 4,562,596 A | 1/1986 | Kornberg | 6,077,298 A | 6/2000 | Tu et al. |
| 4,577,631 A | 3/1986 | Kreamer | 6,099,497 A | 8/2000 | Adams et al. |
| 4,617,932 A | 10/1986 | Kornberg | 6,117,145 A | 9/2000 | Wood et al. |
| 4,665,906 A | 5/1987 | Jervis | 6,152,956 A | 11/2000 | Pierce |
| 4,739,762 A | 4/1988 | Palmaz | 6,156,064 A | 12/2000 | Chouinard |
| 4,787,899 A | 11/1988 | Lazarus | 6,168,615 B1 | 1/2001 | Ken et al. |
| 4,816,339 A | 3/1989 | Tu et al. | 6,200,339 B1 | 3/2001 | Leschinsky et al. |
| 4,878,906 A | 11/1989 | Lindemann et al. | 6,206,893 B1 | 3/2001 | Klein et al. |
| 4,886,062 A | 12/1989 | Wiktor | 6,270,524 B1 | 8/2001 | Kim |
| 4,938,740 A | 7/1990 | Melbin | 6,283,991 B1 | 9/2001 | Cox et al. |
| 4,969,458 A | 11/1990 | Wiktor | 6,290,720 B1 | 9/2001 | Khosravi et al. |
| 5,042,707 A | 8/1991 | Taheri | 6,296,661 B1 | 10/2001 | Davila et al. |
| 5,064,435 A | 11/1991 | Porter | 6,312,458 B1 | 11/2001 | Golds |
| 5,104,404 A | 4/1992 | Wolff | 6,325,823 B1 | 12/2001 | Horzewski et al. |
| 5,122,136 A | 6/1992 | Guglielmi et al. | 6,344,056 B1 | 2/2002 | Dehdashtian |
| 5,133,732 A | 7/1992 | Wiktor | 6,406,420 B1 | 6/2002 | McCarthy |
| 5,234,448 A | 8/1993 | Wholey | 6,428,565 B1 | 8/2002 | Wisselink |
| 5,486,183 A | 1/1996 | Middleman et al. | 6,451,048 B1 | 9/2002 | Berg et al. |
| 5,507,769 A | 4/1996 | Marin et al. | 6,506,211 B1 | 1/2003 | Skubitz et al. |
| 5,509,923 A | 4/1996 | Middleman et al. | 6,565,597 B1 | 5/2003 | Fearnot et al. |
| 5,522,880 A | 6/1996 | Barone et al. | 6,613,078 B1 | 9/2003 | Barone |
| 5,527,322 A | 6/1996 | Klein et al. | 6,635,083 B1 | 10/2003 | Cheng et al. |
| 5,549,662 A | 8/1996 | Fordenbacher | 6,648,901 B2 | 11/2003 | Fleischman et al. |
| 5,554,181 A | 9/1996 | Das | 6,648,911 B1 | 11/2003 | Sirhan |
| 5,556,413 A | 9/1996 | Lam | 6,652,567 B1 | 11/2003 | Deaton |
| 5,562,724 A | 10/1996 | Vorwerk et al. | 6,656,214 B1 | 12/2003 | Fogarty et al. |
| 5,591,229 A | 1/1997 | Parodi | 6,692,520 B1 | 2/2004 | Gambale et al. |
| 5,607,445 A | 3/1997 | Summers | 6,695,833 B1 | 2/2004 | Frantzen |
| 5,613,974 A | 3/1997 | Andreas et al. | 6,730,117 B1 | 5/2004 | Tseng et al. |
| 5,632,746 A | 5/1997 | Middleman et al. | 6,743,195 B2 | 6/2004 | Zucker |
| 5,632,763 A | 5/1997 | Glastra | 6,748,953 B2 | 6/2004 | Sherry et al. |
| 5,632,772 A | 5/1997 | Alcime et al. | 6,752,826 B2 | 6/2004 | Holloway |
| 5,639,278 A | 6/1997 | Dereume et al. | 6,776,794 B1 | 8/2004 | Hong et al. |
| 5,643,340 A | 7/1997 | Nunokawa | 6,808,534 B1 | 10/2004 | Escano |
| 5,653,743 A | 8/1997 | Martin | 6,814,749 B2 | 11/2004 | Cox et al. |
| 5,676,696 A | 10/1997 | Marcade | 6,814,752 B1 | 11/2004 | Chuter |
| 5,676,697 A | 10/1997 | McDonald | 6,824,560 B2 | 11/2004 | Pelton |
| 5,728,134 A | 3/1998 | Barak | 6,846,321 B2 | 1/2005 | Zucker |
| 5,749,879 A | 5/1998 | Middleman et al. | 6,907,285 B2 | 6/2005 | Denker et al. |
| 5,755,770 A | 5/1998 | Ravenscroft | 6,908,477 B2 | 6/2005 | McGuckin, Jr. et al. |
| 5,755,771 A | 5/1998 | Penn et al. | 6,929,660 B1 | 8/2005 | Ainsworth et al. |
| 5,755,774 A | 5/1998 | Pinchuk | 6,942,691 B1 | 9/2005 | Chuter |
| 5,755,777 A | 5/1998 | Chuter | 6,953,469 B2 | 10/2005 | Ryan |
| 5,755,781 A | 5/1998 | Jayaraman | 6,964,679 B1 | 11/2005 | Marcade et al. |
| 5,769,882 A | 6/1998 | Fogarty et al. | 6,986,774 B2 | 1/2006 | Middleman et al. |
| 5,769,884 A | 6/1998 | Solovay | 7,008,441 B2 | 3/2006 | Zucker |
| 5,782,903 A | 7/1998 | Wiktor | 7,044,962 B2 | 5/2006 | Elliott |
| 5,782,906 A | 7/1998 | Marshall et al. | 7,105,020 B2 | 9/2006 | Greenberg et al. |
| 5,824,040 A | 10/1998 | Cox et al. | 7,112,217 B1 | 9/2006 | Kugler et al. |
| 5,827,321 A | 10/1998 | Roubin | 7,115,127 B2 | 10/2006 | Lindenbaum et al. |
| 5,843,170 A | 12/1998 | Ahn | 7,144,421 B2 | 12/2006 | Carpenter et al. |
| 5,855,600 A | 1/1999 | Alt | 7,201,772 B2 | 4/2007 | Schwammenthal et al. |
| 5,860,991 A | 1/1999 | Klein et al. | 7,223,266 B2 | 5/2007 | Lindenbaum et al. |
| 5,876,432 A | 3/1999 | Lau et al. | 7,261,733 B1 | 8/2007 | Brown et al. |
| 5,906,641 A | 5/1999 | Thompson et al. | 7,270,675 B2 | 9/2007 | Chun et al. |
| 5,921,994 A | 7/1999 | Andreas et al. | 7,279,003 B2 | 10/2007 | Berra et al. |
| 5,976,178 A | 11/1999 | Goldstein et al. | 7,294,147 B2 | 11/2007 | Hartley |
| 5,980,552 A | 11/1999 | Pinchasik | 7,306,623 B2 | 12/2007 | Watson |
| 6,015,431 A | 1/2000 | Thornton et al. | 7,341,598 B2 | 3/2008 | Davidson et al. |
| 6,016,810 A | 1/2000 | Ravenscroft | 7,399,313 B2 | 7/2008 | Brown et al. |
| 6,033,435 A | 3/2000 | Penn et al. | 7,407,509 B2 | 8/2008 | Greenberg et al. |
| 6,036,725 A | 3/2000 | Avellanet | 7,429,269 B2 | 9/2008 | Schwammenthal et al. |
| 6,059,824 A | 5/2000 | Taheri | 7,442,204 B2 | 10/2008 | Schwammenthal et al. |
| | | | 7,473,272 B2 | 1/2009 | Pryor |
| | | | 7,537,609 B2 | 5/2009 | Davidson et al. |
| | | | 7,540,881 B2 | 6/2009 | Meyer et al. |
| | | | 7,544,160 B2 | 6/2009 | Gross |
| | | | 7,616,997 B2 | 11/2009 | Kieval et al. |
| | | | 7,637,939 B2 | 12/2009 | Tischler |
| | | | 7,662,161 B2 | 2/2010 | Briganti et al. |
| | | | 7,662,168 B2 | 2/2010 | McGuckin, Jr. et al. |
| | | | 7,678,141 B2 | 3/2010 | Greenan et al. |
| | | | 7,708,704 B2 | 5/2010 | Mittelberg |
| | | | 7,722,626 B2 | 5/2010 | Middleman et al. |
| | | | 7,731,732 B2 | 6/2010 | Ken |
| | | | 7,803,178 B2 | 9/2010 | Whirley et al. |
| | | | 7,815,673 B2 | 10/2010 | Bloom et al. |
| | | | 7,887,575 B2 | 2/2011 | Kujawski |
| | | | 7,959,662 B2 | 6/2011 | Erbel et al. |

(56)

References Cited

U.S. PATENT DOCUMENTS

8,021,418 B2	9/2011	Gerberding et al.	2006/0069426 A1	3/2006	Weinberger
8,052,741 B2	11/2011	Bruszewski et al.	2006/0095104 A1	5/2006	Magers et al.
8,066,755 B2	11/2011	Zacharias et al.	2006/0100684 A1	5/2006	Elliott
8,080,026 B2	12/2011	Konstantino et al.	2006/0106406 A1	5/2006	Weinberger
8,080,053 B2	12/2011	Satasiya et al.	2006/0149360 A1	7/2006	Schwammenthal et al.
8,157,810 B2	4/2012	Case et al.	2006/0155358 A1	7/2006	LaDuca et al.
8,172,892 B2	5/2012	Chuter et al.	2006/0155366 A1	7/2006	LaDuca et al.
8,251,963 B2	8/2012	Chin et al.	2006/0167476 A1	7/2006	Burdulis, Jr. et al.
8,353,898 B2	1/2013	Lutze et al.	2006/0173530 A1	8/2006	Das
8,486,131 B2	7/2013	Shalev	2006/0193892 A1	8/2006	Furst et al.
2001/0004705 A1	6/2001	Killion et al.	2006/0229709 A1	10/2006	Morris et al.
2001/0010006 A1	7/2001	Bachinski et al.	2006/0241740 A1	10/2006	Vardi et al.
2001/0014823 A1	8/2001	Ressemann et al.	2006/0271166 A1	11/2006	Thill et al.
2001/0044651 A1	11/2001	Steinke et al.	2006/0281966 A1*	12/2006	Peacock A61B 17/12 600/37
2001/0044652 A1	11/2001	Moore	2007/0021822 A1	1/2007	Boatman
2001/0047198 A1	11/2001	Drasler et al.	2007/0043425 A1	2/2007	Hartley et al.
2001/0053930 A1	12/2001	Kugler et al.	2007/0050011 A1	3/2007	Klein
2002/0040236 A1	4/2002	Lau et al.	2007/0055350 A1	3/2007	Erickson et al.
2002/0099438 A1	7/2002	Fursty	2007/0055358 A1	3/2007	Krolik et al.
2002/0099441 A1	7/2002	Dehdashtian	2007/0060989 A1	3/2007	Deem et al.
2002/0107564 A1	8/2002	Cox et al.	2007/0061002 A1	3/2007	Paul, Jr. et al.
2002/0123791 A1	9/2002	Harrison	2007/0073373 A1	3/2007	Bonsignore
2002/0156495 A1	10/2002	Brenneman et al.	2007/0088425 A1	4/2007	Schaeffer
2003/0040791 A1	2/2003	Oktay	2007/0112344 A1	5/2007	Keilman
2003/0057156 A1	3/2003	Peterson et al.	2007/0135677 A1	6/2007	Miller et al.
2003/0068296 A1	4/2003	Ricci et al.	2007/0142896 A1	6/2007	Anderson et al.
2003/0093145 A1	5/2003	Lawrence-Brown et al.	2007/0150051 A1	6/2007	Arnault de la et al.
2003/0114061 A1	6/2003	Matsuda et al.	2007/0156167 A1	7/2007	Connors et al.
2003/0125796 A1	7/2003	Dong	2007/0167898 A1	7/2007	Peters et al.
2003/0130720 A1	7/2003	DePalma et al.	2007/0179598 A1	8/2007	Duerig
2003/0139802 A1	7/2003	Wulfman et al.	2007/0185565 A1	8/2007	Schwammenthal et al.
2003/0144725 A1	7/2003	Lombardi	2007/0208410 A1	9/2007	Berra et al.
2003/0153968 A1	8/2003	Geis et al.	2007/0213805 A1	9/2007	Schaeffer et al.
2003/0163187 A1	8/2003	Weber	2007/0213807 A1	9/2007	Roubin
2003/0191523 A1	10/2003	Hojeibane	2007/0219610 A1	9/2007	Israel
2003/0199967 A1	10/2003	Hartley et al.	2007/0219627 A1	9/2007	Chu
2003/0199968 A1	10/2003	Ainsworth et al.	2007/0233229 A1	10/2007	Berra et al.
2003/0204236 A1	10/2003	Letort	2007/0237973 A1	10/2007	Purdy et al.
2003/0212449 A1	11/2003	Cox	2007/0239256 A1	10/2007	Weber et al.
2003/0236567 A1	12/2003	Elliot	2007/0244542 A1	10/2007	Greenan et al.
2004/0015227 A1	1/2004	Vardi et al.	2007/0244543 A1	10/2007	Mitchell
2004/0015229 A1	1/2004	Fulkerson	2007/0244547 A1	10/2007	Greenan
2004/0098091 A1	5/2004	Erbel et al.	2007/0250154 A1	10/2007	Greenberg
2004/0106972 A1	6/2004	Deaton	2007/0255388 A1	11/2007	Rudakov et al.
2004/0106978 A1	6/2004	Greenberg et al.	2008/0002871 A1	1/2008	Gunzert-Marx et al.
2004/0133266 A1	7/2004	Clerc et al.	2008/0015673 A1	1/2008	Chuter
2004/0171978 A1	9/2004	Shalaby	2008/0033527 A1	2/2008	Nunez et al.
2004/0176832 A1	9/2004	Hartley et al.	2008/0058918 A1	3/2008	Watson
2004/0181149 A1	9/2004	Langlotz et al.	2008/0064957 A1	3/2008	Spence
2004/0215319 A1	10/2004	Berra et al.	2008/0086193 A1	4/2008	Thramann
2004/0215327 A1	10/2004	Doig et al.	2008/0109066 A1	5/2008	Quinn
2005/0033406 A1	2/2005	Barnhart et al.	2008/0114445 A1	5/2008	Melsheimer et al.
2005/0049678 A1	3/2005	Cocks et al.	2008/0147173 A1	6/2008	McIlff et al.
2005/0065545 A1	3/2005	Wallace	2008/0167704 A1	7/2008	Wright et al.
2005/0070995 A1	3/2005	Zilla et al.	2008/0176271 A1	7/2008	Silver et al.
2005/0085900 A1	4/2005	Case et al.	2008/0195190 A1	8/2008	Bland et al.
2005/0102018 A1	5/2005	Carpenter et al.	2008/0195191 A1	8/2008	Luo
2005/0102021 A1	5/2005	Osborne	2008/0215134 A1	9/2008	Lawrence-Brown
2005/0131517 A1	6/2005	Hartley et al.	2008/0269789 A1	10/2008	Eli
2005/0143802 A1	6/2005	Soykan et al.	2008/0275540 A1	11/2008	Wen
2005/0149166 A1	7/2005	Schaeffer et al.	2008/0275542 A1	11/2008	LaDuca et al.
2005/0154448 A1	7/2005	Cully et al.	2008/0288044 A1	11/2008	Osborne
2005/0171598 A1	8/2005	Schaeffer et al.	2008/0300665 A1	12/2008	Lootz et al.
2005/0177132 A1	8/2005	Lentz et al.	2008/0319528 A1	12/2008	Yribarren et al.
2005/0203606 A1	9/2005	VanCamp	2009/0012597 A1	1/2009	Doig et al.
2005/0216018 A1	9/2005	Sennett et al.	2009/0012602 A1	1/2009	Quadri
2005/0222649 A1	10/2005	Capuano et al.	2009/0030502 A1	1/2009	Sun et al.
2005/0222667 A1	10/2005	Hunt	2009/0048663 A1	2/2009	Greenberg
2005/0222668 A1	10/2005	Schaeffer et al.	2009/0054967 A1	2/2009	Das
2005/0222669 A1	10/2005	Purdy	2009/0069881 A1	3/2009	Chalekian et al.
2005/0234542 A1	10/2005	Melsheimer	2009/0069882 A1	3/2009	Venturelli
2005/0266042 A1	12/2005	Tseng	2009/0082841 A1	3/2009	Zacharias et al.
2005/0283188 A1	12/2005	Loshakove et al.	2009/0099648 A1	4/2009	Yu
2006/0015170 A1	1/2006	Jones et al.	2009/0099649 A1	4/2009	Chobotov et al.
2006/0052799 A1	3/2006	Middleman et al.	2009/0105809 A1	4/2009	Lee et al.
			2009/0112233 A1	4/2009	Xiao
			2009/0125096 A1	5/2009	Chu et al.
			2009/0138067 A1	5/2009	Pinchuk et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2009/0149877 A1 6/2009 Hanson et al.
 2009/0164001 A1 6/2009 Biggs et al.
 2009/0227997 A1 9/2009 Wang et al.
 2009/0240316 A1 9/2009 Bruszewski
 2009/0248134 A1 10/2009 Dierking et al.
 2009/0254170 A1 10/2009 Hartley et al.
 2009/0259290 A1 10/2009 Bruszewski et al.
 2009/0287145 A1 11/2009 Cragg et al.
 2010/0004728 A1 1/2010 Rao et al.
 2010/0029608 A1 2/2010 Finley et al.
 2010/0063575 A1 3/2010 Shalev
 2010/0070019 A1 3/2010 Shalev
 2010/0161026 A1 6/2010 Bocker et al.
 2010/0211159 A1 8/2010 Schmid et al.
 2010/0256725 A1 10/2010 Rasmussen
 2010/0274345 A1 10/2010 Rust
 2010/0292774 A1 11/2010 Shalev
 2011/0022149 A1 1/2011 Cox et al.
 2011/0093002 A1 4/2011 Rucker et al.
 2011/0125251 A1 5/2011 Cottone
 2011/0208289 A1 8/2011 Shalev
 2011/0208296 A1 8/2011 Duffy et al.
 2011/0208297 A1 8/2011 Tuval et al.
 2011/0208298 A1 8/2011 Tuval et al.
 2011/0218607 A1 9/2011 Arbefeulle et al.
 2011/0257725 A1 10/2011 Argentine et al.
 2011/0262684 A1 10/2011 Wintch et al.
 2011/0264184 A1 10/2011 Heltai
 2012/0143317 A1 6/2012 Cam et al.
 2012/0158038 A1 6/2012 Leschinsky
 2012/0179236 A1 7/2012 Benary
 2012/0323305 A1 12/2012 Benary
 2013/0274866 A1 10/2013 Cox et al.
 2014/0364930 A1 12/2014 Strauss et al.

FOREIGN PATENT DOCUMENTS

EP 1 325 716 7/2003
 JP 2002253682 9/2002
 WO 98/06355 A1 2/1998
 WO 9934748 7/1999
 WO 03/099108 12/2003
 WO 2004/017868 3/2004
 WO 2005/002466 1/2005
 WO 2005/034809 A1 4/2005
 WO 2005/037138 4/2005
 WO 2005/041781 5/2005
 WO 2005/041783 5/2005
 WO 2006/007389 1/2006
 WO 2006/028925 3/2006
 WO 2006/070372 7/2006
 WO 2007/084547 7/2007
 WO 2007/144782 12/2007
 WO 2008/008291 1/2008
 WO 2008/035337 3/2008
 WO 2008/042266 4/2008
 WO 2008/047092 4/2008
 WO 2008/047354 4/2008
 WO 2008/053469 5/2008
 WO 2008/107885 9/2008
 WO 2008/140796 11/2008
 WO 2009/078010 6/2009
 WO 2009/116041 9/2009
 WO 2009/116042 9/2009
 WO 2009/118733 10/2009
 WO 2010/024869 3/2010
 WO 2010/024879 3/2010
 WO 2010/031060 3/2010
 WO 2010/027704 A1 3/2010
 WO 2010/045238 4/2010
 WO 2010/062355 6/2010
 WO 2010/088776 8/2010
 WO 2010/128162 11/2010
 WO 2010/150208 12/2010
 WO 2011/004374 1/2011

WO 2011/007354 1/2011
 WO 2011/055364 5/2011
 WO 2011/064782 6/2011
 WO 2011/067764 6/2011
 WO 2011/070576 6/2011
 WO 2011/080738 7/2011
 WO 2011/095979 8/2011
 WO 2011/106532 9/2011
 WO 2011/106533 9/2011
 WO 2011/106544 9/2011
 WO 2012/049679 4/2012
 WO 2012/104842 8/2012
 WO 2012/111006 8/2012
 WO 2012/117395 9/2012
 WO 2012/176187 12/2012
 WO 2013/005207 1/2013
 WO 2013/030818 3/2013
 WO 2013/030819 3/2013
 WO 2013/065040 5/2013
 WO 2013/084235 6/2013
 WO 2013/171730 11/2013

OTHER PUBLICATIONS

Communication dated Aug. 15, 2014, issued by the United States Patent and Trademark Office in counterpart Application No. 13939798.

Communication dated Sep. 2, 2014, issued by the United States Patent and Trademark Office in counterpart Application No. 12447684.

Communication dated Jul. 30, 2015 from the U.S. Patent and Trademark Office in counterpart application No. 14/240600.

Communication dated Aug. 12, 2015 from the U.S. Patent and Trademark Office in counterpart application No. 13/513397.

Communication dated Sep. 23, 2015 from the U.S. Patent and Trademark Office in counterpart application No. 13/384075.

Communication dated Oct. 2, 2015 from the U.S. Patent and Trademark Office in counterpart application No. 13/577161.

Communication dated Oct. 27, 2015 from the European Patent Office in counterpart application No. 10835608.0.

An Office Action dated Apr. 28, 2014, which issued during the prosecution of U.S. Appl. No. 13/939,798.

An English translation of an Office Action dated Nov. 28, 2013 which issued during the prosecution of Chinese Patent Application No. 200880126889.0.

"E-vita® open plus" product brochure (JOTEC GmbH, Hechingen, Germany), 2010.

Fonseca A et al., "Intravascular ultrasound assessment of the novel AngioSculpt scoring balloon catheter for the treatment of complex coronary lesions," J Invasive Cardiol 20(1):21-7 (Jan. 2008).

Khlif H et al., "Contribution to the Improvement of Textile Vascular Prostheses Crimping," Trends in Applied Sciences Research 6(9):1019-1027 (2011).

An International Search Report dated Sep. 29, 2008, which issued during the prosecution of Applicant's PCT/IL08/000287.

A Written Opinion dated Sep. 29, 2008, which issued during the prosecution of Applicant's PCT/IL08/000287.

An International Search Report dated Feb. 4, 2011, which issued during the prosecution of Applicant's PCT/IB2010/052861.

A Written Opinion dated Feb. 4, 2011, which issued during the prosecution of Applicant's PCT/IB2010/052861.

An International Search Report dated Dec. 3, 2010, which issued during the prosecution of Applicant's PCT/IL2010/000564.

A Written Opinion dated Dec. 3, 2010, which issued during the prosecution of Applicant's PCT/IL2010/000564.

An International Search Report dated Nov. 5, 2010, which issued during the prosecution of Applicant's PCT/IL2010/000549.

A Written Opinion dated Nov. 5, 2010, which issued during the prosecution of Applicant's PCT/IL2010/000549.

An International Search Report dated Aug. 4, 2011, which issued during the prosecution of Applicant's PCT/IL2010/000999.

An International Search Report dated Mar. 10, 2011, which issued during the prosecution of Applicant's PCT/IL2010/000917.

(56)

References Cited

OTHER PUBLICATIONS

An International Search Report dated Mar. 30, 2011, which issued during the prosecution of Applicant's PCT/IL2010/001018.
An International Search Report dated Apr. 18, 2011, which issued during the prosecution of Applicant's PCT/IL2010/001037.
An International Search Report dated May 23, 2011, which issued during the prosecution of Applicant's PCT/IL2010/001087.
An International Search Report dated Jun. 28, 2011, which issued during the prosecution of Applicant's PCT/IL2011/000135.
An International Search Report dated Jun. 30, 2009, which issued during the prosecution of Applicant's PCT/IL2008/001621.
A Written Opinion dated Jun. 30, 2009, which issued during the prosecution of Applicant's PCT/IL2008/001621.
An International Search Report dated Mar. 11, 2009, which issued during the prosecution of Applicant's PCT/IL2007/001312.
A Written Opinion dated Mar. 11, 2009, which issued during the prosecution of Applicant's PCT/IL2007/001312.
An English translation of an Office Action dated Aug. 25, 2011, which issued during the prosecution of Chinese Patent Application No. 200880014919.9.
An Office Action dated Nov. 12, 2010, which issued during the prosecution of U.S. Appl. No. 12/447,684.
An Office Action dated Apr. 27, 2011, which issued during the prosecution of U.S. Appl. No. 12/447,684.
An International Preliminary Report on Patentability dated Aug. 4, 2009, which issued during the prosecution of Applicant's PCT/IL2007/001312.
An English Abstract of JP2002-253682 published Sep. 10, 2002.
An International Search Report and a Written Opinion both dated Jul. 13, 2012, which issued during the prosecution of Applicant's PCT/IL2012/000083.
An International Search Report and a Written Opinion both dated Mar. 15, 2013, which issued during the prosecution of Applicant's PCT/IL2012/050424.
U.S. Appl. No. 61/448,199, filed Mar. 2, 2011.
U.S. Appl. No. 61/014,031, filed Dec. 15, 2007.
An Examiner Interview Summary Report dated Dec. 13, 2010, which issued during the prosecution of U.S. Appl. No. 12/447,684.
U.S. Appl. No. 60/863,373, filed Oct. 29, 2006.
An Office Action together with its English Translation dated Feb. 16, 2013 which issued during the prosecution of Chinese Patent Application No. 200880126889.0.

A Restriction Requirement dated Mar. 21, 2012, which issued during the prosecution of U.S. Appl. No. 12/808,037.
An Office Action dated Jun. 19, 2012, which issued during the prosecution of U.S. Appl. No. 12/808,037.
An Office Action dated Feb. 27, 2013, which issued during the prosecution of U.S. Appl. No. 12/808,037.
A Notice of Allowance dated May 22, 2013, which issued during the prosecution of U.S. Appl. No. 12/808,037.
An International Search Report and a Written Opinion both dated Jul. 17, 2012, which issued during the prosecution of Applicant's PCT/IL2012/000095.
An International Preliminary Report on Patentability dated Sep. 3, 2013, which issued during the prosecution of Applicant's PCT/IL2012/000095.
An International Preliminary Report on Patentability dated Aug. 21, 2013, which issued during the prosecution of Applicant's PCT/IL2012/000083.
An International Search Report and a Written Opinion both dated Oct. 4, 2012, which issued during the prosecution of Applicant's PCT/IL2012/000269.
An International Search Report and a Written Opinion both dated Aug. 31, 2012, which issued during the prosecution of Applicant's PCT/IL2012/000148.
An International Search Report and a Written Opinion both dated Sep. 6, 2012, which issued during the prosecution of Applicant's PCT/IL2012/000190.
An International Search Report and a Written Opinion both dated Sep. 24, 2012, which issued during the prosecution of Applicant's PCT/IL2012/00060.
An International Search Report and a Written Opinion both dated Oct. 1, 2012, which issued during the prosecution of Applicant's PCT/IL2012/000241.
An Office Action dated Oct. 11, 2012, which issued during the prosecution of U.S. Appl. No. 13/031,871.
U.S. Appl. No. 61/443,740, filed Feb. 17, 2011.
An Office Action dated Feb. 25, 2013, which issued during the prosecution of U.S. Appl. No. 13/031,871.
An Extended European Search Report dated Dec. 13, 2012, which issued during the prosecution of Applicant's European App No. 08719912.1.
Communication dated Feb. 3, 2015 from the United States Patent and Trademark Office in counterpart application No. 12/447,684.
Communication dated Nov. 28, 2014 from the European Patent Office in counterpart application No. 08861980.4.

* cited by examiner

FIG. 1

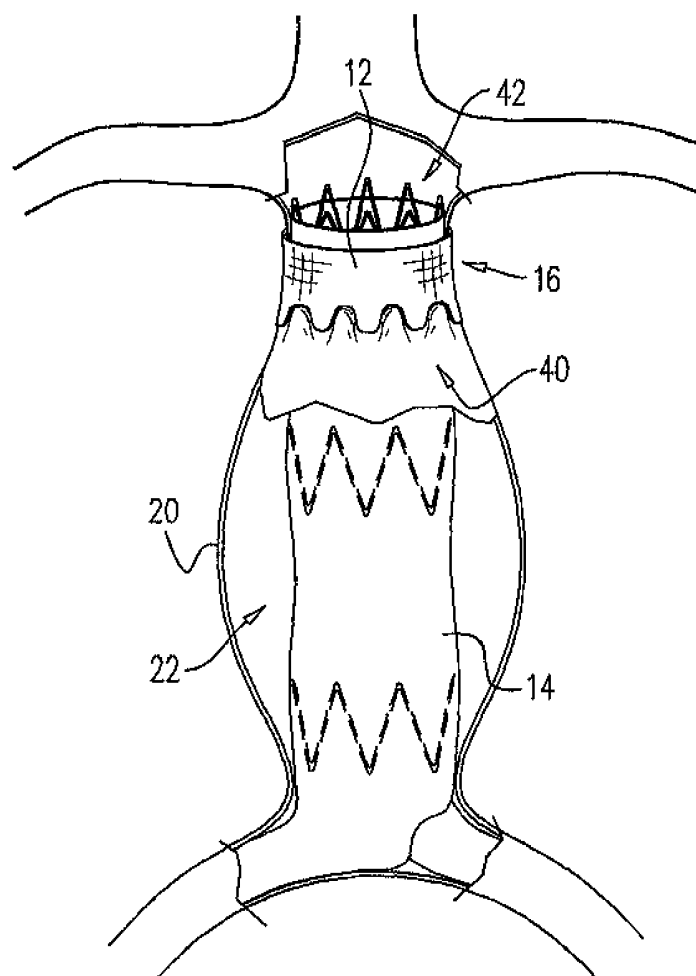


FIG. 2

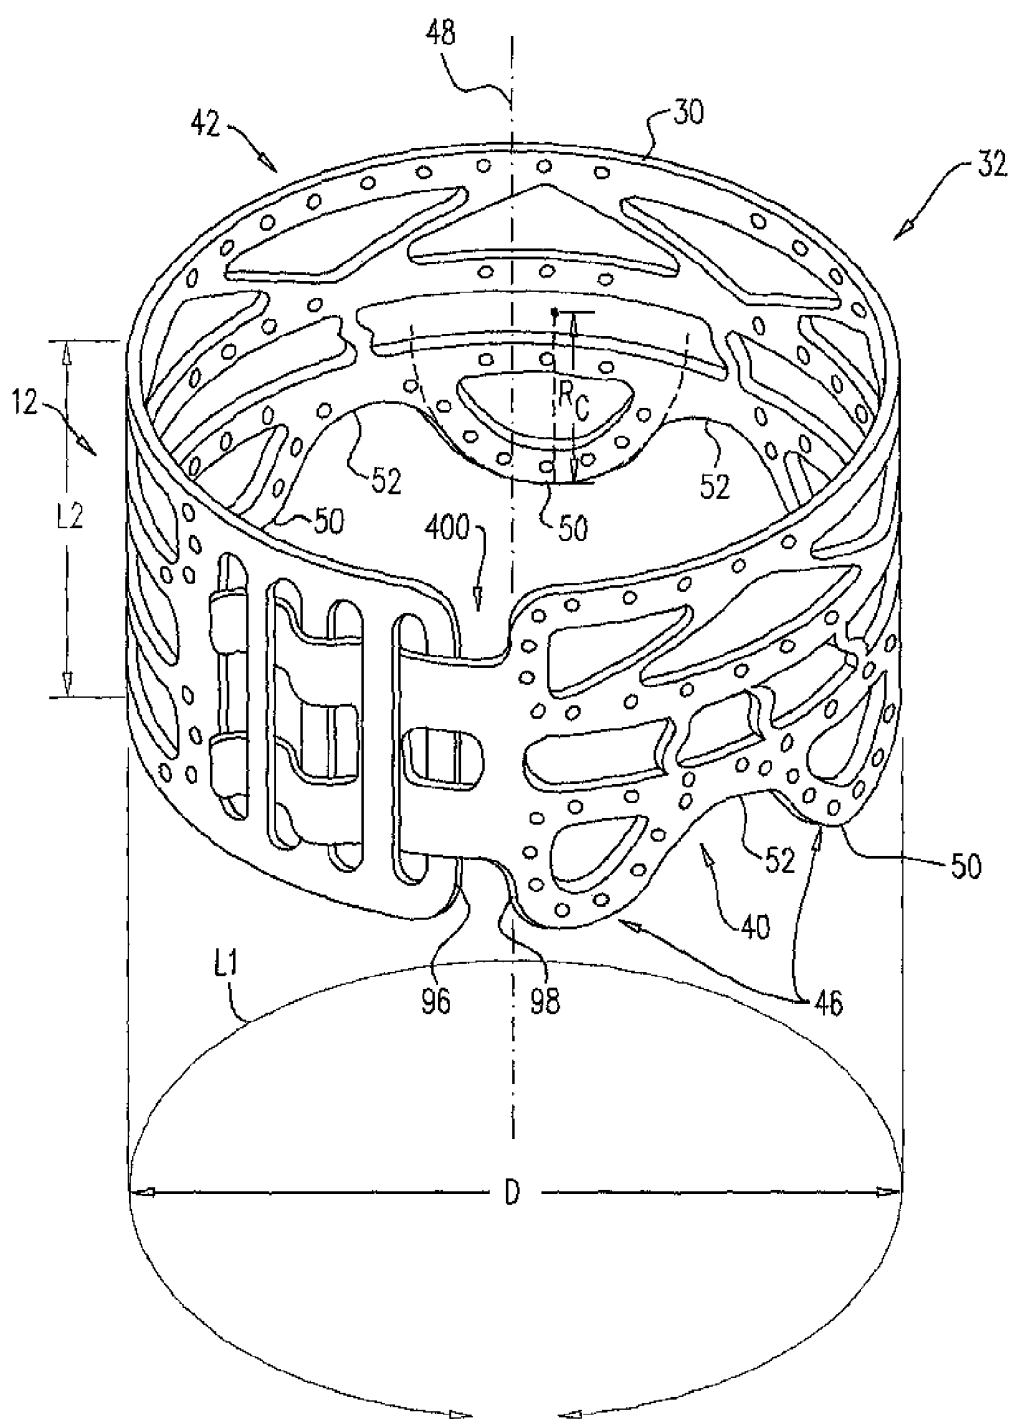


FIG. 3A

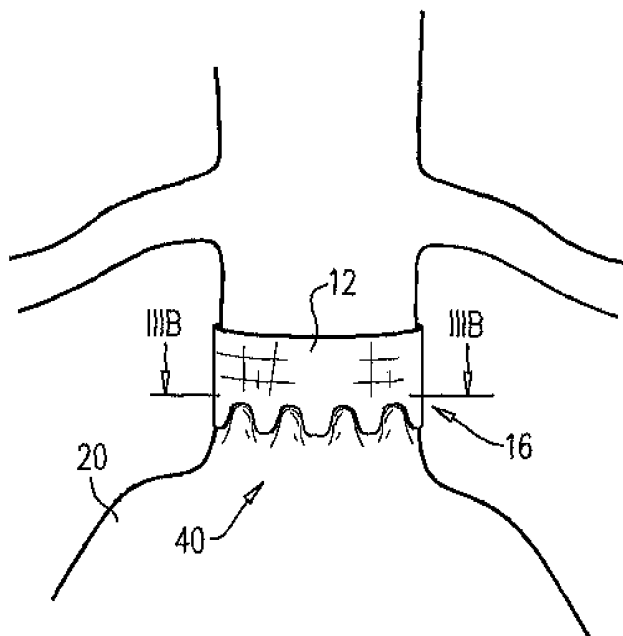


FIG. 3B

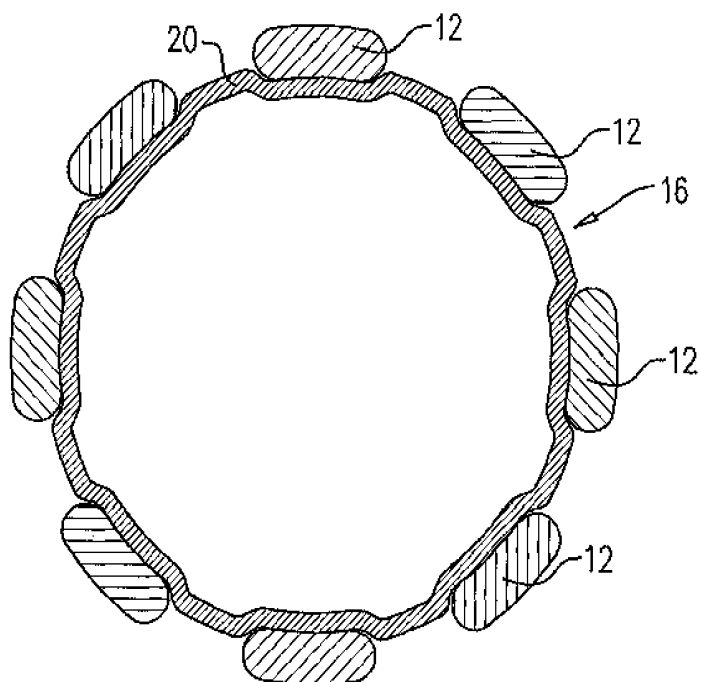


FIG. 3C

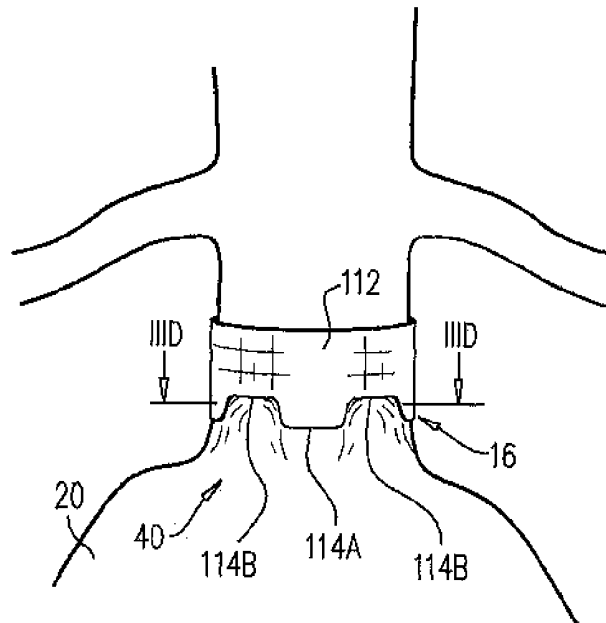


FIG. 3D

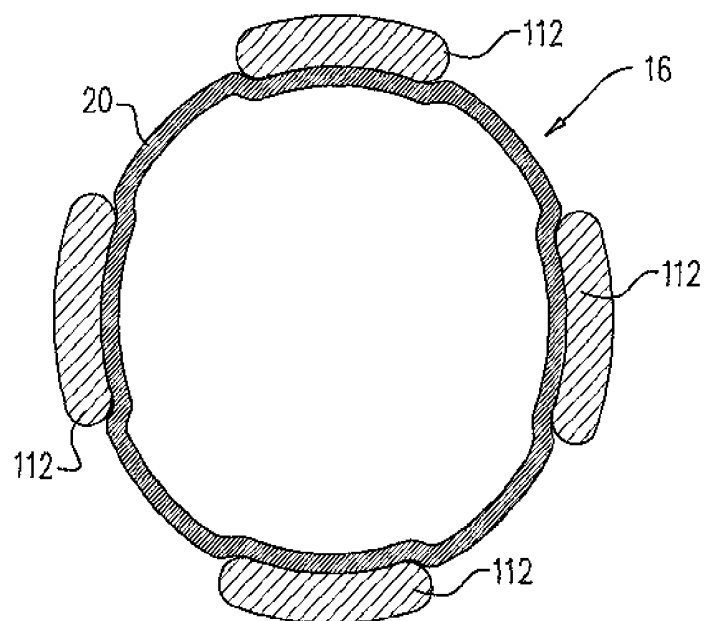
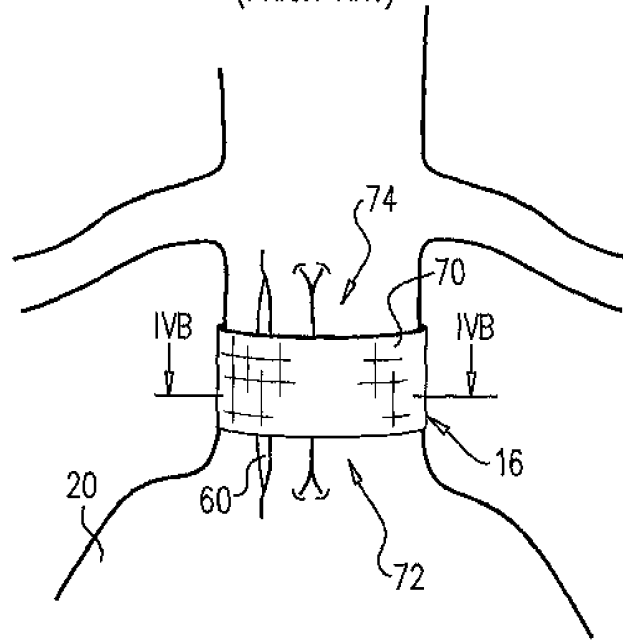
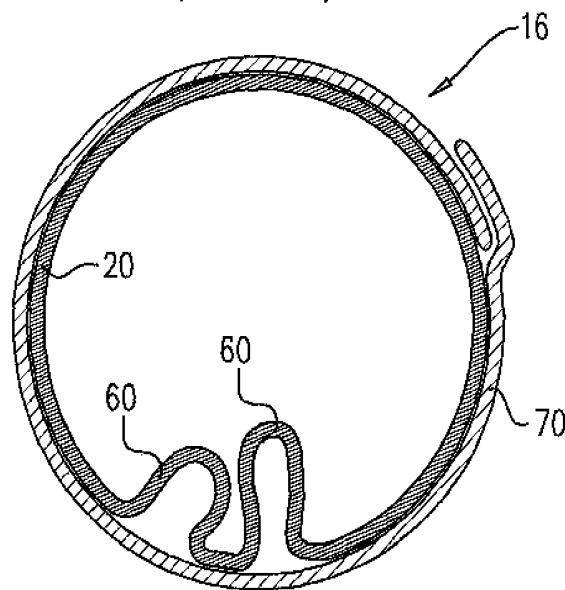



FIG. 4A

(PRIOR ART)

**FIG. 4B**

(PRIOR ART)



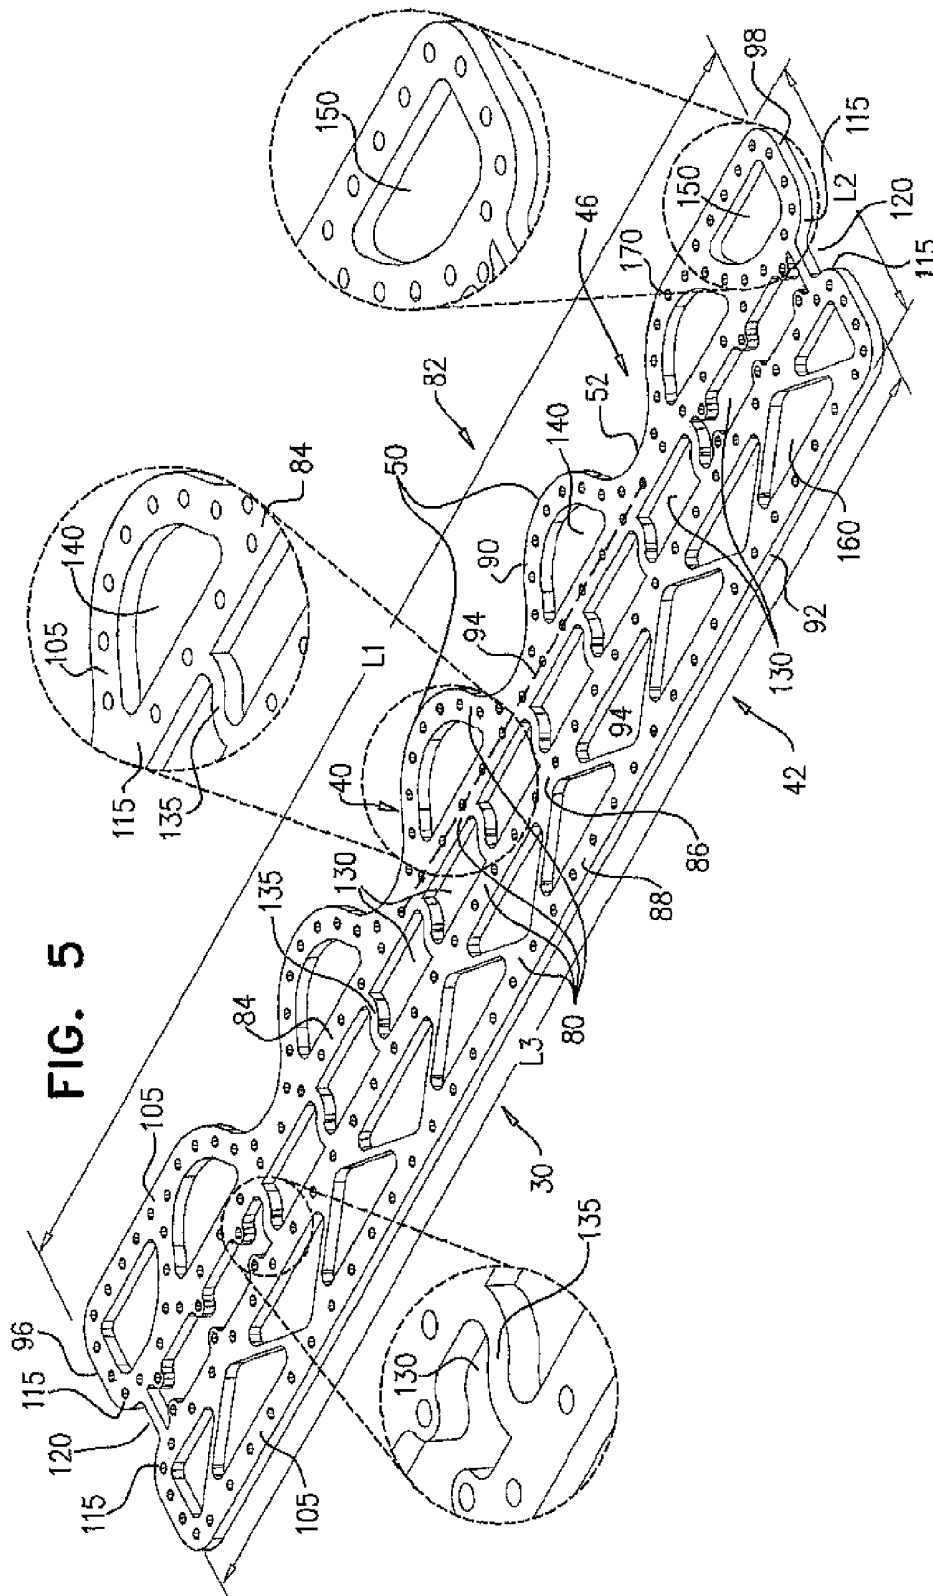

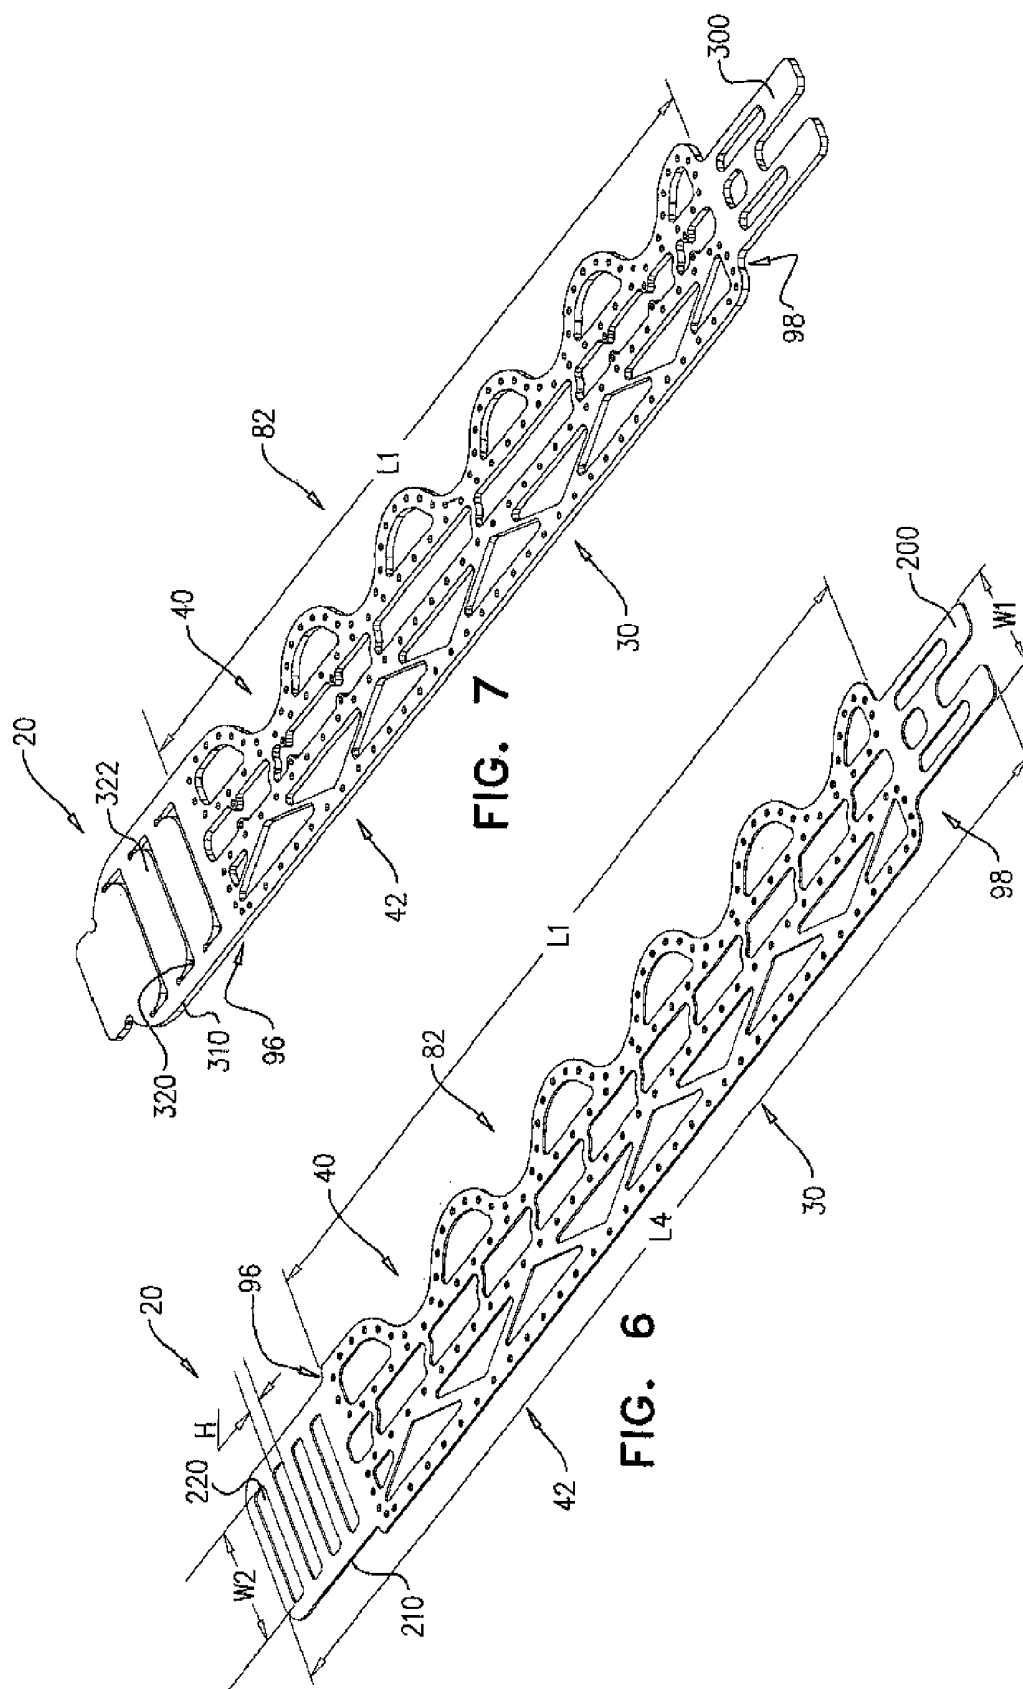


FIG. 8A

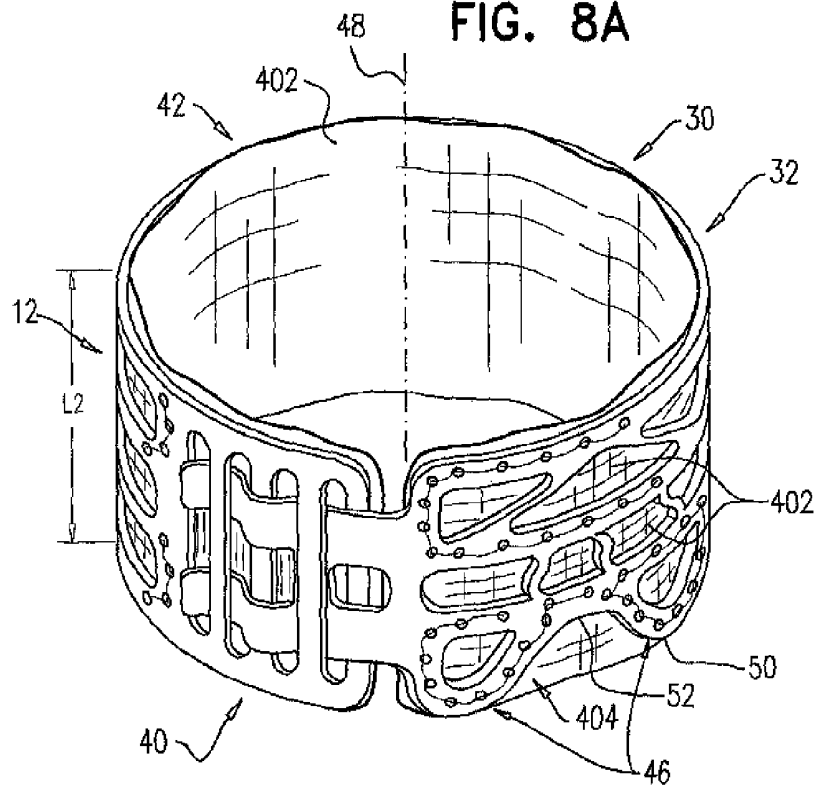


FIG. 8B

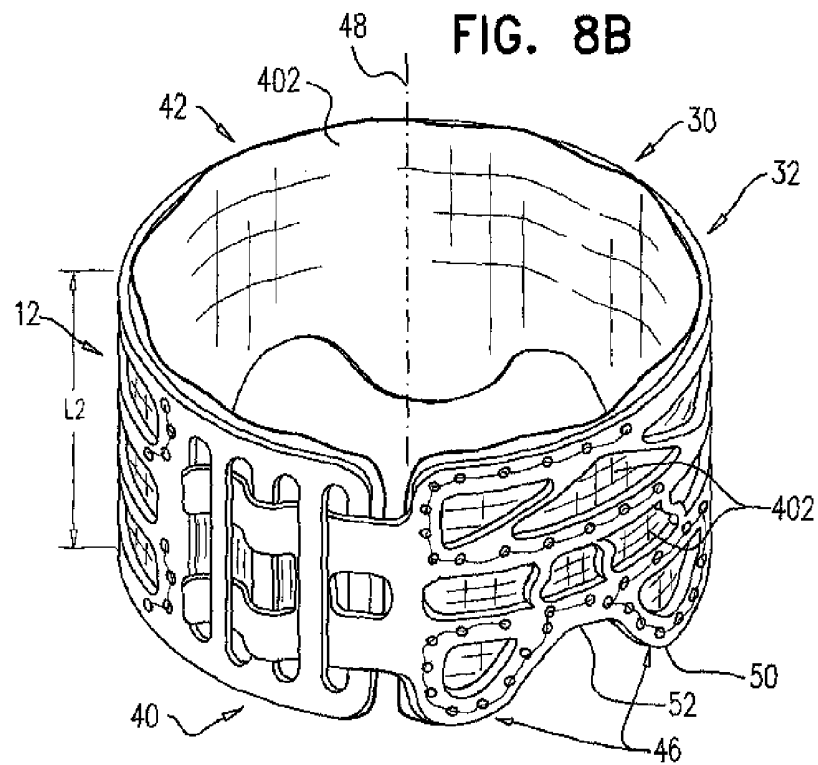


FIG. 9B

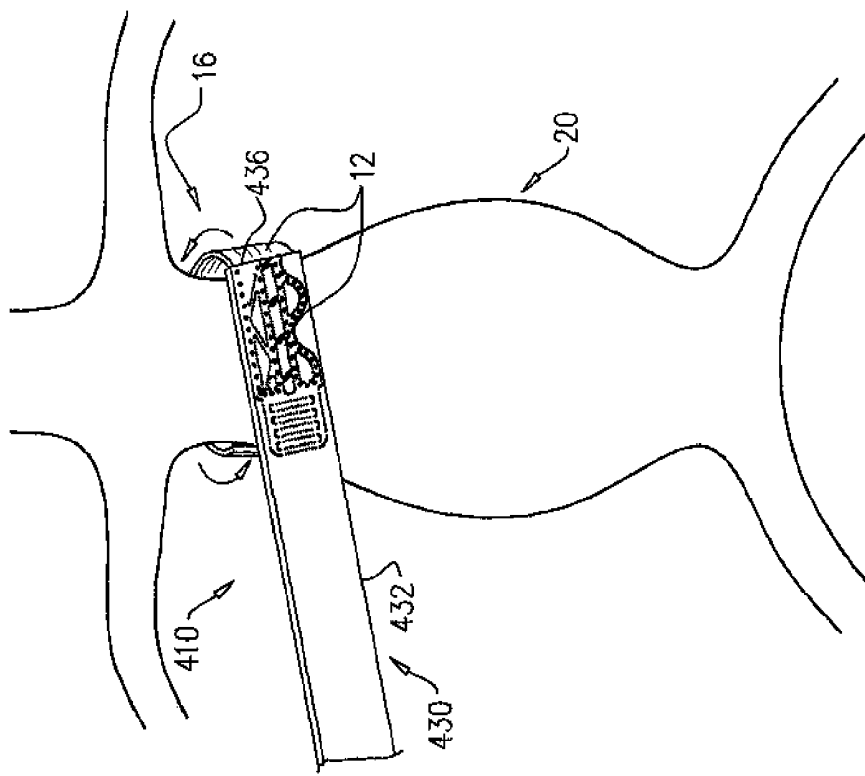


FIG. 9A

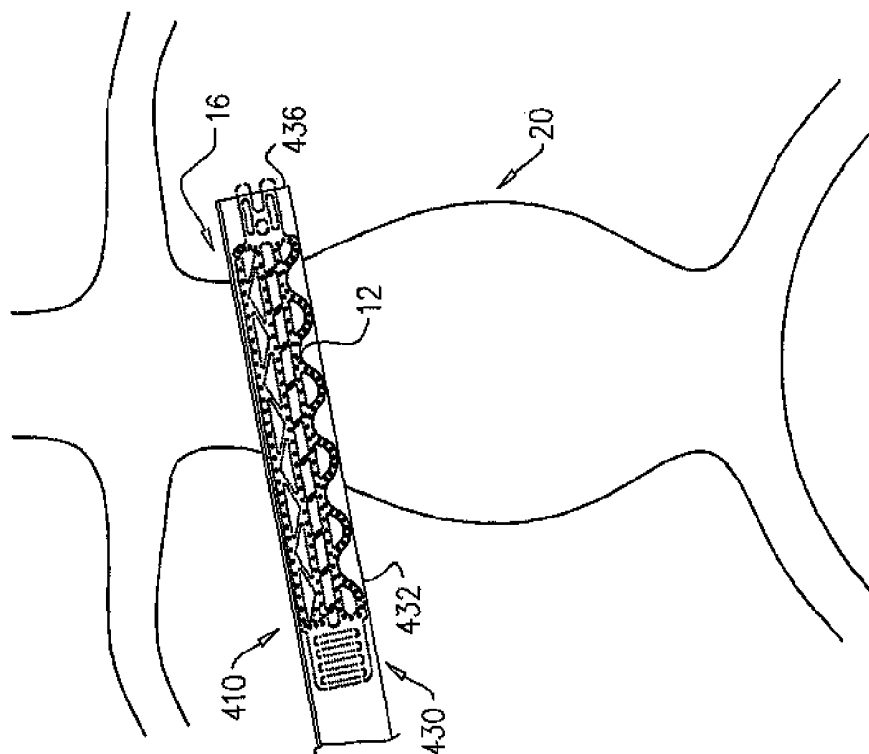


FIG. 9D


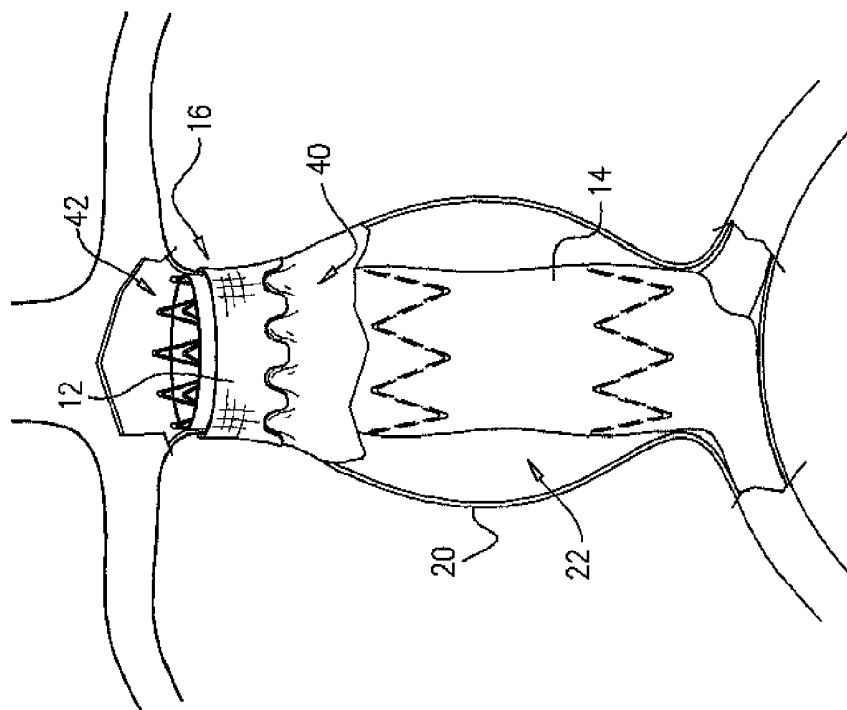


FIG. 9C

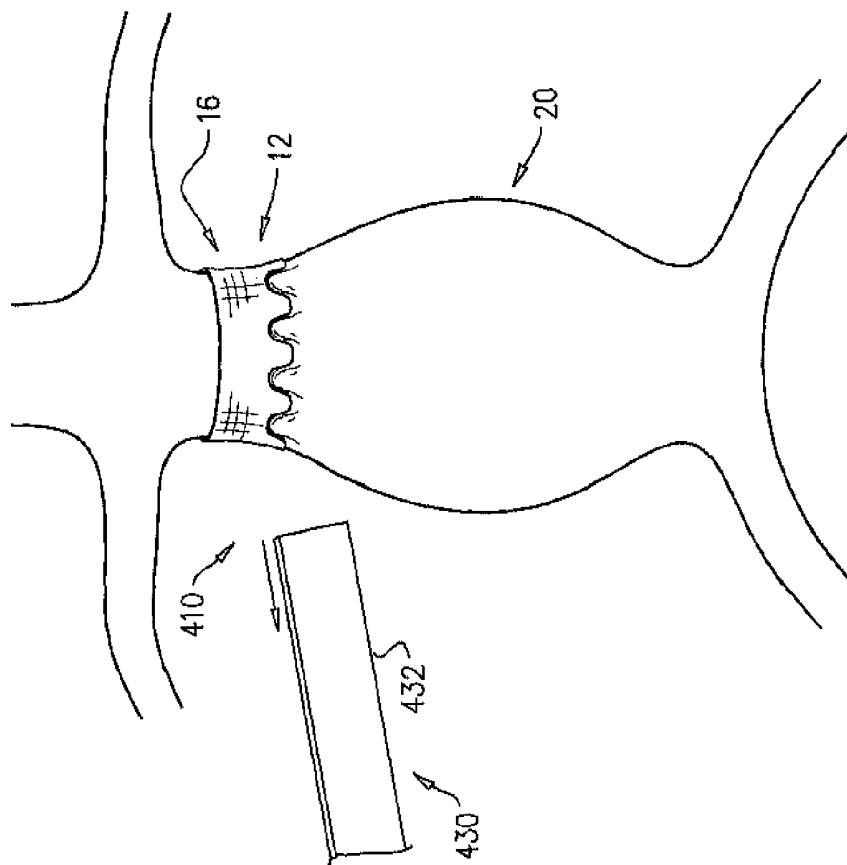

1

REDUCED-STRAIN EXTRA-VASCULAR RING FOR TREATING AORTIC ANEURYSM

CROSS REFERENCE TO RELATED APPLICATIONS

The present patent application is the US national stage of International Application PCT/IL2012/000095, filed Mar. 1, 2012, which claims priority from U.S. Provisional Application No. 61/448,199, filed Mar. 2, 2011, which is assigned to the assignee of the present application and is incorporated herein by reference.

FIELD OF THE APPLICATION

The present invention relates generally to implantable medical devices, and specifically implantable vascular bands.

BACKGROUND OF THE APPLICATION

An aneurysm is a localized, blood-filled dilation (bulge) of a blood vessel caused by disease or weakening of the vessel wall. Left untreated, the aneurysm will frequently rupture, resulting in loss of blood through the rupture and death. Aneurysms are commonly classified by shape, structure and location. Aortic aneurysms are the most common form of arterial aneurysm and are life-threatening. It is common for an aortic aneurysm to occur in the portion of the abdominal aorta between the renal arteries and the iliac arteries. Aneurysms in the abdominal aorta are associated with particularly high mortality; accordingly, current medical standards call for urgent operative repair when aneurysm diameter is larger than 5 cm. Abdominal surgery, however, results in substantial stress to the body. Although the mortality rate for an aortic aneurysm is extremely high, there is also considerable mortality and morbidity associated with open surgical intervention to repair an aortic aneurysm.

Therefore, less invasive techniques have been developed to treat an aortic aneurysm without the attendant risks of intra-abdominal surgery. These techniques include transvascularly introducing an endovascular stent-graft into the aorta. The neck of the aorta at the cephalad end (i.e., above the aneurysm) is usually sufficient to maintain attachment of a stent-graft to the wall of the aorta. However, when an aneurysm is located near the iliac arteries, there may be an ill-defined neck or no neck below the aneurysm. Such an ill-defined neck may provide insufficient healthy aortic tissue to which to successfully mount a stent-graft. Furthermore, much of the abdominal aorta wall may be calcified which may make it difficult to attach the stent-graft to the aortic wall. Unfavorable anatomy relating to the neck of the aneurysm is the most common reason for patients being rejected for Endovascular Repair of Abdominal Aortic Aneurysm (EVAR). A short or absent infrarenal neck, large aortic diameters, and excessive angulation at this level are the main problems. Furthermore, progressive expansion of the aneurysm sac associated with type I endoleak can lead to compromise of the seal at the neck and is the principal indication for secondary intervention for this condition.

PCT Publication WO 2009/078010 to Shalev, and US Patent Application Publication 2010/0292774 in the national stage thereof, which are assigned to the assignee of the present application and is incorporated herein by reference, describe a system for treating an aneurysmatic abdominal aorta, comprising (a) an extra-vascular wrapping (EVW) comprising (i) at least one medical textile member adapted

2

to at least partially encircle a segment of aorta in proximity to the renal arteries, and (ii) a structural member, wherein the EVW is adapted for laparoscopic delivery, and (b) an endovascular stent-graft (ESG) comprising (i) a compressible structural member, and (ii) a substantially fluid impervious fluid flow guide (FFG) attached thereto. Also described is an extra-vascular ring (EVR) adapted to encircle the neck of an aortic aneurysm. Further described are methods for treating an abdominal aortic aneurysm, comprising laparoscopically delivering the extra-vascular wrapping (EVW) and endovascularly placing an endovascular stent-graft (ESG). Also described are methods to treat a type I endoleak. U.S. Provisional Application 61/014,031, filed Dec. 15, 2007, from which the above-referenced applications claim priority, is also incorporated herein by reference.

SUMMARY OF THE APPLICATION

In some applications of the present invention, an extra-vascular ring is provided for deployment around a neck of an aneurysmal aorta, in order to create a generally cylindrical landing zone for an endovascular stent-graft. The endovascular stent-graft is endovascularly deployed in the aorta, spanning an aneurysm thereof, such that a portion of the endovascular stent-graft is positioned against an internal wall of aorta at the landing zone provided by the extra-vascular ring. The landing zone helps create a non-leaking seal between the stent-graft and the wall of the aorta. The extra-vascular ring thus helps secure the aneurysmal neck from widening and/or leaking.

The extra-vascular ring is configured to evenly distribute the pressures and stresses on the partially-dilated tissue of the aortic aneurysm neck. To this end, a structural member of the ring is configured to assume an elongate hollow shape that has first and second longitudinal ends. At least the first longitudinal end has a profile that defines a series of curved portions and has no singularities or discontinuities, which profile extends around at least 50% of the first longitudinal end. The profile serves to homogeneously distribute the strain on the aortic tissue at the first longitudinal end of the ring. The profile provides spaces into which the excess circumference of the aorta can expand, rather than folding inwardly.

For some applications, the profile is a corrugated profile that defines a series of smooth undulations. For these applications, the smooth undulations are shaped so as to define alternating curved peaks and curved valleys. For some applications, the curved peaks are not sharp or traumatic; for example, they may have a radius of curvature equal to at least 3% of the length of the first longitudinal end, when the structural member is in a relaxed state. For some applications, the structural member comprises a plurality of stent struts.

Typically, the structural member is configured to generally not be longitudinally expansible if unrolled to a planar shape, one side of which is defined by the first longitudinal end of the structural member, and accordingly not to be radially expansible when the structural member has the elongate hollow shape. The alternating curved peaks and curved valleys of the corrugated profile of the longitudinal end are not configured to compress or stretch in a direction parallel to the longitudinal end. In other words, the curved peaks are not configured to bend or flex when the structural member is longitudinal stretched.

For some applications, such as in order to provide the longitudinal stability described in the previous paragraph,

when the structural member has the planar shape, at least one of the stent struts extends completely alongside at least two of the undulations (i.e., two of the curved peaks and two of the curved valleys), such that the strut substantially prevents longitudinal stretching of the at least two of the undulations. For some applications, when the structural member has the planar shape, the strut has a length equal to at least 90% of the length of the first longitudinal end.

There is therefore provided, in accordance with an application of the present invention, apparatus for attachment to an aorta of a patient, the apparatus including:

an extra-vascular ring, which includes a structural member, which is configured to assume an elongate hollow shape, which has first and second longitudinal ends, and is suitable for placement at least partially around the aorta so as to provide a generally cylindrical landing zone; and

an endovascular stent-graft, which is suitable for endovascular placement inside the aorta such that a portion of the endovascular stent-graft is positioned against an internal wall of the aorta at the landing zone provided by the structural member,

wherein, if the structural member is unrolled to a planar shape, one side of the planar shape is defined by the first longitudinal end of the structural member, and at least the first longitudinal end has a profile that defines a series of curved portions and has no singularities or discontinuities, which profile extends along at least 50% of the first longitudinal end.

For some applications, the profile is a corrugated profile that defines a series of smooth undulations. For some applications, the corrugated profile has a substantially sinusoidal form.

For some applications, the first and second longitudinal ends are curved at least partially around a longitudinal axis defined by the elongate hollow shape, and the smooth undulations are shaped so as to define alternating curved peaks and curved valleys, which curved peaks extend in a direction away from the second longitudinal end and have a radius of curvature equal to at least 3% of a length of the first longitudinal end measured around the longitudinal axis, when the structural member is in a relaxed state.

For some applications, the smooth undulations are shaped so as to define alternating curved peaks and curved valleys, which curved peaks extend in a direction away from the second longitudinal end, and, if the structural member is unrolled to the planar shape, a radius of curvature of the curved peaks changes by less than 10% if the structural member, while having the planar shape, is longitudinally stretched from a relaxed state by application of a greatest force that is insufficient to cause plastic deformation of the structural member.

For some applications, the structural member includes a plurality of stent struts, and, if the structural member is unrolled to a planar shape, at least one of the stent struts extends completely alongside at least two of the undulations, such that the strut substantially prevents longitudinal stretching of the at least two of the undulations. For some applications, the at least one of the stent struts geometrically encompasses at least one straight line segment that is parallel to the one side and extends completely alongside the at least two of the undulations, when the structural member has the planar shape. For some applications, the at least one of the stent struts is straight when the structural has the planar shape. For some applications, the structural member has the planar shape, the at least one stent strut has a length, measured in a direction parallel to the one side, equal to at least 90% of a length of the one side.

For some applications, if the structural member is unrolled to the planar shape, the first longitudinal end of the structural member has a length that varies by less than 20% if the structural member, while having the planar shape, is longitudinally stretched from a relaxed state by application of a greatest force that is insufficient to cause plastic deformation of the structural member.

For some applications, the profile defines the series of curves interspersed with one or more straight portions.

For any of the applications described above, the structural member may be configured to assume the elongate hollow shape when in a relaxed state.

For any of the applications described above, the structural member may include a super-elastic material.

For any of the applications described above, the structural member may include a shape memory material.

For any of the applications described above, if the structural member is unrolled to the planar shape, the first longitudinal end may have a length that is equal to between 30 and 120 mm; and the elongate hollow shape may have a longitudinal length, measured parallel to a central longitudinal axis of the elongate hollow shape, that equals between 10 and 40 mm.

For any of the applications described above, the structural member, when having the elongate hollow shape, is shaped so as to define a gap that extends longitudinally along an entire longitudinal length of the elongate hollow shape from the first longitudinal end to the second longitudinal end. For some applications, the structural member is shaped so as to define (a) a first extension, which first extension defines at least one slot, and (b) a second extension, which is shaped so as to define a tab adapted to fit into the at least one slot, such that inserting the tab into the slot closes the gap. For some applications, the extra-vascular ring further includes one or more fastening elements for closing the gap.

For any of the applications described above, the apparatus may further include a hollow, generally tubular delivery shaft, in which the extra-vascular ring is removably disposed with the structural member in a deformed state. For some applications, the structural member is configured to automatically transition from the deformed state to a relaxed state as the structural member is deployed from the delivery shaft.

For any of the applications described above, the elongate hollow shape may be generally cylindrical.

There is further provided, in accordance with an application of the present invention, a method including:

providing an extra-vascular ring, which includes a structural member, which is configured to assume an elongate hollow shape, which has first and second longitudinal ends, wherein, if the structural member is unrolled to a planar shape, one side of the planar shape is defined by the first longitudinal end of the structural member, and at least the first longitudinal end has a profile that defines a series of curved portions and has no singularities or discontinuities, which profile extends along at least 50% of the first longitudinal end; and

placing the extra-vascular ring at least partially around a neck of an aneurysmal aorta of a patient so as to provide a generally cylindrical landing zone, such that the profile homogeneously distributes strain on aortic tissue at the first longitudinal end of the structural member.

For some applications, the method further includes placing an endovascular stent-graft inside the aorta such that a portion of the endovascular stent-graft is positioned against an internal wall of the neck at the landing zone provided by the structural member.

For some applications, placing the extra-vascular ring includes advancing, to an external surface of the aorta, a hollow, generally tubular delivery shaft, in which the extra-vascular ring is removably disposed with the structural member in a deformed state. For some applications, advancing the delivery shaft includes advancing the delivery shaft through a laparoscopic working channel to an abdominal location adjacent to renal arteries of the aorta, and laparoscopically placing the extra-vascular stent around the neck of the abdominal aorta in a vicinity of the renal arteries.

For some applications, placing the extra-vascular ring includes identifying the patient as suffering from an aneurysm of an abdominal aorta, and treating the aortic aneurysm by placing the extra-vascular ring at least partially around the neck of the abdominal aorta.

For some applications, providing the extra-vascular ring includes providing the extra-vascular ring in which the profile is a corrugated profile that defines a series of smooth undulations. For some applications, providing the extra-vascular ring includes providing the extra-vascular ring in which the corrugated profile has a substantially sinusoidal form.

For some applications, providing the extra-vascular ring includes providing the extra-vascular ring in which the first and second longitudinal ends are curved at least partially around a longitudinal axis defined by the elongate hollow shape, and the smooth undulations are shaped so as to define alternating curved peaks and curved valleys, which curved peaks extend in a direction away from the second longitudinal end and have a radius of curvature equal to at least 3% of a length of the first longitudinal end measured around the longitudinal axis, when the structural member is in a relaxed state.

For some applications, providing the extra-vascular ring includes providing the extra-vascular ring in which the smooth undulations are shaped so as to define alternating curved peaks and curved valleys, which curved peaks extend in a direction away from the second longitudinal end, and wherein, if the structural member is unrolled to the planar shape, a radius of curvature of the curved peaks changes by less than 10% if the structural member, while having the planar shape, is longitudinally stretched from a relaxed state by application of a greatest force that is insufficient to cause plastic deformation of the structural member.

For some applications, providing the extra-vascular ring includes providing the extra-vascular ring in which the structural member includes a plurality of stent struts, and, if the structural member is unrolled to the planar shape, at least one of the stent struts extends completely alongside at least two of the undulations, such that the strut substantially prevents longitudinal stretching of the at least two of the undulations. For some applications, providing the extra-vascular ring includes providing the extra-vascular ring in which the at least one of the stent struts geometrically encompasses at least one straight line segment that is parallel to the one side and extends completely alongside the at least two of the undulations, when the structural member has the planar shape. For some applications, providing the extra-vascular ring includes providing the extra-vascular ring in which the at least one of the stent struts is straight when the structural has the planar shape. For some applications, providing the extra-vascular ring includes providing the extra-vascular ring in which, when the structural member has the planar shape, the at least one stent strut has a length, measured in a direction parallel to the one side, equal to at least 90% of a length of the one side.

For some applications, providing the extra-vascular ring includes providing the extra-vascular ring characterized in that, if the structural member is unrolled to the planar shape, the first longitudinal end of the structural member has a length that varies by less than 20% if the structural member, while having the planar shape, is longitudinally stretched from a relaxed state by application of a greatest force that is insufficient to cause plastic deformation of the structural member.

For some applications, providing the extra-vascular ring includes providing the extra-vascular ring in which the profile defines the series of curved portions interspersed with one or more straight portions.

For some applications, providing the extra-vascular ring includes providing the extra-vascular ring in which the structural member is configured to assume the elongate hollow shape when in a relaxed state.

For some applications, providing the extra-vascular ring includes providing the extra-vascular ring in which the elongate hollow shape is generally cylindrical.

The present invention will be more fully understood from the following detailed description of embodiments thereof, taken together with the drawings, in which:

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a schematic illustration of an endovascular stent-graft system, in accordance with an application of the present invention;

FIG. 2 is a schematic illustration of a structural member of an extra-vascular ring of the endovascular stent-graft system of FIG. 1, in accordance with an application of the present invention;

FIGS. 3A-B are schematic illustrations of the extra-vascular ring of FIG. 2 deployed around a neck of an aneurysmal aorta, in accordance with an application of the present invention;

FIGS. 3C-D are schematic illustrations of another extra-vascular ring deployed around a neck of an aneurysmal aorta, in accordance with an application of the present invention;

FIGS. 4A-B are schematic illustrations of an extra-vascular ring deployed around a neck of an aneurysmal aorta, as known in the prior art;

FIG. 5 is a schematic illustration of a structural member of the extra-vascular ring of FIG. 2 in a planar unrolled state, in accordance with an application of the present invention;

FIG. 6 is a schematic illustration of another configuration of the structural member of the extra-vascular ring of FIG. 2 in the planar unrolled state, in accordance with an application of the present invention;

FIG. 7 is a schematic illustration of yet another configuration of the structural member of the extra-vascular ring of FIG. 2 in the planar unrolled state, in accordance with an application of the present invention;

FIGS. 8A-B are schematic illustrations of two additional configurations of the extra-vascular ring of FIG. 2, in accordance with respective applications of the present invention; and

FIGS. 9A-D are schematic illustrations of a delivery system and method for delivering the extra-vascular ring of FIG. 2 around an aorta, in accordance with an application of the present invention.

DETAILED DESCRIPTION OF APPLICATIONS

FIG. 1 is a schematic illustration of an endovascular stent-graft system 10, in accordance with an application of

the present invention. System 10 comprises an extra-vascular ring 12 and, for some applications, an endovascular stent-graft 14. When deployed around a neck 16 of an aneurysmal aorta 20, extra-vascular ring 12 creates a generally cylindrical landing zone for endovascular stent-graft 14 (which optionally is bifurcated, as shown). As shown in FIG. 1, endovascular stent-graft 14 is endovascularly deployed in aorta 20, spanning an aneurysm 22 thereof, such that a portion (e.g., a superior distal portion) of endovascular stent-graft 14 is positioned against an internal wall of aorta 20 at the landing zone provided by the extra-vascular ring. The landing zone helps create a non-leaking seal between the stent-graft and the wall of the aorta. Extra-vascular ring 12 thus helps secure the aneurysmal neck from widening and/or leaking. Typically, the landing zone is generally resistant to dilation. Extra-vascular ring 12 comprises a structural member 30 and, optionally, a textile member 402, such as described hereinbelow with reference to FIGS. 8A-B.

FIG. 2 is a schematic illustration of structural member 30 of extra-vascular ring 12, in accordance with an application of the present invention. Structural member 30 is configured to assume an elongate hollow shape 32, as shown in FIG. 2, which, for example, may be generally cylindrical. Elongate hollow shape 32 is suitable for placement at least partially around aorta 20 so as to provide the landing zone. Elongate hollow shape 32 has first and second longitudinal ends 40 and 42. Extra-vascular ring 12 is configured to be placed around aorta 20 oriented with first longitudinal end 40 inferior to second longitudinal end 42, typically with first longitudinal end 40 positioned at an inferior end of neck 16 and second longitudinal end 42 positioned at a superior end of neck 16.

At least first longitudinal end 40 of structural member 30 has a profile that defines a series of curved portions and has no singularities or discontinuities, which profile extends around at least 50% of first longitudinal end 40 (i.e., along at least 50% of a length L1 of first longitudinal end 40 measured around elongate hollow shape 32), such as at least 75%, or 100%. The curved portions rise and fall with respect to a direction that is parallel to a longitudinal axis 48 defined by the elongate hollow shape 32. Equivalently, if structural member 30 is unrolled to a planar shape 82, such as described hereinbelow with reference to FIGS. 5-7, one side of planar shape 82 is defined by first longitudinal end 40, and at least first longitudinal end 40 has the profile that defines the series of curved portions and has no singularities or discontinuities, and the profile extends along at least 50% of first longitudinal end 40, such as at least 75%, or 100%.

For some applications in which the profile extends around or along (depending on whether the structural member is rolled or unrolled) less than 100% of first longitudinal end 40, the profile is provided along two or more portions that are non-contiguous around or along the first longitudinal end. For example, the profile may be provided along two portions that are non-contiguous with each other, each of which extends around or along between 20% and 40% of first longitudinal end 40. For other applications in which the profile extends around or along less than 100% of first longitudinal end 40, the corrugate profile is provided on a single contiguous portion around or along a portion of the first longitudinal end. Typically, any portions of first longitudinal end 40 along which the profile is not provided are not shaped to have any singularities, discontinuities, or sharp changes in direction, e.g., are straight if structural member 30 is unrolled to planar shape 82, such as described hereinbelow with reference to FIGS. 5-7.

For some applications, the profile is a corrugated profile that defines a series of smooth undulations 46. As used herein, including in the claims, the term "corrugated" means having any shape comprising a series of smooth undulations that have no singularities, discontinuities, or sharp changes in direction. Therefore, the corrugated profile does not include any sharp, and thus traumatic, features. For example, the term "corrugated" does not include within its scope sawtooth and square-wave forms. The corrugated profile is provided along first longitudinal end 40 as described in the previous paragraph. For some applications, the corrugated profile has a substantially sinusoidal form (which includes the series of curved portions). Alternatively or additionally, for some applications, at least first longitudinal end 40 of structural member 30 has a waved profile.

As can be seen in FIG. 2, first and second longitudinal ends 40 and 42 are curved at least partially around longitudinal axis 48. Smooth undulations 46 of first longitudinal end 40 are shaped so as to define alternating curved peaks 50 and curved valleys 52. Peaks 50 extend in a direction away from second longitudinal end 42. (Each of the smooth undulations is shaped so as to define exactly one of curved peaks 50 adjacent to exactly one of curved valleys 52.) For some applications, the corrugated profile is shaped so as to define at least 3, no more than 10, and/or between 3 and 10 undulations 46, each of which undulations is shaped so as to define exactly one curved peak 50 and exactly one curved valley 52. For some applications, curved peaks 50 do not include any straight portions. Alternatively or additionally, for some applications, curved valleys 52 do not include any straight portions.

For some applications, curved peaks 50 are not sharp or traumatic; for example, they may have a radius of curvature R_C equal to at least 1.5% (e.g., at least 3%) of length L1 of first longitudinal end 40 measured around longitudinal axis 48, when structural member 30 is in a relaxed state (radius of curvature R_C is measured along the outer surface of the curved peak, as indicated in FIG. 2). (Length L1 is circumferential, i.e., curved, when structural member 30 has elongate hollow shape 32, as shown in FIG. 2. The length is also labeled in FIG. 5, in which the structural member is shown in a planar unrolled state.) For some applications, length L1 is at least 30 mm, no more than 120 mm, and/or between 30 and 120 mm, such as 85 mm. For example, length L1 may be 80 mm, in which case radius of curvature R_C may be at least 1.27 mm. For some applications, elongate hollow shape 32 has a longitudinal length (measured parallel to longitudinal axis 48) of at least 10 mm, no more than 40 mm, and/or between 10 and 40 mm, such as 15 mm.

Elongate hollow shape 32 has an inner diameter D suitable for surrounding a vessel, such as an aorta, e.g., a descending aorta, such as for treating an aortic aneurysm, i.e., large enough to surround the aorta at the point of attachment of extra-vascular ring 12 and small enough such that upon closure, the inner surface of the elongate hollow shape 32 (which may be cylindrical, as mentioned above) makes direct or indirect contact at least partially with the outer surface of the aorta being treated. For applications in which extra-vascular ring 12 further comprises a textile member 402, such as described hereinbelow with reference to FIGS. 8A-B, elongate hollow shape 32 makes indirect contact at least partially with the outer surface of the aorta being treated, via the textile member. For example, inner diameter D may be at least 2 cm, no more than 4 cm, and/or between 2 and 4 cm. For some applications, radius of

curvature R_c of curved peaks **50** is equal to at least 5% (e.g., at least 10%) of inner diameter D when ring **12** is placed around neck **16**.

Reference is now made to FIGS. 3A-B, which are schematic illustrations of extra-vascular ring **12** deployed around neck **16** of aneurysmal aorta **20**, in accordance with an application of the present invention. FIG. 3B is a cross-sectional view of ring **12** and aorta **20** along line IIIB-IIIB of FIG. 3A. The corrugated profile of longitudinal end **40** serves to evenly distribute the pressures and stresses on the partially-dilated tissue of neck **16**, in particular on the section of the aorta in the vicinity of longitudinal end **40** of ring **12**. The corrugated profile serves to homogeneously distribute the strain on the aortic tissue at the first longitudinal end of the ring. As can be seen in FIGS. 3A-B, the corrugated profile effectively diffuses the strain on the aortic wall. The corrugated profile provides spaces into which the excess circumference of the aorta can expand, rather than folding inwardly as described hereinbelow with reference to FIGS. 4A-B.

Reference is made to FIGS. 3C-D, which are schematic illustrations of an extra-vascular ring **112** deployed around neck **16** of aneurysmal aorta **20**, in accordance with an application of the present invention. FIG. 3D is a cross-sectional view of ring **112** and aorta **20** along line IIID-IIID of FIG. 3C. Other than as described below, extra-vascular ring **112** is generally similar to extra-vascular ring **12** described hereinabove and hereinbelow, and may include any of the features of extra-vascular ring **12** described hereinabove and/or hereinbelow. The profile of first longitudinal end **40** of extra-vascular ring **112** includes the series of curved portions interspersed with one or more straight portions **114**. The profile does not have any sharp changes in direction. For example, one or more peaks of the undulations may be shaped so as to define a straight portion **114A**, and/or one or more valleys of the undulations may be shaped so as to define a straight portion **114B**. It is noted that the profile of first longitudinal end **40** of extra-vascular ring **112** is not a square-wave form, because there are no sharp changes in direction, such as right angles, in the profile. The profile of longitudinal end **40** serves to minimize the pressures and stresses on the tissue of the aorta, in particular on the section of the aorta in the vicinity of longitudinal end **40** of ring **112**. The profile serves to homogeneously diffuse the strain on the aortic tissue at the longitudinal ends of the ring. As can be seen in FIGS. 3C-D, the profile effectively diffuses the strain on the aortic wall. The profile provides spaces into which the excess circumference of the aorta can expand, rather than folding inwardly as described hereinbelow with reference to FIGS. 4A-B.

Reference is made to FIGS. 4A-B, which are schematic illustrations of an extra-vascular ring **70** deployed around neck **16** of aneurysmal aorta **20**, as known in the prior art. FIG. 4B is a cross-sectional view of ring **70** and aorta **20** along line IVB-IVB of FIG. 4A. Both longitudinal ends **72** and **74** of ring **70** have a straight profile, as known in the prior art. As can be seen, in order to close ring **70**, it is necessary to place a substantial amount of strain on aorta **20**. As shown in FIG. 4B, this strain can lead to collapse or deformation of part of the aortic wall, which may result, for example, in one or more portions **80** of the wall folding inwardly.

Reference is again made to FIGS. 1, 2, and 3A-B, and additionally to FIG. 5, which is a schematic illustration of structural member **30** of extra-vascular ring **12** in a planar unrolled state, in accordance with an application of the present invention. Extra-vascular ring **12** is shown in a

relaxed state in FIG. 5. Typically, extra-vascular ring **12** is configured to transition between the open planar unrolled state shown in FIG. 5 (or the other configurations described hereinbelow with reference to FIG. 6 or 7), and the rolled state shown in FIGS. 1, 2, and 3A-B. For some applications, extra-vascular ring **12** is placed in the planar unrolled state for delivery in a catheter to the extra-aortic site, such as described hereinbelow with reference to FIG. 9A, and transitions (typically, automatically) to the rolled state around the aorta upon being deployed from the catheter, such as described hereinbelow with reference to FIGS. 9B-C.

Structural member **30** of ring **12** comprises a material suitable for use in treatment of aortic aneurysms and that is capable of being transitioned between an open planar state and a rolled state. For some applications, structural member **30** comprises a shape-memory material or a superelastic material. For example, the shape-memory material may comprise a nickel-titanium alloy such as Nitinol, (which is also super-elastic over a defined temperature range). For some applications, structural member **30** is configured to assume the rolled, elongate hollow shape when in a relaxed state. For some applications, structural member **30**, while in its open planar state is rolled into a ring (such as shown in FIG. 2) of a desired diameter and then heated to fix its dimensions (optionally, the structural member is quickly quenched, e.g., in water, to prevent aging effects).

Alternatively, structural member **30** comprises another material with properties that make it suitable for treatment of aortic aneurysm. Non-limiting examples of such properties include biocompatibility, tensile strength, flexibility, and workability. For some applications, the structural member comprises one or more of these materials (e.g., a biocompatible polymer), and is introduced into the patient by rolling the structural member into a cylinder of small enough diameter to enable introduction by laparoscopic methods, unrolling it in situ, wrapping it around the aorta, and securing it, such as using any of the methods described hereinbelow.

For some applications, structural member **30** comprises a plurality of stent struts **80**. For some applications, the stent struts have a thickness of between 0.1 and 1 mm, such as 0.30 mm.

If structural member **30** is unrolled to planar shape **82**, such as shown in FIG. 5, one side **90** of the planar shape is defined by first longitudinal end **40** of structural member **30**, and another side **92** of the planar shape is defined by second longitudinal end **42** of structural member **30**.

For some applications, length L_1 of side **90** (corresponding to first longitudinal end **40**) varies by less than 20% (e.g., less than 10%) if the structural member, while having planar shape **82**, is longitudinally stretched from a relaxed state by application of a greatest force that is insufficient to cause plastic deformation of the structural member. (Application of a force greater than this greatest force will result in plastic deformation of the structural member, in which case the length might increase substantially before breaking.) In other words, structural member **30** is configured to generally not be longitudinally expansible when it has planar shape **82**, and accordingly not to be radially expansible when it has elongate hollow shape **32**. Alternating curved peaks **50** and curved valleys **52** of the corrugated profile of longitudinal end **40** are not configured to compress or stretch in a direction parallel to longitudinal end **40**. (In order to clarify the term "parallel" in this context, it is noted that undulations **46** of the corrugated profile are disposed about a straight line when the structural member has planar shape **82**; the direc-

tion is parallel to this line; the term "parallel" should also be understood in this way hereinbelow and in the claims.) For some applications, radius of curvature R_C of curved peaks 50 changes by less than 10% (e.g., less than 5%) if the structural member, while having planar shape 82, is longitudinally stretched from a relaxed state by application of a greatest force that is insufficient to cause plastic deformation of the structural member. In other words, curved peaks 50 are not configured to bend or flex when the structural member is longitudinal stretched.

For some applications, such as in order to provide the longitudinal stability described in the previous paragraph, when structural member 30 has planar shape 82, at least one 84 of stent struts 80 extends completely alongside at least two of undulations 46 (i.e., two of curved peaks 50 and two of curved valleys 52), such that strut 84 substantially prevents longitudinal stretching of the at least two of the undulations. For some applications, when structural member 30 has planar shape 82, strut 84 has a length L_3 , measured in a direction parallel to side 90, equal to at least 90% of length L_1 of side 90, such as equal to length L_1 . For some applications, a plurality of stent struts 80 extend completely alongside at least two of undulations 46, such as two of stent struts 80, or three of stent struts 80, as labeled struts 84, 86, and 88 in FIG. 5.

For some applications, stent strut 84 geometrically encompasses at least one straight line segment 94 that is parallel to side 90 and extends completely alongside the at least two of undulations 46, when structural member 30 has planar shape 82. In other words, strut 84 is shaped such that a straight line segment could be drawn on the strut completely alongside the at least two of undulations 46. It is to be understood that straight line segment 94 is an abstract geometric construct provided for purposes of describing the shape of strut 84, rather than a physical element of structural member 30, and thus is typically not actually drawn on the structural member. For some applications, stent strut 84 is straight when structural member 30 is unrolled to planar shape 82.

Reference is still made to FIG. 5. For some applications, planar shape 82 of extra-vascular ring 12 is generally rectangular, with two substantially parallel short sides 96 and 98 and two long sides 90 and 92, each of which is substantially perpendicular to the short sides. For some applications, side 92 (i.e., the side not shown as corrugated) is straight. In other embodiments, both long sides 90 and 92 have respective corrugated profiles along at least 50% of their respective lengths, such as along at least 75%, e.g., 100%, of their respective lengths (configuration not shown). For some applications, planar shape 82 has rounded corners, as shown in FIG. 5 (and FIGS. 6 and 7).

For some applications, the edges of stent struts 80 are at least partially rounded smooth, such as by chemical erosion or electro-chemical erosion, as is known in the stent art. For clarity of illustration, this rounding is not shown in FIG. 5 (or FIGS. 2, 6, 7, and 8A-B).

Reference is again made to FIG. 2. For some applications, longitudinal axis 48 is substantially parallel to short sides 96 and 98 of structural member 30, and long sides 90 and 92 form upper and lower faces of elongate hollow shape 32; for applications in which elongate hollow shape 32 is cylindrical, the long sides form the (open) circular upper and lower faces of the cylinder. As a result, the corrugated profile is transverse to longitudinal axis 48 when structural member 30 is in its rolled state. As described below, the ring is brought to its final diameter after its insertion into the patient's body.

Reference is again made to FIG. 5. For some applications, stent struts 80 are shaped so as to define a plurality of missing portions of structural member 30, i.e., openings through structural member 30. In the exemplary configuration shown in FIG. 5, structural member 30 is shaped so as to define an outer substantially contiguous border 105, which may, for example have a width of about 1.50 ± 0.05 mm. In each of respective central portions 120 (typically the central 3 ram) of short sides 96 and 98, border 105 is recessed by two rounded portions 115, and may be narrower than the remainder of the border (e.g., 0.7 mm in width).

For some applications, a central portion of structural member is shaped so as to define a plurality of missing portions 130, two sides of which missing portions are substantially parallel to long side 92. A blow-up in FIG. 5 shows a detailed view of the edge of one of these missing portions 130, including a separating stent strut 135 between them (in the configuration shown, this separating stent strut is curved and has a typical width of about 0.7 mm).

For some applications, structural member 30 is shaped so as to define missing portions 140 along long side 90 (which has the profile), between undulations 46 and stent strut 84 (described above). For some applications, structural member 30 is shaped so as to define two missing portions 150 nearest short sides 96 and 98, each of which may have the shape of a rectangle truncated by a curve along the side nearest first missing portion 140. Detailed views of missing portions 140 and 150 are shown in respective blow-ups in FIG. 5, in accordance with respective applications of the present invention.

For some applications, structural member 30 is shaped so as to define a series of triangular missing portions 160 with one side parallel to long side 92 and having alternating orientations, between central missing portions 130 and the inside of border 105 (e.g., between struts 86 and 88, described hereinabove).

For some applications, structural member 30 is shaped so as to define a plurality of small (e.g., circular) missing portions 170, which may, for example have a typical diameter of 0.5 ± 0.1 mm. For some applications, missing portions 170 are located on all areas of the structural member at which the material has a width sufficient to support these missing portions. Optionally, missing portions 170 are substantially centered with respect to the width of stent struts 80.

For some applications, the missing portions described above serve one or more of four purposes. First, the missing portions may reduce the weight of structural member 30. Second, the missing portions may reduce the amount of material needed to construct structural member 30. Third, the missing portions may allow free tissue ingrowth there-through. Fourth, the missing portions may be arranged to enhance flexibility of the structural member. It is to be understood that the particular arrangement of missing portions 130 and 170 are shown in the figures by way of example and not limitation, and that other arrangements that achieve the same or similar purposes will be apparent to those skilled in the art who have read the present application, and are within the scope of the present invention.

Reference is now made to FIG. 6, which is a schematic illustration of another configuration of structural member 30 of extra-vascular ring 12 in the planar unrolled state, in accordance with an application of the present invention. In this configuration, structural member 30 comprises, in addition to the elements described above with reference to FIGS. 1, 2, 3A-B, and 5, a tab 200 at one of short sides 96 and 98, and an extension 210 at the other one of short sides 96 and

98. Extension **210** is shaped so as to define a plurality of slots **220**. For some applications, an overall length **L4** of structural member **30**, including tab **200** and extension **210** is at least 30 mm, no more than 150 mm, and/or between 30 and 150 mm, such as about 108 mm; for example, the tab may add about 13 mm to the length of the structural member, and the extension may add about 10 to 20 mm. For some applications, a width **W1** of the tab is about 8.75 mm, a width **W2** of slots **220** is about 12 mm, and a height **H** of the slots is about 1.5 mm. (Length **L1** of first longitudinal end **40** is to be understood herein, including in the claims, as excluding the length of tab **200** and the length of extension **210**.)

Reference is now made to FIG. 7, which is a schematic illustration of yet another configuration of structural member **30** of extra-vascular ring **12** in the planar unrolled state, in accordance with an application of the present invention. As in the configuration described hereinabove with reference to FIG. 6, in this configuration structural member **30** comprises a tab-and-slot assembly, which includes a tab **300** and an extension **310**.

Extension **310** is shaped so as to define slots **320** that include respective flexible flaps **322** that aid in securing tab **300** when the ring is closed. Typically, the overall dimensions of the configuration of FIG. 7 are substantially the same as those of the configuration of FIG. 6. (Length **L1** of first longitudinal end **40** is to be understood herein, including in the claims, as excluding the length of tab **300** and the length of extension **310**.)

Reference is made to FIGS. 2, 5, 6, and 7. For some applications, when extra-vascular ring **12** is brought from its planar, unrolled open state (such as shown in FIGS. 5, 6, and 7) to its rolled state (such as shown in FIG. 2), a gap **400** remains between short sides **96** and **98**. When structural member **30** has elongate hollow shape **32**, gap **400** typically extends longitudinally along an entire longitudinal length of elongate hollow shape **32** from first longitudinal end **40** to second longitudinal end **42**. Short sides **96** and **98** are not brought into contact with each other, and the ring is not otherwise closed, until the ring has been put in place around the patient's aorta. Instead the final closure of the ring (which closes gap **400**) is effected after the ring has been put into place around the patient's aorta. In the case of the configuration described with reference to FIG. 6, the closure is effected by inserting tab **200** into slots **220**, while in the case of the configuration described with reference to FIG. 7, the closure is effected by inserting tab **300** into slots **320**.

Reference is now made to FIGS. 1-3D and 5-7. Structural member **30** may be made by any method known in the art. By way of example and not limitation, the structural member may be fabricated from a rectangular blank by removing the missing portions by any standard means such as punching, stamping, milling, or laser cutting. The curved corners, if provided, and the profile of at least first longitudinal end **40** may produced by any standard means such as cutting or stamping. Alternatively, by way of example and not limitation, the structural member may be cast or molded on a form.

Reference is now made to FIGS. 8A-B, which are schematic illustrations of two additional configurations of extra-vascular ring **12**, in accordance with respective applications of the present invention. Extra-vascular ring **12** may implement either of these configurations in combination with any of the configurations described hereinabove, including with reference to FIGS. 2, 5, 6, and 7. In these configurations, extra-vascular ring **12** further comprises a textile member **402**, securely attached to and at least partially covering structural member **30** (typically an inner surface of the ring).

Textile member **402** comprises an implantable-grade, biologically-compatible fabric, and may comprise, for example, a polyester, a polyethylene (e.g., a poly-ethylene-terephthalate), a polypropylene mesh, a polymeric film material (e.g., polytetrafluoroethylene), a polymeric textile material (e.g., woven polyethylene terephthalate (PET)), natural tissue graft (e.g., saphenous vein or collagen), or a combination thereof. For some applications, textile member **402** comprises a macroporous medical textile member mention, such as described in US Patent Application Publication 2010/0292774 to Shalev, which is assigned to the assignee of the present application and is incorporated herein by reference. Alternatively or additionally, extra-vascular ring **12** comprises an external microporous layer, such as described in the '774 publication.

For some applications, as shown in FIG. 8A, textile member **402** is shaped so as to define portions **404** that extend between adjacent curved peaks **50**. Portions **404** are configured to provide sufficient slack to allow the excess circumference to expand into the spaces provided by the corrugated profile, as described hereinabove with reference to FIGS. 3A-B. For other applications, as shown in FIG. 8B, textile member **402** does not define portions **404**, but rather is shaped so as to provide open areas between adjacent curved peaks **50**. For example, the edge of the textile member may coincide with and have the same shape as the corrugated profile; in this configuration, a first longitudinal end of extra-vascular ring **12** coincides with first longitudinal end **40** of structural member **30**, such that the first longitudinal end of extra-vascular ring **12** has the profile that defines the series of curved portions and has no singularities or discontinuities, e.g., the corrugated profile. Alternatively, the textile member may partially extend between adjacent curved peaks **50** (configuration not shown).

Reference is now made to FIGS. 9A-D, which are schematic illustrations of a delivery system **410** and method for delivering extra-vascular ring **12** around aorta **20**, in accordance with an application of the present invention. Delivery system **10** may be used for delivering extra-vascular ring **12** around aorta **20** (as shown) or other tissue, such as an organ, e.g., as a tubular organ, e.g., another blood vessel or a nerve. Delivery system **410** comprises a catheter **430**, which comprises an outer pull-back shaft **432** having generally rectangular cross sections. The outer pull-back shaft serves as a delivery shaft. Extra-vascular ring **12** is initially removably disposed within outer pull-back shaft **432**, with the extra-vascular ring in a deformed generally planar state, as shown in FIG. 5, 6, or 7. Alternatively, extra-vascular ring **12** is in a rolled state when initially disposed within the outer pull-back shaft (configuration not shown), in which case outer pull-back shaft **432** typically does not have generally rectangular cross sections.

During a first stage of an implantation procedure performed using delivery system **410**, a surgeon creates a working channel, typically laparoscopically or hand-assisted laparoscopically, to an external surface of a portion of a target organ, such as aorta **20**, e.g., neck **16** of an aneurysmal aorta, such as a sub-renal neck **16** immediately inferior (e.g., caudally adjacent) to the renal arteries, as shown in FIGS. 9A-D, or a supra-renal neck, an ascending aortic neck, or a neck adjacent the right subclavian artery (locations not shown). The surgeon advances a distal portion of delivery system **410** to the target organ, such as aorta **20**, as shown in FIG. 9A. Typically, the surgeon advances a distal end **436** of outer pull-back shaft **432** slightly beyond the far side of the aorta, such that that outer pull-back shaft **432** is tangential to the aorta, as shown in FIG. 9A.

As shown in FIG. 9B, the surgeon subsequently proximally withdraws pull-back shaft **432**, while simultaneously preventing proximal movement of extra-vascular ring **12** using a stopper shaft. The stopper shaft is not shown in FIG. 9B; the stopper shaft may be implemented using techniques described in PCT Application PCT/IL2012/000083, filed Feb. 16, 2012, entitled, "Vascular bands and delivery systems therefor," which published as PCT Publication WO 2012/111006, is assigned to the assignee of the present application and is incorporated herein by reference, with reference to FIGS. 3A-14C thereof. Techniques described herein may also be implemented in combination with other techniques described in the '083 application, and/or with techniques described in U.S. Patent Application Publication 2010/0292774, which is assigned to the assignee of the present application and is incorporated herein by reference.

Withdrawal of the pull-back shaft deploys extra-vascular ring **12** from distal end **436** of pull-back shaft **432**. The extra-vascular ring is configured to assume a curved shape upon deployment, and thus wraps around the organ, e.g., the aorta, as the ring is deployed, as shown in FIG. 9B. For some applications, the ring is self-curling, and, to this end, typically comprises a shape memory material, such as a super-elastic metal, e.g., Nitinol, which is heat-set to assume the curled configuration, e.g., a circularly-, helically-, or spirally-bent configuration. For some applications, structural member **30** is configured to automatically transition from the deformed state to a relaxed state as the structural member is deployed from pull-back shaft **432**.

FIG. 9C shows pull-back shaft **432** and extra-vascular ring **12** after the ring has been fully deployed from the shaft. As can be seen, the ring encircles at least a portion of the organ, e.g., the aorta, such as only a portion of or the entire organ. As can also be seen, the surgeon has oriented ring **12** such that first longitudinal end **40** is inferior to second longitudinal end **42**, with first longitudinal end **40** positioned at an inferior end of neck **16** and second longitudinal end **42** positioned at a superior end of neck **16**.

When deployed around neck **16** of an aneurysmal aorta, extra-vascular ring **12** creates a landing zone for endovascular stent-graft **14** (which optionally is bifurcated, as shown). As shown in FIG. 9D, endovascular stent-graft **40** is deployed in the aorta, spanning an aneurysm **22** thereof. A distal portion of the stent-graft is positioned against the internal wall of the aorta at the landing zone. The landing zone provided by extra-vascular ring **12** helps create a non-leaking seal between the stent-graft and the wall of the aorta. Extra-vascular ring **12** thus helps secure aneurysmal neck **16** from widening and/or leaking. Optionally, intra-vascular ring **12** is secured or otherwise attached (optionally, reversibly) to intravascular stent-graft **14**, in order to prevent dislocation of the ring and the intravascular stent-graft along the aorta.

Alternatively, for some applications, endovascular stent-graft **14** is implanted first, and subsequently extra-vascular ring **12** is placed around the aorta.

For some applications, after placement around the aorta, elongate hollow shape **32** of extra-vascular ring **12** subtends an arc of less than 360 degrees, i.e., does not fully surround the aorta. Alternatively, the elongate hollow shape is circumferentially complete upon placement around the aorta.

For some applications, a method for treating an aortic aneurysm comprises (a) identifying a subject having an aneurysm of the abdominal aorta; (b) providing extra-vascular ring **12** in any of the configurations described herein; and (c) positioning the ring around the aorta, inferior to the renal arteries, optionally laparoscopically. Typically,

the ring is compressed to a deformed state during delivery and positioning. The method may further comprise providing intravascular stent-graft **14**, and placing the intravascular stent-graft into the aneurysmal aorta in the subject, optionally laparoscopically. For some applications, identifying the subject having the aneurysm of the abdominal aorta comprises identifying the subject having the aneurysm of the abdominal aorta that is likely to rupture. For some applications, identifying the subject having the aneurysm of the abdominal aorta that is likely to rupture defining an aneurysm of the abdominal aorta that is likely to rupture as an aneurysm that is located within about 2 cm of a renal artery, and determining that the abdominal aneurysm is within about 2 cm of a renal artery of the subject.

For some applications, after placing extra-vascular ring **12** around the aorta, the ring is closed using a closure assembly that comprises one or more fastening elements, such as tab **200** and extension **210**, described hereinabove with reference to FIG. 6, or tab **300** and extension **310**, described hereinabove with reference to FIG. 7. Alternatively, the ring may be closed using other fastening techniques. By way of example and not limitation, the ring may be closed using fastening elements selected from the group consisting of: threads, screws, hooks, zips, fasteners, clips, flaps, claspers, springs, claspers, staplers, grips, zippers, hooks and corresponding eyes, hook and loop reclosable fastener squares, hook and loop reclosable fastener strips, hook and loop reclosable fastener dots, hook-and-loop fasteners such as Velcro-type fasteners, straps, holes and string, sutures, wires, cables, tabs, poppers, nails, buttons and corresponding button holes, press button brackets, glues, adhesives, or any combination thereof.

As used in the present application, including in the claims, "tubular" means having the form of an elongate hollow object that defines a conduit therethrough. A "tubular" structure may have varied cross-sections therealong, and the cross-sections are not necessarily circular. For example, one or more of the cross-sections may be generally circular, or generally elliptical but not circular, or circular.

As used herein, terms referring to polygonal figures (e.g., triangles or rectangles) are to be understood as including substantially polygonal figures with rounded corners and/or substantially polygonal figures bounded by curves other than straight lines. As a non-limiting example, the term "triangle" includes shapes such as those of the triangular portions **160**, described hereinabove with reference to FIG. 5, which have rounded corners.

Furthermore, descriptions of geometric shapes in terms of their ideal geometry are not intended to limit the invention to the ideal geometry, but may include deviations from the ideal geometry that are produced when the invention is used in practice. As a non-limiting example, rolling a rectangle so that two opposite sides meet will form a cylinder. In the description herein, the rolling of a substantially rectangular piece into a substantially cylindrical ring may be treated as if the piece and the ring are ideal geometric figures. The scope of the invention however includes cases where in practice the substantially cylindrical ring thus formed is oblique, such as because of imperfections in manufacturing or errors by the surgeon. Such terms as, for example, "longitudinal axis" and "transverse" are intended only as a means of providing a description of the invention that is sufficiently detailed so as to be understood by one of ordinary skill in the art. With reference to geometrical figures, the term "substantially" is taken to mean that the object in question would be recognized by one of ordinary skill in the art as being intended to have the constraints

implied by the term modified by the word “substantially.” Unless explicitly stated to the contrary, descriptions of geometrical figures are not intended to imply that the figures thus created are within any specific maximum deviation from the ideal structure.

The scope of the present invention includes embodiments described in the following applications, which are assigned to the assignee of the present application and are incorporated herein by reference. In an embodiment, techniques and apparatus described in one or more of the following patent applications are combined with techniques and apparatus described herein:

PCT Application PCT/IL2008/000287, filed Mar. 5, 2008, which published as PCT Publication WO 2008/107885 to Shalev et al., and U.S. application Ser. No. 12/529,936 in the national stage thereof, which published as US Patent Application Publication 2010/0063575 to Shalev et al.

U.S. Provisional Application 60/892,885, filed Mar. 5, 2007

PCT Application PCT/IL2007/001312, filed Oct. 29, 2007, which published as PCT Publication WO/2008/053469 to Shalev, and U.S. application Ser. No. 12/447,684 in the national stage thereof, which published as US Patent Application Publication 2010/0070019 to Shalev

U.S. Provisional Application 60/991,726, filed Dec. 2, 2007

PCT Application PCT/IL2008/001621, filed Dec. 15, 2008, which published as PCT Publication WO 2009/078010, and U.S. application Ser. No. 12/808,037 in the national stage thereof, which published as US Patent Application Publication 2010/0292774

U.S. Provisional Application 61/219,758, filed Jun. 23, 2009

U.S. Provisional Application 61/221,074, filed Jun. 28, 2009

PCT Application PCT/IB2010/052861, filed Jun. 23, 2010, which published as PCT Publication WO 2010/150208, and U.S. application Ser. No. 13/380,278 in the national stage thereof, which issued as U.S. Pat. No. 8,870,938

PCT Application PCT/IL2010/000549, filed Jul. 8, 2010, which published as PCT Publication WO 2011/004374

PCT Application PCT/IL2010/000564, filed Jul. 14, 2010, which published as PCT Publication WO 2011/007354, and U.S. application Ser. No. 13/384,075 in the national stage thereof, which published as U.S. Patent Application Publication 2012/0179236

PCT Application PCT/IL2010/000917, filed Nov. 4, 2010, which published as PCT Publication WO 2011/055364

PCT Application PCT/IL2010/000999, filed Nov. 30, 2010, which published as PCT Publication WO 2011/064782

PCT Application PCT/IL2010/001018, filed Dec. 2, 2010, which published as PCT Publication WO 2011/067764

PCT Application PCT/IL2010/001037, filed Dec. 8, 2010, which published as PCT Publication WO 2011/070576

PCT Application PCT/IL2010/001087, filed Dec. 27, 2010, which published as PCT Publication WO 2011/080738

PCT Application PCT/IL2011/000135, filed Feb. 8, 2011, which published as PCT Publication WO 2011/095979

PCT Application PCT/IL2011/000801, filed Oct. 10, 2011, which published as PCT Publication WO 2012/049679

U.S. application Ser. No. 13/031,871, filed Feb. 22, 2011, which published as US Patent Application Publication 2011/0208289

PCT Application PCT/IL2012/000083, filed Feb. 16, 2012, which published as PCT Publication WO 2012/111006.

It will be appreciated by persons skilled in the art that the present invention is not limited to what has been particularly shown and described hereinabove. Rather, the scope of the present invention includes both combinations and subcombinations of the various features described hereinabove, as well as variations and modifications thereof that are not in the prior art, which would occur to persons skilled in the art upon reading the foregoing description.

The invention claimed is:

1. Apparatus for attachment to an aorta of a patient, the apparatus comprising:

an extra-vascular ring, which comprises a structural member, which is configured to assume, when in a relaxed state, an elongate hollow shape, which (a) has first and second longitudinal ends that are curved at least partially around a longitudinal axis defined by the elongate hollow shape, and (b) is suitable for placement at least partially around the aorta so as to provide a generally cylindrical landing zone; and

an endovascular stent-graft, which is suitable for endovascular placement inside the aorta such that a portion of the endovascular stent-graft is positioned against an internal wall of the aorta at the landing zone provided by the structural member,

wherein, if the structural member is unrolled to a planar shape, one side of the planar shape is defined by the first longitudinal end of the structural member, and at least the first longitudinal end has a profile that defines a series of curved portions and has no singularities or discontinuities, which profile extends along at least 50% of the first longitudinal end, wherein the profile is a corrugated profile that defines a series of smooth undulations that are shaped so as to define alternating curved peaks and curved valleys, which curved peaks extend in a direction away from the second longitudinal end and have a radius of curvature equal to at least 3% of a length of the first longitudinal end,

wherein the length of the first longitudinal end is measured around the longitudinal axis when the structural member is in the relaxed state, and

wherein the structural member comprises a plurality of stent struts, and wherein, if the structural member is unrolled to the planar shape, at least one of the stent struts extends completely alongside at least two of the undulations, such that the strut substantially prevents longitudinal stretching of the at least two of the undulations.

2. The apparatus according to claim 1, wherein the corrugated profile has a substantially sinusoidal form.

3. The apparatus according to claim 1, wherein the at least one of the stent struts geometrically encompasses at least one straight line segment that is parallel to the one side and extends completely alongside the at least two of the undulations, when the structural member has the planar shape.

4. The apparatus according to claim 1, wherein the at least one of the stent struts is straight when the structural member has the planar shape.

5. The apparatus according to claim 1, wherein, when the structural member has the planar shape, the at least one stent strut has a length, measured in a direction parallel to the one side, equal to at least 90% of a length of the one side.

19

6. The apparatus according to claim 1, wherein the profile defines the series of curves interspersed with one or more straight portions.

7. The apparatus according to claim 1,
wherein, if the structural member is unrolled to the planar shape, the length of the first longitudinal end is equal to between 30 and 120 mm, and

wherein the elongate hollow shape has a longitudinal length, measured parallel to the longitudinal axis of the elongate hollow shape, that equals between 10 and 40 mm.

8. The apparatus according to claim 1,
wherein the structural member, when having the elongate hollow shape, is shaped so as to define a gap that extends longitudinally along an entire longitudinal length of the elongate hollow shape from the first longitudinal end to the second longitudinal end, and wherein the structural member is shaped so as to define (a) a first extension, which first extension defines at least one slot, and (b) a second extension, which is shaped so as to define a tab adapted to fit into the at least one slot, such that inserting the tab into the slot closes the gap.

9. The apparatus according to claim 1,
wherein the structural member, when having the elongate hollow shape, is shaped so as to define a gap that extends longitudinally along an entire longitudinal length of the elongate hollow shape from the first longitudinal end to the second longitudinal end, and wherein the extra-vascular ring further comprises one or more fastening elements for closing the gap.

10. The apparatus according to claim 1, further comprising a hollow, generally tubular delivery shaft, in which the extra-vascular ring is removably disposed with the structural member in a deformed state.

11. The apparatus according to claim 1, wherein the structural member comprises a shape memory material, which is heat-set to assume the elongate hollow shape.

12. A method comprising:

providing an extra-vascular ring, which includes a structural member, which is configured to assume, when in a relaxed state, an elongate hollow shape, which has first and second longitudinal ends that are curved at least partially around a longitudinal axis defined by the elongate hollow shape, wherein, if the structural member is unrolled to a planar shape, one side of the planar shape is defined by the first longitudinal end of the structural member, and at least the first longitudinal end has a profile that defines a series of curved portions and has no singularities or discontinuities, which profile extends along at least 50% of the first longitudinal end; wherein the profile is a corrugated profile that defines a series of smooth undulations that are shaped so as to define alternating curved peaks and curved valleys, which curved peaks extend in a direction away from the second longitudinal end and have a radius of curvature equal to at least 3% of a length of the first longitudinal end; wherein the length of the first longitudinal end is measured around the longitudinal axis when the structural member is in the relaxed state; and wherein the structural member comprises a plurality of stent struts; and wherein, if the structural member is unrolled to the planar shape, at least one of the stent struts extends completely alongside at least two of the undulations, such that the strut substantially prevents longitudinal stretching of the at least two of the undulations;

20

placing the extra-vascular ring at least partially around a neck of an aneurysmal aorta of a patient so as to provide a generally cylindrical landing zone, such that the profile homogenously distributes strain on aortic tissue at the first longitudinal end of the structural member; and

placing an endovascular stent-graft inside the aorta such that a portion of the endovascular stent-graft is positioned against an internal wall of the neck at the landing zone provided by the structural member.

13. The method according to claim 12,
wherein placing the extra-vascular ring comprises advancing, to an external surface of the aorta, a hollow, generally tubular delivery shaft, in which the extra-vascular ring is removably disposed with the structural member in a deformed state, and

wherein advancing the delivery shaft comprises advancing the delivery shaft through a laparoscopic working channel to an abdominal location adjacent to renal arteries of the aorta, and laparoscopically placing the extra-vascular stent around the neck of the abdominal aorta in a vicinity of the renal arteries.

14. The method according to claim 12, wherein providing the extra-vascular ring comprises providing the extra-vascular ring in which the corrugated profile has a substantially sinusoidal form.

15. The method according to claim 12, wherein providing the extra-vascular ring comprises providing the extra-vascular ring in which the at least one of the stent struts geometrically encompasses at least one straight line segment that is parallel to the one side and extends completely alongside the at least two of the undulations, when the structural member has the planar shape.

16. The method according to claim 12, wherein providing the extra-vascular ring comprises providing the extra-vascular ring in which the at least one of the stent struts is straight when the structural member has the planar shape.

17. The method according to claim 12, wherein providing the extra-vascular ring comprises providing the extra-vascular ring in which, when the structural member has the planar shape, the at least one stent strut has a length, measured in a direction parallel to the one side, equal to at least 90% of a length of the one side.

18. The method according to claim 12, wherein providing the extra-vascular ring comprises providing the extra-vascular ring in which the profile defines the series of curved portions interspersed with one or more straight portions.

19. The method according to claim 12, wherein placing the extra-vascular ring comprises advancing, to an external surface of the aorta, a hollow, generally tubular delivery shaft, in which the extra-vascular ring is removably disposed with the structural member in a deformed state.

20. The method according to claim 12, wherein placing the extra-vascular ring comprises identifying the patient as suffering from an aneurysm of an abdominal aorta, and treating the aortic aneurysm by placing the extra-vascular ring at least partially around the neck of the abdominal aorta.

21. The method according to claim 12, wherein providing the extra-vascular ring comprises providing the extra-vascular ring in which the structural member comprises a shape memory material, which is heat-set to assume the elongate hollow shape.

专利名称(译)	减少血管外环用于治疗主动脉瘤		
公开(公告)号	US9486341	公开(公告)日	2016-11-08
申请号	US14/001641	申请日	2012-03-01
[标]申请(专利权)人(译)	SHALEV ALON		
申请(专利权)人(译)	SHALEV , ALON		
当前申请(专利权)人(译)	ENDOSPAN LTD.		
[标]发明人	SHALEV ALON		
发明人	SHALEV , ALON		
IPC分类号	A61F2/93 A61F2/07 A61B17/12 A61F2/89		
CPC分类号	A61F2/93 A61F2/07 A61B17/12013 A61F2/89 A61F2220/005 A61F2220/0025 A61F2220/0041 A61F2220/0066 A61F2220/0075 A61F2220/0083 A61F2230/0054		
代理机构(译)	萨格鲁MION , PLLC		
审查员(译)	MCEVOY , THOMAS		
优先权	61/448199 2011-03-02 US		
其他公开文献	US20140052236A1		
外部链接	Espacenet USPTO		

摘要(译)

提供了装置 (10) , 其包括血管外环 (12) 和血管内支架 - 移植物 (14) 。环 (12) 包括结构构件 (30) , 其构造成呈现细长的中空形状 (32) , 其具有第一个第二纵向端部 (40,42) , 并且适于至少部分地围绕主动脉放置 (20) , 以便提供大致圆柱形的着陆区。血管内支架移植物 (14) 适合于主动脉内血管内放置 (20) , 使得一部分支架移植物 (14) 在由结构构件提供的着陆区处 (30) 抵靠主动脉的内壁 (20) 定位。如果结构构件 (30) 展开为平面形状 (82) , 则平面形状 (90) 的一侧 (90) > 82) 由第一纵向末端 (40) 定义, 并且至少第一纵向末端 (40) 具有定义一系列的纵向末端的轮廓弯曲部分并且没有奇点或不连续性, 该轮廓沿第一纵向端部的至少50%延伸 (40) 。

