


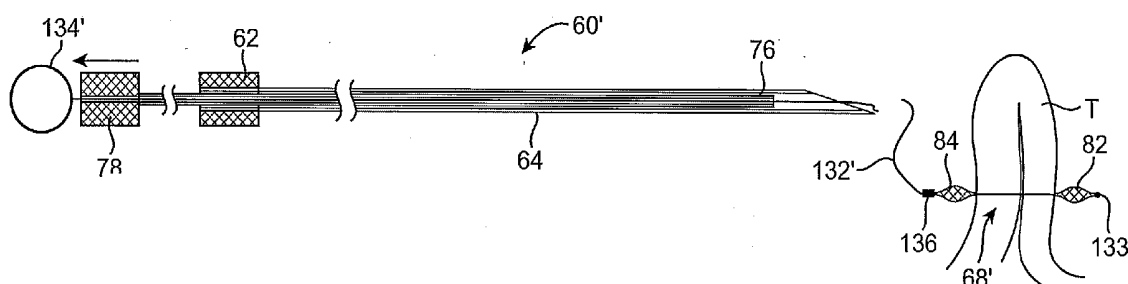

US 20060271074A1

(19) **United States**(12) **Patent Application Publication** (10) **Pub. No.: US 2006/0271074 A1**
(43) **Pub. Date: Nov. 30, 2006**
Ewers et al.(54) **METHODS AND APPARATUS FOR
SECURING AND DEPLOYING TISSUE
ANCHORS****Publication Classification**(51) **Int. Cl.**
A61B 17/04 (2006.01)
(52) **U.S. Cl.** **606/148**(76) Inventors: **Richard C. Ewers**, Fullerton, CA (US);
Cang C. Lam, Irvine, CA (US)Correspondence Address:
LEVINE BAGADE HAN LLP
2483 EAST BAYSHORE ROAD, SUITE 100
PALO ALTO, CA 94303 (US)(21) Appl. No.: **11/412,261**
(22) Filed: **Apr. 26, 2006****Related U.S. Application Data**(63) Continuation-in-part of application No. 11/238,543,
filed on Sep. 30, 2005, which is a continuation-in-part
of application No. 11/139,920, filed on May 26, 2005.(57) **ABSTRACT**

Methods and apparatus for securing and deploying tissue anchors are described herein. A tissue manipulation assembly is pivotably coupled to the distal end of a tubular member. A reconfigurable launch tube is also pivotably coupled to the tissue manipulation assembly, which may be advanced through a shape-lockable endoscopic device, a conventional endoscope, or directly by itself into a patient. A second tool can be used in combination with the tissue manipulation assembly to engage tissue and manipulate the tissue in conjunction with the tissue manipulation assembly. A deployment assembly is provided for securing engaged tissue via one or more tissue anchors, the deployment assembly also being configured to disengage the anchors endoluminally or laparoscopically by applying thermal energy through at least one suture cutting element disposed along the deployment assembly.



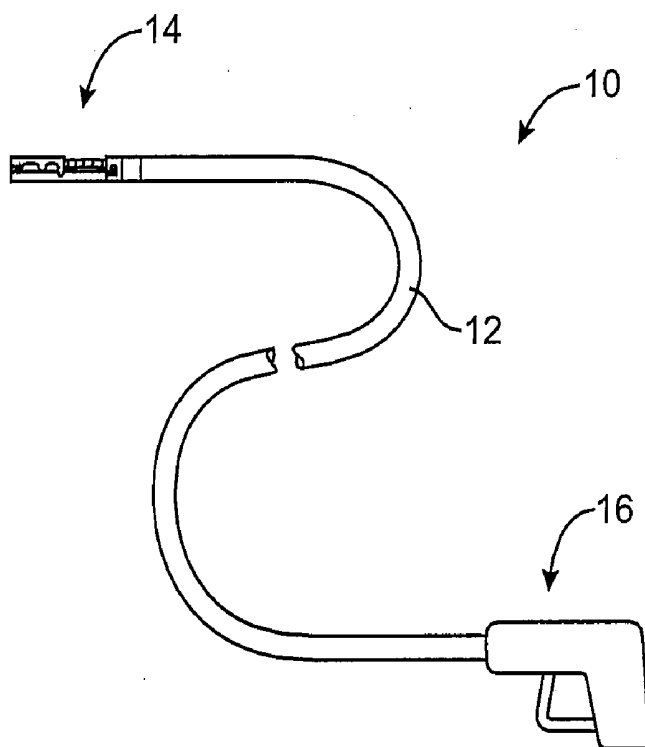


FIG. 1A

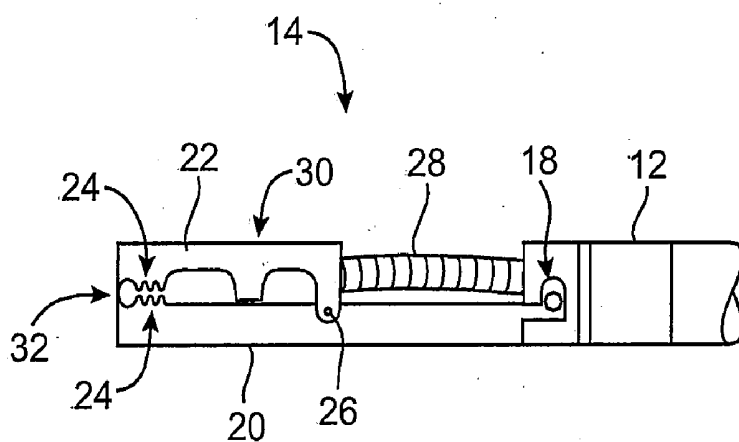


FIG. 1B

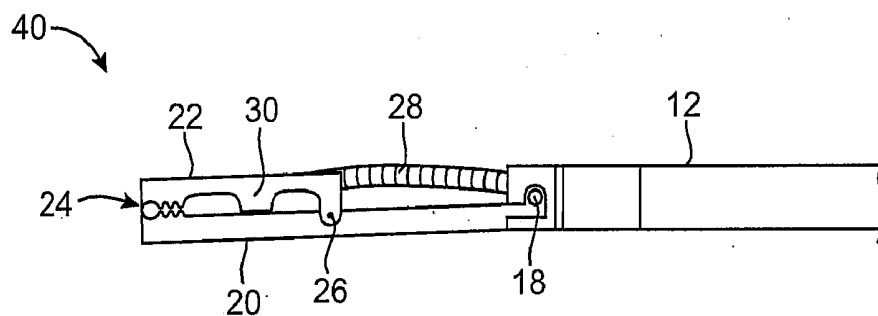


FIG. 2A

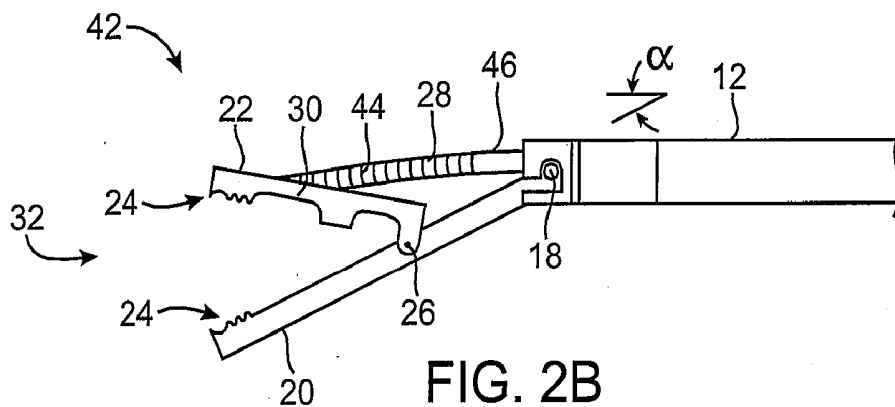


FIG. 2B

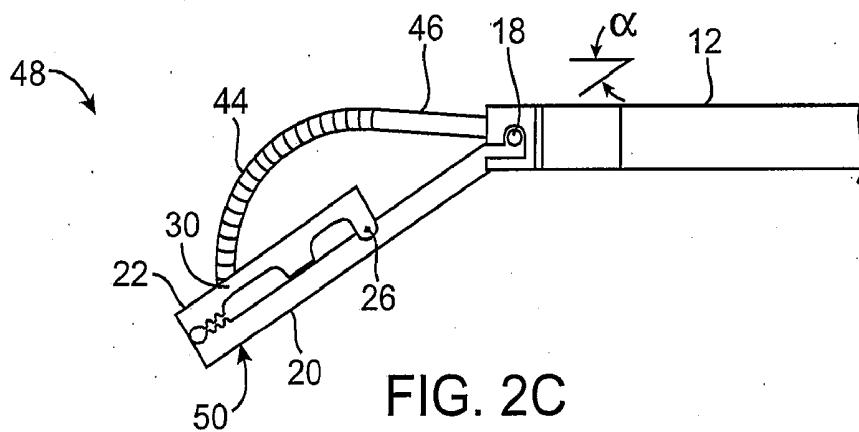


FIG. 2C

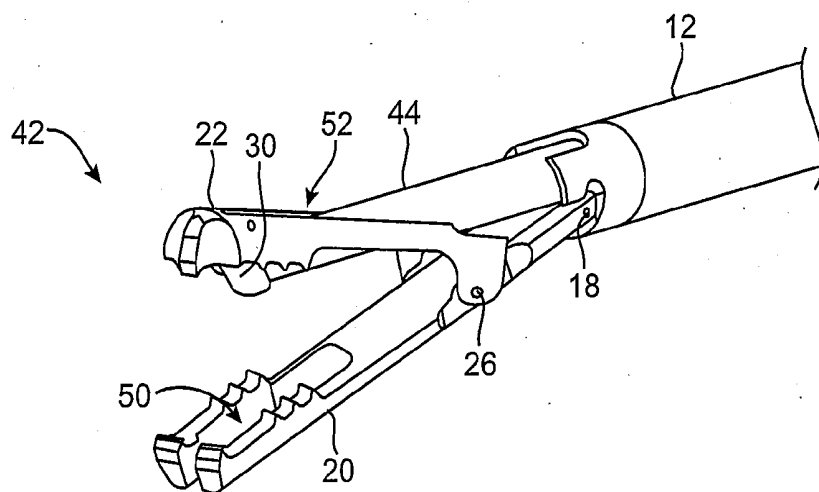


FIG. 3A

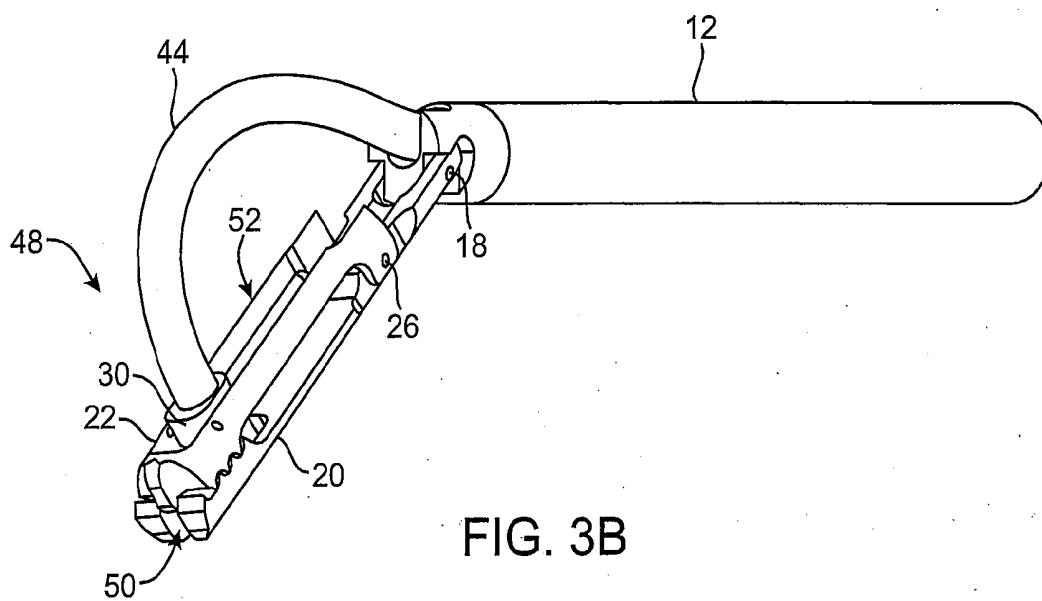


FIG. 3B

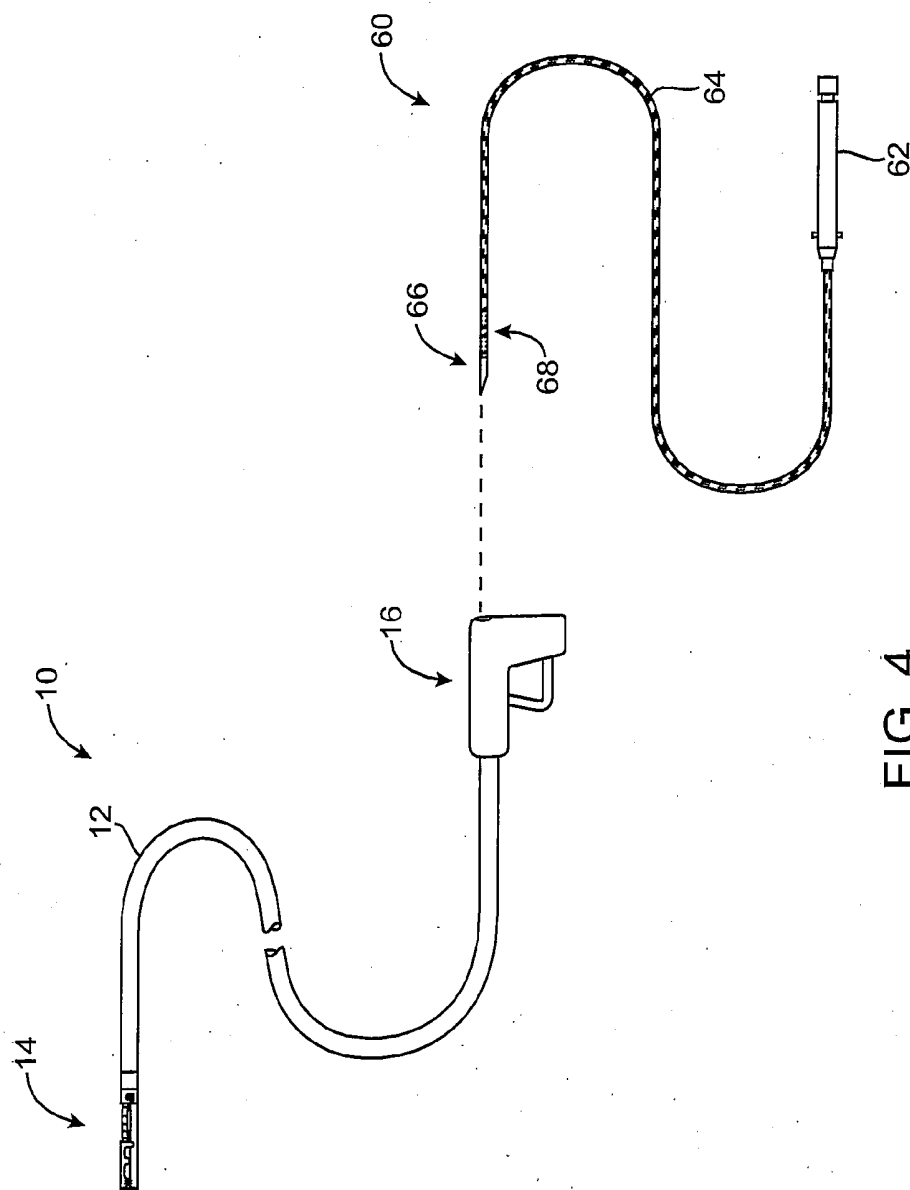


FIG. 4

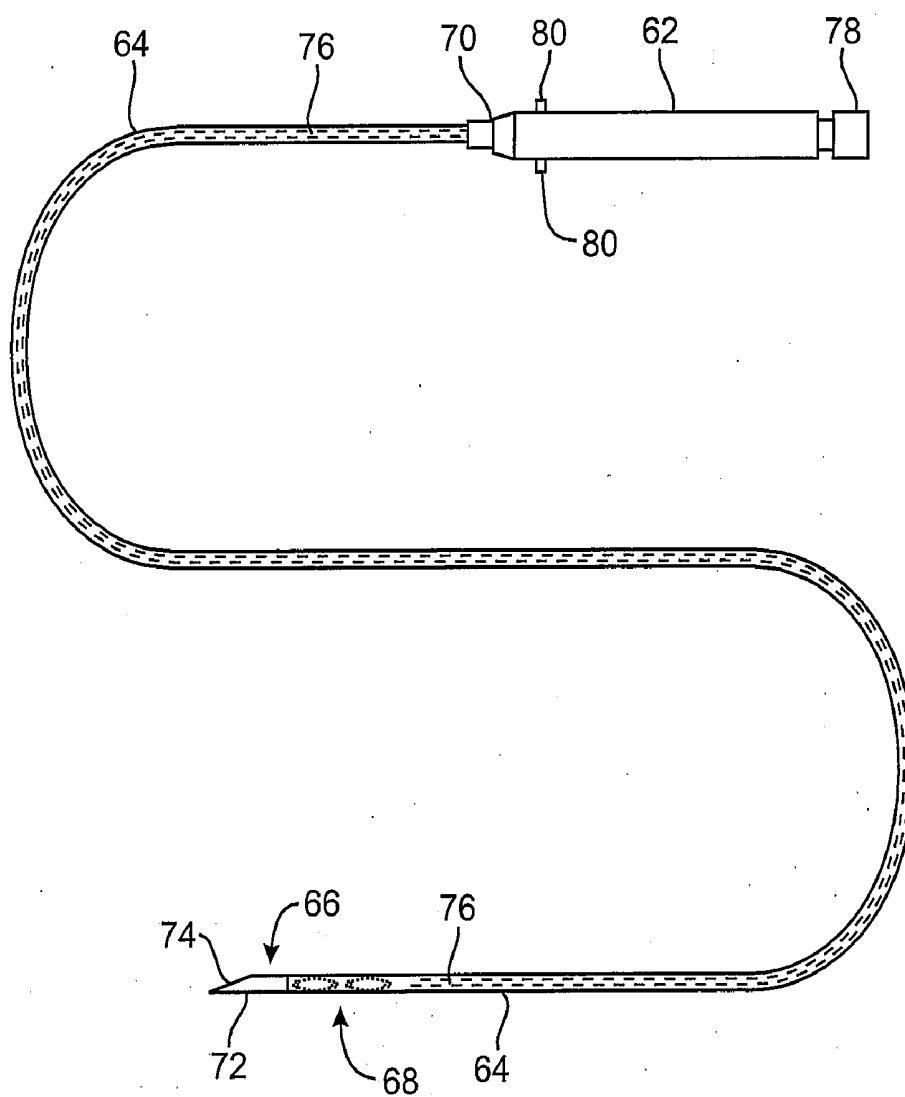


FIG. 5A

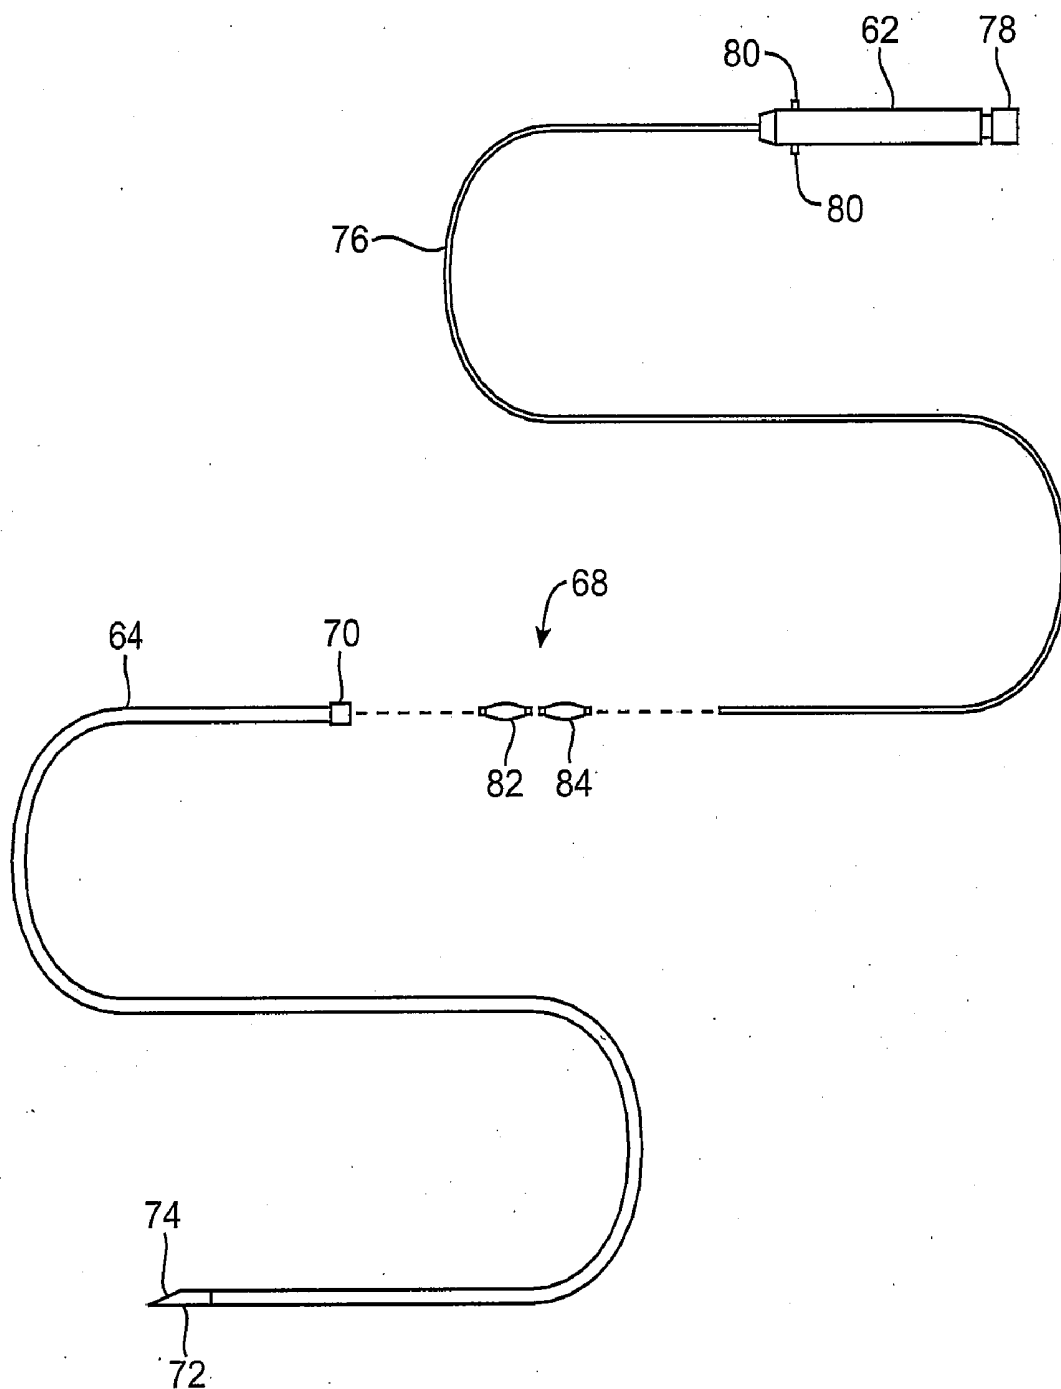


FIG. 5B

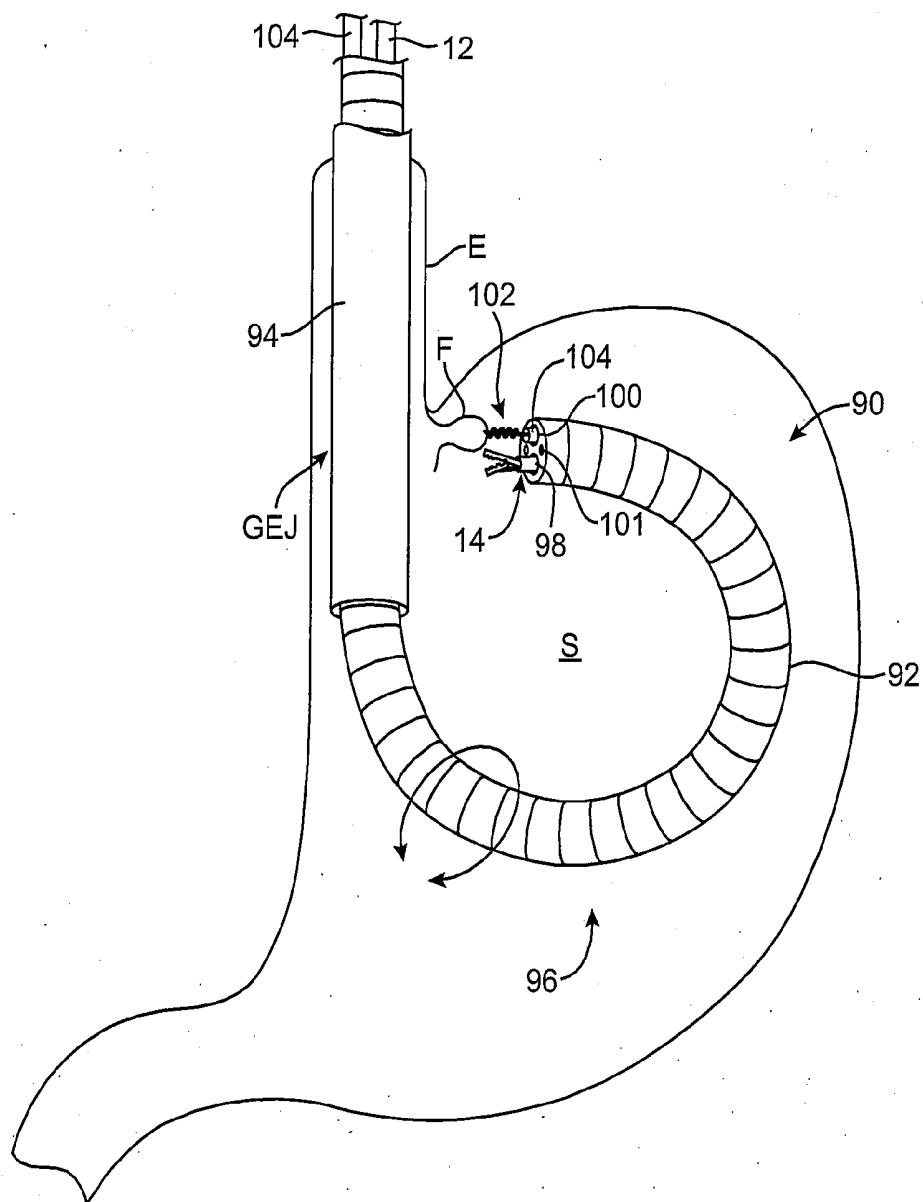


FIG. 6

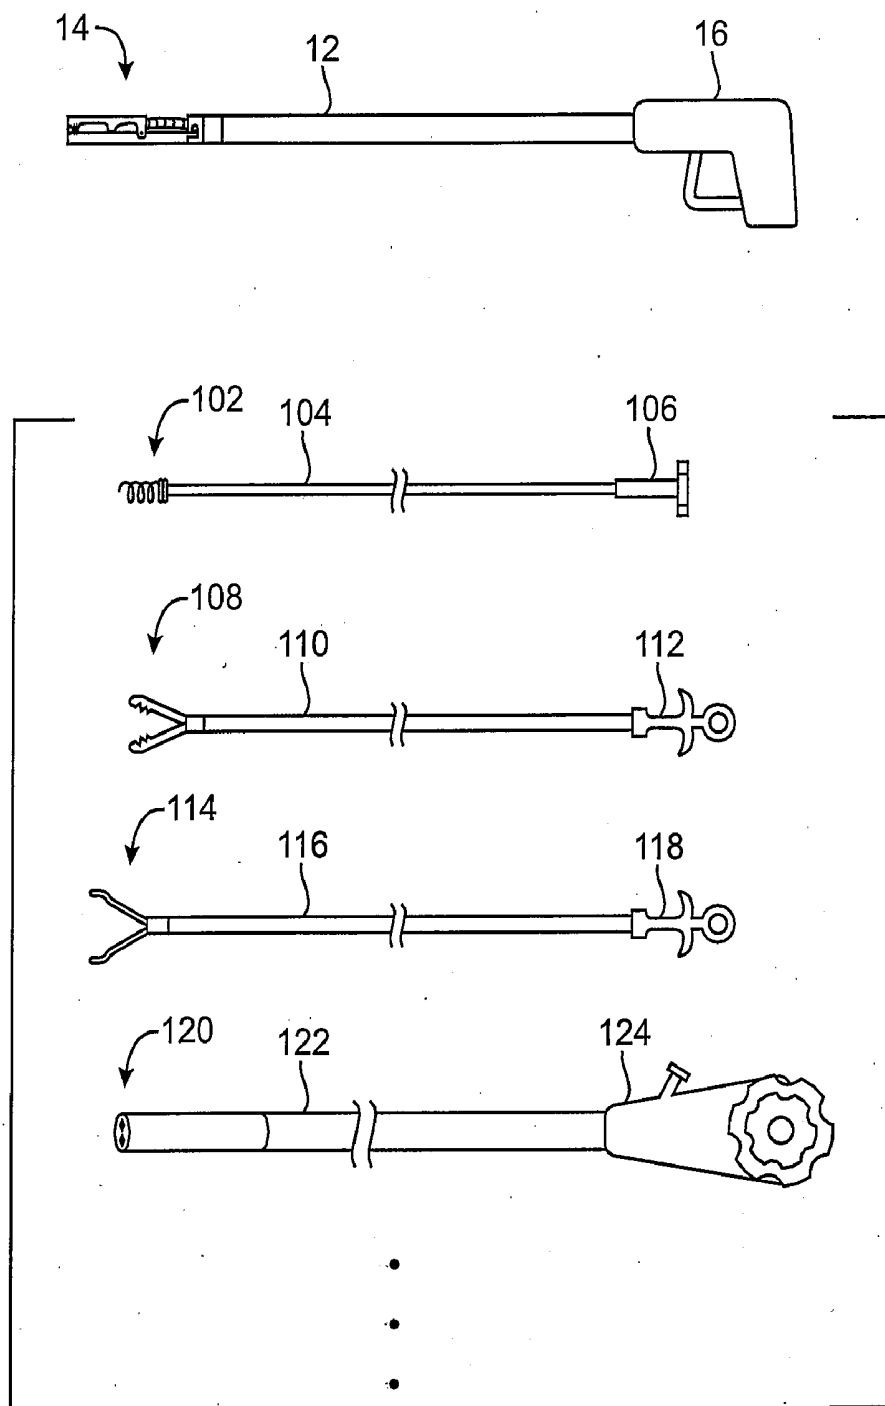


FIG. 7

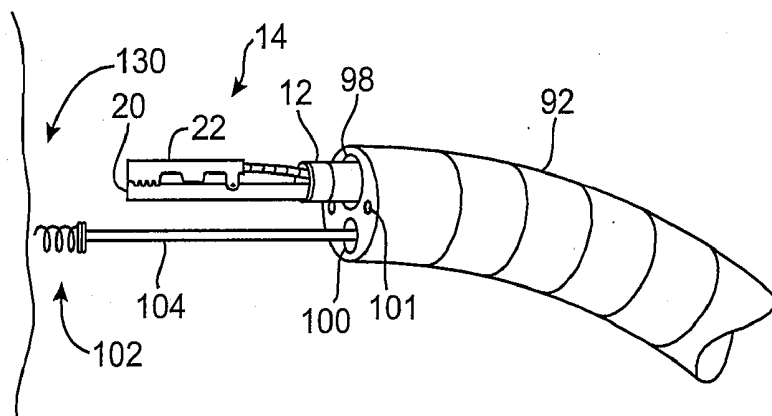


FIG. 8A

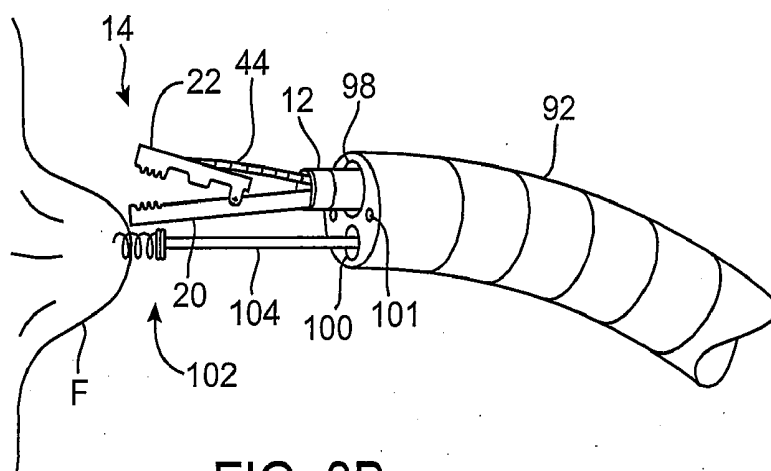


FIG. 8B

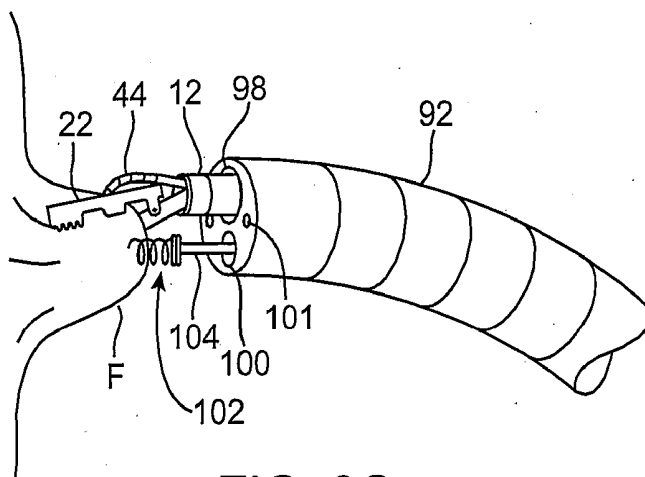


FIG. 8C

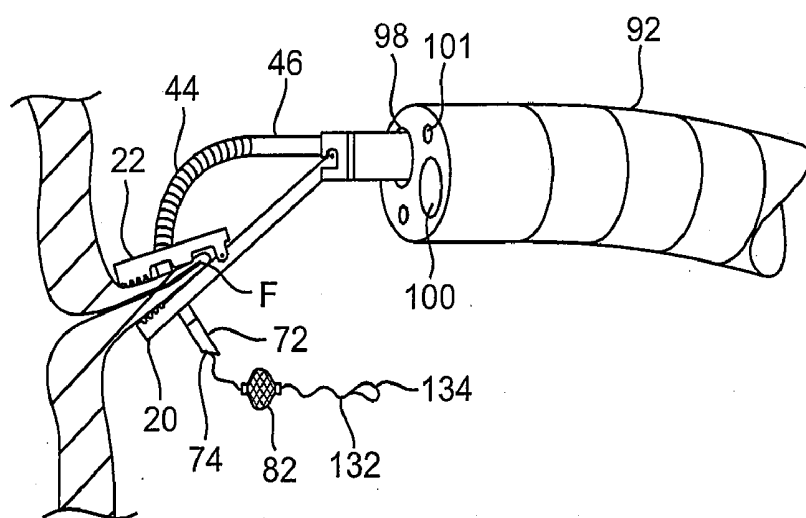


FIG. 8D

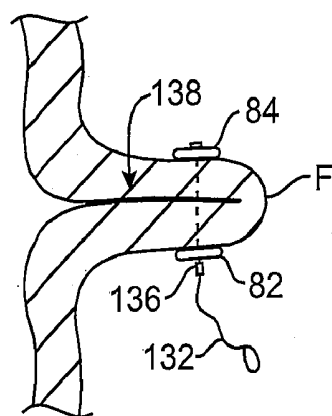


FIG. 9A

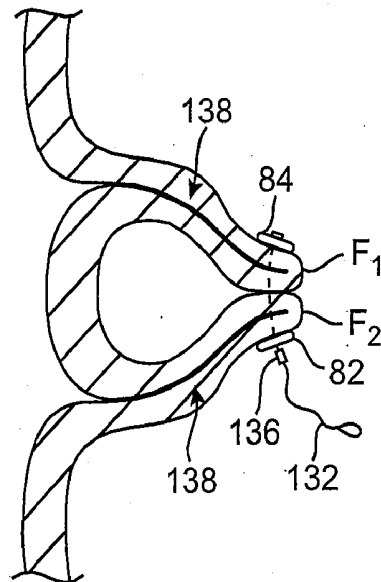
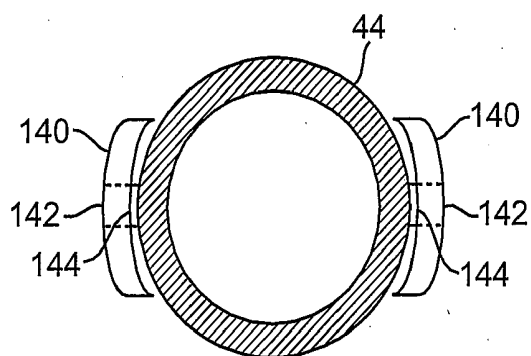
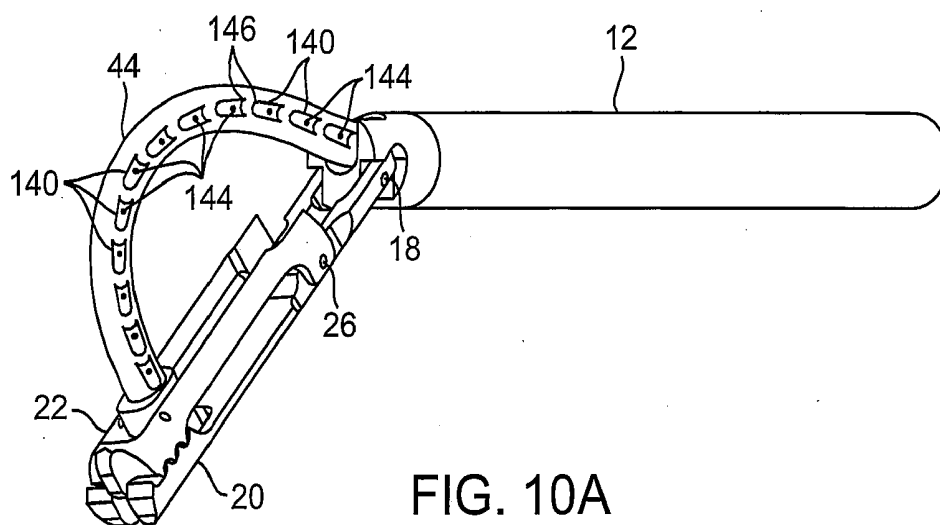


FIG. 9B



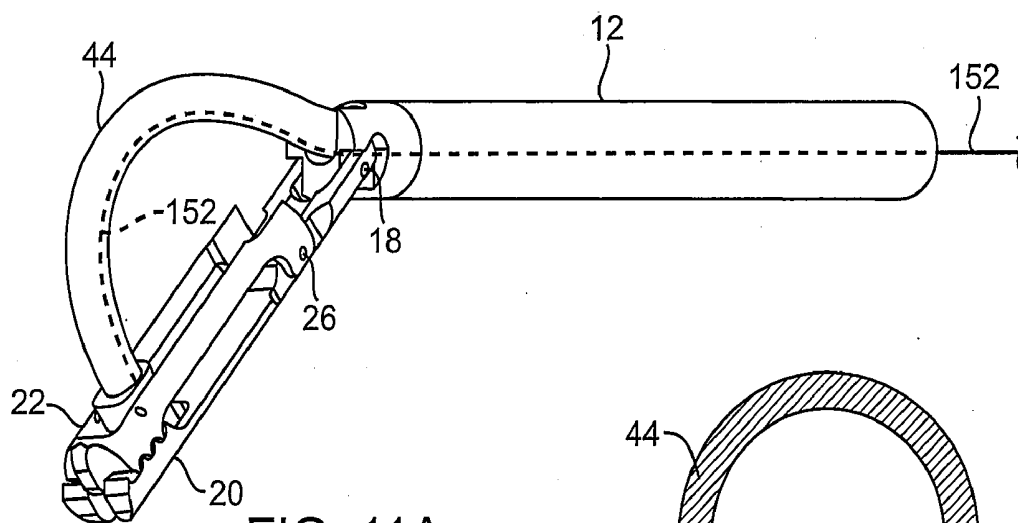


FIG. 11A

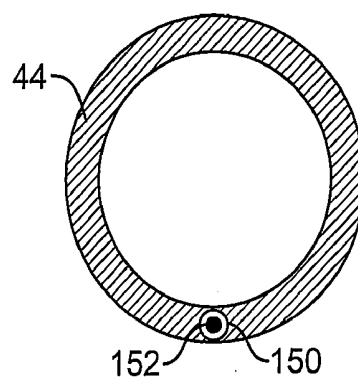


FIG. 11B

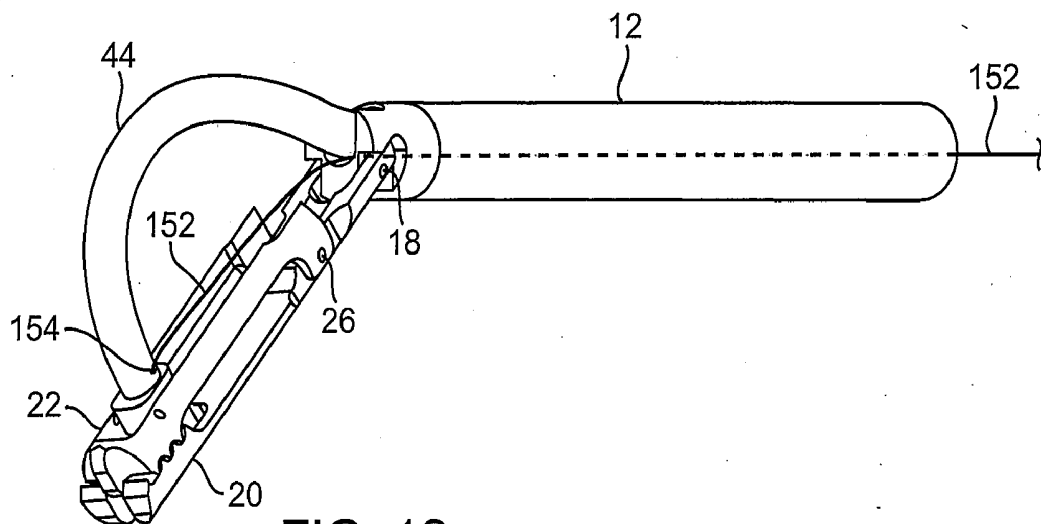
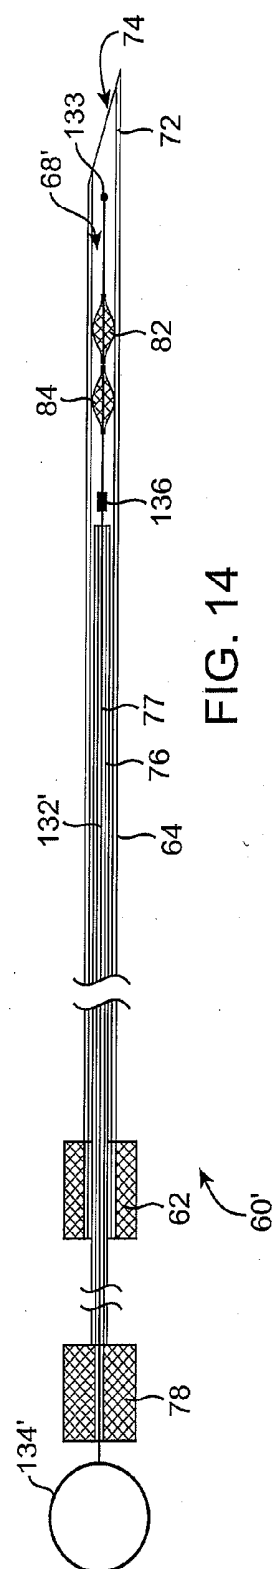
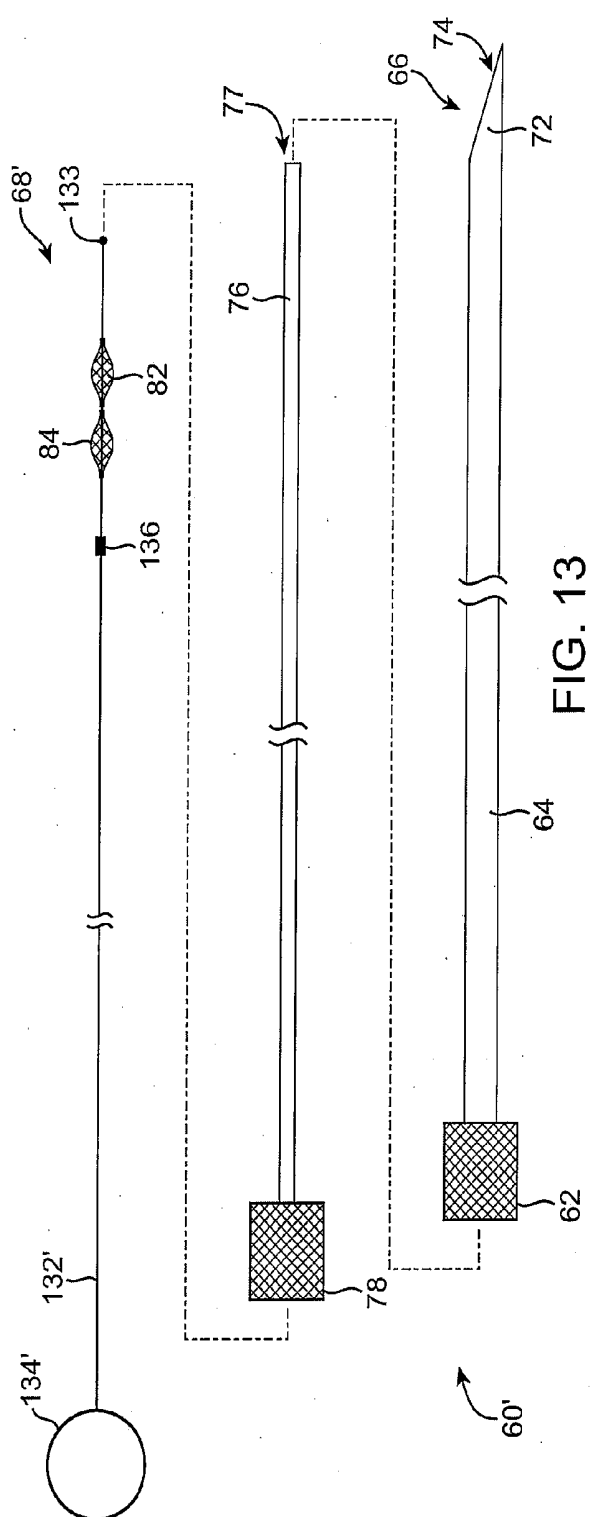
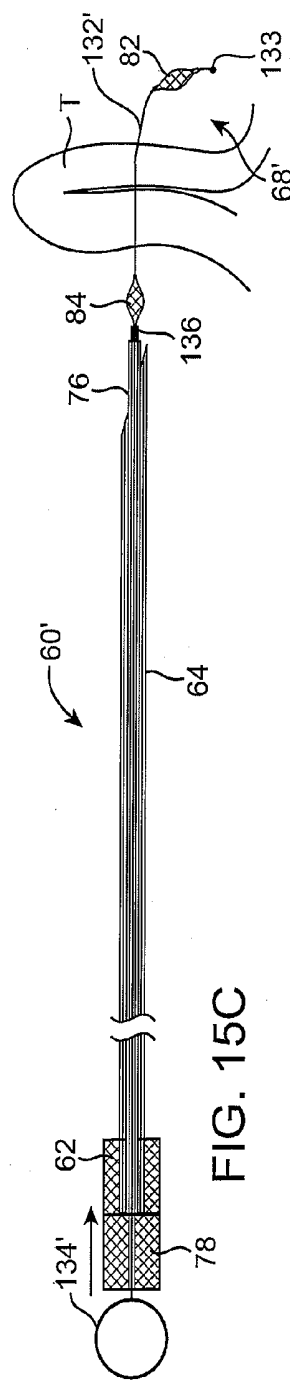
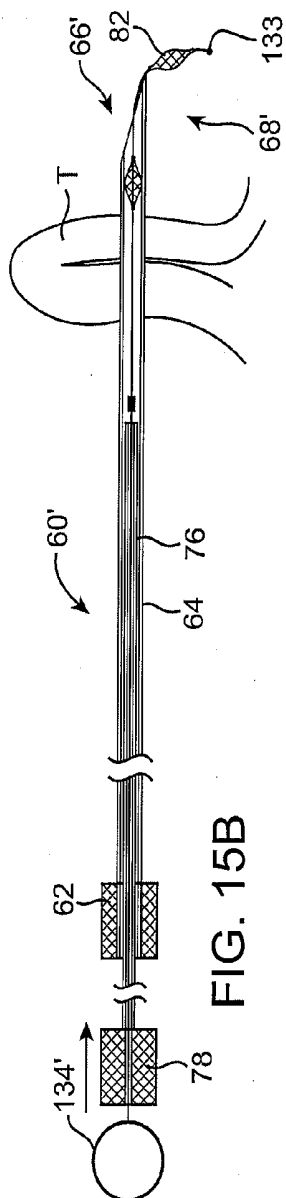
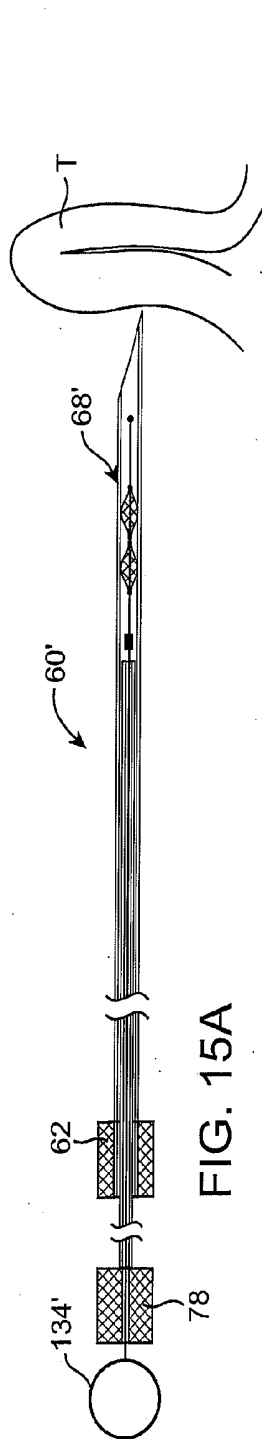
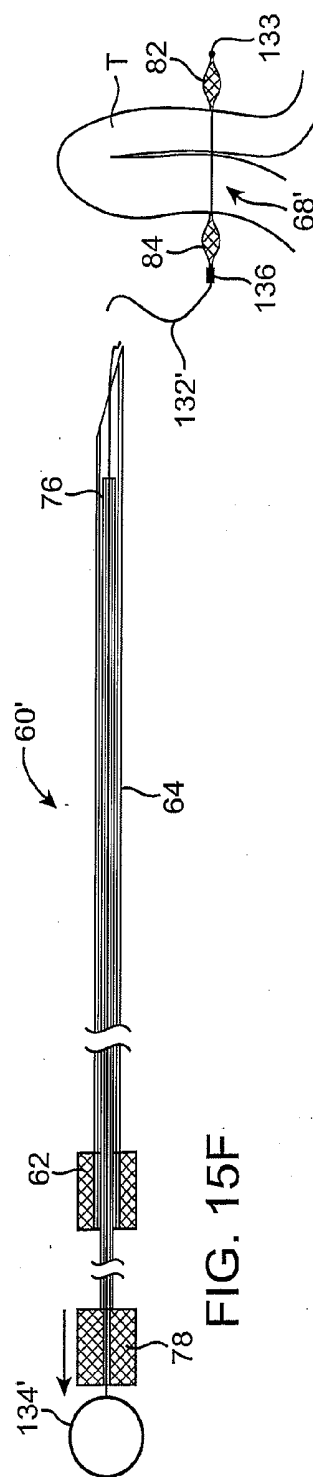
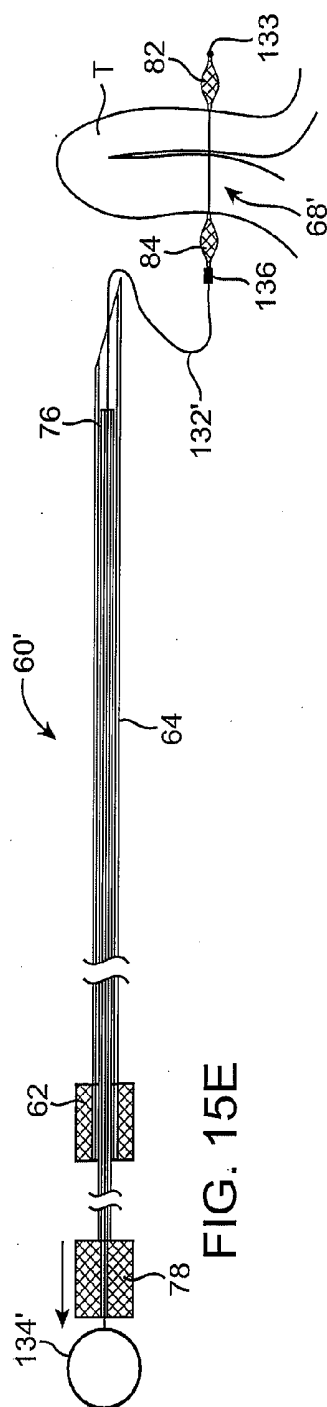
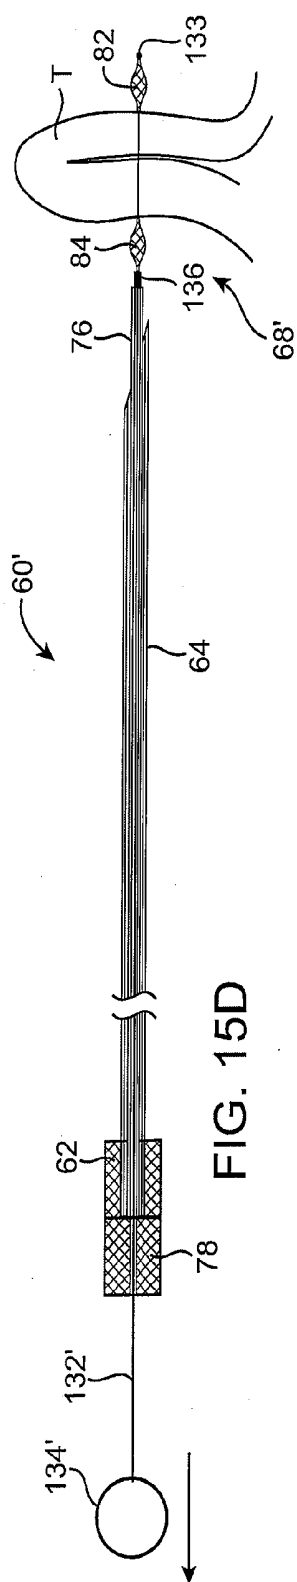


FIG. 12







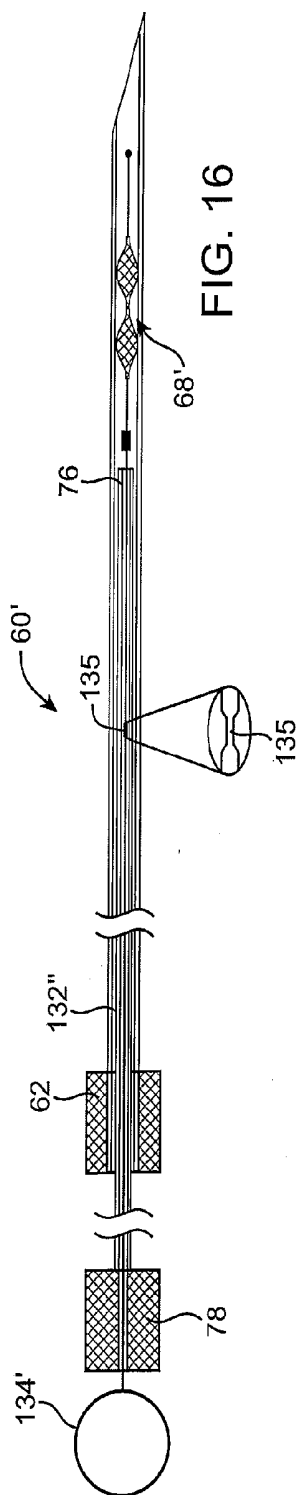


FIG. 16

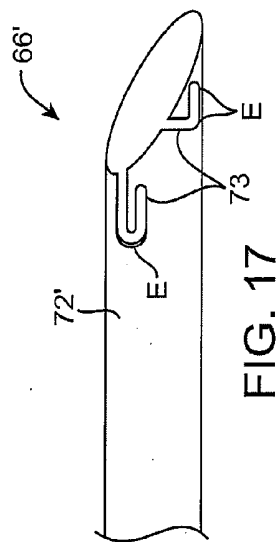


FIG. 17

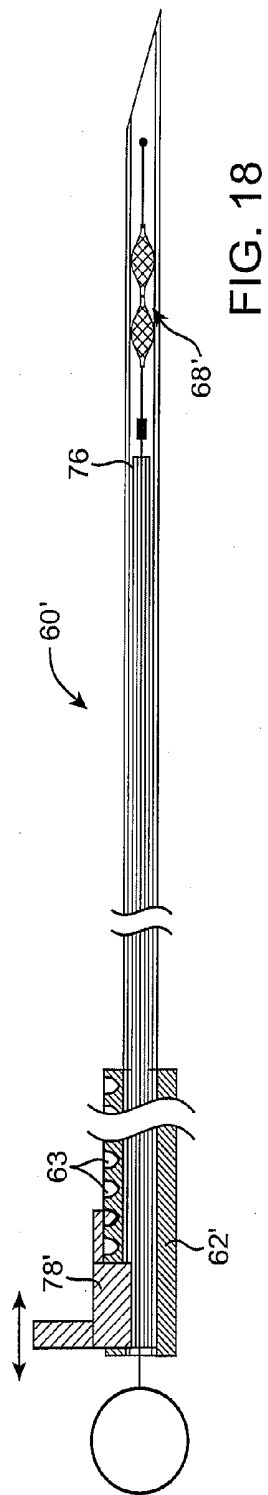
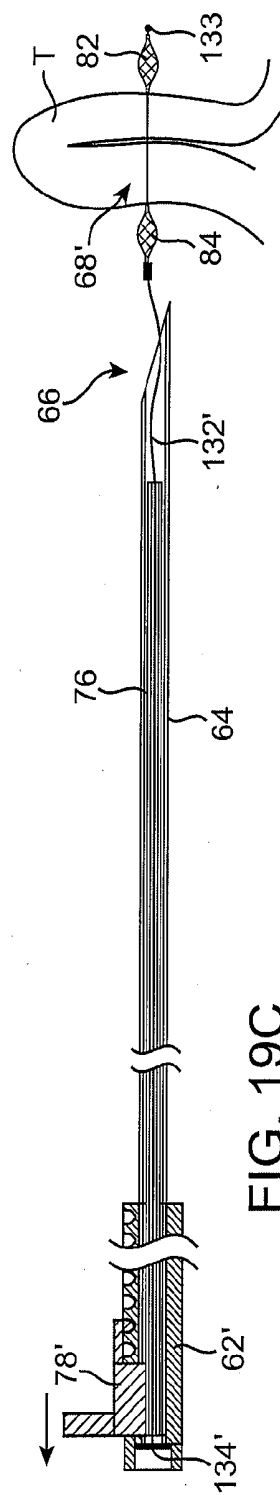
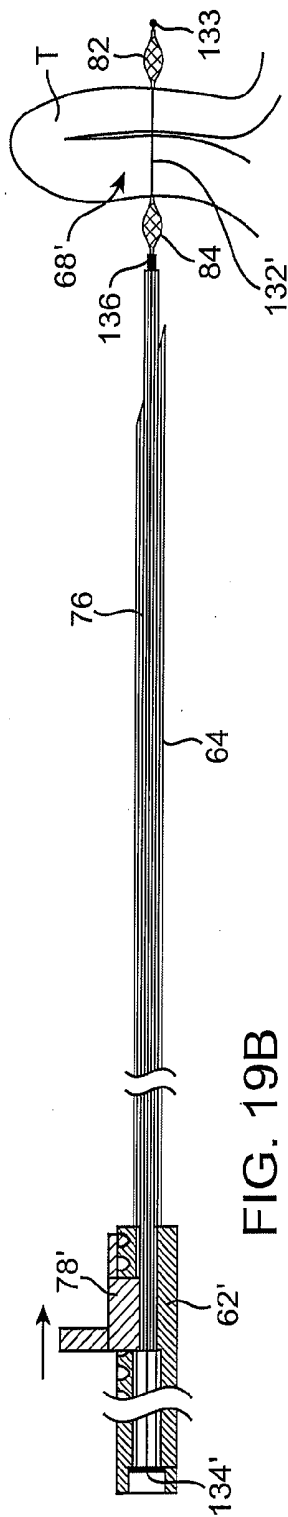
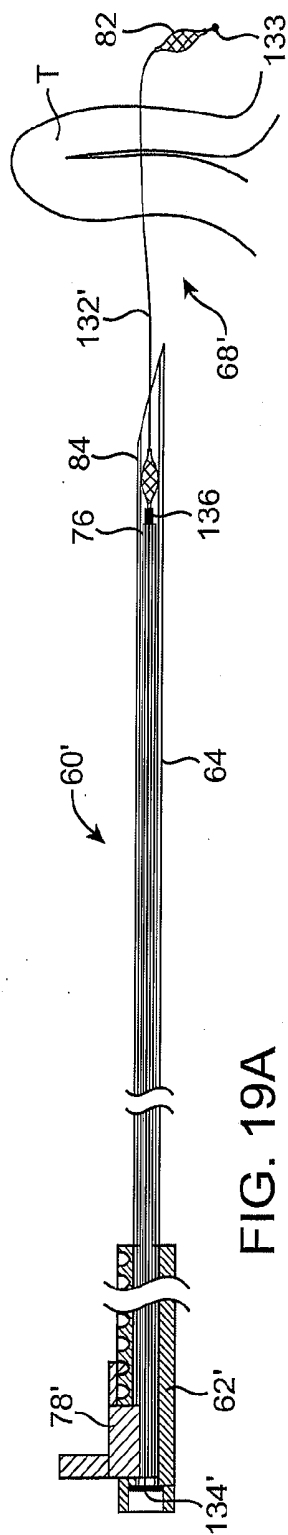


FIG. 18



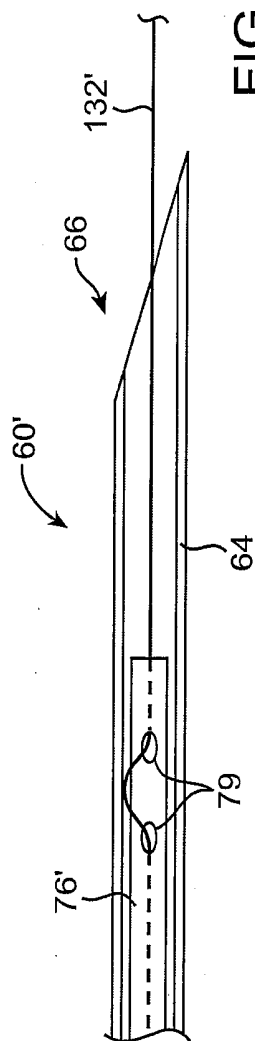


FIG. 20A

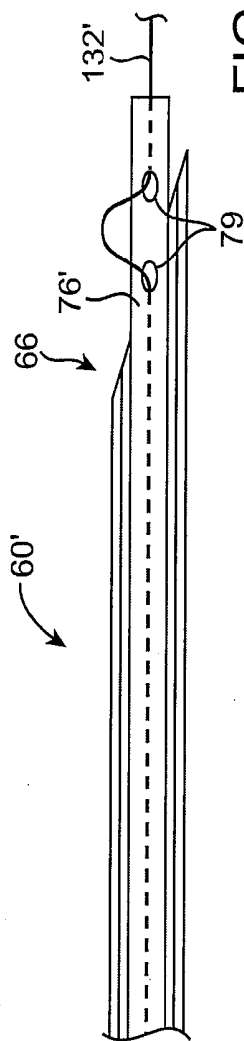


FIG. 20B

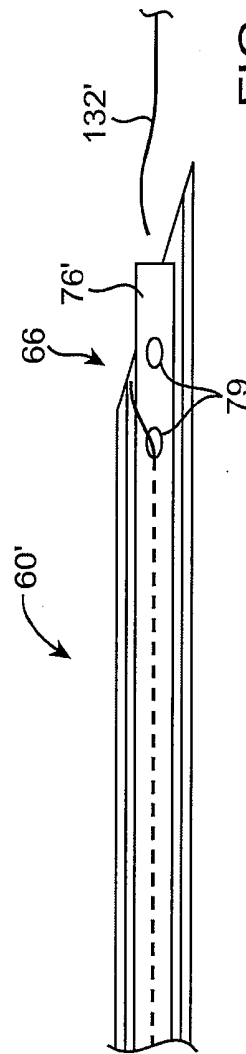
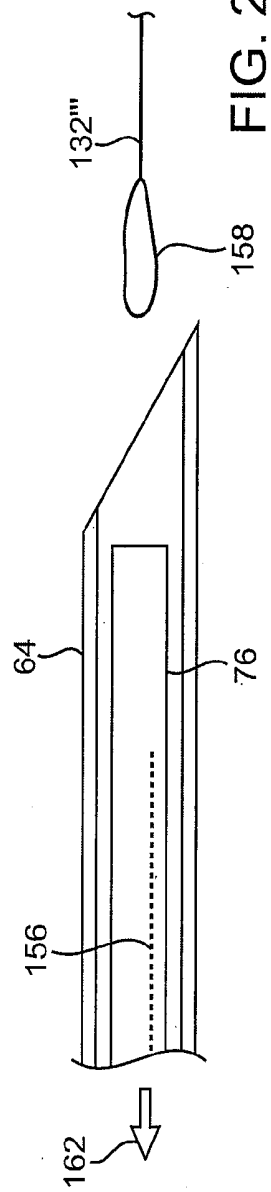
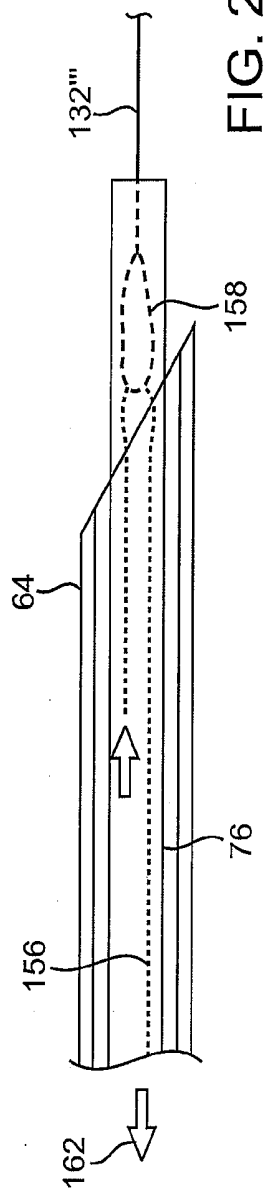
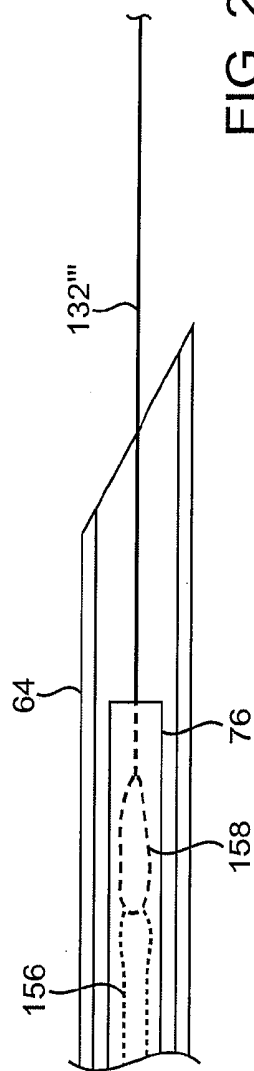
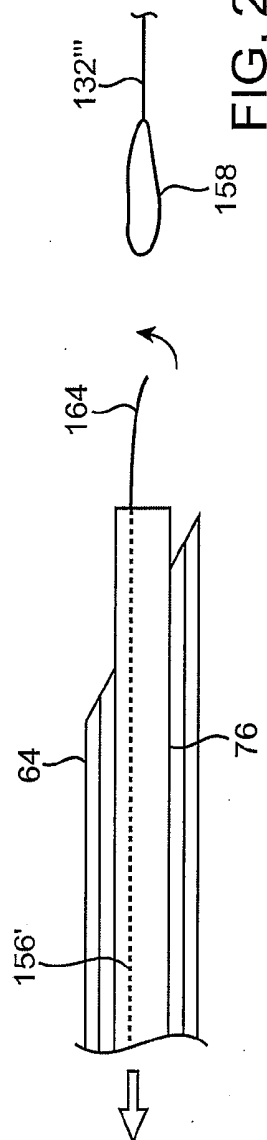
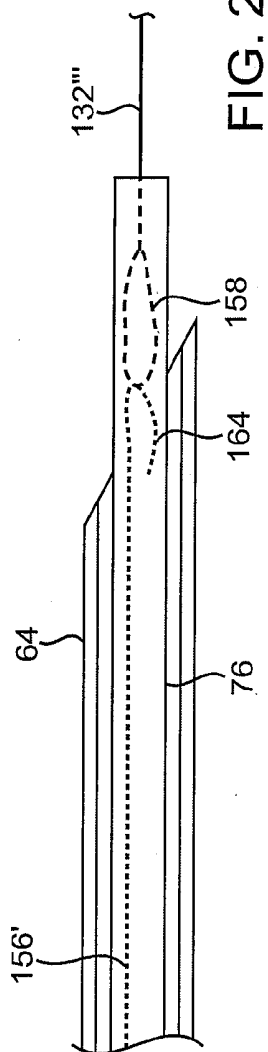
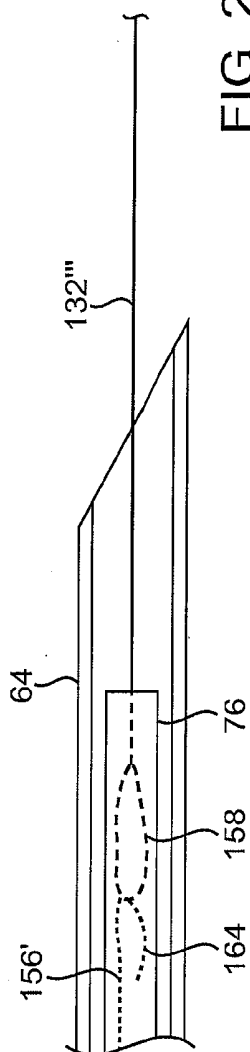
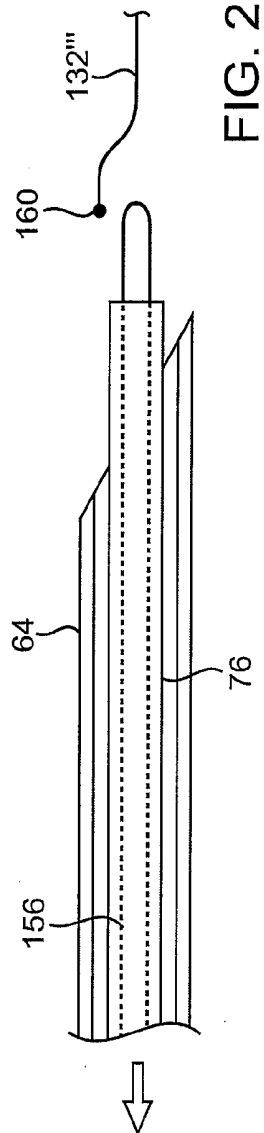
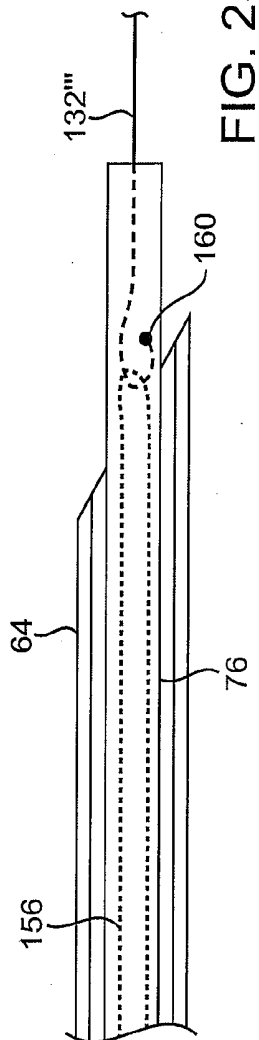
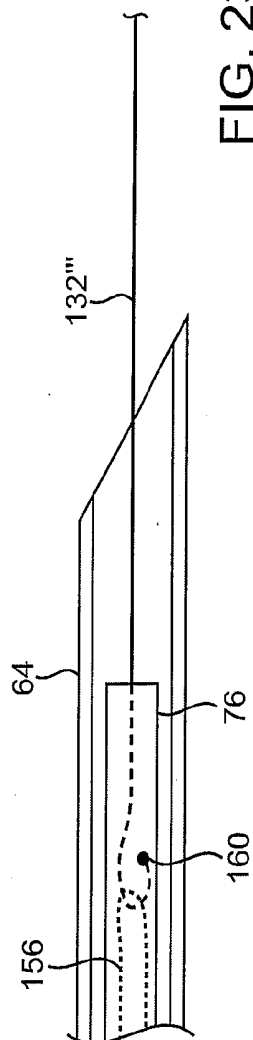


FIG. 20C







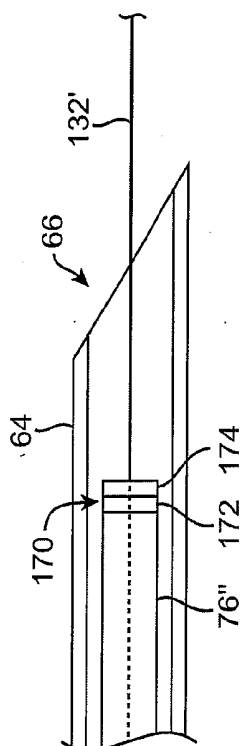


FIG. 24A

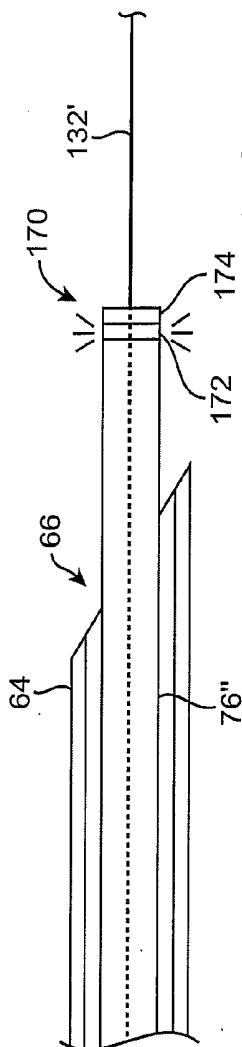


FIG. 24B

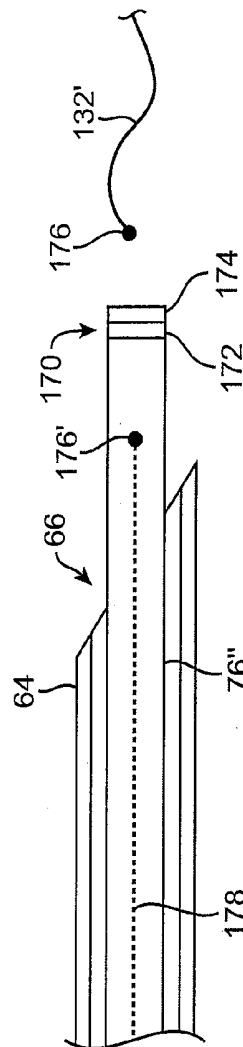


FIG. 24C

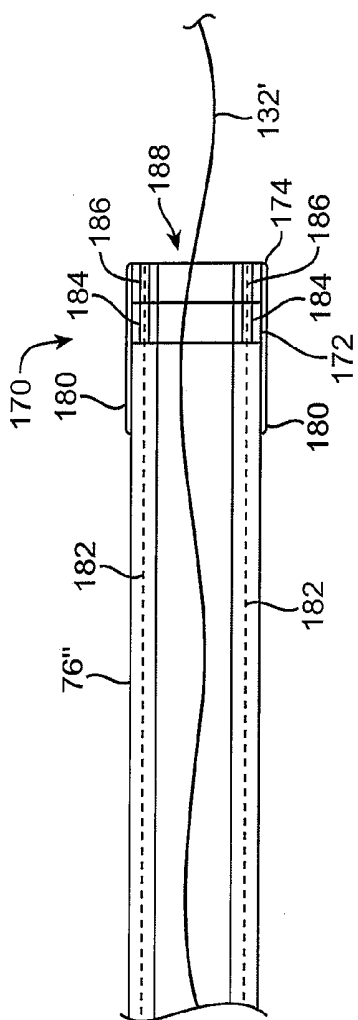


FIG. 25A

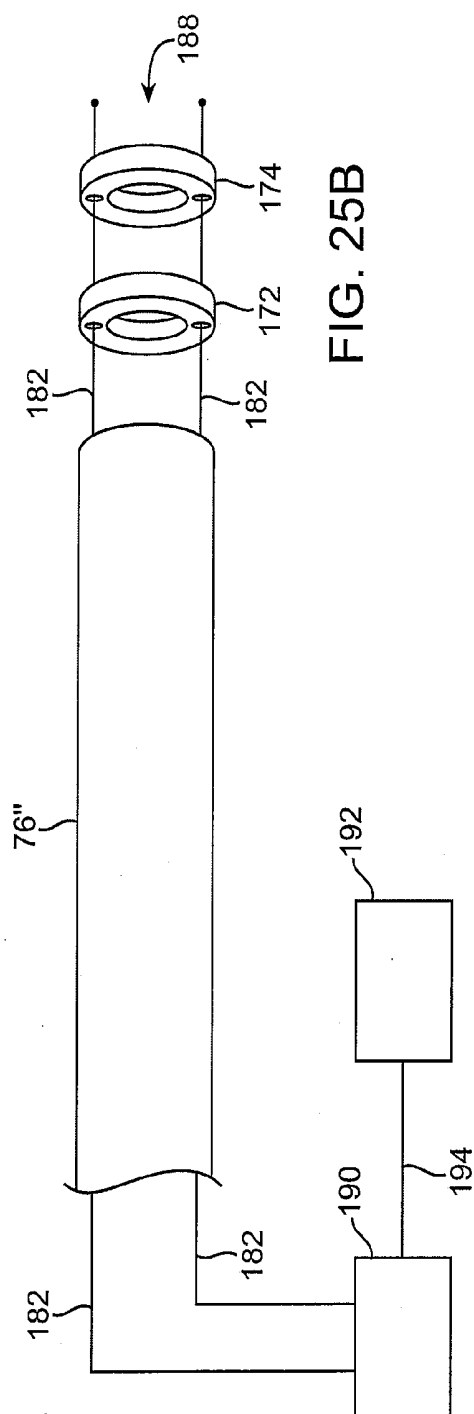


FIG. 25B

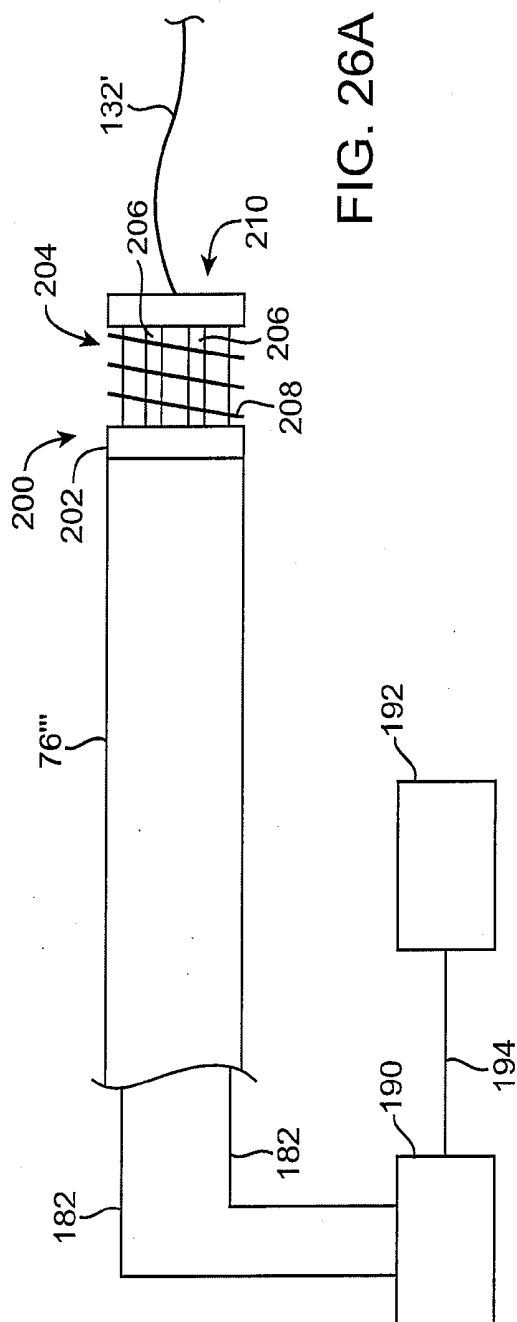


FIG. 26A

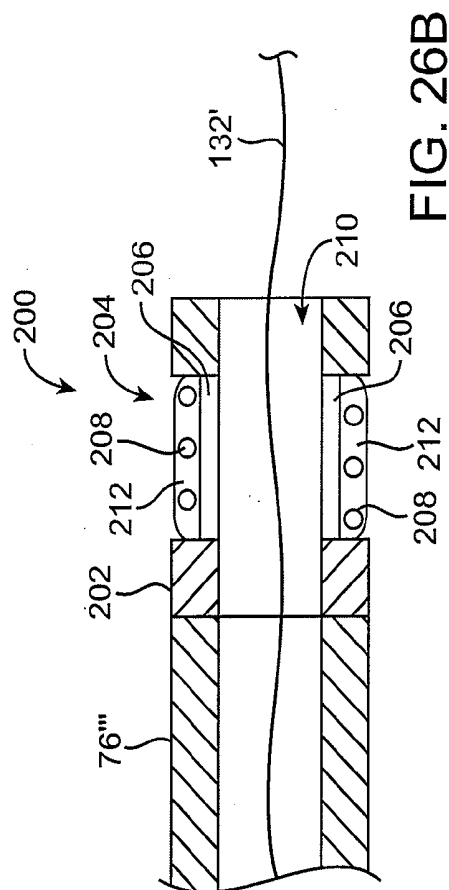
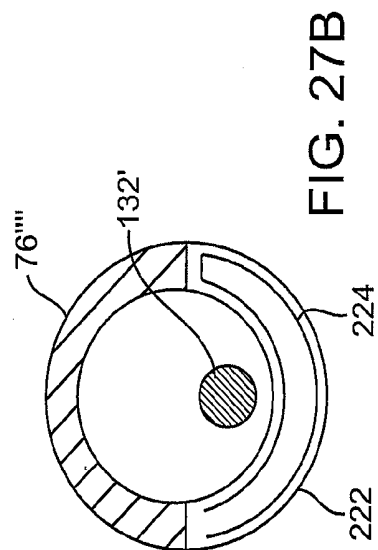
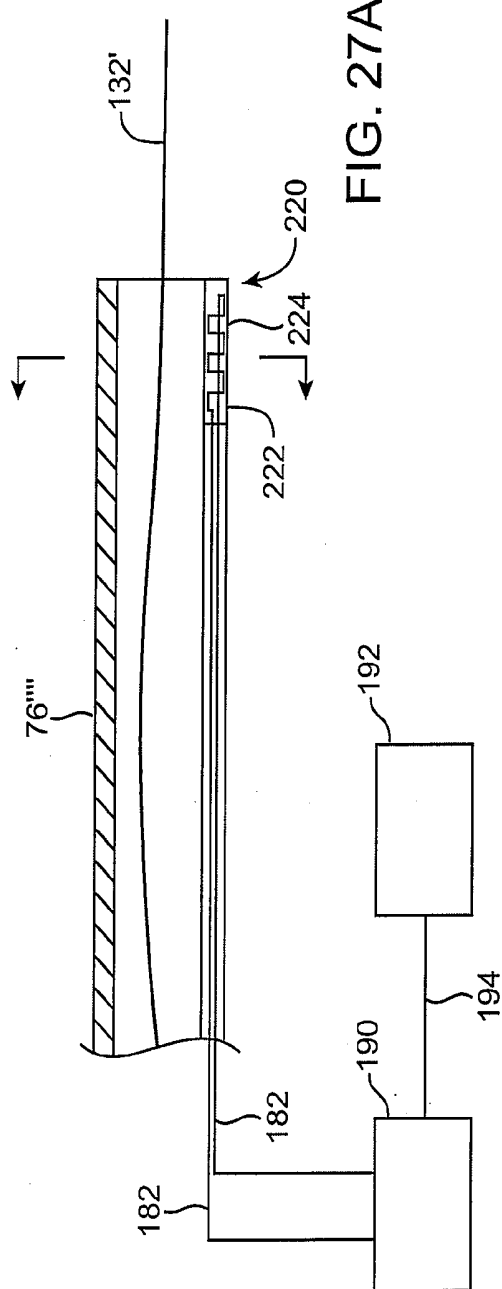


FIG. 26B



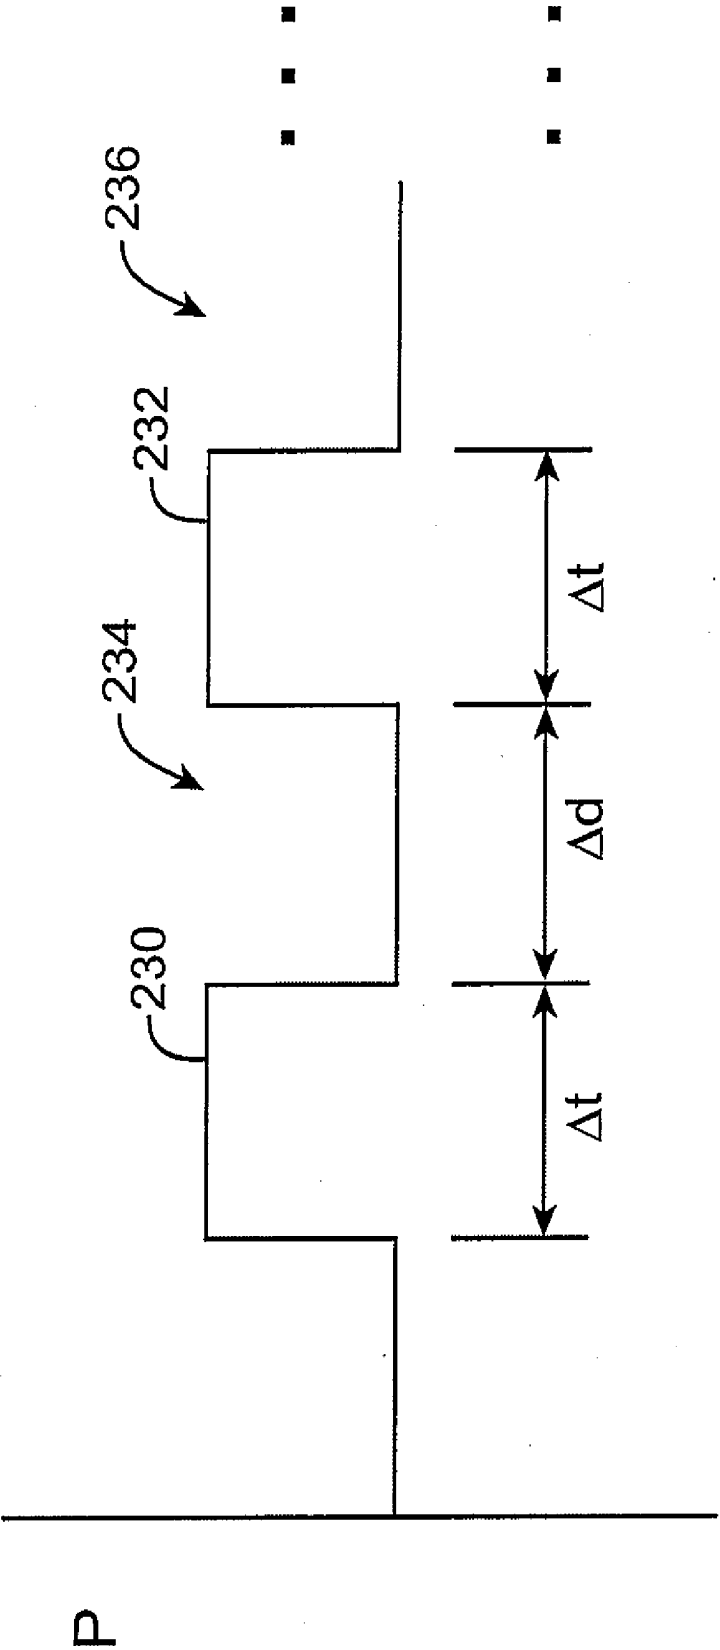


FIG. 28

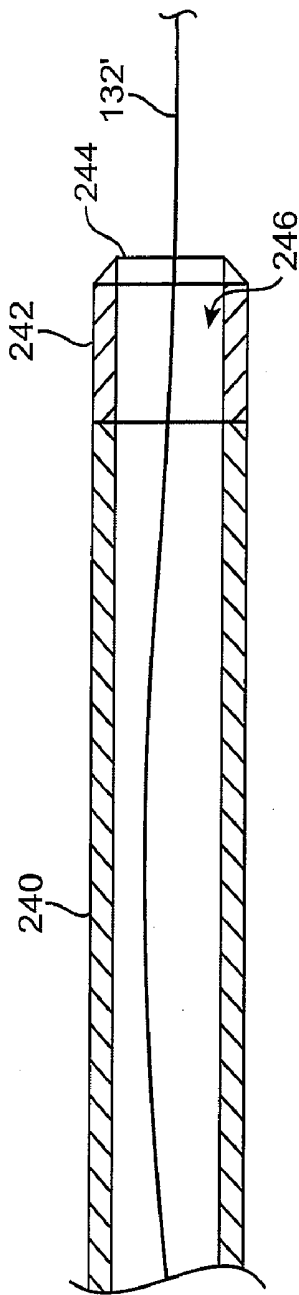


FIG. 29A

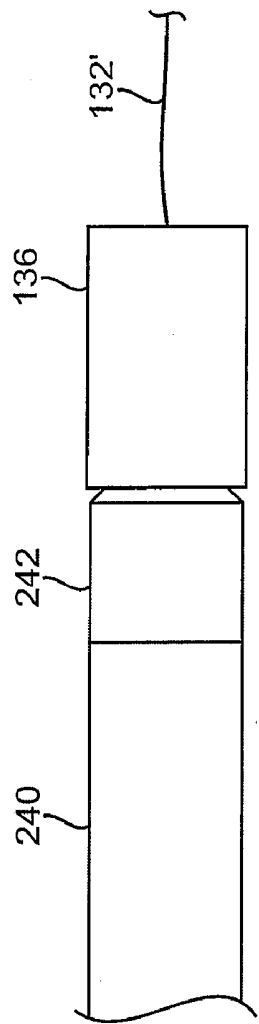
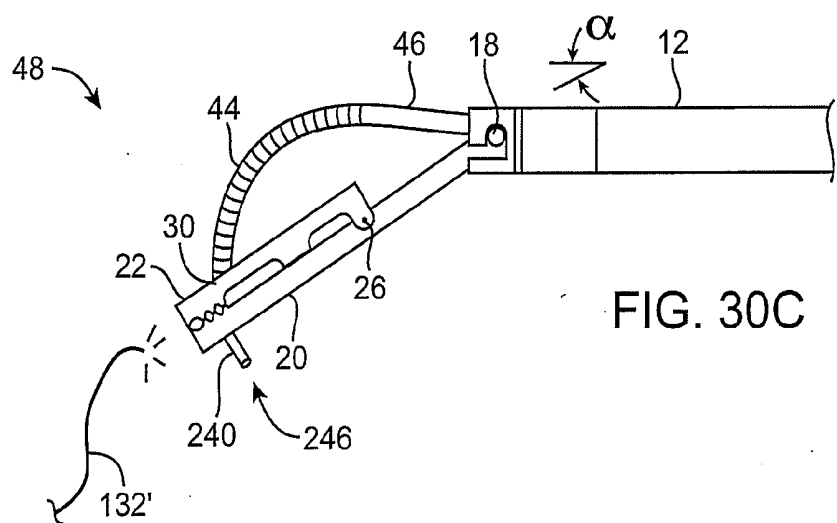
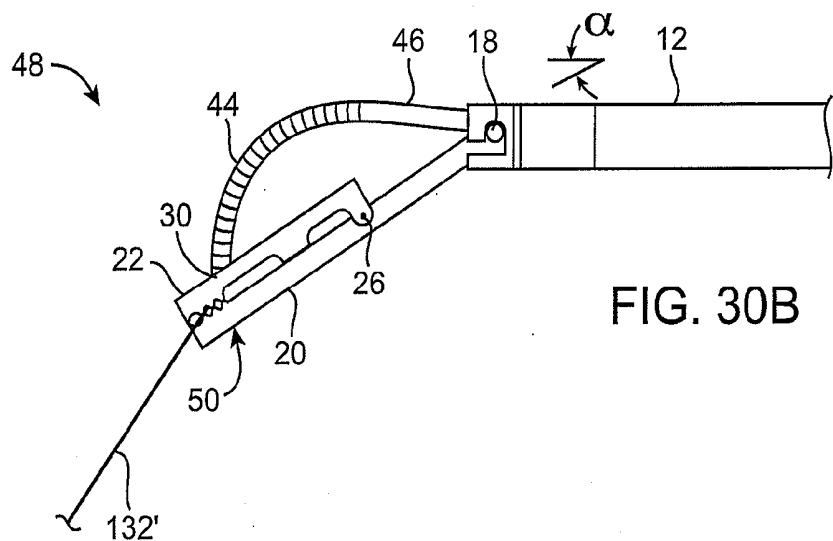
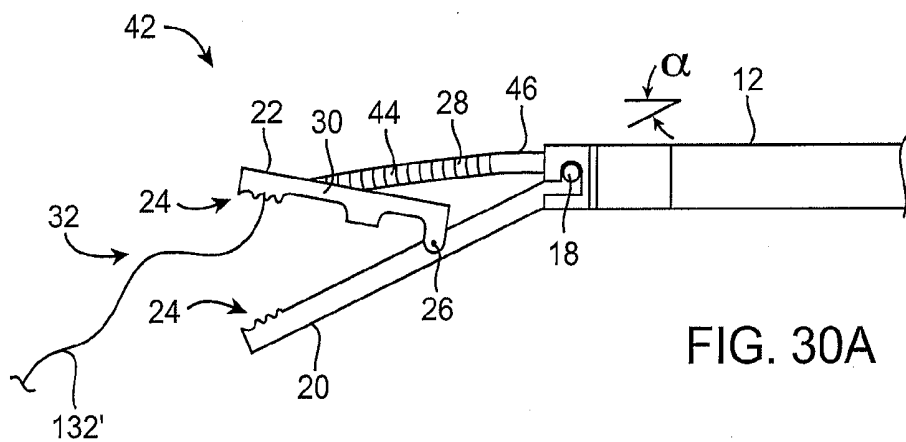
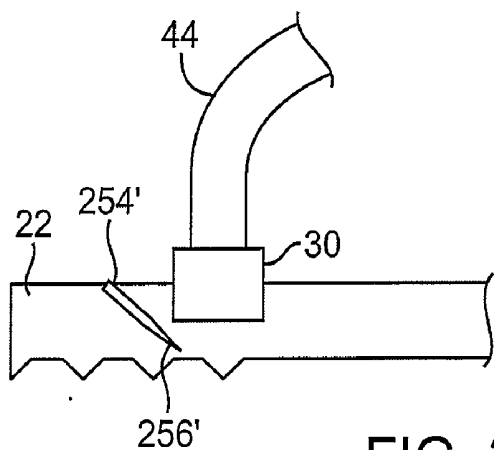
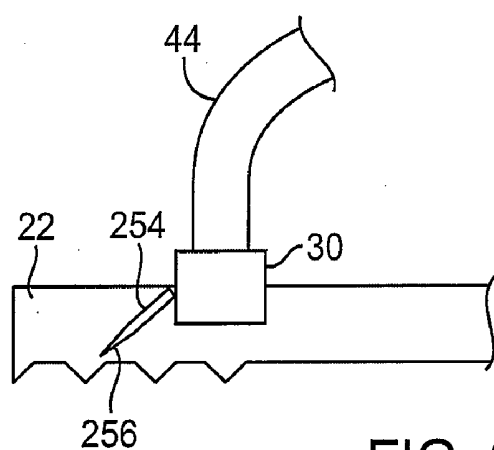
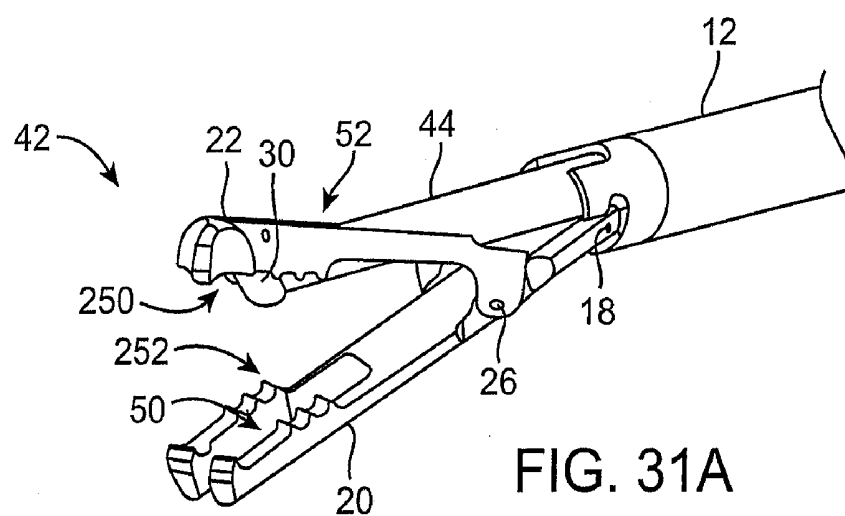


FIG. 29B





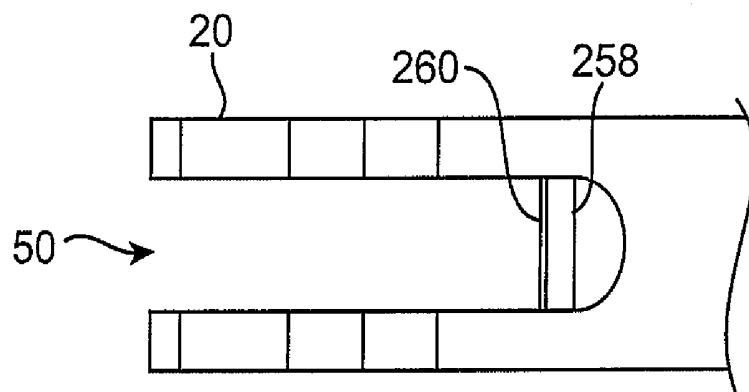


FIG. 31D

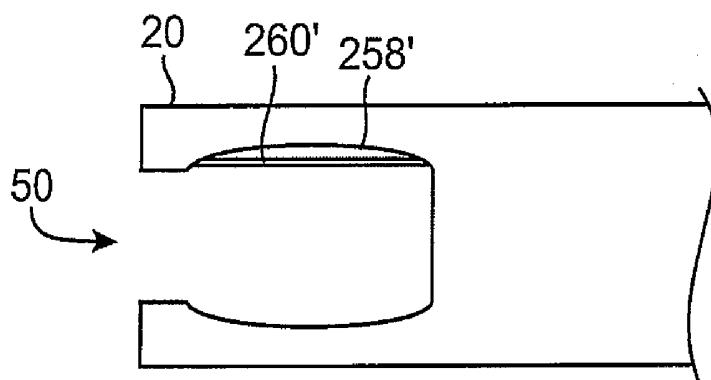


FIG. 31E













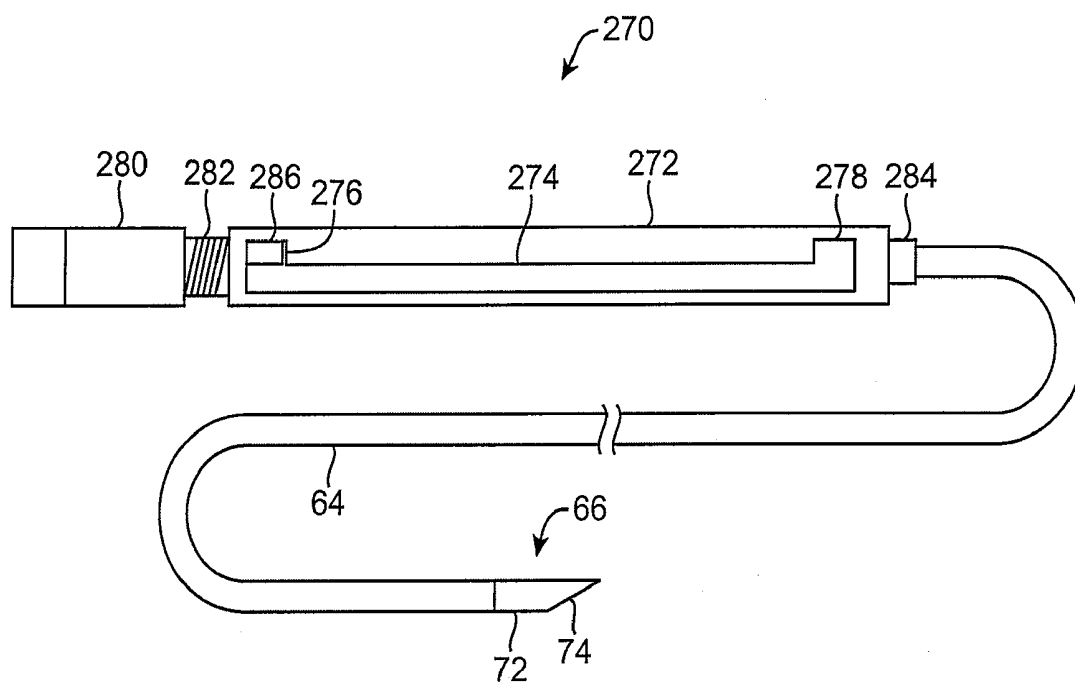


FIG. 32

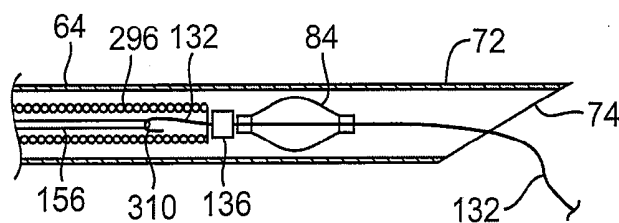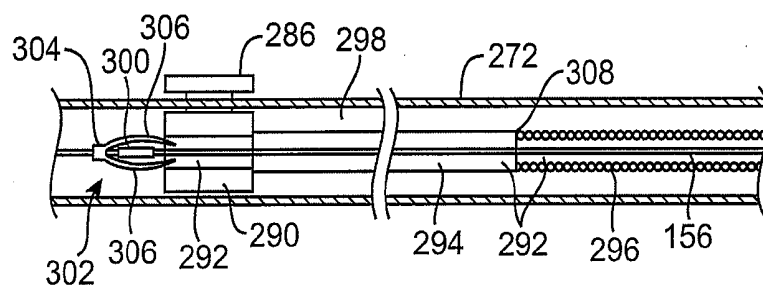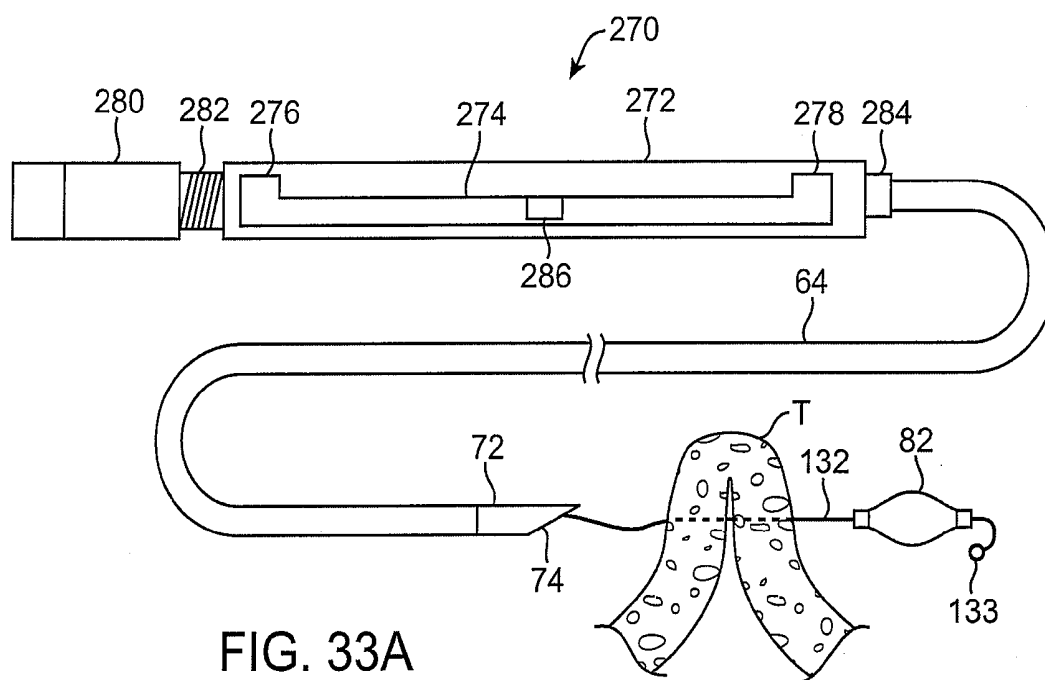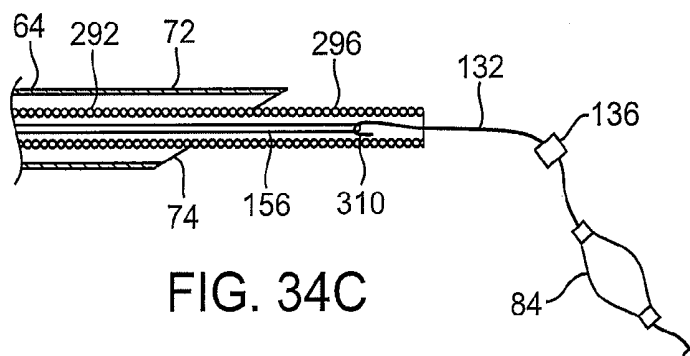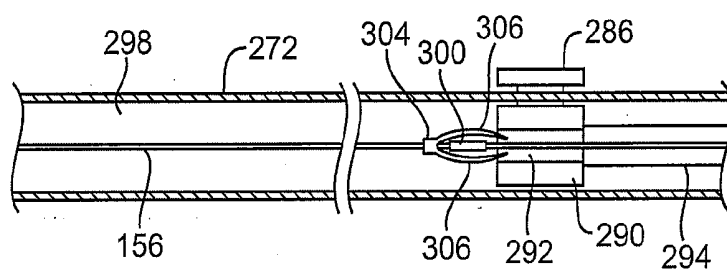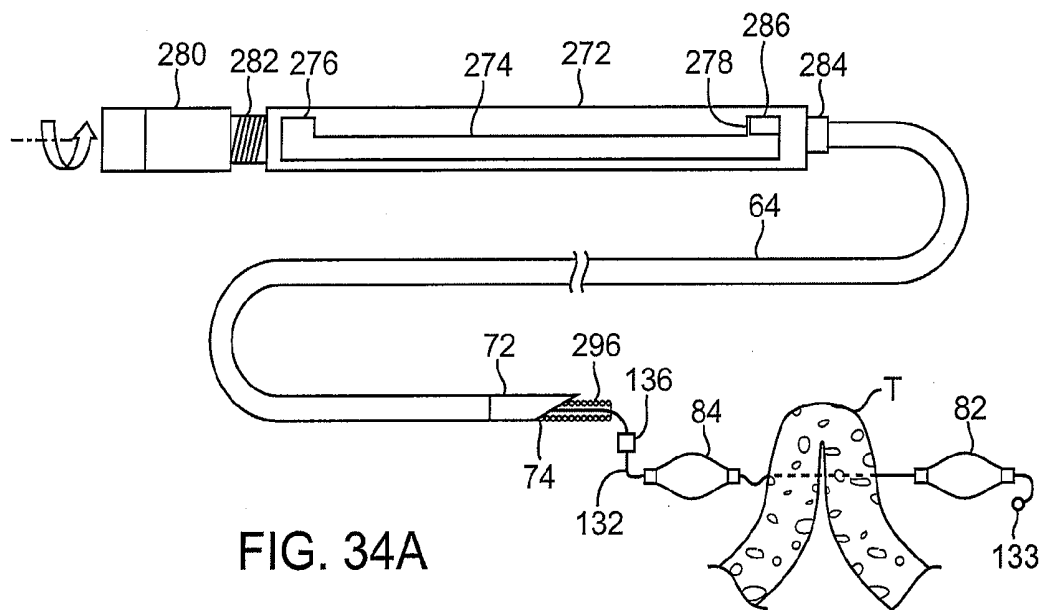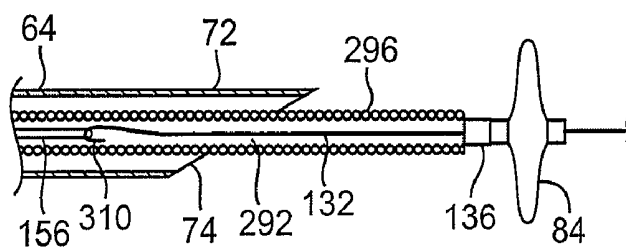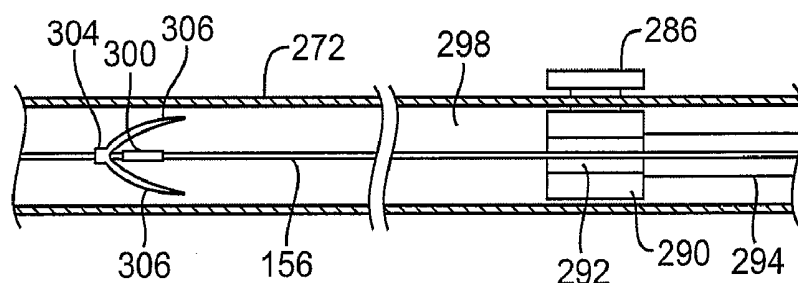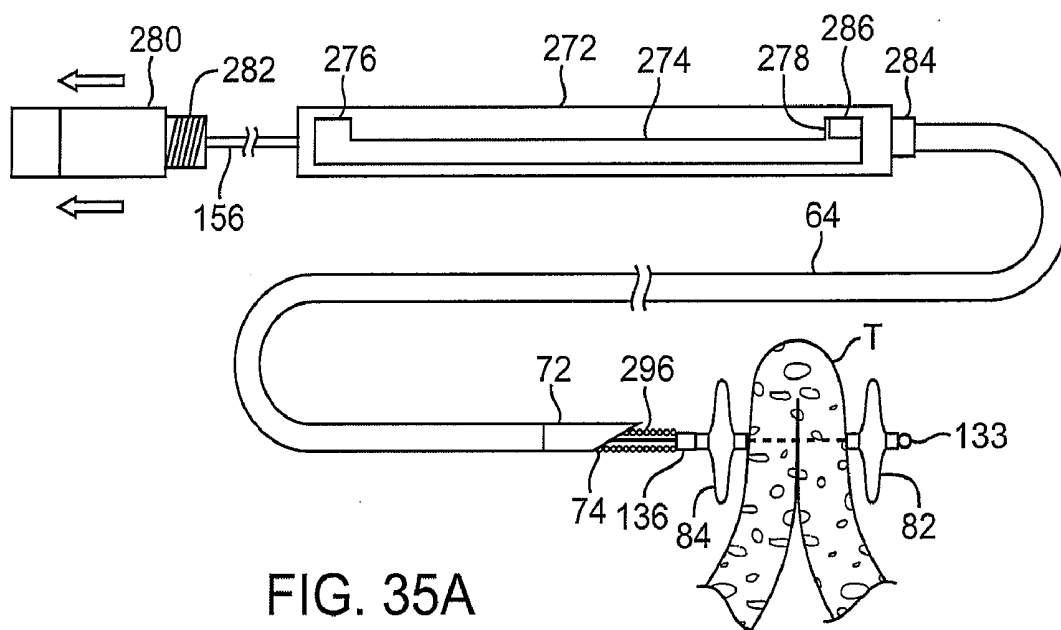

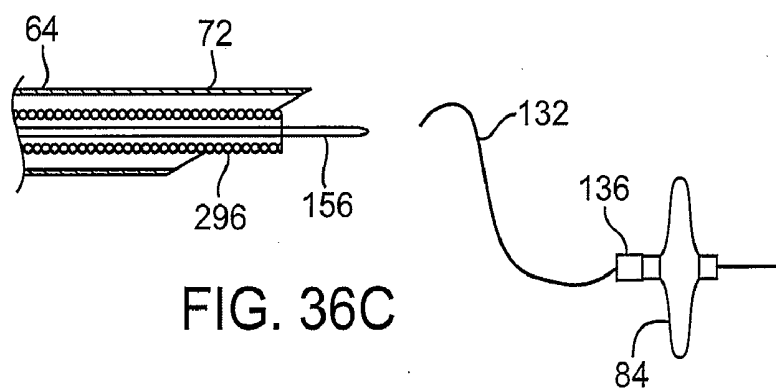

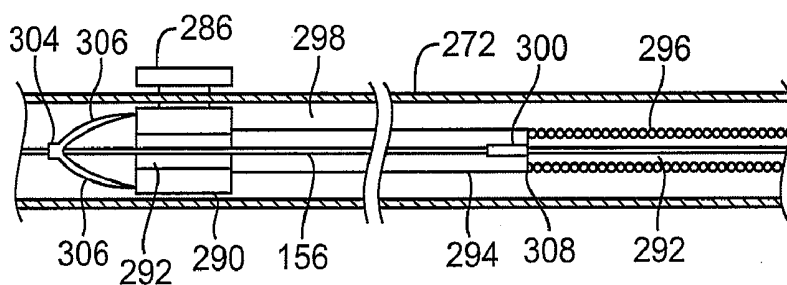

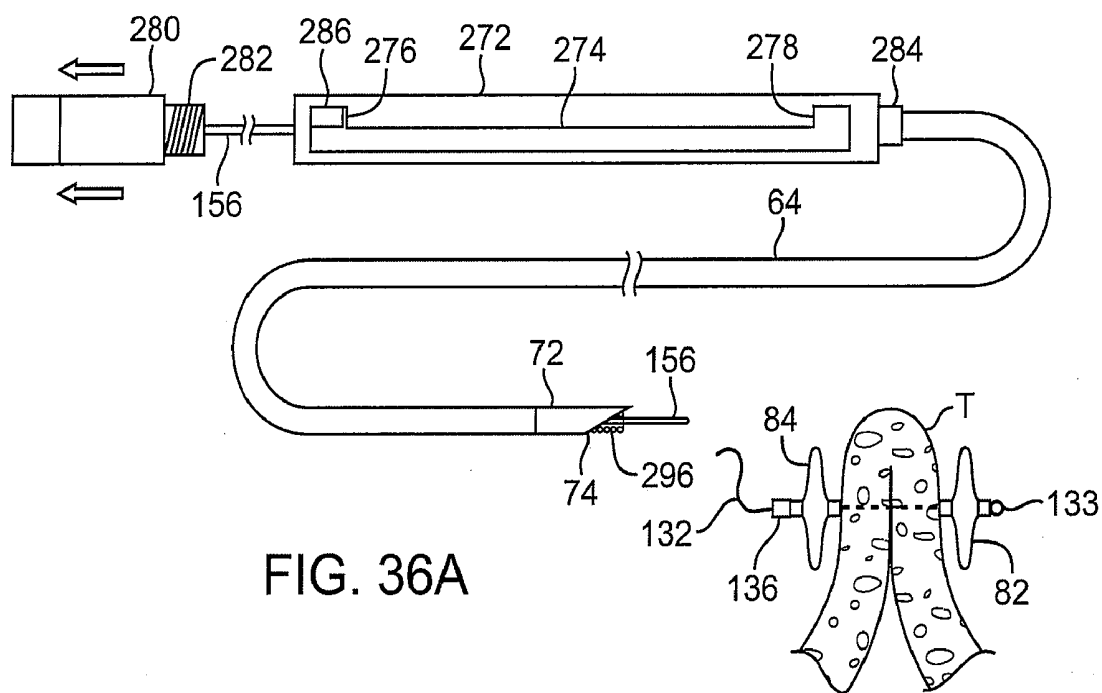

METHODS AND APPARATUS FOR SECURING AND DEPLOYING TISSUE ANCHORS

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] The present application is a continuation-in-part of U.S. patent application Ser. No. 11/238,543 filed Sep. 30, 2005, which is a continuation-in-part of U.S. patent application Ser. No. 11/139,920 filed May 26, 2005, each of which is incorporated herein by reference in its entirety.

FIELD OF THE INVENTION

[0002] The present invention relates to methods and apparatus for securing and deploying tissue anchors. More particularly, the present invention relates to methods and apparatus for endoluminally or laparoscopically securing and deploying anchors within or against tissue, for instance, to form and/or secure tissue folds or to approximate regions of tissue, etc.

BACKGROUND OF THE INVENTION

[0003] A number of surgical techniques have been developed to treat various gastrointestinal disorders. One such example of a pervasive disorder is morbid obesity. Conventional surgical treatment for morbid obesity typically includes, e.g., bypassing an absorptive surface of the small intestine, or reducing the stomach size. However, many conventional surgical procedures may present numerous life-threatening post-operative complications, and may cause atypical diarrhea, electrolytic imbalance, unpredictable weight loss and reflux of nutritious chyme proximal to the site of the anastomosis.

[0004] Furthermore, the sutures or staples that are often used in surgical procedures for gastrointestinal disorders typically require extensive training by the clinician to achieve competent use, and may concentrate significant force over a small surface area of the tissue, thereby potentially causing the suture or staple to tear through the tissue. Many of the surgical procedures require regions of tissue within the body to be approximated towards one another and reliably secured. The gastrointestinal lumen, for instance, includes four tissue layers, where the mucosa layer is the inner-most tissue layer followed by connective tissue, the muscularis layer, and where the serosa layer is the outer-most tissue layer.

[0005] One problem with conventional gastrointestinal reduction systems is that the anchors (or staples) should engage at least the muscularis tissue layer in order to provide a proper foundation. In other words, the mucosa and connective tissue layers typically are not strong enough to sustain the tensile loads imposed by normal movement of the stomach wall during ingestion and processing of food. In particular, these layers tend to stretch elastically rather than firmly hold the anchors (or staples) in position, and accordingly, the more rigid muscularis and/or serosa layer should ideally be engaged. This problem of capturing the muscularis or serosa layers becomes particularly acute where it is desired to place an anchor or other apparatus transesophageally rather than intra-operatively, since care must be taken in piercing the tough stomach wall not to inadvertently puncture adjacent tissue or organs.

[0006] One conventional method for securing anchors within a body lumen to the tissue is to utilize sewing devices to suture the stomach wall into folds. This procedure typically involves advancing a sewing instrument through the working channel of an endoscope and into the stomach and against the stomach wall tissue. The contacted tissue is then typically drawn into the sewing instrument where one or more sutures or tags are implanted to hold the suctioned tissue in a folded condition known as a plication. Another method involves manually creating sutures for securing the plication.

[0007] One of the problems associated with these types of procedures is the time and number of intubations needed to perform the various procedures endoscopically. Another problem is the time required to complete a plication from the surrounding tissue with the body lumen. In the period of time that a patient is anesthetized, procedures such as for the treatment of morbid obesity or for GERD must be performed to completion. Accordingly, the placement and securement of the tissue plication should ideally be relatively quick and performed with a minimal level of confidence.

[0008] Another problem with conventional methods involves ensuring that the staple, knotted suture, or clip is secured tightly against the tissue and that the newly created plication will not relax under any slack which may be created by slipping staples, knots, or clips. Other conventional tissue securement devices such as suture anchors, twist ties, crimps, etc. are also often used to prevent sutures from slipping through tissue. However, many of these types of devices are typically large and unsuitable for low-profile delivery through the body, e.g., transesophageally.

[0009] Moreover, when grasping or clamping onto or upon the layers of tissue with conventional anchors, sutures, staples, clips, etc., many of these devices are configured to be placed only after the tissue has been pliated and not during the actual plication procedure.

SUMMARY OF THE INVENTION

[0010] An example of a tool which may be utilized for endoluminally accessing tissue may generally comprise a flexible catheter or tubular body which may be configured to be sufficiently flexible for advancement into a body lumen, e.g., transorally, percutaneously, laparoscopically, etc. The tubular body may be configured to be torquable such that when a control handle is manipulated and/or rotated by a practitioner from outside the patient's body, the longitudinal and/or torquing force is transmitted along the flexible body such that the distal end of body is advanced, withdrawn, or rotated in a corresponding manner.

[0011] A tissue manipulation assembly may be located at the distal end of the tubular body and is generally used to contact and form tissue folds, as mentioned above. The tissue manipulation assembly may be connected to the distal end of the tubular body via a pivotable coupling, and a lower jaw member may extend distally from the pivotable coupling with an upper jaw member, in this example, pivotably coupled to the lower jaw member via a jaw pivot. The location of the jaw pivot may be positioned at various locations along the lower jaw depending upon a number of factors, e.g., the desired size of the "bite" or opening for accepting tissue between the jaw members, the amount of closing force between the jaw members, etc. One or both jaw

members may also have a number of protrusions, projections, grasping teeth, textured surfaces, etc., on the surface or surfaces of the jaw members to facilitate the adherence of tissue therebetween.

[0012] A launch tube may extend from the handle, through tubular body, and distally from the end of tubular body where a distal end of the launch tube is pivotally connected to the upper jaw member at a pivot. A distal portion of the launch tube may be pivoted into position within a channel or groove defined in upper jaw member to facilitate a low-profile configuration of the tissue manipulation assembly. When articulated, either via the launch tube or other mechanism, the jaw members may be urged into an open configuration to receive tissue in the jaw opening between the jaw members.

[0013] In operation, a shape-lockable endoscopic assembly may be advanced into a patient's stomach per-orally and through the esophagus. Such an endoscopic assembly may generally comprise an endoscopic device, which may have a distal portion that may be articulated and steered to position its distal end anywhere within the stomach. Once desirably configured, the assembly may then be locked or rigidized to maintain its shape or configuration to allow for procedures to be performed on the tissue utilizing any number of tools delivered therethrough.

[0014] The tissue manipulation assembly may be delivered into the patient while in a low-profile configuration, e.g., transorally, through the shape-lockable endoscopic assembly, through an endoscope, an endoscopic device, or directly. Once desirably positioned, the launch tube may be urged proximally via its proximal end at handle. Because the jaw assembly pivot and the relative positioning of the upper jaw pivot along lower jaw member and launch tube pivot along upper jaw member, the proximal movement of the launch tube may effectively articulate upper jaw into an expanded jaw configuration. Proximally urging the launch tube may also urge the lower jaw member to pivot about the assembly pivot and form an angle relative to a longitudinal axis of the tubular body. The opening of the upper jaw relative to the lower jaw creates a jaw opening for grasping or receiving tissue. Moreover, the tissue manipulation assembly may also include a stop located adjacent to the jaw assembly pivot or within the pivot itself.

[0015] A second tool for initially engaging the tissue region of interest may also be deployed and utilized to engage the tissue and to position the engaged tissue between the jaws of the jaw assembly. Any number of tools may be used in combination with the tissue manipulation assembly. Once the tissue has been engaged between the jaw members, a needle assembly may be urged through the launch tube to pierce through the grasped tissue. Once the needle assembly has been passed through the engaged tissue, one or more tissue anchors may be deployed for securing the tissue.

[0016] Once the one or more tissue anchors having been deployed, the tissue may be secured via an anchor deployment assembly, which may generally comprise an elongate member adapted for advancement within a body lumen of the patient and being further adapted to deploy at least one tissue anchor having a length of suture depending therefrom, wherein the elongate member comprises a suture cutting element disposed thereon which is adapted to sever a portion of the suture via thermal energy.

BRIEF DESCRIPTION OF THE DRAWINGS

[0017] FIG. 1A shows a side view of one variation of a tissue manipulation assembly having a flexible body and a handle.

[0018] FIG. 1B illustrates a detail side view of a tissue manipulation assembly in a low-profile configuration connected to the distal end of the tubular body via a pivotable coupling.

[0019] FIGS. 2A to 2C illustrate a method for articulating the tissue manipulation assembly from a low-profile configuration to an opened configuration and to a closed jaw configuration for clamping upon tissue, respectively.

[0020] FIGS. 3A and 3B show detail perspective views of the tissue manipulation assembly in an open and clamped configuration, respectively.

[0021] FIG. 4 shows an assembly view of how a needle deployment assembly may be introduced through a handle and tubular body of the tissue manipulation assembly.

[0022] FIG. 5A shows a detailed assembly view of the needle deployment assembly from FIG. 4.

[0023] FIG. 5B shows an exploded assembly view of the needle deployment assembly from FIG. 5A.

[0024] FIG. 6 illustrates one example in which a shape-lockable endoscopic assembly may be advanced into a patient's stomach per-orally and through the esophagus with a tissue manipulation assembly advanced through a first lumen and a tissue engagement member advanced through a second lumen.

[0025] FIG. 7 illustrates a tissue manipulation assembly and examples of various tools which may be used in combination with the tissue manipulation assembly.

[0026] FIGS. 8A to 8D illustrate an example for performing an endoluminal tissue manipulation and securement procedure utilizing a tissue manipulation assembly in combination with a separate tissue grasping tool within, e.g., a patient's stomach.

[0027] FIG. 9A shows one variation where a single tissue fold may be secured between tissue anchors using the tissue manipulation assembly.

[0028] FIG. 9B shows another variation where two or more tissue folds may be secured between tissue anchors using the tissue manipulation assembly.

[0029] FIGS. 10A and 10B illustrate a variation of the tissue manipulation assembly in a perspective and cross-sectional view, respectively, where a number of reinforcement members or bars may be positioned along the launch tube to increase its column strength.

[0030] FIGS. 11A and 11B illustrate another variation of the tissue manipulation assembly in a perspective and cross-sectional view, respectively, where a pull wire may be routed through the launch tube to facilitate articulation of the launch tube and/or jaw assembly.

[0031] FIG. 12 illustrates yet another variation of the tissue manipulation assembly which may also utilize a pull wire connected directly to the launch tube.

[0032] **FIG. 13** illustrates an exploded view of a variation of an anchor assembly and needle deployment assembly.

[0033] **FIG. 14** illustrates an assembly view, partially in section, of the anchor assembly and needle deployment assembly variation of **FIG. 13**.

[0034] **FIGS. 15A to 15F** illustrate an exemplary method of using the anchor assembly and needle deployment assembly variation of **FIGS. 13 and 14**.

[0035] **FIG. 16** illustrates a variation of the suture element for use with the anchor assembly and needle deployment assembly of **FIGS. 13 to 15**.

[0036] **FIG. 17** illustrates a variation of the needle for use with the anchor assembly and needle deployment assembly variation of **FIGS. 13 to 15**.

[0037] **FIG. 18** illustrates a variation of the control mechanisms for use with the needle deployment assemblies of **FIGS. 13 to 17**.

[0038] **FIGS. 19A to 19C** illustrate an exemplary method of using another variation of the anchor assembly and needle deployment assembly.

[0039] **FIGS. 20A to 20C** are schematic views illustrating another variation of the needle deployment assembly.

[0040] **FIGS. 21A to 21C** illustrate another variation of the needle deployment assembly utilizing a release suture or wire which may be routed through a looped terminal end of a suture element.

[0041] **FIGS. 22A to 22C** illustrate yet another variation of the needle deployment assembly utilizing a reconfigurable hook element which may configure itself from a hooked configuration to an open or straightened configuration.

[0042] **FIGS. 23A to 23C** illustrate yet another variation of the needle deployment assembly utilizing a release suture or wire with an obstructive element to be released from the release suture or wire.

[0043] **FIGS. 24A to 24C** illustrate yet another variation of the needle deployment assembly utilizing a suture cutting thermal element for releasing the suture and anchor assembly.

[0044] **FIGS. 25A and 25B** show partial cross-sectional side and assembly views, respectively, of the suture cutting thermal element assembly of **FIGS. 24A to 24C**.

[0045] **FIGS. 26A and 26B** show side and partial cross-sectional views, respectively, of another suture cutting thermal element.

[0046] **FIGS. 27A and 27B** show partial cross-sectional side and end views of yet another suture cutting thermal element.

[0047] **FIG. 28** shows an example of a cyclical timing profile for heating the thermal element.

[0048] **FIG. 29A** shows another pusher variation having a circumferential cutting edge disposed at the distal end of the pusher.

[0049] **FIG. 29B** shows the instrument of **FIG. 29A** abutted against a locking mechanism for cinching of the tissue anchors against a tissue surface.

[0050] **FIGS. 30A to 30C** illustrate an alternative method for severing the suture utilizing the tissue manipulation assembly.

[0051] **FIGS. 31A to 31B** illustrate examples for incorporating a cutting blade or element along regions of the tissue manipulation assembly.

[0052] **FIG. 32** illustrates another variation of a needle deployment assembly which may endoluminally deploy tissue anchors as well as cinch and release anchor assemblies.

[0053] **FIG. 33A** illustrates the variation of **FIG. 32** having deployed a distal anchor into plicated tissue.

[0054] **FIGS. 33B and 33C** show partial cross-sectional views of the control or housing and the distal portion of the sheath of **FIG. 33A** illustrating advancement of the tissue anchors, respectively.

[0055] **FIG. 34A** illustrates the variation of **FIG. 32** having deployed both tissue anchors into the plicated tissue prior to cinching of the anchors.

[0056] **FIGS. 34B and 34C** show partial cross-sectional views of the control or housing and the distal portion of the sheath of **FIG. 34A** illustrating advancement of both tissue anchors, respectively.

[0057] **FIG. 35A** illustrates the variation of **FIG. 32** where the tissue anchors are cinched towards one another for securing the tissue.

[0058] **FIGS. 35B and 35C** show partial cross-sectional views of the control or housing and the distal portion of the sheath of **FIG. 35A** illustrating cinching of the tissue anchors, respectively.

[0059] **FIG. 36A** illustrates the variation of **FIG. 32** where the cinched tissue anchors are released from the needle deployment assembly.

[0060] **FIGS. 36B and 36C** show partial cross-sectional views of the control or housing and the distal portion of the sheath of **FIG. 36A** illustrating release of the cinched tissue anchors, respectively.

DETAILED DESCRIPTION OF THE INVENTION

[0061] In manipulating tissue or creating tissue folds, a having a distal end effector may be advanced endoluminally, e.g., transorally, transgastrically, etc., into the patient's body, e.g., the stomach. The tissue may be engaged or grasped and the engaged tissue may be manipulated by a surgeon or practitioner from outside the patient's body. Examples of creating and forming tissue plications may be seen in further detail in U.S. patent application Ser. No. 10/955,245 filed Sep. 29, 2004, which has been incorporated herein by reference above, as well as U.S. patent application Ser. No. 10/735,030 filed Dec. 12, 2003, which is incorporated herein by reference in its entirety.

[0062] In engaging, manipulating, and/or securing the tissue, various methods and devices may be implemented. For instance, tissue securement devices may be delivered and positioned via an endoscopic apparatus for contacting a tissue wall of the gastrointestinal lumen, creating one or more tissue folds, and deploying one or more tissue anchors

through the tissue fold(s). The tissue anchor(s) may be disposed through the muscularis and/or serosa layers of the gastrointestinal lumen.

[0063] An illustrative side view of one example of a tool which may be utilized for endoluminally accessing tissue is shown in **FIG. 1A**, which shows assembly **10**. The assembly **10** generally comprises a flexible catheter or tubular body **12** which may be configured to be sufficiently flexible for advancement into a body lumen, e.g., transorally, percutaneously, laparoscopically, etc. Tubular body **12** may be configured to be torqueable through various methods, e.g., utilizing a braided tubular construction, such that when handle **16** is manipulated and/or rotated by a practitioner from outside the patient's body, the longitudinal and/or torquing force is transmitted along body **12** such that the distal end of body **12** is advanced, withdrawn, or rotated in a corresponding manner.

[0064] Tissue manipulation assembly **14** is located at the distal end of tubular body **12** and is generally used to contact and form tissue folds, as mentioned above. **FIG. 1B** shows an illustrative detail side view in which tissue manipulation assembly **14** may be seen connected to the distal end of tubular body **12** via a pivotable coupling **18**. Lower jaw member **20** extends distally from the pivotable coupling **18** and upper jaw member **22**, in this example, may be pivotably coupled to lower jaw member **20** via jaw pivot **26**. The location of jaw pivot **26** may be positioned at various locations along lower jaw **20** depending upon a number of factors, e.g., the desired size of the "bite" or opening for accepting tissue between the jaw members, the amount of closing force between the jaw members, etc. One or both jaw members **20**, **22** may also have a number of protrusions, projections, grasping teeth, textured surfaces, etc., **24** on the surface or surfaces of the jaw members **20**, **22** facing one another to facilitate the adherence of tissue between the jaw members **20**, **22**.

[0065] Launch tube **28** may extend from handle **16**, through tubular body **12**, and distally from the end of tubular body **12** where a distal end of launch tube **28** is pivotally connected to upper jaw member **22** at launch tube pivot **30**. A distal portion of launch tube **28** may be pivoted into position within a channel or groove defined in upper jaw member **22**, to facilitate a low-profile configuration of tissue manipulation assembly **14**. When articulated, either via launch tube **28** or other mechanism, as described further below, jaw members **20**, **22** may be urged into an open configuration to receive tissue in jaw opening **32** between the jaw members **20**, **22**.

[0066] Launch tube **28** may be advanced from its proximal end at handle **16** such that the portion of launch tube **28**, which extends distally from body **12**, is forced to rotate at hinge or pivot **30** and reconfigure itself such that the exposed portion forms a curved or arcuate shape that positions the launch tube opening perpendicularly relative to upper jaw member **22**. Launch tube **28**, or at least the exposed portion of launch tube **28**, may be fabricated from a highly flexible material or it may be fabricated, e.g., from Nitinol tubing material which is adapted to flex, e.g., via circumferential slots, to permit bending.

[0067] **FIGS. 2A** to **2C** illustrate one method for articulating a tissue manipulation assembly into an opened and closed configuration. As shown in **FIG. 2A**, the assembly

may be delivered into a patient while in a low-profile configuration **40**, e.g., transorally, through an endoscope, an endoscopic device, or directly. Once desirably positioned, launch tube **28** may be urged proximally via its proximal end at handle **16**. Because of jaw assembly pivot **18** and the relative positioning of upper jaw pivot **26** along lower jaw member **20** and launch tube pivot **30** along upper jaw member **22**, the proximal movement of launch tube **28** may effectively articulate upper jaw **22** into an expanded jaw configuration **42**, as shown in **FIG. 2B**. Proximally urging launch tube **28** may also urge lower jaw member **20** to pivot about assembly pivot **18** and form an angle, α , relative to a longitudinal axis of tubular body **12**. The opening of upper jaw **22** relative to lower jaw **20** creates jaw opening **32** for grasping or receiving tissue. Moreover, the tissue manipulation assembly may also include a stop located adjacent to jaw assembly pivot **18** or within the pivot **18** itself.

[0068] Once launch tube **28** has been urged proximally, it may be locked into place thus locking the jaw configuration as well. Moreover, having the launch tube **28** articulate the jaw members **20**, **22** in this variation eliminates the need for a separate jaw articulation and/or locking mechanism. Once the tissue has been pulled or manipulated between jaw members **20**, **22**, launch tube **28** may be pushed distally to actuate the jaw members **20**, **22** into a closed, grasping configuration **48**, as shown in **FIG. 2C**, for engagement with the tissue. As launch tube **28** is urged distally through body **12**, lower jaw member **20** may be maintained at the angle, α , relative to the tissue to further facilitate manipulation of the grasped tissue.

[0069] Launch tube **28** may further define a flexible portion **44** distally of a rigid portion **46**. Although launch tube **28** may be fabricated from different materials having differing flexibilities, it may also be fabricated from a single material, as mentioned above, where the flexible portion **44** may be configured, e.g., by slotting, to allow for bending of the launch tube **28** in a plane to form a single curved or arcuate section while the rigid section **46** may extend at least partially into tubular body **12** to provide column strength to launch tube **28** while it is urged distally upon upper jaw member **22** and upon any tissue engaged thereby, as seen in the **FIG. 2C**.

[0070] Once the tissue has been engaged between jaw members **20**, **22**, a needle assembly may be urged through handle **16** and out through launch tube **28**. The needle assembly may pass through lower jaw member **20** via needle assembly opening **50** defined in lower jaw member **20** to pierce through the grasped tissue. Once the needle assembly has been passed through the engaged tissue, one or more tissue anchors may be deployed for securing the tissue, as described in further detail in U.S. patent application Ser. No. 10/955,245, which has been incorporated by reference above.

[0071] **FIGS. 3A** and **3B** show detail perspective views of the tissue manipulation assembly. As shown in **FIG. 3A**, lower jaw member **20** and upper jaw member **22** may be seen its open configuration **42** when the launch tube has been urged proximally. Launch tube channel **52** may also be seen defined within upper jaw member **22** for providing a space for positioning the launch tube when in the low-profile configuration. Also shown is needle assembly opening **50** defined within lower jaw member **20** for passage of the

needle assembly therethrough. **FIG. 3B** shows the assembly in its closed jaw configuration where the launch tube has been urged distally in which it rotates about launch tube pivot **30** such that the opening the launch tube become perpendicular relative to the jaw members **20, 22**.

[0072] Although one particular variation of the jaw members **20, 22** is shown, this is not intended to be limiting in jaw member configuration or operation. Other variations may include various placement of the jaws relative to one another, alternative configurations for articulating the jaw members, alternative configurations for the launch tube placement, etc. Other variations are intended to be within the scope of this disclosure.

[0073] As mentioned above, a needle deployment assembly **60** may be deployed through the assembly **10** by introducing needle deployment assembly **60** into the handle **16** and through tubular body **12**, as shown in the assembly view of **FIG. 4**, such that the needle assembly **66** is advanced from the launch tube and into or through approximated tissue. Once the needle assembly **66** has been advanced through the tissue, the anchor assembly **68** may be deployed or ejected. Anchor assembly **68** is normally positioned within the distal portion of tubular sheath **64**, which extends from needle assembly control or housing **62**. Once the anchor assembly **68** has been fully deployed from sheath **64**, the spent needle deployment assembly **60** may be removed from assembly **10** and another needle deployment assembly may be introduced without having to remove assembly **10** from the patient. The length of sheath **64** is such that it may be passed entirely through the length of tubular body **12** to enable the deployment of needle assembly **66** into and/or through the tissue.

[0074] **FIG. 5A** shows a detailed assembly view of the needle deployment assembly **60** from **FIG. 4**. In this variation, elongate and flexible sheath or catheter **64** may extend removably from needle assembly control or housing **62**. Sheath or catheter **64** and housing **62** may be interconnected via interlock **70** which may be adapted to allow for the securement as well as the rapid release of sheath **64** from housing **62** through any number of fastening methods, e.g., threaded connection, press-fit, releasable pin, etc. Needle body **72**, which may be configured into any one of the variations described above, may extend from the distal end of sheath **64** while maintaining communication between the lumen of sheath **64** and needle opening **74**.

[0075] Elongate pusher **76** may comprise a flexible wire or hypotube which is translationally disposed within sheath **64** and movably connected within housing **62**. A proximally-located actuation member **78** may be rotatably or otherwise connected to housing **62** to selectively actuate the translational movement of elongate pusher **76** relative to sheath **64** for deploying the anchors from needle opening **74**. Anchor assembly **68** may be seen positioned distally of elongate pusher **76** within sheath **64** for deployment from sheath **64**. Needle assembly guides **80** may also be seen protruding from housing **62** for guidance through the locking mechanism described above. **FIG. 5B** shows an exploded assembly view of the needle deployment assembly **60** from **FIG. 5A**. As seen, sheath **64** may be disconnected from housing **62** via interlock **70** to reveal the elongate pusher **76** connected to housing **62** and the distal and proximal anchors **82, 84**, respectively, of anchor assembly **68**.

[0076] With respect to the anchor assemblies, the types of anchors shown and described are intended to be illustrative and are not limited to the variations shown. For instance, the tissue anchor variations may also include "T"-type anchors while other variations may include reconfigurable "basket"-type anchors, which may generally comprise a number of configurable struts or legs extending between at least two collars or support members or reconfigurable mesh structures extending between the two collars. Other variations of these or other types of anchors are also contemplated for use in an anchor assembly. Moreover, a single type of anchor may be used exclusively in an anchor assembly; alternatively, a combination of different anchor types may be used in an anchor assembly. Furthermore, the different types of cinching or locking mechanisms are not intended to be limited to any of the particular variations shown and described but may be utilized in any of the combinations or varying types of anchors as practicable.

[0077] Other variations for the needle assemblies and for the anchors are described in further detail in U.S. patent application Ser. No. 10/955,245, which has been incorporated by reference above.

[0078] In operation when manipulating and securing tissue within a patient's body, a separate elongate shaft having a tool on or near the distal end of the shaft may be utilized in conjunction with the tissue manipulation assembly **14**. Such tools are generally utilized in endoluminal procedures where the tools are delivered through an endoscope. Generally, several different tools may be utilized for performing a procedure endoluminally.

[0079] As illustrated in **FIG. 6**, one such example is shown in which a shape-lockable endoscopic assembly **90** may be advanced into a patient's stomach S per-orally and through the esophagus E. Such an endoscopic assembly **90** may generally comprise an endoscopic device which may have a distal portion which may be articulated and steered to position its distal end anywhere within the stomach S. Once desirably configured, assembly **90** may then be locked or rigidized to maintain its shape or configuration to allow for procedures to be performed on the tissue utilizing any number of tools delivered through the assembly **90**. Shape-lockable assembly **90** and its variations are described in further detail in U.S. patent application Ser. No. 10/734,562 filed Dec. 12, 2003, which is incorporated herein by reference in its entirety.

[0080] Shape-lockable assembly **90** may be generally comprised of shape-lockable endoscopic body **92** having an articulatable distal portion **96**. The endoscopic body **92** may define at least first and second lumens **98, 100**, respectively, through the endoscopic body **92** through which one or more tools may be deployed into the stomach S. Additional lumens may be provided through shape-lockable endoscopic body **92**, such as a visualization lumen **101**, through which an endoscope may be positioned to provide visualization of the region of tissue. Alternatively, an imager such as a CCD imager or optical fibers may be provided in lumen **101** to provide visualization. An optional thin wall sheath **94** may be disposed through the patient's mouth, esophagus E, and possibly past the gastroesophageal junction GEJ into the stomach S. Shape-lockable body **92** may be advanced through esophagus E (and through sheath **94**, if utilized) and into stomach S while disposed in a flexible state.

[0081] Distal steerable portion **96** of endoscopic body **92** may be then articulated to an orientation, e.g., whereby distal portion **96** facilitates engagement of tissue near and/or inferior to the patient's gastroesophageal junction GEJ. Accordingly, distal steerable portion **96** may comprise a number of steering features, as described in further detail in U.S. patent application Ser. No. 10/734,562, incorporated above. With distal steerable portion **96** disposed in a desired configuration or orientation, endoscopic body **92** may be reversibly shape-locked to a rigid state such that the endoscopic body **92** maintains its position within the stomach S. Various methods and apparatus for rigidizing endoscopic body **92** along its length are also described in further detail in U.S. patent application Ser. No. 10/734,562, incorporated above.

[0082] FIG. 6 shows tissue manipulation assembly **14** having been advanced through first lumen **98** and a tissue engagement member **102** positioned upon flexible shaft **104** advanced through second lumen **100**. As the tissue wall of a body lumen, such as the stomach, typically comprises an inner mucosal layer, connective tissue, the muscularis layer and the serosa layer. To obtain a durable purchase, e.g., in performing a stomach reduction procedure, tissue engagement member **102** may be advanced into contact with the tissue and preferably engages the tissue F such that when the tissue engagement member **102** is pulled proximally to draw the engaged tissue F between the jaw members **20**, **22** of tissue manipulation assembly **14**, at least the muscularis tissue layer and the serosa layer is drawn into tissue manipulation assembly **14**.

[0083] As tissue manipulation assembly **14** may be utilized to grasp and secure the engaged tissue, any number of tools may be utilized with tissue manipulation assembly **14**, e.g., through shape-lockable endoscopic body **92**, to engage and manipulate the tissue of interest relative to tissue manipulation assembly **14**. FIG. 7 illustrates tissue manipulation assembly **14** upon flexible body **12** with handle **16** and examples of various tools which may be used in combination with tissue manipulation assembly **14**.

[0084] Turning to FIG. 7, one example of a tool utilizable in combination with tissue manipulation assembly **14** is shown in tissue engagement member **102** as a tissue piercing helix or corkscrew structure upon flexible shaft **104** (as shown in FIG. 6). Tissue engagement member **102** may be rotated about its longitudinal axis to engage the tissue of interest by rotating handle **106** located on the proximal end of flexible shaft **104**. Alternatively, a tool having aggressive tissue graspers **108** positioned upon flexible shaft **110** and articulatable via handle **112** may be utilized in combination with tissue manipulation assembly **14**. Another alternative tool may be tissue graspers **114** positioned upon flexible shaft **116** and articulatable via handle **118**. Tissue graspers **114** may have atraumatic grasping surfaces. In yet another alternative, an endoscope **122** having optical fibers or imager **120** may be utilized for providing visualization. Endoscope **122** may be articulated via handle **124** at its proximal end.

[0085] The examples of the various tools as shown and described are intended merely to be illustrative of the range of tools which may be usable with assembly **14** and are not intended to be limiting in any manner. Any number of other tools may be accordingly utilized and are intended to be within the scope of this disclosure.

[0086] An example of performing an endoluminal tissue manipulation and securement procedure utilizing tissue manipulation assembly **14** in combination with a separate tissue grasping tool within, e.g., a patient's stomach, is illustrated in FIGS. 8A to 8D. As shown in FIG. 8A, once shape-lockable endoscopic body **92** has been introduced into the patient, e.g., trans-orally, trans-anally, percutaneously, etc., and desirably positioned relative to a tissue region of interest **130**, endoscopic body **92** may be rigidized to maintain its configuration within the patient body. Alternatively, it may be left in a flexible state during the procedure.

[0087] The tissue region of interest **130** as well as the procedure may be visualized through visualization lumen **101** or a separate imager, as described above. In either case, tissue manipulation assembly **14** and tissue engagement member **102** may be advanced distally out from endoscopic body **92** through their respective lumens **98**, **100**. Tissue engagement member **102** may be advanced into contact against the tissue surface, as shown in FIG. 8A, and then rotated via its proximal handle until the tissue is engaged. The engaged tissue F may be pulled proximally relative to endoscopic body **92** and tissue manipulation assembly **14** may be actuated via its proximally located handle into an open expanded jaw configuration for receiving the engaged tissue F, as shown in FIG. 8B.

[0088] Alternatively, once the tissue F has been engaged, tissue manipulation assembly **14** may be advanced distally in its open configuration onto the engaged tissue. In yet another variation, tissue engagement member **102** may be omitted entirely and tissue manipulation assembly **14** may be utilized alone to grasp onto the tissue region of interest **130**. In yet another alternative, a second tissue manipulation assembly may be used in combination with tissue manipulation assembly **14**.

[0089] Turning back to FIG. 8B, tissue manipulation assembly **14** may be articulated to receive the engaged tissue F. As shown in FIG. 8C, once engaged tissue F is positioned between jaw members **20**, **22**, the launch tube may be urged proximally to actuate upper jaw member **22** to grasp or clamp upon the tissue F. Tissue engagement member **102** may be retracted from the tissue F or it may be left within the tissue while tissue manipulation assembly engages and secures the tissue F.

[0090] FIG. 8D shows a partial cross-sectional view of the tissue F while engaged to tissue manipulation assembly **14**. Tissue engagement member **102** has been omitted from this view only for the sake of clarity. As mentioned above, member **102** may be left remaining in the tissue F, disengaged from tissue F, or disengaged and removed entirely from endoscopic body **92**, if so desired, and another tool may be advanced through lumen **100** to facilitate the procedure. Once jaw members **20**, **22** have been actuated to clamp or grasp upon tissue F by the launch tube, the launch tube may be automatically positioned into its anchor deployment configuration. The needle assembly may then be urged via manipulation from its proximal end at handle **16** through the launch tube to pierce preferably through a dual serosa layer through engaged tissue F and past lower jaw member **20**. As described above, the engaged tissue F positioned between the jaw members **20**, **22** is desirably engaged such that the needle body **72**, when urged through the tissue F, is disposed through the muscularis and/or serosa layers of the

engaged tissue F. Once needle body 72 has passed through tissue F, one or more expandable tissue anchors may be ejected from needle body 72 through needle opening 74.

[0091] Because needle body 72 may penetrate the tissue wall twice, it exits within the body lumen if utilized within, e.g., the stomach, thus reducing the potential for injury to surrounding organs. As described above, needle body 72 may define needle lumen or opening 74 through which an expandable anchor, e.g., distal anchor 82 and/or proximal anchor 84, may be situated during deployment and positioning of the assembly. A single suture or flexible element 132 (or multiple suture elements) may connect distal anchor 82 and proximal anchor 84 to one another and end in terminal loop 134. For instance, element 132 may comprise various materials such as monofilament, multifilament, or any other conventional suture material, elastic or elastomeric materials, e.g., rubber, etc.

[0092] Once distal anchor 82 has been ejected, needle body 72 may be urged proximally back through tissue F, where proximal anchor 84 may then be ejected from needle body 72 with suture 132 still connecting the two anchors 82, 84 through tissue F. Alternatively, tissue manipulation assembly 14, with suture 132 still depending therefrom, may be disengaged from tissue F and the procedure may be repeated at a second region of tissue where proximal anchor 84 may then be ejected.

[0093] FIG. 9A shows one variation where a single fold F may be secured between proximal anchor 82 and distal anchor 84. With both anchors 82, 84 disposed externally of the launch tube and suture 132 connecting the two, proximal anchor 84 may be urged into contact against tissue F. As the anchors are urged against tissue fold F, distal anchor 82 or a portion of suture 132 may be configured to provide any number of directionally translatable locking mechanisms 136 which provide for movement of an anchor along suture 132 in a first direction and preferably locks, inhibits, or prevents the reverse movement of the anchor back along suture 132.

[0094] FIG. 9B shows another variation where a at least two folds F_1 and F_2 may be secured between proximal anchor 82 and distal anchor 84. After the anchors have been ejected from needle body 72, the anchors may be approximated towards one another over suture 132 thus bringing folds F_1 and F_2 towards one another. Although a single tissue fold and a dual fold are shown in these examples, any number of folds or tissue ridges may be created using the tools disclosed herein. Moreover, these examples are merely intended to be illustrative and not limiting in any way. In either case, it may be generally desirable to form the tissue folds such that serosa-to-serosa contact 138 occurs between the layers of secured tissue, although this may not be necessary.

[0095] Various examples of cinching devices and methods which may be utilized with the tools and devices herein are described in further detail in U.S. patent application Ser. No. 10/840,950 filed May 7, 2004, which has been incorporated herein above.

[0096] In using the launch tube as a jaw actuation mechanism, other variations of the launch tube may be utilized to ensure sufficient strength and force transmission in tissue manipulation assembly 14 for jaw member actuation. One

such example is shown in the perspective view of FIG. 10A, which shows launch tube 44 having a number of reinforcement members or bars 140 aligned along one or both sides of the launch tube to provide for additional column strength. Each of the reinforcement members 140 may be pivotally attached to launch tube 44 via pivot members 144 rotatably secured within pivot channels 142, as seen in the launch tube cross-section in FIG. 10B. Moreover, each of the pivot members 144 may define cooperating adjacent members relative to one another while maintaining contact to allow for the transmission of force between the members 144. Pivot members 144 may be positioned along the length of the exposed launch tube or a portion of the launch tube; moreover, a single side of the launch tube may have pivot members 144 attached thereto. Alternatively, rather than utilizing pivot members, portions of the launch tube itself may be simply thickened to increase its column strength and force transmission capabilities.

[0097] In another variation, as shown in FIG. 11A and the launch tube cross-section in FIG. 11B, a pull wire 152 may be routed through tubular body 12 and launch tube 44 through a pull wire lumen 150 to provide a launch tube and jaw actuation mechanism separate from the launch tube actuation itself. Pull wire 152 may be manipulated via its proximal end at handle 16 by pulling or pushing pull wire 152 to actuate launch tube 44 and/or jaw members 20, 22. Alternatively, as seen in FIG. 12, pull wire 152 may be routed through tubular body 12 and connected directly to launch tube 44 at pull wire attachment point 154 rather than routing it through the launch tube. Again, manipulation of pull wire 152 may be utilized to articulate the launch tube configuration as well as jaw member articulation.

[0098] Referring now to FIGS. 13 and 14, a variation of the anchor assembly and the needle deployment assembly is described. As with previously described needle deployment assembly 60, assembly 60' comprises needle assembly control or housing 62, tubular sheath 64 and needle assembly 66 having needle body 72 with opening 74. Elongate pusher 76 is configured for translation within sheath 64 via actuation member 78. Pusher 76 illustratively comprises a hypotube having lumen 77 defined therethrough.

[0099] In the variation of FIGS. 13 and 14, locking mechanism 136 of anchor assembly 68' is disposed proximal of proximal anchor 84, and the anchor assembly is positioned within the distal portion of tubular sheath 64, such that the distal region of pusher 76 abuts locking mechanism 136. Suture or flexible element 132' comprising distal knot or protrusion 133 extends proximally from the knot in a manner that connects distal anchor 82, proximal anchor 84 and locking mechanism 136. Element 132' then further extends through lumen 77 of pusher 76 to a proximal region of assembly 60' such that element 132' may be manipulated by a medical practitioner from outside a patient. The medical practitioner may, for example, engage previously described suture loop 134, or may engage some other control element 134', such as a ring or handle, disposed at the proximal end of suture element 132'. As will be apparent, in another variation, element 132' may extend to the proximal region of assembly 60' alongside pusher 76 rather than within a lumen of the pusher.

[0100] With reference to FIG. 15, a method of using anchor assembly 68' and needle deployment assembly 60' is

described. For the purposes of illustration, the assemblies are shown securing tissue without use of a tissue manipulation assembly. However, it should be understood that the assemblies alternatively may be used in combination with a tissue manipulation assembly, such as previously described tissue manipulation assembly 14 of assembly 10.

[0101] In FIG. 15A, needle deployment assembly 60' has been positioned in proximity to approximated tissue T. The assembly is advanced such that needle assembly 66 pierces the tissue and is advanced through and across the tissue, as in FIG. 15B. Pusher 76 is advanced within the lumen of sheath 64 via actuation member 78, such that distal anchor 82 of anchor assembly 68' is ejected through opening 74 of needle body 72 of needle assembly 66 on the distal side of approximated tissue T. Needle deployment assembly 60' and pusher 76 then are retracted such that the pusher and needle assembly 66 again are disposed on the proximal side of the approximated tissue, as in FIG. 15C. Next, pusher 76 is distally advanced relative to sheath 64 to eject proximal anchor 84 from the sheath.

[0102] In FIG. 15D, with the proximal and distal anchors of anchor assembly 68' disposed on either side of the approximated tissue, the anchor assembly is cinched by retracting control element 134' relative to needle deployment assembly 60'. Pusher 76 abuts locking mechanism 136 and urges it distally during proximal retraction of element 134', which shortens the length of suture element 132' disposed between distal anchor 82 and proximal anchor 84, thereby cinching anchor assembly 68'. Locking mechanism 136 ensures that the anchors remain cinched by resisting distal passage of element 132' through the mechanism, thereby resisting subsequent separation of the proximal and distal anchors.

[0103] With anchor assembly 68' cinched, pusher 76 is retracted relative to sheath 64 such that needle assembly 66 engages suture element 132', as in FIG. 15E. The needle assembly cuts the suture proximal of locking mechanism 136, as in FIG. 15F. The medical practitioner may facilitate cutting of the suture element by manipulating control element 134' of anchor assembly 68' and/or by manipulating needle assembly control 62 of needle deployment assembly 60'.

[0104] Referring now to FIG. 16, a variation of the suture element of anchor assembly 68' is described. In FIG. 16, suture element 132'' comprises segment 135 of reduced integrity. The segment may for example, comprise fewer suture strands or may be reduced in integrity via chemical, electrical, thermal or physical processing, etc. Segment 135 may locally reduce the tensile strength of element 132'' to a desired threshold. When used to cinch anchor assembly 68' in combination with anchor deployment assembly 60', the segment may obviate a need to cut the suture with needle assembly 66 after cinching of the anchor assembly. Specifically, the anchor assembly may be cinched to a desired tension after which segment 135 plastically deforms and snaps, leaving the anchor assembly cinched and in place.

[0105] With reference to FIG. 17, a variation of the needle assembly of needle deployment assembly 60' is described. Needle body 72' of needle assembly 66' may comprise one or more recessed cut-outs 73 having sharpened edges E for cutting the suture element. After cinching of anchor assembly 68', the suture element may be snagged within a cut-out 73 and cut by the sharpened edge of the cut-out.

[0106] Referring now to FIG. 18, alternative control mechanisms for needle deployment assembly 60' are described. Actuation member 78' for controlling pusher 76 may be integrated with needle assembly control 62', such that the actuation member is advanceable in controlled increments relative to the needle assembly control via detents 63 of the needle assembly control that coast with actuation member 78'.

[0107] With reference to FIG. 19, another variation of the anchor assembly and needle deployment assembly is shown. Control element 134' of anchor assembly 68' is coupled to or abuts needle assembly control 62' of needle deployment assembly 60'. When distal anchor 82 of anchor assembly 68' is disposed on the distal side of approximated tissue T, as in FIG. 19A, the proximal and distal ends of suture element 132' are constrained. Thus, as seen in FIGS. 19A and 19B, advancement of pusher 76 via actuation member 78' advances both proximal anchor 84 and locking mechanism 136 of anchor assembly 68'. This causes the anchor assembly to be progressively cinched as the proximal anchor is advanced. Once the anchor assembly has been ejected from sheath 64, as in FIG. 19B, and adequately cinched, as in FIG. 19C, suture element 132' may be cut proximal of the locking mechanism, e.g., with needle assembly 66 as described previously.

[0108] Referring to FIG. 20, a variation of the needle deployment assembly is described. Pusher 76' comprises suture ports 79 through which suture element 132' of anchor assembly 68' is routed. As seen in FIG. 20A, with pusher 76' disposed within tubular sheath 64 of needle deployment assembly 60', suture element 132' passes out of the pusher between the suture ports and is disposed between the pusher and the interior wall of the tubular sheath. As seen in FIG. 20B, when pusher 76' is advanced through and distal of needle assembly 66, e.g., to eject proximal anchor 84 of anchor assembly 68' from the needle deployment assembly and/or to cinch the anchor assembly, the section of suture element 132' between the suture ports is exposed. Subsequent retraction of the pusher relative to the needle assembly causes the section of exposed suture to contact the sharpened edge of needle assembly 66, thereby severing suture element 132' as in FIG. 20C.

[0109] Turning now to FIG. 21, another variation of the needle deployment assembly is shown. In this variation, suture element 132''' may form a terminal loop 158 through which a release suture or wire 156 may be passed. Release suture or wire 156 may be routed through the length of the needle deployment assembly and through pusher 76, as described above, and both release suture or wire 156 and terminal loop 158 may both be situated within pusher 76, as shown in FIG. 21A. After deployment of the anchors into tissue and cinching of the assembly, as described above, one end of release suture or wire 76 may be pulled or tensioned proximally in the direction shown by arrow 162, as in FIG. 21B. This pulling may draw a terminal end of release suture or wire 156 through pusher 76 until terminal loop 158 of suture element 132''' has been released therefrom, as shown in FIG. 21C.

[0110] In yet another variation shown in FIG. 22A, terminal loop 158 of suture element 132''' may be seen restrained within pusher 76 via reconfigurable hook 164 of release wire 156'. Here, release wire 156' may be fabricated

from a shape memory or superelastic alloy material, such as Nitinol, which has been preformed to reconfigure its terminal end from a hook 164 configuration to a straightened or opened configuration once released from the constraints of pusher 76. Thus, after deployment and cinching of the anchor assembly, release wire 156' may be advanced distally through pusher 76, as shown in FIG. 22B, until reconfigurable hook 164, which is retained in a hooked or obstructive configuration within the lumen of pusher 76, has been advanced out of pusher 76. Once free from the constraints of the lumen, hook 164 may reconfigure itself into an opened or straightened configuration to thereby release terminal loop 158 of suture element 132'', as shown in FIG. 22C. Hook 164 having released terminal loop 158, may then be withdrawn proximally back into pusher 76 in its straightened configuration.

[0111] In another variation shown in FIG. 23A, a terminal end of suture element 132''' may have an obstructive or enlarged element 160, e.g., a knot, formed thereon. The terminal end of suture element 132''' with obstructive element 160 may be looped around release suture or wire 156 and retained within the lumen of pusher 76. After anchor deployment and cinching, release suture or wire 156 may be drawn distally with looped obstructive element 160 retained securely thereto, as shown in FIG. 23B, until obstructive element 160 and release suture or wire 156 have been advanced out of pusher 76. Once free from the constraints of the pusher lumen, obstructive element 160 may be released from release suture or wire 156, as shown in FIG. 23C, to thus release suture element 132'''.

[0112] Turning now to the alternative variation shown in FIGS. 24A to 24C, suture element 132' may be passed through pusher 76'' having heating element assembly 170 disposed upon the distal end of pusher 76''. Heating element assembly 170 may generally comprise a heating element 172, e.g., a resistive metallic conductor such as nichrome, and an insulating element 174 disposed distally of heating element 172, as shown in FIG. 24A. In use, pusher 76'' may be urged distally from needle assembly 66 to cinch the anchors against the tissue surface, as described above. With heating element assembly 170 disposed externally or internally of needle assembly 66, heating element 172 may be powered such that its increase in temperature surpasses the melting point of the suture element 132' passing therethrough, as shown in FIG. 24B. The melting point of the suture 132' will vary depending upon the type of suture utilized.

[0113] Insulating element 174, which may be made from any number of electrically and thermally non-conductive insulating materials such as ceramics, polyimides, etc., may be disposed distal of heating element 172 to prevent inadvertent contact against the tissue by heating element 172 while it is heated although insulating element 174 may be omitted entirely from the assembly 170. As heating element 172 is heated, the portion of suture 132' adjacent to element 172 will be melted and subsequently cut forming melted suture ends 176, 176' on their respective terminal ends of suture element 132' and the remaining suture length 178, as shown in FIG. 24C.

[0114] FIG. 25A shows a partial cross-sectional detail view of the heating element assembly 172 disposed upon the distal end of pusher 76''. As shown, heating element 172 and

insulating element 174 may be positioned adjacent to one another. A covering, coating, or insulating layer 180 (e.g., heatshrink made from FEP, PEEK, Teflon, polyimide, etc.) may be disposed over the heating assembly 170 entirely or at least partially such that heating element 172 is completely encapsulated and insulated from surrounding tissue except for the inner exposed surface within lumen 188, where it may come in contact with or in proximity to the suture for severing the suture element 132'. Electrically conductive wires 182, which may be embedded along the length of pusher 76'', may be routed through heating element assembly 170 via wire contact lumens 184, 186 to not only provide power to heating element 172, but also to provide structural support in maintaining the position of heating element assembly 170 upon the distal end of pusher 76''. Alternatively, the elements 172, 174 of assembly 170 may be attached to one another utilizing any number of mechanical fasteners, e.g., adhesives, threaded connections, interference fitting, etc.

[0115] FIG. 25B shows a partial assembly of pusher 76'' and elements 172, 174 in an exploded view (cover 180 has been omitted for clarity). Wires 182 may pass through heating element assembly 170, along pusher 76'', and proximally into electrical contact with a controller and/or power supply 190 via a standard removable connector or through a direct electrical connection. Controller/power supply 190 may be located externally of the patient as a device separate from pusher 76'' and within or outside a sterile surgical field around the patient. Alternatively, the power supply 190 may be integrated with a proximal portion of the pusher 76''. An actuator 192, such as a foot-operated pedal or hand-operated switch, may be electrically connected via connector 194 to controller/power supply 190 for controlling the actuation of the heating element assembly 170.

[0116] An alternative heating assembly is shown in FIGS. 26A and 26B. FIG. 26A illustrates a partial side view of pusher 76''' having a heating assembly 200 disposed upon the distal end of pusher 76''' with suture element 132' routed therethrough. Heating assembly 200 may generally comprise an insulative body 202 having a circumferentially-defined depression 204. One or more slots, grooves, or openings 206 extending radially through body 202 may be defined within the depression 204 such that an electrically resistive wire 208 which is coiled, wrapped, or otherwise wound around body 202 along depression 204 may effectively transfer heat generated by wire 208 through the one or more openings 206 to melt and separate the portion of suture element 132' positioned within lumen 210 of body 202, as shown in FIG. 26B. A portion of coiled wire 208 may be optionally potted with an insulating material, such as epoxy, within depression 204 to retain the wire 208 in place as well as to insulate the wire 208 from surrounding tissue.

[0117] The heating assembly 200 may be positioned upon the distal end of pusher 76''' utilizing any of the methods described above or generally known. Moreover, conductive wires 182 may be routed along or through pusher 76''' and connected via, e.g., a connector, to controller and/or power supply 190, which may be connected to a foot pedal, hand switch, or other actuator 192, as described above.

[0118] Yet another variation is shown in the partial cross-sectional view of pusher 76''' of FIG. 27A, which shows an alternative heating assembly 220 having a resistive wire or

element 224 encased within a casing or housing 222 which forms a portion of the pusher wall. Although the housing 222 is shown near or at the distal end of pusher 76^{'''}, housing 222 may also be located along the pusher wall proximal to the distal end. FIG. 27B shows a cross-section of a portion of pusher 76^{'''} and housing 222. As shown, resistive wire 224 may be positioned through housing 222 such that heat from the wire 224 may melt or sever the portion of suture 132' adjacent to or in contact with housing 222. As above, wire 224 may be connected to a proximally located controller/power supply 190.

[0119] In the variations described above utilizing a heating element to sever the suture, the heating elements may be powered in a continuous manner until shut off by the user. Alternatively, the power may be configured to operate for a pre-determined period of time once turned on before automatically shutting off. In yet another alternative, the power may pulse in a cyclical manner such that the heating element is heated only for a specified period of time before automatically shutting off for a set period. This cycle may be repeated until the device is turned off. Such features may be incorporated as part of the instrument as a fail-safe feature, is so desired.

[0120] In one example of a cyclical timing profile shown in FIG. 28, once the actuator has been turned on to heat the heating element to sever the suture, the controller connected to the heating element may be configured to pulse the power 230 for a set period of time, Δt , e.g., 1 to 2 seconds. The power may then automatically shut off 234 for a set period of time, Δd , e.g., 1 to 5 seconds; then the power may be automatically turned on again 232 and then off again 236. This may occur for a set number of cycles or for a set period of time before the device is completely shut off or until the user completely shuts the power off upon suture separation.

[0121] In yet another variation for effecting suture separation, an alternative pusher 240 is shown in cross-section in FIG. 29A. Here, pusher 240 may have a needle body 242 with a circumferential cutting edge 244 defined at its distal end, similar to a coring needle, and a lumen 246 defined therethrough for passage of suture element 132'. Once the tissue anchors have been deployed into the tissue, cutting edge 244 may be used to cut or sever suture element 132' passing through pusher 240 and needle body 242. During tissue anchor cinching of the locking mechanism 136 against the tissue anchor, as described above, cutting edge 244 may be optionally tapered to otherwise sized, without obstructing lumen 246, to allow cutting edge 244 to become seated within the locking mechanism 136. Thus, as pusher 240 and needle body 242 abuts against locking mechanism 136 to urge it distally along suture element 132', cutting edge 244 may avoid direct contact against locking mechanism 136 so as to prevent dulling of cutting edge 244.

[0122] Alternatively or additionally, locking mechanism 136 itself may be coated or otherwise covered with a heatshrink material or other soft polymeric material, at least over a proximal portion, so as to present an atraumatic surface to cutting edge 244. In a further alternative, an intermediate element (not shown) made of a suitably soft material, e.g., polymers, may be disposed between needle body 242 and locking mechanism 136 to function as a temporary bumper.

[0123] In use, once the tissue anchors and locking mechanism 136 have been desirably deployed, pusher 240 and

needle body 242 may be extended and the suture element 132' passing through needle body 242 may be simply severed by pulling or urging suture element 132' against cutting edge 244 until separation occurs. In another alternative method for separating suture element 132', FIGS. 30A to 30C illustrate another method utilizing the tissue manipulation assembly described above. Once the tissue anchors and locking mechanism have been deployed from pusher 240 and launch tube 28, as shown in FIG. 30A, lower jaw 20 and upper jaw 22 of the tissue manipulation assembly may be actuated to clamp upon suture element 132', as shown in FIG. 30B.

[0124] The suture element 132' still disposed through pusher 240, which is positioned within the launch tube, may be tensioned at least partially, e.g., by pulling on a proximal end of suture element 132'. With suture element 132' tightly secured between jaw members 20, 22, pusher 240 and needle body 242 may be urged distally through launch tube 28 until cutting edge 244 severs the portion of suture element 132' held tightly by jaw members 20, 22, as shown in FIG. 30C. The tissue manipulation assembly may then be removed from the patient or manipulated to another portion of the body for treatment.

[0125] In yet another variation for suture separation, the tissue manipulation assembly may again be utilized by incorporating a suture cutting element along either or both jaw members 20, 22. For example, as shown in FIG. 31A, a cutting element, e.g., a blade, energizable wire, etc., may be positioned along an upper region 250 of upper jaw 22, or a cutting element may be positioned along a lower region 252 of lower jaw 20, or both may be utilized in combination with one another. FIGS. 31B and 31C show partial side views of upper jaw 22 and deployed launch tube 44 and pivot 30. A cutting blade, for instance, may be positioned adjacent to the launch tube 44 and angled at various directions relative to where the suture exits the launch tube such that the blade does not obstruct deployment of the tissue anchors or suture.

[0126] Placement of the cutting blade, however, is such that the upper jaw 22 may be manipulated to bring the suture element into contact with the blade for severing the suture. FIG. 31B shows blade 254 angled such that cutting edge 256 is directed away from the launch tube 44 opening. Alternatively, blade 154', in FIG. 31C, shows another example where blade 254' may be angled such that cutting edge 256' is directed towards the launch tube 44 opening.

[0127] Rather than integrating a cutting blade along upper jaw 22, one or more cutting blades may instead be incorporated along lower jaw 20. As shown in the example of FIG. 31D, a partial top view of lower jaw 20 is shown with an optional cutting blade 258 with cutting edge 260 integrated near a proximal portion of needle assembly opening 50 defined in lower jaw member 20. Another alternative is shown in FIG. 31E where a cutting blade 258' having a cutting edge 260' may be integrated along a side portion of opening 50. These examples shown are intended to be illustrative and not limited and one or more cutting blades may be integrated along other surfaces of the tissue manipulation assembly as desired. Moreover, cutting blades may be integrated along the lower jaw, upper jaw, or both if so desired. Furthermore, the cutting blades may additionally be energized in further variations to facilitate severing the suture.

[0128] Turning now to FIG. 32, needle deployment assembly 270 is shown as a variation which is similar to that illustrated above in FIGS. 15 and 23. In this example, needle deployment assembly 270 is configured to endoluminally deploy tissue anchors as well as cinch and release anchor assemblies to secure one or more tissue folds. Assembly 270 generally comprises a needle assembly control or housing 272 which may be configured into an elongate shape having a guide track 274 defined therealong. A first locking position 276 may be defined at a proximal end of guide track 274 and a second locking position 278 may be defined at a distal end of guide track 274 where each locking position 276, 278 may be configured, e.g., as a cut-out or transverse section of guide track 274, within which a slidable actuation member 286 (described below) may be parked or locked temporarily.

[0129] Retraction control element 280 may be removably connected via a coupling mechanism such as a threaded connection 282 to the proximal end of control or housing 272 and tubular catheter or sheath 64 may be coupled via sheath attachment 284 at the distal end of control or housing 272. Needle assembly 66, including needle body 72 having needle opening 74, may be attached to the distal end sheath 64, as described above.

[0130] Needle deployment assembly 270 may operate in a similar manner as the variation described above where once needle body 72 has pierced through approximated tissue T, distal anchor 82 may be deployed through needle opening 74 on a distal side of tissue T, as shown in FIG. 33A. Suture element 132 may be seen connecting distal anchor 82 through the pierced tissue T and through needle opening 74. A terminal distal end of suture element 132 may define a distal knot or protrusion 133 to prevent distal anchor 82 from sliding off suture 132. Distal anchor 82, which is originally positioned within sheath 64 proximal or adjacent to needle body 72, may be urged distally through needle opening 74 by sliding actuation member 286 from its parked position in first locking position 276 distally along guide track 274 to a mid-point location. Actuation member 286 may be connected to slider carriage 290 translatable positioned within housing lumen 298 in control or housing 272, as shown in FIG. 33B.

[0131] Slider carriage 290 may be connected to pusher tube 294, which may comprise a hollow tubular member, such as a hypotube, extending at least partially through control or housing 272 and which may extend partly through sheath 64. A distal end of pusher tube 294 may in turn be connected via coil attachment 308 to pusher coil body 296 which may extend through sheath 64 proximal to an anchor assembly disposed within the distal portion of sheath 64. Pusher coil body 296 may be comprised of a tightly-wound coiled body which provides columnar support when pushed or pulled through sheath 64 and which is sufficiently flexible to enable pusher coil body 296 to conform to tortuous configurations. A wire lumen 292 may extend through carriage 290, pusher tube 294, and pusher coil body 296 within which a looped release suture or wire 156 may extend from retraction control member 280 to a cinchable anchor assembly positioned within a distal portion of sheath 64.

[0132] A stop 300 may be crimped or otherwise fixedly positioned along a length of release suture or wire 156 within housing or control 272 with a separate plug mecha-

nism 302 slidably positioned along suture or wire 156 proximal to stop 300. Plug 302 may have a plug body 304 with one or more expandable arms 306 extending distally therefrom, the distal ends of which are temporarily locked within a proximal opening of lumen 292, as illustrated in FIG. 33B. With expandable arms 306 temporarily locked in carriage 290 and encompassing stop 300, when actuation member 286 is pushed distally along guide track 274, carriage 290 is forced distally to urge pusher tube 294 and pusher coil body 296 through sheath 64. Stop 300 is also urged distally along with carriage 290 by plug mechanism 302, which in turn enables the distal portion of looped suture or wire 156 to translate distally with pusher coil body 296 to push the distal anchor 82 from needle body 72, as shown in FIG. 33C. The proximal terminal end 310 of suture element 132 may be passed at least partially through looped suture or wire 156 within pusher coil body 296 such that when suture end 310 is withdrawn within pusher coil body 296 by suture or wire 156, suture end 310 is fixedly retained and prevented from inadvertently releasing or unwinding by the tortuous looped path to prevent the accidental release of one or more anchors 82, 84 from needle body 72.

[0133] Once the distal anchor 82 has been released on a distal side of tissue T, proximal anchor 84 may further be released on a proximal side of tissue T by further urging actuation member 286 distally along guide track 274 until actuation member 286 has reached the terminal end of track 274, where it may be locked into the second locking position 278. Pushing actuation member 286 along track 274 may urge the distal end of pusher coil body 296 distally until it is adjacent to or distal of needle body 72, thereby forcing proximal anchor 84 and locking mechanism 136 from needle opening 74, as illustrated in FIG. 34A. FIG. 34B illustrates the distal movement within control or housing 272 of stop 300 and plug body 304 attached to carriage 290 via expandable arms 306. FIG. 34C illustrates the corresponding distal translation of pusher coil body 296 and release suture or wire 156 through needle opening 74 to urge proximal anchor 84 and locking mechanism 132 therethrough. Terminal suture end 310 is still fixedly retained within pusher coil body 296 by release suture or wire 156.

[0134] To approximate the anchors 82, 84 towards one another and secure the plicated tissue T, retraction control element 280 may be de-coupled or unscrewed via attachment 282 from the proximal end of control or housing 272, as shown in FIG. 34A, and then pulled proximally or tensioned, as shown in FIG. 35A, to pull release suture or wire 156 proximally relative to carriage 290, pusher tube 294, pusher coil body 296, and housing 272. As release wire 156 is pulled, stop 300 is pulled proximally, which in turn may urge plug body 304 proximally relative to the stationary carriage 290. As the plug mechanism is forced proximally, expandable arms 306 may become released from the proximal end of carriage 290 to reconfigure themselves into an expanded configuration, as shown in FIG. 35B.

[0135] Moreover, as release wire 156 is tensioned, the terminal looped end 310 of suture 132, which is threaded at least partially through the looped distal end of release wire 156, may be pulled proximally further into pusher coil body 296, as shown in FIG. 35C, to force the distal knot or protrusion 133 against the distal anchor 82 to approximate anchor 82 towards proximal anchor 84 and locking mecha-

nism 136, thereby securing the plicated tissue T between the collapsed tissue anchors 82, 84.

[0136] With plicated tissue T securely cinched between anchors 82, 84 and locking mechanism 136, actuation member 286 may be released from second locking position 278 and urged proximally along guide track 274, as illustrated in FIG. 36A. The proximal translation of actuation mechanism 286 and carriage 290 may pull pusher tube 294 and pusher coil body 296 proximally relative to sheath 64. As carriage is translated through control or housing 272, stop 300 may pass freely into and through lumen 292 while the expandable arms 306 projecting from plug body 304 may inhibit or prevent the plug from re-entering carriage 290. Accordingly, plug body 304 may be forced to slide proximally along release suture or wire 156, as shown in FIG. 36B.

[0137] With stop 300 freely translating within lumen 292, the tension on release suture or wire 156 from suture element 132 and secured anchors 82, 84 may urge the distal looped end of wire 156 out of pusher coil body 296, thereby allowing suture element 132 to release itself from release suture or wire 156, as illustrated in FIG. 36C. However, stop 300 may be sized with a diameter which is larger than an inner diameter of pusher coil body 296 such that stop 300 is prevented from passing distally into pusher coil body 296. This feature may be utilized to limit the withdrawal of release suture or wire 156 and prevent it from being pulled entirely out of pusher coil body 296 when the anchors are released. Once suture element 132 has been released, needle deployment assembly 270 may be removed from the tissue manipulation assembly 14 or other instrument or from the patient body and another needle deployment assembly 270 may be reinserted to secure another region of tissue.

[0138] Although a number of illustrative variations are described above, it will be apparent to those skilled in the art that various changes and modifications may be made thereto without departing from the scope of the invention. Moreover, although specific configurations and applications may be shown, it is intended that the various features may be utilized in various combinations and in various types of procedures as practicable. It is intended in the appended claims to cover all such changes and modifications that fall within the true spirit and scope of the invention.

What is claimed is:

1. A tissue anchor deployment system, comprising:
 - a housing having a guide defined along a length of the housing;
 - an elongate flexible shaft with a lumen defined there-through and having a proximal end attached to the housing and a distal end having a piercing body attached thereto;
 - an elongate pusher member slidably disposed at least within the elongate shaft;
 - a retraction control member removably connected to the housing; and
 - a release wire slidably disposed within the elongate shaft and secured at a proximal end to the retraction control member.
2. The system of claim 1 wherein the guide defined along the length comprises a channel.

3. The system of claim 1 wherein the guide further defines at least a first locking position along the housing.

4. The system of claim 3 wherein the guide further defines at least a second locking position along the housing.

5. The system of claim 1 further comprising an actuation member translatable along the guide and attached to a proximal end of the elongate pusher member.

6. The system of claim 5 wherein the actuation member comprises a carriage slidably positioned within the housing, the carriage defining a lumen through which the release wire is disposed.

7. The system of claim 1 wherein the elongate flexible shaft comprises a catheter shaft.

8. The system of claim 1 wherein the piercing body comprises a needle body having a lumen defined there-through.

9. The system of claim 1 wherein the elongate pusher member comprises a hollow tubular member having a length.

10. The system of claim 9 wherein the elongate pusher member further comprises a coiled body which is adapted to provide column support when pushed or pulled through the elongate flexible shaft.

11. The system of claim 1 further comprising a stop fixedly attached to a portion of the release wire.

12. The system of claim 11 wherein the stop has a diameter sized to inhibit movement through at least part of the elongate pusher member.

13. The system of claim 11 further comprising a plug member slidably located along the release wire proximal to the stop.

14. The system of claim 13 wherein the plug member comprises one or more expandable arms projecting radially from a plug body in an expanded configuration and over or around the stop in a low-profile configuration.

15. The system of claim 14 wherein the one or more expandable arms are positionable around the stop such that distal ends of the one or more expandable arms are constrained within a proximal end of a carriage positioned within the housing.

16. The system of claim 1 wherein the retraction control member comprises a threaded attachment for connection to the housing.

17. The system of claim 1 wherein the release wire comprises a nitinol wire.

18. The system of claim 1 wherein the release wire forms a loop through the elongate shaft.

19. The system of claim 18 wherein the release wire forms a loop through a length of the elongate pusher member.

20. The system of claim 1 further comprising a deployable tissue anchor assembly slidably positioned within a portion of the elongate shaft distally of the elongate pusher member.

21. The system of claim 20 wherein the tissue anchor assembly comprises at least a first tissue anchor and a second tissue anchor connected by a length of suture.

22. The system of claim 21 wherein a terminal end of the length of suture is passed at least partially through or around the release wire within the elongate shaft.

23. The system of claim 21 further comprising a locking mechanism slidably positioned along the length of suture between the tissue anchor assembly and the elongate pusher member.

24. The system of claim 1 further comprising a tissue grasping tool pivotably coupled to a distal end of an outer

flexible shaft and adapted to be advanced endoluminally into a body lumen, wherein the elongate flexible shaft with the distal end having a piercing body is sized for advancement through the outer flexible shaft and through the tissue grasping tool.

25. The system of claim 24 wherein the tissue grasping tool comprises a first jaw member pivotably coupled to a distal end of the outer flexible shaft, a second jaw member pivotably coupled along the first jaw member, and a launch tube member adapted to urge the first and second jaw members between a low-profile delivery configuration and an expanded grasping configuration.

26. The system of claim 24 further comprising a tissue engagement device having a helical tissue engager adapted to reversibly engage tissue and further adapted to be positioned endoluminally within the body lumen adjacent to the tissue grasping tool.

27. The system of claim 24 further comprising an endoluminal elongate body adapted to transition between a flexible state and a rigid state, wherein the tissue grasping tool and the elongate flexible shaft are removably advanceable there-through.

28. The system of claim 27 wherein the endoluminal elongate body comprises a steerable distal portion.

29. A method of securing tissue within a hollow body organ, comprising:

endoluminally advancing through engaged tissue an elongate flexible shaft having a proximal end attached to a housing and a distal end having a piercing body attached thereto;

actuating an actuation member on the housing to urge an elongate pusher member distally through the elongate flexible shaft such that a first tissue anchor is urged from the piercing body into or against a first side of the engaged tissue;

retracting the elongate flexible shaft to a second side of the engaged tissue;

further actuating the actuation member on the housing to urge the elongate pusher member further distally through the elongate flexible shaft such that a second tissue anchor is urged from the piercing body into or against a second side of the engaged tissue;

tensioning a release wire proximally through the elongate flexible shaft such that a suture element connecting the first and second tissue anchors is tensioned and a stop attached to a portion of the release wire is freed from a plug member located along the release wire proximally of the stop;

retracting the elongate pusher member relative to the elongate flexible shaft such that a distal looped portion of the release wire is exposed to release a terminal end of the suture element.

30. The method of claim 29 wherein endoluminally advancing comprises advancing the elongate flexible shaft trans-esophageally into a stomach.

31. The method of claim 29 wherein actuating an actuation member comprises distally advancing a slide mechanism along the housing to urge the elongate pusher member relative to the elongate flexible shaft.

32. The method of claim 31 further comprising unlocking the actuation member from a first locking position along the housing prior to actuating an actuation member.

33. The method of claim 31 further comprising locking the actuation member into a second locking position along the housing prior to tensioning a release wire.

34. The method of claim 29 wherein further actuating comprises distally advancing a slide mechanism along the housing to a distal position to urge the elongate pusher member relative to the elongate flexible shaft.

35. The method of claim 29 wherein tensioning comprises pulling the release wire proximally through the elongate flexible shaft and housing.

36. The method of claim 29 wherein tensioning comprises approximating the first and second tissue anchors towards one another to secure the engaged tissue therebetween.

37. The method of claim 29 wherein tensioning further comprises uni-directionally advancing a locking mechanism along the suture element proximal to the first and second tissue anchors.

38. The method of claim 29 wherein retracting comprises distally passing the stop at least partially into the elongate pusher member to expose the distal looped portion of the release wire.

39. The method of claim 29 further comprising grasping the tissue within the hollow body organ with a tissue grasping instrument prior to actuating an actuation member.

40. The method of claim 39 wherein endoluminally advancing comprises advancing the elongate flexible shaft through the tissue grasping instrument.

41. The method of claim 40 further comprising advancing the tissue grasping instrument along or through a flexible body with a steerable distal section, wherein the flexible body is adapted to be rigidized to maintain an arbitrary shape.

* * * * *

专利名称(译)	用于固定和展开组织锚的方法和设备		
公开(公告)号	US20060271074A1	公开(公告)日	2006-11-30
申请号	US11/412261	申请日	2006-04-26
[标]申请(专利权)人(译)	EWERS RICHARDÇ 林苍Ç		
申请(专利权)人(译)	EWERS RICHARDÇ 林苍Ç		
当前申请(专利权)人(译)	USGI MEDICAL , INC.		
[标]发明人	EWERS RICHARD C LAM CANG C		
发明人	EWERS, RICHARD C. LAM, CANG C.		
IPC分类号	A61B17/04		
CPC分类号	A61B17/0401 A61B17/0467 A61B17/0469 A61B17/0482 A61B17/29 A61B2017/003 A61B2017/2927 A61B2017/00867 A61B2017/0419 A61B2017/0458 A61B2017/0464 A61B2017/0496 A61B2017/06052 A61B2017/00349		
其他公开文献	US8298291		
外部链接	Espacenet USPTO		

摘要(译)

本文描述了用于固定和展开组织锚的方法和装置。组织操纵组件可枢转地联接到管状构件的远端。可重新配置的发射管也可枢转地耦合到组织操纵组件，其可以通过可形状锁定的内窥镜装置，传统的内窥镜或者直接自身进入患者体内。第二工具可以与组织操纵组件结合使用，以与组织操纵组件一起接合组织并操纵组织。提供了一种展开组件，用于通过一个或多个组织锚固件固定接合的组织，该展开组件还构造通过沿着展开组件设置的至少一个缝合线切割元件施加热能而在腔内或腹腔镜下脱离锚固件。

