



US007483755B2

(12) **United States Patent**
Ingle et al.

(10) **Patent No.:** **US 7,483,755 B2**
(45) **Date of Patent:** ***Jan. 27, 2009**

(54) **DEVICES, METHODS, AND SYSTEMS FOR SHRINKING TISSUES**

(76) Inventors: **Frank Ingle**, 814 Richardson Ct., Palo Alto, CA (US) 94303; **Garry Carter**, 3083 Crestblanca Dr., Pleasanton, CA (US) 94566; **Michael D. Laufer**, 1259 El Camino Real, Menlo Park, CA (US) 94025

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 801 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **10/463,976**

(22) Filed: **Jun. 17, 2003**

(65) **Prior Publication Data**

US 2004/0034400 A1 Feb. 19, 2004

Related U.S. Application Data

(60) Continuation of application No. 09/441,109, filed on Nov. 16, 1999, now Pat. No. 6,772,013, which is a division of application No. 08/910,370, filed on Aug. 13, 1997, now Pat. No. 6,091,995, which is a continuation-in-part of application No. 08/862,875, filed on May 23, 1997, now abandoned, which is a continuation-in-part of application No. 08/748,527, filed on Nov. 8, 1996, now abandoned.

(51) **Int. Cl.**
A61B 5/01 (2006.01)

(52) **U.S. Cl.** **607/138**; 607/101; 607/102;
606/41; 606/46

(58) **Field of Classification Search** 606/41-50;
607/96, 98-99, 101-102

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

373,399 A 11/1887 Hamilton
3,575,158 A 4/1971 Summers
3,749,098 A 7/1973 De Bennetot
3,924,631 A 12/1975 Marcusi, Jr.
3,926,175 A 12/1975 Allen et al.

FOREIGN PATENT DOCUMENTS

GB 9715237 5/1997

(Continued)

OTHER PUBLICATIONS

Benson, Thomas J., *Female Pelvic Floor Disorders: Investigation and Management*, Norton Medical Books, W.W. Norton & Company, New York, 1992, pp. 239-240.

(Continued)


Primary Examiner—Roy D Gibson

(74) *Attorney, Agent, or Firm*—Oppenheimer Wolff & Donnelly LLP

(57) **ABSTRACT**

Devices, systems, and method for treating urinary incontinence generally rely on energy delivered to a patient's own pelvic support tissue to selectively contract or shrink at least a portion of that pelvic support tissue so as to reposition the bladder. The energy will preferably be applied to the endopelvic fascia and/or an arcus tendineus fascia pelvis. The invention provides a variety of devices and methods for applying gentle resistive heating of these and other tissues to cause them to contract without imposing significant injury on the surrounding tissue structures. Alternatively, heat-applying probes are configured to heat tissue structures which comprise or support a patient's urethra. By applying sufficient energy over a predetermined time, the tissue can be raised to a temperature which results in contraction without significant necrosis or other tissue damage. By selectively contracting the support tissues, the bladder neck, sphincter, and other components of the urinary tract responsible for the control of urinary flow can be reconfigured or supported in a manner which reduces urinary leakage.

30 Claims, 22 Drawing Sheets

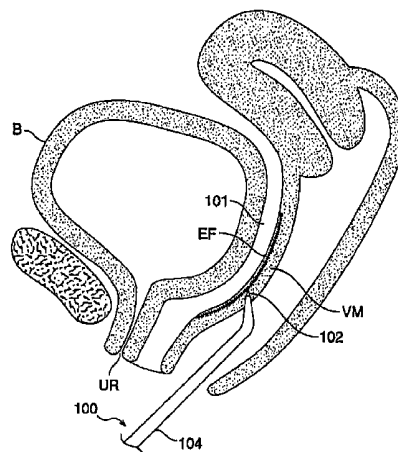

U.S. PATENT DOCUMENTS

| | | | | | | | |
|-----------|---|---------|--------------------|--------------|------|---------|----------------------------|
| 3,939,821 | A | 2/1976 | Roth | 5,609,598 | A | 3/1997 | Laufer et al. |
| 4,311,145 | A | 1/1982 | Esty et al. | 5,681,282 | A | 10/1997 | Eggers et al. |
| 4,326,529 | A | 4/1982 | Doss et al. | 5,683,384 | A | 11/1997 | Gough et al. |
| 4,409,453 | A | 10/1983 | Smith | 5,683,451 | A | 11/1997 | Lenker et al. |
| 4,453,536 | A | 6/1984 | Abild | 5,697,281 | A | 12/1997 | Eggers et al. |
| 4,686,962 | A | 8/1987 | Haber | 5,697,536 | A | 12/1997 | Eggers et al. |
| 4,765,331 | A | 8/1988 | Petruzzi et al. | 5,697,882 | A | 12/1997 | Eggers et al. |
| 4,773,393 | A | 9/1988 | Haber et al. | 5,697,909 | A | 12/1997 | Eggers et al. |
| 4,776,344 | A | 10/1988 | Shirasaki et al. | 5,707,367 | A | 1/1998 | Nilsson |
| 4,802,479 | A | 2/1989 | Haber et al. | 5,709,224 | A | 1/1998 | Behl et al. |
| 4,807,620 | A | 2/1989 | Strul et al. | 5,716,385 | A | 2/1998 | Mittal et al. |
| 4,832,680 | A | 5/1989 | Haber et al. | 5,728,119 | A | 3/1998 | Smith et al. |
| 4,994,019 | A | 2/1991 | Fernandez et al. | 5,782,824 | A * | 7/1998 | Abela et al. 606/15 |
| 5,012,822 | A | 5/1991 | Schwarz | 5,810,847 | A | 9/1998 | Laufer et al. |
| 5,035,696 | A | 7/1991 | Rydell | 5,868,742 | A | 2/1999 | Manes et al. |
| 5,041,109 | A | 8/1991 | Abela | 5,921,954 | A | 7/1999 | Mohr et al. |
| 5,057,106 | A | 10/1991 | Kasevich et al. | 5,954,720 | A | 9/1999 | Wilson et al. |
| 5,098,429 | A | 3/1992 | Sterzer | 5,957,920 | A | 9/1999 | Baker |
| 5,103,804 | A | 4/1992 | Abele et al. | 5,957,961 | A | 9/1999 | Maguire et al. |
| 5,140,999 | A | 8/1992 | Ardito | 5,964,755 | A | 10/1999 | Edwards |
| 5,190,517 | A | 3/1993 | Zieve et al. | 6,015,406 | A | 1/2000 | Goble et al. |
| 5,201,732 | A | 4/1993 | Parins et al. | 6,044,846 | A | 4/2000 | Edwards |
| 5,213,097 | A | 5/1993 | Zeindler | 6,056,744 | A | 5/2000 | Edwards |
| 5,230,334 | A | 7/1993 | Klopotek | 6,073,052 | A | 6/2000 | Zelickson et al. |
| 5,234,409 | A | 8/1993 | Goldberg et al. | 6,159,194 | A | 12/2000 | Eggers et al. |
| 5,256,133 | A | 10/1993 | Spitz | 6,169,926 | B1 | 1/2001 | Baker |
| 5,281,217 | A | 1/1994 | Edwards et al. | 6,197,022 | B1 | 3/2001 | Baker |
| 5,281,218 | A | 1/1994 | Imran | 6,228,078 | B1 | 5/2001 | Eggers et al. |
| 5,282,799 | A | 2/1994 | Rydell | 6,241,753 | B1 | 6/2001 | Knowlton |
| 5,293,869 | A | 3/1994 | Edwards et al. | 6,277,116 | B1 | 8/2001 | Utely et al. |
| 5,304,123 | A | 4/1994 | Atala et al. | 6,419,673 | B1 * | 7/2002 | Edwards et al. 606/41 |
| 5,309,910 | A | 5/1994 | Edwards et al. | 6,425,877 | B1 | 7/2002 | Edwards |
| 5,314,465 | A | 5/1994 | Maurer et al. | 6,428,538 | B1 | 8/2002 | Blewett et al. |
| 5,314,466 | A | 5/1994 | Stern et al. | 6,463,331 | B1 | 10/2002 | Edwards |
| 5,366,490 | A | 11/1994 | Edwards et al. | 6,470,219 | B1 | 10/2002 | Edwards et al. |
| 5,370,671 | A | 12/1994 | Maurer et al. | 6,692,490 | B1 | 2/2004 | Edwards |
| 5,370,675 | A | 12/1994 | Edwards et al. | 2003/0036804 | A1 | 2/2003 | Thomas et al. |
| 5,370,677 | A | 12/1994 | Rudie et al. | 2003/0181897 | A1 | 9/2003 | Thomas et al. |
| 5,370,678 | A | 12/1994 | Edwards et al. | | | | |
| 5,376,064 | A | 12/1994 | Cerny | | | | |
| 5,385,544 | A | 1/1995 | Edwards et al. | | | | |
| 5,403,312 | A | 4/1995 | Yates et al. | | | | |
| 5,405,346 | A | 4/1995 | Grundy et al. | | | | |
| 5,411,475 | A | 5/1995 | Atala et al. | | | | |
| 5,431,649 | A | 7/1995 | Mulier et al. | | | | |
| 5,437,603 | A | 8/1995 | Cerny et al. | | | | |
| 5,437,664 | A | 8/1995 | Cohen et al. | | | | |
| 5,447,529 | A | 9/1995 | Marchlinski et al. | | | | |
| 5,454,809 | A | 10/1995 | Janssen | | | | |
| 5,458,596 | A | 10/1995 | Lax et al. | | | | |
| 5,458,597 | A | 10/1995 | Edwards et al. | | | | |
| 5,462,545 | A | 10/1995 | Wang et al. | | | | |
| 5,496,312 | A | 3/1996 | Klicek | | | | |
| 5,505,730 | A | 4/1996 | Edwards | | | | |
| 5,514,130 | A | 5/1996 | Baker | | | | |
| 5,514,155 | A | 5/1996 | Daneshvar | | | | |
| 5,533,999 | A | 7/1996 | Hood et al. | | | | |
| 5,540,684 | A | 7/1996 | Hassler, Jr. | | | | |
| 5,556,396 | A | 9/1996 | Cohen et al. | | | | |
| 5,558,672 | A | 9/1996 | Edwards et al. | | | | |
| 5,562,720 | A | 10/1996 | Stern et al. | | | | |
| 5,569,241 | A | 10/1996 | Edwards | | | | |
| 5,569,242 | A | 10/1996 | Lax et al. | | | | |
| 5,575,788 | A | 11/1996 | Baker et al. | | | | |
| 5,588,960 | A | 12/1996 | Edwards et al. | | | | |

FOREIGN PATENT DOCUMENTS

| | | |
|----|-------------|---------|
| WO | WO93/07815 | 4/1993 |
| WO | WO96/00041 | 1/1996 |
| WO | WO96/00042 | 1/1996 |
| WO | WO 97/15237 | 5/1997 |
| WO | WO97/15238 | 5/1997 |
| WO | WO97/32532 | 9/1997 |
| WO | WO97/39688 | 10/1997 |
| WO | WO97/43970 | 11/1997 |
| WO | WO97/43971 | 11/1997 |
| WO | WO98/07468 | 2/1998 |
| WO | WO98/38936 | 9/1998 |

OTHER PUBLICATIONS

Finger, Paul T. et al., "Heat Shrinkage of Extraocular Muscle Tendon," *Arch. Ophthalmol.*, vol. 105, May, 1987, pp. 716-718.

Hayes et al., "Prediction of Transient Temperature Fields and Cumulative Tissue Destruction for Radio Frequency Heating of a Tumor," *Medical Physics*, University of Texas, Austin, Texas; 12(6):1985.

Raz, Shlomo, *Female Urology*, Second Edition, W. B. Saunders Company, Philadelphia, Pennsylvania, 1996, pp. 126, 340-342, and 356-357.

Brant R. Fulmer et al., "Acute and Long-Term Outcomes of Radio Frequency Bladder Neck Suspension," *The Journal of Urology*, vol. 167, 141-145, Jan. 2002.

* cited by examiner

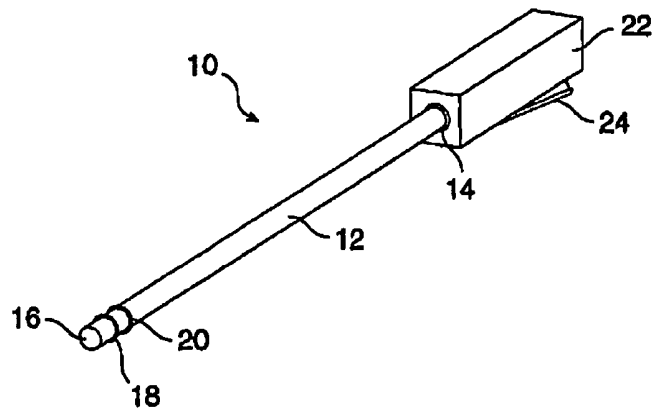


FIG. 1

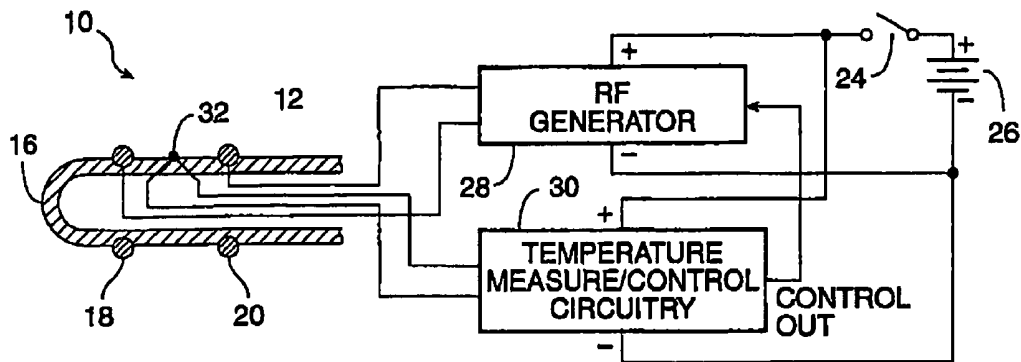


FIG. 2

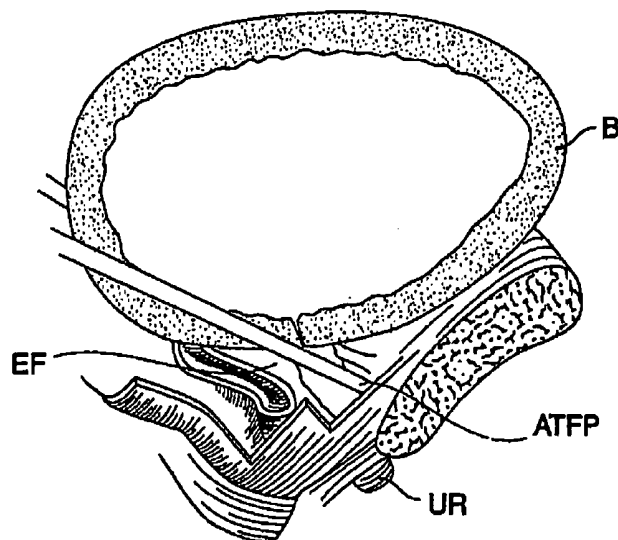


FIG. 3

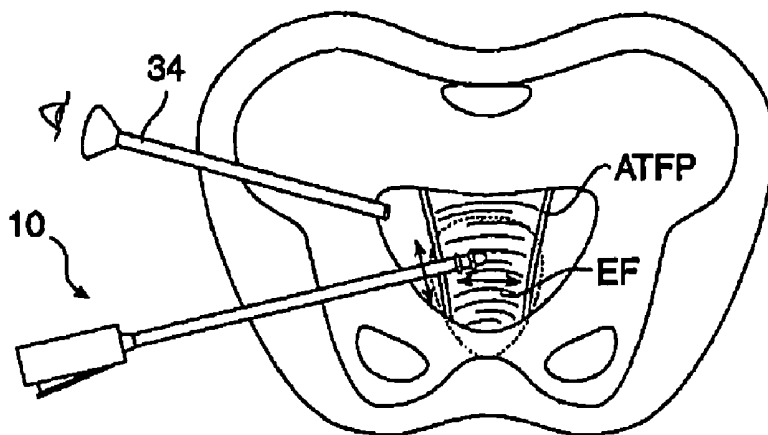


FIG. 4

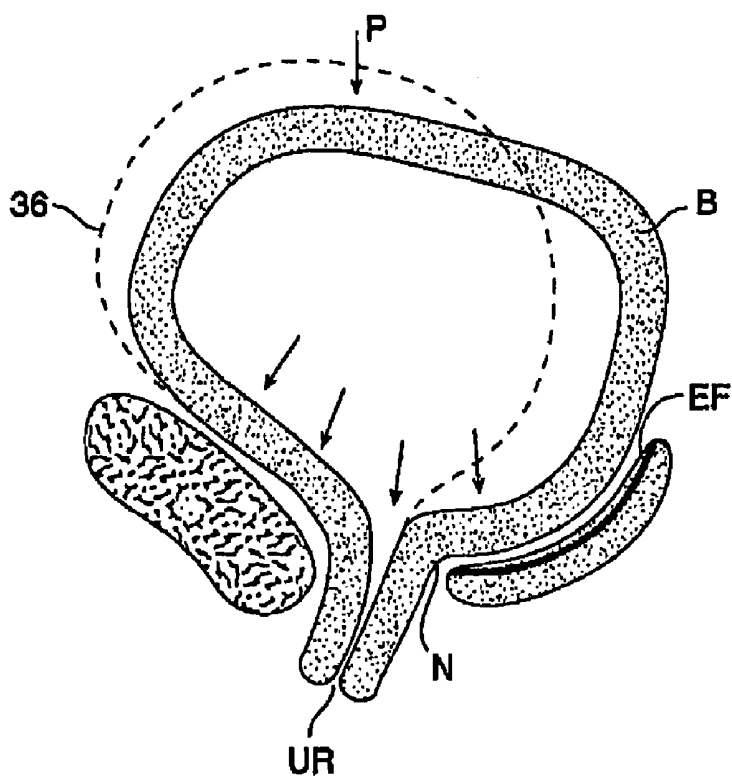


FIG. 5

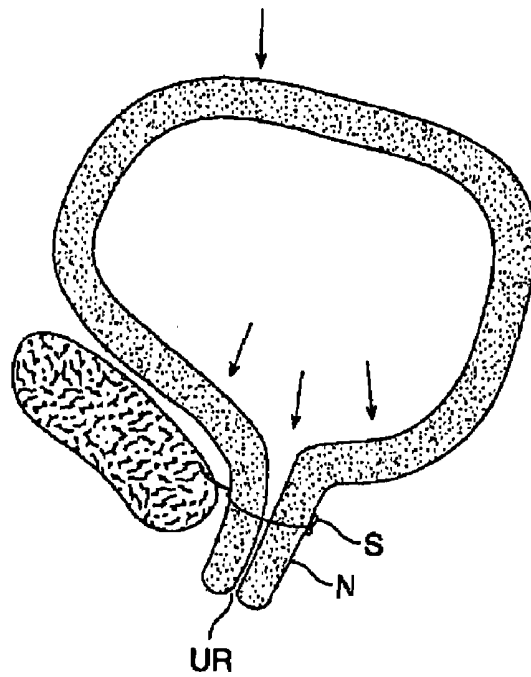


FIG. 6

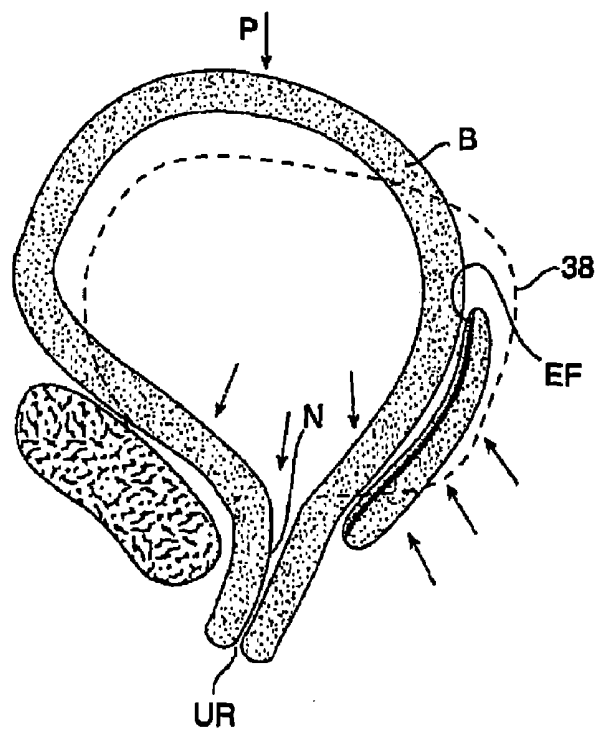


FIG. 7

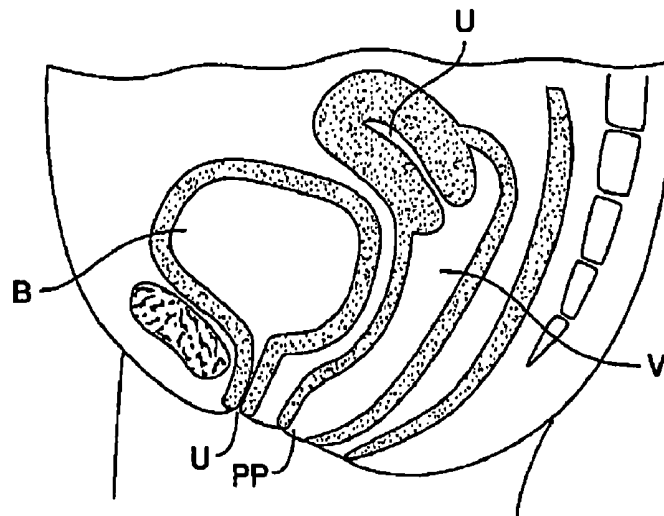


FIG. 7A

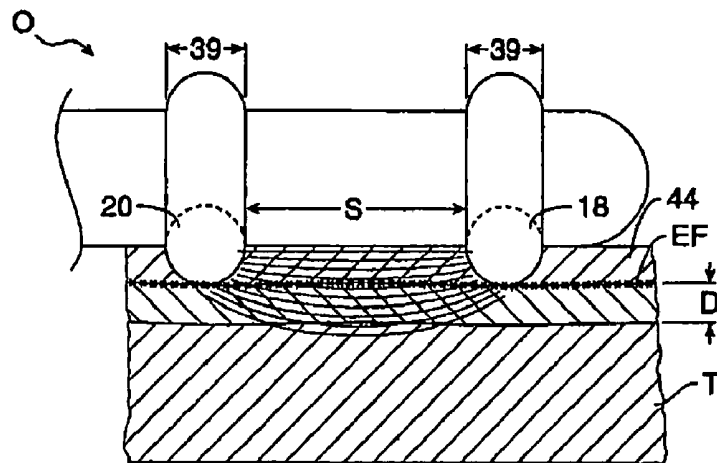


FIG. 8

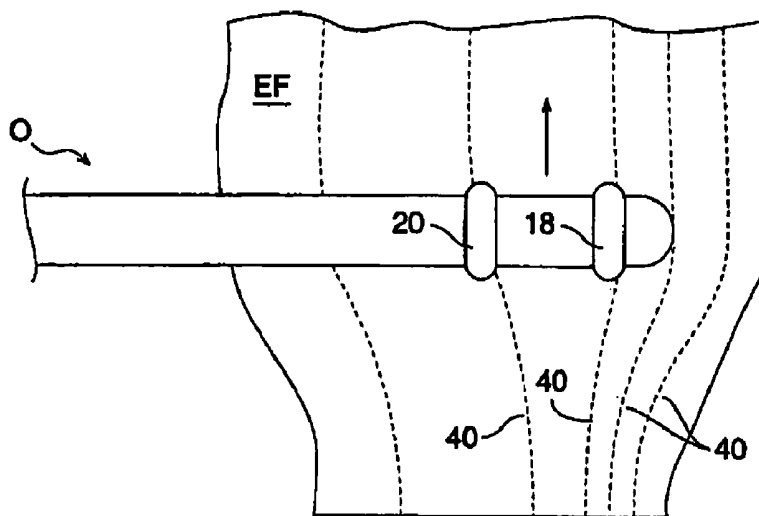


FIG. 9

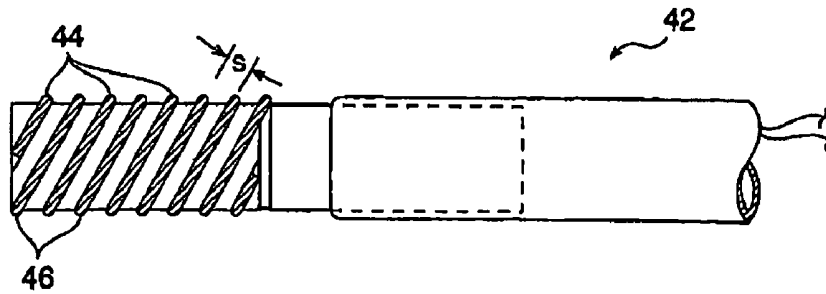


FIG. 10

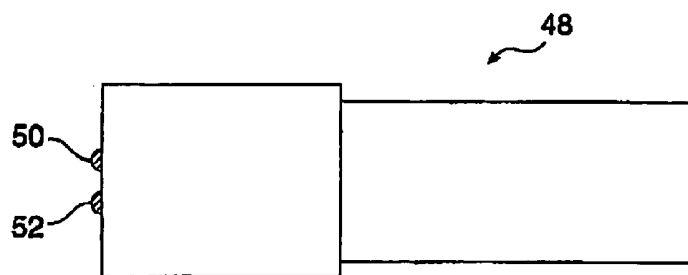


FIG. 11A

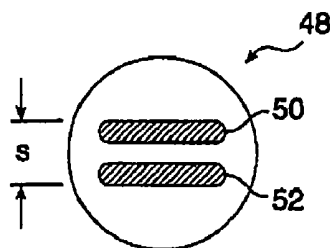


FIG. 11B

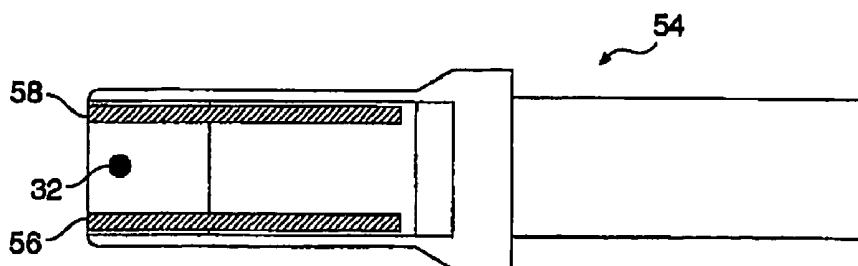


FIG. 12A

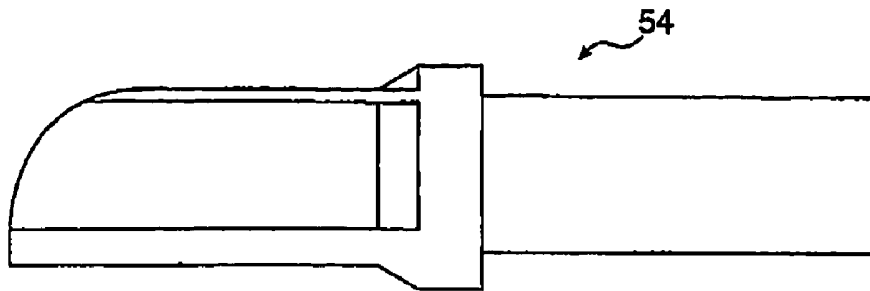


FIG. 12B

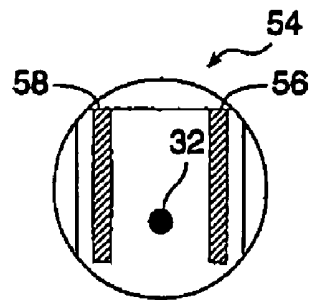


FIG. 12C

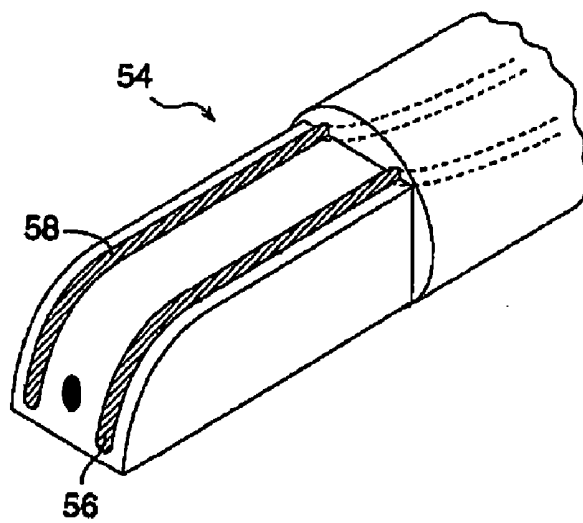
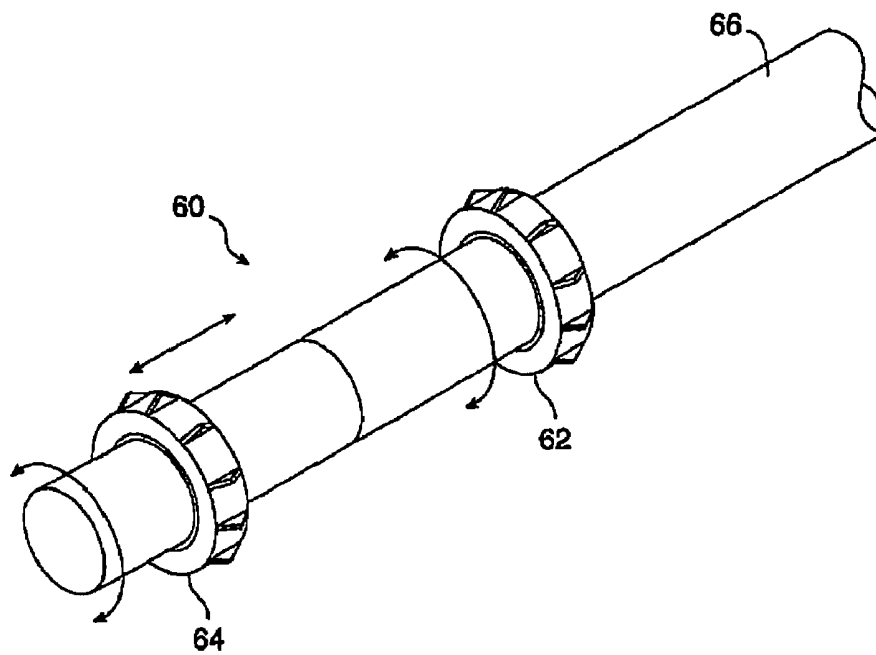
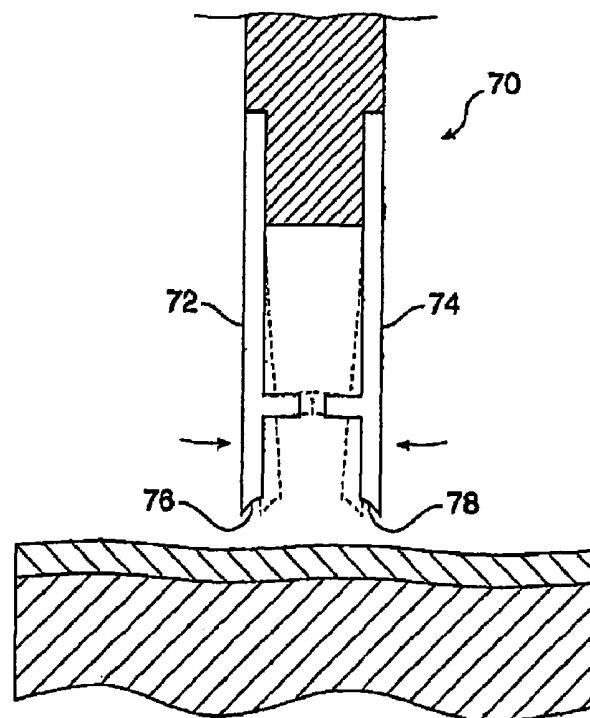


FIG. 12D

*FIG. 13A**FIG. 13B*

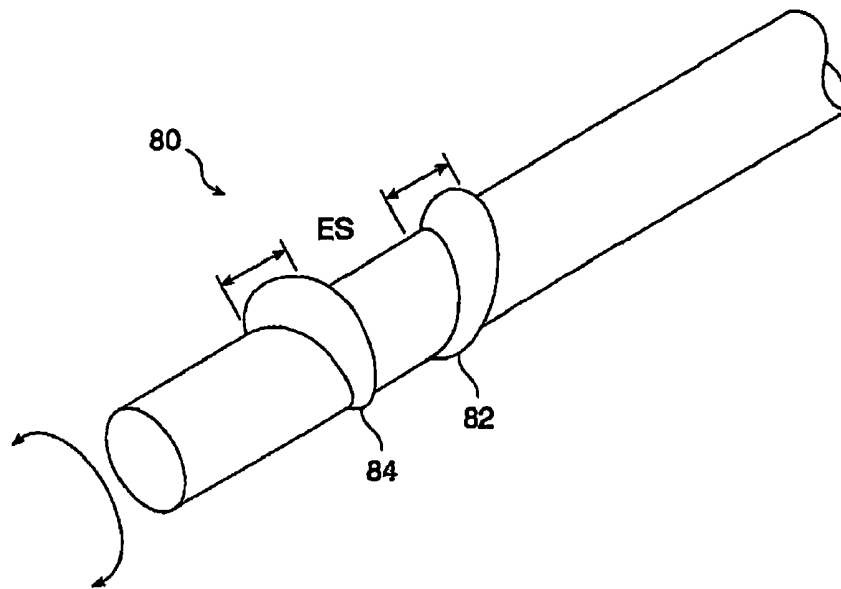


FIG. 13C

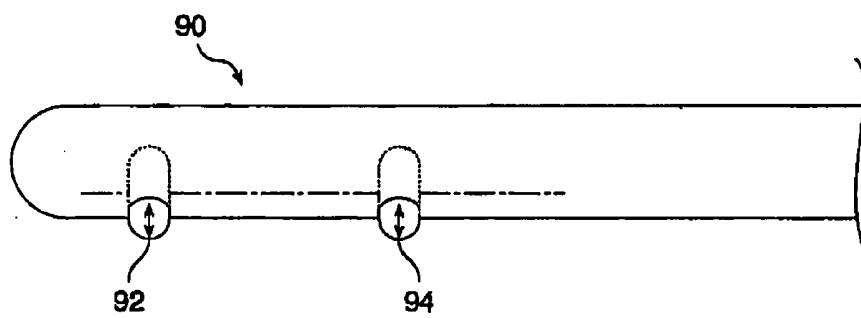


FIG. 14

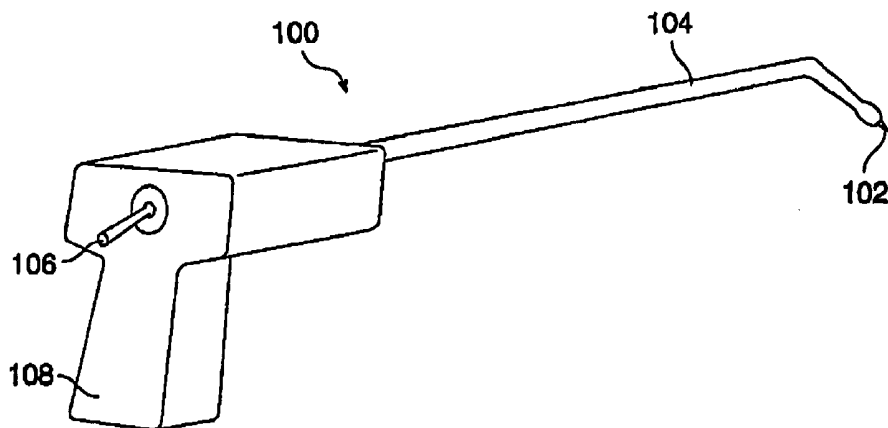


FIG. 15

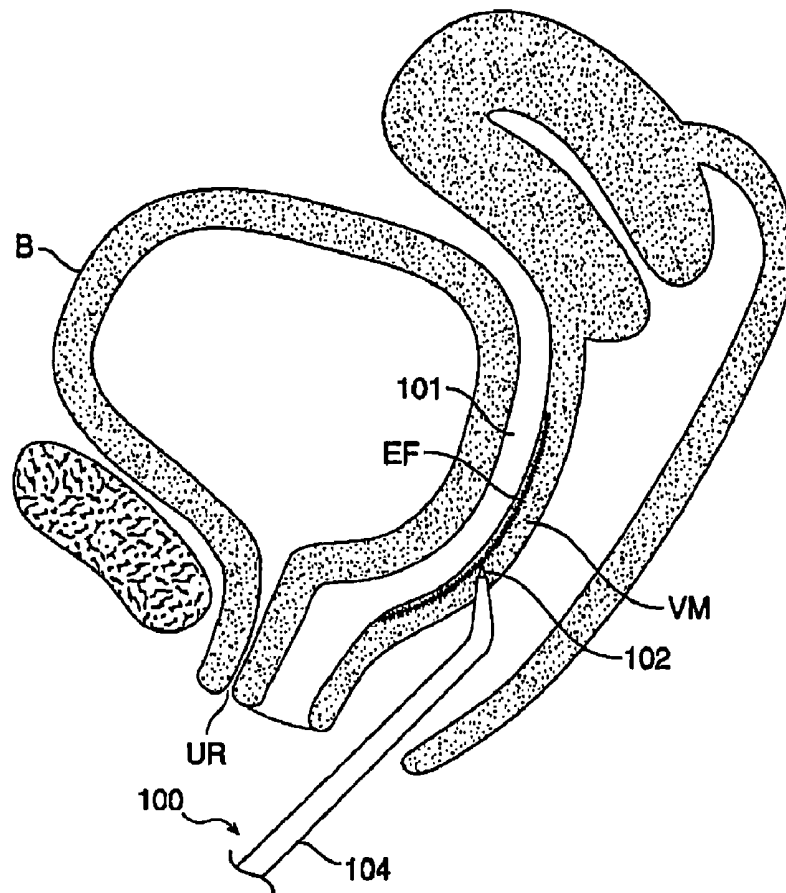


FIG. 15A

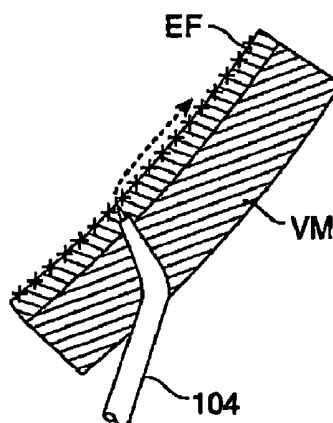


FIG. 15B

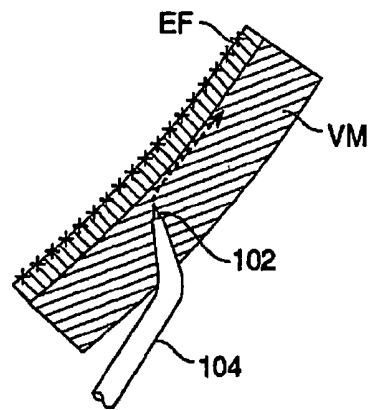


FIG. 15C

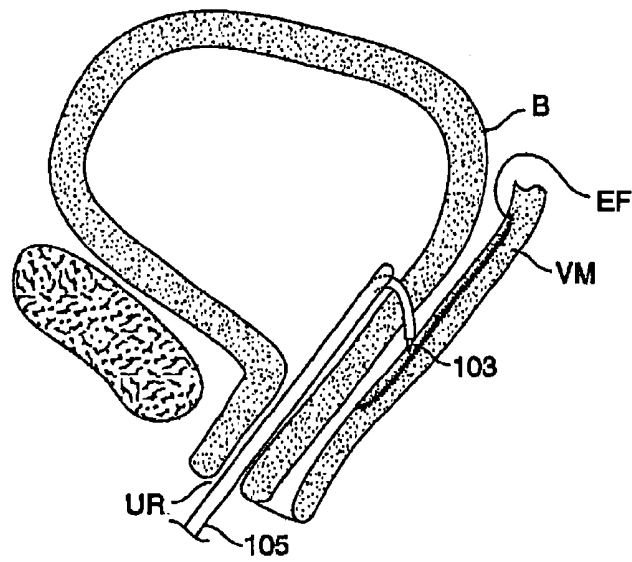


FIG. 15D

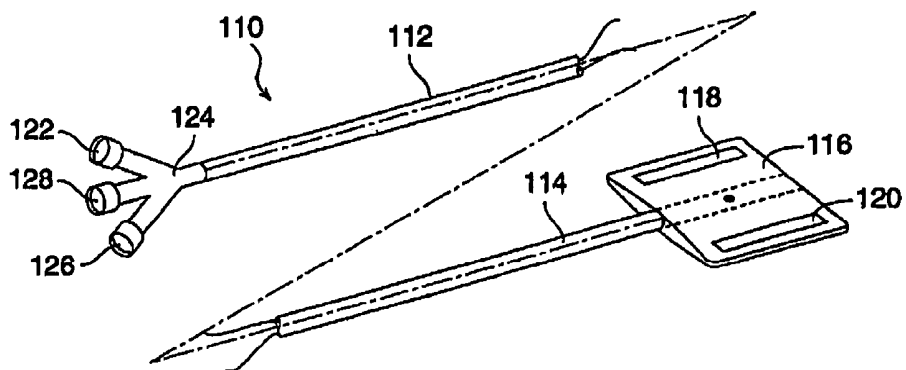


FIG. 16

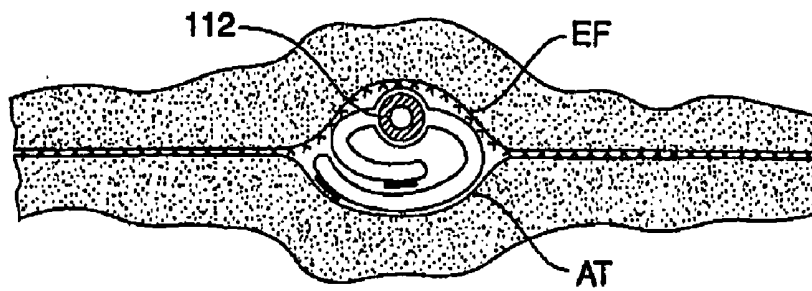


FIG. 17A

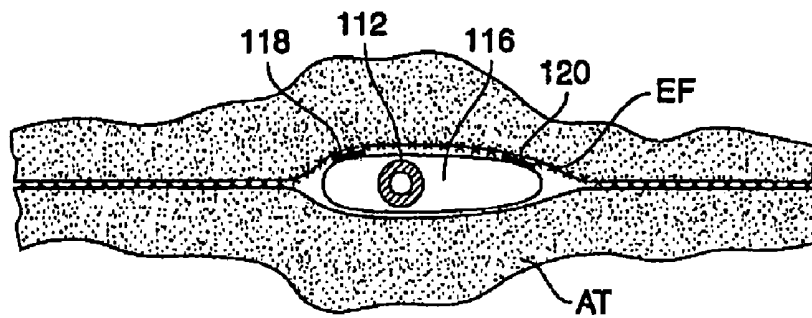


FIG. 17B




FIG. 18A

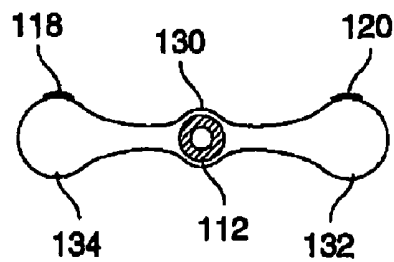


FIG. 18B

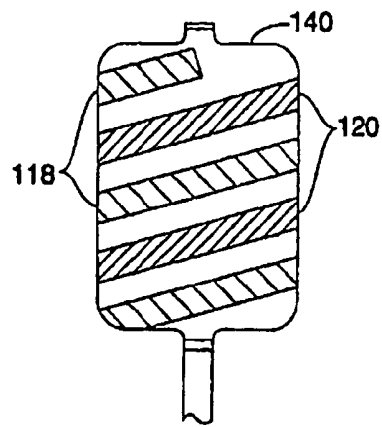


FIG. 19

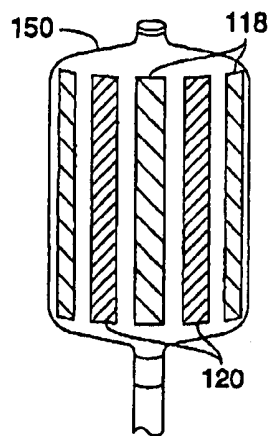


FIG. 20A




FIG. 20B

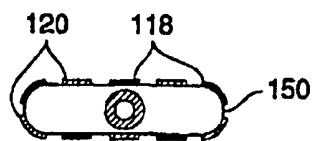


FIG. 20C

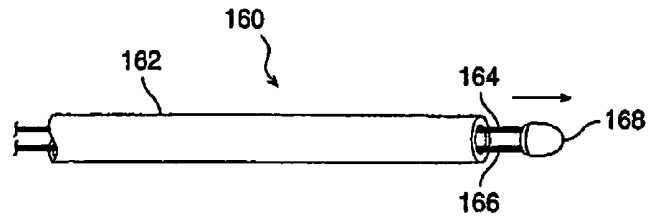


FIG. 21A

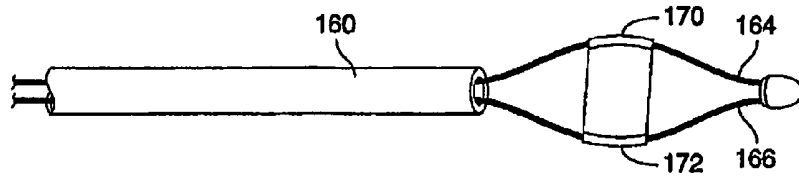


FIG. 21B



FIG. 22A



FIG. 22B

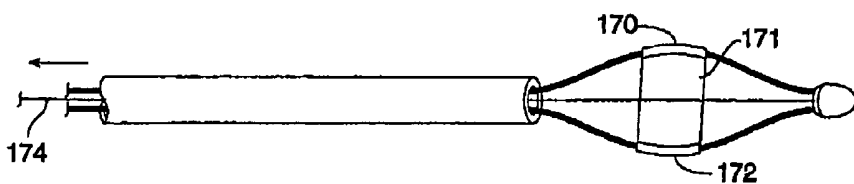


FIG. 22C

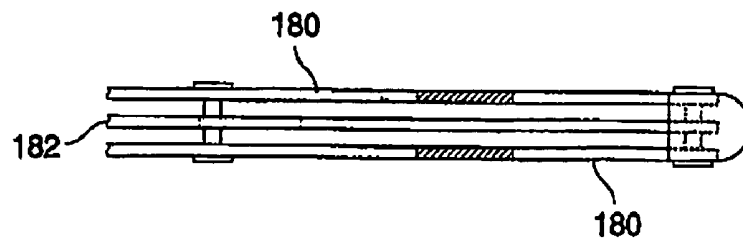


FIG. 23A




FIG. 23B

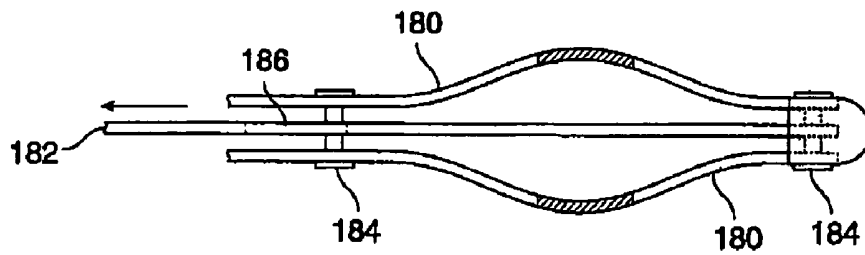


FIG. 23C

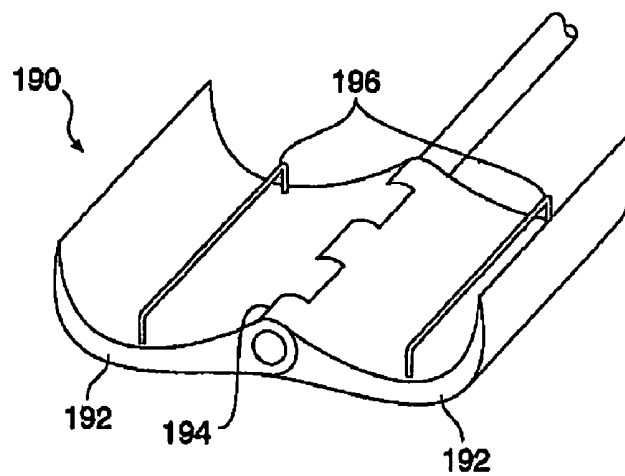


FIG. 24

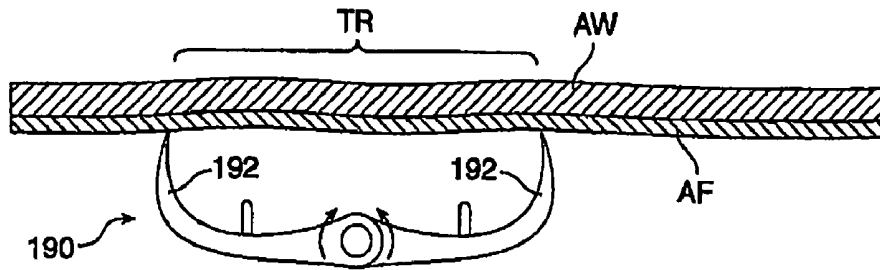


FIG. 25A

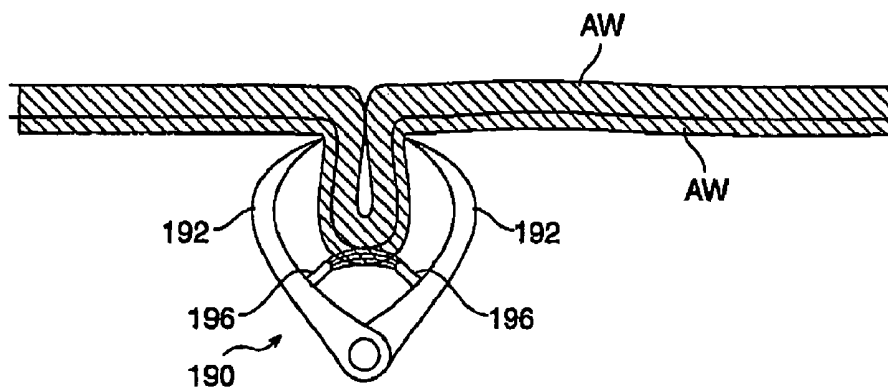


FIG. 25B

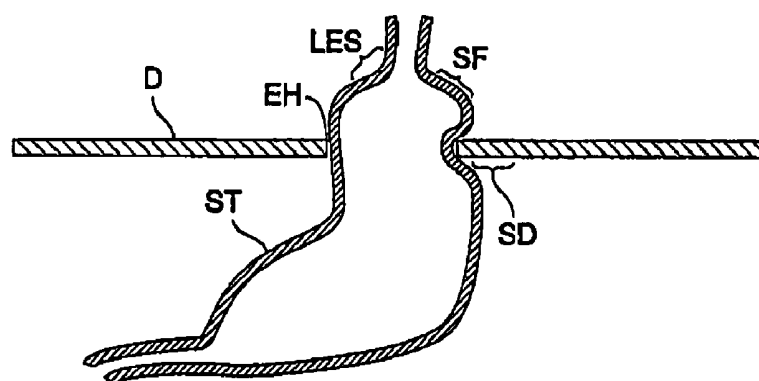


FIG. 26

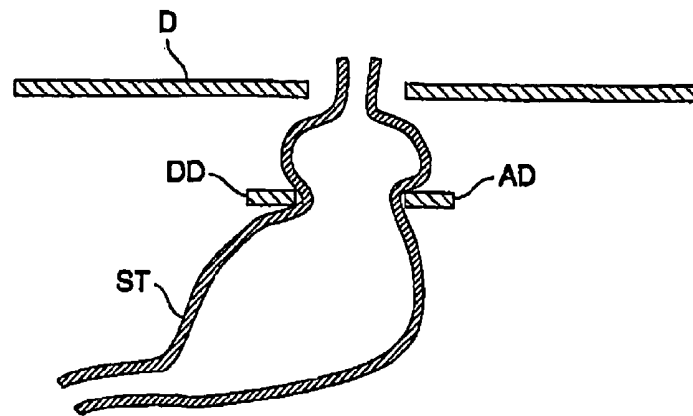


FIG. 26A

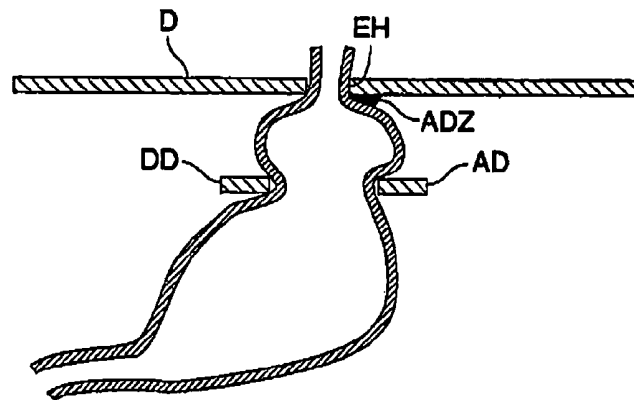


FIG. 26B

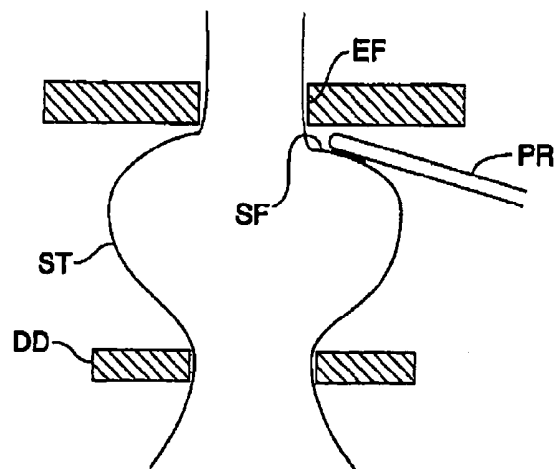


FIG. 26C

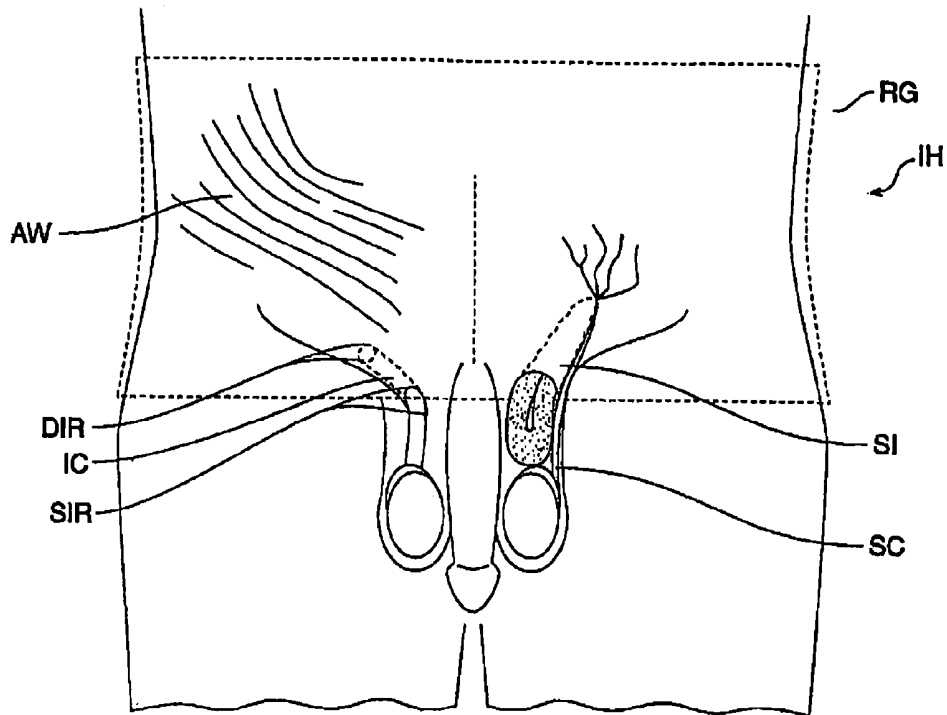


FIG. 27

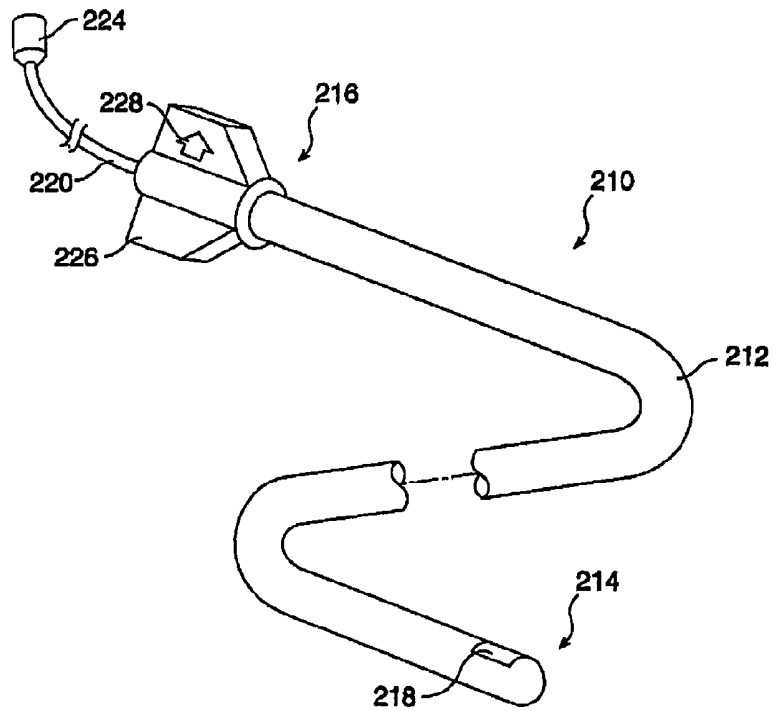


FIG. 28




FIG. 28A




FIG. 28B




FIG. 28C




FIG. 28D

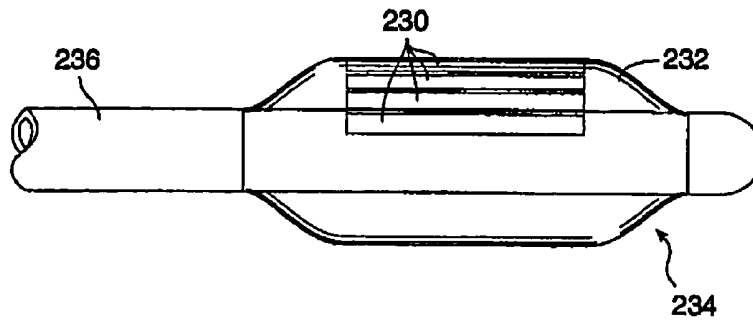


FIG. 29

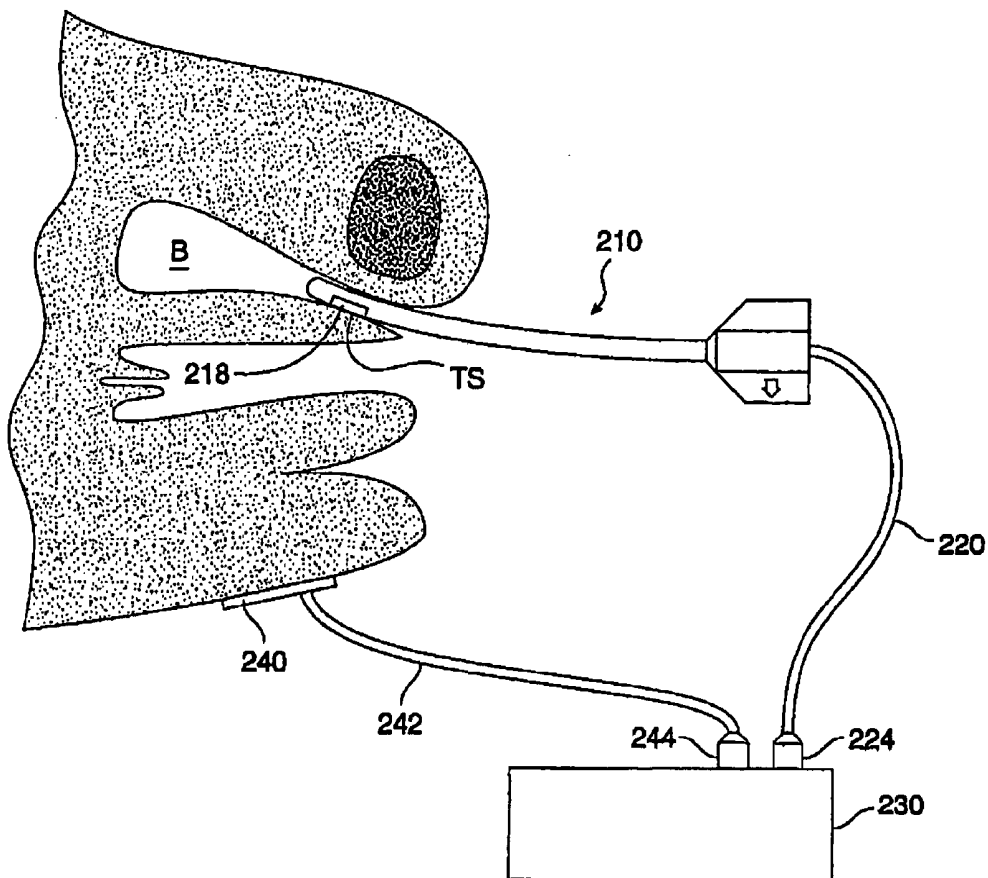


FIG. 30

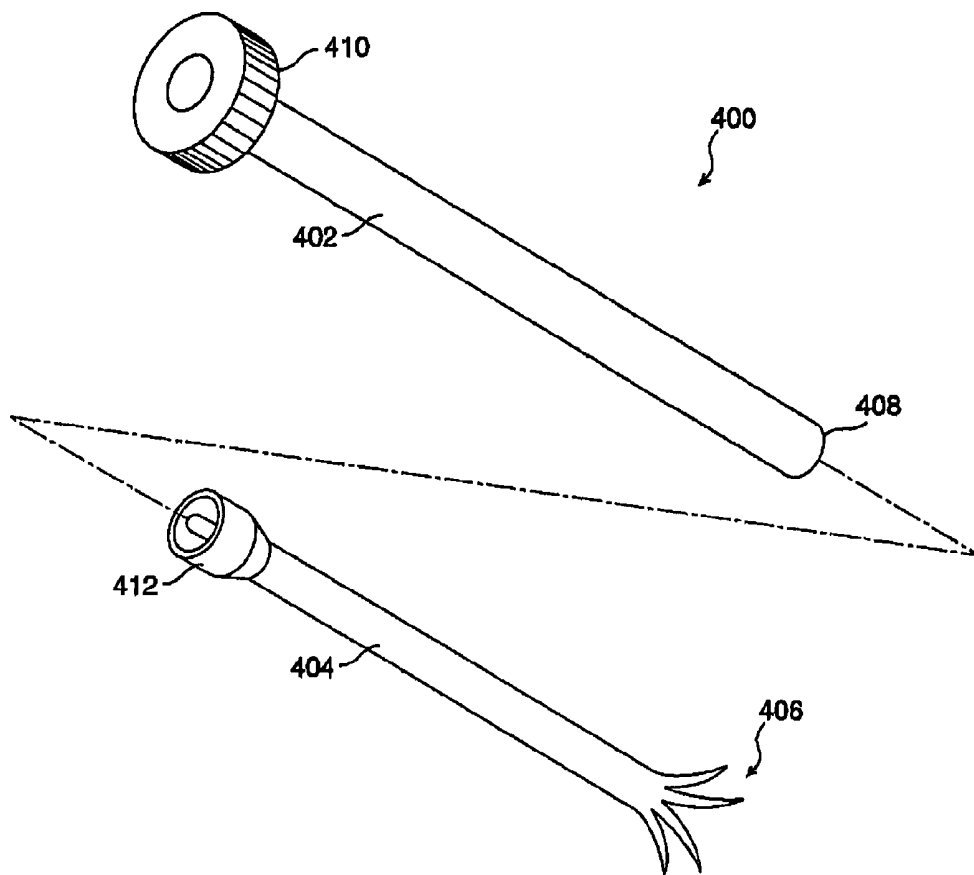


FIG. 31




FIG. 32

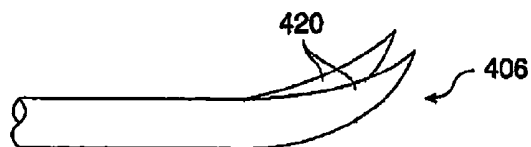


FIG. 33

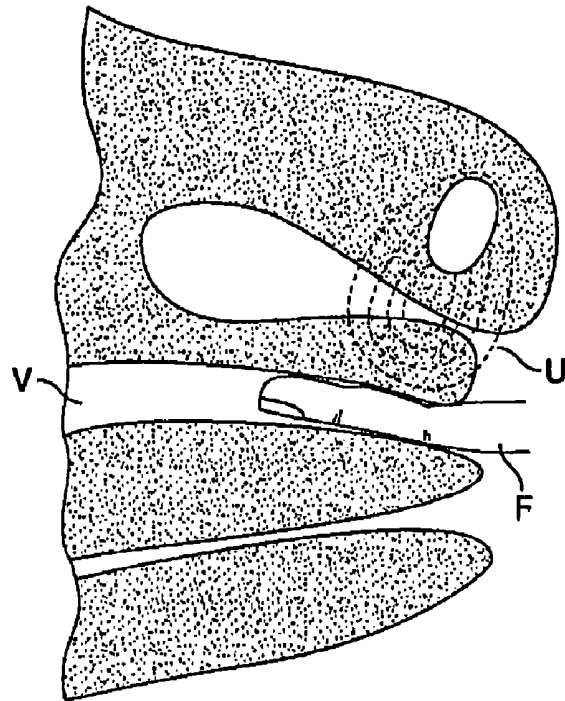


FIG. 34

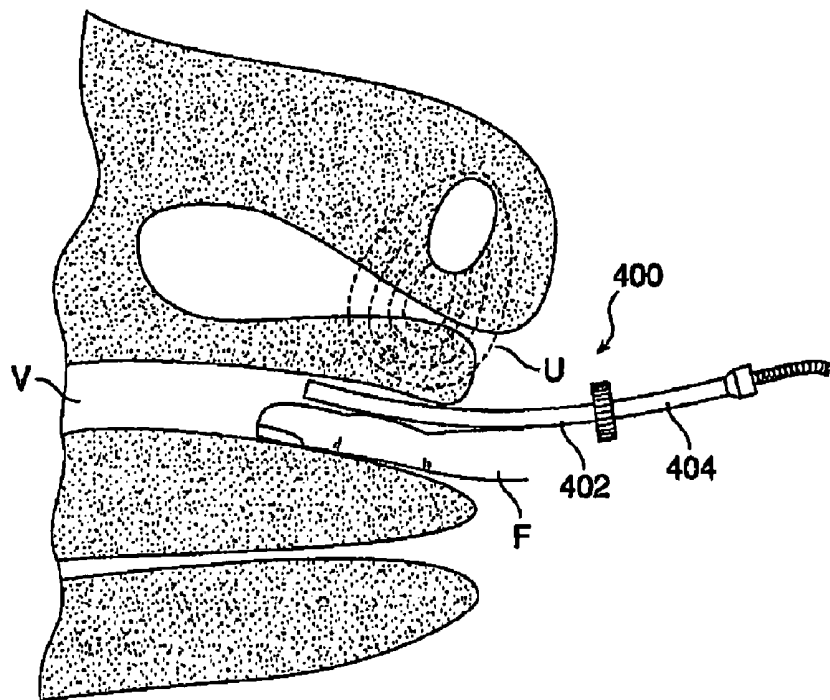


FIG. 35

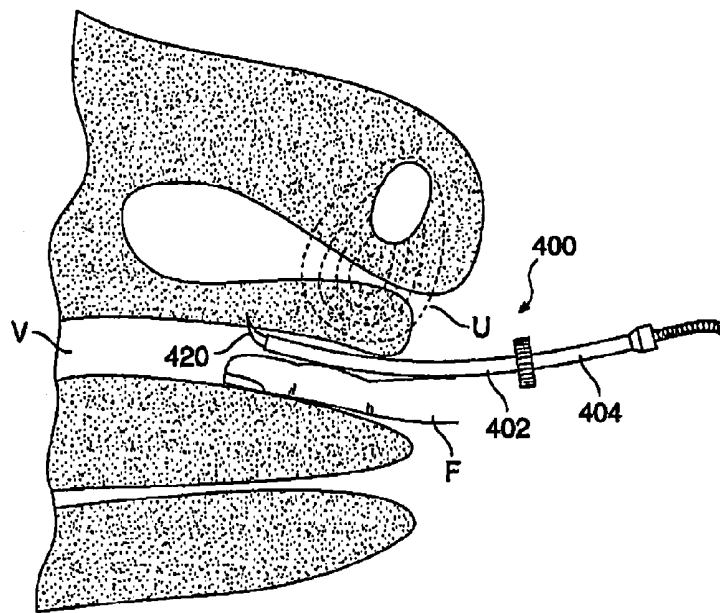


FIG. 36

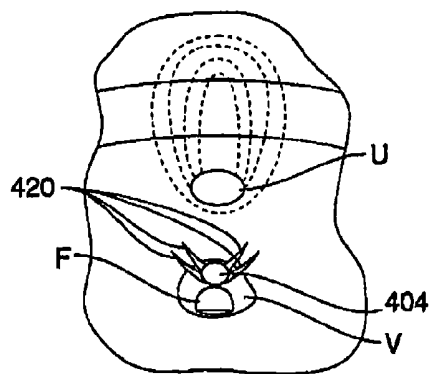


FIG. 37

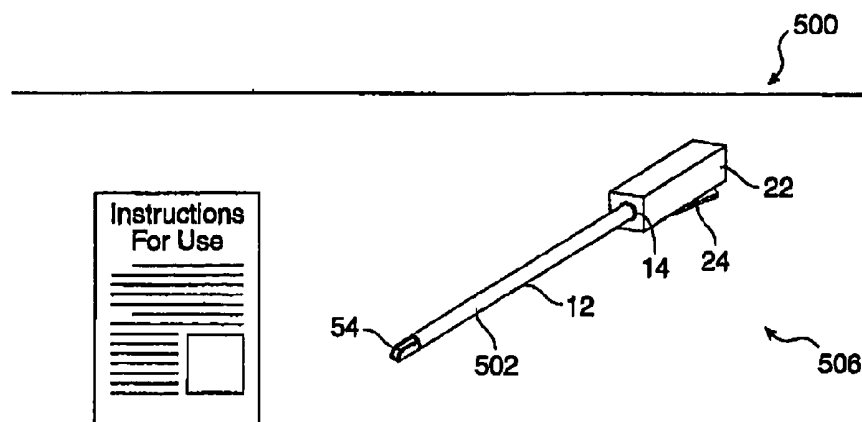


FIG. 38

DEVICES, METHODS, AND SYSTEMS FOR SHRINKING TISSUES

CROSS-REFERENCES TO RELATED APPLICATIONS

This application is a continuation application which claims priority from U.S. patent application Ser. No. 09/441,109 filed Nov. 16, 1999, now U.S. Pat. No. 6,772,013, which is a divisional of U.S. patent application Ser. No. 08/910,370 filed Aug. 13, 1997, now U.S. Pat. No. 6,091,995; which is a continuation-in-part of U.S. patent application Ser. No. 08/862,875, filed May 23, 1997, now abandoned; which is a non-provisional U.S. patent application Ser. No. 08/748,527, filed Nov. 8, 1996, now abandoned; the full disclosures of which are incorporated herein by reference.

This application is related to U.S. patent applications Ser. No. 08/910,775 filed Aug. 13, 1997; Ser. No. 08/910,369 filed Aug. 13, 1997; and Ser. No. 08/910,371 filed Aug. 13, 1997; the full disclosures of which are also incorporated herein by reference.

BACKGROUND OF THE INVENTION

1. Field of the Invention

The present invention generally relates to medical devices, methods, and systems. In a particular aspect, the present invention provides devices, methods, and systems for shrinking tissues, and which are particularly useful for treatment of urinary incontinence in a laparoscopic or minimally invasive manner.

Urinary incontinence arises in both women and men with varying degrees of severity, and from different causes. In men, the condition occurs almost exclusively as a result of prostatectomies which result in mechanical damage to the sphincter. In women, the condition typically arises after pregnancy where musculoskeletal damage has occurred as a result of inelastic stretching of the structures which support the genitourinary tract. Specifically, pregnancy can result in inelastic stretching of the pelvic floor, the external vaginal sphincter, and most often, the tissue structures which support the bladder and bladder neck region. In each of these cases, urinary leakage typically occurs when a patient's intra-abdominal pressure increases as a result of stress, e.g. coughing, sneezing, laughing, exercise, or the like.

Treatment of urinary incontinence can take a variety of forms. Most simply, the patient can wear absorptive devices or clothing, which is often sufficient for minor leakage events. Alternatively or additionally, patients may undertake exercises intended to strengthen the muscles in the pelvic region, or may attempt behavior modification intended to reduce the incidence of urinary leakage.

In cases where such non-interventional approaches are inadequate or unacceptable, the patient may undergo surgery to correct the problem. A variety of procedures have been developed to correct urinary incontinence in women. Several of these procedures are specifically intended to support the bladder neck region. For example, sutures, straps, or other artificial structures are often looped around the bladder neck and affixed to the pelvis, the endopelvic fascia, the ligaments which support the bladder, or the like. Other procedures involve surgical injections of bulking agents, inflatable balloons, or other elements to mechanically support the bladder neck.

Each of these procedures has associated shortcomings. Surgical operations which involve suturing of the tissue structures supporting the urethra or bladder neck region require

great skill and care to achieve the proper level of artificial support. In other words, it is necessary to occlude the urethra or support the tissues sufficiently to inhibit urinary leakage, but not so much that normal intentional voiding of urine is made difficult or impossible. Balloons and other bulking agents which have been inserted can migrate or be absorbed by the body. The presence of such inserts can also be a source of urinary tract infections.

For these reasons, it would be desirable to provide improved devices, methods, and systems for treating fascia, tendons, and other support tissues which have been strained, or which are otherwise too long to provide the desired support. It would be especially desirable to provide improved methods for treating urinary incontinence in men and women. In particular, it would be desirable to provide methods for treating urinary incontinence in a minimally invasive manner with few or no percutaneous tissue penetrations, preferably utilizing laparoscopic or least invasive manner to minimize patient trauma. It would further be desirable to provide incontinence treatment methods which rely on the existing bladder support structures of the body, rather than depending on the specific length of an artificial support. It would also be desirable to provide methods which rely on introduction of a relatively simple probe into the urethra or vaginal, where tissue structures supporting or comprising the urethra may be caused to partially shrink in order to inhibit urinary leakage.

2. Description of the Background Art

Method and apparatus for controlled contraction of soft tissue are described in U.S. Pat. Nos. 5,569,242, and 5,458,596. An RF apparatus for controlled depth ablation of soft tissue is described in U.S. Pat. No. 5,514,130.

A bipolar electrosurgical scalpel with paired loop electrodes is described in U.S. Pat. No. 5,282,799. U.S. Pat. No. 5,201,732 describes a bipolar sphincterotomy utilizing side-by-side parallel wires. A disposable electrosurgical instrument is described in U.S. Pat. No. 4,311,145. U.S. Pat. No. 5,496,312, describes an impedance and temperature generator control.

The following patents and published applications relate to the treatment of urinary incontinence. U.S. Pat. Nos. 5,437,603; 5,411,475; 5,376,064; 5,314,465; 5,304,123; 5,256,133; 5,234,409; 5,140,999; 5,012,822; 4,994,019; 4,832,680; 4,802,479; 4,773,393; 4,686,962; 4,453,536; 3,939,821; 3,926,175; 3,924,631; 3,575,158; 3,749,098; and WO 93/07815.

An electrosurgical probe for the controlled contraction of tissues of the joints and for dermatological indicators is described in U.S. Pat. No. 5,458,596. A bipolar electrosurgical probe having electrodes formed over a restricted arc of its distal end for treatment of, e.g., the esophagus, is described in U.S. Pat. No. 4,765,331. An electrosurgical probe for retrograde sphincterotomy is described in U.S. Pat. No. 5,035,696. Other patents describing electrosurgical probes include U.S. Pat. No. 5,462,545; 5,454,809; 5,447,529; 5,437,664; 5,431,649; 5,405,346; 5,403,312; 5,385,544; 5,370,678; 5,370,677; 5,370,675; 5,366,490; 5,314,446; 5,309,910; 5,293,869; 5,281,218; 5,281,217; 5,190,517; 5,098,429; 5,057,106; 4,807,620; 4,776,344; 4,409,453; and 373,399.

The disclosure of the present application is related to co-pending U.S. patent application Ser. No. 08/610,911, filed on Mar. 5, 1996, having a common inventor but assigned to a different entity.

SUMMARY OF THE INVENTION

The present invention provides improved devices, methods, and systems for shrinking collagenated tissues, and par-

ticularly for treating urinary incontinence. In contrast to prior art methods, the present invention does not rely on implantation of balloons or other materials, nor does it rely on suturing, cutting, or other direct surgical modifications to the genitourinary support tissues. Instead, the present invention relies on delivering energy to a patient's own pelvic support tissue to selectively contract or shrink at least a portion of that pelvic support tissue, thereby raising the position of the bladder. The energy will preferably be applied across bipolar electrodes to the endopelvic fascia and/or the arcus tendineus fascia pelvis. A variety of devices and methods are provided for applying gentle resistive heating to these tissues without significant injury to the support tissues, or to the surrounding tissue structures.

In a first aspect, the present invention provides a probe for heating and contracting fascia. The probe comprises a shaft having a proximal end and a distal end. First and second electrodes are disposed near the distal end of the shaft. These electrodes are simultaneously engageable against the fascia, and are separated by a predetermined distance which limits a depth of tissue heating. A handle is adjacent to the proximal end of the shaft for manipulating the electrodes from outside the patient body.

The bipolar probes of the present invention will generally include a predetermined electrode diameter and electrode separation distance to limit the depth of tissue heating, and will optionally have a temperature sensor mounted between the electrodes. The probe will often be adapted to heat the fascia to temperatures significantly less than most known electrosurgical devices, and may include a control system which limits the total electrical potential applied between the bipolar electrodes to much lower average power levels than known electrosurgical devices. In fact, the present heating probe may be conveniently energized with a battery pack carried in the proximal handle of the probe.

In another aspect, the present invention provides a least invasive probe for heating and contracting fascia of a patient body. The fascia is adjacent to a tissue layer, and the probe comprises a shaft having proximal and distal ends. An electrode is disposed near the distal end of the shaft and is laterally deployable from a narrow configuration to a wide configuration between the fascia and the adjacent tissue layer. The electrode in the wide configuration is exposed to engage the fascia. The electrode in the narrow configuration is disposed along an axis of the shaft to facilitate axial insertion of the probe. A handle is adjacent the proximal end of the shaft for manipulating the electrode from outside the patient body.

In yet another aspect, the present invention provides a probe for heating and contracting target tissues. The probe comprises a shaft having a proximal end and a distal end. At least one electrode is disposed near the distal end of the shaft. A handle is disposed adjacent the proximal end of the shaft for manipulating the at least one electrode from outside the patient body. The handle supports a battery and circuitry for energizing the at least one electrode with sufficient RF electrical potential to heat and contract the target tissue.

Circuitry for converting a direct current to an alternating current will often be coupled to the battery to provide heating while avoiding nerve and/or muscle stimulation. In many embodiments, a control system will be coupled to the electrode so that the target tissue is raised to a temperature within a predetermined range. The temperature of the target tissue may be determined by a tissue temperature sensor disposed near the electrode (ideally being disposed between bipolar electrodes) and/or by monitoring the impedance, resistance, or other electrical characteristics of the tissue/electrode circuit.

In another embodiment, the present invention provides a probe for shrinking collagenated tissue of a patient body. The probe comprises a shaft having a proximal end and a distal end. A grasper is disposed near the distal end of the shaft, and is adapted to draw a region of the tissue inward so as to reduce tension within the region. An energy applying member is disposed adjacent to the grasper. The energy applying member is capable of heating the tissue while the tension is reduced so that the tissue contracts, but without substantially ablating the tissue.

The present invention also provides a method to treat a hyperextending support tissue of a patient body. The hyperextending tissue has a tissue depth, and the method comprises electrically coupling the first electrode to the hyperextending tissue. A second electrode is also electrically coupled to the hyperextending tissue, and an electrical potential is applied across the electrodes while controlling a separation between the first and second electrodes. As a result of this separation control, an electrical current within the hyperextending tissue heats and shrinks the hyperextending tissue, but heating of tissue beyond the tissue depth is minimized.

The present invention also provides a method to treat urinary stress incontinence. The method comprises introducing a probe into a patient body and aligning the probe with a pelvic support tissue within the patient body. The probe is energized to heat and contract a portion of the pelvic support tissue.

In most embodiments, a portion of the pelvic support tissue is gently and resistively heated to between about 60° C. and 110° C., often being between about 60° C. and 80° C., by applying an electrical potential across the electrodes, the electrodes being adapted to engage the fascia surface. This gentle bipolar resistive heating will often be targeted at fascia. Such contraction of the fascia can raise and/or reposition the bladder within the patient body when the fascia is heated to a depth of less than about 2.8 mm, preferably to a depth of less than about 2.0 mm, thereby minimizing collateral injury to the surrounding tissues. The heating depth can be precisely limited by controlling the diameter of the electrode surfaces (electrode surface diameter typically in the range from about 0.25 mm to about 4.0 mm, often being from about 0.25 mm to about 2.0 mm) and the ratio of the spacing between the electrodes to the electrode surface diameter (the spacing typically being between about 1.0 and 4.0 times the surface diameter). Advantageously, a preferred separation distance of between about 2 and 3 times the electrode surface diameters will provide an effective heating depth of about 2 times the electrode surface diameter. Surprisingly, sufficient RF energy for such targeted heating can be provided by a battery pack within a handle of the probe, the battery typically providing between about 5 and 20 watts.

In a second aspect, the present invention provides an endoscopic method for treating urinary stress incontinence. The method comprises introducing a probe into a patient body, and optically imaging the probe and a target tissue. The target tissue comprises a portion of an endopelvic fascia or an arcus tendineus fascia pelvis. The electrode is positioned against the target tissue, and energized to heat and contract the target tissue, without substantially ablating the target tissue.

Once again, heating will often be limited in depth through the use of a bipolar probe having a predetermined electrode diameter, spacing between the electrodes, and power. Heating can be monitored and/or controlled, optionally using feedback from a temperature sensor mounted between the electrodes. Advantageously, repeatedly sweeping the electrodes

across the endopelvic fascia can raise the bladder by discrete increments, typically by between about 0.1 and 3.0 mm with each sweep of the electrodes.

In another aspect, the present invention provides a least invasive method for controllably shrinking fascia. The method comprises inserting a probe into a patient body while the probe is in a narrow configuration. The probe has first and second electrodes, and is expanded to a wider configuration to deploy at least one of the first and second electrodes. The deployed electrodes are engaged against the fascia, and an electrical potential is applied across the electrodes to heat and contract the fascia disposed therebetween.

In yet another aspect, the present invention provides a method for treating a hernia. The hernia comprises a structure which protrudes through a containing tissue. The method comprises applying sufficient energy to the containing tissue adjacent the hernia to heat the containing tissue so that the containing tissue contracts. The contraction mitigates the hernia, but the heat does not substantially ablate the containing tissue.

In another aspect, the invention provides an abdominoplasty method for tightening an abdominal wall. The abdominal wall comprises a fascia, and the method comprises applying sufficient energy to the abdominal wall to heat the fascia so that the abdominal wall contracts. The heat is applied without substantially ablating the abdominal wall and adjacent tissues.

In yet another aspect, the invention provides a method to treat a hyperextending collagenated support tissue of a patient body. The method comprises grasping a region of the hyperextending tissue and drawing the hyperextending tissue inward so as to decrease tension in the region. At least a portion of the drawn region is heated so that the region shrinks, wherein the region is heated without substantially ablating the hyperextending tissue.

In yet another aspect, the invention provides a kit for shrinking a target collagenated tissue within a patient body. The target tissue has a tissue depth, and the kit comprises a probe and instructions for operating the probe. The probe includes a shaft having a proximal end and a distal end. First and second electrodes are disposed near the distal end of the shaft, the electrodes defining a separation distance therebetween. The instructions include the steps of electrically coupling the first and second electrodes with the target tissue, and heating and contracting the target tissue without ablating the target tissue by directing an electrical current flux through the target tissue between the electrodes. The separation distance substantially limits heating beyond the target tissue depth.

In yet another aspect, the invention provides a kit for treating urinary stress incontinence of a patient with a lax pelvic support structure. The kit comprises a probe having a heating element and instructions for operating the probe. Instructions include the steps of coupling the heating element to the pelvic support structure, and applying an amount of energy with the heating element to the pelvic support structure. The energy is sufficient to cause shrinkage of the pelvic support structure, and the shrinkage inhibits urinary incontinence.

In yet another aspect, the invention provides a kit for treating a hernia. The hernia comprises a structure which protrudes through a collagenated containing tissue. The kit comprises a probe having a heating element and instructions for operating the probe. The instructions include the steps of coupling the probe to the containing tissue, and applying an amount of energy from the probe to the containing tissue. The energy is sufficient to heat the containing tissue so that the containing tissue shrinks to mitigate the hernia.

In one exemplary embodiment of the present method, energy is applied from within the patient's urethra, typically by inserting an energy-applying probe into the urethra without having to employ any percutaneous or transmucosal penetrations or incisions. When using such a urethral probe, the energy will typically be applied directly to the urethral wall, either to a single location aligned with the urethral sling or to at least two sites including a first site upstream of the urethral sling and a second site downstream of the urethral sling. By "urethral sling," we mean those supporting tendons and other tissue structures which extend from the pubic bone downward beneath the urethra and urethral sphincter. Application of energy at such location(s) acts to shrink tissue adjacent the urethral lumen and to provide selective "kinks" or closure points at which the urethra can be closed.

In an alternative exemplary embodiment, energy-applying elements are penetrated directly into the pubococcygeal muscles, the iliococcygeal muscles, and/or detrusor urinae muscles (and adjacent fascia) which support the urethra and urinary sphincter. By applying energy directly into these supporting muscles and tissue structures, the muscles can be contracted to provide improved urinary continence. In particular, sufficient muscular integrity can be provided so that urinary leakage does not result from transient increases in intra-abdominal pressure as a result of stress. In the illustrated embodiment, the electrodes are penetrated into the target muscles through the vagina, typically using an introducer having an array of extensible electrodes arranged to contact the target muscles and/or tendons.

In these exemplary embodiments, the energy will typically be applied using an electrode capable of delivering radio frequency (RF) energy directly against the urethral wall or into the supporting tissues in a monopolar or bipolar manner. In the first embodiment, electrodes will usually be surface electrodes, i.e., adapted to contact the luminal wall of the urethra without penetration. In the second embodiment, the electrodes are fashioned as needles or other penetrating members which can penetrate into the urethral wall by a desired distance. In addition to electrodes, the heat-applying elements can be optical fibers (for delivery laser or other light energy), resistive heating elements, inductive heating elements, microwave heating elements, or any other device which can be externally powered to heat tissue to the temperatures and for the times discussed below.

The methods of the present invention may also be performed using devices and systems which access the treated tissue structures from sites other than the urethra or vagina. For example, energy-applying probes can be introduced percutaneously from the patient's abdomen to a desired treatment site, for example the pubococcygeal muscle and tendon, or may alternatively be introduced through the rectum. Alternatively, in female patients, the energy-applying probes can be transmucosally introduced through the vagina, as discussed above. For the purposes of the present invention, it is necessary only that the energy be delivered to a target tissue structure in a manner which permits heating of the tissue to a desired temperature and for time sufficient to contract the tissue by a desired amount.

In addition to RF energy, the devices, systems, and methods of the present invention can rely on other energy sources, such as microwave, light (laser) energy, electrical resistance heating, the delivery of heated fluids, the focusing of ultrasound energy, or any other known energy delivery technique which can be targeted to specific tissue and raise the tissue temperature to the desired range.

When energy is applied directly to the luminal wall, it will be desirable to control the resulting cross-sectional area of the

urethra. Usually, the cross-sectional area will be reduced. Control of the amount of reduction can be effected, for example, by placing the energy-applying elements, such as RF electrodes, on an expandable member which can initially be expanded to contact the elements against the luminal wall. As the luminal wall shrinks, the cross-section area of the expandable member can also be reduced. Alternatively, in instances where the energy is being applied to contract adjacent tissue structures, it may be necessary to further expand the expandable member carrying the electrodes to maintain contact. A variety of specific configurations can be utilized.

In some embodiments, devices according to the present invention will comprise a probe body having a proximal end and a distal end. The body will preferably have a length and diameter selected to permit introduction into the urethra or vagina so that the distal end can be positioned adjacent to the urethral sling or target tissues. One or more electrodes are disposed on the distal end of the probe body to apply energy into the urethral wall in the region of the urethral sling and/or into the tissue structures which support the urethral sling. A connector is provided on the proximal end of the probe body to permit connection to an appropriate power supply. The probe body will typically have a length in the range from 5 cm to 20 cm with electrode lengths in the range from 0.3 cm to 7 cm. The probe body will usually have a diameter in the range from 1 mm to 6 mm. The body will usually be flexible, but could also be rigid. The body should have sufficient torsional rigidity to permit rotational orientation and alignment of the probe within the urethra. The probe will include at least a single electrode, and will often include two or more electrodes which can be connected to the power supply in a monopolar or a bipolar fashion. The electrodes may be surface electrodes (for engaging the urethra wall) or tissue-penetrating electrodes for applying energy into the urethra-supporting tissues. In a specific embodiment, the probe will include two axially-spaced apart electrodes which are positioned and configured so that they will be aligned on the upstream and downstream sides of the urethral sling when applying energy within the urethra. The probe may further comprise an expansion member, such as an expandable balloon, carrying at least one of the electrodes on the catheter body. In a second specific embodiment, the probe includes an array of extensible, tissue-penetration electrodes disposed to penetrate target tissues from the vagina.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a perspective view of a bipolar battery operated probe for laparoscopically heating and contracting fascia, according to the principles of the present invention.

FIG. 2 is a schematic of the functional components of the probe of FIG. 1.

FIG. 3 is a lateral cross-sectional view showing the urinary bladder and bladder support structures.

FIG. 4 is a simplified cross-sectional view of the pelvis showing the endopelvic fascia and arcus tendineus fascia pelvis, and illustrates a method for treating urinary stress incontinence by sweeping the probe of FIG. 1 across the endopelvic fascia to reposition and/or raise the urinary bladder.

FIG. 5 is a cross-sectional view of a patient suffering from urinary stress incontinence due to inelastic stretching of the endopelvic fascia.

FIG. 6 shows a known method for treating urinary stress incontinence by affixing sutures around the bladder neck.

FIG. 7 illustrates improved bladder support provided by selectively contracting the endopelvic fascia as a therapy for urinary stress incontinence, according to the principles of the present invention.

FIG. 7A illustrates a patient suffering from a cystocele in which the bladder protrudes into the vagina, and which may be treated by selectively contracting the pelvic support tissues using the methods of the present invention.

FIG. 8 illustrates how the controlled spacing between the bipolar electrodes of the probe of FIG. 1, relative to the electrode diameter, limits the depth of tissue heating.

FIG. 9 schematically illustrates repeatedly sweeping the bipolar electrodes of the probe of FIG. 1 across the endopelvic fascia to raise the urinary bladder in a series of discrete increments.

FIGS. 10–12D illustrate alternative electrode configurations for use with the probe of FIG. 1.

FIGS. 13A and 13B illustrate bipolar electrodes which move relative to each other when tissue contracts to provide feedback and/or limit tissue heating, according the principle of the present invention.

FIG. 13C illustrates an electrode structure that varies the heating depth with the rotational position of the probe about the axis of the probe.

FIG. 14 illustrates a bipolar fascia contracting probe having roller electrodes to facilitate sweeping the probe over the fascia.

FIG. 15 illustrates a joystick actuated least invasive probe for penetrating through the vaginal mucosa to the mucosa/fascia interface, the endopelvic fascia surface, or the vesicle-vaginal space, the probe having an asymmetric handle to indicate the electrode orientation, according the principles of the present invention.

FIGS. 15A–15D illustrate least invasive methods for accessing the endopelvic fascia through the vaginal mucosa or the bladder wall.

FIG. 16 illustrates an asymmetric least invasive probe having bipolar electrodes which are deployable by inflating a balloon.

FIGS. 17A and 17B schematically illustrate self-orientation of the inflatable electrode assembly of the probe of FIG. 16.

FIGS. 18A and 18B schematically illustrate the deployment of bipolar electrodes by inflating an asymmetric flat balloon with two different inflation media to radiographically verify the orientation of the electrodes.

FIG. 19 illustrates the deployed state of an alternative balloon deployable electrode configuration for use with the least invasive probe of FIG. 15.

FIGS. 20A–20C schematically illustrate the deployed state of a balloon having alternating electrodes, and a method for its use to separate a fascia targeted for contraction from an adjacent tissue surface, after which the balloon is partially deflated for heating and contracting the fascia.

FIGS. 21A and 21B schematically illustrate bipolar electrodes which are supported along resilient elongate structures, in which the elongate structures are biased to separate the electrodes, for use with the least invasive probe of FIG. 15.

FIGS. 22A–22C schematically illustrate an alternative electrode deployment structure in which a pull-wire deflects elongate structures to deploy the electrodes.

FIGS. 23A–23C schematically illustrate an electrode deployment structure in which a central member is tensioned to deflect the electrode support structures resiliently outwardly.

FIG. 24 is a perspective view of an alternative probe for shrinking endopelvic fascia and other collagenated tissues, in

which the probe includes a grasper which reduces tension in the region of tissue to be contracted to enhance shrinkage.

FIGS. 25A and 25B schematically illustrate a method for using the probe of FIG. 24 by grasping the target tissue and drawing a region of the target tissue inward to reduce tension in the engaged tissue, and thereby enhance shrinkage.

FIGS. 26–26C are cross-sectional views of a patient suffering from a hiatal hernia showing a method for treatment using the probes of the present invention.

FIG. 27 illustrates a patient suffering from an inguinal hernia, and identifies regions for treating the inguinal hernia using the methods of the present invention.

FIG. 28 is a perspective view of an exemplary electrosurgical probe constructed in accordance with the principles of the present invention.

FIGS. 28A–28D illustrate alternative electrode configurations for the probe of FIG. 28.

FIG. 29 illustrates a distal probe tip having an expandable balloon carrying an electrode array.

FIG. 30 illustrates a system comprising the probe of FIG. 28 and a power supply performing a procedure in a patient's urethra.

FIG. 31 illustrates a second exemplary electrosurgical probe constructed in accordance with the principles of the present invention.

FIG. 32 is a detailed distal end view of the probe of FIG. 31.

FIG. 33 is a detailed distal side view of the probe of FIG. 31.

FIGS. 34–37 illustrate the use of the probe of FIGS. 31–33 in performing a procedure in a patient's vagina.

FIG. 38 schematically illustrates a kit including a laparoscopic tissue contraction probe, packaged together with pointed instructions for its use to contract tissue as a treatment for urinary incontinence.

DESCRIPTION OF THE SPECIFIC EMBODIMENTS

The present invention generally provides devices, methods, and systems which can selectively shrink fascia and other collagenated tissues. By directing an electrical current flux through such a tissue, ideally between bipolar electrodes directly engaging the tissue, the electrical resistance of the tissue can induce gentle heating and contraction of the tissue without significant injury to the adjacent tissues. Controlling a diameter of the electrode surfaces and a ratio of the surface diameter to a separation distance between the electrodes can limit the depth of heating, while electrode surface shape and size will help determine heating at the electrode/tissue interface. The present invention is particularly well adapted for contraction of fascia and ligaments, and may therefore have applications in a variety of therapies, including traditional and minimally invasive therapies of the pelvis, thorax, and joints. These devices, methods, and systems are adaptable for therapies of specific tissues and conditions including hiatal hernias, abdominal hernias, cystocele, enterocele, rectocele, and uterovaginal prolapse. The present invention will find its most immediate application for the treatment of urinary stress incontinence. In many embodiments, the present invention will effect contraction of a pelvic support tissue to raise a position of the bladder, particularly after the pelvic support tissues have been stressed by pregnancy. Related devices and methods are described in co-pending U.S. patent application Ser. No. 08/910,775 filed on Aug. 13, 1999, the full disclosure of which is incorporated herein by reference.

In general, the present invention is well adapted for treatment of any hyperextending collagenated tissue. As used

herein, the term “hyperextending” encompasses any tissue structure which is excessive in at least one dimension, so that a support function of the tissue is compromised. This excessive length, etc., may be the result of injury, pregnancy, disease, age, a congenital defect, a tear or partial tear, or the like.

Referring now to FIG. 1, a tissue contraction probe 10 includes a shaft 12 having a proximal end 14 and a distal end 16. First and second electrodes 18, 20 are disposed near distal end 16 of shaft 12, while a handle 22 is disposed at the proximal end of the shaft. A switch 24 applies a radiofrequency electrical potential across first and second electrodes 18, 20 to effect gentle resistive heating of electrically conductive tissues which span these electrodes. Surprisingly, power requirements of this targeted bipolar resistive heating are so low that a battery pack contained within handle 22 can sufficiently energize first and second electrodes 18, 20.

As can be understood with reference to FIG. 2, a battery pack 26 energizes probe 10, typically providing a relatively low power radio frequency current. The direct current of the battery is converted to the desired radio frequency by a DC to AC converter of a RF generator 28. The electrical potential applied to first and second electrodes 18, 20 will typically be between about 200 and 1,000 KHz, and will typically have an amplitude of between about 10 and 100 volts ac rms. Such low power heating will substantially avoid arcing between the electrode and the tissue surface, further decreasing the injury to these tissues, and also providing safety to the operator. The RF electrical heating will also desiccate the tissue, increasing its resistance. Since the applied voltage is too low to cause arcing, the delivered power will decrease as the tissue dries, so the tissue damage is superficial and self limiting. This makes treatment less subject to operator error.

A heating controller 30 will often limit at least one of the following: the temperature of the target tissue, the shrinkage of the tissue between the electrodes, and/or the time the target tissue is maintained at an elevated temperature. In some embodiments, tissue heating temperatures will be measured directly using a temperature sensor 32 mounted to the probe between the first and second electrodes 18, 20, or separately inserted into the tissue via an ultrasonically or fluoroscopically guided temperature probe. Alternatively, tissue temperature, contraction, and the like may be determined indirectly by monitoring the electrical characteristics of the tissue itself. In other words, by monitoring the circuit during heating, the tissue resistivity, resistance, capacitance, or the like, can be calculated. From these values, and optionally by monitoring the changes in these electrical characteristics, it may be possible to estimate the temperature or degree of desiccation of the tissue, the amount of shrinkage which has occurred, and the like. Preferably, controller 30 will limit the heating of tissues to a temperature range of between about 60° C. and 110° C., ideally to between about 60° C. and 80° C.

Alternatively, it may be possible to simply limit the electrical potential applied across the electrodes thereby permitting normal thermal conduction to control the maximum temperature. In fact, in some embodiments, a simple timer may be coupled to switch 24, so that a limited amount of energy is applied across first and second electrodes 18, 20, thereby avoiding over-treatment (particularly during spot treatments, as described hereinbelow). The physician simply energizes the time limited circuit after each movement of the electrodes, thereby avoiding unintended over-treatment, and also helping to ensure that sufficient energy is delivered for treatment of each site.

While the exemplary embodiment incorporates battery pack 26 and controller 30 into handle 22, it should be understood that the energizing and control functions may be pro-

vided by structures which are external to probe 10. In such embodiments, couplers for connecting electrodes 18 and 20 to a power source, control circuitry, and the like, will often be provided on housing 22. Battery pack 26 may optionally include two or more batteries. As used herein, a battery may be a single cell or a series of cells, where each cell is a substantially self-contained D.C. energy source.

The pelvic support tissues which generally maintain the position of the urinary bladder B are illustrated in FIG. 3. Of particular importance for the method of the present invention, endopelvic fascia EF defines a hammock-like structure which extends between the arcus tendineus fascia pelvis ATPF, as can be understood with reference to FIG. 4, these latter structures extend substantially between the anterior and posterior portions of the pelvis, so that the endopelvic fascia EF largely defines the pelvic floor.

In women with urinary stress incontinence due to bladder neck hypermobility, the bladder has typically dropped between about 1.0 and 1.5 cm (or more) below its nominal position. This condition is typically due to weakening of the pelvic support structures, including the endopelvic fascia, the arcus tendineus fascia pelvis, and the surrounding ligaments and muscles, often as the result of bearing children.

When a woman with urinary stress incontinence sneezes, coughs, laughs, or exercises, the abdominal pressure often increases momentarily. Such pressure pulses force the bladder to descend still further, shortening the urethra UR and momentarily opening the urinary sphincter.

As can be most clearly understood with reference to FIGS. 3-7, the present invention generally provides a therapy which applies gentle heating to shrink the length of the support tissues and return bladder B to its nominal position. Advantageously, the bladder is still supported by the fascia, muscles, ligaments, and tendons of the original pelvic support tissues. Using gentle resistive heating between bipolar electrodes, the endopelvic fascia EF and arcus tendineus fascia pelvis ATPF are controllably contracted to shrink them and re-elevate the bladder towards its original position.

Tissue contraction with probe 10 will generally be performed in at least one of two modes: spot treatments and line treatments. For example, by engaging the arcus tendineus fascia pelvis at a substantially fixed location with first and second electrodes 18, 20, a discrete portion along that substantially linear structure can be gently heated for a few seconds to the target temperature range. The tough fibrous tendon will then shorten, raising the endopelvic fascia EF which, in turn, raises the overall position of bladder B. Such contractions of a discrete region about a fixed engagement location are herein called spot treatments.

To provide a line treatment, the distal end of probe 10 is swept across endopelvic fascia EF laterally or linearly, as illustrated in FIG. 4. As the electrodes engage the adjacent endopelvic fascia, they raise the temperature of the adjacent tissues, resulting in a line of contracted tissues behind and between the electrode paths. Advantageously, this line of fascia contraction increases the overall tautness of the endopelvic fascia, again raising the overall position of bladder B. This is an example of the use of a single line treatment to effect repositioning of the bladder.

Advantageously, repeatedly sweeping probe 10 across adjacent areas of the endopelvic fascia can raise the bladder in discrete increments. For example, if first and second electrodes 18, 20 are separated by a space of about 3.0 mm, and if the fascia shrinks by about 50% with it each sweep of probe 10, the physician can re-elevate bladder B about 1.5 cm with between 10 and 15 line treatments of the endopelvic fascia.

Similar results may be provided by 10 to 15 spot treatments of the arcus tendineus fascia pelvis, or by some combination of spot and line treatments.

Access to and direction of the therapy, as schematically illustrated in FIG. 4, will often be provided by the minimally invasive methods and devices that have recently been developed. In many embodiments, a laparoscope 34 will allow direct optical imaging, often while the pelvic region is distended using gas insufflation. The present methods may be optically directed using a variety of existing endoscopic structures, depending on the treatment site and access approach. Laparoscopes, arthoscopes, hysteroscopes, or the like may be used (or adapted for use) in the present methods. Alternatively, conventional optical imaging capabilities may be incorporated into probe 10, or specialized fiber optic image guides may be used, either separated from or incorporated into probe 10. In some embodiments, the therapy may be directed using a remote imaging modality, such as fluoroscopy, ultrasound, magnetic resonance imaging, or the like. It is also possible to take advantage of the controlled tissue contraction of the present invention in a more traditionally invasive therapy.

Referring now to FIG. 5, bladder B can be seen to have dropped from its nominal position (shown in phantom by outline 36). While endopelvic fascia EF still supports bladder B to maintain continence when the patient is at rest, a momentary pulse P opens the bladder neck N resulting in a release through urethra UR.

A known treatment for urinary stress incontinence relies on sutures S to hold bladder neck N closed so as to prevent inadvertent voiding, as seen in FIG. 6. Sutures S may be attached to bone anchors affixed to the pubic bone, ligaments higher in the pelvic region, or the like. In any case, loose sutures provide insufficient support of bladder neck N and fail to overcome urinary stress incontinence, while over-tightening of sutures S may make normal urination difficult and/or impossible.

As shown in FIG. 7, by selectively contracting the natural pelvic support tissues, bladder B can be elevated from its lowered position (shown by lowered outline 38). A pressure pulse P is resisted in part by endopelvic fascia EF, which supports the lower portion of the bladder and helps maintain the bladder neck in a closed configuration. In fact, fine-tuning of the support provided by the endopelvic fascia is possible through selective contraction of the anterior portion of the endopelvic fascia to close the bladder neck and raise bladder B upward. Alternatively, lateral repositioning of bladder B to a more forward position may be effected by selectively contracting the dorsal portion of endopelvic fascia EF. Hence, the therapy of the present invention may be tailored to the particular weakening exhibited by a patient's pelvic support structures.

Another condition which is suitable for treatment using the methods of the present invention is illustrated in FIG. 7A. In this patient, a posterior portion PP of bladder B protrudes into vagina V so that an acute angle is formed by the posterior wall of the urethra and the anterior wall of the urinary bladder. Such a condition, generally referred to as cystocele, may be effectively treated by selectively contracting the endopelvic fascia and/or other pelvic support tissues and repositioning the bladder as described above. Additional conditions which may be treated using the methods of the present invention include enterocele (a hernial protrusion through a defect in the rectovaginal or vesicovaginal pouch), rectocele (prolapse or herniation of the rectum), and uterovaginal prolapse (downward movement of the uterus so that the cervix extends into or beyond the vaginal orifice, usually from injuries dur-

ing childbirth or advanced age). For each of these conditions, the methods of the present invention generally make use of the natural support tissues within the pelvis, generally by selectively contracting those support tissues to reposition and/or contain the displaced organs. As will be described in more detail hereinbelow, herniated structures may be treated at least in part by repositioning the protruding structures behind the tissue which nominally contain them, and then selectively contracting the containing tissues to prevent recurrence of the hernia.

Referring now to FIGS. 8 and 9, a depth D of the endopelvic fascia EF (and adjacent tissue T) heated by bipolar probe 10 will depend on the power applied, on a spacing S between first and second electrodes 18, 20, and on the surface diameter 39 of the electrodes. Generally, spacing S will be between about 0.25 and 4.0 mm. More specifically, spacing S will preferably be in the range from about 1 to 4 times the electrode diameter 39, with the electrode diameter often being between about 0.25 and 4.0 mm, preferably being between about 0.25 and 2.0 mm, and ideally being between 0.25 and 1.0 mm. This will limit the heating depth D to generally less than about 2.0 mm, and often to less than 1.0 mm. Advantageously, the temperature gradient along the edge of the treatment zone is quite steep. By such selective heating of the endopelvic fascia EF, collateral damage to the underlying tissues T is limited. Fascia will contract when heat is applied by such a structure for a very short time, the target tissue ideally being heated for a time in a range from about 0.5 to 5 seconds. In general, selectively targeting the fascia adjacent the surface maximizes the tissue contraction provided by heating, and greatly limits necrosis, lesioning, and other collateral injuries to the vaginal mucosa and the muscular tissues which help to support the bladder in the desired position. As more fully explained in application Ser. No. 08/910,775 filed Aug. 13, 1997, the electrodes may be cooled to prevent injury to the engaged tissue surface. Cooling may be provided, for example, by forming the electrodes of thermally conductive tubing, and by running a cold fluid through the tubing.

As illustrated in FIG. 8, a film 41 of saline, either natural or introduced, may be disposed over the engaged tissue surface. Film 41 prevents the electrode surfaces from sticking to the engaged tissue, and can also provide a more even impedance and/or power through the circuitry. Drying of the tissue surface due to CO₂ insufflation may be avoided by providing a saline irrigation of about 1 cc/min. during the tissue contraction procedure.

While spacing S will often be fixed, it should also be understood that the separation between the first and second electrodes may optionally be varied to controllably vary the heating depth D.

The sweeping of first and second electrodes 18, 20 of probe 10 over the endopelvic fascia EF to discretely raise the bladder can be understood with reference to FIG. 9. The endopelvic fascia EF is heated and contracted by the passing electrodes, the fascia typically contracting by an amount within the range between about 30 and 50%. As the electrodes sweep across the fascia surface, they define electrode paths 40. The electrode paths are closer together after probe 10 has swept by, so that the overall width of the endopelvic fascia decreases by an amount of between about 0.3 and 0.5 times electrode spacing S each time probe 10 sweeps over untreated fascia (in our example). Hence, the total distance that the bladder is raised can be varied by varying the number of sweeps of probe 10. The probe will preferably sweep a different section of the endopelvic fascia each time, as fascia which has previously been contracted will undergo only a more limited contraction.

Hence, probe 10 will often be moved axially by an amount of at least the electrode spacing S prior to each sweep.

A variety of alternative electrode configurations are illustrated in FIGS. 10–12D. FIG. 10 illustrates a probe 42 which is otherwise similar to probe 10 of FIG. 1, but which includes first and second interleaved helical electrodes 44, 46. These electrodes alternate about the distal end of helical probe 42 in a “barber pole” configuration. This allows a greater amount of shrinkage each time helical probe 42 engages a fascia or ligament surface, as heating will be provided between each span of the tissue between adjacent electrodes, and also eliminates any need for angular alignment of the probe. Advantageously, spacing S remains substantially uniform over the probe surface.

Distally oriented probe tip 48 includes first and second distally oriented electrodes 50, 52 which are again separated by spacing S. This structure is particularly well-suited for contracting tissues having surfaces which are oriented normal to the axis of the probe, and for spot contraction of certain tissue bands (such as ligaments). An axially-ended probe tip 54 includes alternating first and second axially-ended ribbon or wire electrodes 56, 58, and is adapted for engaging both laterally and proximally oriented tissue surfaces. Note that axial first and second electrodes 56, 58 may comprise ribbon structures or wires which are inset into axially-ended electrode tip 54, thereby avoiding inadvertent engagement of tissues adjacent the target tissue surface. Sensor 32 optionally measures the temperature of the target tissue.

In some embodiments, the electrode structures on the probes of the present invention will provide feedback to the probe regarding the amount of tissue contraction. Referring now to FIG. 13A, a moveable electrode probe 60 includes rotatable first and second electrodes 62, 64 which roll about a shaft 66 to facilitate sweeping of the electrodes over the target surface. The electrodes also include radial protrusions, presenting a structure which looks somewhat like a gear with pointed teeth. The protrusions minimize sliding between the electrode surface and the target tissue surface. Hence, as the engaged tissue contracts along the axis of shaft 66, it draws the first and second rotatable electrodes 62, 64 together.

By measuring the displacement between first electrode 62 and second electrode 64, moveable electrode probe 60 provides an indication of the total tissue shrinkage. The attending physician or an electronic electrode energizing control circuit may make use of this feedback to control tissue heating. Alternatively, the probe may measure the force the contracting tissue imposes on the electrodes without allowing any actual displacement of one electrode relative to the other. Such a structure would maintain the fixed spacing S between the electrodes.

An even simpler feedback mechanism is illustrated in FIG. 13B. Spot contraction probe 70 includes first and second shortable electrodes 72, 74 which will contact each other when the engaged tissue is contracted by a predetermined amount. The shorting of the electrodes will often provide a signal terminating the energizing of the electrodes. The electrodes will optionally have protrusions 76 which press into the tissue surface to avoid sliding.

Those with skill in the art will realize a variety of mechanisms may be used to measure shrinkage of the tissue, including fiber optic measuring mechanisms, micro-switches, strain gauges, or the like. However, the electrode structure illustrated in FIG. 13B has the advantage that the shorting of the electrodes automatically terminates heating, allowing the device to both measure and control shrinkage with a very simple structure.

15

In some embodiments, a variable spacing between first and second bipolar electrodes may allow the surgeon to control the depth of heating. For example, as illustrated in FIG. 13C, rotating a variable spacing probe **80** allows the physician to engage a target tissue surface with alternate portions of angled electrodes **82**, **84** to vary an effective spacing ES therebetween. Note that local electrode surface diameters of angled electrodes **82**, **84** vary with separation, so that a ratio of electrode separation ES to local surface diameter remains about 2 to 1. Clearly, more complex spacing varying mechanisms are also possible.

A wide variety of alternative electrode structures are also possible. Referring now to FIG. 14, a still further alternative embodiment of the present laparoscopic or endoscopic probe **90** has first and second partially enclosed roller electrodes **92**, **94** for rolling against tissue surface without inadvertently engaging the surrounding tissues. More than two rollers may be used, with the polarity of the electrodes generally alternating (as can be understood with reference to FIGS. 10–12B). Such alternating electrodes may instead be defined by axial wires or ribbons in a straight configuration, or may curve in alternating spirals at the distal end of the probe. In some embodiments, the electrodes may be defined by the ends of coaxial tubes with insulating material between the tubes and over the outer tube.

While the shafts supporting the electrodes of the present invention are generally shown as straight structures, many of these embodiments may alternatively incorporate bends in the shafts between the proximal and distal ends. Alternatively, the shafts may be articulated to facilitate engaging the target tissue surface. Hence, the present invention encompasses not only straight shafts, but shafts which are slanted, angled, articulated, flexible, inflatable, or the like, to facilitate engaging a target tissue from the selected approach position.

Referring now to FIG. 15, a least invasive probe **100** includes a distal needle **102** to facilitate inserting an articulated shaft **104** and access the fascia supporting the pelvic floor. The device will typically gain access to this treatment site by percutaneous insertion through the skin of the abdomen, through the wall of the vagina, or through the urethra. A joystick **106** manipulates articulated shaft **104**, which can facilitate positioning the electrodes against the target tissue. Optionally, joystick **106** may also be used to direct needle **102** to penetrate the vagina mucosa or bladder surface.

Methods for accessing endopelvic fascia EF using least invasive probe **100** are illustrated in FIGS. 15A–15C. Shaft **104** is inserted in the vagina and placed against the anterior surface. Needle **102** perforates the vaginal mucosa VM, optionally extending through endopelvic fascia EF to lay adjacent to (and in contact with) the endopelvic fascia between the endopelvic fascia and bladder B in the vesicle-vaginal space **101**. Alternatively, needle **102** may be directed through vaginal mucosa VM without perforating endopelvic fascia EF to lay in contact with the endopelvic fascia between the endopelvic fascia and the vaginal mucosa. In either case, once least invasive probe **100** has accessed endopelvic fascia EF, one or more electrodes will engage and heat the fascia to induce contraction. In some embodiments, a two-pronged needle probe could be used, with each needle having an electrode surface to facilitate bipolar resistive heating. Alternatively, the needle may be removed from the positioned least invasive probe **100** and replaced with a deployable electrode structure, as described hereinbelow.

FIG. 15D illustrates a still further alternative method for accessing endopelvic fascia EF. In this embodiment, a cystoscope **105** is inserted through urethra UR into bladder B. A curved needle **103** punctures through the bladder wall with a

16

retrograde orientation, the needle preferably being clear of the urethral vesicle junctions and trigon. Curved needle **103** is again positioned in contact with endopelvic fascia EF on the anterior surface of the vagina. Such a method may make use of an off-the-shelf cystoscope.

Least invasive probe **100** will often be positioned using a remote imaging mechanism, typically in a fluoroscopically or ultrasonically directed procedure. To help ensure that the electrodes of least invasive probe **100** are properly oriented toward the target tissue, asymmetric handle **108** will often be rotationally affixed relative to the electrode. In some embodiments, electrodes may simply be positioned on the surface of articulatable shaft **104**, on needle **102**, or the like. However, to minimize the cross-section of **104** so as to facilitate percutaneous insertion, it will often be advantageous to include an electrode support structure which is deployable from the shaft once the electrodes are positioned adjacent the target surface. Such a deployable electrode structure may optionally be inserted through articulated shaft **104** after removal of needle **102**, or may instead be incorporated into the distal end of articulated shaft **104**.

An example of a deployable electrode structure is illustrated in FIG. 16. Balloon system **110** includes a shaft **112** having an angular position indicating line **114**. Line **114** helps to indicate the orientation of a distal balloon **116** from the proximal end of the balloon system. In other words, line **114** allows the physician to verify that first and second balloon electrodes **118**, **120** are properly oriented to engage the target tissue.

The use of balloon system **110** will be explained with reference to FIGS. 16, 17A and 17B. Balloon **116** is inserted between the endopelvic fascia EF and an adjacent tissue AT while the balloon system is in a narrow diameter configuration. In the narrow configuration, balloon **116** is deflated and the electrodes are disposed along shaft **112**. Once the deflated balloon is at the desired location, the balloon may be roughly rotationally positioned with reference to line **114** on shaft **112**. Balloon **116** can then be inflated through inflation port **122** on proximal balloon housing **124**. As the balloon inflates, it separates endopelvic fascia EF from adjacent tissue AT. Additionally, as balloon **116** defines a substantially flat structure when inflated, it will tend to self-orient, so that first and second balloon electrodes **118**, **120** engage the endopelvic fascia as shown in FIG. 17B.

In some embodiments, balloon **116** is bilaterally asymmetric to help verify the orientation of the deployed electrodes. The asymmetric feature of balloon **116** may comprise simple radiopaque or ultrasonically imageable markers, differing first and second electrode shapes, or the like. In the embodiment illustrated in FIG. 17B, the balloon is asymmetrically mounted to shaft **112**. When viewed under fluoroscopy, ultrasound, or the like, this asymmetry helps verify the position and orientation of the electrodes.

Once the first and second balloon electrodes **118**, **120** are positioned, the electrodes may be energized through electrical coupler **126**. A third connector **128** on proximal housing **124** may be used for directing insertion of the balloon with a guidewire, gas insufflation, optical imaging, or the like.

A wide variety of alternative balloon configurations may be used. For example, a two-part balloon **130** may be filled in-part with a radiopaque liquid **132**, and in-part with a non-radiopaque gas or liquid **134**, as can be understood with reference to FIGS. 18A and B. Under remote imaging, gas **134** and liquid **132** may be easily distinguished to verify the orientation of the electrodes.

To enhance tissue contraction, it may be convenient to include a larger number of electrodes on the least invasive

probe structure. Typically, these electrodes will be arranged as alternating bipolar structures, as can be understood with reference to FIGS. 19–20C. In some embodiments, the electrodes may be selectively energizable to vary the amount of contraction, and to direct the resistive heating to the target tissue without rotating the probe to a specific orientation. A barber pole balloon 140 having electrodes similar to the structure illustrated in FIG. 10 is shown in FIG. 19.

The balloon structures of the present invention need not necessarily be flat. For example, as illustrated in FIGS. 20A–C, a cylindrical balloon 150 may be inflated to separate the fascia from the adjacent tissue, and to enhance engagement of at least some of the electrodes against the fascia. By selectively energizing the electrodes which engage the endopelvic fascia, collateral damage to the adjacent tissues may be avoided. As illustrated in FIG. 20C, cylindrical balloon 150 may be partially deflated to avoid distention of the endopelvic fascia during heating, and thereby enhance contraction. Such partial deflation may also increase the number of electrodes which engage the target tissue.

Still further alternative deployable electrode support structures are illustrated in FIGS. 21A–23C. For example, a self-spreading electrode system 160 includes a sheath 162 which restrains elongate first and second electrode support structures 164, 166. Once the self-spreading system is positioned at the treatment site, sheath 162 is withdrawn proximally (or atraumatic tip 168 is advanced distally). The resilient support structures separate laterally when released from sheath 162, thereby deploying restrainable electrodes 170, 172. Optionally, a web 171 between the electrodes limits the separation of the electrodes to the desired distance. A similar deployable electrode structure may include elongate electrode support structures which are nominally straight, but which may be laterally displaced by a pull wire 174 to deploy the electrodes, as illustrated in FIGS. 22A–C.

Still further alternative deployable electrode structures are possible. As illustrated in FIGS. 23A–C, lateral deployment of flat electrode support structures 180 may be effected by drawing a middle member 182 proximally. Fasteners 184 support the structures, and interact with a slot 186 in middle member 182 to limit axial movement of the middle member and thereby control the spacing between the deployed electrodes.

As explained above, thermocouples or other temperature sensors may be incorporated into the least invasive probes of the present invention, preferably between the bipolar electrodes. Feedback control may alternatively be provided by monitoring the energizing circuit, as was also explained above. Those of skill in the art will recognize that balloon electrode support structures may make use of single lumen, or multiple lumen shafts for inflation, energizing wires, temperature sensing feedback, guidewires, gas or fluid insertion, and the like.

A grasping probe 190 is illustrated in FIG. 24. Grasping probe 190 includes a pair of arms 192 which rotate about a hinge 194. Electrodes 196 are disposed between arms 192 and oriented so as to engage the surface of the tissue which is grasped by the arms.

A method for using grasping probe 190 is illustrated in FIGS. 25A and 25B. In this embodiment, arms 192 engage abdominal fascia AF of abdominal wall AW. Arms 192 grasp and draw a region of the tissue TR inward so as to reduce tension within the grasped region. Electrodes 196 engage abdominal fascia AF within the tissue region TR, and a current flux is directed between these electrodes to heat and shrink the abdominal fascia.

Preliminary work in connection with the present invention has shown that a wall stress of 1.3 lbs. per linear inch can limit the shrinkage of some fascia to about 20%, rather than the 40% to 50% shrinkage observed when that fascial tissue is not in tension. Hence, the method illustrated in FIGS. 25A and 25B will find a variety of applications for shrinking tissues which would otherwise be under tension during the procedure. Specifically, the illustrated method may be used during abdominoplasty (sometimes referred to as a “tummy tuck”) to selectively shrink the abdominal wall. By reducing tension in the abdominal tissues, the shrinkage provided from the application of heating energy can be increased significantly. Alternatively, the amount of area treated to provide a particular reduction in length of the fascia can be minimized. If sufficient tissue is treated using such a method, the waistline of the patient could be reduced by several inches.

Grasping probe 190 may also be used in a wide variety of procedures, and a variety of grasping structures might be used, generally by grasping a region of the tissue to be treated and pulling the region inward to eliminate and/or reduce tension in the grasped region. The grasped tissue should be free to shrink while grasped by the probe, and the fascia should be exposed for contact with the bipolar electrodes, or otherwise in a position to be heated by a heating element. In some embodiments, the grasped tissue may be heated by a laser, a monopolar radiofrequency electrode, a microwave antennae, focused ultrasound transducer, a heated probe surface, or the like. The grasped fascia may generally be heated by any heating element, and will shrink to a greater extent than would otherwise result from heating tensioned fascia (or other collagenated tissue).

Grasping probe 190 may include a wide variety of alternative grasping structures. In some embodiments, the ends of arms 192 may include protruding points to penetrate into and more firmly grip the fascia. A vacuum mechanism may be used to grasp the tissue region TR between the arms, or discrete vacuum ports on each arm might be used. Arms 192 might slide (rather than pivot) relative to each other, and electrodes 196 may be affixed to a single structure to maintain a predetermined interelectrode separation, and to limit tissue heating depth, as described above.

The devices and methods of the present invention will find particularly advantageous applications for treatment of hernias, as can be generally understood with reference to FIGS. 26 and 27. In FIG. 26, a portion of a stomach ST protrudes through an enlarged esophageal hiatus EH of a diaphragm D. This can lead to severe reflux, in which the acidic stomach juices are persistently regurgitated, eroding the wall of the esophagus and causing a burning pain. These symptoms are often aggravated by a defective lower esophageal sphincter LES. While such conditions may be treated using known methods, particularly using laparoscopic Nissen fundoplication, these surgical procedures require significant amounts of surgical experience and skill to be successful. Lack of experience in these specialized procedures can lead to severe complications, including pneumothorax, dysphasia, recurrent reflux, and loss of motility, thereby making it difficult and/or impossible to eat. Hiatal hernias may include a tear in the diaphragm of between 1 and 5 cm adjacent hiatus EH.

To overcome these disadvantages, the hiatal hernia illustrated in FIG. 26 may instead be treated by selectively shrinking the fascia of diaphragm D. Using the methods and devices of the present invention, the diameter of esophageal hiatus EH can be decreased so that the diaphragm properly contains the stomach. Specifically, stomach ST is repositioned below diaphragm D, and grasping probe 190 (illustrated in FIG. 24) grasps the upper or lower surface of diaphragm D adjacent the

esophageal hiatus. A portion of the diaphragm adjacent the esophageal hiatus is drawn inward, preferably circumferentially so as to decrease the size of the hiatus. The fascia of diaphragm D may then be heated and contracted to prevent stomach ST from again protruding through the diaphragm. Alternatively, probe 10 (illustrated in FIG. 1), or any of the alternative tissue contracting structures described herein, might be used, particularly where diaphragm D is not under tension during treatment.

To improve the competence of lower esophageal sphincter LES, fascia adjacent and external to the sphincter may be treated to close the valve more effectively. In some embodiments, such as where a Nissen procedure would normally be indicated, or where a reinforcing patch might otherwise be placed over the defect to prevent recurrence of the hiatal hernia, the fascial covering of the top of the stomach SF and the corresponding surface of the diaphragm SD may be treated to promote the formation of an adhesion between these surfaces (which will engage each other once stomach ST is properly positioned below diaphragm D). Such an adhesion would decrease the likelihood of recurrence of the hiatal hernia, and may generally reinforce the defect.

A method for treating a hiatal hernia by forming a reinforcing adhesion can be understood with reference to FIGS. 26A–26C. Stomach ST is dissected from the surrounding diaphragm D, with a dissected portion of the diaphragm DD often remaining affixed to the stomach by adhesions AD, as illustrated in FIG. 26A. The resulting enlarged hole in diaphragm D is contracted by shrinking the collagenated diaphragm about the hole, as described above and as illustrated in FIG. 26B. To secure stomach ST below the contracted diaphragm, the adjacent surfaces of the stomach and the diaphragm are treated to promote formation of an adhesion ADZ connecting these tissues. The dissected diaphragm segment DD about stomach ST may be removed to reduce necking, or may be left in place. A probe PR treating a superior surface of stomach ST is illustrated in FIG. 26C. It should be noted that the resulting 2 treated, opposed surfaces will generally develop adhesions, while the treatment of only one of the opposed surfaces will not reliably promote adhesion formation. Once diaphragm D is contracted to properly size esophageal hiatus EH, and once adhesion ADZ connects the diaphragm to the stomach, reoccurrence of the hiatal hernia is substantially inhibited.

The methods and devices of the present invention are also suitable for treatment of inguinal or abdominal hernias, as illustrated in FIG. 27. In inguinal hernia IH, a portion of the small intestine SI protrudes through the inguinal canal IC adjacent the spermatic cord SC. Using the methods of the present invention, the abdominal wall adjacent the deep inguinal ring DIR and/or adjacent the superficial inguinal ring SIR may be selectively contracted about the spermatic cord once the small intestine SI has been pushed back into the abdominal cavity. Selective shrinking of the fascial tissue about the spermatic cord will allow the fascial tissue to properly contain the abdominal organs, often without having to resort to sutures, patches, and the like. Where the abdominal wall is not torn adjacent the hernia, treatment will often be possible without grasping and drawing the tissue inward, as the stretched tissue should not be under tension after the herniated bowel has been repositioned within the abdomen. Work in connection with the present invention has found that even hernias resulting in small tears of the fascial tissue can be corrected by shrinking using a laparoscopic probe similar to that illustrated in FIG. 1. Preferably, such tears will be less than 2 cm in length, ideally being under 1 cm. In some embodiments, particularly where extended tears of the fascial

tissue have been found, the selective shrinking of the present invention may be combined with suturing, patches, and other known hernia repair techniques. Once again, where the abdominal wall is under tension during the treatment procedure, a grasping probe, such as that illustrated in FIG. 24, might be used to enhance the effective contraction of the abdominal wall.

Fascial tissue, once shrunk using the methods of the present invention, has nearly 20 times the strength needed to contain the intestines in place. Nonetheless, to prevent the treated tissue from stretching or tearing during the healing process, a retention girdle RG may be worn. Retention girdle RG may help contain the tremendous forces generated by coughing sneezing, and the like, particularly for a period of about 8 weeks after a selectively shrinking of the fascia.

The present invention optionally relies on inducing controlled shrinkage or contraction of a tissue structure which comprises or supports portions of the patient's urethra. The tissue structure will be one that is responsible in some manner for control of urination and where contraction of the tissue structure will have the effect of reducing urinary leakage. Exemplary tissue structures include the urethral wall, the bladder neck, the bladder, the urethra, bladder suspension ligaments, the sphincter, pelvic ligaments, pelvic floor muscles, fascia, and the like. In one exemplary embodiment, a portion of the urethral wall at or near the urethral sling is heated to contract tissue and create a kink or crease in the wall which provides a preferential closure site for the urethra. In effect, it becomes easier for the patient's weakened tissue support structures to close the urethra and maintain continence. In another exemplary embodiment, the supporting tissues and ligaments are shortened to at least partially reverse the stretching and weakening that has resulted from pregnancy or other patient trauma. By selectively contracting one or more of the pubococcygeal, iliococcygeal and/or detrusor muscles, support of the ureter and urinary sphincter can be substantially improved.

Tissue contraction results from controlled heating of the tissue by affecting the collagen molecules of the tissue. Contraction may occur as a result of heat-induced uncoiling as the collagen β -pleated structure and subsequent re-entwinement as the collagen returns to body temperature. By maintaining the times and temperatures set forth below, significant tissue contraction can be achieved without substantial tissue necrosis.

While the remaining description is specifically directed at an energy-applying probe introduced through the urethra of a female patient, it will be appreciated that the methods of the present invention can be performed with a variety of devices and systems designed to deliver energy to tissue target sites resulting in heating of the tissue and selective contraction of tissue support structures. The temperature of the target tissue structure can here be raised to a value in the range from 70° C. to 95° C., for a time sufficient to effect the desired tissue shrinkage. In these embodiments, the temperature will be raised from 1/2 second to 4 minutes, optionally being from 0.5 minutes to 4 minutes and often from 1 minute to 2 minutes. The total amount of energy delivered will depend in part on which tissue structure is being treated as well as the specific temperature and time selected for the protocol. The power delivered will often be in the range from 1 W to 20 W, usually from 2 W to 5 W.

Referring now to FIG. 28, a heat-applying probe 210 comprises a probe body 212 having a distal end 214 and a proximal end 216. An electrode 218 is disposed near the distal end 214 of the probe body 212 and is connected via electrically conductive wires (not shown) extending the length of the

body and out through a connector cable **220** having a plug **224** at its proximal end. Usually, a proximal handle or hub **226** is provided at the proximal end **216** of the probe body **212**. Conveniently, the hub **226** may include an arrow **228** indicating alignment of the probe hub with the asymmetrically mounted electrode **218**.

The electrode **218** is intended for delivering RF energy when attached to a power supply **230** (FIG. **30**) connected through the plug **224** in cable **220**. As shown in FIGS. **28** and **30**, the single electrode **218** is intended for monopolar operation. The electrode **218** may be formed from many conventional electrically conductive electrode materials, such as stainless steel, platinum, conductive plastic, or the like. The probe may be formed from any conventional medical catheter or probe material, including organic polymers, ceramics, or the like. Usually, the probe body will be sufficiently flexible to be introduced through the urethra with minimal discomfort, but it would also be possible to utilize substantially rigid probes as well.

The energy-applying probe **210** could also be adapted for bipolar operation by including two or more isolated electrode surfaces near its proximal end **218** (with electrically isolated conductors to each of the electrode surfaces). As shown in FIG. **28 B**, a plurality of axially spaced-apart electrode surfaces **218a**, **218b**, **218c**, and **218d** could be connected with an alternating polarity. Alternatively, as shown in FIG. **28C**, a plurality of circumferentially spaced-apart electrodes **218e**, **218f**, **218g**, and **218h** could also be connected with alternating polarity. Usually, each of the electrodes will be connected through the probe body **212** by a single isolated wire or other conductor, terminating in the connector plug **224**. Thus, the multiple electrode configurations of FIGS. **28B** and **28C** can be operated either in a monopolar or bipolar fashion, depending on how the power supply is configured.

A particular electrode configuration including a pair of axially spaced-apart electrodes **218i** and **218j** is illustrated in FIG. **28D**. This electrode configuration is intended for treating the urethral wall at locations immediately upstream and downstream of the urethral sling. Typically, the electrodes will be spaced-apart by distance in the range from 1 mm to 5 mm, preferably from 1.5 mm to 3 mm.

In all the electrode configurations of FIGS. **28–28D**, the total electrode area will usually be in the range from 1 mm² to 10 mm², preferably from 2 mm² to 6 mm². Moreover, the electrodes will be configured to reduce or eliminate electrical current concentrations when operating in a radio frequency mode. Usually, the electrode surfaces will be relatively smooth, and the edges will be insulated or protected by the adjacent probe body **212**. In this way, the electric field or flux emanating from the electrodes **218** will be relatively uniform, resulting in generally even heating of the tissue which is contacted by the electrode.

A further exemplary electrode embodiment is shown in FIG. **29**. There, a plurality of circumferentially spaced-apart electrodes **230** are mounted on an inflatable balloon **232** at the distal end **234** of an energy-applying probe **236**. Each of the electrodes **230** will be connected to a single or to multiple conductors running to the proximal end (not shown) of the energy-applying probe **236**, in a manner similar to that illustrated for probe **210**. By mounting the electrodes **230** on a radially expandable balloon or other expansion member (e.g., an expandable cage), the electrodes can be firmly contacted against an interior surface of the urethra. Moreover, the contact can be maintained as the urethral wall expands or contracts, depending on how the energy is applied.

Referring now to FIG. **30**, use of the energy-applying probe **210** for treating a target site TS in a urethra draining bladder

B is illustrated. The probe **210** is inserted so that electrode **218** contacts the target site TS, which is typically adjacent the urethral sling. The electrode may be positioned based on ultrasonic imaging, fluoroscopic imaging, or the like. Alternatively, the probe may be inserted to a known depth using a scale formed on the exterior of the probe (not shown). After properly positioning the electrode **218**, RF energy is applied from power supply **230** typically at a level in the range from 1 W to 20 W, usually from 2 W to 5 W. As illustrated, the electrode **218** is a monopolar electrode, and a counter electrode **240** will be attached to an external portion of the patient's skin. The counter electrode is connected to the power supply **230** by an appropriate cable **242** and plug **244**. Energy is applied until the tissue temperature is reached and maintained for a desired amount of time. Optionally, a temperature sensor can be provided on the probe **210**, and feedback control of the amount of energy being applied can be implemented. For example, a thermal couple, a thermistor, or other temperature sensor can be mounted adjacent to or within the electrode **218**. Alternatively, a penetrating element (not shown) can be provided on the probe to enter beneath the surface of the urethral wall by a pre-selected distance to measure internal tissue temperature. Other known temperature control techniques could also be utilized.

Referring now to FIGS. **31–33**, a heat-applying probe **400** comprises a probe body having a sheath component **402** and an electrode rod component **404**. The electrode rod **404** is reciprocatably mounted in a lumen of the sheath **403** so that a distal electrode array **406** on the rod **404** may be retracted and extended into and from the distal end **408** of the sheath **402**. A proximal handle **410** is provided on the sheath, and a proximal connector **412** is provided on the electrode rod component **404**.

The electrode array **406**, as illustrated, includes four individual electrode tips **420** each of which has a sharpened distal end suitable for penetrating into tissue, particularly for transmucosal penetration through the vaginal wall into the tissue structures which support the urethra or urinary sphincter. The electrode tips **420** are sufficiently resilient so that they will be radially contracted when the rod **404** is withdrawn proximally into the sheath **408**. The electrode tips **420** will resiliently expand from the sheath when the electrode rod component **404** is advanced distally when the sheath **408** is positioned near the tissue target site, as discussed in more detail below. As illustrated, the electrode tips **420** are commonly connected to a single plug in the connector **412**. Thus, the probe **400** is only suitable for monopolar operation. It will be appreciated, however, that the multiple electrode tips **420** could be connected through separate, isolated conductors within the rod **404** and further be connected through multiple pins in the connector **412**. Thus, the probe **400** could readily be adapted for bipolar operation. Usually, all components of the probe will be insulated, other than the electrode tips **420**. Alternatively, some other portion of the rod **404** or sheath **402** could be formed from electrically conductive material and utilized as a common or indifferent electrode so that the probe could be utilized in a bipolar manner. A variety of such modifications would be possible with the basic probe design.

Referring now to FIGS. **34–37**, use of probe **400** for contracting tissue ligaments which support the urethra in the region of the urethral sling will be described. Initially, the treating physician manually examines the vagina V to locate the region within the vagina beneath the urethral sling. The probe **400** is then introduced into the vagina. Conveniently, the physician may manually locate the probe, again by feeling the region which is supported by the urethral sling. After the sheath **402** of the probe **400** is properly positioned, the rod

component 404 will be distally advanced so that the electrode tips 420 are penetrated into the tissue which supports the urethra, typically the pubococcygeal muscles, iliococcygeal muscles or the detrusor muscle as illustrated in FIGS. 36 and 37. The physician will continue to use a finger F to hold the probe against the vaginal wall to facilitate penetration of the electrode tips 420. RF energy can then be applied through the probe in order to heat the target tissue to temperatures and for time periods within the ranges set forth above. The supporting tissues are thus contracted in order to reduce urinary leakage and enhance patient continence.

The procedures of the present invention result in bulking and buttressing of the supporting tissue structures as the tissue heal. This result is in addition to the tissue contraction, with both the contraction and tissue bulking/buttressing acting to enhance patient continence.

Referring now to FIG. 38, a kit 500 includes a tissue contracting probe 502 and instructions for its use 504. Contracting probe 502 and instructions 504 are disposed in packaging 506. Contracting probe 502 here includes a structure similar to probe 10 of FIG. 1, but has a radially ended tip 54 to facilitate laparoscopically engaging the electrode wires against both laterally and axially oriented tissues. Instructions 504 will often set forth the steps of one or more of the methods described herein above for treating urinary incontinence. Additional elements of the above-described systems may also be included in packaging 506, or may alternatively be packaged separately.

Instructions 504 will often comprise printed material, and may be found in whole or in part on packaging 506. Alternatively, instructions 504 may be in the form of a recording disk or other computer-readable data, a video tape, a sound recording, or the like.

The present invention further encompasses methods for teaching the above-described methods by demonstrating the methods of the present invention on patients, animals, physical or computer models, and the like.

While the exemplary embodiment has been described in some detail, by way of illustration and for clarity of understanding, various modifications, adaptations, and changes will be obvious to those of skill in the art. Therefore, the scope of the present invention is limited solely by the appended claims.

What is claimed is:

1. A method to treat urinary stress incontinence, the method comprising:

introducing a probe into a patient body;
aligning the probe with a collagenous pelvic tissue which supports the urethra within the patient body; and
energizing the probe to heat a portion of the pelvic support tissue so that the pelvic support tissue is contracted to inhibit incontinence.

2. A method as claimed in claim 1, further comprising engaging first and second electrodes against the pelvic support tissue and applying an electrical potential across the first and second electrodes to heat a portion of the pelvic support tissue disposed therebetween so as to reposition a bladder neck within the patient body.

3. A method as claimed in claim 2, further comprising monitoring a temperature of the heated tissue with a temperature sensor of the probe, the sensor being in thermal contact with the heated tissue.

4. A method as claimed in claim 2, wherein the first and second electrodes engage the pelvic support tissue with a predetermined electrode surface diameter and spacing between the electrodes to limit a tissue heating depth.

5. A method as claimed in claim 4, wherein the depth of tissue heating is less than about 2.0 mm, a surface diameter of the electrodes being between about 0.25 and 4.0 mm, the spacing between the first and second electrodes being between about 1 and 4 times the electrode surface diameter.

6. A method as claimed in claim 2, further comprising sweeping the first and second electrodes across the pelvic support tissue while applying the electrical potential to heat a band of the pelvic support tissue substantially bordered by swept paths of the first and second electrodes.

7. A method as claimed in claim 1, wherein the electrical potential has a frequency of between about 100 and 1,000 khz and an amplitude of between about 20 and 200 volts rms.

8. A method as claimed in claim 7, wherein the pelvic support tissue reaches a maximum temperature of between about 60° C. and 110° C. for a time between about 0.5 and 5.0 seconds.

9. A method as claimed in claim 1, further comprising monitoring a temperature of the pelvic support tissue while heating.

10. A method as claimed in claim 1, wherein the aligning step comprises laparoscopically imaging the pelvic support tissue.

11. A method as claimed in claim 1, wherein the introducing step comprises inserting the probe while the probe is in a narrow configuration, and further comprising deploying at least one of the first and second electrodes to a wide configuration prior to the heating step, the wide configuration being wider than the narrow configuration.

12. A method as claimed in claim 1, further comprising laterally repositioning a bladder neck within the patient body by heating an alternative portion of the pelvic support tissue.

13. An endoscopic method for treating urinary stress incontinence, the method comprising:

introducing a probe into a patient body;
optically imaging the probe and a target tissue of the patient body, the target tissue comprising a portion of at least one of an endopelvic fascia and an arcus tendineus fascia pelvis which support the patient's urethra;
positioning an electrode of the probe against the target tissue; and
energizing the electrode to heat and contract the target tissue without substantially ablating the target tissue.

14. An endoscopic method as claimed in claim 13, further comprising engaging first and second electrodes against the target tissue and applying an electrical potential across the first and second electrodes to heat a portion of the target tissue disposed therebetween, wherein the first and second electrodes engage the fascia with a predetermined spacing therebetween to limit a depth tissue heating and to avoid damaging tissue below the target tissue.

15. A method for treating urinary incontinence in a patient, said method comprising applying an amount of energy to a collagenous tissue structure supporting the patient's urethra wherein the amount of energy is sufficient to cause partial shrinkage of the tissue and the tissue shrinkage inhibits urinary incontinence.

16. A method as in claim 15, wherein the tissue structure is selected from the group consisting of a region of the urethra suspension ligaments, pelvic ligaments, pelvic floor muscles, and fascia.

17. A method as in claim 16, wherein the tissue structure comprises the pubococcygeal muscle, the iliococcygeal muscle, or the detrusor muscle and adjacent fascia, and the applying step comprises penetrating an energy-applying element into the tissue structure from the vagina.

25

18. A method as in claim 15, where the amount of energy applied is sufficient to raise the tissue structure to a temperature in the range from 60° C. to 95° C. for a time in the range from 0.5 minute to 4 minutes.

19. A method for treating urinary incontinence in a patient, 5 said method comprising:

inserting a probe into the patient;

advancing a plurality of electrodes from the probe so that the electrodes penetrate a collagenous tissue structure comprising a bladder neck; and 10

applying electrical energy to the collagenous tissue structure with the electrodes to heat the collagenous tissue structure sufficiently to effect shrinkage of the collagenous tissue structure so that the collagenous tissue structure inhibits urinary incontinence. 15

20. A method as in claim 19, wherein the energy is applied as a bipolar RF energy transmitted between the electrodes.

21. A method as in claim 19, wherein an axis of the probe extends from the proximal end to the distal end with the electrodes extending asymmetrically relative to the axis, wherein two electrodes deploy from the probe to penetrate the collagenous tissue structure on a first lateral side of the probe, and wherein two electrodes deploy from the probe to penetrate the collagenous tissue structure on a second lateral side of the probe. 20

22. A method as in claim 19, wherein the collagenous tissue structure further comprises at least one member selected from the group consisting of a urethral wall, a bladder, a ureter, bladder suspension ligaments, a sphincter, pelvic ligaments, pelvic floor muscles, and fascia. 25

23. A method as in claim 19, further comprising adjusting a power level of the energy, wherein the adjusting step is performed in response to internal temperature in the collagenous tissue structure.

24. A method for treating incontinence in a patient, said 35 method comprising:

26

inserting a probe into a urethra of the patient;

electrically coupling at least one electrode of the inserted probe to a collagenous tissue structure;

applying electrical energy to the collagenous tissue structure with the at least one electrode to heat the collagenous tissue structure, wherein the shrinkage provides a kink or closure point along the urethra to inhibit leakage; and

controlling an amount of the energy applied in response to a temperature of the collagenous tissue structure so that the collagenous tissue structure inhibits incontinence.

25. A method as in claim 24, wherein the energy is applied so as to cause bulking and buttressing of the collagenous tissue structure during healing.

26. A method as in claim 24, wherein the energy is applied so as to effect shrinkage of the collagenous tissue structure, the shrinkage and tissue bulking/buttressing acting to enhance patient continence.

27. A method for treating urinary incontinence in a patient, said method comprising:

inserting a probe into the patient;

engaging a plurality of electrodes of the probe against a bladder neck; and

applying sufficient electrical energy to the bladder neck so as to inhibit the urinary incontinence. 25

28. The method of claim 27, further comprising advancing the electrodes from the probe so that the electrodes penetrate into the bladder neck.

29. The method of claim 27, further comprising inserting the probe through the urethra. 30

30. The method of claim 29, further comprising controlling an amount of the energy in response to a temperature of the bladder neck.

* * * * *

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : 7,483,755 B2
APPLICATION NO. : 10/463976
DATED : January 27, 2009
INVENTOR(S) : Frank Ingle

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:


Title Page

Please insert Section:

-- (73) Assignee: AMS Research Corporation, Minnetonka, Minnesota --

Signed and Sealed this

Twenty-eighth Day of July, 2009

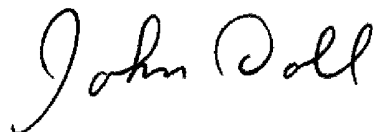A handwritten signature in black ink that reads "John Doll". The signature is written in a cursive style with a large, stylized "J" and "D".

JOHN DOLL
Acting Director of the United States Patent and Trademark Office

| | | | |
|----------------|---|---------|------------|
| 专利名称(译) | 用于收缩组织的装置，方法和系统 | | |
| 公开(公告)号 | US7483755 | 公开(公告)日 | 2009-01-27 |
| 申请号 | US10/463976 | 申请日 | 2003-06-17 |
| [标]申请(专利权)人(译) | 特拉华的SURX一个CORP | | |
| 申请(专利权)人(译) | SURX INC. | | |
| 当前申请(专利权)人(译) | AMS RES CORP | | |
| [标]发明人 | INGLE FRANK CARTER GARRY LAUFER MICHAEL D | | |
| 发明人 | INGLE, FRANK CARTER, GARRY LAUFER, MICHAEL D. | | |
| IPC分类号 | A61B5/01 A61N1/05 A61B18/00 A61B18/12 A61B18/14 A61N1/06 A61N1/40 | | |
| CPC分类号 | A61B18/1482 A61N1/06 A61N1/403 A61B18/14 A61B18/1477 A61B18/1492 A61B2018/00083 A61B2018/00095 A61B2018/00148 A61B2018/00214 A61B2018/00232 A61B2018/00505 A61B2018/ /00517 A61B2018/00523 A61B2018/00553 A61B2018/00559 A61B2018/00898 A61B2018/126 A61B2018/1425 A61B2018/1467 | | |
| 其他公开文献 | US20040034400A1 | | |
| 外部链接 | Espacenet USPTO | | |

摘要(译)

用于治疗尿失禁的装置，系统和方法通常依赖于递送至患者自身骨盆支撑组织的能量，以选择性地收缩或收缩该骨盆支撑组织的至少一部分，以便重新定位膀胱。优选将能量施加到骨盆内筋膜和/或肌腱筋膜骨盆。本发明提供了多种装置和方法，用于对这些和其它组织进行温和的电阻加热，使它们收缩而不会对周围的组织结构造成显著的伤害。或者，热量施加探针被配置为加热包括或支撑患者尿道的组织结构。通过在预定时间内施加足够的能量，可以将组织升高到导致收缩而没有显著坏死或其他组织损伤的温度。通过选择性地收缩支撑组织，可以减少尿液泄漏的方式重新配置或支撑膀胱颈，括约肌和负责控制尿流的泌尿道的其他组件。

