



US010028648B2

(12) **United States Patent**
Goldfain et al.

(10) **Patent No.:** **US 10,028,648 B2**
(45) **Date of Patent:** **Jul. 24, 2018**

(54) **BORESCOPIC OPTICAL SYSTEM FOR MEDICAL DIAGNOSTIC INSTRUMENTS AND MEDICAL DIAGNOSTIC INSTRUMENTS HAVING INTERLOCKING ASSEMBLY FEATURES**

(71) Applicant: **Welch Allyn, Inc.**, Skaneateles Falls, NY (US)

(72) Inventors: **Ervin Goldfain**, Syracuse, NY (US);
Raymond A. Lia, Auburn, NY (US)

(73) Assignee: **WELCH ALLYN, INC.**, Skaneateles Falls, NY (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) Appl. No.: **15/493,500**

(22) Filed: **Apr. 21, 2017**

(65) **Prior Publication Data**

US 2017/0215719 A1 Aug. 3, 2017

Related U.S. Application Data

(63) Continuation of application No. 14/853,282, filed on Sep. 14, 2015, now Pat. No. 9,675,246.

(60) Provisional application No. 62/071,128, filed on Sep. 15, 2014.

(51) **Int. Cl.**

A61B 3/10 (2006.01)
A61B 1/227 (2006.01)
A61B 1/06 (2006.01)
A61B 3/12 (2006.01)
A61B 3/00 (2006.01)

(52) **U.S. Cl.**

CPC **A61B 1/227** (2013.01); **A61B 1/06** (2013.01); **A61B 3/0008** (2013.01); **A61B 3/1208** (2013.01)

(58) **Field of Classification Search**

CPC A61B 3/0008; A61B 3/14; A61B 3/12;
A61B 3/102; A61B 3/0025
USPC 351/200-246
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,586,424 A 6/1971 Schenk et al.
3,698,387 A 10/1972 Moore et al.

(Continued)

FOREIGN PATENT DOCUMENTS

WO WO 2005/020804 A1 3/2005
WO WO 2005/044098 A1 5/2005

OTHER PUBLICATIONS

International Preliminary Report on Patentability and Written Opinion; dated Mar. 21, 2017; 8 pages.

(Continued)


Primary Examiner — Mohammed Hasan

(57) **ABSTRACT**

A medical diagnostic instrument or a plurality of disparate medical diagnostic instruments are configured with a common optical architecture that functionally creates a virtual eye to create closer proximity to a patient and therefore increase the field of view in regard to a target of interest. The optical system includes a distal optical element, at least one relay lens and an eyepiece lens in which the optical system can be integrated within at least one instrument or be provided using a releasable module. Additionally, at least one of a viewing assembly and illumination assembly of at least one medical diagnostic instrument can be assembled using a series of components that are connected by interlocking features.

19 Claims, 38 Drawing Sheets

400

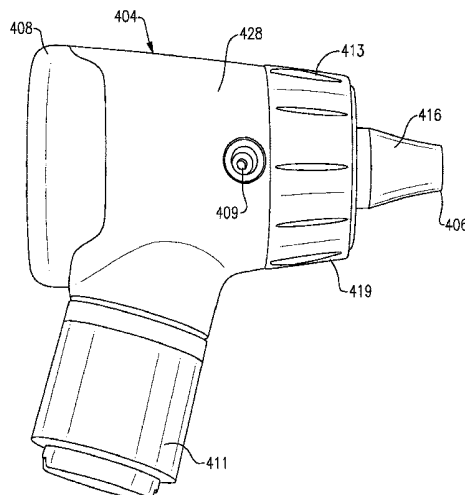

(56)

References Cited

U.S. PATENT DOCUMENTS

3,914,032 A 10/1975 Takano A61B 3/14
351/205

3,978,850 A 9/1976 Moore et al.

4,526,449 A 7/1985 Newman et al.

5,658,235 A 8/1997 Priest et al.

7,364,297 B2 4/2008 Goldfain et al.

7,399,275 B2 * 7/2008 Goldfain A61B 1/00188
600/112

8,066,634 B2 11/2011 Andreassen et al.

8,197,403 B2 6/2012 Strom et al.

8,602,971 B2 12/2013 Farr

9,445,713 B2 * 9/2016 Douglas A61B 1/00009

2005/0110949 A1 5/2005 Goldfain et al.

2008/0309876 A1 12/2008 Massie A61B 3/12
351/219

2010/0081875 A1 4/2010 Fowler et al.

2010/0317924 A1 12/2010 Sisko et al.

2012/0209074 A1 8/2012 Titus

2012/0320340 A1 12/2012 Coleman, III

2013/0178707 A1 7/2013 Kwong

2013/0208241 A1 8/2013 Lawson et al.

2013/0267783 A1 * 10/2013 Davis A61B 1/00188
600/200

2014/0146288 A1 5/2014 Anand A61B 3/0008
351/207



OTHER PUBLICATIONS



Large Field of View, Modular, Stabilized, Adaptive-Optics-Based Scanning Laser Ophthalmoscope; Stephen A. Burns, Remy Tumber and Ann E. Elsner; <http://www.ncbi.nlm.nih.gov/pmc/articles/PMC2443858/pdf/nihms21600>; Published in May 2007; 24 pages.


Adaptive Optics Scanning Laser Ophthalmoscope With Integrated Wide-Field Retinal Imaging and Tracking; R. Daniel Ferguson, Zhangyi Zhong, Daniel X. Hammer, Mircea Mujat, Ankit H. Patel, Cong Deng, Welyao Zou and Stephen A. Burns; <http://www.ncbi.nlm.nih.gov/pmc/articles/PMC3071649/pdf/nihms-250025>; Published in Nov. 2010; 27 pages.

Invitation to Pay Additional Fees, and Where Applicable, Protest Fee: dated Dec. 2, 2015; 6 pages.

* cited by examiner

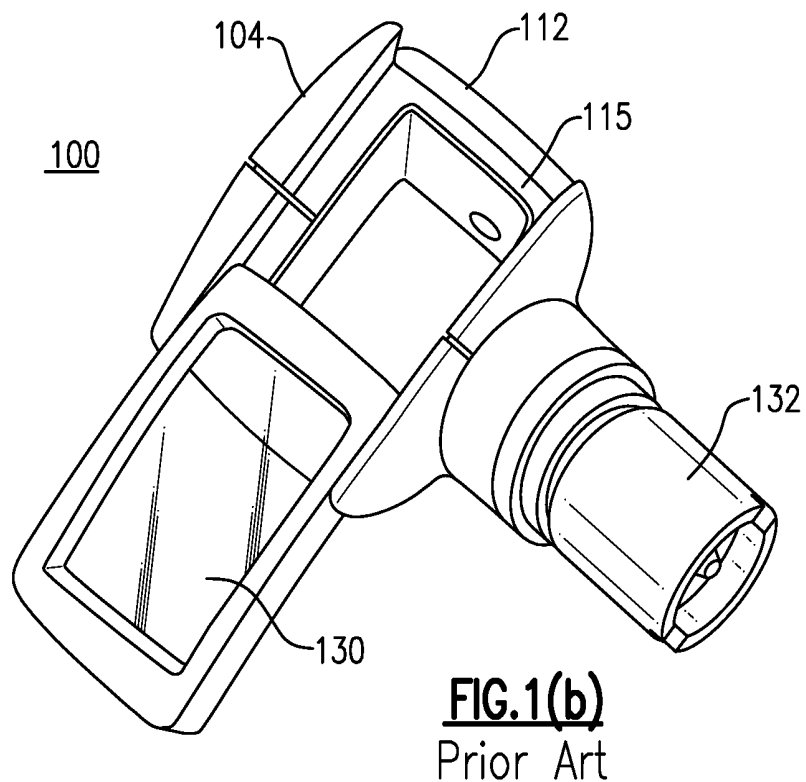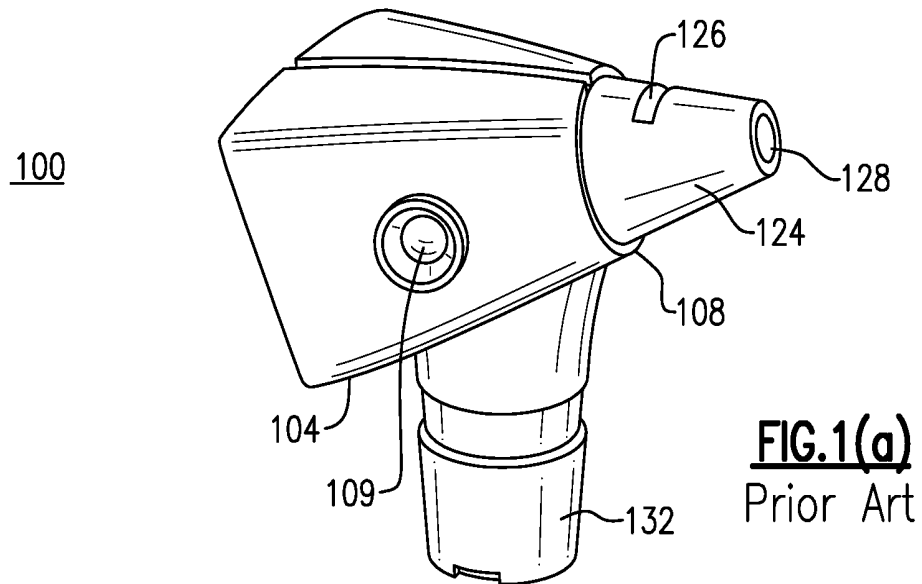

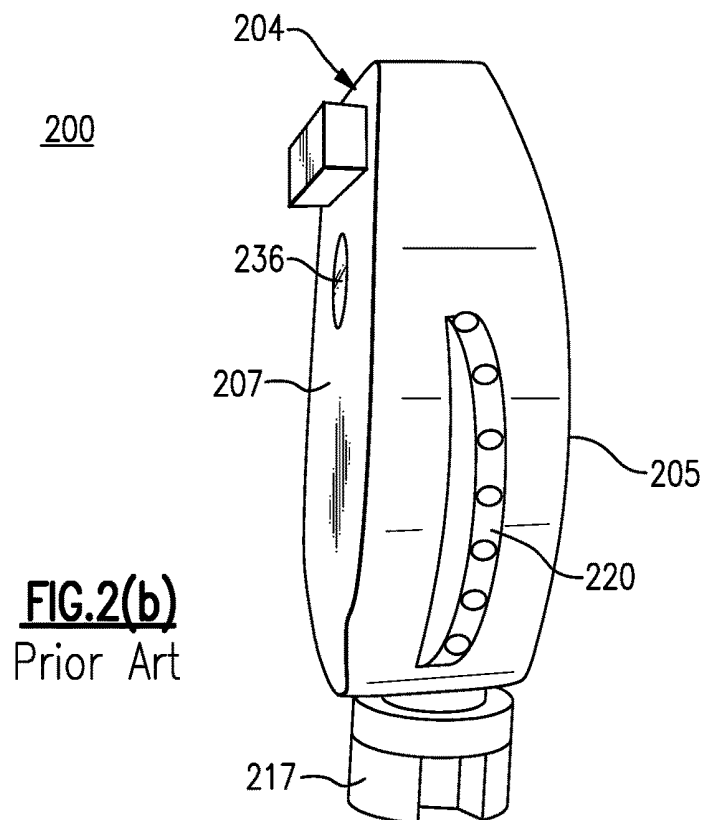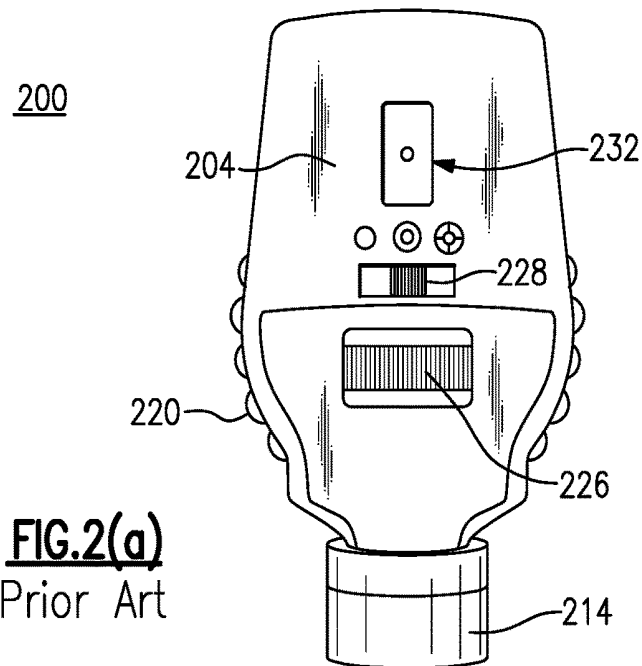

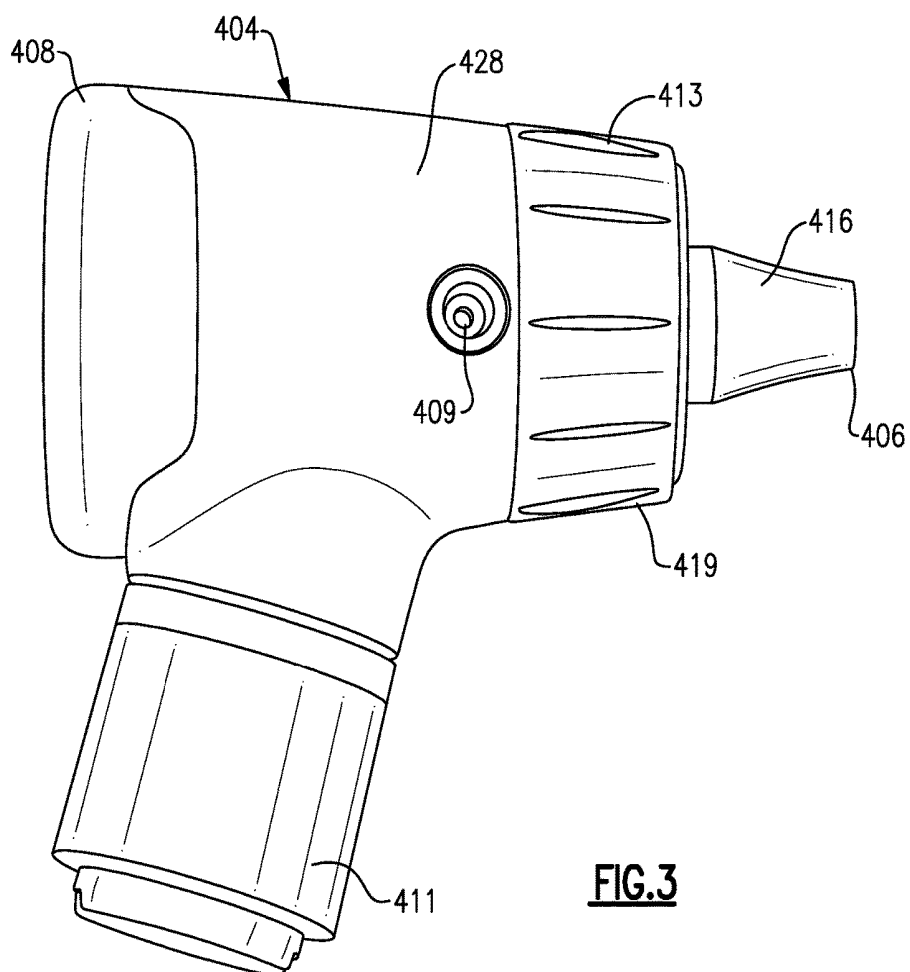400**FIG. 3**

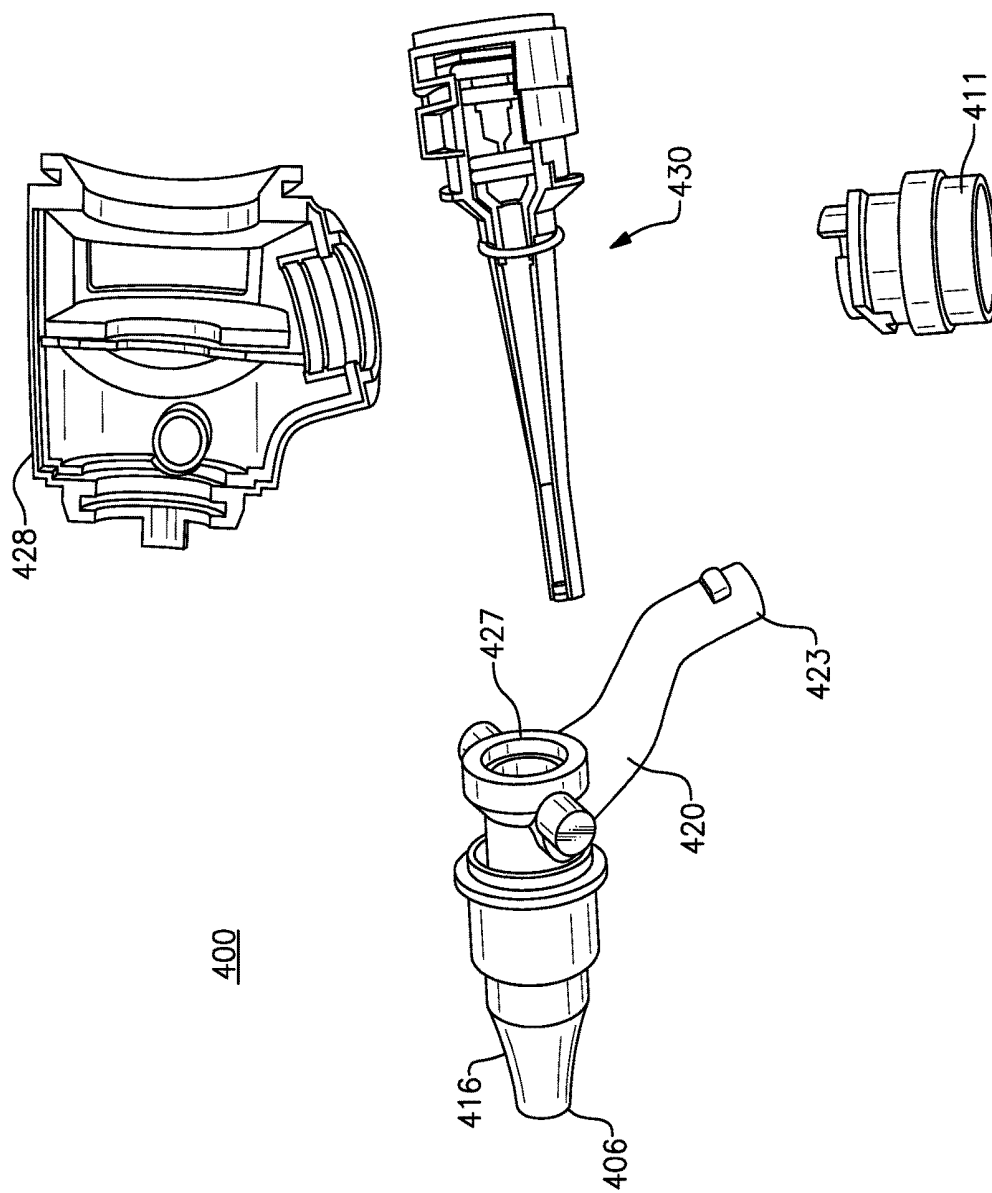


FIG. 4(a)

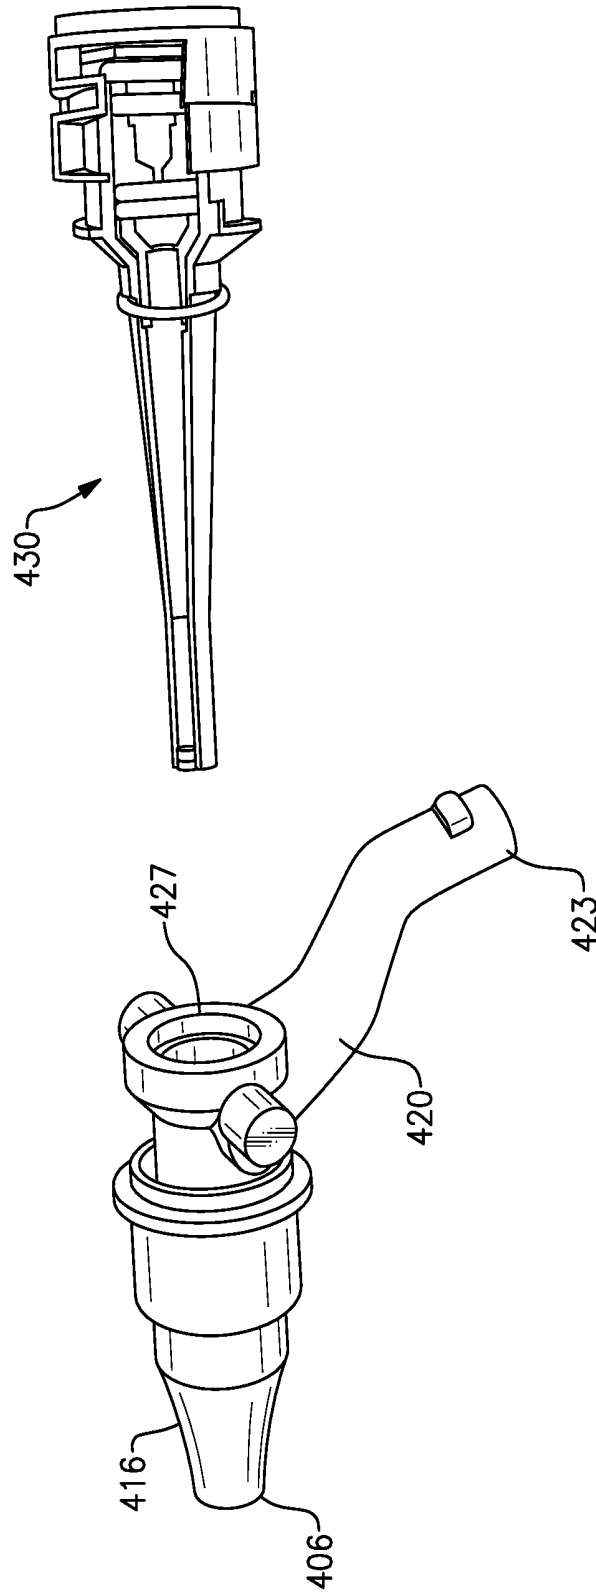
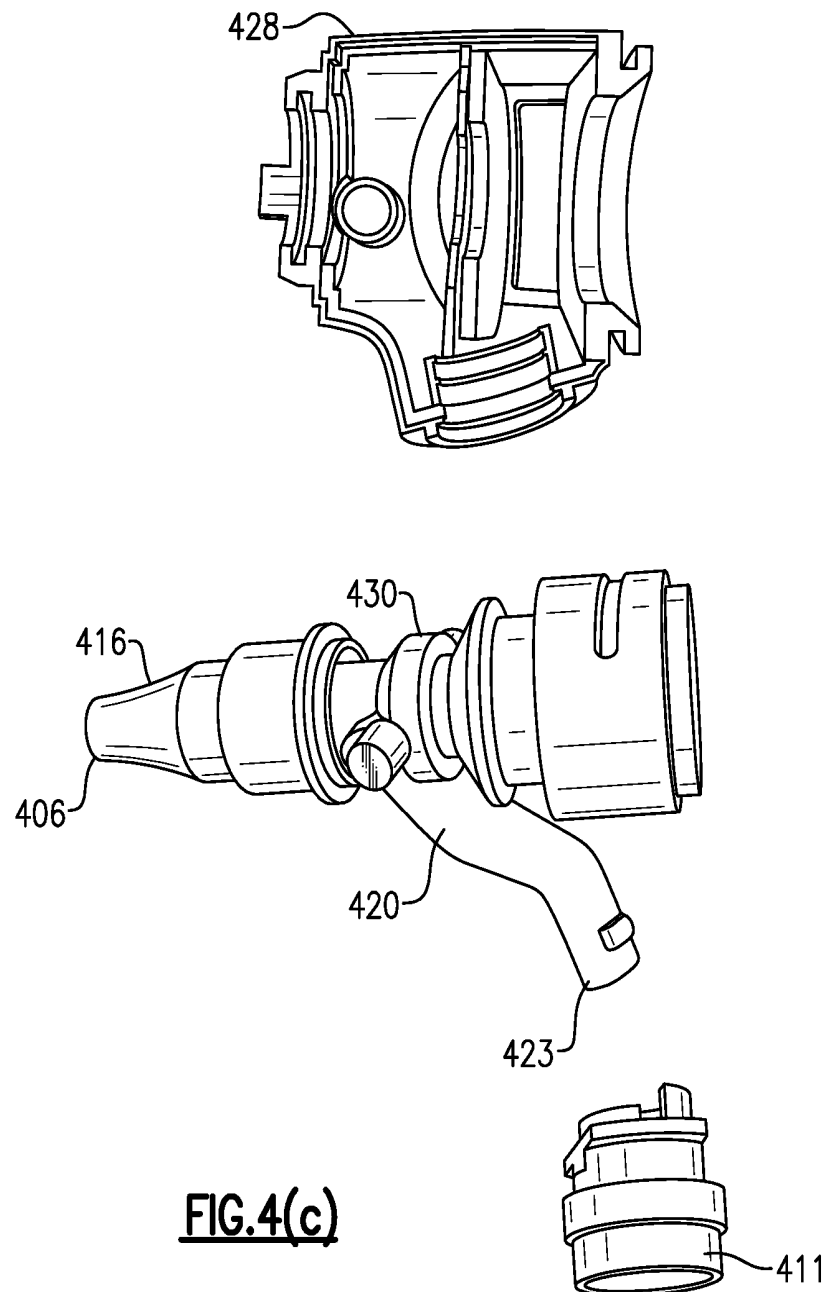
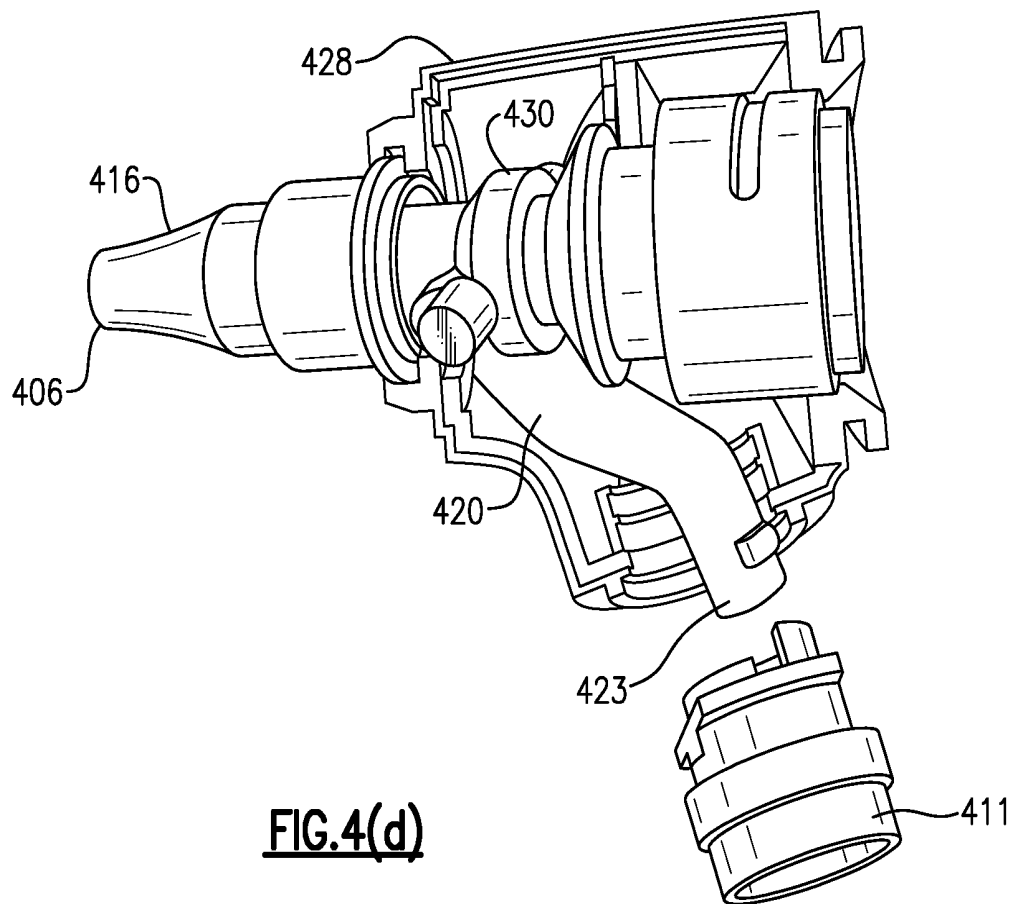


FIG. 4(b)





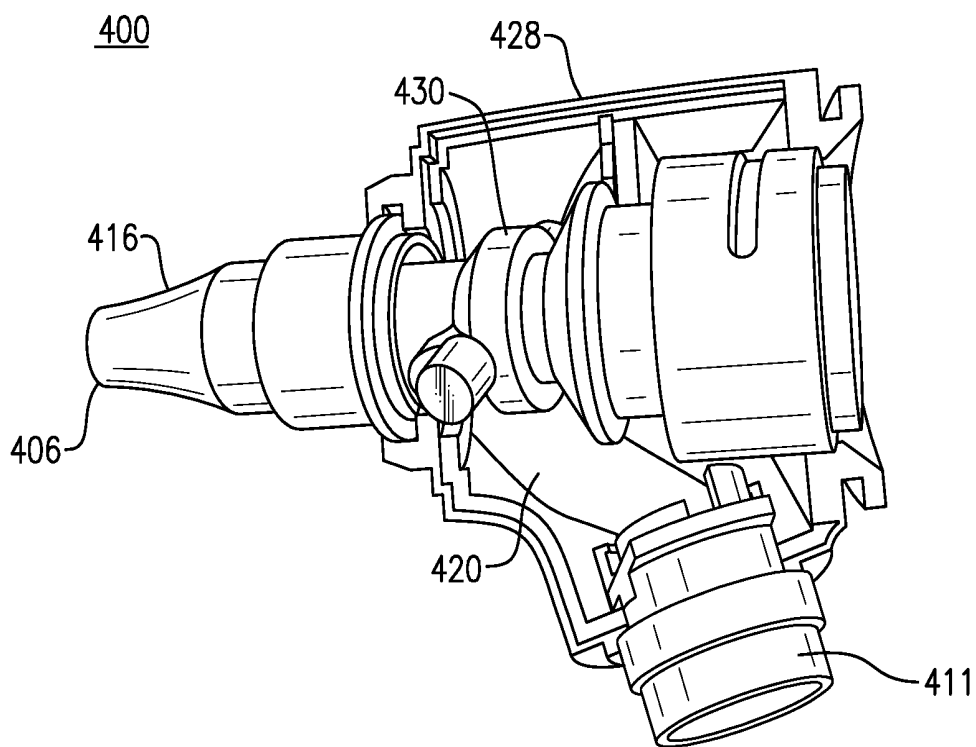


FIG. 4(e)

430

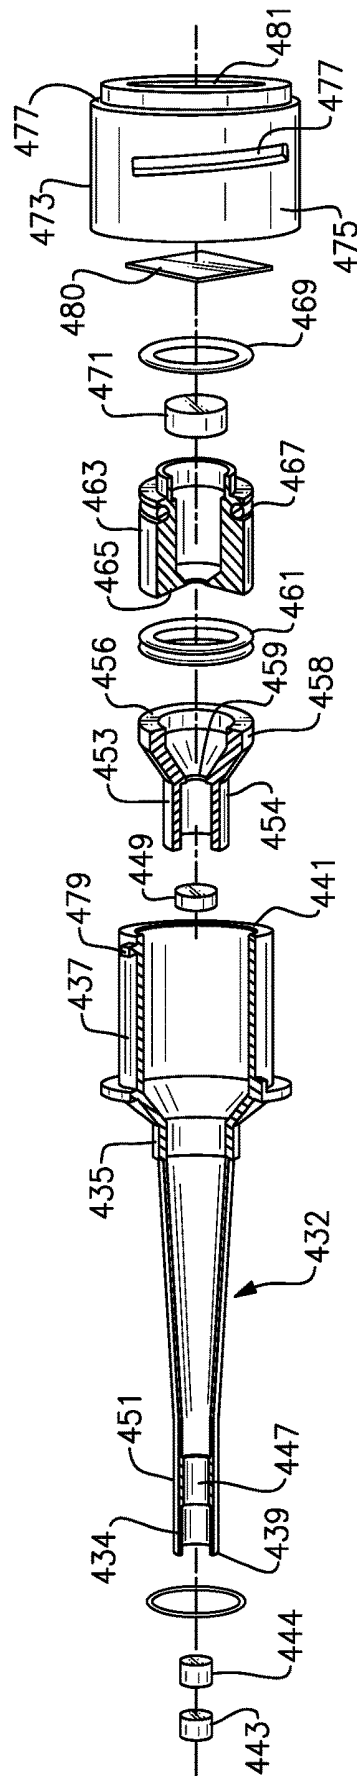


FIG. 4(f)

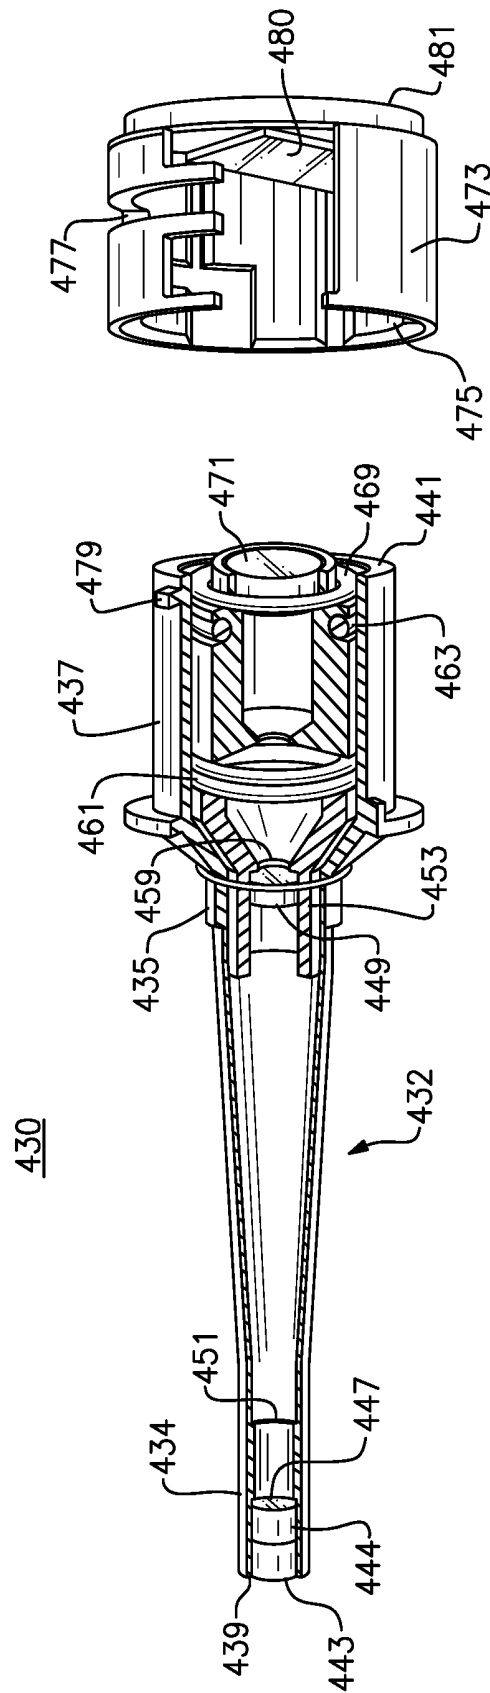


FIG. 4(g)

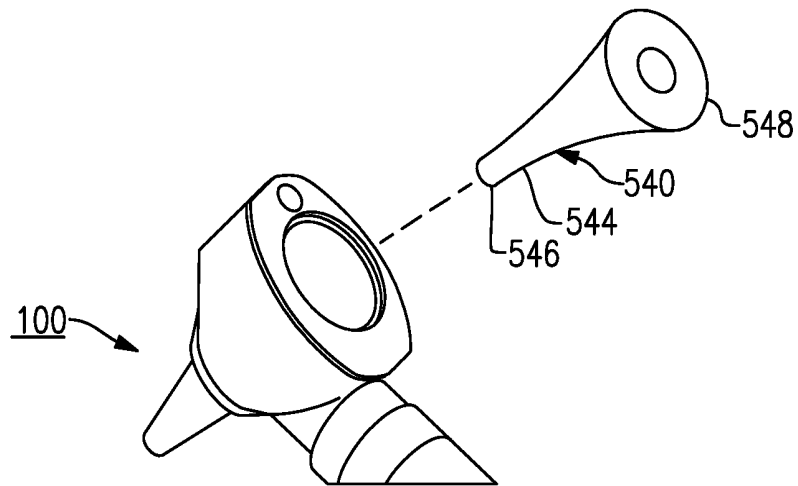


FIG. 5

600

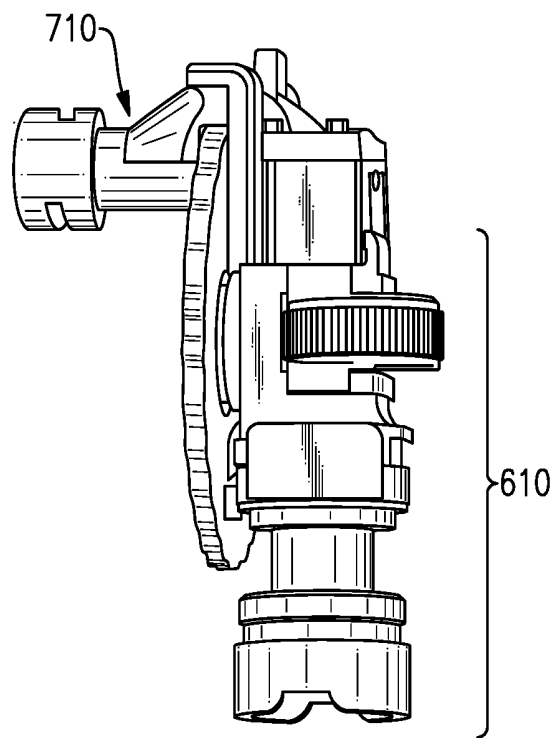


FIG.6

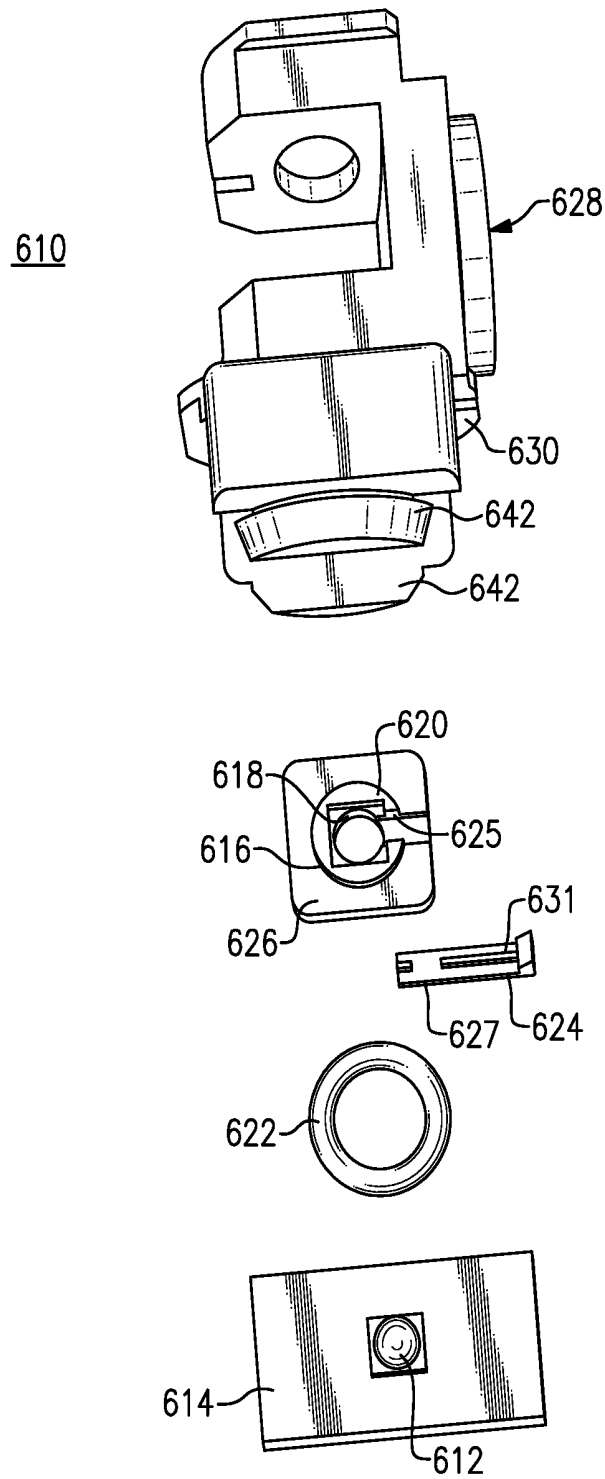
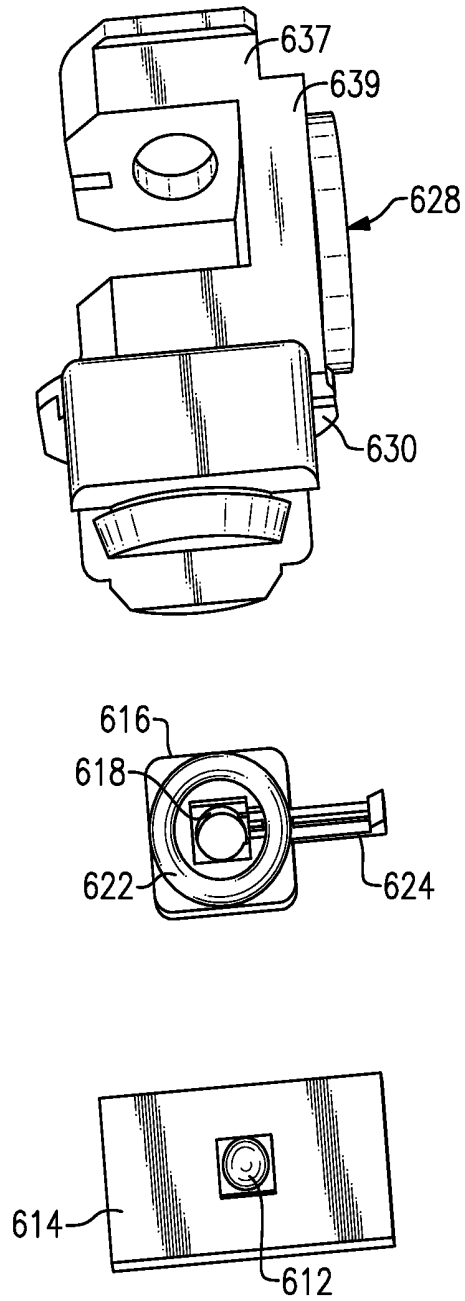


FIG.7(a)

**FIG. 7(b)**

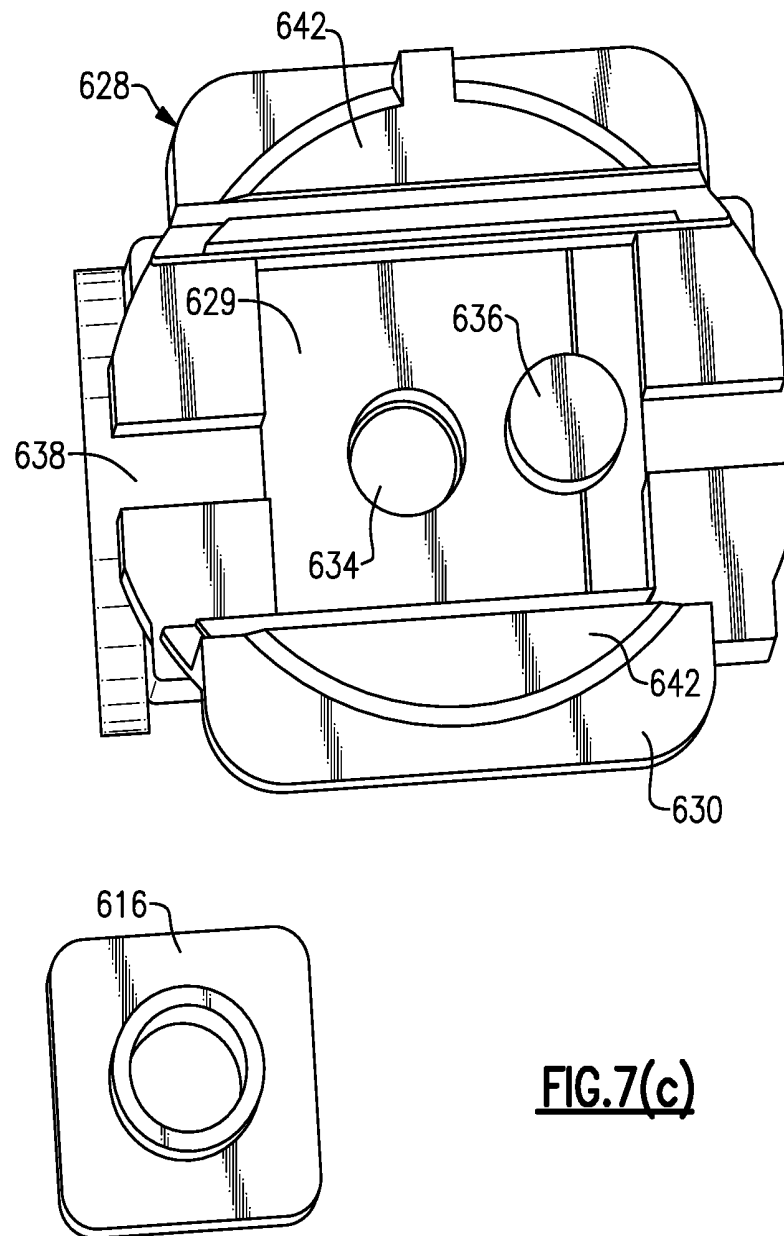


FIG. 7(c)

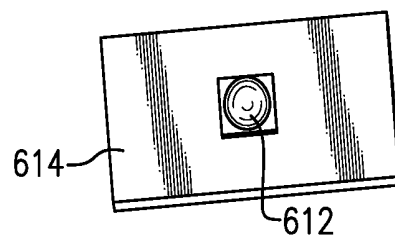
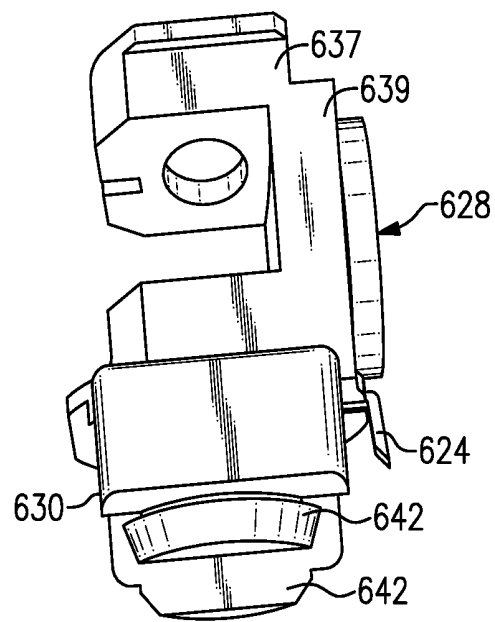


FIG. 7(d)

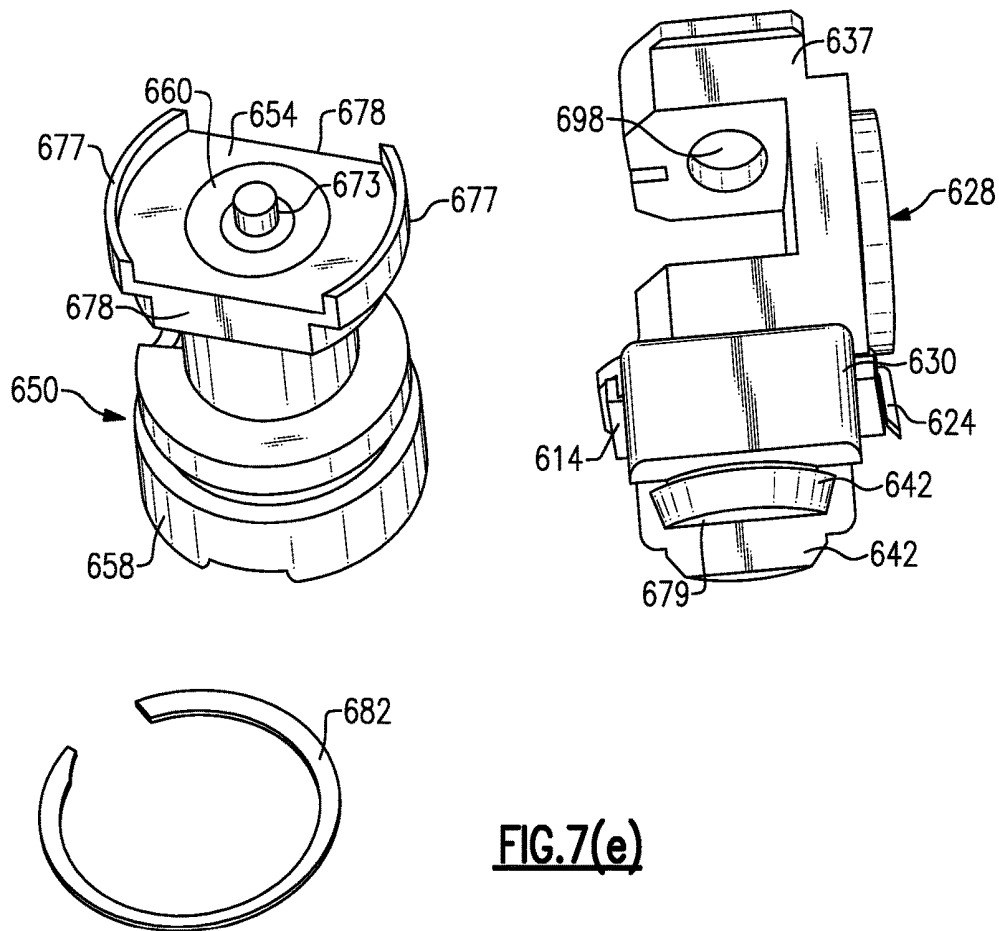
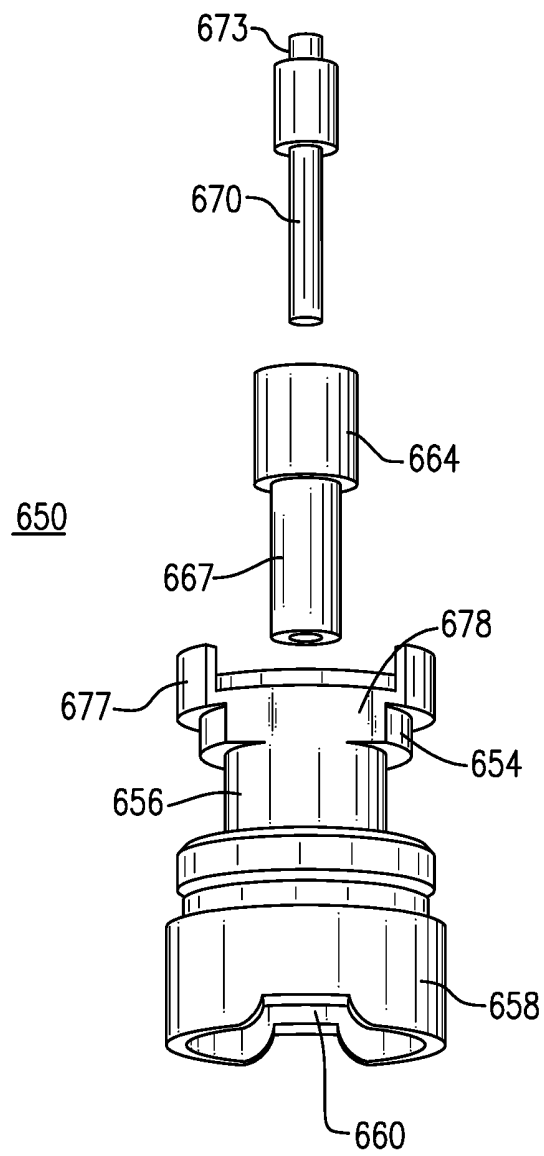


FIG. 7(e)

**FIG. 7(f)**

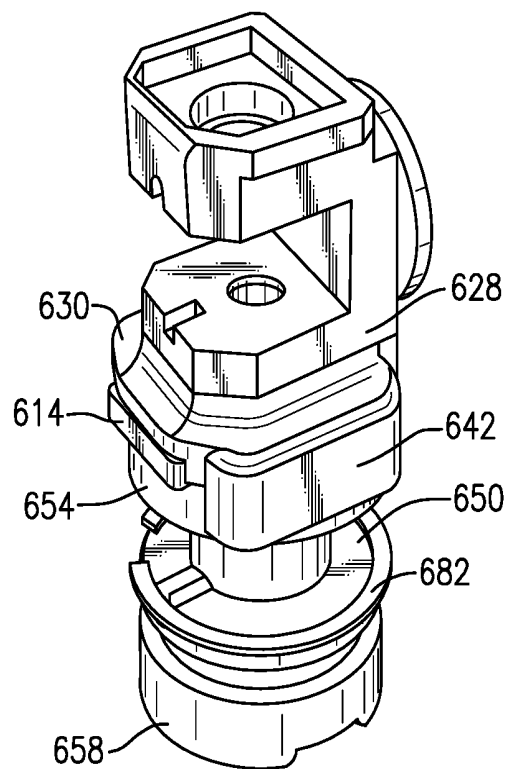


FIG. 7(q)

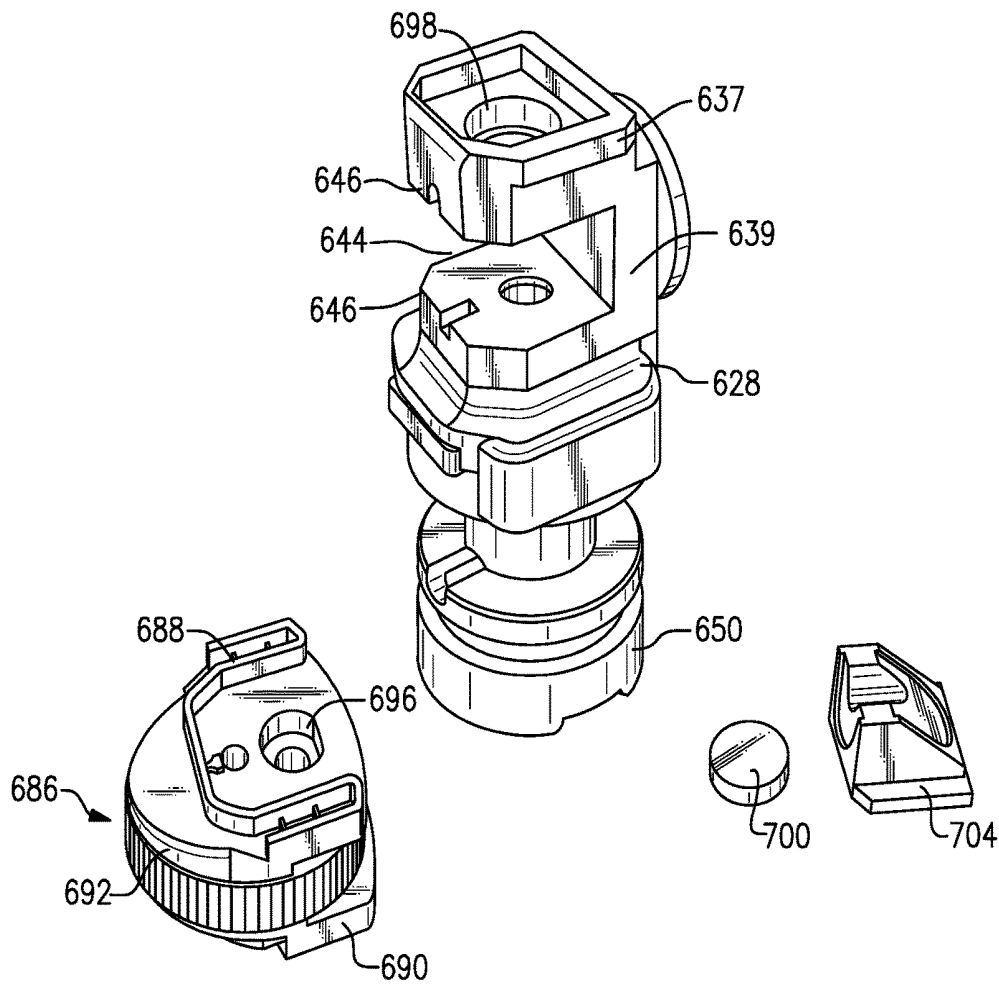


FIG.7(h)

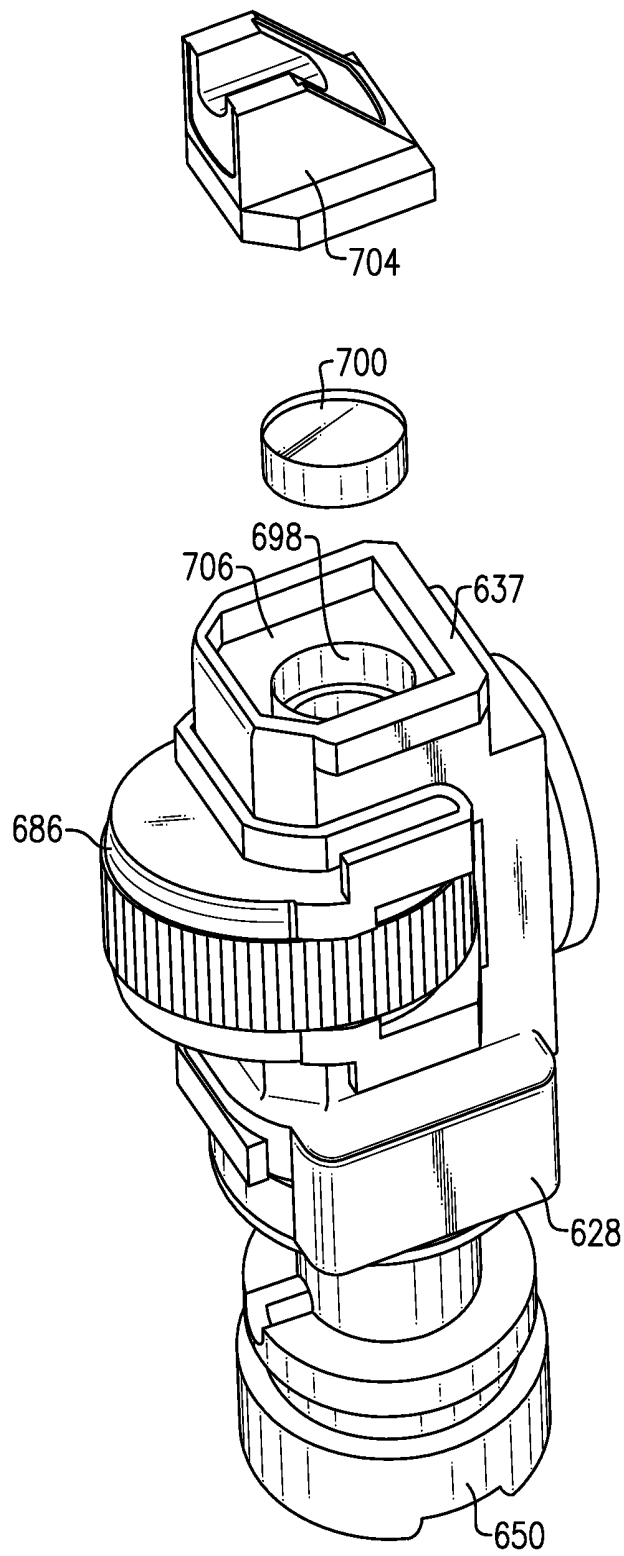
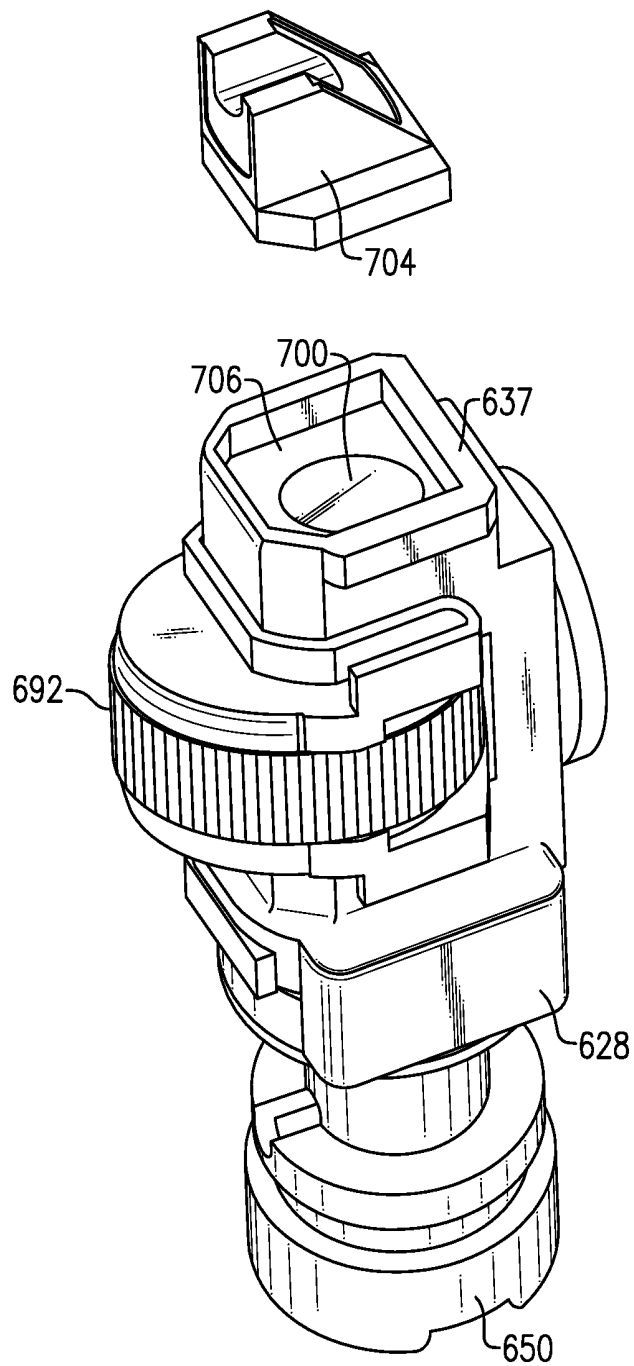


FIG. 7(i)

**FIG. 7(j)**

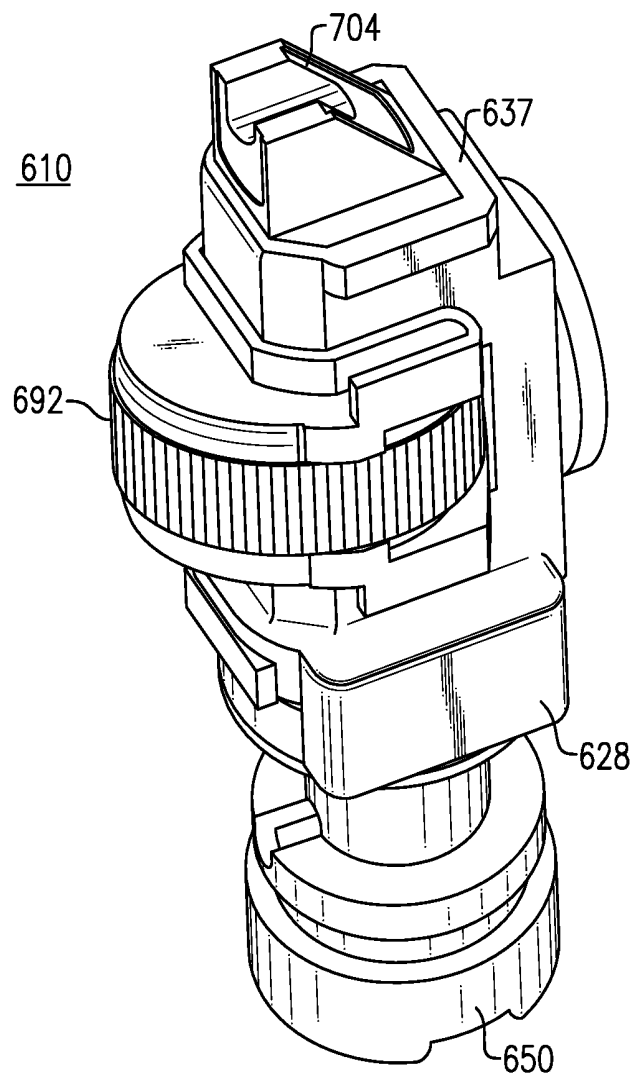


FIG. 7(k)

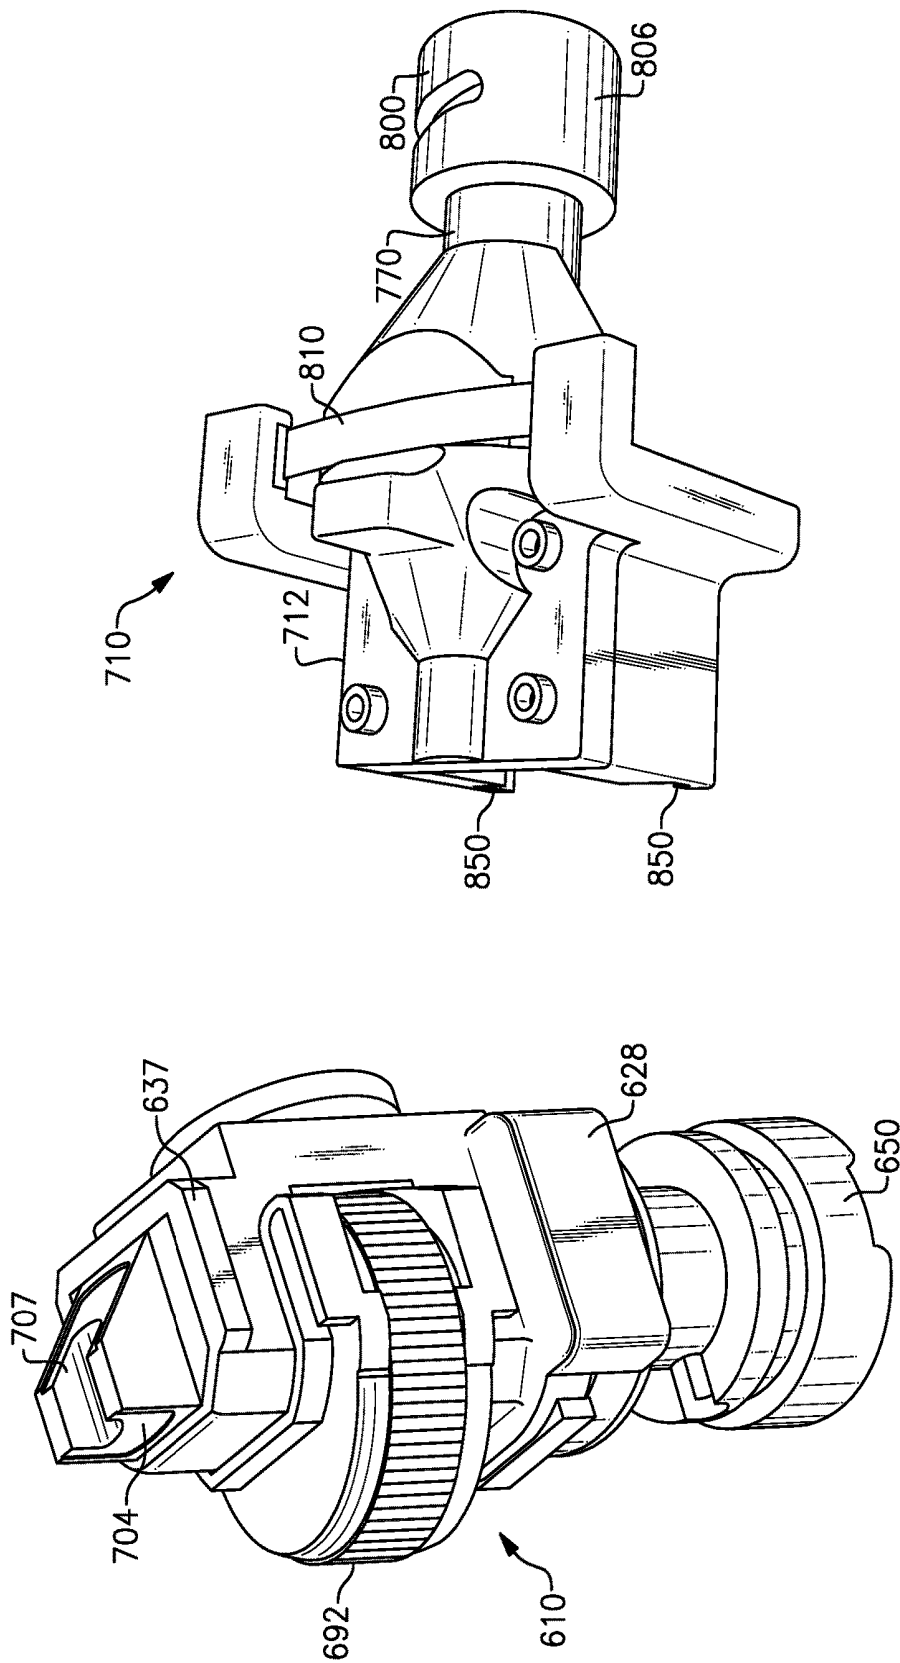


FIG. 8(a)

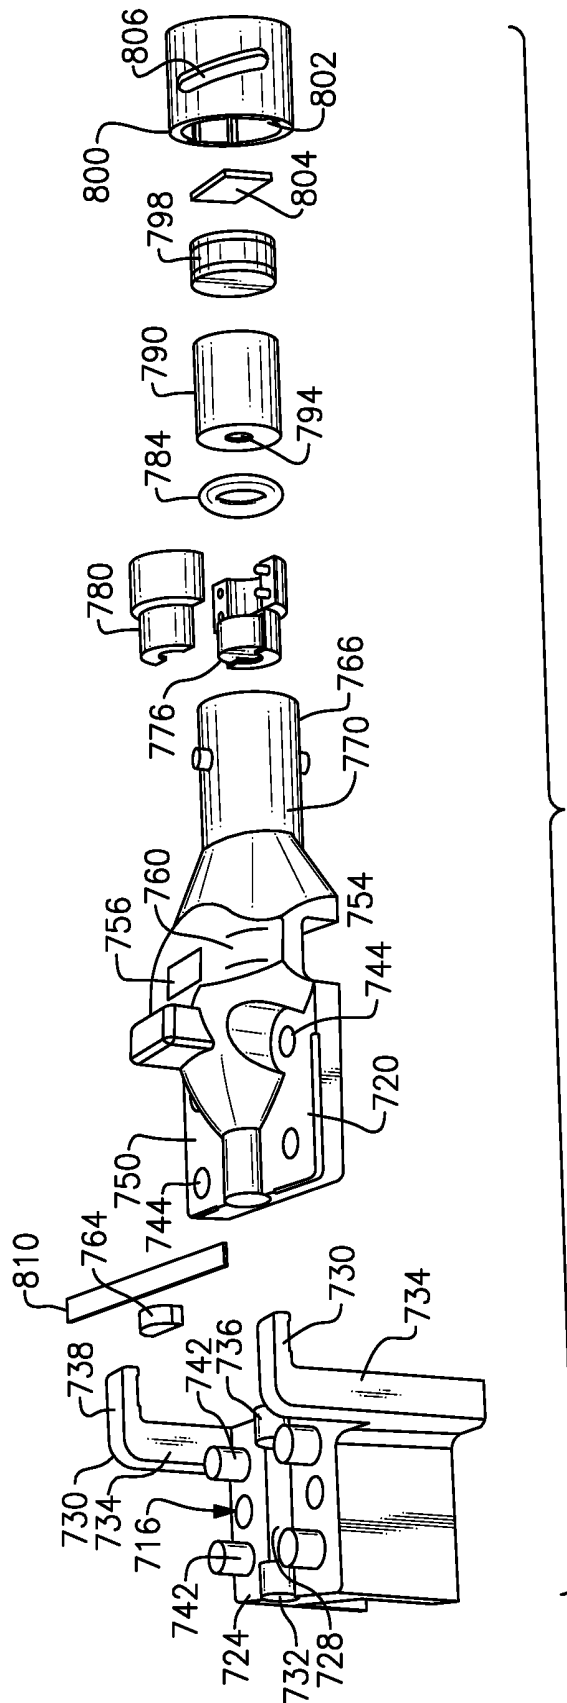


FIG. 8(b)

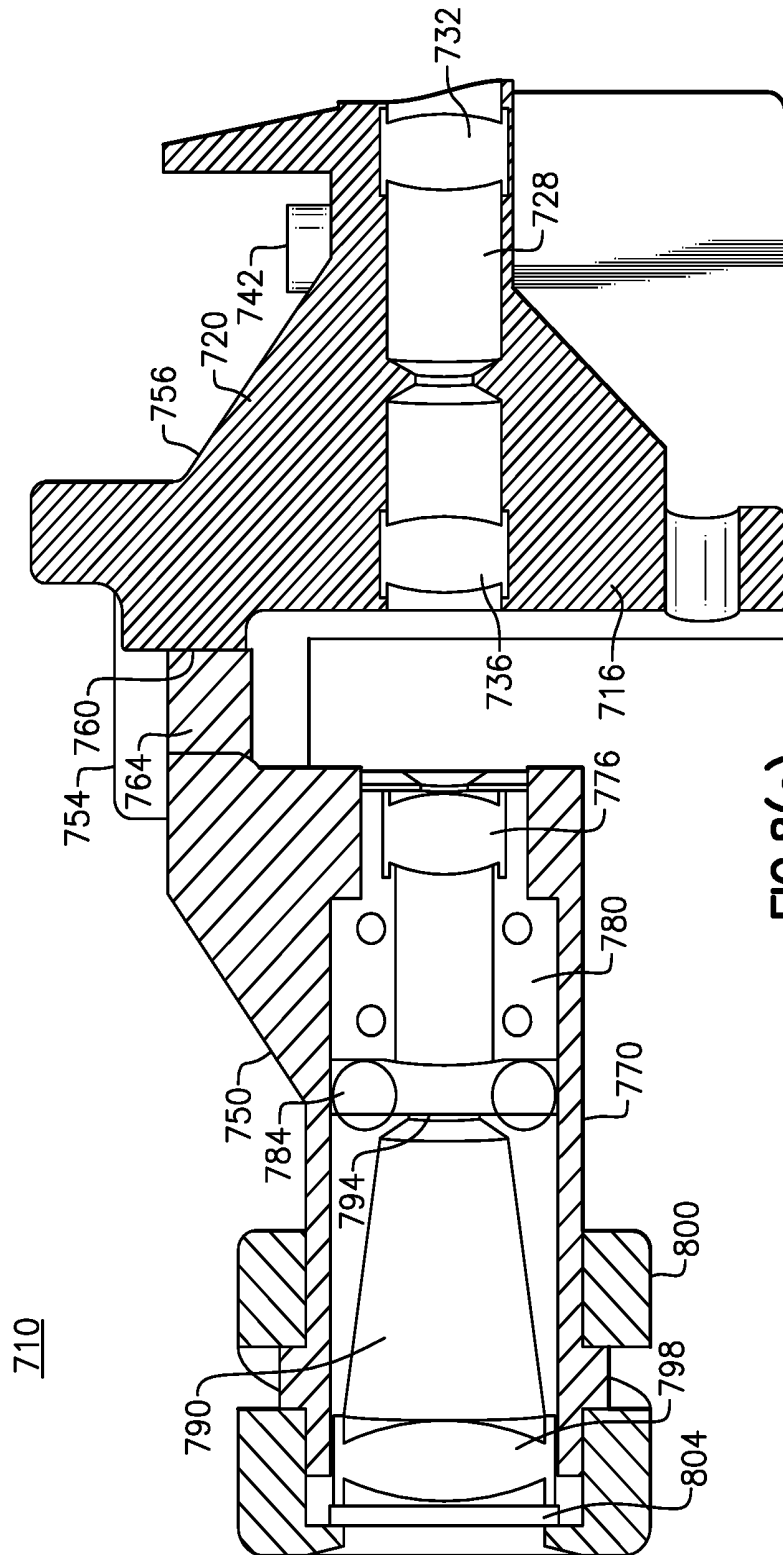
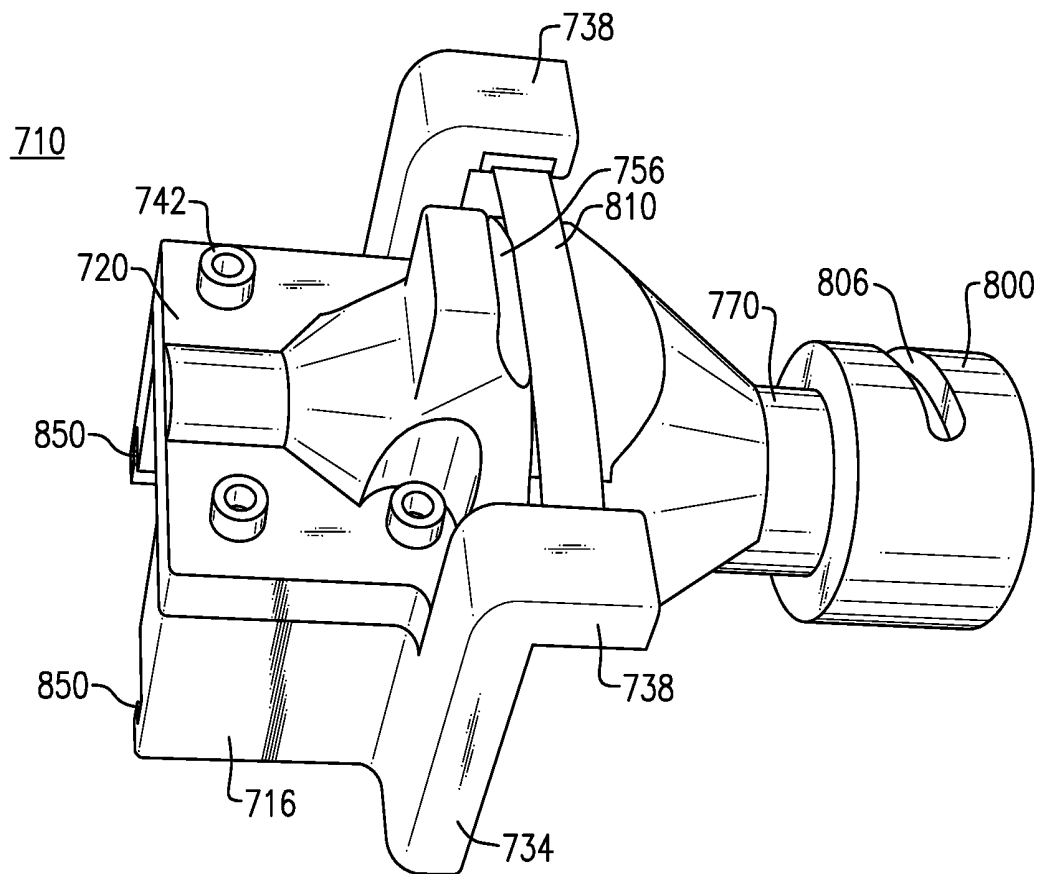


FIG. 8(c)

**FIG. 8(d)**

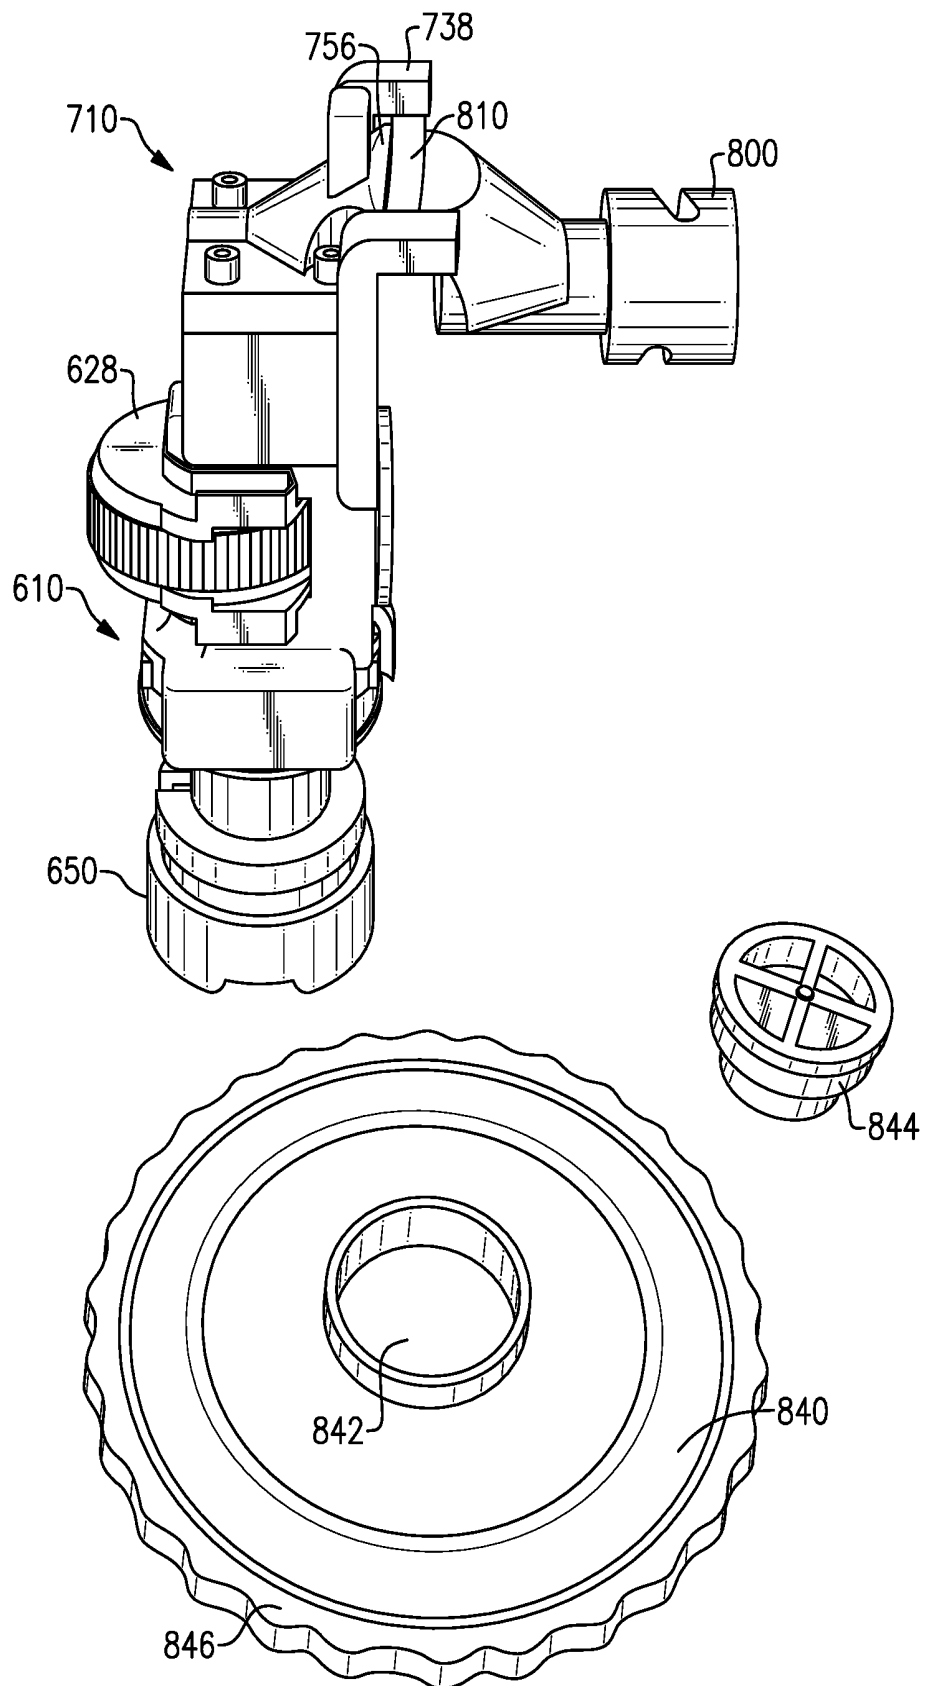
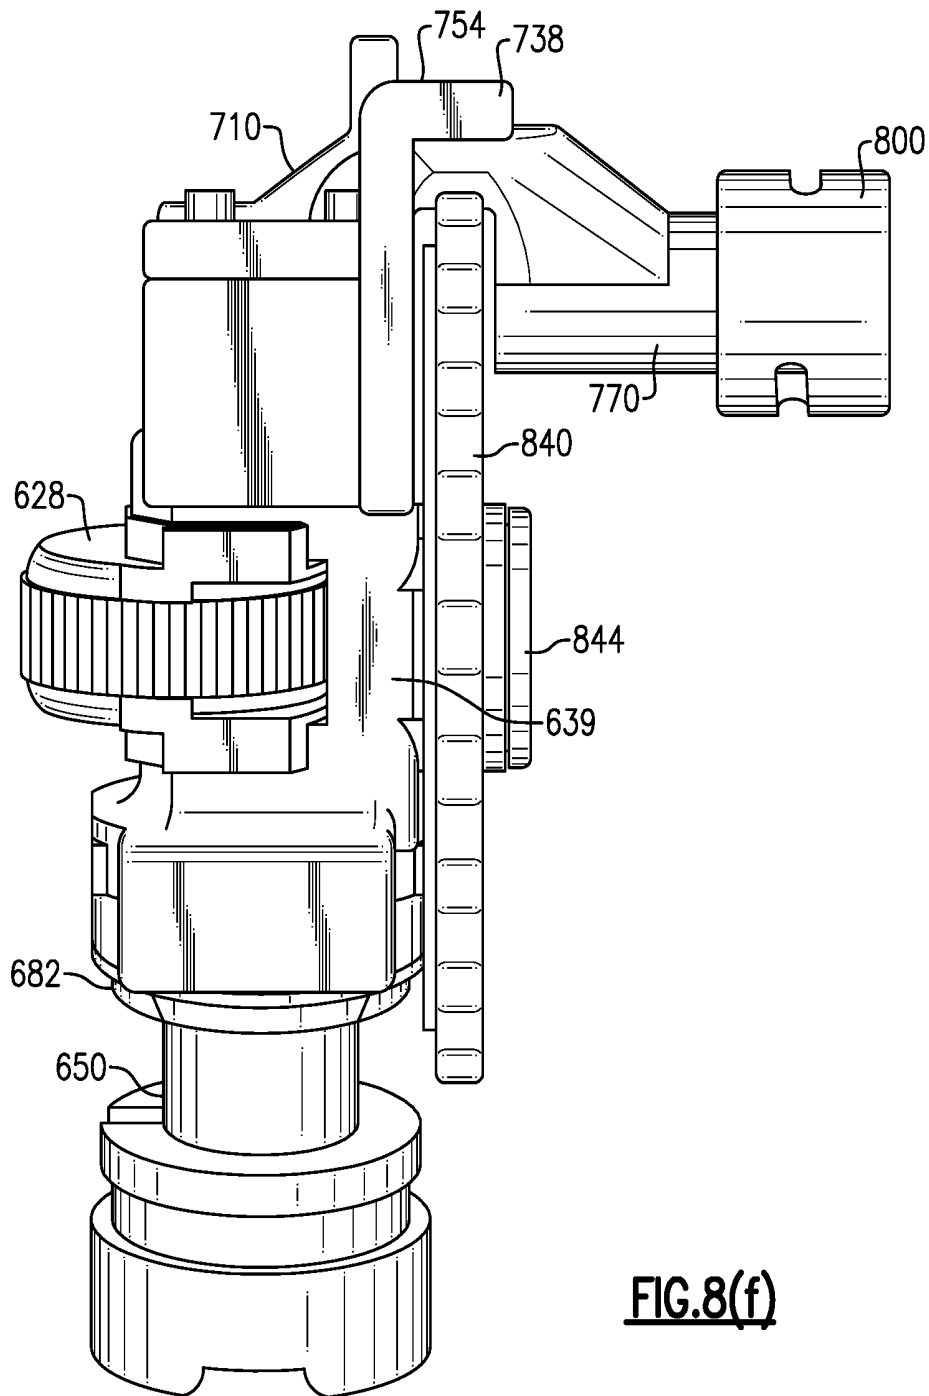
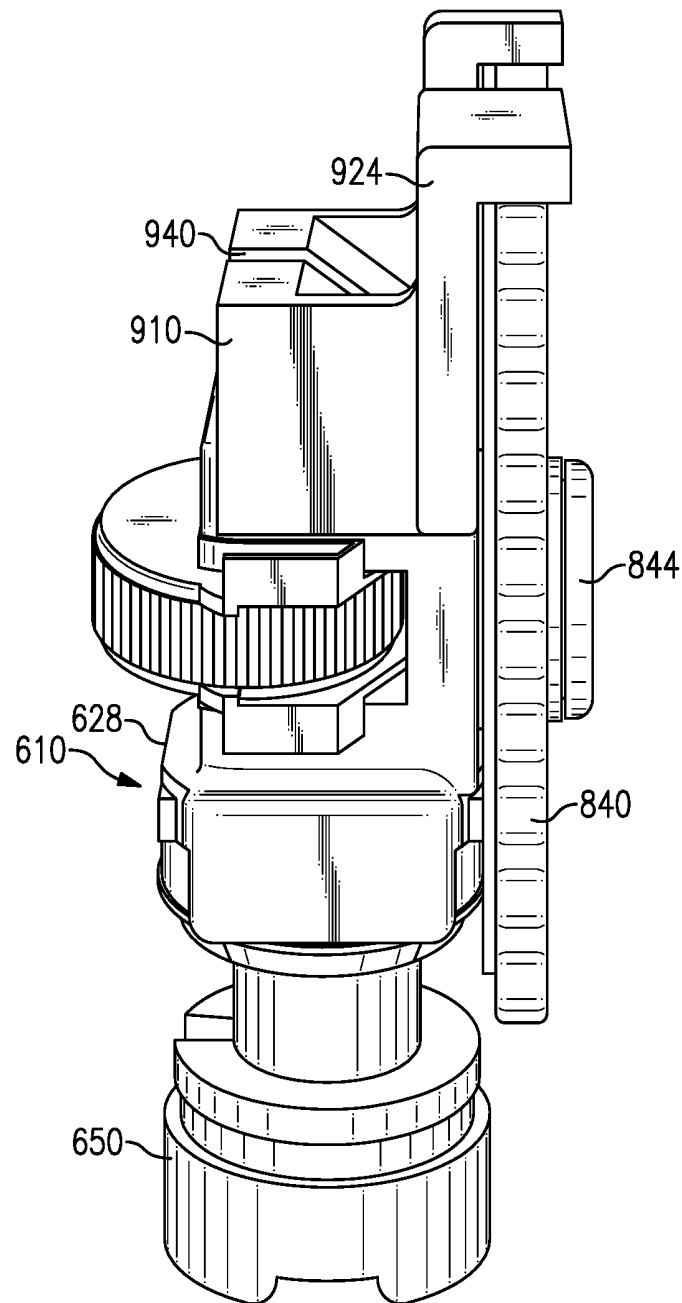


FIG. 8(e)

**FIG. 8(f)**

**FIG. 9(a)**

910

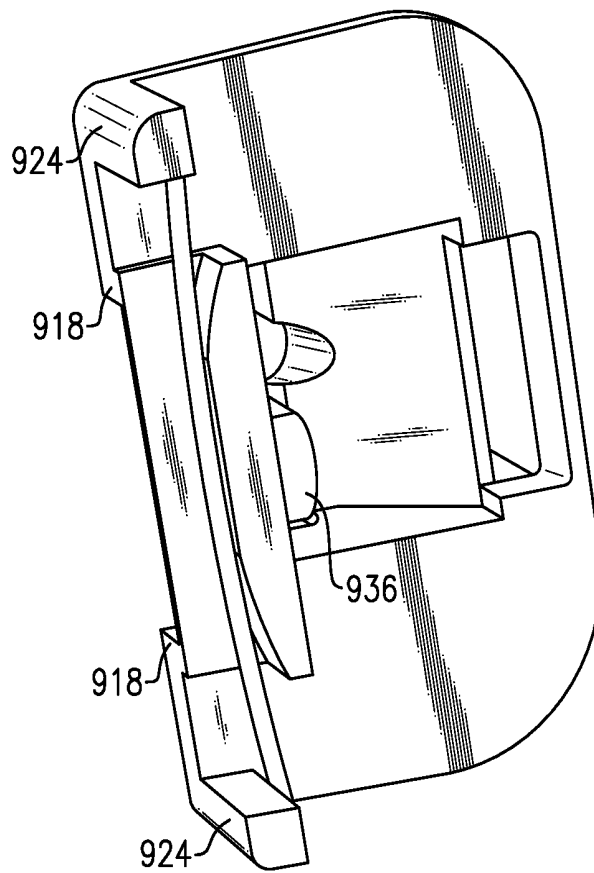
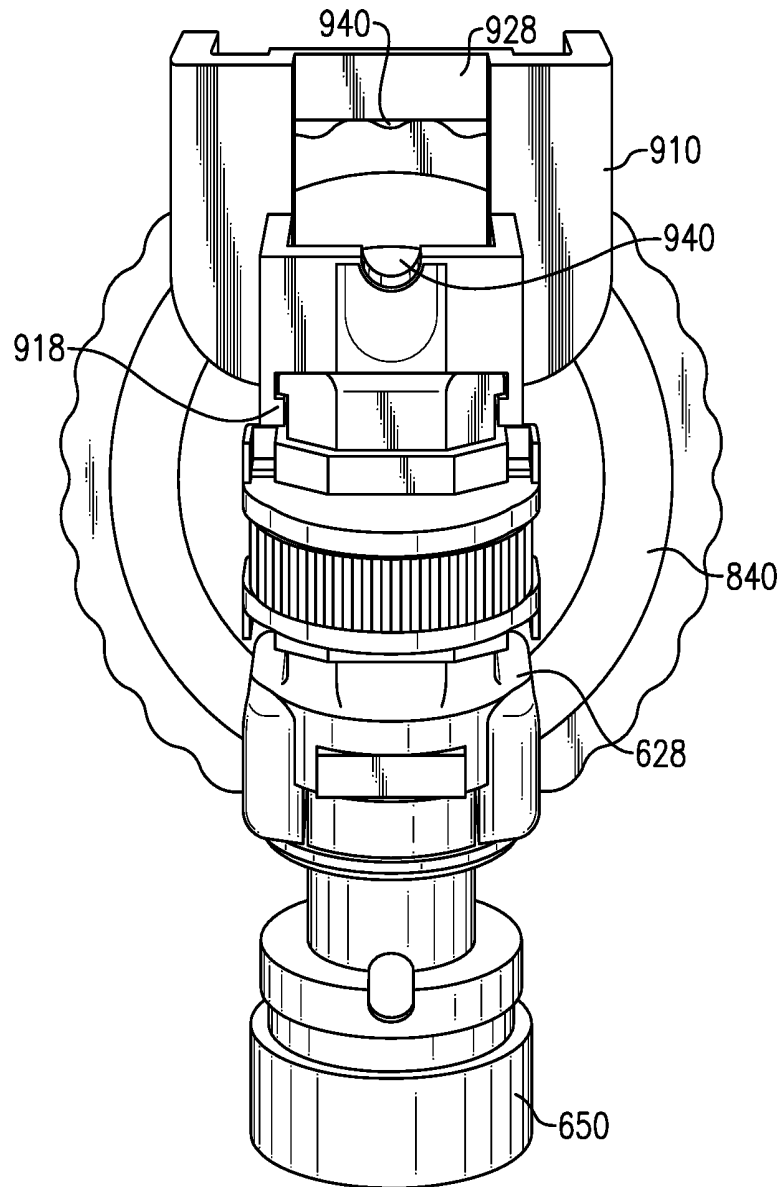
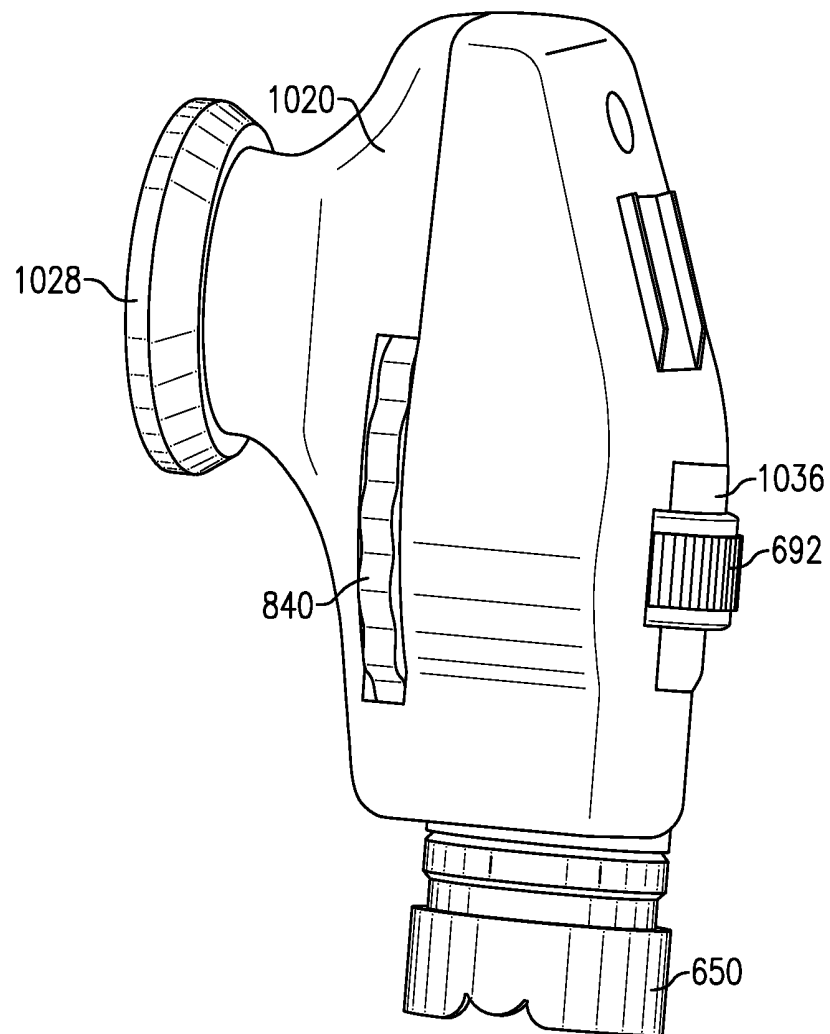
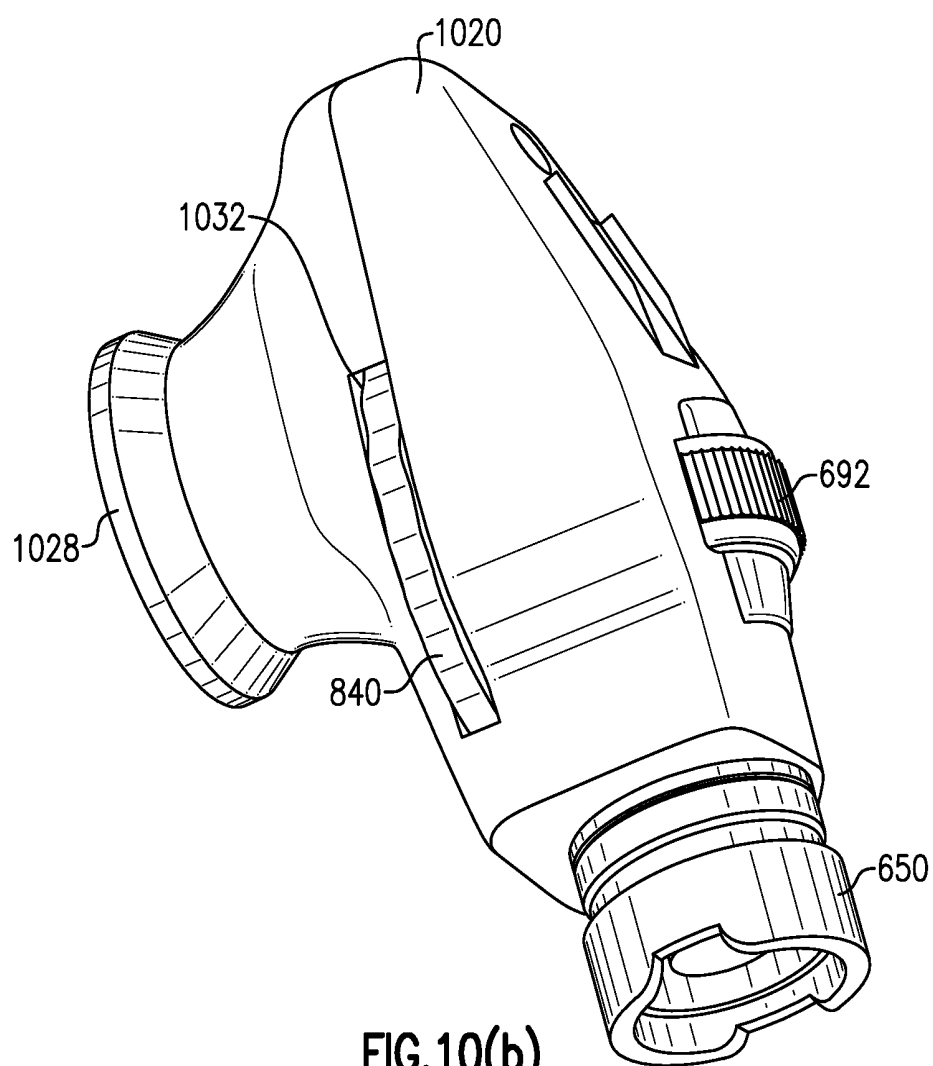
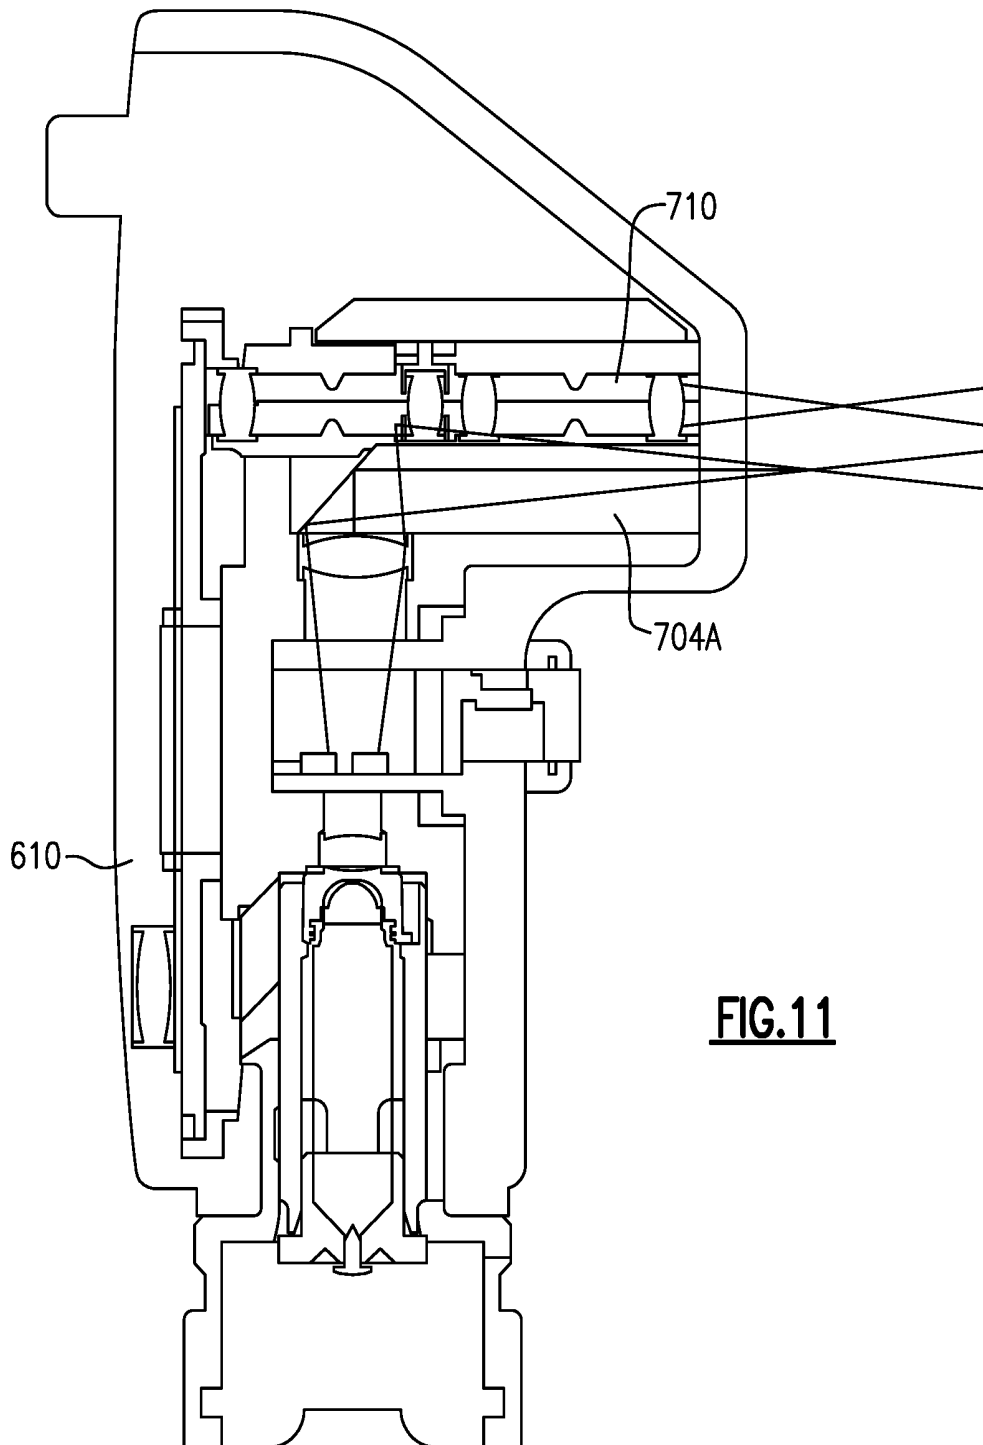


FIG.9(b)

**FIG. 9(c)**

1000FIG. 10(a)





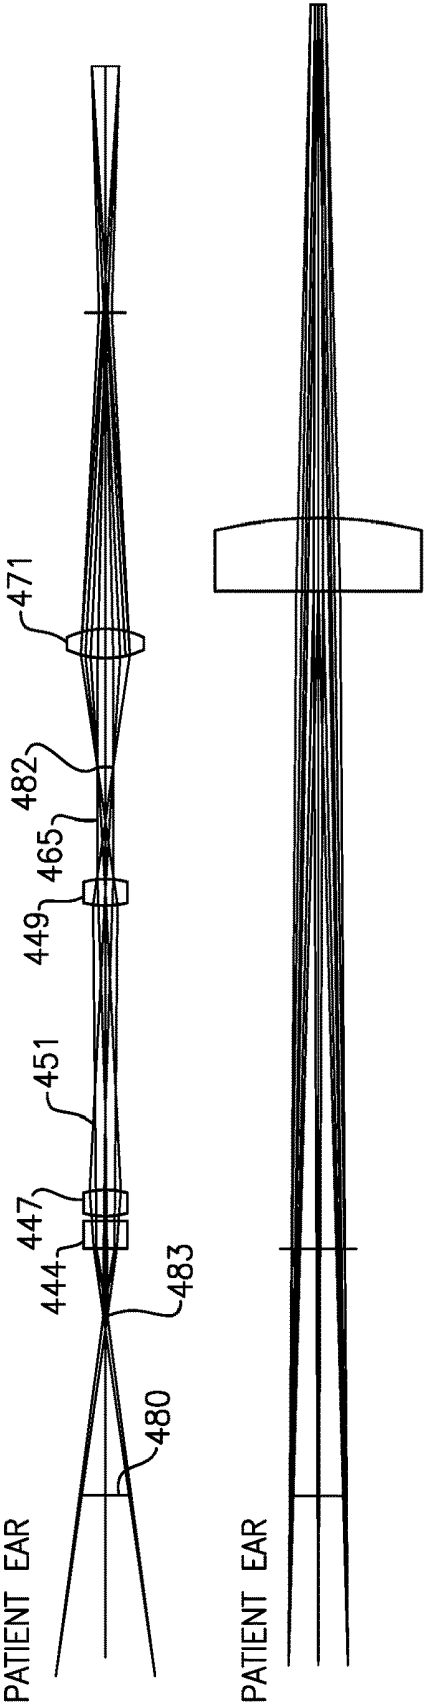


FIG.12

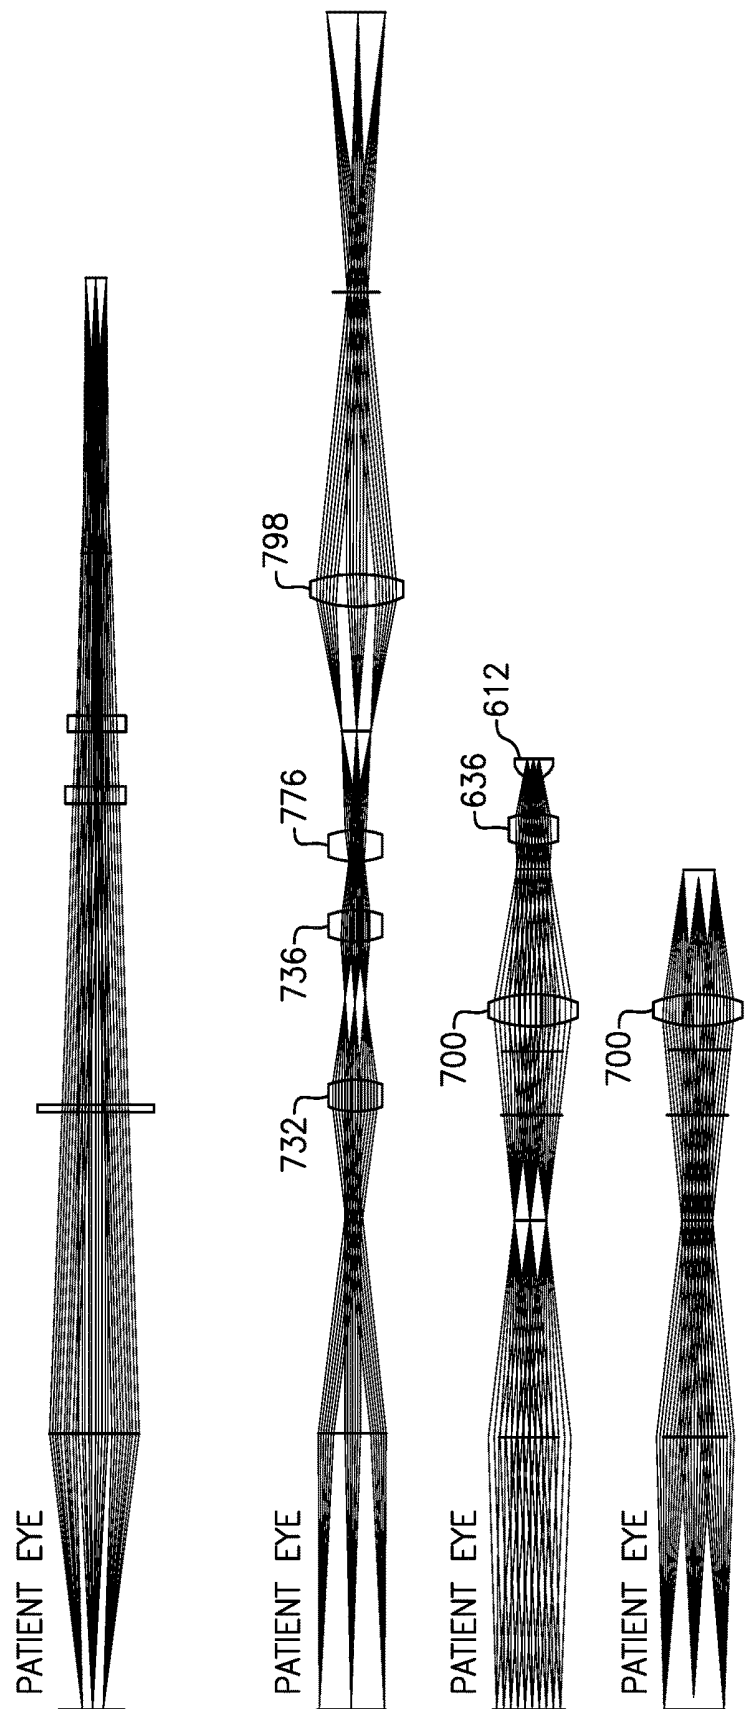


FIG.13

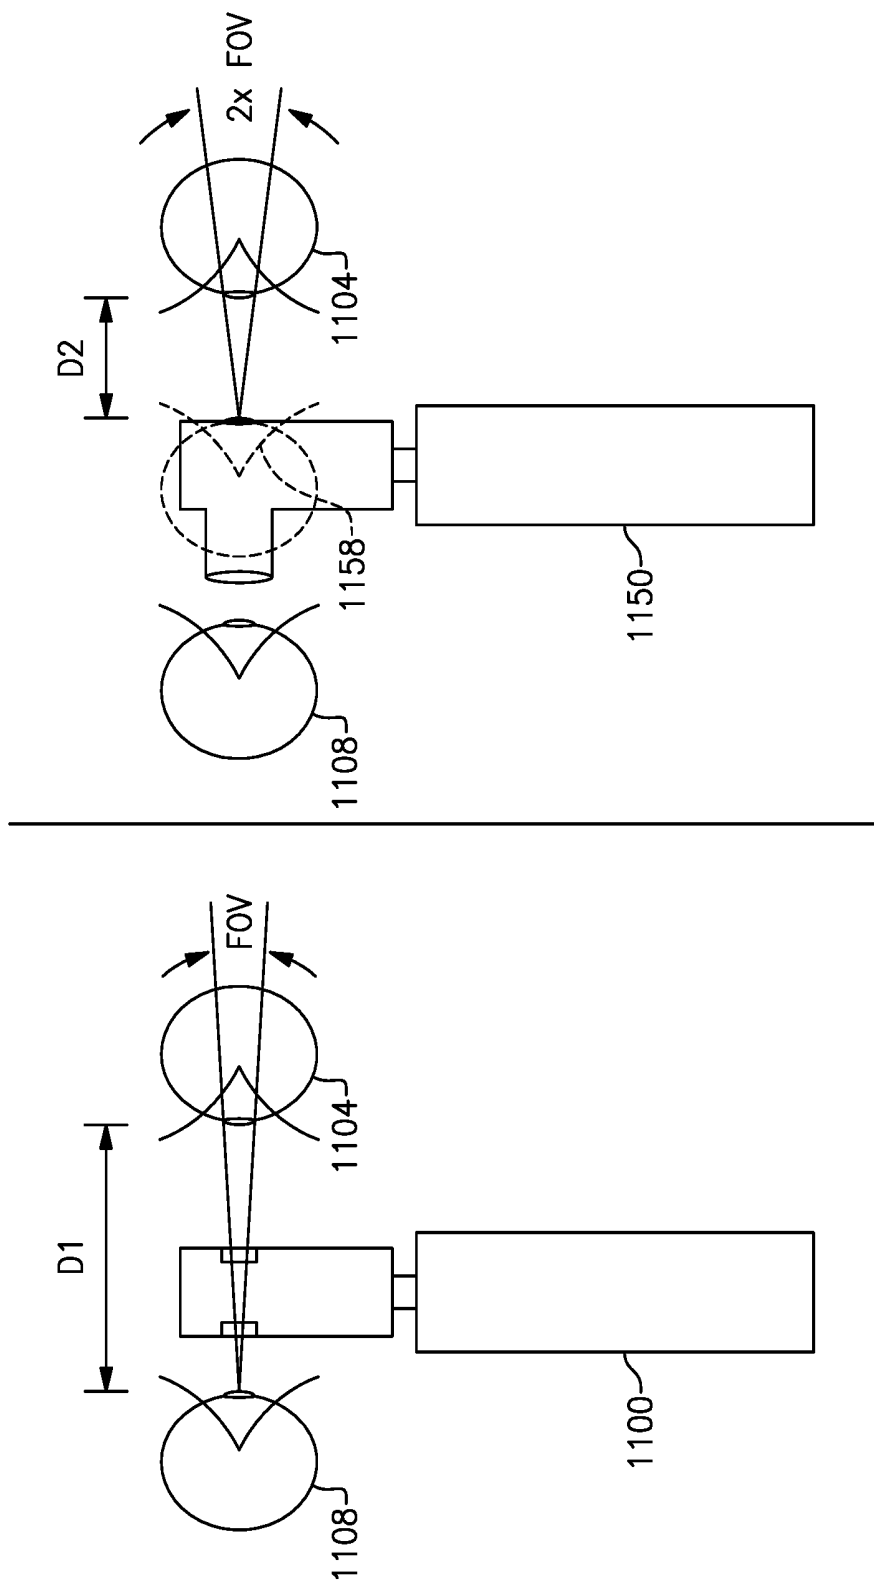


FIG. 14

1

BORESOPIC OPTICAL SYSTEM FOR MEDICAL DIAGNOSTIC INSTRUMENTS AND MEDICAL DIAGNOSTIC INSTRUMENTS HAVING INTERLOCKING ASSEMBLY FEATURES

CROSS REFERENCE TO RELATED APPLICATIONS

This application is a continuation of U.S. patent application Ser. No. 14/853,282, entitled Borescopic Optical System for Medical Diagnostic Instruments and Medical Diagnostic Instruments Having Interlocking Assembly Features, filed Sep. 14, 2015, which claims priority to U.S. Patent Application Ser. No. 62/071,128, entitled Borescopic Optical System for Medical Diagnostic Instruments and Medical Diagnostic Instruments Having Interlocking Assembly Features, filed Sep. 15, 2014, pursuant to relevant portions of 35 U.S.C. § 120 and 37 CFR § 1.53, the entire contents of which is herein incorporated by reference.

TECHNICAL FIELD

This application relates generally to the field of diagnostic medicine and more specifically to a medical diagnostic instrument having an enhanced field of view, as well as an optical architecture that can be commonly shared by a suite of disparate diagnostic instruments.

BACKGROUND

Certain instruments are well known in the medical field for conducting physical assessments of patients and in which separate instruments are used for examining specific target areas. For example, ophthalmoscopes are used by a primary physician or ophthalmologist for examining the eyes, otoscopes are utilized for examining the ear canal and tympanic membrane, and laryngoscopes are used for examining the throat passage.

A general pervasive issue with these physical assessment devices is in providing a suitably large field of view of the intended target of interest. For example, it is desirable and advantageous to be able to access the entire tympanic membrane while using an otoscope. It is further desirable to be able to capture more of the retinal area of the eye all at once during an examination.

An issue in creating a larger field of view is that of the instrument itself. For example and with ophthalmoscopes, the field of view can be expanded by shortening the working distance between the patient and the instrument. The foregoing, however, creates issues in terms of anxiety and discomfort for the patient. It is therefore desirable to provide a medical diagnostic instrument that can provide a larger field of view, but without having to shorten the working distance between the instrument and the patient.

Yet another pervasive issue in the field relates to improving manufacturability of such diagnostic instruments in order to reduce labor and associated material costs by using a minimum number of components, but without sacrificing reliability. To better deal with this concern, it would be extremely beneficial to develop a suitable optical architecture that could be shared between multiple types of physical assessment devices and to develop a simpler manufacturing method for these devices.

BRIEF DESCRIPTION

According to one aspect, there is provided a medical diagnostic instrument configured for viewing a target of

2

interest, the instrument comprising an instrument housing having a distal end, an opposing proximal end and an interior. An optical system that is disposed within the interior of the instrument housing comprises a distal objective lens, at least one intermediately disposed relay lens and a proximal eyepiece lens. Each of the lenses are commonly disposed along an optical axis, in which the optical system is configured to create an entrance pupil distal of the distal end of the instrument in order to create an increased field of view of the target of interest. According to at least one embodiment, the instrument is an ophthalmoscope.

In a preferred version, the herein described optical system creates an entrance pupil that is distal of the instrument housing. This entrance pupil establishes a “virtual eye” of the caregiver that increases the working distance and the field of view by effectively shifting the eye of the caregiver away from the patient’s eye. The optical elements used for purpose of this system can be defined by a plastic molded design in which each of the optical elements are reversible/symmetrical and corrected for optical aberrations by means of aspheric curves. According to at least one embodiment, each of the lenses include a raised peripheral edge to protect the lenses from surface damage. At least one field stop can be provided for minimizing glare or unwanted light from the system.

The optical system can be disposed within a viewing assembly that includes features that enable interlocking connection with the illumination assembly.

In at least one embodiment, the optical system can be integrated as part of the instrument. In one version, a module equipped with the above optical system can be releasably attached to the medical diagnostic instrument to create the entrance pupil and also thereby increase the field of view.

According to yet another aspect, an otoscope is provided that comprises an instrument head having a distal end opening, an opposing proximal end opening and a substantially hollow interior enabling a target of interest to be viewed by a caregiver in a first mode. A module is releasably attachable for insertion into the interior of the instrument head, the module having an optical system that increases the field of view for viewing a target of interest in a second mode.

According to at least embodiment, the module comprises a distal optical element, at least one intermediate relay lens element and a proximal eyepiece lens element, each of the lens elements being aligned with the distal and proximal end openings of the instrument head when attached. The instrument head can include a proximal window that is releasably removable to permit inclusion of the module.

In at least one embodiment, each of the lens elements of the module are made from a molded plastic, wherein each of the lens elements of the module are symmetric and reversible. In at least one version, each of the lens elements in the optical system are interchangeable. According to at least one embodiment, each of the lens elements can further include a raised peripheral edge along each optical surface thereof to minimize damage during handling and assembly.

The at least one relay lens and eyepiece lens element can be axially disposed in relation to at least one flexible member within a module housing, the module further including a twistable retaining cap that can permit minor positional adjustments of the lens elements to effect minor focus adjustments.

According to another aspect, a plurality of medical diagnostic instruments are provided wherein each of the medical diagnostic instruments include an optical system that is configured to produce a virtual pupil at the distal end of the

instrument in order to increase the field of view. The plurality of instruments may include an otoscope and an ophthalmoscope, among others.

In one embodiment, the optical system can be integrated within at least one instrument housing. In another version, a module having the optical system can be releasably attached to at least one of the medical diagnostic instruments.

The optical system can include an objective distal lens, at least one intermediate relay lens and a proximal eyepiece lens, each of the lenses being commonly disposed along an optical axis of the instrument. In one version, each of the lenses of the optical system comprise symmetric reversible optical surfaces. In a preferred version, the lenses can be made from a moldable plastic in which each side of the lens can include a raised peripheral edge that can act in order to minimize damage to the optical surfaces during handling thereof in assembly.

In at least one embodiment, at least one of the medical diagnostic instruments further comprises an illumination assembly and in which the optical system and the illumination assembly can include features to enable an interlocking connection therebetween. In at least one version, the illumination assembly can include a plurality of components having respective features to enable interlocking connection therebetween.

The instruments having the common optical system can include ophthalmoscopes and otoscopes, among others. The optical system can include at least one distal optical element and at least one pair of relay lenses commonly disposed along an optical axis of the instrument and wherein the optical system is configured to create an entrance pupil that is distal of the distal end of the instrument housing in order to create the expanded field of view.

According to yet another aspect, a method is provided for manufacturing a medical diagnostic instrument to increase the effective field of view of the instrument. The method comprises providing an optical system in the instrument, the optical system having at least a distal objective lens, at least one intermediate relay lens and a proximal eyepiece lens in which the optical system is configured to create an entrance pupil distal of a distal end of the instrument.

In one version, each of the lenses of the optical system can be symmetric and reversible. According to one embodiment, the lenses can include a raised peripheral edge along each optical surface that can minimize damage while handling during assembly. In one version, the lenses can be made from plastic.

The medical diagnostic instrument can be at least one of an ophthalmoscope and an otoscope. According to one version, the optical system is provided as a module to an existing medical diagnostic instrument, such as an otoscope, the method further including the step of providing the module for inclusion into the interior of the instrument following removing of a releasable proximal window of the instrument. As such, the otoscope can then be configured to operate in separate modes depending on the inclusion of the releasably attachable module; namely, a first mode that enables the inclusion of tools within the interior of the otoscope, and a second enhanced field of view mode that includes the module.

According to yet another aspect, there is provided an optical module for placement within a medical diagnostic instrument to increase the effective field of view with respect to a target of interest, the module comprising a module housing including at least one distal optical element and at least one pair of relay lenses disposed within an interior of the housing and aligned commonly along an optical axis and

wherein the optical system forms an entrance pupil distal of the distal end of the module to create an entrance pupil.

According to yet another aspect, there is provided a physical assessment device comprising an instrument housing having an interior, a viewing assembly disposed between distal and proximal end openings of the instrument housing, and an illumination assembly including at least one light source for illuminating a target of interest. According to this aspect, at least one of the viewing assembly and illumination assembly can have a plurality of components that are assembled by means of interlocking engagement. According to at least one embodiment, the illumination assembly and viewing assembly can include interlocking features that enable releasable connection therebetween.

According to one version, the illumination assembly can be configured for interlocking connection with a first viewing assembly having a first field of view and a second viewing assembly having a second field of view in which one of the viewing assemblies produces a distal entrance pupil for providing an enhanced field of view of an intended target of interest. In one version, the viewing assembly can be provided with a borescopic optical system comprising a distal objective lens, at least one intermediate relay lens, and a proximal eyepiece lens. The instrument can, for example, be an ophthalmoscope.

In one embodiment, each of the lenses used in the optical system are symmetrical and reversible, enabling the lenses to be easily assembled and without creating manufacturing errors. To further prevent damage to optical surfaces, the lenses can include a raised peripheral edge on each optical surface.

One advantage realized herein is that of modularization which can provide a common optical architecture for a number of disparate medical diagnostic instruments.

Another advantage is that the optical adapter when attached to a medical instrument, such as an otoscope, can further permit access of an intended target by tools, as needed.

Yet another advantage is that an enhanced field of view as provided by the herein described optical system permits more reliable and comprehensive examinations of a patient to be conducted.

Still another advantage realized is that of faster diagnostic patient examinations in that the realized enhanced field of view permits easier navigation by the caregiver of a larger target area in order to find the intended point of interest and to pan the instrument.

Additionally and through the virtual pupil that is created, the target of interest is actually made closer which provides more magnification, thereby making it considerably easier for the caregiver to discern features of the intended medical target.

These and other features and advantages will be readily apparent from the following Detailed Description, which should be read in conjunction with the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1(a) is a side perspective view of a prior art medical diagnostic instrument and more specifically, an otoscope;

FIG. 1(b) is a rear perspective view of the prior art otoscope of FIG. 1(a);

FIG. 2(a) is a front view of another prior art medical diagnostic instrument and more specifically, an ophthalmoscope;

FIG. 2(b) is a side elevational view of the ophthalmoscope of FIG. 2(a);

FIG. 3 is a perspective view of a medical diagnostic instrument made in accordance with an embodiment;

FIGS. 4(a)-4(g) are partial assembly views, shown in sequence, of the medical diagnostic instrument of FIG. 3;

FIG. 5 is a simplified perspective view of a modular version of an optical system for releasable attachment to a medical diagnostic instrument and in accordance with another embodiment;

FIG. 6 is a partially assembled side elevational view of a medical diagnostic instrument made in accordance with another embodiment;

FIG. 7(a)-7(k) depicts sequential partial assembly views of a portion of the medical diagnostic instrument of FIG. 6;

FIGS. 8(a)-(f) depict sequential partial assembly views of an optical assembly for a medical diagnostic instrument made in accordance with an embodiment, including a sectioned view of an optical system which is shown in FIG. 8(c);

FIGS. 9(a)-9(c) depict partial views of a medical diagnostic instrument made in accordance with yet another embodiment;

FIGS. 10(a) and 10(b) are perspective views of the assembled medical diagnostic instrument of FIGS. 9(a)-9(c);

FIG. 11 is a side elevational view, shown in section, of a medical diagnostic instrument in accordance with yet another embodiment;

FIG. 12 is an optical layout comparing a prior art otoscope with an otoscope having an optical system in accordance with an embodiment;

FIG. 13 is an optical layout comparing a prior art ophthalmoscope with an ophthalmoscope configured in accordance with an embodiment; and

FIG. 14 is a schematic depiction comparing a prior direct ophthalmoscope with an instrument configured with an optical system in accordance with an embodiment.

DETAILED DESCRIPTION

The following relates to various embodiments of physical assessment devices or instruments as well as components that are engageable therewith, each of which can be configured with a common optical architecture that permits an enhanced field of view of a medical target of interest. More specifically, the description relates to embodiments that are directed to optical otoscopes and ophthalmoscopes. It will be readily understood that the concepts discussed herein may be applicable to other physical assessment devices, including versions of digitally configured devices employing electronic imagers or devices. In addition and throughout this description, several terms are often used in order to provide a suitable frame of reference with regard to the accompanying drawings. These terms, which include “exterior”, “interior”, “distal”, “proximal”, “inner”, “outer” and the like are not intended to limit the scope of the concepts which are discussed and claimed herein, except in those instances where so specifically indicated.

For purposes of background and referring to FIGS. 1(a) and 1(b), a typically known otoscope 100 is defined by an instrument head 104 having a distal end 108 and an opposing proximal end 112, which further defines a hollow interior 115. An axisymmetric speculum tip element (not shown) can be releasably attached, typically by means of a bayonet-type connection, in overlaying relation onto a truncated frusto-conical insertion portion 124 disposed at the distal end 108

of the instrument head 104. The distal insertion portion 124 includes a slot 126 for releasably engaging an interior feature of the speculum tip element, as well as a distal opening 128 that is aligned with the distal opening of the speculum tip element. When attached to the instrument 100 and in use, the speculum tip element is configured to be placed up to a predetermined distance into the ear canal of a patient.

The caregiver observes the ear canal through a magnifying optic or window 130 that is provided at the proximal end 112 of the instrument head 104. The instrument head 104 is supported by a handle (not shown) that includes at least one rechargeable battery configured to electrically power a contained light source, typically an incandescent or halogen bulb, that is disposed at an upper end of the instrument handle. A lower portion of the instrument head 104 includes a contact disposed in a bayonet connector 132. A polished proximal end of the bundle of optical fibers (not shown) is optically coupled to the light source with the opposing ends encircling the interior of the distal end of the insertion portion 124 to create uniform illumination. An adjustment control, such as a rheostat (not shown), is further provided in order to control the level of illumination. In use, this instrument 100 is configured to have a field of view of approximately 15 degrees, while the diameter of the average tympanic membrane is approximately 7 mm. Details relating to the design and operation of this medical diagnostic instrument, including the attachment to the handle are provided in U.S. Pat. Nos. 3,698,387 and 3,978,850, the entire contents of which are herein incorporated by reference.

With reference to FIGS. 2(a) and 2(b), a known optical ophthalmoscope 200 typically includes an instrument head 204 that includes a distal end 205 and an opposing proximal end 207, the instrument head 204 being supported to and connected through a bayonet connector 214 to an instrument handle (not shown) that contains at least one rechargeable battery connected to a light source provided in the upper end of the handle. As in the case of the otoscope 100, FIG. 1, one polished end of a bundle of optical fibers are optically coupled to the contained light source and the opposing end of the fiber bundle encircles the interior of a distal opening of the instrument head 204 in order to direct illumination toward the target of interest (eye). A diopter wheel 220 is disposed for rotational movement relative to an optical axis of the instrument 200, in which the caregiver can view portions of the eye through an aligned opening 232, 236 provided in the proximal and distal ends 207, 205 of the instrument 200, as well as an aperture wheel 226. The instrument 200 further includes a sliding polarizer red/free switch 228 beneath the opening 232.

Moving the instrument 200 closer to the patient will increase the field of view, but patients are made anxious when the instrument 200 is brought into immediate proximity with the eye, and as a result these instruments 200 are typically used at an appropriate working distance (approximately 13-15 mm) between the patient and the instrument with the instrument having a field of view of approximately 5 degrees. Details relating to the workings, design and operation of this instrument are known found in U.S. Pat. No. 4,526,449, the entire contents of which are herein incorporated by reference.

A medical diagnostic instrument made in accordance with a first exemplary embodiment is provided in FIGS. 3-4(g). More specifically, the instrument 400 is an otoscope having an instrument head 404 defined by respective distal and proximal ends 406, 408. An illumination connector 411 extends from the bottom of the instrument head 404, which

is mechanically and electrically connected to the upper end of an instrument handle (not shown). The instrument head **404** includes a cover **428** having an insufflation port **409**, as well as an attachment and retention mechanism **413** for releasably securing a speculum tip (not shown) in overlaying fashion onto a substantially conical distal insertion portion **416**, the latter mechanism including a rotatable actuator knob **419** disposed in relation to the insertion portion **416**.

Though not shown, the illuminator connector **411** is configured to engage the upper end of the instrument handle, using a bayonet-type connection and in which the instrument handle is configured to retain at least one battery (not shown), such as a rechargeable battery. A light source (not shown) such as an incandescent lamp or bulb is further provided at the upper end of the instrument handle in relation to a bundle of optical fibers. The proximal ends of the optical fiber bundle are polished and optically coupled with the light source. The optical fiber bundle extends into the instrument head **404** and encircle the interior diameter of a distal opening **406** of the conical distal insertion portion **416**. The distal insertion portion **416** is shaped and configured to releasably retain an axisymmetric speculum tip, the latter being configured for insertion to a predetermined distance into the ear canal. The actuator knob **419** of the tip attachment and retention mechanism **413** is configured to engage and/or disengage with corresponding features on the speculum tip based on relative rotation between the speculum tip and the actuator knob **419**. Details relating to the tip attachment and retention mechanism **413** and related aspects of the speculum tip and distal insertion portion **416** are provided, for example, in U.S. Pat. No. 7,399,275, the entire contents of which are herein incorporated by reference.

The following description details an assembly flow or process for the otoscope **400**. First and as shown in FIG. **4(a)**, the herein described otoscope **400** is shown with various components in an exploded view including the illumination connector **411**, the distal insertion portion **416**, an inner former **420**, an optics assembly **430**, and a portion of the outer cover **428**. The inner former **420** is a structural portion of the instrument **400** that includes a lower section **423** configured to receive the optical fiber bundle (not shown) extending upwardly from the light source (not shown) contained within the instrument handle (not shown) for purposes of illumination, similar to that described in regard to the instrument **100** of FIG. **1** as well as an opening **427** that is sized to receive the optics assembly **430**. The tip attachment and retention mechanism **413** is not shown in these assembly views for reasons of clarity.

As shown in FIGS. **4(b)** and **4(c)**, the optics assembly **430** is configured to be fitted within the opening **427** of the inner former **420** with the outer cover **428** being further disposed about the exterior of the optics assembly **430**, as shown in FIG. **4(d)**, and the illumination connector **411** being secured to the bottom of the assemblage, as shown in FIG. **4(e)**. A cutaway version of the assembled otoscope **400** is shown in FIG. **4(e)** without a portion of the outer cover **428** for purposes of clarity. As shown in FIG. **4(e)** and when assembled, the proximal end of the optics assembly **430** is roughly coplanar with the proximal end of the instrument head (i.e., cover **428**).

The components of the herein described optics assembly **430** are shown in an exploded view in FIG. **4(f)**. According to this exemplary embodiment, the optics assembly **430** is defined by a housing **432** having a three separate diametrical sections; namely, a distal section **434**, an intermediate section **435**, and a proximal section **437**. According to this embodiment, the distal section is defined by an extended

length terminating at the intermediate section **435**, the latter having a larger interior diameter than the distal section **434** and the proximal section **437** having a larger diameter than that of the intermediate and distal sections **434**, **435**. Overall, the housing **432** is defined by a cylindrical configuration having tapered axial sections between the distal and intermediate sections **434** and **435** and between the intermediate section **435** and the proximal section **437** of the housing **432**.

The housing **432** is essentially hollow and is further defined by respective distal and proximal end openings **439**, **441** in which the housing **432** is further configured to support a plurality of optical components. A plano window **444** is disposed at the distal end **439** of the housing **432** in the distal section **434** with an objective lens **447** being proximally disposed adjacent a plano window **444**. According to this exemplary embodiment, the objective lens **447** is made from an optical grade plastic, although alternatively, other materials that have optical quality can be substituted. Referring to FIGS. **4(f)** and **4(g)**, a relay lens **449** is further disposed within the intermediate section **435** of the housing **432**, with a field stop **451** being disposed between the relay lens **449** and the objective lens **447**.

Still referring to FIGS. **4(f)** and **4(g)**, a first spacer **453** is proximally disposed relative to the relay lens **449**. The first spacer **453** is defined by a substantially cylindrical configuration having a distal portion **454** that extends into the intermediate section **435** of the housing **432**, a proximal section **456** that is disposed within the proximal section **435** of the housing **432** and an intermediate portion **458** having a taper corresponding to the taper formed between the intermediate and proximal sections **435**, **437** of the housing **432**. The first spacer **453** is substantially hollow, other than being configured with an interior narrowed aperture **459** which is intended to block stray light, the first spacer **453** and aperture **459** being centrally aligned with an optical axis of the assembly **430**. A pair of O-rings **461** are disposed between the first spacer **453** and a proximally disposed second spacer **463**, wherein a field stop **465** is disposed at the distal end of the second spacer **463**. When assembled, the second spacer **463** is disposed within the proximal section **437** of the housing **432** and includes a series of exterior peripheral grooves **467** at the proximal end thereof that are sized and configured to retain at least one O-ring **469**. An eyepiece lens **471** is retained at the proximal end of the second spacer **463**. A retaining cap **473** is configured to engage the exterior of the third section **437** of the housing **432** in which the retaining cap **473** is defined by a cylindrical configuration having an open distal end **475** as well as a set of engagement features, including annular slots **477**, configured to engage corresponding exterior features **479** provided on the exterior of the proximal portion **437** of the housing **432** when the retaining cap **473** is attached thereupon and twisted or rotated in a first direction.

The retaining cap **473** is further configured to retain a plano window **480** that is sandwiched between a rear or proximal wall of the retaining cap **473** and the proximal end of the housing **432**, including the eyepiece lens **471**, wherein the rear wall of the retaining cap **473** further includes a proximal viewing opening **481**.

As assembled, the plano windows **443**, **480** at the distal and proximal ends of the housing **432** provide an effective seal relative to the interior of the optics assembly **430**. Other than the relative sizes of the lenses **447**, **449** and **471**, each of the lenses used herein according to this exemplary embodiment are symmetric, meaning that both the distal and proximal facing sides are defined by the same curvature, which according to the present embodiment is a biconvex

design. In addition, each of the lenses **447**, **449**, **471** according to this exemplary embodiment are made from an optical grade plastic, although any or all of the lenses could also be made from glass or other suitable material of optical quality. At the time of assembly, the engagement of the O-ring **469** as well as the O-rings **461** between the first and second spacers **453** and **469** can create a spring force when engaged by the retaining cap **473**, when twisted, that enables slight focus adjustments to be made to the herein described optics assembly **430**.

When assembled, the distal end of the optics assembly **430** extends into the interior of the conical insertion portion **416** and is substantially aligned with the distal opening **406** thereof. With reference to the optical trace diagram provided at FIG. **11**, illumination from a contained light source in the instrument handle (not shown) can be directed through the distal opening **406** of the instrument head **404** in a manner that is known and in which an enhanced (larger) field of view as compared to prior otoscopes, such as previously described according to FIG. **1**, is produced. More specifically, the herein described optics assembly **430** creates an entrance pupil **483** that is distal to the distal opening **406** of the otoscope **400** in which the contained objective lens **447**, relay lens **449** and eyepiece lens **471** create a upright image of the target of interest through imaging plane **482**. The field stop **451** is provided to reduce the effects of glare while the field stop **465** narrows the light relative to the eyepiece lens **471**, creating a borescopic optical train that effectively shifts the location of the caregiver's pupil to the entrance pupil **483**, thereby creating an expansive field of view.

Referring to FIG. **5** and shown schematically, an alternative instrument version can be contemplated in which an optical module **540**, similar to the herein described optical assembly **430**, can be releasably disposed within the interior of an otoscope, such as the prior art version **100**, FIG. **1**, in lieu of providing an optical assembly that is already integrated within the instrument. According to this version, the module **540** can have a similar configuration to that of the optics assembly of the previously described instrument, the module **540** being defined by a tapering housing **544** that includes a distal end opening **546** and a opposing proximal end opening **548** that are axially aligned along a defined optical axis with the distal and proximal ends of the instrument housing. As in the preceding version, the contained optics produce a virtual pupil equivalent to that of the caregiver's eye which is created distally relative to the distal end of the instrument with the light being directed through a contained relay lens system to the caregiver's eye.

At least one additional pair of relay lenses could be provided in tandem along the herein described optical axis of the instrument, depending on the application/use of the instrument.

A medical diagnostic instrument made in accordance with another exemplary embodiment is herein described with reference to FIGS. **6-8(f)**. The instrument **600** described in accordance with this embodiment is an ophthalmoscope, partially shown without a cover and instrument handle in FIG. **6**, which is configured to function similarly to that previously described with reference to FIG. **2**. The herein described version includes an illumination assembly **610**, having a plurality of components, as well as a viewing or optical assembly **710**.

First referring to FIGS. **7(a)-7(k)**, the assembly flow of an illumination assembly **610** is herein described. As discussed herein, the major components of the illumination assembly **610** can be constructed using a set of interlocking components, facilitating the process of manufacture. At an initial

point of assembly and referring to FIG. **7(a)**, a first series of components are assembled including an LED **612**, such as a white LED, that is disposed onto a upper facing surface of a circuit board **614**. A spacer **616** used in the subassembly includes a defined through aperture **618**, as well as a lower flange **620** that is sized to retain an O-ring **622**. A curved light pipe **624**, made from a light conducting plastic, can be assembled with a portion **627** of light pipe being retained within a slot **625** formed in the bottom surface **626** of the spacer **616** and in which the light pipe **624** includes an external notch **631** that enables the O-ring **622** to secure the light pipe **624** in a predetermined position. Referring to FIGS. **7(c)** and **7(d)**, the spacer **616** can be fitted within a defined recess **629**, FIG. **7(c)**, that is formed in a lower portion **630** of an assembly support member **628** relative to an aperture **634** that retains a lens element **636**, which according to this embodiment is an objective lens. A slot **638** is provided in the lower portion **630** of the assembly support member **628** adjacent the recess **629** that permits the retained light pipe **624** to extend outwardly from the assembly **610**, as shown in FIG. **7(d)**.

In terms of assembly flow and prior to assembling the spacer **616**, the objective lens **636** is placed into the aperture **634** defined in the lower portion **630** of the assembly support member **628**. The assembly support member **628** according to this embodiment includes the lower portion **630**, as well as an upper portion **637** and an intermediate portion **639**. The lower portion **630** of the assembly support member **628** is recessed with a bottom surface having the recess **629** being disposed between a pair of projecting leg portions **642** that are configured and spaced in order to receive an illumination connector **650** as well as the LED **612** and circuit board **614**.

Referring to FIG. **7(e)**, the assembly support member **628** and more specifically the lower portion **630** thereof, is configured to receive the illuminator connector **650**, shown partially exploded in FIG. **7(f)**. The illuminator connector **650** according to this exemplary embodiment is defined by an upper portion **654**, a necked intermediate section **656**, and a lower section **658**, the latter section being defined with a bayonet-type connector. The connector **650** is defined by a through axial center opening **660** defined by a first diameter extending into the intermediate necked portion **656** and a narrower diameter extending into the lower portion **658**, which is essentially hollow. A hollow insulator **664** is installed within the center axial opening **660** of the upper portion **654** of the illuminator connector **650** with a lower portion **667** of the insulator **664** being sized to extend partially into the lower portion **658**. A center conductor **670** made from an electrically conductive material is similarly fitted within the confines of the hollow insulator **664**. When installed, and as shown in the assembled condition of FIG. **7(e)**, an axial contacting end **673** of the center conductor **670** extends outwardly from the insulator **664**, with the end of the insulator **664** being substantially flush with the top surface of the illuminator connector **650**, as shown in FIG. **7(e)**.

Referring to FIGS. **7(e)**, **(f)** and **(g)**, the upper portion **654** of the illuminator connector **650** is shaped and configured to releasably engage the lower portion **630** of the assembly support member **628**, as shown in FIG. **7(g)** in an interlocking manner. More specifically and according to this exemplary embodiment, the upper portion **654** is defined by a pair of diametrically opposed curved portions **677** and a pair of flats **678** that are spaced to fit between the extending leg portions **642** of the lower portion **630**. The curved portions **677** extend above the plane of the top surface of the illuminator connector **650** to provide ample spacing for the

LED 612 and circuit board 614 which is sandwiched therebetween such that the axial contacting end 673 of the center connector 670 can be brought into contact with the circuit board 614. When assembled according to this configuration, the LED 612 and circuit board 614 are retained between the spacer 616 and more specifically, the O-ring 622 and the center conductor 670 of the illumination connector 650 with the curved portions 677 of the illuminator connector 650 being aligned with corresponding curved portions 679 formed at the bottom of the lower portion 630 of the assembly support member 628. A conductive spring clip 682 can be used to secure the assembly support member 628 with the illuminator connector 650 by placement of same over the aligned curved portions 677, following assembly in the position shown in FIG. 7(g).

Referring to FIG. 7(h), and following attachment of the assembly support member 628 to the illumination connector 650, a reticle wheel assembly 686 can be attached to the intermediate portion of the assembly support member 628. According to this embodiment, the reticle wheel assembly 686 includes an upper engagement portion 688, a lower engagement portion 690 and an aperture wheel 692 that is supported for rotation and disposed between the upper and lower engagement portions 688, 690. The reticle wheel assembly 686 is fitted within a defined recess 644 formed in the intermediate section 639 of the assembly support member 628. More specifically, respective upper and lower surfaces defining the recess 644 each include engagement rails 646 that are configured to engage sidewalls of the upper and lower engagement portions 688, 690 of the reticle wheel assembly 686 with the reticle wheel assembly 686 being sized to fit in an interlocking manner with the assembly support member 628. When assembled, a through aperture 696, including a reticle, is aligned with the LED 612, FIG. 4(a), and the lens element along an illumination axis of the assembly 610, as well as a through aperture 698 in the upper section 637 of the assembly support member 628, as shown in FIG. 7(i).

As shown in FIGS. 7(i) and 7(j), a reticle lens 700 is then placed into the through aperture 698. As shown in FIG. 7(k), a prismatic member 704 is then attached to the upper portion 637 of the herein described assembly member 628 and more specifically within a receiving cavity 706 that is formed at the top of the upper portion 637 of the assembly support member 628 and in alignment with the through aperture 698. The prismatic member 704 according to this embodiment includes an angled reflective surface 707. Alternatively, a mirror could be disposed to provide similar functionality. The design of the prismatic member can be suitably varied, such as shown by prismatic member 704A in FIG. 11.

As discussed, each of the components of the herein described illumination assembly 610 can be assembled according to this embodiment in an interlocking fashion without requiring fasteners such as screws, bolts or rivets. That is, each of the components of the foregoing assembly 610 can be built onto one another in a sequential fashion, such as described with reference to FIGS. 7(a)-7(k). The components can be made, for example, from a durable plastic.

Referring to FIG. 8(a), an optical assembly 710 in accordance with an exemplary embodiment is disposed in relation to the herein described illumination assembly 610 prior to assembly therewith. Additional details regarding the optical assembly 710 are herein discussed with reference to FIGS. 8(b) and 8(c) in which the herein described assembly includes a housing 712 made up of an lower or bottom section 716 and an upper or top section 720. The lower

section 716 is defined a top surface 724 having a semicircular groove 728 defined therein in which a first lens 732 is provided at one end of the groove 728 and a second lens 736 is defined at the opposing end of the groove 728. A pair of ears 730 extend upwardly from opposing sides of the lower section 716 relative to the second lens 736, the ears 730 including a vertical portion 734 and a transverse portion 738 extending from the top of the vertical portion 734 in substantially the same direction as the defined groove 728, but outwardly relative to the top surface 724. A plurality of posts 742 extend upwardly from the top surface 724 on opposing sides of the semicircular groove 728.

The upper section 720 of the housing 712 according to this embodiment includes a first portion 750 that is sized to cover the lower section 716, the interior surface (not shown) of this section 720 including a semicircular groove (not shown) that is aligned with the groove 728 provided on the lower section 716 and forming an optical tube with respect to the first and second lenses 732, 736. The first portion 750 is sized to be fitted between the ears 730 of the lower section 716 wherein the spaced ears 730 are sized to extend above the upper section 720 of the housing 712. A second adjacent portion 754 of the top section 720 includes a raised surface 756 that, when assembled, is substantially parallel to the top surface 724 of the lower section 716 but directly beneath and between the transverse ear portions 738, this surface 756 including a center slot or opening 760 that is sized to receive a detent 764.

A third adjoining section 766 of the housing 712 is defined by a tubular section 770 that is aligned with the semicircular groove of the first section 750. A plurality of components are disposed within the tubular section 770, which combines to form an optical system with the two lens elements 732, 736 provided in the semicircular groove 728 formed in the top surface 724 of the lower section 716. It will be understood, however, that this two-part design is exemplary and that other variations and modifications are possible.

Still referring to FIGS. 8(b) and (c), the components disposed within the tubular section 770 of the housing include a relay lens 776 that is positioned within the distal end of a lens carrier 780 having a through aperture. The lens carrier 780 is essentially hollow and for convenience can be built as a two-part assembly to enable assembly of the relay lens 776. The lens carrier 780 is defined by a substantially cylindrical section having a first diameter that is sized to support the relay lens 776 and a second diameter that is retained against a shoulder formed in the tube. An O-ring 784 is disposed between the lens carrier 780 and a spacer 790, the spacer 790 having a field stop 794 at its distal end. An eyepiece lens 798 is disposed in engagement with the proximal end of the spacer 790. Each of the lenses 776, 798 according to this configuration are symmetrical; that is, each lens 776, 798 includes identically curved (convex) distal and proximal surfaces. Additionally and according to at least one version, each of the peripheral edges of the lenses 776, 798 can be raised to prevent damage, such as scratching to the optical surfaces.

A retaining cap 800 engageable with the proximal end of the tubular section 770, the retaining cap 800 includes an open distal end 802 and engagement features, such as annular slots 806, as well as a proximal viewing opening. A plano window 804 is disposed between the eyepiece lens 798 and the rear wall of the retaining cap 800 wherein the retaining cap 800 can be twisted in order to apply a compressive force against the resilient O-rings 784 to effect minor focus adjustments at the factory level, for example, to compensate for manufacturing tolerances.

A thin sheet **810** of copper or other flexible metal can be positioned such that each end of the sheet **810** is secured beneath the extending ear portions **738** and spans across the raised surface **756** of the second section **754**. As discussed herein, this portion of the assembly is used in connection with diopter wheel **840**.

According to this version, the upper portion **720** of the housing **712** includes a plurality of holes **744** that can be aligned with the posts **742** of the lower portion **716** to enable the housing **712** to be secured.

Upon assembly, the optical assembly **710** can be attached to the illumination assembly **610** in which the lower portion **716** includes a pair of spaced rail sections **850** that can be engaged with the upper portion sidewalls **698**, FIG. **8(a)**, of the assembly support member **628**.

Referring to FIG. **8(e)**, the diopter wheel **840** is shown prior to attachment, along with a retention cap or hub **844**. The diopter wheel **840** includes a center through aperture **842** that is aligned with a lateral cavity **699** formed in the intermediate portion **637** of the assembly support member **628**. The hub **844** is engageable with to extend through the aperture **842** and into the cavity **699** to retain the wheel **840**, as shown in FIG. **8(f)**. In this embodiment, the outer periphery **846** of the diopter wheel **840** is caused to extend into the raised second section **754** of the viewing assembly **710** and into contact with the detent **764**, which is held in place by the thin metal sheet **810**, acting as a biasing spring.

The illumination assembly **610** and optical assembly **710** according to this instrument design does not require fasteners, wherein all of the components can be assembled based on a series of interconnecting fits between the various components.

Referring to FIGS. **9(a)**-**10(b)** and according to another embodiment, the preceding illumination assembly can be used with an existing viewing assembly **610**, as would be found, for example, in conjunction with the ophthalmic instrument **200** of FIG. **2**.

A partially assembled version is shown in FIGS. **9(b)** and **9(c)**, wherein the illumination assembly **610** is identical to that previously described and further including a diopter wheel **840** that is attached to the assembly **610**. For purposes of this discussion, similar parts are herein labeled with the same reference numerals for the sake of clarity. The viewing assembly **910** is attached to the upper portion **637** of the illumination assembly **610**, the viewing assembly **910** according to this exemplary embodiment comprising a single component that includes a pair of engagement rails **918** to enable the viewing assembly **910** to slidably engage with the sidewalls **698**, FIG. **8(a)**, of the upper section **637** of the assembly support member **628**. The viewing assembly **910** according to this embodiment includes a pair of upwardly extending ears **924**, similar to those previously described along with a spring support section **928** having a surface **932** disposed between the spaced ears **924**. The surface **932** includes a center opening **936** sized to receive a detent **940** in which the exterior of the surface of the support section **928** supports a thin metallic sheet section **810** whose ends are disposed beneath the ears **924** in order to engage the outer periphery **846** of the supported diopter wheel **840** when rotated. The single component is configured to permit viewing, including a groove disposed on the upper surface.

FIGS. **10(a)** and **10(b)** illustrate a fully assembled version of this latter instrument **1000**, including a cover **1020** having slots **1032** and **1036** each sized to enable access to the

diopter wheel **840** and aperture wheel **692**, as well as a flexible eye cup **1028** at the distal end thereof for contacting the patient.

Functionally, the overall effects provided by the creation of a virtual pupil for each instrument are schematically depicted in FIGS. **12** and **13**, comparing the otoscopic and ophthalmic versions described herein with the prior art versions depicted in FIGS. **1** and **2**, respectively. With the herein described optical systems, the field of view can be increased from about 5 degrees to about 15 degrees for each device and enables the entire tympanic membrane and a larger portion of the retina to be viewed all at once by the caregiver by an otoscope and ophthalmoscope, respectively.

Another illustration of the overall benefit of the herein described invention is shown comparatively with reference to FIG. **14** between a prior art instrument **1100** having a distance **D1** between the eye of the patient **1104** and that of the clinician **1108** and a field of view based on this distance. In the instrument **1150** and creating a "virtual eye" **1158** as previously described the field of view is significantly increased based on the shorter distance between the virtual eye **1158** and that of the patient **1104**. The foregoing advantage is provided in spite of the overall increase in thickness of the instrument **1150**, in which the creation of an entrance pupil (or "virtual eye") reduces the effective working distance between the eye of the caregiver and the patient by negating the thickness of the instrument to permit the extended field of view and using a direct ophthalmoscope.

PARTS LIST FOR FIGS. 1-14

100 instrument (otoscope)
104 instrument head
108 distal end, instrument head
112 proximal end, instrument head
115 hollow interior
124 distal insertion portion
126 slot
128 distal opening
130 magnifying optic or window
132 bayonet connector
200 instrument (ophthalmoscope)
204 instrument head
205 distal end
207 proximal end
214 bayonet connector
220 diopter wheel
226 aperture wheel
228 sliding switch
400 instrument
404 instrument head
406 distal end
408 proximal end
409 insufflation port
411 illumination connector
413 tip attachment and retention mechanism
416 conical insertion portion
419 actuator knob
420 inner former
423 lower portion
427 opening
428 cover
430 optics assembly
432 housing
434 distal section, housing
435 intermediate section, housing
437 proximal section, housing

439 distal opening
 441 proximal opening
 444 plano window
 447 objective lens
 449 relay lens
 451 field stop
 453 first spacer
 454 distal section
 456 proximal section
 457 intermediate section
 459 aperture, narrowed
 461 O-rings
 463 second spacer
 465 field stop
 467 peripheral grooves
 469 O-ring
 471 eyepiece lens
 473 retaining cap
 475 distal open end
 477 annular slots
 479 exterior engagement features
 480 image
 481 proximal viewing opening
 482 image plane
 483 entrance pupil
 540 optical module
 544 housing
 546 distal end opening
 548 proximal end opening
 600 instrument, medical diagnostic
 610 illumination assembly
 612 LED
 614 circuit board
 616 spacer
 618 through aperture, spacer
 620 lower flange
 622 O-ring
 624 curved light pipe
 625 slot
 626 bottom surface
 627 portion of light pipe
 628 assembly support member
 629 recess
 630 lower portion, assembly support member
 631 external notch
 634 aperture
 636 lens element
 637 upper portion, assembly support member
 638 slot
 639 intermediate portion, assembly support member
 642 projecting leg portions
 644 recess
 646 engagement rails
 650 illumination connector
 654 upper portion, illumination connector
 656 intermediate portion, illumination connector
 658 lower portion, illumination connector
 660 axial through opening
 664 insulator
 667 lower portion, insulator
 670 center conductor
 673 axial contacting end
 677 curved portions
 678 flats
 679 curved portions, assembly support member
 682 spring clip
 686 reticle wheel assembly

688 upper engagement portion, wheel assembly
 690 lower engagement portion, wheel assembly
 692 aperture wheel
 696 through aperture
 5 698 sidewalls, upper portion
 699 cavity
 700 reticle lens
 704 prismatic member
 704A prismatic member
 10 706 receiving cavity
 710 optical or viewing assembly
 712 housing
 716 lower or bottom portion
 15 720 upper or top portion
 724 top surface
 728 semi-circular groove
 730 ears
 732 first lens
 20 734 vertical portion
 736 second lens
 738 transverse portion
 742 posts
 744 holes
 25 750 first portion
 754 second portion
 756 raised surface
 760 center slot
 764 detent
 30 766 third portion
 770 tubular portion
 776 relay lens
 780 lens carrier
 784 O-ring
 35 790 spacer
 794 field stop
 798 eyepiece lens
 800 retaining cap
 802 open distal end
 40 804 plano window
 806 annular slots, cap
 810 thin metal sheet
 840 diopter wheel
 842 center aperture
 45 844 hub
 846 outer periphery, diopter wheel
 850 spaced rail portions
 910 viewing assembly
 918 engagement rail portions
 50 924 ears
 928 support section
 932 surface
 936 center opening
 940 groove
 55 1000 instrument
 1020 cover
 1028 eye cup
 1032 slot, cover
 1100 instrument
 60 1104 patient eye
 1108 clinician eye
 1150 instrument
 1158 virtual eye

It will be apparent that other modifications and variations of the foregoing exemplary embodiments will be understood from the foregoing description as well as the following claims.

17

The invention claimed is:

1. An otoscope comprising:

an instrument head having a distal end opening, an opposing proximal end opening, and a substantially hollow interior enabling a target of interest to be viewed by a caregiver in a first viewing mode; and
a module releasably attachable for insertion into the interior of the instrument head, the module having a contained optical system that increases the field of view for viewing a target of interest in a second viewing mode distinct from the first viewing mode, the module extending into a distal end of the instrument head when attached thereto.

2. The otoscope according to claim 1, wherein the optical system of the module comprises a distal lens element, at least one intermediate relay lens element and a proximal eyepiece lens element, each of the lens elements of the contained optical system of the module being aligned with the distal and proximal end openings of the instrument head when the module is attached to the instrument head.

3. The otoscope according to claim 2, wherein each of the lens elements of the contained optical system of the module are made from plastic.

4. The otoscope according to claim 3, wherein each of the lens elements of the contained optical system of the module are reversible.

5. The otoscope according to claim 4, wherein at least some of the lens elements of the contained optical system of the module are interchangeable.

6. The otoscope according to claim 4, wherein each of the lens elements include a raised peripheral edge along each optical surface thereof.

7. The otoscope according to claim 2, wherein the at least one relay lens element and eyepiece lens element are axially disposed in relation to at least one flexible member within the module, the module further including a twistable retaining cap to permit minor positional adjustments of the contained lens elements for focusing.

8. The otoscope according to claim 1, wherein the instrument head includes a proximal window used in the first viewing mode that is releasably removable to permit the module to be inserted into the instrument head for use in the second viewing mode.

9. A physical assessment device comprising:

an instrument housing having an interior;
a viewing assembly disposed between distal and proximal end openings of the instrument housing; and
an illumination assembly including at least one light source for illuminating a target of interest, at least one

18

of the viewing assembly and illumination assembly having a plurality of components that are assembled by interlocking engagement with one another wherein the illumination assembly is configured for interlocking connection with a first viewing assembly having a first field of view and a second viewing assembly having a second view of view.

10. The physical assessment device according to claim 9, wherein the illumination assembly and viewing assembly include interlocking features that enable releasable connection therebetween.

11. The physical assessment device according to claim 9, wherein the instrument is an ophthalmoscope.

12. The physical assessment device according to claim 9, wherein the viewing assembly comprises an optical system that produces a distal entrance pupil for providing an enhanced field of view of a target of interest.

13. The physical assessment device according to claim 12, wherein the viewing assembly comprises a distal objective lens, at least one intermediately disposed relay lens and a proximal eyepiece lens.

14. The physical assessment device according to claim 13, wherein each of the lenses are reversible.

15. The physical assessment device according to claim 14, wherein the lenses each include a raised peripheral edge on each optical surface.

16. The otoscope according to claim 15, in which the optical system is contained within a module that is attached relative to the instrument head, the module extending into a distal end of the instrument head when attached thereto.

17. The otoscope according to claim 16, in which the module is releasably attached to the instrument head.

18. An otoscope comprising:

an instrument head having a distal end opening, an opposing proximal end opening, and a substantially hollow interior; and

an optical system comprising a distal lens element, at least one intermediately disposed relay lens element and a proximal eyepiece lens, each of the lens elements being aligned with the distal end opening and proximal end opening along an optical axis in which each of the lens elements are made from plastic and are defined by symmetrical optical surfaces on opposing sides, enabling the lens elements to be reversibly assembled and optically aligned.

19. The otoscope according to claim 18, wherein each lens element includes a raised peripheral edge on each optical surface.

* * * * *

专利名称(译)	用于医疗诊断仪器和医疗诊断仪器的气孔镜光学系统，具有互锁组装特征		
公开(公告)号	US10028648	公开(公告)日	2018-07-24
申请号	US15/493500	申请日	2017-04-21
[标]申请(专利权)人(译)	伟伦公司		
申请(专利权)人(译)	伟伦，INC.		
当前申请(专利权)人(译)	伟伦，INC.		
[标]发明人	GOLDFAIN ERVIN LIA RAYMOND A		
发明人	GOLDFAIN, ERVIN LIA, RAYMOND A.		
IPC分类号	A61B3/10 A61B1/227 A61B1/06 A61B3/12 A61B3/00		
CPC分类号	A61B1/227 A61B3/1208 A61B3/0008 A61B1/06 A61B3/156 A61B3/12 G02B13/0095		
优先权	62/071128 2014-09-15 US		
其他公开文献	US20170215719A1		
外部链接	Espacenet		

摘要(译)

医学诊断仪器或多个不同的医学诊断仪器配置有共同的光学架构，其在功能上创建虚拟眼睛以产生更接近患者并因此增加关于感兴趣目标的视野。该光学系统包括远端光学元件，至少一个中继透镜和目镜透镜，其中光学系统可以集成在至少一个仪器内或者使用可释放模块提供。另外，至少一个医疗诊断仪器的观察组件和照明组件中的至少一个可以使用通过互锁特征连接的一系列组件来组装。

