



US 20200060699A1

(19) **United States**

(12) **Patent Application Publication**  
**HONDA et al.**

(10) **Pub. No.: US 2020/0060699 A1**

(43) **Pub. Date: Feb. 27, 2020**

(54) **CALCULUS/CALCULI RETRIEVING  
DEVICE AND METHOD**

(52) **U.S. Cl.**  
CPC ..... *A61B 17/22* (2013.01); *A61B 2017/0034*  
(2013.01); *A61B 2017/22079* (2013.01)

(71) Applicant: **TERUMO KABUSHIKI KAISHA,**  
Tokyo (JP)

(72) Inventors: **Kei HONDA,** Hadano-shi (JP); **Makoto  
JINNO,** Tokyo (JP)

(57) **ABSTRACT**

(73) Assignee: **TERUMO KABUSHIKI KAISHA,**  
Tokyo (JP)

A method of retrieving calculus in a living body and relocating the calculus to a different location in the living body involves positioning an elongated member in the living body in which the calculus is located, drawing the calculus in the living body toward the elongated member while the elongated member is positioned in the living body so that the calculus is retained by the elongated member; moving the elongated member so that the elongated member is located at a position in the living body that is different from the position of the elongated member in the living body during the drawing of the calculus toward the elongated member; and releasing the calculus from the elongated member so that the calculus is at a position in the living body different from a location of the calculus in the living body while the calculus is being drawn toward the elongated member.

(21) Appl. No.: **16/668,320**


(22) Filed: **Oct. 30, 2019**


**Related U.S. Application Data**



(62) Division of application No. 14/671,083, filed on Mar. 27, 2015, now Pat. No. 10,485,563.

**Publication Classification**

(51) **Int. Cl.**  
*A61B 17/22* (2006.01)

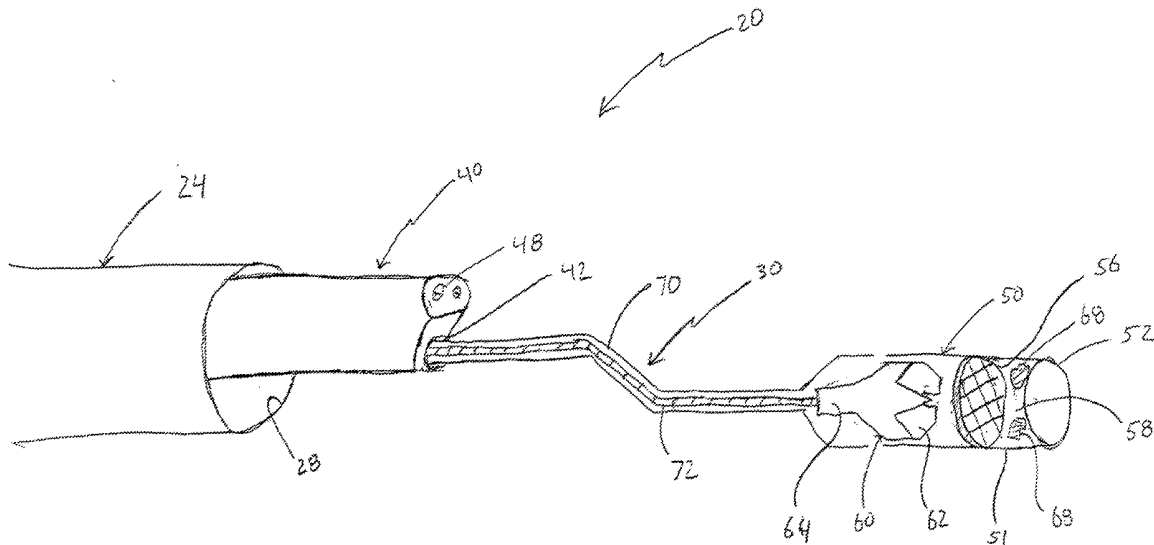

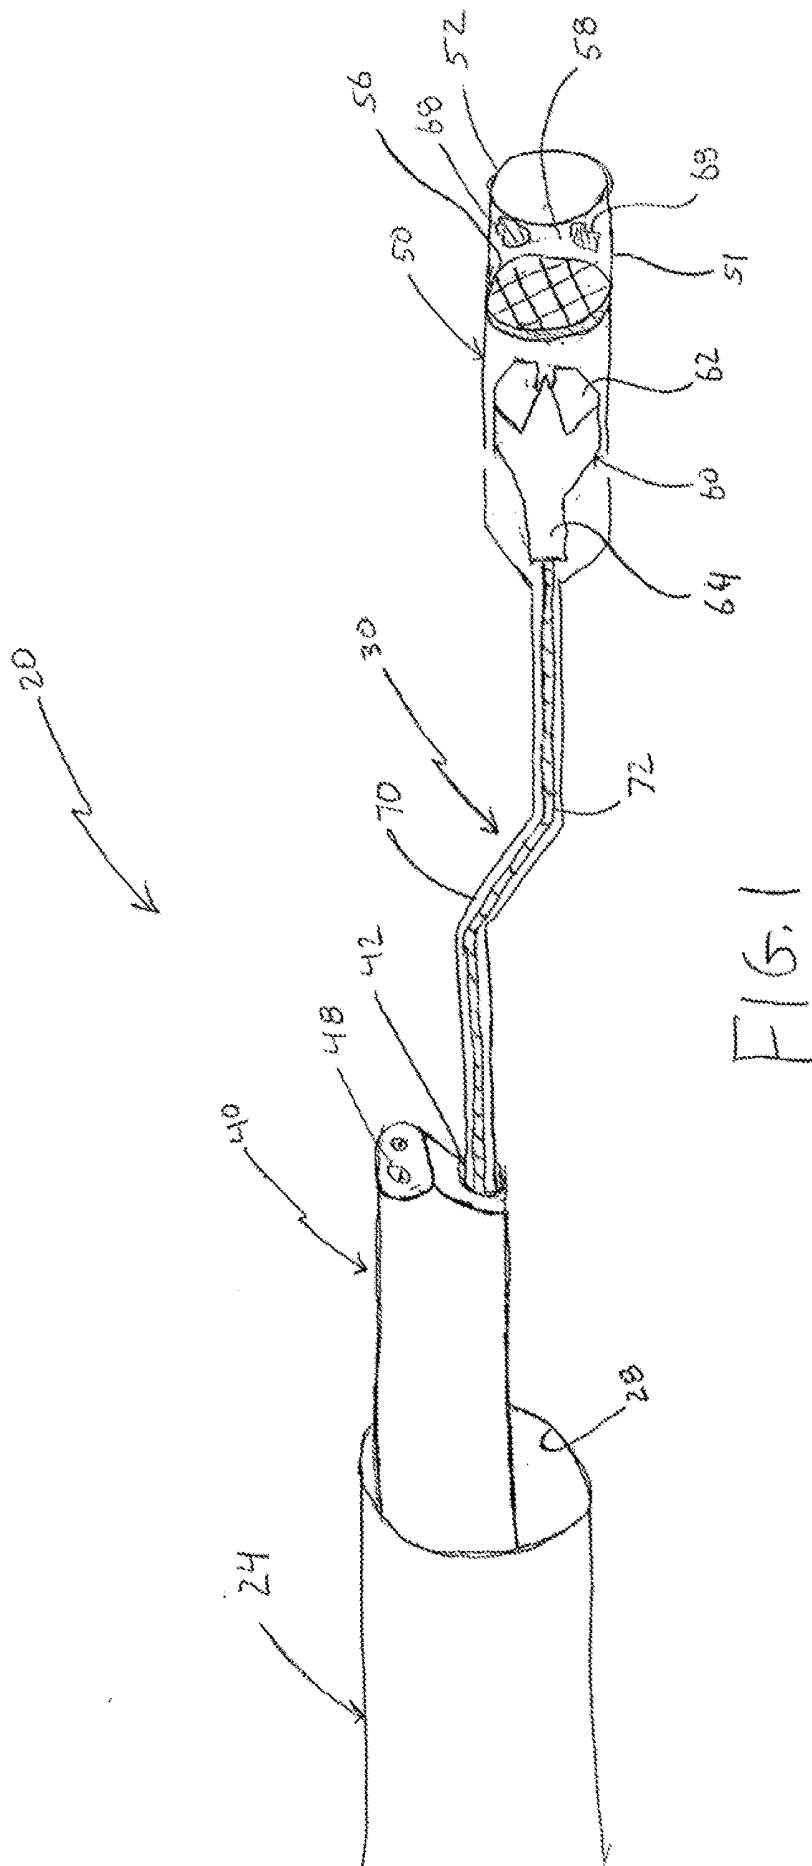

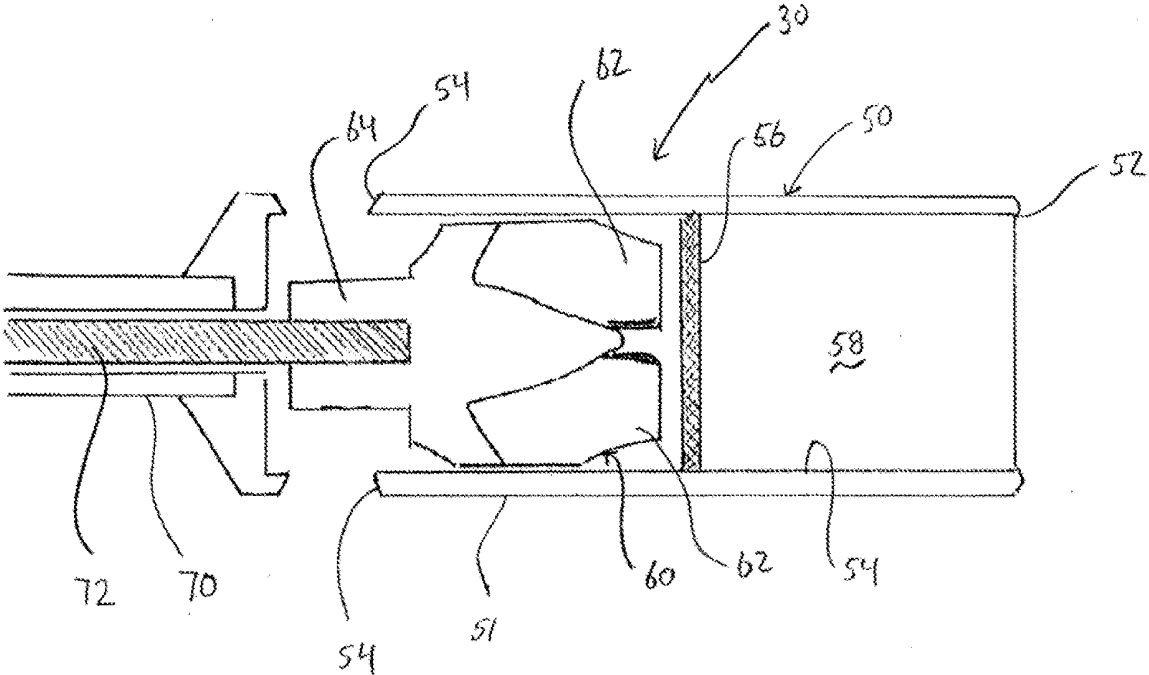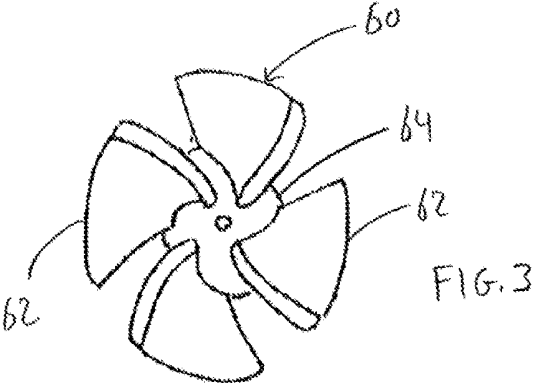

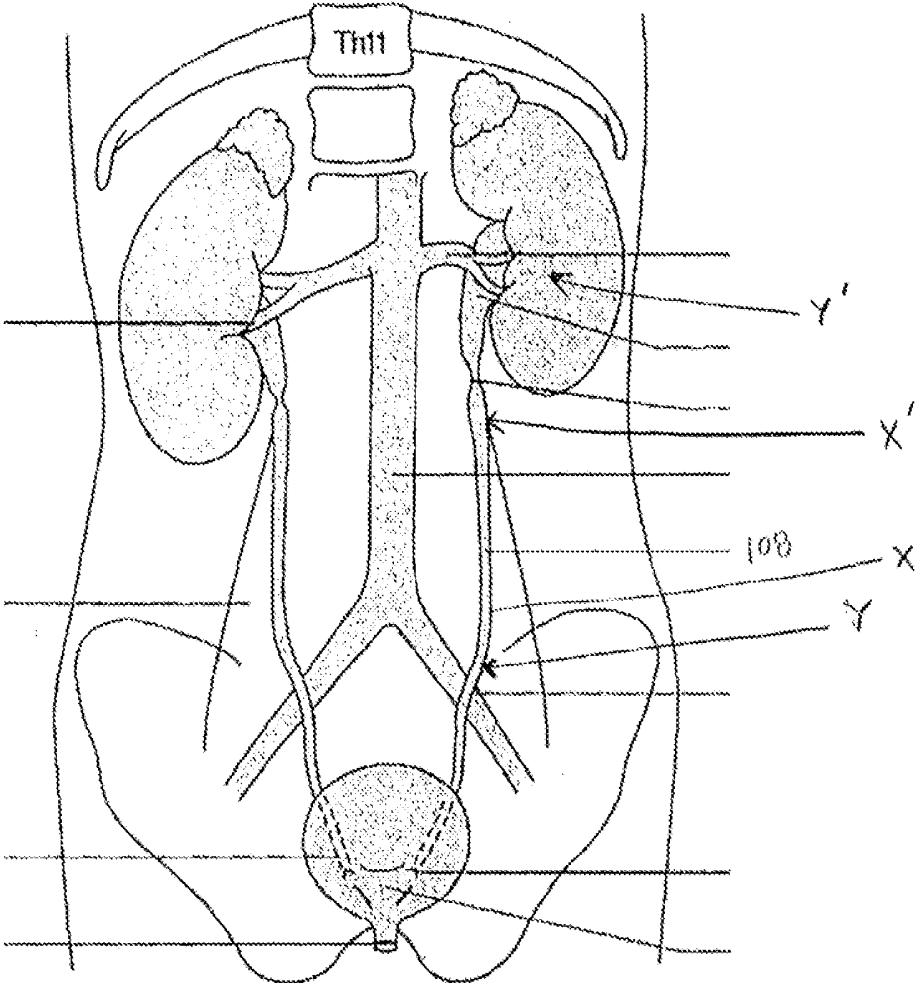


FIG. 4

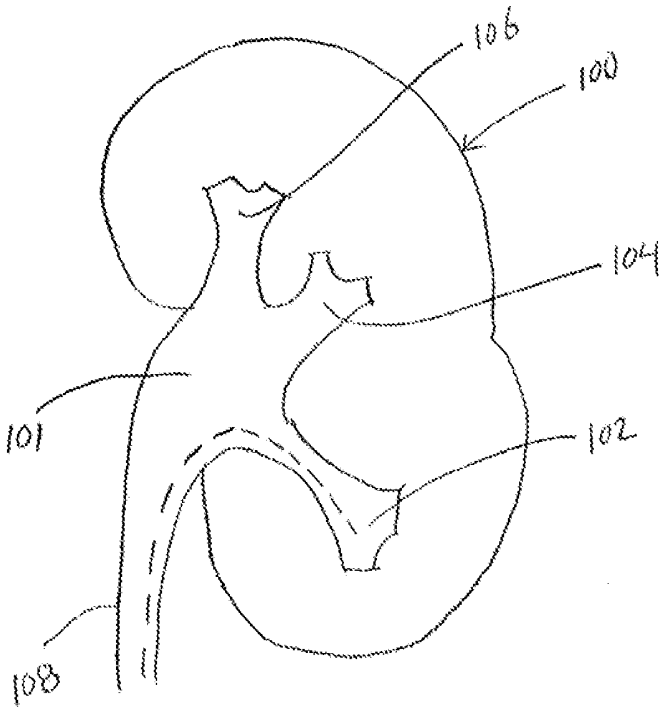
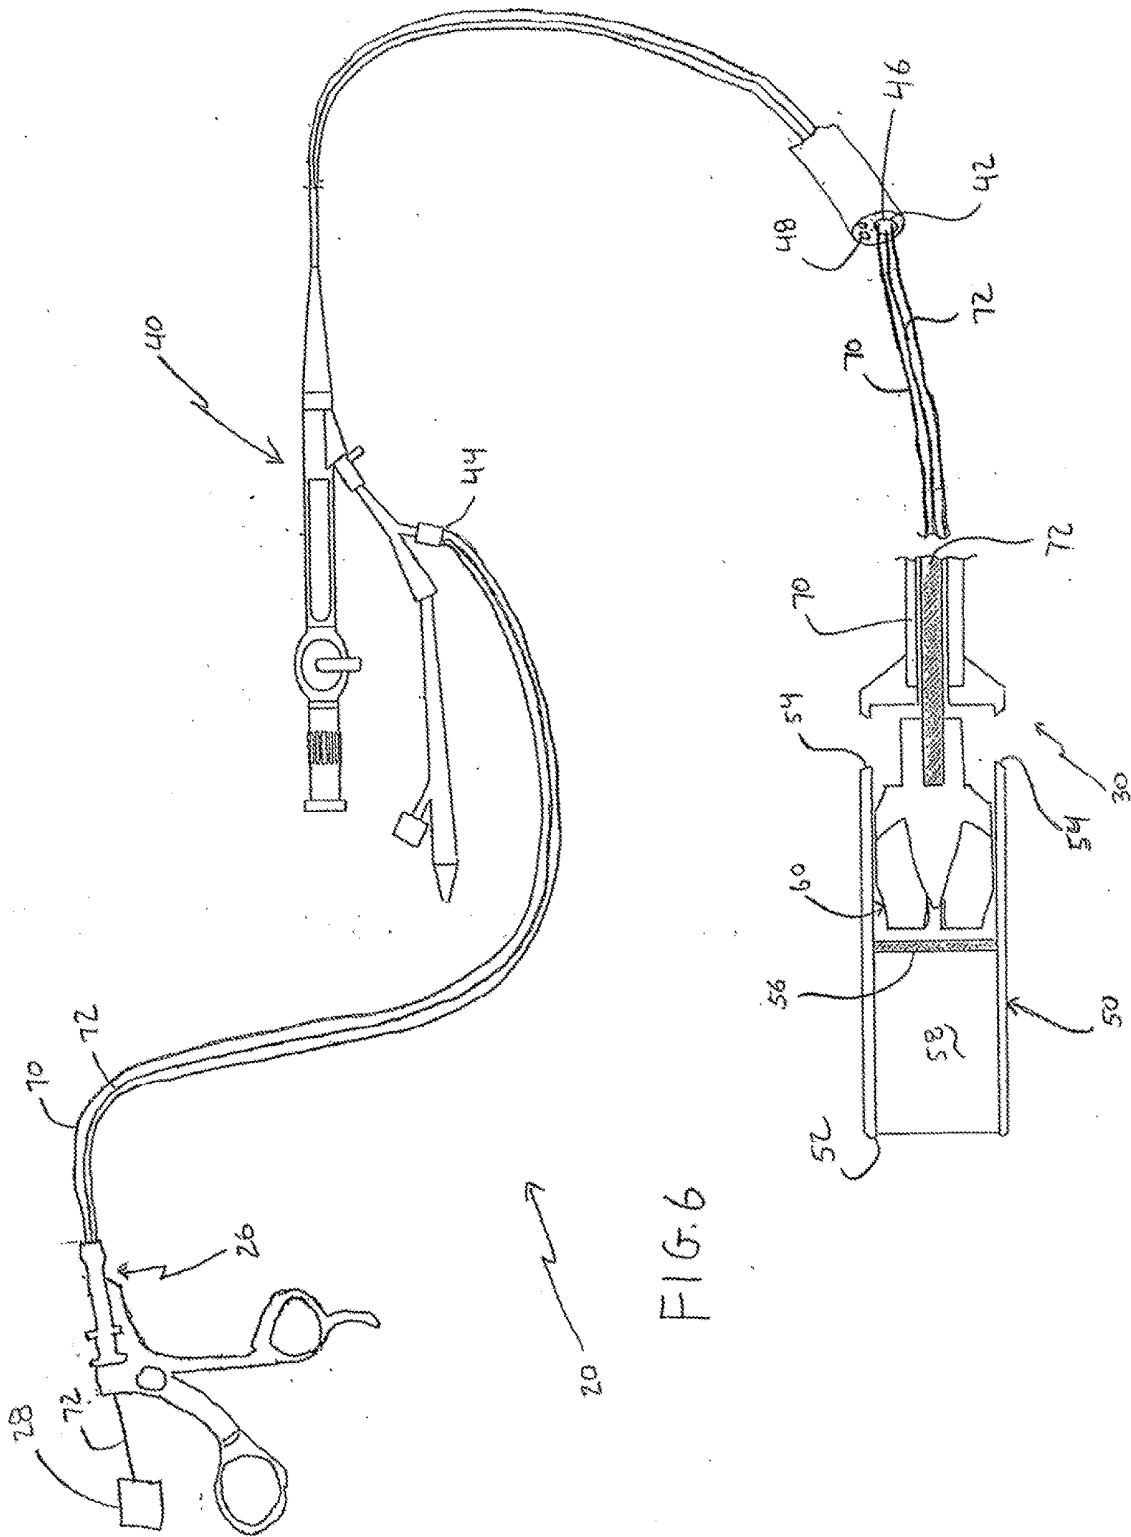


FIG. 5



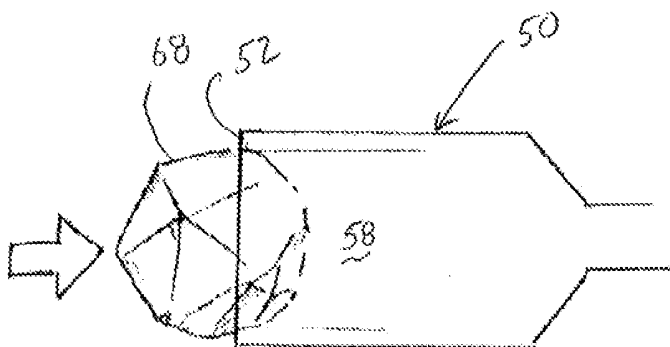


FIG. 7A

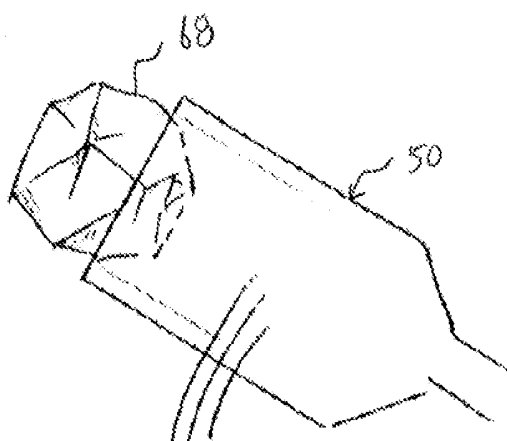


FIG. 7B

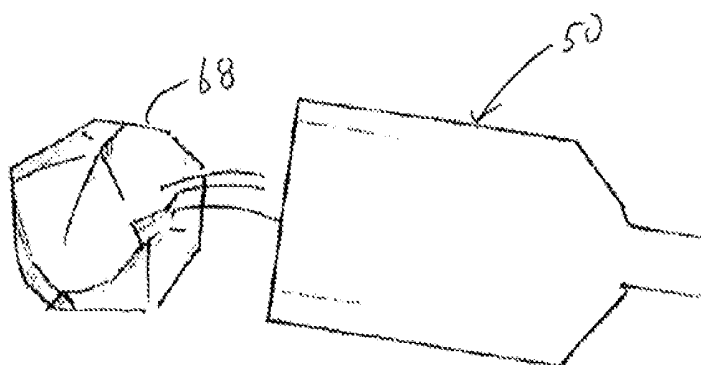


FIG. 7C

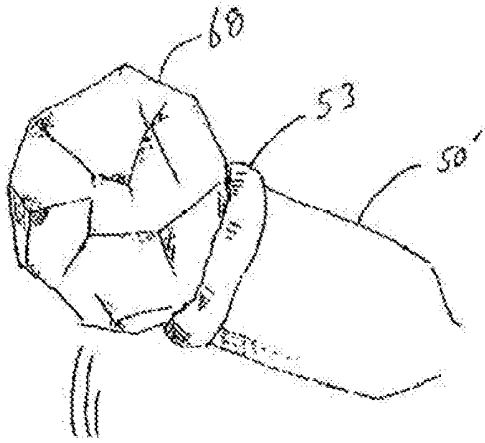


FIG. 9

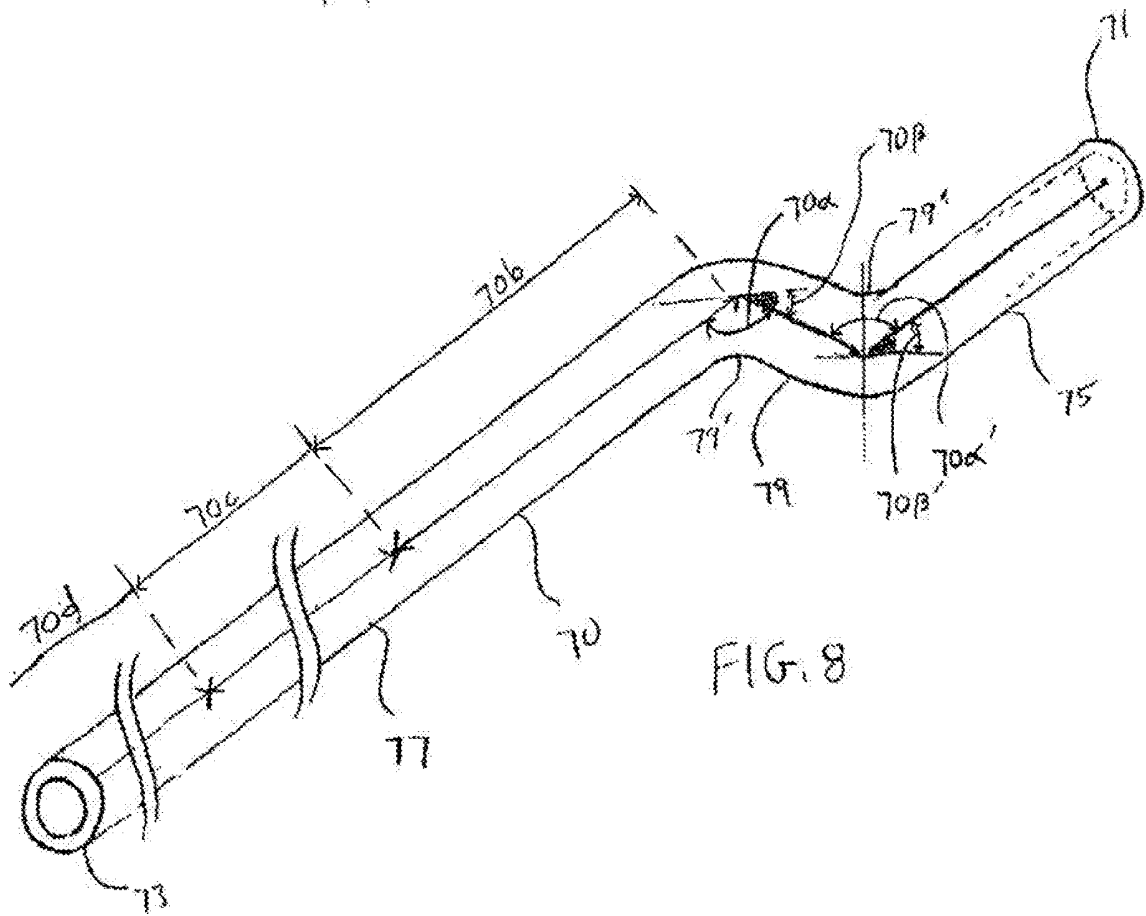
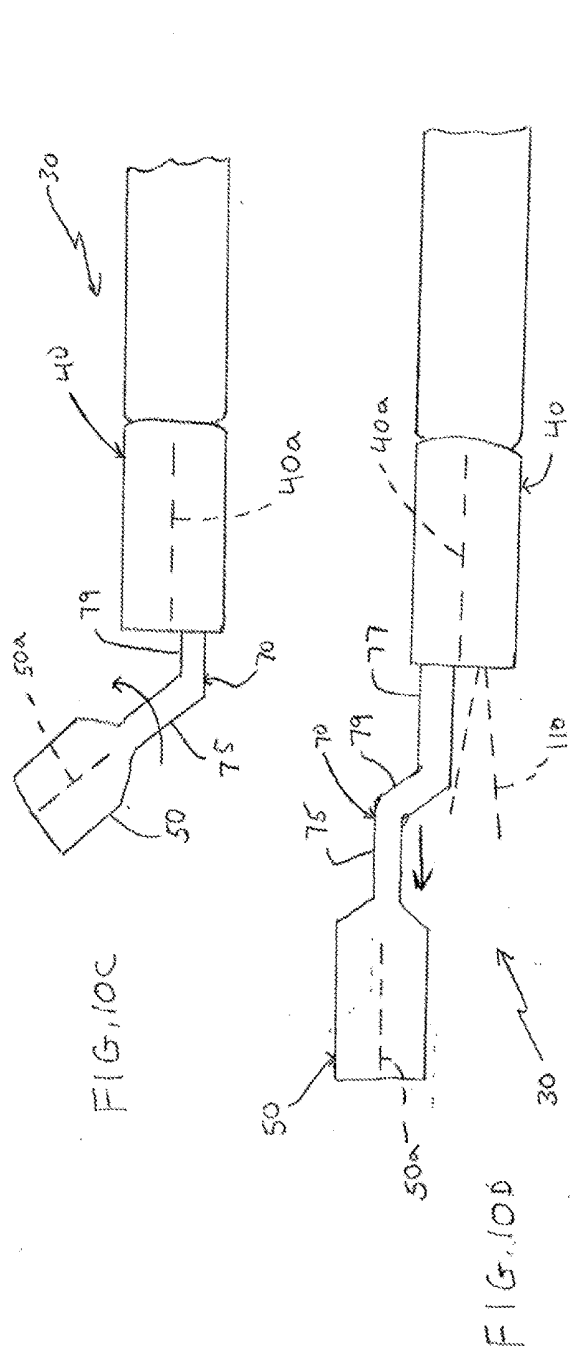
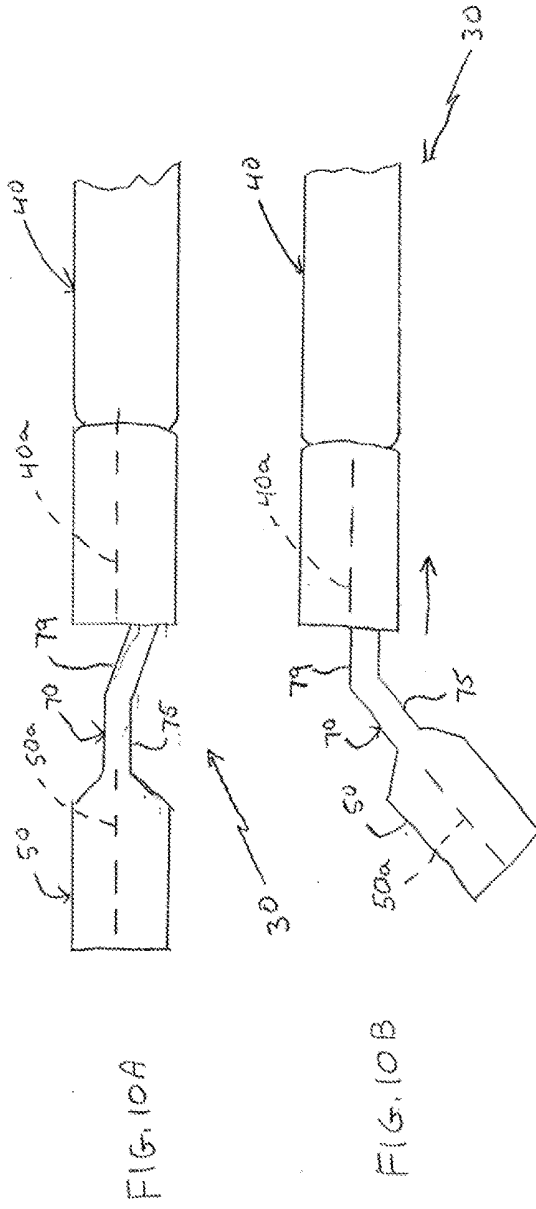


FIG. 8



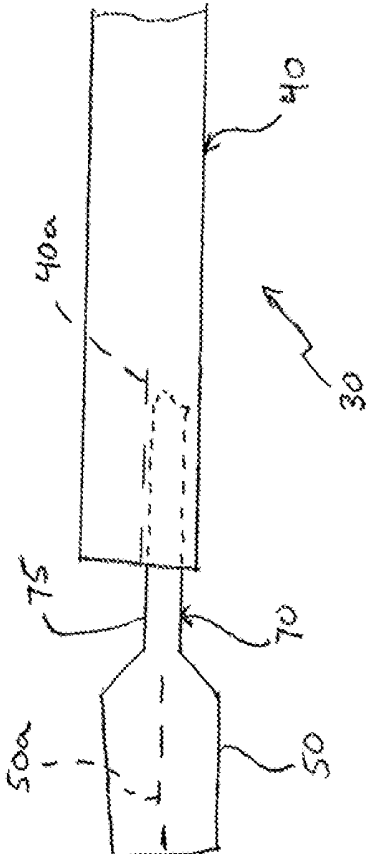
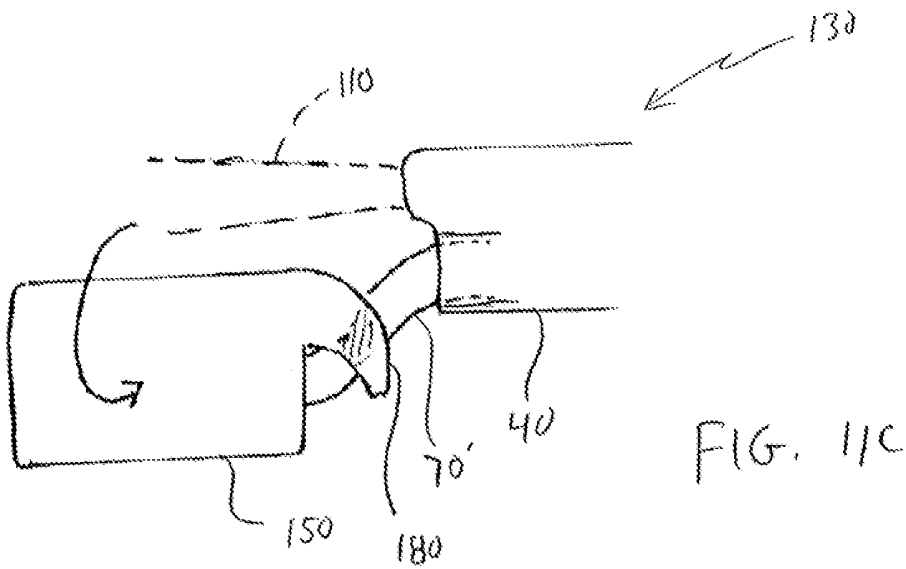
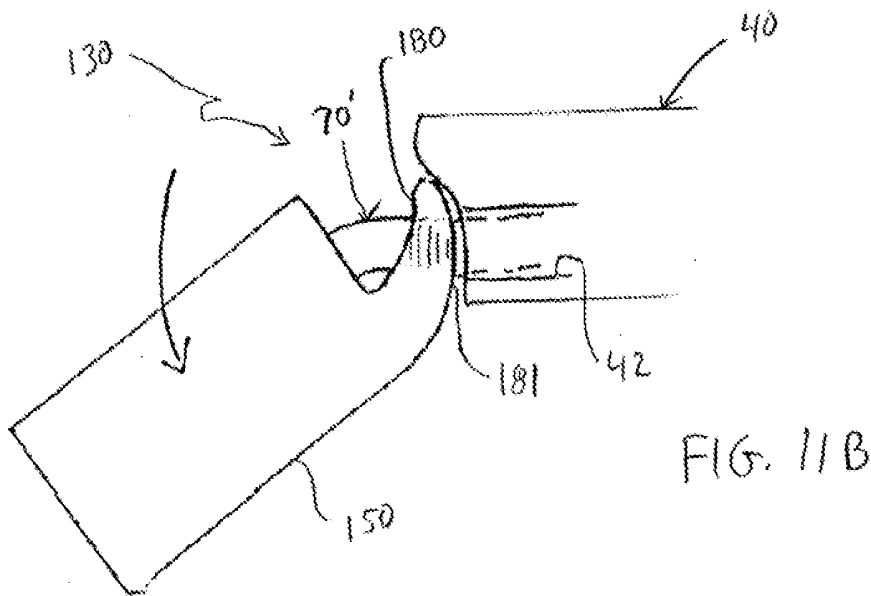
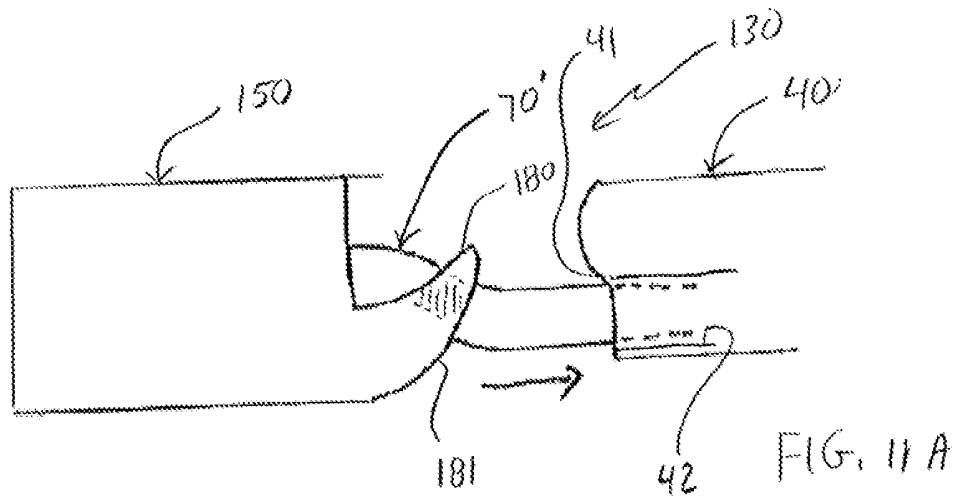
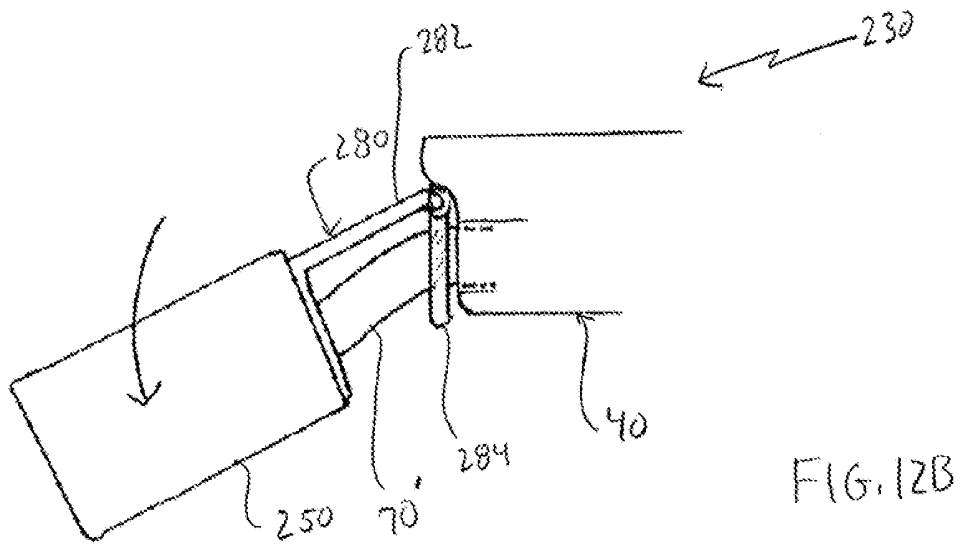
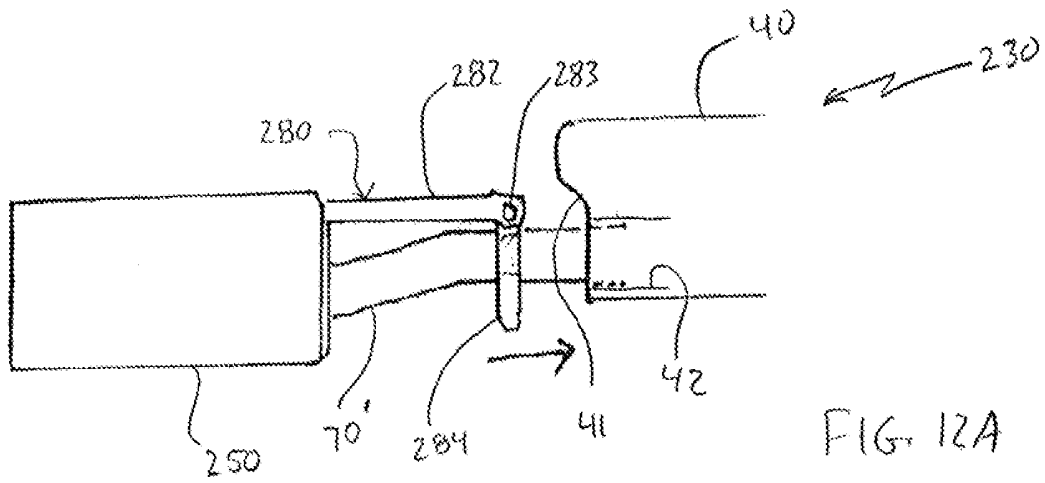
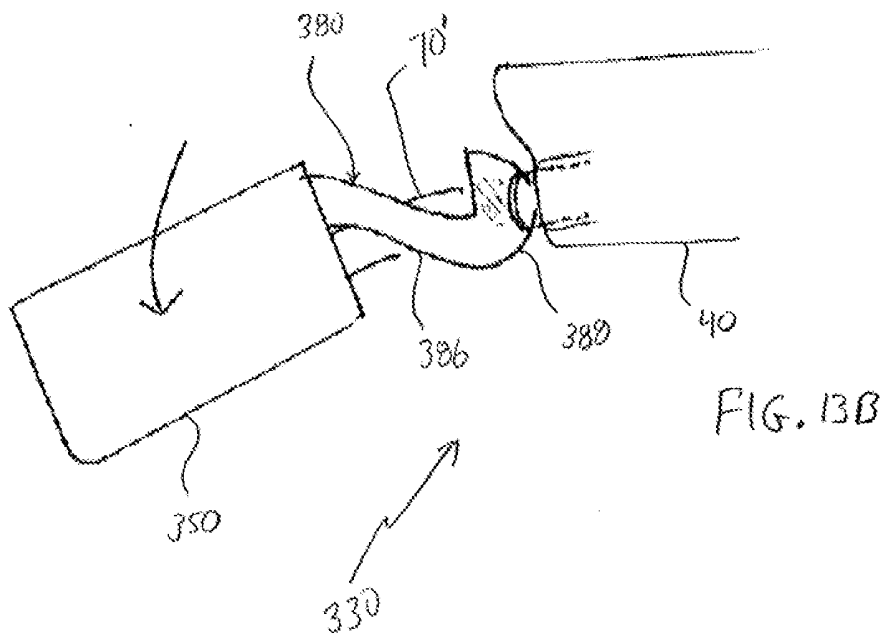
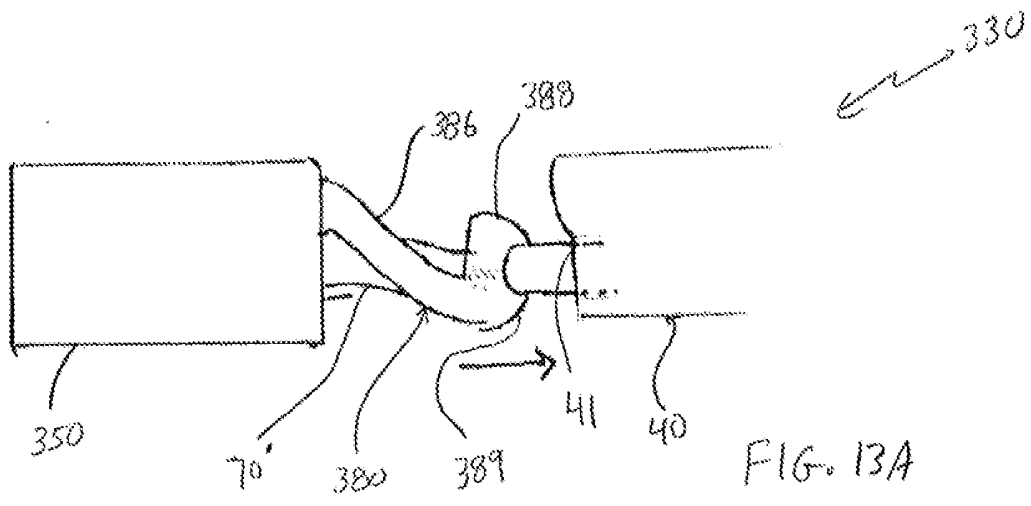
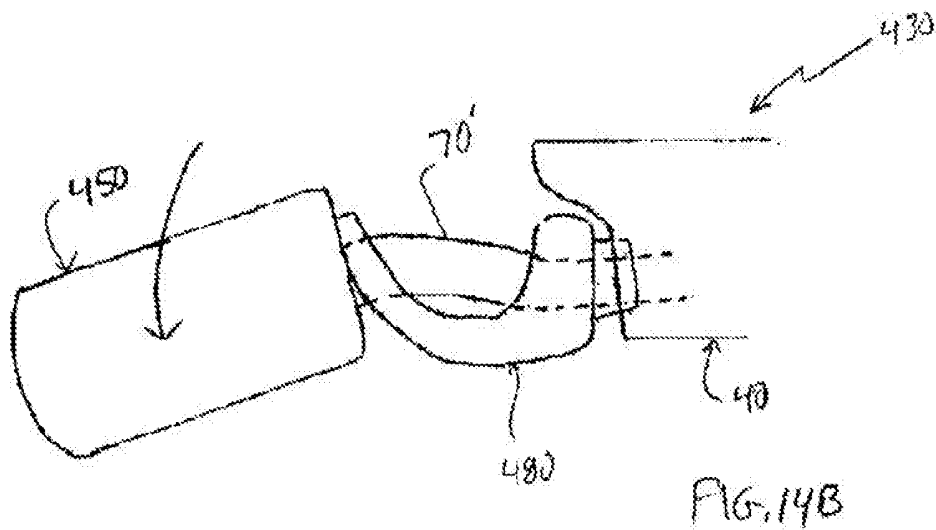
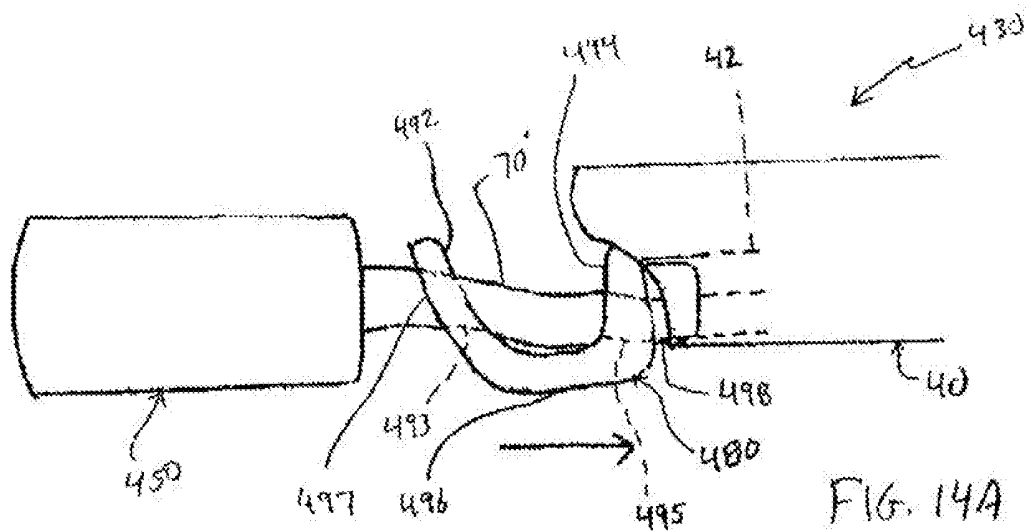


FIG. 10E









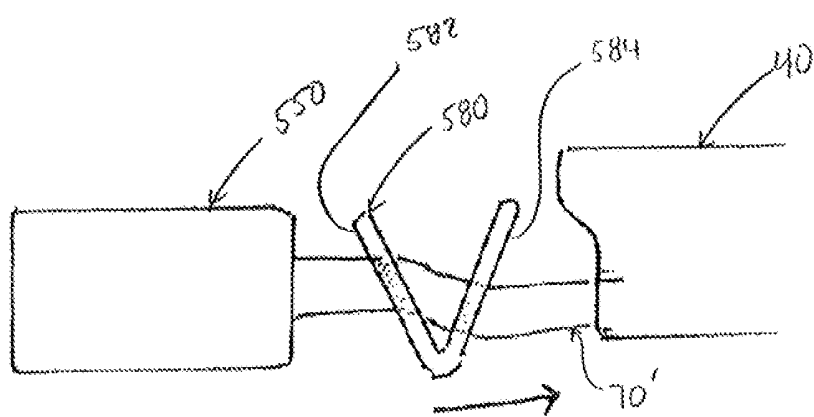


FIG. 15A




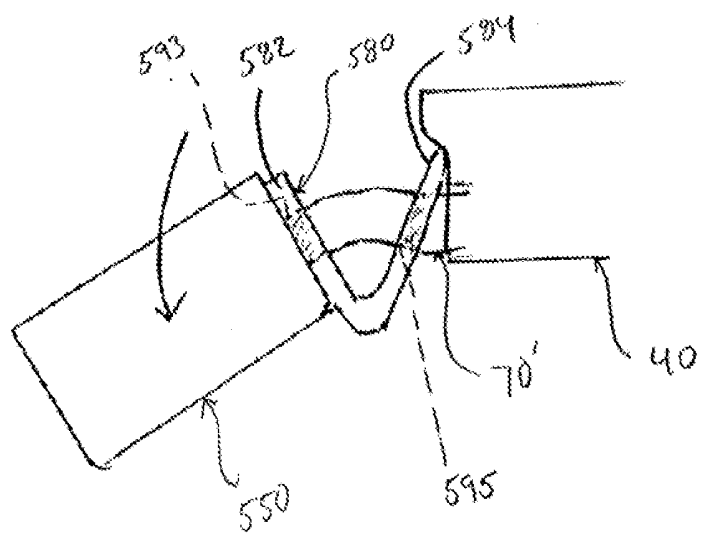


FIG. 15B

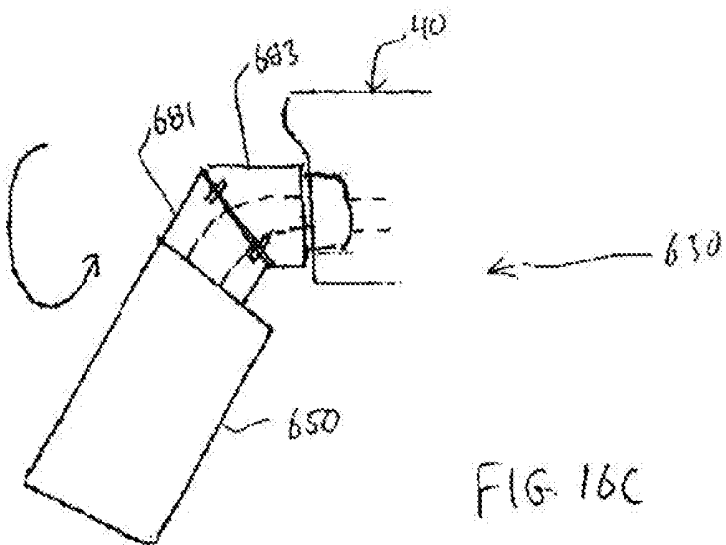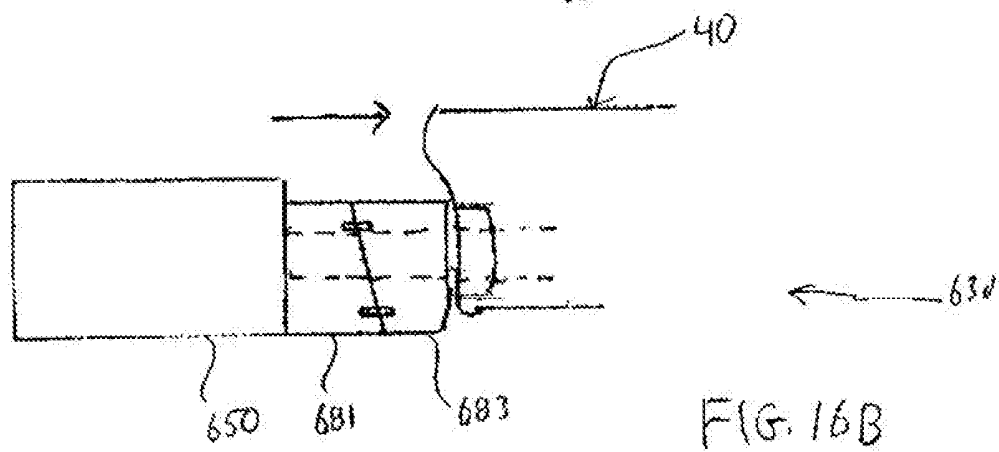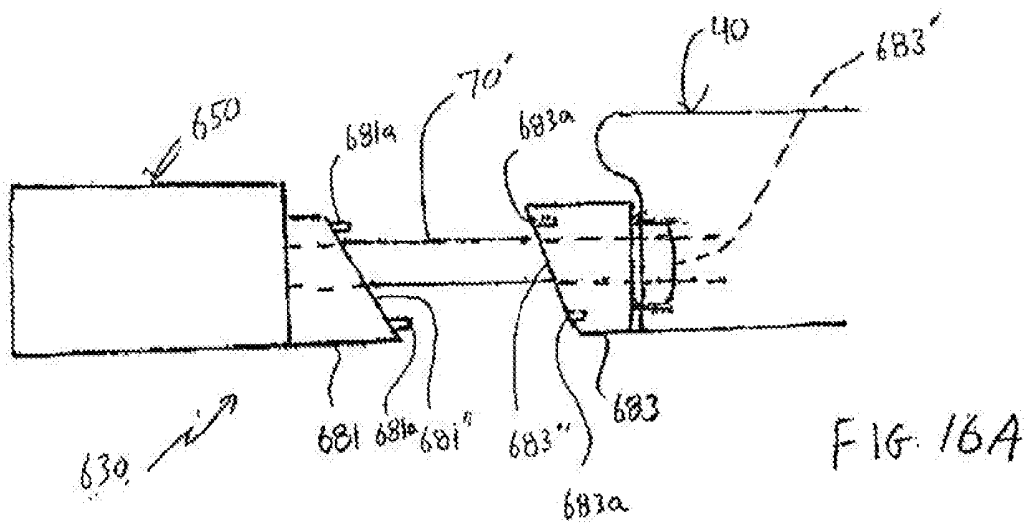

## CALCULUS/CALCULI RETRIEVING DEVICE AND METHOD

### CROSS-REFERENCE TO OTHER APPLICATIONS

[0001] This application is a divisional of U.S. application Ser. No. 14/671,083 filed Mar. 27, 2015 and discloses subject matter related to subject matter described in U.S. application Ser. No. 14/222,021, U.S. application Ser. No. 14/221,954 and U.S. application Ser. No. 14/221,858, the entire content of all four of which is incorporated herein by reference.

### TECHNICAL FIELD

[0002] The present invention generally pertains to methods, systems and devices for retrieving a mass from a human body. More specifically, the invention involves methods, devices and systems for retrieving stone(s) (e.g., calculus or calculi) from a portion of a human body, and moving the retrieved stone(s) to a different location in the living body.

### BACKGROUND DISCUSSION

[0003] The term urinary calculus (e.g., kidney stones and ureteral stones) refers to masses or stones, typically solid particles, that form in the human body and are located in the kidneys and/or the ureter. Calculus can exhibit a variety of chemical compositions including calcium oxalate, calcium phosphate, uric acid, cystine, and struvite.

[0004] Stone disease (e.g., kidney stones and ureteral stones) is a relatively common urological disorder. The presence of calculus in the body can manifest itself in a variety of ways and can produce a number of medical ailments. For example, the presence of calculus in the renal pelvis and/or the renal calix (i.e., the lumen of the kidney) can cause blood in the urine, urinary obstruction, infection, and various degrees of pain ranging from vague flank pain to much more severe pain not capable of being relieved through general pain medication. The presence of stones or calculi in the ureter can result in relatively severe side and back pain, pain below the ribs, and pain that sometimes spreads to the lower abdomen and groin, as well as pain during urination and hematuria.

[0005] Fortunately, many calculi or stones pass out of the body without requiring any specific medical intervention. In those situations where the calculus does not naturally pass out of the body, a medical procedure may be required.

[0006] In the past, three main treatments have been used to treat or address calculus or kidney stones. These include shock wave lithotripsy (ESWL), transurethral lithotripsy or ureteroscopy (URS), and percutaneous nephrouretero lithotripsy (PCNL) which is sometimes also referred to as percutaneous nephrolithotomy (PCN).

[0007] Shock wave lithotripsy is performed as an extracorporeal treatment. This treatment utilizes a machine called a lithotripter that operates by directing ultrasonic or shock waves from outside the body, through the skin and tissue, and at the calculi or stones. Repeated shock waves apply stress to the stones, eventually breaking the individual stones into smaller pieces which can more easily pass through the urinary tract in urine. One benefit associated with shock wave lithotripsy is that it is a rather simple

procedure. But it has been found that there is a relatively high rate of kidney stone recurrence following shock wave lithotripsy.

[0008] Transurethral lithotripsy or ureteroscopy represents one such alternative form of treatment. This treatment involves the use of small fiber optic instrument called a ureteroscope which allows access to the calculus in the ureter or kidney. The ureteroscope can be a rigid ureteroscope or more commonly, a flexible ureteroscope. The ureteroscope allows the medical professional to visualize the stone as the ureteroscope moves along the ureter or enters the kidney by way of the bladder and the urethra. Once the calculus is visualized, a basket-like device is used to grasp smaller stones and remove them. If the calculus is excessively large to remove as a single piece, it can be broken into a smaller pieces by using laser energy.

[0009] The third form of treatment is percutaneous nephrolithotomy. This procedure is often used with relatively larger calculus that cannot be effectively treated with either ESWL or URS. Percutaneous nephrolithotomy involves nephrostomy; making an incision at the appropriate location, needling by paracentesis needle, positioning a guide wire through the paracentesis needle's lumen into the kidney under radiographic guidance, and then expanding perforated site. A nephroscope is then moved into the kidney via nephrostomy to visualize the calculus. Fragmentation of the calculus can be performed using an ultrasonic probe or laser.

[0010] Though these procedures have been commonly used, they are susceptible of certain short comings. For example, the calculus may be located at a place in the living body that is not conducive to treatment by lithotripsy. The calculus may be located in a region of damaged tissue and/or may be located in a small space that is difficult to access with appropriate instrumentation.

### SUMMARY

[0011] One aspect of the disclosure here involves a device for retrieving calculus in a lumen of a living body, wherein the device comprises a shaft an elongated member sized to be positioned in the lumen of the living body, a rotatable impeller positioned inside the elongated member, and a shaft cover. The elongated member includes a suction head housing possessing a distal end, a proximal end and an interior, with the distal end of the suction head housing being open to permit entry of calculus and the proximal end of the suction head housing being closed by a wall through which passes the shaft. The shaft is connected to the rotatable impeller so that the shaft and the rotatable impeller rotate together as a unit. The shaft is connectable to a drive source that is operable to rotate the shaft and the rotatable impeller, with rotation of the rotatable impeller creating suction that draws calculus through the open distal end of the suction head housing and into the interior of the suction head housing. The shaft cover possesses a distal end portion that terminates in a distal end connected to the proximal end of the suction head housing so that the elongated member and the shaft cover axially move and rotate together. The shaft cover also possesses a proximal end portion and covers the shaft. The central axis of the distal end portion of the shaft cover and the central axis of the proximal end portion of the shaft cover are non-coaxial.

[0012] According to another aspect, a device for retrieving calculus in a lumen of a living body comprises: an elongated member sized to be positioned in the lumen of the living

body, the elongated member including a suction head housing disposed on a distal side of the elongated member; a rotatable member positioned inside the elongated member; a shaft connected to the rotatable member so that the shaft and the rotatable member move together as a unit, the shaft being connectable to a drive source to rotate the shaft and the rotatable member, with rotation of the rotatable member creating suction that draws calculus toward the elongated member; a shaft cover possessing a distal end portion having a central axis and a proximal end portion having a central axis, the shaft cover covering the shaft and being connected to the elongated member so that the elongated member and the shaft cover axially move and rotate together; and the central axis of the distal end portion of the shaft cover is offset from the central axis of the proximal end portion of the shaft cover.

[0013] Other features and aspects of the calculus retrieving device and method disclosed here will become more apparent from the following detailed description considered with reference to the accompanying drawing figures in which like elements are designated by like reference numerals.

#### BRIEF DESCRIPTION OF DRAWINGS

[0014] FIG. 1 is a schematic illustration of a system useful to retrieve calculus/calculi, including a retrieving device connected to an operation member (not shown in FIG. 1) through the intermediary of a lumen in an elongated body.

[0015] FIG. 2 is a side view, partially in cross section, of a retrieving device according to an embodiment representing an example of the retrieving device disclosed here.

[0016] FIG. 3 is a front view of the impeller forming a part of the retrieving device shown in FIG. 2.

[0017] FIG. 4 is a schematic illustration of a portion of the human anatomy, including the urinary tract.

[0018] FIG. 5 is a schematic illustration of a human kidney.

[0019] FIG. 6 is a schematic illustration of the retrieving system, including the retrieving device connected to the operation member through the intermediary of an elongated body such as a ureteroscope.

[0020] FIG. 7A illustrates an example of calculus in a living body being retrieved by the retrieving device, FIG. 7B is a schematic illustration of the retrieving device being moved to move the retrieved calculus to a different location in the living body, and FIG. 7C is a schematic illustration of the calculus retrieving device, as the calculus previously retrieved is released.

[0021] FIG. 8 is a prospective view of the shaft cover forming a part of the retrieving device shown in FIG. 1.

[0022] FIG. 9 is a schematic illustration of an embodiment of the retrieving device representing another example of the retrieving device disclosed here.

[0023] FIG. 10A is a side view of the retrieving device outfitted with the shaft cover shown in FIG. 8 according to one operational aspect, FIG. 10B illustrates the retrieving device according to another operational aspect after moving the suction head in the rearward direction to orient the suction head at an angle relative to the elongated body, FIG. 10C illustrates the retrieving device shown in FIG. 10A according to another operational aspect in which the suction head is rotated 180° from the position shown in FIG. 10B, FIG. 10D illustrates the retrieving device shown according to an further operational aspect in which the suction head is

moved forwardly to position the suction head at a location permitting viewing, by way of the ureteroscope, and FIG. 10E illustrates the retrieving device according to an further operational aspect in which the shaft cover is pulled from the position shown in FIG. 10B.

[0024] FIG. 11A is a side view of an embodiment of the retrieving device representing another example of the retrieving device disclosed here in which the retrieving device is configured to angle the suction head relative to the ureteroscope. FIG. 11B illustrates the retrieving device according to another operational aspect after moving the suction head in the rearward direction so that the suction head is angled relative to the ureteroscope, and FIG. 11C illustrates the retrieving device shown in FIG. 11A according to another operational aspect in which the suction head is rotated 180° from the position shown in FIG. 11A.

[0025] FIG. 12A is a side view of an embodiment of the retrieving device representing an additional example of the retrieving device disclosed here in which the retrieving device is configured to angle the suction head relative to the ureteroscope, and FIG. 12B illustrates the retrieving device according to another operational aspect after moving the suction head in the rearward direction so that the suction head is angled relative to the ureteroscope.

[0026] FIG. 13A is a side view of an embodiment of the retrieving device representing another example of the retrieving device disclosed here in which the retrieving device is configured to angle the suction head relative to the ureteroscope, and FIG. 13B illustrates the retrieving device according to another operational aspect after moving the suction head in the rearward direction so that the suction head is angled relative to the ureteroscope.

[0027] FIG. 14A is a side view of an embodiment of the retrieving device representing a further example of the retrieving device disclosed here in which the retrieving device is configured to angle the suction head relative to the ureteroscope, and FIG. 14B illustrates the retrieving device according to another operational aspect after moving the suction head in the rearward direction so that the suction head is angled relative to the ureteroscope.

[0028] FIG. 15A is a side view of an embodiment of the retrieving device representing another example of the retrieving device disclosed here in which the retrieving device is configured to angle the suction head relative to the ureteroscope, and FIG. 15B illustrates the retrieving device according to another operational aspect after moving the suction head in the rearward direction so that the suction head is angled relative to the ureteroscope.

[0029] FIG. 16A is a side view of an embodiment of the retrieving device representing another example of the retrieving device disclosed here in which the retrieving device is configured to angle the suction head relative to the ureteroscope, FIG. 16B illustrates the retrieving device according to another operational aspect after moving the suction head in the rearward direction, and

[0030] FIG. 16C illustrates the retrieving device shown in FIG. 16B according to another operational aspect in which the suction head is rotated 180° from the position shown in FIG. 16C.

#### DETAILED DESCRIPTION

[0031] Set forth below is a detailed description of features and aspects of the retrieving system, device and method described here as examples of the disclosed invention. The

methods, systems, and devices disclosed here for retrieving have particularly useful application to retrieve calculus/calculi located in the living body, including calculus/calculi located in the ureter (ureter stones) and calculus located in the kidneys (kidney stones), though the methods, systems and devices are not limited in this regard. The references below to calculus should be understood to refer to calculus in the singular as well as calculi in the plural.

**[0032]** Generally speaking, the calculus removing/retrieving device disclosed here, as represented by the several embodiments representing examples of the inventive retrieving device (and method), is configured to be positioned inside a living body at a position which will allow the retrieving device to suck-in or draw-in calculus to be retrieved. Set forth below is a detailed description of features and aspects of the calculus retrieving system, including a calculus retrieving device, and method described here by way of various embodiments representing examples of the disclosed inventions. The systems, devices and methods disclosed here for retrieving calculus have particular useful application to retrieve calculus located at places in the human body, where removal of the calculus may be difficult.

**[0033]** Generally speaking, the calculus retrieving device disclosed here, as characterized by the several embodiments representing examples of the inventive calculus retrieving device (and method), is configured to be positioned inside a living body, at a position adjacent the location of calculus to be retrieved from the living body and moved to a new (different) location in the living body. The calculus (stone/stones) is drawn towards the retrieving device by creating a suction force in the retrieving device. After the calculus is retrieved, the calculus is retained or held by the retrieving device, and the retrieving device is moved to the new location in the living body at which the retrieved calculus is to be repositioned. The retained calculus is subsequently released at the new location in the living body. Appropriate procedures (e.g., lithotripsy) can then be performed with respect to the calculus which has been moved

**[0034]** Turning now to the drawing figures, FIG. 1 illustrates, in a schematic fashion, a system 20 for retrieving and moving calculus (stone or stones) located in a living body. The system 20 includes a retrieving device 30 and an elongated body 40 possessing a lumen to deliver the retrieving device 30 to the desired place in the living body. In this illustrated embodiment representing one example of the system disclosed here, the elongated body 40 is a ureteroscope. The ureteroscope includes a lumen or instrument channel 42, which receives a portion of the retrieving device 30, as will be described in more detail below. During use of the retrieving device 30, the ureteroscope 40 is introduced into the living body by way of a ureteral access sheath 24. The ureteroscope 40 passes through a lumen 28 in the ureteral access sheath 24.

**[0035]** Additional details and features associated with the calculus retrieving device 30 can be seen with reference to FIGS. 1, 2 and 3. The calculus retrieving device 30 includes a suction head 50 that includes an elongated body or housing 51 having an open distal end 52. The housing 51 is a tubular housing possessing a lumen 54 defining an interior of the housing 51. The housing 51 can be configured as a cylindrical elongated body or housing.

**[0036]** The retrieving device 30 also includes a rotatable suction-producing part located inside the housing 51. In the illustrated embodiment, the rotatable suction-producing part

is in the form of an impeller 60. As shown in FIGS. 1 and 3, the impeller is positioned in the housing 51 at a location spaced away from (i.e., proximally or rearwardly) the open distal end 52. An example of the impeller 60 is illustrated in FIG. 3. The impeller 60 includes a plurality of circumferentially spaced apart fins or blades 62 that are fixed to a central hub 64. The fins or blades 62 of the impeller 60 may be twisted fins or blades. The hub 64 is fixed or connected to a rotatably driven shaft 72 so that the shaft 72 and the impeller 60 rotate together as a unit. The impeller 60 is configured so that rotation of the impeller 60 in one rotational direction produces suction in the lumen 54 (in the interior) of the housing 51, while rotation of the impeller 60 in the opposite rotational direction produces the opposite result, namely an outwardly directed force out of the lumen 54. The blades 62 of the impeller 60 shown in FIGS. 2 and 3 are preferably twisted from the distal tip of the blades 62 (radially outermost tip of the blades) toward the bottom portion of the impeller where the blades are mounted. When the direction of the impeller rotation is the same as the twist direction of the blades 62, a suction force is generated. This direction of rotation of the impeller is referred to as overspin direction.

**[0037]** The drive shaft 72 that is connected to the hub 64 of the impeller 60 is positioned inside of and covered by a shaft cover 70. In the illustrated embodiment, the drive shaft 72 is completely covered by the shaft cover 70. The shaft cover 70 is fixed to the housing 51 forming the suction head 50 so that movement of the shaft cover 70 results in movement of the suction head 50 (including the housing 51 and the impeller 60).

**[0038]** The housing 51 forming the suction head 50 includes a plurality of circumferentially spaced apart openings or through holes 54. These openings or through holes 54 are positioned closer to the proximal end of the housing 51 than the distal end of the housing 51. These openings or through holes 54 form an exhaust path during operation of the retrieving device, as will become more apparent from the description below. That is, liquid (e.g., water) which has been drawn into the housing 51 of the suction head 50 during operation of the retrieving device 30 is exhausted or discharged out of the suction head 50 by way of the openings or through holes 54.

**[0039]** The suction head 50 further includes a filter 56 located inside the housing 51 at a position between the distal end of the impeller 60 and the open distal end 52 of the suction head 50. This filter 56 is a disc-shaped mesh member that allows the passage of fluid (e.g., liquid such as water), while also preventing the passage of calculus which has been retrieved through operation of the retrieving device 30. The filter 56 possesses an outer periphery (outer circumferential surface) in contact with the inner periphery of the suction head 50. The filter 56 is positionally fixed within the interior of the housing 51 forming the suction head 50.

**[0040]** The suction head 50 also includes a retrieval space 58 located between the filter 56 and the open distal end 52 of the housing 51. As will be described in more detail below, this retrieval space 58 is configured to receive calculus which has been retrieved as a result of the operation of the retrieving device 30.

**[0041]** During operation of the retrieving device 30, the suction head 50 is located at a position in a living body to retrieve calculus. That is, the suction head 50 is positioned relative to the calculus to be retrieved such that during

operation of the retrieving device 30, the calculus will be drawn towards (sucked towards) the suction head 50. When the suction head 50 is properly positioned relative to the calculus to be retrieved, the impeller 60 is rotatably driven through operation of a drive device connected to the drive shaft 72. The drive device rotates the drive shaft 72, which in turn rotates the impeller 60. The impeller 60 is rotatably driven in a direction to create a suction in the interior of the housing 51 that draws calculus toward the open distal end 52 of the suction head 50. The suction force created by the rotation of the impeller 60 draws relatively smaller calculus (schematically shown in FIG. 1 and identified as 68) through the open distal end 52 of the suction head and into the retrieval space 58 in the housing 51. The suction force created by the rotation of the impeller 60 can also draw relatively larger calculus into contact with the distal end of the suction head 50. That is, calculus possessing an outer dimension larger than the size of the open distal end 52 of the suction head 50 can nevertheless be drawn towards the suction head 50 and retained by the suction head 50 by creating sufficient suction force in the interior of the housing 51 that holds the relatively larger calculus in contact with the distal end of the suction head 50.

[0042] Thus, by positioning the suction head 50 in the living body so that the open distal end 52 of the suction head 50 is located at a position that will allow the calculus (i.e., calculus to be retrieved) to be drawn-into or sucked into the retrieval space 58 upon rotational operation of the impeller 60, it is possible to retrieve calculus and hold the retrieved calculus either in the retrieval space 58 or at the distal end of the suction head 50. As the impeller 60 is rotated to draw calculus toward the suction head 50, liquid (e.g., water) is drawn into the retrieval space 58 by way of the distal open end 52 of the suction head 50. This liquid is passed through the filter 56, and is exhausted or discharged outside the housing 51 of the suction head 50 through the openings or through holes 54. On the other hand, the filter 56 is sized to ensure that calculus which is drawn into the retrieval space 58 of the suction head 50, does not pass through the filter 56. The rotational operation of the impeller 60 thus causes liquid flow in which liquid enters the distal open end 52 of the suction head 50, passes through the filter 56, and exits through the through holes or openings 54 in the suction head 50. Depending upon operation of the impeller 60, the liquid exhausted through the openings or through holes 54 can also be at least partially drawn back into the interior of the suction head 50, thus creating a rather turbulent and continuous liquid cycle in which the same liquid is repeatedly drawn into the suction head, exhausted through the suction head 50, drawn into the suction head, etc. This turbulent and continuous liquid cycle can help facilitate retrieval of calculus in the retrieval space 58 of the suction head 50. This is because the suction force per rotation of the impeller is increased. In addition, the calculus tends to float, making it easier to draw-in or retrieve the calculus. When drawing-in calculus in a narrow lumen in a living body (e.g. ureter), the continuous liquid cycle helps prevent fluid surrounding calculus from drying up.

[0043] Set forth next is a description of contexts in which the system for retrieving calculus disclosed here can be used, as well as a description of a manner of operation of the system for retrieving calculus. It is sometimes necessary or desirable to break-up calculus located in a living body. For instance, calculus that is relatively small can be pulled out

of the body, but if the calculus is relatively large (e.g., larger than the ureter diameter), it is not possible to remove the calculus from the living body. In such situations, it would be desirable to break-up the calculus into smaller size pieces. This can oftentimes be accomplished using lithotripsy. But circumstances may make it difficult to perform lithotripsy to break-up calculus in the living body. For example, the calculus may be located at a place where damaged tissue exists, for example in a portion of the ureter in which there is damaged tissue. Alternatively, the calculus may be located in a portion of the living body (e.g., ureter) that is rather small in size (i.e., a narrow space) and difficult to access with appropriate instrumentation and equipment for performing lithotripsy (e.g., a lower calix). The approach described here involves retrieving the calculus, moving the retrieved calculus to a new (different) location which presents a larger space (e.g., the kidney or an upper calix) to perform lithotripsy or which presents a region where there is normal (non-damaged tissue) tissue.

[0044] The retrieving device and system disclosed here are configured to retrieve calculus from one place in the living body, move the retrieved calculus to a new (different) place where, for example, lithotripsy can be more easily performed to break-up the calculus, and then release the retrieved and moved calculus at the new location. By way of example, and with reference to FIG. 4, it is possible to retrieve calculus at the location X in the ureter (representing an example of a region of narrow size or damaged tissue) and move the retrieved calculus to the position X' in the ureter (representing an example of a region of larger size or normal non-damaged tissue). It is also possible to retrieve calculus at the location Y (representing an example of a region of narrow size or damaged tissue) and move the retrieved calculus to the position in the kidney (representing another example of a region of larger size or normal non-damaged tissue).

[0045] To retrieve and move the calculus, the retrieving system 20 shown in FIG. 6 is used. Specifically, the calculus retrieving device 30 is used, together with the operating member 26 and the ureteroscope 40. The operating member 26 is connected to the shaft cover 70, so that operation of the operating member 26 causes the shaft cover 70 to move. That is, the operation of the operating member 26 causes the shaft cover 70 to axially move, which in turn causes the suction head 50 (including the impeller 60 and the filter 56) to also axially move. FIG. 6 schematically illustrates that the shaft 72 positioned within and extending along the axial length of the shaft cover 70 is connected to a driving source 28. Operation of the driving source 28 rotates the shaft 72, which in turn rotates the impeller 60 positioned in the housing 51 of the suction head 50 of the calculus retrieving device 30. As shown in FIG. 6, the shaft cover 70 and the shaft 72 extend from the operating member 26, enter an inlet 44 of the instrument channel 42 in the ureteroscope 40, pass through the ureteroscope 40, and exit at an outlet at the distal end portion 46 of the ureteroscope 40.

[0046] In use, the shaft cover 70 is connected to the housing 51 of the suction head 50, and the proximal end of the shaft cover 70 and the shaft 72 are inserted into the outlet of the instrument channel 42 at the distal end portion 46 of the ureteroscope 40. The shaft cover 70 and the shaft 72 are pushed through the lumen (instrument channel 42) in the ureteroscope 40 until the proximal end of the shaft cover 70 and the proximal end of the shaft 72 exit out of the inlet 44

of the ureteroscope. The proximal end of the shaft 72 is then connected to the driving device 28, while the proximal end of the shaft cover 70 is fixed to the operating member 26.

[0047] The ureteroscope 40 is preferably a flexible ureteroscope. The ureteroscope 40 includes a viewing system that includes an objective lens 48 schematically illustrated in FIGS. 1 and 6. In a known manner, this provides a field of view for the user or operator to facilitate carrying out the procedure involving locating calculus, retrieving the calculus, moving the calculus to the new location and releasing the calculus at the new location.

[0048] Next, the retrieving device 30, arranged distally of the ureteroscope 40 as shown in FIG. 6, is introduced into the living body. This can be accomplished by way of the ureteral access sheath 24 schematically shown in FIG. 1. Once the retrieving device 30 is introduced into the living body, the retrieving device 30 is advanced to the desired position within the living body through operation of the operating member 26. The retrieving device 30 is preferably positioned so that the open distal end 52 of the suction head 50 is positioned near to or adjacent the calculus/calculi to be retrieved. That is, the retrieving device 30 is moved to locate the open distal end 52 at a position relative to the calculus to be retrieved such that during operation of the suction head 50 (rotation of the impeller 60), the resulting suction draws calculus toward the suction head 50.

[0049] After the suction head 50 is properly positioned relative to the calculus to be retrieved, the driving source 28 (e.g., a geared motor) is operated to rotate the impeller 60 in a direction which causes suction to be created in the interior of the suction head 50. This causes the calculus to be sucked or drawn toward the distal open end 52 of the suction head and into the retrieval space 58 at the distal end portion of the suction head 50 (assuming the calculus is sufficiently small). As described above, as the calculus is drawn towards the suction head 50 (into the retrieval space 58), liquid is also drawn into the suction head 50. This liquid is able to pass through the filter 56, and is exhausted through the openings 54. On the other hand, the filter prevents the calculus which has been drawn into the retrieval space 58 from passing through the filter 56. The retrieved calculus which has entered the retrieval space thus remains in the retrieval space 58.

[0050] FIGS. 7A-7C depict three aspects of the method disclosed here involving retrieving calculus 68 through operation of the suction head 50 (FIG. 7A), moving the suction head 50 and the retrieved calculus 68 to a new location (FIG. 7B), and releasing the calculus 68 (FIG. 7C). FIG. 7A generally illustrates calculus 68 that has been drawn towards the suction head 50 and is held against the open distal end 52 of the suction head 50. In this illustrated version, the retrieved calculus 68 possesses an outer dimension greater than the inner dimension of the lumen (retrieval space 58) in the suction head 50. This possibility is only for illustrative purposes, and it is to be understood that a similar operation is performed to retrieve smaller calculus that are able to pass through the open distal end 52 of the suction head and be positioned inside the retrieval space 58, such as schematically illustrated in FIG. 1.

[0051] The retrieval of the calculus 68, the retention of the calculus 68 during movement of the suction head 50, and the release of the retrieved calculus can be accomplished by controlling various operational parameters of the suction head 50. These operational parameters include the rotation

operation of the impeller 60 (ON/OFF), the rotation speed of the impeller 60, and the rotation direction of the impeller. That is, by varying the rotation operation, the rotation speed and the rotation direction of the impeller 60, it is possible to control the retrieval, the retention and the release of the calculus.

[0052] During retrieval of the calculus, the impeller 60 is preferably rotated (i.e., the rotational operation is ON), is rotated at a relatively high speed (e.g., 15,000 rpm-20,000 rpm), and is rotated in the overspin direction intended to create suction in the suction head 50. The calculus 68 is thus drawn toward the open distal end 52 of the suction head 50. If the calculus 68 is smaller than the open distal end 52 of the suction head 50, the calculus 68 will enter the retrieval space 58 as shown in FIG. 1. If the calculus 68 is larger than the open distal end 52 of the suction head 50, the calculus 68 will be held against the distal end of the suction head as shown in FIGS. 7A-7C.

[0053] After the calculus 68 has been retrieved, it is necessary to retain the retrieved calculus 68 in the retrieval space 58 of the suction head 50 or against the distal end of the suction head 50 while moving the suction head 50 to transport the retrieved calculus 68 to the new (different) location. To retain the retrieved calculus 68, the driving device 28 continues to operate (i.e., the rotational operation is ON) so that the impeller 60 continues rotating. The rotation direction of the impeller 60 is the same as the rotation direction of the impeller during retrieval of the calculus. In addition, the rotation speed of the impeller 60 can be the same relatively high speed as the rotation speed of the impeller 60 during retrieval of the calculus/calculi, or can be a slightly slower rotation speed (e.g., 12,000 rpm-15,000 rpm).

[0054] While operating the suction head in the above described manner to retain the retrieved calculus 60, the suction head 50 is moved through operation of the operating member 26 to position the open distal end 52 of the suction head 50 at the new location where the retrieved calculus is to be released. When the suction head reaches this position, it is now necessary to operate the suction head 50 to release the calculus 68. To do this, the operator turns off the operation of the driving source 28 so that the retention power disappears and then the retrieved calculus 60 drops from the open distal end 52 of the suction head 50 naturally. In this rotation-OFF state, the retrieved calculus 60 retained in the retrieval space 58 can be rather easily released by small movement of the suction head 50. In the situation that the release of the calculus 68 should be controlled more exactly or accurately, or the retrieved calculi 60 are difficult to release from the retrieval space 58 because the calculi 60 may be jammed in the retrieval space 58, the operator can change the operation of the driving source 28 so that the driving source rotates the shaft 72 and the impeller 60 in the direction opposite the rotational direction of the impeller and the shaft during retrieval and retention of the calculus/calculi. That is, the impeller 60 is operated in the backspin direction. The rotational speed of the impeller 60 during release of the calculus is preferably slower than the rotational speed of the impeller 60 during retention of the calculus 68 when the suction head 50 is being moved to the new location.

[0055] After releasing the retrieved calculus 68, the retrieving device 30 is removed from the living body, or is moved to a position in the living body to retrieve other calculus.

[0056] As described above, the calculus is preferably retrieved from a portion of the living body which is not well suited to removing the calculus and which does not lend itself to the use of lithotripsy. The use of the retrieving device 30 thus allows the calculus to be retrieved and moved to another location at which lithotripsy can be used to break-up the calculus into smaller pieces so that the smaller pieces can either be removed from the body naturally or by use of appropriate instrumentation. The description above describes use of the retrieving device 30 to retrieving calculus and moving the retrieved calculus to a new location in the living body. But the retrieving device disclosed here is not limited to this manner of use. For example, it is possible to use the retrieving device 30 as an instrument for removing calculus from a living body.

[0057] FIG. 9 illustrates a slight variation on the configuration of the suction head described above and illustrated in FIGS. 1, 2 and 6. The embodiment of the suction head 50' illustrated in FIG. 9 includes a gel-like material 53 that is located at the open distal end of the suction head 50'. The gel-like material 53 constitutes a compressible member 53 that helps to facilitate the retention of the calculus 68 on the suction head so that, for example, the calculus 68 does not become separated from the suction head while the calculus is being conveyed to the new location. The gel-like material 53 provides a greater area of contact with the retrieved calculus 68 than would otherwise be the case. Examples of the gel-like material 53 include silicone, soft rubber and polyurethane. The gel-like material 53 can be used when it is expected that the size of the calculus 68 being retrieved is larger than the opening at the distal end of the suction head 50'. The gel-like material can also be provided at the end of the suction head if small calculus that enter the retrieval space are being retrieved.

[0058] Another aspect of the retrieving device disclosed here is the ability of the retrieving device to retrieve calculus located in regions of the living body that are highly curved and require significant and severe manipulation to reach. The retrieving device includes a particularly configured shaft cover 70 covering the shaft 72. As described above, the distal end of the shaft cover 70 is connected or fixed to the suction head. FIG. 1 generally illustrates the configuration of the shaft cover 70, while FIG. 8 illustrates the configuration of the shaft cover in more detail.

[0059] Referring to FIG. 8, the shaft cover 70 includes a distal section 75, a proximal section 77 and an intermediately located bent section 79 positioned between the distal section 75 and the proximal section 77. In the illustrated embodiment, the distal section 75 and the proximal section 77 are linearly extending (straight) sections. The intermediately located bent section 79 is bounded on opposite ends by respective bends 79'. The distal section 75 extends from the distal end 71 of the shaft cover 70 to the intermediately located bent section 79, and the proximal section 77 extends from the proximal end 73 of the shaft cover 70 to the intermediately located bent section 79. The bent section 79 is a stiff bent section, meaning that if the bent section 79 is not surrounded by or influenced by a rigid lumen, the bent section 79 is always bent, by virtue of the bends 79', relative to the proximal section 77 and the distal section 75. That is,

in the absence of a force or load (external or internal) applied to the bent section, the bent section 79 remains bent. On the other hand, when the bent section 79 is inserted into or positioned in the instrument channel 42 of the ureteroscope, a force or load is applied to the bent section 79 by the straight instrument channel 42 and so the shape of the section 79 is changed from bent to straight (i.e., the bent section 79 is straightened out). When the bent section 79 located in the instrument channel 42 of the ureteroscope is pulled out of the instrument channel 42, the bent section 79 automatically returns to its bent configuration.

[0060] The distal end 71 of the shaft cover 70 is connected or fixed to the suction head 50 while the proximal end 73 of the shaft cover 70 is connected to the operating member 26. In the illustrated embodiment, the central axis of the distal section 75 and the central axis of the proximal section 77 are parallel to one another, but offset from one another so that the proximal section 77 and the distal section 75 are not coaxial.

[0061] FIG. 8 shows that the proximal section 77 of the shaft cover 70 includes three portions, namely the distal portion 70b of the proximal section 77, the intermediate portion 70c of the proximal section 77, and the proximal portion 70d of the proximal section 77. The distal portion 70b of the proximal section 77 is preferably made of a material that is relatively stiff or rigid. The purpose for this relatively stiff or rigid material is to keep the tip positioned position so that the suction head 50 does not bow under its own weight. Appropriate material can be rubber or plastic material. The intermediate section 79 and the distal section 75 of the shaft cover 70 are preferably also made of relatively stiff or rigid material. The intermediate section 79 and the distal section 75 of the shaft cover 70 can be fabricated from the same material forming the distal portion 70b of the proximal section 77.

[0062] The intermediate portion 70c of the proximal section 77 is preferably made of a relatively soft material. The material forming the intermediate portion 70c of the proximal section 77 is softer than the material forming the distal portion 70b of the proximal section 77. The material forming the intermediate portion 70c of the proximal section 77 is thus a material that is more flexible than the relatively stiff or rigid material forming the distal section 70b of the proximal section 77. In other words, the intermediate portion 70c of the proximal section 77 is more flexible than the distal portion 70b of the proximal section 77. The purpose of this material is to help prevent the intermediate portion of the proximal section from negatively impacting the ability of the ureteroscope to deflect.

[0063] The proximal portion 70d of the proximal section 77 is made of a relatively stiff or rigid material that is specifically selected to ensure appropriate torque transmission. That is, the material forming the proximal portion 70d is preferably selected so that torque applied to the proximal portion of the proximal section (e.g., by way of the operating member 26) is appropriately transmitted toward the distal section of the shaft cover 70. The stiffness of the proximal portion 70d is preferably greater than the stiffness of the distal portion 70b.

[0064] To provide an example of the relative lengths of the portions 70b, 70c, 70d forming the proximal section 77 of the cover shaft, the distal portion 70b of the proximal section 77 is preferably 6 mm-15 mm in length, more preferably 8 mm in length, the intermediate portion 70c is preferably 60

mm-150 mm in length, more preferably 80 mm in length and the proximal portion **70d** of the proximal section **77** is preferably 800 mm-1200 mm in length, more preferably 1000 mm in length. Thus, the distal portion **70b** of the proximal section **77** is shorter than the intermediate portion **70c** and the proximal portion **70d** of the proximal section **77**, and the intermediate portion **70c** is shorter than the proximal portion **70d** of the proximal section **77**. In addition, the intermediate section can possess a length of preferably 1 mm-3 mm, more preferably approximately 2 mm while the distal section **75** possesses a length of preferably 3 mm-8 mm, more preferably about 5 mm.

**[0065]** As described above, the intermediately located bent section **79** is bounded on opposite ends by bends **79'**, **79'**. As will be described in more detail below, the bends **79'**, **79'** are preferably configured so that during use, the suction head **50** of the retrieval device **30** is angled at an angle of at least  $25^\circ$  relative to the central axis of the distal end portion of the ureteroscope **40**. To achieve this result, the angles  $70\alpha$ ,  $70\alpha'$  illustrated in FIG. **8** are preferably  $120^\circ$  while the angles  $70\beta$ ,  $70\beta'$  are  $30^\circ$ .

**[0066]** Connecting the suction head to a shaft cover **70** possessing the configuration shown in FIG. **8** imparts the following operational characteristics to the retrieving device. FIG. **10A** illustrates the shaft cover **70** connected to the suction head **50**, while the proximal portion **70d** of the proximal section **77**, the intermediate portion **70c** of the proximal section **77** and a part of the distal portion **70b** of the proximal section **77** are located in the instrument channel of the ureteroscope **40**. The distal section **75** of the shaft cover **70**, the intermediately located bent section **79** of the shaft cover **70** and a part of the distal portion **70b** of the proximal section **77** of the shaft cover **70** are positioned outside the ureteroscope **40** as shown in FIG. **10A**. In this position, the central axis **50a** of the suction head **50** is parallel to, and offset from, the central axis **40a** of the distal end portion of the ureteroscope **40**. The coaxial arrangement of the suction head **50** relative to the ureteroscope **40** is used when advancing the retrieving device through the living body in regions that are not highly curved.

**[0067]** Starting at the position shown in FIG. **10A**, axially moving (pulling) the shaft cover **70** in the proximal direction (i.e., moving the shaft cover **70** in the rearward direction indicated by the rightward arrow in FIG. **10A**) causes the remaining part of the distal portion **70b** of the proximal section **77** of the cover shaft to enter the instrument channel **42** in the ureteroscope **40**, and also causes a part of the bent section **79** of the shaft cover **70** to enter the instrument channel **42** in the ureteroscope **40**. The retrieval device **30** thus takes on the arrangement or configuration shown in FIG. **10B**.

**[0068]** As shown in FIG. **10B**, axially moving a portion of the bent section **79** of the shaft cover **70** into the instrument channel in the ureteroscope **40** causes the suction head **50** to be angled relative to the ureteroscope **40**. In particular, the central axis **50a** of the suction head **50** is oriented at an angle (i.e., an angle other than  $0^\circ$  and  $180^\circ$ ) relative to the central axis **40a** of the distal end portion of the ureteroscope **40**. The angle between the central axis **50a** of the suction head **50** and the central axis **40a** of the ureteroscope **40** is preferably at least  $25^\circ$ , more preferably at least  $30^\circ$ . Angling the suction head **50** relative to the ureteroscope **40** in this manner allows the suction head **50** to access highly curved regions in a

living body that might otherwise be very difficult to access with the suction head orientation shown in FIG. **10A**.

**[0069]** As an example, reference is made to the FIG. **5** schematic illustration of a kidney possessing a lower calix (lower renal calix) **102**, a middle or intermediate calix (middle or intermediate renal calix) **104**, an upper calix (upper renal calix) **106**, and a renal pelvis **101** spaced from the calices **102**, **104**, **106**. To reach calculus in the lower calix **102** requires access by way of the ureter **108** along a path generally indicated by the dotted line FIG. **5**. As can be readily appreciated, this path is highly curved and can be difficult to navigate.

**[0070]** Configuring the retrieval device **30** to include the shaft cover **70** illustrated in FIG. **8**, it is possible to angle the suction head **50** of the retrieval device **30** relative to the ureteroscope **40** in the manner illustrated in FIG. **10B** by axially moving the shaft cover in the rearward direction, thus making it easier to traverse or navigate the path indicated by the dotted line in FIG. **5**. It is thus possible to retrieve calculus in the lower calix **102** and move the retrieved calculus/calculi to the middle or intermediate calix **104** or possibly the upper calix **106**. Lithotripsy can then be more easily carried out with respect to the retrieved and moved calculus.

**[0071]** FIG. **10C** illustrates the retrieval device **30** in a position that is the same as shown in FIG. **10B**, except that the shaft cover **70** is rotated so that the suction head **50** is angled at an orientation  $180^\circ$  relative to the orientation shown in FIG. **10B**. In the position shown in FIG. **10C**, the suction head **50** is angled relative to the ureteroscope **40** so that the angle between the central axis **50a** of the suction head **50** and the central axis **40a** of the ureteroscope **40** is preferably at least  $25^\circ$ , more preferably at least  $30^\circ$ . There are benefits associated with being able to rotate the shaft cover **70** and the suction head **50** from the FIG. **10B** position to the FIG. **10C** position. An ureteroscope is typically equipped with the ability to deflect, but the manner of bending is typically somewhat limited. That is, the movement of the tip portion of the ureteroscope is limited to one plane (uniplanar movement or X-plane movement). It is thus difficult for an operator to freely control the direction or orientation of the suction head relying only on the ureteroscope deflection ability. On the other hand, when the operator rotates the angled suction head from FIG. **10B** to FIG. **10C**, the different plane of movement of the suction head (y-plane movement) is added to the plane of movement ability of the ureteroscope. Further, if the operator pushes/pulls the shaft cover **70**, a still further movement direction is added (z-plane). That is why the operator can control the direction of the suction head freely by rotation (between FIG. **10B** and FIG. **10C**) of the angled-suction head. From another point of view, the installation location of an objective lens of the ureteroscope is off-center. So if the operator rotates the angled suction head from the FIG. **10B** position to the FIG. **10C** position, operator can change the view of the suction head **50**.

**[0072]** FIG. **10D** illustrates the retrieving device in which the shaft cover **70** and the suction head **50** are axially moved in the forward direction (i.e., to the right, as indicated by the arrow, in FIG. **10D**). This causes the suction head **50** to move axially forward, and shift to a position in which the central axis **50a** of the suction head **50** is parallel to and offset (not coaxial) from the central axis **40a** of the distal end

portion of the ureteroscope **40**. This permits a field of view **100** for the operator using the optical system in the ureteroscope **40**.

[0073] FIG. 10E illustrates another operational aspect of the retrieving device **30**. With the retrieving device **30** in the position shown in FIG. 10B (or FIG. 10C), the operator can axially pull-back the shaft cover **70** (i.e., move the shaft cover **70**, together with the suction head **50** and the shaft **72**) so that the shaft cover **70** is moved into the elongated body **40** (ureteroscope), to straighten the bent section **79**. The total length of the tip portion of the device (the suction head+the exposed or uncovered portion of the shaft cover **70**+the unbendable distal end portion of the ureteroscope) is shorter compared to the total length of the tip portion in FIG. 10B. The operational position of the retrieving device shown in FIG. 10E is advantageous when moving or maneuvering the retrieving device into a narrow lumen (e.g., an ureter and an ureteral access sheath).

[0074] FIGS. 11A-11C illustrates an embodiment representing another example of the inventive retrieving device disclosed here. The embodiment shown in FIGS. 11A-11C represents an alternative way of angling the suction head relative to the distal end portion of the ureteroscope. This embodiment of the retrieving device depicted in FIGS. 11A-11C is similar to the embodiment described above and illustrated in FIGS. 10A-10D, except that the angling of the suction head is facilitated by a shaped contact part rather than a shaped tube.

[0075] Referring to FIG. 11A, a contact part **180** is provided between the suction head **150** and the ureteroscope **40**. In this embodiment, the contact part **180** is integrally formed in one piece at the same time with the suction head **150**. The contact part **180** projects rearwardly (in the proximal direction) away from the suction head **150** as illustrated in FIG. 11A. The contact part **180** in this embodiment is a curved projecting portion. The contact part **180** includes a curved surface **181**, namely a convex surface. The retrieval device **130** further includes a shaft cover **70'** is a linearly extending (straight) shaft cover **70'**. FIG. 11A shows that the shaft cover **70'** passes through a hole in the contact part **180** so that the contact part **180** at least partially surrounds the shaft cover **70'**.

[0076] The shaft cover **70'** passes through a hole in the contact part **180** at an angle in FIG. 11A so that the central axis of the suction head **150** and the central axis of the distal end portion of the shaft cover **70'** are parallel to one another, but offset from one another so that the suction head **150** and the distal end portion of the shaft cover **70'** are not coaxial with one another. This offset contributes to angling the suction head by the shaped contact part in FIGS. 11-16. The suction head **150** and the distal end portion of the ureteroscope **40** shown in FIG. 11A are oriented in the manner shown in FIG. 11A while advancing the retrieval device **130** within the narrow lumen (e.g., an ureter or an ureteral access sheath). To manipulate or move the retrieval device through a relatively narrow lumen or to retrieve calculus in a narrow lumen, the operator tends to choose or may prefer the device being in the state shown in FIG. 11A. To manipulate or move the retrieval device through a curved area (e.g., to reach a lower calyx (lower renal calyx)), the operator tends to choose or may prefer the device being in the state depicted in FIG. 11B. To retrieve calculus in a large area (e.g., an open space

in kidney), the operator can use the device positioned in either the state shown in FIG. 11A or the state shown in FIG. 11B.

[0077] To angle the suction head **150** relative to the distal end portion of the ureteroscope **140**, at first the shaft cover **70'** is axially moved or pulled rearwardly (i.e., to the right, in the direction of the arrow, in FIG. 11A) until the contact part **180** comes into direct contact with the curved (concave) distal end surface **41** of the ureteroscope **40**. In this state (the curved surface of the contact part **180** just contacts the distal end surface **41** of the ureteroscope **40**), the suction head **150** is not angled. As the shaft cover **70'** continues to be axially moved in the rearward direction, this contact between the two curved surfaces **181**, **41** helps cause the suction head **150** to become angled relative to the distal end portion of the ureteroscope **40** as illustrated in FIG. 11B. It is thus possible to angle the suction head **50** relative to the ureteroscope **40** by axially moving the shaft cover (and the suction head **50**).

[0078] From the position illustrated in FIG. 11A, it is possible to rotate the suction head **150** by rotating the shaft cover **70'**. The suction head **150** is moved to the position shown in FIG. 11C which is displaced 180° from the position shown in FIG. 11A. In the position of the suction head **150** shown in FIG. 11A, the suction head **150** and the distal end portion of the ureteroscope **40** are parallel and coaxial with one another. By rotating the suction head **150** to the FIG. 11C 11A position, the operator can pass the retrieval device **130** into a relatively narrow lumen (e.g. a ureter and a ureteral access sheath). In the position of the suction head **150** shown in FIG. 11C, the suction head **150** does not obstruct the field of view **110** seen through the objective lens of the ureteroscope **40**. By rotating the suction head **150** in this way, the medical professional can observe in front of the retrieval device **130** to help facilitate the procedure.

[0079] FIGS. 12A and 12B illustrate another embodiment. This embodiment of the retrieval device **230** is similar to the embodiment illustrated in FIGS. 11A-11C, except that the configuration of the contact part is different. The embodiment of the retrieval device **230** shown in FIGS. 12A-12B includes a contact part **280** that includes two sections **282**, **284** connected to one another by a hinge **283**. The two sections **282**, **284** can be plate-shaped elements. One of the sections **282** is fixed to or integral with the suction head **250**, and the other section **284** possesses a through hole through which the shaft cover **70'** passes. The section **284** thus partially surrounds the shaft cover **70'**. The shaft cover **70'** is a linearly extending (straight) shaft cover **70'**.

[0080] In operation, the shaft cover **70'** is moved axially in the rearward direction (i.e., to the right, in the direction of the arrow, in FIG. 12A) and the contact part **280** approaches the curved (concavely curved) distal end surface **41** of the ureteroscope **40** and ultimately contacts the concavely curved distal end surface **41** of the ureteroscope **40**. After the section **282** of the contact part contacts the concavely shaped distal end surface of the ureteroscope **40**, continued axial movement of the shaft cover **70'** in the proximal or rearward direction causes the suction head **250** to become angled relative to the distal end portion of the ureteroscope as shown in FIG. 12B. In this way, the central axis of the suction head **250** forms an angle (i.e., an angle other than 0° and 180°) relative to the central axis of the distal end portion of the ureteroscope **40**. The suction head **250** is preferably angled at an angle of at least 25° relative to the central axis

of the distal end portion of the ureteroscope 40, more preferably at least 30°. The section 284 can help stabilize the contact between the contact part 282 and the distal end surface of the ureteroscope 40.

[0081] FIGS. 13A and 13B illustrate an embodiment representing another example of the retrieving device disclosed here in which the retrieving device is configured to angle the suction head relative to the ureteroscope. This embodiment of the retrieving device differs from the version shown in FIGS. 12A and 12B in that the contact part 380 is a rigid one-piece member. The contact part 380 is integrally formed in one piece with the suction head 350, but can also be separate from the suction head 350 and fixed in place to the suction head 350. The contact part 380 includes an arm 386 projecting away from the suction head 350, and a hemispherical portion 388 configured to contact the concave curved distal end surface 41 of the ureteroscope 40. The hemispherical shaped portion 388 presents a convex surface that directly contacts the concave curved distal end surface 41 of the ureteroscope 40. The hemispherical shaped portion 388 of the contact part 380 includes a through hole or opening through which passes the shaft cover 70' so that a portion of the contact part 380 encircles or surrounds the shaft cover 70'. The shaft cover 70' is a linearly extending (straight) shaft cover 70'.

[0082] In use, the shaft cover 70' is axially moved in the rearward direction (i.e., to the right, in the direction of the arrow, in FIG. 13A). This causes the suction head 350 and the contact portion 380 to also move in the rearward direction until the hemispherical shaped portion 388 directly contacts the distal end surface of the ureteroscope 40. Continued rearward axial movement of the shaft cover 70' causes the suction head 350 to pivot in the manner indicated by the arrow in FIG. 13B so that the suction head 350 is angled relative to the ureteroscope 40. That is, the central axis of the suction head 350 is angled at an angle of at least 25°, preferably at least 30°, relative to the central axis of the distal end portion of the ureteroscope 40.

[0083] FIGS. 14A and 14B illustrate an embodiment representing a further example of the retrieving device disclosed here in which the retrieving device is configured to angle the suction head relative to the ureteroscope. This embodiment of the retrieving device 430 utilizes a contact part 480 that is separate from both the suction head 450 and the ureteroscope 40, but is subsequently mounted on or connected to the distal end portion of the ureteroscope 40. The contact part 480 is a generally U-shaped member defined by two spaced-apart legs 492, 494 connected by an intermediately located base 496. The leg 492 closest to the suction head includes a curved surface 497 facing towards the suction head. A hollow cylindrical element 498 is integrally formed with one of the legs 494 and projects away from the leg 494. The cylindrical element 498 is positioned in the instrument channel 42 at the distal end portion of the ureteroscope 40 so that the contact part 480 is integrated with and held in the ureteroscope 40.

[0084] Each of the legs 492, 494 of the contact part 480 is provided with a through hole 493, 495 through which passes the shaft cover 70'. The shaft cover 70' is a linearly extending (straight) shaft cover 70'. By virtue of the through holes 493, 495 in the legs 492, 494 of the contact part 480, a portion of the contact part 480 surrounds the shaft cover 70' at two spaced apart locations. The shaft cover 70' forming a part of the retrieval device 430 shown in FIGS. 14A and 14B is a

linearly extending (straight) tube. The shaft cover 70' passes through holes 493 and/or 495 in the contact part 180 at an angle as shown in FIG. 14A so that the central axis of the suction head 450 and the central axis of the distal end portion of the shaft cover 70' are parallel to one another, but offset from one another so that the suction head 450 and the distal end portion of the shaft cover 70' are not coaxial.

[0085] In use, the contact part 480 is fitted to the ureteroscope 40 by positioning the cylindrical element 498 in the instrument channel 42 at the distal end portion of the ureteroscope 40. The shaft cover 70' is then axially moved in the proximal direction (i.e., to the right, in the direction of the arrow, in FIG. 14A). This causes the suction head 450 to approach the ureteroscope 40 and eventually move into direct contact with the curved surface 497 on the leg 492 of the contact part 480. As the shaft cover 70' continues to be axially moved (pulled) in the proximal direction, the suction head 450 becomes angled by virtue of the curved surface 497 of the leg 492 of the contact part 480 contacting the suction head 450 so that the suction head 450 becomes angled with respect to the ureteroscope.

[0086] FIGS. 15A and 15B illustrate an embodiment of the retrieving device representing another example of the inventive retrieving device disclosed here. This embodiment of the retrieving device 530 includes a contact part 580 that is separate from both the suction head 550 and the ureteroscope 40. The contact part 580 is a generally V-shaped one-piece contact part that includes two legs 582, 584 connected to one another at a vertex. The two legs 582, 584 diverge away from one another in a direction away from the vertex. Each of the legs 582, 584 includes a respective through hole 593, 595 through which extends the shaft cover 70'. A portion of the contact part 580 thus encircles or surrounds the shaft cover 70' at two spaced apart locations. The shaft cover 70' is a linearly extending (straight) shaft cover 70'.

[0087] In use, the shaft cover 70' is axially moved in the proximal direction (i.e., to the right, in the direction of the arrow, in FIG. 15A). This causes the suction head 550 to also move in the proximal direction. Eventually, the suction head 550 contacts the leg 582 of the contact part 580, and the leg 584 of the contact part 580 contacts the distal end of the ureteroscope 40. As the shaft cover 70' continues to be axially moved (pulled) in the proximal direction, the suction head 550 becomes angled by V-shaped contact part 580 contacting both the suction head 550 and the distal end of the ureteroscope 40 so that the suction head 550 becomes angled with respect to the ureteroscope 40 in the manner illustrated in FIG. 15B. That is, the suction head 550 moves in the direction of the arrow in FIG. 15B so that the central axis of the suction head 550 is disposed at an angle (other than 0° and 180°) relative to the central axis of the distal end portion of the ureteroscope 40. That is, the central axis of the suction head 550 is angled at an angle of at least 25°, preferably at least 30°, relative to the central axis of the distal end portion of the ureteroscope 40.

[0088] It is possible to control the angle of inclination of the suction head 550 relative to the ureteroscope 40 in the embodiment shown in FIGS. 15A and 15B by appropriately selecting the material forming the contact part 580. For example, the contact part 580 can be made of a relatively rigid material, like metal, so that the two legs 582, 584 are relatively stiff and maintain the relative position/orientation when the leg 582 is contacted by the suction head 550 and

the leg **584** contacts the distal end of the ureteroscope **40**. On the other hand, the contact part **580** can be made of a more flexible material such that in the arrangement shown in FIG. **15B**, continued axial movement of the shaft cover **70'** in the proximal or rearward direction varies the angle between the suction head **550** and the ureteroscope **40**.

[**0089**] FIGS. **16A-16C** illustrate an embodiment representing another example of the retrieving device disclosed here. This embodiment of the retrieving device **630** provides another mechanism for angling the suction head **650** relative to the ureteroscope **40**. This embodiment includes a contact part comprised of two separate contact sections **681**, **683**. The first contact section **681** is connected to or fixed to the suction head **650** so that the first contact section **681** and the suction head **650** move together as a unit, while the second contact section **683** includes a cylindrical-shaped projection **683'** that fits into the instrument channel at the distal end portion of the ureteroscope **40** so that the second contact section **683** and the suction head **650** move together as a unit. The second contact section **683** is thus integrated with or connected to the ureteroscope **40**. The first and second contact sections **681**, **683** each include a respective inclined face or surface **681"**, **683"**. Each of these first and second contact sections **681**, **683** also includes a through hole or opening through which extends the shaft cover **70'**. In this embodiment, the shaft cover **70'** is a linearly extending (straight) shaft cover **70'**. Each of the contact sections **681**, **683** thus encircles a portion of the shaft cover **70'**.

[**0090**] Two projections **681a**, **681a** project from the inclined surface **681"** of the first contact section **681** toward the second contact section **683**. Two recesses **683a**, **683a** are provided in the inclined surface **683"** of the second contact section **683**. Each of the recesses **683a**, **683a** is configured to receive one of the projections **681a**, **681a** projecting from the first contact part **681**.

[**0091**] In use, the shaft cover **70'** is axially moved in the proximal direction (i.e., in the rearward direction, indicated by the arrow, in FIG. **16B**) so that the suction head **650** approaches the ureteroscope **40**. Eventually, each of the projections **681a**, **681a** projecting from the first contact section **681** enters the respective recess **683a**, **683a** in the second contact section **683** as shown in FIG. **16B**. The suction head **650** and the ureteroscope **40** are thus locked together (rotationally locked together). In the arrangement shown in FIG. **16B**, the retrieval device **630** is moved through the relatively narrow lumen of the living body toward the desired location.

[**0092**] To angle the suction head **650** relative to the distal end portion of the ureteroscope **40**, the first and second contact sections **681**, **683** are separated from one another so that the projections **681a**, **681a** are separated (spaced) from the respective recess **683a**. The first contact section **681** is rotated 180° relative to the second contact section **683** as illustrated by the arrow in FIG. **16C**. This can be accomplished by rotating the shaft cover **70'** and the suction head **650** relative to the ureteroscope **40**. After rotating the first contact section **681**, the projections **681a**, **681a** projecting from the first contact section **681** are fitted into respective recesses in the second contact section **683** as illustrated in FIG. **16C**. In the angled orientation shown in FIG. **16C**, the recesses in the second contact part **683** that receive the projections **681a**, **681a** differ from (i.e., are angled differently than) the recesses **683a**, **683a** shown in FIG. **16A**.

[**0093**] This embodiment of the retrieving device **630** provides a fixed angular orientation between the central axis of the suction head **650** and the central axis of the distal end portion of the ureteroscope **40**. This angular orientation is defined by the angle of the inclined faces **681"**, **683"** of the first and second contact sections **681**, **683**. It is possible to adjust the angular orientation by changing the angle of inclination of the inclined surfaces **681"**, **683"**.

[**0094**] Each of the embodiments of the retrieving device disclosed above for angularly orientating the suction head relative to the distal end portion of the ureteroscope **40** makes it possible to angularly position the suction head by axially moving the shaft cover and the suction head relative to the ureteroscope. It is thus possible to achieve a desired angular orientation of the suction head without excessive effort and without a complicated construction.

[**0095**] The detailed description above describes a device and method for retrieving/removing calculus from parts of a living body such as the ureter and the renal pelvis. The invention is not limited, however, to the precise embodiments and variations described. Various changes, modifications and equivalents can be effected by one skilled in the art without departing from the spirit and scope of the invention as defined in the accompanying claims. It is expressly intended that all such changes, modifications and equivalents which fall within the scope of the claims are embraced by the claims.

What is claimed is:

1. A device for retrieving calculus in a lumen of a living body comprising:

a shaft;

an elongated member sized to be positioned in the lumen of the living body, the elongated member including a suction head housing possessing a distal end, a proximal end and an interior, the distal end of the suction head housing being open to permit entry of calculus and the proximal end of the suction head housing being closed by a wall through which passes the shaft;

a rotatable impeller positioned inside the elongated member;

the shaft being connected to the rotatable impeller so that the shaft and the rotatable impeller rotate together as a unit, the shaft being connectable to a drive source that is operable to rotate the shaft and the rotatable impeller, with rotation of the rotatable impeller creating suction that draws calculus through the open distal end of the suction head housing and into the interior of the suction head housing;

a shaft cover possessing a distal end portion that terminates in a distal end connected to the proximal end of the suction head housing so that the elongated member and the shaft cover axially move and rotate together, the distal end portion of the shaft cover possessing a central axis, the shaft cover also possessing a proximal end portion that possesses a central axis, the shaft cover covering the shaft; and

the central axis of the distal end portion of the shaft cover and the central axis of the proximal end portion of the shaft cover being non-coaxial.

2. The device according to claim 1, wherein the shaft cover includes an intermediate portion between the distal end portion of the shaft cover and the proximal end portion of the shaft cover, the intermediate portion being a bent portion that is bent when no force is applied to the bent

portion, the shaft cover being movably positionable in a lumen of an elongated body to move between: i) one position in which the distal end portion of the shaft cover is positioned at an inlet to the lumen and the bent portion is located in the lumen so that an angle is formed between the central axis of the elongated member and a central axis of a distal section of the elongated body; and ii) an other position in which the bent portion is positioned at the inlet to the lumen while the distal end portion is positioned outside the elongated body so that the angle between the central axis of the elongated member and the central axis of the distal section of the elongated body in the second position is less than the angle between the central axis of the elongated member and the central axis of the distal section of the elongated body in the first position of the shaft cover.

3. The device according to claim 2, wherein the elongated body is an ureteroscope.

4. The device according to claim 1, wherein the proximal end portion of the shaft cover is a linearly extending proximal end portion and the distal end portion of the shaft cover is a linearly extending distal end portion.

5. The device according to claim 4, wherein the linearly extending proximal end portion and the linearly extending distal end portion each possess an axial extent, the axial extent of the linearly extending proximal end portion being greater than the axial extent of the linearly extending distal end portion.

6. The device according to claim 1, wherein a proximal end portion of the suction head housing is a contact part configured to cause the suction head housing to angularly move relative to the distal end portion of the elongated body when the shaft cover together with the suction head housing is axially moved in a proximal direction relative to an elongated body so that the central axis of the suction head housing is angled relative to the central axis of the distal end portion of the elongated body at an angle other than 0° and 180°.

7. The device according to claim 1, wherein the proximal end portion of the shaft cover is a linearly extending proximal end portion and the distal end portion of the shaft cover is a linearly extending distal end portion, the linearly extending proximal end portion and the linearly extending distal end portion being parallel to one another.

8. A device for retrieving calculus in a lumen of a living body comprising:

an elongated member sized to be positioned in the lumen of the living body, the elongated member including a suction head housing disposed on a distal side of the elongated member;

a rotatable member positioned inside the elongated member;

a shaft connected to the rotatable member so that the shaft and the rotatable member move together as a unit, the shaft being connectable to a drive source to rotate the shaft and the rotatable member, with rotation of the rotatable member creating suction that draws calculus toward the elongated member;

a shaft cover possessing a distal end portion having a central axis and a proximal end portion having a central axis, the shaft cover covering the shaft and being connected to the elongated member so that the elongated member and the shaft cover axially move and rotate together; and

the central axis of the distal end portion of the shaft cover is offset from the central axis of the proximal end portion of the shaft cover.

9. The device according to claim 8, wherein the shaft cover includes a bent section that is bent when no force is applied to the bent section, the bent section being positioned proximally of a distal section of the shaft cover, and the shaft cover being movably positionable in a lumen of an elongated body to move between: i) one position in which the distal section of the shaft cover is positioned at an inlet to the lumen and the bent section is located in the lumen so that an angle is formed between the central axis of the elongated member and a central axis of a distal section of the elongated body; and ii) an other position in which the bent section is positioned at the inlet to the lumen while the distal section is positioned outside the elongated body so that the angle between the central axis of the elongated member and the central axis of the distal section of the elongated body in the second position is less than the angle between the central axis of the elongated member and the central axis of the distal section of the elongated body in the first position of the shaft cover

10. The device according to claim 9, wherein the shaft cover includes a linearly extending proximal section positioned proximal of the bent section, the distal section being a linearly extending distal section, the proximal section possessing a central axis and the distal section possessing a central axis, the central axis of the distal section and the central axis of the proximal section being non-coaxially arranged.

11. The device according to claim 9, wherein the shaft cover includes a linearly extending proximal section positioned proximal of the bent section, the distal section being a linearly extending distal section, the linearly extending proximal section and the linearly extending distal sections each possessing an axial extent, the axial extent of the linearly extending proximal section being greater than the axial extent of the linearly extending distal section.

12. The device according to claim 9, wherein the elongated body is an ureteroscope.

13. The device according to claim 9, wherein a contact part is disposed on a proximal side of the suction head housing, the contact part being configured to cause the suction head housing to angularly move relative to the distal end portion of the elongated body when the shaft cover together with the suction head housing is axially moved in a proximal direction relative to an elongated body so that the central axis of the suction head housing is angled relative to the central axis of the distal end portion of the elongated body at an angle other than 0° and 180°.

14. The device according to claim 13, wherein the contact part is integrally formed in one piece at the same time with the suction head housing.

15. The device according to claim 13, wherein the contact part possesses a curved portion that contacts the distal end of the elongated body when the shaft cover together with the suction head is axially moved in the proximal direction relative to the elongated body to cause the suction head housing to be angled relative to the distal end portion of the elongated body.

16. The device according to claim 13, wherein the contact part surrounds at least a part of the shaft cover.

17. The device according to claim 13, wherein the contact part is separate from the suction head housing and is separate

from the elongated body, the contact part including a projection fitted into the lumen in the elongated body.

**18.** The device according to claim **13**, wherein suction head housing possesses a proximal end facing towards the elongated body, wherein the contact part is separate from the suction head housing and is separate from the elongated body, the contact part possessing a curved end portion that contacts the proximal end of the suction head housing when the shaft cover is moved proximally relative to the elongated body.

**19.** The device according to claim **13**, wherein the elongated body is a ureteroscope.

\* \* \* \* \*

专利名称(译)	演算/结石检索装置及方法		
公开(公告)号	<a href="#">US20200060699A1</a>	公开(公告)日	2020-02-27
申请号	US16/668320	申请日	2019-10-30
[标]申请(专利权)人(译)	泰尔茂株式会社		
申请(专利权)人(译)	泰尔茂株式会社		
当前申请(专利权)人(译)	泰尔茂株式会社		
[标]发明人	HONDA KEI JINNO MAKOTO		
发明人	HONDA, KEI JINNO, MAKOTO		
IPC分类号	A61B17/22		
CPC分类号	A61B2017/0034 A61B2217/005 A61B2017/00738 A61B2017/00553 A61B2017/22079 A61B17/22 A61B2017/22035 A61B2017/00296 A61B2017/00331		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

摘要(译)

检索活体中的微积分并将微积分重新定位到活体中不同位置的方法包括：将细长构件放置在微积分所在的活体中，将活体中的微积分朝细长构件拉动，同时细长构件定位在活体内，使得牙结石被细长构件保持。移动细长构件，以使细长构件位于生物体内的位置，该位置不同于在将牙石向细长构件拉动时在生物体内的细长构件的位置。从长形构件释放牙结石，使得在朝着长形构件拉动牙结石时，牙结石在生物体内的位置不同于活体中牙结石的位置。

