



US007143924B2

(12) **United States Patent**
Scirica et al.

(10) **Patent No.:** **US 7,143,924 B2**
(45) **Date of Patent:** ***Dec. 5, 2006**

- (54) **SURGICAL STAPLING APPARATUS WITH LOCKING MECHANISM**
- (75) Inventors: **Paul A. Scirica**, Huntington, CT (US);
Stanislaw Marczyk, Stratford, CT (US)
- (73) Assignee: **Tyco Healthcare Group LP**, North Haven, CT (US)
- (*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.
- This patent is subject to a terminal disclaimer.

(21) Appl. No.: **11/059,805**

(22) Filed: **Feb. 17, 2005**

(65) **Prior Publication Data**
US 2005/0184124 A1 Aug. 25, 2005

- Related U.S. Application Data**
- (60) Provisional application No. 60/545,619, filed on Feb. 17, 2004.
- (51) **Int. Cl.**
A61B 17/068 (2006.01)
- (52) **U.S. Cl.** **227/175.2; 227/175.1; 227/175.4; 227/182.1**
- (58) **Field of Classification Search** **227/175.2, 227/175.4, 176.1, 182.1, 175.1**
See application file for complete search history.

- (56) **References Cited**
U.S. PATENT DOCUMENTS
- | | | |
|-------------|--------|------------------|
| 3,079,606 A | 3/1963 | Bobrov et al. |
| 3,490,675 A | 1/1970 | Green et al. |
| 3,499,591 A | 3/1970 | Green |
| 4,244,372 A | 1/1981 | Kapitanov et al. |
| 4,429,695 A | 2/1984 | Green |
| 4,520,817 A | 6/1985 | Green |

4,589,413 A	5/1986	Malyshev et al.
4,605,001 A	8/1986	Rothfuss et al.
4,608,981 A	9/1986	Rothfuss et al.
4,610,383 A	9/1986	Rothfuss et al.
4,633,861 A	1/1987	Chow et al.
4,633,874 A	1/1987	Chow et al.
4,672,964 A	6/1987	Dee et al.
4,763,669 A	8/1988	Jaeger
4,863,088 A	9/1989	Redmond et al.
4,880,015 A	11/1989	Nierman
4,892,244 A	1/1990	Fox et al.
4,978,049 A	12/1990	Green
4,991,764 A	2/1991	Mericle
5,040,715 A	8/1991	Green et al.
5,065,929 A	11/1991	Schulze et al.
5,071,052 A	12/1991	Rodak et al.
5,074,454 A	12/1991	Peters
5,083,695 A	1/1992	Foslien et al.
5,111,987 A	5/1992	Moeinzadeh et al.

(Continued)

FOREIGN PATENT DOCUMENTS

DE 4300307 7/1994


(Continued)

Primary Examiner—John Slpos
Assistant Examiner—Michelle Lopez

(57) **ABSTRACT**

The present disclosure provides for a loading unit for use with a surgical stapling apparatus. The loading unit includes a housing portion having a distal end and a proximal end, a drive assembly slidably supported within the housing portion of the loading unit, and a locking member supported on the housing portion of the loading unit. The locking member is movable from a first position wherein the locking member engages the drive assembly and maintains the drive assembly in a ready-to-load position to a second position wherein the locking member permits movement of the drive assembly relative to the housing portion.

20 Claims, 19 Drawing Sheets

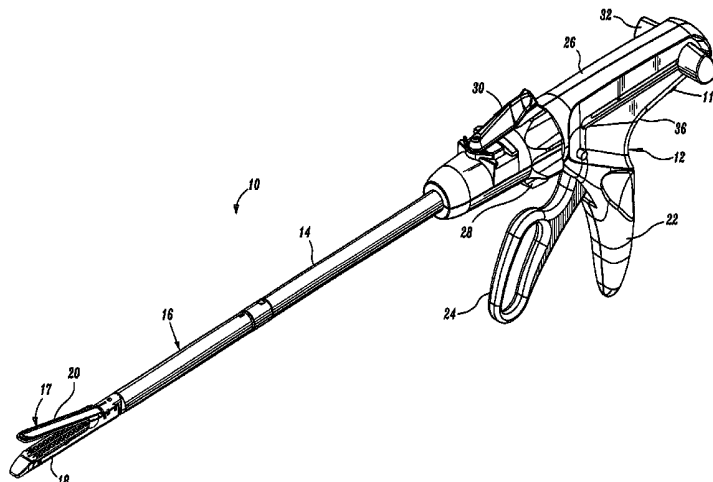

U.S. PATENT DOCUMENTS

5,129,570 A	7/1992	Schulze et al.	5,487,500 A	1/1996	Knodel et al.
5,141,144 A	8/1992	Foslien et al.	5,507,426 A	4/1996	Young et al.
5,152,279 A	10/1992	Wilk	5,535,935 A	7/1996	Vidal et al.
5,209,747 A	5/1993	Knoepfler	5,582,617 A	12/1996	Klieman et al.
RE34,519 E	1/1994	Fox et al.	5,584,425 A *	12/1996	Savage et al. 227/175.2
5,275,608 A	1/1994	Forman et al.	5,605,272 A	2/1997	Witt et al.
5,282,826 A	2/1994	Quadri	5,630,539 A	5/1997	Pyley et al.
5,307,976 A	5/1994	Olson et al.	5,634,584 A	6/1997	Okorochoa et al.
5,312,023 A	5/1994	Green et al.	5,762,255 A	6/1998	Chrisman et al.
5,318,221 A	6/1994	Green et al.	5,797,537 A	8/1998	Oberlin et al.
5,326,013 A	7/1994	Green et al.	5,820,009 A	10/1998	Melling et al.
5,330,502 A	7/1994	Hassler et al.	5,901,895 A	5/1999	Heaton et al.
5,332,142 A	7/1994	Robinson et al.	6,010,054 A	1/2000	Johnson et al.
5,350,391 A	9/1994	Iacovelli	6,032,849 A	3/2000	Mastri et al.
5,354,311 A	10/1994	Kambin et al.	6,109,500 A *	8/2000	Alli et al. 227/175.2
5,374,277 A	12/1994	Hassler	6,241,139 B1	6/2001	Milliman et al.
5,376,095 A	12/1994	Ortiz	6,669,073 B1 *	12/2003	Milliman et al. 227/175.2
5,383,888 A	1/1995	Zvenyatsky et al.	2005/0184123 A1 *	8/2005	Scirica 227/176.1
5,397,046 A	3/1995	Savage et al.	2005/0184125 A1 *	8/2005	Marczyk 227/176.1
5,415,334 A	5/1995	Williamson, IV et al.	FOREIGN PATENT DOCUMENTS		
5,415,335 A	5/1995	Knodel, Jr.	EP	0484677	5/1992
5,433,721 A	7/1995	Hooven et al.	EP	0589306	3/1994
5,465,895 A	11/1995	Knodel et al.	EP	0591948	4/1994
5,467,911 A	11/1995	Tsuruta et al.	EP	0592243	4/1994
5,474,566 A	12/1995	Alesi et al.	EP	0621009	10/1994
5,474,571 A	12/1995	Lang	EP	0656188	6/1995
5,484,451 A	1/1996	Akopov et al.	FR	2681775	10/1991
5,486,185 A	1/1996	Freitas et al.	* cited by examiner		

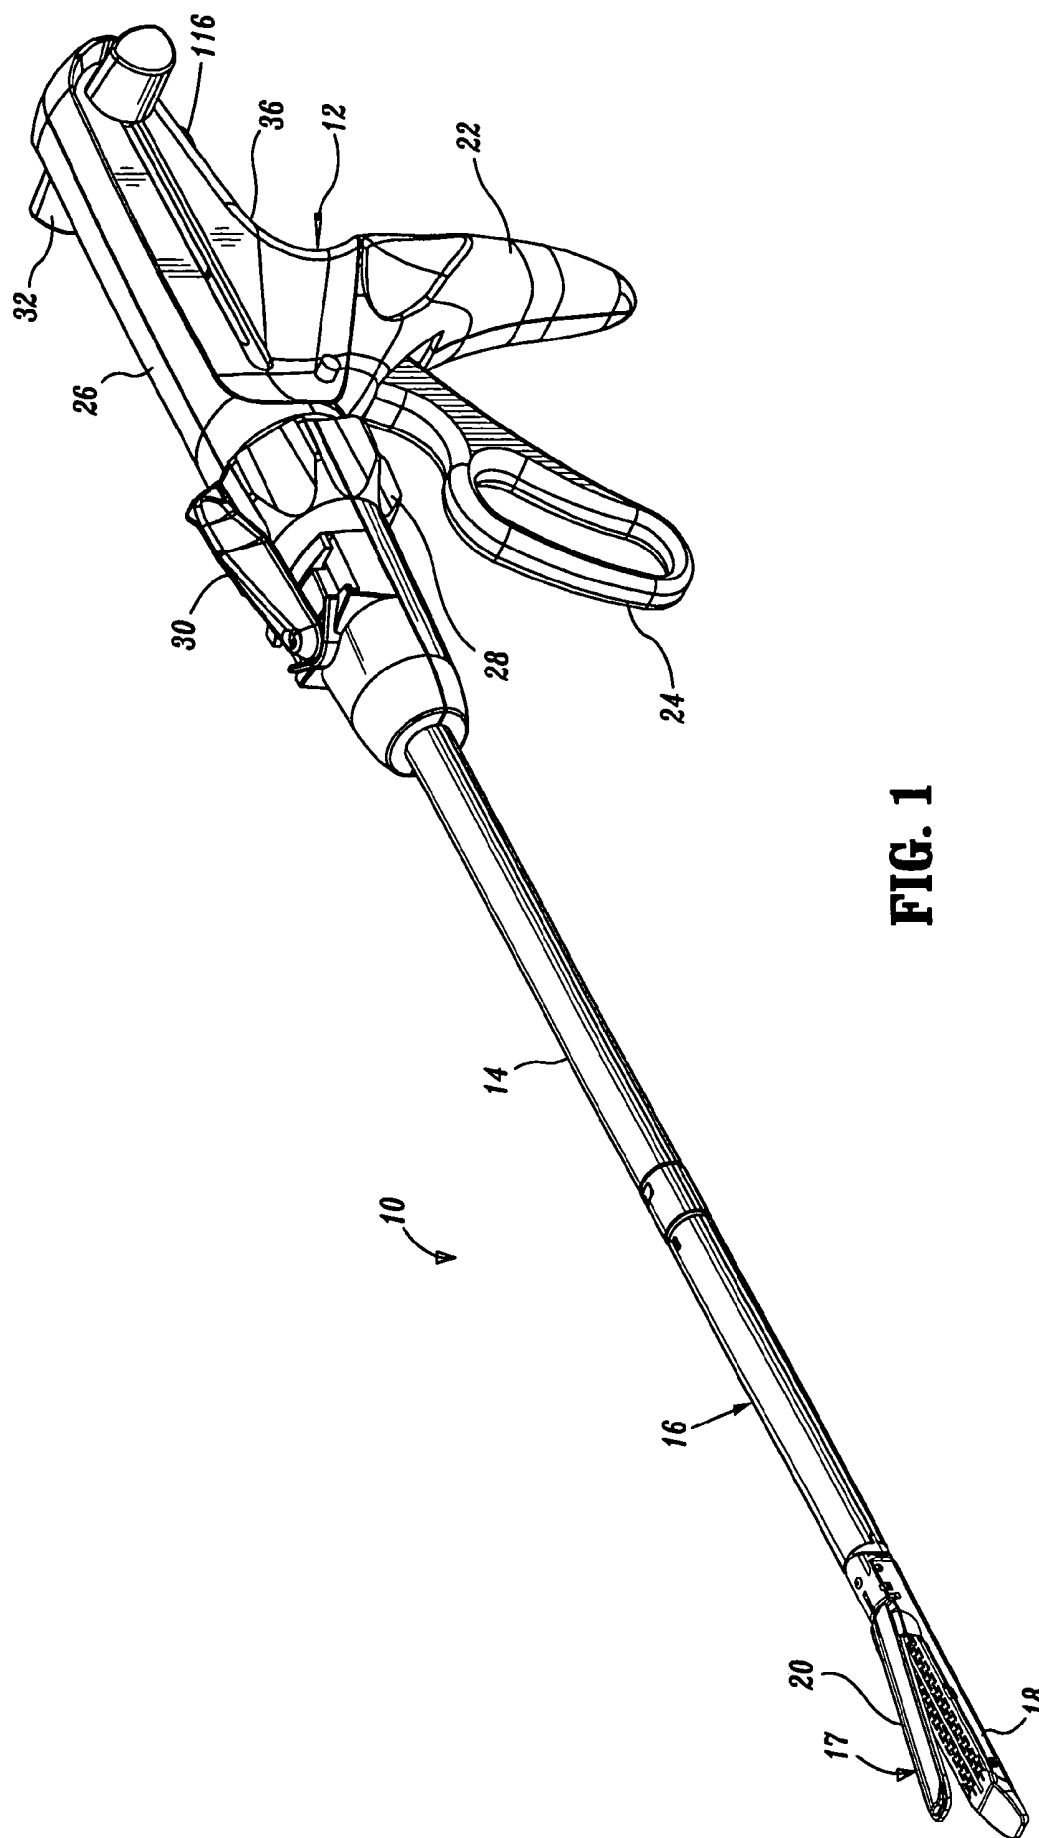


FIG. 1

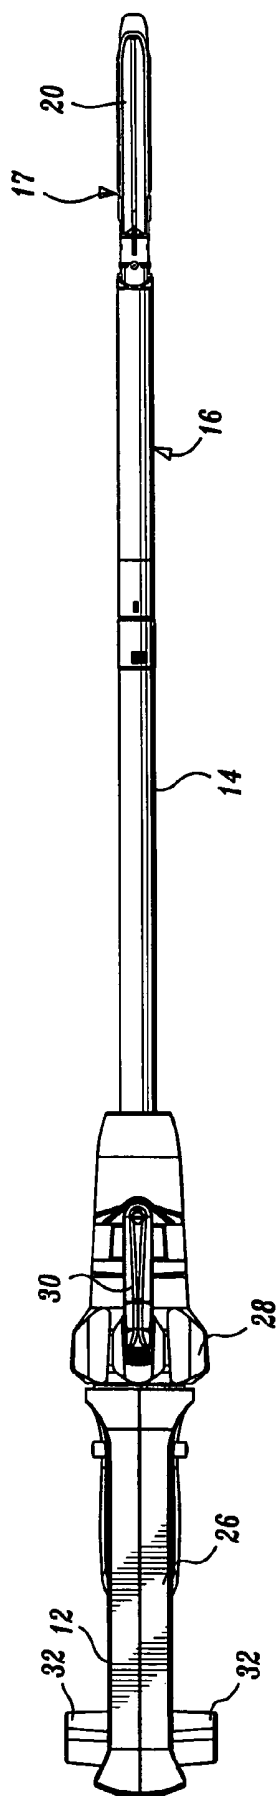


FIG. 2

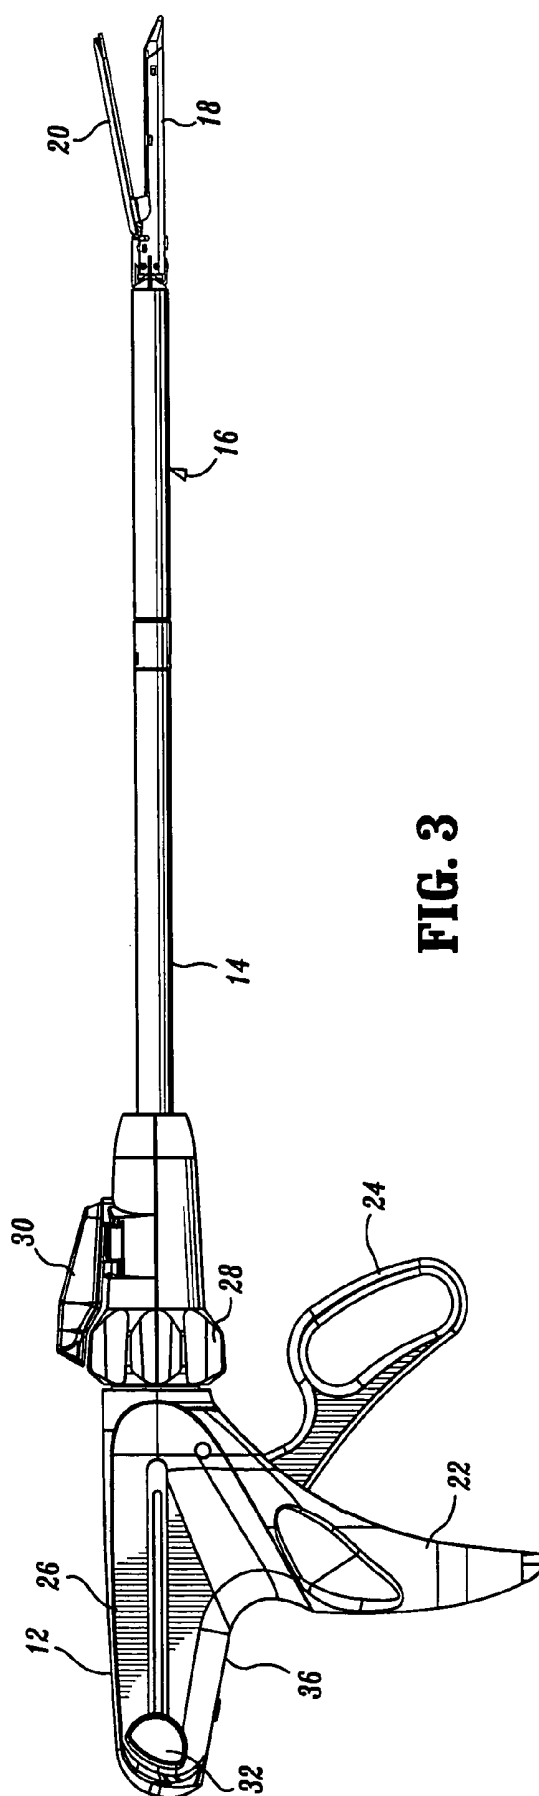


FIG. 3

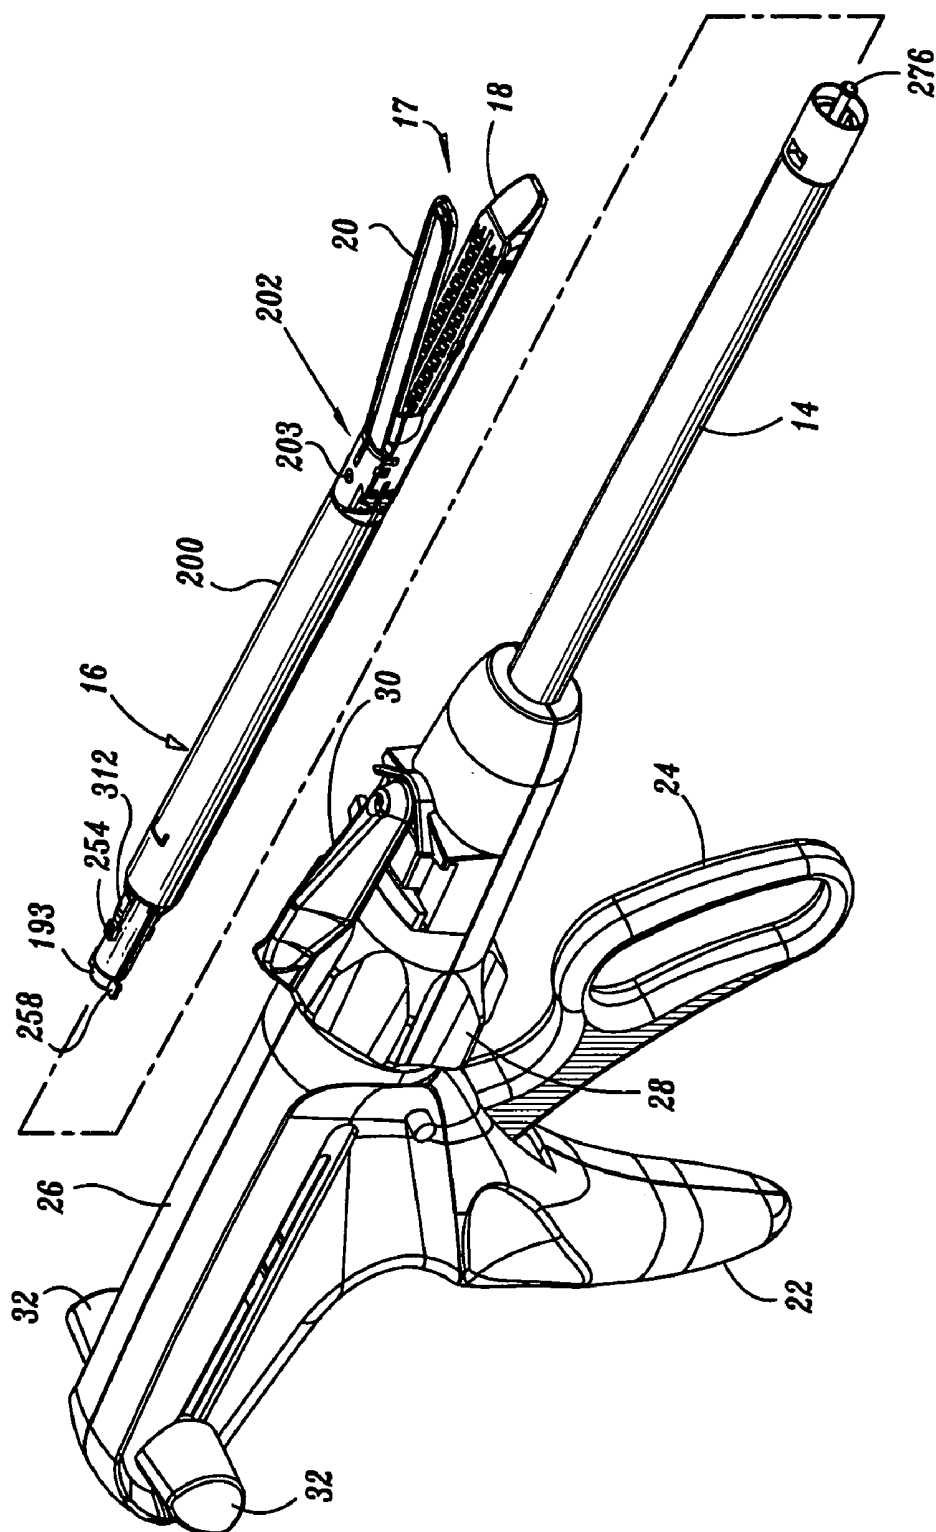


FIG. 4

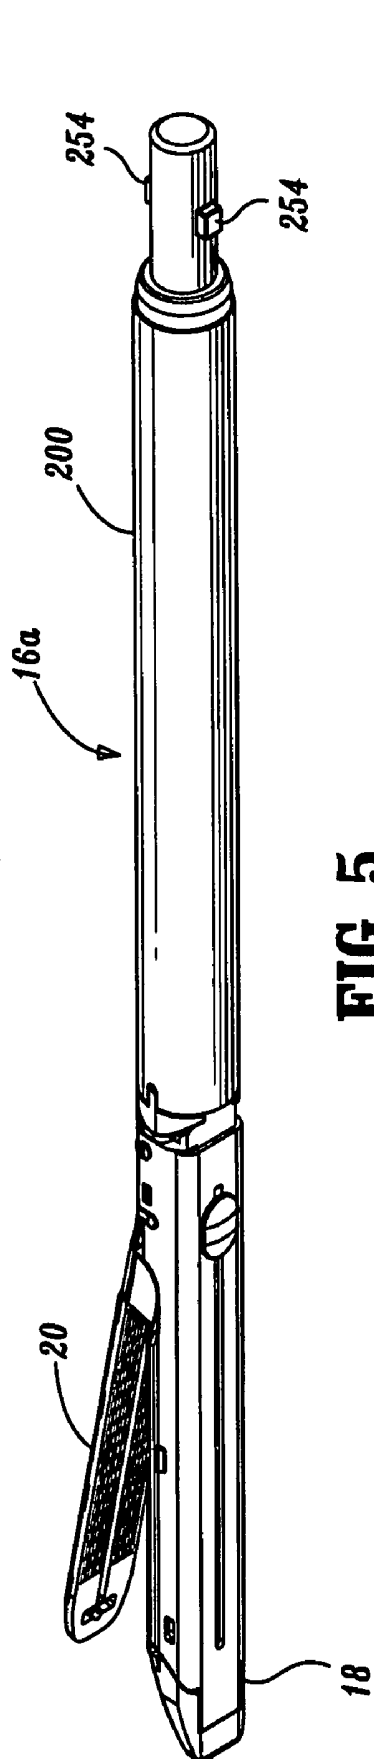


FIG. 5

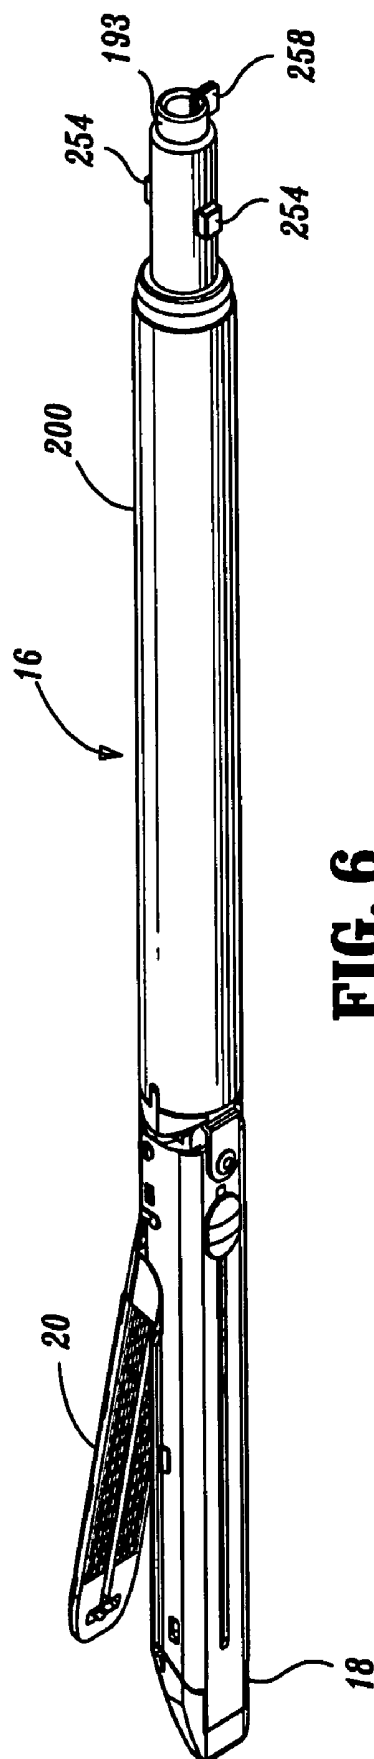


FIG. 6

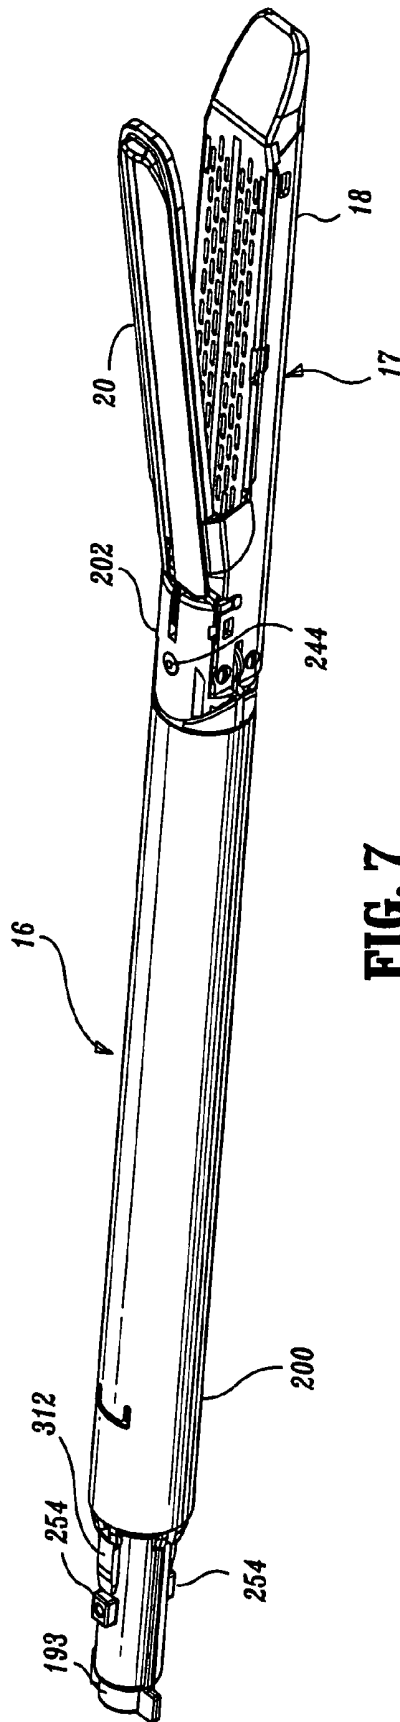


FIG. 7

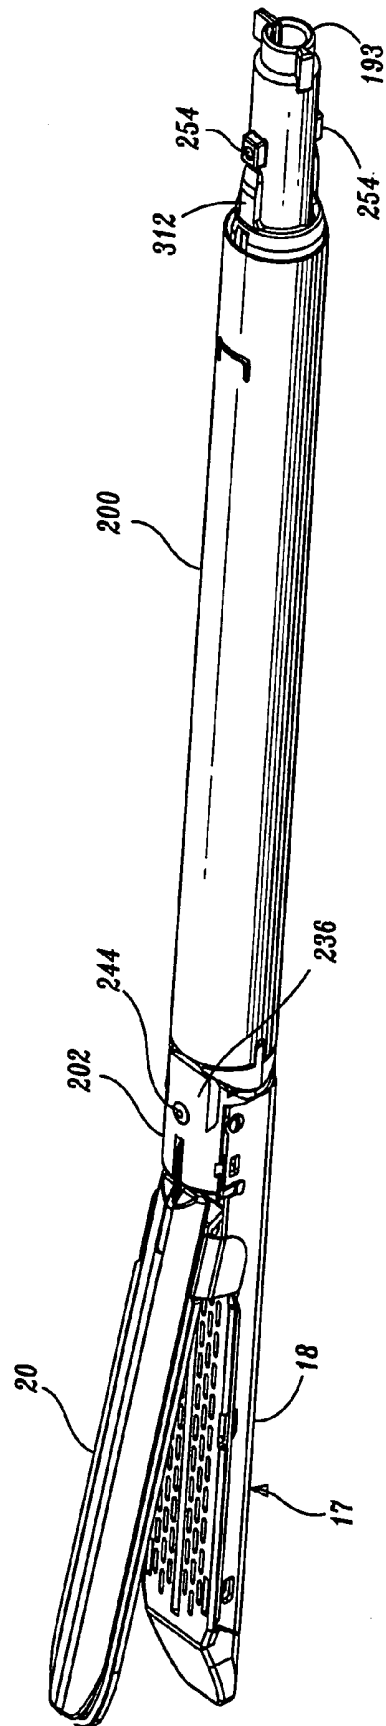


FIG. 8

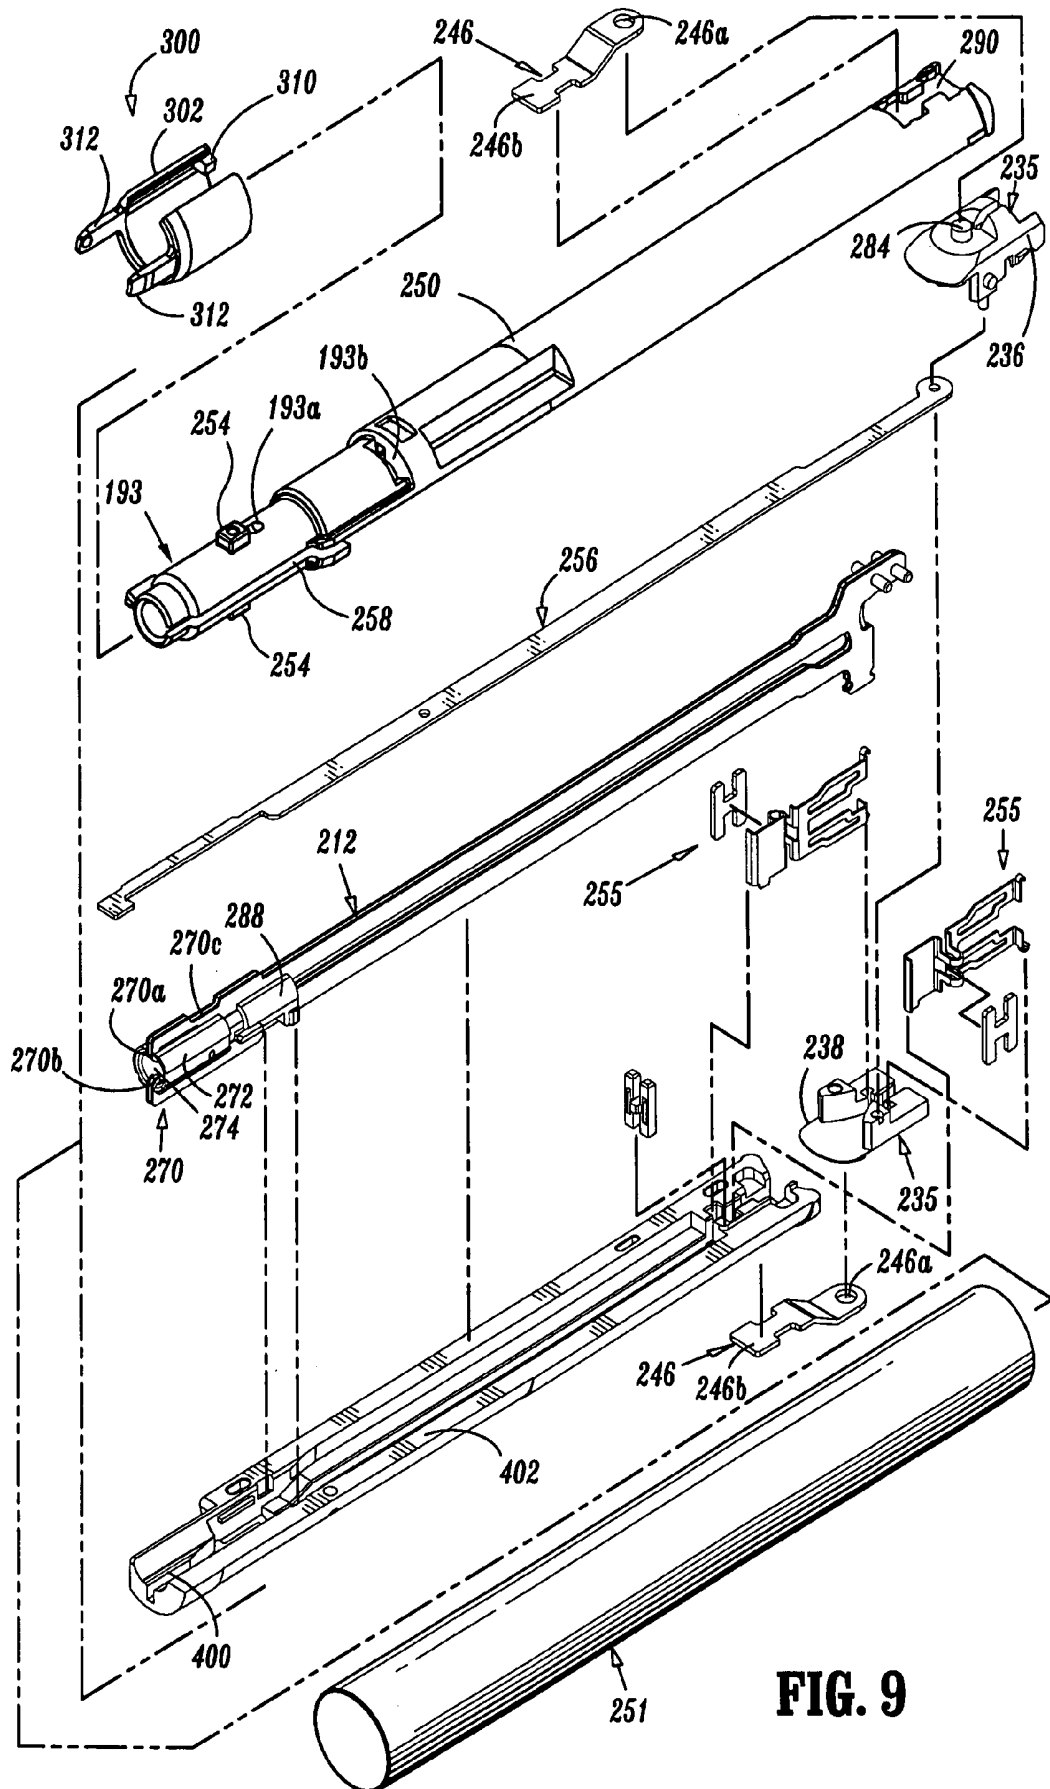
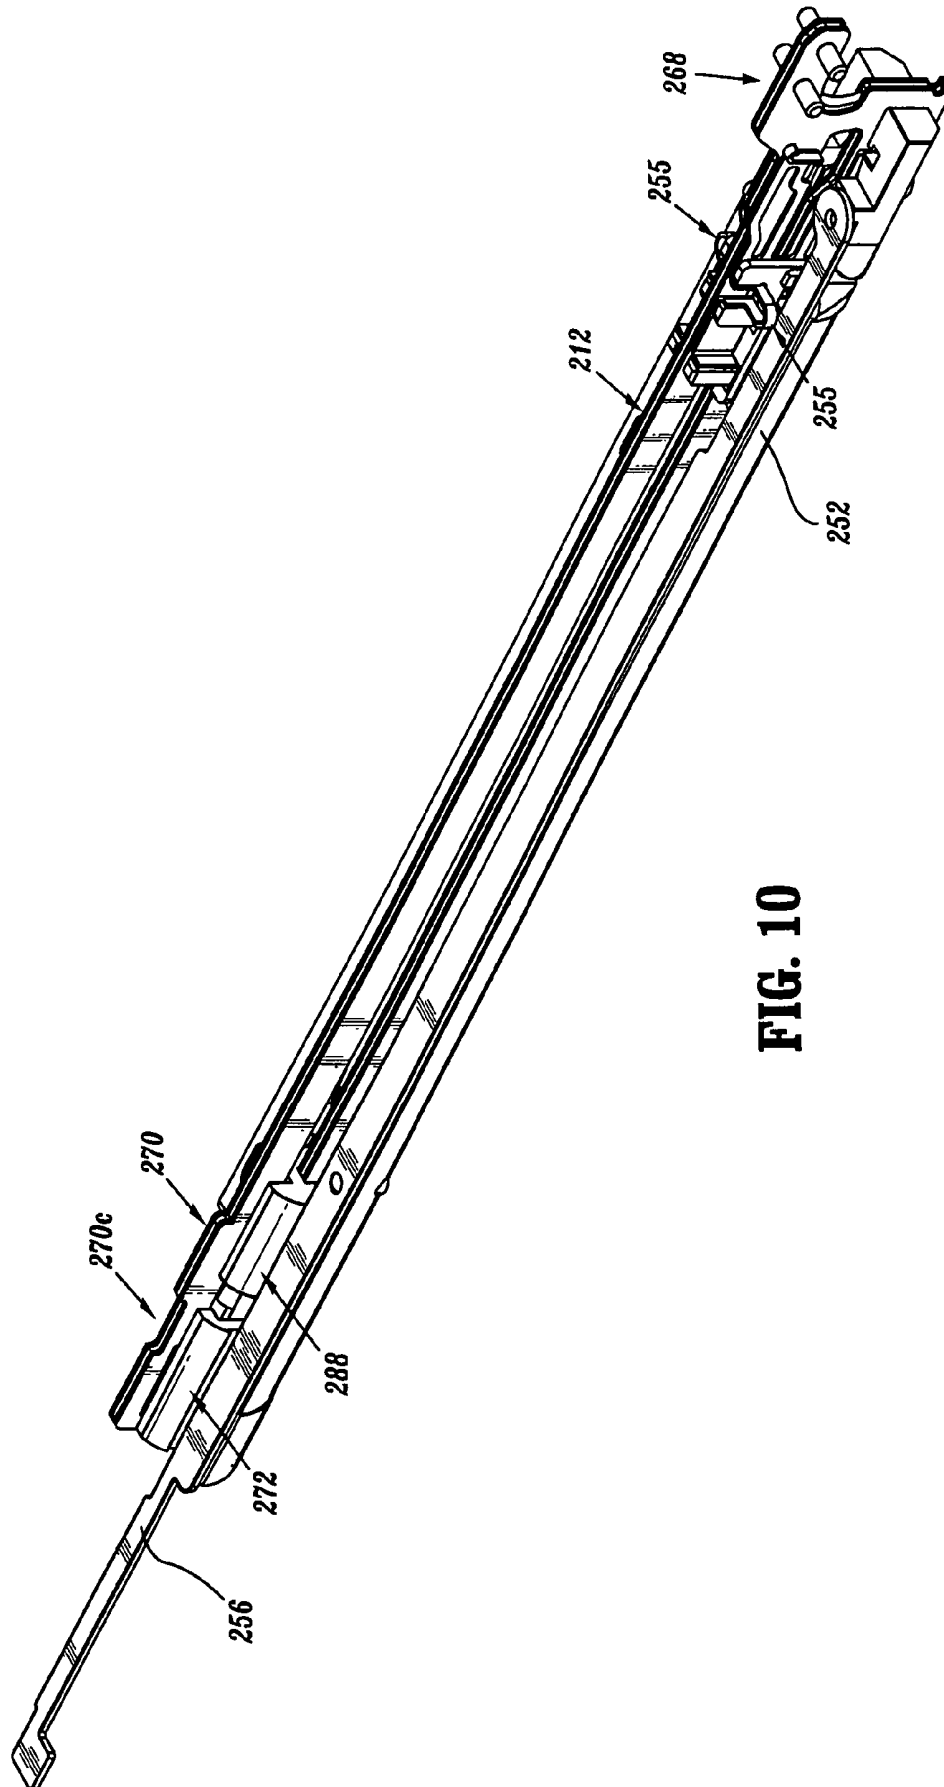


FIG. 9



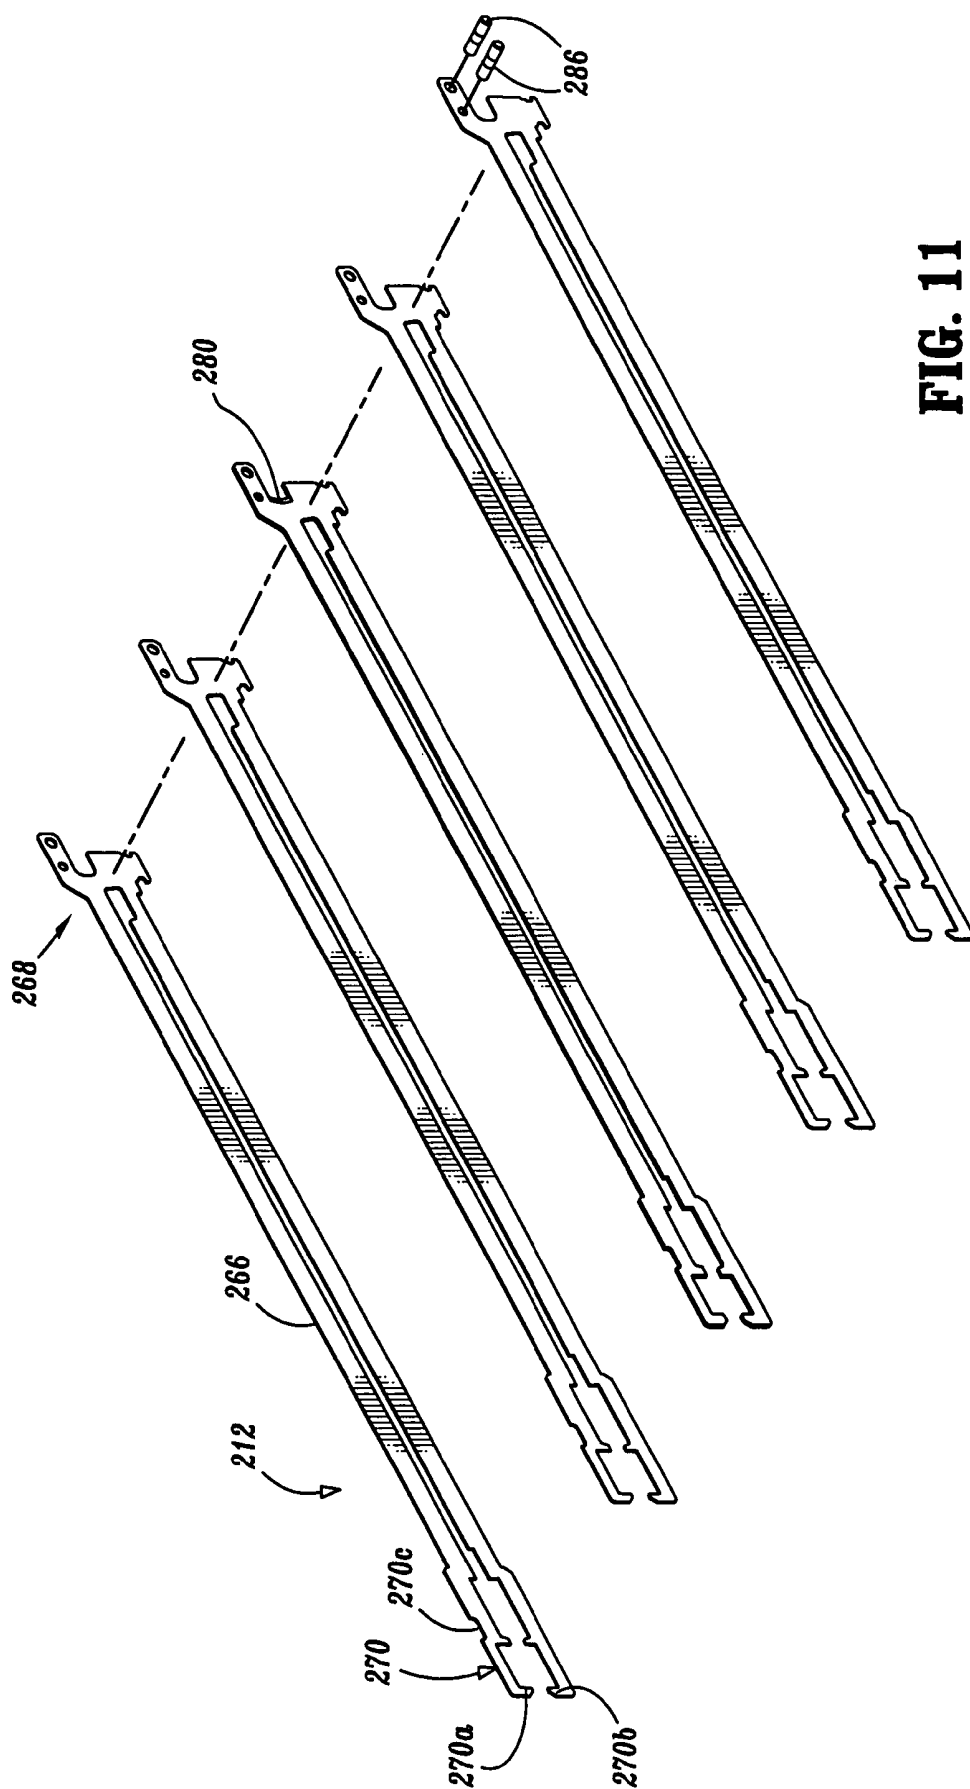
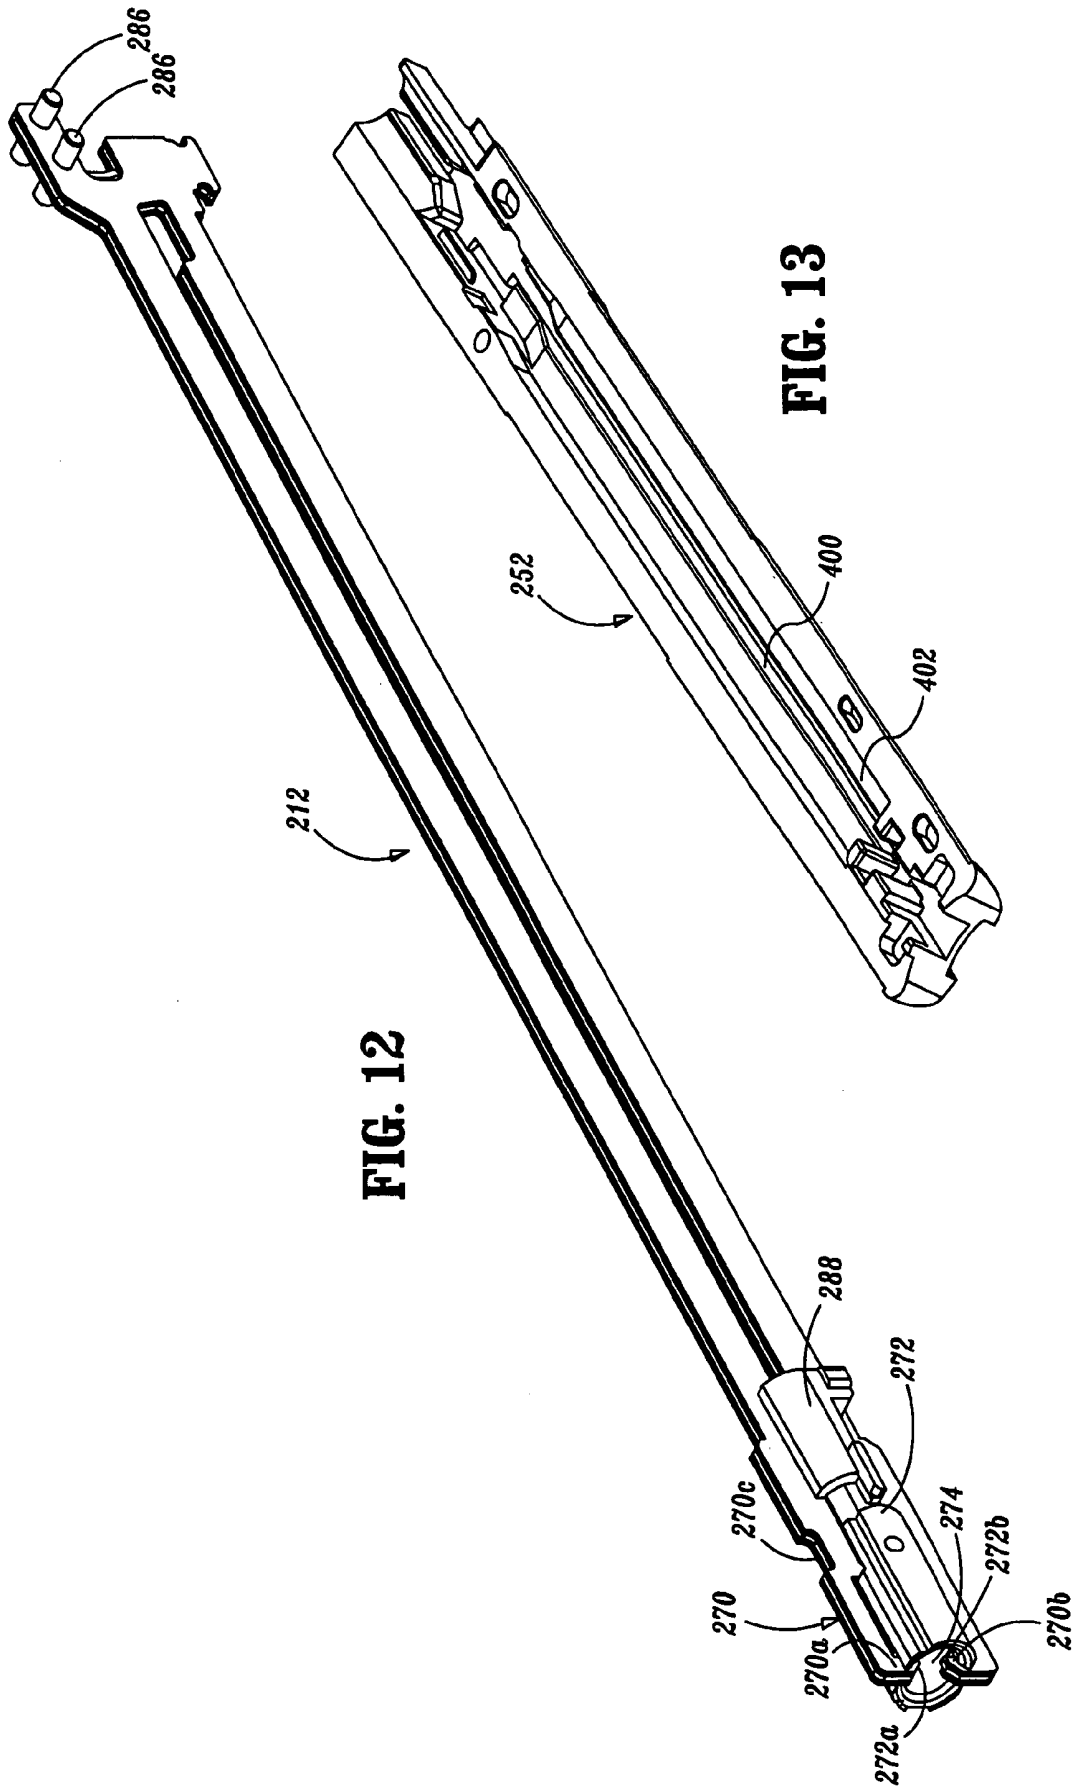
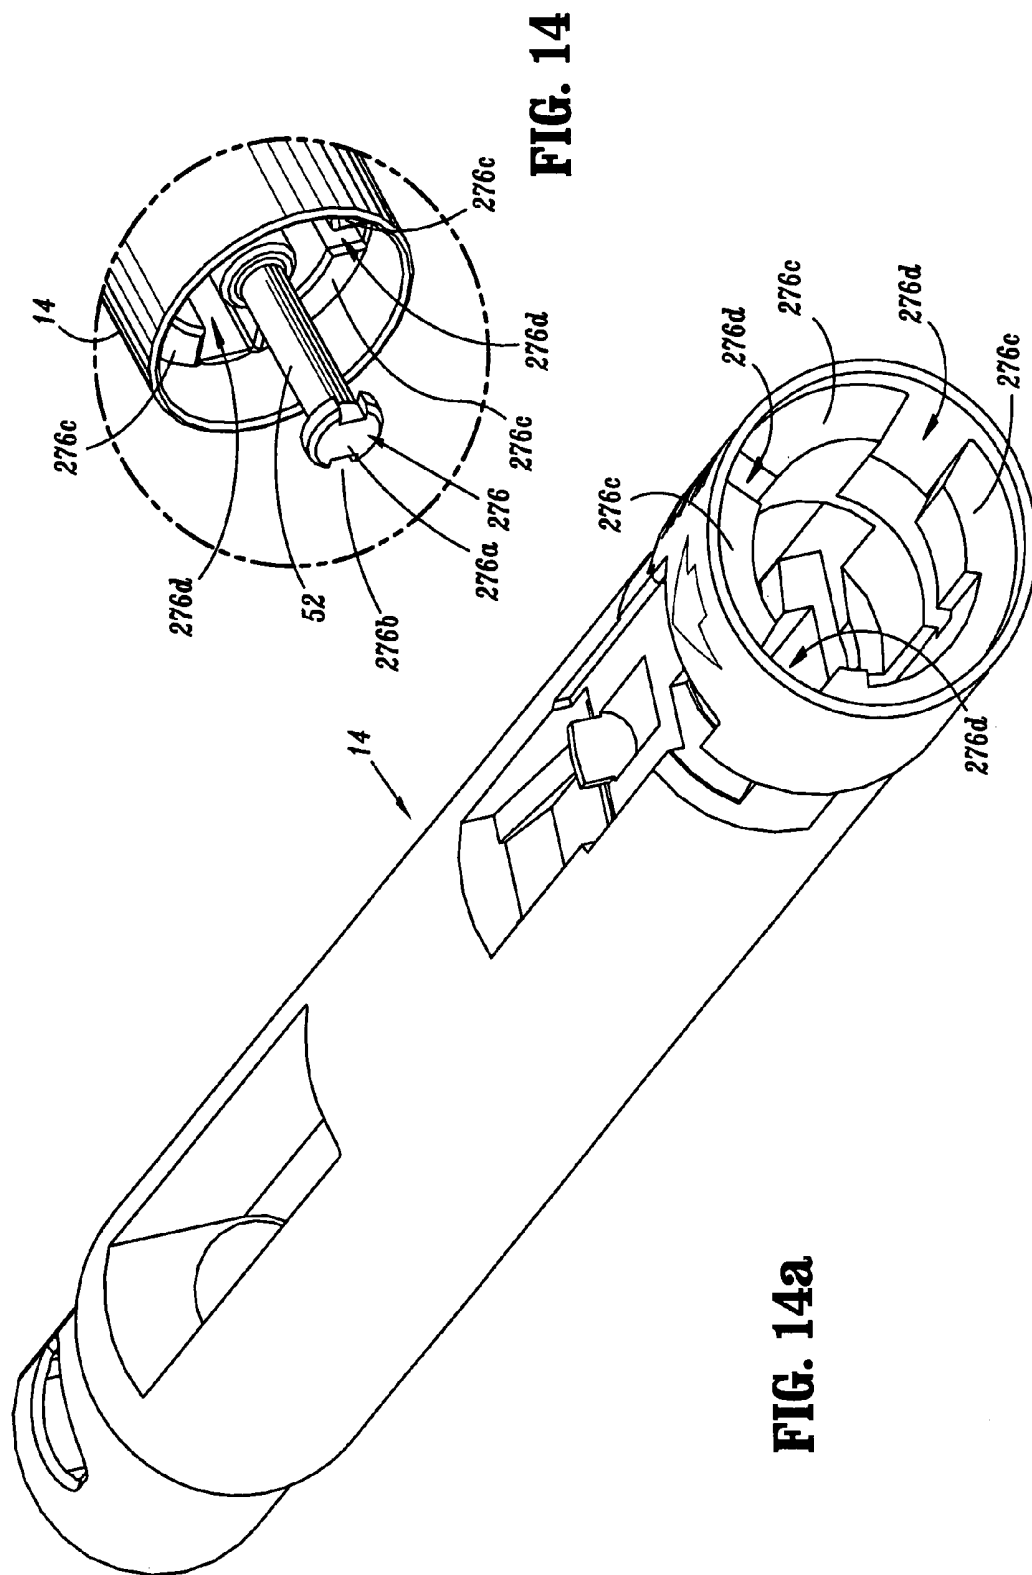


FIG. 11





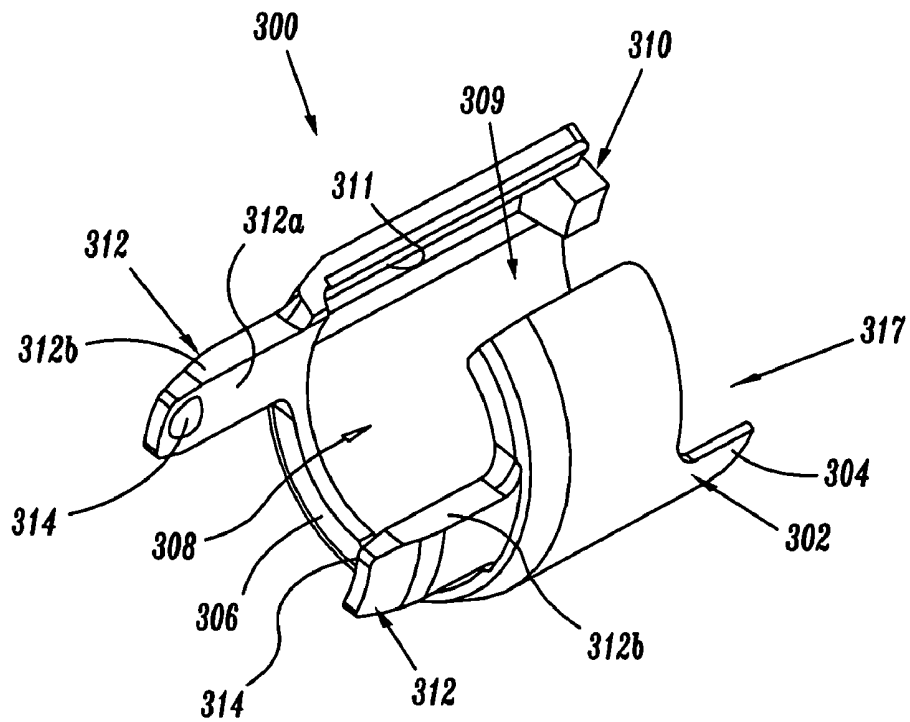


FIG. 15

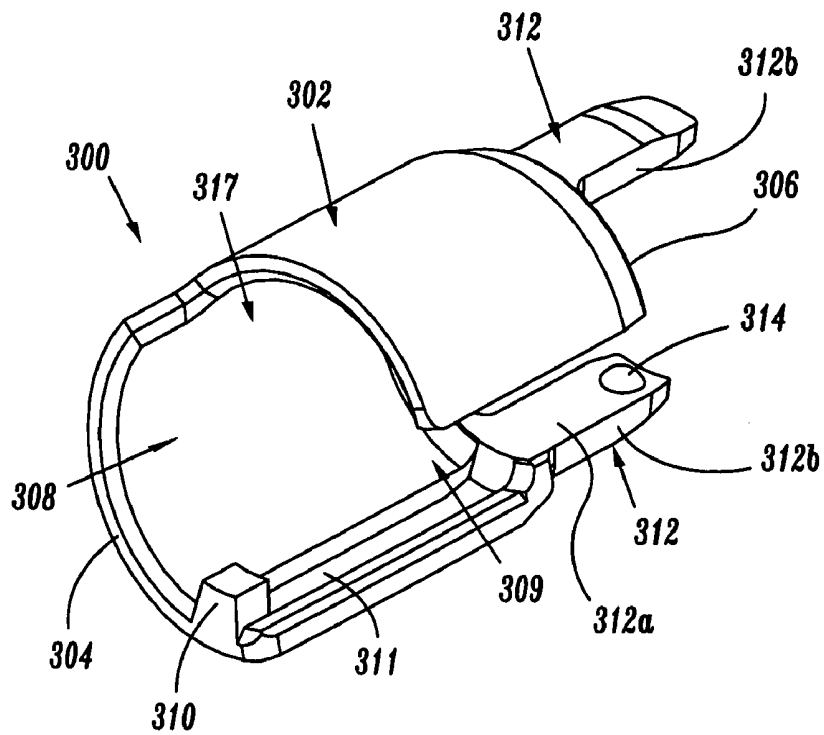
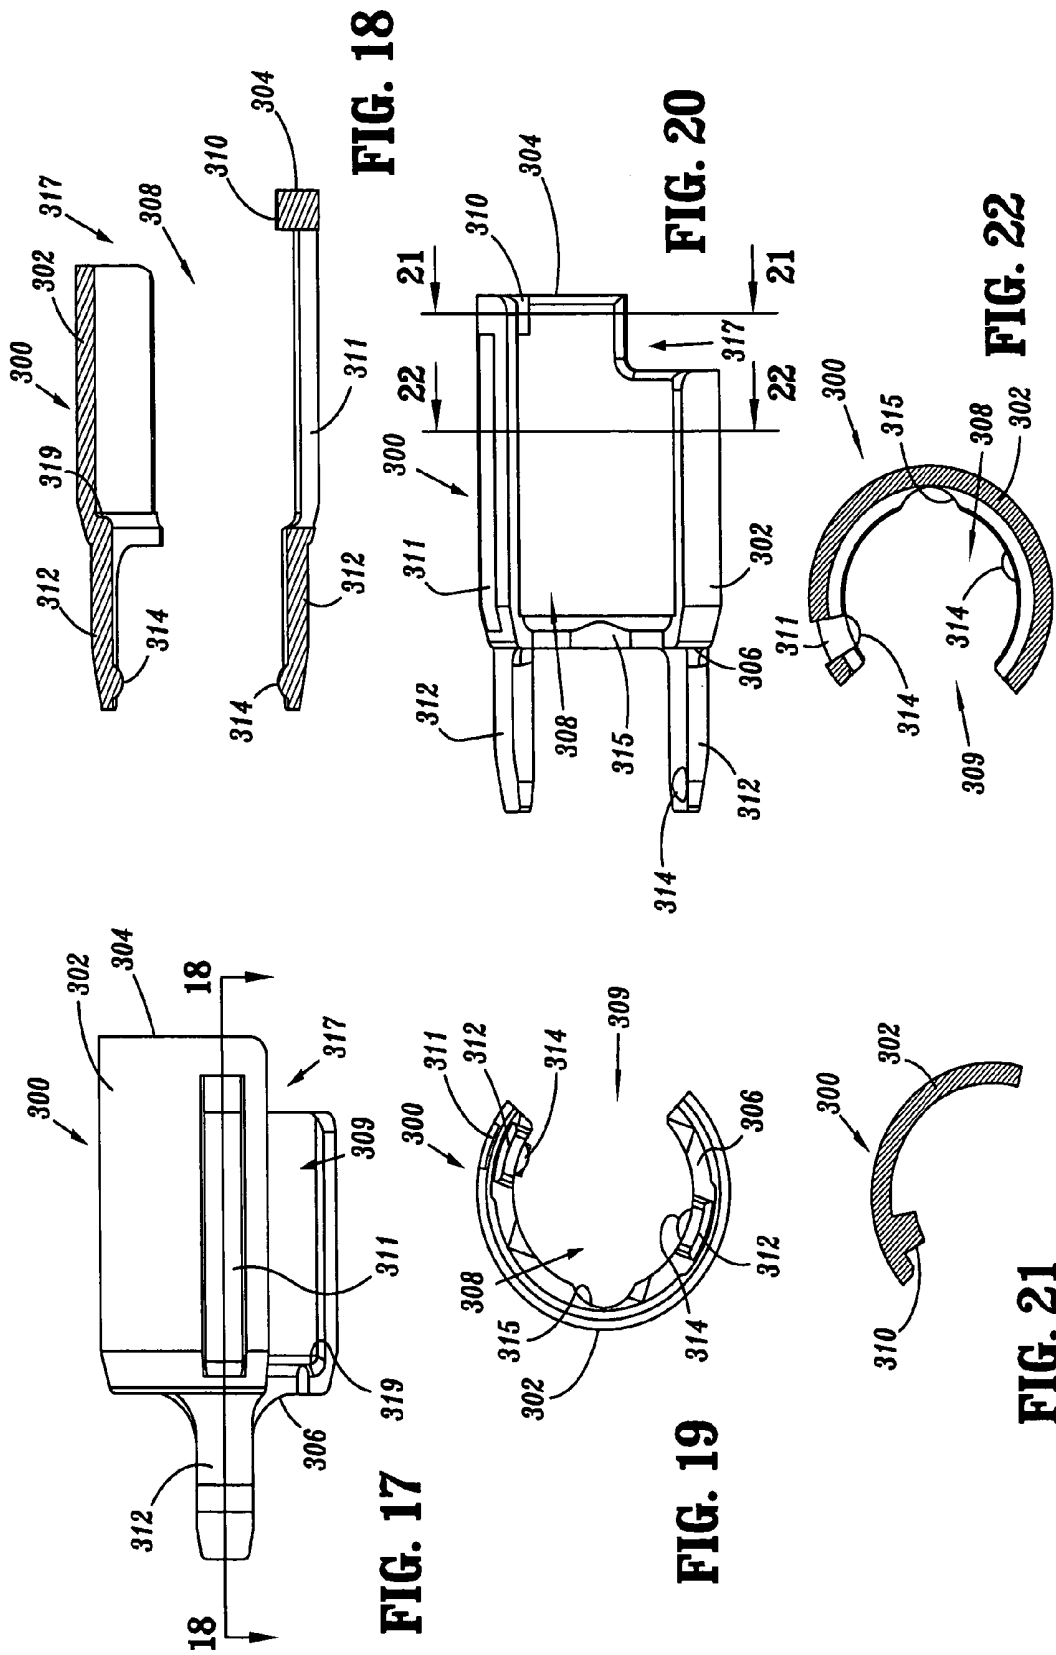
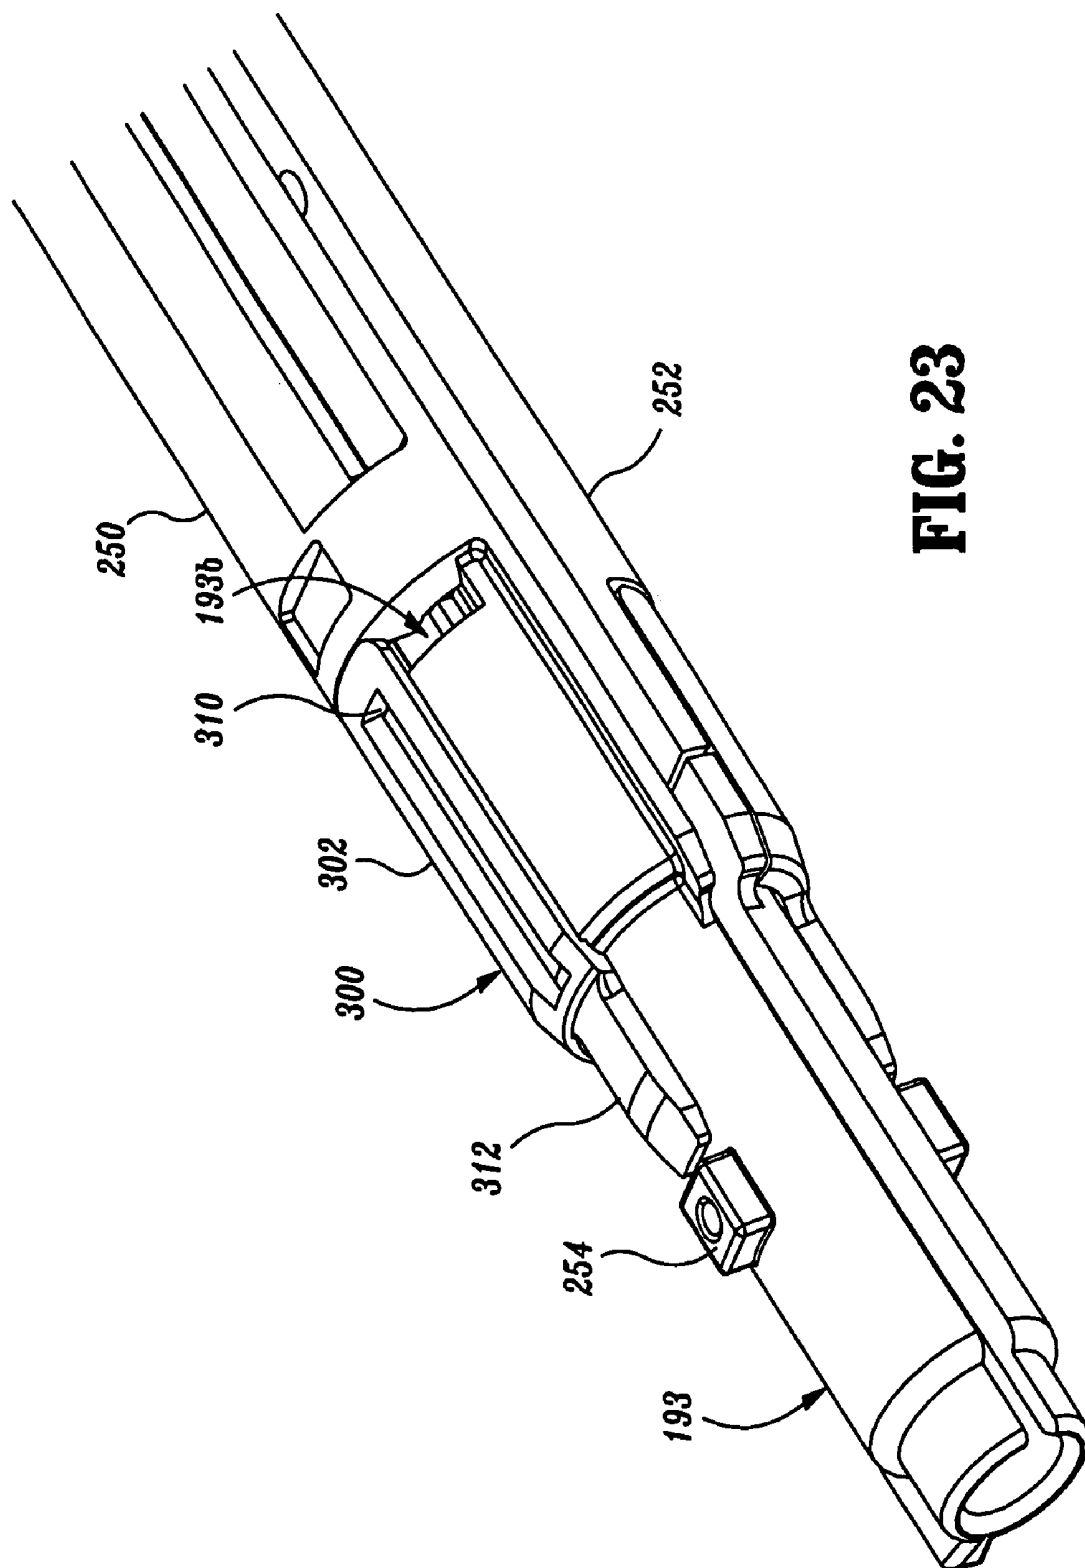


FIG. 16





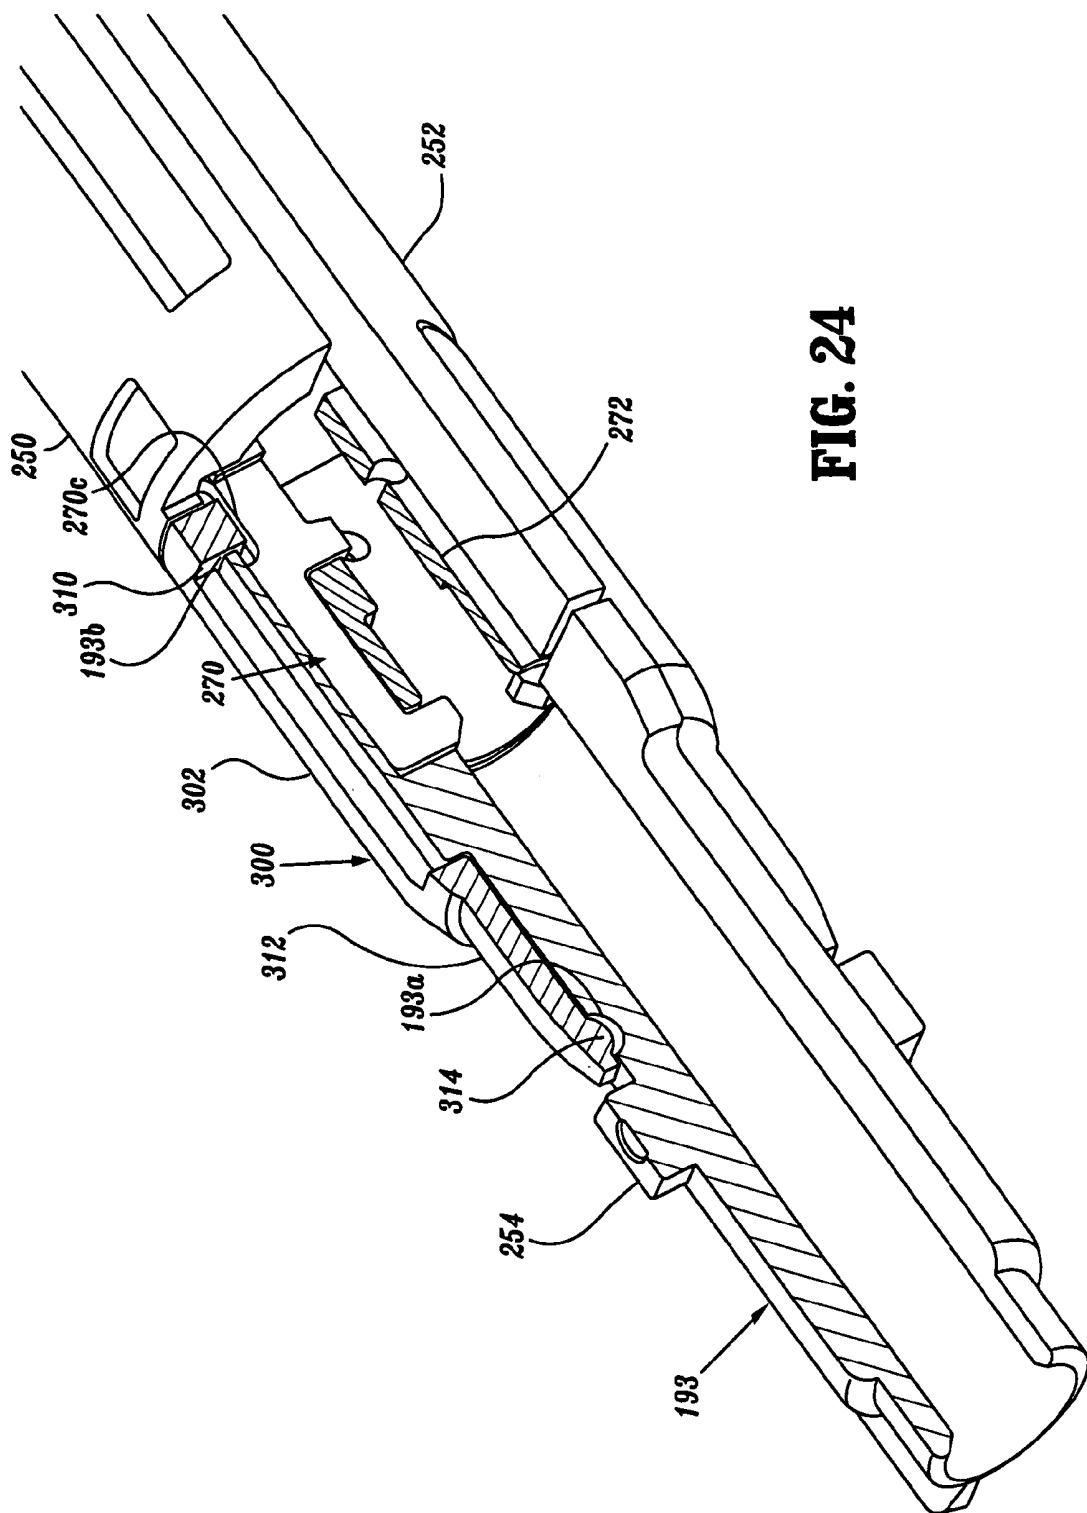


FIG. 24

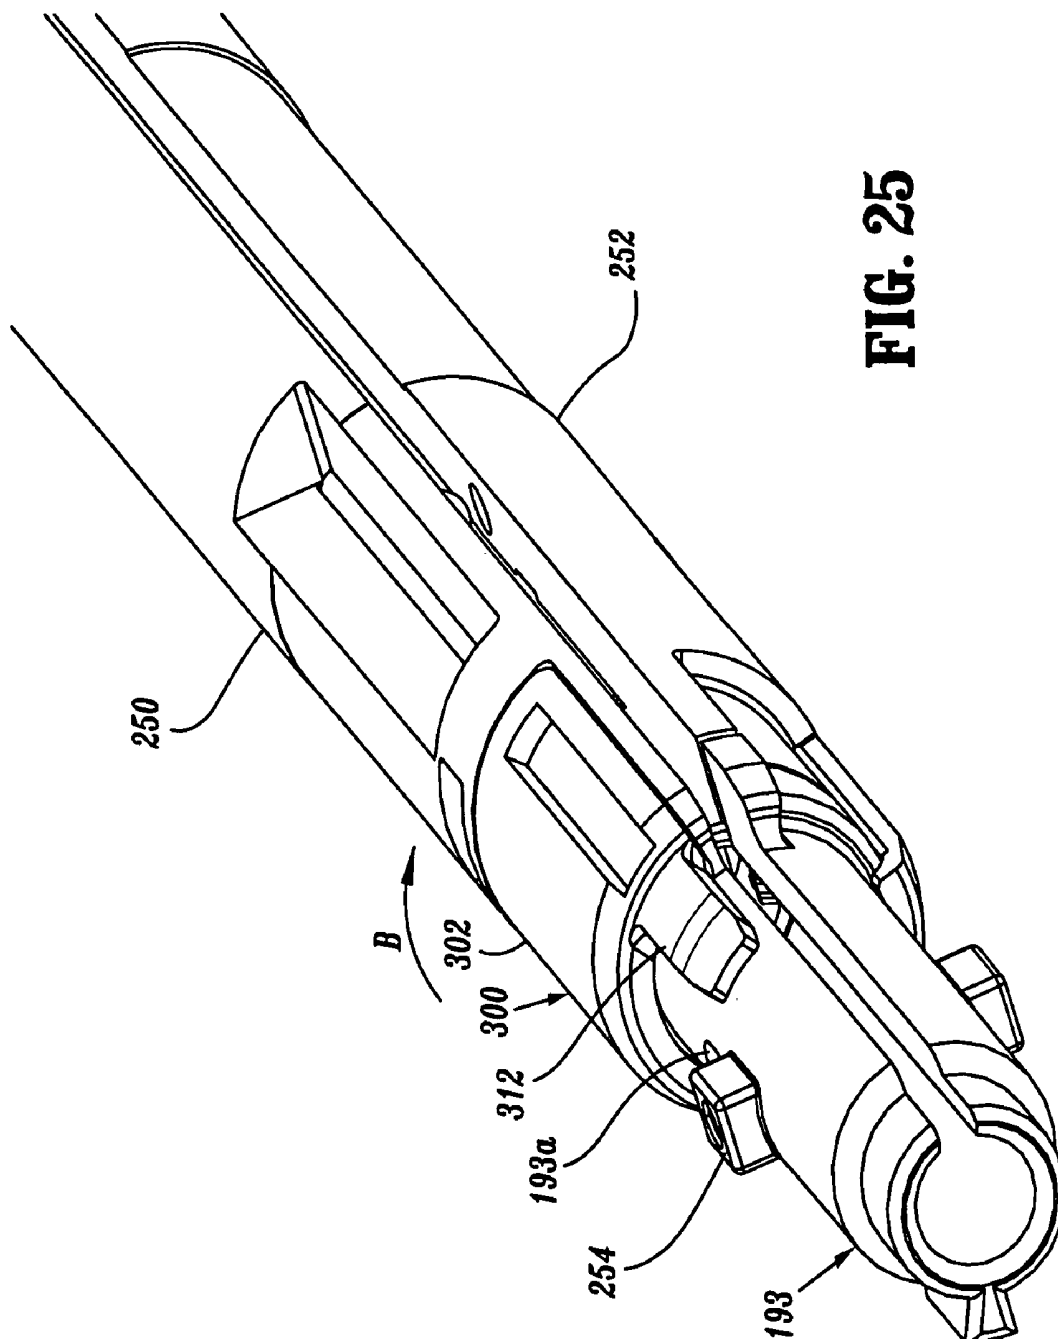
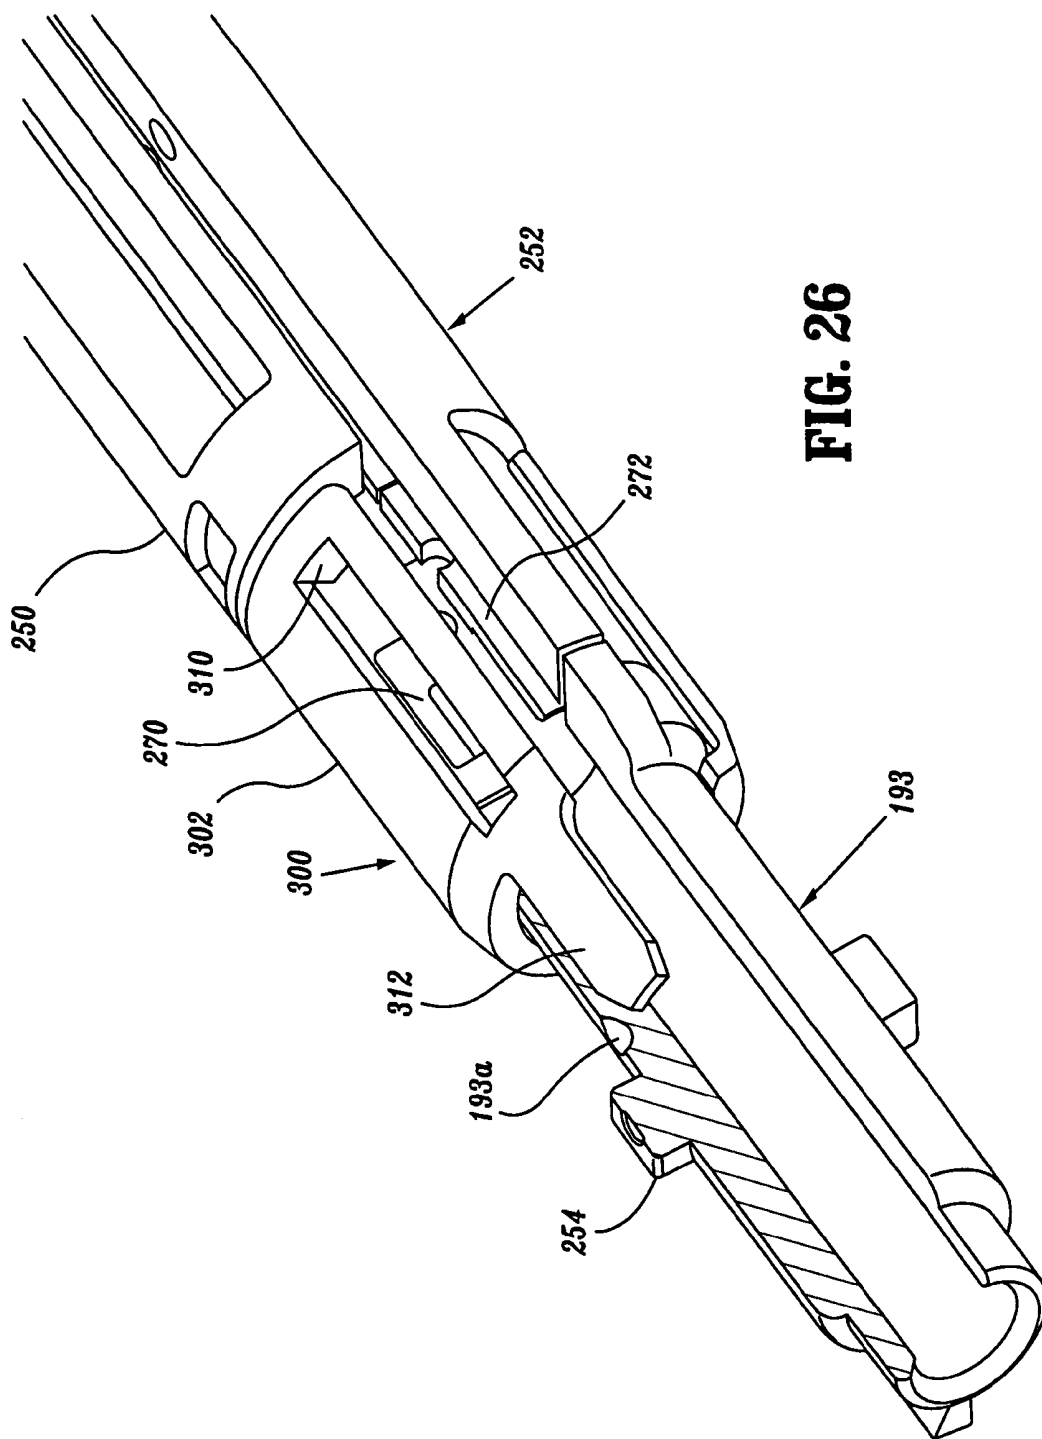


FIG. 25



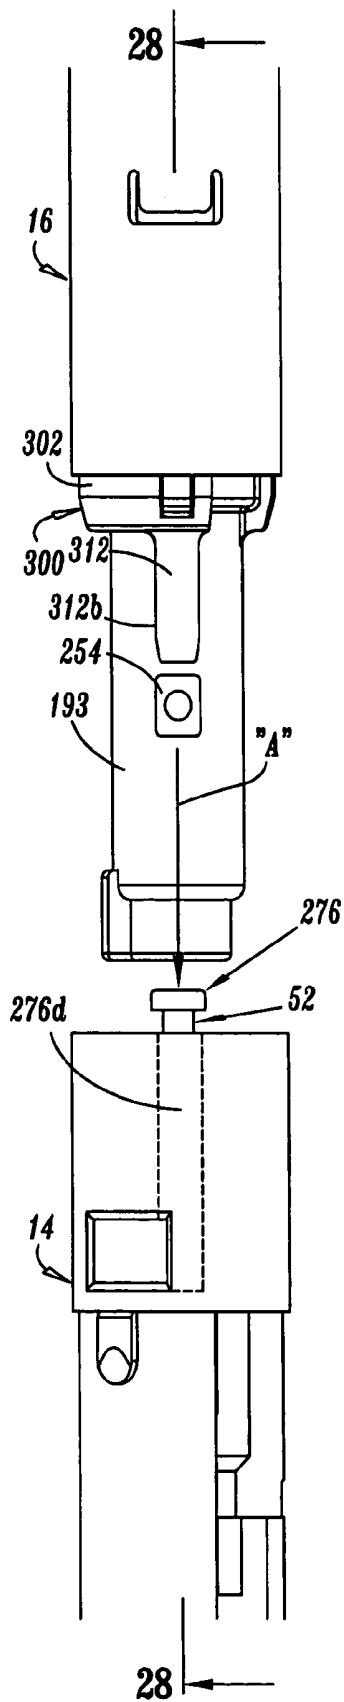


FIG. 27

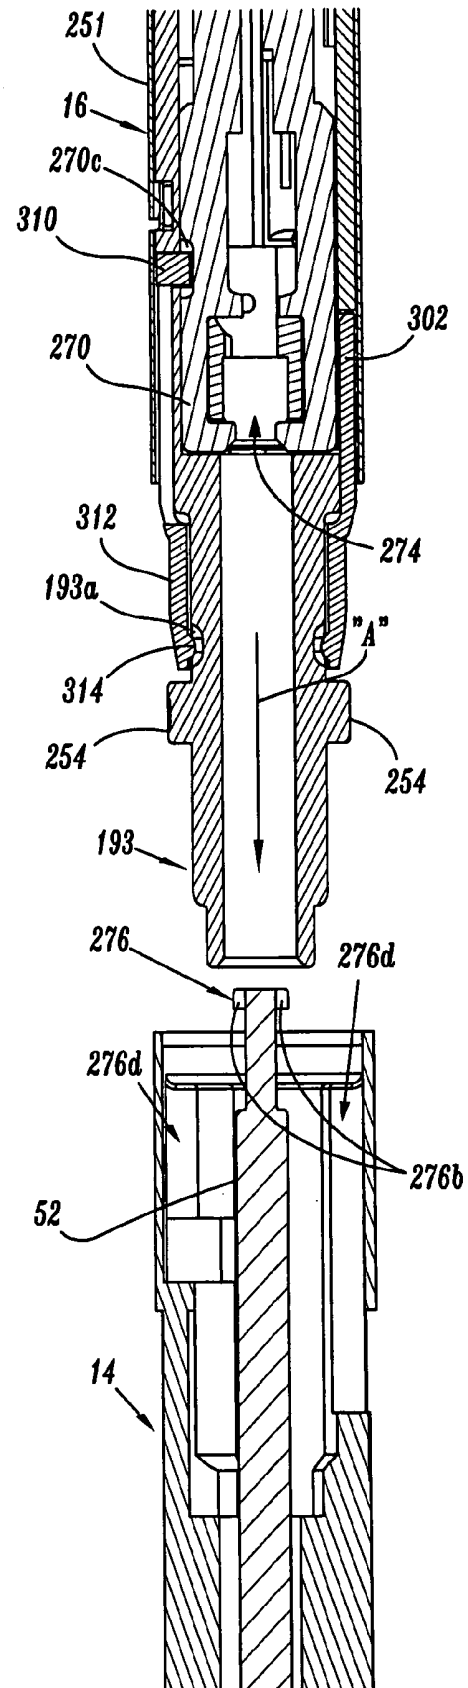


FIG. 28

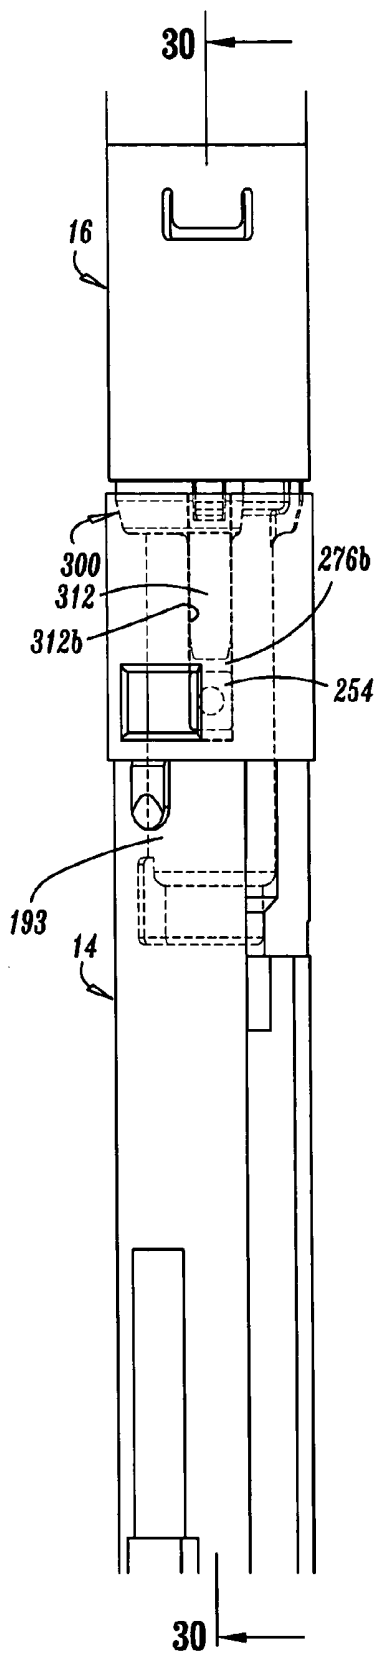


FIG. 29

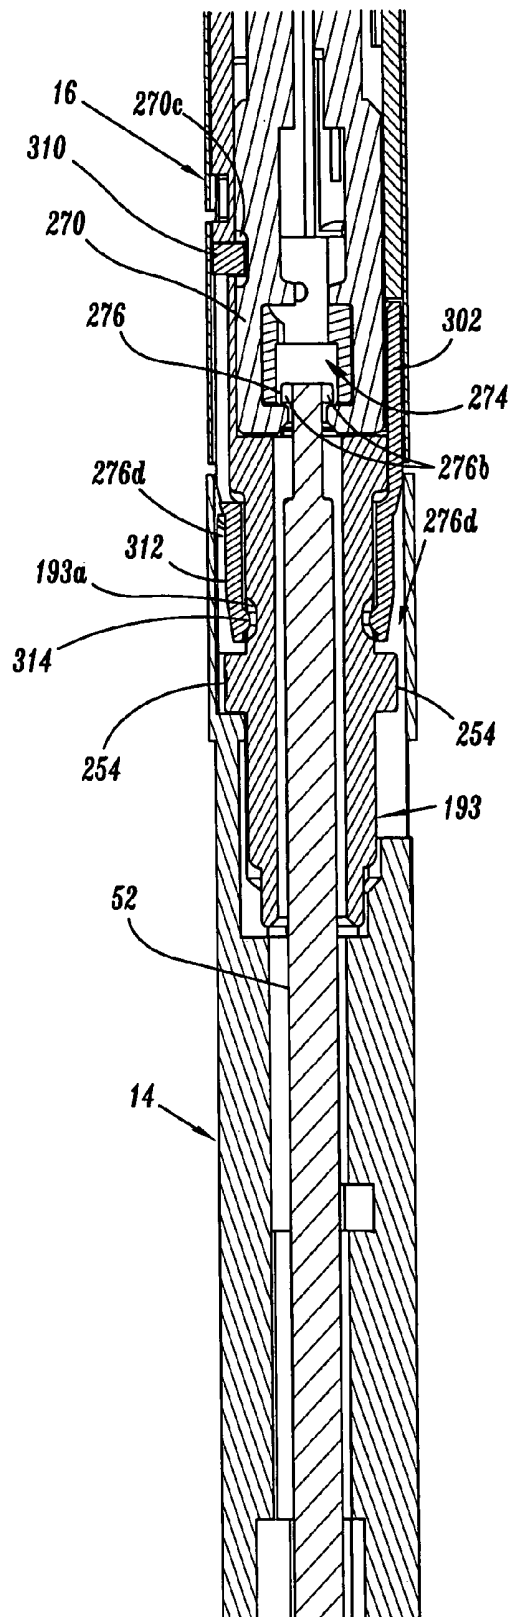


FIG. 30

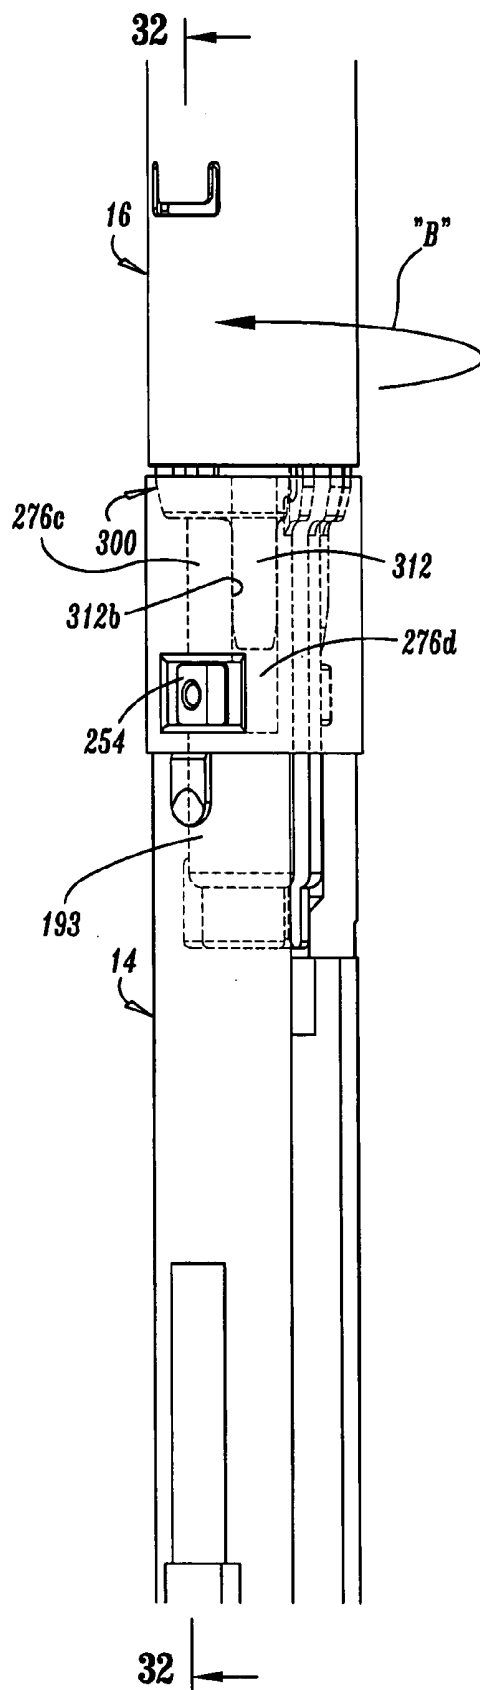


FIG. 31

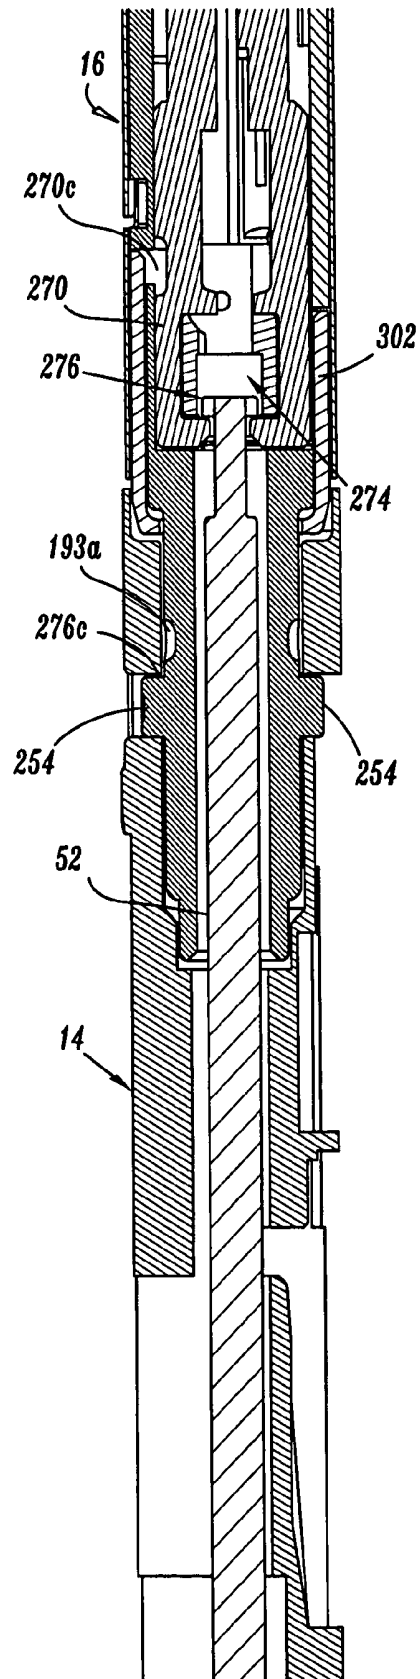


FIG. 32

SURGICAL STAPLING APPARATUS WITH LOCKING MECHANISM

CROSS-REFERENCE TO RELATED APPLICATION

The present application claims the benefit of and priority to U.S. Provisional Application Ser. No. 60/545,619, filed Feb. 17, 2004, the entire content of which being incorporated herein by reference.

BACKGROUND

1. Technical Field

The present disclosure relates to a surgical apparatus, e.g., a surgical stapling apparatus. More particularly, the present disclosure relates to an endoscopic surgical stapling apparatus that includes a locking mechanism including a locking member for retaining the drive assembly of a loading unit, e.g., a single use loading unit ("SULU") or disposable loading unit ("DLU"), at a substantially fixed axial position until the SULU or DLU has been loaded with or secured to a surgical stapling apparatus, to ensure proper or complete engagement of the SULU or DLU, especially its drive assembly, to the surgical stapling apparatus. For simplicity, hereinafter, SULU or DLU will be referred to as "DLU", but it should be understood to include either or both a DLU or SULU.

2. Background of Related Art

Surgical devices wherein tissue is first grasped or clamped between opposing jaw structure and then joined by surgical fasteners are well known in the art. In some instruments a knife is provided to cut the tissue which has been joined by the fasteners. The fasteners are typically in the form of surgical staples but two part polymeric fasteners can also be utilized.

Instruments for this purpose can include two elongated jaw members which are respectively used to capture or clamp tissue. Typically, one of the jaw members carries a staple cartridge which houses a plurality of staples arranged in at least two lateral rows while the other jaw member has an anvil that defines a surface for forming the staple legs as the staples are driven from the staple cartridge. Generally, the stapling operation is effected by cam members that travel longitudinally through the staple cartridge, with the cam members acting upon staple pushers to sequentially eject the staples from the staple cartridge. A knife can travel between the staple rows to longitudinally cut and/or open the stapled tissue between the rows of staples. Such instruments are disclosed, for example, in U.S. Pat. No. 3,079,606 and U.S. Pat. No. 3,490,675.

A later stapler disclosed in U.S. Pat. No. 3,499,591 also applies a double row of staples on each side of the incision. This patent discloses a surgical stapler that has a disposable loading unit in which a cam member moves through an elongate guide path between two sets of staggered staple carrying grooves. Staple drive members are located within the grooves and are positioned in such a manner so as to be contacted by the longitudinally moving cam member to effect ejection of the staples from the staple cartridge of the disposable loading unit. Other examples of such staplers are disclosed in U.S. Pat. Nos. 4,429,695 and 5,065,929.

Each of the instruments described above is designed for use in conventional surgical procedures wherein surgeons have direct manual access to the operative site. However, in endoscopic or laparoscopic procedures, surgery is performed through a small incision or through a narrow cannula

inserted through small entrance wounds in the skin. In order to address the specific needs of endoscopic and/or laparoscopic surgical procedures, endoscopic surgical stapling devices have been developed and are disclosed in, for example, U.S. Pat. No. 5,040,715 (Green, et al.); U.S. Pat. No. 5,307,976 (Olson, et al.); U.S. Pat. No. 5,312,023 (Green, et al.); U.S. Pat. No. 5,318,221 (Green, et al.); U.S. Pat. No. 5,326,013 (Green, et al.); U.S. Pat. No. 5,332,142 (Robinson, et al.); and U.S. Pat. No. 6,241,139 (Milliman et al.), the entire contents of each of which are incorporated herein by reference.

Tyco Healthcare Group, LP, the assignee of the present application, has manufactured and marketed endoscopic stapling instruments, such as the Multifire ENDO GIA™ 30 and Multifire ENDO GIA™ 60 instruments, for a number of years. These instruments include a surgical stapling apparatus and a DLU. Typically, the DLU is attached to the apparatus immediately prior to surgery. After use, the DLU can be removed from the apparatus and a new DLU can be fastened to the apparatus to perform additional stapling and/or cutting operations. These instruments have provided significant clinical benefits. Nonetheless, improvements to these instruments are still possible.

It would be desirable to provide an improved DLU for a surgical stapling apparatus and an improved surgical stapling apparatus having the DLU loaded thereon.

It would also be desirable to provide a locking member for a DLU to assure proper loading of the DLU to the shaft of a surgical stapling apparatus.

Accordingly, it is an object of this disclosure to provide an improved DLU which locks or retains its drive assembly in proper position to be loaded onto the shaft of a surgical stapling apparatus (hereinafter referred to as the or a "ready-to-load position") until the DLU is loaded onto a surgical stapling apparatus to assure that when the DLU is loaded thereto, the drive assembly is properly engaged by, coupled to or connected to a drive member of the shaft, thereby helping to ensure proper operation of the DLU and the surgical stapling apparatus. For example, with the DLU loaded onto the surgical stapling apparatus, after firing of the surgical stapling apparatus, retraction of the control rod will unapproximate or open and/or unclamp the anvil and cartridge assemblies.

An object of the disclosure is to provide an improved DLU that includes a locking member that retains the drive assembly in such ready-to-load position until the DLU is loaded onto the surgical stapling apparatus.

Another object of the disclosure is to provide such a locking member for a DLU.

Another object of the present disclosure is to provide a locking member for a DLU and a DLU having a locking member, such that firing of the surgical stapling apparatus is prevented unless and until the DLU is loaded onto the shaft of the surgical stapling apparatus.

Yet another object of the disclosure is to provide a DLU that, after firing, can be disconnected from the surgical stapling apparatus.

Still another object of the disclosure is to provide a DLU that has only two conditions, one in which it is not loaded and its drive assembly is locked or retained in the ready-to-load position, and another in which the DLU is loaded onto the shaft of a surgical stapling apparatus and in which the drive assembly is unlocked and free to be actuated.

Still another object of the present disclosure is to provide the above objects in a roticulating, i.e., roticlatable, DLU.

In accordance with the present disclosure, a surgical apparatus, e.g., a surgical stapling apparatus, which includes structure for cooperating with a locking mechanism or member of a disposable loading unit for ensuring proper engagement of the disposable loading unit to an end of the surgical apparatus is provided. According to one aspect of the present disclosure, the surgical apparatus includes a housing, a handle supported by the housing, and a loading unit, e.g., a DLU, removably supportable on a distal end of the housing. Preferably, the DLU includes a housing portion including a distal end and a proximal end, a drive assembly slidably supported within the housing portion of the DLU and a locking mechanism or member supported on the housing portion of the DLU. The locking member has a first position wherein the locking member engages and maintains the drive assembly in a ready-to-load position relative to the housing portion, e.g. the proximal end of the housing portion of the DLU. The locking member also has a second position wherein the locking member permits movement of the drive assembly relative to the housing portion.

The drive assembly preferably includes a notch. The locking member preferably includes a cuff-like body portion that substantially surrounds a portion of the proximal end of the housing portion of the housing portion. The locking member further includes a tooth that extends radially inward from the body portion and that is engagable with a notch formed in the drive assembly. In the first position of the locking member, the tooth engages the notch of the drive assembly and maintains the drive assembly in the ready-to-load position. In the second position of the locking member, the tooth is disengaged from the notch of the drive assembly.

The proximal end of the housing portion of the DLU can include an annular slot formed therein, to receive the tooth of the locking member therein.

Preferably, the surgical apparatus is a surgical fastener, preferably a surgical stapler, and more preferably, a laparoscopic or endoscopic surgical stapler.

It is envisioned that the locking member has a proximal end that has at least one finger that extends axially therefrom. As such, when the locking member is in the first position, the finger is axially aligned with a nub extending radially outward from the proximal end of the housing portion and when the locking member is in the second position, the finger is not in axial alignment with the nub of the proximal end of the housing portion.

It is envisioned that the housing has a projection that extends or is extendable radially inward thereof to move the locking member from the first position. In particular, the projection is configured to act on a side surface of the finger of the locking ring as the DLU is rotated into engagement with the housing.

The surgical apparatus may include an elongate body extending from the housing.

Desirably, the housing portion of the DLU defines an insertion tip.

The present disclosure also provides for a loading unit for use with a surgical stapling apparatus. The loading unit includes a housing portion having a distal end and a proximal end, a drive assembly slidably supported within the housing portion of the loading unit, and a locking member supported on the housing portion of the loading unit. The locking member is movable from a first position wherein the locking member engages the drive assembly and maintains the drive assembly in a ready-to-load position to a second

position wherein the locking member permits movement of the drive assembly relative to the housing portion.

The present disclosure further provides for a locking member for maintaining a drive assembly of a loading unit in a ready-to-load position when the loading unit is coupled to a surgical stapling apparatus. The locking member includes a cuff-like body portion that at least partially surrounds a proximal end of the loading unit, and a tooth extending radially inward from the body portion, wherein the tooth selectively engages a notch formed in the drive assembly such that when the locking member is in a first position the tooth engages the notch of the drive assembly and maintains the drive assembly in the ready-to-load position, and when the locking member is in a second position the tooth is disengaged from the notch of the drive assembly.

Additional advantages will become apparent from the description which follows, taken in conjunction with the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

The present disclosure will be further described with reference to the accompanying drawings, wherein like reference numerals refer to like parts in the several views, and wherein:

FIG. 1 is a top perspective view of a preferred embodiment of the presently disclosed surgical stapling apparatus;

FIG. 2 is a top view of the surgical stapling apparatus shown in FIG. 1;

FIG. 3 is a side view of the surgical stapling apparatus shown in FIGS. 1 and 2;

FIG. 4 is a top perspective view of the surgical stapling apparatus of FIGS. 1-3 with the DLU disengaged from the elongate body of the surgical stapling apparatus;

FIG. 5 is a bottom perspective view of a non-articulating DLU for use with the surgical stapling apparatus of FIGS. 1-4;

FIG. 6 is a bottom perspective view of the preferred articulating DLU of the surgical stapling apparatus of FIGS. 1-4;

FIG. 7 is a top perspective view of the DLU of FIG. 6; FIG. 8 is a top perspective view of the DLU of FIGS. 6 and 7;

FIG. 9 is an enlarged top perspective view, with parts separated, of the proximal housing portion and mounting assembly of the DLU of FIGS. 6-8;

FIG. 10 is a top perspective view of the proximal housing portion and mounting assembly of the DLU of FIGS. 6-9 with the upper housing half removed;

FIG. 11 is a top perspective view, with parts separated, of the axial drive assembly of the DLU of FIGS. 6-9;

FIG. 12 is a top perspective view of the axial drive assembly of FIG. 11 of the DLU of FIGS. 6-9;

FIG. 13 is an enlarged top perspective view of the lower housing half of the proximal housing portion of the DLU of FIGS. 6-9;

FIG. 14 is an enlarged perspective view of the distal end of the elongate body of the stapling apparatus shown in FIG. 4;

FIG. 14a is a further enlarged perspective view of the distal end of the elongate body of FIG. 14, shown without the control rod extending therethrough;

FIG. 15 is an enlarged front perspective view of a preferred locking member according to the present disclosure;

FIG. 16 is an enlarged rear perspective view of the locking member of FIG. 15;

5

FIG. 17 is a top elevational view of the locking member of FIGS. 15 and 16;

FIG. 18 is a longitudinal cross-sectional view of the locking member of FIGS. 15–17, as taken through 18–18 of FIG. 17;

FIG. 19 is a front elevational view of the locking member of FIGS. 15–18;

FIG. 20 is a side elevational view of the locking member of FIGS. 15–19;

FIG. 21 is a transverse cross-sectional view of the locking member of FIGS. 15–20, as taken through 21–21 of FIG. 20;

FIG. 22 is a transverse cross-sectional view of the locking member of FIGS. 15–20, as taken through 22–22 of FIG. 20;

FIG. 23 is an enlarged perspective view of the proximal end of the DLU of FIGS. 6–9 illustrating the locking member of FIGS. 15–22 situated in the first position;

FIG. 24 is an enlarged perspective view, partially cut away, of the proximal end of the DLU of FIGS. 6–9 further illustrating the locking member situated in the first position;

FIG. 25 is an enlarged perspective view of the proximal end of the DLU of FIGS. 6–9 illustrating the locking member situated in the second position;

FIG. 26 is an enlarged perspective view, partially cut away, of the proximal end of the DLU of FIGS. 6–9 further illustrating the locking member situated in the second position;

FIG. 27 is a top plan view, with portions broken away, illustrating a first stage in the attachment of the DLU of FIGS. 6–9 to the elongate body of the surgical stapling apparatus shown in FIGS. 1–3;

FIG. 28 is a longitudinal cross-sectional view of the first stage in the attachment of the DLU of FIGS. 6–9 to the elongate body of the surgical stapling apparatus shown in FIGS. 1–3, as taken along line 28–28 of FIG. 27;

FIG. 29 is a top plan view, with portions broken away, illustrating a second stage in the attachment of the DLU of FIGS. 6–9 to the elongate body of the surgical stapling apparatus shown in FIGS. 1–3;

FIG. 30 is a longitudinal cross-sectional view of the second stage in the attachment of the DLU of FIGS. 6–9 to the elongate body of the surgical stapling apparatus shown in FIGS. 1–3, as taken along line 30–30 of FIG. 29;

FIG. 31 is a top plan view, with portions broken away, illustrating a third stage in the attachment of the DLU of FIGS. 6–9 to the elongate body of the surgical stapling apparatus shown in FIGS. 1–3; and

FIG. 32 is a longitudinal cross-sectional view of the third stage in the attachment of the DLU of FIGS. 6–9 to the elongate body of the surgical stapling apparatus shown in FIGS. 1–3, as taken along line 32–32 of FIG. 31.

DETAILED DESCRIPTION OF PREFERRED EMBODIMENTS

Preferred embodiments of the presently disclosed surgical apparatus, DLU and locking mechanism or member will now be described in detail with reference to the drawings, in which like reference numerals designate identical or corresponding elements in each of the several views.

In the drawings and in the description that follows, the term “proximal”, as is traditional, will refer to the end of the stapling apparatus which is closest to the operator, while the term “distal” will refer to the end of the apparatus which is furthest from the operator.

6

FIGS. 1–4 show a surgical apparatus, e.g., surgical stapling apparatus, generally referred to as 10. In the interest of brevity, this disclosure will focus primarily on systems, methods and structures for loading, engaging, coupling or connecting a disposable loading unit (“DLU”) 16 to surgical stapling apparatus 10. A detailed discussion of the remaining components and method of use of surgical stapling apparatus 10, is disclosed in U.S. Pat. No. 6,241,139.

Surgical stapling apparatus 10 is an endoscopic apparatus and includes a handle assembly 12 and an elongated body 14 extending from handle assembly 12. A DLU 16 is releasably secured to the distal end of elongated body 14. While this disclosure relates to the use of a DLU with surgical stapling apparatus 10, it is understood and within the scope of the present disclosure that a single use loading unit (SULU) or other end effector and/or tool assembly can equally be used in cooperation with surgical stapling apparatus 10.

DLU 16 includes a tool 17 having a cartridge assembly 18 housing a plurality of surgical staples (not shown) and an anvil assembly 20 movably secured in relation to cartridge assembly 18. As shown herein, DLU 16 is configured to apply six (6) linear rows of staples, in DLU’s measuring from about 30 mm to about 60 mm in length. DLUs for applying any number of rows of staples, having staple pockets arranged in various patterns and/or DLUs and end effectors having any other lengths, e.g., 45 mm, are also envisioned. Handle assembly 12 includes a stationary handle member 22, a movable handle member 24, and a barrel portion 26.

A rotatable member 28 preferably is mounted on the forward end of barrel portion 26 to facilitate rotation of elongated body 14 and attached DLU 16 with respect to handle assembly 12. An articulation lever 30 preferably is also mounted on the forward end of barrel portion 26 adjacent rotatable member 28 to facilitate articulation of tool assembly 17. Preferably, a pair of knobs 32 are movably positioned along barrel portion 26. Knobs 32 are advanced distally to approximate or close cartridge and/or anvil assembly 18, 20, and retracted proximally to unapproximate or open cartridge and/or anvil assembly 18, 20.

As seen in FIG. 4, DLU 16 is desirably selectively removably couplable to elongated body 14. DLU 16 includes a housing portion 200 having a proximal end adapted to releasably engage the distal end of elongated body 14. A mounting assembly 202 is pivotally secured at 203 to the distal end of housing portion 200, and is configured to receive the proximal end of tool assembly 17 such that pivotal movement of mounting assembly 202 about an axis at 203 perpendicular to the longitudinal axis of housing portion 200 effects articulation of tool assembly 17.

FIGS. 5–8 show various perspective views of DLU 16. Surgical stapling apparatus 10 is capable of receiving a non-articulating DLU 16a, as seen in FIG. 5, or an articulating DLU 16, as seen in FIGS. 6–8. U.S. Pat. No. 6,241,139 includes a detailed discussion of articulating and non-articulating DLU.

With general reference to FIGS. 9, 10, 13 and 23–26 and particular reference to FIGS. 9, 10 and 13, DLU 16 includes a mounting assembly 235. Mounting assembly 235 includes an upper and a lower mounting portion 236, 238, respectively. A centrally located pivot member 284 extends from each of upper and lower mounting portions 236, 238 through respective openings 246a formed in coupling members 246. Coupling members 246 each include an interlocking proximal portion 246b configured to be received in grooves 290 formed in the proximal end of upper and lower housing halves 250, 252 to retain mounting assembly 235 and upper

and lower housing halves **250**, **252** in a longitudinally fixed position in relation to each other.

Upper housing half **250** and lower housing half **252** are contained within an outer sleeve, shell or casing **251**. The proximal end of upper housing half **250** includes engagement nubs **254** for releasably engaging the distal end of body **14**. Nubs **254** form a bayonet-type coupling with the distal end of body **14**. Housing halves **252** and **254** define a channel **400** for slidably receiving axial drive assembly **212** therein. An articulation link **256** is dimensioned to be slidably positioned within a slot **402** formed in upper and lower housing halves **250**, **252**. A pair of blow out plate assemblies **255** are positioned adjacent the distal end of housing portion **200** adjacent the distal end of axial drive assembly **212** to prevent outward buckling and bulging of drive assembly **212** during articulation and firing of surgical stapling apparatus **10**. For a detailed discussion of the structure and operation of blow out plate assemblies **255**, reference is made to International Application Serial No. PCT/US02/32031, filed on Oct. 4, 2002, entitled "Surgical Stapling Device", the entire content of which is herein incorporated by reference.

Referring to FIG. 9, optionally, a locking member **288** may be supported on engagement section **270** of axial drive assembly **212**. In operation, when axial drive assembly **212** is actuated, by applying a predetermined force to movable handle member **24** to advance axial drive assembly **212** distally, locking member **288** provides an audible and tactile indication that surgical stapling apparatus **10** has been actuated. For a detailed discussion of the structure and operation of locking member **288**, reference is made to the aforementioned International Application Serial No. PCT/US02/32031. Locking member **288** may also prevent inadvertent partial actuation of DLU **16**, such as during shipping, by locking axial drive assembly **212** at a fixed position within DLU **16** until a predetermined axial force has been applied to axial drive assembly **212**.

With reference to FIGS. 9–12, axial drive assembly **212** includes an elongated drive beam **266** (FIG. 11) including a distal working head **268** (FIG. 12) and a proximal engagement section **270**. Drive beam **266** may be constructed from a single sheet of material or, preferably, multiple stacked sheets, as shown in FIG. 11. Engagement section **270** includes a pair of resilient engagement fingers **270a** and **270b** which are dimensioned and configured to mountingly engage a pair of corresponding retention slots **272a** and **272b** formed in drive member **272** (FIG. 12). Drive member **272** includes a proximal porthole **274** configured to receive distal end **276** of a drive member, e.g., drive rod or control rod **52** (FIGS. 14 and 16–18) when the proximal end of DLU **16** is being engaged with elongated body **14** of surgical stapling apparatus **10**. Control rod **52** functions to impart axial movement of drive assembly **212** from handle assembly **12**.

With reference to FIGS. 9 and 15–32, DLU **16** further includes a locking member **300** rotatably supported on insertion tip **193** and/or on upper and lower housing halves **250**, **252**. Locking member **300** is preferably movable or manipulatable from a first position (FIGS. 23 and 24), in which locking member **300** maintains drive assembly **212** in a ready-to-load position, to a second position (FIGS. 25 and 26), in which drive assembly **212** is free to move axially. DLU **16** is considered to be loaded to elongate body **14** when locking member **300** is in the second position, i.e., when drive assembly **212** is connected to control rod **52** of elongate body **14**.

As additionally seen in FIGS. 15–22, locking member **300** includes a substantially cylindrical, preferably sleeve or cuff-like, body portion **302** including a distal end **304**, a proximal end **306** and defining a passage **308** therethrough. Locking member **300** further includes a projection or tooth **310** extending radially inward from body portion **302** near distal end **304**. In use, as best seen in FIG. 24 and as will be discussed in greater detail below, when locking member **300** is in a first position (i.e., in a "ready-to-load", locked or coupled position), tooth **310** engages a notch or recess **270c** (FIG. 9) formed in the edge of engagement section **270** of drive assembly **212** to thereby effectively axially lock and maintain drive assembly **212** in the ready-to-load position (e.g., wherein drive assembly **212** is in a retracted or proximal-most position relative to upper housing half **250**). Preferably, the locking mechanism of the present invention includes notch or recess **270c**.

Accordingly, when DLU **16** is being coupled to the distal end of elongate body **14**, locking member **300** ensures that engagement section **270** of drive assembly **212** is in a position to, and properly engages, couples with or connects to distal end **276** (FIG. 14) of control rod **52**. Distal end **276** of control rod **52** has one or more engagement surfaces, preferably, and here shown as, including a head **276a** and a smaller diameter annular recess **276b** just proximal of head **276a** and partially defined by head **276a**. Thereafter, less preferably concomitantly therewith, locking member **300** is manipulated (here rotated) to a second position wherein drive assembly **212** is in an unlocked, operative position in which tooth **310** is released and/or otherwise disengaged from notch **270c** of engagement section **270** of drive assembly **212** such that drive assembly **212** is free to move relative to housing portion **200** or upper and lower housing portions **250**, **252** of DLU **16**. As previously stated, when locking member **300** is in the second position, DLU **16** is considered loaded onto elongate body **14** of surgical stapling apparatus **10**. Thus, drive assembly **212** is free to be actuated and reciprocated axially by drive rod **52** to perform its operative functions of approximating and closing anvil and cartridge assemblies **18**, **20**, driving knife **280** and firing staples, as well as of un-approximating, un-clamping, and retracting drive assembly **212**.

With continued reference to FIGS. 15–22, locking member **300** further includes at least one finger **312** that extends longitudinally from proximal end **306**. Preferably, locking member **300** includes a pair of fingers **312**, at least one of which preferably each of which is axially aligned with tooth **310**. At least one of, preferably both, fingers **312** include a protrusion, nub or detent **314** extending radially inward from an inner surface **312a** of finger(s) **312**. In use, as best seen in FIGS. 24–26 and as will be discussed in greater detail below, protrusion(s) **314** is/are selectively engageable with one or more recesses or dimples **193a** formed in the outer surface of insertion tip **193**. Preferably, when locking member **300** is in the first position, fingers **312** and dimples **193a** are in axial alignment with nubs **254** extending radially outward from insertion tip **193**. Protrusions **314** and dimples **193a** are optionally part of the locking mechanism and create a snap-fit type friction engagement wherein protrusion **314** and dimples **193a** cooperate with one another to prevent and/or otherwise inhibit locking member **300** from inadvertently or prematurely rotating from the first position where tooth **310** engages and axially locks drive assembly into position, to the second position in which tooth **310** is disengaged from drive assembly **212**.

In addition, insertion tip **193** includes a cutout or annular slot **193b** (FIG. 9) formed at least partially about the

circumference of tip 193 to enable tooth 310 to pass there-through and to lockingly engage with notch 270c of engagement section 270. Preferably, slot 193b has sufficient length and depth to allow for tooth 310 to extend below the inside surface of insertion tip 193 and to move within slot 193b as locking member 300 is moved, i.e., rotated, from its first position to its second position to disengage tooth 310 from notch 270c of engagement section 270.

As seen in FIG. 19, body portion 302 of locking member 300 extends annularly about 270° and thereby defines an opening 309 of about 90°. Opening 309 is preferably disposed between fingers 312. Preferably, one of fingers 312 is positioned at an angle of about 70° relative to the center line of opening 309 (FIGS. 19, 20 and 22). Preferably, fingers 312 are diametrically opposed to each other. Proximal end 306 of body portion 302 includes a stress reliever 315 formed therein. Preferably, stress reliever 315 is positioned at a location opposite opening 309. Stress reliever 315 enables body portion 302 to open up or radially expand in order for lock member 300 to be snapped onto or otherwise operatively coupled to insertion tip 193. Distal end 304 of body portion 302 defines a clearance notch 317 extending from opening 309 and substantially opposite tooth 310.

Locking member 300 further includes an aperture and/or window 311 formed in body portion 302 thereof. Aperture 311 is axially aligned with tooth 310 and finger 312. Aperture 311 is provided to facilitate the molding and/or fabrication of locking member 300 to facilitate the removal of locking member 300 from a corresponding fabrication mold and/or tool. Locking member 300 further includes a locating surface, here shoulder 319, formed along the inner circumference of body portion 302 at a position distal of proximal end 306.

Turning now to FIGS. 27–32, a method of use and/or operation of locking member 300, and/or for connecting drive assembly 212 of DLU 16 to control rod 52 of elongate body 14 and for securing DLU 16 to the distal end of elongate body 14, will now be discussed. Prior to attachment, i.e., loading, of DLU 16 to elongate body 14 of stapling apparatus 10 (FIG. 27), locking member 300 is in the first position such that tooth 310 is in engagement with notch 270c of engagement section 270 of drive assembly 212 (FIGS. 23, 24 and 28). As discussed above, engagement of tooth 310 with notch 270c retains drive assembly 212 of DLU 16 in its proximal-most, locked, ready-to-load, position. To secure, attach or load DLU 16 to elongate body 14 of stapling apparatus 10, as seen in FIGS. 27 and 28, insertion tip 193 of DLU 16 is introduced longitudinally into the distal end of elongate body 14, in the direction of arrow “A”, such that nubs 254 are received in channels 276d of elongate body 14 (see also FIGS. 14 and 14a). Channels 276d are defined by projections 276c extending radially inward from elongate body 14 near the distal end thereof (FIGS. 14 and 14a). During the introduction of insertion tip 193 of DLU 16, distal end 276 (FIG. 14) of control rod 52 enters porthole 274 (FIG. 12) provided at the proximal end of drive assembly 212. When insertion tip 193 has been fully inserted (FIGS. 29 and 30) into the distal end of elongate body 14, and more particularly, when nubs 254 have completely passed projections 276c, DLU 16 is rotated, in the direction of arrow “B” (FIGS. 31 and 32), such that projections 276c of elongate body 14 abut against and engage fingers 312 of locking member 300, preferably against a side surface 312b of fingers 312.

Continued rotation of DLU 16, in the direction of arrow “B”, causes projections 276c of elongate body 14 to move fingers 312 and locking member 300 from the first position

to the second position to thereby disengage tooth 310 from notch 270c of engagement section 270 of drive assembly 212, thereby freeing drive assembly 212 to operate in surgical stapling apparatus 10. Movement of locking member 300 from the first position to the second position attaches, secures or loads DLU 16 to or onto elongate shaft 14. With control rod 52 connected at its distal end to drive assembly 212, distal movement of control rod 52 effects distal movement of drive assembly 212 thereby moving cam rollers 286 into engagement with a cam surface (not shown) disposed within anvil assembly 20 to move/urge anvil assembly 20 toward cartridge assembly 18, to fire cartridge assembly 18, and to drive knife blade 280 (FIG. 11) through the tissue.

As can be appreciated, if locking member 300 has been inadvertently moved to the second position, prior to attempting to load DLU 16 to elongate body 14, and drive assembly 212 has prematurely moved distally from its proximal-most or ready-to-load position, locking member 300 can not return to the first position due to tooth 310 not being aligned with notch 270c and abutting against a portion of engagement section 270. In such a situation, if locking member 300 is prevented from returning to the first position, upon attempting to load DLU 16 to elongate body 14, fingers 312 of locking member 300 will abut against and/or otherwise contact projection 276c of elongate body 14 and thus prevent loading of DLU 16 to elongate body 14. Accordingly, the loading of a DLU having a drive assembly, e.g., 212, which is not in its ready-to-load position is prevented.

It will be understood that various modifications may be made to the embodiments disclosed herein. Therefore, the above description should not be construed as limiting, but merely as exemplifications of preferred embodiments. Those skilled in the art will envision other modifications within the scope and spirit of the claims appended hereto.

What is claimed is:

1. A surgical stapling apparatus comprising:

a housing;

a handle supported by the housing; and

a loading unit supportable on a distal end of the housing, the loading unit including:

a housing portion including a distal end and a proximal end;

a drive assembly slidably supported within the housing portion of the loading unit; and

a locking member supported on the housing portion of the loading unit and being independently rotatable relative to the housing of the surgical stapling apparatus while the loading unit is being coupled to said housing of said surgical stapling apparatus, the locking member including a locking portion extending through the housing portion, the locking member being rotatably movable from a first position wherein the locking portion engages the drive assembly and maintains the drive assembly in a ready-to-load position to a second position wherein the locking portion permits movement of the drive assembly relative to the housing portion.

2. The surgical stapling apparatus of claim 1, wherein the drive assembly includes a notch and the locking member includes:

a cuff-like body portion that at least partially surrounds the proximal end of the housing portion; and

a tooth extending radially inward from the body portion, wherein the tooth selectively engages the notch formed in the drive assembly such that when the locking member is in the first position the tooth engages the

11

notch of the drive assembly and maintains the drive assembly in the ready-to-load position, and when the locking member is in the second position the tooth is disengaged from the notch of the drive assembly.

3. The surgical stapling apparatus of claim 2, wherein the proximal end of the housing portion includes an annular slot formed therein for receiving the tooth of the locking member therein.

4. The surgical stapling apparatus of claim 3, wherein the locking member further includes at least one finger extending axially from a proximal end thereof, wherein when the locking member is in the first position, the finger is axially aligned with a nub extending radially outward from the proximal end of the housing portion and when the locking member is in the second position the finger is out of axial alignment with the nub of the proximal end of the housing portion.

5. The surgical stapling apparatus of claim 4, wherein the housing includes a radially inwardly extending projection and the locking member is urged from the first position to the second position by the projection, the projection acting on a side surface of the finger as the loading unit is twisted into engagement in and with the housing.

6. The surgical stapling apparatus of claim 5, wherein each finger of the locking member includes a detent projecting from an inner surface thereof for selective engagement with a complementary recess formed in an outer surface of the proximal end of the housing portion.

7. The surgical stapling apparatus of claim 6, wherein the finger of the locking member is axially aligned with the tooth.

8. The surgical stapling apparatus of claim 7, wherein the locking member includes a pair of opposed fingers extending axially from a proximal end thereof, wherein when the locking member is in the first position, one of the pair of fingers is axially aligned with the nub extending radially outward from the proximal end of the housing portion and when the locking member is in the second position the finger is out of axial alignment with the nub of the proximal end of the housing portion.

9. The surgical stapling apparatus according to claim 8, wherein the surgical stapling apparatus is a laparoscopic or endoscopic stapler.

10. The surgical stapling apparatus according to claim 9, further comprising an elongate body extending from the housing.

11. The surgical stapling apparatus according to claim 10, wherein the proximal end of the housing portion defines an insertion tip.

12. A loading unit selectively supportable on a distal end of an elongate body of a surgical stapling apparatus, the loading unit comprising:

a housing portion including a distal end and a proximal end;

a drive assembly slidably supported within the housing portion; and

a locking member for maintaining a drive assembly in a ready-to-load position while the loading unit is being coupled to the elongate body of the surgical stapling apparatus, the locking member being independently rotatable relative to the housing portion from a first position to a second position, the locking member comprising:

a cuff-like body portion that at least partially surrounds an insertion tip of the loading unit; and

a tooth extending radially inward from the body portion, wherein the tooth selectively engages a notch

12

formed in the drive assembly such that when the locking member is in the first position the tooth engages the notch of the drive assembly and maintains the drive assembly in the ready-to-load position, and when the locking member is in the second position the tooth is disengaged from the notch of the drive assembly.

13. The loading unit according to claim 12, wherein the proximal end of the housing portion includes an annular slot formed therein for receiving the tooth of the locking member therein.

14. The loading unit according to claim 13, wherein the locking member further includes at least one finger extending axially from a proximal end thereof, wherein when the locking member is in the first position, the finger is axially aligned with a nub extending radially outward from the proximal end of the housing portion and when the locking member is in the second position the finger is out of axial alignment with the nub of the proximal end of the housing portion.

15. The loading unit according to claim 14, wherein the locking member is urged from the first position to the second position by a radially inward extending projection provided in the elongate body of the surgical stapling apparatus, the projection acting on a side surface of the finger as the loading unit is twisted into engagement in and with the elongate body.

16. The loading unit according to claim 15, wherein each finger of the locking member includes a detent projecting from an inner surface thereof for selective engagement with a complementary recess formed in an outer surface of the proximal end of the housing portion.

17. The loading unit according to claim 16, wherein the finger of the locking member is axially aligned with the tooth.

18. The loading unit according to claim 17, wherein the locking member includes a pair of opposed fingers extending axially from a proximal end thereof, wherein when the locking member is in the first position, one of the pair of fingers is axially aligned with the nub extending radially outward from the proximal end of the housing portion and when the locking member is in the second position the finger is out of axial alignment with the nub of the proximal end of the housing portion.

19. The loading unit according to claim 18, wherein the loading unit is selectively connectable to at least one of a laparoscopic and an endoscopic stapler.

20. A loading unit selectively supportable on a distal end of an elongate body of a surgical stapling apparatus, the loading unit comprising:

a housing portion including a distal end and a proximal end;

a drive assembly slidably supported within the housing portion; and

a locking member supported on the housing portion and being independently rotatable relative to the housing of the surgical stapling apparatus while the loading unit is being coupled to said housing, of said surgical stapling apparatus the locking member including a locking portion extending through the housing portion, the locking member being movable from a first position wherein the locking portion engages the drive assembly and maintains the drive assembly in a ready-to-load position to a second position wherein the locking portion permits movement of the drive assembly relative to the housing portion.

专利名称(译)	具有锁定机构的外科缝合器械		
公开(公告)号	US7143924	公开(公告)日	2006-12-05
申请号	US11/059805	申请日	2005-02-17
[标]申请(专利权)人(译)	柯惠有限合伙公司		
申请(专利权)人(译)	泰科医疗集团 , LP		
当前申请(专利权)人(译)	COVIDIEN LP		
[标]发明人	SCIRICA PAUL A MARCZYK STANISLAW		
发明人	SCIRICA, PAUL A. MARCZYK, STANISLAW		
IPC分类号	A61B17/068 A61B17/072 A61B17/10 A61B17/32		
CPC分类号	A61B17/07207 A61B2017/0046 A61B2017/07214 A61B2017/320052		
优先权	60/545619 2004-02-17 US		
其他公开文献	US20050184124A1		
外部链接	Espacenet USPTO		

摘要(译)

本公开提供了一种用于外科缝合器械的装载单元。装载单元包括：壳体部分，具有远端和近端；驱动组件，可滑动地支撑在装载单元的壳体部分内；以及锁定构件，支撑在装载单元的壳体部分上。锁定构件可从第一位置移动，其中锁定构件接合驱动组件并将驱动组件保持在准备装载位置至第二位置，其中锁定构件允许驱动组件相对于壳体部分移动。

