



US007621958B2

(12) **United States Patent**  
**Zdeblick et al.**

(10) **Patent No.:** **US 7,621,958 B2**  
(45) **Date of Patent:** **Nov. 24, 2009**

(54) **METHODS AND INSTRUMENTS FOR  
INTERBODY FUSION**

(75) Inventors: **Thomas Zdeblick**, Middleton, WI (US);  
**Thomas McGahan**, Memphis, TN (US)

(73) Assignee: **Warsaw Orthopedic, Inc.**

(\*) Notice: Subject to any disclaimer, the term of this  
patent is extended or adjusted under 35  
U.S.C. 154(b) by 846 days.

(21) Appl. No.: **10/763,719**

(22) Filed: **Jan. 23, 2004**

(65) **Prior Publication Data**

US 2004/0153089 A1 Aug. 5, 2004

**Related U.S. Application Data**

(60) Division of application No. 10/213,864, filed on Aug.  
7, 2002, now Pat. No. 6,695,851, which is a division of  
application No. 09/781,589, filed on Feb. 5, 2001, now  
Pat. No. 6,471,724, which is a division of application  
No. 09/014,901, filed on Jan. 28, 1998, now Pat. No.  
6,206,922, which is a continuation-in-part of applica-  
tion No. 08/604,874, filed on Feb. 22, 1996, now aban-  
doned, which is a continuation-in-part of application  
No. 08/411,017, filed on Mar. 27, 1995, now Pat. No.  
5,782,919.

(51) **Int. Cl.**  
**A61F 2/44** (2006.01)

(52) **U.S. Cl.** ..... **623/17.16; 623/17.11**

(58) **Field of Classification Search** ... **623/17.11-17.16;**  
**606/60-67, 92-96, 246-254**  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

3,486,505 A \* 12/1969 Morrison ..... 606/90  
3,822,697 A 7/1974 Komiya  
3,848,601 A 11/1974 Ma et al. .... 606/61

4,309,777 A 1/1982 Patil ..... 3/1.91  
4,349,921 A 9/1982 Kuntz ..... 623/17.16  
4,501,269 A 2/1985 Bagby ..... 606/61

(Continued)

**FOREIGN PATENT DOCUMENTS**

CA 2015507 4/1990

(Continued)

**OTHER PUBLICATIONS**



*Laparoscopic Bone Dowel Surgical Technique*, by Sofamor Danek  
USA, 1800 Pyramid Place, Memphis, TN 38132, Lit LBD ST95  
Copyright 1995 Sofamor Danek.

*Primary Examiner*—Alvin J Stewart

(57) **ABSTRACT**

A laparoscopic surgical technique is provided for preparing a  
site for implantation of a novel fusion device or implant. In  
accordance with one embodiment of the technique, a laparo-  
scope is provided having an outer sleeve with distraction  
fingers at one end to distract the disc space. The laparoscope  
provides a sealed working channel to the disc space, through  
which the disc space is distracted, the vertebral endplates and  
surrounding disc is reamed, and the fusion device inserted. A  
distraction plug is provided for centering the outer sleeve and  
for providing midline distraction of the disc space. In one  
embodiment, a fusion device includes diverging bone screws  
passing through an end wall and upper and lower walls of the  
device to engage the adjacent vertebrae. In another embodi-  
ment, a connector plate is engaged to bilaterally position  
fusion devices to prevent rotation and resist expulsion of the  
devices from the disc space.

**22 Claims, 19 Drawing Sheets**

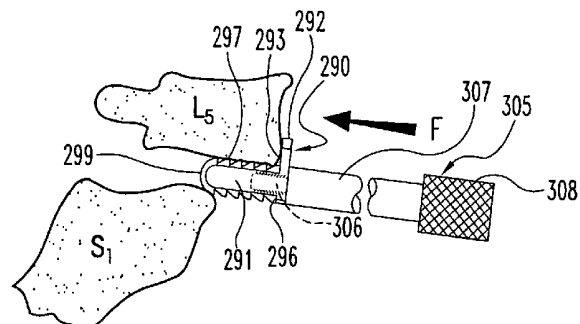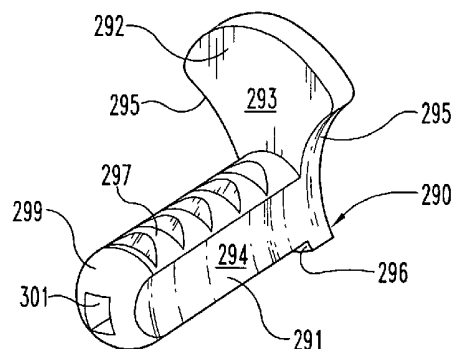

# US 7,621,958 B2

Page 2

## U.S. PATENT DOCUMENTS

4,526,909 A 7/1985 Urist ..... 523/115  
4,545,374 A 10/1985 Jacobson ..... 128/303  
4,573,448 A 3/1986 Kambin ..... 128/1  
4,596,574 A 6/1986 Urist ..... 623/16  
4,599,086 A \* 7/1986 Doty ..... 606/61  
4,678,470 A 7/1987 Nashef et al. .... 623/16  
4,714,469 A 12/1987 Kenna ..... 623/17  
4,736,738 A 4/1988 Lipovsek et al. .... 128/92  
4,743,256 A 5/1988 Brantigan ..... 128/898  
4,743,259 A 5/1988 Bolander et al. .... 623/16  
4,759,766 A 7/1988 Buettner-Janz et al. .... 623/17  
4,772,287 A 9/1988 Ray et al. .... 623/17  
4,820,305 A 4/1989 Harms et al. .... 623/16.11  
4,834,757 A 5/1989 Brantigan ..... 623/17.11  
4,842,545 A \* 6/1989 Tilse ..... 439/393  
4,863,476 A 9/1989 Shepperd ..... 623/17  
4,877,020 A 10/1989 Vich ..... 606/86  
4,878,915 A 11/1989 Brantigan ..... 623/17.11  
4,892,545 A 1/1990 Day et al. .... 623/17  
4,904,261 A 2/1990 Dove et al. .... 623/17.16  
4,917,704 A 4/1990 Frey et al. .... 623/17  
4,932,975 A 6/1990 Main et al. .... 623/17  
4,936,848 A 6/1990 Bagby ..... 623/17.16  
4,961,740 A 10/1990 Ray et al. .... 606/61  
5,002,576 A 3/1991 Fuhrmann et al. .... 623/17  
5,015,247 A 5/1991 Michelson ..... 606/61  
5,020,519 A 6/1991 Hayes et al. .... 128/69  
5,030,474 A 7/1991 Saita et al. .... 427/2  
5,055,104 A 10/1991 Ray ..... 606/61  
5,062,850 A 11/1991 MacMillan et al. .... 623/17  
5,068,122 A 11/1991 Kokubo et al. .... 427/2  
5,071,437 A 12/1991 Steffee ..... 623/17  
5,092,893 A 3/1992 Smith ..... 623/17  
5,108,395 A 4/1992 Laurain ..... 606/61  
5,128,169 A 7/1992 Saita et al. .... 427/2  
RE34,037 E 8/1992 Inoue et al. .... 604/93  
5,147,402 A 9/1992 Bohler et al. .... 623/16  
5,147,404 A 9/1992 Downey ..... 623/17  
5,164,187 A 11/1992 Constantz et al. .... 424/423  
5,188,670 A 2/1993 Constantz ..... 118/667  
5,192,327 A 3/1993 Brantigan ..... 623/17.11  
5,236,456 A 8/1993 O'Leary et al. .... 623/16  
5,236,460 A 8/1993 Berber ..... 623/17  
5,279,831 A 1/1994 Constantz et al. .... 424/423  
5,282,861 A 2/1994 Kaplan ..... 623/23.51  
5,290,312 A 3/1994 Kojimoto et al. .... 623/17.15  
5,306,307 A 4/1994 Senter et al. .... 623/17  
5,306,309 A 4/1994 Wagner et al. .... 623/17  
5,306,310 A 4/1994 Siebels ..... 623/17  
5,330,826 A 7/1994 Taylor et al. .... 428/216  
5,338,433 A 8/1994 Maybee et al. .... 205/178  
5,344,654 A 9/1994 Rueger et al. .... 424/423  
5,348,026 A 9/1994 Davidson ..... 128/898  
5,360,430 A 11/1994 Lin ..... 606/61  
5,397,364 A 3/1995 Kozak et al. .... 623/17  
5,405,391 A 4/1995 Hednerson et al. .... 623/17.15  
5,417,975 A 5/1995 Lussi et al. .... 424/423  
5,423,816 A 6/1995 Lin ..... 606/61  
5,423,817 A 6/1995 Lin ..... 606/61  
5,425,769 A 6/1995 Snyders, Jr. .... 623/16  
5,425,772 A \* 6/1995 Brantigan ..... 623/17.11  
5,431,658 A \* 7/1995 Moskovich ..... 606/99  
5,439,464 A 8/1995 Shapiro ..... 606/83  
5,439,684 A 8/1995 Prewett et al. .... 424/422  
5,443,514 A 8/1995 Steffee ..... 128/898  
5,443,515 A 8/1995 Cohen et al. .... 623/17  
5,455,231 A 10/1995 Constantz et al. .... 514/21  
5,458,638 A 10/1995 Kuslich et al. .... 623/17.11  
5,464,439 A 11/1995 Gendler ..... 623/16  
5,484,437 A 1/1996 Michelson ..... 606/61  
5,489,307 A 2/1996 Kuslich et al. .... 623/17

5,489,308 A 2/1996 Kuslich et al. .... 623/17  
5,507,813 A 4/1996 Dowd et al. .... 623/16  
5,510,396 A 4/1996 Prewett et al. .... 523/113  
5,514,180 A 5/1996 Heggeness et al. .... 623/17  
5,540,688 A 7/1996 Navas ..... 606/61  
5,549,612 A 8/1996 Yapp et al. .... 606/69  
5,562,736 A 10/1996 Ray et al. .... 623/17  
5,571,109 A 11/1996 Bertagnoli  
D377,095 S 12/1996 Michelson ..... D24/155  
D377,096 S 12/1996 Michelson ..... D24/155  
5,585,116 A 12/1996 Boniface et al. .... 424/549  
5,591,235 A 1/1997 Kuslich ..... 606/61  
5,593,409 A 1/1997 Michelson ..... 606/61  
5,601,556 A \* 2/1997 Pisharodi ..... 606/61  
5,609,635 A 3/1997 Michelson ..... 623/17  
5,609,636 A 3/1997 Kohrs et al. .... 623/17.16  
5,645,591 A 7/1997 Kuberasampath et al. .... 623/16  
5,645,598 A 7/1997 Brosnahan, III ..... 623/17  
5,646,084 A 7/1997 Patton et al. .... 502/152  
5,647,872 A 7/1997 Gilbert et al. .... 606/61  
5,658,285 A 8/1997 Marnay et al. .... 606/61  
5,669,909 A 9/1997 Zdeblick et al. .... 606/61  
5,676,666 A 10/1997 Oxland et al. .... 606/61  
5,681,311 A 10/1997 Foley et al. .... 606/61  
5,683,391 A 11/1997 Boyd ..... 606/61  
5,683,394 A 11/1997 Rinner ..... 606/86  
5,683,463 A 11/1997 Godefroy et al. .... 623/17  
5,697,889 A 12/1997 Slotman et al. .... 600/204  
5,697,977 A \* 12/1997 Pisharodi ..... 606/279  
5,741,253 A \* 4/1998 Michelson ..... 606/86 A  
5,766,252 A \* 6/1998 Henry et al. .... 623/17.16  
5,766,253 A 6/1998 Brosnahan, III ..... 623/17  
5,782,831 A \* 7/1998 Sherman et al. .... 606/86 A  
5,797,909 A \* 8/1998 Michelson ..... 606/914  
5,888,224 A \* 3/1999 Beckers et al. .... 623/17.16  
5,904,719 A \* 5/1999 Errico et al. .... 623/17.16  
5,941,880 A \* 8/1999 Errico et al. .... 623/17.11  
6,030,390 A \* 2/2000 Mehdizadeh ..... 606/84  
6,042,582 A \* 3/2000 Ray ..... 606/61  
6,063,088 A \* 5/2000 Winslow ..... 606/86 A  
6,066,175 A \* 5/2000 Henderson et al. .... 623/17.11  
6,149,686 A 11/2000 Kuslich et al. .... 623/17.11  
6,165,219 A \* 12/2000 Kohrs et al. .... 623/17.11  
6,224,631 B1 \* 5/2001 Kohrs ..... 623/17.11  
6,290,724 B1 \* 9/2001 Marino ..... 623/17.11  
6,342,074 B1 1/2002 Simpson ..... 623/17.11  
6,436,139 B1 \* 8/2002 Shapiro et al. .... 623/17.11  
6,471,724 B2 \* 10/2002 Zdeblick et al. .... 623/17.16  
6,491,696 B1 \* 12/2002 Kunkel ..... 606/105  
6,695,851 B2 \* 2/2004 Zdeblick et al. .... 606/96  
6,743,234 B2 \* 6/2004 Burkus et al. .... 606/90  
6,926,737 B2 \* 8/2005 Jackson ..... 623/17.16  
6,942,698 B1 \* 9/2005 Jackson ..... 623/17.16  
7,195,643 B2 \* 3/2007 Jackson ..... 623/17.11  
7,235,105 B2 \* 6/2007 Jackson ..... 623/17.16  
7,244,258 B2 \* 7/2007 Burkus et al. .... 606/90  
7,326,251 B2 \* 2/2008 McCombe et al. .... 623/17.16

## FOREIGN PATENT DOCUMENTS

DE 3505567 A 6/1986  
DE 4302397 A1 1/1992  
EP 0077159 10/1982  
EP 0179695 9/1985  
EP 0307241 3/1989  
EP 0450886 A1 3/1991  
EP 0635246 1/1995  
EP 0646366 5/1995  
EP 0637440 8/1995  
EP 0 676 176 A1 10/1995  
EP 0716840 A2 12/1995  
EP 0796593 A2 3/1997  
FR 2631539 A1 5/1988



# US 7,621,958 B2


Page 3

---


FR	2703580	A1 *	3/1993	..... 623/17.16	WO	WO 95/08306	3/1995
FR	2710519	A1	9/1993		WO	WO 95/15133	6/1995
FR	2727003	A1	11/1994		WO	WO 95/26164	10/1995
FR	2727005	A1	11/1994		WO	WO 96/27321	2/1996
FR	2724312	A1	4/1995		WO	WO 96/22747	8/1996
WO	WO 87/07827		12/1987		WO	WO 96/27345	9/1996
WO	WO 90/00037		1/1990		WO	WO 96/40016	12/1996
WO	WO 91/06261		5/1991		WO	WO 97/20526	6/1997
WO	WO 92/14423		9/1992		WO	WO 97/30666	8/1997
WO	WO 94/11040		5/1994		WO	WO 97/31517	8/1997
WO	WO 94/26893		11/1994				

\* cited by examiner

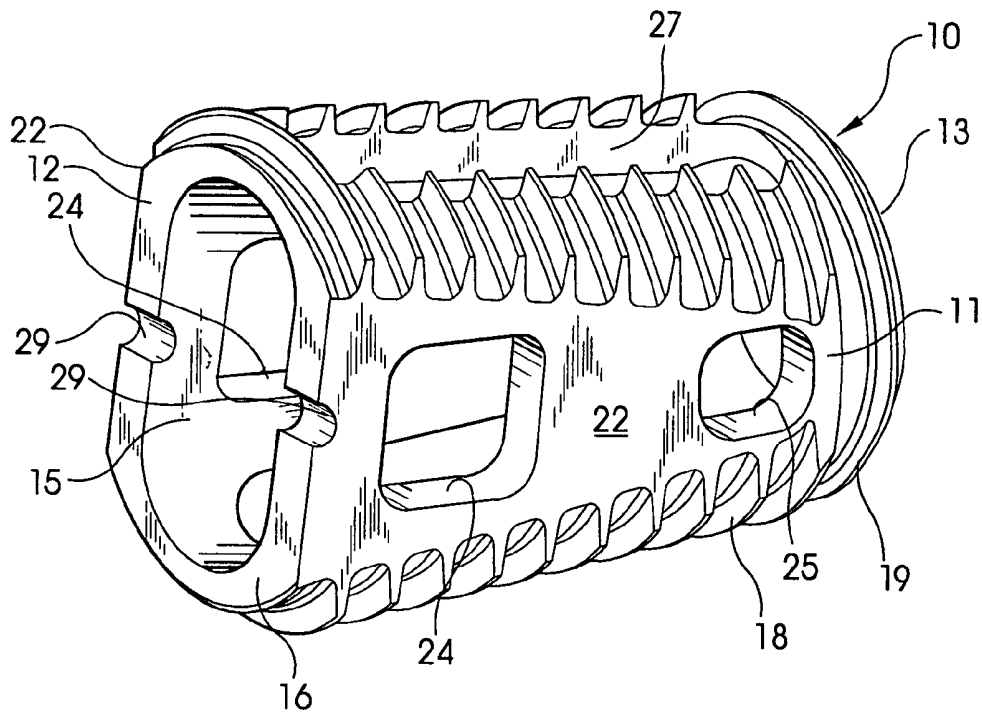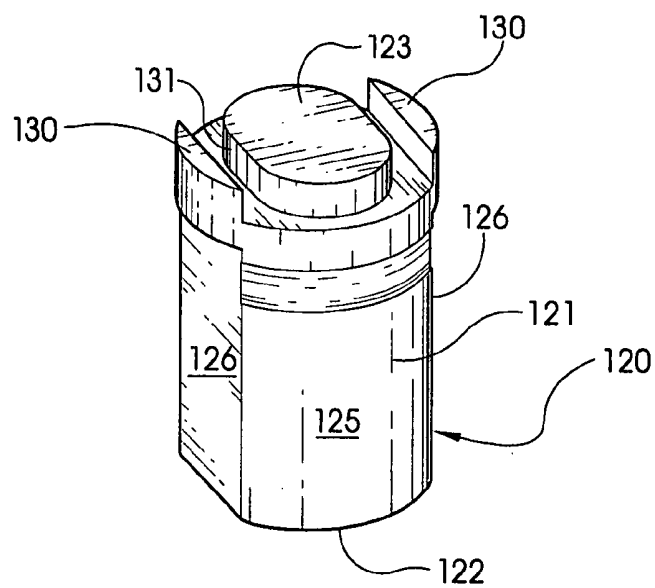
**Fig. 1****Fig 6**

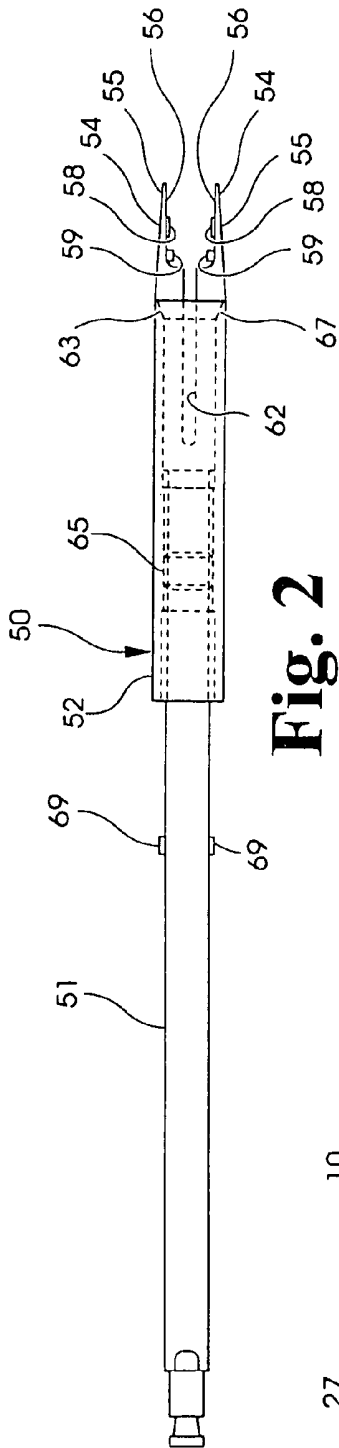

**Fig. 2**

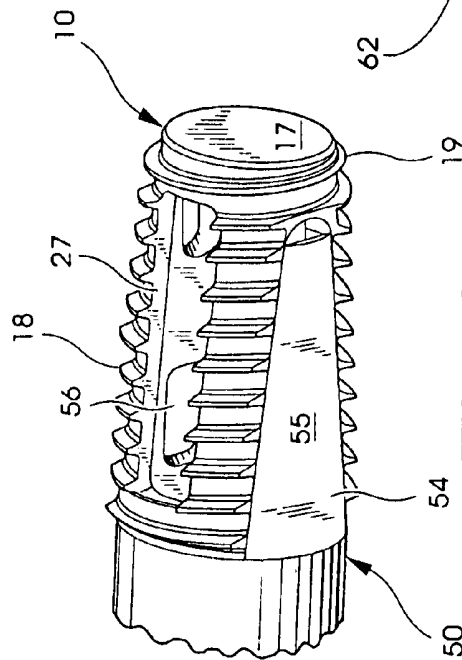

**Fig. 3**

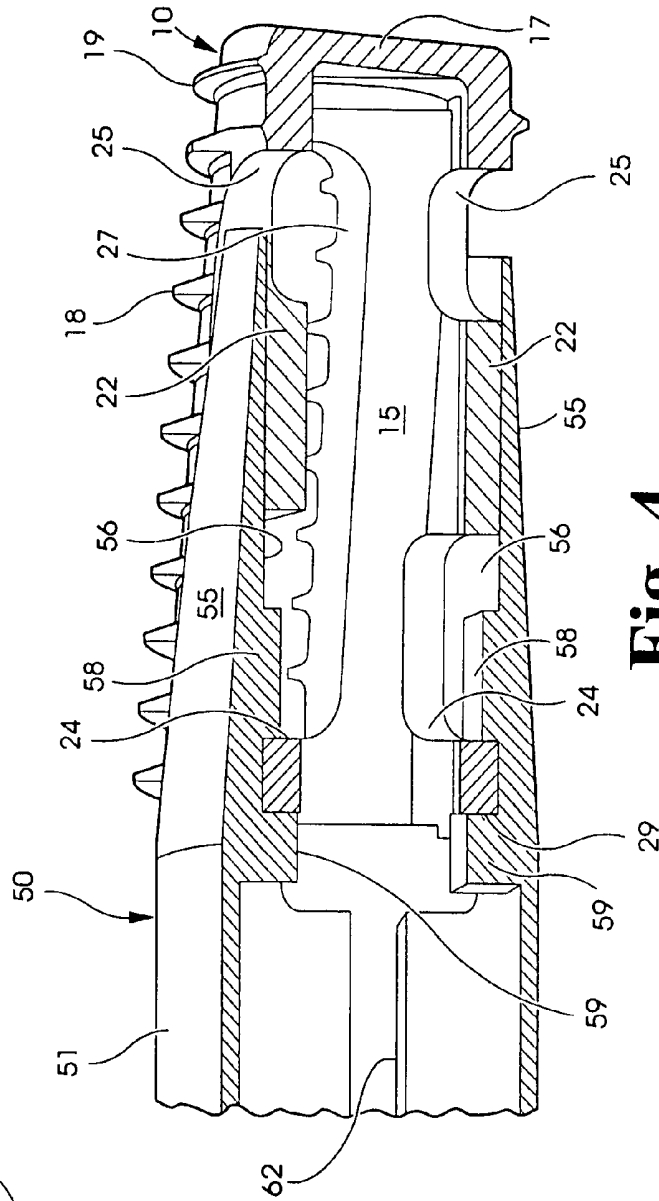

**Fig. 4**

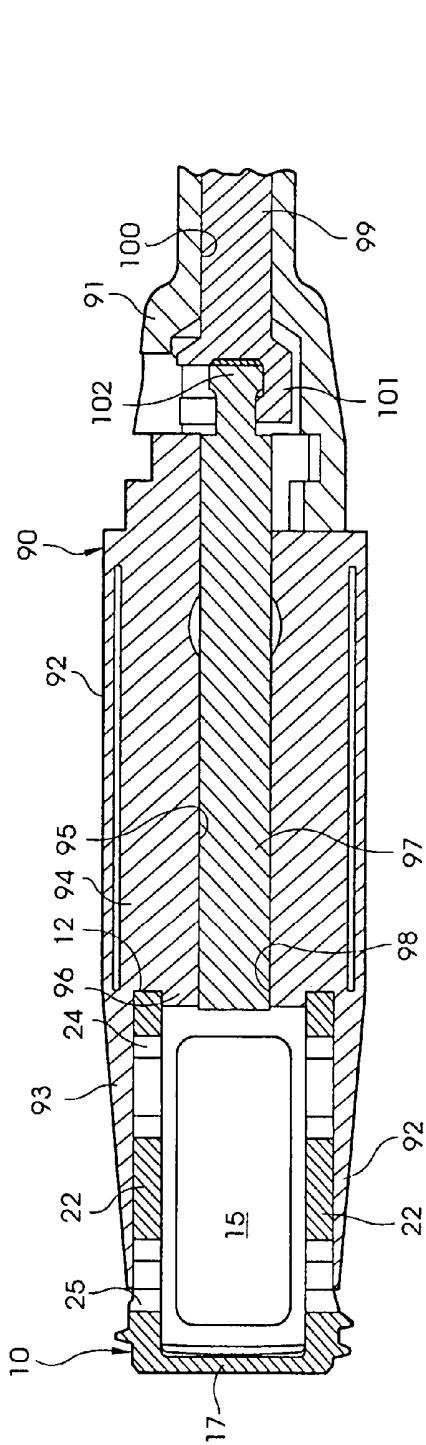


Fig. 5



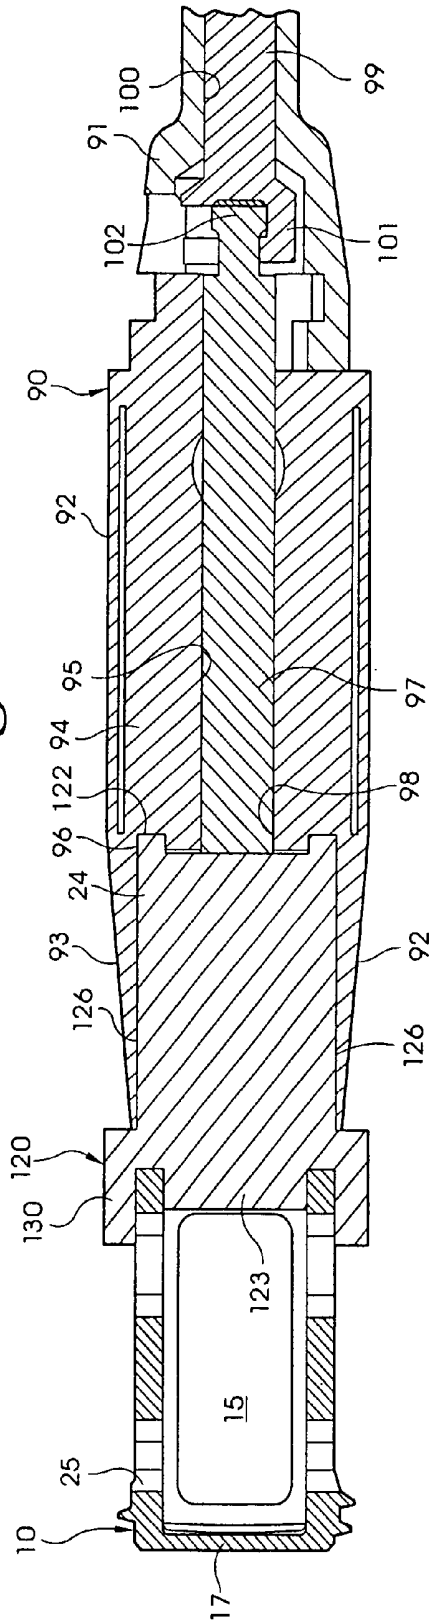



Fig 7

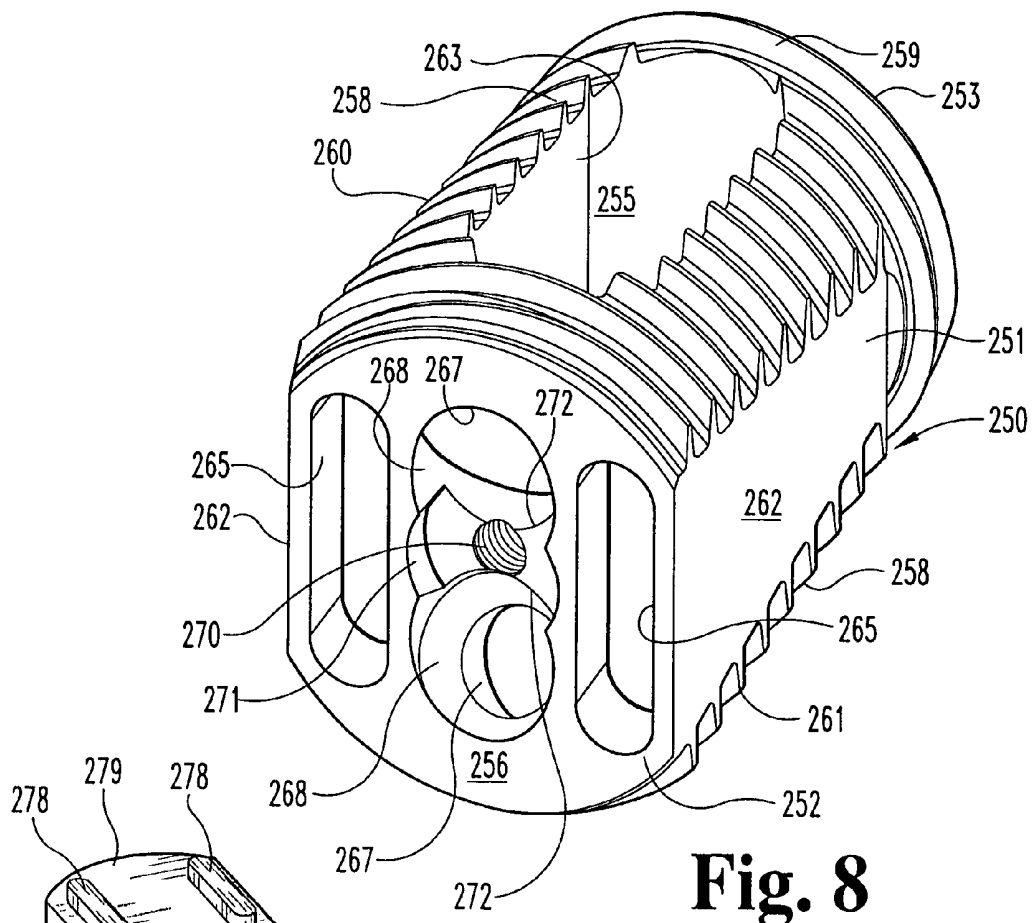

**Fig. 8**

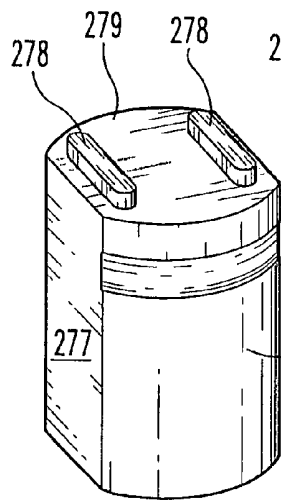


**Fig. 9**

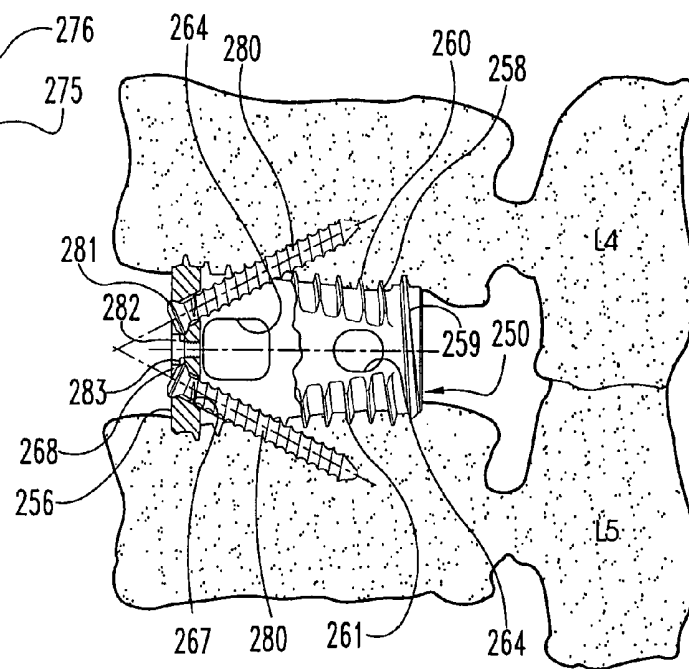


**Fig. 10**

1. Dilate the disc space (slight lordosis):

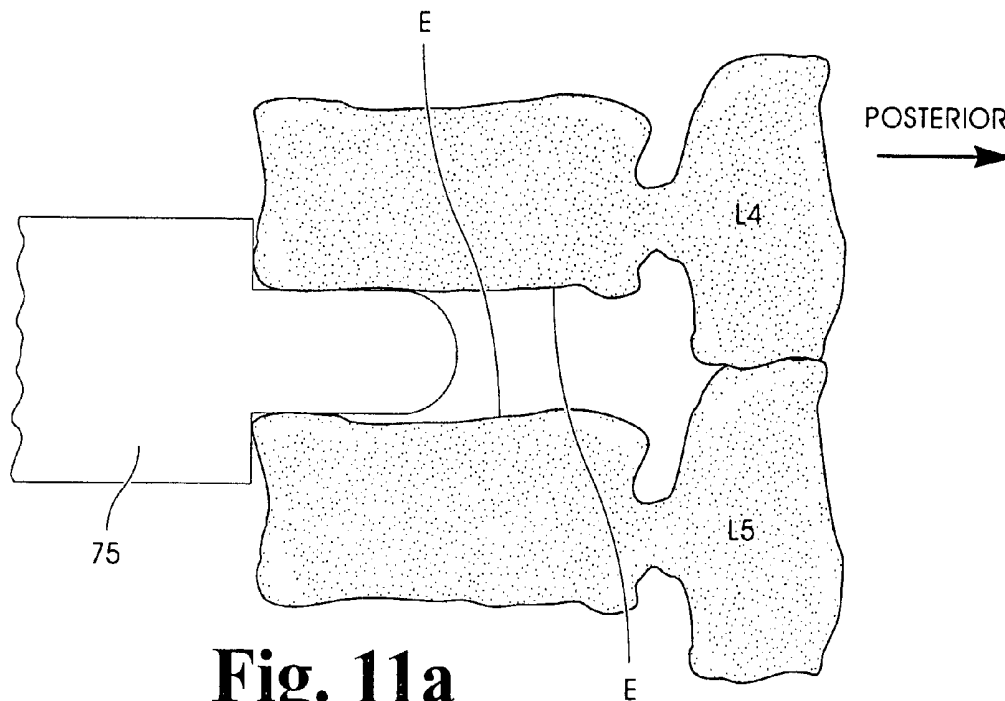

**Fig. 11a**


2. Place outer sleeve & drill minor diameter hole:

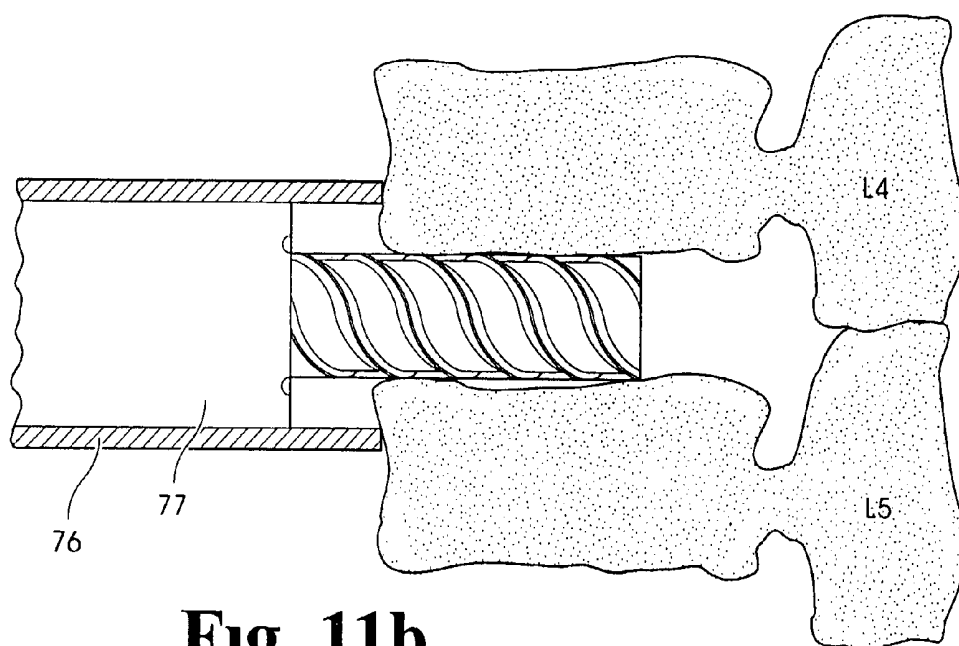

**Fig. 11b**




**3. Insert implant to secure lordosis required**

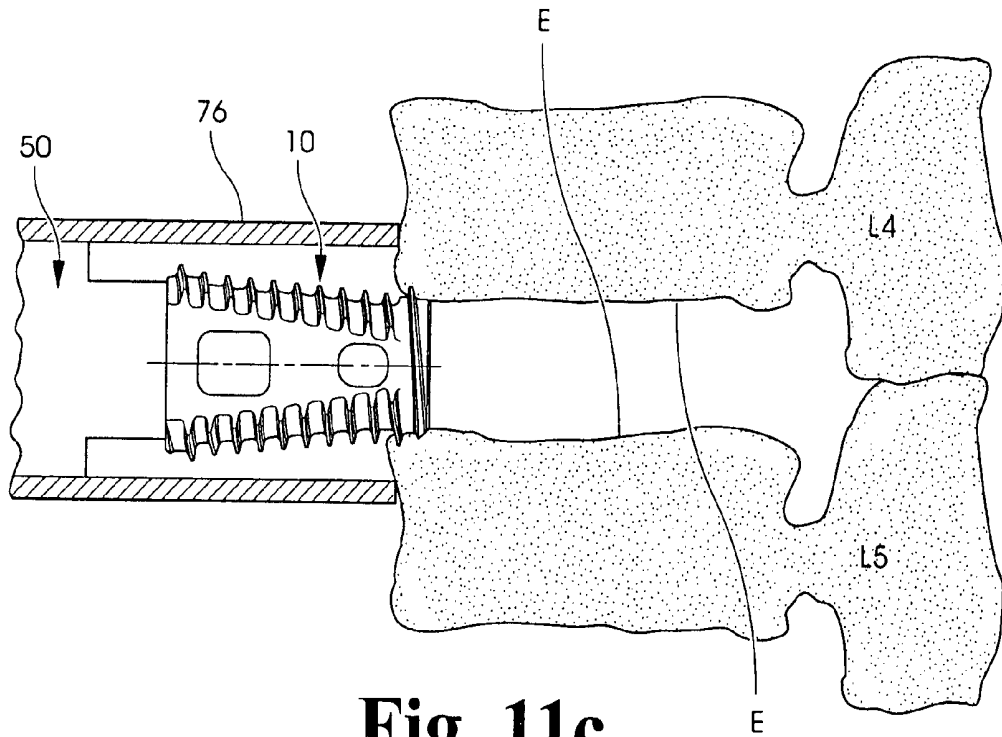


**Fig. 11c**

**4. Remove implant driver**

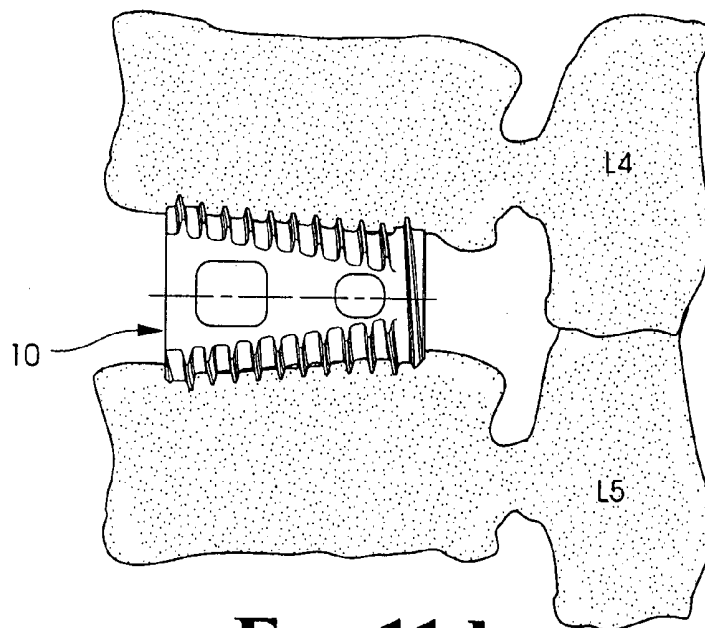


**Fig 11d**

**1. Dilate the disc space:**

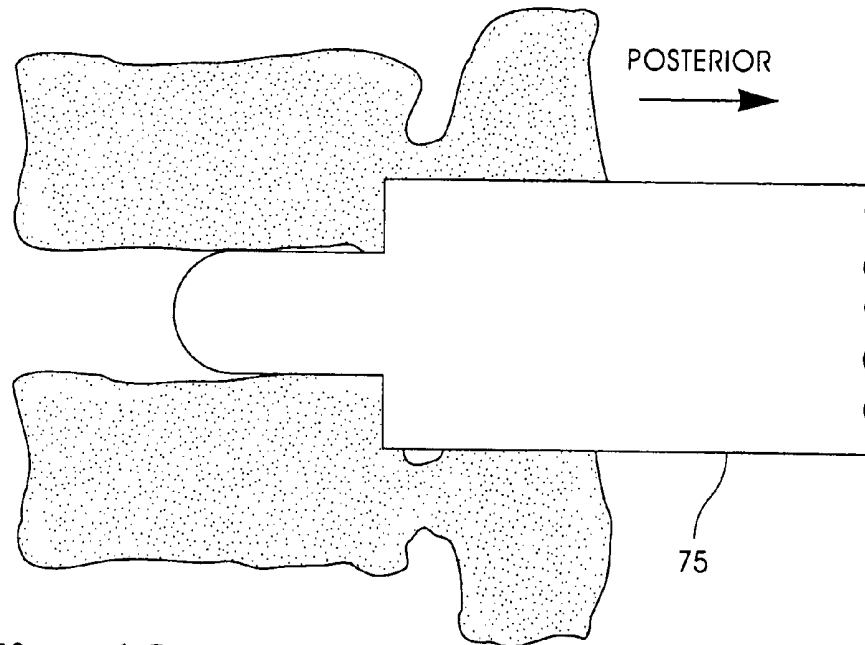




**Fig. 12a**


**2. Place outer sleeve & drill minor diameter hole:**

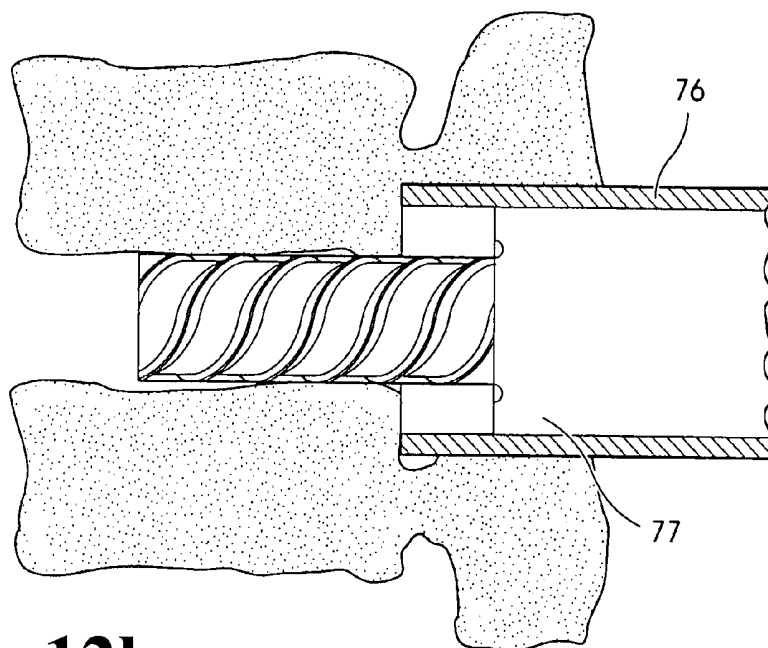


**Fig 12b**

**Fig 12d**

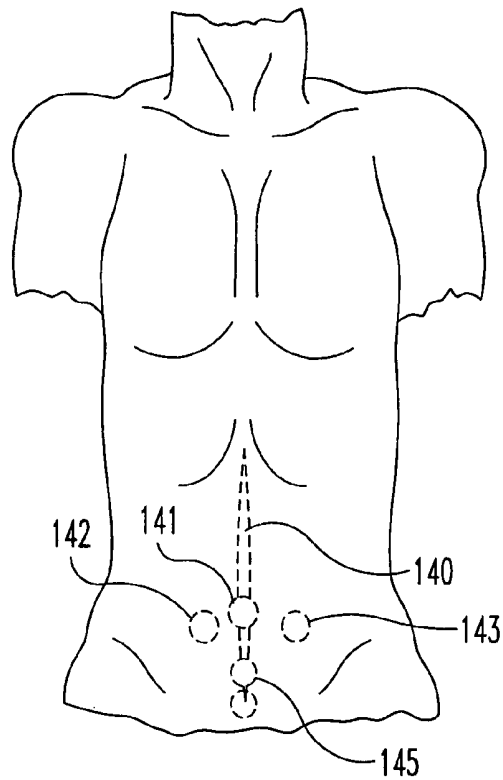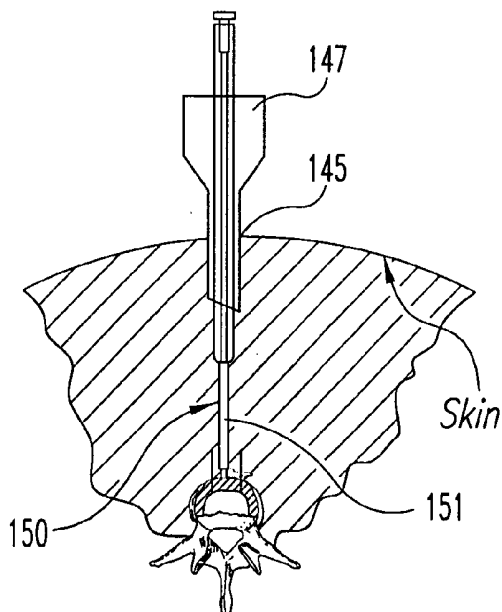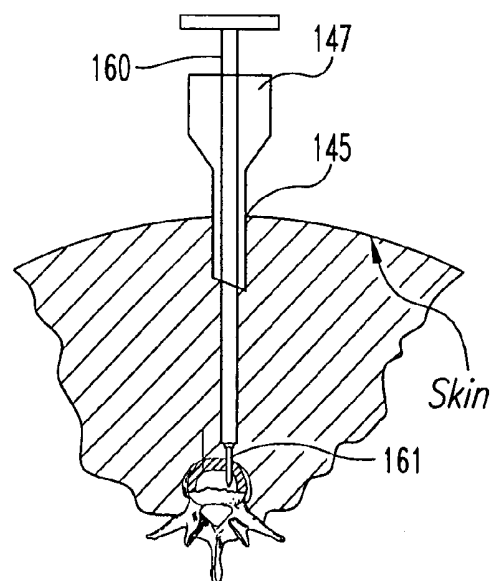
**Fig. 13****Fig. 14****Fig. 16**

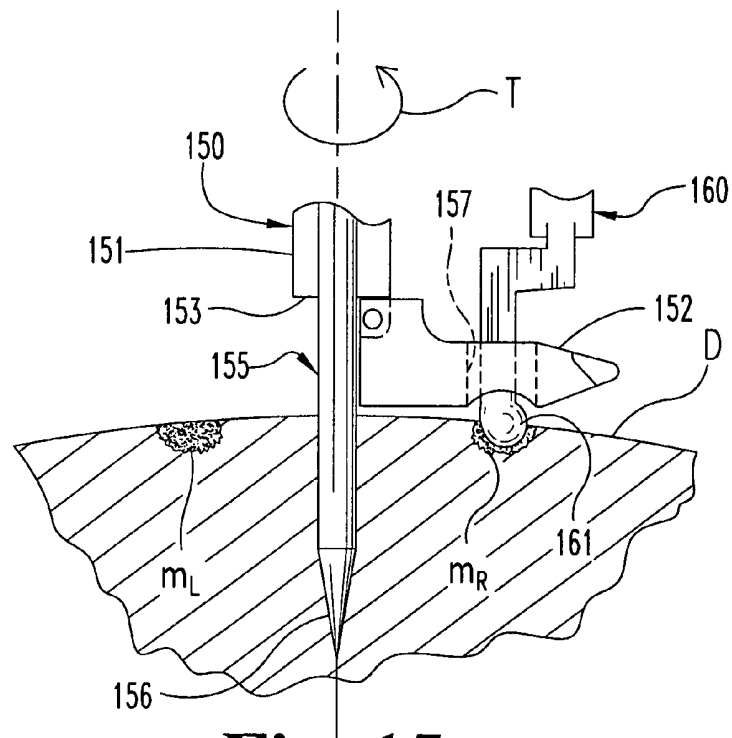


**Fig. 15**

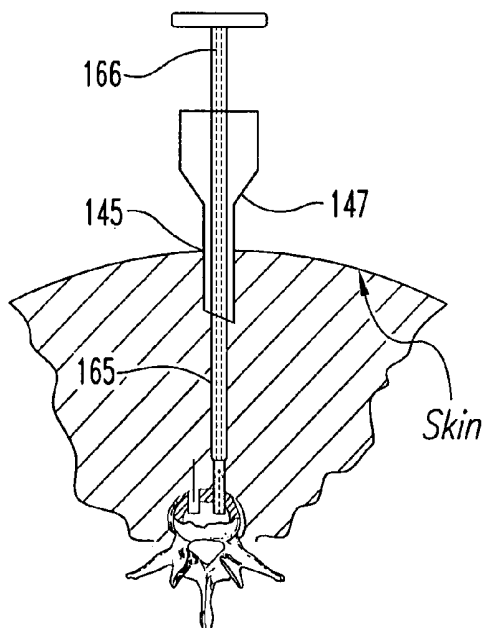


**Fig. 17**

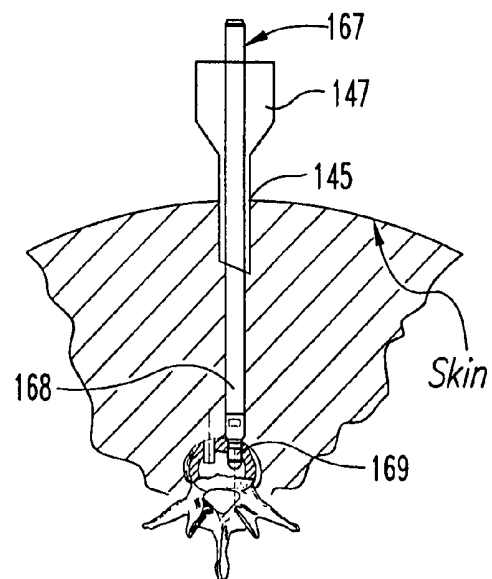


**Fig. 18**

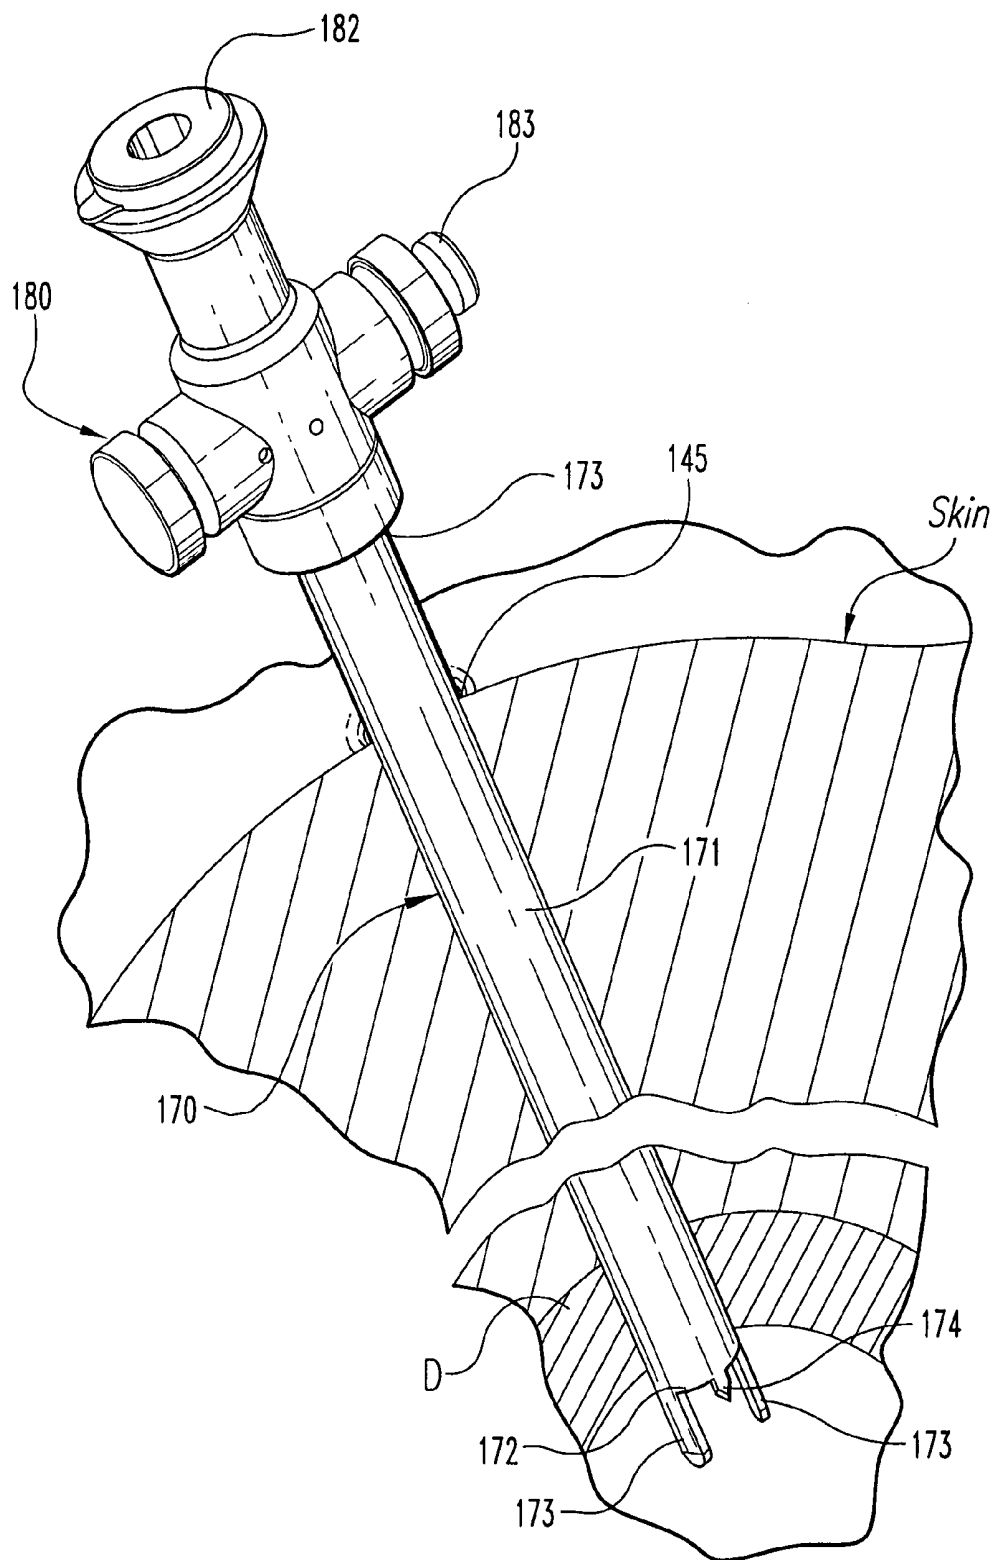**Fig. 19**

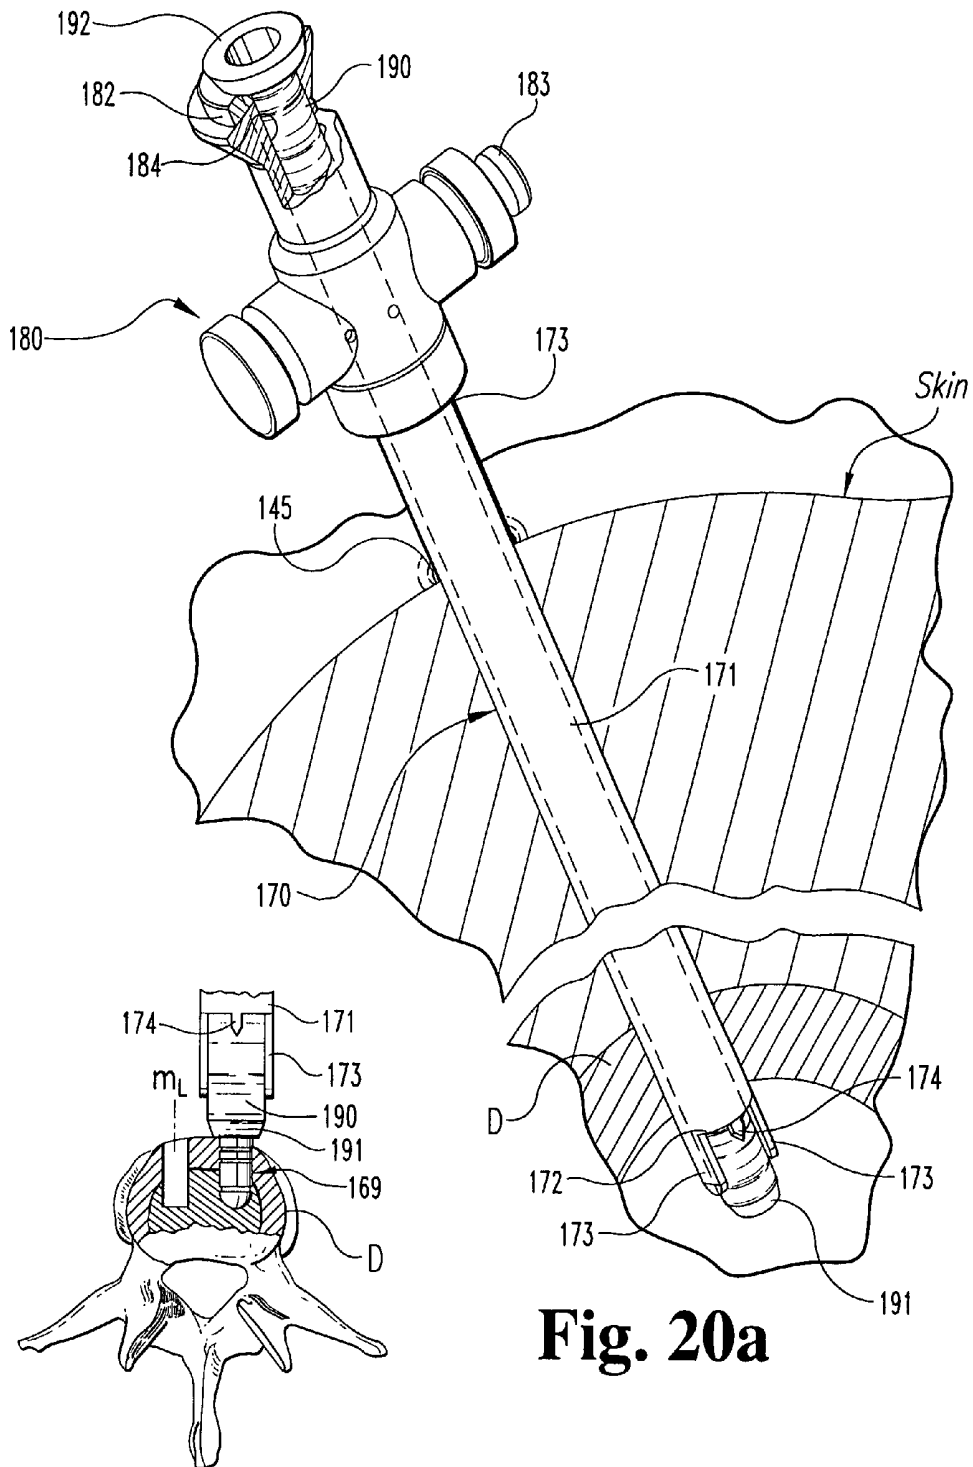


**Fig. 20a**

**Fig 20b**

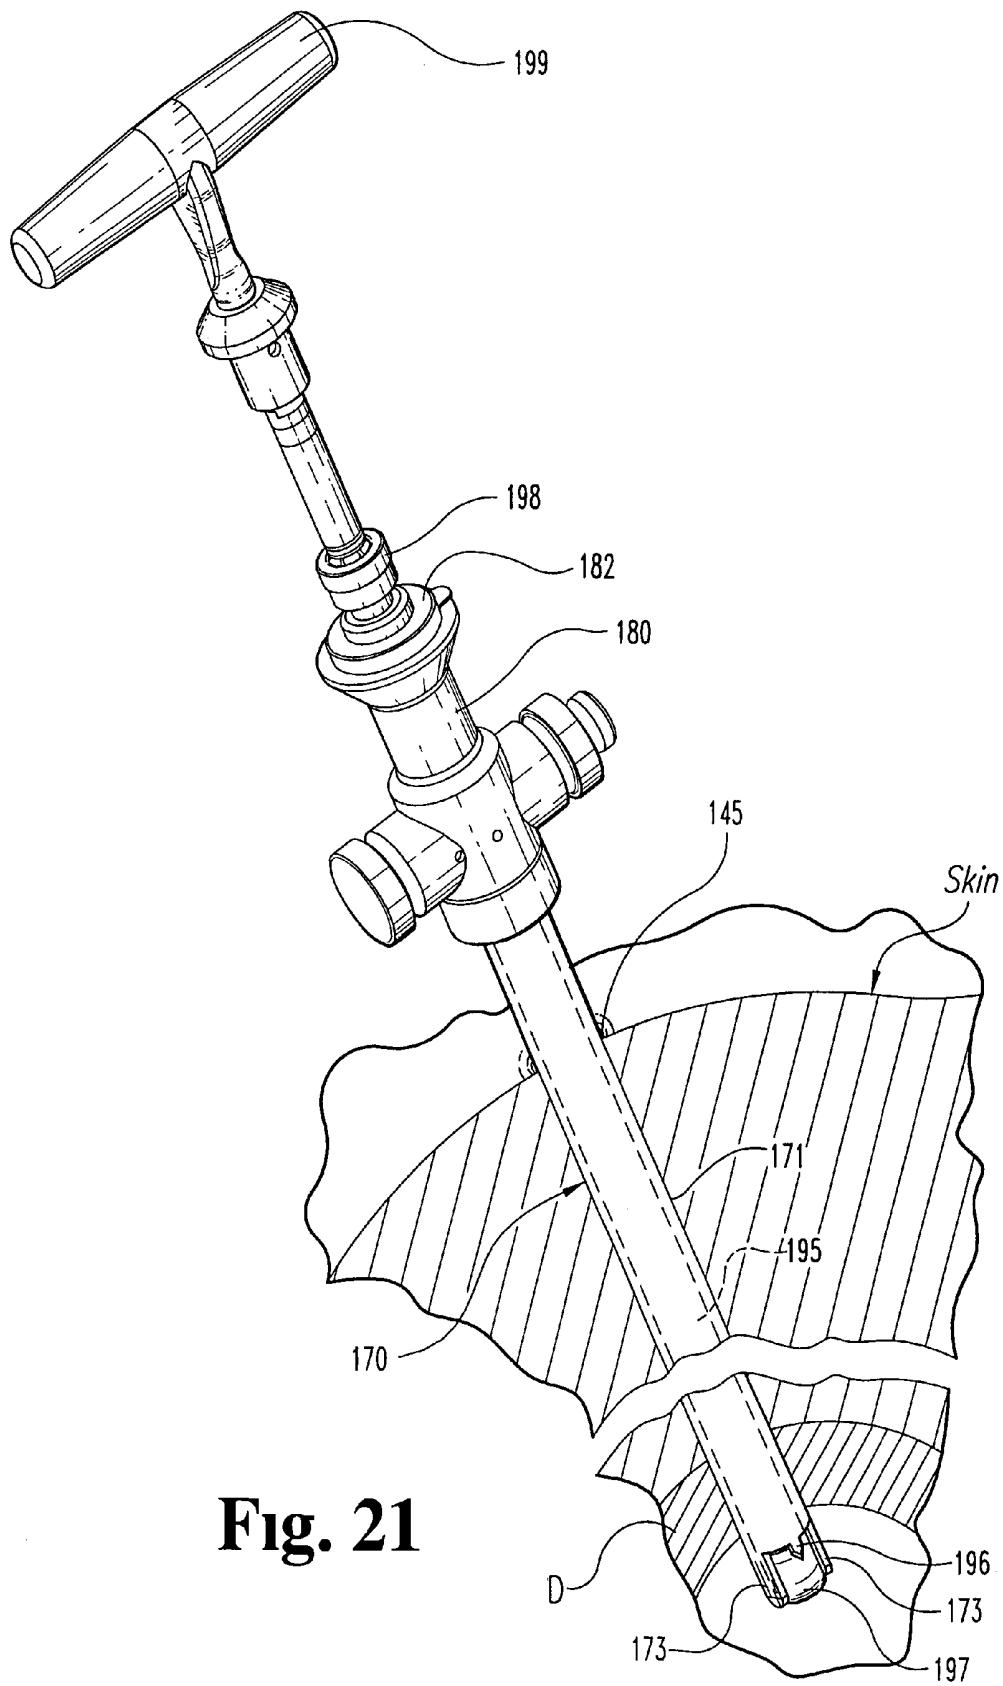


**Fig. 21**




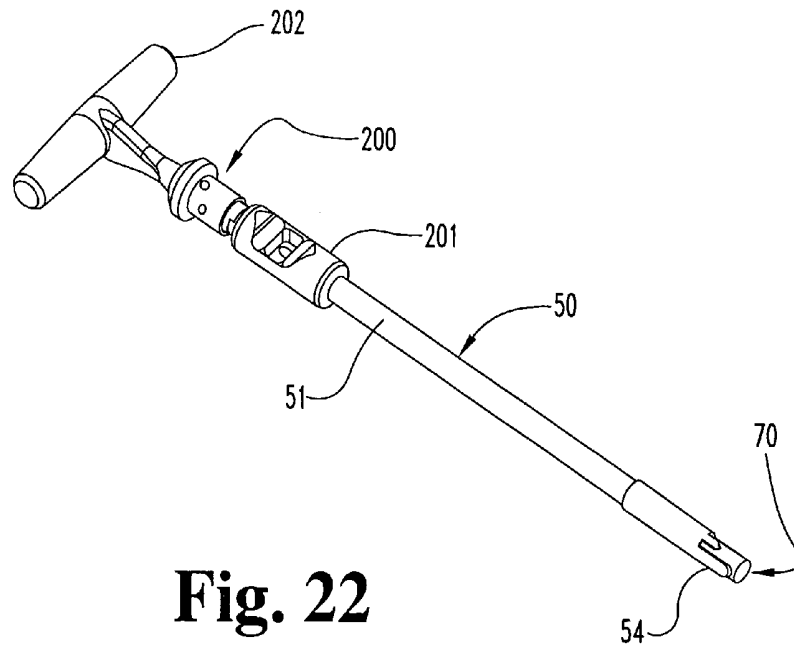


**Fig. 22**

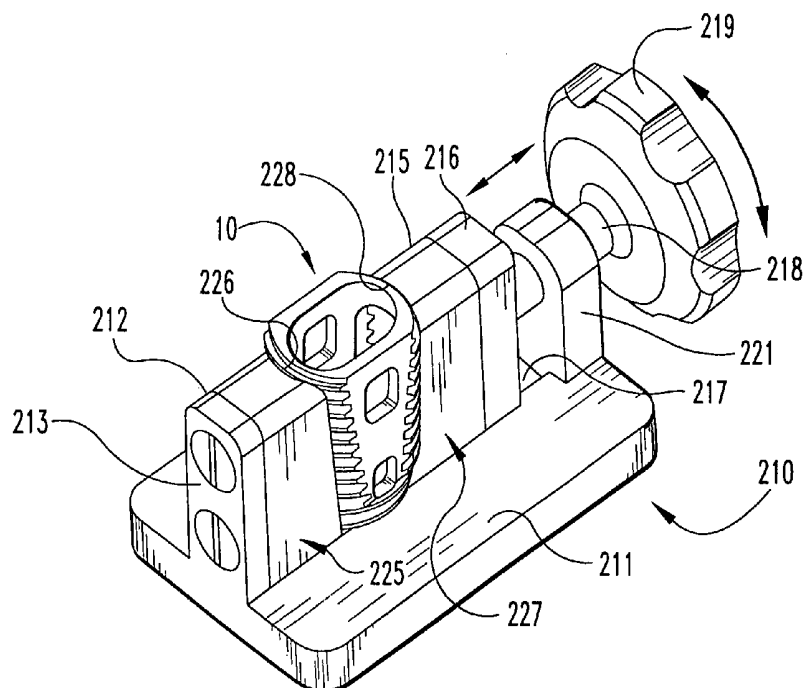


**Fig. 23**

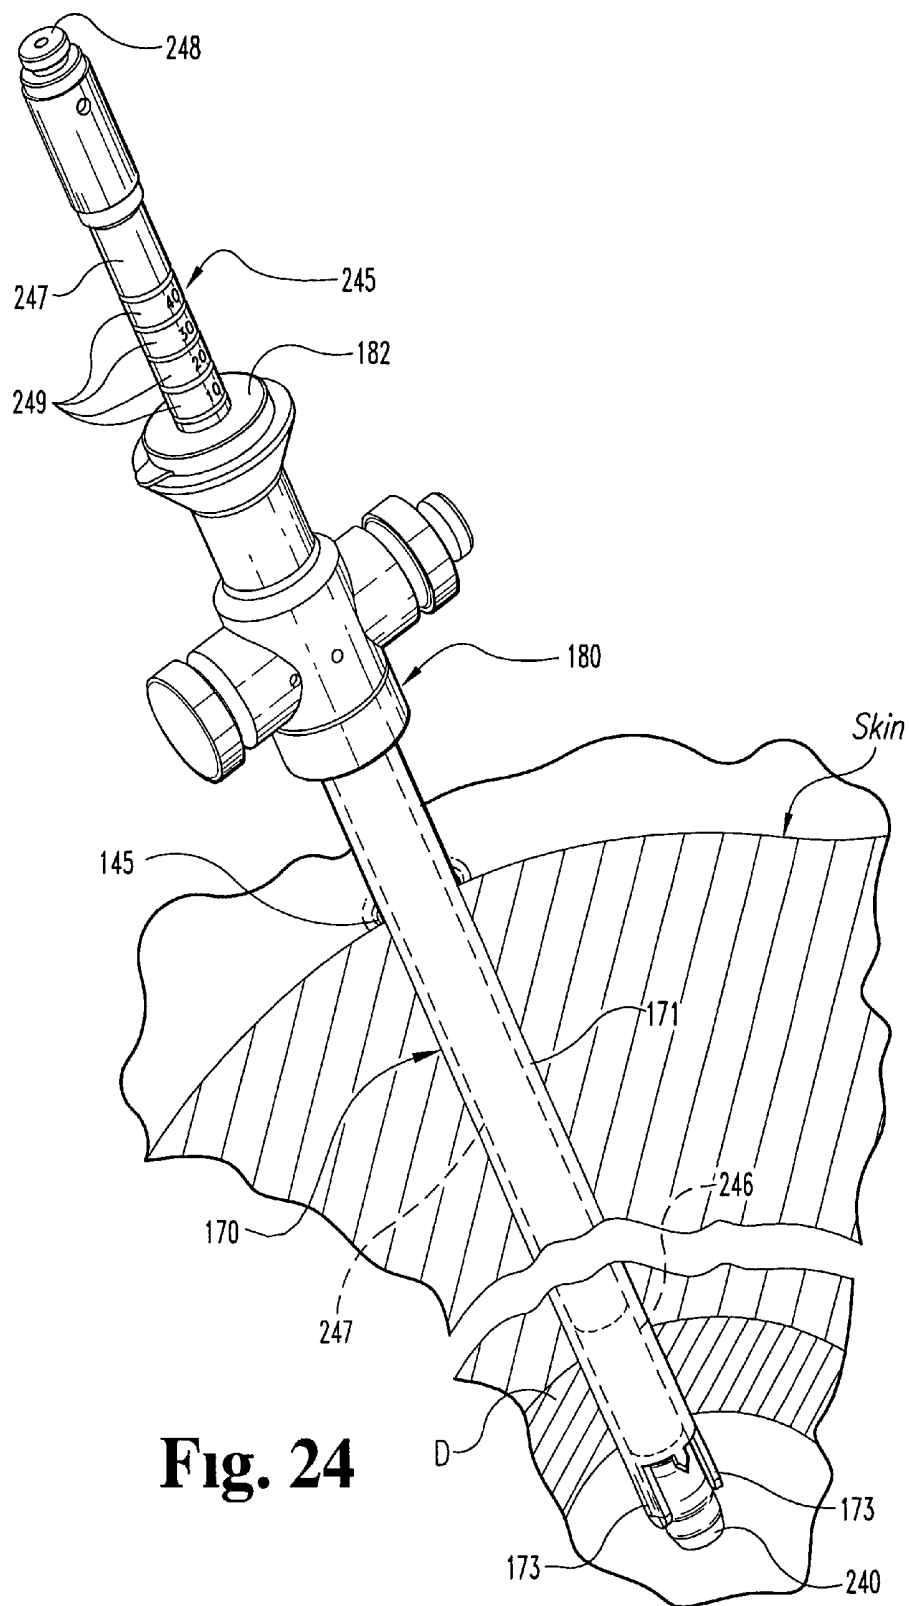


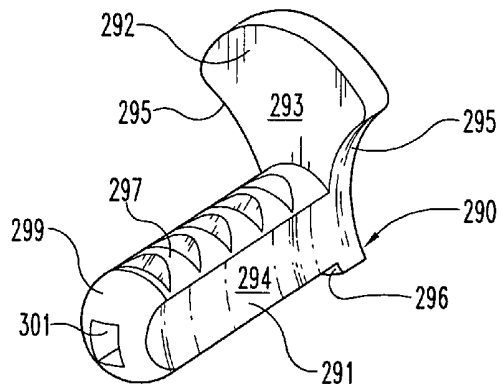


**Fig. 25**

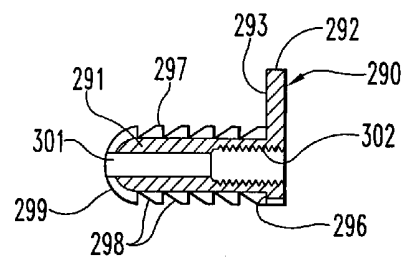


**Fig. 26**

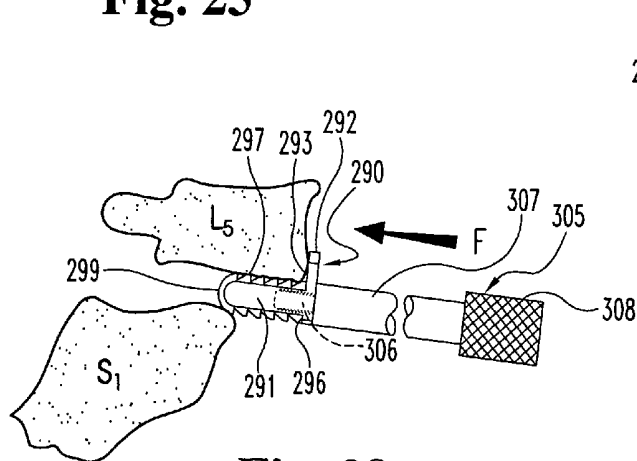


**Fig. 28**

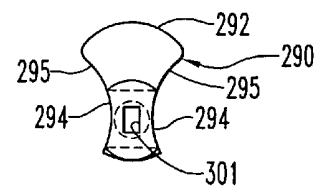



**Fig. 27**

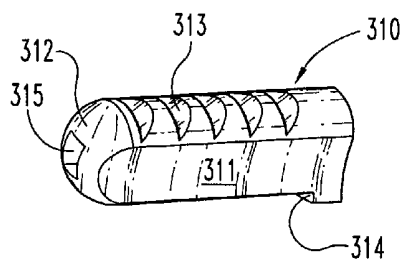


**Fig. 29**

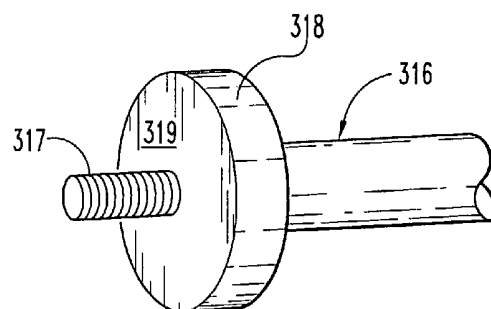


**Fig. 30**

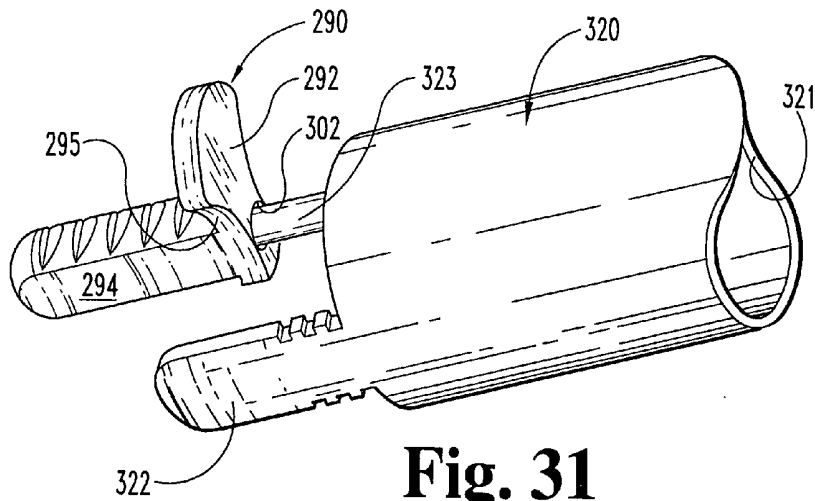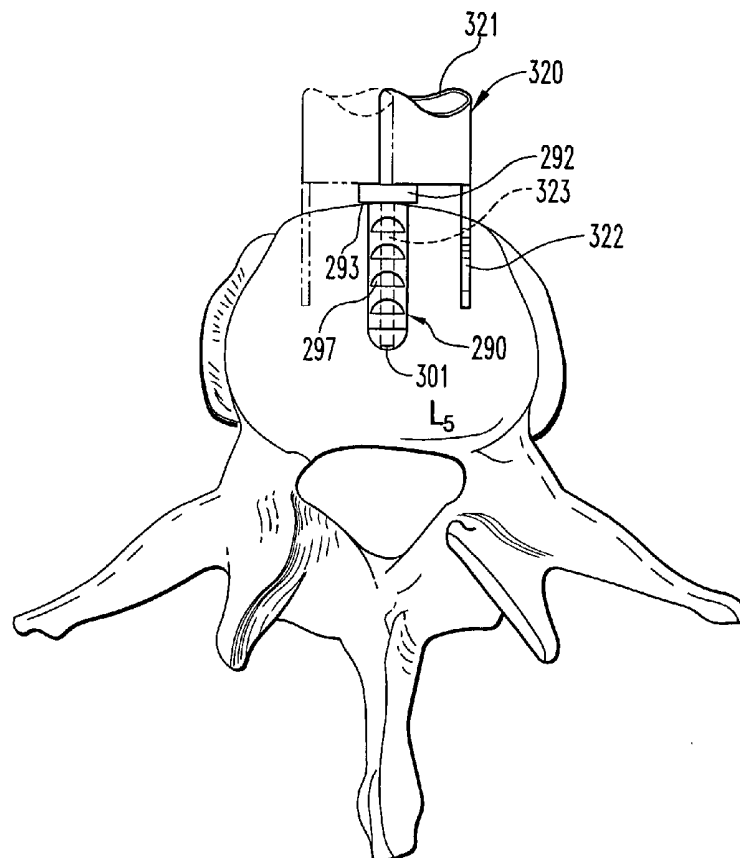
**Fig. 31****Fig 32**

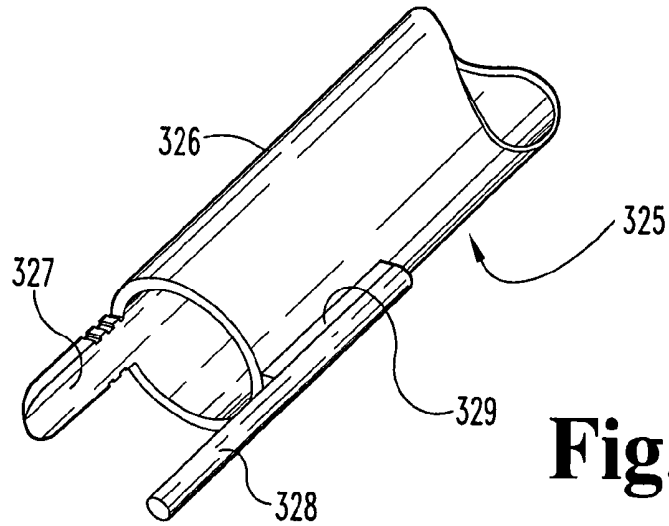


**Fig. 33**

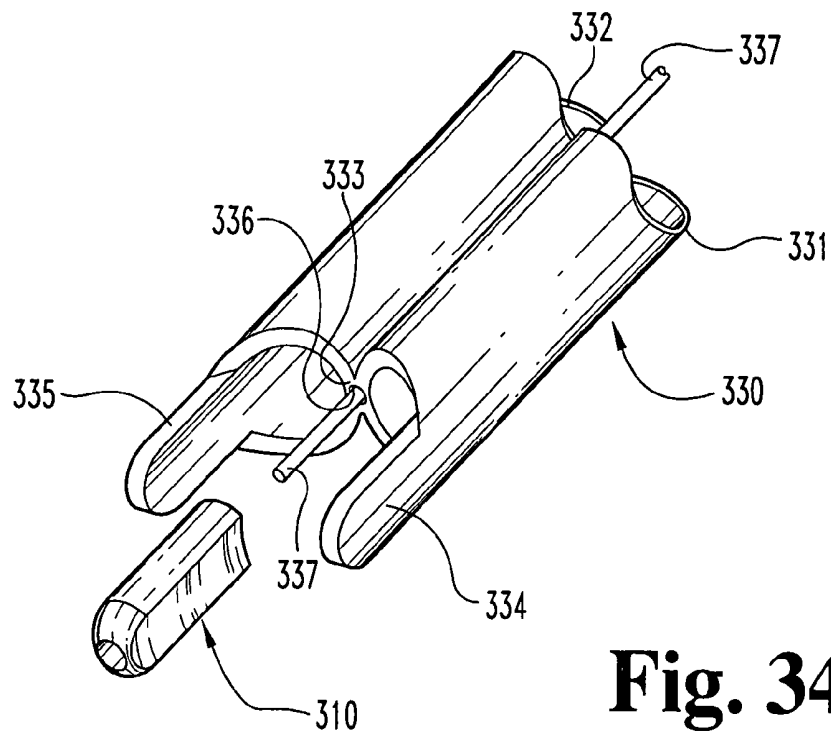

**Fig. 34**

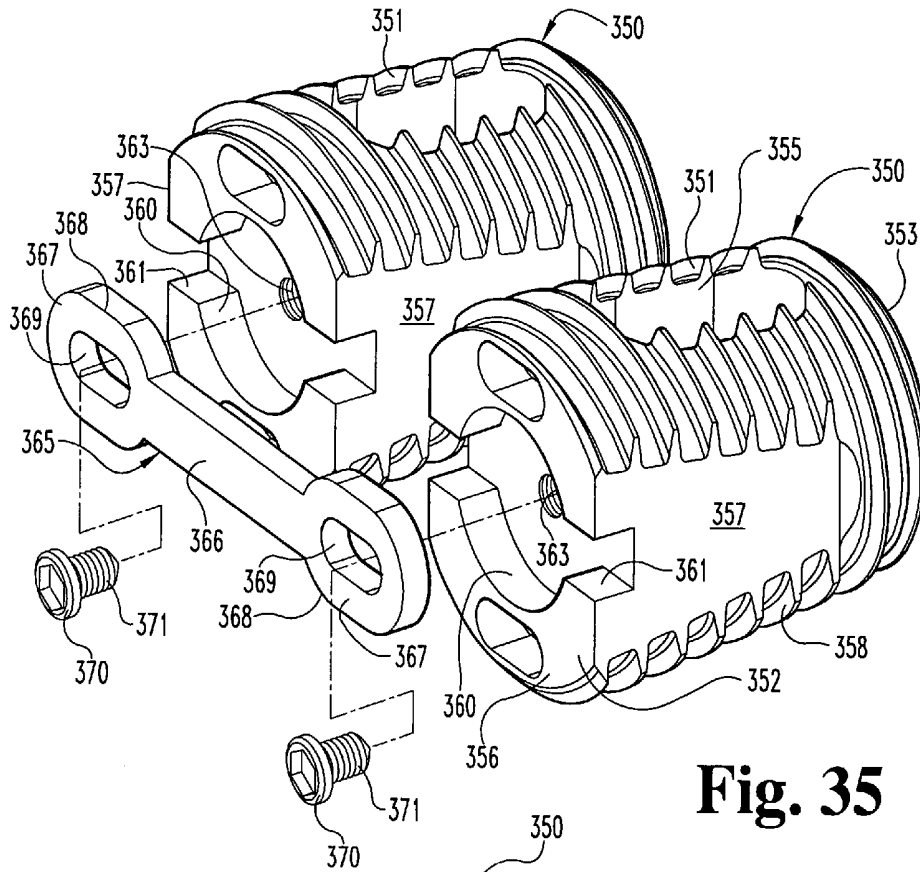

**Fig. 35**

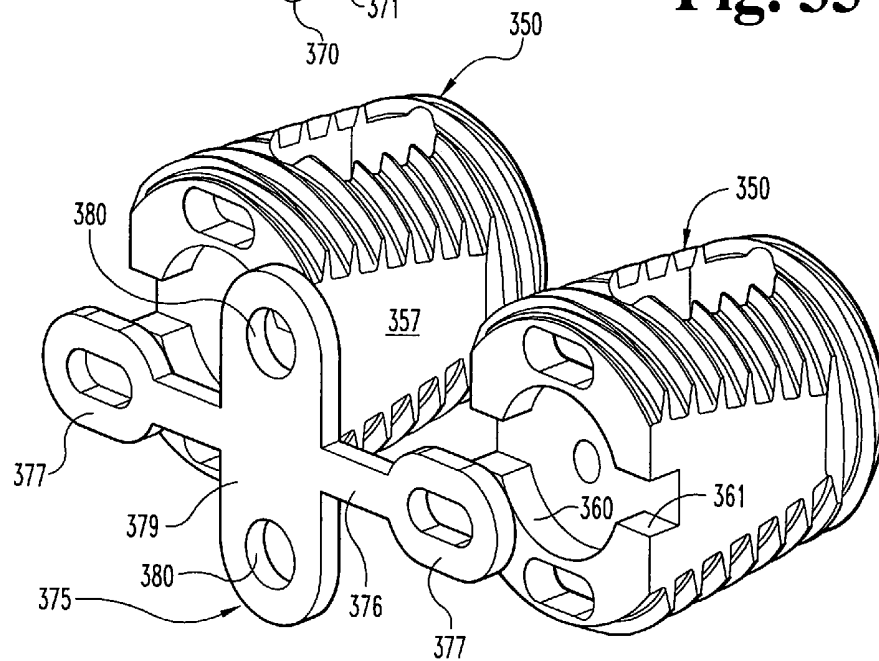

**Fig 36**

## METHODS AND INSTRUMENTS FOR INTERBODY FUSION

This application is a divisional application of U.S. patent application Ser. No. 10/213,864, filed on Aug. 7, 2002 now U.S. Pat. No. 6,695,851, which is a divisional application of U.S. patent application Ser. No. 09/781,589, filed on Feb. 5, 2001, now U.S. Pat. No. 6,471,724, which is a divisional application of U.S. patent application Ser. No. 09/014,901, filed on Jan. 28, 1998, now U.S. Pat. No. 6,206,922, which is a continuation-in-part application of U.S. patent application Ser. No. 08/604,874, filed on Feb. 22, 1996, now abandoned, which is a continuation-in-part application of U.S. patent application Ser. No. 08/411,017, filed on Mar. 27, 1995, now U.S. Pat. No. 5,782,919, the contents of each application hereby being incorporated by reference.

### BACKGROUND OF THE INVENTION

The present invention relates to methods and instruments for performing an interbody fusion of a disc space between two adjacent vertebrae. Specifically, the invention concerns laparoscopic techniques and instruments to prepare a fusion site and to insert fusion devices and implants.

The number of spinal surgeries to correct the causes of low back pain has steadily increased over the last several years. Most often, low back pain originates from damage or defects in the spinal disc between adjacent vertebrae. The disc can be herniated or can be suffering from a variety of degenerative conditions, so that in either case the anatomical function of the spinal disc is disrupted. The most prevalent surgical treatment for these types of conditions has been to fuse the two vertebrae surrounding the affected disc. In most cases, the entire disc will be removed, except for the annulus, by way of a discectomy procedure. Since the damaged disc material has been removed, something must be positioned within the intradiscal space, otherwise the space may collapse resulting in damage to the nerves extending along the spinal column.

The intradiscal space is often filled with bone or a bone substitute in order to prevent disc space collapse and to promote fusion of the two adjacent vertebrae. In early techniques, bone material was simply disposed between the adjacent vertebrae, typically at the posterior aspect of the vertebrae, and the spine column was stabilized by way of a plate or a rod spanning the affected vertebrae. Once fusion occurred the hardware used to maintain the stability of the segment became superfluous. Moreover, the surgical procedures necessary to implant a rod or plate to stabilize the level during fusion were frequently lengthy and involved.

It was therefore determined that a more optimal solution to the stabilization of an excised disc space is to fuse the vertebrae between their respective end plates, preferably with the need for anterior or posterior plating. There have been an extensive number of attempts to develop an acceptable intradiscal implant that could be used to replace a damaged disc and maintain the stability of the disc interspace between the adjacent vertebrae, at least until complete arthrodesis is achieved. These "interbody fusion devices" have taken many forms. For example, one of the more prevalent designs takes the form of a cylindrical implant. These types of implants are represented by the patents to Bagby, U.S. Pat. No. 4,501,269; Brantigan, U.S. Pat. No. 4,878,915; Ray, U.S. Pat. Nos. 4,961,740 and 5,055,104; and Michelson, U.S. Pat. No. 5,015,247. In these cylindrical implants, the exterior portion of the cylinder can be threaded to facilitate insertion or the interbody fusion device, as represented by the Ray, Brantigan and Michelson patents. In the alternative, some of the fusion

implants are designed to be pounded into the intradiscal space and the vertebral end plates. These types of devices are represented by the patents to Brantigan, U.S. Pat. Nos. 4,743,256; 4,834,757 and 5,192,327.

Interbody fusion devices can be generally divided into two basic categories, namely solid implants and implants that are designed to permit bone ingrowth. Solid implants are represented by U.S. Pat. Nos. 4,878,915; 4,743,256; 4,349,921 and 4,714,469. The remaining patents discussed above include some aspect that permits bone to grow across the implant. It has been found that devices that promote natural bone ingrowth achieve a more rapid and stable arthrodesis. The device depicted in the Michelson patent is representative of this type of hollow implant which is typically filled with autologous bone prior to insertion into the intradiscal space. This implant includes a plurality of circular apertures which communicate with the hollow interior of the implant, thereby providing a path for tissue growth between the vertebral end plates and the bone or bone substitute within the implant. In preparing the intradiscal space, the end plates are preferably reduced to bleeding bone to facilitate this tissue ingrowth. During fusion, the metal structure provided by the Michelson implant helps maintain the patency and stability of the motion segment to be fused. In addition, once arthrodesis occurs, the implant itself serves as a sort of anchor for the solid bony mass.

Another interbody fusion device that is designed to permit bone ingrowth is shown in FIG. 1. This device is described and claimed in co-pending parent application Ser. No. 08/411, 017, filed on Mar. 27, 1995, which disclosure is incorporated herein by reference. In one embodiment, this invention contemplates a hollow threaded interbody fusion device **10** configured to restore the normal angular relation between adjacent vertebrae. In particular, the device **10** as shown in FIG. 1 includes an elongated body **11**, tapered along substantially its entire length, defining a hollow interior **15** and having a largest outer diameter at the anterior end **12** of the device to receive the bone growth material. The body **11** includes an outer surface **16** with opposite tapered cylindrical portions and a pair of opposite flat tapered side surfaces **22** between the cylindrical portions. Thus, at an end view, the fusion device gives the appearance of a cylindrical body in which the sides of the body have been truncated along a chord of the body's diameter.

The cylindrical portions include threads **18** for controlled insertion and engagement into the end plates of the adjacent vertebrae. A started thread **19** is provided at the posterior end **13** of the device **10** to facilitate engagement within a prepared bore. The outer surface of this fusion device is tapered along its length at an angle corresponding, in one embodiment, to the normal lordotic angle of the lower lumbar vertebrae. The outer surface is also provided with a number of vascularization openings **24**, **25** defined in the flat side surfaces, and a pair of opposite elongated bone ingrowth slots **27** defined in the cylindrical portions.

Various surgical methods have been devised for the implantation of fusion devices into a subject disc space. A patent to Dr. Gary Michelson, U.S. Pat. No. 5,484,437, discloses one such technique and the associated instruments. As described in more detail in that patent, the surgical technique involved the use of a hollow sleeve having teeth at one end that are driven into the adjacent vertebrae. These teeth and the sleeve maintain the disc space height during the subsequent steps of the procedure. In accordance with one aspect of the invention in the '437 patent, a drill is passed through the hollow sleeve to remove the disc and bone material to produce a prepared bore for the fusion device. The drill is then

removed from the sleeve and the fusion device is positioned within the disc space using an insertion tool.

In another aspect of the procedure and instruments disclosed in the '437 patent, a long distractor is provided having penetrating portions that urge the vertebral bodies apart to facilitate the introduction of the necessary instruments. The long distractor can act as a guide for drilling and reaming tools concentrically advanced over the outside of the distractor to prepare the site for the fusion device.

While the Michelson technique represents a significant advance over prior surgical procedures for the preparation and insertion of fusion devices, the need for improvement remains. In particular, procedures and instruments that preserve the integrity of the surgical site are desirable. The present invention is directed to this need in the field.

### SUMMARY OF THE INVENTION

In accordance with one aspect of the invention, a novel fusion device is provided that integrates a pair of bone screws. The fusion device can be a hollow substantially cylindrical body, such as the device shown in FIG. 1. In this aspect, the device includes a pair of screw bores formed in an end face of the body. The bores are arranged so that bone screws extending through the bores will be driven into the endplates of the adjacent vertebrae. In certain features, the heads of the bone screws are recessed within the body and held in place by a common locking screw. The screws help prevent retrograde expulsion or rotation of the fusion device, or a spacer, from the disc space.

The present invention also contemplates another approach to preventing rotation and/or dislodgment of fusion devices placed bilaterally in the disc space. In one embodiment, a transverse connector plate is engaged by locking screws to the end walls of the bilateral fusion devices. In one feature, the end walls define central recesses and transverse grooves to receive the connector plate. In another embodiment, the connector plate can include screw bores to receive bone screws driven into the vertebrae at a location in between the fusion devices.

In another aspect of the invention, a method is provided for preparing a subject disc space for implantation of a fusion device or implant between adjacent vertebrae. In this technique, a laparoscope is provided that includes an outer sleeve with opposite extensions at one end of the outer sleeve and a laparoscopic port engaged at the outer end of the outer sleeve, the laparoscopic port having a number of seals, with the opposite extensions configured to maintain distraction of the adjacent vertebrae.

The preferred technique comprises the steps of making an incision in the skin of the patient aligned with the subject disc space, retracting tissue beneath the incision to expose the disc annulus; and piercing the disc annulus to create an opening. The outer sleeve of the laparoscope is advanced through the incision, leaving the port outside the skin of the patient while inserting the opposite extensions into the disc space with the outer sleeve contacting the disc annulus. The laparoscope, and particularly, the outer sleeve, creates a protected working channel between the disc space and the laparoscopic port outside the patient.

In a further step of the preferred inventive technique, a reamer is operated through the number of seals and the outer sleeve of the laparoscope to create a prepared bore in the disc material and the adjacent vertebrae for implantation of a device into the bore.

In a most preferred embodiment of the surgical technique, the technique comprises the steps of percutaneously exposing

the annulus of the disc in the subject disc space through an incision in the skin of the patient and piercing the disc annulus to create an opening. A distractor can then be inserted through the incision and through the opening into the disc space to distract the vertebrae adjacent the subject disc space. The laparoscope outer sleeve is then introduced through the incision and over the distractor, leaving the port outside the skin of the patient while inserting the opposite extensions through the opening into the disc space to create the protected working channel between the port and the distractor tip.

In subsequent steps, the distractor is removed and a reamer is advanced through the number of seals of the laparoscope and through the outer sleeve into the disc space to ream the disc space and adjacent vertebrae to create a prepared bore for the fusion implant. After the reamer is removed from the laparoscope, the fusion implant can be advanced through the number of seals and through the outer sleeve into the prepared bore. With the fusion implant in position, the laparoscope can be withdrawn from the patient.

In one aspect of the invention, a switching sleeve is placed within the outer sleeve of the laparoscope with an end of the switching sleeve projecting beyond the opposite fingers of the outer sleeve, the end of the switching sleeve being tapered to minimize trauma to tissue adjacent the subject disc space as the outer sleeve adjacent into the patient with the switching sleeve projecting beyond the opposite extensions of the outer sleeve.

In a further embodiment, the laparoscopic method is used for bilateral placement of two fusion devices into a subject disc space. In addition to the steps previously described, this embodiment of the surgical technique includes unseating the outer sleeve of the laparoscope from the first opening in the disc annulus by withdrawing the laparoscope until the opposite extensions of the outer sleeve are outside the disc annulus. With the switching sleeve in position within the outer sleeve, the laparoscope is moved to the second opening in the disc space without removing the laparoscope from the patient. The steps for preparing the bore to receive a fusion implant can be repeated. In one specific embodiment, these steps are conducted at the second opening with the distractor remaining within the first opening. After a fusion implant is advanced through the number of seals and through the outer sleeve into the second prepared bores the laparoscope can then be returned to the first opening for insertion of another fusion implant. During this step, the fusion implant contained within the second prepared bore maintains distraction of the disc space.

As an adjunct to this inventive technique, a distraction device is provided in one aspect of the invention. The distraction device can include an elongated stem sized for insertion along the A-P midline of the intervertebral disc space. Preferably, opposite surfaces of the device include a number of ridges that operate as bone engaging surfaces to resist expulsion of the device. In one important feature, the stem of the distraction device includes a bore to receive a spike projecting from a tubular body, such as the outer sleeve discussed above. With this feature, the distraction device acts not only as a midline distractor, but also as a centering guide to locate the tubular body through which subsequent surgical procedures can be performed.

In a further feature, the distraction device can include a flange projecting from the stem. The flange has a bone contacting that transmits to the vertebra a force applied to the distraction device (preferably by a manual tool). This flange can be used to reduce a high grade spondylolisthesis condition as the distraction device is driven into the disc space.



One object of the present invention is to provide surgical technique and instruments that permit the preparation of a disc space for insertion of a fusion implant under a sealed condition. A further object of the invention is to implement laparoscopic techniques to implant fusion devices.

With respect to fusion devices, one object is to enhance the stability of the device in situ while reducing the risk of expulsion of the device. Yet another object is to provide means for readily reducing a spondylolisthesis condition from a laparoscopic approach.

One benefit of the present invention is that all of the steps necessary to prepare a disc space and to implant a fusion device can be conducted in a protected environment. In addition, the inventive techniques and instruments allow minimal intrusion into the patient, which minimized the risks normally associated with spinal surgery.

Other objects and benefits can be discerned from the following written description and accompanying figures.

#### DESCRIPTION OF THE FIGURES

FIG. 1 is a side perspective view of a threaded fusion device having a tapered configuration to restore the normal angle of a spinal motion segment.

FIG. 2 is a top elevational view of an implant driver for use in engaging and driving a fusion device such as the device shown in FIG. 1.

FIG. 3 is an enlarged perspective view of the end of the implant driver shown in FIG. 2 engaged to a fusion device such as shown in FIG. 1.

FIG. 4 is an enlarged side cross-sectional view of the implant driver and fusion device shown in FIG. 3.

FIG. 5 is an enlarged side cross-sectional view of an alternative embodiment of an implant driver for engaging and driving a fusion device such as the device shown in FIG. 1.

FIG. 6 is a driving tool attachment according to one aspect of the present invention.

FIG. 7 is an enlarged side cross-sectional view similar to the view in FIG. 5 with the driving tool attachment of FIG. 6 engaged between the implant driver and the fusion device.

FIG. 8 is an end perspective view of a threaded fusion device according to a further embodiment of the invention.

FIG. 9 is a side perspective view of a driving tool attachment according to a further aspect of the present invention in which the driving tool attachment is configured to engage the fusion device depicted in FIG. 8.

FIG. 10 is a side partial cross-sectional view of a fusion device according to the embodiment of FIG. 8 disposed between adjacent vertebrae and engaged in position by a pair of bone screws in accordance with one aspect of the present invention.

FIGS. 11(a)-(d) are lateral representations of the spine showing four steps of a surgical method for implanting a fusion device such as the device in FIG. 1 according to an anterior approach in one aspect of the present invention.

FIGS. 12(a)-(d) are lateral representations of the spine showing four steps of a surgical method for implanting a fusion device such as the device in FIG. 1 according to a posterior approach in a further aspect of the present invention.

FIG. 13 is a frontal view of a patient with locations identified for surgical incisions according to a preferred embodiment of the present inventive laparoscopic surgical technique.

FIG. 14 is an A-P representation of a spinal segment at the laparoscopic surgical site depicting one step of the inventive surgical technique in which bilateral locations are marked on the disc annulus for insertion of a pair of fusion devices, such as the device shown in FIG. 1.

FIG. 15 is an enlarged A-P view of the disc at the spinal segment showing the use of the template represented in FIG. 14 of the invention.

FIG. 16 is an A-P representation of the laparoscopic surgical site depicting a further step of the inventive surgical technique of creating a pilot hole at each of the bilateral locations marked in the step shown in FIG. 14.

FIG. 17 is an A-P representation of the laparoscopic surgical site depicting a further step of the inventive surgical technique of using a trephine to create a bore at each of the bilateral locations marked in the step shown in FIG. 14.

FIG. 18 is an A-P representation of the laparoscopic surgical site depicting a further step of the inventive surgical technique for inserting a distractor into the prepared site at each of the bilateral locations marked in the step shown in FIG. 11.

FIG. 19 is a perspective representation of the laparoscope according to the present invention in which the outer sleeve of the laparoscope is engaged within the subject disc space.

FIG. 20(a) is a perspective representation of the laparoscope of FIG. 19 with a switching sleeve according to one aspect of the invention disposed within the laparoscope.

FIG. 20(b) is an enlarged A-P representation of the laparoscope and switching sleeve of FIG. 20(a) showing the positioning of the distractor tip as depicted in FIG. 18.

FIG. 21 is a perspective representation of the laparoscope of FIG. 19 with a reamer extending through the laparoscope to prepare the site for receiving a fusion device.

FIG. 22 is a perspective view of an implant driver of the type shown in FIG. 2 engaged to a fusion device and including a T-handle assembly engaged to the driver.

FIG. 23 is a perspective view of an implant holder according to one aspect of the present invention.

FIG. 24 is a perspective representation of the laparoscope used to implant a bone dowel within the prepared site and including a bone dowel impactor in accordance with one aspect of the present invention.

FIG. 25 is a top perspective view of a distraction plug in accordance with one embodiment of the present invention.

FIG. 26 is a side cross-sectional view of the distraction plug shown in FIG. 25.

FIG. 27 is an end elevational view of the distraction plug shown in FIGS. 25 and 26.

FIG. 28 is a side view of the distraction plug shown in FIG. 25 as it is inserted between adjacent vertebrae using a plug driver in accordance with one aspect of the present invention.

FIG. 29 is a side perspective view of a distraction plug in accordance with a further embodiment of the present invention.

FIG. 30 is a side perspective view of a plug driver in accordance with a further embodiment of the invention configured for engaging a distractor plug as shown in FIG. 29.

FIG. 31 is a rear perspective view of a percutaneous surgical sleeve in engagement with a distractor plug in accordance with the embodiment shown in FIG. 25.

FIG. 32 is a superior A-P view of a vertebra of the spine with the distractor plug and percutaneous surgical sleeve shown in FIG. 31 disposed within the disc space, with an alternative position of the sleeve shown in phantom.

FIG. 33 is a side perspective view of a percutaneous surgical sleeve in accordance with a further embodiment of the invention with an outrigger spike engaged thereto for attachment to a distractor plug according to FIG. 25 or 29.

FIG. 34 is an end perspective view of a double barrel percutaneous surgical sleeve configured for engaging a distractor plug, such as the distractor plug shown in FIG. 29.

FIG. 35 is a side perspective view of an assembly in accordance with a further embodiment of the present invention utilizing a pair of fusion devices connected by a connector plate.

FIG. 36 is a side perspective view of an alternative embodiment of the assembly with a pair of fusion devices interconnected by an alternative connector plate.

#### DESCRIPTION OF THE PREFERRED EMBODIMENTS

For the purposes of promoting an understanding of the principles of the invention, reference will now be made to the embodiments illustrated in the drawings and specific language will be used to describe the same. It will nevertheless be understood that no limitation of the scope of the invention is thereby intended, such alterations and further modifications in the illustrated device, and such further applications of the principles of the invention as illustrated therein being contemplated as would normally occur to one skilled in the art to which the invention relates.

As described above, one interbody fusion device, as shown in FIG. 1, can be implanted within the intradiscal space. This interbody fusion device 10 can be implanted using the implant driver 50 shown in FIG. 2. The implant driver 50 is comprised of a shaft 51 and sleeve 52 concentrically disposed about the shaft. Tongs 54 are formed at one end of the shaft for gripping the interbody fusion device 10 for implantation. Preferably the tongs include a tapered outer surface 55 and an opposite flat inner surface 56 adapted to engage the truncated side walls 22 of the interbody fusion device as shown in FIGS. 3, 4. Most preferably the tapered outer surface 55 conforms to the root diameter of the interrupted threads 18 of the device 10 so that the tongs 54 essentially complete the full cylindrical shape of the body wall 16. The adaptation of the tongs' tapered outer surface 55 facilitates screw insertion of the interbody fusion device 10 since the outer surface 55 will ride within the tapped bore in the vertebral end plates.

Each of the tongs 54 can be provided with interlocking fingers 58 and a driving projection 59 extending from the inner surface 56, most clearly shown in FIG. 4. Referring again to FIG. 2, the shaft 51 defines a hinge slot 62 supporting each of the pair of tongs 54. The hinge slot 62 is configured so that the tongs will have a naturally biased position spread sufficiently apart to accept the fusion device 10 therebetween. The shaft 51 defines a conical taper 63 between the hinged slot 62 and each of the tongs 54. This conical taper mates with a conical chamfer 67 defined on the inner wall of the sleeve 52. Thus, as the sleeve 52 is advanced toward the tongs 54, the conical chamfer 67 rides against the conical taper 63 to close or compress the hinge slot 62. In this manner, the tongs 54 are pushed toward each other and pressed into gripping engagement with the interbody fusion device situated between the tongs.

The shaft 51 and sleeve 52 are provided with a threaded interface 65 which permits the sleeve 52 to be threaded up and down the length of the shaft. Specifically, the threaded interface 65 includes external threads on the shaft 51 and internal threads on the sleeve 52 having the same pitch so that the sleeve can be readily moved up and down the implant driver 50. The shaft 51 is also provided with a pair of stops 69 which restrict the backward movement of the sleeve 52 to only the extent necessary to allow the tongs 54 to separate a sufficient distance to accept the interbody fusion device 10.

The use of the implant driver 50 is shown with reference to FIGS. 3, 4. As can be seen in FIG. 3, the outer surface 55 of the tongs 54 reside generally flush with the root diameter of the

interrupted threads 18. As seen in FIG. 4, the interlocking fingers 58 can be arranged to fit within the vascularization opening 24 on each of the truncated side walls 22. In a similar fashion, the driving projections 59 engage the driving tool slots 29 at the anterior end 12 of the conical body 11. The combination of the interlocking fingers 58 and driving projections 59 firmly engage the interbody fusion device 10 so that the device can be screw threaded into a tapped or untapped opening in the vertebral bone. The tongs 54 in this embodiment are configured to engage the fusion device 10 and to impart a threading or rotational force to the device. It is understood that the tongs can adopt other configurations depending upon the structure of the fusion device to be implanted. An alternative embodiment of the implant driver is shown in FIG. 5. The driver 90 includes a shaft 91, having a length sufficient to reach into the intradiscal space from outside the patient. Connected to the end of shaft 91 is a head which defines a pair of opposite tongs 93, each of which are configured for flush contact with the flat truncated side walls 22 of the fusion device 10. Like the tongs 54 of the previously described implant driver 50, the outer surface of the tongs is cylindrical to correspond to the cylindrical threaded portion of the device.

Unlike the implant driver 50, the driver 90 of the embodiment in FIG. 5 uses an expanding collet assembly to firmly grip the fusion device 10 for insertion into the body. Specifically, the head 92 defines a collet 94 having a central collet bore 95 formed therethrough. The collet 94 terminates in an annular flange 96 that at least initially has a diameter slightly smaller than the inner diameter of the fusion device 10 at its end 12. An expander shaft 97 slidably extends through the collet bore and includes a flared tip 98 situated adjacent and extending just beyond the annular flange 96. The flared tip 98 of the expander shaft 97 starts at a diameter sized to slide within the collet bore 95 and gradually flares to a diameter larger than the bore.

The implant driver 90 further includes a puller shaft 99 slidably disposed within a bore 100 defined in the shaft 91. The puller shaft 99 has a locking chamber 101 at its end which engages a locking hub 102 formed at the end of the expander shaft 97. The puller shaft 99 projects beyond the end of the shaft 91 for access by the surgeon. When the puller shaft 99 is pulled, it pulls the expander shaft 97 away from the annular flange 96 of the collet 94 so that the flared tip 98 becomes progressively engaged within the collet bore 95. As the tip 98 advances further into the bore 95, the annular flange 96 expands from its initial diameter to a larger second diameter sufficient for firm gripping contact with the interior of the fusion device 10. With the fusion device so engaged, the implant driver can be used to insert the device 10 into the surgical site, after which the expander shaft can be advanced beyond the collet bore to release the flat tip and, consequently, the fusion device.

In certain circumstances, it may be necessary to drive the fusion device 10 deeper into the disc space. When either of the implant drivers 50 or 90 is engaged to the fusion device, the device can be readily advanced farther into the disc space. However, once the implant driver is removed and it is then discovered that the fusion device needs to be repositioned, the flexible nature of the tongs 54 and 93 of the two implant drivers makes reacquisition of the now implanted fusion device difficult. To alleviate this difficulty, a driving tool attachment 120 is provided, as shown in FIG. 6. The driving tool attachment 120 includes a body 121 having a first end 122 and an opposite second end 123. Like the fusion implant, the body 121 of the driving tool attachment 120 includes a cylindrical portion 125 and opposite flat side portions 126.

The opposite side portions **126** are configured to be engaged by the tongs of the above driving tools **50** or **90**.

The driving tool attachment **120** includes a pair of opposing flanges **130** at end **123**. The flanges **130** are configured to engage the opposite flat surface **122** on the fusion implant **10**, in a manner similar to that accomplished by the tongs of the implant driver **50** and **90**. The end **123** also includes a boss **131** which is configured to be inserted into the opening at the end of the implant **10** (see FIG. 7).

In use, the driving tool attachment **120** can be engaged with one of the driving tools **50** or **90**, with the tongs firmly grasping the flat surfaces **126**, as shown in FIG. 7. The driving tool attachment can then be advanced into the disc space with the flanges **130** oriented across the space so that they can readily interface with the flat surfaces **22** of the fusion device **10**. When the driving tool attachment **120** is properly aligned, the boss **131** projects into the hollow opening **15** at the anterior end **12** of the fusion device and the flanges **130** engage the opposite flat surfaces **22** of the device. The driving tool can then be rotated as if the fusion implant were directly engaged to the main driving tool. The attachment readily transmits the rotational driving force to the implant **10** to thread it deeper into the disc space or to retract it back within the disc space. One particular advantage provided by the driving tool attachment **120** is that the relatively flexible tongs of the two driving tools **50** and **90** can be already engaged to the attachment **120** before insertion into the surgical site. This eliminates a great deal of fiddle factor and avoids the risk that the tongs would be unable to firmly grasp the implant **10** when it is already in position within the disc space.

In a further embodiment of the present invention, an interbody fusion device is provided that permits supplemental fastening to the adjacent vertebrae. In particular, an interbody fusion device **250**, as depicted in FIG. 8, includes a hollow body **251** having a first end **252** and a second end **253**. The hollow body **251** defines a hollow interior **255** and includes an end wall **256** at the first end **252**. Like the fusion device **10** shown in FIG. 1, the interbody fusion device **250** includes external threads **258** spanning a substantial portion of the length of the hollow body **251**, and a continuous thread **259** adjacent the second end **253** of the body. Also like the fusion device **10**, the interbody fusion device **250** includes opposite flat sidewalls **262** that interrupt the external threads **258**, as well as opposing slots **263** offset from the flat sidewalls **262** which also interrupts a portion of the external threads **258**. Thus far, the interbody fusion device **250** is substantially similar to the device **10** shown in FIG. 1. For example, the device can be tapered so that it has a larger diameter at the first end **252** than at the second end **253**. In addition, side windows **264** (see FIG. 10) can be provided in the flat sidewalls **262**. The side walls **262** essentially divide the body **251** into upper and lower threaded portions that are configured to be threadedly driven into adjacent vertebrae.

In accordance with this embodiment, the interbody fusion device **250** includes a pair of driver openings **265** defined in the end wall **256** at the first end **252**. Intermediate between the driver openings **265** are a pair of offset screw bores **267**. In this preferred embodiment, the screw bores **267** are formed so that their respective longitudinal axes intersect and project out from the top and bottom portions **260**, **261**. Preferably the axes are arranged to intersect the slots **263** in the top and bottom of the fusion device. In this configuration, the longitudinal axes of the two screw bores intersect outside the hollow body **251** and the end wall **256**, as seen in FIG. 10. A threaded bore **270** is formed between the two screw bores **267**. The screw bores **267** also define a recessed portion **268**,

while the threaded bore defines a recessed portion **271** that intersects each of the recessed portions **268** of the screw bores **267** at an overlap **272**.

In using the interbody fusion device **250**, a driving tool attachment **275** is provided that permits insertion of the device within a properly prepared intervertebral space. As depicted in FIG. 9, the driving tool attachment **275** is similar to the implant driver shown in FIG. 6. In this instance, the driving tool attachment **275** includes a body **276** having opposite flat sidewalls **277**, so that the body is adapted to be engaged by the implant driver **90** in the manner depicted in FIG. 7. In accordance with the present embodiment, the driving tool attachment **275** includes a pair of spaced-apart driving bosses **278** projecting from a mating face **279**. The bosses **278** are sized and shaped to fit within the driver openings **265** when the mating face **279** is in direct contact with the end wall **256** of the fusion device **250**. The driving tool attachment **275** can be engaged to a fusion device, such as device **250**, to permit threading of the device into the intervertebral disc space, such as the space between lumbar vertebrae L4 and L5, as shown in FIG. 10.

With the fusion device **250** appropriately positioned within the intervertebral disc space, a pair of bone screws **280** can be extended through respective screw bores **267** in the hollow body **251**. The screws are passed through the bores **267** until the bone engaging threads of the screws **280** contact the vertebral bone. As the bone screws **280** are threaded into the vertebral bone, the head **281** of each of the bone screws **280** seats within the respective recessed portions **268** of each of the screw bores **267**. In this orientation, the heads **281** of the bone screws **280** are flush with or below the surface of the end wall **256** of the fusion device **250**. At this point, a locking screw **282** can be threaded into the threaded bore **270**. As the locking screw is tightened into the bore **270**, the head **283** of the locking screw contacts the heads **281** of both bone screws **280**. Further tightening of the locking screw **282** causes the head **283** to seat within the recessed portion **271** to trap the heads **281** of the bone screws **280** within their respective screw bores **267**. Thus, the set screw **282** prevents backout of the bone screws **280** when they are engaged within the adjacent vertebrae.

The diverging bone screws **280** provide greater stability to the fusion device **250** than can be achieved with prior threaded devices. The bone screws enhance the resistance to retrograde expulsion of the device and prevents counter-rotation or unthreading. The bone screws **280** can be of a wide range of sized provided that the screws are long enough to achieve an effective purchase in the adjacent vertebrae.

In accordance with additional aspects of the present invention, two methods for implanting an interbody fusion device, such as the devices **10** or **250**, are contemplated. First, with reference to FIGS. 11(a)-11(d), an anterior approach is shown. As a preliminary step, it is necessary to locate appropriate starting points for implanting the fusion device, preferably bilaterally. In the first step of the anterior approach, a distractor **75** is disposed between the vertebral end plates E to dilate the L4-L5 or L5-S1 disc space. (It is understood, of course, that this procedure can be applied at other vertebral levels). In the second step, shown in FIG. 11(b), an outer sleeve **76** is disposed about the disc space. The outer sleeve **76** can be configured to positively engage the anterior aspect of the vertebral bodies to firmly, but temporarily, anchor the outer sleeve **76** in position. In essence, this outer sleeve **76** operates as a working channel for this approach. In the step of FIG. 11(b), a drill **77** of known design is extended through the outer sleeve and used to drill out circular openings in the

adjacent vertebral bodies. The openings can be tapped to facilitate screw insertion of the fusion device **10**, although this step is not necessary.

In the next step shown in FIG. **11(c)**, the fusion device **10** is engaged by the implant driver **50** and extended through the outer sleeve **76** until the starter thread **19** contacts the bone opening. The implant driver **50** can then be used to screw thread the fusion device into the tapped or untapped opening formed in the vertebral end plate **E**. It is understood that in this step, other suitable driving tools could be used, such as a screw driver configured to engage the driving tool slots **29** at the anterior end **12** of the device **10**. The degree of insertion of the fusion device **10** determines the amount of lordosis added or restored to the vertebral level. In the final step, the implant driver is removed leaving the fusion device **10** in position. It can be seen that once implanted, the closed posterior end **13** is directed toward the posterior aspect of the vertebrae. The hollow interior **15** is open at its anterior end **12**, but can be closed by a plastic or metal material, if necessary.

In a second inventive method, as depicted in FIGS. **12(a)**-**12(d)**, a posterior approach is implemented. The first two steps of the posterior approach are similar to that of the prior anterior approach, except that the distractor **75**, outer sleeve **76** and drill **77** are introduced posteriorly at the instrumented motion segment. This approach may require decortication and removal of vertebral bone to accept the outer sleeve **76**. In the third step of this method, the fusion device **10** is inserted through the outer sleeve **76** into the dilated disc space. It is understood that the disc space is preferably dilated only to the extent necessary to receive the implant with the truncated side walls **22** directly facing the vertebral end plates **E**. Thus, as shown in FIG. **12(c)**, the bone ingrowth slot **27** is facing laterally, rather than coronally, as expected for its final implanted position. A suitable driving tool **80** can be provided to project the fusion device **10** through the outer sleeve **76** and into the intradiscal space. In one embodiment, the driving tool **80** includes a projection **81** which is configured to engage a slot opening formed in the end wall at the posterior end **13** of the fusion device **10**. An internal thread (not shown) can be used to fix the device **10** to the driver **80**.

Once the fusion device **10** has been advanced into the intradiscal space to the appropriate depth relative to the pivot axis **P** of the vertebrae, the driving tool **80** is used to rotate the implant in the direction of the rotational arrow **R** in FIG. **12(c)**. As the driving tool **80** is rotated, the device itself rotates so that the interrupted threads **18** start cutting into the vertebral bone at the end plates **E**. In this manner, the implant operates as a cam to separate the adjacent vertebrae in the direction of the spreading direction arrows **S** in FIG. **12(c)**. This camming approach provides a somewhat easier insertion procedure than for the anterior approach of FIGS. **11(a)**-**(d)** in that a single rotation is required to lock the implant into the vertebral bone. In contrast, the formerly discussed screw insertion technique of the anterior approach requires continuous threading of the device into position.

With either the anterior (FIGS. **11(a)**-**(d)**) or the posterior approach (FIGS. **12(a)**-**(d)**), the position of the fusion device **10** with respect to the adjacent vertebrae can be verified by radiograph or other suitable techniques for establishing the angular relationship between the vertebrae. Alternatively, the preferred depth of insertion of the implant can be determined in advance and measured from outside the patient as the implant is positioned between the vertebrae. The depth of insertion of the fusion device can be ascertained using depth markings (not shown) on the implant drivers **50**, **90** or **80**.

In another embodiment of the inventive surgical technique, laparoscopic technology is used to provide a sealed and pro-

tected channel for instruments and implants directed to the subject disc space. In accordance with one aspect of this inventive method, an anterior approach to the L5-S1 motion segment is illustrated. It is of course understood that these same techniques and instruments to be described below could be used at different vertebral levels or in a posterior approach under appropriate conditions.

As depicted in FIG. **13**, the present inventive technique includes making a small incision **140** and preferably inserting an insufflator needle into the abdominal cavity. Fluid is introduced into the abdominal cavity through the insufflator needle to a pressure of preferably approximately 15 mm of mercury to assist in visualization of the surgical site. An initial port **141** for the laparoscope is placed five to ten centimeters cephalad of the umbilicus in the midline ten millimeters in length. The abdomen is visually explored and the patient is placed in steep Trendelenburg. The abdominal wall is visualized endoscopically as two working ports **142**, **143** are placed just lateral to the epigastric vessels, opposite the level or levels to be fused. It is believed to be advantageous to stagger the ports slightly from direct opposition to each other.

The preferred method continues with insertion of retractors through the ports **142**, **143**. The retractors can be used to sweep the small bowel superiorly out of the pelvis. The sigmoid colon is also pulled out of the pelvis and held laterally with the left fan retractor. For fusion at the L5-S1 junction, the sacral promontory and drop-off can be easily seen at this point. The posterior peritoneum overlying the L5-S1 disc space is then incised longitudinally with endoshears for the desired exposure. Using opposing fan retractors as blunt dissectors, the soft tissue underlying the parietal peritoneum can be swept laterally to bilaterally expose the anterior L5-S2 disc annulus. The sacral artery and vein coursing the disc are individually ligated with hemoclips and transected. A dissector can be used to remove residual soft tissue over the disc. Exposure is maintained with the left fan retractor in place holding the colon out of the way. It has been found that usually the right side does not require retraction, so a suction irrigation catheter can be used through this port.

In one specific procedure for the L4-L5 disc, the posterior peritoneum is incised more proximally about 3 centimeters. Again, the left fan is used to retract the colon laterally and with careful blunt dissection the aorta is exposed anteriorly at the bifurcation. The L4-L5 disc is usually right below this point. Left lateral dissection is carried out over the left common iliac vein and artery, gently retracting these vessels to the right. In order to retract these vessels enough to the right for adequate disc exposure the ascending segmental vein branch must be identified and transected. Once this vessel is cut, the artery and vein can then be bluntly retracted to the right with a fan or loop retractor to expose a significant amount of the L4-L5 disc for fusion.

Once the subject disc is exposed, it can be important to align the abdominal entry operating trocar port site **145** with the disc to be fused so that the operating trocar is parallel with the endplates of the disc in the sagittal plane. The entry point is estimated and a small Steinmann pin can be placed either in the interspace or along the patient and checked with lateral C-arm and adjusted accordingly. A 1.5 to 2.5 centimeter incision can be made for placement of the operating trocar. A blunt introducer is placed in the abdomen and an 18 mm working trocar **147** (FIG. **14**) can be placed over it under endoscopic visualization.

In accordance with a further aspect of the present embodiment of the surgical technique, the annular of the subject disc **D** is marked for bilateral placement of a pair of fusion devices. For example, as shown in FIG. **14**, a working trocar **147** is

situated within the working port **145** (see FIG. **13**). The bilateral marks can be made with a template **150**, as shown in general in FIG. **14** and in more detail in FIG. **15**. Greater detail concerning this template and its method of use can be found in U.S. Pat. No. 5,645,549, issued on Jul. 8, 1997. The description of this template in this co-pending application is incorporated herein by reference.

For convenience, a brief description of the template will be made with specific reference to FIG. **15**. In particular, the template **150** includes tubular body **151** and an elongated guide foot **152** that is pivotable connected to the end **153** of the tubular body. A guide wire or stylet **155** extends through the tubular body to pivot the foot **152** to the side. The sharp tip **156** of the stylet can then be used to pierce the disc annulus D. Using a mallet, the template can be secured to the center of the disc space by driving the stylet **156** into the disc tangential to the curvature of the annulus and parallel to the endplates. The template can then be slide down the guide wire or stylet until the foot **152** contacts the disc annulus.

The foot includes an opening **157** through which an electrocautery device **160** can extend. The tip **161** of the electrocautery device is guided through the opening **157** in the foot **152** to contact the disc annulus D. When the tip **161** is energized, it leaves a mark MR that is lateral to the center of the subject disc. The template **150** can then be rotated in the direction of the arrow T so that the foot is situated laterally opposite the first mark MR. At that point, the electrocautery device can be used to make a second mark ML providing the bilateral positions for the two fusion devices.

Once the bilateral marks MR, ML have been made on the disc annulus, the surgeon has a visual indication as to the proper location for placement of the fusion device. Under direct visualization of the insufflated abdominal region by way of a laparoscope through port **141** (FIG. **13**), the surgeon can then direct a T-handle probe **160** through the working port **147** to the either of the cauterization marks MR and ML (FIG. **16**). The T-handle probe **160** includes a sharp tip **161** that is used to break through the disc annulus. The T-handle allows the surgeon to rotate the probe **160** as necessary to facilitate penetration into the annulus. Once an initial opening has been made in the disc annulus by way of the T-handle probe **160**, a T-handle trephine **165** can be used to create pilot holes for subsequent instrumentation. The T-handle trephine **165** can include a series of marking **166** at 5 mm increments to control the depth of insertion of the trephine into the disc space, as shown in FIG. **17**. The markings **166** are compared to the working trocar **147** to gauge the depth of the cutting edge of the trephine, and therefore the depth of the prepared bore in the disc space and vertebral endplates. Again, the T-handle of the trephine allows the surgeon to rotate the trephine **165**. This procedure is repeated at both of the electrocautery marks ML and MR. At this point, the surgeon has two bilateral holes to use for orientation during the remainder of the procedure. The trephine **165** is also preferably used to core into the disc space to form bilateral bores. A rongeur may be used to clear disc material from each of the bilateral bores in the disc.

In accordance with further steps of the present inventive method, a distractor **167** is advanced through the working trocar **147** as shown in FIG. **18**. The distractor has a distractor tip **169** that is selected according to the vertebral level being instrumented. For instance, distractors for a 16 mm size implant can be either 12 mm or 14 mm in width to maintain the disc space at its proper anatomical height. The tip **169** is removably attached to a distractor shaft **168**. Preferably, progressively larger distractor tips are sequentially inserted in alternating fashion into each of the bilateral holes in the disc space and annulus until the annulus is taut and the adjacent

vertebrae are adequately distracted for restoration of a proper disc space height. In one aspect of the invention, the distractor tips **169**, once they are disposed in their bilateral positions, will acts as a centering point or alignment guide for use of the instruments throughout the remainder of the procedure. It is therefore important that the distractor tips **169** be properly located, which can be accurately confirmed with fluoroscopy.

Once the bilateral distractor tips have been properly seated, a shaft extension (not shown) can be engaged to distractor shaft **168**. At this point, in accordance with the preferred embodiment, the disposable trocar **147** is removed and a laparoscope **170** is introduced through the port **145** in the skin and into the disc space, using the distractor shaft and distractor tip as a positioning guide. In accordance with one embodiment of the present invention, the laparoscope **170** includes an outer sleeve **171** having a first end **172** and a second end **173**, as shown in FIG. **19**. The second end **173** is engaged to a laparoscopic port **180** which can be of conventional design. In particular, the laparoscopic port **180** can include a bore **184** (FIG. **20(a)**) extending therethrough and in communication with the interior of the hollow outer sleeve **171**. This bore **184** in the laparoscopic port allows introduction of instruments through the port and into the outer sleeve **171**. The bore is preferably closed by a number of seals **182**, which are configured to accept cylindrical tools and instruments there-through while maintaining tight sealed engagement about the instrument.

The laparoscopic port **180** also preferably includes a trumpet valve **183**, which can be of conventional design. Specifically, the trumpet valve **183** maintains the laparoscopic port **180** in a normally closed position in which its internal bore is closed from communication with the outer sleeve **171**. However, once a instrument is introduced into the port **180** through the seals **182**, the trumpet valve **183** moves aside to allow passage of the instrument or tool into the sleeve **171**.

In a further unique aspect of the invention, the end **172** of the outer sleeve **171** includes a pair of opposite distraction extensions or fingers **173**. These distraction fingers **173** are sized according to the height of the particular disc space. Specifically, the fingers **173** are intended to maintain the spacing between the adjacent vertebrae during subsequent steps of the procedure after the distractor tip **169** has been removed. Thus, the width of the fingers **173** can be varied depending upon the particular vertebral level being instrumented. In addition, the distraction fingers **173** can be tapered to conform to a normal angle between adjacent vertebrae at the instrumented level. The position of the fingers **173** is correlated with the position of the distractor tips within the bilateral bores in the disc space by aligning the fingers **173** with the trumpet valve **183** when the port **180** is engaged to the outer sleeve **171**. When the laparoscope **170** is inserted, the trumpet valves provide a visual indication of the alignment of the fingers. In other words, when the trumpet valve **183** is lateral to the midline, the fingers **173** are properly oriented between the vertebral endplates.

In one specific embodiment, the outer sleeve **171** can include opposite spikes **174** disposed between the distraction fingers **173**. These spikes are preferably configured to penetrate at least partially into the adjacent vertebral bodies, to help maintain the position of the outer sleeve **171** at the surgical site. In some instances, the outer sleeve **171** does not include the teeth **174**. For example, where the procedure is to implant a tapered fusion device, the teeth **174** are preferably eliminated and where the device is a uniform cylinder, the teeth can be retained.

In one embodiment of the present surgical method, the laparoscope **170** can be directly inserted over the distractor

shaft extension (not shown). However, it is believed that the distraction fingers 173 and the spikes 172 can cause trauma to the skin during entry and to the soft tissue surrounding the surgical site during introduction of the laparoscope 170. Thus, a further feature of the preferred embodiment includes a switching sleeve 190, as shown in FIGS. 20(a), (b). The switching sleeve 190 has a length sufficient to span the entire length of the laparoscope 170 from the port seals 182 to the end 172 of the outer sleeve 171. In particular, the switching sleeve 190 has a tapered tip 191 configured to extend beyond the end 172 of the outer sleeve 171, and more particularly beyond the ends of the fingers 173. The switching sleeve 190 also includes a flared tip 192 at its opposite end that is enlarged to prevent its passage through the laparoscopic port 180 and particularly the seals 182.

In accordance with a preferred embodiment of the inventive surgical procedure, the switching sleeve 190 is placed inside the laparoscope 170 prior to insertion into the patient. The switching sleeve 190 has an outer diameter nearly equal to the inner diameter of the outer sleeve 171 to slide in close running fit within the laparoscope 170. The laparoscope 170 and switching sleeve 190 can then be slide over the distractor shaft and with a twisting motion pass through the skin and fascia until the outer sleeve contacts the disc annulus. It is important to consider that the opposite fingers 173 on the outer sleeve 171 of the laparoscope must pass through the opening in the disc space and be aligned between the adjacent vertebrae. As the fingers 173 are pushed into the disc space, the switching sleeve 190 will remain outside the disc annulus as its tapered tip 191 contacts the annulus in the region between the distraction fingers 173 (see FIG. 20(b)). The outer sleeve 171 of the laparoscope 170 is properly oriented when the fingers 173 are correctly oriented between and contacting the adjacent vertebra endplates. The outer sleeve 171 is then seated by striking a driving cap (not shown) mounted on the laparoscopic port, to thereby drive the fingers 173 fully into the disc space between the vertebral endplates and to drive the spikes 174 into the adjacent vertebrae.

With the laparoscope 170 in place, all of the remaining steps of this inventive technique occur under a relatively protected or sealed environment. Specifically, the outer sleeve 171 of the laparoscope provides a sealed passageway from the bilateral bores at locations MR and ML on the disc to the laparoscopic port 180 outside the patient. The laparoscope 170 can be used as a passageway to provide irrigation and aspiration where necessary, without the risk of fluids leaking into the space adjacent the operative site. Moreover, the sealed working channel to the prepared sites in the disc space prevent leakage of abdominal distension fluids into the working channel and disc space. This latter aspect allows direct vision of the surgical site outside the working channel created by the laparoscope.

With the laparoscope 170 in position, the distractor shaft 168 is removed as well as the distractor tip 169 that is disposed between the adjacent vertebrae. Since the fingers 173 of the laparoscope outer sleeve 171 will maintain the spacing between the adjacent vertebrae, the distractor tip is being removed from the disc space to prevent dislodgment of the outer sleeve. In a bilateral procedure, the bilateral bores in the disc each contain a distractor tip. In the preferred method, the right left bore remains in place. Thus, the fingers 173 of the laparoscope engaged within one of the bilateral locations share the distraction load with a distractor tip 169 disposed within the other bilateral location. When the right side is instrumented with a fusion device, as described below, the fingers 173 will be within the left bore in the disc and will share the distraction load with the fusion device.

With the distraction tip removed and the disc space supported by the fingers 173, the next step in the inventive method is the preparation of the vertebral end plates and disc to provide a site for insertion of a fusion device. The switching sleeve 190 is first removed and, in accordance with one aspect of the invention, a reaming sleeve 195 is advanced through the laparoscope 170. As shown in FIG. 21, the reaming sleeve 195 includes spikes 196 that are adapted to penetrate the adjacent vertebral bodies to hold the reaming sleeve in place. One object of the reaming sleeve in this embodiment is to help maintain the position of the laparoscope while the disc material and vertebral end plates are being reamed. This object is of particular importance when the laparoscope outer sleeve 171 does not include the teeth 174. In addition, the spikes 195 on the reaming sleeve 195 will prevent the vertebral bodies from being pushed away or distracted while reaming, since the force generated by the reamer can have a tendency to drive the vertebral bodies apart. This force is particularly present when a tapered fusion device is to be implanted, necessitating cutting conical threads into the vertebra.

In accordance with the invention, an adjustable reamer 197 is extended through the reaming sleeve 195. The reamer 197 can be of conventional design with a cutting surface configured to evacuate the disc space and prepare the adjacent vertebral bodies to receive a threaded implant. The reamer 197 includes an adjustable depth stop 198 disposed adjacent the laparoscopic port 180. The depth stop 198 contacts the seals 182 of the port to prevent introduction of the reamer 197 too deeply into the disc space. The depth of reaming necessary, and consequently the position of the depth stop 198, can be determined prior to this reaming step by review of fluoroscopic images.

The reamer 197 is manually operated by way of a T-handle 199 to successively remove disc tissue and bone from the adjacent vertebral bodies to provide a prepared bore for the fusion implant. Preferably, several passes will be made with the reamer, after which the outer sleeve will be examined visually and fluoroscopically to verify that it remains fully seated within the disc space. In addition, the reaming should be observed under C-arm imaging to prevent reaming into the spinal canal. Preferably, the depth stop 198 will be set at an initial drilling depth less than the anticipated full depth for implant insertion. For example, for an L5-S1 fusion, a 20 mm deep reamed bore may be prepared for a 26 mm long implant.

After the disc material and vertebral bodies have been reamed by the reamer 197, one prepared site is available for insertion of the fusion implant at the right location MR. It is then necessary to prepare the other bilateral location previously marked using the template 150 (location ML in FIG. 15). In the next steps of the inventive method, the reamer 197 is withdrawn as well as the reaming sleeve 195. The laparoscope 170 is then unseated in a controlled manner so that the fingers 174 are disengaged from between the vertebrae and withdrawn through the opening of the disc annulus. However, the laparoscope 170, and particularly the outer sleeve 171, is not removed from the skin after unseating from the disc space. Instead, the outer sleeve is reoriented over the second bilateral location ML (see FIG. 15). Preferably, immediately after the outer sleeve 171 is disengaged from the disc annulus, the switching sleeve 190 is extended back through the outer sleeve 171 so that the tapered end 191 of the sleeve extends beyond the fingers 173. The switching sleeve will then protect the soft tissue surrounding the instrumented disc space as the outer sleeve 171 is repositioned over the second bilateral location ML.

With the laparoscope 170 oriented over the second location ML and with the switching sleeve 190 contacting the disc

annulus, a distractor tip **169** attached to a distractor shaft **168** is extended through the outer sleeve **171**. In the preferred technique, the laparoscope is not yet fully seated at this location ML. The distractor tip **169** is advanced through the bore within the disc and anchored between the adjacent vertebral end plates. The laparoscope **170**, and particularly the outer sleeve **171**, is reseated within the disc space in the manner described above, namely with the distraction fingers **173** disposed between the vertebral end plates. Once the position of the outer sleeve and fingers **173** is confirmed using fluoroscopy, the remaining steps for preparing the vertebral bodies to receive the fusion implant are repeated at the left location ML.

Once the second bore in the disc space has been prepared, the following steps of the technique involve insertion of the implant. In accordance with the present invention, the implant can be a fusion cage of the type shown in FIG. 1 which is tapered to restore the normal curvature at the particular vertebral level. In the case of a fusion cage of the type shown in FIG. 1, the implant driver **50** can be used to implant the device **10**. The implant drive **50** can be substantially as depicted in FIG. 2 and can engage the implant **10** as shown in FIG. 3. In accordance with the present technique, the implant drive **50** can be engaged by a T-handle assembly **200**, as shown in FIG. 22. The T-handle assembly **200** includes a collet **201** which engages the end of the implant drive **50** opposite the gripping tongs **54**. The assembly **200** also includes T-handle **202** which is aligned with the gripping tongs **54** so that the surgeon has a visual indication of the orientation of the tongs **54** when the implant driver **560** is extended through the laparoscope **170**.

In accordance with the preferred technique, the implant drive **50** carrying the fusion device **10** is inserted through the laparoscopic port **180** and through the outer sleeve **171** until the implant **10** contacts the prepared bore within the disc space. At that point, the implant drive **50** can be rotated using the T-handle **202** to thread the implant into the prepared bore. The implant driver **50** can preferably include a plurality of depth markings on the driver shaft **51** beneath the collet **201** to give the surgeon the visual indication of the depth of insertion of the implant **10** into the prepared bore. Once the implant has been screwed in to its predetermined depth, as indicated by the depth markings on the implant drive shaft **51**, insertion of the implant should be halted with the T-handle **202** parallel to the vertebral end plates. With this orientation of the T-handle **202**, the tongs **54** of the implant drive **50** will be exposed to the disc space, rather than in contact with the vertebral bone. Consequently, then the long slots **27** (see FIG. 1) of the fusion device **10** will be directly exposed to and in contact with the vertebral bodies.

With a fusion device **10** implanted within the left location ML, the implant driver is removed from the implant and the laparoscope **170** is unseated from the left bilateral location. Again, the laparoscope **170** is not removed from the skin after unseating, but is simply moved to the next bilateral location MR, preferably with the switching sleeve **190** protecting the surrounding tissue from the distraction fingers **173** of the laparoscope. At this location, the same steps are repeated to implant a second fusion device **10** at this right location.

When each of the implant devices **10** is bilaterally implanted within the disc space, the position of the implants should be confirmed. In some instances, it may be necessary to reposition an implant within the disc space, such as by driving it further into the disc space. In this instance, the driving attachment **120** can be engaged to the implant drive **50** and the attachment **120** engaged with the implanted device **10** to permit additional manipulation of the device.

In switching between the left location RL and the right location MR, it is preferred that the implant drive **50** be fully

removed from the laparoscope **170** and the switching sleeve **190** extended through the outer sleeve **171**. Also, the distractor tip **169** attached to the distractor shaft **168** should then be extended through the switching sleeve **170** and the distractor tip can be used to locate the previous bore at the right location MR. Once the distractor tip **169** is situated within the bore, the outer sleeve **171** can be seated at the right most location in the disc space. With the outer sleeve **171** properly seated, the distractor shaft can be removed to make way for the implant drive **50** carrying a new implant fusion device **10**. Of course, the switching sleeve is removed prior to extending the implant and implant drive through the outer sleeve **171**.

Once both fusion devices are disposed in their bilateral positions at location ML and MR, an A-P radiograph can be taken to assure proper placement. In addition, where possible, it is preferred that additional bone graft material is packed around the implants in situ to further facilitate fusion.

As discussed above, the fusion device **10** includes a hollow opening **15** to receive bone growth material. In one specific embodiment, this bone growth material can include autogenous bone harvested from the patient's anterior iliac crest. Autograft bone from other locations, autologous bone, allograft, bone growth substitutes or other bone material capable of promoting or inducing bone ingrowth can be loaded into the implant. In the preferred technique, the interior **15** of each fusion implant **10** is filled prior to insertion of the implant into the disc space.

To facilitate this "pre-loading" of the fusion material, an implant holder **210** is provided in accordance with the invention (FIG. 23). This holder **210** includes a base **211** that includes a fixed clamp section **212** and a movable clamp section **215**. The fixed clamp section **212** includes a flange **213** projecting from the base **211**. The movable clamp section includes an impactor plate **216** that slides within a groove **217** formed in the base **211**. The impactor plate **216** is connected by a threaded shaft **218** to a knob **219**. The threaded shaft is rotationally supported by an upstanding flange **221** attached to base **211**. The upstanding flange **221** includes a threaded bore (not shown) through which the threaded shaft **218** extends. As the knob **219** is rotated, the shaft rotates within the threaded bore of the flange **221** to move the impactor plate **216** forward toward the fixed clamp half **212**.

In accordance with the present embodiment, a pair of blocks **225** and **226** are provided which are disposed adjacent a corresponding one of clamp sections **212** and **215**. The blocks **225** and **227** include implant engagement surfaces **226** and **228** which are configured to match the outer shape of the implant at its large slots **27**. These blocks, therefore, serve to close off the slots **27** as bone growth material is packed into the opening **15** of the implant **10**. In one specific embodiment, the blocks **225** and **227** are formed of plastic to effectively seal the large openings **27** in the sides of the implant **10**. Once the bone growth material has been tightly compacted within the implant device **10**, the knob **219** can be rotated in the opposite direction to release the movable clamp **216** from the device **10**.

In accordance with another aspect of the present invention, the laparoscope **170** can be used to implant a bone dowel **240**, as depicted in FIG. 24. The bone dowel **240** can be of a variety of configurations, such as an allograft Crock dowel, autograft tricortical or button dowels, manufactured composite dowels or hybrid dowels (e.g., an autogeneous button combined with allograft Crock dowel). While it is preferable that the bone dowel **240** be cylindrical, this configuration is not essential to the invention, provided the dowel is configured to pass easily through the outer sleeve **171** of the laparoscope.



In accordance with this embodiments, the disc space and adjacent vertebral bodies are prepared as described above (see, FIGS. 13-21 and accompanying text). In the preferred technique for implanting a bone dowel, the reamer 197 is used to create a partially cylindrical cut in the vertebral endplates to receive a cylindrical dowel. Alternatively, if a non-cylindrical dowel is used, the endplates can be prepared accordingly. It is understood that the dowel will typically have a uniform outer diameter or width corresponding to the disc space height. Unlike the fusion device 10 discussed above the bone dowel is not tapered; however, preparation of the vertebral bodies with the tapered distraction fingers 173 of the outer sleeve 171 providing an appropriate angle will allow the implanted bone dowel to retain this angle.

Once the disc space and vertebral endplates have been prepared to receive the dowel, the bone dowel 240 is dropped into the laparoscope through outer sleeve 171. Due to the precise fit between the bone dowel and the vertebral endplates, resistance will be experienced during insertion of the dowel. An impactor 245 is provided to drive the dowel into its prepared site. The impactor includes an impactor head 246 that is preferably threaded engaged to an impactor shaft 247. The head and shaft are sized for a close running fit through the outer sleeve 171. Preferably, the impactor head 246 can be provided to be implanted. Also preferably, the impactor shaft 247 will have a smaller diameter so that it can be used with impactor heads and outer sleeves of several diameters.

The impactor shaft 247 includes a driving cap 248 that can be stricken by a hammer or similar tool to drive the bone dowel into the prepared site in a controlled manner. Preferably, the impactor shaft also includes a series of depth markings 249 corresponding to the depth of insertion of the bone dowel 240 into the disc space. The final position of the dowel can be verified later by A-P radiograph. The second bone dowel can be inserted in a similar manner and additional bone graft placed between the bilateral bone dowels.

The present invention involves instruments and surgical techniques usable at any level of the spine. For simplicity, the above discussion has focused on fusion of the L5-S1 disc space. The dimensions of each of the components of the instruments would be sized appropriately for the specific vertebral level being instrumented. For example, the fusion devices 10 may be offered in several sizes, including 12 mm, 14 mm, and 16 mm. Based upon the size of the fusion implant, the trephine 165 can be provided in several sizes, such as trephines to form bores having a diameter of 6 mm, 8 mm or 10 mm.

The distractor tips 169 are also sized according to the size of the fusion device to be implanted. Preferably, the distractors are smaller than the fusion device. For example, for a 16 mm fusion device, the distractor tips 169 can be either 12 mm or 14 mm. For a 16 mm fusion device, a 16 mm reaming sleeve is provided to accept a 16 mm reamer to prepare a hole of the same diameter within the disc space and vertebral bodies. Smaller reamers and reaming sleeves would be provided for smaller fusion devices. As previously described, the outer sleeve 171 of the laparoscope 170 is preferably a 2 mm in diameter to readily accept all of the instruments and sleeves passing therethrough during the several steps of the inventive procedure.

In the surgical techniques described above in relation to FIGS. 13-21, an outer sleeve 171 is utilized which incorporated fingers 173 that served to maintain distraction of the intervertebral space. In addition, the prior illustrated technique utilizes a series of distractor tips 169 that are used to maintain distraction at one side of the disc space while a fusion device is implanted in the other bilateral location. A

further embodiment of the present invention provides an improvement to this technique. Specifically, this improvement resides in a distraction mechanism that is centrally disposed between the bilateral fusion device locations. This centralized distraction provides a more uniform distraction across the entire disc space than can be provided by a distractor tip, such as tip 169, situated at one side or the other of the intervertebral space.

In accordance with the embodiment of the invention shown in FIGS. 25-27, a distractor plug 290 is provided that includes an elongated stem 291 terminating at one end in a fan-shaped flange 292. The stem is sized to be maintained within the disc space. In one specific embodiment, the stem 291 has a length of about 22 mm. The flange 292 includes a forward facing bone contacting face 293 that is adapted to contact the vertebral bone in a manner disclosed herein. The elongated stem 291 includes opposite inwardly curved or concave walls 194. The curved walls 194 of the stem 291 merge into or are contiguous with opposite curved or concave edges 195 of the flange 292. In accordance with the present invention, these curved walls 294 and curved edges 295 are preferably sized to provide clearance for the outer diameter of various tools and instruments that might be advanced into the intervertebral disc space through an outer sleeve, such as the sleeve 171 described above. In a specific embodiment, these contiguous curved walls 194 and edges 195 are defined at a diameter of between 20 mm-29 mm.

The distractor plug 290 further includes a locking surface 297 at the top and bottom portions of the elongated stem 291 and intermediate between the opposite curved walls 294. These locking surfaces 297 can have a variety of configurations; however, in one specific embodiment, these locking surfaces 297 includes a series of ridges 298 that are adapted to provide a modest grip on the endplates of the adjacent vertebrae that will contact the elongated stem 291 of the distractor plug 290. In accordance with the invention, the elongated stem 291 has a height between the two locking surfaces 297 that approximates the distracted height of the disc space to be instrumented. In the case of a threaded fusion device, such as the device 250, this height of the elongated stem 291 will be less than the outer crest diameter of the threads of the fusion device 250. In a specific embodiment, the top and bottom locking surfaces 297 define an outer diameter of between 10 mm-14 mm.

The distractor sleeve 290 further includes a lower stop face 296 that is integral with the flange 292 but that is on the opposite side of the elongated stem 291 from the bone contacting face 293. The elongated stem 291 is hollow with a bore extending along its length, as shown in FIG. 26. The stem 291 defines a threaded bore 302 at the end adjacent the flange 292. The threaded bore merges into and communicates with a keyed bore 301 that is at the opposite end of the distractor plug 290. The opposite end of the stem 291 of the plug 290 forms a blunt nose 299 through which the keyed bore 301 exits. In the illustrated embodiment, the keyed bore 301 is square in configuration. Alternatively, the keyed bore can have a variety of shapes that permit a keyed interface with a similarly shaped spike extending through the bore 301.

In its use, the distractor plug 290 is configured to be pushed into the intervertebral disc space between adjacent vertebrae. The distractor plug 290 is particularly well suited to providing distraction in a disc space spanning a spondylolisthesis condition. In this condition, one of the vertebrae is anteriorly offset from an adjacent vertebrae. In the condition specifically illustrated in FIG. 28, the superior lower lumbar vertebrae L5 is offset from the inferior sacral vertebra S1. Thus, the



distractor plug **290** is advanced anteriorly into the disc space between the lumbar vertebra L5 and sacrum S1.

The blunt nose **299** first contacts the adjacent vertebrae and provides a smooth and steady distraction as the remainder of the plug, namely the elongated stem **291**, comes in contact with the endplates of the adjacent vertebrae. In order to drive the distractor plug **290** into this disc space, the present invention contemplates a plug driver **305**. While the plug driver **305** can have a variety of configurations, in its simplest form the driver **305** includes a threaded stem **306** projecting from an elongated bar **307**. A handle **308** is formed at an opposite end of the bar **307** to provide a gripping surface to push the plug driver **305** toward the instrumented disc space. The threaded stem **306** of the plug driver **305** is configured to engage the threaded bore **302** of the distractor plug **290**. Thus, the distractor plug **290** is first threaded onto the end of the plug driver **305** and then subsequently advanced anteriorly into the disc space between the adjacent vertebrae.

As a force **F** is applied to the distractor plug **290** through the plug driver **305**, the flange **292** is advanced toward the lumbar vertebra L5 until the bone contacting face **293** is in contact with the vertebra. At this point, further force **F** applied to the distractor plug **290** not only pushes the elongated stem **291** into the intervertebral space, but also pushes the lumbar vertebra L5 into its proper alignment with the sacrum S1.

As the distractor plug **290** is advanced further into the intervertebral space, the upper and lower locking surfaces **297**, and particularly the ridges **298**, grip the adjacent vertebral endplates to prevent retrograde expulsion of the distractor plug **290**. The locking surfaces **297** of the distractor plug **290** provide a sufficiently strong engagement between the vertebral endplates to also prevent restoration of the original spondylolisthesis condition. The distractor plug **290** is pushed further into the intervertebral space until the stop face **296** of the flange **292** contacts the inferior vertebra, in this case the sacrum S1. It is understood that this stop face **296** can have a variety of configurations depending upon the desired final orientation of the two vertebrae relative to each other. For instance, the flange **292** can be wider at the stop face **296** than at the bone contacting face **292** so that the anterior portion of the displaced vertebra still retains some anterior offset from the anterior portion of the properly positioned vertebra.

It is known that some threaded cages can permit a reduction of a spondylolisthesis condition, provided the condition is only a grade one. The distractor plug **290**, and particularly the locking surface **297** of the stem **291** and the flange **292**, permit reduction of higher grade spondylolisthesis conditions. The flange and locking surfaces reduce the risk of slippage between the inferior and superior vertebrae as the superior vertebra is reduced.

In an alternative embodiment, a distractor plug **310** is provided that does not include a flange, as in the case of the distractor plug **290** shown in FIG. **25**. Specifically, the distractor plug **310** shown in FIG. **20** includes an opposite curved or concave sidewall **311**, a blunt nose **312** and opposite locking surface **313**. Each of these features is substantially similar to the features of the distractor plug **290**. Likewise, the distractor plug **310** includes a stop face **314** that is adapted to contact the inferior vertebra during the reduction process. Finally, the distractor plug **310** is hollow and includes a threaded bore (not shown) and an integral keyed bore **315**.

With this embodiment, the primary reduction force is provided by the driver **316**, depicted in FIG. **30**. This driver includes a threaded stem **317** that is adapted to engage the threaded bore (not shown) in the distractor plug **310** of FIG. **29**. A driving flange **318** is formed so that the threaded stem

projects outward from the driving flange **318**. The driving flange **318** includes a bone contacting surface **319** that at least initially contacts only the end of the distractor plug **310** when the stem **317** is threaded into the plug. Once the driver **316** is used to push the distractor plug **310** in place, the bone contacting face **319** abuts the displaced vertebra and is used to transmit a force to reduce that vertebra.

As described above, the distractor plugs **290** and **310** first provide a means for reducing a spondylolisthesis condition. Once the vertebral offset has been reduced, the driving tools can be removed and the distractor plugs **290**, **310** left in position in the intervertebral disc space. At this point, a further feature of the distractor plugs comes into play. Specifically looking, for example, at the distractor plug **290**, the hollow stem **291**, and particularly the keyed bore **301** provides an interface for a percutaneous surgical sleeve. In one embodiment, such a sleeve **320** includes a tubular body **321** as shown in FIG. **31**. A distraction extension **322** is formed at one end of the tubular body **321**. This distraction extension preferably has a height that is comparable to the height of the elongated stem **291** so that the extension can assist in maintaining the distracted height of the intervertebral space.

Substantially 180 degrees opposite from the distraction extension **322** is a locating spike **323**. In the specific embodiment, the locating spike **323** integrally extends from the end of the tubular body **321** contiguous with the outer wall of the body. This locating spike **323** is configured to extend first through the threaded bore **302** and finally through the keyed bore **301** of the distractor plug **290**. The locating spike **323** preferably has a shape that conforms to the shape of the keyed bore **301**. In the specific embodiment, that shape is a square, although other configurations can be utilized that prevent relative rotation between the distractor plug **290** and the locating spike **323**. The locating spike is preferably long enough to extend through the entire stem **291** without projecting beyond the blunt end **299** of the distraction device.

The manner of use of the distractor plug and sleeve combination is shown in FIG. **32**. In particular, it can be seen that a distractor plug **290** is centrally located within the intervertebral disc space. The distractor plug **290** then serves as a locator of an anchor for the sleeve **320**. Specifically, the locating spike **323** projects into the distractor plug **290** into keyed engagement with the keyed bore **301**. As shown in FIG. **32**, the sleeve **320** is oriented to the right of the centrally disposed distractor plug **290** so that the distraction extension **322** provides outboard support for the distracted disc space. In this position, the sleeve **320** can then be used to perform the drilling and reaming operations previously described particularly in connection with FIG. **21**, as well as the step of inserting the fusion device as also described above. The curved wall **294** and curved edge **295** of the flange **292** provide clearance for insertion of the various cylindrical tools and cylindrical fusion device into the intervertebral space.

Once a fusion site has been prepared at the right side of the disc space, the sleeve **320** can be retracted, so that the locating spike **323** is pulled out of the keyed bore **301** of the distractor plug **290**. The sleeve **320** can then be rotated to the position shown in phantom in FIG. **32** with the tubular body **321** directed to the left of the intervertebral disc space. The same operations can be performed at this location in the intervertebral space. Using the distractor plug **290** and the sleeve **320**, the present invention provides a means to maintain midline distraction through the center line of the intervertebral disc space. Moreover, the distractor plug provides a constant fixed pivot point for the various operations involved in implanting an interbody fusion device.

In accordance with another embodiment of the invention, a sleeve 325 is provided as shown in FIG. 33. In this embodiment, the sleeve 25 includes a tubular body 326 that has a distraction extension 327 projecting from one side of one end of the sleeve. Unlike the sleeve 320, the sleeve 325 includes a separate outrigger spike 328 that is fixed to the tubular body by way of an engagement flange 329. It is understood that the outrigger spike 328 could be integrally formed with the tubular body 326 or connected to the body in some other fashion. Nevertheless, a primary feature of the sleeve 325 is that the spike 328 is disposed outside the diameter or outer wall of the tubular body 326. In this manner, the sleeve 325 and its hollow cannula opening can be offset further from the midline of the intervertebral disc space. Thus, interbody fusion devices, such as device 350, can be disposed farther outboard within that space using the sleeve 320.

In a further embodiment, a double-barrel sleeve 330 is provided. In this embodiment, two tubular bodies 331 and 332 are affixed at a joint 333. Each tubular body 331, 332 includes a respective distractor extension 334, 335. As with the other sleeve embodiments, the distractor extensions 334, 335 have a width that approximates the width of the distractor plug.

In this embodiment, a bore 336 is formed at the joint 333 between the two tubular bodies 331, 332. A spike, in the form of an elongated rod 337, is configured to extend through the bore 336. This spike can then engage a distractor plug, such as the distractor plug 310 shown in FIG. 34. With this double-barrel sleeve 330, there is no need to retract the sleeve, rotated to the bilateral position and re-dispose it within a distractor plug, as in the embodiment of FIG. 32. This double-barrel sleeve 330 provides an additional distractor extension, so that distraction is achieved not only at the midline location of the distractor plug 310, but also at the outboard positions of the distractor extensions 334, 335. Again, the distractor extensions are arranged together with the distractor plug so that various percutaneous operations can be occurring through the double-barrel sleeve of and in the intervertebral disc space.

One problem that faces many interbody fusion devices is the risk of backing out or retrograde expulsion of the device. In the case of push-in implants, the natural compressive forces achieved by the disc annulus in a distracted space can have a tendency to squeeze the fusion devices in a retrograde direction. These same forces, coupled with relative movement between the instrumented vertebrae, can also cause threaded fusion devices to slowly unthread. In accordance with the present invention, one embodiment of a fusion cage is provided that is designed to prevent this counter rotation of the fusion device. The fusion device 250 shown in FIG. 8 includes a pair of bone screws that are threaded into the adjacent vertebrae. These bone screws prevent the fusion device 250 from rotating within their prepared bores.

Another approach is presented in FIGS. 35-36. In this approach, bilaterally placed fusion devices are connected laterally across the disc space, thereby preventing each device from rotating. In a first embodiment shown in FIG. 35, a pair of fusion devices 350 are provided that include a hollow body 351 having a first end 352 and a second end 353. As with the fusion devices previously discussed, the devices 350 each include a hollow interior 355 and an end wall 356. The devices also include external threads 358 that are adapted to be threaded into a prepared bore in adjacent vertebrae.

In a deviation from the previously discussed fusion devices, the fusion device 350 includes a recess 360 formed in the end wall 356. A lateral groove 361 traverses the recess 360 and opens at the flat side walls 357 of the device 350. Each device also includes a threaded bore 363 centrally formed at

the base of the recess 360. When each fusion device 350 is placed bilaterally within an instrumented disc space, the devices are separated by some distance, as depicted in FIG. 35. This distance is spanned by a connector plate 365. The connector plate includes an elongate arm 366 having mating ends 367 formed at the ends of the arm. Each of the mating ends 367 defines an outer wall 368 that is generally configured to conform to the recesses 360 in each of the fusion devices 350. The elongate arm 366 is configured to rest within the groove 361 so that the connector plate 365 can span between and interconnect the two fusion devices 350.

The connector plate 365 is provided with a slot 369 at each of the mating ends 367. This slot is oriented directly above the threaded bore 363 in the end wall 356 of the fusion device 350. A locking screw 370 having a threaded stem 371 is provided that extends through each slot 369 and into the threaded bore 363. The locking screw 370 is then tightened into the bore to clamp the connector plate 365 to each of the interbody fusion devices 350. Thus, the presence of the connector plate 365 when disposed within the grooves 361 of the adjacent fusion devices, prevents each fusion device 350 from rotating when within the patient. The length of the connector plate 365 is dictated by the spacing of the fusion devices 350 within the disc space.

In an additional embodiment, a connector plate 375 is shown in FIG. 36. The connector plate includes an elongate arm 376 with mating ends 377, each element of which is similar to the like named elements of the connector plate 365. However, in an alternative configuration, the connector plate 375 includes an intermediate plate 379 that preferably projects perpendicularly outward from the elongate arm 376. The intermediate plate 379 is generally in the middle of the connector plate 375 and sized to sit between each of the fusion devices 350. In one specific embodiment, the intermediate plate 379 has a width that is sufficient so that the plate 379 is in contact with one side wall 357 of the adjacent devices 350.

In the illustrated embodiments, the focus has been on threaded fusion devices. However, it is understood that the present invention has utility in implanting non-threaded fusion devices, threaded and non-threaded spacers, and cylindrical or non-cylindrical devices or plugs.

In a further aspect of this embodiment, the intermediate plate 379 is provided with angled screw bores 380. In particular, these screw bores are angled so that a bone screw inserted through the bores can be driven upward into the vertebral endplates of the adjacent vertebrae. Preferably, the screw bores are oriented at an angle similar to the angle of the screw bores 268 of the fusion device 250. Thus, the connector plate 375 provides an additional degree of security to prevent retrograde expulsion of the interbody fusion device 350.

While the invention has been illustrated and described in detail in the drawings and foregoing description, the same is to be considered as illustrative and not restrictive in character, it being understood that only the preferred embodiment has been shown and described and that all changes and modifications that come within the spirit of the invention are desired to be protected.

What is claimed is:

1. A distraction device for distracting the disc space between adjacent vertebrae, comprising:

an elongated stem having a height corresponding to a desired height of distraction for the disc space, said stem having a first end and a second end defining a longitudinal axis therebetween and a length along said axis that is sized to be maintained within the disc space when said elongated stem is driven into the disc space; and

25

a flange at said first end projecting outward from said longitudinal axis of said stem, said flange having a bone contacting face for contacting at least one of the vertebrae when said stem is driven into the disc space and for transmitting a reduction force to the vertebra upon application of an external force to the distraction device; and wherein said elongated stem defines a bore extending between said first end and said second end, said bore including a keyed bore adjacent said second end, said keyed bore having a non-circular configuration for receiving a complementary-shaped portion of a tool therethrough, and wherein said bore includes a threaded bore adjacent said first end for receiving a threaded portion of a tool therein.

2. A distraction device for distracting the disc space between adjacent vertebrae, comprising:

an elongated stem having a height corresponding to a desired height of distraction for the disc space, said stem having a first end and a second end defining a longitudinal axis therebetween and a length along said axis that is sized to be maintained within the disc space when said elongated stem is driven into the disc space; and

a flange at said first end projecting outward from said longitudinal axis of said stem, said flange having a bone contacting face for contacting at least one of the vertebrae when said stem is driven into the disc space and for transmitting a reduction force to the vertebra upon application of an external force to the distraction device; and wherein said elongated stem has opposite top and bottom portions, said top and bottom portions having a bone engaging surface configured to resist expulsion of said elongated stem from the disc space, said elongated stem including side portions between said top and bottom portions, said side portions each defining an inwardly curved surface, said flange including inwardly curved side edges contiguous with said inwardly curved surface of a corresponding one of said side portions.

3. A distraction device for distracting the disc space between adjacent vertebrae, comprising:

an elongated stem having a height corresponding to a desired height of distraction for the disc space, said stem having a first end and a second end defining a longitudinal axis therebetween and a length along said axis that is sized to be maintained within the disc space when said elongated stem is driven into the disc space; and

a flange at said first end projecting outward from said longitudinal axis of said stem, said flange having a bone contacting face for contacting at least one of the vertebrae when said stem is driven into the disc space and for transmitting a reduction force to the vertebra upon application of an external force to the distraction device, wherein said flange is fan shaped including concave side edges and is substantially perpendicular to said longitudinal axis of said elongated stem; and

an elongated driver shaft extending generally along said longitudinal axis and sized to extend outside of the disc space for transmission of said external force to the distraction device.

4. The distraction device of claim 3, wherein said elongated stem includes opposite top and bottom surfaces configured to contact a superior and an inferior vertebra, respectively;

said flange projects from said stem in a direction toward the superior vertebra; and

the device includes a stop face at said first end of said stem projecting in a direction toward the inferior vertebra.

26

5. The distraction device according to claim 4, wherein said elongated stem defines a bore extending between said first end and said second end.

6. The distraction device according to claim 5, wherein said bore includes a threaded bore adjacent said first end for receiving a threaded portion of a tool therein.

7. The distraction device according to claim 4, wherein said top and bottom surfaces each comprise a bone engaging surface configured to resist expulsion of said elongated stem from the disc space.

8. The distraction device according to claim 7, wherein said bone engaging surface includes a plurality of ridges defined thereon.

9. A distraction device for distracting an intervertebral space between adjacent vertebrae, comprising:

a stem portion extending along a longitudinal axis and adapted for insertion within the intervertebral space, said stem portion having a first end, a second end, and upper and lower surfaces defining a height corresponding to a select distracted height of the intervertebral space and including side portions, each of said side portions defining a side surface having a concave curvature extending between said upper and lower surfaces; and

a transverse flange portion at said first end projecting outward from said longitudinal axis of said stem portion and having a bone side contacting face adapted to engage one side of the adjacent vertebrae when said stem portion is inserted into the intervertebral space to transmit an axial force to said one of the adjacent vertebrae.

10. The distraction device of claim 9, wherein said flange portion includes concave side edges, each of said concave side edges being contiguous with a corresponding one of said concave side surfaces of said side portions.

11. The distraction device of claim 9, further comprising: an elongated driver shaft extending generally along said axis and sized to extend outside of the intervertebral space, and wherein said elongated driver shaft is threadably engaged with said stem portion.

12. The distraction device of claim 9, wherein said stem portion is configured for selective engagement with a surgical instrument.

13. The distraction device of claim 9, wherein said stem portion is configured for selective engagement with a surgical instrument, one of said stem portion and said surgical instrument defining a passage, another of said stem portion and said surgical instrument defining a projection at least partially received within said passage to locate said surgical instrument relative to the adjacent vertebrae.

14. A distraction device for distracting an intervertebral space between adjacent vertebrae, comprising:

a stem portion extending along a longitudinal axis and adapted for insertion within the intervertebral space, said stem portion having a height corresponding to a select distracted height of the intervertebral space; and

a transverse flange portion having a fan-shaped configuration including concave side edges and a bone contacting face adapted to engage one of the adjacent vertebrae when said stem portion is inserted into the intervertebral space to transmit an axial force to said one of the adjacent vertebrae; and

an elongated driver shaft extending generally along said axis and sized to extend outside of the intervertebral space for application of an external force to the distraction device to transmit said axial force to said one of the adjacent vertebrae.

27

15. A method for performing a surgical procedure on adjacent vertebrae having a spondylolisthesis condition wherein one of the adjacent vertebrae is anteriorly offset relative to the other of the adjacent vertebrae, comprising:

providing a device including an axial stem portion, a transverse flange portion, and a transverse stop portion arranged generally opposite the transverse flange portion;

inserting the axial stem portion into an intervertebral space between the adjacent vertebrae;

engaging the transverse flange portion against one of the adjacent vertebrae and transmitting an axial reduction force to the anteriorly offset vertebra to reduce the spondylolisthesis condition; and

engaging the transverse stop portion against an opposite one of the adjacent vertebrae to limit the inserting.

16. The method of claim 15, wherein said stem portion includes top and bottom bone engaging surfaces configured to resist expulsion of said stem portion from the intervertebral space.

17. The method of claim 16, wherein said top and bottom bone engaging surfaces each define a plurality of ridges configured to resist expulsion of said stem portion from the intervertebral space.

18. The method of claim 15, wherein said transverse flange portion is formed integral with said stem portion and together define a single-piece, monolithic structure.

19. The method of claim 18, wherein said transverse stop portion is formed integral with said stem portion and together define a portion of said single-piece, monolithic structure.

20. The method of claim 15, further comprising:

providing the device with an elongated driver shaft extending in an axial direction and sized to extend outside of the intervertebral space; and

applying an external force to the elongated driver shaft resulting in the transmitting of the axial reduction force to the anteriorly offset vertebra to reduce the spondylolisthesis condition.

28

21. The method of claim 15, wherein said stem portion has a height corresponding to a select distracted height of the intervertebral space; and

wherein said stem portion includes a rounded leading end portion to facilitate insertion of said stem portion into the intervertebral space and distraction of the adjacent vertebrae, said stem portion having opposite top and bottom bone engaging surfaces with said height of said stem portion defined between said opposite top and bottom bone engaging surfaces; and

wherein said rounded leading end portion of said stem portion defines a curvature extending along said height between said opposite top and bottom bone engaging surfaces to facilitate insertion of said stem portion into the intervertebral space and distraction of the adjacent vertebrae.

22. A method for performing a surgical procedure on adjacent vertebrae having a spondylolisthesis condition wherein one of the adjacent vertebrae is anteriorly offset relative to the other of the adjacent vertebrae, comprising:

providing a device including an axial stem portion and a transverse flange portion, the axial stem portion configured for selective engagement with a surgical instrument;

inserting the axial stem portion into an intervertebral space between the adjacent vertebrae; and

engaging the transverse flange portion against one of the adjacent vertebrae and transmitting an axial reduction force to the anteriorly offset vertebra to reduce the spondylolisthesis condition;

selectively engaging the surgical instrument with the axial stem portion, the surgical instrument comprising a tubular sleeve; and

advancing a surgical device through the tubular sleeve toward the intervertebral space.

\* \* \* \* \*

UNITED STATES PATENT AND TRADEMARK OFFICE  
**CERTIFICATE OF CORRECTION**

PATENT NO. : 7,621,958 B2  
APPLICATION NO. : 10/763719  
DATED : November 24, 2009  
INVENTOR(S) : Zdeblick et al.

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:


On the Title Page:

The first or sole Notice should read --

Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 801 days.

Signed and Sealed this

Fourteenth Day of December, 2010

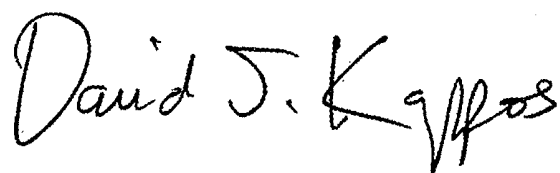A handwritten signature in black ink, reading "David J. Kappos". The signature is written in a cursive, flowing style with a large initial 'D' and 'K'.

David J. Kappos  
*Director of the United States Patent and Trademark Office*

专利名称(译)	椎体间融合的方法和仪器		
公开(公告)号	<a href="#">US7621958</a>	公开(公告)日	2009-11-24
申请号	US10/763719	申请日	2004-01-22
[标]申请(专利权)人(译)	ZDEBLICK THOMAS 麦加恩THOMAS		
申请(专利权)人(译)	ZDEBLICK THOMAS 麦加恩THOMAS		
当前申请(专利权)人(译)	华沙整形外科, INC.		
[标]发明人	ZDEBLICK THOMAS MCGAHAN THOMAS		
发明人	ZDEBLICK, THOMAS MCGAHAN, THOMAS		
IPC分类号	A61F2/44 A61B17/58 A61B1/00 A61B1/313 A61B17/00 A61B17/02 A61B17/16 A61B17/17 A61B17/28 A61B17/34 A61B17/70 A61B17/86 A61B17/88 A61B19/00 A61F2/00 A61F2/28 A61F2/30 A61F2/46		
CPC分类号	A61B1/3132 A61B17/025 A61B17/1671 A61B17/1757 A61B17/282 A61F2/446 A61F2/4601 A61F2/4611 A61B1/3135 A61F2230/0067 A61B17/7059 A61B17/86 A61B2017/00238 A61B2017/00261 A61B2017/0256 A61B2017/3488 A61B2019/5404 A61B2019/5437 A61F2/442 A61F2002/2835 A61F2002/2839 A61F2002/30123 A61F2002/30153 A61F2002/30179 A61F2002/3021 A61F2002/30217 A61F2002/30329 A61F2002/30433 A61F2002/30507 A61F2002/30604 A61F2002/30774 A61F2002/30777 A61F2002/30785 A61F2002/30787 A61F2002/30789 A61F2002/3082 A61F2002/30858 A61F2002/30863 A61F2002/30871 A61F2002/30874 A61F2002/4475 A61F2002/448 A61F2002/4627 A61F2002/4635 A61F2220/0025 A61F2220/0041 A61F2230/0006 A61F2230/0019 A61F2230/0058 A61B2090/3904 A61B2090/3937 A61F2002/30593 A61F2002/30873		
其他公开文献	US20040153089A1		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

#### 摘要(译)

提供了腹腔镜手术技术，用于制备用于植入新型融合装置或植入物的部位。根据本技术的一个实施例，提供了一种腹腔镜，其具有外套管，该外套管在一端具有牵引指状物以分散椎间盘空间。腹腔镜为椎间盘空间提供密封的工作通道，椎间盘空间通过该通道分散，椎骨终板和周围的椎间盘被扩孔，并且融合装置被插入。提供了一个牵引插头，用于使外套筒对中并提供盘空间的中线分开。在一个实施例中，融合装置包括穿过端壁和装置的上壁和下壁以与相邻椎骨接合的发散骨螺钉。在另一个实施例中，连接板接合以双向地定位融合装置，以防止旋转并防止装置从盘空间排出。

