



US009662131B2

(12) **United States Patent**
Omori et al.

(10) **Patent No.:** **US 9,662,131 B2**
(45) **Date of Patent:** **May 30, 2017**

(54) **MANIPULATOR FOR MEDICAL USE**

2017/00398; A61B 2017/0046; A61B
2017/291; A61B 2017/2912; A61B
2017/2913; A61B 2017/2919; A61B
2017/2924;

(75) Inventors: **Shigeru Omori**, Kanagawa-ken (JP);
Shuichi Uenohara, Fujinomiya (JP);
Makoto Jinno, Tokyo (JP)

(Continued)

(73) Assignee: **Karl Storz GmbH & Co. KG**,
Tuttlingen (DE)

(56) **References Cited**

U.S. PATENT DOCUMENTS

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 1167 days.

2,765,930 A * 10/1956 Greer et al. 414/7
4,782,833 A * 11/1988 Einhorn et al. 606/80
5,649,955 A * 7/1997 Hashimoto et al. 606/205
(Continued)

(21) Appl. No.: **11/939,287**

FOREIGN PATENT DOCUMENTS

(22) Filed: **Nov. 13, 2007**

DE 41 36 861 A1 5/1993
EP 0 677 275 A2 10/1995

(65) **Prior Publication Data**

US 2009/0112229 A1 Apr. 30, 2009

(Continued)

(30) **Foreign Application Priority Data**

Oct. 31, 2007 (JP) 2007-283313

OTHER PUBLICATIONS

Office Action mailed Sep. 19, 2011, in co-pending U.S. Appl. No.
12/261,829.

(Continued)

(51) **Int. Cl.**

A61B 17/29 (2006.01)
A61B 17/00 (2006.01)
A61B 34/00 (2016.01)

Primary Examiner — Ryan J Severson

(74) *Attorney, Agent, or Firm* — Whitmyer IP Group LLC

(52) **U.S. Cl.**

CPC **A61B 17/29** (2013.01); **A61B 34/70**
(2016.02); **A61B 34/71** (2016.02); **A61B**
2017/0046 (2013.01); **A61B 2017/00398**
(2013.01); **A61B 2017/2927** (2013.01);
(Continued)


(57) **ABSTRACT**

A medical manipulator comprises a distal end working unit including a gripper as an end effector, an operating unit for operating the distal end working unit, a coupling interconnecting the distal end working unit and the operating unit, and an attitude changing mechanism for changing an attitude of the distal end working unit. When the operating unit is operated by an operator, the end effector is mechanically operated by a transmitting member. The attitude changing mechanism is operated by a bending drive source and a rotational drive source, which are operated when the operating unit is operated by the operator.

(58) **Field of Classification Search**

CPC A61B 2019/2242; A61B 2019/2276; A61B
2017/2927; A61B 17/29; A61B 19/22;
A61B 2017/2939; A61B 2017/2929;
A61B 2017/2932; A61B 2917/2932;
A61B 17/2909; A61B 34/71; A61B

5 Claims, 57 Drawing Sheets

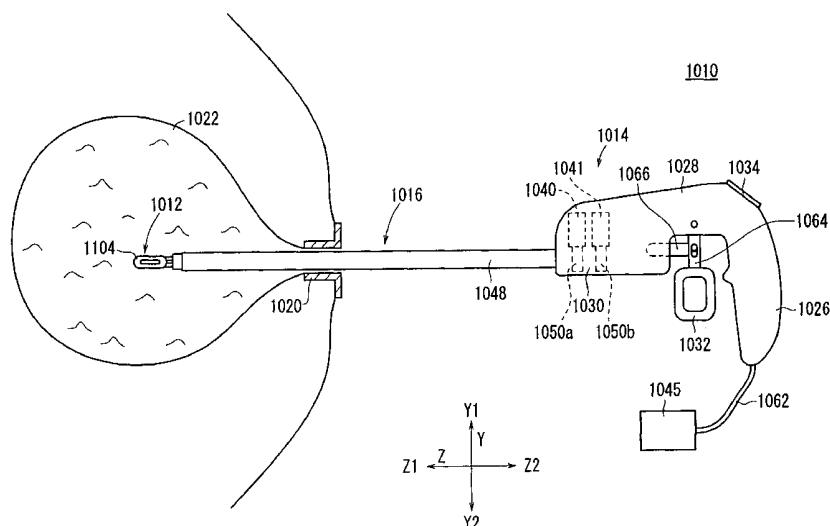

(52) U.S. Cl.

CPC A61B 2017/2929 (2013.01); A61B
2017/2932 (2013.01); A61B 2034/742
(2016.02)

(58) Field of Classification Search

CPC A61B 2017/2925; A61B 2017/2926; A61B
2017/293; A61B 2017/2931
USPC 606/205, 167, 170, 174, 206; 433/159;
901/31, 34, 36

See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

5,792,165 A * 8/1998 Klieman A61B 17/29
606/170
5,938,678 A * 8/1999 Zirps A61B 17/29
606/167
6,077,287 A * 6/2000 Taylor et al. 606/170
6,889,116 B2 * 5/2005 Jinno 700/245
2003/0236549 A1 12/2003 Bonadio et al.
2004/0266574 A1 12/2004 Jinno et al.
2005/0090809 A1 4/2005 Cooper et al.
2007/0208375 A1 9/2007 Nishizawa et al.
2009/0112230 A1 4/2009 Jinno

FOREIGN PATENT DOCUMENTS

EP	1 707 153 A1	10/2006
JP	63-176092 U	11/1988
JP	63-288147	11/1988
JP	8-33628	2/1996
JP	10-179601	7/1998
JP	2001-276091	10/2001
JP	2002-102248	4/2002
JP	2002-282257	10/2002
JP	2003-61969	3/2003
JP	2003-111765	4/2003
JP	3421117	4/2003
JP	2004-122286	4/2004
JP	2004-301275	10/2004
JP	2006-247804	9/2006

OTHER PUBLICATIONS

Office Action issued Dec. 18, 2012 in Japanese Application No. 2007-283313 (With Partial English Translation).
Japanese Office Action issued Apr. 24, 2012, in Patent Application No. 2007-283323 (with Partial English-language translation).
Office Action issued Apr. 16, 2013 in Japanese Application No. 2007-283313 (With Partial English Translation).

* cited by examiner

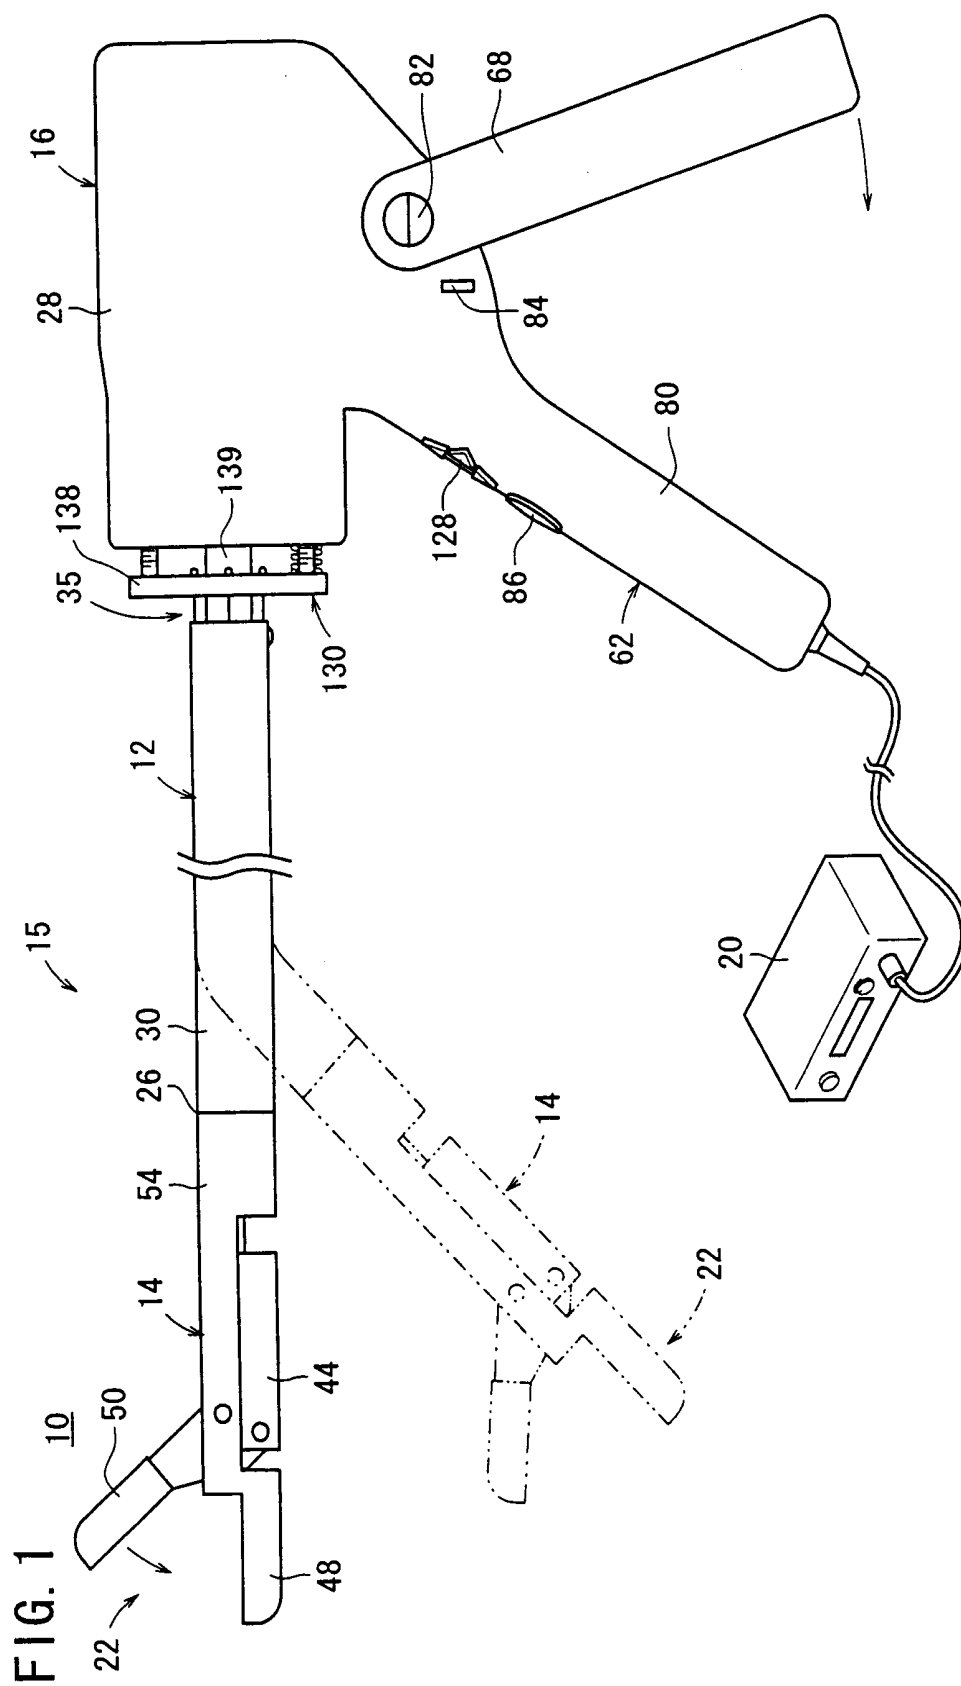


FIG. 2

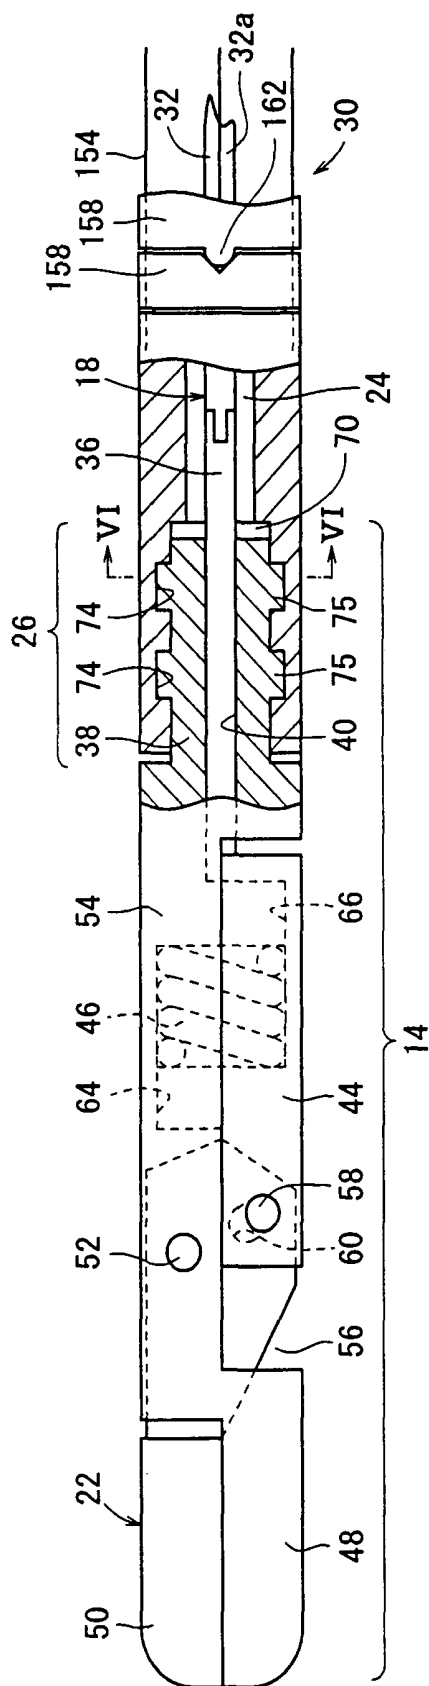


FIG. 3

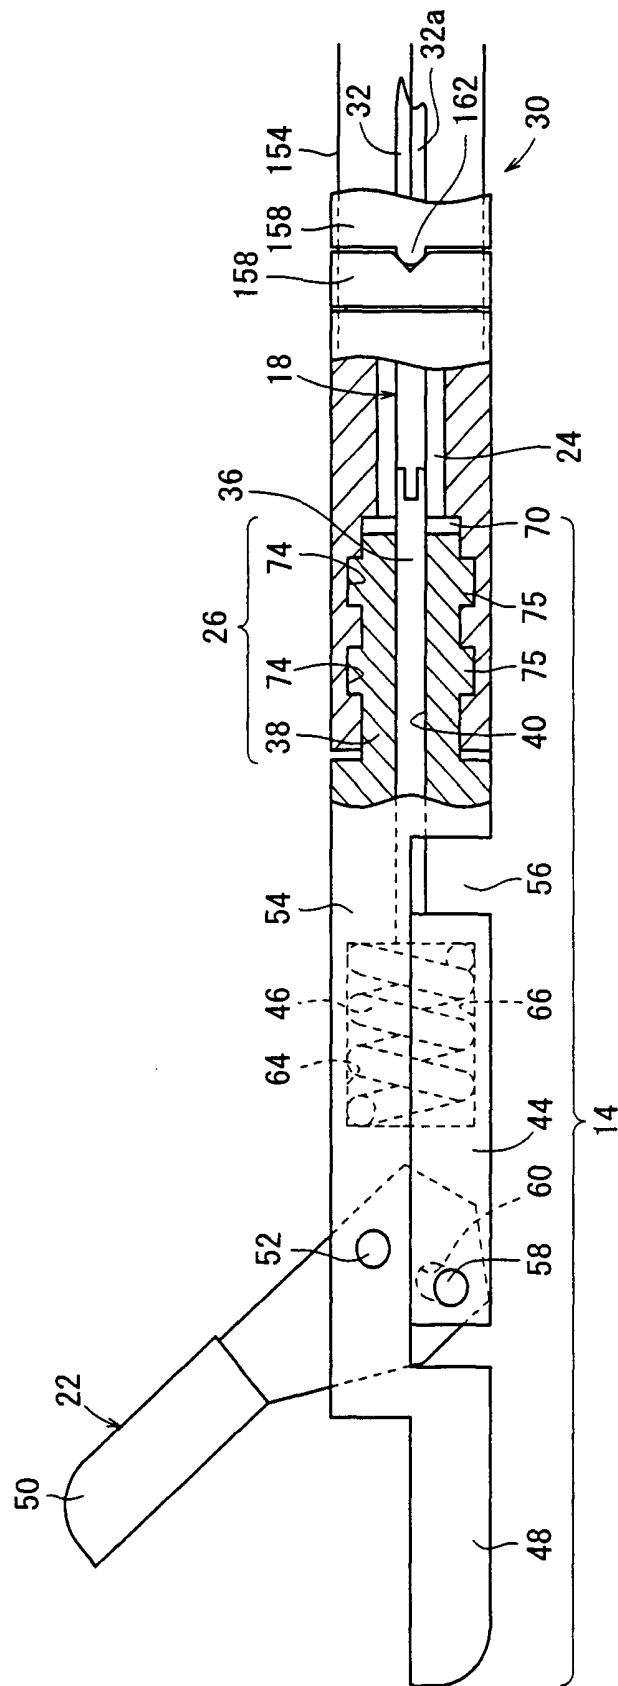


FIG. 4

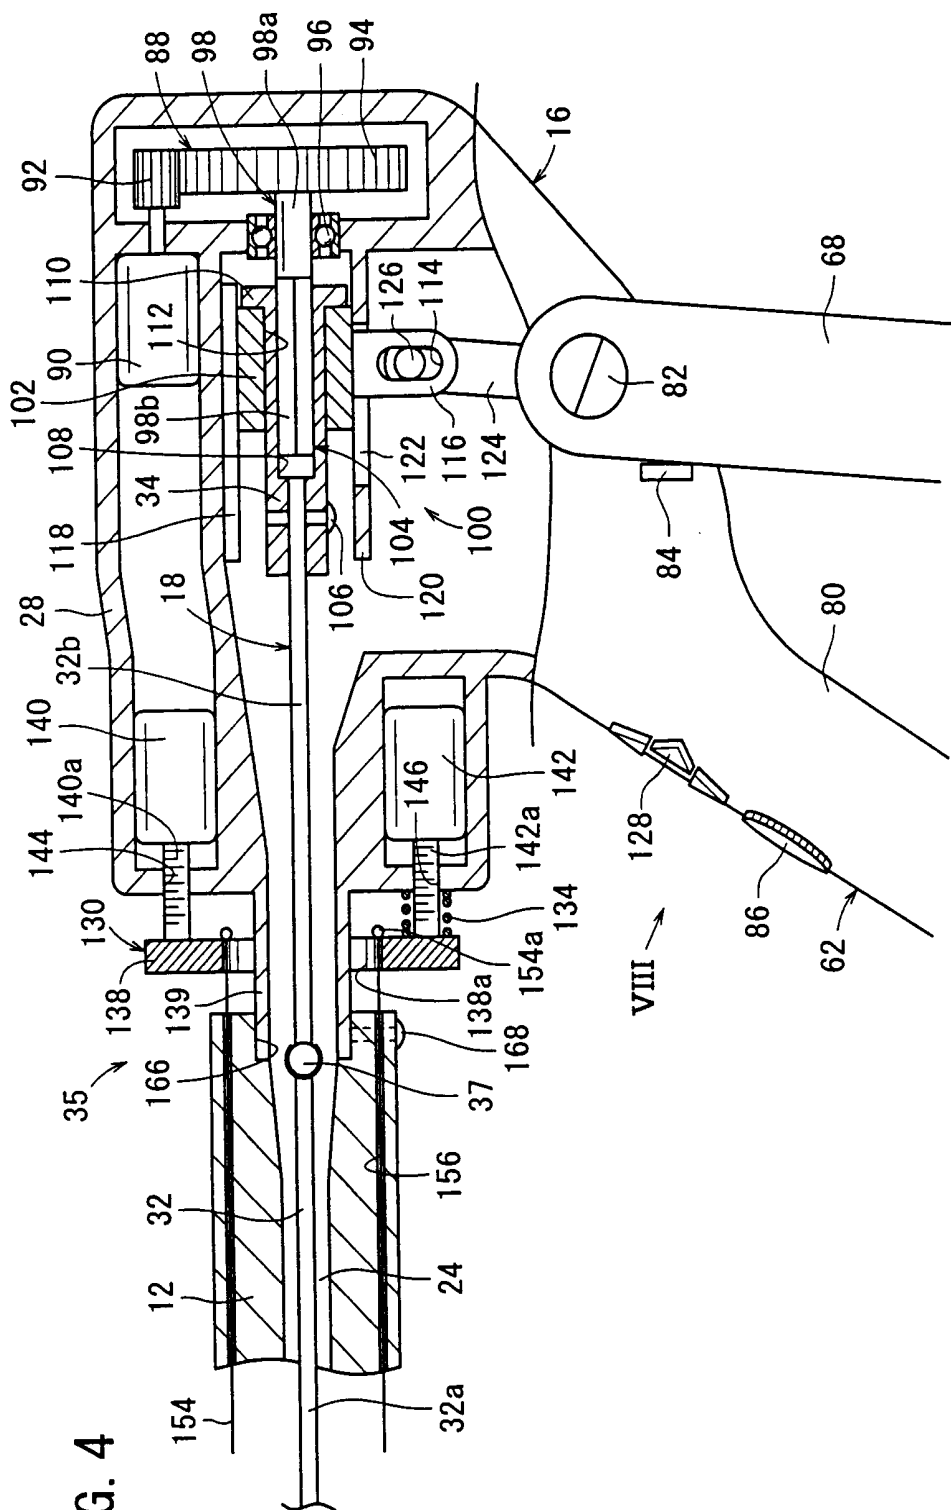


FIG. 5

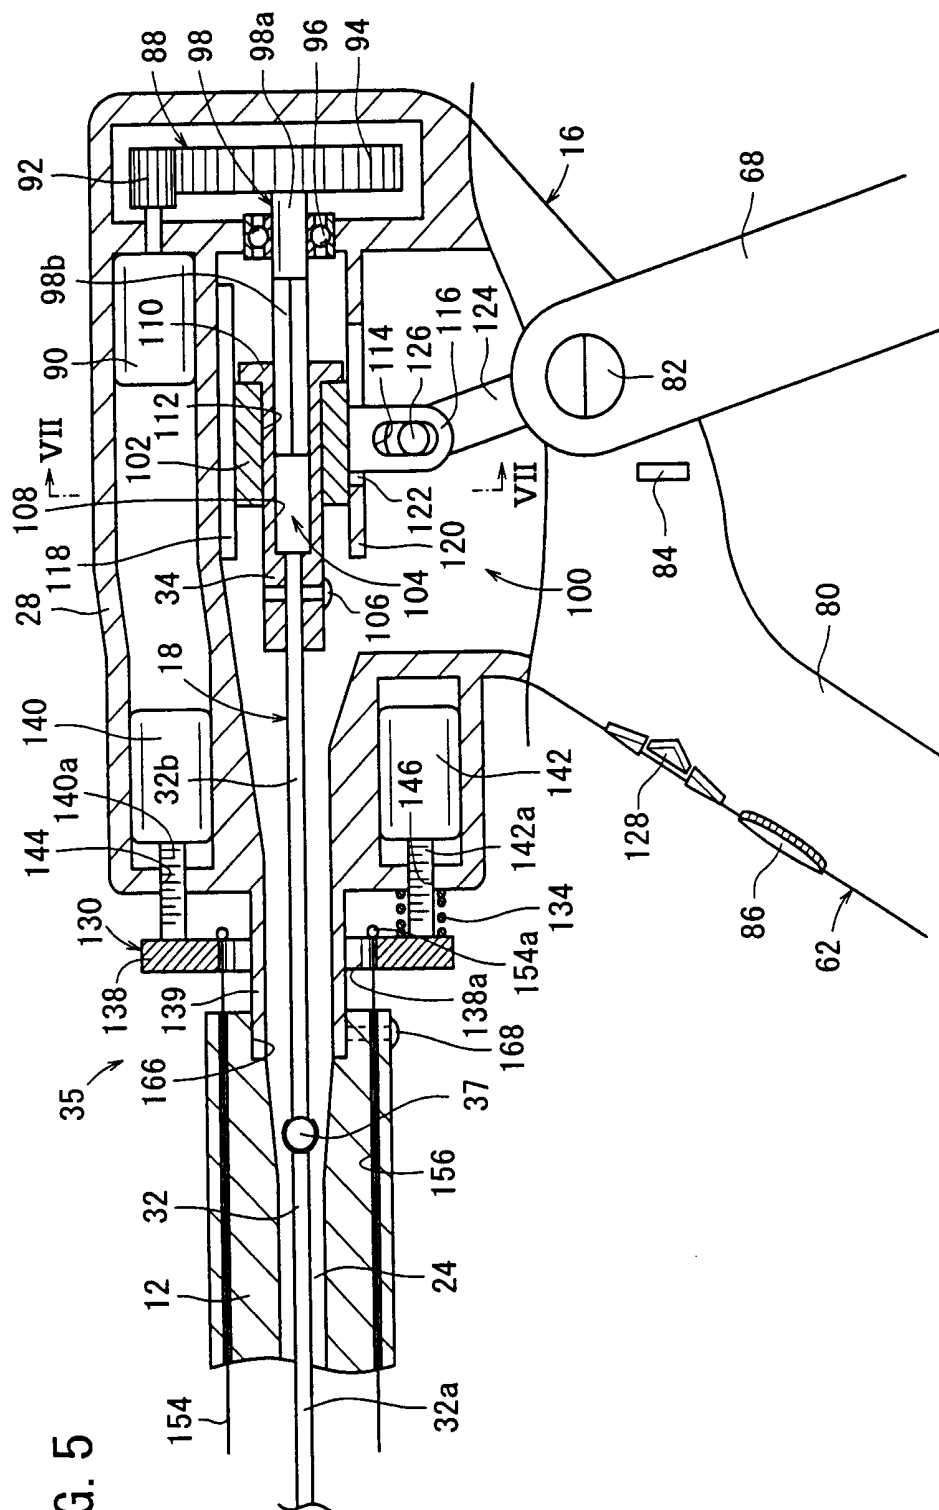


FIG. 6

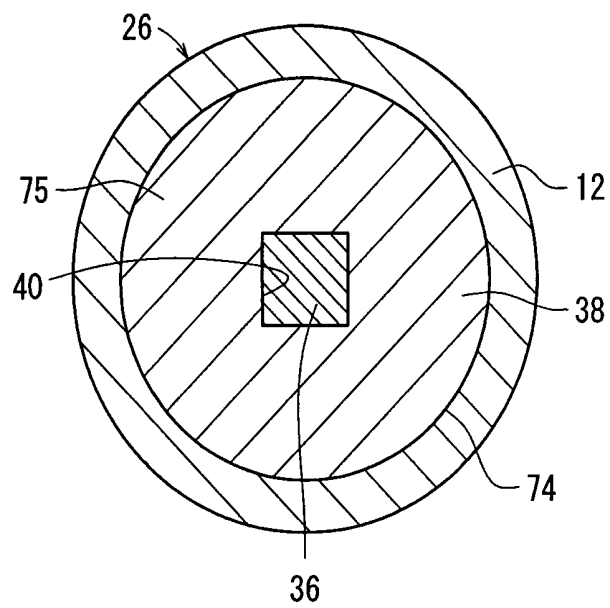


FIG. 7

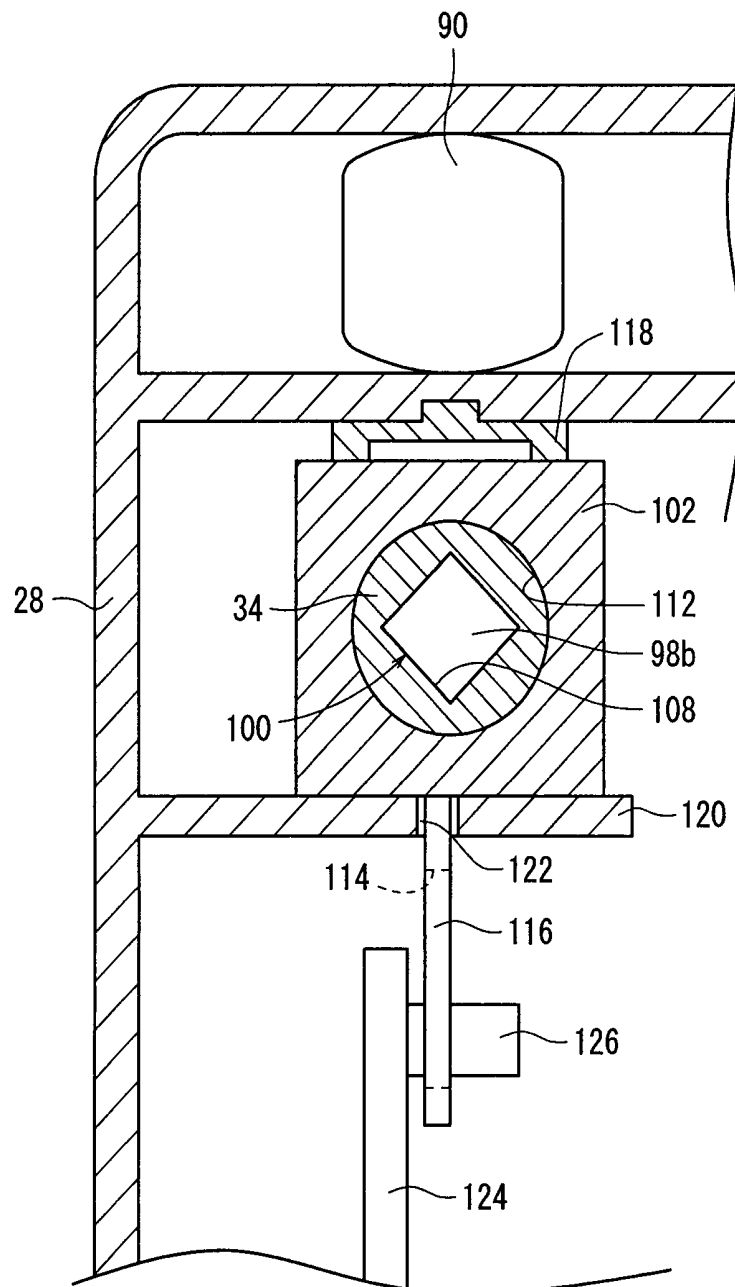
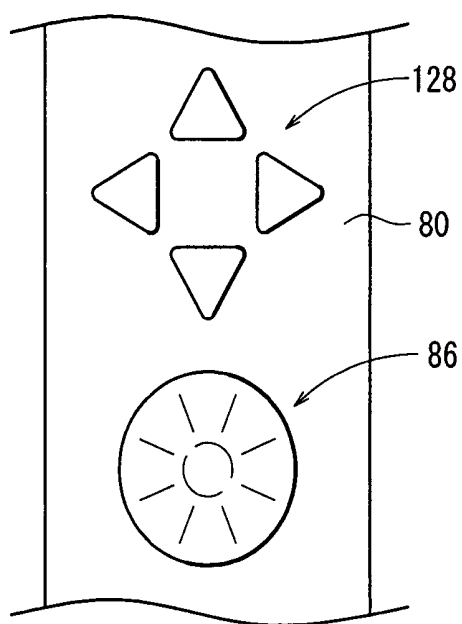


FIG. 8



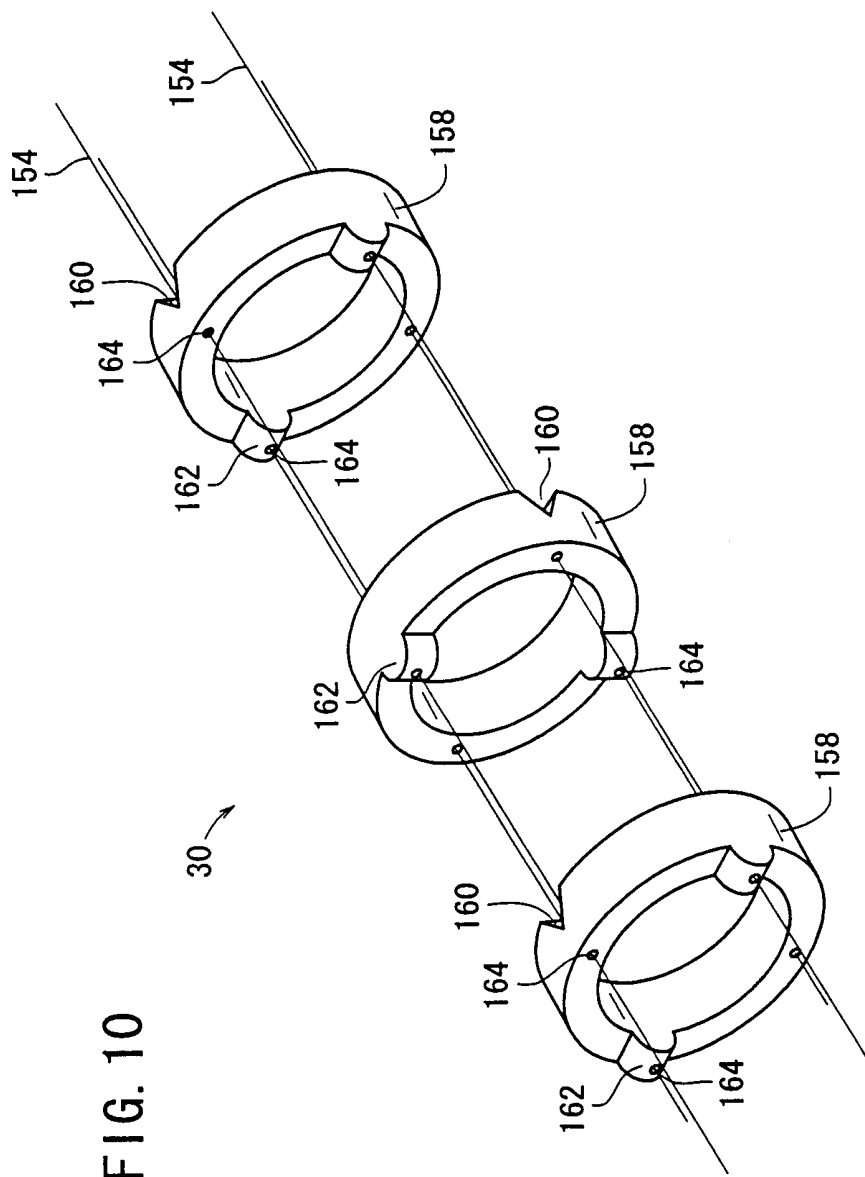
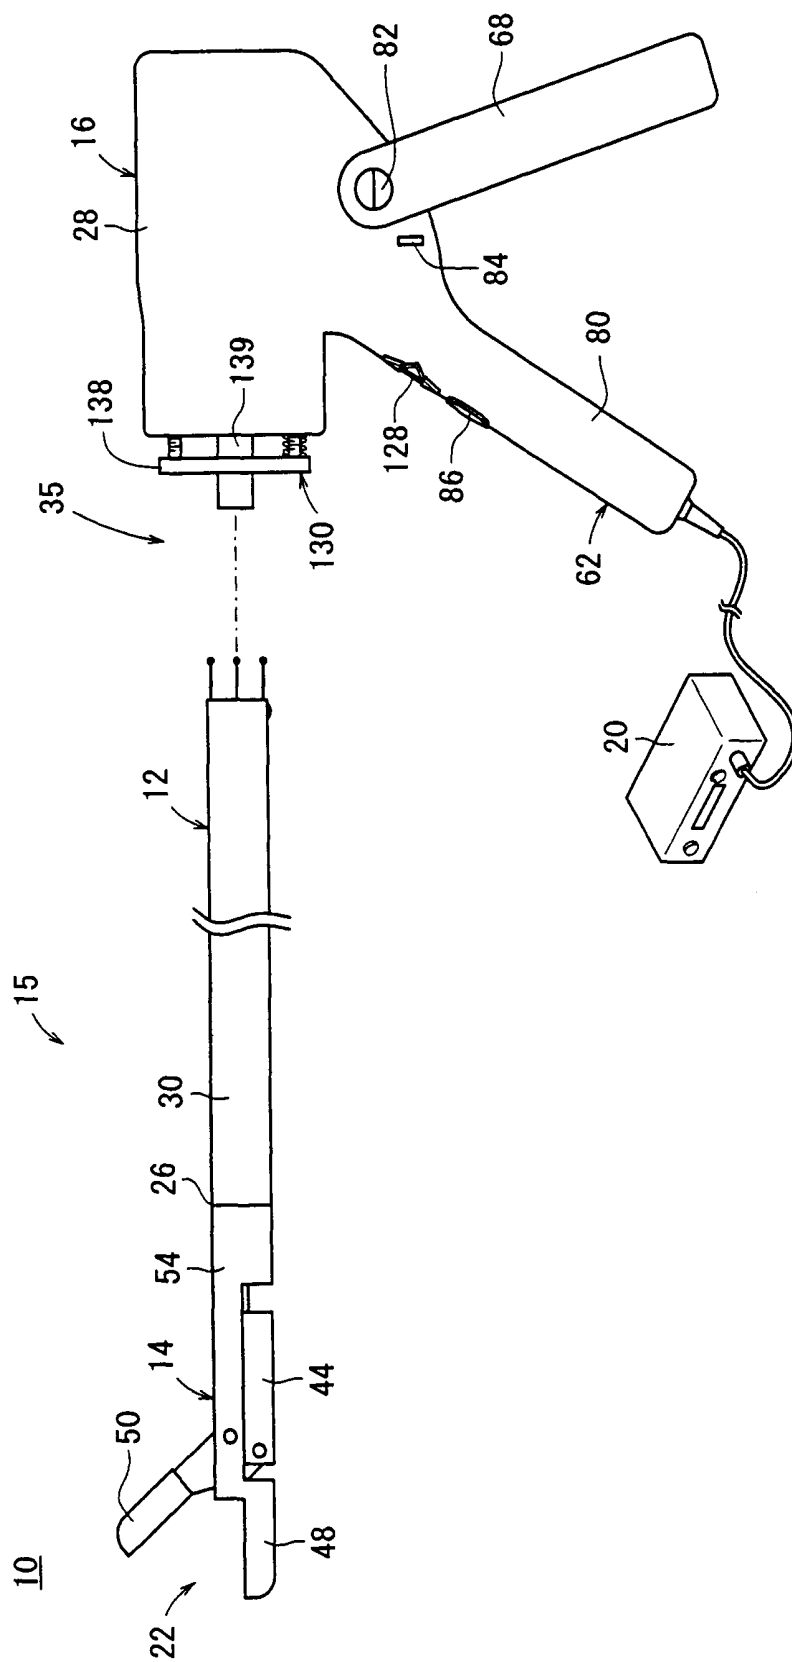
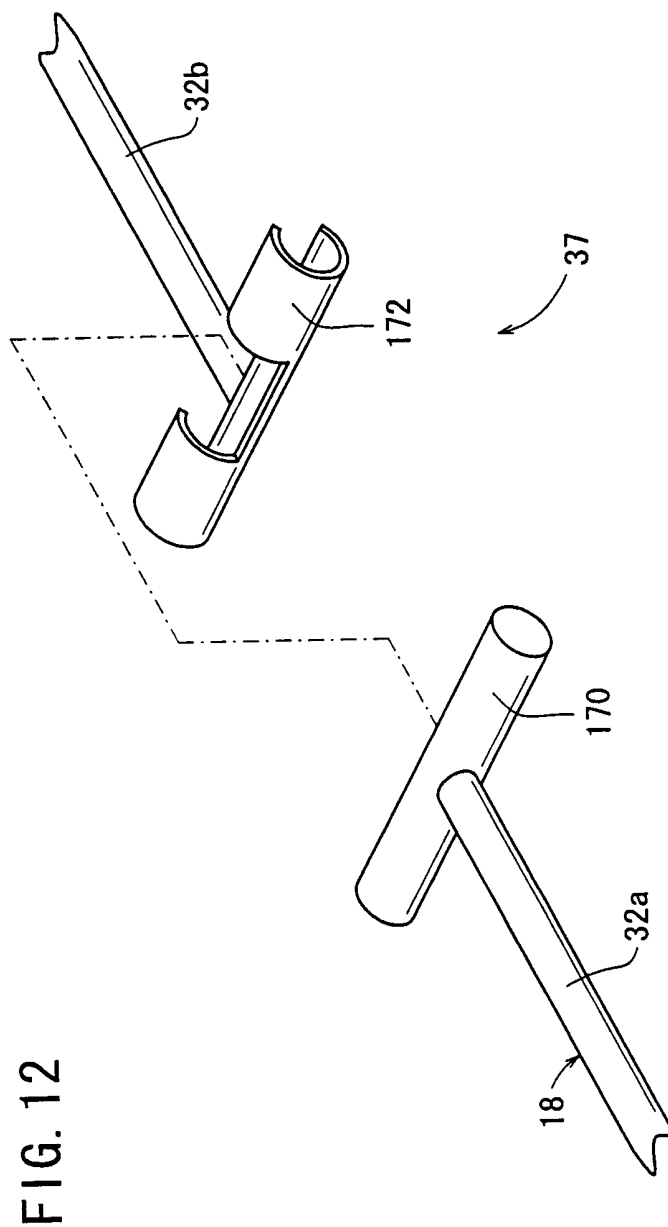
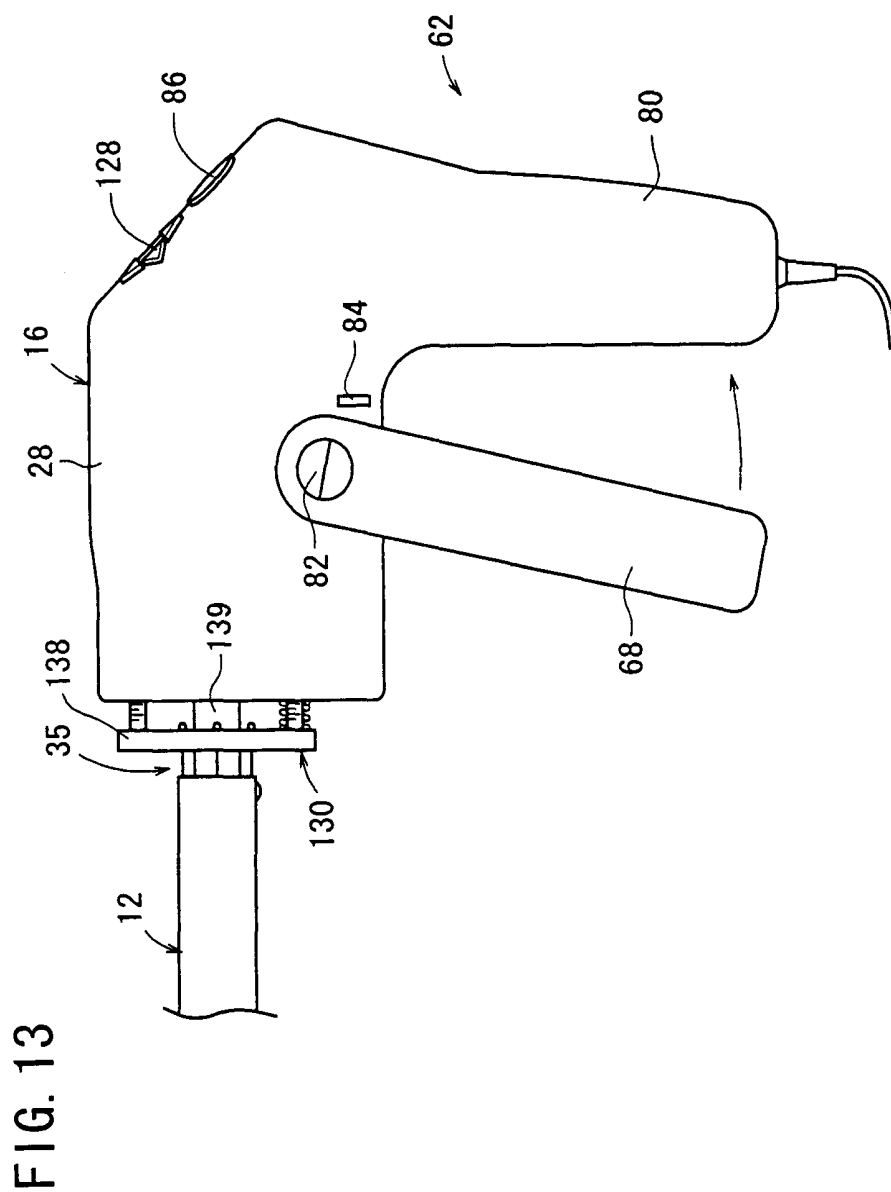


FIG. 11







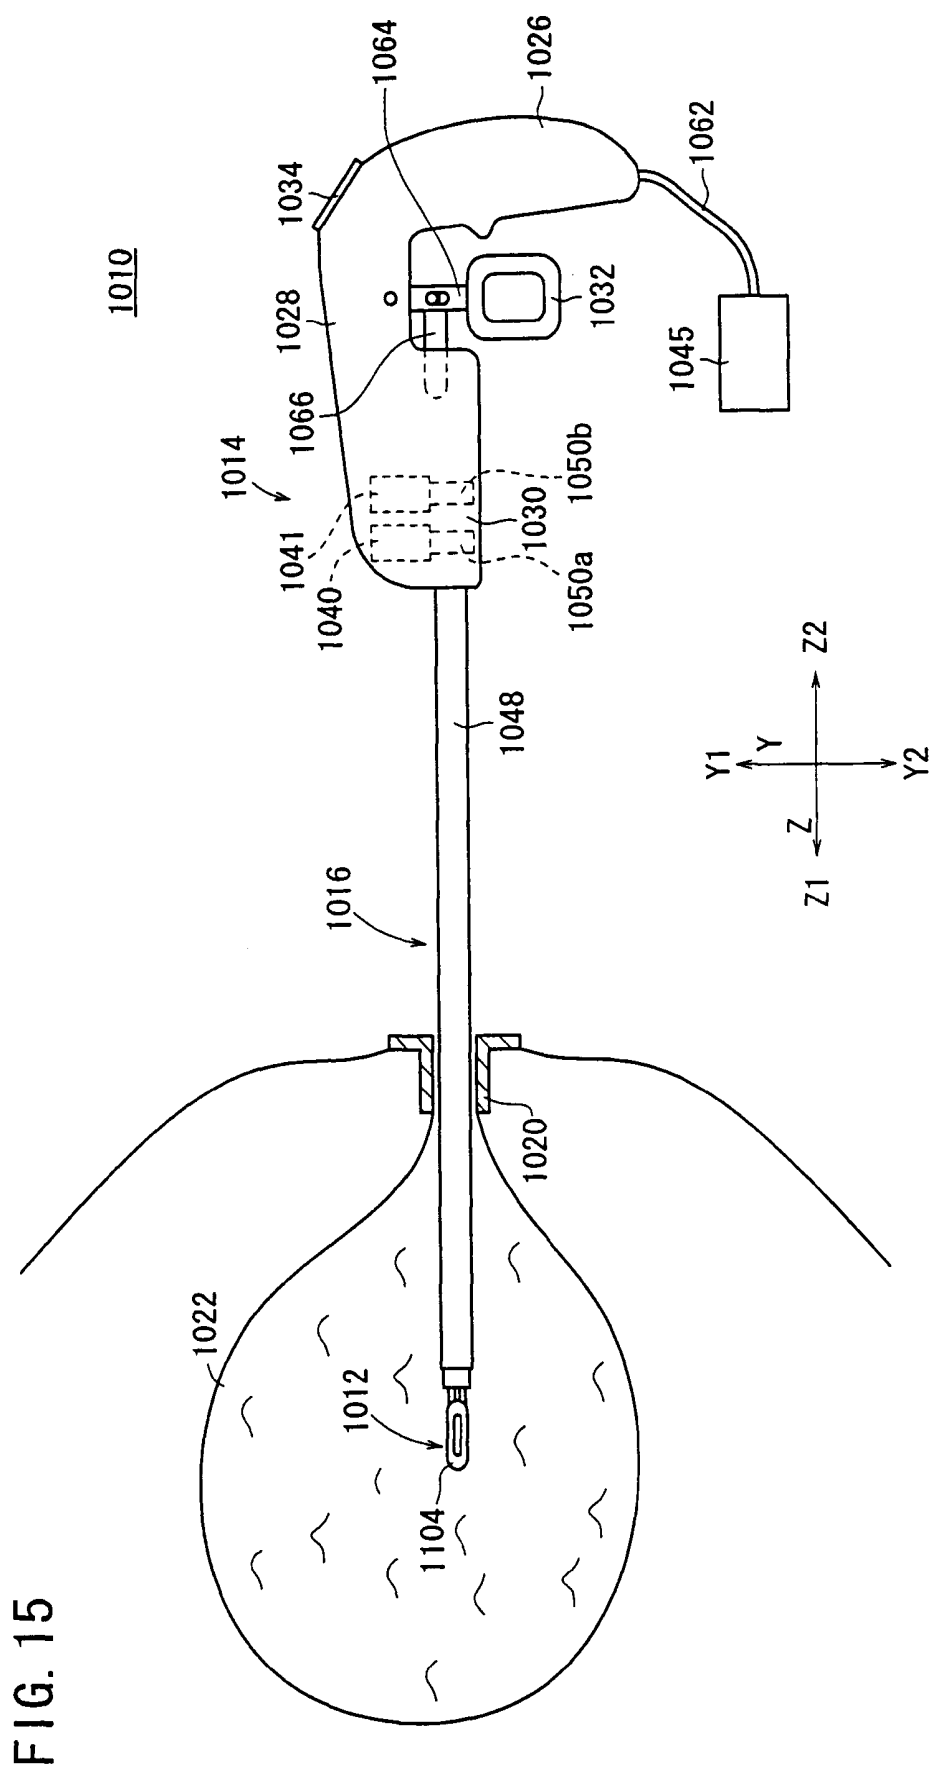


FIG. 16

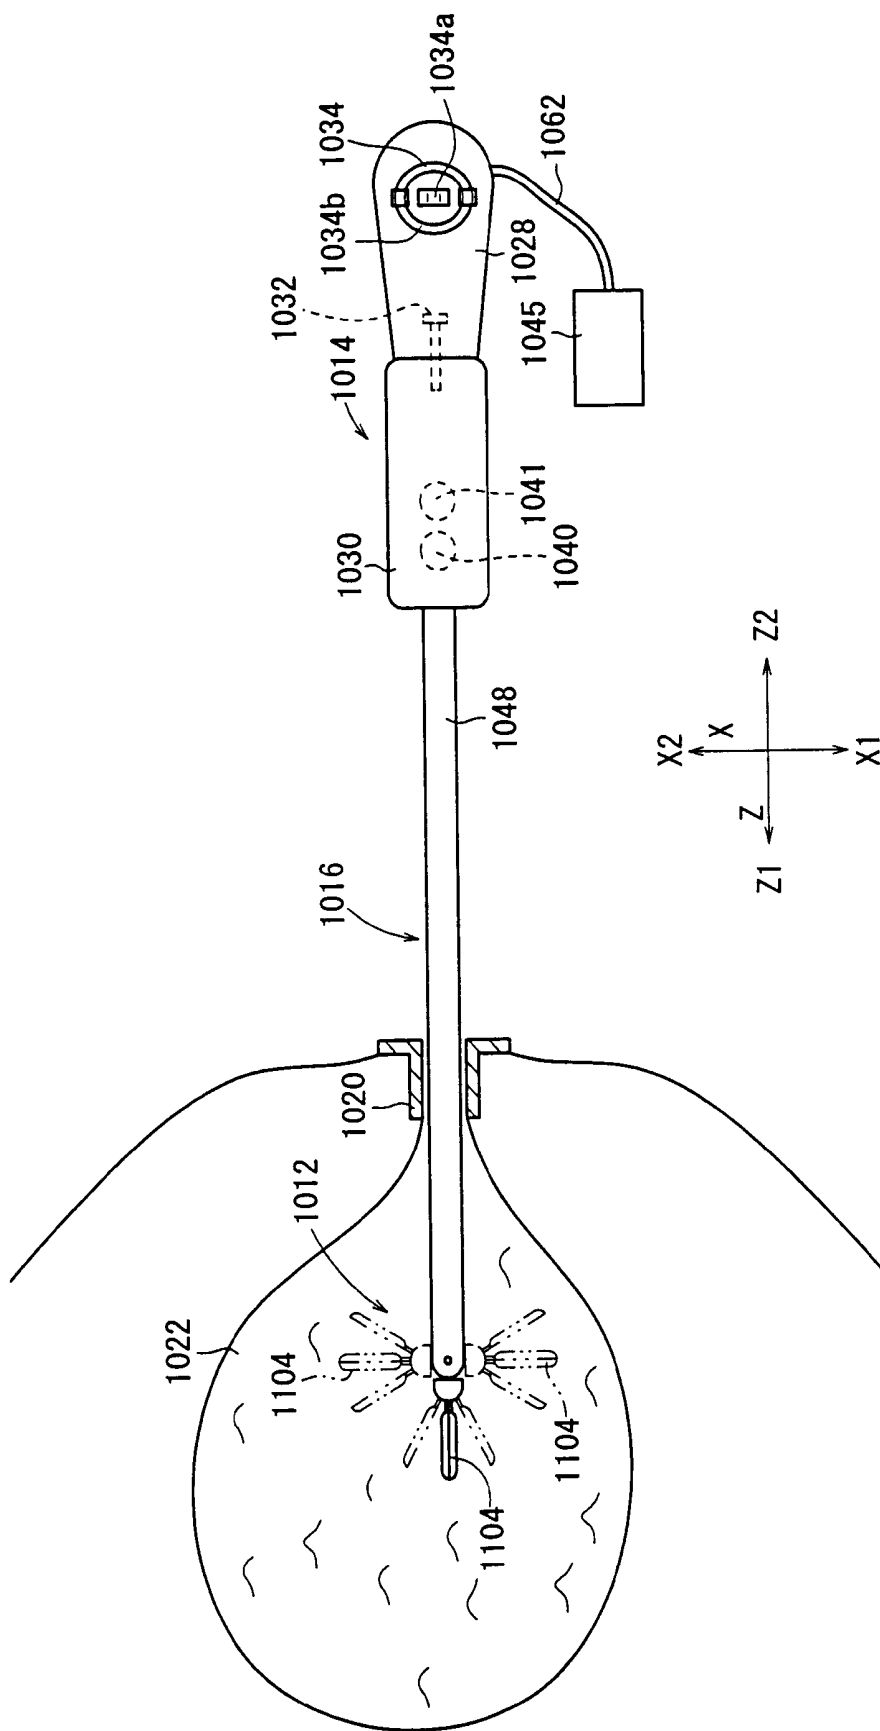


FIG. 17

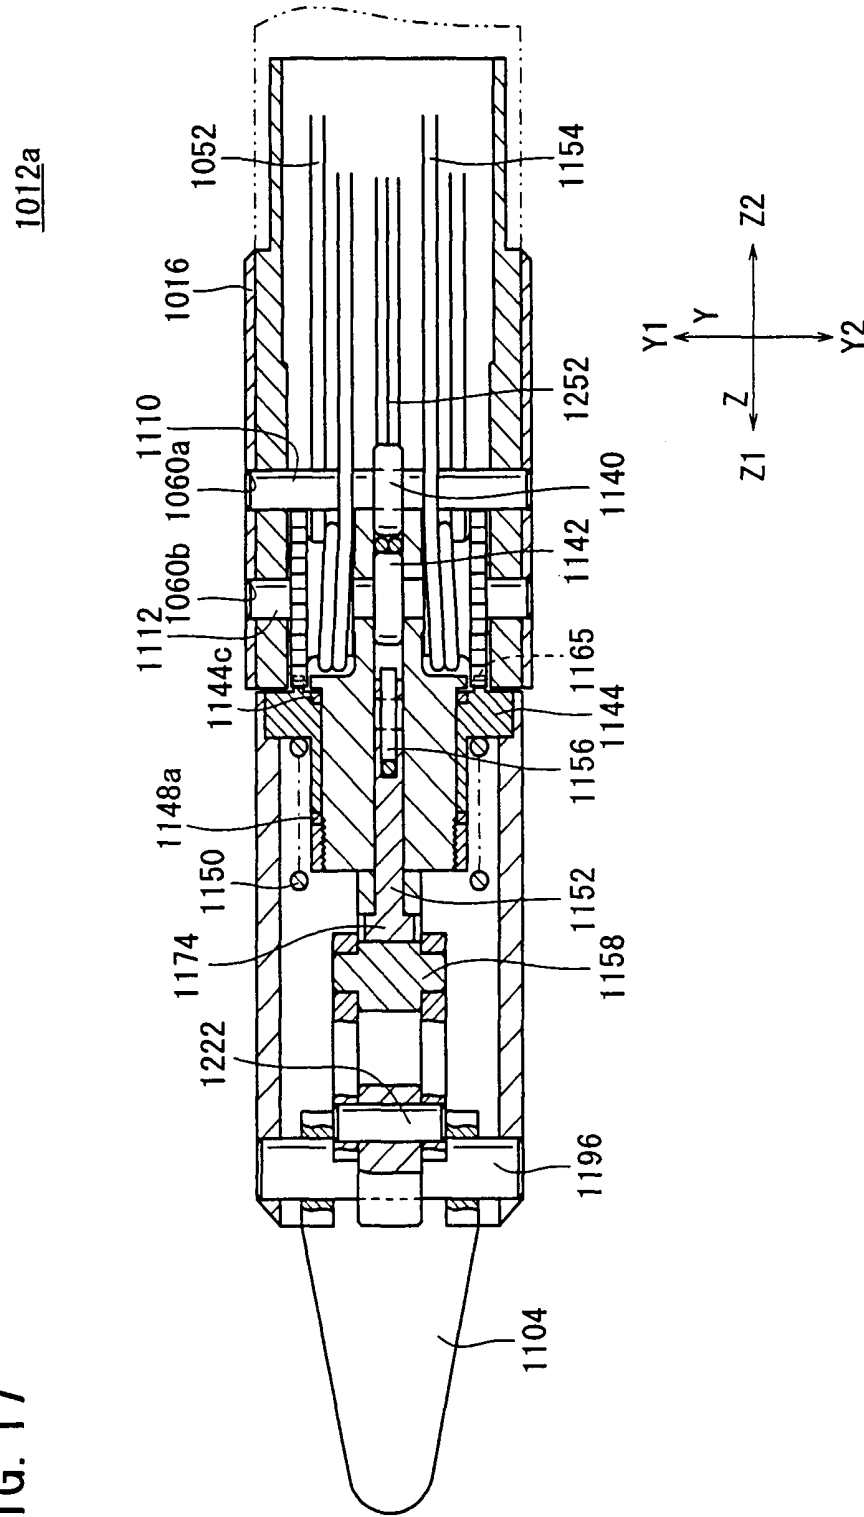


FIG. 18

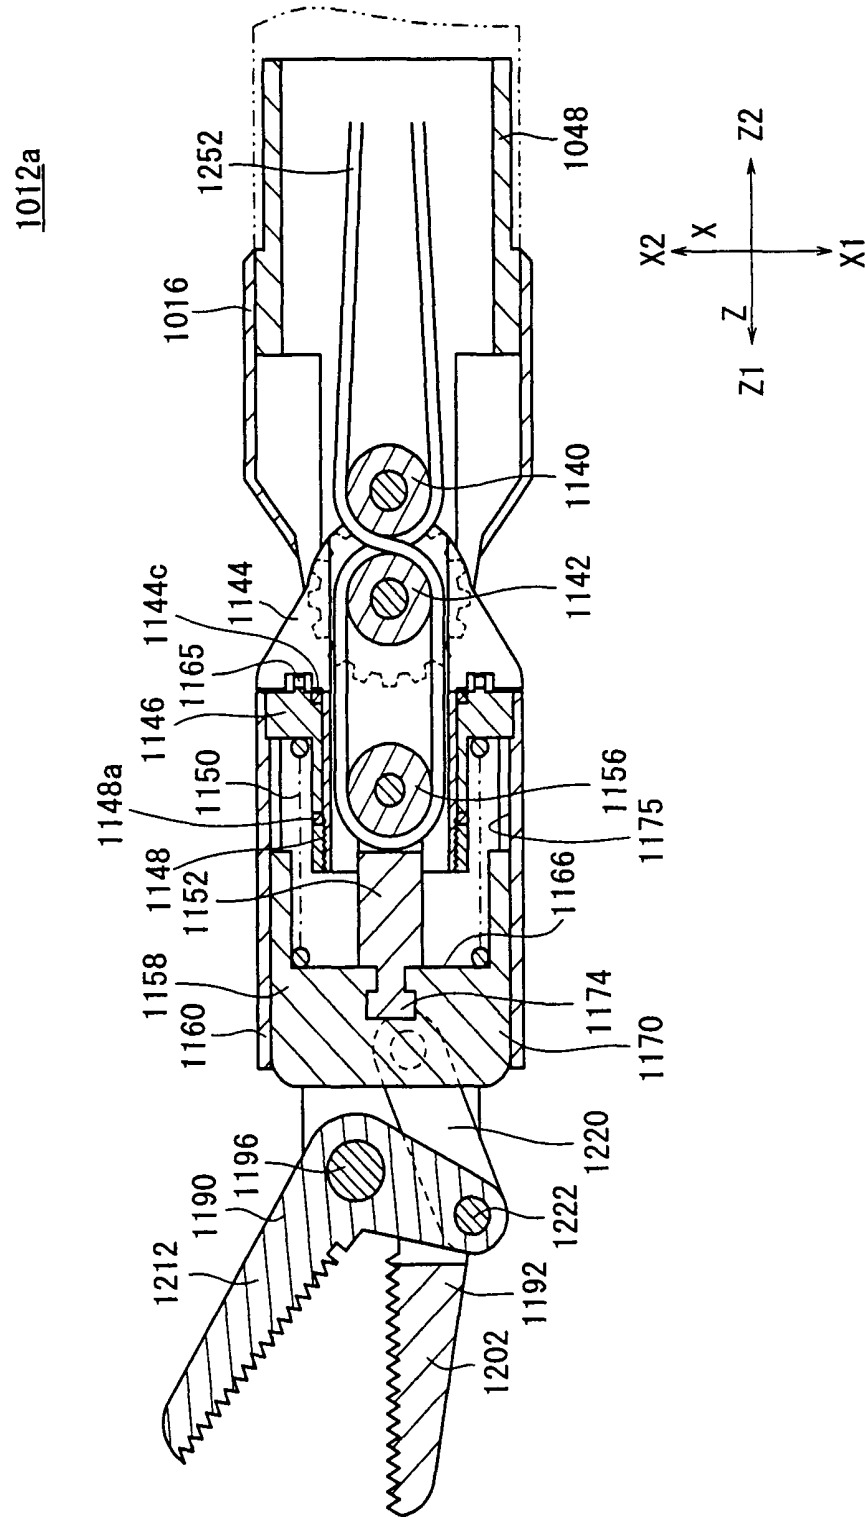


FIG. 19

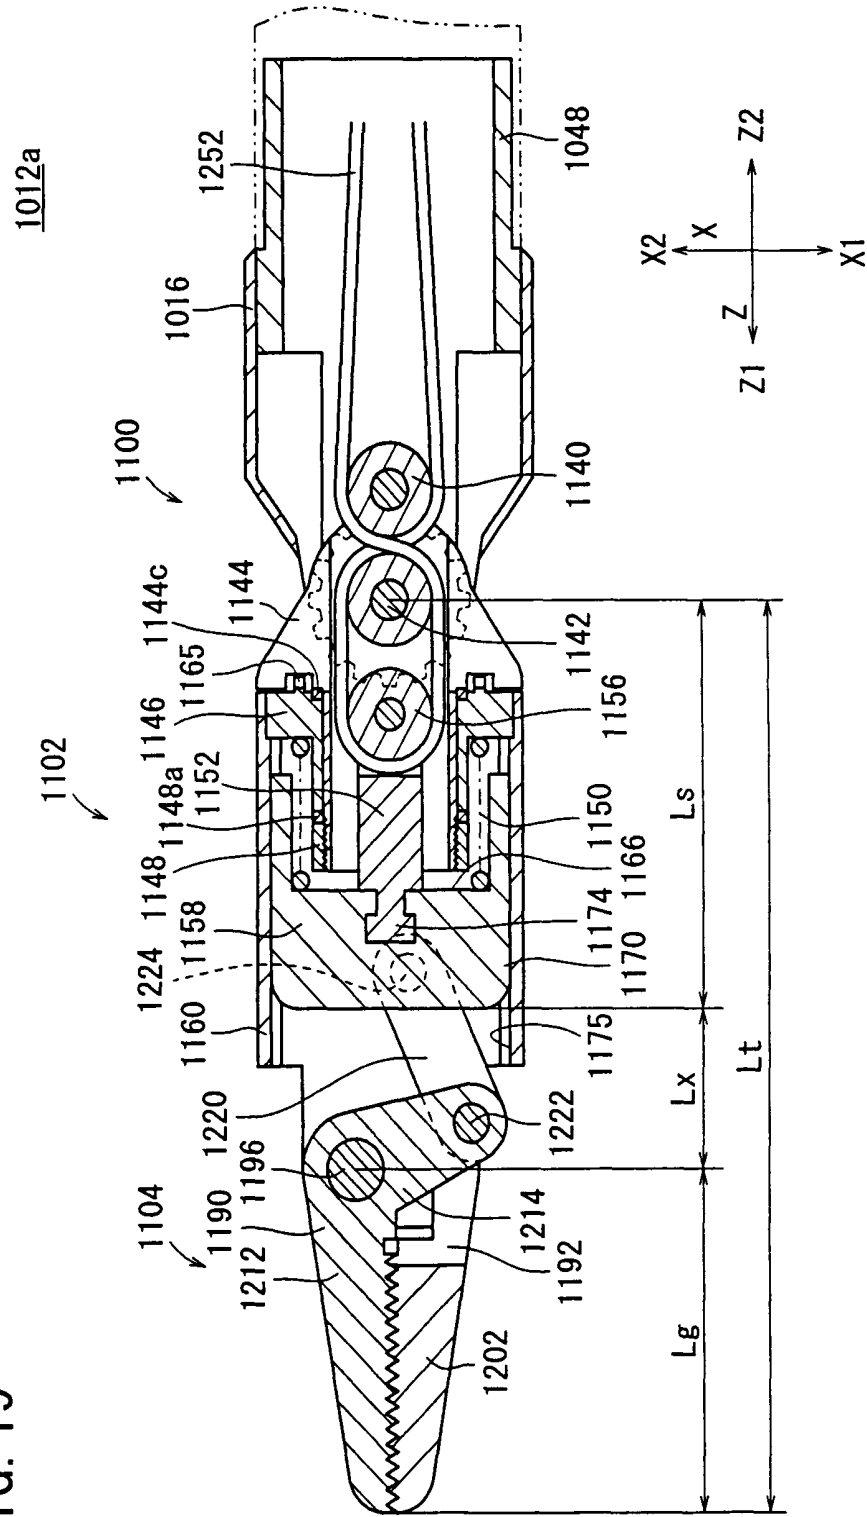
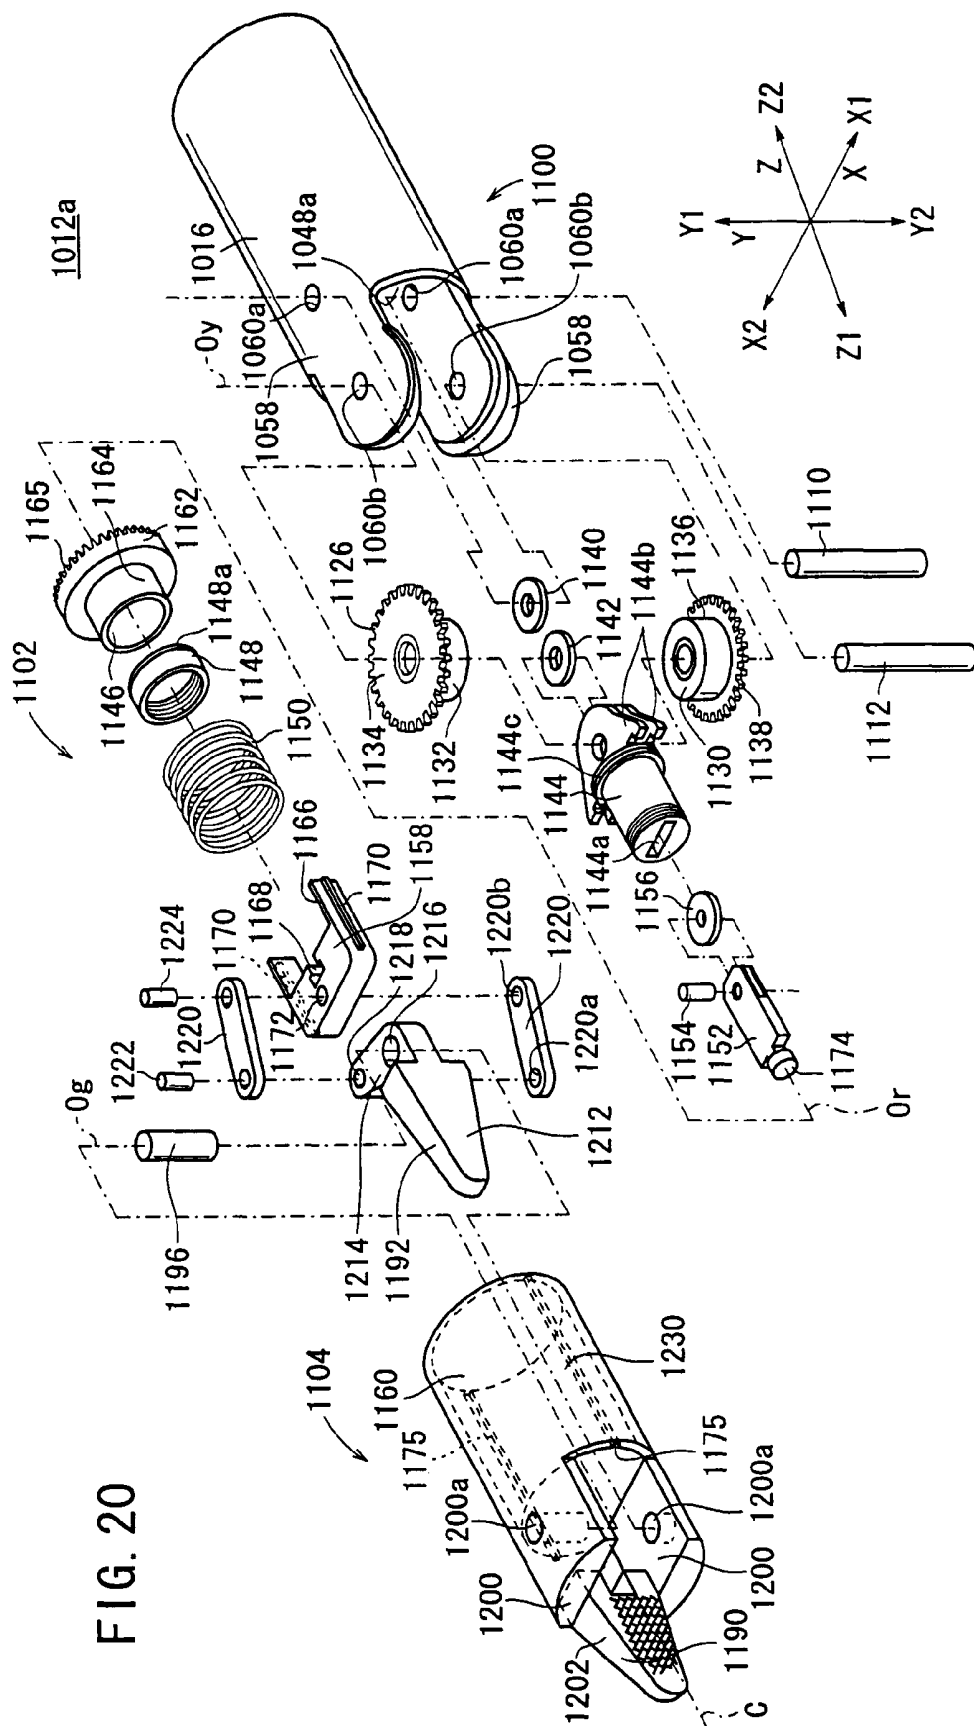


FIG. 20



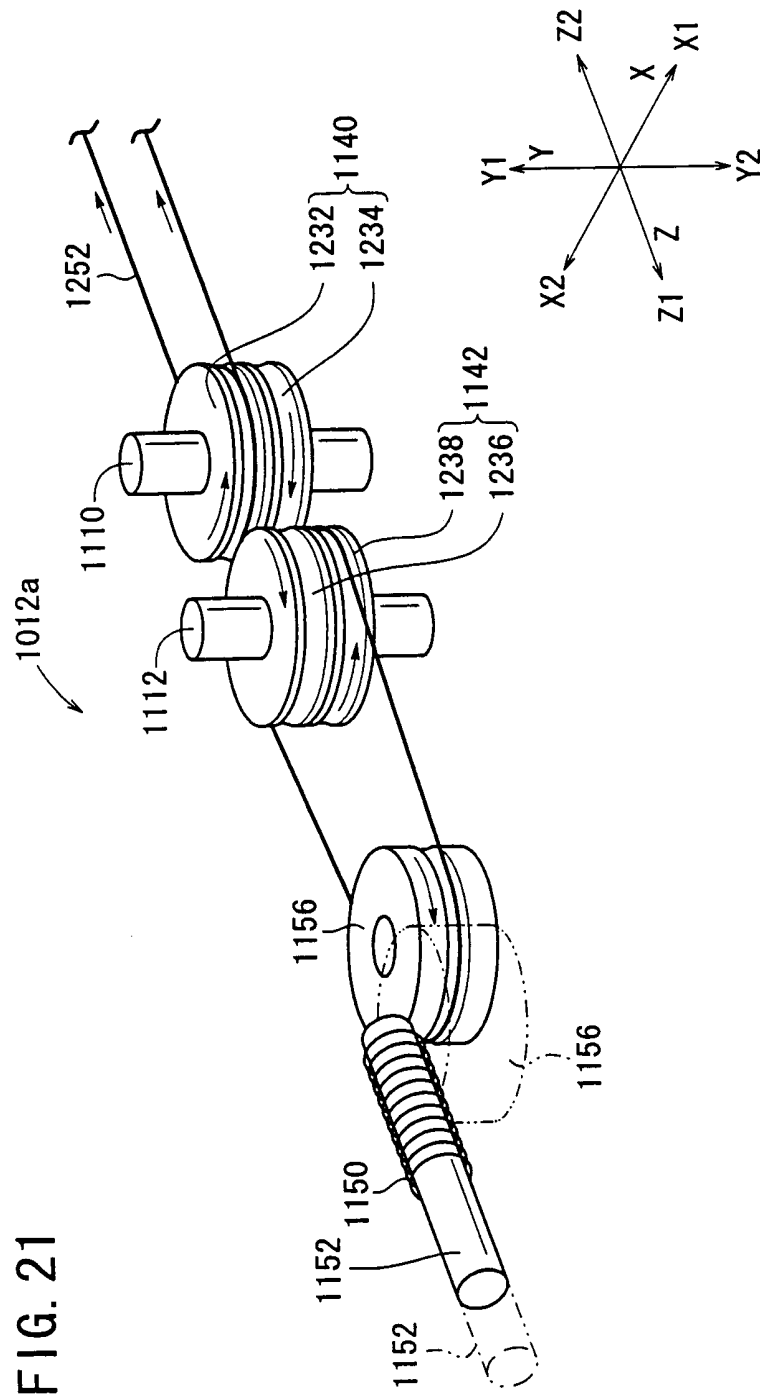


FIG. 22

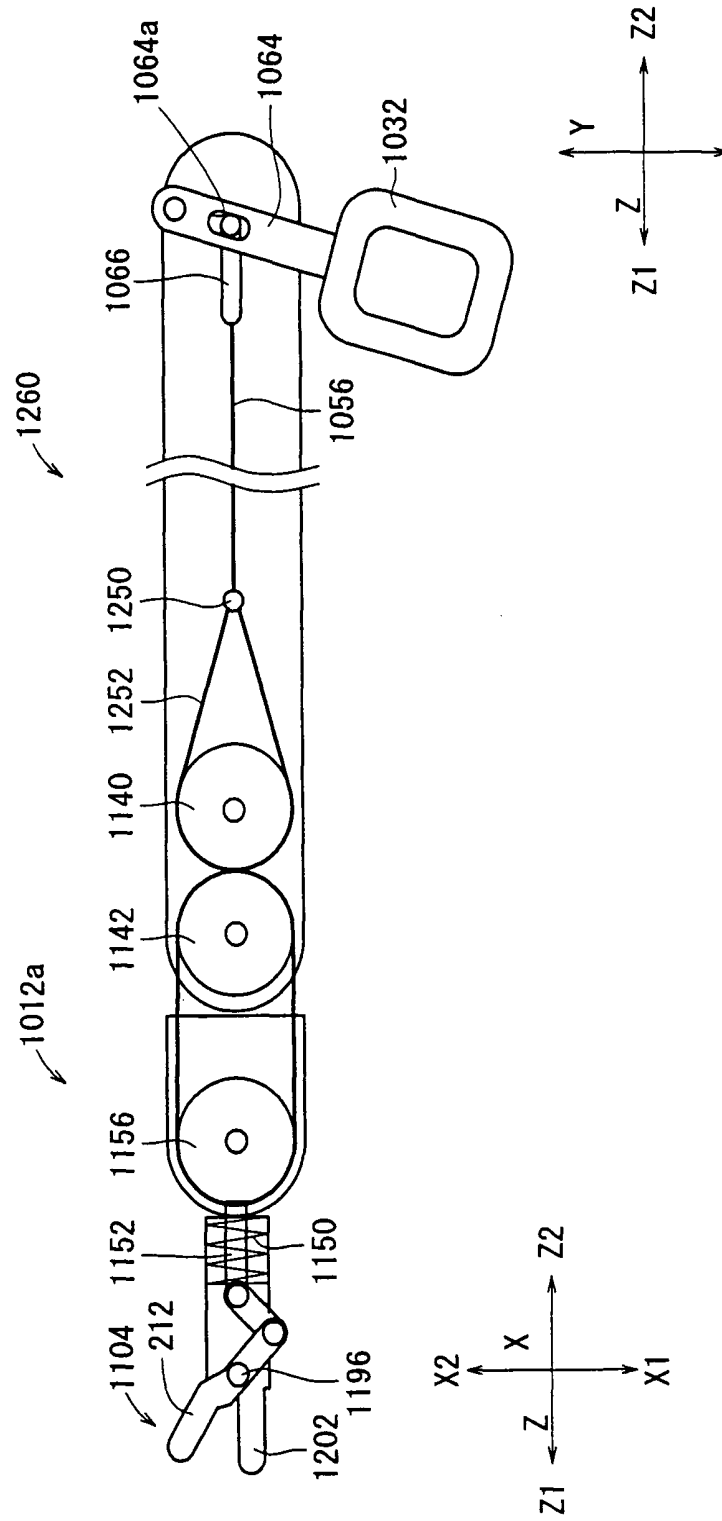


FIG. 23

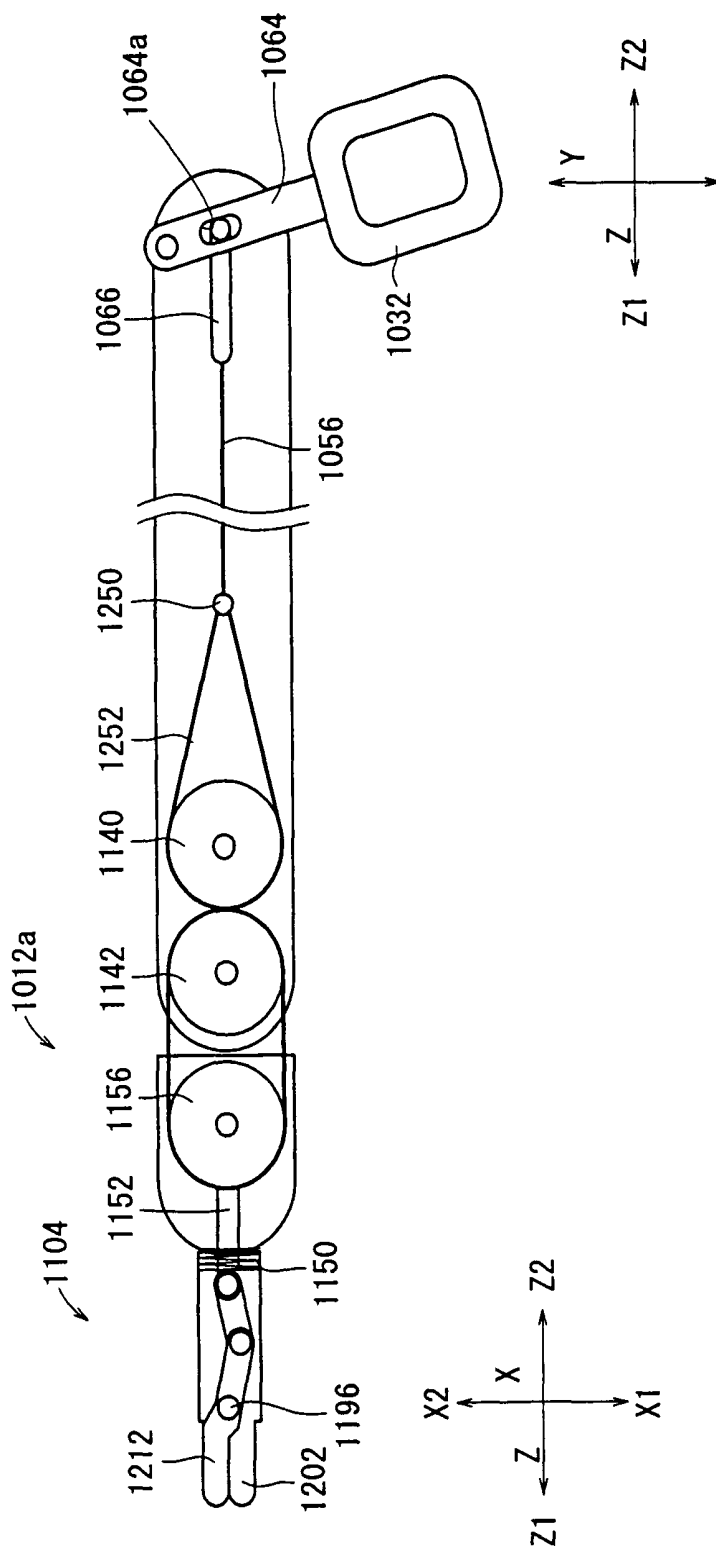


FIG. 24

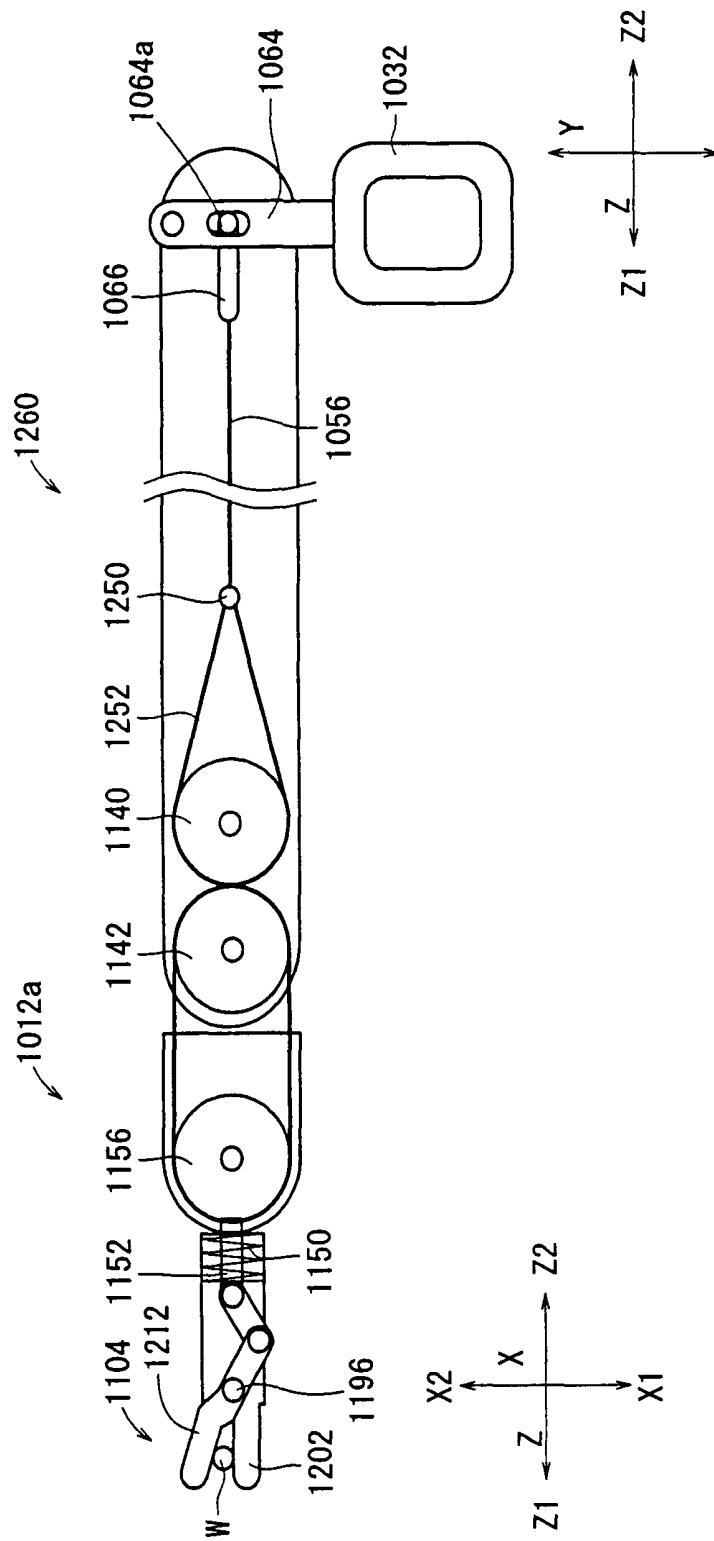


FIG. 26

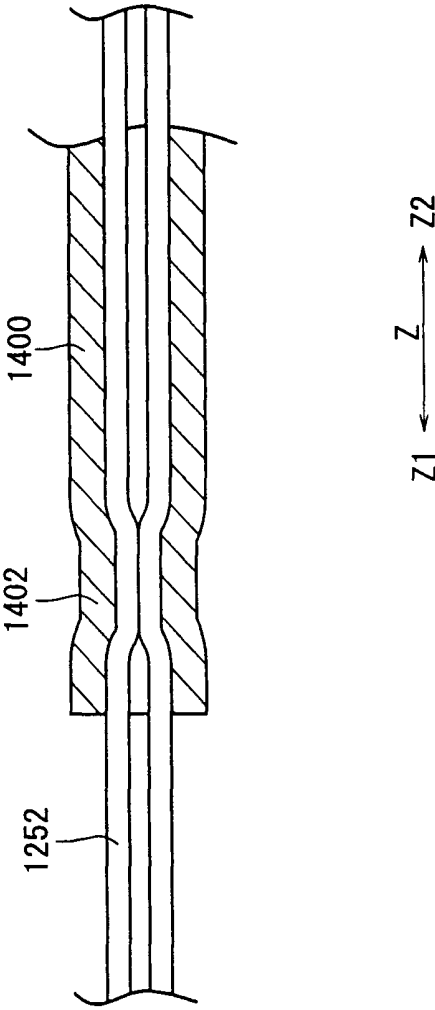


FIG. 27

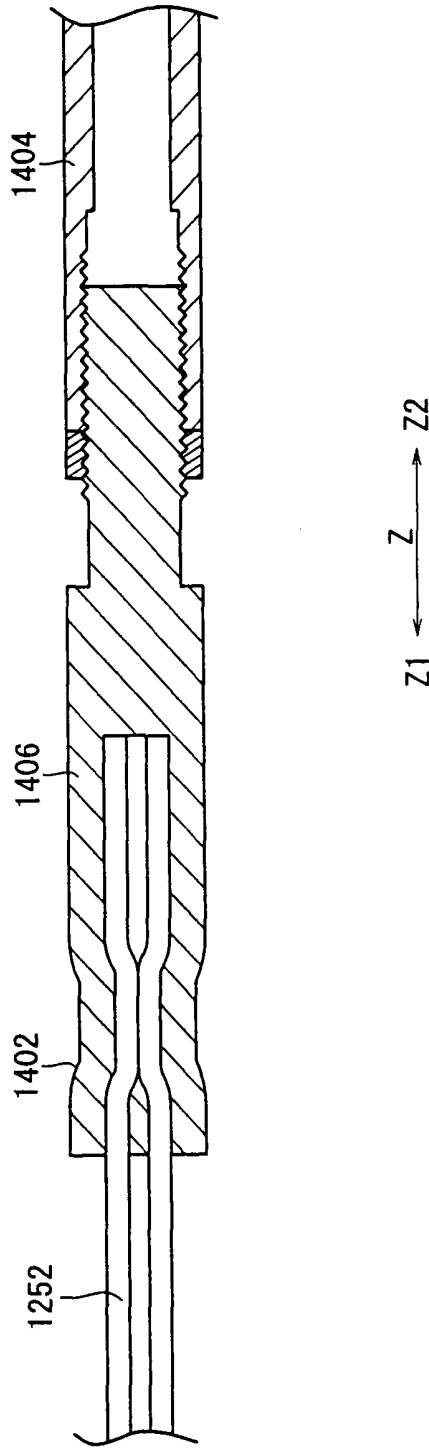


FIG. 28

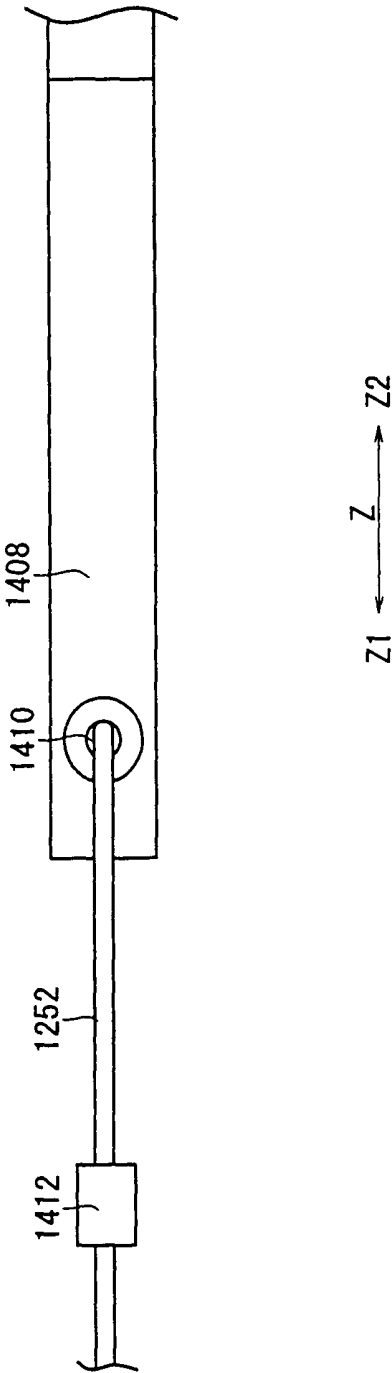


FIG. 29

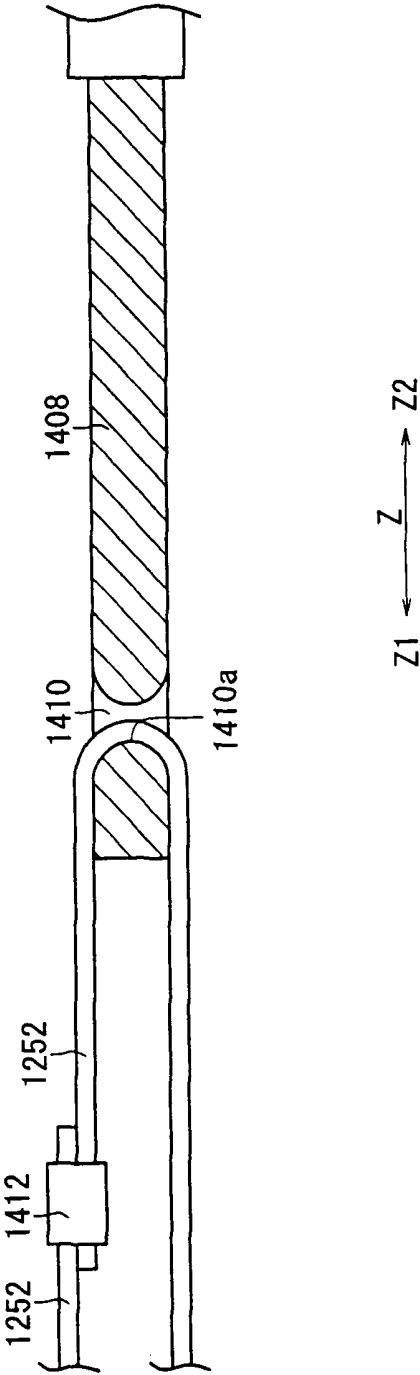


FIG. 30

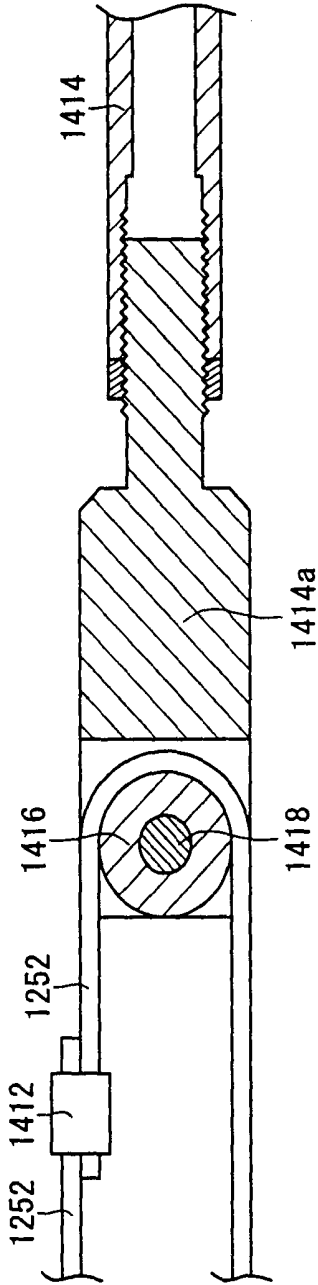
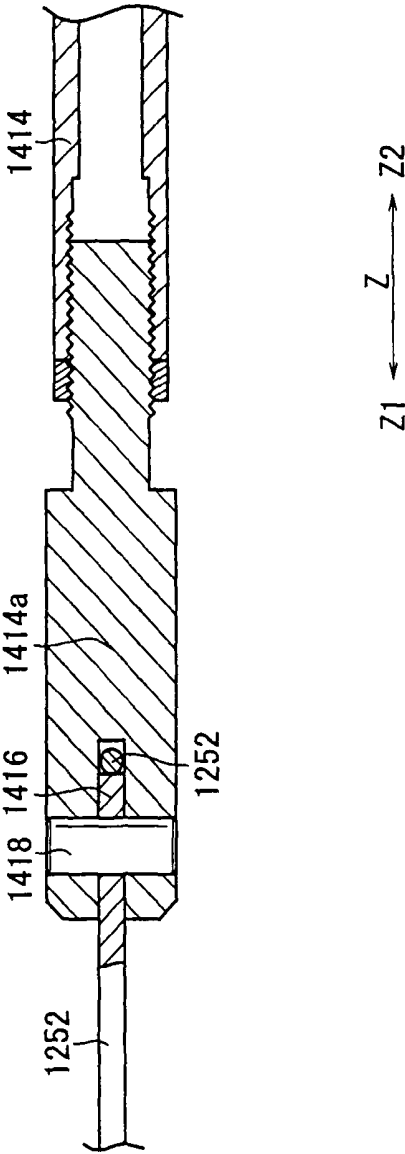


FIG. 31



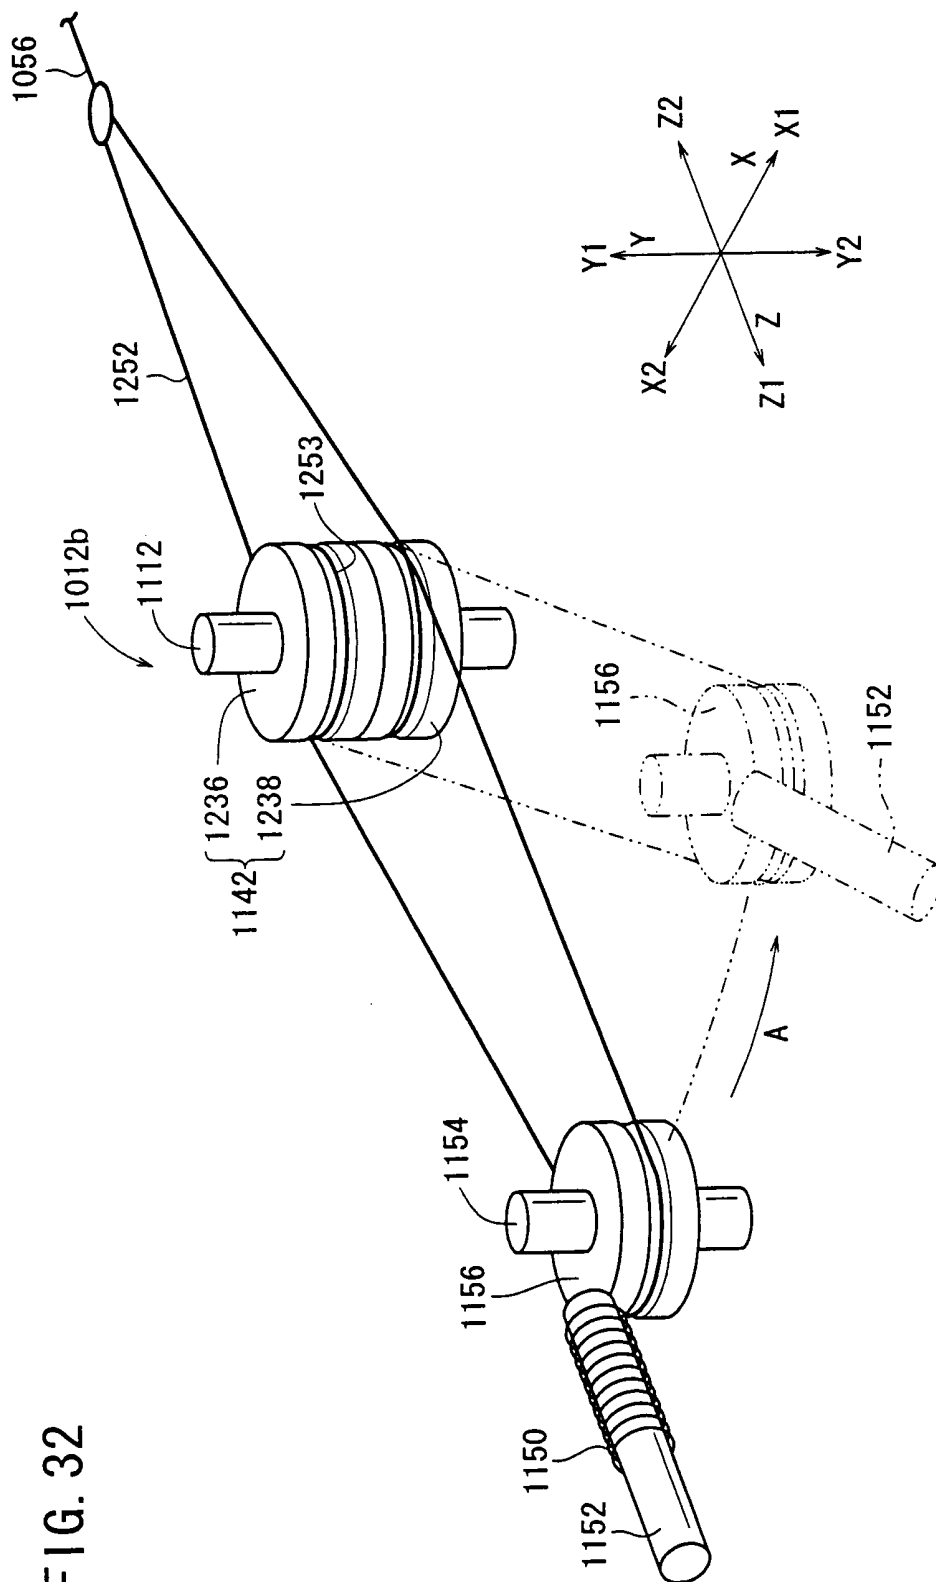


FIG. 32

FIG. 34

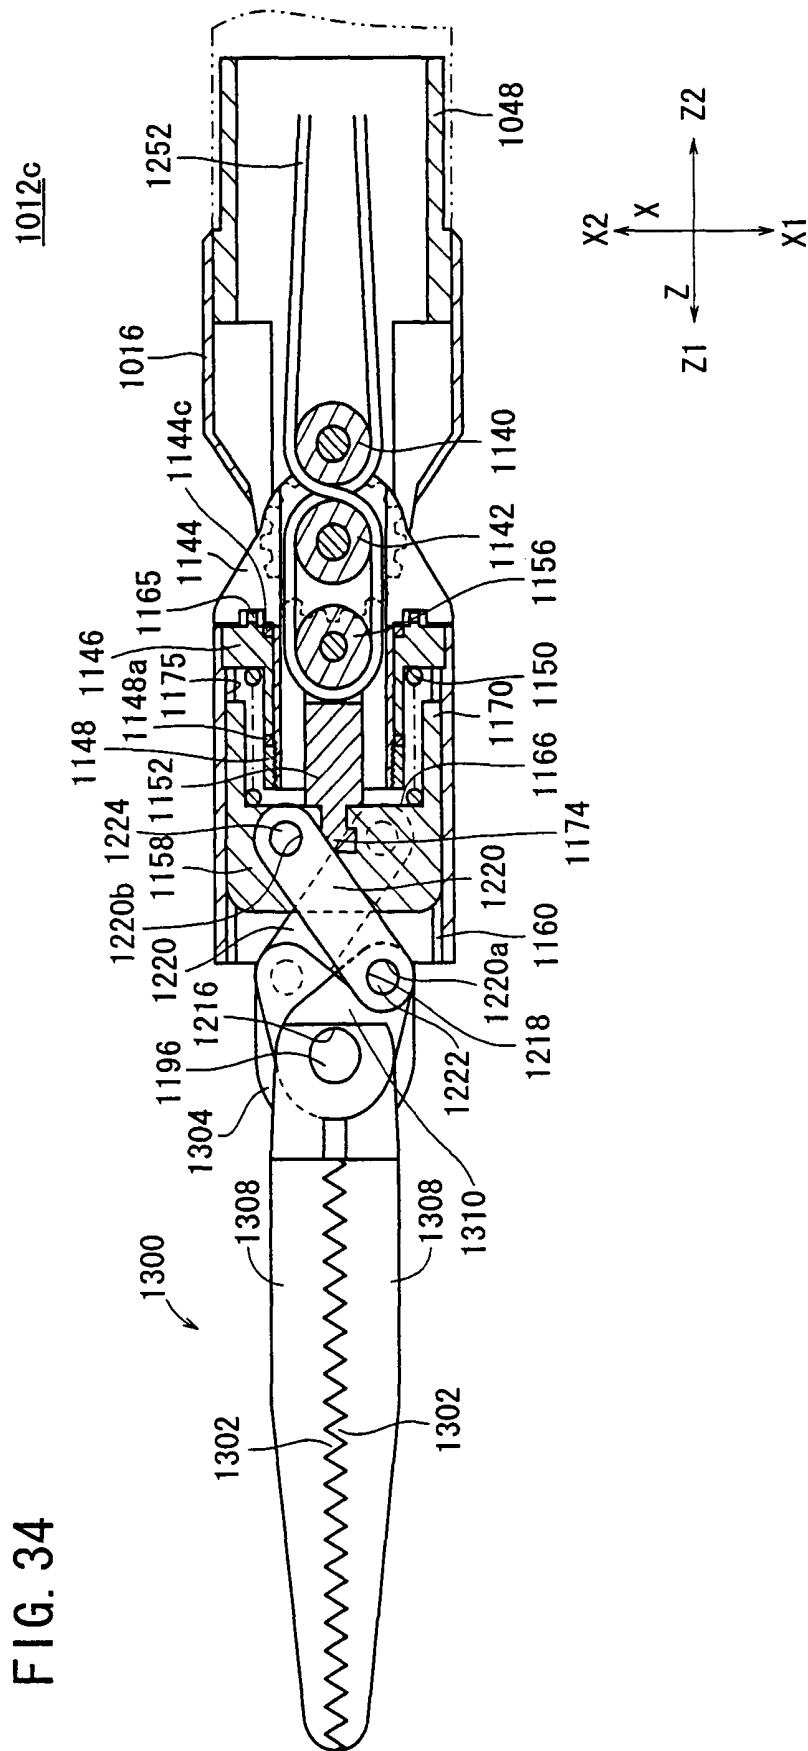
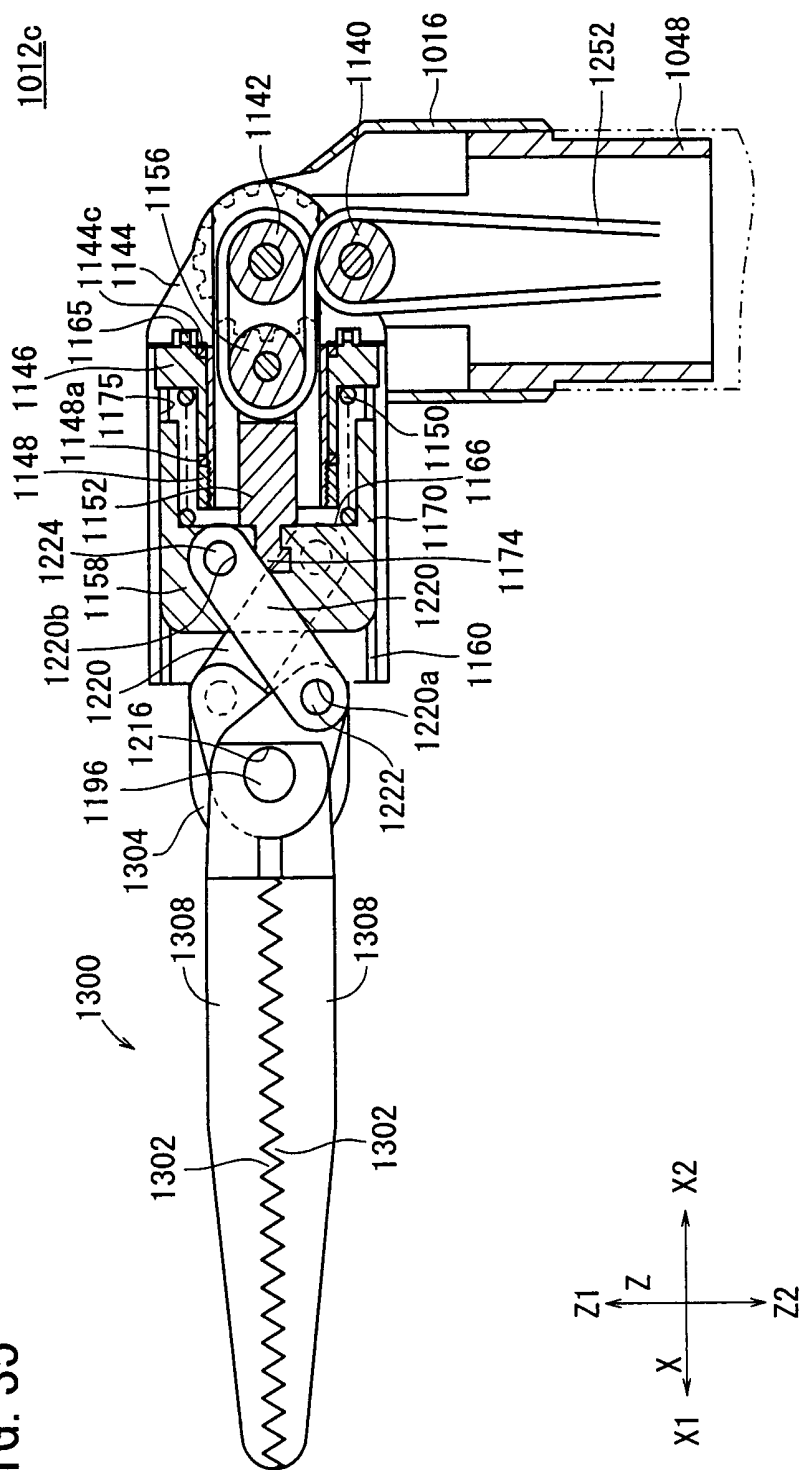
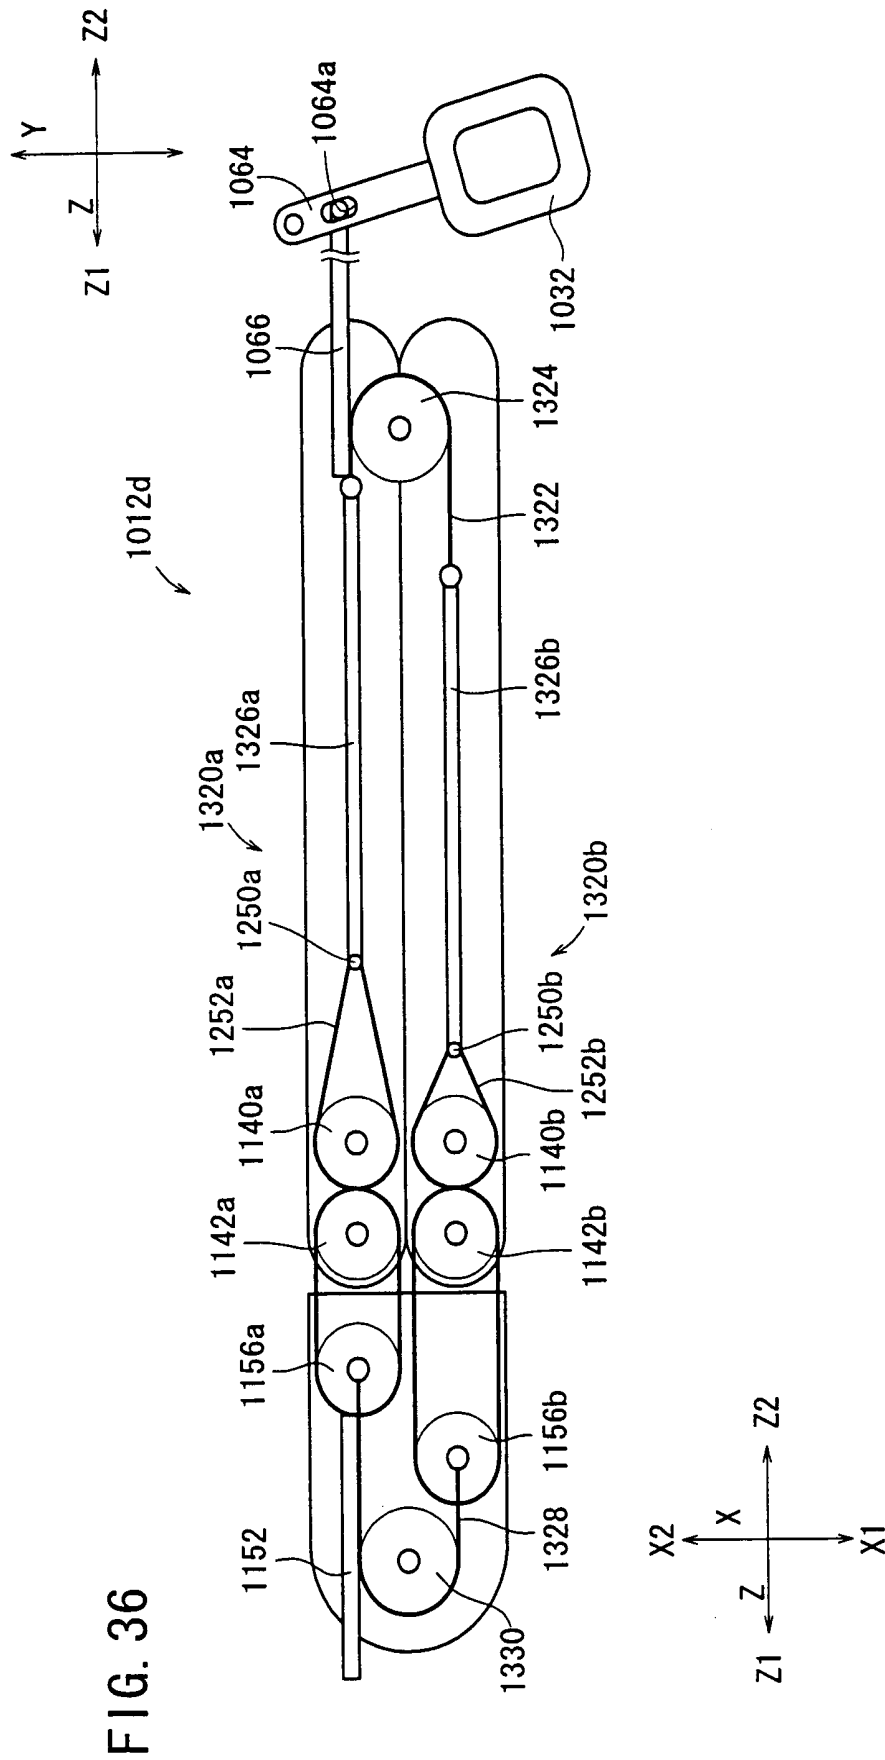
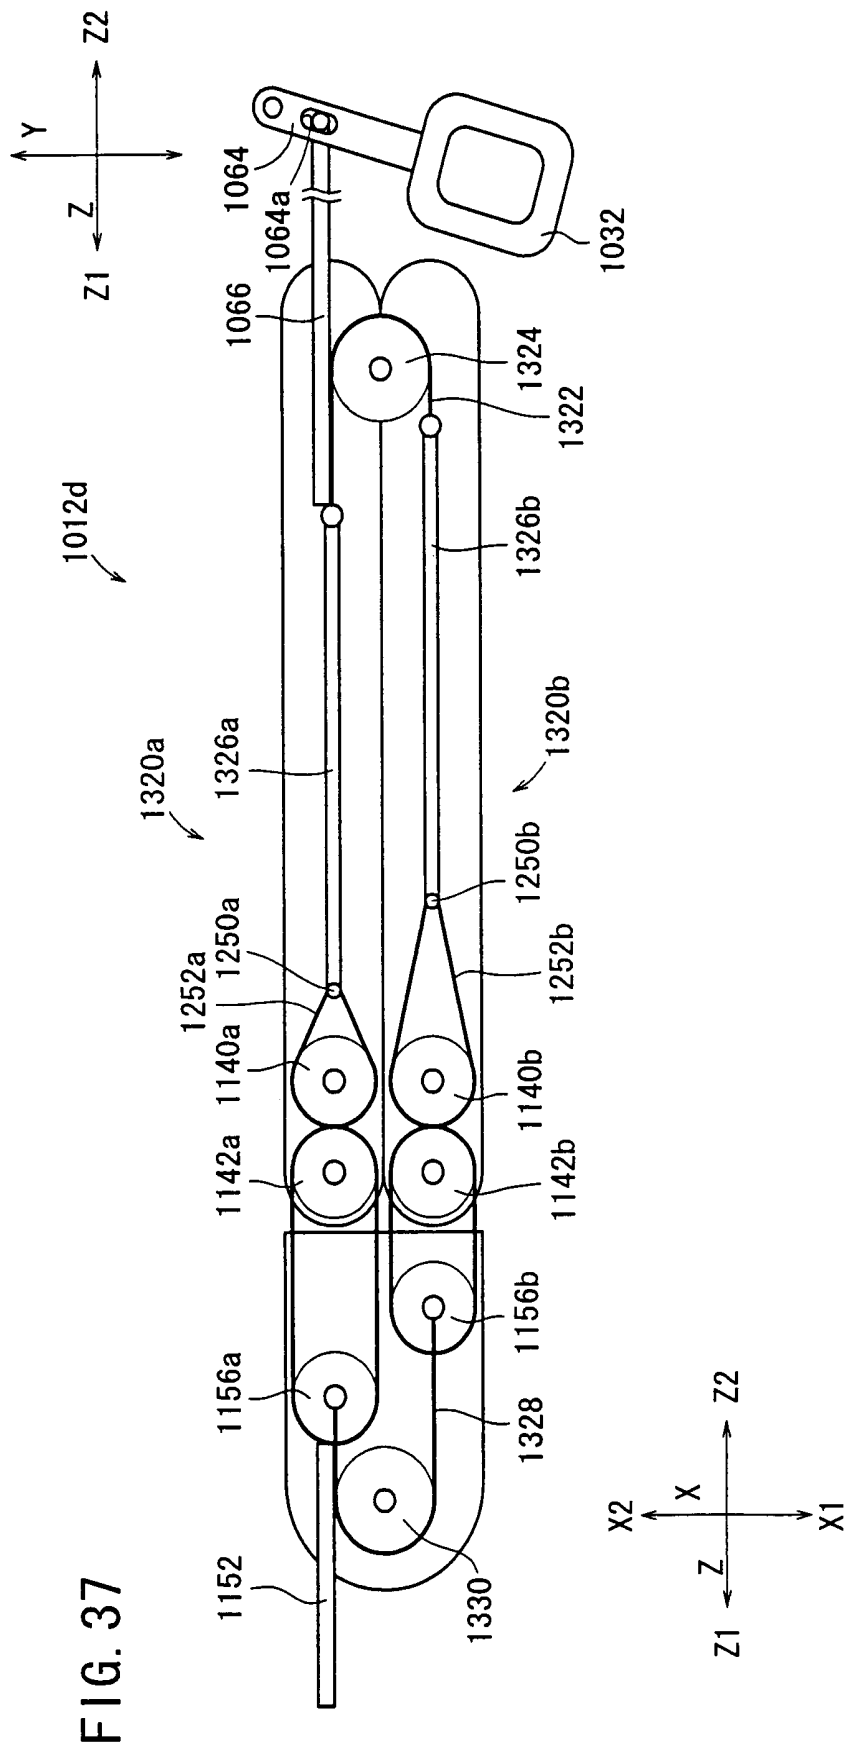
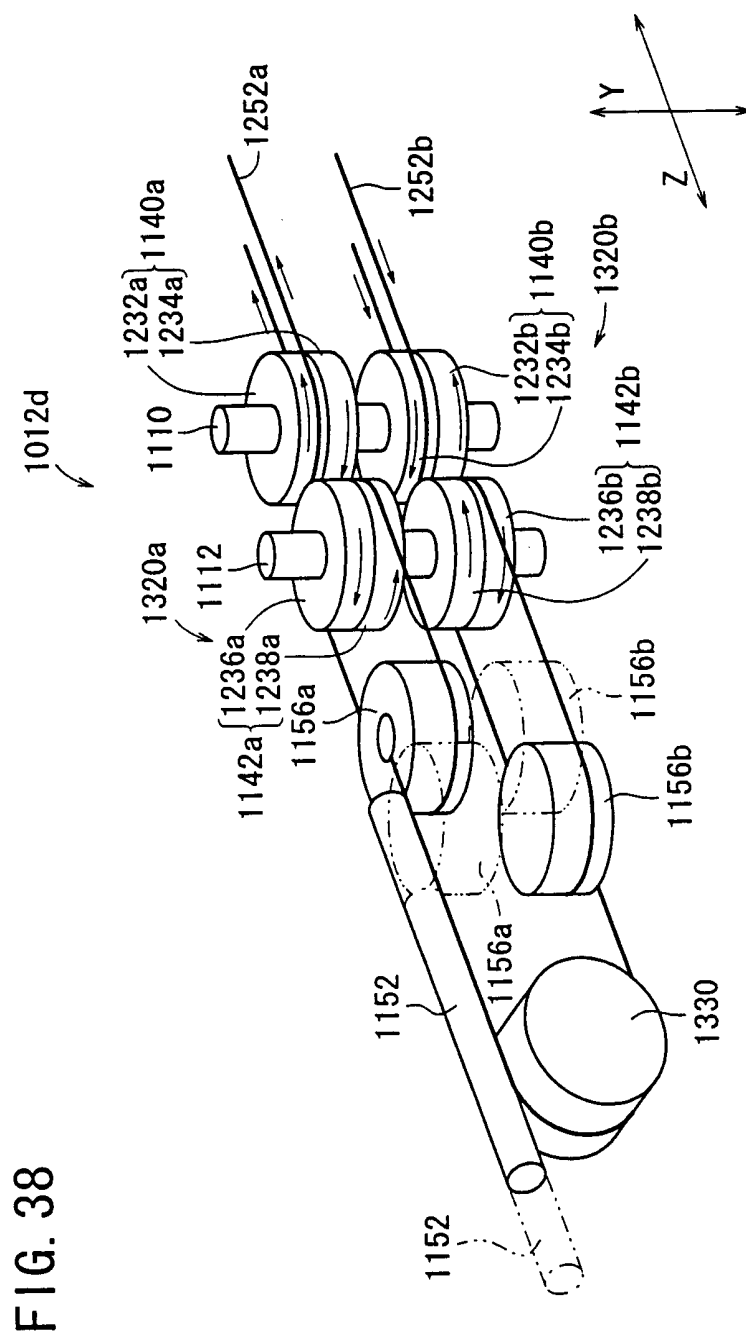


FIG. 35









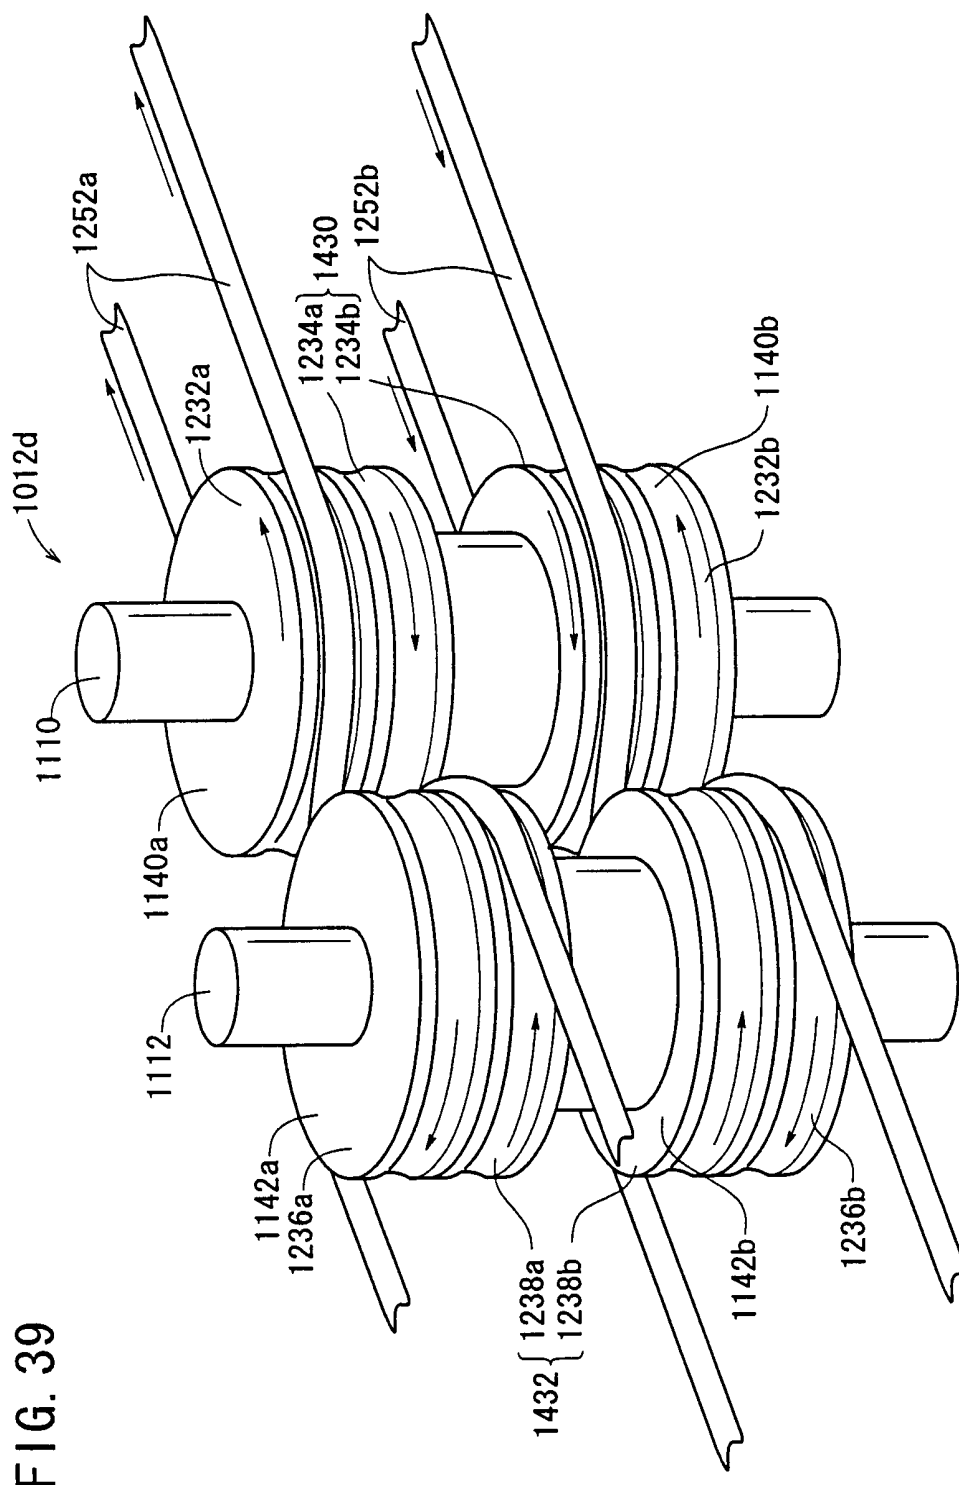


FIG. 40

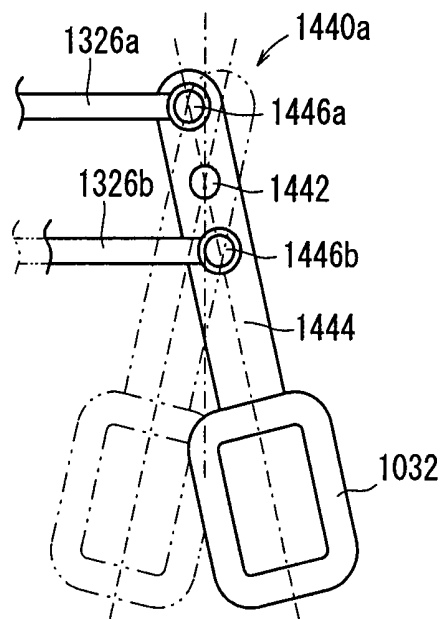


FIG. 41

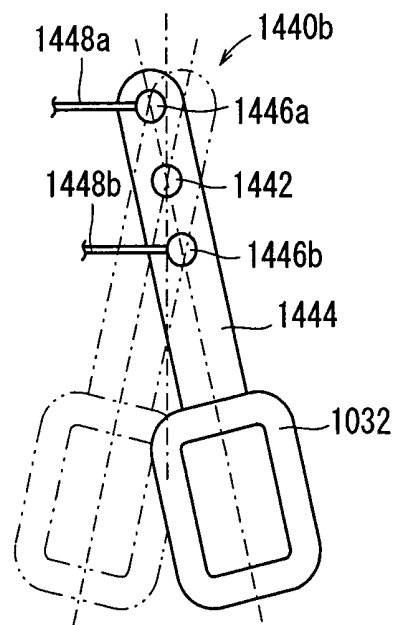


FIG. 42

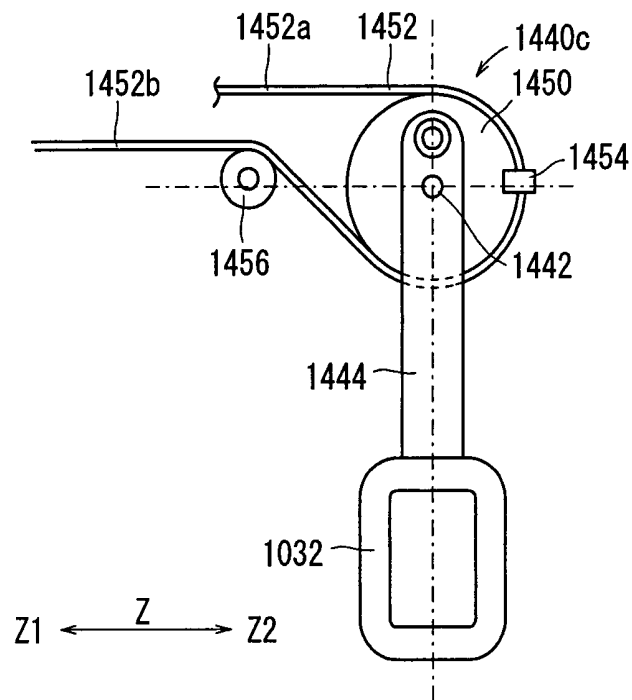


FIG. 43

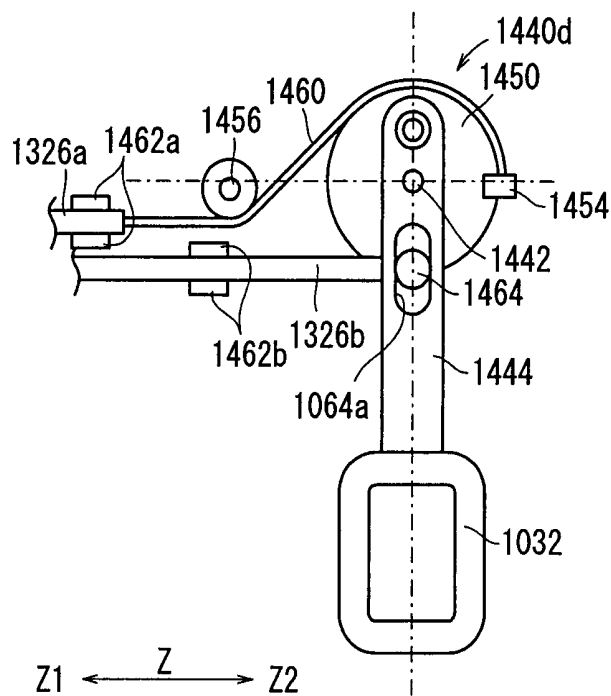


FIG. 44

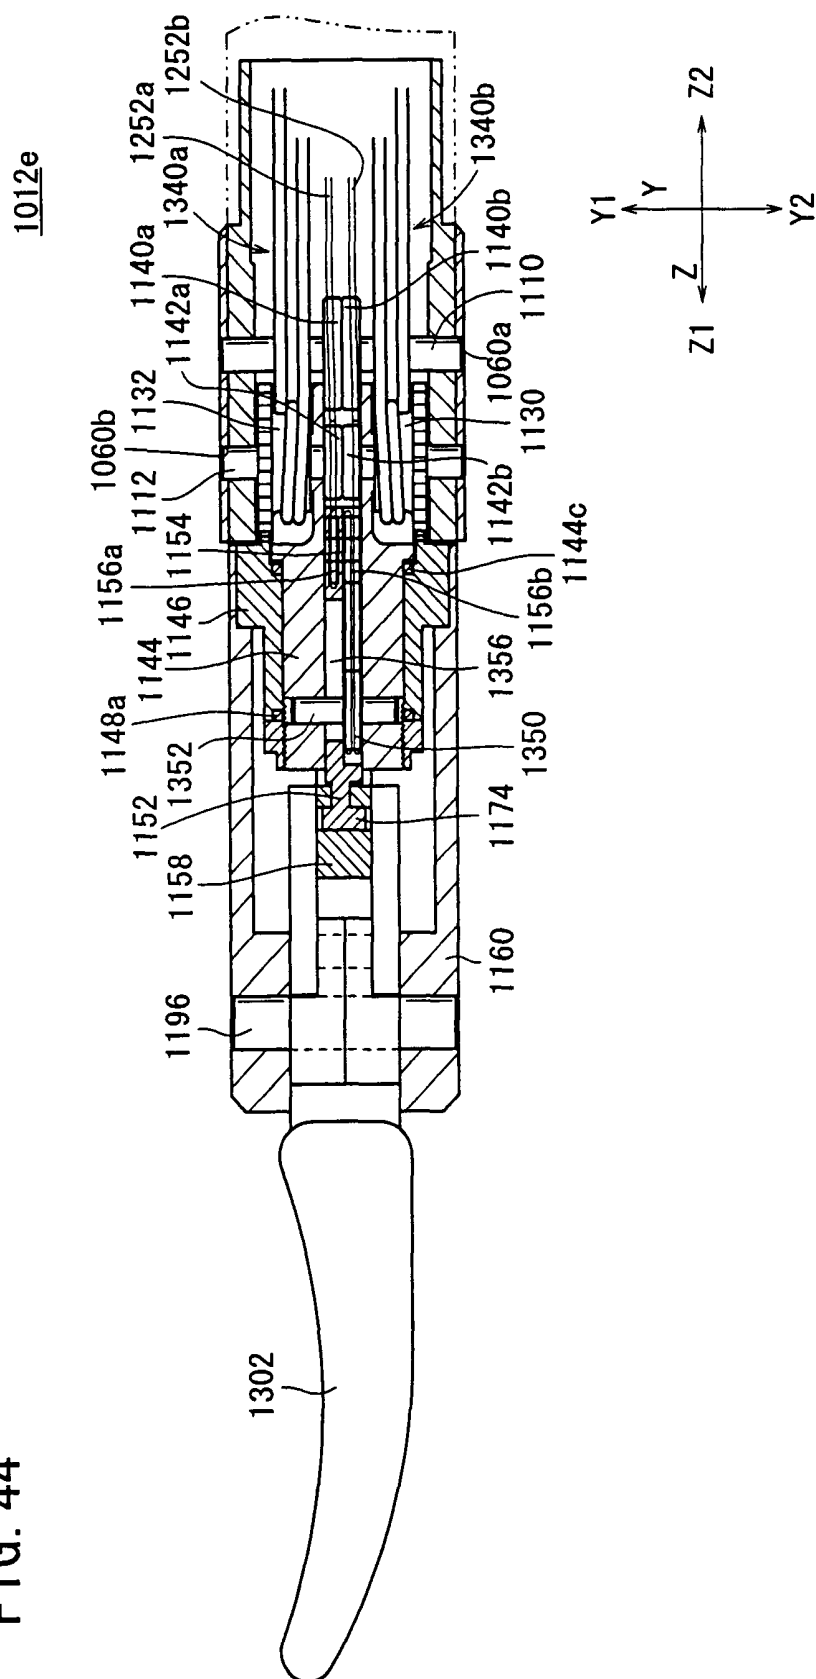


FIG. 45

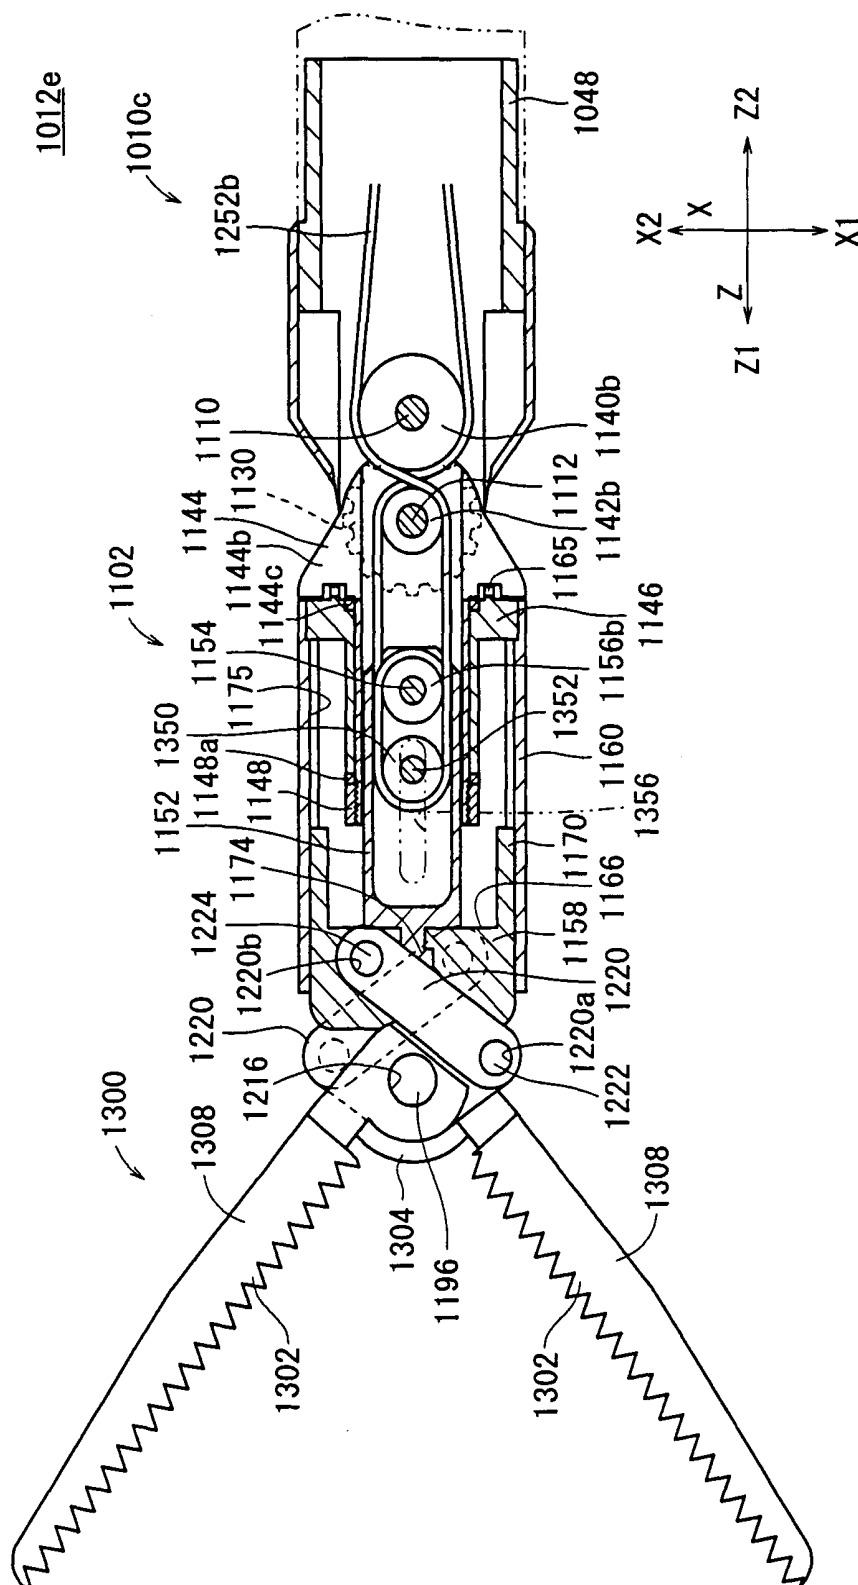
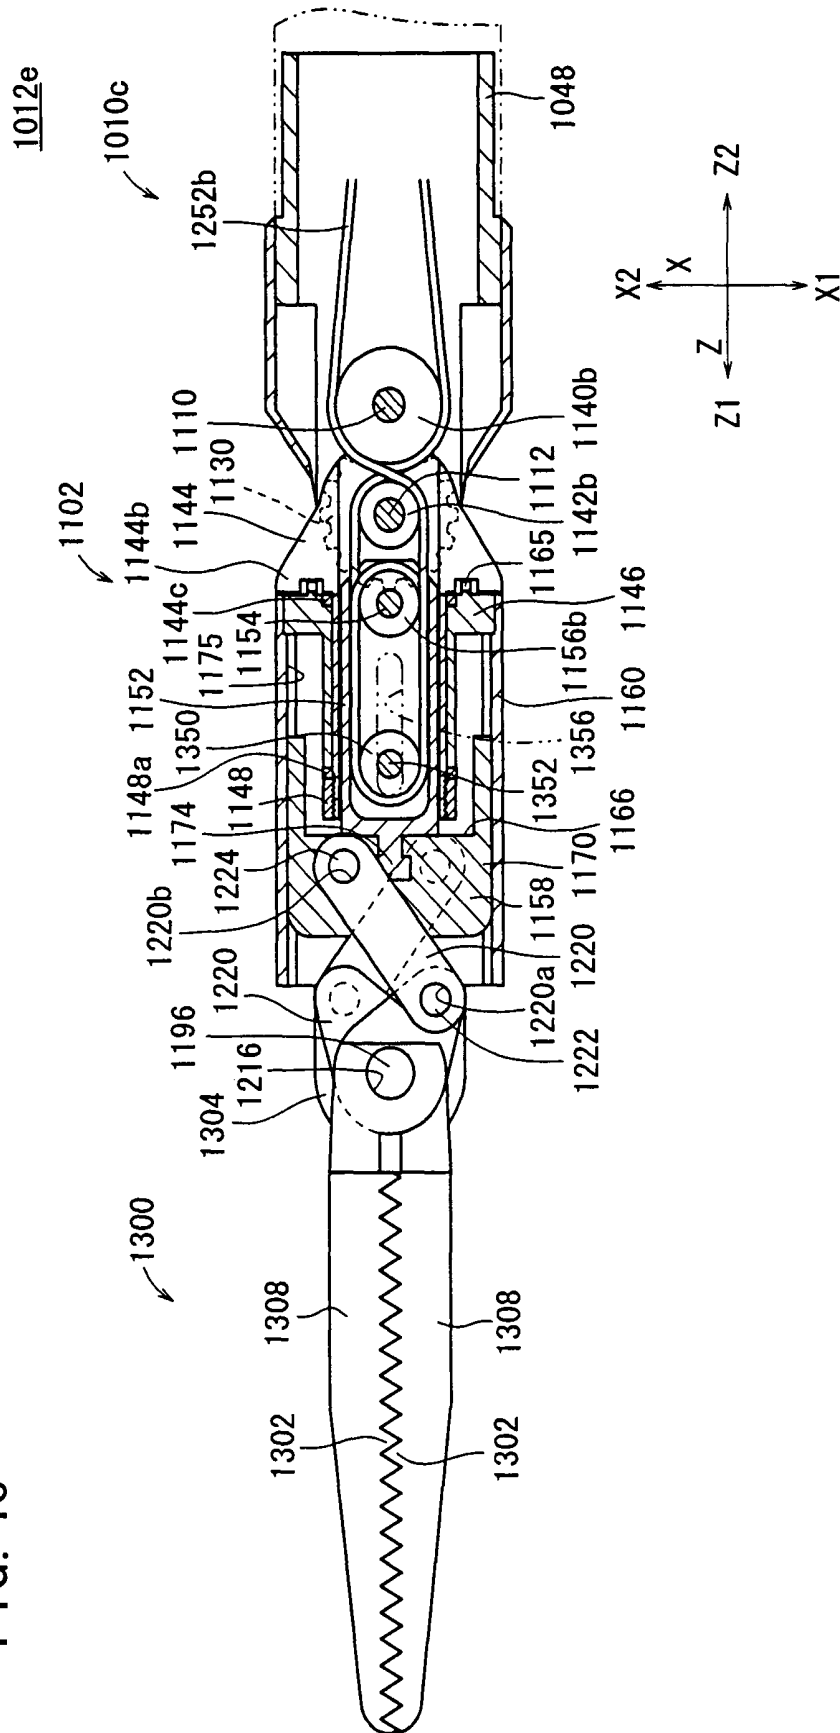


FIG. 46



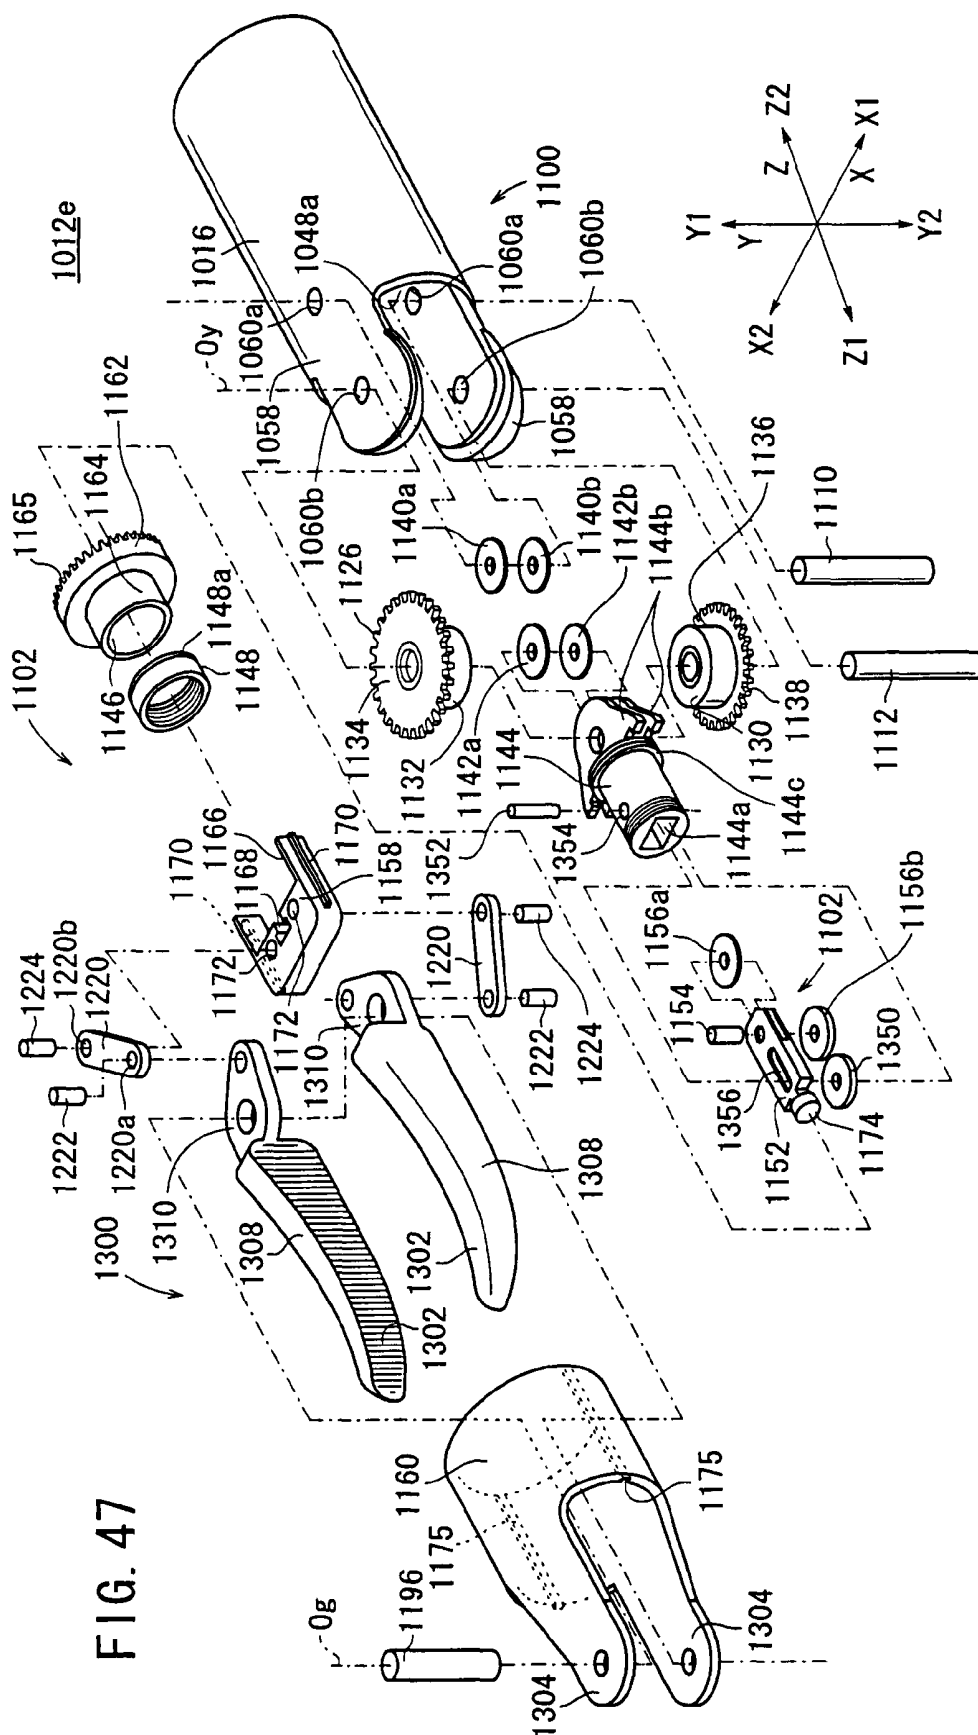


FIG. 48

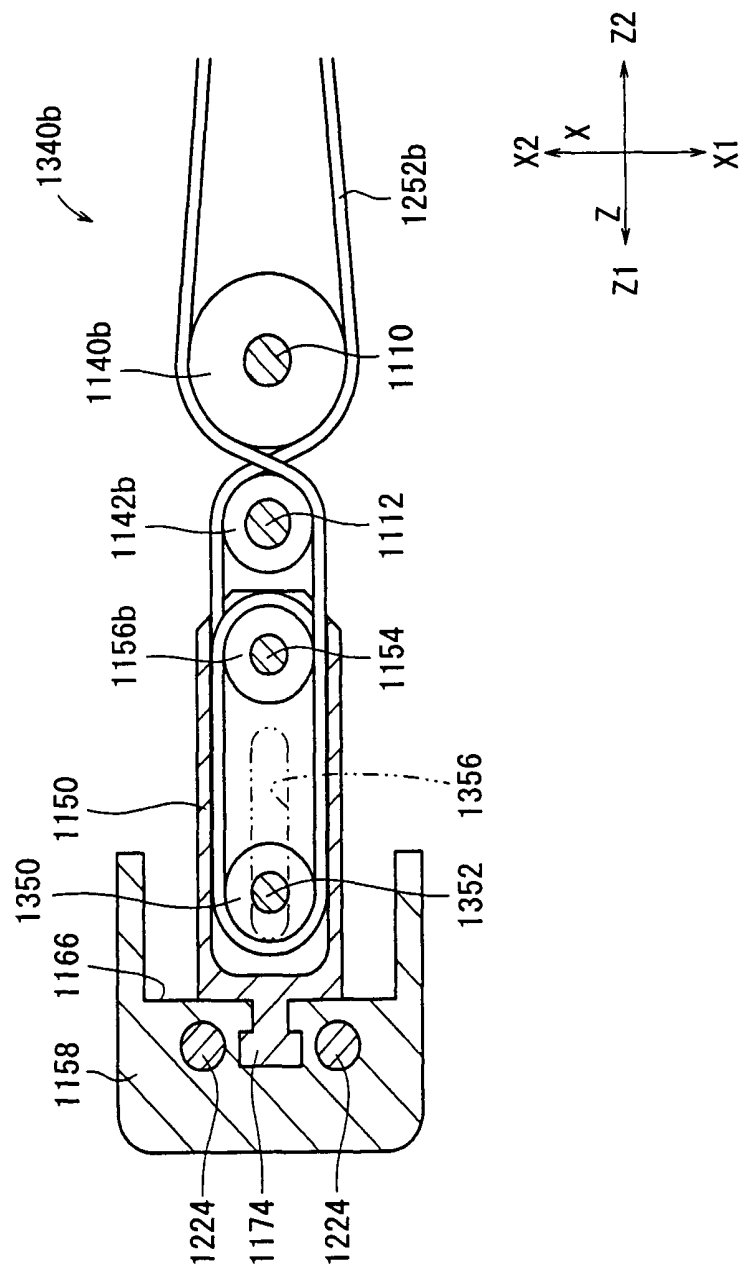


FIG. 49

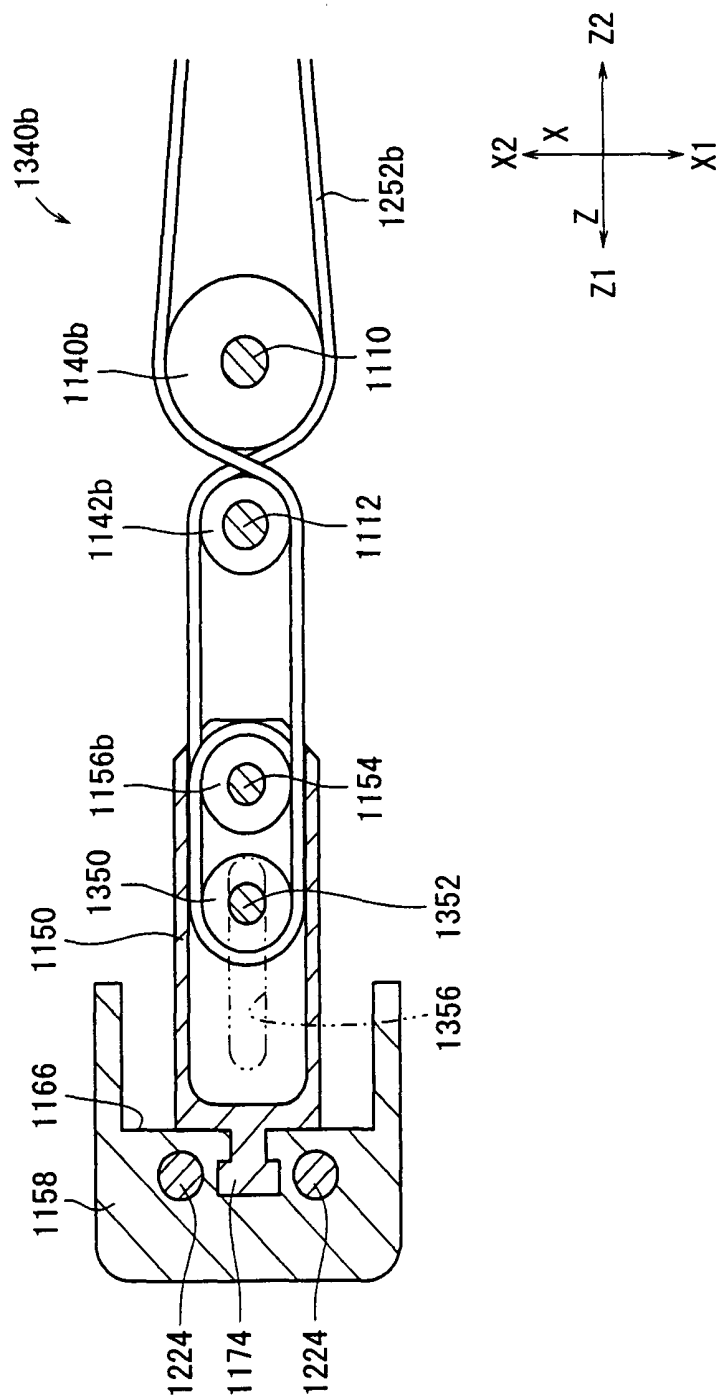


FIG. 50

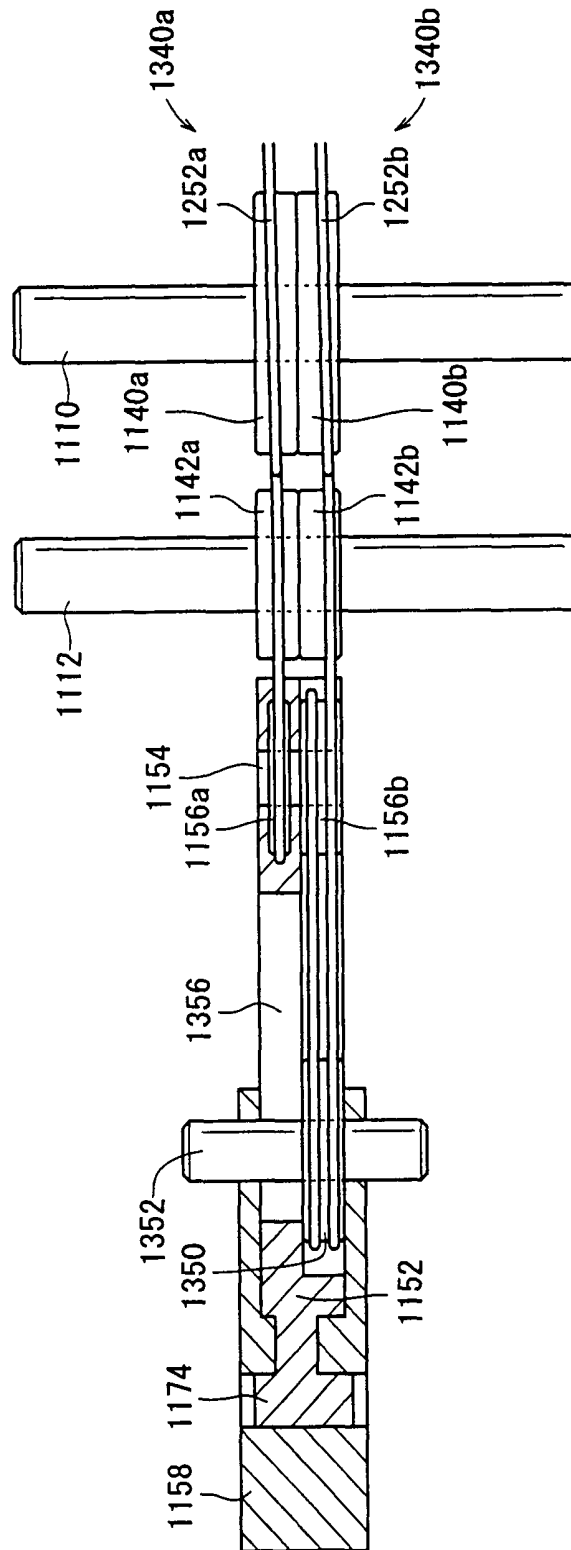


FIG. 51

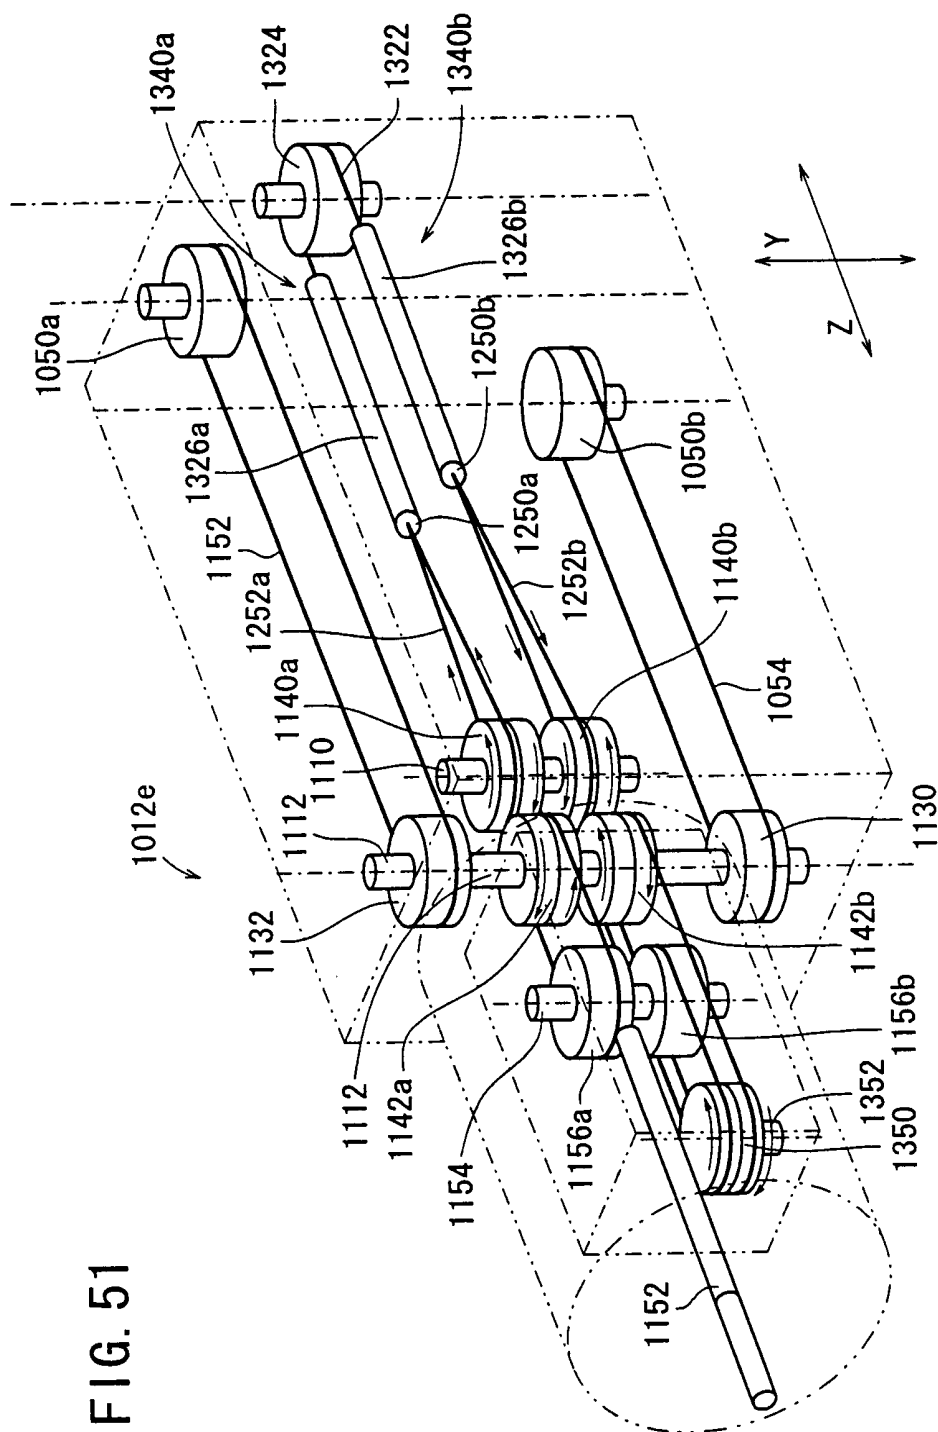


FIG. 52

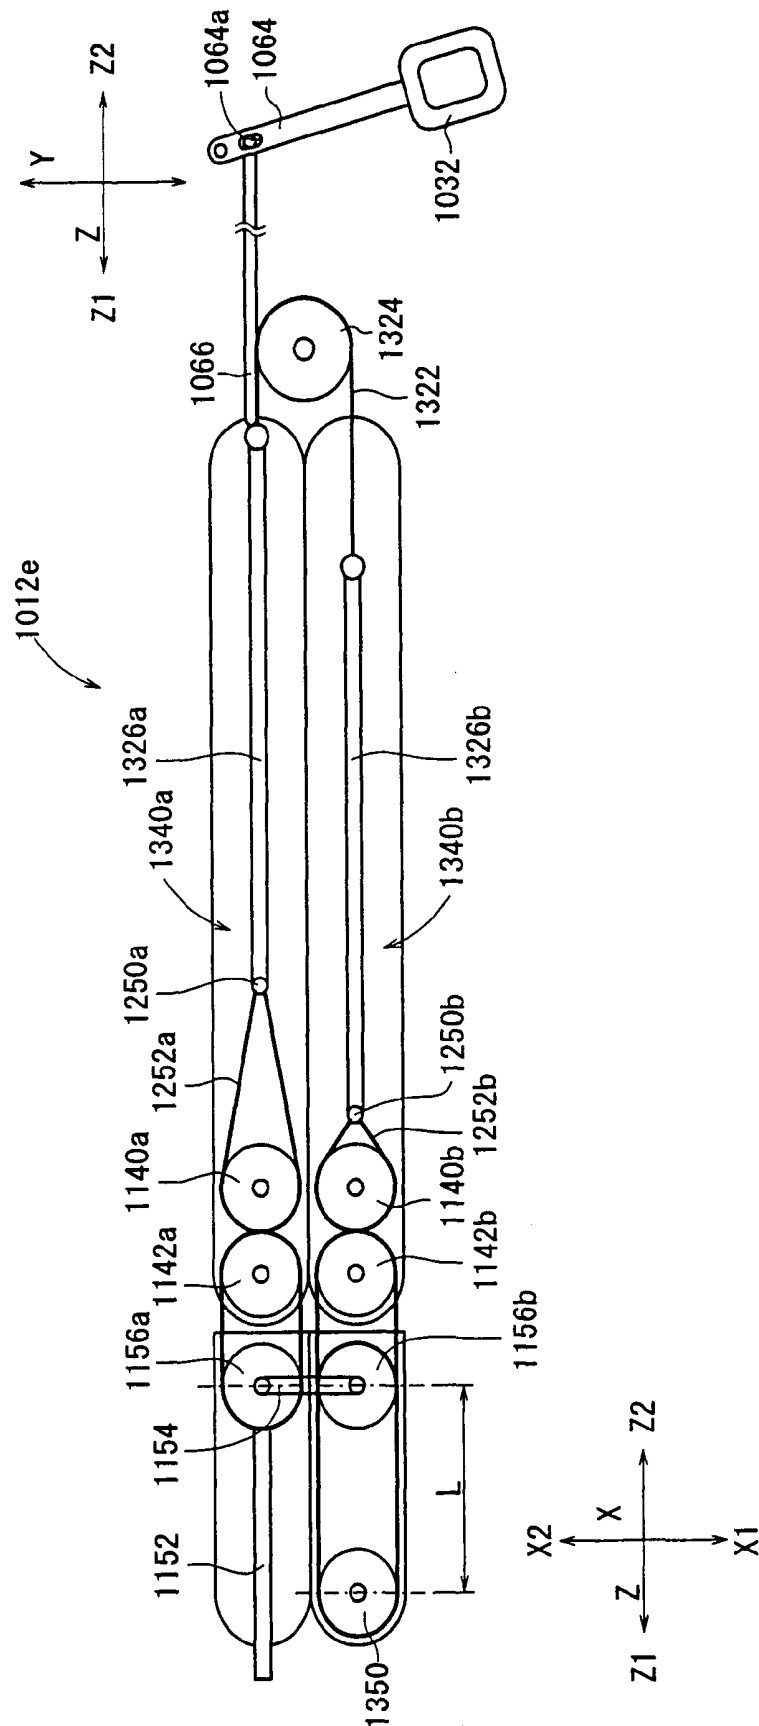


FIG. 53

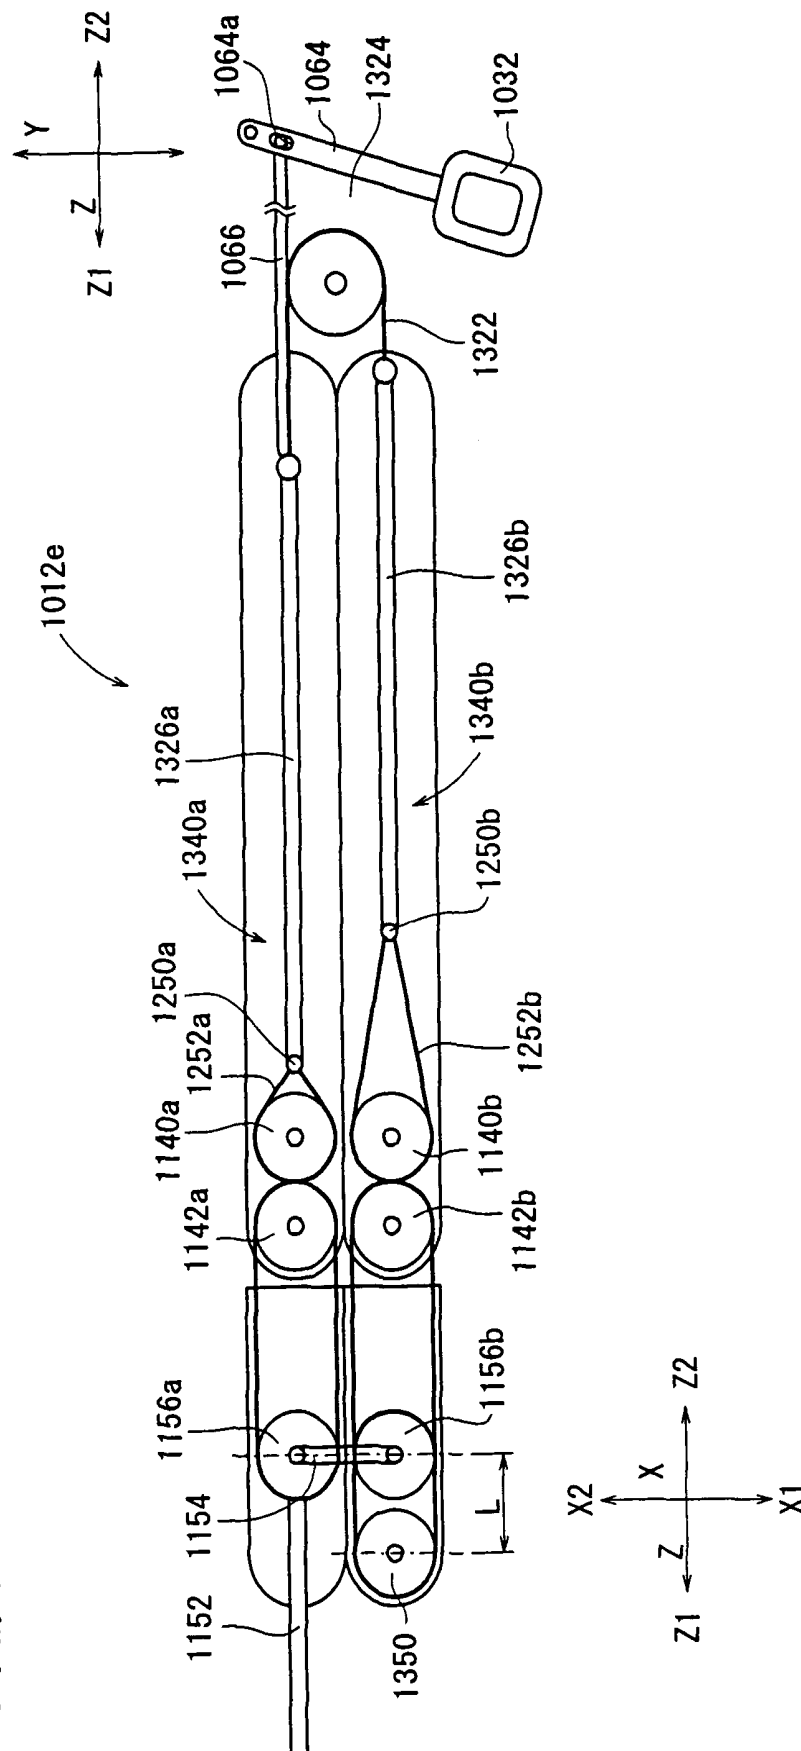


FIG. 54

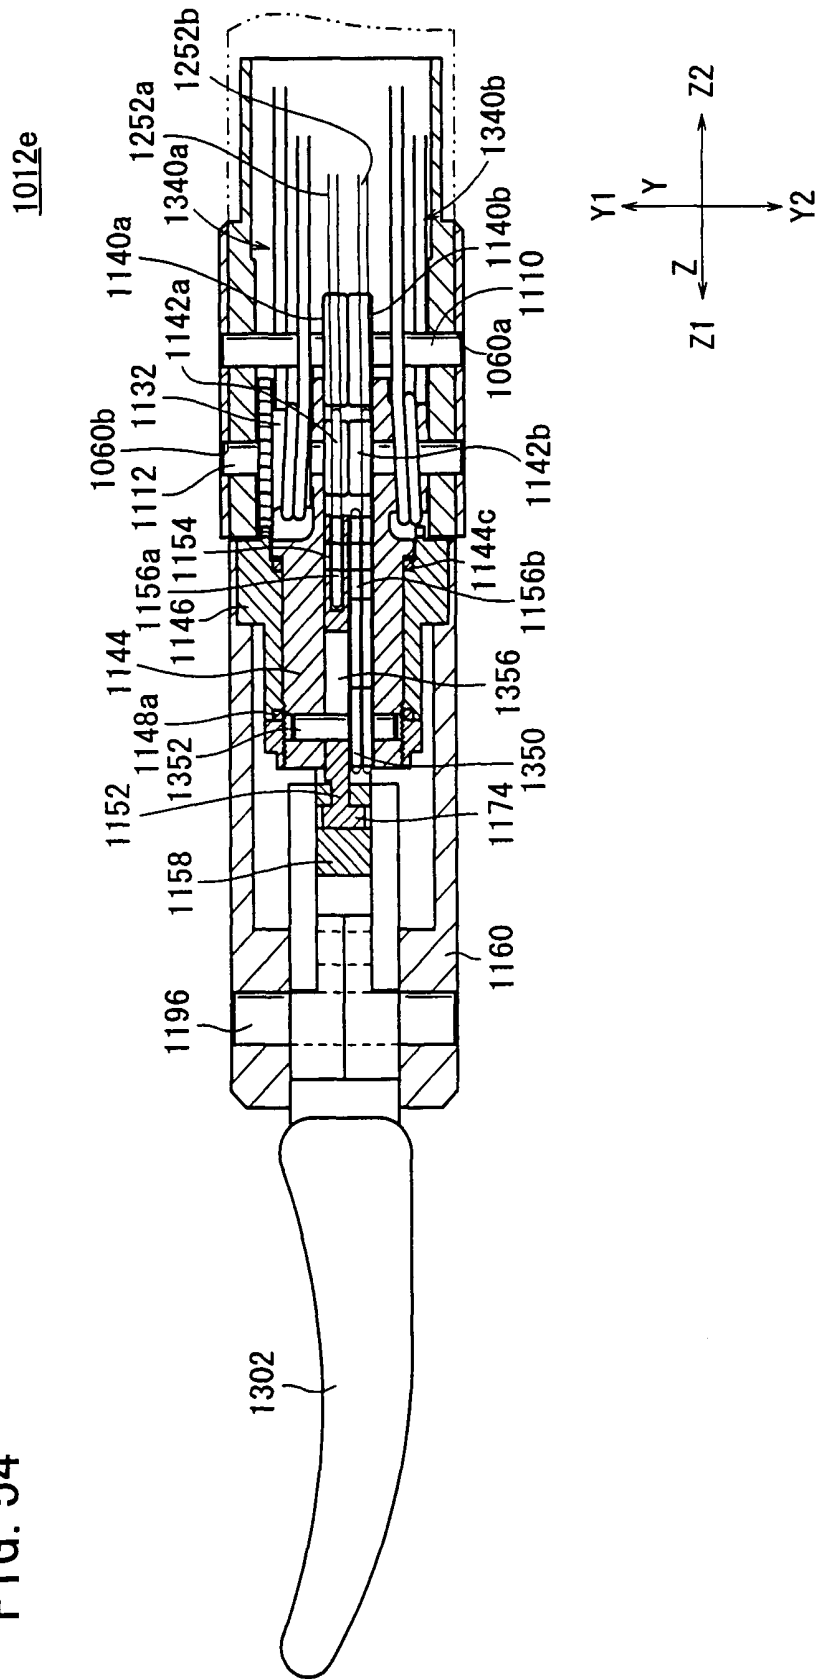


FIG. 55

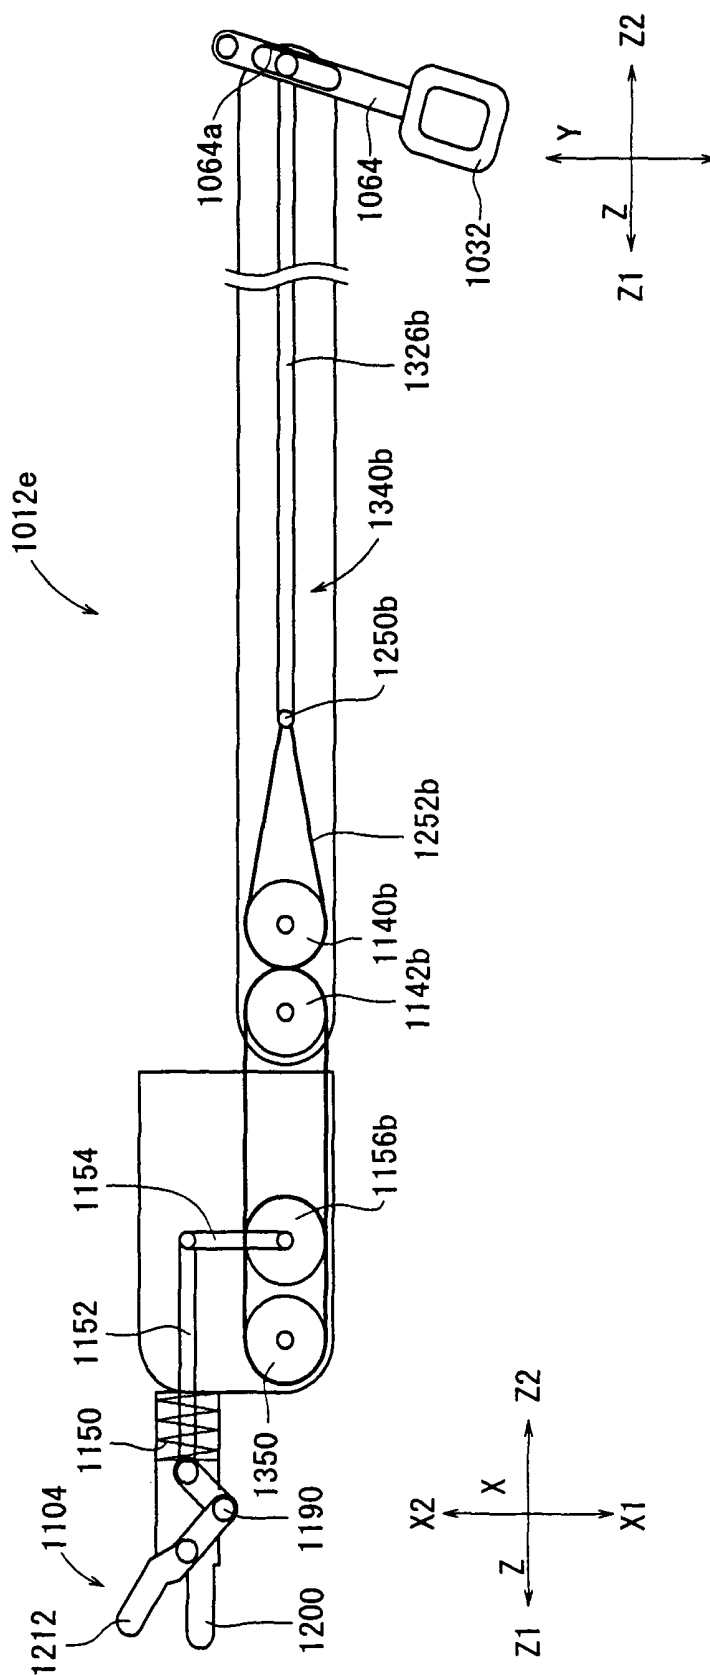


FIG. 56A

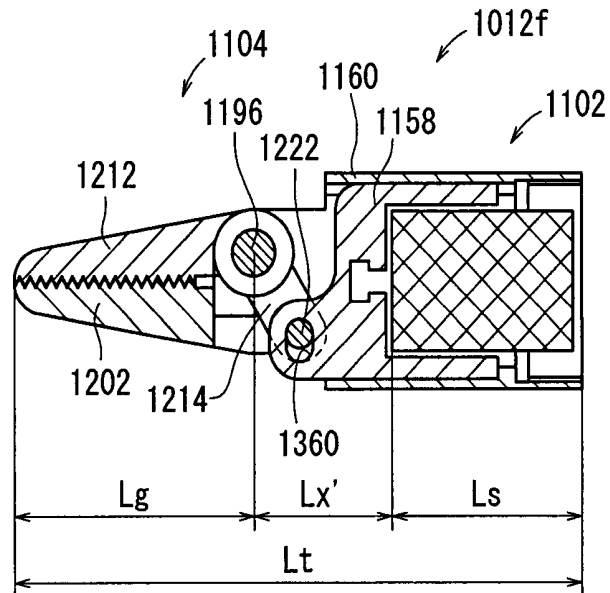


FIG. 56B


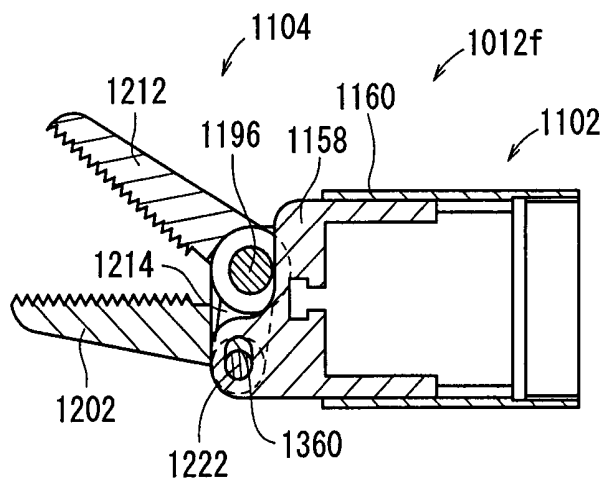


FIG. 57

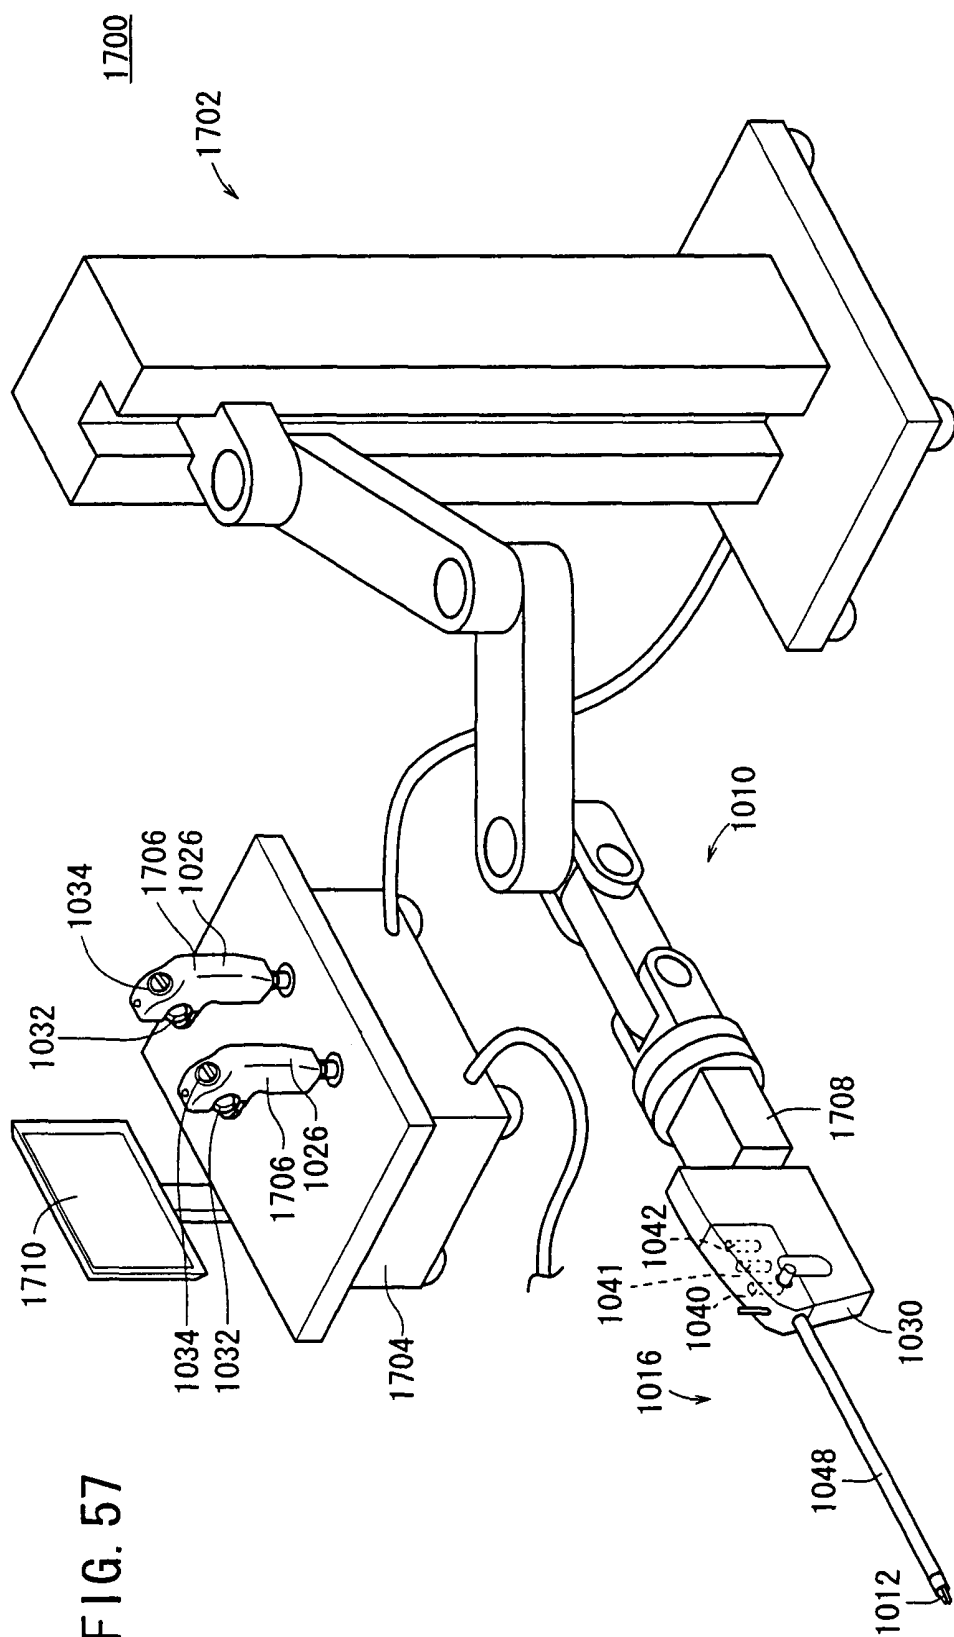

MANIPULATOR FOR MEDICAL USE**BACKGROUND OF THE INVENTION****Field of the Invention**

The present invention relates to a medical manipulator for use in laparoscopic surgery, for example.

Description of the Related Art

In recent years, attention has been drawn to laparoscopic surgery for removal of the appendix and gall bladder, without opening the abdominal cavity, rather than abdominal surgery. During laparoscopic surgery, it is customary to insert four trocars, for example, through the abdominal wall and into the abdominal cavity, to monitor the abdominal cavity with a small camera inserted through one of the trocars, and to manipulate forceps, scissors, an electrosurgical knife, etc., inserted through the other trocars in order to perform a surgical operation on the affected part in the abdominal cavity.

The applicant has proposed a surgical instrument (medical manipulator) for use in such laparoscopic surgery. The proposed surgical instrument comprises a long instrument body and a tip end portion, which can be rotated with respect to the long instrument body, for bringing a medical working unit on the tip end portion into a desired attitude while keeping the medical working unit close to a body region to be surgically treated. For details, reference should be made to Japanese Patent No. 3421117.

The medical manipulator is required to allow the surgeon to perform various appropriate techniques quickly depending on the position and size of the affected part, for removing, suturing, and tying-knot the affected part. According to Japanese Laid-Open Patent Publication Nos. 2002-102248 and 2004-301275, there have been proposed medical manipulators, which can be manipulated simply, with a high degree of freedom.

The medical manipulator disclosed in Japanese Patent No. 3421117, for example, allows the operator to manipulate a rotary manipulating member to directly rotate the medical working unit on the tip end portion. It has been desired that the medical manipulator be operable with greater ease, in order to perform appropriate techniques quickly depending on the position and size of the affected part.

SUMMARY OF THE INVENTION

It is a general object of the present invention to provide a medical manipulator that can be operated with greater ease.

According to an embodiment of the present invention, there is provided a medical manipulator comprising a distal end working unit including an end effector, an operating unit for operating the distal end working unit, a coupling interconnecting the distal end working unit and the operating unit, and an attitude changing mechanism for changing an attitude of the distal end working unit, wherein the end effector is mechanically operated by a transmitting member when the operating unit is operated by the operator, and wherein the attitude changing mechanism is operated by an actuator which is operated when the operating unit is operated by the operator.

With the above structure, the end effector is opened, closed, turned, and otherwise operated mechanically manually by the operator, and the attitude of the distal end working unit is changed by the actuator, which operates the attitude changing mechanism. Therefore, while the end effector can easily and reliably be operated to treat an affected region with desired gripping forces, the attitude of

the end effector can quickly and easily be changed by the actuator. The operability of the medical manipulator can thus be increased. In other words, the medical manipulator can easily be operated to open, close, turn, and otherwise operate the end effector, and also to change the attitude of the distal end working unit, whereby the operability of the medical manipulator is increased.

The attitude changing mechanism may comprise a bending mechanism for bending a portion of the coupling, and a rotating mechanism for rotating the distal end working unit about an axis. The rotating mechanism is capable of rotating the distal end working unit about a bent axis when the distal end working unit is bent out of parallelism with an axis of the coupling by the bending mechanism.

If the coupling is detachably mounted on the operating unit, then the distal end working unit, depending on the type of the end effector, can be replaced on the single operating unit. Also, the coupling and the distal end working unit can be sterilized at a high temperature. The medical manipulator can thus have increased versatility and maintainability.

If the operating unit includes a handle that is angularly movable by the operator to move the transmitting member back and forth, then the operability of the medical manipulator for opening and closing the end effector is increased.

The transmitting member may include a flexible member and a cylindrical member around which the flexible member is wound. The cylindrical member around which the flexible member is wound provides a simple and lightweight structure for allowing the attitude of the attitude changing mechanism to be changed so as to not interfere with the state of the end effector.

The attitude changing mechanism may include a rotational shaft comprising a cylindrical member, and the transmitting member may include a flexible member having a portion wound around the cylindrical member, whereby the transmitting member operates the end effector through the flexible member. The flexible member that is wound around the cylindrical member provides a simple and lightweight structure for actuating the end effector through the flexible member, and for changing the attitude of the attitude changing mechanism so as not to interfere with the state of the end effector, using the cylindrical member as the rotational shaft.

The above and other objects, features, and advantages of the present invention will become more apparent from the following description when taken in conjunction with the accompanying drawings in which preferred embodiments of the present invention are shown by way of illustrative example.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a side elevational view showing an overall structure of a medical manipulator according to an embodiment of the present invention;

FIG. 2 is an enlarged side elevational view, partly in cross section, of a distal end portion of the medical manipulator shown in FIG. 1;

FIG. 3 is an enlarged side elevational view, partly in cross section, of the distal end portion, with a gripper being opened from the state shown in FIG. 2;

FIG. 4 is an enlarged side elevational view, partly in cross section, of an operating unit of the medical manipulator shown in FIG. 1;

FIG. 5 is an enlarged side elevational view, partly in cross section, of the operating unit, with the gripper being opened from the state shown in FIG. 4;

FIG. 6 is a cross-sectional view taken along line VI-VI of FIG. 2;

FIG. 7 is a cross-sectional view taken along line VII-VII of FIG. 5;

FIG. 8 is a front elevational view, partially omitted from illustration, as viewed in the direction indicated by the arrow VIII in FIG. 4;

FIG. 9 is an exploded perspective view showing a structural example of a bending mechanism for bending a curvable portion of a coupling;

FIG. 10 is an exploded perspective view showing a portion of a structural example of the curvable portion of the coupling;

FIG. 11 is a side elevational view of the medical manipulator shown in FIG. 1, which is separated at the coupling;

FIG. 12 is a perspective view of a linear body of a transmitting member, which is separated at a connector;

FIG. 13 is a side elevational view showing another structural example of the medical manipulator shown in FIG. 1;

FIG. 14 is an enlarged side elevational view, partly in cross section, showing another structural example of the distal end portion of the medical manipulator shown in FIG. 1;

FIG. 15 is a side elevational view of a medical manipulator according to another embodiment of the present invention;

FIG. 16 is a plan view of the medical manipulator shown in FIG. 15;

FIG. 17 is a sectional side elevational view of a distal end working unit according to a first structural example;

FIG. 18 is a sectional plan view of the distal end working unit according to the first structural example;

FIG. 19 is a sectional side elevational view of the distal end working unit according to the first structural example, with a gripper being closed;

FIG. 20 is an exploded perspective view of the distal end working unit according to the first structural example;

FIG. 21 is a schematic structural view of the distal end working unit according to the first structural example;

FIG. 22 is a schematic side elevational view of the distal end working unit according to the first structural example, with a trigger lever being in a non-operated state;

FIG. 23 is a schematic side elevational view of the distal end working unit according to the first structural example, with the trigger lever being fully pulled;

FIG. 24 is a schematic side elevational view of the distal end working unit according to the first structural example, with the trigger lever being pulled to an intermediate position;

FIG. 25 is a schematic side elevational view of the distal end working unit according to the first structural example, with a roll axis being operated in one direction;

FIG. 26 is a schematic view of a connected portion of an end of a passive wire according to a first modification;

FIG. 27 is a schematic view of a connected portion of an end of a passive wire according to a second modification;

FIG. 28 is a schematic plan view of a connected portion of an end of a passive wire according to a third modification;

FIG. 29 is a schematic sectional side elevational view of the connected portion of the end of the passive wire according to the third modification;

FIG. 30 is a schematic sectional plan view of a connected portion of an end of a passive wire according to a fourth modification;

FIG. 31 is a schematic sectional side elevational view of the connected portion of the end of the passive wire according to the fourth modification;

FIG. 32 is a schematic structural view of a distal end working unit according to a second structural example;

FIG. 33 is a sectional side elevational view of a distal end working unit according to a third structural example;

FIG. 34 is a sectional side elevational view of the distal end working unit according to the third structural example, with a gripper being closed;

FIG. 35 is a schematic side elevational view of the distal end working unit according to the third structural example, with a roll axis being operated in one direction;

FIG. 36 is a schematic side elevational view of a distal end working unit according to a fourth structural example, with a trigger lever being pushed out;

FIG. 37 is a schematic side elevational view of the distal end working unit according to the fourth structural example, with the trigger lever being fully pulled;

FIG. 38 is a schematic structural view of a distal end working unit according to a fourth structural example;

FIG. 39 is an enlarged perspective view of an idle pulley and a guide pulley of the distal end working unit according to the fourth structural example;

FIG. 40 is a schematic view of a drive member advancing and retracting mechanism according to a first example;

FIG. 41 is a schematic view of a drive member advancing and retracting mechanism according to a second example;

FIG. 42 is a schematic view of a drive member advancing and retracting mechanism according to a third example;

FIG. 43 is a schematic view of a drive member advancing and retracting mechanism according to a fourth example;

FIG. 44 is a sectional side elevational view of a distal end working unit according to a fifth structural example;

FIG. 45 is a sectional plan view of the distal end working unit according to the fifth structural example;

FIG. 46 is a sectional side elevational view of the distal end working unit according to the fifth structural example, with a gripper being closed;

FIG. 47 is an exploded perspective view of the distal end working unit according to the fifth structural example;

FIG. 48 is a plan view, partly in cross section, of a second end effector drive mechanism with a trigger lever being pushed out;

FIG. 49 is a plan view, partly in cross section, of the second end effector drive mechanism with the trigger lever being fully pulled;

FIG. 50 is a side elevational view, partly in cross section, of the second end effector drive mechanism with the trigger lever being pushed out;

FIG. 51 is a schematic structural view of the distal end working unit according to the fifth structural example;

FIG. 52 is a schematic side elevational view of the distal end working unit according to the fifth structural example, with the trigger lever being fully pulled;

FIG. 53 is a schematic side elevational view of the distal end working unit according to the fifth structural example, with the trigger lever being pushed out;

FIG. 54 is a sectional side elevational view of a distal end working unit according to a first modification of the fifth structural example;

FIG. 55 is a sectional side elevational view of a distal end working unit according to a second modification of the fifth structural example;

FIG. 56A is a schematic sectional side elevational view of a distal end working unit, with a gripper link portion thereof being omitted from illustration;

FIG. 56B is a schematic sectional side elevational view of the distal end working unit, with the gripper link portion thereof being omitted from illustration, and with a gripper being opened; and

FIG. 57 is a schematic perspective view of a surgical robot system with a working unit connected to the distal end of a robot arm.

DESCRIPTION OF THE PREFERRED EMBODIMENTS

Preferred embodiments of medical manipulators according to the present invention will be described in detail below with reference to the accompanying drawings.

FIG. 1 is a side elevational view showing an overall structure of a medical manipulator 10 according to an embodiment of the present invention. According to the present embodiment, the medical manipulator 10 will be described for use as a forceps, which is used mainly in laparoscopic surgery. However, the present invention is applicable to various surgical instruments such as pincers, and electric electrosurgical knives, for example, other than forceps. In the following description, the right hand end of the medical manipulator 10 shown in FIG. 1 will be referred to as a proximal end, and the left hand end as a distal end, as well as in the other figures.

The medical manipulator 10 comprises a distal end working unit 14 having a gripper 22 on its distal end as an end effector for performing a surgical operation on the affected part, a working unit (main manipulator body) 15 including an elongate small-diameter coupling 12 coupled to a proximal end of the distal end working unit 14, an operating unit 16 coupled to a proximal end of the coupling 12, and an elongate transmitting member 18 (see FIG. 2) extending through the coupling 12 and connecting the distal end working unit 14 and the operating unit 16 to each other. A controller 20 serving as a control unit for driving and controlling various actuators housed in the medical manipulator 10 is connected to the operating unit 16.

FIG. 2 is an enlarged side elevational view, partly in cross section, of the distal end working unit 14 of the medical manipulator 10 shown in FIG. 1, showing a condition in which the gripper 22 on the distal end working unit 14 is closed. FIG. 3 is an enlarged side elevational view, partly in cross section, with the gripper 22 being opened from the state shown in FIG. 2. FIG. 4 is an enlarged side elevational view, partly in cross section, of the operating unit 16 of the medical manipulator shown in FIG. 1, showing a condition in which the gripper 22 on the distal end working unit 14 is closed. FIG. 5 is an enlarged side elevational view, partly in cross section, with the gripper 22 being opened from the state shown in FIG. 4.

The coupling 12 comprises a hollow elongate small-diameter member having a space 24 formed therein, which accommodates the transmitting member 18, etc. A joint (an attitude changing mechanism, a rotating mechanism) 26 rotatably coupled to the distal end working unit 14 is disposed on a distal end of the coupling 12 (see FIGS. 1 and 2). The coupling 12 has a proximal end coupled to a main operating unit body 28 of the operating unit 16 (see FIGS. 1 and 4).

The coupling 12 has a transverse cross-sectional shape (a cross-sectional shape perpendicular to the axial direction thereof), which may be a circular shape, an elliptical shape, a polygonal shape, or the like, and is not limited to any particular shape. In the present embodiment, as shown in FIG. 6, the coupling 12 has a circular transverse cross-

sectional shape, and has an outside diameter that enables the coupling to be inserted into a trocar (not shown), e.g., in the range of from 5 to 10 mm.

In the present embodiment, the coupling 12 has a straight shape, as shown in FIG. 1, but the coupling 12 may be curved or bent in any desired shape. The coupling 12 has at least one curvable portion (an attitude changing mechanism, a bending mechanism) 30, which can be curved (bent) to a desired shape (see FIG. 1), for increasing the range at which a living tissue can be surgically treated with the gripper 22, and for making it possible to perform a surgical treatment at a proper attitude.

The transmitting member 18 that extends through the coupling 12 comprises a linear body 32, a first coupling member 34 coupled to a proximal end of the linear body 32, and a rod-shaped second coupling member 36 coupled to a distal end of the linear body 32. The linear body 32 has a connector 37 (see FIGS. 4 and 12) positioned near to a detachable joint 35 by which the coupling 12 and the operating unit 16 are detachably joined to each other. The connector 37 allows a distal end portion 32a and a proximal end portion 32b to be detachably joined to each other. The distal end portion 32a extends into the distal end working unit 14, and the proximal end portion 32b extends into the main operating unit body 28 (see FIGS. 2 and 4).

The linear body 32 should preferably be flexible (bendable) over its entire length or over a portion thereof, at least a portion thereof corresponding to the curvable portion 30. The linear body 32 may comprise wires such as metal wires made of stainless steel, tungsten, superelastic alloy, or the like, piano wires, ropes, chains, or the like, or fibers made of a polymeric material that can withstand relatively high tension, such as polyamide (wholly aromatic polyamide), polyester, ultrahigh molecular weight polyethylene, carbon fibers (hereinafter referred to as high-tension fibers), or a cluster of any of such wires, or other composites. The straight portion, other than the portion that corresponds to the curvable portion 30, may comprise a rigid non-flexible body. The linear body 32, in the form of a cluster of wires, should preferably be made up of one or more wires (particularly metal wires), having one or more wires of the same or different types wound (e.g., helically) around the wires, and one or more wires of the same or different types wound therearound in a direction opposite to the last-mentioned one or more wires. The linear body thus constructed is advantageous in that it is excellent in following a pulling action of the operating unit 16, while suppressing a change in length (distortion) due to twisting and bending when the linear body 32 is rotated. The outside diameter of the linear body 32 is not limited to any particular value, but may preferably be in the range of from about 1.0 to 2.5 mm, particularly in the range of from about 1.0 to 1.5 mm, according to the present embodiment.

As shown in FIGS. 2 and 6, the second coupling member 36 has a square transverse cross-sectional shape. The joint 26 includes a protrusion 38 having a passage 40 formed centrally therein. The second coupling member 36 is slidably inserted inside the passage 40. The passage 40 has a transverse cross-sectional shape that is substantially identical to the transverse cross-sectional shape of the second coupling member 36. The second coupling member 36 has a distal end portion extending into the distal end working unit 14, and which is coupled to or integrally combined with the proximal end of a slider 44, described later.

The transverse cross-sectional shape of the second coupling member 36 may be a noncircular shape, e.g., a triangular shape, a hexagonal shape, a semicircular shape, a

straight-line shape, a crisscross shape, an L shape, or the like, rather than a square shape, for preventing the second coupling member 36 from rotating with respect to the passage 40. The second coupling member 36 may be made of a metal material such as aluminum, brass, stainless steel, tungsten, carbon steel, a superelastic alloy, or the like, or from a relatively hard resin such as polycarbonate, polyethylene, polypropylene, hard polyvinyl chloride, polyester, or the like, or the high-tension fibers described above.

As shown in FIGS. 2 and 3, the distal end working unit 14 includes a gripper 22 as an end effector for treating the affected part, and a coil spring 46 for biasing the slider 44 to move in one direction (toward the distal end). The gripper 22 serves as a forceps mechanism for gripping a living tissue, and includes a pair of openable/closable members, one of which is movable, i.e., a fixed pinching member 48 and a movable pinching member 50 that is angularly movable with respect to the fixed pinching member 48. The movable pinching member 50 has a proximal end angularly movably mounted on a main distal end body 54 by a pin 52. Although the gripper 22 has only one of its pinching members openable in the present embodiment, both of the pinching members thereof may be openable.

The main distal end body 54 has a recess 56 formed in a lower portion thereof (i.e., the lower portion as shown in FIG. 2). The slider 44 is disposed in the recess 56 so as to be slidable in the longitudinal direction of the distal end working unit 14. The slider 44 has a pin 58 projecting on a distal end thereof, which is inserted in an oblong hole 60 that is formed in a lower portion of the proximal end of the movable pinching member 50.

When a handle unit 62, described later, is operated to pull the transmitting member 18 toward the proximal end so as to position the slider 44 in the proximal end portion of the recess 56, the fixed pinching member 48 and the movable pinching member 50 are in a closed position (see FIG. 2). When the gripping force on the handle unit 62 is reduced or removed, the transmitting member 18 is moved toward the distal end, thereby moving the slider 44 toward the distal end of the recess 56. The pin 58 presses an inner peripheral surface of the oblong hole 60, turning and opening the movable pinching member 50 about the pin 52 (see FIG. 3). The oblong hole 60 may be dispensed with, and as the slider 44 moves, the slider 44 may be distorted to absorb the vertical movement in FIG. 2 of the pin 58.

The coil spring 46 is housed in a compressed state within a recess 64 formed in the main distal end body 54 and a recess 66 formed in the slider 44. The coil spring 46 comprises a biasing means for biasing the slider 44 toward the distal end under a resilient force thereof, i.e., for biasing the movable pinching member 50 in an opening direction. Since the medical manipulator 10 according to the present embodiment includes the coil spring 46 as the biasing means in the distal end working unit 14, it is unnecessary to provide a leaf spring or the like inside the handle unit 62 for biasing a movable handle 68 in an opening direction, for example. Thus, the operating unit 16 is simple in structure for enabling better operability.

As shown in FIGS. 2 and 3, the joint 26 includes a recess 70 having a circular transverse cross-sectional shape, which communicates with the space 24 in the coupling 12 and which is open at the distal end face of the coupling 12. The protrusion 38 has a circular transverse cross-sectional shape, which projects from the proximal end of the main distal end body 54 and is inserted into the recess 70.

The protrusion 38 includes the passage 40 formed axially centrally therein and having a transverse cross-sectional

shape, which is substantially identical to the transverse cross-sectional shape of the second coupling member 36. When the second coupling member 36 is inserted in the passage 40, the rotational force of the transmitting member 18 can be transmitted to the protrusion 38 and the main distal end body 54.

Two ring-shaped grooves 74, which are axially spaced from each other by a predetermined distance, are formed in the inner circumferential surface of the recess 70. The protrusion 38 has two ring-shaped lands 75 extending circumferentially at respective positions corresponding to the grooves 74. The lands 75 are inserted respectively into the grooves 74. The lands 75 are not limited to having continuous ring shapes, but may be disposed intermittently in the circumferential direction.

The joint 26 of the above structure allows the distal end working unit 14 to rotate (roll) with respect to the coupling 12, but makes the distal end working unit 14 unable to move axially. Therefore, the joint 26 is reliably capable of preventing the distal end working unit 14 from becoming dislodged or experiencing wobbling. The joint 26 may have a rotational resistance reducing means (not shown) for reducing the rotational resistance of the distal end working unit 14. According to a specific example, the rotational resistance reducing means may comprise a lubricant, such as lubricating oil or a layer of a low-friction material such as polytetrafluoroethylene, silicone, polyethylene, polyacetal, or the like, interposed between the recess 70 and the protrusion 38. The rotational resistance reducing means allows the distal end working unit 14 to rotate more smoothly.

As shown in FIGS. 1, 4, and 5, the operating unit 16 is mounted on the proximal end of the coupling 12 for remotely opening and closing (turning) the gripper 22, bending the distal end working unit 14 in the curvable portion 30, and rotating the distal end working unit 14 with respect to the coupling 12.

The operating unit 16 includes the handle unit 62, which comprises a fixed handle 80 fixed to or integrally combined with the main operating unit body 28, and a movable handle 68 which can be opened and closed (turned) with respect to the fixed handle 80. The movable handle 68 has an upper end thereof angularly movably mounted on the main operating unit body 28 by a shaft member 82.

A stopper 84 projects from the outer surface of a lower portion of the main operating unit body 28, for engaging the movable handle 68 so as to limit an angularly movable range thereof, for thereby preventing the transmitting member 18 from being broken when an excessive gripping force is applied to the handle unit 62. As shown in FIG. 13, the fixed handle 80 and the movable handle 68 may be switched in position. According to such a modification, a rotating action input unit 86 and a bending action input unit 128, to be described later, may be placed on an upper portion of the proximal end of the main operating unit body 28, for enabling better operability.

The operating unit 16 has a rotating action mechanism 88 disposed in the proximal end of the main operating unit body 28, which can be actuated by operation of a disk-shaped rotating action input unit 86 (see FIG. 8) mounted on the fixed handle 80.

The rotating action mechanism 88 comprises a rotational drive source (actuator) 90 such as a motor, for example, a small-diameter drive gear 92 coupled to the rotational shaft of the rotational drive source 90, a large-diameter driven gear 94 held in mesh with the drive gear 92, and a bearing 96 by which the driven gear 94 is rotatably supported on the

proximal end of the main operating unit body 28. The rotational drive source 90 is energized under the control of the controller 20, based on operation of the rotating action input unit 86. The driven gear 94 has a rotational shaft 98, comprising a cylindrical portion 98a on its proximal end portion and a prismatic portion 98b on its distal end portion. The cylindrical portion 98a is supported by the bearing 96.

The main operating unit body 28 houses therein a converting means 100 for converting angular movement of the movable handle 68 into longitudinal movement of the transmitting member 18, and transmitting a rotational force produced by rotation of the driven gear 94 to the transmitting member 18. The converting means 100 comprises a support member 102 by which the first coupling member 34 is rotatably supported, and a rotational force transmitting mechanism 104 for transmitting rotational force from the driven gear 94 to the first coupling member 34.

The proximal end portion 32b of the linear body 32 is fixed to the distal end portion of the first coupling member 34 by a pin 106. The first coupling member 34 comprises a hollow cylindrical member having a passage 108 with a square transverse cross-sectional shape formed centrally therein (see FIG. 7), in which the prismatic portion 98b of the rotational shaft 98 of the driven gear 94 is inserted. The first coupling member 34 includes a flange 110 on a proximal end thereof, which engages with the proximal end face of the support member 102.

The support member 102 has a through hole 112 with a circular transverse cross-sectional shape formed therein, in which the first coupling member 34 is inserted. A tongue 116 with an oblong hole 114 formed therein projects from a lower portion of the support member 102. The support member 102 is supported by guide members 118, 120 disposed in the main operating unit body 28, for enabling sliding movement in the longitudinal direction of the transmitting member 18. The tongue 116 projects downwardly through a slit 122 formed in the lower guide member 120.

The movable handle 68 has a projecting member 124 on an upper portion thereof, which is inserted into the main operating unit body 28. A pin 126 mounted on the upper end of the projecting member 124 is inserted into the oblong hole 114 of the tongue 116 (see FIGS. 4 and 7).

The rotational force transmitting mechanism 104 is made up of the prismatic portion 98b of the rotational shaft 98 of the driven gear 94, together with the passage 108 into which the prismatic portion 98b is inserted. The prismatic portion 98b is axially movable with respect to the passage 108, but cannot be rotated with respect to the passage 108 regardless of the depth at which the prismatic portion 98b is inserted into the passage 108. Therefore, the rotational force of the driven gear 94 is transmitted through the prismatic portion 98b and the passage 108 to the first coupling member 34, thereby rotating the transmitting member 18 in its entirety.

The transverse cross-sectional shape of the prismatic portion 98b may be a noncircular shape, e.g., a triangular shape, a hexagonal shape, a semicircular shape, a straight-line shape, a crisscross shape, an L shape, or the like, rather than a square shape, for preventing the prismatic portion 98b from rotating with respect to the passage 108. The rotational force transmitting mechanism 104 comprises a mechanism for mechanically transmitting rotational force from the rotational drive source 90 to the transmitting member 18. The rotational force transmitting mechanism 104 may be actuated by a wire, a chain, a timing belt, a link, a rod, a gear, or the like. Preferably, the rotational force transmitting mechanism 104 is actuated by a mechanical component in the form of a solid body that is nonelastic in the power

transmitting direction. Although a wire, a chain, or the like, is slightly elongatable inevitably under tension, it is still regarded as a mechanical component in the form of a nonelastic solid body. The actuating mechanisms may be used to allow the rotating action mechanism 88 and the distal end working unit 14 to rotate in opposite directions, or at different speeds.

The operating unit 16 has a bending action mechanism 130 disposed on the distal end of the main operating unit body 28, which can be actuated by operation of the bending action input unit 128 for bending the curvable portion 30. The bending action input unit 128 is mounted on the fixed handle 80 and comprises four triangular buttons pointing in upper, lower (front, rear), left, and right directions.

As shown in FIGS. 4, 5, and 9, the bending action mechanism 130 comprises two coil springs 132, 134 projecting from the distal end face of the main operating unit body 28, a pivotal shaft (bearing ball) 136 disposed parallel to the coil springs 132, 134, and a tilt plate (swing plate) 138 coupled to distal ends of the coil springs 132, 134, and spaced a predetermined distance from the distal end face of the main operating unit body 28, in confronting relation thereto. The tilt plate 138 has a hole 138a formed centrally therein, through which there is inserted a protrusion 139 having a substantially hollow cylindrical shape that projects on the distal end of the main operating unit body 28, and which is coupled to the coupling 12.

The bending action mechanism 130 also includes two bending drive sources (actuators) 140, 142 disposed in the main operating unit body 28, comprising geared motors, for example. The bending drive sources 140, 142 have respective drive shafts with respective axially movable screws 140a, 142a coupled thereto. The axially movable screws 140a, 142a are threaded respectively into threaded holes 144, 146 formed in the distal end of the main operating unit body 28, and have distal ends held respectively in abutment against two respective bearing surfaces 148, 150 on diagonally opposite corners of the tilt plate 138.

The bending action mechanism 130 operates as follows: When the bending drive sources 140, 142 are energized under the control of the controller 20, the axially movable screws 140a, 142a are moved axially so as to tilt the tilt plate 138 through a desired angle in desired directions (the directions indicated by the arrows A, B in FIG. 9) about the spherical distal end surface of the pivotal shaft 136, while being resiliently supported by the coil springs 132, 134. Since one of the bearing surfaces 150 is horizontally elongate, even when the tilt plate 138 is in a tilted state, the axially movable screw 142a is reliably held against the bearing surface 150 and the tilt plate 138 can swing smoothly while the other axially movable screw 140a is held against the bearing surface 148. The tilt plate 138 of the bending action mechanism 130 may be tilted using a mechanism that includes a general structure for swinging an optical mirror.

The hole 138a of the tilt plate 138 includes four slits 152 formed in upper, lower, left, and right directions thereof, as shown. Wires 154 are inserted from the inner circumferential portion of the hole 138a into the respective slits 152. The wires 154 have larger-diameter portions 154a on respective proximal ends thereof, which engage the proximal end face of the tilt plate 138. The wires 154 extend through four respective through holes 156 formed axially in the coupling 12, and extend to the curvable portion 30.

FIG. 10 is an exploded perspective view showing a portion of a structural example of the curvable portion 30 of the coupling 12. The curvable portion 30 comprises a

11

plurality of nodal rings **158**, which are joined together and angularly movable with respect to each other. In FIG. **10**, the curvable portion **30** will be described as comprising three nodal rings **158**, for example. However, the curvable portion **30** is not limited to being made up of three nodal rings **158**, but may comprise four through thirty nodal rings **158**.

Each of the nodal rings **158** includes a pair of V-shaped slots **160** formed in one of the surfaces, in diametrically opposite relation to each other across the center of the nodal ring **158**, and a pair of semicylindrical ridges **162** disposed on the other surface, in diametrically opposite relation to each other across the center of the nodal ring **158**. The semicylindrical ridges **162** are angularly displaced by 90° from the slots **160**. Two adjacent nodal rings **158** are oriented such that the slots **160** thereof are angularly displaced from each other by 90°. The nodal rings **158** are joined such that the ridges **162** of one of the nodal rings **158** are inserted into corresponding slots **160** of the other nodal ring **158**.

Each of the nodal rings **158** has through holes **164** formed therein at the slots **160** and the ridges **162**. The four wires **154**, whose larger-diameter portions **154a** engage with the tilt plate **138**, are inserted through the corresponding through holes **164** of the nodal rings **158**. The wires **154** have respective distal ends coupled to the nodal ring **158** disposed in the distal end of the curvable portion **30** (see FIGS. **2** and **3**). In this manner, the nodal rings **158** are placed together and combined substantially integrally with one another.

When the ridges **162** are inserted into the slots **160**, a gap is created between two adjacent nodal rings **158**, thereby allowing the ridges **162** to move angularly within the slots **160** and further allowing the adjacent nodal rings **158** to move angularly with respect to each other. Although the angle through which the adjacent pair of nodal rings **158** is angularly movable is small, the sum of the angles of a plurality of adjacent pairs of nodal rings **158** is large enough so as to allow the entire curvable portion **30** to be curved through a desired angle (e.g., in a range of from 60 to 120°), thus making it possible to bend the distal end working unit **14** (grripper **22**) such that it is not parallel to the longitudinal axis of the coupling **12**.

When the bending action input unit **128** is operated, the bending action mechanism **130** is actuated under the control of the controller **20** to tilt the tilt plate **138** through a desired angle, and to axially move the wires **154** respective distances for thereby bending the curvable portion **30** upwardly, downwardly (forwardly, rearwardly), leftwardly, and rightwardly through desired angles on the transverse cross-sectional plane of the coupling **12**. Specifically, the curvable portion **30** is actively bent or curved when pulled by the tilt plate **138** through the wires **154**. The directions in which the curvable portion **30** is curved, and the number of such directions (the degree of freedom), are not limited to any particular values. Although not shown, the outer circumferential surface of each nodal ring **158** may be covered with a layer made up of an elastic or a flexible material.

The curvable portion **30** is not limited to having the illustrated structure, but may comprise a bellows tube or a flexible tube. The coupling **12** may comprise a hard pipe serving as the distal end portion together with a hard pipe serving as the proximal end portion, wherein the hard pipes are angularly movably connected by a single shaft or a plurality of shafts for bending the curvable portion **30**. Alternatively, the curvable portion **30** may comprise a bending mechanism having a pivot shaft.

As shown in FIG. **11**, in the medical manipulator **10** according to the present embodiment, the operating unit **16**

12

and the coupling **12** are detachably (separably) connected to each other by means of the detachable joint **35**. Specifically, in the detachable joint **35**, by which the coupling **12** and the operating unit **16** are detachably joined to each other, the protrusion **139** that projects on the distal end of the operating unit **16** is inserted into a hole **166** formed in the proximal end of the coupling **12**, and a setscrew **168** is tightened against the protrusion **139** from the outer circumferential surface toward the inner circumferential surface of the coupling **12**, thereby fastening the coupling **12** and the operating unit **16** together (see FIGS. **4** and **5**).

In order to separate the coupling **12** and the operating unit **16** from each other, therefore, the wires **154** are released from the slits **152** of the tilt plate **138**, the setscrew **168** is loosened, and the protrusion **139** of the operating unit **16** is pulled out of the hole **166** of the coupling **12** (see FIG. **11**). At this time, the linear body **32** can easily be divided when the distal end portion **32a** and the proximal end portion **32b** are separated from each other at the connector **37**, by releasing a T-shaped bar **170** on the distal end of the distal end portion **32a** from a T-shaped hook **172** provided on the distal end of the proximal end portion **32b** (see FIG. **12**). Accordingly, various working units **15**, with distal end working units having various end effectors, may easily be replaced and used on a single operating unit **16**, so that the medical manipulator **10** has increased versatility and is low in cost. Since the working unit **15** can easily be separated from the operating unit **16**, the working unit **15** (the distal end working unit **14**) is easily maintained, enabling replacement, cleaning, and/or high-temperature sterilization thereof.

With the medical manipulator **10** thus constructed, as the gripper **22** is operated (opened and closed or angularly rotated), and the distal end working unit **14** is rotated by the single transmitting member **18**, the installation space of the transmitting member **18** within the coupling **12** may be small. Accordingly, the coupling **12** may be thinner, while the distal end working unit **14** and the operating unit **16** may both be simpler in structure. The medical manipulator **10** according to the present embodiment can thus appropriately be used for performing laparoscopic surgery, brain surgery, thoracoscopic surgery, urologic surgery, or the like.

Operations of the medical manipulator **10** shall be described below.

In an initial state (non-operated state), the gripper **22** is open under the bias of the coil spring **46**, and the movable handle **68** is open (see FIGS. **1**, **3**, and **5**). When the operator grips the handle unit **62** by the hand, and turns the movable handle **68** in the direction indicated by the arrow in FIG. **1**, the projecting member **124** is turned clockwise about the shaft member **82**, thus causing the pin **126** to be pressed against the inner peripheral surface of the proximal end of the oblong hole **114** in order to move the tongue **116** and the support member **102** along the guide members **118**, **120** (the state shown in FIG. **4**). Since the flange **110** engages with the proximal end of the support member **102**, the first coupling member **34** moves in the same direction as the support member **102**, thereby pulling the transmitting member **18** toward the proximal end. Since the support member **102** moves toward the proximal end, the distal end of the prismatic portion **98b** is inserted relatively deeply into the passage **108**.

When the transmitting member **18** is pulled toward the proximal end, the slider **44** moves within the recess **56** toward the proximal end thereof, against the bias of the coil spring **46**. Therefore, the pin **58** presses the inner peripheral surface of the proximal end of the oblong hole **60**, thereby

turning the movable pinching member 50 counterclockwise in FIG. 2 about the pin 52, and hence closing the movable pinching member 50 (the state shown in FIG. 2).

When the operator releases the hand from the handle unit 62, or reduces the gripping force on the handle unit 62, the slider 44 moves within the recess 56 toward the distal end thereof under the bias of the coil spring 46. Therefore, the pin 58 presses the inner peripheral surface of the distal end of the oblong hole 60, turning the movable pinching member 50 clockwise in FIG. 3 about the pin 52, and hence opening the movable pinching member 50 (the state shown in FIG. 3).

As the slider 44 moves toward the distal end, the transmitting member 18 also moves in the same direction. At the proximal end of the transmitting member 18, the flange 110 presses the support member 102, thereby moving the support member 102 and the tongue 116 toward the distal end along the guide members 118, 120. The inner peripheral surface of the proximal end of the oblong hole 114 presses the pin 126, turning the projecting member 124 and the movable handle 68 clockwise in FIG. 5 about the shaft member 82. The movable handle 68 now returns to its original open state (the state shown in FIG. 5). As the support member 102 moves toward the direction of the distal end, the distal end of the prismatic portion 98b moves nearly to the center of the passage 108 along the longitudinal direction thereof.

The movable pinching member 50 is opened and closed in mechanically (directly) ganged relation to the movable handle 68 when it is opened and closed. Therefore, if the gripper 22 grips an object (a surgical instrument or living tissue) when the movable handle 68 is manually pulled to a certain extent, then the gripper 22 and the slider 44 are unable to move further, so that the operator can feel through the fingertips that the object has been gripped.

If the object is a hard object, such as a surgical instrument, then the movable handle 68 is no longer movable at all in the closing direction. The operator can feel that the hard object has been gripped, and can reliably grip the object with strong forces, because the operator can transmit manual forces mechanically and directly to the gripper 22, rather than via an electromagnetic means. If gripping forces equivalent to manual forces were to be generated by a motor, then the motor would need to be considerably large in size and heavy, such a motor could not be housed readily in the main operating unit body 28, and would make the medical manipulator 10 heavier.

If the object is a soft object, such as a living tissue or the like, then the movable handle 68 can be displaced slightly in the closing direction, depending on the elasticity of the object. Therefore, the operator can feel that the soft object has been gripped, while recognizing how soft the object is, and can adjust the forces at which the object is gripped.

When the transmitting member 18 or the like is worn or degraded, friction increases and is transmitted to the movable handle 68, allowing the operator to sense a change in state, or an abnormal state, of the drive system, and hence, the operator can judge the timing of maintenance more appropriately.

As described above, since the movable pinching member 50 is opened and closed in a mechanically (directly) ganged relation to the movable handle 68 when it is opened and closed, the opening (gripping) forces of the fixed pinching member 48 and the movable pinching member 50 correspond to the opening (gripping) forces of the fixed handle 80

and the movable handle 68. Therefore, the operator can easily operate the gripper 22 with any desired opening (gripping) forces.

Specifically, the manual operation of the movable handle 68 is mechanically transmitted so as to open and close the gripper 22. The transmitting member 18, the slider 44, etc., provide an operation transmitting unit, which serves as a means for mechanically transmitting manual operations between the movable handle 68 and the gripper 22.

The term "mechanically" as used herein refers to a system for transmitting manual operations via a wire, a chain, a timing belt, a link, a rod, a gear, or the like, which is actuated primarily by a mechanical component in the form of a nonelastic solid body in the power transmitting direction, as described above. Although a wire, a chain, or the like is slightly elongatable inevitably under tension, it is still regarded as a mechanical component in the form of a nonelastic solid body. For example, although the transmitting member 18 has a flexible portion corresponding to at least the curvable portion 30, the transmitting member 18 is placed under an appropriate tension by the coil spring 46. When the gripper 22 is closed, the transmitting member 18 is pulled toward the operating unit 16 by the movable handle 68, and the transmitting member 18 essentially is not elastically deformed, or is inevitably elastically deformed only to an extent that is trouble-free in operation, thereby providing a mechanical connecting means (mechanical transferring means).

When the rotating action input unit 86 is operated in order to energize the rotational drive source 90 to rotate the driven gear 94, regardless of whether the movable pinching member 50 is opened or closed (regardless of the degree of opening thereof), rotating forces are transmitted successively to the prismatic portion 98b of the rotational shaft 98, the passage 108, the first coupling member 34, the linear body 32, the second coupling member 36, the passage 40, the protrusion 38, and the main distal end body 54, thereby rotating the distal end working unit 14. Thus, the rotating action mechanism 88 and the joint 26 function as a rotating mechanism, for rotating the distal end working unit 14 about its own axis. The direction that the driven gear 94 is driven is the same as the direction in which the distal end working unit 14 rotates.

The gripper 22 can be opened and closed, and the distal end working unit 14 can be rotated, when the coupling 12 is straight, bent, or curved. With the medical manipulator 10 according to the present embodiment, since the curvable portion 30 is not rotated, but rather only the distal end working unit 14 is rotated, even when the coupling 12 is bent or curved (i.e., the state indicated by the two-dot-and-dash lines in FIG. 1), as it rotates, the distal end working unit 14 is not swung about an axis that extends from the curvable portion 30 toward the proximal end. Therefore, the attitude of the gripper 22 (the direction in which the living tissue is gripped) can be changed, while the gripper 22 remains proximate to the region that is to be surgically treated.

With respect to the bending action mechanism 130, by simply operating the bending action input unit 128 to energize the bending drive sources 140, 142, regardless of whether the movable pinching member 50 is opened or closed (regardless of the degree of opening thereof), it is possible to tilt the tilt plate 138 to any desired angle, thereby easily bending the coupling 12 to a desired angle at the curvable portion 30. Specifically, the curvable portion 30 and the bending action mechanism 130 function as a bending mechanism for bending the gripper 22 in a direction

15

crossing the axial direction of the coupling 12, so as to change the attitude of the gripper 22 easily and quickly.

With the medical manipulator 10 according to the present embodiment, as described above, the coupling 12 can be bent by the bending action mechanism 130, and the curvable portion 30 and the distal end working unit 14 can be rotated by the rotating action mechanism 88 easily and quickly through the bending drive sources 140, 142 and the rotational drive source 90, which serve as actuators, under the control of the controller 20, simply when the operator uses his fingertips to operate the bending action input unit 128 and the rotating action input unit 86 on the operating unit 16. Accordingly, the medical manipulator 10 has high operability. Specifically, in the medical manipulator 10, the bending mechanism for bending a portion (the curvable portion 30) of the coupling 12, and the rotating mechanism for rotating the distal end working unit 14 function cooperatively as an attitude changing mechanism, for changing the attitude of the distal end working unit 14, and such mechanisms operate through the actuators. The gripper 22 of the distal end working unit 14 is opened and closed (angularly moved) by the operator, who manually operates the fixed handle 80 and the movable handle 68 mechanically (directly) independently of the operation of the bending action mechanism 130, etc. Since the gripper 22 can be operated for acquiring desired gripping forces, the operator can treat the affected part more appropriately, while feeling the hardness of the gripped object. Specifically, it is ideal to operate the end effector (the gripper 22) by transmitting a manual action mechanically and directly thereto. Further, the best approach is to simplify operations of the bending action mechanism 130, the curvable portion 30, and the rotating action mechanism 88, which provide other attitude axes, i.e., the operation of the attitude changing mechanism, using the actuators (the bending drive sources 140, 142 and the rotational drive source 90). In other words, according to the present invention, since the distal end working unit 14 can easily be changed in attitude simply by pressing buttons with a single fingertip, for example, the attitude changing actions do not interfere with other actions of the operator to open and close the gripper 22 and to move the medical manipulator 10 in its entirety using the arm, thereby allowing the operator to perform a more intuitive surgical treatment.

FIG. 14 is an enlarged side elevational view, partly in cross section, showing another structural example of the distal end portion of the medical manipulator 10 shown in FIG. 1.

A distal end working unit 180, as shown in FIG. 14, is arranged to have a biasing means, for biasing the movable pinching member 50 in the opening direction, disposed in the vicinity of the distal end working unit 14. The coil spring 46 is housed in a large-diameter portion 182, which is greater in diameter than the space 24, formed at a position adjacent to the proximal end of the joint 26 of the coupling 12. Within the large-diameter portion 182, the second coupling member 36 extends through the coil spring 46, and a disk-shaped flange 184 is fixed to or integrally combined with a portion of the second coupling member 36, which extends from the coil spring 46 toward the distal end. The coil spring 46 in the compressed state has a proximal end thereof held against the proximal end face of the large-diameter portion 182, and a distal end held against the flange 184, and biases the second coupling member 36 toward the distal end.

The biasing means is not limited to the coil spring 46, but may comprise another spring, such as a torsion spring, a leaf spring, or the like, or an elastic material such as rubber, or

16

a permanent magnet or an electromagnet. The biasing means may be disposed within the operating unit 16.

During surgical operations, a large peeling force may be required in the direction (peeling direction) in order to open the gripper 22 for peeling off tissue. If the coil spring 46 is replaced with a tension spring, and the pushing action of the movable handle 68 is transmitted directly to the gripper 22 via the slider 44, then a large peeling force can be produced. On the medical manipulator 10, the force applied in the opening direction of the gripper 22 is transmitted to the movable handle 68. Specifically, when the gripper 22 abuts against a living tissue or a surgical instrument in the opening direction thereof at the time the gripper 22 is opened, the movable handle 68 stops moving in the opening direction. Thus, the operator can feel that the gripper 22 has come into abutment against something.

The rotating action mechanism 88, the bending action mechanism 130, the joint 26, the converting means 100, the operating unit 16, the detachable joint 35, the connector 37, etc., are not limited to the aforementioned illustrated structural details. In the present embodiment, the surgical operation means may comprise a pair of opening and closing members, which are angularly movable, or which may be openable and closable by being translated. Further, the surgical operation means may comprise a single member, which is angularly movable, such as a bendable forceps, an electrosurgical knife, an ultrasonic knife, or the like.

The rotational drive source 90 and the bending drive sources 140, 142, which are actuators for actuating the rotating action mechanism 88 and the bending action mechanism 130, may comprise fluid-pressure actuators, using a fluid such as a gas, a liquid, or the like, for example, rather than electric motors.

The rotating action input unit 86 and the bending action input unit 128 may also be constructed as foot switches, rather than being provided on the operating unit 16. In this case, foot switches may be placed at the operator's feet for allowing the operator to perform manual techniques more smoothly.

The movable handle 68, the rotating action input unit 86, and the bending action input unit 128 on the operating unit 16 are not limited to the positions, forms, and operating methods that have been illustrated above. The rotating action input unit 86 may be replaced with operating rollers, buttons, or a joystick. Further, various positions and methods that allow the manipulator to be easily operated may be selected and designed.

A medical manipulator 1010 according to another embodiment will be described below with reference to FIGS. 15 to 57.

As shown in FIG. 15, the medical manipulator 1010 according to the present embodiment makes up part of a medical manipulator system, and is connected to a controller 1045.

The controller 1045, which serves to control the medical manipulator 1010 electrically, is connected via a connector to a cable 1062 extending from a lower end of a grip handle 1026. The controller 1045 can control a plurality of medical manipulators 1010 independently of each other. Of course, a controller for controlling a single medical manipulator 1010 may also be used.

The medical manipulator 1010 includes a distal end working unit 1012 for gripping a portion of a living tissue, and a curved needle, or the like for performing a given surgical treatment. The medical manipulator 1010 usually is referred to as a gripping forceps or a needle driver (needle holder).

As shown in FIGS. 15 and 16, the medical manipulator 1010 comprises an operating unit 1014, which is held and operated by the hand, and a working unit 1016 fixed to the operating unit 1014. The operating unit 1014 and the working unit 1016 are integrally combined with each other. However, depending on conditions, the operating unit 1014 and the working unit 1016 may be separable from each other.

In the following description, it shall be assumed that transverse directions in FIGS. 15 and 16 are referred to as X directions, vertical directions as Y directions, and longitudinal directions of a connector shaft 1048 as Z directions. Among the X directions, the rightward direction as viewed from the distal end is referred to as an X1 direction, and the leftward direction as an X2 direction. Among the Y directions, the upward direction is referred to as a Y1 direction, and the downward direction as a Y2 direction. Among the Z directions, the forward direction is referred to as a Z1 direction, and the rearward direction as a Z2 direction. Unless otherwise noted, these directions represent directions of the medical manipulator 1010 when it is in a neutral posture. The above definitions of directions are for illustrative purposes only. The medical manipulator 1010 can be used in any of various orientations, e.g., it may be used upside down.

The working unit 1016 comprises a distal end working unit 1012 for performing working operations, and an elongate hollow connector shaft (coupling) 1048 coupling the distal end working unit 1012 and the operating unit 1014 to each other. The distal end working unit 1012 and the connector shaft 1048 have a small diameter, and can be inserted into a body cavity 1022 through a trocar 1020 in the form of a hollow cylinder mounted inside an abdominal region or the like of the patient. The working unit 1012 is actuated by a composite input unit 1034 in order to perform various techniques to grip, remove, suture, or tie-knot an affected part of the patient's body within the body cavity 1022.

The operating unit 1014 includes a grip handle 1026, which is gripped by the hand, a bridge 1028 extending from an upper portion of the grip handle 1026, and an actuator block 1030 and a trigger lever (input unit) 1032, which are connected to a distal end of the bridge 1028.

As shown in FIG. 15, the grip handle 1026 of the operating unit 1014 extends in the Y2 direction from the end of the bridge 1028, and has a length suitable for being gripped by the hand. The composite input unit 1034 is disposed on the grip handle 1026.

The cable 1062 connected to the controller 1045 is disposed on a lower end of the grip handle 1026 while being integrally connected to the grip handle 1026. The grip handle 1026 and the cable 1062 may be connected to each other by a connector.

The composite input unit 1034 makes up a composite input means for imparting rotational commands in rolling (shaft rotating) and yawing (left and right) directions to the distal end working unit 1012. For example, commands in the yawing direction are given by a first input means 1034a, which operate in the lateral direction, whereas commands in the rolling direction are given by a second input means 1034b, which operate in the shaft rotating direction. The trigger lever 1032 comprises an input means for imparting opening and closing commands for an end effector 1104 (see FIG. 15) of the distal end working unit 1012. Although the end effector 1104 is available in various forms, the medical manipulator 1010 employs an openable and closable gripper.

The composite input unit 1034 includes an input sensor for detecting a control variable, and supplies a detection operation signal (e.g., an analog signal) to the controller 1045.

The trigger lever 1032 comprises a lever disposed below the bridge 1028 and is disposed at a position where it can easily be operated by the index finger. The trigger lever 1032 is connected to the actuator block 1030 by a first link 1064 and a second link 1066, and is movable toward and away from the grip handle 1026. The first link 1064 pivots swingably about a portion of the bridge 1028, and the trigger lever 1032 is mounted on the end of the first link 1064 in the Y2 direction. The second link 1066 projects in the Z2 direction from the actuator block 1030 and engages in an oblong hole 1064a formed in the first link 1064. The second link 1066 is movable back and forth in the longitudinal direction in the oblong hole 1064a when the trigger lever 1032 is moved.

The second link 1066 is connected to an end of a wire (drive member) 1056. When the trigger lever 1032 is pulled, the wire 1056 also is pulled in unison therewith. Since the wire 1056 is used as a drive member (transmitting member) connected to the second link 1066, the number of parts used can be reduced, and the medical manipulator 1010 is reduced in weight.

The drive member connected to the second link 1066 may comprise a rigid linearly movable rod (or link), for example, rather than the wire 1056. Since a rod is generally more rigid than the wire, the rod may be used as a linearly movable member for producing large gripping forces. The rod and the second link 1066 may be combined integrally with each other.

Links, gears, etc., may be operatively disposed between the second link 1066 and the wire 1056, for adjusting the operating forces and strokes of the operator.

The actuator block 1030 houses motors (attitude axis actuators) 1040, 1041 therein corresponding to the respective mechanisms of two out of three degrees of freedom, which are incorporated in the distal end working unit 1012. The motors 1040, 1041 are arrayed in parallel with each other in the longitudinal direction of the connector shaft 1048. The motors 1040, 1041 correspond to movements in both rolling and yawing directions of the distal end working unit 1012, i.e., movements of the attitude changing mechanism, for changing the attitude of the distal end working unit 1012. The motors 1040, 1041 are small in size and diameter, thus enabling the actuator block 1030 to be compact and flat in shape. The motors 1040, 1041 can be energized to rotate the drive shafts under the control of the controller 1045, based on operation of the operating unit 1014. The motors 1040, 1041 are combined with angle sensors, for detecting rotational angles and supplying the detected angle signals to the controller 1045. The angle sensors may comprise rotary encoders, for example. Rather than electric motors, the actuators may comprise fluid-pressure actuators, using a fluid such as a gas, liquid, or the like, for example.

The actuator block 1030 houses pulleys 1050a, 1050b therein, which are connected, respectively, to the drive shafts of the motors 1040, 1041.

Wires 1052, 1054 are wound respectively around the pulleys 1050a, 1050b, and extend through a hollow region 1048a (see FIG. 20) in the connector shaft 1048 toward the distal end working unit 1012. The wires 1052, 1054 may both be of the same type and have the same diameter.

The composite input unit 1034 and the trigger lever 1032 of the operating unit 1014 are not limited to the above-described and illustrated positions, forms, and operating

methods. For example, the composite input unit **1034** may be replaced with operating rollers, buttons, or a joystick. Further, other positions and methods, which allow the manipulator to be easily operated, may be selected and designed.

A manual operation applied to the trigger lever **1032** is mechanically transmitted to open and close the end effector **1104**. The first link **1064**, the second link **1066**, the wire **1056**, and an end effector driving mechanism **1260**, to be described later, serve as a means (transmitting members) for mechanically transmitting a manual action between the trigger lever **1032** and the end effector **1104**, and make up an operation transmitting unit.

The term "mechanically" refers to a system for transmitting manual operations via a wire, a chain, a timing belt, a link, a rod, a gear, or the like, which is mainly actuated in the power transmitting direction by a mechanical component in the form of a nonelastic solid body. Although a wire, a chain, or the like, is slightly elongatable inevitably under tension, it is still regarded as a mechanical component in the form of a nonelastic solid body.

First through fifth structural examples **1012a** through **1012e**, and a modification **1012f** of the distal end working unit **1012**, shall be described below.

As shown in FIGS. **17**, **18**, **19**, **20**, and **21**, the distal end working unit **1012a** according to the first structural example comprises a wire-driven mechanism **1100**, a composite mechanism **1102**, and an end effector **1104**. The distal end working unit **1012** incorporates therein mechanisms providing three degrees of freedom. These mechanisms include a mechanism having a first degree of freedom for angularly moving a portion of the distal end working unit **1012** that is positioned ahead of a first rotational axis Oy extending along the Y direction, in a yawing direction about the first rotational axis Oy, a mechanism having a second degree of freedom for angularly moving the portion of the distal end working unit **1012** in a rolling direction about a second rotational axis Or, and a mechanism having a third degree of freedom for opening and closing the end effector **1104** on the distal end of the distal end working unit **1012** about a third rotational axis Og.

The first rotational axis Oy of the mechanism having the first degree of freedom may be angularly movable out of parallelism with an axis C, which extends from the proximal end to the distal end of the connector shaft **1048**. The second rotational axis Or of the mechanism having the second degree of freedom may be angularly movable, about an axis along the direction in which the distal end (the end effector **1104**) of the distal end working unit **1012** extends, with the distal end portion thereof being rotatable in the rolling direction.

The mechanism having the first degree of freedom (i.e., which is movable in the yawing direction) comprises a bending mechanism having an operable range of $\pm 90^\circ$ or greater, for example. The mechanism having the second degree of freedom (i.e., which is movable in the rolling direction) comprises a rotating mechanism having an operable range of $\pm 180^\circ$ or greater, for example. The mechanism having the third degree of freedom (i.e., the end effector **1104**) may be opened through **400** or greater, for example.

The end effector **1104** comprises a member for performing actual work during an operation. The first rotational axis Oy and the second rotational axis Or are attitude axes of the attitude changing mechanism, for changing the attitude of the end effector **1104** for facilitating the work. Generally, the mechanism having the third degree of freedom for opening and closing the end effector **1104** is referred to as a gripper

(or a gripper axis). The mechanism having the first degree of freedom for turning in a yawing direction is referred to as a yaw axis, and the mechanism having the second degree of freedom for turning in a rolling direction is referred to as a roll axis.

The wire-driven mechanism **1100** is disposed between a pair of tongue pieces **1058** and serves to convert reciprocating movement of the respective wires **1052**, **1054** into rotational movement, and to transmit such rotational movement to a composite mechanism **1102**. The wire-driven mechanism **1100** includes a shaft **1110**, which is inserted into shaft holes **1060a**, **1060a**, and a shaft **1112**, which is inserted into shaft holes **1060b**, **1060b**. The shafts **1110**, **1112** are press-fitted or welded securely to the shaft holes **1060a**, **1060b**. The shaft **1112** is aligned axially with the first rotational axis Oy.

Gear bodies **1126**, **1130**, which are symmetrically shaped in the Y direction, are mounted respectively on both ends of the shaft **1112**, respectively, in the Y direction. The gear body **1126** comprises a tubular member **1132** and a first gear **1134** disposed concentrically on an upper portion of the tubular member **1132**. The gear body **1130** is essentially identical in shape to the gear body **1126**, and is aligned with the gear body **1126** in the Y direction. The gear body **1130** comprises a tubular member **1136** and a second gear **1138** disposed concentrically on a lower portion of the tubular member **1136**. The gears **1134**, **1138** are held in mesh with upper and lower ends of the face gear **1165** of a gear body **1146**, to be described later.

The tubular member **1136** is substantially identical in diameter and shape to the tubular member **1132**. Wires **1052**, **1054** are wound around the tubular members **1132**, **1136** and have portions fastened thereto by a securing means. The wires **1052**, **1054** are wound 1.5 turns (540°) around the tubular members **1132**, **1136**.

When the wires **1052**, **1054** are rotated, the gear bodies **1126**, **1130** are rotated about the shaft **1112**. When the gear bodies **1126**, **1130** are rotated at the same speed and in the same direction, the gear body **1146** swings with respect to the shaft **1112** and moves in a yawing direction. When the gear bodies **1126**, **1130** are rotated at the same speed and in the opposite direction, the gear body **1146** is rotated about the second rotational axis Or and moves in a rolling direction. When the gear bodies **1126**, **1130** are rotated at different speeds, the gear body **1146** undergoes a composite motion in both yawing and rolling directions. The gear body **1126**, the gear body **1130**, and the gear body **1146** collectively make up a differential mechanism.

An idle pulley (a cylindrical member, a transmitting member) **1140** is rotatably supported substantially centrally on the shaft **1110**. A guide pulley (a cylindrical member, a transmitting member) **1142** is rotatably supported substantially centrally on the shaft **1112**. The idle pulley **1140** serves to keep a driven wire (a flexible member, a transmitting member) **1252** wound around the guide pulley **1142** through a constant angle (about 180° on both sides) at all times. Instead of using the idle pulley **1140**, the driven wire **1252** may also be wound one or more turns around the guide pulley **1142**. The idle pulley **1140** and the guide pulley **1142** may have a smooth surface, and may be made of a material having a small coefficient of friction, in order to reduce slippage and frictional wear on the driven wire **1252** (see FIG. **22**). The guide pulley **1142** is disposed around the yaw axis Oy of the attitude changing mechanism.

A main shaft **1144** is rotatably supported on the shaft **1112** between the gear body **1126** and the guide pulley **1142**, as well as between the guide pulley **1142** and the gear body

1130. The main shaft **1144** has a sleeve projecting toward the composite mechanism **1102**. The main shaft **1144** has a square hole **1144a** formed axially therein. The main shaft **1144** includes two auxiliary plates **1144b** disposed on one end in the **Z2** direction for holding both surfaces of the guide pulley **1142** in the **Y** direction. The auxiliary plates **1144b** have respective holes through which the shaft **1112** extends. The auxiliary plates **1144b** have chevron shapes, which become progressively wider in the **Z1** direction, for preventing foreign matter such as threads from entering therein.

The composite mechanism **1102** includes an opening/closing mechanism for opening and closing the end effector **1104**, and an attitude changing mechanism for changing the attitude of the end effector **1104**.

The composite mechanism **1102** comprises a gear body **1146** rotatably fitted over the circumferential surface of the sleeve of the main shaft **1144**, a nut **1148** mounted on the distal end of the main shaft **1144**, a spring **1150**, a rod (a transmitting member) **1152** with a square cross-sectional shape and having an end in the **Z2** direction, which is inserted into the hole **1144a**, a driven pulley (a cylindrical member, a transmitting member) **1156** rotatably supported on the end in the **Z2** direction of the rod **1152** by a pin **1154**, a driven plate (a transmitting member) **1158**, and a hollow cylindrical cover **1160**. The spring **1150** comprises a compression spring. The end in the **Z2** direction of the rod **1152** is channel-shaped for improving slidability thereof with respect to the driven pulley **1156**, and the end of the rod **1152** projects largely in the **Z2** direction.

A thrust bearing **1144c** made of resin is disposed on the portion of the main shaft **1144** that abuts against the gear body **1146**. A further thrust bearing **1148a** made of resin is disposed on the portion of the nut **1148** that abuts against the gear body **1146**. The thrust bearings **1144c** and **1148a** have a low coefficient of friction, for reducing wear and torque on the abutting portions, and for preventing loads from being applied directly to the face gear **1165**. The thrust bearings **1144c**, **1148a** comprise slide bearings, for example, but may comprise rolling bearings, thereby allowing the medical manipulator to operate smoothly about the roll axis even when the end effector **1104** is strongly closed or opened, i.e., even when the gear body **1146** abuts firmly against the main shaft **1144**.

The gear body **1146** is of a stepped shape, comprising a large-diameter portion **1162** in the **Z2** direction, a small-diameter portion **1164** in the **Z1** direction, and a face gear **1165** on the end of the large-diameter portion **1162** in the **Z2** direction. The face gear **1165** is held in mesh with the gears **1134**, **1138**. The gear body **1146** prevents the nut **1148** from becoming dislodged from the main shaft **1144**. The large-diameter portion **1162** has an externally threaded outer circumferential surface.

The driven plate **1158** has a recess **1166** in the **Z2** direction, an engaging cavity **1168** formed in the bottom of the recess **1166**, axial ribs **1170** disposed respectively on both surfaces in the **Y** direction, and a link hole **1172**. The engaging cavity **1168** has a shape that is engageable with a mushroom-shaped knob **1174** on the distal end of the rod **1152**. When the mushroom-shaped knob **1174** engages in the engaging cavity **1168**, the driven plate **1158** and the rod **1152** are capable of rotating relatively with respect to each other about the roll axis. The driven plate **1158** has a width that is substantially equal to the inside diameter of the cover **1160**.

The cover **1160** has a size that is large enough to cover the composite mechanism **1102** substantially in its entirety, and serves to prevent foreign matter (living tissue, medications, threads, etc.) from entering into the composite mechanism

1102 and the end effector **1104**. The cover **1160** has two axial grooves **1175** formed in an inner circumferential surface thereof in diametrically confronting relation to each other. The ribs **1170** of the driven plate **1158** are fitted respectively in the grooves **1175** for axially guiding the driven plate **1158**. Since the knob **1174** engages in the engaging cavity **1168** of the driven plate **1158**, the driven pulley **1156** is axially movable back and forth within the hole **1144a**, in unison with the driven plate **1158** and the rod **1152**, and can roll about the rod **1152**. The cover **1160** is fixed to the large-diameter portion **1162** of the gear body **1146** by threaded engagement therewith, or by a press-fitted engagement, or the like.

The spring **1150** is fitted between the step of the gear body **1146** and the recess **1166** of the driven plate **1158**, for normally biasing the driven plate **1158** to move forward into abutment against a stopper.

The end effector **1104** comprises a first end effector member **1190**, a second end effector member **1192**, and a pin **1196**. The pin **1196** is disposed on the third rotational axis **Og**.

The first end effector member **1190** has a pair of side walls **1200** facing each other laterally, holes **1200a** formed respectively in the distal ends of the side walls **1200**, and a first gripper **1202** projecting in the **Z1** direction from lower portions of the distal ends of the side walls **1200**. The hole **1200a** has a diameter such that the pin **1196** can be press-fitted into the hole **1200a**. The first gripper **1202** becomes progressively narrower in the **Z1** direction and includes an arcuate distal end portion. The first gripper **1202** has a number of conical teeth disposed closely together over the entire surface thereof, which faces in the **Y1** direction. The first end effector member **1190** is coupled to the cover **1160** by a given coupling means. For example, the first end effector member **1190** and the cover **1160** may be of an integral structure, providing a composite tubular body **1230**.

The cover **1160** is coupled at a proximal portion to the gear body **1146** (by threaded engagement, press-fitted engagement, welding, or the like). When the gear body **1146** is rotated, the cover **1160** and the first end effector member **1190** operate about the roll axis.

The second end effector member **1192** is L-shaped, comprising a second gripper **1212** extending in the **Z** direction, and a lever **1214** bent about 60° with respect to the second gripper **1212**. The second end effector member **1192** has a hole **1216** formed in the L-shaped bent corner, and the lever **1214** has a hole **1218** formed therein near to the end portion thereof. When the pin **1196** is inserted into the hole **1216**, the second end effector member **1192** is swingable about the third rotational axis **Og**. The second gripper **1212** has a shape that is identical to the first gripper **1202**, yet is disposed in an inverted fashion. When the second end effector member **1192** is angularly moved about the third rotational axis **Og**, the second end effector member **1192** abuts against the first gripper **1202** for gripping a curved needle or the like.

The lever **1214** and the driven plate **1158** are joined to each other by two parallel gripper links **1220**. Specifically, a pin **1222** is inserted into holes **1220a** formed in respective ends of the gripper links **1220** and the hole **1218**, whereas a pin **1124** is inserted into holes **1220b** formed respectively in other ends of the gripper links **1220** and the hole **1172**.

The position of the pin **1124**, by which the gripper links **1220** are pivotally supported, is slightly offset from the central axis in FIG. 19 (as viewed in side elevation). However, the pin **1124** may be positioned on the central axis as viewed in side elevation. The position of the pin **1124** may

be determined in view of the balance of acting forces, the space, and the ease with which to assemble the parts. The pins may be integrally combined with the gripper links 1220.

Two gripper links 1220 are disposed in parallel to each other, for adequately balancing the forces, and for preventing the application of inadvertent moment loads. Depending on design conditions, only one gripper link may be employed.

When the driven pulley 1156, the rod 1152, and the driven plate 1158 are moved in the Z2 direction, the lever 1214 also is pulled in the Z2 direction, causing the second gripper 1212 to move toward the first gripper 1202 so as to grip an object therebetween. Conversely, when the driven pulley 1156, the rod 1152, and the driven plate 1158 are moved in the Z1 direction by action of the spring 1150, the lever 1214 also is pushed in the Z1 direction, causing the second gripper 1212 to move away from the first gripper 1202 and open the end effector 1104. Since the driven plate 1158 is normally biased by the spring 1150 to move in the Z1 direction, when the medical manipulator is not manually operated, the second gripper 1212 is spaced from the first gripper 1202 thereby opening the end effector 1104. The spring 1150 is effective to keep the wire 1056 and the driven wire 1252 under a suitable tension and prevent them from sagging. Therefore, play between the various parts is prevented and the medical manipulator is capable of gripping objects with high responsiveness.

For the sake of brevity, the term "end effector 1104" will hereinafter be used to refer to the first gripper 1202 and the second gripper 1212.

As shown in FIG. 21, the idle pulley 1140 comprises two parallel pulleys, i.e., a first layer idle pulley (first layer idle cylindrical body) 1232 and a second layer idle pulley (second layer idle cylindrical body) 1234, which are aligned coaxially with each other. The guide pulley 1142 comprises two parallel pulleys, i.e., a first layer guide pulley (first layer guide cylindrical body) 1236 and a second layer guide pulley (second layer guide cylindrical body) 1238, which are aligned coaxially with each other.

At the end in the Z2 direction in FIG. 21, one of the stretches of the driven wire 1252 is held against surfaces of the first layer idle pulley 1232 in the X1 and Z1 directions, and also is held against surfaces of the first layer guide pulley 1236 in the Z2 and X2 directions, while extending to the driven pulley 1156.

At the end in the Z2 direction in FIG. 21, the other stretch of the driven wire 1252 is held against surfaces of the second layer idle pulley 1234 in the X2 and Z1 directions, and also is held against surfaces of the second layer guide pulley 1238 in the Z2 and X1 directions, while extending to the driven pulley 1156.

When the wire 1056 (see FIG. 22) is pulled in the Z2 direction, for example, the first layer idle pulley 1232 and the second layer guide pulley 1238 are rotated counterclockwise as viewed in plan, whereas the second layer idle pulley 1234 and the first layer guide pulley 1236 are rotated clockwise as viewed in plan. Since each of the idle pulley 1140 and the guide pulley 1142 comprises two parallel coaxial pulleys, the pulleys are rotatable in opposite directions when the driven wire 1252 held thereagainst is moved, and hence the pulleys operate smoothly.

As shown in FIG. 22, the end of the wire 1056 in the Z1 direction is connected to both ends of the driven wire (a flexible member) 1252 by a terminal 1250 (or welding, through hole, etc.). The driven wire 1252 is in the form of a ring-like flexible member, having a portion thereof connected to the wire 1056, and may alternatively comprise a

rope, a resin wire, a piano wire, a chain, or the like. The term "ring-shaped" should be interpreted in a broad sense. The flexible member does not necessarily need to be applied to the entire length. That is, at least the portion of the driven wire 1252, which is wound around each of the pulleys, may be a flexible member with the linear portion thereof being connected by a rigid member. The driven wire 1252 may make up part of the wire 1056.

The driven wire 1252 passes from the wire 1056, serving as a drive member, along the idle pulley 1140 in the X1 direction (first side) and extends to the X2 direction (second side), and then passes along the guide pulley 1142 in the X2 direction and extends to the surface of the driven pulley 1156 in the X2 direction. The driven wire 1252 is then wound in a half turn around the surface of the driven pulley 1156 in the Z1 direction and extends to the surface thereof in the X1 direction, and while oriented in the X2 direction, the driven wire 1252 passes along the idle pulley 1140 in the X2 direction and extends to the terminal 1250.

The driven wire 1252 thus passes through a circulatory path, having its starting and ending points at the terminal 1250. The driven wire 1252 passes along both sides of the idle pulley 1140 and is wound around the driven pulley 1156, while crossing over itself between the idle pulley 1140 and the guide pulley 1142, thereby making up a substantially 8-shaped configuration. The terminal 1250 and the driven wire 1252 are mechanically connected to the trigger lever 1032 by the wire 1056.

The term "mechanically" refers to a system for actuating members via a mechanical component, in the form of a solid body that is nonelastic in the power transmitting direction. Although the wire 1056 is a flexible member, it is appropriately tensioned by the spring 1150. For closing the end effector 1104, the wire 1056 is pulled in the Z2 direction by the trigger lever 1032 and essentially is not elastically deformed, or inevitably is elastically deformed only to an extent that is trouble-free in operation, thereby providing a mechanical connecting means. The driven wire 1252 crosses over itself as viewed in plan.

The idle pulley 1140, the guide pulley 1142, and the driven pulley 1156 have substantially the same diameter, which is a sufficiently large diameter, to the extent possible by the layout, such that the driven wire 1252 will not become bent. The terminal 1250 is disposed in a position appropriately spaced from the idle pulley 1140, so that the driven wire 1252 will not be bent excessively. Both ends of the driven wire 1252 form an acute angle at the terminal 1250. Since the spring 1150 (see FIG. 18) biases the driven plate 1158 to move in the Z1 direction, the driven pulley 1156 and the driven plate 1158 undergo forces in the Z1 direction. The driven wire 1252 and the wire 1056 are thus placed appropriately in a state of tension, and are not slackened. The gap between the idle pulley 1140 and the guide pulley 1142 is small, e.g., substantially the same as the width of the driven wire 1252.

The idle pulley 1140, the guide pulley 1142, and the driven pulley 1156 may have flanges on upper and lower surfaces thereof, or may have concave side surfaces for preventing the driven wire 1252 from dropping off.

For illustrative purposes, the wire 1056, the driven wire 1252, the idle pulley 1140, the guide pulley 1142, the driven pulley 1156, and the end effector 1104, shall be referred to collectively as an end effector driving mechanism 1260. In the end effector driving mechanism 1260, as shown in FIG. 22, the driven wire 1252, the idle pulley 1140, the guide pulley 1142, and the driven pulley 1156 are arranged along

the central line from a proximal end to a distal end. The end effector **1104** is coupled to the driven pulley **1156** by the rod **1152**.

Operation of the medical manipulator **1010** thus constructed shall be described below.

As shown in FIG. **22**, when the trigger lever **1032** is not touched, the end effector **1104** is opened under the resiliency of the spring **1150**. The X direction in FIGS. **22**, **23**, **24**, **25**, **36**, **37**, **52**, **53**, and **55** is indicated with respect to the distal end working unit **1012a**, and the vertical direction of the trigger lever **1032** corresponds to the Y directions.

As shown in FIG. **23**, when the trigger lever **1032** is fully pulled by hand, the wire **1056** pulls the driven wire **1252**, moving the driven pulley **1156** and the rod **1152** in the Z2 direction while compressing the spring **1150**, thereby closing the end effector **1104**. In other words, the end effector **1104** is closed when the transmitting members, including the wire **1056**, the driven wire **1252**, and the driven pulley **1156**, are pulled. At this time, the trigger lever **1032** requires forces for compressing the spring **1150**. For opening the end effector **1104**, the force applied to the trigger lever **1032** is released, thereby allowing the rod **1152** to be pushed toward the distal end under the restorative force of the spring **1150**, and returning the end effector **1104** to the open state.

Since the driven wire **1252** is ring-shaped, it provides two left and right stretches. Therefore, the forces applied to close the end effector **1104** are divided into substantially equal forces, which act as tensile forces on respective stretches of the driven wire **1252**. Therefore, the driven wire **1252** may have a diameter that is smaller than the wire **1056**, and may be sufficiently flexible.

As shown in FIG. **24**, when the end effector **1104** grips an object (a surgical instrument, a living tissue, or the like) W at the time the trigger lever **1032** is pulled to a certain extent by the hand, the end effector **1104**, the driven plate **1158**, the rod **1152**, and the driven pulley **1156** are essentially no longer moved further, or are moved only a distance corresponding to the elastic deformation of the driven wire **1252** and other components and the elastic deformation of the object W. The driven wire **1252**, the wire **1056**, and the trigger lever **1032** are not moved further in the Z2 direction, thereby allowing the operator to feel, with the fingertip, that the end effector **1104** has gripped the object W.

If the object W is a hard object such as a surgical instrument or the like, then the trigger lever **1032** is essentially unable to move in the Z2 direction. The operator can thus feel that the end effector **1104** has gripped something hard, and the end effector **1104** can reliably grip the object W with strong forces, because the operator can transmit manual forces mechanically and directly to the end effector **1104**, rather than via electromagnetic means. If gripping forces equivalent to such manual forces were to be generated by a motor, then the motor would need to be considerably large and heavy, and could not be housed readily inside the actuator block **1030**, and further, would make the medical manipulator **1010** heavier.

If the object W is a soft object such as a living tissue or the like, then the trigger lever **1032** is slightly displaceable in the Z2 direction depending on the resiliency of the object W. The operator can thus feel that the end effector **1104** has gripped something soft, and can recognize how soft the object W is as well as adjust the forces with which the object W is gripped.

When the wires, etc., are worn or become degraded, friction increases and is transmitted to the trigger lever **1032**, allowing the operator to sense a change in state, or an

abnormal state, of the drive system. Hence, the operator can judge the timing of maintenance more appropriately.

As shown in FIG. **25**, when the end effector **1104** is operated about the yaw axis, the driven pulley **1156** rotates about itself, while revolving around the guide pulley **1142**. Since the distance between the driven pulley **1156** and the guide pulley **1142** remains unchanged, the rod **1152** is not relatively actuated and there is no mechanical interference. When the end effector **1104** is operated about the roll axis, since the rod **1152** is disposed so as to pass through the center of the roll axis, the rod **1152** is not actuated and there is no mechanical interference. In other words, the effector driving mechanism **1260** provides a non-interfering construction.

Since the idle pulley **1140** and the guide pulley **1142** are sufficiently close to each other, even when the end effector **1104** is actuated 90° about the yaw axis, the angle through which the driven wire **1252** is wound around the driven pulley **1156** remains essentially unchanged, and substantially no torque that interferes with the yaw and roll axes is generated in response to the gripping action.

If the idle pulley **1140** and the guide pulley **1142** are spaced from each other by a certain distance, then when the end effector **1104** is operated significantly about the roll axis, the driven wire **1252** is spaced from one of the surfaces of the guide pulley **1142**. The driven wire **1252** is thus brought out of balance in the X direction (reference state) about the yaw axis, producing an interference torque about the yaw axis. For maximizing the operating range about the yaw axis, it is desirable to position the idle pulley **1140** and the guide pulley **1142** sufficiently close to each other. Actually, inasmuch as the driven wire **1252** passes between the idle pulley **1140** and the guide pulley **1142**, a certain gap is needed therebetween. Also, the gap between portions of those pulleys (except for the flanges on the upper and lower surfaces) around which the driven wire **1252** is wound may be of a size that is 1 to 2 times the thickness of the driven wire **1252**.

If the operating range about the yaw axis does not need to be increased, then the idle pulley **1140** and the guide pulley **1142** may be appropriately spaced from each other. Even if the yaw axis is bent, the end effector **1104** can be opened and closed by operating the trigger lever **1032**, so as to cause the driven wire **1252** to actuate the driven pulley **1156**.

As the yaw-axis operation and the roll-axis operation do not cause mechanical interference with opening and closing operations of the end effector **1104**, the drive mechanism of the distal end working unit **1012a** for actuating the end effector **1104** does not require any correcting means for compensating for interference, or any other type of correcting means (e.g., corrective actuators and assisting mechanisms) including mechanisms and actuators. Therefore, the medical manipulator **1010** is simple and lightweight in structure. Operating forces applied to the trigger lever **1032** can efficiently be transmitted to the end effector **1104** without affecting other drive systems. Consequently, the end effector **1104** can exert strong gripping (or peeling) forces. Inasmuch as the medical manipulator **1010** is lightweight, the operator can reduce the forces needed to support the medical manipulator **1010**. As a result, the medical manipulator **1010** enables the operator to perform techniques suitably over a long period of time, and also to better feel the forces at which tissue is pierced with a suture needle, along with reactive forces from the tissue.

The medical manipulator **1010** is an energy saver because the end effector **1104** can be opened and closed manually by the trigger lever **1032**.

A link mechanism, which is a reversal of the above link mechanism, may be used, such that the end effector **1104** is closed when it is not operated on by the hand. In this case, the end effector **1104** can be opened when the trigger lever **1032** is pulled. The reversal link mechanism may be such that the closed state of the end effector **1104**, i.e., the state in which the second gripper **1212** is superposed on the first gripper **1202**, as shown in FIG. 22 for example, is an initial state. When the trigger lever **1032** is pulled in the initial state, the second gripper **1212** is turned counterclockwise and spaced from the first gripper **1202**, thereby opening the end effector **1104**.

During surgical operations, a large peeling force may be required in a direction (peeling direction) to open the end effector **1104**, for the purpose of peeling off tissue. If the pulling action of the trigger lever **1032** is directly transmitted to the end effector **1104** through the reversal link structure, then a large peeling force can be produced.

In this case, with the medical manipulator **1010**, the forces in the opening direction of the end effector **1104** are transmitted to the trigger lever **1032**. In other words, when the end effector **1104** is opened and abuts against living tissue, a surgical instrument, or the like, in the opening direction, the trigger lever **1032** is unable to move in the Z1 direction. The operator thus can sense that the end effector **1104** abuts against something.

Since the difference between the yaw axis and the pitch axis of the distal end working unit **1012** represents an initial attitude or a relative attitude with respect to the operating unit, the yaw axis may be replaced with the pitch axis. Therefore, the distal end working unit **1012** may have the yaw axis and the pitch axis. The attitude axes (corresponding to the yaw axis and the roll axis on the distal end working unit **1012**) may be actuated by rods, links, torque tubes, or the like, for example, or any combination thereof, rather than by means of wires (flexible members) and gears.

The idle pulley **1140**, the guide pulley **1142**, and the driven pulley **1156** may not necessarily be pulleys, but may comprise cylindrical bodies (cylindrical members) around which wires can be wound, if they allow the flexible member to slip thereon. The cylindrical bodies are to be interpreted in a broad sense, and include hollow cylindrical bodies and arcuate columnar bodies. If the angle of the operational range of a pulley is small according to design conditions, then the wire may be wound in less than one turn around the pulley. In this case, the pulley may be an arcuate columnar body.

If the driven pulley **1156** is nonrotatable with respect to the pin **1154** (the driven pulley **1156** is fixed to the rod **1152**), then since the driven wire **1252** is not held in abutment against a semiarculate portion of the driven pulley **1156** that is closer to the guide pulley (in the Z2 direction), the semiarculate portion of the driven pulley **1156** is not required, and hence the driven pulley **1156** may be in the form of a cylindrical body, having only a semiarculate portion closer to the distal end thereof. If a return pulley **1350**, similarly, has a portion held out of abutment against the driven wire **1252**, then the return pulley **1350** may be a partly arcuate cylindrical body, thereby enabling the composite mechanism **1102** to be reduced in length.

Modifications of the junction at the end of the driven wire **1252**, which correspond to the terminal **1250**, shall be described below with reference to FIGS. 26 to 31.

According to a first modification of the function at the end of the driven wire **1252**, as shown in FIG. 26, both ends of the driven wire **1252** are inserted into the opening at the distal end of a pipe (driving member) **1400**, and a portion

1402 proximate the opening at the distal end is pressed so as to compress the inserted ends. The driven wire **1252** can thus be secured in place easily.

According to a second modification of the function at the end of the driven wire **1252**, as shown in FIG. 27, a pipe **1406** is threaded into the distal end of a rod (driving member) **1404**. Similar to the pipe **1400** shown in FIG. 26, the pipe **1406** compresses both ends of the driven wire **1252**. Thus, with this arrangement, the rod **1404** and the pipe **1406** are detachably connected to each other, for facilitating assembly and maintenance. Such threaded engagement allows the pipe **1406** to project adjustably from the rod **1404**, for adjusting the length and tension of the driven wire **1252**. The pipe **1406** may further be secured by a double-nut structure.

According to a third modification of the function at the end of the driven wire **1252**, as shown in FIGS. 28 and 29, the driven wire **1252** is inserted through a hole **1410** formed in the distal end of a rod (driving member) **1408**. The hole **1410** has an arcuate wall **1410a** facing in the Z2 direction, which is engaged by the driven wire **1252**. The driven wire **1252** slides against the arcuate wall **1410a**. When the rod **1408** is pulled in the Z2 direction, the driven wire **1252** can be pulled in the X direction with good balance.

The driven wire **1252**, which comprises a single wire, has both ends thereof fixed to a securing member **1412**, and hence is of a ring shape. The securing member **1412** is disposed in a location other than the junction to the rod **1408** as a driving member, and allows the length and tension of the driven wire **1252** to be adjusted. Hence, the third modification is simple in structure.

According to a fourth modification of the function at the end of the driven wire **1252**, as shown in FIGS. 30 and 31, a roller **1416** is mounted at a distal end portion **1414a** of a rod (driving member) **1414**, and the driven wire **1252** is wound around the roller **1416**. The roller **1416** is rotatably supported on a pin **1418**. The driven wire **1252**, as it is wound around the roller **1416**, is movable back and forth. When the rod **1414** is pulled in the Z2 direction, the driven wire **1252** can be pulled in the X direction with good balance, even if the yaw axis is not bent. The distal end portion **1414a** is threaded into the rod **1414**. According to the fourth modification, the paired stretches of the driven wire **1252**, which are spaced in the Y direction, are tensioned uniformly so as to lengthen the service life of the driven wire **1252** and to make the paired upper and lower stretches of the driven wire **1252** parallel to each other.

Since the paired stretches of the driven wire **1252**, which are spaced in the Y direction, are parallel to each other, the rod **1414** may be disposed in a position close to the distal end working unit **1012a**, thereby shortening the driven wire **1252** and reducing elongation of the driven wire **1252**, so as to increase the responsiveness thereof.

A distal end working unit **1012b** according to a second structural example will be described below. Those parts of the distal end working unit **1012b** (as well as the distal end working units **1012c** through **1012f**) that are identical to those of the distal end working unit **1012a** shall be denoted by identical reference characters, and these features will not be described in detail below.

As shown in FIG. 32, the distal end working unit **1012b** is of a structure that is similar to the distal end working unit **1012a**, except that the idle pulley **1140** (see FIG. 21) is dispensed with. In the distal end working unit **1012b**, the driven wire **1252** is wound in one turn or more around the guide pulley **1142** from two directions. Specifically, the driven wire **1252** is wound around the first layer guide pulley

1236 from the X2 direction, and is wound around the second layer guide pulley 1238 from the X1 direction. The distal end working unit 1012b operates in the same manner as the distal end working unit 1012a. When the driven wire 1252 is pulled in the Z2 direction, the guide pulley 1142 and the driven pulley 1156 are pulled to operate the end effector 1104, and also to operate the end effector 1104 in the yawing directions, about the shaft 1112 (see the imaginary lines in FIG. 32). If the operation range about the yaw axis is one-sided (0° to 90°), then only one stretch of the driven wire 1252 may be wound in one turn or more around the guide pulley 1142. For example, in FIG. 32, in order to operate the end effector 1104 only in one direction, as indicated by the arrow A, about the yaw axis, the turn 1253 of the driven wire 1252, which is wound around the first layer guide pulley 1236 in the X1 direction, is not required. The driven wire 1252 may be held only against the surface of the first layer guide pulley 1236, which faces in the X2 direction.

The distal end working unit 1012b is simpler in structure than the distal end working unit 1012a, because it does not require the idle pulley 1140. On the other hand, with the distal end working unit 1012a, the length of the driven wire 1252, which is wound around the guide pulley 1142, is shorter for providing less friction, and the overall length of the driven wire 1252 is shorter than in the case of the distal end working unit 1012b. Since the number of turns around the guide pulley 1142 is smaller, the guide pulley 1142 may be thinner. Whether the distal end working unit 1012a or the distal end working unit 1012b is to be employed may be determined depending on design conditions.

The structures shown in FIGS. 26 to 32 are also applicable to the distal end working units 1012c through 1012f, to be described below.

The distal end working unit 1012c according to a third structural example will be described below.

As shown in FIG. 33, the distal end working unit 1012c is different from the distal end working unit 1012a in terms of the structure of the end effector 1104.

The distal end working unit 1012c includes an end effector 1300 having a double-sided-open type structure, with a pair of grippers 1302 being movable thereon. The end effector 1300 comprises a gripper base 1304 integrally combined with the cover 1160, a pair of end effector members 1308 movable about a pin 1196 mounted on the gripper base 1304, and a pair of gripper links 1220.

Each of the end effector members 1308 has an L shape, similar to the second end effector member 1192, and comprises a gripper 1302 extending in the Z1 direction and a lever 1310 bent about 35° and extending from the gripper 1302. The L-shaped bent corner includes a hole 1216 formed therein, and the pin 1196 is inserted into the hole 1216, so that the end effector members 1308 are swingable about the third rotational axis Og.

Each of the end effector members 1308 is coupled to a pin 1224 on the driven plate 1158 by a single side gripper link 1220. The driven plate 1158 has two link holes 1172 disposed in symmetrical positions with respect to the Y direction in FIG. 33. The gripper links 1220 cross each other, as viewed in side elevation.

The wire-driven mechanism 1100 and the composite mechanism 1102, other than the end effector 1300 of the distal end working unit 1012c, are identical in structure to those of the distal end working unit 1012a described above.

Since the grippers 1302 are disposed in confronting positions, the distal end working unit 1012c is capable of exerting well-balanced forces, without imposing inadvertent moment loads.

As shown in FIGS. 33 and 34, the end effector members 1308 are basically actuated in synchronism in response to operation of the rod 1152. Therefore, the end effector members 1308 are openable and closable symmetrically with respect to the central axis.

As shown in FIG. 35, when the end effector 1300 moves about the yaw axis, since the yaw-axis mechanism and the mechanism for actuating the end effector 1300 are held out of interference with each other, the degree of opening of the end effector 1300 does not change. Conversely, when the end effector 1300 is opened and closed, the end effector 1300 does not move about the yaw axis or the roll axis.

Since the end effector 1300 is mechanically connected directly to the trigger lever 1032, the end effector 1300 produces strong gripping forces, wherein the forces applied to the end effector 1300 are transmitted to the trigger lever 1032.

The distal end working unit 1012d according to a fourth structural example will be described below. With the distal end working units 1012a through 1012c described above, the trigger lever 1032 is pulled actively (i.e., the grippers are closed/opened) by a manual force, and the trigger lever 1032 is passively returned by the force of the spring 1150, so that the force is applied in one direction only for opening/closing the grippers. With the distal end working unit 1012d according to the fourth structural example (as well as with the distal end working unit 1012e), a manual force is applied actively to pull and return the trigger lever 1032, whereby a force is applied in both directions. The spring 1150 for generating forces is dispensed with. The distal end working unit 1012d may be used as a gripping forceps as well as a peeling forceps.

As shown in FIG. 36, the distal end working unit 1012d includes two mechanisms, i.e., a first end effector driving mechanism 1320a and a second end effector driving mechanism 1320b, corresponding to the end effector driving mechanism 1260 (see FIG. 22). Components of the first end effector driving mechanism 1320a are denoted by reference characters with an "a" appended thereto, and components of the second end effector driving mechanism 1320b are denoted by reference characters with a "b" appended thereto, so that they can be distinguished from each other. In FIGS. 36 and 37 (as well as FIGS. 52 and 53), the first end effector driving mechanism 1320a and the second end effector driving mechanism 1320b are shown in parallel with each other on the sheets, for facilitating understanding. If the distal end working unit 1012d is incorporated in an actual medical manipulator 1010, then, as shown in FIG. 38 (and FIG. 51), the pulleys are juxtaposed axially (i.e., in the Y direction) such that the rotational shafts of the idle pulleys (cylindrical members, transmitting members) 1140a, 1140b are disposed coaxially with each other, and the rotational shafts of the guide pulleys (cylindrical members, transmitting members) 1142a, 1142b also are disposed coaxially with each other. In other words, the idle pulleys 1140a, 1140b are supported commonly on the shaft 1110 (see FIG. 38), whereas the guide pulleys 1142a, 1142b are supported commonly on the shaft 1112. The guide pulleys 1142a, 1142b, which are coaxial with each other, simplify the yaw axis operating mechanism.

The distal end working unit 1012d comprises a first end effector driving mechanism 1320a, a second end effector driving mechanism 1320b, a drive coupling wire (a drive

coupling flexible member, a transmitting member) **1322**, and a drive coupling pulley (a cylindrical member, a transmitting member) **1324**, around which the drive coupling wire **1322** is wound. With this arrangement, the first end effector driving mechanism **1320a** and the second end effector driving mechanism **1320b** can be operated in opposite phase, so as to move a drive link (a transmitting member) **1326a** and a drive link (a transmitting member) **1326b** easily in opposite directions.

Although not illustrated, the distal end working unit **1012d** includes a wire-driven mechanism **1100**, a composite mechanism **1102**, and an end effector **1104**, which are identical to those of the distal end working unit **1012a**.

The drive coupling wire **1322** has one end thereof connected to the proximal end of the drive link **1326a** of the first end effector driving mechanism **1320a**, and the other end thereof connected to the proximal end of the drive link **1326b** of the second end effector driving mechanism **1320b**. The drive links **1326a**, **1326b** correspond to the wire **1056**, and are connected to terminals **1250a**, **1250b** at respective ends of driven wires **1252a**, **1252b**. In the distal end working unit **1012d**, the drive links **1326a**, **1326b** may be replaced with wires. In such a case, the drive coupling wire **1322** may have both ends thereof directly connected to the terminals **1250a**, **1250b**.

The second link **1066** (see FIG. 22) has one end connected to the drive link **1326a**, which can be moved back and forth by the trigger lever **1032**. Since the drive coupling wire **1322** and the drive link **1326b** are connected to the drive link **1326a** around the drive coupling pulley **1324**, the drive link **1326a** and the drive link **1326b** are moved back and forth in opposite directions when the second link **1066** is moved back and forth.

The trigger lever **1032** can actuate the drive link **1326a** and the drive link **1326b** through a rack and pinion mechanism, which includes a rack mounted on the second link **1066**, and a pinion mounted on the drive coupling pulley **1324**. The drive coupling pulley **1324** may be disposed in the distal end working unit **1012d** (i.e., on a distal end of the connector shaft **1048**), or may be disposed in the operating unit **1014**.

The distal end working unit **1012d** also includes a driven coupling wire (a driven coupling flexible member, a transmitting member) **1328**, having one end connected to a driven pulley (a flexible member, a transmitting member) **1156a** of the first end effector driving mechanism **1320a** and another end connected to a driven pulley (a flexible member, a transmitting member) **1156b** of the second end effector driving mechanism **1320b**, and a driven coupling pulley (a cylindrical member, a transmitting member) **1330** around which the driven coupling wire **1328** is wound. In this arrangement, the first end effector driving mechanism **1320a** and the second end effector driving mechanism **1320b** can be operated in opposite phase so as to move the rod **1152** back and forth.

Either one of the driven pulley **1156a** and the driven pulley **1156b** is rotatably held by the rod **1152**. The rod **1152** may be fixed to a linear portion of the driven coupling wire **1328**. The rod **1152** may also be connected to the driven coupling pulley **1330** by a rack and pinion mechanism. In other words, the rod **1152** may bring about back-and-forth movement of the driven pulleys **1156a**, **1156b** or the driven coupling wire **1328**.

If the drive coupling wire **1322** and the driven coupling wire **1328** are placed under an initial tension of ON or higher, and are made free from sagging, various parts of the

distal end working unit are prevented from having play, and the distal end working unit can grip the object with high responsiveness.

As shown in FIG. 36, when the trigger lever **1032** is fully pulled by the hand, the drive link **1326a** pulls the driven wire **1252a** in order to move the driven pulley **1156a** and the rod **1152** in the Z2 direction, thereby closing the end effector **1104**. In other words, the end effector **1104** is closed by pulling the transmitting members, including the drive link **1326a**, the driven wire **1252a**, and the driven pulley **1156a**.

In the second end effective driving mechanism **1320b**, since the drive link **1326b** is disposed such that it is pushed outward, the drive link **1326b** does not obstruct the operation of the rod **1152**. Since the driven wire **1252b** produces only tensile forces (i.e., the driven wire **1252b** does not transmit compressive forces), the driven wire **1252b** basically does not contribute to the transmission of power.

At this time, when the end effector **1104** grips the object W, the driven wire **1252**, the drive link **1326**, and the trigger lever **1032** are unable to move further in the Z2 direction, thereby allowing the operator to feel, with the fingertip, that the end effector **1104** has gripped the object W. The operator also can sense the hardness of the object W. These actions can easily be understood by referring to FIGS. 36 and 24, because the distal end working unit **1012a**, as shown in FIG. 24, is essentially equivalent to the distal end working unit **1012d** shown in FIG. 36, although the second end effector driving mechanism **1320b** is dispensed with.

As shown in FIG. 37, when the trigger lever **1032** is fully pushed out by the hand, the drive coupling wire **1322** is moved counterclockwise in FIG. 37, and the drive link **1326b** pulls the driven wire **1252b** in order to move the driven pulley **1156b** in the Z2 direction. The driven coupling wire **1328** moves in a counterclockwise direction, and the rod **1152** and the driven pulley **1156a** move in the Z1 direction toward the distal end, thereby opening the end effector **1104**.

Since the forces for pushing out the trigger lever **1032** by hand are mechanically and directly transmitted to the end effector **1104** by the second end effector driving mechanism **1320b**, the end effector **1104** can be opened with a desired strong force, rather than given forces such as from an elastic body. Therefore, using an outer side surface of the end effector **1104**, the distal end working unit can appropriately be used to perform techniques for peeling off living tissue or for opening a hole.

When the object W is brought into contact with the outer side surface of the end effector **1104**, the driven wire **1252b**, the drive link **1326b**, and the trigger lever **1032** are no longer moved further in the Z1 direction, thereby allowing the operator to feel, with the fingertip, that the outer side surface of the end effector **1104** has contacted the object W. The operator also can sense the hardness of the object W.

The distal end working unit **1012d** can operate about the yaw axis and the roll axis, in the same manner as the distal end working unit **1012a**. Although not shown, when the distal end working unit **1012d** operates about the yaw axis, the composite mechanism **1102** and the end effector **1104**, which are closer to the distal end than the shafts (see FIG. 38) of the guide pulleys **1142a** and **1042b**, swing in yawing directions about the shafts of the guide pulleys **1142a** and **1042b**. Since the distal end working unit **1012d** makes up a non-interference mechanism, similar to the distal end working unit **1012a**, when the distal end working unit **1012d** operates about the yaw axis, the degree at which the end effector **1104** is opened remains unchanged. Conversely, when the degree of opening of the end effector **1104** is

changed, the yaw axis is not operated. The end effector **1104** and the roll axis are related to each other in the same manner.

The distal end working unit **1012d** (as well as the distal end working unit **1012e**) does not require the spring **1150**. Depending on design conditions, the spring **1150** may be provided to bias the rod **1152** to move toward either the distal end or the proximal end. This arrangement makes it possible to hold the end effector open or closed when the trigger lever **1032** is not operated. If sufficient space is not available in the distal end working unit **1012d**, then the spring **1150** may also be disposed in the trigger lever **1032**.

As shown in FIG. **38**, in the distal end working unit **1012d**, the idle pulleys **1140a**, **1140b** have respective outer first layer idle pulleys **1232a**, **1232b**, which are coaxial with each other, and respective inner second layer idle pulleys **1234a**, **1234b**, which also are coaxial with each other. The guide pulleys **1142a**, **1142b** have respective outer first layer guide pulleys **1236a**, **1236b**, which are coaxial with each other, and respective inner second layer guide pulleys **1238a**, **1238b**, which also are coaxial with each other. This structure is similar to the structure shown in FIG. **21**, allowing the paired pulleys to rotate in opposite directions for enabling smooth operation.

As shown in FIG. **39**, the inner two second layer idle pulleys **1234a**, **1234b** may be formed integrally with each other, jointly making up a central common idle pulley **1430**. The inner two second layer guide pulleys **1238a**, **1238b** may be formed integrally with each other, jointly making up a central common guide pulley **1432**.

Specifically, since the drive links **1326a** and **1326b** move the same distance in opposite directions, the wires move as indicated by the arrows in FIG. **39**, thereby rotating the second layer idle pulley **1234a** and the second layer idle pulley **1234b** through the same angle and in the same direction (clockwise in FIG. **39**), while also rotating the second layer guide pulley **1238a** and the second layer guide pulley **1238b** through the same angle and in the same direction (counterclockwise in FIG. **39**). Therefore, such members do not need to be disposed separately, but may make up an integral central common idle pulley **1430** and an integral central common guide pulley **1432**, which are of a simple structure. In FIG. **39**, the second layer guide pulley **1238a** and the second layer guide pulley **1238b** are shown as being slightly spaced from each other, whereas the second layer idle pulley **1234a** and the second layer idle pulley **1234b** also are shown as being slightly spaced from each other, for facilitating understanding. However, the distance between them may essentially be nil.

Drive member advancing and retracting mechanisms **1440a** through **1440d**, according to first through fourth examples, for moving the first end effector driving mechanism **1320a** and the second end effector driving mechanism **1320b** over substantially the same distance and in opposite directions, shall be described below with reference to FIGS. **40** to **43**.

As shown in FIG. **40**, the drive member advancing and retracting mechanism **1440a** according to the first example comprises an arm **1444** rotatably about a pivot **1442**, a rotational engaging member **1446a**, which is slightly spaced from the pivot **1442** in the Y1 direction, and a rotational engaging member **1446b**, which is slightly spaced from the pivot **1442** in the Y2 direction. The distances from the pivot **1442** to the two rotational engaging members **1446a**, **1446b** are substantially equal to each other. The drive link **1326a** has a proximal end thereof that rotatably engages with the rotational engaging member **1446a**. The drive link **1326b**

has a proximal end thereof that rotatably engages with the rotational engaging member **1446b**.

The arm **1444** corresponds to the first link **1064** described above. The trigger lever **1032** is mounted on the lower end of the arm **1444**.

As shown in FIG. **41**, as with the drive member advancing and retracting mechanism **1440a**, the drive member advancing and retracting mechanism **1440b** according to the second example comprises the arm **1444**, the pivot **1442**, and the rotational engaging members **1446a**, **1446b**. A wire **1448a** is connected to the rotational engaging member **1446a**, and a wire **1448b** is connected to the rotational engaging member **1446b**. The other end of the wire **1448a** is connected to the driven wire **1252a** (see FIG. **36**) by the terminal **1250a**, whereas the other end of the wire **1448b** is connected to the driven wire **1252b** (see FIG. **36**) by the terminal **1250b**.

As shown in FIG. **42**, the drive member advancing and retracting mechanism **1440c** according to the third example comprises the arm **1444**, a rotary operating member **1450** fixed to the arm **1444**, a wire **1452** wound around the rotary operating member **1450**, a securing member **1454** securing a portion of the wire **1452** to the rotary operating member **1450**, and an idler **1456** that is held against a portion of the wire **1452** near to the rotary operating member **1450**. The rotary operating member **1450** is in the form of a thin cylindrical body and operates as a pulley. Specifically, the wire **1452** has a portion **1452a** thereof that is held in contact with an upper portion of the rotary operating member **1450**, and another portion **1452b** thereof held in contact with a portion of the rotary operating member **1450**, which faces in the Y2 direction.

The rotary operating member **1450** rotates in unison with the arm **1444** about the pivot **1442**. The portion **1452a** of the wire **1452** from the securing member **1454** is connected to the driven wire **1252a** (see FIG. **36**) by the terminal **1250a**. The other portion **1452b** of the wire **1452** is connected to the driven wire **1252b** (see FIG. **36**) by the terminal **1250b**.

The rotary operating member **1450** has an appropriate large diameter, so as to be capable of fully pulling the driven wire **1252a** and the driven wire **1252b**. The securing member **1454** is disposed in a position such that it does not prevent the wire **1452** from being drawn in and fed out.

The idler **1456** is held against the wire **1452**, thereby defining the layout and path of the wire **1452** through the hollow region **1048a** in the connector shaft **1048** to hold the portions **1452a**, **1452b** of the wire **1452** closely to each other. The idler **1456** may double as a tensioner for the wire **1452**.

As shown in FIG. **43**, the drive member advancing and retracting mechanism **1440d** according to the fourth example comprises the arm **1444**, the rotary operating member **1450**, a wire **1460**, the securing member **1454**, and the idler **1456**. The wire **1460** has a distal end thereof connected to the proximal end of the drive link **1326a**, and a proximal end portion wound around the upper portion of the rotary operating member **1450**. The proximal end is fixed to the rotary operating member **1450** by the securing member **1454**. The idler **1456** is disposed in engagement with the wire **1460**, for defining the layout and path of the wire **1460** and the drive link **1326a**.

The proximal end of the drive link **1326b** is rotatably supported on a lower engaging member **1464** of the rotary operating member **1450**. The arm **1444** has an oblong hole **1064a** formed therein for guiding the lower engaging member **1464**. The drive link **1326a** and the drive link **1326b** are supported for back and forth movement in the Z direction by means of guides **1462a**, **1462b**.

The drive member advancing and retracting mechanisms **1440a** through **1440d** make it possible to move the first end effector driving mechanism **1320a** and the second end effector driving mechanism **1320b** over substantially the same distance in opposite directions. The drive member advancing and retracting mechanisms **1440a** through **1440d** may also be applied to the distal end working unit **1012e**, as shall be described below.

The distal end working unit **1012e** according to the fifth structural example will be described below. The distal end working unit **1012e** includes a first end effector driving mechanism **1340a** and a second end effector driving mechanism **1340b**.

As shown in FIGS. **44**, **45**, **46** and **47**, the first end effector driving mechanism **1340a** is essentially the same as the above-described first end effector driving mechanism **1320a** (see FIG. **36**). The second end effector driving mechanism **1340b** differs from the second end effector driving mechanism **1320b** (see FIG. **36**) described above, in that a return pulley (a cylindrical member, a transmitting member) **1350** is added thereto, and the driven coupling wire **1328** and the driven coupling pulley **1330** are dispensed with. The driven pulley **1156a** and the driven pulley **1156b** are disposed coaxially.

The main shaft **1144** has a diametrical hole **1354** formed therein, with a pin **1352** inserted and fixed therein. The hole **1354** extends through the sleeve of the main shaft **1144** across the hole **1144a**.

The rod (transmitting member) **1152** has an oblong hole **1356** formed therein, which extends axially and has a width large enough to allow the pin **1352** to be inserted there-through. The rod **1152** is disposed at a position that is slightly offset from the axis of the working unit **1016** in the Y1 direction. The knob **1174** on the distal end is disposed on the axis (see FIG. **22**). However, the rod **1152** may also be positioned centrally.

As with the driven pulley **1156** (see FIG. **20**), the driven pulley **1156a** is rotatably supported by the pin **1154** on the end of the rod **1152**, in the Z2 direction. The pin **1154** extends through the rod **1152** and projects in the Y2 direction, with the driven pulley **1156b** being supported on the projecting end thereof. The driven pulley **1156b** has a width large enough to support two turns of the driven wire **1252b**. The hole **1144a** has a height large enough so that the driven pulleys **1156a**, **1156b** and the rod **1152** may be inserted therein. The driven pulleys **1156a**, **1156b** are coaxially supported by the pin **1154** in the hole **1144a** for independent rotation.

Within the hole **1144a**, the pin **1352** is inserted into the oblong hole **1356** and the central hole in the return pulley **1350** from the Y1 direction and toward the Y2 direction, thus allowing the rod **1152** and the driven pulleys **1156a**, **1156b** to move axially back and forth. The return pulley **1350** is supported rotatably by the pin **1352**, is fixed in position, and has a width large enough to support two turns of the driven wire **1252b**. If the return pulley **1350** is of a two-layer structure, then the return pulley **1350** can be rotated in opposite directions when the end effector is opened and closed, thereby reducing friction between the wire and the pulley.

As shown in FIGS. **48**, **49**, and **50**, in the second end effector driving mechanism **1340b**, the return pulley **1350** is disposed more closely to the distal end than the driven pulley **1156b**, and the driven wire **1252b** is wound around the driven pulley **1156b** and the return pulley **1350**. In other words, the driven wire **1252b** passes from the terminal **1250b** of the drive link **1326b** of the driving member,

through the side of the idle pulley **1140b** that faces in the X1 direction, and then extends in the X2 direction, passing through the side of the guide pulley **1142b** that faces in the X2 direction, and extends to the surface of the driven pulley **1156b**, which faces in the X2 direction. The driven wire **1252b** extends in the Z1 direction to the surface of the return pulley **1350** that faces the X2 direction, is wound in a half turn around the surface of the return pulley **1350** that faces the X1 direction, and then returns in the Z2 direction.

The driven wire **1252b** is wound in a half turn around the surface of the driven pulley **1156b**, which faces the Z2 direction. The driven wire **1252b** passes through the side thereof, which faces in the X2 direction, and extends again toward the return pulley **1350**. The driven wire **1252b** is wound in a half turn around the surface of the return pulley **1350**, which faces the Z1 direction, and returns toward the X2 direction. Thereafter, the driven wire **1252b** extends from the side of the guide pulley **1142b**, which faces in the X1 direction, to the side of the idle pulley **1140b**, which faces in the X2 direction, and is connected to the terminal **1250b** of the drive link **1326b**. The terminal **1250** and the driven wire **1252b** are mechanically connected to the trigger lever **1032** by the drive link **1326b**.

The idle pulley **1140b** is greater in diameter than the guide pulley **1142b** in FIGS. **48**, **49**, and **50**, for preventing the gears **1134**, **1138** (see FIG. **20**) disposed adjacent to the guide pulley **1142b** from interfering with the shaft **1110**, and for holding the idle pulley **1140b** and the guide pulley **1142b** close to each other.

FIG. **51** schematically shows the distal end working unit **1012e**, for facilitating understanding of the structure thereof.

As shown in FIG. **52**, when the trigger lever **1032** is fully pulled by the hand, the rod **1152** moves in the Z2 direction to close the end effector **1300**. At this time, the operations and advantages of the distal end working unit **1012e** are the same as those of the distal end working units shown in FIGS. **23** and **36**, and such features will not be described in detail below.

Since the driven pulley **1156b** is arranged coaxially with the driven pulley **1156a**, the driven pulley **1156b** is displaced in unison with the driven pulley **1156a** in the Z2 direction. Since the drive link **1326b** is displaced and pushed out, the driven wire **1252b** and the drive coupling wire **1322** do not sag. The distance between the driven pulley **1156b** and the return pulley **1350** is represented by L.

As shown in FIG. **53**, when the trigger lever **1032** is fully pushed out by hand, the drive coupling wire **1322** moves counterclockwise in FIG. **53**, and the drive link **1326b** acts to pull the driven wire **1252b**. Since the distal end portion of the driven wire **1252a** is wound around the return pulley **1350**, which is fixed in position, the driven wire **1252a** does not move in its entirety, and the driven pulley **1156b** moves in the Z1 direction depending on the distance that the drive link **1326b** moves, thereby reducing the distance L. Since the distance L is reduced, the driven wire **1252a** is fed out accordingly toward the drive link **1326b**, which is allowed to move. The driven pulley **1156b** thus acts as a movable pulley, whereas the return pulley **1350** acts as a fixed pulley.

Since the driven pulley **1156a** is coaxial with the driven pulley **1156b**, the driven pulley **1156a** is displaced in unison with the driven pulley **1156b** in the Z1 direction, thereby pushing the rod **1152** in the Z1 direction to open the end effector **1300**.

Since the forces for pushing out the trigger lever **1032** by hand are transmitted directly and mechanically to the end effector **1300** by the second end effector driving mechanism **1320b**, the end effector **1300** can be opened with a desired

strong force, rather than by given forces such as from an elastic body. Therefore, the distal end working unit can appropriately be used to perform techniques for peeling off living tissue or for opening a hole using an outer side surface of the end effector **1300**.

When the object **W** is brought into contact with the outer side surface of the end effector **1300**, the driven wire **1252b**, the drive link **1326b**, and the trigger lever **1032** are no longer moved further in the **Z1** direction, thus allowing the operator to feel, with the fingertip, that the outer side surface of the end effector **1300** has contacted the object **W**. The operator also can feel the hardness of the object **W**.

The distal end working units **1012d**, **1012e** can operate about the yaw axis and the roll axis in the same manner as the distal end working unit **1012a**. Although not shown, when the distal end working unit **1012e** operates about the yaw axis, the composite mechanism **1102** and the end effector **1300**, which are positioned more closely to the distal end than the shafts (see FIG. 51) of the guide pulley **1142a** and the guide pulley **1042b**, swing in the yawing direction about the shafts of the guide pulley **1142a** and the guide pulley **1042b**. Since the distal end working unit **1012e** is a non-interference mechanism, as with the distal end working unit **1012a**, when the distal end working unit **1012e** operates about the yaw axis, the degree at which the end effector **1300** is opened remains unchanged. Conversely, when the degree of opening of the end effector **1300** is changed, the yaw axis is not operated. The end effector **1300** and the roll axis are related to each other in the same manner.

Since the driven pulleys **1156a**, **1156b** slide over the same distance and in the same direction, they can be disposed coaxially with each other, such that the distal end working unit **1012e** enables increased housing and space efficiency. Further, the distal end working unit **1012e** is made up of a reduced number of parts, and can easily be assembled and serviced for maintenance. Since the driven pulleys **1156a**, **1156b** slide in unison with each other, only one sliding movement assembly is sufficient. With the distal end working unit **1012d**, however, since the driven pulleys **1156a**, **1156b** slide in opposite directions, two sliding movement assemblies are required.

All the pulleys of the distal end working unit **1012e**, i.e., the idle pulleys **1140a**, **1140b**, the guide pulleys **1142a**, **1142b**, the driven pulleys **1156a**, **1156b**, and the return pulley **1350**, have their rotational shafts positioned parallel to each other (in the **Y** directions), and the pulleys are laid out efficiently without dead spaces. The driven coupling pulley **1330** of the distal end working unit **1012d**, however, has an axis that extends perpendicularly to the other pulleys.

The distal end working unit **1012e** does not require the driven coupling wire **1328** or the wire fastening means thereof, which are provided in the distal end working unit **1012d**. The distal end working unit **1012e** is simpler in structure, since it does not require the driven coupling pulley **1330** in the distal end working unit **1012d**.

The wire drive ratio of the distal end working unit **1012e** at the time the end effector **1300** is operated to grip and open is 1:1, as with the distal end working unit **1012d**, and is well balanced.

In the distal end working unit **1012e**, the face gear **1165** together with the gears **1134**, **1138** make up a differential gear. According to a first modification, as shown in FIG. 54, the face gear **1165** is held in mesh with the gear **1134** only, and portions thereof corresponding to the main shaft **1144** and the gear body **1130** (see FIG. 20) may be of an integral structure. The distal end working unit thus operates about the roll axis based on the action of the wire **1052** via the gear

1134, and operates about the yaw axis by swinging the main shaft **1144**, based on a coordinated operation of the wires **1052**, **1054**.

As shown in FIG. 55, according to a second modification of the distal end working unit **1012e**, the second end effector driving mechanism **1340b** having the return pulley **1350** is employed, and the first end effector driving mechanism **1340a** is dispensed with. According to this modification, the spring **1150** may be provided to make up for the action of the first end effector driving mechanism **1340a**, which is dispensed with. While the spring **1150** is a compression spring in the distal end working unit **1012a** (see FIG. 22) according to the first structural example, according to the second modification, the spring **1150** comprises a tension spring for resiliently biasing the end effector to close itself. The trigger lever **1032** is connected to the drive link **1326a**. According to the modification shown in FIG. 55, the idle pulley **1140b** may be dispensed with. As with the distal end working unit **1012b** (see FIG. 32), according to the second structural example, the driven wire **1252** may be wound in one turn or more around the guide pulley **1142b** from at least one direction. If two distal end working units **1012e** according to the second embodiment shown in FIG. 55 are combined in parallel with each other, then manual forces work actively when the trigger lever **1032** is pulled and returned, and forces are produced in both directions. Hence, the spring **1150** for producing forces may be dispensed with. The distal end working unit may be used as a gripping forceps as well as a peeling forceps.

Although the distal end working unit **1012e** comprises a double-sided-open-type of end effector **1300**, the distal end working unit **1012e** may also incorporate a single-sided-open-type of end effector **1104** (see FIG. 19), or another type of end effector.

The distal end working units **1012a** through **1012e** are not limited to the above structures, but may consist of various other structures as well.

For example, as shown in FIG. 56A, a distal end working unit **1012f** according to a modification does not include the gripper links **1220** (see FIG. 19), but rather, the driven plate **1158** and the lever **1214** are connected to each other by the pin **1222** and an oblong hole **1360**. The pin **1222** is fixed to the lever **1214**. According to this modification, with the distal end working unit **1012f**, when the pin **1222** slides inside the oblong hole **1360**, the second gripper **1212** is turned so as to open and close the end effector (see FIG. 56B). The distal end working unit **1012f** can be made up of a reduced number of parts, since the gripper link **1220** and the pin **1224** (see FIG. 19) are dispensed with.

The distal end working unit **1012f** includes a wire-and-pulley non-interference mechanism (i.e., composite mechanism **1102**), which is basically of the same structure as the distal end working unit **1012f**, and has the same length **Ls**. The length **Lg** from the pin **1196** forming the gripper axis to the distal end can be of the same dimension as the distal end working unit **1012a** shown in FIG. 19. The connector length **Lx'** from the front surface of the driven plate **1158** to the pin **1196** can be considerably smaller than the connector length **Lx** (see FIG. 19) of the distal end working unit **1012a**, thus resulting in a reduction in the overall length **Lt** of the distal end working unit **1012f**.

Accordingly, the distal end working unit **1012f** can easily be operated by bending the yaw-axis joint in the body cavity **1022**, even if the body cavity **1022** is small, and makes it possible to perform operations in deeper and smaller spaces. The distal end working unit **1012f** may be applied to a structure in which two grippers, such as gripping forceps,

are opened and closed. Furthermore, linear motion of the rod **1152** may be converted into rotary motion by gears for gripping objects. The end effector is not limited to being a gripper type, but may comprise rotary electrodes or the like having scissors, or an opening and closing unit.

The wire-and-pulley non-interference mechanism according to the present embodiment has a wider operable range (e.g., of +90°) and a more compact structure than the conventional type (e.g., a soft mirror type) including a curved portion corresponding to the connector shaft **1048** and other non-interference mechanisms. Therefore, the distance from the curved or bent portion, corresponding to a joint, to the distal end may be reduced, thereby allowing the end effector to approach the living body freely and without limitations, and to operate in small spaces.

As described above, the end effector driving mechanisms **1260**, **1320a**, **1320b**, **1340a** and **1340b** of the medical manipulator **1010** according to the present embodiment have structures that are kept out of interference with the other operating axes, thereby making it possible to easily construct the distal end working unit with high degrees of freedom, and to realize strong gripping forces (or peeling forces). The transmitting members (drive members, the wire **1056**, etc.), which are mechanically connected to the manually operated input unit, allow the operator to feel the external forces that are applied to the distal end working unit **1012** reliably and easily. Moreover, the end effector driving mechanisms **1260**, **1320a**, **1320b**, **1340a**, **1340b** are made up of a simple structure that is free of gears.

Specifically, with the medical manipulator **1010** according to the present embodiment, the transmitting members involved in opening and closing the gripper include the driven wire **1252**, which comprises a flexible member, together with the guide pulley **1142** and the driven pulley **1156**, which form cylindrical members around which the driven wire **1252** is wound. The cylindrical members around which the flexible member is wound are made up of a simple and lightweight structure, and can change the attitude of the attitude changing mechanism so as not to interfere with the state of the end effector.

Stated otherwise, with the medical manipulator **1010** according to the present embodiment, the guide pulley **1142**, forming a cylindrical member, is provided as a rotational shaft in the attitude changing mechanism, and the transmitting members include the driven wire **1252**, making up a flexible member that is partially wound around the guide pulley **1142**, and the end effector that is operable through the driven wire **1252**. Since a flexible member is used, which is wound around the cylindrical member, the medical manipulator is simple and lightweight in structure, and the end effector can be actuated through the flexible member. The attitude of the attitude changing mechanism can be changed so as not to interfere with the state of the end effector, using the cylindrical member as a rotational shaft.

The above embodiment may be applied to the surgical robot system **1700** shown in FIG. **57**, for example.

The surgical robot system **1700** includes an articulated robot arm **1702**, and a console **1704** with the working unit **1016** connected to the distal end of the robot arm **1702**. The distal end of the robot arm **1702** incorporates therein a mechanism, which operates the same as the medical manipulator **1010**. The robot arm **1702** may be any means for moving the working unit **1016**, and is not limited to an installed type, but may also be of an autonomous movable type. The console **1704** may be of a table type, a control panel type, or the like.

The robot arm **1702** preferably has six or more independent joints (rotary shafts, slide shafts, etc.) for setting the position and orientation of the working unit **1016** as desired. The medical manipulator **1010** is integrally combined with the distal end **1708** of the robot arm **1702**. The medical manipulator **1010** includes a motor **1042** (an actuator ganged with the manually operable input unit) instead of the trigger lever **1032** (see FIG. **22**). The motor **1042** actuates the wire **1056** (see FIG. **22**) or the drive coupling pulley **1324** (see FIG. **36**).

The robot arm **1702** operates under control of the console **1704**, and may be automatically actuatable according to a program, or actuated by joysticks **1706** mounted on the console **1704**, or by a combination of the program and the joysticks **1706**. The console **1704** includes functions of the controller **1045**. The working unit **1016** includes the distal end working unit **1012** (**1012a** through **1012f**).

The console **1704** includes the two joysticks **1706** serving as an operation commander, and a monitor **1710**. Although not shown, the two joysticks **1706** are capable of individually operating two robot arms **1702**. The two joysticks **1706** are disposed in respective positions where they can easily be operated by both hands of the operator. The monitor **1710** displays information such as an image produced by a soft mirror.

The joysticks **1706** can be moved vertically and horizontally, twisted, and tilted. The robot arm **1702** can be moved depending on movements of the joysticks **1706**. The joysticks **1706** may be master arms. A communication means between the robot arm **1702** and the console includes a wired system, a wireless system, a network system, and a combination thereof.

The joysticks **1706** have respective trigger levers **1032**, which can be operated to energize the motor **1042**.

The type of medical manipulator is not limited to a forceps, but may be scissors, a tying-knot device, a needle holder, or a knife such as an electrosurgical knife, an ultrasonic knife, a laser knife, or the like. The medical manipulator is not limited to one that is used in performing laparoscopic surgery.

The medical manipulator according to the present invention is not limited to the above-described embodiments, but may include any of various additional and/or modified structures without departing from the gist of the present invention.

What is claimed is:

1. A medical manipulator comprising:

a distal end working unit that is disposed on a distal end of a shaft, the distal end working unit being openable and closable for a gripping operation and being movable in a rolling direction and in a yaw direction, the distal end working unit mechanically and manually openable and closable, without intervention of a motor, for a gripping operation through a transmitting member when an operating unit is operated by an operator, the operating unit having a trigger lever for mechanical and manual opening and closing of the distal end working unit for the gripping operation, the transmitting member including a flexible member and a cylindrical member around which said flexible member is wound, and the distal end working unit adapted to be operated in the rolling direction and in the yaw direction by a motor energized when said operating unit is operated by the operator.

2. The medical manipulator according to claim 1, wherein the distal end working unit comprises forceps.

41

3. The medical manipulator according to claim 1, wherein the medical manipulator is adapted to be used for performing laparoscopic surgery, brain surgery, thoracoscopic surgery, or urologic surgery.

4. The medical manipulator according to claim 1, wherein the medical manipulator is adapted to be used for performing brain surgery, thoracoscopic surgery, or urologic surgery.

5. The medical manipulator according to claim 1, wherein the operating unit is adapted to be detachably attached to a proximal end of the shaft for operating said distal end working unit.

* * * * *

42

专利名称(译)	医用机械手		
公开(公告)号	US9662131	公开(公告)日	2017-05-30
申请号	US11/939287	申请日	2007-11-13
[标]申请(专利权)人(译)	泰尔茂株式会社		
申请(专利权)人(译)	泰尔茂株式会社		
[标]发明人	OMORI SHIGERU UENOHARA SHUICHI JINNO MAKOTO		
发明人	OMORI, SHIGERU UENOHARA, SHUICHI JINNO, MAKOTO		
IPC分类号	A61B17/29 A61B17/00 A61B34/00		
CPC分类号	A61B17/29 A61B34/70 A61B34/71 A61B2017/0046 A61B2017/00398 A61B2017/2927 A61B2017/2929 A61B2017/2932 A61B2034/742		
代理机构(译)	WHITMYER IP集团有限责任公司		
优先权	2007283313 2007-10-31 JP		
其他公开文献	US20090112229A1		
外部链接	Espacenet USPTO		

摘要(译)

医疗操纵器包括远端工作单元，其包括作为末端执行器的夹具，用于操作远端工作单元的操作单元，将远端工作单元和操作单元互连的联接器，以及用于改变姿态的姿态改变机构远端工作单元。当操作者操作操作单元时，末端执行器由传动构件机械操作。姿态改变机构由弯曲驱动源和旋转驱动源操作，弯曲驱动源和旋转驱动源在操作者操作操作单元时操作。

