



US 20150080481A1

(19) **United States**
(12) **Patent Application Publication**
Zarins et al.

(10) **Pub. No.: US 2015/0080481 A1**
(43) **Pub. Date: Mar. 19, 2015**

(54) **METHODS FOR RENAL NEUROMODULATION**

(71) Applicants: **Denise Zarins**, Saratoga, CA (US); **Hanson Gifford, III**, Woodside, CA (US); **Mark Deem**, Mountain View, CA (US); **Douglas Sutton**, Pacifica, CA (US); **Howard R. Levin**, Teaneck, NJ (US); **Mark Gelfand**, New York, NY (US)

(72) Inventors: **Denise Zarins**, Saratoga, CA (US); **Hanson Gifford, III**, Woodside, CA (US); **Mark Deem**, Mountain View, CA (US); **Douglas Sutton**, Pacifica, CA (US); **Howard R. Levin**, Teaneck, NJ (US); **Mark Gelfand**, New York, NY (US)

(21) Appl. No.: **14/254,205**

(22) Filed: **Apr. 16, 2014**

Related U.S. Application Data

(63) Continuation of application No. 13/898,830, filed on May 21, 2013, now Pat. No. 8,774,922, which is a continuation of application No. 11/368,809, filed on Mar. 6, 2006, now Pat. No. 8,551,069, which is a continuation-in-part of application No. 10/408,665, filed on Apr. 8, 2003, now Pat. No. 7,162,303, said application No. 11/368,809 is a continuation-in-part of application No. 11/133,925, filed on May 20, 2005, now Pat. No. 8,771,252, which is a continuation of application No. 10/900,199, filed on Jul. 28, 2004, now Pat. No. 6,978,174, which is a continuation-in-part of application No. 10/408,665, filed on Apr. 8, 2003, now Pat. No. 7,162,303, said application No. 11/368,809 is a continuation-in-part of application No. 11/189,563, filed on Jul. 25, 2005, now Pat. No. 8,145,316, which is a continuation-in-part of application No. 11/129,765, filed on May 13, 2005, now Pat. No. 7,653,438, which is a continuation-in-part of application No. 10/408,665, filed on Apr. 8, 2003, now Pat. No. 7,162,303, said application No. 11/368,809 is a continuation-in-part of application No. 11/266,993, filed on Nov. 4, 2005, now Pat. No. 7,756,583, which is a continuation-in-part of

application No. 11/363,867, filed on Feb. 27, 2006, now Pat. No. 7,620,451, which is a continuation-in-part of application No. 11/189,563, filed on Jul. 25, 2005, now Pat. No. 8,145,316, which is a continuation-in-part of application No. 11/266,993, filed on Nov. 4, 2005, now Pat. No. 7,756,583.


(60) Provisional application No. 60/442,970, filed on Jan. 29, 2003, provisional application No. 60/415,575, filed on Oct. 3, 2002, provisional application No. 60/370,190, filed on Apr. 8, 2002, provisional application No. 60/616,254, filed on Oct. 5, 2004, provisional application No. 60/624,793, filed on Nov. 2, 2004, provisional application No. 60/813,589, filed on Dec. 29, 2005.

Publication Classification

(51) **Int. Cl.**
A61B 18/12 (2006.01)
A61B 18/04 (2006.01)
A61N 7/00 (2006.01)
A61N 1/36 (2006.01)
(52) **U.S. Cl.**
CPC *A61B 18/12* (2013.01); *A61N 1/36117* (2013.01); *A61B 18/04* (2013.01); *A61N 7/00* (2013.01); *A61B 2018/00434* (2013.01)
USPC ... **514/789**; 606/32; 607/44; 606/27; 606/169

(57) **ABSTRACT**

Methods and apparatus are provided for treating contrast nephropathy, e.g., via a pulsed electric field, via a stimulation electric field, via localized drug delivery, via high frequency ultrasound, via thermal techniques, etc. Such neuromodulation may effectuate irreversible electroporation or electrofusion, necrosis and/or inducement of apoptosis, alteration of gene expression, action potential attenuation or blockade, changes in cytokine up-regulation and other conditions in target neural fibers. In some embodiments, neuromodulation is applied to neural fibers that contribute to renal function. In some embodiments, such neuromodulation is performed in a bilateral fashion. Bilateral renal neuromodulation may provide enhanced therapeutic effect in some patients as compared to renal neuromodulation performed unilaterally, i.e., as compared to renal neuromodulation performed on neural tissue innervating a single kidney.

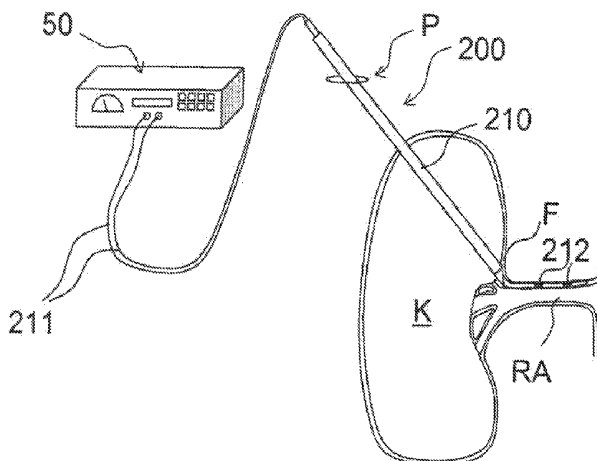

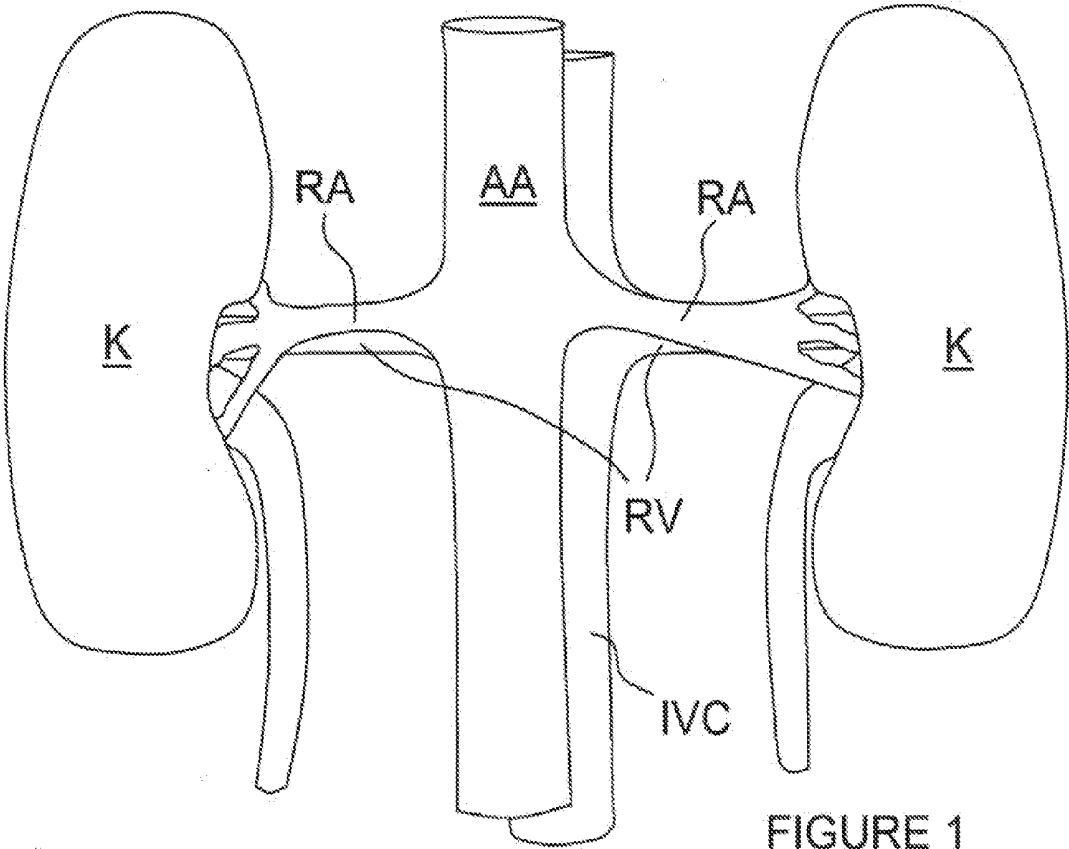
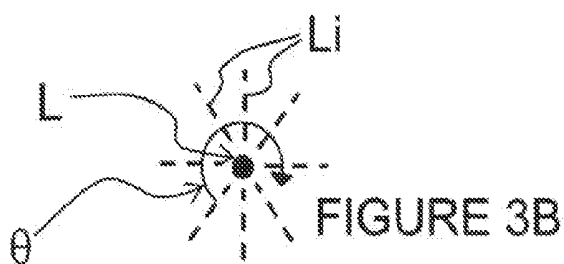
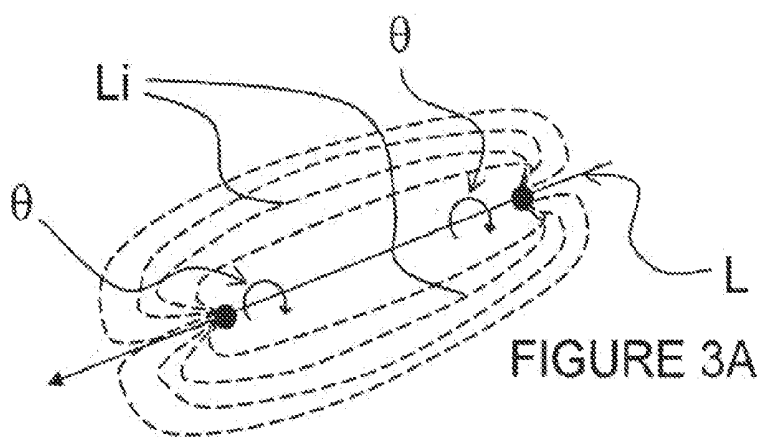
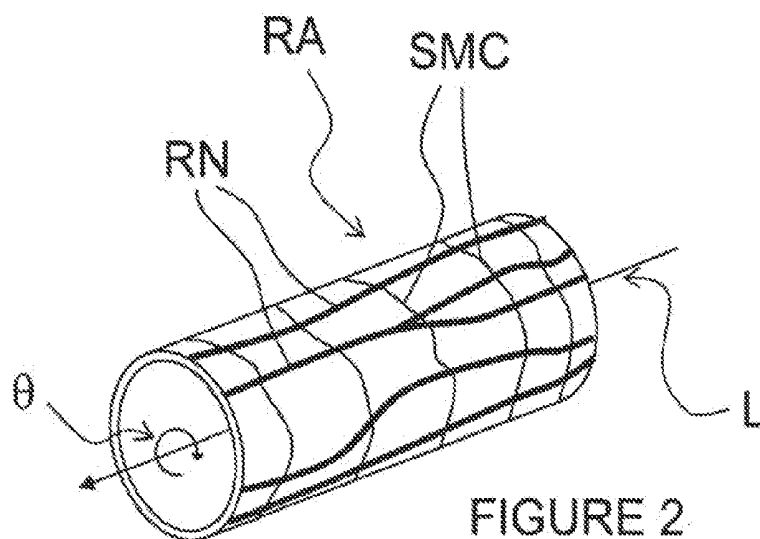
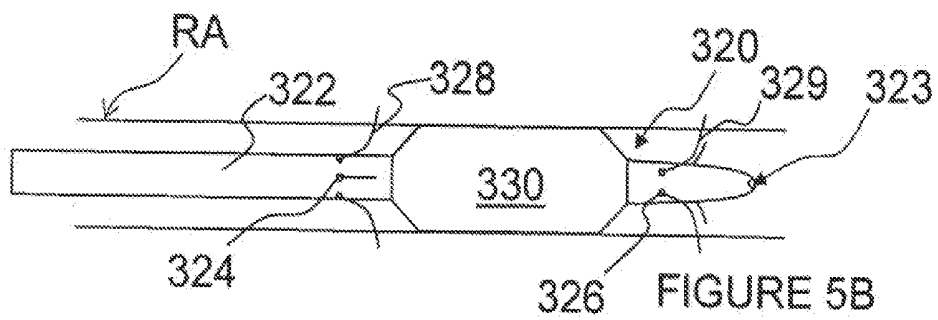
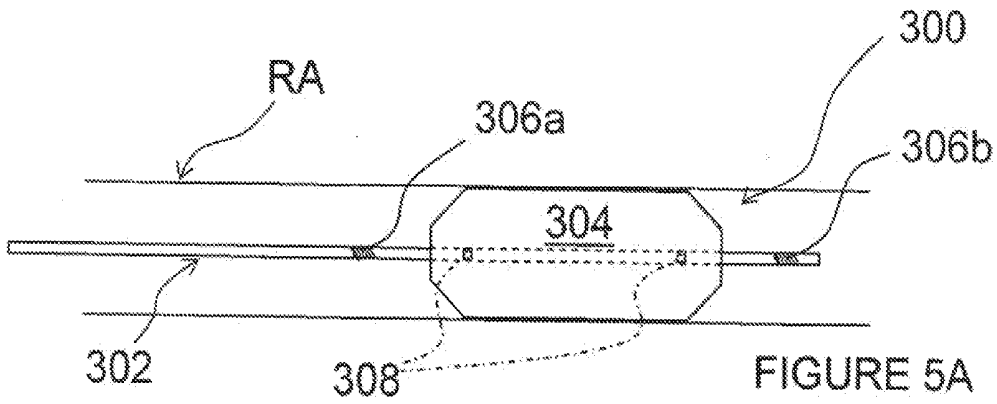
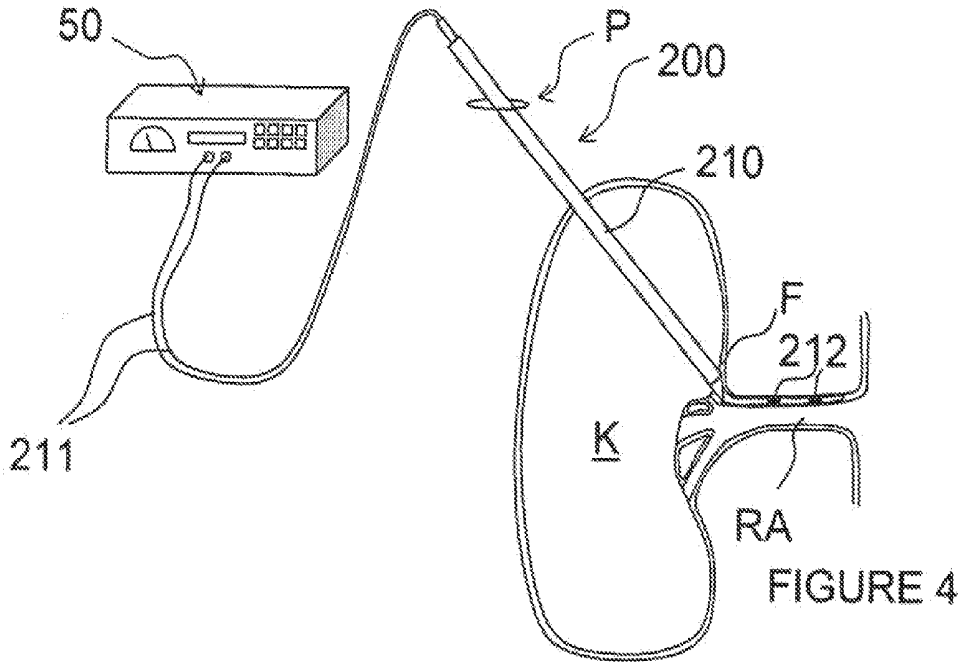


FIGURE 1





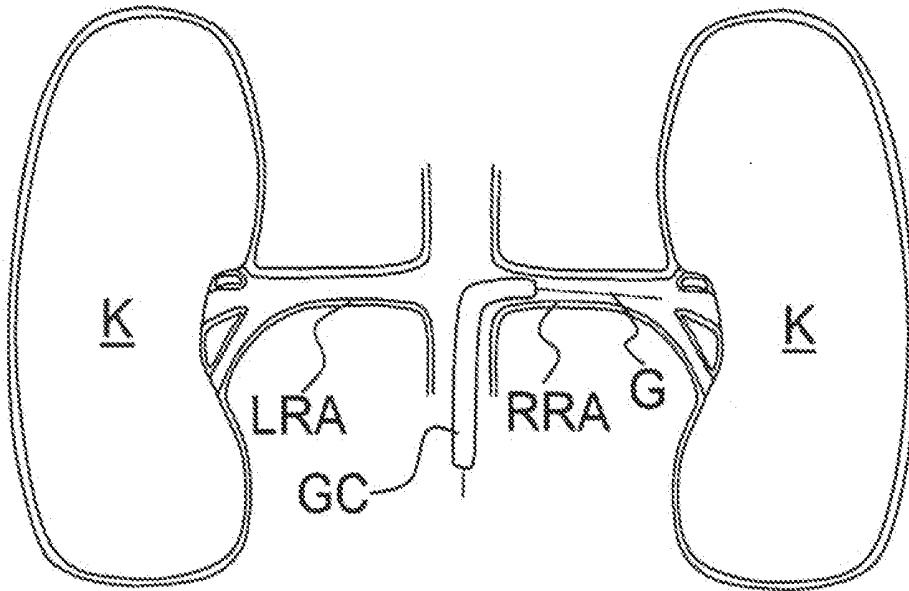


FIGURE 6A

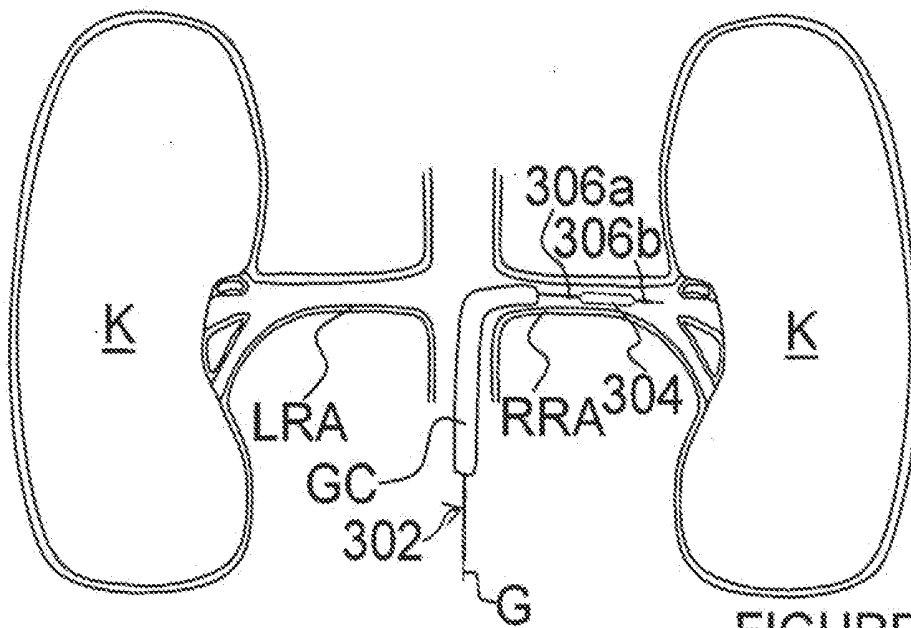


FIGURE 6B

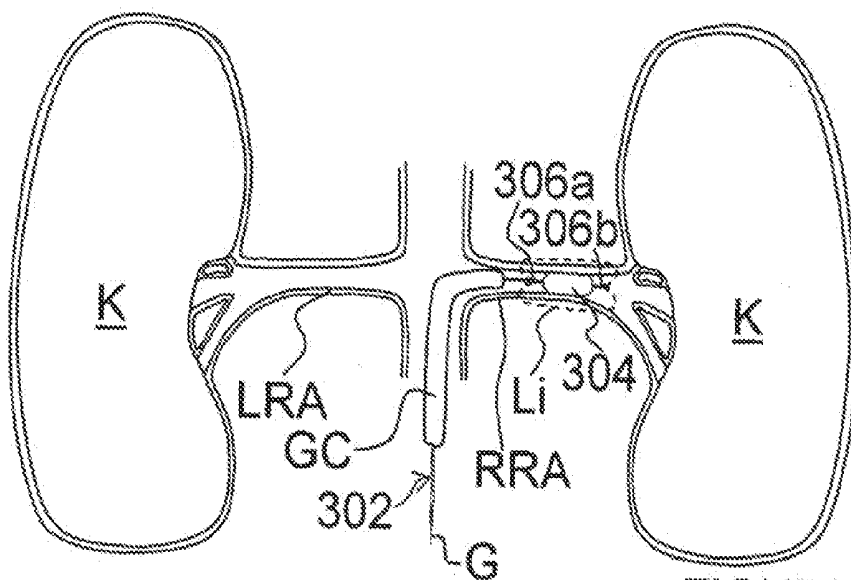


FIGURE 6C

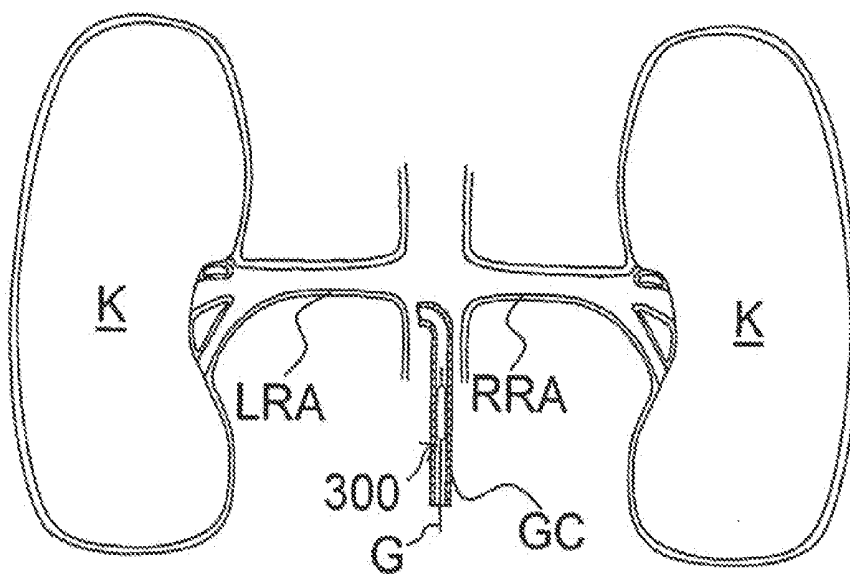


FIGURE 6D

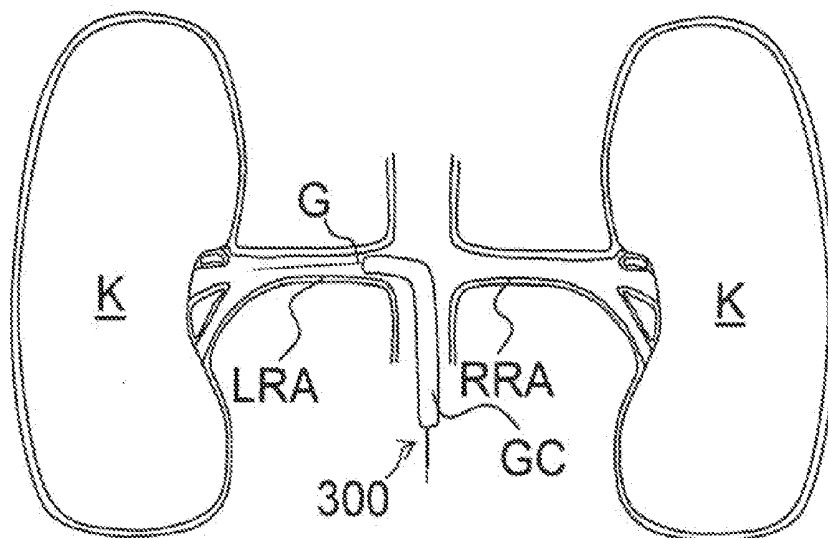


FIGURE 6E

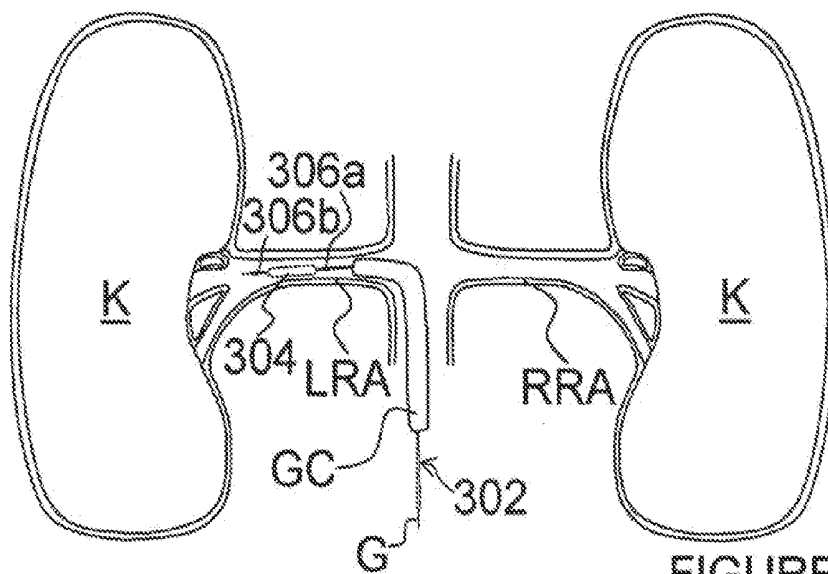


FIGURE 6F

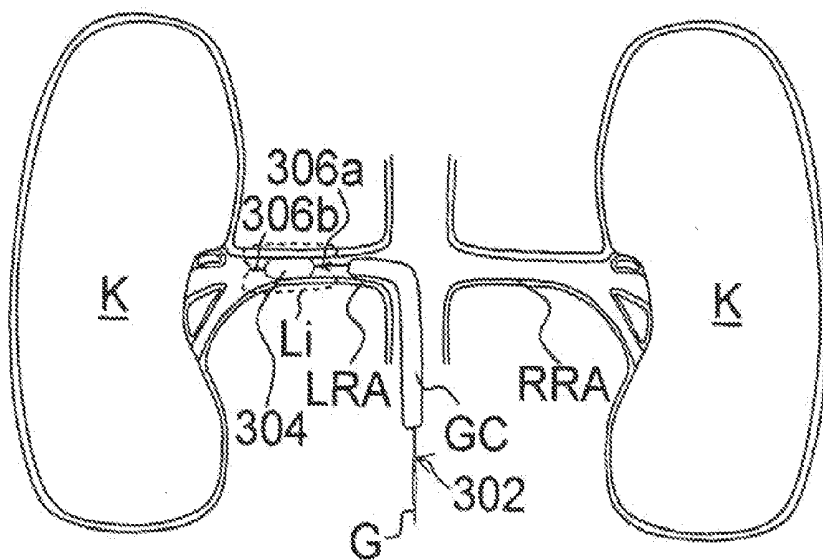


FIGURE 6G

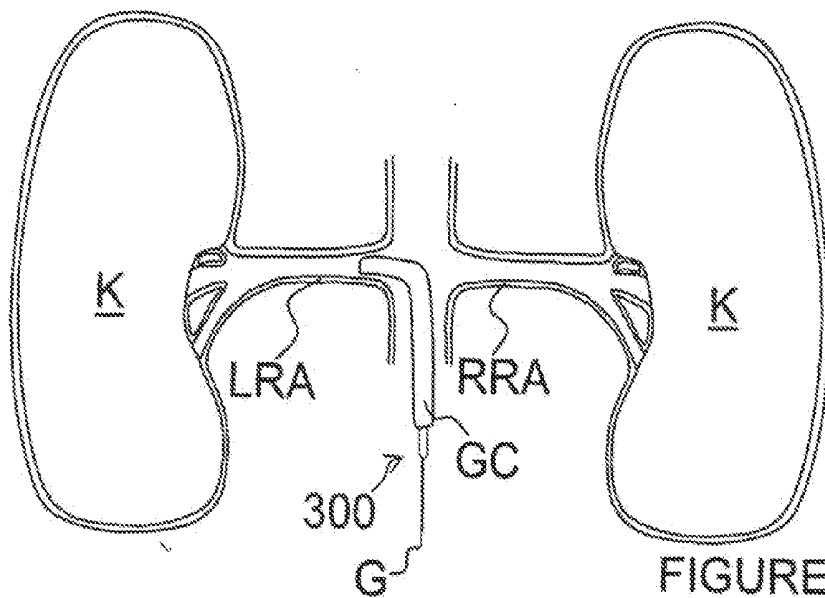
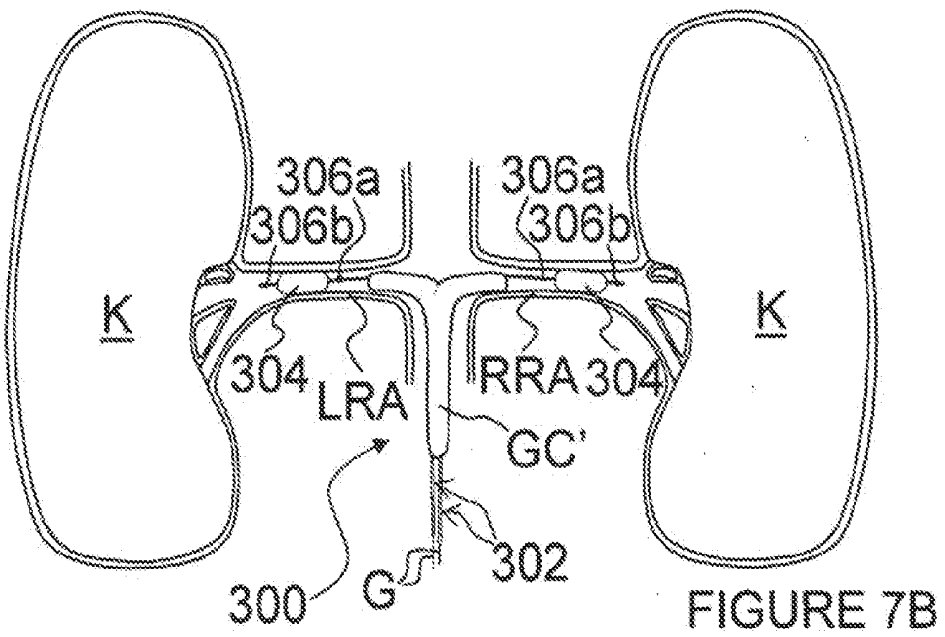
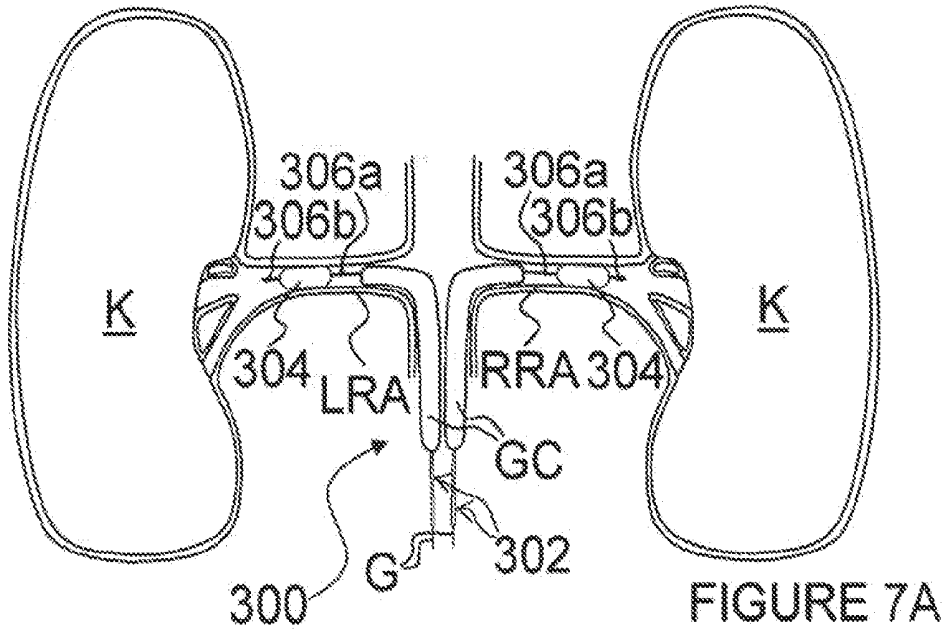


FIGURE 6H



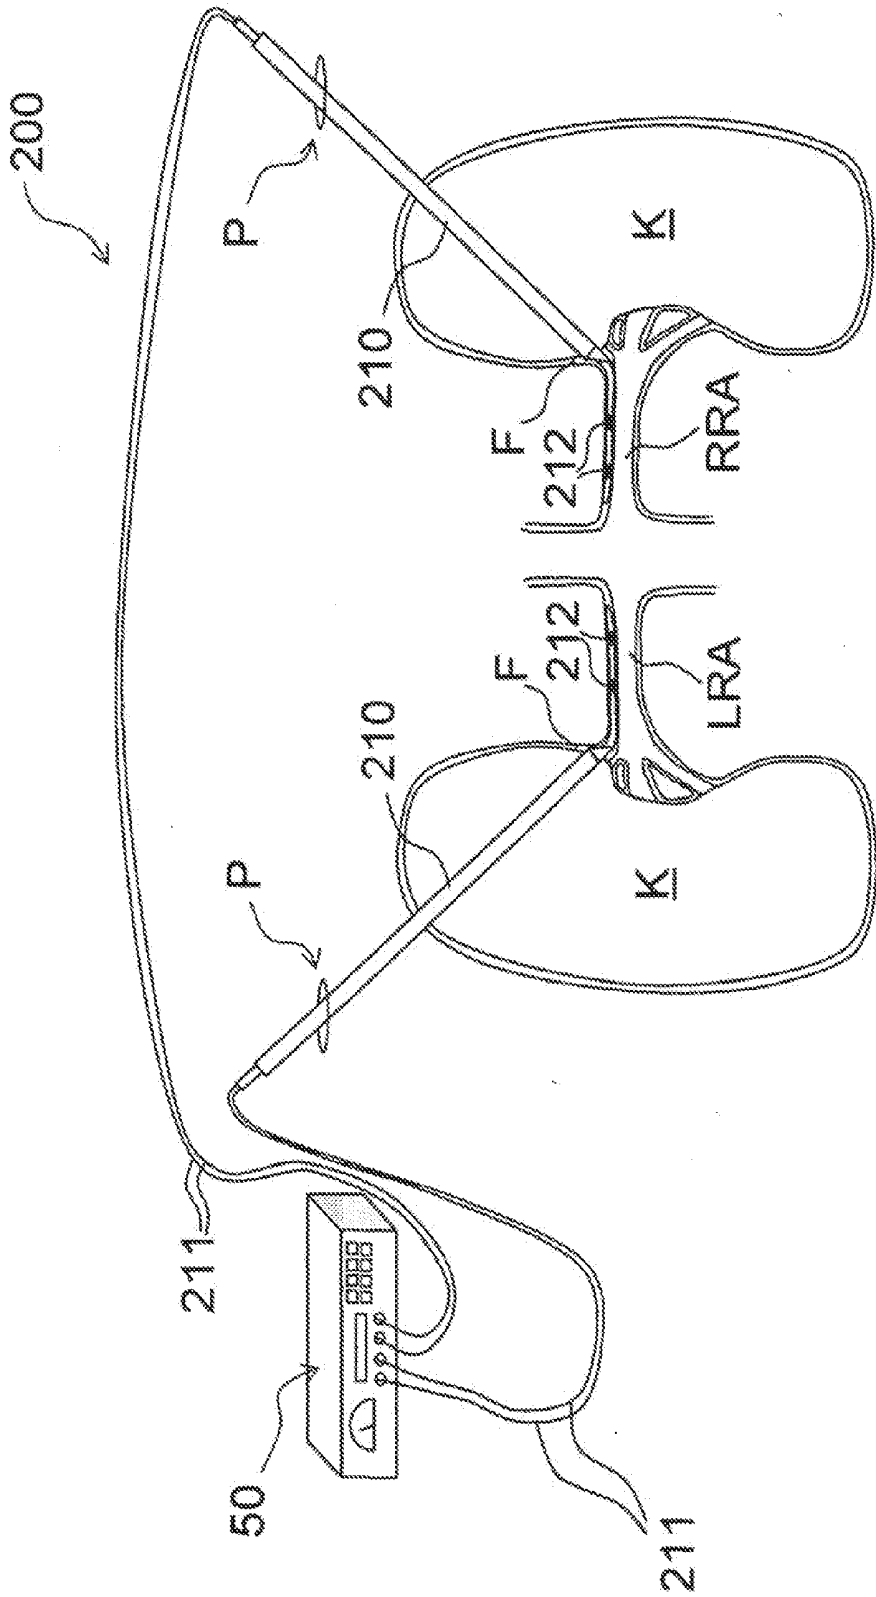


FIGURE 8

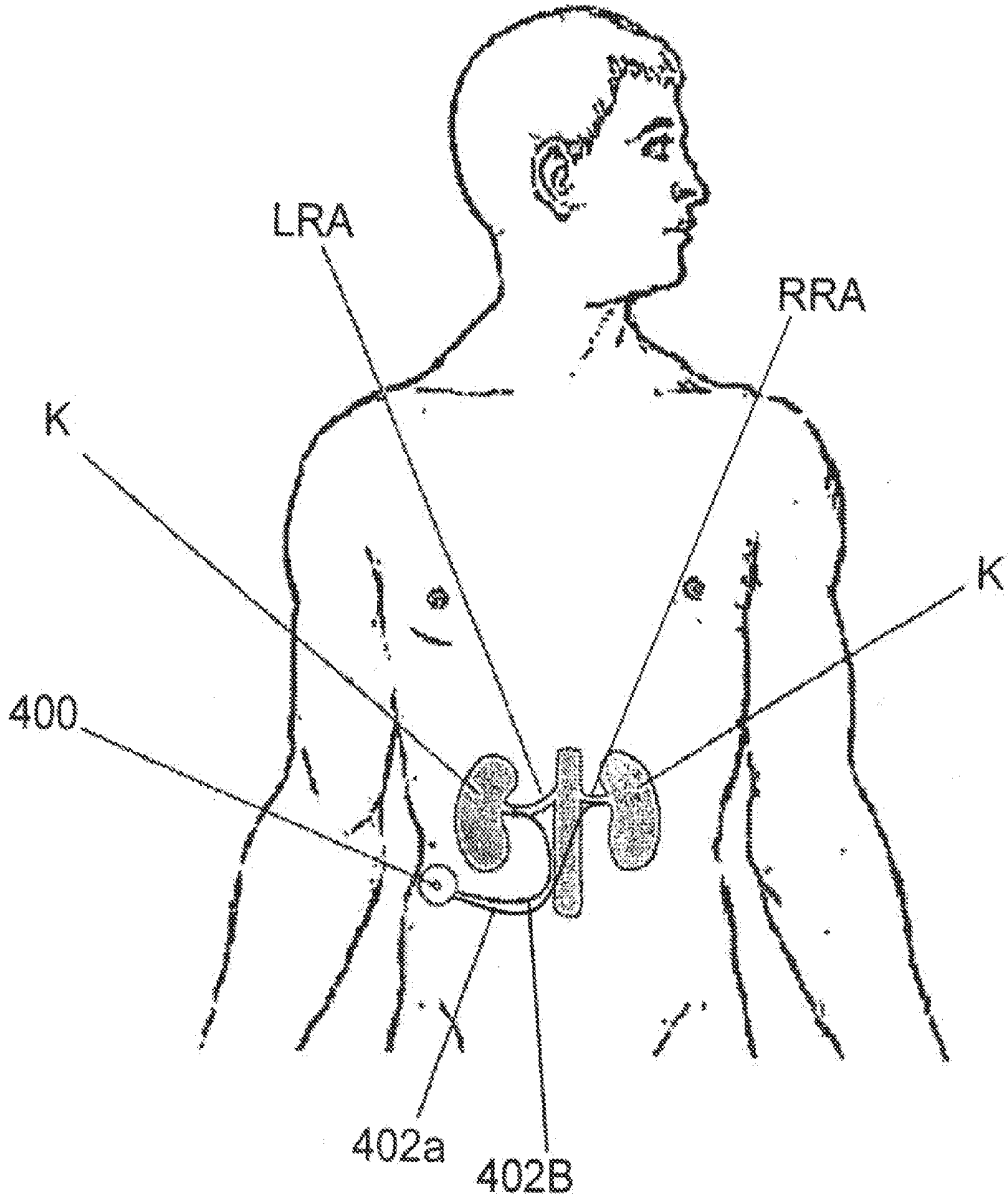


Figure 9

METHODS FOR RENAL NEUROMODULATION

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] The present application is a continuation-in-part of each of the following co-pending United States patent applications:

[0002] (1) U.S. patent application Ser. No. 10/408,665, filed on Apr. 8, 2003 (published as United States Patent Publication 2003/0216792 on Nov. 20, 2003), which claims the benefit of U.S. Provisional Patent Application Nos. 60/442,970, filed on Jan. 29, 2003; 60/415,575, filed on Oct. 3, 2002; and 60/370,190, filed on Apr. 8, 2002.

[0003] (2) U.S. patent application Ser. No. 11/133,925, filed on May 20, 2005, which is a continuation of U.S. patent application Ser. No. 10/900,199, filed on Jul. 28, 2004 (now U.S. Pat. No. 6,978,174), which is a continuation-in-part of U.S. patent application Ser. No. 10/408,665, filed on Apr. 8, 2003.

[0004] (3) U.S. patent application Ser. No. 11/189,563, filed on Jul. 25, 2005, which is a continuation-in-part of U.S. patent application Ser. No. 11/129/765, filed on May 13, 2005, which claims the benefit of U.S. Provisional Patent Application Nos. 60/616,254, filed on Oct. 5, 2004; and 60/624,793, filed on Nov. 2, 2004.

[0005] (4) U.S. patent application Ser. No. 11/266,933, filed on Nov. 4, 2005.

[0006] (5) U.S. patent application Ser. No. _____, filed on Feb. 27, 2006, entitled Methods and Apparatus for Pulsed Electric Field Neuromodulation Via an Intra-To-Extravascular Approach (Attorney Docket No. 57856.8010US1), which (a) claims the benefit of U.S. Provisional Application No. _____, filed on Dec. 29, 2005, entitled Methods and Apparatus for Pulsed Electric Field Neuromodulation Via an Intra-To-Extravascular Approach (Attorney Docket No. 57856.8010US and originally filed as U.S. application Ser. No. 11/324,188), and (b) is a continuation-in-part of each of U.S. patent application Ser. No. 11/189,563, filed on Jul. 25, 2005, and U.S. patent application Ser. No. 11/266,933, filed on Nov. 4, 2005.

[0007] All of the foregoing applications, publication and patent are incorporated herein by reference in their entireties.

INCORPORATION BY REFERENCE

[0008] All publications and patent applications mentioned in this specification are herein incorporated by reference to the same extent as if each individual publication or patent application was specifically and individually indicated to be incorporated by reference.

TECHNICAL FIELD

[0009] The present invention relates to methods and apparatus for neuromodulation. In some embodiments, the present invention relates to methods and apparatus for achieving bilateral renal neuromodulation.

BACKGROUND

[0010] Congestive Heart failure (“CHF”) is a condition that occurs when the heart becomes damaged and reduces blood flow to the organs of the body. If blood flow decreases sufficiently, kidney function becomes altered, which results in fluid retention, abnormal hormone secretions and increased

constriction of blood vessels. These results increase the workload of the heart and further decrease the capacity of the heart to pump blood through the kidneys and circulatory system.

[0011] It is believed that progressively decreasing perfusion of the kidneys is a principal non-cardiac cause perpetuating the downward spiral of CHF. Moreover, the fluid overload and associated clinical symptoms resulting from these physiologic changes result in additional hospital admissions, poor quality of life and additional costs to the health care system.

[0012] In addition to their role in the progression of CHF, the kidneys play a significant role in the progression of Chronic Renal Failure (“CRF”), End-Stage Renal Disease (“ESRD”), hypertension (pathologically high blood pressure) and other cardio-renal diseases. The functions of the kidneys can be summarized under three broad categories: filtering blood and excreting waste products generated by the body’s metabolism; regulating salt, water, electrolyte and acid-base balance; and secreting hormones to maintain vital organ blood flow. Without properly functioning kidneys, a patient will suffer water retention, reduced urine flow and an accumulation of waste toxins in the blood and body. These conditions result from reduced renal function or renal failure (kidney failure) and are believed to increase the workload of the heart. In a CHF patient, renal failure will cause the heart to further deteriorate as fluids are retained and blood toxins accumulate due to the poorly functioning kidneys.

[0013] It has been established in animal models that the heart failure condition results in abnormally high sympathetic activation of the kidneys. An increase in renal sympathetic nerve activity leads to decreased removal of water and sodium from the body, as well as increased renin secretion. Increased renin secretion leads to vasoconstriction of blood vessels supplying the kidneys which causes decreased renal blood flow. Reduction of sympathetic renal nerve activity, e.g., via denervation, may reverse these processes.

[0014] Applicants have previously described methods and apparatus for treating renal disorders by applying a pulsed electric field to neural fibers that contribute to renal function. See, for example, Applicants’ co-pending U.S. patent application Ser. No. 11/129,765, filed on May 13, 2005, and Ser. No. 11/189,563, filed on Jul. 25, 2005, both of which are incorporated herein by reference in their entireties. A pulsed electric field (“PEF”) may initiate renal neuromodulation, e.g., denervation, for example, via irreversible electroporation or via electrofusion. The PEF may be delivered from apparatus positioned intravascularly, extravascularly, intra-to-extravascularly or a combination thereof. Additional methods and apparatus for achieving renal neuromodulation, e.g., via localized drug delivery (such as by a drug pump or infusion catheter) or via use of a stimulation electric field, etc, are described, for example, in co-owned and co-pending U.S. patent application Ser. No. 10/408,665, filed Apr. 8, 2003, and U.S. Pat. No. 6,978,174, both of which are incorporated herein by reference in their entireties.

[0015] As used herein, electrofusion comprises fusion of neighboring cells induced by exposure to an electric field. Contact between target neighboring cells for the purposes of electrofusion may be achieved in a variety of ways, including, for example, via dielectrophoresis. In tissue, the target cells may already be in contact, thus facilitating electrofusion.

[0016] As used herein, electroporation and electropermeabilization are methods of manipulating the cell membrane or intracellular apparatus. For example, the porosity of a cell

membrane may be increased by inducing a sufficient voltage across the cell membrane through, e.g., short, high-voltage pulses. The extent of porosity in the cell membrane (e.g., size and number of pores) and the duration of effect (e.g., temporary or permanent) are a function of multiple variables, such as field strength, pulse width, duty cycle, electric field orientation, cell type or size and/or other parameters.

[0017] Cell membrane pores will generally close spontaneously upon termination of relatively lower strength electric fields or relatively shorter pulse widths (herein defined as “reversible electroporation”). However, each cell or cell type has a critical threshold above which pores do not close such that pore formation is no longer reversible; this result is defined as “irreversible electroporation,” “irreversible breakdown” or “irreversible damage.” At this point, the cell membrane ruptures and/or irreversible chemical imbalances caused by the high porosity occur. Such high porosity can be the result of a single large hole and/or a plurality of smaller holes.

[0018] A potential challenge of using intravascular PEF systems for treating renal disorders is to selectively electroporate target cells without affecting other cells. For example, it may be desirable to irreversibly electroporate renal nerve cells that travel along or in proximity to renal vasculature, but it may not be desirable to damage the smooth muscle cells of which the vasculature is composed. As a result, an overly aggressive course of PEF therapy may persistently injure the renal vasculature, but an overly conservative course of PEF therapy may not achieve the desired renal neuromodulation.

[0019] Applicants have previously described methods and apparatus for monitoring tissue impedance or conductivity to determine the effects of pulsed electric field therapy, e.g., to determine an extent of electroporation and/or its degree of irreversibility. See, for example, Applicant’s co-pending U.S. patent application Ser. No. 11/233,814, filed Sep. 23, 2005, which is incorporated herein by reference in its entirety. Pulsed electric field electroporation of tissue causes a decrease in tissue impedance and an increase in tissue conductivity. If induced electroporation is reversible, tissue impedance and conductivity should approximate baseline levels upon cessation of the pulsed electric field. However, if electroporation is irreversible, impedance and conductivity changes should persist after terminating the pulsed electric field. Thus, monitoring the impedance or conductivity of target and/or non-target tissue may be utilized to determine the onset of electroporation and to determine the type or extent of electroporation. Furthermore, monitoring data may be used in one or more manual or automatic feedback loops to control the electroporation.

[0020] It would be desirable to provide methods and apparatus for achieving bilateral renal neuromodulation.

SUMMARY

[0021] The present invention provides methods and apparatus for neuromodulation, e.g., via a pulsed electric field (“PEF”), via a stimulation electric field, via localized drug delivery, via high frequency ultrasound, via thermal techniques, combinations thereof, etc. Such neuromodulation may, for example, effectuate irreversible electroporation or electrofusion, necrosis and/or inducement of apoptosis, alteration of gene expression, action potential blockade or attenuation, changes in cytokine up-regulation and other conditions in target neural fibers. In some patients, when the neuromodulatory methods and apparatus of the present invention are

applied to renal nerves and/or other neural fibers that contribute to renal neural functions, applicants believe that the neuromodulatory effects induced by the neuromodulation might result in increased urine output, decreased plasma renin levels, decreased tissue (e.g., kidney) and/or urine catecholamines (e.g., norepinephrine), increased urinary sodium excretion, and/or controlled blood pressure. Furthermore, applicants believe that these or other changes might prevent or treat congestive heart failure, hypertension, acute myocardial infarction, end-stage renal disease, contrast nephropathy, other renal system diseases, and/or other renal or cardiorenal anomalies. The methods and apparatus described herein could be used to modulate efferent or afferent nerve signals, as well as combinations of efferent and afferent nerve signals.

[0022] Renal neuromodulation preferably is performed in a bilateral fashion, such that neural fibers contributing to renal function of both the right and left kidneys are modulated. Bilateral renal neuromodulation may provide enhanced therapeutic effect in some patients as compared to renal neuromodulation performed unilaterally, i.e., as compared to renal neuromodulation performed on neural tissue innervating a single kidney. In some embodiments, concurrent modulation of neural fibers that contribute to both right and left renal function may be achieved. In additional or alternative embodiments, such modulation of the right and left neural fibers may be sequential. Bilateral renal neuromodulation may be continuous or intermittent, as desired.

[0023] When utilizing an electric field, the electric field parameters may be altered and combined in any combination, as desired. Such parameters can include, but are not limited to, voltage, field strength, pulse width, pulse duration, the shape of the pulse, the number of pulses and/or the interval between pulses (e.g., duty cycle), etc. For example, when utilizing a pulsed electric field, suitable field strengths can be up to about 10,000 V/cm and suitable pulse widths can be up to about 1 second. Suitable shapes of the pulse waveform include, for example, AC waveforms, sinusoidal waves, cosine waves, combinations of sine and cosine waves, DC waveforms, DC-shifted AC waveforms, RF waveforms, square waves, trapezoidal waves, exponentially-decaying waves, or combinations. The field includes at least one pulse, and in many applications the field includes a plurality of pulses. Suitable pulse intervals include, for example, intervals less than about 10 seconds. These parameters are provided as suitable examples and in no way should be considered limiting.

BRIEF DESCRIPTION OF THE DRAWINGS

[0024] Several embodiments of the present invention will be apparent upon consideration of the following detailed description, taken in conjunction with the accompanying drawings, in which like reference characters refer to like parts throughout, and in which:

[0025] FIG. 1 is a schematic view illustrating human renal anatomy.

[0026] FIG. 2 is a schematic isometric detail view showing the location of the renal nerves relative to the renal artery.

[0027] FIGS. 3A and 3B are schematic isometric and end views, respectively, illustrating orienting of an electric field for selectively affecting renal nerves.

[0028] FIG. 4 is a schematic side view, partially in section, illustrating an example of an extravascular method and apparatus for renal neuromodulation.

[0029] FIGS. 5A and 5B are schematic side views, partially in section, illustrating examples of, respectively, intravascular and intra-to-extravascular methods and apparatus for renal neuromodulation.

[0030] FIGS. 6A-6H are schematic side views, partially in section, illustrating methods of achieving bilateral renal neuromodulation utilizing apparatus of the present invention, illustratively utilizing the apparatus of FIG. 5A.

[0031] FIGS. 7A and 7B are schematic side views, partially in section, illustrating methods of achieving concurrent bilateral renal neuromodulation utilizing embodiments of the apparatus of FIG. 5A.

[0032] FIG. 8 is a schematic side view, partially in section, illustrating methods of achieving concurrent bilateral renal neuromodulation utilizing an alternative embodiment of the apparatus of FIG. 4.

[0033] FIG. 9 is a schematic view illustrating an example of methods and apparatus for achieving bilateral renal neuromodulation via localized drug delivery.

DETAILED DESCRIPTION

A. Overview

[0034] The present invention relates to methods and apparatus for neuromodulation, e.g., denervation. In some embodiments, the present invention provides methods and apparatus for achieving bilateral renal neuromodulation. Bilateral renal neuromodulation may provide enhanced therapeutic effect in some patients as compared to renal neuromodulation performed unilaterally, i.e., as compared to renal neuromodulation performed on neural tissue innervating a single kidney. In some embodiments, concurrent modulation of neural fibers that contribute to both right and left renal function may be achieved. In additional or alternative embodiments, such modulation of the right and left neural fibers may be sequential. Bilateral renal neuromodulation may be continuous or intermittent, as desired.

[0035] The methods and apparatus of the present invention may be used to modulate neural fibers that contribute to renal function and may exploit any suitable neuromodulatory techniques that will achieve the desired neuromodulation. For example, any suitable electrical signal or field parameters, e.g., any electric field that will achieve the desired neuromodulation (e.g., electroporative effect) may be utilized. Alternatively or additionally, neuromodulation may be achieved via localized delivery of a neuromodulatory agent or drug. To better understand the structures of devices of the present invention and the methods of using such devices for bilateral renal neuromodulation, it is instructive to examine the renal anatomy in humans.

B. Selected Embodiments of Methods for Neuromodulation

[0036] With reference now to FIG. 1, the human renal anatomy includes kidneys K that are supplied with oxygenated blood by renal arteries RA, which are connected to the heart by the abdominal aorta AA. Deoxygenated blood flows from the kidneys to the heart via renal veins RV and the inferior vena cava IVC. FIG. 2 illustrates a portion of the renal anatomy in greater detail. More specifically, the renal anatomy also includes renal nerves RN extending longitudinally along the lengthwise dimension L of renal artery RA generally within the adventitia of the artery. The renal artery RA has smooth muscle cells SMC that surround the arterial

circumference and spiral around the angular axis θ of the artery. The smooth muscle cells of the renal artery accordingly have a lengthwise or longer dimension extending transverse (i.e., non-parallel) to the lengthwise dimension of the renal artery. The misalignment of the lengthwise dimensions of the renal nerves and the smooth muscle cells is defined as "cellular misalignment."

[0037] Referring to FIGS. 3A and 3B, the cellular misalignment of the renal nerves and the smooth muscle cells may be exploited to selectively affect renal nerve cells with reduced effect on smooth muscle cells. More specifically, because larger cells require a lower electric field strength to exceed the cell membrane irreversibility threshold voltage or energy for irreversible electroporation, embodiments of electrodes of the present invention may be configured to align at least a portion of an electric field generated by the electrodes with or near the longer dimensions of the cells to be affected. In specific embodiments, the device has electrodes configured to create an electrical field aligned with or near the lengthwise dimension L of the renal artery RA to affect renal nerves RN. By aligning an electric field so that the field preferentially aligns with the lengthwise aspect of the cell rather than the diametric or radial aspect of the cell, lower field strengths may be used to affect target neural cells, e.g., to necrose or fuse the target cells, to induce apoptosis, to alter gene expression, to attenuate or block action potentials, to change cytokine up-regulation and/or to induce other suitable processes. This is expected to reduce total energy delivered to the system and to mitigate effects on non-target cells in the electric field.

[0038] Similarly, the lengthwise or longer dimensions of tissues overlying or underlying the target nerve are orthogonal or otherwise off-axis (e.g., transverse) with respect to the longer dimensions of the nerve cells. Thus, in addition to aligning a pulsed electric field ("PEF") with the lengthwise or longer dimensions of the target cells, the PEF may propagate along the lateral or shorter dimensions of the non-target cells (i.e., such that the PEF propagates at least partially out of alignment with non-target smooth muscle cells SMC). Therefore, as seen in FIGS. 3A and 3B, applying a PEF with propagation lines LI generally aligned with the longitudinal dimension L of the renal artery RA is expected to preferentially cause electroporation (e.g., irreversible electroporation), electrofusion or other neuromodulation in cells of the target renal nerves RN without unduly affecting the non-target arterial smooth muscle cells SMC. The pulsed electric field may propagate in a single plane along the longitudinal axis of the renal artery, or may propagate in the longitudinal direction along any angular segment θ through a range of 0° - 360° .

[0039] A PEF system placed within and/or in proximity to the wall of the renal artery may propagate an electric field having a longitudinal portion that is aligned to run with the longitudinal dimension of the artery in the region of the renal nerves RN and the smooth muscle cells SMC of the vessel wall so that the wall of the artery remains at least substantially intact while the outer nerve cells are destroyed, fused or otherwise affected. Monitoring elements may be utilized to assess an extent of, e.g., electroporation, induced in renal nerves and/or in smooth muscle cells, as well as to adjust PEF parameters to achieve a desired effect.

C. Exemplary Embodiments of Systems and Additional Methods for Neuromodulation

[0040] With reference to FIGS. 4 and 5, examples of PEF systems and methods are described. FIG. 4 shows one

embodiment of an extravascular pulsed electric field apparatus **200** that includes one or more electrodes configured to deliver a pulsed electric field to renal neural fibers to achieve renal neuromodulation. The apparatus of FIG. **4** is configured for temporary extravascular placement; however, it should be understood that partially or completely implantable extravascular apparatus additionally or alternatively may be utilized. Applicants have previously described extravascular PEF systems, for example, in co-pending U.S. patent application Ser. No. 11/189,563, filed Jul. 25, 2005, which has been incorporated herein by reference in its entirety.

[0041] In FIG. **4**, apparatus **200** comprises a laparoscopic or percutaneous PEF system having a probe **210** configured for insertion in proximity to the track of the renal neural supply along the renal artery or vein or hilum and/or within Gerota's fascia under, e.g., CT or radiographic guidance. At least one electrode **212** is configured for delivery through the probe **210** to a treatment site for delivery of pulsed electric field therapy. The electrode(s) **212**, for example, may be mounted on a catheter and electrically coupled to a pulse generator **50** via wires **211**. In an alternative embodiment, a distal section of the probe **210** may have one electrode **212**, and the probe may have an electrical connector to couple the probe to the pulse generator **50** for delivering a PEF to the electrodes(s) **212**.

[0042] The pulsed electric field generator **50** is located external to the patient. The generator, as well as any of the PEF-delivery electrode embodiments described herein, may be utilized with any embodiment of the present invention for delivery of a PEF with desired field parameters. It should be understood that PEF-delivery electrodes of embodiments described hereinafter may be electrically connected to the generator even though the generator is not explicitly shown or described with each embodiment.

[0043] The electrode(s) **212** can be individual electrodes that are electrically independent of each other, a segmented electrode with commonly connected contacts, or a continuous electrode. A segmented electrode may, for example, be formed by providing a slotted tube fitted onto the electrode, or by electrically connecting a series of individual electrodes. Individual electrodes or groups of electrodes **212** may be configured to provide a bipolar signal. The electrodes **212** may be dynamically assignable to facilitate monopolar and/or bipolar energy delivery between any of the electrodes and/or between any of the electrodes and an external ground pad. Such a ground pad may, for example, be attached externally to the patient's skin, e.g., to the patient's leg or flank. In FIG. **4**, the electrodes **212** comprise a bipolar electrode pair. The probe **210** and the electrodes **212** may be similar to the standard needle or trocar-type used clinically for pulsed RF nerve block. Alternatively, the apparatus **200** may comprise a flexible and/or custom-designed probe for the renal application described herein.

[0044] In FIG. **4**, the percutaneous probe **210** has been advanced through a percutaneous access site P into proximity with a patient's renal artery RA. The probe pierces the patient's Gerota's fascia F, and the electrodes **212** are advanced into position through the probe and along the annular space between the patient's artery and fascia. Once properly positioned, pulsed electric field therapy may be applied to target neural fibers across the bipolar electrodes **212**. Such PEF therapy may, for example, at least partially denervate the kidney innervated by the target neural fibers through irreversible electroporation of cells of the target neural fibers. The

electrodes **212** optionally also may be used to monitor the electroporative effects of the PEF therapy. After treatment, the apparatus **200** may be removed from the patient to conclude the procedure.

[0045] Referring now to FIG. **5A**, an embodiment of an intravascular PEF system is described. Applicants have previously described intravascular PEF systems, for example, in co-pending U.S. patent application Ser. No. 11/129,765, filed May 13, 2005, which has been incorporated herein by reference in its entirety. The embodiment of FIG. **5A** includes an apparatus **300** comprising a catheter **302** having a centering element **304** (e.g., a balloon, an expandable wire basket, other mechanical expanders, etc.), shaft electrodes **306a** and **306b** disposed along the shaft of the catheter, and optional radiopaque markers **308** disposed along the shaft of the catheter in the region of the centering element **304**. The electrodes **306a-b**, for example, can be arranged such that the electrode **306a** is near a proximal end of the centering element **304** and the electrode **306b** is near the distal end of the centering element **304**. The electrodes **306** are electrically coupled to the pulse generator **50** (see FIG. **4**), which is disposed external to the patient, for delivery of the PEF therapy.

[0046] The centering element **304** may comprise an impedance-altering element that alters the impedance between electrodes **306a** and **306b** during the PEF therapy, for example, to better direct the PEF therapy across the vessel wall. This may reduce an applied voltage required to achieve desired renal neuromodulation. Applicants have previously described use of an impedance-altering element, for example, in co-pending U.S. patent application Ser. No. 11/266,993, filed Nov. 4, 2005, which is incorporated herein by reference in its entirety. When the centering element **304** comprises an inflatable balloon, the balloon may serve as both the centering element for the electrodes **306** and as an impedance-altering electrical insulator for directing an electric field delivered across the electrodes, e.g., for directing the electric field into or across the vessel wall for modulation of target neural fibers. Electrical insulation provided by the element **304** may reduce the magnitude of applied voltage or other parameters of the pulsed electric field necessary to achieve desired field strength at the target fibers.

[0047] The electrodes **306** can be individual electrodes (i.e., independent contacts), a segmented electrode with commonly connected contacts, or a single continuous electrode. Furthermore, the electrodes **306** may be configured to provide a bipolar signal, or the electrodes **306** may be used together or individually in conjunction with a separate patient ground pad for monopolar use. As an alternative or in addition to placement of the electrodes **306** along the central shaft of catheter **302**, as in FIG. **5A**, the electrodes **306** may be attached to the centering element **304** such that they contact the wall of the renal artery RA. In such a variation, the electrodes may, for example, be affixed to the inside surface, outside surface or at least partially embedded within the wall of the centering element. The electrodes optionally may be used to monitor the effects of PEF therapy, as described hereinafter. As it may be desirable to reduce or minimize physical contact between the PEF-delivery electrodes and the vessel wall during delivery of PEF therapy, e.g., to reduce the potential for injuring the wall, the electrodes **306** may, for example, comprise a first set of electrodes attached to the shaft of the catheter for delivering the PEF therapy, and the device may further include a second set of electrodes optionally attached to the

centering element **304** for monitoring the effects of PEF therapy delivered via the electrodes **306**.

[0048] In use, the catheter **302** may be delivered to the renal artery RA as shown, or it may be delivered to a renal vein or to any other vessel in proximity to neural tissue contributing to renal function, in a low profile delivery configuration, for example, through a guide catheter. Once positioned within the renal vasculature, the optional centering element **304** may be expanded into contact with an interior wall of the vessel. A pulsed electric field then may be generated by the PEF generator **50**, transferred through the catheter **302** to the electrodes **306**, and delivered via the electrodes **306** across the wall of the artery. The PEF therapy modulates the activity along neural fibers that contribute to renal function, e.g., at least partially denervates the kidney innervated by the neural fibers. This may be achieved, for example, via irreversible electroporation, electrofusion and/or inducement of apoptosis in the nerve cells. In many applications, the electrodes are arranged so that the pulsed electric field is aligned with the longitudinal dimension of the renal artery to facilitate modulation of renal nerves with little effect on non-target smooth muscle cells or other cells.

[0049] In addition to extravascular and intravascular PEF systems, intra-to-extravascular PEF systems may be provided having electrode(s) that are delivered to an intravascular position, then at least partially passed through/across the vessel wall to an extravascular position prior to delivery of PEF therapy. Intra-to-extravascular positioning of the electrode(s) may place the electrode(s) in closer proximity to target neural fibers during the PEF therapy compared to fully intravascular positioning of the electrode(s). Applicants have previously described intra-to-extravascular PEF systems, for example, in co-pending U.S. patent application Ser. No. 11/324,188 (hereinafter, "the '188 application"), filed Dec. 29, 2005, which is incorporated herein by reference in its entirety.

[0050] With reference to FIG. 5B, one embodiment of an intra-to-extravascular ("ITEV") PEF system, described previously in the '188 application, is shown. ITEV PEF system **320** comprises a catheter **322** having (a) a plurality of proximal electrode lumens terminating at proximal side ports **324**, (b) a plurality of distal electrode lumens terminating at distal side ports **326**, and (c) a guidewire lumen **323**. The catheter **322** preferably comprises an equal number of proximal and distal electrode lumens and side ports. The system **320** also includes proximal needle electrodes **328** that may be advanced through the proximal electrode lumens and the proximal side ports **324**, as well as distal needle electrodes **329** that may be advanced through the distal electrode lumens and the distal side ports **326**.

[0051] Catheter **322** comprises an optional expandable centering element **330**, which may comprise an inflatable balloon or an expandable basket or cage. In use, the centering element **330** may be expanded prior to deployment of the needle electrodes **328** and **329** in order to center the catheter **322** within the patient's vessel (e.g., within renal artery RA). Centering the catheter **322** is expected to facilitate delivery of all needle electrodes to desired depths within/external to the patient's vessel (e.g., to deliver all of the needle electrodes approximately to the same depth). In FIG. 5B, the illustrated centering element **330** is positioned between the proximal side ports **324** and the distal side ports **326**, i.e., between the delivery positions of the proximal and distal electrodes. However, it should be understood that centering element **330** additionally or alternatively may be positioned at a different loca-

tion or at multiple locations along the length of the catheter **322** (e.g., at a location proximal of the side ports **324** and/or at a location distal of the side ports **326**).

[0052] As illustrated in FIG. 5B, the catheter **322** may be advanced to a treatment site within the patient's vasculature (e.g., to a treatment site within the patient's renal artery RA) over a guidewire (not shown) via the lumen **323**. During intravascular delivery, the electrodes **328** and **329** may be positioned such that their non-insulated and sharpened distal regions are positioned within the proximal and distal lumens, respectively. Once positioned at a treatment site, a medical practitioner may advance the electrodes via their proximal regions that are located external to the patient. Such advancement causes the distal regions of the electrodes **328** and **329** to exit side ports **324** and **326**, respectively, and pierce the wall of the patient's vasculature such that the electrodes are positioned extravascularly via an ITEV approach.

[0053] The proximal electrodes **328** can be connected to PEF generator **50** as active electrodes and the distal electrodes **329** can serve as return electrodes. In this manner, the proximal and distal electrodes form bipolar electrode pairs that align PEF therapy with a longitudinal axis or direction of the patient's vasculature. As will be apparent, the distal electrodes **329** alternatively may comprise the active electrodes and the proximal electrodes **328** may comprise the return electrodes. Furthermore, the proximal and/or the distal electrodes may comprise both active and return electrodes. Any combination of active and distal electrodes may be utilized, as desired.

[0054] When the electrodes **328** and **329** are connected to PEF generator **50** and are positioned extravascularly, and with centering element **330** optionally expanded, PEF therapy may proceed to achieve desired neuromodulation. After completion of the PEF therapy, the electrodes may be retracted within the proximal and distal lumens, and centering element **330** may be collapsed for retrieval. ITEV PEF system **320** then may be removed from the patient to complete the procedure. Additionally or alternatively, the system may be repositioned to provide PEF therapy at another treatment site, for example, to provide bilateral renal neuromodulation.

[0055] It is expected that PEF therapy, as well as other methods and apparatus of the present invention for neuromodulation (e.g., stimulation electric fields, localized drug delivery, high frequency ultrasound, thermal techniques, etc.), whether delivered extravascularly, intravascularly, intra-to-extravascularly or a combination thereof, may, for example, effectuate irreversible electroporation or electrofusion, necrosis and/or inducement of apoptosis, alteration of gene expression, action potential blockade or attenuation, changes in cytokine up-regulation and other conditions in target neural fibers. In some patients, when such neuromodulatory methods and apparatus are applied to renal nerves and/or other neural fibers that contribute to renal neural functions, applicants believe that the neuromodulatory effects induced by the neuromodulation might result in increased urine output, decreased plasma renin levels, decreased tissue (e.g., kidney) and/or urine catecholamines (e.g., norepinephrine), increased urinary sodium excretion, and/or controlled blood pressure. Furthermore, applicants believe that these or other changes might prevent or treat congestive heart failure, hypertension, acute myocardial infarction, end-stage renal disease, contrast nephropathy, other renal system diseases, and/or other renal or cardio-renal anomalies for a period of months, potentially up to six months or more. This time

period may be sufficient to allow the body to heal; for example, this period may reduce the risk of CHF onset after an acute myocardial infarction, thereby alleviating a need for subsequent re-treatment. Alternatively, as symptoms reoccur, or at regularly scheduled intervals, the patient may return to the physician for a repeat therapy. The methods and apparatus described herein could be used to modulate efferent or afferent nerve signals, as well as combinations of efferent and afferent nerve signals. Neuromodulation in accordance with the present invention preferably is achieved without completely physically severing, i.e., without fully cutting, the target neural fibers. However, it should be understood that such neuromodulation may functionally sever the neural fibers, even though the fibers may not be completely physically severed. Apparatus and methods described herein illustratively are configured for percutaneous use. Such percutaneous use may be endoluminal, laparoscopic, a combination thereof, etc.

[0056] The apparatus described above with respect to FIGS. 4 and 5 additionally may be used to quantify the efficacy, extent or cell selectivity of PEF therapy to monitor and/or control the therapy. When a pulsed electric field initiates electroporation, the impedance of the electroporated tissue begins to decrease and the conductivity of the tissue begins to increase. If the electroporation is reversible, the tissue electrical parameters will return or approximate baseline values upon cessation of the PEF. However, if the electroporation is irreversible, the changes in tissue parameters will persist after termination of the PEF. These phenomena may be utilized to monitor both the onset and the effects of PEF therapy. For example, electroporation may be monitored directly using, for example, conductivity measurements or impedance measurements, such as Electrical Impedance Tomography (“EIT”) and/or other electrical impedance/conductivity measurements like an electrical impedance or conductivity index. Such electroporation monitoring data optionally may be used in one or more feedback loops to control delivery of PEF therapy.

[0057] In order to collect the desired monitoring data, additional monitoring electrodes optionally may be provided in proximity to the monitored tissue. The distance between such monitoring electrodes preferably would be specified prior to therapy delivery and used to determine conductivity from impedance or conductance measurements. For the purposes of the present invention, the imaginary part of impedance may be ignored such that impedance is defined as voltage divided by current, while conductance may be defined as the inverse of impedance (i.e., current divided by voltage), and conductivity may be defined as conductance per unit distance. Applicants have previously described methods and apparatus for monitoring PEF therapy, as well as exemplary PEF waveforms, in co-pending U.S. patent application Ser. No. 11/233, 814, filed Sep. 23, 2005, which has been incorporated herein by reference in its entirety.

[0058] Although the embodiments of FIGS. 4 and 5 illustratively comprise bipolar apparatus, it should be understood that monopolar apparatus alternatively may be utilized. For example, an active monopolar electrode may be positioned intravascularly, extravascularly or intra-to-extravascularly in proximity to target neural fibers that contribute to renal function. A return electrode ground pad may be attached to the exterior of the patient. Finally, PEF therapy may be delivered between the in vivo monopolar electrode and the ground

pad to effectuate desired renal neuromodulation. Monopolar apparatus additionally may be utilized for bilateral renal neuromodulation.

[0059] It may be desirable to achieve bilateral renal neuromodulation. Bilateral neuromodulation may enhance the therapeutic effect in some patients as compared to renal neuromodulation performed unilaterally, i.e., as compared to renal neuromodulation performed on neural tissue innervating a single kidney. For example, bilateral renal neuromodulation may further reduce clinical symptoms of CHF, hypertension, acute myocardial infarction, contrast nephropathy, renal disease and/or other cardio-renal diseases. FIGS. 6A-6H illustrate stages of a method for bilateral renal neuromodulation utilizing the intravascular apparatus of FIG. 5A. However, it should be understood that such bilateral neuromodulation alternatively may be achieved utilizing the extravascular apparatus of FIG. 4, utilizing the intra-to-extravascular apparatus of FIG. 5B, or utilizing any alternative intravascular apparatus, extravascular apparatus, intra-to-extravascular apparatus (including monopolar apparatus) or combination thereof.

[0060] As seen in FIGS. 6A and 6E, a guide catheter GC and a guidewire G may be advanced into position within, or in proximity to, either the patient’s left renal artery LRA or right renal artery RRA. In FIG. 6A, the guidewire illustratively has been positioned in the right renal artery RRA, but it should be understood that the order of bilateral renal neuromodulation illustrated in FIGS. 6A-6H alternatively may be reversed. Additionally or alternatively, bilateral renal neuromodulation may be performed concurrently on both right and left neural fibers that contribute to renal function, as in FIGS. 7-9, rather than sequentially, as in FIGS. 6.

[0061] With the guidewire and the guide catheter positioned in the right renal artery, the catheter 302 of the apparatus 300 may be advanced over the guidewire and through the guide catheter into position within the artery. As seen in FIG. 6B, the optional centering element 304 of the catheter 302 is in a reduced delivery configuration during delivery of the catheter to the renal artery. In FIG. 6C, once the catheter is properly positioned for PEF therapy, the element 304 optionally may be expanded into contact with the vessel wall, and the guidewire G may be retracted from the treatment zone, e.g., may be removed from the patient or may be positioned more proximally within the patient’s aorta.

[0062] Expansion of element 304 may center the electrodes 306 within the vessel and/or may alter impedance between the electrodes. With apparatus 300 positioned and deployed as desired, PEF therapy may be delivered in a bipolar fashion across the electrodes 306 to achieve renal neuromodulation in neural fibers that contribute to right renal function, e.g., to at least partially achieve renal denervation of the right kidney. As illustrated by propagation lines LL, the pulsed electric field may be aligned with a longitudinal dimension of the renal artery RA and may pass across the vessel wall. The alignment and propagation path of the pulsed electric field is expected to preferentially modulate cells of the target renal nerves without unduly affecting non-target arterial smooth muscle cells.

[0063] As seen in FIG. 6D, after completion of the PEF therapy, the element 304 may be collapsed back to the reduced delivery profile, and the catheter 302 may be retracted from the right renal artery RRA, for example, to a position in the guide catheter GC within the patient’s abdominal aorta. Likewise, the guide catheter GC may be retracted to a position within the patient’s aorta. The retracted guide cath-

eter may be repositioned, e.g., rotated, such that its distal outlet is generally aligned with the left renal artery LRA. The guidewire G than may be re-advanced through the catheter 302 and the guide catheter GC to a position within the left renal artery LRA, as shown in FIG. 6E (as will be apparent, the order of advancement of the guidewire and the guide catheter optionally may be reversed when accessing either renal artery).

[0064] Next, the catheter 302 may be re-advanced over the guidewire and through the guide catheter into position within the left renal artery, as shown in FIG. 6F. In FIG. 6G, once the catheter is properly positioned for PEF therapy, the element 304 optionally may be expanded into contact with the vessel wall, and the guidewire G may be retracted to a position proximal of the treatment site. PEF therapy then may be delivered in a bipolar fashion across the electrodes 306, for example, along propagation lines LI, to achieve renal neuromodulation in neural fibers that contribute to left renal function, e.g., to at least partially achieve renal denervation of the left kidney. As seen in FIG. 6H, after completion of the bilateral PEF therapy, the element 304 may be collapsed back to the reduced delivery profile, and the catheter 302, as well as the guidewire G and the guide catheter GC, may be removed from the patient to complete the bilateral renal neuromodulation procedure.

[0065] As discussed previously, bilateral renal neuromodulation optionally may be performed concurrently on fibers that contribute to both right and left renal function. FIGS. 7A and 7B illustrate embodiments of apparatus 300 for performing concurrent bilateral renal neuromodulation. In the embodiment of FIG. 7A, apparatus 300 comprises dual PEF therapy catheters 302, as well as dual guidewires G and guide catheters GC. One catheter 302 is positioned within the right renal artery RRA, and the other catheter 302 is positioned within the left renal artery LRA. With catheters 302 positioned in both the right and left renal arteries, PEF therapy may be delivered concurrently by the catheters 302 to achieve concurrent bilateral renal neuromodulation, illustratively via an intravascular approach.

[0066] In one example, separate arteriotomy sites may be made in the patient's right and left femoral arteries for percutaneous delivery of the two catheters 302. Alternatively, both catheters 302 may be delivered through a single femoral access site, either through dual guide catheters or through a single guide catheter. FIG. 7B illustrates an example of apparatus 300 for concurrent bilateral renal neuromodulation utilizing a single arteriotomy access site. In the example of FIG. 7B, both catheters 302 are delivered through a custom bifurcated guide catheter GC' having a bifurcated distal region for concurrently delivering the catheters 302 to the right and left renal arteries. Concurrent (or sequential) bilateral PEF therapy then may proceed.

[0067] FIG. 8 illustrates additional methods and apparatus for concurrent bilateral renal neuromodulation. In FIG. 8, an embodiment of extravascular apparatus 200 comprising dual probes 210 and electrodes 212. The electrodes have been positioned in the vicinity of both the left renal artery LRA and the right renal artery RRA. PEF therapy may be delivered concurrently by the electrodes 212 to achieve concurrent bilateral renal neuromodulation, illustratively via an extravascular approach.

[0068] As will be apparent, intra-to-extravascular apparatus alternatively may be utilized for bilateral renal neuromodulation. Such bilateral renal neuromodulation may be

performed sequentially, concurrently or a combination thereof. For example, ITEV PEF system 320 of FIG. 5B may be utilized for bilateral renal neuromodulation.

[0069] Additional methods and apparatus for achieving renal neuromodulation, e.g., via localized drug delivery (such as by a drug pump or infusion catheter) or via use of a stimulation electric field, etc, also may be utilized. Examples of such methods and apparatus have been described previously, for example, in co-owned and co-pending U.S. patent application Ser. No. 10/408,665, filed Apr. 8, 2003, and in U.S. Pat. No. 6,978,174, both of which have been incorporated herein by reference in their entireties.

[0070] FIG. 9 shows one example of methods and apparatus for achieving bilateral renal neuromodulation via localized drug delivery. In FIG. 9, drug reservoir 400, illustratively an implantable drug pump, has been implanted within the patient. Drug delivery catheters 402a and 402b are connected to the drug reservoir and extend to the vicinity of the right renal artery RRA and the left renal artery LRA, respectively, for delivery of one or more neuromodulatory agents or drugs capable of modulating neural fibers that contribute renal function. Delivering the agent(s) through catheters 402a and 402b may achieve bilateral renal neuromodulation. Such drug delivery through catheters 402a and 402b may be conducted concurrently or sequentially, as well as continuously or intermittently, as desired, in order to provide concurrent or sequential, continuous or intermittent, renal neuromodulation, respectively.

[0071] In an alternative embodiment of the apparatus of FIG. 9, catheters 402a and 402b may only temporarily be positioned at a desired location, e.g., for acute delivery of the neuromodulatory agent(s) from an external drug reservoir, such as a syringe. Such temporary positioning may comprise, for example, intravascular, extravascular and/or intra-to-extravascular placement of the catheters. In another alternative embodiment, the drug reservoir 400 may be replaced with an implantable neurostimulator or a pacemaker-type device, and catheters 402 may be replaced with electrical leads coupled to the neurostimulator for delivery of an electric field, such as a pulsed electric field or a stimulation electric field, to the target neural fibers. In yet another alternative embodiment, electrical techniques may be combined with delivery of neuromodulatory agent(s) to achieve desired bilateral renal neuromodulation.

[0072] Although preferred illustrative variations of the present invention are described above, it will be apparent to those skilled in the art that various changes and modifications may be made thereto without departing from the invention. For example, although the variations primarily have been described for use in combination with pulsed electric fields, it should be understood that any other electric field may be delivered as desired, including stimulation or nerve block electric fields, and any other alternative neuromodulatory techniques, such as localized delivery of a neuromodulatory agent or drug, may be utilized. It is intended in the appended claims to cover all such changes and modifications that fall within the true spirit and scope of the invention.

1-20. (canceled)

21. A method for treating hypertension, the method comprising:

modulating a function of a neural fiber that contributes to renal function of a kidney of a patient,

wherein modulating the function of the neural fiber further comprises modulating the function without completely physically severing the neural fiber.

22. The method of claim **21**, wherein modulating the function of the neural fiber further comprises modulating the function of the neural fiber via an electric field.

23. The method of claim **22**, wherein modulating the function of the neural fiber via an electric field further comprises exposing the neural fiber to a pulsed electric field.

24. The method of claim **22**, wherein modulating the function of the neural fiber via an electric field further comprises exposing the neural fiber to a stimulation electric field.

25. The method of claim **21**, wherein modulating the function of the neural fiber further comprises delivering a neuro-modulatory agent to the neural fiber.

26. The method of claim **21**, wherein modulating the function of the neural fiber further comprises at least partially denervating the kidney.

27. The method of claim **21**, wherein modulating the function of the neural fiber further comprises inducing an effect in the neural fiber chosen from the group consisting of irreversible electroporation, electrofusion, necrosis, apoptosis, gene expression alteration, cytokine up-regulation alteration, and combinations thereof.

28. The method of claim **21**, wherein modulating the function of the neural fiber further comprises thermally modulating the function of the neural fiber.

29. The method of claim **21**, wherein modulating the function of the neural fiber further comprises modulating the function of the neural fiber with high frequency ultrasound.

30. A method for treating hypertension, the method comprising:

modulating a function of a neural fiber that contributes to renal function of a kidney of a patient,

wherein modulating the function of the neural fiber further comprises modulating the function via a percutaneous approach.

31. The method of claim **30**, wherein modulating the function via a percutaneous approach further comprises modulating the function via a laparoscopic approach.

32. The method of claim **30**, wherein modulating the function via a percutaneous approach further comprises modulating the function via an endoluminal approach.

33. The method of claim **30**, wherein modulating the function of the neural fiber further comprises modulating the function of the neural fiber via an electric field.

34. The method of claim **33**, wherein modulating the function of the neural fiber via an electric field further comprises exposing the neural fiber to a pulsed electric field.

35. The method of claim **33**, wherein modulating the function of the neural fiber via an electric field further comprises exposing the neural fiber to a stimulation electric field.

36. The method of claim **30**, wherein modulating the function of the neural fiber further comprises delivering a neuro-modulatory agent to the neural fiber.

37. The method of claim **30**, wherein modulating the function of the neural fiber further comprises at least partially denervating the kidney.

38. The method of claim **30**, wherein modulating the function of the neural fiber further comprises inducing an effect in the neural fiber chosen from the group consisting of irreversible electroporation, electrofusion, necrosis, apoptosis, gene expression alteration, cytokine up-regulation alteration, and combinations thereof.

39. The method of claim **30**, wherein modulating the function of the neural fiber further comprises thermally modulating the function of the neural fiber.

40. The method of claim **30**, wherein modulating the function of the neural fiber further comprises modulating the function of the neural fiber with high frequency ultrasound.

* * * * *

专利名称(译)	肾神经调节的方法		
公开(公告)号	US20150080481A1	公开(公告)日	2015-03-19
申请号	US14/254205	申请日	2014-04-16
[标]申请(专利权)人(译)	ZARINS DENISE GIFFORD III HANSON DEEM MARK SUTTON DOUGLAS LEVIN霍华德 - [R MARK盖尔芬德		
申请(专利权)人(译)	ZARINS , DENISE 吉福德III , HANSON DEEM , MARK SUTTON , DOUGLAS LEVIN , 霍华德R. 盖尔芬德 , MARK		
当前申请(专利权)人(译)	ZARINS , DENISE 吉福德III , HANSON DEEM , MARK SUTTON , DOUGLAS LEVIN , 霍华德R. 盖尔芬德 , MARK		
[标]发明人	ZARINS DENISE GIFFORD III HANSON DEEM MARK SUTTON DOUGLAS LEVIN HOWARD R GELFAND MARK		
发明人	ZARINS, DENISE GIFFORD, III, HANSON DEEM, MARK SUTTON, DOUGLAS LEVIN, HOWARD R. GELFAND, MARK		
IPC分类号	A61B18/12 A61B18/04 A61N7/00 A61N1/36		
CPC分类号	A61B18/12 A61N1/36117 A61B18/04 A61B2018/00613 A61B2018/00434 A61N2007/003 A61N7/00 A61B18/1492 A61B2018/0022 A61B2018/00267 A61B2018/00404 A61B2018/00511 A61B2018/00577 A61B2018/00642 A61B2018/00648 A61B2018/00791 A61B2018/00875 A61N1/0551		
优先权	60/616254 2004-10-05 US 60/624793 2004-11-02 US 60/442970 2003-01-29 US 60/813589 2005-12-29 US 60/415575 2002-10-03 US 60/370190 2002-04-08 US		
其他公开文献	US9474563		

摘要(译)

提供了用于治疗造影剂肾病的方法和装置，例如，通过脉冲电场，通过刺激电场，通过局部药物递送，通过高频超声，通过热技术等。这种神经调节可以实现不可逆的电穿孔或电融合，坏死和/或细胞凋亡的诱导，基因表达的改变，动作电位衰减或阻断，细胞因子上调的变化和靶神经纤维中的其他条件。在一些实施方案中，神经调节应用于有助于肾功能的神经纤维。在一些实施方案中，这种神经调节以双侧方式进行。与单侧进行的肾神经调节相比，双侧肾神经调节可以在一些患者中提供增强的治疗效果，即，与在支配单个肾的神经组织上进行的肾神经调节相比。

Continuation of application No. 13/898,830, filed on May 21, 2013, now Pat. No. 8,774,922, which is a continuation of application No. 11/368,809, filed on Mar. 6, 2006, now Pat. No. 8,551,069, which is a continuation-in-part of application No. 10/408,665, filed on Apr. 8, 2003, now Pat. No. 7,162,303, said application No. 11/368,809 is a continuation-in-part of application No. 11/133,925, filed on May 20, 2005, now Pat. No. 8,771,252, which is a continuation of application No. 10/900,199, filed on Jul. 28, 2004, now Pat. No. 6,978,174, which is a continuation-in-part of application No. 10/408,665, filed on Apr. 8, 2003, now Pat. No. 7,162,303, said application No. 11/368,809 is a continuation-in-part of application No. 11/189,563, filed on Jul. 25, 2005, now Pat. No. 8,145,316, which is a continuation-in-part of application No. 11/129,765, filed on May 13, 2005, now Pat. No. 7,653,438, which is a continuation-in-part of application No. 10/408,665, filed on Apr. 8, 2003, now Pat. No. 7,162,303, said application No. 11/368,809 is a continuation-in-part of application No. 11/266,993, filed on Nov. 4, 2005, now Pat. No. 7,756,583, which is a continuation-in-part of